

## ภาคผนวกที่ 4

เอกสารการสอบเทียบความถูกต้องของเครื่องมือ

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
<b>1. คุณภาพอากาศในบรรยากาศ</b> Total Suspended Particulate (TSP)	High Volume Air Sampler Rec No. R08, R13, R14 B. No. R08, R13, R14	Digital Balance
Carbon Monoxide	Personal Pump SKC No. R13, R33, R44	CO Analyzer No. R03
Nitrogen Dioxide	NO <sub>2</sub> Analyzer No. R01, B12, B15	NO <sub>2</sub> Analyzer No. R01, B12, B15
<b>2. คุณภาพอากาศจากปล่อง</b> Total Suspended Particulate (TSP)	Console No. R04, R05 Pitot Tube No. B24, B38, B58	Digital Balance
Carbon Monoxide (CO)	Personal Pump SKC No. R08, R19, R26, R27 Rotameter No. H-R02	CO Analyzer No. B01
Oxides of Nitrogen (NO <sub>x</sub> )	Vacuum Gauge	Spectrophotometer
Xylene	Personal Pump SKC No. R24 Rotameter No. L-R02	GC/FID
Acetic Acid	Personal Pump SKC No. R38 Rotameter No. L-R02	GC/FID
<b>3. คุณภาพอากาศในสถานประกอบการ</b> Total Dust	Personal Pump No. R02, R17, R34, R37 Rotameter No. H-R02	Digital Balance
Xylene	Personal Pump SKC No. R03, R12, R14, R15, R17, R24, R40, R44 Rotameter No. L-R02	GC/FID
Acetic Acid	Personal Pump SKC No. R02, R07, R17, R19, R22, R24, R30, R40, R42 Rotameter No. L-R02	GC/FID
Methyl Acetate	Personal Pump SKC No. R07, R19, R25, R33 Rotameter No. L-R02	GC/FID
Methanol	Personal Pump SKC No. R27, R45 Rotameter No. L-R02	GC/FID
<b>4. ระดับเสียง</b> L <sub>eq</sub> 24 hr, L <sub>90</sub> , L <sub>eq</sub> 8 hr	Acoustic Calibrator Integrated Sound Level Meter No. ACO-R07, R08, R09, R10, R23, R46	-

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ต่อ)

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
5. คุณภาพน้ำทิ้ง		
pH	-	pH Meter
Temperature	-	Thermometer
Total Suspended Solids	-	Digital Balance
Total Dissolved Solids	-	Digital Balance
BOD <sub>5</sub>	-	BOD Analyzer
COD	-	COD Reactor
Grease & Oil	-	Digital Balance
Manganese	-	Inductively Coupled Plasma
Conductivity	-	Conductivity Meter

คุณภาพอากาศในบรรยากาศ





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

### Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B35	B35	01/11/2023	y = 1.247x - 5.373	0.999
B36	B36	02/11/2023	y = 1.190x - 2.630	0.995
B37	B37	01/11/2023	y = 1.188x - 2.249	0.999
B38	B38	01/11/2023	y = 1.191x - 5.051	0.995
B39	B39	01/11/2023	y = 1.230x - 3.335	0.995
B40	B40	02/11/2023	y = 1.172x - 2.695	0.998
B41	B41	02/11/2023	y = 1.169x - 2.206	0.998
B42	B42	02/11/2023	y = 1.212x - 5.591	0.998
B43	B43	03/11/2023	y = 1.223x - 3.058	0.997
B44	B44	01/11/2023	y = 1.194x - 2.207	0.996
R01	R01	08/11/2023	y = 1.199x - 4.374	0.998
R02	R02	06/11/2023	y = 1.229x - 6.243	0.999
R03	R03	08/11/2023	y = 1.239x - 7.264	0.998
R04	R04	09/11/2023	y = 1.182x - 3.161	0.998
R05	R05	09/11/2023	y = 1.141x - 2.095	0.997
R06	R06	03/11/2023	y = 1.155x - 2.543	0.997
R07	R07	09/11/2023	y = 1.057x + 1.380	0.999
R08	R08	02/11/2023	y = 1.230x - 6.615	0.997
R09	R09	04/11/2023	y = 1.188x - 1.331	0.997
R10	R10	04/11/2023	y = 1.213x - 3.571	0.998
R11	R11	01/11/2023	y = 1.136x - 2.259	0.999
R12	R12	01/11/2023	y = 1.145x - 3.404	0.998
R13	R13	02/11/2023	y = 1.076x - 0.153	0.999
R14	R14	02/11/2023	y = 1.166x + 1.197	0.996
R15	R15	09/11/2023	y = 1.171x - 4.139	0.997
R16	R16	09/11/2023	y = 1.142x - 3.462	0.999
R17	R17	01/11/2023	y = 1.169x - 3.932	0.998
R18	R18	01/11/2023	y = 1.192x - 4.280	0.998
R19	R19	01/11/2023	y = 1.158x - 4.004	0.996
R20	R20	02/11/2023	y = 1.191x - 4.426	0.997

Calibrated by :



Approved by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25 ± 3 °C  
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)			y	R <sup>2</sup>
					1	2	3	1	2	3		
R01	SKC	224-PCXR4	602467	02/10/2023	1,000	1,500	2,000	1,001	1,499	1,999	1.010x - 22.581	0.999
R02	SKC	224-PCXR4	626450	06/10/2023	1,000	2,000	3,000	996	1,493	1,986	0.992x + 3.742	1.000
R03	SKC	224-PCXR4	691592	06/10/2023	1,000	1,500	2,000	989	1,495	1,994	0.999x - 6.866	1.000
R04	SKC	224-PCXR4	691672	06/10/2023	1,000	1,500	2,000	998	1,491	1,989	0.991x + 5.421	1.000
R05	SKC	224-PCXR4	798470	06/10/2023	1,000	1,500	2,000	999	1,495	1,995	1.005x - 18.995	0.999
R06	SKC	224-PCXR4	798456	02/10/2023	1,000	1,500	2,000	1,000	1,488	1,987	0.986x + 13.398	1.000
R07	SKC	224-PCXR4	798480	02/10/2023	1,000	1,500	2,000	1,000	1,497	1,998	1.009x - 21.689	0.999
R08	SKC	224-PCXR4	883215	05/10/2023	1,000	1,500	2,000	994	1,500	1,990	0.995x + 3.109	1.000
R09	SKC	224-PCXR4	034650	05/10/2023	1,000	1,500	2,000	999	1,497	1,996	1.008x - 21.526	0.999
R10	SKC	224-PCXR4	091765	05/10/2023	1,000	1,500	2,000	996	1,493	1,994	1.000x - 6.596	1.000
R11	SKC	224-PCXR4	091763	04/10/2023	1,000	1,500	2,000	998	1,496	1,983	0.998x - 9.346	0.999
R12	SKC	224-PCXR4	091568	04/10/2023	1,000	1,500	2,000	1,000	1,497	1,999	1.009x - 21.948	0.999
R13	SKC	224-PCXR4	091638	02/10/2023	1,000	1,500	2,000	994	1,495	1,986	0.993x + 2.981	1.000
R14	SKC	224-PCXR4	091764	06/10/2023	1,000	1,500	2,000	998	1,498	2,000	1.012x - 26.788	0.999
R15	SKC	224-PCXR8	529457	06/10/2023	1,000	1,500	2,000	995	1,492	1,987	0.994x + 1.457	1.000
R16	SKC	224-PCXR8	529643	04/10/2023	1,000	1,500	2,000	1,000	1,498	1,997	1.007x - 17.908	0.999
R17	SKC	224-PCXR8	529645	07/10/2023	1,000	1,500	2,000	998	1,496	1,998	1.011x - 25.546	0.999
R18	SKC	224-PCXR8	566756	03/10/2023	1,000	1,500	2,000	994	1,490	1,989	0.995x - 1.759	1.000
R19	SKC	224-PCXR8	566802	02/10/2023	1,000	1,500	2,000	1,000	1,496	1,999	1.010x - 22.864	0.999
R20	SKC	224-PCXR8	529089	06/10/2023	1,000	1,500	2,000	992	1,506	1,996	1.008x - 22.151	0.999
R21	SKC	224-PCXR8	665728	02/10/2023	1,000	1,500	2,000	992	1,486	1,994	1.002x - 11.842	1.000
R22	SKC	224-PCXR8	707444	03/10/2023	1,000	1,500	2,000	1,001	1,500	1,999	1.007x - 18.171	0.999
R23	SKC	224-PCXR8	761067	06/10/2023	1,000	1,500	2,000	1,000	1,488	1,993	0.992x + 5.744	1.000
R24	SKC	224-PCXR8	707893	05/10/2023	1,000	1,500	2,000	994	1,505	1,996	1.005x - 15.010	0.999
R25	SKC	224-PCXR8	761052	06/10/2023	1,000	1,500	2,000	999	1,495	1,989	0.991x + 5.640	1.000
R26	SKC	224-PCXR8	707956	07/10/2023	1,000	1,500	2,000	1,010	1,497	2,002	0.999x - 2.874	0.999
R27	SKC	224-PCXR8	707398	07/10/2023	1,000	1,500	2,000	1,001	1,496	1,997	1.008x - 20.237	0.999
R28	SKC	224-PCXR8	707481	07/10/2023	1,000	1,500	2,000	993	1,506	1,995	1.002x - 10.719	1.000
R29	SKC	224-PCXR8	707402	04/10/2023	1,000	1,500	2,000	995	1,495	1,989	0.995x + 1.091	1.000
R30	SKC	224-PCXR8	093811	04/10/2023	1,000	1,500	2,000	998	1,495	1,992	0.997x - 0.693	1.000
R31	SKC	224-PCXR8	093183	06/10/2023	1,000	1,500	2,000	999	1,502	1,997	0.988x + 9.127	0.999
R32	SKC	224-PCXR8	671950	07/10/2023	1,000	1,500	2,000	998	1,495	1,994	0.998x - 3.451	1.000
R33	SKC	224-PCXR4	626254	07/10/2023	1,000	1,500	2,000	992	1,503	1,995	1.011x - 30.016	0.999
R34	SKC	224-PCXR4	626131	03/10/2023	1,000	1,500	2,000	990	1,499	1,997	1.014x - 32.986	0.999
R35	SKC	224-PCXR8	707460	07/10/2023	1,000	1,500	2,000	990	1,501	1,997	1.005x - 15.898	1.000
R36	SKC	224-PCXR8	707446	05/10/2023	1,000	1,500	2,000	1,000	1,497	1,997	1.002x - 7.547	1.000
R37	SKC	224-PCXR8	707432	02/10/2023	1,000	1,500	2,000	995	1,498	1,995	0.999x - 4.856	1.000
R38	SKC	224-PCXR8	707349	02/10/2023	1,000	1,500	2,000	991	1,496	1,992	1.000x - 7.364	1.000
R39	SKC	224-PCXR8	761095	06/10/2023	1,000	1,500	2,000	995	1,489	1,985	0.990x + 6.253	1.000

Calibrated by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24. Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
R40	SKC	224-PCXR4	612753	07/10/2023	1,000	1,500	2,000	999	1,496	1,996	1.008x – 21.287	0.999
R41	SKC	224-PCXR4	626140	03/10/2023	1,000	1,500	2,000	990	1,499	1,996	1.013x – 31.991	0.999
R42	SKC	224-PCXR4	626463	07/10/2023	1,000	1,500	2,000	998	1,493	1,994	0.998x – 4.088	1.000
R43	SKC	224-PCXR4	626129	07/10/2023	1,000	1,500	2,000	1,001	1,498	1,999	1.010x – 21.673	0.999
R44	SKC	224-PCXR4	602753	07/10/2023	1,000	1,500	2,000	994	1,492	1,990	0.997x – 4.275	1.000
R45	SKC	224-PCXR4	626137	06/10/2023	1,000	1,500	2,000	992	1,487	1,996	1.006x – 16.996	1.000

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### CALIBRATION REPORT

#### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 13 November 2023

BRAND : API

MODEL : 200E

NO. NOX-R01

SERIAL NO. 769

#### Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 08 August 2023

Serial No. : 911

#### Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : A00726SV

Certified Date : 05 January 2023

Expired Date : 05 January 2026

Cylinder Conc. : 48.8 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.6 °C

% RH 48

#### CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	399.9	-0.025	400.0	1.007
NO <sub>x</sub> Span	400	400.2	0.050	400.0	1.010

#### API Model 200E NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	512	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	102.9	mV	-20 - 150
AZERO	93.6	mV	-20 - 150
HVPS	675	V	420 - 900 constant
RCELL TEMP	50.0	°C	50 ± 1
BOX TEMP	29.4	°C	8 - 48
PMT TEMP	7.2	°C	7 ± 2
MOLY TEMP	315.2	°C	315 ± 5
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.007	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.010	-	1.0 ± 0.3
NO Offset	1.5	mV	-20 to +150
NO <sub>x</sub> Offset	0.9	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	13 November 2023	BRAND :	API	MODEL :	200A
NO.	NOX-B12	SERIAL NO.	2675		
Calibrator (Dilution System)					
Brand	: API			Model	: 700
Last Cal. Date	: 08 August 2023			Serial No.	: 911
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00726SV
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH 48					
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.008
NO <sub>x</sub> Span	400	400.2	0.050	400.0	1.012
API Model 200A NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	507	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.3	mV	-20 - 150		
AZERO	94.1	mV	-20 - 150		
HVPS	673	V	420 - 900 constant		
RCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.1	°C	8 - 48		
PMT TEMP	7.3	°C	7 ± 2		
MOLY TEMP	314.8	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000		
NO Slope	1.008	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.012	-	1.0 ± 0.3		
NO Offset	1.6	mV	-20 to +150		
NO <sub>x</sub> Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

Approved by :






บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

CALIBRATION REPORT						
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER						
DATE :	13 November 2023	BRAND :	API	MODEL :	200A	
NO.	NOX-B15	SERIAL NO.	213			
Calibrator (Dilution System)						
Brand	: API			Model	: 700	
Last Cal. Date	: 08 August 2023			Serial No.	: 911	
Reference Standard Gas						
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00726SV	
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm	
CALIBRATING CONDITION						
Pressure	1011	mmbar	Temp.	24.6	°C	
% RH						48
CALIBRATION SETTING						
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB		
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope	
Zero	0	0.10	-	0	-	
NO Span	400	399.7	-0.075	400.0	1.005	
NO <sub>x</sub> Span	400	400.1	0.025	400.0	1.009	
API Model 200A NO <sub>x</sub> Analyzer Check List						
Test Values	Observed Value	Units	Nominal Range			
RANGE	500	PPB	500 standard			
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air			
SAMPLE FLOW	509	cc/min	500 ± 50			
OZONE FLOW	79	cc/min	80 ± 15			
PMT	103.1	mV	-20 - 150			
AZERO	93.8	mV	-20 - 150			
HVPS	672	V	420 - 900 constant			
RCELL TEMP	50.4	°C	50 ± 1			
BOX TEMP	29.2	°C	8 - 48			
PMT TEMP	7.1	°C	7 ± 2			
MOLY TEMP	315.3	°C	315 ± 5			
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant			
SAMPLE PRESS	28.7	IN-Hg-A	25 - 30 constant			
NO Span Conc	400	PPB	20 - 20,000			
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000			
NO Slope	1.005	-	1.0 ± 0.3			
NO <sub>x</sub> Slope	1.009	-	1.0 ± 0.3			
NO-Offset	1.4	mV	-20 to +150			
NO <sub>x</sub> Offset	0.9	mV	-20 to 150			
Stability at Zero	0.1	PPB	< 0.2			
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas			

Calibrated by :



Approved by :

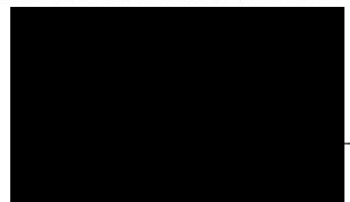



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905

**ID No** : BA 05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** : 

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23° C  $\pm$  1° C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY M  
COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	02 November 2023	Brand :	API	Model :	300E
No.	CO-R03			Serial No.	1352
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 08 August 2023			Serial No. : 911		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D196045		
Certified Date : 16 April 2022		Expired Date : 15 April 2024		Cylinder Conc. : 4,570 ppm	
Calibrating Condition					
Pressure : 1011 mmbar		Temp. : 24.5 °C		% RH : 48	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	0.11	-	0	
CO Span	40.00	39.98	-0.050	40.00	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4013.5	mV	2500-4800 mV		
CO Reference	3946.1	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.5	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	808	CC/Min	800 ± 10%		
Sample Temperature	48.5	°C	48 ± 4		
Bench Temperature	48.2	°C	48 ± 2		
Wheel Temperature	68.5	°C	68 ± 2		
Box Temperature	30.7	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3049.2	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by : \_\_\_\_\_

Approved by : \_\_\_\_\_

คุณภาพอากาศจากปล่อง



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## Console Calibration Report

Calibration Method

Critical Orifices


### Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	$\Delta H_{@}$ (mmH <sub>2</sub> O)
B01	1563	02/06/2023	1.002	50.06
B02	8002514	05/06/2023	0.998	49.11
B03	1503016	01/06/2023	1.004	50.26
B04	00006659	05/06/2023	0.996	49.89
B05	00007428	02/06/2023	0.997	49.51
R01	1561	01/06/2023	0.995	49.93
R02	8002513	02/06/2023	1.003	49.77
R03	1570	01/06/2023	0.996	49.70
R04	8002519	05/06/2023	0.995	49.44
R05	1503015	01/06/2023	0.997	50.37


Remark : Accept Value of y (test) is  $0.97 < y < 1.03$

Accept Value of  $\Delta H_{@}$  (test) is  $46.7 \pm 6.4$  (mmH<sub>2</sub>O)

Calibrated by :

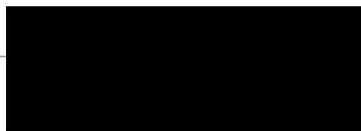

Approved by :

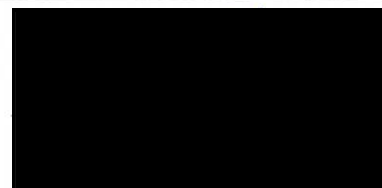



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## Pitot Tube Calibration Report

Calibration Method


Standard Pitot Tube

### Calibration Data


Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	02/05/2023	0.85	0.84
B04	S	0.99	02/05/2023	0.84	0.84
B05	S	0.99	02/05/2023	0.84	0.83
B07	S	0.99	02/05/2023	0.83	0.84
B08	S	0.99	03/05/2023	0.84	0.85
B09	S	0.99	04/05/2023	0.85	0.84
B11	S	0.99	04/05/2023	0.84	0.83
B16	S	0.99	04/05/2023	0.84	0.85
B18	S	0.99	02/05/2023	0.84	0.84
B19	S	0.99	02/05/2023	0.85	0.84
B21	S	0.99	03/05/2023	0.84	0.85
B24	S	0.99	03/05/2023	0.84	0.83
B27	S	0.99	02/05/2023	0.83	0.84
B30	S	0.99	04/05/2023	0.84	0.84
B31	S	0.99	02/05/2023	0.83	0.84
B33	S	0.99	03/05/2023	0.85	0.84
B35	S	0.99	02/05/2023	0.84	0.83

Remark : Accept value of Cp (test) is  $0.84 \pm 0.01$

Calibrated by :

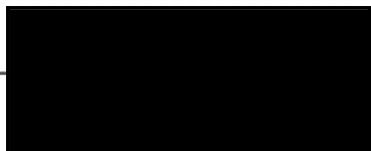

Approved by :

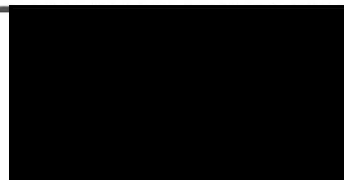





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

## Pitot Tube Calibration Report

Calibration Method


Standard Pitot Tube

### Calibration Data


Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	02/05/2023	0.84	0.84
B37	S	0.99	02/05/2023	0.83	0.84
B38	S	0.99	03/05/2023	0.85	0.84
B39	S	0.99	03/05/2023	0.84	0.83
B40	S	0.99	02/05/2023	0.84	0.83
B41	S	0.99	02/05/2023	0.84	0.84
B44	S	0.99	03/05/2023	0.85	0.84
B45	S	0.99	03/05/2023	0.85	0.84
B46	S	0.99	04/05/2023	0.84	0.83
B47	S	0.99	03/05/2023	0.84	0.85
B48	S	0.99	03/05/2023	0.83	0.84
B49	S	0.99	03/05/2023	0.85	0.84
B54	S	0.99	03/05/2023	0.83	0.84
B56	S	0.99	02/05/2023	0.84	0.85
B57	S	0.99	02/05/2023	0.84	0.83
B58	S	0.99	02/05/2023	0.85	0.84

Remark : Accept value of Cp (test) is  $0.84 \pm 0.01$

Calibrated by :



Approved by :

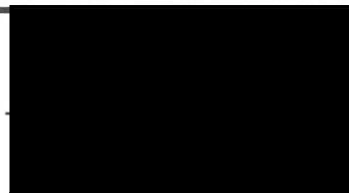



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com... www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
R01	SKC	224-PCXR4	602467	06/07/2023	1,000	1,500	2,000	991	1,506	2,002	1.007x – 14.479	1.000
R02	SKC	224-PCXR4	626450	06/07/2023	1,000	2,000	3,000	997	1,497	1,988	0.988x + 12.256	1.000
R03	SKC	224-PCXR4	691592	06/07/2023	1,000	1,500	2,000	1,002	1,498	2,002	1.003x – 5.881	1.000
R04	SKC	224-PCXR4	691672	06/07/2023	1,000	1,500	2,000	995	1,491	1,994	0.997x – 2.717	1.000
R05	SKC	224-PCXR4	798470	06/07/2023	1,000	1,500	2,000	992	1,505	1,997	1.001x – 6.538	1.000
R06	SKC	224-PCXR4	798456	06/07/2023	1,000	1,500	2,000	994	1,497	1,993	0.994x – 0.976	1.000
R07	SKC	224-PCXR4	798480	04/07/2023	1,000	1,500	2,000	993	1,490	1,997	1.007x – 16.177	1.000
R08	SKC	224-PCXR4	883215	04/07/2023	1,000	1,500	2,000	1,010	1,499	2,003	0.989x + 11.332	0.999
R09	SKC	224-PCXR4	034650	04/07/2023	1,000	1,500	2,000	990	1,503	2,000	1.011x – 24.548	1.000
R10	SKC	224-PCXR4	091765	07/07/2023	1,000	1,500	2,000	996	1,509	1,992	0.999x + 0.299	1.000
R11	SKC	224-PCXR4	091763	07/07/2023	1,000	1,500	2,000	999	1,497	1,985	1.000x – 9.834	0.999
R12	SKC	224-PCXR4	091568	07/07/2023	1,000	1,500	2,000	995	1,499	1,998	1.001x – 6.774	1.000
R13	SKC	224-PCXR4	091638	07/07/2023	1,000	1,500	2,000	1,001	1,510	1,989	0.988x + 16.559	1.000
R14	SKC	224-PCXR4	091764	07/07/2023	1,000	1,500	2,000	993	1,501	1,997	1.013x – 30.102	0.999
R15	SKC	224-PCXR8	529457	07/07/2023	1,000	1,500	2,000	1,000	1,499	2,001	0.998x – 3.682	0.999
R16	SKC	224-PCXR8	529643	05/07/2023	1,000	1,500	2,000	997	1,494	1,992	0.992x + 2.530	1.000
R17	SKC	224-PCXR8	529645	05/07/2023	1,000	1,500	2,000	994	1,507	1,998	1.006x – 15.440	0.999
R18	SKC	224-PCXR8	566756	05/07/2023	1,000	1,500	2,000	990	1,496	1,996	1.000x – 6.873	1.000
R19	SKC	224-PCXR8	566802	05/07/2023	1,000	1,500	2,000	1,001	1,497	1,998	1.003x – 14.352	0.999
R20	SKC	224-PCXR8	529089	03/07/2023	1,000	1,500	2,000	990	1,499	2,001	1.019x – 39.318	0.999
R21	SKC	224-PCXR8	665728	03/07/2023	1,000	1,500	2,000	997	1,493	1,997	0.999x – 3.765	1.000
R22	SKC	224-PCXR8	707444	03/07/2023	1,000	1,500	2,000	1,002	1,511	2,001	1.000x – 2.666	0.999
R23	SKC	224-PCXR8	761067	05/07/2023	1,000	1,500	2,000	1,011	1,475	1,989	0.980x + 20.504	0.999
R24	SKC	224-PCXR8	707893	04/07/2023	1,000	1,500	2,000	995	1,507	1,998	1.007x – 16.619	0.999
R25	SKC	224-PCXR8	761052	04/07/2023	1,000	1,500	2,000	1,009	1,494	1,993	0.984x + 21.169	1.000
R26	SKC	224-PCXR8	707956	06/07/2023	1,000	1,500	2,000	1,011	1,499	2,004	1.001x – 3.674	0.999
R27	SKC	224-PCXR8	707398	06/07/2023	1,000	1,500	2,000	995	1,499	1,999	1.005x – 14.830	1.000
R28	SKC	224-PCXR8	707481	04/07/2023	1,000	1,500	2,000	1,003	1,499	2,000	1.001x – 11.858	0.998
R29	SKC	224-PCXR8	707402	04/07/2023	1,000	1,500	2,000	1,002	1,492	1,987	0.985x + 16.145	1.000
R30	SKC	224-PCXR8	093811	07/07/2023	1,000	1,500	2,000	999	1,492	1,991	0.994x + 4.391	1.000
R31	SKC	224-PCXR8	093183	04/07/2023	1,000	1,500	2,000	1,000	1,499	1,999	0.989x + 8.339	0.999
R32	SKC	224-PCXR8	671950	04/07/2023	1,000	1,500	2,000	997	1,499	1,991	0.995x + 4.048	1.000
R33	SKC	224-PCXR4	626254	04/07/2023	1,000	1,500	2,000	993	1,501	1,998	1.014x – 32.194	0.999
R34	SKC	224-PCXR4	626131	04/07/2023	1,000	1,500	2,000	1,001	1,498	2,002	1.006x – 12.316	1.000
R35	SKC	224-PCXR8	707460	03/07/2023	1,000	1,500	2,000	998	1,496	1,993	0.993x + 5.945	1.000
R36	SKC	224-PCXR8	707446	07/07/2023	1,000	1,500	2,000	1,003	1,497	1,999	1.008x – 18.814	0.999
R37	SKC	224-PCXR8	707432	07/07/2023	1,000	1,500	2,000	995	1,497	1,998	0.995x + 5.662	1.000
R38	SKC	224-PCXR8	707349	07/07/2023	1,000	1,500	2,000	996	1,498	1,999	1.002x – 7.662	1.000
R39	SKC	224-PCXR8	761095	04/07/2023	1,000	1,500	2,000	1,000	1,514	1,992	0.984x + 18.826	0.999

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-R01	Dwyer	VFB-65	05/07/2023	500	1,000	2,000	501.2	993.0	1978.7	0.999x - 3.855	0.999
H-R02	Dwyer	VFB-65	05/07/2023	500	1,000	2,000	501.5	998.1	1986.7	1.000x - 2.024	1.000
H-R03	Dwyer	VFB-65	04/07/2023	500	1,000	2,000	501.2	989.3	1995.7	0.992x + 3.827	1.000
H-R04	Dwyer	VFB-65	10/07/2023	500	1,000	2,000	496.3	991.2	2014.5	1.006x - 10.883	1.000
H-R05	Dwyer	VFB-65	05/07/2023	500	1,000	2,000	499.1	987.9	1988.7	1.002x - 6.676	1.000
H-R06	Dwyer	VFB-65	06/07/2023	500	1,000	2,000	504.7	994.0	1980.6	0.998x - 1.539	0.999

Calibrated by :

Approved by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
L-R01	Dwyer	VFA-21	05/07/2023	50	100	200	50.6	100.9	204.1	0.983x + 2.913	1.000
L-R02	Dwyer	VFA-21	05/07/2023	50	100	200	50.4	101.9	200.8	1.003x – 0.034	0.999
L-R03	Dwyer	VFA-21	04/07/2023	50	100	200	50.1	100.1	202.1	1.006x + 0.170	1.000
L-R04	Dwyer	VFA-21	10/07/2023	50	100	200	50.2	100.8	203.3	1.002x + 0.502	1.000
L-R05	Dwyer	VFA-21	05/07/2023	50	100	200	50.1	101.1	202.8	0.999x + 0.445	0.999
L-R06	Dwyer	VFA-21	06/07/2023	50	100	200	50.7	101.3	202.5	0.998x + 1.435	1.000

Calibrated by :

Approved by :



## CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220066-3]  
CLID. NO. : 212201114  
JOB CONTROL NO. : 230725081569


CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 25 July 2023

DATE OF ISSUED : 31 July 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee  
Calibration Engineer

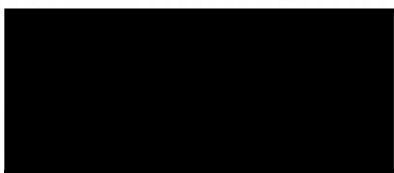

Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
31 July 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23081569

F3-011-04/01-12

page 1 of 3



@clccalibration



CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE	:	VACUUM GAUGE
MANUFACTURER	:	HI-LIGHT
MODEL / TYPE	:	N/A
SERIAL NO.	:	N/A[64-220066-3]
DATE OF CALIBRATION	:	26 July 2023
DUE DATE OF CALIBRATION	:	26 July 2024

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).

Certificate No. MP-0035-23, Due Date 02 February 2024.

#### UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2$ . It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q23081569

F3-011-04/01-12

page 2 of 3



@clccalibration



**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

### CALIBRATION DATA

#### CORRECTION OF PRESSURE

DUC Test point ( inHg )	STD Reading ( kPa )		Conversion to inHg		Correction ( inHg )	
	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-16.66	-16.69	-4.9	-4.9	+0.1	+0.1
-10	-33.79	-33.79	-10.0	-10.0	0.0	0.0
-15	-50.76	-50.76	-15.0	-15.0	0.0	0.0
-20	-67.79	-67.82	-20.0	-20.0	0.0	0.0
-25	-84.68	-84.72	-25.0	-25.0	0.0	0.0
-30	-101.51	-101.51	-30.0	-30.0	0.0	0.0

Uncertainty of measurement  $\pm 0.2$  inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q23081569

F3-011-04/01-12

page 3 of 3



@clccalibration





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)



CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY :

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23°C  $\pm$  1°C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT






บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	03 July 2023	Brand :	API	Model :	300E
No.	CO-B01			Serial No.	782
Calibrator (Dilution System)					
Brand : API			Model : 700		
Last Cal. Date : 06 September 2022			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)			Cylinder No. : D196045		
Certified Date : 16 April 2022		Expired Date : 15 April 2024		Cylinder Conc. : 4,570 ppm	
Calibrating Condition					
Pressure : 1011 mmbar		Temp. : 24.6 °C		% RH : 49	
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	0.11	-	0	
CO Span	40.00	40.06	0.150	40.00	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	< 1 ppm With Zero Air		
CO Measure	4015.2	mV	2500-4800 mV		
CO Reference	3947.7	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.7	In-Hg-A	~2" < Ambient Absolute Pressure		
Sample Flow	806	CC/Min	800 ± 10%		
Sample Temperature	48.5	°C	48 ± 4		
Bench Temperature	48.2	°C	48 ± 2		
Wheel Temperature	68.4	°C	68 ± 2		
Box Temperature	30.7	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3037.6	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibrated by :



Approved by :

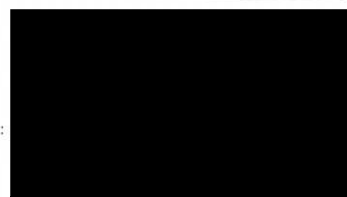

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com <http://www.sithiphorn.com>

NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : SP23016

Pages : 1 of 3


## Calibration Certificate

**Equipment :** UV-VIS SPECTROPHOTOMETER  
**Manufacturer :** PERKINELMER  
**Model :** LAMBDA 25  
**Serial No.:** 501S14123010  
**ID No.:** SP03/58  
**Calibration Mode :** WAVELENGTH ACCURACY  
PHOTOMETRIC ACCURACY  
**Condition As Found :** GOOD  
**Customer :** S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,  
CHOMPHON, CHATUCHAK,  
BANGKOK 10900, THAILAND.  
**Location :** ORGANIC LABORATORY IV  
**Ambient Temperature :** ( 25.0 ± 5 ) °C  
**Relative Humidity :** ( 48.4 ± 25 ) %  
**Received Date :** 30 AUGUST 2023  
**Calibration Date :** 30 AUGUST 2023  
**Date of Issue :** 31 AUGUST 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

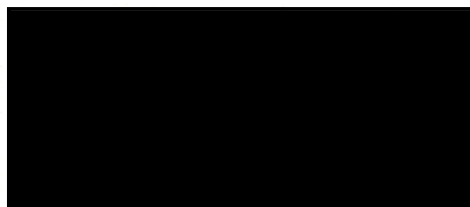

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : SP23016

Job No. : VC66SP0014

Pages : 2 of 3

**Calibration Method :**

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

**Condition of this result of calibration :**

## 1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	106864	01/11/2024
Didymium liquid	RM-DL	28912	106905	02/11/2024
Neutral density filter	RM-1N2N3N	13877	106918	03/11/2024
Potassium dichromate solutions	RM-0204060810	14204	106902	02/11/2024
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology, NIST.

**Result of calibration : Wavelength Accuracy**

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.3	0.05	0.16	2.00
	467.82	468.0	0.18	0.16	2.00
	536.56	536.6	0.04	0.16	2.00
	640.50	640.4	-0.10	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.0	0.06	0.16	2.00

UUC\* = Unit Under Calibration



Continuation of Calibration Certificate

Cert. No. : SP23016  
Job No. : VC66SP0014  
Pages : 3 of 3

**Result of calibration : Photometric Accuracy**

(Without adjustment)

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0517	1.0564	0.0047	0.0031	2.00
		29914	0.7	0.7445	0.7460	0.0015	0.0032	2.00
		29381	0.5	0.5416	0.5429	0.0013	0.0032	2.00
	546.1	29360	1.0	0.9821	0.9849	0.0028	0.0030	2.00
		29914	0.7	0.6961	0.6961	0.0000	0.0030	2.00
		29381	0.5	0.5073	0.5073	0.0000	0.0030	2.00
	590.0	29360	1.0	1.0222	1.0244	0.0022	0.0030	2.00
		29914	0.7	0.7237	0.7234	-0.0003	0.0030	2.00
		29381	0.5	0.5361	0.5360	-0.0001	0.0031	2.00
	635.0	29360	1.0	0.9753	0.9775	0.0022	0.0030	2.00
		29914	0.7	0.6910	0.6910	0.0000	0.0030	2.00
		29381	0.5	0.5211	0.5210	-0.0001	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2422	0.2462	0.0040	0.0101	2.00	
		40	0.4866	0.4900	0.0034	0.0115	2.00	
		60	0.7414	0.7390	-0.0024	0.0068	2.00	
		80	0.9858	0.9871	0.0013	0.0093	2.00	
		100	1.2442	1.2480	0.0038	0.0087	2.00	

UUC\* = Unit Under Calibration

**Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230**

Resolution of Wavelength Mode 0.1 nm  
Resolution of Photometric Mode 0.0001 A  
Parameter Setting  
Measurement Mode Wavelength, Absorbance  
Wavelength Scan 1100 nm-190 nm  
Scanning Speed 7.5 nm/min  
Data Pitch 0.1 nm  
Band width(Wavelength) 1.0 nm  
Band width(Vis) 1.0 nm  
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transimission T(%)	Absorbance(A)
0.0111	3.9564

\*\*Specific Acceptance :

Transmission  $\leq$  1.0 T(%), Absorbance  $\geq$  2.0 A

\*\*Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95%

End of Calibration Certificate





## GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0823/21044

Instrument Type : GC

Model : CP-3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 09/08/2023

### ELECTRONIC TEST

CPU	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
LCD TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
VENT TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
KEY ECHO TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DESTRUCTION RAM TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

### RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detector ( FID Channel Front)

INJECTOR : Capillary Injector Model 1079

#### GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column: Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218 g/L C14, C15, C16 in hexane

SENSITIVITY TEST: C15. ( Area count ) = 362,972 Counts.



**Detector Sensitivity ( FID )**

Detector Response	Result	Specification
Baseline Noise (µV)	1.47	≤ 50
Baseline Drift (%)	0.09	≤ 1
Sensitivity ( S/N for C15)	19,600	≥ 1,024

**Temperature Specification**

Temperature	Set	Result	Specification
Column Oven (° C)	80	80	± 5
Injector (° C)	220	220	± 5
Detector (° C)	300	300	± 5
Incubator (° C)	60	N/A	± 5

**Relative Standard Deviation % ( % RSD)**

Checkout Procedure	Result	Specification
Area C15 ( %)	1.52	≤ 5
Retention Time C15( %)	0.01	≤ 0.5

APPROVAL :

Signature

Engineer

Date : 09/08/2023







บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

### Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	357,863
C15 Area 2	357,824
C15 Area 3	367,724
C15 Area 4	361,724
C15 Area 5	369,724
C15 Area Average	362,972
* % RSD ( < 5 % )	1.52

\* The precision specification should be less than 2.0 % RSD \*\* ( Relative Standard Deviation ) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five ( 5 ) samples.

\*\* (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = ( \text{std.dev} / \text{avg} ) * 100$$

Compliance	
Performance by	
Date	



Comments			
Reviewed by		Date	09/08/2023



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

### Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	4.125
C15 RT 2	4.125
C15 RT 3	4.125
C15 RT 4	4.124
C15 RT 5	4.124
C15 RT Average	4.122
* % RSD ( < 0.5 % )	0.01

\* The precision specification should be less than 0.5 % RSD \*\* ( Relative Standard Deviation ) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five ( 5 ) samples.

\*\* (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = ( \text{std.dev} / \text{avg} ) * 100$$

Compliance	
Performance by	
Date	



Comments			
Reviewed by			Date 09/08/2023



VARIAN

คุณภาพอากาศในสถานประกอบการ





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com... www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
R01	SKC	224-PCXR4	602467	06/07/2023	1,000	1,500	2,000	991	1,506	2,002	1.007x – 14.479	1.000
R02	SKC	224-PCXR4	626450	06/07/2023	1,000	2,000	3,000	997	1,497	1,988	0.988x + 12.256	1.000
R03	SKC	224-PCXR4	691592	06/07/2023	1,000	1,500	2,000	1,002	1,498	2,002	1.003x – 5.881	1.000
R04	SKC	224-PCXR4	691672	06/07/2023	1,000	1,500	2,000	995	1,491	1,994	0.997x – 2.717	1.000
R05	SKC	224-PCXR4	798470	06/07/2023	1,000	1,500	2,000	992	1,505	1,997	1.001x – 6.538	1.000
R06	SKC	224-PCXR4	798456	06/07/2023	1,000	1,500	2,000	994	1,497	1,993	0.994x – 0.976	1.000
R07	SKC	224-PCXR4	798480	04/07/2023	1,000	1,500	2,000	993	1,490	1,997	1.007x – 16.177	1.000
R08	SKC	224-PCXR4	883215	04/07/2023	1,000	1,500	2,000	1,010	1,499	2,003	0.989x + 11.332	0.999
R09	SKC	224-PCXR4	034650	04/07/2023	1,000	1,500	2,000	990	1,503	2,000	1.011x – 24.548	1.000
R10	SKC	224-PCXR4	091765	07/07/2023	1,000	1,500	2,000	996	1,509	1,992	0.999x + 0.299	1.000
R11	SKC	224-PCXR4	091763	07/07/2023	1,000	1,500	2,000	999	1,497	1,985	1.000x – 9.834	0.999
R12	SKC	224-PCXR4	091568	07/07/2023	1,000	1,500	2,000	995	1,499	1,998	1.001x – 6.774	1.000
R13	SKC	224-PCXR4	091638	07/07/2023	1,000	1,500	2,000	1,001	1,510	1,989	0.988x + 16.559	1.000
R14	SKC	224-PCXR4	091764	07/07/2023	1,000	1,500	2,000	993	1,501	1,997	1.013x – 30.102	0.999
R15	SKC	224-PCXR8	529457	07/07/2023	1,000	1,500	2,000	1,000	1,499	2,001	0.998x – 3.682	0.999
R16	SKC	224-PCXR8	529643	05/07/2023	1,000	1,500	2,000	997	1,494	1,992	0.992x + 2.530	1.000
R17	SKC	224-PCXR8	529645	05/07/2023	1,000	1,500	2,000	994	1,507	1,998	1.006x – 15.440	0.999
R18	SKC	224-PCXR8	566756	05/07/2023	1,000	1,500	2,000	990	1,496	1,996	1.000x – 6.873	1.000
R19	SKC	224-PCXR8	566802	05/07/2023	1,000	1,500	2,000	1,001	1,497	1,998	1.003x – 14.352	0.999
R20	SKC	224-PCXR8	529089	03/07/2023	1,000	1,500	2,000	990	1,499	2,001	1.019x – 39.318	0.999
R21	SKC	224-PCXR8	665728	03/07/2023	1,000	1,500	2,000	997	1,493	1,997	0.999x – 3.765	1.000
R22	SKC	224-PCXR8	707444	03/07/2023	1,000	1,500	2,000	1,002	1,511	2,001	1.000x – 2.666	0.999
R23	SKC	224-PCXR8	761067	05/07/2023	1,000	1,500	2,000	1,011	1,475	1,989	0.980x + 20.504	0.999
R24	SKC	224-PCXR8	707893	04/07/2023	1,000	1,500	2,000	995	1,507	1,998	1.007x – 16.619	0.999
R25	SKC	224-PCXR8	761052	04/07/2023	1,000	1,500	2,000	1,009	1,494	1,993	0.984x + 21.169	1.000
R26	SKC	224-PCXR8	707956	06/07/2023	1,000	1,500	2,000	1,011	1,499	2,004	1.001x – 3.674	0.999
R27	SKC	224-PCXR8	707398	06/07/2023	1,000	1,500	2,000	995	1,499	1,999	1.005x – 14.830	1.000
R28	SKC	224-PCXR8	707481	04/07/2023	1,000	1,500	2,000	1,003	1,499	2,000	1.001x – 11.858	0.998
R29	SKC	224-PCXR8	707402	04/07/2023	1,000	1,500	2,000	1,002	1,492	1,987	0.985x + 16.145	1.000
R30	SKC	224-PCXR8	093811	07/07/2023	1,000	1,500	2,000	999	1,492	1,991	0.994x + 4.391	1.000
R31	SKC	224-PCXR8	093183	04/07/2023	1,000	1,500	2,000	1,000	1,499	1,999	0.989x + 8.339	0.999
R32	SKC	224-PCXR8	671950	04/07/2023	1,000	1,500	2,000	997	1,499	1,991	0.995x + 4.048	1.000
R33	SKC	224-PCXR4	626254	04/07/2023	1,000	1,500	2,000	993	1,501	1,998	1.014x – 32.194	0.999
R34	SKC	224-PCXR4	626131	04/07/2023	1,000	1,500	2,000	1,001	1,498	2,002	1.006x – 12.316	1.000
R35	SKC	224-PCXR8	707460	03/07/2023	1,000	1,500	2,000	998	1,496	1,993	0.993x + 5.945	1.000
R36	SKC	224-PCXR8	707446	07/07/2023	1,000	1,500	2,000	1,003	1,497	1,999	1.008x – 18.814	0.999
R37	SKC	224-PCXR8	707432	07/07/2023	1,000	1,500	2,000	995	1,497	1,998	0.995x + 5.662	1.000
R38	SKC	224-PCXR8	707349	07/07/2023	1,000	1,500	2,000	996	1,498	1,999	1.002x – 7.662	1.000
R39	SKC	224-PCXR8	761095	04/07/2023	1,000	1,500	2,000	1,000	1,514	1,992	0.984x + 18.826	0.999

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature . 25  $\pm$  3  $^{\circ}$ C  
Pressure . 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
R40	SKC	224-PCXR4	612753	07/07/2023	1,000	1,500	2,000	1,000	1,500	2,001	1.007x – 13.778	1.000
R41	SKC	224-PCXR4	626140	05/07/2023	1,000	1,500	2,000	991	1,508	2,006	1.021x – 39.143	0.999
R42	SKC	224-PCXR4	626463	05/07/2023	1,000	1,500	2,000	997	1,492	1,997	1.000x – 2.482	1.000
R43	SKC	224-PCXR4	626129	05/07/2023	1,000	1,500	2,000	1,002	1,500	2,003	1.011x – 20.839	0.999
R44	SKC	224-PCXR4	602753	05/07/2023	1,000	1,500	2,000	1,001	1,494	1,991	0.994x + 2.925	1.000
R45	SKC	224-PCXR4	626137	05/07/2023	1,000	1,500	2,000	991	1,504	2,000	1.018x – 37.211	0.999

Calibrated by :

Approved by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-R01	Dwyer	VFB-65	05/07/2023	500	1,000	2,000	501.2	993.0	1978.7	0.999x – 3.855	0.999
H-R02	Dwyer	VFB-65	05/07/2023	500	1,000	2,000	501.5	998.1	1986.7	1.000x – 2.024	1.000
H-R03	Dwyer	VFB-65	04/07/2023	500	1,000	2,000	501.2	989.3	1995.7	0.992x + 3.827	1.000
H-R04	Dwyer	VFB-65	10/07/2023	500	1,000	2,000	496.3	991.2	2014.5	1.006x – 10.883	1.000
H-R05	Dwyer	VFB-65	05/07/2023	500	1,000	2,000	499.1	987.9	1988.7	1.002x – 6.676	1.000
H-R06	Dwyer	VFB-65	06/07/2023	500	1,000	2,000	504.7	994.0	1980.6	0.998x – 1.539	0.999

Calibrated by :

Approved by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
L-R01	Dwyer	VFA-21	05/07/2023	50	100	200	50.6	100.9	204.1	0.983x + 2.913	1.000
L-R02	Dwyer	VFA-21	05/07/2023	50	100	200	50.4	101.9	200.8	1.003x – 0.034	0.999
L-R03	Dwyer	VFA-21	04/07/2023	50	100	200	50.1	100.1	202.1	1.006x + 0.170	1.000
L-R04	Dwyer	VFA-21	10/07/2023	50	100	200	50.2	100.8	203.3	1.002x + 0.502	1.000
L-R05	Dwyer	VFA-21	05/07/2023	50	100	200	50.1	101.1	202.8	0.999x + 0.445	0.999
L-R06	Dwyer	VFA-21	06/07/2023	50	100	200	50.7	101.3	202.5	0.998x + 1.435	1.000

Calibrated by :

Approved by :





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY :

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23° C  $\pm$  1° C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY  
COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





## GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0823/21044

Instrument Type : GC

Model : CP-3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 09/08/2023

### ELECTRONIC TEST

CPU	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
LCD TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
VENT TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
KEY ECHO TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DESTRUCTION RAM TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

### RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detector ( FID Channel Front)

INJECTOR : Capillary Injector Model 1079

#### GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column: Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218 g/L C14, C15, C16 in hexane

SENSITIVITY TEST: C15. ( Area count ) = 362,972 Counts.





## Detector Sensitivity ( FID )

Detector Response	Result	Specification
Baseline Noise ( $\mu$ V)	1.47	$\leq 50$
Baseline Drift (%)	0.09	$\leq 1$
Sensitivity ( S/N for C15)	19,600	$\geq 1,024$

## Temperature Specification

Temperature	Set	Result	Specification
Column Oven ( $^{\circ}$ C)	80	80	$\pm 5$
Injector ( $^{\circ}$ C)	220	220	$\pm 5$
Detector ( $^{\circ}$ C)	300	300	$\pm 5$
Incubator ( $^{\circ}$ C)	60	N/A	$\pm 5$

## Relative Standard Deviation % ( % RSD)

Checkout Procedure	Result	Specification
Area C15 ( %)	1.52	$\leq 5$
Retention Time C15( %)	0.01	$\leq 0.5$

APPROVED

Signature:

Engineer

Date : 09/08/2023







บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

### Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	357,863
C15 Area 2	357,824
C15 Area 3	367,724
C15 Area 4	361,724
C15 Area 5	369,724
C15 Area Average	362,972
* % RSD ( < 5 % )	1.52

\* The precision specification should be less than 2.0 % RSD \*\* ( Relative Standard Deviation ) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five ( 5 ) samples.

\*\* (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = ( \text{std.dev} / \text{avg} ) * 100$$

Compliance	
Performance by	
Date	



Comments			
Reviewed by		Date	09/08/2023



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

### Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	4.125
C15 RT 2	4.125
C15 RT 3	4.125
C15 RT 4	4.124
C15 RT 5	4.124
C15 RT Average	4.122
* % RSD ( < 0.5 % )	0.01

\* The precision specification should be less than 0.5 % RSD \*\* ( Relative Standard Deviation ) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five ( 5 ) samples.

\*\* (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = ( \text{std.dev} / \text{avg} ) * 100$$

Compliance	
Performance by	
Date	



Comments			
Reviewed by			Date 09/08/2023



VARIAN



ระดับเสียง

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

## CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.  
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.  
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.  
4. Digital Multimeter Agilent 34401A S/N MY44005560.  
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.  
6. Audio Analyzer Keithley 2015-P S/N 4106495.  
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 27 Mar. 2023

Date of Calibration : 29 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa , Corrected to Reference Conditions : 101.325 kPa , 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.94	-0.06	$\pm 0.10$	$\pm 0.40$ dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	$\pm 1.5$	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	$\pm 0.50$	$\pm 3.0\%$

Note : 1. No adjustment.


2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :



Approved by :

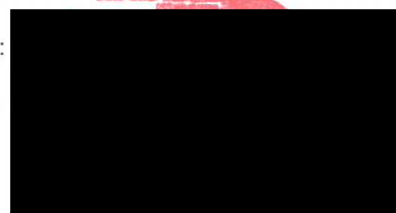

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 29 Mar. 2023

Date of Issue : 30 Mar. 2023

Ref : 2011266032701228001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise R\_483/23

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	29 March 2023
		Due Date	29 March 2024


### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R09	ACO	6236	00172035	17 September 2023	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.94 ± 0.10 dB	

Calibrated by :



Approved by :







บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R\_659/23

## Sound Level Meter Calibration Report


### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	29 March 2023
		Due Date	29 March 2024


### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R08	ACO	6236	00152082	14 November 2023	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.94 ± 0.10 dB	

Calibrated by :



Approved by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise R\_482/23

## Sound Level Meter Calibration Report


### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	29 March 2023
		Due Date	29 March 2024


### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R07	ACO	6236	00152080	17 September 2023	94.0	94.0
ACO-R10	ACO	6236	00172037	17 September 2023	94.1	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.94 ± 0.10 dB	

Calibrated by :



Approved by :







บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72; Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Noise R\_658/23

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	29 March 2023
		Due Date	29 March 2024


### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R23	ACO	6236	00192035	14 November 2023	94.0	94.0
ACO-R46	ACO	6236	00192058	14 November 2023	94.1	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.94 ± 0.10 dB	

Calibrated by :



Approved by :

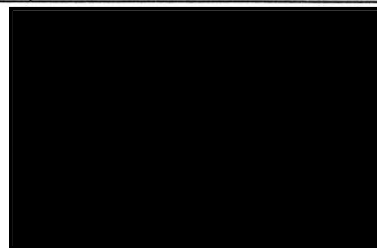

คุณภาพน้ำทิ้ง





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 23E8494  
REFERENCE No : 70413-1


PAGE : 1 OF 3

## Certificate of Calibration

**EQUIPMENT** : pH METER  
**MANUFACTURER** : HANNA  
**MODEL** : HI 3512  
**SERIAL No** : TH118035  
**ID No** : pH04/56  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 06-Sep-23

**APPROVED BY** : 

**ISSUED DATE** : 06-Sep-23

**RECEIVED DATE** : 31-Aug-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 2 OF 3

## Calibration Report

EQUIPMENT : pH METER  
MANUFACTURER : HANNA  
ID No : pH04/56  
RECEIVED DATE : 31-Aug-23  
AMBIENT TEMPERATURE : 23 ° C ± 3 ° C  
MODEL : HI 3512  
SERIAL NUMBER : TH118035  
CALIBRATION DATE : 06-Sep-23  
RELATIVE HUMIDITY : 50 % RH ± 10% RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	23E1312	19-Apr-24
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION : ADJUSTMENT

#### 1. DISPLAY UNIT ONLY

SLOPE FACTOR  $k = 2.303 \text{ RT/F} = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.6	-0.49	-0.290	0.15	2.00
354.95	355.4	-0.45	0.741	0.15	2.00
295.80	296.3	-0.50	1.773	0.15	2.00
236.64	237.1	-0.46	2.804	0.15	2.00
177.48	177.9	-0.42	3.835	0.15	2.00
118.32	118.7	-0.38	4.867	0.15	2.00
59.16	59.6	-0.44	5.898	0.15	2.00
0.00	0.4	-0.40	6.930	0.15	2.00
-59.16	-58.8	-0.36	7.961	0.15	2.00
-118.32	-117.9	-0.42	8.992	0.15	2.00
-177.48	-177.1	-0.38	10.024	0.15	2.00
-236.64	-236.3	-0.34	11.055	0.15	2.00
-295.80	-295.5	-0.30	12.087	0.15	2.00
-354.95	-354.6	-0.35	13.118	0.15	2.00
-414.11	-413.8	-0.31	14.149	0.15	2.00





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 3 OF 3

## Calibration Report

### RESULT OF CALIBRATION (CONTINUE) :

#### 2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ pH)	COVERAGE FACTOR k
4.006	4.006	0.000	4.015	0.012	2.00
7.000	7.000	0.000	6.914	0.012	2.00
10.008	10.010	-0.002	9.996	0.014	2.00

#### 3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ( $^{\circ}$ C)	UUC READING ( $^{\circ}$ C)	CORRECTION ( $^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ $^{\circ}$ C)	COVERAGE FACTOR k
25.005	25.0	0.005	---	0.0085	2.00

#### 4. PERCENT SLOPE 100%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



## Certificate of Calibration

**Certificate No. :** 66-400065-2

**Page : 1 of 2**

**Submitted by :** S. P. S Consulting Service Co.,Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

**Equipment :** Liquid in Glass Thermometer

**Manufacturer :** SK

**Model :** N/A

**Range :** 0 °C to 100 °C

**Resolution :** 1 °C

**Serial No. :** N/A

**Immersion :** Total

**ID No. :** TM21/59

**Environment :** Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

**Date of Received :** 01 February 2023

**Date of Calibration :** 06 February 2023

**Date of Issue :** 06 February 2023

**Calibrated by :** Chortip Samchusri

**Calibration Method :** This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units


1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)
400004	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)

Approved by



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.





## Certificate of Calibration

**Certificate No. :** 66-400065-2

**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

Ice point check : UUC\* reading 0 ° C Standard reading 0.3606 ° C

Standard Reading ( ° C )	UUC Reading ( ° C )	Correction ( ° C )	Uncertainty ( ± ° C )
20.3607	20	0.4	0.31


### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$  ,  
providing a level of confidence of approximately 95%

- o0o -







CERTIFICATE No : 23M2442

REFERENCE No : 68471-2

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : SARTORIUS

**MODEL** : BSA224S-CW

**SERIAL No** : 36591843

**ID No** : BA 09/61

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** : 

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23





CERTIFICATE No : 23M2442

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	MODEL	:	BSA224S-CW
MANUFACTURER	:	SARTORIUS	S/N	:	36591843
ID No	:	BA 09/61	RECEIVED DATE	:	10-Mar-23
AIR PRESSURE	:	1010mbar $\pm$ 1mbar	CALIBRATION DATE	:	10-Mar-23
AMBIENT TEMPERATURE	:	23° C $\pm$ 1° C	RELATIVE HUMIDITY	:	49 %RH $\pm$ 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000058
0.1	0.1000	0.0000	0.000059
0.2	0.2000	0.0000	0.000059
0.5	0.5000	0.0000	0.000060
1.0	1.0000	0.0000	0.000060
2.0	2.0000	0.0000	0.000061
5.0	5.0000	0.0000	0.000063
10.0	10.0000	0.0000	0.000067
20.0	20.0001	-0.0001	0.000073
50.0	50.0000	0.0000	0.00011
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	99.9999
3	99.9998
4	100.0001
5	100.0000
OFF-CENTER LOADING	0.0002

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERT.No.: HS-U017D

Calibration Date : 3 Apr 23  
 Submitted by : S.P.S CONSULTING SERVICE CO.,LTD  
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,  
 Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C  
 Avg Water Temp : 20 °C  
 Air Pressure : 760.00 mmHg  
 Salinity : 0 ppt

Model : YSI 5000  
 S/N : 15B100751  
 Probe : YSI 5010  
 S/N : 22D100097  
 ID NO. : -  
 Air Temp ref : S/N. E00522  
 Barometric ref : S/N. E00522  
 Water Temp ref : S/N. 11431  
 Technician : Kittipong M.

#### Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-
Overall Status	(PASS)		

#### Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature

(Kittipong Maekwong)

Laboratory Manager

(Natenapha Pisatkunchon)





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 23T0959

REFERENCE No : 68047-2

PAGE : 1 OF 3

## Certificate of Calibration

**EQUIPMENT** : COD REACTOR

**MANUFACTURER** : HACH

**MODEL** : DRB200

**SERIAL No** : 15110C0235

**ID No** : CRB 05/59

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 07-Feb-23

**APPROVED BY** :

**ISSUED DATE** : 07-Feb-23

**RECEIVED DATE** : 31-Jan-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02





CERTIFICATE No : 23T0959

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : COD REACTOR  
MANUFACTURER : HACH  
ID NUMBER : CRB 05/59  
RECEIVED DATE : 31-Jan-23  
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB200  
SERIAL NUMBER : 15110C0235  
CALIBRATION DATE : 07-Feb-23  
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	22T7511	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

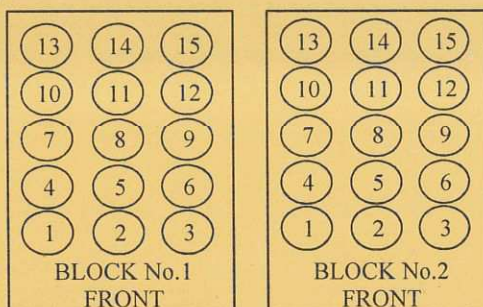

### TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	149.4
	2	149.5
	3	149.4
	4	149.4
	5	149.7
	6	149.6
	7	149.4
	8	149.3
	9	149.6
	10	149.6
	11	149.7
	12	149.3
	13	149.5
	14	149.4
	15	149.6
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>Customer :</b> <u>S.P.S.Consulting Service Co.,Ltd</u>	<b>Date Tested:</b> <u>January 4, 2024</u>	
	<b>Recommendation Recertification</b>	
<b>Address :</b> <u>7 Soi Phaholyothin 24</u>	<b>Period</b> <u>6</u> <b>Months</b>	
<u>Paholyothin Road</u>	<b>Recertification Due:</b> <u>July 4, 2024</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	<b>Date Last Certified:</b> <u>July 6, 2023</u>	
<b>User Name:</b> <u>[REDACTED]</u>	<b>Visit Number:</b> <u>2 of 2</u>	
<b>Phone:</b> <u>083-9269252</u>	<b>PerkinElmer Phone:</b> <u>02-719-6420 ext 206</u>	
<b>Fax:</b> <u>02-513-4221</u>	<b>PerkinElmer Fax:</b> <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
<b>MODEL</b>	<b>SERIAL NUMBER</b>	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>December 30, 2024</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>March 30, 2024</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>February 28, 2024</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2024</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 4, 2024**1. MECHANICAL CHECKS**

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK**2. OPTICAL CHECKS**

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK**3. COOLING SYSTEM CHECKS**

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A**4. PERFORMANCE CHECKS**

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

SERIAL NUMBER : 077C7042401DATE TESTED : January 4, 2024

PARAMETER		SPECIFICATION		FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.007		0.00529	
	Ni 231.604 nm	≤ 0.008		0.00672	
	Ni 341.476 nm	≤ 0.012		0.00793	
Spectral Resolution : VIS	La 408.672 nm	≤ 0.020		0.01588	
	Ba 455.403 nm	≤ 0.025		0.02280	
Precision					
	As 193.656 nm	% RSD	< 1.0	0.92	%
	Zn 213.856 nm	% RSD	< 1.0	0.95	%
	Mn 257.610 nm	% RSD	< 1.0	0.75	%
	La 379.478 nm	% RSD	< 1.0	0.44	%
	Ba 455.403 nm	% RSD	< 1.0	0.46	%
	Ba 493.408 nm	% RSD	< 1.0	0.37	%
Detection Limits : Axial	Tl 190.080 nm	3(sd)		19.99	ppb
	As 193.696 nm	3(sd)		26.66	ppb
	Pb 220.353 nm	3(sd)		1.81	ppb
Detection Limits : Radial	As 193.696 nm	3(sd)		38.21	ppb
	Zn 213.856 nm	3(sd)		2.48	ppb
	Mn 257.610 nm	3(sd)		0.59	ppb
	La 379.478 nm	3(sd)		5.52	ppb
	Ba 455.403 nm	3(sd)		0.13	ppb
	Ba 493.408 nm	3(sd)		1.08	ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd 226.502 nm	≤ 150 ppb		141.47	
BEC : Radial (IB X 1000)/(IS-IB)	Mn 257.610 nm	≤ 45 ppb		29.04	



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 4, 2024**Remarks :**

Commissioning follow as commissioning performance sheets.

---

---

---

---

---

---

---

---

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

**Service Department PerkinElmer Ltd.****Authorized Representative**

( Mr. Wiphan Promlunda )

Service Engineer



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : CONDUCTIVITY METER  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : SEVEN COMPACT S230  
SERIAL NO. : C141708983/5821320179  
CLID. NO. : 272300452  
JOB CONTROL NO. : 230211016445

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 11 February 2023

DATE OF ISSUED : 15 February 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer

Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
15 February 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23016445

F3-011-04/01-12

page 1 of 4



@clccalibration

## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : CONDUCTIVITY METER  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : SEVEN COMPACT S230  
SERIAL NO. : C141708983/5821320179  
DATE OF CALIBRATION : 13 February 2023

#### ENVIRONMENT CONDITIONS :

Temperature :  $(25 \pm 2.5) ^\circ\text{C}$  Relative Humidity :  $(50 \pm 15) \% \text{ RH}$

#### PROCEDURE USED :

This instrument [ Conductivity Meter ] was calibrated under procedure No. **WI-305-130**. The calibration was performed by direct measurement with Certified Reference Material (CRM) and Reference Material (RM) .

This instrument [ Temperature ] was calibrated under procedure No. **WI-305-244**. The calibration was performed by Comparison with Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

1. Potassium Chloride Solution ( nominal 1.41 mS/cm , nominal 12.8 mS/cm )
2. Conductivity Solution , Hanna Product Code HI 7033L Lot Number 6436.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, ASL Model T100-250-1D S/N. L0193A-1-1.





## TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Merck Co., Ltd.

Certificate No. HC02139203 , HC04515254. Due Date 30 June 2023 , 30 November 2023.

2. The measurements are traceable to International System of Units (SI) , through Hanna instruments.

Certificate No. 12E12 , Due Date May 2024 .

3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q22130792, Due Date 05 January 2024.

4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0823/65, Due Date 22 August 2023.

5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).

Certificate No. TT-0166-22, Due Date 01 December 2023.

## UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"



## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Conductivity Meter.

### CALIBRATION DATA

#### 1. Conductivity Solution Test @ 25°C

Standard Conductivity Solution	DUC Reading	Uncertainty of Measurement	k Factor
*84.00 µS/cm	84.04 µS/cm [Cell Constant 0.548589]	± 1.00 µS/cm	2,00
1412.0 µS/cm	1413 µS/cm [Cell Constant 0.548589]	± 21.0 µS/cm	2,00
12.85 mS/cm	12.88 mS/cm [Cell Constant 0.573538]	± 0.19 mS/cm	2,00

Note. \* means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 138 of 138

#### \*2. Temperature Result [ Probe Conductivity ]

Immersion depth (mm)	Actual Temperature ( °C )	DUC Reading ( °C )	Correction ( °C )	Uncertainty ± ( °C )
100	25.00	25.0	0.00	0.07

Note. The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2,00$ .

\* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###





คุณภาพดิน

# Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: CN10630014  
Organization Name: S.P.S.Consulting Service Co.,Ltd.  
Organization Location: 7 Soi Paholyothin 24 Bangkok 10900  
Date: September 1, 2023 2:41:39 PM  
EQP Name: AgilentRecommended , AgilentRecommended  
EQP Revision: GC.02.50, GCMS.02.50  
Overall Qualification Status: Pass

## System Inspection and Basic Safety and Operation

Name: 6890

Setpoint Status: Pass

## Overall System Inspection and Basic Safety and Operation Test Status

Pass

## Inlet Pressure Decay

Name: 6890

Front SSL

Setpoint Status: Pass

Pressure: 25.0 psi

Pressure Change: -0.2 psi /5 minutes

Agilent Recommended:  $\geq -2.0$  and  $\leq 0.5$ 

## Overall Inlet Pressure Decay Test Status

Pass

## Inlet Pressure Accuracy

Name: 6890

Front SSL

Date: September 1, 2023 2:41:39 PM  
System ID: CN10630014



## Setpoint Status:

Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	24.8	psi
Accuracy:			0.2	psi
Agilent Recommended:			<= 1.2	

## Overall Inlet Pressure Accuracy Test Status

Pass

## Inlet Pressure Accuracy

Name:

6890

Back

SSL

## Setpoint Status:

Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	24.9	psi
Accuracy:			0.1	psi
Agilent Recommended:			<= 1.2	

## Overall Inlet Pressure Accuracy Test Status

Pass

## Detector Flow Accuracy

Name:

6890

Front

FID

## Setpoint Status:

Pass

Flow Type:

Fuel

Setpoint:

30.0

mL/min

Measured Flow:

30.8

mL/min

Accuracy:

0.8

mL/min

Agilent Recommended:

&lt;=

10.0

% setpoint

( 3.0

mL/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Date:

September 1, 2023 2:41:39 PM

System ID:

CN10630014

## Setpoint Status:

Pass

Flow Type:

Oxidizer

Setpoint:

400.0

mL/min

Measured Flow:

395.3

mL/min

Accuracy:

4.7

mL/min

Agilent Recommended:

&lt;=

10.0

% setpoint

(

40.0

mL/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

## Setpoint Status:

Pass

Flow Type:

Makeup

Setpoint:

25.0

mL/min

Measured Flow:

24.7

mL/min

Accuracy:

0.3

mL/min

Agilent Recommended:

&lt;=

10.0

% setpoint

(

2.5

mL/min

)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

## Overall Detector Flow Accuracy Test Status

Pass

## GC Oven Temperature Accuracy

Name:

6890

Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

230.0

229.5

°C

Accuracy:

-0.5

°C

Agilent Recommended:

&gt;=

-1.0

% setpoint in K

(

-5.0

°C

)

&lt;=

1.0

% setpoint in K

(

5.0

°C

)

Date:

September 1, 2023 2:41:39 PM

System ID:

CN10630014



## Setpoint Status:

Pass

Zone:

Oven

Setpoint/Actual

Temperature:

100.0

99.8

°C

Accuracy:

-0.2

°C

Agilent Recommended:

&gt;=

-1.0

% setpoint in K

(

-3.7

°C

)

&lt;=

1.0

% setpoint in K

(

3.7

°C

)

## Overall GC Oven Temperature Accuracy Test Status

Pass

## GC Oven Temperature Stability

Name:

6890

## Setpoint Status:

Pass

Setpoint/Average

Temperature:

100.0

99.83333

°C

Stability:

0.1

°C

Agilent Recommended:

&lt;=

0.5

## Overall GC Oven Temperature Stability Test Status

Pass

## Scouting Run

Tested Combination1

Front

SSL

/ Front

FID

Injection Tower

Name:

7683B

## Setpoint Status:

Completed

Injection Volume on Column:

1.0

uL

## Overall Scouting Run Status

Completed

## Noise and Drift

Tested Combination1

Front

SSL

/ Front

FID

Date:

September 1, 2023 2:41:39 PM

System ID:

CN10630014

Name: 6890

Setpoint Status: Pass

Base Signal: 15.8 pA

	ASTM Noise counts	Drift counts/Hr
Agilent Recommended:	443.17	18437.04
Status:	<= 768.00 Pass	<= 19200.00 Pass

## Overall Noise and Drift Test Status

Pass

## Injection Precision

Tested Combination1	Front	SSL	/ Front	FID
Name:	7683B			
Setpoint Status:	Pass			
Injection Volume on Column:	1.0	uL		
Area RSD:	0.67	%	Retention Time RSD:	0.02 %
Agilent Recommended:	<= 3.00		<= 1.00	

## Overall Injection Precision Test Status

Pass

## Signal to Noise

Tested Combination1	Front	SSL	/ Front	FID
	Injection Tower			
Name:	6890			
Setpoint Status:	Pass			
Signal to Noise:	671482			
Agilent Recommended:	>= 300000			

Date: September 1, 2023 2:41:39 PM

System ID: CN10630014



## Overall Signal to Noise Test Status

Pass

## Log Amp

Tested Combination2 Back SSL / External SQ

Name: 5975A

Setpoint Status: Pass

## Overall Log Amp Test Status

Pass

## RFPA

Tested Combination2 Back SSL / External SQ

Name: 5975A

Setpoint Status: Pass

Amu: 1050 m/z

Drift After Five Minutes:

12 mV

RFPA Voltage:

466 mV

Agilent Recommended:

&gt;= -100 and &lt;= 100

&lt;= 1100

## Overall RFPA Test Status

Pass

## Tune EI

Tested Combination2 Back SSL / External SQ

Name: 5975A

Setpoint Status: Pass

Filament: 1

Setpoint Status: Pass

Filament: 2

## Overall Tune EI Test Status

Pass

**Signal to Noise EI****Tested Combination** Back SSL / External SQ**Name:** 5975A**Source:** EI - Inert**Filament:**

1

**Setpoint Status:** Pass**Signal to Noise:** 113**Agilent Recommended:**  $\geq$  80**Source:** EI - Inert**Filament:**

2

**Setpoint Status:** Pass**Signal to Noise:** 183**Agilent Recommended:**  $\geq$  80**Overall Signal to Noise EI Test Status**

Pass

**Date:** September 1, 2023 2:41:39 PM  
**System ID:** CN10630014



## Instrument Details

### Purpose

This section describes the as found system configuration.

### Details

#### System

System ID	CN10630014
Manufacturer	Agilent Technologies
Name	6890

#### Tested Combination1

Injection Technique	Injection Tower
Inlet	Front
Detector	Front
LTM Included?	No

#### Tested Combination2

Injection Technique	Manual Injection
Inlet	Back
Detector	External
LTM Included?	No

#### Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7683B
Model Number	G2913A
Serial Number	CN64136101
Firmware Revision	A.11.02
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

## Sampler 2

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

## Mainframe 1

Manufacturer	Agilent Technologies
Name	6890
Model Number	G1530N
Serial Number	CN630014
Firmware Revision	N.06.07
Oven Type	Standard

## Inlet 1

Manufacturer	Agilent Technologies
Name	6890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

## Inlet 2

Manufacturer	Agilent Technologies
Name	6890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes



## Detector 1

Manufacturer	Agilent Technologies
Name	6890
Type	FID
Adapter	Packed
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

## Detector 2

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

## Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5975A
Serial Number	US61633454
Firmware Revision	5.02.09
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

## MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Inert
Number of filaments	2

## Electronic Signature

### Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

### Details

Full Name of Signer:	Adirek Rattanawijit
Logged On User Name:	adirek.rattanawijit@non.agilent.com
Signature Creation Date:	September 1, 2023
Reason for Signature:	Executed protocol and published this original version of document

### Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

### Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

---

Date:	September 1, 2023 2:41:39 PM
System ID:	CN10630014



User Name: adlrek.rattanawijit  
 Hostname: C614-QA

System Id: CN10630014  
 Print Date: September 1, 2023 2:41:42 PM

## SPS\_OQGCMS\_CN10630014\_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 1, 2023 1:29:16 PM	Audit	SessionCreated	Session	None
September 1, 2023 1:29:16 PM	Start	Configuration	Session	None
September 1, 2023 1:29:16 PM	Audit	Entitlement	Licensing	User is Nonpaying and does not require an unlock code
September 1, 2023 1:32:47 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.50/Gc.02.50.eqp], EQP File Name: [Gc.02.50.eqp], EQP Name: [AgilentRecommended] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.50/GcMs.02.50.eqp], EQP File Name: [GcMs.02.50.eqp], EQP Name: [AgilentRecommended]
September 1, 2023 1:32:50 PM	End	Configuration	Session	None
September 1, 2023 1:32:54 PM	Start	Qualification	Session	OQ
September 1, 2023 1:32:54 PM	Start	Execution	System Inspection and Basic Safety and Operation - 6890: - Qualitative Test - No setpoints associated	None
September 1, 2023 1:33:23 PM	End	Execution	System Inspection and Basic Safety and Operation - 6890: - Qualitative Test - No setpoints associated	Run Count : 1

Page 1 / 9

User Name: adirek.rattanawijit  
 Hostname: C614-QA

System Id: CN10630014  
 Print Date: September 1, 2023 2:41:42 PM

## SPS\_OQGCMS\_CN10630014\_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 1, 2023 1:33:26 PM	Start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and ≤ 0.5 psi	None
September 1, 2023 1:33:34 PM	End	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and ≤ 0.5 psi	Run Count : 1
September 1, 2023 1:33:37 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: ≤ 1.2 psi	None
September 1, 2023 1:33:41 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: ≤ 1.2 psi	Run Count : 1
September 1, 2023 1:33:43 PM	Start	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: ≤ 1.2 psi	None
September 1, 2023 1:33:50 PM	End	Execution	Inlet Pressure Accuracy - Back SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: ≤ 1.2 psi	Run Count : 1
September 1, 2023 1:33:53 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: ≤ 10.0% setpoint	None
September 1, 2023 1:34:00 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: ≤ 10.0% setpoint	Run Count : 1
September 1, 2023 1:34:02 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: ≤ 10.0% setpoint	None
September 1, 2023 1:34:12 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: ≤ 10.0% setpoint	Run Count : 1

Page 2 / 9

Date: September 1, 2023 2:41:39 PM  
 System ID: CN10630014



User Name: adirek.rattanawijit  
 Hostname: C614-QA

System Id: CN10630014  
 Print Date: September 1, 2023 2:41:42 PM

## SPS\_OQGCMS\_CN10630014\_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 1, 2023 1:34:14 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
September 1, 2023 1:34:21 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
September 1, 2023 1:34:23 PM	Start	Execution	GC Oven Temperature Accuracy - 6890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
September 1, 2023 1:34:50 PM	Audit	Data	GC Oven Temperature Accuracy - 6890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
September 1, 2023 1:34:52 PM	End	Execution	GC Oven Temperature Accuracy - 6890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
September 1, 2023 1:34:55 PM	Start	Execution	GC Oven Temperature Accuracy - 6890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
September 1, 2023 1:35:33 PM	Audit	Data	GC Oven Temperature Accuracy - 6890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
September 1, 2023 1:35:35 PM	End	Execution	GC Oven Temperature Accuracy - 6890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
September 1, 2023 1:35:37 PM	Start	Execution	GC Oven Temperature Stability - 6890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None

Page 3 / 9

User Name: adlrek.rattanawijit

System Id: CN10630014

Hostname: C614-QA

Print Date: September 1, 2023 2:41:42 PM

## SPS\_OQGCMS\_CN10630014\_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 1, 2023 1:36:42 PM	Audit	Data	GC Oven Temperature Stability - 6890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
September 1, 2023 1:36:44 PM	End	Execution	GC Oven Temperature Stability - 6890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
September 1, 2023 1:36:47 PM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
September 1, 2023 1:37:18 PM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : C:\Users\Win 10 Home\Desktop\OQPV_GC\S PS\OQPV2023\OQPV2023\S COUT_001.D\FID1A.CH
September 1, 2023 1:37:41 PM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
September 1, 2023 1:37:44 PM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None
September 1, 2023 1:38:02 PM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : C:\Users\Win 10 Home\Desktop\OQPV_GC\S PS\OQPV2023\OQPV2023\N D_001.D\FID1A.CH
September 1, 2023 1:38:08 PM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1

Page 4 / 9

Date: September 1, 2023 2:41:39 PM  
System ID: CN10630014



User Name: adirek.rattanawijit

System Id: CN10630014

Hostname: C614-QA

Print Date: September 1, 2023 2:41:42 PM

## SPS\_OQGCMS\_CN10630014\_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 1, 2023 1:38:23 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Back SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 80	None
September 1, 2023 1:38:23 PM	Start	Execution	Tune EI - 5975A SQ: - Source: - None EI - Inert Filament 2 (Qualitative - No setpoints associated)	
September 1, 2023 1:38:58 PM	End	Execution	Tune EI - 5975A SQ: - Source: - Run Count : 1 EI - Inert Filament 2 (Qualitative - No setpoints associated)	
September 1, 2023 1:39:01 PM	Start	Execution	Tune EI - 5975A SQ: - Source: - None EI - Inert Filament 1 (Qualitative - No setpoints associated)	
September 1, 2023 1:39:16 PM	End	Execution	Tune EI - 5975A SQ: - Source: - Run Count : 1 EI - Inert Filament 1 (Qualitative - No setpoints associated)	
September 1, 2023 1:39:18 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Back SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 80	None
September 1, 2023 1:39:27 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Back SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 80	Data files Path : C:\Users\WIn10 Home\Desktop\OQPV_GC\S PS\OQPV2023\OQPV2023\S N_F1_001.D\data.ms
September 1, 2023 1:40:37 PM	End	Execution	Signal to Noise EI - Liquid Injection, Back SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 80	Run Count : 1
September 1, 2023 1:40:41 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Back SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 80	None

Page 5 / 9

User Name: adlrek.rattanawijit  
 Hostname: C614-QA

System id: CN10630014  
 Print Date: September 1, 2023 2:41:42 PM

## SPS\_OQGCMS\_CN10630014\_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 1, 2023 1:41:07 PM	Audit	Data	Signal to Noise EI - Liquid Injection, Back SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 80	Data files Path : C:\Users\Win10\Home\Desktop\OQPV_GCIS PS\OQPV2023\OQPV2023\SN_F2_001.D\data.ms
September 1, 2023 1:43:13 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Back SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 80	None
September 1, 2023 1:43:24 PM	Start	Execution	Signal to Noise EI - Liquid Injection, Back SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 80	None
September 1, 2023 1:43:36 PM	End	Execution	Signal to Noise EI - Liquid Injection, Back SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 80	Run Count : 1
September 1, 2023 1:43:41 PM	Start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
September 1, 2023 1:57:52 PM	Audit	AcqRestarted	Session	None
September 1, 2023 2:01:02 PM	Audit	SessionReloaded	Session	None
September 1, 2023 2:01:05 PM	Start	Qualification	Session	OQ
September 1, 2023 2:01:05 PM	Start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None

User Name: adirek.rattanawijit

System Id: CN10630014

Hostname: C614-QA

Print Date: September 1, 2023 2:41:42 PM

## SPS\_OQGCMS\_CN10630014\_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 1, 2023 2:01:39 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Win10 Home\Desktop\OQPV_GC\SPS\OQPV2023\IP_002.D\FID 1A.CH
September 1, 2023 2:01:39 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Win10 Home\Desktop\OQPV_GC\SPS\OQPV2023\IP_003.D\FID 1A.CH
September 1, 2023 2:01:39 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Win10 Home\Desktop\OQPV_GC\SPS\OQPV2023\IP_004.D\FID 1A.CH
September 1, 2023 2:01:39 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Win10 Home\Desktop\OQPV_GC\SPS\OQPV2023\IP_005.D\FID 1A.CH
September 1, 2023 2:01:39 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Win10 Home\Desktop\OQPV_GC\SPS\OQPV2023\IP_006.D\FID 1A.CH
September 1, 2023 2:01:39 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : C:\Users\Win10 Home\Desktop\OQPV_GC\SPS\OQPV2023\IP_007.D\FID 1A.CH
September 1, 2023 2:01:51 PM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1



User Name: adirek.rattanawijit  
 Hostname: C614-QA

System Id: CN10630014  
 Print Date: September 1, 2023 2:41:42 PM

## SPS\_OQGCMS\_CN10630014\_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 1, 2023 2:01:54 PM	Start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	None
September 1, 2023 2:02:04 PM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : C:\Users\Win 10 Home\Desktop\OQPV_GC\SPS\OQPV2023\SN_001.D\FID1A.CH
September 1, 2023 2:02:16 PM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1
September 1, 2023 2:03:19 PM	Start	Execution	Log Amp - 5975A SQ: - Source: EI - Inert	None
September 1, 2023 2:06:05 PM	End	Execution	Log Amp - 5975A SQ: - Source: EI - Inert	Run Count : 1
September 1, 2023 2:06:07 PM	Start	Execution	RFPA - 5975A SQ: - Source: EI - Inert	None
September 1, 2023 2:17:21 PM	End	Qualification	Session	OQ
September 1, 2023 2:17:21 PM	Start	Reporting	Session	None
September 1, 2023 2:24:55 PM	End	Reporting	Session	None
September 1, 2023 2:24:55 PM	Start	Qualification	Session	OQ
September 1, 2023 2:25:10 PM	Start	Execution	RFPA - 5975A SQ: - Source: EI - Inert	None
September 1, 2023 2:34:26 PM	End	Execution	RFPA - 5975A SQ: - Source: EI - Inert	Run Count : 1
September 1, 2023 2:36:18 PM	End	Qualification	Session	OQ

Page 8 / 9

Date: September 1, 2023 2:41:39 PM  
 System ID: CN10630014

User Name: adirek.rattanawijit  
Hostname: C614-QA

System Id: CN10630014  
Print Date: September 1, 2023 2:41:42 PM

## SPS\_OQGCMS\_CN10630014\_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
September 1, 2023 2:36:18 PM	Start	Reporting	Session	None
September 1, 2023 2:40:24 PM	Audit	Reporting	Session	Report Generated : Certificate

<b>Customer :</b>	S.P.S.Consulting Service Co.,Ltd	Date Tested:	January 4, 2024
<b>Address :</b>	7 Soi Phaholyothin 24 Paholyothin Road Jompol Chatuchak, Bangkok 1090	Recommendation Recertification Period	6 Months
<b>User Name:</b>	[REDACTED]	Recertification Due:	July 4, 2024
<b>Phone:</b>	083-9269252	Date Last Certified:	July 6, 2023
<b>Fax:</b>	02-513-4221	Visit Number:	2 of 2
		PerkinElmer Phone:	02-719-6420 ext 206
		PerkinElmer Fax:	02-318-5597

Page 1 of 4





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 4, 2024**1. MECHANICAL CHECKS**

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK**2. OPTICAL CHECKS**

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK**3. COOLING SYSTEM CHECKS**

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A**4. PERFORMANCE CHECKS**

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER :** 077C7042401
**DATE TESTED :** January 4, 2024

PARAMETER		SPECIFICATION		FINAL VALUE	
<b>Spectral Resolution : UV</b>	<b>As</b> 193.696 nm	≤ 0.007		0.00529	
	<b>Ni</b> 231.604 nm	≤ 0.008		0.00672	
	<b>Ni</b> 341.476 nm	≤ 0.012		0.00793	
<b>Spectral Resolution : VIS</b>	<b>La</b> 408.672 nm	≤ 0.020		0.01588	
	<b>Ba</b> 455.403 nm	≤ 0.025		0.02280	
<b>Precision</b>					
	<b>As</b> 193.656 nm	% RSD	< 1.0	0.92	%
	<b>Zn</b> 213.856 nm	% RSD	< 1.0	0.95	%
	<b>Mn</b> 257.610 nm	% RSD	< 1.0	0.75	%
	<b>La</b> 379.478 nm	% RSD	< 1.0	0.44	%
	<b>Ba</b> 455.403 nm	% RSD	< 1.0	0.46	%
	<b>Ba</b> 493.408 nm	% RSD	< 1.0	0.37	%
<b>Detection Limits : Axial</b>	<b>Tl</b> 190.080 nm	3(sd)		19.99	ppb
	<b>As</b> 193.696 nm	3(sd)		26.66	ppb
	<b>Pb</b> 220.353 nm	3(sd)		1.81	ppb
<b>Detection Limits : Radial</b>	<b>As</b> 193.696 nm	3(sd)		38.21	ppb
	<b>Zn</b> 213.856 nm	3(sd)		2.48	ppb
	<b>Mn</b> 257.610 nm	3(sd)		0.59	ppb
	<b>La</b> 379.478 nm	3(sd)		5.52	ppb
	<b>Ba</b> 455.403 nm	3(sd)		0.13	ppb
	<b>Ba</b> 493.408 nm	3(sd)		1.08	ppb
<b>BEC : Axial</b> (IB X 500)/(IS-IB)	<b>Cd</b> 226.502 nm	≤ 150 ppb		141.47	
<b>BEC : Radial</b> (IB X 1000)/(IS-IB)	<b>Mn</b> 257.610 nm	≤ 45 ppb		29.04	



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 4, 2024**Remarks :**

Commissioning follow as commissioning performance sheets.

---

---

---

---

---

---

---

---

This is to certify that the above tests have been performed and the configuration tested

☒

meets

☐

does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

**Service Department PerkinElmer Ltd**

**Authorized Representative:**

( Mr. Wiphan Promlumda )

Service Engineer