

ภาคผนวก จ

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Songkhla Lab	Iron	ICP-MS	SGK_CL0048	2-Aug-23	2-Feb-25	18
Songkhla Lab	Iron	Cold Room Water	SGK_CL0065	31-Jan-23	31-Jul-24	18
Songkhla Lab	Conductivity	Conductivity Meter	SGK_CL0032	3-May-23	3-May-24	12
Songkhla Lab	pH at 25 °C	pH meter	SGK_CL0030	28-Apr-23	28-Oct-24	18
Songkhla Lab	Turbidity	Turbidity Meter	SGK_FS0046	30-May-23	30-May-24	12
Songkhla Lab	BOD	Incubator	SGK_CL0028	13-Jul-23	13-Jan-25	18
Songkhla Lab	BOD	DO/BOD Analyser	SGK_CL0073	21-Nov-22	21-May-24	18
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Oil & Grease	Water Bath	SGK_CL0035	13-Jul-23	13-Jan-25	18
Songkhla Lab	Sulfide	Cold Room Water	SGK_CL0065	31-Jan-23	31-Jul-24	18
Songkhla Lab	Total Dissolved Solids 103-105°C	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Dissolved Solids 103-105°C	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Suspended Solids	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Mixed Liqour Suspended Solids	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Total Coliform	Autoclave	SGK_ML0001	5-Jan-23	5-Jul-24	18
Songkhla Lab	Total Coliform	Incubator	SGK_ML0013	6-Aug-22	6-Feb-24	18
Songkhla Lab	Total Coliform	pH Meter	SGK_ML0016	5-Jan-23	5-Jul-24	18
Songkhla Lab	Total Coliform	Water Bath	SGK_ML0021	30-Jan-23	30-Jul-24	18
Songkhla Lab	Residual Free Chlorine	Chlorine Meter	SGK_FS0137	3-Aug-22	27-Jun-24	18
Water Lab	Bicarbonate Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Carbonate Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Chloride	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	Hydroxide Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Methyl Orange Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Permanent Hardness	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Phenolphthalein Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Residual Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Temporary Hardness	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Total Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Total Hardness	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Total Coliform	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Incubator	BKK_ML0012	21-Nov-22	21-May-24	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0366	17-May-23	17-May-24	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	12-Jul-23	12-Jul-24	12



Agilent Technologies

Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A,D
968 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel. +662 637 6363
Fax: +662 632 4334
Email: ccc-smt@agilent.com
Website: www.agilent.com/chem

Customer Contact:

ALS Laboratory Group (Thailand) Co
Ltd
Branch Number 0002
114/1 Moo8 Banplu Subdistric Hat
Yai District
TAX ID : 0105540004859
kanitta.hemprasatpor@alsglobal.com
0811721334

Invoice To:

ALS Laboratory Group (Thailand) Co
Ltd
Branch Number 0002
114/1 Moo8 Banplu Subdistric Hat
Yai District SONGKHLA 90250

Payer:

ALS Laboratory Group (Thailand) Co
Ltd Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan
Luang
BANGKOK 10250

Delivery Site:

ALS Laboratory Group (Thailand) Co
Ltd
Branch Number 0002
114/1 Moo8 Banplu Subdistric Hat
Yai District

Location:

Room
Bldg
Lab
Dept

SERVICE REPORT

Customer Purchase Order Number:	Customer Number: 70579367
Service Request:	Service Request Date:
Service Order: 6005939422	Service Confirmation: 6905074481

REVIEW BYKovinna J.....
APPROVED BYKanitta H.....
NEXT CAL. DATE2/02/25.....

Direct Inquiries to:

Contact Name:	Customer Contact Center
Contact E-mail:	ccc-smt@agilent.com
Contact Telephone:	+662 637 6363
Contact Fax:	+662 632 4334

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our
full range of laboratory productivity solutions optimized for your
applications and workflows. Visit us at www.agilent.com/chem

Agilent Technologies (Thailand) Limited. Head Office
U Chu Liang Bldg. 22/F Unit A,D
968 Rama 4 Road, Silom, Bangrak,
Bangkok 10500 Thailand
Tax ID : 0105542068218

Citibank N.A. Bangkok Branch
399 Interchange 21 Building, Sukhumvit Road, Klongtoey Nau
Sub-district, Wattana District, Bangkok 10110 Thailand
Acc. No: 012-4452-007 ,
THB:Krung Thai Bank PCL
Siam Square Br.,416/1-2 Rama I Rd.,Pathumwan, BKK 10330
Thailand

ORIGINAL

Service Confirmation Number: 6905074481

Service Confirmation Date: 02.08.2023

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7900	ICPMS 7900 System			
G7201C	ICP-MS MassHunter SW only (excludes PC)	USH3799575	ICP MS 7900	SYS-IM-7900
G8403A	Agilent 7900 ICP-MS	JP16511669	ICP MS 7900	SYS-IM-7900
G8411A	ISIS 3 for Agilent 7850/7900/8900	JP16510379	ICP MS 7900	SYS-IM-7900

Service Items:



Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EOQ	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	02.08.2023	02.08.2023
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement - 100 % covered		

Additional Information:

Service Confirmation Number: 6905074481

Service Confirmation Date: 02.08.2023

Service Information:

Problem Description: WU-S-DQ-IM-7900-5001093854		
Service Provided: -Perform OQ hardware. -Test OQ of instrument ICP-MS = SGK_CL0048. All tests Passed.		
Service Overview Code: Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
Reported Hours: 9.0	Travel Hours: 3.0	
Customer Field Service Representative Name: Uthai Ngamlertsirichai	Customer Field Service Representative Signature: 	Date: 02 Aug 2023
Customer Name: KANITTA HEMPRASATPORN	Customer Signature: 	Date: 02 Aug 2023
Additional Comments:		



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 3-Feb-2023

Certificate No. : 23TH0527

CSR No. : A073/03634

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru,
A. Hat Yai, Songkhla 90250 TH

Calibration Place : Chemical Laboratory

Instrument Name : Cold Room Water

Manufacturer : MODULAR

Model : N/A

Serial No. : N/A

ID No. : SGK_CL0065

Resolution : 0.1 °C

Received Date : 31-Jan-2023

Calibrated Date : 31-Jan-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	Ananta B.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	31/07/24

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on G-20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :


Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

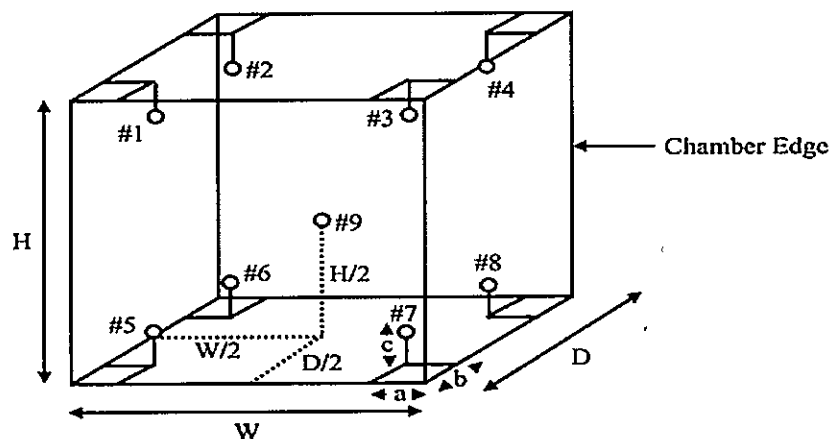

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 40.0 cm
H = 40.0 cm
D = 33.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Cold Room Water and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)														
	#1	#2	#3	#4	#5	#6	#7	#8	#9	Ref.10	#11	#12	#13	#14	#15
4	3.18	3.39	3.54	3.77	3.99	3.86	3.85	3.92	4.02	3.86	3.78	3.84	3.85	4.09	3.91

The uncertainty of measurement was $\pm$ 0.38 °C

3. Performance Result

The performance of the Cold Room Water are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability ($\pm$ °C)	Temperature Uniformity (°C)	Overall Variation (°C)
4	4.0	4.0	1.23	0.50	0.84

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI-18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH553

Page.: 1 of 2

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	Mettler Toledo
Model :	SevenCompact S230
Serial No. :	B608134488
ID No. :	SGK_CL0032
Condition As-Received:	Used Item
Received Date :	28 April 2023
Calibration Date :	03 May 2023
Reference :	2304-0804DSC-2
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8, Kanjanavanij Rd., Banphru, Hatyai, Songkhla 90250, Thailand
Ambient Temperature :	(25 $\pm$ 2.5) °C
Relative Humidity :	(50 $\pm$ 15) %
Calibration Procedure:	In -house method : - CP-CH6 : based on direct measurement by using certified reference material (CRM)
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	 Approved Signatory
☒ Malee Butkruea ☐ Saithip Meangmai ☐ Warakorn Lerngagtrakul	
Issue Date :	16 May 2023

REVIEW BY	 Ananta B.
APPROVED BY	 Kanitta H.
NEXT CAL. DATE	03/05/24

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0054235



Cert.No.: 23CH553

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	1963878	130RC095	22I1140	12 Sep 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
84.000 $\mu\text{S/cm}$	CPA Chem	823326	20 June 2023
1413.0 $\mu\text{S/cm}$	CPA Chem	826595	09 July 2023

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 1413.0 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 5816340156

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement ($\pm$)	Coverage factor k
84.000 $\mu\text{S/cm}$	91.0 $\mu\text{S/cm}$	88.4 $\mu\text{S/cm}$	0.62 $\mu\text{S/cm}$	2.00
1413.0 $\mu\text{S/cm}$	1490 $\mu\text{S/cm}$	1414 $\mu\text{S/cm}$	9.2 $\mu\text{S/cm}$	2.00

Remark - UUC* = Unit Under Calibration

- Adjustment Cell constant = 0.101842 cm^{-1}

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malu.

a 1161556



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.seal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23CH0203

CSR No. : A088/04367

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK_CL0030

Electrode No. : 1204613

Received Date : 28-Apr-2023

Calibrated Date : 28-Apr-2023

Ambient Temperature : (25 ± 3) °C

Relative Humidity : (55 ± 15) %

REVIEW BY	Ananta B.
APPROVED BY	Kamrta H.
NEXT CAL. DATE	28 / 10 / 2024

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH

- SCaL : Sounthern Calibration Service Co., Ltd.,

- WK : WK Electric Co., Ltd.

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

**Details of Calibration****1. Reference Standard Equipment Used:**

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02994	1777	5-Sep-2024
Standard Solution	7.000	C03007	1787	17-Oct-2024
Standard Solution	10.012	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024
Digital Thermometer With Sensor	DP-77	I.360896	22SDTH005	8-Aug-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :**1. Electrical Measurement**

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)
	(mV)	(pH)		
177.48	177.5	3.70	-0.02	0.17
0.00	0.0	6.70	0.00	0.13
-177.48	-177.4	9.80	-0.08	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.005	3.97	159.2	0.035	0.0090
6.999	6.98	-15.4	0.019	0.013
10.012	9.95	-188.0	0.062	0.036

3. After Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.005	3.97	158.9	0.035	0.0090
6.999	7.01	-17.5	-0.011	0.013
10.012	9.98	-187.6	0.032	0.036

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	25.032	25.1	-0.068	0.11

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Internal Calibration

REVIEW BY	Somsak J.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	30/5/24

Equipment : Turbidity Meter
ID No. : SGK_FS0046
Calibrate Date : May30 ,2023

Manufacture : HACH
Model : 2100Q/QIS
Serial No. : 19030C074494

Calibration Point	1st (NTU)	2nd (NTU)	3rd (NTU)	AVG (NTU)	Specifications	Evaluate
Standard 20 NTU	20.1	20.0	20.1	20.1	19 to 21 NTU	Pass
Standard 100 NTU	100.0	100.0	101.0	100.3	95 to 105 NTU	Pass
Standard 800 NTU	800.0	800.0	800.1	800.0	760 to 840 NTU	Pass

Calibrated by Somsak J.
(Scientist 2)

Approved by : Kanitta H.
(Section head)

PC 14/02/23

HACH COMPANY



An ISO 9001 Certified Company

P.O.Box 389
Loveland, CO 80539
(970) 669-3050

Certificate of Analysis

This is a Component of 2659405-TH lot A2307

Page 1

COMMODITY: STABLCAL|sup|TS|sup0 FORMAZIN STANDARD 20 NTU
COMMODITY NUMBER: 2684801 MANUFACTURE DATE: DATE OF ANALYSIS:
LOT NUMBER: A2304 11/14/2022 11/18/2022

TEST	SPECIFICATIONS	RESULTS
Turbidity	19 to 21 NTU	20.3 NTU

The expiration date is Feb 2024

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NIST does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

Certified by

Scott Als
Analytical Services Chemist

fe 17/02/23

HACH COMPANY



An ISO 9001 Certified Company

P.O.Box 389
Loveland, CO 80539
(970) 669-3050

Certificate of Analysis

This is a Component of 2659405-TH lot A2307

Page 1

COMMODITY: STABLCAL|sup|TS|sup0 FORMAZIN STANDARD 100 NTU
COMMODITY NUMBER: 2684901 MANUFACTURE DATE: DATE OF ANALYSIS:
LOT NUMBER: A2299 11/10/2022 11/17/2022

TEST	SPECIFICATIONS	RESULTS
Turbidity	95 to 105 NTU	102.0 NTU

The expiration date is Feb 2024

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NIST does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

A handwritten signature in cursive script that reads "Scott Als".

Certified by

Scott Als
Analytical Services Chemist

PC 17/02/2

HACH COMPANY



An ISO 9001 Certified Company

P.O.Box 389
Loveland, CO 80539
(970) 669-3050

Certificate of Analysis

This is a Component of 2659405-TH lot A2307

Page 1

COMMODITY: STABLCAL|sup|TS|sup0 FORMAZIN STANDARD 800 NTU
COMMODITY NUMBER: 2660501 MANUFACTURE DATE: DATE OF ANALYSIS:
LOT NUMBER: A2318 11/29/2022 12/5/2022

TEST	SPECIFICATIONS	RESULTS
Turbidity	760 to 840 NTU	817.0 NTU

The expiration date is Feb 2024

Formazin and StablCal® solutions provided by Hach are not NIST traceable because the NIST does not carry turbidity standards. However, the use of Formazin and StablCal® as used in Hach method 8195 are accepted by the EPA as a primary standard to be used in the calibration of turbidity instruments.

A handwritten signature in cursive script that reads "Scott Als".

Certified by

Scott Als
Analytical Services Chemist



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 16-Jul-2023

Certificate No. : 23TH3096

CSR No. : A095/04743

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory
Instrument Name : Incubator
Manufacturer : Memmert
Model : ICP750
Serial No. : F816.0063
ID No. : SGK_CL0028
Resolution : 0.1 °C
Received Date : 13-Jul-2023
Calibrated Date : 13-Jul-2023
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BYAnanta B.....
APPROVED BYKamtha H.....
NEXT CAL. DATE13/01/25.....

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- ScaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	23SDAT004	23-May-2024


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (☒) Without Adjustment (☐) After Adjustment

1. Sensor Installation Diagram

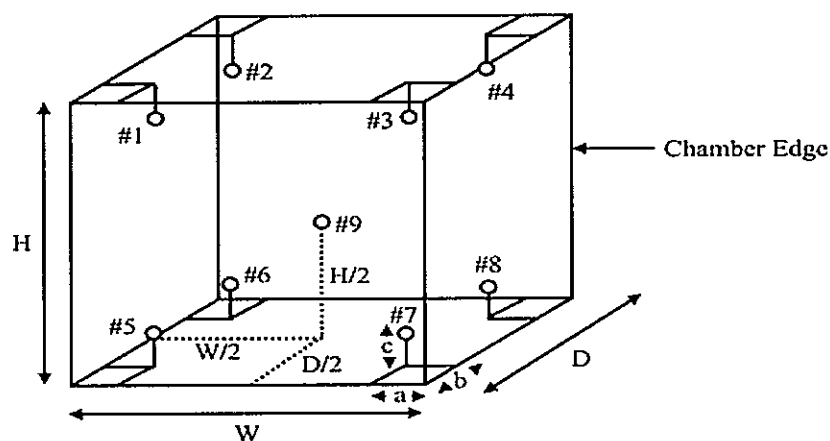

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 40.0 cm
H = 40.0 cm
D = 33.0 cm



Certificate No. : 23TH3096

CSR No. : A095/04743

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
20	20.10	20.04	20.03	19.97	20.08	20.23	20.10	19.94	20.07	0.38

3. Performance Result

The performance of the Incubator are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
20	20.0	20.0	0.14	0.17	0.32

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM162

Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000

Serial No. : 17B101473

ID No. : SGK_CL0073

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Songkhla Branch.
114/1 Moo 8, Kanjanavanij Rd., Banphru,

Location : TPA Chemistry Calibration Lab.2

Received Order : 18 November 2022

Calibrated Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Warakorn Lerngagtrakul

REVIEW BY	Ananta B.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	21 Nov 24.

Approved by :

Malu.

Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date :

22 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0047729



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2111-0663DSC-2

Cert. No.: 22LM162

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Digital Thermometer	1523	3240076	221249	02 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17B100103

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.001	19.88	-0.121	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Maku-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW259

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000
Serial No. :	17B101473
ID No. :	SGK_CL0073
Received Date :	18 November 2022
Test Date :	21 November 2022
Reference :	2211-0663DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8, Kanjanavanij Rd., Banphru, Hatyai, Songkhla 90250, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 Approved Signatory
☒ Malee Butkruea ☐ Saithip Meangmai ☐ Warakorn Lerngagtrakul	
Issue Date :	22 November 2022



Cert.No.: 22TW259

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.12	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu.

a 1136621

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com

**SARTORIUS**

Certificate

of Calibration

REVIEW BY Ananta B.
APPROVED BY Kanitta H.
NEXT CAL. DATE 25/1/23-24

Model Number : MSE224S-100-DUCertificate No. : 23BCI0044Description : Analytical BalanceIssued Date : Friday, January 27, 2023Serial Number : 0034705158Reference No. : 202361ID No. : SGK_CL0045Manufacturer : SartoriusPage No. : 1 of 2Customer Name : ALS Laboratory Group (Thailand) Co., Ltd.Songkhla Branch: 114/1 Moo 8 Karnchanawanich Rd., T. Ban Phru, A. Hat Yai, Songkhla. 90250.Calibrated Place : Balance Room.Calibrated By : Mr. Chonchai InthanaCalibration Date : Wednesday, January 25, 2023

Calibration

Procedure No. : This calibration was conducted byUsing in-house calibration procedure number (WI-003)Based on UKAS LAB 14 : 2019**Metrological data :**Capacity : 220 g Readability : 0.0001 g**Ambients Conditions:**Temperature : 22.4 °C ± 3.0 °CHumidity : 65.0 % RH ± 5.0 % RHPressure : ± **Reasons for calibration**☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ MaintenanceEquipment Condition: ☒ Good Operate ☐ Fair**Measurement Method UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 1kg E2 s/n 37929119	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

Mr. Chonchai Inthana (Technical Manager)

S
T
A
M
P

Certificate of Calibration

Model Number : MSE224S-100-DU

Certificate No. : 23BCI0044

Description : Analytical Balance

Issued Date : Friday, January 27, 2023

Serial Number : 0034705158

Reference No. : 202361

ID No. SGK_CL0045

Manufacturer : Sartorius

Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0001	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0000
	20.0000	200.0001
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0000	200.0001
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0001
	20.0000	200.0001
Standard Deviation	0.00003	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g
Tolerance 0.0004 g



	Difference
1	—
2	0.0001
3	0.0000
4	0.0000
5	0.0000
6	—

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00013
0.1	0.1000	0.1000	0.0000	0.00013
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	200.0001	0.0001	0.00030

End of Report.



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23TH1728

CSR No. : A088/04367

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Hot Air Oven

Manufacturer : Memmert

Model : UF110

Serial No. : B416.3387

ID No. : SGK_CL0024

Resolution : 0.1 °C

Received Date : 28-Apr-2023

Calibrated Date : 28-Apr-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	 Ananta B.
APPROVED BY	 Kanitta H. 10
NEXT CAL. DATE	 28/11/2024 10

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- ScaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

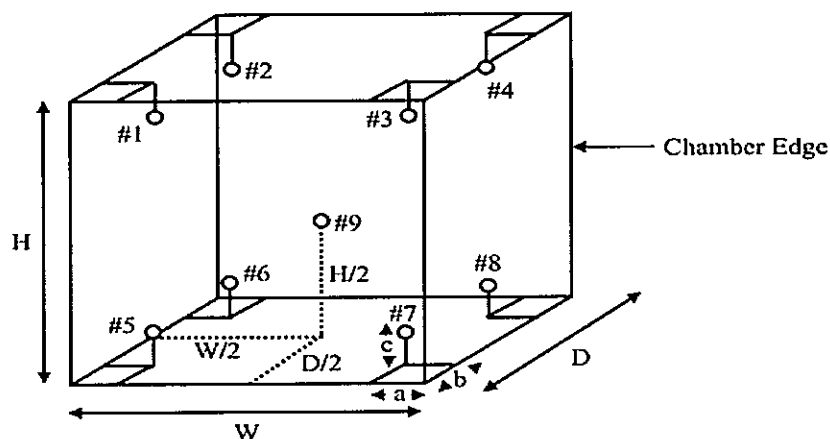

Sensor Installation Details

a = 5.0 cm

b = 5.0 cm

c = 5.0 cm

Dimension of the chamber

W = 40.0 cm

H = 40.0 cm

D = 33.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.48	40.28	40.28	39.91	40.17	40.09	39.93	40.27	39.89	0.36
70	70.36	70.23	70.58	69.74	69.99	69.92	69.86	70.13	70.04	0.36
103	103.19	103.12	103.46	103.37	103.10	103.54	103.43	103.06	103.40	0.36
104	104.31	104.23	104.62	103.77	104.12	104.06	103.90	104.20	104.56	0.36
105	105.07	105.03	105.48	105.27	105.12	105.01	105.01	105.00	104.96	0.36
180	180.31	180.00	180.00	180.07	180.18	180.05	180.01	180.10	180.24	0.41

3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
40	40.0	40.0	0.20	0.70	0.72
70	70.0	70.0	0.20	0.60	0.94
103	103.0	103.0	0.20	0.43	0.54
104	104.0	104.0	0.10	0.79	0.88
105	105.0	105.0	0.10	0.59	0.69
180	180.0	180.0	0.10	0.38	0.38

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 16-Jul-2023

Certificate No. : 23TH3097

CSR No. : A095/04743

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Water Bath

Manufacturer : Memmert

Model : WNE29

Serial No. : L616.0538

ID No. : SGK_CL0035

Resolution : 0.1 °C

Received Date : 13-Jul-2023

Calibrated Date : 13-Jul-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY Ananta B.

APPROVED BY Kanitha B.

NEXT CAL. DATE 13/01/25

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980
(reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017


Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement
according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

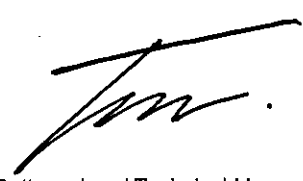
Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	23SDAT004	23-May-2024

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration .:

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

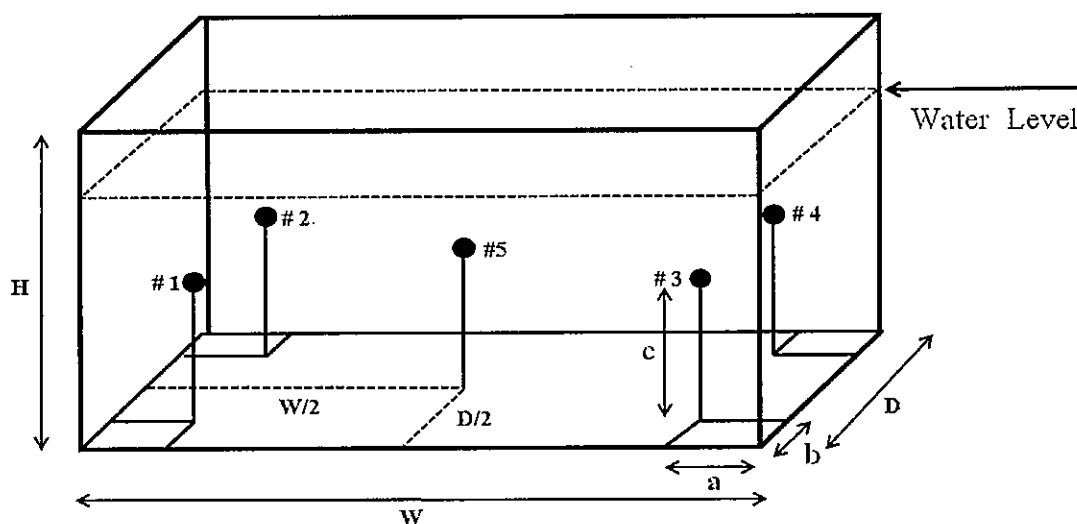

Sensor Installation Details

a = 5 cm
b = 5 cm
c = 5 cm

Dimension of the chamber

W = 45 cm
H = 30 cm
D = 35 cm



Certificate No. : 23TH3097

CSR No. : A095/04743

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
80	79.17	79.47	79.43	79.25	79.38	0.14

3. Performance Result

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
80	80.0	80.0	0.24	0.38	0.38

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 8-Jan-2023

Certificate No. : 23TH0050

CSR No. : A047/02339

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Autoclave

Manufacturer : TOMY

Model : SX-700

Serial No. : 52134079

ID No. : SGK_ML0001

Resolution : 1 °C

Received Date : 5-Jan-2023

Calibrated Date : 5-Jan-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	Nattawut P.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	Jul 05-May-2024
	Nattawut P.

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.16.013 based on BS 2646 : 1993 (part 5)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :


Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	GL220	C90432223	22SDAT005	4-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :.

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

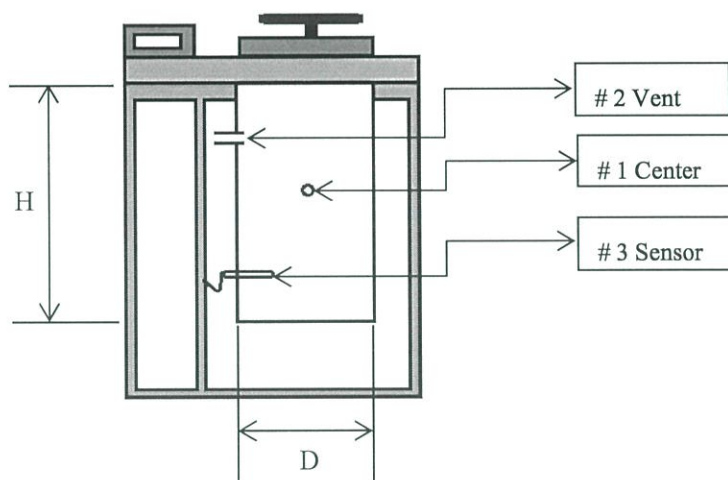

Chamber Diameter (D) : 30 cm

Chamber Height (H) : 70 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Autoclave and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)			Pressure Reading	Uncertainty (± °C)
	Center #1	Vent #2	Sensor #3		
115	115.5	115.4	115.5	0.07 MPa	0.76
118	118.7	118.9	119.1	0.09 MPa	0.76
121	122.0	122.1	122.1	0.11 MPa	0.76

3. Performance Result

The performance of the Autoclave are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
115	115	115	0.20	0.30	0.30
118	118	118	0.70	0.70	0.90
121	121	121	0.50	0.40	0.60

- Operating Time = 1800.65 sec

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 9-Aug-2022

Certificate No. : 22OV529

CSR No. : A037/01847

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Incubator

Manufacturer : Memmert

Model : ICP750

Serial No. : F816.0061

ID No. : SGK_ML0013

Resolution : 0.1 °C

Received Date : 6-Aug-2022

Calibrated Date : 6-Aug-2022

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	APPROVED BY
APPROVED BY	APPROVED BY
NEXT CAL. DATE	

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on G-20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCAL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

(☒) Without Adjustment

(☐) After Adjustment

1. Sensor Installation Diagram

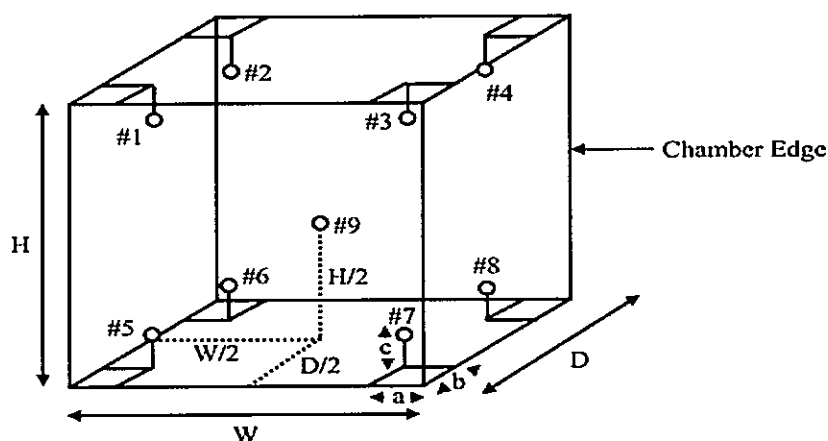

Sensor Installation Details

a = 5.0 cm

b = 5.0 cm

c = 5.0 cm

Dimension of the chamber

W = 104.0 cm

H = 120.0 cm

D = 60.0 cm



Certificate No. : 22OV529

CSR No. : A037/01847

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
35	34.99	34.92	34.95	34.88	34.96	35.00	34.94	34.94	34.94	0.38

3. Performance Result

The performance of the Incubator are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
35	35.0	35.0	0.10	0.12	0.19

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

CALIBRATION CERTIFICATE

Issued Date : 8-Jan-2023

Certificate No. : 23CH0016

CSR No. : A047/02339

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : pH meter

Manufacturer : Sartorius

Model : Basic pH Meter PB-10

Serial No. : C70160695

ID No. : SGK_ML0016

Electrode No. : N/A

Received Date : 5-Jan-2023

Calibrated Date : 5-Jan-2023

Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \%$

REVIEW BY	Nattawut P.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	05-Jul-24 Nattawut P.

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH
- WK : WK Electric Co., Ltd.

Calibrated by : Jessadagon Lemhud

Approved by :



Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02950	1733	22-Apr-2024
Standard Solution	7.000	C03001	1783	23-Sep-2024
Standard Solution	10.013	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading (mV)	Correction (mV)	Uncertainty (± mV)
177.48	177.4	0.08	0.17
0.00	0.0	0.00	0.13
-177.48	-177.4	-0.08	0.17

2. Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading (pH)	Correction (pH)	Uncertainty (± pH)
4.004	4.02	-0.016	0.011
7.000	7.01	-0.010	0.013
10.013	10.02	-0.007	0.036

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 2-Feb-2023

Certificate No. : 23TH0521

CSR No. : A075/03704

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Microbiological Laboratory

Instrument Name : Water Bath

Manufacturer : Memmert

Model : WPE45

Serial No. : L716.0558

ID No. : SGK_ML0021

Resolution : 0.1 °C

Received Date : 30-Jan-2023

Calibrated Date : 30-Jan-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY	Nattawut P.
APPROVED BY	Kanitta H.
NEXT CAL. DATE	30-Jul-24

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- ScaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration ∴

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

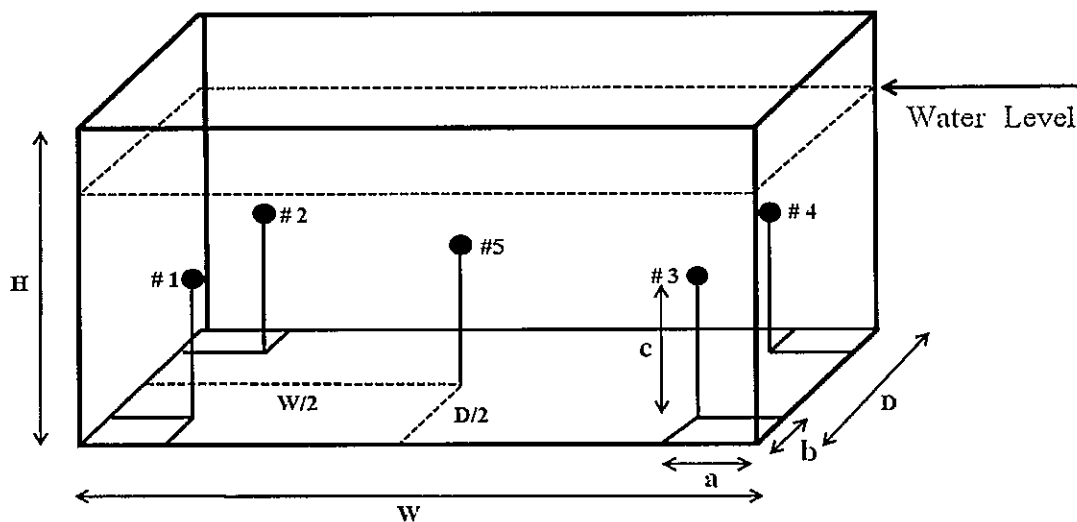

Sensor Installation Details

$a = 5 \text{ cm}$
 $b = 5 \text{ cm}$
 $c = 5 \text{ cm}$

Dimension of the chamber

$W = 45 \text{ cm}$
 $H = 30 \text{ cm}$
 $D = 35 \text{ cm}$



Certificate No. : 23TH0521

CSR No. : A075/03704

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
44.5	44.47	44.48	44.45	44.51	44.50	0.14

3. Performance Result

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
44.5	44.5	44.5	0.10	0.24	0.25

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...

Certificate Number CPH-0089-23

REVIEW BY	<u>Pittkanya Th</u>
APPROVED BY	<u>Sept S.</u>
NEXT CAL. DATE	<u>27 Jun 2024</u>

Calibration Certificate

Seven2Go™ pro Optical DO S9

Customer

Company	ALS Laboratory Group (Thailand) Co., Ltd.
Address	114/1 Moo.8, Karnchanawanich Rd., Thumbol Ban Phru, Amphur Hatyai
	Songkhla 90250
Customer ID number	301603330
Customer representative	-

Instrument

Type	Seven2Go S9	Instrument Serial Number	C316032694
Internal identification	-	Firmware version	1.02.01

Technical specifications

Measuring Range	0.00 ... 50.0 mg/L (ppm)	0.0 ... 500 %	
Resolution	0.01 mg/L	0.1 %	
Limit of Error	± 0.1 in range 0 ... 8 mg/L	± 10 %	
	± 0.2 in range 8 ... 20 mg/L		
	± 10 % in range 20 ... 50 mg/L		
Temperature range ATC	0 ... 50 °C	Pressure range	500 ... 1100 mbar
Resolution	0.1 °C	Resolution	1 mbar
Limit of Error	± 0.1 °C	Limit of Error	± 2 %

Procedure Statement

METTLER TOLEDO Seven2Go Service Manual Section B (Doc. No. 30232219) will be used as referring documentation to adjust and certify the instrument indicated in the "Type" and "Serial number" section. The measurement results of this certification were obtained at ambient conditions.

Certificate Number CPH-0089-23

Test Equipment

Digital Input tester Manufacturer METTLER TOLEDO
Type 51302672

Certified barometric pressure meter	Manufacturer	HUMLOG20 THIP
	Type	-

Serial number	170.0115.0802.028
Certificate number	22H1639
Date of Certification	August 3, 2022

Check of Digital Input

Digital sensor input	Sensor recognition	The sensor was recognized correctly by the meter	Passed
----------------------	--------------------	--	--------

Certification Measurements

Barometric pressure input	Designation	Measured value Certified meter	Measured value DO meter	Max. Tolerance	Passed / Failed
	Ambient pressure	1004.2 mbar	1005 mbar	2 %	Passed

Summary of Certification

Certification of instrument

Passed

The instrument referred to in this certificate has fulfilled the criteria of the certification. This is indicated by the notation Passed in the column above.

Remarks	Service Order : 0370243164
---------	----------------------------

Certification of the instrument was performed by

Name	Sookjai Sriwisait	Function	Service Technician
-------------	-------------------	-----------------	--------------------

Company METTLER TOLEDO

Date June 28, 2023 Signature

Performance Test

Attachment to Certificate No. CPH-0089-23

DO Sensor

Type: InLab OptiOx S/N: 999075

Measurement

Test	Measurement Probe	
	Before Adjustment	After Adjustment
Air	89.7%	100.0%
Pressure	1005 mbar	1005 mbar
Temperature	25.1 °C	25.1 °C

Remarks: N/A

Place: Chemical Laboratory Calibration Date: June 28, 2023

Service Specialist: Sookjai Sriwisait Signature: Sookjai S.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CG3154

Page.: 1 of 2

Certificate of Calibration

Equipment :

Burette

Capacity :

50 mL

Serial No. :

-

ID. No. :

BKK_EN0171

Manufacturer :

Witeg

Made in :

Germany

Submitted by :

ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.
Khwaeng Phatthanakan, Khet Suan Luang
Bangkok 10250 Thailand

Ambient Temperature :

(20 $\pm$ 2.5) °C

Relative Humidity :

(50 $\pm$ 10) %

Barometric Pressure :

759 mmHg

Calibration Procedure :

ASTM E 542 - 01

Calibrated by :

Panward Pramklam

Approved by :

Approved Signatory

() Pornthippa Tameyakul

() Malee Butkruea

(☒) Ponpan Paipim

() Srisuda Khamtha

Issue Date :

31 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0044607



Equipment : Burette
Received Date : 26 August 2022
Condition As-Received : Used Item
Calibration Date : 30 August 2022
Reference : 2208-0918DSC-2

Cert.No.: 22CG3154

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	AE200S	N03679	140RC001	21MM429	NIMT	22 Sep 2022
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	22H1243	NIST,NIMT	09 June 2023
3) Thermometer	-	1594592	140EC010	22I181	NIMT	10 Feb 2023

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
50	49.9959	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

a 1123908

REVIEW BY Aulcharawan S.APPROVED BY Sararat M.NEXT CAL. DATE 12 Jan 24

Certificate of Calibration

ICS-2100: Anion (ID#659)

This certificate is to verify that instrument below are calibrated


by Archemica Lab Co., Ltd.

ICS-2100 S/N: 15010977

AS-HV S/N: 5450A36659

For

ALS Laboratory Group (Thailand) Co., Ltd.



Operator Signature: Nutdanai

Date: Jan 12, 2023

(Mr.Nutdanai Laekhwan)

Application Chemist



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1103

Page : 1 of 3

Certificate of Calibration

Equipment : Autoclave
Manufacturer : Sanyo
Model : MLS-3781
Serial No. : 830167
ID No. : BKK_ML0037
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : Media Preparation Room
Received Order : 17 July 2023
Calibration Date : 17 July 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Preecha Hlahib

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
() Malee Butkruea
(✓) Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0053615



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2307-0285OC-3

Cert. No.: 23TM1103

Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)


It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

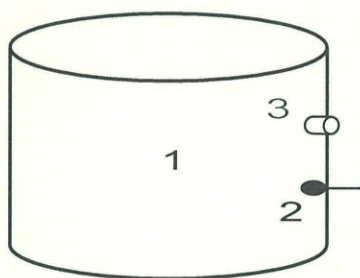

	<u>Environmental</u>		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	22	53	220
Finished of Calibration	22	54	220

<u>Position</u>	<u>Description</u>	<u>Ref. Std. ID No.:</u>
1 =	Center of chamber	22-17TC-01
2 =	Temperature sensor	23-17TC-02
3 =	Exhaust port	19-17TC-03

Handwritten signature



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2307-0285OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM1103

Page : 3 of 3

Operating parameter Set : Temperature = 121 °C

Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
121	121	1	120.877	0.39	0.12	1.0	2
		2	120.870				
		3	120.866				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Yunit



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1570

Page : 1 of 3

Certificate of Calibration

Equipment : CO2 Incubator

Manufacturer : ShelLab

Model : TC 2123 2E

Serial No. : 0701199

ID No. : BKK_ML0012

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Presumptive Testing Lab

Received Order : 21 November 2022

Calibration Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

REVIEW BY	Sithichok
APPROVED BY	[Signature]
NEXT CAL. DATE	21/05/24

Approved by :

Malee

Approved Signatory

- () Pornthippa Tameyakul
(✓) Malee Butkruea
() Suwit Imjai

Issue Date :

29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0048154



Equipment : CO2 Incubator
 Condition As-Received : Used Item
 Reference : 2211-0623OC-5

Cert. No.: 22TM1570

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Result of Calibration :- (*) After Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration

	Beginning	Finished
Temp. (°C)	25	26
REL.Humid. (%)	52	50
AC Supply (Volt)	221	220

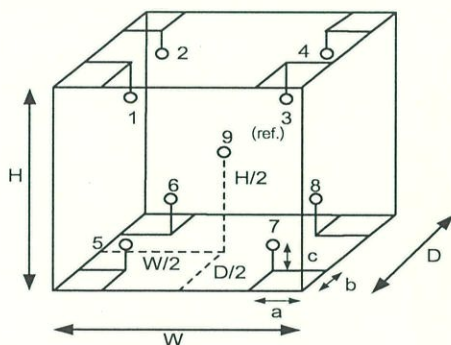

Position :	Ref. Std. ID No.:
1	19-15RTD-01
2	19-15RTD-02
3	19-15RTD-03
4	19-15RTD-04
5	19-15RTD-05
6	21-15RTD-06
7	19-15RTD-07
8	19-15RTD-08
9 (ref.)	19-15RTD-09

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.40 m
 W = 0.40 m
 H = 0.35 m
 Capacity = 0.056 m³

Malu



Equipment : CO2 Incubator
Condition As-Received : Used Item
Reference : 2211-0623OC-5
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1570

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
44.0	44.0	44.0	0.076	0.25	0.30	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
44.0	43.968	44.086	44.090	44.063	43.951	43.897	44.011	43.983	44.133

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu .



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1571

Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Binder

Model : ED 240/E2

Serial No. : 00-15533

ID No. : BKK_ML0013

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 21 November 2022

Calibration Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by :

Malee

Approved Signatory

() Pornthippa Tameyakul

(✓) Malee Butkruea

() Suwit Imjai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0048150



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2211-0623OC-1

Cert. No.: 22TM1571

Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) After Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

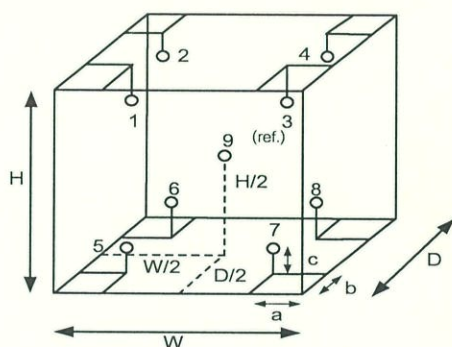

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	53	55
AC Supply (Volt)	219	220

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

Probe Installation Details :

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
 W = 0.80 m
 H = 0.60 m
 Capacity = 0.24 m³

Malu.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1571

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 1 of 5

Certificate of Calibration

Equipment : Digestion Unit

Manufacturer : SCP Science

Model : DigiPRER HT

Serial No. : HTC1120480658

Customer Code : BKK_EN0366

ID No. : T2635A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250


Customer Location : Wet Chemistry Lab 1

Date of Receipt : 10 May 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 29 MAY 2023

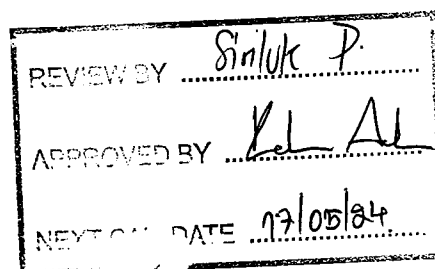

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 2 of 5

Calibration Report

Equipment : Digestion Unit
Date of Calibration : 17 May 2023
Environment : Temperature : 23.9 - 26.3 °C
Line Voltage : 221.8 - 225.9 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A1-(CH17-CH20)	T230547	18 April 2024
DATA LOGGER	34970A	T149	T230547	18 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 54 Minute At 380 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By. 

Certificate No. T230902

Page 3 of 5

Calibration Report

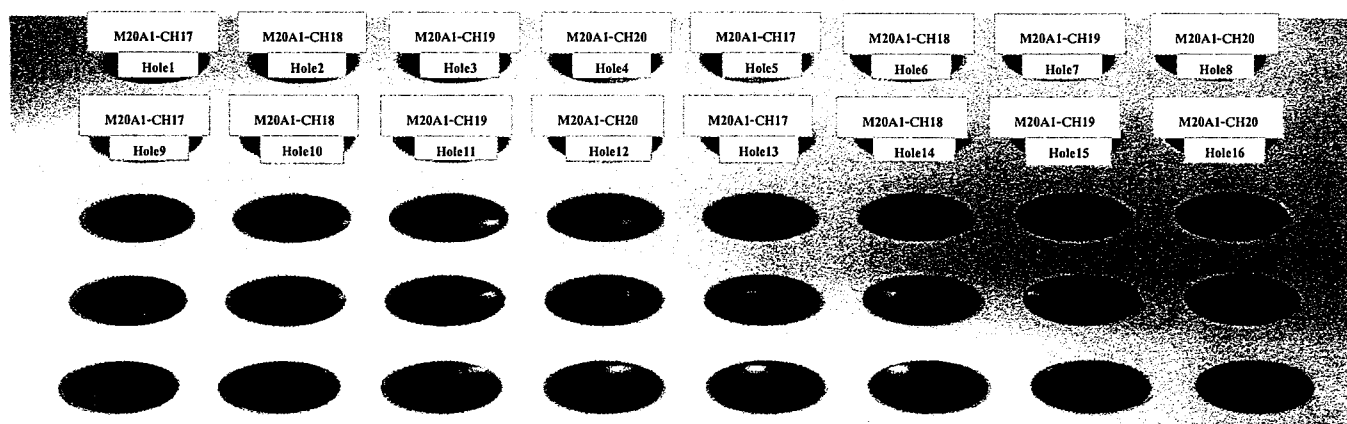


FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.3	379.0	379.2	380.2	377.5	379.5	380.7	380.1
			Min °C	376.8	378.6	378.9	379.9	377.0	379.0	380.2	379.6
			Average °C	377.0	378.8	379.1	380.0	377.3	379.2	380.4	379.9
			Stability ± °C	0.2	0.2	0.2	0.2	0.3	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole9	Hole10	Hole11	Hole12	Hole13	Hole14	Hole15	Hole16
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.1	378.9	379.7	379.9	379.3	379.6	379.5	377.4
			Min °C	376.7	378.5	379.3	379.5	378.9	379.1	379.0	377.0
			Average °C	376.9	378.7	379.5	379.7	379.1	379.4	379.3	377.2
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.3	0.3	0.2


Approved By.



Certificate No. T230902

Page 4 of 5

Calibration Report

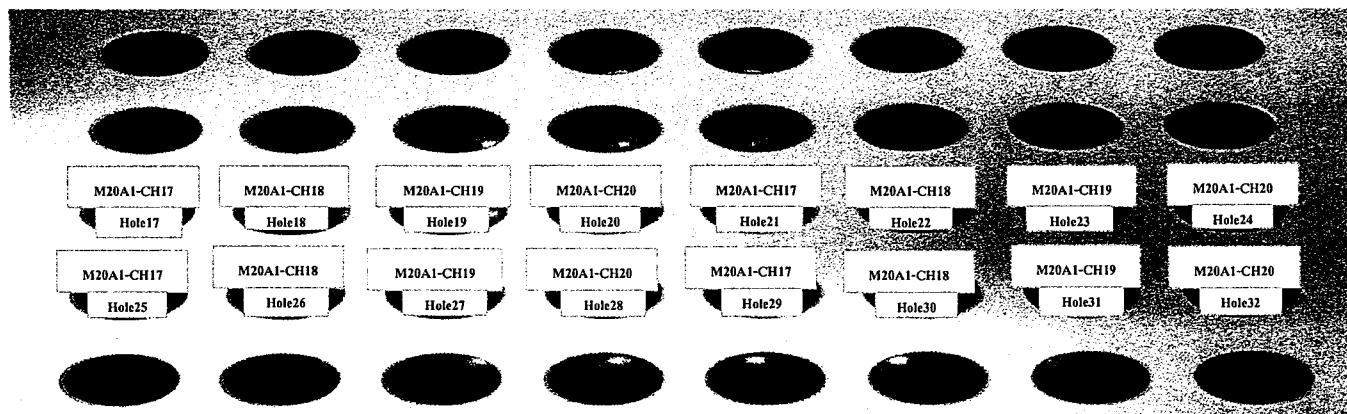


FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole17	Hole18	Hole19	Hole20	Hole21	Hole22	Hole23	Hole24
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.4	380.1	380.1	380.0	379.1	379.8	379.6	377.8
			Min °C	377.8	379.6	379.7	379.3	378.6	379.2	379.2	377.3
			Average °C	378.1	379.9	379.9	379.7	378.9	379.5	379.4	377.5
			Stability ± °C	0.3	0.3	0.2	0.3	0.3	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole25	Hole26	Hole27	Hole28	Hole29	Hole30	Hole31	Hole32
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.9	379.4	380.1	380.1	379.3	379.6	378.9	377.3
			Min °C	377.4	378.9	379.7	379.7	378.8	378.9	378.4	376.7
			Average °C	377.7	379.2	379.9	379.9	379.0	379.3	378.6	377.0
			Stability ± °C	0.3	0.3	0.2	0.2	0.3	0.4	0.3	0.3


Approved By.



Certificate No. T230902

Page 5 of 5

Calibration Report

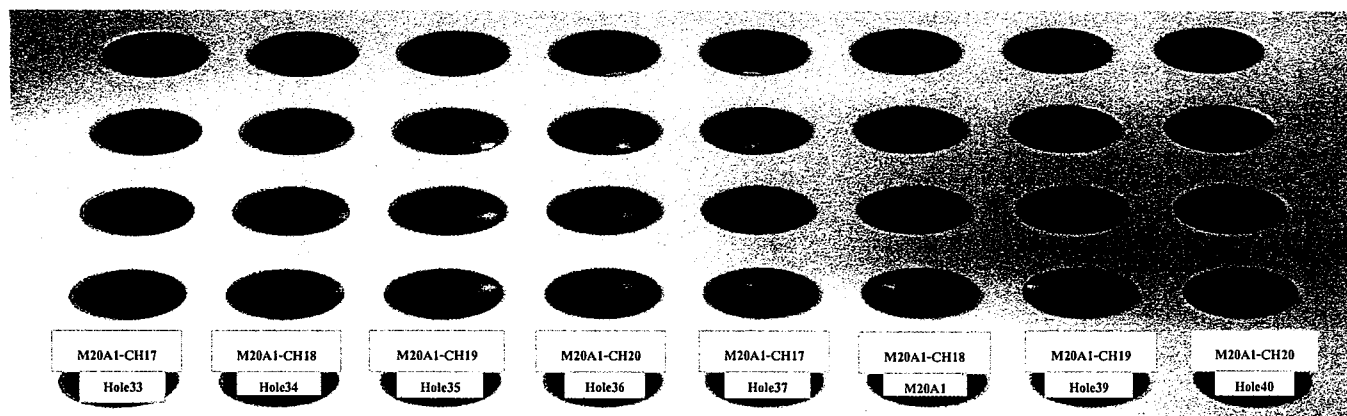

FRONT

Measurement Results


Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole33	Hole34	Hole35	Hole36	Hole37	Hole38	Hole39	Hole40
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.7	378.0	378.3	379.0	378.2	378.5	377.3	377.4
			Min °C	377.3	377.6	377.9	378.6	377.7	378.1	376.9	377.0
			Average °C	377.5	377.8	378.1	378.8	378.0	378.3	377.1	377.2
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.2	0.2	0.2

 The expanded uncertainty of temperature measurement was ± 1.85 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

 The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %.

 Approved By. 



บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.

4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพมหานคร 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รวม							12/7 ck					

Periodical maintenance check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	☐	☒	
2.ISE tubing change	☒	☒	none
3.Syringe check/change		☒	
4.Dispensing check/ change		☒	
5.Waste tubing change when necessary		☒	
6.Lamp check/change	☐	☒	
7.Mixer paddle/paddle change(not Konelab20)		☒	
8.ISE needles check/change		☒	none
9.Pump tubing check/ chance	☐	☒	
10.Broken/worn out part check /change		☒	
11.Peristaltic pump check /cleaning/ lubrication	☐	☒	
12.Heating check		☒	
13.Cooling check		☒	
14.Dispenser mechanic check/adjustment	☐	☒	
15.Cuvette transfer mechanic check/adjustment	☐	☒	
16.Dispenser movement check/adjustment	☐	☒	
17.Sample/reagent register check/adjustment	☐	☒	
18.Dispensing tubing tightness check	☐	☒	
19.Photometer and optics cleaning/check/adjustment	☐	☒	
20.Workstation PC cleaning if necessary	☐	☒	
21.Mechanic cleaning/lubrication	☐	☒	
22.Instrument cleaning if necessary	☐	☒	
23.Complete analyzer testing with waterblank/QC or sample	☐	☒	
24.Test parameters/Adjustment/config. Save to USB key	☐	☒	
25.UPS Test	☐	☒	

Place: ALS LAB Instrument: k90 Aquakem
Date/Time: 12/7/66 Serial no: 22781
Service done by: ๑๗๖๕ Install date:
Signature of customer: ๑๗๖๕ Date/Time: 12/7/66

Laboratory
Analyzer User

7/12/2023 21:21

Performed	7/12/2023
Lot	W166

=====

ACCEPTANCE CRITERIA

=====

	Result	Limit	Warning
Temperature (?C)	37.7	37.0 +/- 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	1.17	<1.7	
Photometric noise			
Max SD L340_2 (mA)	0.19	<2.0	
Max SD L340_4 (mA)	1.06	<3.0	
Linearity of photometer			
Slope	1.0188	0.94 - 1.06	
Curvature	0.0035	+/- 0.02	
Max bias from linear fit (mA)	3.2	<15.0	
Max delta %	-2.0	+/- 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (?l)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (?l)	4.13	3.85 - 4.40	
XDISP2 CV%	0.58	<2.0	
XDISP4 CV%	0.70	<2.0	
XDISP10 CV%	0.59	<2.0	
Needle 0 ?l volume			
Average (A)	0.009	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (?l)	0.06	<0.32	

=====

OTHER INFORMATION

=====

Dispensing ratio		Photom., noise: SD (mA)	
Posit	Result (A)	Posit	L340_2 L340_4
1	0.1592	1	0.07 0.64
2	0.1624	2	0.09 1.06
3	0.1631	3	0.14 0.50
4	0.1631	4	0.13 0.53
5	0.1625	5	0.19 0.38
6	0.1650	6	0.02 0.64

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.311
XDISP4	0.616
XDISP10	1.478

Linearity of photometer

L340_	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.001	0.005	-0.004	-394.7
2	0.512	0.519	-0.007	-1.5
3	1.523	1.550	-0.027	-1.8
4	2.027	2.066	-0.039	-1.9
5	2.532	2.582	-0.050	-2.0

