

ภาคผนวก จ

เอกสารการสอบเทียบเครื่องมือตรวจวิเคราะห์



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	pH at 25 °C	pH meter	BKK_EN0072	12-Sep-22	12-Mar-24	18
Water Lab	Sulfide	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Sulfide	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0148	4-Jul-23	4-Jan-25	18
Water Lab	BOD	DO Meter	BKK_EN0205	3-Aug-22	3-Feb-24	18
Water Lab	BOD	Incubator	BKK_EN0304	5-Apr-23	5-Apr-24	12
Water Lab	Settleable Solids	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0366	17-May-23	17-May-24	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	12-Jul-23	12-Jul-24	12
Water Lab	Total Dissolved Solids 103-105°C	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Dissolved Solids 103-105°C	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0002	8-Feb-23	8-Feb-24	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0273	29-Nov-22	29-May-24	18
Water Lab	Fecal Coliform	Autoclave	BKK_ML0043	10-Apr-23	10-Oct-24	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	20-Apr-23	20-Apr-24	12
Water Lab	Total Coliform	Autoclave	BKK_ML0043	10-Apr-23	10-Oct-24	18
Water Lab	Total Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Residual Free Chlorine	Chlorine Meter	BKK_LG0032	28-Feb-23	28-Feb-24	12
Water Lab	Residual Chlorine	Chlorine Meter	BKK_LG0032	28-Feb-23	28-Feb-24	12
Water Lab	Ammonia Nitrogen	Discrete analyzer	BKK_EN0037	5-Jan-23	5-Jan-24	12
Water Lab	Total Alkalinity	Burette	BKK_EN0171	30-Aug-22	1-Mar-24	18
Water Lab	Calcium Hardness	Burette	BKK_EN0296	24-Dec-21	24-Jun-23	18
Water Lab	Nitrate	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	Chloride	Ion Chromatography	BKK_EN0069	12-Jan-23	12-Jan-24	12
Water Lab	Cyanuric acid	Spectrophotometer	SGK_CL0038	24-Jan-23	24-Jan-24	12
Water Lab	<i>Staphylococcus aureus</i>	Autoclave	BKK_ML0041	20-May-22	20-Nov-23	18
Water Lab	<i>Staphylococcus aureus</i>	Incubator	BKK_ML0010	21-Jan-22	22-Jul-23	18
Water Lab	<i>Staphylococcus aureus</i>	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	<i>Pseudomonas aeruginosa</i>	Autoclave	BKK_ML0041	20-May-22	20-Nov-23	18
Water Lab	<i>Pseudomonas aeruginosa</i>	Incubator	BKK_ML0010	21-Jan-22	22-Jul-23	18
Water Lab	<i>Pseudomonas aeruginosa</i>	Water Bath	BKK_ML0049	19-Jan-23	19-Jan-24	12
Water Lab	<i>Pseudomonas aeruginosa</i>	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	Color	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	Turbidity	Chamber (Cold Room)	BKK_EN0167	30-Jun-22	30-Dec-23	18
Water Lab	<i>Escherichia coli</i>	Autoclave	BKK_ML0043	10-Apr-23	10-Oct-24	18
Water Lab	<i>Escherichia coli</i>	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	<i>Escherichia coli</i>	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	<i>Escherichia coli</i>	Water Bath	BKK_ML0056	20-Apr-23	20-Apr-24	12



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CH1222
Page.: 1 of 2

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Mettler Toledo
Model : Seven Compact S220
Serial No. : B520948426
ID No. : BKK_EN0072
Condition As-Received: Used Item
Received Date : 09 September 2022
Calibration Date : 12 September 2022
Reference : 2209-0312DSC-1
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement
with certified reference material (CRM)

Calibrated by : Warakorn Lerngagtrakul

Approved by :

(✓) Malee Butkruea
() Saithip Meangmai
() Warakorn Lerngagtrakul

Issue Date : 15 September 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No.: 22CH1222
Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument : -

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	823320	20 June 2024
pH 6.985	CPA chem	794122	14 Feb 2023
pH 10.008	CPA chem	823323	20 June 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter	4.000	177.48	177.4	4.000	0.058	2.00
S/N.: B520948426	7.000	0.00	0.0	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor k
pH Electrode S/N.:PCE-86-EX1001	4.008	3.999	153.9	0.0055	2.09
	6.985	7.017	-13.7	0.0084	2.00
	10.008	9.996	-179.0	0.0078	2.06

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-oOo-

Malee

a 1126274



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CG3154
Page.: 1 of 2

Certificate of Calibration

Equipment : Burette
Capacity : 50 mL
Serial No. : -
ID. No. : BKK_EN0171

Manufacturer : Witeg
Made in : Germany

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.
Khwaeng Phatthanakan, Khet Suan Luang
Bangkok 10250 Thailand

Ambient Temperature : (20 ± 2.5) °C
Relative Humidity : (50 ± 10) %
Barometric Pressure : 759 mmHg
Calibration Procedure : ASTM E 542 - 01

Calibrated by : Panward Pramklam

Approved by :

- () Pornthippa Tameyakul
() Malee Butkruea
(X) Ponpan Paipim
() Srisuda Khamtha

Issue Date : 31 August 2022

REVIEW BY	Sinluk P.
APPROVED BY	KLAL
NEXT CAL. DATE	29/03/2024



Equipment : Burette
Received Date : 26 August 2022
Condition As-Received : Used Item
Calibration Date : 30 August 2022
Reference : 2208-0918DSC-2

Cert.No.: 22CG3154
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	AE200S	N03679	140RC001	21MM429	NIMT	22 Sep 2022
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	22H1243	NIST,NIMT	09 June 2023
3) Thermometer	-	1594592	140EC010	22I181	NIMT	10 Feb 2023

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
50	49.9959	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th



NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T221644

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cold Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.


104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250



Customer Location : Environmental Laboratory

Date of Receipt : 27 June 2022

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 04 JUL 2022

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	30/12/23



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T221644

Page 2 of 4

Calibration Report

Equipment : Chamber (Cold Room)

Date of Calibration : 30 June - 1 July 2022

Environment : Temperature : 18.9-23.7 °C

Line Voltage : 222.9-226.5 V

Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T210009	30 July 2022
TC	TYPE T	TN171-TN180	T210009	30 July 2022
DATA LOGGER	34970A	T149	T210009	30 July 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour - Minute At 3 °C

Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max

☐ Close

☒ Not Available

5. Adjustment :

() without adjustment

(X) after adjustment

Approved By: 


The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T221644

Page 3 of 4

Calibration Report

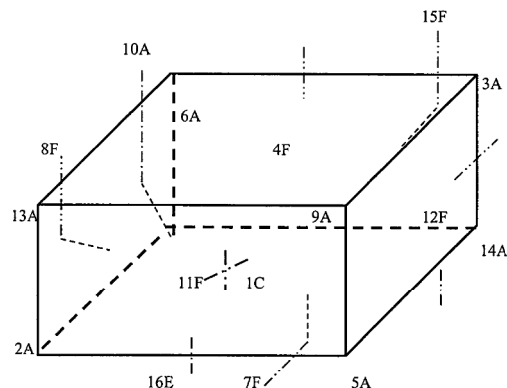

C = Centre, F = Centre of Face, A = Corner, E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN171
12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175
16E	=	TN176

Approved By. _____



Certificate No. T221644

Page 4 of 4

Calibration Report

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)									
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	2.71	2.82	2.75	2.89	2.95	3.68	3.02	2.96	3.03	2.85
	TN171	TN172	TN173	TN174	TN175	TN176				
	2.97	3.02	2.89	3.04	2.97	3.33				

Chamber (Cold Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average					
3.0	2.9 , 4.0	3.2	2.99	1.05	1.30	1.66	2.00

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____





SARTORIUS

Certificate of Calibration

REVIEW BY Sirint P.
APPROVED BY LL AL
NEXT CAL. DATE 8/2/24

Model Number : MSE224S-100-DU Certificate No. : 23BCI0072
Description : Analytical Balance Issued Date : Monday, February 13, 2023
Serial Number : 26207042 Reference No. : 203245
ID No. : BKK_EN0002
Manufacturer : Sartorius Page No. : 1 of 2

Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.
104 Phatthanakan 40,Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.

Calibrated Place : Balance Room

Calibrated By : Mr. Chonchai Inthana
Calibration Date : Wednesday, February 08, 2023
Calibration Procedure No. : This calibration was conducted by Using in-house calibration procedure number (WI-003) Based on UKAS LAB 14 : 2019

Metrological data :
Capacity : 220 g Readability : 0.0001 g
Reasons for calibration
☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance
Ambients Conditions:
Temperature : 23.2 °C ± 5.0 °C
Humidity : 60.0 % RH ± 10.0 % RH
Pressure : ±
Equipment Condition: ☒ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Chonchai Inthana

Mr.Chonchai Inthana(Technical Manager)




SARTORIUS

Certificate of Calibration

Model Number : MSE224S-100-DU Certificate No. : 23BCI0072
Description : Analytical Balance Issued Date : Monday, February 13, 2023
Serial Number : 26207042 Reference No. : 203245
ID No. : BKK_EN0002
Manufacturer : Sartorius Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability		
The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.		
Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	199.9999
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0001	200.0000
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0000	199.9999
Tolerance	20.0000	199.9999
0.0001 g	20.0000	200.0000
	20.0001	199.9999
Standard Deviation		0.00004 0.00005

Eccentricity (Off-center loading error)			
The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).			
Nominal value :	50	g	
Tolerance	0.0004	g	
		Difference	
		1	—
		2	-0.0001
		3	0.0000
		4	0.0001
		5	0.0000
		6	—

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value	Conventional Mass Value	Displayed Value	Deviation	Uncertainty
(g)	(g)	(g)	(g)	(g)
0.01	0.0100	0.0100	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	199.9999	-0.0001	0.00030

End of Report.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T231303

Page 1 of 3

Certificate of Calibration

Equipment : Liquid Bath (Water)

Manufacturer : MEMMERT

Model : WNB29

Serial No. : L611.0135

Customer Code : BKK_EN0148

ID No. : T6455A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250


Customer Location : ORGANIC PREPARATION LAB

Date of Receipt : 27 June 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By : Bm Lm / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 11 JUL 2023



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L14118/31-08-64



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



Certificate No. T231303

Page 2 of 3

Calibration Report

Equipment : Liquid Bath (Water)

Date of Calibration : 4 July 2023

Environment : Temperature : 22.2-22.5 °C

Line Voltage : 221.6-224.8 V

Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to W1-T36 (based on ASTM E715-80 (Reapproved 2001)).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1,CH6-CH7,CH9-CH10)	T230545	10 April 2024
DATA LOGGER	34970A	T149	T230545	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour 45 Minute At 60 °C

5. Adjustment :

(X) without adjustment

() after adjustment

Approved By : Bm Lm

FM-L15 117/15-05-63



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.




NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T231303

Page 3 of 3

Calibration Report

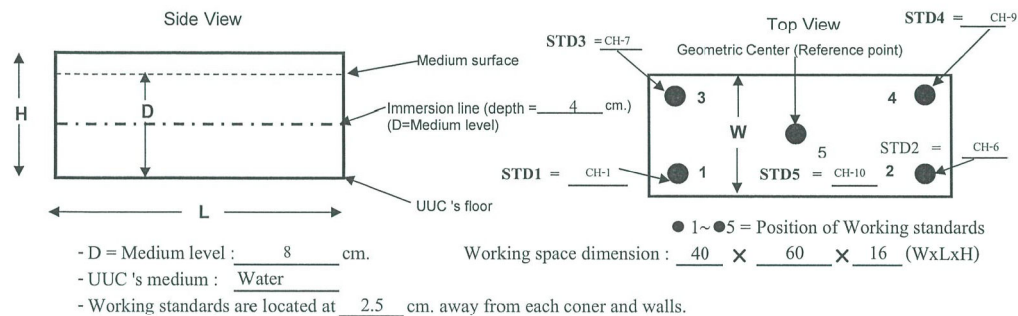

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	CH-1	CH-6	CH-7	CH-9	CH-10
60	60.03	60.06	60.24	60.11	60.18
85	84.79	84.83	85.42	85.05	85.20
95	93.71	93.83	94.62	94.15	94.42

Liquid Bath (Water)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (± °C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
61.0	60.9 , 61.1	61.0	60.12	0.13	0.19	0.29	2.04
86.0	85.8 , 86.2	86.0	85.06	0.19	0.47	0.44	2.17
95.0	94.6 , 95	94.9	94.15	0.32	0.65	0.55	2.13

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. Sam Lina



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW178

Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter

Manufacturer : YSI

Model : 5100

Serial No. : 15L103204

ID No. : BKK_EN0205

Received Date : 02 August 2022

Test Date : 03 August 2022

Reference : 2208-0060DSC-1

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %

Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by : Malee Butkruea
Approved Signatory

(✓) Malee Butkruea
() Saithip Meangmai
() Warakorn Lernagatrakul

Issue Date : 4 August 2022

REVIEW BY	<u>Siriruk P.</u>
APPROVED BY	<u>Malee Butkruea</u>
NEXT CAL. DATE	<u>03/02/24</u>



Cert.No.: 22TW178
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	21MM430	21 Sep 2022

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 17A100064

Titration Method (Azide Modification Method)	DO Meter Reading	Standard Deviation
(mg/L)	(mg/L)	(mg/L)
8.06	8.07	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency. The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory.

-o0o-

Malee

a 1119718



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22LM107
Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor
Manufacturer : YSI
Model : 5100
Serial No. : 15L103204
ID No. : BKK_EN0205
Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : TPA On Site Calibration Laboratory
Received Order : 2 August 2022
Calibrated Date : 4 August 2022
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Man Pattanapongpaiboon
Approved by : *Malee*
Approved Signatory
() Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai
Issue Date : 9 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0044131



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2208-0060DSC-2
Procedure Used :-

Cert. No.: 22LM107
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Digital Thermometer	1502A	A52847	2111144	20 Oct 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 18C100772

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
20.00	60	20.002	19.93	-0.072	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malu.

a 1120698



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.com



Certificate No. T230682

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Incubator)

Manufacturer : MEMMERT

Model : ICP 750

Serial No. : F819.0021

Customer Code : BKK_EN0304

ID No. : T9572A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250


Customer Location : Wet Chemistry Lab 2

Date of Receipt : 30 March 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By : Boonchai Suriyawong / Boonchai Suriyawong (Assistant Calibration Manager)

Date of Issue : 10 APR 2023



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L14118/31-08-64



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T230682

Calibration Report

Page 2 of 4

Equipment : Chamber (Incubator)
Date of Calibration : 5 April 2023 (Finished Time 4:30 PM)
Environment : Temperature 22.9-28.6 °C
Line Voltage 221.7-225.5 V

Condition of this results of test. :

1. This instrument was calibrated by insert 12 standard resistance thermometer into its chamber and test according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986.)

All data show below were final values and the initial data may be obtained upon request.

The temperature scale used was based on ITS - 90.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	37-(CH1-10)	T222493	28 November 2023
RTD	100 ohm	36-(CH1-10)	T222493	28 November 2023
DATA LOGGER	34970A	T193	T222493	28 November 2023

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

UUC Description :

Time Constant 1 Hour 37 Minute At 20 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Result of test :

() without adjustment (X) after adjustment

Approved By



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.




NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No T230682

Calibration Report

Page 3 of 4

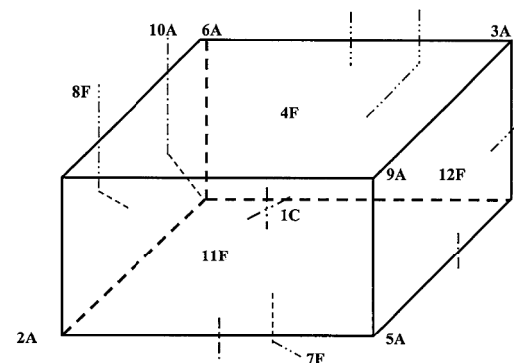

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	37CH1
2A	=	37CH2
3A	=	37CH3
4F	=	37CH4
5A	=	37CH5
6A	=	37CH6
7F	=	37CH7
8F	=	37CH8
9A	=	37CH9
10A	=	37CH10

11F	=	36CH1
12F	=	36CH2

Approved By



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T230682

Calibration Report

Page 4 of 4

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)									
	37CH1	37CH2	37CH3	37CH4	37CH5	37CH6	37CH7	37CH8	37CH9	37CH10
20.0	20.26	20.17	20.10	20.15	20.12	19.96	20.14	19.69	20.20	19.82
	36CH1	36CH2								
	20.03	20.04								

Chamber (Incubator)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
20.0	19.9 , 20.1	20.0	19.98	0.19	0.53	0.38	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By 



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 1 of 5

Certificate of Calibration

Equipment : Digestion Unit

Manufacturer : SCP Science

Model : DigiPRER HT

Serial No. : HTC1120480658

Customer Code : BKK_EN0366

ID No. : T2635A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.


104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 1

Date of Receipt : 10 May 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 29 MAY 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 2 of 5

Calibration Report

Equipment : Digestion Unit
Date of Calibration : 17 May 2023
Environment : Temperature : 23.9 - 26.3 °C
Line Voltage : 221.8 - 225.9 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A1-(CH17-CH20)	T230547	18 April 2024
DATA LOGGER	34970A	T149	T230547	18 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 54 Minute At 380 °C

Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☒ Max

☐ Close

☒ Not Available

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By

Certificate No. T230902

Page 3 of 5

Calibration Report

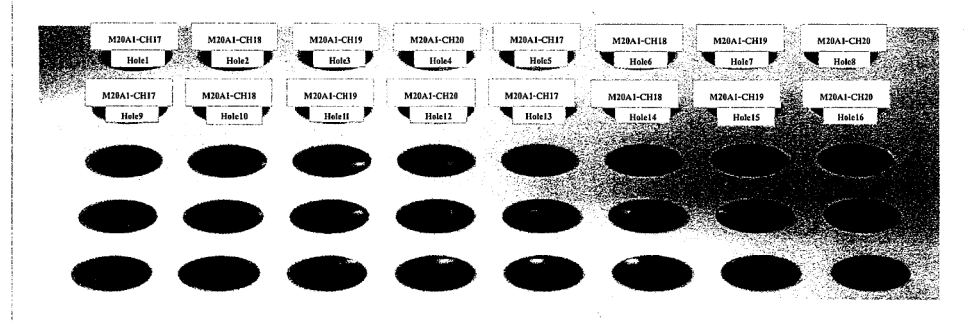

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
				Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8
380.0	380.0	379.4 - 380.7	Reading	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
			Max °C	377.3	379.0	379.2	380.2	377.5	379.5	380.7	380.1
			Min °C	376.8	378.6	378.9	379.9	377.0	379.0	380.2	379.6
			Average °C	377.0	378.8	379.1	380.0	377.3	379.2	380.4	379.9
			Stability ± °C	0.2	0.2	0.2	0.2	0.3	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
				Hole9	Hole10	Hole11	Hole12	Hole13	Hole14	Hole15	Hole16
380.0	380.0	379.4 - 380.7	Reading	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
			Max °C	377.1	378.9	379.7	379.9	379.3	379.6	379.5	377.4
			Min °C	376.7	378.5	379.3	379.5	378.9	379.1	379.0	377.0
			Average °C	376.9	378.7	379.5	379.7	379.1	379.4	379.3	377.2
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.3	0.3	0.2

Approved By



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110


Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Page 4 of 5

Calibration Report

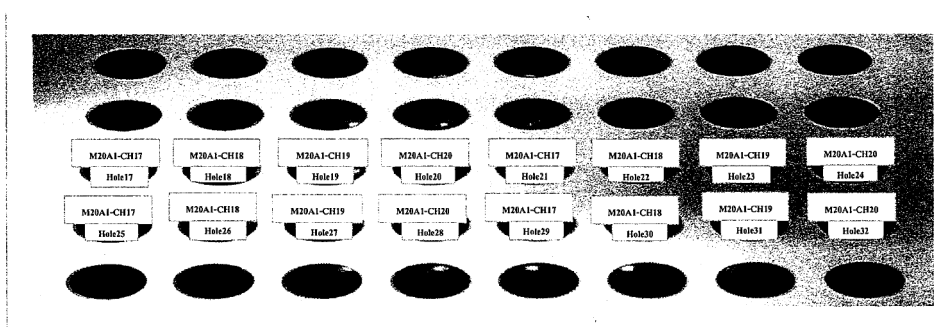

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole17	Hole18	Hole19	Hole20	Hole21	Hole22	Hole23	Hole24
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	378.4	380.1	380.1	380.0	379.1	379.8	379.6	377.8
			Min °C	377.8	379.6	379.7	379.3	378.6	379.2	379.2	377.3
			Average °C	378.1	379.9	379.9	379.7	378.9	379.5	379.4	377.5
			Stability ± °C	0.3	0.3	0.2	0.3	0.3	0.3	0.2	0.2


Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole25	Hole26	Hole27	Hole28	Hole29	Hole30	Hole31	Hole32
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.9	379.4	380.1	380.1	379.3	379.6	378.9	377.3
			Min °C	377.4	378.9	379.7	379.7	378.8	378.9	378.4	376.7
			Average °C	377.7	379.2	379.9	379.9	379.0	379.3	378.6	377.0
			Stability ± °C	0.3	0.3	0.2	0.2	0.3	0.4	0.3	0.3

Approved By

Certificate No. T230902

Page 5 of 5

Calibration Report

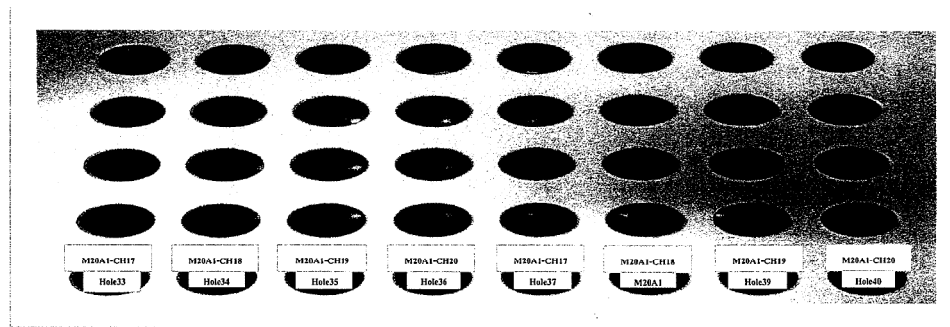

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	Hole33	Hole34	Hole35	Hole36	Hole37	Hole38	Hole39	Hole40
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.7	378.0	378.3	379.0	378.2	378.5	377.3	377.4
			Min °C	377.3	377.6	377.9	378.6	377.7	378.1	376.9	377.0
			Average °C	377.5	377.8	378.1	378.8	378.0	378.3	377.1	377.2
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.2	0.2	0.2

The expanded uncertainty of temperature measurement was ± 1.85 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95 %.

Approved By



บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.

4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพฯ 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
4 Soi Udomsak 14, Bangna, Bangkok 10260 Tel: (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รวม							ck					

Periodical maintenance check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	☐	☒	
2.ISE tubing change	☒	☒	none
3.Syringe check/change		☒	
4.Dispensing check/ change		☒	
5.Waste tubing change when necessary		☒	
6.Lamp check/change	☐	☒	
7.Mixer paddle/paddle change(not Konelab20)		☒	
8.ISE needles check/change		☒	none
9.Pump tubing check/ chance	☐	☒	
10.Broken/worn out part check /change		☒	
11.Peristaltic pump check /cleaning/ lubrication	☐	☒	
12.Heating check		☒	
13.Cooling check		☒	
14.Dispenser mechanic check/adjustment	☐	☒	
15.Cuvette transfer mechanic check/adjustment	☐	☒	
16.Dispenser movement check/adjustment	☐	☒	
17.Sample/reagent register check/adjustment	☐	☒	
18.Dispensing tubing tightness check	☐	☒	
19.Photometer and optics cleaning/check/adjustment	☐	☒	
20.Workstation PC cleaning if necessary	☐	☒	
21.Mechanic cleaning/lubrication	☐	☒	
22.Instrument cleaning if necessary	☐	☒	
23.Complete analyzer testing with waterblank/QC or sample	☐	☒	
24.Test parameters/Adjustment/config. Save to USB key	☐	☒	
25.UPS Test	☐	☒	

Place: ALS LAB Instrument: 890 Aquakem
Date/Time: 12/7/66 Serial no: 28981
Service done by: 57758 Install date:
Signature of customer: 81471 Date/Time: 12/7/66

Accuracy results Aquakem 7.2.AQ2 Page: 1

Laboratory
Analyzer User

7/12/2023 21:21

Performed 7/12/2023
Lot W166

ACCEPTANCE CRITERIA

	Result	Limit	Warning
Temperature (?C)	37.7	37.0 +/- 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	1.17	<1.7	
Photometric noise			
Max SD L340_2 (mA)	0.19	<2.0	
Max SD L340_4 (mA)	1.06	<3.0	
Linearity of photometer			
Slope	1.0188	0.94 - 1.06	
Curvature	0.0035	+/- 0.02	
Max bias from linear fit (mA)	3.2	<15.0	
Max delta %	-2.0	+/- 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (?l)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (?l)	4.13	3.85 - 4.40	
XDISP2 CV%	0.58	<2.0	
XDISP4 CV%	0.70	<2.0	
XDISP10 CV%	0.59	<2.0	
Needle 0 ?l volume			
Average (A)	0.009	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (?l)	0.06	<0.32	

OTHER INFORMATION

Dispensing ratio	Photom. noise: SD (mA)
Posit Result (A)	Posit L340_2 L340_4
1 0.1592	1 0.07 0.64
2 0.1624	2 0.09 1.06
3 0.1631	3 0.14 0.50
4 0.1631	4 0.13 0.53
5 0.1625	5 0.19 0.38
6 0.1650	6 0.02 0.64

Laboratory
Analyzer User


7/12/2023 21:21

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.311
XDISP4	0.616
XDISP10	1.478

Linearity of photometer

L340_	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.001	0.005	-0.004	-394.7
2	0.512	0.519	-0.007	-1.5
3	1.523	1.550	-0.027	-1.8
4	2.027	2.066	-0.039	-1.9
5	2.532	2.582	-0.050	-2.0

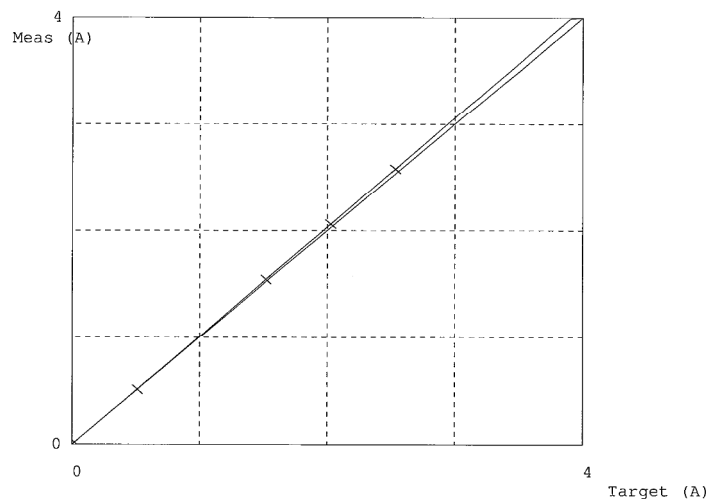

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel: +66 3627 3096 Fax: +66 3627 3100

Bangkok Tel: +668 9205 6851, +669 8247 2360

Website: www.scieco.co.th E-Mail: calibrate@scg.com



Certificate No. T222502

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Oven)

Manufacturer : Memmert

Model : UF 450

Serial No. : B7170531

Customer Code : BKK_EN0273

ID No. : T8042A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250



Customer Location : Oven Room

Date of Receipt : 23 November 2022

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  /Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 DEC 2022

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	29/05/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Certificate No. T222502

Page 2 of 4

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 29 November 2022
Environment : Temperature : 29.1-29.6 °C
Line Voltage : 221.3-223.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors and nine standard thermocouples type T into its chamber , the other one resistance thermometer detector use for ambient temperature measurement .
The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	27-(CH1-10)	T210004	30 December 2022
TC	TYPE T	TN261-TN270	T210010	30 December 2022
DATA LOGGER	34970A	T149	T210004	30 December 2022

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 49 Minute At 104 °C
Fresh Air Damper ☒ Open ☐ Min ☐ Medium ☒ Max
☐ Close
☐ Not Available

5. Adjustment :

() without adjustment

(X) after adjustment


Approved By. Bm Lari



Certificate No. T222502

Page 3 of 4

Calibration Report

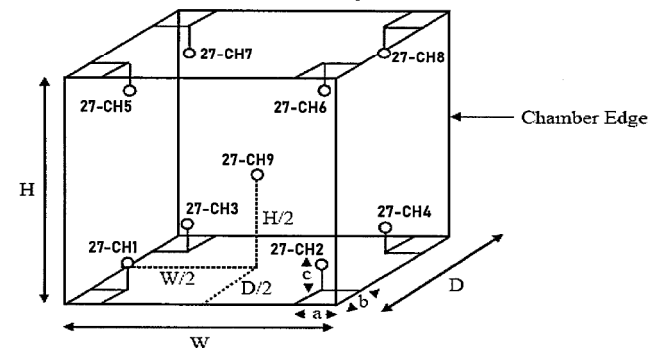

Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.
Size of Installed Standard sensor number 27-CH1 to number 27-CH8 : a = 5 cm. , b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number 27-CH9 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)								
	27-CH1	27-CH2	27-CH3	27-CH4	27-CH5	27-CH6	27-CH7	27-CH8	27-CH9
104	104.07	103.60	103.45	104.02	104.47	103.57	104.59	103.78	104.18

Chamber (Oven)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min , Max	Average					
104.0	-	104.0	103.97	0.07	0.70	0.42	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. Bm Lari



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.




NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T222502

Page 4 of 4

Calibration Report

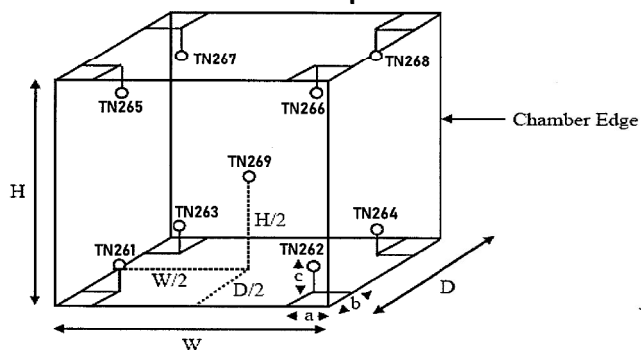

Remark :

Internal Dimensions of Chamber : W (Width) = 104 cm. , H (Height) = 72 cm. and D (Depth) = 60 cm.
Size of Installed Standard sensor number TN261 to number TN268 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
Size of Installed Standard sensor number TN269 : W/2 = 104 cm./2 , H/2 = 72 cm./2 and D/2 = 60cm./2

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)								
	TN261	TN262	TN263	TN264	TN265	TN266	TN267	TN268	TN269
180	179.14	179.17	179.65	179.26	180.41	179.64	181.18	180.99	180.36

Chamber (Oven)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
180.0	-	180.0	179.98	0.38	1.78	1.10	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing

a level of confidence of approximately 95 % .

Approved By:

FM-L15 117/15-05-63



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484

Cert. No.: 23TM568

Page : 1 of 3

Certificate of Calibration

Equipment : Autoclave
Manufacturer : AES Laboratory
Model : Masterclave 528
Serial No. : 34677152
ID No. : BKK_ML0043

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Media Preperation Room

Received Order : 10 April 2023
Calibration Date : 10 April 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Preecha Hlahib

Approved by :
Approved Signatory

() Pornthippa Tameyakul
(/) Malee Butkruea
() Suwit Imjai

Issue Date : 24 April 2023

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration and Testing Equipment Services.

A 0010941



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2304-0148OC-2
Cert. No.: 23TM568
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY49023932	22LM97	29 Jul 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**


(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)

It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source



	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	60	220
Finished of Calibration	26	65	221

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	21-16TC-04
2 =	Temperature sensor	21-16TC-05
3 =	Exhaust port	21-16TC-06

Malu.



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2304-0148OC-2
Cert. No.: 23TM568
Page : 3 of 3

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Operating parameter Set : Temperature = 121.0 °C

Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (-)	Uncertainty (± °C)	Coverage Factor k
121.0	121.0	1	120.989	0.23	-	0.75	2
		2	120.957				
		3	121.068				

Operating parameter Set : Temperature = 37.0 °C

Sterilization period = 30 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (-)	Uncertainty (± °C)	Coverage Factor k
37.0	37.0	1	36.876	0.29	-	0.66	2
		2	36.868				
		3	37.015				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1146
Page : 1 of 3

Certificate of Calibration

Equipment : Incubator
Manufacturer : SHEL-LAB
Model : 1915A
Serial No. : 0200599
ID No. : BKK_ML0010
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : Incubation & Micrological Reading
Received Order : 17 July 2023
Calibration Date : 17 July 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Man Pattanapongpaiboon

Approved by :

Malee
Approved Signatory

() Pornthippa Tameyakul
() Malee Butkruea
() Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1
Procedure Used :-

Cert. No.: 23TM1146
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	56
AC Supply (Volt)	221	223

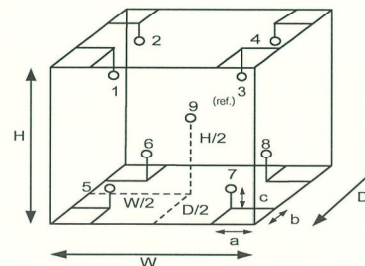

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.50 m
W = 0.75 m
H = 1.2 m
Capacity = 0.45 m³

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Malee



Equipment : Incubator
 Condition As-Received : Used Item
 Reference : 2307-0285OC-1
Result of Calibration :- (*) Without Adjustment
 Function of UUC* : Temperature Source
 Fresh air setting : Close

Cert. No.: 23TM1146
 Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.055	0.30	0.44	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.888	34.933	34.815	34.813	35.064	35.019	35.156	35.141	35.087	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malee

a 1172188



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
 CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
 534/4 PATTANAKARNROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
 TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1571
 Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Binder

Model : ED 240/E2

Serial No. : 00-15533

ID No. : BKK_ML0013

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
 104 Phatthanakan 40, Phatthanakan Rd.,
 Khwaeng Phatthanakan, Khet Suan Luang,
 Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 21 November 2022

Calibration Date : 21 November 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by : *Malee*
 Approved Signatory

() Pornthippa Tameyakul
 (✓) Malee Butkruea
 () Suwit Imjai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
 Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

REVIEW BY	<i>Sithichok</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	21/05/24

A 0048150



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1

Cert. No.: 22TM1571
Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) After Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

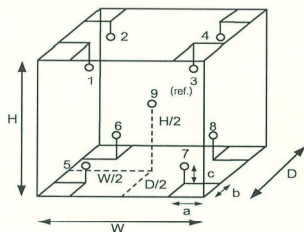

Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
W = 0.80 m
H = 0.60 m
Capacity = 0.24 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	53	55
AC Supply (Volt)	219	220

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

Malu.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1571
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
334/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10230
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM637
Page : 1 of 3

Certificate of Calibration

Equipment : Water Bath

Manufacturer : Memmert

Model : WNE 45

Serial No. : L712.0429

ID No. : BKK_ML0056

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Incubator & Microbiological Reading

Received Order : 20 April 2023

Calibration Date : 20 April 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Kunchit Promprat

Approved by : 
Approved Signatory

() Pornthippa Tameyakul

() Malee Butkruea

() Suwit Imjai

Issue Date : 24 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2304-0253OC-1

Cert. No.: 23TM637
Page : 2 of 3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44073381	22LM78/1	12 May 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	45	223
Finished of Calibration	25	43	223

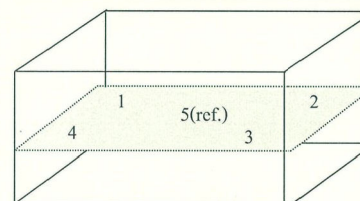

Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016





Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2304-0253OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM637
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.492	44.463	44.475	44.510	44.491	0.15
45.0	45.0	45.0	45.005	44.962	44.979	45.016	44.986	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor <i>k</i>
44.5	0.051	0.022	2
45.0	0.080	0.026	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu

a 1158264

HACH COMPANY

C/O AB Sciex (Thailand) Limited, Building D Room No. D3 11, 3rd Floor, No. 735/4, Srinakarin Road, Pattanakarn, Suanluang, Bangkok
Phone +66 (02) 026-3529 Ext. 0 | Fax +66(02) 026-3572 | www.sea.hach.com

LABX 2300391

Test Report

Customers	ALS Laboratory Group (Thailand) Co., Ltd.		
Equipment	Chlorine Meter	Manufacturer	HACH
Controller Model	Pocket II Cl2	ID No.	BKK_LG0032
Controller Serial No.	18110E374141	Sensor Serial No.	-
Date of test	28/02/2023	Period	-
Environment temperature	25.0 °C	Humidity	56.0 %RH

Results

Instrument Checked

Item	Characteristic	Before		After		Remark
1	Visual Inspect	☒ Pass	☐ Fail	☒ Pass	☐ Fail	
2	Power Supply (4.5 – 6.5 VDC)	6.0 VDC		6.0 VDC		
3	Display Check	☒ Pass	☐ Fail	☒ Pass	☐ Fail	
4	Keyboard Check	☒ Pass	☐ Fail	☒ Pass	☐ Fail	
5	Function System Program	☒ Pass	☐ Fail	☒ Pass	☐ Fail	

Warning and Error Checked

Item	Event	Before		After	
6	Error list	☒ None	☐ Appear	☒ None	☐ Appear

Check with Standard

Item	Characteristic	Before		After		Remark
	DPD-CHLORINE-LR					
7	Blank (0.00 mg/l)	0.00	mg/l	0.00	mg/l	
8	Standard Cl2 No. 1 (0.23 ± 0.09 mg/l)	0.25	mg/l	0.24	mg/l	
9	Standard Cl2 No. 2 (0.89 ± 0.10 mg/l)	0.92	mg/l	0.90	mg/l	
10	Standard Cl2 No. 3 (1.64 ± 0.14 mg/l)	1.66	mg/l	1.64	mg/l	
	DPD-CHLORINE-HR					
11	Blank (0.0 mg/l)	0.0	mg/l	0.0	mg/l	
12	Standard Cl2 No. 1 (2.1 ± 0.2 mg/l)	2.2	mg/l	2.1	mg/l	
13	Standard Cl2 No. 2 (3.9 ± 0.3 mg/l)	3.9	mg/l	3.9	mg/l	
14	Standard Cl2 No. 3 (6.8 ± 0.6 mg/l)	6.8	mg/l	6.8	mg/l	

REVIEW BY *Chayathorn P.*
APPROVED BY *Haralorn P.*
NEXT CAL. DATE 28/02/24



HACH COMPANY

C/O AB Sciex (Thailand) Limited, Building D Room No. D3 11, 3rd Floor, No. 735/4, Srinakarin Road, Pattanakarn, Suanluang, Bangkok
 |Phone +66 (02) 026-3529 Ext. 0 | Fax +66(02) 026-3572 | www.sea.hach.com

LABX 2300391

Summary of checked

- ☒ The instrument can work normally and efficiently. (เครื่องมือวัดสามารถทำงานได้ปกติและมีประสิทธิภาพ)
☐ The instrument can work but it's requiring to maintenance. (เครื่องมือวัดสามารถทำงานได้แต่ต้องบำรุงรักษา)
☐ The instrument could not work it's requiring to repair. (เครื่องมือวัดไม่สามารถทำงานได้และต้องการซ่อมบำรุง)

Remark:

Standard Equipment Used

Equipment	Equipment I.D.		
Standard Chlorine DPD-CHLORINE-LR	Lot No. A2131	Exp date :	May-24
Standard Chlorine DPD-CHLORINE-HR	Lot No. A2104	Exp date :	Apr-24
Digital multi meter	S/N : 97270010	Due date :	23-Jun-23
Thermo hygrometer	S/N : 41413945	Due date :	17-Aug-23

Test By :

WILAILAK S.

(Miss Wilailak Sawangpun)

Service Engineer



Approved By

Position

S. Sany

(Mr. Suanun Sartyangkool)

Assistant Service Division Manager



บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.

4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพฯ 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
 4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รวม	PM 6M CK											

Periodical maintenance check list for Konelab

	6M	12M	Note!
1. Diluent-wash tubing change	☒	☐	
2. ISE tubing change	☒	☒	none.
3. Syringe check/change	☐	☐	
4. Dispensing check/ change	☐	☐	
5. Waste tubing change when necessary	☐	☐	
6. Lamp check/change	☒	☐	
7. Mixer paddle/paddle change(not Konelab20)	☐	☐	
8. ISE needles check/change	☐	☐	
9. Pump tubing check/ change	☒	☐	
10. Broken/worn out part check /change	☐	☐	
11. Peristaltic pump check /cleaning/ lubrication	☒	☐	
12. Heating check	☐	☐	
13. Cooling check	☐	☐	
14. Dispenser mechanic check/adjustment	☒	☐	
15. Cuvette transfer mechanic check/adjustment	☒	☐	
16. Dispenser movement check/adjustment	☒	☐	
17. Sample/reagent register check/adjustment	☒	☐	
18. Dispensing tubing tightness check	☒	☐	
19. Photometer and optics cleaning/check/adjustment	☒	☐	
20. Workstation PC cleaning if necessary	☒	☐	
21. Mechanic cleaning/lubrication	☒	☐	
22. Instrument cleaning if necessary	☒	☐	
23. Complete analyzer testing with waterblank/QC or sample	☒	☐	
24. Test parameters/Adjustment/config. Save to USB key	☒	☐	
25. UPS Test	☒	☐	

Place: ALS Laboratory Instrument: Kae Aquakem 250

Date/Time: 05-01-66 Serial no: 89781

Service done by: Sae Se Install date:

Signature of customer: Sae Se Date/Time:



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 21CG5290
Page.: 1 of 2

Certificate of Calibration

Equipment : Burette
Capacity : 10 mL
Serial No. : -
ID. No. : BKK_EN0296

Manufacturer : Witeg
Made in : Germany

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.
Khwaeng Phatthanakan, Khet Suan Luang
Bangkok 10250 Thailand

Ambient Temperature : $(20 \pm 2.5) ^\circ\text{C}$
Relative Humidity : $(50 \pm 10) \%$
Barometric Pressure : 759 mmHg
Calibration Procedure : ASTM E 542 - 01

Calibrated by : Panward Pramklam

Approved by : Malee
Approved Signatory

() Pornthippa Tameyakul
(✓) Malee Butkruea
() Ponpan Paipim
() Srisuda Khamtha

Issue Date : 27 December 2021

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Burette
Received Date : 22 December 2021
Condition As-Received : Used Item
Calibration Date : 24 December 2021
Reference : 2112-0571DSC-13

Cert.No.: 21CG5290
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	AE200S	N03679	140RC001	21MM429	NIMT	22 Sep 2022
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	21H1366	NIST,NIMT	21 June 2022
3) Thermometer	-	0834181	140EC005	21I836	NIMT	03 Aug 2022

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.
3. True value is converted to true volume at the standard temperature of $20 ^\circ\text{C}$

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty ($\pm$ mL)	k Factor
10	9.9982	0.0038	2.00

Remark mL = cm^3

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Malee



Certificate of Calibration

ICS-2100: Anion (ID#659)

This certificate is to verify that instrument below are calibrated
by Archemica Lab Co., Ltd.

ICS-2100 S/N: 15010977

AS-HV S/N: 5450A36659

For

ALS Laboratory Group (Thailand) Co., Ltd.

Operator Signature: _____ Date: Jan 12, 2023

(Mr. Nutsanai Laekhwan)

Application Chemist

REVIEW BY Aulcharawan S.
APPROVED BY Sarat M.
NEXT CAL. DATE 12 Jan 24



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-20 FAX. 0-2719-9484



Cert.No.: 23CHO30
Page.: 1 of 3

Certificate of Calibration

Equipment :	Spectrophotometer
Manufacturer :	HACH
Model :	DR 3900
Serial No. :	1687645
ID No. :	SGK_CL0038
Condition As-Received:	Used Item
Received Date :	23 January 2023
Calibration Date :	24 January 2023
Reference :	2301-0661OC-1
Submitted by :	ALS Laboratory Group (Thailand) Co., Ltd. Songkhla Branch. 114/1 Moo 8 , Kanjanavanij Rd., Banphru , Hatyai , Songkhla 90250 , Thailand
Calibration Place :	Chemistry Room
Ambient Temperature :	(28.3 - 27.3) °C (On-Site)
Relative Humidity :	(49.6 - 49.9) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-01

Calibrated by : Kunchit Promprat

Approved by :

Malee Butkrua

Approved Signatory

- (☒) Malee Butkrua
(☐) Saithip Meangmai
(☐) Warakorn Lemgagrakul

Issue Date : 7 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert. No. : 23CHO30

Page : 2 of 3

Condition of calibration result**1. Reference Standard Material :**

Material	Serial No.	Certificate No.	Due date
1. Absorbance Standard set	32593	100581	30 Mar 2024
2. Wavelength Standard set	29829	94776	02 Sep 2023
3. Wavelength Standard set	29829	94777	02 Sep 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained at :
- National Physical Laboratory (NPL), The United Kingdom of Great Britain and Northern Ireland
- National Institute of Standards and Technology (NIST), The United States of America

4. Spectral BandWidth : 5 nm
Scan Speed : - nm/min

Calibration Results : without adjustment**Wavelength Accuracy**

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement ($\pm$ nm)	Coverage Factor <i>k</i>
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	514	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
684.70	685	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00



Cert. No. : 23CHO30

Page : 3 of 3

Calibration Results : without adjustment**Photometric Accuracy**

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement ($\pm$ Abs)	Coverage Factor <i>k</i>
420.0	Zero	0.000	0.0028	2.00
	0.5701	0.568	0.0029	2.00
	0.7147	0.712	0.0030	2.00
	1.0031	0.999	0.0030	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5552	0.553	0.0029	2.00
	0.7031	0.700	0.0030	2.00
	0.9867	0.981	0.0029	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5178	0.517	0.0030	2.00
	0.6642	0.663	0.0029	2.00
	0.9312	0.930	0.0030	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5195	0.517	0.0030	2.00
	0.7007	0.698	0.0029	2.00
	0.9833	0.979	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5537	0.550	0.0030	2.00
	0.7763	0.771	0.0029	2.00
	1.0912	1.083	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5615	0.558	0.0029	2.00
	0.7659	0.762	0.0030	2.00
	1.0763	1.070	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

a 1146846

a 1146845



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM676

Page.: 1 of 3

Certificate of Calibration

Equipment : Autoclave
Manufacturer : TOMY
Model : SX-700
Serial No. : 48134190
ID No. : BKK_ML0041

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Location : Media Preparation Room

Received Order : 20 May 2022
Calibration Date : 20 May 2022
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Preecha Hlahib

Approved by :

Approved Signatory

() Pornthippa Tameyakul
() Malee Butkruea
(✓) Suwit Imjai

Issue Date : 24 May 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2205-0404OC-2
Procedure Used :-

Cert. No.: 22TM676

Page.: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013823	22LM24	26 Feb 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)
It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source



	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	24	55	220
Finished of Calibration	26	57	221

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	19-17TC-11
2 =	Temperature sensor	19-17TC-12
3 =	Exhaust port	19-17TC-13

a 1109670

A 0041435



Equipment : Autoclave
 Condition As-Received : Used Item
 Reference : 2205-0404OC-2
 Result of Calibration :- (*) Without Adjustment

Cert. No.: 22TM676
 Page.: 3 of 3

Operating parameter Set : Temperature = 108 °C
 Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
108	108	1	107.536	0.19	0.04	0.91	2
		2	107.542				
		3	107.471				

Operating parameter Set : Temperature = 115 °C
 Sterilization period = 20 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
115	115	1	114.502	0.15	0.08	0.89	2
		2	114.582				
		3	114.539				

Operating parameter Set : Temperature = 118 °C
 Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
118	118	1	117.517	0.094	0.09	0.88	2
		2	117.616				
		3	117.530				

Result of Calibration :- (*) Without Adjustment

Operating parameter Set : Temperature = 121 °C
 Sterilization period = 30 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
121	121	1	120.400	0.18	1.1	0.90	2
		2	120.511				
		3	120.465				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Signature

a 1109669



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
 CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
 534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
 TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM102
 Page.: 1 of 3

Certificate of Calibration

Equipment : Incubator

Manufacturer : SHEL-LAB

Model : 1915A

Serial No. : 0200599

ID No. : BKK_ML0010

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
 104 Phatthanakan 40, Phatthanakan Rd.,
 Khwaeng Phatthanakan, Khet Suan Luang,
 Bangkok 10250 Thailand

Location : Incubation & Micrological Reading

Received Order : 21 January 2022

Calibration Date : 21 January 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by : *Malee*
 Approved Signatory

() Pornthippa Tameyakul
 () Malee Butkruea
 () Suwit Imjai

Issue Date : 3 February 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
 Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0037377



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2201-0616OC-1

Cert. No.: 22TM102
Page.: 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013711	21LM7	16 Jun 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

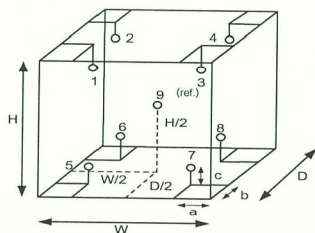

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.90 m
W = 0.75 m
H = 1.2 m
Capacity = 0.81 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	25
REL.Humid. (%)	53	54
AC Supply (Volt)	220	221

Position :	Ref. Std. ID No.:
1	18-18RTD-01
2	18-18RTD-02
3	18-18RTD-03
4	18-18RTD-04
5	18-18RTD-05
6	18-18RTD-06
7	18-18RTD-07
8	18-18RTD-08
9 (ref.)	18-18RTD-09

Malu.



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2201-0616OC-1

Cert. No.: 22TM102
Page.: 3 of 3

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
35.0	35.0	35.0	0.043	0.41	0.42	0.30	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
35.0	34.801	34.868	34.862	35.012	35.040	35.010	35.084	35.040	35.178

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM104
Page : 1 of 3

Certificate of Calibration

Equipment : Water Bath

Manufacturer : Memmert

Model : WB 45

Serial No. : L799.0009

ID No. : BKK_ML0049

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Biochemical Lab

Received Order : 19 January 2023

Calibration Date : 19 January 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Khit Ruttanaprapachai

Approved by : 
Approved Signatory

() Pornthippa Tameyakul

(✓) Malee Butkruea

() Suwit Imjai

Issue Date : 2 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2301-0577OC-1
Procedure Used :-

Cert. No.: 23TM104
Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	
Beginning of Calibration	23	53	221
Finished of Calibration	24	57	222

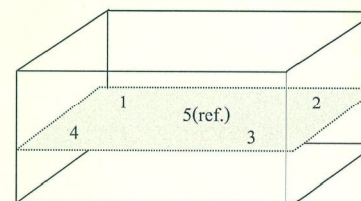

Front

Position :	Ref. Std. ID No.:
1	70RC143
2	70RC144
3	70RC145
4	70RC146
5(ref.)	70RC147





Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2301-0577OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM104
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)				
			Position				
			1	2	3	4	5 (ref.)
42.0	44.9	44.9	41.996	42.005	41.974	42.021	42.036

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
42.0	0.11	0.037	0.15	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.