

ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

ลำดับที่ 1	คุณภาพอากาศในบรรยากาศ
ลำดับที่ 2	คุณภาพอากาศจากแหล่งกำเนิด
ลำดับที่ 3	ระดับเสียง
ลำดับที่ 4	คุณภาพน้ำ
ลำดับที่ 5	คุณภาพอากาศในการทำงาน
ลำดับที่ 6	ระดับเสียงในการทำงาน
ลำดับที่ 7	ระดับความร้อนในการทำงาน

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ระยะดำเนินการ)**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
1. คุณภาพอากาศในบรรยากาศ Total Suspended Particulate (TSP)	High Volume Air Sampler Blow No. R06, R08	Digital Balance
Particulate Matter less than 10 microns (PM-10)	High Volume PM-10 Air Sampler Blow No. R16, R17	Digital Balance
Nitrogen Dioxide (NO _x)	NO/NO ₂ /NO _x Analyzer No. R05, R07	NO/NO ₂ /NO _x Analyzer No. R05, R07
2. คุณภาพอากาศจากปล่อง Total Suspended Particulate (TSP)	Console No. R05 Pitot Tube No. B35	Digital Balance
Oxides of Nitrogen (NO _x)	Vacuum Gauge	Spectrophotometer
3. ระดับเสียงในบรรยากาศ L _{eq} 24 hr, L ₉₀ , L _{max} , L _{dn}	Acoustic Calibrator Sound Level Meter No. ACO-R08, R09, R10, R11, R20	-
4. คุณภาพน้ำ pH	-	pH Meter
Total Suspended Solids (TSS)	-	Digital Balance
COD	-	COD Reactor
Grease & Oil	-	Digital Balance
5. คุณภาพอากาศในสถานที่ทำงาน Total Dust	Personal Pump SKC No. R14, R16 Rotameter No. H- R05	Digital Balance
Respirable Dust	Personal Pump SKC No. R13 Rotameter No. H- R05	Digital Balance
Aluminium	Personal Pump SKC No. R28, R31 Rotameter No. H- R05	ICP
Hydrogen Fluoride	Personal Pump SKC No. R23 Rotameter No. L-R05	Ion Chromatography
Oil Mist	Personal Pump SKC No. R25 Rotameter No. L- R05	Ion Chromatography
6. ระดับเสียงในการทำงาน L _{eq} 1 hr, L _{eq} 8 hr และ	Acoustic Calibrator Sound Level Meter ACO No. R25, R28, R30	-
Noise Dose	Acoustic Calibrator Sound Level Meter ACO No. R03, R05, R13	-
7. ระดับความร้อนในการทำงาน WBGT	Heat Meter No. R04, R09, R11	-

คุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-0370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R ²
B35	B35	01/11/2023	y = 1.247x-5.373	0.999
B36	B36	02/11/2023	y = 1.190x-2.630	0.995
B37	B37	01/11/2023	y = 1.188x-2.249	0.999
B38	B38	01/11/2023	y = 1.191x-5.051	0.995
B39	B39	01/11/2023	y = 1.230x-3.335	0.995
B40	B40	02/11/2023	y = 1.172x-2.695	0.998
B41	B41	02/11/2023	y = 1.169x-2.206	0.998
B42	B42	02/11/2023	y = 1.212x-5.591	0.998
B43	B43	03/11/2023	y = 1.223x-3.058	0.997
B44	B44	01/11/2023	y = 1.194x-2.207	0.996
R01	R01	08/11/2023	y = 1.199x-4.374	0.998
R02	R02	06/11/2023	y = 1.229x-6.243	0.999
R03	R03	08/11/2023	y = 1.239x-7.264	0.998
R04	R04	09/11/2023	y = 1.182x-3.161	0.998
R05	R05	09/11/2023	y = 1.141x-2.095	0.997
R06	R06	03/11/2023	y = 1.155x-2.543	0.997
R07	R07	09/11/2023	y = 1.057x+1.380	0.999
R08	R08	02/11/2023	y = 1.230x-6.615	0.997
R09	R09	04/11/2023	y = 1.188x-1.331	0.997
R10	R10	04/11/2023	y = 1.213x-3.671	0.998
R11	R11	01/11/2023	y = 1.136x-2.259	0.999
R12	R12	01/11/2023	y = 1.145x-3.404	0.998
R13	R13	02/11/2023	y = 1.076x-0.153	0.999
R14	R14	02/11/2023	y = 1.166x+1.197	0.996
R15	R15	09/11/2023	y = 1.171x-4.139	0.997
R16	R16	09/11/2023	y = 1.142x-3.462	0.999
R17	R17	01/11/2023	y = 1.169x-3.932	0.998
R18	R18	01/11/2023	y = 1.192x-4.280	0.998
R19	R19	01/11/2023	y = 1.158x-4.004	0.996
R20	R20	02/11/2023	y = 1.191x-4.426	0.997



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-0370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R ²
R01	R01	01/11/2023	y = 1.166x-2.827	0.999
R02	R02	01/11/2023	y = 1.140x+0.079	0.998
R03	R03	02/11/2023	y = 1.176x-2.983	0.999
R04	R04	01/11/2023	y = 1.155x-3.417	0.996
R05	R05	01/11/2023	y = 1.193x-5.553	0.998
R06	R06	08/11/2023	y = 1.173x-2.245	0.998
R07	R07	08/11/2023	y = 1.183x-3.521	0.999
R08	R08	06/11/2023	y = 1.195x-5.732	0.997
R09	R09	01/11/2023	y = 1.161x-3.857	0.995
R10	R10	09/11/2023	y = 1.181x-4.105	0.998
R11	R11	09/11/2023	y = 1.155x-0.430	0.996
R12	R12	09/11/2023	y = 1.196x-4.411	0.999
R13	R13	09/11/2023	y = 1.188x-3.031	0.996
R14	R14	01/11/2023	y = 1.167x-2.357	0.998
R15	R15	02/11/2023	y = 1.186x-3.860	0.998
R16	R16	02/11/2023	y = 1.187x-2.636	0.999
R17	R17	02/11/2023	y = 1.169x-3.318	0.996
R18	R18	03/11/2023	y = 1.190x-4.826	0.997
R19	R19	01/11/2023	y = 1.152x-2.131	0.996
R20	R20	01/11/2023	y = 1.183x-4.568	0.997



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	17 December 2023	BRAND :	API	MODEL :	200E
NO.	NOX-R05	SERIAL NO.	4413		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 08 August 2023		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: D636192	
Certified Date	: 20 April 2022		Expired Date	: 20 April 2024	
Cylinder Conc.	: 49.1 ppm				
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	400.1	0.025	400.0	1.009
NO _x Span	400	400.3	0.075	400.0	1.013
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	505	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.2	mV	-20 - 150		
AZERO	93.8	mV	-20 - 150		
HVPS	674	V	420 - 900 constant		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.2	°C	8 - 48		
PMT TEMP	7.4	°C	7 ± 2		
MOLY TEMP	315.3	°C	315 ± 5		
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.009	-	1.0 ± 0.3		
NO _x Slope	1.013	-	1.0 ± 0.3		
NO Offset	1.6	mV	-20 to +150		
NO _x Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO ₂ / NO _x ANALYZER					
DATE :	17 December 2023	BRAND :	API	MODEL :	200E
NO.	NOX-R07	SERIAL NO.	4468		
Calibrator (Dilution System)					
Brand	: API		Model	: 700	
Last Cal. Date	: 08 August 2023		Serial No.	: 911	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: D636192	
Certified Date	: 20 April 2022		Expired Date	: 20 April 2024	
Cylinder Conc.	: 49.1 ppm				
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.9	-0.025	400.0	1.007
NO _x Span	400	400.2	0.050	400.0	1.011
API Model 200E NO _x Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	510	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.3	mV	-20 - 150		
AZERO	94.0	mV	-20 - 150		
HVPS	670	V	420 - 900 constant		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.5	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	314.8	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO _x Span Conc	400	PPB	20 - 20,000		
NO Slope	1.007	-	1.0 ± 0.3		
NO _x Slope	1.011	-	1.0 ± 0.3		
NO Offset	1.5	mV	-20 to +150		
NO _x Offset	0.9	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		



CERTIFICATE No : 23M2441
REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA 05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY :

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23° C \pm 1° C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

- THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.
- REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25
- THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
- THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
- THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

- ZERO SETTING FUNCTION : NORMAL
- TARE FUNCTION : NORMAL
- REPEATABILITY OF READING AT 200 g WAS 0 g
- DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STAND
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY
END OF CALIBRATION REPORT

คุณภาพอากาศจากแหล่งกำเนิด



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH _g (mmH ₂ O)
B01	1563	04/09/2023	0.997	50.11
B02	8002514	06/09/2023	1.002	49.25
B03	1503016	05/09/2023	0.998	50.44
B04	00006659	05/09/2023	1.004	49.37
B05	00007428	05/09/2023	0.996	49.77
R01	1561	06/09/2023	1.004	49.86
R02	8002513	08/09/2023	1.005	50.36
R03	1570	07/09/2023	0.997	49.55
R04	8002519	04/09/2023	1.004	49.69
R05	1503015	07/09/2023	0.999	50.08

Remark : Accept Value of y (test) is $0.97 < y < 1.03$

Accept Value of DH_g (test) is 46.7 ± 6.4 (mmH₂O)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	01/11/2023	0.84	0.85
B04	S	0.99	01/11/2023	0.84	0.84
B05	S	0.99	01/11/2023	0.85	0.84
B07	S	0.99	01/11/2023	0.84	0.83
B08	S	0.99	02/11/2023	0.85	0.84
B09	S	0.99	02/11/2023	0.84	0.84
B11	S	0.99	02/11/2023	0.85	0.84
B16	S	0.99	03/11/2023	0.84	0.84
B18	S	0.99	03/11/2023	0.84	0.85
B19	S	0.99	03/11/2023	0.84	0.85
B21	S	0.99	02/11/2023	0.84	0.84
B24	S	0.99	02/11/2023	0.84	0.83
B27	S	0.99	02/11/2023	0.85	0.84
B30	S	0.99	01/11/2023	0.84	0.85
B31	S	0.99	02/11/2023	0.84	0.84
B33	S	0.99	02/11/2023	0.84	0.85
B35	S	0.99	02/11/2023	0.84	0.84



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : HI-LIGHT
MODEL / TYPE : N/A
SERIAL NO. : N/A[64-220088-1]
CLID. NO. : 212301419
JOB CONTROL NO. : 230725081570

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 25 July 2023

DATE OF ISSUED : 31 July 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee

Approved By :

31 July 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23081570

F3-011-04/01-12

page 1 of 3



@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : HI-LIGHT
MODEL / TYPE : N/A
SERIAL NO. : N/A[64-220088-1]
DATE OF CALIBRATION : 26 July 2023
DUE DATE OF CALIBRATION : 26 July 2024

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-05 according to DKD-R 6-1 as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0035-23, Due Date 02 February 2024.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q23081570

F3-011-04/01-12

page 2 of 3



@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (kPa)		Conversion to inHg		Correction (inHg)	
	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-15.07	-15.10	-4.5	-4.5	+0.5	+0.5
-10	-32.10	-32.13	-9.5	-9.5	+0.5	+0.5
-15	-49.20	-49.23	-14.5	-14.5	+0.5	+0.5
-20	-66.26	-66.26	-19.6	-19.6	+0.4	+0.4
-25	-83.30	-83.33	-24.6	-24.6	+0.4	+0.4
-30	-100.39	-100.39	-29.6	-29.6	+0.4	+0.4

Uncertainty of measurement ± 0.2 inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23081570

F3-011-04/01-12

page 3 of 3



@clccalibration



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 939-4370-77, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 $^{\circ}\text{C}$
Pressure : 1010 ± 15 mmbar

Personal Pump Data					Calibration Data							
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B01	SKC	224-PCXR4	262101	02/10/2023	1,000	1,500	2,000	997	1,494	1,995	0.998x - 5.198	1.000
B02	SKC	224-PCXR4	626166	02/10/2023	1,000	1,500	2,000	995	1,491	1,987	0.995x - 0.239	1.000
B03	SKC	224-PCXR4	612968	02/10/2023	1,000	1,500	2,000	994	1,498	1,996	1.004x - 17.211	0.999
B04	SKC	224-PCXR4	602804	03/10/2023	1,000	1,500	2,000	1,001	1,502	1,997	0.999x - 3.961	1.000
B05	SKC	224-PCXR4	612693	03/10/2023	1,000	1,500	2,000	1,000	1,500	1,998	1.008x - 19.564	0.999
B06	SKC	224-PCXR4	262188	04/10/2023	1,000	1,500	2,000	999	1,497	1,998	1.005x - 13.275	1.000
B07	SKC	224-PCXR4	626262	04/10/2023	1,000	1,500	2,000	997	1,491	1,992	0.995x + 0.103	1.000
B08	SKC	224-PCXR4	626100	03/10/2023	1,000	1,500	2,000	995	1,490	1,994	0.999x - 3.162	1.000
B09	SKC	224-PCXR4	626479	04/10/2023	1,000	1,500	2,000	1,012	1,500	2,001	0.998x + 1.604	0.999
B10	SKC	224-PCXR4	091950	05/10/2023	1,000	1,500	2,000	992	1,486	1,994	1.002x - 11.842	1.000
B11	SKC	224-PCXR8	564315	05/10/2023	1,000	1,500	2,000	993	1,501	1,996	1.010x - 26.335	0.999
B12	SKC	224-PCXR4	034656	05/10/2023	1,000	1,500	2,000	1,000	1,496	1,998	1.007x - 17.721	0.999
B13	SKC	224-PCXR4	602073	04/10/2023	1,000	1,500	2,000	1,000	1,488	1,987	0.986x + 13.398	1.000
B14	SKC	224-PCXR4	626313	04/10/2023	1,000	1,500	2,000	996	1,493	1,996	0.999x - 2.380	1.000
B15	SKC	224-PCXR4	626474	06/10/2023	1,000	1,500	2,000	1,000	1,498	1,998	1.007x - 16.567	0.999
B16	SKC	224-PCXR4	626477	06/10/2023	1,000	1,500	2,000	1,001	1,498	1,999	1.010x - 21.673	0.999
B17	SKC	224-PCXR4	626860	06/10/2023	1,000	1,500	2,000	1,000	1,492	1,998	0.997x - 1.859	1.000
B18	SKC	224-PCXR4	691484	03/10/2023	1,000	1,500	2,000	995	1,494	1,992	1.000x - 5.493	1.000
B19	SKC	224-PCXR4	691599	02/10/2023	1,000	1,500	2,000	991	1,500	1,998	1.015x - 32.922	0.999
B20	SKC	224-PCXR4	691587	02/10/2023	1,000	1,500	2,000	1,001	1,496	1,999	1.010x - 23.222	0.999
B21	SKC	224-PCXR4	691531	03/10/2023	1,000	1,500	2,000	994	1,491	1,997	1.004x - 12.881	1.000
B22	SKC	224-PCXR4	691654	03/10/2023	1,000	1,500	2,000	991	1,492	1,994	1.002x - 9.860	1.000
B23	SKC	224-PCXR4	798393	02/10/2023	1,000	1,500	2,000	991	1,498	1,997	1.014x - 33.810	0.999
B24	SKC	224-PCXR4	626363	02/10/2023	1,000	1,500	2,000	1,001	1,499	2,001	1.011x - 23.676	0.999
B25	SKC	224-PCXR4	798489	04/10/2023	1,000	1,500	2,000	996	1,497	1,989	0.991x + 6.619	1.000
B26	SKC	224-PCXR4	798479	05/10/2023	1,000	1,500	2,000	996	1,492	1,990	0.996x - 1.146	1.000
B27	SKC	224-PCXR4	691673	09/10/2023	1,000	1,500	2,000	989	1,506	1,998	1.016x - 34.646	0.999
B28	SKC	224-PCXR4	691570	09/10/2023	1,000	1,500	2,000	992	1,487	1,996	1.006x - 16.996	1.000
B29	SKC	224-PCXR4	626472	09/10/2023	1,000	1,500	2,000	998	1,495	1,992	0.997x - 0.693	1.000
B30	SKC	224-PCXR4	691489	03/10/2023	1,000	1,500	2,000	993	1,490	1,990	0.999x - 7.320	1.000
B31	SKC	224-PCXR4	691509	03/10/2023	1,000	1,500	2,000	1,001	1,497	1,997	1.007x - 18.788	0.999
B32	SKC	224-PCXR4	091567	04/10/2023	1,000	1,500	2,000	998	1,499	1,996	1.009x - 22.780	0.999
B33	SKC	224-PCXR4	091756	05/10/2023	1,000	1,500	2,000	1,000	1,489	1,994	0.995x - 0.223	1.000
B34	SKC	224-PCXR4	612962	05/10/2023	1,000	1,500	2,000	992	1,501	1,997	1.013x - 31.362	0.999
B35	SKC	224-PCXR4	602682	03/10/2023	1,000	1,500	2,000	998	1,496	1,998	0.998x - 7.157	0.999
B36	SKC	224-PCXR4	626164	07/10/2023	1,000	1,500	2,000	995	1,487	1,990	0.991x + 3.901	1.000
B37	SKC	224-PCXR4	626256	02/10/2023	1,000	1,500	2,000	990	1,500	1,993	1.000x - 6.520	1.000
B38	SKC	224-PCXR4	626167	03/10/2023	1,000	1,500	2,000	989	1,498	1,995	1.015x - 35.470	0.999
B39	SKC	224-PCXR8	034637	09/10/2023	1,000	1,500	2,000	991	1,505	1,995	1.005x - 14.533	0.999



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data				Calibration Data							
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)			y	R ²
				1	2	3	1	2	3		
H-R01	Dwyer	VFB-65	02/10/2023	500	1,000	2,000	502.9	994.2	1977.4	1.003x - 7.740	0.999
H-R02	Dwyer	VFB-65	06/10/2023	500	1,000	2,000	495.9	996.6	2008.4	0.995x + 3.124	1.000
H-R03	Dwyer	VFB-65	04/10/2023	500	1,000	2,000	504.3	990.1	1969.6	0.987x + 9.890	1.000
H-R04	Dwyer	VFB-65	02/10/2023	500	1,000	2,000	496.9	986.1	2006.2	1.004x - 15.756	0.999
H-R05	Dwyer	VFB-65	03/10/2023	500	1,000	2,000	503.1	991.3	2014.3	1.000x - 1.636	1.000
H-R06	Dwyer	VFB-65	05/10/2023	500	1,000	2,000	499.2	997.2	1974.6	0.994x + 3.462	0.999



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com



CERTIFICATE No : 23M2441
REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA 05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.
CALIBRATION DATE : 10-Mar-23

APPROVED BY

ISSUED DATE : 16-Mar-23
RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar ± 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23° C ± 1° C RELATIVE HUMIDITY : 49 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR

POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY

COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**SITHIPHORN ASSOCIATES CO.,LTD.
CALIBRATION LABORATORY**

451-451/1 Sirinthorn Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com <http://www.sithiphorn.com>

NSC-TISI-TIS 17025
CALIBRATION 0394

Cert. No. : SP23016

Pages 1 of 3

Calibration Certificate

Equipment : UV-VIS SPECTROPHOTOMETER
Manufacturer : PERKINELMER
Model : LAMBDA 25
Serial No.: 501S14123010
ID No.: SP03/58
Calibration Mode : WAVELENGTH ACCURACY
PHOTOMETRIC ACCURACY
Condition As Found : GOOD
Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,
CHOMPHON, CHATUCHAK,
BANGKOK 10900, THAILAND.
Location : ORGANIC LABORATORY IV
Ambient Temperature : (25.0 ± 5) °C
Relative Humidity : (48.4 ± 25) %
Received Date : 30 AUGUST 2023
Calibration Date : 30 AUGUST 2023
Date of Issue : 31 AUGUST 2023

Calibrated by :

Approved by :

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Continuation of Calibration Certificate

Cert. No. : SP23016
Job No. : VC66SP0014
Pages : 2 of 3

Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01
The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution
The calibration procedure used was based on ASTM E275-01, ASTM E925-02

Condition of this result of calibration :

1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	106864	01/11/2024
Didymium liquid	RM-DL	28912	106905	02/11/2024
Neutral density filter	RM-1N2N3N	13877	106918	03/11/2024
Potassium dichromate solutions	RM-0204060810	14204	106902	02/11/2024
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology, NIST.

Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.3	0.05	0.16	2.00
	467.82	468.0	0.18	0.16	2.00
	536.56	536.6	0.04	0.16	2.00
	640.50	640.4	-0.10	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.0	0.06	0.16	2.00

UUC* = Unit Under Calibration

Continuation of Calibration Certificate

Cert. No. : SP23016
Job No. : VC66SP0014
Pages : 3 of 3

Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0517	1.0564	0.0047	0.0031	2.00
		29914	0.7	0.7445	0.7460	0.0015	0.0032	2.00
		29381	0.5	0.5416	0.5429	0.0013	0.0032	2.00
	546.1	29360	1.0	0.9821	0.9849	0.0028	0.0030	2.00
		29914	0.7	0.6961	0.6961	0.0000	0.0030	2.00
		29381	0.5	0.5073	0.5073	0.0000	0.0030	2.00
	590.0	29360	1.0	1.0222	1.0244	0.0022	0.0030	2.00
		29914	0.7	0.7237	0.7234	-0.0003	0.0030	2.00
		29381	0.5	0.5361	0.5360	-0.0001	0.0031	2.00
	635.0	29360	1.0	0.9753	0.9775	0.0022	0.0030	2.00
		29914	0.7	0.6910	0.6910	0.0000	0.0030	2.00
		29381	0.5	0.5211	0.5210	-0.0001	0.0032	2.00
RM-0204060810	235.0	20		0.2422	0.2462	0.0040	0.0101	2.00
		40		0.4866	0.4900	0.0034	0.0115	2.00
		60		0.7414	0.7390	-0.0024	0.0068	2.00
		80		0.9858	0.9871	0.0013	0.0093	2.00
		100		1.2442	1.2480	0.0038	0.0087	2.00

UUC* = Unit Under Calibration

Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230

Resolution of Wavelength Mode 0.1 nm

Resolution of Photometric Mode 0.0001 A

Parameter Setting

Measurement Mode Wavelength, Absorbance

Wavelength Scan 1100 nm-190 nm

Scanning Speed 7.5 nm/min

Data Pitch 0.1 nm

Band width(Wavelength) 1.0 nm

Band width(Vis) 1.0 nm

Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transmission T(%)	Absorbance(A)
0.0111	3.9564

**Specific Acceptance :

Transmission ≤ 1.0 T(%), Absorbance ≥ 2.0 A

**Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k ,
providing a level of confidence of approximately 95%

End of Calibration Certificate



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chulachai, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spicon.com, www.spicon.com

Calibration Report			
Non-Dispersive Infrared CO Analyzer			
Date :	13 December 2023	Brand :	API
No.	CO-802	Model :	300E
		Serial No.	965
Calibrator (Dilution System)			
Brand :	API	Model :	700
Last Cal. Date :	08 August 2023	Serial No.	911
Reference Standard Gas			
Standard Gas :	Carbon Monoxide (CO)	Cylinder No. :	D196045
Certified Date :	16 April 2022	Expired Date :	15 April 2024
		Cylinder Conc. :	4,570 ppm
Calibrating Condition			
Pressure	1011 mmbar	Temp.	24.5 °C
		% RH	48
Calibration Setting			
Span	Initial Reading (Before Adj.), PPM		Final Reading (After Adj.), PPM
Set Point	Expected Concentration	Analyzer Response	%Dif
Zero	0	-0.10	-
CO Span	40.00	39.97	-0.075
			40.00
API Model 300E CO Analyzer Check List			
Parameter	Observed Value	Units	Nominal Range
Range	50	PPM	0-1000 ppm
Stability	0.10	PPM	< 1 ppm With Zero Air
CO Measure	4015.7	mV	2500-4800 mV
CO Reference	3948.5	mV	2500-4800 mV
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air
Sample Pressure	28.4	In-Hg-A	~2" < Ambient Absolute Pressure
Sample Flow	804	CC/Min	800 ± 10%
Sample Temperature	48.2	°C	48 ± 4
Bench Temperature	48.0	°C	48 ± 2
Wheel Temperature	68.5	°C	68 ± 2
Box Temperature	30.9	°C	Ambient Temp + 7 ± 10
Photo-Drive	3038.1	mV	250 mV to 4750 mV
Slope	1.017	-	1.0 ± 0.3
Offset	0.2	-	0 ± 0.3

ระดับเสียง



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N 4106495.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 27 Mar. 2023

Date of Calibration : 29 Mar. 2023

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa , Corrected to Reference Conditions : 101.325 kPa , 23.0 $^\circ\text{C}$ and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.94	-0.06	± 0.10	$\pm 0.40 \text{ dB}$

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The information on actual reading was not attached.

Date of Calibration : 29 Mar. 2023

Date of Issue : 30 Mar. 2023

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Noise R_735/23

Sound Level Meter Calibration Report

Acoustic Calibrator Data						
Brand	ACO			Number	AC 03/56	
Model	2127			Serial No.	130006	
Calibration Range	94 dB, 1000 Hz			Last Calibration	29 March 2023	
				Due Date	29 March 2024	
Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R08	ACO	6236	00152082	17 December 2023	94.0	94.0
ACO-R09	ACO	6236	00172035	17 December 2023	94.1	94.0
ACO-R10	ACO	6236	00172037	17 December 2023	94.0	94.0
ACO-R11	ACO	6236	00172038	17 December 2023	94.0	94.0
ACO-R20	ACO	6236	00182003	17 December 2023	94.1	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.94 ± 0.10 dB	



คุณภาพน้ำ



Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A.D
968 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel. +662 637 6363
Fax: +662 632 4334
Email: ccc-smt@agilent.com
Website: www.agilent.com/chem

Service Confirmation Number: 6904837529

Service Confirmation Date: 06.04.2023

Customer Contact:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan
TAX ID : 0105540004859
bounced-imchom.chanattagarn@alsglobal.com
227158760519

Invoice To:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Delivery Site:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Location:

Room
Bldg
Lab
Dept

SERVICE REPORT

Customer Purchase Order Number:	Customer Number: 70371013
Service Request:	Service Request Date:
Service Order: 6006068207	Service Confirmation: 6904837529

**Direct Inquiries to:**

Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

[products](#) | [applications](#) | [software](#) | [services](#)

Learn more about Agilent's Special Offers, Products, Services and our
full range of laboratory productivity solutions optimized for your
applications and workflows. Visit us at www.agilent.com/chem

Agilent Technologies (Thailand) Limited, Head Office
U Chu Liang Bldg. 22/F Unit A.D
968 Rama 4 Road, Silom, Bangrak,
Bangkok 10500 Thailand
Tax ID : 0105542068218

Citibank N.A. Bangkok Branch
399 Interchange 21 Building, Sukhumvit Road, Klongtoey Nau
Sub-district, Wattana District, Bangkok 10110 Thailand
Acc. No: 012-4452-007,
THB:Krung Thai Bank PCL
Siam Square Br.,416/1-2 Rama I Rd.,Pathumwan, BKK 10330
Thailand

ORIGINAL

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7900	ICPMS 7900 System			
G8410A	SPS 4 Autosampler	AU15430722	ICP MS 7900	SYS-IM-7900
G8411A	ISIS 3 for Agilent 7850/7900/8900	JP15510227	ICP MS 7900	SYS-IM-7900
G3292A	PSC 6106T Chiller	2U15A1948	ICP MS 7900	SYS-IM-7900
G8403A	Agilent 7900 ICP-MS	JP15471169	ICP MS 7900	SYS-IM-7900

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EOQ	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	06.04.2023	06.04.2023
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement - 100 % covered		

Additional Information:

Service Confirmation Number: 6904837529

Service Confirmation Date: 06.04.2023

Service Information:

Problem Description:
WU-S-OQ-ICP MS 7900-5001143313

Service Provided:
Test OQ control of instrument ICPMS = BKK_EL0043. After done all instrument test all Pass.

Service Overview Code:
Reason Code: Scheduled Service
Diagnosis Code: Scheduled Service
Resolution Code: Scheduled Service

Reported Hours:
6.0

Travel Hours:
1.0

**Customer Field Service
Representative Name:**
Panthep Kurasathain

Customer Name:
Anchalee Khamjan

Additional Comments:



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1517
Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Memmert

Model : UFE 500

Serial No. : G511.1572

ID No. : RYG_EN0010

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T. Maenam Khu,
A. Pluakdaeng,
Rayong 21140 Thailand

Location : Oven Room

Received Order : 20 October 2022

Calibration Date : 20 October 2022

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

() Pornthippa Tameyakul

(/) Malee Butkruea

() Suwit Imjai

Issue Date : 2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2210-0376OC-2

Cert. No.: 22TM1517
 Page : 2 of 3

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY49023932	22LM97	29 Jul 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

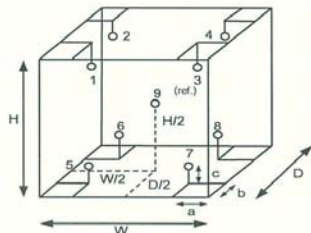

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	54	59
AC Supply (Volt)	223	225

Ref. Std. ID No.: @ Calibration Point

Position :	(180) °C	(104) °C
1	21-16TC-01	20-16RTD-01
2	21-16TC-02	20-16RTD-02
3	21-16TC-03	20-16RTD-03
4	21-16TC-04	20-16RTD-04
5	21-16TC-05	22-16RTD-05
6	21-16TC-06	20-16RTD-06
7	21-16TC-07	20-16RTD-07
8	21-16TC-08	22-16RTD-08
9 (ref.)	21-16TC-09	22-16RTD-09

Probe Installation Details :

a = 5.0 cm	D = 0.40 m
b = 5.0 cm	W = 0.56 m
c = 5.0 cm	H = 0.48 m
	Capacity = 0.11 m³



Equipment : Hot Air Oven
 Condition As-Received : Used Item
 Reference : 2210-0376OC-2

Cert. No.: 22TM1517
 Page : 3 of 3

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
104.0	104.0	104.0	0.076	0.52	0.60	0.42	2
180.0	180.0	180.0	0.13	0.88	1.2	1.1	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.768	103.734	103.723	103.800	104.215	104.131	104.132	103.740	103.747
180.0	179.723	179.359	179.439	179.489	180.361	180.114	180.131	180.243	179.605

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1518
Page : 1 of 3

Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Memmert

Model : UF 110

Serial No. : B416.2420

ID No. : RYG_EN001

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T. Maenam Khu,
A. Pluakdaeng,
Rayong 21140 Thailand

Location : Oven Room

Received Order : 20 October 2022
Calibration Date : 20 October 2022
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

() Pornthippa Tar
(✓) Malee Butkrue
() Suwit Imjai

Issue Date : 2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0046907



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-0376OC-3
Procedure Used :-

Cert. No.: 22TM1518
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY49023932	22LM97	29 Jul 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	54	59
AC Supply (Volt)	223	225

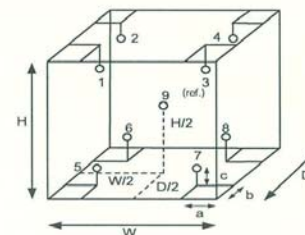

Probe Installation Details :		Dimension of Chamber :	
a =	5.0 cm	D =	0.40 m
b =	5.0 cm	W =	0.56 m
c =	5.0 cm	H =	0.48 m
		Capacity =	0.11 m³

Ref. Std. ID No.: @ Calibration Point		
Position :	(180) °C	(104) °C
1	21-16TC-01	20-16RTD-01
2	21-16TC-02	20-16RTD-02
3	21-16TC-03	20-16RTD-03
4	21-16TC-04	20-16RTD-04
5	21-16TC-05	22-16RTD-05
6	21-16TC-06	20-16RTD-06
7	21-16TC-07	20-16RTD-07
8	21-16TC-08	22-16RTD-08
9 (ref.)	21-16TC-09	22-16RTD-09

a 1132468



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2210-0376OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 22TM1518

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
104.0	104.0	104.0	0.15	0.74	1.1	0.42	2
180.0	180.0	180.0	0.15	1.2	1.8	1.1	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	104.479	103.888	104.462	104.206	103.963	104.129	103.657	104.058	104.287
180.0	180.379	179.934	180.821	179.799	180.592	179.804	179.131	179.543	180.237

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation


UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

a 1132467



Certificate of Calibration

Equipment: SPECTROPHOTOMETER
Model: DR6000
Serial No. (or ID.): 1627845 (RYG_EN0037)
Manufacturer: HACH
Condition: In Condition

Certificate No.: C06220464
Issued Date: 27 September 2022
Job No.: KSPR2212224
Page: 1 of 3

Customer: ALS Laboratory Group (Thailand)
616/10 Moo 5 T.Maenam Khu
A.Pluakdaeng, Rayong 21140

Environment Condition: Temperature 23.1 °C
Humidity 65.4 %RH

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) (Wet Chemistry)
616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr. Chattuphon Foithong

Calibration Date: 27 September 2022

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Sarna Scientific Limited.

The standard for Wavelength Certificate No. 91418 and 91435

The standard for Photometric Certificate No. 91441 and 101088

The standard for Stray light Certificate No. 101041 and 101040

The standard for Spectral resolution Certificate No. 101037

Authorized Signatory

This certificate is issued on the basis of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท เทคโนโลยี ดีเคเอส เอเซีย จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CALFM-C06-13: 20 Jul 2022

Calibration Results:

Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.4	0.21	0.14
536.66	536.7	-0.04	0.14
637.98	638.3	-0.32	0.14
748.48	748.8	-0.32	0.14
807.03	807.4	-0.37	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.5605	0.563	-0.0025	0.0045
	0.7334	0.737	-0.0036	0.0045
	1.0534	1.057	-0.0036	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.5503	0.553	-0.0027	0.0045
	0.7179	0.720	-0.0021	0.0045
	1.0312	1.034	-0.0028	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.5024	0.506	-0.0036	0.0045
	0.6693	0.672	-0.0027	0.0045
	0.9604	0.964	-0.0036	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.5168	0.519	-0.0022	0.0045
	0.6903	0.691	-0.0007	0.0045
	0.9904	0.992	-0.0016	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.5525	0.554	-0.0015	0.0045
	0.7175	0.718	-0.0005	0.0045
	1.0301	1.031	-0.0009	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.5367	0.538	-0.0013	0.0045
	0.6847	0.685	-0.0003	0.0046
	0.9823	0.983	-0.0007	0.0045

Calibration Results:

Without Adjustment

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7423	0.744	-0.0017	0.0083
257 nm	0.0000	0.000	0.0000	0.0080
	0.8609	0.861	-0.0001	0.0084
313 nm	0.0000	0.000	0.0000	0.0080
	0.2895	0.292	-0.0025	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6381	0.638	0.0001	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.67 +/- 0.11 nm	260.7	2.1	1.678
391.94 +/- 0.11 nm	391.9	1.7	1.770

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.60	266.63	1.39	2.00
UUC: Wavelength (nm)	268.2	266.1		
Std Absorbance (A)	0.4810	0.3176		
Absorbance (A)	0.373	0.268		

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate



ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2212224

ชนิดเครื่องมือ: SPECTROPHOTOMETER รุ่น: DR6000

หมายเลขเครื่อง: 1627845

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
27 Sep 2022			27 Sep 2022		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตซ์ ปิด – เปิด เครื่อง (On-Off Swich)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) ≥ 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	656.1 ได้ 656.1 nm
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV $< 3,000$ hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible $< 5,000$ hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันเปื้อน Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (≥ 2.5 ไม่นเกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

เพิ่มเติม/ข้อแนะนำ :

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phraekhonong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-R31-03: 20 Jul 2022



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T231670

Page 1 of 5

Certificate of Calibration

Equipment : HEATING BLOCK

Manufacturer : Environmental Express

Model : B300 240

Serial No. : 2017 CODW115

Customer Code : RYG_EN0142

ID No. : T6770A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)

616/10 Moo 5 T.Maenam Khu,
A.Pluakdaeng, Rayong 21140

Customer Location : Environment Laboratory

Date of Receipt : 13 September 2023

Calibrated By : Sujin Nakrakrod (Site Calibration Manager)

Approved By

Date of Issue

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L12 109/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231670

Page 2 of 5

Calibration Report

Equipment : HEATING BLOCK
Date of Calibration : 19 September 2023
Environment : Temperature : 21.9°C-23.0°C
Line Voltage : 226.1-235.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 29 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN221-TN230	T230546	10 April 2024
TC	TYPE T	TN231-TN240	T230546	10 April 2024
TC	TYPE T	TN261-TN270	T230548	10 April 2024
DATA LOGGER	34970A	T149	T230546	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 18 Minute At 150 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

() without adjustment

(X) after adjustment



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110


Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231670

Page 3 of 5

Calibration Report

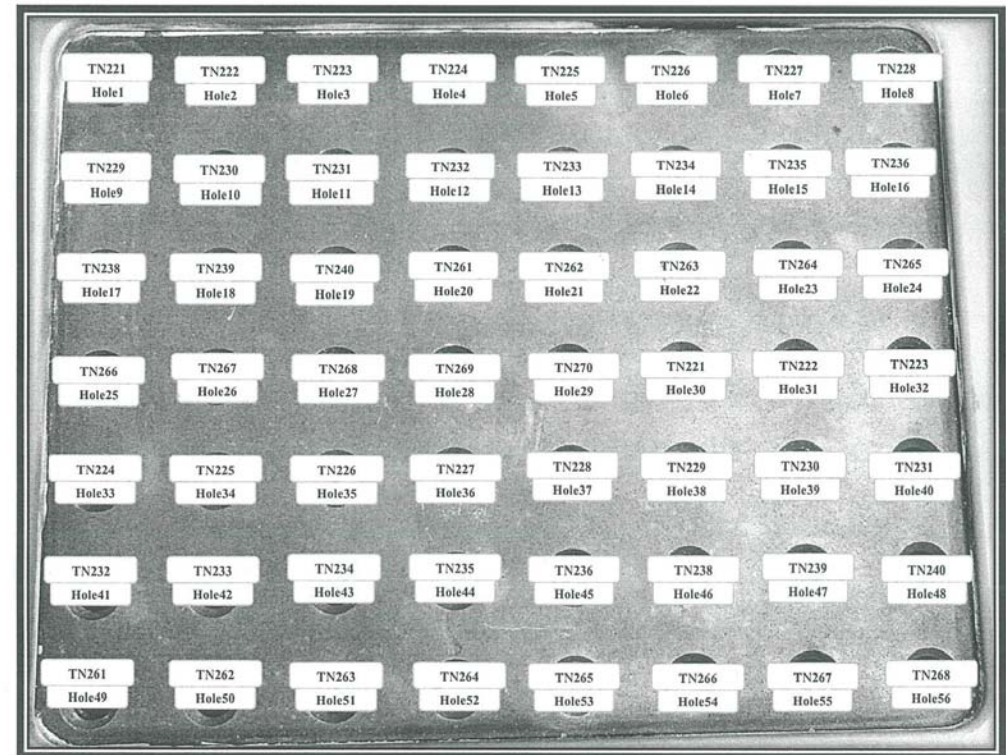

FRONT





Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231670

Page 4 of 5

Calibration Report

Measurement Results

		Average Standard Reading at each position (°C)							
		Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8
Calibration Point		TN221	TN222	TN223	TN224	TN225	TN226	TN227	TN228
CAL POINT	Max	149.65	150.05	149.35	150.43	149.29	149.33	149.62	149.48
150	Min	149.44	149.84	149.14	150.22	149.06	149.04	149.36	149.21
	Average	149.55	149.94	149.25	150.32	149.18	149.19	149.49	149.35
		Hole9	Hole10	Hole11	Hole12	Hole13	Hole14	Hole15	Hole16
		TN229	TN230	TN231	TN232	TN233	TN234	TN235	TN236
Max	149.46	150.08	150.08	149.90	149.42	150.34	149.47	149.37	
Min	149.22	149.85	149.88	149.68	149.22	150.10	149.24	149.11	
Average	149.34	149.96	149.98	149.79	149.32	150.22	149.35	149.24	
		Hole17	Hole18	Hole19	Hole20	Hole21	Hole22	Hole23	Hole24
		TN238	TN239	TN240	TN261	TN262	TN263	TN264	TN265
Max	150.84	150.49	149.98	149.28	150.17	150.17	149.30	149.28	
Min	150.61	150.30	149.79	149.10	149.89	149.89	149.07	149.01	
Average	150.72	150.40	149.88	149.19	150.03	150.03	149.18	149.14	
		Hole25	Hole26	Hole27	Hole28	Hole29	Hole30	Hole31	Hole32
		TN266	TN267	TN268	TN269	TN270	TN221	TN222	TN223
Max	150.79	149.49	149.90	150.00	149.90	150.44	150.92	150.55	
Min	150.52	149.24	149.67	149.73	149.60	150.23	150.73	150.36	
Average	150.66	149.36	149.79	149.86	149.75	150.34	150.82	150.45	



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231670

Page 5 of 5

Calibration Report

Measurement Results

		Average Standard Reading at each position (° C)							
		Hole33	Hole34	Hole35	Hole36	Hole37	Hole38	Hole39	Hole40
Calibration Point		TN224	TN225	TN226	TN267	TN228	TN229	TN230	TN231
CAL POINT	Max	150.20	150.35	149.13	150.04	150.45	149.74	150.37	149.58
150	Min	150.22	148.94	148.94	149.85	150.28	149.59	150.24	149.32
	Average	150.21	149.65	149.04	149.94	150.36	149.67	150.31	149.45
		Hole41	Hole42	Hole43	Hole44	Hole45	Hole46	Hole47	Hole48
		TN232	TN233	TN234	TN235	TN236	TN238	TN239	TN240
Max	149.43	149.91	150.74	150.55	150.45	151.17	150.84	149.59	
Min	149.25	149.70	150.54	150.39	150.29	151.01	150.70	149.45	
Average	149.34	149.80	150.64	150.47	150.37	151.09	150.77	149.52	
		Hole49	Hole50	Hole51	Hole52	Hole53	Hole54	Hole55	Hole56
		TN261	TN262	TN263	TN264	TN265	TN266	TN267	TN268
Max	149.38	150.01	151.00	150.99	150.00	151.04	150.46	149.27	
Min	149.22	149.83	150.85	150.79	149.84	150.89	150.30	149.13	
Average	149.30	149.92	150.93	150.89	149.92	150.97	150.38	149.20	

HEATING BLOCK				Temperature Distribution	
Setting (° C)	Reading (°C)		Stability (± ° C)	Uncertainty (± ° C)	
	Min , Max	Average			
150.0	149.9 , 150.1		0.16	0.97	

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied

a level of confidence of approximately 95 % .

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com



Certificate of Calibration

Model Number : MCE224S-2S00-U
Description : Analytical Balance
Serial Number : 0038101399
ID No. : RYG_EN0163
Manufacturer : Sartorius

Certificate No. : [REDACTED]
Issued Date : Friday, March 03, 2023
Reference No. : 204833
Page No. : 1 of 2

Customer Name : ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd. (Balance Room)
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated By : Mr.Chonchai Inthana
Calibration Date : Wednesday, March 01, 2023

Calibration Procedure No. : This calibration was conducted by
Using in-house calibration procedure number (WI-003)
Based on UKAS LAB 14 : 2019

Metrological data :
Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:
Temperature : 24.2 °C ± 5.0 °C
Humidity : 60.0 % RH ± 10.0 % RH
Pressure : ±

Reasons for calibration
☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance

Equipment Condition: ☒ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

SARTORIUS

Certificate of Calibration

Model Number : MCE224S-2S00-U
Description : Analytical Balance
Serial Number : 0038101399
ID No. : RYG_EN0163
Manufacturer : Sartorius

Certificate No. : 23BCI0111
Issued Date : Friday, March 03, 2023
Reference No. : 204833
Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability

The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0000
	20.0000	199.9999
Nominal Value : (High Load)	20.0001	200.0000
200 g	20.0000	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0001	200.0001
	20.0000	200.0000
Standard Deviation		0.00004 0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).


Nominal value :	100	g
Tolerance	0.0004	g
	Difference	
	1	-
	2	0.0001
	3	0.0000
	4	-0.0001
	5	-0.0001
	6	-

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance		0.0002 g			
Nominal Value	Conventional Mass Value	Displayed Value	Deviation	Uncertainty	
(g)	(g)	(g)	(g)	(g)	
0.01	0.0100	0.0100	0.0000	0.00012	
0.05	0.0500	0.0500	0.0000	0.00012	
0.1	0.1000	0.1000	0.0000	0.00012	
0.5	0.5000	0.5000	0.0000	0.00012	
1	1.0000	1.0000	0.0000	0.00012	
5	5.0000	5.0000	0.0000	0.00013	
10	10.0000	10.0000	0.0000	0.00013	
20	20.0000	20.0000	0.0000	0.00024	
50	50.0000	50.0000	0.0000	0.00014	
100	100.0000	100.0000	0.0000	0.00018	
200	200.0000	200.0000	0.0000	0.00032	

End of Report.



Certificate of Calibration

Equipment: SPECTROPHOTOMETER
Model: DR3900
Serial No. (or ID.): 2021761 (RYG_EN0179)
Manufacturer: HACH
Condition: In Condition

Certificate No.: C06230442
Issued Date: 22 September 2023
Job No.: WO-00005382
Page: 1 of 3

Customer: ALS Laboratory Group (Thailand) Co., Ltd.
 616/10 Moo 5 T.Maenam Khu,
 A.Pluakdaeng, Rayong 21140, Thailand.

Environment Condition: Temperature 24.1 °C ±
 Humidity 61.6 %RH ±

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch) (Wet Chemistry)
 616/10 Moo 5 T.Maenam Khu,
 A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr.Nattapat Rungueang
Calibration Date: 18 September 2023
The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04
Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Sarna Scientific Limited.

The standard for Wavelength Certificate No. 111583 and 111584
 The standard for Photometric Certificate No. 9114984
 The standard for Stray light Certificate No. 111585

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีซี จำกัด
 DKSH Technology Limited
 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
 2533 Sukhumvit Road, Bangchak, Phra Khanong, Bangkok 10260
 Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 5 nm and UUC at 5 nm				
Standard Wavelength	Unit Under Calibration	Correction	Uncertainty	
418.40	418	0.40	0.59	
537.00	536	1.00	0.59	
638.00	638	0.00	0.59	
747.61	748	-0.39	0.59	
807.04	807	0.04	0.59	

Photometric Accuracy (Absorbance)				
Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2930	0.289	0.0040	0.0045
	0.5168	0.517	-0.0002	0.0045
	1.0298	1.026	0.0038	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2867	0.281	0.0057	0.0045
	0.5073	0.506	0.0013	0.0045
	1.0083	1.003	0.0053	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2516	0.249	0.0026	0.0045
	0.4595	0.461	-0.0015	0.0045
	0.9334	0.933	0.0004	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2461	0.244	0.0021	0.0045
	0.4652	0.466	-0.0008	0.0045
	0.9468	0.945	0.0018	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2594	0.257	0.0024	0.0045
	0.5040	0.504	0.0000	0.0045
	1.0032	1.000	0.0032	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2579	0.256	0.0019	0.0045
	0.4971	0.497	0.0001	0.0045
	0.9720	0.970	0.0020	0.0045

บริษัท ดีเคเอส อีซี จำกัด
 DKSH Technology Limited
 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
 2533 Sukhumvit Road, Bangchak, Phra Khanong, Bangkok 10260
 Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:
Without Adjustment

Stray light *	Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
	391.44 +/- 0.11 nm	391	3.6	1.444

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00005382

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: DR3900

หมายเลขเครื่อง: 2021761

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
18 Sep 2023			18 Sep 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด - เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	807nm=807.3nm
<input type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่นเกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

เพิ่มเติม/ข้อแนะนำ :

คุณภาพอากาศในการทำงาน



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data									
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve		
					Setting			Actual (Q std.)					
					1	2	3	1	2	3	y	R ²	
R01	SKC	224-PCXR4	602467	02/10/2023	1,000	1,500	2,000	1,001	1,499	1,999	1.010x - 22.581	0.999	
R02	SKC	224-PCXR4	626450	06/10/2023	1,000	2,000	3,000	996	1,493	1,986	0.992x + 3.742	1.000	
R03	SKC	224-PCXR4	691592	06/10/2023	1,000	1,500	2,000	989	1,495	1,994	0.999x - 6.866	1.000	
R04	SKC	224-PCXR4	691672	06/10/2023	1,000	1,500	2,000	998	1,491	1,989	0.991x + 5.421	1.000	
R05	SKC	224-PCXR4	798470	06/10/2023	1,000	1,500	2,000	999	1,495	1,995	1.005x - 18.995	0.999	
R06	SKC	224-PCXR4	798456	02/10/2023	1,000	1,500	2,000	1,000	1,488	1,987	0.986x + 13.398	1.000	
R07	SKC	224-PCXR4	798480	02/10/2023	1,000	1,500	2,000	1,000	1,497	1,998	1.009x - 21.689	0.999	
R08	SKC	224-PCXR4	883215	05/10/2023	1,000	1,500	2,000	994	1,500	1,990	0.995x + 3.109	1.000	
R09	SKC	224-PCXR4	034650	05/10/2023	1,000	1,500	2,000	999	1,497	1,996	1.008x - 21.526	0.999	
R10	SKC	224-PCXR4	091765	05/10/2023	1,000	1,500	2,000	996	1,493	1,994	1.000x - 6.596	1.000	
R11	SKC	224-PCXR4	091763	04/10/2023	1,000	1,500	2,000	998	1,496	1,983	0.998x - 9.346	0.999	
R12	SKC	224-PCXR4	091568	04/10/2023	1,000	1,500	2,000	1,000	1,497	1,999	1.009x - 21.948	0.999	
R13	SKC	224-PCXR4	091638	02/10/2023	1,000	1,500	2,000	994	1,495	1,986	0.993x + 2.981	1.000	
R14	SKC	224-PCXR4	091764	06/10/2023	1,000	1,500	2,000	998	1,498	2,000	1.012x - 26.788	0.999	
R15	SKC	224-PCXR8	529457	06/10/2023	1,000	1,500	2,000	995	1,492	1,987	0.994x + 1.457	1.000	
R16	SKC	224-PCXR8	529643	04/10/2023	1,000	1,500	2,000	1,000	1,498	1,997	1.007x - 17.908	0.999	
R17	SKC	224-PCXR8	529645	07/10/2023	1,000	1,500	2,000	998	1,496	1,998	1.011x - 25.546	0.999	
R18	SKC	224-PCXR8	566756	03/10/2023	1,000	1,500	2,000	994	1,490	1,989	0.995x - 1.759	1.000	
R19	SKC	224-PCXR8	566802	02/10/2023	1,000	1,500	2,000	1,000	1,496	1,999	1.010x - 22.864	0.999	
R20	SKC	224-PCXR8	529089	06/10/2023	1,000	1,500	2,000	992	1,506	1,996	1.008x - 22.151	0.999	
R21	SKC	224-PCXR8	665728	02/10/2023	1,000	1,500	2,000	992	1,486	1,994	1.002x - 11.842	1.000	
R22	SKC	224-PCXR8	707444	03/10/2023	1,000	1,500	2,000	1,001	1,500	1,999	1.007x - 18.171	0.999	
R23	SKC	224-PCXR8	761067	06/10/2023	1,000	1,500	2,000	1,000	1,488	1,993	0.992x + 5.744	1.000	
R24	SKC	224-PCXR8	707893	05/10/2023	1,000	1,500	2,000	994	1,505	1,996	1.005x - 15.010	0.999	
R25	SKC	224-PCXR8	761052	06/10/2023	1,000	1,500	2,000	999	1,495	1,989	0.991x + 5.640	1.000	
R26	SKC	224-PCXR8	707956	07/10/2023	1,000	1,500	2,000	1,010	1,497	2,002	0.999x - 2.874	0.999	
R27	SKC	224-PCXR8	707398	07/10/2023	1,000	1,500	2,000	1,001	1,496	1,997	1.008x - 20.237	0.999	
R28	SKC	224-PCXR8	707481	07/10/2023	1,000	1,500	2,000	993	1,506	1,995	1.002x - 10.719	1.000	
R29	SKC	224-PCXR8	707402	04/10/2023	1,000	1,500	2,000	995	1,495	1,989	0.995x + 1.091	1.000	
R30	SKC	224-PCXR8	093811	04/10/2023	1,000	1,500	2,000	998	1,495	1,992	0.997x - 0.693	1.000	
R31	SKC	224-PCXR8	093183	06/10/2023	1,000	1,500	2,000	999	1,502	1,997	0.988x + 9.127	0.999	
R32	SKC	224-PCXR8	671950	07/10/2023	1,000	1,500	2,000	998	1,495	1,994	0.998x - 3.451	1.000	
R33	SKC	224-PCXR4	626254	07/10/2023	1,000	1,500	2,000	992	1,503	1,995	1.011x - 30.016	0.999	
R34	SKC	224-PCXR4	626131	03/10/2023	1,000	1,500	2,000	990	1,499	1,997	1.014x - 32.986	0.999	
R35	SKC	224-PCXR8	707460	07/10/2023	1,000	1,500	2,000	990	1,501	1,997	1.005x - 15.898	1.000	
R36	SKC	224-PCXR8	707446	05/10/2023	1,000	1,500	2,000	1,000	1,497	1,997	1.002x - 7.547	1.000	
R37	SKC	224-PCXR8	707432	02/10/2023	1,000	1,500	2,000	995	1,498	1,995	0.999x - 4.856	1.000	



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-R01	Dwyer	VFB-65	02/10/2023	500	1,000	2,000	502.9	994.2	1977.4	1.003x - 7.740	0.999
H-R02	Dwyer	VFB-65	06/10/2023	500	1,000	2,000	495.9	996.6	2008.4	0.995x + 3.124	1.000
H-R03	Dwyer	VFB-65	04/10/2023	500	1,000	2,000	504.3	990.1	1969.6	0.987x + 9.890	1.000
H-R04	Dwyer	VFB-65	02/10/2023	500	1,000	2,000	496.9	986.1	2006.2	1.004x - 15.756	0.999



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-R01	Dwyer	VFA-21	02/10/2023	50	100	200	50.4	98.3	200.4	0.989x + 0.553	1.000
L-R02	Dwyer	VFA-21	06/10/2023	50	100	200	49.3	100.6	199.3	1.002x - 1.123	0.999
L-R03	Dwyer	VFA-21	04/10/2023	50	100	200	50.1	99.3	200.7	1.001x - 0.261	1.000
L-R04	Dwyer	VFA-21	02/10/2023	50	100	200	50.1	100.7	200.6	1.006x - 1.002	0.999



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com



CERTIFICATE No : 23M2441
REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA 05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY :

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23° C \pm 1° C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA. THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

WO-01981290/2023

Customer : S.P.S.Consulting Service Co.,Ltd Date Tested: July 6, 2023
Recommendation Recertification
Address : 7 Soi Phaholyothin 24 Period 6 Months
Paholyothin Road Recertification Due: January 6, 2024
Jompol Chatuchak, Bangkok 1090 Date Last Certified: January 11, 2023
User Name: K.Phenpha Vipphasthawit Visit Number: 1 of 2
Phone: 083-9269252 PerkinElmer Phone: 02-719-6420 ext 206
Fax: 02-513-4221 PerkinElmer Fax: 02-318-5597

CONFIGURATION TESTED

MODEL SERIAL NUMBER
OPTIMA 5300DV 077C7042401

TESTED EQUIPMENT CALIBRATION NUMBER EXPIRATION
IPV Methods

TEST STANDARD USED PART NUMBER EXPIRATION DATE
Multielement Standard N069-1579 October 30, 2023
Wavecal Solution N058-2152 September 30, 2023
VIS Wavecal solution N930-2946 August 30, 2023
Instrument Cal. STD4 N930-0221 November 30, 2023

CUSTOMER SUPPLIED COMMENTS CUSTOMER INITIALS
2 % HNO3
10 % HNO3

Page 1 of 4



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER 077C7042401 **DATE TESTED** July 6, 2023

1. MECHANICAL CHECKS

- A. Inspect and clean all fans and filters. ☐ OK
- B. Inspect and replace as necessary, all torch components including the RF coil. ☐ OK
- C. Inspect all tubing for sign of clacking or leaking. ☐ OK
- D. Adjust water and gas pressure regulator settings. ☐ OK
- E. Inspect and leak check pneumatics drawers. ☐ OK
- F. Clean the exterior of the instrument. ☐ OK

2. OPTICAL CHECKS

- A. Inspect and clean all optical components. ☐ OK
- B. As required, check and replace all purgefilters. ☐ OK
- C. Recheck optical alignment. ☐ OK

3. COOLING SYSTEM CHECKS

- A. Perform preventive maintenance on chiller. ☐ OK
- B. Flush out the chiller every year. ☐ N/A

4. PERFORMANCE CHECKS

- A. Torch View Alignment. ☐ OK
- B. Wavelength Calibration. ☐ OK



MAINTENANCE AND TEST CERTIFICATE MODEL

OPTIMA 5300DV

SERIAL NUMBER : 077C7042401 **DATE TESTED** : July 6, 2023

PARAMETER	SPECIFICATION			FINAL VALUE
Spectral Resolution : UV	As	193.696 nm	≤ 0.007	<u>0.00534</u>
	Ni	231.604 nm	≤ 0.008	<u>0.00682</u>
	Ni	341.476 nm	≤ 0.012	<u>0.00794</u>
Spectral Resolution : VIS	La	408.672 nm	≤ 0.020	<u>0.01613</u>
	Ba	455.403 nm	≤ 0.025	<u>0.02282</u>
Precision	As	193.656 nm	% RSD < 1.0	<u>0.23</u> %
	Zn	213.856 nm	% RSD < 1.0	<u>0.09</u> %
	Mn	257.610 nm	% RSD < 1.0	<u>0.58</u> %
	La	379.478 nm	% RSD < 1.0	<u>0.38</u> %
	Ba	455.403 nm	% RSD < 1.0	<u>0.42</u> %
	Ba	493.408 nm	% RSD < 1.0	<u>0.41</u> %
Detection Limits : Axial	Ti	190.080 nm	3(sd)	<u>2.37</u> ppb
	As	193.696 nm	3(sd)	<u>6.78</u> ppb
	Pb	220.353 nm	3(sd)	<u>0.82</u> ppb
Detection Limits : Radial	As	193.696 nm	3(sd)	<u>23.56</u> ppb
	Zn	213.856 nm	3(sd)	<u>2.85</u> ppb
	Mn	257.610 nm	3(sd)	<u>3.66</u> ppb
	La	379.478 nm	3(sd)	<u>5.10</u> ppb
	Ba	455.403 nm	3(sd)	<u>0.12</u> ppb
	Ba	493.408 nm	3(sd)	<u>1.17</u> ppb
BEC : Axial (IB X 500)/(IS-IB)	Cd	226.502 nm	≤ 150 ppb	<u>117.07</u>
BEC : Radial (IB X 1000)/(IS-IB)	Mn	257.610 nm	≤ 45 ppb	<u>22.09</u>



MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 5300DV

SERIAL NUMBER 077C7042401DATE TESTED July 6, 2023

Remarks :

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,
including warranty terms.

**Certificate of Calibration****Aquion : Anion (ID#894)**

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

S.P.S. Consulting Service Co., Ltd.

ระดับเสียงในการทำงาน



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Keithley 2015-P S/N 4106495.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 27 Mar. 2023

Date of Calibration : 29 Mar. 2023

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa , Corrected to Reference Conditions : 101.325 kPa , 23.0 $^\circ\text{C}$ and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.94	-0.06	± 0.10	$\pm 0.40 \text{ dB}$

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

cluded.

Approved by

Electri

Indust

Date of Calibration : 29 Mar. 2023

Date of Issue : 30 Mar. 2023

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : ssp@spscs.com, www.spscs.com

Noise R_743/23

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	29 March 2023
		Due Date	29 March 2024

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-R25	ACO	6236	00192037	30 December 2023	94.0	94.0
ACO-R28	ACO	6236	00192040	30 December 2023	94.1	94.0
ACO-R30	ACO	6236	00192042	30 December 2023	94.0	94.0



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0639

MTC No. EEL. BP. 39/0866

CALIBRATION CERTIFICATE

Submitted by : S.P.S Consulting Services Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Ambient Environment

Description : Sound Calibrator

Temperature : (23 ± 3) °C

Manufacturer : SVANTEK

Relative Humidity : (50 ± 15) %

Model : SV34

Ambient Pressure : (101.325 ± 1.500) kPa

Serial No. : 33137

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 11 Aug. 2023

Date of Calibration : 22 Aug. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phaholyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0639

MTC No. EEL. BP. 39/0866

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	113.53	-0.47	± 0.10	± 0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	± 1.5	$\pm 2.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.39	± 0.50	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 579-4379-72 Fax : (662) 513-4321 E-mail : sales@spscon.com, www.spscon.com

Noise Dose R_744/23

Noise Dose Meter Calibration Report

Acoustic Calibrator Data

Brand	SVANTEK	Number	SV 01/60
Model	SV34	Serial No.	33137
Calibration Range	114 dB, 1000 Hz	Last Calibration	22 August 2023
		Due Date	22 August 2024

Calibration Data

Sound Level Meter Data				Calibration Data	
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]
					Before Adjustment After Adjustment
NMD-R03	SVANTEK	SV-104IS	60153	20 December 2023	113.5 113.5
NMD-R05	SVANTEK	SV-104IS	60155	20 December 2023	113.6 113.5
NMD-R13	SVANTEK	SV-104IS	63438	20 December 2023	113.5 113.5

Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR) 113.53 \pm 0.10 dB

ระดับความร้อนในการทำงาน



Certificate of Calibration

Certificate Number : SPR23030505-5 Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Metrosonics

Model : hs-32

Serial Number : MCD070035

ID. Number : R05

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C Received Date : 30 Mar 2023
Relative Humidity : 50 % ± 15 % Calibration Date : 31 Mar 2023
Location of Calibration : In-Lab Recommend Due Date : 31 Mar 2024
Calibration Procedure : SP-CPT-04-13 Date of Issue : 01 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be



Calibration Report

Certificate Number : SPR23030505-5 Page : 2 of 3

Reference Standards


Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

Quality Reborn Co., Ltd



Result of Calibration

Certificate No. : SPR23030505-5

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	29.9	-0.113	0.50
35.0	35.010	34.9	-0.110	0.50
40.0	40.015	39.9	-0.115	0.50

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	29.9	-0.113	0.50
35.0	35.010	34.9	-0.110	0.50
40.0	40.015	39.9	-0.115	0.50

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	29.8	-0.213	0.50
35.0	35.010	34.8	-0.210	0.50
40.0	40.015	39.8	-0.215	0.50

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

Heat R120_1

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	R05	Verification Date :	20 December 2023
Brand :	METROSONICS	Ambient Temp. :	24.5 °C
Model :	hs-32	Barometric Pressure :	1011 mmbar
Serial No. :	MCD070035	Relative Humidity :	49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.4	0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			



Certificate of Calibration

Certificate Number : SPR23030505-6 Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 32

Serial Number : TPE080058

ID. Number : R07

Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C Received Date : 30 Mar 2023

Relative Humidity : 50 % ± 15 % Calibration Date : 31 Mar 2023

Location of Calibration : In-Lab Recommend Due Date : 31 Mar 2024

Calibration Procedure : SP-CPT-04-13 Date of Issue : 01 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).



Calibration Report

Certificate Number : SPR23030505-6 Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

Quality Reborn Co., Ltd



Result of Calibration

Certificate No. : SPR23030505-6

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.4	0.387	0.50
35.0	35.010	35.4	0.390	0.50
40.0	40.015	40.4	0.385	0.50

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.3	0.287	0.50
35.0	35.010	35.3	0.290	0.50
40.0	40.015	40.3	0.285	0.50

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.3	0.287	0.50
35.0	35.010	35.3	0.290	0.50
40.0	40.015	40.3	0.285	0.50

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



Heat R120_2

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	R07	Verification Date :	20 December 2023
Brand :	Quest Technologies	Ambient Temp. :	24.5 °C
Model :	QUESTemp 32	Barometric Pressure :	1011 mmbar
Serial No. :	TPE080058	Relative Humidity :	49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.6	-0.1	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			



Certificate of Calibration

Certificate Number : SPR23030505-8 Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment Name : Area Heat Stress Monitor
Manufacturer : Quest Technologies
Model : QUESTemp 32
Serial Number : TPE070001
ID. Number : R12

Environmental Conditions
Ambient Temperature : 23 °C ± 2 °C Received Date : 30 Mar 2023
Relative Humidity : 50 % ± 15 % Calibration Date : 31 Mar 2023
Location of Calibration : In-Lab Recommend Due Date : 31 Mar 2024
Calibration Procedure : SP-CPT-04-13 Date of Issue : 01 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).



Calibration Report

Certificate Number : SPR23030505-8 Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
SP Metrology - SP Metrology system (Thailand) Co.Ltd.
Quality Reborn Co., Ltd



Result of Calibration

Certificate No. : SPR23030505-8

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.0	-0.013	0.50
35.0	35.010	35.0	-0.010	0.50
40.0	40.015	40.0	-0.015	0.50

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.0	-0.013	0.50
35.0	35.010	35.0	-0.010	0.50
40.0	40.015	40.0	-0.015	0.50

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty (±)
30.0	30.013	30.1	0.087	0.50
35.0	35.010	35.1	0.090	0.50
40.0	40.015	40.1	0.085	0.50

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2$, providing a level of confidence approximately 95%.

- End of Certificate -



Heat R120_3

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	R12	Verification Date :	20 December 2023
Brand :	Quest Technologies	Ambient Temp. :	24.5 °C
Model :	QUESTemp 32	Barometric Pressure :	1011 mmbar
Serial No. :	TPE070001	Relative Humidity :	49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.5	0.0	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.2	-0.1	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.3	0.0	± 0.5
UUC* = UNIT UNDER CALIBRATION			