analytikjena
An Endress+Hauser Company

REVIEW BY Orawan T.
APPROVED BY Sawitr N
NEXT CAL. DATE 24/05/24

Maintenance Protocol

Atomic Fluorescence Spectrometer

mercur DUO / mercur DUO plus

analytikjena
An Endress+Hauser Company

Serial-No.: K170A0143 Customer-No.:

Date: 24 May 2023 Carried out by: Srichai Fak-on

Maintenance with following Operational Qualification (OQ) ☐
(requires a separate OQ protocol)

Company	บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด
User	
Department	ห้องแลบปฏิบัติการ
Street	104 ซอย 40 ถนนพัฒนาการ แขวงสวนหลวง เขตสวนหลวง
Zip Code, City	กรุงเทพมหานคร 10250
Country	ประเทศไทย
Phone	
Fax	
E-mail	

Maintenance works basic unit

tightness visual check inside the Mercur	☑
visual check if gold-traps are broken	☑
visual check if spectrometer is contaminated	☑
visual check of the fluorescence cell	☑
visual check of the absorption cell, incl. window	☑
reactor cleaning	☑
check pump-hose, if necessary change it	☑
check swivel drive (SEV)	☑
check drying-hose, output gas-liquid-separator	☑
test Bubble-Sensor	☑
check gas flows	☑
check volume flows, reagents	☑
recording stray light values	☑
measurement with 30 ng/l	☑

Maintenance works Autosampler

Serial No.: 701 739

lubricate the dosing-winding (Teflon-grease-spray)	☑
clean the dosing cylinder, if necessary exchange it	☑
lubricate the winding system of the height drive with some drops of oil	☑
check the toothed belt	☑
check the position of the mechanical stopper (height: 13mm)	☑
check the pump rate of mixing pump (<14s AS52, typ.7s/<20s AS52S, typ.10s)	☑
check the pump rate of washing cup	☑
check the electrical hose connections for good contact	☑
check the connectors of the magnetic valves	☑
check the dosing hose for buckling, if necessary exchange it	☑

Device parameter		nominal value	actual value
visual check general tightness inside the Mercur		o.k.: ☑	changed: ☐
visual check Goldtraps		o.k.: ☑	changed: ☐
visual check spectrometer			
Fluorescence cell		o.k.: ☑	changed: ☐
Absorption cell, incl. window		o.k.: ☑	changed: ☐
lens		o.k.: ☑	changed: ☐
Swivel drive (SEV)		o.k.: ☑	changed: ☐
check pump hoses		o.k.: ☑	changed: ☐
check hoses and hose connectors		o.k.: ☑	changed: ☐
check and clean reactor		o.k.: ☑	changed: ☐
check drying hose output Gas-liquid-seperator		o.k.: ☑	changed: ☐
check bubble-sensor		o.k.: ☑	not o.k.: ☐
Check gasflow			
Argon pressure valve 4		1.2 – 1.5 bar	1.5 bar
Valve 1		10 Nl/h or 0.166 NL/min	0.163 NL/min
Valve 2		50 Nl/h or 0.833 NL/min	0.403 NL/min
Valve 3		5 Nl/h or 0.083 NL/min	0.140 NL/min
Valve 4		10 Nl/h or 0.166 NL/min	0.108 NL/min
Check liquidflow			
Acid		2.5ml/min ± 1 ml	2.5 ml/min
Red.-agent		2.5ml/min ± 1 ml	2.5 ml/min
Sample		10ml/min ± 2 ml	10 ml/min
Adventitious light - values	**(V)**	**from file**	
	100	0	0
	200	0	0
	300	0	0
	350	0	0
	400	0	0
	450	2	2
	500	5	5
	550	10	10
	575	15	14
	600	20	20

Device parameter	nominal value	actual value
Analytical parameters Fluorescence cell		
Conditions.: max.conc.: 10µg/L PMT-voltage: ...360.....V		
Blank-solution		Int ...0.00024...
without enrichment / FBR 30 ng/L	Int > 0.0015 RSD < 3 %	Int_1..0.00172... RSD.0.45.....%
Conditions.: max.conc.: 1.7µg/L PMT-voltage: ...352.....V		
Blank-solution		Int...0.00370.....
with enrichment / FBR 30 ng/L	Int > 0.008 RSD < 3 %	Int_2..0.01060... RSD.2.38.....%
Fok.- factor (Int_2 / Int_1)	> 3.5	6.16
Analytical parameters Absorption cell		
Blank-solution		Ext.0.00093.....
without enrichment / FBR 100 ng/L	Ext. > 0.0012 RSD < 5 %	Ext.0.00449... RSD.2.58.....%
Comments		

Soichai Fakan.

Signature Technician

24 May 2023

Place, Date (DD/MM/YYYY)

Oranan T.

Signature Customer

24 May 2023

Place, Date (DD/MM/YYYY)

analytikjena
An Endress+Hauser Company

35 Moo 5. 345 Road, Khlong Khoi, Pak Kret,
Nonthaburi. 11120 Thailand.
Phone: +66(2) 1062970-72
Fax: +66(2) 1062973
www.analytik-jena.com

Service Report

Customer's address :	Customer's Ref. No.
บริษัท เอเคอเอส แอนอรกาอี กรุ๊ป (ประเทศไทย) จำกัด 104 ซอย 40 ถนนกำนันทม แขวงบางนาใต้ เขตบางนา กรุงเทพมหานคร 10250.	
E-mail :	Phone : / Fax :

☑ Analytik Jena Instruments (Thailand) Ltd.
☐ Analytik Jena Far East (Thailand) Ltd.


Job No. 2305282 PM.	User :	Service Engineer : [illegible]	Date : 24/5/2023	Page : 1/1
Instrument model : Mercur	Serial No. K170A0143		Software Version No. 4.7.10.0	

☐ Repair (RE) ☑ Maintenance (PM) ☐ Installation (IN) ☐ Warranty ☐ Application (AP) ☐ Site Prep.(SP) ☐ Visit(VI)

Fault / Claim : - ทำการเปลี่ยน Pump ตามใบสั่งซื้อเลขที่ Po. No. 23001112 / (INV2305-037) ☐☐☐ Error Code
- ทำตามการ PM Contract Year 2023 (1 Time / Year 2023)

Action taken :
- Maintenance Work Basic Unit
- Check Device parameter.
- Check gas flow.
- Check liquid flow.
- Check Adventitious light - Values

Test run Analytical parameter Fluorescence cell
Test run Analytical parameter Absorption cell

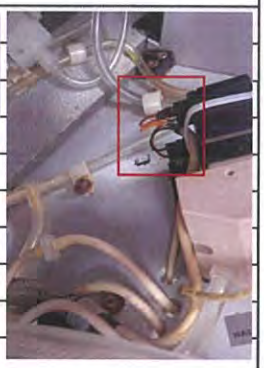การเปลี่ยนปั๊ม



Action Pending / Recommendation : เครื่องทำงานปกติดี



การเปลี่ยนตามรอบ Valve Bubber sensor.

☐ Spare Part ☐ Instrument Configuration :

Item No.	Name	Quantity	Unit Price
1.			
2.			
3.			
4.			
5.			
6.			
7.			
8.			

Herewith the undersigned confirm the time devoted, the work performed, the perfect function of the device, and the receipt/delivery of the specified spare parts. *Traveled hours and kilometers can only be entered after the return of the service engineer.	Date / Signature of Customer Orawan T.	Date / Signature of Service Engineer	Work completed? ☑ Yes ☐ No

Services are subject to the General Terms and Conditions of Analytik Jena AG, which will be sent on request.

Mercur

Report file:	C:\WinAAS\TMP\2023\May\Pro_032			
Program version:	4.7.10.0	Printed on:	5/24/2023	12:46
		Recording started on	5/24/2023	12:35 GMT+7.0
Operator:	PSU,OTA			
Laboratory:	ALS-BKK			
Code:	II_Hg095_2023			

Remarks:

Food,water

Method parameters Hg

Method	Without enrichment / FBR 30ng/L_PM24052023		
Created on	5/24/2023 Time 12:27		
Program	---		

Parameters Mercur Technique: Hg fluorescence

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	30 s
PMT	360 V		
AZ time	5 s	Peak smoothing	8/5
Delay	0 s		

Working mode	w/o enrich.	System cleaning	Acid
FBR technique	on	Wash time acid	10 s
Pump speed	3	Soaking time	20 s
Sample load time	10 s	Gas load time	5 NL/h
Reaction time	10 s		
Waiting time AZ	5 s		
Delay	0 s		
Purge time1	28 s		
Purge time2	15 s	Gas wash time2	10 NL/h

Autosampler

Autosampler	AS51S/F	Tray type	87/139
Working mode	continuous		
Dilution	---		

QC parameters

QC type	Conc. check		
QC check samp. 1	---	QC check samp. 2	---
Conc.	---	Conc.	---
Error limit	---	Error limit	---
Rep. measurement	off	Reaction	flag + continue
QC std.1 no.	1(30.000 ng/L)	QC std.2 no.	1(30.000 ng/L)
QC std.1 limit	± 50.00%	QC std.2 limit	± 50.00%
QC std. act.	flag + continue		
Expect. blank abs.	0.0100± 0.0100	Reaction	flag + continue
QC precision	off		
		Reaction	off
		QC Recal.factor	Off

Calibration settings

Calib. meth	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	Mean	Meas. cycles	2
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		

Calibration standards

Hg


No	Name	State	Pos	Conc./ ng/L	Ints	SD	RSD/%
1	Cal-Zero	(--)	79	0.000	H: **0.000249** A: 0.004274	**0.000132** 0.001698	**53.13** 39.72
2	Cal-Std1	(--)	80	30.000	H: **0.001720** A: 0.02172	**0.000007** 0.000023	**0.459** 0.107

Calibration function 1 **5/24/2023 12:44 Calibration (Peak height)**

Ints=k1+k2*conc

k1=0.000249 k2=0.000049 Recal. factor: ---

Slope	0.00005 Ints/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L		
Lower limit	0 ng/L	Upper limit	33.0 ng/L
Detection limit	---	Deter. limit	---

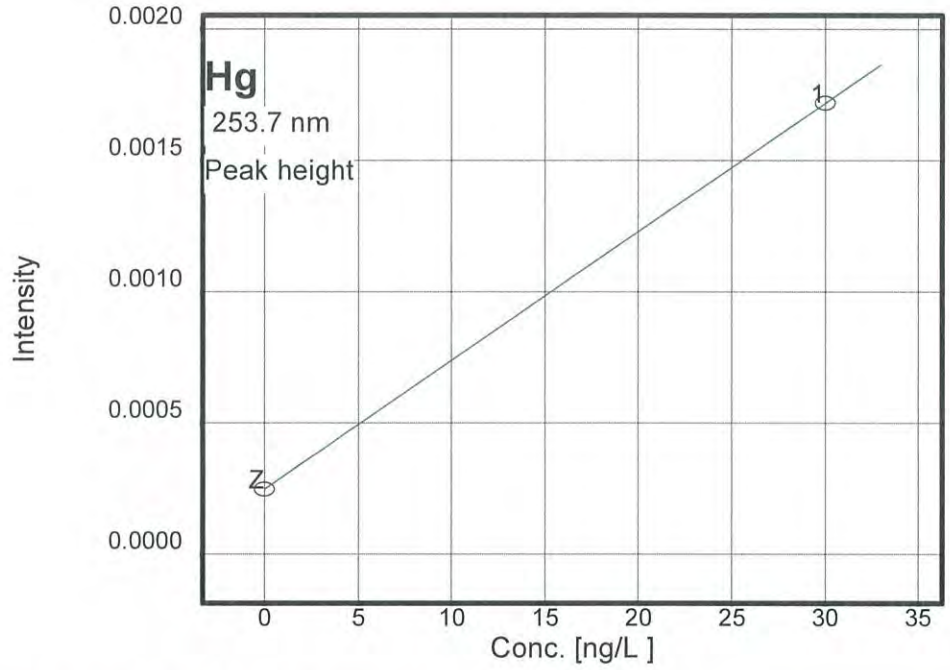



Measurements and events (sorted by time)

Hg	Without enrichment / FBR 30ng/L_PM 24052023					5/24/2023	12:35
ID	**Conc.**	**Ints**	**BG**	**SD**	**RSD/%**	**Int. type**	**Time**
Cal-Zero		0.000143				PkH	12:37
		0.000397					12:38
		0.000207					12:40
	0ng/L	0.000249		0.0001324	53.13		12:40
Cal-Std1		0.001720				PkH	12:42
		0.001712					12:43
		0.001728					12:44
	30.00ng/L	0.001720		0.000007897	0.459		12:44
Calibration	Calibration function: 01						12:44

Peak plots

Hg

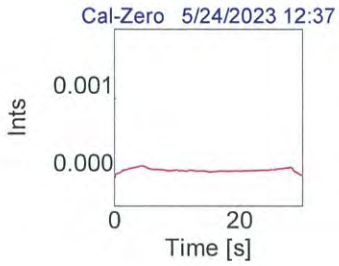

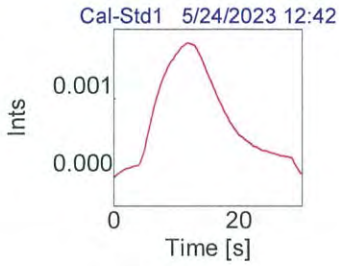

Mercur

Report file:	C:\WinAAS\TMP\2023\May\Pro_033			
Program version:	4.7.10.0	Printed on:	5/24/2023	14:01
		Recording started on	5/24/2023	13:37 GMT+7.0
Operator:	PSU,OTA			
Laboratory:	ALS-BKK			
Code:	II_Hg095_2023			

Remarks:

Food,water

Method parameters Hg

Method	Enrichment / FER 30ng/L PM_24052023		
Created on	5/24/2023 Time 13:36		
Program	---		

Parameters Mercur Technique: Hg fluorescence

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	40 s
PMT	352 V		
AZ time	5 s	Peak smoothing	12/11
Delay	0 s		

Working mode	Enr. w/o reload.	System cleaning	Off
FBR technique	off	Wash time acid	10 s
Pump speed	3	Soaking time	20 s
Sample load time	10 s	Gas load time	10 NL/h
Reaction time	10 s		
Waiting time AZ	10 s	Gas AZ wait	10 NL/h
Purge time1	30 s		
Purge time2	15 s	Gas wash time2	5 NL/h
Purge time3	20 s		
Heat.time coll.1	20 s	Cool. time coll.1	30 s

QC parameters

QC type	Conc. check		
QC check samp. 1	---	QC check samp. 2	---
Conc.	---	Conc.	---
Error limit	---	Error limit	---
Rep. measurement	off	Reaction	flag + continue
QC std.1 no.	1(30.000 ng/L)	QC std.2 no.	1(30.000 ng/L)
QC std.1 limit	± 50.00%	QC std.2 limit	± 50.00%
QC std. act.	flag + continue		
Expect. blank abs.	0.0100± 0.0100	Reaction	flag + continue
QC precision	off		
		Reaction	off
		QC Recal.factor	Off

Calibration settings

Calib. meth	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	off	Meas. cycles	1
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		

Calibration standards

Hg


No	Name	State	Pos	Conc./ ng/L	Ints	SD	RSD/%
1	Cal-Zero	(--)	##	0.000	H: **0.003700** A: 0.02531	**0.000081** 0.000153	**2.192** 0.607
2	Cal-Std1	(--)	##	30.000	H: **0.01060** A: 0.06689	**0.000253** 0.002766	**2.386** 4.136

Calibration function 1 **5/24/2023 14:00 Calibration (Peak height)**

Ints=k1+k2*conc

k1=0.003700 k2=0.000230 Recal. factor: ---

Slope	0.00023 Ints/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L		
Lower limit	0 ng/L	Upper limit	33.0 ng/L
Detection limit	---	Deter. limit	---

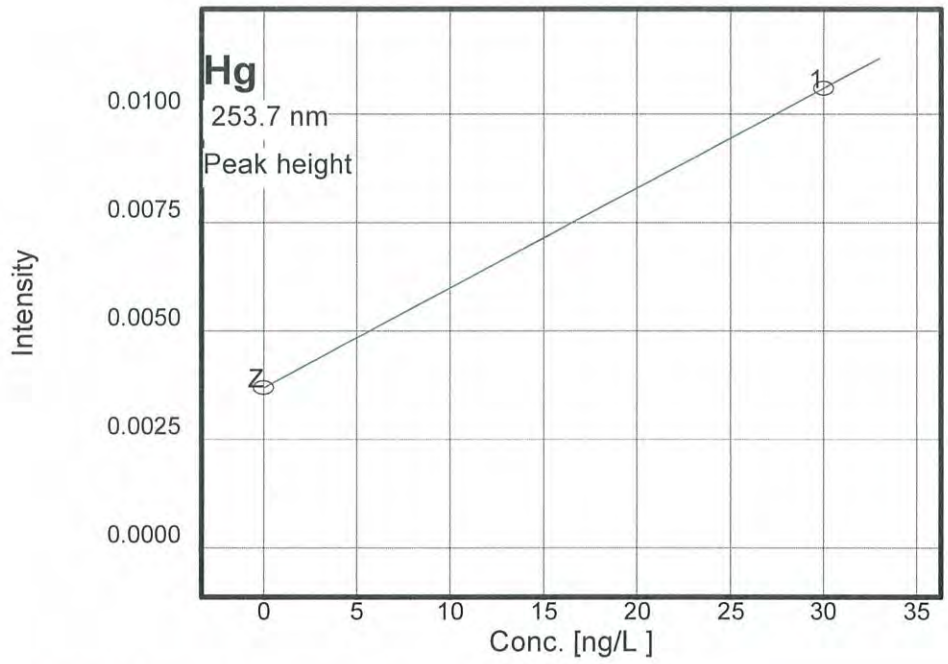



Measurements and events (sorted by time)


Hg	Enrichment / FER 30ng/L PM_24052023					5/24/2023	13:37
ID	**Conc.**	**Ints**	**BG**	**SD**	**RSD/%**	**Int. type**	**Time**
Cal-Zero		0.003792				PkH	13:41
		0.003666					13:43
		0.003640					13:44
	0ng/L	0.003700		0.000081090	2.192		13:44
Cal-Std1		0.009498				PkH	13:49
		0.008333					13:50
		0.008961					13:52
	30.00ng/L	0.008931		0.0005830	6.528		13:52
Cal-Std1		0.01031				PkH	13:57
		0.01074					13:58
		0.01076					14:00
	30.00ng/L	0.01060		0.0002530	2.386		14:00
Calibration	Calibration function: 01						14:00

Peak plots

Hg

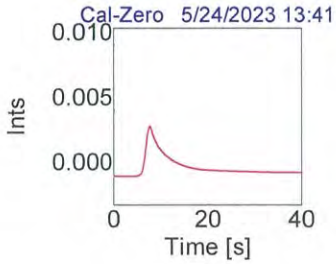

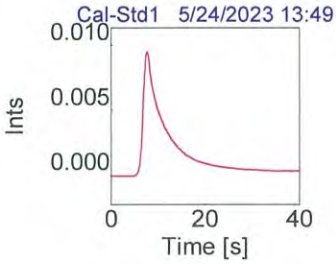

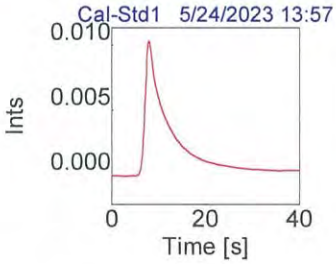

Mercur

Report file:	C:\WinAAS\TMP\2023\May\Pro_034		
Program version:	4.7.10.0	Printed on:	5/24/2023 14:33
		Recording started on	5/24/2023 14:19 GMT+7.0
Operator:	PSU,OTA		
Laboratory:	ALS-BKK		
Code:	II_Hg095_2023		

Remarks:

Food,water

Method parameters — Hg

Method	Without enrichment / Abs / FBR 100ng/L_PM 24052023
Created on	5/24/2023 Time 14:18
Program	---

Parameters Mercur Technique: Hg absorption

Line	253.7 nm		
Lamp type	Hg-LP		
Integr. mode	Peak height	Integr. time	55 s
PMT	225 V		
AZ time	5 s	Peak smoothing	2/5
Delay	8 s		

Working mode	w/o enrich.	System cleaning	Acid
FBR technique	on	Wash time acid	15 s
Pump speed	4	Soaking time	20 s
Sample load time	8 s	Gas load time	5 NL/h
Reaction time	12 s		
Waiting time AZ	15 s		
Delay	10 s		
Purge time1	50 s		
Purge time2	10 s	Gas wash time2	10 NL/h

QC parameters

QC type	Conc. check		
QC check samp. 1	---	QC check samp. 2	---
Conc.	---	Conc.	---
Error limit	---	Error limit	---
Rep. measurement	off	Reaction	flag + continue
QC std.1 no.	1(100.00 ng/L)	QC std.2 no.	1(100.00 ng/L)
QC std.1 limit	± 50.00%	QC std.2 limit	± 0.00%
QC std. act.	flag + continue		
Expect. blank abs.	0.0100± 0.0100	Reaction	flag + continue
QC precision	off		
		Reaction	off
		QC Recal.factor	Off

Calibration settings

Calib. meth	Standard calib.	Calibr. unit	ng/L
No. standards	1	Conversion fac.	1000000
Type of standards	---	Standard prep.	Premixed
		Blank correct.	---
		Recalib. std. no.	---
Output unit	µg/L	Conversion fac.	1000
Calib. stat.	Mean	Meas. cycles	3
		Blind cycles	1
Stock sol. 1	---	Stock sol. 2	---
Stock sol. 3	---	Stock sol. 4	---
Type of cal. curve	linear	Intercept	calculated
Weighted cal.	off	Grubbs stat.	off
Check of cal. curve	no outlier test		

Sample statistics

Stat. mode	Mean	Meas. cycles	2
Confid. level	95.4 %	Blind cycles	1
Grubbs stat.	---		

Calibration standards

Hg


No	Name	State	Pos	Conc./ ng/L	Abs	SD	RSD/%
1	Cal-Zero	(--)	##	0.00	H: **0.000932** A: 0.035926	**0.000138** 0.006208	**14.88** 17.28
2	Cal-Std1	(--)	##	100.00	H: **0.004494** A: 0.061286	**0.000116** 0.001275	**2.586** 2.082

Calibration function 1 **5/24/2023 14:33 Calibration (Peak height)**

Abs=k1+k2*conc

k1=0.000932 k2=0.000036 Recal. factor: ---

Slope	0.00004 Abs/(ng/L)	R2-adjusted	1.0000
sc0	1.00000 ng/L	Charact. conc.	122.411 (ng/L)/1%I
Lower limit	0 ng/L	Upper limit	110. ng/L
Detection limit	---	Deter. limit	---

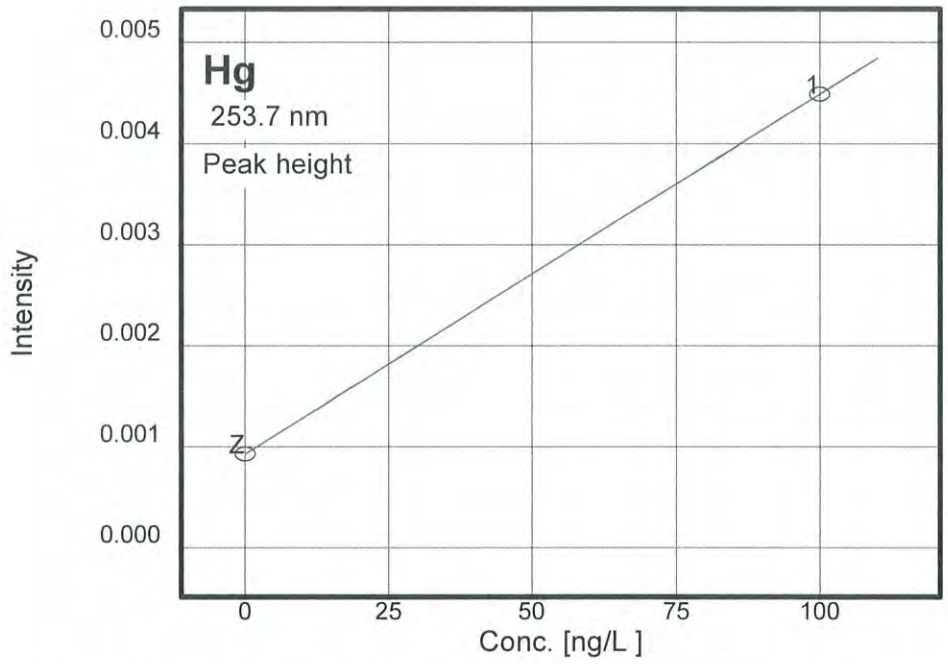



Measurements and events (sorted by time)

Hg	Without enrichment / Abs / FBR 100ng/L_PM 24052023					5/24/2023	14:19
ID	**Conc.**	**Abs**	**BG**	**SD**	**RSD/%**	**Int. type**	**Time**
Cal-Zero		0.001039				PkH	14:22
		0.000775					14:23
		0.000981					14:25
	0ng/L	0.000932		0.00013872	14.88		14:25
Cal-Std1		0.004528				PkH	14:29
		0.004364					14:31
		0.004589					14:33
	100.ng/L	0.004494		0.00011623	2.586		14:33
Calibration	Calibration function: 01						14:33

Peak plots

Hg

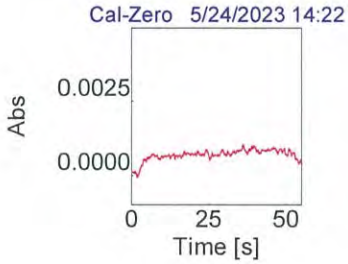

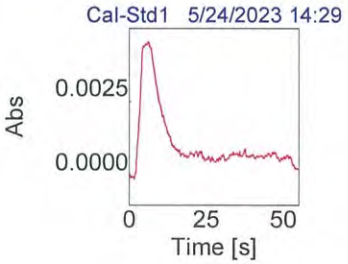

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM1103
Page : 1 of 3

Certificate of Calibration

Equipment :	Autoclave
Manufacturer :	Sanyo
Model :	MLS-3781
Serial No. :	830167
ID No. :	BKK_ML0037
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Media Preparation Room
Received Order :	17 July 2023
Calibration Date :	17 July 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Preecha Hlahib

REVIEW BY Sithichok
APPROVED BY
NEXT CAL. DATE 17/07/25

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul
( ) Malee Butkruea
(✓) Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0053615

Equipment : Autoclave **Cert. No.:** 23TM1103

Condition As-Received : Used Item

Reference : 2307-0285OC-3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.
4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)


It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directry concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

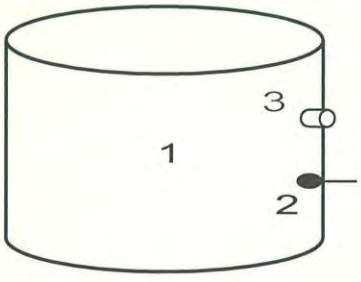

	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	22	53	220
Finished of Calibration	22	54	220

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	22-17TC-01
2 =	Temperature sensor	23-17TC-02
3 =	Exhaust port	19-17TC-03

Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2307-0285OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM1103

Operating parameter Set : Temperature = 121 °C
Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor *k*
121	121	1	120.877	0.39	0.12	1.0	2
		2	120.870				
		3	120.866				

Average* : The average of 30 values in each position.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

Laboratory
Analyzer User


7/12/2023 21:21

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.311
XDISP4	0.616
XDISP10	1.478

Linearity of photometer

L340_	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.001	0.005	-0.004	-394.7
2	0.512	0.519	-0.007	-1.5
3	1.523	1.550	-0.027	-1.8
4	2.027	2.066	-0.039	-1.9
5	2.532	2.582	-0.050	-2.0

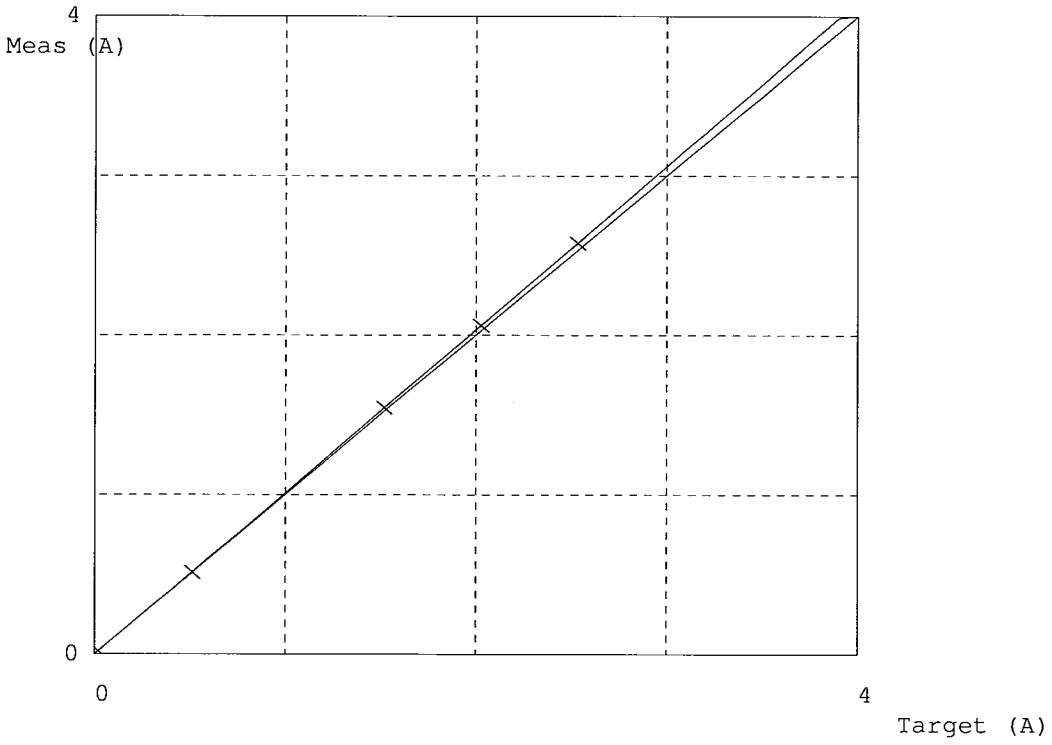

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM1146
Page : 1 of 3

Certificate of Calibration

Equipment :	Incubator
Manufacturer :	SHEL-LAB
Model :	1915A
Serial No. :	0200599
ID No. :	BKK_ML0010
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthakan Rd., Khwawng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Incubation & Micrological Reading
Received Order :	17 July 2023
Calibration Date :	17 July 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Man Pattanapongpaiboon

REVIEW BY sithichok
APPROVED BY
NEXT CAL. DATE 17/01/25

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul
(/) Malee Butkruea
( ) Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056489

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1

Cert. No.: 23TM1146

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	56
AC Supply (Volt)	221	223

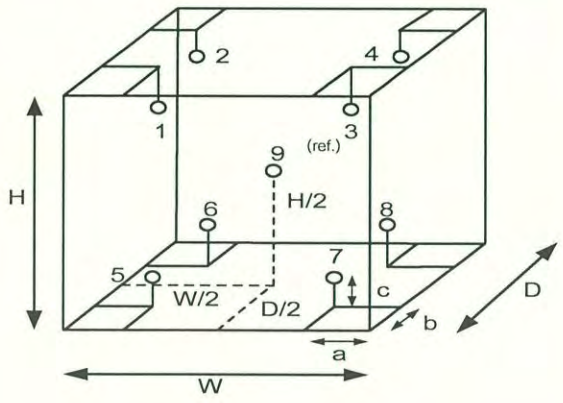

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.50	m
W =	0.75	m
H =	1.2	m
Capacity =	0.45	m^3

Malu .

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 23TM1146

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
35.0	35.0	35.0	0.055	0.30	0.44	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.888	34.933	34.815	34.813	35.064	35.019	35.156	35.141	35.087	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

Malee.

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 22TM1571
Page : 1 of 3

Certificate of Calibration

Equipment :	Hot Air Oven
Manufacturer :	Binder
Model :	ED 240/E2
Serial No. :	00-15533
ID No. :	BKK_ML0013
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Media Preparatiom Room
Received Order :	21 November 2022
Calibration Date :	21 November 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Krisda Malee

REVIEW BY Sithichok
APPROVED BY
NEXT CAL. DATE 21/05/24

Approved by : Malu.
Approved Signatory

( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0048150

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1

Cert. No.: 22TM1571

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration


1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	53	55
AC Supply (Volt)	219	220

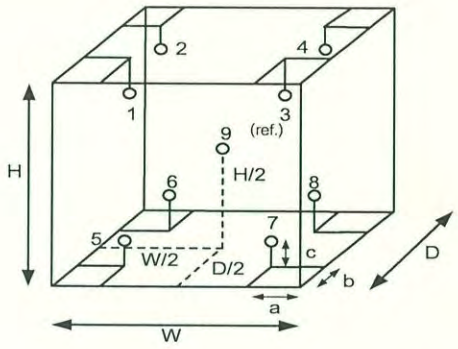

Probe Installation Details :

a =	5.0	cm
b =	5.0	cm
c =	5.0	cm

Dimension of Chamber :

D =	0.50	m
W =	0.80	m
H =	0.60	m
Capacity =	0.24	m^3

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

Malu.

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1571

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (±°C)	Coverage Factor *k*
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point (°C)	Measured Temperature (°C) Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

Malu

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM637
Page : 1 of 3

Certificate of Calibration

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WNE 45
Serial No. :	L712.0429
ID No. :	BKK_ML0056
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Incubator & Microbiological Reading
Received Order :	20 April 2023
Calibration Date :	20 April 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %

REVIEW BY Sithichok
APPROVED BY
NEXT CAL. DATE 20/4/24

Calibrated by : Kunchit Promprat

Approved by : Malee.
Approved Signatory

( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 24 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0053357

Equipment : Water Bath **Cert. No.:** 23TM637

Condition As-Received : Used Item

Reference : 2304-0253OC-1

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44073381	22LM78/1	12 May 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	45	223
Finished of Calibration	25	43	223

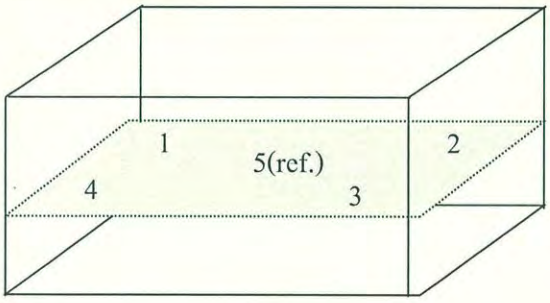

Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2304-0253OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM637

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C) Position					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.492	44.463	44.475	44.510	44.491	0.15
45.0	45.0	45.0	45.005	44.962	44.979	45.016	44.986	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor *k*
44.5	0.051	0.022	2
45.0	0.080	0.026	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

Malee.

© 2022 by Agilent Technologies

Agilent CrossLab Compliance Services

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID:	GM-10
Organization Name:	ALS Laboratory Group (Thailand) Co., Ltd.
Organization Location:	104 Patthanakarn 40, Patthanakarn Rd., Kwang Suan Luang, Khet Suan Luang, Bangkok 10250
Date:	May 25, 2023 11:05:07 AM
EQP Name:	AgilentRecommended , AgilentRecommended
EQP Revision:	GC.02.52, GCMS.02.51
Overall Qualification Status:	Pass

REVIEW BY Suchada T.

APPROVED BY Nant Sant

NEXT CAL. DATE 25 Nov 24

CDS Logon Verification - GC

Logon: SESSIONNAME

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: **Pass**

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front MMI

Setpoint Status: **Pass**

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	24.9	psi

Accuracy:		0.1	psi
Agilent Recommended:	<=	1.2	

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:	7890					
Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	230.0	230.0	°C			
Accuracy:		0.0	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-5.0	°C)
	<=	1.0	% setpoint in K	(	5.0	°C)
Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	100.0	100.0	°C			
Accuracy:		0.0	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-3.7	°C)
	<=	1.0	% setpoint in K	(	3.7	°C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:	7890			
Setpoint Status:	**Pass**			
	Setpoint/Average			
Temperature:	100.0	100.0333	°C	
Stability:		0.1	°C	
Agilent Recommended:	<=	0.5		

Overall GC Oven Temperature Stability Test Status

Pass

Date: May 25, 2023 11:05:07 AM
System ID: GM-10

Tune EI

Tested Combination1	Front	MMI	/ External	TQ	
Name:	7000D				
Setpoint Status:	**Pass**				
Filament:	1				
Setpoint Status:	**Pass**				
Filament:	2				

Overall Tune EI Test Status

Pass

Scouting Run

Tested Combination1	Front	MMI	/ External	TQ	
	Injection Tower				
Name:	7693A				
Source:	EI - Extractor				
Setpoint Status:	**Completed**				
Injection Volume on Column:	1.0	uL			

Overall Scouting Run Status

Completed

Instrument Detection Limit

Tested Combination1	Front	MMI	/ External	TQ	
	Injection Tower				
Name:	7693A				
Source:	EI - Extractor				

Setpoint Status:	**Pass**		
Injection Volume on Column:	1.0 uL		
	Area		Retention Time
Minimum RSD:	10.98 %		0.05 %
Agilent Recommended:	<= 12.00		<= 1.00
Status:	Pass		Pass
Instrument Detection Limit:	3.69552 fg		
Agilent Recommended:	<= 4.03800		
Status:	Pass		

Overall Instrument Detection Limit Test Status

Pass

Mass Ratio Precision

Tested Combination1	Front	MMI	/ External	TQ
	Injection Tower			
Name:	7693A			
Source:	EI - Extractor			
Setpoint Status:	**Pass**			
Injection Volume on Column:	1.0 uL			
	Area Mass 1 Abundance*s		Mass Ratio	
RSD:	3.22 %		4.06 %	
Agilent Recommended:	<= 5.00		<= 5.00	
	Pass		Pass	

Overall Mass Ratio Precision Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GM-10
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN18180003
Firmware Revision	A.11.02
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN18170137
Firmware Revision	A.11.03
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN18153080
Firmware Revision	B.02.05
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	MMI
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Inlet 2

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Back
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	TQ
Name	7000D
Serial Number	US1826U108
Firmware Revision	G.7000.085A
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Nattapat Hengcharoen
Logged On User Name:	nattapat.hengcharoen@agilent.com
Signature Creation Date:	May 25, 2023
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: nattapat.hongcharoen
Hostname: ASBKKWX265

System Id: GM-10
Print Date: May 25, 2023 11:05:08 AM

ALS_GM-10 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 22, 2023 1:32:30 PM	Audit	SessionCreated	Session	None
May 22, 2023 1:32:30 PM	Start	Configuration	Session	None
May 22, 2023 1:32:30 PM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
May 22, 2023 1:37:48 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.52/Gc.02.52.eqp], EQP File Name: [Gc.02.52.eqp], EQP Name: [AgilentRecommended],Protocol Revision :[Gc.02.52] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.51/GcMs.02.51.eqp], EQP File Name: [GcMs.02.51.eqp], EQP Name: [AgilentRecommended]
May 22, 2023 1:37:52 PM	End	Configuration	Session	None
May 22, 2023 1:37:55 PM	Start	Qualification	Session	OQ
May 22, 2023 1:37:55 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
May 22, 2023 2:02:27 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
May 22, 2023 2:02:33 PM	Start	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	None

User Name: nattapat.hengcharoen
Hostname: ASBKKWX265

System Id: GM-10
Print Date: May 25, 2023 11:05:08 AM

ALS_GM-10 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 22, 2023 2:02:37 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
May 22, 2023 2:03:33 PM	End	Execution	CDS Logon Verification - GC : - Qualitative test	Run Count : 1
May 22, 2023 2:34:48 PM	Start	Execution	System Inspection and Basic Safety end Operation - 7890: - Qualitative Test - No setpoints associated	None
May 22, 2023 2:35:02 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
May 22, 2023 2:35:17 PM	Start	Execution	Inlet Pressure Accuracy - Front MMI: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
May 22, 2023 2:35:22 PM	End	Execution	Inlet Pressure Accuracy - Front MMI: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
May 22, 2023 2:35:24 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
May 22, 2023 2:35:48 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
May 22, 2023 2:35:54 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1

User Name: nattapat.hengcharoen
Hostname: ASBKKWX265

System Id: GM-10
Print Date: May 25, 2023 11:05:08 AM

ALS_GM-10 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 22, 2023 2:35:55 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
May 22, 2023 2:59:09 PM	Start	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	None
May 22, 2023 3:08:09 PM	Start	Execution	Scouting Run - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
May 22, 2023 3:10:34 PM	Start	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	None
May 22, 2023 3:12:01 PM	Start	Execution	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	None
May 22, 2023 3:17:49 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
May 22, 2023 3:17:55 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
May 22, 2023 3:18:05 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

User Name: nattapat.hengcharoen
Hostname: ASBKKWX265

System Id: GM-10
Print Date: May 25, 2023 11:05:08 AM

ALS_GM-10 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 22, 2023 3:18:07 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
May 22, 2023 3:39:07 PM	Start	Execution	Scouting Run - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
May 22, 2023 3:39:10 PM	Start	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	None
May 22, 2023 4:02:59 PM	Start	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	None
May 22, 2023 4:03:06 PM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
May 22, 2023 4:03:52 PM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
May 22, 2023 4:03:54 PM	End	Execution	GC Oven Temperature Stebility - 7890: - Temperature : Qven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
May 23, 2023 3:58:15 PM	Audit	AceClosed	Session	None
Mey 24, 2023 4:03:19 PM	Audit	AceRestarted	Session	None
May 24, 2023 4:14:45 PM	Audit	AceClosed	Session	None
May 25, 2023 10:13:57 AM	Audit	AceRestarted	Session	None
May 25, 2023 10:27:12 AM	Audit	SessionReloaded	Session	None

User Name: nattapat.hengcharoen
Hostname: ASBKKWX265

System Id: GM-10
Print Date: May 25, 2023 11:05:08 AM

ALS_GM-10 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 25, 2023 10:27:13 AM	Start	Qualification	Session	OQ
May 25, 2023 10:27:16 AM	Start	Execution	Tune EI - 7000D TQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	None
May 25, 2023 10:27:42 AM	Start	Execution	Tune EI - 7000D TQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	None
May 25, 2023 10:27:56 AM	End	Execution	Tune EI - 7000D TQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
May 25, 2023 10:27:57 AM	Start	Execution	Tune EI - 7000D TQ: - Source: - EI - Extractor Filament 2 (Qualitative - No setpoints associated)	None
May 25, 2023 10:28:07 AM	End	Execution	Tune EI - 7000D TQ: - Source: - EI - Extractor Filament 2 (Qualitative - No setpoints associated)	Run Count : 1
May 25, 2023 10:28:08 AM	Start	Execution	Scouting Run - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
May 25, 2023 10:28:17 AM	Start	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	None
May 25, 2023 10:28:20 AM	Start	Execution	Scouting Run - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None

User Name: nattapat.hengcharoen
Hostname: ASBKKWX265

System Id: GM-10
Print Date: May 25, 2023 11:05:08 AM

ALS_GM-10 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 25, 2023 10:28:58 AM	Audit	Data	Scouting Run - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\SQ_01.D
May 25, 2023 10:29:24 AM	End	Execution	Scouting Run - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Run Count : 1
May 25, 2023 10:29:25 AM	Start	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	None
May 25, 2023 10:30:00 AM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_001.D
May 25, 2023 10:30:00 AM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_002.D
May 25, 2023 10:30:00 AM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_003.D
May 25, 2023 10:30:00 AM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_004.D

User Name: nattapat.hengcharoen
Hostname: ASBKKWX265

System Id: GM-10
Print Date: May 25, 2023 11:05:08 AM

ALS_GM-10 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 25, 2023 10:30:00 AM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_005.D
May 25, 2023 10:30:00 AM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_006.D
May 25, 2023 10:30:00 AM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_007.D
May 25, 2023 10:30:00 AM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_008.D
May 25, 2023 10:30:00 AM	Audit	Data	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_009.D
May 25, 2023 10:30:01 AM	Audit	Date	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\IDL_010.D
May 25, 2023 10:30:19 AM	End	Execution	Instrument Detection Limit - Injection Tower, Front MMI, TQ: - Source: - EI - Extractor - RSD L (Area): <= 12.00% - RSD L (Ret. Time): <= 1.00%	Run Count : 1

User Name: nattapat.hengcharoen
Hostname: ASBKKWX265

System Id: GM-10
Print Date: May 25, 2023 11:05:08 AM

ALS_GM-10 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 25, 2023 10:30:22 AM	Start	Execution	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	None
May 25, 2023 10:30:49 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\MRP_01.D
May 25, 2023 10:30:49 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\MRP_02.D
May 25, 2023 10:30:49 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\MRP_03.D
May 25, 2023 10:30:49 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\MRP_04.D
May 25, 2023 10:30:49 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\MRP_05.D
May 25, 2023 10:30:49 AM	Audit	Data	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \Agilent\OQ_2023\MRP_06.D
May 25, 2023 10:30:57 AM	End	Execution	Mass Ratio Precision - Injection Tower, Front MMI, TQ: - Source: EI - Extractor - L (RSD): <= 5.00%	Run Count : 1
May 25, 2023 10:31:02 AM	End	Qualification	Session	OQ

User Name: nattapat.hengcharoen
Hostname: ASBKKWX265

System Id: GM-10
Print Date: May 25, 2023 11:05:08 AM

ALS_GM-10 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
May 25, 2023 10:31:02 AM	Start	Reporting	Session	None
May 25, 2023 11:04:34 AM	Audit	Reporting	Session	Report Generated : Certificate

© 2022 by Agilent Technologies

Agilent CrossLab Compliance Services

Certificate of System Qualification

GC-OQ + GCMS-OQ

REVIEW BY

APPROVED BY

NEXT CAL. DATE 25-Oct-2024

System ID:	GM-3
Organization Name:	ALS Laboratory Group (Thailand) Co.,Ltd.
Organization Location:	104 Phattanakan40, Patthanakarn Rd., Suan Luang Bangkok 10250
Date:	April 25, 2023 3:53:07 PM
EQP Name:	AgilentRecommended , AgilentRecommended
EQP Revision:	GC.02.52, GCMS.02.53
Overall Qualification Status:	Pass

CDS Logon Verification - GC

Logon: nanthawadee. somboon

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: **Pass**

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: **Pass**

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.2	psi
Accuracy:			0.2	psi
Agilent Recommended:			<= 1.2	

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:	7890					
Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	230.0	231.2	°C			
Accuracy:		1.2	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-5.0	°C)
	<=	1.0	% setpoint in K	(	5.0	°C)

Setpoint Status:	**Pass**					
Zone:	Oven					
	Setpoint/Actual					
Temperature:	100.0	100.6	°C			
Accuracy:		0.6	°C			
Agilent Recommended:	>=	-1.0	% setpoint in K	(	-3.7	°C)
	<=	1.0	% setpoint in K	(	3.7	°C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:	7890			
Setpoint Status:	**Pass**			
	Setpoint/Average			
Temperature:	100.0	100.5333	°C	
Stability:		0.1	°C	
Agilent Recommended:	<=	0.5		

Overall GC Oven Temperature Stability Test Status

Pass

Date: April 25, 2023 3:53:07 PM
System ID: GM-3

Log Amp

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Setpoint Status:	**Pass**			

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Setpoint Status:	**Pass**			

Amu: 1050 m/z

	Drift After Five Minutes:					RFPA Voltage:	
	5	mV				500	mV
Agilent Recommended:	>=	-100	and	<=	100	<=	1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			
Setpoint Status:	**Pass**			
Filament:	1			
Setpoint Status:	**Pass**			
Filament:	2			

Overall Tune EI Test Status

Pass

Scouting Run

Date: April 25, 2023 3:53:07 PM
System ID: GM-3

Tested Combination1	Front	SSL	/ External	SQ
	Injection Tower			
Name:	7693A			
Source:	EI - Inert			

Setpoint Status: **Completed**

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Signal to Noise EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5975C inert XL with TAD			

Source: EI - Inert Filament: 1

Setpoint Status: **Pass**

Signal to Noise: 1152

Agilent Recommended: >= 320

Source: EI - Inert Filament: 2

Setpoint Status: **Pass**

Signal to Noise: 3894

Agilent Recommended: >= 320

Overall Signal to Noise EI Test Status

Pass

Injection Precision

Tested Combination1	Front	SSL	/ External	SQ
Name:	7693A			
Source:	EI - Inert			

Setpoint Status:	**Pass**				
Injection Volume on Column:	1.0	uL			
Area RSD:	2.65	%	Retention Time RSD:	0.01	%
Agilent Recommended:	<= 5.00			<= 1.00	

Overall Injection Precision Test Status

Pass

Mass Ratio Precision

Tested Combination1	Front Injection Tower	SSL	/ External	SQ
Name:	7693A			
Source:	EI - Inert			

Setpoint Status:	**Pass**				
Injection Volume on Column:	1.0	uL			
	Area Mass 1 Abundance*s		Mass Ratio		
RSD:	2.65	%	0.51	%	
Agilent Recommended:	<= 5.00		<= 5.00		
	Pass		Pass		

Overall Mass Ratio Precision Test Status

Pass

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	GM-3
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4513A
Serial Number	CN12520102
Firmware Revision	A.10.07
Component ID/Asset No.	BKK_EN0051
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Sampler 2

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN12490026
Firmware Revision	A.10.16
Component ID/Asset No.	BKK_EN0052
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3440A
Serial Number	CN1252119
Firmware Revision	A.01.14
Component ID/Asset No.	BKK_EN0049
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5975C inert XL with TAD
Model Number	G3172A
Serial Number	US13013A11
Firmware Revision	7.02.29
High Vacuum System	Turbo Pump
Scouting Run Standard	MRP Std
Component ID/Asset No.	BKK_EN0050

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Inert
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Adirek Rattanawijit
Logged On User Name:	adirek.rattanawijit@non.agilent.com
Signature Creation Date:	April 25, 2023
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: adirek.rattanawijit
Hostname: ASBKKWX314

System Id: GM-3
Print Date: April 25, 2023 3:53:10 PM

ALS_OQGCMS_GM-3_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 25, 2023 12:13:47 PM	Audit	Date	Session	Transaction Log file is either corrupted or deleted
April 25, 2023 12:13:47 PM	Audit	Entitlement	Licensing	Session identifier generated: 0800-000G-0000-02RV-VW5G
April 25, 2023 12:13:47 PM	Audit	SessionCreeted	Session	None
April 25, 2023 12:13:47 PM	Start	Configuration	Session	None
April 25, 2023 12:16:43 PM	Audit	Entitlement	Licensing	Succesfully unlocked session identified by 0800-000G-0000-02RV-VW5G with unlock code ZXT0-HEV9-4TK0-9CG1-3W4G
April 25, 2023 12:35:37 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.52/Gc.02.52.eqp], EQP File Name: [Gc.02.52.eqp], EQP Name: [AgilentRecommended] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.53/GcMs.02.53.eqp], EQP File Name: [GcMs.02.53.eqp], EQP Name: [AgilentRecommended]
April 25, 2023 12:36:29 PM	End	Configuration	Session	None
April 25, 2023 12:36:35 PM	Start	Qualification	Session	OQ
April 25, 2023 12:36:35 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None

Page 1 / 9

User Name: adirek.rattanawijit
Hostname: ASBKKWX314

System Id: GM-3
Print Date: April 25, 2023 3:53:10 PM

ALS_OQGCMS_GM-3_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 25, 2023 12:45:27 PM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
April 25, 2023 12:46:03 PM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
April 25, 2023 12:46:05 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
April 25, 2023 12:46:15 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
April 25, 2023 12:46:24 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
April 25, 2023 12:47:14 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
April 25, 2023 12:47:16 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
April 25, 2023 12:47:18 PM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
April 25, 2023 12:47:56 PM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

User Name: adirek.rattanawijit
Hostname: ASBKKWX314

System Id: GM-3
Print Date: April 25, 2023 3:53:10 PM

ALS_OQGCMS_GM-3_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 25, 2023 12:47:59 PM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
April 25, 2023 12:48:01 PM	Start	Execution	GC Oven Temparature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
April 25, 2023 12:49:10 PM	Audit	Data	GC Qven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
April 25, 2023 12:49:13 PM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
April 25, 2023 12:49:15 PM	Stert	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
April 25, 2023 12:50:54 PM	Start	Execution	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	None
April 25, 2023 12:50:59 PM	Start	Execution	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	None
April 25, 2023 1:45:29 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
April 25, 2023 2:04:37 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
April 25, 2023 2:07:02 PM	Start	Execution	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	None

User Name: adirek.rattanawijit
Hostname: ASBKKWX314

System Id: GM-3
Print Date: April 25, 2023 3:53:10 PM

ALS_OQGCMS_GM-3_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 25, 2023 2:07:32 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_002.D
April 25, 2023 2:07:32 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_003.D
April 25, 2023 2:07:32 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_004.D
April 25, 2023 2:07:32 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_005.D
April 25, 2023 2:07:32 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_006.D
April 25, 2023 2:07:32 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_007.D
April 25, 2023 2:08:32 PM	End	Execution	Injection Precision - Injection Tower, Front SSL, SQ: - Source: - EI - Inert L (Area): <= 5.00% - L (Ret. Time): <= 1.00%	Run Count : 1
April 25, 2023 2:08:40 PM	Start	Execution	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	None

User Name: adirek.rattanawijit
Hostname: ASBKKWX314

System Id: GM-3
Print Date: April 25, 2023 3:53:10 PM

ALS_OQGCMS_GM-3_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 25, 2023 2:08:54 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_002.D
April 25, 2023 2:08:54 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_003.D
April 25, 2023 2:08:54 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_004.D
April 25, 2023 2:08:54 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_005.D
April 25, 2023 2:08:54 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_006.D
April 25, 2023 2:08:54 PM	Audit	Data	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\MRP_007.D
April 25, 2023 2:09:07 PM	End	Execution	Mass Ratio Precision - Injection Tower, Front SSL, SQ: - Source: EI - Inert - L (RSD): <= 5.00%	Run Count : 1
April 25, 2023 2:09:12 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None

User Name: adirek.rattanawijit
Hostname: ASBKKWX314

System Id: GM-3
Print Date: April 25, 2023 3:53:10 PM

ALS_OQGCMS_GM-3_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 25, 2023 2:23:24 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
April 25, 2023 2:23:49 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
April 25, 2023 2:24:34 PM	End	Execution	CDS Logon Verification - GC : - Qualitative test	Run Count : 1
April 25, 2023 2:24:43 PM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
April 25, 2023 2:26:07 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
April 25, 2023 2:27:10 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\SN_F1_001.D
April 25, 2023 2:30:51 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\SN_F1_001.D
April 25, 2023 2:35:07 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 1 (Qualitative - No setpoints associated)	None
April 25, 2023 2:35:26 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 1 (Qualitative - No setpoints associated)	Run Count : 1

User Name: adirek.rattanawijit
Hostname: ASBKKWX314

System Id: GM-3
Print Date: April 25, 2023 3:53:10 PM

ALS_OQGCMS_GM-3_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 25, 2023 2:35:28 PM	Start	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 2 (Qualitative - No setpoints associated)	None
April 25, 2023 2:35:47 PM	End	Execution	Tune EI - 5975C inert XL with TAD SQ: - Source: - EI - Inert Filament 2 (Qualitative - No setpoints associated)	Run Count : 1
April 25, 2023 2:35:54 PM	Start	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	None
April 25, 2023 2:37:31 PM	Audit	Data	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\Scout_001.D
April 25, 2023 2:38:33 PM	End	Execution	Scouting Run - Injection Tower, Front SSL, SQ: - Source: - EI - Inert- Part of GCMS System Preparation	Run Count : 1
April 25, 2023 2:41:02 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
April 25, 2023 2:41:06 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\SN_F1_001.D
April 25, 2023 2:46:21 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\SN_F1_002.D

User Name: adlrek.rattanawljit
Hostname: ASBKKWX314

System Id: GM-3
Print Date: April 25, 2023 3:53:10 PM

ALS_OQGCMS_GM-3_2023 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
April 25, 2023 2:49:12 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	None
April 25, 2023 2:49:14 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
April 25, 2023 2:49:23 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Data files Path : O:\MassHunter\GCMS\1\data \OQPV2023\SN_F1_002.D
April 25, 2023 3:02:36 PM	Start	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
April 25, 2023 3:05:59 PM	End	Execution	Log Amp - 5975C inert XL with TAD SQ: - Source: EI - Inert	Run Count : 1
April 25, 2023 3:06:02 PM	Start	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
April 25, 2023 3:11:18 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	None
April 25, 2023 3:13:36 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\SN_F1_01.D
April 25, 2023 3:15:24 PM	End	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 1 - L: >= 320	Run Count : 1

User Name: adirek.rattanawijit
Hostname: ASBKKWX314

System Id: GM-3
Print Date: April 25, 2023 3:53:10 PM

ALS_OQGCMS_GM-3_2023 Transaction log :

Time	Transection State	Activity Performed	Type of Transaction	Optional Information
April 25, 2023 3:15:27 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	None
April 25, 2023 3:15:38 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	None
April 25, 2023 3:15:43 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\SN_F2_01.D
April 25, 2023 3:16:36 PM	Start	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Inert	None
April 25, 2023 3:17:05 PM	End	Execution	RFPA - 5975C inert XL with TAD SQ: - Source: EI - Inert	Run Count : 1
April 25, 2023 3:24:10 PM	Start	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	None
April 25, 2023 3:31:57 PM	Audit	Data	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	Data files Path : D:\MassHunter\GCMS\1\data \OQPV2023\SN_F2_001.D
April 25, 2023 3:33:58 PM	End	Execution	Signal to Noise EI - Injection Tower, Front SSL, SQ: - Source: EI - Inert using Filament 2 - L: >= 320	Run Count : 1
April 25, 2023 3:35:15 PM	End	Qualification	Session	OQ
April 25, 2023 3:35:15 PM	Start	Reporting	Session	None
April 25, 2023 3:51:45 PM	Audit	Reporting	Session	Report Generated : Certificate

บริษัท ดับเบิ้ล เอส ไดแอคนอสติคส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.
4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพฯ 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รอบ							12/7 CE					

Periodical maintenace check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	☐	☑	
2.ISE tubing change	☒	☒	none
3.Syringe check/change		☑	
4.Dispensing check/ change		☑	
5.Waste tubing change when necessary		☑	
6.Lamp check/change	☐	☑	
7.Mixer paddle/paddle change(not Konelab20)		☑	
8.ISE needles check/change		☒	none
9.Pump tubing check/ chance	☐	☑	
10.Broken/worn out part check /change		☑	
11.Peristaltic pump check /cleaning/ lubrication	☐	☑	
12.Heating check		☑	
13.Cooling check		☑	
14.Dispenser mechanic check/adjustment	☐	☑	
15.Cuvette transfer mechanic check/adjustment	☐	☑	
16.Dispenser movement check/adjustment	☐	☑	
17.Sample/reagent register check/adjustment	☐	☑	
18.Dispensing tubing tightness check	☐	☑	
19.Photometer and optics cleaning/check/adjustment	☐	☑	
20.Workstation PC cleaning if necessary	☐	☑	
21.Mechanic cleaning/lubrication	☐	☑	
22.Instrument cleaning if necessary	☐	☑	
23.Complete analyzer testing with waterblank/QC or sample	☐	☑	
24.Test parameters/Adjustment/config. Save to USB key	☐	☑	
25.UPS Test	☐	☑	

Place: ALS LAB **Instrument:** k90 Aqualeem

Date/Time: 12/7/66 **Serial no:** 22781

Service done by: [illegible] **Install date:**

Signature of customer: [illegible] **Date/Time:** 12/7/66

Laboratory
Analyzer User

7/12/2023 21:21

Performed	7/12/2023
Lot	W166

ACCEPTANCE CRITERIA

	Result	Limit	Warning
Temperature (?C)	37.7	37.0 +/- 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	1.17	<1.7	
Photometric noise			
Max SD L340_2 (mA)	0.19	<2.0	
Max SD L340_4 (mA)	1.06	<3.0	
Linearity of photometer			
Slope	1.0188	0.94 - 1.06	
Curvature	0.0035	+/- 0.02	
Max bias from linear fit (mA)	3.2	<15.0	
Max delta %	-2.0	+/- 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (?l)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (?l)	4.13	3.85 - 4.40	
XDISP2 CV%	0.58	<2.0	
XDISP4 CV%	0.70	<2.0	
XDISP10 CV%	0.59	<2.0	
Needle 0 ?l volume			
Average (A)	0.009	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (?l)	0.06	<0.32	

OTHER INFORMATION

Dispensing ratio

Posit	Result (A)
1	0.1592
2	0.1624
3	0.1631
4	0.1631
5	0.1625
6	0.1650

Photom. noise: SD (mA)

Posit	L340_2	L340_4
1	0.07	0.64
2	0.09	1.06
3	0.14	0.50
4	0.13	0.53
5	0.19	0.38
6	0.02	0.64

Laboratory
Analyzer User


7/12/2023 21:21

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.311
XDISP4	0.616
XDISP10	1.478

Linearity of photometer

L340_	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.001	0.005	-0.004	-394.7
2	0.512	0.519	-0.007	-1.5
3	1.523	1.550	-0.027	-1.8
4	2.027	2.066	-0.039	-1.9
5	2.532	2.582	-0.050	-2.0

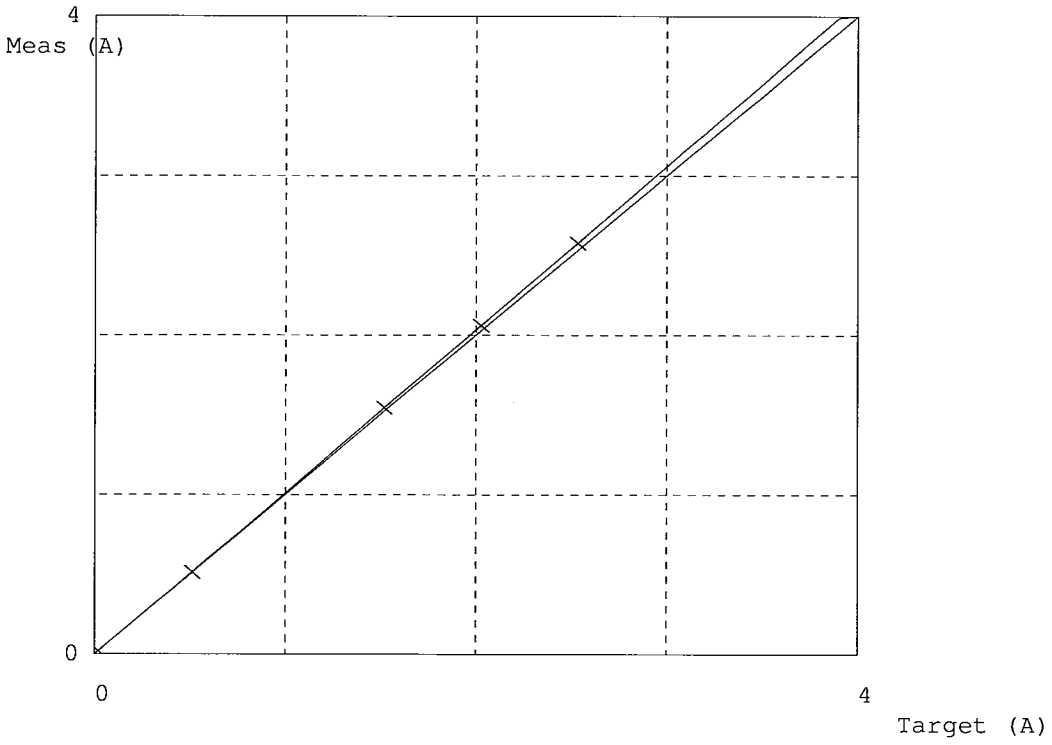

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate of Calibration

Equipment	:	**Chamber (Cold Room)**
Manufacturer	:	**KOLDTECH**
Model	:	**KM-240**
Serial No.	:	**TBN-1012061/06**
Customer Code	:	**BKK_EN0168**
ID No.	:	**T2462A3**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd.**
		104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
		Khet Suan Luang, Bangkok 10250
Customer Location	:	**Environmental Laboratory**
Date of Receipt	:	**27 June 2022**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	_____ **/ Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	04 JUL 2022

REVIEW BY Sirilak P.
APPROVED BY KL AL
NEXT CAL. DATE 01/07/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

SCG

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

NSC-TISI-TIS 17025
CALIBRATION 0244

Calibration Report

Equipment : **Chamber (Cold Room)**
Date of Calibration : **1 July 2022**
Environment : **Temperature : 18.9-23.7 °C**
Line Voltage : 222.9-226.5 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T210009	30 July 2022
TC	TYPE T	TN171-TN180	T210009	30 July 2022
DATA LOGGER	34970A	T149	T210009	30 July 2022

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 6 Hour 28 Minute At 3 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By.

SCG

Metrological Center


SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T221645

Calibration Report

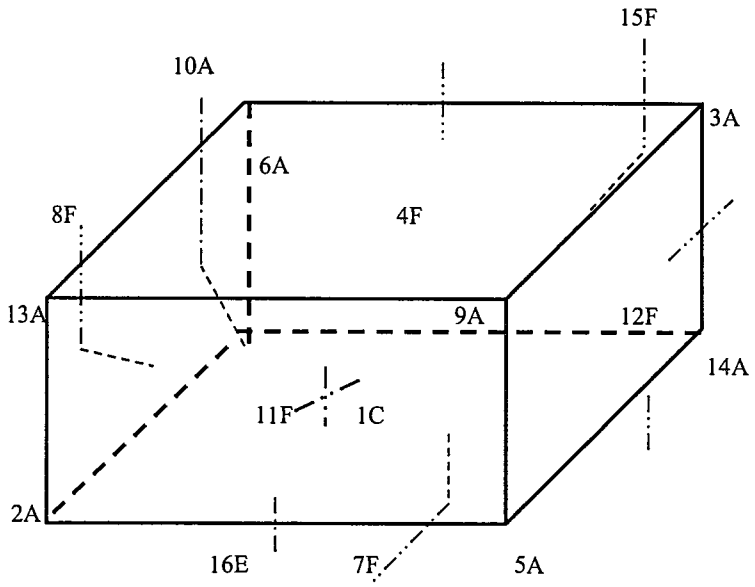

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN171
12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175
16E	=	TN176

Approved By.

SCG

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

NSC-TISI-TIS 17025
CALIBRATION 0244

Certificate No. T221645

Calibration Report

Measurement Results:

	Average Standard Reading at each position (°C)									
Calibration Point	**TN161**	**TN162**	**TN163**	**TN164**	**TN165**	**TN166**	**TN167**	**TN168**	**TN169**	**TN170**
3	2.91	2.97	2.80	3.09	3.00	2.99	3.22	2.86	3.17	3.19
	TN171	**TN172**	**TN173**	**TN174**	**TN175**	**TN176**				
	2.95	3.41	2.71	3.30	3.04	3.01				

Chamber (Cold Room)			**Temperature Distribution**				
Setting (°C)	**Reading (°C)**		**Average (°C)**	**Stability (±°C)**	**Uniformity (°C)**	**Uncertainty (±°C)**	**Coverage Factor *k***
	Min , Max	**Average**					
3.0	2.8 , 4.0	3.2	3.04	1.33	0.93	1.91	2.00

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By.

Agilent Technologies

Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A,D
968 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel. +662 637 6363
Fax: +662 632 4334
Email: ccc-smt@agilent.com
Website: www.agilent.com/chem

Customer Contact:
ALS Laboratory Group (Thailand) Co Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

TAX ID : 0105540004859

Chanattagarn.lmchom@alsglobal.com
27603068

Invoice To:
ALS Laboratory Group (Thailand) Co Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

SERVICE REPORT

Customer Purchase Order Number:	**Customer Number:** 70371013
Service Request:	**Service Request Date:**
Service Order: 6006033911	**Service Confirmation:** 6904800024

REVIEW BY Thitima S.
APPROVED BY Sawitr N.
NEXT CAL DATE 19 Sep 2024

Delivery Site:
ALS Laboratory Group (Thailand) Co Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Location:
Room
Bldg
Lab
Dept

Direct Inquiries to:
Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at www.agilent.com/chem

Service Confirmation Number: 6904800024

Service Confirmation Date: 20.03.2023

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IO-5100	ICP-OES 5100/5110 System			
G8010A	Agilent 5100 SVDV ICP-OES Spectrometer	MY16010005	ICP OES 5100	SYS-IO-5100
G8410A	SPS 4 Autosampler	AU15440764	ICP OES 5100	SYS-IO-5100

Service Items:



Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EOQ	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	20.03.2023	20.03.2023

Additional Information:

Service Confirmation Number: 6904800024

Service Confirmation Date: 20.03.2023

Service Information:

Problem Description: WU-S-OQ-IO-5100-5001143313		
Service Provided: Complete OQHW 5100ICPOES Equipment ID: BKK_EL0037, all tests passed		
Service Overview Code: Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
Reported Hours: 4.0	**Travel Hours:** 2.0	
Customer Field Service Representative Name: **Kanyakorn Sukpathrajarern**	**Customer Field Service Representative Signature:** 	**Date:** **20 Mar 2023**
Customer Name: **Thitima Boonpeng**	**Customer Signature:** 	**Date:** **20 Mar 2023**
Additional Comments:		

REVIEW BY Chanatt S.
APPROVED BY Saowalux N.
NEXT CAL. DATE 6/12/24

Scientist Instrument

Performance Verification Certificate
for Mercury Analyzer

PRODUCT ID	***Quicktrace M-8000 , Teledyne Leeman Labs***
Equipment ID	**BKK_EL0128 Mercury Analyzer** **S/N: US22133002** **BKK_EL0129 Autosampler** **S/N : 052222A560**
Customer Name	ALS Laboratory Group (Thailand) Co., Ltd.
Address	104 Soi Pattana 40, Pattana Rd. Suan Luang, Suan Luang Bangkok 10250 Thailand

Date of Qualified **December 6, 2023**
Next Due date **December 6, 2024**

This certifies for products which was performed in acceptable criteria specifications

Autosampler & Sample Introduction	**PASSED**
Analyzer	**PASSED**
Gas Liquid Separator & Dryer	**PASSED**
CVAFS Detector	**PASSED**
Electronics/Mechanical	**PASSED**
Data station/PC	**PASSED**
Analytical test	**PASSED**

Provided by

Scientist Instrument Co.,Ltd.
113 Soi Ekachai 44, Ekachai Road
Khlong Bang Phran, Bangbon
Bangkok 10150 Thailand

Certified by .....
Thunraphol Sakdayos

Service Engineer

SCG
CEMENT-BUILDING MATERIALS

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T220730

Certificate of Calibration

Equipment	:	HEATING BLOCK
Manufacturer	:	Environmental Express
Model	:	SC 196
Serial No.	:	6974CECW3285
Customer Code	:	BKK_EL0054
ID No.	:	T5306A3
Customer	:	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250
Customer Location	:	Acid Digestion Lab
Date of Receipt	:	30 March 2022
Calibrated By	:	Watcharapon Sangtong (Technician)
Approved By	:	_____ / Sujjar Naknakred (Site Calibration Manager)
Date of Issue	:	12 APR 2022

REVIEW BY Tattaporn C.
APPROVED BY Sawitri N.
NEXT CAL. DATE 7/10/23

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Equipment : **HEATING BLOCK**
Date of Calibration : **7 April 2022**
Environment : **Temperature : 21.8-23.1 °C**
Line Voltage : 221.6-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.
   All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN221-TN230	T210008	08 June 2022
TC	TYPE T	TN231-TN240	T210008	08 June 2022
DATA LOGGER	34970A	T149	T210008	08 June 2022

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 2 Hour 25 Minute At 95 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   ( ) without adjustment (X) after adjustment

Approved By._____

Metrological Center


SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

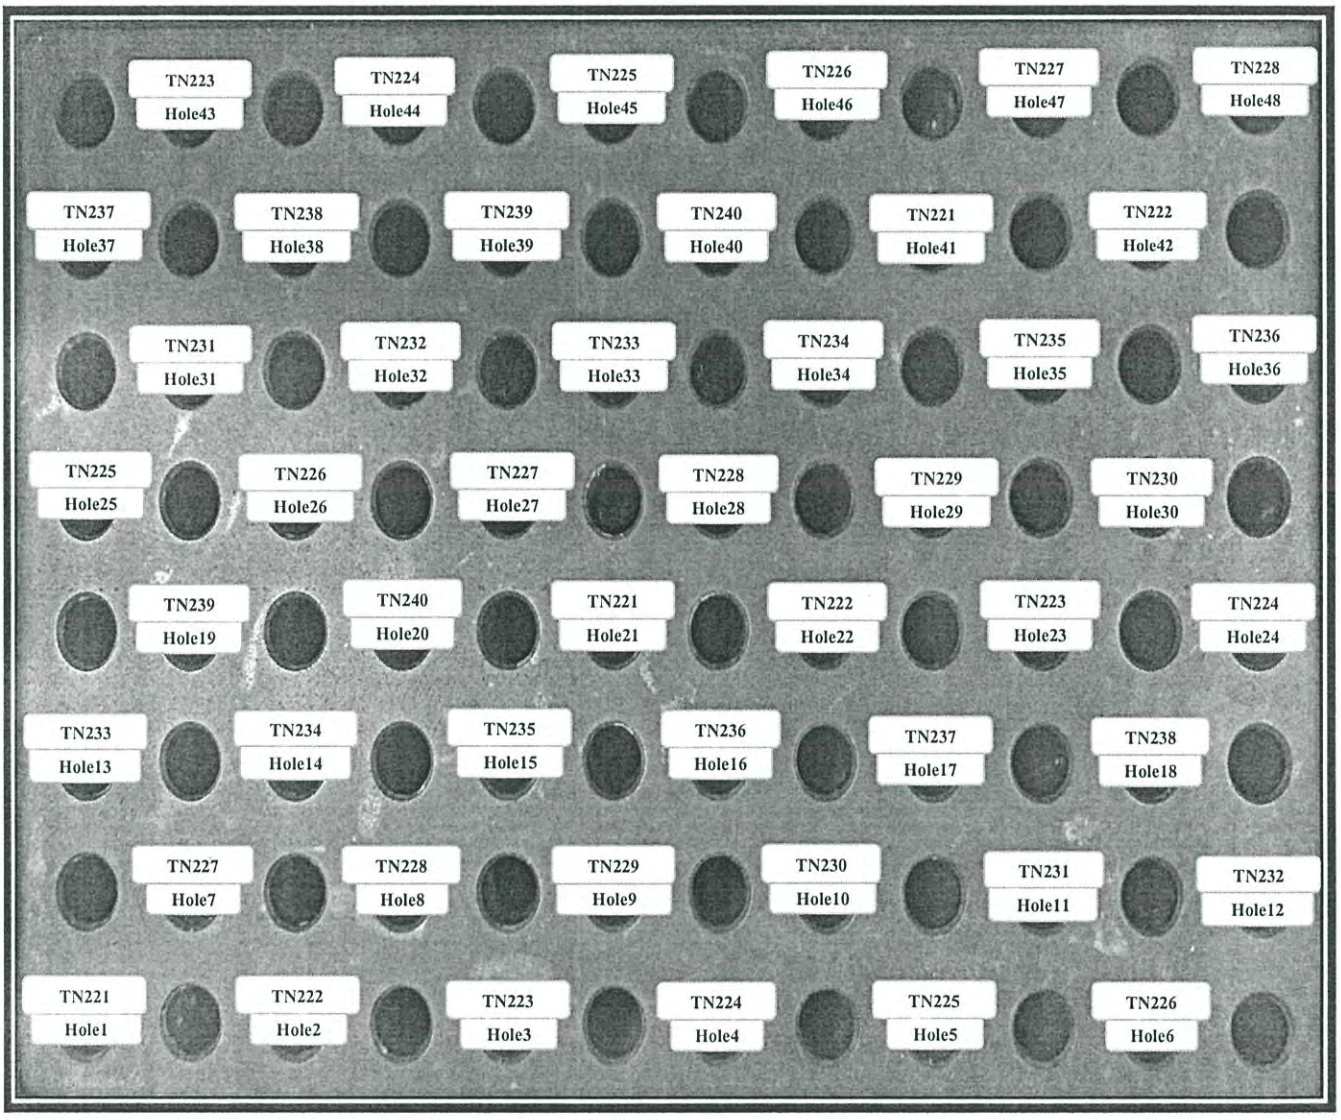

FRONT CONTROL

Approved By. _____

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		**TN221**	**TN222**	**TN223**	**TN224**	**TN225**	**TN226**
CAL POINT	Max	93.60	93.82	94.05	94.20	94.36	94.26
95	Min	93.07	93.26	93.51	93.66	93.82	93.71
	Average	93.33	93.54	93.78	93.93	94.09	93.98
R2 Hole7-Hole12		**TN227**	**TN228**	**TN229**	**TN230**	**TN231**	**TN232**
	Max	94.59	94.79	94.63	94.55	94.82	95.00
	Min	94.05	94.25	94.08	93.97	94.26	94.44
	Average	94.32	94.52	94.36	94.26	94.54	94.72
R3 Hole13-Hole18		**TN233**	**TN234**	**TN235**	**TN236**	**TN237**	**TN238**
	Max	95.03	94.54	94.78	94.84	95.06	94.73
	Min	94.46	93.98	94.20	94.28	94.49	94.18
	Average	94.74	94.26	94.49	94.56	94.78	94.45
R4 Hole19-Hole24		**TN239**	**TN240**	**TN221**	**TN222**	**TN223**	**TN224**
	Max	94.89	94.82	95.73	95.85	95.73	96.10
	Min	94.33	94.26	95.51	95.62	95.51	95.85
	Average	94.61	94.54	95.62	95.73	95.62	95.97
R5 Hole25-Hole30		**TN225**	**TN226**	**TN227**	**TN228**	**TN229**	**TN230**
	Max	96.28	96.39	96.37	96.54	96.19	96.04
	Min	96.01	96.10	96.02	96.20	95.89	95.71
	Average	96.15	96.24	96.20	96.37	96.04	95.88
R6 Hole31-Hole36		**TN231**	**TN232**	**TN233**	**TN234**	**TN235**	**TN236**
	Max	96.84	96.97	97.03	96.48	96.33	95.76
	Min	96.53	96.65	96.71	96.08	95.98	95.43
	Average	96.68	96.81	96.87	96.28	96.16	95.60
R7 Hole37-Hole42		**TN237**	**TN238**	**TN239**	**TN240**	**TN221**	**TN222**
	Max	96.46	96.15	96.19	96.06	96.95	97.09
	Min	96.13	95.84	95.85	95.72	96.64	96.78
	Average	96.30	95.99	96.02	95.89	96.80	96.93
R8 Hole43-Hole48		**TN223**	**TN224**	**TN225**	**TN226**	**TN227**	**TN228**
	Max	96.91	96.58	96.13	96.19	96.34	96.19
	Min	96.55	96.21	95.80	95.87	96.03	95.88
	Average	96.73	96.40	95.96	96.03	96.18	96.03

Approved By. _____

SCG
CEMENT-BUILDING MATERIALS

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110
Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109
Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		**TN221**	**TN222**	**TN223**	**TN224**	**TN225**	**TN226**
CAL POINT	Max	104.47	104.65	104.79	105.31	105.47	105.46
105	Min	104.15	104.27	104.45	104.98	105.14	105.20
	Average	104.31	104.46	104.62	105.15	105.31	105.33
R2 Hole7-Hole12		**TN227**	**TN228**	**TN229**	**TN230**	**TN231**	**TN232**
	Max	105.55	105.73	105.65	105.84	105.97	106.07
	Min	105.28	105.43	105.35	105.52	105.68	105.83
	Average	105.42	105.58	105.50	105.68	105.82	105.95
R3 Hole13-Hole18		**TN233**	**TN234**	**TN235**	**TN236**	**TN237**	**TN238**
	Max	106.14	106.06	105.81	106.05	105.81	105.87
	Min	105.85	105.81	105.55	105.80	105.53	105.64
	Average	106.00	105.94	105.68	105.92	105.67	105.75
R4 Hole19-Hole24		**TN239**	**TN240**	**TN221**	**TN222**	**TN223**	**TN224**
	Max	105.86	105.60	104.44	104.51	104.28	104.78
	Min	105.61	105.37	104.27	104.35	104.12	104.61
	Average	105.74	105.48	104.35	104.43	104.20	104.69
R5 Hole25-Hole30		**TN225**	**TN226**	**TN227**	**TN228**	**TN229**	**TN230**
	Max	104.94	104.93	104.97	105.08	104.68	104.69
	Min	104.77	104.75	104.76	104.90	104.51	104.49
	Average	104.85	104.84	104.86	104.99	104.60	104.59
R6 Hole31-Hole36		**TN231**	**TN232**	**TN233**	**TN234**	**TN235**	**TN236**
	Max	105.44	105.45	105.61	104.95	104.84	104.42
	Min	105.27	105.27	105.44	104.76	104.66	104.25
	Average	105.36	105.36	105.53	104.86	104.75	104.33
R7 Hole37-Hole42		**TN237**	**TN238**	**TN239**	**TN240**	**TN221**	**TN222**
	Max	105.17	104.70	104.59	104.51	105.22	105.53
	Min	105.00	104.53	104.41	104.35	105.04	105.37
	Average	105.08	104.62	104.50	104.43	105.13	105.45
R8 Hole43-Hole48		**TN223**	**TN224**	**TN225**	**TN226**	**TN227**	**TN228**
	Max	105.61	105.45	105.10	104.77	104.87	105.02
	Min	105.44	105.28	104.92	104.60	104.70	104.85
	Average	105.53	105.37	105.01	104.69	104.79	104.93

Approved By. _____

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (±°C)	Uncertainty (±°C)
	Min , Max	Average		
100.0	100.0 , 100.4	100.1	0.29	0.83
105.0	105.0 , 105.4	105.1	0.20	0.79

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangrak Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

Bara Scientific
Solution of Success

NSC-TISI-TIS 17025
CALIBRATION 0209

Certificate of Calibration

Certificate No.	BSCC-UV-307/22
Equipment	UV/Vis Spectrophotometer
Model	UV-1800
Manufacturer	Shimadzu
Serial No.	A11454908533CD
ID No.	BKK_EN0018
Date of receipt	16 September 2022
Date of calibration	16 September 2022
Date of issue	23 September 2022

REVIEW BY Sirilak P.
APPROVED BY
16/9/23
NEXT CAL. DATE ~~23/9/22~~

Customer name	ALS Laboratory Group (Thailand) Co., Ltd.
Address	104 Soi Phatthanakan 40, Phatthanakan Road, Phatthanakan, Suan Luang, Bangkok 10250
Temperature	(22.1-23.3) °C (On site)
Humidity	(58.8-63.2) %RH (On site)
Equipment condition	Good Operation
Calibration Location	Organic Prep
Calibration Procedure	In-house method WI-UV-702-01 based on ASTM E275-01
Traceability	Wavelength Accuracy is traceable to certificate No. 95917 and 95918 Photometric Accuracy is traceable to certificate No. 95924 and 95937 Stray Light is traceable to certificate No. 95908 The above certificate are traceble to SI unit through Starna Scientific Ltd. (UKAS accredited calibration laboratory NO. 0659)
Calibrated by	Mr.Waruth Janphung

Approved by

Mr.Kanchit Choothep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the resuits are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangrak Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

NSC-TISI-TIS 17025
CALIBRATION 0209

Certificate of Calibration

Certificate No. **BSCC-UV-307/22** Number of Page(s) 2 of 3

Calibration Results:

1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
241.70	241.65	-0.05	0.18
334.02	333.92	-0.10	0.18
418.53	418.46	-0.07	0.18
572.99	572.96	-0.03	0.18
879.41	879.17	-0.24	0.18

2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.0075
	0.7467	0.7461	-0.0006	0.0075
257	0.0000	0.0000	0.0000	0.0075
	0.8662	0.8647	-0.0015	0.0075
313	0.0000	0.0000	0.0000	0.0075
	0.2904	0.2911	0.0007	0.0075
350	0.0000	0.0000	0.0000	0.0075
	0.6429	0.6426	-0.0003	0.0075

*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the resuits are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

Bara Scientific Co., Ltd.
968 U Chu Liang Building Floor7 Rama4 Road
Silom Bangrak Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

NSC-TISI-TIS 17025
CALIBRATION 0209

Certificate of Calibration

Certificate No. **BSCC-UV-307/22** Number of Page(s) 3 of 3

Calibration Results:

3.Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5783	0.5777	-0.0006	0.0042
	0.7628	0.7635	0.0007	0.0046
	1.0206	1.0230	0.0024	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5621	0.5618	-0.0003	0.0042
	0.7455	0.7460	0.0005	0.0048
	0.9985	1.0005	0.0020	0.0042
465.0	0.0000	0.0000	0.0000	0.0042
	0.5227	0.5219	-0.0008	0.0042
	0.6880	0.6884	0.0004	0.0051
	0.9487	0.9503	0.0016	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5207	0.5199	-0.0008	0.0042
	0.6973	0.6971	-0.0002	0.0049
	0.9959	0.9964	0.0005	0.0042
590.0	0.0000	0.0000	0.0000	0.0042
	0.5544	0.5534	-0.0010	0.0042
	0.7253	0.7242	-0.0011	0.0050
	1.0942	1.0943	0.0001	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5616	0.5606	-0.0010	0.0042
	0.6927	0.6921	-0.0006	0.0053
	1.0881	1.0885	0.0004	0.0042

*CNR = Customer not request

4.Stray Light*

Standard cut-off wavelenght (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.96±0.11nm	200.30	0.9505	2.0229

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A
***Stray Light not NSC-ONSC Accredited.**

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

*****End of Certificate*****

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.
Advertising the report / Certificate and publicity of the resuits are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.

Scientist Instrument

REVIEW BY P. Suvijaring
APPROVED BY Sauta N.
NEXT CAL. DATE 30/11/23

Performance Verification Certificate

for Mercury Analyzer

Product ID *Quicktrace M-8000 , Teledyne Leeman Labs*

Equipment ID **BKK_EL0128 Mercury Analyzer**
S/N: US22133002

BKK_EL0129 Autosampler
S/N: 052222A560

Customer Name ALS Laboratory Group (Thailand) Co., Ltd.
Address 104 Soi Pattana 40, Pattana Rd. Suan Luang, Suan Luang
Bangkok 10250 Thailand

Date of Qualified **November 30, 2022**
Next Due date **November 30, 2023**

This certifies for products which was performed in acceptable criteria specifications

Autosampler & Sample Introduction	**PASSED**
Analyzer	**PASSED**
Gas Liquid Separator & Dryer	**PASSED**
CVFS Detector	**PASSED**
Electronics/Mechanical	**PASSED**
Data station/PC	**PASSED**
Analytical test	**PASSED**

Provided by

Scientist Instrument Co.,Ltd.
113 Soi Ekachai 44, Ekachai Road
Khlong Bang Phran, Bangbon
Bangkok 10150 Thailand

Certified by .....

Thunraphol Sakdayos

Service Engineer

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 , e-mail: service.thailand@sartorius.com

NSC-TISI-TIS 17025
CALIBRATION 0426

SARTORIUS

REVIEW BY Sirilut P.
APPROVED BY
NEXT CAL. DATE 8/2/24

Certificate of Calibration

Model Number : MSE224S-100-DU
Description : Analytical Balance
Serial Number : 26207042
ID No. : BKK_EN0002
Manufacturer : Sartorius

Certificate No. : 23BCI0072
Issued Date : Monday, February 13, 2023
Reference No. : 203245
Page No. : 1 0f 2

Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.
104 Phatthanakan 40,Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.
Calibrated Place : Balance Room

Calibrated By : Mr. Chonchai Inthana
Calibration Date : Wednesday, February 08, 2023

Calibration Procedure No. : This calibration was conducted by
Using in-house calibration procedure number (WI-003)
Based on UKAS LAB 14 : 2019

Metrological data :
Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:
Temperature : 23.2 °C ± 5.0 °C
Humidity : 60.0 % RH ± 10.0 % RH
Pressure _ ± _

Reasons for calibration
☐ New Installation ☐ Service / Repaired ☑ Re-calibration/ Maintenance

Equipment Condition: ☑ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Cetificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Mr.Chonchai Inthana(Technical Manager)

STAMP SARTORIUS (THAILAND) CO., LTD. SARTORIUS ISO/IEC 17025:2017

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

SARTORIUS

Certificate of Calibration

Model Number :	MSE224S-100-DU	Certificate No. :	23BCI0072
Description :	Analytical Balance	Issued Date :	Monday, February 13, 2023
Serial Number :	26207042	Reference No. :	203245
ID No. :	BKK_EN0002		
Manufacturer :	Sartorius	Page No. :	2 of 2

Calibration Results : Without Adjustment

Repeatability


The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.


Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	199.9999
Tolerance	20.0000	200.0000
0.0001 g	20.0000	199.9999
	20.0001	200.0000
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0000	199.9999
Tolerance	20.0000	199.9999
0.0001 g	20.0000	200.0000
	20.0001	199.9999
Standard Deviation	0.00004	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximim capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g
Tolerance *0.0004* g





	Difference
1	–
2	-0.0001
3	0.0000
4	0.0001
5	0.0000
6	–

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance *0.0002* g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	199.9999	-0.0001	0.00030

End of Report.

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	Seven Compact S220
Serial No. :	B520948426
ID No. :	BKK_EN0072
Condition As-Received:	Used Item
Received Date :	09 September 2022
Calibration Date :	12 September 2022
Reference :	2209-0312DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)

REVIEW BY Sirilak P.
APPROVED BY
NEXT CAL. DATE 12/03/24

Calibrated by : Warakorn Lerngagtrakul

Approved by : Malee.
Approved Signatory

(✓) Malee Butkruea
( ) Saithip Meangmai
( ) Warakorn Lerngagtrakul

Issue Date : 15 September 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of this calibration result

1. Reference Standard Instrument : -

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023

This certification is traceable to the International System of Unit maintained at:-
- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	823320	20 June 2024
pH 6.985	CPA chem	794122	14 Feb 2023
pH 10.008	CPA chem	823323	20 June 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor *k*
	pH	mV	mV	pH		
pH Meter	4.000	177.48	177.4	4.000	0.058	2.00
S/N.: B520948426	7.000	0.00	0.0	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor *k*
pH Electrode	4.008	3.999	153.9	0.0055	2.09
S/N.:PCE-86-EX1001	6.985	7.017	-13.7	0.0084	2.00
	10.008	9.996	-179.0	0.0078	2.06

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.

DKSH

NSC-TISI-TIS 17025
Calibration 0087

Certificate of Calibration

Equipment:	CONDUCTIVITY METER			Certificate No.:	C24230001
Model:	ORION STAR A215			Issued Date:	5 January 2023
Serial No. (or ID.):	X58031			Job No.:	KSPR2216356
Manufacturer:	Thermo Scientific			Page:	1 of 2
Electrode Serial No.	YV1-18416	Model :	ORION 013005MD	Brand :	Thermo Scientific
Condition:	In Condition				

Customer: ALS Laboratory Group (Thailand) Co., Ltd.
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Environment Condition:

Temperature	21.6	°C	±	0.2	°C
Humidity	58.0	%RH	±	2.0	%RH

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd. (Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By: Mr.Nattapat Rungrueang

Calibration Date: 3 January 2023

The Method used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14

Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 838317, 838313, 838315

(Mr. Nattapat Rungrueang)
Person in charge

(Mr. Nitinun Srihawan)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Before Adjustment

Standard Conductivity Solution		Unit Under Calibration Reading		Correction		Coverage Factor (k)	Uncertainty (±)	
84.000	µS/cm	102.4	µS/cm	-18.400	µS/cm	2.00	0.69	µS/cm
1413.0	µS/cm	1689	µS/cm	-276.0	µS/cm	2.00	11	µS/cm
12.881	mS/cm	15.42	mS/cm	-2.5390	mS/cm	2.00	0.098	mS/cm

After Adjustment ; at 84.0 µS/cm, 1413 µS/cm, 12.88 mS/cm

Standard Conductivity Solution		Unit Under Calibration Reading		Correction		Coverage Factor (k)	Uncertainty (±)	
84.000	µS/cm	84.09	µS/cm	-0.090	µS/cm	2.00	0.68	µS/cm
1413.0	µS/cm	1413	µS/cm	0.0	µS/cm	2.00	11	µS/cm
12.881	mS/cm	12.89	mS/cm	-0.0090	mS/cm	2.00	0.098	mS/cm

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2216356

ชนิดเครื่องมือ: CONDUCTIVITY METER รุ่น: ORION STAR A215 หมายเลขเครื่อง: X58031

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
03 Jan 2023			03 Jan 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
☑	☐	1. ความสมบูรณ์เครื่อง	☑	☐	
☑	☐	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☑	☐	
☑	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	☑	☐	
☑	☐	4. ปุ่มกด (Keypad)	☑	☐	
☑	☐	5. หน้าจอ (Display, Screen Contrast)	☑	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☐	☐	8. ความยาวคลื่น (Wavelength Check)	☐	☐	
☐	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☐	☐	
☐	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☐	☐	
☐	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☐	☐	
		pH Meter and Conductivity Meter			
☑	☐	12. อิเล็คโทรด (Electrode and Connection Cable)	☑	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	☐	☐	
☑	☐	15. ขาจับอิเล็คโทรด (Stand)	☑	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

ข้อแนะนำ : _____

Mr.Nattapat Rungrueang

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

DKSH

NSC-TISI-TIS 17025
Calibration 0067

Certificate of Calibration

Equipment:	CONDUCTIVITY METER			Certificate No.:	C24230001
Model:	ORION STAR A215			Issued Date:	5 January 2023
Serial No. (or ID.):	X58031			Job No.:	KSPR2216356
Manufacturer:	Thermo Scientific			Page:	1 of 2
Electrode Serial No.	YV1-18416	Model :	ORION 013005MD	Brand :	Thermo Scientific
Condition:	In Condition				

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE .....

Customer: ALS Laboratory Group (Thailand) Co., Ltd.
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Environment Condition:	Temperature	21.6	°C	±	0.2	°C
	Humidity	58.0	%RH	±	2.0	%RH

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd. (Wet Chemistry Lab 2)
104 Soi Pattanakarn 40, Pattanakarn Rd.,
Suan Luang, Bangkok 10250 Thailand

Calibration By: Mr.Nattapat Rungrueang

Calibration Date: 3 January 2023

The Method used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14

Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 838317, 838313, 838315

(Mr. Nattapat Rungrueang)
Person in charge

(Mr. Nitinun Srihawan)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Calibration Results:

Before Adjustment

Standard Conductivity Solution		Unit Under Calibration Reading		Correction		Coverage Factor (k)	Uncertainty (±)	
84.000	µS/cm	102.4	µS/cm	-18.400	µS/cm	2.00	0.69	µS/cm
1413.0	µS/cm	1689	µS/cm	-276.0	µS/cm	2.00	11	µS/cm
12.881	mS/cm	15.42	mS/cm	-2.5390	mS/cm	2.00	0.098	mS/cm

After Adjustment ; at 84.0 µS/cm, 1413 µS/cm, 12.88 mS/cm

Standard Conductivity Solution		Unit Under Calibration Reading		Correction		Coverage Factor (k)	Uncertainty (±)	
84.000	µS/cm	84.09	µS/cm	-0.090	µS/cm	2.00	0.68	µS/cm
1413.0	µS/cm	1413	µS/cm	0.0	µS/cm	2.00	11	µS/cm
12.881	mS/cm	12.89	mS/cm	-0.0090	mS/cm	2.00	0.098	mS/cm

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2216356

ชนิดเครื่องมือ: CONDUCTIVITY METER รุ่น: ORION STAR A215 หมายเลขเครื่อง: X58031

ตรวจสอบ (รับ) 03 Jan 2023 ปกติ	ตรวจสอบ (รับ) 03 Jan 2023 ไม่ปกติ	รายการตรวจเช็ค	ตรวจสอบ (ส่ง) 03 Jan 2023 ปกติ	ตรวจสอบ (ส่ง) 03 Jan 2023 ไม่ปกติ	หมายเหตุ
		General			
☑	☐	1. ความสมบูรณ์เครื่อง	☑	☐	
☑	☐	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	☑	☐	
☑	☐	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Swicth)	☑	☐	
☑	☐	4. ปุ่มกด (Keypad)	☑	☐	
☑	☐	5. หน้าจอ (Display, Screen Contrast)	☑	☐	
		Spectrophotometer			
☐	☐	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	☐	☐	
☐	☐	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	☐	☐	
☐	☐	8. ความยาวคลื่น (Wavelength Check)	☐	☐	
☐	☐	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	☐	☐	
☐	☐	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	☐	☐	
☐	☐	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	☐	☐	
		pH Meter and Conductivity Meter			
☑	☐	12. อิเล็คโทรด (Electrode and Connection Cable)	☑	☐	
☐	☐	13. ระดับสารละลายใน Electrode (Level KCl)	☐	☐	
☐	☐	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	☐	☐	
☑	☐	15. ขาจับอิเล็คโทรด (Stand)	☑	☐	
		Turbidimeter			
☐	☐	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	☐	☐	
☐	☐	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	☐	☐	
		Automatic titrator			
☐	☐	18. สภาพ Piston Burettes	☐	☐	
☐	☐	19. Function Rinsing and Dosing	☐	☐	
☐	☐	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	☐	☐	

ข้อแนะนำ : _____

Mr.Nattapat Rungrueang

Service Engineer

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

ภาคผนวก ณ

สำเนาหนังสืออนุญาตขึ้นทะเบียน

ห้องปฏิบัติการวิเคราะห์เอกชน



ที่ อก ๐๓๑๐(๑)/ ๓๐๖๙

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ เขตราชเทวี
กรุงเทพมหานคร ๑๐๔๐๐

๒๘ มกราคม ๒๕๖๕

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๓๐ กรกฎาคม ๒๕๖๓

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ แผ่น
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๖๒ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๕๙ รายการ น้ำใต้ดิน จำนวน ๑๒๖ รายการ อากาศเสีย ๑๖ รายการ สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน ๓๕ รายการ และดิน จำนวน ๑๒๕ รายการ รวมทั้งสิ้นจำนวน ๓๖๑ รายการ ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กันยายน ๒๕๖๖ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๒๐๒ ๔๑๔๖ ๐ ๒๒๐๒ ๔๐๐๒
โทรสาร ๐ ๒๓๕๔ ๓๒๐๘ ๐ ๒๓๕๔ ๓๔๑๕

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔

ที่ อก ๐๓๑๐(๑)/ ลงวันที่ ๒๘ มกราคม ๒๕๖๔

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย

๑) นางสาวยุพาพร จันทร์เปล่ง	ทะเบียนเลขที่ ว-๒๐๔-ค-๔๗๐๐
๒) นางสาวชัชนัย โกมารกุล ณ นคร	ทะเบียนเลขที่ ว-๒๐๔-ค-๔๗๐๑
๓) นายศรายุทธ จิตรานนท์	ทะเบียนเลขที่ ว-๒๐๔-ค-๔๗๐๒
๔) นางสาวกนกกร เอนก	ทะเบียนเลขที่ ว-๒๐๔-ค-๖๑๑๑
๕) นายสุริยา สอนแก้ว	ทะเบียนเลขที่ ว-๒๐๔-ค-๖๑๑๒
๖) นายวิชาญ ชุณหรัต	ทะเบียนเลขที่ ว-๒๐๔-ค-๖๑๑๓

(นายศิระ จันทร์เฉิด)

นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๓๐๖๙ ลงวันที่ ๒๘ มกราคม ๒๕๖๕

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๖๒ ราย

๑) นางสาวจินดา โขจุลธรรม ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๐๘
๒) นางสาวสาวิตรี น้อยเสงี่ยม ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๐๙
๓) นางสาวชณัฐกาญจน์ อิ่มชม ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๐
๔) นางสาวนรินทร์ สายเส็ง ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๕
๕) นางสาวนันทวดี สมบูรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๖
๖) นางสาวศรัณยา เฉลิมธำรงค์ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๗
๗) นางสาวสรารัศมิ์ มงคลจิรวุฒิ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๙
๘) นางสาวศิริลักษณ์ พึ่งแพง ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๒๐
๙) นายนพพงศ์ จันทรุพันธุ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๐๘
๑๐) นายนรเศรษฐ์ โกมาลย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๑
๑๑) นายธันวา จริยา ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๔
๑๒) นางสาวเกศรินทร์ แก้วมั่น ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๖
๑๓) นางสาวสุวิมล ชัยเรืองวุฒิ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๗
๑๔) นางสาวสุชาดา ธรรมถาวร ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๑
๑๕) นางสาวเปมิกา ชัยเดชธนกุล ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๓
๑๖) นางสาวศศิธร หมูสวัสดิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๔
๑๗) นางสาวเสาวลักษณ์ ภู่นภาอำพร ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๕
๑๘) นายอภิสิทธิ์ สิงหา ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๖
๑๙) นายศักดิ์สิทธิ์ ไพศาลพิสุทธิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๗
๒๐) ว่าที่ร้อยตรีหญิง พรรณิภา ขำเจริญ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๘
๒๑) นางจิลดา คำภูแก้ว ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๓๑
๒๒) นางสาวอรวรรณ รักยง ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๑๕
๒๓) นางสาวนพรัตน์ แย้มกรานต์ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๑๙
๒๔) นายจุลเดช วารินทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๐
๒๕) นางสาวดายุรัตน์ ร้องคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๑
๒๖) นายนคร สุขเจริญ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๒
๒๗) นายบัญชา นามเขตต์ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๓
๒๘) นายพรมมี ศรีปัตเนตร ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๕
๒๙) นายอุทิศ อุ่นสิม ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๖
๓๐) ว่าที่ร้อยตรี เฉลิมเกียรติ อมรศรีเสริม ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๘
๓๑) นางสาววริยา สร้างนา ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๙
๓๒) นายอนุพงศ์ รัตนศรีประเสริฐ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๓๐
๓๓) นางสาวจุฑารัตน์ โอนสันเทียะ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๒๔๒
๓๔) นางสาวจารุวรรณ พิมพ์อภิกฤติยา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๗๖

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

๓๕) นางสาวปรางค์ทิพย์...

๓๕) นางสาวปรางค์ทิพย์ กิจไพศาลศักดิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๗๙
๓๖) นางสาวเตือนใจ ทางกลาง ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๐
๓๗) นางสาวจิราพร ศิริเวช ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๒
๓๘) นายวรากร ผูกรักษ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๓
๓๙) นายทนง วิริยะสหกิจ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๔
๔๐) นายธนิต เจนจบ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๕
๔๑) นายคณิศร ขำเพชร ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๖
๔๒) นายอรรคพล นิยมวิทยาพัน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๗
๔๓) นายภูวิช พรหมสะอาด ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๘
๔๔) นายธนเดช โภคาพิพัฒน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๙
๔๕) นายชวฤทธิ์ วงษ์จันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๐
๔๖) นายอาทิตย์ ศรีเสน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๑
๔๗) นายเจษดินทร์ คงศักดิไทย ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๒
๔๘) นายจรัส บุญยิ่ง ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๕
๔๙) นายธนาณัติ เอนก ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๖
๕๐) นายอภิวัฒน์ ทุมหนู ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๗
๕๑) นางสาวสุภาขวัญ มาก ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๘
๕๒) นางสาวทัตพร ชวาลสมบูรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๐
๕๓) นางสาวธิติมา บุญเพ็ง ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๑
๕๔) นางสาวกนกอร เข็มเพ็ชร ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๒
๕๕) นางสาวพัชรียา หงษ์สมดี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๓
๕๖) นางสาวภานิดา สุรวงศ์ตระกูล ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๔
๕๗) นางสาวภานุมาศ นามวัฒน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๕
๕๘) นางสาวอุไรรัตน์ ทึงสร้างแป้น ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๖
๕๙) นายธีรวัฒน์ ปวงสุข ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๗
๖๐) นายอิทธิพล ยะโส ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๘
๖๑) นายประพจน์ วรรณชูชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๙
๖๒) นายชยธร พวงทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๐
๖๓) นางสาวกนกวรรณ จันทบาล ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๑
๖๔) นางสาวเกษร หลักบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๒
๖๕) นายสิทธิโชค ธงเงิน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๓
๖๖) นางศิลาวรรณ ใจบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๕
๖๗) นางสาวพรรณธิดา พุ่มคง ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๘
๖๘) นางสาวศรวณีย์ ยิ่งดี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๙
๖๙) นายนวภัทร ศรีวิริยะ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๐
๗๐) นายสุวิชา ทองอ่อน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๑
๗๑) นายวิญญู บุญตะนัย ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๓

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

๗๒) นายสมบูรณ์...

๗๒) นายสมบูรณ์ บุตรจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๔
๗๓) นายวิรัตน์ ไชยนะรา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๕
๗๔) นายนฤเบศน์ เพิ่มพูน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๖
๗๕) นายจิรณัฐ ขาวละออ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๗
๗๖) นายสมโภช วันสา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๙
๗๗) นายอัสรี นามบุรี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๑๗
๗๘) นายณัฐนันท์ ปานประเสริฐ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๑๙
๗๙) นายอัศวเรศ จ่อสาว ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๐
๘๐) นายประเสริฐ สุระขันธ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๑
๘๑) นายนุกูล จันทร์เนียม ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๒
๘๒) นายพีรพงษ์ ทองคูณปรีดา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๓
๘๓) นายนฤพล ทองนุช ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๔
๘๔) นายอนุวัฒน์ ม่วงแพร ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๕
๘๕) นายเจตศราวุฒิ ปัตตะมะ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๖
๘๖) นายกฤษณะ สายวรรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๗
๘๗) นายพิชัย บุญยงค์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๘
๘๘) นายภานุพงศ์ โฮมวงศ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๙
๘๙) นายสามารถ คุ้มปลี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๐
๙๐) นายสัญชัย โกศรีนาม ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๑
๙๑) นายณัฐวุฒิ ศรีประเสริฐ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๒
๙๒) นายชวัลธัช นาคพนม ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๓
๙๓) นายพงศธร ชัยทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๕
๙๔) ว่าที่ร้อยตรี ภาณุพงศ์ แสนศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๖
๙๕) นายสิทธิโชค ทาสีดา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๗
๙๖) นายธนากร อินสุตา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๘
๙๗) นางสาววรณิชชา ชาติวันชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๙
๙๘) นางสาวพิมพ์ตะวัน มินากูล ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๔๑
๙๙) นางสาวเพชรัตน์ สิงห์สมบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๔๒
๑๐๐) นางสาวชญานิน พรหมจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๔๓
๑๐๑) นายกีรติ ทวีราช ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๘๖
๑๐๒) นายจักริน หมั่นวิชา ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๘๗
๑๐๓) นายฉัตรชัย สุขเปีย ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๘๘
๑๐๔) นายณรนนท์ ต๊ะทองคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๘๙
๑๐๕) นายดุลยพล สนนอก ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๐
๑๐๖) นายทักษ์ดนัย อุบลศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๑
๑๐๗) นายธนศวร นามะกุณณา ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๒
๑๐๘) นายธิติพงศ์ บัวแดง ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๓

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

๑๐๙) นายนนทชัย...

๑๐๙) นายนนทชัย อุปถัมภ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๔
๑๑๐) นายนัฐพล คุณสุทธิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๕
๑๑๑) นายนันทวัฒน์ สาริน ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๖
๑๑๒) นายปิยะนัฐ พลมะศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๗
๑๑๓) นายพงศ์สิริ โสมเขียว ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๘
๑๑๔) นายพีรพัฒน์ ก่ำคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๙
๑๑๕) นายภาณุพงศ์ มานิตย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๐
๑๑๖) นายมงคล ผลาทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๑
๑๑๗) นายมุนินทร์ พูลศิริ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๒
๑๑๘) นายสิรินนท์ ทองอั้น ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๓
๑๑๙) นายอเนชา ทันสมัย ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๔
๑๒๐) นายอดิศักดิ์ ผมไผ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๕
๑๒๑) นายอนันตชัย วีสม ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๖
๑๒๒) นายณัฐดนัย เจือละออง ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๗
๑๒๓) นายวรวุธ ดีนัก ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๘
๑๒๔) นายแสงตะวัน นะตะสัต ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๙
๑๒๕) นายยุทธพงศ์ รัตนะ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๐
๑๒๖) นายชยัณวุฒิ ไชยฮะนิจ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๑
๑๒๗) นายวิศรุต ศรีธรรมมา ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๒
๑๒๘) นายนนทกร เผือกผ่อง ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๓
๑๒๙) นายกำชัย สุทธะ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๔
๑๓๐) นางสาวณัฐภรณ์ รักทะเล ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๑๙
๑๓๑) นางสาวประภาภรณ์ บุตรพรม ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๐
๑๓๒) นางสาวนิลาวัลย์ นามพรม ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๑
๑๓๓) นางสาวพัชรินทร์ แสนสร้อย ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๒
๑๓๔) นายไพรวัลย์ เปรี่ยมพิมาย ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๓
๑๓๕) นางสาวศุภมาศ ทองมาก ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๔
๑๓๖) นางสาวลลิตา จิตรสว่าง ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๕
๑๓๗) นางสาวชไมพร เสิกภู่เขียว ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๖
๑๓๘) นางสาวกฤติมาพร คำมีแก่น ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๗
๑๓๙) นางสาวสกุลรัตน์ ภาคภูมิ ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๘
๑๔๐) นางสาวกาญจนา คงคูณ ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๙
๑๔๑) นางสาวไพรินทร์ ศรีรูปี ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๐
๑๔๒) นางสาวทิพเนตร ผุยปัญญา ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๑
๑๔๓) นางสาวสาธิตา ปานทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๒
๑๔๔) นางสาวอริสา ทองนวล ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๓
๑๔๕) นางสาวอรยา ค้าคล่อง ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๔

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

๑๔๖) นางสาวชุดาภรณ์...

๑๔๖) นางสาวชุดาภรณ์ สุนทรสนาน	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๕
๑๔๗) นางสาวสุดารัตน์ นนท์ประสาท	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๖
๑๔๘) นางสาวรัชนีกร เนียมกลาง	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๗
๑๔๙) นางสาวกัญญารัตน์ ศรีนิลทา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๘
๑๕๐) นางสาวอัญชลี คำจันทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๙
๑๕๑) นายบุญฤทธิ์ เอี่ยมเทศ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๐
๑๕๒) นายศิริวัฒน์ พานิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๑
๑๕๓) นางสาวศุภรดา ปั้นมยุรา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๒
๑๕๔) นางสาวพาฤดี คุณนาน	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๓
๑๕๕) นางสาวจิราเจต ฟองดา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๔
๑๕๖) นางสาวกนกภรณ์ อุระ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๕
๑๕๗) นางสาวอารยา มีชัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๖
๑๕๘) นางสาวจิตสุภา ประเทืองสุข	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๗
๑๕๙) นางสาวอริสา วิริยขันติธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๘
๑๖๐) นางสาววิชชุตา นาคผจญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๙
๑๖๑) นางสาวพนิดา ยอดอินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๕๐
๑๖๒) นางสาวนันทิยา จันทะลุน	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๕๑

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๑๐๖๙ ลงวันที่ ๒๘ มกราคม ๒๕๖๔

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๖๑ รายการ

น้ำเสีย จำนวน 59 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method[4]
2	Aldicarb Sulfone	High-Performance Liquid Chromatographic Method[4]
3	Aldicarb Sulfoxide	High-Performance Liquid Chromatographic Method[4]
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
5	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
6	Barium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
7	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
8	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
9	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
10	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
11	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method[4] 2) 5-Day BOD Test, Membrane Electrode Method[4]
12	Carbaryl	High-Performance Liquid Chromatographic Method[4]
13	Carbofuran	High-Performance Liquid Chromatographic Method[4]
14	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
15	Chemical Oxygen Demand	1) Closed Reflux, Colorimetric Method[4] 2) Closed Reflux, Tritimetric Method[4]
16	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
17	Chromium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[4]
18	Color	ADMI Weighted-Ordinate Spectrophotometric Method

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

19 Copper...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Copper	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
20	Cyanide	Distillation, Colorimetric Method[4]
21	2,4´-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
22	4,4´-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
23	2,4´-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
24	4,4´-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
25	2,4´-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
26	4,4´-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
27	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
28	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
29	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
30	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
31	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
32	Endrin Aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
33	Formaldehyde	Distillation, Colorimetric Method[3]
34	Free Chlorine	1) DPD Ferrous Titrimetric Method[4] 2) Iodometric Method[4]
35	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
36	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
37	Hexavalent Chromium	Filtration, Colorimetric Method[4]
38	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method[4]
39	Lead	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
40	Manganese	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
41	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma/Mass spectrometric Method[4]
42	Methiocarb	High-Performance Liquid Chromatographic Method[4]
43	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]

44 Methomyl...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
...ปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
44	Methomyl	High-Performance Liquid Chromatographic Method[4]
45	Nickel	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
46	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method[4] 2) Soxhlet Extraction Method[4]
47	Oxamyl	High-Performance Liquid Chromatographic Method[4]
48	Propoxur	High-Performance Liquid Chromatographic Method[4]
49	pH	Electrometric Method[4]
50	Phenols	1) Distillation, Chloroform Extraction Method[4] 2) Distillation, Direct Photometric Method[4]
51	Selenium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
52	Sulfide	Iodometric Method[4]
53	Temperature	Laboratory and Field Methods[4]
54	Total Dissolved Solids	Dried at 180 ^{0}C[4]
55	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method[4]
56	Total Suspended Solids	Dried at 103-105 ^{0}C[4]
57	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
58	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation[4]
59	Zinc	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[4]

<u>น้ำใต้ดิน จำนวน 126 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]

3 Aldrin...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
8	Barium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
13	Benzoic Acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
15	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

18 Bis(2-ethylhexyl)phthalate...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4] Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[4]
22	Butyl Benzyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
27	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

34 Chromium (III)...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation[4]
35	Chromium (VI)	Colorimetric Method[4]
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
37	Cyanide	Distillation, Colorimetric Method[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
39	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
40	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
41	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
43	Di-n-Butyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
47	3,3-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]

51 cis-1,2-Dichloroethylene...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และรองเลขาธิการปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
57	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
58	Diethyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
63	Di-n-Octyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
64	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
65	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

68 Fluorene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
69	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
70	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
74	α-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
75	β-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
76	γ-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
81	Lead	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
83	Mercury	1) Cold Vapor Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

84 Methanol...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
กองทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[4]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
89	2-Methylnapthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
95	N-Nitrosodi-n-Propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB 1242 - PCB 1248 - PCB 1254 - PCB 1260	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

97 Pentachlorophenol...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
98	pH	Electrometric Method[4]
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
100	Phenol	1) Distillation, Direct Photometric Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
102	Selenium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
103	Silver	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
104	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
106	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
107	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
109	TPH (C_5-C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,24]
110	TPH ($C_{>8}$-C_{16})	Solvent Extraction, Gas Chromatographic Method[9,21]
111	TPH ($C_{>16}$-C_{35})	Solvent Extraction, Gas Chromatographic Method[9,21]
112	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
113	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]

114 1,1,2-Trichloroethane...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
114	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
115	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
118	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
119	Vanadium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
120	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
121	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
122	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
123	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
124	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
125	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
126	Zinc	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

<u>อากาศเสีย (ปล่องระบาย) จำนวน 16 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic, Digestion, Inductively Coupled Plasma Method[5]
2	Arsenic	Isokinetic, Digestion, Inductively Coupled Plasma Method[5]

3 Carbon Monoxide...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Carbon Monoxide	1) Sampling Bag Non-Dispersive Infrared Method[5] 2) Non-Dispersive Infrared Method[5] 3) Instrumental Analyzer Method[5]
4	Chlorine	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method [5]
5	Copper	Isokinetic, Digestion, Inductively Coupled Plasma Method[5]
6	Dioxins	Isokinetic Sampling, Analysis by ISO/IEC 17025 Accredited Laboratory or Analysis by Department of Industrial Works Registered Laboratory (Dioxins/Furans Analysis Approved)[5]
7	Hydrogen Chloride	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method[5]
8	Hydrogen Sulfide	Absorption Sampling, Iodometric Method[5]
9	Lead	Isokinetic, Digestion, Inductively Coupled Plasma Method[5]
10	Mercury	1) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[5] 2) Isokinetic, Digestion, Inductively Coupled Plasma Method[5]
11	Opacity	Ringelmann's Method[2]
12	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method[5] 2) Chemiluminescence Method[5] 3) Instrumental Analyzer Method[5]
13	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method[5] 2) UV Fluorescence Method[5] 3) Instrumental Analyzer Method[5]
14	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method[5]
15	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method[5]
16	Xylene	Adsorption Sampling, Gas Chromatographic Method[5]

สิ่งปฏิกูล...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
3	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

6 Cadmium...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,19,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
8	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
9	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method[1,6,15,17] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method[1,6,16,17] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,15,17] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8, 16,17]
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method[1,6,17] 2) Alkaline Digestion, Colorimetric Method[8,17]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

11 Cobalt...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
12	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25]

2) Soxhlet...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
20	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[1,6,18]

2) Waste Extraction...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Waste Extraction, Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method[1,6,19] 3) Waste Extraction, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[1,6,20] 4) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[18] 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method[19] 6) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[20]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
24	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
25	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
26	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

27 Polychlorinated...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

28 Pentachlorophenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
28	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
29	pH	Electrometric Method[29,30]
30	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
31	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16]
32	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
33	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15]

4) Digestion...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
35	Zinc	4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

<u>ดิน จำนวน 125 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
3	Aldrin	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
4	Anthracene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
7	Atrazine	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
8	Barium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

9 Benz(a)anthracene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
9	Benz(a)anthracene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
11	Benzo(b)fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
12	Benzo(k)fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
13	Benzoic acid	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
14	Benzo(a)pyrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
15	Benzo(g,h,i)perylene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
17	Bis(2-chloroethyl)ether	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
18	Bis(2-ethylhexyl)phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
21	Butanol	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[12,24]
22	Butyl Benzyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
24	Carbazole	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

26 Carbon tetrachloride...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
27	Chlordane	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
28	p-Chloroaniline	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
32	2-Chlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,15,17] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,16,17]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method[8,17]
36	Chrysene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
37	Cyanide	Extraction, Distillation, Colorimetric Method[26,27,28]
38	2,4-D	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
39	DDD	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]

40 DDE...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	DDE	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
41	DDT	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
42	Dibenz(a,h)anthracene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
43	Di-n-Butyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
47	3,3-Dichlorobenzidine	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
53	2,4-Dichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]

57 Dieldrin...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
57	Dieldrin	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
58	Diethyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
59	2,4-Dimethylphenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
60	2,4-Dinitrophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
61	2,4-Dinitrotoluene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
62	2,6-Dinitrotoluene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
63	Di-n-Octyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
64	Endosulfan	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
65	Endrin	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
67	Fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
68	Fluorene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
69	Heptachlor	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
70	Heptachlor Epoxide	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]

71 Hexachlorobenzene...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
71	Hexachlorobenzene	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
74	α-HCH	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
75	β-HCH	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
76	γ-HCH	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
77	Hexachlorocyclopentadiene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
78	Hexachloroethane	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
79	Indeno(1,2,3-cd)pyrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
80	Isophorone	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
81	Lead	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[18]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

2) Thermal...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry[19] 3) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[20]
84	Methanol	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[12,24]
85	Methoxychlor	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
88	2-methylphenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
89	2-Methylnaphthalene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
91	Naphthalene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
93	Nitrobenzene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
94	N-Nitrosodiphenylamine	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
95	N-Nitrosodi-n-propylamine	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
96	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232	1) Soxhlet Extraction, Gas Chromatographic Method [10,23] 2) Automated Soxhlet Extraction, Gas Chromatographic Method [23,32]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

- Aroclor 1242...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
	- Aroclor 1242	
	- Aroclor 1248	
	- Aroclor 1254	
	- Aroclor 1260	
	- 2-Chlorobiphenyl	
	- 2,2',3,5'-Tetrachlorobiphenyl	
	- 2,2',5,5'-Tetrachlorobiphenyl	
	- 2,3',4,4'-Tetrachlorobiphenyl	
	- 2,2',3,4,5'-Pentachlorobiphenyl	
	- 2,2',4,5,5'-Pentachlorobiphenyl	
	- 2,3,3',4',6-Pentachlorobiphenyl	
	- 2,2',3,4,4',5'-Hexachlorobiphenyl	
	- 2,2',3,4,5,5'-Hexachlorobiphenyl	
	- 2,2',3,5,5',6-Hexachlorobiphenyl	
	- 2,2',4,4',5,5'-Hexachlorobiphenyl	
	- 2,2',3,3',4,4',5-Heptachlorobiphenyl	
	- 2,2',3,4,4',5,5'-Heptachlorobiphenyl	
	- 2,2',3,4,4',5',6-Heptachlorobiphenyl	
	- 2,2',3,4',5,5',6-Heptachlorobiphenyl	
	- 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	
97	Pentachlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
98	Phenanthrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
99	Phenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
100	Pyrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดลอบมลพิษ
และทะเบียนห้องปฏิบัติการ

101 Selenium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
101	Selenium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
102	Silver	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
103	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
106	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
107	Toxaphene	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
108	TPH (C_5–C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
109	TPH ($C_{>8}$– C_{16})	1) Solvent Extraction, Gas Chromatographic Method[11,21] 2) Automated Soxhlet Extraction, Gas Chromatographic Method[21,31]
110	TPH ($C_{>16}$ – C_{35})	1) Solvent Extraction, Gas Chromatographic Method[11,21] 2) Automated Soxhlet Extraction, Gas Chromatographic Method[21,31]
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
115	2,4,5-Trichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

116 2,4,6-Trichlorophenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
116	2,4,6-Trichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
118	Vanadium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
119	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
120	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
121	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
122	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
123	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
125	Zinc	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.**ราชกิจจานุเบกษา.** 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. **ราชกิจจานุเบกษา.** 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. **คู่มือวิเคราะห์น้ำเสีย.** พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 23rd ed. Washington, DC: APHA, 2017.

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2019.

6. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846,** 1997.

7. United States...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sludges and Sediments and Soils. SW-846 Method 3050B,** 1996.

8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A,** 1996.

9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C,** 1996.

10. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soxhlet Extraction. SW-846 Method 3540C,** 1996.

11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Microscale Solvent Extraction (MSE). SW-846 Method 3570,** 2002.

12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds (VOCs) in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A,** 2014.

13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Purge-and-Trap for Aqueous Samples. SW-846 Method 5030B,** 1996.

14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035,** 1996.

15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma- Atomic Emission Spectrometry. SW-846 Method 6010B,** 1996.

16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Mass Spectrometry. SW-846 Method 6020A,** 2007.

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A,** 1992.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B,** 2007.

19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473,** 2007

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

20. United States...

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Sediment and Tissue Sample by Atomic Fluorescence Spectrometry. SW-846 Method 7474,** 2007.

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID.SW-846 Method 8015B,** 1996.

22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B,** 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinate Biphenyls (PCBs) by Gas Chromatography. SW-846 Method 8082,** 1996.

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8260D,** 2018.

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8270E,** 2018.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation SW-846 Method 9010B,** 1996.

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A,** 1996.

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014,** 2014.

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C,** 2004.

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soil and Waste pH. SW-846 Method 9045D,** 2004.

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Automated Soxhlet Extraction. SW-846 Method 3541,** 1994.

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ



ที่ อก ๐๓๑๐(๑)/ ๕๓๗๙

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๙ มีนาคม ๒๕๖๖

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๔ กุมภาพันธ์ ๒๕๖๖

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๙ ราย

๑) นายนคร สุขเจริญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๒
๒) นายบัญชา นามเขตต์	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๓
๓) นายอรรคพล นิยมวิทยาพัน	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๗
๔) นางสาวพัชรียา หงษ์สมดี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๓
๕) นางสาวภานิดา สุรวงศ์ตระกูล	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๔
๖) นางสาวศรวณีย์ ยิ่งดี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๙
๗) นายสมโภช วันสา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๙
๘) นายณัฐนันท์ ปานประเสริฐ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๑๙
๙) ว่าที่ร้อยตรีภาณุพงศ์ แสนศรี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๖
๑๐) นายมุนินทร์ พูลศิริ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๒
๑๑) นายณัฐดนัย เจือละออง	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๗
๑๒) นางสาวกาญจนา คงคูณ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๙
๑๓) นางสาวรัชนีกร เนียมกลาง	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๗
๑๔) นางสาวกัญญารัตน์ ศรีนิลทา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๘
๑๕) นายศิริวัฒน์ พานิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๑
๑๖) นางสาวกนกภรณ์ อุระ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๕
๑๗) นางสาวจิตสุภา ประเทืองสุข	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๗
๑๘) นางสาวอริสา วิริยขันติธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๘
๑๙) นางสาวพนิดา ยอดอินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๕๐

๒. ให้เพิ่มเจ้าหน้าที่...

๒. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ ราย

๑) นายกาจบัณฑิต กิตติศุภวณิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๑
๒) นายภัทรพล สว่างใจธรรม์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๒
๓) นายนราธิป เทือกชัยคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๓
๔) นายศิริโชค พงษ์ประสม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๔
๕) นายณัฐวุฒิ ด้วงแพง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๕

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ที่ อก ๐๓๑๐(๑)/๑๐๖๙ ลงวันที่ ๒๘ มกราคม ๒๕๖๔ คือในวันที่ ๒ กันยายน ๒๕๖๖ ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางริกาญจน์ ฉัตรสกุลวิไล)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ที่ อก ๐๓๑๐(๑)/ ๖๑๒๕

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๓ มีนาคม ๒๕๖๖

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑๐ มีนาคม ๒๕๖๖

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เปลี่ยนแปลงชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จากเดิม นางสาวสรารัศมิ์ มงคลจิรวุฒิ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๙ เป็น นางสาวธัญญธร มงคลจิรวุฒิ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๙

ทั้งนี้ หากท่านมีความประสงค์จะยื่นคำขอใดๆ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์

คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน

วันที่ 4 **เดือน** สิงหาคม **พ.ศ** 2566

ข้าพเจ้า ( ) ผู้รับใบอนุญาตประกอบกิจการโรงงาน .....

(√) บริษัท/ห้างหุ้นส่วนจำกัด เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

ตั้งอยู่ที่เลขที่ 104 หมู่ที่ - ตรอก/ซอย พัฒนาการ 40

ถนน พัฒนาการ ตำบล/แขวง พัฒนาการ

อำเภอ/เขต สวนหลวง จังหวัด กรุงเทพมหานคร รหัสไปรษณีย์ 10250

โทรศัพท์ 02 760-3040 โทรสาร 0 2 760-3197

ได้รับทราบระเบียบกรมโรงงานอุตสาหกรรมว่าด้วยการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน พ.ศ. 2560 โดยตลอดแล้วและยินยอมปฏิบัติตามระเบียบฯทุกประการ และได้แนบเอกสารต่างๆ ตามรายการเอกสารประกอบการพิจารณา (แบบ ปอ.1-1) มาพร้อมนี้

กองวิจัยและเตือนภัยมลพิษโรงงาน
รับที่ 1656/66
วันที่ 2 ส.ค. 2566
เวลา 10.54 น.

<u>รายการขอดำเนินการ</u>

การดำเนินการ	รายละเอียด (รายการ)				
	น้ำเสีย/น้ำทิ้ง	น้ำใต้ดิน	อากาศเสีย	สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว	ดิน
[ ] ขอขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน					
[√] ต่ออายุห้องปฏิบัติการวิเคราะห์เอกชน	59	126	16	35	125
[√] เปลี่ยนแปลงสารมลพิษที่วิเคราะห์ (√) เพิ่มสารมลพิษ ( ) ยกเลิกสารมลพิษ	-	-	12	-	-
[√] เปลี่ยนแปลงบุคลากร (√) เพิ่มบุคลากร (√) ยกเลิกบุคลากร	จำนวน 38 ราย (รายละเอียดตาม แบบ ปว.1) จำนวน 2 ราย (รายละเอียดตาม แบบ ปว.1)				
[ ] ยกเลิกห้องปฏิบัติการวิเคราะห์เอกชน					
[ ] อื่นๆ ..โปรดระบุ.....					

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ
รับที่ ๕๕๕/๖๖
วันที่ ๗ ส.ค. ๖๖
เวลา ๑๓.๐๘ น.

จึงเรียนมาเพื่อโปรดพิจารณา

ลงชื่อ .....

(นางทัศนีย์ เลขากุลพร)

ผู้มีอำนาจลงนามแทนนิติบุคคล

ประทับตรา (ถ้ามี)

เรียน กวท.
เพื่อโปรดพิจารณา

(นายประสม ดำรงพงษ์)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

ALS Laboratory Group (Thailand) Co., Ltd.



ที่ อก ๐๓๑๐(๓)/ ๖๔๗๐

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๘ มิถุนายน ๒๕๖๔

เรื่อง ขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๙ เมษายน ๒๕๖๔

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๒ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน พร้อมรายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ และรายการสารมลพิษที่จะทำการวิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน มีเลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

๑) นายเดช ช้างชน	ทะเบียนเลขที่ ว-๓๒๓-ค-๙๔๔๒
๒) นางวิลาวัณย์ บริรักษ์	ทะเบียนเลขที่ ว-๓๒๓-ค-๙๔๔๓
๓) นายสุพจน์ สลามเต๊ะ	ทะเบียนเลขที่ ว-๓๒๓-ค-๙๔๔๔

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์

๑) นางสาวนฤมล บรรจงกิจ	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๔๕
๒) นางพจนา สีดา	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๔๖
๓) นางสาวธนิตา กุลสุริวงศ์	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๔๗
๔) นายพิทยา ทองแตง	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๔๘
๕) นางชลธิชา สุบงกช	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๔๙
๖) ว่าที่ ร.ต.รณชัย ม่วงมา	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๐
๗) นายวราวุฒิ พับพา	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๑
๘) นายศักดิ์นรินทร์ จรัสกาย	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๒
๙) นายสุรศักดิ์ สาชิน	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๓
๑๐) นางสาวเพชรคุณ ภวภูตานนท์	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๔
๑๑) นายสถาพร ถาแก้ว	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๕
๑๒) นายสุทธิ์ดำรงค์ โชคปิตินันท์	ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๖

๑๓) นายวัลลภ...

๑๓) นายวัลลภ หันไชยเนาว์ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๗
๑๔) นางสาววนาลี เหรียญตระกูล ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๘
๑๕) นางสาววนิดา ผดุงจิตต์ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๕๙
๑๖) นายธนะสิทธิ์ วงศ์ษาไชย ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๐
๑๗) นายชัยนุสรณ์ เลิศนันทกุลชัย ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๑
๑๘) นายสัจจา เพ็ชรแสวง ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๒
๑๙) นายกันตภณ มณีสัมพันธ์ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๓
๒๐) นางสาวจันทนีย์ โกเมนชนะ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๔
๒๑) นายธารินทร์ อ๊อกจินดา ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๕
๒๒) นายศุภณัฐ พิสัยพันธ์ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๖
๒๓) นายศุภชัย วงศ์สุริย์ฉาย ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๗
๒๔) นายปฐมพงศ์ กรสวัสดิ์ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๘
๒๕) นายไสว ต้นโพธิ์ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๖๙
๒๖) นางสาวกิตติยา สัญญาอริยาภรณ์ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๐
๒๗) นางสาวเจษฎาพร ศรีบุญเรือง ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๑
๒๘) นางสาวมธุรินทร์ สิงห์เงา ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๒
๒๙) นางสาวธิดารัตน์ ศิริมังคะโร ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๓
๓๐) นายพิพัฒน์ นิภัทร์เศรษฐ์ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๔
๓๑) นายศิริวิทย์ เรืองสม ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๕
๓๒) นายปาราเมศ สัตยาคุณ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๖
๓๓) นายนฤนาท ธรรมสะโร ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๗
๓๔) นางสาวศุภรัตน์ โสจันทร์ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๘
๓๕) นายพชรกร อินทรเสนา ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๗๙
๓๖) นายทิวากร เชื้อมาก ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๘๐
๓๗) นายอนุรักษ์ ทองขจรศักดา ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๘๑
๓๘) นายอภิชาติ วิลาศ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๘๒
๓๙) นายจรัสระวี ศรีรักษา ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๘๓
๔๐) นายประสานมิตร เขื่อนเพชร ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๘๔
๔๑) นายภานุวัฒน์ วังบง ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๘๕
๔๒) นายสันติ ชัยชนะ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๘๖
๔๓) นายสิทธิชัย แก้วเกตุ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๘๗
๔๔) นายทินกร กุลชาติ ทะเบียนเลขที่ ว-๓๒๓-จ-๙๔๘๘

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๑๔ รายการ อากาศเสีย (ปล่องระบาย) จำนวน ๗ รายการ และน้ำใต้ดิน จำนวน ๓ รายการ รวมทั้งสิ้นจำนวน ๒๔ รายการ ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้มีอายุ ๓ ปี นับจากวันที่กรมโรงงานอุตสาหกรรมออกหนังสือ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางจินตา เตชะศรินทร์)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม
๒๘ มิ.ย. ๒๕๖๔

กองวิจัยและเตือนภัยมลพิษโรงงาน
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๘๐๕ ๗๒๖๑-๓
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๓๒๓
ที่ อก ๐๓๑๐(๓)/ ๖๔๗๐ ลงวันที่ ๒๘ มิถุนายน ๒๕๖๔

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๒๔ รายการ

น้ำเสีย จำนวน 14 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method[2]
		2) 5-Day BOD Test, Azide Modification Method[2]
2	Chemical Oxygen Demand	1) Open Reflux, Titrimetric Method[2]
		2) Closed Reflux, Colorimetric Method[2]
		3) Closed Reflux, Titrimetric Method[2]
3	Color	ADMI Weighted – Ordinate Spectrophotometric Method[2]
4	Cyanide	Distillation, Colorimetric Method[2]
5	Formaldehyde	Distillation, Colorimetric Method[1]
6	Free Chlorine	DPD-Ferrous Titrimetric Method[2]
7	Oil and Grease	Liquid-Liquid Partition-Gravimetric Method[2]
8	pH	Electrometric Method[2]
9	Phenols	1) Distillation, Chloroform Extraction Method[2]
		2) Distillation, Direct Photometric Method[2]
10	Sulfide	ZnS Precipitation, Iodometric Method[2]
11	Temperature	Laboratory and Field Method[2]
12	Total Dissolved Solids	Dried at 180 ^{O}C[2]
13	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method[2]
14	Total Suspended Solids	Dried at 103-105 ^{O}C[2]

อากาศเสีย (ปล่องระบาย) จำนวน 7 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Carbon Monoxide	1) Sampling Bag, Non-Dispersive Infrared Method[5]
		2) Instrumental Analyzer Method[8]
2	Hydrogen Sulfide	Absorption Sampling, Iodometric Method[5]
3	Opacity	Ringelmann's Method[3,4]
4	Oxide of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method[6]
		2) Instrumental Analyzer Method[9]
5	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method[5]
		2) Instrumental Analyzer Method[10]

วิชุดา สัมฤทธิ์

(นางสาววิชุดา สัมฤทธิ์ผล)
ผู้อำนวยการ
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

Sulfuric Acid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
6	Sulfuric Acid	Isokinetic Sampling, Barium – Thorin Titrimetric Method[6]
7	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method[7]

น้ำใต้ดิน จำนวน 3 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Cyanide	Distillation, Colorimetric Method[2]
2	pH	Electrometric Method[2]
3	Phenols	Distillation, Direct Photometric Method[2]

เอกสารอ้างอิง

1. ธงชัย พรรณสวัสดิ์ และวิบูลย์ลักษณ์ วิสุทธิศักดิ์, บรรณาธิการ. (2547) **คู่มือวิเคราะห์น้ำเสีย.** พิมพ์ครั้งที่ 4. กรุงเทพฯ: สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย.

2. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 23rd ed. Washington, DC : APHA, 2017

3. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. **ราชกิจจานุเบกษา.** 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

4. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของของหม้อน้ำของโรงงาน. **ราชกิจจานุเบกษา.** 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

5. United States Environmental Protection. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2017.

6. United States Environmental Protection. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2019.

7. United States Environmental Protection. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2020.

8. United States Environmental Protection Agency. **Determination of Carbon Monoxide Emissions from Stationary Sources; Instrumental Analyzer Procedure.** 40 CFR 60. Appendix A Method 10, 2017.

9. United States Environmental Protection Agency. **Determination of Oxide of Nitrogen Emissions from Stationary Sources; Instrumental Analyzer Procedure.** 40 CFR 60. Appendix A Method 7E, 2019.

10. United States Environmental Protection Agency. **Determination of Sulfur Dioxide Emissions from Stationary Sources; Instrumental Analyzer Procedure.** 40 CFR 60. Appendix A Method 6C, 2017.

วิชุดา สัมฤทธิ์

(นางสาววิชุดา สัมฤทธิ์ผล)
ผู้อำนวยการ
ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก

สำเนา

ที่ อก ๐๓๒๐/ ๑๐๕๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๒ มี.ค. ๒๕๖๖

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอเปลี่ยนแปลงบุคลากร ของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑๔ มีนาคม ๒๕๖๖

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

ก. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ ราย

๑) นางสาวเจษฎาพร ศรีบุญเรือง	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๑
๒) นางสาวมธุรินทร์ สิงห์เงา	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๗๒
๓) นางสาววนิดา ผดุงจิตต์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๕๙
๔) นายศุภณัฐ พิสัยพันธ์	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๖๖
๕) นายสิทธิชัย แก้วเกตุ	ทะเบียนเลขที่	ว-๓๒๓-จ-๙๔๘๗

ข. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๒ ราย

๑) นายณัฐพงษ์ เพ็งชาวนา	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๐๑
๒) นางสาวกัลยทรรศน์ รักดี	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๐๒
๓) นางสาวจุฑารัตน์ สีทองหลาง	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๐๓
๔) นางสาวจิตสุภา ประเทืองสุข	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๐๔
๕) นายสรรเสริญ คุ่ยยกสุย	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๐๕
๖) นายณัฐวุฒิ อถมพรมราช	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๐๖
๗) นายจิตกร สีวะสา	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๐๗
๘) นายสิฑปวิชญ์ สุวรรณรัตน์	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๐๘
๙) นายสิทธิพันธ์ เสนาซิว	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๐๙
๑๐) นายอนุเวศน์ เตมา	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๑๐
๑๑) นายสุรวิทย์ นราพงษ์	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๑๑
๑๒) นายอดิศักดิ์ ตะริศูนย์	ทะเบียนเลขที่	ว-๓๒๓-จ-๐๐๑๒

อนึ่ง...

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ที่ อก ๐๓๑๐(๓)/๖๔๗๐ ลงวันที่ ๒๘ มิถุนายน ๒๕๖๔ คือในวันที่ ๒๘ มิถุนายน ๒๕๖๗ ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรมตาม QR Code ท้ายหนังสือนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายทวี อำพาพันธ์)
ผู้อำนวยการศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์



ที่ อก ๐๓๒๐/๒๕๖๓

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๐ พ.ย. ๒๕๖๖

เรื่อง เปลี่ยนแปลงสารมลพิษของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอเปลี่ยนแปลงสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๕ ตุลาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำนวน ๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๓๒๓ สถานที่ตั้งเลขที่ ๖๑๖/๑๐ หมู่ที่ ๕ ตำบลแม่น้ำคู้ อำเภอปลวกแดง จังหวัดระยอง ขอเปลี่ยนแปลงสารมลพิษของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในน้ำเสีย จำนวน ๑๓ รายการ และน้ำใต้ดิน ๓ รายการ ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนที่ อก ๐๓๑๐(๓)/๖๔๗๐ ลงวันที่ ๒๘ มิถุนายน ๒๕๖๔ คือในวันที่ ๒๘ มิถุนายน ๒๕๖๗ ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายทวี อำพาพันธ์)
ผู้อำนวยการศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคตะวันออก
โทร. ๐ ๓๓๑๓ ๖๐๕๙ ต่อ ๕๐๐๑-๒
ไปรษณีย์อิเล็กทรอนิกส์ eirw@diw.mail.go.th

เอกสารแนบท้ายหนังสือเปลี่ยนแปลงสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๓๒๓
ที่ อก ๐๓๒๐/๑๕๑๕๓ ลงวันที่ ๑๐ พ.ย. ๒๕๖๗

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๖ รายการ

น้ำเสีย จำนวน 13 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	1) 5-Day BOD Test, Membrane Electrode Method
		2) 5-Day BOD Test, Azide Modification Method
2	Chemical Oxygen Demand	1) Open Reflux, Titrimetric Method
		2) Closed Reflux, Colorimetric Method
		3) Closed Reflux, Titrimetric Method
3	Color	ADMI Weighted–Ordinate Spectrophotometric Method
4	Cyanide	Distillation, Colorimetric Method
5	Free Chlorine	DPD Ferrous Titrimetric Method
6	Oil and Grease	Liquid-Liquid, Partition-Gravimetric Method
7	pH	Electrometric Method
8	Phenols	1) Distillation, Chloroform Extraction Method
		2) Distillation, Direct Photometric Method
9	Sulfide	ZnS Precipitation, Iodometric Method
10	Temperature	Field Method
11	Total Dissolved Solids	Dried at 180 ^{O}C
12	Total Kjeldahl Nitrogen	Semi-Macro Kjeldahl Method
13	Total Suspended Solids	Dried at 103-105 ^{O}C

น้ำใต้ดิน จำนวน 3 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Cyanide	Distillation, Colorimetric Method
2	pH	Electrometric Method
3	Phenols	Distillation, Direct Photometric Method

เอกสารอ้างอิง

APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24th ed. Washington, DC : APHA, 2023



จัดทำโดย บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

104 ซอยพัฒนาการ 40 ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพฯ 10250
โทรศัพท์ 0-2760-3000 โทรสาร 0-2760-3197

www.alsglobal.com