

ภาคผนวก จ

ใบแสดงการตรวจเทียบเครื่องมือ  
(Calibration Data Sheets)



## High Volume TSP & PM-10 Calibration Data Sheet

Calibration Location : SECOT Co.,Ltd. Calibration Date : Jan 11, 2023  
 Hi-Vol Pump No. : BH-009 Indicator No. : CM-01  
 Amb. Temp (°C) : 27 Press (mmHg) : 760  
 Calibration by : Mr.Nattachai C.

Plate	Indicate (X) ( cm. )	True H <sub>2</sub> O ( in. )	Actual Flow (Y) (cfm)	XY	X <sup>2</sup>	Remark
18	18.60	13.40	60.88	1,132.37	345.96	
13	15.40	10.20	53.45	823.13	237.16	
10	12.20	8.30	48.34	589.75	148.84	
7	8.00	5.20	38.53	308.24	64.00	
5	4.60	3.10	30.04	138.18	21.16	
Sum	58.80	40.20	231.24	2,991.67	817.12	

Calibrated by : Nattachai C. Approved by : Wittaya K.



## High Volume TSP & PM-10 Calibration Data Sheet

Calibration Location : SECOT Co.,Ltd. Calibration Date : Jan 11, 2023  
 Hi-Vol Pump No. : BH-024 Indicator No. : CM-01  
 Amb. Temp (°C) : 27 Press (mmHg) : 760  
 Calibration by : Mr.Nattachai C.

Plate	Indicate (X) ( cm. )	True H <sub>2</sub> O ( in. )	Actual Flow (Y) (cfm)	XY	X <sup>2</sup>	Remark
18	19.00	13.00	59.98	1,139.62	361.00	
13	15.60	10.50	54.21	845.68	243.36	
10	12.20	8.10	47.77	582.79	148.84	
7	8.00	5.20	38.53	308.24	64.00	
5	4.80	3.10	30.04	144.19	23.04	
Sum	59.60	39.90	230.53	3,020.52	840.24	

Calibrated by : Nattachai C. Approved by : Wittaya K.



# NOX-NO Analyzer Performance Test

Date : 9 Jan 23

Temp: (°C) 25

Barometric Pressure: Pb (mmHg) 760

Analyzer Type :	Nox
Brand :	API
Model :	200A
S/N :	1523


Dilutor :	Teledyne 700E 587
Zero Air :	M701 S/N 1044
STD GAS :	EB0108319

NOX-NO Single Point Calibration

Supply Gas	Ref Value	NOX Analyzer Disp.	NO Analyzer Disp.	Slope - Offset
Zero	0.0	2.0	1.0	0.988
Span	447.0	446.6	451.00	0.988

NOX-NO MultiPoint Calibration

Ref Value	NOX Analyzer Disp.	NO Analyzer Disp.	Output Difference	
			NOx Percent Diff abs.	NO Percent Diff abs.
0.00	2.00	1.0	-	-
100.00	98.60	98.1	1.4	1.9
200.00	196.60	195.1	1.7	2.5
400.00	396.70	396.1	0.8	1.0
Average Diff (%)			1.3	1.8

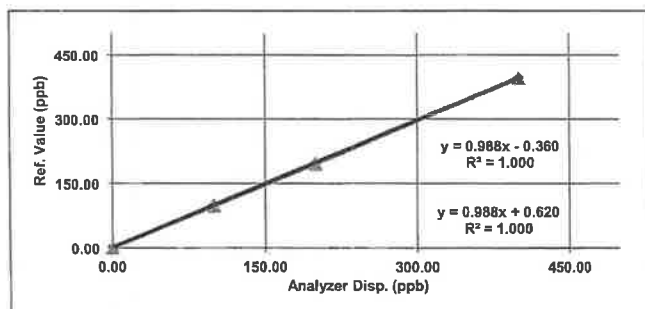Calibrated by : RataniApproved by : M. Haya K.

# NOX-NO Analyzer Performance Test

Date : 9 Jan 23

Temp: (°C) 25

Barometric Pressure: Pb (mmHg) 760

Analyzer Type :	Nox
Brand :	API
Model :	200A
S/N :	1528


Dilutor :	Teledyne 700E 587
Zero Air :	M701 S/N 1044
STD GAS :	EB0108319

NOX-NO Single Point Calibration

Supply Gas	Ref Value	NOX Analyzer Disp.	NO Analyzer Disp.	Slope - Offset
Zero	0.0	0.9	0.5	0.994
Span	450.0	444.4	444.30	0.997

NOX-NO MultiPoint Calibration

Ref Value	NOX Analyzer Disp.	NO Analyzer Disp.	Output Difference	
			NOx Percent Diff abs.	NO Percent Diff abs.
0.00	0.90	0.5	-	-
100.00	98.20	97.7	1.8	2.3
200.00	199.60	198.3	0.2	0.8
400.00	398.80	397.4	0.3	0.7
Average Diff (%)			0.8	1.3

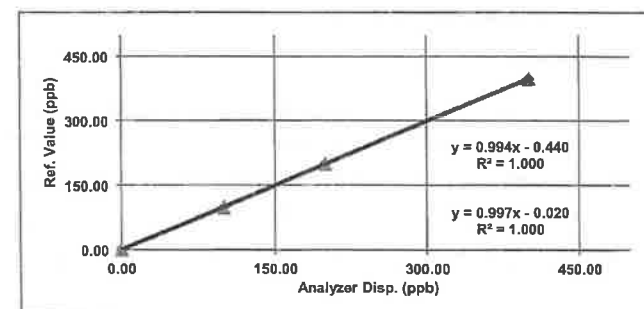Calibrated by : RataniApproved by : M. Haya K.

Sheet No. : CAL-M5006/01/23



## CONTROL UNIT CALIBRATION

(Metric units, mm)

Date 16 Jan 23

Initial Final Average  
Barometric press, Pb 759 759 759 mmHg

## Dry Gas Meter Data

Console No. M50-06

Metering System ID

DGM Number 333249

DGM Model MST-C2-1

Calibrated by : Montri P.

## Reference Dry Gas Meter Data

Serial No. 358794

Model S110

Correction factor (Yr) 1.0079

Last Calibration Date 9 Dec 22

Orifice manometer setting, ΔH mm H2O	Ref. DGM Volume V <sub>r</sub> Liters	DGM Volume V <sub>m</sub> Liters	Temperature (°C)				Time Θ min	DGM Correction factor (Y)	ΔH@ mm
			Ref DGM T <sub>r</sub>	Dry Gas Meter					
				Inlet T <sub>i</sub>	Outlet T <sub>o</sub>	Avg T <sub>m</sub>			
12.5	100.1	100.9	25	25	24	24.5	8.60	0.9968	41.8649
25.0	100.0	100.4	25	25	24	24.5	6.13	0.9998	42.6722
50.0	100.1	100.6	25	25	24	24.5	4.53	0.9963	46.5503
76.0	99.9	100.4	25	25	24	24.5	3.75	0.9949	48.5425
100.0	100.0	99.3	25	25	24	24.5	3.75	1.0031	45.5096
150.0	100.2	98.7	25	25	24	24.5	2.58	1.0070	45.2316

Average 0.9997 45.0618

Approved by : Ladawan W.

Sheet No. : CAL-M509/01/23



## CONTROL UNIT CALIBRATION

(Metric units, mm)

Date 16 Jan 23

Initial Final Average  
Barometric press, Pb 759 759 759 mmHg

## Dry Gas Meter Data

Console No. M50-09

Metering System ID

DGM Number 972135

DGM Model ES-110

Calibrated by : Montri P.

## Reference Dry Gas Meter Data

Serial No. 358794

Model S110

Correction factor (Yr) 1.0079

Last Calibration Date 9 Dec 22

Orifice manometer setting, ΔH mm H2O	Ref. DGM Volume V <sub>r</sub> Liters	DGM Volume V <sub>m</sub> Liters	Temperature (°C)				Time ⊙ min	DGM Correction factor (Y)	ΔH@ mm
			Ref DGM T <sub>r</sub>	Dry Gas Meter					
				Inlet T <sub>i</sub>	Outlet T <sub>o</sub>	Avg T <sub>m</sub>			
12.5	100.3	101.9	25	25	24	24.5	9.72	0.9891	53.2869
25.0	100.0	101.6	25	25	24	24.5	6.50	0.9882	47.9400
50.0	100.1	100.5	25	25	24	24.5	4.80	0.9973	52.2127
76.0	100.1	99.3	25	25	24	24.5	3.72	1.0070	47.5062
100.0	100.3	99.0	25	25	24	24.5	3.72	1.0089	47.2038
150.0	100.3	99.0	25	25	24	24.5	2.58	1.0050	45.1359

Average 0.9992 48.8809

Approved by : Ladawan W.



## PITOT TUBE CALIBRATION

Calibration Location: SECOT

Calibration Date : 06-01-2023

Calibrated duct No.: 1

Calibration Standard Pitot tube data

Pitot No. : Std-01

Coefficient (Cp) : 1

Type S Pitot No. : PS20-01

Calibrated by : Mr. Montri P.

## A Side Calibration

Run No.	$\Delta P_{std}$ (mm H <sub>2</sub> O)	$\Delta P_s$ (mm H <sub>2</sub> O)	Cp(s)	Deviation, $\delta$ Cp(s) - Cp(A)
1	7.50	10.75	0.8353	-0.0033
2	7.50	10.50	0.8452	0.0066
3	7.50	10.75	0.8353	-0.0033

C<sub>P(A),avg</sub> 0.8386

## B Side Calibration

Run No.	$\Delta P_{std}$ (mm H <sub>2</sub> O)	$\Delta P_s$ (mm H <sub>2</sub> O)	Cp(s)	Deviation, $\delta$ Cp(s) - Cp(B)
1	7.50	10.50	0.8452	0.0033
2	7.50	10.75	0.8353	-0.0066
3	7.50	10.50	0.8452	0.0033

C<sub>P(B),avg</sub> 0.8419

|CP(A)-CP(B)| = 0.0033

C<sub>P(Avg)</sub> = 0.8402

Approved by : Ladawan W.

\*\*\*  $\delta$  must be  $\leq 0.01$  for the test to be acceptable \*\*\*  
 \*\*\* |CP(A)-CP(B)| must also be  $< 0.01$  if average of Cp(A) and Cp(B) is not be used \*\*\*



## PITOT TUBE CALIBRATION

Calibration Location: SECOT

Calibration Date : 06-01-2023

Calibrated duct No.: 1

Calibration Standard Pitot tube data

Pitot No. : Std-01

Coefficient (Cp) : 1

Type S Pitot No. : PS20-02

Calibrated by : Mr. Montri P.

## A Side Calibration

Run No.	$\Delta P_{std}$ (mm H <sub>2</sub> O)	$\Delta P_s$ (mm H <sub>2</sub> O)	Cp(s)	Deviation, $\delta$ Cp(s) - Cp(A)
1	7.50	10.75	0.8353	0.0032
2	7.50	11.00	0.8257	-0.0064
3	7.50	10.75	0.8353	0.0032

C<sub>P(A),avg</sub> 0.8321

## B Side Calibration

Run No.	$\Delta P_{std}$ (mm H <sub>2</sub> O)	$\Delta P_s$ (mm H <sub>2</sub> O)	Cp(s)	Deviation, $\delta$ Cp(s) - Cp(B)
1	7.50	10.75	0.8353	-0.0033
2	7.50	10.50	0.8452	0.0066
3	7.50	10.75	0.8353	-0.0033

C<sub>P(B),avg</sub> 0.8386

|CP(A)-CP(B)| = 0.0065

C<sub>P(Avg)</sub> = 0.8353

Approved by : Ladawan W.

\*\*\*  $\delta$  must be  $\leq 0.01$  for the test to be acceptable \*\*\*  
 \*\*\* |CP(A)-CP(B)| must also be  $< 0.01$  if average of Cp(A) and Cp(B) is not be used \*\*\*

Certificate Of Analysis  
Special Gases Mixture

## Customer Details

Name: Secot Co., Ltd. Address: 239 Rimklongprpa Rd. Bangsue Khet Bangsue Bangkok 10800 Customer Tag No.:

## Certificate Details

Number: 0499/23 Date of Issue: 23-Feb-2023 Expiry date: 22-Feb-2027  
Material Details  
Production Order: 90176404 Material Code: 429900-J-62 Cylinder No.: 44157  
Gas content: 6.560 M<sup>3</sup> (nominal) Filling pressure: 145 bar (g) Valve: CGA 590 BRASS  
Cylinder Owner: LINDE Cylinder Material: STEEL Cylinder Size: 47 L

## Laboratory Report

Component	Normal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>
Oxygen	15.0%	15.1%	± 2% relative	(2) I-PB-354
In Nitrogen				

## Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.

Storage condition: Keep in well ventilation and secure area.

## Comments

## Note:

- All results expressed in this report are on mole/mole basis, unless otherwise specified.
- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
- (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasontorn  
Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Certificate Of Analysis  
Special Gases Mixture

## Customer Details

Name: Secot Co., Ltd. Address: 239 Rimklongpropa Rd. Bangsue Khet Bangsue Bangkok 10800 Customer Tag No.:

## Certificate Details

Number: 0484/23 Date of Issue: 22-Feb-2023 Expiry date: 21-Feb-2027  
Material Details  
Production Order: 90176403 Material Code: 478100-J-62 Cylinder No.: 12360  
Gas content: 6.520 M<sup>3</sup> (nominal) Filling pressure: 145 bar (g) Valve: CGA 590 BRASS  
Cylinder Owner: LINDE Cylinder Material: STEEL Cylinder Size: 47 L

## Laboratory Report

Component	Normal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>
Oxygen	8.00%	7.94%	± 2% relative	(1) SG-O-01
In Nitrogen				

## Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.

Storage condition: Keep in well ventilation and secure area.

## Comments

## Note:

- All results expressed in this report are on mole/mole basis, unless otherwise specified.
- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
- (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasontorn  
Signatory for and on behalf of Linde (Thailand) Co., Ltd.



### Certificate Of Analysis

Special Gases Mixture

#### Customer Details

Name: Secot Co., Ltd. Address: 239, Rimklongprapa Rd., Bangsue, Bangkok 10800 Customer Tag No.:

#### Certificate Details

Number: 0329/22 Date of Issue: 9-Feb-2022 Expiry date: 9-Feb-2024  
 Material Details  
 Production Order: 90169718 Material Code: S11500-SK-34 Cylinder No.: D636060  
 Gas content: 5.20 M<sup>3</sup> Filling pressure: 137.0 bar Valve: CGA 660 SS  
 Cylinder Owner: LINDE Cylinder Material: Spectra seal Cylinder Size: 40 L

#### Laboratory Report

##### Analytical Result

Component	Normal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>	Assay Date
Nitric Oxide	20.0 ppm	19.8 ppm	± 1% relative	(6) I-PB-352	1-Feb & 8-Feb-22
Other NOx impurity		Less than 0.9 ppm			
Carbon Monoxide	20.0 ppm	20.0 ppm	± 1% relative	(6) I-PB-352	1-Feb & 8-Feb-22
In Nitrogen					

##### Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Nitric Oxide	13326156	25.61 ± 0.13 ppm	6-May-2023
Carbon Monoxide	ND52320	25.03 ± 0.13 ppm	7-Oct-2023
In Nitrogen			

##### Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-NO	1-Feb-2022
FTIR Spectrometers Nicolet iS50	FTIR-CO	28-Jan-2022

#### Recommend usage condition

Minimum utilization: 5% of actual content or before expiry date whichever comes first.  
 Storage condition: Keep in well ventilation and secure area.

#### Comments

When reordering, please quote the material number

#### Note:

1. All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1.
2. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
3. (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Page 1 of 1

This report shall not be reproduced except in full

บริษัท สยาม (ประเทศไทย) จำกัด (มหาชน)

15 Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangnaew

Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93 Fax (66) 38.570-323

Sukanya Parinyasontorn

Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Linde (Thailand) Public Company Limited

Iss:K/2, 15 Oct 2021

15 Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangnaew

Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93 Fax (66) 38.570-323

PB-002/F006



### Certificate Of Analysis

Special Gases Mixture

#### Customer Details

Name: Secot Co., Ltd. Address: 239, Rimklongprapa Rd., Bangsue, Bangkok 10800 Customer Tag No.:

#### Certificate Details

Number: 0330/22 Date of Issue: 8-Feb-2022 Expiry date: 8-Feb-2024  
 Material Details  
 Production Order: 90169720 Material Code: 436700-SK-34 Cylinder No.: D636021  
 Gas content: 5.23 M<sup>3</sup> Filling pressure: 137.0 bar Valve: CGA 660 SS  
 Cylinder Owner: LINDE Cylinder Material: Spectra seal Cylinder Size: 40 L

#### Laboratory Report

##### Analytical Result

Component	Normal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>	Assay Date
Nitric Oxide	80.0 ppm	78.5 ppm	± 1% relative	(6) I-PB-352	1-Feb & 8-Feb-22
Other NOx impurity		Less than 3.9 ppm			
Carbon Monoxide	80.0 ppm	81.1 ppm	± 1% relative	(6) I-PB-352	1-Feb & 8-Feb-22
In Nitrogen					

##### Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Nitric Oxide	D022358	70.7 ± 0.2 ppm	5-Mar-2023
Carbon Monoxide	D022358	70.8 ± 0.2 ppm	5-Mar-2023
In Nitrogen			

##### Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-NO	10-Jan-2022
FTIR Spectrometers Nicolet iS50	FTIR-CO	8-Jan-2022

#### Recommend usage condition

Minimum utilization: 5% of actual content or before expiry date whichever comes first.  
 Storage condition: Keep in well ventilation and secure area.

#### Comments

When reordering, please quote the material number

#### Note:

1. All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1.
2. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
3. (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Page 1 of 1

This report shall not be reproduced except in full

บริษัท สยาม (ประเทศไทย) จำกัด (มหาชน)

15 Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangnaew

Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93 Fax (66) 38.570-323

Sukanya Parinyasontorn

Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Linde (Thailand) Public Company Limited

Iss:K/2, 15 Oct 2021

15 Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangnaew

Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93 Fax (66) 38.570-323

PB-002/F006



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-66/0270

MTC.No.23-66/0270-01

Number of page(s) 2

## CALIBRATION CERTIFICATE

### Nomenclature : DRYCAL

Manufacturer : Mesa Labs

Serial No.: 114069

Model : Defender 520-H

Scale range : 300 ml/min to 30,000 ml/min

Subdivision : ( 0.0001, 0.001 ) L/min

Submitted by : SECOT CO.,LTD.

239, Rimklongprapa Road, Bangsue,  
Bangkok 10800, Thailand.

Received date : 23 February 2023 Condition of measured item : Normal

Calibration date : 7 March 2023

Standard	Certificate No.	Date due	Traceability
RTD Thermometer	PSL-T 643/65	1-Jun-24	TISTR
Primary Flow Calibrator S/N 119521	MW-0012-21	31-Mar-23	NIMT
Primary Flow Calibrator S/N 119216	MW-0013-21	25-Mar-23	NIMT

Calibrated by : *Terasak Panna*

(Mr.Terasak Panna)

Approved by : *Ms. Kirana Luanghirun*

(Ms.Kirana Luanghirun)

Director

Mechanical Engineering Standards Laboratory

Ref. 2013266022300798001

Issued Date 13 March 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-66/0270

2/2

MTC.No.23-66/0270-01

Calibration point : (1.5, 5.0, 10, 15, 25) L/min

Ambient condition : Temperature ( 23 ± 3 ) °C , Relative humidity ( 55 ± 15 ) %

Atmospheric pressure ( 1010±13 ) hPa

Calibration method : The flowmeter (UUC) was calibrated by comparison method with  
standard flowmeter according to CP-370.01.

The reported value is the value that converted to value at reference condition  
within pressure and temperature of the actual gas entering the UUC

### Measurement data :

UUC Value (L/min)	Standard Value (L/min)	Temperature (°C)	Pressure (hPa)	Deviation (%)	Uncertainty (%)
1.5038	1.5112	24.852	1008.50	-0.49	0.86
5.0113	5.0314	24.854	1008.82	-0.40	0.86
10.077	10.058	24.851	1009.71	+0.19	0.96
15.071	15.038	24.900	1010.91	+0.22	0.96
25.077	24.983	24.914	1014.55	+0.38	0.96

The reported expanded uncertainties are based on standard uncertainties multiplied by  
a coverage factor  $k=2$ , which provides a level of confidence of approximately 95%.

The end of calibration certificate.

T<sub>g</sub>

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th





THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-66/0270

MTC.No.23-66/0270-02

Number of page(s) 2

## CALIBRATION CERTIFICATE

**Nomenclature : DRYCAL**

Manufacturer : Mesa Labs

Serial No.: 160100

Model : Defender 520-L

Scale range : 5 ml/min to 500 ml/min

Subdivision : ( 0.001, 0.01 ) ml/min

**Submitted by : SECOT CO.,LTD.**

239, Rimklongprapa Road, Bangsue,

Bangkok 10800, Thailand.

**Received date :** 23 February 2023 **Condition of measured item :** Normal

**Calibration date :** 8 March 2023

**Standard :**

Standard	Certificate No.	Date due	Traceability
RTD Thermometer	PSL-T 643/65	1-Jun-24	TISTR
Primary Flow Calibrator S/N 117982	MW-0011-21	8-Apr-23	NIMT

**Calibrated by :** Terasak Panna

(Mr.Terasak Panna)

**Approved by :**

(Ms.Kirana Luanghirun)

Director

Mechanical Engineering Standards Laboratory

Ref. 2013266022300798002

Issued Date 13 March 2023

The results relate only to the items tested/calibrated or value assigned

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Mechanical Engineering Standards Laboratory Soi 1, Bangpoo Industrial Estate, Muang, Samutprakan 10280, Thailand.

Request No.23-66/0270

2/2

MTC.No.23-66/0270-02

**Calibration point :** (20, 50, 100, 200, 400) ml/min

**Ambient condition :** Temperature ( 23 ± 3 ) °C , Relative humidity ( 55 ± 15 ) %

Atmospheric pressure ( 1010±13 ) hPa

**Calibration method :** The flowmeter (UUC) was calibrated by comparison method with standard flowmeter according to CP-370.01.

The reported value is the value that converted to value at reference condition within pressure and temperature of the actual gas entering the UUC

**Measurement data :**

UUC Value (ml/min)	Standard Value (ml/min)	Temperature (°C)	Pressure (hPa)	Deviation (%)	Uncertainty (%)
20.138	19.883	24.930	1008.44	+1.28	1.17
51.152	50.908	24.920	1008.44	+0.48	1.02
101.04	100.71	24.897	1008.43	+0.33	1.06
200.25	199.64	24.904	1008.54	+0.31	1.01
401.00	396.85	24.837	1008.80	+1.05	1.00

The reported expanded uncertainties are based on standard uncertainties multiplied by a coverage factor  $k=2$ , which provides a level of confidence of approximately 95%.

The end of calibration certificate.

The results relate only to the items tested/calibrated or value assigned

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 18, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
CIRRUS	RC 110A	95168	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Cirrus	CR110A	CB1101	114.1	-0.1
2	Cirrus	CR110A	CB1102	114.0	0.0
3	Cirrus	CR110A	CB1103	114.4	-0.4

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 18, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
PULSAR	22R	79781	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Pulsar	22	PB614	114.1	-0.1
2	Pulsar	22	PB617	114.7	-0.7
3	Pulsar	22	PB618	114.0	0.0
4	Pulsar	22	PB632	114.4	-0.4
5	Pulsar	22	PB636	114.3	-0.3
6	Pulsar	22	PB637	114.2	-0.2

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 29, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
CIRRUS	RC 110A	95168	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Cirrus	CR110A	CB1041	114.2	-0.2
2	Cirrus	CR110A	CB1042	114.1	-0.1
3	Cirrus	CR110A	CB1043	114.1	-0.1
4	Cirrus	CR110A	CB1047	114.3	-0.3

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 29, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
PULSAR	22R	79781	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Pulsar	22	PB614	114.1	-0.1
2	Pulsar	22	PB618	113.8	0.2
3	Pulsar	22	PB621	114.0	0.0
4	Pulsar	22	PB637	114.1	-0.1

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Oct 27, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
CIRRUS	RC 110A	95168	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Cirrus	CR110A	CB1023	114.3	-0.3
2	Cirrus	CR110A	CB1025	114.0	0.0
3	Cirrus	CR110A	CB1026	114.4	-0.4
4	Cirrus	CR110A	CB1040	114.1	-0.1
5	Cirrus	CR110A	CB1041	113.6	0.4
6	Cirrus	CR110A	CB1042	114.3	-0.3
7	Cirrus	CR110A	CB1043	114.5	-0.5

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Oct 27, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
PULSAR	22R	79781	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Pulsar	22	PB614	114.2	-0.2
2	Pulsar	22	PB617	114.6	-0.6
3	Pulsar	22	PB618	113.6	0.4
4	Pulsar	22	PB621	114.2	-0.2
5	Pulsar	22	PB636	114.4	-0.4
6	Pulsar	23	PB637	114.3	-0.3
7	Pulsar	24	PB644	114.0	0.0

Calibrated by :

Approved by :

## CERTIFICATE OF CALIBRATION

ISSUED BY **Noisemeters**

DATE OF ISSUE **16 March 2023** CERTIFICATE NUMBER **189327**

**NoiseMeters**

**NoiseMeters**  
Acoustic House  
Bridlington Road  
Hunmanby  
YO14 0PH  
United Kingdom  
www.noisemeters.com

Page 1 of 1

Test engineer:  
Nigel Smith  
Electronically signed:



### doseBadge Reader

#### Instrument

Manufacturer: Cirrus Research plc  
Model Number: RC:110A

Serial Number: 95168  
Notes:

#### Calibration Procedure

The tests were carried out in accordance with the requirements of IEC 60942:2003 where applicable.

Date of Calibration: 16 March 2023

#### Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

#### Calibration Results

	Level (dB)	Frequency (Hz)	Distortion (% THD + Noise)
Initial	113.90	999.3	0.61
Adjusted	114.00	999.2	0.61
Uncertainty	± 0.11	± 0.14	± 0.10
Tolerances	± 0.60	± 2.00	± 4.00

#### Environmental Conditions

Pressure: 99.27 kPa  
Temperature: 23.3 °C  
Humidity: 37.6 %

#### Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

## CERTIFICATE OF CALIBRATION

ISSUED BY **Noisemeters**

DATE OF ISSUE **28 April 2023** CERTIFICATE NUMBER **191319**

**NoiseMeters**

**NoiseMeters**  
Acoustic House  
Bridlington Road  
Hunmanby  
YO14 0PH  
United Kingdom  
www.noisemeters.com

Page 1 of 1

Test engineer:  
Rebecca Thomas  
Electronically signed:



### doseBadge Reader

#### Instrument

Manufacturer: Pulsar Instruments Plc  
Model Number: Model 22R

Serial Number: 79781  
Notes:

#### Calibration Procedure

The tests were carried out in accordance with the requirements of IEC 60942:2003 where applicable.

Date of Calibration: 26 April 2023

#### Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

#### Calibration Results

	Level (dB)	Frequency (Hz)	Distortion (% THD + Noise)
Result	114.00	999.0	0.47
Uncertainty	± 0.11	± 0.14	± 0.10
Tolerances	± 0.60	± 2.00	± 4.00

No adjustments were made during this calibration.

#### Environmental Conditions

Pressure: 101.00 kPa  
Temperature: 22.4 °C  
Humidity: 33.7 %

#### Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 18, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
CIRRUS	RC 110A	95168	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Cirrus	CR110A	CB1023	114.0	0.0
2	Cirrus	CR110A	CB1025	113.8	0.2
3	Cirrus	CR110A	CB1026	114.0	0.0
4	Cirrus	CR110A	CB1040	114.1	-0.1
5	Cirrus	CR110A	CB1041	114.0	0.0
6	Cirrus	CR110A	CB1042	113.4	0.6
7	Cirrus	CR110A	CB1043	114.0	0.0

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 18, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
PULSAR	22R	79781	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Pulsar	22	PB621	114.0	0.0
2	Pulsar	22	PB643	113.8	0.2

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 29, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
CIRRUS	RC 110A	95168	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Cirrus	CR110A	CB1048	114.0	0.0
2	Cirrus	CR110A	CB1049	113.9	0.1

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 29, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
PULSAR	22R	79781	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Pulsar	22	PB636	114.2	-0.2
2	Pulsar	22	PB644	114.0	0.0

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Nov 16, 23

### ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
CIRRUS	RC 110A	95168	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Cirrus	CR110A	CB1023	114.1	-0.1
2	Cirrus	CR110A	CB1025	114.2	-0.2
3	Cirrus	CR110A	CB1026	113.7	0.3
4	Cirrus	CR110A	CB1040	114.0	0.0
5	Cirrus	CR110A	CB1041	113.9	0.1
6	Cirrus	CR110A	CB1042	114.2	-0.2
7	Cirrus	CR110A	CB1043	113.9	0.1

Calibrated by :

Approved by :



## NOISE DOSE METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Nov 16, 23

### ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
PULSAR	22R	79781	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Pulsar	22	PB617	114.5	-0.5
2	Pulsar	22	PB618	114.3	-0.3
3	Pulsar	22	PB621	114.1	-0.1
4	Pulsar	22	PB636	114.4	-0.4
5	Pulsar	22	PB637	114.2	-0.2
6	Pulsar	22	PB644	114.1	-0.1

Calibrated by :

Approved by :



# CERTIFICATE OF CALIBRATION

ISSUED BY Noisemeters

DATE OF ISSUE 16 March 2023 CERTIFICATE NUMBER 189327

NoiseMeters

NoiseMeters  
Acoustic House  
Bridlington Road  
Hunmanby  
YO14 0PH  
United Kingdom  
www.noisemeters.com

Page 1 of 1

Test engineer:  
Nigel Smith  
Electronically signed:



## doseBadge Reader

### Instrument

Manufacturer: Cirrus Research plc Serial Number: 95168  
Model Number: RC:110A Notes:

### Calibration Procedure

The tests were carried out in accordance with the requirements of IEC 60942:2003 where applicable.

Date of Calibration: 16 March 2023

### Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

### Calibration Results

	Level (dB)	Frequency (Hz)	Distortion (% THD + Noise)
Initial	113.90	999.3	0.61
Adjusted	114.00	999.2	0.61
Uncertainty	± 0.11	± 0.14	± 0.10
Tolerances	± 0.60	± 2.00	± 4.00

### Environmental Conditions

Pressure: 99.27 kPa  
Temperature: 23.3 °C  
Humidity: 37.6 %

### Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

# CERTIFICATE OF CALIBRATION

ISSUED BY Noisemeters

DATE OF ISSUE 28 April 2023 CERTIFICATE NUMBER 191319

NoiseMeters

NoiseMeters  
Acoustic House  
Bridlington Road  
Hunmanby  
YO14 0PH  
United Kingdom  
www.noisemeters.com

Page 1 of 1

Test engineer:  
Rebecca Thomas  
Electronically signed:



## doseBadge Reader

### Instrument

Manufacturer: Pulsar Instruments Plc Serial Number: 79781  
Model Number: Model 22R Notes:

### Calibration Procedure

The tests were carried out in accordance with the requirements of IEC 60942:2003 where applicable.

Date of Calibration: 26 April 2023

### Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

### Calibration Results

	Level (dB)	Frequency (Hz)	Distortion (% THD + Noise)
Result	114.00	999.0	0.47
Uncertainty	± 0.11	± 0.14	± 0.10
Tolerances	± 0.60	± 2.00	± 4.00

No adjustments were made during this calibration.

### Environmental Conditions

Pressure: 101.00 kPa  
Temperature: 22.4 °C  
Humidity: 33.7 %

### Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

Sheet No. : NC-74-2023-038



## SOUND LEVEL METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 30, 23

### ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Frequency (Hz)	Ref.Calibrated (dB)	Eff.Calibrated (dB)
RION	NC-74	34283648	1000.00	94.0	94.0

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
13	RION	NL-21	00521703	94.0	0.0
34	RION	NL-21	00187489	93.8	0.2
56	RION	NL-21	00187511	93.6	0.4
66	RION	NL-21	00487723	94.1	-0.1
77	RION	NL-21	00487734	93.8	0.2

Calibrated by :

Approved by :

Preeda S.

NC-74-2023-038/Cal/15/09/2023

SECOT CO., LTD.  
239 Rimklongprapa Rd. Bangsue, Bangkok, 10900, THAILAND  
Tel: (662) 959-3600 Fax: (662) 959-3535  
E-Mail: envserv@secot.co.th

Sheet No. : NC-74-2023-053



## SOUND LEVEL METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Nov 20, 23

### ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Frequency (Hz)	Ref.Calibrated (dB)	Eff.Calibrated (dB)
RION	NC-74	34283648	1000.00	94.0	94.0

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
95	RION	NL-21	00198277	94.0	0.0

Calibrated by :

Approved by :

Preeda S.

NC-74-2023-053/Cal/11/12/2023

SECOT CO., LTD.  
239 Rimklongprapa Rd. Bangsue, Bangkok, 10900, THAILAND  
Tel: (662) 959-3600 Fax: (662) 959-3535  
E-Mail: envserv@secot.co.th



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20230033EA  
Operation No.: CP2023010024

### Certificate of Calibration

Equipment: Sound Calibrator

Manufacturer: RION

Model/Type: NC-74

Serial No.: 34283648

ID No.:

Customer: SECOT Co.,Ltd.

Address: 239 Rimklongprapa Rd., Bangsue,  
Bangkok 10800 Thailand

Received Date: 10 January 2023

Calibrated Date: 13 January 2023

Issued Date: 16 January 2023

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

( Mr. Sittichai Swaksuriyawong )  
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20230033EA

### Calibration Report

Equipment: Sound Calibrator  
Manufacturer: RION  
Model/Type: NC-74  
Serial No.: 34283648  
ID No.:  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 15 ) %  
Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-  
IEC 60942:2017

#### Condition of this result of calibration

##### 1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1020-22	14 June 2023
2) Waveform Generator	33511B	MY52302264	CK20220058EA	19 June 2023
3) Audio Analyzing DMM	2015-P	4079144	E1U221042	16 March 2023
4) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P220024 CD20220165EA	17 March 2023 24 July 2023

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

#### Result of Calibration:-

##### 1. Function : Sound pressure level

Normal	Specified Sound	Measured value	Deviated value <sup>[1]</sup>	Acceptance limit <sup>[3]</sup>
Frequency (Hz)	Pressure level (dB)	(dB)	(dB)	(dB)
1000	94	94.24	0.24	±0.25

##### 2. Function : Frequency

Normal Sound	Specified Frequency	Measured value	Deviated value <sup>[2]</sup>	Acceptance limit <sup>[3]</sup>
Pressure level (cB)	(Hz)	(Hz)	(%)	(%)
94	1000	1003.0	0.3	±0.7



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20230033EA

Calibration Report

3. Function : Total distortion + noise

Normal	Normal	Measured value <sup>[4]</sup>	Acceptance limit <sup>[5]</sup>
Sound Pressure level (dB)	Frequency (Hz)	(%)	(%)
94	1000	1.3	2.5

Uncertainty of measurement

Function	Uncertainty	Maximum-permitted uncertainty of measurement
Sound pressure level	0.10 dB	0.15 dB
Frequency	0.10 %	0.20 %
Total distortion + noise	0.40 %	0.50 %

Note: [1] The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.  
[2] The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.  
[3] The acceptance limit is for the deviated value.  
[4] The measured value is the total distortion + noise, measured over the frequency range from 20 Hz to 20 kHz.  
[5] The acceptance limit is for the Measured value.

Remarks: 1. Using the 1/2-inch microphone adaptor NC-74-002.  
2. Acceptance limit was IEC 60942:2017 Class 1.  
3. The coverage factor  $k = 2.00$

-- End of Report --

Sheet No. : CR-515-2023-115



SOUND LEVEL METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 18, 23

ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Frequency (Hz)	Ref.Calibrated (dB)	Eff.Calibrated (dB)
Cirrus	CR:515	94296	1000.00	94.0	93.8

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	SCARLET	ST-21D	820722	93.8	0.0
2	SCARLET	ST-21D	820723	93.8	0.0
4	SCARLET	ST-21D	820725	93.8	0.0
6	SCARLET	ST-21D	820727	93.6	0.2
9	SCARLET	ST-21D	820730	93.7	0.1

Calibrated by :

Approved by :



## SOUND LEVEL METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Aug 18, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Frequency (Hz)	Ref.Calibrated (dB)	Eff.Calibrated (dB)
Cirrus	CR:515	94296	1000.00	94.0	93.8

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
5	SCARLET	ST-21D	820726	93.8	0.0
8	SCARLET	ST-21D	820729	93.8	0.0

Calibrated by :

Approved by :



## SOUND LEVEL METER CALIBRATION

Calibration Location: SECOT

Calibration Date: Nov 16, 23

## ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Frequency (Hz)	Ref.Calibrated (dB)	Eff.Calibrated (dB)
Cirrus	CR:515	94296	1000.00	94.0	93.8

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	SCARLET	ST-21D	820722	93.8	0.0
6	SCARLET	ST-21D	820727	93.8	0.0

Calibrated by :

Approved by :



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,

Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280

Tel: +66 2709 4860 Fax: +66 2324 0917



NSC-TISI-TIS 17025  
CALIBRATION 0119

Certificate No.: CP20220368EA

Operation No.: CP2022120011

## Certificate of Calibration

Equipment: Sound Calibrator

Manufacturer: Cirrus Research Plc

Model/Type: CR:515

Serial No.: 94296

ID No.:

Customer: SECOT Co.,Ltd.

Address: 239 Rimklongprapa Rd., Bangsue,  
Bangkok 10800 Thailand

Received Date: 14 December 2022

Calibrated Date: 20 December 2022

Issued Date: 23 December 2022

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

  
( Mr. Sittichai Swaksuriyawong )  
Group Manager

This report was prepared electronically using applicable electronic signature, Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor ( $k$ ) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE  
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20220368EA

## Calibration Report

Equipment: Sound Calibrator

Manufacturer: Cirrus Research Plc

Model/Type: CR:515

Serial No.: 94296

ID No.:

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Pressure: (101.3 ± 1.5) kPa

Method of Calibration :-

IEC 60942:2017

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2661000	AA-1020-22	14 June 2023
2) Waveform Generator	33511B	MY52302264	CK20220058EA	19 June 2023
3) Audio Analyzing DMM	2015-P	4079144	E1U221042	16 March 2023
4) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P220024 CD20220165EA	17 March 2023 24 July 2023

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

### Result of Calibration:-

1. Function : Sound pressure level

Normal	Specified Sound	Measured value	Deviated value <sup>[1]</sup>	Acceptance limit <sup>[3]</sup>
Frequency (Hz)	Pressure level (dB)	(dB)	(dB)	(dB)
1000	94	93.90	-0.10	±0.25

2. Function : Frequency

Normal Sound	Specified Frequency	Measured value	Deviated value <sup>[2]</sup>	Acceptance limit <sup>[3]</sup>
Pressure level (dB)	(Hz)	(Hz)	(%)	(%)
94	1000	1000.3	0.0	±0.7

Certificate No.: CP20220368EA

### Calibration Report

#### 3. Function : Total distortion + noise

Normal	Normal	Measured value <sup>[4]</sup>	Acceptance limit <sup>[5]</sup>
Sound Pressure level (dB)	Frequency (Hz)	(%)	(%)
94	1000	0.9	2.5

#### Uncertainty of measurement

Function	Uncertainty	Maximum-permitted uncertainty of measurement
Sound pressure level	0.10 dB	0.15 dB
Frequency	0.10 %	0.20 %
Total distortion + noise	0.40 %	0.50 %

- Note:
- [1] The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.
  - [2] The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.
  - [3] The acceptance limit is for the deviated value.
  - [4] The measured value is the total distortion + noise, measured over the frequency range from 20 Hz to 20 kHz.
  - [5] The acceptance limit is for the Measured value.

Remarks: 1. Acceptance limit was IEC 60942:2017 Class 1.  
2. The coverage factor  $k = 2.00$

-- End of Report --



### MAINTENANCE REPORT

#### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

#### 3110 + HGA600 + FIAS100 + AMALGAM

<b>Customer :</b> บริษัท ชีคอต จำกัด	<b>Date Tested:</b> June 15, 2566
<b>Address :</b> 239 ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพฯ 10800	<b>Recommendation Recertification</b>
	Period 6 Months
<b>User Name:</b> คุณ อารยา	<b>Recertification Due:</b> December 15, 2566
<b>Phone:</b> 02-9593600 ext. 507	<b>Date Last Certified:</b> December 16, 2565
<b>E-mail:</b> labmail@secot.co.th	<b>Visit Number:</b> 1 OF 2
	<b>TH Onesource Phone:</b> 081-7316733
	<b>E-mail:</b> thonesource@gmail.com

#### CONFIGURATION TESTED

MODEL	SERIAL NUMBER	SOFTWARE
AA-3110	311N6062102	AAWINLAB 3.2
HGA 600	2698	
AS 60	2124	
FIAS 100	1114	
AMALGAM	160S2110102	

TEST STANDARD USED	PART NUMBER
Copper	N9300183
GFAAS Mixed STD	N9300244
PE standard of Mercury	N9300174



**MAINTENANCE REPORT**  
**ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL**  
**3110 + HGA600 + FIAS100 + AMALGAM**

SERIAL NUMBER 311N6062102 DATE TESTED June 15, 2566

**1. OPTIC CHECKS**

A. Optical alignment condition (if necessary)

☐ OK

B. Condition of Mirrors, Lenses etc.

☐ OK

C. D2 and HCL beam adjust (if necessary)

☐ OK**2. ELECTRONICS CHECKS**

A. Power Supplies

+ 5.00 Vdc  $\pm$  0.2 Vdc

+ 5.0 Vdc

+ 11.50 Vdc  $\pm$  0.2 Vdc

+ 11.4 Vdc

+ 15.00 Vdc  $\pm$  1.0 Vdc

+ 15.2 Vdc

- 15.00 Vdc  $\pm$  1.0 Vdc

- 14.9 Vdc

B. D2 Power supplies

+150 Vdc

NA Vdc

+ 450 Vdc

NA Vdc

C. PMT Power supply

- 250 Vdc

-249.2 Vdc

**3. GAS SYSTEM CHECKS**

A. Leak test all internal and external gas box joints

☐ OK

B. All gas box safety features

☐ OK

C. Burner system including nebulizer and all o-ring and gasket

☐ OK

D. Drain system

☐ OK**4. FIAS CHECK**

A. Output power supplies

+5 VDC  $\pm$  0.25 VDC.5.01 VDC.+40 VDC  $\pm$  0.5 VDC.40.01 VDC.☐ OK

B. Valve and pump clean

☐ OK

**MAINTENANCE REPORT**  
**ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL**  
**3110 + HGA600 + FIAS100 + AMALGAM**

SERIAL NUMBER 311N6062102 DATE TESTED June 15, 2566

**5. PERFORMANCE TEST FOR FLAME**

A. Performance Tests with PE standard.

A1. Run Std. Of Cu and Cr at 324.8 ; 357.9 nm, Concentration 4, 4 ppm respectivelyResults = 0.228, 0.244 Abs, with flow spoiler. respectivelyCharacteristic Concentration 0.077 ; 0.072 mg/L respectivelyA2. Run Std. of Pb at 283.3 nm; Concentration 20 ppmResults = 0.205 Abs, with flow spoiler.Characteristic Concentration 0.429 mg/L

B. Performance Tests (For C2H2 + N2O Flame)

Run Std. Of Al at 309.3 nm; Concentration 50 ppmResults = 0.217 Abs, with flow spoiler.Characteristic Concentration 1.014 mg/L**6. PERFORMANCE TEST FOR FIAS****ACTUAL VALUE**

A. Characteristic mass for Mercury

( 500 ul of 10 ug/l Hg for 0.07 Abs. )

0.074 Abs.Characteristic Mass 314 pg / 0.0044 Abs.297.3 pg/0.0044 Abs.RSD  $\leq$  2%1.24 %

B. Characteristic mass for Arsenic

( 500 ul of 10 ug/l As for 0.45 Abs. )

0.482 Abs.Characteristic Mass 48 pg / 0.0044 Abs.45.6 pg/0.0044 Abs.RSD  $\leq$  2%1.54 %

C. Characteristic mass for Mercury Amalgamation

( 1000 ul of 1.0 ug/l Hg for 0.03 Abs. )

0.032 Abs.Characteristic Mass 147 pg / 0.0044 Abs.137.5 pg/0.0044 Abs.RSD  $\leq$  2%1.76 %





**MAINTENANCE REPORT**  
**ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL**  
**3110 + HGA600 + FIAS100 + AMALGAM**

SERIAL NUMBER 311N6062102 DATE TESTED June 15, 2566

**7. PERFORMANCE CHECK FOR FURNACE**

A. Internal & External gas flow

☐ OK

B. Contract Cylinder ( replace if necessary )

☐ OK

C. Quartz Windows

☐ OK

D. Gas Tubing and Joins

☐ OK

E. Cooling System

☐ OK

**8. AUTOSAMPLER CHECK**

A. Arm and gears

☐ OK

B. Sample and Rinse Pump

☐ OK

C. Tray and Sensors

☐ OK

**9. PERFORMANCE TEST FOR FURNACE**

**Test run using Chromium**

1. Standard Deviation after 5 replicates of blank  $\leq 0.005$

0.004

2. Characteristic mass ( 5 ug / L for Cr, 3 pg/0.0044 A-s )

3.0 pg / 0.0044 A-s

Peak Area

0.148 A-s

Relative Standard Deviation  $\leq 2.0$  %

0.24 %

**Test run using Lead**

Characteristic mass ( 20 ug / L for Pb, 10 pg/0.0044 A-s )

9.3 pg / 0.0044 A-s

Peak Area

0.188 A-s

Relative Standard Deviation  $\leq 2.0$  %

0.64 %



**MAINTENANCE REPORT**  
**ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL**  
**3110 + HGA600 + FIAS100 + AMALGAM**

SERIAL NUMBER 311N6062102 DATE TESTED June 15, 2566

Remarks :

NA Mean no applicant

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

**TH ONE SOURCE CO., LTD.**

*Krungchai T.*

( Krungchai Treevichien )

Customer Support Engineer



## Agilent CrossLab Start Up Services

### Agilent 7890 Gas Chromatograph

### Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.



#### Agilent 7890 GC Preventive Maintenance Checklist



### Introduction

#### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

#### Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our **Support Home page** <http://www.agilent.com/search/support>.
- **Videos** about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- **7890B Manuals** are also available on Agilent.com:
  - **Safety**  
[https://www.agilent.com/cs/library/usermanuals/public/7890B\\_Safety.pdf](https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf)
  - **Installation and First Startup**  
[https://www.agilent.com/cs/library/usermanuals/Public/7890B\\_Installation.pdf](https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf)
  - **Operation Manual**  
[https://www.agilent.com/cs/library/usermanuals/Public/7890B\\_Operation.pdf](https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf)
  - **Maintaining Your GC**  
[https://www.agilent.com/cs/library/usermanuals/public/G8430-90052%207890B\\_Maintaining%20Guide.pdf](https://www.agilent.com/cs/library/usermanuals/public/G8430-90052%207890B_Maintaining%20Guide.pdf)





## Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Complete the total number of pages field in the Service Completion section.
- **Ask the customer to sign the Service Completion section including the customer's and your signature.**

## Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.



## System Information

- ☒ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID

GC7890B

CN15343147

Instrument System Site and Location

Secot Co., Ltd.

Instrument room.

List System Component Product Numbers

List the Serial Numbers of each Component

1.

GC7890B

CN15343147

2.

GC4513A

CN1910080

3.

GC4514A

CN19080006

4.

5.

6.

7.

8.

9.

10.

## Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.



## Preventive Maintenance Procedure

### Clean and inspect GC

- ☒ Unplug power cord from the power source.
- ☒ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☒ Inspect internal connectors for proper contact and placement.
- ☒ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☒ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☒ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☒ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

### Inlet and detector consumable replacement

- ☒ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – “Maintaining Your GC” - for the inlet(s) installed.
- ☒ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☒ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☒ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the Ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

### Zero Sensors and Leak test

- ☒ Zero all pressure sensors per the procedure in the 7890 “Advanced User Guide”.
- ☒ Perform inlet pressure decay test(s) as defined in the 7890 “Troubleshooting Manual”.  
If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☒ Record if test passed or failed in the results table.

## ALS Maintenance

- ☐ Section NOT applicable
- ☒ Check all cabling and configuration settings between GC, tray, and injectors.
- ☒ Vacuum or remove any dust, especially around fans.
- ☒ Check operation of all fans.
- ☒ Check syringe for smooth plunger operation.
- ☒ Check for smooth operation of the needle support – clean if necessary

## Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions
- ☒ After equilibration, check and record the post PM detector signal output values.  
Results should be similar or lower than the detector outputs recorded prior to PM.
- ☐ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

## Signature Page

## Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.  
☒ Record the Preventive Maintenance service activity in the customer's records/logbook.  
☒ Update/reset instrument maintenance counters as appropriate.  
☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.  
☒ Complete the Service Engineer Comments section if there are additional comments.  
☒ Review with the customer this service, parts replaced, and test results obtained.  
☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.  
☐ Supply the customer with a copy of the Smart Alerts flyer.  
☐ Describe Smart Alerts to the customer.  
☐ Install Smart Alerts if requested.

## 7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output <i>FID</i>	<i>N/A</i>	<i>126-2</i>
Back detector output <i>FID</i>	<i>N/A</i>	<i>22-6</i>
AUX detector output	<i>N/A</i>	<i>N/A</i>
Pressure decay test	Expected test result	Actual test result
Front inlet pressure decay test	Pass	<i>Pass</i>
Back inlet pressure decay test	Pass	<i>Pass</i>

## 7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	<i>N/A</i>
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	<i>2</i>
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	<i>N/A</i>
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	<i>N/A</i>
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	<i>N/A</i>
PP Inlet PM kit	5188-6498	7890A/B	<i>N/A</i>
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	<i>N/A</i>
MMI Cleaning Kit	G3510-60820	7890A/B	<i>N/A</i>
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	<i>N/A</i>
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	<i>N/A</i>
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	<i>1</i>
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	<i>N/A</i>
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	<i>1</i>
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	<i>N/A</i>
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	<i>N/A</i>
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	<i>N/A</i>
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	<i>N/A</i>
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	<i>N/A</i>
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	<i>N/A</i>
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	<i>N/A</i>
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	<i>N/A</i>
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	<i>N/A</i>



Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 606041153  
Agilent signature SAH  
Customer signature Mam Saengutthai  
Date service completed 29 May 2023  
Total number of pages in this document 9 pages

Certificate of Completion



Learner Name: Saengutthai Saeng Tarak  
Title Of Course: AN-ASP/CE/CSF-GC-1-001-Mt: 7890/7820 GC and OL GC Standalone Chemstation I&F/ Service  
Completion Date: November 23, 2014  
Certified By Company: Learning at Agilent

All Service and Support training certificates have the following specific limitations.


A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's Safety Alerts, Service Notes, Internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.

# Certificate of Completion

Learner Name:	Saenguthai Saeng Tarak
Title Of Course:	AN-CE-GC-IL-022-A: Advanced GC Detectors Application and Troubleshooting Labs
Completion Date:	November 25, 2014
Certified By Company:	Learning at Agilent

All Service and Support training certificates have the following specific limitations.

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.



**Certificate of Completion**

Learner Name:	Saenguthai Tarak
Title Of Course:	AN-CE-GC-MS-2-041-D: 5977 EKC/HES MSD GC-MS OPER. HW SW - Intro, Repair and Troubleshooting
Completion Date:	March 18, 2016
Certified By Company:	Learning at Agilent

A certificate for Service and Support training is only valid while employed by Agilent Technologies or while working as an Agilent-authorized service provider, through which the service employee has ongoing access to Agilent's Safety Alerts, Service Notes, internal technical updates, update training, current documentation, technical support, current parts, and parts updates. Completion of training alone, without being employed by Agilent Technologies, does not qualify an individual to safely install, service or maintain Agilent products.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 23CH4  
Page.: 1 of 3

## Certificate of Calibration

**Equipment :** pH Meter  
**Manufacturer :** Hapna  
**Model :** HI98190  
**Serial No. :** 06470022101  
**ID No. :** pH No.19  
**Condition As-Received:** Used Item  
**Received Date :** 03 January 2023  
**Calibration Date :** 04 January 2023  
**Reference :** 2301-0006DN-1  
**Submitted by :** Secot Co.,Ltd.  
239 Rimklongprapa Road,  
Bangsue, Bangkok 10800  
**Ambient Temperature :** (25 ± 2.5) °C  
**Relative Humidity :** (50 ± 15) %  
**Calibration Procedure :** In - house method :  
- CP-CH5 by direct measurement with standard  
voltage calibrator and direct measurement with  
certified reference material (CRM)  
- CP-CH8 by comparison with standard thermometer

**Calibrated by :** Warakorn Lernagatrakul

**Approved by :**

Approved Signatory

- ( / ) Malee Butkruea  
( ) Saithip Meangmai  
( ) Warakorn Lernagatrakul

**Issue Date :** 10 January 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 23CH4  
Page.: 2 of 3

### Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Ref. Standard Thermometer	4982054	110RC044	2211306	27 Oct 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	826588	09 July 2024
pH 6.987	CPA chem	823322	20 June 2023
pH 10.008	CPA chem	826590	09 July 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

### Calibration Results

**Function :** pH Measurement

**Performing three buffers standard curve by using buffer nominal pH (4,7,10)**

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading ( mV )	Uncertainty of pH measurement (±)	Coverage factor k
pH Electrode	4.008	4.010	157.9	0.0044	2.00
S/N.: 0920044N	6.987	6.990	-1.6	0.0086	2.00
	10.008	10.007	-163.7	0.0065	2.00

**Remark** - Can not connect the BNC because the plug does not match with the socket.





Cert.No.: 23CH4

Page.: 3 of 3

#### Calibration Results

Function : Temperature Measurement

(\*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : HI12963

- Serial No. : 0920044N

Dimension of probe;

- Length : 105 mm.

- Diameter : 14 mm.

- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
20.0	20.002	20.0	-0.002	0.13	2.00
25.0	25.003	25.0	-0.003	0.13	2.00
30.0	30.005	30.0	-0.005	0.13	2.00
35.0	35.002	35.0	-0.002	0.13	2.00

Remark : - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o-o-

Mali

a 1142464



Request Service No. 098/66

Page 1 of 3

#### Calibration Certificate

Nomenclature : Brand : Mettler Toledo Type : Top-Loading Electronic Balance

Model : AG245 Serial No. : 1117293916 (198129-0)

Submitted by : Laboratory of SECOT CO., LTD.

Location of Calibration : BAL Room , 6<sup>th</sup> Floor, Secot Co., Ltd.

Calibration range : 0 – 200 g Scale division : 0.00001 g (41g)/ 0.0001 g (210g)

Calibration date : May 25, 2023

Reference Standard No. M220177, M2302167S, M2303005N

Traceable to : Metrological Center SCI ECO Services Company Limited.

Thai Calibration Services CO., LTD.

Ambient Condition : Temperature 25.70 – 25.90 °C

Humidity 50.70 – 51.20 % RH

Calibrated By : Sasipa Jaidee

(Miss Sasipa Jaidee)

Testing Officer

Date : 25/05/2023

Approved By : Nanna Poowanapetch

(Miss Narisa Poowanapetch)

Chief of Technical Management

Date : 25/05/2023

Issued Date : May 26, 2023

## Measurement Report

Request Service No. 098/66

Page 2 of 3

Description : Brand : Mettler Toledo

Type : Top-Loading Electronic Balance

Model : AG245

Serial No. : 1117293916 (198129-0)

Calibration range : 0 – 200 g

Scale division : 0.00001 g (41g)/ 0.0001 g (210g)

Calibration date : May 25, 2023

Ambient Condition : Temperature 25,70-25,90 °C Relative humidity 50.70-51.20 % RH

Measurement data :

### 1. Repeatability of Reading :

Load (g)	Standard Deviation of Reading (g)	Maximum Difference between Successive Reading (g)
50	0.000052	0.0001
100	0.000071	0.0002
150	0.000067	0.0002
200	0.000071	0.0002

### 2. Off-Center Loading :

A Mass of 50.0000 g was placed and moved to various position on the pan.

Unit : g

Center	Front	Left	Back	Right	Center	Maximum Difference
50.00040	50.00062	50.00078	50.00000	50.00010	50.00040	0.00038

Issued Date : May 26, 2023

Request Service No.098/66

Page 3 of 3

### 3. Departure from Nominal Value :

Reading (g)	Correction (g)	Uncertainty (+/- g)
0	0.000000	± 0.000008
0.5	-0.000017	± 0.000014
1	-0.000026	± 0.000018
10	-0.000099	± 0.000033
20	-0.000168	± 0.000046
40	-0.000339	± 0.000072
60	-0.00058	± 0.00011
80	-0.00059	± 0.00014
100	-0.00070	± 0.00016
120	-0.00069	± 0.00018
140	-0.00096	± 0.00020
160	-0.00082	± 0.00023
180	-0.00089	± 0.00024
200	-0.00118	± 0.00027

Calibrated by : Sasipa Jaidee Approved By : Naim Poowasanpeth

(Miss Sasipa Jaidee)

(Miss Narisa Poowasanpeth)

Testing Officer

Chief of Technical Management

Date : 25/05/2023

Date : 25/05/2023

Issued Date : May 26, 2023



Request Service No.100/66

Page 1 of 3

### Calibration Certificate

Nomenclature : Brand : Sartorius Type : Top-Loading Electronic Balance

Model : BSA224S-CW Serial No. : 32191636

Submitted by : Laboratory of SECOT CO., LTD.

Location of Calibration : BAL Room , 6<sup>th</sup> Floor, Secot Co., Ltd.

Calibration range : 0 – 200 g Scale division : 0.0001 g (220 g)

Calibration date : May 23, 2023

Reference Standard No. M220177, M2302167S, M2303005N

Traceable to : Metrological Center SCI ECO Services Co., Ltd., Thai Calibration services Co., Ltd

Ambient Condition : Temperature 24.60-24.80 °C

Humidity 50.6-51.4 % RH

Calibrated By : *Khemchuda Insorn*

(Miss Khemchuda Insorn)

Approved By : *Narisa Poowasanpetch*

(Miss Narisa Poowasanpetch)

Testing Officer

Chief of Technical Management

Date : *24/05/2023*

Date : *24/05/2023*

Issued Date : May 24, 2023

### Measurement Report

Request Service No.100/66

Page 2 of 3

Description : Brand : Sartorius

Type : Top-Loading Electronic Balance

Model : BSA224S-CW

Serial No. : 32191636

Calibration range : 0 – 200 g

Scale division : 0.0001 g (220 g)

Calibration date : May 23, 2023

Ambient Condition : Temperature 24.60-24.80 °C Relative humidity 50.6-51.4 % RH

Measurement data :

1. Repeatability of Reading :

Load (g)	Standard Deviation of Reading (g)	Maximum Difference between Successive Reading (g)
50	0.00007	0.0002
100	0.00005	0.0001
150	0.00006	0.0002
200	0.00006	0.0002

2. Off-Center Loading :

A Mass of 50.0000 g was placed and moved to various position on the pan.

Unit : g

Center	Front	Left	Back	Right	Center	Maximum Difference
49.99976	49.99988	49.99984	49.99984	49.99990	49.99976	0.00012

Issued Date : May 24, 2023

## 3. Departure from Nominal Value :

Reading (g)	Correction (g)	Uncertainty (+/- g)
0	0.00000	$\pm 0.00008$
1	+ 0.00004	$\pm 0.00008$
5	- 0.00005	$\pm 0.00008$
10	+ 0.00020	$\pm 0.00008$
20	+ 0.00027	$\pm 0.00008$
40	+ 0.00022	$\pm 0.00010$
60	+ 0.00018	$\pm 0.00012$
80	+ 0.00019	$\pm 0.00014$
100	+ 0.00028	$\pm 0.00016$
120	+ 0.00027	$\pm 0.00018$
140	+ 0.00036	$\pm 0.00020$
160	+ 0.00040	$\pm 0.00022$
180	+ 0.00058	$\pm 0.00024$
200	+ 0.00052	$\pm 0.00027$

Calibrated by :

(Miss Khemchuda Insorn)

Testing Officer

Date :

24/05/2023

Approved By :

(Miss Narisa Poowasanpetch)

Chief of Technical Management

Date :

24/05/2023

Issued Date : May 24, 2023



## Calibration Certificate

Nomenclature : Brand : Mettler Toledo Type : Top-Loading Electronic Balance

Model : AB204-S Serial No. : 1123163292 (209359)

Submitted by : Laboratory of SECOT CO., LTD.

Location of Calibration : BAL Room , 6<sup>th</sup> Floor, Secot Co., Ltd.

Calibration range : 0 – 200 g Scale division : 0.0001 g (220 g)

Calibration date : May 25, 2023

Reference Standard No. M220177, M2302167S, M2303005N

Traceable to : Metrological Center SCI ECO Services Company Limited.

: THAI CALIBRATION SERVICES CO., LTD.

Ambient Condition : Temperature 25.20 - 25.50 °C

Humidity 49.7 – 53.4 % RH

Calibrated By :

Janista Kui-on

(Miss Janista Kui-on)

Testing Officer

Date : 25/05/2023

Approved By :

Narisa Poowasanpetch

(Miss Narisa Poowasanpetch)

Chief of Technical Management

Date : 25/05/2023

Issued Date : May 25, 2023

## Measurement Report

Request Service No. 101/66

Page 2 of 3

Description : Brand : Mettler Toledo Type : Top-Loading Electronic Balance

Model : AB204-S Serial No. : 1123163292 (209359)

Calibration range : 0 – 200 g Scale division : 0.0001 g (220 g)

Calibration date : May 25, 2023

Ambient Condition : Temperature 25.20-25.50 °C Relative humidity 49.7-53.4 % RH

Measurement data :

### 1. Repeatability of Reading :

Load (g)	Standard Deviation of Reading (g)	Maximum Difference between Successive Reading (g)
50	0.00006	0.0002
100	0.00008	0.0002
150	0.00010	0.0003
200	0.00007	0.0002

### 2. Off-Center Loading :

A Mass of 50.0000 g was placed and moved to various position on the pan.

Unit : g

Center	Front	Left	Back	Right	Center	Maximum Difference
50.00002	50.00004	50.00022	50.00012	49.99998	49.99998	0.00024

Issued Date : May 25, 2023

Request Service No.101/66

Page 3 of 3

### 3. Departure from Nominal Value :

Reading (g)	Correction (g)	Uncertainty (+/- g)
0	0.00000	± 0.00008
1	-0.00004	± 0.00008
5	-0.00003	± 0.00012
10	+0.00002	± 0.00010
20	-0.00007	± 0.00009
40	-0.00010	± 0.00012
60	-0.00022	± 0.00016
80	-0.00037	± 0.00014
100	-0.00007	± 0.00016
120	-0.00083	± 0.00018
140	-0.00078	± 0.00021
160	-0.00084	± 0.00023
180	-0.00085	± 0.00026
200	-0.00082	± 0.00027

Calibrated by : Janista Kui-on

(Miss Janista Kui-on)

Testing Officer

Date : 25/05/2023

Approved By : Nanna Poowasanpetch

(Miss Narisa Poowasanpetch)

Chief of Technical Management

Date : 25/05/2023

Issued Date : May 25, 2023

## Calibration Certificate

**Certificate No.:** 2304081-003-01  
**Client name:** SECOT CO., LTD.  
**Address:** 239 Rimklongprapa Road,  
Bangsue, Bangsue, Bangkok 10800

Page 1 of 3

**Equipment:** CHAMBER (Hot Air Oven)

**Manufacturer:** BINDER

**Model:** ED 53

**Serial No.:** 01-27152

**ID No.:** N/A

**Order No.:** 2304081

**Operation No.:** 2304081-003

**Date of Receipt:** 27 July 2023

**Date of Calibration:** 27 July 2023

**Calibrated by** Mr. Worapob Sooktong  
Scientist

**Approved by**   
( Mr. Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 7 August 2023 **Responsible for the Technical Management Team**

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

FC-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2304081-003-01  
**Equipment:** CHAMBER (Hot Air Oven)  
Model: ED 53 Serial No.: 01-27152  
Resolution: 1 °C ID No.: N/A  
Manufacturer: BINDER

**Date of Calibration:** 27 July 2023

Page 2 of 3

**Location:** Laboratory, SECOT CO., LTD.

**Environment Condition:** Ambient Temperature ( 32 ± 1 ) °C  
Relative Humidity ( 52 ± 2 ) %  
Line Voltage ( 228 ± 1 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.  
- The temperature scale used was based on ITS - 90.  
- All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016894	TE 660380-01	22 April 2024	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/ RTD#101-109			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description :

Time of Record 1 Hour 9 Minute At 104, 110 and 180 °C  
Fresh air Damper ☐ Open Position ☐  
☒ Close  
☐ Not Available

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

FC-012 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2304081-003-01  
**Equipment:** CHAMBER (Hot Air Oven)  
**Model:** ED 53 **Serial No.:** 01-27152  
**Resolution:** 1 °C **ID No.:** N/A  
**Manufacturer:** BINDER

**Date of Calibration:** 27 July 2023

Page 3 of 3

**Calibration point:** 104, 110 and 180 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	31.7	50.3	227.1
MAX	32.7	53.5	228.5




Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
104	104.79	105.05	104.60	104.30	104.35	103.88	104.29	103.87	103.82	0.78
110	111.06	111.10	110.65	110.38	110.01	109.70	109.80	109.76	109.80	0.80
180	181.06	181.08	180.58	180.53	180.43	180.25	179.97	180.71	180.08	0.90

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
104	104	104	104	0.22	1.23	1.55
110	110	110	110	0.25	1.30	1.80
177	177	177	177	0.32	0.99	1.54

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Certificate

**Certificate No.:** 2303092-001-01  
**Client name:** SECOT CO., LTD.  
**Address:** 239 Rimklongprapa Road, Bangsue, Bangsue, Bangkok 10800

Page 1 of 3

**Equipment:** CHAMBER (Hot Air Oven)

**Manufacturer:** MEMMERT

**Model:** UF 55

**Serial No.:** B213.0295

**ID No.:** N/A

**Order No.:** 2303092

**Operation No.:** 2303092-001

**Date of Receipt:** 26 May 2023

**Date of Calibration:** 26 May 2023

**Calibrated by** Mr.Jerawut Prapawuttipong  
Scientist

**Approved by** ( Mr.Pheraphat Tuanjit )  
Manager, Division of Calibration Laboratory  
Responsible for the Technical Management Team

**Date of Issue:** 30 May 2023

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2303092-001-01  
**Equipment:** CHAMBER (Hot Air Oven)  
**Model:** UF 55 **Serial No.:** B213.0295  
**Resolution:** 0.1 °C **ID No.:** N/A  
**Manufacturer:** MEMMERT  
**Date of Calibration:** 26 May 2023

Page 2 of 3

**Location:** Walkway Laboratory, SECOT CO., LTD.  
**Environment Condition:**  
Ambient Temperature ( 30.5 ± 1 ) °C  
Relative Humidity ( 60 ± 5 ) %  
Line Voltage ( 220 ± 5 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.  
- The temperature scale used was based on ITS - 90.  
- All data show below were final values and the initial data may be obtained upon request.

### Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016851	TE 660495-01	7 May 2024	NATIONAL FOOD INSTITUTE
	RTD	CH#201-209/ RTD#201-209			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description :

Time of Record 1 Hour 9 Minute At 80.0, 104.0 and 180.0 °C  
Fresh air Damper ☐ Open Position ☐  
☒ Close Fan 80%  
☐ Not Available

- Result of Calibration : ☒ Without adjustment ☐ After adjustment



## Calibration Report

**Certificate No.:** 2303092-001-01  
**Equipment:** CHAMBER (Hot Air Oven)  
**Model:** UF 55 **Serial No.:** B213.0295  
**Resolution:** 0.1 °C **ID No.:** N/A  
**Manufacturer:** MEMMERT  
**Date of Calibration:** 26 May 2023

Page 3 of 3

**Calibration point:** 80.0, 104.0 and 180.0 °C

### Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	30.0	55	215.0
MAX	31.0	65	225.0

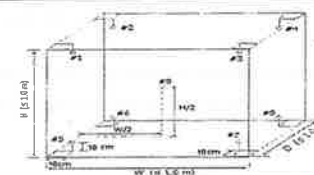


Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
80.0	80.00	80.08	79.98	80.01	80.11	80.00	79.89	80.02	80.12	0.46
104.0	104.05	104.03	104.19	104.09	104.06	104.10	103.89	104.17	104.29	0.53
180.0	179.88	180.12	180.02	180.20	180.27	180.36	179.93	180.04	180.11	0.90

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
80.0	80.0	80.0	80.0	0.077	0.23	0.33
104.0	104.0	104.0	104.0	0.094	0.40	0.51
180.0	180.0	180.0	180.0	0.17	0.26	0.77

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----






## Calibration Certificate

**Certificate No.:** 2303092-002-01  
**Client name:** SECOT CO., LTD.  
**Address:** 239 Rimklongprapa Road, Bangsue,  
 Bangsue, Bangkok 10800

Page 1 of 3

**Equipment:** CHAMBER (Hot Air Oven)  
**Manufacturer:** MEMMERT  
**Model:** UM 400  
**Serial No.:** B419.1400  
**ID No.:** N/A  
**Order No.:** 2303092  
**Operation No.:** 2303092-002  
**Date of Receipt:** 26 May 2023  
**Date of Calibration:** 26 May 2023

**Calibrated by** Mr.Jerawut Prapawuttipong **Approved by**   
 Scientist ( Mr.Pheraphat Tuanjit )  
 Manager, Division of Calibration Laboratory  
**Date of Issue:** 30 May 2023 **Responsible for the Technical Management Team**

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2303092-002-01  
**Equipment:** CHAMBER (Hot Air Oven)  
 Model: UM 400 Serial No.: B419.1400  
 Resolution: 1 °C ID No.: N/A  
 Manufacturer: MEMMERT  
**Date of Calibration:** 26 May 2023

Page 2 of 3

**Location:** Walkway Laboratory, SECOT CO., LTD.  
**Environment Condition:** Ambient Temperature ( 30.5 ± 1 ) °C  
 Relative Humidity ( 60 ± 5 ) %  
 Line Voltage ( 220 ± 5 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
  - The temperature scale used was based on ITS - 90.
  - All data show below were final values and the initial data may be obtained upon request.
- Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016851	TE 660495-01	7 May 2024	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/ RTD#101-109			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description :

Time of Record 1 Hour 9 Minute At 150 °C  
 Fresh air Damper ☐ Open Position ☐  
☒ Close Fan ☐  
☐ Not Available

- Result of Calibration : ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Report

<b>Certificate No.:</b>	2303092-002-01		
<b>Equipment:</b>	CHAMBER (Hot Air Oven)		
	Model:	UM 400	Serial No.: B419.1400
	Resolution:	1 °C	ID No.: N/A
	Manufacturer:	MEMMERT	


Date of Calibration: 26 May 2023

Page 3 of 3

Calibration point: 150 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	30.0	55	215.0
MAX	31.0	65	225.0

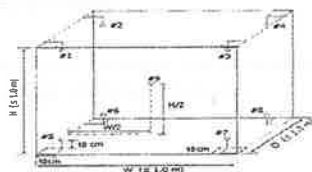

**Table1 : Reporting of Temperature**

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
150	150.84	151.35	150.78	151.22	149.63	151.51	150.53	151.02	150.13	0.89

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
As Mark 150	174	174	174	0.42	1.4	2.5

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

**Overall Variation** = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Certificate

**Certificate No.:** 2304081-001-01  
**Client name:** SECOT CO., LTD.  
**Address:** 239 Rimklongprapa Road,  
 Bangsue, Bangsue, Bangkok 10800

Page 1 of 3

**Equipment:** CHAMBER (Incubator)

**Manufacturer:** MEMMERT

**Model:** ICP 400

Serial No.: K406.0004

ID No.: N/A

**Order No.:** 2304081

**Operation No.:** 2304081-001

**Date of Receipt:** 27 July 2023

**Date of Calibration:** 27 July 2023

**Calibrated by** Mr. Worapob Sooktong  
Scientist

Approved by   
( Mr.Pheraphat Tuanjit )

**Manager, Division of Calibration Laboratory**

**Responsible for the Technical Management Team**

Date of Issue: 7 August 2023

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

Certificate No.:	2304081-001-01		
Equipment:	CHAMBER (Incubator)		
	Model:	ICP 400	Serial No.: K406.0004
	Resolution:	0.1 °C	ID No.: N/A
	Manufacturer:	MEMMERT	
Date of Calibration:	27 July 2023		

Page 2 of 3

<b>Location:</b>	Laboratory, SECOT CO., LTD.
<b>Environment Condition:</b>	Ambient Temperature ( 30 ± 1 ) °C
	Relative Humidity ( 54 ± 1 ) %
	Line Voltage ( 228 ± 0 ) Volt

**Condition of this results of Calibration:**

1. This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
  - All data show below were final values and the initial data may be obtained upon request.

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016894	TE 660380-01	22 April 2024	NATIONAL FOOD INSTITUTE
	RTD	CH#301-309/ RTD#301-309			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item :      Good

UUC Description :

Time of Record 1 Hour 9 Minute At 20.0 °C

Fresh air Damper	-	Open	Position	-
	X	Close		
	-	Not Available		

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Report

Certificate No.:	2304081-001-01		
Equipment:	CHAMBER (Incubator)		
	Model:	ICP 400	Serial No.: K406.0004
	Resolution:	0.1 °C	ID No.: N/A
	Manufacturer:	MEMMERT	

Page 3 of 3

Date of Calibration:	27 July 2023
Calibration point:	20.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	28.6	53.0	227.3
MAX	31.4	54.1	228.1

Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
20.0	20.42	20.39	20.40	20.43	20.47	20.49	20.42	20.41	20.43	0.27




Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
20.0	20.0	20.1	20.0	0.065	0.053	0.220

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65




## Calibration Certificate

**Certificate No.:** 2304081-002-01  
**Client name:** SECOT CO., LTD.  
**Address:** 239 Rimklongprapa Road,  
 Bangsue, Bangsue, Bangkok 10800

Page 1 of 3

**Equipment:** Water Bath  
**Manufacturer:** MEMMERT  
**Model:** WB 29  
**Serial No.:** I698.0051  
**ID No.:** N/A  
**Order No.:** 2304081  
**Operation No.:** 2304081-002  
**Date of Receipt:** 27 July 2023  
**Date of Calibration:** 27 July 2023

**Calibrated by** Mr.Worapob Sooktong  
 Scientist

**Approved by**   
 ( Mr.Pheraphat Tuanjit )  
 Manager, Division of Calibration Laboratory  
 Responsible for the Technical Management Team

**Date of Issue:** 7 August 2023

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2304081-002-01  
**Equipment:** Water Bath  
 Model: WB 29 Serial No.: I698.0051  
 Resolution: 0.1 °C ID No.: N/A  
 Manufacturer: MEMMERT

**Date of Calibration:** 27 July 2023

Page 2 of 3

**Location:** Laboratory, SECOT CO., LTD.  
**Environment Condition:** Ambient Temperature ( 24 ± 1 ) °C  
 Relative Humidity ( 58 ± 2 ) %  
 Line Voltage ( 229 ± 1 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 5 standard thermometer into its liquid bath and calibration according to W-TE-011 based on ASTM E715-80 (2016): Standard Specification for Gravity-Convection and Forced-Circulation Water Baths.  
 - The temperature scale used is ITS - 90.  
 - All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016894	TE 660380-01	22 April 2024	NATIONAL FOOD INSTITUTE
	RTD	RTD#201-205 / CH#201-205			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description:

Time of Record 1 Hour 9 Minute At 95.0 °C

7. Result of Calibration :
- |   |                    |
|---|--------------------|
| X | Without adjustment |
|   | After adjustment   |

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Report


**Certificate No.:** 2304081-002-01  
**Equipment:** Water Bath  
 Model: WB 29 Serial No.: I698.0051  
 Resolution: 0.1 °C ID No.: N/A  
 Manufacturer: MEMMERT  
**Date of Calibration:** 27 July 2023

Page 3 of 3

**Calibration point:** 95.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	23.0	56.3	227.5
Max	25.0	60.2	229.6

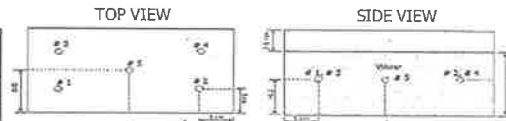

**Table 1 : Reporting of Temperature**

**Sensor Installation Location**

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.5 is REF)					Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	
95.0	95.03	94.96	95.10	94.97	95.02	0.28

**Table 2 : Reporting of Characterization Result**

UUC* Setting (°C)	UUC* reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
95.0	94.9	95.1	95.0	0.18	0.080	0.47

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----





## Agilent CrossLab Start Up Services

### Agilent 7890 Gas Chromatograph

### Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.



## Agilent 7890 GC Preventive Maintenance Checklist



### Introduction

#### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

#### Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our **Support Home page** <http://www.agilent.com/search/support>.
- **Videos** about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- **7890B Manuals** are also available on Agilent.com:
  - **Safety**  
[https://www.agilent.com/cs/library/usermanuals/public/7890B\\_Safety.pdf](https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf)
  - **Installation and First Startup**  
[https://www.agilent.com/cs/library/usermanuals/Public/7890B\\_Installation.pdf](https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf)
  - **Operation Manual**  
[https://www.agilent.com/cs/library/usermanuals/Public/7890B\\_Operation.pdf](https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf)
  - **Maintaining Your GC**  
[https://www.agilent.com/cs/library/usermanuals/public/G3430-90052-207890B\\_Maintaining%20Guide.pdf](https://www.agilent.com/cs/library/usermanuals/public/G3430-90052-207890B_Maintaining%20Guide.pdf)

Revision: 2.00, Issued: December 30, 2020  
 Agile Document Number: D0007063  
 DE number: 44165.759722222  
 © Agilent Technologies, Inc. 2020

Page 1 of 4



## Service Engineer's Responsibilities

- **Contact the customer** and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Completion section including the customer's and your signature.**

## Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

## System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID

CN13201053

Instrument System Site and Location

SECOT, Bangkok

List System Component Product Numbers

List the Serial Numbers of each Component

1.	G4340A	CN13201053
2.	G4513A	CN13380106
3.	G4514A	CN13230031
4.		
5.		
6.		
7.		
8.		
9.		
10.		

## Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save Instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

## Preventive Maintenance Procedure

### Clean and inspect GC

- ☒ Unplug power cord from the power source.
- ☒ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☒ Inspect internal connectors for proper contact and placement.
- ☒ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☒ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☒ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☒ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

### Inlet and detector consumable replacement

- ☒ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – "Maintaining Your GC" - for the **Inlet(s) Installed**.
- ☒ Replace the **split vent trap** cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☒ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☐ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

### Zero Sensors and Leak test

- ☒ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ☒ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual".  
If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☒ Record if test passed or failed in the results table.

## ALS Maintenance

- ☐ Section NOT applicable
- ☒ Check all cabling and configuration settings between GC, tray, and injectors.
- ☒ Vacuum or remove any dust, especially around fans.
- ☒ Check operation of all fans.
- ☒ Check syringe for smooth plunger operation.
- ☒ Check for smooth operation of the needle support – clean if necessary

## Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions
- ☒ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☒ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.



## Signature Page

## Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.  
☒ Record the Preventive Maintenance service activity in the customer's records/logbook.  
☒ Update/reset instrument maintenance counters as appropriate.  
☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.  
☒ Complete the Service Engineer Comments section if there are additional comments.  
☒ Review with the customer this service, parts replaced, and test results obtained.  
☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.  
☐ Supply the customer with a copy of the Smart Alerts flyer.  
☐ Describe Smart Alerts to the customer.  
☐ Install Smart Alerts if requested.

## 7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output	N/A	N/A
Back detector output		
AUX detector output		
Pressure decay test	Expected test result	Actual test result
Front inlet pressure decay test	Pass	PASS
Back inlet pressure decay test	Pass	N/A

## 7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	1
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	
PP Inlet PM kit	5188-6498	7890A/B	
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	
MMI Cleaning Kit	G3510-60820	7890A/B	
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	

### Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

### Service Completion

Service request number 6005830413

Date service completed 22 Feb 2023

Agilent signature [Signature]

Customer signature [Signature]

Total number of pages in this document \_\_\_\_\_

## Agilent Preventive Maintenance Services

### Agilent GCMS Preventive Maintenance

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.

## Introduction

This checklist covers the following model(s):

Type	Model
SQ	5973 Series MSD
SQ	5975 Series MSD
SQ	5977 Series MSD
TQ	7000 Series MS/MS
TQ	7010 Series MS/MS
QTOF	7200 Series QTOF
QTOF	7250 Series QTOF

## Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the **Parts Lists** section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

## Important Customer Web Links

- To access Agilent training and education, visit <http://www.agilent.com/chem/training> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.

- To access the **Agilent Resource Center** web page, visit <https://www.agilent.com/en-us/agilentresources>. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- Need to place a service call?** Flexible Repair Options | Agilent

## Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Service not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page.
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Verification section.
- Complete Signature Page and attach Signature Page to Service Order.

## Additional Instruction Notes

- Preventive maintenance is a factory recommended procedure designed to reduce the likelihood of electromechanical failures. Failure to perform preventive maintenance may reduce the long-term reliability of certain instruments and systems. Two preventative maintenances (PMs) per year are recommended; the Major PM Service will be performed annually with an Interim PM performed 6 months after the Major PM.

## Instrument Maintenance

Select the appropriate service to be performed.

- ☐ Interim Preventive Maintenance (when available, is typically 6 months or at the request of the customer)
- ☒ Major Preventive Maintenance (Yearly)
- ☐ Enhanced Preventive Maintenance (when available, is provided "As needed")

## System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID

Instrument System Site and Location

SECOT, Bangkok

List System Component Product Numbers

List the Serial Numbers of each Component

1.

G3172A

U513343B01

2.

3.

4.

5.

6.

7.

8.

9.

### Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components and implementation of Service Notes
- ☐ Check for required firmware updates and verify with customers if they would like them installed. Firmware update(s) are strongly recommended.

### Customer Responsibilities

Customers should ensure that all necessary operating supplies, consumables, and usage-dependent items such as gases, vials, syringes, calibrant solution and solvents required for successful preventive maintenance are available. A customer representative should be available while the preventive maintenance is being performed.

### Important notice for customers

The customer should complete the following before the Support Provider arrives on site:

- ☐ Perform an autotune and retain the printed tune report just prior to the start of the PM to verify performance of the equipment.

**Note:** it is recommended to have the customer run the autotune and tune evaluation prior to the PM and then start the vent cycle so that the instrument will be ready for the service representative.

### Definition of the Task/Recommended items within the document

Task		Recommended		
Yes	No	Interim	Major	As Needed
<input checked="" type="checkbox"/>				Yes selected means that the task was done or the part was required.
	<input checked="" type="checkbox"/>			No selected means that the task was not done or the part was not required.
		<input checked="" type="checkbox"/>		Interim selected means that this task is recommended to be done at 6-month intervals
			<input checked="" type="checkbox"/>	Major selected means that this task is recommended to be done yearly; if the customer would like a service to be done at the 6-month interval then the service could be purchased
				<input checked="" type="checkbox"/> As needed selected means that the task was done or the part was used as needed. For example, there could be two types of filters that could be used and this was the one selected.

## Preventive Maintenance Procedures

☐ Service Not Applicable

### Interim / Major Preventive Maintenance – GCMS

Yes/No	Interim/Major	Description
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Perform general inspection of system for cleanliness.
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Discuss any problems the customer is having with the instrument.
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Review customer maintenance records and exclude maintenance on recently serviced items.
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Review the most recent autotune report. This will give a starting point for evaluating spectral peaks, baseline noise, peak shape, mass assignments and resolution.

### Interim / Major Preventive Maintenance – System Checks

☐ Service Not Applicable

Yes/No	Interim/Major	System Checks
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Verify that calibration peaks were seen prior to starting the PM.
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Vent the instrument.
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Inspect vacuum hoses, pump, exhaust tubing, and power cords for excessive wear.
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Visually inspect calibrant levels – PFTBA PFDTD (if appl.), IRM (if appl.), Refill if available.
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Look for any obvious external damage or problems.
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Clean air intake(s). Cosmetic cover(s) may need to be removed.
<input type="checkbox"/>	<input type="checkbox"/>	Verify system line voltage meets instrument specifications: Yes <input checked="" type="checkbox"/> No <input type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	For Hydroinert systems, verify customer is running hydrogen: Yes <input type="checkbox"/> No <input type="checkbox"/>

### Interim / Major Preventive Maintenance – Wet Mechanical vacuum pumps

☐ Service Not Applicable

Yes/No	Interim/Major	Wet Mechanical vacuum pumps
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	

<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Check for evidence of oil leakage. Check pump gasket for leakage.
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Drain and replace mechanical pump oil.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Replace Oil Mist Filter if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Discuss with customer the need for more frequent oil changes if the oil is dirty.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Don't use mist filters with Chemical Ionization.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed. Visually confirm that no oil returns up vacuum hose.

### Interim / Major Preventive Maintenance – Dry Mechanical vacuum pumps - Diaphragm

☒ Service Not Applicable

Yes/No	Interim/Major	Dry Mechanical vacuum pumps - Diaphragm
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Check for evidence of poor vacuum – Turbo power demand, poor manifold vacuum, etc.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Clear air flow paths of dust.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	If vacuum is poor, then replace the diaphragm pump.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.

### Interim / Major Preventive Maintenance – Dry Mechanical vacuum pumps - Scroll

☒ Service Not Applicable

Yes/No	Interim/Major	Dry Mechanical vacuum pumps - Scroll
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Replace the tips seal on the IDP pump.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Check for evidence of poor vacuum – Turbo power demand, poor manifold vacuum, etc.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Replace the Exhaust Filter if required.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Discuss with customer the need for more frequent changes, if needed.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Inform customer that pump gas ballast should be installed all the time.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.

## Interim / Major Preventive Maintenance – Cleaning System and Filters

☐ Service Not Applicable

				Cleaning System and Filters
Yes/No	Interim	Major		Description
				Fans
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Remove dust from fans and vent covers.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Verify fans are functional and that there is enough space around the instrument for proper cooling.
				Source cleaning (all sources except HydroInert)
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Open analyzer and remove the source.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Disassemble, Clean, Re-assemble source.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Re-install source and close analyzer.
				HydroInert Source
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Source NOT to be abrasively cleaned. No cleaning required at PM, if a decrease in performance is observed, recommend to the customer that filaments, insulators (repeller and lens stack), extractor lens, and repeller lens may need to be replaced to restore performance. HydroInert source should not be run with helium carrier.
				Filters
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Replace RMSH-2 Helium gas filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Replace RMSN-2 Nitrogen gas filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	Replace RMSHY-2 Hydrogen gas filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CP17988 – Gas Clean Carrier Gas Kit for 7890 for Nitrogen or Helium: Bracket, Mount, and Filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CP17974 – Gas Clean Filter Kit GC/MS 1/8"; Mount and Filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	CP17973 – Gas Clean Filter, Replacement Filter – if applicable.
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	5190-9071 – Methane Gas Filter – if applicable.

## Interim / Major Preventive Maintenance – System Post Check

☐ Service Not Applicable

				System post-check
Yes/No	Interim	Major		Description
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Pump system back down. Wait until system stability has been achieved.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Verify system vacuum reading(s) via the gauge controller.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Leak Check
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Verify system in manual tune
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Compare against previous tune file report(s)
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Change to Tune and verify that all temperatures, pressures, and gas flows reach method set points
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Check manually that you have calibration peaks.
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	EI Autotune Performed

Guidance: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument setup and checkout.

## Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☒ Complete Signature Page and attach Signature Page to Service Order.

## Test Results

Test Description	Expected Test Result	Actual Test Result
------------------	----------------------	--------------------

## Consumed PM Parts

### Common MS Filters and Seals – 5973/5975/5977/7000/7010/7200/7250 Series

Part Description	Part Number	Interim	Major	As Needed
Helium gas filter – if required	RMSH-2		✓	✓
Nitrogen gas filter – if required	RMSN-2		✓	✓
Big Universal Trap, 1/8" fittings, Hydrogen, if required	RMSHY-2		✓	✓
Gas Clean Carrier Gas Kit for 7890 for Nitrogen or Helium; Bracket, Mount and Filter – if required	CP17988		✓	✓
Gas Clean Filter Kit GC/MS 1/8 in (complete replacement kit) – if required	CP17974		✓	✓
Gas Clean GS/MS Filter – if required	CP17973		✓	✓
Chemical Ionization Gas Purifier (CI systems) – if required	5190-9071		✓	✓
Agilent AVF Platinum, 1 quart	5191-5351	✓	✓	
Gas filters need to be changed only if required				

### MS Maintenance Supplies for 5973/5975/5977 Series

Part Description	Part Number	Interim	Major	As Needed
Diffusion pump fluid (Diffusion Pump Models)	6040-0809 Qty 2	✓	✓	✓
IDP-3 Tip Seal Replacement Kit (IDP-3 Dry Pump Models)	G7077-57018	✓	✓	✓
IDP-3 Tip Seal Replacement Kit (no tools – CSD P/N)	5190-9561	✓	✓	✓
IDP-3 Tip Seal Replacement Kit (no tools – VPD P/N)	IDP3TS	✓	✓	✓
Filter element for IDP-3	REPLSLRFILTER 2	✓	✓	✓
DS42 Oil Mist Eliminator 3/4G & 3/8	SR03706556	✓	✓	✓
Exhaust oil mist trap (thread) Edwards/Pfeiffer	G1099-80039	✓	✓	✓
Repeller Insulator	G1099-20133			✓
Lens stack Insulator	G3870-20530			✓
Lens insulator for Extractor (ring insulator)	G3870-20445			✓
HydroInert Extractor lens (5mm)	G7078-20909			✓
HydroInert Repeller	G7078-20902			✓



## MS Maintenance Supplies for 7000/7010 Series

Part Description	Part Number	Interim	Major	As Needed
Nitrogen gas filter	RMSN-2		✓	✓
IDP-10 Tip Seal Replacement Kit (IDP-10 Dry Scroll Pump Models)	G7004-67023		✓	✓
IDP-10 Tip Seal Replacement Kit (no tools – VPD P/N)	X3807-67000		✓	✓
Oil Mist Filter RV5	G6600-80043		✓	✓
Filter element for the IDP-10	REPLSLRFILTER 1		✓	✓
Repeller Insulator	G1099-20133			✓
Lens stack insulator	G3870-20530			✓
Lens insulator for Extractor (ring insulator)	G3870-20445			✓
HydroInert Extractor lens (9mm)	G7078-20909			✓
HydroInert Repeller	G7078-20902			✓

## MS Maintenance Supplies for 7200/7250 Series

Part Description	Part Number	Interim	Major	As Needed
Nitrogen gas filter – if required	RMSN-2		✓	✓
RIS Probe Maintenance Kit (7200 Series only)	G7004-67023		✓	✓
DS202 Oil Mist Eliminator	X3807-67000		✓	✓
IDP-15 Tip Seal Replacement Kit (IDP-15 Dry Pump Models)	G6600-80043		✓	✓
IDP-15 Tip Seal Replacement Kit (no tools – VPD P/N)	REPLSLRFILTER 1		✓	✓
Filter element, for SH-110/SH-112/IDP-15 exhaust silencer	G1099-20133		✓	✓
DS 3/B MAG. PLUG AND GASKET	G3870-20530		✓	✓

## MS Maintenance Supplies for JetClean

Part Description	Part Number	Interim	Major	As Needed
Big Universal Trap, 1/8" fittings, Hydrogen, if required	RMSHY-2		✓	✓

## Consumed Parts Reference

(Purchased by customer, not included as part of PM)

## Common MSD Maintenance Supplies 5973/5975/5977/7000/7010/7200/7250 Series

Part Description	Part Number	Interim	Major	As Needed
EI High Temperature Filaments	G7005-60061 Qty 2			✓
HES EI Filaments	G7002-60001			✓
LE-EI Filaments	G3850-60021			✓
CI High Temperature Filament – all MSDs	G7005-60072			✓
PFTBA GC/MS Tuning Standard calibrant	05971-60571			✓
PFTD calibrant, 1 mL	8500-8510			✓
FFET, IRM calibrant for GC QTOF 0.5 mL	5190-0531			✓

## MSD Maintenance Supplies 5973/5975/5977 Series

Part Description	Part Number	Interim	Major	As Needed
CI Interface tip seal (tip and spring combo)	G1999-60412			✓
CI Interface tip seal (tip only)	G3870-20542			✓
CI Interface tip seal spring (spring only)	G1999-20023			✓
Repeller insulator	G1099-20133 Qty 2			✓
Lens insulator/holder (HES)	G7002-20074			✓
Ring heater/sensor assembly (HES)	G7002-60043			✓
Ceramic insulator for Extractor (HES)	G7002-20064			✓
Transfer-Line Tip Cap, Threaded	G3870-20547			✓
Transfer-Line Tip Base, Threaded	G3870-20548			✓
Lens stack insulator	G3870-20530			✓
Lens insulator for Extractor (ring insulator)	G3870-20445			✓
HydroInert Extractor lens (9mm)	G7078-20909			✓
HydroInert Repeller	G7078-20902			✓

## MS Maintenance Supplies for 7000/7010 Series

Part Description	Part Number	Interim	Major	As Needed
CI interface tip seal - 7000	G1999-60412			✓
CI interface tip seal - 7010	G7002-60412			✓
CI interface tip seal (tip only)	G3870-20542			✓
CI interface tip seal spring (spring only)	G1999-20023			✓
Repeller insulator - 7000	G1099-20133 Qty 2			✓
Lens insulator/holder (HES)	G7002-20074			✓
Ring heater/sensor assembly (HES)	G7002-60043			✓
Ceramic insulator for Extractor (HES)	G7002-20064			✓
Transfer-Line Tip Cap, Threaded	G3870-20547			✓
Transfer-Line Tip Base, Threaded	G3870-20548			✓
Lens stack insulator	G3870-20530			✓
Lens insulator for Extractor (ring insulator)	G3870-20445			✓
HydroNert Extractor lens (9mm)	G7078-20909			✓
HydroNert Repeller	<del>G7078-20902</del>			✓

## MS Maintenance Supplies for 7200 Series

Part Description	Part Number	Interim	Major	As Needed
Extractor Lens Insulator	G7005-20133			✓
Ion Focus Insulator	G7005-20442			✓
Ring Heater/Sensor Assembly	G7005-60110			✓
RIS Xfer Tip	G7005-20542			✓
RIS Xfer Tip Spring	G7005-20024			✓

## MS Maintenance Supplies for 7250 Series

Part Description	Part Number	Interim	Major	As Needed
Lens insulator/holder (HES)	G7002-20074			✓
Ring heater/sensor assembly (HES)	G7002-60043			✓
Ceramic insulator for Extractor (HES)	G7002-20064			✓
Transfer-Line Tip Cap, Threaded	G3870-20547			✓

Part Description	Part Number	Interim	Major	As Needed
Transfer-Line Tip Base, Threaded	G3870-20548			✓
EI Extractor Transfer Tip	G3870-20542			✓
CI Tip Compression Spring	G1999-20023			✓

## MS Maintenance Supplies for Intuvo 9000 MS Series

Part Description	Part Number	Interim	Major	As Needed
Swaged MS Tail - Packaged	G4590-60009			✓
Swaged MS Tail (HES) - Packaged	G4590-60109			✓

## Common MS Maintenance Supplies

Part Description	Part Number	Interim	Major	As Needed
Abrasive paper, 90 um	5067-5396			✓
Alumina powder	393706201			✓
Cloths, clean (pkg of 15)	05980-60051			✓
Cloths, cleaning (pkg of 300)	9310-4828			✓
Cotton swabs (pkg of 100)	5080-5400			✓
Gloves, clean, large	8650-0030			✓
Gloves, clean, small	8650-0029			✓

## Signature Page

### Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the service review or other items of interest for the customer, please write in this box.

### Service Verification

Service Request Number: 6005830893

Date of Service Completion: 22 Feb 2023

Service Engineer Name: SMV N.

Customer Name:

Service Engineer Signature:

Total number of pages in this document:

### Teledyne Tekmar ATOMX Purge and Trap Preventive Maintenance Checklist - Standard

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results. Delivered by highly-trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak.

For more information about Agilent Technologies services please visit our web site using the following URL <http://www.chem.agilent.com/en-us/products/services/pages/default.aspx>

### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of additional or special procedures and/or parts for the instrument service, then these must be ordered separately and charged as a repair, which may incur additional costs.

### Service Engineer's Responsibilities

- Only complete/printout pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using a "X" or tick mark "✓" in the checkbox.
- Complete Not Applicable check boxes to indicate services not delivered, as needed.
- Complete the PM service in the order of the tasks listed.
- Complete the Service Review section together with the customer.

Teledyne Tekmar ATOMX Purge and Trap  
Preventive Maintenance Checklist - Standard



Agilent Technologies

## System Information

### Guidance

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument system name and ID	
Instrument system site and location	
SECOT, Bangkok	
List system component product numbers	List the serial numbers of each component
1. THR-ATOMX	1. 0913201002
2.	2.
3.	3.
4.	4.
5.	5.
6.	6.
7.	7.
8.	8.
9.	9.
10.	10.

## Preparation

- ☒ Discuss any specific issues with the customer prior to starting.
- ☒ Review the instrument logbook.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform general inspection of system for cleanliness
- ☒ Check for proper installation of safety-related parts, assemblies, sensors etc
- ☒ Check for required firmware updates and verify with customers if they would like it installed.

Issued: 30-09-2019, Revision:02

Copyright © 2013

Agilent Technologies

Select pages for required products or Page 2 of 5

Teledyne Tekmar ATOMX Purge and Trap  
Preventive Maintenance Checklist - Standard



Agilent Technologies

## Check External Supplies

- ☐ Section NOT Applicable
- ☒ Verify the gas source is supplying an input pressure of 50 - 100 psi to the ATOMX. If the customer is using a gas cylinder, verify the cylinder is at 500+ psi.
- ☒ Verify that the waste container has sufficient volume to contain the waste generated. Empty if necessary.
- ☒ Replace the DI water supply with fresh DI water.
  - ☐ Make sure the DI water supply is sufficient for sample analysis (1 Liter minimum)
- ☒ Make sure the methanol supply is sufficient for sample analysis.

## Atomx Leak and Pressure Check

- ☐ Section NOT Applicable
- ☒ Scan through the sample log to verify that the purge pressures are staying consistent throughout the daily runs.
- ☒ Use the Teldink software to check the standard pressure.
- ☒ Run a leak check to ensure that the unit is leak tight.

## Inspect ATOMX Hardware

- ☐ Section NOT Applicable
- ☒ Check the tray vial holes for foreign particles. Clean if necessary.
- ☒ Inspect the needle for particles or sample build up. Clean if necessary.
- ☒ Inspect the sparger glassware for damage and/or discoloration that could restrict flow or cause contamination. Replace if necessary.
- ☒ Inspect the drain tubing for clogging. Replace the drain line if necessary.
- ☒ Lubricate the ATOMX Carousel Drive. Refer to the diagram on page 6-25 of the ATOMX User Manual for lubrication points. Teledyne Tekmar recommends using DuPont Krytox lubrication.
- ☒ Lubricate the ATOMX Elevator. Refer to the diagram on page 6-32 of the ATOMX User Manual for lubrication points. Teledyne Tekmar recommends using DuPont Krytox lubrication.

## Restore Instrument

### Guidance

If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Issued: 30-09-2019, Revision:02

Copyright © 2013

Agilent Technologies

Select pages for required products or Page 3 of 5

Teledyne Tekmar ATOMX Purge and Trap  
Preventive Maintenance Checklist - Standard



Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☐ Record the PM service activity in the customer's instrument records/logbook
- ☐ Update/reset instrument maintenance counters as appropriate
- ☐ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☐ Complete the Service Engineer Comments section below if there are additional comments
- ☐ Review the service and any test results with the customer.
- ☐ If the Instrument firmware was updated, record the details of the change in the Service Engineer's Comments box below or if necessary, in the customer's IQ records.

Product or Product Type Test Results Table

Test Description	Expected Test Result	Actual Test Result
Leak Test	Pass	Pass

Product or Product Type Parts List Table

Part Description	Part Number	Product or Model# where used	Quantity Consumed
Sparger Glassware	Ask the customer what size sparger glassware they are using; refer to the ATOMX parts list for part numbers.	TMR-ATOMX	1
Lubricant, Dupont Krytox	15-0293-000	TMR-ATOMX	1
Tubing, Drain, Self Retracting	15-0087-002	TMR-ATOMX	1

Issued: 30-09-2019, Revision: 02

Copyright © 2013

Agilent Technologies

Select pages for required products or Page 4 of 5

Teledyne Tekmar ATOMX Purge and Trap  
Preventive Maintenance Checklist - Standard



Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write in this box.

Other Important Customer Web Links

- ☐ How to get information on your product: Literature Library - <http://www.agilent.com/chem/library>
- ☐ Need to know more? - [www.agilent.com/chem/education](http://www.agilent.com/chem/education)
- ☐ Need technical support, FAQs? - [www.agilent.com/chem/techsupp](http://www.agilent.com/chem/techsupp)
- ☐ Need supplies? - [www.agilent.com/chem/supplies](http://www.agilent.com/chem/supplies)

Service Completion

Service request number 6005830843 Date service completed 22 Feb 2023

Agilent signature [Signature] Customer signature [Signature]

Number of pages in this document \_\_\_\_\_

Issued: 30-09-2019, Revision: 02

Copyright © 2013

Agilent Technologies

Select pages for required products or Page 5 of 5

ภาคผนวก จ

---

หนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
จากกรมโรงงานอุตสาหกรรม



ที่ อก ๐๓๑๐(๑)/ ๑๑ ๐๑ ๖

กรมโรงงานอุตสาหกรรม  
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท  
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๐ กรกฎาคม ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท ซีคอต จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๗ เมษายน ๒๕๖๖

- สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น  
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น  
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๙ แผ่น

ตามหนังสือที่อ้างถึง บริษัท ซีคอต จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๓๙ สถานที่ ตั้งเลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ซีคอต จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

- ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐ ราย ตามสิ่งที่ส่งมาด้วย ๑  
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๘ ราย ตามสิ่งที่ส่งมาด้วย ๒  
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ พฤษภาคม ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม คำทรงษ์)

กองวิจัยและเตือนภัยมลพิษโรงงาน

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน  
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๔

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"



ส่งที่ส่งมาด้วย ๑

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท ซีคอต จำกัด

เลขทะเบียน ว-๒๓๙

ที่ อก ๐๓๑๐(๑)/ ๑๑ ๐๑ ๖

ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๖

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐ ราย

- ๑) นายขรรชัย เกรียงไกรอุดม  
๒) นางสมฤดี เกรียงไกรอุดม  
๓) นางอารยา ทิพรัักษ์  
๔) นางสาวเชมชุดา อินทร์ศรี  
๕) นางสาวปรีดา สมใจ  
๖) นางสาวอรุณญา มาดา  
๗) นางสาวลดาวัลย์ วงศ์เจริญ  
๘) นางสาวณัฏฐพร เกตวันดี  
๙) นางสาวนริสา ภูวสรเพ็ชญ์  
๑๐) นางสาวศิริวรรณ นิยมสง่า

- ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๐๒  
ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๐๓  
ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๐๔  
ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๐๕  
ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๐๖  
ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๐๗  
ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๐๘  
ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๐๙  
ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๑๐  
ทะเบียนเลขที่ ว-๒๓๙-ก-๐๐๑๑

วิมล

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
บริษัท ซีคอฟ จำกัด เลขทะเบียน ว-๒๓๙  
ที่ อก ๐๓๑๐(๑)/ ๑๑ ๐๑ ๖ ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย ๒

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๘ ราย

๑) นางสาวสุตาพร สุนทร	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๑
๒) นางสาวสุชาทิพย์ เทียนเคี้ยว	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๓
๓) นางสาวสุนันทา ศิริวัฒนานนท์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๔
๔) นายบวร ศิขัยยะ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๕
๕) นางสาวเกศรินทร์ วรเดชาวิทยา	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๖
๖) นายอนันต์ วัฒนวันนา	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๗
๗) นายชิตพล สมประสงค์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๘
๘) นางสาวศศิธร พรหมประเสริฐ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๐๙
๙) นายศิวะนนท์ กุลวงษ์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๐
๑๐) นางสาวอลิษา คณิรานนท์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๑
๑๑) นางสาวสิริวรรณ แก้วชิงดวง	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๒
๑๒) นางสาวปัทมวรรณ สุวรรณวิโรจน์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๓
๑๓) นางสาวกนิษฐา เจริญเชื้อ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๔
๑๔) นายวิชรกานต์ ประมาคเต	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๕
๑๕) นายชอง เสงขลกุล	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๖
๑๖) นางสาวกฤษณา จันทุม	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๗
๑๗) นางสาวพนภา บุตรธรรม	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๘
๑๘) นางสาวธาริณี อาจปลิว	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๑๙
๑๙) นายอนันต์ ช่างล้อ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๐
๒๐) นางสาวพัชรา สมานันท์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๑
๒๑) นางสาวจุฑารัตน์ แจ่มเรือน	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๒
๒๒) นางสาวจณิสตา กุ้ยอ่อน	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๓
๒๓) นายกิตติพงศ์ ณะเกิงสุข	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๔
๒๔) นายจิรวัฒน์ โคตรคำหาญ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๕
๒๕) นายชนะพล อัครผล	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๖
๒๖) นางสาวทิพย์สุดา วรรณการ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๗
๒๗) นายสิทธิชัย สว่างวงศ์ไชย	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๘
๒๘) นายพิษณุ สีนามเพ็ง	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๒๙
๒๙) นายรัตนชัย ขอบทำกิจ	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๐
๓๐) นายธนาวุฒิ ค่วนแสง	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๑
๓๑) นายณัฐชัย ไชยโคตร	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๒
๓๒) นายณัฐดนัย กฤษณะโสม	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๓
๓๓) นายศุภชัย สุขใหม่	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๔
๓๔) นายรอมฎอน เหลี่ยมหมาด	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๕
๓๕) นางสาวสุภาวดี บัวแก้ว	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๖
๓๖) นางสาวมาริยาณี ฮาแว	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๗
๓๗) นางสาววิระยา ปัจฉิมบุรณ์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๘
๓๘) นางสาวศลิษา อินทรีย์	ทะเบียนเลขที่	ว-๒๓๙-จ-๐๐๓๙

3/11/1

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
บริษัท ซีคอฟ จำกัด เลขทะเบียน ว-๒๓๙  
ที่ อก ๐๓๑๐(๑)/ ๑๑ ๐๑ ๖ ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย ๓

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๕๕ รายการ

น้ำเสีย จำนวน 45 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
3	Barium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
4	α-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
5	β-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
6	δ-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
7	γ-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>

3/11/1



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method <sup>[4]</sup> 2) 5-Day BOD Test, Membrane Electrode Method <sup>[4]</sup>
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
10	Chemical Oxygen Demand	1) Open Reflux, Titrimetric method <sup>[4]</sup> 2) Closed Reflux, Colorimetric method <sup>[4]</sup> 3) Closed Reflux, Titrimetric Method <sup>[4]</sup>
11	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
12	Chromium	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method <sup>[4]</sup>
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
15	Cyanide	Distillation, Colorimetric method <sup>[4]</sup>
16	4,4'-DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	4,4'-DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
18	4,4'-DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
19	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
20	Endosulfan I	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
21	Endosulfan II	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
22	Endosulfan Sulfate	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
23	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
24	Endrin Aldehyde	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
25	Formaldehyde	Distillation, Colorimetric Method <sup>[3]</sup>
26	Free Chlorine	1) Iodometric Method <sup>[4]</sup> 2) DPD Colorimetric Method <sup>[4]</sup>
27	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass-Spectrometric Method <sup>[4]</sup>
28	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
29	Hexavalent Chromium	1) Colorimetric Method <sup>[4]</sup> 2) Extraction, Air-Acetylene Flame Method <sup>[4]</sup>
30	Lead	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
31	Manganese	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
32	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[4]</sup>
33	Methoxychlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
34	Nickel	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup>

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
35	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method <sup>[4]</sup> 2) Soxhlet Extraction Method <sup>[4]</sup>
36	pH	Electrometric Method <sup>[4]</sup>
37	Phenols	1) Distillation, Chloroform Extraction Method <sup>[4]</sup> 2) Distillation, Direct Photometric Method <sup>[4]</sup>
38	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
39	Sulfide	1) Iodometric method <sup>[4]</sup> 2) Methylene blue method <sup>[4]</sup>
40	Temperature	Laboratory and Field Methods <sup>[4]</sup>
41	Total Dissolved Solids	Dried at 180 °C <sup>[4]</sup>
42	Total Kjeldahl Nitrogen	1) Macro Kjeldahl Method <sup>[4]</sup> 2) Semi-Micro Kjeldahl Method <sup>[4]</sup>
43	Total Suspended Solids	Dried at 103-105 °C <sup>[4]</sup>
44	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method; Colorimetric Method; Calculation <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation <sup>[4]</sup>
45	Zinc	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>


น้ำใต้ดิน จำนวน 125 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
2	Acetone	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
3	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
5	Antimony	Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
8	Barium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
10	Benzene	Purge and Trap Gas Chromatographic/Mass spectrometric Method <sup>[4]</sup>
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup> 3 มล)


ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
15	Benzo(g,h,i)perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
16	Beryllium	Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
20	Bromoform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
21	Butanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
23	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
25	Carbon disulfide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup> 3 มล)

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
29	Chlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
31	Chloroform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
34	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method; Colorimetric Method; Calculation <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Spectrometric Method; Colorimetric Method; Calculation <sup>[4]</sup>
35	Chromium (VI)	1) Colorimetric Method <sup>[4]</sup> 2) Extraction, Air-Acetylene Flame Method <sup>[4]</sup>
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup> <i>ส่งมป</i>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
37	Cyanide	1) Distillation, Titrimetric Method <sup>[4]</sup> 2) Distillation, Colorimetric Method <sup>[4]</sup>
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
39	DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
40	DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
41	DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
44	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
45	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
46	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
47	3,3'-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup> <i>ส่งมป</i>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
54	1,2-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
57	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
64	Endosulfan	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 

2) Liquid-Liquid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
65	Endrin	2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup> 1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
66	Ethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
69	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
70	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
72	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
73	n-Hexane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
74	$\alpha$ -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
75	$\beta$ -HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 

2) Liquid-Liquid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
76	$\gamma$ -HCH	2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup> 1) Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup> 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
82	Manganese	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[4]</sup>
84	Methanol	Purge and Trap Gas Chromatographic/ Mass spectrometric Method <sup>[4]</sup>
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
86	Methyl bromide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>

87 Methylene chloride...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
87	Methylene chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
89	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
90	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
96	Polychlorinated Biphenyls - PCB-1016 - PCB-1221 - PCB-1232 - PCB-1242 - PCB-1248 - PCB-1254 - PCB-1260	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
98	pH	Electrometric method <sup>[4]</sup>

99 Phenanthrene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
100	Phenol	1) Distillation, Chloroform Extraction Method <sup>[4]</sup> 2) Distillation, Direct Photometric Method <sup>[4]</sup> 3) Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
102	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
103	Silver	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
104	Styrene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
107	Toluene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
108	TPH (C <sub>5</sub> -C <sub>8</sub> )	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[12,25]</sup>
109	TPH (C <sub>8</sub> -C <sub>16</sub> )	1) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[9,21]</sup> 2) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass spectrometric Method <sup>[9,25]</sup>
110	TPH (C <sub>16</sub> -C <sub>35</sub> )	1) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[9,21]</sup> <i>sim</i>

2) Separatory...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass spectrometric Method <sup>[9,25]</sup>
111	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
112	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
113	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
114	Trichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
115	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
116	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
117	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
118	Vanadium	Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
119	Vinyl acetate	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
120	Vinyl chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
121	m-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
122	o-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
123	p-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup>
124	Xylene (Total)	Purge and Trap Gas Chromatographic/Mass Spectrometric Method <sup>[4]</sup> <i>sim</i>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
125	Zinc	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>

อากาศเสีย (ปล่อยระบาย) จำนวน 27 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
2	Arsenic	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
3	Beryllium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
4	Cadmium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
5	Carbon monoxide	Instrumental Analyzer Method <sup>[5]</sup>
6	Chlorine	1) Absorption Sampling, Ion Chromatographic Method <sup>[5]</sup> 2) Isokinetic Sampling, Ion Chromatographic Method <sup>[5]</sup>
7	Chromium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup> 3mg/L

8 Cobalt...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
9	Copper	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
10	Cresol	Adsorption Sampling, Gas Chromatographic Method <sup>[5]</sup>
11	Dioxin/Furans	Isokinetic Sampling <sup>[5]</sup>
12	Hydrogen chloride	1) Absorption Sampling, Ion Chromatographic Method <sup>[5]</sup> 2) Isokinetic Sampling, Ion Chromatographic Method <sup>[5]</sup>
13	Hydrogen Fluoride	1) Absorption Sampling, Ion Chromatographic Method <sup>[5]</sup> 2) Isokinetic Sampling, Ion Chromatographic Method <sup>[5]</sup>
14	Hydrogen Sulfide	Absorption Sampling, Iodometric Method <sup>[5]</sup>
15	Lead	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
16	Manganese	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
17	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[5]</sup>
18	Nickel	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup> 3mg/L

19 Opacity...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Opacity	Ringelmann's Method <sup>[2]</sup>
20	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method <sup>[5]</sup> 2) Absorption Sampling, Ion Chromatographic Method <sup>[5]</sup> 3) Instrumental Analyzer Method <sup>[5]</sup>
21	Selenium	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
22	Sulfur dioxide	1) Isokinetic Sampling, Barium-Thorin Titrimetric Method <sup>[5]</sup> 2) Absorption Sampling, Barium-Thorin Titrimetric Method <sup>[5]</sup> 3) Instrumental Analyzer Method <sup>[5]</sup>
23	Sulfuric acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method <sup>[5]</sup>
24	Tin	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
25	Total Suspended Particulate	1) Isokinetic Sampling, Gravimetric Method <sup>[5]</sup> 2) Paired Train, Isokinetic Sampling, Gravimetric Method <sup>[5]</sup>
26	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
27	Xylene	1) Adsorption Sampling, Gas Chromatographic Method <sup>[5]</sup> 2) Adsorption Sampling, Gas Chromatographic/ Mass Spectrometric Method <sup>[5]</sup>

สิ่งปฏิกูล...

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 34 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,6,9,22]</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[1,6,9,27]</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
2	Antimony	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
3	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
4	Barium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,15]</sup>

2) Waste Extraction...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
5	Beryllium	2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
7	Chlordane	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
8	Chromium	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,9,22]</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[1,9,27]</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup> 1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> <i>3) Digestion...</i>

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
9	Chromium (III)	3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup> 1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation <sup>[1,6,15,17]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation <sup>[1,6,14,17]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation <sup>[7,8,15,17]</sup> 4) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation <sup>[7,8,14,17]</sup>
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method <sup>[1,17]</sup> 2) Alkaline Digestion, Colorimetric Method <sup>[8,17]</sup>
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup> <i>3) Digestion...</i>

13 2,4-D...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	2,4-D	1) Waste Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(1,25)</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(25)</sup>
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(1,9,22)</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(1,9,27)</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,27)</sup>
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(1,9,22)</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(1,9,27)</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,27)</sup>
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(1,9,22)</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(1,9,27)</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,27)</sup>

17 Dieldrin...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(1,9,22)</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(1,9,27)</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,27)</sup>
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(1,9,22)</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(1,9,27)</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,27)</sup>
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>(1,9,22)</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(1,9,27)</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>(10,22)</sup> 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>(10,27)</sup>
20	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>(1,6,15)</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>(1,6,14)</sup>

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
21	Lindane	3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup> 1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,9,22]</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,27]</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[1,18]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[19]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,9,22]</sup> 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,27]</sup> 3) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup> 4) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>


24 Molybdenum...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
24	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
25	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
26	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,9,23]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
27	Pentachlorophenol	1) Waste Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,25]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[25]</sup>
28	pH	Electrometric Method <sup>[31,32]</sup>
29	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[1,6,20]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,20]</sup>


4) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
30	Silver	4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
31	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
32	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[1,12,26]</sup> 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[12,26]</sup>
33	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
34	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,15]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,14]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>

ดิน จำนวน 124 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup> 

2 Acetone...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
3	Aldrin	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
4	Anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
5	Antimony	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
7	Atrazine	Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,24]</sup>
8	Barium	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
9	Benz(a)anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
10	Benzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
11	Benzo(b)fluoranthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
12	Benzo(k)fluoranthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
13	Benzoic acid	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup> 

14 Benzo(a)pyrene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
14	Benzo(a)pyrene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
15	Benzo(g,h,i)perylene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
16	Beryllium	Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
17	Bis(2-chloroethyl)ether	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
18	Bis(2-ethylhexyl)phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[13,26]</sup>
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[13,26]</sup>
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[13,26]</sup>
22	Butyl benzyl phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
23	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
24	Carbazole	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[13,26]</sup>
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[13,26]</sup>
27	Chlordane	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[11,27]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
28	p-Chloroaniline	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[13,26]</sup>
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[13,26]</sup>
31	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
32	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
34	Chromium (III)	1) Digestion, Flame Atomic Absorption Spectrometric Method; Colorimetric Method; Calculation <sup>[7,8,15,17]</sup> 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation <sup>[7,8,14,17]</sup>
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method <sup>[8,17]</sup>
36	Chrysene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
37	Cyanide	1) Extraction, Distillation, Titrimetric Method <sup>[28,29,30]</sup> 2) Extraction, Distillation, Colorimetric Method <sup>[28,29,30]</sup>
38	2,4-D	Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[24]</sup>
39	DDD	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[11,27]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	DDE	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
41	DDT	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
42	Dibenz(a,h)anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
43	Di-n-butyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
47	3,3'-Dichlorobenzidine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
53	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>

54 1,2-Dichloropropane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
57	Dieldrin	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
58	Diethyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
59	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
60	2,4-Dinitrophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
61	2,4-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
62	2,6-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
63	Di-n-Octyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
64	Endosulfan	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
65	Endrin	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>

67 Fluoranthene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
67	Fluoranthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
68	Fluorene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,27]</sup>
69	Heptachlor	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[11,27]</sup>
70	Heptachlor epoxide	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[11,27]</sup>
71	Hexachlorobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[13,26]</sup>
74	α-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[11,27]</sup>
75	β-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[11,27]</sup>
76	γ-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[11,27]</sup>
77	Hexachlorocyclopentadiene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>

78 Hexachloroethane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
78	Hexachloroethane	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
79	Indeno(1,2,3-cd)pyrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
80	Isophorone	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
81	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
82	Manganese	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[19]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
84	Methanol	Ultrasonic Extraction, Direct Aqueous Injection, Gas Chromatographic Method <sup>[11,21]</sup>
85	Methoxychlor	1) Ultrasonic Extraction, Gas Chromatographic Method <sup>[11,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[11,27]</sup>
86	Methyl bromide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
87	Methylene chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
88	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
89	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>

90 Methyl tert-butyl ether...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
91	Naphthalene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
92	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
93	Nitrobenzene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
94	N-Nitrosodiphenylamine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
95	N-Nitrosodi-n-propylamine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
96	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
97	Pentachlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[24]</sup>
98	Phenanthrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
99	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[11,27]</sup>
100	Pyrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,27]</sup>
101	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,20]</sup>

2) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
102	Silver	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,14]</sup>
103	Styrene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
106	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
107	TPH (C <sub>5</sub> -C <sub>9</sub> )	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
108	TPH (C <sub>8</sub> -C <sub>16</sub> )	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,21]</sup> 2) Soxhlet Extraction, Gas Chromatographic/Mass spectrometric Method <sup>[10,26]</sup>
109	TPH (C <sub>15</sub> -C <sub>35</sub> )	1) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,21]</sup> 2) Soxhlet Extraction, Gas Chromatographic/Mass spectrometric Method <sup>[10,26]</sup>
110	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
111	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
112	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>
113	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[13,26]</sup>

114 2,4,5-Trichlorophenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
114	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>(11,27)</sup>
115	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>(11,27)</sup>
116	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(13,26)</sup>
117	Vanadium	Digestion, Inductively Coupled Plasma Method <sup>(7,14)</sup>
118	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass spectrometric Method <sup>(13,26)</sup>
119	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(13,26)</sup>
120	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(13,26)</sup>
121	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(13,26)</sup>
122	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(13,26)</sup>
123	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>(13,26)</sup>
124	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>(7,15)</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>(7,14)</sup>

#### เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แก๊สเป็นเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

4. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 23<sup>rd</sup> ed. Washington, DC: APHA, 2017.
5. United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2023.
6. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846, 2020.
7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B, 1996.
8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A, 1996.
9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C, 1996.
10. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soxhlet Extraction. SW-846 Method 3540C, 1996.
11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction. SW-846 Method 3550C, 2007.
12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Purge-and-Trap for Aqueous Samples. SW-846 Method 5030C, 2003.
13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035, 1996.
14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Inductively Coupled Plasma-optical Emission Spectrometry. SW-846 Method 6010D, 2018.
15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B, 2007.
16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Antimony and Arsenic (Atomic Absorption, Borohydride Reduction). SW-846 Method 7062, 1994.

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Chromium, Hexavalent (Colorimetric), SW-846 Method 7196A, 1992.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Mercury in Liquid Waste (Manual Cold-Vapor Technique, SW-846 Method 7470A, 1994.

19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique, SW-846 Method 7471B, 2007.

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Selenium (Atomic Absorption, Borohydride Reduction), SW-846 Method 7742, 1994.

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D, 2003.


22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Organochlorine Pesticide by Gas Chromatography. SW-846 Method 8081B, 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Polychlorinated Biphenyls (PCBs) By Gas Chromatography. SW-846 Method 8082A, 2007.

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Organophosphorus Compounds by Gas Chromatography. SW-846 Method 8141B, 2007.

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Chlorinated Herbicides By GC Using Methylation or Pentafluorobenzoylation Derivatization. SW-846 Method 8151A, 1996.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8260D, 2018.

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SemiVolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E, 2018. 


28. United States...

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Total and Amenable Cyanide: Distillation. SW-846 Method 9010C, 2004.

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Cyanide Extraction Procedure for Solids and Oils. SW-846 Method 9013A, 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric. SW-846 Method 9014, 2014.

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. pH Electrometric Measurement. SW-846 Method 9040C, 2004.

32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Solid and Waste pH. SW-846 Method 9045D, 2004. 

ภาคผนวก ข

ใบรับรองความสามารถห้องปฏิบัติการ  
และขอบข่ายการรับรองห้องปฏิบัติการทดสอบ  
ตามมาตรฐาน ISO/IEC 17025 จากสำนักงานมาตรฐานอุตสาหกรรม



แบบ กษ./สมอ.๒  
Form NSC/TISI 2

ใบรับรองเลขที่ 24-LB0026  
(Certificate No.)

## ใบรับรองระบบงาน (Certificate of Accreditation)

อาศัยอำนาจตามความในพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑  
(By Virtue of National Standardization Act B.E. 2551 (2008))

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Secretary-General, Thai Industrial Standards Institute)

ออกใบรับรองฉบับนี้ให้  
(Issues this certificate to)

บริษัท ซีคอต จำกัด ฝ่ายห้องปฏิบัติการทดสอบด้านสิ่งแวดล้อม  
(Secot Company Limited, Environmental Laboratory Division)

ตั้งอยู่เลขที่  
(Address)

๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร  
(239 Rimkongprapa Road, Bangsue, Bangsue, Bangkok)

ได้รับการรับรองความสามารถ  
(Certificate of competence)

ตามมาตรฐานเลขที่ มอก. ๑๗๐๒๕ - ๒๕๖๑  
(Standard No. TIS 17025-2561 (2018) (ISO/IEC 17025: 2017))

ข้อกำหนดทั่วไปว่าด้วยความสามารถของ ห้องปฏิบัติการทดสอบและห้องปฏิบัติการสอบเทียบ  
(General requirements for the competence of testing and calibration laboratories)

หมายเลขการรับรองที่ ทดสอบ ๐๓๙๔  
(Accreditation No. Testing 0394)

โดยมีรายละเอียดสาขาและขอบข่ายที่ใบรับรอง แสดงไว้ใน QR CODE และ [www.tisi.go.th](http://www.tisi.go.th)  
(Details of the scheme and scope of the certificate are shown in QR CODE and [www.tisi.go.th](http://www.tisi.go.th))

ออกให้ ณ วันที่ ๖ ธันวาคม พ.ศ. ๒๕๖๖  
(Issue date : 6 December B.E. 2566 (2023))

  
(นายวีระศักดิ์ เพ็งหล่ง)  
(นายวีระศักดิ์ เพ็งหล่ง)

ผู้อำนวยการสำนักงานคณะกรรมการการมาตรฐานแห่งชาติ  
ปฏิบัติราชการแทน  
เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม



Signed by สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม (สมอ.)  
Thai Industrial Standards Institute (TISI)  
Date: 2023-12-06T08:49:04 476+07:00

กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Ministry of Industry Thailand, Thai Industrial Standards Institute)



รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)  
ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ชื่อห้องปฏิบัติการ  
(Laboratory Name)

หมายเลขการรับรองที่  
(Accreditation No.)

ฉบับที่ 02  
(Issue No.02)

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

บริษัท ซีคอต จำกัด ฝ่ายห้องปฏิบัติการทดสอบด้านสิ่งแวดล้อม  
(Secot Company Limited, Environmental Laboratory Division)

ทดสอบ 0394  
(Testing 0394)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

☒ถาวร  
(Permanent)

☐นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสังแวดล้อม (environmental field) 1. น้ำและน้ำเสีย (water and wastewater)	- โลหะหนัก (heavy metals) • สารหนู (Arsenic, As) 0.000 5 mg/L ถึง 0.090 0 mg/L  • สารหนู (Arsenic, As) 0.05 mg/L ถึง 4.50 mg/L  • แบเรียม (Barium, Ba) 0.02 mg/L ถึง 4.50 mg/L  • แคดเมียม (Cadmium, Cd) 0.01 mg/L ถึง 4.50 mg/L  • โครเมียม (Chromium, Cr) 0.01 mg/L ถึง 4.50 mg/L	- Standard Methods for the Examination of Water and Wastewater, APHA , AWWA, WEF, 23 <sup>rd</sup> edition , 2017, Part 3030 F and Part 3114 C  - Standard Methods for the Examination of Water and Wastewater, APHA , AWWA, WEF, 23 <sup>rd</sup> edition , 2017, Part 3030 E and Part 3120 B

กระทรวงอุตสาหกรรมสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม  
(Ministry of Industry, Thai Industrial Standards Institute)

หน้า 1/9

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026

(Certification No. 24-LB0026)



ฉบับที่ 02

(Issue No.02)

ออกให้ตั้งแต่วันที่

(Valid from)

30 ตุลาคม พ.ศ. 2566

(30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571

(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ ถาวร  
(Permanent)

☐ นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>1. น้ำและน้ำเสีย (ต่อ) (water and wastewater) (cont.)</p>	<p>- โลหะหนัก (heavy metals)</p> <ul style="list-style-type: none"> <li>ทองแดง (Copper, Cu) 0.02 mg/L ถึง 4.50 mg/L</li> <li>เหล็ก (Iron, Fe) 0.05 mg/L ถึง 9.00 mg/L</li> <li>ตะกั่ว (Lead, Pb) 0.03 mg/L ถึง 4.50 mg/L</li> <li>แมงกานีส (Manganese, Mn) 0.01 mg/L ถึง 9.00 mg/L</li> <li>นิกเกิล (Nickel, Ni) 0.01 mg/L ถึง 4.50 mg/L</li> <li>สังกะสี (Zinc, Zn) 0.02 mg/L ถึง 9.00 mg/L</li> </ul>	<p>- Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23<sup>rd</sup> edition, 2017, Part 3030 E and Part 3120 B</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026

(Certification No. 24-LB0026)



ฉบับที่ 02

(Issue No.02)

ออกให้ตั้งแต่วันที่

(Valid from)

30 ตุลาคม พ.ศ. 2566

(30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571

(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ ถาวร  
(Permanent)

☐ นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>1. น้ำและน้ำเสีย (ต่อ) (water and wastewater) (cont.)</p>	<p>- ซีโอดี (Chemical oxygen demand, COD) 100 mg/L ถึง 4 000 mg/L</p>	<p>- Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF, 23<sup>rd</sup> edition, 2017, Part 5220 D</p>
<p>2. บริเวณทำงาน (workplace)</p>	<p>- ฝุ่นละอองรวม (Total dust) 0.10 mg/filter ถึง 2.00 mg/filter</p> <p>- ฝุ่นละอองขนาดเล็ก (Respirable dust) 0.10 mg/filter ถึง 2.00 mg/filter</p>	<p>- NIOSH Manual of Analytical Methods (NMAM), method 0500, 4<sup>th</sup> edition, 15<sup>th</sup> August 1994 (Exclude Sampling)</p> <p>- NIOSH Manual of Analytical Methods (NMAM), method 0600, 4<sup>th</sup> edition, 15<sup>th</sup> January 1998 (Exclude Sampling)</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)  
ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))  
สถานภาพห้องปฏิบัติการ ☒ ถาวร (Permanent) ☐ นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>2. บริเวณทำงาน (ต่อ) (workplace) (cont.)</p>	<ul style="list-style-type: none"> <li>เบนซีน (Benzene) 1.10 µg/tube ถึง 420 µg/tube</li> <li>โทลูอีน (Toluene) 1.10 µg/tube ถึง 420 µg/tube</li> <li>โทโครไซลีน (Total xylenes) 2.20 µg/tube ถึง 840 µg/tube</li> <li>เมตา, พารา-ไซลีน (m, p- Xylene) 1.10 µg/tube ถึง 420 µg/tube</li> <li>ออร์โธ-ไซลีน (o- Xylene) 1.10 µg/tube ถึง 420 µg/tube</li> </ul>	<ul style="list-style-type: none"> <li>- NIOSH Manual of Analytical Methods (NMAM) , method 1501, 4<sup>th</sup> edition , 15<sup>th</sup> March 2003 (Exclude Sampling)</li> </ul>
<p>3. ปล่องระบายอากาศ (stack)</p>	<ul style="list-style-type: none"> <li>- ซัลเฟอร์ไดออกไซด์ (Sulfur dioxide ) 1.00 mg/L ถึง 16 000 mg/L (solution)</li> </ul>	<ul style="list-style-type: none"> <li>- US.EPA , Code of Federal Regulations , 40 CFR 60 appendix A , method 6 , July 2019 (Exclude Sampling)</li> </ul>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)  
ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))  
สถานภาพห้องปฏิบัติการ ☒ ถาวร (Permanent) ☐ นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>3. ปล่องระบายอากาศ (ต่อ) (stack) (cont.)</p>	<ul style="list-style-type: none"> <li>- ไฮโดรเจนฟลูออไรด์ (Hydrogen fluoride) 5 µg/sample ถึง 400 µg/sample</li> <li>- ไฮโดรเจนคลอไรด์ (Hydrogen chloride) 5 µg/sample ถึง 400 µg/sample</li> </ul>	<ul style="list-style-type: none"> <li>- WI-7.2-1-22 based on US.EPA , Code of Federal Regulations , 40 CFR 60 appendix A, method 26 , 2019 (Exclude Sampling)</li> </ul>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026

(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☒นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ambient air)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs)</p> <ul style="list-style-type: none"> <li>คลอโรเอทีน (Chloroethene) 0.05 <math>\mu\text{g}/\text{m}^3</math> ถึง 51.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>1,3-บิวทาไดเอิน (1,3-butadiene) 0.04 <math>\mu\text{g}/\text{m}^3</math> ถึง 44.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>โบรมอมีเทน (Bromomethane) 0.08 <math>\mu\text{g}/\text{m}^3</math> ถึง 77.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>อะครอลีน (Acrolein) 0.05 <math>\mu\text{g}/\text{m}^3</math> ถึง 45.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> </ul>	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ

(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026

(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☒นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)</p>	<p>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs)</p> <ul style="list-style-type: none"> <li>อะครีโลไนไตรล์ (Acrylonitrile) 0.04 <math>\mu\text{g}/\text{m}^3</math> ถึง 43.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>ไดคลอโรมีเทน (Dichloromethane) 0.14 <math>\mu\text{g}/\text{m}^3</math> to 69.00 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>คาร์บอนไดซัลไฟด์ (Carbon disulfide) 0.06 <math>\mu\text{g}/\text{m}^3</math> ถึง 62.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>ไตรคลอโรมีเทน (Trichloromethane) 0.20 <math>\mu\text{g}/\text{m}^3</math> ถึง 97.00 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>1,2-ไดคลอโรเอทีน (1,2-dichloroethane) 0.08 <math>\mu\text{g}/\text{m}^3</math> ถึง 80.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> </ul>	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>



รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☒นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)</p>	<ul style="list-style-type: none"> <li>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs)</li> <li>• เบนซีน (Benzene) 0.06 <math>\mu\text{g}/\text{m}^3</math> ถึง 63.00 <math>\mu\text{g}/\text{m}^3</math> (0.02 ppbv ถึง 20.00 ppbv)</li> <li>• คาร์บอนเตตระคลอไรด์ (Carbon tetrachloride) 0.25 <math>\mu\text{g}/\text{m}^3</math> ถึง 125 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>• ไตรคลอโรเอทิลีน (Trichloroethylene) 0.21 <math>\mu\text{g}/\text{m}^3</math> ถึง 107 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>• 1,2-ไดคลอโรโพรเพน (1,2-dichloropropane) 0.18 <math>\mu\text{g}/\text{m}^3</math> ถึง 92.00 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>• เตตระคลอโรเอทิลีน (Tetrachloroethylene) 0.27 <math>\mu\text{g}/\text{m}^3</math> ถึง 135 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> </ul>	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ  
(Scope of Accreditation for Testing)

ใบรับรองเลขที่ 24-LB0026  
(Certification No. 24-LB0026)



ฉบับที่ 02  
(Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566  
(Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571  
(Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ  
(Laboratory status)

☒ถาวร  
(Permanent)

☒นอกสถานที่  
(Site)

☐ชั่วคราว  
(Temporary)

☐เคลื่อนที่  
(Mobile)

☐หลายสถานที่  
(Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
<p>สาขาส่งแวดล้อม (environmental field)</p> <p>4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)</p>	<ul style="list-style-type: none"> <li>- สารอินทรีย์ระเหยง่าย (Volatile organic compounds ,VOCs)</li> <li>• 1,2-ไดโบรมออีเทน (1,2-dibromoethane) 0.31 <math>\mu\text{g}/\text{m}^3</math> ถึง 153 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> <li>• 1,1,2,2-เตตระคลอโรอีเทน (1,1,2,2-tetrachloroethane) 0.69 <math>\mu\text{g}/\text{m}^3</math> ถึง 137 <math>\mu\text{g}/\text{m}^3</math> (0.10 ppbv ถึง 20.00 ppbv)</li> <li>• เบนซิลคลอไรด์ (Benzyl chloride) 0.52 <math>\mu\text{g}/\text{m}^3</math> ถึง 103 <math>\mu\text{g}/\text{m}^3</math> (0.10 ppbv ถึง 20.00 ppbv)</li> <li>• 1,4-ไดคลอโรเบนซีน (1,4-dichlorobenzene) 0.24 <math>\mu\text{g}/\text{m}^3</math> ถึง 120 <math>\mu\text{g}/\text{m}^3</math> (0.04 ppbv ถึง 20.00 ppbv)</li> </ul>	<p>- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999</p>

ภาคผนวก ข

ใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัด  
และวิเคราะห์สถานะการทำงาน  
จากกรรมสวัสดิการและคุ้มครองแรงงาน



แบบ กก.บญ  
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน  
ใบอนุญาต  
เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับแสงสว่าง

ใบอนุญาตเลขที่ ๑๕๐๒-๐๓-๒๕๖๕-๐๐๔๙

อนุญาตให้.....บริษัท ซีตอท จำกัด.....

เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๒๐๐๑๙๗๖

ตั้งอยู่เลขที่ ๒๓๙ ถนนวิมลอุบลประจักษ์ แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวงกำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงานเกี่ยวกับความร้อน แสงสว่าง และเสียง พ.ศ. ๒๕๕๙ ในการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับแสงสว่าง ประกอบกับกฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริม ความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๕ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม

ข-๑๑-๐๔๐๒-๐๔๙-๐๓-๖๕

(ลงนาม)

(นายศักดิ์ศิลป์ ดุลาธร)

ตำแหน่ง ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากร (เพิ่มเติม)  
แนบท้ายใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สถานะการทำงานเกี่ยวกับระดับแสงสว่าง  
ของบริษัท ซีคอท จำกัด

ใบอนุญาตเลขที่ ๐๔๐๒-๐๓๑๕๖๕-๐๐๔๙

- |                   |           |
|-------------------|-----------|
| ๑. นางสาวศลิษา    | อินริย์   |
| ๒. นางสาวมาริยาณี | ชานแว     |
| ๓. นางสาววิระยา   | ปัจฉิมบุญ |

ทั้งนี้ ตั้งแต่วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖



(นายสมพจน์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต  
เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สถานะการทำงานเกี่ยวกับระดับแสงสว่าง  
ของบริษัท ซีคอท จำกัด

ใบอนุญาตเลขที่ ๐๔๐๒-๐๓-๒๕๖๕-๐๐๔๙

- |                   |                |
|-------------------|----------------|
| ๑. นางสาวสุนันทา  | ศิริวัฒน์วนนท์ |
| ๒. นางสาวกนิษฐา   | เจริญเชื้อ     |
| ๓. นางสาวปัทมวรรณ | สุวรรณวิโรจน์  |
| ๔. นางสาวอลิษา    | คณิวรานนท์     |
| ๕. นางสาวชนิดา    | หล้าสาย        |

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕



(นายสมพจน์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน



แบบ ภ.บญ  
ฉ.1/คค

กรมสวัสดิการและคุ้มครองแรงงาน

ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับความร้อน

ใบอนุญาตเลขที่ ๑๔๑๑-๑๓-๒๕๖๕-๑๑๔๘

อนุญาตให้ บริษัท ชีคอต จำกัด

เลขทะเบียนนิติบุคคล ๐๘๐๕๕๓๖๐๐๐๑๖๖

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวง กำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงานเกี่ยวกับความร้อน แสงสว่าง และเสียง พ.ศ. ๒๕๕๙ ในการตรวจวัดและวิเคราะห์สภาวะการทำงาน เกี่ยวกับระดับความร้อน ประกอบกับกฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริม ความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๕ ราย ดังรายชื่อแนบท้าย ใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม

ข-๑๓-๐๔๐๑-๐๔๘-๐๓-๖๕

(ลงนาม)  (นายทะเบียน)

(นายศักดิ์สิทธิ์ ตูลาธร)

ตำแหน่ง ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากร (เพิ่มเติม)  
แนบท้ายใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับความร้อน  
ของบริษัท ซีคोट จำกัด

ใบอนุญาตเลขที่ ๐๔๐๑-๐๓-๒๕๖๕-๐๐๔๘

- |                   |             |
|-------------------|-------------|
| ๑. นางสาวศลิษา    | อินริย์     |
| ๒. นางสาวมาริยาณี | ฮาแว        |
| ๓. นางสาววิระยา   | ปัจฉิมบุรณ์ |

ทั้งนี้ ตั้งแต่วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖



(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน


รายชื่อบุคลากรแนบท้ายใบอนุญาต  
เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับความร้อน  
ของบริษัท ซีคोट จำกัด

ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

- |                   |                |
|-------------------|----------------|
| ๑. นางสาวสุนันทา  | ศิริคุณิณานนท์ |
| ๒. นางสาวกนิษฐา   | เจริญเชื้อ     |
| ๓. นางสาวปัทมวรรณ | สุวรรณวิโรจน์  |
| ๔. นางสาวอลิษา    | คณิธรานนท์     |
| ๕. นางสาวชนิดา    | หล้าสาย        |

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕



(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน



แบบ กภ.บุญ  
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน

ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาพการทำงานเกี่ยวกับระดับเสียง

ใบอนุญาตเลขที่ ๑๔๑๓-๐๓-๒๕๖๕-๑๑๔๔

อนุญาตให้.....บริษัท ซีแอล จิวเก็ด.....

เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๖๐๐๑๙๗๖

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประเวศ แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวงกำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงานเกี่ยวกับความร้อน แสงสว่าง และเสียง พ.ศ. ๒๕๕๙ ในการตรวจวัดและวิเคราะห์สภาพการทำงานเกี่ยวกับระดับเสียง ประกอบกับกฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริม ความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๕ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม

ข-๑๑-๐๔๐๓-๐๔๘-๐๑-๖๕

(ลงนาม)

(นายทะเบียน)

(นายศักดิ์ศิลป์ ตูลาธร)

ตำแหน่ง ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากร (เพิ่มเติม)  
แนบท้ายใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาพการทำงานเกี่ยวกับระดับเสียง  
ของบริษัท ซีคอท จำกัด

ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

- |                   |             |
|-------------------|-------------|
| ๑. นางสาวศลิษา    | อินริย์     |
| ๒. นางสาวมาธิยาณี | ยาแว        |
| ๓. นางสาววิระยา   | ปัจฉิมบุรณ์ |

ทั้งนี้ ตั้งแต่วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖



(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต  
เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาพการทำงานเกี่ยวกับระดับเสียง  
ของบริษัท ซีคอท จำกัด

ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

- |                   |                |
|-------------------|----------------|
| ๑. นางสาวสุนันทา  | ศิริพัฒน์นันท์ |
| ๒. นางสาวกนิษฐา   | เจริญเชื้อ     |
| ๓. นางสาวปัทมวรรณ | สุวรรณวิโรจน์  |
| ๔. นางสาวอลิษา    | คณิธรานนท์     |
| ๕. นางสาวชนิตา    | หล้าสาย        |

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕



(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน





ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตราย  
ในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย

ใบอนุญาตเลขที่ ๐๒๐๑-๐๓-๒๕๖๕-๐๐๔๙

อนุญาตให้ บริษัท สีสอน จำกัด

[illegible]

ตั้งอยู่ เลขที่ ๒๓๙ ถนนพหลโยธิน แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร.....

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวง กำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงานเกี่ยวกับสารเคมีอันตราย พ.ศ. ๒๕๕๖ ในการเป็นผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย ประกอบกับกฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริมความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๑๔ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕

*[Signature]*

(นายสมพจน์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม  
๗-๓๓-๐๒๐๓-๐๔๘-๐๓-๖๕

(ลงนาม) \_\_\_\_\_ (นายทะเบียน)

(นายศักดิ์ศิลป์ ตระอา)

ผู้อำนวยการกองความปลอดภัยแรงงาน



แบบ กภ.บุญ  
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน

ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตราย  
ในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย

ใบอนุญาตเลขที่ ๐๒๐๒-๐๓-๒๕๖๕-๐๐๓๔

อนุญาตให้ บริษัท ซีคอน จำกัด

เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๖๐๐๑๙๗๖

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวง  
กำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม  
ในการทำงานเกี่ยวกับสารเคมีอันตราย พ.ศ. ๒๕๕๖ ในการเป็นผู้ให้บริการวิเคราะห์ระดับความเข้มข้น  
ของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย ประกอบกับ  
กฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริมความปลอดภัย อาชีวอนามัย และสภาพแวดล้อม  
ในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน  
พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๑๔ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต  
เป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงาน  
และสถานที่เก็บรักษาสารเคมีอันตราย  
ของบริษัท ซีคอน จำกัด  
ใบอนุญาตเลขที่ ๐๒๐๑-๐๓-๒๕๖๕-๐๐๔๔

๑. นายชิตพล	สมประสงค์
๒. นายอนันต์	พิมวันนา
๓. นายวิวัฒน์	กุลวงษ์
๔. นายวัชรกานต์	ประมาคะเต
๕. นายธนโชติ	ช่างหล่อ
๖. นายกิตติพงษ์	ทะเก็งสุข
๗. นายจิรวัดน์	โคตรคำหาญ
๘. นายศุภกิจ	ศิษฏกา
๙. นางสาวธัญลักษณ์	โยธา
๑๐. นางสาวทิพย์สุดา	วรรณการ
๑๑. นางสาวสายธาร	ภูเขียว
๑๒. นายภาคภูมิ	แทนไทย
๑๓. นายธนาวุฒิ	ด่วนแสง
๑๔. นายรัตนชัย	ชอบทำกิจ

ทั้งนี้ ตั้งแต่วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน

อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต  
เป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงาน  
และสถานที่เก็บรักษาสารเคมีอันตราย  
ของบริษัท ซีคอท จำกัด  
ใบอนุญาตเลขที่ ๐๒๐๒-๐๓-๒๕๖๕-๐๐๓๔

- |                       |              |
|-----------------------|--------------|
| ๑. นางสาวนริสา        | ภูธรเพ็ญ     |
| ๒. นางอารยา           | ทิพักษ์      |
| ๓. นางสาวศิริวรรณ     | ฉิมสง่า      |
| ๔. นางสาวสุชาทิพย์    | เทียนदैย     |
| ๕. นางสาวพรณา         | บุตรธรรม     |
| ๖. นางสาวธารณี        | อาจปลิว      |
| ๗. นางสาวกฤษณา        | จันทุม       |
| ๘. นางสาวพัชรา        | สมานฉันท     |
| ๙. นางสาวจณิสตา       | กัยออน       |
| ๑๐. นางสาวศศิภา       | ใจดี         |
| ๑๑. นางสาวจุฑารัตน์   | แจ่มเรือน    |
| ๑๒. นางสาวณัฐศิริ     | เลิศธีรพัฒน์ |
| ๑๓. นางสาวสัญญาลักษณ์ | อินทระสิทธิ์ |
| ๑๔. นางสาวสุดาพร      | สุนทร        |

ทั้งนี้ ตั้งแต่วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕



(นายสมพงษ์ กวางแก้ว)

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม

๖-๓๓-๐๒๐๒-๐๓๔-๒๕-๖๕

(ลงนาม)  (นายทะเบียน)

(นายศักดิ์ศิลป์ ตูลาธร)

ผู้อำนวยการกองความปลอดภัยแรงงาน