

Certificate of Calibration

Certificate No. : 66-200125-1

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46, Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : Electronic Balance

Manufacturer : SHIMADZU Model : AX200

Serial No. : D432620040 ID No. : 114

Capacity : 200 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (29.3 to 29.9) °C

Relative Humidity : (56.1 to 60) %

Air Pressure : 1007.0 mbar

Date of Received : 19 April 2023

Date of Calibration : 19 April 2023

Date of Issue : 22 April 2023

Calibrated by : Satja Sangkhum

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-200125-1

Page : 2 of 2

Result of Calibration : Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)	Error before Adjustment (g)
0.01	0.0000	0.000085	0.0000
0.1	0.0000	0.000085	0.0000
0.5	0.0001	0.000086	0.0001
1	0.0000	0.00011	0.0001
10	0.0000	0.00012	0.0000
20	-0.0001	0.00011	0.0003
50	0.0000	0.00014	0.0005
100	0.0000	0.00020	0.0005
150	0.0000	0.00038	0.0000
200	0.0004	0.00038	-0.0002

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error Load test : 50 g

A	B	C	D	E	
0.0000	0.0000	0.0000	0.0001	0.0000	g



Repeatability Load test : 200 g

Stdev. : 0.00005 g

- o0o -



Certificate of Calibration

Certificate No. : 66-400195-5

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46, Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : Air Chamber (Oven)

Manufacturer : Memmert

Model : UNB 500

Range : N/A °C

Resolution : 0.5 °C

Serial No. : C507.1007

ID No. : 012

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (25.0 to 26.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (229.0 to 230.0) V

Date of Received : 19 April 2023

Date of Calibration : 19 April 2023

Date of Issue : 22 April 2023

Calibrated by : Bunjerd Masri

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400023 66-400184-1

03 Oct 2023

National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400195-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

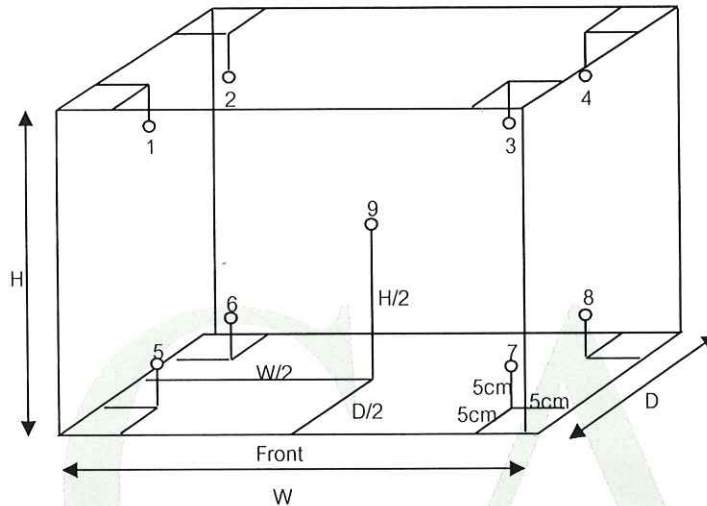

Inside of Chamber

W = 0.56 m

D = 0.40 m

H = 0.48 m

Capacity = 0.11 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	105.5	105.5	105.2	105.4	105.1	105.3	101.9	103.9	100.6	103.5	103.3	1.0

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	105.5	105.5	3.0	0.3	5.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-400196-1

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46, Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : Air Chamber (Incubator)

Manufacturer : Lovibond

Model : ET636-6

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 9982523-03

ID No. : 011

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (24.0 to 25.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (229.0 to 230.0) V

Date of Received : 19 April 2023

Date of Calibration : 19 April 2023

Date of Issue : 22 April 2023

Calibrated by : Bunjerd Masri

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400047	66-400066-2	03 Aug 2023	National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400196-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

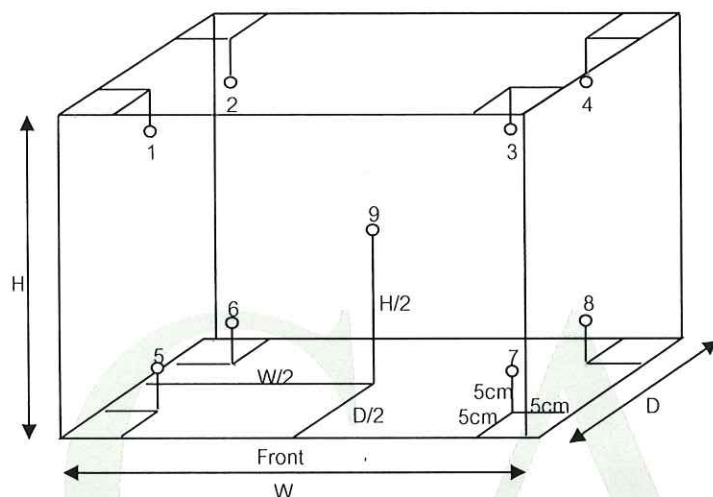

Inside of Chamber

W = 0.53 m

D = 0.43 m

H = 1.40 m

Capacity = 0.32 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	21.0	21.0	20.12	20.18	20.29	20.29	20.16	20.03	19.93	19.87	20.01	0.42

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	21.0	21.0	0.32	0.19	0.6

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



www.calibratech.co.th



Certificate of Calibration

Certificate No.: WK2304-173-14

Page 1 of 2

Customer : HVE COMPANY LIMITED
603 Soi Charansanitwong 46 Charansanitwong Road,
Bang Phlat, Bangkok 10700

Instrument	: pH Meter	Ambient Temperature	: (25 ± 2) °C
Manufacturer	: HANNA	Humidity	: (50 ± 15) %RH
Model	: HI 221	Received Date	: 26-Apr-23
Serial No.	: 08376721	Calibrated Date	: 2-May-23
Identity No.	: N/A	Issued Date	: 3-May-23
Range	: See to Data	Calibrated Location	: In Lab
Resolution	: See to Data		
Calibration Method	: CP-WK-C01 and CP-WK-T06		

Reference standard instruments :

<u>Instrument</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>	<u>Traceability to</u>
pH Buffer # 4	PH216.L5	880819	13-Mar-24	CPAchem Ltd.
pH Buffer # 7	PH107.L5	880818	13-Mar-24	CPAchem Ltd.
pH Buffer # 10	PH220.L5	880822	13-Mar-24	CPAchem Ltd.
Digital Thermometer	382081948	WK2210-140-5	24-Oct-23	WK Electric Co.,Ltd.
Temperature Indicator with PRT Standard	4507	PSL-T 0292/65	11-Feb-24	TISTR

TISTR : Thailand Institute of Scientific and Technological Research.

This result calibrate was found accurate as shown on date place of calibrate only

This certificate is traceability to the International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence approximately 95%

Calibrated by : Ms. Usa Phuangphiphat

Approved by :

Ms. Budsagorn Patcha

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Calibration Results

Certificate No.: WK2304-173-14

Page 2 of 2

Calibration Result of the Accuracy

Function : pH Measurement

Range : 4 pH to 10 pH

Resolution : 0.01 pH

Unit : pH

STD Solution	UUC Reading	Error	Uncertainty (± pH)
4.00	4.02	0.02	0.0080
7.00	7.02	0.02	0.010
10.00	9.98	-0.02	0.010

Function : Temperature Measurement

Range : 25 °C

Resolution : 0.1 °C

Unit : °C

Temperature Setting	STD Reading	UUC Reading	Error	Uncertainty (± °C)
25	25.069	25.2	0.131	0.032

(X) Without Adjustment () After Adjustment

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

**** End of Certificate****



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 23TW93

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	Digicon
Model :	DO-552SD
Serial No. :	AG.35318
ID No. :	-
Received Date :	31 March 2023
Test Date :	03 April 2023
Reference :	2303-1117DN-1
Submitted by :	HVE Co.,Ltd 603 Soi Jarransanitwong 46, Jarransanitwong Road, Bang Yi Khan, Bang Phlat, Bangkok 10700
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 Approved Signatory
(<input checked="" type="checkbox"/>) Malee Butkruea	
(<input type="checkbox"/>) Saithip Meangmai	
(<input type="checkbox"/>) Warakorn Lerngagtrakul	
Issue Date :	5 April 2023

B 0311635



Cert.No.: 23TW93

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 07-07

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.16	8.0	0.055

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu.

a 1156571



บริษัท กิตติสิทธ์ เอ็นเตอร์ไพรส์ จำกัด (สำนักงานใหญ่)

KITTISIT ENTERPRISE CO.,LTD

38/76, 38/77 หมู่ 3 ตำบลคูคต อำเภอลำลูกกา จังหวัดปทุมธานี 12130

โทร : 02-991-0963 แฟกซ์ : 02-991-0986 มือถือ : 089-455-1486

E-mail sale@ktssci.com ,www.ktssci.com



CERTIFICATE OF CALIBRATION

Certificate No : 22-072

Page : 1 of 5

Customer : HVE CO ., LTD .
Address : 603 Soi Jarunsanitwong 46 , Jarunsanitwong Road , Bangyeekun
Bangplad , Bangkok 10700
Instrument : UV/Vis Spectrophotometer
Manufacturer : Thermo Scientific
Model : G10S UV-VIS
Serial Number : 2L9Q310003
Environment : Temperature (Before 26.7 °C , After 27.0 °C)
: Humidity (Before 55.6 %RH , After 56.7 %RH)
Received Date : 2/11/2022
Calibration Date : 8/11/2022
Issue Date : 10/11/2022
Calibration Status : No Adjustment
Calibration Area : Onsite Laboratory Room

Calibrated By : Apichit Puttachart
(Mr. Apichit Puttachart)

Approved By : [Signature]
(Mr. Puttipong Busayakitisit)

F-2401-01/26-07-60

Certificate No : 22-072

Page : 2 of 5

1. Wavelength Accuracy

Spectral slit width: 2.00 nm

1.1 CRMs : Holmium Glass Filter

Traceability : Traceable to the International System of Unit through Starna Certificat 94650

Filter STDs(nm) Certificate	Average Measuring Value(nm)	Correction (nm)	Uncertainty ±(nm)
241.74	241.40	0.34	0.12
279.44	279.30	0.14	0.12
287.98	287.89	0.09	0.13
334.10	334.10	0.00	0.12
361.00	360.80	0.20	0.12
418.61	418.60	0.01	0.12
453.63	453.60	0.03	0.12
460.05	460.00	0.05	0.12
536.66	536.80	-0.14	0.12
637.98	638.56	-0.58	0.14

1.2 CRMs : Didymium Glass Filter

Traceability : Traceable to the International System of Unit through Starna Certificat 94647

Filter STDs(nm) Certificate	Average Measuring Value(nm)	Correction (nm)	Uncertainty ±(nm)
585.29	585.70	-0.41	0.12
684.49	685.10	-0.61	0.12
740.18	741.00	-0.82	0.12
748.48	749.20	-0.72	0.12
807.03	807.80	-0.77	0.12

F-2401-01/26-07-60

2. Photometric Accuracy

Certificate No : 22-072

CRMs : Neutral Density Glass Filters

Page : 3 of 5

Traceability: Traceable to the International System of Unit through Starna Certificate 94683

Spectral slit width: 2.00 nm

2.1 Reading scale at 420.0 nm. (* Not Accredited)

Filter STDs (Abs.) Certificate	Average Measuring Value (A)	Correction (A)	Uncertainty ±(A)
0.0000	0.0000	0.0000	0.0028
0.5732	0.5720	0.0012	0.0056
0.7135	0.7130	0.0005	0.0050
1.0269	1.0280	-0.0011	0.0034

2.2 Reading scale at 440.0 nm.

Filter STDs (Abs.) Certificate	Average Measuring Value (A)	Correction (A)	Uncertainty ±(A)
0.0000	0.0000	0.0000	0.0028
0.5582	0.5570	0.0012	0.0056
0.7019	0.7010	0.0009	0.0050
1.0099	1.0100	-0.0001	0.0034

2.3 Reading scale at 465.0 nm.

Filter STDs (Abs.) Certificate	Average Measuring Value (A)	Correction (A)	Uncertainty ±(A)
0.0000	0.0000	0.0000	0.0028
0.5209	0.5190	0.0019	0.0053
0.6631	0.6620	0.0011	0.0049
0.9531	0.9530	0.0001	0.0032

Certificate No : 22-072

Page : 4 of 5

2.4 Reading scale at 546.1 nm.

Filter STDs (Abs.) Certificate	Average Measuring Value (A)	Correction (A)	Uncertainty ±(A)
0.0000	0.0000	0.0000	0.0028
0.5224	0.5200	0.0024	0.0043
0.6997	0.6970	0.0027	0.0041
1.0066	1.0040	0.0026	0.0028

2.5 Reading scale at 590.0 nm.

Filter STDs (Abs.) Certificate	Average Measuring Value (A)	Correction (A)	Uncertainty ±(A)
0.0000	0.0000	0.0000	0.0028
0.5564	0.5530	0.0034	0.0038
0.7750	0.7710	0.0040	0.0037
1.1171	1.1130	0.0041	0.0029

2.6 Reading scale at 635.0 nm.

Filter STDs (Abs.) Certificate	Average Measuring Value (A)	Correction (A)	Uncertainty ±(A)
0.0000	0.0000	0.0000	0.0028
0.5638	0.5610	0.0028	0.0035
0.7644	0.7610	0.0034	0.0035
1.1014	1.0990	0.0024	0.0029

Certificate No : 22-072

Page : 5 of 5

3. Photometric Accuracy

CRMs : Potassium Dichromate 60 mg/l CRMs Serial Number : 35553

Blank Serial Number : 105079

Traceability : Traceable to NIST through Starna Certificate

94662

Spectral slit width : 2.00 nm

	Certificate (Abs.)	Average Measuring Value (A)	Correct (A)	Uncertainty ±(A)
Blank	0.0000	0.0000	0.0000	0.0049
235 nm	0.7454	0.7413	0.0041	0.0062
Blank	0.0000	0.0000	0.0000	0.0049
257 nm	0.8651	0.8590	0.0061	0.0058
Blank	0.0000	0.0000	0.0000	0.0049
313 nm	0.2895	0.2900	-0.0005	0.0052
Blank	0.0000	0.0000	0.0000	0.0049
350 nm	0.6415	0.6370	0.0045	0.0052

4. Stray Light (*Not Accredited)

CRMs : Potassium Iodide aqueous solution

CRM Serial Number : 35557

Traceability : Traceable to NIST through Starna Certificate

94670

Spectral slit width: 2.00 nm

Wavelength (nm)	Certificate	Average Measuring
260.3	>2A	2.3741
260.3	<1%T	0.42

Note

1. Calibration Method

1.1 Wavelength Accuracy : Measuring Wavelength by CRMs base on ASTM E925/ASTM E275-08

1.2 Photometric Accuracy : Measuring Absorbance by CRMs based on ASTM E925/ASTM E275-08

1.3 Stray light : Measuring Absorbance and Transmittance by CRMs base on ASTM E387

2. Uncertainty of Measurement : The report uncertainty of measurement was based on standand uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%

3. This result of calibration was found accurate as show on date and place of calibration only.

4. This certificate was certificate only for the our calibrated instrument.

F-2401-01/26-07-60