

---

## เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์

Certificate No.: MC 2307702

Page 2 of 3

**The Reference Standard Instrument :**

| Description                                     | Certificate No. | Serial No. | Due date   | Traceable thru |
|---|-----------------|------------|------------|----------------|
| Data Acquisition/Switch Unit                    | MC 2303173      | MY41010916 | 9 Mar 2024 | MCAL           |
| With Thermocouple Type " T " ID. No.171 to 1719 |                 |            |            |                |

**Traceability :**

The measurement standard traceable to the international system of units (SI) through certificate as mentioned above

**1. Calibration Procedure:**

This Instrument was calibration according to TLAS G-20 by comparison with calibrated thermocouple type T under no load condition. The Thermocouples were placed on nine points and located one thermocouple in each of the eight corners of the chamber and was away from the each wall of 5 cm to 10 cm. And placed the ninth thermocouple within 2.5 cm of the geometric center of the chamber.

**Temperature Uniformity** - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.

**Temperature Stability** - one-half of the greatest maximum difference of measured temperatures at any one sensor.

**Overall Variation** - The Difference of the maximum and minimum measured temperatures throughout observation.

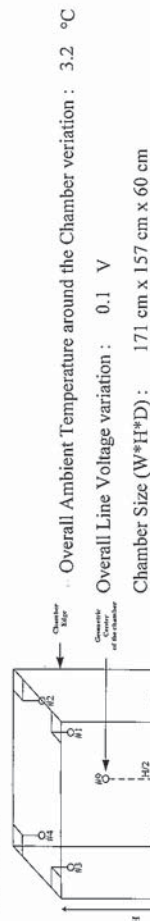


Figure 1 : Sensor Installation Location

Checked by : *Thanagorn*

[MCF-Q-077 ; Rev.6 ; Date : 22/04/2021]

# Certificate of Calibration

## TEMPERATURE CONTROLLER ENCLOSURES



Certificate No.: MC 2307702

Page 1 of 3



|                          |   |               |                |
|--------------------------|---|---------------|----------------|
| Customer                 | : Water Analysis Center Co., Ltd.   | Received Date | : 11 July 2023 |
| Reference Job No.        | : 23-1577   |               |                |
| Description              | : Refrigerator  |               |                |
| Manufacturer             | : SANDEN INTERCOOL  | Model         | : SEC-1500SBD  |
| Serial No.               | : SEC1500201A-0708-00304  | ID. No.       | : WWL0038      |
| Marking                  | : Additionally for the purpose of identification by this laboratory a label marked with this certificate number ( MC 2307702 ) has been attached to the case. |               |                |
| Method                   | : In-House calibration procedure MWI-T-033 this method is reference to TLAS G-20 "Temperature Controlled Enclosures".   |               |                |
| Location of Calibration  | : Water Analysis Center Co., Ltd. ; Laboratory.   |               |                |
| Environmental Conditions | : Ambient Temperature : ( 25.3 to 25.9 ) °C   |               |                |
|                          | Relative Humidity : ( 65.2 to 67.9 ) %  |               |                |
| Date of Calibration      | : 11 July 2023  | Date of Issue | : 12 July 2023 |

Checked by : *Thanagorn* Approved by : *Aittipong*  
Thanagorn Limchaicharoen Aittipong Kanjanawasit  
( Calibration Supervisor ) ( Technical Manager )

**The uncertainties are for a confidence probability of approximately 95%**

This certificate is issued in accordance with the conditions of accreditation granted by the National Standardization Council of Thailand-Office of the National Standardization Council that has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of Master Calibration Co., Ltd.

[MCF-Q-077 ; Rev.6 ; Date : 22/04/2021]

Certificate No.: MC 2307702

Page 3 of 3

## 2. Result of calibration :

### Temperature Measurement Accuracy Test

| Indicating Temperature (°C) | Measured Temperature (°C) at Spread Locations |     |     |     |     |     |     |     |         | Uncertainty (±°C) |
|-----------------------------|---|-----|-----|-----|-----|-----|-----|-----|---------|-------------------|
|                             | #1  | #2  | #3  | #4  | #5  | #6  | #7  | #8  | Ref. #9 |                   |
| 2.5                         | 4.4   | 4.2 | 4.2 | 4.2 | 4.0 | 3.9 | 4.1 | 4.0 | 3.8     | 0.86              |

### Chamber Characterization Result

| Controller Temperature (°C) | Indicating Temperature (°C) | Temperature Stability (±°C) | Temperature Uniformity (°C) | Overall Variation (°C) |
|-----------------------------|-----------------------------|-----------------------------|-----------------------------|------------------------|
| 2.0                         | 2.5                         | 1.50                        | 1.01                        | 3.3                    |

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

This certificate will certify of the calibrated equipment only.

End of Certificate

Checked by : *Thanngin*

[MCF-Q-077 ; Rev.6 ; Date : 22/04/2021]



THAI HEART CALIBRATION CO., LTD.  
102/11 Moo 5, Phraek Sai, Bangna Suburb, Bangkok 10700  
Tel. 0-2394-9109, 0-2394-9108, 0-2394-9107, 0-2394-9106  
Fax 0-2394-9105, 0-2394-9104, 0-2394-9103, 0-2394-9102



# CERTIFICATE OF CALIBRATION

Certificate No.: C0-1907007/23 Page 1 of total 2 pages

**Customer**  
WATER ANALYSIS CENTER CO., LTD.  
1/94 Moo 5, T.Kanham,  
A.U-thai, Ayutthaya 13210

**Equipment** Conductivity Meter  
**Manufacturer** EUTECH  
**Serial No.** 2657889  
**Description** -  
**Model** CON 2700  
**ID No.** WWL 0136

**Environmental Conditions**  
Ambient Temperature: (20 ± 2) °C  
Relative Humidity: (50 ± 10) %  
Atmospheric Pressure: -

**Calibration Location** Jayhawks Laboratory (CL&GL)  
**Received Date** 19 July 2023  
**Calibration Date** 19 July 2023  
**Date of Issue** 20 July 2023  
**Condition of Artifacts** Used conditions but can be calibrated

Checked by *[Signature]* Approved by *[Signature]*  
Act as Technical Manager Representative of Managing Director

( ) (Krisyosl K.) ( ) (Sakda Y.)  
( ) (Patiphan K.) (✓) (Onnapa P.)  
( ) (Pongsak H.) ( ) (Nitiphong K.)  
( ) (Kanung C.) ( ) (Nonthachai K.)  
( ) (Pramong P.) ( ) (Noppol P.)  
( ) (Dr. Ekachai Puttitwong)

This calibration certificate shall not be reproduced other than in full except with the prior written approval of the Thai Heart Calibration Co., Ltd.

FE-169

REV.02 02/24/21





Certificate No.: C0-1808005/23

Page 2 of total 4 pages

Reference Method:

- The calibration method used was CP-178 based on an in-house method.
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard:

| Type                 | pH Value | Lot No. | Due Date     | Traceability |
|----------------------|----------|---------|--------------|--------------|
| pH Standard Solution | 4.01     | 030822  | Feb. 9, 2024 | NIMT         |
|                      | 7.01     | 300522  | Feb. 9, 2024 |              |
|                      | 10.01    | 230822  | Feb. 7, 2024 |              |

ภาคผนวก ซ-4

| Type                            | Model       | Serial No.            | Certificate No. | Due Date      | Traceability |
|---------------------------------|-------------|-----------------------|-----------------|---------------|--------------|
| Documenting Process Calibrator  | 754         | 2630521               | 10-2412001/22   | Dec. 23, 2023 | THC          |
| Digital Thermometer with Sensor | 1523 / 5622 | 1709138 / 4605984-005 | 10-0806001/23   | Jun. 8, 2024  |              |

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- NIMT, National Institute of Metrology (Thailand).
- THC, Thai Heart Calibration Co., Ltd.

Measurement Results:

1. Function Simulated pH Meter

| Standard Applied<br>(mV) | Nominal Value<br>(pH) | UUC Reading |        | Uncertainty<br>(± mV) |
|--------------------------|-----------------------|-------------|--------|-----------------------|
|                          |                       | pH          | mV     |                       |
| 177.48                   | 4.00                  | 4.01        | 177.4  | 0.060                 |
| 0.00                     | 7.00                  | 7.00        | 0.0    | 0.060                 |
| -177.48                  | 10.00                 | 10.01       | -177.4 | 0.060                 |

UUC : Unit Under Calibration

Note : Adjust Curve to simulate pH (4,7,10)

Certificate No.: C0-1808005/23

Page 3 of total 4 pages

Measurement Results (Cont.):

2. Calibration of pH Electrode (Serial No.: 3222623)

| pH Standard Solution<br>(pH) | Measured Value |        | Uncertainty<br>(± pH) |
|------------------------------|----------------|--------|-----------------------|
|                              | (pH)           | (mV)   |                       |
| 4.01                         | 4.01           | 180.0  | 0.013                 |
| 7.01                         | 7.00           | 4.0    | 0.013                 |
| 10.01                        | 10.01          | -172.0 | 0.013                 |

Note : Adjust Curve to Buffer Solution pH (4,7,10)  
Temperature stability of micro bath :  $25 \pm 0.2^{\circ}\text{C}$

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.



THAI HEART CALIBRATION CO., LTD.  
112/11 Moo 5, Phadessa - Mueang Samut Prakan 10380  
Tel. 02-919-2162, 02-919-8356, 02-919-8396 Fax. 02-919-8807



Automation

AUTOMATION SERVICE CO., LTD.  
CALIBRATION LABORATORY

Cert. No. WAC-065  
Page 1 of 2

SV 201003/2023

Certificate No.: C0-1808005/23

Page 4 of total 4 pages

#### Reference Method:

- The calibration method used was CP-096 based on an in-house method.
- The temperature scale used was an ITS-90.
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

#### Reference Standard Instruments:

| Type                            | Model     | Serial No. | Cert. No.     | Due Date      | Traceability |
|---------------------------------|-----------|------------|---------------|---------------|--------------|
| Thermometer Readout             | 1529-R    | B7C853     | 10-0911001/22 | Nov. 9, 2023  | THC          |
| Platinum Resistance Thermometer | 5626      | 4854       | COA30047      | Oct. 22, 2023 | FLUKE        |
| Liquid Bath                     | XORTS-40A | XO111019   | 10-2405001/23 | May 25, 2025  | THC          |

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- THC, Thai Heart Calibration Co., Ltd.
- FLUKE, Fluke Corporation, U.S.A.

#### Measurement Results:

(X) Without Adjustment

Dimension of probe : Diameter 4 mm. Sensor Type : RTD (PT100)

| Immersion Depth (mm.) | Standard Reading (°C) | UUC Reading (°C) | Correction (°C) | Uncertainty (± °C) |
|-----------------------|-----------------------|------------------|-----------------|--------------------|
| 120                   | 22.00                 | 22.2             | -0.20           | 0.065              |
| 120                   | 25.00                 | 25.2             | -0.20           | 0.065              |
| 120                   | 28.00                 | 28.2             | -0.20           | 0.065              |

UUC : Unit Under Calibration

The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -

Calibrated by Pongsak  
REV.02 02/24/21

FE-169

## CERTIFICATE OF CALIBRATION

Instrument : DO Meter  
Model : DO-31P  
Serial No. : 780065  
Manufacturer : TOA-DKK  
Measuring Range : 0.00 ~ 20.00 mg/l

Machine : -  
Location : -

Customer : Water Analysis Center Co., Ltd.  
1/94 Moo.5 T.Kanham, A.U.-Thai  
Ayutthaya 13210 Thailand

Date Of Received : 05 / 01 / 2023  
Date Of Calibration : 05 / 01 / 2023

Ambient Condition : Temperature 25 °C  
Humidity 50 % RH

Calibrated By :

P. Yooyen  
(Ms. Phanee Yooyen)  
Technician

Approved By :

Pongit (for)  
(Mr. Nipon Phungsomsak)  
Technical Manager

Date Of Issue : 09 / 01 / 2023

This Certificate may not be reproduced other than in full, except with the prior written approval of the head of the industrial instruments calibration center.





# AUTOMATION SERVICE CO.,LTD.

## CALIBRATION LABORATORY

Instrument : DO Meter  
Model : DO-31P  
Serial No. : 780065

Cert. No. WAC-065  
Page 2 of 2

### Calibrate Procedure

- ☐ This instrument was calibrated by comparison with standard solution (PH/ORP)
- ☐ This instrument was calibrated by comparison with scattering plate value (Turbidity)
- ☒ This instrument was calibrated by comparison with conductivity (Conductivity)
- ☒ This instrument was calibrated by comparison with Sodium sulfite anhydrous (DO)

### Condition of this result of calibration

- 1). Reference Standard Solution

| Standard             | Lot No       | Batch     | Cert. No. | Due Date    |
|----------------------|--------------|-----------|-----------|-------------|
| Sodium Sulfite Power | 1.06657.0500 | K54224057 | -         | 30 Sep 2023 |

- 2). Traceability This certification is traceable to
  - ☒ Merck KGaA 64271 Darmstadt
  - ☐ DKK Corporation

### Result Of Calibration

| Standard Solution |      | Before Adjust |        | After Adjust |       |
|-------------------|------|---------------|--------|--------------|-------|
| (mg/l) at 24.1°C  |      | Indicator     | Error  | Indicator    | Error |
| Zero              | 0.00 | 0.05          | + 0.05 | 0.00         | -     |
| Span              | 8.25 | 7.13          | - 1.12 | 8.25         | -     |

DO Electrode No. OE270AA(5) S/N 111F0029

Calibrated By P. Yooyen  
(Ms. Phancee Yooyen )  
Technician



**Master Calibration Co.,Ltd.**  
547 Soi Ratchadaniwot, Kwaeng Samsenok, Khet Huaykwang, Bangkok 10310  
Tel : (02) 274 2978-9, (02) 2742987-8 Fax : (02) 274 2518, (02) 274 2989  
Website : www.mastercalibration.com E-mail : calibrate@mastercalibration.com

## Certificate of Calibration

TEMPERATURE  
CONTROLLER ENCLOSURES



Certificate No.: MC 2303684

Page 1 of 3



Customer : Water Analysis Center Co., Ltd.  
1/94 Moo 5, T.Kantiam, A.U-Thai, Ayuthaya 13210.

Reference Job No. : 23-0729 Received Date : 23 March 2023  
Description : Oven  
Manufacturer : Memmert Model : UF260  
Serial No. : B620.0814 ID. No. : WWL0212  
Marking : Additionally for the purpose of identification by this laboratory a label marked

with this certificate number ( MC 2303684 ) has been attached to the case.

Method : In-House calibration procedure MWI-T-033 this method is reference to

TLAS G-20 "Temperature Controlled Enclosures".

Location of Calibration : Water Analysis Center Co., Ltd. ; Laboratory.

Environmental Conditions : Ambient Temperature : ( 27.1 to 29.3 ) °C

Relative Humidity : ( 38.0 to 72.2 ) %

Date of Calibration : 23 March 2023 Date of Issue : 24 March 2023

Checked by : Thungorn Approved by : Aittipong  
Thanagorn Limchaicharoen Aittipong Kaljanawasit  
( Calibration Supervisor ) ( Technical Manager )

The uncertainties are for a confidence probability of approximately 95%

This certificate is issued in accordance with the conditions of accreditation granted by the National Standardization Council of Thailand-Office of the National Standardization Council that has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the

Certificate No.: MC 2303684

Page 2 of 3

## The Reference Standard :

| Description                                      | Certificate No. | Serial No. | Due date     |
|--|-----------------|------------|--------------|
| Data Acquisition/Switch Unit                     | MC 2303173      | MY41010916 | 9 March 2024 |
| With Thermocouple Type " T " ID. No.17/1 to 17/9 |                 |            |              |

This certificate is traceable to the international system of units maintained at:

- Master Calibration Co., Ltd.


## 1. Calibration Procedure:

This Instrument was calibration according to TLAS G-20 by comparison with calibrated thermocouple type T under no load condition. The Thermocouples were placed on nine points and located one thermocouple in each of the eight corners of the chamber and was away from the each wall of 5 cm to 10 cm. And placed the ninth thermocouple within 2.5 cm of the geometric center of the chamber.

**Temperature Uniformity** - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.

**Temperature Stability** - one-half of the greatest maximum difference of measured temperatures at any one sensor.

**Overall Variation** - The Difference of the maximum and minimum measured temperatures throughout observation.

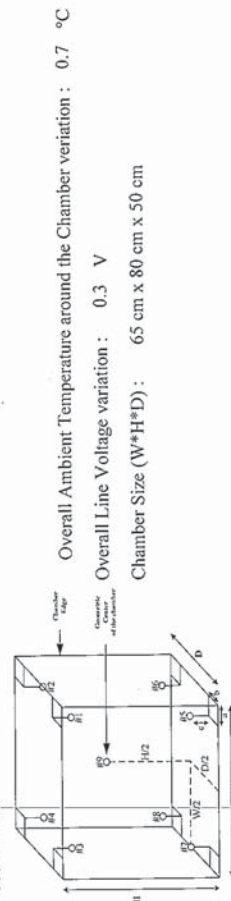

Overall Ambient Temperature around the Chamber variation : 0.7 °C  
Overall Line Voltage variation : 0.3 V  
Chamber Size (W\*H\*D) : 65 cm x 80 cm x 50 cm

Figure 1.1 Sensor Installation Location

Certificate No.: MC 2303684

Page 3 of 3

## 2. Result of calibration :

### Temperature Measurement Accuracy Test

| Indicating Temperature (°C) | Measured Temperature (°C) at Spread Locations |       |       |       |       |       |       |       |         | Uncertainty (±°C) |
|-----------------------------|---|-------|-------|-------|-------|-------|-------|-------|---------|-------------------|
|                             | #1  | #2    | #3    | #4    | #5    | #6    | #7    | #8    | Ref. #9 |                   |
| 104                         | 103.7   | 103.9 | 103.6 | 103.8 | 103.7 | 104.2 | 104.1 | 104.2 | 104.3   | 0.58              |
| 180                         | 179.4   | 179.8 | 179.4 | 179.7 | 179.4 | 179.9 | 179.8 | 180.2 | 180.0   | 1.3               |

### Chamber Characterization Result

| Controller Temperature (°C) | Indicating Temperature (°C) | Temperature Stability (±°C) | Temperature Uniformity (°C) | Overall Variation (°C) |
|-----------------------------|-----------------------------|-----------------------------|-----------------------------|------------------------|
| 104                         | 104                         | 0.32                        | 0.84                        | 1.2                    |
| 180                         | 180                         | 0.4                         | 0.9                         | 1.3                    |

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

This report will certify of the calibrated equipment only.

End of Certificate





## Certificate of Calibration

**Equipment:** Balance  
**Model:** BL 210S  
**Serial No. (or ID.):** 15808131 (WWL 0022)  
**Manufacturer:** Sartorius  
**Condition:** In condition

**Certificate No.:** C01223710  
**Issued Date:** 07 December 2022  
**Job No.:** KSPR2215481  
**Page:** 1 of 2

**Customer:** Water Analysis Center Co., Ltd.  
1/94 Moo 5, Rojana Industrial Park, Rojana Road,  
Tambol Kanham, Amphur U-Thai, Ayutthaya 13210 Thailand

**Environment Condition:** Temperature 25 °C ± 0.9 °C  
Humidity 48 %RH ± 4.9 %RH

**Calibration Place:** Water Analysis Center Co., Ltd. (แหล่งเครื่องจักร)  
1/94 Moo 5, Rojana Industrial Park, Rojana Road,  
Tambol Kanham, Amphur U-Thai, Ayutthaya 13210 Thailand

**Calibration By:** Mr. Pradit Siriboot  
**Calibration Date:** 07 December 2022  
**The Method used:** In-house method, CAL-WI-47, based on UKAS Lab 14  
**Traceability:** This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02221864

(Mr. Pradit Siriboot)  
Person in charge

(Mr. Rungrod Jenkitrakulchai)  
Authorized signatory

This certificate is issued for the units of measurement according to the International System of Units (SI). It provides traceability of measurement to International or national standard or other recognized national standard laboratories.  
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).  
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 หมู่ 5 ถนน อโยธยา-สุพรรณบุรี กิโลเมตรที่ 12860




Certificate No.: C01223710

Page: 2 of 2

### Calibration Results:

#### Without Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

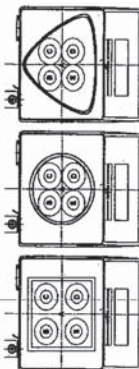

| Nominal Test Value |  |  |  |  | Reference Points (g) |        |        |
|--------------------|--|--|--|--|----------------------|--------|--------|
|                    |  |  |  |  | A                    | B      | C      |
|                    |  |  |  |  | -                    | 0.0001 | 0.0001 |
|                    |  |  |  |  | D                    |        |        |
|                    |  |  |  |  | E                    |        |        |
|                    |  |  |  |  | -0.0002              |        |        |
|                    |  |  |  |  | -0.0001              |        |        |

Repeatability: Determination of the standard deviation of weighing balance., Readability

0.0001 (g)

| Nominal test value (g) | Standard Deviation |
|------------------------|--------------------|
| 20                     | 0.00007            |
| 200                    | 0.00007            |

Error of Indication from nominal or conventional mass value., Readability

0.0001 (g)

| Nominal Value (g) | Conventional Mass (g) | Displayed Value (g) | Error of Indication (g) | Uncertainty (g) | k    |
|-------------------|-----------------------|---------------------|-------------------------|-----------------|------|
| 1                 | 1.00001               | 1.0000              | 0.0000                  | 0.00012         | 2.08 |
| 2                 | 2.00001               | 2.0000              | 0.0000                  | 0.00012         | 2.08 |
| 5                 | 5.00003               | 5.0000              | 0.0000                  | 0.00012         | 2.07 |
| 10                | 10.00002              | 10.0000             | 0.0000                  | 0.00013         | 2.07 |
| 20                | 20.00001              | 20.0000             | 0.0000                  | 0.00013         | 2.06 |
| 50                | 50.00003              | 50.0000             | 0.0000                  | 0.00014         | 2.04 |
| 70                | 70.00004              | 70.0001             | 0.0001                  | 0.00017         | 2.02 |
| 100               | 100.00002             | 100.0001            | 0.0001                  | 0.00018         | 2.01 |
| 120               | 120.00003             | 120.0001            | 0.0001                  | 0.00022         | 2.01 |
| 150               | 150.00005             | 150.0003            | 0.0003                  | 0.00024         | 2.00 |
| 200               | 200.00006             | 200.0004            | 0.0003                  | 0.00030         | 2.00 |

The End of Certificate

บริษัท ดีเคเอส เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 หมู่ 5 ถนน อโยธยา-สุพรรณบุรี กิโลเมตรที่ 12860