

ภาคผนวกที่ 4

ใบรับรองการสอบเทียบเครื่องมือ



บริษัท เอ็ม อี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ.นนทบุรี 11110

36/659 Moo 6 Tambol Bangrakpattana Amphur Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	November 14, 2023
Project Site				Start Time	9:35 AM
Sampler Number	TSP No.5	Transfer Standard Type	Orifice	Stop Time	9:40 AM
Motor Serial Number	BL-05	Calibrator Model	TE-5025A	Person	
Recorder Serial Number	-	Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_{2O}(Pa/P_{std})(T_{std}/Ta)]^{1/2}$		Qstd = (1/m)[(A-b)]	IC = I[(Pa/P _{std})(T _{std} /Ta)] ^{1/2}	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O		(m ³ /min)	(inch)					
5	1.7	1.7	3.4	1.81903	0.93616	1.0	0.99	305.0	757.0		
7	2.2	2.2	4.4	2.06931	1.06696	1.6	1.58	305.0	757.0		
10	4.0	4.1	8.1	2.80764	1.45283	2.5	2.47	305.0	757.0		
13	5.2	5.2	10.4	3.18138	1.64815	3.4	3.35	305.0	757.0		
18	6.4	6.4	12.8	3.52943	1.83004	4.0	3.95	305.0	757.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	1.91345	Linear Equation		Average	305.0	757.0	
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.994156	Pstd(mmHg)	760.0
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	r	0.9970737	T _{NTP}	298.0
Result							C=(Pa/Pstd)*(Tstd/Ta)	0.973192407
							C=(Pa/Pstd)*(Tstd/Ta) ^{0.5}	0.986505148

COMMENT

Andersen Instruments, Inc.

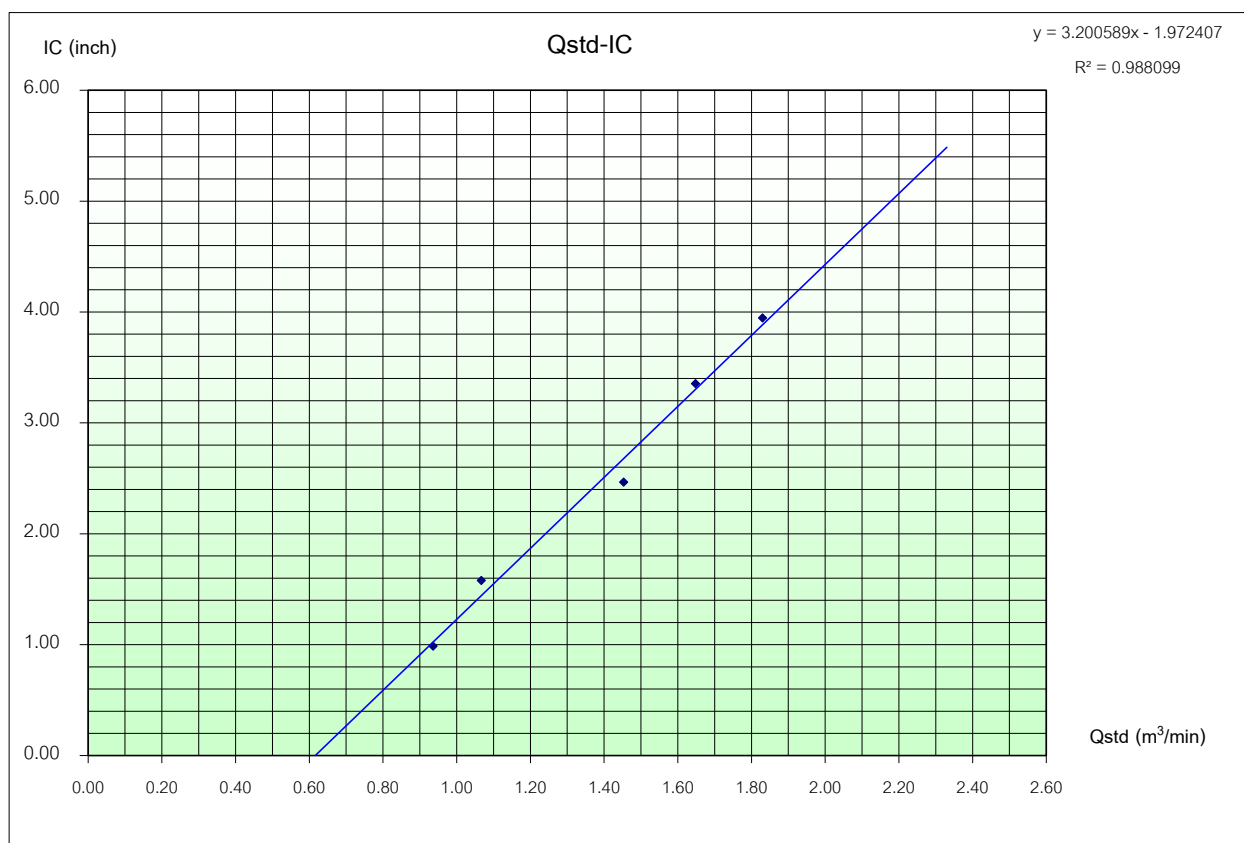

Calibrated By

(Mr.Preecha Srisuk)
Field Environmental

Approved By

(Mr.Jarung Jamnongbut)
Division Manager



บริษัท เอ็ม ซี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ.นนทบุรี 11110

36/659 Moo 6 Tambol Bangrakpattana Amphur Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	November 14, 2023
Project Site				Start Time	9:05 AM
Sampler Number	TSP No.2	Transfer Standard Type	Orifice	Stop Time	9:10 AM
Motor Serial Number	BL-02	Calibrator Model	TE-5025A	Person	
Recorder Serial Number	-	Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric	Start	Stop
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication (inch)	$IC = I[(Pa/P_{std})(T_{std}/T_a)]^{1/2}$	(*K = °C+273)	Pressure (mmHg)	Meter	Meter
	Positive	Negative	ΔH ₂ O								
5	1.7	1.7	3.4	1.81903	0.93616	1.6	1.58	305.0	757.0		
7	2.8	2.8	5.6	2.33450	1.20555	2.5	2.47	305.0	757.0		
10	4.2	4.3	8.5	2.87613	1.48862	4.0	3.95	305.0	757.0		
13	5.4	5.4	10.8	3.24199	1.67982	5.1	5.03	305.0	757.0		
18	6.6	6.7	13.3	3.59770	1.86573	6.2	6.12	305.0	757.0		

Linear Regression Y ON X : Y= mX + b

1	Slope (m)	1.91345	Linear Equation		Average	305.0	757.0		
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)	1.133	r ²	0.971641	Pstd(mmHg)	760.0	
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)	0	r	0.9857185	T _{NTP}	298.0	
Result						(Pa/Pstd)*(Tstd/Ta)		0.973192407	
						C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.986505148	

COMMENT

Andersen Instruments, Inc.

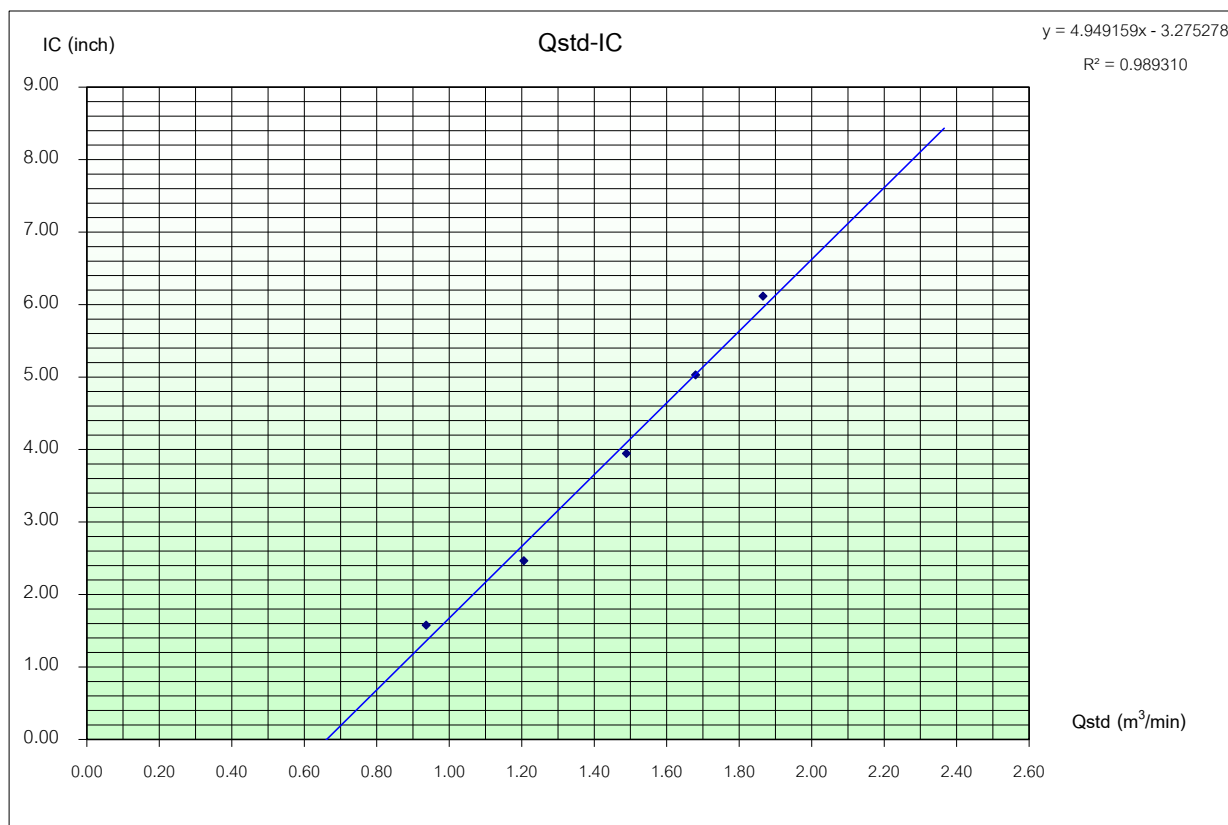

Calibrated By

(Mr.Preecha Srisuk)
Field Environmental

Approved By

(Mr.Jarung Jamnongbut)
Division Manager



บริษัท เอ็ม ซี ที จำกัด MET CO.,LTD.

36/659 หมู่ 6 ต.บางรักพัฒนา อ.บางบัวทอง จ. นนทบุรี 11110

36/659 Moo 6 Tambol Bangrakpattana Amphur Bangbuatong Nontaburi 11110

Tel : 0 2920 1458-9 Fax : 0 2920 1460 E-mail : met_jj@yahoo.com

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	November 14, 2023
Project Site				Start Time	9:25 AM
Sampler Number	TSP No.4	Transfer Standard Type	Orifice	Stop Time	9:30 AM
Motor Serial Number	BL-04	Calibrator Model	TE-5025A	Person	
Recorder Serial Number	-	Calibrator Serial Number	1		


Plate No.	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric Pressure	Start Meter	Stop Meter
	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication (inch)	$IC = [(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	(°K = °C+273)	(mmHg)		
	Positive	Negative	ΔH ₂ O								
5	1.5	1.5	3.0	1.70868	0.87849	1.1	1.09	305.0	757.0		
7	1.7	1.7	3.4	1.81903	0.93616	1.6	1.58	305.0	757.0		
10	2.7	2.7	5.4	2.29243	1.18357	2.5	2.47	305.0	757.0		
13	5.5	5.5	11.0	3.27187	1.69544	3.2	3.16	305.0	757.0		
18	5.9	6.0	11.9	3.40309	1.76402	4.0	3.95	305.0	757.0		

Linear Regression Y ON X : Y= mX + b

			Average								
1	Slope (m)	1.91345	Linear Equation			r^2		0.978461	Pstd(mmHg)	760.0	
2	Intercept (b)	0.02773	Set Point Flow Rate (X) (m ³ /min)		1.133	r		0.9891719	T _{NTP}	298.0	
3	Correlation Coefficient (r)	0.99995	Final Set Flow Rate = (I)		0			(Pa/Pstd)*(Tstd/Ta)		0.973192407	
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.986505148	

COMMENT

Andersen Instruments, Inc.

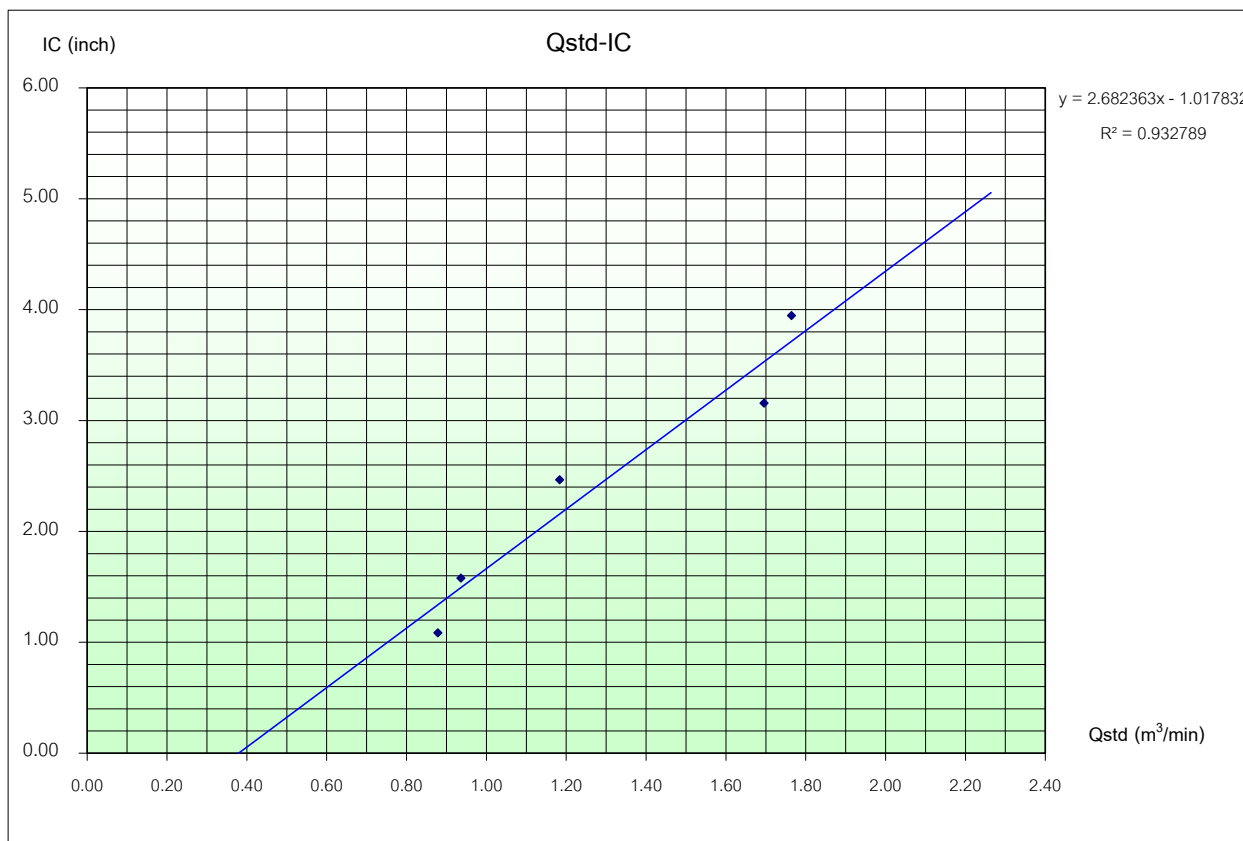

Calibrated By

(Mr.Preecha Srisuk)
Field Environmental

Approved By

(Mr.Jarung Jamnongbut)
Division Manager



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 14 November 2023

Instruments Information

Analyzer Type: NO/NO ₂ /NO _x Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 72706374
---	--

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 46.05 PPM SO ₂ Conc 46.01 PPM CO Conc 4,487 PPM Cylinder number CC507080 Expire Date: 23 Jul. 2025

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	395.2	400.0	-1.2
NO _x	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

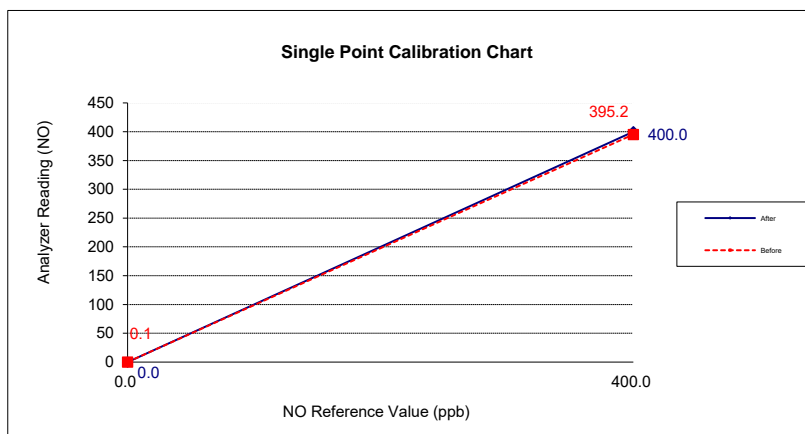

Calibrate By : Mr. Pasagorn Samol



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 14 November 2023

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 72706374
--	--

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 46.05 PPM SO2 Conc 46.01 PPM CO Conc 4,487 PPM Cylinder number CC507080 Expire Date: 23 Jul. 2025

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	395.2	400.0	-1.2
NOx	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

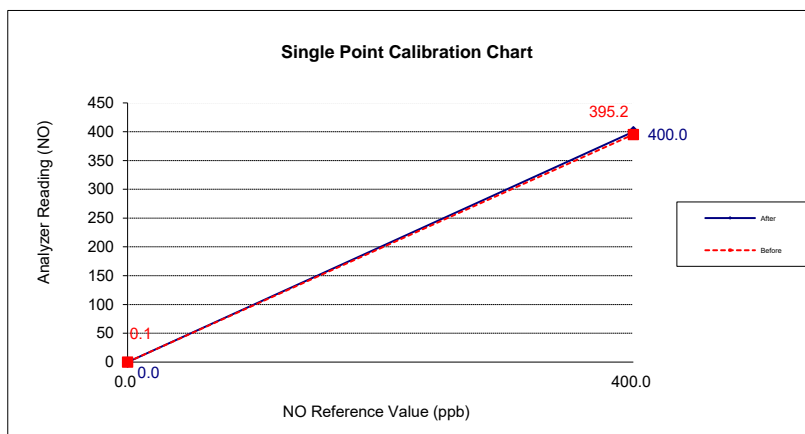

Calibrate By : Mr. Pasagorn Samol



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 14 November 2023

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 40	Manufacturer ECOTECH S/N: E020040
---	--------------------------------------

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	397.6	400.0	-0.6
NOx	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

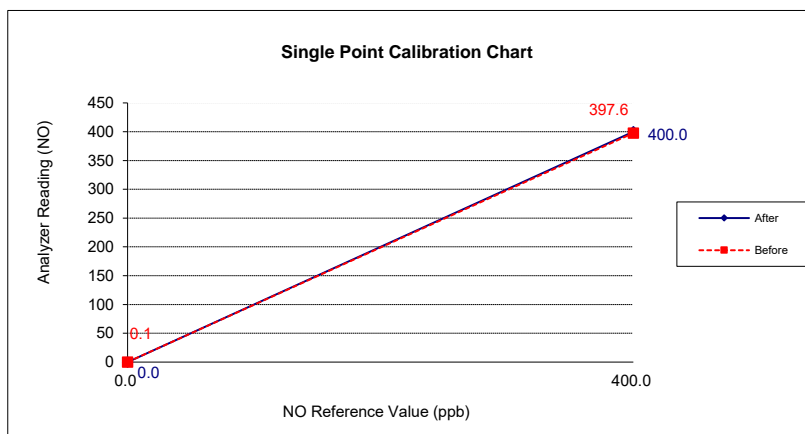

Calibrate By : Mr. Pasagorn Samol



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 14 November 2023

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 40	Manufacturer ECOTECH S/N: E020040
---	--------------------------------------

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	397.6	400.0	-0.6
NOx	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

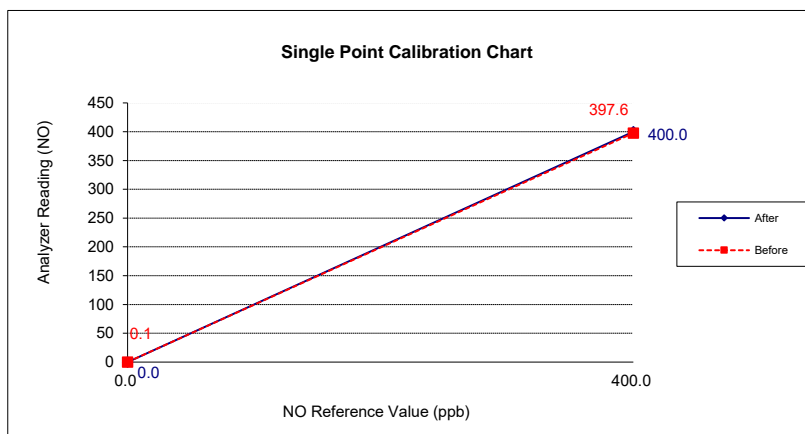

Calibrate By : Mr. Pasagorn Samol



บริษัท เอ็นไวร์ เซอร์วิส จำกัด
ENVIR SERVICE CO., LTD.

บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201

42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bankok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 14 November 2023

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer Thermo Environmental S/N: 72706371
--	--

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API Model 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	393.4	400.0	-1.7
NOx	0.1	0.0	0.1	396.7	400.0	-0.8

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NOx	0.0	0.0	0.0	400.0	400.0	0.0

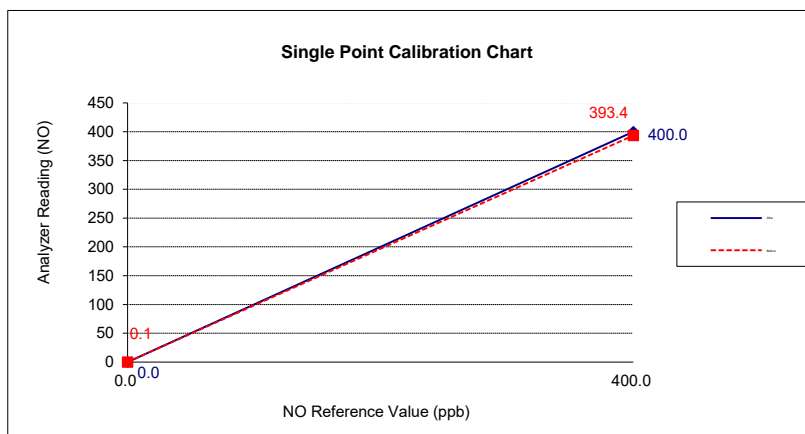

Calibrate By : Mr. Pasagorn Samol



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201
ENVIR SERVICE CO., LTD.

Analyzer Performance Test

Calibrated Date: 14 November 2023

Instruments Information

Analyzer Type: SO2 Analyzer Model: 50	Manufacturer ECOTECH S/N: E020050
--	--------------------------------------

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.3	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

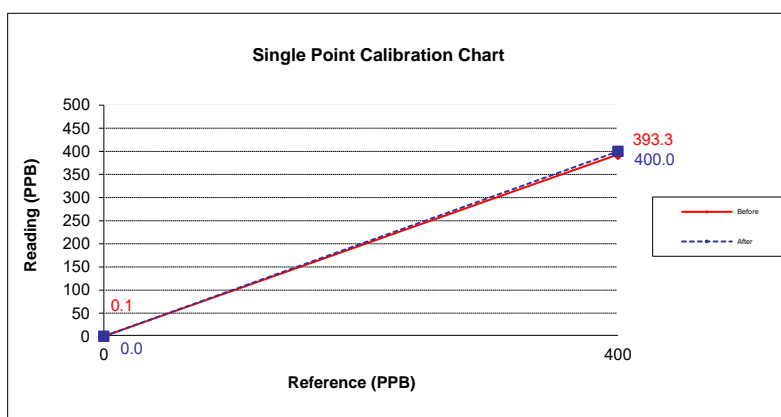

Calibrate By :

Mr.PASAGORN SAMOL



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201
ENVIR SERVICE CO., LTD.

Analyzer Performance Test

Calibrated Date: 14 November 2023

Instruments Information

Analyzer Type: SO2 Analyzer Model: 100A	Manufacturer API S/N: 196
--	------------------------------

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.5	-1.6
After	0.0	0.0	0.0	400.0	400.0	0.0

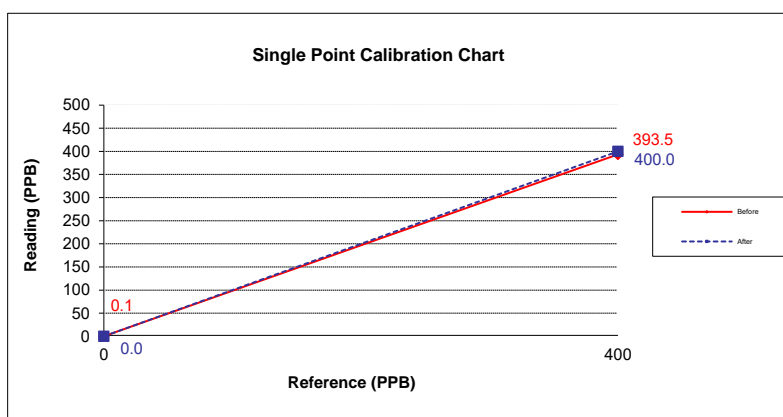

Calibrate By :

Mr.PASAGORN SAMOL



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201
ENVIR SERVICE CO., LTD.

Analyzer Performance Test

Calibrated Date: 14 November 2023

Instruments Information

Analyzer Type: SO2 Analyzer Model: 100A	Manufacturer API S/N: 193
--	------------------------------

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.4	-1.7
After	0.0	0.0	0.0	400.0	400.0	0.0

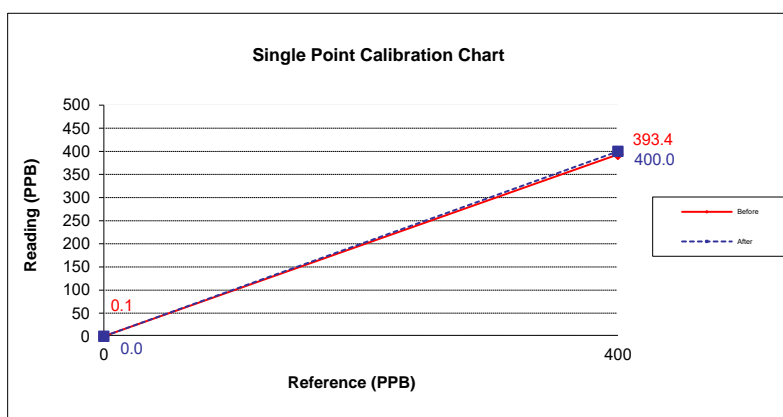

Calibrate By :

Mr.PASAGORN SAMOL



บริษัท เอ็นไวร์ เซอร์วิส จำกัด

42 รามอินทรา 14 แยก 9 แขวงท่าแร้ง เขตบางเขน กรุงเทพฯ 10230 โทรศัพท์ 02-9435814-5 โทรสาร 02-9438201
บริษัท เอ็นไวร์ เซอร์วิส จำกัด 42 Raminthra 14 yeak 9, Tha Rang, Bangkhen, Bangkok 10230 Tel : 02-9435814-5 Fax : 02-9438201

Analyzer Performance Test

Calibrated Date: 14 November 2023

Instruments Information

Analyzer Type: SO2 Analyzer Model: 100A	Manufacturer API S/N: 405
--	------------------------------

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model Dasibi Model 5008 S/N: 705 ZERO AIR Generator API MODEL 701 S/N: 1924	NO Conc 55.47 PPM SO2 Conc 55.11 PPM CO Conc 4,535 PPM Cylinder number EB0129027 Expire Date: 29 Oct. 2027

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	0.1	0.1	400.0	393.5	-1.6
After	0.0	0.0	0.0	400.0	400.0	0.0

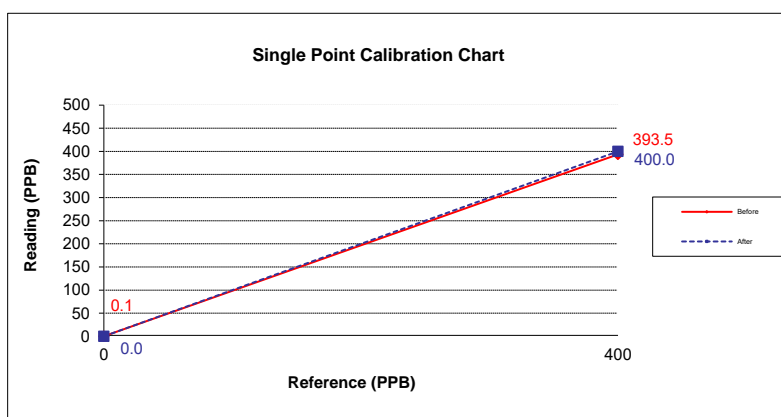

Calibrate By :

Mr.PASAGORN SAMOL



MULTIPOINT CALIBRATION

Nitrogen Oxide Analyzer

Station	MET CO.,LTD				
Brand	ECOTECH	Zero setting	0	Station Temp.	25 °C
Model	Serinus 40	Span Instrument Gain	2.63	Date	5-Jan-22
Range	500 ppb	Start Time	13:00	Span Source	Gas Cal 3000
S/N	12-1001	Finish Time	14:30		

NO Channel				
Span Set Point	Expect Concentration (ppb)	Analyzer Response (ppb)	Difference (ppb)	Percent Diff.
Zero	0	0	0	-
Point 1	400	392	-8	-2.00
Point 2	200	196	-4	-2.00
Point 3	100	97	-3	-3.00
Average Difference (%)				-2.33
Slope = 1.0055		Intercept = 0.5221		Correlation Coefficient = 1.000

NO _x Channel				
Span Set Point	Expect Concentration (ppb)	Analyzer Response (ppb)	Difference (ppb)	Percent Diff.
Zero	0	1	1	-
Point 1	400	400	0	0.00
Point 2	200	202	2	1.00
Point 3	100	104	4	4.00
Average Difference (%)				1.67
Slope = 0.996		Intercept = 2.1211		Correlation Coefficient = 1.000

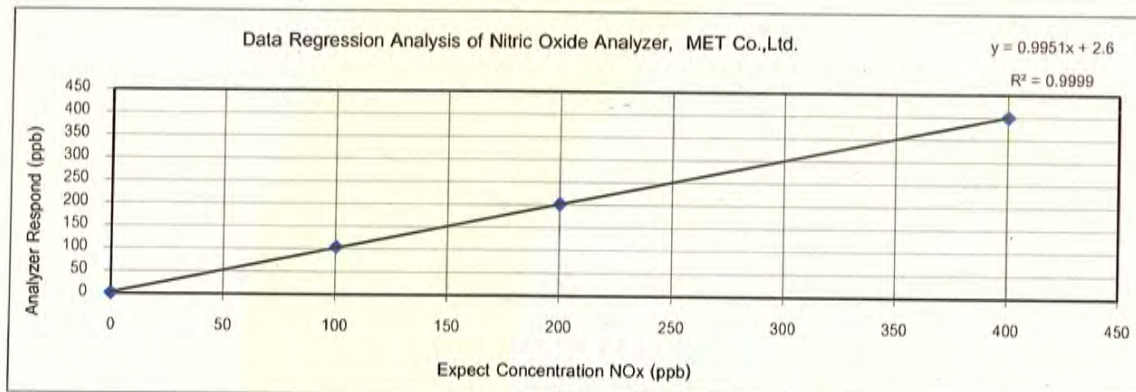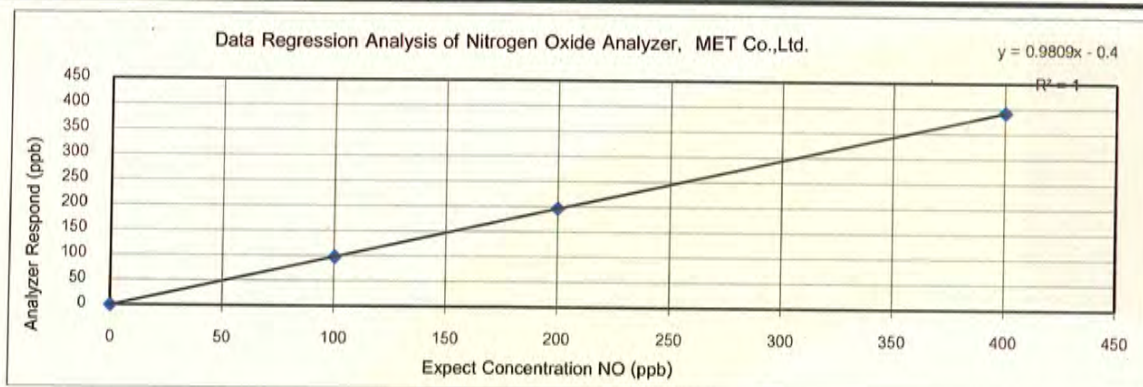

บริษัท สิทธีพรแอสโซซิเอต จำกัด

Signature

บริษัท สิทธีพร แอสโซซิเอต จำกัด

Sithiporn Associates Co., Ltd.

451-451/1 ถนนสิรินธร แขวงบางบำหรุ เขตบางพลัด กรุงเทพฯ 10700 โทร. 0-2433-8331, 0-2435-8800, 0-2434-9191 แฟกซ์ : 0-2433-1679, 0-2434-9510

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok 10700 Thailand Tel. (662) 433-8331, 435-8800, 434-9191 Fax: (662) 433-1679, 434-9510

EMAIL:center@sithiporn.com www.sithiporn.com



National Institute of Metrology (Thailand)

Certificate of Calibration



Certificate No. : AA-2022-23
Issued by : Acoustics Laboratory
Acoustics and Vibration Group



Page 1 of 5 pages

MEASUREMENT ITEM : Sound Calibrator
MANUFACTURER : RION
MODEL/TYPE : NC-75
SERIAL NUMBER : 34480442
CUSTOMER : MET Co., Ltd.
36/659 Moo 6, T. Bangrakphatthana,
A. Bangbuathong, Nonthaburi 11110
MEASUREMENT DATE : 25 August 2023

The reported measurement result relates only to the measurand and applies only at the time of measurement.

*The calibration results only marked with an asterisk * in this certificate are not included in the scope of accreditation.*

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%. This calibration certificate may not be reproduced other than in full except with the permission of the Director of National Institute of Metrology (Thailand).

Reference	Date	Authorized Signatory	Person in charge
AUVC132-01/23	25 August 2023	 (Dr. Charun Yafa)	 (Sawitri Srisatjarak)

This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognize the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

National Institute of Metrology (Thailand)

Ministry of Higher Education, Science, Research and Innovation

3/4-5 Moo 3, Klong 5, Klong Luang, Pathumthani 12120, Thailand. Tel: (66) 2577 5100, Fax: (66) 2577 3659

75/7 Rama VI Road, Rachathewi, Bangkok 10400, Thailand. Tel: (66) 2354 3700, Fax: (66) 2354 3692



UNCERTAINTY OF MEASUREMENT

The stated uncertainty is the expanded uncertainty obtained by multiplying the standard uncertainty by the coverage factor $k=2$. It has been determined in accordance with EA publication EA-4/02 M:2013 "Evaluation of the Uncertainty of Measurement in Calibration" and JCGM 100:2008 "Evaluation of measurement data --Guide to the Expression of Uncertainty in Measurement (GUM 1995 with minor corrections)". The value of the measured lies within the assigned range of value with a probability of 95 %.

Parameter	Uncertainty at SPL94 dB	Maximum-permitted uncertainty of measurement for a coverage probability of 95%	Unit
1.Sound Pressure level	0.08	0.15	dB
2. Frequency	0.1	0.2	%
3. THD+N	0.1	0.5	%

TRACEABILITY

This certificate provides traceability of measurement to recognized national standards, and to the realization of the International System of Units (SI).



ENVIRONMENTAL CONDITIONS

Ambient condition in the laboratory are as follows :

Temperature	:	(23.0 ± 1.0)	°C
Pressure	:	(101.325 ± 1.500)	kPa
Relative Humidity	:	(50.0 ± 15.0)	%

Reference Condition : 101.325 kPa , 23.0 °C and 50.0 %RH.

Calibration Condition

Preconditionings : 16 hours at ambient conditions.

Measurement Conditions : The average values during measurement are
 (100.343 ± 0.036) kPa, (22.0 ± 0.3) °C and (53.0 ± 2.0) %RH

MEASUREMENT METHOD

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone. The insert voltage technique was employed and the measurement procedure was based on IEC 60942: 2017.

Reference Microphone

4180 serial no.1395446

TABULATION OF RESULTS

The following tables give the calibration results and associated measurement uncertainties at 95% of confidence level. The calibration results of sound pressure level which quoted in dB with reference to 20 µPa are corrected to the values under the reference environmental conditions.

The calibration results exclude the calibrator pressure correction but include the microphone volume correction, which was obtained from the manufacturer instruction manual of the sound calibrator, at the level of 0 dB.

MEASUREMENT RESULTS

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value ^[1] (dB)	Acceptance Limit ^[2] (dB)
Microphone 4180 Serial No.1395446			
94	94.15	0.15	± 0.25

Note ^[1] : The deviated value is the absolute value of the difference between the measured value and the corresponding specified sound pressure level.

Note ^[2] : The acceptance limit is obtained from IEC 60942: 2017.

2. Frequency*

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ^[3] (%)	Acceptance Limit ^[4] (%)
At the sound pressure level of 94 dB			
1000	1000.0	0.0	± 0.7

Note ^[3] : The deviated value is the absolute value of the difference in percent between the measured value and the corresponding specified frequency.

Note ^[4] : The acceptance limit is obtained from IEC 60942: 2017.



3. Total distortion + Noise*

Microphone 4180 Serial No.1395446

Measured value ^[5] (%)	Maximum total distortion + Noise ^[6] (%)
At the sound pressure level of 94 dB	
0.2	2.5

Note ^[5]: The measured value is the total distortion, measured over the frequency range from 20 Hz to 20 kHz.

Note ^[6]: The maximum total distortion + noise is obtained from IEC 60942: 2017.

End of Certificate of Calibration

NIMT



Certificate of Calibration

Certificate Number : SPR23010010-4

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 76239

ID. Number : SLM-35

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :

(Mr.)

Authorized Signatory



Calibration Report

Certificate Number : SPR23010010-4

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-4

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010010-1

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : Rion

Model : NL-21

Serial Number : 00722042

ID. Number : SLM-46

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 04 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).


Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :

([Redacted Signature])

Authorized Signatory



Calibration Report

Certificate Number : SPR23010010-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010010-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010249-5

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222064

ID. Number : SLM-31

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 19 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 23 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 23 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 24 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Approved by :

Calibration Officer

Authorized Signatory



Calibration Report

Certificate Number : SPR23010249-5

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010249-5

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.1	114.1	0.1	0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.3	94.2	0.3	0.2	0.15
114	114.1	114.1	0.1	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010249-3

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222070

ID. Number : SLM-37

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 19 Jan 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 23 Jan 2023

Location of Calibration : In-Lab

Recommend Due Date : 23 Jan 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 24 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Karoon Pengsalung

Calibration Officer

Approved by :

(M

Authorized Signatory



Calibration Report

Certificate Number : SPR23010249-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010249-3

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.2	94.2	0.2	0.2	0.15
114	114.2	114.2	0.2	0.2	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23010249-1

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222071

ID. Number : SLM-38

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Jan 2023

Calibration Date : 23 Jan 2023

Recommend Due Date : 23 Jan 2024

Date of Issue : 24 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :



Authorized Signatory



Calibration Report

Certificate Number : SPR23010249-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010249-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.5	94.5	0.5	0.5	0.15
114	114.4	114.4	0.4	0.4	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

– End of Certificate –



Certificate of Calibration

Certificate Number : SPR23010249-8

Page : 1 of 3

Customer : MET CO.,LTD.

36/659 Moo. 6 Tambol Bangragpattana, Amphur Bangbuatong,
Nonthaburi 11110

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 222073

ID. Number : SLM-40

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Jan 2023

Calibration Date : 23 Jan 2023

Recommend Due Date : 23 Jan 2024

Date of Issue : 24 Jan 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by :

Authorized Signatory



Calibration Report

Certificate Number : SPR23010249-8

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	SC-942	B014059	EEL.BP. 34/1264	22 Dec 2023

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23010249-8

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.2	94.2	0.2	0.2	0.15
114	114.1	114.1	0.1	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

Certificate of Calibration

Certificate No. : 66-200067-2

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : AND Model : FX-2000i
Serial No. : 15639789 ID No. : MET-EB03/61
Capacity : 2200 g Resolution : 0.01 g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (26.7 to 26.8) °C
Relative Humidity : (53.4 to 61.0) %
Air Pressure : 1013.0 mbar

Date of Received : 02 March 2023

Date of Calibration : 02 March 2023

Date of Issue : 13 March 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
F181-F1821	66-210034-1	30 Jul 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-200067-2

Page : 2 of 2

Result of Calibration : After Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)	Error before Adjustment (g)
200	0.00	0.0083	0.02
500	0.00	0.0085	0.06
600	0.00	0.0086	0.07
700	0.00	0.0087	0.08
800	0.00	0.0089	0.09
1000	0.00	0.0093	0.11
1200	0.00	0.011	0.14
1500	-0.01	0.011	0.18
2000	-0.02	0.012	0.25
2200	-0.02	0.023	0.28


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 500 g

A	B	C	D	E	
0.00	-0.02	-0.02	-0.01	0.00	g



Repeatability

Load test : 2000 g

Stdev. : 0.000 g

- o0o -



Qualification of GC-MS System

GC-OQ

System ID: CN2138A118_MET
Organization Name: MET Company Limited
Organization Location: 36/659 Moo 6 Tambol Bangrakpattana Nonthaburi 11110 Thailand

Date: March 28, 2023 1:45:04 PM
EQP Name: AgilentRecommended
EQP Revision: GC.02.52
Overall Qualification Status: Pass

GC-MS System Logon

Logon: Saenguthai Tarak

Overall CDS Logon Verification - GC Test Status

Pass

GC-MS System Setpoint and Operation Test Status

Name: 8890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

GC-MS System Setpoint and Operation Test

Name: 8890

Front SSL

Setpoint Status: Pass

Pressure: 25.0 psi

Pressure Change: -0.1 psi /5 minutes

Agilent Recommended: ≥ -2.0 and ≤ 0.5

Date: March 28, 2023 1:45:04 PM
System ID: CN2138A118_MET

Overall Inlet Pressure Decay Test Status

Pass

Name: 8890
Front SSL

Setpoint Status: Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25.0	psi
Accuracy:			0.0	psi
Agilent Recommended:			<= 1.2	

Overall Inlet Pressure Accuracy Test Status

Pass

Name: 8890
Front FID

Setpoint Status: Pass

Flow Type:	Fuel				
Setpoint:	30.0	mL/min	Measured Flow:	30.1	mL/min
Accuracy:		0.1	mL/min		
Agilent Recommended:		<= 10.0	% setpoint	(3.0	ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Setpoint Status: Pass

Flow Type:	Oxidizer				
Setpoint:	400.0	mL/min	Measured Flow:	389.2	mL/min
Accuracy:		10.8	mL/min		
Agilent Recommended:		<= 10.0	% setpoint	(40.0	ml/min)

Limit is percentage of setpoint or 0.5 ml/minute, whichever is largest.

Date: March 28, 2023 1:45:04 PM
System ID: CN2138A118_MET

Setpoint Status: Pass

Flow Type: Makeup

Setpoint: 25.0 mL/min Measured Flow: 25.1 mL/min

Accuracy: 0.1 mL/min

Agilent Recommended: \leq 10.0 % setpoint (2.5 mL/min)

Limit is percentage of setpoint or 0.5 mL/minute, whichever is largest.

Overall Detector Flow Accuracy Test Status

Pass

Name: 8890

Setpoint Status: Pass

Zone: Oven

Setpoint/Actual

Temperature: 230.0 230.3 °C

Accuracy: 0.3 °C

Agilent Recommended: \geq -1.0 % setpoint in K (-5.0 °C) \leq 1.0 % setpoint in K (5.0 °C)**Setpoint Status:** Pass

Zone: Oven

Setpoint/Actual

Temperature: 100.0 100.3 °C

Accuracy: 0.3 °C

Agilent Recommended: \geq -1.0 % setpoint in K (-3.7 °C) \leq 1.0 % setpoint in K (3.7 °C)**Overall GC Oven Temperature Accuracy Test Status**

Pass

Name: 8890

Date: March 28, 2023 1:45:04 PM

System ID: CN2138A118_MET

Setpoint Average

Temperature: 100.0 100.2167 °C
Stability: 0.1 °C
Agilent Recommended: <= 0.5

Overall GC Oven Temperature Stability Test Status

Pass

Tested Combination1 Front SSL / Front FID
Injection Tower
Name: 7693A

Setpoint Status: Completed

Injection Volume on Column: 1.0 uL

Overall Scouting Run Status

Completed

Tested Combination1 Front SSL / Front FID
Name: 8890

Setpoint Status: Pass

Base Signal: 8.9 pA

ASTM Noise

Drift

pA

pA/Hr

0.05

0.94

Agilent Recommended: <= 0.10

<= 2.50

Status: Pass

Pass

Overall Noise and Drift Test Status

Pass

Date: March 28, 2023 1:45:04 PM
System ID: CN2138A118_MET

Tested Combination1 Front SSL / Front FID

Name: 7693A

Setpoint Status: **Pass**

Injection Volume on Column: 1.0 uL

Area RSD: 0.44 % Retention Time RSD: 0.17 %

Agilent Recommended: <= 3.00 <= 1.00

Overall Injection Precision Test Status

Pass

Tested Combination1 Front SSL / Front FID

Injection Tower

Name: 8890

Setpoint Status: **Pass**

Signal to Noise: 2198451

Agilent Recommended: >= 300000

Overall Signal to Noise Test Status

Pass

Injection Tower Data

System Configuration

This section describes the as found system configuration.

System

System ID	CN2138A118_MET
Manufacturer	Agilent Technologies
Name	8890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Injection Tower
Inlet	Front
Detector	Front
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Injection Tower
Name	7693A
Model Number	G4514A
Serial Number	CN22047055
Firmware Revision	A.11.03
Usage	Sample Injection
Location	Front
Syringe Volume (µL)	10

Date: March 28, 2023 1:45:04 PM
System ID: CN2138A118_MET

Sampler 2

Manufacturer	Agilent Technologies
Type	Tray
Name	7693A
Model Number	G4514A
Serial Number	CN22047055
Firmware Revision	A.11.03
Vial Heater	Not installed

Mainframe 1

Manufacturer	Agilent Technologies
Name	8890
Model Number	G3540A
Serial Number	CN2138A118
Firmware Revision	2.5.1.9
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	8890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	8890
Type	FID
Adapter	Capillary
Control Type	Electronic Pressure Control (EPC)
Location	Front
Makeup Gas	Nitrogen

Date: March 28, 2023 1:45:04 PM
System ID: CN2138A118_MET

Agilent e-Signature

Notice

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Saenguthai Tarak
Logged On User Name:	saenguthai.tarak@non.agilent.com
Signature Creation Date:	March 28, 2023
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Date:	March 28, 2023 1:45:04 PM
System ID:	CN2138A118_MET

CN2138A118 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 28, 2023 12:26:58 PM	Audit	SessionCreated	Session	None
March 28, 2023 12:26:58 PM	Audit	Entitlement	Licensing	Session identifier generated: 0800-0002-0000-08HM-Q85 G
March 28, 2023 12:26:58 PM	Start	Configuration	Session	None
March 28, 2023 12:32:02 PM	Audit	Entitlement	Licensing	Successfully unlocked session identified by 0800-0002-0000-08HM-Q85 G with unlock code xb1b-ckbx-4v0e-kzg1-0c4g
March 28, 2023 12:39:59 PM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.52/Gc.02.52.eqp], EQP File Name: [Gc.02.52.eqp], EQP Name: [AgilentRecommended], Protocol Revision :[Gc.02.52]
March 28, 2023 12:40:04 PM	End	Configuration	Session	None
March 28, 2023 12:40:11 PM	Start	Qualification	Session	OQ
March 28, 2023 12:40:12 PM	Start	Execution	CDS Logon Verification - GC : - Qualitative test	None
March 28, 2023 12:43:12 PM	End	Execution	CDS Logon Verification - GC : - Qualitative test	Run Count : 1
March 28, 2023 12:43:15 PM	Start	Execution	System Inspection and Basic Safety and Operation - 8890: - Qualitative Test - No setpoints associated	None

Page 1 / 6

Date: March 28, 2023 1:45:04 PM
System ID: CN2138A118_MET

Page 9 / 14

CN2138A118 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 28, 2023 12:43:31 PM	End	Execution	System Inspection and Basic Safety and Operation - 8890: - Qualitative Test - No setpoints associated	Run Count : 1
March 28, 2023 12:43:34 PM	Start	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	None
March 28, 2023 12:43:41 PM	End	Execution	Inlet Pressure Decay - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: >= -2.0 psi and <= 0.5 psi	Run Count : 1
March 28, 2023 12:43:43 PM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
March 28, 2023 12:43:48 PM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
March 28, 2023 12:43:50 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	None
March 28, 2023 12:44:12 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 28, 2023 12:44:20 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Fuel - S: 30.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 28, 2023 12:44:22 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	None
March 28, 2023 12:44:42 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry

Page 2 / 6

Date: March 28, 2023 1:45:04 PM
System ID: CN2138A118_MET

Page 10 / 14

CN2138A118 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 28, 2023 12:44:47 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Oxidizer - S: 400.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 28, 2023 12:44:52 PM	Start	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	None
March 28, 2023 12:45:03 PM	Audit	Data	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Manual Data Entry
March 28, 2023 12:45:07 PM	End	Execution	Detector Flow Accuracy - Front FID: - Type : Makeup - S: 25.0 mL/min - L: <= 10.0% setpoint	Run Count : 1
March 28, 2023 12:45:09 PM	Start	Execution	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
March 28, 2023 12:45:28 PM	Audit	Data	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
March 28, 2023 12:45:30 PM	End	Execution	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
March 28, 2023 12:45:31 PM	Start	Execution	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
March 28, 2023 12:45:48 PM	Audit	Data	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

Page 3 / 6

Date: March 28, 2023 1:45:04 PM
System ID: CN2138A118_MET

Page 11 / 14

CN2138A118 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 28, 2023 12:45:51 PM	End	Execution	GC Oven Temperature Accuracy - 8890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
March 28, 2023 12:45:53 PM	Start	Execution	GC Oven Temperature Stability - 8890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
March 28, 2023 12:46:53 PM	Audit	Data	GC Oven Temperature Stability - 8890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
March 28, 2023 12:46:57 PM	End	Execution	GC Oven Temperature Stability - 8890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
March 28, 2023 12:47:01 PM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
March 28, 2023 12:50:08 PM	Start	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	None
March 28, 2023 12:51:05 PM	Audit	Data	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Data files Path : F:\Data\SC011.D\FID1A.ch
March 28, 2023 12:51:52 PM	End	Execution	GC Scouting Run - Injection Tower, Front SSL, Front FID: - Part of System Preparation - No limits associated	Run Count : 1
March 28, 2023 12:51:57 PM	Start	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	None

Page 4 / 6

Date: March 28, 2023 1:45:04 PM
System ID: CN2138A118_MET

Page 12 / 14

CN2138A118 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 28, 2023 12:52:26 PM	Audit	Data	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Data files Path : F:\Data\ND012.D\FID1A.ch
March 28, 2023 12:53:21 PM	End	Execution	Noise and Drift - Front FID: - Detector FID - L (Noise): <= 0.10 pA - L (Drift): <= 2.50 pA/hour	Run Count : 1
March 28, 2023 12:53:28 PM	Start	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	None
March 28, 2023 1:12:20 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : F:\Data\Pre0107.D\FID1A.ch
March 28, 2023 1:12:20 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : F:\Data\Pre0108.D\FID1A.ch
March 28, 2023 1:12:20 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : F:\Data\Pre0109.D\FID1A.ch
March 28, 2023 1:12:20 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : F:\Data\Pre0110.D\FID1A.ch
March 28, 2023 1:12:24 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : F:\Data\Pre0111.D\FID1A.ch

CN2138A118 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
March 28, 2023 1:12:25 PM	Audit	Data	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Data files Path : F:\Data\Pre0112.D\FID1A.ch
March 28, 2023 1:13:38 PM	End	Execution	Injection Precision - Injection Tower, Front SSL, Front FID: - GC - L (Area): <= 3.00% - L (Ret. Time): <= 1.00%	Run Count : 1
March 28, 2023 1:13:49 PM	Start	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	None
March 28, 2023 1:16:08 PM	Audit	Data	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Data files Path : F:\Data\SN01.D\FID1A.ch
March 28, 2023 1:17:06 PM	End	Execution	Signal to Noise - Injection Tower, Front SSL, Front FID: - Detector FID - L: >= 300000	Run Count : 1
March 28, 2023 1:17:14 PM	End	Qualification	Session	OQ
March 28, 2023 1:17:14 PM	Start	Reporting	Session	None
March 28, 2023 1:43:49 PM	Audit	Reporting	Session	Report Generated : Certificate

ENVIR SERVICE CO., LTD.

42 RAMINTHRA 14 YEAK 9, THA RAENG, BANGKHEN, BANGKOK 10230
TAX ID 0105555170865
TEL 029435814-5 FAX 02-9438201



CALIBRATION CERTIFICATE

Certificate No. : 202103009

Date of issue : 23 April 21

Instrument Description	:	VOC Meter
Instrument Model	:	AQ VOC-V2
Instrument Serial No.	:	14656
ID No. or Control	:	-
Manufacture	:	E Instruments
Probe Description	:	-
Probe Model	:	-
Probe Serial	:	-
Customer Name	:	MET Co., Ltd.
Customer address	:	36/659 Moo 6 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110
Total Page of Certificate	:	2 Pages
Receiving Date	:	19 April 21
Parameter of Calibration	:	Gas Calibration (ISOBUTYLENE 103.13 PPM)
Condition Place	:	42 Raminthra 14 Yeak 9, Tha Raeng, Bangkhen, Bangkok 10230
Date of Calibration	:	23 April 21

Calibration by

Approve by

Kittisak Junsangwattana
Technician

Pasagorn Samol
Technician Manager

ENVIR SERVICE CO., LTD.

42 RAMINTHRA 14 YEAK 9, THA RAENG, BANGKHEN, BANGKOK 10230

TAX ID 0105555170865

TEL 029435814-5 FAX 02-9438201



CALIBRATION CERTIFICATE

Certificate No. : 202103009

Date of issue : 23 April 21

Standard References

Standard	Reference No.	Date
NITROGEN 99.999% (UHP)	Cylinder No. 809804	13-2-21
ISOBUTYLENE 103.13 PPM	Lot#GAP-248-100-2	April 4, 2021

Measured room conditions

Temperature : 25 °C

Humidity : 51 %RH

Pressure : 1010 mbra.

Calibration conditions

Gas Temperature : 21 °C

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift%
Nitrogen	0.1	0.0	0.1	0.0	0.0	0.0
ISOBUTYLENE 100 PPM	0.1	0.0	0.1	110.4	103.1	-6.6

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (ppm)	Reading Value (ppm)	Expected Value (ppm)	Drift%
Nitrogen	0.0	0.0	0.0	0.0	0.0	0.0
ISOBUTYLENE 100 PPM	0.0	0.0	0.0	104.1	103.1	-1.0

Factory Calibration Certificate

Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT) METER
Series No	3522210130
Type	JT2011-E2A

Integrity check of instrument

Appearance	✓
Parts integrity	✓
Screen display or touch	✓
Instrument button	✓
Power supply	✓
battery	✓
Data storage and export	✓
Deviation degree of comparison test with standard instrument	✓

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	25.0	25.2	-0.2	0.2
	30.0	29.9	0.1	0.2
	35.0	35.1	-0.1	0.2
	40.0	39.8	0.2	0.2
	45.0	44.9	0.1	0.2
DRY	25.0	24.8	0.2	0.2
	30.0	30.2	-0.2	0.2
	35.0	35.2	-0.2	0.2
	40.0	39.8	0.2	0.2
	45.0	44.9	0.1	0.2
GLOBE	25.0	24.8	0.2	0.2
	30.0	29.9	0.1	0.2
	35.0	34.8	0.2	0.2
	40.0	39.8	0.2	0.2
	45.0	44.9	0.1	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH±10RH%

Reference Standard : Standard Mercury Thermometers , Manufacturer: BGRI, Model: STA, SN : 2-56,

Calibrated Date : 30 March 2022, Calibration Certificate No.: RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer

Date : February 23, 2023

Factory Calibration Certificate

JANTYTECH
建通科技

Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT) METER
Series No	3522210131
Type	JT2011-E2A

Integrity check of instrument

Appearance	✓
Parts integrity	✓
Screen display or touch	✓
Instrument button	✓
Power supply	✓
battery	✓
Data storage and export	✓
Deviation degree of comparison test with standard instrument	✓

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	25.0	25.2	-0.2	0.2
	30.0	30.2	-0.2	0.2
	35.0	34.8	0.2	0.2
	40.0	40.1	-0.1	0.2
	45.0	44.9	0.1	0.2
DRY	25.0	24.8	0.2	0.2
	30.0	30.2	-0.2	0.2
	35.0	35.2	-0.2	0.2
	40.0	40.2	-0.2	0.2
	45.0	45.2	-0.2	0.2
GLOBE	25.0	24.8	0.2	0.2
	30.0	29.9	0.1	0.2
	35.0	35.1	-0.1	0.2
	40.0	39.9	0.1	0.2
	45.0	44.9	0.1	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH±10RH%

Reference Standard : Standard Mercury Thermometers , Manufacturer: BGRI, Model: STA, SN : 2-56,

Calibrated Date : 30 March 2022, Calibration Certificate No.: RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer :

Date : February 23, 2023



JANTYTECH
建通科技

Factory Calibration Certificate

Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT) METER
Series No	3522210132
Type	JT2011-E2A

Integrity check of instrument

Appearance	✓
Parts integrity	✓
Screen display or touch	✓
Instrument button	✓
Power supply	✓
battery	✓
Data storage and export	✓
Deviation degree of comparison test with standard instrument	✓

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	25.0	24.9	0.1	0.2
	30.0	29.9	0.1	0.2
	35.0	35.1	-0.1	0.2
	40.0	40.1	-0.1	0.2
	45.0	45.2	-0.2	0.2
DRY	25.0	25.1	-0.1	0.2
	30.0	30.1	-0.1	0.2
	35.0	34.8	0.2	0.2
	40.0	40.1	-0.1	0.2
	45.0	44.9	0.1	0.2
GLOBE	25.0	24.9	0.2	0.2
	30.0	29.9	0.1	0.2
	35.0	34.8	0.2	0.2
	40.0	40.1	-0.1	0.2
	45.0	45.2	-0.2	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH±10RH%

Reference Standard : Standard Mercury Thermometers , Manufacturer: BGRI, Model: STA, SN : 2-56,

Calibrated Date : 30 March 2022, Calibration Certificate No.: RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer

Date : February 23, 2023



JANTYTECH
建通科技

Factory Calibration Certificate

Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT) METER
Series No	3522210133
Type	JT2011-E2A

Integrity check of instrument

Appearance	✓
Parts integrity	✓
Screen display or touch	✓
Instrument button	✓
Power supply	✓
battery	✓
Data storage and export	✓
Deviation degree of comparison test with standard instrument	✓

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	25.0	25.1	-0.1	0.2
	30.0	30.2	-0.2	0.2
	35.0	34.9	0.1	0.2
	40.0	39.8	0.2	0.2
	45.0	45.2	-0.2	0.2
DRY	25.0	24.9	0.1	0.2
	30.0	29.8	0.2	0.2
	35.0	34.9	0.1	0.2
	40.0	40.2	-0.2	0.2
	45.0	45.1	-0.1	0.2
GLOBE	25.0	25.2	-0.2	0.2
	30.0	29.9	0.1	0.2
	35.0	34.8	0.2	0.2
	40.0	39.8	0.2	0.2
	45.0	44.9	0.1	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH±10RH%


Reference Standard : Standard Mercury Thermometers , Manufacturer: BGRI, Model: STA, SN : 2-56,

Calibrated Date : 30 March 2022, Calibration Certificate No.: RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer : _____

Date : _____

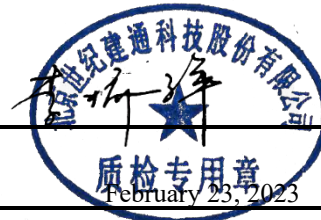

Factory Calibration Certificate

Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT) METER
Series No	3522210134
Type	JT2011-E2A

Integrity check of instrument

Appearance	✓
Parts integrity	✓
Screen display or touch	✓
Instrument button	✓
Power supply	✓
battery	✓
Data storage and export	✓
Deviation degree of comparison test with standard instrument	✓

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	25.0	25.1	-0.1	0.2
	30.0	29.8	0.2	0.2
	35.0	34.9	0.1	0.2
	40.0	40.1	-0.1	0.2
	45.0	44.8	0.2	0.2
DRY	25.0	24.8	0.2	0.2
	30.0	29.8	0.2	0.2
	35.0	34.9	0.1	0.2
	40.0	40.2	-0.2	0.2
	45.0	45.1	-0.1	0.2
GLOBE	25.0	24.9	0.1	0.2
	30.0	29.9	0.1	0.2
	35.0	34.8	0.2	0.2
	40.0	40.2	-0.2	0.2
	45.0	45.1	-0.1	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH±10RH%

Reference Standard : Standard Mercury Thermometers , Manufacturer: BGRI, Model: STA, SN : 2-56,

Calibrated Date : 30 March 2022, Calibration Certificate No.: RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer : _____

Date : February 23, 2023



Factory Calibration Certificate



Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT) METER
Series No	3522210135
Type	JT2011-E2A

Integrity check of instrument

Appearance	✓
Parts integrity	✓
Screen display or touch	✓
Instrument button	✓
Power supply	✓
battery	✓
Data storage and export	✓
Deviation degree of comparison test with standard instrument	✓

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	25.0	24.9	0.1	0.2
	30.0	30.2	-0.2	0.2
	35.0	34.8	0.2	0.2
	40.0	39.8	0.2	0.2
	45.0	45.1	-0.1	0.2
DRY	25.0	24.8	0.2	0.2
	30.0	30.1	-0.1	0.2
	35.0	34.9	0.1	0.2
	40.0	39.8	0.2	0.2
	45.0	44.9	0.1	0.2
GLOBE	25.0	25.2	-0.2	0.2
	30.0	30.1	-0.1	0.2
	35.0	35.2	-0.2	0.2
	40.0	39.8	0.2	0.2
	45.0	44.9	0.1	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH±10RH%


Reference Standard : Standard Mercury Thermometers , Manufacturer: BGRI, Model: STA, SN : 2-56,

Calibrated Date : 30 March 2022, Calibration Certificate No.: RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer : _____

Date : _____

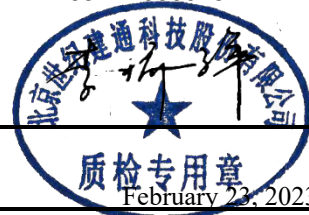

JANTYTECH
建通科技

Factory Calibration Certificate

Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT) METER
Series No	3522210136
Type	JT2011-E2A

Integrity check of instrument

Appearance	✓
Parts integrity	✓
Screen display or touch	✓
Instrument button	✓
Power supply	✓
battery	✓
Data storage and export	✓
Deviation degree of comparison test with standard instrument	✓

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	25.0	24.9	0.1	0.2
	30.0	29.9	0.1	0.2
	35.0	35.1	-0.1	0.2
	40.0	39.8	0.2	0.2
	45.0	45.1	-0.1	0.2
DRY	25.0	25.2	-0.2	0.2
	30.0	29.8	0.2	0.2
	35.0	35.2	-0.2	0.2
	40.0	39.8	0.2	0.2
	45.0	44.8	0.2	0.2
GLOBE	25.0	25.2	-0.2	0.2
	30.0	30.1	-0.1	0.2
	35.0	34.9	0.1	0.2
	40.0	39.8	0.2	0.2
	45.0	45.1	-0.1	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH±10RH%


Reference Standard : Standard Mercury Thermometers , Manufacturer: BGRI, Model: STA, SN : 2-56,

Calibrated Date : 30 March 2022, Calibration Certificate No.: RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer : _____

Date : _____

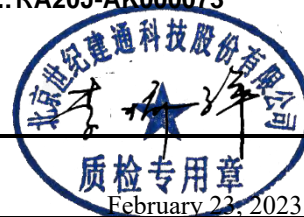

JANTYTECH
建通科技

Factory Calibration Certificate

Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT) METER
Series No	3522210137
Type	JT2011-E2A

Integrity check of instrument

Appearance	✓
Parts integrity	✓
Screen display or touch	✓
Instrument button	✓
Power supply	✓
battery	✓
Data storage and export	✓
Deviation degree of comparison test with standard instrument	✓

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	25.0	25.2	-0.2	0.2
	30.0	30.1	-0.1	0.2
	35.0	34.9	0.1	0.2
	40.0	40.2	-0.2	0.2
	45.0	44.8	0.2	0.2
DRY	25.0	24.9	0.1	0.2
	30.0	30.1	-0.1	0.2
	35.0	34.9	0.1	0.2
	40.0	39.8	0.2	0.2
	45.0	45.1	-0.1	0.2
GLOBE	25.0	24.8	0.2	0.2
	30.0	29.9	0.1	0.2
	35.0	34.9	0.1	0.2
	40.0	40.1	-0.1	0.2
	45.0	45.2	-0.2	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH±10RH%


Reference Standard : Standard Mercury Thermometers , Manufacturer: BGRI, Model: STA, SN : 2-56,

Calibrated Date : 30 March 2022, Calibration Certificate No.: RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer : _____

Date : _____

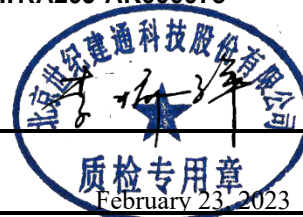

JANTYTECH
建通科技

Factory Calibration Certificate

Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT) METER
Series No	3522210138
Type	JT2011-E2A

Integrity check of instrument

Appearance	✓
Parts integrity	✓
Screen display or touch	✓
Instrument button	✓
Power supply	✓
battery	✓
Data storage and export	✓
Deviation degree of comparison test with standard instrument	✓

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	25.0	25.1	-0.1	0.2
	30.0	30.1	-0.1	0.2
	35.0	35.2	-0.2	0.2
	40.0	39.8	0.2	0.2
	45.0	45.1	-0.1	0.2
DRY	25.0	24.8	0.2	0.2
	30.0	29.9	0.1	0.2
	35.0	35.2	-0.2	0.2
	40.0	39.9	0.1	0.2
	45.0	45.2	-0.2	0.2
GLOBE	25.0	25.1	-0.1	0.2
	30.0	29.9	0.1	0.2
	35.0	35.2	-0.2	0.2
	40.0	39.8	0.2	0.2
	45.0	44.9	0.1	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH±10RH%


Reference Standard : Standard Mercury Thermometers , Manufacturer: BGRI, Model: STA, SN : 2-56,

Calibrated Date : 30 March 2022, Calibration Certificate No.: RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer : _____

Date : _____

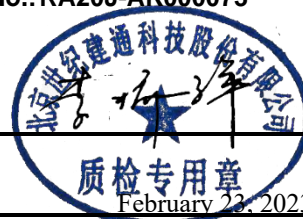



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkac Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202301038-001

Date Issued : 16-Jan-23

Customer : MET CO.,LTD.
36/659 Moo 6 T. Bangrakpattana A.Bangbuatong Nonthaburi 11110

Equipment : Heat Stress Meter

Manufacturer : Metrosonic

Model : hs-32

Serial No. : MCE010018

ID No./Tag No. : HT-02

Date Received : 13-Jan-23

Date Calibrated : 13-Jan-23

Calibrated by : Mr. Apiwat Peanrungrot

Calibration Method or Calibration Procedure Used

In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

(M)



Certificate No. : L202301038-001

Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD Reading ($^\circ\text{C}$)	UUC Reading ($^\circ\text{C}$)			UUC Error ($^\circ\text{C}$)	Measurement Uncertainty ($\pm^\circ\text{C}$)
		Before Adjusted	After Adjusted		
24.00	WET	23.9	-	-0.10	0.35
28.01	DRY	27.7	-	-0.31	0.40
30.00	GLOBE	30.1	-	0.10	0.35
27.02	WET	26.9	-	-0.12	0.35
32.00	DRY	31.9	-	-0.10	0.40
35.00	GLOBE	35.1	-	0.10	0.35
30.00	WET	29.8	-	-0.20	0.35
36.01	DRY	35.6	-	-0.41	0.40
40.01	GLOBE	40.0	-	-0.01	0.35

STD = Standard

UUC = Unit Under Calibration

Description of UUC :

Range	0 to 100	$^\circ\text{C}$
Resolution	0.1	$^\circ\text{C}$

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202210258-006 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 10-Nov-23

End of Certificate

Certificate of Calibration

Certificate No. : 66-400476-3 **Page : 1 of 2**

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Refrigerator)
Manufacturer : Sanden Intercool Model : YPR-068S
Range : N/A °C Resolution : 1 °C
Serial No. : YPR0659S-141200060R ID No. : MET-RE03/59

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (29.5 to 30.5) °C
Relative Humidity : (54 to 57) %
Line Voltage : (220.5 to 221.8) V

Date of Received : 23 August 2023

Date of Calibration : 23 August 2023

Date of Issue : 23 August 2023

Calibrated by : Bunjerd Masri

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400028	66-400184-3	04 Oct 2023	National Institute of Metrology Thailand (NIMT)

Approved by :



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400476-3 **Page : 1 of 2**

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Refrigerator)
Manufacturer : Sanden Intercool Model : YPR-068S
Range : N/A °C Resolution : 1 °C
Serial No. : YPR0659S-141200060R ID No. : MET-RE03/59

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (29.5 to 30.5) °C
Relative Humidity : (54 to 57) %
Line Voltage : (220.5 to 221.8) V

Date of Received : 23 August 2023

Date of Calibration : 23 August 2023

Date of Issue : 23 August 2023

Calibrated by : Bunjerd Masri

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400028	66-400184-3	04 Oct 2023	National Institute of Metrology Thailand (NIMT)

Approved by :



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400476-3


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

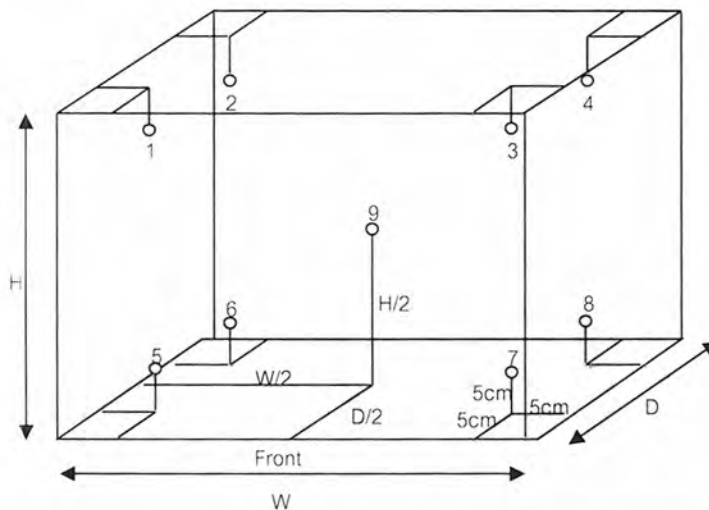

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.45 m

Capacity = 0.50 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
3	3	3	4.3	4.1	4.3	4.3	2.9	3.4	3.0	3.4	3.3	0.83

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
3	3	3	1.1	0.1	1.7

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-400619-1

Page : 1 of 2

Submitted by : MET Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Refrigerator)

Manufacturer : Sanden Intercool

Model : SRC-680SRTM

Range : N/A °C

Resolution : 1 °C

Serial No. : SRC680201-1107-00165

ID No. : MET-RE 01/54

Environment : On site calibration was carried out at the Laboratory, MET Company Limited

Ambient Temperature : (29.0 to 30.0) °C

Relative Humidity : (55 to 60) %

Line Voltage : (226.5 to 228.2) V

Date of Received : 07 November 2023

Date of Calibration : 07 November 2023

Date of Issue : 11 November 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400042	66-400453-1	31 Jan 2024	National Institute of Metrology Thailand (NIMT)

Approved by



Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400619-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

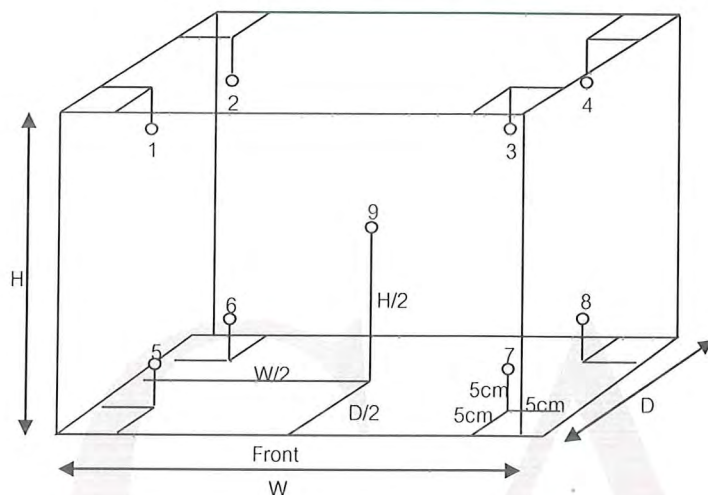

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.35 m

Capacity = 0.47 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
3	2	2	3.84	3.95	3.07	3.10	3.47	3.74	3.67	3.90	2.93	0.75

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
3	2	2	1.09	0.17	1.31

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-400476-3


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

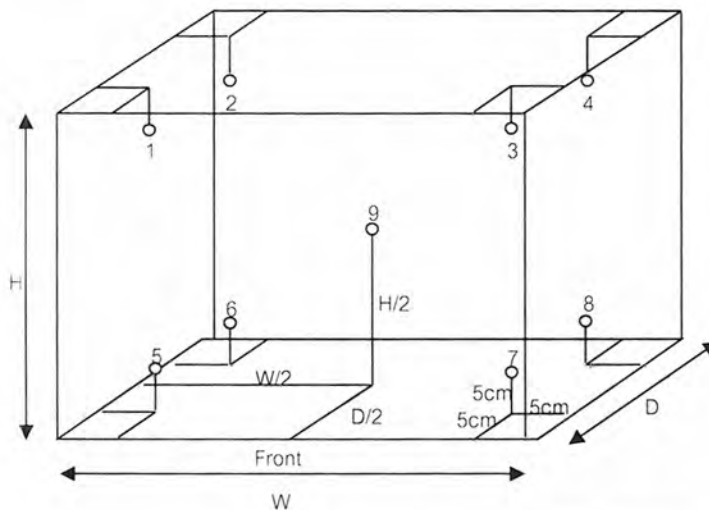

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.45 m

Capacity = 0.50 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
3	3	3	4.3	4.1	4.3	4.3	2.9	3.4	3.0	3.4	3.3	0.83

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
3	3	3	1.1	0.1	1.7

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-400619-1

Page : 1 of 2

Submitted by : MET Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Refrigerator)

Manufacturer : Sanden Intercool

Model : SRC-680SRTM

Range : N/A °C

Resolution : 1 °C

Serial No. : SRC680201-1107-00165

ID No. : MET-RE 01/54

Environment : On site calibration was carried out at the Laboratory, MET Company Limited

Ambient Temperature : (29.0 to 30.0) °C

Relative Humidity : (55 to 60) %

Line Voltage : (226.5 to 228.2) V

Date of Received : 07 November 2023

Date of Calibration : 07 November 2023

Date of Issue : 11 November 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400042	66-400453-1	31 Jan 2024	National Institute of Metrology Thailand (NIMT)

Approved by



Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400619-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

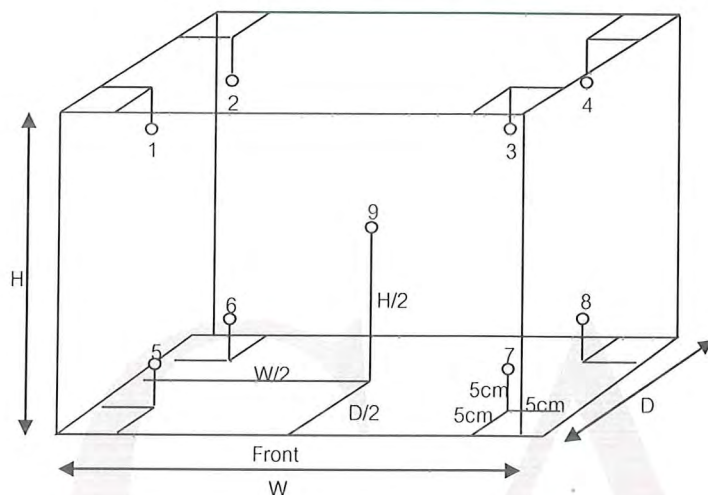

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.35 m

Capacity = 0.47 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
3	2	2	3.84	3.95	3.07	3.10	3.47	3.74	3.67	3.90	2.93	0.75

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
3	2	2	1.09	0.17	1.31

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-200253-1

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : Sartorius Model : BSA224S-CW
Serial No. : 35090472 ID No. : MET-EB 02/60
Capacity : 220 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (25.6 to 25.8) °C
Relative Humidity : (57.3 to 57.8) %
Air Pressure : 1005.0 mbar

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 11 August 2022

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 5, July 2015

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02213103	18 Nov 2022	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Signature)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-200253-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.05	0.0000	0.00011
0.1	0.0000	0.00013
0.5	0.0000	0.00013
1	0.0000	0.00011
5	0.0000	0.00011
10	0.0001	0.00011
50	0.0001	0.00013
100	0.0000	0.00020
150	0.0000	0.00038
200	0.0000	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.11$, providing a level of confidence of approximately 95%

Eccentric error Load test : 50 g

A	B	C	D	E	
0.0001	0.0001	0.0001	0.0000	0.0000	g



Repeatability Load test : 200 g

Stdev. : 0.00005 g

- o0o -



Certificate of Calibration

Certificate No. : 66-200271-1

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : Sartorius Model : BSA224S-CW
Serial No. : 35090472 ID No. : MET-EB 02/60
Capacity : 220 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (25.0 to 25.6) °C
Relative Humidity : (52.3 to 55.6) %
Air Pressure : 1005.0 mbar

Date of Received : 23 August 2023

Date of Calibration : 23 August 2023

Date of Issue : 25 August 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C0222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Signature)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-200271-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.05	0.0000	0.00011
0.1	0.0000	0.00011
0.5	0.0001	0.00011
1	0.0000	0.00011
5	0.0000	0.00011
10	0.0001	0.00012
50	0.0001	0.00014
100	0.0001	0.00020
150	0.0001	0.00038
200	0.0000	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.11$, providing a level of confidence of approximately 95%

Eccentric error Load test : 50 g

A	B	C	D	E	
0.0001	0.0001	0.0001	0.0001	0.0000	g



Repeatability Load test : 200 g

Stdev. : 0.00005 g

- oOo -



Certificate of Calibration

Certificate No. : 66-400012-1

Page : 1 of 2

Submitted by : M E T Company Limited
6/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Digital Thermometer with Thermistor Probe
Temperature Indicator

Manufacturer :	Thermo Scientific	Model :	pH 150
Range :	N/A	Resolution :	0.1 °C
Serial No. :	2657036	ID No. :	MET-PH04/60
Thermistor Probe			
Model :	PHWPTEM01W	Sheath Material :	Stainless
Diameter :	3 mm.	Length :	85 mm.
Serial No. :	237	ID No. :	MET-PH04/60

Environment : Ambient Temperature : (23 ± 2) °C
Relative Humidity : (50 ± 15) %
Line Voltage : (220 ± 22) VAC

Date of Received : 05 January 2023

Date of Calibration : 11 January 2023

Date of Issue : 11 January 2023

Calibrated by : Bunjerd Masri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-20	04 Mar 2022	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)
400004	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400012-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
85	10.0035	9.8	0.2	0.11
85	50.0025	50.0	0.0	0.11

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -



Certificate of Calibration

Certificate No. : 64-400425-5

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Incubator)

Manufacturer : M-LAB

Model : BIC-140

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 240412

ID No. : MET-BI01/55

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by : Permpoon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400032	65-400274-1	25 Nov 2022	National Institute of Metrology Thailand (NIMT)

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. :64-400425-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

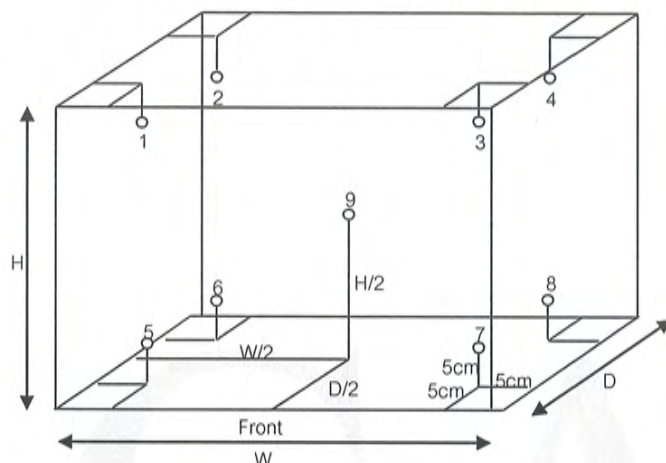

Inside of Chamber

W = 0.37 m

D = 0.33 m

H = 1.14 m

Capacity = 0.14 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	19.8	19.7	19.6	19.6	20.4	20.2	20.3	19.8	19.9	0.54

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.6	0.1	1.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-400476-5

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Incubator)
Manufacturer : M-LAB Model : BIC-140
Range : N/A °C Resolution : 0.1 °C
Serial No. : 240412 ID No. : MET-BI01/55

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (31.0 to 32.0) °C
Relative Humidity : (55 to 60) %
Line Voltage : (210.0 to 210.8) V

Date of Received : 23 August 2023

Date of Calibration : 23 August 2023

Date of Issue : 23 August 2023

Calibrated by : Permpon Chanpu


Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400043	66-400226-1	27 Oct 2023	National Institute of Metrology Thailand (NIMT)

Approved by :

()
Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400476-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

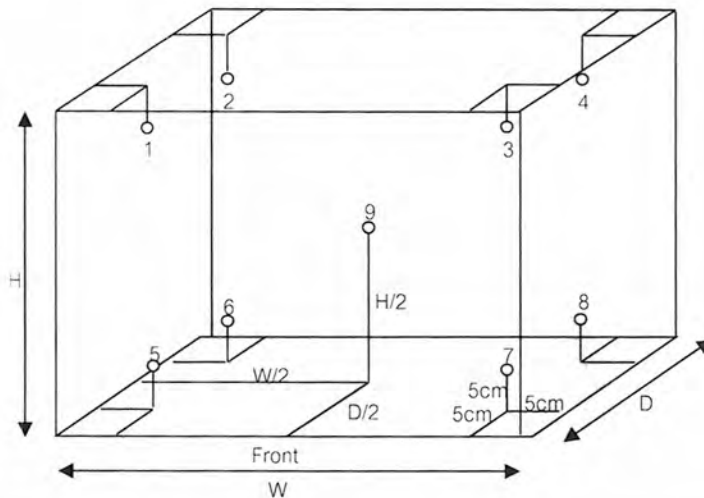

Inside of Chamber

W = 0.37 m

D = 0.33 m

H = 1.14 m

Capacity = 0.14 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	19.94	19.63	19.66	19.60	20.31	20.38	20.27	20.01	20.22	0.34

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.68	0.05	0.9

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Calibration Certificate

Cert. No. : CT-23-05-23470

Page : 1 of 4

Issued date : 08 May 2023

Equipment : COD Reader , Manufacturer : MLAB , Model : DB1602

S/N = 0169 , Customer ID = -

Client : M E T COMPANY LIMITED.

36/659 M.6 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

Received Date : 03 May 2023

Ref. Job No. : SO6605-00001

Calibrate by : Mr.Pramot Srisukum

Cert. prepare by : Ms.Nattanicha Panumram

Calibrated Date : 03 May 2023

Approved by : Mr.Montree Ruschasetkul

Calibration Place : Laboratory room

Environment Condition : Temperature 28.6 ± 0.4 (°C) , Humidity 59.5 ± 3.5 (%RH)

Calibration Method : Measure temperature distribution by 9 channel in flat level. , (MTEC WI No. # WICAL-02-005-R01)

Reference Standard Instrument :

No	Instrument	code	Model	Due date
1	Temperature Datalogger	MTEC-CE-0180	MLAB	10/2023
2	Thermo Hygrometer	MTEC-CE-0181	TH-03A	06/2023

Condition of certificate :

(1) This certificate is traceable to International System of units (SI Units). , (2) This certificate was certified only for the instrument we calibrated. , (3) This result of calibration was found accurate as show on date and place of calibration only. , (4) The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k =$ (see result table) , providing a level of confidence of approximately 95%. , (5) This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Division, Metrology Technical Co.,Ltd.

Certificate No. : CT-23-05-23470

Calibration Result :

Page : 2 of 4

Condition of UUC :


- 1) Without Adjustment
- 2) Immersion : 1/2 of the depth of the hole

(1) The quoted uncertainty include with * Stability*.

(2) Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors , for at least half an hour after reaching steted state.

(3) Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

(4) Overall variation = The difference of the maximum and the minimum measured temperature throughout observation time.

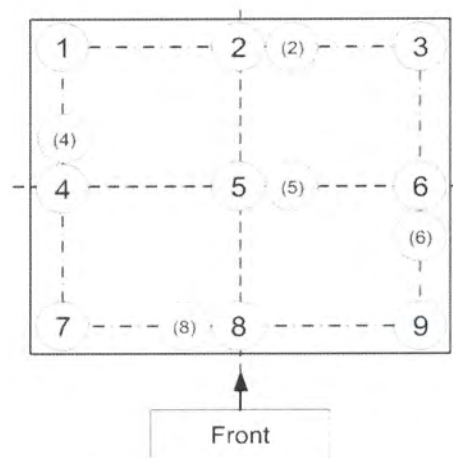

Pic 1 : Position of each sensor No.

Section 1 : Report of Temperature distribution

Unit : (°c)

Calibration Point	UUC Setting (*)	UUC Reading (*)	Measured Temperature @ Sensor No.									Uncertainty (±)	k(**)
			#1	#2	#3	#4	#5	#6	#7	#8	#9		
150	150	150	150.51	149.89	150.16	149.93	150.56	150.67	149.80	150.25	149.76	0.627	2

(*) = The average of 30 values in each point , (**) = Coverage factor (k) value

Section 2 : Report of Chamber Performance

Unit : (°c)

Calibration Point	UUC Setting	UUC Reading (*)	Temperature Uniformity	Temperature Stability (± °c)	Temperature Overall Variation
150	150	150	1	0.05	1

(*) = The average of 30 values in each point

Approved Signatory : ..

Certificate No. : CT-23-05-23470

Page : 3 of 4


Section 3 : Possible of temperature. Show minimum and maximum of the average values and Include with uncertainty of measurement. The average values is average of each position standard sensor throughtout observation time.

Unit : (°c)

Calibration Point	UUC Setting ^(*)	UUC Reading ^(*)	Possible of Minimum temperature	Possible of Maximum temperature
150	150	150	149.14	151.30

(*) = The average of 30 values in each point

Section 4 : Trend of accuracy

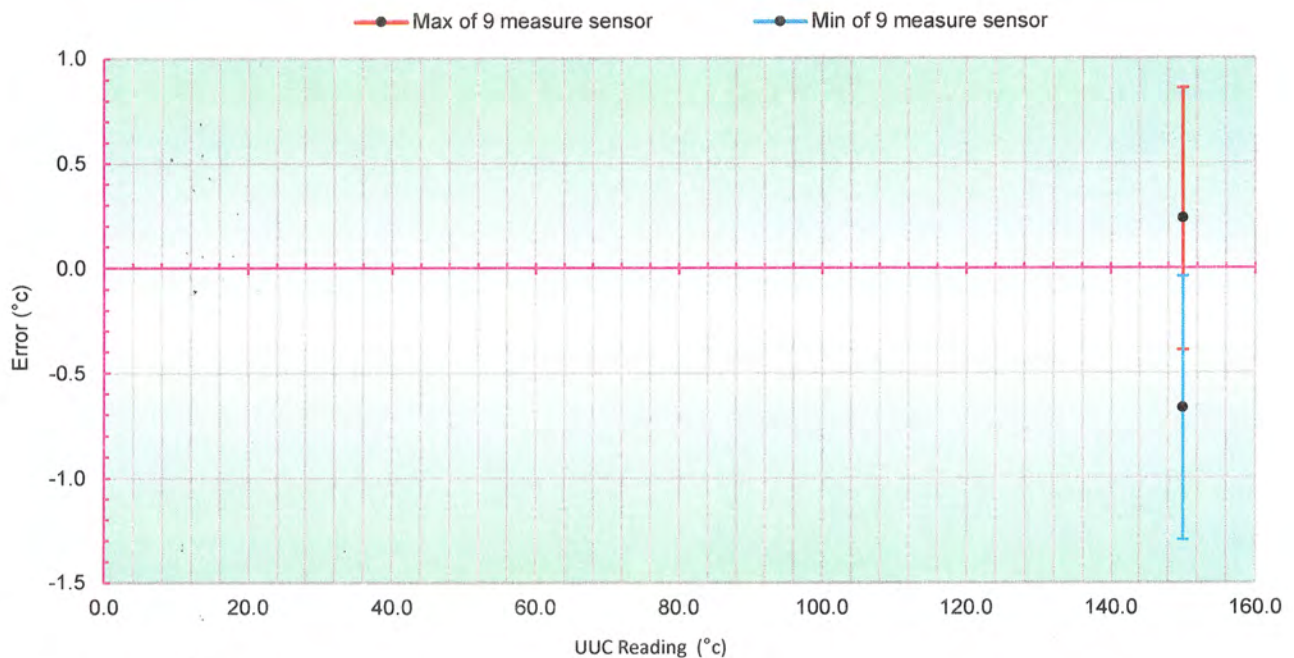


Approved Signatory :

Certificate No. : CT-23-05-23470

Page : 4 of 4

Section 5 : Graph report for Temperature distribution , not include uncertainty of measurement

(5.1) Temperature Distribution at UUC Reading 150 °C

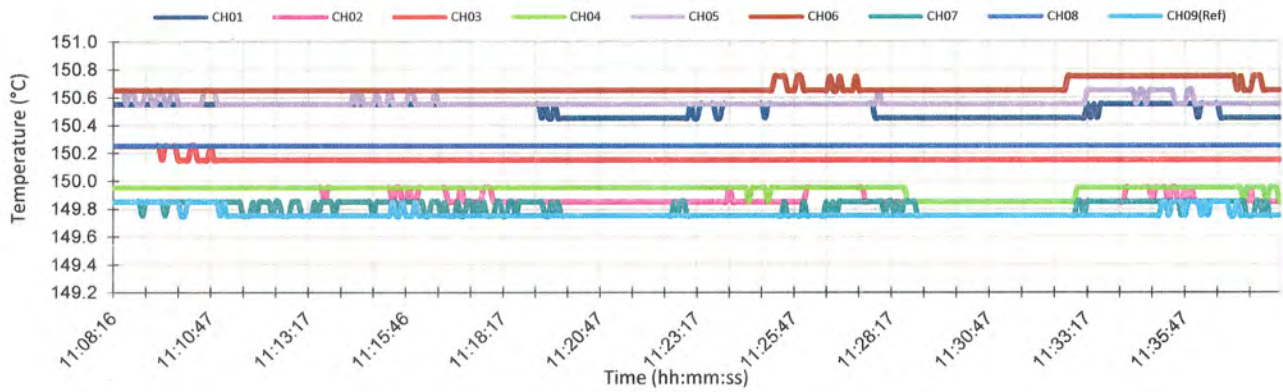

Approved Signatory : 

Packing List

Unit : K-446 Kjeldigester standard



151111112791000281006111

Serial Number 1000281006

Page 1(1)

Item	Pieces	Description		
11059833	1.0000	Packing parts Kjeldigester K-446/K-449 Beipackteile K-446/K-449		✓ OK
037377	5.0000	Sample tubes 300 ml (set of 4) Probengläser 300 ml (Set à 4 Stück)		✓ OK
11059754	1.0000	Rack 20 cpl. Rack 20 kpl.		✓ OK
11058955	1.0000	Aspiration device Kjeldigester K-446/K-449 cpl. Absaugeinheit K-446/K-449		✓ OK
040444	1.0000	Weighing boat 20pcs. Wägeschiffchen 20 Stk.		✓ OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V		✓ OK
11058825	1.0000	Fume collection tube with ball joint Dampfsammelrohr mit Kugelschliff		✓ OK
11592548	1.0000	Kjeldahl Practice Guide en Kjeldahl Practice Guide en		✓ OK
11593546	1.0000	Operation Manual K-446/K-449 english Bedienungsanleitung K-446/K-449 englisch		✓ OK
11593635	1.0000	Supplementary sheet Kjeldigester K-446/K-449 Beiblatt K-446/K-449		✓ OK

Packed by





BUCHI Certificate Final Test Inspection

Unit : BÜCHI KjeldDigester K-446

Serial number 1000281006

Examination Procedure

1. **Visual control of the glass parts and the unit**

✓ OK

- No scratches on the coated surface
- Mounted in accordance to the specific drawing

2. **Security tests**

✓ OK

- High voltage test in accordance with EN 61010-1 (IEC 1010)
- Ground connection test in accordance with EN 61010-1 (IEC 1010)

3. **Functional tests**

Operating panel

✓ OK

- All buttons are working
- Cooling system is working after the instrument has been switched on

Connector plugs

✓ OK

- Scrubber connector is working

Heating element

✓ OK

- Heating-up temperature 420 °C is reached after 40 minutes
- Temperature calibration at 420 °C (3 measuring points)

4. **Completeness of order checked**

✓ OK

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications

Packing List

Unit : K-415 TripleScrub 230V










151111112781000281005111

Serial Number

1000281005

Page 1(1)

Item	Pieces	Description		
11057332	1.0000	Tray for adsorption storage Ablage für Adsorption		✓ OK
048355	1.0000	Silicone hose D6/9 L=3m Silikonschlauch D6/9 L=3.0m		✓ OK
033701	1.0000	Glass wool 30g Glaswolle 30g		✓ OK
028737	2.0000	Hose clamp Anschlussklemme		✓ OK
11064971	1.0000	Activated Charcoal 2-6mm, 150g Aktivkohle 2-6mm, 150g		✓ OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V		✓ OK
11593505	1.0000	Operation Manual K-415 english Bedienungsanleitung K-415 english		✓ OK

Packed by





BUCHI Certificate Final Test Inspection

Unit : BÜCHI Scrubber K-415

Serial number 1000281005

Examination Procedure

1. **Visual control of the glass parts and the unit**

✓ OK

- No scratches or splinters on the glass parts
- Mounted in accordance to the specific drawing

2. **Security tests**

✓ OK

- High voltage test in accordance with EN 61010-1 (IEC 1010)
- Ground connection test in accordance with EN 61010-1 (IEC 1010)

3. **Functional tests**

Vacuum test

✓ OK


- Bypass valve open: Pressure is 0 - 65 mbar below the atmospheric pressure
- Bypass valve closed: Pressure is 400 mbar (+/- 10 %) below the atmospheric pressure

4. **Completeness of order checked**

✓ OK

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications





Packing List

Unit : K-360 Plastik Basic



151111113001000281014111

Serial Number

1000281014

Page 1(1)

Item	Pieces	Description		
043410	3.0000	Canister 10L thin-walled Kanister 10L dünnwandig		OK
043603	1.0000	Packing parts K-360 Beipackteile K-360		OK
047871	1.0000	Suppl. sheet distillation unit Beiblatt Distillation Unit		OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V		OK
11592548	1.0000	Kjeldahl Practice Guide en Kjeldahl Practice Guide en		OK
093176	1.0000	Operation Manual K-360 english Bedienungsanleitung K-360 englisch		OK

Packed by





BUCHI Certificate Final Test Inspection

Unit : BÜCHI BÜCHI Kjelflex K-360

Serial number 1000281014

Examination Procedure

1. **Visual control of the glass parts and the unit** ✓ OK

- No scratches on the coated surface or splinters on the glass parts
- Mounted in accordance to the specific drawing

2. **Security tests** ✓ OK

- High voltage test in accordance with EN 61010-1:2002 (IEC 61010-1, VDE 0411)
- Ground connection test in accordance with EN 61010-1:2002 (IEC 61010-1, VDE 0411)
- Safety door sensor checked

3. **Functional tests** ✓ OK
Electronics

- Electronic modul is tested with the checking device PG157
- Connector plugs are working

Operating panel ✓ OK

- Display is working
- All buttons of the keypad are working

Pump testing ✓ OK

- All pumps are working
- All pumps (exception: water pump of the steam generator) are precalibrated

Valve testing ✓ OK

- All valves are working

Steam generator testing ✓ OK

- The steam generator is filled with water
- The steam generator valve is working
- The amount of distillate corresponds to specifications

Further testing ✓ OK

- Beeper is working

4. **Unit configuration and completeness of order checked** ✓ OK

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications



Certificate of Calibration

Certificate No. : 66-400476-2

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Binder

Model : ED53

Range : N/A °C

Resolution : 1 °C

Serial No. : 13-07419

ID No. : MET-OV02/57

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (31.0 to 32.0) °C

Relative Humidity : (55 to 60) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 23 August 2023

Date of Calibration : 23 August 2023

Date of Issue : 23 August 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400030

66-400227-1

24 Oct 2023

National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400476-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

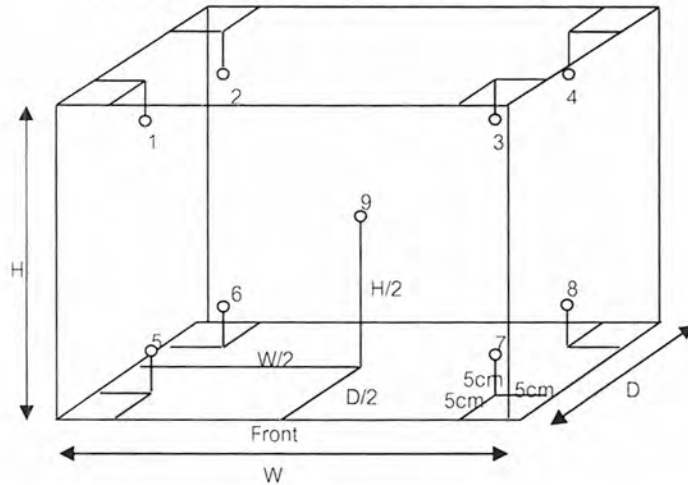

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
104	110	110	105.0	105.0	105.0	104.9	103.9	103.9	104.2	104.2	104.2	0.94
180	184	184	180.1	181.9	180.8	179.7	180.2	180.8	180.7	180.8	180.2	1.2

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
104	110	110	1.0	0.2	1.3
180	184	184	1.9	0.3	2.7

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-400424-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Memmert

Model : UM 100

Range : N/A °C

Resolution : 0.1 °C

Serial No. : b197.0985

ID No. : MET-OV01/46

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 10 August 2022

Date of Calibration : 10 August 2022

Date of Issue : 13 August 2022

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400032

65-400274-1

25 Nov 2022

National Institute of Metrology Thailand (NIMT)

Approved by :

(Bur

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-400424-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

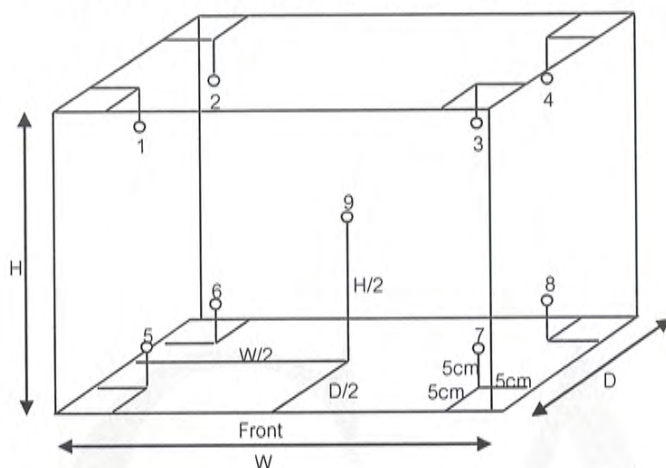

Inside of Chamber

W = 0.32 m

D = 0.18 m

H = 0.24 m

Capacity = 0.01 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
180.0	180.0	180.0	181.2	181.3	180.6	180.4	179.9	181.0	179.5	179.1	180.0	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
180.0	180.0	180.0	1.4	0.3	2.5

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-300143-9

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Measuring Pipette

Manufacturer : KIMAX

Capacity : 10 ml Graduation : 0.1 ml

ID No. : MET-MP10:04-64

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1001.6 mbar.

Date of Received : 09 March 2022

Date of Calibration : 15 March 2022

Date of Issue : 15 March 2022

Calibrated by : Wipa Tovadee

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241003	64-200354-2	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-300143-9

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 1.57 sec.

Nominal Volume (ml)	Measuring Volume (ml)
2	2.0572
5	5.0897
10	10.0529

Uncertainty of measurement with in \pm 0.0039 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 65-300144-4

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Buret

Manufacturer : Witeg

Class : A

Capacity : 10 ml

Graduation : 0.02 ml

ID No. : MET-MB-01/64

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1007.1 mbar.

Date of Received : 09 March 2022

Date of Calibration : 15 March 2022

Date of Issue : 15 March 2022

Calibrated by : Wipa Tovadee

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241003	64-200354-2	02 Jun 2022	National Institute of Metrology (Thailand) (NIMT)

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 65-300144-4

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 31.89 sec.

Nominal Volume (ml)	Measuring Volume (ml)
2	2.0091
5	5.0223
10	10.0425

Uncertainty of measurement with in \pm 0.0039 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-300123-4

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Burette

Manufacturer : TS

Class : A

Capacity : 10 ml

Graduation : 0.02 ml

ID No. : MET-BU10:02/64

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1015.1 mbar.

Date of Received : 02 March 2023

Date of Calibration : 09 March 2023

Date of Issue : 09 March 2023

Calibrated by : Arcerat Sombun


Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	65-200370-4	02 Jun 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-300123-4

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 36.97 sec.

Nominal Volume (ml)	Measuring Volume (ml)
2	2.0008
5	5.0035
10	10.0072

Uncertainty of measurement with in \pm 0.0039 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -

