

ภาคผนวกที่ 4

ใบรับรองการสอบเทียบเครื่องมือ

Certificate of Calibration

Certificate No. : 66-400476-4

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Refrigerator)

Manufacturer : Sanden Intercool

Model : YPR-068S

Range : N/A °C

Resolution : 1 °C

Serial No. : YPR0682S-140100003R

ID No. : MET-RE02/57

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (29.5 to 30.5) °C

Relative Humidity : (54 to 57) %

Line Voltage : (220.5 to 221.8) V

Date of Received : 23 August 2023

Date of Calibration : 23 August 2023

Date of Issue : 23 August 2023

Calibrated by : Bunjerd Masri

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400023

66-400184-1

03 Oct 2023

National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400476-4


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

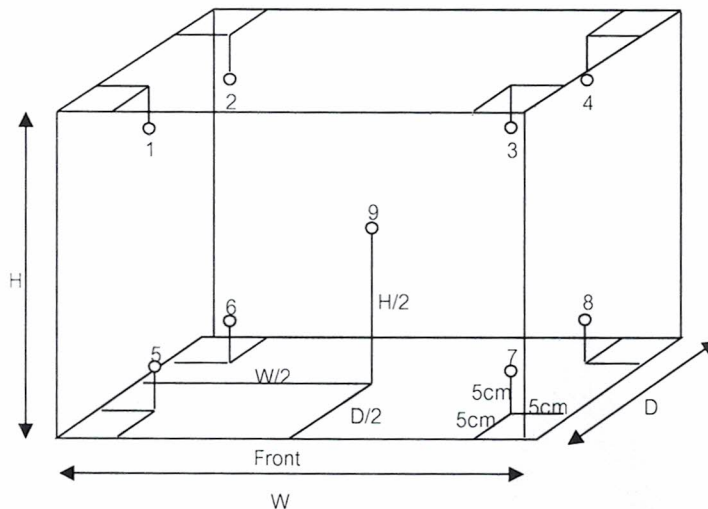

Inside of Chamber
 $W = 0.58 \text{ m}$
 $D = 0.60 \text{ m}$
 $H = 1.45 \text{ m}$
 $\text{Capacity} = 0.50 \text{ m}^3$

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
3	2	2	4.4	3.7	4.3	3.9	4.1	4.3	3.9	4.2	3.2	0.89

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
3	2	2	1.5	0.3	1.7

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

B



Certificate of Calibration

Certificate No. : 66-420023-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : pH Meter with electrode

pH meter

Manufacturer : Thermo Scientific Model : pH 150

Range : N/A pH Resolution : 0.01 pH

Serial No. : 2943538 ID No. : MET-PH06/63

Electrode

Model : N/A Serial No. : 66365

Environment : Ambient Temperature : $(25 \pm 2) ^\circ \text{C}$

Relative Humidity : $(50 \pm 15) \%$

Date of Received : 02 March 2023

Date of Calibration : 04 March 2023

Date of Issue : 04 March 2023

Calibrated by : Bunjerd Masri

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
440001	21E997	17 Mar 2023	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

<u>pH</u>	<u>Cert. No.</u>	<u>Lot No.</u>	<u>Exp. Date</u>	<u>Traceability</u>
4.008	61235182	857394	11 Dec 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61267169	857395	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61260481	857396	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-420023-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.4	0.1	0.060
	0.0000	7	7.00	-0.1	0.1	0.058
	-177.4800	10	10.00	-177.6	0.1	0.060

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-400476-5

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Incubator)
Manufacturer : M-LAB Model : BIC-140
Range : N/A °C Resolution : 0.1 °C
Serial No. : 240412 ID No. : MET-BI01/55

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (31.0 to 32.0) °C
Relative Humidity : (55 to 60) %
Line Voltage : (210.0 to 210.8) V

Date of Received : 23 August 2023

Date of Calibration : 23 August 2023

Date of Issue : 23 August 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400043	66-400226-1	27 Oct 2023	National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400476-5


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

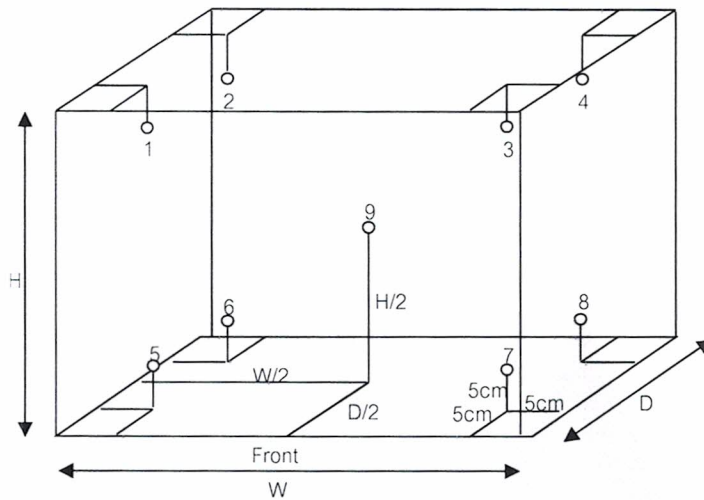

Inside of Chamber

W = 0.37 m

D = 0.33 m

H = 1.14 m

Capacity = 0.14 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	19.94	19.63	19.66	19.60	20.31	20.38	20.27	20.01	20.22	0.34

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.68	0.05	0.9

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-200067-1

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance
Manufacturer : METTLER TOLEDO Model : AG285
Serial No. : 1122140126 ID No. : MET-EB01/46
Capacity : 210 g Resolution : 0.00001g/81g, 0.0001g/210g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (26.4 to 26.8) °C
Relative Humidity : (54.9 to 58.8) %
Air Pressure : 1013.0 mbar

Date of Received : 02 March 2023

Date of Calibration : 02 March 2023

Date of Issue : 13 March 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-200067-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.01	0.00001	0.000020
0.1	0.00000	0.000019
1	-0.00002	0.000031
5	-0.00004	0.000043
10	-0.00008	0.000054
20	-0.00027	0.000071
50	-0.00059	0.00011
100	-0.0009	0.00023
150	-0.0012	0.00038
200	-0.0019	0.00040


This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.43$, providing a level of confidence of approximately 95%

Eccentric error Load test : 50 g

A	B	C	D	E
0.00055	0.00027	-0.00015	-0.00018	0.00000

g



Repeatability Load test : 200 g

Stdev. : 0.000053 g

- oOo -

Handwritten signature



Certificate of Calibration

Certificate No. : 66-400476-2

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)

Manufacturer : Binder

Model : ED53

Range : N/A °C

Resolution : 1 °C

Serial No. : 13-07419

ID No. : MET-OV02/57

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (31.0 to 32.0) °C

Relative Humidity : (55 to 60) %

Line Voltage : (210.0 to 210.8) V

Date of Received : 23 August 2023

Date of Calibration : 23 August 2023

Date of Issue : 23 August 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400030 66-400227-1

24 Oct 2023

National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400476-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

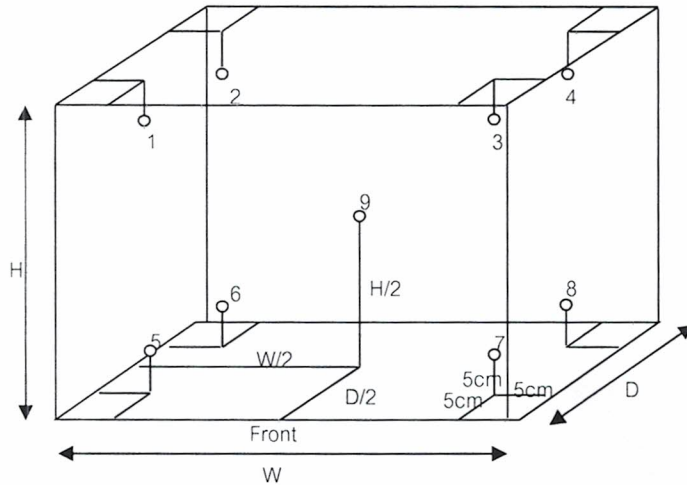

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.40 m

Capacity = 0.05 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
104	110	110	105.0	105.0	105.0	104.9	103.9	103.9	104.2	104.2	104.2	0.94
180	184	184	180.1	181.9	180.8	179.7	180.2	180.8	180.7	180.8	180.2	1.2

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
104	110	110	1.0	0.2	1.3
180	184	184	1.9	0.3	2.7

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-400476-1

Page : 1 of 2

Submitted by : M E T Company Limited
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Air Chamber (Oven)
Manufacturer : Memmert Model : UM 100
Range : N/A °C Resolution : 0.1 °C
Serial No. : b197.0985 ID No. : MET-OV01/46

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited
Ambient Temperature : (31.0 to 32.0) °C
Relative Humidity : (55 to 60) %
Line Voltage : (210.0 to 210.8) V

Date of Received : 23 August 2023

Date of Calibration : 23 August 2023

Date of Issue : 23 August 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400032	66-400228-1	25 Oct 2023	National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400476-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

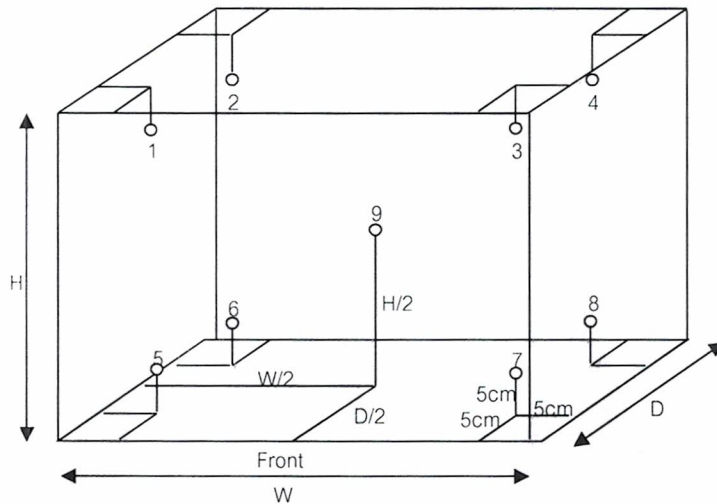

Inside of Chamber

W = 0.32 m

D = 0.18 m

H = 0.24 m

Capacity = 0.01 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
180.0	180.0	180.0	181.7	180.1	180.5	180.7	181.5	181.7	181.3	181.4	180.1	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
180.0	180.0	180.0	1.7	0.2	2.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Packing List

Unit : K-446 Kjeldigester standard



151111112791000281006111

Serial Number 1000281006

Page 1(1)

Item	Pieces	Description		
11059833	1.0000	Packing parts Kjeldigester K-446/K-449 Beipackteile K-446/K-449		✓ OK
037377	5.0000	Sample tubes 300 ml (set of 4) Probengläser 300 ml (Set à 4 Stück)		✓ OK
11059754	1.0000	Rack 20 cpl. Rack 20 kpl.		✓ OK
11058955	1.0000	Aspiration device Kjeldigester K-446/K-449 cpl. Absaugeinheit K-446/K-449		✓ OK
040444	1.0000	Weighing boat 20pcs. Wägeschiffchen 20 Stk.		✓ OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V		✓ OK
11058825	1.0000	Fume collection tube with ball joint Dampfsammelrohr mit Kugelschliff		✓ OK
11592548	1.0000	Kjeldahl Practice Guide en Kjeldahl Practice Guide en		✓ OK
11593546	1.0000	Operation Manual K-446/K-449 english Bedienungsanleitung K-446/K-449 englisch		✓ OK
11593635	1.0000	Supplementary sheet Kjeldigester K-446/K-449 Beiblatt K-446/K-449		✓ OK

Packed by





BUCHI Certificate Final Test Inspection

Unit : BÜCHI Kjeldigester K-446

Serial number 1000281006

Examination Procedure

1. **Visual control of the glass parts and the unit**

✓ OK

- No scratches on the coated surface
- Mounted in accordance to the specific drawing

2. **Security tests**

✓ OK

- High voltage test in accordance with EN 61010-1 (IEC 1010)
- Ground connection test in accordance with EN 61010-1 (IEC 1010)

3. **Functional tests**

Operating panel

✓ OK

- All buttons are working
- Cooling system is working after the instrument has been switched on

Connector plugs

✓ OK

- Scrubber connector is working

Heating element

✓ OK

- Heating-up temperature 420 °C is reached after 40 minutes
- Temperature calibration at 420 °C (3 measuring points)

4. **Completeness of order checked**

✓ OK

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications

H.-P. Gohn, Quality Manager

Signature, Date:

Packing List

Unit : K-415 TripleScrub 230V



151111112781000281005111

Serial Number

1000281005

Page 1(1)

Item	Pieces	Description		
11057332	1.0000	Tray for adsorption storage Ablage für Adsorption		✓ OK
048355	1.0000	Silicone hose D6/9 L=3m Silikonschlauch D6/9 L=3.0m		✓ OK
033701	1.0000	Glass wool 30g Glaswolle 30g		✓ OK
028737	2.0000	Hose clamp Anschlussklemme		✓ OK
11064971	1.0000	Activated Charcoal 2-6mm, 150g Aktivkohle 2-6mm, 150g		✓ OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V		✓ OK
11593505	1.0000	Operation Manual K-415 english Bedienungsanleitung K-415 englisch		✓ OK

Packed by

h. J. J.





BUCHI Certificate Final Test Inspection

Unit : BÜCHI Scrubber K-415

Serial number 1000281005

Examination Procedure

1. Visual control of the glass parts and the unit

✓ OK

- No scratches or splinters on the glass parts
- Mounted in accordance to the specific drawing

2. Security tests

✓ OK

- High voltage test in accordance with EN 61010-1 (IEC 1010)
- Ground connection test in accordance with EN 61010-1 (IEC 1010)

3. Functional tests

Vacuum test

✓ OK

- Bypass valve open: Pressure is 0 - 65 mbar below the atmospheric pressure
- Bypass valve closed: Pressure is 400 mbar (+/- 10 %) below the atmospheric pressure

4. Completeness of order checked

✓ OK

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications

H.-P. Gohn, Quality Manager

Signature, Date:

Wipfer 12.09.17

Packing List

Unit : K-360 Plastik Basic





151111113001000281014111

Serial Number

1000281014

Page 1(1)

Item	Pieces	Description		
043410	3.0000	Canister 10L thin-walled Kanister 10L dünnwandig		✓ OK
043603	1.0000	Packing parts K-360 Beipackteile K-360		✓ OK
047871	1.0000	Suppl. sheet distillation unit Beiblatt Distillation Unit		✓ OK
010020	1.0000	Power cable type USA, 3 pole 120V Anschlusskabel USA W 120V		✓ OK
11592548	1.0000	Kjeldahl Practice Guide en Kjeldahl Practice Guide en		✓ OK
093176	1.0000	Operation Manual K-360 english Bedienungsanleitung K-360 englisch		✓ OK

Packed by







BUCHI Certificate Final Test Inspection

Unit : BÜCHI BÜCHI Kjelflex K-360

Serial number 1000281014

Examination Procedure

1. **Visual control of the glass parts and the unit** ✓ OK

 - No scratches on the coated surface or splinters on the glass parts
 - Mounted in accordance to the specific drawing
2. **Security tests** ✓ OK

 - High voltage test in accordance with EN 61010-1:2002 (IEC 61010-1, VDE 0411)
 - Ground connection test in accordance with EN 61010-1:2002 (IEC 61010-1, VDE 0411)
 - Safety door sensor checked
3. **Functional tests** ✓ OK

Electronics

 - Electronic modul is tested with the checking device PG157
 - Connector plugs are working

Operating panel ✓ OK

 - Display is working
 - All buttons of the keypad are working

Pump testing ✓ OK

 - All pumps are working
 - All pumps (exception: water pump of the steam generator) are precalibrated

Valve testing ✓ OK

 - All valves are working

Steam generator testing ✓ OK

 - The steam generator is filled with water
 - The steam generator valve is working
 - The amount of distillate corresponds to specifications

Further testing ✓ OK

 - Beeper is working
4. **Unit configuration and completeness of order checked** ✓ OK

BÜCHI Labortechnik AG hereby declares that this unit is in accordance with the specifications

H.-P. Gohn, Quality Manager

Signature, Date: CS 12.09.17

Certificate of Calibration

Certificate No. : 66-300123-5

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Burette

Manufacturer : Witeg

Class : B

Capacity : 50 ml

Graduation : 0.1 ml

ID No. : MET-BU50:01/64

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1014.7 mbar.

Date of Received : 02 March 2023

Date of Calibration : 09 March 2023

Date of Issue : 09 March 2023

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	65-200370-4	02 Jun 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :



(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



www.calibratech.co.th

Certificate of Calibration

Certificate No. : 66-300123-5

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 25.30 sec.

Nominal Volume (ml)	Measuring Volume (ml)
10	10.0010
25	24.9818
50	49.9603

Uncertainty of measurement with in \pm 0.011 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -

D.



Certificate of Calibration

Certificate No. : 66-400013-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Liquid in Glass Thermometer

Manufacturer : SK

Model : N/A

Range : 0 °C to 100 °C

Resolution : 1 °C

Serial No. : N/A

Immersion : Total

ID No. : MET-TH09/20

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

Date of Received : 05 January 2023

Date of Calibration : 07 January to 10 January 2023

Date of Issue : 10 January 2023

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)
400004	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)

Approved by :



(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400013-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Ice point check : UUC* reading 0 °C Standard reading 0.8073 °C

Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
11.3107	10	1.3	0.31
50.6036	50	0.6	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

B



Certificate of Calibration

Certificate No. : 66-300003-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6 T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Volumetric Flask

Manufacturer : ISOLAB

Class : A

Capacity : 1000 ml

ID No. : MET:VF1000:02/61

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1012.0 mbar.

Date of Received : 05 January 2023

Date of Calibration : 13 January 2023

Date of Issue : 13 January 2023

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	65-200370-1	02 Jun 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :



(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-300003-1

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
1000	1000.55

Uncertainty of measurement with in \pm 0.14 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -

D.





MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : S2022090647-0002

Date Issued : 03-Oct-22

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment : Incubator

Manufacturer : BINDER

Model : BD 240

Serial No. : 12-17739

ID No./Tag No. : IN 04/56

Date Received : 30-Sep-22

Date Calibrated : 30-Sep-22

Calibrated by : Mr. Surat Aumarb

Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sarayuth T.
(Mr. Sarayuth Tochua)



Page 1 of 2

Certificate No. : S2022090647-0002

Environment : Ambient Temperature : Start record 26.3 °C, Stop record 26.5 °C
Relative Humidity : Start record 54.3 %RH, Stop record 54.6 %RH


Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability ¹ (°C)	Measured Uniformity ² (°C)	Overall Variation ³ (°C)
35	35.0	35.0	0.04	0.12	0.19

Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	STD No. 6 (°C)	STD No. 7 (°C)	STD No. 8 (°C)	STD No. 9 (°C)	Uncertainty ⁴ ±°C
35	34.81	34.79	34.80	34.83	34.90	34.89	34.89	34.87	34.90	0.18

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. 0

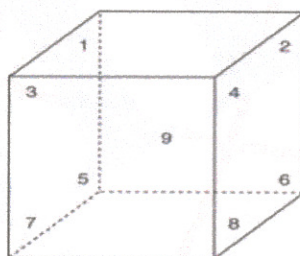

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. AD2207-125-0001 for Digital Thermometer with Probe (Agilent) Module 1 (73) NTC, Pt1000 Serial No. MY44024042, Due 01-Feb-23

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate