

ภาคผนวก ข.

เอกสารรับรองเครื่องมือการตรวจวัด

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Banggood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

NSG-TISI-TIS17025  
CALIBRATION 0030

## Certificate of Calibration

Certificate No. : 66-420087-1

Page : 1 of 2

Submitted by : M Green Group Co.,Ltd.

188/46 Wisatusukhakhon 25, Pracha-Utid Rd., Thungkru Bangkok 10140 Thailand

Equipment : pH Meter with electrode

pH meter

Manufacturer : Eutech

Model : pH 700

Range : N/A

pH

Resolution : 0.01 pH

Serial No. : 2884323

ID No. : N/A

Electrode

Model : N/A

Serial No. : 01X099320

Environment : On site calibration was carried out at the Laboratory, M Green Group Co.,Ltd.

Ambient Temperature : (25.0 to 25.5)°C

Relative Humidity : (45 to 50) %

Date of Received : 20 September 2023

Date of Calibration : 20 September 2023

Date of Issue : 25 September 2023

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No. Cert. No. Due Date Traceability

400005 SG-E-00307/66 23 Aug 2025 National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61270213	915161	19 Jul 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.985	61275614	898428	28 May 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	915163	19 Jul 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by

Laboratory Manager

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Banggood, Pakkred, Nonthaburi 11120

Tel (02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 66-420087-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage ( mV )	Nominal Value ( pH )	UUC Reading		Correction ( mV )	Uncertainty ( ± mV )
			( pH )	( mV )		
4, 7, 10	177.4800	4	4.00	177.5	0.0	0.12
	0.0000	7	7.00	0.1	-0.1	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer ( pH )	UUC Reading ( pH )	Correction ( pH )	Uncertainty ( ± pH )
4, 7, 10	4.008	4.01	0.00	0.010
	6.985	7.00	-0.01	0.011
	9.997	10.01	-0.01	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o O o -

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025  
CALIBRATION 0030

## Certificate of Calibration

Certificate No. : 66-400519-1 Page : 1 of 2

Submitted by : M Green Group Co.,Ltd.  
188/46 Wisatesukhakhon 25, Pracha-Utid Rd., Thungkru Bangkok 10140 Thailand

Equipment : Digital Thermometer with Thermistor probe  
Temperature Indicator

Manufacturer : Eutech Model : pH 700

Range : N/A °C Resolution : 0.1 °C

Serial No. : 2884323 ID No. : N/A

Thermistor probe

Model : N/A Sheath Material : Stainless

Diameter : 3.2 mm. Length : 100 mm.

Serial No. : PHSTEMB01P ID No. : N/A

Environment : On site calibration was carried out at the M Green Group Co.,Ltd.

Ambient Temperature : (25.0 to 26.0) °C

Relative Humidity : (56 to 60) %

Line Voltage : (224.0 to 225.2) VAC

Date of Received : 20 September 2023

Date of Calibration : 20 September 2023

Date of Issue : 25 September 2023

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003  
by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0074-22	20 Jun 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	22E569	22 Feb 2024	National Institute of Metrology Thailand (NIMT)

Approved

Laboratory Manager

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel (02) 964-6211 Fax (02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 66-400519 Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth ( mm. )	Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
100	25.006	24.9	0.1	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ ,  
providing a level of confidence of approximately 95%

- o0o -

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasam 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel (02) 964-6211 Fax (02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

NSC-TISI-TIS1/025  
CALIBRATION 0030

## Certificate of Calibration

Certificate No. : 66-200300-1 Page : 1 of 2

Submitted by : M Green Group Co., Ltd.  
188/46 Wisatesuknakhon 25, Pracha-Utid Rd., Thungkru, Bangkok 10140 ThailandEquipment : Electronic Balance  
Manufacturer : SHIMADZU Model : AP225WD  
Serial No. : D316300690  
Capacity : 220 g Resolution : 0.00001g/102g, 0.0001g/220gEnvironment : On site calibration was carried out at the Laboratory, M Green Group Co., Ltd.  
Ambient Temperature : (25.6 to 26.7) °C  
Relative Humidity : (54.4 to 56.6) %  
Air Pressure : 1010.0 mbar

Date of Received : 20 September 2023

Date of Calibration : 20 September 2023

Date of Issue : 22 September 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14  
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasam 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel (02) 964-6211 Fax (02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 66-200300-1 Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good


Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty ± (g)
0.001	0.00000	0.000012
0.01	0.00000	0.000013
0.1	0.00000	0.000015
1	0.00000	0.000026
10	0.00000	0.000053
20	-0.00003	0.000071
50	0.00004	0.00011
100	-0.00009	0.00020
150	0.00000	0.00038
200	-0.0001	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.15$ , providing a level of confidence of approximately 95%

Eccentric error	Load test : 50 g
A B C D E	
-0.00003 0.00000 0.00000 -0.00005 0.00000	g



Repeatability	Load test : 200 g
Stdev.	0.000048 g

- o O o -



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpoed, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax (02) 964-5155, e-mail calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

Certificate No. : 66-400531-1

Page : 1 of 2

Submitted by :

M Green Group Co., Ltd.

188/46 Wisatesuknakhon 25, Pracha-Utid Rd., Thungkru, Bangkok 10140 Thailand

Equipment :

Liquid in Glass Thermometer

Manufacturer : N/A

Model : N/A

Range : 0 °C to 100 °C

Resolution : 1 °C

Serial No. : N/A

Immersion : Total

ID No. : 94-49747

Environment :

Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

Date of Received :

21 September 2023

Date of Calibration :

23 September to 26 September 2023

Date of Issue :

26 September 2022

Calibrated by :

Chortip Samchusri

Calibration Method :

This instrument was calibrated by In-house method comparison technique CAL-M4001

based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments :

This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
--------	-----------	----------	--------------

400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)
--------	------------	-------------	---

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
--------	-----------	----------	--------------

400003	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)
--------	---------	-------------	---

400004	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)
--------	---------	-------------	---

Approv

Laboratory Manager

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpoed, Pakkred, Nonthaburi 11120

Tel (02) 964-6211 Fax (02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 66-400531-1

Page : 2 of 2

Result of Calibration :

Without Adjustment

UUC Condition As-Received : Good

Function :

Temperature measurement

Ice point check : UUC\* reading 0 °C Standard reading 0.0352 °C

Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
39.7228	40	-0.3	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 ,  
providing a level of confidence of approximately 95%

- oOo -

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-P0031-01



CAL-P0031-01



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel (02) 964-6211 Fax (02) 964-5155, e-mail calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025  
CALIBRATION 0030

## Certificate of Calibration

**Certificate No. :** 66-400520-1 **Page : 1 of 2**

**Submitted by :** M Green Group Co., Ltd.  
188/46 Wisatesukhakhon 25, Pracha-Utid Rd., Thungkru Bangkok 10140 Thailand

**Equipment :** Air Chamber (Refrigerator)  
**Manufacturer :** Biobase **Model :** BXC-V250M (II)  
**Range :** N/A °C **Resolution :** 0.1 °C  
**Serial No. :** YC025025190108 **ID No. :** N/A

**Environment :** On site calibration was carried out at the Laboratory, M Green Group Co., Ltd.  
**Ambient Temperature :** (25.0 to 26.0) °C  
**Relative Humidity :** (40 to 50) %  
**Line Voltage :** (226.0 to 230.0) V

**Date of Received :** 20 September 2023  
**Date of Calibration :** 20 September 2023  
**Date of Issue :** 25 September 2023  
**Calibrated by :** Pernipon Chanpu  
**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400042	66-400453-1	31 Jan 2024	National Institute of Metrology Thailand (NIMT)

Approved by

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

**Certificate No. :** 66-400520-1


**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

This instrument was setting air ventilation at position 0 (close)

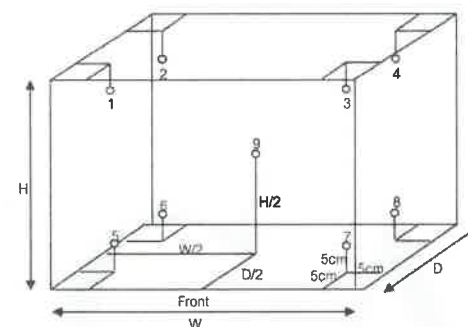

Inside of Chamber

W = 0.50 m

D = 0.40 m

H = 1.20 m

Capacity = 0.24 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
4.0	2.0	2.0	4.05	4.04	4.27	4.89	4.10	4.05	4.92	4.37	4.43	0.46

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
4.0	2.0	2.0	0.60	0.21	1.2

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax (02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

NSC-TISI-TIS 17025  
CALIBRATION 0030

## Certificate of Calibration

Certificate No. : 66-400520-2

Page : 1 of 2

Submitted by :

M Green Group Co., Ltd.

188/46 Wisatesukhakhon 25, Pracha-Uttd Rd., Thungkru Bangkok 10140 Thailand

Equipment :

Air Chamber (Oven)

Manufacturer : Memmert

Model : UF110

Range : N/A °C

Resolution : 0.1 °C

Serial No. : B419.1092

ID No. : N/A

Environment :

On site calibration was carried out at the Laboratory, M Green Group Co., Ltd.

Ambient Temperature : (25.0 to 26.0) °C

Relative Humidity : (40 to 50) %

Line Voltage : (226.0 to 230.0) V

Date of Received :

20 September 2023

Date of Calibration :

20 September 2023

Date of Issue :

25 September 2023

Calibrated by :

Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.

Cert. No.

Due Date

Traceability

400046 &amp; 400028

66-400184-3

04 Oct 2023

National Institute of Metrology Thailand (NIMT)

Approved

Laboratory Manager

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax (02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 66-400520-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

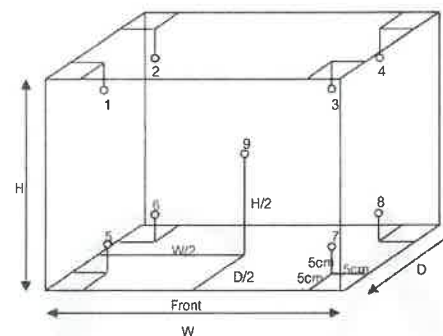

Inside of Chamber

W = 0.56 m

D = 0.40 m

H = 0.48 m

Capacity = 0.11 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
103.0	103.0	103.0	103.3	103.0	103.7	103.3	103.1	103.0	103.8	102.7	103.3	0.69
105.0	105.0	105.0	105.3	105.0	105.7	105.3	105.2	105.0	105.8	104.6	105.3	0.71
180.0	180.0	180.0	180.4	180.1	181.2	180.4	180.3	180.0	181.4	179.0	180.5	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
103.0	103.0	103.0	0.8	0.1	1.3
105.0	105.0	105.0	0.9	0.1	1.4
180.0	180.0	180.0	1.7	0.2	2.7

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

- o0o -

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd



CAL-P0031-01



CAL-P0031-01

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

NSC-TISI-TIS17025  
CALIBRATION 0030

## Certificate of Calibration

Certificate No. : 66-400520-3

Page : 1 of 2

Submitted by :

M Green Group Co., Ltd.

188/46 Wisatesukhakhon 25, Pracha-Utid Rd., Thungkru Bangkok 10140 Thailand

Equipment :

Water Bath

Manufacturer : Memmert

Model : WNB29

Range : N/A °C

Resolution : 0.1 °C

Serial No. : L619.0037

ID No. : N/A

Environment :

On site calibration was carried out at the Laboratory, M Green Group Co., Ltd.

Ambient Temperature : (25.0 to 26.0) °C

Relative Humidity : (40 to 50) %

Line Voltage : (226.0 to 230.0) V

Date of Received :

20 September 2023

Date of Calibration :

20 September 2023

Date of Issue :

25 September 2023

Calibrated by :

Penphon Chanpu

Calibration Method :

This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80

The temperature scale used was based on ITS-90

Reference Standard Instruments :

This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD probe

ID No.

Cert. No.

Due Date

Traceability

400046 &amp; 400024

66-400184-2

06 Oct 2023

National Institute of Metrology Thailand (NIMT)

Approved

Laboratory Manager

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax (02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration


Certificate No. : 66-400520-3

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

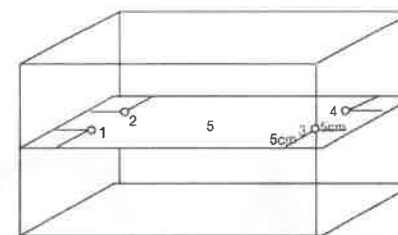

Front

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @					Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)
			Sensor No.							
			1	2	3	4	5			
85.0	85.0	85.0	85.08	85.04	84.98	85.17	85.02	0.18	0.2	0.05

**Remark** The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

- o0o -

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co., Ltd.





# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025  
CALIBRATION 0030

## Certificate of Calibration

Certificate No. : 66-400520-4

Page : 1 of 2

Submitted by : M Green Group Co., Ltd.

188/46 Wisatesukhakhon 25, Pracha-Uttd Rd., Thungkru Bangkok 10140 Thailand

Equipment : Air Chamber (Incubator)

Manufacturer : Biobase

Model : Biochemistry Incubator

Range : 0 °C to 65 °C

Resolution : 0.1 °C

Serial No. : KYP1502202003

ID No. : N/A

Environment : On site calibration was carried out at the Laboratory, M Green Group Co., Ltd.

Ambient Temperature : (25.0 to 25.5) °C

Relative Humidity : (45 to 50) %

Line Voltage : (226.0 to 230.0) V

Date of Received : 20 September 2023

Date of Calibration : 20 September 2023

Date of Issue : 25 September 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD Probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400043 66-400226-1

27 Oct 2023

National Institute of Metrology Thailand (NIMT)

Approved

Laboratory Manager

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 66-400520-4


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

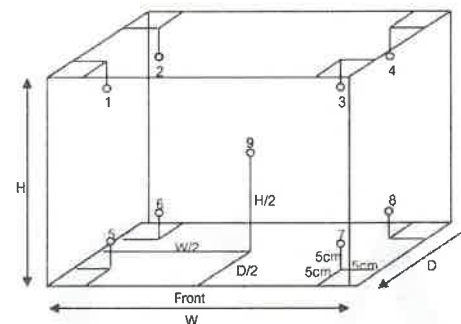

Inside of Chamber

W = 0.45 m

D = 0.41 m

H = 0.85 m

Capacity = 0.16 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	20.14	20.04	19.91	19.97	20.03	19.96	19.91	19.96	19.92	0.70

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.28	0.37	0.8

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

- o0o -

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co., Ltd.



CAL-P0033-03



CAL-P0033-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax (02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025  
CALIBRATION 0030

## Certificate of Calibration

**Certificate No.** : 66-300589-7

**Page** : 1 of 2

**Submitted by** : M Green Group Co., Ltd.

188/46 Wisatesuknakhon 25, Pracha-Utid Rd., Thungkru, Bangkok 10140 Thailand

**Equipment** : Burette

Manufacturer : GLASSCO

Class : A

Capacity : 10 ml

Graduation : 0.05 ml

ID No. : 2212-0344-1

**Environment** : Ambient Temperature :  $(20 \pm 3)$  °C

Relative Humidity :  $(50 \pm 10)$  %

Air Pressure : 1006.7 mbar.

**Date of Received** : 20 September 2023

**Date of Calibration** : 27 September 2023

**Date of Issue** : 27 September 2023

**Calibrated by** : Wipa Tovadee

**Calibration Method** : In-house method CAL-M3001 based on ASTM E 542-01

**Reference Standard Instruments** : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241003	66-200196-2	02 Dec 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :

Supervisor

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel (02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

**Certificate No.** : 66-300589-7

**Page** : 2 of 2

**Result of Calibration** : This result of true Volume is referred to standard temperature at 20 °C

**UUC Condition As-Received** : Good

Delivery Time : 21.33 sec.

Nominal Volume ( ml )	Measuring Volume ( ml )
10	9.9913

Uncertainty of measurement with in  $\pm$  0.0039 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.00$ ,  
providing a level of confidence of approximately 95%

- o0o -

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

**Certificate No.** : 66-300589-8

**Page** : 1 of 2

**Submitted by** : M Green Group Co., Ltd.

188/46 Wisetusuknakhon 25, Pracha-Uttd Rd., Thungkru, Bangkok 10140 Thailand

**Equipment** : Burette

Manufacturer : GLASSCO

Class : A

Capacity : 25 ml

Graduation : 0.1 ml

ID No. : 2212-0344-2

**Environment** : Ambient Temperature :  $(20 \pm 3)$  °C

Relative Humidity :  $(50 \pm 10)$  %

Air Pressure : 1006.7 mbar.

**Date of Received** : 20 September 2023

**Date of Calibration** : 27 September 2023

**Date of Issue** : 27 September 2023

**Calibrated by** : Wipa Tovadee

**Calibration Method** : In-house method CAL-M3001 based on ASTM E 542-01

**Reference Standard Instruments** : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241003	66-200196-2	02 Dec 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :

Supervisor

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel (02) 964-6211 Fax (02) 964-5155, e-mail calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

**Certificate No.** : 66-300589-8

**Page** : 2 of 2

**Result of Calibration** : This result of true Volume is referred to standard temperature at 20 °C

**UUC Condition As-Received** : Good

Delivery Time : 46.01 sec.

Nominal Volume ( ml )	Measuring Volume ( ml )
25	24.9741

Uncertainty of measurement with in  $\pm$  0.0066 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.00$ , providing a level of confidence of approximately 95%

- oOo -

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd



CAL-P0031-03



CAL-P0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech\_cal@yahoo.com, calibratech\_cal@hotmail.com

## Certificate of Calibration

**Certificate No.** : 66-300590-1

**Page** : 1 of 2

**Submitted by** : M Green Group Co., Ltd.

188/46 Wisatesuknakhon 25, Pracha-Uttd Rd., Thungkru, Bangkok 10140 Thailand

**Equipment** : Imhoff Cone

**Manufacturer** : VITLAB

**Capacity** : 1000 ml **Graduation** : 50 ml

**ID No.** : CY1000/01/22

**Environment** : Ambient Temperature :  $(20 \pm 3)$  °C

Relative Humidity :  $(50 \pm 10)$  %

Air Pressure : 1005.4 mbar.

**Date of Received** : 20 September 2023

**Date of Calibration** : 26 September 2023

**Date of Issue** : 26 September 2023

**Calibrated by** : Arcerat Sombun

**Calibration Method** : In-house method CAL-M3001 based on ASTM E 542-01

**Reference Standard Instruments** : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	66-200196-1	02 Dec 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-01

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech\_cal@yahoo.com, calibratech\_cal@hotmail.com

## Certificate of Calibration

**Certificate No.** : 66-300590-1

**Page** : 2 of 2

**Result of Calibration** : This result of true Volume is referred to standard temperature at 20 °C

**UUC Condition As-Received** : Good

Nominal Volume ( ml )	Measuring Volume ( ml )
500	501.19
1000	1010.67

Uncertainty of measurement with in  $\pm$  0.17 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.00$ , providing a level of confidence of approximately 95%

- o0o -



CAL-F0031-01



การดูแลบำรุงรักษาเชิงป้องกัน

Preventive Maintenance



ซ15

ใบรับรองการทวนสอบ “เครื่องกลั่นไนโตรเจน”

(Calibration Certificate of Distillation Unit VAPODEST

VAP20, VAP30s)



บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

ฝ่ายบริการหลังการขาย

โทร 0 2 639 7000 E-mail: [service.tech.th@dksh.com](mailto:service.tech.th@dksh.com)

ฝ่ายขายและการตลาด

โทร 0 2 639 7000 E-Mail : [marketing.tech.th@dksh.com](mailto:marketing.tech.th@dksh.com)

Website : [www.dksh.co.th/technology/scientific-thailand](http://www.dksh.co.th/technology/scientific-thailand)

## เงื่อนไขการให้บริการ Preventive Maintenance

บริษัทฯ จะส่งวิศวกรผู้ชำนาญ เพื่อให้บริการตามขอบข่ายของการบริการ เฉพาะ ในวันและเวลา ราชการ หากมีความประสงค์ที่จะรับบริการนอกเหนือจากวัน เวลา ราชการ (วันหยุดเสาร์ – อาทิตย์ หรือวันหยุด นักชดถุณ) บริษัทฯ จะคิดค่าบริการเพิ่มเติมตามอัตราที่กฎหมายแรงงานกำหนดไว้

### ขอบข่ายการบริการ

- ตรวจสอบสภาพการทำงานต่าง ๆ ของเครื่องมือ
- ทดสอบประสิทธิภาพการทำงาน of เครื่องมือ
- รายการผลการตรวจสอบเครื่องมือ

### หมายเหตุ

- ราคารันไม่รวมถึงค่าบริการซ่อม หรือ เปลี่ยนอะไหล่ที่ชำรุดเสียหาย หรือหมดสภาพการใช้งาน
- ในกรณีที่ผู้รับบริการอยู่นอกเขตพื้นที่ให้บริการ บริษัทฯ จำเป็นต้องคิดค่าใช้จ่ายเพิ่มเติม ได้แก่ ค่าเดินทาง เป็นต้น
- บริษัทฯ ขอสงวนสิทธิ์ในการเปลี่ยนแปลงราคา โดยไม่แจ้งให้ทราบล่วงหน้า

## ช่องทางการติดต่อ



DKSH Technology Limited (บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด)  
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260  
เลขประจำตัวผู้เสียภาษี 010-555-001-4547 (สำนักงานใหญ่)



LINE: @dkshscientific



Call center 0 2 639 7000



DKSH Scientific



[www.dksh.com/scientific-thailand](http://www.dksh.com/scientific-thailand)



[marketing.th@dksh.com](mailto:marketing.th@dksh.com)



@dkshscientific

# Preventive Maintenance Contract

จำนวนในการทำสัญญาบริการ ..... ครั้ง ต่อ ปี  
ครั้งที่ 1/1 วันที่ ..... 28 Mar. 2023 .....

## รายละเอียดผู้รับบริการ

หน่วยงาน	บริษัท เทสท์ เทคโนโลยี จำกัด		
ที่อยู่	30,32 ซอยพระรามที่ 2 ซอย 63 ถนนพระรามที่ 2 แขวงสามชัย เขตบางขุนเทียน กรุงเทพมหานคร 10150		
โทรศัพท์	0-2893-4211-7	แฟกซ์	0-2893-4218

## ผู้ติดต่อ

ชื่อ - นามสกุล	คุณมริสา วิเศษสังข์		
ตำแหน่ง	หัวหน้าส่วน		
โทรศัพท์	0-2893-4211-7	เบอร์ตอ	แฟกซ์ 0-2893-4218
E-mail	Lab_center@testtech.co.th		

## รายละเอียดผู้ให้บริการ

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด (ฝ่ายบริการหลังการขาย) (สำนักงานใหญ่)	
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260	
โทรศัพท์ 0 2 693 7000 Email: siriporn.sy@dksh.com Line ID : siripon3007	
เจ้าหน้าที่ประสานงาน : คุณศิริพร อู่ทองจ้อย โทรศัพท์ 090 678 6924 , 02 301 7467	
เจ้าหน้าที่ผู้ให้บริการ	นายจิรายุส สกลอด
ตำแหน่ง	Specialist, Technical Service.
โทรศัพท์	0938138736 แฟกซ์ -
E-mail	Jirayut.js@dksh.com


ลงนามผู้รับบริการ		ลงนามผู้ให้บริการ	
ตัวบรรจง	(.....)	ตัวบรรจง	
ตำแหน่ง		ตำแหน่ง	Specialist, Technical Service
วันที่ / ประทับตราบริษัท		วันที่ / ประทับตราบริษัท	28/3/2023

JOB No: Lep/2302591..... MODEL: Vap30..... S/N: 003718.....

## Part : Operational Qualification (OQ)


ตรวจสอบสภาพเครื่อง

FRONT

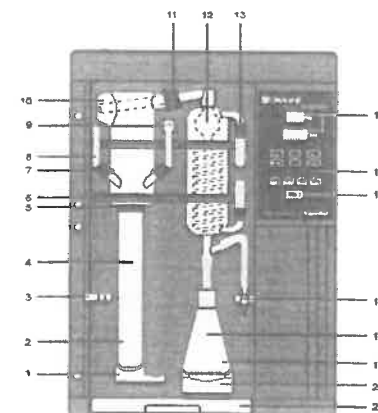

	Pass	Fail	N/A	Remark
1. Quick clamping device with wedge	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
2. Kjeldatherm digestion tube	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
3. Holder for steam inlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
4. PTFP-Inlet tubing, steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
5. Viton-cone	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
6. Clamping for glassware	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
7. Screw cap GL18 with silicone seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
8. PTFP-Inlet tubing, NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
9. PP-Distributor with PP-threaded joint	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
10. Distribution head, glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
11. Screw cap GL32 with silicone seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
12. Distillation condenser	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
13. Screw cap GL14 with plastic screw connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
14. Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
15. Keyboard, chemical-resistant	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
16. Main switch, green	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
17. Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
18. Distillate outlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
19. Erlenmeyer flask	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
20. Platform	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
21. Drip tray	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....

REAR

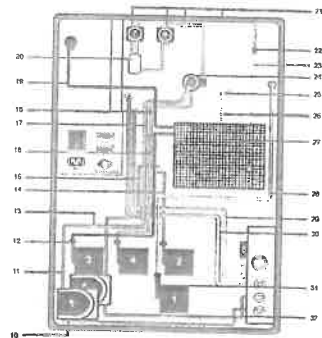

	Pass	Fail	N/A	Remark
1. Diaphragm pump NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
2. Diaphragm pump H <sub>3</sub> BO <sub>3</sub>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
3. Diaphragm pump H <sub>2</sub> O for steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
4. Diaphragm pump H <sub>2</sub> O for sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
5. Peristaltic pump for suction sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
6. Peristaltic pump for suction receiver	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option
7. Pinch-solenoid valve, steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
8. Magnetic valve with pressure control	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
9. Pinch-solenoid valve, shut-off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
10. Verprene-tubing 4x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
11. Verprene-tubing 4x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
12. Non-return valve for diaphragm pumps	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
13. Tubing reduction PP 51x10x5 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
14. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
15. Silicone tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option
16. Silicone -tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
17. Verprene-tubing 8x12 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
18. Verprene tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
19. Silicone tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
20. Ventilation glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
21. Novoprene-tubing 4.8x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
22. Tubing reduction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
23. Silicone tubing 6x10 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
24. PP-distributor with PP-thread	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
25. SKT-valve (built in with brass fitting)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
26. Silicone tubing 8x16x80 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
27. Steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
28. PTFE-inlet tubing NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
29. Silicone tubing 8x16 for cooling water inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
30. Silicone tubing 8x16 for cooling water outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
31. Viton-tubing 6x12*50 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
32. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option

## รายละเอียดการตรวจสอบ

### ขั้นตอนการบริการ

#### ตรวจสอบระบบไฟฟ้า (Electrical Test)

- ความต้านทานทางไฟฟ้าของเครื่องกับกราวด์
- กระแสไฟฟ้าที่ใช้งาน

#### ตรวจสอบสภาพเครื่อง (Optical Test)

- Main cable
- Electric wiring
- Pumps
- Distribution Head
- Condensor
- Steam generator
- Tubing
- Viton cone

#### ตรวจสอบ Function การทำงาน (The Function Test)

- ระบบสร้างและควบคุมความดันของ Steam
- ระบบการเติมน้ำเข้า Sample Tube
- ระบบการเติม Na OH
- ระบบการ Suction ตั้ง Sample Tube และ Receiver



รายงานผลการให้บิกร

1. TECHNICAL DATA

	Pass	Fail	N/A	Remark
Main Supply 220 volt + 10% 50 Hz with ground	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Nominal current	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	..... 6 a
1.1 COOLING WATER BATH	Pass	Fail	N/A	Remark
Temperature 15-20 °C	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Control Temperature	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....

1.2 OPTICAL TEST VAP..30..

	Pass	Fail	N/A	Remark
Screw cap GL14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Screw cap GL18	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Screw cap GL32	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Distillation Head	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Condensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Viton Cone	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Ventilation Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Micro Switch Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....

2.SYSTEM COOLING WATER INLET

	Pass	Fail	N/A	Remark
Cooling Water Inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Magnetic valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....

3.SYSTEM CONTROL

	Pass	Fail	N/A	Remark
Key Board	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Program	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Adding H <sub>2</sub> O	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
Adding NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Adding H <sub>2</sub> BO <sub>3</sub>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
Suction Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only

4.SYSTEM DISTILLATION

	Pass	Fail	N/A	Remark
Boiler	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Level Sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Novoprene-Tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Solenoid Valve Shut-Off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Solenoid Valve Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Excess Pressure Detector	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Ventilation Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Heater	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....

5. PUMP

	Pass	Fail	N/A	Remark
Pump H <sub>2</sub> O Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Pump H <sub>2</sub> O Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Pump NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Pump H <sub>3</sub> BO <sub>3</sub>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
- Non-Return Valve	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
Pump Suction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....

6. The Following Program Run :

	Pass	Fail	N/A	Remark
Addition H <sub>2</sub> O 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Addition NaOH 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Addition H <sub>2</sub> BO <sub>3</sub> 0-99 sec.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	.....
Reaction Time 0-99 min.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Distillation Time 0-99 min	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Steam Capacity 30%-100%	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
Suction Time 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....
The Instrument is in perfect technical shape	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	.....

Remark :

.....

.....

Part : ข้อมูลสนับสนุนด้านเทคนิค (General Technical Support)

การบำรุงรักษาทั่วไป (Basic maintenance)

### Cleaning

Glass parts and suction pump should be cleaned before long periods of non-usage (i.e. holidays). This way blockages caused by crystalline deposits are avoided.

The following program should be run:

Addition $H_2BO_3$	0	s
Addition $H_2O$ :	13	s
Addition NaOH:	0	s
Reaction time:	0	s
Distillation time:	7	min.
Steam capacity:	100	%
Suction time:	20	s

Place an empty digestion tube and an Erlenmeyer flask into position, and start the program.

In case of extreme deposits in the glassware you can clean the system by putting about 10 ml of sulphuric acid into the digestion tube.

### Error Code

The micro-processor continually surveys all the functions of the distillation system. As soon as an error arises it is shown on the display and accompanied by an acoustic signal.

Error message	Measures
No tap water	Check cooling water inlet for blockages. Ensure the tap is turned on
No sample tube	Insert tube
Check chemicals	Check set of tanks
Low water Press Enter	Check the water inlet distilled $H_2O$
Filling Steam generator	This message disappears as soon as steam generator is filled

After the above mentioned errors are corrected, the following message is displayed.

Error message	Measures
Stop Prog. No. x Continue=Enter	Enter=continue of interrupted program Reset=Standby-mode

### Other error messages

Error message	Measures
Wait for steam	Message disappears as soon as stand-by is reached
Add sol. > 1min Continue=Enter	Check programming Enter=continue of interrupted program Reset=Standby-mode
Program undefined	Check programming
Excess steam pressure	Switch the system off and call service
Sensor error	Switch the system off and call service



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com




CERTIFICATE No : 23T1387  
REFERENCE No : 68174-5

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 110  
SERIAL No : D415.0802  
ID No : EQL-190  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.  
CALIBRATION DATE : 13-Feb-23

APPROVED BY : 

ISSUED DATE : 14-Feb-23

RECEIVED DATE : 13-Feb-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23T1387

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 110  
ID No : EQL-190  
RECEIVED DATE : 13-Feb-23  
AMBIENT TEMPERATURE : 24 °C ± 1 °C  
S/N : D415.0802  
CALIBRATION DATE : 13-Feb-23  
RELATIVE HUMIDITY : 50 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	6635300	22T7509	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT



FRONT

### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 5  
Overall Line Voltage (V) variation : 8  
Instrument Condition : Normal  
Chamber Size (W\*L\*H): 56\*40\*48 cm

### CHAMBER PERFORMANCE

Calibration Point (°C)	Controller Temperature (°C)	Indicating Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
37.0	37.0	37.0	36.93	0.07	0.16	0.26
44.0	44.0	44.0	44.17	0.07	0.22	0.27

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
37.0	37.0	36.97	36.95	36.94	36.96	36.94	36.92	36.91	36.90	36.84	0.25
44.0	44.0	44.21	44.23	44.09	44.23	44.23	44.13	44.21	44.15	44.07	0.36

NOTE 1: THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

F-G010 REV : 02



CERTIFICATE No : 23T1386  
REFERENCE No : 68174-4

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 160  
SERIAL No : D518.0082  
No : EQL-205  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.  
CALIBRATION DATE : 13-Feb-23

APPROVED BY : 

ISSUED DATE : 14-Feb-23

RECEIVED DATE : 13-Feb-23



CERTIFICATE No : 23T1386

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 160  
ID No : EQL-205  
RECEIVED DATE : 13-Feb-23  
AMBIENT TEMPERATURE : 24 °C ± 1 °C  
S/N : D518.0082  
CALIBRATION DATE : 13-Feb-23  
RELATIVE HUMIDITY : 50 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

### 2-REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	6635300	22T7509	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT



FRONT

### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 2
Overall Line Voltage (V) variation : 9
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*72 cm

### CHAMBER PERFORMANCE

Calibration Point (°C)	Controller Temperature (°C)	Indicating Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35.0	35.0	35.0	34.99	0.02	0.14	0.20
36.0	36.0	36.0	36.00	0.03	0.14	0.22
41.5	41.5	41.5	41.46	0.05	0.10	0.19

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
35.0	35.0	34.91	34.94	34.93	34.93	34.98	35.03	35.08	35.01	35.08	0.25
36.0	36.0	35.93	35.95	35.95	35.94	36.00	36.05	36.10	36.01	36.10	0.25
41.5	41.5	41.46	41.47	41.41	41.47	41.50	41.47	41.45	41.43	41.49	0.36

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com



CERTIFICATE No : 23T1385  
REFERENCE No : 68174-3

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 160  
SERIAL No : D518.0240  
ID No : EQL-218  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.  
CALIBRATION DATE : 13-Feb-23

APPROVED BY : 

ISSUED DATE : 14-Feb-23

RECEIVED DATE : 13-Feb-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23T1385

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 160  
ID No : EQL-218  
RECEIVED DATE : 13-Feb-23  
AMBIENT TEMPERATURE : 24 °C ± 1 °C  
S/N : D518.0240  
CALIBRATION DATE : 13-Feb-23  
RELATIVE HUMIDITY : 50 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

### REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2633A	6633300	22T7509	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT



FRONT

### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 2  
Overall Line Voltage (V) variation : 12  
Instrument Condition : Normal  
Chamber Size (W\*L\*H): 56\*40\*72 cm

### CHAMBER PERFORMANCE

Calibration Point (°C)	Controller Temperature (°C)	Indicating Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35.0	35.0	35.0	35.00	0.05	0.15	0.26
36.0	36.0	36.0	36.00	0.04	0.16	0.26

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
35.0	35.0	34.94	34.98	34.93	34.97	35.07	35.10	34.94	35.04	35.05	0.25
36.0	36.0	35.94	35.97	35.92	35.96	36.07	36.11	35.95	36.05	36.05	0.25


NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



F-G010 REV : 02



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com



CERTIFICATE No : 23T1384  
REFERENCE No : 68174-2

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 160  
SERIAL No : D519.0140  
ID No : EQL-231  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.  
CALIBRATION DATE : 13-Feb-23

APPROVED BY :   
ISSUED DATE : 14-Feb-23  
RECEIVED DATE : 13-Feb-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23T1384

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : INCUBATOR  
MANUFACTURER : MEMMERT  
MODEL : IF 160  
ID No : EQL-231  
RECEIVED DATE : 13-Feb-23  
AMBIENT TEMPERATURE : 24 °C ± 1 °C  
S/N : D519.0140  
CALIBRATION DATE : 13-Feb-23  
RELATIVE HUMIDITY : 50 %RH ± 10 %RH


### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	6633300	22T7509	10-Jul-23
3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.				
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.				
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:- - NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.				

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT



FRONT

### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 2
Overall Line Voltage (V) variation : 8
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*72 cm

### CHAMBER PERFORMANCE

Calibration Point (°C)	Controller Temperature (°C)	Indicating Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35.0	35.0	35.0	35.03	0.08	0.17	0.32
37.0	37.0	37.0	37.02	0.08	0.22	0.32
41.5	41.5	41.5	41.54	0.04	0.13	0.20

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
35.0	35.0	34.92	35.02	34.99	35.01	35.04	35.03	35.06	35.09	35.10	0.25
37.0	37.0	37.00	36.99	36.95	36.95	37.00	37.02	37.09	37.07	37.11	0.25
41.5	41.5	41.52	41.51	41.47	41.49	41.54	41.53	41.62	41.58	41.56	0.36

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

F-G010 REV : 02



CERTIFICATE No : 23T1391  
REFERENCE No : 68175-1

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : AUTOCLAVE  
MANUFACTURER : HIRAYAMA  
MODEL : HVE-50  
SERIAL No : 30612085166  
No : EQL-155  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD.,  
SAMAEDAM, BANGKHUNTHIAN, BANGKOK  
10150

CALIBRATED BY : PRASERT P.  
CALIBRATION DATE : 13-Feb-23

APPROVED BY : [Redacted]

ISSUED DATE : 14-Feb-23

RECEIVED DATE : 13-Feb-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02



CERTIFICATE No : 23T1391

PAGE : 2 OF 2

## Calibration Report


EQUIPMENT : AUTOCLAVE  
MANUFACTURER : HIRAYAMA  
ID NUMBER : EQL-155  
RECEIVED DATE : 13-Feb-23  
AMBIENT TEMPERATURE : 30° C ± 1° C  
MODEL : HVE-50  
SERIAL NUMBER : 30612085166  
CALIBRATION DATE : 13-Feb-23  
RELATIVE HUMIDITY : 50 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

- THIS INSTRUMENT WAS CALIBRATED BASED ON BS 2646 : Part 5 : 1993 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON FIVE LOCATIONS AS SHOWN IN THE PICTURE. TWO PROBES WERE PLACES NEAR TOP AND BOTTOM WALL AND EACH PROBE WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE THIRD PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE INSTRUMENT CHAMBER. PROBE NUMBER 4 WAS ATTACHED TO THE LOAD TEMPERATURE PROBE, IF FITTED, WITHIN 20 mm OF ITS TIP. PROBE NUMBER 5 WAS PLACED IN THE CHAMBER DRAIN OR VENT WITHIN 100 mm OF ITS CONNECTION TO THE CHAMBER.
- REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER	VALPROBE	S350, DV35, DN94	23T0885	27-Jan-24
3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.				
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.				
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.				

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

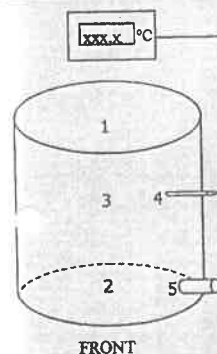

### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber variation : 1.2 °C  
Autoclave Condition : Normal  
Chamber Size (Diameter\*H): 30 \* 71 cm

### CHAMBER PERFORMANCE

Controller Temperature (°C)	Average All Locations (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)	Pressure (MPa)	Holding time (min).	Operating Cycle time (min)
116	116.48	0.09	0.10	0.27	0.090	15	60
122	122.43	0.09	0.13	0.27	0.130	15	60

### TEMPERATURE MEASUREMENT ACCURACY TEST (°C)

Cont Temp	Ind Temp	Measured Temperature ( °C) at Spread Locations					Uncertainty ( ± °C)
		#1	#2	#3	#4	#5	
116	116	116.45	116.50	116.53	116.45	116.45	0.59
122	122	122.40	122.46	122.50	122.39	122.39	0.59

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT OF TEMPERATURE MEASUREMENT ACCURACY TEST EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.  
NOTE 2 : THE STABILITY TERM IN THE UNCERTAINTY BUDGET WAS REPLACED BY THE STANDARD REPEATABILITY.  
NOTE 3 : LOCATION 3 WAS REFERENCE LOCATION.  
NOTE 4 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23M259

Page : 1 of 2

Equipment : Standard Weight

Manufacturer: LS

Model : -

Serial No.: -

ID No.: EQL-121

Condition As-Received: Used Item

Received Date: 02 February 2023

Calibration Date: 07 February 2023

Reference: 2302-0080DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1008.9 mbar

30, 32 Rama II Soi 63, Rama II Rd.,

Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-M01 according to comparison method against standard weights on the basis of weighings at an average air density of 1.2 kg/m<sup>3</sup> and a temperature of 23.4 °C material density of weight is 8000 kg/m<sup>3</sup>.

### Condition of this result of calibration

#### 1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard weight Set (E2)	YCS31-712-00	50202965	MM-0109-22	11 Jul 2024

2.This certificate is not certified for any commercial transaction.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Chaowalit Rittirak  
Issue Date : 08 February 2023

Approved Signatory :

[ ] Phalinee Prabpaipal

[x] Sura Suwannasri

[ ] Chaowalit Rittirak

Cert No.: 23M259

Page: 2 of 2

### Result of calibration

Without adjustment

Nominal Value	Conventional mass	Uncertainty of Measurement ( ± )	Maximum Permissible error ( ± )
50 g	50.00015 g	0.10 mg	0.30 mg

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-000-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23M260

Page : 1 of 2

Cert No.: 23M260

Page: 2 of 2

Equipment : Standard Weight

Manufacturer :

Model :

Serial No. :

ID No. : EQL-258

Condition As-Received: Used Item

Received Date: 02 February 2023

Calibration Date: 07 February 2023

Reference: 2302-0080DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1012 mbar

30, 32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkokhuan, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-M01 according to comparison method against standard weights on the basis of weighings at an average air density of 1.2 kg/m<sup>3</sup> and a temperature of 23.6 °C material density of weight is 8000 kg/m<sup>3</sup>.

### Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard weight Set (E2)	YCS31-712-00	50202965	MM-0109-22	11 Jul 2024

2.This certificate is not certified for any commercial transaction.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Chaowalit Rittirak

Issue Date : 08 February 2023

Approved Signatory :

[ ] Phalinee Prabpalpal

[x] Sura Suwannasri

[ ] Chaowalit Rittirak

### Result of calibration

Without adjustment

Nominal Value	Conventional mass	Uncertainty of Measurement ( ± )	Maximum Permissible error ( ± )
2 kg	2.0000034 kg	3.0 mg	10 mg

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

B 0307756

a 1146232



ICP02329207

MAINTENANCE AND TEST CERTIFICATE MODEL  
OPTIMA 8000

Customer : บริษัท เทสท์ เทคโนโลยี จำกัด	Date Tested: May 18, 2023
Address : 30, 32 ซอยพระรามที่ 2 ซอย 63 ถนนพระรามที่ 2 แขวงสามต้น เขตบางขุนเทียน กรุงเทพฯ 10150	Recommendation Recertification Period 12 Recertification Due: May 17, 2024 Date Last Certified: May 19, 2022 Visit Number: 1 of 1
User Name: คุณอ้อยใจ สระจันทร์	PerkinElmer Phone: 02-719-6420 ext 206
Phone: 02-893-4211-17	PerkinElmer Fax: 02-318-5597
Fax: lab_center@testtech.co.th	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
OPTIMA 8000	078S1411171C	WinLab32 Version 5.5.0.0714
N0772045	2F1441085	PN:6150T21E4Q1E
EQL-180		
TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
IPV Methods		
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
Mixed standard 1/10	N069-1579	NOV 30, 2023
Mixed standard 1/100	N930-0221	NOV 30, 2023
CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
2 % HNO3		
10 % HNO3		

Page 1 of 4



ICP02329207

MAINTENANCE AND TEST CERTIFICATE MODEL  
OPTIMA 8000

SERIAL NUMBER : 078S1411171C	DATE TESTED : May 18, 2023
<b>1. MECHANICAL CHECKS</b>	
A. Inspect and clean all fans and filters.	<input type="checkbox"/>
B. Inspect and replace as necessary, all torch components including the RF coil.	<input type="checkbox"/>
C. Inspect all tubing for sign of clacking or leaking.	<input type="checkbox"/>
D. Adjust water and gas pressure regulator settings.	<input type="checkbox"/>
E. Inspect and leak check pneumatics drawers.	<input type="checkbox"/>
F. Clean the exterior of the instrument.	<input type="checkbox"/>
<b>2. OPTICAL CHECKS</b>	
A. Inspect and clean all optical components.	<input type="checkbox"/>
B. As required, check and replace all purgefilters.	<input type="checkbox"/>
C. Recheck optical alignment.	<input type="checkbox"/>
<b>3. COOLING SYSTEM CHECKS</b>	
A. Perform preventive maintenance on chiller.	<input type="checkbox"/>
B. Flush out the chiller every six months.	<input type="checkbox"/>
<b>4. PERFORMANCE CHECKS</b>	
A. Torch View Alignment.	<input type="checkbox"/>
B. Wavelength Calibration.	<input type="checkbox"/>

Page 2 of 4



ICP02329207

MAINTENANCE AND TEST CERTIFICATE MODEL  
OPTIMA 8000

SERIAL NUMBER : 078S1411171C		DATE TESTED : May 18, 2023	
PARAMETER	SPECIFICATION	FINAL VALUE	
Spectral Resolution : UV	As 193.696 nm	≤ 0.009 nm	0.00720 nm
	Ni 231.604 nm	≤ 0.011 nm	0.00892 nm
	Ni 341.476 nm	≤ 0.015 nm	0.01343 nm
Spectral Resolution : VIS	Ba 455.403 nm	≤ 0.020 nm	0.01726 nm
Precision	Zn 206.200 nm	% RSD ≤ 1.0 %	0.35 %
	Mg 280.271 nm	% RSD ≤ 1.0 %	0.19 %
	Mg 285.213 nm	% RSD ≤ 1.0 %	0.19 %
	Ba 455.403 nm	% RSD ≤ 1.0 %	0.13 %
Detection Limits : Axial	Ti 190.801 nm	3(SD) ppb ≤ 10 ppb	1.54 ppb
	As 193.696 nm	3(SD) ppb ≤ 10 ppb	2.10 ppb
	Se 196.026 nm	3(SD) ppb ≤ 5.0 ppb	2.43 ppb
	Pb 220.353 nm	3(SD) ppb ≤ 3.0 ppb	1.40 ppb
Detection Limits : Radial	As 193.696 nm	3(SD) ppb ≤ 60 ppb	4.44 ppb
	Zn 213.857 nm	3(SD) ppb ≤ 2.0 ppb	0.12 ppb
	Mn 257.610 nm	3(SD) ppb ≤ 1.0 ppb	0.05 ppb
	La 379.478 nm	3(SD) ppb ≤ 3.0 ppb	0.21 ppb
	Ba 455.403 nm	3(SD) ppb ≤ 0.3 ppb	0.01 ppb
	Ba 493.408 nm	3(SD) ppb ≤ 0.6 ppb	0.01 ppb
BEC : Axial (1B X 1000)/(1S-1B)	Mn 257.610 nm	≤ 30 ppb	6.83 ppb
BEC : Radial (1B X 1000)/(1S-1B)	Mn 257.610 nm	≤ 30 ppb	9.29 ppb

Page 3 of 4



ICP02329207

MAINTENANCE REPORT AND IPV TEST CERTIFICATE  
OPTIMA 8000

SERIAL NUMBER : 078S1411171C		DATE TESTED : May 18, 2023	
Remarks :			
Commissioning follow as commissioning performance sheets.			
This is to certify that the above tests have been performed and the configuration tested			
<input checked="" type="checkbox"/> meets			
<input type="checkbox"/> does not meet			
the PerkinElmer Specifications listed on this certificate.			
This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.			
Service Department PerkinElmer Ltd.			
Authorized Representative : ( [Redacted] )			
Customer Support Engineer			

Page 4 of 4



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T230022

Page 1 of 4

## Certificate of Calibration

Equipment : Chamber ( Cooling Room )  
 Manufacturer : -  
 Model : -  
 Serial No. : -  
 Customer Code : EQL-167  
 ID No. : T1447A1  
 Customer : Test Tech Co.,Ltd  
 30, 32 Rama II Soi 63, Rama II Rd., Samaedam,  
 Bangkhunthian Bangkok 10150

Customer Location : LABORATORY FLOOR 3

Date of Receipt : 13 January 2023

Calibrated By [Redacted] akred ( Site Calibration Manager )

Approved By [Redacted] Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 24 JAN 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L14118/31-08-64



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



Certificate No. T230022

Page 2 of 4

## Calibration Report

Equipment : Chamber ( Cooling Room )  
 Date of Calibration : 18 January 2023  
 Environment : Temperature : 25.0-27.2 °C  
 Line Voltage : 221.9-227.3 V  
 Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001) and AS2853-1986 ).  
 All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

### 2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN141-TN150	T222123	5 October 2023
TC	TYPE T	TN151-TN160	T222123	5 October 2023
DATA LOGGER	34970A	T150	T222123	5 October 2023

### 3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)

### 4. Condition of calibrated item : good

#### Equipment Description :

Time Constant 2 Hour 8 Minute At 3 °C  
 Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

### 5. Adjustment :

( ) without adjustment

( X ) after adjustment

Approved By [Redacted]

FM-L15 117/15-05-63



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.




NSC-TISI-TIS 17025  
CALIBRATION 0244

Certificate No. T230022

Page 3 of 4

## Calibration Report

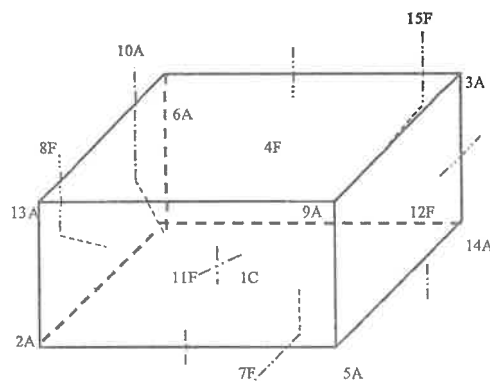

C = Centre, F = Centre of Face, A = Corner, E = Centre of Edge

1C	=	TN141
2A	=	TN142
3A	=	TN143
4F	=	TN144
5A	=	TN145
6A	=	TN146
7F	=	TN147
8F	=	TN148
9A	=	TN149
10A	=	TN150

11F	=	TN151
12F	=	TN152
13A	=	TN153
14A	=	TN154
15F	=	TN155

Approved By

FM-L15 I17/15-05-63



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



NSC-TISI-TIS 17025  
CALIBRATION 0244

Certificate No. T230022

Page 4 of 4

## Calibration Report

### Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)									
	TN141	TN142	TN143	TN144	TN145	TN146	TN147	TN148	TN149	TN150
3	2.93	2.77	2.79	2.26	3.04	3.39	2.91	3.05	3.54	2.95
	TN151	TN152	TN153	TN154	TN155					
	3.32	3.28	3.00	2.96	2.90					

Chamber ( Cooling Room )			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min , Max	Average					
3.0	2.9 , 3.1	3.0	3.01	0.47	1.04	0.98	2.00

\* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By

FM-L15 I17/15-05-63



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.com



NSC-TISI-TIS 17025  
CALIBRATION 0244

Certificate No. T230121

Page 1 of 4

## Certificate of Calibration

**Equipment** : Chamber ( Cooling Room )

**Manufacturer** : -

**Model** : -

**Serial No.** : -

**Customer Code** : EQL-181

**ID No.** : T0399A5

**Customer** : Test Tech Co.,Ltd  
30, 32 Rama II Soi 63, Rama II Rd., Samaedam,  
Bangkhunthian Bangkok 10150

**Customer Location** : LABORATORY FLOOR 4

**Date of Receipt** : 26 January 2023

**Calibrated By** : Sujjar Naknakred ( Site Calibration Manager )

**Approved By** : [Redacted] / Boonchai Suriyawong (Site Calibration Manager)

**Date of Issue** : 01 FEB 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is Issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L14118/31-08-64



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



NSC-TISI-TIS 17025  
CALIBRATION 0244

Certificate No. T230121

Page 2 of 4

## Calibration Report

**Equipment** : Chamber ( Cooling Room )

**Date of Calibration** : 30 January 2023

**Environment** : Temperature : 25.0-27.2 °C  
Line Voltage : 221.9-227.3 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

- This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001) and AS2853-1986 ). All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
- Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN141-TN150	T222123	5 October 2023
TC	TYPE T	TN151-TN160	T222123	5 October 2023
DATA LOGGER	34970A	T150	T222123	5 October 2023
- This certificate is traceable to :  
National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244.)
- Condition of calibrated item : good  
Equipment Description :  
Time Constant  $\frac{1}{30}$  Hour Minute At  $\frac{3}{3}$  °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

- Adjustment :  
( ) without adjustment ( X ) after adjustment

Approved By—

FM-L15 117/15-05-63



# Metrological Center

SCI ECO Services Company Limited


33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



Page 3 of 4

Certificate No. T230121

## Calibration Report

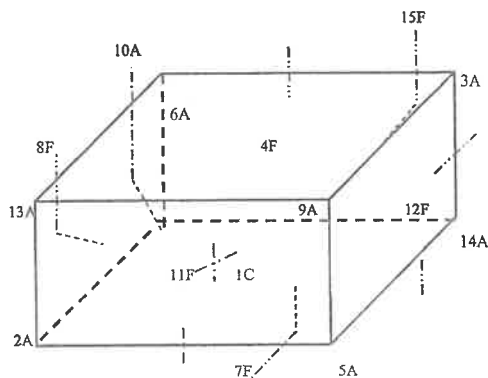

C = Centre, F = Centre of Face, A = Corner, E = Centre of Edge

1C	=	TN141
2A	=	TN142
3A	=	TN143
4F	=	TN144
5A	=	TN145
6A	=	TN146
7F	=	TN147
8F	=	TN148
9A	=	TN149
10A	=	TN150

11F	=	TN151
12F	=	TN152
13A	=	TN153
14A	=	TN154
15F	=	TN155

Approved By

FM-L15 117/15-05-63



# Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



Page 4 of 4

Certificate No. T230121

## Calibration Report

### Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)									
	TN141	TN142	TN143	TN144	TN145	TN146	TN147	TN148	TN149	TN150
3	2.84	2.89	3.01	3.07	3.13	3.19	3.04	2.99	3.15	2.94
	TN151	TN152	TN153	TN154	TN155					
	2.99	2.99	3.14	2.85	2.88					

Chamber (Cooling Room)			Temperature Distribution				
S g (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min, Max	Average					
3.0	2.8, 3.1	3.0	3.01	0.48	0.93	0.99	2.00

\* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By

FM-L15 117/15-05-63





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23H2216  
Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: EQL-064

Condition As-Received: Used Item

Received Date: 12 October 2023

Calibration Date: 17 October 2023  
to 20 October 2023

Reference: 2310-0447DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

30, 32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

#### 1.Reference standards Instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Handheld Thermometer With Sensor	1523	3240076	23I305	15 Mar 2024
2) Dew Point Hygrometer	Optidew 401	164756	TH-0158-22	13 Dec 2023

#### 2.The certificate is valid only to the item calibrated on date and place of calibration.

#### 3.This Certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Surasit Phansudnoi  
Issue Date : 26 October 2023

Approved Signatory :

- [ ] Chakrit Waewwanjua  
[ ] Ponthippa Tameyakul  
[✓] Viporn Tantiyawutti

B 0327545



Cert. No.: 23H2216  
Page.: 2 of 2

Result of Calibration:- Without Adjustment  
Function: Humidity Measurement

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	30.1	30.0	-0.1	1.5
25.0	40.1	39.0	-1.1	1.5
25.0	50.1	49.0	-1.1	1.7
25.0	60.0	59.0	-1.0	1.7
25.0	75.2	75.5	0.3	1.8

Result of Calibration:- Without Adjustment  
Function: Temperature Measurement

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
15.046	15.0	-0.046	0.72
19.975	20.0	0.025	0.72
25.022	25.0	-0.022	0.72
30.000	30.0	0.000	0.72

UUC\* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-000-

a 1185882



CERTIFICATE No : 23M6754  
REFERENCE No : 69854-1

PAGE : 1 OF 2

### Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE  
MANUFACTURER : SARTORIUS  
MODEL : BP210S  
SERIAL No : S0736477  
ID No : EQL-008  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD.,  
SAMAEDAM, BANGKHUNTHIAN, BANGKOK  
10150

CALIBRATED BY : PRASERT D.  
CALIBRATION DATE : 13-Jul-23

APPROVED BY : [Signature]

ISSUED DATE : 17-Jul-23

RECEIVED DATE : 13-Jul-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV 03



CERTIFICATE No : 23M6754

PAGE : 2 OF 2

### Calibration Report

EQUIPMENT : DIGITAL BALANCE  
MANUFACTURER : SARTORIUS  
ID No : EQL-008  
AIR PRESSURE : 1011mbar  $\pm$  1mbar  
AMBIENT TEMPERATURE : 23° C  $\pm$  1° C  
MODEL : BP210S  
S/N : S0736477  
RECEIVED DATE : 13-Jul-23  
CALIBRATION DATE : 13-Jul-23  
RELATIVE HUMIDITY : 50 %RH  $\pm$  10 % RH

#### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING INTERNAL WEIGHT TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN. THE INTERNAL WEIGHT WAS CHECKED BY USING

#### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-


- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

**RESULT OF CALIBRATION** :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 200 g WAS 0 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	49.9999	0.0001	0.00012
100.0	99.9999	0.0001	0.00019
200.0	199.9997	0.0003	0.00032

#### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9998
2	99.9997
3	99.9998
4	99.9998
5	99.9998
OFF-CENTER LOADING	0.0001

6. INTERNAL WEIGHT ERROR : 0.00049999999988177 g

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A  
COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com




CERTIFICATE No : 23T8798  
REFERENCE No : 70515-6

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL : UFE 500  
SERIAL No : G508.0791  
ID No : EQL-128  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.  
CALIBRATION DATE : 11-Sep-23

APPROVED BY :   
ISSUED DATE : 15-Sep-23  
RECEIVED DATE : 11-Sep-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

P-G010 REV : 03



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23T8798

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL : UFE 500  
ID No : EQL-128  
RECEIVED DATE : 11-Sep-23  
AMBIENT TEMPERATURE : 24 °C ± 1 °C  
S/N : G508.0791  
CALIBRATION DATE : 11-Sep-23  
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	23T6636	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT



FRONT

### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 10
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

### CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.49	0.28	0.66	0.93
180.0	180.25	0.32	0.62	1.11

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.46	104.13	104.45	104.28	104.57	104.67	104.60	104.58	104.67	0.38
180.0	180.0	180.27	179.85	180.41	179.93	180.19	180.54	180.41	180.51	180.13	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com



CERTIFICATE No : 23T8799  
REFERENCE No : 70515-7

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL : UFE 500  
SERIAL No : G512.2005  
ID No : EQL-161  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.  
CALIBRATION DATE : 11-Sep-23

APPROVED BY : [Redacted Signature]

ISSUED DATE : 15-Sep-23

RECEIVED DATE : 11-Sep-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 03



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23T8799

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL : UFE 500  
ID No : EQL-161  
RECEIVED DATE : 11-Sep-23  
AMBIENT TEMPERATURE : 24 °C ± 1 °C  
S/N : G512.2005  
CALIBRATION DATE : 11-Sep-23  
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	23T6636	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT



### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 10
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

### CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	103.96	0.14	0.58	0.73
180.0	179.55	0.22	0.93	1.47

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.16	104.13	104.20	103.98	103.76	103.76	104.06	103.71	103.93	0.38
180.0	180.0	179.73	179.89	180.04	179.54	179.30	178.98	179.75	178.97	179.77	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

# Certificate of Calibration

Certificate No.: C08230153

Page 2 of 2

Equipment: TURBIDIMETER  
Model: 2100N  
Serial No. (or ID.): 970400003415 (EQL-024)  
Manufacturer: HACH  
Condition: In Condition  
Certificate No.: C08230153  
Issued Date: 15 September 2023  
Job No.: WO-00005226  
Page: 1 of 2

Customer: TEST TECH CO., LTD.  
30,32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhuntien Bangkok 10150 Thailand

Environment Condition: Temperature 23 °C ± 2 °C  
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Miss.Orawan Khlaiphloi  
Calibration Date: 14 September 2023  
The Method used: In house method, CAL-WI-23, base on Hach Manufacturer Method 8195  
Traceability: This certificate is traceable to Primary standard Fromazin and StabiCal accepted by United States Environmental Protection Agency (EPA) through Hach Company Certificate No. A1075 , A1074 , A1091 , A1074 , A1074

## Calibration Results:

### Before Adjustment

Std Turbidity (NTU)	UUC Reading	Correction	Deviation	Uncertainty
0.050	0.088	-0.038	0.0	0.070
20.40	19.1	1.30	0.0	1.0
205.0	195	10.0	0.5	10
1028.0	952	76.0	0.9	50
4068.0	3942	126.0	0.9	200

### After Adjustment

Std Turbidity (NTU)	UUC Reading	Correction	Deviation	Uncertainty
0.050	0.084	-0.034	0.0	0.070
20.40	20.4	0.00	0.0	1.0
205.0	205	0.0	0.5	10
1028.0	1026	2.0	0.5	50
4068.0	4063	5.0	0.5	200

The End of Certificate



Person in charge



Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - In Asia and Beyond.

CAL-FM-C08-08: 20 Jul 2022

Delivering Growth - In Asia and Beyond.

CAL-FM-C08-08: 20 Jul 2022

ใบรับรองการทวนสอบ “เครื่อง Spectrophotometer”  
(Calibration Certificate of Spectrophotometer)

14



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor7 Rama4 Road  
Silom Bangrak Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



## Certificate of Calibration

Number of Page(s) 1 of 3

<b>Certificate No.</b>	BSCC-UV-163/23
<b>Equipment</b>	UV/Vis Spectrophotometer
<b>Model</b>	UV-1900i
<b>Manufacturer</b>	Shimadzu
<b>Serial No.</b>	A12535780311ML
<b>ID No.</b>	EQL-233
<b>Date of receipt</b>	27 April 2023
<b>Date of calibration</b>	27 April 2023
<b>Date of issue</b>	8 May 2023
<b>Customer name</b>	Test Tech Co., Ltd.
<b>Address</b>	30, 32 Rama II Soi 63, Rama II RD., Samaedam, Bangkhunthian, Bangkok 10150
<b>Temperature</b>	(23.5-24.4) °C (On site)
<b>Humidity</b>	(50.8-48.2) %RH (On site)
<b>Equipment condition</b>	Good Operation
<b>Calibration Location</b>	Clean Room Circubond
<b>Calibration Procedure</b>	In-house method WI-UV-702-01 based on ASTM E275-01
<b>Traceability</b>	Wavelength Accuracy is traceable to certificate No. 96367 and 96366 Photometric Accuracy is traceable to certificate No. 99925 and 96363 Stray Light is traceable to certificate No. 96346 The above certificate are traceable to SI unit through Starna Scientific Ltd. (UKAS accredited calibration laboratory NO. 0659)
<b>Calibrated by</b>	Mr.Poomjai Korsawatvorakul

Approved by



Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention In this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

Certificate No.

BSCC-UV-163/23

Number of Page(s)

2 of 3

## Calibration Results:

### 1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty ( $\pm$ nm)
279.44	279.17	-0.27	0.18
418.53	418.45	-0.08	0.18
536.52	536.58	0.06	0.18
684.50	684.62	0.12	0.18
879.41	879.43	0.02	0.18

### 2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm$ A)
235	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
257	0.0000	0.0000	0.0000	0.0075
	0.8552	0.8532	-0.0020	0.0075
313	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
350	0.0000	0.0001	0.0001	0.0075
	0.6349	0.6336	-0.0013	0.0075

\*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

Certificate No.

BSCC-UV-163/23

Number of Page(s)

3 of 3

## Calibration Results:

### 3.Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm$ A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5472	0.5485	0.0013	0.0042
	0.7637	0.7637	0.0000	0.0042
	1.0480	1.0484	0.0004	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5371	0.5384	0.0013	0.0042
	0.7457	0.7457	0.0000	0.0042
	1.0233	1.0247	0.0014	0.0042
465.0	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
546.1	0.0000	0.0000	0.0000	0.0042
	0.5006	0.5017	0.0011	0.0042
	0.6961	0.6954	-0.0007	0.0042
	0.9563	0.9565	0.0002	0.0042
590.0	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
	CNR	CNR	CNR	0.0042
635.0	0.0000	0.0000	0.0000	0.0042
	0.5137	0.5147	0.0010	0.0042
	0.6907	0.6900	-0.0007	0.0042
	0.9533	0.9536	0.0003	0.0042

\*CNR = Customer not request

### 4.Stray Light\*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC) Wavelength (nm)	Transmission (%)	Absorbance (A)
200.91 $\pm$ 0.11nm	200.55	0.9670	2.0147

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A  
\*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\*\*\*End of Certificate\*\*\*

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.





## Certificate of Calibration



Certificate No.: C06230165

Page 2 of 3

### Calibration Results:

Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm				
Standard Wavelength	Unit Under Calibration	Correction	Uncertainty	
418.61	418.5	0.11	0.13	
536.66	536.7	-0.04	0.13	
637.98	637.9	0.08	0.13	
748.48	748.7	-0.22	0.13	
807.03	807.5	-0.47	0.13	

Photometric Accuracy (Absorbance)				
Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.5816	0.580	0.0016	0.0045
	0.7130	0.712	0.0010	0.0045
	1.0151	1.013	0.0021	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.5649	0.563	0.0019	0.0045
	0.7012	0.699	0.0022	0.0045
	0.9982	0.996	0.0022	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.5249	0.524	0.0009	0.0045
	0.6621	0.661	0.0011	0.0045
	0.9420	0.939	0.0030	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.5214	0.520	0.0014	0.0045
	0.6982	0.697	0.0012	0.0045
	0.9947	0.992	0.0027	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.5549	0.553	0.0019	0.0045
	0.7736	0.771	0.0026	0.0045
	1.1041	1.101	0.0031	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.5621	0.561	0.0011	0.0045
	0.7630	0.761	0.0020	0.0045
	1.0890	1.086	0.0030	0.0045

Equipment: SPECTROPHOTOMETER  
Model: DR6000  
Serial No. (or ID.): 1693421 (EQL-197)  
Manufacturer: HACH  
Condition: In Condition

Certificate No.: C06230165  
Issued Date: 24 April 2023  
Job No.: KSPR2306121  
Page: 1 of 3

Customer: TEST TECH CO., LTD.  
30,32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhuntien Bangkok 10150 Thailand

Environment Condition: Temperature 25.3 °C ± 0.2 °C  
Humidity 48.9 %RH ± 1.7 %RH

Calibration Place: TEST TECH CO., LTD. (แผนกน้ำดี)  
30,32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhuntien Bangkok 10150 Thailand

Calibration By: Mr. Atachai Ngamchanat  
Calibration Date: 21 April 2023  
The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04  
Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 93907 and 93914  
The standard for Photometric Certificate No. 94010 and 93900  
The standard for Stray light Certificate No. 93903 and 93902  
The standard for Spectral resolution Certificate No. 103140

Person in charge

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงบางนา เขตคลองเตย กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phraekhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงบางนา เขตคลองเตย กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phraekhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand



Certificate No.: C06230165

Page 3 of 3

## Calibration Results:

Without Adjustment

Photometric Accuracy (Absorbance)				
Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7440	0.737	0.0070	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8635	0.855	0.0085	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2902	0.288	0.0022	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6409	0.634	0.0069	0.0080
Stray light *				
Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance ( A)	
260.51 +/- 0.11 nm	260.5	0.7	2.155	
391.84 +/- 0.11 nm	391.8	1.2	1.921	
Spectral Resolution *				
Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength ( nm )	268.73	266.77	1.35	2.00
UUC: Wavelength (nm)	268.6	266.6		
Std Absorbance ( A)	0.4237	0.2591		
Absorbance ( A)	0.385	0.285		

\* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate

บริษัท ดีเคเอส อีเซีย จำกัด  
DKSH Technology Limited  
2533 สุขุมวิท Road, Bangkok, Phra Khanong, Bangkok 10260  
Phone: +66 2839 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C06-15: 12 Sep 2022



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 23CH92

Page.: 1 of 3

## Certificate of Calibration

Equipment : Conductivity Meter  
Manufacturer : TOA  
Model : CM-41X  
Serial No. : 842572  
ID No. : EQL-211  
Condition As-Received: Used Item  
Received Date : 19 January 2023  
Calibration Date : 20 January 2023  
Reference : 2301-0614DN-1  
Submitted by : TEST TECH CO.,LTD. (HEAD Office)  
30, 32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhunthian, Bangkok 10150  
Ambient Temperature : (25 ± 2.5) °C  
Relative Humidity : (50 ± 15) %  
Calibration Procedure: In-house method :  
- CP-CH6 by direct measurement  
with certified reference material (CRM)  
- CP-CH8 by comparison with standard thermometer  
Calibrated by : Warakorn Lernagatrakul

Approved by :

( / ) Malee Butkruea  
( ) Sathip Meangmai  
( ) Warakorn Lernagatrakul

Issue Date :

24 January 2023

The Uncertainties are for a confidence probability of approximately 95 %

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0049391



Cert.No.: 23CH92

Page.: 2 of 3

**Condition of this result of calibration**

**1. Reference Standard Instrument :-**

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	1963878	130RC095	2211140	12 Sep 2023
2) Ref. Std. Thermometer	4982054	110RC044	2211306	27 Oct 2023

This certification is traceable to the International System of Unit maintained at:-

- Traceable to National Institute of Metrology (Thailand), NIMT

**2. Certified Reference Materials :-**

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
147.0 $\mu\text{S/cm}$	CPA Chem	823327	20 June 2023
1.413 mS/cm	CPA Chem	823328	20 June 2023
12.880 mS/cm	CPA Chem	823329	20 June 2023

- Control Conductivity calibration solution temperature by Water bath ( $25 \pm 0.1$ )  $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration results**

**Function :** Conductivity Measurement

(\*) After Adjustment at 147.0, 1413.0, 12880  $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 806F0005

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement ( $\pm$ )	Coverage factor k
147.0 $\mu\text{S/cm}$	150.3 $\mu\text{S/cm}$	147.0 $\mu\text{S/cm}$	0.99 $\mu\text{S/cm}$	2.00
1.413 mS/cm	1.428 mS/cm	1.413 mS/cm	0.0092 mS/cm	2.00
12.880 mS/cm	12.71 mS/cm	12.88 mS/cm	0.086 mS/cm	2.00

**Remark**

- UUC\* = Unit Under Calibration
- 147.0  $\mu\text{S/cm}$  Adjustment Cell constant =  $98.5\text{m}^{-1}$
- 1.413 mS/cm Adjustment Cell constant =  $99.5\text{m}^{-1}$
- 12.880 mS/cm Adjustment Cell constant =  $101.8\text{m}^{-1}$

*malu.*

a 1144880



Cert.No.: 23CH92

Page.: 3 of 3

**Calibration Results**

**Function :** Temperature Measurement

(\*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : CT-58101B
- Serial No. : 806F0005

Dimension of probe;

- Length : 114 mm.
- Diameter : 12 mm.
- Immersion Depth : 100 mm.

Calibration Point ( $^{\circ}\text{C}$ )	Standard Temperature ( $^{\circ}\text{C}$ )	UUC* Reading ( $^{\circ}\text{C}$ )	Error ( $^{\circ}\text{C}$ )	Uncertainty of Measurement ( $\pm$ $^{\circ}\text{C}$ )	Coverage factor k
25.0	25.003	25.0	-0.003	0.13	2.00

**Remark :** - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

*malu.*

a 1144879



CERTIFICATE No : 23T8796  
REFERENCE No : 70515-4

PAGE : 1 OF 2

### Certificate of Calibration

EQUIPMENT : WATER BATH  
MANUFACTURER : MEMMERT  
MODEL : WNE 45  
SERIAL No : L720.0266  
ID No : EQL-241  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 16-Aug-23

APPROVED BY :

ISSUED DATE : 16-Aug-23

RECEIVED DATE : 16-Aug-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 23T8796

PAGE : 2 OF 2

### Calibration Report

EQUIPMENT : WATER BATH  
MANUFACTURER : MEMMERT  
ID NUMBER : EQL-241  
RECEIVED DATE : 16-Aug-23  
AMBIENT TEMPERATURE : 25 °C ± 1 °C  
MODEL : WNE 45  
SERIAL NUMBER : L720.0266  
CALIBRATION DATE : 16-Aug-23  
RELATIVE HUMIDITY : 50 %RH ± 10 % RH

#### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO ASTM E715-80 (REAPPROVED 2001) BY COMPARISON WITH CALIBRATED RTD. THE PROBES WERE PLACED ON FIVE POINTS AND LOCATED ONE PROBE IN EACH OF THE FOUR CORNERS OF THE BATH AND PLACED THE FIFTH RTD WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE WATER VOLUME (REFERENCE LOCATION) UNDER NO LOAD CONDITION.

#### 2. REFERENCE STANDARD INSTRUMENTS :-


INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	2625A	6603614	23T6642	19-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

**RESULT OF CALIBRATION :-** WITHOUT ADJUSTMENT



PROBE INSTALLATION  
POSITION IN THE BATH

#### GENERAL INFORMATION

Overall Variation of Ambient Temperature around the Bath (°C) : 0.6
Overall Variation of Line Voltage (V) : 3
Instrument Condition : Normal
Bath Inner Size (W*L*H) : 59*35*20 cm

#### BATH PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (±°C)	Temperature Stability (±°C)	Radius Uniformity (°C)	Axial Uniformity (°C)	Overall Variation (°C)
83.0	83.09	0.05	0.07	0.05	0.16
92.0	92.13	0.11	0.06	0.06	0.28

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations					Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	
83.0	83.0	83.08	83.09	83.06	83.11	83.12	0.15
92.0	92.0	92.11	92.13	92.10	92.16	92.16	0.19

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE BATH.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2. PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT