

ANALYTICAL BALANCE (DU)

Model. : XS205DU

Serial No. : 1126323724

NSC-TISI-TIS17025
CALIBRATION 0152

Page 1 of 4

Certificate No. : 23-006683
Sample Code : 23-02820-006

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by Mr. Thanadol Pholthep
Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)

NSC-TISI-TIS17025
CALIBRATION 0152

Page 2 of 4

Certificate No. : 23-006683
Sample Code : 23-02820-006

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 220 g
Resolution : 0.01 mg / 0.1 mg
Serial No. : 1126323724
ID No. : LABE 05/1

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input checked="" type="checkbox"/> No adjustment	Nominal value	40	30
<input type="checkbox"/> Adjustment	Standard weight	40.000042	30.000045
	Average reading of indicator	40.000015	30.000019
	Standard deviation	0.000004	0.000007

Unit : g	Range : 200	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input checked="" type="checkbox"/> No adjustment	Nominal value	100	200
<input type="checkbox"/> Adjustment	Standard weight	100.000022	200.000199
	Average reading of indicator	100.00001	200.00004
	Standard deviation	0.00004	0.00008

COPY

Certificate No. : 23-006683
Sample Code : 23-02820-006

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.99800	0	0.9980
40	0.99800	100	0.9980
80	0.99800	200	0.9980

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.0000090	2.01
0.01	0.0100036	0.01000	0.00000	0.0000093	2.01
0.1	0.1000062	0.10000	0.00001	0.000012	2.00
1	1.0000036	1.00001	-0.00001	0.000014	2.00
5	5.0000044	5.00003	-0.00003	0.000020	2.00
10	10.000000	10.00007	-0.00007	0.000032	2.00
20	20.000016	20.00011	-0.00009	0.000036	2.00
50	50.000029	50.00013	-0.00010	0.000067	2.00
100	100.000022	100.0001	-0.0001	0.00016	2.00
150	150.000051	150.0001	0.0000	0.00023	2.00
200	200.000199	200.0003	-0.0001	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 23-006683
Sample Code : 23-02820-006


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan	<input type="radio"/> Circle <input type="radio"/> Triangular <input checked="" type="radio"/> Rectangular	Test weight : 50 and 100 Unit : g
Range	80	200
Position	Reading of indicator	Reading of indicator
1	50.00014	100.0001
2	50.00014	99.9998
3	50.00006	100.0000
4	50.00010	100.0001
5	50.00017	100.0001
6	50.00014	100.0001
Maximum difference	0.00008	0.0003

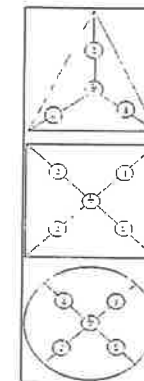

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-57	22-060639	27 June 2023

6. Ambient conditions	Min	Max
Temperature (°C)	21.3	22.4
Relative Humidity (%Rh)	39.2	40.4
Air pressure (hPa)	1008.4	1010.1

- End of Report -

ANALYTICAL BALANCE

Model. : SECURA224-1S

Serial No. : 0036707137



Certificate No. : 23-006682
Sample Code : 23-02820-005

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-1S

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 20 January 2023

Date of Calibration : 20 January 2023

Calibrated by Mr. Thanadol Pholthep
Scientist

Approved by

(Mr. Somchai Neampunt)


Signed for Director

Issue date 25 January 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-006682
Sample Code : 23-02820-005

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : SARTORIUS
Model : SECURA224-1S
Capacity : Max 220 g
Resolution : 0.0001 g
Serial No. : 0036707137
ID No. : LABE 05/2

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
	Nominal value	100	200
<input checked="" type="checkbox"/> No adjustment	Standard weight	100.000022	200.000199
<input type="checkbox"/> Adjustment	Average reading of indicator	99.9998	199.9999
	Standard deviation	0.00007	0.00007
Unit : g	Range : -	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
	Nominal value	-	-
<input type="checkbox"/> No adjustment	Standard weight	-	-
<input type="checkbox"/> Adjustment	Average reading of indicator	-	-
	Standard deviation	-	-

Certificate No. : 23-006682
Sample Code : 23-02820-005

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 220

Test Point	Sensitivity, S
0	0.9980
100	0.9980
200	0.9980

Range : 220

Test Point	Sensitivity, S
0	0.9980
100	0.9980
200	0.9980

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.00011	2.04
0.01	0.0100036	0.0100	0.0000	0.00011	2.04
0.1	0.1000062	0.1000	0.0000	0.00011	2.04
1	1.0000036	1.0000	0.0000	0.00011	2.04
2	2.0000128	2.0000	0.0000	0.00011	2.04
5	5.0000044	5.0000	0.0000	0.00011	2.04
10	10.0000000	10.0000	0.0000	0.00011	2.03
20	20.000016	20.0000	0.0000	0.00012	2.03
50	50.000029	50.0000	0.0000	0.00013	2.02
100	100.000022	99.9998	0.0002	0.00017	2.01
200	200.000199	200.0000	0.0002	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 23-006682
Sample Code : 23-02820-005


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan		<input checked="" type="radio"/> Circle <input type="radio"/> Triangular <input type="radio"/> Rectangular	Test weight : 100 Unit : g
Range	220		
Position	Reading of indicator	Reading of indicator	
1	99.9998		
2	100.0001		
3	99.9997		
4	99.9998		
5	99.9998		
6	99.9998		
Maximum difference	0.0003		

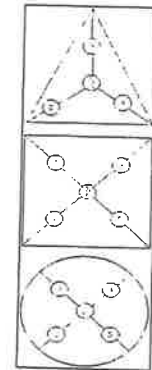

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019
2. This result of calibration was found accurate as shown on date and place of calibration only.
3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

- Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-57	22-060639	27 June 2023

6. Ambient conditions	Min	Max
Temperature (°C)	21.2	22.5
Relative Humidity (%Rh)	37.1	44.3
Air pressure (hPa)	1012.1	1013.0

- End of Report -

AUTOCLAVE

Model : FLS-1000

Serial No. : 55169083

CERTIFICATE OF CALIBRATION

Certificate No. : 23-082126

Sample Code : 23-30826-004

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Autoclave Room)

Equipment : Autoclave

Manufacturer : TOMY

Model : FLS-1000

Serial No. : 55169083

ID No. : LABE 43/2

Date of Receipt : 24 July 2023

Date of Calibration : 24 July 2023

Condition of Calibration

1. Environment
- 1.1 Ambient temperature : Maximum 32.3 °C ; Minimum 30.6 °C
- 1.2 Relative humidity : Maximum 58.9 % ; Minimum 56.3 %
- 1.3 Line voltage supplied : Maximum 226.5 VAC ; Minimum 221.6 VAC

2. Calibration method

The calibration use in-house method: WI-CL-025 based on BS 2646 part 5: 1993 Item 3.1.

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Temperature Data Logger	HiTemp 140	LB-TEM-25	23-030851	23 March 2024
3.2 Temperature Data Logger	HiTemp 140	LB-TEM-26	23-030852	23 March 2024
3.3 Temperature Data Logger	HiTemp 140	LB-TEM-27	23-030853	23 March 2024

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Sarawoot Thammo
Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date : 25 July 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310

TEL 02-516-2422
FAX 02-516-6949

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH

FM-CL-114

Rev 01

Effective Date 15/10/21

REPORT OF CALIBRATION

Certificate No. : 23-082126

Sample Code : 23-30826-004

Results of Calibration

Resolution : 1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading		Measured Temperature at each positions (°C)			Uncertainty ± (°C)	Coverage factor k
		Temperature (°C)	Pressure (MPa)	# 1	# 2	# 3		
121	121	122	0.11	121.78	121.78	121.76	0.63	2.00

2. Characterization results

Calibration Point (°C)	Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
121	0.05	0.04	0.12

Notes

1. UUC* = Unit Under Calibration
2. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
3. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
4. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
5. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
6. UUC* reading - the average reading of indicating device that forms the integral part of the autoclave.
7. Calibration results without adjustment.




Figure: Example of sensor
installation Positions

- Standard 1 : 1 - In the chamber drain, within 100 mm
- Standard 2 : 2 - In the upper half of the chamber
- Standard 3 : 3 - Attached to the load temperature probe, within 20 mm

The stated expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with ISO 15020.

- End of Report -

361 Soi Ladprao 122, Ladprao Road,
Phlabphla, Wang Thonglang, Bangkok 10310
FM-CL-114

TEL 02-516-2422
FAX 02-516-6949
Rev 1/16

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date 15/10/21

BOD INCUBATOR

ID No. : LABE 19/2



Page 1 of 3

CERTIFICATE OF CALIBRATION

Certificate No. : 22-136844
Sample Code : 22-51164-006

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Siiracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : N/A Model : N/A

Serial No. : S540040277 ID No. : LABE 19/2

Date of Receipt : 21 December 2022 Date of Calibration : 21 December 2022

Condition of Calibration

1. Environment
- | | | | | |
|---------------------------|---------|-----------|---------|-----------|
| 1.1 Ambient temperature | Maximum | 25.1 °C | Minimum | 24.3 °C |
| 1.2 Relative humidity | Maximum | 52.3 % | Minimum | 48.5 % |
| 1.3 Line voltage supplied | Maximum | 223.6 VAC | Minimum | 221.9 VAC |

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-P100)	LB-DA-11 (RTD-148 to RTD-155, RTD-227)	22-040308	24 April 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by : Mr. Natthan Phosri
Scientist

Approved by :
Signed for Director

(Mr. Somchai Neampunt)

Issue date : 26 December 2022

The uncertainties are for a confidence probability of approximately 95%

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)



NSC-TIS1-TIS17025
CALIBRATION 0152

Page 2 of 3

REPORT OF CALIBRATION

Certificate No. : 22-136844
Sample Code : 22-51164-006

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			#1	#2	#3	#4	#5	#6	#7	#8	#9 ^{Ref}		
20	20.0	20.0	19.65	19.56	19.47	19.29	20.96	20.47	20.23	20.58	20.29	0.35	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.13	1.09	1.90

Notes

UUC* = Unit Under Calibration

COPY

COPY

REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 22-136844

Sample Code : 22-51164-006

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 60 cm ; D = 70 cm ; H = 124 cm
3. Air valve or fresh air level : Off
4. Fan level : open
5. The quoted uncertainty includes* Stability of chamber and loading effect in chamber at 20% of uniformity *.
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

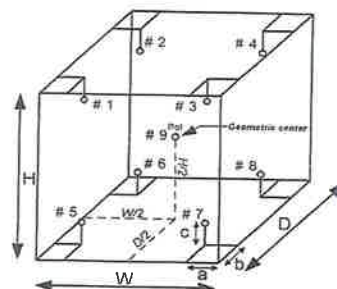


Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY

BOD INCUBATOR

ID No. : LABE 19/5



Page 1 of 3

CERTIFICATE OF CALIBRATION

Certificate No. : 23-040768
Sample Code : 23-16178-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : Lovibond Model : Tc445S

Serial No. : 0520/005227 ID No. : LABE 19/5

Date of Receipt : 21 April 2023 Date of Calibration : 21 April 2023

Condition of Calibration

1. Environment
- | | | | | | | |
|---------------------------|---|---------|-----------|---|---------|-----------|
| 1.1 Ambient temperature | : | Maximum | 36.1 °C | : | Minimum | 34.5 °C |
| 1.2 Relative humidity | : | Maximum | 51.8 % | : | Minimum | 49.3 % |
| 1.3 Line voltage supplied | : | Maximum | 224.7 VAC | : | Minimum | 221.9 VAC |

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-08 (RTD-239 to RTD-247)	22-077888	09 August 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr. Sarawoot Thammo

Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date 24 April 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

NSC-TISI-TIS17025
CALIBRATION 0152

Page 2 of 3

REPORT OF CALIBRATION

Certificate No. : 23-040768

Sample Code : 23-16178-002

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{Ref}		
20	20.0	20.0	20.06	19.92	19.96	19.89	19.93	20.08	19.97	19.79	19.86	0.42	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.32	0.37	0.85

Notes

- UUC* = Unit Under Calibration

NSC-TISI-TIS17025
CALIBRATION 0152

Page 3 of 3

REPORT OF CALIBRATION


Certificate No. : 23-040768

Sample Code : 23-16178-002

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 60 cm ; D = 56 cm ; H = 146 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes" Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

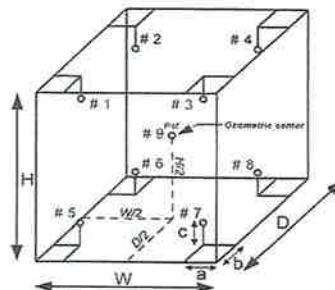Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

End of Report

COPY

DO

Model : YSI 5000

Serial No. : 18E101961



CERT.No.: HS-U055H

Harikul Science Co.,Ltd.
694 Soi Ratchadanivet 24, Pracharatbampnen,
Samsaennok, Huaikhwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com
Certificate of Calibration

Calibration Date : 25 Aug 23

Submitted by : Eastern Thai Consulting 1992 Company Limited
683 Moo.11 Sukaphibal8 Rd., Nongkham, Sriracha,
Chonburi 20230

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Model : YSI 5000
S/N : 18E101961
Probe : YSI 5010
S/N : 18A100724
ID NO. :
Air Temp ref : S/N. F8065C26
Barometric ref : S/N. F8065C26
Water Temp ref : S/N. 11430
Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.07	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.07	(PASS)	-
Measurement 9 (mg/l)	9.07	(PASS)	-
Measurement 10 (mg/l)	9.07	(PASS)	-
Mean Measurement	9.07	mg/l	-
Inaccuracy	0.02	mg/l	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature
(Kittipong Maekwong)

COPY

Supreecha S
Laboratory Manager
(Supreecha Sumaritam)

Hot Air Oven

Model. : UM 400

Serial No. : 900982

NSC-TISI-TIS17025
CALIBRATION 0152

Page 1 of 3

CERTIFICATE OF CALIBRATION

Certificate No. : 23-018635

Sample Code : 23-07651-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhaphiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert Model : UM 400

Serial No. : 900982 ID No. : LABE 17/1

Date of Receipt : 21 February 2023 Date of Calibration : 21 February 2023

Condition of Calibration

1. Environment
- | | | | | |
|---------------------------|---------|-----------|---------|-----------|
| 1.1 Ambient temperature | Maximum | 31.2 °C | Minimum | 28.7 °C |
| 1.2 Relative humidity | Maximum | 50.2 % | Minimum | 40.1 % |
| 1.3 Line voltage supplied | Maximum | 223.9 VAC | Minimum | 221.5 VAC |

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data acquisition with sensor (RTD-P100)	LB-DA-12 (RTD-158 to RTD-166)	22-040312	02 May 2023

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr. Sarawoot Thammo

Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date 24 February 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

NSC-TISI-TIS17025
CALIBRATION 0152

Page 2 of 3

REPORT OF CALIBRATION

Certificate No. : 23-018635

Sample Code : 23-07651-001

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)										Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 ^{Ref}	# 10		
85	85.0	85.0	85.18	85.04	84.62	84.82	85.03	85.04	85.00	84.96	85.08		0.25	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
85	0.07	0.49	0.68

Notes

- UUC* = Unit Under Calibration

COPY

COPY

NSC-TISI-TIS17025
CALIBRATION 0152

Page 3 of 3

REPORT OF CALIBRATION


Certificate No. : 23-018635

Sample Code : 23-07651-001

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes " Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

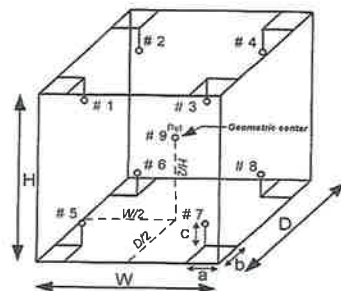Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY

LIQUID IN GLASS THERMOMETER

Model : Total immersion

Serial No. : 43560

Calibration Certificate

Certificate No.: 2300368-001-01
Client name: EASTERN THAI CONSULTING 1992 CO., LTD.
Address: 683 Moo 11, Sukhapibarn 8 Rd.,
 Nongkham, Sriracha, Chonburi 20230

Page 1 of 3

Equipment: Liquid-in-Glass Thermometer
Manufacturer: Precision
Model / Type: Total Immersion
Serial No.: 43560
ID No.: LABE 16/1
Order No.: 2300368
Operation No.: 2300368-001
Date of Receipt: 7 November 2022
Date of Calibration: 15 November 2022

Calibrated by Mr.Nuttapol Niyomchat
 Specialist

Approved by

(Mr.Pheraphat Tuanjit)

Manager, Division of Calibration Laboratory

Responsible for the Technical Management Team

Date of Issue: 18 November 2022

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2300368-001-01
Equipment: Liquid-in-Glass Thermometer Type: Total Immersion
 Range: -1.9 to 101.1 °C Resolution: 0.1 °C
 ID No.: LABE 16/1 Serial No.: 43560
 Manufacturer: Precision
Date of Calibration: 15 November 2022

Page 2 of 3

Location: Temperature Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature 23 °C ± 3 °C
 Relative Humidity 55 % ± 15 %

Condition of this results of Calibration:

- Calibration Method : - In-house method : W-TE-015 based on ASTM E77-07
 - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
 - The temperature Scale in use at this laboratory is the International Temperature Scale of 1990 (ITS-90).

2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
BLACK STACK THERMOMETER	1560/2560	A39258/A39719	PSL-T 0674/65	7-Jun-23	TISTR
Platinum Resistance Thermometer (PRT)	5615	808926			

Support Equipment : - Ice point Unit, ID No.: 614/21

- Low Temperature Bath (Deep Well Compact Bath), Model: 7381, S/N: B53496.
- Low Temperature Bath (Deep Well Compact Bath), Model: 7341, S/N: A5A084.
- High Temperature Bath (Deep Well Compact Bath), Model: 6331, S/N: A5A087.

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good
- Result of Calibration : ☒ Without adjustment ☐ After adjustment

COPY

F-CS-012 Revision: 01 Date: 20-04-65



pH Meter

Model. : SevenCompact S220

Serial No. : B448305208

NSC-TIS1-TIS17025
CALIBRATION 0152

Page 1 of 3

CERTIFICATE OF CALIBRATION

Certificate No. : 23-011524

Sample Code : 23-04833-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : pH Meter

Manufacturer : METTLER TOLEDO Model : SevenCompact S220

Serial No. : B448305208 ID No. : LABE 11/4

Date of Receipt : 01 February 2023 Date of Calibration : 01 February 2023

Condition of Calibration

1. Environment

1.1 Ambient temperature : 25.0 \pm 2.5 $^{\circ}$ C 1.2 Relative humidity : 55.0 % \pm 15.0 %

2. Calibration method

In house method WI-CL-019: based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	22E3240	03 October 2023
3.2 Digital Thermometer	LB-TH-33	22-107027	02 October 2023
Certified Reference Material	Lot. No.	Ref No.	Expire Date
3.3 Buffer Solution pH 4.008	838357	PH216.L5	15 September 2024
3.4 Buffer Solution pH 6.985	838358	PH107.L5	15 September 2023
3.5 Buffer Solution pH 10.008	838359	PH220.L5	15 September 2023

4. This certificate is traceable to the international system of unit (SI Unit).

4.1 Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).

4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

4.4 Buffer Solution No. 3.4 traceable to CPA chem (BIM RefN HI-27 LotN 04.06.2021 ; BIM RefN HI-28 LotN 28.05.2021 ; BIM RefN HI-27 LotN 04.06.2021 ; BIM RefN HI-28 LotN 28.05.2021 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr.Anupong Lakawin

Scientist

Approved by

(Ms. Pawana Pan-on)


Signed for Director

Issue date 03 February 2023

The uncertainties are for a confidence probability of approximately 95%

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)

NSC-TIS1-TIS17025
CALIBRATION 0152

Page 2 of 3

REPORT OF CALIBRATION

Certificate No. : 23-011524

Sample Code : 23-04833-001

Equipment : pH Meter Resolution : 0.01 pH ; 0.1 mV ; 0.1 $^{\circ}$ C
Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B448305208 ID No. : LABE 11/4
Range : -2.000 pH to 20.000 pH ; \pm 2000.0 mV ; -5.0 $^{\circ}$ C to 130.0 $^{\circ}$ C

Results of Calibration

Part 1. DC Voltage measurement

pH Meter Serial No. : B448305208

Nominal Value pH	Applied DC Voltage mV	Average indicator reading		Uncertainty mV	Coverage factor k
		mV	pH		
0	414.113	414.0	0.00	\pm 0.083	2.00
4	177.477	177.5	4.00	\pm 0.083	2.00
7	0.000	0.1	7.00	\pm 0.083	2.00
10	-177.477	-178.3	10.00	\pm 0.083	2.00
14	-414.113	-413.8	14.00	\pm 0.083	2.00

Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Electrode Serial No. : 2365921

Three-Point Calibration at pH4 and pH7 Percent Slope : 99.6 , at pH7 and pH10 Percent Slope : 98.4

Standard Buffer Solution pH (@ 25 $^{\circ}$ C)	Average indicator reading		Error Value pH	Uncertainty pH	Coverage factor k
	pH	mV			
4.008	4.01	184.2	0.002	\pm 0.011	2.00
6.985	6.99	8.9	0.005	\pm 0.010	2.00
10.008	10.01	-166.8	0.002	\pm 0.010	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k which for a normal distribution corresponds to a coverage probability of approximately 95% The standard uncertainty of measurement has been determined in accordance with UKAS M3003

NSC-TISI-TIS17025
CALIBRATION 0152

Page 3 of 3

REPORT OF CALIBRATION

Certificate No. : 23-011524

Sample Code : 23-04833-001

Equipment : pH Meter (Digital Thermometer with sensor)

Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220
Serial No. : B448305208 ID No. : LABE 11/4
Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM
Serial No. : 2365921 ID No. : N/A

Condition of Calibration

1. Environment 1.1 Ambient temperature : 23.0 °C ± 3.0 °C
1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer
2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.
2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

3. Reference standard instrument

Instrument	Model	ID. No.	Certificate No.	Due date
3.1 Platinum Resistance Thermometer	PT-100	RTD-90	22-107027	02 October 2023
3.2 Thermometer Readout	GT-11	LB-TH-33	22-107027	02 October 2023

4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration			Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C	Correction value °C		
25	25.002	120	25.0	+ 0.002	± 0.13	2.00

Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of report -

COPY

STANDARD WEIGHT 50 g



Certificate No. : 22-052238
Sample Code : 22-19150-003

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by Mr. Somwang Sangdee
Scientist

Issue date 31 May 2022

Approved by

(Mr. Somchai Neampunt)

Signed for Director

COPY

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052238
Sample Code : 22-19150-003

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
50 g	-0.324	49.999676 g	0.10	0.30	LABE 10/1

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

COPY

Certificate No. : 22-052238

Sample Code : 22-19150-003

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration:

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.20 kg/m^3

2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

STANDARD WEIGHT 100 g



Certificate No. : 22-052239
Sample Code : 22-19150-004

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052239
Sample Code : 22-19150-004

REPORT OF CALIBRATION

Equipment : Standard Weight 100 g
Manufacturer : N/A
Class : N/A
Serial No. : N/A
ID No. : LABE 10/2

Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
100 g	-0.171	99.999829 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY



Certificate No. : 22-052239

Sample Code : 22-19150-004

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.18 kg/m^3

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY

STANDARD WEIGHT 50 g



Certificate No. : 22-052237
Sample Code : 22-19150-002

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapiban 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Approved by : (Mr. Somchai Neampunt)
Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052237
Sample Code : 22-19150-002

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g
Manufacturer : N/A
Class : N/A
Serial No. : N/A
ID No. : LABE 10/4

Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional Mass	Expanded Uncertainty	Maximum Permissible Error	ID No.
	(mg)		(mg)	± (mg)	
50 g	-0.111	49.999889 g	0.10	0.30	LABE 10/4

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

Certificate No. : 22-052237
Sample Code : 22-19150-002

Page 3 of 3

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.18 kg/m^3
2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)
3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -



COPY

Calibration Report

Certificate No.: 2300368-001-01
Equipment: Liquid-in-Glass Thermometer Type: Total Immersion
Range: -1.9 to 101.1 °C Resolution: 0.1 °C
ID No.: LABE 16/1 Serial No.: 43560
Manufacturer: Precision

Date of Calibration: 15 November 2022 Page 3 of 3

Calibration point: 3.0, 25.0 and 50.0 °C
Calibration result:

Reporting of ice-point or reference point

UUC* Reading (°C)	Standard Temperature/Ice Point (°C)	Correction Value (°C)	Uncertainty ± (°C)
0.0	0.0032	0.0	0.091

Reporting of temperature calibration point

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
25.0	24.9990	0.0	0.088
50.0	49.9943	0.0	0.088

Note

* UUC* : Unit Under Calibration

COPY

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k=2$, providing a level of confidence of approximately 95 %.

----- End -----

