



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 22M1563

Page : 1 of 2

Equipment : Standard Weight

Manufacturer: -

Model : -

Serial No.: M 0030/11

ID No.: EQL-139

Condition As-Received: Used Item

Received Date: 11 August 2022

Calibration Date: 24 August 2022

Reference: 2208-0438DN

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1008 mbar

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

30, 32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-M01 according to comparison method against standard weights on the basis of weighings at an average air density of 1.2 kg/m<sup>3</sup> and a temperature of 23.0 °C material density of weight is 8000 kg/m<sup>3</sup>.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard weight Set (E2)	YCS31-712-00	50202965	MM-0109-22	11 Jul 2024

2.This certificate is not certified for any commercial transaction.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Chaowalit Rittirak

Issue Date : 25 August 2022

Approved Signatory :

[  
[  
[

B 0295804



Cert No.: 22M1563

Page: 2 of 2

**Result of calibration**

Without adjustment

Nominal Value	Conventional mass	Uncertainty of Measurement ( $\pm$ )	Maximum Permissible error ( $\pm$ )
2 g	2.000020 g	0.040 mg	0.12 mg

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-



**a 1122451**



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 22M1562

Page : 1 of 2

Equipment : Standard Weight

Manufacturer: Mettler Toledo

Model :

Serial No.: 11119459

ID No.: EQL-149

Condition As-Received: Used Item

Received Date: 11 August 2022

Calibration Date: 24 August 2022

Reference: 2208-0438DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1008 mbar

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

30, 32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-M01 according to comparison method against standard weights on the basis of weighings at an average air density of 1.2 kg/m<sup>3</sup> and a temperature of 23.0 °C material density of weight is 8000 kg/m<sup>3</sup>.

### Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard weight Set (E2)	YCS31-712-00	50202965	MM-0109-22	11 Jul 2024

2.This certificate is not certified for any commercial transaction.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Chaowalit Rittirak  
Issue Date : 25 August 2022

Approved Signatory :

[ ]  
[ ]  
[ ]

B 0295803



Cert No.: 22M1562

Page: 2 of 2

**Result of calibration**

Without adjustment

Nominal Value	Conventional mass	Uncertainty of Measurement ( $\pm$ )	Maximum Permissible error ( $\pm$ )
20 g	20.000011 g	0.080 mg	0.25 mg

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

a 1122452



## Certificate of Calibration

Equipment:	TURBIDIMETER	Certificate No.:	C08230153
Model:	2100N	Issued Date:	15 September 2023
Serial No. (or ID.):	970400003415 (EQL-024)	Job No.:	WO-00005226
Manufacturer:	HACH	Page:	1 of 2
Condition:	In Condition		

**Customer:** TEST TECH CO., LTD.  
30,32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhuntien Bangkok 10150 Thailand

**Environment Condition:** Temperature 23 °C ± 2 °C  
Humidity 50 %RH ± 15 %RH

**Calibration Place:** Environment Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260 Thailand

**Calibration By:** Miss.Orawan Khlaiphloi

**Calibration Date:** 14 September 2023

**The Method used:** In house method, CAL-WI-23, base on Hach Manufacturer Method 8195

**Traceability:** This certificate is traceable to Primary standard Fromazin and StablCal accepted by United States Environmental Protection Agency (EPA) through Hach Company  
Certificate No. A1075 , A1074 , A1091 , A1074 , A1074



Person in charge



Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

**Calibration Results:**
**Before Adjustment**

Std Turbidity (NTU)	UUC Reading	Correction	Deviation	Uncertainty
0.050	0.088	-0.038	0.0	0.070
20.40	19.1	1.30	0.0	1.0
205.0	195	10.0	0.5	10
1028.0	952	76.0	0.9	50
4068.0	3942	126.0	0.9	200

**After Adjustment**

Std Turbidity (NTU)	UUC Reading	Correction	Deviation	Uncertainty
0.050	0.084	-0.034	0.0	0.070
20.40	20.4	0.00	0.0	1.0
205.0	205	0.0	0.5	10
1028.0	1026	2.0	0.5	50
4068.0	4063	5.0	0.5	200

**The End of Certificate**

๗5

---

ใบรับรองการสอบเทียบ “เครื่องวัด pH”  
(Calibration Certificate of pH Meter)



**QUALITY CALIBRATION CO.,LTD.**  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 23E0843  
REFERENCE No : 67999-1

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : pH METER  
**MANUFACTURER** : DKK-TOA  
**MODEL** : HM-25R  
**SERIAL No** : 760205  
**ID No** : EQL-183  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

**CALIBRATED BY** : 

**CALIBRATION DATE** : 27-Jan-23

**APPROVED BY** : 

**ISSUED DATE** : 03-Jan-23

**RECEIVED DATE** : 27-Jan-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E0843

PAGE : 2 OF 2

**Calibration Report**

EQUIPMENT : pH METER  
MANUFACTURER : DKK-TOA  
ID No : EQL-183  
RECEIVED DATE : 27-Jan-23  
AMBIENT TEMPERATURE : 23°C ± 1°C

MODEL : HM-25R  
SERIAL NUMBER : 760205  
CALIBRATION DATE : 27-Jan-23  
RELATIVE HUMIDITY : 51 %RH ± 10 % RH

**CONDITION OF THIS RESULTS OF CALIBRATION**

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER SOLUTION.
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/ LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC719181	4880-12119147	05-Apr-23
2) pH STANDARD SOLUTION	00651-08	CC718727	4881-12110709	31-Mar-23
3) pH STANDARD SOLUTION	00651-10	CC717045	4882-12065386	17-Mar-23
4) PROCESS CALIBRATOR	CA150	91S6079	22E1145	31-Mar-23
5) BATH	260014	1247.48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

**RESULT OF CALIBRATION : WITHOUT ADJUSTMENT****1. DISPLAY UNIT WITH pH ELECTRODE S/N: 202F0138MK**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	ACTUAL READING (mV)	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.007	4.01	-0.003	178	0.013	2.0
7.004	7.00	0.004	0.0	0.013	2.0
10.014	10.01	0.004	-177	0.014	2.0

**2. DISPLAY UNIT MEASUREMENT TEMPERATURE WITH PROBE**

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
25.002	25.0	80	0.002	0.21

**3. PERCENT SLOPE 98%**

UUC : UNIT UNDER CALIBRATION

THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

F-C





**QUALITY CALIBRATION CO.,LTD.**  
235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584




CERTIFICATE No : 21E11277  
REFERENCE No : 63049-1

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : pH METER  
**MANUFACTURER** : TOA DKK  
**MODEL** : HM-41X  
**SERIAL No** : 784787  
**ID No** : EQL-199  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

**CALIBRATED BY** :   
**CALIBRATION DATE** : 15-Oct-21

**APPROVED BY** :   
**ISSUED DATE** : 15-Oct-21  
**RECEIVED DATE** : 15-Oct-21

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 21E11277

PAGE : 2 OF 2

**Calibration Report**

EQUIPMENT : pH METER  
MANUFACTURER : TOA DKK  
ID No : EQL-199  
RECEIVED DATE : 15-Oct-21  
AMBIENT TEMPERATURE : 25° C ± 1° C  
MODEL : HM-41X  
SERIAL NUMBER : 784787  
CALIBRATION DATE : 15-Oct-21  
RELATIVE HUMIDITY : 51 %RH ± 10 % RH

**CONDITION OF THIS RESULTS OF CALIBRATION**

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTROD WAS CALIBRATED BY USING STANDARD pH BUFFER SOLUTION.
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-06	CC719181	4880-12119147	05-Apr-23
2) pH STANDARD SOLUTION	00651-08	CC718727	4881-12110709	31-Mar-23
3) pH STANDARD SOLUTION	00651-10	CC717045	4882-12065386	17-Mar-23
4) PROCESS CALIBRATOR	744	7514008	21E1392	29-Apr-22
5) BATH	260014	1247 48074	21T9121	10-Sep-22
6) THERMOMETER WITH PROBE	421504	55000379	21T9129	14-Sep-22
7) STANDARD THERMOMETER	2560	A14546	PSL-T0049/64	23-Nov-22

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

**RESULT OF CALIBRATION : ADJUSTMENT****1. DISPLAY UNIT WITH pH ELECTRODE S/N: 903F0008MK**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	ACTUAL READING (mV)	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.007	4.01	-0.003	177	0.013	2.00
7.003	7.00	0.003	0	0.013	2.00
10.014	10.01	0.004	-177	0.014	2.00

**2. DISPLAY UNIT MEASUREMENT TEMPERATURE WITH PROBE**

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
25.008	25.0	80	0.008	0.21

**UUC : UNIT UNDER CALIBRATION**

THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

---

ใบรับรองการสอบเทียบ “เครื่องวัดอุณหภูมิ-ความชื้นสัมพัทธ์”  
(Calibration Certificate of Thermo - Hygrometer)



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23H2216

Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: EQL-064

Condition As-Received: Used Item

Received Date: 12 October 2023

Calibration Date: 17 October 2023  
to 20 October 2023

Reference: 2310-0447DN

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

30, 32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Handheld Thermometer With Sensor	1523	3240076	23I305	15 Mar 2024
2) Dew Point Hygrometer	Optidew 401	164756	TH-0158-22	13 Dec 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Surasit Phansudnoi  
Issue Date : 26 October 2023

Approved Signatory :

[  
[  
[✓

B 0327545



Cert. No.: 23H2216

Page.: 2 of 2

**Result of Calibration:-**

Without Adjustment

Function: Humidity Measurement

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	30.1	30.0	-0.1	1.5
25.0	40.1	39.0	-1.1	1.5
25.0	50.1	49.0	-1.1	1.7
25.0	60.0	59.0	-1.0	1.7
25.0	75.2	75.5	0.3	1.8

**Result of Calibration:-**

Without Adjustment

Function: Temperature Measurement

<u>Standard</u> <u>Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (±°C)
15.046	15.0	-0.046	0.72
19.975	20.0	0.025	0.72
25.022	25.0	-0.022	0.72
30.000	30.0	0.000	0.72

**UUC\*** : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor  $k = 2.00$ , providing confidence level approximately 95%.

-o0o-



a 1185882

๗7

---

ใบรับรองการสอบเทียบ “ตู้อบ”  
(Calibration Certificate of Oven)







**QUALITY CALIBRATION CO.,LTD.**  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com




CERTIFICATE No : 23T8798  
REFERENCE No : 70515-6

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : HOT AIR OVEN  
**MANUFACTURER** : MEMMERT  
**MODEL** : UFE 500  
**SERIAL No** : G508.0791  
**ID No** : EQL-128  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

**CALIBRATED BY** :   
**CALIBRATION DATE** : 11-Sep-23

**APPROVED BY** :   
**ISSUED DATE** : 15-Sep-23  
**RECEIVED DATE** : 11-Sep-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 03



CERTIFICATE No : 23T8798

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL : UFE 500  
ID No : EQL-128  
RECEIVED DATE : 11-Sep-23  
AMBIENT TEMPERATURE : 24 °C ± 1 °C  
S/N : G508.0791  
CALIBRATION DATE : 11-Sep-23  
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	23T6636	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

**RESULT OF CALIBRATION :-** WITHOUT ADJUSTMENT

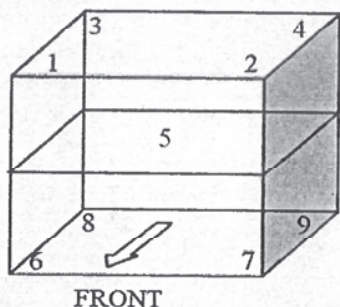

### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 10
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

### CHAMBER PERFORMANCE

Calibrate Piont (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.49	0.28	0.66	0.93
180.0	180.25	0.32	0.62	1.11

### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.46	104.13	104.45	104.28	104.57	104.67	104.60	104.58	104.67	0.38
180.0	180.0	180.27	179.85	180.41	179.93	180.19	180.54	180.41	180.51	180.13	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





**QUALITY CALIBRATION CO.,LTD.**  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
[www.qcalibration.com](http://www.qcalibration.com)




CERTIFICATE No : 23T8799  
REFERENCE No : 70515-7

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : HOT AIR OVEN  
**MANUFACTURER** : MEMMERT  
**MODEL** : UFE 500  
**SERIAL No** : G512.2005  
**ID No** : EQL-161  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

**CALIBRATED BY** :   
**CALIBRATION DATE** : 11-Sep-23

**APPROVED BY** :   
**ISSUED DATE** : 15-Sep-23  
**RECEIVED DATE** : 11-Sep-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 03



# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23T8799

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL : UFE 500  
ID No : EQL-161  
RECEIVED DATE : 11-Sep-23  
AMBIENT TEMPERATURE : 24 °C ± 1 °C  
S/N : G512.2005  
CALIBRATION DATE : 11-Sep-23  
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	23T6636	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

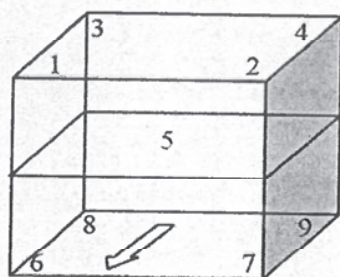

FRONT

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 10
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

#### CHAMBER PERFORMANCE

Calibrate Piont (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	103.96	0.14	0.58	0.73
180.0	179.55	0.22	0.93	1.47

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.16	104.13	104.20	103.98	103.76	103.76	104.06	103.71	103.93	0.38
180.0	180.0	179.73	179.89	180.04	179.54	179.30	178.98	179.75	178.97	179.77	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





**QUALITY CALIBRATION CO.,LTD.**  
235 Petchkasem 63/2 Road, Laksong, Bangkok, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com




CERTIFICATE No : 23T8797  
REFERENCE No : 70515-5

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : HOT AIR OVEN  
**MANUFACTURER** : MEMMERT  
**MODEL** : UF 110  
**SERIAL No** : B414.0764  
**ID No** : EQL-169  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

**CALIBRATED BY** :   
**CALIBRATION DATE** : 11-Sep-23

**APPROVED BY** :   
**ISSUED DATE** : 15-Sep-23  
**RECEIVED DATE** : 11-Sep-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 03



CERTIFICATE No : 23T8797

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : HOT AIR OVEN  
MANUFACTURER : MEMMERT  
MODEL : UF 110  
ID No : EQL-169  
RECEIVED DATE : 11-Sep-23  
AMBIENT TEMPERATURE : 24 °C ± 1 °C

S/N : B414.0764  
CALIBRATION DATE : 11-Sep-23  
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	23T6636	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

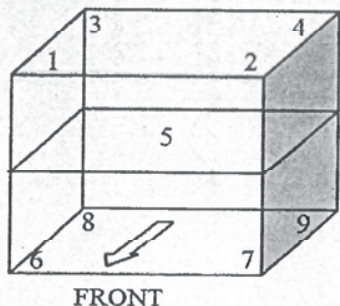

#### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 3
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

#### CHAMBER PERFORMANCE

Calibrate Point (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.04	0.10	0.55	1.06
120.0	120.10	0.11	0.65	1.20
140.0	140.03	0.14	0.77	1.33
150.0	150.05	0.14	0.79	1.48

#### TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.34	104.25	104.10	104.00	104.05	103.61	103.93	103.57	104.54	0.38
120.0	120.0	120.39	120.38	120.27	120.06	120.13	119.57	119.98	119.52	120.56	0.46
140.0	140.0	140.47	140.39	140.24	139.99	140.01	139.39	139.94	139.30	140.54	0.46
150.0	150.0	150.55	150.49	150.32	150.00	149.98	149.35	149.97	149.25	150.57	0.46

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



๗๘

---

ใบรับรองการสอบเทียบ “เครื่องชั่ง”

(Calibration Certificate of Electronic Balance)





**QUALITY CALIBRATION CO.,LTD.**  
235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
[www.qcalibration.com](http://www.qcalibration.com)




CERTIFICATE No : 23M6754  
REFERENCE No : 69854-1

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE  
**MANUFACTURER** : SARTORIUS  
**MODEL** : BP210S  
**SERIAL No** : S0736477  
**ID No** : EQL-008  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD.,  
SAMAEDAM, BANGKHUNTHIAN, BANGKOK  
10150

**CALIBRATED BY** :   
**CALIBRATION DATE** : 13-Jul-23

**APPROVED BY** :   
**ISSUED DATE** : 17-Jul-23  
**RECEIVED DATE** : 13-Jul-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



## QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23M6754

PAGE : 2 OF 2

### Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BP210S  
MANUFACTURER : SARTORIUS S/N : S0736477  
ID No : EQL-008 RECEIVED DATE : 13-Jul-23  
AIR PRESSURE : 1011mbar  $\pm$  1mbar CALIBRATION DATE : 13-Jul-23  
AMBIENT TEMPERATURE : 23°C  $\pm$  1°C RELATIVE HUMIDITY : 50 %RH  $\pm$  10 % RH

#### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING INTERNAL WEIGHT TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN. THE INTERNAL WEIGHT WAS CHECKED BY USING

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

#### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	49.9999	0.0001	0.00012
100.0	99.9999	0.0001	0.00019
200.0	199.9997	0.0003	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9998
2	99.9997
3	99.9998
4	99.9998
5	99.9998
OFF-CENTER LOADING	0.0001

6. INTERNAL WEIGHT ERROR : 0.00049999999988177 g

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY M COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 23M8800  
REFERENCE No : 70515-8

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE  
MANUFACTURER : AND  
MODEL : GR-200  
SERIAL No : 14243876  
ID No : EQL-130  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,  
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY :   
CALIBRATION DATE : 11-Sep-23

APPROVED BY :   
ISSUED DATE : 15-Sep-23  
RECEIVED DATE : 11-Sep-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 23M8800

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : GR-200  
MANUFACTURER : AND S/N : 14243876  
ID No : EQL-130 RECEIVED DATE : 11-Sep-23  
AIR PRESSURE : 1011mbar + 1mbar CALIBRATION DATE : 11-Sep-23  
AMBIENT TEMPERATURE : 24° C ± 1° C RELATIVE HUMIDITY : 50 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0000	0.0000	0.000094
50.0	50.0000	0.0000	0.00012
100.0	100.0000	0.0000	0.00019
200.0	200.0000	0.0000	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0001
3	100.0001
4	99.9999
5	100.0001
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT






CERTIFICATE No : 23M11118  
REFERENCE No : 71188-2


PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE  
MANUFACTURER : SARTORIUS  
MODEL : BCA3202I-1S  
SERIAL No : 0039407364  
ID No : EQL-257  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : TEST TECH CO., LTD.  
30,32 RAMA II SOI 63, RAMA II RD.,  
SAMAEDAM, BANGKHUNTHIAN, BANGKOK  
10150

CALIBRATED BY : 

CALIBRATION DATE : 09-Nov-23

APPROVED BY : 

ISSUED DATE : 13-Nov-23

RECEIVED DATE : 09-Nov-23





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23M11118

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BCA32021-1S  
MANUFACTURER : SARTORIUS S/N : 0039407364  
ID No : EQL-257 RECEIVED DATE : 09-Nov-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 09-Nov-23  
AMBIENT TEMPERATURE : 23°C  $\pm$  1°C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	---	0094-51	23M1296	07-Feb-24
2) STANDARD WEIGHT	---	QK-I-009	23M1297	07-Feb-24
3) STANDARD WEIGHT	---	QK-I-010	M2302003S	01-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 2500 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.00	0.00	0.012
10.0	10.00	0.00	0.012
20.0	20.00	0.00	0.012
50.0	50.00	0.00	0.012
100.0	100.00	0.00	0.012
200.0	200.00	0.00	0.012
500.0	500.00	0.00	0.012
700.0	700.00	0.00	0.012
1000.0	1000.00	0.00	0.012
2000.0	2000.00	0.00	0.012
3000.0	3000.00	0.00	0.012

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	1000.00
2	1000.00
3	1000.00
4	1000.00
5	1000.00
OFF-CENTER LOADING	0.00

NOTE : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



## Certificate of Calibration

Equipment:	Balance	Certificate No.:	C01232449
Model:	BCA224I-1S	Issued Date:	08 July 2023
Serial No. (or ID.):	0043402017 (EQL - 268)	Job No.:	KSPR2310693
Manufacturer:	Sartorius	Page:	1 of 2
Condition:	New		

**Customer:** TEST TECH CO., LTD.  
30,32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhuntien Bangkok 10150 Thailand.

**Environment Condition:** Temperature 23 °C ± 0.4 °C  
Humidity 59 %RH ± 4.2 %RH

**Calibration Place:** TEST TECH CO., LTD. ( 302 Room )  
30,32 Rama II Soi 63, Rama II Rd.,  
Samaedam, Bangkhuntien Bangkok 10150 Thailand.

**Calibration By:**

**Calibration Date:** 07 July 2023

**The Method used:** In-house method, CAL-WI-47, based on UKAS Lab 14

**Traceability:** This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02220533



Person in charge



Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

DKSH Technology Limited

2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260

2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.


CAL-FM-C01-14: 12 Sep 20



### Calibration Results:

#### Without Adjustment

**Eccentric Error:** Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

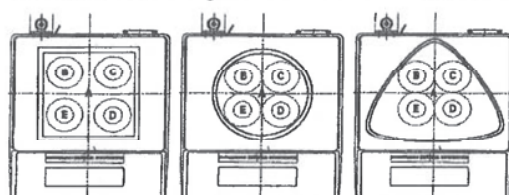			Nominal Test Value		100	(g)
Reference Points (g)						
A	B	C	D	E		
-	0.0000	0.0000	-0.0001	-0.0001		

**Repeatability:** Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
20	0.00004
200	0.00005

**Error of Indication from nominal or conventional mass value.,** Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of Indication (g)	Uncertainty (g)	k
0.001	0.00100	0.0010	0.0000	0.00010	2.03
0.01	0.01000	0.0100	0.0000	0.00010	2.03
0.1	0.10001	0.1000	0.0000	0.00010	2.03
0.5	0.50000	0.5000	0.0000	0.00010	2.03
1	1.00001	1.0000	0.0000	0.00010	2.03
2	2.00002	2.0000	0.0000	0.00010	2.03
5	5.00002	5.0000	0.0000	0.00011	2.03
10	10.00002	10.0000	0.0000	0.00011	2.03
20	20.00000	20.0000	0.0000	0.00011	2.02
25	25.00003	25.0000	0.0000	0.00012	2.02
50	49.99996	50.0000	0.0000	0.00013	2.01
100	100.00002	100.0000	0.0000	0.00017	2.00
120	120.00002	120.0000	0.0000	0.00021	2.00
150	149.99998	150.0000	0.0000	0.00023	2.00
200	200.00004	200.0000	0.0000	0.00029	2.00

### The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
 DKSH Technology Limited  
 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260  
 2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
 Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-C01-14: 12 Sep 20