

ภาคผนวก ฎ  
เอกสารสอบเทียบเครื่องมือ

---



## List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
<b>Ambient</b>									
1	Mass Flow Meter	VOCs	Alicat Scientific, Inc.	MB-5SCCM-D/5M 71015	Miracle International Technology Co.,Ltd.	L202309298-0002	27 Sep 23	26 Sep 24	-
2	Aneroid Barometer	VOCs	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23P1855	2 Jun 23	1 Jun 24	-
3	Dial Thermo-Hygrometer	VOCs	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23H1201	5 Jun 23	5 Jun 24	-
4	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Environmental Instrument	42C 42C-67174-356	UAE Consultant Co.,Ltd.	11012023	11 Jan 23	10 Jan 24	-
5	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
6	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387067	UAE Consultant Co.,Ltd.	09022023	9 Feb 23	8 Feb 24	-
7	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
8	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2301DR0024	Thai Meteorological Department	176/23	10 Apr 23	9 Apr 24	-



## CALIBRATION CERTIFICATE

Certificate No. : L202309298-0002  
Date Issued : 28-Sep-23

**Customer** : United Analyst and Engineering Consultant Co.,Ltd.  
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

**Equipment** : Mass Flow Meter

**Manufacturer** : Alicat Scientific  
**Model** : MB-5SCCM-D/5M  
**Serial No.** : 71015  
**ID No./Tag No.** : UAE.EMA2.119/2555  
**Date Received** : 25-Sep-23  
**Date Calibrated** : 27-Sep-23  
**Calibrated by** : Mr. Jame Khaothong

### Calibration Method or Calibration Procedure Used

In-house method : CP-34 by comparison against mass flow calibrator.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

### Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:   
(Mr. Sarayuth Tochua)



Page 1 of 3

เอกสารไม่ควบคุม

Certificate No. : L202309298-0002

**Environment** : Ambient temperature : ( 23 ± 2 ) °C  
Relative humidity : ( 50 ± 15 ) % RH  
**Capacity Range** : 5 ml/min  
**Calibration Media** : Air  
**Type** : Mass Flowmeter


**Unit Under Calibration Reference Condition** : Pressure 101.325 kPa(abs) , 25 °C , Air

Temperature ( °C )	Pressure ( kPa )	UUC Reading ( ml/min )	STD Reading ( ml/min )	Error ( ml/min )	Uncertainty ( ± ml/min )	MPE ( ± ml/min )	Pass / Fail Simple Acceptance
23.81	100.52	0.000	0.000 *	0.000	0.063	0.010	Pass
23.81	104.15	2.002	1.994	0.008	0.094	0.026	Pass
23.82	105.79	3.001	2.990	0.011	0.13	0.034	Pass
23.86	106.28	3.305	3.290	0.015	0.14	0.036	Pass
23.87	107.53	4.006	3.974	0.032	0.16	0.042	Pass
23.97	109.53	5.004	4.964	0.040	0.19	0.050	Pass

**Error = Unit Under Calibration - Standard** Pass = |error| ≤ |MPE|

Fail = |error| > |MPE|

Marked \* are not included in the NSC-ONSC accreditation schedule for our laboratory.

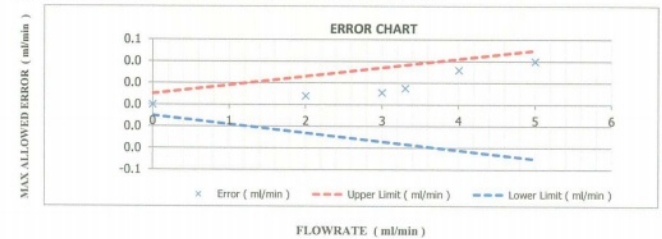

Page 2 of 3

Certificate No. : L202309298-0002

Note : The actual flow rate is determined by the equation :

$$Q_{Meas} = Q_{Ref} \times \frac{P_{Ref}}{P_{Meas}} \times \frac{T_{Meas}}{T_{Ref}}$$

; Q = Flow rate  
 ; P = Absolute pressure  
 ; T = Absolute temperature  
 ; Subscript "Meas" = Measurement condition  
 ; Subscript "Ref" = Reference condition

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

### Traceability of Certificate :

The International System of Units (SI) through

NIMT Calibration Certificate No. MW-0013-22 for Mass Flow Calibrator (20 SCCM) Serial No. G500971G20, Due 22-Feb-24

End of Certificate

Page 3 of 3

เอกสารไม่ควบคุม

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484

## Certificate of Calibration

Certificate No. : 23P1855  
Page : 1 of 2

**Equipment** : Aneroid Barometer  
**Manufacturer** : Barigo  
**Model** : -  
**Serial No.** : -  
**ID No.** : UAE.ANV.122/2550  
**Condition As-Received** : Used Item  
**Received Date** : 26 May 2023  
**Calibration Date** : 02 June 2023

**Reference** : 2305-0919WSC  
**Ambient Temperature** : ( 23 ± 2 ) °C  
**Relative Humidity** : ( 50 ± 15 ) %  
**Atmospheric Pressure** : 1007 mbar

**Submitted by** : United Analyst and Engineering Consultant Co.,Ltd.  
81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

**Procedure used** : The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using "DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

**Condition of this result of calibration**

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505048	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.  
3.This result of calibration was made on requested at the point specified by customer.  
4.This result of calibration instrument was in absolute pressure.  
5.This instrument was used clean air as pressure media.  
6.The certificate is valid only to the item calibrated on date and place of calibration.  
7.This Certification is traceable to the International System of Unit maintained through:-  
-National Institute of Metrology Thailand (NIMT)

**Calibrated by** : Suksan Khankaew  
**Issue Date** : 08 June 2023

**Approved Signatory** :   
[ ] Phalinee Prabpaipal  
[ ] Sura Suwannasri  
✓ Attapol Panurach

เอกสารไม่ควบคุม

B 0316955



Cert.No.: 23P1855  
Page: 2 of 2

Result of calibration:- Without adjustment  
Function:- Absolute Pressure Measurement

Range: 960 hPa to 1030 hPa  
Scale Interval: 1 hPa (The Fifth Estimate)

Increasing Pressure

Applied Pressure (hPa)	958.50	969.59	980.35	990.39	1001.01	1011.15	1020.94	1031.45
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	1.50	0.41	-0.35	-0.39	-1.01	-1.15	-0.94	-1.45

Decreasing Pressure

Applied Pressure (hPa)	1031.45	1021.61	1012.16	1002.38	992.17	982.20	970.69	959.32
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-1.45	-1.61	-2.16	-2.38	-2.17	-2.20	-0.69	0.68

The uncertainty of measurement was  $\pm 0.30$  hPa

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-000-

Aitapoi R

เอกสารไม่ควบคุม  
a 1165504



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3800-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 23H1201  
Page: 1 of 2

Equipment: Dial Thermo-Hygrometer

Manufacturer: Barigo

Model: -

Serial No.: -

ID No.: UAE.EMA.014/2555

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 30 May 2023  
to 06 June 2023

Reference: 2305-0919WSC

Ambient Temperature: (  $25 \pm 3$  ) °C

Relative Humidity: (  $50 \pm 20$  ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Hygro-M2 Dew Point Monitor	5112	2360195	20703	02 Aug 2023
2) Handheld Thermometer With Sensor	1523	3240076	231305	15 Mar 2024

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Standards and Technology (NIST), The United States of America

-Technology Promotion Association (Thailand-Japan), NSQ-ONSAC Accredited No. Calibration 0008

Calibrated by: Somchai Durtwor  
Issue Date: 07 June 2023

Approved Signatory:   
[ ] Chakrit Waeewanjua  
[ ] Ponthippa Tameyakul  
[ ] Viporn Tantiyawutti

เอกสารไม่ควบคุม  
B 0316275



Cert. No.: 23H1201  
Page: 2 of 2

Result of Calibration:-  
Function: Humidity Measurement

Before Adjustment

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	55	14.9	1.6
25.0	60.0	66	6.0	1.7
25.0	80.0	78	-2.0	1.9

Result of Calibration:-  
Function: Humidity Measurement

After Adjustment

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	46	5.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	72	-8.0	1.9

Result of Calibration:-  
Function: Temperature Measurement

Without Adjustment

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
19.987	20.0	0.013	0.72
30.016	30.0	-0.016	0.72
39.944	39.0	-0.944	0.72

UUC\* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k = 2.00$ , providing confidence level approximately 95%.

-000-

Aitapoi R

เอกสารไม่ควบคุม  
a 1165294



United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date: Jan 11, 2023

Equipment: Gas Analyzer (NO<sub>2</sub>) Model: 42C  
Manufacturer: Thermo Scientific Serial Number: 42C-67174-356

Standard Gas Concentration


Sulphur Dioxide (SO <sub>2</sub> )	44.68	PPM	Manufacturer:	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model:	1461
Methane (CH <sub>4</sub> )	-	PPM	Serial Number:	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No.:	EB0143262			
Expiration Date:	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.3	0.30	0.30
Level 2 20.00%	100.0	100.3	0.30	0.30
Level 3 40.00%	200.0	200.7	0.70	0.35
Level 4 60.00%	300.0	300.4	0.40	0.13
Level 5 80.00%	400.0	400.0	0.00	0.00

Remark: Measuring Range 500.0 ppb  
Acceptable Limit  $\pm 5\%$

Average Difference (%) 0.22

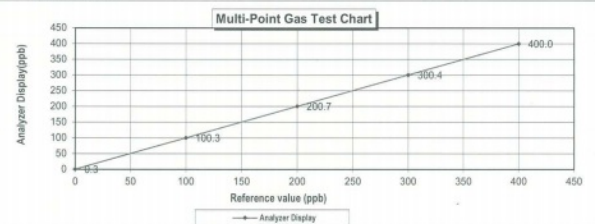

Calculate by  
Aphiwat K  
11.01.23

Approve by  
Ponthippa K  
11.01.23

เอกสารไม่ควบคุม



CERTIFICATE OF ANALYSIS  
Grade of Product: EPA Protocol

Part Number: E04N189E15A0133      Release Number: 22-402135167-1  
Cylinder Number: E04N143262      Cylinder Volume: 44.4 CF  
Laboratory: 24 - Durham (SAP) - NG      Cylinder Pressure: 2015 PSIG  
PGVP Number: 822021      Valve Outlet: 800  
Gas Code: CO,N2,O2,SO2,BAL,N      Certification Date: Jun 21, 2021  
Expiration Date: Jun 21, 2024

Certification performed in accordance with EPA Testable Field of Use and Certification of Operator Calibration Standards (40 CFR 201.27) document EPA 9004-12831 using the zero procedure. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty of stated below with a confidence level of 95%. It does not include any impurities which affect the use of this calibration. Volume of concentrations is given in % by volume. See also the following notes:  
Do Not Use The cylinder below 100 psig, i.e., 6.8 barg or less.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
COX	48.03 PPM	48.96 PPM	G1	± 1.4% NIST Traceable	09/14/2021, 09/21/2021
NITROGEN DIOXIDE	48.03 PPM	48.96 PPM	G1	± 1.4% NIST Traceable	09/14/2021, 09/21/2021
SULFUR DIOXIDE	48.03 PPM	48.96 PPM	G1	± 1.4% NIST Traceable	09/14/2021, 09/21/2021
CARBON MONOXIDE	1800 PPM	1804 PPM	G1	± 1.0% NIST Traceable	09/14/2021, 09/21/2021
NITROGEN	Balance	Balance	G1	± 0.7% NIST Traceable	09/14/2021, 09/21/2021

Type	Lot ID	Cylinder No.	Concentration	Uncertainty	Expiration Date
NITROGEN	22061120	01103863	48.92 PPM NITROGEN DIOXIDE	± 1.0%	Feb 07, 2025
PHOSPHORUS	12388	D639023	9.31 PPM NITROGEN DIOXIDE	± 2.0%	Feb 20, 2023
CHLORINE	431423856/C2	04055581	4.34 PPM NITROGEN DIOXIDE	± 2.1	Feb 18, 2023
NITROGEN	16011345	DC473277	49.38 PPM SULFUR DIOXIDE	± 0.8%	Jun 17, 2022
NITROGEN	4390110	DC473277	80.8 PPM CARBON MONOXIDE	± 0.6%	Nov 15, 2025

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nielsen 6703 AHROBC1332 CO	FIR	Jun 03, 2021
Nielsen 6703 AHROBC1332 NO	FIR	Jun 03, 2021
Nielsen 6703 AHROBC1332 NO2	FIR	Jun 03, 2021
Nielsen 6703 AHROBC1332 SO2	FIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO# 45221022807

CHOSES W/T: 28.40 g

NET WT: 4.73 kg

The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



เอกสารไม่ควบคุม

## MULTI-POINT GAS TEST REPORT

Test Date : Feb 9, 2023

Equipment : Gas Analyzer (SO<sub>2</sub>)      Model : 431  
Manufacturer : Thermo SCIENTIFIC      Serial Number : CM22387067


## Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	44.68	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	45.94	PPM	Model :	1461
Methane (CH <sub>4</sub> )	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	E04N143262			
Expiration Date :	Jun 24, 2024			

## Dilutor Detail

## Multi-point gas test data

	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	0.60	0.60	0.60
Level 3	40.00%	200.0	0.70	0.35	0.35
Level 4	60.00%	300.0	0.90	0.30	0.30
Level 5	80.00%	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)		
Acceptable Limit ± 5%			0.25		

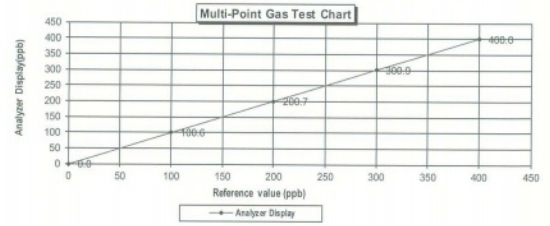

Calculate by

Strichan Sangsri  
9/2/23

Approved by

Patron  
9/2/23

Page 1 of 1

เอกสารไม่ควบคุม



## THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## Calibration Certificate

Issued by : Calibration &amp; Test Section : Meteorological Instruments Bureau

Date of Issue : 10 April, 2023

Certification No. 176/23

Page : 1 of 5

Object : WIRELESS ANEMOMETER

Manufacturer : SCARLET

Type : WIRELESS RECEIVER : WL-21

WIND SENSOR : WL-21

Mfg Code : WIRELESS RECEIVER : 2301DR0024

WIND SENSOR : 2301DT0024

Customer : United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1007.5 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER : Theodor Friedrich : Dry No. 8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057

: ThermoSchneider No. 918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. 14220015

: Digital Barometer Vaisala Type PTB330 No. 14320001

Calibrated by : Watchapol Subwat

Signed :

(Authorized Signatory)

Mr. Watchapol Subwat

Mr. Pissat Promsat

for the Chief

Sub-Standard Instrument

เอกสารไม่ควบคุม



## THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## The Result of Calibration

10 April, 2023

Certification No. 176/23

Page : 2 of 5

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Velocity	Velocity	Correction
Ultrasonic Anemometer	m/sec	inches H2O	inches H2O	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	6.9	0.14
9.02	-	-	-	9.0	0.02
11.02	-	-	-	11.0	0.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Wind Aloft Plotting Board.	
U.S. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	

Calibrated by :

Mr. Watchapol Subwat

Mechanical Engineer

Calibration &amp; Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



## The Result of Calibration

Certification No. 176/23

10 April, 2023

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
1013.17	1013	0.17
1013.43	1013	0.43
1014.15	1014	0.15
1014.22	1014	0.22
1009.63	1009	0.63
1009.71	1009	0.71
1009.95	1010	-0.05
1010.31	1010	0.31
1010.72	1011	-0.28
1010.80	1011	-0.20
1011.47	1011	0.47
1011.21	1011	0.21
1011.33	1011	0.33
1011.59	1012	-0.41
1011.89	1012	-0.11
1012.40	1013	-0.60
1008.64	1009	-0.36
1008.80	1009	-0.20
1009.25	1010	-0.75
1009.45	1010	-0.55

Average

0.01

Calibrated by :

Mr. Watcharapol Subwat  
Mechanical Engineer

Calibration &amp; Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



## The Result of Calibration

Certification No. 176/23

10 April, 2023

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
759.94	760	-0.06
760.13	760	0.13
760.67	761	-0.33
760.73	761	-0.27
757.28	757	0.28
757.34	757	0.34
757.52	757	0.52
757.79	758	-0.21
758.10	758	0.10
758.16	758	0.16
758.66	759	-0.34
758.47	758	0.47
758.56	759	-0.44
758.75	759	-0.25
758.98	759	-0.02
759.36	759	0.36
756.54	757	-0.46
756.66	757	-0.34
757.00	757	0.00
757.15	757	0.15

Average

0.01

Calibrated by :

Mr. Watcharapol Subwat  
Mechanical Engineer

Calibration &amp; Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



## The Result of Calibration

Certification No. 176/23

10 April, 2023

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.15	45.3	-0.15
31.05	31.1	-0.05
15.32	15.4	-0.08

Calibrated by :

Mr. Watcharapol Subwat  
Mechanical Engineer

Calibration &amp; Test Section

Meteorological Instruments Bureau


เอกสารไม่ควบคุม





Cert.No.: 23MM331  
Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Electronic Balance  
**Manufacturer :** Mettler Toledo  
**Model :** AB204-S  
**Serial No. :** 1128312528  
**ID No. :** UAE.AIR.019/2550  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
**Location :** Balance Room 2  
**Received order :** 07 April 2023  
**Calibration Date :** 07 April 2023  
**Ambient Temperature :** 15 °C to 40 °C  
**Relative Humidity :** 30 % to 90 %  
**Calibrated by :** Suwit Imjai  
**Approved by :**   
( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
**Issue Date :** 10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written

Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



**Equipment :** Electronic Balance  
**Condition As-Received :** Used Item  
**Reference :** 2304-0015OC-1  
**Procedure used :-**

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

### Condition of this result of calibration

1. Reference standard instruments:-

- | Instruments                 | Model | Serial No. | ID No.  | Test report No. | Due date    |
|-----------------------------|-------|------------|---------|-----------------|-------------|
| 1) Standard Weight Set (E2) | 15884 | 24053      | 70RC007 | MM-0010-22      | 20 Jan 2024 |
2. This certificate is valid only to the item calibrated on date and place of calibration.  
3. This result of calibration was made on requested at the point specified by customer.  
4. This certificate is not certified for any commercial transaction.  
5. This certification is traceable to the International System of Unit.

**Result of calibration** ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

**Range capacity :** 0 g to 220 g **Resolution** 0.0001 g

**Before Adjustment :**

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
( g )	( g )	( g )	( ± mg )	( k )
100	99.9999	+0.0001	0.19	2.03
200	200.0001	-0.0001	0.29	2.00

**After Adjustment :**

1. **Determination of the standard deviation of weighing machine** ( n = 10 )


Applied Weight	Standard Deviation of Reading ( g )
( g )	
100	0.00007
200	0.00007

เอกสารไม่ควบคุม



**Equipment :** Electronic Balance  
**Condition As-Received :** Used Item  
**Reference :** 2304-0015OC-1

Cert.No.: 23MM331  
Page: 3 of 3



Maximum difference between off-center and central loading

Position 1	Position 2	Position 3	Position 4	Position 5	
( g )	( g )	( g )	( g )	( g )	( g )
-0.0001	-0.0002	+0.0004	-0.0001	-0.0006	0.0005

### 3. Departure from nominal value

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
( g )	( g )	( g )	( ± mg )	( k )
Unload	0.0000	0.0000	0.15	2.13
0.1	0.0999	+0.0001	0.15	2.13
1	0.9999	+0.0001	0.15	2.13
5	4.9999	+0.0001	0.15	2.13
10	9.9999	+0.0001	0.15	2.11
20	20.0000	0.0000	0.15	2.11
50	50.0000	0.0000	0.16	2.06
70	69.9999	+0.0001	0.18	2.04
100	99.9999	+0.0001	0.19	2.03
150	150.0003	-0.0003	0.29	2.00
200	200.0005	-0.0005	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



Cert.No.: 23MM332  
Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Electronic Balance  
**Manufacturer :** Mettler Toledo  
**Model :** AB204-S /FACT  
**Serial No. :** B108115858  
**ID No. :** UAE.AIR.016/2555  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
**Location :** Balance Room 2  
**Received order :** 07 April 2023  
**Calibration Date :** 07 April 2023  
**Ambient Temperature :** 15 °C to 40 °C  
**Relative Humidity :** 30 % to 90 %  
**Calibrated by :** Suwit Imjai  
**Approved by :**   
( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
**Issue Date :** 10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written

Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

เอกสารไม่ควบคุม





Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2304-0015OC-2  
Cert.No.: 23MM332  
Page: 2 of 3

**Procedure used :-**

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

**Condition of this result of calibration**

**1. Reference standard instruments:-**

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

**Result of calibration** ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

**Range capacity :** 0 g to 220 g **Resolution** 0.0001 g

**Before Adjustment :**

Applied Weight ( g )	Balance Reading ( g )	Correction ( g )	Measurement Uncertainty ( ± mg )	Coverage Factor ( k )
100	100.0002	-0.0002	0.21	2.06
200	200.0003	-0.0003	0.29	2.00

**After Adjustment :**

**1. Determination of the standard deviation of weighing machine** ( n = 10 )

Applied Weight ( g )	Standard Deviation of Reading ( g )
100	0.00009
200	0.00007

เอกสารไม่ควบคุม




Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2304-0015OC-2  
Cert.No.: 23MM332  
Page: 3 of 3

**Result of calibration**

**2. Effect of off center loading**

A mass of 100 g was placed to various position on the pan.  
The weighing machine reading error obtained is given in the table



Maximum difference between  
off-center and central loading  
( g )

Position 1 ( g )	Position 2 ( g )	Position 3 ( g )	Position 4 ( g )	Position 5 ( g )
+0.0001	-0.0003	+0.0003	+0.0006	+0.0002

0.0005

**3. Departure from nominal value**

Applied Weight ( g )	Balance Reading ( g )	Correction ( g )	Measurement Uncertainty ( ± mg )	Coverage Factor ( k )
Unload	0.0000	0.0000	0.18	2.17
0.1	0.0999	+0.0001	0.18	2.17
1	0.9998	+0.0002	0.18	2.17
5	5.0000	0.0000	0.18	2.17
10	10.0000	0.0000	0.18	2.17
20	20.0000	0.0000	0.18	2.15
50	50.0001	-0.0001	0.19	2.11
70	70.0001	-0.0001	0.20	2.07
100	100.0002	-0.0002	0.21	2.06
150	150.0004	-0.0004	0.29	2.00
200	200.0005	-0.0005	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23MM333  
Page.: 1 of 3

**Certificate of Calibration**

**Equipment :** Electronic Balance  
**Manufacturer :** Mettler Toledo  
**Model :** XP6  
**Serial No. :** B322373893  
**ID No. :** UAE.AIR.019/2556  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
**Location :** Balance Room 2  
**Received order :** 07 April 2023  
**Calibration Date :** 07 April 2023  
**Ambient Temperature :** 15 °C to 40 °C  
**Relative Humidity :** 30 % to 90 %  
**Calibrated by :** Suwit Imjai  
**Approved by :**   
( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
**Issue Date :** 10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written

Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2304-0015OC-3  
Cert.No.: 23MM333  
Page: 2 of 3

**Procedure used :-**

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

**Condition of this result of calibration**

**1. Reference standard instruments:-**

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

**Result of calibration** ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

**Range capacity :** 0 g to 6.1 g **Resolution** 0.000001 g

**Before Adjustment :**

Applied Weight ( g )	Balance Reading ( g )	Correction ( g )	Measurement Uncertainty ( ± mg )	Coverage Factor ( k )
3	2.999987	+0.000013	0.026	2.00
6	6.000003	-0.000003	0.036	2.00

**After Adjustment :**

**1. Determination of the standard deviation of weighing machine** ( n = 10 )

Applied Weight ( g )	Standard Deviation of Reading ( g )
3	0.0000027
6	0.0000030


เอกสารไม่ควบคุม





Equipment : Electronic Balance  
 Condition As-Received : Used Item  
 Reference : 2304-0015OC-3

Cert.No.: 23MM333  
 Page: 3 of 3



## 2. Effect of off center loading

A mass of 2 g was placed to various position on the pan.  
 The weighing machine reading error obtained is given in the table

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)	Maximum difference between off-center and central loading (g)
-0.000006	-0.000007	-0.000007	-0.000010	-0.000002	0.000004

## 3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
Unload	0.000000	0.000000	0.0060	2.37
0.01	0.009998	+0.000002	0.0060	2.13
0.05	0.050003	-0.000003	0.0070	2.05
0.1	0.100007	-0.000007	0.0090	2.03
0.15	0.150000	0.000000	0.011	2.00
0.17	0.169998	+0.000002	0.014	2.00
0.2	0.200002	-0.000002	0.014	2.00
1.5	1.500001	-0.000001	0.020	2.00
3	2.999990	+0.000010	0.026	2.00
4.5	4.499994	+0.000006	0.036	2.00
6	5.999982	+0.000018	0.036	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

## Agilent CrossLab Start Up Services

## Agilent 8890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure consistent performance and long instrument life.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

เอกสารไม่ควบคุม

## Agilent 8890 GC Preventive Maintenance Checklist

## Introduction

### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

### Important Customer Web Links

- For more information about Agilent Technologies services, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The Agilent Community is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access Agilent University, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful Agilent Resource Center web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our Support Home page <http://www.agilent.com/search/support>.
- Videos about specific preparation requirements for your instrument can be found by searching the Agilent YouTube channel at <https://www.youtube.com/user/agilent>.

เอกสารไม่ควบคุม

## Agilent 8890 GC Preventive Maintenance Checklist

## Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the fields for page numbers at the foot of each selected page.
- Complete the total number of pages field in the Service Completion section.
- Ask the customer to sign the Service Completion section including the customer's and your signature.

## Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any modification.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

เอกสารไม่ควบคุม

## System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	CN1945A066
Instrument System Site and Location	VAE GCMS (405)

List System Component Product Numbers	List the Serial Numbers of each Component
1. 87922A	CN1945A066
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	
10.	

## Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 4 of 9 

เอกสารไม่ควบคุม

## Preventive Maintenance Procedure

## Clean and inspect GC

- ☒ Unplug power cord from the power source.
- ☒ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☒ Inspect internal connectors for proper contact and placement.
- ☒ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☒ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☒ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☒ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

## Inlet and detector consumable replacement

- ☒ Replace the split vent trap cartridge filter using the Maintenance procedure from either the Browser User interfaces on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☒ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☒ For the inlets installed, perform inlet maintenance using the Maintenance procedure from the Browser User interfaces. Record the results. (Leak and Restriction Test)
- ☐ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination - clean as necessary.

## Zero Sensors and Leak test

- ☒ Zero all pressure sensors using the Browser interface.
- ☒ Perform inlet pressure decay test(s) from the diagnostics screen on the Browser User interface. Record if test passed or failed in the results table.

Note: If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 5 of 9 

เอกสารไม่ควบคุม

## ALS Maintenance

- ☒ Section NOT applicable
- ☐ Check all cabling and configuration settings between GC, tray, and injectors.
- ☐ Vacuum or remove any dust, especially around fans.
- ☐ Check operation of all fans.
- ☐ Check syringe for smooth plunger operation.
- ☐ Check for smooth operation of the needle support - clean if necessary

## Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions
- ☒ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☐ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

## Signature Page


## Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review with the customer this service, parts replaced, and test results obtained.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

## PM Test Results Table

Test description	Before PM Service	After PM Service
Front detector output	N/A	N/A
Back detector output	N/A	N/A
AUX 1 detector output	N/A	N/A
AUX 2 detector output	N/A	N/A
Test description	Expected test result	Actual test result
Leak and Restriction Test after front inlet maintenance	Pass	Pass
Leak and Restriction Test after back inlet maintenance	Pass	N/A
Leak and Restriction Test after front inlet Split Vent Trap replacement	Pass	Pass
Leak and Restriction Test after back inlet Split Vent Trap replacement	Pass	N/A
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	N/A

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 6 of 9 

เอกสารไม่ควบคุม

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 7 of 9 

เอกสารไม่ควบคุม



## PM Parts List Table

Note: The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Split	5188-6496	8890 GC	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2295	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	8890 GC	N/A
PP Inlet PM kit	5188-6498	8890 GC	N/A
Split vent from PM kit, single seal/edge (for MMI, PTV & VI)	5188-6495	8890 GC	N/A
MMI Cleaning Kit	G3510-60820	8890 GC	N/A
PTV Septumless Head Rebuild Kit	5182-9747	8890 GC	N/A
PTV Septumless Head Rebuild Kit	5182-9747	8890 GC	N/A
Ignitor (glow plug) assembly with O-ring	19231-60680	8890 GC	N/A
FID Collector Rebuild/Cleaning Kit	G1531-67000	8890 GC	N/A
FID Collector Replacement Kit	G1531-67001	8890 GC	N/A
Standard .011-inch FID Jet	5200-0176	8890 GC	N/A
Universal .018-inch FID Jet	5200-0177	8890 GC	N/A

## Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

## Service Completion

Service request number 600 5953599 Date service completed 14 June 2023  
 Agilent signature SWT Customer signature \_\_\_\_\_  
 Total number of pages in this document 9 pages

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 8 of 9

เอกสารไม่ควบคุม

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 9 of 9

เอกสารไม่ควบคุม



## Calibration Certificate

Certificate No.: 2301846-001-01  
 Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
 Address: 3 Soi Udomsuk 41, Sukhumvit Road,  
 Bangchack, Prakanong, Bangkok 10260

Page 1 of 5

Equipment: pH Meter  
 Manufacturer: Mettler Toledo  
 Model: SevenEasy TM S20 pH  
 Serial No.: 1231155210  
 ID No.: UAE.WAT.010/2553  
 Order No.: 2301846  
 Operation No.: 2301846-001  
 Date of Receipt: 17 February 2023  
 Date of Calibration: 24 February 2023

Calibrated by Mr.Worapob Sooktong Scientist Approved by N. Nittapol Niyomchart (Mr.Nittapol Niyomchart) Specialist, Division of Calibration Laboratory Responsible for the Technical Management Team  
 Date of Issue: 24 February 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

Certificate No.: 2301846-001-01  
 Equipment: pH Meter Resolution: 0.01 pH ; 1 mV  
 Manufacturer: Mettler Toledo Model: SevenEasy TM S20 pH  
 Serial No.: 1231155210 Type: Bench top  
 ID No.: UAE.WAT.010/2553

Date of Calibration: 24 February 2023 Page 2 of 5

Location: Chemical Calibration Laboratory, National Food Institute  
 Environment Condition: Ambient Temperature: ( 25.1 ± 1.5 ) °C Relative Humidity: ( 50 ± 5 ) %  
 Condition of Equipment: Good Condition  
 Condition of this Results of Calibration

1. Calibration Method In house method : W-CC-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fluke	22E1959	17 June 2023
2.2 Digital Thermometer	2709007	Fluke	CC 650577-01	30 October 2023
2.3 Thermo-Hygro Meter	NFI.BTH 007/18	PONPE 490	QR22-0886	26 April 2023
Certified Reference Material	Lot No.	Manufacturer	Ref No.	Expiry Date
2.4 pH buffer 4.008 (Primary pH buffer Solution)	832606	CPAchem	PH216.L5	8 August 2024
2.5 pH buffer 6.865 (Primary pH buffer Solution)	832607	CPAchem	PH217.L5	8 August 2024
2.6 pH buffer 10.01 (Primary pH buffer Solution)	832609	CPAchem	PH220.L5	8 August 2023
2.7 pH buffer 7.00 (Standard pH buffer Solution)	832610	CPAchem	PH107.L5	8 August 2023

3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments No.2.2	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Instruments No.2.3	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0292
3.4 Certified Reference Material No. 2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No.2.7	traceable to	BIM RefN H-27 LotN 04.06.2021; BIM RefN H-28 LotN 28.05.2021; BIM RefN H-27 LotN 04.06.2021; BIM RefN H-28 LotN 28.05.2021, the Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

## Calibration Report

**Certificate No.:** 2301846-001-01  
**Equipment:** pH Meter  
**Resolution:** 0.01 pH ; 1 mV  
**Manufacturer:** Mettler Toledo  
**Model:** SevenEasy TM S20 pH  
**Serial No.:** 1231155210  
**Type:** Bench top  
**ID No.:** UAE.WAT.010/2553  
**Date of Calibration:** 24 February 2023 Page 3 of 5

**Calibration Results:**  
1. Calibration of pH Meter (Manual Temperature Compensation at 25 °C)

Nominal pH	DC Voltage Standard (mV)	Average Indicator Reading		Uncertainty (mV)	Coverage Factor (k)
		mV	pH		
0	414.120	414	0.00	0.58	2.00
2	295.814	296	2.00	0.58	2.00
4	177.464	178	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.000	0	7.00	0.58	2.00
8	-59.158	-59	8.00	0.58	2.00
10	-177.460	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.117	-414	14.00	0.58	2.00

2. Calibration of pH Meter with Electrode (Manual Temperature Compensation at 25 °C)  
**Equipment:** pH Electrode  
**Type:** Combined Electrode  
**Manufacturer:** Mettler Toledo  
**Model:** InLab Solids  
**Serial No.:** 9018311  
**ID No.:** N/A  
**Performance of Electrode system:** (Three-Point Calibration at pH 4, pH 7 and pH 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty (± pH)	Coverage Factor (k)
	pH	mV			
4.008	4.01	186	-	0.0071	2.00
6.865	6.90	19	97.88	0.0075	2.00
10.008	10.01	-160	97.29	0.0095	2.00
6.985	6.99	15	-	0.0092	2.00

F-CS-012 Revision: 01 Date: 20-04-65

*N. Niyomchart*

เอกสารไม่ควบคุม



## Calibration Report

**Certificate No.:** 2301846-001-01  
**Equipment:** Digital Thermometer with RTD  
**Resolution:** 0.1 °C  
**Model:** SevenEasy TM S20 pH  
**Serial No.:** 1231155210  
**ID No.:** UAE.WAT.010/2553  
**Manufacturer:** Mettler Toledo  
**Date of Calibration:** 24 February 2023 Page 4 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute  
**Environment Condition:** Ambient Temperature 25 °C ± 1 °C  
Relative Humidity 48 % ± 3 %

### Condition of this results of Calibration:

1. Calibration Method : - In house method: W-TE-025 by comparison with standard thermometer.  
- The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.  
- The temperature scale in use at this laboratory is the International Temperature scale of 1990 (ITS-90).
2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1523	2118154	PSL-T 0673/65	07-Jun-23	TISTR
Platinum Resistance Thermometer (PRT)	5627A	877332			

Support Equipment : - Low Temperature Bath (Micro Bath), Model: 7103, S/N: A39538,AN65 A85181.

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

*N. Niyomchart*

เอกสารไม่ควบคุม



## Calibration Report

**Certificate No.:** 2301846-001-01  
**Equipment:** Digital Thermometer with RTD  
**Resolution:** 0.1 °C  
**Model:** SevenEasy TM S20 pH  
**Serial No.:** 1231155210  
**ID No.:** UAE.WAT.010/2553  
**Manufacturer:** Mettler Toledo  
**Date of Calibration:** 24 February 2023 Page 5 of 5

**Calibration point:** 15.0, 25.0 and 35.0 °C

**Calibration result:**  
- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.  
- Description of probe, model : - S/N : -  
Dimension of probe : Diameter 9 mm., Length 120 mm.,  
Sheath material : Stainless Steel

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.1	15.015	- 0.1	0.11
25.0	25.014	0.0	0.11
35.1	35.016	- 0.1	0.11

### Note

- UUC\* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

*N. Niyomchart*

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม



## Calibration Certificate

**Certificate No.:** 2302181-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 5

**Equipment:** pH Meter  
**Manufacturer:** METTLER TOLEDO  
**Model:** SevenEasy pH  
**Serial No.:** 1230525212  
**ID No.:** UAE.WAS.003/2553  
**Order No.:** 2302181  
**Operation No.:** 2302181-001  
**Date of Receipt:** 14 March 2023  
**Date of Calibration:** 24 March 2023

**Calibrated by:** Mr.Pheraphat Tuanjit  
**Scientist**  
**Approved by:** *N. Niyomchart*  
(Mr.Nuttapol Niyomchart)  
Specialist, Division of Calibration Laboratory  
Responsible for the Technical Management Team  
**Date of Issue:** 24 March 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม





## Calibration Report

**Certificate No.:** 2302181-001-01  
**Equipment:** pH Meter  
**Resolution:** 0.01 pH ; 1 mV  
**Manufacturer:** METTLER TOLEDO  
**Model:** SevenEasy pH  
**Serial No.:** 1230525212  
**Type:** Bench top  
**ID No.:** UAE.WAS.003/2553

**Date of Calibration:** 24 March 2023 **Page 2 of 5**

**Location:** Chemical Calibration Laboratory, National Food Institute  
**Environment Condition:** Ambient Temperature: ( 23.4 ± 1.5 ) °C Relative Humidity: ( 52 ± 3 ) %  
**Condition of Equipment:** Good Condition

### Condition of this Results of Calibration

1. Calibration Method  
In house method : W-CC-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)
2. Reference Standards / Certified Reference Material
 

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fuke	22E1959	17 June 2023
2.2 Digital Thermometer	2709007	Fuke	CC-650557-01	30 October 2023
2.3 Thermo-Hygro Meter	NFLBTH003/17	PONPE	TE 650555-01	21 September 2023

Certified Reference Material	Lot No.	Manufacturer	Ref No	Expires Date
2.4 pH buffer 4.008 (Primary pH buffer Solution)	873608	CPAchem	PH216.L5	16 February 2025
2.5 pH buffer 6.865 (Primary pH buffer Solution)	873609	CPAchem	PH217.L5	16 February 2025
2.6 pH buffer 10.01 (Primary pH buffer Solution)	873611	CPAchem	PH220.L5	16 February 2024
2.7 pH buffer 7.00 (Standard pH buffer Solution)	873612	CPAchem	PH107.L5	16 February 2024
3. This certification is traceable to The International System of Unit (SI Unit)
 

3.1 Instruments No.2.1	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.008
3.2 Instruments No.2.2	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Instruments No.2.3	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.4 Certified Reference Material No. 2.4 to 2.6	traceable to	Primary measurement method- Hammett cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No.2.7	traceable to	BIM Ref N Hi-13 Lot N 25.05.2022; BIM Ref N Hi-16 Lot N 02.06.2022; BIM Ref N Hi-13 Lot N 25.05.2022; BIM Ref N Hi-16 Lot N 02.06.2022, the Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.

F-CS-012 Revision: 01 Date: 20-04-65

*N. Nigudat*

## Calibration Report

**Certificate No.:** 2302181-001-01  
**Equipment:** pH Meter  
**Resolution:** 0.01 pH ; 1 mV  
**Manufacturer:** METTLER TOLEDO  
**Model:** SevenEasy pH  
**Serial No.:** 1230525212  
**Type:** Bench top  
**ID No.:** UAE.WAS.003/2553

**Date of Calibration:** 24 March 2023 **Page 3 of 5**

**Calibration Results:**  
1. Calibration of pH Meter ( Manual Temperature Compensation at 25 °C )

Nominal pH	DC Voltage Standard ( mV )	Average Indicator Reading		Uncertainty ( ±mV )	Coverage Factor ( k )
		mV	pH		
0	414.120	414	0.00	0.58	2.00
2	295.814	296	2.00	0.58	2.00
4	177.464	178	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.000	0	7.00	0.58	2.00
8	-59.158	-59	8.00	0.58	2.00
10	-177.460	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.117	-414	14.00	0.58	2.00

2. Calibration of pH Meter with Electrode ( Manual Temperature Compensation at 25 °C )

**Equipment:** pH Electrode **Type:** Combined Electrode  
**Manufacturer:** METTLER TOLEDO **Model:** InLab Solids  
**Serial No.:** 1156883 **ID No.:** N/A

**Performance of Electrode system** (Three-Point Calibration at pH 4, pH 7 and pH 10)

Certified Value (±25 °C pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty ( ± pH )	Coverage Factor ( k )
	pH	mV			
4.008	4.01	187	-	0.0071	2.00
6.865	6.86	22	97.86	0.0075	2.00
10.010	10.01	-160	97.66	0.0086	2.00
6.985	6.99	14	-	0.0093	2.00

F-CS-012 Revision: 01 Date: 20-04-65

*N. Nigudat*

## Calibration Report

**Certificate No.:** 2302181-001-01  
**Equipment:** Digital Thermometer with RTD (pH Meter)  
**Resolution:** 0.1 °C **Model:** SevenEasy pH  
**Serial No.:** 1230525212 **ID No.:** UAE.WAS.003/2553  
**Manufacturer:** METTLER TOLEDO

**Date of Calibration:** 24 March 2023 **Page 4 of 5**

**Location:** Chemical Calibration Laboratory, National Food Institute  
**Environment Condition:** Ambient Temperature 25 °C ± 1 °C  
Relative Humidity 55 % ± 5 %

### Condition of this results of Calibration:

1. Calibration Method : - In house method: W-TE-025 by comparison with standard thermometer.  
- The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.  
- The temperature scale in use at this laboratory is the International Temperature scale of 1990 ( ITS-90 ).
2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1521	A85997	TE 660039-01	10-Dec-23	NATIONAL FOOD INSTITUTE
Platinum Resistance Thermometer (PRT)	385	509201			

Support Equipment : - Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

*N. Nigudat*

## Calibration Report

**Certificate No.:** 2302181-001-01  
**Equipment:** Digital Thermometer with RTD (pH Meter)  
**Resolution:** 0.1 °C **Model:** SevenEasy pH  
**Serial No.:** 1230525212 **ID No.:** UAE.WAS.003/2553  
**Manufacturer:** METTLER TOLEDO

**Date of Calibration:** 24 March 2023 **Page 5 of 5**

**Calibration point:** 15.0, 25.0 and 30.0 °C

### Calibration result:

- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.
- Description of probe, model : N/A S/N : N/A
- Dimension of probe : Diameter 3 mm., Length 120 mm.,
- Sheath material : N/A

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ( ± °C )
15.2	14.999	- 0.2	0.12
25.2	24.999	- 0.2	0.12
30.2	29.999	- 0.2	0.12

### Note

- UUC\* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

F-CS-012 Revision: 01 Date: 20-04-65

*N. Nigudat*





## Certificate of Calibration

Equipment: CONDUCTIVITY METER  
Model: Lab 955  
Serial No. (or ID.): 16300356  
Manufacturer: SI Analytics  
Electrode Serial No. 16070067  
Condition: In Condition

Certificate No.: C24230059  
Issued Date: 16 March 2023  
Job No.: KSPR2304472  
Page: 1 of 2  
Model: LF413T  
Brand: SI Analytics

Customer: United Analyst and Engineering Consultant Company Limited  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangchak, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature 23 °C ± 2 °C  
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Mr. Atachai Ngamchanat  
Calibration Date: 16 March 2023  
The Method used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14  
Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 838312, 838313, 838316

### Calibration Results:

#### Before Adjustment

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor (k)	Uncertainty (±)
25.000 µS/cm	24.5 µS/cm	0.500 µS/cm	2.00	0.21 µS/cm
1413.0 µS/cm	1403 µS/cm	10.0 µS/cm	2.00	9.0 µS/cm
111.3 mS/cm	108.5 mS/cm	2.80 mS/cm	2.00	0.67 mS/cm

#### After Adjustment ; at 1413 µS/cm

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor (k)	Uncertainty (±)
25.000 µS/cm	24.8 µS/cm	0.200 µS/cm	2.00	0.21 µS/cm
1413.0 µS/cm	1413 µS/cm	0.0 µS/cm	2.00	9.0 µS/cm
111.3 mS/cm	108.8 mS/cm	2.50 mS/cm	2.00	0.67 mS/cm

The End of Certificate

(Mr. Atachai Ngamchanat)

Person in charge

(Mr. Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.  
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).  
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.  
บริษัท ดีเคเอส อีเซีย จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/certifco-thailand

Delivering Growth - In Asia and Beyond.

CAL-FM-C24-09: 12 Sep 2022

บริษัท ดีเคเอส อีเซีย จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/certifco-thailand

Delivering Growth - In Asia and Beyond.

CAL-FM-C24-09: 12 Sep 2022

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

## ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: KSPR2304472

ชนิดเครื่องมือ: CONDUCTIVITY METER รุ่น: Lab 955

หมายเลขเครื่อง: 16300356

ตรวจสอบ (วัน)		รายการตรวจเช็ค	ตรวจสอบ (ตั้ง)		หมายเหตุ
16 Mar 2023			16 Mar 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด ( ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิทช์ ปิด – เปิด เครื่อง (On-Off Switch)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. ขั้วอิเล็กโทรด ( Electrode and Connection Cable )	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl )	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่นเกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ: Electrode วัดอุณหภูมิได้ 25.1°C โดย Control Waterbath ที่ 25.0 ± 0.1°C

Mr. Atachai Ngamchanat

Service Engineer

เอกสารไม่ควบคุม

บริษัท ดีเคเอส อีเซีย จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/certifco-thailand

Delivering Growth - In Asia and Beyond.

CAL-FM-R31-03: 20 Jul 2022



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23MM113  
Page.: 1 of 3

## Certificate of Calibration

Equipment : Electronic Balance  
Manufacturer : Mettler Toledo  
Model : XSR205  
Serial No. : C210685394  
ID No. : UAE.WAO.010/2565  
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
Location : Balance Room  
Received order : 26 April 2023  
Calibration Date : 26 April 2023  
Ambient Temperature : 15 °C to 40 °C  
Relative Humidity : 30 % to 90 %  
Calibrated by : Man Pattanapongpaiboon  
Approved by :   
( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
(✓) Suwit Imjai  
Issue Date : 2 May 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2304-0459OC-2  
Procedure used :-

Cert.No.: 23MM113  
Page: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

#### Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.

5. This certification is traceable to the International System of Unit.

Result of calibration ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

Range capacity :	0 g to 81 g	Resolution	0.00001 g
	81 g to 220 g	Resolution	0.0001 g

Before Adjustment :

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
( g )	( g )	( g )	( ± mg )	( k )
80	79.99992	+0.00008	0.15	2.00
200	199.9995	+0.0005	0.29	2.00

After Adjustment :

1. Determination of the standard deviation of weighing machine ( n = 10 )

Applied Weight	Standard Deviation of Reading ( g )
( g )	
80	0.000007
200	0.00004


เอกสารไม่ควบคุม

a 1159272



Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2304-0459OC-2  
Result of calibration

Cert.No.: 23MM113  
Page: 3 of 3



#### 2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.

The weighing machine reading error obtained is given in the table

Position 1	Position 2	Position 3	Position 4	Position 5	Maximum difference between off-center and central loading
( g )	( g )	( g )	( g )	( g )	( g )
-0.0001	-0.0001	0.0000	-0.0001	-0.0001	0.0001

#### 3. Departure from nominal value

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
( g )	( g )	( g )	( ± mg )	( k )
Unload	0.00000	0.00000	0.014	2.11
0.05	0.04999	+0.00001	0.015	2.09
0.1	0.09999	+0.00001	0.015	2.07
1	1.00000	0.00000	0.018	2.04
5	5.00000	0.00000	0.026	2.00
20	20.00002	-0.00002	0.045	2.00
50	50.00002	-0.00002	0.080	2.00
80	80.00002	-0.00002	0.15	2.00
100	100.00000	0.00000	0.17	2.00
150	150.00000	0.00000	0.29	2.00
200	199.99999	+0.00001	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

a 1159271



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM373  
Page : 1 of 3

## Certificate of Calibration

Equipment : Hot Air Oven  
Manufacturer : Memmert  
Model : UF 55  
Serial No. : B212.0411  
ID No. : UAE.WAO.005/2556  
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
Location : Lab Floor 2  
Received Order : 11 April 2023  
Calibration Date : 11 - 12 April 2023  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
Calibrated by : Krisda Malee

Approved by :   
Approved Signatory

( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
( ) Suwit Imjai

Issue Date : 24 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0053359



Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2304-0156OC-1  
Procedure Used :-

Cert. No.: 23TM373  
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34972A	MY59003411	22LM165	26 Nov 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	27	28
REL.Humid. ( % )	45	44
AC Supply ( Volt )	221	220



Probe Installation Details : Dimension of Chamber :  
a = 5.0 cm D = 0.50 m  
b = 5.0 cm W = 0.80 m  
c = 5.0 cm H = 0.75 m  
Capacity = 0.30 m<sup>3</sup>

Ref. Std. ID No.: @ Calibration Point		
Position :	( 120 to 180 ) °C	( 104 ) °C
1	18-20TC-01	20RTD-2/1
2	18-20TC-02	20RTD-2/2
3	18-20TC-03	20RTD-2/3
4	18-20TC-04	20RTD-2/4
5	18-20TC-05	20RTD-2/5
6	18-20TC-06	20RTD-2/6
7	18-20TC-07	20RTD-2/7
8	18-20TC-08	20RTD-2/8
9 (ref.)	18-20TC-09	20RTD-2/9

เอกสารไม่ควบคุม

a 1158261



Equipment : Hot Air Oven  
 Condition As-Received : Used Item  
 Reference : 2304-0156OC-1  
 Result of Calibration :- ( \* ) Without Adjustment  
 Function of UUC\* : Temperature Source  
 Fresh air setting : Close

Cert. No.: 23TM373  
 Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor k
104.0	104.0	104.0	0.054	0.59	0.95	2
120.0	120.0	120.0	0.12	0.89	1.5	2
180.0	180.0	180.0	0.12	1.5	2.5	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	104.512	104.016	104.542	104.407	103.704	103.729	104.167	104.158	104.001	0.42
120.0	120.317	119.768	120.524	120.232	119.363	119.209	119.888	119.797	119.735	1.1
180.0	180.878	179.819	181.357	180.871	179.303	179.139	180.230	180.055	179.960	1.1

**Average\*** : The average of 30 values in each position.  
**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.  
**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.  
**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.  
**UUC\*** : Unit Under Calibration  
 Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

Walu.

เอกสารไม่ควบคุม

a 1158260



## LS 45/50B/55 - Preventive Maintenance report

Company Name:	United analyst and Engineering Consultant Co.,Ltd.		
Address:	3 Soi Udomsuk 41, Sukumvit Road, Phrakhanong, Bangkok 10260		
User Name :	K. Primpun	WO Number:	WO-01624974
Telephone Number :	02-763-2828	Certificate Number :	FLR1001-2023
Customer Support Engineer :	Tanongsak	P.M. Number	1 of 1
PM Performed: (DD-MMM-YYYY)	2-Feb-2023	Next PM Due Date: (DD-MMM-YYYY)	2-Feb-2024

### Scope

The purpose of this PM is to ensure the continued functionality of the PerkinElmer Fluorescence Spectrophotometer by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

### General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

### Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2009 PerkinElmer, Inc.

### Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose. PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

เอกสารไม่ควบคุม page 1



## Component List

Component Specific Model	Serial #	Software Version	Configuration Notes
LS55	81440	4.00.03	
-	-	-	-
-	-	-	-

## Parts Lists

Test standard Used				
Part Number (if applicable)	Description			
C 520-7440	Stanadard Fluorence Intensity Filter			
B050 7805	Sealed Water Cell			
Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)

เอกสารไม่ควบคุม page 2



## Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

### 1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Perform general inspection of system for cleanliness.

### 2. Optical checks and Clean:

- ☒ Lamp Alignment/Intensity
- ☒ Sample Compartment and Windows
- ☒ Mirror and Grating Alignment
- ☒ Filter Wheel
- ☒ Cell Holder Alignment

### 3. Mechanical:

- ☒ Physical inspection – Please write any comments in the additional comments section.
- ☒ Grating Drive Mechanism.
- ☒ Slit Drive Mechanism.
- ☒ Sample Holder

### 4. Test:

- ☒ Emission Wavelength Accuracy.

Emission Wavelength Accuracy		Actual Value	Validation Criteria
Target Peak (nm)		(nm)	Accuracy Limit ±/-(nm)
Target Peak # 1	253.7	254.0	± 1.0 nm
Target Peak # 2	507.3	507.4	± 1.0 nm
Target Peak # 3	626.0	625.8	± 1.0 nm

เอกสารไม่ควบคุม page 3



☒ Excitation Wavelength Accuracy.

Excitation Wavelength Accuracy		Actual Value	Validation Criteria
Target Peak (nm)		(nm)	Accuracy Limit +/- (nm)
Target Peak # 1	253.7	253.2	± 1.0 nm
Target Peak # 2	365.0	365.4	± 1.0 nm
Target Peak # 3	507.3	508.0	± 1.0 nm

☒ Emission Slit calibration.

Emission Slit		Actual Value	Validation Criteria
Target Value (nm)		(nm)	Accuracy Limit +/- (nm)
Target Peak # 1	2.5	2.63	± 0.5 nm
Target Peak # 2	5.0	4.75	± 0.5 nm
Target Peak # 3	10.0	9.99	+ 1.0 / - 0.5 nm

☒ Excitation Wavelength Repeatability.

Emission Slit		Actual Value	Validation Criteria
Target Value (nm)		(nm)	Accuracy Limit +/- (nm)
Target Peak # 1	2.5	2.57	± 0.5 nm
Target Peak # 2	5.0	5.08	± 0.5 nm
Target Peak # 3	10.0	9.80	+ 1.0 / - 0.5 nm

เอกสารไม่ควบคุม Page 4

☒ Water Raman Sensitivity

	Actual Value
Signal to Noise	288 : 1
Drift	0.03

☒ Stray Light

	Actual Value
Stray Light at 290nm	2.64
Stray Light at 300nm	0.77

#### 5. Accessory (where applicable):

- ☐ Micro Plate Reader
- ☐ Integrating Sphere
- ☐ Multi Cell Holder
- ☐ Water Jacketed Cell Holder
- ☐ etc. ....

#### 6. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand
- ☒ Attach PM sticker.
- ☐ Update Logbook.

เอกสารไม่ควบคุม Page 5

### Additional Comments

Additional Comments Regarding the PM
Reference intensity low





### Review

The PM checks and if applicable performance tests for LS 45/50B/55 have been completed.

This LS 45/50B/55 Passes ☒ Fails ☐ the PM.

Review of Preventive Maintenance:	
Authorized PerkinElmer Representative:	Date: 2-Feb-23 (DD-MMM-YYYY)
Authorized Customer Representative:	Date: 2-Feb-23 (DD-MMM-YYYY)

เอกสารไม่ควบคุม Page 6

 DQE Services Co., Ltd. 32 Soi Ladprao-Wanghin 55, Ladprao-Wanghin Rd., Ladprao, Bangkok 10230 Phone : +66 (0)2 538 2054, Email : dqeservicesinfo@gmail.com		
<b>CERTIFICATE OF CALIBRATION</b>		
Certificate No. :	SP23-021	Page 1 of 5
Customer :	United Analyst and Engineering Consultant Co., Ltd. (Head Office)	
Address :	3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260	
Location of calibration :	Laboratory 315	
Equipment :	UV-Vis Spectrophotometer	
Manufacturer :	Agilent Technologies	
Model :	Cary 60	
Serial No. :	MY15410009	
ID No. :	N/A	
Received Date :	20 May 2023	
Calibration Date :	20 May 2023	
Issue Date :	23 May 2023	
Condition Instrument :	Good	
Calibrated by :	 (Mr. Tanawut Rittidach) Technical Manager	Approved by :  (Ms. Chonthicha Sangnern) Quality Manager
The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only. The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.		

เอกสารไม่ควบคุม



## REPORT OF CALIBRATION

Certificate No. : SP23-021

Page 2 of 5

Environment Condition : Ambient Temperature  $25 \pm 5$  °C

Relative humidity  $55 \pm 20$  %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	95935	22 October 2023
Absorbance Standard set	25757	95929	22 October 2023
Wavelength Standard set	25806	95916	22 October 2023
Wavelength Standard set	25758	95915	22 October 2023

Traceability This certification is traceable to the International System of Unit maintained at National

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม



## REPORT OF CALIBRATION

Certificate No. : SP23-021

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5787	0.5742	0.0045	0.0031	2.00
	1.0490	1.0423	0.0067	0.0029	2.00
	2.1900	2.1847	0.0053	0.0075	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5607	0.5577	0.0030	0.0034	2.00
	1.0247	1.0234	0.0013	0.0035	2.00
	2.1229	2.1171	0.0058	0.0088	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5236	0.5184	0.0052	0.0029	2.00
	0.9634	0.9607	0.0027	0.0029	2.00
	1.9763	1.9715	0.0048	0.0081	2.00
546.1	0.0000	-0.0001	0.0001	0.0028	2.00
	0.5191	0.5159	0.0032	0.0031	2.00
	1.0003	0.9980	0.0023	0.0033	2.00
	1.9987	1.9917	0.0070	0.0087	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5523	0.5501	0.0022	0.0030	2.00
	1.0809	1.0808	0.0001	0.0030	2.00
	2.0391	2.0336	0.0055	0.0081	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5601	0.5585	0.0016	0.0031	2.00
	1.0512	1.0485	0.0027	0.0030	2.00
	1.9294	1.9317	-0.0023	0.0083	2.00

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม



## REPORT OF CALIBRATION

Certificate No. : SP23-021

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7478	0.7436	0.0042	0.0058	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8686	0.8648	0.0038	0.0064	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2912	0.2908	0.0004	0.0052	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6448	0.6398	0.0050	0.0058	2.00

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม



## REPORT OF CALIBRATION

Certificate No. : SP23-021

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.5	0.31	0.18	2.00
334.06	333.5	0.56	0.18	2.00
360.93	360.3	0.63	0.18	2.00
418.59	418.0	0.59	0.18	2.00
445.94	445.3	0.64	0.18	2.00
453.66	453.0	0.66	0.18	2.00
460.02	459.6	0.42	0.18	2.00
536.59	536.4	0.19	0.18	2.00
637.98	638.3	-0.32	0.18	2.00
431.38	431.0	0.38	0.18	2.00
472.50	472.5	0.00	0.18	2.00
513.47	513.5	-0.03	0.18	2.00
528.88	529.0	-0.12	0.18	2.00
573.17	573.0	0.17	0.18	2.00
585.35	585.0	0.35	0.20	2.00
684.40	684.5	-0.10	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.5	0.05	0.18	2.00
807.03	807.0	0.03	0.18	2.00
879.28	879.5	-0.22	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%

- \* Indicates non TISI accredited

- End of Certificate -

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม





Request No. 25-66 / 0323

MTC. ACL.No. 387 / 66

## CALIBRATION CERTIFICATE

NOMENCLATURE : 1. Atomic Absorption Spectrophotometer "Agilent Technologies"

Model AA240FS, Serial No. MY13160001

2. Working standard solution "Inorganic Ventures"

Multi Analyte Custom Grade Solution, Lot No. S2-MEB708640

SUBMITTED BY : United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk41, Sukhumvit Road, Bangkok, Prakanong, Bangkok 10260

CALIBRATION PROCEDURE : 1. Performance Verification of Atomic Absorption Spectrophotometer (WI-500-02-30)

2. Estimation Uncertainty of Measurement in Analytical Chemistry (QP-513)

CALIBRATION RANGE: 0.02,0.10,0.30,0.50,0.70 mg/l at 228.8 nm.Cd, 0.10,0.20,0.30,0.50,0.70 mg/l at 357.9 nm.Cr, 0.05,0.10,0.30,0.50,0.70 mg/l at 324.7 nm.Cu, 0.10,0.30,0.50,0.70,1.00 mg/l at 248.3 nm.Fe, 0.20,0.50,0.70,1.00,1.50 mg/l at 217.0 nm.Pb, 0.05,0.10,0.30,0.50,0.70 mg/l at 279.5 nm.Mn, 0.10,0.30,0.50,0.70,1.00 mg/l at 232.0 nm.Ni, 0.05,0.10,0.30,0.50,0.70 mg/l at 213.9 nm.Zn



CALIBRATION DATE : 2 February 2023

REFERENCE MATERIAL : Traceable to NIST "Carlo Erba", "PanReac AppliChem"

Cadmium Lot No. 1152457, Chromium Lot No. 1793249, Copper Batch No. T117098A, Iron Batch No. T126087A, Lead Lot No. 1227873, Manganese Batch No. T109228A, Nickel Batch No. T270178A, Zinc Batch No. T820140A

AMBIENT CONDITIONS : Temperature 22 °C Relative humidity 58 %

The Atomic Absorption Spectrophotometer has been calibrated against Reference Material traceable to National Institute of Standards and Technology ( NIST ) by The Analytical Chemistry Laboratory. The results are attached herewith.

Calibrated by   
( Mr. Danai Srithongkum )Approved by   
( Miss Sutadha Deawtong )2.   
( Mr. Atipat Ratana )Senior Technical Officer  
Acting Director of Analytical Chemistry Laboratory

Ref. 2015266012600366001

Issued Date : 15 February 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.


FMBL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Tel. (66) 0 2577 9009  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtg@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2374 6292  
Fax. (66) 0 2374 6292  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม



Request No. 25-66 / 0323

1 / 5

MTC. ACL. No. 387 / 66

## CALIBRATION DATA

## 1. Noise Level

Element	Cd	Cr	Cu	Fe	Pb	Mn	Ni	Zn
Absorbance	0.0020	0.0000	0.0008	0.0000	-0.0009	0.0021	-0.0016	-0.0022
	0.0015	0.0006	0.0005	-0.0009	-0.0014	0.0018	0.0002	-0.0023
	0.0014	0.0006	0.0010	-0.0009	0.0015	0.0008	-0.0004	-0.0015
	0.0021	-0.0008	0.0013	-0.0010	0.0005	0.0005	-0.0008	-0.0004
	0.0020	-0.0012	0.0004	0.0003	-0.0004	0.0001	-0.0024	-0.001
	0.0021	-0.0011	0.0011	0.0003	0.0006	0.0009	-0.0002	-0.0013
	0.0017	-0.0009	0.0001	-0.0015	0.0010	0.0007	0.0001	-0.0016
	0.0024	-0.0012	0.0004	-0.0002	0.0008	-0.0005	-0.0012	-0.0019
	0.0011	-0.0002	0.0015	-0.0004	0.0004	0.0008	-0.0003	-0.0017
	0.0017	0.0000	0.0009	0.0004	0.0001	0.0015	-0.0009	-0.0024
	0.0019	-0.0004	0.0004	0.0000	0.0006	0.0010	-0.0005	-0.0016
	0.0016	-0.0025	0.0003	0.0005	0.0009	-0.0004	-0.0013	-0.0016
	0.0018	-0.0014	0.001	-0.0009	-0.0006	0.0010	-0.0004	-0.0017
	0.0019	-0.0006	0.0011	-0.0008	0.0011	0.0004	-0.0003	-0.0005
	0.0024	0.0003	0.0005	-0.0012	-0.0002	0.0012	-0.0006	-0.0011
	0.0023	-0.0012	0.0006	-0.0007	0.0002	0.0014	-0.0012	-0.0013
	0.0020	-0.0014	0.0009	-0.0018	0.0003	0.0012	-0.0012	-0.0013
	0.0010	-0.0015	0.0002	0.0004	0.0017	0.0011	-0.0018	-0.0013
	0.0016	-0.0011	0.0013	0.0003	0.0007	0.0026	-0.0006	-0.0006
	0.0001	-0.0007	0.0009	-0.0003	0.0008	0.0008	0.0000	-0.0001
Average Absorbance	0.002	-0.001	0.001	0.000	0.000	0.001	-0.001	-0.001

Continue 2 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Tel. (66) 0 2577 9009  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtg@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2374 6292  
Fax. (66) 0 2374 6292  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม

Request No. 25-66 / 0323

2 / 5

MTC. ACL. No. 387 / 66

## 2. Precision

Element	Conc. (mg/l)	Absorbance										Ave. Abs.	SD	%RSD
Cd	0.02	0.0085	0.0084	0.0090	0.0089	0.0089	0.0090	0.0086	0.0092	0.0090	0.0089	0.009	0.0003	2.88
	0.30	0.0995	0.1001	0.1007	0.1004	0.1004	0.0995	0.0997	0.0998	0.0999	0.0996	0.100	0.0005	0.45
	0.70	0.2238	0.2229	0.2244	0.2249	0.2243	0.2235	0.2231	0.2251	0.2240	0.224	0.0007	0.33	
Cr	0.10	0.0088	0.0087	0.0094	0.0086	0.0086	0.0091	0.0099	0.0095	0.0076	0.0085	0.009	0.0006	7.25
	0.30	0.0257	0.0265	0.0255	0.0270	0.0266	0.0258	0.0261	0.0262	0.0274	0.0262	0.026	0.0006	2.25
	0.70	0.0573	0.0590	0.0580	0.0576	0.0578	0.0579	0.0593	0.0599	0.0586	0.0594	0.058	0.0009	1.51
Cu	0.05	0.0083	0.0084	0.0084	0.0075	0.0086	0.0086	0.0081	0.0080	0.0087	0.0092	0.008	0.0005	5.45
	0.30	0.0430	0.0444	0.0426	0.0429	0.0435	0.0432	0.0428	0.0441	0.0427	0.0436	0.043	0.0006	1.41
	0.70	0.0981	0.0992	0.0990	0.0997	0.0977	0.0986	0.0990	0.0982	0.0988	0.0980	0.099	0.0006	0.63
Fe	0.10	0.0109	0.0104	0.0087	0.0100	0.0087	0.0094	0.0102	0.0092	0.0094	0.0100	0.010	0.0007	7.53
	0.50	0.0456	0.0442	0.0450	0.0444	0.0450	0.0455	0.0455	0.0441	0.0446	0.0444	0.045	0.0006	1.27
	1.00	0.0904	0.0901	0.0891	0.0876	0.0873	0.0901	0.0876	0.0886	0.0879	0.0901	0.089	0.0012	1.38
Pb	0.20	0.0093	0.0099	0.0104	0.0102	0.0104	0.0109	0.0102	0.0103	0.0115	0.0117	0.010	0.0007	6.85
	0.70	0.0344	0.0336	0.0336	0.0328	0.0338	0.0346	0.0336	0.0331	0.0343	0.0350	0.034	0.0007	2.02
	1.50	0.0709	0.0718	0.0706	0.0713	0.0698	0.0718	0.0712	0.0713	0.0715	0.0719	0.071	0.0006	0.90
Mn	0.05	0.0115	0.0130	0.0131	0.0127	0.0135	0.0136	0.0124	0.0133	0.0124	0.0130	0.013	0.0006	4.88
	0.30	0.0709	0.0700	0.0714	0.0704	0.0700	0.0705	0.0714	0.0698	0.0694	0.0700	0.070	0.0007	0.96
	0.70	0.1619	0.1633	0.1646	0.1638	0.1646	0.1614	0.1632	0.1614	0.1636	0.1652	0.163	0.0014	0.83
Ni	0.10	0.0113	0.0105	0.0113	0.0114	0.0110	0.0113	0.0117	0.0112	0.0107	0.0117	0.011	0.0004	3.45
	0.50	0.0509	0.0517	0.0508	0.0502	0.0517	0.0516	0.0516	0.0523	0.0518	0.0503	0.051	0.0007	1.36
	1.00	0.0997	0.1006	0.1006	0.1006	0.0996	0.0998	0.1007	0.1000	0.1013	0.0999	0.100	0.0006	0.55
Zn	0.05	0.0315	0.0309	0.0322	0.0304	0.0329	0.0312	0.0313	0.0319	0.0308	0.0311	0.031	0.0007	2.35
	0.30	0.1705	0.1728	0.1688	0.1693	0.1711	0.1704	0.1704	0.1707	0.1708	0.1688	0.170	0.0012	0.70
	0.70	0.3559	0.3572	0.3548	0.3560	0.3559	0.3550	0.3579	0.3552	0.3574	0.3573	0.356	0.0011	0.31

Continue 3 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Tel. (66) 0 2577 9009  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtg@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2374 6292  
Fax. (66) 0 2374 6292  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม



Request No. 25-66 / 0323

3 / 5

MTC. ACL. No. 387 / 66

## 3. Trueness

## 3.1 Reading on wavelength- Cadmium(Cd) at 228.8 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cd	0.02002	0.021	0.001	4.90	± 0.005
	0.30030	0.298	-0.002	0.77	± 0.005
	0.70070	0.675	-0.026	3.67	± 0.008

## 3.2 Reading on wavelength- Chromium (Cr) at 357.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cr	0.1001	0.101	0.001	0.90	± 0.009
	0.3003	0.293	-0.007	2.43	± 0.012
	0.7007	0.648	-0.053	7.52	± 0.023

## 3.3 Reading on wavelength- Copper (Cu) at 324.7 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cu	0.050	0.046	-0.004	8.00	± 0.003
	0.300	0.289	-0.011	3.67	± 0.009
	0.700	0.674	-0.026	3.71	± 0.020

Continue 4 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Tel. (66) 0 2577 9009  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtg@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2374 6292  
Fax. (66) 0 2374 6292  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม



Request No. 25-66 / 0323

4 / 5

MTC. ACL. No. 387 / 66

## 3.4 Reading on wavelength- Iron (Fe) at 248.3 nm.

Element	Standard Value of RM (mg/L)	Reading (mg/L)	Error of Measurement (mg/L)	Error of Measurement (%)	Uncertainty (mg/L)
Fe	0.100	0.095	-0.005	5.00	± 0.014
	0.500	0.474	-0.026	5.20	± 0.016
	1.000	0.950	-0.050	5.00	± 0.029

## 3.5 Reading on wavelength- Lead (Pb) at 217.0 nm.

Element	Standard Value of RM (mg/L)	Reading (mg/L)	Error of Measurement (mg/L)	Error of Measurement (%)	Uncertainty (mg/L)
Pb	0.200	0.207	0.007	3.50	± 0.014
	0.700	0.673	-0.027	3.86	± 0.030
	1.500	1.417	-0.083	5.53	± 0.061

## 3.6 Reading on wavelength- Manganese (Mn) at 279.5 nm.

Element	Standard Value of RM (mg/L)	Reading (mg/L)	Error of Measurement (mg/L)	Error of Measurement (%)	Uncertainty (mg/L)
Mn	0.04995	0.046	-0.004	7.91	± 0.005
	0.29970	0.294	-0.0057	1.90	± 0.007
	0.69930	0.694	-0.0053	0.76	± 0.014

Continue 5 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website: www.tistr.or.th

Office/Laboratory  
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 23719 0392  
Fax. (66) 0 23719 0392  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม

Request No. 25-66 / 0323

5 / 5

MTC. ACL. No. 387 / 66

## 3.7 Reading on wavelength- Nickel (Ni) at 232.0 nm.

Element	Standard Value of RM (mg/L)	Reading (mg/L)	Error of Measurement (mg/L)	Error of Measurement (%)	Uncertainty (mg/L)
Ni	0.1001	0.103	0.003	2.90	± 0.013
	0.5005	0.501	0.001	0.10	± 0.018
	1.0010	0.987	-0.014	1.40	± 0.032

## 3.8 Reading on wavelength- Zinc (Zn) at 213.9 nm.

Element	Standard Value of RM (mg/L)	Reading (mg/L)	Error of Measurement (mg/L)	Error of Measurement (%)	Uncertainty (mg/L)
Zn	0.050	0.046	-0.004	8.00	± 0.013
	0.300	0.311	0.011	3.67	± 0.013
	0.700	0.665	-0.035	5.00	± 0.019

Remark : The reported uncertainty is an expanded uncertainty calculated using a coverage factor of 2 (k = 2)  
which gives a level of confidence of approximately 95%

Calibrated by 1. Dani Srithongkum

(Mr. Danai Srithongkum)

2. Atipat

(Mr. Atipat Ratana)

Approved by Saladee Deawong

(Miss Saladee Deawong)

Senior Technical Officer

Acting Director of

Analytical Chemistry Laboratory

Issued Date : 15 February 2023

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website: www.tistr.or.th

Office/Laboratory  
Sol 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 23719 0392  
Fax. (66) 0 23719 0392  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม

Agilent 5110 and 5100 ICP-OES  
Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results. Delivered by highly-trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak.

For more information about Agilent Technologies services please visit our web site using the following URL <http://www.agilent.com/en-us/services/analytical-instrument-services>

## Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of additional or special procedures and/or parts for the instrument service, then these must be ordered separately and charged as a repair, which may incur additional

## Service Engineer's Responsibilities

- Only complete/printout pages that relate to the system being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using a "X" or tick mark "✓" in the checkbox.
- Complete Not Applicable check boxes to indicate services not delivered, as needed.
- Complete the PM service in the order of the tasks listed.
- Complete the Service Review section together with the customer.

เอกสารไม่ควบคุม

Agilent 5110 and 5100 ICP-OES  
Preventive Maintenance Checklist

## System Information

Instrument system name and ID	ICP 5110 VDV
Instrument system site and location	UAE / 3rd Floor Laboratory
List system component product numbers	List the serial numbers of each component
1. G 8015 A	1. MY 18030001
2. G 8018 A	2. 1801-01988
3.	3.
4.	4.
5.	5.
6.	6.
7.	7.
8.	8.
9.	9.
10.	10.

ICP-OES Configuration table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray (OneNeb) other
Spray Chamber	Cyclonic Single Pass   Cyclonic Double Pass   other
Torch	Radial   Dual View   other
Injector Diameter	2.4mm   1.8mm   1.4mm   0.8mm   other
Injector Material	Quartz   Ceramic   other

เอกสารไม่ควบคุม



**Agilent 5110 and 5100 ICP-OES  
Preventive Maintenance Checklist**
**General Preparation**

- ☒ Discuss any specific questions or issues with the customer prior to starting.
- ☒ Review the instrument logbook.
- ☒ Perform general external inspection of system for cleanliness.
- ☒ Check for proper installation of safety-related parts, assemblies, sensors etc.
- ☒ Check for required firmware/software updates and verify with customers if they would like it installed.
- ☒ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. *N/A*
- ☒ Run Instrument Performance test and record results in Instrument Performance Test Results Table - Pre PM.

**Inspect and clean the system**

- ☒ Look for any obvious external damage or problems.
- ☒ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☒ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☒ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- ☒ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☒ Replace the polychromator purge filter.
- ☒ Replace the radial pre-optics window
- ☒ Replace the axial pre-optics window for SVDV and VDV instruments.
- ☒ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☒ Replace air inlet dust filter.
- ☒ Replace high capacity air inlet dust filter element if installed. *N/A*
- ☒ Remove and clean instrument water inlet filter.

**G8481A Cooling water system**

- ☐ **Section NOT Applicable**
- ☒ Drain cooling fluid and remove any particles from the chiller reservoir
- ☒ Remove, clean and reinstall water inlet metal mesh filter.
- ☒ Re fill with Polyclear cooling fluid.
- ☒ Clean the cooling system Air filter and the condenser by compressed air or vacuum cleaner.

Issued: 3 February 2017, Revision: 1.1

 Copyright © 2017  
Page 3 of 8

Agilent Technologies

เอกสารไม่ควบคุม

**Agilent 5110 and 5100 ICP-OES  
Preventive Maintenance Checklist**
**SPS 3 Auto Sampler**

- ☒ **Section NOT Applicable**
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

**SPS 4 Auto Sampler**

- ☒ **Section NOT Applicable**
- ☐ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☐ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner
- ☐ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☐ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles

**AVS 4, 6, 7**

- ☒ **Section NOT Applicable**
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks

**Instrument Adjustment**

- ☒ Check position of Zn peak, adjust if required.
- ☒ Check Argon Ratio, adjust to specified value if required.
- ☒ Perform Detector Calibration.
- ☒ Perform Instrument Calibration.
- ☒ Run Instrument Performance Test and record results in Instrument Performance Test Results Table - Post PM.
- ☒ For systems using ICP Expert version 7.3 and above run the following Instrument tests and record the result in the Instrument Test Results Table
  - ☒ Subsystem Communications Test
  - ☒ Air Flow

Issued: 3 February 2017, Revision: 1.1

 Copyright © 2017  
Page 4 of 8

Agilent Technologies

เอกสารไม่ควบคุม

**Agilent 5110 and 5100 ICP-OES  
Preventive Maintenance Checklist**

- ☒ Water Flow
- ☒ Gas Flows
- ☒ RF Generator
- ☒ Camera Test
- ☒ Optics Test
- ☒ Nebulizer Test

**Instrument Performance Test Results Table**

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	4100.6	8364.0	4375.0	8400.8
Mn 257.610 nm SRBR	11064.7	31842.1	12801.7	30846.2
Al 396.152 nm SBR	7.5	14.9	9.9	16.8
K 766.491 nm SBR	5.1	36.8	6.4	29.7

\* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

**Instrument Test Results Table**

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

Issued: 3 February 2017, Revision: 1.1

 Copyright © 2017  
Page 5 of 8

Agilent Technologies

เอกสารไม่ควบคุม

**Agilent 5110 and 5100 ICP-OES  
Preventive Maintenance Checklist**
**ICP-OES Status Results Table**

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	224.540	VAC	224.973	VAC
Mains Current	0.204	A	0.104	A
Instrument Temperature	22.8	°C	22.7	°C
RF Air Flow (sensor speed)	15.0	Hz	13.0	Hz
Plasma Exhaust Temperature	No measurement		26.7	°C
Water Flow Oscillator	No measurement		1.64	L/min
Water Flow Detector	1.06	L/min	1.06	L/min
Water Inlet Temperature	18.0	°C	18.0	°C
Polychromator Temperature	35.0	°C	35.0	°C
CCD Temperature	-39.8	°C	-39.8	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	671.94	kPa	627.33	kPa
Purge Gas Supply Pressure*1	674.90	kPa	643.40	kPa
Option Gas Supply Pressure*1	N/A	kPa	N/A	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		164.63	kPa
Plasma Gas Flow	No measurement		11.92	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1200	W
RF Supply Current	No measurement		8.663	A
RF Supply Voltage	No measurement		184.660	V

\*1 If option installed

Issued: 3 February 2017, Revision: 1.1

 Copyright © 2017  
Page 6 of 8

Agilent Technologies

เอกสารไม่ควบคุม

# Agilent 5110 and 5100 ICP-OES Preventive Maintenance Checklist

## ICP-OES Parts List Table

Part description	Part Number	Product / Model # where used	Quantity Consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Polyclear Cooling Fluid	G3292-80010	G8481A	
Purge Gas Filter	G8010-60136	All	1
Air inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	
PVC waste tubing, 8mm od x 5mm id, 2m	G8410-80122	SPS 4	
Additional Parts may be required from engineers stock:			
X axis drive belt	5410047500	SPS 3	
Z axis drive belt	5410047400	SPS 3	
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged,	3710049000	SPS 4	

## Restore system

For HF applications, ask the customer to reinstall their sample introduction system.

Leave system in an idle state: on and purging.

Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

## Service Review

- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section below if there are additional comments.

Issued: 3 February 2017, Revision: 1.1

Copyright © 2017  
Page 7 of 8

Agilent Technologies

เอกสารไม่ควบคุม

# Agilent 5110 and 5100 ICP-OES Preventive Maintenance Checklist

- ☒ Review the service and any test results with the customer.
- ☒ If the Instrument firmware was updated, record the details of the change in the Service Engineer's Comments box below or if necessary, in the customer's IQ records.

## Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

## Other Important Customer Web Links

How to get information on your product:

- ☒ Literature Library - <http://www.agilent.com/en-us/products/icp-oes/icp-oes-systems/5110-icp-oes#literature>
- ☒ Need to know more? - <http://www.agilent.com/crosslab/university/>
- ☒ Need technical support, FAQs? - <http://www.agilent.com/en-us/support/landing/icp-oes>
- ☒ Need supplies? - [www.agilent.com/chem/supplies](http://www.agilent.com/chem/supplies)

## Service Completion

Service request number 6005625287 Date service completed 30 Nov 2022

Agilent signature Woravit T. Customer signature Jim

Document part number: G8014-90075

Issued: 3 February 2017, Revision: 1.1

Copyright © 2017  
Page 8 of 8

Agilent Technologies

เอกสารไม่ควบคุม

## Report Summary

Instrument Model Agilent 5100/5110 VDV ICP-OES  
Instrument ID G8011A/G8015A  
Instrument Serial Number MY18030001  
Software Version 7.3.1.9507  
Firmware Version 3442  
Tested By Test Before PM  
Test Completed On 11/30/2022 9:35:32 AM

## Result Summary

Subsystem Communications Test Skipped  
Air Flow Test Skipped  
Water Flow Test Skipped  
Gas Flows Test Skipped  
RF Generator Test Skipped  
Camera Test Skipped  
Optics Test Skipped  
Advanced Valve System Test Skipped  
Resolution Test Pass  
Sensitivity Test Pass  
Precision Test Pass

เอกสารไม่ควบคุม

## Resolution Test

Pass

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.62
As (188.980 nm)	≤ 8.20	6.20
C (193.027 nm)	≤ 11.50	8.35
Mo (202.032 nm)	≤ 8.20	6.41
Cr (206.158 nm)	≤ 13.40	9.04
Zn (213.857 nm)	≤ 8.70	6.62
Pb (220.353 nm)	≤ 9.50	7.13
Co (228.615 nm)	≤ 17.20	11.71
Ba (230.424 nm)	≤ 9.40	7.21
Mn (257.610 nm)	≤ 13.30	9.50
Mn (260.568 nm)	≤ 20.30	14.33
Cr (267.716 nm)	≤ 11.00	8.14
Cu (324.754 nm)	≤ 25.00	18.98
Cu (327.395 nm)	≤ 14.20	11.24
Sr (338.071 nm)	≤ 33.50	24.47
Ba (455.403 nm)	≤ 44.00	33.88
Sr (460.733 nm)	≤ 36.00	17.22
Ba (493.408 nm)	≤ 36.00	25.48
Ba (614.171 nm)	≤ 42.00	25.47
Ar (675.283 nm)	≤ 74.00	59.82
K (766.491 nm)	≤ 80.00	64.94

เอกสารไม่ควบคุม



Sensitivity Test				Pass		
Radial						
Element	Wavelength	Specification	Method	Ratio	Standard	Blank
As	(188.980 nm)	≥ 46.0	SRBR	147.7	1156.5	55.5
Se	(196.026 nm)	≥ 41.0	SRBR	111.1	1195.3	97.7
Zn	(213.857 nm)	≥ 1421.0	SRBR	4100.6	51959.5	159.6
Pb	(220.353 nm)	≥ 46.0	SRBR	192.5	2808.6	185.7
Mn	(257.610 nm)	≥ 3518.0	SRBR	11064.7	264165.0	567.6
Al	(396.152 nm)	≥ 3.4	SBR	7.5	49047.9	5770.5
Ba	(493.408 nm)	≥ 34.0	SBR	107.4	1887710.3	17407.5
K	(766.491 nm)	≥ 1.8	SBR	5.1	100805.9	16626.4
Axial						
Element	Wavelength	Specification	Method	Ratio	Standard	Blank
As	(188.980 nm)	≥ 208.0	SRBR	234.9	3056.4	152.9
Se	(196.026 nm)	≥ 159.0	SRBR	218.1	3865.1	271.6
Zn	(206.200 nm)	≥ 234.0	SRBR	1306.5	15850.4	144.5
Zn	(213.857 nm)	≥ 1743.0	SRBR	8364.0	183037.8	476.4
Cd	(214.439 nm)	≥ 4227.0	SRBR	7718.5	143240.2	342.8
Pb	(220.353 nm)	≥ 320.0	SRBR	576.3	14465.2	580.4
Mn	(257.610 nm)	≥ 10625.0	SRBR	31842.1	1411257.3	1958.9
Cr	(267.716 nm)	≥ 1048.0	SRBR	4492.1	183110.6	1632.2
Cu	(324.754 nm)	≥ 19.0	SBR	46.2	371487.5	7862.9
Al	(396.152 nm)	≥ 6.0	SBR	14.9	278447.4	17552.6
Ba	(493.408 nm)	≥ 60.0	SBR	190.6	10061527.3	52519.8
K	(766.491 nm)	≥ 24.0	SBR	38.8	1922163.4	50858.1

Page 3 of 4

เอกสารไม่ควบคุม

Precision Test			Pass
Radial			
Element	Wavelength	Specification	Measured Value % RSD
As	(188.980 nm)	≤ 2.60	0.82
Se	(196.026 nm)	≤ 2.60	0.71
Zn	(213.857 nm)	≤ 1.50	0.43
Pb	(220.353 nm)	≤ 2.60	0.76
Mn	(257.610 nm)	≤ 1.50	0.60
Al	(396.152 nm)	≤ 1.50	0.48
Ba	(493.408 nm)	≤ 1.50	0.89
K	(766.491 nm)	≤ 1.50	0.42
Axial			
Element	Wavelength	Specification	Measured Value % RSD
As	(188.980 nm)	≤ 1.50	0.57
Se	(196.026 nm)	≤ 1.50	0.76
Zn	(206.200 nm)	≤ 1.50	0.61
Zn	(213.857 nm)	≤ 1.50	0.51
Cd	(214.439 nm)	≤ 1.50	0.55
Pb	(220.353 nm)	≤ 1.50	0.52
Mn	(257.610 nm)	≤ 1.50	0.54
Cr	(267.716 nm)	≤ 1.50	0.54
Cu	(324.754 nm)	≤ 1.50	0.69
Al	(396.152 nm)	≤ 1.50	0.91
Ba	(493.408 nm)	≤ 1.50	0.85
K	(766.491 nm)	≤ 1.50	1.22

Page 4 of 4

เอกสารไม่ควบคุม

Report Summary		
Instrument Model	Agilent 5100/5110 VDV ICP-OES	
Instrument ID	G8011A/G8015A	
Instrument Serial Number	MY18030001	
Software Version	7.3.1.9507	
Firmware Version	3442	
Tested By	PM Functional test	
Test Completed On	11/30/2022 11:43:36 AM	
Result Summary		
Subsystem Communications Test	Pass	
Air Flow Test	Pass	
Water Flow Test	Pass	
Gas Flows Test	Pass	
RF Generator Test	Pass	
Camera Test	Pass	
Optics Test	Skipped	
Advanced Valve System Test	Skipped	
Resolution Test	Skipped	
Sensitivity Test	Skipped	
Precision Test	Skipped	
Subsystem Communications Test		
Pass		
Air Flow Test		
Pass		
30% Air Flow (relative speed)	75% Air Flow (relative speed)	
14.00	19.00	
Water Flow Test		
Pass		
RF Water Flow(L/min)	Camera Water Flow (L/min)	Water Inlet Temperature (°C)
1.44	1.05	18.51

Page 1 of 2

เอกสารไม่ควบคุม

Gas Flows Test			Pass		
Nebulizer Target Flow	Actual Flow	Back Pressure	Auxiliary Target Flow	Actual Flow	Back Pressure
0.70	0.70	163.37	2.00	1.99	108.49
Makeup Target Flow	Actual Flow	Back Pressure	Plasma Target Flow	Actual Flow	Back Pressure
2.00	2.00	112.85	18.00	17.91	23.46
RF Generator Test			Pass		
RF Power Supply Test		Passed			
RF Power Supply (V)		147.437			
RF Oscillator Test		Passed			
RF Oscillator Frequency (MHz)		0.000			
Work Coil Current (A)		45.069			
RF Power Supply Current (A)		1.997			
Camera Test			Pass		
	Integration Time (ms)	Standard Deviation	Status		
Electronic Offset Test	1000	5.305	Passed		
Dark Current Test	6000	0.578	Passed		
Array Test	5	0.024	Passed		
Linearity Test		0.118	Passed		

Page 2 of 2

เอกสารไม่ควบคุม

Report Summary		
Instrument Model	Agilent 5100/5110 VDV ICP-OES	
Instrument ID	G8011A/G8015A	
Instrument Serial Number	MY18030001	
Software Version	7.3.1.9507	
Firmware Version	3442	
Tested By	PM Performance test	
Test Completed On	11/30/2022 12:10:42 PM	
Result Summary		
Subsystem Communications Test	Skipped	
Air Flow Test	Skipped	
Water Flow Test	Skipped	
Gas Flows Test	Skipped	
RF Generator Test	Skipped	
Camera Test	Skipped	
Optics Test	Pass	
Advanced Valve System Test	Skipped	
Resolution Test	Pass	
Sensitivity Test	Pass	
Precision Test	Pass	
Optics Test	Pass	
	Radial	Axial
Intensity	5674608	5823476
Wavelength	737.212	737.212

Page 1 of 4

เอกสารไม่ควบคุม

Resolution Test			Pass
Element	Wavelength	Specification	Width
N	(174.213 nm)	≤ 9.40	6.79
As	(188.980 nm)	≤ 8.20	6.09
C	(193.027 nm)	≤ 11.50	8.29
Mo	(202.032 nm)	≤ 8.20	6.30
Cr	(206.158 nm)	≤ 13.40	9.05
Zn	(213.857 nm)	≤ 8.70	6.77
Pb	(220.353 nm)	≤ 9.50	7.02
Co	(228.615 nm)	≤ 17.20	11.67
Ba	(230.424 nm)	≤ 9.40	7.39
Mn	(257.610 nm)	≤ 13.30	9.48
Mn	(260.568 nm)	≤ 20.30	14.25
Cr	(267.716 nm)	≤ 11.00	7.94
Cu	(324.754 nm)	≤ 25.00	18.99
Cu	(327.395 nm)	≤ 14.20	11.33
Sr	(338.071 nm)	≤ 33.50	24.44
Ba	(455.403 nm)	≤ 44.00	33.86
Sr	(460.733 nm)	≤ 36.00	17.51
Ba	(493.408 nm)	≤ 36.00	25.56
Ba	(614.171 nm)	≤ 42.00	24.96
Ar	(675.283 nm)	≤ 74.00	59.38
K	(766.491 nm)	≤ 80.00	65.63

Page 2 of 4

เอกสารไม่ควบคุม

Sensitivity Test						Pass
Radial						
Element	Wavelength	Specification	Method	Ratio	Standard	Blank
As	(188.980 nm)	≥ 46.0	SRBR	147.8	1149.3	54.8
Se	(196.026 nm)	≥ 41.0	SRBR	111.6	1222.8	101.0
Zn	(213.857 nm)	≥ 1421.0	SRBR	4375.0	52592.3	143.7
Pb	(220.353 nm)	≥ 46.0	SRBR	199.8	2744.4	166.5
Mn	(257.610 nm)	≥ 3518.0	SRBR	12801.7	285591.3	496.0
Al	(396.152 nm)	≥ 3.4	SBR	9.9	52888.6	4873.6
Ba	(493.408 nm)	≥ 34.0	SBR	154.6	2287291.6	14698.1
K	(766.491 nm)	≥ 1.8	SBR	6.4	106701.6	14350.9
Axial						
Element	Wavelength	Specification	Method	Ratio	Standard	Blank
As	(188.980 nm)	≥ 208.0	SRBR	242.4	3170.1	154.8
Se	(196.026 nm)	≥ 159.0	SRBR	226.1	4134.5	289.3
Zn	(206.200 nm)	≥ 234.0	SRBR	1128.6	13782.0	146.5
Zn	(213.857 nm)	≥ 1743.0	SRBR	8400.8	177166.3	442.5
Cd	(214.439 nm)	≥ 4227.0	SRBR	7001.9	125884.2	321.6
Pb	(220.353 nm)	≥ 320.0	SRBR	536.3	12909.3	532.6
Mn	(257.610 nm)	≥ 10625.0	SRBR	30846.2	1287989.0	1738.8
Cr	(267.716 nm)	≥ 1048.0	SRBR	4396.0	167335.6	1424.4
Cu	(324.754 nm)	≥ 19.0	SBR	52.1	373690.7	7033.1
Al	(396.152 nm)	≥ 6.0	SBR	16.8	268357.7	15112.4
Ba	(493.408 nm)	≥ 60.0	SBR	225.2	10173441.5	44971.7
K	(766.491 nm)	≥ 24.0	SBR	39.7	1874136.2	46055.7

Page 3 of 4

เอกสารไม่ควบคุม

Precision Test			Pass
Radial			
Element	Wavelength	Specification	Measured Value % RSD
As	(188.980 nm)	≤ 2.60	0.60
Se	(196.026 nm)	≤ 2.60	0.84
Zn	(213.857 nm)	≤ 1.50	0.29
Pb	(220.353 nm)	≤ 2.60	0.59
Mn	(257.610 nm)	≤ 1.50	0.28
Al	(396.152 nm)	≤ 1.50	0.28
Ba	(493.408 nm)	≤ 1.50	0.59
K	(766.491 nm)	≤ 1.50	0.23
Axial			
Element	Wavelength	Specification	Measured Value % RSD
As	(188.980 nm)	≤ 1.50	0.71
Se	(196.026 nm)	≤ 1.50	0.43
Zn	(206.200 nm)	≤ 1.50	0.46
Zn	(213.857 nm)	≤ 1.50	0.37
Cd	(214.439 nm)	≤ 1.50	0.48
Pb	(220.353 nm)	≤ 1.50	0.48
Mn	(257.610 nm)	≤ 1.50	0.74
Cr	(267.716 nm)	≤ 1.50	0.26
Cu	(324.754 nm)	≤ 1.50	0.51
Al	(396.152 nm)	≤ 1.50	0.45
Ba	(493.408 nm)	≤ 1.50	0.81
K	(766.491 nm)	≤ 1.50	0.84

Page 4 of 4

เอกสารไม่ควบคุม



## Automatic Mercury Analyzer

Model RA-4500

## Preventive Maintenance Report

Serial No. : 17780278

Soft version : Ver 2.0.7

ROM version : Ver 2.0.1

Date : 11 July 2023

PM by : Pradit Mayong  
( Pradit M. )Approved by : Pathom S.  
( Pathom S. )

Coax Group Corporation Ltd.

1131/62,64,325-331 Nakornchaisri road,

Kwang ThanonNakornchaisri, Dusit, Bangkok 10300 Thailand

Tel. 02-2435263, 02-6682436 Fax. 02-2437386

เอกสารไม่ควบคุม

## Inspection result

ITEM	STANDARD	RESULT	JUDGE
1. Self Check	1.1 Heating	PASS	OK
	1.2 Cooling	PASS	OK
	1.3 Leak	PASS	OK
	1.4 Optical system	PASS	OK
	1.5 Drift	PASS	OK

## 2. Analytical curve inspection(AREA)

2.1 No Pretreatment (Low Conc.)	Correlation coefficient	1.0000	OK
	( r ) ≥ 0.9990		

## 3. Repeatability(AREA)


3.1 No Pretreatment 100ppb, n=5	1.	99.12	ppb
	2.	101.48	ppb
	3.	101.24	ppb
	4.	102.34	ppb
	5.	101.92	ppb
	C.V. ≤ 5%	1.23%	OK

4. Blank	Below 1.0 (AREA)	0.2062	OK
----------	------------------	--------	----

เอกสารไม่ควบคุม


Title : Preventive Maintenance RA-4500 sn:17780278  
 Date : 7/11/2023  
 Name : Coax Group  
 Memo : Calibration Curve 0-10ng

## Calib



## STD

No.	STD [ppb]	SVOL [mL]	CVOL [mL]	DVOL [mL]	STD [ng]	AREA [ON]	MEAS [ng]	Dev [%]	Note
1	100.000	0.000	5.000	0.000	0.0859	-0.0353	-		
2	100.000	0.025	5.000	5.000	2.500	3.7687	2.5845	3.4	
3	100.000	0.050	5.000	5.000	5.000	7.1028	4.9562	0.9	
4	100.000	0.075	5.000	5.000	7.500	10.6441	7.4753	0.3	
5	100.000	0.100	5.000	5.000	10.000	14.2203	10.0193	0.2	

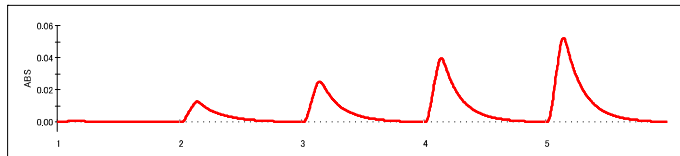

## SMP

No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	hg 100 ppb	0.050	5.000	5.000	7.1027	4.9561	99.122	
2	hg 100 ppb	0.050	5.000	5.000	7.2687	5.0742	101.484	
3	hg 100 ppb	0.050	5.000	5.000	7.2514	5.0619	101.238	
4	hg 100 ppb	0.050	5.000	5.000	7.3285	5.1168	102.336	
5	hg 100 ppb	0.050	5.000	5.000	7.2996	5.0962	101.924	

## Statistics

No.	NAME	TRY	AV [ug/L]	SD [ug/L]	Cv [%]
1	hg 100 ppb	5	101.2208	1.246264	1.23

เอกสารไม่ควบคุม

NIPON INSTRUMENTS CORPORATION


เอกสารไม่ควบคุม

NIPON INSTRUMENTS CORPORATION

Title : Preventive Maintenance RA-4500 sn:17780278  
Date : 7/11/2023  
Name : Coax Group  
Memo : Blank

SMP

No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	Blank				0.2062	0.0503		

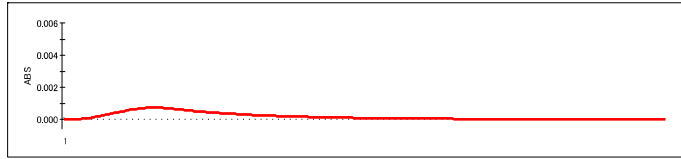

## Agilent CrossLab Start Up Services

### Agilent 8890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure consistent performance and long life expectancy of your investment.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

เอกสารไม่ควบคุม

NIC NIPPON INSTRUMENTS CORPORATION

เอกสารไม่ควบคุม

#### Agilent 8890 GC Preventive Maintenance Checklist

### Introduction

#### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

#### Important Customer Web Links

- For more information about **Agilent Technologies** services, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our **Support Home page** <http://www.agilent.com/search/support>.
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube channel** at <https://www.youtube.com/user/agilent>.

เอกสารไม่ควบคุม

#### Agilent 8890 GC Preventive Maintenance Checklist

### Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.  
*Only select those items that relate to the system or module being serviced.*
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "Section not applicable" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.  
*Complete the service tasks in the order of the tasks listed.*
- Complete the fields for page numbers at the foot of each selected page.
- Complete the total number of pages field in the Service Completion section.
- Ask the customer to sign the Service Completion section including the customer's and your signature.

### Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any modification notes.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

เอกสารไม่ควบคุม



## System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	CN1945A066
Instrument System Site and Location	VAE GCMS (405)

List System Component Product Numbers	List the Serial Numbers of each Component
1. 87922A	CN1945A066
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	
10.	

## Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 4 of 9 

เอกสารไม่ควบคุม

## Preventive Maintenance Procedure

## Clean and inspect GC

- ☒ Unplug power cord from the power source.
- ☒ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☒ Inspect internal connectors for proper contact and placement.
- ☒ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☒ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☒ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☒ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

## Inlet and detector consumable replacement

- ☒ Replace the split vent trap cartridge filter using the Maintenance procedure from either the Browser User interfaces on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☒ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☒ For the inlets installed, perform inlet maintenance using the Maintenance procedure from the Browser User interfaces. Record the results. (Leak and Restriction Test)
- ☐ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination - clean as necessary.

## Zero Sensors and Leak test

- ☒ Zero all pressure sensors using the Browser interface.
- ☒ Perform inlet pressure decay test(s) from the diagnostics screen on the Browser User interface. Record if test passed or failed in the results table.

Note: If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 5 of 9 

เอกสารไม่ควบคุม

## ALS Maintenance

- ☒ Section NOT applicable
- ☐ Check all cabling and configuration settings between GC, tray, and injectors.
- ☐ Vacuum or remove any dust, especially around fans.
- ☐ Check operation of all fans.
- ☐ Check syringe for smooth plunger operation.
- ☐ Check for smooth operation of the needle support - clean if necessary

## Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions
- ☒ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☐ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

## Signature Page


## Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review with the customer this service, parts replaced, and test results obtained.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

## PM Test Results Table

Test description	Before PM Service	After PM Service
Front detector output	N/A	N/A
Back detector output	N/A	N/A
AUX 1 detector output	N/A	N/A
AUX 2 detector output	N/A	N/A
Test description	Expected test result	Actual test result
Leak and Restriction Test after front inlet maintenance	Pass	Pass
Leak and Restriction Test after back inlet maintenance	Pass	N/A
Leak and Restriction Test after front inlet Split Vent Trap replacement	Pass	Pass
Leak and Restriction Test after back inlet Split Vent Trap replacement	Pass	N/A
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	N/A

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 6 of 9 

เอกสารไม่ควบคุม

Revision: 2.01, Issued: September 14, 2021  
 Agile Document Number: D0013610  
 DE number: 44166.759722222  
 © Agilent Technologies, Inc. 2021

Page 7 of 9 

เอกสารไม่ควบคุม

**PM Parts List Table**

Note: The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Gold Seal	5188-6497	8890 GC	1
SSL Capillary Inlet PM kit, Split	5188-6496	8890 GC	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2295	8890 GC	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	8890 GC	N/A
PP Inlet PM kit	5188-6498	8890 GC	N/A
Splitless Inlet PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	8890 GC	N/A
MMI Cleaning Kit	G3510-60820	8890 GC	N/A
PTV Septumless Head Rebuild Kit	5182-9747	8890 GC	N/A
PTV Septumless Head Rebuild Kit	5182-9747	8890 GC	N/A
Ignitor (glow plug) assembly with O-ring	19231-60680	8890 GC	N/A
FID Collector Rebuild/Cleaning Kit	G1531-67000	8890 GC	N/A
FID Collector Replacement Kit	G1531-67001	8890 GC	N/A
Standard .011-inch FID Jet	5200-0176	8890 GC	N/A
Universal .018-inch FID Jet	5200-0177	8890 GC	N/A

**Service Engineer Comments**

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

**Service Completion**

Service request number 600 5953599 Date service completed 14 June 2023  
 Agilent signature SMT Customer signature \_\_\_\_\_  
 Total number of pages in this document 9 pages

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม