

ภาคผนวก ฎ
เอกสารสอบเทียบเครื่องมือ



List of Instruments Certification for Air & Noise Quality Analysis

รหัส : 2022-006174

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Thermo Scientific	G25A 158M	Tisch Environmental, Inc.	05072022	5 Jul 22	4 Jul 24	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	22P803	12 Mar 22	11 Mar 23	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	22P2728	22 Jul 22	21 Jul 23	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	22H1587	27 Jul 22	26 Jul 23	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Fisher Scientific	42C 0517512000	UAE Consultant Co., Ltd.	07042022	7 Apr 22	6 Apr 23	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Electron	42C 0517512001	UAE Consultant Co., Ltd.	07042022	7 Apr 22	6 Apr 23	-
7	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
8	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i JC1606001757	UAE Consultant Co., Ltd.	22042022	22 Apr 22	21 Apr 23	-
9	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i JC1606001758	UAE Consultant Co., Ltd.	22042022	22 Apr 22	21 Apr 23	-
10	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
11	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV35A 73246	Innovative Instrument Co., Ltd.	22-ACT-405	1 Jul 22	30 Jun 23	-
12	Sound Level Meter	L _{Aeq} 24 hours, L _{Aeq} 5 minutes, L _{Adn} , L _{A90} L _{Amax} , Annoyance Noise	Larson Davis	LxT2 0005400	Innovative Instrument Co., Ltd.	22-ACT-036	21 Jan 22	20 Jan 23	-
13	Sound Level Meter	L _{Aeq} 24 hours, L _{Aeq} 5 minutes, L _{Adn} , L _{A90} L _{Amax} , Annoyance Noise	Larson Davis	LxT2 0005402	Innovative Instrument Co., Ltd.	22-ACT-103	11 Feb 22	10 Feb 23	-

Certificate of Calibration

Calibration Certification Information				
Cal. Date:	July 5, 2022	Rootsmeter S/N:	438320	Ta: 297 °K
Operator:	Jim Tisch	Pa:	750.1	mm Hg
Calibration Model #:	G25A	Calibrator S/N:	158M	

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3240	3.2	2.00
2	3	4	1	0.9480	6.4	4.00
3	5	6	1	0.8480	7.9	5.00
4	7	8	1	0.8060	8.7	5.50
5	9	10	1	0.6670	12.7	8.00

Data Tabulation				
Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9860	0.7447	1.4073	0.9957	0.7521
0.9818	1.0357	1.9902	0.9915	1.0459
0.9798	1.1554	2.2251	0.9895	1.1668
0.9788	1.2143	2.3337	0.9884	1.2263
0.9735	1.4395	2.8146	0.9831	1.4739
m=		1.96745	m=	
b=		-0.05315	b=	
r=		0.99995	r=	
QSTD			QA	

Calculations				
Vstd=	ΔVol((Pa-ΔP)/Pstd)(Tstd/Ta)	Va=	ΔVol((Pa-ΔP)/Pa)	
Qstd=	Vstd/ΔTime	Qa=	Va/ΔTime	
For subsequent flow rate calculations:				
Qstd=	1/m $\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b$	Qa=	1/m $\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b$	

Standard Conditions	
Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH:	calibrator manometer reading (in H2O)
ΔP:	rootsmeter manometer reading (mm Hg)
Ta:	actual absolute temperature (°K)
Pa:	actual barometric pressure (mm Hg)
b:	intercept
m:	slope

RECALIBRATION	
US EPA recommends annual recalibration per 1998	
40 Code of Federal Regulations Part 50 to 51,	
Appendix B to Part 50, Reference Method for the	
Determination of Suspended Particulate Matter in	
the Atmosphere, 9.2.17, page 30	



Certificate of Calibration

Certificate No.: 22P803
Page: 1 of 2

Equipment:	U Tube Manometer	This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.
Manufacturer:	Dwyer	
Model:	1221-36-W/M	
Serial No.:	-	
ID No.:	UAE.EFM.179/2561	
Condition As-Received:	Used Item	
Received Date:	03 March 2022	
Calibration Date:	12 March 2022	
Reference:	2203-0131WSC	Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
Ambient Temperature:	(23 ± 2) °C	
Relative Humidity:	(50 ± 15) %	81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Atmospheric Pressure:	1010 mbar	

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using * DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 * as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0110-21	09 Aug 2022
2.This result of calibration was made on requested at the point specified by customer.				
3.Scale and conversion factor is 1 kPa = 4.0146293 inH2O				
4.This instrument was used clean air as pressure media.				
5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.				
6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.				
7.The certificate is valid only to the item calibrated on date and place of calibration.				
8.This Certification is traceable to the International System of Unit maintained at:-				
-National Institute of Metrology Thailand (NIMT)				

Calibrated by : Suwit Aussarree
Issue Date : 14 March 2022

Approved Signatory : Attapol P.
[] Phalinee Prabpaipal
[] Sura Suwannasri
✓ Attapol Panurach



Cert.No.: 22P803
Page: 2 of 2

Result of calibration:- Without adjustment
Function:- Pressure Measurement
Increasing Pressure

Range: 0 inH2O to 36 inH2O
Scale Interval: 0.1 inH2O(The Fifth Estimate)

UUC Indication				
Applied Pressure (inH2O)	High-port side (inH2O)	Low-port side (inH2O)	ΔP (inH2O)	Error (inH2O)
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-0.96	1.96	-0.04
4.00	2.00	-1.96	3.96	-0.04
6.00	3.00	-2.96	5.96	-0.04
8.00	4.00	-3.94	7.94	-0.06
10.00	5.00	-4.94	9.94	-0.06
12.00	6.00	-5.94	11.94	-0.06
14.00	7.02	-6.94	13.96	-0.04
16.00	8.02	-7.94	15.96	-0.04
18.00	9.04	-8.96	18.00	0.00
20.00	10.04	-9.96	20.00	0.00
22.00	11.06	-10.96	22.02	0.02
24.00	12.06	-11.96	24.02	0.02
26.00	13.08	-12.98	26.06	0.06
28.00	14.08	-13.98	28.06	0.06
30.00	15.10	-14.98	30.08	0.08
32.00	16.10	-15.98	32.08	0.08
34.00	17.08	-16.98	34.06	0.06
35.50	17.86	-18.00	35.86	0.36

The uncertainty of measurement was ± 0.11 inH2O

* UUC = Unit Under Calibration

* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-00o-



Certificate of Calibration

Certificate No.: 22P2728
Page: 1 of 2

Equipment:	Aneroid Barometer	This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.
Manufacturer:	Barigo	
Model:	-	
Serial No.:	-	
ID No.:	UAE.ANV.152/2550	
Condition As-Received:	Used Item	
Received Date:	20 July 2022	
Calibration Date:	22 July 2022	
Reference:	2207-0584WSC	Submitted by: United Analyst and Engineering Consultant Co.,Ltd.
Ambient Temperature:	(23 ± 2) °C	
Relative Humidity:	(50 ± 15) %	81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Atmospheric Pressure:	1010 mbar	

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using * DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 * as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DP1142	1422505046	MP-0076-22	02 May 2023
2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.				
3.This result of calibration was made on requested at the point specified by customer.				
4.This result of calibration instrument was in absolute pressure.				
5.This instrument was used clean air as pressure media.				
6.The certificate is valid only to the item calibrated on date and place of calibration.				
7.This Certification is traceable to the International System of Unit maintained at:-				
-National Institute of Metrology Thailand (NIMT)				

Calibrated by : Suwit Aussarree
Issue Date : 25 July 2022

Approved Signatory : Attapol P.
[] Phalinee Prabpaipal
[] Sura Suwannasri
✓ Attapol Panurach



Cert.No.: 22P2728
Page: 2 of 2

Result of calibration:- Without adjustment
Function:- Absolute Pressure Measurement

Range: 960 hPa to 1030 hPa
Scale Interval: 1 hPa (The Fifth Estimate)

Increasing Pressure

Applied Pressure (hPa)	956.27	967.46	978.89	989.56	999.85	1009.89	1020.55	1031.06
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	3.73	2.54	1.11	0.44	0.15	0.11	-0.55	-1.06

Decreasing Pressure

Applied Pressure (hPa)	1031.19	1020.73	1009.91	999.92	989.72	979.13	967.71	956.64
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-1.19	-0.73	0.09	0.08	0.28	0.87	2.29	3.36

The uncertainty of measurement was ± 0.30 hPa

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-000-

เอกสารไมควบคุม
a 1118529



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 22H1587
Page: 1 of 2

Equipment: Dial Thermo-Hygrometer

Manufacturer: Barigo

Model: -

Serial No.: -

ID No.: UAE.ANV.127/2550

Condition As-Received: Used Item

Received Date: 20 July 2022

Calibration Date: 22 July 2022

Reference: 2207-0586W5C

Ambient Temperature: $(25 \pm 3) ^\circ\text{C}$

Relative Humidity: $(50 \pm 20) \%$

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udumuk 41, Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Chilled Mirror Hygrometer Sensor	Dew Prime II	31863	19714	17 Sep 2022
2) Standard Humidity/Temperature Meter	400	10240757	TH-0125-21	13 Dec 2022

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Standards and Technology (NIST), The United States of America

-National Institute of Metrology Thailand (NIMT)

Calibrated by: Somchai Durmwor
Issue Date: 03 August 2022

Approved Signatory: [] Chakrit Waewanjua
[] Pornthippa Tameyakul
[] Viporn Tantiyawutti

เอกสารไมควบคุม
B 0293723



Cert. No.: 22H1587
Page: 2 of 2

Result of Calibration:-

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
($^\circ\text{C}$)	(%R.H.)	(%R.H.)	(%R.H.)	(\pm %R.H.)
25.0	40.1	38	-2.1	1.6
25.0	60.0	57	-3.0	1.8
25.0	80.0	74	-6.0	2.0

Result of Calibration:-

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
($^\circ\text{C}$)	(%R.H.)	(%R.H.)	(%R.H.)	(\pm %R.H.)
25.0	40.1	40	-0.1	1.6
25.0	60.0	60	0.0	1.8
25.0	80.0	77	-3.0	2.0

Result of Calibration:-

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
($^\circ\text{C}$)	(%R.H.)	(%R.H.)	(%R.H.)	(\pm %R.H.)
20.00	20.0	20.0	0.00	0.72
25.04	25.0	25.0	-0.04	0.72
30.01	30.0	30.0	-0.01	0.72
35.04	35.0	35.0	-0.04	0.72
39.98	40.0	40.0	0.02	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-000-

เอกสารไมควบคุม
a 1119773



United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udumuk 41, Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Tel. 0 2763 2828 Fax 0 2763 2800 www.uaeconsultant.com E-mail: uae@uaeconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date: Apr 7, 2022


Equipment: Gas Analyzer (NO₂) Model: 42C
Manufacturer: Thermo Electron Corporation Serial Number: 0517512000

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	44.75	PPM	Manufacturer:	Thermo Scientific
Nitric Oxide (NO)	45.35	PPM	Model:	146i
Methane (CH ₄)	-	PPM	Serial Number:	1180540071
Carbon Monoxide (CO)	1007			
Cylinder No.:	CC159599			
Expiration Date:	Jul 30, 2022			

Multi-point gas test data

Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.50	0.50	0.50
Level 2	20.00%	100.0	100.5	0.50	0.50
Level 3	40.00%	200.0	200.4	0.40	0.20
Level 4	60.00%	300.0	300.5	0.50	0.17
Level 5	80.00%	400.0	400.6	0.60	0.15
Remark: Measuring Range 500.0 ppb			Average Difference (%)		
Acceptable Limit $\pm 5\%$			0.30		

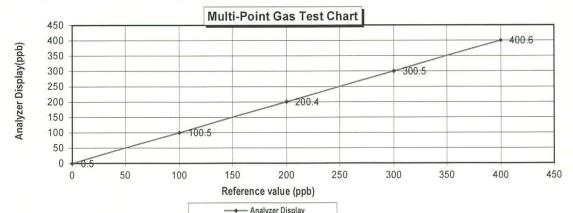

Calculate by

Signature: [Signature]
Date: 21/4/22

Approve by

Signature: [Signature]
Date: 21/4/22

เอกสารไมควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Apr 7, 2022

Equipment : Gas Analyzer (NO₂) Model : 42C
Manufacturer : Thermo Electron Corporation Serial Number : 0517512001

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.75 PPM
Nitric Oxide (NO) 45.35 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 1007 PPM
Cylinder No. : CCI59599
Expiration Date : Jul 30, 2022

Dilutor Detail


Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.9	0.90	0.90
Level 2	20.00%	100.0	100.5	0.50	0.50
Level 3	40.00%	200.0	200.3	0.30	0.15
Level 4	60.00%	300.0	300.7	0.70	0.23
Level 5	80.00%	400.0	400.8	0.80	0.20

Remark : Measuring Range 500.0 ppb
:Acceptable Limit $\pm 5\%$

Multi-Point Gas Test Chart

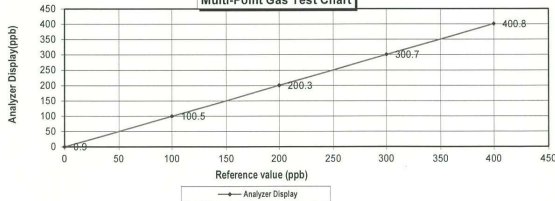

Calculate by

Signature
22/4/22

Approve by

Signature
5/1 Apr 2022

เอกสารไม่ควบคุม

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04NI99E15A01D3 Reference Number: 122-402135167-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO₂,BALN Certification Date: Jun 21, 2021
Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Array and Certification of Ozone Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.
Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.58 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20061120	C0708068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D685025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMS	401423838102	C050581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	C0473277	48.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14080119	C0434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.8%	Nov 15, 2025

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO ₂	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO ₂	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807
GROSS WT: 28.40kg
NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



CERT 3082.01

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Apr 22, 2022

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : JC1606001757

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.75 PPM
Nitric Oxide (NO) 45.35 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 1007 PPM
Cylinder No. : CCI59599
Expiration Date : Jul 30, 2022

Dilutor Detail


Manufacturer : Thermo SCIENTIFIC
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.70	0.70
Level 2	20.00%	100.0	100.5	0.50	0.50
Level 3	40.00%	200.0	200.4	0.40	0.20
Level 4	60.00%	300.0	300.7	0.70	0.23
Level 5	80.00%	400.0	400.5	0.50	0.12

Remark : Measuring Range 500.0 ppb
:Acceptable Limit $\pm 5\%$

Multi-Point Gas Test Chart

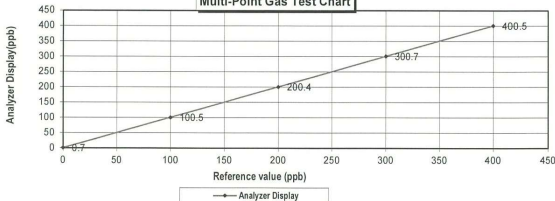

Calculate by

Signature
22/4/22

Approve by

Signature
22/4/22

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Apr 22, 2022

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo Scientific Serial Number : JC1606001758

Standard Gas Concentration

Sulphur Dioxide (SO₂) 44.75 PPM
Nitric Oxide (NO) 45.35 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 1007 PPM
Cylinder No. : CCI59599
Expiration Date : Jul 30, 2022

Dilutor Detail


Manufacturer : Thermo SCIENTIFIC
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Level	Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.6	0.60	0.60
Level 2	20.00%	100.0	100.7	0.70	0.70
Level 3	40.00%	200.0	200.5	0.50	0.25
Level 4	60.00%	300.0	300.7	0.70	0.23
Level 5	80.00%	400.0	400.5	0.50	0.12

Remark : Measuring Range 500.0 ppb
:Acceptable Limit $\pm 5\%$

Multi-Point Gas Test Chart

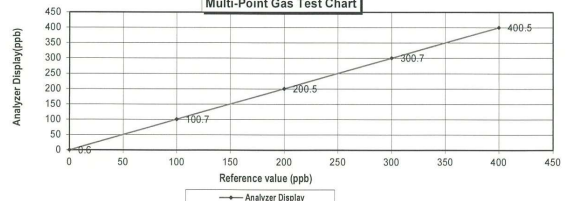

Calculate by

Signature
22/4/22

Approve by

Signature
22/4/22

เอกสารไม่ควบคุม

CERTIFICATE OF ANALYSIS
Grade of Product: EPA Protocol

Part Number: E04N199E15A01D3
Cylinder Number: EB0143262
Laboratory: 124 - Durham (SAP) - NC
PGVP Number: B22021
Gas Code: CO,NO,NOX,SO2,BALN
Expiration Date: Jun 21, 2024
Reference Number: 122-402135167-1
Cylinder Volume: 144.4 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 660
Certification Date: Jun 21, 2021

Certification performed in accordance with "EPA Traceability Protocol for Array and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/931, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.58 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				06/14/2021

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20061120	C0708068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D885025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMS	401423838102	C0505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	C0473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14080119	C0434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.8%	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO2	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807
GROSS WT: 28.40kg
NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



เอกสารไม่ควบคุม

Certificate of Calibration

Customer Name : UNITED ANALYST AND ENGINEERING CONSULTANT
CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260
Certificate No : 22-ACT-405
Request No : Req-2022-1080

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : SVANTEK
Model : SV 35A
Serial Number : 73246
ID : UAE.EFM.104/2561
Class : 1
Range : 94 , 114 dB / 1000 Hz
Instrument Status : Used

Calibration Environment and Details

Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 15 June 2022
Calibration Date : 1 July 2022
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	31 May 2023
THD Multimeter	2015	1047765	NIMT	2 February 2023

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : Mr. Pacit Mathavorn
Calibration Engineer Supervisor
Issue Date : 1 July 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 22-ACT-405
Request No : Req-2022-1080

Calibration Results : Without Adjustment						
Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 1 (± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	93.80	-0.20	-	-	0.12	0.25
114 dB / 1000 Hz	113.77	-0.23	-	-	0.11	0.25

Frequency of Sound pressure level						
Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.10	0.70
114 dB / 1000 Hz	1000.00	0.00	-	-	0.10	0.70

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)						
Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 1 (± %)
	Measured (%)		Measured (%)			
94 dB / 1000 Hz	0.09		-		0.40	2.5
114 dB / 1000 Hz	0.31		-		0.40	2.5

Note :

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate of Calibration

Customer Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260
Certificate No : 22-ACT-036
Request No : Req-2022-0095

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : LARSON DAVIS
Model : LxT2
Serial Number : 0005400
ID : UAE.EFM.037/2564
Resolution : 0.1 dB
Microphone Class : 2
Microphone Model : 375A04
Microphone S/N : 328676
Preamplifier Model : PRMLxT2C
Preamplifier S/N : 073803
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 14 January 2022
Calibrated Date : 21 January 2022
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	15 September 2022	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	14 June 2022	TSI
Audio Generator	Svante	Svan401	131	18 October 2022	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppadon Luangart
Calibration Officer

Approved By : Mr. Pacit Mathavorn
Calibration Engineer Supervisor
Issue Date : 21 January 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 22-ACT-036
Request No : Req-2022-0095

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		Adjust		UNCERTAINTY	Acceptance
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	(± dB)	Limit
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)		
1000 Hz 114.00 dB	113.85	113.9	+0.05	113.9	0.05	0.20	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN.58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(± dB)
UUC Weighting		
A	29.0	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(± dB)
UUC Weighting		
A	28.8	0.10
C	28.2	0.10
Z	32.9	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A	C	Z		
FAST / 37-139	(dB)	(dB)	(dB)	(± dB)	(± dB)
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)
125 Hz	-0.1	0.1	0.0	0.50	2.0
1000 Hz	0.0	0.0	0.0	0.60	1.0
4000 Hz	0.5	0.5	0.6	0.60	3.0
8000 Hz	0.4	0.4	0.5	0.70	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovator Instrument Co., Ltd.
เอกสารไม่ควบคุม date 01/07/19

Certificate No : 22-ACT-036
Request No : Req-2022-0095

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)		
FAST / 37-139	(dB)	(dB)	(dB)	(± dB)	(± dB)
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)
63 Hz	-0.2	-0.1	0.0	0.2	2.0
125 Hz	-0.1	0.0	0.0		1.5
250 Hz	-0.1	0.0	0.0		1.5
500 Hz	-0.1	0.0	0.0		1.5
1000 Hz	0.0	0.0	0.0		1.0
2000 Hz	0.0	0.0	0.0		2.0
4000 Hz	0.0	0.0	0.0		3.0
8000 Hz	-0.1	0.0	0.0		5
16000 Hz	-0.1	-0.1	0.0		+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC	ERR		
FAST / 37-139	REF	(dB)	(dB)	(± dB)	(± dB)
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	(± dB)
A	114.00	114.0	0.0	0.2	0.2
C	114.00	114.0	0.0		0.2
Z	114.00	114.0	0.0		0.2

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC	ERR		
37-139 / A	REF	(dB)	(dB)	(± dB)	(± dB)
UUC Time Response	(dB)	(dB)	(dB)	(± dB)	(± dB)
Fast	114.00	114.0	0.0	0.2	0.1
Slow	114.00	114.0	0.0		0.1
Leq	114.00	114.0	0.0		0.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovator Instrument Co., Ltd.
เอกสารไม่ควบคุม date 01/07/19

Certificate No : 22-ACT-036
Request No : Req-2022-0095

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37-139	UUC	(± dB)	(± dB)
STD Setting	(dB)	(± dB)	(± dB)
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC	ERR		
FAST / A / 37-139	REF	(dB)	(dB)	(± dB)	(± dB)
STD dB	(dB)	(dB)	(dB)	(± dB)	(± dB)
139.00	139	139.0	0.0	0.3	1.1
134.00	134	134.0	0.0		1.1
129.00	129	129.0	0.0		1.1
124.00	124	124.0	0.0		1.1
119.00	119	119.0	0.0		1.1
114.00	114	114.0	0.0		1.1
109.00	109	109.0	0.0		1.1
104.00	104	104.0	0.0		1.1
99.00	99	99.0	0.0		1.1
94.00	94	93.9	-0.1		1.1
89.00	89	88.9	-0.1		1.1
84.00	84	83.9	-0.1		1.1
79.00	79	78.9	-0.1		1.1
74.00	74	73.9	-0.1		1.1
69.00	69	69.0	0.0		1.1
64.00	64	63.9	-0.1		1.1
59.00	59	59.0	0.0		1.1
54.00	54	54.0	0.0		1.1
49.00	49	49.0	0.0		0.8
44.00	44	44.1	0.1		1.1
39.00	39	39.3	0.3		1.1
38.00	38	38.3	0.3		1.1
37.00	37	37.5	0.5		1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovator Instrument Co., Ltd.
เอกสารไม่ควบคุม date 01/07/19

Certificate No : 22-ACT-036
Request No : Req-2022-0095

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC	ERR		
FAST / A	REF	(dB)	(dB)	(± dB)	(± dB)
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)
37-139	42.9	43.2	0.3	0.3	1.1
	114	114.0	0.0		1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
			UUC	ERR		
A / 37-139	Toneburst	Ref	(dB)	(dB)	(± dB)	(± dB)
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)
Fast	200	135.0	135.0	0.0	0.3	1
	2	118.0	117.8	-0.2		+1.0, -2.5
	0.25	109.0	108.8	-0.2		+1.5, -5.0
Slow	200	128.6	128.5	-0.1		1
	2	109.0	108.8	-0.2		+1.0, -5.0
	0.25	100.0	99.9	-0.1		+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC	ERR		
FAST / C / 95-142	REF	(dB)	(dB)	(± dB)	(± dB)
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)
Complete cycle	137.4	136.9	-0.50	0.2	3.0
Positive half cycle	136.4	136.2	-0.20		2.0
Negative half cycle	136.4	136.2	-0.20		2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovator Instrument Co., Ltd.
เอกสารไม่ควบคุม date 01/07/19

Certificate No : 22-ACT-036
Request No : Req-2022-0095

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37-139	UUC	(± dB)	(± dB)
STD Setting	(dB)		
Positive one-half cycle	142.1		
Negative one-half cycle	141.9		
Deviated	0.2	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance Limit
FAST / A / 37-139	UUC	(± dB)	(± dB)
STD Setting	(dB)		
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 22-ACT-103
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok Request No : Req-2022-0230
10260

Unit Under Calibration Details

Measurement item : Sound Level Meter Microphone Class : 2
Manufacturer : LARSON DAVIS Microphone Model : 375A04
Model : LxT2 Microphone S/N : 328668
Serial Number : 0005402 Preamplifier Model : PRMLxT2C
ID : UAE.EFM.038/2564 Preamplifier S/N : 071540
Resolution : 0.1 dB Intrument Status : Used

Calibration Environment and Details


Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 31 January 2022
Calibrated Date : 11 February 2022
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic


Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	15 September 2022	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	14 June 2022	TSI
Audio Generator	SvanteK	Svan401	131	18 October 2022	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Calibration Officer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor
Issue Date : 11 February 2022

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.0 Issue date 01/07/11

เอกสารไม่ควบคุม

Certificate No : 22-ACT-103
Request No : Req-2022-0230

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		Adjust		UNCERTAINTY	Acceptance
FAST / A / 37-139		UUC	ERR	UUC	ERR		
Calibrator Setting	Level	(dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)
1000 Hz 114.00 dB	113.85	114.0	+0.15	113.9	0.05	0.20	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN:58079

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		(± dB)
UUC Weighting	(dB)	
A	28.1	0.10

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		(± dB)
UUC Weighting	(dB)	
A	28.1	0.10
C	27.9	0.10
Z	34.4	0.10

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY	Acceptance Limit
FAST / 37-139	A	C	Z	(± dB)	(± dB)
STD Setting	(dB)	(dB)	(dB)		
125 Hz	0.0	0.1	0.1	0.50	2.0
1000 Hz	0.0	0.0	0.0	0.60	1.0
4000 Hz	0.9	0.9	1.0	0.60	3.0
8000 Hz	0.7	0.7	0.8	0.70	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.0 Issue date 01/07/11

เอกสารไม่ควบคุม

Certificate No : 22-ACT-103
Request No : Req-2022-0230

5. Electrical signal test of frequency weightings, Weighting network responce with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY	Acceptance Limit
FAST / 37-139	A (dB)	C (dB)	Z (dB)	(± dB)	(± dB)
STD Setting					
63 Hz	-0.2	0.0	0.0	0.2	2.0
125 Hz	-0.1	0.0	0.0		1.5
250 Hz	-0.1	0.0	0.0		1.5
500 Hz	-0.1	0.0	0.0		1.5
1000 Hz	0.0	0.0	0.0		1.0
2000 Hz	0.0	0.1	0.0		2.0
4000 Hz	0.0	0.0	0.0		3.0
8000 Hz	0.0	0.0	0.0		5.0
16000 Hz	-0.1	-0.1	-0.1		+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit
FAST / 37-139	REF	UUC	ERR	(± dB)	(± dB)
UUC Weighting	(dB)	(dB)	(dB)		
A	114.00	114.0	0.0	0.2	0.2
C	114.00	114.0	0.0		0.2
Z	114.00	114.0	0.0		0.2

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance Limit
37-139 / A	REF	UUC	ERR	(± dB)	(± dB)
UUC Time Responce	(dB)	(dB)	(dB)		
Fast	114.00	114.0	0.0	0.2	0.1
Slow	114.00	114.0	0.0		0.1
Leq	114.00	114.0	0.0		0.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-SLM-01 Rev.0 Issue date 01/07/11

เอกสารไม่ควบคุม

Certificate No : 22-ACT-103
Request No : Req-2022-0230

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC		
STD Setting	(dB)		
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting		Anticipated		Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139		REF	UUC	ERR			
STD dB		(dB)	(dB)	(dB)			
139.00		139	139.0	0.0	0.3		1.1
134.00		134	134.0	0.0			1.1
129.00		129	129.0	0.0			1.1
124.00		124	124.0	0.0			1.1
119.00		119	119.0	0.0			1.1
114.00		114	114.0	0.0			1.1
109.00		109	109.0	0.0			1.1
104.00		104	104.0	0.0			1.1
99.00		99	99.0	0.0			1.1
94.00		94	94.0	0.0			1.1
89.00		89	89.0	0.0			1.1
84.00		84	84.0	0.0			1.1
79.00		79	79.0	0.0			1.1
74.00		74	74.0	0.0			1.1
69.00		69	69.0	0.0			1.1
64.00		64	64.0	0.0			1.1
59.00		59	59.0	0.0			1.1
54.00		54	54.0	0.0			1.1
49.00		49	49.0	0.0			1.1
44.00		44	44.0	0.0			1.1
39.00		39	39.3	0.3			1.1
38.00		38	38.3	0.3			1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd
FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-103
Request No : Req-2022-0230

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance
FAST / A		REF	UUC		ERR
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)
37-139	43.2	42.9	-0.3	0.3	1.1
	114	114.0	0.0		1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance
A / 37-139	Toneburst	Ref	UUC	ERR		Limit
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)
Fast	200	135.0	135.0	0.0	0.3	1.0
	2	118.0	117.7	-0.3		+1.0, -2.5
	0.25	109.0	108.7	-0.3		+1.5, -5.0
Slow	200	128.6	128.5	-0.1		1.0
	2	109.0	108.9	-0.1		+1.0, -5.0
SEL	200	129.0	129.0	0.0		1.0
	2	109.0	109.0	0.0		+1.0, -2.5
	0.25	100.0	99.9	-0.1		+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance
FAST / C / 95-142	REF (dB)	UUC (dB)	ERR (dB)		Limit (± dB)
STD Setting					
Complete cycle	137.4	136.7	-0.70	0.2	3.0
Positive half cycle	136.4	136.1	-0.30		2.0
Negative half cycle	136.4	136.2	-0.20		2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd
FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม

Certificate No : 22-ACT-103
Request No : Req-2022-0230

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance
FAST/ A / 37-139	UUC		Limit
STD Setting	(dB)		(± dB)
Positive one-half cycle	142.2		
Negative one-half cycle	142.3		
Deviated	-0.1	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)		(± dB)
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd
FM-708-SLM-01 Rev.0 Issue date 01/07/15

เอกสารไม่ควบคุม