



๐ ๔ พุทธศักราช ๒๕๖๔

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๑๒ กรกฎาคม ๒๕๖๔

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด จำนวน ๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด ขอต่ออายุหนังสือ  
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๑๙ สถานที่ตั้งเลขที่ ๖๓/๑๓ ซอยเพชรเกษม ๗  
แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด  
ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- |                           |               |              |
|---------------------------|---------------|--------------|
| ๑) นายธวัชชัย จงวุฒิชัย   | ทะเบียนเลขที่ | ว-๒๑๙-ค-๕๑๒๔ |
| ๒) นางสาวปณิดา พันธะจักษ์ | ทะเบียนเลขที่ | ว-๒๑๙-ค-๖๖๙๙ |
| ๓) นางสาวจามจุรี คำปุย    | ทะเบียนเลขที่ | ว-๒๑๙-ค-๖๖๖๓ |

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์

- |  |               |              |
|--|---------------|--------------|
| ๑) นางสาวธัญชนก ชำขุน                  | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๔๑๖ |
| ๒) ว่าที่ร้อยตรีหญิงสาวตรี เวียงจันทร์ | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๔๑๗ |
| ๓) นางสาวภาณุชนารถ เชื้อวชาญ           | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๔๑๘ |
| ๔) นางสาววันวิสา หวังแวกลาง            | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๔๑๙ |
| ๕) นางสาวธิดารัตน์ กลัดตลาด            | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๔๒๐ |
| ๖) นางสาวรัตตชา ศรีปราสาท              | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๔๒๑ |
| ๗) นางสาวแพรวพรรณ กองกะแซง             | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๔๒๒ |
| ๘) นางสาวจุลชา สมบุญ                   | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๔๒๓ |
| ๙) นางสาวนิจินา มะติยาภักดิ์           | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๔๒๔ |
| ๑๐) นางสาวเบญจพร อินแก้ว               | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๖๖๔ |
| ๑๑) นายธนทัต เวชกิจ                    | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๖๖๕ |
| ๑๒) นายปริญญา กล้าน้อย                 | ทะเบียนเลขที่ | ว-๒๑๙-จ-๙๖๖๖ |

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๙ รายการ และ  
อากาศเสีย จำนวน ๕ รายการ รวมทั้งสิ้น ๑๔ รายการ ตามสิ่งที่ส่งมาด้วย



หนังสือฉบับนี้จะหมดอายุในวันที่ ๑๕ สิงหาคม ๒๕๖๗ หากประสงค์จะต่ออายุหนังสือ  
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อ  
กรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางจินดา เตชะศรีนทร์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน  
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน  
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ  
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๔-๖  
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙  
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.gmail.go.th



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด เลขทะเบียน ว-๒๑๙  
ที่ อก ๐๓๑๐(๑)/ ๑ ๐ ๔๓ ๑ ลงวันที่ ๐๔ พฤศจิกายน ๒๕๖๔

ขอข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๔ รายการ

**น้ำเสีย จำนวน 9 รายการ**

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method <sup>[3]</sup> 2) 5-Day BOD Test, Membrane Electrode Method <sup>[3]</sup>
2	Free Chlorine	Iodometric Method <sup>[3]</sup>
3	Oil & Grease	Liquid-Liquid, Partition-Gravimetric Method <sup>[3]</sup>
4	pH	Electrometric Method <sup>[3]</sup>
5	Sulfide	Iodometric Method <sup>[3]</sup>
6	Temperature	Laboratory and Field Methods <sup>[3]</sup>
7	Total Dissolved Solids	Dried at 180 °C <sup>[3]</sup>
8	Total Kjeldahl Nitrogen	Macro-Kjeldahl Method <sup>[3]</sup>
9	Total Suspended Solids	Dried at 103-105 °C <sup>[3]</sup>

**อากาศเสีย (ปล่องระบาย) จำนวน 5 รายการ**

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Carbon Monoxide	Instrumental Analyzer <sup>[4]</sup>
2	Opacity	Ringelmann's Method <sup>[1,2]</sup>
3	Oxides of Nitrogen	Instrumental Analyzer <sup>[4]</sup>
4	Sulfur Dioxide	Instrumental Analyzer <sup>[4]</sup>
5	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method <sup>[4]</sup>

**เอกสารอ้างอิง**

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณ  
เขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แก๊สเป็นเชื้อเพลิง.  
ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125 ง.
2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณ  
เขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงงาน. ราชกิจจานุเบกษา. 4 ธันวาคม 2549.  
เล่มที่ 123 ตอนพิเศษ 125 ง.
3. APHA, AWWA, WEF. Standard Methods for the Examination of Water and  
Wastewater. 23<sup>rd</sup> ed. Washington, DC: APHA, 2017.
4. United States Environmental Protection Agency. Standards of Performance for  
New Stationary Sources. 40 CFR 60. Appendix A, 2018.

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

และทะเบียนห้องปฏิบัติการ





ที่ อก ๐๓๑๐(๑)/ ๑ ๒ ๓ ๗ ๒

กรมโรงงานอุตสาหกรรม  
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท  
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒ ๘ สิงหาคม ๒๕๖๖

เรื่อง ขันทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอชวีอี จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๑๘ พฤษภาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
บริษัท เอชวีอี จำกัด จำนวน ๒ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอชวีอี จำกัด ขอขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน พร้อม  
รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์และรายการสารมลพิษ  
ที่จะทำการวิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอชวีอี จำกัด ขันทะเบียนห้องปฏิบัติการ  
วิเคราะห์เอกชน มีเลขทะเบียน ว-๓๕๘ สถานที่ตั้งเลขที่ ๖๐๓ ซอยจรัญสนิทวงศ์ ๔๖ แขวงบางยี่ขัน  
เขตบางพลัด กรุงเทพมหานคร โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- |                             |                            |
|-----------------------------|----------------------------|
| ๑) นายเอกลักษณ์ สีสลาบริหาร | ทะเบียนเลขที่ ว-๓๕๘-ค-๐๐๐๑ |
| ๒) นางสาวทิพวรรณ วงศ์บุญตัน | ทะเบียนเลขที่ ว-๓๕๘-ค-๐๐๐๒ |
| ๓) นายพล ม่วงใหญ่           | ทะเบียนเลขที่ ว-๓๕๘-ค-๐๐๐๓ |

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์

- |                             |                            |
|-----------------------------|----------------------------|
| ๑) นางสาวสุปรียา หล้าอิน    | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๑ |
| ๒) นางสาวจิราภรณ์ ผงผานอก   | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๒ |
| ๓) นายธรรมรัตน์ จริยวัฒนสุข | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๓ |
| ๔) นางสาวธนภรณ์ กำทา        | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๔ |
| ๕) นางสาวณัฐรดา คงบัน       | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๕ |
| ๖) นายฐานันท์ นิภารัตน์     | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๖ |
| ๗) นายมนโรด สุดจันทร์       | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๗ |

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสียและอากาศเสีย ตามสิ่งที่

ส่งมาด้วย

หนังสือฉบับ...



หนังสือฉบับนี้มีอายุครั้งละ ๓ ปี นับจากวันที่กรมโรงงานอุตสาหกรรมออกหนังสือหากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนทั้งนี้สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายประสม คำรพงษ์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน  
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th





เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอชวีอี จำกัด

เลขทะเบียน ว-๓๕๘

ที่ อก ๐๓๑๐(๑)/ ๑ ๒ ๓ ๗ ๒

ลงวันที่ ๒๘ สิงหาคม ๒๕๖๖

ขอข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ รายการ

น้ำเสีย จำนวน 30 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
2	Aldicarb sulfone	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
3	Aldicarb sulfoxide	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
5	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
6	Biochemical Oxygen Demand	5-Day BOD Test, Azide Modification Method <sup>[1]</sup>
7	Carbaryl	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
8	Carbofuran	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
9	Chemical Oxygen Demand	Closed Reflux, Titrimetric Method <sup>[1]</sup>
10	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
11	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
12	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
13	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
14	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
15	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
16	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
17	Heptachlo Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1]</sup>
18	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
19	Methiocarb	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
20	Methomyl	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
21	1-Naphthol	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
22	Oil & Grease	Liquid-Liquid, Partition-Gravimetric Method <sup>[1]</sup>
23	Oxamyl	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
24	pH	Electrometric Method <sup>[1]</sup>
25	Propoxur	High-Performance Liquid Chromatographic Method <sup>[1]</sup>
26	Sulfide	Iodometric Method <sup>[1]</sup>
27	Temperature	Laboratory and Field Methods <sup>[1]</sup>
28	Total Dissolved Solids	Dried at 180 °C <sup>[1]</sup>
29	Total Kjeldahl Nitrogen	Macro Kjeldahl Method <sup>[1]</sup>
30	Total Suspended Solids	Dried at 103-105 °C <sup>[1]</sup>



**อากาศเสีย (ปล่อยระบาย) จำนวน 1 รายการ**

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Opacity	Ringelmann's Method <sup>[2]</sup>

**เอกสารอ้างอิง**

1. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23<sup>rd</sup> ed. Washington, DC: APHA, 2017.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำของโรงงาน พ.ศ. 2549. **ราชกิจจานุเบกษา**. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.





Ref No. : 0303/16367

## CERTIFICATE OF TESTING LABORATORY ACCREDITATION

This is to certify that

**HVE Co., Ltd.**

**603 Soi Jarunsanitwong 46, Jarunsanitwong Road,  
Bangyee Khan, Bang Phlat, Bangkok 10700**

has successfully undergone assessment according to ISO/IEC 17025 : 2017  
and under the Bureau of Laboratory Accreditation, Department of Science Service  
for the requirements, regulations and criteria for the competence of testing laboratories

**Accreditation Number TESTING - 0090**

The scope of accreditation is as annexed hereto

Issue date : **22<sup>nd</sup> November 2021**

Expired date : **21<sup>st</sup> November 2025**

Signature : 

(Mrs. Pochaman Tagheen)

Director of Bureau of Laboratory Accreditation

Bureau of Laboratory Accreditation, Department of Science Service,  
Ministry of Higher Education, Science, Research and Innovation





ใบรับรองเลขที่ 21T033/1246

## ใบรับรองห้องปฏิบัติการ

อาศัยอำนาจตามความในพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

ออกใบรับรองฉบับนี้ให้

มหาวิทยาลัยสวนดุสิต

ศูนย์สิ่งแวดล้อม

มีห้องปฏิบัติการตั้งอยู่เลขที่

๒๒๘-๒๒๘/๑-๓ ถนนสีรินธร แขวงบางพลัด เขตบางพลัด กรุงเทพมหานคร

ได้รับการรับรองความสามารถห้องปฏิบัติการทดสอบ

ตามมาตรฐานเลขที่ มอก. 17025-2561 (ISO/IEC 17025 : 2017)

ข้อกำหนดทั่วไปว่าด้วยความสามารถห้องปฏิบัติการทดสอบและสอบเทียบ

หมายเลขการรับรองที่ ทดสอบ ๐๒๘๐

โดยมีสาขาการรับรองตามรายละเอียดแนบท้ายใบรับรอง

ตั้งแต่ วันที่ ๘ มีนาคม พ.ศ. ๒๕๖๔

ถึง วันที่ ๗ มีนาคม พ.ศ. ๒๕๖๗

ออกให้ ณ วันที่ ๑๙ มี.ค. ๒๕๖๔

(นางกมลวรรณ จำเลิศวัฒน์)

รองเลขาธิการ ปฏิบัติราชการแทน

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม



**รายละเอียดแนบท้ายใบรับรองห้องปฏิบัติการทดสอบ**  
**ใบรับรองเลขที่ 21T033/1246**

ชื่อห้องปฏิบัติการ                      ห้องปฏิบัติการทดสอบ ศูนย์สิ่งแวดล้อม มหาวิทยาลัยสวนดุสิต  
ที่อยู่                                      เลขที่ 228-228/1-3 ถนนสีรินธร แขวงบางพลัด เขตบางพลัด กรุงเทพมหานคร  
หมายเลขการรับรองที่                      ทดสอบ 0280  
สถานภาพห้องปฏิบัติการ                      ☒ ถาวร                      ☐ นอกสถานที่                      ☐ชั่วคราว                      ☐ เคลื่อนที่

สาขาทดสอบ	รายการทดสอบ	วิธีทดสอบ
สาขาสิ่งแวดล้อม น้ำและน้ำเสีย (water and wastewater)	- pH 4.0 to 10.0  - Total solids (TS) 20 mg/l to 1 000 mg/l  - Total suspended solids (TSS) 20 mg/l to 1 000 mg/l  - Total dissolved solids (TDS) 20 mg/l to 1 000 mg/l  - Chemical oxygen demand (COD) 40 mg/l to 400 mg/l	- Standard Methods for The Examination of Water and Wastewater, APHA, AWWA, WEF 23 <sup>rd</sup> Edition 2017, part 4500-H <sup>+</sup> B  - Standard Methods for The Examination of Water and Wastewater, APHA, AWWA, WEF 23 <sup>rd</sup> Edition 2017, part 2540 B  - Standard Methods for The Examination of Water and Wastewater, APHA, AWWA, WEF 23 <sup>rd</sup> Edition 2017, part 2540 D  - Standard Methods for The Examination of Water and Wastewater, APHA, AWWA, WEF 23 <sup>rd</sup> Edition 2017, part 2540 C  - Standard Methods for The Examination of Water and Wastewater, APHA, AWWA, WEF 23 <sup>rd</sup> Edition 2017, part 5220 C

ออกให้ ณ วันที่     **๑๙ มี.ค. ๒๕๖๔**

(นางกมลวรรณ ฉ่ำเลิศวัฒน์)  
รองอธิการ ปฏิบัติราชการแทน  
อธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม



## CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : DO METER  
MANUFACTURER : HANNA INSTRUMENTS  
MODEL / TYPE : HI5421/HI76483  
SERIAL NO. : 04240005101/KC1A11T8H  
CLID. NO. : 272101220  
JOB CONTROL NO. : 230425044469

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 25 April 2023

DATE OF ISSUED : 28 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
28 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to  
the International System of Units (SI)

Certificate No. Q23044469

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE	:	DO METER
MANUFACTURER	:	HANNA INSTRUMENTS
MODEL / TYPE	:	HI5421/HI76483
SERIAL NO.	:	04240005101/KC1A11T8H
DATE OF CALIBRATION	:	26 April 2023

---

#### ENVIRONMENT CONDITIONS :

Temperature :  $(25 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-06**. The calibration was performed by direct measurement with Certified Reference Material (CRM).

#### REFERENCE STANDARD USED :

Dissolved Oxygen, Sigma-Alorich Product ID QC3077-500ML .

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Merck Co., Ltd.

Lot LRAD0713.01 , Due Date September 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 % .  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23044469

F3-011-04/01-12

page 2 of 3







**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The table in the following gives the calibration results and associated measurement uncertainties of Do Meter.

## CALIBRATION DATA

Nominal Value ( mg/L )	DUC Reading ( mg/L )	Correction ( mg/L )	Uncertainty ( mg/L )
5.91	5.92	-0.01	± 0.22

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 4 of 54

**This report is valid for the above stated instrument/s only.**

CALIBRATION LABORATORY Co., LTD.

**CLC**

**### End of Certificate ###**

Certificate No. Q23044469

F3-011-04/01-12

page 3 of 3



@clccalibration





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : pH METER  
MANUFACTURER : HANNA INSTRUMENTS  
MODEL / TYPE : HI5521/HI1131  
SERIAL NO. : 04160019101/061334CN  
CLID. NO. : 272101219  
JOB CONTROL NO. : 230425044468

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 25 April 2023

DATE OF ISSUED : 28 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Sukgasem Seehanart  
Calibration Engineer



Approved By :

Mongkol Yotsoontorn  
Authorized Signatory

28 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23044468

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION

### FOR

**NOMENCLATURE** : pH METER  
**MANUFACTURER** : HANNA INSTRUMENTS  
**MODEL / TYPE** : HI5521/HI1131  
**SERIAL NO.** : 04160019101/061334CN  
**DATE OF CALIBRATION** : 26 April 2023

---

#### ENVIRONMENT CONDITIONS :

**Temperature** :  $(25 \pm 2.5) ^\circ\text{C}$  **Relative Humidity** :  $(50 \pm 15) \% \text{ RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-128**. The calibration was performed by direct measurement with Certified Reference Material (CRM).

#### REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06-664-260, 11754256, Lot Number CC728484.

#### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).  
Lot Number. 160221 , 180121. Due Date 05 May 2023.
2. The measurements are traceable to International System of Units (SI) , through Control Company.  
Certificate No. 4281-12405788 , Due Date 30 June 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23044468

F3-011-04/01-12

page 2 of 3







**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

## CALIBRATION DATA

### pH METER RESULT @ 25 °C

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement ( $\pm$ pH)	k Factor
4.000	3.98	132.0	+0.020	0.014	2,20
6.996	7.00	-41.1	-0.004	0.015	2,06
10.007	10.01	192.5	-0.003	0.100	2,05

Technical Note. Setting function CAL 3 point ( 4,7,10 ).

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 91 of 138

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q23044468

F3-011-04/01-12

page 3 of 3



@clccalibration



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMOMETER  
MANUFACTURER : HANNA INSTRUMENTS  
MODEL / TYPE : HI5521/HI7662-W  
SERIAL NO. : 04160019101/0615024N  
CLID. NO. : 232202088  
JOB CONTROL NO. : 230425044467

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 25 April 2023

DATE OF ISSUED : 02 May 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Monthira Treechum  
Calibration Engineer

Approved By :

Mongkol Yotsoontorn  
Authorized Signatory  
02 May 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23044467

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION FOR

NOMENCLATURE : DIGITAL THERMOMETER  
MANUFACTURER : HANNA INSTRUMENTS  
MODEL / TYPE : HI5521/HI7662-W  
SERIAL NO. : 04160019101/0615024N  
DATE OF CALIBRATION : 27 April 2023

### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$  Relative Humidity :  $(55 \pm 10) \% \text{ RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-187** based on **ASTM E 644-11:2019** as calibration guidelines.  
The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
2. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03.
3. IPRT, ASL Model T100-250-1D S/N. L0193A-1-1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd. Certificate No. Q22130792, Due Date 05 January 2024.
2. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0010/66, Due Date 06 November 2023.
3. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand). Certificate No. TT-0166-22, Due Date 01 December 2023.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23044467**

F3-011-04/01-12

page 2 of 3





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The DUC Reading were recorded and the means value were reported of five times measurement in the table below.

## CALIBRATION DATA

### CORRECTION OF TEMPERATURE [ THERMISTOR ]

Immersion depth (mm)	Actual Temperature ( °C )	DUC Reading ( °C )	Correction ( °C )	Uncertainty $\pm$ ( °C )
105	24.00	24.1	-0.10	0.07
	25.01	25.1	-0.09	
	27.00	27.1	-0.10	

Note. Probe  $\varnothing$  3.5 mm

Materials : Metal Sheath.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 35 of 138

**This report is valid for the above stated instrument/s only.**

**### End of Certificate ###**

Certificate No. Q23044467

F3-011-04/01-12

page 3 of 3



@clccalibration





**GIIC Calibration Laboratory**

700/20-21 Phaholyothin Rd., Samsennai, Phayathai,  
Bangkok 10400 Thailand

**Tel** : +66 (02) 615 4999

**Fax** : +66 (02) 615 4644

**E-mail** : cal@giic.co.th



NSC-TISI-TIS 17025  
CALIBRATION 0256

CERTIFICATE No.: CAL00706-23

PAGE : 1

OF : 3

## Certificate of Calibration

Equipment : DIGITAL THERMO-HYGROMETER  
Manufacturer : DIGICON  
Model / Type : TH-03  
Serial No. : 115092766  
ID No. : -  
Customer : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3rd Floor, Phetkasem 7/1, Watthapra,  
Bangkokyai, Bangkok 10600 Thailand.  
C.S.R. No. : H0000744-23  
Received Date : 01 June 2023  
Calibration Date : 08 June 2023 - 09 June 2023

Calibrated By : MR. TONTRAKARN SRIKACHA

Approved By : MR. TONTRAKARN SRIKACHA

Issue Date : 09 June 2023

The uncertainties are for a level of confidence of approximately 95%.

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

OF: 3

GIICLAB-FM-7.8-002 Rev.00 (20/01/20)



CERTIFICATE No.: CAL00706-23

PAGE : 3

OF : 3

## CALIBRATION REPORT

The temperature scale used was based on ITS-90.

All data shown below were as-received values without adjustment.

### Calibration result :

Function : Temperature Measurement.

Standard Temperature (°C)	<sup>1</sup> UUC Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)
10.011	10	-0.011	0.83
24.985	25	0.015	0.91
40.004	40	-0.004	1.0

Function : Humidity Measurement. : ( 25.05 °C )

Standard Humidity (% rh)	<sup>1</sup> UUC Reading (% rh)	Error (% rh)	Uncertainty of Measurement (± % rh)
24.96	21	-3.96	1.8
49.98	42	-7.98	1.8
84.95	80	-4.95	2.9

<sup>1</sup>UUC = Unit Under Calibration

This result of calibration was found accurate as show on data and place of calibration only.

- END -



CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : ELECTRONIC BALANCE  
MANUFACTURER : SARTORIUS  
MODEL / TYPE : BSA224S-CW  
SERIAL NO. : 35790699  
CLID. NO. : 362101186  
JOB CONTROL NO. : 230518053313

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 18 May 2023

DATE OF ISSUED : 08 June 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Chonvit Thongnat  
Calibration Engineer



Approved By :

Mongkol Yotsoontorn  
Authorized Signatory  
08 June 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23053313

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE	:	ELECTRONIC BALANCE
MANUFACTURER	:	SARTORIUS
MODEL / TYPE	:	BSA224S-CW
SERIAL NO.	:	35790699
LOCATION SITE	:	LABORATORY
DATE OF CALIBRATION	:	02 June 2023

---

#### ENVIRONMENT CONDITIONS :

Temperature : 27 °C to 28 °C

Relative Humidity : 54 % to 56 %

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-46** according to **EURAMET cg-18 Version 4.0 (11/2015)**.

The calibration was performed by Comparison with Weight Set which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Weight Set, Mettler Toledo Class E2 S/N. 158850.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).

Certificate No. MM-0120-21, Due Date 17 December 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95%. It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23053313**

F3-011-04/01-12

page 2 of 3



@clccalibration



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

## CALIBRATION DATA


### 1. Error of indications

Nominal Test Value ( g )	Conventional mass ( g )	Display Value ( g )	Error of Balance ( g )	Uncertainty $\pm$ ( mg )	Coverage factor <i>k</i>
Unload	0.0000	0.0000	0.0000	0.06	2,00
20.0000	20.0000	19.9999	-0.0001	0.09	2,00
40.0000	40.0000	40.0000	0.0000	0.12	2,00
60.0000	59.9999	60.0000	+0.0001	0.14	2,00
80.0000	79.9999	80.0000	+0.0001	0.18	2,00
100.0000	100.0000	100.0000	0.0000	0.15	2,00
120.0000	120.0000	120.0000	0.0000	0.29	2,00
140.0000	140.0000	139.9999	-0.0001	0.29	2,00
160.0000	159.9999	160.0000	+0.0001	0.29	2,00
180.0000	179.9999	179.9999	0.0000	0.30	2,00
200.0000	199.9997	199.9997	0.0000	0.29	2,00
220.0000	219.9997	219.9998	+0.0001	0.49	2,00

### 2. Repeatability of indications

Nominal Test Value ( g )	Standard Deviation of Reading ( g )
200.0000	0.00000

### 3. Effect of eccentric application of a load on the indication

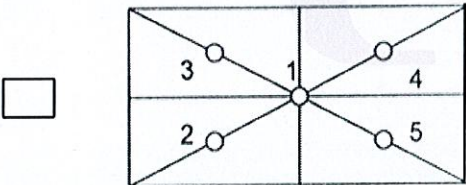						
Nominal Test Value ( g )	Display Value ( g )					Maximum Difference of Center Value ( g )
	Position 1	Position 2	Position 3	Position 4	Position 5	
50.0000	50.0000	50.0000	50.0000	50.0000	50.0000	0.0000

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 116 of 138

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q23053313

F3-011-04/01-12

page 3 of 3



@clccalibration





CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : REFRIGERATOR [FREEZER]  
MANUFACTURER : SHIMAX  
MODEL / TYPE : MAC3D  
SERIAL NO. : N/A[011/190118]  
CLID. NO. : 332200066  
JOB CONTROL NO. : 230518053320

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 18 May 2023

DATE OF ISSUED : 06 June 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Wenick Inchaisri  
Calibration Engineer



Approved By :

Mongkol Yotsoontorn  
Authorized Signatory  
06 June 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units ( SI )

Certificate No. Q23053320

F3-011-04/01-12

page 1 of 4



@clccalibration



## REPORT OF CALIBRATION

### FOR

**NOMENCLATURE** : REFRIGERATOR [FREEZER]  
**MANUFACTURER** : SHIMAX  
**MODEL / TYPE** : MAC3D  
**SERIAL NO.** : N/A[011/190118]  
**LOCATION SITE** : OKLA 67  
**DATE OF CALIBRATION** : 02 June 2023

---

#### ENVIRONMENT CONDITIONS :

Temperature : 29 °C to 30 °C

Relative Humidity : 52 % to 54 %

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-165** according to **TLAS G-20-1/02-08** as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q22066550, Due Date 07 July 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23053320

F3-011-04/01-12

page 2 of 4





## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring refrigerator [freezer].

### CALIBRATION DATA

#### 1. REFRIGERATOR [FREEZER] PERFORMANCE

DUC		Measured Uniformity	Measured Stability	Measured Overall
Setting ( °C )	Indicating ( °C )	( °C )	( °C )	Variation ( °C )
2.0	2.0	1.11	0.16	1.69
4.0	4.0	1.18	0.23	1.74
6.0	6.0	1.25	0.14	1.56





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com




## CALIBRATION DATA

### 2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature ( °C )@Probe No.9 is Ref.									Uncertainty $\pm$ ( °C )	Coverage factor <i>k</i>
Setting ( °C )	Indicating ( °C )	1	2	3	4	5	6	7	8	9		
2.0	2.0	3.03	2.43	1.86	1.58	2.76	2.64	1.83	2.94	2.01	0.52	2,00
4.0	4.0	4.61	4.04	3.50	3.25	4.26	4.01	3.38	4.09	3.53	0.57	2,00
6.0	6.0	6.20	5.61	5.10	4.88	5.88	5.57	4.97	5.58	5.05	0.53	2,00

Technical Note : W = 50 cm, D = 38 cm, H = 125 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 129 of 138

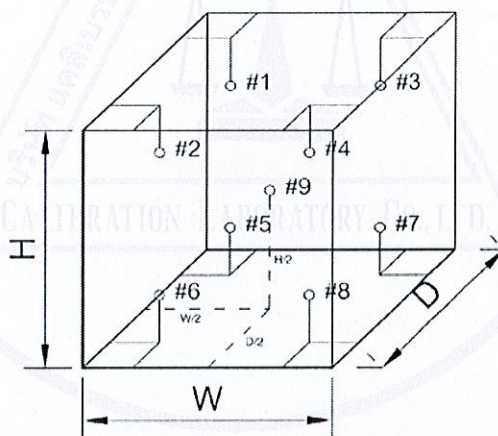

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q23053320

F3-011-04/01-12

page 4 of 4



@clccalibration





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : HOT AIR OVEN  
MANUFACTURER : KWF  
MODEL / TYPE : S0V70B  
SERIAL NO. : KWF2021021902[OKLA-LAB-013/170621]  
CLID. NO. : 332101755  
JOB CONTROL NO. : 230518053317

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 18 May 2023

DATE OF ISSUED : 06 June 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Wenick Inchaisri  
Calibration Engineer



Approved By :

Mongkol Yotsoontorn  
Authorized Signatory  
06 June 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23053317

F3-011-04/01-12

page 1 of 4



@clccalibration



**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

**NOMENCLATURE** : **HOT AIR OVEN**  
**MANUFACTURER** : **KWF**  
**MODEL / TYPE** : **S0V70B**  
**SERIAL NO.** : **KWF2021021902[OKLA-LAB-013/170621]**  
**LOCATION SITE** : **LABORATORY**  
**DATE OF CALIBRATION** : **02 June 2023**

#### ENVIRONMENT CONDITIONS :

Temperature : 29 °C to 30 °C

Relative Humidity : 52 % to 54 %

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-165** according to **TLAS G-20-1/02-08** as calibration guidelines.

The calibration was performed by using Hydra Data Bucket which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Hydra Data Bucket, Fluke Model 2635A S/N. 6496317.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q22098934, Due Date 29 September 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23053317**

**F3-011-04/01-12**

page 2 of 4



@clccalibration





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The table in the following gives the calibration results and associated measurement uncertainties of the measuring hot air oven.

## CALIBRATION DATA

### 1. HOT AIR OVEN PERFORMANCE

DUC		Measured Uniformity ( °C )	Measured Stability ( °C )	Measured Overall Variation ( °C )
Setting ( °C )	Indicating ( °C )			
104.0	104.0	1.77	0.31	2.12
140.0	140.0	2.83	0.54	3.35
160.0	160.0	3.53	0.49	4.30
180.0	180.0	4.31	0.80	5.70

Certificate No. Q23053317

F3-011-04/01-12

page 3 of 4



@clccalibration



**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com




## CALIBRATION DATA

### 2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature ( °C )@Probe No.9 is Ref.									Uncertainty $\pm$ ( °C )	Coverage factor <i>k</i>
Setting ( °C )	Indicating ( °C )	1	2	3	4	5	6	7	8	9		
104.0	104.0	106.36	105.72	106.73	105.53	105.62	105.38	105.19	105.54	106.79	1.15	2,00
140.0	140.0	142.72	141.68	143.28	141.44	141.34	140.66	140.82	141.13	143.12	1.36	2,00
160.0	160.0	162.70	161.52	163.53	161.43	161.04	159.97	160.54	160.68	163.08	1.50	2,00
180.0	180.0	183.26	181.95	184.40	182.07	181.27	179.71	180.88	180.76	183.54	1.70	2,00

Technical Note : W = 40 cm, D = 35 cm, H = 50 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 129 of 138

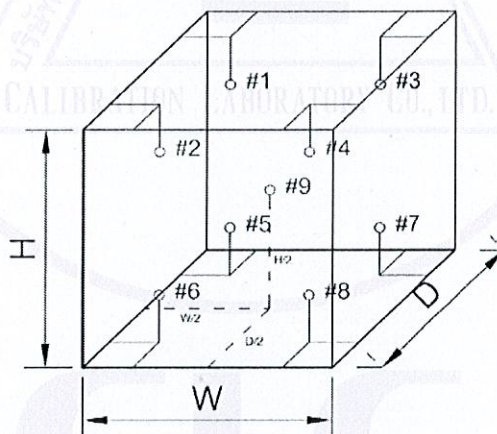

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q23053317

F3-011-04/01-12

page 4 of 4



@clccalibration





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : INCUBATOR  
MANUFACTURER : S-COOL  
MODEL / TYPE : SM 61 M  
SERIAL NO. : 18021147[012/190118]  
CLID. NO. : 332101758  
JOB CONTROL NO. : 230518053316

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 18 May 2023

DATE OF ISSUED : 06 June 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Wenick Inchaisri  
Calibration Engineer



Approved By :

Mongkol Yotsoontorn  
Authorized Signatory  
06 June 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23053316

F3-011-04/01-12

page 1 of 4



@clccalibration





CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : INCUBATOR  
MANUFACTURER : S-COOL  
MODEL / TYPE : SM 61 M  
SERIAL NO. : 18021147[012/190118]  
LOCATION SITE : LABORATORY  
DATE OF CALIBRATION : 02 June 2023

#### ENVIRONMENT CONDITIONS :

Temperature : 29 °C to 30 °C

Relative Humidity : 52% to 54 %

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-165** according to **TLAS G-20-1/02-08** as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q22066550, Due Date 07 July 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23053316

F3-011-04/01-12

page 2 of 4



@clccalibration





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The table in the following gives the calibration results and associated measurement uncertainties of the measuring incubator.

## CALIBRATION DATA

### 1. INCUBATOR PERFORMANCE

DUC		Measured Uniformity ( °C )	Measured Stability ( °C )	Measured Overall Variation ( °C )
Setting ( °C )	Indicating ( °C )			
20.0	20.0	0.61	0.09	1.18

Certificate No. Q23053316

F3-011-04/01-12

page 3 of 4



@clccalibration


## CALIBRATION DATA

### 2. TEMPERATURE DISTRIBUTION

DUC		Measured Temperature ( °C )@Probe No.9 is Ref.									Uncertainty ± ( °C )	Coverage factor <i>k</i>
Setting ( °C )	Indicating ( °C )	1	2	3	4	5	6	7	8	9		
20.0	20.0	20.04	19.81	19.41	19.12	20.11	19.58	19.65	19.44	19.59	0.45	2,00

Technical Note : W = 48 cm, D = 44 cm, H = 130 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 129 of 138

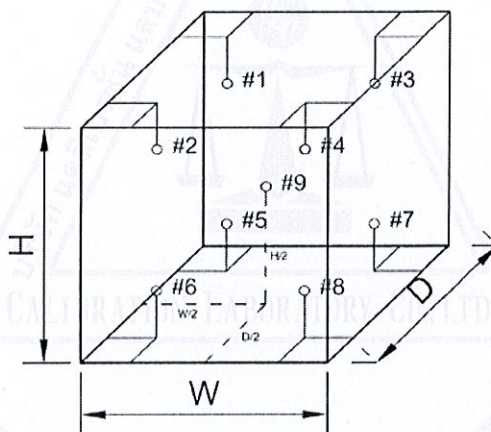

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q23053316

F3-011-04/01-12

page 4 of 4



@clccalibration





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : WATER BATH  
MANUFACTURER : LABTECH  
MODEL / TYPE : LWB-222A  
SERIAL NO. : BCCLJ23001C[OKLA-LAB-008/122011]  
CLID. NO. : 332103272  
JOB CONTROL NO. : 230518053319

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 18 May 2023

DATE OF ISSUED : 06 June 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Wenick Inchaisri

Calibration Engineer



Approved By :

Mongkol Yotsoontorn

Authorized Signatory

06 June 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23053319

F3-011-04/01-12

page 1 of 4



@clccalibration



## REPORT OF CALIBRATION

### FOR

**NOMENCLATURE** : **WATER BATH**  
**MANUFACTURER** : **LABTECH**  
**MODEL / TYPE** : **LWB-222A**  
**SERIAL NO.** : **BCCLJ23001C[OKLA-LAB-008/122011]**  
**LOCATION SITE** : **OKLA TESTING**  
**DATE OF CALIBRATION** : **02 June 2023**

#### ENVIRONMENT CONDITIONS :

Temperature : 29 °C to 30 °C

Relative Humidity : 52% to 54%

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-135** based on **ASTM E 715-80:2016** as calibration guidelines.

The calibration was performed by using Hydra Data Logger which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Hydra Data Logger, Fluke Model 2620 S/N. 5592550.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q23022733, Due Date 01 September 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23053319**

F3-011-04/01-12

page 2 of 4







**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The table in the following gives the calibration results and associated measurement uncertainties of the measuring water bath.

## CALIBRATION DATA

### 1. WATER BATH PERFORMANCE

Test Point ( °C )	DUC Reading ( °C )	Uniformity ( °C )	Stability ( °C )
60	-	0.5	0.3

Certificate No. Q23053319

F3-011-04/01-12

page 3 of 4



@clccalibration



CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC


## CALIBRATION DATA

### 2. TEMPERATURE DISTRIBUTION

Test Point ( ° C )	DUC Reading ( ° C )	STD Reading ( ° C )					Uncertainty $\pm$ ( ° C )
		Probe No. 1	Probe No. 2	Probe No. 3	Probe No. 4	Probe No. 5	
60	-	60.0	60.0	60.1	59.9	60.0	0.9

Technical Note : W = 50 cm, D = 30 cm, H = 15 cm.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 128 of 138

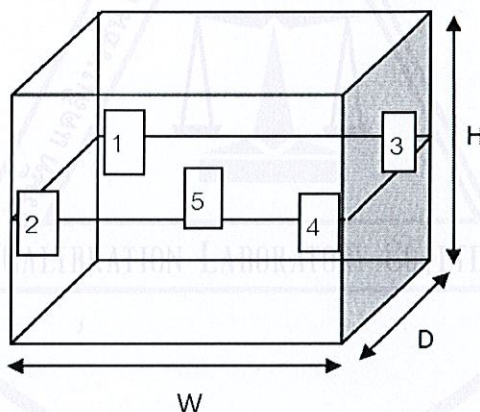

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q23053319

F3-011-04/01-12

page 4 of 4



@clccalibration



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : BURETTE  
MANUFACTURER : ISO LAB  
MODEL / TYPE : 25 ml  
SERIAL NO. : N/A[EM-MBR10002/17]  
CLID. NO. : 272201671  
JOB CONTROL NO. : 230425044052


CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 25 April 2023

DATE OF ISSUED : 02 May 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Sechanart  
Calibration Engineer

Approved By :   
Mongkol Yotsoontorn  
Authorized Signatory  
02 May 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the  
International System of Units (SI)

Certificate No. Q23044052

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION FOR

NOMENCLATURE : BURETTE  
MANUFACTURER : ISO LAB  
MODEL / TYPE : 25 ml  
SERIAL NO. : N/A[EM-MBR10002/17]  
DATE OF CALIBRATION : 27 April 2023

### ENVIRONMENT CONDITIONS :

Temperature :  $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 10) \% \text{ RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-86** according to **ASTM E542-01:2021** as calibration guidelines.

The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23044052**

F3-011-04/01-12

page 2 of 3







CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

## CALIBRATION DATA

### CORRECTION OF VOLUME

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
5	5.0003	+0.0003	0.0038	2,00
15	15.0044	+0.0044	0.0066	2,00
25	25.0092	+0.0092	0.0068	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 94 of 138

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q23044052

F3-011-04/01-12

page 3 of 3



@clccalibration

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : CYLINDER  
MANUFACTURER : FAVORIT  
MODEL / TYPE : 50 ml  
SERIAL NO. : N/A [EM-VPP02501/21]  
CLID. NO. : 272300782  
JOB CONTROL NO. : 230328034770

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 04 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Sukgasem Seehanart  
Calibration Engineer



Approved By :

Mongkol Yotsoontorn

Authorized Signatory

04 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23034770

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION FOR

NOMENCLATURE : CYLINDER  
MANUFACTURER : FAVORIT  
MODEL / TYPE : 50 ml  
SERIAL NO. : N/A [EM-VPP02501/21]  
DATE OF CALIBRATION : 31 March 2023

### ENVIRONMENT CONDITIONS :

Temperature :  $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 10) \% \text{ RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-84** according to **ASTM E542-01:2021** as calibration guidelines.  
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer  
which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.  
Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.  
Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.  
Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.  
Certificate No. Q23010604, Due Date 02 February 2024.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23034770**

F3-011-04/01-12

page 2 of 3



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

## CALIBRATION DATA

### CORRECTION OF VOLUME

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
50	50.1999	+0.1999	0.0180	2,00

Type of glassware : ☒ to Contain ☐ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 94 of 138

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q23034770

F3-011-04/01-12

page 3 of 3



@clccalibration



## CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : CYLINDER  
MANUFACTURER : BOROSIL  
MODEL / TYPE : 500 ml  
SERIAL NO. : 0334-58  
CLID. NO. : 272201292  
JOB CONTROL NO. : 230328034769

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 04 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
04 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the  
International System of Units ( SI )

Certificate No. Q23034769

F3-011-04/01-12

page 1 of 3



@clccalibration

## REPORT OF CALIBRATION FOR

NOMENCLATURE : CYLINDER  
MANUFACTURER : BOROSIL  
MODEL / TYPE : 500 ml  
SERIAL NO. : 0334-58  
DATE OF CALIBRATION : 31 March 2023

### ENVIRONMENT CONDITIONS :

Temperature :  $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 10) \% \text{ RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-84** according to **ASTM E542-01:2021** as calibration guidelines.  
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model Secura6102-1s S/N.0042104938.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22121337, Due Date 01 December 2023.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034769

F3-011-04/01-12

page 2 of 3



@clccalibration



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

## CALIBRATION DATA

### CORRECTION OF VOLUME

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
500	498.75	-1.25	0.10	2,00

Type of glassware : ☒ to Contain ☐ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 94 of 138

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q23034769

F3-011-04/01-12

page 3 of 3



@clccalibration

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : MEASURING PIPETTE  
MANUFACTURER : GLASSCO  
MODEL / TYPE : 1 ml  
SERIAL NO. : N/A[EM-MER01001/19]  
CLID. NO. : 272201297  
JOB CONTROL NO. : 230328034780

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
03 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the  
International System of Units ( SI )

Certificate No. Q23034780

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION FOR

NOMENCLATURE : MEASURING PIPETTE  
MANUFACTURER : GLASSCO  
MODEL / TYPE : 1 ml  
SERIAL NO. : N/A[EM-MER01001/19]  
DATE OF CALIBRATION : 29 March 2023

### ENVIRONMENT CONDITIONS :

Temperature :  $(20 \pm 2.5) ^\circ\text{C}$  Relative Humidity :  $(50 \pm 10) \% \text{ RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.  
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23034780**

F3-011-04/01-12

page 2 of 3



@clccalibration



**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

## CALIBRATION DATA

### CORRECTION OF VOLUME

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
*0.1	0.1015	+0.0015	0.0024	2,00
*0.5	0.5012	+0.0012	0.0025	2,00
1	1.0003	+0.0003	0.0025	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. \* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

**This report is valid for the above stated instrument/s only.**

**CLC**

### End of Certificate ###

Certificate No. Q23034780

F3-011-04/01-12

page 3 of 3



@clccalibration



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : MEASURING PIPETTE  
MANUFACTURER : GLASSCO  
MODEL / TYPE : 5 ml  
SERIAL NO. : N/A[EM-MER01001/18]  
CLID. NO. : 272201296  
JOB CONTROL NO. : 230328034779

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory

03 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the  
International System of Units (SI)

Certificate No. Q23034779

F3-011-04/01-12

page 1 of 3



@clccalibration

## REPORT OF CALIBRATION FOR

NOMENCLATURE : MEASURING PIPETTE  
MANUFACTURER : GLASSCO  
MODEL / TYPE : 5 ml  
SERIAL NO. : N/A[EM-MER01001/18]  
DATE OF CALIBRATION : 29 March 2023

### ENVIRONMENT CONDITIONS :

Temperature :  $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 10) \% \text{ RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.  
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. **Q23034779**

F3-011-04/01-12

page 2 of 3



@clccalibration





CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

## CALIBRATION DATA

### CORRECTION OF VOLUME

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
*0.5	0.5034	+0.0034	0.0025	2,00
2.5	2.4871	-0.0129	0.0029	2,00
5	4.9818	-0.0182	0.0029	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. \* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

This report is valid for the above stated instrument/s only.

CLC

### End of Certificate ###

Certificate No. Q23034779

F3-011-04/01-12

page 3 of 3



@clccalibration



**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : MEASURING PIPETTE  
MANUFACTURER : GLASSCO  
MODEL / TYPE : 10 ml  
SERIAL NO. : N/A[EM-MER01001/17]  
CLID. NO. : 272000237  
JOB CONTROL NO. : 230328034778

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
03 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the  
International System of Units ( SI )

Certificate No. Q23034778

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION FOR

NOMENCLATURE : MEASURING PIPETTE  
MANUFACTURER : GLASSCO  
MODEL / TYPE : 10 ml  
SERIAL NO. : N/A[EM-MER01001/17]  
DATE OF CALIBRATION : 29 March 2023

### ENVIRONMENT CONDITIONS :

Temperature :  $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 10) \% \text{ RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.  
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034778

F3-011-04/01-12

page 2 of 3



@clccalibration

**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

## CALIBRATION DATA

### **CORRECTION OF VOLUME**

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
1	1.0058	+0.0058	0.0025	2,00
5	4.9937	-0.0063	0.0029	2,00
10	9.9802	-0.0198	0.0039	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

**This report is valid for the above stated instrument/s only.**

**### End of Certificate ###**

Certificate No. Q23034778

F3-011-04/01-12

page 3 of 3



@clccalibration





**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : VOLUMETRIC PIPETTE  
MANUFACTURER : GLASSCO  
MODEL / TYPE : 20 ml  
SERIAL NO. : N/A[EM-VPP20201/17]  
CLID. NO. : 272101208  
JOB CONTROL NO. : 230328034775

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Sukgasem Sechanart  
Calibration Engineer



Approved By :

Mongkol Yotsoontorn  
Authorized Signatory  
03 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23034775

F3-011-04/01-12

page 1 of 3



@clccalibration

## REPORT OF CALIBRATION FOR

NOMENCLATURE : VOLUMETRIC PIPETTE  
MANUFACTURER : GLASSCO  
MODEL / TYPE : 20 ml  
SERIAL NO. : N/A[EM-VPP20201/17]  
DATE OF CALIBRATION : 29 March 2023

### ENVIRONMENT CONDITIONS :

Temperature :  $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 10) \% \text{ RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.  
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034775

F3-011-04/01-12

page 2 of 3



@clccalibration





CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

## CALIBRATION DATA

### **CORRECTION OF VOLUME**

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
20	20.0020	+0.0020	0.0072	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q23034775

F3-011-04/01-12

page 3 of 3



@clccalibration



**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025  
CALIBRATION 0059  
CLC

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VOLUMETRIC PIPETTE  
MANUFACTURER : HBG  
MODEL / TYPE : 25 ml  
SERIAL NO. : N/A[EM-VPP02501/17]  
CLID. NO. : 272000238  
JOB CONTROL NO. : 230328034774

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 03 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Sukgasem Seehanart  
Calibration Engineer



Approved By :

Mongkol Yotsoontorn

Authorized Signatory

03 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23034774

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION FOR

NOMENCLATURE : VOLUMETRIC PIPETTE  
MANUFACTURER : HBG  
MODEL / TYPE : 25 ml  
SERIAL NO. : N/A[EM-VPP02501/17]  
DATE OF CALIBRATION : 29 March 2023

### ENVIRONMENT CONDITIONS :

Temperature :  $(20 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 10) \% \text{ RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-89** according to **ASTM E542-01:2021** as calibration guidelines.  
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23034774

F3-011-04/01-12

page 2 of 3



@clccalibration

**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

## CALIBRATION DATA

### CORRECTION OF VOLUME

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
25	24.9589	-0.0411	0.0076	2,00

Type of glassware : ☐ to Contain ☒ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 96 of 138

**This report is valid for the above stated instrument/s only.**

CALIBRATION LABORATORY Co., LTD.

**CLC**

### End of Certificate ###

Certificate No. Q23034774

F3-011-04/01-12

page 3 of 3



@clccalibration



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VOLUMETRIC FLASK  
MANUFACTURER : SCI  
MODEL / TYPE : 100 ml  
SERIAL NO. : N/A[EM-VPP02501/17]  
CLID. NO. : 272101212  
JOB CONTROL NO. : 230328034773

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 05 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory

05 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the  
International System of Units (SI)

Certificate No. Q23034773

F3-011-04/01-12

page 1 of 3



@clccalibration

## REPORT OF CALIBRATION

### FOR

**NOMENCLATURE** : **VOLUMETRIC FLASK**  
**MANUFACTURER** : **SCI**  
**MODEL / TYPE** : **100 ml**  
**SERIAL NO.** : **N/A[EM-VPP02501/17]**  
**DATE OF CALIBRATION** : **03 April 2023**

#### ENVIRONMENT CONDITIONS :

**Temperature :**  $(20 \pm 2.5) ^\circ\text{C}$

**Relative Humidity :**  $(50 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-88** according to **ASTM E542-01:2021** as calibration guidelines.  
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model CPA224S S/N.23908487.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

#### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23019117, Due Date 22 February 2024.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

**Certificate No. Q23034773**

**F3-011-04/01-12**

page 2 of 3



@clccalibration



## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

### CALIBRATION DATA

#### CORRECTION OF VOLUME

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
100	99.9589	-0.0411	0.0190	2,00

Type of glassware : ☒ to Contain ☐ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 95 of 138

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q23034773

F3-011-04/01-12

page 3 of 3



@clccalibration

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VOLUMETRIC FLASK  
MANUFACTURER : BOROSIL  
MODEL / TYPE : 500 ml  
SERIAL NO. : N/A[EM-VPP02501/18]  
CLID. NO. : 272201295  
JOB CONTROL NO. : 230328034772

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.  
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,  
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 28 March 2023

DATE OF ISSUED : 06 April 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory

06 April 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the  
International System of Units (SI)

Certificate No. Q23034772

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION FOR

**NOMENCLATURE** : **VOLUMETRIC FLASK**  
**MANUFACTURER** : **BOROSIL**  
**MODEL / TYPE** : **500 ml**  
**SERIAL NO.** : **N/A[EM-VPP02501/18]**  
**DATE OF CALIBRATION** : **03 April 2023**

### ENVIRONMENT CONDITIONS :

**Temperature** :  $(20 \pm 2.5) ^\circ\text{C}$

**Relative Humidity** :  $(50 \pm 10) \% \text{RH}$

### PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-88** according to **ASTM E542-01:2021** as calibration guidelines.  
The calibration was performed by using Electronic Balance, Thermo-hygrograph, Barometer and Thermometer which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Barometer, Barigo S/N.001.
2. Electronic Balance, Sartorius Model Secura6102-1s S/N.0042104938.
3. Thermo-hygrograph, Isuzu Model 3-3126 S/N.30760420.
4. Thermometer, Brannan S/N. 1.

### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23006081, Due Date 19 January 2024.
2. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22121337, Due Date 01 December 2023.
3. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q22130804, Due Date 04 January 2024.
4. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd. Certificate No. Q23010604, Due Date 02 February 2024.

### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

**Certificate No. Q23034772**

**F3-011-04/01-12**

page 2 of 3



@clccalibration



## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The calibration was performed by applied volume to the Device Under Calibration (DUC) . The actual volume readings from STD were reported in average of seven times measurements.

### CALIBRATION DATA

#### CORRECTION OF VOLUME

DUC Test point ( ml )	Actual volume ( ml )	Correction ( ml )	Uncertainty $\pm$ ( ml )	Coverage factor $k$
500	500.04	+0.04	0.09	2,00

Type of glassware : ☒ to Contain ☐ to Deliver

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 95 of 138

**This report is valid for the above stated instrument/s only.**

CALIBRATION LABORATORY Co.,LTD.

CLC

### End of Certificate ###

Certificate No. Q23034772

F3-011-04/01-12

page 3 of 3



@clccalibration