ภาคผนวก จ

ใบรับรองการสอบเทียบเครื่องมือ

right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Suspended Particulate	High Volume	SGK_FS0119	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	BKK_EN0004	8-Feb-23	8-Feb-24	12
Ambient	Particulate Matter (PM-10)	High Volume	SGK_FS0087	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	BKK_EN0004	8-Feb-23	8-Feb-24	12
Ambient	Nitrogen Dioxide	NO_2 Analyzer	BKK_FS1084	1-Jul-23	1-Jan-24	6
Ambient	Sulfur Dioxide	SO_2 Analyzer	SGK_FS0095	2-Jul-23	2-Jan-24	6
Ambient	Carbon Monoxide	CO Analyzer	SGK_FS0068	1-Jul-23	1-Jan-24	6
Ambient	Total Hydrocarbon	THC Analyzer	BKK_FS0804	1-Jul-23	1-Jan-24	6
Songkhla Lab	Total Coliform	Autoclave	SGK_ML0001	5-Jan-23	5-Jul-24	18
Songkhla Lab	Total Coliform	Incubator	SGK_ML0013	6-Aug-22	6-Feb-24	18
Songkhla Lab	Total Coliform	pH Meter	SGK_ML0016	5-Jan-23	5-Jul-24	18
Songkhla Lab	Total Coliform	Water Bath	SGK_ML0021	30-Jan-23	30-Jul-24	18
Songkhla Lab	Fecal Coliform	Autoclave	SGK_ML0001	5-Jan-23	5-Jul-24	18
Songkhla Lab	Fecal Coliform	Incubator	SGK_ML0013	6-Aug-22	6-Feb-24	18
Songkhla Lab	Fecal Coliform	pH Meter	SGK_ML0016	5-Jan-23	5-Jul-24	18
Songkhla Lab	Fecal Coliform	Water Bath	SGK_ML0021	30-Jan-23	30-Jul-24	18
Songkhla Lab	*Staphylococcus aureus*	Autoclave	SGK_ML0002	5-Jan-23	5-Jul-24	18
Songkhla Lab	*Staphylococcus aureus*	Incubator	SGK_ML0013	6-Aug-22	6-Feb-24	18
Songkhla Lab	*Staphylococcus aureus*	pH meter	SGK_ML0016	5-Jan-23	5-Jul-24	18
Songkhla Lab	*Escherichia coli*	Autoclave	SGK_ML0002	5-Jan-23	5-Jul-24	18
Songkhla Lab	*Escherichia coli*	Incubator	SGK_ML0013	6-Aug-22	6-Feb-24	18
Songkhla Lab	*Escherichia coli*	pH meter	SGK_ML0016	5-Jan-23	5-Jul-24	18
Songkhla Lab	*Escherichia coli*	Water Bath	SGK_ML0021	30-Jan-23	30-Jul-24	18
Songkhla Lab	BOD	Incubator	SGK_CL0028	13-Jul-23	13-Jan-25	18
Songkhla Lab	BOD	DO/BOD Analyser	SGK_CL0073	21-Nov-22	21-May-24	18
Songkhla Lab	pH at 25 °C	pH meter	SGK_CL0030	28-Apr-23	28-Oct-24	18
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Oil & Grease	Water Bath	SGK_CL0035	13-Jul-23	13-Jan-25	18
Songkhla Lab	Sulfide	Cold Room Water	SGK_CL0065	31-Jan-23	31-Jul-24	18
Songkhla Lab	Total Dissolved Solids 103-105℃	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Dissolved Solids 103-105℃	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	25-Jan-23	25-Jan-24	12
Songkhla Lab	Total Suspended Solids	Oven	SGK_CL0024	28-Apr-23	28-Oct-24	18
Songkhla Lab	Residual Free Chlorine	Chlorine Meter	SGK_FS0048	16-Mar-23	16-Mar-24	12
Songkhla Lab	Total Chlorine	Chlorine Meter	SGK_FS0048	16-Mar-23	16-Mar-24	12
Water Lab	Cyanuric acid	Spectrophotometer	SGK_CL0038	24-Jan-23	24-Jan-24	12
Water Lab	Ammonium	Discrete analyzer	BKK_EN0037	12-Jul-23	12-Jul-24	12
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0366	17-May-23	17-May-24	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	12-Jul-23	12-Jul-24	12
Water Lab	*Pseudomonas aeruginosa*	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	*Pseudomonas aeruginosa*	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	*Pseudomonas aeruginosa*	Water Bath	BKK_ML0049	19-Jan-23	19-Jan-24	12
Water Lab	*Pseudomonas aeruginosa*	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	*Clostridium perfringens*	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	*Clostridium perfringens*	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	*Clostridium perfringens*	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Water Lab	*Legionella spp.*	Balance	BKK_ML0001	8-Feb-23	8-Feb-24	12
Water Lab	*Legionella spp.*	Autoclave	BKK_ML0041	4-Oct-23	4-Apr-25	18
Water Lab	*Legionella spp.*	Incubator	BKK_ML0189	3-Oct-23	3-Oct-24	12
Water Lab	*Legionella spp.*	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18

High Volume Air Sampler Calibration Worksheet

Project Site :	Stone Bitter Co.,Ltd.	**Barometric Pressure (mm Hg) :**	754
Calibrate Location :	ที่จอดรถยนต์ภายนอกอาคาร	**Temperature (°C) :**	29
Calibrate Date :	23-Nov-23	**High Volume ID :**	SGK_FS0119
CalibrationSheet No.:	**C-231123-SGK_FS0119**	**High Volume Model :**	TE-5170D
Calibrator ID:	SGK_FS0034	**High Volume S/N :**	1062
Calibrator Model :	TE-5028A	**Calibrator Slope :**	1.55835
Calibrator S/N :	3449	**Calibrator Intercept :**	-0.0282

Test No.	Delta H_2O (inch)	Q_{std} (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.4	1.0118	40	Slope : 40.6723
2	3.2	1.1640	46	Intercept : -1.2900
3	3.8	1.2659	50	Correlation Coefficient : 0.9998
4	4.4	1.3600	54	
5	5.4	1.5036	60	

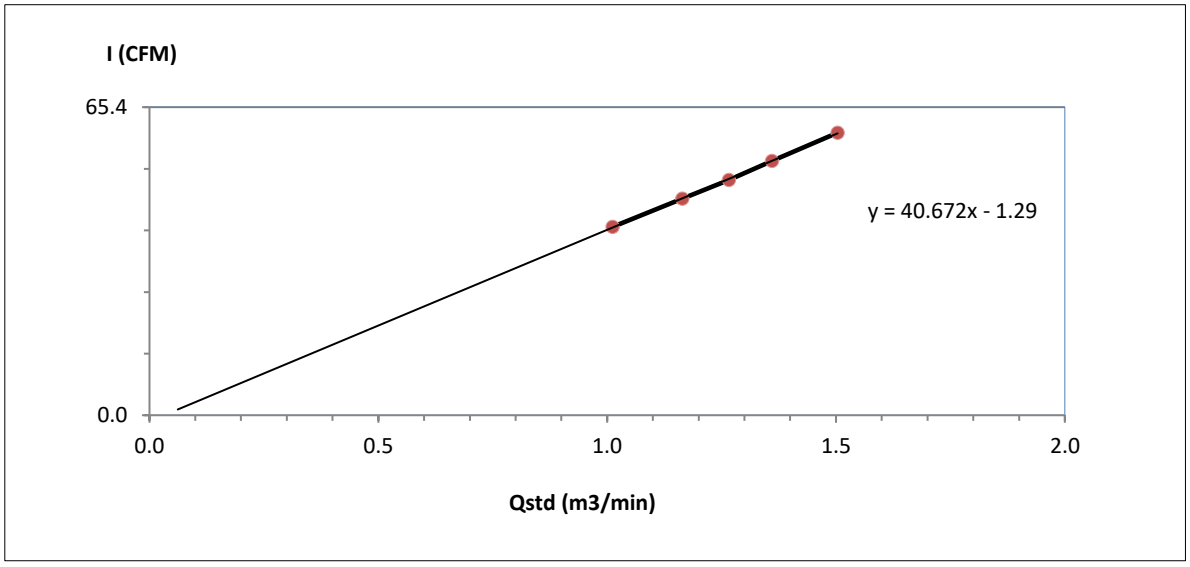

Calibrated by _____

(Mr.Apiwat Chanta)
Field Scientist(2)

Approved by : _____

(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 , e-mail: service.thailand@sartorius.com

NSC-TISI-TIS 17025
CALIBRATION 0426

SARTORIUS

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 8/2/24

Certificate of Calibration

Model Number :	XP105DU	Certificate No. :	23BCI0071
Description :	Semi-micro Balance	Issued Date :	Monday, February 13, 2023
Serial Number :	1123091884	Reference No. :	203245
ID No.	BKK_EN0004		
Manufacturer :	Mettler Toledo	Page No. :	1 0f 3

Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.
104 Phatthanakan 40,Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.

Calibrated Place : Balance Room.

Calibrated By : Mr. Chonchai Inthana
Calibration Date : Wednesday, February 08, 2023

Calibration Procedure No. : This calibration was conducted by
Using in-house calibration procedure number (WI-003)
Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 31/120 g Readability : 0.0001 g

Ambients Conditions:

Temperature :	21.0 °C	±	3.0 °C
Humidity :	65.0 % RH	±	5.0 % RH
Pressure	_	±	_

Reasons for calibration

☐ New Installation ☐ Service / Repaired ☑ Re-calibration/ Maintenance

Equipment Condition: ☑ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Cetificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 1kg E2 s/n 37929119	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Mr.Chonchai Inthana(Technical Manager)

STAMP

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 Fax: +66 2643-8367,

SARTORIUS

Certificate of Calibration

Model Number :	XP105DU	Certificate No. :	23BCI0071
Description :	Semi-micro Balance	Issued Date :	Monday, February 13, 2023
Serial Number :	1123091884	Reference No. :	203245
ID No.	BKK_EN0004		
Manufacturer :	Mettler Toledo	Page No. :	2 of 3

Calibration Results : Without Adjustment

Repeatability

The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)		
2 g	2.00002	20.00002
Tolerance	2.00001	20.00001
N/A g	2.00002	20.00001
	2.00002	20.00001
	2.00002	20.00000
Nominal Value : (High Load)	2.00002	20.00000
20 g	2.00002	20.00001
Tolerance	2.00002	20.00000
N/A g	2.00001	20.00000
	2.00001	20.00001
Standard Deviation	0.000005	0.000007

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximim capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 20 g
Tolerance *N/A* g





	Difference
1	–
2	-0.00002
3	-0.00004
4	0.00002
5	0.00003
6	–

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance *N/A* g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.1	0.10000	0.10000	0.00000	0.000022
0.5	0.50001	0.50000	-0.00001	0.000023
1	1.00000	1.00000	0.00000	0.000024
2	2.00002	2.00001	-0.00001	0.000026
5	5.00002	5.00002	0.00000	0.000030
10	10.00002	10.00002	0.00000	0.000035
15	15.00004	15.00004	0.00000	0.000053
20	20.00000	20.00000	0.00000	0.000053
25	25.00002	25.00002	0.00000	0.000089
30	30.00002	30.00004	0.00002	0.000089

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 Fax: +66 2643-8367,

SARTORIUS

Certificate of Calibration

Model Number : XS105DU
Description : Semi-micro Balance
Serial Number : 1123091884
ID No. BKK_EN0004
Manufacturer : Mettler Toledo

Certificate No. : 23BCI0071
Issued Date : Monday, February 13, 2023
Reference No. : 203245

Calibration Results : Without Adjustment

Repeatability

The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load) g
Tolerance *N/A* g

Nominal Value : (High Load) 100 g
Tolerance *N/A* g

	100.0000
	100.0000
	100.0000
	100.0000
	100.0000
	100.0000
	100.0000
	99.9999
	100.0000
	100.0000
Standard Deviation	0.00003

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximim capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : g
Tolerance *N/A* g





	Difference
1	–
2	–
3	–
4	–
5	–
6	–

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance *N/A* g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
50	50.0000	50.0000	0.0000	0.00012
55	55.0000	55.0000	0.0000	0.00015
60	60.0000	60.0000	0.0000	0.00015
65	65.0001	65.0001	0.0000	0.00015
70	70.0000	70.0000	0.0000	0.00015
80	80.0000	80.0000	0.0000	0.00017
90	90.0001	90.0001	0.0000	0.00018
100	100.0000	100.0000	0.0000	0.00018
110	110.0000	110.0000	0.0000	0.00026
120	120.0000	120.0000	0.0000	0.00026

End of Report.

High Volume Air Sampler Calibration Worksheet

Project Site :	Stone Bitter Co.,Ltd.	**Barometric Pressure (mm Hg) :**	754
Calibrate Location :	ที่จอดรถยนต์ภายนอกอาคาร	**Temperature (°C) :**	29
Calibrate Date :	23-Nov-23	**High Volume ID :**	SGK_FS0087
CalibrationSheet No.:	**C-231123-SGK_FS0087**	**High Volume Model :**	TE-5009X
Calibrator ID:	SGK_FS0034	**High Volume S/N :**	5993
Calibrator Model :	TE-5028A	**Calibrator Slope :**	0.97611
Calibrator S/N :	3449	**Calibrator Intercept :**	-0.01774

Test No.	Delta H_2O (inch)	Qa (m^3/min)	I : Chart (CFM)	Linear Regression
1	2.0	0.935	30	Slope : 50.2820
2	2.4	1.022	36	Intercept : -16.5705
3	3.0	1.141	40	Correlation Coefficient : 0.9944
4	3.4	1.213	44	
5	4.0	1.314	50	

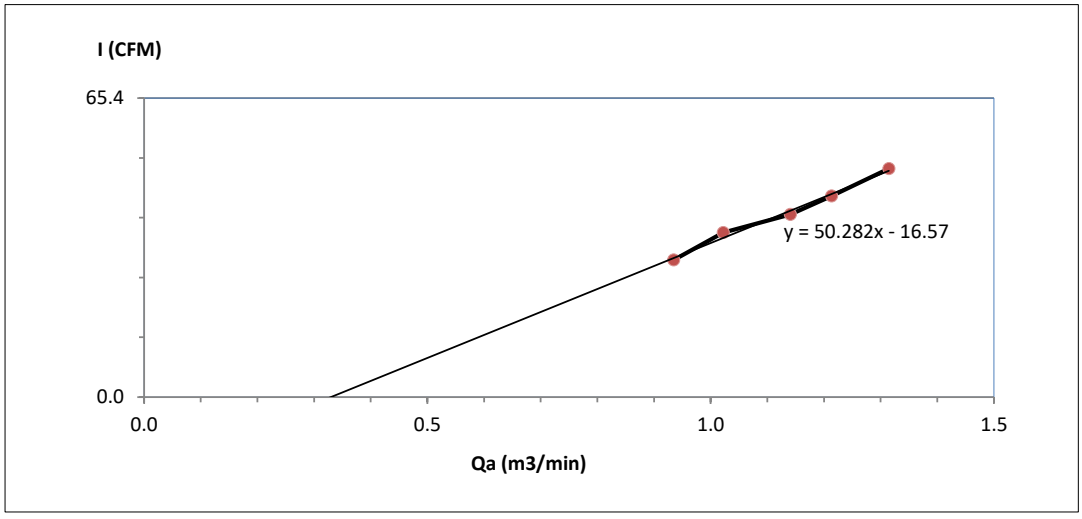

Calibrated by _____

(Mr.Apiwat Chanta)
Field Scientist(2)

Approved by : _____

(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)

MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-23	Equipment Name	NOx Analyzer
Manufacturer	HORIBA	Model	APNA-370
Serial No.	WJ38T7NG	Equipment ID	BKK_FS1084
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.88	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	100.10	0.10	0.10	100.70	0.70	0.70
2	200.00	198.50	-1.50	-0.75	198.30	-1.70	-0.85
3	300.00	301.70	1.70	0.57	301.60	1.60	0.53
4	400.00	401.60	1.60	0.40	402.10	2.10	0.53
AVERAGE (%)				0.08			0.20

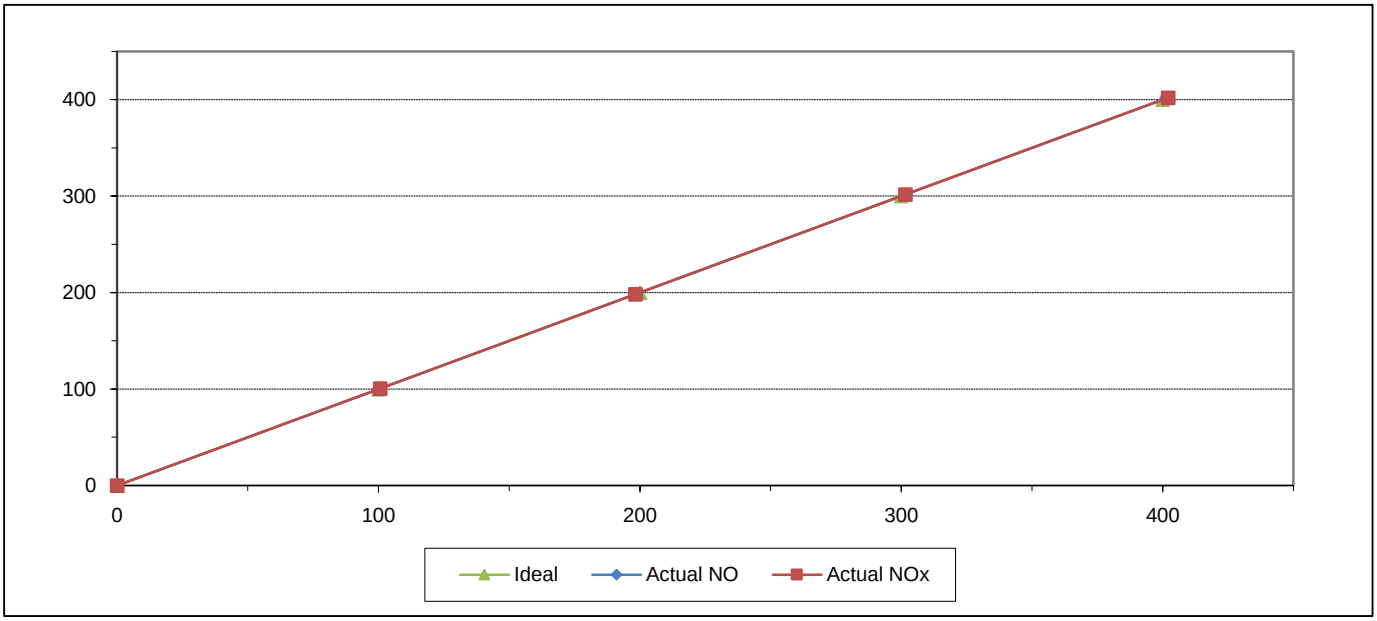

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	2-Jul-23	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	3EYT4WAA	Equipment ID	SGK_FS0095
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.90	-1.10	-1.10
2	200.00	198.60	-1.40	-0.70
3	300.00	298.20	-1.80	-0.60
4	400.00	397.30	-2.70	-0.67
AVERAGE (%)				-0.60

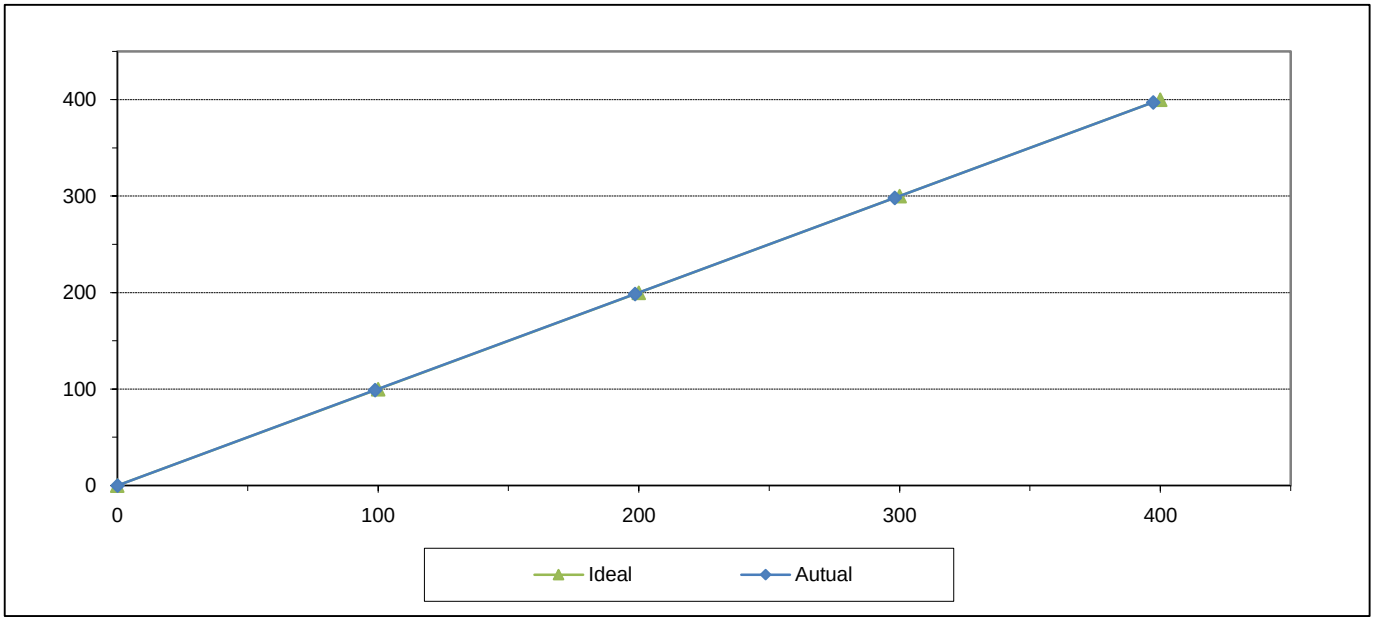

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-23	Equipment Name	CO Analyzer
Manufacturer	Teledyne API	Model	T300
Serial No.	3630	Equipment ID	SGK_FS0068
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	55.22	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Actual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.70	-1.30	-1.30
2	200.00	198.80	-1.20	-0.60
3	300.00	297.40	-2.60	-0.87
4	400.00	395.90	-4.10	-1.03
AVERAGE (%)				-0.74

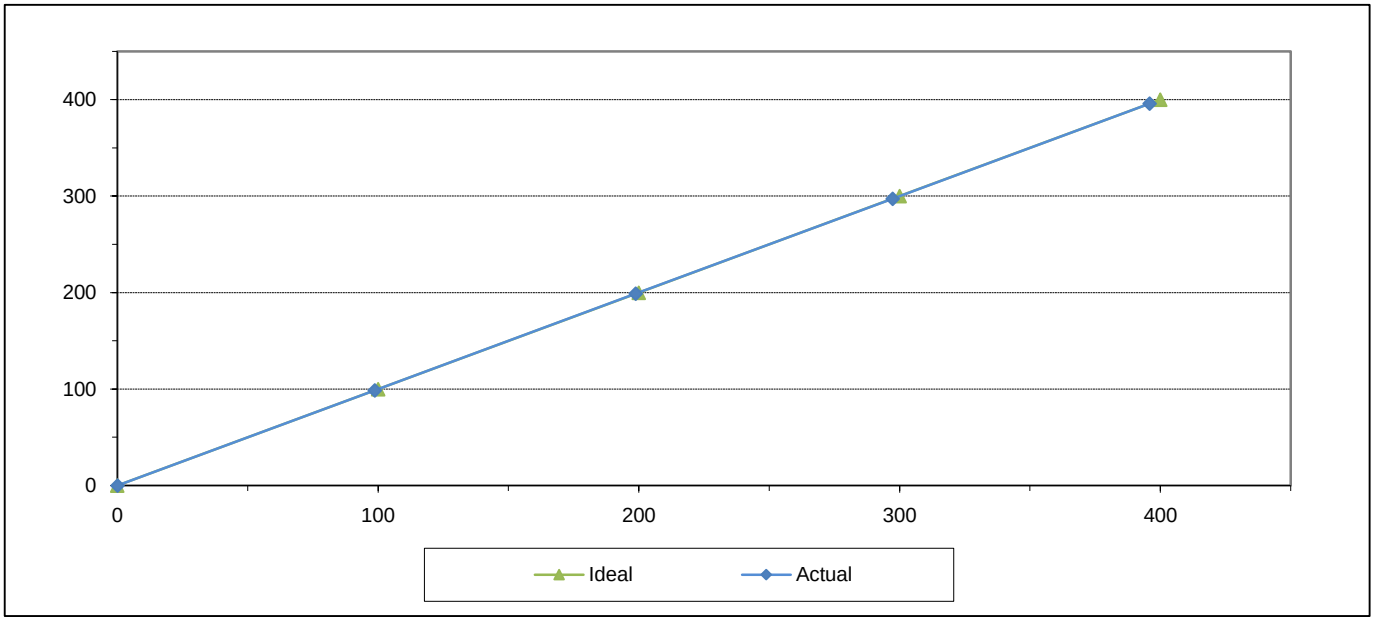

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

MULTIPOINT CALIBRATION REPORT

Calibration Date	1-Jul-23	Equipment Name	THC Analyzer
Manufacturer	HORIBA	Model	APHA-370
Serial No.	TPXJ6KFL	Equipment ID	BKK_FS0804
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Conc. (PPM C3H8)	50.9	Cylinder No.	D612257
Cylinder Pressure (psi)	1800	Certified By	Linde
Certified Date	27-Jun-18	Expired Date	27-Jun-26

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	99.10	-0.90	-0.90
2	200.00	199.80	-0.20	-0.10
3	300.00	298.10	-1.90	-0.63
4	400.00	396.80	-3.20	-0.80
AVERAGE (%)				-0.47

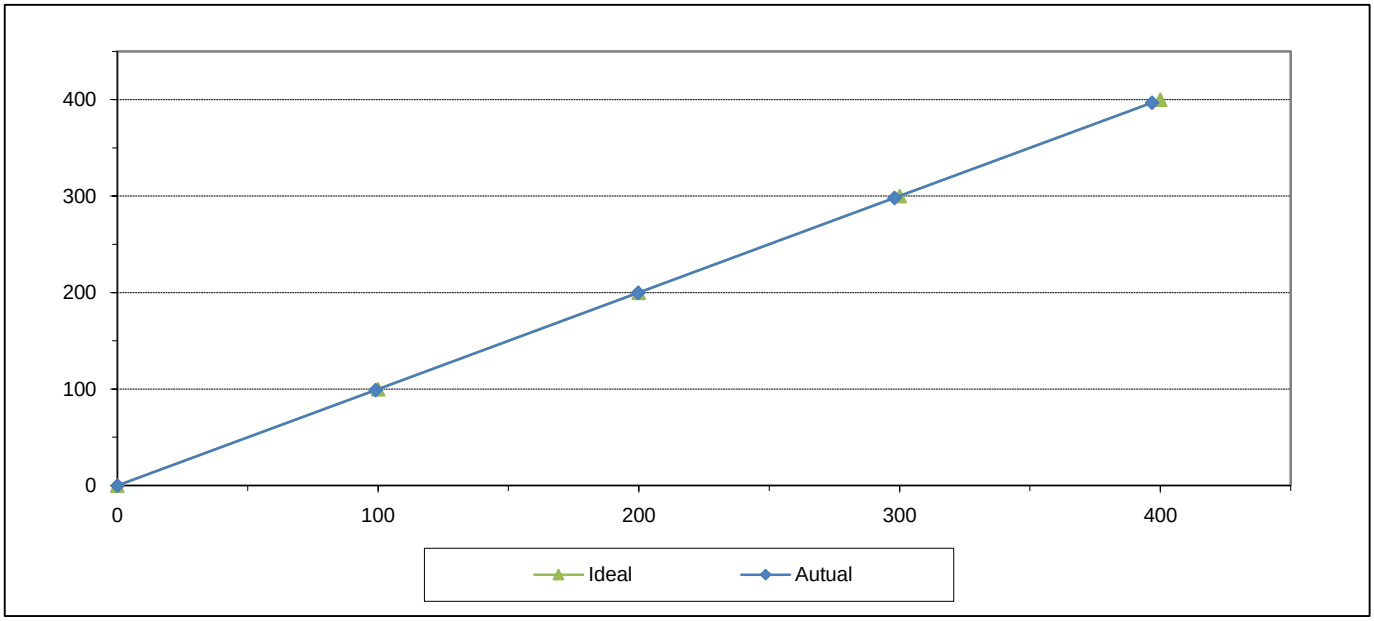

Calibrated By

(Mr.Jirawut Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr.Sarayuth Jittranont)
Assistant General Manager

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

NSC-TISI-TIS17025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 8-Jan-2023

Certificate No. : 23TH0050
CSR No. : A047/02339
Page. : 1 of 3

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru, Amphoe Hat Yai, Songkhla, 90250
Calibration Place	:	Microbiological Laboratory
Instrument Name	:	Autoclave
Manufacturer	:	TOMY
Model	:	SX-700
Serial No.	:	52134079
ID No.	:	SGK_ML0001
Resolution	:	1 °C
Received Date	:	5-Jan-2023
Calibrated Date	:	5-Jan-2023
Ambient Temperature	:	(30 ± 10) °C
Relative Humidity	:	(50 ± 30) %

REVIEW BY ....
APPROVED L. .....
NEXT CAL. DATE 05-Jul-2024

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.16.013 based on BS 2646 : 1993 (part 5)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

SCaL

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	GL220	C90432223	22SDAT005	4-May-2023

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :. (✓) Without Adjustment ( ) After Adjustment

1. Sensor Installation Diagram

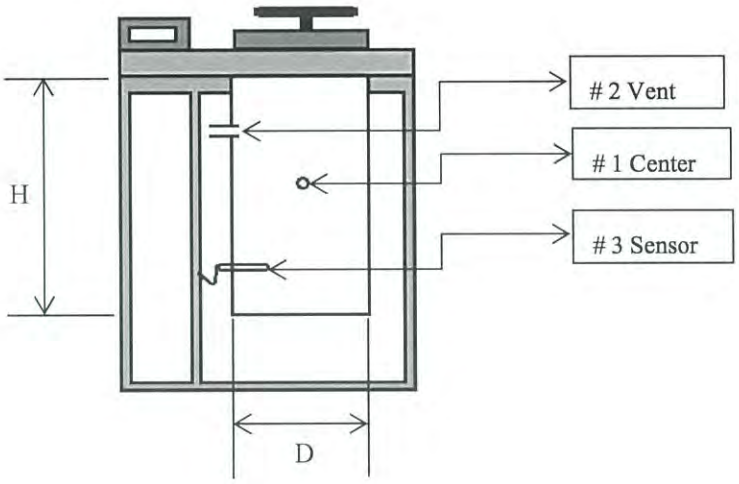

Chamber Diameter (D) : 30 cm

Chamber Height (H) : 70 cm

Result of Calibration :.

2. Temperature Measurement Accuracy Test

The measurement results of the Autoclave and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)			Pressure Reading	Uncertainty (±°C)
	Center #1	Vent #2	Sensor #3		
115	115.5	115.4	115.5	0.07 MPa	0.76
118	118.7	118.9	119.1	0.09 MPa	0.76
121	122.0	122.1	122.1	0.11 MPa	0.76

3. Performance Result

The performance of the Autoclave are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
115	115	115	0.20	0.30	0.30
118	118	118	0.70	0.70	0.90
121	121	121	0.50	0.40	0.60

- Operating Time = 1800.65 sec
- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

... End ...

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

NSC-TISI-TIS17025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 9-Aug-2022

Certificate No. : 22OV529
CSR No. : A037/01847

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru, Amphoe Hat Yai, Songkhla, 90250
Calibration Place	:	Microbiological Laboratory
Instrument Name	:	Incubartor
Manufacturer	:	Memmert
Model	:	ICP750
Serial No.	:	F816.0061
ID No.	:	SGK_ML0013
Resolution	:	0.1 °C
Received Date	:	6-Aug-2022
Calibrated Date	:	6-Aug-2022
Ambient Temperature	:	(30 ± 10) °C
Relative Humidity	:	(50 ± 30) %

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 06/02/2024

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on G-20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

SCaL

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisiton/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :. (✓) Without Adjustment ( ) After Adjustment

1. Sensor Installation Diagram

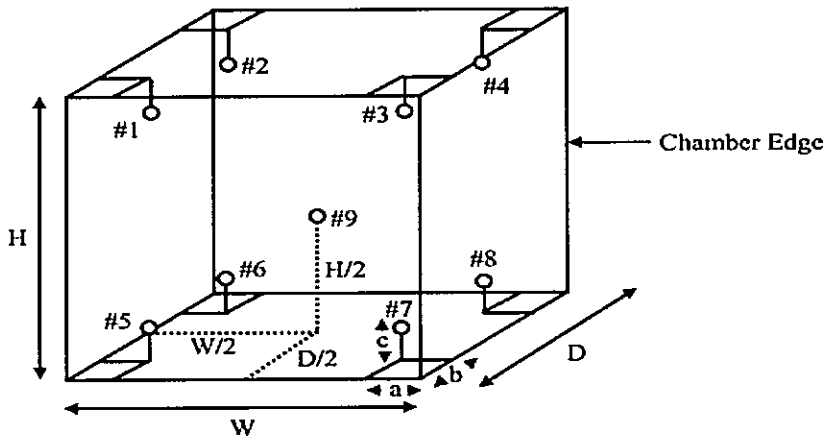

Sensor Installation Details			Dimension of the chamber		
a =	5.0	cm	W =	104.0	cm
b =	5.0	cm	H =	120.0	cm
c =	5.0	cm	D =	60.0	cm

SCaL

Certificate No. : 22OV529

CSR No. : A037/01847

Result of Calibration :.

2. Temperature Measurement Accuracy Test

The measurement results of the Incubartor and associates are reported in the manner as shown below

Cal point	Measured Standard Temperature At Spread Locations (°C)									Uncertainty
(°C)	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	(±°C)
35	34.99	34.92	34.95	34.88	34.96	35.00	34.94	34.94	34.94	0.38

3. Performance Result

The performance of the Incubartor are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
35	35.0	35.0	0.10	0.12	0.19

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

NSC-TISI-TIS17025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 8-Jan-2023

Certificate No. : 23CH0016
CSR No. : A047/02339

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru, Amphoe Hat Yai, Songkhla, 90250
Calibration Place	:	Microbiological Laboratory
Instrument Name	:	pH meter
Manufacturer	:	Sartorius
Model	:	Basic pH Meter PB-10
Serial No.	:	C70160695
ID No.	:	SGK_ML0016
Electrode No.	:	N/A
Received Date	:	5-Jan-2023
Calibrated Date	:	5-Jan-2023
Ambient Temperature	:	(25 ± 3) °C
Relative Humidity	:	(55 ± 15) %

REVIEW BY ....!
APPROVED BY
NEXT CAL. DATE 05-Jul-24

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH
- WK : WK Electric Co., Ltd.

Calibrated by : Jessadagon Lemhud

Approved by :

Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02950	1733	22-Apr-2024
Standard Solution	7.000	C03001	1783	23-Sep-2024
Standard Solution	10.013	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :. (✓) Without Adjustment ( ) After Adjustment

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading (mV)	Correction (mV)	Uncertainty (± mV)
177.48	177.4	0.08	0.17
0.00	0.0	0.00	0.13
-177.48	-177.4	-0.08	0.17

2. Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading (pH)	Correction (pH)	Uncertainty (± pH)
4.004	4.02	-0.016	0.011
7.000	7.01	-0.010	0.013
10.013	10.02	-0.007	0.036

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

NSC-TISI-TIST7025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 2-Feb-2023

Certificate No. : 23TH0521
CSR No. : A075/03704
Page. : 1 of 3

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru, Amphoe Hat Yai, Songkhla, 90250
Calibration Place	:	Microbiological Laboratory
Instrument Name	:	Water Bath
Manufacturer	:	Memmert
Model	:	WPE45
Serial No.	:	L716.0558
ID No.	:	SGK_ML0021
Resolution	:	0.1 °C
Received Date	:	30-Jan-2023
Calibrated Date	:	30-Jan-2023
Ambient Temperature	:	(30 ± 10) °C
Relative Humidity	:	(50 ± 30) %

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 30-Jul-24

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

SCaL

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisiton/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :. (✓) Without Adjustment ( ) After Adjustment

1. Sensor Installation Diagram

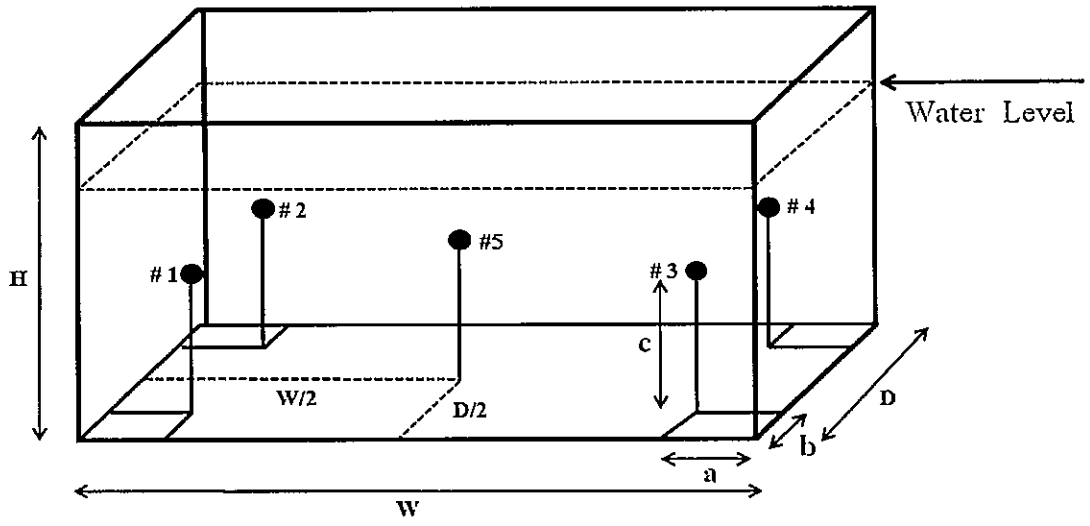

Sensor Installation Details			Dimension of the chamber		
a =	5	cm	W =	45	cm
b =	5	cm	H =	30	cm
c =	5	cm	D =	35	cm

SCaL

Result of Calibration :.

2. Temperature Measurement Accuracy Test

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (±°C)
	#1	#2	#3	#4	Ref.5	
44.5	44.47	44.48	44.45	44.51	44.50	0.14

3. Performance Result

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
44.5	44.5	44.5	0.10	0.24	0.25

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

NSC-TISI-TIS17025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 8-Jan-2023

Certificate No. : 23TH0049

CSR No. : A047/02339

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru, Amphoe Hat Yai, Songkhla, 90250
Calibration Place	:	Microbiological Laboratory
Instrument Name	:	Autoclave
Manufacturer	:	TOMY
Model	:	SX-700
Serial No.	:	52134080
ID No.	:	SGK_ML0002
Resolution	:	1 °C
Received Date	:	5-Jan-2023
Calibrated Date	:	5-Jan-2023
Ambient Temperature	:	(30 ± 10) °C
Relative Humidity	:	(50 ± 30) %

REVIEW BY .....

APPROVED B .....

NEXT CAL. DATE 05 - Jul - 24

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.16.013 based on BS 2646 : 1993 (part 5)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Kanyarat Chaipet / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data logger With Sensor	GL220	C90432223	22SDAT005	4-May-2023

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :. (✓) Without Adjustment ( ) After Adjustment

1. Sensor Installation Diagram

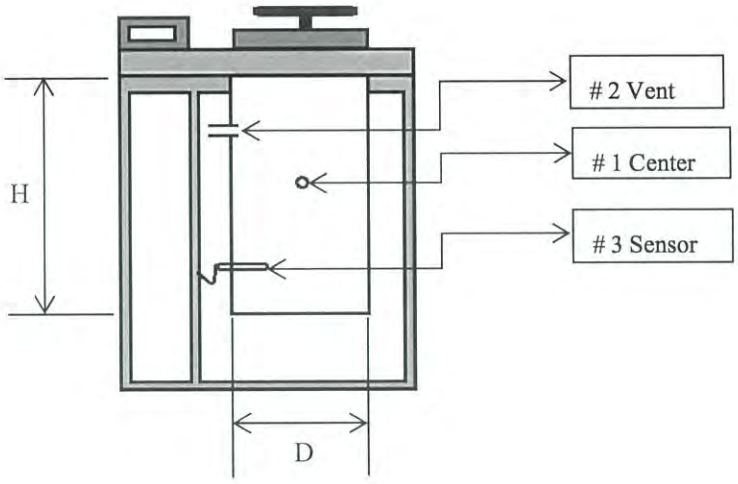

Chamber Diameter (D) : 30 cm

Chamber Height (H) : 70 cm

Result of Calibration :.

2. Temperature Measurement Accuracy Test

The measurement results of the Autoclave and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)			Pressure Reading	Uncertainty (±°C)
	Center #1	Vent #2	Sensor #3		
115	115.1	115.0	115.1	0.07 MPa	0.76
118	119.1	119.0	119.0	0.09 MPa	0.76
121	122.2	122.1	122.1	0.11 MPa	0.76

3. Performance Result

The performance of the Autoclave are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
115	115	115	0.10	0.10	0.40
118	118	118	0.10	0.30	0.30
121	121	121	0.10	0.10	0.20

- Operating Time = 900.45 sec
- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

... End ...

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

NSC-TISI-TIS17025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 16-Jul-2023

Certificate No. : 23TH3096
CSR No. : A095/04743

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru, Amphoe Hat Yai, Songkhla, 90250
Calibration Place	:	Chemical Laboratory
Instrument Name	:	Incubator
Manufacturer	:	Memmert
Model	:	ICP750
Serial No.	:	F816.0063
ID No.	:	SGK_CL0028
Resolution	:	0.1 °C
Received Date	:	13-Jul-2023
Calibrated Date	:	13-Jul-2023
Ambient Temperature	:	(30 ± 10) °C
Relative Humidity	:	(50 ± 30) %

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 13/01/25

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :
Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

SCaL

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisiton/Switch Unit	34970A	MY58009813	23SDAT004	23-May-2024

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :. (✓) Without Adjustment ( ) After Adjustment

1. Sensor Installation Diagram

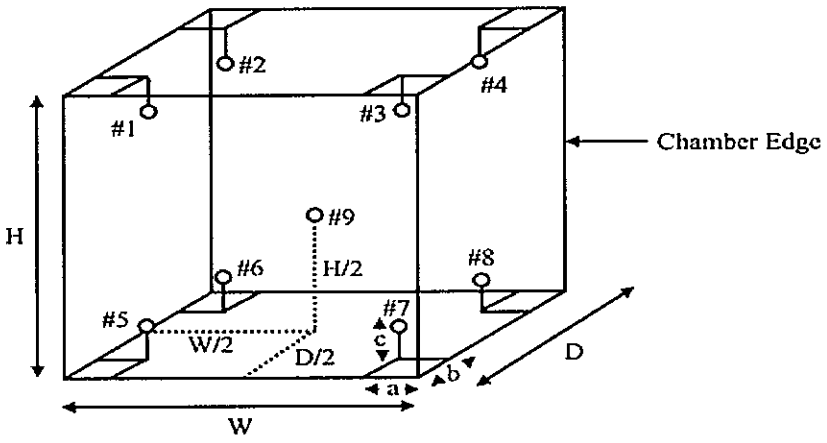

Sensor Installation Details			Dimension of the chamber		
a =	5.0	cm	W =	40.0	cm
b =	5.0	cm	H =	40.0	cm
c =	5.0	cm	D =	33.0	cm

SCaL

Result of Calibration :.

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point	Measured Standard Temperature At Spread Locations (°C)									Uncertainty
(°C)	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	(±°C)
20	20.10	20.04	20.03	19.97	20.08	20.23	20.10	19.94	20.07	0.38

3. Performance Result

The performance of the Incubator are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
20	20.0	20.0	0.14	0.17	0.32

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment :	DO Meter with Sensor
Manufacturer :	YSI
Model :	5000
Serial No. :	17B101473
ID No. :	SGK_CL0073
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8, Kanjanavanij Rd., Banphru,
Location :	TPA Chemistry Calibration Lab.2
Received Order :	18 November 2022
Calibrated Date :	21 November 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
AC Line Voltage :	(220 ± 22) V
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	Approved Signatory

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 21/05/24.

( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 22 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2111-0663DSC-2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Digital Thermometer	1523	3240076	22I249	02 Mar 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17B100103

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor *k*
20.00	60	20.001	19.88	-0.121	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000
Serial No. :	17B101473
ID No. :	SGK_CL0073
Received Date :	18 November 2022
Test Date :	21 November 2022
Reference :	2211-0663DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8, Kanjanavanij Rd., Banphru, Hatyai, Songkhla 90250, Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	_____ Approved Signatory

(✓) Malee Butkruea
( ) Saithip Meangmai
( ) Warakorn Lerngagtrakul

Issue Date : 22 November 2022

Condition of this result of calibration

1. Reference Standard Instruments :
   This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center,Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.12	8.12	0.0045

This report was certified only for the instrument we tested.It is allowable to use for study the system efficiency,The environmental impact control and present to organization it may concerned Intend to use for advertising and referral purpose is prohibited.This report may not be reproduced other in full,without written approval of the laboratory

-o0o-

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

ilac-MRA THAILAND
NSC TISI-TIS17025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23CH0203
CSR No. : A088/04367
Page. : 1 of 2

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru, Amphoe Hat Yai, Songkhla, 90250
Calibration Place	:	Chemical Laboratory
Instrument Name	:	pH meter
Manufacturer	:	Mettler Toledo
Model	:	S220
Serial No.	:	B625631849
ID No.	:	SGK_CL0030
Electrode No.	:	1204613
Received Date	:	28-Apr-2023
Calibrated Date	:	28-Apr-2023
Ambient Temperature	:	(25 ± 3) °C
Relative Humidity	:	(55 ± 15) %

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 28 / 10 /2024

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- HACH : HACH LANGE GmbH
- SCaL : Sounthern Calibration Service Co., Ltd.,
- WK : WK Electric Co., Ltd.

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

SCaL

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.005	C02994	1777	5-Sep-2024
Standard Solution	7.000	C03007	1787	17-Oct-2024
Standard Solution	10.012	C02953	1735	29-Apr-2024
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	5-Jun-2024
Digital Thermometer With Sensor	DP-77	I.360896	22SDTH005	8-Aug-2023

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :.

1. Electrical Measurement

Applied Voltage	pH meter Reading		Correction	Uncertainty
(mV)	(mV)	(pH)	(mV)	(± mV)
177.48	177.5	3.70	-0.02	0.17
0.00	0.0	6.70	0.00	0.13
-177.48	-177.4	9.80	-0.08	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions	pH meter Reading		Correction	Uncertainty
(pH)	(pH)	(mV)	(pH)	(± pH)
4.005	3.97	159.2	0.035	0.0090
6.999	6.98	-15.4	0.019	0.013
10.012	9.95	-188.0	0.062	0.036

3. After Sample Test Measurement

Standard Buffer Solutions	pH meter Reading		Correction	Uncertainty
(pH)	(pH)	(mV)	(pH)	(± pH)
4.005	3.97	158.9	0.035	0.0090
6.999	7.01	-17.5	-0.011	0.013
10.012	9.98	-187.6	0.032	0.036

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (±°C)
25	25.032	25.1	-0.068	0.11

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 , e-mail: service.thailand@sartorius.com

NSC-TISI-TIS 17025
CALIBRATION 0426

SARTORIUS

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 25/1/23 24

Certificate of Calibration

Model Number :	MSE224S-100-DU	Certificate No. :	23BCI0044
Description :	Analytical Balance	Issued Date :	Friday, January 27, 2023
Serial Number :	0034705158	Reference No. :	202361
ID No.	SGK_CL0045		
Manufacturer :	Sartorius	Page No. :	1 0f 2

Customer Name : ALS Laboratory Group (Thailand) Co., Ltd.
Songkhla Branch:114/1 Moo 8 Karnchanawanich Rd.,T. Ban Phru, A. Hat Yai,Songkhla. 90250.

Calibrated Place : Balance Room.

Calibrated By : Mr. Chonchai Inthana
Calibration Date : Wednesday, January 25, 2023

Calibration Procedure No. : This calibration was conducted by
Using in-house calibration procedure number (WI-003)
Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:

Temperature :	22.4 °C	±	3.0 °C
Humidity :	65.0 % RH	±	5.0 % RH
Pressure	_	±	_

Reasons for calibration

☐ New Installation ☐ Service / Repaired ☑ Re-calibration/ Maintenance

Equipment Condition: ☑ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Cetificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 1kg E2 s/n 37929119	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Mr.Chonchai Inthana(Technical Manager)

STAMP

SARTORIUS (THAILAND) CO., LTD. SARTORIUS ISO/IEC 17025:2017

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 Fax: +66 2643-8367,

SARTORIUS

Certificate of Calibration

Model Number :	MSE224S-100-DU	Certificate No. :	23BCI0044
Description :	Analytical Balance	Issued Date :	Friday, January 27, 2023
Serial Number :	0034705158	Reference No. :	202361
ID No.	SGK_CL0045		
Manufacturer :	Sartorius	Page No. :	2 of 2

Calibration Results : Without Adjustment

Repeatability

The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0001	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0000
	20.0000	200.0001
Nominal Value : (High Load)	20.0000	200.0000
200 g	20.0000	200.0001
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0001
	20.0000	200.0001
Standard Deviation	0.00003	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximim capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g
Tolerance *0.0004* g





	Difference
1	–
2	0.0001
3	0.0000
4	0.0000
5	0.0000
6	–

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance *0.0002* g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00013
0.1	0.1000	0.1000	0.0000	0.00013
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	200.0001	0.0001	0.00030

End of Report.

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

ilac-MRA
THAILAND
NSC-TISI-TIS17025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 1-May-2023

Certificate No. : 23TH1728
CSR No. : A088/04367
Page. : 1 of 3

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru, Amphoe Hat Yai, Songkhla, 90250
Calibration Place	:	Chemical Laboratory
Instrument Name	:	Hot Air Oven
Manufacturer	:	Memmert
Model	:	UF110
Serial No.	:	B416.3387
ID No.	:	SGK_CL0024
Resolution	:	0.1 °C
Received Date	:	28-Apr-2023
Calibrated Date	:	28-Apr-2023
Ambient Temperature	:	(30 ± 10) °C
Relative Humidity	:	(50 ± 30) %

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 28/4/2024

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

SCaL

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisiton/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :. (✓) Without Adjustment ( ) After Adjustment

1. Sensor Installation Diagram

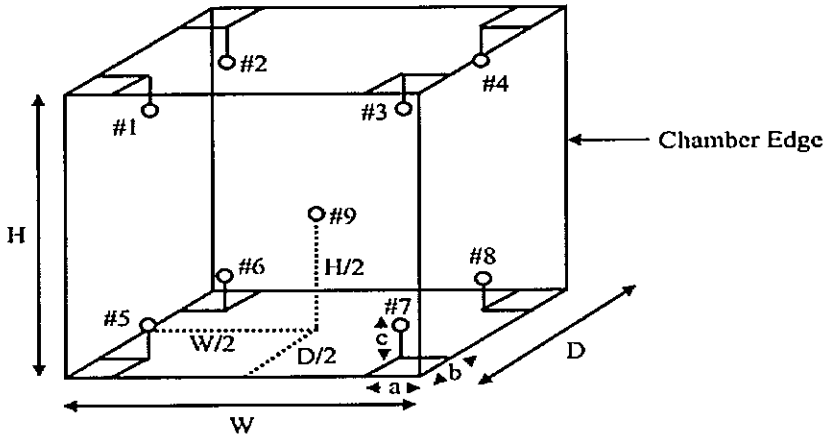

Sensor Installation Details				Dimension of the chamber			
a	=	5.0	cm	W	=	40.0	cm
b	=	5.0	cm	H	=	40.0	cm
c	=	5.0	cm	D	=	33.0	cm

SCaL

Result of Calibration :.

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.48	40.28	40.28	39.91	40.17	40.09	39.93	40.27	39.89	0.36
70	70.36	70.23	70.58	69.74	69.99	69.92	69.86	70.13	70.04	0.36
103	103.19	103.12	103.46	103.37	103.10	103.54	103.43	103.06	103.40	0.36
104	104.31	104.23	104.62	103.77	104.12	104.06	103.90	104.20	104.56	0.36
105	105.07	105.03	105.48	105.27	105.12	105.01	105.01	105.00	104.96	0.36
180	180.31	180.00	180.00	180.07	180.18	180.05	180.01	180.10	180.24	0.41

3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
40	40.0	40.0	0.20	0.70	0.72
70	70.0	70.0	0.20	0.60	0.94
103	103.0	103.0	0.20	0.43	0.54
104	104.0	104.0	0.10	0.79	0.88
105	105.0	105.0	0.10	0.59	0.69
180	180.0	180.0	0.10	0.38	0.38

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

NSC-TISI-TISI7025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 16-Jul-2023

Certificate No. : 23TH3097

CSR No. : A095/04743

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru, Amphoe Hat Yai, Songkhla, 90250
Calibration Place	:	Chemical Laboratory
Instrument Name	:	Water Bath
Manufacturer	:	Memmert
Model	:	WNE29
Serial No.	:	L616.0538
ID No.	:	SGK_CL0035
Resolution	:	0.1 °C
Received Date	:	13-Jul-2023
Calibrated Date	:	13-Jul-2023
Ambient Temperature	:	(30 ± 10) °C
Relative Humidity	:	(50 ± 30) %

REVIEW BY .....

APPROVED BY .....

NEXT CAL. DATE 13/01/25 .....

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980 (reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

SCaL

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisiton/Switch Unit	34970A	MY58009813	23SDAT004	23-May-2024

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :. (✓) Without Adjustment ( ) After Adjustment

1. Sensor Installation Diagram

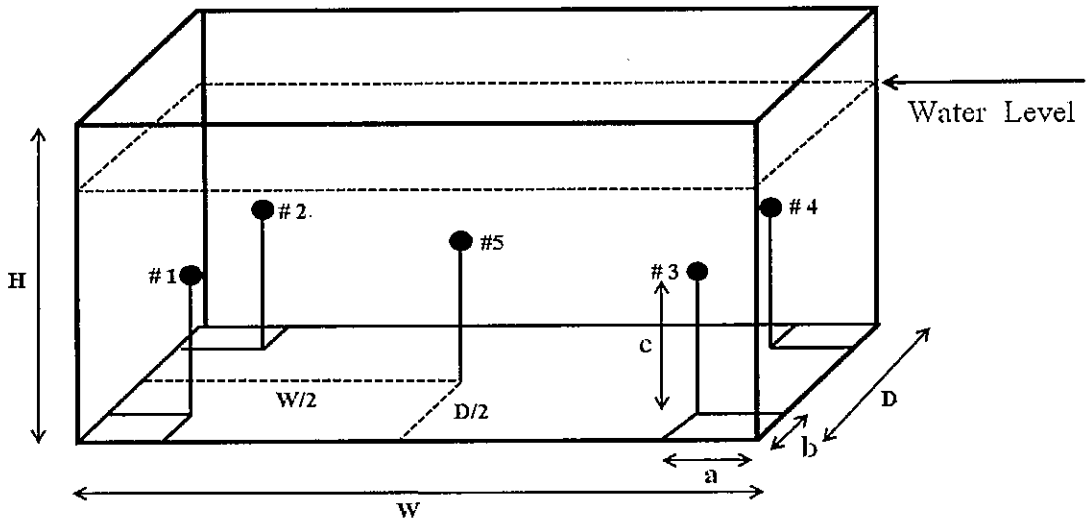

Sensor Installation Details			Dimension of the chamber		
a =	5	cm	W =	45	cm
b =	5	cm	H =	30	cm
c =	5	cm	D =	35	cm

SCaL

Result of Calibration :.

2. Temperature Measurement Accuracy Test

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point	Measured Standard Temperature At Spread Locations (°C)					Uncertainty
(°C)	#1	#2	#3	#4	Ref.5	(±°C)
80	79.17	79.47	79.43	79.25	79.38	0.14

3. Performance Result

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
80	80.0	80.0	0.24	0.38	0.38

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

Southern Calibration Service Co., Ltd.
669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com

NSC-TIST-TIS17025
CALIBRATION 0294

CALIBRATION CERTIFICATE

Issued Date : 3-Feb-2023

Certificate No. : 23TH0527
CSR No. : A073/03634
Page. : 1 of 3

Customer	:	ALS Laboratory Group (Thailand) Co., Ltd 114/1 Moo 8 Karnchanawanich Rd. T.Ban Phru, A. Hat Yai, Songkhla 90250 TH
Calibration Place	:	Chemical Laboratory
Instrument Name	:	Cold Room Water
Manufacturer	:	MODULAR
Model	:	N/A
Serial No.	:	N/A
ID No.	:	SGK_CL0065
Resolution	:	0.1 °C
Received Date	:	31-Jan-2023
Calibrated Date	:	31-Jan-2023
Ambient Temperature	:	(30 ± 10) °C
Relative Humidity	:	(50 ± 30) %

REVIEW BY ...
APPROVED BY .....
NEXT CAL. DATE 31/07/24

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on G-20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

SCaL

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisiton/Switch Unit	34970A	MY58009813	22SDAT004	24-May-2023

2. The resultes reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or mulfunction

Result of Calibration :. (✓) Without Adjustment ( ) After Adjustment

1. Sensor Installation Diagram

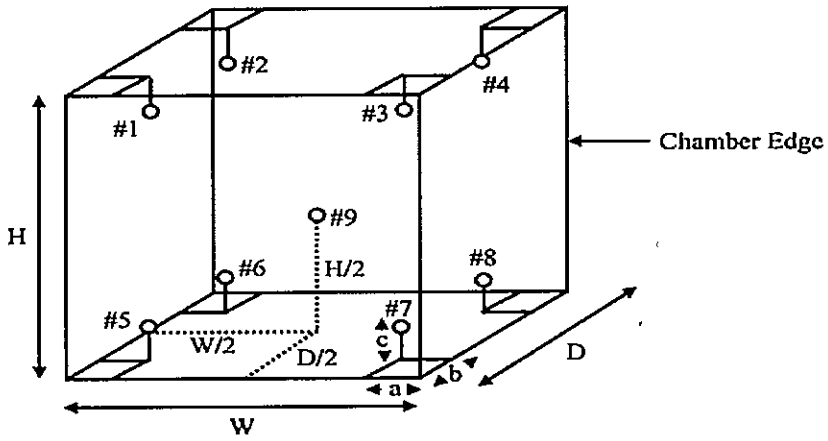

Sensor Installation Details			Dimension of the chamber		
a =	5.0	cm	W =	40.0	cm
b =	5.0	cm	H =	40.0	cm
c =	5.0	cm	D =	33.0	cm

SCaL

Result of Calibration :.

2. Temperature Measurement Accuracy Test

The measurement results of the Cold Room Water and associates are reported in the manner as shown below

Cal point	Measured Standard Temperature At Spread Locations (°C)														
(°C)	#1	#2	#3	#4	#5	#6	#7	#8	# 9	Ref.10	# 11	# 12	# 13	# 14	# 15
4	3.18	3.39	3.54	3.77	3.99	3.86	3.85	3.92	4.02	3.86	3.78	3.84	3.85	4.09	3.91

The uncertainty of measurement was ± 0.38 °C

3. Performance Result

The performance of the Cold Room Water are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
4	4.0	4.0	1.23	0.50	0.84

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

... End ...

HACH COMPANY
C/O AB Sciex (Thailand) Limited, Building D Room No. D3 11, 3rd Floor , No. 735/4, Srinakarin Road, Pattanakarn, Suanluang, Bangkok
|Phone +66 (02) 026-3529 Ext. 0 | Fax +66(02) 026-3572| www.sea.hach.com|

LABX 2300865

Test Report

Customers	:	ALS Laboratory Group (Thailand) Co., Ltd.			
Equipment	:	Chlorine Meter	Manufacturer	:	HACH
Controller Model	:	DR300	Sensor Model	:	-
Controller Serial No.	:	19040A000666	ID Serial No.	:	SGK_FS0048
Date of test	:	16/03/2023	Period	:	1 Year
Environment temperature	:	25.0 °C	Humidity	:	60.0 %RH

Results

Instrument Checked

Item	*Characteristic*	*Before*	*After*	*Remark*
1	Visual Inspect	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
2	Power Supply (4.5 – 6.0 VDC)	6.0 VDC	6.0 VDC	
3	Display Check	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
4	Keyboard Check	☑ Pass ☐ Fail	☑ Pass ☐ Fail	
5	Function System Program	☑ Pass ☐ Fail	☑ Pass ☐ Fail	

Warning and Error Checked

Item	*Event*	*Before*	*After*
6	Error list	☑ None ☐ Appear_____	☑ None ☐ Appear_____

Check with Standard

Item	*Characteristic*	*Before*	*After*	*Remark*
	DPD-CHLORINE-LR			
7	Blank (0.00 mg/l)	0.00 mg/l	0.00 mg/l	
8	Standard Cl2 No. 1 (0.23 ± 0.09 mg/l)	0.25 mg/l	0.24 mg/l	
9	Standard Cl2 No. 2 (0,89 ± 0.10 mg/l)	0.91 mg/l	0.89 mg/l	
10	Standard Cl2 No. 3 (1.64 ± 0.14 mg/l)	1.67 mg/l	1.64 mg/l	
	DPD-CHLORINE-HR			
11	Blank (0.0 mg/l)	0.0 mg/l	0.0 mg/l	
12	Standard Cl2 No. 1 (2.2 ± 0.2 mg/l)	2.2 mg/l	2.2 mg/l	
13	Standard Cl2 No. 2 (4.1 ± 0.3 mg/l)	4.1 mg/l	4.1 mg/l	
14	Standard Cl2 No. 3 (7.0 ± 0.6 mg/l)	7.0 mg/l	7.0 mg/l	

REVIEW BY .....

APPROVED BY .....

NEXT CAL. DATE 16/03/24

HACH
Be Right™

HACH COMPANY
C/O AB Sciex (Thailand) Limited, Building D Room No. D3 11, 3rd Floor , No. 735/4, Srinakarin Road, Pattanakarn, Suanluang, Bangkok
|Phone +66 (02) 026-3529 Ext. 0 | Fax +66(02) 026-3572| www.sea.hach.com|

LABX 2300865

Summary of checked

- ☑ The instrument can work normally and efficiently. (เครื่องมือวัดสามารถทำงานได้ปกติและมีประสิทธิภาพ)
- ☐ The instrument can work but it's requiring to maintenance. (เครื่องมือวัดสามารถทำงานได้แต่ต้องบำรุงรักษา)
- ☐ The instrument could not work it's requiring to repair. (เครื่องมือวัดไม่สามารถทำงานได้และต้องการซ่อมบำรุง)

Remark:

Standard Equipment Used

Equipment	Equipment I.D.			
Standard Chlorine DPD-CHLORINE-LR	Lot No.	A2131	Exp date :	May-24
Standard Chlorine DPD-CHLORINE-HR	Lot No.	A2104	Exp date :	Apr-24
Digital multi meter	S/N :	97270010	Due date :	23-Jun-23
Thermo hygrometer	S/N :	41413945	Due date :	17-Aug-23

Test By : (Miss Wilailak Sawangpun) Service Engineer

Approved by : (Mr. Suanun Sartyangkool) Position : Assistant Service Division Manager

HACH Be Right™

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert.No.: 23CHO30
Page.: 1 of 3

Certificate of Calibration

Equipment :	Spectrophotometer
Manufacturer :	HACH
Model :	DR 3900
Serial No. :	1687645
ID No. :	SGK_CL0038
Condition As-Received:	Used Item
Received Date :	23 January 2023
Calibration Date :	24 January 2023
Reference :	2301-0661OC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 , Kanjanavanij Rd., Banphru , Hatyai , Songkhla 90250 , Thailand
Calibration Place :	Chemistry Room
Ambient Temperature :	(28.3 - 27.3) °C (On-Site)
Relative Humidity :	(49.6 - 49.9) % (On-Site)
Calibration Procedure :	In - house method : CP-OCH4 based on ASTM E 275-01

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 24/01/24

Calibrated by : Kunchit Promprat

Approved by :

Approved Signatory

(✓) Malee Butkruea
( ) Saithip Meangmai
( ) Warakorn Lerngagtrakul

Issue Date : 7 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Condition of calibration result

1. Reference Standard Material :

Material	Serial No.	Certificate No.	Due date
1. Absorbance Standard set	32593	100581	30 Mar 2024
2. Wavelength Standard set	29829	94776	02 Sep 2023
3. Wavelength Standard set	29829	94777	02 Sep 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certificate is traceable to the International System of Unit maintained at :
   - National Physical Laboratory (NPL), The United Kingdom of Great Britain and Northern Ireland
   - National Institute of Standards and Technology (NIST), The United States of America
4. Spectral BandWidth : 5 nm
   Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (± nm)	Coverage Factor *k*
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	514	0.59	2.00
537.00	536	0.59	2.00
638.00	638	0.59	2.00
684.70	685	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (±Abs)	Coverage Factor *k*
420.0	Zero	0.000	0.0028	2.00
	0.5701	0.568	0.0029	2.00
	0.7147	0.712	0.0030	2.00
	1.0031	0.999	0.0030	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5552	0.553	0.0029	2.00
	0.7031	0.700	0.0030	2.00
	0.9867	0.981	0.0029	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5178	0.517	0.0030	2.00
	0.6642	0.663	0.0029	2.00
	0.9312	0.930	0.0030	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5195	0.517	0.0030	2.00
	0.7007	0.698	0.0029	2.00
	0.9833	0.979	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5537	0.550	0.0030	2.00
	0.7763	0.771	0.0029	2.00
	1.0912	1.083	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5615	0.558	0.0029	2.00
	0.7659	0.762	0.0030	2.00
	1.0763	1.070	0.0028	2.00

Remark

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

บริษัท ดับเบิ้ล เอส ไดแอคนอสติคส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.
4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพฯ 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รอบ							12/7 CL					

Periodical maintenace check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	☐	☑	
2.ISE tubing change	☒	☒	none
3.Syringe check/change		☑	
4.Dispensing check/ change		☑	
5.Waste tubing change when necessary		☑	
6.Lamp check/change	☐	☑	
7.Mixer paddle/paddle change(not Konelab20)		☑	
8.ISE needles check/change		☒	none
9.Pump tubing check/ chance	☐	☑	
10.Broken/worn out part check /change		☑	
11.Peristaltic pump check /cleaning/ lubrication	☐	☑	
12.Heating check		☑	
13.Cooling check		☑	
14.Dispenser mechanic check/adjustment	☐	☑	
15.Cuvette transfer mechanic check/adjustment	☐	☑	
16.Dispenser movement check/adjustment	☐	☑	
17.Sample/reagent register check/adjustment	☐	☑	
18.Dispensing tubing tightness check	☐	☑	
19.Photometer and optics cleaning/check/adjustment	☐	☑	
20.Workstation PC cleaning if necessary	☐	☑	
21.Mechanic cleaning/lubrication	☐	☑	
22.Instrument cleaning if necessary	☐	☑	
23.Complete analyzer testing with waterblank/QC or sample	☐	☑	
24.Test parameters/Adjustment/config. Save to USB key	☐	☑	
25.UPS Test	☐	☑	

Place: ALS LAB **Instrument:** k90 Aqualeem

Date/Time: 12/7/66 **Serial no:** 22781

Service done by: ..... **Install date:** .....

Signature of customer: ..... **Date/Time:** 12/7/66

Laboratory
Analyzer User

7/12/2023 21:21

Performed	7/12/2023	
Lot	W166	

ACCEPTANCE CRITERIA

	Result	Limit	Warning
Temperature (?C)	37.7	37.0 +/- 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	1.17	<1.7	
Photometric noise			
Max SD L340_2 (mA)	0.19	<2.0	
Max SD L340_4 (mA)	1.06	<3.0	
Linearity of photometer			
Slope	1.0188	0.94 - 1.06	
Curvature	0.0035	+/- 0.02	
Max bias from linear fit (mA)	3.2	<15.0	
Max delta %	-2.0	+/- 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (?l)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (?l)	4.13	3.85 - 4.40	
XDISP2 CV%	0.58	<2.0	
XDISP4 CV%	0.70	<2.0	
XDISP10 CV%	0.59	<2.0	
Needle 0 ?l volume			
Average (A)	0.009	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (?l)	0.06	<0.32	

OTHER INFORMATION

Dispensing ratio

Posit	Result (A)
1	0.1592
2	0.1624
3	0.1631
4	0.1631
5	0.1625
6	0.1650

Photom. noise: SD (mA)

Posit	L340_2	L340_4
1	0.07	0.64
2	0.09	1.06
3	0.14	0.50
4	0.13	0.53
5	0.19	0.38
6	0.02	0.64

Laboratory
Analyzer User

7/12/2023 21:21

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.311
XDISP4	0.616
XDISP10	1.478

Linearity of photometer

L340_	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.001	0.005	-0.004	-394.7
2	0.512	0.519	-0.007	-1.5
3	1.523	1.550	-0.027	-1.8
4	2.027	2.066	-0.039	-1.9
5	2.532	2.582	-0.050	-2.0

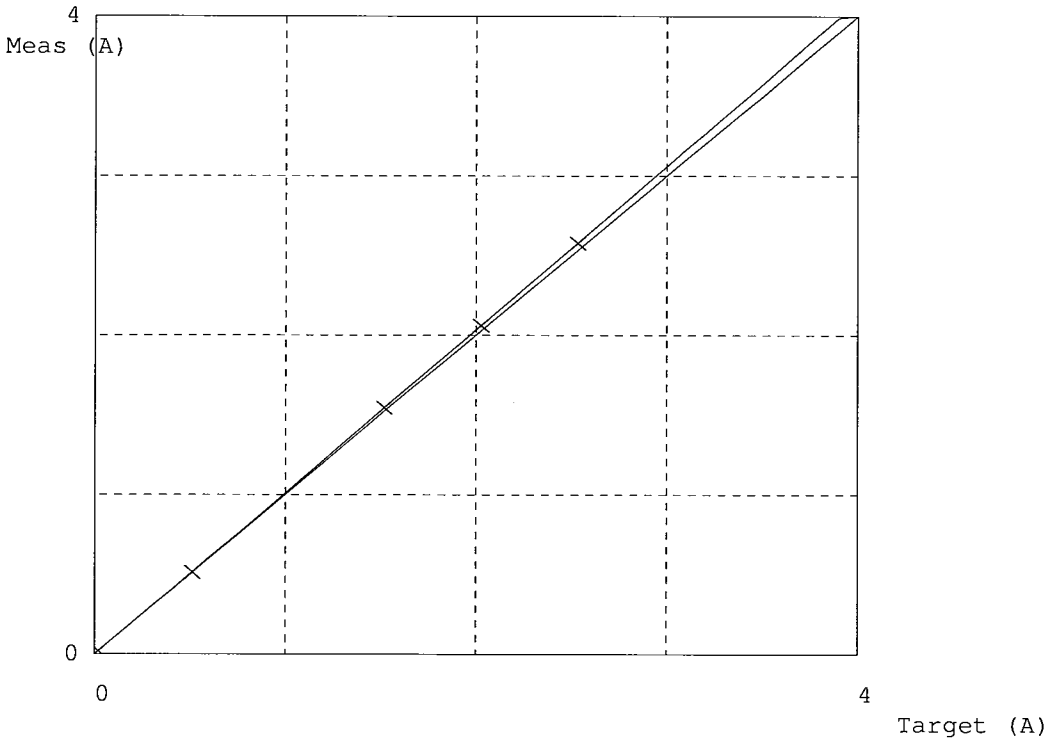

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate of Calibration

Equipment	:	**Digestion Unit**
Manufacturer	:	**SCP Science**
Model	:	**DigiPRER HT**
Serial No.	:	**HTC1120480658**
Customer Code	:	**BKK_EN0366**
ID No.	:	**T2635A5**
Customer	:	**ALS Laboratory Group (Thailand) Co.,Ltd.**
		104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
		Khet Suan Luang, Bangkok 10250
Customer Location	:	**Wet Chemistry Lab 1**
Date of Receipt	:	**10 May 2023**
Calibrated By	:	**Sujjar Naknakred (Site Calibration Manager)**
Approved By	:	_____ **/ Boonchai Suriyawong (Site Calibration Manager)**
Date of Issue	:	29 MAY 2023

REVIEW BY ..

APPROVED BY .....

NEXT CAL. DATE 17/05/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

Equipment : **Digestion Unit**
Date of Calibration : **17 May 2023**
Environment : **Temperature : 23.9 - 26.3 °C**
Line Voltage : 221.8 - 225.9 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.
2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A1-(CH17-CH20)	T230547	18 April 2024
DATA LOGGER	34970A	T149	T230547	18 April 2024

3. This certificate is traceable to :
   National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)
4. Condition of calibrated item : good
   Equipment Description :
   Time Constant 1 Hour 54 Minute At 380 °C
   Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
   ☐ Close
   ☒ Not Available
5. Adjustment :
   (X) without adjustment ( ) after adjustment

Approved By_____

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Calibration Report

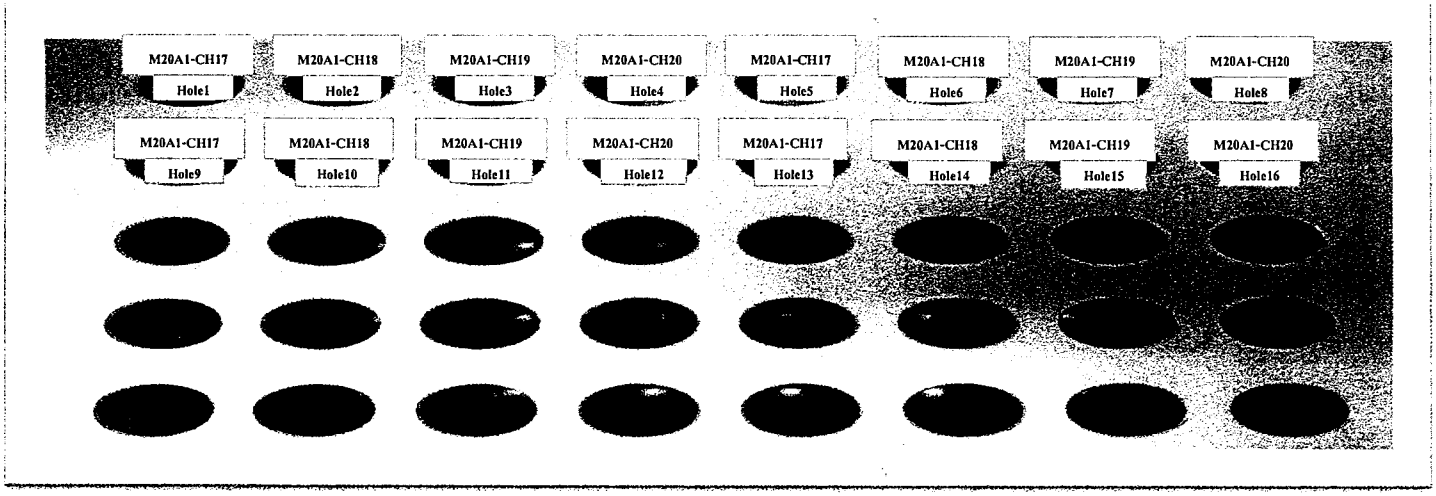

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
				Hole1	Hole2	Hole3	Hole4	Hole5	Hole6	Hole7	Hole8
(°C)	(°C)	(°C)	Reading	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.3	379.0	379.2	380.2	377.5	379.5	380.7	380.1
			Min °C	376.8	378.6	378.9	379.9	377.0	379.0	380.2	379.6
			Average °C	**377.0**	**378.8**	**379.1**	**380.0**	**377.3**	**379.2**	**380.4**	**379.9**
			Stability ± °C	0.2	0.2	0.2	0.2	0.3	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
				Hole9	Hole10	Hole11	Hole12	Hole13	Hole14	Hole15	Hole16
(°C)	(°C)	(°C)	Reading	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.1	378.9	379.7	379.9	379.3	379.6	379.5	377.4
			Min °C	376.7	378.5	379.3	379.5	378.9	379.1	379.0	377.0
			Average °C	**376.9**	**378.7**	**379.5**	**379.7**	**379.1**	**379.4**	**379.3**	**377.2**
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.3	0.3	0.2

Approved By._____

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Calibration Report

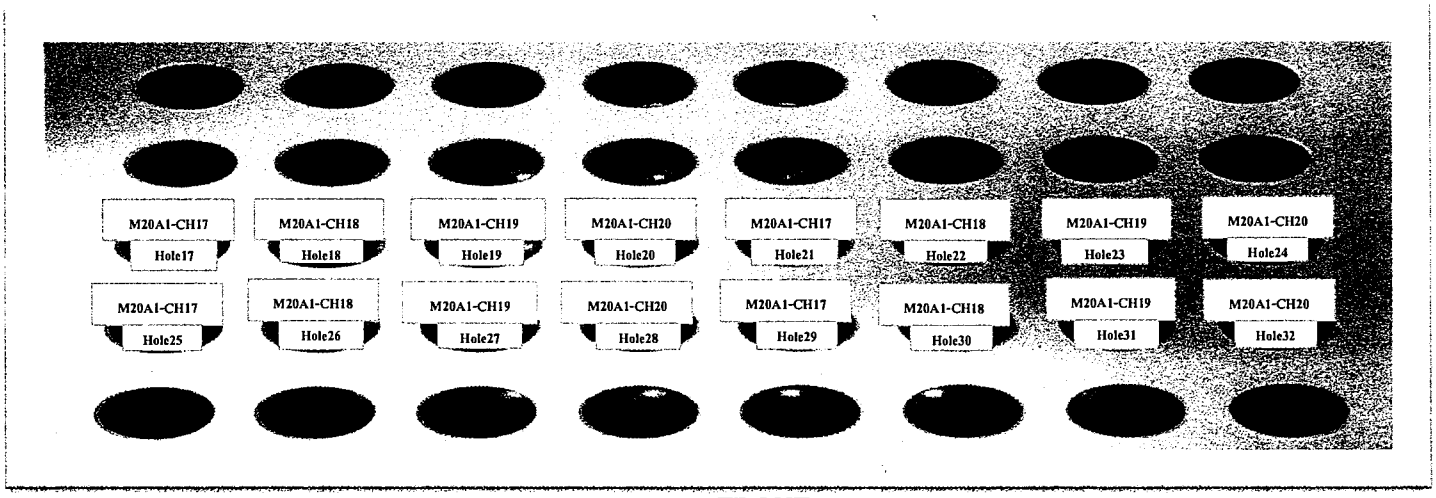

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
(^{o}C)	(^{o}C)	(^{o}C)	Reading	Hole17	Hole18	Hole19	Hole20	Hole21	Hole22	Hole23	Hole24
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max ^{o}C	378.4	380.1	380.1	380.0	379.1	379.8	379.6	377.8
			Min ^{o}C	377.8	379.6	379.7	379.3	378.6	379.2	379.2	377.3
			Average ^{o}C	**378.1**	**379.9**	**379.9**	**379.7**	**378.9**	**379.5**	**379.4**	**377.5**
			Stability $\pm$ ^{o}C	0.3	0.3	0.2	0.3	0.3	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
(^{o}C)	(^{o}C)	(^{o}C)	Reading	Hole25	Hole26	Hole27	Hole28	Hole29	Hole30	Hole31	Hole32
				M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max ^{o}C	377.9	379.4	380.1	380.1	379.3	379.6	378.9	377.3
			Min ^{o}C	377.4	378.9	379.7	379.7	378.8	378.9	378.4	376.7
			Average ^{o}C	**377.7**	**379.2**	**379.9**	**379.9**	**379.0**	**379.3**	**378.6**	**377.0**
			Stability $\pm$ ^{o}C	0.3	0.3	0.2	0.2	0.3	0.4	0.3	0.3

Approved By._____

Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T230902

Calibration Report

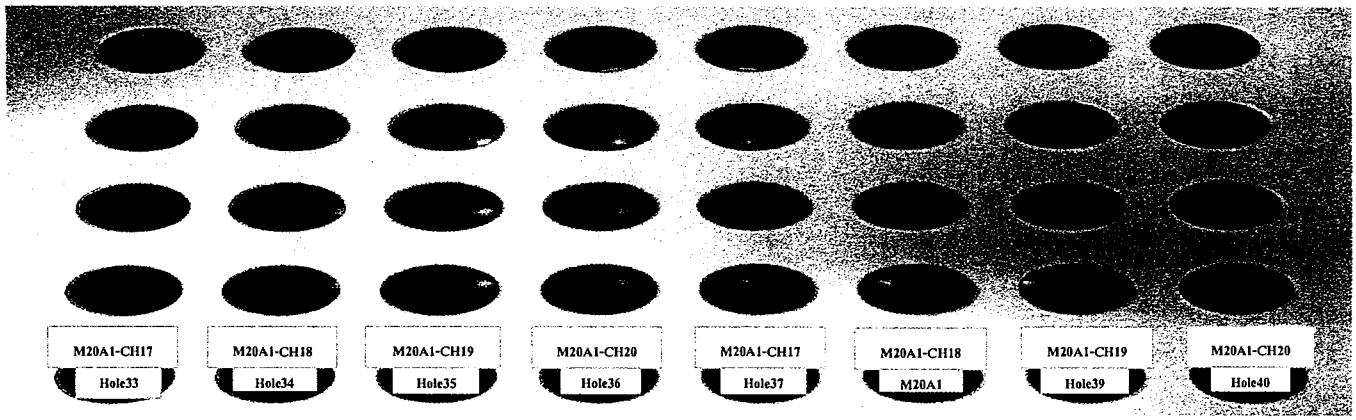

FRONT

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Stardards at Block							
				Hole33	Hole34	Hole35	Hole36	Hole37	Hole38	Hole39	Hole40
(°C)	(°C)	(°C)	Reading	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20	M20A1-CH17	M20A1-CH18	M20A1-CH19	M20A1-CH20
380.0	380.0	379.4 - 380.7	Max °C	377.7	378.0	378.3	379.0	378.2	378.5	377.3	377.4
			Min °C	377.3	377.6	377.9	378.6	377.7	378.1	376.9	377.0
			Average °C	**377.5**	**377.8**	**378.1**	**378.8**	**378.0**	**378.3**	**377.1**	**377.2**
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.2	0.2	0.2

The expanded uncertainty of temperature measurement was ± 1.85 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2 , providing a level of confidence of approximately 95 % .

Approved By._____

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM1103
Page : 1 of 3

Certificate of Calibration

Equipment :	Autoclave
Manufacturer :	Sanyo
Model :	MLS-3781
Serial No. :	830167
ID No. :	BKK_ML0037
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Media Preparation Room
Received Order :	17 July 2023
Calibration Date :	17 July 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Preecha Hlahib

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 17/07/25

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul
( ) Malee Butkruea
(✓) Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0053615

Equipment : Autoclave **Cert. No.:** 23TM1103

Condition As-Received : Used Item

Reference : 2307-0285OC-3

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.
4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)

It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directry concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

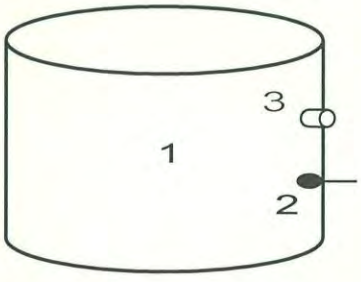

	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	22	53	220
Finished of Calibration	22	54	220

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	22-17TC-01
2 =	Temperature sensor	23-17TC-02
3 =	Exhaust port	19-17TC-03

Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2307-0285OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM1103

Operating parameter Set : Temperature = 121 °C
Sterilization period = 15 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor *k*
121	121	1	120.877	0.39	0.12	1.0	2
		2	120.870				
		3	120.866				

Average* : The average of 30 values in each position.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM1146
Page : 1 of 3

Certificate of Calibration

Equipment :	Incubator
Manufacturer :	SHEL-LAB
Model :	1915A
Serial No. :	0200599
ID No. :	BKK_ML0010
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthakan Rd., Khwawng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Incubation & Micrological Reading
Received Order :	17 July 2023
Calibration Date :	17 July 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Man Pattanapongpaiboon

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 17/01/25

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056489

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1

Cert. No.: 23TM1146

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	56
AC Supply (Volt)	221	223

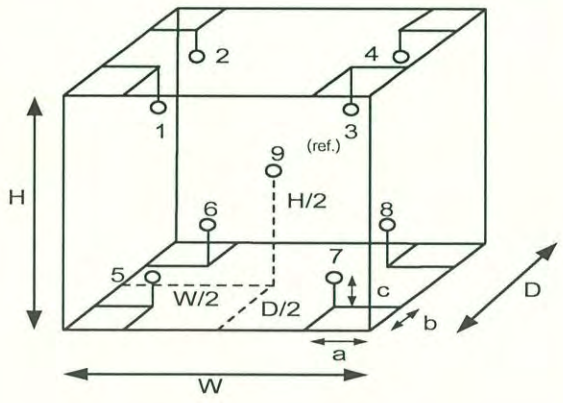

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.50	m
W =	0.75	m
H =	1.2	m
Capacity =	0.45	m^3

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 23TM1146

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
35.0	35.0	35.0	0.055	0.30	0.44	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.888	34.933	34.815	34.813	35.064	35.019	35.156	35.141	35.087	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment :	Water Bath
Manufacturer :	Memmert
Model :	WB 45
Serial No. :	L799.0009
ID No. :	BKK_ML0049
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Biochemical Lab
Received Order :	19 January 2023
Calibration Date :	19 January 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Khit Ruttanaprapachai

REVIEW BY ....
APPROVED BY
NEXT CAL. DATE 19/01/24

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 2 February 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2301-0577OC-1

Cert. No.: 23TM104

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	23	53	221
Finished of Calibration	24	57	222

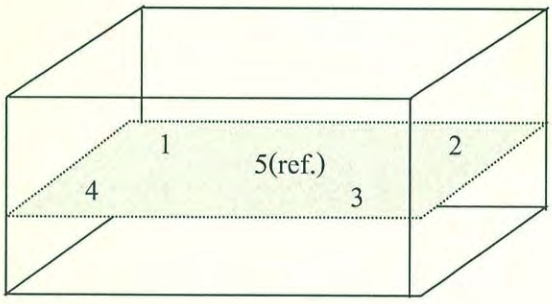

Front

Position :	Ref. Std. ID No.:
1	70RC143
2	70RC144
3	70RC145
4	70RC146
5(ref.)	70RC147

Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2301-0577OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM104

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C) Position				
			1	2	3	4	5 (ref.)
42.0	44.9	44.9	41.996	42.005	41.974	42.021	42.036

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor *k*
42.0	0.11	0.037	0.15	2

Average* : The average of 30 values in each position.
Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Stability : One-half of the greatest maximum difference of measured temperature at any one probe.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 22TM1571
Page : 1 of 3

Certificate of Calibration

Equipment :	Hot Air Oven
Manufacturer :	Binder
Model :	ED 240/E2
Serial No. :	00-15533
ID No. :	BKK_ML0013
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Media Preparatiom Room
Received Order :	21 November 2022
Calibration Date :	21 November 2022
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Krisda Malee

REVIEW BY ...
APPROVED BY
NEXT CAL. DATE 21/05/24

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul
(✓) Malee Butkruea
( ) Suwit Imjai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0048150

Equipment : Hot Air Oven

Condition As-Received : Used Item

Reference : 2211-0623OC-1

Cert. No.: 22TM1571

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) After Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. (°C)	26	26
REL.Humid. (%)	53	55
AC Supply (Volt)	219	220

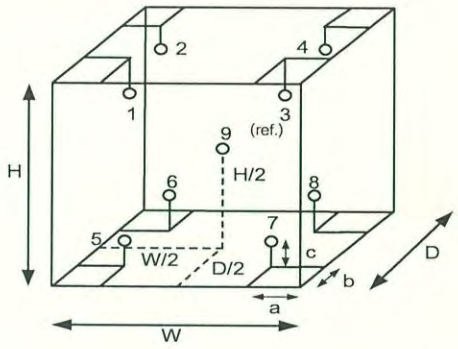

Probe Installation Details :

a =	5.0	cm
b =	5.0	cm
c =	5.0	cm

Dimension of Chamber :

D =	0.50	m
W =	0.80	m
H =	0.60	m
Capacity =	0.24	m^3

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2211-0623OC-1
Result of Calibration :- (*) After Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 22TM1571

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (±°C)	Coverage Factor *k*
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point (°C)	Measured Temperature (°C) Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 , e-mail: service.thailand@sartorius.com

NSC-TISI-TIS 17025
CALIBRATION 0426

SARTORIUS

REVIEW BY ...
APPROVED BY
NEXT CAL. DATE 8/2/24

Certificate of Calibration

Model Number :	CP3202S	Certificate No. :	23BCI0073
Description :	Precision Balance	Issued Date :	Monday, February 13, 2023
Serial Number :	16704832	Reference No. :	203245
ID No.	BKK_ML0001		
Manufacturer :	Sartorius	Page No. :	1 0f 2

Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.

Calibrated Place : Balance Room.

Calibrated By : Mr.Chonchai Inthana
Calibration Date : Wednesday, February 08, 2023

Calibration Procedure No. : This calibration was conducted by
Using in-house calibration procedure number (WI-003)
Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 3,200 g Readability : 0.01 g

Ambients Conditions:

Temperature :	23.5 °C	±	3.0 °C
Humidity :	56.0 % RH	±	5.0 % RH
Pressure		±	_

Reasons for calibration

☐ New Installation ☐ Service / Repaired ☑ Re-calibration/ Maintenance

Equipment Condition: ☑ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Cetificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Mr.Chonchai Inthana(Technical Manager)

STAMP

SARTORIUS (THAILAND) CO., LTD. SARTORIUS ISO/IEC 17025:2017

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

SARTORIUS

Certificate of Calibration

Model Number :	CP3202S	Certificate No. :	23BCI0073
Description :	Precision Balance	Issued Date :	Monday, February 13, 2023
Serial Number :	16704832	Reference No. :	203245
ID No. :	BKK_ML0001		
Manufacturer :	Sartorius	Page No. :	2 of 2

Calibration Results : Without Adjustment

Repeatability

The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	200.00	1999.99
200 g	200.00	2000.00
Tolerance	200.00	1999.99
0.01 g	199.99	2000.00
	200.00	2000.00
Nominal Value : (High Load)	200.00	1999.99
2000 g	200.00	1999.99
Tolerance	199.99	2000.00
0.01 g	200.00	2000.00
	200.00	2000.00
Standard Deviation	0.004	0.005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximim capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 1000 g
Tolerance *0.06* g





	Difference
1	–
2	0.00
3	0.00
4	0.00
5	0.00
6	-

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance *0.02* g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
1	1.00	1.00	0.00	0.013
5	5.00	5.00	0.00	0.013
10	10.00	10.00	0.00	0.013
20	20.00	20.00	0.00	0.013
50	50.00	50.00	0.00	0.013
100	100.00	100.00	0.00	0.013
500	500.00	500.00	0.00	0.013
1000	1000.00	1000.00	0.00	0.014
2000	2000.00	2000.00	0.00	0.014
3000	3000.00	3000.00	0.00	0.014

End of Report.

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Certificate of Calibration

Equipment :	Autoclave
Manufacturer :	TOMY
Model :	SX-700
Serial No. :	48134190
ID No. :	BKK_ML0041
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Location :	Media Preparation Room
Received Order :	03 October 2023
Calibration Date :	04 October 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Khit Ruttanaprapachai

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 04/04/25 ~~03/10/24~~

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul
(✓) Ponpan Paipim
( ) Suwit Imjai

Issue Date : 11 October 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Autoclave **Cert. No.:** 23TM1408

Condition As-Received : Used Item

Reference : 2310-0006OC-6

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.
4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)

It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directry concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

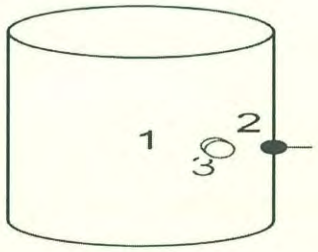

	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	26	64	221
Finished of Calibration	27	67	222

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	19-17TC-08
2 =	Temperature sensor	19-17TC-09
3 =	Exhaust port	19-17TC-10

Equipment : Autoclave

Condition As-Received : Used Item

Reference : 2310-0006OC-6

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Cert. No.: 23TM1408

Operating parameter Set : Temperature = 108 °C

Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor *k*
108	108	1	108.352	0.12	0.04	0.90	2
		2	108.263				
		3	108.140				

Operating parameter Set : Temperature = 115 °C

Sterilization period = 20 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor *k*
115	115	1	115.376	0.13	0.08	0.90	2
		2	115.297				
		3	115.157				

Operating parameter Set : Temperature = 118 °C

Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor *k*
118	118	1	118.083	0.11	0.09	0.90	2
		2	118.037				
		3	117.954				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

Equipment : Autoclave

Condition As-Received : Used Item

Reference : 2310-0006OC-6

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Cert. No.: 23TM1408

Operating parameter Set : Temperature = 121 °C

Sterilization period = 30 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor *k*
121	121	1	121.186	0.17	0.11	0.91	2
		2	121.082				
		3	120.980				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was excluded stability.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484

NSC-TISI-TIS17025
CALIBRATION 0008

Cert. No.: 23TM1366

Certificate of Calibration

Equipment :	Incubator
Manufacturer :	Memmert
Model :	ICP 750
Serial No. :	F816.0004
ID No. :	BKK_ML0189
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang , Bangkok 10250 Thailand
Location :	Incubation & Microbiological Reading
Received Order :	03 October 2023
Calibration Date :	03 October 2023
Ambient Temperature :	(26 ± 10) °C
Relative Humidity :	(50 ± 30) %
Calibrated by :	Man Pattanapongpaiboon

REVIEW BY .....
APPROVED BY .....
NEXT CAL. DATE 03/10/24

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul
(✓) Ponpan Paipim
( ) Suwit Imjai

Issue Date : 11 October 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2310-0006OC-3

Cert. No.: 23TM1366

Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	56
AC Supply (Volt)	222	224

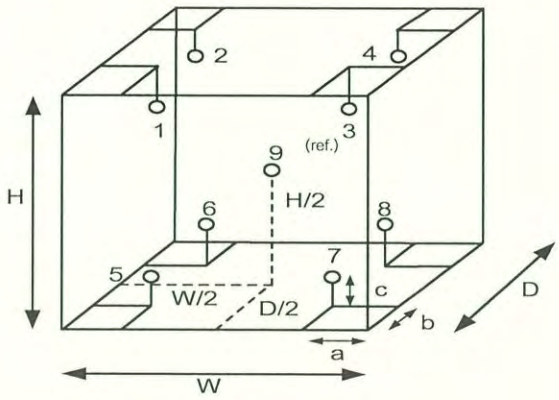

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	19-16RTD-04
5	19-16RTD-05
6	19-16RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09

Probe Installation Details :

a =	10	cm
b =	10	cm
c =	10	cm

Dimension of Chamber :

D =	0.50	m
W =	1.1	m
H =	0.80	m
Capacity =	0.44	m^3

Equipment : Incubator
Condition As-Received : Used Item
Reference : 2310-0006OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 23TM1366

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor *k*
37.0	37.0	37.0	0.026	0.13	0.18	2

Calibration Point (°C)	Measured Temperature (°C) Position									Uncertainty (±°C)
	1	2	3	4	5	6	7	8	9 (ref.)	
37.0	36.994	36.907	37.045	37.002	37.007	37.002	37.008	36.995	36.923	0.30

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor ***k***, providing a level of confidence of approximately 95 %.

-o0o-

ภาคผนวก ฉ

สำเนาหนังสือใบอนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

ที่ อก ๐๓๑๐(๑)/ ๓๐๖๙

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ เขตราชเทวี
กรุงเทพมหานคร ๑๐๔๐๐

๒๘ มกราคม ๒๕๖๕

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๓๐ กรกฎาคม ๒๕๖๓

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ แผ่น
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกขน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๖๒ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๕๙ รายการ น้ำใต้ดิน จำนวน ๑๒๖ รายการ อากาศเสีย ๑๖ รายการ สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน ๓๕ รายการ และดิน จำนวน ๑๒๕ รายการ รวมทั้งสิ้นจำนวน ๓๖๑ รายการ ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ กันยายน ๒๕๖๖ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๒๐๒ ๔๑๔๖ ๐ ๒๒๐๒ ๔๐๐๒
โทรสาร ๐ ๒๓๕๔ ๓๒๐๘ ๐ ๒๓๕๔ ๓๔๑๕

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔

ที่ อก ๐๓๑๐(๑)/ ลงวันที่ ๒๘ มกราคม ๒๕๖๕

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๖ ราย

๑) นางสาวยุพาพร จันทร์เปล่ง	ทะเบียนเลขที่ ว-๒๐๔-ค-๔๗๐๐
๒) นางสาวชัชนัย โกมารกุล ณ นคร	ทะเบียนเลขที่ ว-๒๐๔-ค-๔๗๐๑
๓) นายศรายุทธ จิตรานนท์	ทะเบียนเลขที่ ว-๒๐๔-ค-๔๗๐๒
๔) นางสาวกนกกร เอนก	ทะเบียนเลขที่ ว-๒๐๔-ค-๖๑๑๑
๕) นายสุริยา สอนแก้ว	ทะเบียนเลขที่ ว-๒๐๔-ค-๖๑๑๒
๖) นายวิชาญ ชุณหรัต	ทะเบียนเลขที่ ว-๒๐๔-ค-๖๑๑๓

(นายศิระ จันทร์เฉิด)

นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๓๐๖๙ ลงวันที่ ๒๘ มกราคม ๒๕๖๕

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๖๒ ราย

๑) นางสาวจินดา โขจุลธรรม ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๐๘
๒) นางสาวสาวิตรี น้อยเสงี่ยม ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๐๙
๓) นางสาวชณัฐกาญจน์ อิ่มชม ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๐
๔) นางสาวนรินทร์ สายเส็ง ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๕
๕) นางสาวนันทวดี สมบูรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๖
๖) นางสาวศรัณยา เฉลิมธำรงค์ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๗
๗) นางสาวสรารัศมิ์ มงคลจิรวุฒิ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๙
๘) นางสาวศิริลักษณ์ พึ่งแพง ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๒๐
๙) นายนพพงศ์ จันทรุพันธุ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๐๘
๑๐) นายนรเศรษฐ์ โกมาลย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๑
๑๑) นายธันวา จริยา ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๔
๑๒) นางสาวเกศรินทร์ แก้วมั่น ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๖
๑๓) นางสาวสุวิมล ชัยเรืองวุฒิ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๑๗
๑๔) นางสาวสุชาดา ธรรมถาวร ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๑
๑๕) นางสาวเปมิกา ขัยเดชธนกุล ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๓
๑๖) นางสาวศศิธร หมูสวัสดิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๔
๑๗) นางสาวเสาวลักษณ์ ภู่นภาอำพร ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๕
๑๘) นายอภิสิทธิ์ สิงหา ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๖
๑๙) นายศักดิ์สิทธิ์ ไพศาลพิสุทธิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๗
๒๐) ว่าที่ร้อยตรีหญิง พรรณิภา ขำเจริญ ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๒๘
๒๑) นางจิลตา คำภูแก้ว ทะเบียนเลขที่ ว-๒๐๔-จ-๕๔๓๑
๒๒) นางสาวอรวรรณ รักยง ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๑๕
๒๓) นางสาวนพรัตน์ แย้มกรานต์ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๑๙
๒๔) นายจุลเดช วารินทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๐
๒๕) นางสาวดายุรัตน์ ร้องคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๑
๒๖) นายนคร สุขเจริญ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๒
๒๗) นายบัญชา นามเขตต์ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๓
๒๘) นายพรมมี ศรีปัตเนตร ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๕
๒๙) นายอุทิศ อุ่นสิม ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๖
๓๐) ว่าที่ร้อยตรี เฉลิมเกียรติ อมรศรีเสริม ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๘
๓๑) นางสาววริยา สร้างนา ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๙
๓๒) นายอนุพงศ์ รัตนศรีประเสริฐ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๓๐
๓๓) นางสาวจุฑารัตน์ โอนสันเทียะ ทะเบียนเลขที่ ว-๒๐๔-จ-๖๒๔๒
๓๔) นางสาวจารุวรรณ พิมพ์อภิกเดียา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๗๖

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

๓๕) นางสาวปรางค์ทิพย์...

๓๕) นางสาวปรางค์ทิพย์ กิจไพศาลศักดิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๗๙
๓๖) นางสาวเตือนใจ ทางกลาง ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๐
๓๗) นางสาวจิราพร ศิริเวช ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๒
๓๘) นายวรากร ผูกรักษ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๓
๓๙) นายทนง วิริยะสหกิจ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๔
๔๐) นายธนิต เจนจบ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๕
๔๑) นายคณิศร ขำเพชร ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๖
๔๒) นายอรรคพล นิยมวิทยาพัน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๗
๔๓) นายภูวิช พรหมสะอาด ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๘
๔๔) นายธนเดช โภคาพิพัฒน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๙
๔๕) นายชวฤทธิ์ วงษ์จันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๐
๔๖) นายอาทิตย์ ศรีเสน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๑
๔๗) นายเจษดินทร์ คงศักดิไทย ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๒
๔๘) นายจรัส บุญยิ่ง ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๕
๔๙) นายธนาณัติ เอนก ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๖
๕๐) นายอภิวัฒน์ ทุมหนู ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๗
๕๑) นางสาวสุภาขวัญ มาก ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๙๘
๕๒) นางสาวทัตพร ขวาลสมบูรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๐
๕๓) นางสาวธิติมา บุญเพ็ง ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๑
๕๔) นางสาวกนกอร เข็มเพ็ชร ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๒
๕๕) นางสาวพัชรียา หงษ์สมดี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๓
๕๖) นางสาวภานิดา สุรวงศ์ตระกูล ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๔
๕๗) นางสาวภานุมาศ นามวัฒน์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๕
๕๘) นางสาวอุไรรัตน์ ทีงสร้างแป้น ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๖
๕๙) นายธีรวัฒน์ ปวงสุข ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๗
๖๐) นายอิทธิพล ยะโส ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๘
๖๑) นายประพจน์ วรรณชูชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๙
๖๒) นายขยธร พวงทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๐
๖๓) นางสาวกนกวรรณ จันทบาล ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๑
๖๔) นางสาวเกษร หลักบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๒
๖๕) นายสิทธิโชค ธงเงิน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๑๓
๖๖) นางศิลาวรรณ ใจบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๕
๖๗) นางสาวพรรณธิดา พุ่มคง ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๘
๖๘) นางสาวศรวณีย์ ยิ่งดี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๙
๖๙) นายนวภัทร ศรีวิริยะ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๐
๗๐) นายสุวิชา ทองอ่อน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๑
๗๑) นายวิญญู บุญตะนัย ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๓

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

๗๒) นายสมบูรณ์...

๗๒) นายสมบูรณ์ บุตรจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๔
๗๓) นายวิรัตน์ ไชยนะรา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๕
๗๔) นายนฤเบศน์ เพิ่มพูน ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๖
๗๕) นายจิรณัฐ ขาวละออ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๗
๗๖) นายสมโภช วันสา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๙
๗๗) นายอัสรี นามบุรี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๑๗
๗๘) นายณัฐนันท์ ปานประเสริฐ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๑๙
๗๙) นายอัศวเรศ จ่อสาว ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๐
๘๐) นายประเสริฐ สุระขันธ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๑
๘๑) นายนุกูล จันทร์เนียม ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๒
๘๒) นายพีรพงษ์ ทองคูณปรีดา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๓
๘๓) นายนฤพล ทองนุช ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๔
๘๔) นายอนุวัฒน์ ม่วงแพร ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๕
๘๕) นายเจตศราวุฒิ ปัตตะมะ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๖
๘๖) นายกฤษณะ สายวรรณ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๗
๘๗) นายพิชัย บุญยงค์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๘
๘๘) นายภานุพงศ์ โฮมวงศ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๒๙
๘๙) นายสามารถ คุ้มปลี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๐
๙๐) นายสัญชัย โกศรีนาม ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๑
๙๑) นายณัฐวุฒิ ศรีประเสริฐ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๒
๙๒) นายขวัลธัช นาคพนม ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๓
๙๓) นายพงศธร ชัยทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๕
๙๔) ว่าที่ร้อยตรี ภาณุพงศ์ แสนศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๖
๙๕) นายสิทธิโชค ทาสีดา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๗
๙๖) นายธนากร อินสุตา ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๘
๙๗) นางสาววรณิชชา ชาติวันชัย ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๙
๙๘) นางสาวพิมพ์ตะวัน มินากูล ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๔๑
๙๙) นางสาวเพชรัตน์ สิงห์สมบุญ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๔๒
๑๐๐) นางสาวชญานิน พรหมจันทร์ ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๔๓
๑๐๑) นายกีรติ ทวีราช ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๘๖
๑๐๒) นายจักริน หมั่นวิชา ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๘๗
๑๐๓) นายฉัตรชัย สุขเปีย ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๘๘
๑๐๔) นายณรนนท์ ต๊ะทองคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๘๙
๑๐๕) นายดุลยพล สนนอก ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๐
๑๐๖) นายทักษ์ดนัย อุบลศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๑
๑๐๗) นายธนศวร นามะกุณณา ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๒
๑๐๘) นายธิติพงศ์ บัวแดง ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๓

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

๑๐๙) นายนนทชัย...

๑๐๙) นายนนทชัย อุปถัมภ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๔
๑๑๐) นายนัฐพล คุณสุทธิ์ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๕
๑๑๑) นายนันทวัฒน์ สาริน ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๖
๑๑๒) นายปิยะนัฐ พลมะศรี ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๗
๑๑๓) นายพงศ์สิริ โสมเขียว ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๘
๑๑๔) นายพีรพัฒน์ กำคำ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๕๙๙
๑๑๕) นายภาณุพงศ์ มานิตย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๐
๑๑๖) นายมงคล ผลาทิพย์ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๑
๑๑๗) นายมุนินทร์ พูลศิริ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๒
๑๑๘) นายสิรินนท์ ทองอั้น ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๓
๑๑๙) นายอเนขา ทันสมัย ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๔
๑๒๐) นายอดิศักดิ์ ผมไผ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๕
๑๒๑) นายอนันตชัย วีสม ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๖
๑๒๒) นายณัฐดนัย เจือละออง ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๗
๑๒๓) นายวรวุธ ดีนัก ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๘
๑๒๔) นายแสงตะวัน นะตะสัต ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๙
๑๒๕) นายยุทธพงศ์ รัตนะ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๐
๑๒๖) นายชยัณวุฒิ ไชยฮะนิจ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๑
๑๒๗) นายวิศรุต ศรีธรรมมา ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๒
๑๒๘) นายนนทกร เผือกผ่อง ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๓
๑๒๙) นายกำชัย สุทธะ ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๑๔
๑๓๐) นางสาวณัฐภรณ์ รักทะเล ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๑๙
๑๓๑) นางสาวประภาภรณ์ บุตรพรม ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๐
๑๓๒) นางสาวนิลาวัลย์ นามพรม ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๑
๑๓๓) นางสาวพัชรินทร์ แสนสร้อย ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๒
๑๓๔) นายไพรวัลย์ เปรี่ยมพิมาย ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๓
๑๓๕) นางสาวศุภมาศ ทองมาก ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๔
๑๓๖) นางสาวลลิตา จิตรสว่าง ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๕
๑๓๗) นางสาวชไมพร เสิกภู่เขียว ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๖
๑๓๘) นางสาวกฤติมาพร คำมีแก่น ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๗
๑๓๙) นางสาวสกุลรัตน์ ภาคภูมิ ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๘
๑๔๐) นางสาวกาญจนา คงคูณ ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๙
๑๔๑) นางสาวไพรินทร์ ศรีรูปี ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๐
๑๔๒) นางสาวทิพเนตร ผุยปัญญา ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๑
๑๔๓) นางสาวสาธิตา ปานทอง ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๒
๑๔๔) นางสาวอริสา ทองนวล ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๓
๑๔๕) นางสาวอรยา ค้าคล่อง ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๔

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

๑๔๖) นางสาวชุดาภรณ์...

๑๔๖) นางสาวชุดาภรณ์ สุนทรสนาน	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๕
๑๔๗) นางสาวสุดารัตน์ นนท์ประสาท	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๖
๑๔๘) นางสาวรัชนีกร เนียมกลาง	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๗
๑๔๙) นางสาวกัญญารัตน์ ศรีนิลทา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๘
๑๕๐) นางสาวอัญชลี คำจันทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๙
๑๕๑) นายบุญฤทธิ์ เอี่ยมเทศ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๐
๑๕๒) นายศิริวัฒน์ พานิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๑
๑๕๓) นางสาวศุภรดา ปั้นมยุรา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๒
๑๕๔) นางสาวพาฤดี คุณนาน	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๓
๑๕๕) นางสาวจิราเจต ฟองดา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๔
๑๕๖) นางสาวกนกภรณ์ อุระ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๕
๑๕๗) นางสาวอารยา มีชัย	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๖
๑๕๘) นางสาวจิตสุภา ประเทืองสุข	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๗
๑๕๙) นางสาวอริสา วิริยขันติธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๘
๑๖๐) นางสาววิชชุตา นาคผจญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๙
๑๖๑) นางสาวพนิดา ยอดอินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๕๐
๑๖๒) นางสาวนันทิยา จันทะลุน	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๕๑

(นายศิระ จันทร์เฉิด)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๐๔
ที่ อก ๐๓๑๐(๑)/ ๑๐๖๙ ลงวันที่ ๒๘ มกราคม ๒๕๖๔

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๖๑ รายการ

น้ำเสีย จำนวน 59 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method[4]
2	Aldicarb Sulfone	High-Performance Liquid Chromatographic Method[4]
3	Aldicarb Sulfoxide	High-Performance Liquid Chromatographic Method[4]
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
5	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
6	Barium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
7	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
8	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
9	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
10	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
11	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method[4] 2) 5-Day BOD Test, Membrane Electrode Method[4]
12	Carbaryl	High-Performance Liquid Chromatographic Method[4]
13	Carbofuran	High-Performance Liquid Chromatographic Method[4]
14	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
15	Chemical Oxygen Demand	1) Closed Reflux, Colorimetric Method[4] 2) Closed Reflux, Tritimetric Method[4]
16	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
17	Chromium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[4]
18	Color	ADMI Weighted-Ordinate Spectrophotometric Method

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

19 Copper...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Copper	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
20	Cyanide	Distillation, Colorimetric Method[4]
21	2,4´-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
22	4,4´-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
23	2,4´-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
24	4,4´-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
25	2,4´-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
26	4,4´-DDT	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
27	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
28	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
29	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
30	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
31	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
32	Endrin Aldehyde	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
33	Formaldehyde	Distillation, Colorimetric Method[3]
34	Free Chlorine	1) DPD Ferrous Titrimetric Method[4] 2) Iodometric Method[4]
35	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
36	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
37	Hexavalent Chromium	Filtration, Colorimetric Method[4]
38	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method[4]
39	Lead	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
40	Manganese	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
41	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma/Mass spectrometric Method[4]
42	Methiocarb	High-Performance Liquid Chromatographic Method[4]
43	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]

44 Methomyl...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
44	Methomyl	High-Performance Liquid Chromatographic Method[4]
45	Nickel	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
46	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method[4] 2) Soxhlet Extraction Method[4]
47	Oxamyl	High-Performance Liquid Chromatographic Method[4]
48	Propoxur	High-Performance Liquid Chromatographic Method[4]
49	pH	Electrometric Method[4]
50	Phenols	1) Distillation, Chloroform Extraction Method[4] 2) Distillation, Direct Photometric Method[4]
51	Selenium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
52	Sulfide	Iodometric Method[4]
53	Temperature	Laboratory and Field Methods[4]
54	Total Dissolved Solids	Dried at 180 ^{0}C[4]
55	Total Kjeldahl Nitrogen	Semi-Micro Kjeldahl Method[4]
56	Total Suspended Solids	Dried at 103-105 ^{0}C[4]
57	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
58	Trivalent Chromium	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation[4]
59	Zinc	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[4]

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]

3 Aldrin...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
8	Barium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
13	Benzoic Acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
15	Benzo[g,h,i]perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

18 Bis(2-ethylhexyl)phthalate...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4] Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[4]
22	Butyl Benzyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
27	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

34 Chromium (III)...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Colorimetric Method; Calculation[4]
35	Chromium (VI)	Colorimetric Method[4]
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
37	Cyanide	Distillation, Colorimetric Method[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
39	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
40	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
41	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
43	Di-n-Butyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
47	3,3-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]

51 cis-1,2-Dichloroethylene...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และระเบียบข้อบังคับปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
57	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
58	Diethyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
63	Di-n-Octyl Phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
64	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
65	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

68 Fluorene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
69	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
70	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
74	α-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
75	β-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
76	γ-HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
81	Lead	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
83	Mercury	1) Cold Vapor Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

84 Methanol...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
นักวิทยาศาสตร์ชำนาญการพิเศษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
84	Methanol	1) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4] 2) Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[4]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
89	2-Methylnapthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
95	N-Nitrosodi-n-Propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
96	Polychlorinated Biphenyls - PCB 1016 - PCB 1221 - PCB 1232 - PCB 1242 - PCB 1248 - PCB 1254 - PCB 1260	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

97 Pentachlorophenol...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
98	pH	Electrometric Method[4]
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
100	Phenol	1) Distillation, Direct Photometric Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
102	Selenium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
103	Silver	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
104	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
106	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
107	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
109	TPH (C_5-C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,24]
110	TPH ($C_{>8}$-C_{16})	Solvent Extraction, Gas Chromatographic Method[9,21]
111	TPH ($C_{>16}$-C_{35})	Solvent Extraction, Gas Chromatographic Method[9,21]
112	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
113	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]

114 1,1,2-Trichloroethane...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดลอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
114	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
115	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
118	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
119	Vanadium	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]
120	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
121	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
122	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
123	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
124	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
125	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[4]
126	Zinc	1) Digestion, Inductively Coupled Plasma Method[4] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[4]

<u>อากาศเสีย (ปล่องระบาย) จำนวน 16 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic, Digestion, Inductively Coupled Plasma Method[5]
2	Arsenic	Isokinetic, Digestion, Inductively Coupled Plasma Method[5]

3 Carbon Monoxide...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Carbon Monoxide	1) Sampling Bag Non-Dispersive Infrared Method[5] 2) Non-Dispersive Infrared Method[5] 3) Instrumental Analyzer Method[5]
4	Chlorine	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method [5]
5	Copper	Isokinetic, Digestion, Inductively Coupled Plasma Method[5]
6	Dioxins	Isokinetic Sampling, Analysis by ISO/IEC 17025 Accredited Laboratory or Analysis by Department of Industrial Works Registered Laboratory (Dioxins/Furans Analysis Approved)[5]
7	Hydrogen Chloride	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method[5]
8	Hydrogen Sulfide	Absorption Sampling, Iodometric Method[5]
9	Lead	Isokinetic, Digestion, Inductively Coupled Plasma Method[5]
10	Mercury	1) Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[5] 2) Isokinetic, Digestion, Inductively Coupled Plasma Method[5]
11	Opacity	Ringelmann's Method[2]
12	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic Acid Method[5] 2) Chemiluminescence Method[5] 3) Instrumental Analyzer Method[5]
13	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method[5] 2) UV Fluorescence Method[5] 3) Instrumental Analyzer Method[5]
14	Sulfuric Acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method[5]
15	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method[5]
16	Xylene	Adsorption Sampling, Gas Chromatographic Method[5]

สิ่งปฏิกูล...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 35 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
2	Antimony	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
3	Arsenic	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
4	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

6 Cadmium...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
6	Cadmium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,19,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
8	Chromium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
9	Chromium (III)	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation Method[1,6,15,17] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation Method[1,6,16,17] 3) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,15,17] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8, 16,17]
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method[1,6,17] 2) Alkaline Digestion, Colorimetric Method[8,17]

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

11 Cobalt...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
12	Copper	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
13	2,4-D	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25]

2) Soxhlet...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method[10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
20	Lead	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[1,6,18]

2) Waste Extraction...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Waste Extraction, Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method[1,6,19] 3) Waste Extraction, Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[1,6,20] 4) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[18] 5) Thermal Decomposition Amalgamation and Atomic Absorption Spectrometric Method[19] 6) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[20]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
24	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
25	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
26	Nickel	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

27 Polychlorinated...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,3-Dichlorobiphenyl - 2,2',5-Trichlorobiphenyl - 2,4',5-Trichlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23] 2) Soxhlet Extraction, Gas Chromatographic Method[10,23] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]

28 Pentachlorophenol...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
28	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
29	pH	Electrometric Method[29,30]
30	Selenium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
31	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16]
32	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
33	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[1,9,25] 2) Soxhlet Extraction, Gas Chromatographic Method [10,22] 3) Automated Soxhlet Extraction, Gas Chromatographic Method [22,31]
34	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15]

4) Digestion...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
35	Zinc	4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16] 1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[1,6,16] 3) Digestion, Inductively Coupled Plasma Method[7,15] 4) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

<u>ดิน จำนวน 125 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
3	Aldrin	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
4	Anthracene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
5	Antimony	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
6	Arsenic	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
7	Atrazine	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
8	Barium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

9 Benz(a)anthracene...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
9	Benz(a)anthracene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
11	Benzo(b)fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
12	Benzo(k)fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
13	Benzoic acid	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
14	Benzo(a)pyrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
15	Benzo(g,h,i)perylene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
16	Beryllium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
17	Bis(2-chloroethyl)ether	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
18	Bis(2-ethylhexyl)phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
21	Butanol	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[12,24]
22	Butyl Benzyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
23	Cadmium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
24	Carbazole	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
25	Carbon Disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]

26 Carbon tetrachloride...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
27	Chlordane	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
28	p-Chloroaniline	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
31	Chloroform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
32	2-Chlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
33	Chromium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
34	Chromium (III)	1) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,15,17] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation Method[7,8,16,17]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method[8,17]
36	Chrysene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
37	Cyanide	Extraction, Distillation, Colorimetric Method[26,27,28]
38	2,4-D	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
39	DDD	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]

40 DDE...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	DDE	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
41	DDT	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
42	Dibenz(a,h)anthracene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
43	Di-n-Butyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
47	3,3-Dichlorobenzidine	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
53	2,4-Dichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]

57 Dieldrin...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
57	Dieldrin	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
58	Diethyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
59	2,4-Dimethylphenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
60	2,4-Dinitrophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
61	2,4-Dinitrotoluene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
62	2,6-Dinitrotoluene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
63	Di-n-Octyl Phthalate	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
64	Endosulfan	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
65	Endrin	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
67	Fluoranthene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
68	Fluorene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
69	Heptachlor	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
70	Heptachlor Epoxide	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]

71 Hexachlorobenzene...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
71	Hexachlorobenzene	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
74	α-HCH	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
75	β-HCH	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
76	γ-HCH	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
77	Hexachlorocyclopentadiene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
78	Hexachloroethane	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
79	Indeno(1,2,3-cd)pyrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
80	Isophorone	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
81	Lead	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
82	Manganese	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[18]

2) Thermal...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry[19] 3) Digestion, Cold-Vapor Atomic Fluorescence Spectrometric Method[20]
84	Methanol	Equilibrium Headspace, Gas Chromatographic/ Mass Spectrometric Method[12,24]
85	Methoxychlor	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
86	Methyl Bromide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
87	Methylene Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
88	2-methylphenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
89	2-Methylnaphthalene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
90	Methyl tert-Butyl Ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
91	Naphthalene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
92	Nickel	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
93	Nitrobenzene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
94	N-Nitrosodiphenylamine	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
95	N-Nitrosodi-n-propylamine	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
96	Polychlorinated biphenyls (PCBs) - Aroclor 1016 - Aroclor 1221 - Aroclor 1232	1) Soxhlet Extraction, Gas Chromatographic Method [10,23] 2) Automated Soxhlet Extraction, Gas Chromatographic Method [23,32]

- Aroclor 1242...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
	- Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260 - 2-Chlorobiphenyl - 2,2',3,5'-Tetrachlorobiphenyl - 2,2',5,5'-Tetrachlorobiphenyl - 2,3',4,4'-Tetrachlorobiphenyl - 2,2',3,4,5'-Pentachlorobiphenyl - 2,2',4,5,5'-Pentachlorobiphenyl - 2,3,3',4',6-Pentachlorobiphenyl - 2,2',3,4,4',5'-Hexachlorobiphenyl - 2,2',3,4,5,5'-Hexachlorobiphenyl - 2,2',3,5,5',6-Hexachlorobiphenyl - 2,2',4,4',5,5'-Hexachlorobiphenyl - 2,2',3,3',4,4',5-Heptachlorobiphenyl - 2,2',3,4,4',5,5'-Heptachlorobiphenyl - 2,2',3,4,4',5',6-Heptachlorobiphenyl - 2,2',3,4',5,5',6-Heptachlorobiphenyl - 2,2',3,3',4,4',5,5',6-Nonachlorobiphenyl	
97	Pentachlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
98	Phenanthrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
99	Phenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
100	Pyrene	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]

)

101 Selenium...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดลองมลพิษ
และทะเบียนห้องปฏิบัติการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
101	Selenium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
102	Silver	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
103	Styrene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
106	Toluene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
107	Toxaphene	1) Soxhlet Extraction, Gas Chromatographic Method[10,22] 2) Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
108	TPH (C_5–C_8)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
109	TPH ($C_{>8}$– C_{16})	1) Solvent Extraction, Gas Chromatographic Method[11,21] 2) Automated Soxhlet Extraction, Gas Chromatographic Method[21,31]
110	TPH ($C_{>16}$ – C_{35})	1) Solvent Extraction, Gas Chromatographic Method[11,21] 2) Automated Soxhlet Extraction, Gas Chromatographic Method[21,31]
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
115	2,4,5-Trichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]

116 2,4,6-Trichlorophenol...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
116	2,4,6-Trichlorophenol	Automated Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[25,31]
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
118	Vanadium	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]
119	Vinyl Acetate	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
120	Vinyl Chloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
121	m-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
122	o-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
123	p-Xylene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[14,24]
125	Zinc	1) Digestion, Inductively Coupled Plasma Method[7,15] 2) Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[7,16]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.**ราชกิจจานุเบกษา.** 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. **ราชกิจจานุเบกษา.** 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. **คู่มือวิเคราะห์น้ำเสีย.** พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 23rd ed. Washington, DC: APHA, 2017.

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2019.

6. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846,** 1997.

7. United States...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ

7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sludges and Sediments and Soils. SW-846 Method 3050B,** 1996.

8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A,** 1996.

9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C,** 1996.

10. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soxhlet Extraction. SW-846 Method 3540C,** 1996.

11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Microscale Solvent Extraction (MSE). SW-846 Method 3570,** 2002.

12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds (VOCs) in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A,** 2014.

13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Purge-and-Trap for Aqueous Samples. SW-846 Method 5030B,** 1996.

14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035,** 1996.

15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma- Atomic Emission Spectrometry. SW-846 Method 6010B,** 1996.

16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-Mass Spectrometry. SW-846 Method 6020A,** 2007.

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric). SW-846 Method 7196A,** 1992.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique). SW-846 Method 7471B,** 2007.

19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solids and Solutions by Thermal Decomposition, Amalgamation, and Atomic Absorption Spectrophotometry. SW-846 Method 7473,** 2007

20. United States...

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Mercury in Sediment and Tissue Sample by Atomic Fluorescence Spectrometry. SW-846 Method 7474, 2007.

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Nonhalogenated Organics Using GC/FID.SW-846 Method 8015B, 1996.

22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Organochlorine Pesticides by Gas Chromatography. SW-846 Method 8081B, 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Polychlorinate Biphenyls (PCBs) by Gas Chromatography. SW-846 Method 8082, 1996.

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8260D, 2018.

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Semivolatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8270E, 2018.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Total and Amenable Cyanide: Distillation SW-846 Method 9010B, 1996.

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Cyanide Extraction Procedure for Solids and Oil. SW-846 Method 9013A, 1996.

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric Procedures. SW-846 Method 9014, 2014.

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. pH Electrometric Measurement. SW-846 Method 9040C, 2004.

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soil and Waste pH. SW-846 Method 9045D, 2004.

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Automated Soxhlet Extraction. SW-846 Method 3541, 1994.

(นางริกาญจน์ ฉัตรสกุลวิไล)
ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ

ที่ อก ๐๓๑๐(๑)/ ๕๓๗๙

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๐๙ มีนาคม ๒๕๖๖

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๔ กุมภาพันธ์ ๒๕๖๖

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นดังนี้

๑. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑๙ ราย

๑) นายนคร สุขเจริญ	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๒
๒) นายบัญชา นามเขตต์	ทะเบียนเลขที่ ว-๒๐๔-จ-๖๑๒๓
๓) นายอรรคพล นิยมวิทยาพัน	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๐๘๗
๔) นางสาวพัชรียา หงษ์สมดี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๓
๕) นางสาวภานิดา สุรวงศ์ตระกูล	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๑๐๔
๖) นางสาวศรวณีย์ ยิ่งดี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๐๙
๗) นายสมโภช วันสา	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๕๑๙
๘) นายณัฐนันท์ ปานประเสริฐ	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๑๙
๙) ว่าที่ร้อยตรีภาณุพงศ์ แสนศรี	ทะเบียนเลขที่ ว-๒๐๔-จ-๗๘๓๖
๑๐) นายมุนินทร์ พูลศิริ	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๒
๑๑) นายณัฐดนัย เจือละออง	ทะเบียนเลขที่ ว-๒๐๔-จ-๘๖๐๗
๑๒) นางสาวกาญจนา คงคูณ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๒๙
๑๓) นางสาวรัชนีกร เนียมกลาง	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๗
๑๔) นางสาวกัญญารัตน์ ศรีนิลทา	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๓๘
๑๕) นายศิริวัฒน์ พานิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๑
๑๖) นางสาวกนกภรณ์ อุระ	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๕
๑๗) นางสาวจิตสุภา ประเทืองสุข	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๗
๑๘) นางสาวอริสา วิริยขันติธรรม	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๔๘
๑๙) นางสาวพนิดา ยอดอินทร์	ทะเบียนเลขที่ ว-๒๐๔-จ-๙๒๕๐

๒. ให้เพิ่มเจ้าหน้าที่...

๒. ให้เพิ่มเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๕ ราย

๑) นายกาจบัณฑิต กิตติศุภวณิชย์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๑
๒) นายภัทรพล สว่างใจธรรม์	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๒
๓) นายนราธิป เทือกชัยคำ	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๓
๔) นายศิริโชค พงษ์ประสม	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๔
๕) นายณัฐวุฒิ ด้วงแพง	ทะเบียนเลขที่ ว-๒๐๔-จ-๐๐๐๕

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ที่ อก ๐๓๑๐(๑)/๑๐๖๙ ลงวันที่ ๒๘ มกราคม ๒๕๖๔ คือในวันที่ ๒ กันยายน ๒๕๖๖ ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นางริกาญจน์ ฉัตรสกุลวิไล)
นักวิทยาศาสตร์ชำนาญการพิเศษ รักษาราชการแทน
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ที่ อก ๐๓๑๐(๑)/ ๖๑๒๕

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๓ มีนาคม ๒๕๖๖

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑๐ มีนาคม ๒๕๖๖

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๐๔ สถานที่ตั้งเลขที่ ๑๐๔ ซอยพัฒนาการ ๔๐ ถนนพัฒนาการ แขวงพัฒนาการ เขตสวนหลวง กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้เปลี่ยนแปลงชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จากเดิม นางสาวสรารัศมิ์ มงคลจิรวุฒิ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๙ เป็น นางสาวธัญญธร มงคลจิรวุฒิ ทะเบียนเลขที่ ว-๒๐๔-จ-๔๗๑๙

ทั้งนี้ หากท่านมีความประสงค์จะยื่นคำขอใดๆ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม ตาม QR Code ท้ายหนังสือฉบับนี้

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ยื่นคำขอผ่านระบบอิเล็กทรอนิกส์

คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน

วันที่ 4 **เดือน** สิงหาคม **พ.ศ** 2566

ข้าพเจ้า ( ) ผู้รับใบอนุญาตประกอบกิจการโรงงาน .....

(√) บริษัท/ห้างหุ้นส่วนจำกัด เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

กองวิจัยและเตือนภัยมลพิษโรงงาน
รับที่ 1656/66
วันที่ 7 ส.ค. 2566
เวลา 10.54 น.

ตั้งอยู่ที่เลขที่ 104 หมู่ที่ - ตรอก/ซอย พัฒนาการ 40

ถนน พัฒนาการ ตำบล/แขวง พัฒนาการ

อำเภอ/เขต สวนหลวง จังหวัด กรุงเทพมหานคร รหัสไปรษณีย์ 10250

โทรศัพท์ 02 760-3040 โทรสาร 0 2 760-3197

ได้รับทราบระเบียบกรมโรงงานอุตสาหกรรมว่าด้วยการขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน พ.ศ. 2560 โดยตลอดแล้วและยินยอมปฏิบัติตามระเบียบฯทุกประการ และได้แนบเอกสารต่างๆ ตามรายการเอกสารประกอบการพิจารณา (แบบ ปอ.1-1) มาพร้อมนี้

<u>รายการขอดำเนินการ</u>

การดำเนินการ	รายละเอียด (รายการ)				
	น้ำเสีย/น้ำทิ้ง	น้ำใต้ดิน	อากาศเสีย	สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว	ดิน
[ ] ขอขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน					
[√] ต่ออายุห้องปฏิบัติการวิเคราะห์เอกชน	59	126	16	35	125
[√] เปลี่ยนแปลงสารมลพิษที่วิเคราะห์ (√) เพิ่มสารมลพิษ ( ) ยกเลิกสารมลพิษ	-	-	12	-	-
[√] เปลี่ยนแปลงบุคลากร (√) เพิ่มบุคลากร (√) ยกเลิกบุคลากร	จำนวน 38 ราย (รายละเอียดตาม แบบ ปว.1) จำนวน 2 ราย (รายละเอียดตาม แบบ ปว.1)				
[ ] ยกเลิกห้องปฏิบัติการวิเคราะห์เอกชน					
[ ] อื่นๆ ..โปรดระบุ.....					

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
รับที่ ๕๕๕/๖๖
วันที่ ๗ ส.ค. ๖๖
เวลา ๑๓.๐๘ น.

จึงเรียนมาเพื่อโปรดพิจารณา

ลงชื่อ .....

(นางทัศนีย์ เลขากุลพร)

ผู้มีอำนาจลงนามแทนนิติบุคคล

ประทับตรา (ถ้ามี)

เรียน กวท.
เพื่อโปรดพิจารณา

(นายประสม ดำรงพงษ์)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน

ALS Laboratory Group (Thailand) Co., Ltd.

ที่ อก ๐๓๒๒/๑๓๖๕๙

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๕ ก.ย. ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๑๔ กรกฎาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด จำนวน ๓ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๖๗ สถานที่ตั้ง เลขที่ ๑๑๔/๑ หมู่ที่ ๘ ถนนกาญจนวนิช ตำบลบ้านพรุ อำเภอหาดใหญ่ จังหวัดสงขลา ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์
นางสาวกนิษฐา เหมประสาทพร ทะเบียนเลขที่ ว-๒๖๗-ค-๐๐๐๑

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์
๑) นางสาวอินทิรา คงประยูร ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๐๑
๒) นางสาวอมรรัตน์ เพชรประดับ ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๐๒
๓) นายทักษิณ อินโตรม ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๐๓
๔) นางสาวอณันฑา บุญเพ็ชร ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๐๔
๕) นางสาวสุทธิรัก ทิพย์รัตน์ ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๐๕
๖) นางสาวนริสา นฤมิตร ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๐๖
๗) นายวุฒิชัย ทวยเจริญ ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๐๗
๘) นายยงศิลป์ รังษี ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๐๘
๙) นายอภิวัฒน์ ฉันทะ ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๐๙
๑๐) นายศิริชัย เกลี้ยงเกิด ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๐
๑๑) นายสมศักดิ์ จันทร์คง ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๑
๑๒) นางสาวพิชญา ศุภรานนท์ ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๒
๑๓) นายปัญญา เกียรติพุฒิรักษ์ ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๓
๑๔) นางสาวศศินิภา รอดทองอ่อน ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๔
๑๕) นางสาวชุติมา สุขสวัสดิ์ ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๕
๑๖) นางสาวจันทิมา คงทน ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๖
๑๗) นางสาวกุลวดี เรืองประพันธ์ ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๗
๑๘) นางสาวอาทิตยา เมืองแก้ว ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๘
๑๙) นางสาวกวินณา ฉุ้นย่อง ทะเบียนเลขที่ ว-๒๖๗-จ-๐๐๑๙

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสียและอากาศเสีย ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้....

หนังสือฉบับนี้จะหมดอายุในวันที่ ๑๖ สิงหาคม ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายนเรศวร์ ตรียงค์)
ผู้อำนวยการศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคใต้
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

ศูนย์วิจัยและเตือนภัยมลพิษโรงงานภาคใต้
โทร. ๐ ๗๔๓๒ ๕๐๒๙, ๐ ๗๔๘๙ ๐๖๓๔ ต่อ ๕๒๐๑
ไปรษณีย์อิเล็กทรอนิกส์ sirw@diw.mail.go.th

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอแอลเอส แลบอราทอรี กรุ๊ป (ประเทศไทย) จำกัด เลขทะเบียน ว-๒๖๗
ที่ อก ๐๓๒๒/๑๓๖๕๙ ลงวันที่ ๒๕ ก.ย. ๒๕๖๖

ขอบข่ายสารมลพิษที่ได้รับการขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๗ รายการ

น้ำเสีย จำนวน 25 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Arsenic	Digestion, Inductively Coupled Plasma/Mass Spectrometric Method [1]
2	Barium	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
3	Biochemical Oxygen Demand	5-Day BOD Test, Azide Modification Method[1] 5-Day BOD Test, Membrane Electrode Method[1]
4	Cadmium	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
5	Chemical Oxygen Demand	Closed Reflux, Colorimetric Method[1] Closed Reflux, Titrimetric Method[1]
6	Chromium	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
7	Color	ADMI Weighted-Ordinate Spectrophotometric Method[1]
8	Copper	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
9	Formaldehyde	Distillation, Colorimetric Method[2]
10	Free Chlorine	DPD Ferrous Titrimetric Method[1]
11	Hexavalent Chromium	Filtration, Colorimetric Method[1]
12	Lead	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
13	Manganese	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
14	Mercury	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
15	Nickel	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
16	Oil & Grease	Liquid-Liquid, Partition-Gravimetric Method[1]

17 pH...

(นางสาวบุษยา รัตนสุภา)
นักวิทยาศาสตร์ชำนาญการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	pH	Electrometric Method[1]
18	Phenol	Distillation, Direct Photometric Method[1]
19	Selenium	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
20	Sulfide	ZnS Precipitation, Iodometric Method[1]
21	Temperature	Laboratory and Field Methods[1]
22	Total Dissolved Solids	Dried at 180 °C[1]
23	Total Suspended Solids	Dried at 103-105 °C[1]
24	Trivalent Chromium	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]
25	Zinc	Digestion, Inductively Coupled Plasma/ Mass Spectrometric Method[1]

<u>อากาศเสีย จำนวน 12 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[3]
2	Arsenic	Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[3]
3	Carbon Monoxide	Sampling Bag Non-Dispersive Infrared Method[3]
4	Copper	Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[3]
5	Dioxins	Isokinetic Sampling, Analysis by ISO/LEC 17025 Accredited Laboratory or Analysis by Department of Industrial Works Registered Laboratory[3]
6	Hydrogen Sulfide	Absorption, Iodometric Method[3]
7	Lead	Isokinetic Sampling, Digestion, Inductively Coupled Plasma/Mass Spectrometric Method[3]
8	Opacity	Ringelmann's Method[4]
9	Oxides of Nitrogen	Absorption Sampling, Phenoldisulfonic acid Method[3]
10	Sulfur Dioxide	Absorption Sampling, Barium-Thorin Titrimetric Method[3]
11	Sulfuric acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method[3]
12	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method[3]

<u>เอกสารอ้างอิง....</u>

(นางสาวบุษยา รัตนสุภา)
นักวิทยาศาสตร์ชำนาญการ

<u>เอกสารอ้างอิง</u>

1. APHA, AWWA, WEF. Standard Methods for the Examination of Water and Wastewater. 24th ed. Washington, DC: APHA, 2023.

2. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

3. United States Environmental Protection Agency. Standards of Performance for New Stationary Sources. 40 CFR 60. Appendix A, 2020.

4. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

(นางสาวบุษยา รัตนสุภา)
นักวิทยาศาสตร์ชำนาญการ