

ภาคผนวกที่ 5

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัด

- 5-1 เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศ
- 5-2 เอกสารสอบเทียบเครื่องมือตรวจวัดระดับเสียงโดยทั่วไป
- 5-3 เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพน้ำ



ภาคผนวกที่ 5-1

เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศ





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Flow measurement laboratory
Calibration services department.



NSC – TISI – TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : COF-014-66

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : TISCH
MODEL/TYPE : TE-5028
SERIAL NUMBER : 3945
ID NUMBER : TNP-F-CAL02
CONDITION AS-RECEIVED : Used item
CUSTOMER : TNP Environment Co., Ltd.
332/173 Vision Smart Life Village, Bangrak Phatthana,
Bang Bua Thong District, Nonthaburi 11110

RECEIVED DATE : 29 Sep 2023
MEASUREMENT DATE : 01 Oct 2023
ISSUE DATE : 01 Oct 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 25.1 °C and 57.0 %RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the VSL (National Metrology Institute of Netherlands) via Certificate number: G2211901

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol



Approved signatory



Calibration Department Manager

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{\text{Orifice}}$ inH ₂ O	γ	Standard Flow [Q_s] m ³ /min
1	0.705	755.985	24.95	23.76	68.702	1.098	1.045	0.641
2	1.005	756.073	24.81	23.66	53.939	2.343	1.527	0.933
3	1.122	756.065	24.44	23.62	48.579	2.981	1.724	1.050
4	1.166	756.080	24.33	23.58	46.771	3.229	1.794	1.093
5	1.421	756.160	24.48	23.64	34.286	4.973	2.226	1.356

Slope (m): 1.65230
 Intercept (b): -0.01279
 Correlation coefficient (r): 0.99984
 Uncertainty ($k=2$): 0.015 m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_{meter} mmHg	$\Delta p_{\text{Orifice}}$ inH ₂ O	γ	Standard Flow [Q_s] m ³ /min
1	0.705	755.985	24.95	23.76	68.702	1.098	0.658	0.644
2	1.005	756.073	24.81	23.66	53.939	2.343	0.961	0.937
3	1.122	756.065	24.44	23.62	48.579	2.981	1.083	1.053
4	1.166	756.080	24.33	23.58	46.771	3.229	1.127	1.097
5	1.421	756.160	24.48	23.64	34.286	4.973	1.399	1.360

Slope (m): 1.03492
 Intercept (b): -0.00806
 Correlation coefficient (r): 0.99984
 Uncertainty ($k = 2$): 0.015 m³/min

End of Certificate of Calibration



Site and Calibration Information

Location	: TNP Environment Co.,Ltd.	Date	: 20-Oct-23
Serial	: TNP-F-03-TSP	Tech	: [REDACTED]

Site Conditions

Barometric Pressure (mmHg)	: 759	Corrected Pressure (mmHg)	: 759
Temperature (deg C)	: 30	Temperature (deg K)	: 303
Average Press.(mmHg)	: 759	Corrected Average (mmHg)	: 759
Average Temp.(deg C)	: 30	Average Temp.(deg K)	: 303

Calibration Orifice

Make	: Tish Environment	Qstd Slope	: 1.69297
Model	: TE-5028A	Qstd Intercept	: -0.02071
Serial	: 3945	Date Certified	: October 1, 2023

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (Chart)	IC (Corrected)	Linear Regression	
1	7.60	1.637	59.00	59.46	Slope	: 30.5480
2	5.80	1.422	54.00	53.52	Intercept	: 9.7476
3	4.60	1.268	49.00	48.56	Corr. Coeff	: 0.9996
4	3.50	1.107	44.00	43.61	# of Observations : 5	
5	2.40	0.919	38.00	37.66		

Calibrate By :	[REDACTED]
Approved By :	[REDACTED]

Site and Calibration Information

Location : TNP Environment Co.,Ltd.
Serial : TNP-F-01-TSP

Date : 20-Oct-23
Tech : [REDACTED]

Site Conditions

Barometric Pressure (mmHg)	: 759	Corrected Pressure (mmHg)	: 759
Temperature (deg C)	: 30	Temperature (deg K)	: 303
Average Press.(mmHg)	: 759	Corrected Average (mmHg)	: 759
Average Temp.(deg C)	: 30	Average Temp.(deg K)	: 303

Calibration Office

Make	: Tish Environment	Qstd Slope	: 1.69297
Model	: TE-5028A	Qstd Intercept	: -0.02707
Serial	: 3945	Date Certified	: October 1, 2023

Calibration Information

Plate or	H2O	Qstd	I	IC	Linear Regression	
Test #	(In)	(m3/min)	(Chart)	(Corrected)	Slope	: 34.84626
1	7.20	1.587	56.00	56.49	Intercept	: 0.434914
2	5.50	1.401	49.00	48.56	Corr. Coeff	: 0.9928
3	4.50	1.258	44.00	44.60		
4	3.40	1.111	38.00	37.66	# of Observations	: 5
5	2.40	0.923	34.00	33.70		

Calibrate By : [REDACTED]

Approved By : [REDACTED]

Site and Calibration Information

Location	: TNP Environment Co.,Ltd.	Date	: 20-Oct-23
Serial	: TNP-F-02-TSP	Tech	: [REDACTED]

Site Conditions

Barometric Pressure (mmHg)	: 759	Corrected Pressure (mmHg)	: 759
Temperature (deg C)	: 30	Temperature (deg K)	: 303
Average Press.(mmHg)	: 759	Corrected Average (mmHg)	: 759
Average Temp.(deg C)	: 30	Average Temp.(deg K)	: 303

Calibration Orifice

Make	: Tish Environment	Qstd Slope	: 1.69297
Model	: TE-5028A	Qstd Intercept	: -0.02707
Serial	: 3945	Date Certified	: October 1, 2023

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (Chart)	IC (Corrected)	Linear Regression	
1	7.30	1.598	58.00	57.48	Slope	: 33.9984
2	5.60	1.401	54.00	53.52	Intercept	: 4.50629
3	4.50	1.258	49.00	47.57	Corr. Coeff	: 0.9908
4	3.50	1.095	43.00	42.62	# of Observations	: 5
5	2.40	0.923	35.00	34.69		

Calibrate By	:	[REDACTED]
Approved By	:	[REDACTED]

Site and Calibration Information

Location : TNP Environment Co.,Ltd.
Serial : TNP-F-09-TSP

Date : 20-Oct-23
Tech :

Site Conditions

Barometric Pressure (mmHg) : 759	Corrected Pressure (mmHg) : 759
Temperature (deg C) : 30	Temperature (deg K) : 303
Average Press.(mmHg) : 759	Corrected Average (mmHg) : 759
Average Temp.(deg C) : 30	Average Temp.(deg K) : 303

Calibration Orifice

Make : Tish Environment
Model : TE-5028A
Serial : 3945

Qstd Slope : 1.69297
Qstd Intercept : -0.02707
Date Certified : October 1, 2023

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (Chart)	IC (Corrected)	Linear Regression	
1	7.40	1.640	56.00	55.50	Slope	: 29.8403
2	5.60	1.414	50.00	49.55	Intercept	: 6.9021
3	4.40	1.244	45.00	44.60	Corr. Coeff	: 0.9971
4	3.40	1.095	39.00	38.65	# of Observations	: 5
5	2.40	0.923	35.00	34.69		

Calibrate By :

Approved By :

Site and Calibration Information

Location	: TNP Environment Co.,Ltd.	Date	: 20-Oct-23
Serial	: TNP-F-08-TSP	Tech	: [REDACTED]

Site Conditions

Barometric Pressure (mmHg)	: 759	Corrected Pressure (mmHg)	: 759
Temperature (deg C)	: 30	Temperature (deg K)	: 303
Average Press.(mmHg)	: 759	Corrected Average (mmHg)	: 759
Average Temp.(deg C)	: 30	Average Temp.(deg K)	: 303

Calibration Office

Make	: Tish Environment	Qstd Slope	: 1.69297
Model	: TE-5026A	Qstd Intercept	: -0.02707
Serial	: 3945	Date Certified	: October 1, 2023

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (Chart)	IC (Corrected)	Linear Regression	
1	7.20	1.565	57.00	56.49	Slope	: 35.5446
2	5.70	1.414	52.00	50.54	Intercept	: 0.3713
3	4.60	1.272	45.00	44.60	Corr. Coeff	: 0.9980
4	3.40	1.095	40.00	39.64	# of Observations	: 5
5	2.30	0.904	33.00	32.71		

Calibrate By : [REDACTED]

Approved By : [REDACTED]

Site Information

Location :	TNP Environment Co.,Ltd.	Date :	26-Oct-23
Serial :	TNP-F-04-PM10	Tech :	

Site Conditions

Barometric Pressure (mmHg) :	760	Corrected Pressure (mmHg) :	760
Temperature (deg C) :	29	Temperature (deg K) :	302
Average Press.(mmHg) :	760	Corrected Average (mmHg) :	760
Average Temp.(deg C) :	29	Average Temp.(deg K) :	302

Calibration Orifice

Make :	Tish Environment	Slope :	1.69297
Model :	TE-5028A	Intercept :	-0.02707
Serial :	3945	Calibration Due Date :	October 1, 2022

Calibration Data

Plate or Test #	H2O (in)	Qa (m3/min)	I (Chart)	IC (Corrected)	Linear Regression	
1	7.00	1.001	57.00	35.93	Slope	: 35.3408
2	5.50	0.889	51.00	32.15	Intercept	: 0.6370
3	4.20	0.779	45.00	28.37	Corr. Coeff	: 0.9995
4	3.40	0.703	40.00	25.21	# of Observations	: 5
5	2.60	0.605	35.00	22.06		

Calibrate By :	
Approved By :	

Site Information

Location	: TNP Environment Co.,Ltd.	Date	: 26-Oct-23
Serial	: TNP-F-05-PM10	Tech	: [REDACTED]

Site Conditions

Barometric Pressure (mmHg)	: 760	Corrected Pressure (mmHg)	: 760
Temperature (deg C)	: 29	Temperature (deg K)	: 302
Average Press.(mmHg)	: 760	Corrected Average (mmHg)	: 760
Average Temp.(deg C)	: 29	Average Temp.(deg K)	: 302

Calibration Orifice

Make	: Tish Environment	Slope	: 1.69297
Model	: TE-5028A	Intercept	: -0.02707
Serial	: 3945	Calibration Due Date	: October 1, 2022

Calibration Data

Plate or Test #	H2O (in)	Qa (m3/min)	I (Chart)	IC (Corrected)	Linear Regression	
1	6.90	0.994	57.00	35.69	Slope	: 51.7506
2	5.80	0.913	51.00	31.94	Intercept	: -15.5102
3	4.80	0.832	42.00	26.30	Corr. Coeff	: 0.9979
4	4.10	0.770	38.00	23.79	# of Observations	: 5
5	3.30	0.682	33.00	18.79		

Calibrate By	:	[REDACTED]
Approved By	:	[REDACTED]

Site Information

Location	: TNP Environment Co.,Ltd.	Date	: 26-Oct-23
Serial	: TNP-F-02-PM10	Tech	: [REDACTED]

Site Conditions

Barometric Pressure (mmHg)	: 760	Corrected Pressure (mmHg)	: 760
Temperature (deg C)	: 29	Temperature (deg K)	: 302
Average Press.(mmHg)	: 760	Corrected Average (mmHg)	: 760
Average Temp.(deg C)	: 29	Average Temp.(deg K)	: 302

Calibration Orifice

Make	: Tish Environment	Slope	: 1.69297
Model	: TE-5028A	Intercept	: -0.02707
Serial	: 3945	Calibration Due Date	: October 1, 2023

Calibration Data

Plate or Test #	H2O (in)	Qa (m3/min)	I (Chart)	IC (Corrected)	Linear Regression	
1	7.00	1.001	57.00	35.93	Slope	: 42.4302
2	5.70	0.905	52.00	32.78	Intercept	: -6.4391
3	4.60	0.815	44.00	27.74	Corr. Coeff	: 0.9910
4	3.80	0.742	38.00	23.95	# of Observations	: 5
5	2.80	0.639	34.00	21.43		

Calibrate By	:	[REDACTED]
Approved By	:	[REDACTED]

Site Information

Location	: TNP Environment Co.,Ltd.	Date	: 26-Oct-23
Serial	: TNP-F-06-PM10	Tech	: [REDACTED]

Site Conditions

Barometric Pressure (mmHg)	: 760	Corrected Pressure (mmHg)	: 760
Temperature (deg C)	: 29	Temperature (deg K)	: 302
Average Press.(mmHg)	: 760	Corrected Average (mmHg)	: 760
Average Temp.(deg C)	: 29	Average Temp.(deg K)	: 302

Calibration Orifice

Make	: Tish Environment	Slope	: 1.69297
Model	: TE-5028A	Intercept	: -0.02707
Serial	: 3945	Calibration Due Date	: October 1, 2023

Calibration Data

Plate or Test #	H2O (in)	Qa (m3/min)	I (Chart)	IC (Corrected)	Linear Regression	
1	7.20	1.015	60.00	37.19	Slope	: 52.3347
2	6.40	0.958	56.00	35.30	Intercept	: -14.8713
3	5.30	0.873	51.00	32.15	Corr. Coeff	: 0.9861
4	4.40	0.797	44.00	27.74	# of Observations	: 5
5	3.30	0.692	34.00	20.17		

Calibrate By	:	[REDACTED]
Approved By	:	[REDACTED]

Site Information

Location	: TNP Environment Co.,Ltd.	Date	: 26-Oct-23
Serial	: TNP-F-03-PM10	Tech	: [REDACTED]

Site Conditions

Barometric Pressure (mmHg)	: 760	Corrected Pressure (mmHg)	: 760
Temperature (deg C)	: 29	Temperature (deg K)	: 302
Average Press.(mmHg)	: 760	Corrected Average (mmHg)	: 760
Average Temp.(deg C)	: 29	Average Temp.(deg K)	: 302

Calibration Orifice

Make	: Tish Environment	Slope	: 1.69297
Model	: TE-5028A	Intercept	: -0.02707
Serial	: 3945	Calibration Due Date	: October 1, 2023

Calibration Data

Plate or Test #	H2O (in)	Qa (m3/min)	I (Chart)	IC (Corrected)	Linear Regression	
1	6.80	0.987	57.00	35.93	Slope	: 49.2516
2	5.90	0.920	50.00	31.52	Intercept	: -13.1042
3	5.00	0.849	45.00	28.37	Corr. Coeff	: 0.9963
4	3.80	0.742	38.00	23.95	# of Observations	: 5
5	3.20	0.682	33.00	20.17		

Calibrate By	:	[REDACTED]
Approved By	:	[REDACTED]



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



CALIBRATION CERTIFICATE

Certificate No.S2306518S

page 1 of 2

Customer : TNP ENVIRONMENT CO., LTD.

332/173 Moo 3 Tambon Bang Rak Phatthana,

Amphoe Bang Bua Thong, Nonthaburi 11110

Equipment : Non-automatic weighing instrument (Electronic instrument)

Manufacturer : Shimadzu

Order No. : 66S2523-1

Model : AP225WD

Ambient temperature : $(26.9 \pm 5.0) ^\circ\text{C}$

Accuracy class : -

Relative humidity : $(52.0 \pm 10.0) \%$

Capacity : 10 g / 220 g

Received date : 21-Jun-2023

Resolution : 0.00001 g / 0.0001 g

Date of calibration : 21-Jun-2023

Serial No. : D316301848

Date of issue : 24-Jun-2023

ID No. : TNP.LAB.30

Condition of the balance : Good working conditions

Place of calibration : ห้อง LAB

Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.

Condition of reference standard weight

Instrument	Nominal value	Serial No.	Certificate No.	Due-date	Density (kg/m ³)
1 Standard weight set	1 mg to 2 kg	15885+15849	M2210001S	8-Oct-2023	7950

Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By : Aekhasak Silarut
Technician

Approved Signatory :

This calibration certificate may not be reproduced other than in full,
except with the prior written approval of the head of TCS calibration laboratory.



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



CALIBRATION CERTIFICATE

Certificate No.S2306518S


page 2 of 2

The repeatability of indication

Nominal Value (g)	Standard Deviation of reading (g)	Maximum difference between successive reading (g)	n
100	0.000005	0.00001	5
200	0.00005	0.0001	5

The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading (g)
Point 1	100.0000
Point 2	100.0002
Point 3	100.0001
Point 4	100.0000
Point 5	100.0001
Eccentric Value	0.0002



The error of indication

Nominal Value (g)	Value of Reference Standard Weight (g)	Balance Reading (g)	Correction (g)	Uncertainty (±) (g)	k
Unload	0.00000	0.00000	0.00000	0.000016	2.32
0.1	0.10000	0.10003	-0.00003	0.000019	2.10
0.5	0.50000	0.50001	-0.00001	0.000023	2.04
1	1.00001	1.00000	+0.00001	0.000026	2.00
5	5.00000	5.00001	-0.00001	0.000038	2.00
10	9.99999	10.00001	-0.00002	0.000046	2.00
20	20.0000	20.0000	0.0000	0.000085	2.00
50	50.0000	50.0001	-0.0001	0.00011	2.00
100	100.0000	100.0000	0.0000	0.00018	2.00
200	200.0000	200.0004	-0.0004	0.00034	2.00

Remark : Adjustment, External weight nominal value 100 g, Standard weight of Lab

Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor (k), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

This report will certify of the calibrated equipment only.

--End--



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



CALIBRATION CERTIFICATE

Certificate No.S2306519S

page 1 of 2

Customer : TNP ENVIRONMENT CO., LTD.

332/173 Moo 3 Tambon Bang Rak Phatthana,

Amphoe Bang Bua Thong, Nonthaburi 11110

Equipment : Non-automatic weighing instrument (Electronic instrument)

Manufacturer : Sartorius

Order No. : 66S2523-2

Model : SECURA224-1S

Ambient temperature : $(26.8 \pm 5.0) ^\circ\text{C}$

Accuracy class : -

Relative humidity : $(52.0 \pm 10.0) \%$

Capacity : 220 g

Received date : 21-Jun-2023

Resolution : 0.0001 g

Date of calibration : 21-Jun-2023

Serial No. : 0041305301

Date of issue : 24-Jun-2023

ID No. : TNP.LAB.31

Condition of the balance : Good working conditions

Place of calibration : ห้อง LAB

Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.

Condition of reference standard weight

Instrument	Nominal value	Serial No.	Certificate No.	Due-date	Density (kg/m ³)
1 Standard weight set	1 mg to 2 kg	15885+15849	M2210001S	8-Oct-2023	7950

Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By : Aekhasak Silarut
Technician

Approved Signatory :

This calibration certificate may not be reproduced other than in full,
except with the prior written approval of the head of TCS calibration laboratory.



THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



CALIBRATION CERTIFICATE

Certificate No.S2306519S


page 2 of 2

The repeatability of indication

Nominal Value (g)	Standard Deviation of reading (g)	Maximum difference between successive reading (g)	n
200	0.00000	0.0000	5

The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading (g)
Point 1	100.0000
Point 2	100.0000
Point 3	100.0000
Point 4	99.9998
Point 5	99.9998
Eccentric Value	0.0002



The error of indication

Nominal Value (g)	Value of Reference Standard Weight (g)	Balance Reading (g)	Correction (g)	Uncertainty (±) (g)	k
Unload	0.0000	0.0000	0.0000	0.000082	2.00
0.1	0.1000	0.1000	0.0000	0.000083	2.00
0.5	0.5000	0.5000	0.0000	0.000084	2.00
1	1.0000	0.9999	+0.0001	0.000085	2.00
5	5.0000	5.0000	0.0000	0.000090	2.00
10	10.0000	10.0000	0.0000	0.000094	2.00
20	20.0000	20.0001	-0.0001	0.00011	2.00
50	50.0000	50.0001	-0.0001	0.00013	2.00
100	100.0000	100.0000	0.0000	0.00019	2.00
200	200.0000	199.9998	+0.0002	0.00033	2.00

Remark : Without adjustment

Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor (k), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

This report will certify of the calibrated equipment only.

--End--

Analyzer Performance Test

Calibrated Date: 2023-Nov-1

Instruments Information

Analyzer Type : CH4-NMHC-THC Analyzer

Manufacturer : HORIBA

Model : APHA-360CE

Serial Number : 423740300209

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Methane (CH₄) 181.0 PPM

Propane 180.7 PPM

Cylinder number EB0123130

Expire Date: 3 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.1	0.1	50.0	49.1	-1.8
NMHC	0.0	0.1	0.1	50.0	48.9	-2.2

Calibration Report (After adjust)

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Methane	0.0	0.0	0.0	50.0	50.0	0.0
NMHC	0.0	0.0	0.0	50.0	50.0	0.0

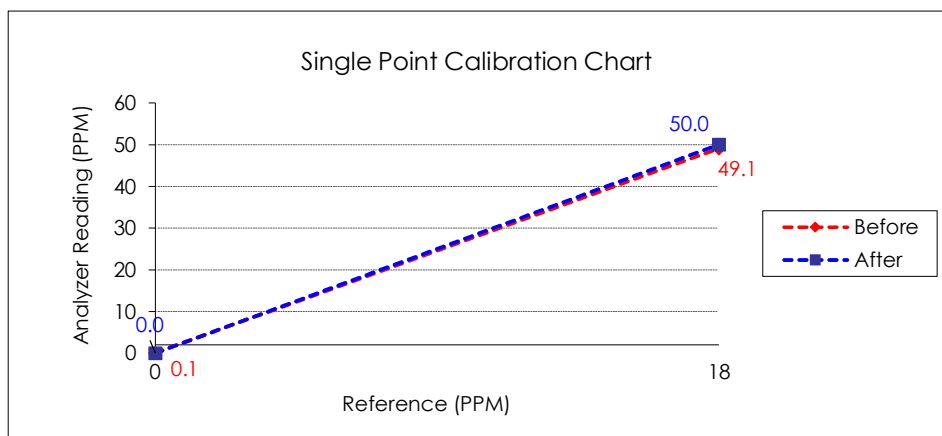

Calibrate By



Approve by



Analyzer Performance Test

Calibrated Date: 31 October 2023

Instruments Information

Analyzer Type : CO Analyzer
Model : 48C

Manufacturer : Thermo Environmental
Serial Number : 48CHL-67713-358

Calibrator Unit

Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Generator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM
Sulphur Dioxide (SO₂) 55.11 PPM
Carbon Monoxide (CO) 4,535 PPM
Cylinder number EB0129027
Expire Date: 29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	45.0	44.1	-2.0
After	0.0	0.0	0.0	45.0	45.0	0.0

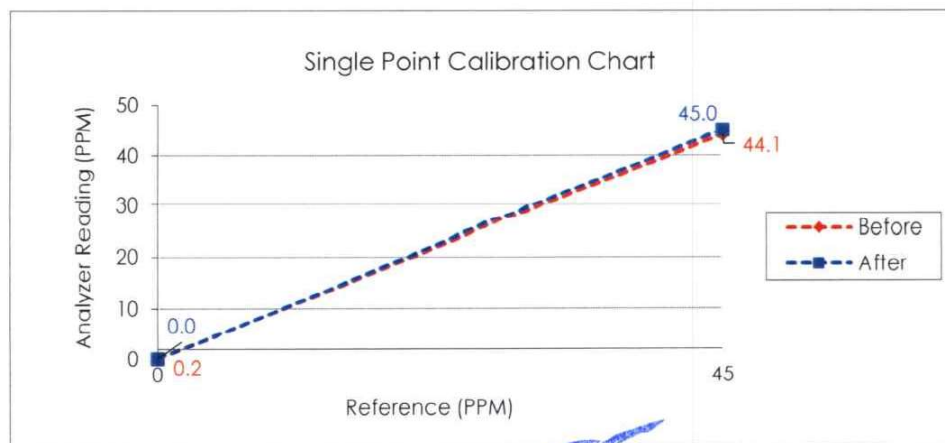

Calibrate By :



Approve by :



Analyzer Performance Test

Calibrated Date: 17 September 2023

Instruments Information

Analyzer Type : CO Analyzer

Model : 48C

Manufacturer : Thermo Environmental

Serial Number : 48C-79177-391

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM

Sulphur Dioxide (SO₂) 55.11 PPM

Carbon Monoxide (CO) 4,535 PPM


Cylinder number EB0129027

Expire Date: 29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	45.0	44.3	-1.6
After	0.0	0.0	0.0	45.0	45.0	0.0

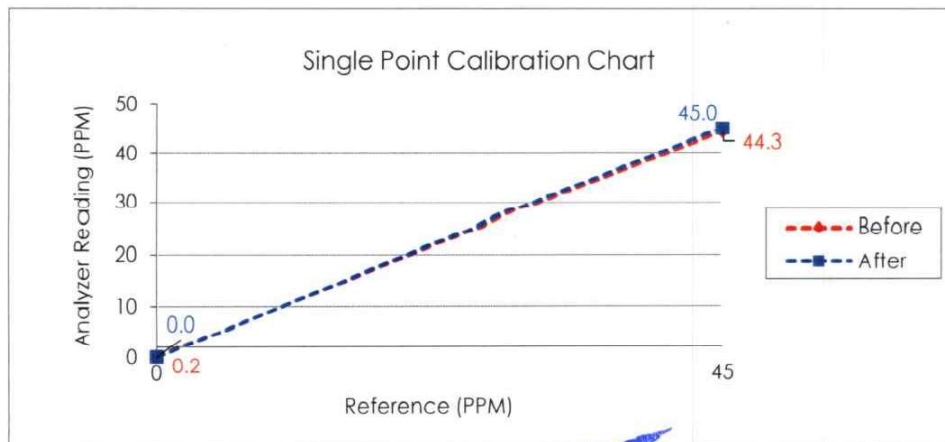

Calibrate By :



Approve by :



Analyzer Performance Test

Calibrated Date: 17 October 2023

Instruments Information

Analyzer Type : CO Analyzer
Model : 48C

Manufacturer : Thermo Environmental
Serial Number : 0401304259

Calibrator Unit

Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Generator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM
Sulphur Dioxide (SO₂) 55.11 PPM
Carbon Monoxide (CO) 4,535 PPM
Cylinder number EB0129027
Expire Date: 29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	45.0	44.2	-1.7
After	0.0	0.0	0.0	45.0	45.0	0.0

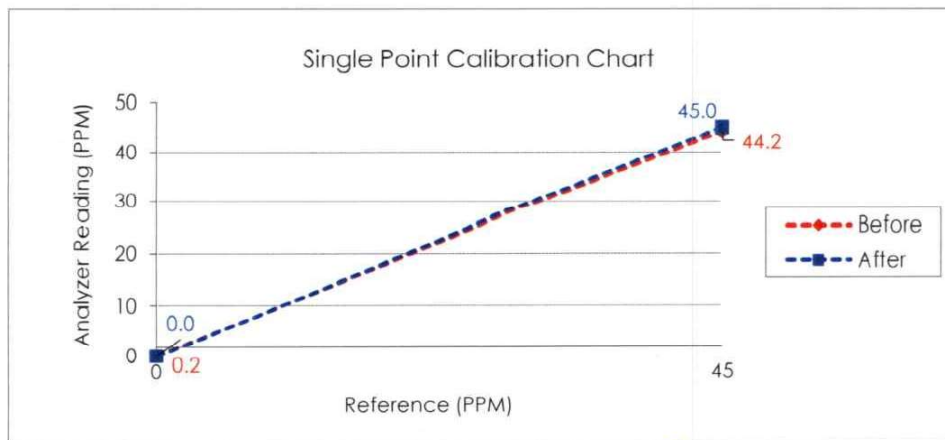

Calibrate By :



Approved By :



Analyzer Performance Test

Calibrated Date: 03 November 2023

Instruments Information

Analyzer Type : CO Analyzer
Model : 6050

Manufacturer : Sabio
Serial Number : 20300719

Calibrator Unit

Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Generator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM
Sulphur Dioxide (SO₂) 55.11 PPM
Carbon Monoxide (CO) 4,535 PPM
Cylinder number EB0129027
Expire Date: 29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	45.0	44.5	-1.1
After	0.0	0.0	0.0	45.0	45.0	0.0

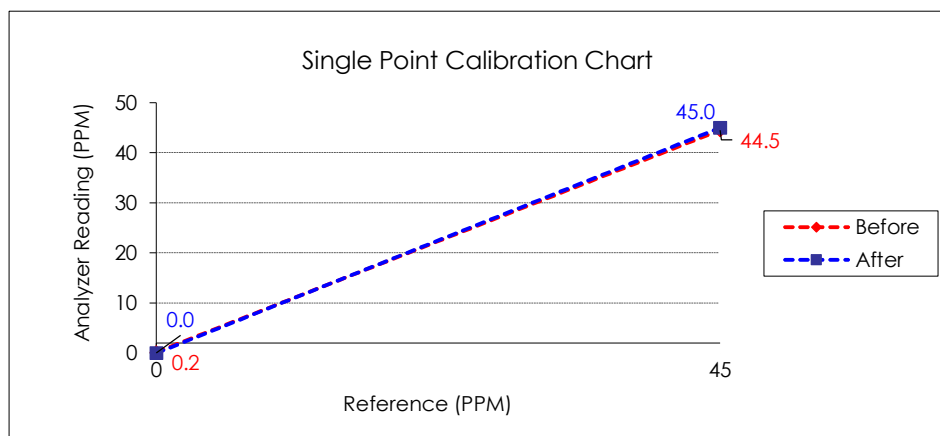

Calibrate By :



Approve by :



Analyzer Performance Test

Calibrated Date: 17 October 2023

Instruments Information

Analyzer Type : CO Analyzer
Model : 48C

Manufacturer : Thermo Environmental
Serial Number : 48C-67530-357

Calibrator Unit

Dilutor Model : Dasibi Model 5008
Serial Number : 705
ZERO AIR Generator : API MODEL 701
Serial Number : 1924


Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM
Sulphur Dioxide (SO₂) 55.11 PPM
Carbon Monoxide (CO) 4,535 PPM
Cylinder number EB0129027
Expire Date: 29 Oct. 2027

Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report

	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.2	0.2	45.0	44.3	-1.6
After	0.0	0.0	0.0	45.0	45.0	0.0

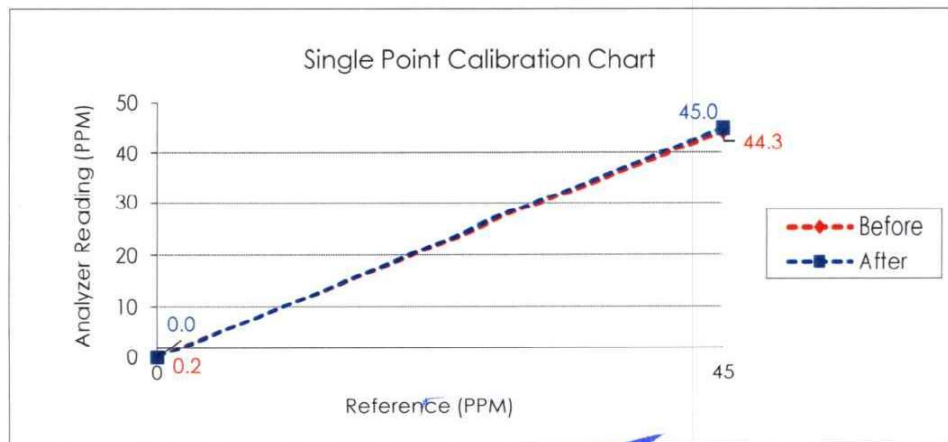

Calibrate By :



Approve by



Analyzer Performance Test

Calibrated Date: 18 September 2023

Instruments Information

Analyzer Type : NO-NO₂-NO_x Analyzer

Manufacturer : Thermo Environmental

Model : 42C

Serial Number : 0413406269

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM

Sulphur Dioxide (SO₂) 55.11 PPM

Carbon Monoxide (CO) 4,535 PPM

Cylinder number EB0129027

Expire Date: 29 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	393.4	-1.7
NO _x	0.0	0.0	0.0	400.0	394.6	-1.3

Calibration Report (After Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

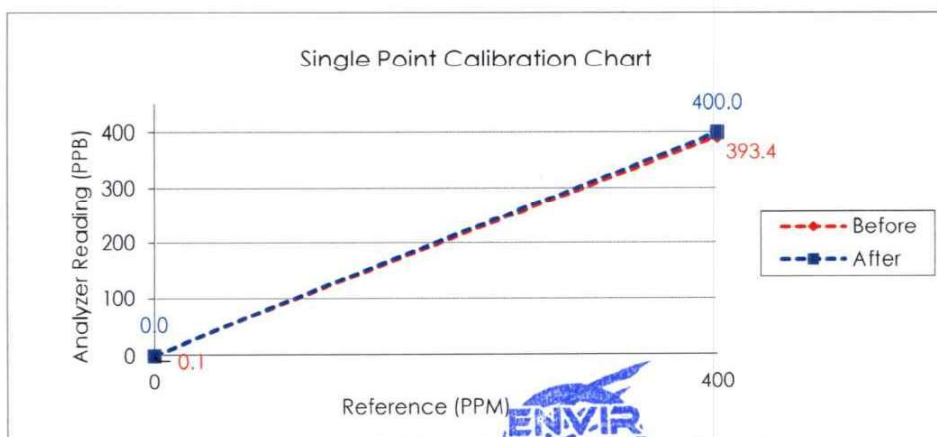

Calibrate By :

Approve by :

Analyzer Performance Test

Calibrated Date: 18 October 2023

Instruments Information

Analyzer Type : NO-NO₂-NO_x Analyzer

Manufacturer : Thermo Environmental

Model : 42C

Serial Number : 0527613258

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Standard Gas Concentration

Serial Number : 705

Nitric Oxide (NO) 55.47 PPM

ZERO AIR Generator : API MODEL 701

Sulphur Dioxide (SO₂) 55.11 PPM

Serial Number : 1924

Carbon Monoxide (CO) 4,535 PPM

Cylinder number EB0129027

Expire Date: 29 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	393.4	-1.7
NO _x	0.0	0.0	0.0	400.0	394.7	-1.3

Calibration Report (After Adjust)


Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

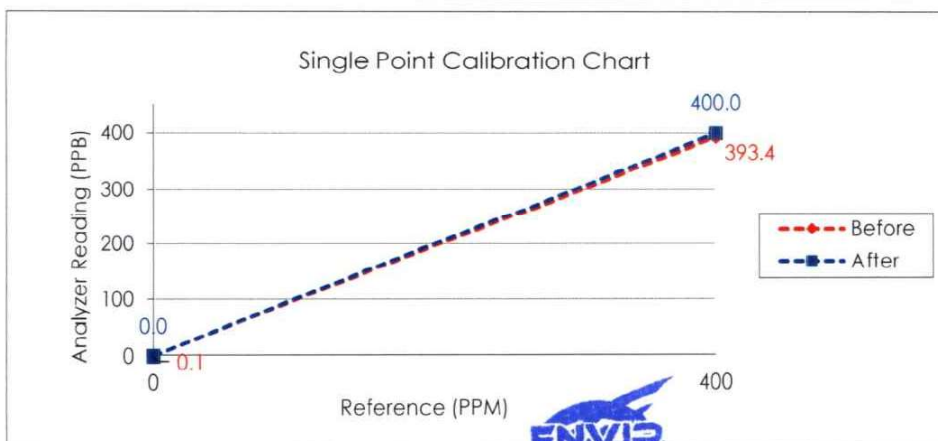

Calibrate By :



Approve by :



Analyzer Performance Test

Calibrated Date: 18 October 2023

Instruments Information

Analyzer Type : NO-NO₂-NO_x Analyzer

Manufacturer : Thermo Environmental

Model : 42C

Serial Number : 0518112467

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM

Sulphur Dioxide (SO₂) 55.11 PPM

Carbon Monoxide (CO) 4,535 PPM

Cylinder number EB0129027

Expire Date: 29 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before Adjust)


Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	393.2	-1.7
NO _x	0.0	0.0	0.0	400.0	394.7	-1.3

Calibration Report (After Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

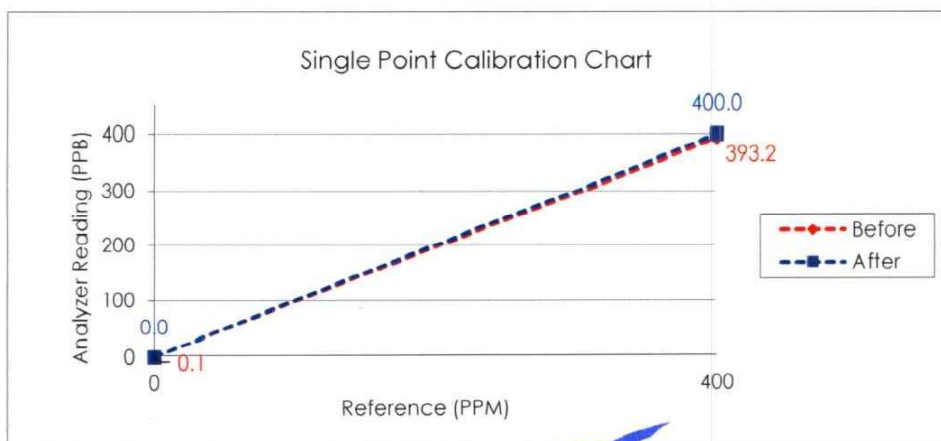

Calibrate By :



Analyzer Performance Test

Calibrated Date: 04 November 2023

Instruments Information

Analyzer Type : NO-NO₂-NO_x Analyzer

Manufacturer : Teledyne

Model : 200E

Serial Number : 1831

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM

Sulphur Dioxide (SO₂) 55.11 PPM

Carbon Monoxide (CO) 4,535 PPM

Cylinder number EB0129027

Expire Date: 29 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	395.1	-1.2
NO _x	0.0	0.0	0.0	400.0	395.4	-1.2

Calibration Report (After Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

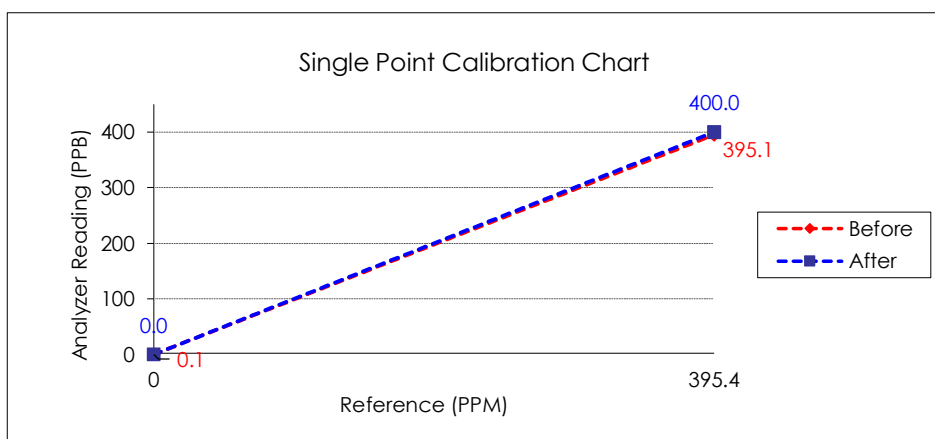

Calibrate By :

Approve by :

Analyzer Performance Test

Calibrated Date: 31 October 2023

Instruments Information

Analyzer Type : NO-NO₂-NO_x Analyzer

Manufacturer : Thermo Environmental

Model : 42C

Serial Number : 42C-70987-367

Calibrator Unit

Dilutor Model : Dasibi Model 5008

Serial Number : 705

ZERO AIR Generator : API MODEL 701

Serial Number : 1924

Standard Gas Concentration

Nitric Oxide (NO) 55.47 PPM

Sulphur Dioxide (SO₂) 55.11 PPM

Carbon Monoxide (CO) 4,535 PPM

Cylinder number EB0129027

Expire Date: 29 Oct. 2027


Environment : Temperature 25.5 °C Humidity: 51 %RH

Calibration Report (Before Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	393.1	-1.7
NO _x	0.0	0.0	0.0	400.0	394.4	-1.4

Calibration Report (After Adjust)

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
NO	0.0	0.1	0.1	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

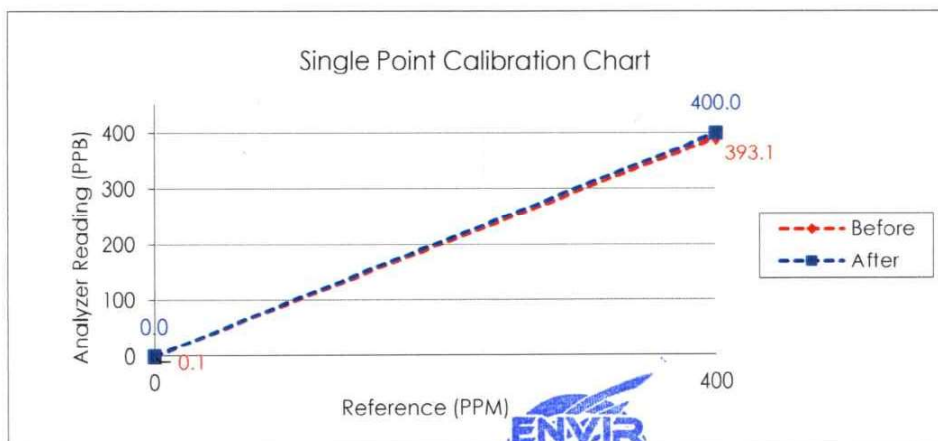

Calibrate By :



Approve by :





Certificate of Calibration

Certificate Number : SPR23030516-3

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Wireless Anemometer

Manufacturer : SCARLET TECH

Model : WL-21

Serial Number : 2112DR0105

ID. Number : TNP-F-W05

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Received Date : 30 Mar 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 03 Apr 2023

Location of Calibration : In-Lab

Recommend Due Date : 03 Apr 2024

Calibration Procedure : SP-CPM-04-10

Date of Issue : 04 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :

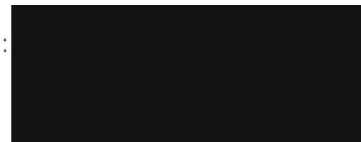

Authorized Signatory



Calibration Report

Certificate Number : SPR23030516-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Barometer	MHB-382SD	52188	L202302141-001	21 Feb 2024
Air Flow Meter (Pitot Tube)	TA400	200600812	L202302141-002	21 Feb 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

MIT - Miracle International Technology Co.,Ltd.



Result of Calibration

Certificate No. : SPR23030516-3

Page : 3 of 3

Range : 0.3 to 50 m/s

Unit : m/s

Temperature (°C)	Barometric Pressure (hPa)	Standard Reading	UUC Reading	Error	Uncertainty (±)
23.0	1007.0	2.55	2.6	0.05	0.25
23.0	1007.0	4.96	4.9	-0.06	0.25
23.0	1007.0	9.92	9.8	-0.12	0.33
23.0	1007.0	14.43	14.5	0.07	0.42

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95 %

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23030516-2

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Wireless Anemometer

Manufacturer : SCARLET TECH

Model : WL-21

Serial Number : 2112DR0114

ID. Number : TNP-F-W04

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Received Date : 30 Mar 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 03 Apr 2023

Location of Calibration : In-Lab

Recommend Due Date : 03 Apr 2024

Calibration Procedure : SP-CPM-04-10

Date of Issue : 04 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



Calibration Report

Certificate Number : SPR23030516-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Barometer	MHB-382SD	52188	L202302141-001	21 Feb 2024
Air Flow Meter (Pitot Tube)	TA400	200600812	L202302141-002	21 Feb 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
MIT - Miracle International Technology Co.,Ltd.



Result of Calibration

Certificate No. : SPR23030516-2

Page : 3 of 3

Range : 0.3 to 50 m/s

Unit : m/s

Temperature (°C)	Barometric Pressure (hPa)	Standard Reading	UUC Reading	Error	Uncertainty (±)
23.0	1007.0	2.55	2.4	-0.15	0.25
23.0	1007.0	4.96	4.8	-0.16	0.25
23.0	1007.0	9.92	9.8	-0.12	0.33
23.0	1007.0	14.43	14.3	-0.13	0.42

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95 %

- End of Certificate -

Certificate Number

CL-026-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE
SERIAL NUMBER
ID NUMBER
CONDITION AS-RECEIVED
CUSTOMER

: Cup anemometer
: Davis
: Sensor: -
Data logger: 6152CM
: Sensor: -
Data logger: BF200121006
: TNP-F-W01
: Used item
: TNP Environment Co., Ltd.
332/173 Vision Smart Life Village, Bangrak Phatthana,
Bang Bua Thong District, Nonthaburi 11110

RECEIVED DATE : 17 Feb 2023
MEASUREMENT DATE : 20 Feb 2023
ISSUE DATE : 24 Feb 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area ¹	900	cm ²
: Win direction frontal area ²	95	cm ²
: Diameter of mounting pipe ³	-	mm
: Blockage ratio of test object ⁴	0.106	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.6) °C, (48.1) %RH and (1011.8) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory:

Calibration Department Manager

Calibration procedure:

The cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0052-21 and MW-0066-22

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

v_{std} ⁶ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	v_{uuc} ⁷ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
0.982	23.60	23.55	0.9	-0.1	0.52
2.032	23.50	23.55	1.8	-0.2	0.53
3.039	23.64	23.55	2.9	-0.2	0.59
4.139	23.62	23.55	4.2	0.1	0.60
4.98	23.40	23.55	5.0	0.0	0.53
5.94	23.70	23.55	5.9	0.0	0.68
7.02	23.28	23.55	7.2	0.2	0.53
8.13	23.50	23.55	8.3	0.2	0.60
9.06	23.46	23.55	9.1	0.0	0.60
10.03	23.40	23.55	10.1	0.1	0.60
11.09	23.46	23.55	11.2	0.1	0.54
12.05	23.50	23.55	12.2	0.1	0.57
13.13	23.50	23.55	13.2	0.0	0.58
14.16	23.50	23.55	14.3	0.1	0.54
15.10	23.50	23.55	15.3	0.2	0.57
16.20	23.50	23.55	16.2	0.0	0.57

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP

Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

End of Certificate of Calibration

NAC
JIRANATE ASSOCIATES CO., LTD.

Certificate Number

CL-024-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE

SERIAL NUMBER

ID NUMBER
CONDITION AS-RECEIVED
CUSTOMER

: Wind Direction Sensor
: Davis
: Sensor: -
Data logger: 6152CM
: Sensor: -
Data logger: BF200121006
: TNP-F-W01
: Used item
: TNP Environment Co., Ltd.
332/173 Vision Smart Life Village, Bangrak Phatthana,
Bang Bua Thong District, Nonthaburi 11110

RECEIVED DATE
MEASUREMENT DATE
ISSUE DATE

: 17 Feb 2023
: 24 Feb 2023
: 24 Feb 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION

: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

: Wind tunnel cross-section area ¹	900	cm ²
: Win direction frontal area ²	49	cm ²
: Diameter of mounting pipe ³	-	mm
: Blockage ratio of test object ⁴	0.054	[-]

Preconditioning

: 24 hours at ambient conditions.

Measurement Condition

: The average values during measurement are (23.6)°C, (53.7) %RH and (1012.6 hPa).

TABULATION OF RESULTS:


The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol



Approved signatory: ...

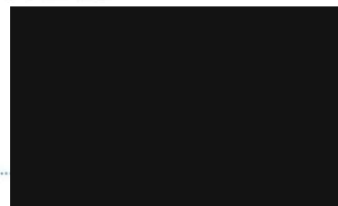

Calibration Department Manager

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D°_{std} Degree (°)	D°_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.01	45.000	45	0	0.74
	90.000	87	-3	0.68
	135.000	132	-3	0.68
	180.000	177	-3	0.68
	225.000	225	0	0.91
	270.000	270	0	0.58
	315.000	313	-3	0.76
	360.000	359	-1	0.58

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration



End of Certificate of Calibration

Certificate Number

CL-027-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Cup anemometer
MANUFACTURER : Davis
MODEL/TYPE : Sensor: -
Data logger: 6152CM
SERIAL NUMBER : Sensor: -
Data logger: BF210628045
ID NUMBER : TNP-F-W02
CONDITION AS-RECEIVED : Used item
CUSTOMER : TNP Environment Co., Ltd.
332/173 Vision Smart Life Village, Bangrak Phatthana,
Bang Bua Thong District, Nonthaburi 11110

RECEIVED DATE : 17 Feb 2023
MEASUREMENT DATE : 20 Feb 2023
ISSUE DATE : 24 Feb 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS	: Wind tunnel cross-section area ¹	900	cm ²
	Win direction frontal area ²	95	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.106	[-]

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are (23.5) °C, (48.3) %RH and (1017.3) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Calibration Department Manager

Calibration procedure:

The cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test section of Eiffel-type wind tunnel with 900 cm² cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0052-21 and MW-0066-22

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Remark:

- ¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


V_{std} ⁶ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} ⁷ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
0.982	23.44	23.50	0.9	-0.1	0.14
2.021	23.50	23.50	2.2	0.2	0.16
3.039	23.50	23.50	3.1	0.1	0.29
4.114	23.60	23.50	4.3	0.2	0.35
4.97	23.34	23.50	5.1	0.1	0.16
5.92	23.58	23.50	6.1	0.2	0.35
7.04	23.50	23.50	7.2	0.2	0.17
8.09	23.42	23.50	8.6	0.5	0.26
9.07	23.22	23.50	9.6	0.5	0.30
10.06	23.50	23.50	10.5	0.4	0.29
11.11	23.20	23.50	11.6	0.5	0.19
12.10	23.48	23.50	12.5	0.4	0.20
13.14	23.32	23.50	13.5	0.3	0.34
14.20	23.30	23.50	14.8	0.6	0.21
15.19	23.36	23.50	15.7	0.5	0.33
16.23	23.38	23.50	16.6	0.4	0.32

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Velocity of standard

⁷ Velocity of Unit Under Calibration

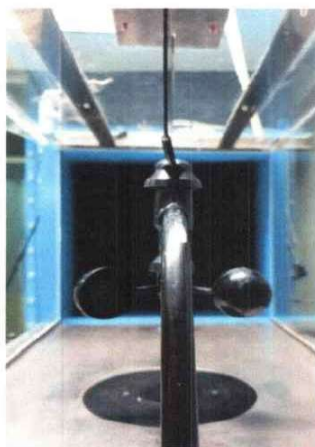PHOTO OF CALIBRATION SET-UP

Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.

End of Certificate of Calibration

JIRANATEE ASSOCIATES CO., LTD.

Certificate Number

CL-025-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor
MANUFACTURER : Davis
MODEL/TYPE : Sensor: -
Data logger: 6152CM
SERIAL NUMBER : Sensor: -
Data logger: BF210628045
ID NUMBER : TNP-F-W02
CONDITION AS-RECEIVED : Used item
CUSTOMER : TNP Environment Co., Ltd.
332/173 Vision Smart Life Village, Bangrak Phatthana,
Bang Bua Thong District, Nonthaburi 11110

RECEIVED DATE : 17 Feb 2023
MEASUREMENT DATE : 24 Feb 2023
ISSUE DATE : 24 Feb 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

PLACE OF CALIBRATION : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION	: Wind tunnel cross-section area ¹	900	cm ²
	Win direction frontal area ²	49	cm ²
	Diameter of mounting pipe ³	-	mm
	Blockage ratio of test object ⁴	0.054	[-]

Preconditioning : 24 hours at ambient conditions.

Measurement Condition : The average values during measurement are (23.7)°C, (49.2) %RH and (1015.3 hPa).

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

- ☒ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol

Approved signatory: ...

Calibration Department Manager

Remark:

¹ Nozzle cross-section area of the wind tunnel

² Projected cross-section area of the tested object include mounting pipe

³ Diameter of mounting pipe

⁴ Ratio ² to ¹

MEASUREMENT RESULTS⁵

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D°_{std} Degree (°)	D°_{uuc} Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.02	45.000	43	-2	0.91
	90.000	88	-3	0.76
	135.001	135	-1	0.76
	180.000	180	0	1.2
	225.000	225	0	0.91
	270.000	270	0	0.74
	315.000	315	0	0.97
	360.000	359	-1	0.58

Remark:

⁵ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

⁶ Direction of standard

⁷ Direction of Unit Under Calibration



End of Certificate of Calibration



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 24 October, 2023

Certification No. 372/23

Page : 1 of 2

Object : WIRELESS ANEMOMETER

Manufacturer : SCARLET

Type : WL-21

Serial No. : Wireless Receiver 2206DR0081 ID No. : TNP-F-W07
Wind Sensor 2205DT0026

Customer : TNP ENVIRONMENT CO.,LTD.
332/173 Moo 3 T.Bang Rak Phatthana,
A.Bang Bua Thong, Nonthaburi 11110.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1002.5 hPa

NATIONAL STANDARD WIND TUNNEL :

: Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

: Standard Velocity at 0 - 20 m/sec

Calibrated by :

Mechanical Engineer





THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 372/23

24 October, 2023

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacumm inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.00	-	-	-	6.9	0.10
9.02	-	-	-	9.0	0.12
11.01	-	-	-	11.0	0.01
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.1	-0.18
-	0.754	0.751	25.03	25.3	-0.27
-	1.083	1.083	30.03	30.4	-0.37

Wind Aloft Plotting Board.	
U.S. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	270
90	180
180	0
270	90

Calibrated by :

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



ภาคผนวกที่ 5-2

เอกสารสอบเทียบเครื่องมือตรวจวัดระดับเสียงโดยทั่วไป





Certificate of Calibration

Certificate Number : SPR23070550-1

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Sound Calibrator

Manufacturer : KEPLER

Model : KSM-42C

Serial Number : 160100568

ID. Number : TNP-F-CAL01

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 31 Jul 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 02 Aug 2023

Location of Calibration : In-Lab

Recommend Due Date : 02 Aug 2024

Calibration Procedure : In-House Method

Date of Issue : 03 Aug 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :

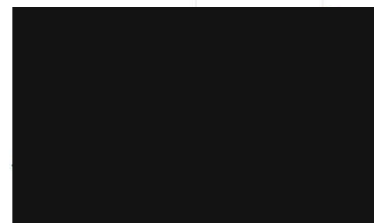

Authorized Signatory



Calibration Report

Certificate Number : SPR23070550-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Measuring Receiver	8902A	2950A02471	EF-0001-23	12 Jan 2024
AUDIO Analyzer	8903B	3011A09975	EL05303/23	14 Feb 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

NIMT - The National Institute of Metrology, Thailand.

PCAL - Professional Calibration & Services Co.,Ltd



Result of Calibration

Certificate No. : SPR23070550-1

Page : 3 of 3

Function : Sound Level

UUC Setting (\pm dB)	Standard Reading (dB)	Error (dB)	Uncertainty (\pm dB)
94	94.0	0.0	1.5
114	114.0	0.0	1.5

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23060536-5

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Sound Level Meter

Manufacturer : Scarlet Tech

Model : ST-25D

Serial Number : 10340950

ID. Number : TNP-F-S27

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 30 Jun 2023

Calibration Date : 11 Jul 2023

Recommend Due Date : 11 Jul 2024


Date of Issue : 12 Jul 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :

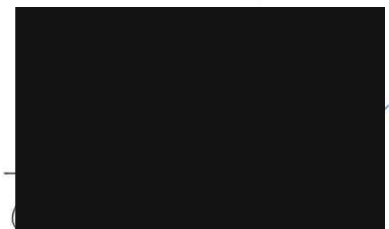

Authorized Signatory



Calibration Report

Certificate Number : SPR23060536-5

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23060536-5

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.3	94.3	0.3	0.3	0.15
114	114.2	114.2	0.2	0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.3	94.3	0.3	0.3	0.15
114	114.2	114.2	0.2	0.2	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23060536-1

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Sound Level Meter

Manufacturer : Scarlet Tech

Model : ST-25D

Serial Number : 10340942

ID. Number : TNP-F-S23

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 30 Jun 2023

Calibration Date : 11 Jul 2023

Recommend Due Date : 11 Jul 2024

Date of Issue : 12 Jul 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



Calibration Report

Certificate Number : SPR23060536-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23060536-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.3	114.3	0.3	0.3	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.3	114.3	0.3	0.3	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23060537-1

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Sound Level Meter

Manufacturer : Scarlet Tech

Model : ST-25D

Serial Number : 10340947

ID. Number : TNP-F-S28

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 30 Jun 2023

Calibration Date : 11 Jul 2023

Recommend Due Date : 11 Jul 2024

Date of Issue : 12 Jul 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :

Calibration Officer

Approved by :

Authorized Signatory



Calibration Report

Certificate Number : SPR23060537-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23060537-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15


Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23080172-2

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Sound Level Meter

Manufacturer : Scarlet Tech

Model : ST-25D

Serial Number : 10340948

ID. Number : TNP-F-S29

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 14 Aug 2023

Calibration Date : 14 Aug 2023

Recommend Due Date : 14 Aug 2024

Date of Issue : 15 Aug 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :




Calibration Officer

Approved by :



Authorized Signatory



Calibration Report

Certificate Number : SPR23080172-2

Page : 2 of 3


Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23080172-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.1	0.0	0.1	0.15
114	114.1	114.1	0.1	0.1	0.15


Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23060536-3

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Sound Level Meter

Manufacturer : Scarlet Tech

Model : ST-25D

Serial Number : 10340945

ID. Number : TNP-F-S25

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 30 Jun 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 11 Jul 2023

Location of Calibration : In-Lab

Recommend Due Date : 11 Jul 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 12 Jul 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :



Calibration Officer

Approved by :



Authorized Signatory



Calibration Report

Certificate Number : SPR23060536-3

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23060536-3

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.2	114.2	0.2	0.2	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.2	114.2	0.2	0.2	0.15


Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23080172-3

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Sound Level Meter

Manufacturer : Scarlet Tech

Model : ST-25D

Serial Number : 10340949

ID. Number : TNP-F-S30

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 14 Aug 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 14 Aug 2023

Location of Calibration : In-Lab

Recommend Due Date : 14 Aug 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 15 Aug 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by :




Calibration Officer

Approved by :



Authorized Signatory



Calibration Report

Certificate Number : SPR23080172-3

Page : 2 of 3


Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23080172-3

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.1	0.0	0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15


Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23080172-1

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi
11110

Equipment Name : Sound Level Meter

Manufacturer : Scarlet Tech

Model : ST-25D

Serial Number : 10340944

ID. Number : TNP-F-S24

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$ Received Date : 14 Aug 2023

Relative Humidity : $50\% \pm 15\%$ Calibration Date : 14 Aug 2023

Location of Calibration : In-Lab Recommend Due Date : 14 Aug 2024

Calibration Procedure : SP-CPE-04-01 Date of Issue : 15 Aug 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : [Redacted]

Approved by : [Redacted]

Calibration Officer

Authorized Signatory



Calibration Report

Certificate Number : SPR23080172-1

Page : 2 of 3


Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23080172-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

ภาคผนวกที่ 5-3

เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพน้ำ





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23T238

Page : 1 of 2

Equipment : Liquid-in Glass Thermometer

Manufacturer: SK

Model : -

Serial No.: -

ID No.: TNP.LAB.12

Condition As-Received: Used Item

Received Date: 27 January 2023

Calibration Date: 07 February 2023
to 10 February 2023

Reference: 2301-0937WN

Submitted by: TNP ENVIRONMENT CO.,LTD

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

332/173 Moo 3, Bang Rak Phatthana, Bang Bua Thong,
Nonthaburi 11110

Procedure used: Calibration were conducted using in-house calibration procedure CP-T02 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Digital Thermometer	1529	A7A609	22I1274	17 Oct 2023
2) Industrial Platinum Resistance Thermometer	5627-12	571975	22I1274	17 Oct 2023

2.The UUC* was immersed into liquid bath temperature controller and the top about 12 mm of the liquid column above the bath medium in every calibration points.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by :

Issue Date : 14 February 2023

Approved Signatory :

[]

[]

[✓]

B 0307331



Cert. No.: 23T238

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Temperature measurement.

Type:

Total Immersion

Scale Division:

1 °C

Reference point (0 °C) Error = -0.9681 °C, with Uncertainty of Measurement of ± 0.16 °C

<u>UUC*</u> <u>Reading</u> (°C)	<u>Standard</u> <u>Temperature</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (\pm °C)
20	21.4342	-1.4342	0.16
30	31.5544	-1.5544	0.16
40	41.1382	-1.1382	0.16

Note: UUC* : Unit Under Calibration

The UUC* readings were made under magnification and resolved to one tenth of one scale division.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484




Cert.No.: 23CH126

Page.: 1 of 2

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Adwa
Model : AD 12
Serial No. : 1328
ID No. : TNP.LAB.13
Condition As-Received: Used Item
Received Date : 27 January 2023
Calibration Date : 30 January 2023
Reference : 2301-0937WN-2
Submitted by : TNP ENVIRONMENT CO.,LTD
332/173 Moo 3, Bang Rak Phatthana,
Bang Bua Thong, Nonthaburi 11110
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement
with certified reference material (CRM)

Calibrated by :



Approved by :



Issue Date :

31 January 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written

Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0050390



Cert.No.: 23CH126

Page.: 2 of 2

Condition of this calibration result

1. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	826588	09 July 2024
pH 6.987	CPA chem	826589	09 July 2023
pH 10.008	CPA chem	826590	09 July 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing two buffers standard curve by using buffer nominal pH (4,7)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (\pm)	Coverage factor k
pH Electrode S/N.: 1328	4.008	4.01	N/A	0.0085	2.05
	6.987	6.99	N/A	0.011	2.00
	10.008	10.02	N/A	0.0095	2.00

Remark - pH meter does not have voltage mode.
- Can not connect the BNC because the plug does not match with the socket.
- N/A = Not Available

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23H487

Page : 1 of 2

Equipment : Digital Thermo-Hygrometer

Manufacturer: EXTECH

Model : 448515

Serial No.: PONPE5899555

ID No.: TNP.LAB.22

Condition As-Received: Used Item

Received Date: 02 March 2023

Calibration Date: 07 March 2023

Reference: 2303-0104WN

Submitted by: TNP ENVIRONMENT CO.,LTD.

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

332/173 Moo 3, Bang Rak Phatthana, Bang Bua Thong,
Nonthaburi 11110

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Hygro-M2 Dew Point Monitor	5112	2360195	20703	02 Aug 2023
2) Standard Humidity/Temperature Meter	400	10203027	TH-0082-22	22 Aug 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained at:-

- National Institute of Standards and Technology (NIST) , The United States of America
- National Institute of Metrology Thailand (NIMT)

Calibrated by : [REDACTED]
Issue Date : 10 March 2023

Approved Signatory : [REDACTED]

[REDACTED]

B 0310048



Cert. No.: 23H487

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Humidity Measurement

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	50.1	29	-21.1	1.6

Result of Calibration:-

Without Adjustment

Function:

Temperature Measurement

<u>Standard</u> <u>Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (±°C)
20.06	19.9	-0.16	0.46
24.99	25.1	0.11	0.46

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-o0o-

CERT.No.: HS-U039F

Certificate of Calibration

Calibration Date : 20 Jun 23

Submitted by : TNP ENVIRONMENT COMPANY LIMITED.

332/173 Moo. 3, Tambon Bang Rak Phatthana,

Amphoe Bang Bua Thong, Nonthaburi 11110

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 757.00 mmHg

Salinity : 0 ppt

Model : YSI 4010-2W

S/N : 22051520

Probe : YSI 4100

S/N : 22C102711

ID NO. : -

Air Temp ref : S/N. E00522

Barometric ref : S/N. E00522

Water Temp ref : S/N. 11431

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.05	(PASS)	-
Measurement 2 (mg/l)	9.05	(PASS)	-
Measurement 3 (mg/l)	9.04	(PASS)	-
Measurement 4 (mg/l)	9.03	(PASS)	-
Measurement 5 (mg/l)	9.04	(PASS)	-
Measurement 6 (mg/l)	9.04	(PASS)	-
Measurement 7 (mg/l)	9.04	(PASS)	-
Measurement 8 (mg/l)	9.03	(PASS)	-
Measurement 9 (mg/l)	9.03	(PASS)	-
Measurement 10 (mg/l)	9.03	(PASS)	-

Mean Measurement	9.04	mg/l	-	-
Inaccuracy	0.05	mg/l	-	-

Overall Status (PASS)


Manufacturer Specification

Accuracy = +/- 0.2 mg/l


- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



(Kittipong Maekwong)



(Natenapha Pisatkunchon)

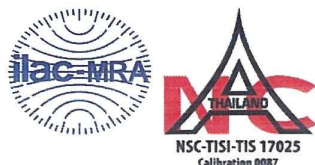

Certificate of Calibration

Equipment:	Balance	Certificate No.:	C01223732
Model:	PX623	Issued Date:	09 December 2022
Serial No. (or ID.):	C236754745	Job No.:	KSPR2215576
Manufacturer:	Ohaus	Page:	1 of 2
Condition:	New		

Customer: United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,
Phrakhanong District, Bangkok, THAILAND 10260

Environment Condition: Temperature 26 °C ± 0.5 °C
Humidity 53 %RH ± 3.9 %RH

Calibration Place: United Analyst and Engineering Consultant Co., Ltd. (301 Microbiology Room)
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,
Phrakhanong District, Bangkok, THAILAND 10260

Calibration By: Mr. Adisai Maknoi

Calibration Date: 09 December 2022

The Method used: In-house method, CAL-WI-47, based on UKAS Lab 14

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02221765



Person in charge



Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.


The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

Calibration Results:

Without Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

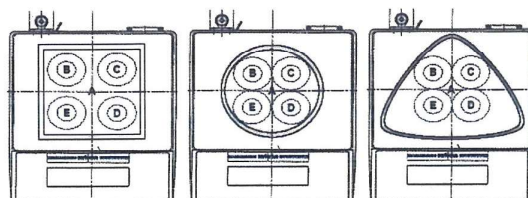			Nominal Test Value		200	(g)
Reference Points (g)						
A	B	C	D	E		
-	0.000	0.000	0.000	0.000		

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.001 (g)

Nominal test value (g)	Standard Deviation
50	0.0004
500	0.0005

Error of indication from nominal or conventional mass value., Readability 0.001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of Indication (g)	Uncertainty (g)	k
1	1.0000	1.000	0.000	0.0010	2.03
5	5.0001	5.000	0.000	0.0010	2.03
10	10.0001	10.000	0.000	0.0010	2.03
20	20.0001	20.000	0.000	0.0010	2.03
50	50.0001	50.000	0.000	0.0010	2.03
100	100.0001	100.000	0.000	0.0011	2.03
200	200.0004	200.000	0.000	0.0011	2.02
300	300.0005	300.000	-0.001	0.0013	2.01
400	400.0008	400.001	0.000	0.0014	2.01
500	500.0003	500.000	0.000	0.0017	2.00
600	600.0004	600.000	0.000	0.0019	2.00

The End of Certificate

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The error of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, UKAS Lab14. Therefore, those parameters have not been assessed separately.

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk $< 50\%$ PFA.
- ☒ Choice B Non-binary statement with guard band ($w = 1 U$), Pass or Fail Specific Risk $< 2.5\%$ PFA and Condition Pass or Condition Fail Specific Risk $< 50\%$ PFA.
- ☐ Choice C Customer defined, Customers may define arbitrary multiple of r to have applied as guard band ($w = r U$).
- ; PFA – Probability of False Accept



Authorized signatory

Statements of conformity:

Without Adjustment

Readability; 0.001 g

Nominal Value g	Error of indication g	Guard band (w) g	Tolerance (\pm) g	Conformity
1	0.000	0.0010	0.002	Pass
5	0.000	0.0010	0.010	Pass
10	0.000	0.0010	0.020	Pass
20	0.000	0.0010	0.040	Pass
50	0.000	0.0010	0.100	Pass
100	0.000	0.0011	0.200	Pass
200	0.000	0.0011	0.400	Pass
300	-0.001	0.0013	0.600	Pass
400	0.000	0.0014	0.800	Pass
500	0.000	0.0017	1.000	Pass
600	0.000	0.0019	1.200	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.


The End of Statements of conformity

Without Adjustment

Job No.KSPR2215576

Readability:0.001g

Error of indication

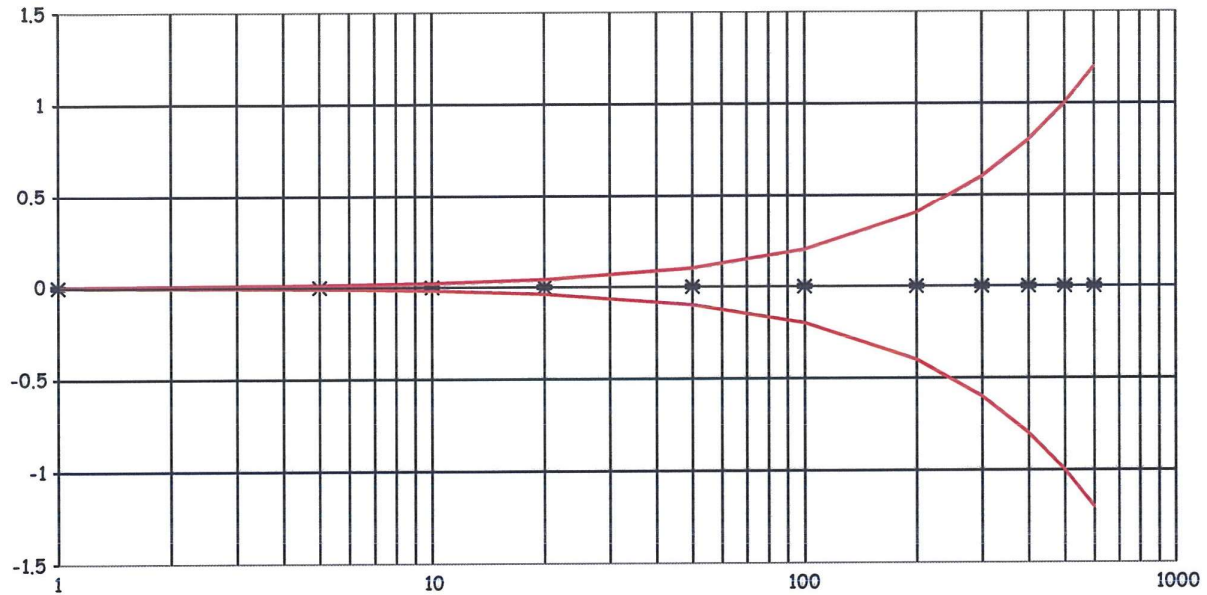

x Error of indication
--- Lower Acceptance limit
--- Upper Specification

— Uncert (+)
--- Upper Acceptance limit

— Uncert (-)
--- Lower Specification

Display of balance

เอกสารไม่ควบคุม