

## ภาคผนวกที่ 4

ใบรับรองการสอบเทียบเครื่องมือ

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

Certificate No. : 66-400012-2

Page : 1 of 2

Submitted by : M E T Company Limited  
36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

Equipment : Digital Thermometer with Thermistor Probe  
Temperature Indicator  
Manufacturer : Eutech Model : pH 150  
Range : N/A Resolution : 0.1 °C  
Serial No. : 2913288 ID No. : MET-PH05/63  
Thermistor Probe  
Model : PHWPTEM01W Sheath Material : Stainless  
Diameter : 3 mm. Length : 85 mm.  
Serial No. : 459 ID No. : MET-PH05/63

Environment : Ambient Temperature : (23 ± 2) °C  
Relative Humidity : (50 ± 15) %  
Line Voltage : (220 ± 22) VAC

Date of Received : 05 January 2023

Date of Calibration : 11 January 2023

Date of Issue : 11 January 2023

Calibrated by : [Redacted]

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)
400004	21E1850	14 Jun 2023	National Institute of Metrology Thailand (NIMT)

Approve

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 66-400012-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth ( mm. )	Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
85	10.0012	10.1	-0.1	0.11
85	50.0024	50.4	-0.4	0.11

### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- 000 -



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpoed, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025  
CALIBRATION 0030

## Certificate of Calibration

Certificate No. : 66-420023-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : pH Meter with electrode

pH meter

Manufacturer : Thermo Scientific Model : pH 150

Range : N/A pH Resolution : 0.01 pH

Serial No. : 2943538 ID No. : MET-PH06/63

Electrode

Model : N/A Serial No. : 66365

Environment : Ambient Temperature : (25 ± 2) °C

Relative Humidity : (50 ± 15) %

Date of Received : 02 March 2023

Date of Calibration : 04 March 2023

Date of Issue : 04 March 2023

Calibrated by :

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
440001	21E997	17 Mar 2023	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61235182	857394	11 Dec 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61267169	857395	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61260481	857396	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpoed, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 66-420023-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage ( mV )	Nominal Value ( pH )	UUC Reading		Correction ( mV )	Uncertainty ( ± mV )
			( pH )	( mV )		
4, 7, 10	177.4800	4	4.00	177.4	0.1	0.060
	0.0000	7	7.00	-0.1	0.1	0.058
	-177.4800	10	10.00	-177.6	0.1	0.060

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer ( pH )	UUC Reading ( pH )	Correction ( pH )	Uncertainty ( ± pH )
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- oOo -



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

Certificate No. : 66-200067-1

Page : 1 of 2

Submitted by : M E T Company Limited

36/659 Moo 6, T. Bangrakpattana, A. Bangbuatong, Nonthaburi 11110

Equipment : Electronic Balance

Manufacturer : METTLER TOLEDO Model : AG285

Serial No. : 1122140126 ID No. : MET-EB01/46

Capacity : 210 g Resolution : 0.00001g/81g, 0.0001g/210g

Environment : On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (26.4 to 26.8) °C

Relative Humidity : (54.9 to 58.8) %

Air Pressure : 1013.0 mbar

Date of Received : 02 March 2023

Date of Calibration : 02 March 2023

Date of Issue : 13 March 2023

Calibrated by : [Redacted]

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14  
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by : [Redacted]

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

Certificate No. : 66-200067-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty ± (g)
0.01	0.00001	0.000020
0.1	0.00000	0.000019
1	-0.00002	0.000031
5	-0.00004	0.000043
10	-0.00008	0.000054
20	-0.00027	0.000071
50	-0.00059	0.00011
100	-0.0009	0.00023
150	-0.0012	0.00038
200	-0.0019	0.00040

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2.43$ , providing a level of confidence of approximately 95%

Eccentric error Load test : 50 g  
A B C D E  
0.00055 0.00027 -0.00015 -0.00018 0.00000 g



Repeatability Load test : 200 g  
Stdev. : 0.000053 g

- o o o -



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpoed, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

**Certificate No. :** 66-400476-4

**Page : 1 of 2**

**Submitted by :** M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

**Equipment :** Air Chamber (Refrigerator)

Manufacturer : Sanden Intercool

Model : YPR-068S

Range : N/A °C

Resolution : 1 °C

Serial No. : YPR0682S-140100003R

ID No. : MET-RE02/57

**Environment :** On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (29.5 to 30.5) °C

Relative Humidity : (54 to 57) %

Line Voltage : (220.5 to 221.8) V

**Date of Received :** 23 August 2023

**Date of Calibration :** 23 August 2023

**Date of Issue :** 23 August 2023

**Calibrated by :**

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units Standard Digital Thermometer with Thermocouple probe

ID No.	Cert.No.	Due Date	Traceability
400046 & 400023	66-400184-1	03 Oct 2023	National Institute of Metrology Thailand (NIMT)

Approved by

Supervisor

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpoed, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

**Certificate No. :** 66-400476-4


**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

This instrument was setting air ventilation at position 0 (close)

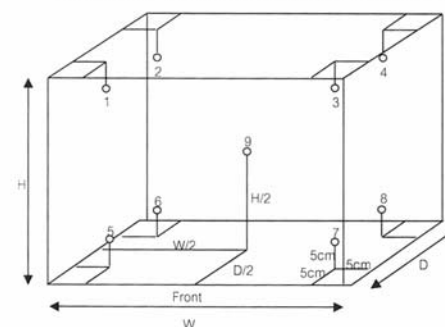

Inside of Chamber

W = 0.58 m

D = 0.60 m

H = 1.45 m

Capacity = 0.50 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
3	2	2	4.4	3.7	4.3	3.9	4.1	4.3	3.9	4.2	3.2	0.89

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
3	2	2	1.5	0.3	1.7

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%

- o0o -

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL-F0031-03





# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

**Certificate No. :** 66-400476-1

**Page :** 1 of 2

**Submitted by :** M E T Company Limited

36/659 Moo 6, T.Bangrakpattana, A.Bangbuatong, Nonthaburi 11110

**Equipment :** Air Chamber (Oven)

Manufacturer : Memmert

Model : UM 100

Range : N/A °C

Resolution : 0.1 °C

Serial No. : b197.0985

ID No. : MET-OV01/46

**Environment :** On site calibration was carried out at the Laboratory, M E T Company Limited

Ambient Temperature : (31.0 to 32.0) °C

Relative Humidity : (55 to 60) %

Line Voltage : (210.0 to 210.8) V

**Date of Received :** 23 August 2023

**Date of Calibration :** 23 August 2023

**Date of Issue :** 23 August 2023

**Calibrated by :**

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

**ID No.** **Cert.No.** **Due Date** **Traceability**

400029 & 400032 66-400228-1 25 Oct 2023 National Institute of Metrology Thailand (NIMT)

Approved by

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

**Certificate No. :** 66-400476-1


**Page :** 2 of 2

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

This instrument was setting air ventilation at position 0 (close)

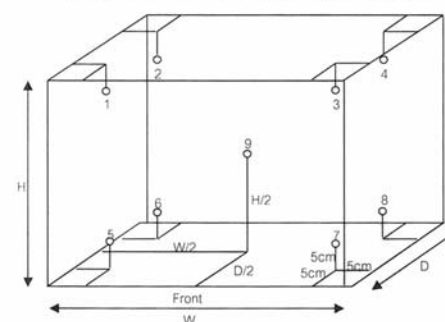

Inside of Chamber

W = 0.32 m

D = 0.18 m

H = 0.24 m

Capacity = 0.01 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
180.0	180.0	180.0	181.7	180.1	180.5	180.7	181.5	181.7	181.3	181.4	180.1	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
180.0	180.0	180.0	1.7	0.2	2.0

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



CAL-F0031-03