

ภาคผนวกที่ 5

เอกสารการสอบเทียบเครื่องมือตรวจวิเคราะห์คุณภาพน้ำทิ้ง

ตารางสรุปรายการเอกสารการสอบเทียบเครื่องมือตรวจวิเคราะห์น้ำทิ้ง

| รายการตรวจวัด | เครื่องมือเก็บตัวอย่าง | เครื่องมือตรวจวิเคราะห์ |
|--------------------------|------------------------|-------------------------|
| | ชื่อเครื่องมือ | ชื่อเครื่องมือ |
| คุณภาพน้ำทิ้ง | | |
| - pH | - | - pH Meter |
| - BOD ₅ | - | - BOD Analyzer |
| - TSS | - | - Electronic Balance |
| - TDS | - | - Electronic Balance |
| - Settleable Solids | - | - Electronic Balance |
| - TKN | - | - Electronic Balance |
| - Sulfide | - | - Electronic Balance |
| - Grease & Oil | - | - Electronic Balance |
| - TCB | - | - Incubator |
| - FCB | - | - Water Bath |
| - Free Chlorine | - | - |
| - Standard plate count | - | - Water Bath |
| - <i>Legionella</i> spp. | - | - Incubator |



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 23E8494
REFERENCE No : 70413-1

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : HANNA
MODEL : HI 3512
SERIAL No : TH118035
ID No : pH04/56
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 06-Sep-23

APPROVED BY :

ISSUED DATE : 06-Sep-23

RECEIVED DATE : 31-Aug-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 2 OF 3

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : HANNA
ID No : pH04/56
RECEIVED DATE : 31-Aug-23
AMBIENT TEMPERATURE : 23 ° C ± 3 ° C
MODEL : HI 3512
SERIAL NUMBER : TH118035
CALIBRATION DATE : 06-Sep-23
RELATIVE HUMIDITY : 50 % RH ± 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

- THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
- REFERENCE STANDARD INSTRUMENTS :-

| INSTRUMENT | MODEL | SERIAL No/ LOT No | CERTIFICATE No | DUE DATE |
|---------------------------|----------|----------------------|----------------|-----------|
| 1) pH STANDARD SOLUTION | 00651-06 | CC767907 | 4880-13836406 | 29-Dec-24 |
| 2) pH STANDARD SOLUTION | 00651-08 | CC765602 | 4881-13757019 | 18-Nov-24 |
| 3) pH STANDARD SOLUTION | 00651-10 | CC767180 | 4882-13813369 | 14-Dec-24 |
| 4) PROCESS CALIBRATOR | CA150 | 91S6079 | 23E1312 | 19-Apr-24 |
| 5) BATH | 260014 | 1247 48074 | 22T9870 | 13-Sep-23 |
| 6) THERMOMETER WITH PROBE | 421504 | 55000379 | 22T9904 | 13-Sep-23 |

- THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
- THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
- THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT

1. DISPLAY UNIT ONLY

SLOPE FACTOR $k = 2.303 RT/F = 59 \text{ mV/pH}$

| mV APPLIED | UUC READING (mV) | CORRECTION (mV) | UUC READING (pH) | UNCERTAINTY OF MEASUREMENT (± mV) | COVERAGE FACTOR k |
|---------------|---------------------|--------------------|---------------------|---|-------------------------|
| 414.11 | 414.6 | -0.49 | -0.290 | 0.15 | 2.00 |
| 354.95 | 355.4 | -0.45 | 0.741 | 0.15 | 2.00 |
| 295.80 | 296.3 | -0.50 | 1.773 | 0.15 | 2.00 |
| 236.64 | 237.1 | -0.46 | 2.804 | 0.15 | 2.00 |
| 177.48 | 177.9 | -0.42 | 3.835 | 0.15 | 2.00 |
| 118.32 | 118.7 | -0.38 | 4.867 | 0.15 | 2.00 |
| 59.16 | 59.6 | -0.44 | 5.898 | 0.15 | 2.00 |
| 0.00 | 0.4 | -0.40 | 6.930 | 0.15 | 2.00 |
| -59.16 | -58.8 | -0.36 | 7.961 | 0.15 | 2.00 |
| -118.32 | -117.9 | -0.42 | 8.992 | 0.15 | 2.00 |
| -177.48 | -177.1 | -0.38 | 10.024 | 0.15 | 2.00 |
| -236.64 | -236.3 | -0.34 | 11.055 | 0.15 | 2.00 |
| -295.80 | -295.5 | -0.30 | 12.087 | 0.15 | 2.00 |
| -354.95 | -354.6 | -0.35 | 13.118 | 0.15 | 2.00 |
| -414.11 | -413.8 | -0.31 | 14.149 | 0.15 | 2.00 |

END OF CALIBRATION REPORT PAGE 2 OF 3



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 3 OF 3

Calibration Report

RESULT OF CALIBRATION (CONTINUE) :

2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M

| STANDARD pH BUFFER SOLUTION (pH) | UUC READING (pH) | CORRECTION (pH) | VALUE BEFORE ADJUSTMENT | UNCERTAINTY OF MEASUREMENT (\pm pH) | COVERAGE FACTOR k |
|--|---------------------|--------------------|-------------------------------|--|-------------------------|
| 4.006 | 4.006 | 0.000 | 4.015 | 0.012 | 2.00 |
| 7.000 | 7.000 | 0.000 | 6.914 | 0.012 | 2.00 |
| 10.008 | 10.010 | -0.002 | 9.996 | 0.014 | 2.00 |

3. DISPLAY UNIT WITH TEMPERATURE

| STANDARD READING ($^{\circ}$ C) | UUC READING ($^{\circ}$ C) | CORRECTION ($^{\circ}$ C) | VALUE BEFORE ADJUSTMENT | UNCERTAINTY OF MEASUREMENT (\pm $^{\circ}$ C) | COVERAGE FACTOR k |
|--|--------------------------------|-------------------------------|-------------------------------|--|-------------------------|
| 25.005 | 25.0 | 0.005 | --- | 0.0085 | 2.00 |

4. PERCENT SLOPE 100%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 22TW248

Page.: 1 of 2

Certificate of Testing

| | |
|--|--|
| Equipment : | DO Meter |
| Manufacturer : | Eco Sense |
| Model : | DO 200A |
| Serial No. : | JC 06721 |
| ID No. : | B12 |
| Received Date : | 31 October 2022 |
| Test Date : | 02 November 2022 |
| Reference : | 2210-0981WN-1 |
| Submitted by : | S.P.S. Consulting Service Co.,Ltd. 7 Phaholyothin 24, Phaholyothin Road., Jompol, Chatuchak, Bangkok 10900 |
| Laboratory Condition : | Temperature (25 ± 5) °C Humidity (50 ± 20) % |
| Test Procedure : | In - house method : CP-CH9 by Comparison Technique with Azide Modification Method |
| Tested by : | Walalak Sirithean |
| Approved by : |  Approved Signatory |
| <input checked="" type="checkbox"/> Malee Butkruea <input type="checkbox"/> Saithip Meangmai <input type="checkbox"/> Warakorn Lerngagtrakul | |
| Issue Date : | 7 November 2022 |



Cert.No.: 22TW248

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

| <u>Instruments</u> | <u>Serial No.</u> | <u>ID No.</u> | <u>Certificate No.</u> | <u>Due Date</u> |
|--------------------|-------------------|---------------|------------------------|-----------------|
| 1) Burette | - | 130BU10 | 21CG1389 | 25 Mar 2023 |
| 2) Balance | 1126143764 | 140RC004 | 22MM50 | 20 Sep 2023 |

2. Standard Material :-

| <u>Material</u> | <u>Manufacturer</u> | <u>Lot.No.</u> | <u>Assay</u> |
|---------------------------------|---------------------|----------------|--------------|
| Sodium Thiosulfate pentahydrate | Merck | AM1763316 | 100.2% |

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 21D100513

| Titration Method (Azide Modification Method) (mg/L) | DO Meter Reading (mg/L) | Standard Deviation (mg/L) |
|--|--|--------------------------------------|
| 8.12 | 8.12 | 0.0084 |

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

a 1134238

CERT.No.: HS-U017D

Calibration Date : 3 Apr 23
 Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
 Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C
 Avg Water Temp : 20 °C
 Air Pressure : 760.00 mmHg
 Salinity : 0 ppt

Model : YSI 5000
 S/N : 15B100751
 Probe : YSI 5010
 S/N : 22D100097
 ID NO. : -
 Air Temp ref : S/N. E00522
 Barometric ref : S/N. E00522
 Water Temp ref : S/N. 11431
 Technician : Kittipong M.

Calibration Details

| Calibration Point | 100% air sat. (@20 °C, DO = 9.09 mg/l) | (status) | (status) |
|-----------------------|---|----------|----------|
| Measurement 1 (mg/l) | 9.08 | (PASS) | - |
| Measurement 2 (mg/l) | 9.08 | (PASS) | - |
| Measurement 3 (mg/l) | 9.08 | (PASS) | - |
| Measurement 4 (mg/l) | 9.08 | (PASS) | - |
| Measurement 5 (mg/l) | 9.08 | (PASS) | - |
| Measurement 6 (mg/l) | 9.08 | (PASS) | - |
| Measurement 7 (mg/l) | 9.08 | (PASS) | - |
| Measurement 8 (mg/l) | 9.08 | (PASS) | - |
| Measurement 9 (mg/l) | 9.08 | (PASS) | - |
| Measurement 10 (mg/l) | 9.08 | (PASS) | - |

| | | | |
|------------------|------|------|---|
| Mean Measurement | 9.08 | mg/l | - |
| Inaccuracy | 0.01 | mg/l | - |

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature

(Kittipong Maekwong)

Laboratory Manager

(Natenapha Pisatkunchon)



CERTIFICATE No : 23M2442

REFERENCE No : 68471-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY : 

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23



CERTIFICATE No : 23M2442

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA 09/61 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23° C \pm 1° C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

| INSTRUMENT | MODEL | SERIAL No | CERTIFICATE No | DUE DATE |
|------------------------|-------|-----------|----------------|-----------|
| 1) STANDARD WEIGHT SET | E2 | QK-I-151 | M2302013S | 02-Feb-25 |
| 2) STANDARD WEIGHT | E2 | 15843 | M2302014S | 02-Feb-25 |

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

| NOMINAL VALUE (g) | BALANCE READING (g) | CORRECTION (g) | UNCERTAINTY (\pm g) |
|-------------------|---------------------|----------------|------------------------|
| 0.0 | 0.0000 | 0.0000 | 0.000058 |
| 0.1 | 0.1000 | 0.0000 | 0.000059 |
| 0.2 | 0.2000 | 0.0000 | 0.000059 |
| 0.5 | 0.5000 | 0.0000 | 0.000060 |
| 1.0 | 1.0000 | 0.0000 | 0.000060 |
| 2.0 | 2.0000 | 0.0000 | 0.000061 |
| 5.0 | 5.0000 | 0.0000 | 0.000063 |
| 10.0 | 10.0000 | 0.0000 | 0.000067 |
| 20.0 | 20.0001 | -0.0001 | 0.000073 |
| 50.0 | 50.0000 | 0.0000 | 0.00011 |
| 100.0 | 100.0001 | -0.0001 | 0.00019 |
| 200.0 | 200.0000 | 0.0000 | 0.00032 |

5. OFF CENTER LOADING ERROR



| POINT | READING (g) |
|--------------------|-------------|
| 1 | 100.0000 |
| 2 | 99.9999 |
| 3 | 99.9998 |
| 4 | 100.0001 |
| 5 | 100.0000 |
| OFF-CENTER LOADING | 0.0002 |

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : METTLER TOLEDO

MODEL : XS105DU

SERIAL No : 1126422905

ID No : BA 05/50


CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY :

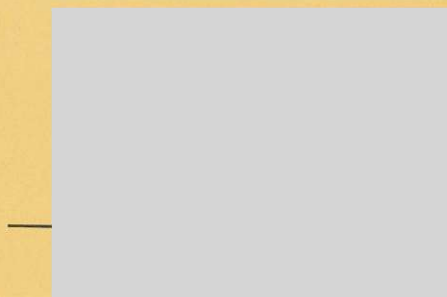

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 23M2441

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 10-Mar-23
AMBIENT TEMPERATURE : 23° C \pm 1° C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

| INSTRUMENT | MODEL | SERIAL No | CERTIFICATE No | DUE DATE |
|------------------------|-------|-----------|----------------|-----------|
| 1) STANDARD WEIGHT SET | E2 | QK-I-151 | M2302013S | 02-Feb-25 |
| 2) STANDARD WEIGHT | E2 | 15843 | M2302014S | 02-Feb-25 |

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

| NOMINAL VALUE (g) | BALANCE READING (g) | CORRECTION (g) | UNCERTAINTY (\pm g) |
|-------------------|---------------------|----------------|------------------------|
| 0.00 | 0.00000 | 0.00000 | 0.000039 |
| 0.02 | 0.02000 | 0.00000 | 0.000039 |
| 0.10 | 0.10000 | 0.00000 | 0.000039 |
| 0.20 | 0.20001 | -0.00001 | 0.000040 |
| 0.50 | 0.50001 | -0.00001 | 0.000040 |
| 1.00 | 1.00000 | 0.00000 | 0.000041 |
| 2.00 | 2.00003 | -0.00003 | 0.000042 |
| 5.00 | 5.00001 | -0.00001 | 0.000046 |
| 10.00 | 10.00003 | -0.00003 | 0.000053 |
| 20.00 | 20.00005 | -0.00005 | 0.000067 |
| 50.00 | 50.00001 | -0.00001 | 0.00011 |
| 100.00 | 100.00001 | -0.00001 | 0.00019 |
| 200.00 | 200.00001 | -0.00001 | 0.00032 |

5. OFF CENTER LOADING ERROR



| POINT | READING (g) |
|--------------------|-------------|
| 1 | 50.0000 |
| 2 | 50.0001 |
| 3 | 50.0000 |
| 4 | 50.0000 |
| 5 | 49.9999 |
| OFF-CENTER LOADING | 0.0001 |

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



MIRACLE INTERNATIONAL TECHNOLOGY CO.,LTD

214 Bangwack Rd. Bangpai Bangkac Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : S2023090437-0003

Date Issued : 28-Sep-23

Customer : S.P.S. CONSULTING SERVICE CO., LTD.
7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,
Bangkok 10900

Equipment : Incubator

Manufacturer : BINDER

Model : BD 115

Serial No. : 12-16967

ID No./Tag No. : IN 05/56

Date Received : 22-Sep-23

Date Calibrated : 22-Sep-23

Calibrated by : Mr. Jame Khaothong

Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by

(Mr. Sarayuth Tochua)



Page 1 of 2

Certificate No. : S2023090437-0003

Environment : Ambient Temperature : Start record 24.3 °C, Stop record 24.5 °C

Relative Humidity : Start record 54.8 %RH, Stop record 54.6 %RH

| Calibration Temperature (°C) | Setting Temperature (°C) | Indicating Temperature (°C) | Measured Stability ¹ (°C) | Measured Uniformity ² (°C) | Overall Variation ³ (°C) |
|------------------------------|--------------------------|-----------------------------|--------------------------------------|---------------------------------------|-------------------------------------|
| 35 | 35.0 | 35.0 | 0.08 | 0.17 | 0.31 |
| 41.5 | 41.5 | 41.5 | 0.04 | 0.18 | 0.25 |

Without adjustment

| Calibration Temperature (°C) | STD No. 1 (°C) | STD No. 2 (°C) | STD No. 3 (°C) | STD No. 4 (°C) | STD No. 5 (°C) | STD No. 6 (°C) | STD No. 7 (°C) | STD No. 8 (°C) | STD No. 9 (°C) | Uncertainty ⁴ ±°C |
|------------------------------|----------------|----------------|----------------|----------------|----------------|----------------|----------------|----------------|----------------|------------------------------|
| 35 | 34.83 | 34.85 | 34.97 | 34.82 | 34.84 | 34.95 | 34.90 | 34.80 | 34.93 | 0.23 |
| 41.5 | 41.36 | 41.38 | 41.46 | 41.32 | 41.28 | 41.48 | 41.40 | 41.33 | 41.44 | 0.23 |


| Calibration Temperature (°C) | MPE (±°C) | Pass / Fail with Guard Band | | | | | | | | |
|------------------------------|-----------|-----------------------------|------------|------------|------------|------------|------------|------------|------------|------------|
| | | No. 1 (°C) | No. 2 (°C) | No. 3 (°C) | No. 4 (°C) | No. 5 (°C) | No. 6 (°C) | No. 7 (°C) | No. 8 (°C) | No. 9 (°C) |
| 35.00 | 0.5 | Pass | Pass | Pass | Pass | Pass | Pass | Pass | Pass | Pass |
| 41.50 | 0.5 | Pass | Pass | Pass | Pass | Pass | Pass | Pass | Pass | Pass |

Pass = $|\text{error}| + |\text{uncertainty}| \leq |\text{MPE}|$

Fail = $|\text{error}| + |\text{uncertainty}| > |\text{MPE}|$

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. 0



Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202306247-001 for Data Acquisition STD-286 Module 1 Serial No. MY44023139, Due 24-Dec-23

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate



CERTIFICATE No : 23T2448

REFERENCE No : 68471-8

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : WATER BATH

MANUFACTURER : MEMMERT

MODEL : WNB29

SERIAL No : L614.0123

ID No : WB 05/58

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 10-Mar-23

APPROVED BY :

ISSUED DATE : 17-Mar-23

RECEIVED DATE : 10-Mar-23



CERTIFICATE No : 23T2448

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : WATER BATH
MANUFACTURER : MEMMERT
ID NUMBER : WB 05/58
RECEIVED DATE : 10-Mar-23
AMBIENT TEMPERATURE : 26 °C ± 1 °C
MODEL : WNB29
SERIAL NUMBER : L614.0123
CALIBRATION DATE : 10-Mar-23
RELATIVE HUMIDITY : 51 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO ASTM E715-80 (REAPPROVED 2001) BY COMPARISON WITH CALIBRATED RTD. THE PROBES WERE PLACED ON FIVE POINTS AND LOCATED ONE PROBE IN EACH OF THE FOUR CORNERS OF THE BATH AND PLACED THE FIFTH RTD WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE WATER VOLUME (REFERENCE LOCATION) UNDER NO LOAD CONDITION.

2. REFERENCE STANDARD INSTRUMENTS :-

| INSTRUMENT | MODEL | SERIAL No | CERTIFICATE No | DUE DATE |
|-------------------------|-------|-----------|----------------|-----------|
| 1) DATA LOGGER WITH RTD | 2625A | 6603614 | 22T7514 | 05-Jul-23 |


3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

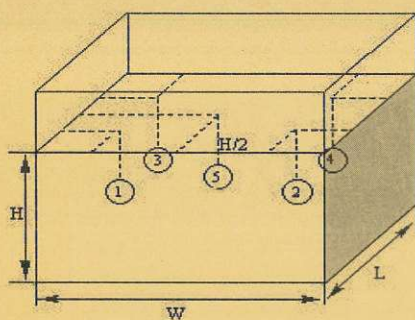

PROBE INSTALLATION
POSITION IN THE BATH

GENERAL INFORMATION

| |
|---|
| Overall Variation of Ambient Temperature around the Bath (°C) : 0.9 |
| Overall Variation of Line Voltage (V) : 0 |
| Instrument Condition : Normal |

BATH PERFORMANCE

| Controller Temperature (°C) | Temperature Stability (±°C) | Radius Uniformity (°C) | Axial Uniformity (°C) | Overall Variation (°C) |
|-----------------------------|-----------------------------|------------------------|-----------------------|------------------------|
| 50.4 | 0.12 | 0.14 | 0.15 | 0.34 |
| 60.4 | 0.18 | 0.23 | 0.19 | 0.50 |

TEMPERATURE MEASUREMENT ACCURACY TEST

| Controller Temp (°C) | Indicating Temp (°C) | Measured Temperature (°C) at Spread Locations | | | | | Uncertainty (± °C) |
|----------------------|----------------------|---|-------|-------|-------|--------|--------------------|
| | | #1 | #2 | #3 | #4 | Ref. 5 | |
| 50.4 | 50.4 | 49.45 | 49.42 | 49.36 | 49.32 | 49.42 | 0.19 |
| 60.4 | 60.4 | 60.17 | 60.20 | 60.06 | 59.97 | 60.18 | 0.25 |

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE BATH.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT