

ภาคผนวก ง.

เอกสารผลการสอบเทียบเครื่องมือตรวจวัด



บริษัท เอ็นไวโรแล็บ จำกัด 540,540/1 ซอยบางนา 7 แขวงบางนาแค เขตบางนา กรุงเทพมหานคร 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-5577-8 Fax: 02-802-5773 E-mail : info@evltesting.com



TSP High Volume Sampler Calibration

Verification Report No.

E6608 -TSP 01

<input checked="" type="checkbox"/> PM <input type="checkbox"/> Onsite	Site: บริษัท เอ็นไวโรแล็บ จำกัด	Date: 1 Aug 23
	UTM: 47P N1514475 E654269	Technical: Sanayu J.
	Sampler: ETSP-30	Approval: Wisan R.
	Recorder: ECRANG15315224	

CONDITIONS

Barometric Press. (hPa): 1008.4
Temperature (deg C): 32.0
Average Press. (hPa): 1013.0
Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 756.4
Temperature (deg K): 305.0
Corrected Avg. Press. (mm Hg): 759.8
Average Temp. (deg K): 303.0


CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc
Model: TE-5028A
Serial#: 1328

Qstd Slope: 1.63957
Qstd Intercept: -0.01202
Date Certified: 19 Jan 2023

CALIBRATIONS

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	13.34	2,204	64.0	63.11	Slope = 28.0271
2	10.62	1,967	56.0	55.22	Intercept = 1.1718
3	8.01	1,710	50.0	49.30	Corr. coeff. = 0.9933
4	5.02	1,355	42.0	41.42	# of Observations: 5
5	3.12	1,070	30.0	29.58	Range of Chart: 33
					at 1.1 - 1.7 m3/min.: 49

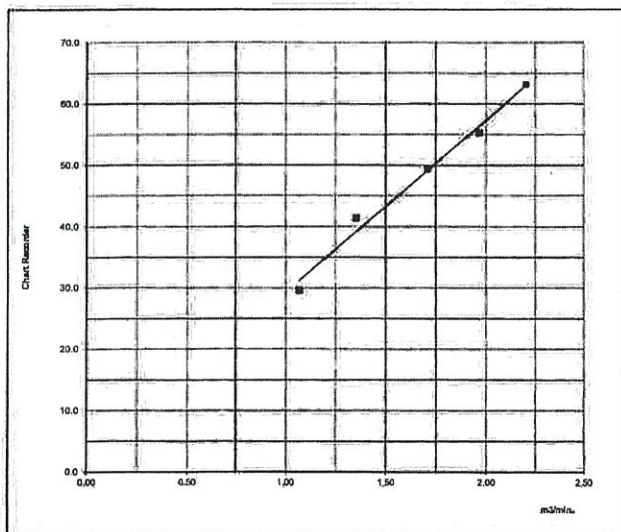

Calibrated by :

(Sanayu Jantason)
1 August 2023

Approved by :

(Wisan Ritthikamon)
1 August 2023

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.

www.evltesting.com

Environmental responsibility with accuracy measurement

FE-MNT-28 Rev.00:01/08/63



รับรองสำเนาถูกต้อง
จัดการฝ่ายควบคุมคุณภาพ



บริษัท เอวิแล็บ จำกัด (มหาชน) 100/100 หมู่ 10 ตำบลบ้านใหม่ อำเภอเมือง จังหวัดเชียงใหม่ 50100
โทรศัพท์ 053-8121111 โทรสาร 053-8121112 อีเมล evl@evl.co.th
เว็บไซต์ www.evtesting.com



TSP High Volume Sampler Calibration

Verification Report No.

E6608 -TSP 02

☐ PM ☐ Onsite

Site: บริษัท เ็นไวแล็บ จำกัด

UTM : 47P N1514475 E654269

Sampler: ETSP-35

Recorder: ECRANG15315224

Date: 1 Aug 23

Technical: Sanayu J.

Approval: Wisan R.

CONDITIONS

Barometric Press. (hPa): 1008.4

Temperature (deg C): 32.0

Average Press. (hPa): 1013.0

Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 756.4

Temperature (deg K): 305.0

Corrected Avg. Press. (mm Hg): 759.8

Average Temp. (deg K): 303.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5028A

Serial#: 1328


Qstd Slope: 1.63957

Qstd Intercept: -0.01202

Date Certified: 19 Jan 2023

CALIBRATIONS

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	LINEAR REGRESSION
1	13.10	2.184	56.0	55.22	Slope = 22.3711
2	10.20	1.928	48.0	47.33	Intercept = 4.8237
3	8.10	1.719	42.0	41.42	Corr. coeff. = 0.9913
4	5.10	1.366	36.0	35.50	# of Observations: 5
5	3.12	1.070	30.0	29.58	Range of Chart 30
					at 1.1 - 1.7 m3/min. 43

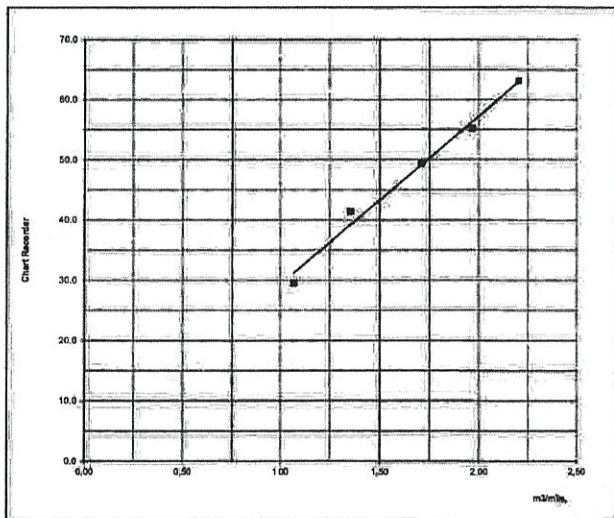

Calibrated by :

(Sanayu Jantason)

1 August 2023

Approved by :

(Wisan Ritthikamon)

1 August 2023

This report shall not be reproduced except in full, without the written approval of Evl Lab Co., Ltd.

www.evtesting.com

Environmental Laboratory with ISO 9001:2015 and ISO 17025:2017

Rev. 001/01/23



รับรองสำเนาถูกต้อง



๒๖ **จัดการป่าเต็งรังเดิมเดิมภาพ**



บริษัท เอ็นไวเลบ จำกัด 540,543/1 ซอยวิภาวดี 7 แขวงวิภาวดี เขตวิภาวดี กรุงเทพมหานคร 10560
EnviLab Co., Ltd. 540,543/1 Soi Bangkhae 7 Bangkok Bangkok Bangkok 10560
Tel : 02-802-3577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



PM10 High Volume Sampler Calibration

Verification Report No.

E6608 -PM 02

☒ PM ☐ Onsite

Site: บริษัท เอ็นไวเลบ จำกัด

UTM : 47P N1514475 E654269

Sampler: EPM-33

Recorder: ECRDS01618124

Date: 1 Aug 23

Technical: Sanayu J.

Approval: Wisan R.

CONDITIONS

Barometric Press. (hPa): 1008.4

Temperature (deg C): 32.0

Average Press. (hPa): 1013.0

Average Temp. (deg C): 30.0

Corrected Pressure (mm Hg): 756.4

Temperature (deg K): 305.0

Corrected Avg.Press. (mm Hg): 759.8

Average Temp. (deg K): 303.0

CALIBRATION ORIFICE

Brand: Tisch Environmental, Inc

Model: TE-5028A

Serial#: 1328


Qstd Slope: 1.02667

Qstd Intercept: -0.00753

Date Certified: 19 Jan 2023

CALIBRATIONS

Plate or Test #	H2O (in)	Qa (m3/min)	J (chart)	IC (corrected)	LINEAR REGRESSION
1	12.50	2.194	50.0	31.75	Slope = 11.1760
2	9.60	1.924	46.0	29.21	Intercept = 7.5147
3	7.40	1.690	42.0	26.67	Corr. coeff. = 0.9990
4	4.52	1.322	35.0	22.23	SFR = 1.143
5	2.80	1.042	30.0	19.05	SSP = 31.94
					# of Observations: 5
					Range of Chart 31
					at SFR $\pm 10\%$ 33

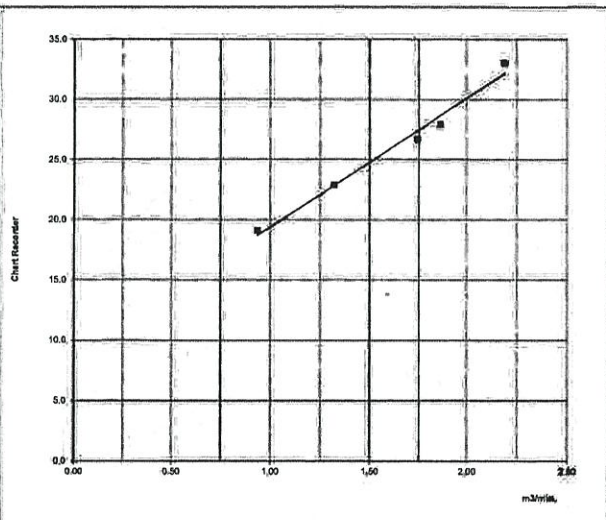

Calibrated by :

(Sanayu Jantason)

1 August 2023

Approved by :

(Wisan Ritthikamon)

1 August 2023

This report shall not be reproduced except in full, without the written approval of EnviLab Co., Ltd.

www.evltesting.com

PM10 Cal; Rev.07 / Iss.Date; Mar 17, 2020

REV-001-28 Rev.0001/04/23



รับรองสำเนาถูกต้อง



neediss

บริษัท นีดีส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.

535 ซอยบางนา 7 แขวงบางนา เขตบางนา กรุงเทพมหานคร 10160 535 Soi Bangnae 7 Bangnae Bangkok Bangkok
Tel. 02-802-3980-2 Fax. 02-802-3983 Email: neediss@neediss.com



SO₂ Analyzer Verification Test Report

Calibration Report No.: 6608008

Page:1/1

Calibrated Date: 2-Aug-23

☒ PM ☐ Onsite

Instruments Information

Analyzer Type: SO2 Analyzer Model: THERMO.,43C	Manufacturer THERMO S/N: ESOTE43C103362
---	--

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO2 Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 26.2 °C

Humidity: 53 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	1.6	1.6	400.0	408	2.0
After	0.0	0.2	0.2	400.0	402	0.5

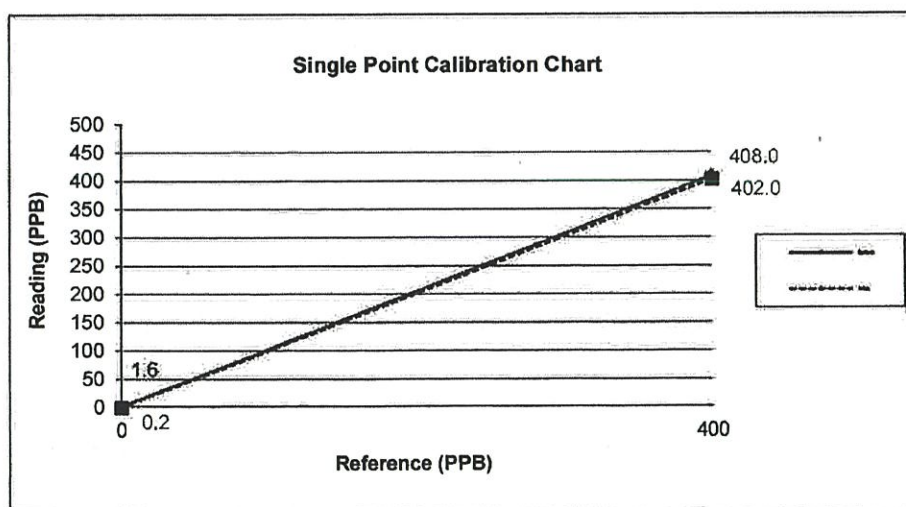

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.



www.neediss.com

We know the best way to save environment



เราช่วยกัน

รับรองสำเนาถูกต้อง

**neediss**บริษัท นีดีส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.535 ซอยบางพลี 7 แขวงบางพลี เขตบางพลี กรุงเทพฯ 10160 535 Soi Bangkhoe 7 Bangkhoe Bangkok
Tel. 02-602-3780-2 Fax. 02-602-3788 E:info@neediss.com

MODEL : SO2 ANALYZER Model 43C THERMO

DATE : 2-08-2023

S/N : ESOTE43C103362

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 (V)	-650	-653
LAMP VOLTAGE 950 - 1,200 (V)	990	985
LAMP INTENSITY 20000 - 50000 Hz	32568	32577
INTER TEMP 15 - 45 DEG C	37	37
CHAMBER TEMP 47 - 51 C	49	49
COOLER TEMP -5 - (-2) DEG C	-2.5	-2.5
PRESSURE 400 - 1000.0 mm Hg	764	765
FLOW 0.350 - 0.650 LPM	0.42	0.4

Calibrate By : Sirir PoonlakApprove By : Sarawat Keawsrinual

Sirirat Poonlak

Sarawat Keawsrinual

Date:

2-Aug-23

Date:

2-Aug-23

neediss

Neediss Supply Instrument Co., Ltd

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

We know the best thing to save environment



รับรองสำเนาถูกต้อง



neediss

บริษัท นีดีส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.

536 ซอย นานา 7 แขวง นานา เขต วังน้อย กรุงเทพมหานคร 10160 536 Soi Bangkok 7 Bangkok Bangkok Bangkok
Tel. 02-802-3980-2 Fax. 02-802-3988 Email: info@neediss.com



SO₂ Analyzer Verification Test Report

Calibration Report No.: 6608007

Page:1/1

Calibrated Date: 2-Aug-23

☒ PM ☐ Onsite

Instruments Information

Analyzer Type: SO2 Analyzer Model: THERMO.,43C	Manufacturer THERMO S/N: ESOTE43C053884
---	--

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO2 Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 26.0 °C

Humidity: 52 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPB)	Reading (PPB)	Drift (PPB)	Reference (PPB)	Reading (PPB)	Drift%
Before	0.0	3.2	0.0	400.0	405	1.3
After	0.0	0.3	0.3	400.0	400	0.0

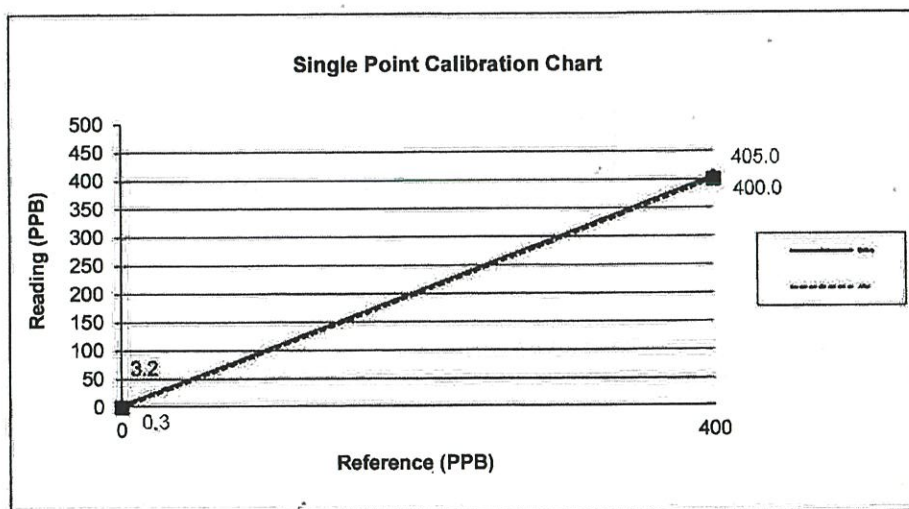

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.



www.neediss.com

We know the best way to save environment



รับรองสำเนาถูกต้อง

มีอายุการใช้งานตามคู่มือการใช้งาน

**neediss**

บริษัท นีดิส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.
536 ซอยพหลโยธิน 7 แขวงพญาไท เขตพญาไท กรุงเทพมหานคร 10160 536 Soi Bangkhai 7 Bangkhai Bangkok Bangkok
Tel. 02-802-3780-2 Fax. 02-802-3785 E-mail: neediss@neediss.com



MODEL : SO2 ANALYZER Model 43C THERMO

DATE : 2-08-2023

S/N : ESOTE43C053884

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 (V)	-650	-653
LAMP VOLTAGE 950 - 1,200 (V)	990	985
LAMP INTENSITY 20000 - 50000.Hz	32568	32577
INTER TEMP 15 - 45 DEG C	37	37
CHAMBER TEMP 47 - 51 C	49	49
COOLER TEMP -5 - (-2) DEG C	-2.5	-2.5
PRESSURE 400 - 1000.0 mm Hg	764	765
FLOW 0.350 - 0.650 LPM	0.42	0.4

Calibrate By : Sirirat PoonlakApprove By : K

Sirirat Poonlak

Sarawat Keawsrinul

Date:

2-Aug-23

Date:

2-Aug-23

neediss

Neediss Supply Instrument Co., Ltd

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

www.neediss.com

We know the best thing to save environment



รับรองสำเนาถูกต้อง

**neediss**บริษัท นีดีส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.536 ซอยบางนา 7 แขวงบางนา เขต บางนา กรุงเทพมหานคร 10160 536 Soi Bangnae 7 Bangnae Bangkok Bangkok
Tel. 02-802-3980-2 Fax. 02-802-3988 Email: neediss.com**NOx Analyzer Verification Test Report**

Calibration Report No.: 6608006

Page:1/2

Calibrated Date: 2-Aug-23

☒ PM ☐ Onsite**Instruments Information**Analyzer Type: NO/NO2/NOx Analyzer
Model: 42CManufacturer THERMO
S/N: ENOTE42CD75279**Calibration System**

Calibrator Unit	Standard Gas
Dilutor Model ESA MGC101	NO Conc 44.68 PPM
S/N: 792	SO2 Conc 45.34 PPM
ZERO AIR Generator ZAG7001	CO Conc 4500 PPM
S/N: 644	Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 26.4 °C


Humidity: 55 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	4.0	0.0	4.0	411	400.0	1.4
NO ₂	2.3	0.0	2.3	4.0	0.0	0.5
NOx	6.3	0.0	6.3	415	400.0	1.8

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.6	0.0	0.6	403	400.0	0.4
NO ₂	0.3	0.0	0.3	2.0	0.0	0.2
NOx	0.9	0.0	0.9	405	400.0	0.6

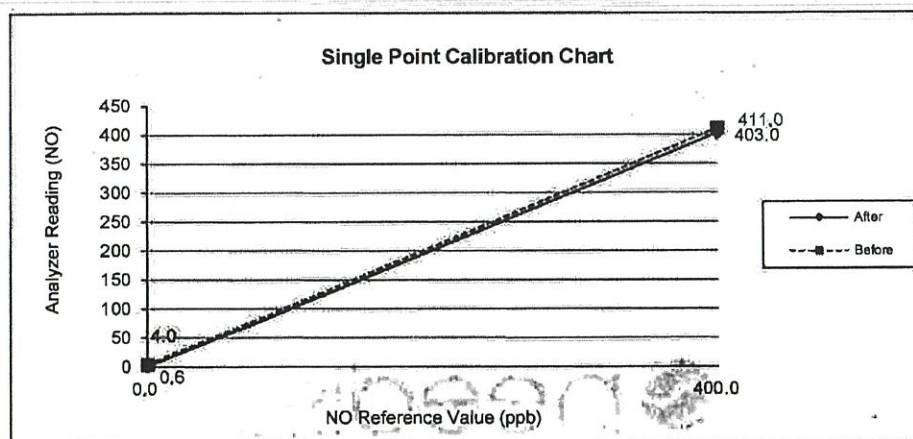

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

สิ่งที่ดีกว่า to save environment

รับรองสำเนาถูกต้อง

**neediss**บริษัท นีดีส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.535 ซอยนาเกลือ 7 แขวงนาเกลือ เขตนาเกลือ กรุงเทพมหานคร 10160 535 Soi Bangkhoe 7 Bangkhoe Bangkok Bangkok
Tel. 02-802-3980-2 Fax. 02-802-3988 E:info@neediss.com

MODEL : NOx ANALYZER Model 42C THERMO

DATE : 2-08-2023

S/N : ENOTE42CD75279

Page:2/2

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 (V)	-675	-678
LAMP VOLTAGE 950 - 1,200 (V)		
INTER TEMP 15 - 45 DEG C	43	43
CHAMBER TEMP 47 - 51 C	49	50
COOLER TEMP -5 - (-2) DEG C	-2	-2
PRESSURE 400 - 1000.0 mm Hg	350	380
SAMPLE FLOW 0.350 - 0.900 LPM	0.45	0.46
OZONEATOR FLOW 0.035 - 0.075 LPM	0.05	0.05
No/Nox BKG	12/9.0	12/9.1
No/Nox Slope	1.0/0.8	0.9/0.8

Calibrate By : Sirir PoonlakApprove By : Sarawat Keawsrinal

Sirirat Poonlak

Sarawat Keawsrinal

Date:

2-Aug-23

Date:

2-Aug-23

**neediss**

Neediss Supply Instrument Co.,Ltd

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

www.neediss.com

Working to save environment

รับรองสำเนาถูกต้อง

**neediss**บริษัท นีดิส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.535 ซอยบางนาแบริด 7 แขวงบางนาแบริด เขตบางนา กรุงเทพมหานคร 10160 535 Soi Bangnae 7 Bangkhuae Bangkok Bangkok
Tel. 02-802-3980-2 Fax. 02-802-3989 Email: neediss.com

NOx Analyzer Verification Test Report

Calibration Report No.: 6608005

Page:1/2

Calibrated Date: 2-Aug-23

☒ PM ☐ Onsite

Instruments Information

Analyzer Type: NO/NO2/NOx Analyzer Model: 42C	Manufacturer THERMO S/N: ENOTE42C789390
--	--

Calibration System

Calibrator Unit	Standard Gas
Difutor Model ESA MGC101 S/N: 792 ZERO AIR Generator ZAG7001 S/N: 644	NO Conc 44.68 PPM SO2 Conc 45.34 PPM CO Conc 4500 PPM Expire Date: Feb 19,2024 EB0140762

Environment: Temperature 26.5 °C


Humidity: 56 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	3.5	0.0	3.5	390	400.0	-1.3
NO ₂	1.9	0.0	1.9	6.0	0.0	0.8
NOx	5.4	0.0	5.4	396	400.0	-0.5

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.3	0.0	0.3	400	400.0	0.0
NO ₂	0.2	0.0	0.2	3.0	0.0	0.4
NOx	0.5	0.0	0.5	403	400.0	0.4

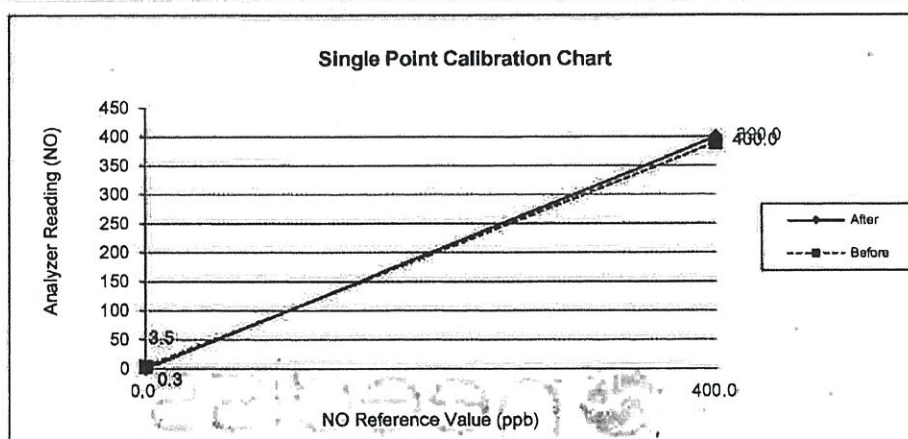

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

Working to save environment.

รับรองสำเนาถูกต้อง

**neediss**บริษัท นีดิส ซัพพลาย อินสตรูเมนต์ จำกัด
Neediss Supply Instrument Co., Ltd.536 ซอยรามคำแหง 7 แขวงรามคำแหง เขตบางนา กรุงเทพมหานคร 10160 536 Soi Bangkhoe 7, Bangkhoe Bangkok Bangkok
Tel. 02-802-3980-2 Fax. 02-802-3988 Email: neediss.com

MODEL : NOx ANALYZER Model 42C THERMO

DATE : 2-08-2023

S/N : ENOTE42C789390

Page:2/2

Test Function Value	Before	After
Range 500 (PPB)	500	500
PMT VOLTS -450 - -850 (V)	-675	-678
LAMP VOLTAGE 950 - 1,200 (V)		
INTER TEMP 15 - 45 DEG C	43	43
CHAMBER TEMP 47 - 51 C	49	50
COOLER TEMP -5 - (-2) DEG C	-2	-2
PRESSURE 400 - 1000.0 mm Hg	350	380
SAMPLE FLOW 0.350 - 0.900 LPM	0.45	0.46
OZONEATOR FLOW 0.035 - 0.075 LPM	0.05	0.05
No/Nox BKG	12/9.0	12/9.1
No/Nox Slope	1.0/0.8	0.9/0.8

Calibrate By : Sirir PoonlakApprove By : Sarawat Keawsrinual

Sirirat Poonlak

Sarawat Keawsrinual

Date:

2-Aug-23

Date:

2-Aug-23



Neediss Supply Instrument Co., Ltd.

This report not be reproduced except in full, without the written approval of Neediss Supply Instrument Co., Ltd.

**www.neediss.com**

thing to save environment

รับรองสำเนาถูกต้อง



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



สงวนลิขสิทธิ์ในเอกสารนี้

Verification Test Report

Report No.:

CONDO -SLM 01

☒ PM ☐ Onsite UTM : 47P N 1514455 E 654248

Calibrated Date: 1 August 2023

Site : บริษัทเอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 45

Serial : 0012

Environment: Temperature 25 °C Humidity 71 %RH

Reference Standard: Acoustic Calibrator Class 1 Model CB011,CESVA

Serial No.T252953

Date of Calibration : 02 December 2022

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.92	93.95	0.03	93.92

Calibrated By:

(Sanayu Jantason)

Date:

1 August 2023

Approve By:

(Wisan Ritthikamon)

Date:

1 August 2023

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.





บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางกะปิ 7 แขวงบางกะปิ เขตบางกะปิ กรุงเทพฯ 10140
Envilab Co., Ltd. 540,540/1 Soi Bangkapi 7 Bangkapi Bangkok Bangkok 10140
Tel: 02-802-3577-8 Fax: 02-802-3773 E-mail: info@evltesting.com



Verification Test Report

Report No.:

CONDO -SLM 02

☐ PM

☐ Onsite UTM:

47P N 1514455 E 654248

Calibrated Date: 1 August 2023

Site : บริษัทเอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 45

Serial : 0013

Environment: Temperature 25 °C Humidity 71 %RH

Reference Standard: Acoustic Calibrator Class 1 Model CB011,CESVA

Serial No.T252953

Date of Calibration : 02 December 2022

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.92	93.97	0.05	93.92

Calibrated By:

(Sanayu Jantason)

Date:

1 August 2023

Approve By:

(Wisan Ritthikamon)

Date:

1 August 2023

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.



Certificate of Calibration

Calibration Certification Information

Cal. Date: January 18, 2023 Rootsmeter S/N: 438320 Ta: 294 °K
 Operator: Jim Tisch Pa: 750.1 mm Hg
 Calibration Model #: TE-5025A Calibrator S/N: 0759

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3960	3.2	2.00
2	3	4	1	0.9950	6.4	4.00
3	5	6	1	0.8850	8.0	5.00
4	7	8	1	0.8450	8.8	5.50
5	9	10	1	0.6990	12.8	8.00

Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)
0.9961	0.7135	1.4145	0.9957	0.7133	0.8854
0.9918	0.9968	2.0004	0.9915	0.9964	1.2521
0.9897	1.1183	2.2365	0.9893	1.1179	1.3999
0.9886	1.1700	2.3456	0.9883	1.1695	1.4683
0.9833	1.4067	2.8289	0.9829	1.4062	1.7708
QSTD	m=	2.03736	QA	m=	1.27576
	b=	-0.03733		b=	-0.02337
	r=	0.99997		r=	0.99997

Calculations

Vstd= $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va= $\Delta Vol((Pa-\Delta P)/Pa)$
Qstd= $Vstd/\Delta Time$	Qa= $Va/\Delta Time$
For subsequent flow rate calculations:	
Qstd= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$

Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH:	calibrator manometer reading (in H2O)
ΔP:	rootsmeter manometer reading (mm Hg)
Ta:	actual absolute temperature (°K)
Pa:	actual barometric pressure (mm Hg)
b:	intercept
m:	slope

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



CAL

Calibratech Co., Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSO-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 66-200035-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance

Manufacturer : Sartorius

Model : SECURA224-1S

Serial No. : 0034803270

ID No. : ELABBALANCEN04

Capacity : 220 g

Resolution : 0.0001 g

Environment : On site calibration was carried out at the Balance Room, Envilab Co., Ltd.

Ambient Temperature : (23.4 to 23.7) °C

Relative Humidity : (61.4 to 62.8) %

Air Pressure : 1011.0 mbar

Date of Received : 02 February 2023

Date of Calibration : 02 February 2023

Date of Issue : 04 February 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14

Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.

Cert. No.

Due Date

Traceability

E261-E2624

C02222345

10 Nov 2023

National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co., Ltd.

CAL-F0031-03



รวมรองสำเนาหลักฐาน

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 66-200035-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.01	0.0001	0.00011
0.1	0.0001	0.00011
1	0.0000	0.00011
2	0.0001	0.00011
5	0.0000	0.00012
10	0.0000	0.00011
20	0.0000	0.00013
50	0.0001	0.00014
100	0.0000	0.00020
200	-0.0001	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.11$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g
A B C D E
-0.0001 0.0001 0.0000 -0.0001 0.0000 g



Repeatability

Load test : 200 g
Stdev. : 0.00000 g

- o o o -



Envilab Co., Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSO-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 66-200035-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : Sartorius **Model :** SECURA3102-1S
Serial No. : 0034409695 **ID No. :** ELABBALANCEN03
Capacity : 3100 g **Resolution :** 0.01 g

Environment : On site calibration was carried out at the Balance Room, Envilab Co., Ltd.
Ambient Temperature : (23.4 to 23.6) °C
Relative Humidity : (59.5 to 61.9) %
Air Pressure : 1011.0 mbar

Date of Received : 02 February 2023

Date of Calibration : 02 February 2023

Date of Issue : 04 February 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
F181-F1821	66-210034-1	30 Jul 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-TR0031-03



รับรองสารเพื่อลูกค้า

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 66-200035-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
10	0.00	0.0082
20	0.00	0.0082
50	0.00	0.0082
100	0.00	0.0082
200	0.00	0.0083
500	0.00	0.0085
1000	0.00	0.0110
1500	0.00	0.012
2000	0.00	0.012
3000	0.00	0.023

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error Load test : 1000 g

A	B	C	D	E	
0.00	-0.01	0.01	0.00	0.00	g



Repeatability Load test : 2000 g

 Sdev. : 0.000 g

- o0o -



Envilab Co., Ltd.

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ





THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0123

MTC No. EEL. BP. 76/1165

CALIBRATION CERTIFICATE

Submitted by : Envilab Co.,Ltd.

Address : 540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae, Bangkok 10160.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Acoustic Calibrator

Manufacturer : CESVA

Model : CB011

Serial No. : T252953

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

- Standards used :
1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
 2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
 3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
 4. Digital Multimeter Agilent 34401A S/N MY44005560.
 5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
 6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.
 7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 28 Nov. 2022

Date of Calibration : 2 Dec. 2022

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : ee@tistr.or.th



รับรองสำเนาถูกต้อง



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0123

MTC No. EEL. BP. 76/1165

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	93.92	-0.08	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	1000.0	0.0	± 1.5	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	1.30	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :



(Mr. Weerachai Deechaiyae)

Approved by :



Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 2 Dec. 2022

Date of Issue : 2 Dec. 2022

Ref : 2011265112805100001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : malee@tistr.or.th



รับรองสำเนาถูกต้อง

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD
Part Number: E05NI91E15A0003
Cylinder Number: EB0146406
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12022
Gas Code: CO, CO₂, NO, NO_x, SO₂, BALN

Reference Number: 160-402305646-1
Cylinder Volume: 148.7 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 660
Certification Date: Jan 03, 2022

Expiration Date: Jan 03, 2030

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	12/27/2021, 01/03/2022
CARBON MONOXIDE	100.0 PPM	98.02 PPM	G1	+/- 0.5% NIST Traceable	12/27/2021
NITRIC OXIDE	100.0 PPM	100.1 PPM	G1	+/- 1.0% NIST Traceable	12/27/2021, 01/03/2022
SULFUR DIOXIDE	100.0 PPM	100.2 PPM	G1	+/- 1.0% NIST Traceable	12/27/2021, 01/03/2022
CARBON DIOXIDE	8.000 %	7.962 %	G1	+/- 0.9% NIST Traceable	12/27/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	09010241	KAL004894	98.48 PPM CARBON MONOXIDE/NITROGEN	+/- 0.5%	Oct 16, 2024
NTRM	200610-56	CC733475	98.61 PPM NITRIC OXIDE/NITROGEN	+/- 0.6%	Oct 06, 2026
GMIS	124206889119	CC322885	4.294 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Sep 03, 2024
NTRM	11010419	KAL004813	99.6 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jul 28, 2023
NTRM	08010636	K019200	13.94 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	Jan 30, 2024

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO2	FTIR	Dec 02, 2021
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Dec 09, 2021
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Dec 16, 2021
Nicolet iS50 FTIR AUP2010245 NO2	FTIR	Dec 29, 2021
Nicolet iS50 FTIR AUP2010245 SO2	FTIR	Dec 23, 2021

Triad Data Available Upon Request

NOTES: Gross Weight: 28.1 Kg, Net Weight: 5.1 Kg.

UF-0X5CX



[Signature]
Approved for Release





CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q22080017

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14632/UM14632[EVMINMMATE4632]
CLID. NO. : 252101369
JOB CONTROL NO. : 220809080017

CUSTOMER : ENVILAB CO., LTD.
540, 540/1 SOI BANGKHAE 7, BANGKHAE,
BANGKHAE, BANGKOK 10160 THAILAND

DATE OF RECEIVED : 09 August 2022

DATE OF ISSUED : 23 August 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory
23 August 2022

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22080017A1

F3-012-04/01-12



รับรองสำเนาถูกต้อง

page 1 of 3




@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM14632/UM14632[EVMINMMATE4632]
DATE OF CALIBRATION	:	10 August 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.
The calibration was performed by using Digital Multimeter, High Resolution Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
2. High Resolution Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0112-21, Due Date 26 October 2022.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0001/22, Due Date 22 February 2023.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0009-22, Due Date 22 June 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22080017

F3-011-04/01-12

page 2 of 3



รับรองสำเนาถูกต้อง



@clccalibration



CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel, 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	± (% of rdg.)
10	50 Hz	peak	10.000	10.224	-0.224	2.3
20	50 Hz		20.000	20.477	-0.477	1.8
30	50 Hz		30.000	30.692	-0.692	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 1 of 54

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22080017

F3-011-04/01-12

page 3 of 3



รับรองสำเนาถูกต้อง
รับรองสำเนาถูกต้อง




@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



Supplement to Calibration Certificate No. Q22080016

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VIBRATION METER
MANUFACTURER : INSTANTEL
MODEL / TYPE : 721A2601/721A3301
SERIAL NO. : UM14628/UM14628[EVMINMMATE4628]
CLID. NO. : 252101368
JOB CONTROL NO. : 220809080016

CUSTOMER : ENVILAB CO., LTD.
540, 540/1 SOI BANGKHAE 7, BANGKHAE,
BANGKHAE, BANGKOK 10160 THAILAND

DATE OF RECEIVED : 09 August 2022

DATE OF ISSUED : 23 August 2022

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Suwit Phuanbusabong
Calibration Engineer



Approved By : Mongkol Yotsoontorn
Authorized Signatory
23 August 2022

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q22080016A1

F3-012-04/01-12



รับรองสำเนาถูกต้อง

page 1 of 3




@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION FOR

NOMENCLATURE	:	VIBRATION METER
MANUFACTURER	:	INSTANTEL
MODEL / TYPE	:	721A2601/721A3301
SERIAL NO.	:	UM14628/UM14628[EVMINMMATE4628]
DATE OF CALIBRATION	:	10 August 2022

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPEE-08** based on **ISO 16063-21** as calibration guideline.
The calibration was performed by using Digital Multimeter, High Resolution Programmable Timer/Counter, Accelerometer and Measuring Amplifier which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Digital Multimeter, Hewlett Packard Model 34401A S/N. 3146A75935.
2. High Resolution Programmable Timer/Counter, Philips Model PM6680B S/N. SM607101.
3. Accelerometer with Measuring Amplifier, Bruel & Kjaer Model 8305, 2525 S/N. 397018, 2434988.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. EE-0112-21, Due Date 26 October 2022.
2. The measurements are traceable to International System of Units (SI), through Aeronautical Radio of Thailand Ltd. Certificate No. 07-0001/22, Due Date 22 February 2023.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand) Certificate No. AV-0009-22, Due Date 22 June 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2021)"

Certificate No. Q22080016

F3-011-04/01-12

page 2 of 3



รับรองสำเนาถูกต้อง



@clccalibration



CALIBRATION LABORATORY CO., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

CALIBRATION DATA

VELOCITY RESULT

Test point		Mode	STD Reading	DUC Reading	Correction	Uncertainty
(mm/s)	(frequency)		(mm/s)	(mm/s)	(mm/s)	\pm (% of rdg.)
10	50 Hz	peak	10.000	10.107	-0.107	2.3
20	50 Hz		20.000	20.343	-0.343	1.8
30	50 Hz		30.000	30.581	-0.581	1.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 1 of 54

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q22080016

F3-011-04/01-12

page 3 of 3



รับรองสำเนาถูกต้อง



@clccalibration

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSO-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 66-200066-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : METTLER TOLEDO **Model :** XSR205DU
Serial No. : B911363567 **ID No. :** ELABBALANCEN06
Capacity : 220 g **Resolution :** 0.00001g/81g, 0.0001g/220g

Environment : On site calibration was carried out at the B304 Balance Room, Envilab Co., Ltd.
Ambient Temperature : (24.6 to 24.9) °C
Relative Humidity : (57.0 to 67.8) %
Air Pressure : 1015.0 mbar

Date of Received : 01 March 2023

Date of Calibration : 01 March 2023

Date of Issue : 04 March 2023

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02222345	10 Nov 2023	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0021-03



Envilab Co Ltd

ผู้จัดการฝ่ายควบคุมคุณภาพ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 66-200066-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.1	0.00000	0.000014
0.5	0.00002	0.000022
1	0.00000	0.000026
2	0.00001	0.000034
5	-0.00001	0.000043
10	0.00000	0.000053
50	0.00004	0.00011
100	-0.0001	0.00020
150	-0.0001	0.00038
200	-0.0002	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k =$ 2.07 ,
providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

0.00000 0.00000 0.00001 0.00001 0.00000 g

C	D
E	
B	A

Repeatability

Load test : 200 g

Stdev. : 0.000042 g

- o O o -

Handwritten signature



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 66-410024-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Digital Thermo-Hygrometer
Manufacturer : Jedto Model : HTC-1
Range Temperature : N/A °C Resolution : 0.1 °C
Range Humidity : N/A %R.H. Resolution : 1 %R.H.
Serial No. : PONPE5852094 ID No. : ELABTMHTC10003

Environment : Ambient Temperature : $(23 \pm 2) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$

Date of Received : 08 March 2023
Date of Calibration : 09 March 2023
Date of Issue : 09 March 2023
Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013
by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units
Digital Indicator with Standard Probe Temp&Hum

ID No.	Cert. No.	Due Date	Traceability
400034 & 400036	SG-H-00021/66	11 Jul 2023	Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 66-410024-1

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement

Reference Humidity @ 50 %R.H.

Standard Temperature ($^{\circ}\text{C}$)	UUC Reading ($^{\circ}\text{C}$)	Correction ($^{\circ}\text{C}$)	Uncertainty ($\pm^{\circ}\text{C}$)
25.01	25.0	0.0	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 $^{\circ}\text{C}$

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty ($\pm\%$ R.H.)
50.00	49	1	2.2


Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSO-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 66-420018-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : pH Meter with electrode
pH meter
Manufacturer : Adwa Model : AD 12
Range : -2.00 to 16.00 pH Resolution : 0.01 pH
Serial No. : 11004090402 ID No. : ELABPHADWA1201

Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$

Date of Received : 08 February 2023

Date of Calibration : 13 February 2023

Date of Issue : 13 February 2023

Calibrated by : Bunjerd Masri

Calibration Method : In-house method CAL-M4201 direct measurement by using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61235182	857394	11 Dec 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61267169	857395	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
10.010	61260481	857396	11 Dec 2023	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-00031-03



Envilab Co. Ltd. บริการถ่ายโอนความถูกต้อง

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 66-420018-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (\pm pH)
4, 7	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
7,10	6.986	7.00	-0.01	0.011
	10.010	10.01	0.00	0.014

Remark

1 UUC : Unit Under Calibration

2 pH meter does not have voltage mode because the plug can not BNC socket

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

B.





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 23TW79

Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : Hanna
Model : HI9146-04
Serial No. : G00007931
ID No. : ELABDOHI914601
Received Date : 17 March 2023
Test Date : 20 March 2023
Reference : 2303-0651DN-1
Submitted by : Envilab Co.,Ltd (Head office)
540, 540/1 Soi Bangkhæ 7,
Bangkhæ, Bangkhæ, Bangkok 10160
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technlque with Azide Modification Method
Tested by : Walalak Sirithean
Approved by : 
Approved Signatory

(/) Malee Butkruea
() Saithip Meangmai
() Warakorn Lernagatrakul

Issue Date : 23 March 2023



B 0310344

รับรองสำเนาถูกต้อง
ผู้จัดการฝ่ายควบคุมคุณภาพ



Cert.No.: 23TW79

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	21CG1389	25 Mar 2023
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: KC1A01TAF

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.14	8.16	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Malu .



รับรองสำเนาถูกต้อง

a 1154259

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSD-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 66-400101-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Air Chamber (Incubator)

Manufacturer : Memmert

Model : IF 75

Range : N/A °C

Resolution : 0.1 °C

Serial No. : D319.0066

ID No. : ELABINCUBATOR2

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (23.0 to 24.5) °C

Relative Humidity : (55 to 60) %

Line Voltage : (224.5 to 226.0) V

Date of Received : 21 February 2023

Date of Calibration : 21 February 2023

Date of Issue : 21 February 2023

Calibrated by : Bunjerd Masri

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400047

66-400066-2

03 Aug 2023

National Institute of Metrology Thailand (NIMT)

Approved by :

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL/F0031-03



รับรองการปฏิบัติงาน
ด้วยมาตรฐานคุณภาพ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. :66-400101-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

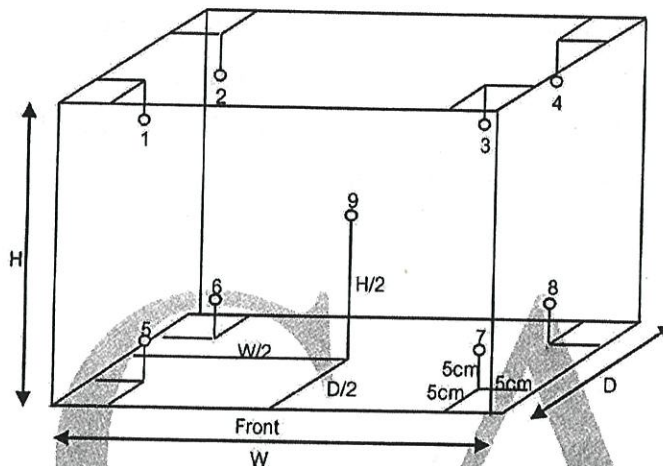

Inside of Chamber

W = 0.40 m

D = 0.56 m

H = 0.33 m

Capacity = 0.07 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.										Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9		
35.0	35.3	35.3	35.00	35.12	35.14	35.10	35.08	35.00	34.89	34.84	35.09	0.30	
37.0	37.3	37.3	36.96	37.11	37.12	37.08	37.06	36.98	36.81	36.81	37.07	0.30	

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
35.0	35.3	35.3	0.28	0.03	0.3
37.0	37.3	37.3	0.29	0.04	0.4

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 65-400577-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Air Chamber (Refrigerator)
Manufacturer : M-LAB Model : BIC-140
Range : N/A °C Resolution : 0.1 °C
Serial No. : 1011 ID No. : ELABBODC140N03

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (22.0 to 23.0) °C

Relative Humidity : (55 to 58) %

Line Voltage : (224.0 to 226.0) V

Date of Received : 11 November 2022

Date of Calibration : 11 November 2022

Date of Issue : 12 November 2022

Calibrated by : Bunjerd Masri


Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400028	65-400522-3	03 Apr 2023	National Institute of Metrology Thailand (NIMT)

Approved by : 
(Bunjerd Masri)
Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



บริษัท แคลบราเทค จำกัด
ผู้ให้บริการด้านความแม่นยำ

CAL

Calibratech Co.,Ltd.

7/106/7 Moo 2, Sukhprachasan 3 Rd., Bangpoo, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 65-400577-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

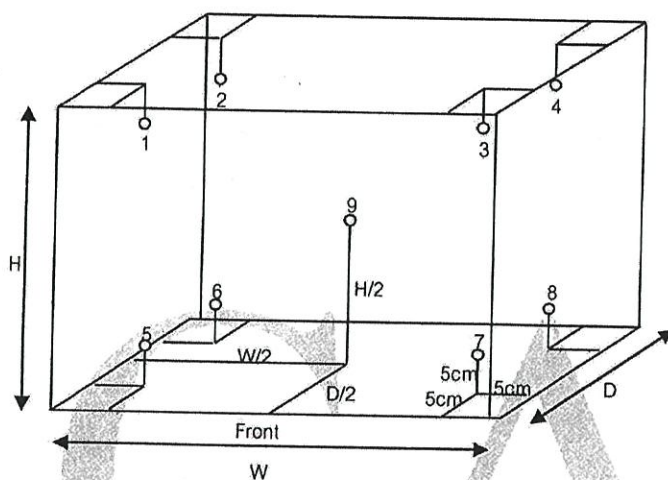

Inside of Chamber

W = 0.38 m

D = 0.35 m

H = 1.15 m

Capacity = 0.15 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
4.0	4.0	4.0	3.9	3.9	4.1	3.5	4.1	4.1	4.1	3.8	4.2	0.56

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
4.0	4.0	4.0	0.7	0.1	0.7

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

B



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120
Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSO-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 66-400156-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Air Chamber (Oven)
Manufacturer : Memmert
Range : N/A °C
Serial No. : B319.0600
Model : UF 75
Resolution : 0.1 °C
ID No. : ELABHAOVEN0600

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (30.0 to 30.8) °C

Relative Humidity : (60 to 65) %

Line Voltage : (224.2 to 225.2) V

Date of Received : 23 March 2023

Date of Calibration : 23 March 2023

Date of Issue : 25 March 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	65-400548-1	26 Apr 2023	National Institute of Metrology Thailand (NIMT)

Approved by :

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd



CAL-000156-2

รับรองมาตรฐานการสอบเทียบ
ตามข้อกำหนดของ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. :66-400156-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

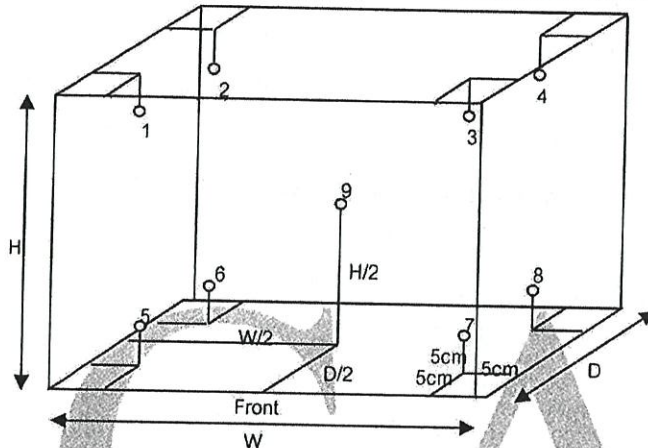

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.56 m

Capacity = 0.07 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	103.5	103.5	104.3	104.3	104.3	104.2	104.3	104.1	103.7	104.0	104.3	0.70
110.0	109.5	109.5	110.3	110.3	110.3	110.3	110.3	110.1	109.7	110.0	110.3	0.71
180.0	179.0	179.0	179.4	180.1	180.3	180.1	180.6	179.9	179.2	179.6	180.4	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	103.5	103.5	0.7	0.1	0.8
110.0	109.5	109.5	0.8	0.1	1.0
180.0	179.0	179.0	1.4	0.2	1.5

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

B



Certificate of Calibration

Certificate No. : 66-400056-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Water Bath

Manufacturer : Memmert

Model : WNB29

Range : N/A °C

Resolution : 0.1 °C

Serial No. : L617.0156

ID No. : ELABWBWNB29N01

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (22.5 to 23.0) °C

Relative Humidity : (45 to 50) %

Line Voltage : (224.0 to 225.0)V

Date of Received : 02 February 2023

Date of Calibration : 02 February 2023


Date of Issue : 04 February 2023

Calibrated by : Permpoon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400031	65-400549-1	22 Apr 2023	National Institute of Metrology Thailand (NIMT)

Approved by : 
(Bunjerd Masri)
Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration


Certificate No. : 66-400056-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

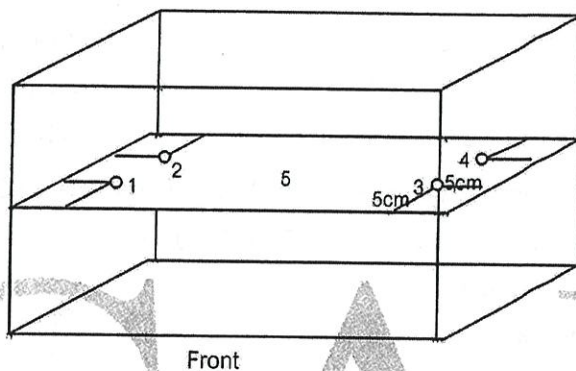

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor					Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)
			No.							
			1	2	3	4	5			
95.0	95.0	95.0	95.41	95.41	95.68	95.62	95.57	0.22	0.33	0.10

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -

B✓



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 66-300140-2

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhao 7, Bangkhao, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 50 ml

Graduation : 1 ml

ID No. : C-WW-003/23

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Air Pressure : 1009.9 mbar.

Date of Received : 15 March 2023

Date of Calibration : 20 March 2023

Date of Issue : 20 March 2023

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-01

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	65-200370-1	02 Jun 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-0003-003



Envilab Co.,Ltd.

ผู้จัดการฝ่ายควบคุมคุณภาพ

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 66-300140-2

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
30	29.98
50	50.12

Uncertainty of measurement with in \pm 0.054 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- oOo -

D.

