

ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือที่ใช้ในการตรวจวิเคราะห์

---

แผนการติดตามตรวจสอบคุณภาพสิ่งแวดล้อม

โครงการโรงไฟฟ้าชีวมวล SPP มิตรผล ไบโอ-เพาเวอร์ 5 บริษัท มิตรผล ไบโอ-เพาเวอร์ (อุเวียง) จำกัด

ระหว่างเดือนมกราคม-มิถุนายน พ.ศ. 2567

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Laboratory Instrument/Equipments.(คุณภาพอากาศ)									
1	Analytical Balance	ฝุ่นละออง (TSP), ฝุ่นทุกขนาด ฝุ่นละอองขนาดเล็กกว่า 10 ไมครอน (Readability 0.1 mg)	Mettler-Toledo	MS204TS/00  C252436235	National Food Institute,  Ministry of Industry, Thailand	2402420-003-01	19 Apr 24	18 Apr 25	-
2	Analytical Balance	ฝุ่นละอองขนาดเล็กกว่า 2.5 ไมครอน (PM-2.5) ฝุ่นขนาดที่เข้าถึงและสะสมในถุงลม ปอดได้ (Readability 0.001 mg)	Mettler-Toledo	XP6 /  B322373893	National Food Institute,  Ministry of Industry, Thailand	2402420-002-01	19 Apr 24	18 Apr 25	-
Equipment for Water Quality Analysis									
3	pH Meter	ความเป็นกรด-ด่าง อุณหภูมิ	Mettler-Toledo	Seven Easy S20 /  1230525212	DKSH (Thailand) Ltd.	C07240167	9 Apr 24	8 Apr 25	-
4	Conductivity Meter	ความเค็ม ความนำไฟฟ้า	SI Analytics	Lab955 /  16300356	DKSH (Thailand) Ltd.	C24240057	11 Mar 24	10 Mar 25	-
5	Analytical Balance	ของแข็งแขวนลอย ของแข็งละลายทั้งหมด (Readability 0.01 mg)	Mettler-Toledo	XSR205DU /  C210685394	National Food Institute,  Ministry of Industry, Thailand	2402283-002-01	2 Apr 24	1 Apr 25	-
6	Hot Air Oven	ของแข็งทั้งหมด	Memmert	UF55 /  B216.1666	National Food Institute,  Ministry of Industry, Thailand	2400141-001-01	11 Oct 23	10 Oct 24	-
7	Analytical Balance	น้ำมันและไขมัน (Readability 0.1 mg)	Mettler-Toledo	AB-204S/FACT /  1129361010	Technology Promotion Association  (Thailand-Japan)	24MM292	11 May 24	10 May 25	-

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Equipment for Water Quality Analysis									
8	BOD Incubator	บีโอดี	Arco	UC4-1320 / (UAE.WAO.015/2561)	Technology Promotion Association (Thailand-Japan)	24TM303	10 Feb 24	9 Feb 25	-
9	DO Meter		YSI	5100 / 11B101863	Technology Promotion Association (Thailand-Japan)	24TW39	21 Feb 24	20 Feb 25	-
10	COD Reactor (Heating Block)	ซีโอดี	Hanna	HI839800-02 / 6480019101	Hanna Instruments (Thailand) Ltd.	HIT-2413-0434	25 Mar 24	24 Mar 25	-
11	Digestor Unit	ทีเคเอ็น	FOSS TECATOR	DT2520 / 91794469	FOSS South East Asia	9809	8 Feb 24	7 Feb 25	-
12	Distillation Unit (Kjeldahl Method)		FOSS TECATOR	KT200 / 91790524	FOSS South East Asia	9810	9 Feb 24	7 Feb 25	-
13	Atomic Absorption Spectrophotometer (AAS)	ตะกั่ว, สารหนู, ทองแดง, นิกเกิล แคดเมียม, อาร์เซนิก, แมงกานีส อลูมิเนียม, เหล็ก	Agilent Technologies	System ID:G8432A AA240FS / MY13160001	Agilent Technologies (Thailand) Co.,Ltd.	MTC.ACL.No 358/67	11 Mar 24	10 Mar 25	-
14	Inductively Coupled Plasma (ICP)		Agilent Technologies	System ID:G8015A G8015AA / MY18030001	Agilent Technologies (Thailand) Co.,Ltd.	Preventive Maintenance Checklist	13 Nov 23	12 Nov 24	-

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Equipment for Water Quality Analysis									
15	Cold Vapor Atomic Absorption Spectrophotometer (CVAAS)	ปรอท	Nippon Instrument Corporation	RA-4500 / 17780278	Coax Group Corporation Ltd.	Preventive Maintenance Report	11 Jul 23	10 Jul 24	-
16	UV-VIS Spectrophotometer	ฟอสฟอรัสทั้งหมด	Hitachi	U-1900 / 2021-064	DQE Services Co.,Ltd.	SP24-008	16 Jan 24	15 Jan 25	-
17	UV-VIS Spectrophotometer	ไนโตรเจน-ไนโตรเจนซีโอดี		U-2900 / 21E22-009	DQE Services Co.,Ltd.	SP24-001	4 Jan 24	3 Jan 25	-
18	Incubator	โคลิฟอร์มทั้งหมด	Memmert	IPP 260 / V615.0187	Technology Promotion Association (Thailand-Japan)	24TM648	1 Apr 24	31 Mar 25	-
19	Incubator	ฟิเคิลโคลิฟอร์มแบคทีเรีย	Memmert	IPP 260 / V618.0033	Technology Promotion Association (Thailand-Japan)	24TM651	2 Apr 24	1 Apr 25	-
20	Water Bath		Memmert	WNE 14 / L416.0606	Technology Promotion Association (Thailand-Japan)	24TM29	10 Feb 24	8 Feb 25	-
21	Water Bath		Memmert	WNE 14 / L416.0612	Technology Promotion Association (Thailand-Japan)	24TM30	10 Feb 24	8 Feb 25	-
22	Auto Clave		ALP	CL-40L / 807298	National Food Institute, Ministry of Industry, Thailand	2304203-001-01	10 Aug 23	9 Aug 24	-
23	Auto Clave		ALP	CL-40L / 808763	National Food Institute, Ministry of Industry, Thailand	2402281-001-01	2 Apr 24	1 Apr 25	-
24	Analytical Balance		OHAUS	PX623 / C236754745	DKSH (Thailand) Ltd.	C01234158	7 Dec 23	6 Dec 24	-



รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate	Apex Instruments, USA.	XC-572-V 1904011	Envi Equipment Service Co., Ltd.	E23-08066	5 Aug 23	4 Aug 24	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide	Testo	Testo 350 60899617	Entech Industrial Sution Co., Ltd.	G 660614	5 Oct 23	4 Oct 24	-
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Thermo Scientific	G25A 158M	Jiranatee Associates Co., Ltd.	COF-001-66	14 Jul 23	13 Jul 24	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	23P1403	9 May 23	8 May 24	-
3	Air Flow Meter	Particular Matter (PM <sub>2.5</sub> )	Mesa Labs	DeltaCal DC1 158850	Innovative Instrument Co.,Ltd.	23-AFM-187	30 Aug 23	29 Aug 24	-
4	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> ) Particular Matter (PM <sub>2.5</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23P1857	2 Jun 23	1 Jun 24	-
5	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> ) Particular Matter (PM <sub>2.5</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23H1200	6 Jun 23	5 Jun 24	-

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Ambient									
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM08130002	UAE Consultant Co.,Ltd.	01112023	1 Nov 23	31 Oct 24	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050148	UAE Consultant Co.,Ltd.	13112023	13 Nov 23	12 Nov 24	-
8	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050149	UAE Consultant Co.,Ltd.	01112023	1 Nov 23	31 Oct 24	-
9	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050150	UAE Consultant Co.,Ltd.	01112023	1 Nov 23	31 Oct 24	-
10	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387065	UAE Consultant Co.,Ltd.	03112023	3 Nov 23	2 Nov 24	-
12	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387066	UAE Consultant Co.,Ltd.	03112023	3 Nov 23	2 Nov 24	-
13	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1200906875	UAE Consultant Co.,Ltd.	03112023	3 Nov 23	2 Nov 24	-

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Ambient									
14	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1200906876	UAE Consultant Co.,Ltd.	09112023	9 Nov 23	8 Nov 24	-
15	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
16	Wind Speed/Wind Direction	WS/WD	LSI LASTEM	E-LOG305 20080020	Thai Meteorological Department	284/23	15 Aug 23	14 Aug 24	-
17	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	01dB	CAL31 82795	Innovative Instrument Co.,Ltd.	23-ACT-109	27 Jun 23	26 Jun 24	-
18	Sound Level Meter	L <sub>Aeq</sub> 24 hours, L <sub>Amax</sub> , L <sub>A90</sub> , L <sub>Adn</sub>	Rion, Japan	NL-62 00130357	Innovative Instrument Co.,Ltd.	CP20230291EA	3 Jul 23	2 Jul 24	-
19	Sound Level Meter	L <sub>Aeq</sub> 24 hours, L <sub>Amax</sub> , L <sub>A90</sub> , L <sub>Adn</sub>	Rion, Japan	NL-62 00130359	Sithiporn Associates Co., Ltd.	ACL23182	8 Jun 23	7 Jun 24	-
20	Sound Level Meter	L <sub>Aeq</sub> 24 hours, L <sub>Amax</sub> , L <sub>A90</sub> , L <sub>Adn</sub>	Rion, Japan	NL-62 00391458	Sithiporn Associates Co., Ltd.	ACL24063	18 Jan 24	17 Jan 25	-

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA1G0019	Technology Promotion Association (Thailand-Japan)	23CH1226	27 Sep 23	26 Sep 24	-
2	DO Meter	DO	Horiba	LAQUA-DO210 HE1D0008	Technology Promotion Association (Thailand-Japan)	23TW219	27 Sep 23	26 Sep 24	-
3	Conductivity Meter	Conductivity	Horiba	LAQUA-EC210 HCOJ0020	Technology Promotion Association (Thailand-Japan)	23CH1571	14 Dec 23	13 Dec 24	-

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Workplace									
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Svantek	SV36 107224	Innovative Instrument Co.,Ltd.	23-ACT-117	4 Aug 23	3 Aug 24	-
2	Sound Level Meter	$L_{Aeq\ 8\ hrs}$ $L_{Amax}$	Rion, Japan	NL-42 00558037	Sithiporn Associates Co., Ltd.	ACL23179	8 Jun 23	7 Jun 24	-
3	Sound Level Meter	$L_{Aeq\ 8\ hrs}$ $L_{Amax}$	Rion, Japan	NL-42 00409178	Sithiporn Associates Co., Ltd.	ACL23131	26 Apr 23	25 Apr 24	-
4	Sound Level Meter	$L_{Aeq\ 8\ hrs}$ $L_{Amax}$	Rion, Japan	NL-42 01010781	Sithiporn Associates Co., Ltd.	ACL23147	9 May 23	8 May 24	-
5	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 67627	Innovative Instrument Co.,Ltd.	23-NDM-222	29 Aug 23	28 Aug 24	-
6	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 128363	Innovative Instrument Co.,Ltd.	23-NDM-089	8 May 23	7 May 24	-
7	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 128477	Innovative Instrument Co.,Ltd.	23-NDM-097	9 May 23	8 May 24	-
8	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 67629	Innovative Instrument Co.,Ltd.	23-NDM-190	11 Aug 23	10 Aug 24	-

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Workplace									
9	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 128475	Innovative Instrument Co.,Ltd.	23-NDM-096	9 May 23	8 May 24	-
10	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104 110833	Innovative Instrument Co.,Ltd.	23-NDM-268	27 Oct 23	26 Oct 24	-
11	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104 117696	Innovative Instrument Co.,Ltd.	23-NDM-105	12 May 23	11 May 24	-
12	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 128372	Innovative Instrument Co.,Ltd.	23-NDM-091	9 May 23	8 May 24	-
13	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 128360	Innovative Instrument Co.,Ltd.	23-NDM-088	8 May 23	7 May 24	-
14	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104 117730	Innovative Instrument Co.,Ltd.	23-NDM-106	12 May 23	11 May 24	-
15	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 128477	Innovative Instrument Co.,Ltd.	23-NDM-097	9 May 23	8 May 24	-
16	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104 117688	Innovative Instrument Co.,Ltd.	23-NDM-108	12 May 23	11 May 24	-
17	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104IS 128367	Innovative Instrument Co.,Ltd.	23-NDM-090	8 May 23	7 May 24	-

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Workplace									
18	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104 143225	Innovative Instrument Co.,Ltd.	23-NDM-179	7 Aug 23	6 Aug 24	-
19	Noise Dosimeter	Noise Dosimeter	Svantek	SV 104 143231	Innovative Instrument Co.,Ltd.	23-NDM-185	7 Aug 23	6 Aug 24	-
20	Primary Flow Calibrator	Calibrate personal pump	TSI,Inc	4146 41462327002	Innovative Instrument Co., Ltd.	23-AFM-144	24 Jul 23	23 Jul 24	-
21	Aneroid Barometer	Total Dust Respirable Dust	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23P1859	2 Jun 23	1 Jun 24	-
22	Digital Thermo - Hygrometer	Total Dust Respirable Dust	Digicon	TH-02 395034174	Technology Promotion Association (Thailand-Japan)	23H1102	24 May 23	23 May 24	-
23	Thermal Environment Monitor	Heat Meter	3M	QuesTemp 34 TEH020027	Innovative Instrument Co.,Ltd.	23-TPM-192	3 Apr 23	2 Apr 24	-
24	Thermal Environment Monitor	Heat Meter	TSI QUEST	QuesTemp 32 TPT030008	Innovative Instrument Co.,Ltd.	23-TPM-502	2 Nov 23	1 Nov 24	-
25	Digital Lux Meter	Lux	Extech Instrument, Taiwan	407026 A 056652	Innovative Instrument Co., Ltd.	23-LXM-139	20 Apr 23	19 Apr 24	-

## Calibration Certificate

**Certificate No.:** 2402420-003-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** MS204TS/00  
**Serial No.:** C252436235  
**ID No.:** UAE.AIR.023/2566  
**Order No.:** 2402420  
**Operation No.:** 2402420-003  
**Date of Receipt:** 19 April 2024  
**Date of Calibration:** 19 April 2024

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by** *P. Jaengkarnkit*  
( Miss Preeyaporn Jaengkarnkit )

Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

**Date of Issue:** 23 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2402420-003-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** MS204TS/00

**Resolution:** 0.0001 g

**Serial No.:** C252436235

**ID No.:** UAE.AIR.023/2566

**Capacity:** 220 g

**Date of Calibration:** 19 April 2024

Page 2 of 3

**Environment Condition:** Ambient Temperature: 21.7 ± 1.5 °C Relative Humidity: 65 ± 6.7 %

**Place of Calibration:** Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

**Condition of This Results of Calibration:**

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M2311181S	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M2311182S	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

**Calibration Results:**




**1. Repeatability of Reading:**

Nominal Value ( g )	Standard Deviation of Reading ( g )
100	0.000074
200	0.000074

**2. Off-Center Error:**

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
100.0005	100.0006	100.0003	100.0006	100.0003	100.0005	0.0002

*P. Jaenghaulit*  
23 April 2024

## Calibration Report

**Certificate No.:** 2402420-003-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** MS204TS/00

**Resolution:** 0.0001 g

**Serial No.:** C252436235

**ID No.:** UAE.AIR.023/2566

**Capacity:** 220 g

**Date of Calibration:** 19 April 2024

Page 3 of 3

**Calibration Results:** (Continued)

**Calibration Range:** 0-200 g

**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000094	2.00
0.1	0.10000	0.1000	0.0000	0.000094	2.00
1	0.99998	1.0000	0.0000	0.000097	2.00
5	4.99997	5.0000	0.0000	0.000096	2.00
10	10.00002	10.0000	0.0000	0.00012	2.00
20	20.00003	20.0001	-0.0001	0.00014	2.00
50	49.99998	50.0003	-0.0003	0.00012	2.00
70	70.00000	70.0005	-0.0005	0.00017	2.00
100	99.99997	100.0006	-0.0006	0.00017	2.00
150	149.99994	150.0012	-0.0013	0.00022	2.00
200	200.00001	200.0015	-0.0015	0.00028	2.00

*P. Jaengbanchit*  
23 April 2024

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Certificate

**Certificate No.:** 2402420-002-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** XP6  
**Serial No.:** B322373893  
**ID No.:** UAE.AIR.019/2556  
**Order No.:** 2402420  
**Operation No.:** 2402420-002  
**Date of Receipt:** 19 April 2024  
**Date of Calibration:** 19 April 2024

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by**   
( Miss Preeyaporn Jaengkarnkit )

Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

**Date of Issue:** 23 April 2024

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2402420-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XP6

**Resolution:** 0.000001 g

**Serial No.:** B322373893

**ID No.:** UAE.AIR.019/2556

**Capacity:** 6.1 g

**Date of Calibration:** 19 April 2024

Page 2 of 3

**Environment Condition:** Ambient Temperature: 22.6 ± 1.8 °C Relative Humidity: 48 ± 6.0 %

**Place of Calibration:** Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

**Condition of This Results of Calibration:**

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M2311181S	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M2311182S	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

**Calibration Results:**




**1. Repeatability of Reading:**

Nominal Value ( g )	Standard Deviation of Reading ( g )
3	0.00000057
6	0.00000019

**2. Off-Center Error:**

A mass of 2 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
1.999981	1.999983	1.999980	1.999984	1.999983	1.999981	0.000003

F-CS-012 Revision: 01 Date: 20-04-65

P. Jongsakulkit  
23 April 2024

## Calibration Report

**Certificate No.:** 2402420-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XP6

**Resolution:** 0.000001 g

**Serial No.:** B322373893

**ID No.:** UAE.AIR.019/2556

**Capacity:** 6.1 g

**Date of Calibration:** 19 April 2024

Page 3 of 3

**Calibration Results:** (Continued)

**Calibration Range:** 0-6 g

**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.0000000	0.000000	0.000000	0.0000032	2.00
0.01	0.0099970	0.009999	-0.000002	0.0000047	2.00
0.05	0.0500010	0.050003	-0.000002	0.0000048	2.00
0.10	0.1000010	0.100001	0.000000	0.0000069	2.00
0.15	0.1500020	0.150002	0.000000	0.0000083	2.00
0.17	0.1700050	0.170006	-0.000001	0.000012	2.00
0.20	0.1999990	0.200002	-0.000003	0.0000083	2.00
1.50	1.4999750	1.499971	0.000004	0.000027	2.00
3.00	2.9999680	2.999959	0.000009	0.000028	2.00
4.50	4.4999810	4.499967	0.000014	0.000022	2.00
6.00	5.9999490	5.999931	0.000018	0.000032	2.00

*S. Jongsakul*  
23 April 2024

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Certificate

**Certificate No.:** 2302181-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 5

**Equipment:** pH Meter  
**Manufacturer:** METTLER TOLEDO  
**Model:** SevenEasy pH  
**Serial No.:** 1230525212  
**ID No.:** UAE.WAS.003/2553  
**Order No.:** 2302181  
**Operation No.:** 2302181-001  
**Date of Receipt:** 14 March 2023  
**Date of Calibration:** 24 March 2023

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by**   
( Mr.Nuttapol Niyomchart )

Specialist, Division of Calibration Laboratory

**Date of Issue:** 24 March 2023

Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2302181-001-01

**Equipment:**

pH Meter

**Resolution:** 0.01 pH ; 1 mV

**Manufacturer:** METTLER TOLEDO

**Model:** SevenEasy pH

**Serial No.:** 1230525212

**Type:** Bench top

**ID No.:** UAE.WAS.003/2553

**Date of Calibration:** 24 March 2023

Page 2 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute

**Environment Condition:** **Ambient Temperature:** ( 23.4 ± 1.5 ) °C **Relative Humidity:** ( 52 ± 3 ) %

**Condition of Equipment:** Good Condition

**Condition of this Results of Calibration**

1. Calibration Method In house method : W-CC-002 based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

<u>Instruments</u>	<u>Serial / ID No.</u>	<u>Manufacturer</u>	<u>Certificate No.</u>	<u>Due Date</u>
2.1 DC Voltage Calibrator	2709007	Fluke	22E1959	17 June 2023
2.2 Digital Thermometer	2709007	Fluke	CC-650557-01	30 October 2023
2.3 Thermo-Hygro Meter	NFI.BTH003/17	PONPE	TE 650555-01	21 September 2023
<u>Certified Reference Material</u>	<u>Lot. No.</u>	<u>Manufacturer</u>	<u>Ref N</u>	<u>Expire Date</u>
2.4 pH buffer 4.008 (Primary pH buffer Solution)	873608	CPAchem	PH216.L5	16 February 2025
2.5 pH buffer 6.865 (Primary pH buffer Solution)	873609	CPAchem	PH217.L5	16 February 2025
2.6 pH buffer 10.01 (Primary pH buffer Solution)	873611	CPAchem	PH220.L5	16 February 2024
2.7 pH buffer 7.00 (Standard pH buffer Solution)	873612	CPAchem	PH107.L5	16 February 2024

3. This certification is traceable to The International System of Unit (SI Unit)

3.1 Instruments No.2.1	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments No.2.2	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Instruments No.2.3	through	NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.4 Certified Reference Material No. 2.4 to 2.6	traceable to	Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material No.2.7	traceable to	BIM RefN HI-13 LotN 25.05.2022; BIM RefN HI-16 LotN 02.06.2022; BIM RefN HI-13 LotN 25.05.2022; BIM RefN HI-16 LotN 02.06.2022, the Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

*N. Niyadach*

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Report

Certificate No.: 2302181-001-01

Equipment:

pH Meter

Resolution: 0.01 pH ; 1 mV

Manufacturer: METTLER TOLEDO

Model: SevenEasy pH

Serial No.: 1230525212

Type: Bench top

ID No.: UAE.WAS.003/2553

Date of Calibration: 24 March 2023

Page 3 of 5

### Calibration Results:

#### 1. Calibration of pH Meter

( Manual Temperature Compensation at 25 °C )

Nominal pH	DC Voltage Standard ( mV )	Average Indicator Reading		Uncertainty ( ±mV )	Coverage Factor ( k )
		mV	pH		
0	414.120	414	0.00	0.58	2.00
2	295.814	296	2.00	0.58	2.00
4	177.464	178	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.000	0	7.00	0.58	2.00
8	-59.158	-59	8.00	0.58	2.00
10	-177.460	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.117	-414	14.00	0.58	2.00

#### 2. Calibration of pH Meter with Electrode ( Manual Temperature Compensation at 25 °C )

Equipment: pH Electrode

Type: Combined Electrode

Manufacturer: METTLER TOLEDO

Model: InLab Solids

Serial No.: 1156883

ID.No. N/A

Performance of Electrode system (Three-Point Calibration at pH 4, pH 7 and pH 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty ( ± pH )	Coverage Factor ( k )
	pH	mV			
4.008	4.01	187	-	0.0071	2.00
6.865	6.86	22	97.86	0.0075	2.00
10.010	10.01	-160	97.66	0.0086	2.00
6.985	6.99	14	-	0.0093	2.00

F-CS-012 Revision: 01 Date: 20-04-65

*N. Inpudat*





## Calibration Report

**Certificate No.:** 2302181-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

Resolution: 0.1 °C Model: SevenEasy pH

Serial No.: 1230525212 ID No.: UAE.WAS.003/2553

Manufacturer: METTLER TOLEDO

**Date of Calibration:** 24 March 2023

Page 4 of 5

**Location:** Chemical Calibration Laboratory, National Food Institute

**Environment Condition:** Ambient Temperature 25 °C ± 1 °C

Relative Humidity 55 % ± 5 %

### Condition of this results of Calibration:

- Calibration Method : - In house method: W-TE-025 by comparison with standard thermometer.  
- The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.  
- The temperature scale in use at this laboratory is the International Temperature scale of 1990 ( ITS-90 ).

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1521	A85997	TE 660039-01	10-Dec-23	NATIONAL FOOD INSTITUTE
Platinum Resistance Thermometer (PRT)	385	509201			

Support Equipment : - Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good
- Result of Calibration : ☒ Without adjustment ☐ After adjustment

N. mignobert

F-CS-012 Revision: 01 Date: 20-04-65

## Calibration Report

**Certificate No.:** 2302181-001-01

**Equipment:** Digital Thermometer with RTD (pH Meter)

Resolution: 0.1 °C Model: SevenEasy pH

Serial No.: 1230525212 ID No.: UAE.WAS.003/2553

Manufacturer: METTLER TOLEDO

**Date of Calibration:** 24 March 2023

Page 5 of 5

**Calibration point:** 15.0, 25.0 and 30.0 °C

**Calibration result:**

- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.
- Description of probe, model : N/A S/N : N/A
- Dimension of probe : Diameter 3 mm., Length 120 mm.,
- Sheath material : N/A

UUC* Reading (°C)	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.2	14.999	- 0.2	0.12
25.2	24.999	- 0.2	0.12
30.2	29.999	- 0.2	0.12

Note

- UUC\* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

*N. Vinyuth*

F-CS-012 Revision: 01 Date: 20-04-65





# Certificate of Calibration

Equipment:	CONDUCTIVITY METER	Certificate No.:	C24240057		
Model:	Lab 955	Issued Date:	11 March 2024		
Serial No. (or ID.):	16300356	Job No.:	WO-00020309		
Manufacturer:	SI Analytic	Page:	1 of 2		
Electrode Serial No.	16070067	Model :	LF413T	Brand :	SI Analytic
Condition:	In Condition				

**Customer:** United Analyst and Engineering Consultant Company Limited  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangckak, Prakanong, Bangkok 10260 Thailand

**Environment Condition:** Temperature 23 °C ± 2 °C  
Humidity 50 %RH ± 15 %RH

**Calibration Place:** Environment Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260 Thailand

**Calibration By:** Mr. Pongpisut Suebchantha

**Calibration Date:** 11 March 2024

**The Method used:** In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14

**Traceability:** This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 960753, 890591, 890593



(Mr.Pongpisut Suebchantha)

Person in charge



(Mr.Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

**เอกสารไม่ควบคุม**

CAL-FM-C24-09: 12 Sep 2022



**Calibration Results:****Before Adjustment**

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor ( k )	Uncertainty ( ± )
25.000 $\mu\text{S/cm}$	26.7 $\mu\text{S/cm}$	-1.700 $\mu\text{S/cm}$	2.00	0.21 $\mu\text{S/cm}$
1413.0 $\mu\text{S/cm}$	1428 $\mu\text{S/cm}$	-15.0 $\mu\text{S/cm}$	2.00	9.0 $\mu\text{S/cm}$
111.3 mS/cm	108.4 mS/cm	2.9 mS/cm	2.00	0.67 mS/cm

**After Adjustment ; at 1413  $\mu\text{S/cm}$** 

Standard Conductivity Solution	Unit Under Calibration Reading	Correction	Coverage Factor ( k )	Uncertainty ( ± )
25.000 $\mu\text{S/cm}$	25.9 $\mu\text{S/cm}$	-0.900 $\mu\text{S/cm}$	2.00	0.21 $\mu\text{S/cm}$
1413.0 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	0.0 $\mu\text{S/cm}$	2.00	9.0 $\mu\text{S/cm}$
111.3 mS/cm	107.5 mS/cm	3.8 mS/cm	2.00	0.67 mS/cm

**The End of Certificate**

## Calibration Certificate

**Certificate No.:** 2402283-002-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 4

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** XSR205DU  
**Serial No.:** C210685394  
**ID No.:** UAE.WAO.010/2565  
**Order No.:** 2402283  
**Operation No.:** 2402283-002  
**Date of Receipt:** 2 April 2024  
**Date of Calibration:** 2 April 2024

**Calibrated by** Mr.Jerawut Prapawuttipong  
Scientist

**Approved by**



( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 9 April 2024

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2402283-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 220 g

**Date of Calibration:** 2 April 2024

Page 2 of 4

**Environment Condition:** Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 47.5 ± 2.5 %

**Place of Calibration:** Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

**Condition of This Results of Calibration:**

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M2304053S	8 April 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 016/23	Quality Reborn	QR24-0343	9 February 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

**Calibration Results:**




**1. Repeatability of Reading:**

Nominal Value ( g )	Standard Deviation of Reading ( g )
40	0.0000042
80	0.0000052
100	0.000048
200	0.000048

**2. Off-Center Error:**

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
100.0000	100.0001	99.9999	99.9999	100.0001	100.0000	0.0001



F-CS-012 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2402283-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 220 g

**Date of Calibration:** 2 April 2024

Page 3 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 0 - 80 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: 0 - 80 g ; Resolution: 0.00001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.000000	0.00000	0.00000	0.0000086	2.00
0.001	0.001003	0.00101	-0.00001	0.0000089	2.00
0.005	0.005003	0.00500	0.00000	0.0000092	2.00
0.01	0.010003	0.01000	0.00000	0.0000089	2.00
0.05	0.049996	0.05000	0.00000	0.0000096	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50001	0.00001	0.000014	2.00
1	1.000003	1.00002	-0.00002	0.000016	2.00
2	2.000023	2.00001	0.00001	0.000017	2.00
5	5.000017	5.00002	0.00000	0.000020	2.00
10	10.000009	10.00000	0.00001	0.000026	2.00
20	20.000031	20.00000	0.00003	0.000037	2.00
30	30.000040	30.00001	0.00003	0.000050	2.00
50	50.000028	50.00002	0.00001	0.000068	2.00
80	80.000068	80.00002	0.00005	0.00011	2.00

# Calibration Report

**Certificate No.:** 2402283-002-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XSR205DU

**Resolution:** 0.00001 g / 0.0001 g

**Serial No.:** C210685394

**ID No.:** UAE.WAO.010/2565

**Capacity:** 220 g

**Date of Calibration:** 2 April 2024

Page 4 of 4

**Calibration Results:** (Continued)

**Calibration Range:** 81 - 200 g

**Calibration Adjustment:** Internal Calibration

**3. Departure from Nominal Value:** (Range: 81 - 200 g ; Resolution: 0.0001 g )

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor <i>k</i>
90	90.00010	90.0001	0.0000	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00015	2.00
110	110.00007	110.0001	0.0000	0.00016	2.00
120	120.00009	120.0000	0.0001	0.00017	2.00
130	130.00010	130.0000	0.0001	0.00019	2.00
140	140.00014	140.0000	0.0001	0.00020	2.00
150	150.00009	150.0001	0.0000	0.00020	2.00
160	160.00010	160.0001	0.0000	0.00022	2.00
170	170.00012	170.0001	0.0000	0.00023	2.00
200	200.00016	200.0002	0.0000	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

----- End -----



F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Certificate

**Certificate No.:** 2400141-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

**Equipment:** CHAMBER (Hot Air Oven)

**Manufacturer:** MEMMERT

**Model:** UF 55

**Serial No.:** B216.1666

**ID No.:** UAE.WAO.027/2559


**Order No.:** 2400141

**Operation No.:** 2400141-001

**Date of Receipt:** 11 October 2023

**Date of Calibration:** 11 October 2023

**Calibrated by** Mr.Worapob Sooktong  
Scientist

**Approved by**   
( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 16 October 2023

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

## Calibration Report

**Certificate No.:** 2400141-001-01

**Equipment:** CHAMBER (Hot Air Oven)

Model: UF 55 Serial No.: B216.1666

Resolution: 0.1 °C ID No.: UAE.WAO.027/2559

Manufacturer: MEMMERT

**Date of Calibration:** 11 October 2023

Page 2 of 3

**Location:** Laboratory, Floor 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

**Environment Condition:**  
Ambient Temperature ( 28 ± 1 ) °C  
Relative Humidity ( 63 ± 2 ) %  
Line Voltage ( 228 ± 1 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.  
- The temperature scale used was based on ITS - 90.  
- All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016894	TE 660380-01	22 April 2024	NATIONAL FOOD INSTITUTE
	RTD	CH#201-209/ RTD#201-209			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

### UUC Description :

Time of Record 1 Hour 9 Minute At 104.0, 140.0 and 180.0 °C  
Fresh air Damper ☐ Open Position ☐  
☒ Close  
☐ Not Available

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment






# Calibration Report

**Certificate No.:** 2400141-001-01  
**Equipment:** CHAMBER (Hot Air Oven)  
Model: UF 55 Serial No.: B216.1666  
Resolution: 0.1 °C ID No.: UAE.WAO.027/2559  
Manufacturer: MEMMERT


**Date of Calibration:** 11 October 2023

Page 3 of 3

**Calibration point:** 104.0, 140.0 and 180.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	28.2	61.4	227.4
MAX	28.3	65.1	229.3

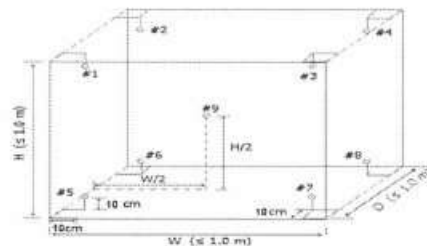

**Table1 : Reporting of Temperature**

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
104.0	104.05	103.98	104.02	104.08	104.00	104.05	103.99	104.17	104.00	0.53
140.0	140.09	139.99	139.91	140.05	139.99	139.91	139.97	140.26	139.97	0.73
180.0	180.46	180.33	180.25	180.28	180.33	179.96	180.31	180.64	180.16	0.90

**Table 2 : Reporting of Characterization Result**

UUC* Setting (°C)	UUC* reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
104.0	104.0	104.0	104.0	0.090	0.18	0.38
140.0	140.0	140.1	140.0	0.075	0.28	0.47
180.0	180.0	180.1	180.0	0.13	0.48	0.88

**Note** The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

----- End -----

*Handwritten signature*





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert.No.: 24MM292

Page.: 1 of 3

**Equipment :** Electronic Balance

**Manufacturer :** Mettler Toledo

**Model :** AB204-S/FACT

**Serial No. :** 1129361010

**ID No. :** UAE.WAS.002/2552

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Balance Room (108)

**Received order :** 11 May 2024

**Calibration Date :** 11 May 2024

**Ambient Temperature :** 15 °C to 40 °C

**Relative Humidity :** 30 % to 90 %

**Calibrated by :** Khit Ruttanaprapachai

**Approved by :**   
Approved Signatory

( ) Ponpan Paipim  
( ) Suwit Imjai  
(✓) Kunchit Promprat

**Issue Date :** 15 May 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2405-0166OC-1  
Procedure used :-

Cert.No.: 24MM292

Page: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14 according to direct measurement method against standard weight.

**Condition of this result of calibration**

1. Reference standard instruments:-

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Test report No.</u>	<u>Due date</u>
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0013-24	25 Jan 2026

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This result of calibration was made on requested at the point specified by customer.

4. This certificate is not certified for any commercial transaction.

5. This certification is traceable to the International System of Unit.

**Result of calibration** ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g Resolution 0.0001 g

Before Adjustment :

<u>Applied Weight</u>	<u>Balance Reading</u>	<u>Correction</u>	<u>Measurement Uncertainty</u>	<u>Coverage Factor</u>
( g )	( g )	( g )	( $\pm$ mg )	( k )
100	100.0000	0.0000	0.19	2.03
200	200.0006	-0.0006	0.30	2

After Adjustment :

1. Determination of the standard deviation of weighing machine ( n = 10 )

<u>Applied Weight</u>	<u>Standard Deviation of Reading ( g )</u>
( g )	
100	0.00007
200	0.00005





Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2405-0166OC-1


Cert.No.: 24MM292

Page: 3 of 3

### Result of calibration

#### 2. Effect of off center loading

A mass of 100 g was placed at various positions on the pan.  
The weighing machine reading error obtained is given in the table

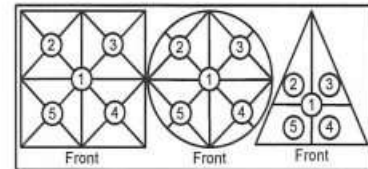

Maximum difference between  
off-center and central loading

Position 1	Position 2	Position 3	Position 4	Position 5
( g )	( g )	( g )	( g )	( g )
-0.0004	-0.0004	-0.0003	-0.0003	-0.0004

( g )  
0.0001

#### 3. Departure from nominal value

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
( g )	( g )	( g )	( $\pm$ mg )	( $k$ )
Unload	0.0000	0.0000	0.15	2.13
0.01	0.0100	0.0000	0.15	2.13
0.05	0.0500	0.0000	0.15	2.13
0.1	0.1000	0.0000	0.15	2.13
0.5	0.5000	0.0000	0.15	2.13
1	1.0000	0.0000	0.15	2.13
10	10.0000	0.0000	0.15	2.11
50	49.9999	+0.0001	0.17	2.06
100	99.9999	+0.0001	0.19	2.03
150	149.9998	+0.0002	0.29	2
200	199.9990	+0.0010	0.30	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 24TM303

Page : 1 of 3

## Certificate of Calibration

**Equipment :** BOD Incubator

**Manufacturer :** Arco

**Model :** UC4-1320

**Serial No. :** 13URC4S013201

**ID No. :** UAE.WAO.015/2561

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Lab Floor 2

**Received Order :** 10 February 2024

**Calibration Date :** 10 February 2024

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Tawatchai Pama

**Approved by :**

  
Approved Signatory

- ( ) Pornthippa Tameyakul  
( ☒ ) Unnopphol Harachai  
( ) Suwit Imjai

**Issue Date :** 19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2402-0234OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Not Available

Cert. No.: 24TM303

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
20.0	20.1	19.9	0.37	0.72	1.4	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.873	19.803	20.322	19.690	19.615	19.585	19.612	19.558	19.645	0.58

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม





Equipment : BOD Incubator  
Condition As-Received : Used Item  
Reference : 2402-0234OC-1

Cert. No.: 24TM303

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY59003411	23LM208	TPA	27 Dec 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available

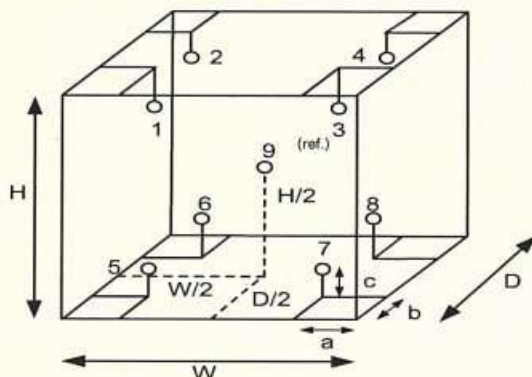

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	28	31
REL.Humid. ( % )	70	65
AC Supply ( Volt )	233	234

Position :	Ref. Std. ID No.:
1	20RTD-2/1
2	20RTD-2/2
3	20RTD-2/3
4	20RTD-2/4
5	20RTD-2/5
6	20RTD-2/6
7	20RTD-2/7
8	20RTD-2/8
9 (ref.)	20RTD-2/9

**Probe Installation Details :**

a = 10 cm  
b = 10 cm  
c = 10 cm

**Dimension of Chamber :**

D = 0.62 m  
W = 1.2 m  
H = 1.2 m  
Capacity = 0.89 m<sup>3</sup>

เอกสารไม่ควบคุม



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 24TW39

**Page.:** 1 of 2

## Certificate of Testing

<b>Equipment :</b>	DO Meter
<b>Manufacturer :</b>	YSI
<b>Model :</b>	5100
<b>Serial No. :</b>	11B 101863
<b>ID No. :</b>	UAE.WAO.004/2554
<b>Received Date :</b>	20 February 2024
<b>Test Date :</b>	21 February 2024
<b>Reference :</b>	2402-0629DSC-1
<b>Submitted by :</b>	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
<b>Laboratory Condition :</b>	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
<b>Test Procedure :</b>	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
<b>Tested by :</b>	Walalak Sirithean
<b>Approved by :</b>	 Approved Signatory
( ) Pornthippa Tameyakul	
( ) Unnopphol Harachai	
(✓) Saithip Meangmai	
<b>Issue Date :</b>	22 February 2024

**เอกสารไม่ควบคุม**



Cert.No.: 24TW39

Page.: 2 of 2

**Condition of this result of calibration**

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 22B100125

<b>Titration Method (Azide Modification Method) (mg/L)</b>	<b>DO Meter Reading (mg/L)</b>	<b>Standard Deviation (mg/L)</b>
8.20	8.19	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study  
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced  
other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม 




Certificate No. : HIT-2413-0434

Page : 1 of 2

**CERTIFICATE OF CALIBRATION**

<b>Equipment :</b>	COD Test Tube Heater		
<b>Meter Model :</b>	HI839800-02	<b>Serial No. :</b>	06480019101
<b>Tube Heater :</b>	25 Vial Capacity	<b>Resolution :</b>	0.1°C
<b>Temperature Range :</b>	(-10 to 160)°C	<b>Temperature of Reaction :</b>	150°C
<b>Manufacturer :</b>	Hanna Instruments	<b>Made in :</b>	Romania
<b>Condition As-Received :</b>	Used Product	<b>Reference :</b>	RE240528
<b>Ambient Temperature :</b>	(25 ± 2)°C	<b>Relative Humidity :</b>	(50 ± 15)%RH
<b>Customer name :</b>	United Analyst and Engineering Consultant Co., Ltd. 3 Soi Udomsuk 41, Sukhumvit Rd., Bangchak, Phrakhanong, Bangkok 10260		
<b>Received date :</b>	25 March 2024		
<b>Calibrate date :</b>	25 March 2024		
<b>Issue date :</b>	27 March 2024		
<b>Calibrated Location :</b>	Hanna Instruments (Thailand) Ltd.		
<b>Calibration Procedure :</b>	This calibrator was conducted by using in-house: calibration procedure CP-04 by using certified reference standard instruments.		

**Calibrated by :** ☒ Mr. Pichit Petthong  
☐ Mr. Channarong Soinak

**Approved by :**   
Mr. Anan Suwanchaisakul  
Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

\*\* This certificate may not be reproduced other than in full, except with the prior written \*\*

approval of the head of Hanna Instrument (Thailand).

เอกสารไม่ควบคุม

**Condition of this calibration result:**

Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Data Acquisition Switch Unit	34970A	MY44065265	WK2307-164-1	WK Electric Co., Ltd.
Digital Thermo-Hygrometer	HT-771SD	AI.07155	24H41	Technology Promotion Association (Thailand-Japan).

**Calibration Result:**

Measurement Temperature Source Accuracy for COD Reactor.

Capacity (Vial)	Nominal Value (°C)	Average Value (°C)	Uncertainty of Measurement (±°C)
25 Vial	150.0	150.0	0.50

Unit : °C

(1A)	(2A)	(3A)	(4A)	(5A)
149.477	149.183	150.029	150.627	149.731
(1B)	(2B)	(3B)	(4B)	(5B)
149.845	150.325	150.275	149.688	150.599
(1C)	(2C)	(3C)	(4C)	(5C)
149.869	150.077	150.571	150.217	150.409
(1D)	(2D)	(3D)	(4D)	(5D)
149.295	150.434	150.347	150.243	150.390
(1E)	(2E)	(3E)	(4E)	(5E)
149.911	149.301	150.232	150.162	149.418

Figure: Shows the location of the temperature source.

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

\*\* End of certificate \*\*

เอกสารไม่ควบคุม

# FOSS

## Customer Service Report

FOSS South East Asia

3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,  
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Report No:

9809

Date:

8 Feb 2024

Customer:

UAE

Address:

Bangkok

Instrument:

DT2520

Serial:

91794469

Hours

Travel To Customer

Start

08:00

Finish

09:30

Labour

14:00

16:00

2hrs

Travel From Customer

16:00

18:00

2hrs

## Job Type

Application		Special		Standard			
Normal	x	Courtesy Visit	x	Installation	x	Training	x
Distributor	x	PMA Onboarding	x	Quote	x	In House	x
Internal	x	Warranty	x	Repair	x	PM	x
Digital Service	x	Sales Support	x	Remote	x	Other	x

PO/Quote Number:

If applicable

PMA Type

FOSScare If applicable

Contract No.

If applicable

## Details of Work / Test

## Condition / Status

# PM DT2520

- ตรวจสอบสายเคเบิล
- ตรวจสอบ connection
- ตรวจสอบ cable kit, temp cut out
- ตรวจสอบ meter
- 300 - 1000 = 10 min
- 300 - 420 = 37 min
- Instrument 4190 meter = 4190

ok done

Instrument Ready for Use

OK

Not OK

If not OK - Comment

Part No:

Batch

Description

Qty

60079652

23.09.2023

Cable kit digester

1

10013554

13.01.2023

Temperature cutout

1

I confirm this report is accurate and complete

Signed FOSS

[Signature]

Signed Customer

[Signature]

Name

Name

Would you be willing to participate in a brief survey in order to tell us how we performed?

Email

เอกสารไม่ควบคุม



# FOSS

## Customer Service Report

FOSS South East Asia

3388 Sirinrat Building, 25th – 26th Floor, Unit No. 3388/90,  
Rama IV Road, Klongton , Klongtoey, Bangkok, Thailand 10110

Report No:

9810

Date:

9 Feb 2024

**Customer:**

UAE

Instrument:

KT 200

**Address:**

BANGKOK

Serial:

91790524

### Hours

### Travel To Customer

## Start

08-AD

### Finish

09350

**Labour**

09:30

12:06

100

Travel From Customer

14.27

16.2

1

Job Type							
Application		Special		Standard			
Normal	x	Courtesy Visit	x	Installation	x	Training	x
Distributor	x	PMA Onboarding	x	Quote	x	In House	x
Internal	x	Warranty	x	Repair	x	PM	x
Digital Service	x	Sales Support	x	Remote	x	Other	x

**PO/Quote Number:**

If applicable

PMA Type

Fosscore

if applicable

Contract No. \_\_\_\_\_

if applicable

Details of Work / Test		Condition / Status
# PM K200		
- 10000725 SOLAH Head - Brassan Janson 3 min 100 ml Alkaline 30 ml - 30 ml - 10000725 PM K200 - 10000725 PM K200		} done
# 10000725 SOLAH Head - Brassan Janson 3 min 100 ml		
10000725 SOLAH Head Composite 1 PC		
Instrument Ready for Use	<input checked="" type="radio"/> OK	
	<input type="radio"/> Not OK	
		If not OK - Comment

Part No:	Batch	Description	Qty
10009965	14.12.2020	Poss PM test kit 200 lejelit Annalysse 2100	1

I confirm this report is accurate and complete

## Signed FOSS

**Signed Customer**

Name \_\_\_\_\_

Name \_\_\_\_\_

*Would you be willing to participate in a brief survey in order to tell us how we performed?*

Email

## เอกสารไม่ควบคุม

Request No. 25-67 / 0275

MTC. ACL.No. 358 / 67

## CALIBRATION CERTIFICATE

**NOMENCLATURE :** 1. Atomic Absorption Spectrophotometer "Agilent Technologies"

Model AA240FS, Serial No. MY13160001

2. Working standard solution "Inorganic Ventures"

Multi Analyte Custom Grade Solution, Lot No. S2-MEB675610

**SUBMITTED BY :** United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

**CALIBRATION PROCEDURE :** 1. Performance Verification of Atomic Absorption Spectrophotometer  
(WI-500-02-30)

2. Estimation Uncertainty of Measurement in Analytical Chemistry (QP-513)

**CALIBRATION RANGE:** 0.02, 0.10, 0.30, 0.50, 0.70 mg/l at 228.8 nm.Cd, 0.10, 0.20, 0.30, 0.50, 0.70 mg/l at 357.9 nm.Cr,  
0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 324.7 nm.Cu, 0.10, 0.30, 0.50, 0.70, 1.00 mg/l at 248.3 nm.Fe,  
0.20, 0.50, 0.70, 1.00, 1.50 mg/l at 217.0 nm.Pb, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 279.5 nm.Mn,  
0.10, 0.30, 0.50, 0.70, 1.00 mg/l at 232.0 nm.Ni, 0.05, 0.10, 0.30, 0.50, 0.70 mg/l at 213.9 nm.Zn

**CALIBRATION DATE :** 2 February 2024

**REFERENCE MATERIAL :** Traceable to NIST "Agilent Technologies", "CARLO ERBA"

Cadmium Lot No. 0006589926, Chromium Lot No. 0112384886, Copper Batch No. T117098A, Iron Batch No. T126087A,  
Lead Lot No. 1227873, Manganese Batch No. T109228A, Nickel Batch No. T270178A, Zinc Batch No. T820140A

**AMBIENT CONDITIONS :** Temperature  $25 \pm 5$  °C Relative humidity  $50 \pm 20$  %

The Atomic Absorption Spectrophotometer has been calibrated against Reference Material traceable to National Institute of Standards and Technology ( NIST ) by The Analytical Chemistry Laboratory. The results are attached herewith.

Calibrated by ..... Atipat .....

( Mr. Atipat Ratana )

Approved by ..... Sulatta .....

(Miss Sutadde Deawtong)

Director of Analytical Chemistry Laboratory

Ref. 2015267020100454001

Issued Date : 11 March 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 8592  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม



# CALIBRATION DATA

## 1. Noise Level

Element	Cd	Cr	Cu	Fe	Pb	Mn	Ni	Zn
Absorbance	0.0006	0.0004	-0.0003	0.0001	-0.0011	-0.0005	0.0008	0.0004
	0.001	0.0017	-0.0009	0.0008	0.0001	0.0002	-0.0003	0.0007
	0.0006	0.0017	-0.0020	0.0005	0.0005	0.0004	0.0013	0.0014
	0.0001	0.0018	-0.0007	0.0005	0.0004	-0.0003	-0.0001	0.0010
	-0.0001	0.0019	-0.0014	0.0003	0.0010	0.0000	0.0002	-0.0001
	0.0011	0.0014	-0.0017	0.0009	-0.0008	0.0004	0.0006	0.0010
	-0.0002	0.0015	-0.0015	0.0003	0.0002	-0.0008	0.0009	0.0013
	0.0006	0.0012	-0.0001	0.0006	0.0008	0.0001	-0.0002	0.0013
	0.0008	0.0009	-0.0003	0.0003	0.0005	0.0002	0.0001	0.0007
	0.0012	0.0011	-0.0012	0.0008	0.0003	0.0004	0.0004	0.0013
	0.0003	0.0015	-0.0019	0.0001	-0.0002	0.0000	-0.0003	0.0003
	0.0005	0.0017	-0.0019	-0.0007	0.0000	-0.0007	0.0005	0.0005
	-0.0006	0.0016	0.0000	0.0006	-0.0001	0.0013	0.0006	0.0010
	0.0003	0.0011	-0.0002	0.0001	-0.0007	0.0009	0.0009	0.0002
	0.0003	0.0012	-0.0011	0.0007	-0.0003	-0.0003	0.0010	0.0009
	0.0004	0.0018	-0.0016	-0.0004	-0.0006	0.0008	0.0007	0.0007
	-0.0001	0.0018	-0.0018	0.0013	-0.0006	-0.0001	0.0014	0.0006
	0.0003	0.0017	-0.0001	0.0001	-0.0012	-0.0004	0.0001	0.0002
	0.0010	0.0018	-0.0007	0.0003	-0.0005	-0.0002	0.001	0.0003
	0.0004	0.0019	-0.0008	-0.0001	-0.0004	0.0003	0.0002	0.0008
Average Absorbance	0.000	0.001	-0.001	0.000	0.000	0.000	0.000	0.001

Continue 2 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2519 8392  
E-mail : sumalee@tistr.or.th


เอกสารไม่ควบคุม

## 2. Precision

Element	Conc. (mg/l)	Absorbance										Ave. Abs.	SD	%RSD
Cd	0.02	0.0078	0.0076	0.0069	0.0075	0.0071	0.0070	0.0076	0.0074	0.0077	0.0067	0.007	0.0004	5.15
	0.30	0.1008	0.1007	0.0999	0.0997	0.1000	0.0996	0.1008	0.1002	0.1005	0.0999	0.100	0.0005	0.46
	0.70	0.2301	0.2306	0.2277	0.2305	0.2310	0.2295	0.2290	0.2293	0.2305	0.2296	0.230	0.0010	0.42
Cr	0.10	0.0094	0.0093	0.0093	0.0098	0.0094	0.0095	0.0090	0.0090	0.0094	0.0090	0.009	0.0003	2.75
	0.30	0.0241	0.0236	0.0221	0.0238	0.0231	0.0226	0.0231	0.0223	0.0230	0.0231	0.023	0.0006	2.75
	0.70	0.0500	0.0500	0.0500	0.0524	0.0499	0.0511	0.0509	0.0512	0.0515	0.0504	0.051	0.0008	1.63
Cu	0.05	0.0061	0.0062	0.0064	0.0061	0.0069	0.0069	0.0061	0.0062	0.0064	0.0061	0.006	0.0003	5.00
	0.30	0.0419	0.0411	0.0402	0.0407	0.0405	0.0404	0.0399	0.0400	0.0399	0.0400	0.040	0.0006	1.58
	0.70	0.0960	0.0960	0.0960	0.0959	0.0947	0.0955	0.0952	0.0952	0.0951	0.0955	0.096	0.0005	0.48
Fe	0.10	0.0096	0.0101	0.0103	0.0100	0.0099	0.0096	0.0106	0.0099	0.0105	0.0102	0.010	0.0003	3.38
	0.50	0.0424	0.0415	0.0428	0.0427	0.0421	0.0426	0.0413	0.0430	0.0421	0.0419	0.042	0.0006	1.33
	1.00	0.0830	0.0839	0.0847	0.0834	0.0832	0.0820	0.0839	0.0838	0.0837	0.0845	0.084	0.0008	0.92
Pb	0.20	0.0078	0.0074	0.0078	0.0078	0.0076	0.0078	0.0077	0.0078	0.0078	0.0077	0.008	0.0001	1.71
	0.70	0.0278	0.0273	0.0271	0.0267	0.0270	0.0264	0.0274	0.0273	0.0269	0.0269	0.027	0.0004	1.45
	1.50	0.0551	0.0548	0.0552	0.0555	0.0547	0.0546	0.0544	0.0544	0.0549	0.0547	0.055	0.0004	0.64
Mn	0.05	0.0116	0.0107	0.0110	0.0103	0.0108	0.0108	0.0112	0.0107	0.0109	0.0108	0.011	0.0003	3.15
	0.30	0.0650	0.0649	0.0649	0.0651	0.0646	0.0646	0.0649	0.0646	0.0640	0.0648	0.065	0.0003	0.48
	0.70	0.1463	0.1465	0.1459	0.1471	0.1475	0.1474	0.1487	0.1473	0.1462	0.1468	0.147	0.0008	0.56
Ni	0.10	0.0095	0.0100	0.0096	0.0103	0.0102	0.0096	0.0100	0.0095	0.0097	0.0096	0.010	0.0003	3.04
	0.50	0.0443	0.0433	0.0438	0.0444	0.0430	0.0437	0.0444	0.0437	0.0438	0.0434	0.044	0.0005	1.09
	1.00	0.0812	0.0820	0.0834	0.0829	0.0818	0.0829	0.0831	0.0835	0.0816	0.0819	0.082	0.0008	0.99
Zn	0.05	0.0374	0.0377	0.0373	0.0377	0.0374	0.0377	0.0373	0.0371	0.0371	0.0374	0.037	0.0002	0.61
	0.30	0.1985	0.1993	0.1975	0.1992	0.1979	0.1988	0.1995	0.1985	0.1974	0.2004	0.199	0.0009	0.47
	0.70	0.4027	0.4031	0.4019	0.4021	0.4023	0.3981	0.4042	0.4025	0.3993	0.3997	0.402	0.0019	0.48

Continue 3 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE



The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

## Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

## Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

## Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม



### 3. Trueness

#### 3.1 Reading on wavelength- Cadmium(Cd) at 228.8 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cd	0.020	0.020	0.000	1.10	± 0.005
	0.301	0.301	0.000	0.11	± 0.005
	0.707	0.693	-0.013	1.85	± 0.008

#### 3.2 Reading on wavelength- Chromium (Cr) at 357.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cr	0.1007	0.104	0.004	3.49	± 0.009
	0.3035	0.297	-0.006	2.11	± 0.012
	0.7071	0.685	-0.023	3.19	± 0.023

#### 3.3 Reading on wavelength- Copper (Cu) at 324.7 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Cu	0.051	0.047	-0.004	7.58	± 0.003
	0.303	0.296	-0.007	2.19	± 0.009
	0.704	0.698	-0.005	0.74	± 0.020

*Sumalee*

Continue 4 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2626 1378 ext. 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

**เอกสารไม่ควบคุม**

Request No. 25-67 / 0275

4 / 5

MTC. ACL. No. 358 / 67

3.4 Reading on wavelength- Iron (Fe) at 248.3 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Fe	0.100	0.104	0.005	4.60	± 0.014
	0.500	0.482	-0.018	3.55	± 0.016
	1.006	0.968	-0.038	3.75	± 0.029

3.5 Reading on wavelength- Lead (Pb) at 217.0 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Pb	0.201	0.202	0.001	0.34	± 0.014
	0.706	0.719	0.012	1.73	± 0.030
	1.513	1.459	-0.054	3.57	± 0.061

3.6 Reading on wavelength- Manganese (Mn) at 279.5 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Mn	0.0505	0.050	0.000	0.83	± 0.005
	0.3031	0.306	0.003	1.12	± 0.007
	0.7023	0.698	-0.004	0.62	± 0.014

*Sumalee*

Continue 5 / 5

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 8592  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

**เอกสารไม่ควบคุม**



Request No. 25-67 / 0275

5 / 5

MTC. ACL. No. 358 / 67

3.7 Reading on wavelength- Nickel (Ni) at 232.0 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Ni	0.101	0.098	-0.003	2.90	± 0.013
	0.508	0.502	-0.006	1.16	± 0.018
	1.012	0.962	-0.051	5.02	± 0.032

3.8 Reading on wavelength- Zinc (Zn) at 213.9 nm.

Element	Standard Value of RM (mg/l)	Reading (mg/l)	Error of Measurement (mg/l)	Error of Measurement (%)	Uncertainty (mg/l)
Zn	0.050	0.045	-0.005	9.39	± 0.013
	0.303	0.324	0.021	7.04	± 0.013
	0.707	0.675	-0.032	4.52	± 0.019

Remark : The reported uncertainty is an expanded uncertainty calculated using a coverage factor of 2 ( $k = 2$ ) which gives a level of confidence of approximately 95%

Calibrated by ..... Atipat .....

(Mr. Atipat Ratana)

Approved by ..... Suladda .....

(Miss Suladda Deawtong)

Director of Analytical Chemistry Laboratory

Issued Date : 11 March 2024

INDUSTRIAL METROLOGY AND TESTING SERVICE CENTRE

End of Certificate

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 8592

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

เอกสารไม่ควบคุม

## Agilent CrossLab Start Up Services

### Agilent 5100 5110 ICP-OES Preventive Maintenance

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.

## Introduction

### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

## Important Customer Web Links

- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit <https://www.agilent.com/en-us/agilentresources>. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>
- **Need to place a service call?** [Flexible Repair Options | Agilent](#)



## Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Service not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Verification section including the customer's and your signature.**

## Instrument Maintenance

### System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5110 VDV ICP-OES
Instrument System Site and Location	UAE

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 8013A	MY 18030001
2.	
3.	
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray <u>OneNeb</u> Conikal   Other
Spray Chamber	Cyclonic Single Pass   <u>Cyclonic Double Pass</u>   Other
Torch	Radial   <u>Dual View</u>   Other
Torch Type	One Piece   <u>Semi Demountable</u>   Fully Demountable   Other
Injector Diameter	2.4mm   <u>1.8mm</u>   1.4mm   0.8mm   Other
Injector Material	<u>Quartz</u>   Ceramic   Other

## Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components and implementation of Service Notes
- ☒ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. *N/A*
- ☒ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

## Preventive Maintenance Procedures

### Record Pre-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table – Pre-PM.

### Clean and inspect ICP-OES system

- ☒ Look for any obvious external damage or problems.
- ☒ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☒ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☒ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- ☒ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☒ Replace the polychromator purge filter.
- ☒ Replace the radial pre-optics window
- ☒ Replace the axial pre-optics window for SVDV and VDV instruments.
- ☒ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☒ Replace air inlet dust filter.
- ☐ Replace high capacity air inlet dust filter element if installed. *N/A*
- ☒ Remove and clean instrument water inlet filter.

### Agilent Water Recirculator

- ☐ **Service not applicable**
- ☒ Drain cooling fluid and remove any particles from the chiller reservoir
- ☒ Remove, clean and reinstall water inlet metal mesh filter if present.
- ☒ Re fill with Agilent Cool Clear cooling fluid.
- ☒ Clean the cooling system Air filter and the condenser.



### SPS 3 Auto Sampler

- ☒ **Service not applicable**
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

### SPS 4 Auto sampler

- ☒ **Service not applicable**
- ☐ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☐ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- ☐ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☐ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☐ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles
- ☐ Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

### AVS 4, 6, 7 Advanced Valve System

- ☒ **Service not applicable**
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks

## ICP-OES adjustment

- ☒ Check position of Zn peak, adjust if required.
- ☒ Check Argon Ratio, adjust to specified value if required.
- ☒ Perform Detector Calibration.
- ☒ Perform Instrument Calibration.

## Record Post-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table - Post PM.
- ☒ For systems using ICP Expert version 7.3 and above, run the following Instrument tests
  - ☒ Subsystem Communications Test
  - ☒ Air Flow
  - ☒ Water Flow
  - ☒ Gas Flows
  - ☒ RF Generator
  - ☒ Camera Test
  - ☒ Optics Test
  - ☒ Nebulizer Test
- ☒ Record the result in the Instrument Test Results Table

## Restore Instrument

- ☐ For HF applications, ask the customer to reinstall their sample introduction system. *N/A*
- ☒ Leave system in an idle state: on and purging.
- ☒ Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

## Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☒ **Complete the Signature Page with both Service Engineer and Customer signatures.**

## Test Results

### Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	4190.3	6849.9	4700.8	7564.2
Mn 257.610 nm SRBR	13681.0	27295.3	14569.1	29992.5
Al 396.152 nm SBR	12.1	14.6	11.5	15.6
K 766.491 nm SBR	8.0	31.2	7.4	39.7

\* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

### Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass



### ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	225.153	VAC	220.613	VAC
Mains Current	0.090	A	0.219	A
Instrument Temperature	24.0	°C	25.1	°C
RF Air Flow (sensor speed)	15.0	Hz	19.0	Hz
Plasma Exhaust Temperature	No measurement		39.2	°C
Water Flow Oscillator	No measurement		1.37	L/min
Water Flow Detector	0.84	L/min	0.81	L/min
Water Inlet Temperature	17.3	°C	17.8	°C
Polychromator Temperature	35.0	°C	35.0	°C
CCD Temperature	-39.8	°C	-39.8	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	659.52	kPa	608.63	kPa
Purge Gas Supply Pressure*1	656.41	kPa	627.71	kPa
Option Gas Supply Pressure*1	-	kPa	-	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		166.30	kPa
Plasma Gas Flow	No measurement		11.98	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1199.5	W
RF Supply Current	No measurement		8.223	A
RF Supply Voltage	No measurement		194.481	V

\*1 If option installed

## Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	-
Purge Gas Filter	G8010-60136	All	1
Air inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	-
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	-
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	-
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	-
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	-
PVC waste tubing, 8mm od x 5mm id, 2m	G8410-80122	SPS 4	-
<b>Additional Parts may be required from engineer's stock:</b>			
X axis drive belt	5410047500	SPS 3	-
Z axis drive belt	5410047400	SPS 3	-
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged,	3710049000	SPS 4	-

## Consumed Parts Reference (Purchased by customer, not included as part of PM)

☐ Section Not Applicable.

Part Description	Part Number	Product or Model# where used	Quantity consumed

## Signature Page

### Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

## Service Verification

Service Request Number:

6006371120

Service Engineer Name:

Kanyakorn S.

Service Engineer Signature:

Kanyakorn S.

Total number of pages in this document:

14

Date Service Completed:

13 Nov 2023

Customer Name:

Aphorn Onkong

Customer Signature:

Aphorn Onkong

### Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Kanyakorn S.
Test Completed On	11/13/2023 9:18:24 AM

### Result Summary

Subsystem Communications Test	Skipped
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Fail
Precision Test	Pass



Resolution Test			Pass
Element Wavelength	Specification	Width	
N (174.213 nm)	≤ 9.40	6.92	
As (188.980 nm)	≤ 8.20	6.12	
C (193.027 nm)	≤ 11.50	8.31	
Mo (202.032 nm)	≤ 8.20	6.35	
Cr (206.158 nm)	≤ 13.40	8.99	
Zn (213.857 nm)	≤ 8.70	6.64	
Pb (220.353 nm)	≤ 9.50	7.06	
Co (228.615 nm)	≤ 17.20	11.68	
Ba (230.424 nm)	≤ 9.40	7.27	
Mn (257.610 nm)	≤ 13.30	9.46	
Mn (260.568 nm)	≤ 20.30	14.18	
Cr (267.716 nm)	≤ 11.00	8.01	
Cu (324.754 nm)	≤ 25.00	18.89	
Cu (327.395 nm)	≤ 14.20	11.29	
Sr (338.071 nm)	≤ 33.50	24.46	
Ba (455.403 nm)	≤ 44.00	33.62	
Sr (460.733 nm)	≤ 36.00	17.37	
Ba (493.408 nm)	≤ 36.00	25.47	
Ba (614.171 nm)	≤ 42.00	25.43	
Ar (675.283 nm)	≤ 74.00	60.50	
K (766.491 nm)	≤ 80.00	65.33	

Sensitivity Test			Fail		
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	142.0	958.5	41.7
Se (196.026 nm)	≥ 41.0	SRBR	105.9	937.4	67.5
Zn (213.857 nm)	≥ 1421.0	SRBR	4190.3	44372.5	111.6
Pb (220.353 nm)	≥ 46.0	SRBR	213.9	2521.3	125.4
Mn (257.610 nm)	≥ 3518.0	SRBR	13681.0	279651.7	416.6
Al (396.152 nm)	≥ 3.4	SBR	12.1	52269.7	3994.3
Ba (493.408 nm)	≥ 34.0	SBR	185.8	2294372.8	12280.0
K (766.491 nm)	≥ 1.8	SBR	8.0	107401.4	11876.7
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	189.4	2285.0	129.5
Se (196.026 nm)	≥ 159.0	SRBR	168.7	2813.7	233.8
Zn (206.200 nm)	≥ 234.0	SRBR	905.0	10158.4	123.0
Zn (213.857 nm)	≥ 1743.0	SRBR	6849.9	135760.6	390.5
Cd (214.439 nm)	≥ 4227.0	SRBR	5597.6	92921.3	273.9
Pb (220.353 nm)	≥ 320.0	SRBR	454.8	10111.2	451.1
Mn (257.610 nm)	≥ 10625.0	SRBR	27295.3	1126118.1	1697.0
Cr (267.716 nm)	≥ 1048.0	SRBR	3948.2	144875.3	1322.0
Cu (324.754 nm)	≥ 19.0	SBR	49.2	341489.7	6798.2
Al (396.152 nm)	≥ 6.0	SBR	14.6	235321.6	15043.9
Ba (493.408 nm)	≥ 60.0	SBR	183.3	8393101.3	45538.3
K (766.491 nm)	≥ 24.0	SBR	31.2	1447045.2	44917.1

**Precision Test****Pass****Radial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 2.60	1.22
Se (196.026 nm)	≤ 2.60	0.76
Zn (213.857 nm)	≤ 1.50	0.33
Pb (220.353 nm)	≤ 2.60	0.86
Mn (257.610 nm)	≤ 1.50	0.45
Al (396.152 nm)	≤ 1.50	0.37
Ba (493.408 nm)	≤ 1.50	0.68
K (766.491 nm)	≤ 1.50	0.33

**Axial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 1.50	0.63
Se (196.026 nm)	≤ 1.50	0.87
Zn (206.200 nm)	≤ 1.50	0.59
Zn (213.857 nm)	≤ 1.50	0.46
Cd (214.439 nm)	≤ 1.50	0.70
Pb (220.353 nm)	≤ 1.50	0.36
Mn (257.610 nm)	≤ 1.50	0.95
Cr (267.716 nm)	≤ 1.50	0.56
Cu (324.754 nm)	≤ 1.50	0.69
Al (396.152 nm)	≤ 1.50	0.63
Ba (493.408 nm)	≤ 1.50	0.86
K (766.491 nm)	≤ 1.50	1.13

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Kanyakorn S.
Test Completed On	11/13/2023 11:10:02 AM

Subsystem Communications Test	Pass
Air Flow Test	Skipped
Water Flow Test	Skipped
Gas Flows Test	Skipped
RF Generator Test	Skipped
Camera Test	Skipped
Optics Test	Pass
Advanced Valve System Test	Skipped
Resolution Test	Pass
Sensitivity Test	Pass
Precision Test	Pass
Subsystem Communications Test	Pass

	Radial	Axial
Intensity	3522064	4003312
Wavelength	737.212	737.212



Resolution Test		Pass
Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.92
As (188.980 nm)	≤ 8.20	6.08
C (193.027 nm)	≤ 11.50	8.33
Mo (202.032 nm)	≤ 8.20	6.31
Cr (206.158 nm)	≤ 13.40	8.98
Zn (213.857 nm)	≤ 8.70	6.73
Pb (220.353 nm)	≤ 9.50	7.02
Co (228.615 nm)	≤ 17.20	11.65
Ba (230.424 nm)	≤ 9.40	7.38
Mn (257.610 nm)	≤ 13.30	9.46
Mn (260.568 nm)	≤ 20.30	14.05
Cr (267.716 nm)	≤ 11.00	7.92
Cu (324.754 nm)	≤ 25.00	18.84
Cu (327.395 nm)	≤ 14.20	11.31
Sr (338.071 nm)	≤ 33.50	24.18
Ba (455.403 nm)	≤ 44.00	33.28
Sr (460.733 nm)	≤ 36.00	17.41
Ba (493.408 nm)	≤ 36.00	25.43
Ba (614.171 nm)	≤ 42.00	25.27
Ar (675.283 nm)	≤ 74.00	56.87
K (766.491 nm)	≤ 80.00	65.88

Sensitivity Test			Pass		
Radial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	168.6	1284.6	53.3
Se (196.026 nm)	≥ 41.0	SRBR	122.4	1256.0	90.7
Zn (213.857 nm)	≥ 1421.0	SRBR	4700.8	53870.1	130.7
Pb (220.353 nm)	≥ 46.0	SRBR	236.0	3100.6	155.7
Mn (257.610 nm)	≥ 3518.0	SRBR	14569.1	318398.1	476.2
Al (396.152 nm)	≥ 3.4	SBR	11.5	59510.5	4761.6
Ba (493.408 nm)	≥ 34.0	SBR	170.6	2490835.6	14514.2
K (766.491 nm)	≥ 1.8	SBR	7.4	117698.7	14024.1
Axial					
Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	214.5	2706.2	142.8
Se (196.026 nm)	≥ 159.0	SRBR	188.0	3262.8	255.9
Zn (206.200 nm)	≥ 234.0	SRBR	1088.2	12794.8	135.3
Zn (213.857 nm)	≥ 1743.0	SRBR	7564.2	156883.9	427.8
Cd (214.439 nm)	≥ 4227.0	SRBR	6647.3	116281.7	304.4
Pb (220.353 nm)	≥ 320.0	SRBR	519.3	12490.2	530.3
Mn (257.610 nm)	≥ 10625.0	SRBR	29992.5	1305852.5	1890.2
Cr (267.716 nm)	≥ 1048.0	SRBR	4366.6	173343.4	1547.9
Cu (324.754 nm)	≥ 19.0	SBR	46.8	361093.0	7560.5
Al (396.152 nm)	≥ 6.0	SBR	15.6	274029.5	16498.6
Ba (493.408 nm)	≥ 60.0	SBR	203.6	9028914.5	44122.1
K (766.491 nm)	≥ 24.0	SBR	39.7	1701521.4	41771.8

**Precision Test****Pass****Radial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 2.60	0.85
Se (196.026 nm)	≤ 2.60	1.26
Zn (213.857 nm)	≤ 1.50	0.42
Pb (220.353 nm)	≤ 2.60	0.54
Mn (257.610 nm)	≤ 1.50	0.60
Al (396.152 nm)	≤ 1.50	0.47
Ba (493.408 nm)	≤ 1.50	0.68
K (766.491 nm)	≤ 1.50	0.50

**Axial**

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 1.50	0.42
Se (196.026 nm)	≤ 1.50	0.66
Zn (206.200 nm)	≤ 1.50	0.42
Zn (213.857 nm)	≤ 1.50	0.54
Cd (214.439 nm)	≤ 1.50	0.42
Pb (220.353 nm)	≤ 1.50	0.22
Mn (257.610 nm)	≤ 1.50	0.54
Cr (267.716 nm)	≤ 1.50	0.49
Cu (324.754 nm)	≤ 1.50	0.85
Al (396.152 nm)	≤ 1.50	0.61
Ba (493.408 nm)	≤ 1.50	0.78
K (766.491 nm)	≤ 1.50	1.00

### Report Summary

Instrument Model	Agilent 5100/5110 VDV ICP-OES
Instrument ID	G8011A/G8015A
Instrument Serial Number	MY18030001
Software Version	7.3.1.9507
Firmware Version	3442
Tested By	Kanyakorn S.
Test Completed On	11/13/2023 11:15:43 AM

### Result Summary

Subsystem Communications Test	Pass
Air Flow Test	Pass
Water Flow Test	Pass
Gas Flows Test	Pass
RF Generator Test	Pass
Camera Test	Pass
Optics Test	Skipped
Advanced Valve System Test	Skipped
Resolution Test	Skipped
Sensitivity Test	Skipped
Precision Test	Skipped

**Subsystem Communications Test** **Pass**

**Air Flow Test** **Pass**

30% Air Flow (relative speed)	75% Air Flow (relative speed)
14.00	20.00

**Water Flow Test** **Pass**

RF Water Flow(L/min)	Camera Water Flow (L/min)	Water Inlet Temperature (°C)
1.27	0.81	20.37



**Gas Flows Test****Pass**

Nebulizer Target Flow	Actual Flow	Back Pressure	Auxiliary Target Flow	Actual Flow	Back Pressure
0.70	0.70	271.62	2.00	2.00	111.13
Makeup Target Flow	Actual Flow	Back Pressure	Plasma Target Flow	Actual Flow	Back Pressure
2.00	2.00	116.00	18.00	17.94	23.11

**RF Generator Test****Pass**

RF Power Supply Test	Passed
RF Power Supply (V)	147.380
RF Oscillator Test	Passed
RF Oscillator Frequency (MHz)	25.843
Work Coil Current (A)	44.410
RF Power Supply Current (A)	1.999

**Camera Test****Pass**

	Integration Time (ms)	Standard Deviation	Status
Electronic Offset Test	1000	5.361	Passed
Dark Current Test	6000	0.779	Passed
Array Test	5	0.025	Passed
Linearity Test		0.118	Passed

UNITED ANALYST AND ENGINEERING CONSULTANT COMPANY Ltd.

Automatic Mercury Analyzer

Model RA-4500


Preventive Maintenance Report


Serial No. : 17780278

Soft version : Ver 2.0.7

ROM version : Ver 2.0.1

Date : 11 July 2023

PM by :   
( Pradit M. )

Approved by :   
( Pathom S. )



**Coax Group Corporation Ltd.**

1131/62,64,325-331 Nakornchaisri road,

Kwang Thanon Nakornchaisri, Dusit, Bangkok 10300 Thailand

Tel. 02-2435263, 02-6682436 Fax. 02-2437386

เอกสารไม่ควบคุม


## Inspection result

ITEM		STANDARD	RESULT	JUDGE
1. Self Check	1.1 Heating		PASS	OK
	1.2 Cooling		PASS	OK
	1.3 Leak		PASS	OK
	1.4 Optical system		PASS	OK
	1.5 Drift		PASS	OK
2. Analytical curve inspection(AREA)				
	2.1 No Pretreatment (Low Conc.)	Correlation coefficient ( r ) $\geq$ 0.9990	1.0000	OK
3. Repeatability(AREA)				
	3.1 No Pretreatment 100ppb, n=5		1. 99.12 ppb 2. 101.48 ppb 3. 101.24 ppb 4. 102.34 ppb 5. 101.92 ppb	
		C.V. $\leq$ 5%	1.23%	OK
4. Blank				
		Below 1.0 (AREA)	0.2062	OK

เอกสารไม่ควบคุม


Title : Preventive Maintenance RA-4500 sn:17780278  
 Date : 7/11/2023  
 Name : Coax Group  
 Memo : Calibration Curve 0-10ng

#### Calib

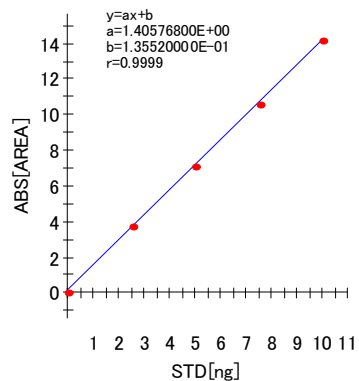

#### STD

No.	STD [ppb]	SVOL [mL]	CVOL [mL]	DVOL [mL]	STD [ng]	AREA [ON]	MEAS [ng]	Dev [%]	Note
1	100.000	0.000	5.000	5.000	0.000	0.0859	-0.0353	-	
2	100.000	0.025	5.000	5.000	2.500	3.7687	2.5845	3.4	
3	100.000	0.050	5.000	5.000	5.000	7.1028	4.9562	0.9	
4	100.000	0.075	5.000	5.000	7.500	10.6441	7.4753	0.3	
5	100.000	0.100	5.000	5.000	10.000	14.2203	10.0193	0.2	

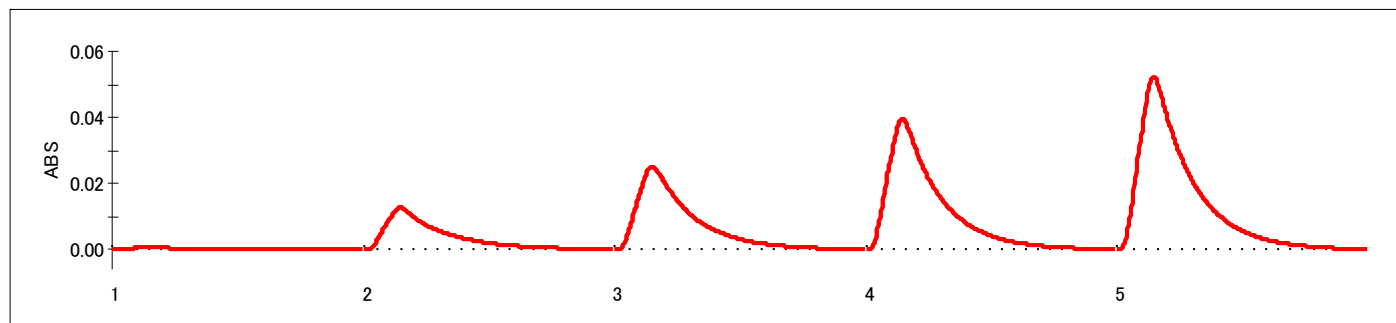

#### SMP


No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	hg 100 ppb	0.050	5.000	5.000	7.1027	4.9561	99.122	
2	hg 100 ppb	0.050	5.000	5.000	7.2687	5.0742	101.484	
3	hg 100 ppb	0.050	5.000	5.000	7.2514	5.0619	101.238	
4	hg 100 ppb	0.050	5.000	5.000	7.3285	5.1168	102.336	
5	hg 100 ppb	0.050	5.000	5.000	7.2996	5.0962	101.924	

#### Statistics

No.	NAME	TRY	AV [ug/L]	SD [ug/L]	Cv [%]
1	hg 100 ppb	5	101.2208	1.246264	1.23

เอกสารไม่ควบคุม



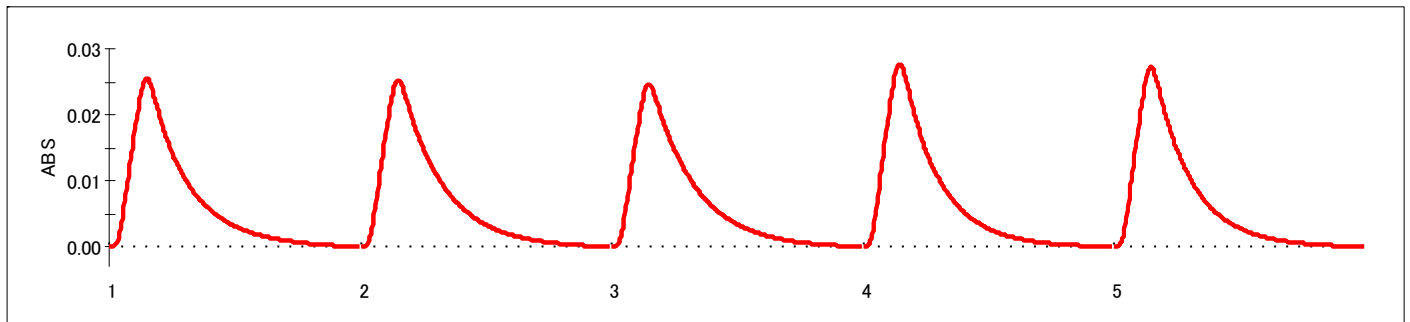

#### Self Check


Heat check:PASS!! ( 24.9degC[05:00] -> 28.9degC[02:31])  
Sensor check:PASS!! ( 78- 18= 60)  
Leak check:PASS!! (0.17L/min)  
Sig/Ref check:PASS!! (Sig:3.73V, Ref:3.94V)  
Drift check:PASS!! (-0.0027882 - -0.0032876 = 0.0004993)

เอกสารไม่ควบคุม

Title : Preventive Maintenance RA-4500 sn:17780278  
Date : 7/11/2023  
Name : Coax Group  
Memo : Blank

SMP

No.	NAME	SVOL [mL]	CVOL [mL]	DVOL [mL]	AREA [ON]	MEAS [ng]	CONC [ug/L]	Note
1	Blank				0.2062	0.0503		

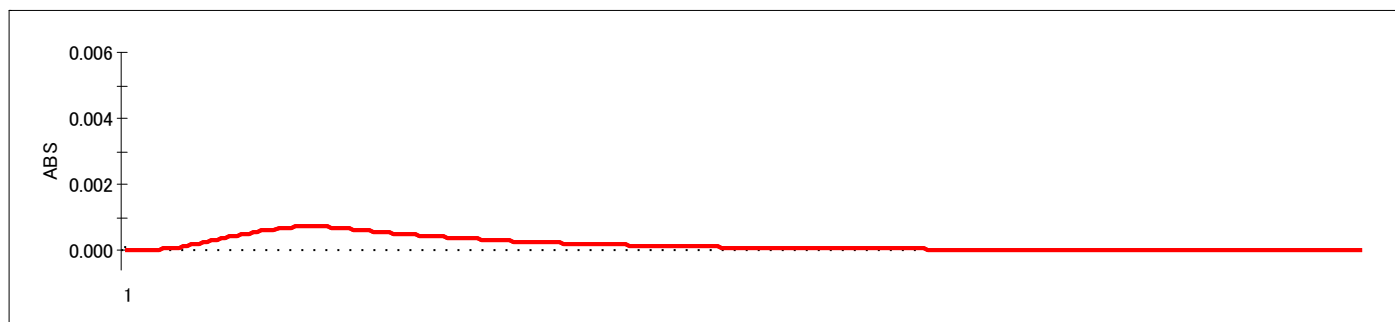

เอกสารไม่ควบคุม

## CERTIFICATE OF CALIBRATION

**Certificate No. :** SP24-008

Page 1 of 5

**Customer :** United Analyst and Engineering Consultant Co.,Ltd. (Head Office)**Address :** 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260**Location of calibration :** Laboratory 315**Equipment :** UV-Vis Spectrophotometer**Manufacturer :** Hitachi**Model :** U-1900**Serial No. :** 2021-064**ID No. :** UAE.WAS.006/2552**Received Date :** 16 January 2024**Calibration Date :** 16 January 2024**Issue Date :** 19 January 2024**Condition Instrument :** Good**Calibrated by :**  
( Mr.Tanawut Rittidach )

Technical Manager

**Approved by :**  
( Ms. Chonthicha Sangngern )

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

## REPORT OF CALIBRATION

**Certificate No. :** SP24-008

Page 2 of 5

**Environment Condition :** Ambient Temperature  $25 \pm 5$  °CRelative humidity  $55 \pm 20$  %RH**Calibration method :** In-house method CP-01 Based on ASTM E275-08**Certified Reference Materials :**

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

**Traceability :** This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Sarna Scientific Limited

**Spectral Band Width of UUC :** 4.0 nm.**Scan Speed of UUC :** 200 nm/min**Scan Interval of UUC :** 0.1 nm.**Resolution of UUC :** Photometric 0.001 Abs.

Wavelength 0.1 nm.



## REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.575	0.0030	0.0031	2.00
	1.0484	1.046	0.0024	0.0029	2.00
	2.1876	2.186	0.0016	0.0080	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0034	2.00
	1.0239	1.024	-0.0001	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.520	0.0030	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.516	0.0021	0.0031	2.00
	1.0002	0.999	0.0012	0.0033	2.00
	1.9973	1.994	0.0033	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.550	0.0017	0.0030	2.00
	1.0803	1.080	0.0003	0.0030	2.00
	2.0373	2.032	0.0053	0.0080	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.558	0.0011	0.0031	2.00
	1.0518	1.051	0.0008	0.0030	2.00
	1.9274	1.923	0.0044	0.0079	2.00

เอกสารไม่ควบคุม

## REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 4 of 5

### Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.748	-0.0011	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.865	0.0024	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.293	-0.0011	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.641	0.0020	0.0055	2.00

## REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 5 of 5

### Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.54	241.1	0.44	0.18	2.00
279.40	278.9	0.50	0.18	2.00
288.70	288.0	0.70	0.18	2.00
334.22	333.8	0.42	0.18	2.00
361.26	360.8	0.46	0.18	2.00
418.48	418.2	0.28	0.18	2.00
446.70	446.0	0.70	0.18	2.00
453.20	453.1	0.10	0.18	2.00
460.06	459.6	0.46	0.18	2.00
536.90	536.4	0.50	0.18	2.00
637.94	637.6	0.34	0.18	2.00
440.74	440.1	0.64	0.18	2.00
472.22	472.0	0.22	0.18	2.00
513.70	513.5	0.20	0.18	2.00
528.72	528.2	0.52	0.18	2.00
574.60	574.3	0.30	0.18	2.00
585.48	585.0	0.48	0.20	2.00
684.63	684.2	0.43	0.18	2.00
740.27	740.0	0.27	0.20	2.00
748.28	747.8	0.48	0.18	2.00
807.16	806.8	0.36	0.18	2.00
879.70	879.2	0.50	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement *U* is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- \* Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม



## CERTIFICATE OF CALIBRATION

**Certificate No. :** SP24-001

Page 1 of 5

**Customer :** United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

**Address :** 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

**Location of calibration :** Laboratory 213

**Equipment :** UV-Vis Spectrophotometer

**Manufacturer :** Hitachi

**Model :** U-2900

**Serial No. :** 21E22-009

**ID No. :** UAE.WAT.051/2564


**Received Date :** 4 January 2024

**Calibration Date :** 4 January 2024

**Issue Date :** 5 January 2024

**Condition Instrument :** Good

**Calibrated by :**

  
( Mr.Tanawut Rittidach )

Technical Manager

**Approved by :**

  
( Ms. Chonthicha Sangngern )

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.



## REPORT OF CALIBRATION

**Certificate No. :** SP24-001

Page 2 of 5

**Environment Condition :** Ambient Temperature  $25 \pm 5$  °CRelative humidity  $55 \pm 20$  %RH**Calibration method :** In-house method CP-01 Based on ASTM E275-08**Certified Reference Materials :**

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

**Traceability :** This certification is traceable to the International System of Unit maintained at National -  
Institute of Standards and Technology (NIST) through Starna Scientific Limited

**Spectral Band Width of UUC :** 1.5 nm.**Scan Speed of UUC :** 200 nm/min**Scan Interval of UUC :** 0.1 nm.**Resolution of UUC :** Photometric 0.001 Abs.

Wavelength 0.1 nm.

## REPORT OF CALIBRATION

Certificate No. : SP24-001

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.575	0.0030	0.0031	2.00
	1.0484	1.045	0.0034	0.0029	2.00
	2.1876	2.192	-0.0044	0.0080	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0034	2.00
	1.0239	1.023	0.0009	0.0035	2.00
	2.1230	2.125	-0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.520	0.0030	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.516	0.0021	0.0031	2.00
	1.0002	0.997	0.0032	0.0033	2.00
	1.9973	1.993	0.0043	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.550	0.0017	0.0030	2.00
	1.0803	1.079	0.0013	0.0030	2.00
	2.0373	2.032	0.0053	0.0080	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.558	0.0011	0.0031	2.00
	1.0518	1.050	0.0018	0.0030	2.00
	1.9274	1.923	0.0044	0.0079	2.00

เอกสารไม่ควบคุม

## REPORT OF CALIBRATION

Certificate No. : SP24-001

Page 4 of 5

### Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.743	0.0039	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.862	0.0054	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.289	0.0029	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.641	0.0020	0.0055	2.00



## REPORT OF CALIBRATION

Certificate No. : SP24-001

Page 5 of 5

### Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.72	241.2	0.52	0.18	2.00
279.45	279.0	0.45	0.18	2.00
287.81	287.4	0.41	0.18	2.00
334.06	333.8	0.26	0.18	2.00
360.93	360.6	0.33	0.18	2.00
418.59	418.4	0.19	0.18	2.00
445.94	445.8	0.14	0.18	2.00
453.66	453.4	0.26	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.4	0.19	0.18	2.00
637.98	638.0	-0.02	0.18	2.00
431.38	431.2	0.18	0.18	2.00
472.50	472.5	0.00	0.18	2.00
513.47	513.4	0.07	0.18	2.00
528.88	528.9	-0.02	0.18	2.00
573.17	573.4	-0.23	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	684.4	0.00	0.18	2.00
740.72	741.0	-0.28	0.20	2.00
748.55	748.8	-0.25	0.18	2.00
807.03	807.1	-0.07	0.18	2.00
879.28	879.5	-0.22	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement *U* is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- \* Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert. No.: 24TM648

Page : 1 of 3

Equipment : Incubator  
Manufacturer : Memmert  
Model : IPP 260  
Serial No. : V615.0187  
ID No. : UAE.MIC.003/2559  
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260  
Location : Microbiology Laboratory  
Received Order : 01 April 2024  
Calibration Date : 01 April 2024  
Ambient Temperature : (  $26 \pm 10$  ) °C  
Relative Humidity : (  $50 \pm 30$  ) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

Approved Signatory

( ) Ponpan Paipim  
(✓) Suwit Imjai  
( ) Kunchit Promprat

Issue Date :

7 April 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2404-0003OC-1

Cert. No.: 24TM648

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	24	24
REL.Humid. ( % )	54	57
AC Supply ( Volt )	221	223

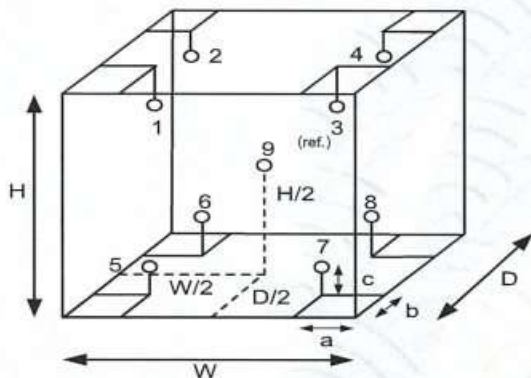

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	19-16RTD-04
5	19-16RTD-05
6	19-16RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09

**Probe Installation Details :**

a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm

**Dimension of Chamber :**

D = 0.50 m  
W = 0.64 m  
H = 0.80 m  
Capacity = 0.26 m<sup>3</sup>





Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2404-0003OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 24TM648

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.028	0.13	0.24	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.908	35.004	34.989	35.099	35.089	35.095	34.921	34.936	35.002	0.30

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert. No.: 24TM651

Page : 1 of 3

**Equipment :** Incubator

**Manufacturer :** Memmert

**Model :** IPP 260

**Serial No. :** V618.0033

**ID No. :** UAE.MIC.021/2561

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Microbiology Laboratory (302)

**Received Order :** 01 April 2024

**Calibration Date :** 02 April 2024

**Ambient Temperature :** (  $26 \pm 10$  ) °C

**Relative Humidity :** (  $50 \pm 30$  ) %

**Calibrated by :** Man Pattanapongpaiboon

**Approved by :**   
Approved Signatory

( ) Ponpan Paipim  
( ☒ ) Suwit Imjai  
( ) Kunchit Promprat

**Issue Date :** 7 April 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2404-0003OC-3

Cert. No.: 24TM651

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	25	25
REL.Humid. ( % )	54	57
AC Supply ( Volt )	221	224

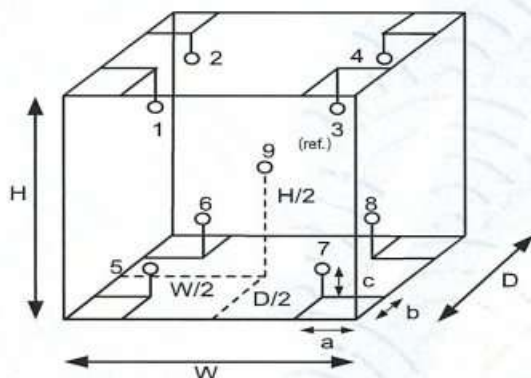

Position :	Ref. Std. ID No.:
1	20-16RTD-01
2	20-16RTD-02
3	20-16RTD-03
4	23-16RTD-04
5	22-16RTD-05
6	20-16RTD-06
7	20-16RTD-07
8	22-16RTD-08
9 (ref.)	22-16RTD-09

**Probe Installation Details :**

a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm

**Dimension of Chamber :**

D = 0.50 m  
W = 0.64 m  
H = 0.80 m  
Capacity = 0.26 m<sup>3</sup>



Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2404-0003OC-3  
**Result of Calibration :-** ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 24TM651

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
22.0	22.0	22.0	0.039	0.22	0.42	2
44.0	44.0	44.0	0.048	0.50	0.90	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
22.0	22.008	22.034	22.039	22.021	21.746	21.698	21.668	21.668	21.846	0.30
44.0	44.267	44.602	44.293	44.402	44.004	43.961	43.756	44.000	44.205	0.30

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 24TM29

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Water Bath

**Manufacturer :** Memmert

**Model :** WNE 14

**Serial No. :** L416.0606

**ID No. :** UAE.MIC.002/2560

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Microbiology Laboratory

**Received Order :** 10 February 2024


**Calibration Date :** 10 February 2024

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Krisda Malee

**Approved by :**

  
Approved Signatory

- ( ) Pornthippa Tameyakul  
( ☒ ) Unnophol Harachai  
( ) Suwit Imjai

**Issue Date :**

19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2402-0232OC-2

Cert. No.: 24TM29

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	Environmental		AC Voltage Supply
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	26	51	220
Finished of Calibration	25	50	221

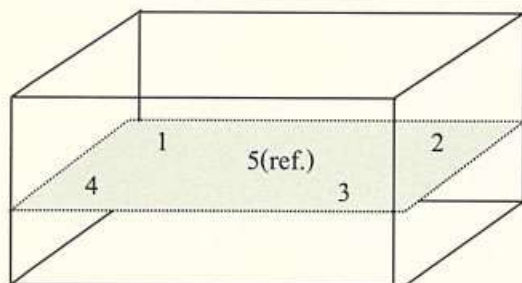

Front

Position :	Ref. Std. ID No.:
1	N37P301419
2	N37P300732
3	N37P301420
4	N37P301421
5(ref.)	N37P301425

เอกสารไม่ควบคุม





Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2402-0232OC-2  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 24TM29

Page : 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty  ( ± °C )
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.4	44.4	44.508	44.469	44.502	44.521	44.527	0.15

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <i>k</i>
44.5	0.15	0.074	2

**Average\*** : The average of 30 values in each position.

**Uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 24TM30

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Water Bath

**Manufacturer :** Memmert

**Model :** WNE 14

**Serial No. :** L416.0612

**ID No. :** UAE.MIC.003/2560

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Microbiology Laboratory

**Received Order :** 10 February 2024

**Calibration Date :** 10 February 2024

**Ambient Temperature :** (  $26 \pm 10$  ) °C

**Relative Humidity :** (  $50 \pm 30$  ) %

**Calibrated by :** Krisda Malee

**Approved by :**

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ☒ ) Unnophol Harachai  
( ) Suwit Imjai

**Issue Date :**

19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2402-0232OC-3

**Cert. No.:** 24TM30

**Page :** 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	Environmental		AC Voltage Supply
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	24	54	221
Finished of Calibration	26	55	220

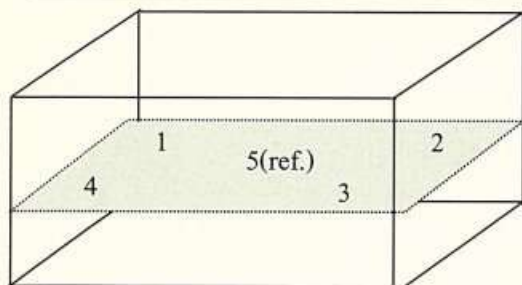

Front

Position :	Ref. Std. ID No.:
1	N37P301419
2	N37P300732
3	N37P301420
4	N37P301421
5(ref.)	N37P301425

เอกสารไม่ควบคุม



Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2402-0232OC-3  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source

Cert. No.: 24TM30

Page : 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty  ( ± °C )
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.6	44.6	44.491	44.463	44.496	44.518	44.528	0.15

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <i>k</i>
44.5	0.12	0.059	2

**Average\* :** The average of 30 values in each position.

**Uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability :** One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม




## Calibration Certificate

**Certificate No.:** 2304203-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakanong, Bangkok 10260

Page 1 of 3

**Equipment:** Autoclave  
**Manufacturer:** ALP  
**Model:** CL-40L  
**Serial No.:** 807298  
**ID No.:** UAE.MIC.019/2560  
**Order No.:** 2304203  
**Operation No.:** 2304203-001  
**Date of Receipt:** 10 August 2023  
**Date of Calibration:** 10 August 2023

**Calibrated by** Mr.Worapob Sooktong  
Scientist

**Approved by**   
( Mr.Pheraphat Tuanjit )  
Manager, Division of Calibration Laboratory  
Responsible for the Technical Management Team

**Date of Issue:** 15 August 2023

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2304203-001-01  
**Equipment:** Autoclave  
 Model: CL-40L Serial No.: 807298  
 Resolution: 1 °C ID No.: UAE.MIC.019/2560  
 Manufacturer: ALP  
**Date of Calibration:** 10 August 2023

Page 2 of 3

**Location:** 301, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Environment Condition:** Ambient Temperature ( 28 ± 1 ) °C  
 Relative Humidity ( 65 ± 2 ) %  
 Line Voltage ( 225 ± 1 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard temperature recorder with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1(2021) : Autoclaves for sterilization in laboratories Design, construction, safety and performance Specification.
  - The temperature scale used was based on ITS - 90.
  - All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-2	S25601	NC-22-11-22-176	9-Nov-23	MADGETECH INC.
	HiTemp140-2	S25602	NC-22-11-22-175	9-Nov-23	MADGETECH INC.
	HiTemp140-2	R54918	TE 660383-01	8-Apr-24	NATIONAL FOOD INSTITUTE

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good

UUC Description : Setting program function sterilization : STERILIZE/NORMAL

Time of sterilization 15 Minute At 121 °C

8. Result of Calibration :
- |                                     |                    |
|-------------------------------------|--------------------|
| <input checked="" type="checkbox"/> | Without adjustment |
| <input type="checkbox"/>            | After adjustment   |






## Calibration Report

**Certificate No.:** 2304203-001-01  
**Equipment:** Autoclave  
Model: CL-40L Serial No.: 807298  
Resolution: 1 °C ID No.: UAE.MIC.019/2560  
Manufacturer: ALP


**Date of Calibration:** 10 August 2023

Page 3 of 3

**Calibration point:** 121 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	27.0	63.5	223.3
Max	28.3	67.3	225.9

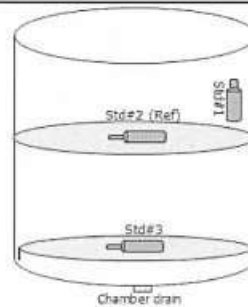

Standard Set Position

Std#1 = Attached to the load temperature probe, within 20 mm.  
Std#2 = In the upper half of the chamber  
Std#3 = In the chamber drain, within 100 mm.

**Table1 : Reporting of Temperature**

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
121	121.68	121.70	121.66	0.66

**Table 2 : Reporting of Characterization Result**

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPa			
121	121	121	121	0.10	0.11	0.12	0.23

### Note

The quoted uncertainty include " Stability " and " Loading effect ( 20% of Uniformity )"

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

*Handwritten signature*



## Calibration Certificate

**Certificate No.:** 2402281-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

**Equipment:** Autoclave  
**Manufacturer:** ALP  
**Model:** CL-40L  
**Serial No.:** 808763  
**ID No.:** UAE.MIC.026/2563  
**Order No.:** 2402281  
**Operation No.:** 2402281-001  
**Date of Receipt:** 2 April 2024  
**Date of Calibration:** 2 April 2024

**Calibrated by** Mr.Jerawut Prapawuttipong  
Scientist

**Approved by**

( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 9 April 2024

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2402281-001-01  
**Equipment:** Autoclave  
Model: CL-40L Serial No.: 808763  
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563  
Manufacturer: ALP  
**Date of Calibration:** 2 April 2024

Page 2 of 3

**Location:** LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Environment Condition:** Ambient Temperature ( 25 ± 1 ) °C  
Relative Humidity ( 55 ± 7 ) %  
Line Voltage ( 225 ± 5 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard temperature recorder with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1(2021) : Autoclaves for sterilization in laboratories Design, construction, safety and performance Specification.  
- The temperature scale used was based on ITS - 90 .  
- All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-2	R54918	TE 660383-01	8 April 2024	NATIONAL FOOD INSTITUTE
	HiTemp140-2	S25601	TE 670033-01	9 November 2024	MADGETECH INC.
	HiTemp140-2	S25602	TE 670034-01	9 November 2024	MADGETECH INC.

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good

UUC Description : Setting program function sterilization : STERILIZE/NORMAL

Time of sterilization 15 Minute At 115.0 and 121.0 °C

8. Result of Calibration : ☒ Without adjustment  
☐ After adjustment




## Calibration Report

**Certificate No.:** 2402281-001-01  
**Equipment:** Autoclave  
Model: CL-40L Serial No.: 808763  
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563  
Manufacturer: ALP


**Date of Calibration:** 2 April 2024

Page 3 of 3

**Calibration point:** 115.0 and 121.0 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	24.4	48.6	220
Max	25.5	62.1	230

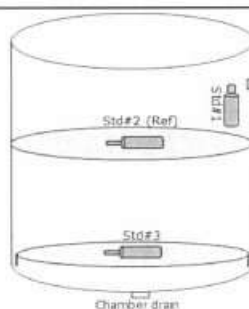

Standard at Position

Std#1 = Attached to the load temperature probe, within 20 mm.  
Std#2 = In the upper half of the chamber  
Std#3 = In the chamber drain, within 100 mm.

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
115.0	115.28	115.35	115.38	0.64
121.0	121.28	121.36	121.37	0.64

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPa			
115.0	115.0	115.1	115.0	0.08	0.19	0.13	0.48
121.0	121.0	121.1	121.0	0.12	0.17	0.10	0.38

### Note

The quoted uncertainty include " Stability " and " Loading effect ( 20% of Uniformity )"

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----






## Calibration Certificate

**Certificate No.:** 2402419-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

**Equipment:** Electronic Balance  
**Manufacturer:** OHAUS  
**Model:** PX623  
**Serial No.:** C236754745  
**ID No.:** UAE.MIC.055/2565  
**Order No.:** 2402419  
**Operation No.:** 2402419-001  
**Date of Receipt:** 19 April 2024  
**Date of Calibration:** 19 April 2024

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by**   
( Miss Preeyaporn Jaengkarnkit )

Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

**Date of Issue:** 23 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



# Calibration Report

**Certificate No.:** 2402419-001-01

**Equipment:** Electronic Balance

**Manufacturer:** OHAUS

**Model:** PX623

**Resolution:** 0.001 g

**Serial No.:** C236754745

**ID No.:** UAE.MIC.055/2565

**Capacity:** 620 g

**Date of Calibration:** 19 April 2024

Page 2 of 3

**Environment Condition:** Ambient Temperature: 26.0 ± 0.3 °C Relative Humidity: 57 ± 8.4 %

**Place of Calibration:** Room 301, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

## Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500g	15882	TCS	M23111825	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

## Calibration Results:




### 1. Repeatability of Reading:

Nominal Value ( g )	Standard Deviation of Reading ( g )
300	0.00067
600	0.0010

### 2. Off-Center Error:

A mass of 200 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1 ( g )	2 ( g )	3 ( g )	4 ( g )	5 ( g )	6 ( g )	(Maximum Difference) ( g )
200.000	200.002	200.001	199.999	200.000	200.000	0.002

F-CS-012 Revision: 01 Date: 20-04-65

*P. Jenghantit*  
23 April 2024



## Calibration Report

**Certificate No.:** 2402419-001-01

**Equipment:** Electronic Balance

**Manufacturer:** OHAUS

**Model:** PX623

**Resolution:** 0.001 g

**Serial No.:** C236754745

**ID No.:** UAE.MIC.055/2565

**Capacity:** 620 g

**Date of Calibration:** 19 April 2024

Page 3 of 3

**Calibration Results:** (Continued)

**Calibration Range:** 0-600 g

**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.0000	0.000	0.000	0.00093	2.00
1	1.0000	1.000	0.000	0.00093	2.00
5	5.0000	5.000	0.000	0.00093	2.00
10	10.0000	10.000	0.000	0.00093	2.00
20	20.0000	20.000	0.000	0.00093	2.00
50	50.0000	50.001	-0.001	0.00093	2.00
100	100.0000	100.001	-0.001	0.00094	2.00
200	200.0000	200.001	-0.001	0.0011	2.00
300	300.0000	300.003	-0.003	0.0011	2.00
400	399.9999	400.003	-0.003	0.0012	2.00
500	499.9999	500.003	-0.003	0.0013	2.00
600	599.9999	600.002	-0.002	0.0014	2.00

*P. Jongsakulwitt*  
23 April 2024

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



102019-001-01					Equipment : Electronic Balance			
Brand: OHAUS					Model: PX623			
Serial No.: C236754745					ID No.: JALM C 055/2565			
Nominal Value	Standard Value	Average Reading	Error	Correction	Uncertainty (U)	U +   Error   Total Error	Judgement	(Total Error < Judgement ) Result (Pass / Fail)
(g)	(g)	(g)	(g)	(g)	(g)	(g)	(±g)	
0	0.0000	0.000	0.000	0.000	0.00093	0.001	0.005	Pass
1	1.0000	1.000	0.000	0.000	0.00093	0.001	0.005	Pass
5	5.0000	5.000	0.000	0.000	0.00093	0.001	0.005	Pass
10	10.0000	10.000	0.000	0.000	0.00093	0.001	0.005	Pass
20	20.0000	20.000	0.000	0.000	0.00093	0.001	0.005	Pass
50	50.0000	50.001	0.001	-0.001	0.00093	0.002	0.005	Pass
100	100.0000	100.001	0.001	0.001	0.00094	0.002	0.005	Pass
200	200.0000	200.001	0.001	-0.001	0.00110	0.002	0.005	Pass
300	300.0000	300.003	0.003	-0.003	0.0011	0.004	0.010	Pass
400	399.9999	400.003	0.003	-0.003	0.0012	0.004	0.010	Pass
500	499.9999	500.003	0.003	-0.003	0.0013	0.004	0.010	Pass
600	599.9999	600.002	0.002	-0.002	0.0014	0.003	0.010	Pass

UC \* : Unit Under Calibration

Remarks:

เอกสารไม่ควบคุม

**Envi Equipment Service Co., Ltd.**

110/254 Moo 3, Tumbon Bang Rak Phatthana, Amphur Bang Bua Thong, Nonthaburi 11110

Tel. 098 362 9152, 089 478 7885

E-mail: sales@envi-ees.com

Certificate No. : E23-08066

Page : 1 of 6

**CERTIFICATE OF CALIBRATION**

**Customer** : United Analyst and Engineering Consultant Co., Ltd.

**Address** : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

**Description of Equipment** : Console meter

**Manufacturer** : Apex Instrument

**Model Number** : XC-572-V

**Serial Number** : 1904011

**ID./Control No.** : -

**Environment Conditions** : Temperature (25 ± 2) °C  
Humidity (50 ± 15) % RH

**Cal. Date** : 05/08/2023

**Issue Date** : 05/08/2023

**Calibration Method or Calibration Procedure Used**

US EPA Method (United State Environmental Protection Agency)


This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (IS).

**Result of Calibration**

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : Mr. Sanya Sangnil

Approved by :   
(Mr. Mana Fuekhud)  
Technical Manger



**เอกสารไม่ควบคุม**

## METHOD 5 CONSOLE CALIBRATION USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425 5-POINT METRIC UNIT

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	05/08/2023	09:50 AM	Std Temp	293	K
Console Serial Number	1904011	Calibration Reference No.		SER23-08027		Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure		758.99		K <sub>1</sub>	0.386	
DGM Serial Number	00004114	Calibration Meter Gamma		0.999		Console Leak Check		PASS

Calibration Data									
Run Time	Metering Console					Calibration Meter			
Elapsed	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
(Q)	(P <sub>m</sub> )	(V <sub>mi</sub> )	(V <sub>mf</sub> )	(t <sub>mi</sub> )	(t <sub>mf</sub> )	(V <sub>wi</sub> )	(V <sub>wf</sub> )	(t <sub>wi</sub> )	(t <sub>wf</sub> )
min	mm H <sub>2</sub> O	m <sup>3</sup>	m <sup>3</sup>	°C	°C	m <sup>3</sup>	m <sup>3</sup>	°C	°C
12.35	13.0	1342.996	1343.136	29	29	155.32046	155.46168	27	27
12.42	13.0	1343.136	1343.276	29	29	155.46168	155.60264	27	27
8.80	26.0	1343.282	1343.422	29	29	155.60872	155.75014	27	27
8.80	26.0	1343.422	1343.562	30	30	155.75014	155.89098	26	26
13.95	40.0	1343.569	1343.849	30	30	155.89796	156.17902	26	26
13.95	40.0	1343.849	1344.129	31	31	156.17902	156.45838	26	26
10.50	70.0	1344.138	1344.418	31	31	156.46734	156.74556	26	26
10.47	70.0	1344.418	1344.698	32	32	156.74556	157.02264	26	26
9.12	90.0	1344.711	1344.991	32	32	157.03528	157.31088	26	26
9.12	90.0	1344.991	1345.271	32	32	157.31088	157.58638	25	25





**METHOD 5 CONSOLE CALIBRATION**  
**USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425**  
**5-POINT METRIC UNIT**

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	05/08/2023	09:50 AM	Std Temp	293	K
Console Serial Number	1904011	Calibration Reference No.		SER23-08027		Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure		758.99	mmHg	K <sub>1</sub>	0.386	
DGM Serial Number	00004114	Calibration Meter Gamma		0.999		Console Leak Check		PASS

Calibration Data								
Results								
Standardized Data				Dry Gas Meter				
Dry Gas Meter		Calibration Meter		Calibration Factor		Flowrate		
(V <sub>m(std)</sub> )	(Q <sub>m(std)</sub> )	(V <sub>w(std)</sub> )	(Q <sub>w(std)</sub> )	Value	Variation	Std & Corr	.0212 m <sup>3</sup> <sub>std</sub> /min	Variation
m <sup>3</sup>	m <sup>3</sup> /min	m <sup>3</sup>	m <sup>3</sup> /min	(Y)	(ΔY)	(Q <sub>m(std)(corr)</sub> )	(ΔH <sub>@</sub> )	(ΔH <sub>@</sub> )
						m <sup>3</sup> /min	mm H <sub>2</sub> O	
0.137	0.011	0.138	0.011	1.006	0.014	0.011	46.171	-0.333
0.137	0.011	0.137	0.011	1.005	0.012	0.011	46.843	0.339
0.137	0.016	0.138	0.016	1.007	0.014	0.016	46.870	0.366
0.137	0.016	0.138	0.016	1.002	0.010	0.016	47.099	0.595
0.275	0.020	0.275	0.020	0.999	0.006	0.020	45.847	-0.657
0.275	0.020	0.273	0.020	0.993	0.000	0.020	46.407	-0.097
0.276	0.026	0.272	0.026	0.986	-0.007	0.026	46.656	0.152
0.276	0.026	0.271	0.026	0.982	-0.011	0.026	46.743	0.239
0.276	0.030	0.269	0.030	0.975	-0.018	0.030	46.263	-0.241
0.277	0.030	0.270	0.030	0.974	-0.018	0.030	46.142	-0.362
				0.993	Y Average		46.504	ΔH <sub>@</sub> Average

**Note:** For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is  $\pm 0.02$ .

For  $\Delta H_{@}$ , orifice pressure differential that equates to 0.75 cfm (0.0212 m<sup>3</sup>/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is  $\pm 0.2$  inches (5.1mm) H<sub>2</sub>O.



Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	1904011
DGM Model Number	SK25EX
DGM Serial Number	00004114


Calibration Conditions			
Date	Time	05/08/2023	09:50 AM
Calibration Reference No.	SER23-08027		
Barometric Pressure	758.99	mmHg	
Calibration Meter Gamma	0.999		

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K <sub>1</sub>	0.386	
Console Leak Check	PASS	

Calibration Date: 5-8-2023

Calibration Reference No: SER23-08027

Meter Gamma vs Flowrate

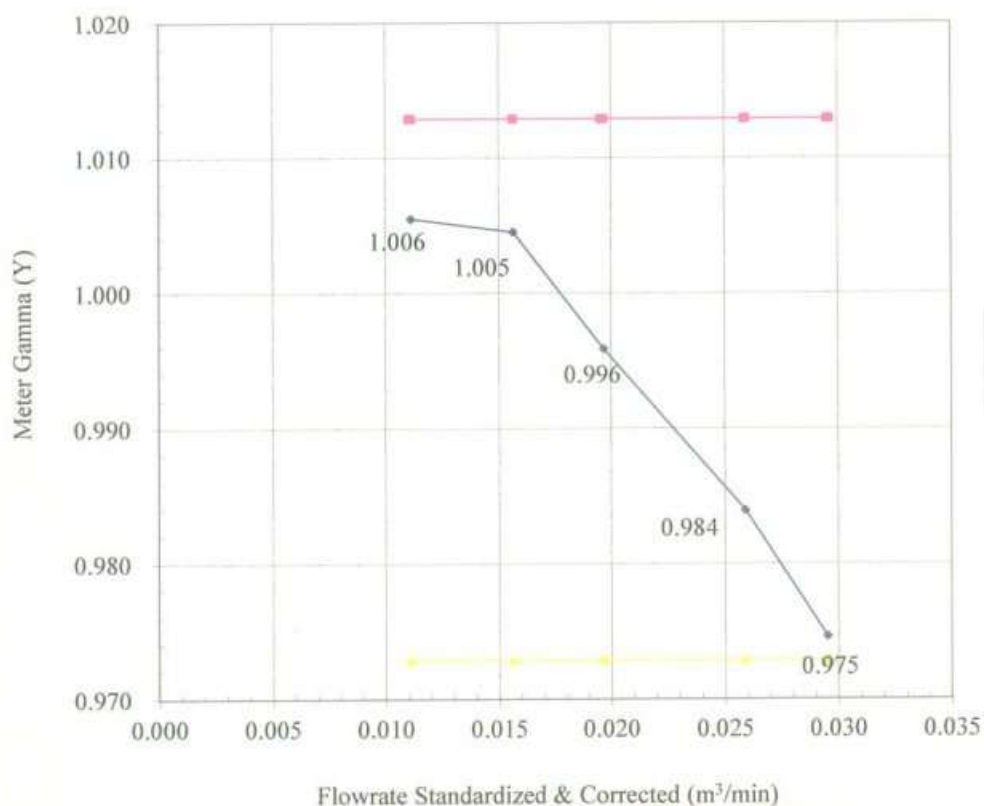

Console Serial: 1904011

Console Model: XC-572-V



เอกสารไม่ควบคุม

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	1904011
DGM Model Number	SK25EX
DGM Serial Number	00004114


Calibration Conditions			
Date	Time	05/08/2023	09:50 AM
Calibration Reference No.	SER23-08027		
Barometric Pressure	758.99	mmHg	
Calibration Meter Gamma	0.999		

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K <sub>1</sub>	0.386	
Console Leak Check	PASS	

Calibration Date: 5-8-2023

Calibration Reference No: SER23-08027

Meter Pressure vs Flowrate

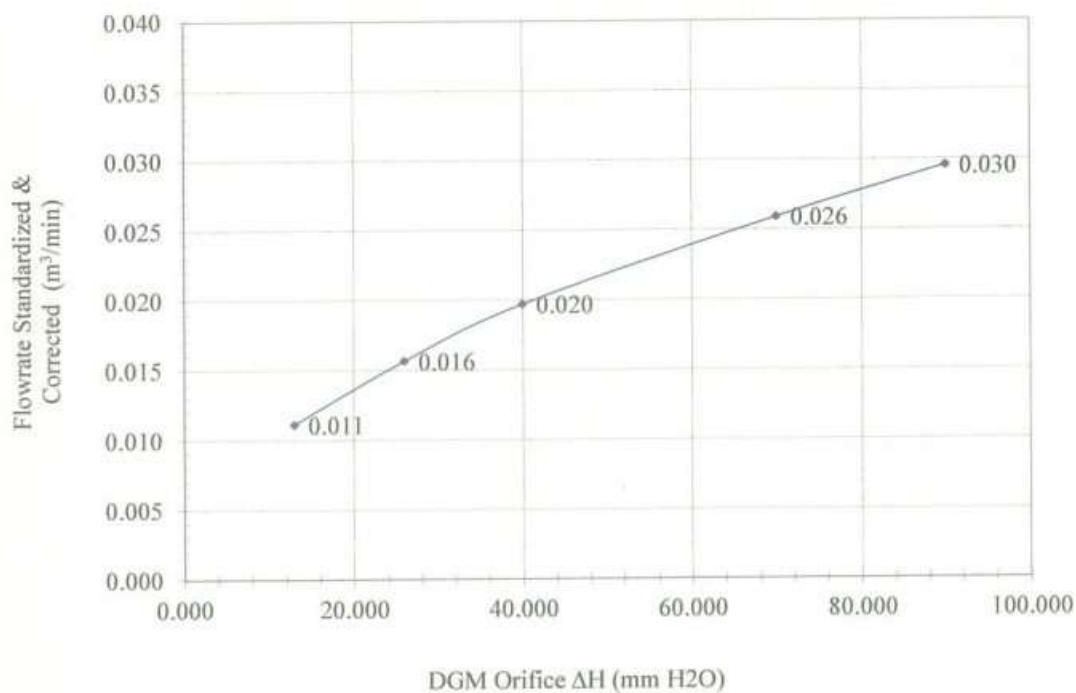

Console Serial: 1904011

Console Model: XC-572-V



เอกสารไม่ควบคุม



## THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information	
Console Model Number	XC-572-V
Console Serial Number	1904011
DGM Model Number	SK25EX
DGM Serial Number	00004114
Meter Box Model Number	JENCO 765 KF
Meter Box Serial Number	JC 17215

Calibration Conditions			
Date	Time	05/08/2023	12:10 PM
Calibration Reference No.	SER23-08027		
Reference Thermometer	DIGICON		
Serial Number	183169105		

Results											
Console Thermocouple Simulator											
Channel and test point	Meter Box Channel Temperature Reading ( °C )										
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1038.0
Stack	-17.0	25.0	37.0	93.0	149.0	258.0	370.0	481.0	592.0	814.0	1037.0
Aux	-16.0	25.0	37.0	93.0	149.0						
Probe	-17.0	24.0	37.0	93.0	149.0						
Filter	-16.0	24.0	37.0	93.0	149.0						
Oven	-16.0	24.0	37.0	93.0	149.0						
Exit	-16.0	24.0	37.0								

### Tolerance Range

Stack      ± 1.50%      Absolute  
 Probe      ± 3.0 °C  
 Filter      ± 3.0 °C

Meter      ± 3.0 °C  
 Exit      ± 2.0 °C



เอกสารไม่ควบคุม



**Certificate No:** G 660614

**Date of issue :** 06-Oct-23

**Instrument description :** Flue Gas Analyzer  
**Instrument model :** Testo 350 New  
**Control unit serial no. :** 03099402/701  
**Instrument serial no. :** 60899617/701  
**ID no. or control no. :** UAE.EFM. 007/2560  
**Manufacturer :** Testo SE & Co. KGaA  
**Probe description :** -  
**Probe model :** -  
**Probe serial no. :** -  
**Customer name :** United Analyst and Engineering Consultant Co., Ltd.  
**Customer address :** 81 Soi Udomsuk 41, Sukhumvit Rd., Bangchak, Phrakhanong, Bangkok 10260

**Total pages of certificate :** 2 Pages  
**Receiving no. :** L-233264  
**Receiving date. :** 28-Sep-23  
**Parameter of calibration :** Gas Calibration(Oxygen 2.498,10.04,21.02 %vol, Carbon Monoxide 80.14,302,1003 ppm, Nitrogen Dioxide 30.34,80.96,201.9 ppm, Nitric Oxide 30.01,151.5,322.5 ppm, Sulphur Dioxide 50.36,100.8,600.8 ppm)  
**Condition of UUC. :** Used  
**Ambient condition :** All of the Measurement were carried out the stabilized laboratory  
Temperature : 23 ± 5 °C  
Humidity : 55 ± 15 %RH  
**Calibration place :** 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210  
**Calibration procedure no. :** This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C

*The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement Multiplied by coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.*

*This certificate is applied only to item under test Environmental condition.*

*This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.*

*This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).*

**Date of calibration :** 05-Oct-23

*Kwanchai K.*

Mr. Kwanchai Khamdoun  
Calibration Technician

*Nongluck W.*

Mrs. Nongluck Wongsettee  
Technical Manager

**Certificate No.:** G 660614

**Standard References (Table 1)**

Standard	Certificate No.	Vendor	Due date
Oxygen ( O <sub>2</sub> ) 2.498 % Vol	4219/21	Linde	30-Sep-25
Oxygen ( O <sub>2</sub> ) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen ( O <sub>2</sub> ) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide ( CO ) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide ( CO ) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide ( CO ) 1003 ppm	2584/23	Linde	10-Sep-25
Nitrogen Dioxide ( NO <sub>2</sub> ) 30.34 ppm	2703/22	Linde	22-Aug-24
Nitrogen Dioxide ( NO <sub>2</sub> ) 80.96 ppm	3240/21	Linde	26-Jun-24
Nitrogen Dioxide ( NO <sub>2</sub> ) 201.9 ppm	1975/23	Linde	17-Jul-25
Nitric Oxide ( NO ) 30.01 ppm	CG-0014-23	Nimt	19-Feb-25
Nitric Oxide ( NO ) 151.5 ppm	0161/23	Linde	22-Jan-25
Nitric Oxide ( NO ) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide ( SO <sub>2</sub> ) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide ( SO <sub>2</sub> ) 100.8 ppm	3507/22	Linde	09-Nov-24
Sulphur Dioxide ( SO <sub>2</sub> ) 600.8 ppm	2003/23	Linde	17-Jul-25

**Measured room conditions**

Temperature : 22.1 °C Humidity : 66.7 %RH Pressure : 1009.4 mbar

**Calibration conditions**

Gas Temperature : 23 °C Flow rate : 1,100 ml/min Gas pressure : 1019.4 mbar

**Calibration Results (Without adjustment) (Table 2)**

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O <sub>2</sub> (%Vol)	2.498	2.48	-0.018	0.15
O <sub>2</sub> (%Vol)	10.04	10.07	0.03	0.20
O <sub>2</sub> (%Vol)	21.02	21.10	0.08	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	302	304	2	6.0
CO (ppm)	1003	1008	5	12
NO <sub>2</sub> (ppm)	30.34	28.2	-2.14	8.0
NO <sub>2</sub> (ppm)	80.96	80.5	-0.46	8.0
NO <sub>2</sub> (ppm)	201.9	204.7	2.8	12
NO (ppm)	30.01	29	-1.01	8.0
NO (ppm)	151.5	152	0.5	8.0
NO (ppm)	322.5	322	-0.5	12
SO <sub>2</sub> (ppm)	50.36	50	-0.36	6.0
SO <sub>2</sub> (ppm)	100.8	103	2.2	6.0
SO <sub>2</sub> (ppm)	600.8	606	5.2	13

**Remark :** 1 cmol/mol = 1 %vol. 1 μmol/mol = 1 ppm.

**End of Report**



JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Flow measurement laboratory  
Calibration services department.



## CERTIFICATE OF CALIBRATION

Certificate No. : COF-001-66

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Top Load Orifice  
**MANUFACTURER** : Graseby GMW  
**MODEL/TYPE** : G25A  
**SERIAL NUMBER** : 158M  
**ID NUMBER** : UAE.EMA2.033/2554  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : United Analyst and Engineering Consultant Co., Ltd.  
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,  
Bangkok 10260

**RECEIVED DATE** : 07 Jul 2023  
**MEASUREMENT DATE** : 14 Jul 2023  
**ISSUE DATE** : 18 Jul 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: $23.0 \pm 3.0$	°C
Relative Humidity	: $55.0 \pm 15.0$	%RH
Atmospheric Pressure	: $1010 \pm 10$	hPa

### CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.  
Measurement Condition : The average values during measurement are 23.7 °C and 52.9%RH.

**NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

### Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the VSL (National Metrology Institute of Netherlands) via Certificate number: G2211901

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor  $k=2$ , Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen  
Calibration Department Manager

เอกสารไม่ควบคุม



**MEASUREMENT RESULTS:**

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

**Table 1:** The results of  $Q$  Standard calibration data

Plate	Flow rate $m^3/min$	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p_{meter}$ mmHg	$\Delta p_{Orifice}$ inH <sub>2</sub> O	$Y$	Standard Flow [ $Q_s$ ] $m^3/min$
1	0.700	753.503	23.71	23.16	48.213	1.565	1.248	0.653
2	1.003	753.442	23.75	23.36	52.965	3.186	1.781	0.930
3	1.115	753.274	23.95	23.57	35.125	4.160	2.034	1.059
4	1.175	753.263	23.94	23.73	26.925	4.729	2.169	1.127
5	1.412	753.351	24.03	23.75	25.751	6.920	2.623	1.358

Slope ( $m$ ): 1.95114  
 Intercept ( $b$ ): -0.02950  
 Correlation coefficient ( $r$ ): 0.99975  
 Uncertainty ( $k=2$ ): 0.015  $m^3/min$

**Table 2:** The results of  $Q$  actual calibration data

Plate	Flow rate $m^3/min$	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p_{meter}$ mmHg	$\Delta p_{Orifice}$ inH <sub>2</sub> O	$Y$	Standard Flow [ $Q_o$ ] $m^3/min$
1	0.700	753.503	23.71	23.16	48.213	1.565	0.785	0.656
2	1.003	753.442	23.75	23.36	52.965	3.186	1.120	0.934
3	1.115	753.274	23.95	23.57	35.125	4.160	1.281	1.064
4	1.175	753.263	23.94	23.73	26.925	4.729	1.366	1.133
5	1.412	753.351	24.03	23.75	25.751	6.920	1.652	1.365

Slope ( $m$ ): 1.22204  
 Intercept ( $b$ ): -0.01853  
 Correlation coefficient ( $r$ ): 0.99975  
 Uncertainty ( $k=2$ ): 0.015  $m^3/min$

\*\*\*End of Certificate of Calibration\*\*\*



เอกสารไม่ควบคุม





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484

## Certificate of Calibration

Certificate No. : 23P1403

Page : 1 of 2

Equipment : U-Tube Manometer

Manufacturer: Dwyer

Model : 1221-36-W/M

Serial No.: -

ID No.: UAE.EFM.181/2561

Condition As-Received: Used Item

Received Date: 26 April 2023

Calibration Date: 09 May 2023

Reference: 2304-0703WSC

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1010 mbar

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

**Procedure used:** The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Pressure Calibrator	PC106P	1189	MP-0137-22	24 Aug 2023

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH<sub>2</sub>O

4.This instrument was used clean air as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suwit Aussarree

Issue Date : 11 May 2023

Approved Signatory :

Attapol P.  
[ ] Phalinee Prabpaipal  
[ ] Sura Suwannasri  
✓ Attapol Panurach

เอกสารไม่ควบคุม

B 0314243



Cert.No.: 23P1403

Page: 2 of 2

Result of calibration:- Without adjustment

Function:- Pressure Measurement

Increasing Pressure

Range : 0 inH<sub>2</sub>O to 36 inH<sub>2</sub>O

Scale Interval : 0.1 inH<sub>2</sub>O ( The Fifth Estimate )

<u>Applied Pressure</u> (inH <sub>2</sub> O)	<u>UUC Indication</u>		<u>ΔP</u> (inH <sub>2</sub> O)	<u>Error</u> (inH <sub>2</sub> O)
	<u>High-port side</u> (inH <sub>2</sub> O)	<u>Low-port side</u> (inH <sub>2</sub> O)		
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.02	8.02	0.02
10.00	5.00	-5.02	10.02	0.02
12.00	6.00	-6.02	12.02	0.02
14.00	6.98	-7.00	13.98	-0.02
16.00	7.98	-8.00	15.98	-0.02
18.00	8.98	-9.00	17.98	-0.02
20.00	9.98	-10.00	19.98	-0.02
22.00	11.00	-11.02	22.02	0.02
24.00	12.00	-12.02	24.02	0.02
26.00	13.00	-13.04	26.04	0.04
28.00	14.00	-14.04	28.04	0.04
30.00	15.00	-15.02	30.02	0.02
32.00	16.00	-16.02	32.02	0.02
34.00	16.96	-17.00	33.96	-0.04
35.80	17.96	-18.00	35.96	0.16

The uncertainty of measurement was  $\pm 0.11$  inH<sub>2</sub>O

\* UUC = Unit Under Calibration

\* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.

เอกสารไม่ควบคุม  
a 1160342

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok  
10260

Certificate No : 23-AFM-187

Request No : Req-2023-1655

### Unit Under Calibration Details

Measurement Item : Air Flow Meter  
Manufacturer : BGI  
Model : Delta Cal DC1  
Serial Number : 158850  
ID : UAE.EFM.038/2561  
Location of Calibration : LAB 4 AIR VELOCITY METER

Sensor Model : -

Sensor Serial Number : -

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 7 August 2023  
Calibration Date : 30 August 2023  
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 High flow	18501012012	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	7 November 2023


### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 30 August 2023



Certificate No : 23-AFM-187

Request No : Req-2023-1655

**Result of Calibration :**

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Uncertainty (l/min)
25.10	100.70	14.50	14.50	0.00	0.20
25.10	100.70	15.00	14.99	-0.01	0.21
25.00	100.70	15.80	15.79	-0.01	0.22
24.90	100.70	16.67	16.65	-0.02	0.23
24.80	100.70	18.30	18.26	-0.04	0.26

**Note**

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At 25.0 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate

P = Absolute Pressure

T = Absolute Temperature

Meas = Measurement Condition

ref = Standard Condition

\* Indicates non accredited

**End of Certificate**



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO., LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

Certificate No : 23-TPM-424

Request No : Req-2023-1655

Page : 1/2

### Unit Under Calibration Details

Calibration Parameter	: Temperature	Range Calibration	: 20 °C to 50 °C
Instrument Name	: Air Flow meter	Type of Sensor	: RTD
Manufacturer	: BGI	Sensor Diameter (mm)	: 3
Model	: Delta Cal DC1	Calibration Position (mm)	: 45
Serial Number	: 158850	Instrument Status	: Used
Resolution	: 0.1 °C		
ID Number	: UAE.EFM.038/2561		

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 15 %RH  
Received Date : 7 August 2023  
Calibrated Date : 30 August 2023  
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

**Reference Standard** : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN:  
08000057, ID: 02-TPM Which was calibrated on 27 Febuary 2023, Calibration Certificate No. : QR23-  
0494

**Traceability** : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.:  
Calibration 0292

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Approved By :

*me*

Mr. Noppadon Luangart

Technical Manager

Issue Date :

30 August 2023



**Calibration Note**

UUC Adjustment : Not Adjust

**Certificate No : 23-TPM-424**

**Request No : Req-2023-1655**

**Page : 2/2**

**Result of Calibration :**

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
Ta	20.032	20.0	0.0	0.13
	25.034	25.0	0.0	0.13
	30.035	30.0	0.0	0.13
	35.036	35.0	0.0	0.13
	40.038	40.1	- 0.1	0.13
	45.041	45.1	- 0.1	0.13
	50.044	50.2	- 0.2	0.13

**End of Certificate**

**Calibrated By :**

Mr. Sittichok Jirapukdeesakul

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO., LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

Certificate No : 23-TPM-458

Request No : Req-2023-1977

Page : 1/2

### Unit Under Calibration Details

Calibration Parameter	: Temperature	Range Calibration	: 20 °C to 50 °C
Instrument Name	: Air Flow meter	Type of Sensor	: RTD
Manufacturer	: BGI	Sensor Diameter (mm)	: 3
Model	: Delta Cal DC1	Calibration Position (mm)	: 45
Serial Number	: 158850	Instrument Status	: Used
Resolution	: 0.1 °C		
ID Number	: UAE.EFM.038/2561		

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 15 %RH  
Received Date : 14 September 2023  
Calibrated Date : 27 September 2023  
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.


**Reference Standard** : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN: 08000057, ID: 02-TPM Which was calibrated on 27 Febuary 2023, Calibration Certificate No. : QR23-0494

**Traceability** : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Approved By :

  
Mr. Noppadon Luangart  
Technical Manager

Issue Date :

27 September 2023

**Calibration Note**

UUC Adjustment : Not Adjust

Certificate No : 23-TPM-458

Request No : Req-2023-1977

Page : 2/2

**Result of Calibration :**

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
Tf	20.033	20.0	0.0	0.13
	25.033	25.0	0.0	0.13
	30.033	30.0	0.0	0.13
	35.034	35.1	- 0.1	0.13
	40.040	40.1	- 0.1	0.13
	45.039	45.1	- 0.1	0.13
	50.043	50.1	- 0.1	0.13

End of Certificate

Calibrated By :



Mr. Sittichok Jirapukdeesakul





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23P1857

Page : 1 of 2

Equipment : Aneroid Barometer  
Manufacturer: Barigo  
Model : -  
Serial No.: -  
ID No.: UAE.ANV.151/2550

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 02 June 2023

Reference: 2305-0919WSC

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

Atmospheric Pressure: 1007 mbar

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.This result of calibration instrument was in absolute pressure.

5.This instrument was used clean air as pressure media.

6.The certificate is valid only to the item calibrated on date and place of calibration.

7.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew  
Issue Date : 08 June 2023

Approved Signatory : Attapol P.  
[ ] Phalinee Prabpaipal  
[ ] Sura Suwannasri  
[x] Attapol Panurach

เอกสารไม่ควบคุม  
B 0316957



Cert.No.: 23P1857

Page: 2 of 2

Result of calibration:- Without adjustment

Range : 960 hPa to 1030 hPa

Function:- Absolute Pressure Measurement

Scale Interval : 1 hPa ( The Fifth Estimate )

Increasing Pressure

Applied Pressure (hPa)	960.27	971.66	982.37	994.32	1001.76	1010.97	1020.99	1030.52
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	-0.27	-1.66	-2.37	-4.32	-1.76	-0.97	-0.99	-0.52

Decreasing Pressure

Applied Pressure (hPa)	1030.52	1021.07	1011.30	1001.83	992.38	982.43	971.77	960.50
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-0.52	-1.07	-1.30	-1.83	-2.38	-2.43	-1.77	-0.50

The uncertainty of measurement was  $\pm 0.30$  hPa

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.

เอกสารไม่ควบคุม  
a 1165501



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX: 0-2719-9484



## Certificate of Calibration

Certificate No. : 23H1200

Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: UAE.ANV.130/2550

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 30 May 2023  
to 06 June 2023

Reference: 2305-0919WSC

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

**Procedure used:** Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

1. Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Hygro-M2 Dew Point Monitor	5112	2360195	20703	02 Aug 2023
2) Handheld Thermometer With Sensor	1523	3240076	231305	15 Mar 2024


2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

- National Institute of Standards and Technology (NIST) , The United States of America
- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Somchai Dumwor  
Issue Date : 07 June 2023

Approved Signatory :

-   
☒ Chakrit Waewwanjua  
☐ Pornthippa Tameyakul  
☐ Viporn Tantiyawutti

เอกสารไม่ควบคุม  
B 0316274





Cert. No.: 23H1200

Page.: 2 of 2

**Result of Calibration:-**

Before Adjustment

Function:

Humidity Measurement

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	40.1	48	7.9	1.6
25.0	60.0	63	3.0	1.7
25.0	80.0	76	-4.0	1.9

**Result of Calibration:-**

After Adjustment

Function:

Humidity Measurement

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	40.1	44	3.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	75	-5.0	1.9

**Result of Calibration:-**

Without Adjustment

Function:

Temperature Measurement

<u>Standard</u> <u>Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (±°C)
19.987	20.0	0.013	0.72
30.016	30.0	-0.016	0.72
39.944	39.5	-0.444	0.72

UUC\* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor  $k = 2.00$ , providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม  
a 1165295



### MULTI-POINT GAS TEST REPORT

**Test Date** : Jan 11, 2023

**Equipment** : Gas Analyzer (NO<sub>2</sub>)

**Model** : 42i

**Manufacturer** : Thermo Scientific

**Serial Number** : CM08130002

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 21, 2024


#### Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.4	0.40	0.20	0.20
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.22

Multi-Point Gas Test Chart

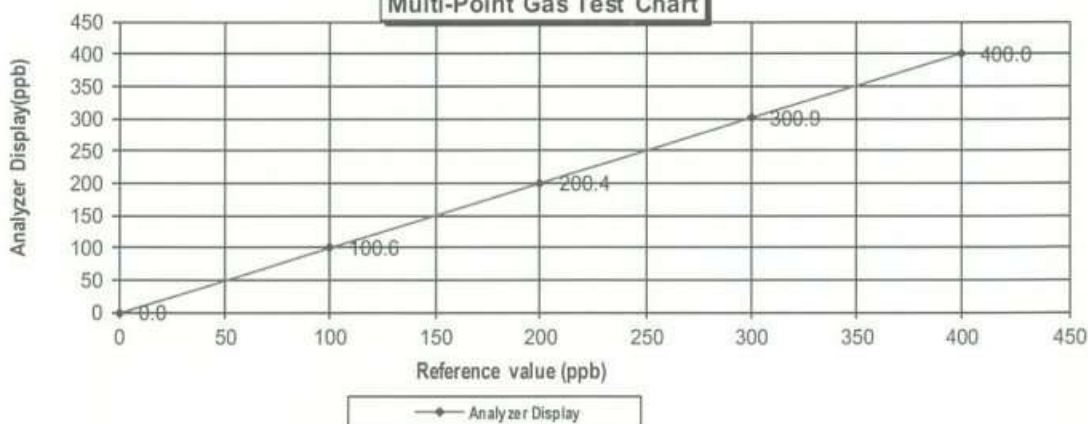

Calculate by

*Sirichai Sornngou*  
11 / 1 / 66

Approve by

*Pattinorn*  
11 / Jan / 2023

### MULTI-POINT GAS TEST REPORT

**Test Date** : Feb 15, 2023

**Equipment :** Gas Analyzer (NO<sub>2</sub>)

**Model :** 42i

**Manufacturer :** Thermo Scientific

**Serial Number :** CM19050148

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 21, 2024


#### Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.2	0.20	0.20	0.20
Level 3	40.00%	200.0	201.0	1.00	0.50	0.50
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.20

Multi-Point Gas Test Chart

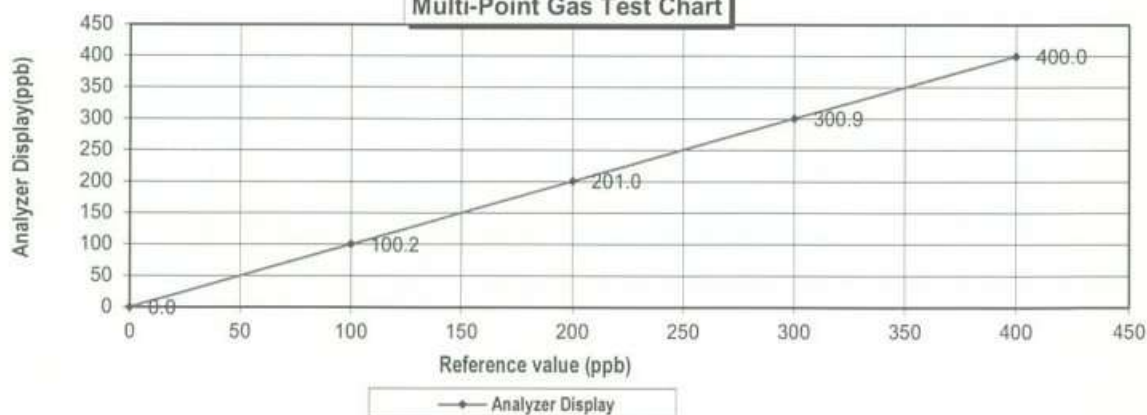

Calculate by

*Sirichai Yamgarn*  
15 / 2 / 66

Approve by

*Prakarn K*  
15 Feb 2023

### MULTI-POINT GAS TEST REPORT

Test Date : Jan 9, 2023

Equipment : Gas Analyzer (NO<sub>2</sub>)

Model : 42i

Manufacturer : Thermo Scientific

Serial Number : CM19050149

#### Standard Gas Concentration

Sulphur Dioxide (SO<sub>2</sub>) 44.68 PPM  
Nitric Oxide (NO) 45.94 PPM  
Methane (CH<sub>4</sub>) - PPM  
Carbon Monoxide (CO) 984.8 PPM  
Cylinder No. : EB0143262  
Expiration Date : Jun 21, 2024


#### Dilutor Detail

Manufacturer : Thermo Scientific  
Model : 146i  
Serial Number : 1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[ % Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	201.2	1.20	0.60	0.60
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)		0.32	

Multi-Point Gas Test Chart

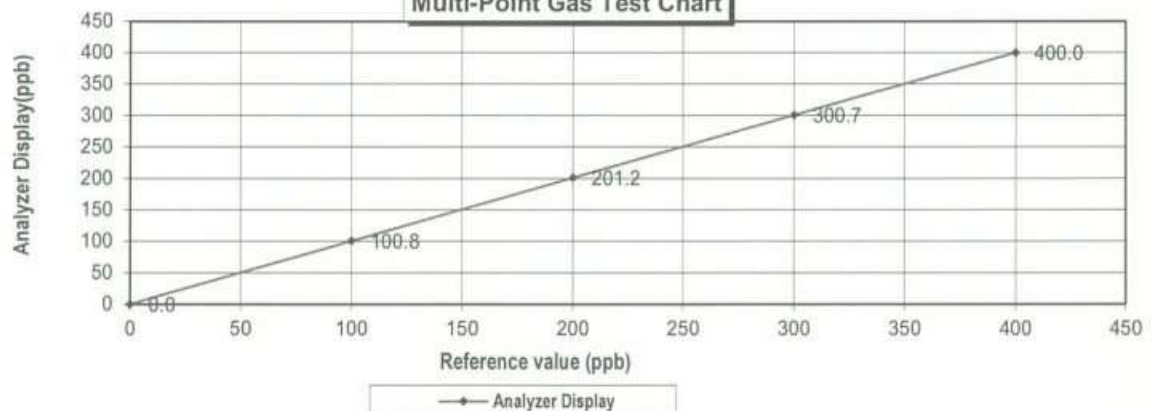

Calculate by

*Sirichai Samgaw*  
9 / 1 / 66

Approve by

*Pattana*  
9 / Jan / 2023



### MULTI-POINT GAS TEST REPORT

**Test Date** : Jan 16, 2023

**Equipment** : Gas Analyzer (NO<sub>2</sub>) **Model** : 42i  
**Manufacturer** : Thermo Scientific **Serial Number** : CM19050150

#### Standard Gas Concentration


Sulphur Dioxide (SO<sub>2</sub>) 44.68  
Nitric Oxide (NO) 45.94  
Methane (CH<sub>4</sub>) -  
Carbon Monoxide (CO) 984.8  
Cylinder No. : EB0143262  
Expiration Date : Jun 21, 2024

#### Dilutor Detail

Manufacturer : Thermo Scientific  
Model : 146i  
Serial Number : 1180540071

#### Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.5	0.50	0.50	0.50
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.21
:Acceptable Limit $\pm 5\%$						

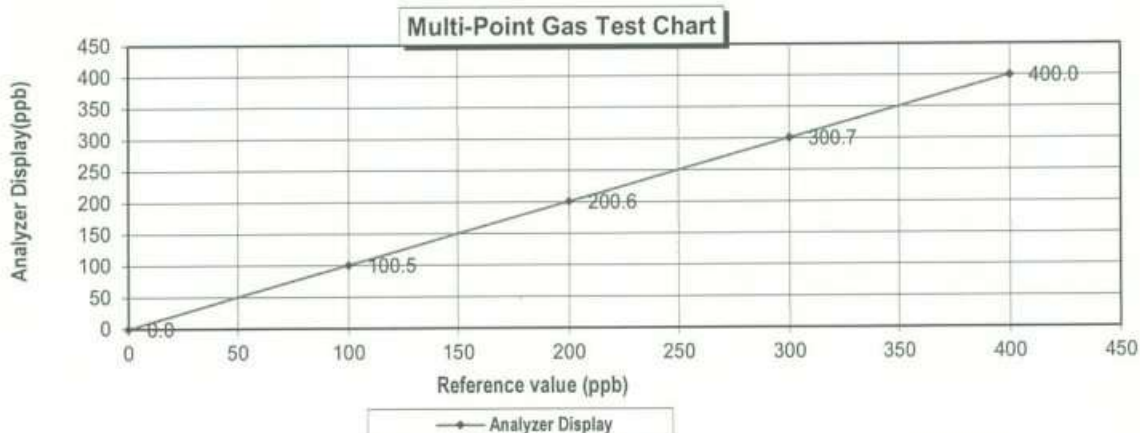

Calculate by

Aphiwat h.  
16 / 01 / 66

Approve by

16 / Jan / 2023



# CERTIFICATE OF ANALYSIS

## Grade of Product: EPA Protocol

Part Number:	E04NI99E15A01D3	Reference Number:	122-402135167-1
Cylinder Number:	EB0143262	Cylinder Volume:	144.4 CF
Laboratory:	124 - Durham (SAP) - NC	Cylinder Pressure:	2015 PSIG
PGVP Number:	B22021	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.68 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20061120	CC708068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D685025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505581	4,348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14060119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/-0.6%	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO2	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

*[Signature]*

Approved for Release



CERT 3082.01

เอกสารไม่ควบคุม

### MULTI-POINT GAS TEST REPORT

**Test Date** : Nov 3, 2023

**Equipment** : Gas Analyzer (SO<sub>2</sub>)

**Model** : 43i

**Manufacturer** : Thermo SCIENTIFIC

**Serial Number** : 1180540065

#### Standard Gas Concentration


Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 24, 2024

#### Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.70	0.70	0.70
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.5	0.50	0.25	0.25
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.41
:Acceptable Limit $\pm$ 5%						

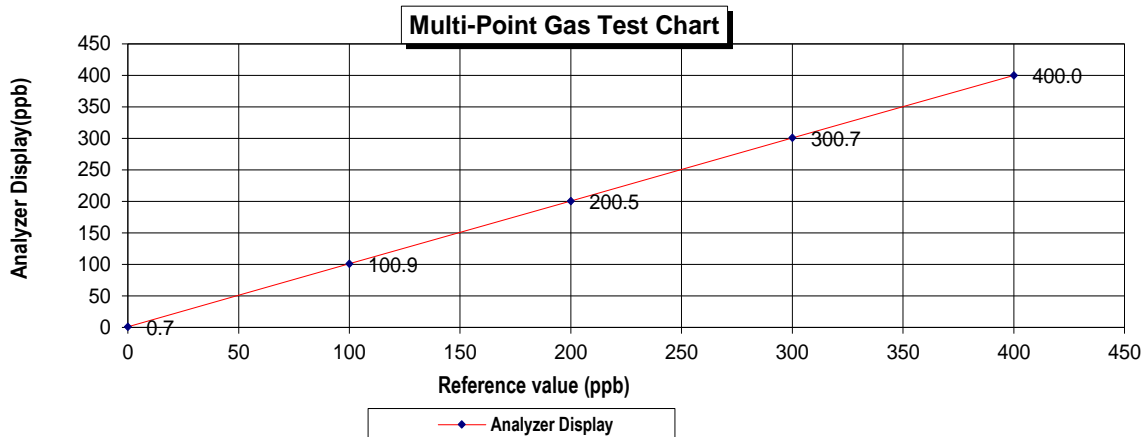

Calculate by

*Grichai. G*

03 / Nov / 2023

Approve by

*Petkarn B.*

03 / Nov / 2023

### MULTI-POINT GAS TEST REPORT

**Test Date** : Nov 9, 2023

**Equipment** : Gas Analyzer (SO<sub>2</sub>)

**Model** : 43i

**Manufacturer** : Thermo SCIENTIFIC

**Serial Number** : 1180540066

#### Standard Gas Concentration


Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 24, 2024

#### Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.7	0.70	0.70	0.70
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.42

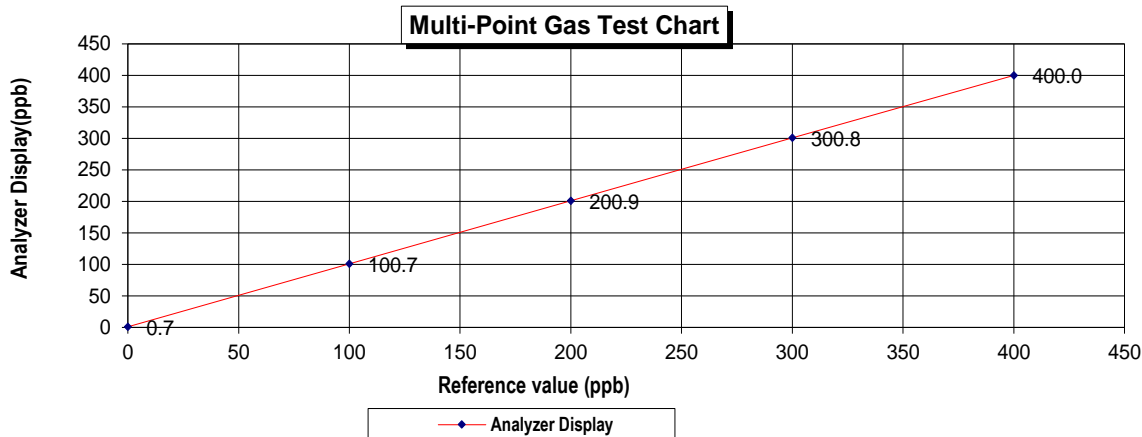

Calculate by

*Girichai C.*  
.....  
9 / 11 / 66

Approve by

*Kitom B.*  
.....  
9 / Nov / 2023

### MULTI-POINT GAS TEST REPORT

**Test Date** : Nov 9, 2023

**Equipment** : Gas Analyzer (SO<sub>2</sub>)

**Model** : 43i

**Manufacturer** : Thermo SCIENTIFIC

**Serial Number** : 1180540067

#### Standard Gas Concentration


Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 24, 2024

#### Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.8	0.80	0.80	0.80
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	201.3	1.30	0.65	0.65
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.48

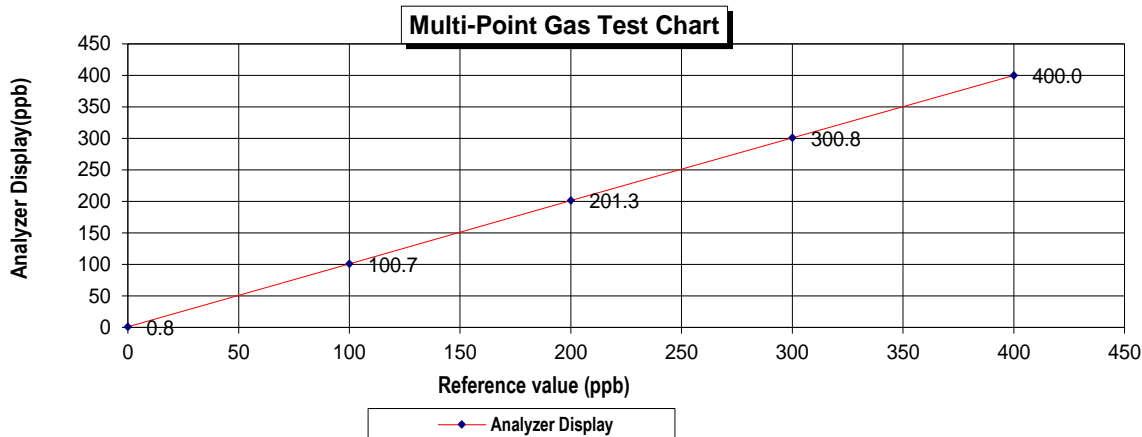

Calculate by

*Grichai. Cy*

.....9...../.....11...../.....66.....

Approve by

*Pattana A.*

.....9...../.....Nov...../.....2023.....



### MULTI-POINT GAS TEST REPORT

**Test Date** : Nov 9, 2023

**Equipment** : Gas Analyzer (SO<sub>2</sub>)

**Model** : 43i

**Manufacturer** : Thermo SCIENTIFIC

**Serial Number** : 1200906876

#### Standard Gas Concentration


Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 24, 2024

#### Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.6	0.60	0.60	0.60
Level 2	20.00%	100.0	100.5	0.50	0.50	0.50
Level 3	40.00%	200.0	201.9	1.90	0.94	0.94
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.46

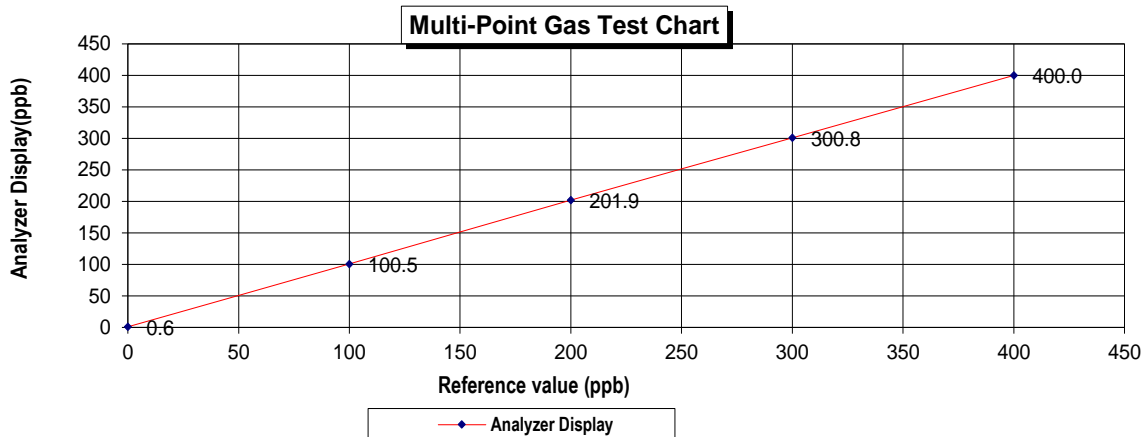

Calculate by

*Grichai. G.*  
.....  
9 / 11 / 66

Approve by

*Petkarn A.*  
.....  
9 / Nov / 2023

# CERTIFICATE OF ANALYSIS

## Grade of Product: EPA Protocol

Part Number:	E04NI99E15A01D3	Reference Number:	122-402135167-1
Cylinder Number:	EB0143262	Cylinder Volume:	144.4 CF
Laboratory:	124 - Durham (SAP) - NC	Cylinder Pressure:	2015 PSIG
PGVP Number:	B22021	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.68 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20061120	CC708068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D685025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505581	4,348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14060119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/-0.6%	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO2	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

*[Signature]*

Approved for Release



CERT 3082.01

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 15 August, 2023

Certification No. 284/23

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : LSI

Type : Dato Logger E-LOG 305 wind speed and wind direction DNA 821

Serial No. : Dato Logger 20070022 wind speed and wind direction 20040186

ID No. : No.16

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1012.5 hPa

### NATIONAL STANDARD WIND TUNNEL :

: Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

### JAPAN QUALITY ASSURANCE ORGANIZATION

Calibrated by : Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Signed :

Mr. Pisood Promsut



(Authorised Signatory)

for the Chief

Sub-Standard Instrument

เอกสารไม่ควบคุม



## THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

### The Result of Calibration

Certification No. 284/23

15 August, 2023

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches	Vacuum inches	Pressure hPa	Velocity m/sec	Correction m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	2.9	0.12
5.00	-	-	-	4.5	0.50
7.04	-	-	-	6.9	0.14
9.02	-	-	-	8.6	0.42
11.01	-	-	-	11.0	0.01
13.01	-	-	-	12.6	0.41
15.01	-	-	-	15.0	0.01
17.02	-	-	-	16.6	0.42
20.02	-	-	-	19.9	0.12

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

*Watcharapol*

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau



เอกสารไม่ควบคุม



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Prakanong, Bangkok 10260

Certificate No : 23-ACT-109  
Request No : Req-2023-1406

### Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1  
Manufacturer : 01dB Range : 94 dB / 1000 Hz  
Model : CAL31 Intrument Status : Used  
Serial Number : 82795  
ID : UAE.EFM.113/2560

### Calibration Environment and Details

Temperature : ( 23 ±2 °C )  
Humidity : ( 50 ± 20 %RH )  
Barometric Pressure : ( 1013 ±10.0 hPa )  
Received Date : 26 June 2023  
Calibration Date : 27 June 2023  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	31 May 2024
THD Multimeter	2015	1047765	NIMT	31 January 2024

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Calibrated By : me  
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By : ปณิศา  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 27 June 2023

Certificate No : 23-ACT-109

Request No : Req-2023-1406

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB)	Acceptance limit Class 1 ( ± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	94.11	0.11	-	-	0.13	0.25

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.08	-	0.40	2.5

Note :

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL23182

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-62 / Microphone UC-59L / Preamplifier NH-26  
**Serial No.:** 00130359 / 02371 / 00390  
**ID No.:** UAE.EFM.105/2556

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 29 MAY 2023  
**Calibration Date :** 07-08 JUNE 2023  
**Date of Issue :** 09 JUNE 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.3	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

## Continuation of Calibration Certificate

Cert. No. : ACL23182  
Job No. : VC66AC0062  
Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	94.0	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	9.5
C - weight	13.9
Flat	23.3

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.3	0.3	0.3	± 1.0
1000	0.1	0.1	0.1	± 0.7
8000	0.1	0.1	0.1	+ 1.5, - 2.5

## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	-0.1	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.0	0.1	+ 1.5, - 2.5
16000	0.0	-1.3	-1.2	+ 2.5, -16.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.1



## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	±0.8
136.0	136.1	0.1	±0.8
135.0	135.1	0.1	±0.8
134.0	134.1	0.1	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8



Continuation of Calibration Certificate

Cert. No. : ACL23182  
Job No. : VC66AC0062  
Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±0.8

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
One	136.4	136.0	-0.4	±2.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	132.9	-0.1	±1.0
Positive half cycle	135.4	135.1	-0.3	±1.0
Negative half cycle	135.4	135.0	-0.4	±1.0

## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACL23033

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-62/ Microphone UC-59L / Preamplifier NH-26  
**Serial No.:** 00391458 / 01748 / 01553  
**ID No.:** -

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 06 JANUARY 2023  
**Calibration Date :** 09 JANUARY 2023  
**Date of Issue :** 16 JANUARY 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL23033

Job No. : VC66AC0023

Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0007-22	04-Feb-23
Waveform Generator	33511B	MY52302742	EF-0008-22	04-Feb-23
Digital Multimeter	33461A	MY53220104	EEL.BP. 04/0265	09-Feb-23
Digital Multimeter	33461A	MY53220076	EEL.BP. 03/0265	09-Feb-23
Digital Multimeter	34461A	MY60024273	EEL.BP. 05/0265	09-Feb-23
Programmable Attenuator	MAT-1070	62100114	EF-0009-22	07-Feb-23
Condenser Microphone	4180	2977900	AA-1013-22	24-Feb-23
Measuring Amplifier	NA-42KAI	34560495	AA-3005-22	22-Feb-23

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



## Continuation of Calibration Certificate

Cert. No. : ACL23033  
Job No. : VC66AC0023  
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.3	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

## Continuation of Calibration Certificate

Cert. No. : ACL23033

Job No. : VC66AC0023

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.95)	94.0	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
15.9

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	11.4
C - weight	16.5
Flat	23.7

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.4	0.4	0.4	± 1.0
1000	0.2	0.2	0.2	± 0.7
8000	-0.6	-0.6	-0.6	+ 1.5, - 2.5

Continuation of Calibration Certificate

Cert. No. : ACL23033  
Job No. : VC66AC0023  
Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	-0.1	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

**5. Frequency and time weightings at 1 kHz**

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	0.0	-
C - weight	94.0	0.0	± 0.2
Flat	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	0.0	-
Slow	94.0	0.0	± 0.1
Leq	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.1



## Continuation of Calibration Certificate

Cert. No. : ACL23033

Job No. : VC66AC0023

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	27.0	0.0	±0.8
26.0	26.0	0.0	±0.8
25.0	25.0	0.0	±0.8



Continuation of Calibration Certificate

Cert. No. : ACL23033  
Job No. : VC66AC0023  
Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±0.8

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
One	136.4	135.7	-0.7	±2.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	-
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

Continuation of Calibration Certificate

Cert. No. : ACL23033

Job No. : VC66AC0023

Pages : 8 of 8

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

**End of Calibration Certificate**



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANILUANG, SUANILUANG BANGKOK 10250  
TEL. 0-2717 3000 29 FAX. 0-2719-9484



Cert.No.: 23CH1226

Page.: 1 of 3

## Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Horiba
Model :	LAQUA-PH210
Serial No. :	HA1G0019
ID No. :	UAE.EFM.202/2564(EFM.pH.10/64)
Condition As-Received:	Used Item
Received Date :	26 September 2023
Calibration Date :	27 September 2023
Reference :	2309-0881WSC-4
Submitted by :	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature :	(25 $\pm$ 2.5) °C
Relative Humidity :	(50 $\pm$ 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Saithip

Approved Signatory

- (☒) Saithip Meangmai  
( ) Warakorn Lerngagtrakul  
( ) Ponpan Paipim

Issue Date : 2 October 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0059073



Cert.No.: 23CH1226

Page.: 2 of 3

**Condition of this calibration result**

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 Jul 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	913598	14 July 2025
pH 6.986	CPA chem	863833	28 Dec 2023
pH 9.997	CPA chem	913600	14 July 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function : mV Measurement**

**Performing standard curve by Fluke at pH (4,7)(7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: HA1G0019	4.00	177.48	177.6	4.01	0.058	2.00
	7.00	0.00	0.2	7.00	0.058	2.00
	7.00	0.00	0.2	7.00	0.058	2.00
	10.00	-177.48	-177.2	10.01	0.058	2.00

Saitip

เอกสารไม่ควบคุม

a 1182400





Cert.No.: 23CH1226

Page.: 3 of 3

**Calibration Results****Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading ( mV )	Uncertainty of pH measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: -	4.008	4.01	141.5	0.0079	2.00
	6.986	6.98	-34.9	0.011	2.00
	6.986	7.00	-34.2	0.011	2.00
	9.997	10.01	-205.7	0.0085	2.00

**Function : Temperature Measurement**

(\*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652

- Serial No. : -

Dimension of probe;

- Length : 103 mm

- Diameter : 16 mm

- Immersion Depth : 90 mm

Calibration Point ( $^{\circ}\text{C}$ )	Standard Temperature ( $^{\circ}\text{C}$ )	UUC* Reading ( $^{\circ}\text{C}$ )	Error ( $^{\circ}\text{C}$ )	Uncertainty of measurement ( $\pm$ $^{\circ}\text{C}$ )	Coverage factor $k$
25.0	25.002	25.0	-0.002	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00
35.0	35.003	35.0	-0.003	0.13	2.00

Remark : - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

Saitip

เอกสารไม่ควบคุม

a 1182399



**TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)**  
**CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES**


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

**Cert.No.:** 23TW219

**Page.:** 1 of 2

## Certificate of Testing

<b>Equipment :</b>	DO Meter
<b>Manufacturer :</b>	Horiba
<b>Model :</b>	LAQUA-DO210
<b>Serial No. :</b>	HE1D0008
<b>ID No. :</b>	UAE.EFM.207/2564(EFM.DO.09/64)
<b>Received Date :</b>	26 September 2023
<b>Test Date :</b>	27 September 2023
<b>Reference :</b>	2309-0884WSC-3
<b>Submitted by :</b>	United Analyst and Engineering Consultant Co.,Ltd. 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
<b>Laboratory Condition :</b>	Temperature ( $25 \pm 5$ ) °C Humidity ( $50 \pm 20$ ) %
<b>Test Procedure :</b>	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
<b>Tested by :</b>	Walalak Sirithean
<b>Approved by :</b>	 Approved Signatory
( <input checked="" type="checkbox"/> ) Saithip Meangmai	
( <input type="checkbox"/> ) Warakorn Lerngagtrakul	
( <input type="checkbox"/> ) Ponpan Paipim	
<b>Issue Date :</b>	29 September 2023

**เอกสารไม่ควบคุม**

B 0325261



Cert.No.: 23TW219

Page.: 2 of 2

**Condition of this result of calibration**

**1. Reference Standard Instruments :**

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1124013382	140RC006	23MM18	20 Feb 2024

**2. Standard Material :-**

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

**Result :** Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 9K1B0020

<b>Titration Method (Azide Modification Method) (mg/L)</b>	<b>DO Meter Reading (mg/L)</b>	<b>Standard Deviation (mg/L)</b>
8.16	8.16	0.0071

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency. The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Saithep

เอกสารไม่ควบคุม

a 1182622



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23LM168

Page.: 1 of 2

## Certificate of Calibration

**Equipment :** DO Meter with Sensor

**Manufacturer :** Horiba

**Model :** LAQUA-DO210

**Serial No. :** HE1D0008

**ID No. :** UAE.EFM.207/2564(EFM.DO.09/64)

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** TPA Chemistry Calibration Laboratory

**Received Order :** 25 September 2023

**Calibrated Date :** 29 September 2023

**Ambient Temperature :** (  $26 \pm 10$  ) °C

**Relative Humidity :** (  $50 \pm 30$  ) %

**AC Line Voltage :** (  $220 \pm 22$  ) V

**Calibrated by :** Krisda Malee

**Approved by :**

  
Approved Signatory

( ) Pornthippa Tameyakul  
( ) Ponpan Paipim  
(✓) Suwit Imjai

**Issue Date :** 5 October 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0059010





**Equipment :** DO Meter with Sensor  
**Condition As-Received :** Used Item  
**Reference :** 2309-0884WSC-4  
**Procedure Used :-**

**Cert. No.:** 23LM168

**Page.:** 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer ( IPRT ) into Temperature Bath.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	2211285	TPA	21 Oct 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function :** Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 18F100252

<u>Calibration Point</u> ( °C )	<u>Immersion Depth</u> ( mm )	<u>Standard Temperature</u> ( °C )	<u>UUC* Reading</u> ( °C )	<u>Error</u> ( °C )	<u>Uncertainty</u> ( ± °C )	<u>Coverage Factor</u> <i>k</i>
25.0	100	25.004	24.8	-0.204	0.16	2.00
30.0	100	30.000	29.8	-0.200	0.16	2.00
35.0	100	34.998	34.8	-0.198	0.16	2.00

**UUC\* :** Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

*Signature*

**เอกสารไม่ควบคุม**

a 1183569



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH1571

Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Conductivity Meter  
**Manufacturer :** Horiba  
**Model :** LAQUA-EC210  
**Serial No. :** HC0J0020  
**ID No. :** UAE.EFM.078/2564(EFM.SCT.04/64)  
**Condition As-Received:** Used Item  
**Received Date :** 13 December 2023  
**Calibration Date :** 14 December 2023  
**Reference :** 2312-0277WSC-2  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260  
**Ambient Temperature :**  $(25 \pm 2.5) ^\circ\text{C}$   
**Relative Humidity :**  $(50 \pm 15) \%$   
**Calibration Procedure:** In-house method :  
- CP-CH6 by direct measurement  
with certified reference material (CRM)  
- CP-CH8 by comparison with standard thermometer

**Calibrated by :** Walalak Sirithean

**Approved by :**

*Saithip*

Approved Signatory

- ☒ Saithip Meangmai  
☐ Warakorn Lerngagtrakul  
☐ Ponpan Paipim

**Issue Date :** 18 December 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Cert.No.: 23CH1571

Page.: 2 of 3

**Condition of this result of calibration**

**1. Reference Standard Instrument :-**

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	9549224	130RC003	23I435	10 Apr 2024
2) Ref. Std.Thermometer	4982054	110RC044	23I908	26 July 2024

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

**2. Certified Reference Materials :-**

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
1413.0 $\mu\text{S/cm}$	CPA Chem	931955	30 Sep 2024
12.880 mS/cm	CPA Chem	913597	14 July 2024

- Control Conductivity calibration solution temperature by Water bath ( $25 \pm 0.1$ )  $^{\circ}\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration results**

**Function : Conductivity Measurement**

**(\*) After Adjustment at 1413.0  $\mu\text{S/cm}$**

**Conductivity Electrode Serial No.: 9B0K0167**

<b>Standard Conductivity Solution</b>	<b>Before Adjustment UUC* Reading</b>	<b>After Adjustment UUC* Reading</b>	<b>Uncertainty of Measurement (<math>\pm</math>)</b>	<b>Coverage factor k</b>
1413.0 $\mu\text{S/cm}$	1402 $\mu\text{S/cm}$	1413 $\mu\text{S/cm}$	9.2 $\mu\text{S/cm}$	2.00
12.880 mS/cm	12.30 mS/cm	12.64 mS/cm	0.086 mS/cm	2.00

**Remark** - UUC\* = Unit Under Calibration

Saitip

เอกสารไม่ควบคุม



Cert.No.: 23CH1571

Page.: 3 of 3

### Calibration Results

**Function : Temperature Measurement**

**(\*) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : 9383  
- Serial No. : 9B0K0167

Dimension of probe;

- Length : 104 mm  
- Diameter : 16 mm  
- Immersion Depth : 90 mm

Calibration Point ( °C )	Standard Temperature ( °C )	UUC* Reading ( °C )	Error ( °C )	Uncertainty of Measurement ( ± °C )	Coverage factor <i>k</i>
25.0	25.001	25.0	-0.001	0.13	2.00
30.0	30.001	30.0	-0.001	0.13	2.00
35.0	35.000	35.1	0.100	0.13	2.00

**Remark : - UUC\* = Unit Under Calibration**

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Sailhip

เอกสารไม่ควบคุม



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Prakanong, Bangkok 10260

Certificate No : 23-ACT-117  
Request No : Req-2023-1546

### Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1  
Manufacturer : SVANTEK Range : 94 , 114 dB / 1000 Hz  
Model : SV 36 Instrument Status : Used  
Serial Number : 107224  
ID : UAE.EFM.171/2564

### Calibration Environment and Details


Temperature : ( 23 ±2 °C )  
Humidity : ( 50 ± 20 %RH )  
Barometric Pressure : ( 1013 ±10.0 hPa )  
Received Date : 21 July 2023  
Calibration Date : 4 August 2023  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	31 May 2024
THD Multimeter	2015	1047765	NIMT	31 January 2024

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 4 August 2023

Certificate No : 23-ACT-117

Request No : Req-2023-1546

**Sound pressure level**

**Calibration Results : Without Adjustment**

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB)	Acceptance limit Class 1 ( ± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	94.03	0.03	-	-	0.13	0.25
114 dB / 1000 Hz	114.11	0.11	-	-	0.13	0.25

**Frequency of Sound pressure level**

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70

**Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)**

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.26	-	0.40	2.5
114 dB / 1000 Hz	0.38	-	0.40	2.5

**Note :**

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

**End of Calibration**

# SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACL23179

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00558037 / 200032 / 47892  
**ID No.:** UAE.EFM.036/2558

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 29 MAY 2023  
**Calibration Date :** 07 -08 JUNE 2023  
**Date of Issue :** 09 JUNE 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL23179

Job No. : VC66AC0062

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



## Continuation of Calibration Certificate

Cert. No. : ACL23179

Job No. : VC66AC0062

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

## Continuation of Calibration Certificate

Cert. No. : ACL23179

Job No. : VC66AC0062

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
15.4

## 2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.2
Flat	24.1

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.0	0.1	0.1	± 1.5
1000	-0.1	-0.1	-0.1	± 1.0
8000	1.6	1.7	1.7	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL23179

Job No. : VC66AC0062

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL23179

Job No. : VC66AC0062

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.1	0.1	$\pm 1.1$
84.0	84.1	0.1	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.1	0.1	$\pm 1.1$
69.0	69.1	0.1	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.1	0.1	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	29.0	0.0	$\pm 1.1$
28.0	28.0	0.0	$\pm 1.1$
27.0	27.0	0.0	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	25.0	0.0	$\pm 1.1$



Continuation of Calibration Certificate

Cert. No. : ACL23179

Job No. : VC66AC0062

Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.4	-1.0	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.1	0.1	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.3	-0.1	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL23179

Job No. : VC66AC0062

Pages : 8 of 8

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.8	89.6	-0.2	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

**End of Calibration Certificate**

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : ACL23131

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00409178 / 185837 / 90624  
**ID No.:** UAE.EFM.017/2564

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 18 APRIL 2023  
**Calibration Date :** 24 -26 APRIL 2023  
**Date of Issue :** 27 APRIL 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL23131

Job No. : VC66AC0048

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



## Continuation of Calibration Certificate

Cert. No. : ACL23131

Job No. : VC66AC0048

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

## Continuation of Calibration Certificate

Cert. No. : ACL23131

Job No. : VC66AC0048

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
14.8

## 2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.1
Flat	23.9

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.3	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	1.3	1.3	1.3	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL23131  
Job No. : VC66AC0048  
Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	-0.1	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL23131

Job No. : VC66AC0048

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	$\pm 1.1$
136.0	136.1	0.1	$\pm 1.1$
135.0	135.1	0.1	$\pm 1.1$
134.0	134.1	0.1	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.1	0.1	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.1	0.1	$\pm 1.1$
114.0	114.1	0.1	$\pm 1.1$
109.0	109.1	0.1	$\pm 1.1$
104.0	104.1	0.1	$\pm 1.1$
99.0	99.1	0.1	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.1	0.1	$\pm 1.1$
28.0	28.0	0.0	$\pm 1.1$
27.0	27.1	0.1	$\pm 1.1$
26.0	26.1	0.1	$\pm 1.1$
25.0	25.1	0.1	$\pm 1.1$



Continuation of Calibration Certificate

Cert. No. : ACL23131

Job No. : VC66AC0048

Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.1	-0.3	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

## Continuation of Calibration Certificate

Cert. No. : ACL23131

Job No. : VC66AC0048

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL23147

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 01010781 / 194536 / 14659  
**ID No.:** UAE.EFM.084/2565

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 MAY 2023  
**Calibration Date :** 08 -09 MAY 2023  
**Date of Issue :** 10 MAY 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL23147

Job No. : VC66AC0053

Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



## Continuation of Calibration Certificate

Cert. No. : ACL23147

Job No. : VC66AC0053

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

## Continuation of Calibration Certificate

Cert. No. : ACL23147

Job No. : VC66AC0053

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise****2.1 Normal test**

Measured Value ( dB )
14.4

**2.2** The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	10.8
C - weight	17.1
Flat	22.8

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.4	0.5	0.5	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL23147

Job No. : VC66AC0053

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL23147

Job No. : VC66AC0053

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	53.9	-0.1	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	38.9	-0.1	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	27.9	-0.1	$\pm 1.1$
27.0	26.9	-0.1	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	24.8	-0.2	$\pm 1.1$



Continuation of Calibration Certificate

Cert. No. : ACL23147  
Job No. : VC66AC0053  
Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

**Continuation of Calibration Certificate**

**Cert. No. : ACL23147**  
**Job No. : VC66AC0053**  
**Pages : 8 of 8**

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

**End of Calibration Certificate**

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 23-NDM-222  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260 Request No : Req-2023-1748

### Unit Under Calibration Details

Measurement item : Noise Dosimeter Microphone Class : 2  
Manufacturer : SVANTEK Microphone Model : SV 27IS  
Model : SV 104IS Microphone S/N : 68647  
Serial Number : 67627 Preamplifier Model : -  
ID : - Preamplifier S/N : -  
Resolution : 0.1 dB Instrument Status : Used

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 21 August 2023  
Calibrated Date : 29 August 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	25 July 2024	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 29 August 2023

Certificate No : 23-NDM-222

Request No : Req-2023-1748

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.18	3.13	-1.57	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 60-140	A	C	(± dB)	(± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.5	0.6	0.40	2.0
125 Hz	-0.8	-0.5	0.40	1.5
250 Hz	-0.4	0.1	0.40	1.5
500 Hz	-0.1	0.3	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.4	0.8	0.40	2.0
4000 Hz	1.5	1.3	0.40	3.0
8000 Hz	-2.0	-1.9	0.40	5.0



Certificate No : 23-NDM-222

Request No : Req-2023-1748

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	60.4	80.4	90.2	100.1	110.0	114.0	120.0	130.0	140.0
	Error	(dB)	0.4	0.4	0.2	0.1	0.0	0.0	0.0	0.0	0.0
8000 Hz	Ref	(dB)				88.9	98.9	108.9	112.9	118.9	128.9
	Level A	(dB)				88.9	98.9	108.9	112.9	118.9	128.8
	Error	(dB)				0.0	0.0	0.0	0.0	-0.1	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	0.99	-1.00		
1000 Hz 110 dB	180	180	2.00	1.98	-1.00		
1000 Hz 120 dB	36	36	4.00	3.94	-1.50		
1000 Hz 120 dB	72	72	8.00	7.87	-1.63	5.6	
1000 Hz 120 dB	90	90	10.00	9.90	-1.00		
1000 Hz 120 dB	180	180	20.00	19.78	-1.10		
1000 Hz 120 dB	360	360	40.00	39.42	-1.45		
1000 Hz 120 dB	720	720	80.00	79.18	-1.02		

Certificate No : 23-NDM-222  
 Request No : Req-2023-1748

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error	(Pa <sup>2</sup> h)	Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)		(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	0.98	-0.02		-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error	(%)	Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)		(%)
Burst 1 ms, 95 dB	2846	2846	1.00	0.98	-2.00		-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	0.98	-2.00	5.6	-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	0.99	-1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances
FAST / A / 60-140	UUC	UUC	Different		Limit
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.13	0.00	3.7	-21 - +26
Continuous Rectangle -		10.13			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-089

Request No : Req-2023-0902

### Unit Under Calibration Details

Measurement item : Noise Dosimeter  
Manufacturer : SVANTEK  
Model : SV 104IS  
Serial Number : 128363  
ID : -  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : SV 27IS  
Microphone S/N : 133706  
Preamplifier Model : -  
Preamplifier S/N : -  
Instrument Status : New

### Calibration Environment and Details


Temperature :  $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$   
Humidity :  $50\% \text{RH} \pm 20\% \text{RH}$   
Barometric Pressure :  $1013 \text{ hPa} \pm 10 \text{ hPa}$   
Received Date : 25 April 2023  
Calibrated Date : 8 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 8 May 2023

Certificate No : 23-NDM-089

Request No : Req-2023-0902

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.13	-1.88	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 60-140	A	C	(± dB)	(± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.4	0.5	0.40	2.0
125 Hz	0.3	0.8	0.40	1.5
250 Hz	0.1	0.6	0.40	1.5
500 Hz	0.1	0.5	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	-0.5	-0.1	0.40	2.0
4000 Hz	0.8	1.0	0.40	3.0
8000 Hz	-1.0	-1.0	0.40	5.0



Certificate No : 23-NDM-089

Request No : Req-2023-0902

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High										
1000 Hz	Ref	(dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0	
	Level A	(dB)	60.4	80.4	90.1	100.0	110.0	114.0	120.0	130.0	139.9	
	Error	(dB)	0.4	0.4	0.1	0.0	0.0	0.0	0.0	0.0	-0.1	
8000 Hz	Ref	(dB)			88.9	98.9	108.9	112.9	118.9	128.9	138.9	
	Level A	(dB)			88.9	98.9	108.9	112.9	118.9	128.8	138.8	
	Error	(dB)			0.0	0.0	0.0	0.0	0.0	-0.1	-0.1	
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8	
	Level A	(dB)						87.8	93.8	103.8	113.8	
	Error	(dB)						0.0	0.0	0.0	0.0	
Tolerances Limit		(±dB)	1.0									
UNCERTAINTY		(±dB)	0.3									

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> ·h)	(Pa <sup>2</sup> ·h)	(%)	(%)	(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	0.99	-1.00		
1000 Hz 110 dB	180	180	2.00	1.98	-1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	5.6	
1000 Hz 120 dB	90	90	10.00	10.13	+1.30		
1000 Hz 120 dB	180	180	20.00	20.22	+1.10		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

Certificate No : 23-NDM-089

Request No : Req-2023-0902

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	0.98	-0.02	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	0.98	-2.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	0.98	-2.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	0.99	-1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	UUC	UUC	Different		
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	28	10.13	0.00	3.7	-21 - +26
Continuous Rectangle -		10.13			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-097

Request No : Req-2023-0902

### Unit Under Calibration Details

Measurement item : Noise Dosimeter  
Manufacturer : SVANTEK  
Model : SV 104IS  
Serial Number : 128477  
ID : -  
Resolution : 0.1 dB

Microphone Class : 2  
Microphone Model : SV 27IS  
Microphone S/N : 85456  
Preamplifier Model : -  
Preamplifier S/N : -  
Instrument Status : New

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 25 April 2023  
Calibrated Date : 9 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 9 May 2023

Certificate No : 23-NDM-097

Request No : Req-2023-0902

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.13	-1.88	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 60-140	A	C		
STD Setting	(dB)	(dB)	(± dB)	(± dB)
*63 Hz	0.4	0.5	0.40	2.0
125 Hz	-0.4	0.0	0.40	1.5
250 Hz	-0.5	0.0	0.40	1.5
500 Hz	-0.4	0.0	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.4	0.8	0.40	2.0
4000 Hz	1.4	1.2	0.40	3.0
8000 Hz	-1.9	-1.9	0.40	5.0



Certificate No : 23-NDM-097

Request No : Req-2023-0902

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	59.9	80.1	90.1	100.0	110.0	114.0	120.0	130.0	139.9
	Error	(dB)	-0.1	0.1	0.1	0.0	0.0	0.0	0.0	0.0	-0.1
8000 Hz	Ref	(dB)					88.9	98.9	108.9	112.9	118.9
	Level A	(dB)					88.9	98.9	108.9	112.9	118.9
	Error	(dB)					0.0	0.0	0.0	0.0	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	1.01	+1.00		
1000 Hz 110 dB	180	180	2.00	2.02	+1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	5.6	
1000 Hz 120 dB	90	90	10.00	9.90	-1.00		
1000 Hz 120 dB	180	180	20.00	19.76	-1.20		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

Certificate No : 23-NDM-097

Request No : Req-2023-0902

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	UUC	UUC	Different		
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.37	0.00	3.7	-21 - +26
Continuous Rectangle -		10.37			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-190  
Request No : Req-2023-1548

### Unit Under Calibration Details

Measurement item :	Noise Dosimeter	Microphone Class :	2
Manufacturer :	SVANTEK	Microphone Model :	SV 27IS
Model :	SV 104IS	Microphone S/N :	68643
Serial Number :	67629	Preamplifier Model :	-
ID :	-	Preamplifier S/N :	-
Resolution :	0.1 dB	Intrument Status :	Used

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 21 July 2023  
Calibrated Date : 11 August 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	25 July 2024	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 11 August 2023

Certificate No : 23-NDM-190

Request No : Req-2023-1548

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.18	3.13	-1.57	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 60-140	A	C	( ± dB)	( ± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.2	0.2	0.40	2.0
125 Hz	-0.3	0.0	0.40	1.5
250 Hz	-0.2	0.3	0.40	1.5
500 Hz	0.1	0.5	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.3	0.7	0.40	2.0
4000 Hz	1.2	1.0	0.40	3.0
8000 Hz	-1.7	-1.6	0.40	5.0



Certificate No : 23-NDM-190

Request No : Req-2023-1548

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	59.8	80.0	90.1	100.0	110.0	114.0	120.0	130.0	140.0
	Error	(dB)	-0.2	0.0	0.1	0.0	0.0	0.0	0.0	0.0	0.0
8000 Hz	Ref	(dB)				88.9	98.9	108.9	112.9	118.9	128.9
	Level A	(dB)				88.9	98.9	108.9	112.9	118.9	128.9
	Error	(dB)				0.0	0.0	0.0	0.0	0.0	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	1.01	+1.00		
1000 Hz 110 dB	180	180	2.00	2.02	+1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	5.6	
1000 Hz 120 dB	90	90	10.00	10.13	+1.30		
1000 Hz 120 dB	180	180	20.00	20.22	+1.10		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

Certificate No : 23-NDM-190

Request No : Req-2023-1548

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error	(Pa <sup>2</sup> h)	Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)		(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	0.98	-0.02	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error	5.6	Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)		(%)
Burst 1 ms, 95 dB	2846	2846	1.00	0.98	-2.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	0.98	-2.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	0.99	-1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances
FAST / A / 60-140	UUC	UUC	Different	3.7	Limit
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)		(%)
Continuous Rectangle +	30	10.13	0.00	3.7	-21 - +26
Continuous Rectangle -		10.13			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-096

Request No : Req-2023-0902

### Unit Under Calibration Details

Measurement item :	Noise Dosimeter	Microphone Class :	2
Manufacturer :	SVANTEK	Microphone Model :	SV 27IS
Model :	SV 104IS	Microphone S/N :	68312
Serial Number :	128475	Preamplifier Model :	-
ID :	-	Preamplifier S/N :	-
Resolution :	0.1 dB	Instrument Status :	New

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 25 April 2023  
Calibrated Date : 9 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 9 May 2023

Certificate No : 23-NDM-096

Request No : Req-2023-0902

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.13	-1.88	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 60-140	A	C	(± dB)	(± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.1	0.2	0.40	2.0
125 Hz	-0.7	-0.3	0.40	1.5
250 Hz	-0.6	-0.1	0.40	1.5
500 Hz	-0.4	0.0	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.5	0.9	0.40	2.0
4000 Hz	1.8	1.6	0.40	3.0
8000 Hz	-2.2	-2.2	0.40	5.0



Certificate No : 23-NDM-096

Request No : Req-2023-0902

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	59.9	80.2	90.2	100.1	110.1	114.0	120.1	130.0	140.0
	Error	(dB)	-0.1	0.2	0.2	0.1	0.1	0.0	0.1	0.0	0.0
8000 Hz	Ref	(dB)			88.9	98.9	108.9	112.9	118.9	128.9	138.9
	Level A	(dB)			89.0	98.9	108.9	112.9	118.9	128.9	138.8
	Error	(dB)			0.1	0.0	0.0	0.0	0.0	0.0	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	0.99	-1.00		
1000 Hz 110 dB	180	180	2.00	1.98	-1.00		
1000 Hz 120 dB	36	36	4.00	3.94	-1.50		
1000 Hz 120 dB	72	72	8.00	7.87	-1.63	5.6	
1000 Hz 120 dB	90	90	10.00	9.90	-1.00		
1000 Hz 120 dB	180	180	20.00	19.76	-1.20		
1000 Hz 120 dB	360	360	40.00	39.42	-1.45		
1000 Hz 120 dB	720	720	80.00	78.66	-1.68		

Certificate No : 23-NDM-096

Request No : Req-2023-0902

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time		Exposure Measurement		UNCERTAINTY	Tolerances
FAST / A / 60-140	UUC		UUC	Different		Limit
Calibrator Setting	(s)		(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29		10.13	0.00	3.7	-21 - +26
Continuous Rectangle -			10.13			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 23-NDM-268  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260 Request No : Req-2023-1465

### Unit Under Calibration Details

Measurement item : Noise Dosimeter Microphone Class : 2  
Manufacturer : SVANTEK Microphone Model : SV27  
Model : SV 104 Microphone S/N : 103079  
Serial Number : 110833 Preamplifier Model : -  
ID : - Preamplifier S/N : -  
Resolution : 0.1 dB Instrument Status : Used

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 5 July 2023  
Calibrated Date : 27 October 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	25 July 2024	TSI
Standard Microphone	GRAS	40AN	188273	21 August 2024	GRAS
Sine Generator	Svantek	Svan401	131	9 October 2024	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 27 October 2023

Certificate No : 23-NDM-268

Request No : Req-2023-1465

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.18	3.13	-1.57	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 55-140	A	C	( ± dB)	( ± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.2	0.0	0.40	2.0
125 Hz	-0.1	0.0	0.40	1.5
250 Hz	-0.2	-0.1	0.40	1.5
500 Hz	0.0	0.1	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.2	0.3	0.40	2.0
4000 Hz	2.5	2.5	0.40	3.0
8000 Hz	-3.0	-3.1	0.40	5.0



Certificate No : 23-NDM-268

Request No : Req-2023-1465

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	55.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	54.7	80.5	90.2	100.1	110.0	114.0	120.0	130.0	140.0
	Error	(dB)	-0.3	0.5	0.2	0.1	0.0	0.0	0.0	0.0	0.0
8000 Hz	Ref	(dB)				88.9	98.9	108.9	112.9	118.9	128.9
	Level A	(dB)				88.9	98.9	108.9	112.9	118.8	128.8
	Error	(dB)				0.0	0.0	0.0	0.0	-0.1	-0.2
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.51	+2.00		
1000 Hz 110 dB	90	90	1.00	1.01	+1.00		
1000 Hz 110 dB	180	180	2.00	2.02	+1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	5.6	
1000 Hz 120 dB	90	90	10.00	10.13	+1.30		
1000 Hz 120 dB	180	180	20.00	20.22	+1.10		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

Certificate No : 23-NDM-268

Request No : Req-2023-1465

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error	(Pa <sup>2</sup> h)	Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)		(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error	5.6	Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)		(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances
FAST / A / 55-140	UUC	UUC	Different	3.7	Limit
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)		(%)
Continuous Rectangle +	29	10.37	0.00	3.7	-21 - +26
Continuous Rectangle -		10.37			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 23-NDM-105  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260 Request No : Req-2023-0951

### Unit Under Calibration Details

Measurement item : Noise Dosimeter Microphone Class : 2  
Manufacturer : SVANTEK Microphone Model : SV 27  
Model : SV 104 Microphone S/N : 112804  
Serial Number : 117696 Preamplifier Model : -  
ID : - Preamplifier S/N : -  
Resolution : 0.1 dB Intrument Status : Used

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 4 May 2023  
Calibrated Date : 12 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 12 May 2023



Certificate No : 23-NDM-105

Request No : Req-2023-0951

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.20	+0.31	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 55-140	A	C	(± dB)	(± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.1	0.2	0.40	2.0
125 Hz	-0.8	-0.3	0.40	1.5
250 Hz	-0.4	0.1	0.40	1.5
500 Hz	-0.1	0.3	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	-0.1	0.3	0.40	2.0
4000 Hz	1.7	1.8	0.40	3.0
8000 Hz	-2.2	-2.3	0.40	5.0



Request No : Req-2023-0951

Certificate No : 23-NDM-105

Request No : Req-2023-0951

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances
	UUC	UUC	Different		Limit
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.37	0.00	3.7	-21 - +26
Continuous Rectangle -		10.37			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-091  
Request No : Req-2023-0902

### Unit Under Calibration Details

Measurement item : Noise Dosimeter  
Manufacturer : SVANTEK  
Model : SV 104IS  
Serial Number : 128372  
ID : -  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : SV 27IS  
Microphone S/N : 133718  
Preamplifier Model : -  
Preamplifier S/N : -  
Instrument Status : New

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 25 April 2023  
Calibrated Date : 9 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 9 May 2023

Certificate No : 23-NDM-091

Request No : Req-2023-0902

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.13	-1.88	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 60-140	A	C	(± dB)	(± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.4	0.5	0.40	2.0
125 Hz	0.2	0.6	0.40	1.5
250 Hz	0.1	0.6	0.40	1.5
500 Hz	0.1	0.5	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	-0.3	0.1	0.40	2.0
4000 Hz	0.6	0.8	0.40	3.0
8000 Hz	-1.7	-1.9	0.40	5.0



Certificate No : 23-NDM-091

Request No : Req-2023-0902

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	60.2	80.1	90.1	100.1	110.1	114.0	120.0	130.0	140.0
	Error	(dB)	0.2	0.1	0.1	0.1	0.1	0.0	0.0	0.0	0.0
8000 Hz	Ref	(dB)			88.9	98.9	108.9	112.9	118.9	128.9	138.9
	Level A	(dB)			88.9	98.9	108.9	112.9	118.9	128.8	138.7
	Error	(dB)			0.0	0.0	0.0	0.0	0.0	-0.1	-0.2
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)		(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	0.99	-1.00		
1000 Hz 110 dB	180	180	2.00	1.98	-1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	82.6	
1000 Hz 120 dB	90	90	10.00	9.90	-1.00		
1000 Hz 120 dB	180	180	20.00	19.76	-1.20		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

Certificate No : 23-NDM-091  
 Request No : Req-2023-0902

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	UUC	UUC	Different		
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.37	0.00	3.7	-21 - +26
Continuous Rectangle -		10.37			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-088  
Request No : Req-2023-0902

### Unit Under Calibration Details

Measurement item :	Noise Dosimeter	Microphone Class :	2
Manufacturer :	SVANTEK	Microphone Model :	SV 27IS
Model :	SV 104IS	Microphone S/N :	133702
Serial Number :	128360	Preamplifier Model :	-
ID :	-	Preamplifier S/N :	-
Resolution :	0.1 dB	Instrument Status :	New

### Calibration Environment and Details


Temperature :  $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$   
Humidity :  $50\% \text{RH} \pm 20\% \text{RH}$   
Barometric Pressure :  $1013 \text{ hPa} \pm 10 \text{ hPa}$   
Received Date : 25 April 2023  
Calibrated Date : 8 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 8 May 2023

Certificate No : 23-NDM-088

Request No : Req-2023-0902

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.20	+0.31	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079.

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 60-140	A	C	(± dB)	(± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.2	0.3	0.40	2.0
125 Hz	-0.1	0.4	0.40	1.5
250 Hz	-0.3	0.2	0.40	1.5
500 Hz	-0.2	0.2	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.4	0.8	0.40	2.0
4000 Hz	1.7	1.9	0.40	3.0
8000 Hz	-2.0	-2.2	0.40	5.0



Certificate No : 23-NDM-088

Request No : Req-2023-0902

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High										
1000 Hz	Ref	(dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0	
	Level A	(dB)	59.9	80.0	90.0	100.0	110.0	114.0	120.0	129.9	139.9	
	Error	(dB)	-0.1	0.0	0.0	0.0	0.0	0.0	0.0	-0.1	-0.1	
8000 Hz	Ref	(dB)			88.9	98.9	108.9	112.9	118.9	128.9	138.9	
	Level A	(dB)			88.9	98.9	108.9	112.9	118.9	128.8	138.8	
	Error	(dB)			0.0	0.0	0.0	0.0	0.0	-0.1	-0.1	
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8	
	Level A	(dB)						87.8	93.8	103.8	113.8	
	Error	(dB)						0.0	0.0	0.0	0.0	
Tolerances Limit		(±dB)	1.0									
UNCERTAINTY		(±dB)	0.3									

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> ·h)	(Pa <sup>2</sup> ·h)	(%)		(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	1.01	+1.00		
1000 Hz 110 dB	180	180	2.00	2.02	+1.00		
1000 Hz 120 dB	36	36	4.00	3.94	-1.50		
1000 Hz 120 dB	72	72	8.00	7.87	-1.63	5.6	
1000 Hz 120 dB	90	90	10.00	9.90	-1.00		
1000 Hz 120 dB	180	180	20.00	19.76	-1.20		
1000 Hz 120 dB	360	360	40.00	39.42	-1.45		
1000 Hz 120 dB	720	720	80.00	78.66	-1.68		

Certificate No : 23-NDM-088

Request No : Req-2023-0902

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	0.99	-0.01	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	0.99	-1.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	0.99	-1.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.00	0.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	UUC	UUC	Different		
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.37	0.00	3.7	-21 - +26
Continuous Rectangle -		10.37			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-106

Request No : Req-2023-0952

### Unit Under Calibration Details

Measurement item : Noise Dosimeter  
Manufacturer : SVANTEK  
Model : SV 104  
Serial Number : 117730  
ID : -  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : SV 27  
Microphone S/N : 77362  
Preamplifier Model : -  
Preamplifier S/N : -  
Instrument Status : Used

### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 4 May 2023  
Calibrated Date : 12 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic

### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By : me  
Mr. Noppadon Luangart  
Calibration Officer

Approved By : ปจ  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 12 May 2023

Certificate No : 23-NDM-106

Request No : Req-2023-0952

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.13	-1.88	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 55-140	A	C	( ± dB)	( ± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.3	0.4	0.40	2.0
125 Hz	-0.3	0.2	0.40	1.5
250 Hz	-0.3	0.2	0.40	1.5
500 Hz	-0.2	0.2	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	-0.1	0.3	0.40	2.0
4000 Hz	1.3	1.4	0.40	3.0
8000 Hz	-2.0	-2.1	0.40	5.0





Certificate No : 23-NDM-106

Request No : Req-2023-0952

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	UUC	UUC	Different		
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.37	0.00	3.7	-21 - +26
Continuous Rectangle -		10.37			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-097

Request No : Req-2023-0902

### Unit Under Calibration Details

Measurement item : Noise Dosimeter  
Manufacturer : SVANTEK  
Model : SV 104IS  
Serial Number : 128477  
ID : -  
Resolution : 0.1 dB

Microphone Class : 2  
Microphone Model : SV 27IS  
Microphone S/N : 85456  
Preamplifier Model : -  
Preamplifier S/N : -  
Instrument Status : New

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 25 April 2023  
Calibrated Date : 9 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 9 May 2023

Certificate No : 23-NDM-097

Request No : Req-2023-0902

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.13	-1.88	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 60-140	A	C		
STD Setting	(dB)	(dB)	(± dB)	(± dB)
*63 Hz	0.4	0.5	0.40	2.0
125 Hz	-0.4	0.0	0.40	1.5
250 Hz	-0.5	0.0	0.40	1.5
500 Hz	-0.4	0.0	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.4	0.8	0.40	2.0
4000 Hz	1.4	1.2	0.40	3.0
8000 Hz	-1.9	-1.9	0.40	5.0



Certificate No : 23-NDM-097

Request No : Req-2023-0902

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	59.9	80.1	90.1	100.0	110.0	114.0	120.0	130.0	139.9
	Error	(dB)	-0.1	0.1	0.1	0.0	0.0	0.0	0.0	0.0	-0.1
8000 Hz	Ref	(dB)					88.9	98.9	108.9	112.9	118.9
	Level A	(dB)					88.9	98.9	108.9	112.9	118.9
	Error	(dB)					0.0	0.0	0.0	0.0	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5,6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	1.01	+1.00		
1000 Hz 110 dB	180	180	2.00	2.02	+1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	5,6	
1000 Hz 120 dB	90	90	10.00	9.90	-1.00		
1000 Hz 120 dB	180	180	20.00	19.76	-1.20		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

Certificate No : 23-NDM-097

Request No : Req-2023-0902

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances Limit
FAST / A / 60-140	UUC	UUC	Different		
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.37	0.00	3.7	-21 - +26
Continuous Rectangle -		10.37			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-108

Request No : Req-2023-0954

### Unit Under Calibration Details

Measurement item : Noise Dosimeter  
Manufacturer : SVANTEK  
Model : SV 104  
Serial Number : 117688  
ID : -  
Resolution : 0.1 dB  
Microphone Class : 2  
Microphone Model : SV 27  
Microphone S/N : 112933  
Preamplifier Model : -  
Preamplifier S/N : -  
Instrument Status : Used

### Calibration Environment and Details

Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 4 May 2023  
Calibrated Date : 12 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic

### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By : me  
Mr. Noppadon Luangart  
Calibration Officer

Approved By : ภาวิ  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 12 May 2023

Certificate No : 23-NDM-108

Request No : Req-2023-0954

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.20	+0.31	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances
	A	C		Limit
FAST / 55-140	(dB)	(dB)	( ± dB)	( ± dB)
STD Setting				
*63 Hz	0.0	0.1	0.40	2.0
125 Hz	-0.4	0.1	0.40	1.5
250 Hz	-0.4	0.1	0.40	1.5
500 Hz	-0.2	0.2	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.2	0.6	0.40	2.0
4000 Hz	1.8	1.9	0.40	3.0
8000 Hz	-3.3	-3.4	0.40	5.0



Certificate No : 23-NDM-108

Request No : Req-2023-0954

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	55.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	54.5	80.1	90.1	100.0	110.0	114.0	119.9	129.9	139.9
	Error	(dB)	-0.5	0.1	0.1	0.0	0.0	0.0	-0.1	-0.1	-0.1
8000 Hz	Ref	(dB)					88.9	98.9	108.9	112.9	118.9
	Level A	(dB)					88.9	98.9	108.9	112.9	118.9
	Error	(dB)					0.0	0.0	0.0	0.0	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting							
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	0.99	-1.00		
1000 Hz 110 dB	180	180	2.00	1.98	-1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	5.6	
1000 Hz 120 dB	90	90	10.00	10.13	+1.30		
1000 Hz 120 dB	180	180	20.00	20.22	+1.10		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

Certificate No : 23-NDM-108

Request No : Req-2023-0954

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error	(Pa <sup>2</sup> h)	Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)		(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error	(% )	Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(% )		(% )
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances
FAST / A / 55-140	UUC	UUC	Different	(% )	Limit
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(% )		(% )
Continuous Rectangle +	29	10.37	0.00	3.7	-21 - +26
Continuous Rectangle -		10.37			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-NDM-090

Request No : Req-2023-0902

### Unit Under Calibration Details

Measurement item :	Noise Dosimeter	Microphone Class :	2
Manufacturer :	SVANTEK	Microphone Model :	SV 27IS
Model :	SV 104IS	Microphone S/N :	133712
Serial Number :	128367	Preamplifier Model :	-
ID :	-	Preamplifier S/N :	-
Resolution :	0.1 dB	Instrument Status :	New

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 25 April 2023  
Calibrated Date : 8 May 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	29 June 2023	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 8 May 2023

Certificate No : 23-NDM-090

Request No : Req-2023-0902

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> ·h)	(Pa <sup>2</sup> ·h)	(%)	(%)	Limit
1000 Hz 114 dB	120	120	3.19	3.20	+0.31	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 60-140	A	C		
STD Setting	(dB)	(dB)	(± dB)	(± dB)
*63 Hz	-0.1	0.0	0.40	2.0
125 Hz	0.1	0.5	0.40	1.5
250 Hz	-0.1	0.4	0.40	1.5
500 Hz	0.0	0.4	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	-0.4	0.0	0.40	2.0
4000 Hz	0.9	1.1	0.40	3.0
8000 Hz	-1.9	-2.0	0.40	5.0



Certificate No : 23-NDM-090

Request No : Req-2023-0902

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	60.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	59.8	80.0	90.0	100.1	110.0	114.0	120.0	130.0	140.0
	Error	(dB)	-0.2	0.0	0.0	0.1	0.0	0.0	0.0	0.0	0.0
8000 Hz	Ref	(dB)			88.9	98.9	108.9	112.9	118.9	128.9	138.9
	Level A	(dB)			88.9	98.9	108.9	112.9	118.9	128.8	138.8
	Error	(dB)			0.0	0.0	0.0	0.0	0.0	-0.1	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> ·h)	(Pa <sup>2</sup> ·h)	(%)		(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	0.99	-1.00		
1000 Hz 110 dB	180	180	2.00	1.98	-1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	5.6	
1000 Hz 120 dB	90	90	10.00	10.13	+1.30		
1000 Hz 120 dB	180	180	20.00	20.22	+1.10		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

Certificate No : 23-NDM-090

Request No : Req-2023-0902

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	0.98	-0.02	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 60-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	0.98	-2.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	0.98	-2.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	0.99	-1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances
FAST / A / 60-140	UUC	UUC	Different		Limit
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	28	10.13	0.00	3.7	-21 - +26
Continuous Rectangle -		10.13			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 23-NDM-179  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260 Request No : Req-2023-1488

### Unit Under Calibration Details

Measurement item : Noise Dosimeter Microphone Class : 2  
Manufacturer : SVANTEK Microphone Model : SV 27  
Model : SV 104 Microphone S/N : 139831  
Serial Number : 143225 Preamplifier Model : -  
ID : - Preamplifier S/N : -  
Resolution : 0.1 dB Intrument Status : New

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 12 July 2023  
Calibrated Date : 7 August 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	25 July 2024	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 7 August 2023

Certificate No : 23-NDM-179

Request No : Req-2023-1488

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	Limit
1000 Hz 114 dB	120	120	3.18	3.13	-1.57	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances
FAST / 55-140	A	C	(± dB)	Limit
STD Setting	(dB)	(dB)		(± dB)
*63 Hz	0.0	0.1	0.40	2.0
125 Hz	0.7	0.9	0.40	1.5
250 Hz	0.3	0.8	0.40	1.5
500 Hz	0.3	0.7	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	-0.6	-0.2	0.40	2.0
4000 Hz	2.3	2.4	0.40	3.0
8000 Hz	-2.9	-2.9	0.40	5.0



Certificate No : 23-NDM-179

Request No : Req-2023-1488

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	55.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	54.5	80.1	90.1	100.1	110.0	114.0	120.0	130.0	140.0
	Error	(dB)	-0.5	0.1	0.1	0.1	0.0	0.0	0.0	0.0	0.0
8000 Hz	Ref	(dB)			88.9	98.9	108.9	112.9	118.9	128.9	138.9
	Level A	(dB)			89.0	98.9	108.9	112.9	118.9	128.9	138.8
	Error	(dB)			0.1	0.0	0.0	0.0	0.0	0.0	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)		
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	1.01	+1.00		
1000 Hz 110 dB	180	180	2.00	2.02	+1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	5.6	
1000 Hz 120 dB	90	90	10.00	9.90	-1.00		
1000 Hz 120 dB	180	180	20.00	20.22	+1.10		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

Certificate No : 23-NDM-179

Request No : Req-2023-1488

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances
FAST / A / 55-140	UUC	UUC	Different		Limit
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.37	0.00	3.7	-21 - +26
Continuous Rectangle -		10.37			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 23-NDM-185  
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260 Request No : Req-2023-1488

### Unit Under Calibration Details

Measurement item : Noise Dosimeter Microphone Class : 2  
Manufacturer : SVANTEK Microphone Model : SV 27  
Model : SV 104 Microphone S/N : 136863  
Serial Number : 143231 Preamplifier Model : -  
ID : - Preamplifier S/N : -  
Resolution : 0.1 dB Intrument Status : New

### Calibration Environment and Details


Temperature : 23 °C ± 2 °C  
Humidity : 50 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 12 July 2023  
Calibrated Date : 7 August 2023  
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252 : 2017  
Location of Calibration : Lab Acoustic


### Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	25 July 2024	TSI
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Sine Generator	Svantek	Svan401	131	12 October 2023	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Calibration Officer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 7 August 2023

Certificate No : 23-NDM-185

Request No : Req-2023-1488

### 1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.18	3.13	-1.57	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 58079

### 2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances Limit
FAST / 55-140	A	C	(± dB)	(± dB)
STD Setting	(dB)	(dB)		
*63 Hz	0.0	0.1	0.40	2.0
125 Hz	0.3	0.6	0.40	1.5
250 Hz	0.0	0.5	0.40	1.5
500 Hz	0.1	0.5	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	-0.4	0.0	0.40	2.0
4000 Hz	1.7	1.8	0.40	3.0
8000 Hz	-2.9	-2.9	0.40	5.0



Certificate No : 23-NDM-185

Request No : Req-2023-1488

### 3. Linearity of response to steady signals

#### a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting		FAST / A / High									
1000 Hz	Ref	(dB)	55.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0
	Level A	(dB)	54.6	80.1	90.1	100.0	110.0	114.0	120.0	130.0	140.0
	Error	(dB)	-0.4	0.1	0.1	0.0	0.0	0.0	0.0	0.0	0.0
8000 Hz	Ref	(dB)					88.9	98.9	108.9	112.9	118.9
	Level A	(dB)					88.9	98.9	108.9	112.9	118.8
	Error	(dB)					0.0	0.0	0.0	-0.1	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8	113.8
	Level A	(dB)						87.8	93.8	103.8	113.8
	Error	(dB)						0.0	0.0	0.0	0.0
Tolerances Limit		(±dB)	1.0								
UNCERTAINTY		(±dB)	0.3								

#### b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances  Limit  (%)
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)		
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	0.99	-1.00		
1000 Hz 110 dB	180	180	2.00	1.98	-1.00		
1000 Hz 120 dB	36	36	4.00	3.94	-1.50		
1000 Hz 120 dB	72	72	8.00	7.87	-1.63	5.6	
1000 Hz 120 dB	90	90	10.00	9.90	-1.00		
1000 Hz 120 dB	180	180	20.00	19.76	-1.20		
1000 Hz 120 dB	360	360	40.00	39.42	-1.45		
1000 Hz 120 dB	720	720	80.00	78.66	-1.68		

Certificate No : 23-NDM-185

Request No : Req-2023-1488

#### 4. Response to short duration

##### a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 - +0.41

##### b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		
Calibrator Setting	(s)	(s)	(Pa <sup>2</sup> h)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 - +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 - +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 - +41

#### 5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances Limit
FAST / A / 55-140	UUC	UUC	Different		
Calibrator Setting	(s)	(Pa <sup>2</sup> h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.13	0.00	3.7	-21 - +26
Continuous Rectangle -		10.13			

\* Indicates non accredited

End of Certificate

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

Certificate No : 23-AFM-144

Request No : Req-2023-1509

### Unit Under Calibration Details

Measurement Item : Primary Flow Calibrator  
Manufacturer : TSI  
Model : 4146 Sensor Model : -  
Serial Number : 41462327002 Sensor Serial Number : -  
ID : -  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 18 July 2023  
Calibration Date : 24 July 2023  
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	11 July 2024
Temperature meter	GT 11	12000077	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	7 November 2023


### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor  
Issue Date : 24 July 2023

Certificate No : 23-AFM-144

Request No : Req-2023-1509

Result of Calibration :

Temperature (°C)	Pressure (kPa)	STD (L/min)	UUC (L/min)	Error (L/min)	Uncertainty (L/min)
25.40	100.84	0.020	0.020	0.000	0.001
25.40	100.83	0.050	0.051	0.001	0.003
25.40	100.84	0.101	0.104	0.003	0.003
25.40	100.82	0.203	0.211	0.008	0.006
25.40	100.81	0.506	0.509	0.003	0.007
25.40	100.81	1.004	1.004	0.000	0.014
25.30	100.80	1.707	1.706	-0.001	0.024
25.30	100.81	2.003	2.006	0.003	0.028
25.20	100.80	3.009	3.038	0.029	0.042
25.20	100.79	4.003	4.029	0.026	0.055
25.30	100.79	5.004	5.027	0.023	0.069

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature

Meas = Measurement Condition ref = Standard Condition

\* Indicates non accredited

End of Certificate





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23P1859

Page : 1 of 2

Equipment : Aneroid Barometer  
Manufacturer: Barigo  
Model : -  
Serial No.: -  
ID No.: UAE.ANV.123/2550

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 02 June 2023

Reference: 2305-0919WSC

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

Ambient Temperature: ( 23  $\pm$  2 ) °C

Relative Humidity: ( 50  $\pm$  15 ) %

Atmospheric Pressure: 1007 mbar

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.This result of calibration instrument was in absolute pressure.

5.This instrument was used clean air as pressure media.

6.The certificate is valid only to the item calibrated on date and place of calibration.

7.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew  
Issue Date : 08 June 2023

Approved Signatory :

Attapol P.  
[ ] Phalinee Prabpaipal  
[ ] Sura Suwannasri  
[x] Attapol Panurach

เอกสารไม่ควบคุม  
B 0316959



Cert.No.: 23P1859

Page: 2 of 2

Result of calibration:- Without adjustment

Range : 960 hPa to 1030 hPa

Function:- Absolute Pressure Measurement

Scale Interval : 1 hPa ( The Fifth Estimate )

Increasing Pressure

Applied Pressure (hPa)	958.80	969.94	981.10	991.92	1003.33	1013.39	1024.48	1035.27
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	1.20	0.06	-1.10	-1.92	-3.33	-3.39	-4.48	-5.27

Decreasing Pressure

Applied Pressure (hPa)	1035.27	1023.97	1013.46	1003.54	992.07	981.34	970.00	959.03
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-5.27	-3.97	-3.46	-3.54	-2.07	-1.34	0.00	0.97

The uncertainty of measurement was  $\pm 0.30$  hPa

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.

เอกสารไม่ควบคุม  
a 1165505



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23H1102

Page : 1 of 2

Equipment : Digital Thermo-Hygrometer

Manufacturer: Digicon

Model : TH-02

Serial No.: 395034174

ID No.: UAE.EFM.185/2565

Condition As-Received: Used Item

Received Date: 18 May 2023

Calibration Date: 22 May 2023  
to 24 May 2023

Reference: 2305-0641WSC

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Chilled Mirror Hygrometer	Dew Master	44730	20563A	14 Jun 2023
2) Handheld Thermometer With Sensor	1521	A5A339	2211251	12 Oct 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

- National Institute of Standards and Technology (NIST) , The United States of America
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Kraipop Onrat  
Issue Date : 25 May 2023

Approved Signatory :

-   
☒ Chakrit Waewwanjua  
☐ Pornthippa Tameyakul  
☐ Viporn Tantiyawutti

เอกสารไม่ควบคุม

B 0314980





Cert. No.: 23H1102

Page.: 2 of 2

**Result of Calibration:-**

Without Adjustment

Function:

Humidity Measurement

<u>Reference Temperature</u> (°C)	<u>Standard Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty of Measurement</u> (±%R.H.)
25.0	40.1	40	-0.1	1.3
25.0	50.1	50	-0.1	1.6
25.0	60.0	59	-1.0	1.6
25.0	70.2	68	-2.2	1.6

**Result of Calibration:-**

Without Adjustment

Function:

Temperature Measurement

<u>Standard Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty of Measurement</u> (±°C)
20.014	20.4	0.386	0.42
25.022	25.6	0.578	0.42
30.033	30.2	0.167	0.42
40.000	39.9	-0.100	0.42

**UUC\*** : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor  $k = 2.00$ , providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม  
a 1162979





**Calibration Note**

UUC Adjustment : Not Adjust

Certificate No : 23-TPM-192

Request No : Req-2023-0710

Page : 2/2

**Result of Calibration :**

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	20.032	20.2	- 0.2	0.13
	25.033	25.2	- 0.2	0.13
	30.037	30.2	- 0.2	0.13
	35.038	35.2	- 0.2	0.13
	40.041	40.2	- 0.2	0.13
	45.040	45.2	- 0.2	0.13
	50.043	50.2	- 0.2	0.13
	60.050	60.2	- 0.2	0.13
DRY	20.033	19.8	+ 0.2	0.13
	25.035	24.8	+ 0.2	0.13
	30.034	29.8	+ 0.2	0.13
	35.037	34.8	+ 0.2	0.13
	40.039	39.8	+ 0.2	0.13
	45.042	44.8	+ 0.2	0.13
	50.044	49.9	+ 0.1	0.13
	60.047	59.9	+ 0.1	0.13
GLOBE	20.031	19.8	+ 0.2	0.13
	25.033	24.8	+ 0.2	0.13
	30.036	29.8	+ 0.2	0.13
	35.037	34.8	+ 0.2	0.13
	40.041	39.8	+ 0.2	0.13
	45.043	44.8	+ 0.2	0.13
	50.045	49.9	+ 0.1	0.13
	60.049	59.9	+ 0.1	0.13

End of Certificate

Calibrated By :



Mr. Sittichok Jirapukdeesakun



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

Certificate No : 23-TPM-502

Request No : Req-2023-2230

Page : 1/2

### Unit Under Calibration Details

Calibration Parameter	: Temperature	
Instrument Name	: Thermal Environment Monitor	Range Calibration : 20 °C to 60 °C
Manufacturer	: TSI QUEST	Type of Sensor : RTD
Model	: QT-32	Sensor Diameter (mm) : 4.5
Serial Number	: TPT030008	Calibration Position (mm) : 67.5
Resolution	: 0.1 °C	Instrument Status : Used
ID Number	: UAE.EFM.219/2562	

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 15 %RH  
Received Date : 18 October 2023  
Calibrated Date : 2 November 2023  
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN: 08000057, ID: 02-TPM Which was calibrated on 27 Febuary 2023, Calibration Certificate No. : QR23-0494

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Approved By :

Mr. Noppadon Luangart

Technical Manager

Issue Date :

2 November 2023



**Calibration Note**

UUC Adjustment : Not Adjust

Certificate No : 23-TPM-502

Request No : Req-2023-2230

Page : 2/2

**Result of Calibration :**

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	20.031	20.0	0.0	0.13
	25.033	25.0	0.0	0.13
	30.035	30.0	0.0	0.13
	35.036	35.0	0.0	0.13
	40.040	40.0	0.0	0.13
	45.040	45.0	0.0	0.13
	50.043	50.0	0.0	0.13
	60.047	60.0	0.0	0.13
DRY	20.033	20.1	- 0.1	0.13
	25.036	25.1	- 0.1	0.13
	30.037	30.1	- 0.1	0.13
	35.039	35.1	- 0.1	0.13
	40.039	40.1	- 0.1	0.13
	45.041	45.1	- 0.1	0.13
	50.043	50.1	- 0.1	0.13
	60.045	60.1	- 0.1	0.13
GLOBE	20.032	20.0	0.0	0.13
	25.033	25.0	0.0	0.13
	30.034	30.0	0.0	0.13
	35.035	35.0	0.0	0.13
	40.038	40.0	0.0	0.13
	45.040	45.0	0.0	0.13
	50.043	50.0	0.0	0.13
	60.046	60.0	0.0	0.13

End of Certificate

Calibrated By :

*Sittichok*

Mr. Sittichok Jirapukdeesakul



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT  
CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

Certificate No : 23-LXM-139

Request No : Req-2023-0706

Page : 1/2

### Unit Under Calibration Details

Instrument Name : Digital Lux Meter  
Manufacturer : EXTECH  
Model : 407026  
Serial Number : A056652  
Resolution : 1 lx  
ID Number : UAE.EFM.126/2565

Range Calibration : 2000 , 20000 lx

Intrument Status : Used

### Calibration Environment and Details

Temperature : 25 °C ± 2 °C  
Humidity : 60 %RH ± 20 %RH  
Received Date : 28 March 2023  
Calibrated Date : 20 April 2023

Calibration Procedure : The measurement was done in accordance with CP-LXM-01

Reference Standard : Photometer and Illuminance Sensor, Serial No.: 30662/2, 30592/2, which was calibrated on 11 November 2022,  
Certificate No.: TP-1027-22

Traceability : This Certificate is traceable to International System of Unit (SI) Unit through National Institute of  
Metrology (Thailand)

### Note

The reported uncertainty is based on a standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Approved By :



Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date :

20 April 2023

