

ภาคผนวก จ

เอกสารเทียบเครื่องมือที่ใช้ในการตรวจวิเคราะห์

---

รายการใบรับรองสอบเทียบ/ทวนสอบ เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์คุณภาพน้ำ									
1	Incubator	Coliform Bacteria  Standard Plate Count  E.Coli  Legionella sp.	Binder	KB 400 /  20220000000301	DKSH (Thailand) Ltd.	C31231210	10 Jun 23	8 Jun 24	-
2	Incubator		Binder	KB 400 /  20220000022479	DKSH (Thailand) Ltd.	C31231678	10 Aug 23	8 Aug 24	-
3	Water Bath		Memmert	WB 14 /  L401.0569	Technology Promotion Association  (Thailand-Japan)	23TM1078	10 Jul 23	8 Jul 24	-
4	Water Bath		Memmert	WNB 14 /  L407.0756	Technology Promotion Association  (Thailand-Japan)	23TM1079	10 Jul 23	8 Jul 24	-
5	Auto Clave		ALP	CL-40L /  810010	DKSH (Thailand) Ltd.	C11230106	9 Jun 23	7 Jun 24	-
6	Auto Clave		ALP	CL-40L /  807298	Nationai food institude ministry  of Industry	2304203-001-01	10 Aug 23	8 Aug 24	-
7	Analytical Balance		OHAUS	PX623 /  C236754745	DKSH (Thailand) Ltd.	C01234158	8 Dec 23	6 Dec 24	-

Due Date of Calibration\* : Based on the annual calibration plan. At least 1 time per year.



## Certificate of Calibration

<b>Equipment:</b>	Incubator	<b>Certificate No.:</b>	C31231210
<b>Model:</b>	KB 400	<b>Issued Date:</b>	10 June 2023
<b>Serial No.(or ID):</b>	20220000000301	<b>Job No.:</b>	KSPR2308771
<b>Manufacturer:</b>	Binder	<b>Page:</b>	1 of 3
<b>Condition:</b>	In Condition	<b>Ventilation Valve:</b>	None
<b>Shelves(pc.):</b>	5		

**Customer:** United Analyst and Engineering Consultant Company Limited.  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangckak, Prakanong, Bangkok 10260 Thailand.

**Environment Condition:**

Temperature:	21 °C	±	0.7 °C
Humidity:	58 %RH	±	4.0 %RH
Voltage:	229 VAC	±	1.3 VAC

**Calibration Place:** United Analyst and Engineering Consultant Company Limited.  
3 Soi Udomsuk 41 Sukhumvit Road, (Microbiology Laboratory)  
Bangckak, Prakanong, Bangkok 10260 Thailand.

**Calibration By:** Mr. Amornthep Phumpho

**Calibration Date:** 09 June 2023

**The Method used:** In house method, CAL-WI-16, base on TLAS-G20

**Traceability:** This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.  
Certificate No. C10220023

(Mr. Amornthep Phumpho)

Person in charge


(Mr. Udon Srichana)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

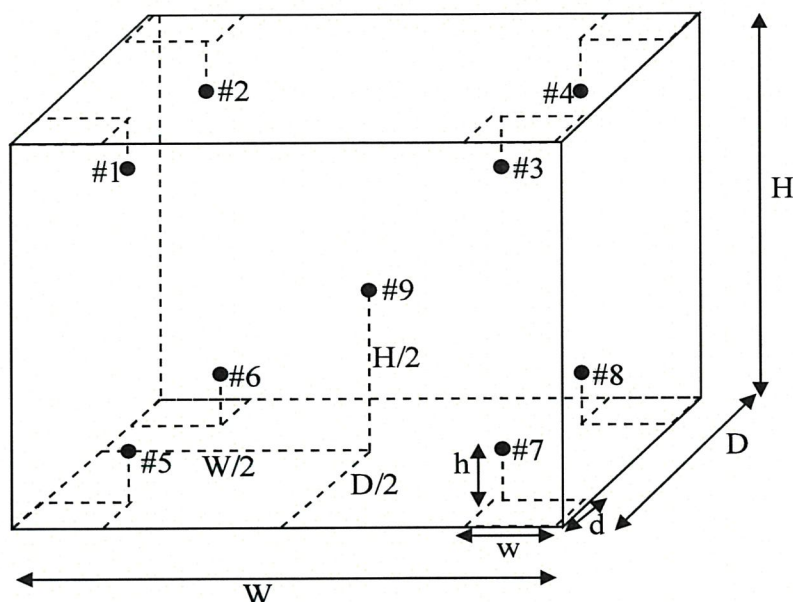

### Standard Installation Locations

Volume (Calibration Zone)= 188 (Liters)

Inside chamber:  $W = 65 \text{ (cm)}$   $D = 48 \text{ (cm)}$   $H = 127 \text{ (cm)}$

Standard Locations (#1, #2, #3, #4):  $w = 7 \text{ (cm)}$   $d = 5 \text{ (cm)}$   $h = 15 \text{ (cm)}$

Standard Locations (#5, #6, #7, #8):  $w = 7 \text{ (cm)}$   $d = 5 \text{ (cm)}$   $h = 15 \text{ (cm)}$

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	1	2	3	4	5	6	7	8	9

### Definitions

**Indicating Temperature:** The average reading of indicating device which forms the integral part of the enclosure.

**Measured Temperature:** The average reading of standards at any positions or location.

**Measured Uniformity:** The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

**Measured Stability:** The one-half of greatest maximum difference of measured temperatures at any one probe.

**Overall Variation:** The difference of maximum and minimum measured temperatures throughout observation time.



## Calibration Results:

### Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 35.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	35.23	0.23	0.23
#2	35.14	0.14	0.23
#3	35.13	0.13	0.23
#4	34.95	-0.05	0.23
#5	35.08	0.08	0.23
#6	35.05	0.05	0.23
#7	34.96	-0.04	0.23
#8	34.79	-0.21	0.23
#9	35.00	0.00	0.23

### Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
35.0	35.0	35.0	35.23	35.14	35.13	34.95	35.08	35.05	34.96	34.79	35.00	0.23

### Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
35.0	0.26	0.06	0.48

Note: \* Maximum uncertainty of the each position

**The End of Certificate**



# Certificate of Calibration

<b>Equipment:</b>	Cooled Incubator	<b>Certificate No.:</b>	C31231678
<b>Model:</b>	KB 400	<b>Issued Date:</b>	10 August 2023
<b>Serial No.(or ID):</b>	20220000022479	<b>Job No.:</b>	WO-00002652
<b>Manufacturer:</b>	Binder	<b>Page:</b>	1 of 3
<b>Condition:</b>	New	<b>Ventilation Valve:</b>	None
<b>Shelves(pc.):</b>	5		

**Customer:** United Analyst and Engineering Consultant Company Limited.  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangckak, Prakanong, Bangkok 10260 Thailand.

**Environment Condition:**

Temperature:	25 °C	±	1.9 °C
Humidity:	49 %RH	±	5.3 %RH
Voltage:	232 VAC	±	1.2 VAC

**Calibration Place:** United Analyst and Engineering Consultant Company Limited. ( Control Area )  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangckak, Prakanong, Bangkok 10260 Thailand.

**Calibration By:** Mr. Thanakrit Raksapol

**Calibration Date:** 07 August 2023

**The Method used:** In house method, CAL-WI-16, base on TLAS-G20

**Traceability:** This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.  
Certificate No. C10230019



(Mr. Thanakrit Raksapol)

Person in charge



(Mr. Udon Srichana)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.


บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

**เอกสารไม่ควบคุม**

CAL-FM-C31-10: 12 Sep 2022



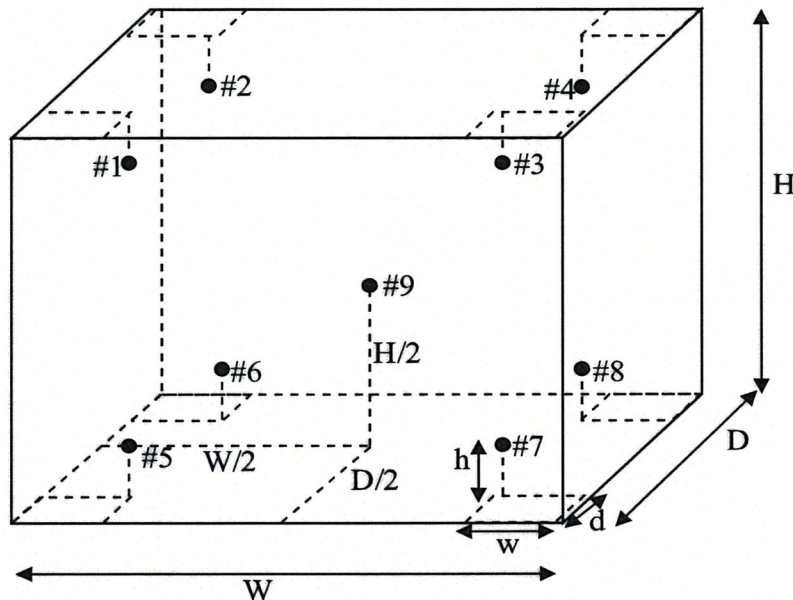

### Standard Installation Locations

Volume (Calibration Zone)= 193 (Liters)

Inside chamber:	W = 65 (cm)	D = 49 (cm)	H = 127 (cm)
Standard Locations (#1, #2, #3, #4):	w = 7 (cm)	d = 5 (cm)	h = 15 (cm)
Standard Locations (#5, #6, #7, #8):	w = 7 (cm)	d = 5 (cm)	h = 15 (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	301	302	303	304	305	306	307	308	309

### Definitions

**Indicating Temperature:** The average reading of indicating device which forms the integral part of the enclosure.

**Measured Temperature:** The average reading of standards at any positions or location.

**Measured Uniformity:** The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

**Measured Stability:** The one-half of greatest maximum difference of measured temperatures at any one probe.

**Overall Variation:** The difference of maximum and minimum measured temperatures throughout observation time.

## Calibration Results:

### Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 35.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	35.11	0.11	0.23
#2	35.04	0.04	0.23
#3	35.03	0.03	0.23
#4	35.13	0.13	0.23
#5	35.02	0.02	0.23
#6	35.07	0.07	0.23
#7	34.97	-0.03	0.23
#8	34.97	-0.03	0.23
#9	35.10	0.10	0.23

### Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
35.0	35.0	35.0	35.11	35.04	35.03	35.13	35.02	35.07	34.97	34.97	35.10	0.23

### Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
35.0	0.16	0.04	0.22

Note: \* Maximum uncertainty of the each position

**The End of Certificate**



## Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The correction of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, TLAS-G20. Therefore, those parameters have not been assessed separately.

### Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ( $w = 0$ ), Specific Risk < 50% PFA.
- ☒ Choice B Non-binary statement with guard band ( $w = 1 U$ ), Pass or Fail Specific Risk < 2.5% PFA and Condition Pass or Condition Fail Specific Risk < 50% PFA.
- ☐ Choice C Customer defined, Customers may define arbitrary multiple of  $r$  to have applied as guard band ( $w = r U$ ) .  
; PFA – Probability of False Accept

(Mr. Udon Srichana)  
Authorized signatory

### Without adjustment

Desired Temperature : 35.0°C Tolerances : 0.5 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 35.0 °C



Locations	Measured (°C)	Correction* (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	35.11	0.11	0.23	0.5	Pass
#2	35.04	0.04	0.23	0.5	Pass
#3	35.03	0.03	0.23	0.5	Pass
#4	35.13	0.13	0.23	0.5	Pass
#5	35.02	0.02	0.23	0.5	Pass
#6	35.07	0.07	0.23	0.5	Pass
#7	34.97	-0.03	0.23	0.5	Pass
#8	34.97	-0.03	0.23	0.5	Pass
#9	35.10	0.10	0.23	0.5	Pass

Correction\* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

### The End of Statements of Conformity



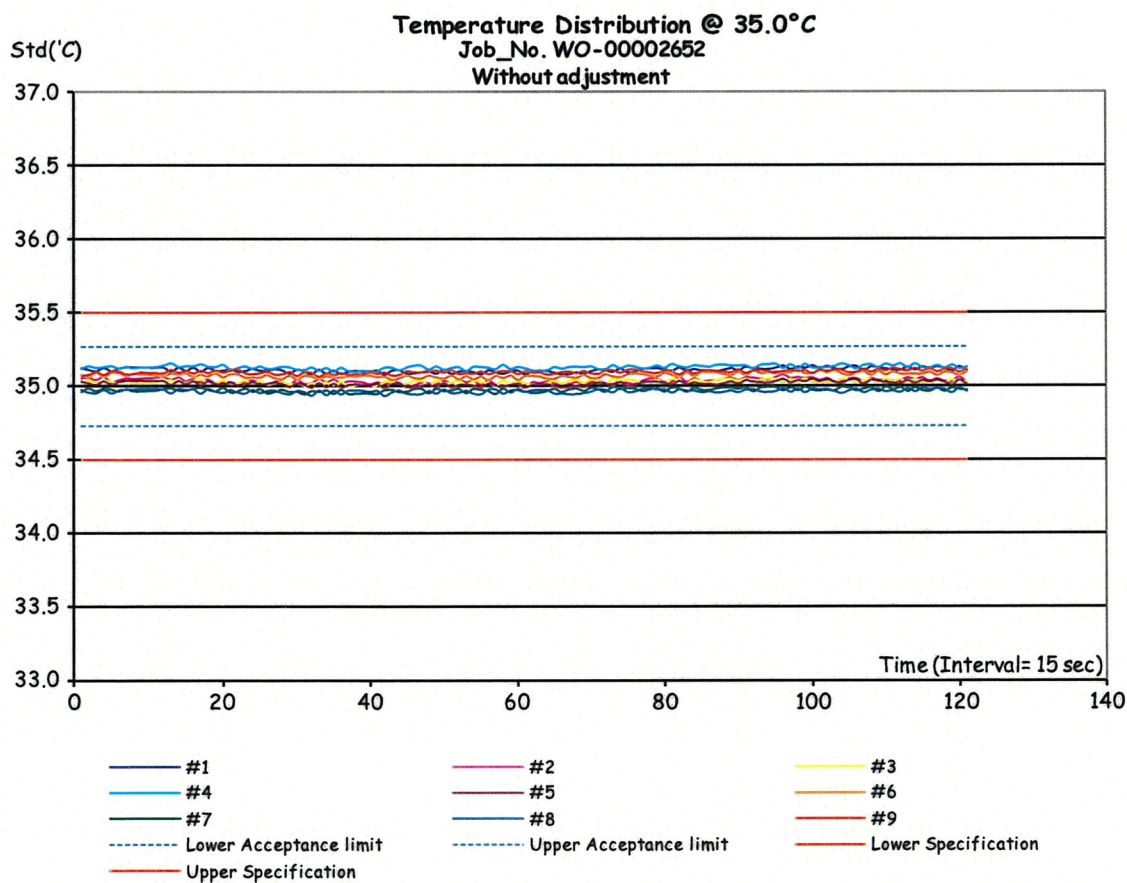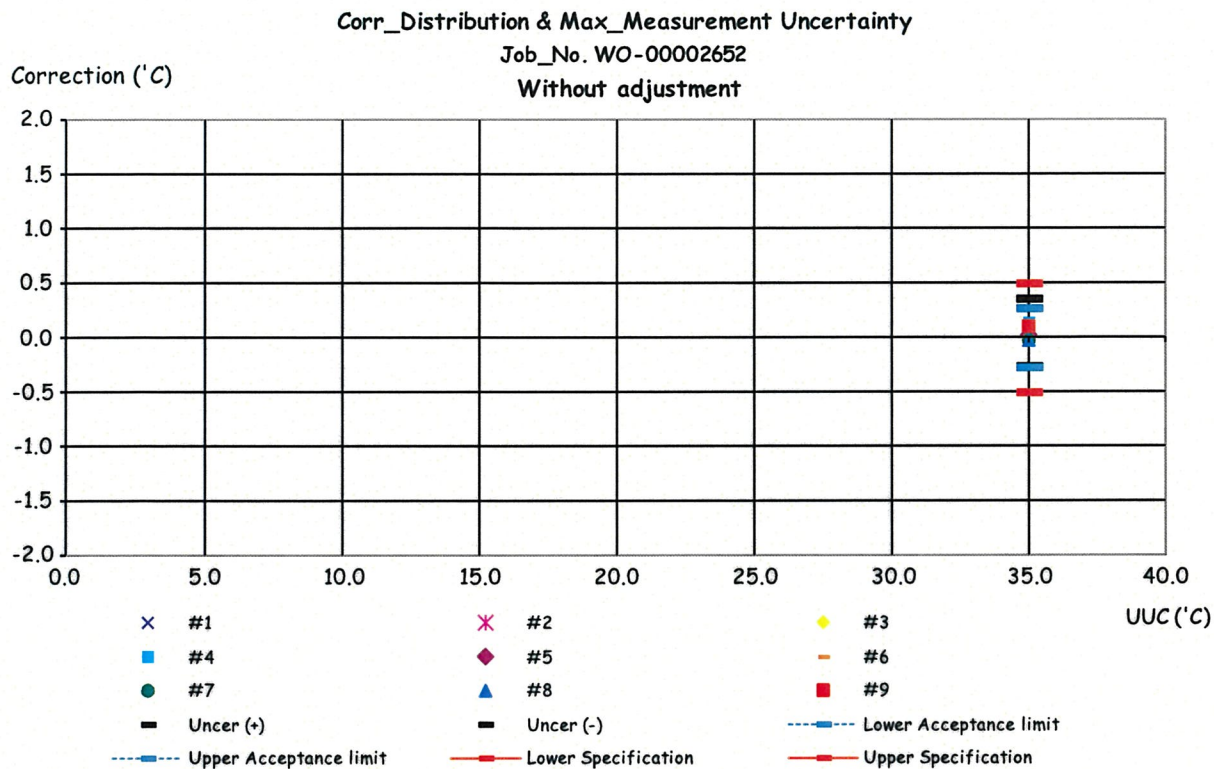

**เอกสารไม่ควบคุม**

## ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: WO-00002652

ชนิดเครื่องมือ: Cooled Incubator

รุ่น: KB 400

หมายเลขเครื่อง: 20220000022479.000

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
07 Aug 2023			07 Aug 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การแสดงผล Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. การทำงาน พัดลม	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	6. สภาพ Lever of Ventilation valve	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สภาพ Lever door open / close	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. สภาพ Door seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานของระบบ Safety	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. การทำงานของระบบทำความเย็น	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	11. การทำงานของระบบทำความร้อน	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. สภาพตัวเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	13. สภาพแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ :

Mr. Thanakrit Raksapol  
Service Engineer





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1078

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Water Bath

**Manufacturer :** Memmert

**Model :** WB 14

**Serial No. :** I401.0569

**ID No. :** UAE.MIC.004/2544

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Microbiology Laboratory

**Received Order :** 10 July 2023  
**Calibration Date :** 10 July 2023  
**Ambient Temperature :** ( 26 ± 10 ) °C  
**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Man Pattanapongpaiboon

**Approved by :**

Approved Signatory

( ) Pornthippa Tameyakul  
( ✓ ) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 20 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0056395





**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2307-0087OC-5

**Cert. No.:** 23TM1078

**Page :** 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY59003411	22LM165	TPA	26 Nov 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	Environmental		AC Voltage Supply
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	25	58	223
Finished of Calibration	25	61	224

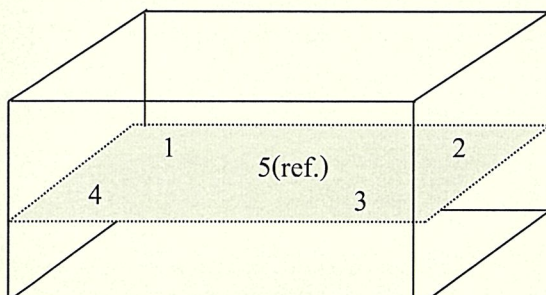

Front

Position :	Ref. Std. ID No.:
1	4804539-001
2	4804539-002
3	4804539-003
4	4804539-004
5(ref.)	4804539-005

เอกสารไม่ควบคุม

a 1172089





Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2307-0087OC-5  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 23TM1078

Page : 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty  ( ± °C )
			Position					
			1	2	3	4	5 (ref.)	
41.5	41.5	41.5	41.438	41.407	41.413	41.331	41.448	0.16

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <i>k</i>
41.5	0.21	0.082	2

**Average\*** : The average of 30 values in each position.

**Uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

a 1172088





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1079

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Water Bath

**Manufacturer :** Memmert

**Model :** WNB 14

**Serial No. :** L407.0756

**ID No. :** UAE.MIC.024/2550

**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong,  
Bangkok 10260

**Location :** Microbiology Laboratory

**Received Order :** 10 July 2023

**Calibration Date :** 10 July 2023

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Man Pattanapongpaiboon

**Approved by :**

Approved Signatory

( ) Pornthippa Tameyakul  
( ✓ ) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 20 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2307-0087OC-6  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 23TM1079

Page : 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty  ( ± °C )
			Position					
			1	2	3	4	5 (ref.)	
44.5	45.0	45.0	44.428	44.374	44.397	44.378	44.387	0.15
45.0	45.5	45.5	44.933	44.878	44.902	44.877	44.902	0.15

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <i>k</i>
44.5	0.084	0.040	2
45.0	0.19	0.076	2

**Average\*** : The average of 30 values in each position.

**Uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่คว



**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2307-0087OC-6

**Cert. No.:** 23TM1079

**Page :** 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY59003411	22LM165	TPA	26 Nov 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	Environmental		AC Voltage Supply
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	25	57	222
Finished of Calibration	25	58	223

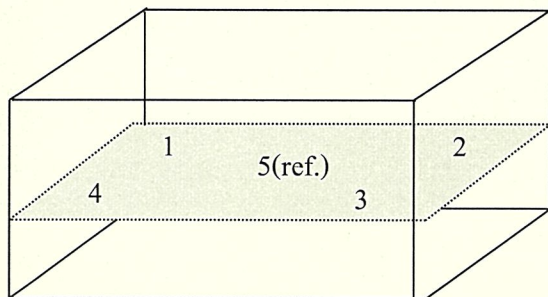

Front

Position :	Ref. Std. ID No.:
1	4804539-001
2	4804539-002
3	4804539-003
4	4804539-004
5(ref.)	4804539-005

เอกสารไม่ค





# Certificate of Calibration

<b>Equipment:</b>	Autoclave	<b>Certificate No.:</b>	C11230106
<b>Model:</b>	CL-40L	<b>Issued Date:</b>	11 June 2023
<b>Serial No. (or ID.):</b>	810010	<b>Job No.:</b>	KSPR2308770
<b>Manufacturer:</b>	ALP	<b>Page:</b>	1 of 4
<b>Condition:</b>	In Condition		

**Customer:** United Analyst and Engineering Consultant Company Limited.  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangkok, Prakanong, Bangkok 10260 Thailand.

**Environment Condition:** Temperature: 22 °C ± 0.8 °C  
Humidity: 58 %RH ± 4.0 %RH  
Voltage: 229 VAC ± 1.3 VAC

**Calibration Place:** United Analyst and Engineering Consultant Company Limited. (301 Room)  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangkok, Prakanong, Bangkok 10260 Thailand.

**Calibration By:** Mr. Amornthep Phumpho

**Calibration Date:** 09 June 2023

**The Method used:** In house method, CAL-WI-18, base on BS 2646 : Part 5

**Traceability:** This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Quality reborn Co., Ltd.  
Certificate No.QR23-0086

  
(Mr. Amornthep Phumpho)

Person in charge


  
(Mr. Udon Srichana)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

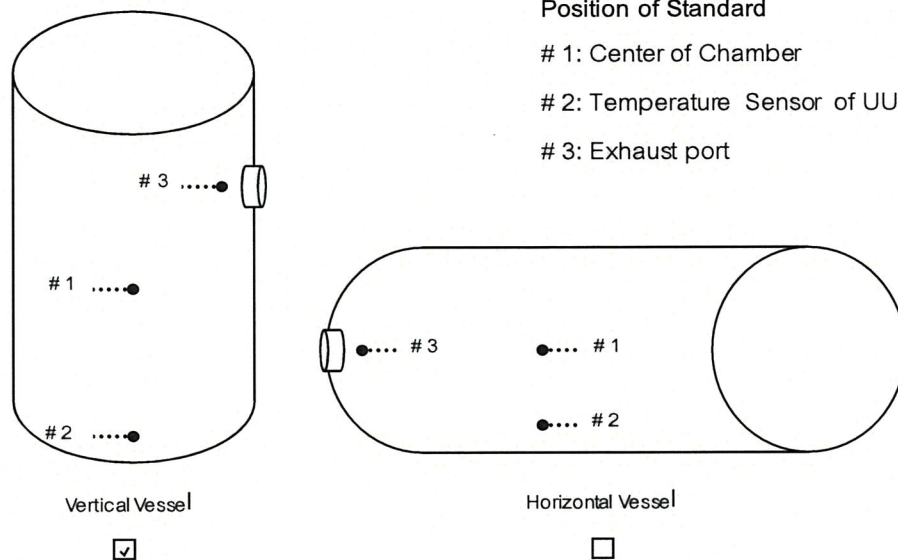

### Standard Installation Locations

- Standard Locations (#1): Geometric center of the chamber
- Standard Locations (#2): Distance from temperature sensor of UUC 2 (cm.)
- Standard Locations (#3): Distance from the wall 5 (cm.)

Position of Std	#1	#2	#3
Channel of Logger	4	5	6

### Definitions

**Indicating Temperature:** The average reading of indicating device which forms the integral part of the enclosure.

**Measured Temperature:** The average reading of standards at any positions or location.

**Measured Stability:** The one-half of greatest maximum difference of measured temperatures at any one probe.



**Calibration Results:**
**Without adjustment**

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 115.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	115.34	0.34	0.35
#2	115.43	0.43	0.35
#3	115.43	0.43	0.35

**Temperature Distribution**

Temperature			Pressure	Measured Temperature at Spread Locations			Uncertainty (± °C)*
Desired (°C)	Setting (°C)	Indicating (°C)	Indicating Mpa	#1 (°C)	#2 (°C)	#3 (°C)	
115	115	115.0	0.08	115.34	115.43	115.43	0.35

**Chamber Characterization**

Indicating Temperature (°C)	Indicating Pressure Mpa	Measured Stability (± °C)
115.0	0.08	0.15

Note: \* Maximum uncertainty of the each position

Record every 10 seconds after reaching steady state or after one achieved complete cycle.

### Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 121.0 °C

Locations	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
#1	121.34	0.34	0.35
#2	121.40	0.40	0.35
#3	121.26	0.26	0.35

### Temperature Distribution

Temperature			Pressure	Measured Temperature at Spread Locations			Uncertainty (± °C)*
Desired (°C)	Setting (°C)	Indicating (°C)	Indicating Mpa	#1 (°C)	#2 (°C)	#3 (°C)	
121	121	121.0	0.12	121.34	121.40	121.26	0.35

### Chamber Characterization

Indicating Temperature (°C)	Indicating Pressure Mpa	Measured Stability (± °C)
121.0	0.12	0.07

Note: \* Maximum uncertainty of the each position

Record every 10 seconds after reaching steady state or after one achieved complete cycle.

**The End of Certificate**

## Calibration Certificate

**Certificate No.:** 2304203-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

**Equipment:** Autoclave  
**Manufacturer:** ALP  
**Model:** CL-40L  
**Serial No.:** 807298  
**ID No.:** UAE.MIC.019/2560  
**Order No.:** 2304203  
**Operation No.:** 2304203-001  
**Date of Receipt:** 10 August 2023  
**Date of Calibration:** 10 August 2023

**Calibrated by** Mr.Worapob Sooktong  
Scientist

**Approved by**

( Mr.Pheraphat Tuanjit )

Manager, Division of Calibration Laboratory

**Date of Issue:** 15 August 2023

Responsible for the Technical Management Team

**The uncertainties are for a confidence probability of approximately 95 %.**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2304203-001-01  
**Equipment:** Autoclave  
 Model: CL-40L Serial No.: 807298  
 Resolution: 1 °C ID No.: UAE.MIC.019/2560  
 Manufacturer: ALP  
**Date of Calibration:** 10 August 2023

Page 2 of 3

**Location:** 301, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Environment Condition:** Ambient Temperature ( 28 ± 1 ) °C  
 Relative Humidity ( 65 ± 2 ) %  
 Line Voltage ( 225 ± 1 ) Volt

### Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard temperature recorder with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1(2021) : Autoclaves for sterilization in laboratories Design, construction, safety and performance Specification.  
 - The temperature scale used was based on ITS - 90.  
 - All data show below were final values and the initial data may be obtained upon request.

### 2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-2	S25601	NC-22-11-22-176	9-Nov-23	MADGETECH INC.
	HiTemp140-2	S25602	NC-22-11-22-175	9-Nov-23	MADGETECH INC.
	HiTemp140-2	R54918	TE 660383-01	8-Apr-24	NATIONAL FOOD INSTITUTE

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good

UUC Description : Setting program function sterilization : STERILIZE/NORMAL

Time of sterilization 15 Minute At 121 °C

8. Result of Calibration : ☒ Without adjustment  
☐ After adjustment



# Calibration Report

**Certificate No.:** 2304203-001-01

**Equipment:** Autoclave

Model: CL-40L

Serial No.: 807298

Resolution: 1 °C

ID No.: UAE.MIC.019/2560

Manufacturer: ALP


**Date of Calibration:** 10 August 2023

Page 3 of 3

**Calibration point:** 121 °C

**Calibration result:**

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	27.0	63.5	223.3
Max	28.3	67.3	225.9

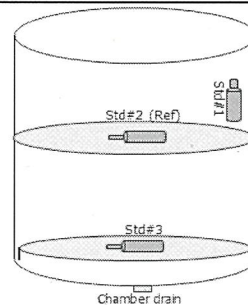

Standard at Position

Std#1 = Attached to the load temperature probe, within 20 mm.  
Std#2 = In the upper half of the chamber  
Std#3 = In the chamber drain, within 100 mm.

**Table1 : Reporting of Temperature**

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
121	121.68	121.70	121.66	0.66

**Table 2 : Reporting of Characterization Result**

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPa			
121	121	121	121	0.10	0.11	0.12	0.23

## Note

The quoted uncertainty include " Stability " and " Loading effect ( 20% of Uniformity )"

UUC\* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.


Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----





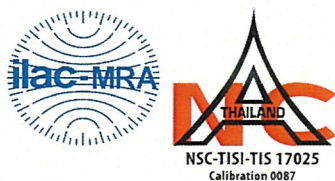

# Certificate of Calibration

<b>Equipment:</b>	Balance	<b>Certificate No.:</b>	C01234158
<b>Model:</b>	PX623	<b>Issued Date:</b>	08 December 2023
<b>Serial No. (or ID.):</b>	C236754745 (UAE.MIC.055/2565)	<b>Job No.:</b>	WO-00011251
<b>Manufacturer:</b>	Ohaus	<b>Page:</b>	1 of 3
<b>Condition:</b>	In condition		

**Customer:** United Analyst and Engineering Consultant Co., Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,  
Phrakhanong District, Bangkok, THAILAND 10260

**Environment Condition:** Temperature 25 °C ± 0.5 °C  
Humidity 54 %RH ± 1.7 %RH

**Calibration Place:** United Analyst and Engineering Consultant Co., Ltd. (301 Microbiology Room)  
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,  
Phrakhanong District, Bangkok, THAILAND 10260

**Calibration By:** Mr. Adisai Maknoi

**Calibration Date:** 07 December 2023

**The Method used:** In-house method, CAL-WI-47, based on UKAS Lab 14

**Traceability:** This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02222534

  
(Mr. Adisai Maknoi)

Person in charge

  
(Mr. Rungrod Jenkitrakulchai)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

## Calibration Results:

### Before Adjustment

**Eccentric Error:** Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

									Nominal Test Value		200	(g)
Reference Points (g)												
A		B		C		D		E				
-		0.000		-0.003		0.000		0.001				

**Repeatability:** Determination of the standard deviation of weighing balance., Readability 0.001 (g)

Nominal test value (g)	Standard Deviation
50	0.0006
500	0.0008


**Error of indication from nominal or conventional mass value.,** Readability 0.001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of Indication (g)	Uncertainty (g)	k
1	1.0000	1.000	0.000	0.0013	2.10
5	5.0001	5.000	0.000	0.0013	2.10
10	10.0001	10.001	0.001	0.0013	2.10
20	20.0000	20.000	0.000	0.0013	2.09
50	50.0001	50.000	0.000	0.0013	2.09
100	100.0001	100.001	0.001	0.0013	2.09
200	200.0004	200.002	0.002	0.0014	2.07
300	300.0005	300.002	0.002	0.0015	2.05
400	400.0006	400.004	0.003	0.0016	2.03
500	500.0006	500.008	0.007	0.0019	2.02
600	600.0007	600.009	0.008	0.0021	2.01



### After Adjustment

**Eccentric Error:** Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

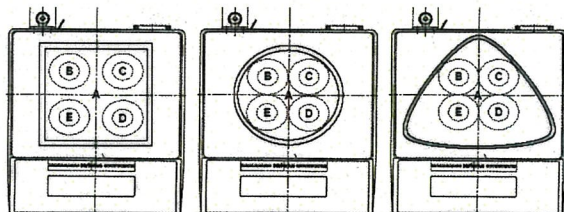

Nominal Test Value 200 (g)

Reference Points (g)				
A	B	C	D	E
-	0.001	-0.002	-0.002	0.001

**Repeatability:** Determination of the standard deviation of weighing balance., Readability 0.001 (g)

Nominal test value (g)	Standard Deviation
50	0.0006
500	0.0008

**Error of indication from nominal or conventional mass value.,** Readability 0.001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of Indication (g)	Uncertainty (g)	k
1	1.0000	1.000	0.000	0.0013	2.10
5	5.0001	5.000	0.000	0.0013	2.10
10	10.0001	10.000	0.000	0.0013	2.10
20	20.0000	20.000	0.000	0.0013	2.10
50	50.0001	50.000	0.000	0.0013	2.10
100	100.0001	100.000	0.000	0.0014	2.09
200	200.0004	200.000	0.000	0.0014	2.07
300	300.0005	300.001	0.001	0.0015	2.05
400	400.0006	400.002	0.001	0.0017	2.04
500	500.0006	500.001	0.000	0.0019	2.02
600	600.0007	600.002	0.001	0.0021	2.01

**The End of Certificate**

## Statements of conformity:


This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The error of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, UKAS Lab14. Therefore, those parameters have not been assessed separately.

### Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ( $w = 0$ ), Specific Risk < 50% PFA.
- ☒ Choice B Non-binary statement with guard band ( $w = 1 U$ ), Pass or Fail Specific Risk < 2.5% PFA and Condition Pass or Condition Fail Specific Risk < 50% PFA.
- ☐ Choice C Customer defined, Customers may define arbitrary multiple of  $r$  to have applied as guard band ( $w = r U$ ).
- ; PFA – Probability of False Accept



(Mr. Rungrod Jenkittrakulchai)

Authorized signatory



**Statements of conformity:****Before Adjustment**

Readability; 0.001 g

Nominal Value g	Error of indication g	Guard band (w) g	Tolerance ( $\pm$ ) g	Conformity
1	0.000	0.0013	0.002	Pass
5	0.000	0.0013	0.010	Pass
10	0.001	0.0013	0.020	Pass
20	0.000	0.0013	0.040	Pass
50	0.000	0.0013	0.100	Pass
100	0.001	0.0013	0.200	Pass
200	0.002	0.0014	0.400	Pass
300	0.002	0.0015	0.600	Pass
400	0.003	0.0016	0.800	Pass
500	0.007	0.0019	1.000	Pass
600	0.008	0.0021	1.200	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

**Statements of conformity:****After Adjustment**

Readability; 0.001 g

Nominal Value g	Error of indication g	Guard band (w) g	Tolerance ( $\pm$ ) g	Conformity
1	0.000	0.0013	0.002	Pass
5	0.000	0.0013	0.010	Pass
10	0.000	0.0013	0.020	Pass
20	0.000	0.0013	0.040	Pass
50	0.000	0.0013	0.100	Pass
100	0.000	0.0014	0.200	Pass
200	0.000	0.0014	0.400	Pass
300	0.001	0.0015	0.600	Pass
400	0.001	0.0017	0.800	Pass
500	0.000	0.0019	1.000	Pass
600	0.001	0.0021	1.200	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

**The End of Statements of conformity**




### Before Adjustment

Job No. WO-00011251

Readability: 0.001g

Error of indication

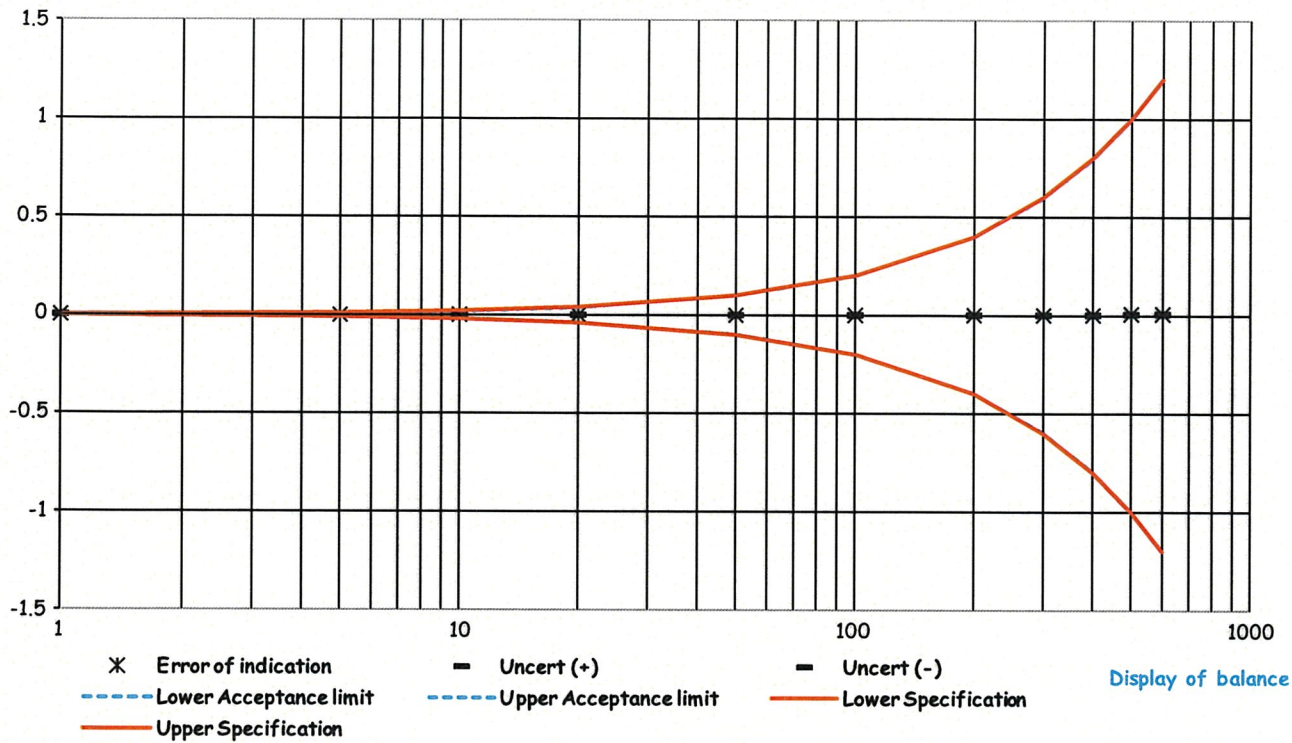


### After Adjust

Job No. WO-00011251

Readability: 0.001g

Error of indication

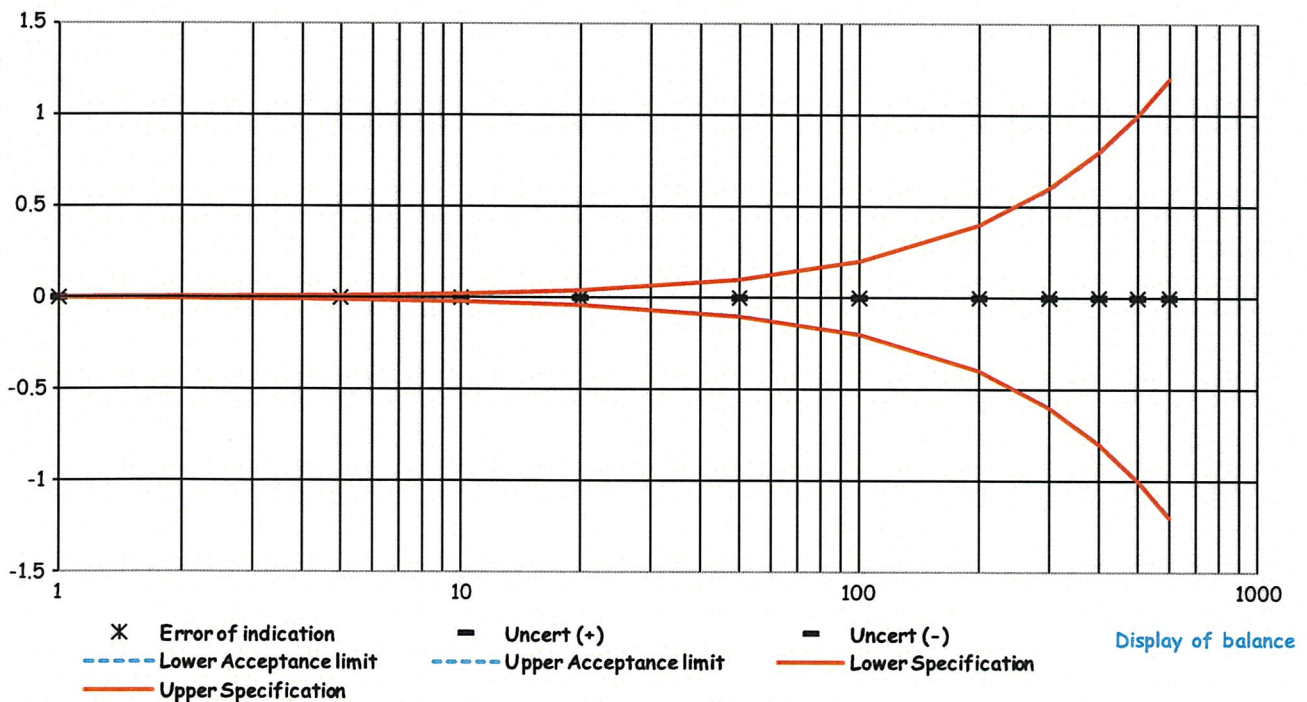

เอกสารไม่ควบคุม

## ใบตรวจสอบสภาพเครื่องชั่ง

เลขที่ใบงาน: WO-00011251

ชนิดเครื่องมือ: Balance

รุ่น: PX623

หมายเลขเครื่อง: C236754745

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
07 Dec 2023			07 Dec 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ/Adapter, power supply 220/110V	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสมบูรณ์ชุดกระจกกันลม (Cover)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. ความสมบูรณ์ชุดของระดับน้ำ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การปรับระดับของขาตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. การตอบสนองของปุ่มกด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. ความสมบูรณ์ของ Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. การแสดงผลของ Display หลังวางน้ำหนัก	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ชุดรองจานชั่ง (Stopper) / pan support	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานของ Function Internal / External	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. ความสะอาดของตัวเครื่องภายนอกและแกน load cell	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. สภาวะแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

หมายเหตุเพิ่มเติม/ข้อแนะนำ :

---



---



---

Mr. Adisai Maknoi

Service Engineer



List of Instruments Certification for Water Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	YSI	Pro 10 18C101710	Technology Promotion Association (Thailand-Japan)	23CH933	26 Jul 23	24 Jul 24	-
2	pH Meter	pH	EcoSense	pH100A JC03354	Technology Promotion Association (Thailand-Japan)	23CH1487	22 Nov 23	20 Nov 24	-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484



NSC-TISI-TIS17025  
CALIBRATION 0008

Cert.No.: 23CH933

Page.: 1 of 3

## Certificate of Calibration

**Equipment :** pH Meter  
**Manufacturer :** YSI  
**Model :** Pro 10  
**Serial No. :** 18C101710  
**ID No. :** UAE.EFM.194/2561(ENV.pH.03/61)  
**Condition As-Received:** Used Item  
**Received Date :** 25 July 2023  
**Calibration Date :** 26 July 2023  
**Reference :** 2307-0790WSC-1  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260  
**Ambient Temperature :** (25 ± 2.5) °C  
**Relative Humidity :** (50 ± 15) %  
**Calibration Procedure :** In - house method :  
- CP-CH5 by direct measurement with standard  
voltage calibrator and direct measurement with  
certified reference material (CRM)  
- CP-CH8 by comparison with standard thermometer

**Calibrated by :** Warakorn Lerngagtrakul

**Approved by :**

Approved Signatory

- ( ) Malee Butkruea  
( ✓ ) Saithip Meangmai  
( ) Warakorn Lerngagtrakul

**Issue Date :** 27 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม





Cert.No.: 23CH933

Page.: 2 of 3

**Condition of this calibration result**

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Ref. Standard Thermometer	A5A339	60RC020	22I1251	11 Oct 2023

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	863832	28 Dec 2024
pH 6.986	CPA chem	863833	28 Dec 2023
pH 10.010	CPA chem	863835	28 Dec 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function : pH Measurement**

**Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)**

<u>Unit Under Calibration</u>	<u>Standard pH Buffer Solution</u>	<u>Actual pH Reading</u>	<u>Actual mV Reading ( mV )</u>	<u>Uncertainty of pH measurement (±)</u>	<u>Coverage factor k</u>
pH Electrode S/N.: 18C100767	4.008	4.01	171.0	0.0079	2.00
	6.986	6.99	-1.3	0.0099	2.00
	6.986	6.99	0.0	0.0099	2.00
	10.010	10.00	-171.0	0.0096	2.00

**Remark** - Can not connect the BNC because the plug does not match with the socket.



Cert.No.: 23CH933

Page.: 3 of 3

### Calibration Results

#### Function : Temperature Measurement

#### ( \* ) Without adjustment

This equipment was connected with Temperature Probe;

- Model : PRO30 COND-T

- Serial No. : 18C100767

Dimension of probe;

- Length : 7 mm

- Diameter : 2.5 mm

- Immersion Depth : 90 mm

Calibration Point ( °C )	Standard Temperature ( °C )	UUC* Reading ( °C )	Error ( °C )	Uncertainty of measurement ( ± °C )	Coverage factor <i>k</i>
25.0	25.004	25.0	-0.004	0.13	2.00
30.0	30.002	30.0	-0.002	0.13	2.00
35.0	35.002	35.0	-0.002	0.13	2.00

Remark : - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

เอก บคม

1177155





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH1487

Page.: 1 of 3

## Certificate of Calibration

**Equipment :** pH Meter  
**Manufacturer :** EcoSense  
**Model :** pH100A  
**Serial No. :** JC03354  
**ID No. :** UAE.EFM.063/2562(ENV.pH 03/62)  
**Condition As-Received:** Used Item  
**Received Date :** 21 November 2023  
**Calibration Date :** 22 November 2023  
**Reference :** 2311-0720WSC-1  
**Submitted by :** United Analyst and Engineering Consultant Co.,Ltd.  
3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260  
  
**Ambient Temperature :** (25 ± 2.5) °C  
**Relative Humidity :** (50 ± 15) %  
**Calibration Procedure :** In - house method :  
- CP-CH5 by direct measurement with standard  
voltage calibrator and direct measurement with  
certified reference material (CRM)  
- CP-CH8 by comparison with standard thermometer

**Calibrated by :** Warakorn Lerngagtrakul

**Approved by :**

Approved Signatory

- (✓) Saithip Meangmai  
( ) Warakorn Lerngagtrakul  
( ) Ponpan Paipim

**Issue Date :** 27 November 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม  
A 0061266



Cert.No.: 23CH1487

Page.: 2 of 3

**Condition of this calibration result**

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	913598	14 July 2025
pH 6.985	CPA chem	913599	14 July 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function : mV Measurement**

**Performing standard curve by Fluke at pH (4,7)(7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: JC03354	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-178	10.01	0.58	2.00





Cert.No.: 23CH1487

Page.: 3 of 3

**Calibration Results****Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading ( mV )	Uncertainty of pH measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 230906SIA605377	4.008	4.01	174	0.0085	2.05
	6.985	7.00	-2	0.0099	2.00
	6.985	7.00	-2	0.0093	2.00
	9.997	10.00	-177	0.0092	2.00

**Function : Temperature Measurement****( \* ) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : -

- Serial No. : 230906SIA605377

Dimension of probe;

- Length : 110 mm

- Diameter : 12 mm

- Immersion Depth : 100 mm

Calibration Point ( $^{\circ}\text{C}$ )	Standard Temperature ( $^{\circ}\text{C}$ )	UUC* Reading ( $^{\circ}\text{C}$ )	Error ( $^{\circ}\text{C}$ )	Uncertainty of measurement ( $\pm$ $^{\circ}\text{C}$ )	Coverage factor $k$
25.0	25.002	25.1	0.098	0.13	2.00
30.0	30.001	30.1	0.099	0.13	2.00
35.0	35.003	35.0	-0.003	0.13	2.00

**Remark : - UUC\* = Unit Under Calibration**

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-