

---

## เอกสารการสอบเทียบความถูกต้องของเครื่องมือ

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
<b>1. คุณภาพอากาศ</b> <u>คุณภาพอากาศในบรรยากาศ</u> - Total Suspended Particulate  - Nitrogen Dioxide  - o-Xylene  - Maleic Anhydride  <u>คุณภาพอากาศจากปล่อง</u> - Total Suspended Particulate  - Oxide of Nitrogen - Carbon Monoxide  - o-Xylene  - Maleic Anhydride  <u>คุณภาพอากาศในสถานประกอบการ</u> - Total Dust  - Octhanol  - Dioctyl Phthalate  - o-Xylene	- High Volume Air Sampler No. B32, B37, B42  - NO <sub>x</sub> Analyzer No. B02, B18, B22  - Personal Pump SKC No. B04, B43, B47, B53, B55  - Rotameter No. L-B05  - Personal Pump SKC No. B01, B04, B06, B10, B12  - Rotameter No. L-B05  - Console No. R05 - Pitot Tube No. B35  - Vacuum Gauge - Personal Pump SKC No. B52 - Rotameter No. H-B08  - Personal Pump SKC No. B74 - Rotameter No. L-B08 - Pitot Tube No. B35  - Personal Pump SKC No. B72 - Rotameter No. H-B08 - Pitot Tube No. B35  - Personal Pump SKC No. B75, R48 - Rotameter No. H-B06, H-B08  - Personal Pump SKC No. B58, R51 - Rotameter No. L-B06, L-B08  - Personal Pump SKC No. B49, B52, B59, B82, R49, R50 - Rotameter No. H-B06, H-B08  - Personal Pump SKC No. B55, R47 - Rotameter No. L-B06, L-B08	- Digital Balance  - NO <sub>x</sub> Analyzer No. B02, B18, B22  - GC/FID  - HPLC Meter  - Digital Balance  - Spectrophotometer - CO Analyzer No. B01  - GC/FID  - HPLC Meter  - Digital Balance  - GC/FID  - GC/FID  - GC/FID

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ต่อ)

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
<b>2. ระดับเสียง</b> <u>ระดับเสียงในบรรยากาศ</u> - $L_{eq}$ 24 hr  <u>ระดับเสียงในสถานประกอบการ</u> - $L_{eq}$ 8 hr และ $L_{max}$  - Noise Dose	- Acoustic Calibrator - Sound Level Meter No. ACO-B41  - Acoustic Calibrator - Sound Level Meter No. ACO-B18, B29, B33, B36 - Acoustic Calibrator - Noise Dosimeter No. NMD-B08, B09, B10	-  -  -
<b>3. คุณภาพน้ำ</b> <u>คุณภาพน้ำทิ้ง</u> - pH - Total Suspended Solids - Total Dissolved Solid - COD - BOD <sub>5</sub> - Grease & Oil <u>คุณภาพน้ำใต้ดินจากบ่อสังเกตการณ์</u> - pH - o-Xylene - Phthalate esters - 2-Ethylhexanol - Total Petroleum Hydrocarbon	- - - - - - - - -	- pH Meter - Digital Balance - Digital Balance - COD Reactor - DO Meter - Digital Balance  - pH Meter - GC/MS - GC/MS - GC/MS - GC/FID
<b>4. ระดับความร้อนในสถานประกอบการ</b> - WBGT	- Heat Stress WBGT Meter No. B30, B31	- Heat Stress WBGT Meter No. B30, B31
<b>5. ระดับความเข้มของแสงสว่างในสถานประกอบการ</b> - Light	- Lux Meter No. B11	-

คุณภาพอากาศ





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ซอยพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10000  
7 Soi Phaholyothin 24, Phaholyothin Rd., Juntong, Chatuchak, Bangkok 10000  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sales@spsc.com, www.spsc.com

High Volume Air Sampler Calibration Report				
Calibration Method : Multipoint Orifice Flow Transfer Standard		Model : TE 5025A	S/N : 3611	
Calibration Data				
High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B01	B01	10/05/2024	y = 1.153x-1.666	1.000
B02	B02	06/05/2024	y = 1.118x+2.367	0.999
B03	B03	06/05/2024	y = 1.188x-5.422	1.000
B04	B04	07/05/2024	y = 1.263x-5.863	0.999
B05	B05	07/05/2024	y = 1.265x-7.057	0.999
B06	B06	09/05/2024	y = 1.213x-4.898	0.997
B07	B07	07/05/2024	y = 1.193x-4.616	0.999
B08	B08	07/05/2024	y = 1.207x-4.482	0.998
B09	B09	06/05/2024	y = 1.216x-4.533	1.000
B10	B10	07/05/2024	y = 1.170x-0.607	1.000
B11	B11	07/05/2024	y = 1.135x-1.256	0.999
B12	B12	07/05/2024	y = 1.211x-4.879	0.997
B13	B13	07/05/2024	y = 1.237x-4.608	1.000
B14	B14	06/05/2024	y = 1.252x-5.906	0.998
B15	B15	09/05/2024	y = 1.192x-2.587	0.999
B16	B16	06/05/2024	y = 1.133x-0.425	0.996
B17	B17	06/05/2024	y = 1.250x-4.910	0.997
B18	B18	06/05/2024	y = 1.181x-4.244	0.998
B19	B19	09/05/2024	y = 1.246x-8.218	0.999
B20	B20	08/05/2024	y = 1.218x-4.223	0.999
B21	B21	08/05/2024	y = 1.189x-4.448	0.998
B22	B22	09/05/2024	y = 1.195x-6.295	0.999
B23	B23	06/05/2024	y = 1.247x-5.137	0.999
B24	B24	09/05/2024	y = 1.157x-1.861	0.998
B25	B25	07/05/2024	y = 1.079x+1.324	1.000
B26	B26	07/05/2024	y = 1.204x-3.730	0.997
B27	B27	07/05/2024	y = 1.140x-2.924	0.999
B28	B28	07/05/2024	y = 1.220x-7.484	0.999
B29	B29	07/05/2024	y = 1.215x-3.783	1.000
B30	B30	10/05/2024	y = 1.198x-3.745	0.998
B31	B31	10/05/2024	y = 1.209x-4.851	1.000
B32	B32	10/05/2024	y = 1.199x-0.772	0.998
B33	B33	10/05/2024	y = 1.237x-4.394	0.997
B34	B34	10/05/2024	y = 1.191x-4.725	0.999
Calibrated by : [Redacted]				



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ซอยพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10000  
7 Soi Phaholyothin 24, Phaholyothin Rd., Juntong, Chatuchak, Bangkok 10000  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sales@spsc.com, www.spsc.com

High Volume Air Sampler Calibration Report				
Calibration Method : Multipoint Orifice Flow Transfer Standard		Model : TE 5025A		S/N : 3611
Calibration Data				
High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B35	B35	06/05/2024	y = 1.193x-4.091	0.999
B36	B36	10/05/2024	y = 1.172x-3.010	0.998
B37	B37	06/05/2024	y = 1.212x-2.568	1.000
B38	B38	06/05/2024	y = 1.187x-3.844	0.997
B39	B39	06/05/2024	y = 1.178x-0.811	0.999
B40	B40	06/05/2024	y = 1.221x-5.480	0.998
B41	B41	06/05/2024	y = 1.219x-4.443	0.997
B42	B42	07/05/2024	y = 1.167x-2.748	0.997
B43	B43	07/05/2024	y = 1.161x-0.034	0.999
B44	B44	07/05/2024	y = 1.249x-4.278	0.999
R01	R01	07/05/2024	y = 1.183x-4.631	0.997
R02	R02	07/05/2024	y = 1.237x-5.919	0.998
R03	R03	07/05/2024	y = 1.234x-7.377	1.000
R04	R04	10/05/2024	y = 1.250x-6.680	0.996
R05	R05	10/05/2024	y = 1.176x-4.403	0.999
R06	R06	06/05/2024	y = 1.195x-4.419	0.999
R07	R07	06/05/2024	y = 1.061x+1.385	0.999
R08	R08	06/05/2024	y = 1.169x-1.426	0.999
R09	R09	06/05/2024	y = 1.150x-0.930	0.998
R10	R10	06/05/2024	y = 1.246x-6.734	0.999
R11	R11	06/05/2024	y = 1.171x-2.938	0.999
R12	R12	10/05/2024	y = 1.149x-3.415	0.998
R13	R13	10/05/2024	y = 1.158x-3.158	0.999
R14	R14	10/05/2024	y = 1.236x-4.390	1.000
R15	R15	06/05/2024	y = 1.229x-7.704	0.998
R16	R16	06/05/2024	y = 1.242x-7.570	0.998
R17	R17	07/05/2024	y = 1.211x-5.039	0.998
R18	R18	07/05/2024	y = 1.226x-5.530	0.999
R19	R19	07/05/2024	y = 1.185x-4.311	0.999
R20	R20	09/05/2024	y = 1.193x-4.417	1.000
Calibrated by : [REDACTED]				

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	10 June 2024	BRAND :	API	MODEL :	200A
NO.	NOX-B02	SERIAL NO.	2409		
Calibrator (Dilution System)					
Brand :	Teledyne	Model :	700		
Last Cal. Date :	30 October 2023	Serial No. :	421		
Reference Standard Gas					
Standard Gas :	Nitric Oxide (NO)	Cylinder No. :	A00726SV		
Certified Date :	05 January 2023	Expired Date :	05 January 2026	Cylinder Conc. :	48.8 ppm
CALIBRATING CONDITION					
Pressure :	1011 mmbar	Temp. :	24.5 °C	% RH :	50
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Diff	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.8	-0.050	400.0	1.008
NO <sub>x</sub> Span	400	400.2	0.050	400.0	1.011
API Model 200A NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	511	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.3	mV	-20 ~ 150		
AZERO	94.1	mV	-20 ~ 150		
HVPS	675	V	420 ~ 900 constant		
RCCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.1	°C	8 ~ 48		
PMT TEMP	7.3	°C	7 ± 2		
MOLY TEMP	314.9	°C	315 ± 5		
RCCELL PRESS	8.2	IN-Hg-A	2 ~ 10 constant		
SAMPLE PRESS	28.4	IN-Hg-A	25 ~ 30 constant		
NO Span Conc	400	PPB	20 ~ 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 ~ 20,000		
NO Slope	1.008	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.011	-	1.0 ± 0.3		
NO Offset	1.5	mV	-20 to +150		
NO <sub>x</sub> Offset	0.9	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	10 June 2024	BRAND :	API	MODEL :	TML-41M
NO.	NOX-B18	SERIAL NO.	N07543		
Calibrator (Dilution System)					
Brand :	Teledyne	Model :	700		
Last Cal. Date :	30 October 2023	Serial No. :	421		
Reference Standard Gas					
Standard Gas :	Nitric Oxide (NO)	Cylinder No. :	A00726SV		
Certified Date :	05 January 2023	Expired Date :	05 January 2026	Cylinder Conc. :	48.8 ppm
CALIBRATING CONDITION					
Pressure :	1011 mmbar	Temp. :	24.5 °C	% RH :	50
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Diff	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	400.1	0.025	400.0	1.010
NO <sub>x</sub> Span	400	400.4	0.100	400.0	1.014
API Model TML-41M NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	509	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.2	mV	-20 ~ 150		
AZERO	93.9	mV	-20 ~ 150		
HVPS	671	V	420 ~ 900 constant		
RCCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	28.8	°C	8 ~ 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	315.4	°C	315 ± 5		
RCCELL PRESS	8.5	IN-Hg-A	2 ~ 10 constant		
SAMPLE PRESS	28.7	IN-Hg-A	25 ~ 30 constant		
NO Span Conc	400	PPB	20 ~ 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 ~ 20,000		
NO Slope	1.010	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.014	-	1.0 ± 0.3		
NO Offset	1.7	mV	-20 to +150		
NO <sub>x</sub> Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 แขวงพญาไท เขตพญาไท กรุงเทพฯ 10000  
Tel : (662) 939-4379-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	10 June 2024	BRAND :	API	MODEL :	TML-41M
NO.	NOX-B22	SERIAL NO.	NO1618		
Calibrator (Dilution System)					
Brand :	Teledyne	Model :	700		
Last Cal. Date :	30 October 2023	Serial No. :	421		
Reference Standard Gas					
Standard Gas :	Nitric Oxide (NO)	Cylinder No. :	A00726SV		
Certified Date :	05 January 2023	Expired Date :	05 January 2026	Cylinder Conc. :	48.8 ppm
CALIBRATING CONDITION					
Pressure	1011 mmbar	Temp.	24.5 °C	% RH	50
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Diff	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.9	-0.025	400.0	1.000
NO <sub>x</sub> Span	400	400.1	0.025	400.0	1.010
API Model TML-41M NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	504	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.0	mV	-20 ~ 150		
AZERO	93.7	mV	-20 ~ 150		
HVPS	673	V	420 ~ 900 constant		
RCCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.3	°C	8 ~ 48		
PMT TEMP	7.5	°C	7 ± 2		
MOLY TEMP	315.1	°C	315 ± 5		
RCCELL PRESS	8.4	IN-Hg-A	2 ~ 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 ~ 30 constant		
NO Span Conc	400	PPB	20 ~ 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 ~ 20,000		
NO Slope	1.006	-	1.0 ± 0.3		
NO <sub>2</sub> Slope	1.010	-	1.0 ± 0.3		
NO Offset	1.4	mV	-20 to +150		
NO <sub>2</sub> Offset	0.9	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibra



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 แขวงพญาไท เขตพญาไท กรุงเทพฯ 10000  
Tel : (662) 939-4379-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report												
Calibration Method : Dry Cal Primary Flowmeter				Model : Defender 510-H			S/N : 136164					
Environmental Conditions												
Temperature		25 ± 3 °C		Pressure		1010 ± 15 mmbar						
Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)			Setting (Q std.)			Value From Calibration Curve	
					1	2	3	1	2	3	y	R <sup>2</sup>
801	SKC	224-PCX04	262101	05/04/2024	1.000	1.500	2.000	993	1.498	1.998	1.001x - 3.430	1.000
802	SKC	224-PCX04	626166	05/04/2024	1.000	1.500	2.000	1.004	1.506	2.000	1.007x - 16.572	0.999
803	SKC	224-PCX04	612968	09/04/2024	1.000	1.500	2.000	997	1.498	2.004	1.008x - 13.756	1.000
804	SKC	224-PCX04	602804	08/04/2024	1.000	1.500	2.000	1.001	1.511	1.993	0.997x + 4.427	1.000
805	SKC	224-PCX04	612695	08/04/2024	1.000	1.500	2.000	1.005	1.510	2.002	1.009x - 16.400	0.999
806	SKC	224-PCX04	262186	08/04/2024	1.000	1.500	2.000	1.003	1.510	2.004	1.005x - 8.687	0.999
807	SKC	224-PCX04	626262	05/04/2024	1.000	1.500	2.000	997	1.500	1.996	0.995x + 4.930	1.000
808	SKC	224-PCX04	626100	04/04/2024	1.000	1.500	2.000	1.003	1.508	2.002	1.011x - 19.679	0.999
809	SKC	224-PCX04	626479	06/04/2024	1.000	1.500	2.000	996	1.499	1.994	0.996x + 3.159	1.000
810	SKC	224-PCX04	091950	04/04/2024	1.000	1.500	2.000	995	1.512	2.000	1.015x - 30.041	0.998
811	SKC	224-PCX04	564315	08/04/2024	1.000	1.500	2.000	994	1.494	2.000	1.006x - 10.717	1.000
812	SKC	224-PCX04	034656	08/04/2024	1.000	1.500	2.000	1.005	1.511	2.002	1.008x - 14.857	0.999
813	SKC	224-PCX04	602073	05/04/2024	1.000	1.500	2.000	998	1.501	1.997	0.998x + 2.728	1.000
814	SKC	224-PCX04	626313	04/04/2024	1.000	1.500	2.000	998	1.491	1.991	0.996x + 4.411	1.000
815	SKC	224-PCX04	626474	04/04/2024	1.000	1.500	2.000	1.004	1.505	2.003	1.009x - 16.951	0.999
816	SKC	224-PCX04	626477	04/04/2024	1.000	1.500	2.000	997	1.502	2.000	1.005x - 13.936	1.000
817	SKC	224-PCX04	626860	05/04/2024	1.000	1.500	2.000	998	1.495	1.990	0.995x + 3.681	1.000
818	SKC	224-PCX04	691804	05/04/2024	1.000	1.500	2.000	1.004	1.506	2.001	1.007x - 12.627	0.999
819	SKC	224-PCX04	691599	08/04/2024	1.000	1.500	2.000	994	1.507	1.997	1.003x - 4.519	1.000
820	SKC	224-PCX04	691587	08/04/2024	1.000	1.500	2.000	993	1.514	1.999	1.013x - 27.943	0.998
821	SKC	224-PCX04	691531	08/04/2024	1.000	1.500	2.000	997	1.498	1.993	0.996x - 1.121	1.000
822	SKC	224-PCX04	691654	08/04/2024	1.000	1.500	2.000	1.002	1.500	2.005	1.013x - 23.316	0.999
823	SKC	224-PCX04	798393	09/04/2024	1.000	1.500	2.000	995	1.506	1.999	1.014x - 26.370	0.999
824	SKC	224-PCX04	626363	04/04/2024	1.000	1.500	2.000	997	1.505	2.003	1.016x - 28.805	0.999
825	SKC	224-PCX04	798489	04/04/2024	1.000	1.500	2.000	1.000	1.494	2.002	0.999x - 1.300	1.000
826	SKC	224-PCX04	798479	05/04/2024	1.000	1.500	2.000	1.001	1.501	1.997	0.998x + 2.010	1.000
827	SKC	224-PCX04	691673	08/04/2024	1.000	1.500	2.000	995	1.505	2.001	1.016x - 28.031	0.999
828	SKC	224-PCX04	691570	08/04/2024	1.000	1.500	2.000	1.004	1.498	2.000	1.007x - 15.352	0.999
829	SKC	224-PCX04	626472	08/04/2024	1.000	1.500	2.000	1.003	1.496	2.003	1.003x - 5.903	1.000
830	SKC	224-PCX04	691489	05/04/2024	1.000	1.500	2.000	1.005	1.511	2.005	1.007x - 8.527	0.999
831	SKC	224-PCX04	691509	08/04/2024	1.000	1.500	2.000	991	1.495	1.998	1.006x - 14.067	1.000
832	SKC	224-PCX04	091567	05/04/2024	1.000	1.500	2.000	993	1.504	1.999	1.013x - 26.659	0.999
833	SKC	224-PCX04	091756	05/04/2024	1.000	1.500	2.000	994	1.503	1.995	1.008x - 2.836	1.000
834	SKC	224-PCX04	612962	08/04/2024	1.000	1.500	2.000	1.004	1.503	2.001	1.006x - 11.343	0.999
835	SKC	224-PCX04	602682	08/04/2024	1.000	1.500	2.000	997	1.496	1.995	0.998x - 2.772	1.000
836	SKC	224-PCX04	626164	05/04/2024	1.000	1.500	2.000	997	1.506	2.000	1.006x - 14.159	0.999
837	SKC	224-PCX04	626256	04/04/2024	1.000	1.500	2.000	997	1.507	1.998	1.010x - 23.269	0.999
838	SKC	224-PCX04	626167	04/04/2024	1.000	1.500	2.000	996	1.496	1.997	1.004x - 7.259	1.000
839	SKC	224-PCX04	034637	04/04/2024	1.000	1.500	2.000	1.007	1.499	2.000	1.003x - 11.120	0.999
840	SKC	224-PCX04	798369	08/04/2024	1.000	1.500	2.000	995	1.506	2.001	1.013x - 26.810	0.999
Calibrated by :												





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 แขวงพญาไท เขตพญาไท กรุงเทพมหานคร 10500  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10500  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25 ± 3 °C  
Pressure : 1010 ± 15 mmbar

Personal Pump Data					Calibration Data							
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B41	SKC	224-PCXR4	612669	05/04/2024	1,000	1,500	2,000	1,001	1,498	1,990	0.994x + 6.342	1.000
B42	SKC	224-PCXR4	626041	04/04/2024	1,000	1,500	2,000	1,006	1,496	1,990	0.984x + 20.844	1.000
B43	SKC	224-PCXR4	034636	04/04/2024	1,000	1,500	2,000	998	1,498	1,989	0.989x + 12.360	1.000
B44	SKC	224-PCXR8	529341	09/04/2024	1,000	1,500	2,000	1,000	1,501	2,002	1.005x - 9.213	1.000
B45	SKC	224-PCXR8	529594	04/04/2024	1,000	1,500	2,000	1,002	1,502	1,989	0.988x + 16.584	1.000
B46	SKC	224-PCXR8	566743	04/04/2024	1,000	1,500	2,000	996	1,507	2,001	1.012x - 24.724	0.999
B47	SKC	224-PCXR8	566747	08/04/2024	1,000	1,500	2,000	1,005	1,500	2,002	1.007x - 16.424	0.999
B48	SKC	224-PCXR8	566753	09/04/2024	1,000	1,500	2,000	998	1,492	1,997	0.998x - 1.157	1.000
B49	SKC	224-PCXR8	566780	08/04/2024	1,000	1,500	2,000	1,004	1,503	2,005	1.009x - 18.040	0.999
B50	SKC	224-PCXR8	500400	04/04/2024	1,000	1,500	2,000	1,003	1,495	2,003	1.000x - 1.783	1.000
B51	SKC	224-PCXR8	500363	04/04/2024	1,000	1,500	2,000	995	1,500	2,002	1.013x - 28.701	0.999
B52	SKC	224-PCXR8	093186	04/04/2024	1,000	1,500	2,000	992	1,494	1,991	0.996x + 6.116	1.000
B53	SKC	224-PCXR8	707670	08/04/2024	1,000	1,500	2,000	1,000	1,502	2,001	1.006x - 16.999	0.999
B54	SKC	224-PCXR3	509821	08/04/2024	1,000	1,500	2,000	996	1,503	2,002	1.015x - 30.009	0.999
B55	SKC	224-PCXR3	510710	05/04/2024	1,000	1,500	2,000	1,000	1,494	1,993	0.995x + 0.963	1.000
B56	SKC	224-PCXR3	511450	09/04/2024	1,000	1,500	2,000	1,004	1,499	2,000	1.002x - 4.651	1.000
B57	SKC	224-PCXR3	510798	08/04/2024	1,000	1,500	2,000	996	1,494	1,998	1.000x - 2.680	1.000
B58	SKC	224-PCXR3	509852	08/04/2024	1,000	1,500	2,000	1,002	1,501	2,000	1.006x - 16.480	0.999
B59	SKC	224-PCXR3	509862	08/04/2024	1,000	1,500	2,000	997	1,501	1,998	0.999x + 1.041	1.000
B60	SKC	224-PCXR3	512655	05/04/2024	1,000	1,500	2,000	1,005	1,507	2,003	1.003x - 4.627	1.000
B61	SKC	224-PCXR3	503915	05/04/2024	1,000	1,500	2,000	993	1,490	2,000	1.004x - 12.823	1.000
B62	SKC	224-PCXR3	505975	05/04/2024	1,000	1,500	2,000	1,001	1,495	1,997	0.995x + 2.616	1.000
B63	SKC	224-PCXR3	511432	05/04/2024	1,000	1,500	2,000	993	1,503	1,999	1.014x - 30.715	0.999
B64	SKC	224-PCXR3	508302	08/04/2024	1,000	1,500	2,000	1,000	1,493	1,987	0.988x + 13.991	1.000
B65	SKC	224-PCXR3	508310	09/04/2024	1,000	1,500	2,000	1,003	1,500	2,003	1.006x - 12.021	1.000
B66	SKC	224-PCXR3	509861	08/04/2024	1,000	1,500	2,000	1,004	1,489	1,990	0.986x + 16.775	1.000
B67	SKC	224-PCXR3	506295	04/04/2024	1,000	1,500	2,000	997	1,506	2,003	1.004x - 9.094	1.000
B68	SKC	224-PCXR3	505872	04/04/2024	1,000	1,500	2,000	1,004	1,490	1,997	0.992x + 7.829	1.000
B69	SKC	224-PCXR3	508373	04/04/2024	1,000	1,500	2,000	1,005	1,500	1,998	1.006x - 13.832	0.999
B70	SKC	224-PCXR3	510623	08/04/2024	1,000	1,500	2,000	995	1,491	1,996	1.000x - 8.938	1.000
B71	SKC	224-PCXR3	508367	08/04/2024	1,000	1,500	2,000	996	1,504	2,000	1.012x - 27.372	0.999
B72	SKC	224-PCXR3	505977	09/04/2024	1,000	1,500	2,000	1,001	1,500	1,995	0.994x + 5.791	1.000
B73	SKC	224-PCXR3	512656	04/04/2024	1,000	1,500	2,000	1,002	1,499	2,002	1.007x - 12.671	1.000
B74	SKC	224-PCXR3	505993	04/04/2024	1,000	1,500	2,000	995	1,495	1,996	1.003x - 9.987	1.000
B75	SKC	224-PCXR3	509820	05/04/2024	1,000	1,500	2,000	998	1,497	1,993	0.997x + 1.432	1.000
B76	SKC	224-PCXR3	509851	05/04/2024	1,000	1,500	2,000	992	1,497	2,000	1.008x - 17.753	1.000
B77	SKC	224-PCXR3	508301	05/04/2024	1,000	1,500	2,000	1,004	1,499	2,001	1.010x - 19.743	0.999
B78	SKC	224-PCXR3	510677	08/04/2024	1,000	1,500	2,000	997	1,505	2,001	1.013x - 27.321	0.999
B79	SKC	224-PCXR3	510920	09/04/2024	1,000	1,500	2,000	995	1,495	1,993	1.006x - 4.702	1.000

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 แขวงพญาไท เขตพญาไท กรุงเทพมหานคร 10500  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10500  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25 ± 3 °C  
Pressure : 1010 ± 15 mmbar

Personal Pump Data					Calibration Data							
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
R01	SKC	224-PCXR4	602467	04/04/2024	1,000	1,500	2,000	994	1,506	2,006	1.009x - 15.012	1.000
R02	SKC	224-PCXR4	626450	04/04/2024	1,000	2,000	3,000	999	1,497	1,989	0.988x + 13.944	1.000
R03	SKC	224-PCXR4	691592	09/04/2024	1,000	1,500	2,000	1,006	1,498	2,005	1.011x - 20.963	0.999
R04	SKC	224-PCXR4	691672	02/04/2024	1,000	1,500	2,000	998	1,491	1,995	0.996x + 0.630	1.000
R05	SKC	224-PCXR4	798470	04/04/2024	1,000	1,500	2,000	995	1,508	1,998	1.010x - 23.496	0.999
R06	SKC	224-PCXR4	798456	05/04/2024	1,000	1,500	2,000	998	1,500	1,997	1.001x - 5.085	1.000
R07	SKC	224-PCXR4	798480	02/04/2024	1,000	1,500	2,000	996	1,491	2,002	1.009x - 17.230	1.000
R08	SKC	224-PCXR4	883215	04/04/2024	1,000	1,500	2,000	1,010	1,502	2,007	1.001x + 9.255	1.000
R09	SKC	224-PCXR4	034650	05/04/2024	1,000	1,500	2,000	994	1,503	2,003	1.017x + 34.105	0.999
R10	SKC	224-PCXR4	091765	05/04/2024	1,000	1,500	2,000	998	1,497	1,996	1.001x - 3.929	1.000
R11	SKC	224-PCXR4	091763	05/04/2024	1,000	1,500	2,000	1,001	1,501	2,001	1.010x - 21.251	0.999
R12	SKC	224-PCXR4	091568	04/04/2024	1,000	1,500	2,000	997	1,500	2,002	1.009x - 9.014	1.000
R13	SKC	224-PCXR6	091638	08/04/2024	1,000	1,500	2,000	1,003	1,503	1,993	0.990x + 13.944	1.000
R14	SKC	224-PCXR4	091764	09/04/2024	1,000	1,500	2,000	995	1,501	1,998	1.013x - 27.899	0.999
R15	SKC	224-PCXR8	529457	04/04/2024	1,000	1,500	2,000	1,002	1,501	2,003	1.005x - 8.870	1.000
R16	SKC	224-PCXR8	529643	08/04/2024	1,000	1,500	2,000	999	1,497	1,995	1.000x - 4.367	1.000
R17	SKC	224-PCXR8	529645	04/04/2024	1,000	1,500	2,000	997	1,507	2,003	1.012x - 23.233	0.999
R18	SKC	224-PCXR8	566756	08/04/2024	1,000	1,500	2,000	992	1,499	1,999	1.002x - 7.159	1.000
R19	SKC	224-PCXR8	566802	04/04/2024	1,000	1,500	2,000	1,002	1,497	2,002	1.011x - 21.211	0.999
R20	SKC	224-PCXR8	529089	08/04/2024	1,000	1,500	2,000	994	1,501	2,004	1.013x - 24.274	1.000
R21	SKC	224-PCXR8	665728	04/04/2024	1,000	1,500	2,000	1,000	1,496	1,998	0.999x - 1.284	1.000
R22	SKC	224-PCXR8	707444	04/04/2024	1,000	1,500	2,000	1,001	1,501	2,004	1.006x - 10.948	1.000
R23	SKC	224-PCXR8	761067	04/04/2024	1,000	1,500	2,000	997	1,493	1,992	0.994x + 2.840	1.000
R24	SKC	224-PCXR8	707893	02/04/2024	1,000	1,500	2,000	997	1,507	1,998	1.006x - 14.046	0.999
R25	SKC	224-PCXR6	761052	09/04/2024	1,000	1,500	2,000	1,009	1,494	1,996	0.987x + 17.592	1.000
R26	SKC	224-PCXR8	707956	08/04/2024	1,000	1,500	2,000	1,003	1,500	2,004	1.009x - 15.934	0.999
R27	SKC	224-PCXR8	707398	09/04/2024	1,000	1,500	2,000	995	1,502	2,003	1.008x - 17.958	1.000
R28	SKC	224-PCXR8	707481	09/04/2024	1,000	1,500	2,000	1,003	1,500	2,003	1.012x - 22.471	0.999
R29	SKC	224-PCXR8	707402	08/04/2024	1,000	1,500	2,000	1,003	1,495	1,992	0.987x + 16.057	1.000
R30	SKC	224-PCXR8	093831	05/04/2024	1,000	1,500	2,000	999	1,494	1,993	0.991x + 0.921	1.000
R31	SKC	224-PCXR8	093183	04/04/2024	1,000	1,500	2,000	1,002	1,504	2,001	1.001x + 1.728	1.000
R32	SKC	224-PCXR6	761950	09/04/2024	1,000	1,500	2,000	999	1,502	1,996	0.997x + 3.418	1.000
R33	SKC	224-PCXR6	626255	04/04/2024	1,000	1,500	2,000	996	1,499	2,001	1.010x - 22.367	0.999
R34	SKC	224-PCXR4	626131	04/04/2024	1,000	1,500	2,000	1,000	1,501	2,005	1.008x - 14.071	1.000
R35	SKC	224-PCXR8	707460	05/04/2024	1,000	1,500	2,000	996	1,496	1,996	0.997x + 1.671	1.000
R36	SKC	224-PCXR8	707446	02/04/2024	1,000	1,500	2,000	1,002	1,499	2,000	1.010x - 20.385	0.999
R37	SKC	224-PCXR8	707432	04/04/2024	1,000	1,500	2,000	998	1,497	1,999	0.997x + 1.683	1.000
R38	SKC	224-PCXR8	707349	04/04/2024	1,000	1,500	2,000	996	1,499	2,000	1.000x - 3.701	1.000
R39	SKC	224-PCXR6	761095	09/04/2024	1,000	1,500	2,000	1,002	1,496	1,993	0.996x + 2.987	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25 ± 3 °C  
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data									
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve		
					Setting			Actual (Q std.)					
					1	2	3	1	2	3	y	R <sup>2</sup>	
R40	SKC	224-PCR16	612753	06/04/2024	1,000	1,500	2,000	998	1,499	1,997	1.011x - 23.404	0.999	
R41	SKC	224-PCR16	626140	05/04/2024	1,000	1,500	2,000	993	1,507	1,999	1.013x - 27.249	0.999	
R42	SKC	224-PCR16	626463	02/04/2024	1,000	1,500	2,000	1,000	1,495	1,996	0.998x + 1.113	1.000	
R43	SKC	224-PCR16	626129	09/04/2024	1,000	1,500	2,000	1,004	1,503	2,004	1.010x - 18.786	0.999	
R44	SKC	224-PCR16	602753	05/04/2024	1,000	1,500	2,000	1,003	1,494	1,992	0.993x + 5.576	1.000	
R45	SKC	224-PCR16	626137	09/04/2024	1,000	1,500	2,000	994	1,507	2,004	1.011x - 21.270	1.000	
R47	SKC	224-PCR16	A129234	06/04/2024	1,000	1,500	2,000	993	1,509	2,001	1.014x - 28.446	0.999	
R48	SKC	224-PCR16	A129253	06/04/2024	1,000	1,500	2,000	1,000	1,494	1,999	0.999x - 0.164	1.000	
R49	SKC	224-PCR16	A129168	08/04/2024	1,000	1,500	2,000	1,003	1,501	2,005	1.012x - 21.059	0.999	
R50	SKC	224-PCR16	A129282	08/04/2024	1,000	1,500	2,000	1,002	1,496	1,993	0.993x + 2.808	1.000	
R51	SKC	224-PCR16	A129264	08/04/2024	1,000	1,500	2,000	995	1,505	2,002	1.005x - 10.182	1.000	

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Calibration Data

Rotameter Data				Calibration Data									
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve			
				Flow Rate (Reading)			Actual (Q std.)						
				1	2	3	1	2	3	y	R <sup>2</sup>		
H-801	Dwyer	VFB-65	06/04/2024	500	1,000	2,000	504.3	992.1	1976.8	0.991x + 6.353	1.000		
H-802	Dwyer	VFB-65	04/04/2024	300	1,000	2,000	496.5	998.8	1996.7	0.995x + 4.247	1.000		
H-803	Dwyer	VFB-65	05/04/2024	300	1,000	2,000	498.6	991.4	2011.0	1.003x - 12.161	0.999		
H-804	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	501.4	1000.9	2008.3	0.998x - 1.566	1.000		
H-805	Dwyer	VFB-65	06/04/2024	500	1,000	2,000	502.4	999.5	1974.5	0.979x + 24.520	0.999		
H-806	Dwyer	VFB-65	04/04/2024	300	1,000	2,000	504.7	996.0	1984.4	1.005x - 6.145	1.000		
H-807	Dwyer	VFB-65	05/04/2024	500	1,000	2,000	502.2	992.8	2017.1	1.000x - 0.160	1.000		
H-808	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	500.3	1000.7	1980.2	0.995x + 5.203	0.999		
H-809	Dwyer	VFB-65	05/04/2024	500	1,000	2,000	503.3	1005.0	2011.1	0.994x + 13.348	1.000		
H-810	Dwyer	VFB-65	06/04/2024	500	1,000	2,000	498.2	1001.7	2008.8	0.995x + 5.854	1.000		

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ซอยพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jomjol, Chaituck, Bangkok 10900  
Tel : (662) 939-4379-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender S10-H

S/N : 136164

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)			y	R <sup>2</sup>
				1	2	3	1	2	3		
L-801	Dwyer	VFA-21	08/04/2024	50	100	200	50.7	98.8	199.3	0.987x + 1.039	1.000
L-802	Dwyer	VFA-21	04/04/2024	50	100	200	50.2	98.6	198.3	0.998x + 0.180	0.999
L-803	Dwyer	VFA-21	05/04/2024	50	100	200	50.5	98.8	197.9	1.012x - 1.915	1.000
L-804	Dwyer	VFA-21	04/04/2024	50	100	200	49.8	101.6	201.9	1.010x - 0.036	1.000
L-805	Dwyer	VFA-21	08/04/2024	50	100	200	50.9	99.0	201.2	0.998x + 0.999	1.000
L-806	Dwyer	VFA-21	04/04/2024	50	100	200	50.1	99.4	202.7	1.011x - 0.423	1.000
L-807	Dwyer	VFA-21	05/04/2024	50	100	200	50.3	99.9	200.5	1.009x - 0.861	1.000
L-808	Dwyer	VFA-21	04/04/2024	50	100	200	50.6	100.8	198.9	1.002x - 0.189	1.000
L-809	Dwyer	VFA-21	09/04/2024	50	100	200	50.1	99.4	200.6	0.997x + 0.731	1.000
L-810	Dwyer	VFA-21	08/04/2024	50	100	200	51.0	98.9	202.8	0.996x + 1.709	0.999

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ซอยพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jomjol, Chaituck, Bangkok 10900  
Tel : (662) 939-4379-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### Console Calibration Report

Calibration Method

Critical Orifices

Calibration Data				
Console Data		Calibration Data		
No.	Serial No.	Date	y	$\Delta H_g$ (mmH <sub>2</sub> O)
B01	1563	03/06/2024	0.996	50.07
B02	8002514	04/06/2024	0.995	49.98
B03	1503016	04/06/2024	0.994	50.19
B04	00006659	03/06/2024	0.995	50.28
B05	00007428	03/06/2024	0.997	49.75
R01	1561	05/06/2024	0.994	50.23
R02	8002513	04/06/2024	0.993	50.35
R03	1570	03/06/2024	0.994	50.12
R04	8002519	05/06/2024	0.993	49.89
R05	1503015	04/06/2024	0.996	49.92

Remark : Accept Value of y (test) is  $0.97 < y < 1.03$

Accept Value of  $\Delta H_g$  (test) is  $46.7 \pm 6.4$  (mmH<sub>2</sub>O)

Calibrated by



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 แขวงพหลโยธิน เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 913-4221 E-mail : sales@spscs.com www.spscs.com

### Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

#### Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	06/05/2024	0.84	0.84
B04	S	0.99	06/05/2024	0.84	0.85
B05	S	0.99	07/05/2024	0.84	0.83
B07	S	0.99	07/05/2024	0.84	0.84
B08	S	0.99	07/05/2024	0.84	0.85
B09	S	0.99	07/05/2024	0.83	0.84
B11	S	0.99	07/05/2024	0.84	0.85
B16	S	0.99	08/05/2024	0.84	0.84
B18	S	0.99	08/05/2024	0.85	0.84
B19	S	0.99	08/05/2024	0.84	0.85
B21	S	0.99	07/05/2024	0.84	0.84
B24	S	0.99	07/05/2024	0.84	0.84
B27	S	0.99	06/05/2024	0.85	0.84
B30	S	0.99	09/05/2024	0.84	0.84
B31	S	0.99	09/05/2024	0.84	0.84
B33	S	0.99	09/05/2024	0.83	0.84
B35	S	0.99	07/05/2024	0.84	0.84

Remark : Accept value of Cp (test) is 0.84  $\pm$  0.01

Calibrated by :

## CALIBRATION LABORATORY CO., LTD.

2/10-11, 14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail: sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220066-4]  
CLID. NO. : 212201115  
JOB CONTROL NO. : 230725081568

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 25 July 2023

DATE OF ISSUED : 31 July 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee  
Calibration Engineer

Approved By :

Authorized Signatory  
31 July 2023

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units ( SI )

Certificate No. Q23081568

F3-011-04/01-12

page 1 of 3







## CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



### REPORT OF CALIBRATION

#### FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220066-4]  
DATE OF CALIBRATION : 26 July 2023  
DUE DATE OF CALIBRATION : 26 July 2024

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-05 according to DKD-R 6-1 as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand). Certificate No. MP-0035-23, Due Date 02 February 2024.

#### UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2$ . It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q23081568

F3-011-04/01-12

page 2 of 3



@clccalibration



## CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



#### CONDITION OF CALIBRATION ITEM : GOOD

#### MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

#### CALIBRATION DATA

##### CORRECTION OF PRESSURE

DUC Test point ( inHg )	STD Reading ( kPa )		Conversion to inHg		Correction ( inHg )	
	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-17.61	-17.95	-5.2	-5.3	-0.2	-0.3
-10	-34.54	-34.54	-10.2	-10.2	-0.2	-0.2
-15	-51.13	-51.47	-15.1	-15.2	-0.1	-0.2
-20	-67.72	-68.06	-20.0	-20.1	0.0	-0.1
-25	-84.31	-84.31	-24.9	-24.9	+0.1	+0.1
-30	-101.24	-101.24	-29.9	-29.9	+0.1	+0.1

Uncertainty of measurement  $\pm 0.2$  inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q23081568

F3-011-04/01-12

page 3 of 3



@clccalibration





CERTIFICATE No : 24M2227  
REFERENCE No : 72448-1

PAGE : 1 OF 2

### Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE  
MANUFACTURER : METTLER TOLEDO  
MODEL : XS105DU  
SERIAL No : 1126422905  
ID No : BA05/50  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL., CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 08-Mar-24

APPROVED BY :

ISSUED DATE : 14-Mar-24

RECEIVED DATE : 08-Mar-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

F-G010 REV 03



CERTIFICATE No : 24M2227

PAGE : 2 OF 2

### Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA05/50 RECEIVED DATE : 08-Mar-24  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 08-Mar-24  
AMBIENT TEMPERATURE : 25° C  $\pm$  1° C RELATIVE HUMIDITY : 53 %RH  $\pm$  10 % RH

#### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

#### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-


- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

#### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL
2. TARE FUNCTION : NORMAL
3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g
4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02001	-0.00001	0.000065
0.10	0.10002	-0.00002	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	9.99994	0.00006	0.000070
20.00	20.00008	-0.00008	0.000078
50.00	50.0000	0.0000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0001	-0.0001	0.00022

#### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200  
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

### GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0823/21044

Instrument Type : GC

Model : CP-3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 09/08/2023

#### ELECTRONIC TEST

CPU	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
LCD TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
VENT TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
KEY ECHO TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DESTRUCTION RAM TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

#### RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detector ( FID Channel Front)

INJECTOR : Capillary Injector Model 1079

#### GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1 min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column:Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218 g/L C14,C15,C16 in hexane

SENSITIVITY TEST: C15. ( Area count ) = 362,972 Counts.



VARIAN

1/2

SERVICE DEPARTMENT  
FR-SV-029 Rev. 04



บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200  
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

#### Detector Sensitivity ( FID )


Detector Response	Result	Specification
Baseline Noise (µV)	1.47	≤ 50
Baseline Drift (%)	0.09	≤ 1
Sensitivity ( S/N for C15)	19,600	≥ 1,024

#### Temperature Specification

Temperature	Set	Result	Specification
Column Oven (° C)	80	80	± 5
Injector (° C)	220	220	± 5
Detector (° C)	300	300	± 5
Incubator (° C)	60	N/A	± 5

#### Relative Standard Deviation % ( % RSD)

Checkout Procedure	Result	Specification
Area C15 ( % )	1.52	≤ 5
Retention Time C15( % )	0.01	≤ 0.5



VARIAN

2/2

SERVICE DEPARTMENT  
FR-SV-029 Rev. 04



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200  
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

#### Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	357,863
C15 Area 2	357,824
C15 Area 3	367,724
C15 Area 4	361,724
C15 Area 5	369,724
C15 Area Average	362,972
* % RSD ( < 5 % )	1.52

\* The precision specification should be less than 2.0 % RSD \*\* ( Relative Standard Deviation ) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five ( 5 ) samples.

\*\* (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = ( \text{std.dev} / \text{avg} ) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by		
Date	08/08/2023	



Comments

Reviewed by



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200  
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

#### Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	4.125
C15 RT 2	4.125
C15 RT 3	4.125
C15 RT 4	4.124
C15 RT 5	4.124
C15 RT Average	4.122
* % RSD ( < 0.5 % )	0.01

\* The precision specification should be less than 0.5 % RSD \*\* ( Relative Standard Deviation ) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five ( 5 ) samples.

\*\* (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = ( \text{std.dev} / \text{avg} ) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by		
Date		



VARIAN

1/1

SERVICE DEPARTMENT



VARIAN

1/1

SERVICE DEPARTMENT


Title :  
Run File : d:\ceiA0A gc\ceiA0A-NeSEA\drive-d\2017\2023\08\blk2023.run  
Method File : C:\star\data\TU\cal2023\baseline FID.mth  
Sample ID : Blk2023

Injection Date: 9/8/2566 13:13 Calculation Date: 9/8/2566 13:34

Operator : watsamon Detector Type: 3800 (10 Volts)  
Workstation: GC-LAB Bus Address : 44  
Instrument : Sample Rate : 10.00 Hz  
Channel : Front = FID Run Time : 21.208 min

\*\* GC Workstation Version 6.41 \*\* 03334-6390-826-0764 \*\*

Chart Speed = 1.03 cm/min Attenuation = 1 Zero Offset = 3%  
Start Time = 0.000 min End Time = 21.208 min Min / Tick = 1.00

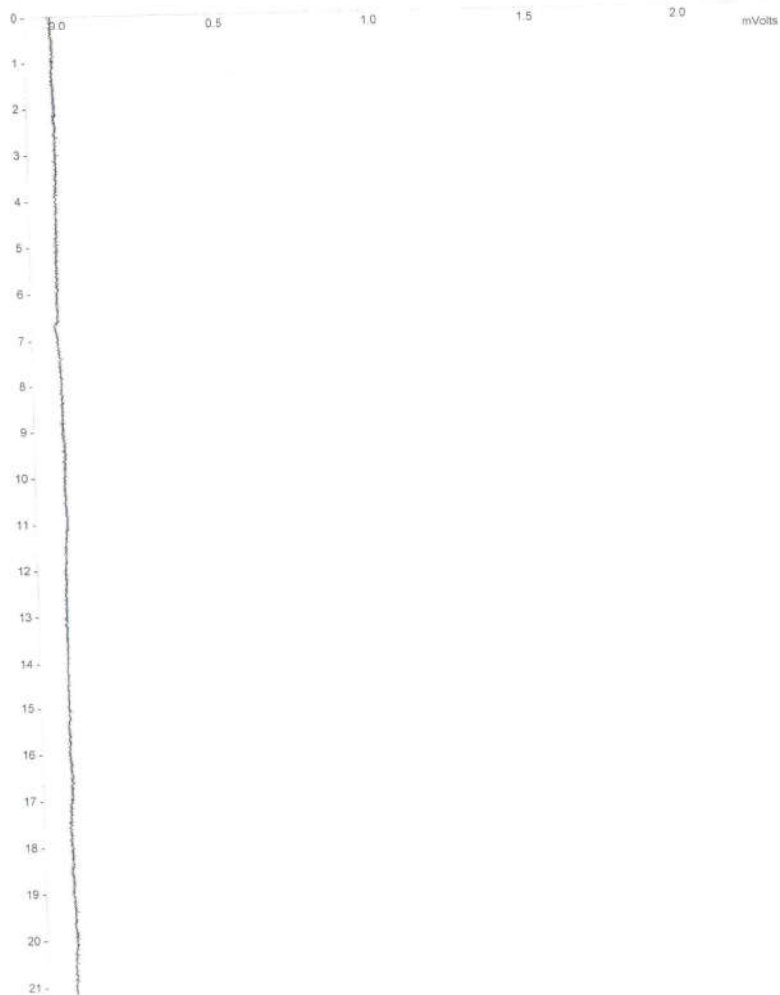

Print Date: Wed Aug 09 13:35:26 2023 Page 1 of 1

Title :  
Run File : d:\ceiA0A gc\ceiA0A-NeSEA\drive-d\2017\2023\08\blk2023.run  
Method File : C:\star\data\TU\cal2023\baseline FID.mth  
Sample ID : Blk2023

Injection Date: 9/8/2566 13:13 Calculation Date: 9/8/2566 13:34

Operator : watsamon Detector Type: 3800 (10 Volts)  
Workstation: GC-LAB Bus Address : 44  
Instrument : Sample Rate : 10.00 Hz  
Channel : Front = FID Run Time : 21.208 min

\*\* GC Workstation Version 6.41 \*\* 03334-6390-826-0764 \*\*

Run Mode : Blank Baseline  
Peak Measurement: Peak Area  
Calculation Type: External Standard

Peak No.	Peak Name	Result ( )	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	1/2 (sec)	Status Codes
Totals:		0.0000		0.000	0			

Total Unidentified Counts : 0 counts  
Detected Peaks: 0 Rejected Peaks: 0 Identified Peaks: 0  
Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0  
Baseline Offset: -14 microVolts LSB: 1 microVolts  
Noise (used): 19 microVolts - monitored before this run  
Manual injection



Title : c:\star\data\tu\cal2023\fid\calfid2023003.run  
Run File : d:\method-gc\star c\star\method\cp-wax\without glasswool\calfid2023003-front.mth  
Method File : d:\method-gc\star c\star\method\cp-wax\without glasswool\calfid2023003-front.mth  
Sample ID : Manual Sample

Injection Date: 9/8/2566 10:31 Calculation Date: 9/8/2566 10:40

Operator : watsamon Detector Type: 3800 (10 Volts)  
Workstation: Local Disk Bus Address : 44  
Instrument : Sample Rate : 10.00 Hz  
Channel : Front = FID Run Time : 7.993 min

\*\* GC Workstation Version 6.41 \*\* 03334-6390-826-0764 \*\*

Run Mode : Analysis  
Peak Measurement: Peak Area  
Calculation Type: External Standard

Peak No.	Peak Name	Result	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
1	C14	33.8385	3.520	-0.003	352495	BB	2.2	C
2	C15	33.4804	4.125	-0.006	357824	BB	2.3	C
3	C16	32.6143	4.699	-0.001	344951	BB	2.2	C
Totals:					99.9332			

Status Codes:

C - Out of calibration range

Total Unidentified Counts : 0 counts

Detected Peaks: 3 Rejected Peaks: 0 Identified Peaks: 3

Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0

Baseline Offset: 28 microVolts LSB: 1 microVolts

Noise (used): 26 microVolts - monitored before this run

Manual Injection

Callb. out of range; No Recovery Action Specified


Title :  
Run File : c:\star\data\tu\cal2023\fid\calfid2023003.run  
Method File : d:\method-gc\star c\star\method\cp-wax\without glasswool\calfid2023003-front.mth  
Sample ID : Manual Sample

Injection Date: 9/8/2566 10:31 Calculation Date: 9/8/2566 10:40

Operator : watsamon Detector Type: 3800 (10 Volts)  
Workstation: Local Disk Bus Address : 44  
Instrument : Sample Rate : 10.00 Hz  
Channel : Front = FID Run Time : 7.993 min


\*\* GC Workstation Version 6.41 \*\* 03334-6390-826-0764 \*\*

Chart Speed = 2.73 cm/min Attenuation = 70 Zero Offset = 2%  
Start Time = 0.000 min End Time = 7.993 min Min / Tick = 1.00

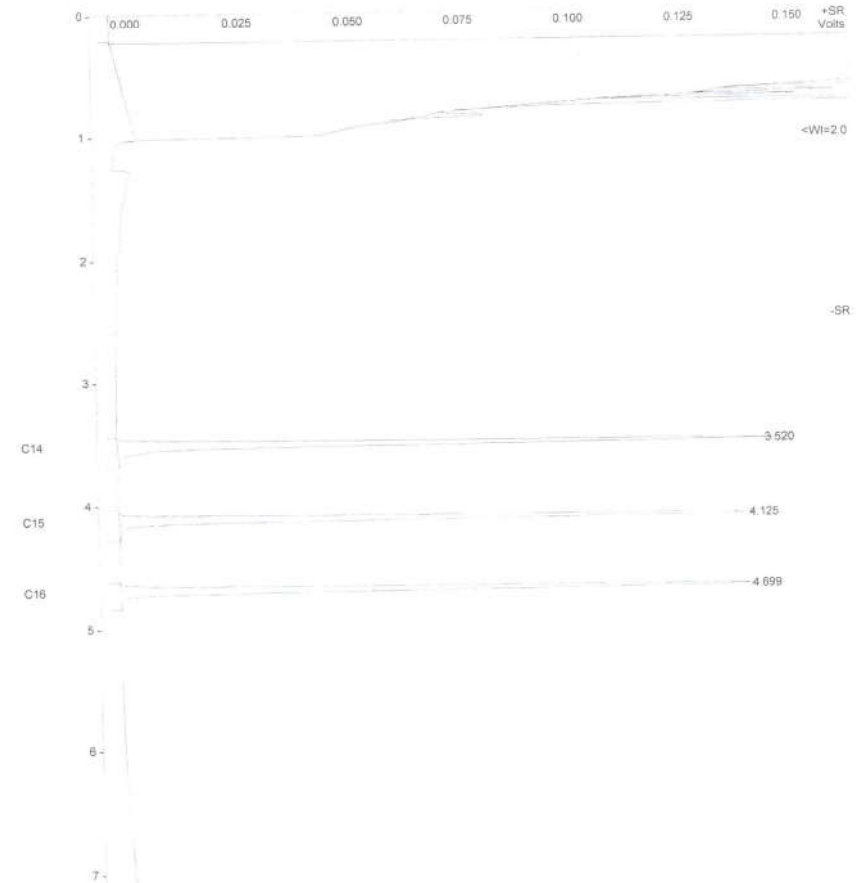


Sample ID: **fid std**

Operator (Inj): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (Inj):

  
**VARIAN**  
Run Mode: Analysis  
Peak Measurement: Peak Area  
Calculation Type: External Std.

c:\star\data\tu\cal2023\fid\calfid2023001.run

A = FID 10 V RESULTS

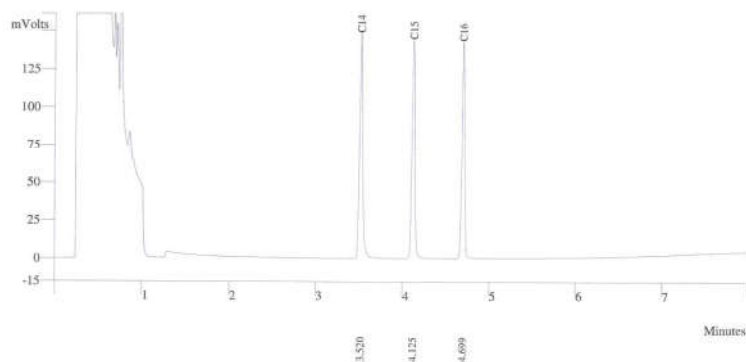

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	359491	BB	2.2
2	C15	33.4804	4.125	357863	BB	2.3
3	C16	32.6143	4.699	344951	BB	2.2
Totals		99.9312		1062305		


Sample ID: **fid std**

Operator (Inj): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (Inj):

  
**VARIAN**  
Run Mode: Analysis  
Peak Measurement: Peak Area  
Calculation Type: External Std.

c:\star\data\tu\cal2023\fid\calfid2023001.run

A = FID 10 V RESULTS

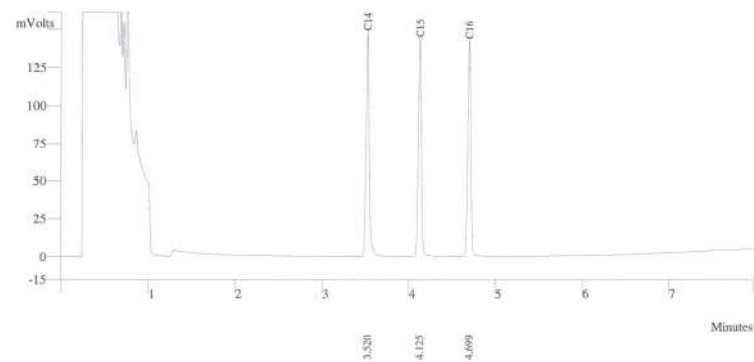

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	362495	BB	2.2
2	C15	33.4804	4.125	357824	BB	2.3
3	C16	32.6143	4.699	344951	BB	2.2
Totals		99.9332		1065270		


Sample ID: fid std

Operator (Inj): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (Inj):



c:\star\data\tu\cal2023\fid\calfid2023002.run

A = FID 10 V RESULTS

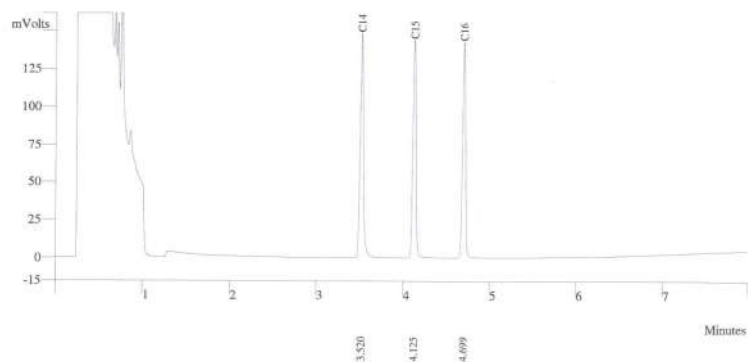


Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	362495	BB	2.2
2	C15	33.4824	4.125	367724	BB	2.3
3	C16	32.6143	4.699	354951	BB	2.2
Totals		99.9352		1085170		




Sample ID: fid std

Operator (Inj): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (Inj):



c:\star\data\tu\cal2023\fid\calfid2023002.run

A = FID 10 V RESULTS

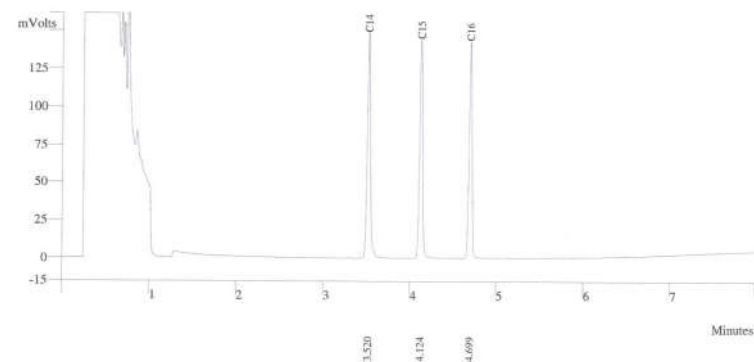


Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	362495	BB	2.2
2	C15	33.4824	4.124	361724	BB	2.3
3	C16	32.6143	4.699	354991	BB	2.2
Totals		99.9352		1079210		




Sample ID: fid std

Operator (In): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (In):

  
**VARIAN**  
Run Mode: Analysis  
Peak Measurement: Peak Area  
Calculation Type: External Std.

c:\star\data\tu\cal2023\fid\calfid2023002.run

A = FID 10 V RESULTS

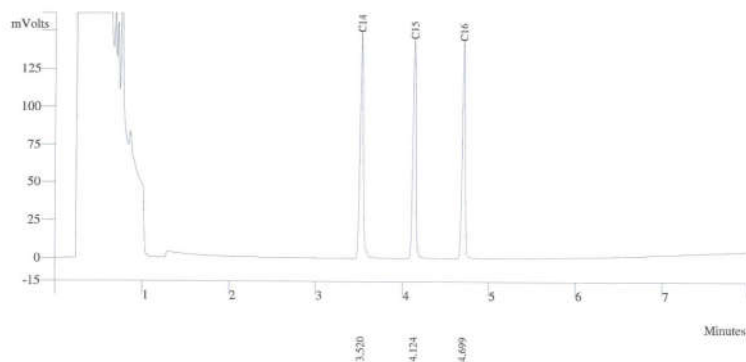

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	362495	BB	2.2
2	C15	33.4824	4.124	369724	BB	2.3
3	C16	32.6143	4.699	354591	BB	2.2
Totals		99.9552		1087210		



THAI UNIQUE CO.,LTD.

1 OF 1



Agilent Technologies

## Certificate of Analysis

## FID-TCD Performance Evaluation Sample Kit

Agilent Part Number: 5080-8842, 18710-60170

Sample Lot Number: 0006637856

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

Concentrations:		
n-tetradecane	0.218 g/L ( $\pm 0.5\%$ )	0.033 w/w %
n-pentadecane	0.218 g/L ( $\pm 0.5\%$ )	0.033 w/w %
n-hexadecane	0.218 g/L ( $\pm 0.5\%$ )	0.033 w/w %


Solvent: hexane

Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z-540-1 and ISO 9001.

Purities:	
n-tetradecane	99.6%
n-pentadecane	99%
n-hexadecane	99%
hexane	99%

## Typical Analytical Spectrum or Chromatography

GC Chromatography – n-tetradecane, n-pentadecane, and n-hexadecane in hexane

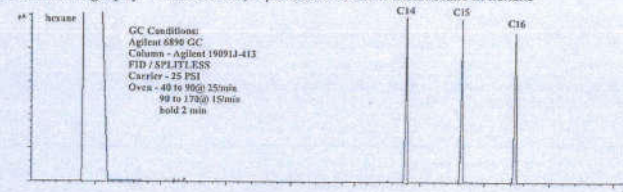

Date of release: 30 September 2021

Date of expiration: 31 October 2023



# Certificate

It is hereby certified that

**Suwarot Trikainut**

Has successfully completed the Application Training for

**Basic Gas Chromatography and Sampler**

Training Contents were:

**Hardware Operation, Software Operation, Data analysis and**

**Troubleshooting : Model**

**CP-3800, 3900, 450-GC, 430-GC, 456-GC, 436-GC**

At Thai Unique Co., Ltd, Bangkok, Thailand

On 15<sup>th</sup> March, 2019

Service Manager

Business Unit  
**Technology**



## CERTIFICATE OF QUALIFICATION

Qualification Date : 13 June 2024

Next Due : 12 June 2025

<b>Certificate No.</b>	QUAL2024_023
<b>Customer Name</b>	S.P.S Consulting Service Co.,Ltd
<b>Address</b>	7 Soi Phaholyothin 24, Phaholyothin Road, Ladyao, Jatujak, Bangkok, 10900
<b>Phone</b>	+66 (0) 2939 4370
<b>Fax</b>	-

### Instrument Identification

Model	Serial No.	Manufacturer
e2695	M13SM7942A	WATERS
Column Heater/Cooler	C14SMC892G	WATERS
2489 UV/Vis Detector	B1487E998A	WATERS

### Operational And Performance Qualification Test Completed

<input checked="" type="checkbox"/> 1. Flow Rate Accuracy Test	<input checked="" type="checkbox"/> 7. Injector Linearity & Accuracy Test
<input checked="" type="checkbox"/> 2. Column Temperature Accuracy Test	<input checked="" type="checkbox"/> 8. Injector Carryover Test
<input checked="" type="checkbox"/> 3. Sample Temperature Accuracy Test	<input checked="" type="checkbox"/> 9. Flow Rate Linearity Test
<input checked="" type="checkbox"/> 4. System Precision Test	<input checked="" type="checkbox"/> 10. Compositional Precision Test
<input checked="" type="checkbox"/> 5. Wavelength Accuracy Test	<input checked="" type="checkbox"/> 11. Noise and Drift Test
<input checked="" type="checkbox"/> 6. Detector Linearity & Sensitivity Test	<input checked="" type="checkbox"/> 12. Signal to Noise Test

Result Of Qualification: **Passes & Certifies For 1 Year**

Qualified By

Approved By

(M)

Engineer Technical Services

Manager, Technical Services

- The document is invalid if without authorize signatures and reference numbers.
- The data and numbers on this document cannot be changed and replaced in any cases.
- The expired date is valid on the date specified and cannot be reprinted or rewrite in any cases.
- The inspector can check the operator by the address mentioned on above only.
- Reprint, rewrite and supply without authorized permission is strictly prohibited.

### DKSH (Thailand) Limited

2106 Fantree 4 Building, Sukhumvit Rd., Phrakhanong-Tai, Phrakhanong, Bangkok 10260, Thailand  
Phone +662 301 7200, Fax +66 2333 1014, www.dksh.co.th/tech

Delivering growth – in Asia and beyond

ศูนย์บริการลูกค้าเทคโนโลยี - Technology service call center  
☎ 02 639 7000

# SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : SP23016

Pages : 1 of 3

## Calibration Certificate

**Equipment :** UV-VIS SPECTROPHOTOMETER  
**Manufacturer :** PERKINELMER  
**Model :** LAMBDA 25  
**Serial No.:** 501S14123010  
**ID No.:** SP03/58  
**Calibration Mode :** WAVELENGTH ACCURACY  
PHOTOMETRIC ACCURACY  
**Condition As Found :** GOOD  
**Customer :** S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,  
CHOMPHON, CHATUCHAK,  
BANGKOK 10900, THAILAND.  
**Location :** ORGANIC LABORATORY IV  
**Ambient Temperature :** ( 25.0 ± 5 ) °C  
**Relative Humidity :** ( 48.4 ± 25 ) %  
**Received Date :** 30 AUGUST 2023  
**Calibration Date :** 30 AUGUST 2023  
**Date of Issue :** 31 AUGUST 2023

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN  
associates

SITHIPORN ASSOCIATES CO.,LTD.  
CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : SP23016

Job No. : VC66SP0014

Pages : 2 of 3

### Calibration Method :

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01  
The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution  
The calibration procedure used was based on ASTM E275-01, ASTM E925-02

### Condition of this result of calibration :

#### 1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	106864	01/11/2024
Didymium liquid	RM-DL	28912	106905	02/11/2024
Neutral density filter	RM-IN2N3N	13877	106918	03/11/2024
Potassium dichromate solutions	RM-0204060810	14204	106902	02/11/2024
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology, NIST.

### Result of calibration : Wavelength Accuracy

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.3	0.05	0.16	2.00
	467.82	468.0	0.18	0.16	2.00
	536.56	536.6	0.04	0.16	2.00
	640.50	640.4	-0.10	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.0	0.06	0.16	2.00

UUC\* = Unit Under Calibration

QF-TS12-04-4-020664

## Continuation of Calibration Certificate

Cert. No. : SP23016  
Job No. : VC66SP0014  
Pages : 3 of 3

## Result of calibration : Photometric Accuracy

(Without adjustment)

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0517	1.0564	0.0047	0.0031	2.00
		29914	0.7	0.7445	0.7460	0.0015	0.0032	2.00
		29381	0.5	0.5416	0.5429	0.0013	0.0032	2.00
	546.1	29360	1.0	0.9821	0.9849	0.0028	0.0030	2.00
		29914	0.7	0.6961	0.6961	0.0000	0.0030	2.00
		29381	0.5	0.5073	0.5073	0.0000	0.0030	2.00
	590.0	29360	1.0	1.0222	1.0244	0.0022	0.0030	2.00
		29914	0.7	0.7237	0.7234	-0.0003	0.0030	2.00
		29381	0.5	0.5361	0.5360	-0.0001	0.0031	2.00
	635.0	29360	1.0	0.9753	0.9775	0.0022	0.0030	2.00
		29914	0.7	0.6910	0.6910	0.0000	0.0030	2.00
		29381	0.5	0.5211	0.5210	-0.0001	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	20	20	0.2422	0.2462	0.0040	0.0101	2.00	
		40	0.4866	0.4900	0.0034	0.0115	2.00	
	235.0	60	0.7414	0.7390	-0.0024	0.0068	2.00	
		80	0.9858	0.9871	0.0013	0.0093	2.00	
		100	1.2442	1.2480	0.0038	0.0087	2.00	

UUC\* = Unit Under Calibration

## Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230

Resolution of Wavelength Mode 0.1 nm  
Resolution of Photometric Mode 0.0001 A

## Parameter Setting

Measurement Mode Wavelength, Absorbance  
Wavelength Scan 1100 nm-190 nm  
Scanning Speed 7.5 nm/min  
Data Pitch 0.1 nm  
Band width(Wavelength) 1.0 nm  
Band width(Vis) 1.0 nm  
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transmission T(%)	Absorbance(A)
0.0111	3.9564

\*\*Specific Acceptance :

Transmission  $\leq 1.0$  T(%), Absorbance  $\geq 2.0$  A

\*\*Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95%

End of Calibration Certificate

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยเทศบาล 24 แขวงคลองเตย เขตคลองเตย กรุงเทพฯ 10900  
Tel: (02) 539-4370-12 Fax: (02) 533-4231 E-mail: info@sps.co.th www.sps.co.th

Calibration Report			
Non-Dispersive Infrared CO Analyzer			
Date : 04 June 2024	Brand : API	Model : 300E	
No. : CO-801		Serial No. : 782	
Calibrator (Dilution System)			
Brand : API		Model : 700	
Last Cal. Date : 08 August 2023		Serial No. : 911	
Reference Standard Gas			
Standard Gas : Carbon Monoxide (CO)		Cylinder No. : 0711839	
Certified Date : 16 March 2024	Expired Date : 14 March 2032	Cylinder Conc. : 4.580 ppm	
Calibrating Condition			
Pressure : 1011 mmbar	Temp. : 24.6 °C	% RH : 50	
Calibration Setting			
Span	Initial Reading (Before Adj.) PPM		Final Reading (After Adj.) PPM
Set Point	Expected Concentration	Analyzer Response	%OF Analyzer Response
Zero	0	0.11	-
CO Span	40.00	40.05	0.125
API Model 300E CO Analyzer Check List			
Parameter	Observed Value	Units	Nominal Range
Range	50	PPM	0-1000 ppm
Stability	0.10	PPM	+ 1 ppm With Zero Air
CO Measure	4015.6	mV	2500-4800 mV
CO Reference	3999.1	mV	2500-4800 mV
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air
Sample Pressure	28.4	in-Hg-A	-2" - Ambient Absolute Pressure
Sample Flow	807	CC/Min	800 ± 10%
Sample Temperature	48.4	°C	48 ± 4
Bench Temperature	48.2	°C	48 ± 2
Wheel Temperature	68.3	°C	68 ± 2
Box Temperature	50.8	°C	
Photo-Drive	3039.5	mV	Ambient Temp + 7 ± 10
Slope	1.017	-	250 mV to 4750 mV
Offset	0.2	-	1.0 ± 0.3

Calibrated by :

ระดับเสียง

Noise B\_220\_24

Sound Level Meter Calibration Report

Acoustic Calibrator Data			
Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	04 March 2024
		Due Date	04 March 2025

Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B18	ACO	6236	00172048	12 June 2024	93.9	93.9
ACO-B29	ACO	6236	00182011	12 June 2024	94.1	93.9
ACO-B33	ACO	6236	00182015	12 June 2024	93.9	93.9
ACO-B36	ACO	6236	00192027	12 June 2024	93.9	93.9
ACO-B41	ACO	6236	00192032	12 June 2024	94.0	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.85 ± 0.10 dB	

Calibrated by :

Noise Dose B\_220\_1/24

Noise Dose Meter Calibration Report

Acoustic Calibrator Data			
Brand	SVANTEK	Number	SV 03/60
Model	SV34	Serial No.	83820
Calibration Range	114 dB, 1000 Hz	Last Calibration	22 August 2023
		Due Date	22 August 2024

Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B08	SVANTEK	SV-104IS	80818	12 June 2024	114.0	114.0
NMD-B09	SVANTEK	SV-104IS	80829	12 June 2024	114.1	114.0
NMD-B10	SVANTEK	SV-104IS	80830	12 June 2024	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.01 ± 0.10 dB	

Calibrated by :





ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24030285-12

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,  
Bangkok 10900

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 192032

ID. Number : ACO-B41

### Environmental Conditions

Ambient Temperature : 23 °C ± 3 °C

Relative Humidity : 50 % ± 15 %

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Mar 2024

Calibration Date : 23 Mar 2024

Recommend Due Date : 23 Mar 2025

Date of Issue : 24 Mar 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by

Authorized Signatory

SP-FM-04-15 rev.0



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24030285-12

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

### Traceability

This certification is traceable to the International System of Unit maintained at :  
TISTR - Thailand Institute of Scientific and Technological Research

SP-FM-04-15 rev.0



ID LINE : IEC17025



## Result of Calibration

Certificate Number : SPR24030285-12

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24050262-1

Page : 1 of 3

Customer

: S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,  
Bangkok 10900

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 172048

ID. Number : ACO-B18

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 17 May 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 20 May 2024

Location of Calibration : In-Lab

Recommend Due Date : 20 May 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 21 May 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by



Authorized Signatory



Certificate Number : SPR24050262-1

Page : 2 of 3

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

This certification is traceable to the International System of Unit maintained at :  
TISTR - Thailand Institute of Scientific and Technological Research

Certificate Number : SPR24050262-1

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.1	114.1	0.1	0.1	0.15

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -





ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24030285-10

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,  
Bangkok 10900

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 182011

ID. Number : ACO-B29

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity :  $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Mar 2024

Calibration Date : 23 Mar 2024

Recommend Due Date : 23 Mar 2025

Date of Issue : 24 Mar 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by



Authorized Signatory



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24030285-10

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

### Traceability

This certification is traceable to the International System of Unit maintained at :  
TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



## Result of Calibration

Certificate Number : SPR24030285-10

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24050262-2

Page : 1 of 3

Customer

: S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,  
Bangkok 10900

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 182015

ID. Number : ACO-B33

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$  Received Date : 17 May 2024

Relative Humidity :  $50\% \pm 15\%$  Calibration Date : 20 May 2024

Location of Calibration : In-Lab Recommend Due Date : 20 May 2025

Calibration Procedure : SP-CPE-04-01 Date of Issue : 21 May 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by :

( )

Authorized Signatory





# Calibration Report

Certificate Number : SPR24050262-2

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

## Traceability

This certification is traceable to the International System of Unit maintained at :  
TISTR - Thailand Institute of Scientific and Technological Research



### Result of Calibration

Certificate Number : SPR24050262-2

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.7	113.7	-0.3	-0.3	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	113.7	113.7	-0.3	-0.3	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -



ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24030285-11

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,  
Bangkok 10900

Equipment Name : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial Number : 192027

ID. Number : ACO-B36

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity :  $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Mar 2024

Calibration Date : 23 Mar 2024

Recommend Due Date : 23 Mar 2025

Date of Issue : 24 Mar 2024


### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by



Authorized Signatory



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24030285-11

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

### Traceability

This certification is traceable to the International System of Unit maintained at :  
TISTR - Thailand Institute of Scientific and Technological Research





ID LINE : IEC17025



## Result of Calibration

Certificate Number : SPR24030285-11

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	114.1	114.1	0.1	0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	93.9	93.9	-0.1	-0.1	0.15
114	114.1	113.9	0.1	-0.1	0.15

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0349

MTC No. EEL. BP. 55/0367

## CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co., Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok, 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Noise Dosimeter

Manufacturer : Svantek

Model : SV-104IS

Serial No. : 80818

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.5) \text{ kPa}$

### Standards used :

Multifunction Acoustic Calibrator Brüel&Kjær 4226 S/N 2810358 with Coupler UA0915 S/N 2810358.

### Calibration Procedure :

This instrument was calibrated by using calibration procedure no CP-102-01, which was based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2006). This calibration procedure was related to the acoustical signal test of frequency weightings using a multifunction acoustic calibrator.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%.

Date of Receipt : 15 Mar. 2024

Date of Calibration : 26 Mar. 2024

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from

### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9036  
Fax. (66) 0 2577 9009

### Office/Laboratory

668 Mu 2 Tambon Bangpoo Mai, Amphoe Muang Samutprakan,  
Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
(66) 08 3219 9440  
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

### Office

196 Phahonyothin Road, Ladyao, Chatuchak,  
Bangkok 10900, Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0349

MTC No. EEL. BP. 55/0367

**Acoustic signal test of frequency weightings**

Frequency (Hz)	Deviation from response curve		Uncertainty (±dB)	Tolerance Limits Class 2 (±dB)
	A-weighting (dB)	C-weighting (dB)		
125	-0.1	-0.3	0.25	2.0
1 000	-0.4	-0.3	0.25	1.4
4 000	-0.3	-0.3	0.25	3.6

- Note :**
- 1) There was no adjustment.
  - 2) The calibration was performed at a sound pressure level of 114 dB.
  - 3) The measured values did not include the correction of microphone of UUT.
  - 4) The deviation was produced from the absolute difference between the measured values and the responding sound pressure levels in IEC 61672-1 (2002).

Calibrated by :

*G. Sanaey*

(Mr. Sanaey Grajang)

Approved by :

*Prawate Kluaypa*

(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory  
Industrial Metrology and Testing Service Centre

Ref : 2011267031501086001

Date of Calibration : 26 Mar. 2024

Date of Issue : 27 Mar. 2024

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

**Head Office**  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9036  
Fax. (66) 0 2577 9009

**Office/Laboratory**  
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,  
Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
(66) 08 3219 9440  
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

**Office**  
196 Phahonyothin Road, Ladyao, Chatuchak,  
Bangkok 10900, Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0349

MTC No. EEL. BP. 56/0367

**CALIBRATION CERTIFICATE**

Submitted by : S.P.S.Consulting Service Co., Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok, 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Ambient Environment

Description : Noise Dosimeter

Temperature : (23 ± 3) °C

Manufacturer : Svantek

Relative Humidity : (50 ± 15) %

Model : SV-104IS

Ambient Pressure : (101.325 ± 1.5) kPa

Serial No. : 80829

Standards used :

Multifunction Acoustic Calibrator Brüel&Kjær 4226 S/N 2810358 with Coupler UA0915 S/N 2810358.

Calibration Procedure :

This instrument was calibrated by using calibration procedure no CP-102-01, which was based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2006). This calibration procedure was related to the acoustical signal test of frequency weightings using a multifunction acoustic calibrator.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Receipt : 15 Mar. 2024

Date of Calibration : 26 Mar. 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

**Head Office**  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9036  
Fax. (66) 0 2577 9009

**Office/Laboratory**  
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,  
Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
(66) 08 3219 9440  
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

**Office**  
196 Phahonyothin Road, Ladyao, Chatuchak,  
Bangkok 10900, Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
(66) 08 1889 6827





THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0349

MTC No. EEL. BP. 56/0367

Acoustic signal test of frequency weightings

Frequency (Hz)	Deviation from response curve		Uncertainty (±dB)	Tolerance Limits Class 2 (±dB)
	A-weighting (dB)	C-weighting (dB)		
125	0.1	0.1	0.25	2.0
1 000	-0.2	-0.1	0.25	1.4
4 000	-0.4	-0.4	0.25	3.6

- Note : 1) There was no adjustment.  
2) The calibration was performed at a sound pressure level of 114 dB.  
3) The measured values did not include the correction of microphone of UUT.  
4) The deviation was produced from the absolute difference between the measured values and the responding sound pressure levels in IEC 61672-1 (2002).

Calibrated by : [Redacted] Approved by : [Redacted]

Electrical and Electronic Standards Laboratory  
Industrial Metrology and Testing Service Centre

Ref : 2011267031501086002

Date of Calibration : 26 Mar. 2024

Date of Issue : 27 Mar. 2024

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9036  
Fax. (66) 0 2577 9009

Office/Laboratory  
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,  
Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
(66) 08 3219 9440  
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office  
196 Phahonyothin Road, Ladyao, Chatuchak,  
Bangkok 10900, Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0349

MTC No. EEL. BP. 57/0367

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co., Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok, 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Ambient Environment

Description : Noise Dosimeter

Temperature : (23 ± 3) °C

Manufacturer : Svantek

Relative Humidity : (50 ± 15) %

Model : SV-104IS

Ambient Pressure : (101.325 ± 1.5) kPa

Serial No. : 80830

Standards used :

Multifunction Acoustic Calibrator Brüel&Kjær 4226 S/N 2810358 with Coupler UA0915 S/N 2810358.

Calibration Procedure :

This instrument was calibrated by using calibration procedure no CP-102-01, which was based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2006). This calibration procedure was related to the acoustical signal test of frequency weightings using a multifunction acoustic calibrator.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Receipt : 15 Mar. 2024

Date of Calibration : 26 Mar. 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from

FM.BLMTC.002 Rev.5

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9036  
Fax. (66) 0 2577 9009

Office/Laboratory  
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,  
Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
(66) 08 3219 9440  
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office  
196 Phahonyothin Road, Ladyao, Chatuchak,  
Bangkok 10900, Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0349

MTC No. EEL. BP. 57/0367

Acoustic signal test of frequency weightings

Frequency (Hz)	Deviation from response curve		Uncertainty (+dB)	Tolerance Limits Class 2 (+dB)
	A-weighting (dB)	C-weighting (dB)		
125	-0.4	-0.3	0.25	2.0
1 000	-0.1	-0.2	0.25	1.4
4 000	0.3	0.2	0.25	3.6

- Note :**
- 1) There was no adjustment.
  - 2) The calibration was performed at a sound pressure level of 114 dB.
  - 3) The measured values did not include the correction of microphone of UUT.
  - 4) The deviation was produced from the absolute difference between the measured values and the responding sound pressure levels in IEC 61672-1 (2002).

Calibrated by

.....

Electrical and Electronic Standards Laboratory  
Industrial Metrology and Testing Service Centre

Ref : 2011267031501086003

Date of Calibration : 26 Mar. 2024

Date of Issue : 27 Mar. 2024

2 / 2

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.5

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9036  
Fax. (66) 0 2577 9009

Office/Laboratory

668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,  
Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
(66) 08 3219 9440  
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

Office

196 Phahonyothin Road, Ladyao, Chatuchak,  
Bangkok 10900, Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
(66) 08 1889 6827



คุณภาพน้ำ

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkac, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



NSC-TISI-TIS17025  
CALIBRATION BODY

CERTIFICATE No : 23E8494  
REFERENCE No : 70413-1

PAGE : 1 OF 3

**Certificate of Calibration**

**EQUIPMENT** : pH METER  
**MANUFACTURER** : HANNA  
**MODEL** : HI 3512  
**SERIAL No** : TH118035  
**ID No** : pH04/56  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 06-Sep-23

**APPROVED BY** :

**ISSUED DATE** : 06-Sep-23

**RECEIVED DATE** : 31-Aug-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV 03

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkac, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 2 OF 3

**Calibration Report**

**EQUIPMENT** : pH METER  
**MANUFACTURER** : HANNA  
**ID No** : pH04/56  
**RECEIVED DATE** : 31-Aug-23  
**AMBIENT TEMPERATURE** : 23 ° C ± 3 ° C  
**MODEL** : HI 3512  
**SERIAL NUMBER** : TH118035  
**CALIBRATION DATE** : 06-Sep-23  
**RELATIVE HUMIDITY** : 50 % RH ± 10% RH

**CONDITION OF THIS RESULTS OF CALIBRATION**

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTROD WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/ LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	23E1312	19-Apr-24
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

**RESULT OF CALIBRATION : ADJUSTMENT**

1. DISPLAY UNIT ONLY

SLOPE FACTOR k = 2.303 RT/F = 59 mV/pH

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.6	-0.49	-0.290	0.15	2.00
354.95	355.4	-0.45	0.741	0.15	2.00
295.80	296.3	-0.50	1.773	0.15	2.00
236.64	237.1	-0.46	2.804	0.15	2.00
177.48	177.9	-0.42	3.835	0.15	2.00
118.32	118.7	-0.38	4.867	0.15	2.00
59.16	59.6	-0.44	5.898	0.15	2.00
0.00	0.4	-0.40	6.930	0.15	2.00
-59.16	-58.8	-0.36	7.961	0.15	2.00
-118.32	-117.9	-0.42	8.992	0.15	2.00
-177.48	-177.1	-0.38	10.024	0.15	2.00
-236.64	-236.3	-0.34	11.055	0.15	2.00
-295.80	-295.5	-0.30	12.087	0.15	2.00
-354.95	-354.6	-0.35	13.118	0.15	2.00
-414.11	-413.8	-0.31	14.149	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3



# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 3 OF 3

## Calibration Report

### RESULT OF CALIBRATION (CONTINUE) :

#### 2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ pH)	COVERAGE FACTOR k
4.006	4.006	0.000	4.015	0.012	2.00
7.000	7.000	0.000	6.914	0.012	2.00
10.008	10.010	-0.002	9.996	0.014	2.00

#### 3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ( $^{\circ}$ C)	UUC READING ( $^{\circ}$ C)	CORRECTION ( $^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ $^{\circ}$ C)	COVERAGE FACTOR k
25.005	25.0	0.005	---	0.0085	2.00

#### 4. PERCENT SLOPE 100%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
[www.qcalibration.com](http://www.qcalibration.com)




CERTIFICATE No : 24M2229  
REFERENCE No : 72448-3

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE  
MANUFACTURER : SARTORIUS  
MODEL : BSA224S-CW  
SERIAL No : 36591843  
ID No : BA 09/61  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.  
CALIBRATION DATE : 08-Mar-24

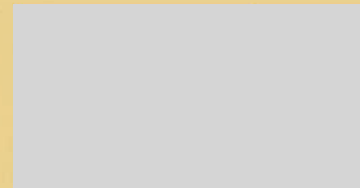APPROVED BY :   
ISSUED DATE : 14-Mar-24  
RECEIVED DATE : 08-Mar-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 24M2229

PAGE : 2 OF 2

**Calibration Report**

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW  
MANUFACTURER : SARTORIUS S/N : 36591843  
ID No : BA 09/61 RECEIVED DATE : 08-Mar-24  
AIR PRESSURE : 1010mbar ± 1mbar CALIBRATION DATE : 08-Mar-24  
AMBIENT TEMPERATURE : 25° C ± 1° C RELATIVE HUMIDITY : 55 %RH ± 10 % RH

**CONDITION OF THIS RESULTS OF CALIBRATION**

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

**2. REFERENCE STANDARD INSTRUMENTS :-**

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

**RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT**


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (± g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	50.0000	0.0000	0.00012
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

**5. OFF CENTER LOADING ERROR**

POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERT.No.: HS-V015C

Calibration Date : 20 Mar 24

Submitted by : ASIA LAB @ CONSULTANT CO.,LTD  
184 Soi Phutthamonthon Sai 2 Soi 12,  
Bangphai, Bangkae, Bangkok 10160

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Model : YSI 5000

S/N : 15B100751

Probe : YSI 5010

S/N : 22D100097

ID NO. : -

Air Temp ref : S/N. F8065C26

Barometric ref : S/N. F8065C26

Water Temp ref : S/N. 11430

Technician : Kittipong M.

**Calibration Details**

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-

Mean Measurement	9.08	mg/l	-	-
Inaccuracy	0.01	mg/l	-	-

Overall Status (PASS)

**Manufacturer Specification**

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

(Kittipong Maekwong)

(Supreecha Sumartam)

Harikul Science Co.,Ltd.

694 Soi Ratchadanivet 24, Pracharatbamphen,  
Samsaennok, Huaikhwang, Bangkok 10310

Tel: 0-2274-2456 Fax: 0-2274-2443

Email: info@harikul.com www.harikul.com

Certificate of Calibration





CERT.No.: HS-U017D

Harikul Science Co.,Ltd.  
694 Soi Ratchadaniwet 24, Pracharatbampnen,  
Samsaennok, Huaikhwang, Bangkok 10310  
Tel: 0-2274-2456 Fax: 0-2274-2443  
Email: info@harikul.com www.harikul.com

Certificate of Calibration

Calibration Date : 3 Apr 23

Submitted by : S.P.S CONSULTING SERVICE CO.,LTD

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,  
Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Model : YSI 5000

S/N : 15B100751

Probe : YSI 5010

S/N : 22D100097

ID NO. : -

Air Temp ref : S/N. E00522

Barometric ref : S/N. E00522

Water Temp ref : S/N. 11431

Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-

Mean Measurement	9.08	mg/l	-	-
Inaccuracy	0.01	mg/l	-	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

(Kittipong Maekwong)

(Natenapha Pisatkunchon)

Turbomass/Clarus Mass/ SQ8 MS Preventive Maintenance (PM)

Company Name:	S.P.S. Consulting Service Co.,Ltd		
Address (Instrument Location):	7 Soi Phaholyothin24 Phaholyothin Road, Jompol, Chatuchak, Bangkok, 10900.		
Serial Number:	648N4050804	PM Number:	1 of 2
Customer Name (if applicable):	Ms. Naruecha	Telephone Number:	NA
Service Engineer Name:	Monchai Kitcharoenkeat	Service Order Number:	WO-02760693
Date PM Performed: (DD-MMM-YYYY)	22-Feb-2024	Next PM Due Date: (DD-MMM-YYYY)	22-Aug-2024

Part Number	Release	Publication Date	
TH09370064	C	March 2013	

Scope

The purpose of this PM is to ensure the continued functionality of the Turbomass/Clarus MS SQ8 MS by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer. The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners. **Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.** PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

### Component List

Component / Specific Model	Serial #	Software Version	Configuration Notes
Clarus680	680S14042502	Totalchrom6.3	PSS,PSS,FID
Clarus SQ8	648N4050804	Turbomass 6.4	
Atom X	US14113002	Tekma AtomX	

### Parts lists

Parts Included with the PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
N/A				
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A				

### Procedure Checklist

Use ( x ) to check off those steps in the checklist that have been completed.

#### General:

- ☒ Column type Elite 624.
- ☒ Carrier gas flow rate 1 ml/min.
- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Check incoming AC line voltage for proper levels and grounding.

#### Mechanical:

- ☒ Inspect and clean all fans and filters.
- ☒ Check the level of FC-43 calibration compound in reference gas bulb and fill if necessary.
- ☒ Change the oil in the fore pump.
- ☒ Inspect cartridge in fore pump vacuum filter; replace adsorbent bead if necessary.
- ☒ Replace the exhaust vapor mist filter on the fore pump.
- ☒ Remove and clean the ion source assembly. Use the Insulator Replacement Kit and/or Optics Replacement Kit if necessary.
- ☒ Replace the filament.
- ☒ Remove and clean the pre-quad rods.
- ☒ Observe Wide Range Gauge pressure; clean/adjust if required.
- ☒ Inspect and clean as needed all PC boards and bottom inside of MS chassis.

#### Electrical:

- ☒ Check head amp offset. Adjust if necessary for proper value (Service Manual ).

#### Operational Tests:

- ☒ Vacuum pressure.
- ☒ Air/water leak check
- ☒ AutoTune and mass calibration.
- ☒ Make a Chromatographic injection to verify peak shape and integrity only (not meant for sensitivity test).

#### PC Maintenance:

- ☒ Delete all unnecessary temporary files.
- ☒ Empty deleted files from recycle bin.
- ☒ Perform hard drive defragmentation.

#### Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand.

#### Additional Comments

Additional Comments Regarding the PM

#### Review

<i>The preventive maintenance checks and if applicable performance tests for Turbomass/ Clarus Mass/ SQ8 have been completed.</i>		
<i>This Turbomass/ClarusMS/SQ8</i>	<i>Pass</i>	<i>the preventive maintenance.</i>
<b>Review of Preventive Maintenance:</b>		
Authorized PerkinElmer Representative Monchai Kitcharoenkeat	<i>monchai</i>	Date: 22-Feb-2024 (DD-MM-YYYY)
Authorized Customer Representative:	<i>naruacha</i>	Date: 22-Feb-2024 (DD-MM-YYYY)

#### GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0823/21044

Instrument Type : GC

Model : CP-3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 09/08/2023

#### ELECTRONIC TEST

CPU	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
LCD TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
VENT TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
KEY ECHO TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DESTRUCTION RAM TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

#### RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detector ( FID Channel Front)

INJECTOR : Capillary Injector Model 1079

#### GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column: Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218 g/L C14, C15, C16 in hexane

SENSITIVITY TEST: C15. ( Area count ) = 362,972 Counts.



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200  
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

#### Detector Sensitivity ( FID )

Detector Response	Result	Specification
Baseline Noise (µV)	1.47	≤ 50
Baseline Drift (%)	0.09	≤ 1
Sensitivity ( S/N for C15)	19,600	≥ 1,024

#### Temperature Specification

Temperature	Set	Result	Specification
Column Oven (° C)	80	80	± 5
Injector (° C)	220	220	± 5
Detector (° C)	300	300	± 5
Incubator (° C)	60	N/A	± 5

#### Relative Standard Deviation % ( % RSD)

Checkout Procedure	Result	Specification
Area C15 ( % )	1.52	≤ 5
Retention Time C15( % )	0.01	≤ 0.5

APPRO

Signatu

Engine

Date : 09/08/2023



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200  
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

#### Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	357,863
C15 Area 2	357,824
C15 Area 3	367,724
C15 Area 4	361,724
C15 Area 5	369,724
C15 Area Average	362,972
* % RSD ( < 5 % )	1.52

\* The precision specification should be less than 2.0 % RSD \*\* ( Relative Standard Deviation ) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five ( 5 ) samples.

\*\* (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = ( \text{std.dev} / \text{avg} ) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by		
Date		



Comments	
Reviewed by	



VARIAN

2/2

SERVICE DEPARTMENT  
FR-SV-029 Rev. 04



VARIAN

1/1

SERVICE DEPARTMENT





บริษัท ไทยยูนิค จำกัด THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200  
80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

#### Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	4.125
C15 RT 2	4.125
C15 RT 3	4.125
C15 RT 4	4.124
C15 RT 5	4.124
C15 RT Average	4.122
* % RSD ( < 0.5 % )	0.01

\* The precision specification should be less than 0.5 % RSD \*\* ( Relative Standard Deviation ) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five ( 5 ) samples.

\*\* (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = ( \text{std.dev} / \text{avg.} ) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by		
Date	09/08/2023	



Comments		
Reviewed by		


Title :  
Run File : d:\ceifa0A gc\ceifa0A.Ne\$EA\drive-d\2017\2023\08\blk2023.run  
Method File : C:\star\data\TU\cal2023\baseline FID.mth  
Sample ID : Blk2023

Injection Date: 9/8/2566 13:13 Calculation Date: 9/8/2566 13:34

Operator : watsamon Detector Type: 3800 (10 Volts)  
Workstation: GC-LAB Bus Address : 44  
Instrument : Sample Rate : 10.00 Hz  
Channel : Front = FID Run Time : 21.208 min

\*\* GC Workstation Version 6.41 \*\* 03334-6390-826-0764 \*\*

Chart Speed = 1.03 cm/min Attenuation = 1 Zero Offset = 3%  
Start Time = 0.000 min End Time = 21.208 min Min / Tick = 1.00

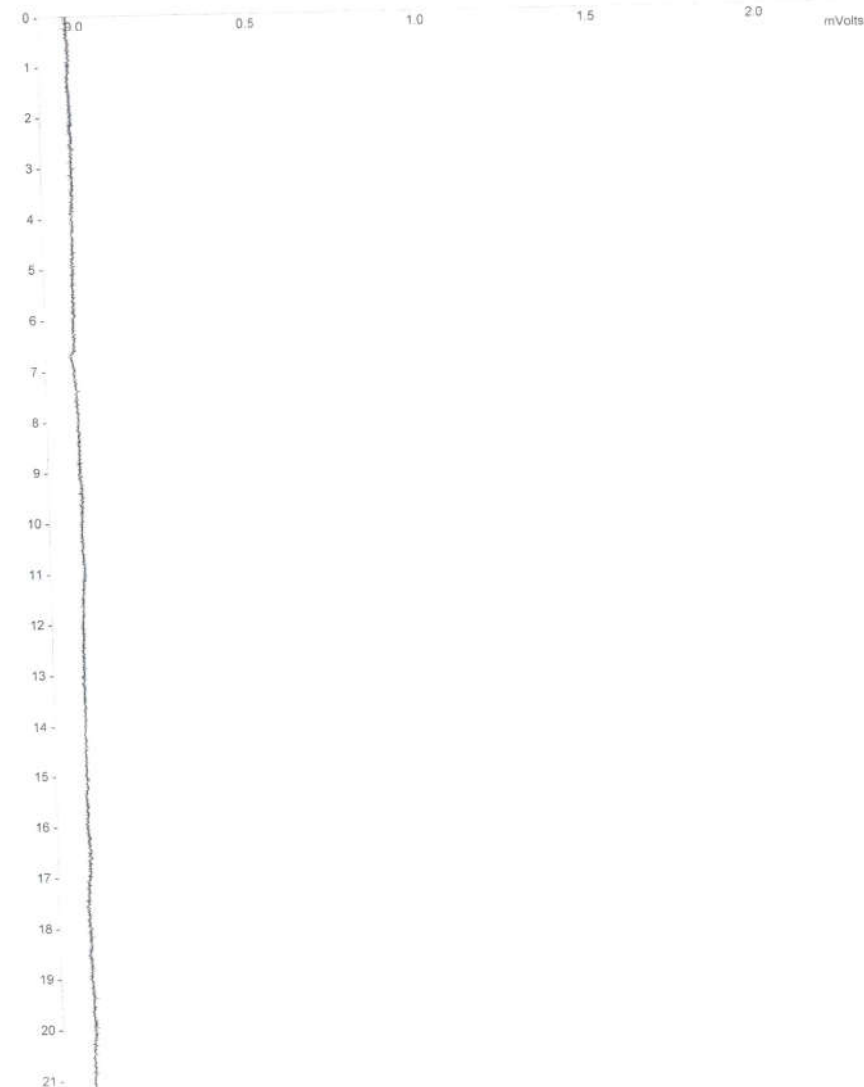

VARIAN

Title :  
Run File : d:\ceifa0A\_gc\ceifa0A\_NeSEA\drive-d\2017\2023\08\blk2023.run  
Method File : C:\star\data\TU\cal2023\baseline FID.mth  
Sample ID : Blk2023

Injection Date: 9/8/2566 13:13 Calculation Date: 9/8/2566 13:34

Operator : watsamon Detector Type: 3800 (10 Volts)  
Workstation: GC-LAB Bus Address : 44  
Instrument : Sample Rate : 10.00 Hz  
Channel : Front = FID Run Time : 21.208 min

\*\* GC Workstation Version 6.41 \*\* 03334-6390-826-0764 \*\*

Run Mode : Blank Baseline  
Peak Measurement: Peak Area  
Calculation Type: External Standard

Peak No.	Peak Name	Result ( )	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
Totals:		0.0000		0.000	0			

Total Unidentified Counts : 0 counts

Detected Peaks: 0 Rejected Peaks: 0 Identified Peaks: 0

Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0

Baseline Offset: -14 microVolts LSB: 1 microVolts

Noise (used): 19 microVolts - monitored before this run

Manual injection

Title :  
Run File : c:\star\data\tu\cal2023\fid\calfid2023003.run  
Method File : d:\method-gc\star c\star\method\cp-wax\without glasswool\calfid2023003-front.mth  
Sample ID : Manual Sample

Injection Date: 9/8/2566 10:31 Calculation Date: 9/8/2566 10:40

Operator : watsamon Detector Type: 3800 (10 Volts)  
Workstation: Local Disk Bus Address : 44  
Instrument : Sample Rate : 10.00 Hz  
Channel : Front = FID Run Time : 7.993 min

\*\* GC Workstation Version 6.41 \*\* 03334-6390-826-0764 \*\*

Run Mode : Analysis  
Peak Measurement: Peak Area  
Calculation Type: External Standard

Peak No.	Peak Name	Result ( )	Ret. Time (min)	Time Offset (min)	Area (counts)	Sep. Code	Width 1/2 (sec)	Status Codes
1	C14	33.8385	3.520	-0.003	362495	BB	2.2	C
2	C15	33.4804	4.125	-0.006	357824	BB	2.3	C
3	C16	32.6143	4.699	-0.001	344951	BB	2.2	
Totals:		99.9332		-0.010	1065270			

Status Codes:

C - Out of calibration range

Total Unidentified Counts : 0 counts

Detected Peaks: 3 Rejected Peaks: 0 Identified Peaks: 3

Multiplier: 1 Divisor: 1 Unidentified Peak Factor: 0

Baseline Offset: 28 microVolts LSB: 1 microVolts

Noise (used): 26 microVolts - monitored before this run

Manual injection

Calib. out of range: No Recovery Action Specified

\*\*\*\*\*


Title :  
Run File : c:\star\data\tu\cal2023\fid\calfid2023003.run  
Method File : d:\method-gc\star c\star\method\cp-wax\without glasswool\calfid2023003-front.mth  
Sample ID : Manual Sample

Injection Date: 9/8/2566 10:31 Calculation Date: 9/8/2566 10:40

Operator : watsamon Detector Type: 3800 (10 Volts)  
Workstation: Local Disk Bus Address : 44  
Instrument : Sample Rate : 10.00 Hz  
Channel : Front = FID Run Time : 7.993 min

\*\* GC Workstation Version 6.41 \*\* Q3334-6390-826-0764 \*\*

Chart Speed = 2.73 cm/min Attenuation = 70 Zero Offset = 2%  
Start Time = 0.000 min End Time = 7.993 min Min / Tick = 1.00

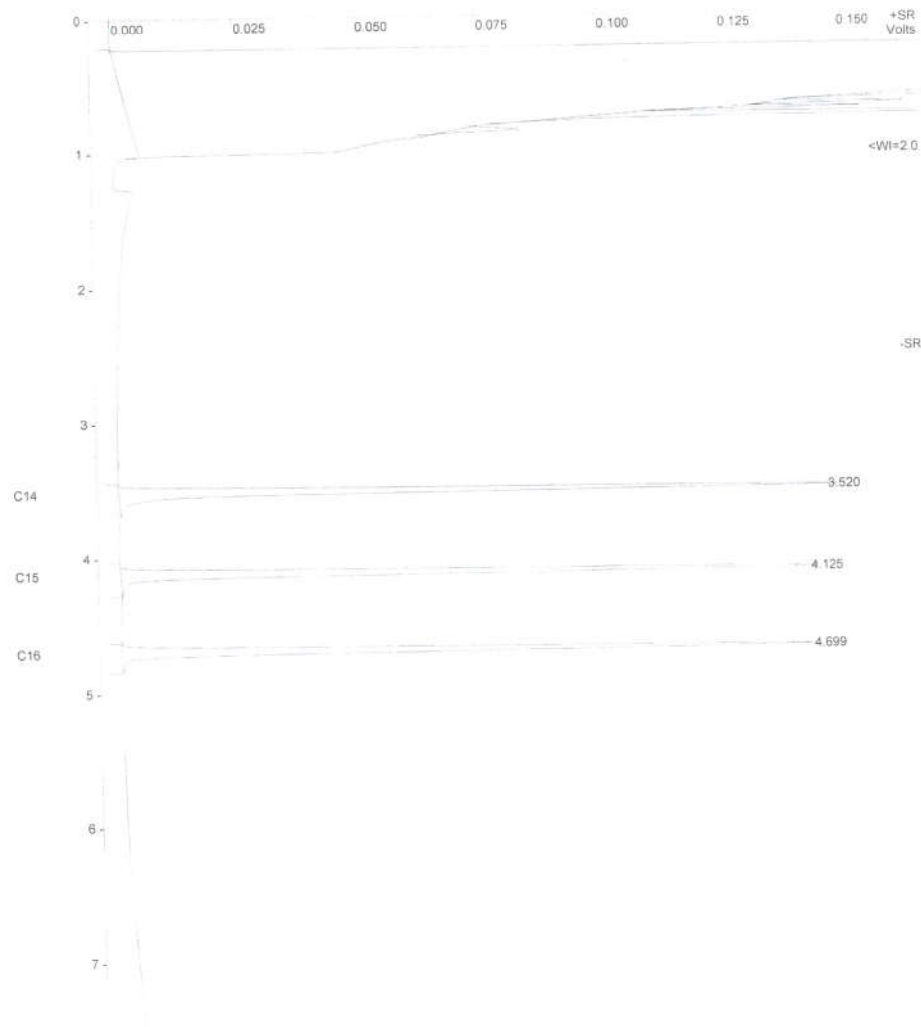

## S.P.S Consulting Service Co.,Ltd.

Sample ID: fid std

Operator (Inj): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (Inj):




**VARIAN**

Run Mode: Analysis  
Peak Measurement: Peak Area  
Calculation Type: External Std.

c:\star\data\tu\cal2023\fid\calfid2023001.run

A = FID 10 V RESULTS

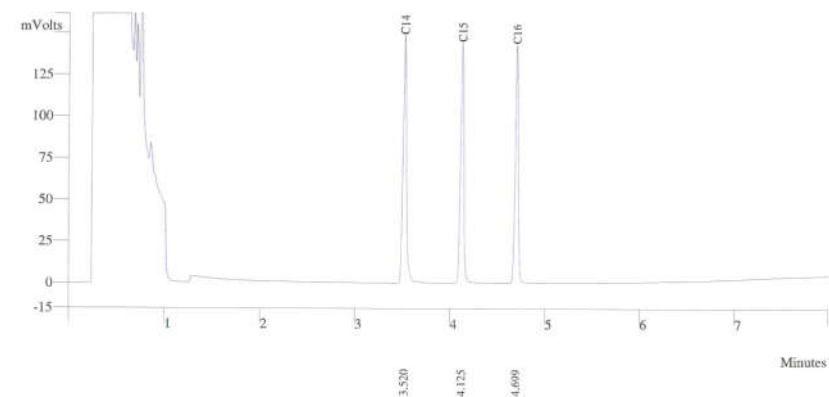

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	359491	BB	2.2
2	C15	33.4804	4.125	357863	BB	2.3
3	C16	32.6143	4.699	344951	BB	2.2
Totals		99.9312		1062305		



THAI UNIQUE CO.,LTD.


Sample ID: **fid std**

Operator (Inj): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (Inj):



c:\star\data\tu\cal2023\fid\calfid2023001.run

A = FID 10 V RESULTS

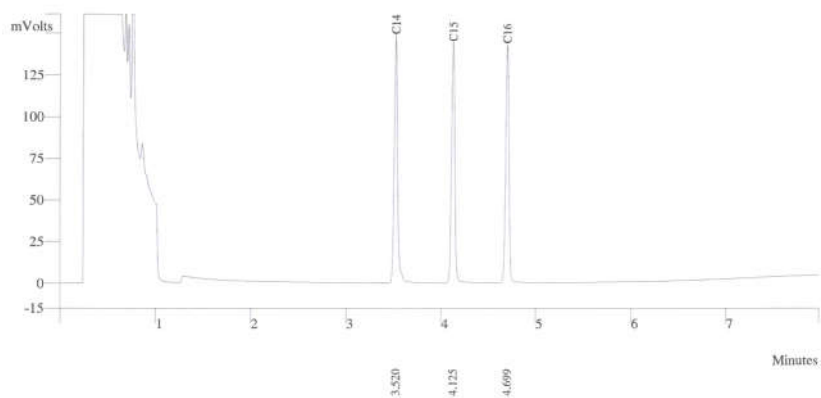

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	362495	BB	2.2
2	C15	33.4804	4.125	357824	BB	2.3
3	C16	32.6143	4.699	344951	BB	2.2
Totals		99.9332		1065270		


Sample ID: **fid std**

Operator (Inj): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (Inj):



c:\star\data\tu\cal2023\fid\calfid2023002.run

A = FID 10 V RESULTS

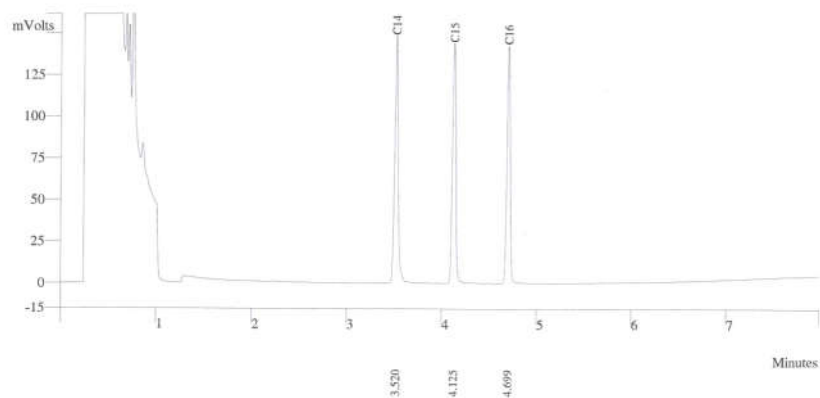

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	362495	BB	2.2
2	C15	33.4824	4.125	367724	BB	2.3
3	C16	32.6143	4.699	354951	BB	2.2
Totals		99.9352		1085170		






Sample ID: **fid std**

Operator (Inj): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (Inj):



c:\star\data\tu\cal2023\fid\calfid2023002.run

A = FID 10 V RESULTS

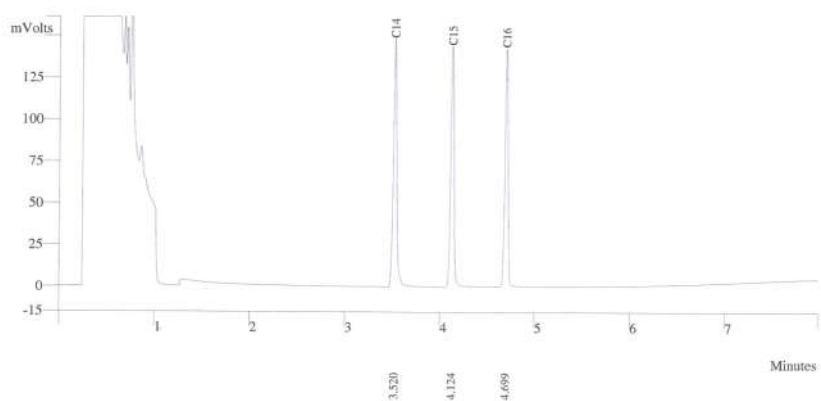

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	362495	BB	2.2
2	C15	33.4824	4.124	361724	BB	2.3
3	C16	32.6143	4.699	354991	BB	2.2
Totals		99.9352		1079210		


Sample ID: **fid std**

Operator (Inj): Suwarot  
Injection Date: 09/08/2023  
Calc Date: 09/08/2023  
Run Time (min): 7.993  
Workstation: Local Disk  
Instrument (Inj):



c:\star\data\tu\cal2023\fid\calfid2023002.run

A = FID 10 V RESULTS

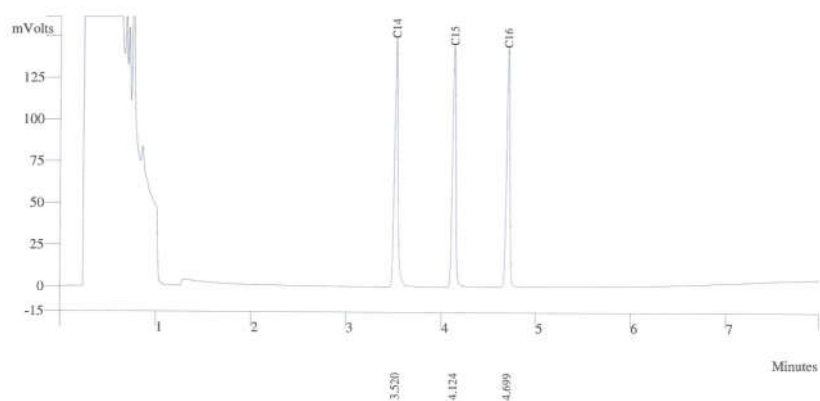

Peak No	Peak Name	Result ()	Ret Time (min)	Peak Area (counts)	Sep. Code	Width 1/2 (sec)
1	C14	33.8385	3.520	362495	BB	2.2
2	C15	33.4824	4.124	369724	BB	2.3
3	C16	32.6143	4.699	354591	BB	2.2
Totals		99.9552		1087210		





Agilent Technologies

## Certificate of Analysis

### FID-TCD Performance Evaluation Sample Kit

**Agilent Part**

Number: 5080-8842, 18710-60170

**Sample Lot**

Number: 0006637856

This analytical reference material was manufactured and verified in accordance with an ISO 9001 registered quality system, and the analyte concentrations were verified by an ISO 17025 accredited laboratory. The certified value for each analyte was determined gravimetrically.

**Concentrations:**

n-tetradecane	0.218 g/L ( $\pm 0.5\%$ )	0.033 w/w %
n-pentadecane	0.218 g/L ( $\pm 0.5\%$ )	0.033 w/w %
n-hexadecane	0.218 g/L ( $\pm 0.5\%$ )	0.033 w/w %

Solvent: hexane


Calibrated Class A glassware and clean bottles were used in the manufacture of this standard. Balances used in the manufacture of this standard are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z-540-1 and ISO 9001.

**Purities:**

n-tetradecane	99.6%
n-pentadecane	99%
n-hexadecane	99%
hexane	99%

**Typical Analytical Spectrum or Chromatography**

GC Chromatography – n-tetradecane, n-pentadecane, and n-hexadecane in hexane

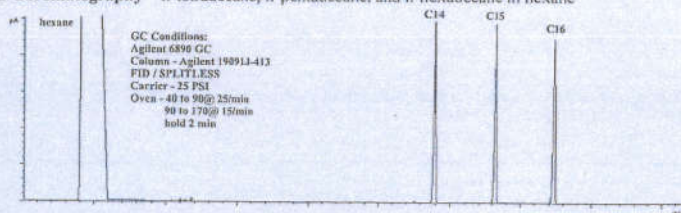

Date of release: 30 September 2021

Date of expiration: 31 October 2023

*Monica Bourgeois*

Monica Bourgeois  
QMS Representative

## Certificate

It is hereby certified that

**Suwarot Trikainut**

Has successfully completed the Application Training for

**Basic Gas Chromatography and Sampler**

Training Contents were:


**Hardware Operation, Software Operation, Data analysis and**

**Troubleshooting : Model**

**CP-3800, 3900, 450-GC, 430-GC, 456-GC, 436-GC**

At Thai Unique Co., Ltd, Bangkok, Thailand

On 15<sup>th</sup> March, 2019



Service Manager

ระดับความร้อน



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Heat 096\_1

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	B30	Verification Date :	10 April 2024
Brand :	3M	Ambient Temp. :	24.5 °C
Model :	QUESTemp <sup>o</sup> 32	Barometric Pressure :	1011 mmbar
Serial No. :	TPH050057	Relative Humidity :	49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.5	0.0	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.1	0.0	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.2	0.1	± 0.5
UUC* = UNIT UNDER CALIBRATION			



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Heat 096\_2

Heat Stress WBGT Meter Verification Report			
Verification Data			
Heat Stress WBGT Meter No. :	B31	Verification Date :	10 April 2024
Brand :	3M	Ambient Temp. :	24.5 °C
Model :	QUESTemp <sup>o</sup> 32	Barometric Pressure :	1011 mmbar
Serial No. :	TPH050047	Relative Humidity :	49 %
Verification Module (Electronic Sensor Check) :			
Verification Module No. : 21 WB = 12.5 °C, DB = 47.1 °C, G = 69.3 °C			
Result of Verification : Without Adjustment			
Wet Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
12.5	12.3	0.2	± 0.5
Dry Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
47.1	47.3	-0.2	± 0.5
Globe Probe Temperature Measurement			
Verification Module Reading (°C)	UUC* Reading (°C)	Correction (°C)	Tolerance Limit (°C)
69.3	69.3	0.0	± 0.5
UUC* = UNIT UNDER CALIBRATION			

Verifie





## Certificate of Calibration

Certificate Number : SPR23110050-4

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,  
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 32

Serial Number : TPH050047

ID. Number : B31

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Received Date : 03 Nov 2023

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 03 Nov 2023

Location of Calibration : In-Lab

Recommend Due Date : 03 Nov 2024

Calibration Procedure : SP-CPT-04-13

Date of Issue : 04 Nov 2023

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Pitak Srisutam

Calibration Officer

Approved by :

(M)

Authorized Signatory



## Calibration Report

Certificate Number : SPR23110050-4

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

Quality Reborn Co., Ltd



## Result of Calibration

Certificate No. : SPR23110050-4

Page : 3 of 3

Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
30.0	30.014	30.1	0.086	0.20
35.0	35.012	35.1	0.088	0.20
40.0	40.017	40.1	0.083	0.20

Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
30.0	30.014	30.1	0.086	0.20
35.0	35.012	35.1	0.088	0.20
40.0	40.017	40.1	0.083	0.20

Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Humidity Setting	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
30.0	30.014	30.2	0.186	0.20
35.0	35.012	35.2	0.188	0.20
40.0	40.017	40.2	0.183	0.20

Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2$ , providing a level of confidence approximately 95%.

- End of Certificate -



# Certificate of Calibration

Certificate Number : SPR23110050-3

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,  
Bangkok 10900

Equipment Name : Area Heat Stress Monitor

Manufacturer : Quest Technologies

Model : QUESTemp 32

Serial Number : TPH050057

ID. Number : B30

### Environmental Conditions

Ambient Temperature : 23 °C ± 2 °C      Received Date : 03 Nov 2023

Relative Humidity : 50 %  $\pm$  15 % Calibration Date : 03 Nov 2023

Location of Calibration : In-Lab      Recommend Due Date : 03 Nov 2024

Calibration Procedure : SP-CPT-04-13 Date of Issue : 04 Nov 2023

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Pitak Srisutam

Calibration Officer

Approved by :

Authorized Signatory



## Calibration Report

Certificate Number : SPR23110050-3

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Humidity Chamber	TH-80S	N/A	SPR23010480-5	22 Feb 2024
THERMO-HYGROMETER	5020A	A47046	QR23-0176	26 Jan 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :

SP Metrology - SP Metrology system (Thailand) Co.Ltd.

Quality Reborn Co., Ltd



## Result of Calibration

Certificate No. : SPR23110050-3

Page : 3 of 3

### Temperature Accuracy in the Measurement. (WET)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
30.0	30.014	30.2	0.186	0.20
35.0	35.012	35.2	0.188	0.20
40.0	40.017	40.2	0.183	0.20

### Temperature Accuracy in the Measurement. (DRY)

Unit : °C

Temperature Setting	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
30.0	30.014	30.1	0.086	0.20
35.0	35.012	35.1	0.088	0.20
40.0	40.017	40.1	0.083	0.20

### Temperature Accuracy in the Measurement. (GLOBE)

Unit : °C

Humidity Setting	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
30.0	30.014	30.2	0.186	0.20
35.0	35.012	35.2	0.188	0.20
40.0	40.017	40.2	0.183	0.20

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2$ , providing a level of confidence approximately 95%.

- End of Certificate -

ระดับความเข้มของแสงสว่าง





ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24010295-4

Page : 1 of 3

Customer : S.P.S. CONSULTING SERVICE CO., LTD.

7 Soi Phaholyothin 24 Phaholyothin Road., Jompol, Chatuchak,  
Bangkok 10900

Equipment Name : Light Meter

Manufacturer : Extech

Model : 407026

Serial Number : A.055615

ID. Number : LUX-B11

### Environmental Conditions

Ambient Temperature :  $23\text{ }^{\circ}\text{C} \pm 3\text{ }^{\circ}\text{C}$

Relative Humidity :  $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-32

Received Date : 19 Jan 2024

Calibration Date : 23 Jan 2024

Recommend Due Date : 23 Jan 2025

Date of Issue : 24 Jan 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Calibration Officer

Approved by

Authorized Signatory

SP-FM-04-15 rev.0



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24010295-4

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Digital Light Meter	LX-73	Q842777	23PH462	05 Sep 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :  
TPA - Technology Promotion Association (Thailand-Japan)

SP-FM-04-15 rev.0



ID LINE : IEC17025



## Result of Calibration

Certificate No. : SPR24010295-4

Page : 3 of 3

Function: Illumination Measurement

Unit : Lux

Calibration Point	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
100	100.0	99	-1	1.7
200	200	199	-1	6.6
300	300	300	0	7
1000	1000	1009	9	13
2000	2000	1980	-20	26
3000	3000	2990	-10	39

### Note:

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95 %

- End of Certificate -

---

หนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการ  
วิเคราะห์เอกชน



ที่ อก ๐๓๑๐(๑)/ ๑๔ ๓ ๒ ๑

กรมโรงงานอุตสาหกรรม  
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท  
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๑ ตุลาคม ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอส.พี.เอส. คอนสตรัคติ้ง เซอร์วิส จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๒๒ มิถุนายน ๒๕๖๖

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น  
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ แผ่น  
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๔ แผ่น  
ตามหนังสือที่อ้างถึง บริษัท เอส.พี.เอส. คอนสตรัคติ้ง เซอร์วิส จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน  
เลขทะเบียน ว-๐๑๑ สถานที่ตั้งเลขที่ ๗ ซอยพหลโยธิน ๒๔ ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร  
กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอส.พี.เอส. คอนสตรัคติ้ง เซอร์วิส จำกัด ต่ออายุ  
หนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๓๔ ราย ตามสิ่งที่ส่งมาด้วย ๑  
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๔๗ ราย ตามสิ่งที่ส่งมาด้วย ๒  
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูล  
หรือวัสดุที่ไม่ใช่แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๑๐ กรกฎาคม ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือ  
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงาน  
อุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ทั้งนี้  
สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

ผู้อำนวยการกองวิจัยและเฝ้าระวังมลพิษโรงงาน  
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเฝ้าระวังมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอส.พี.เอส. คอนสตรัคติ้ง เซอร์วิส จำกัด

เลขทะเบียน ว-๐๑๑

ที่ อก ๐๓๑๐(๑)/ ๑๔ ๓ ๒ ๑

ลงวันที่ ๑๑ ตุลาคม ๒๕๖๖

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๓๔ ราย



สิ่งที่ส่งมาด้วย ๒

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

เลขทะเบียน ว-๐๑๑

ที่ อก ๐๓๑๐(๑)/ ๑๔๓๒๑

ลงวันที่ ๑๑ ตุลาคม ๒๕๖๖

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๔๗ ราย

- ๒ -

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

เลขทะเบียน ๖-๐๑๑

ที่ ออ ๐๓๑๐(๑)/ ๑๔ ๓ ๒ ๑

ลงวันที่ ๑๑ ตุลาคม ๒๕๖๖

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๗๙ รายการ

น้ำเสีย จำนวน 62 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
2	Aldicarb Sulfone	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
3	Aldicarb Sulfoxide	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
5	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
6	Barium	Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
7	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
8	β-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
9	δ-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
10	γ-BHC	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
11	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method <sup>[4]</sup> 2) 5-Day BOD Test, Membrane Electrode Method <sup>[4]</sup>
12	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>

13 Carbaryl...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	Carbaryl	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
14	Carbofuran	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
15	Chemical Oxygen Demand	1) Open Reflux, Titrimetric method <sup>[4]</sup> 2) Closed Reflux, Colorimetric method <sup>[4]</sup> 3) Closed Reflux, Titrimetric Method <sup>[4]</sup>
16	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
17	Chromium	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
18	Color	ADMI Weighted-Ordinate Spectrophotometric Method <sup>[4]</sup>
19	Copper	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
20	Cyanide	Distillation, Colorimetric method <sup>[4]</sup>
21	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
22	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
23	4,4'-DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
24	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
25	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>

25 Endosulfan II...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
26	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
27	Endosulfan Sulfate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
28	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
29	Endrin aldehyde	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
30	Formaldehyde	Distillation, Colorimetric Method <sup>[3]</sup>
31	Free Chlorine	1) Iodometric Method <sup>[4]</sup> 2) DPD Colorimetric Method <sup>[4]</sup>
32	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
33	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
34	Hexavalent Chromium	Colorimetric Method <sup>[4]</sup>
35	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
36	Lead	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
37	Malathion	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
38	Manganese	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
39	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[4]</sup>

40 methiocarb...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	Methiocarb	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
41	Methomyl	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
42	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
43	Methyl parathion	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
44	1-Naphthol	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
45	Nickel	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
46	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method <sup>[4]</sup> 2) Soxhlet Extraction Method <sup>[4]</sup>
47	Oxamyl	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
48	pH	Electrometric Method <sup>[4]</sup>
49	Phenols	1) Distillation, Chloroform Extraction Method <sup>[4]</sup> 2) Distillation, Direct Photometric Method <sup>[4]</sup>
50	Propoxur	High-Performance Liquid Chromatographic Method <sup>[4]</sup>
51	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
52	Settleable Solids	Settleable Solids Method <sup>[4]</sup>
53	Sulfide	1) Iodometric method <sup>[4]</sup> 2) Methylene blue method <sup>[4]</sup>
54	Temperature	Laboratory and Field Methods <sup>[4]</sup>
55	Total Dissolved Solids	Dried at 180 °C <sup>[4]</sup>

56 Kjeldahl Nitrogen...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
56	Total Kjeldahl Nitrogen	Macro-Kjeldahl Method <sup>[4]</sup>
57	Total Phosphorous	Digestion, Colorimetric Method <sup>[4]</sup>
58	Total Suspended Solids	Dried at 103-105 °C <sup>[4]</sup>
59	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
60	Trivalent Chromium	Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation <sup>[4]</sup>
61	Turbidity	Nephelometric Method <sup>[4]</sup>
62	Zinc	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>

น้ำใต้ดิน จำนวน 126 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
2	Acetone	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
3	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
5	Antimony	Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>

8 Barium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Barium	Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
10	Benzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
15	Benzo(g,h,i)perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
16	Beryllium	Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
20	Bromoform	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
21	Butanol	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
23	Cadmium	Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
25	Carbon disulfide	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
27	Chlordane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
29	Chlorobenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
31	Chloroform	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
34	Chromium (III)	Digestion, Inductively Coupled Plasma Spectrometric Method; Colorimetric Method; Calculation <sup>[4]</sup>
35	Chromium (VI)	Colorimetric Method <sup>[4]</sup>
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
37	Cyanide	Distillation, Colorimetric M

38 2,4-D...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[4]</sup>
39	DDD	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
40	DDE	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
41	DDT	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
44	1,2-Dichlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
45	1,3-Dichlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
46	1,4-Dichlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
47	3,3'-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Metho

54 1,2-Dichloropropane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
54	1,2-Dichloropropane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
57	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
64	Endosulfan	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
65	Endrin	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
66	Ethylbenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
69	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>

70 Heptachlor epoxide...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
70	Heptachlor epoxide	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
72	Hexachloro-1,3-butadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
73	n-Hexane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
74	$\alpha$ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
75	$\beta$ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
76	$\gamma$ -HCH	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method <sup>[4]</sup> 3) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
82	Manganese	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>

83 Mercury...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[4]</sup>
84	Methanol	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
86	Methyl bromide	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
87	Methylene chloride	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
89	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
96	Polychlorinated Biphenyls - PCB-1016 - PCB-1221 - PCB-1232	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>

- PCB-1242...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
	- PCB-1242 - PCB-1248 - PCB-1254 - PCB-1260	
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
98	pH	Electrometric method <sup>[4]</sup>
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
100	Phenol	1) Distillation, Chloroform Extraction Method <sup>[4]</sup> 2) Distillation, Direct Photometric Method <sup>[4]</sup>
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
102	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[4]</sup>
103	Silver	Digestion, Inductively Coupled Plasma Method <sup>[4]</sup>
104	Styrene	Purge and Trap Gas Chromatographic/ Mass spectrometric Method <sup>[4]</sup>
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
107	Toluene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
108	Toxaphene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
109	TPH (C <sub>5</sub> -C <sub>8</sub> )	Purge and Trap, Gas Chromatographic Method <sup>[13,22]</sup>
110	TPH (C <sub>9</sub> -C <sub>16</sub> )	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[9,22]</sup>
111	TPH (C <sub>16</sub> -C <sub>35</sub> )	Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[9,22]</sup>

112 1,2,4-Trichlorobenzene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
112	1,2,4-Trichlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
113	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
114	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
115	Trichloroethylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
116	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
117	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
118	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
119	Vanadium	Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>
120	Vinyl acetate	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
121	Vinyl chloride	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
122	m-Xylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
123	o-Xylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
124	p-Xylene	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
125	Xylene (Total)	Purge and Trap Gas Chromatographic/ Mass Spectrometric Method <sup>[4]</sup>
126	Zinc	1) Digestion, Direct Air-Acetylene Flame Method <sup>[4]</sup> 2) Digestion, Inductively Coupled Plasma Spectrometric Method <sup>[4]</sup>

อากาศเสีย...

อากาศเสีย (ปล่องระบาย) จำนวน 28 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
2	Arsenic	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
3	Beryllium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
4	Cadmium	1) Isokinetic Sampling, Digestion, Direct Air- Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
5	Carbon Monoxide	Instrumental Analyzer Method <sup>[5]</sup>
6	Chlorine	1) Absorption Sampling, Ion Chromatographic Method <sup>[5]</sup> 2) Isokinetic Sampling, Ion Chromatographic Method <sup>[5]</sup>
7	Chromium	1) Isokinetic Sampling, Digestion, Direct Air- Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
8	Cobalt	1) Isokinetic Sampling, Digestion, Direct Air- Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
9	Copper	1) Isokinetic Sampling, Digestion, Direct Air- Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>

10 Cresol...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
10	Cresol	Adsorption Sampling, Gas Chromatographic Method <sup>[5]</sup>
11	Dioxins/Furans	Isokinetic Sampling <sup>[5]</sup>
12	Hydrogen Chloride	1) Absorption Sampling, Ion Chromatographic Method <sup>[5]</sup> 2) Isokinetic Sampling, Ion Chromatographic Method <sup>[5]</sup>
13	Hydrogen Fluoride	1) Absorption Sampling, Ion Chromatographic Method <sup>[5]</sup> 2) Isokinetic Sampling, Ion Chromatographic Method <sup>[5]</sup>
14	Hydrogen Sulfide	Absorption Sampling, Iodometric Method <sup>[5]</sup>
15	Lead	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
16	Manganese	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
17	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[5]</sup>
18	Nickel	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method <sup>[5]</sup> 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
19	Opacity	Ringelmann's Method <sup>[2]</sup>
20	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method <sup>[5]</sup> 2) Instrumental Analyzer Method <sup>[5]</sup>
21	Selenium	Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[5]</sup>

22 Sulfur Dioxide...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
22	Sulfur Dioxide	1) Absorption Sampling, Barium-Thorin Titrimetric Method <sup>[5]</sup> 2) Isokinetic Sampling, Barium-Thorin Titrimetric Method <sup>[5]</sup> 3) Instrumental Analyzer Method <sup>[5]</sup>
23	Sulfuric acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method <sup>[5]</sup>
24	Tellurium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
25	Tin	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
26	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method <sup>[5]</sup>
27	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method <sup>[5]</sup>
28	Xylene	1) Adsorption Sampling, Gas Chromatographic Method <sup>[5]</sup> 2) Adsorption Sampling, Gas Chromatographic/Mass Spectrometric Method <sup>[5]</sup>

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 38 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acrylonitrile	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[1,13,27]</sup> 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
2	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,9,23]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>

3 Antimony...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
3	Antimony	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
4	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[1,6,17]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,17]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
5	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
6	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
7	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>

8 Chlordane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,28]</sup> 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
9	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method <sup>[1,18]</sup> 2) Alkaline Digestion, Colorimetric Method <sup>[8,18]</sup>
11	Cobalt	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>

13 2,4-D...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	2,4-D	1) Waste Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[1,26]</sup>
		2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[26]</sup>
14	DDD	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic Method <sup>[1,9,23]</sup>
		2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
15	DDE	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic Method <sup>[1,9,23]</sup>
		2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
16	DDT	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic Method <sup>[1,9,23]</sup>
		2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic Method <sup>[1,9,23]</sup>
		2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic Method <sup>[1,9,23]</sup>
		2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic Method <sup>[1,9,23]</sup>

2) Soxhlet Extraction...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
20	Kepone	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,28]</sup>
		2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[11,28]</sup>
21	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup>
		2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup>
		3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup>
		4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
22	Lindane	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,28]</sup>
		2) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method <sup>[10,28]</sup>
23	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[1,19]</sup>
		2) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[20]</sup>
24	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic Method <sup>[1,9,23]</sup>
		2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
25	Mirex	1) Waste Extraction, Separatory Funnel Liquid- Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,28]</sup>
		2) Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>

26 Molybdenum...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
26	Molybdenum	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
27	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
28	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,28]</sup> 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
29	Pentachlorophenol	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,28]</sup> 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
30	pH	Electrometric Method <sup>[32,33]</sup>

31 Selenium...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[1,6,21]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,21]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
32	Silver	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
33	Silvex	1) Waste Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,26]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[26]</sup>
34	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
35	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,28]</sup> 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>

36 Trichloroethylene...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
36	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[1,13,27]</sup> 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
37	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
38	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,6,16]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,6,15]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>

**ดิน จำนวน 125 รายการ**

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
2	Acetone	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
3	Aldrin	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
4	Anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
5	Antimony	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>

6 Arsenic...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,17]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
7	Atrazine	Soxhlet Extraction, Gas Chromatographic Method <sup>[10,25]</sup>
8	Barium	Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
9	Benz(a)anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
10	Benzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
11	Benzo(b)fluoranthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
12	Benzo(k)fluoranthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
13	Benzoic acid	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
14	Benzo(a)pyrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
15	Benzo(g,h,i)perylene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
16	Beryllium	Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
17	Bis(2-chloroethyl)ether	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
18	Bis(2-ethylhexyl)phthalate	Soxhlet Extraction, Gas Chromatographic Method <sup>[10,24]</sup>
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
20	Bromoform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>

Butanol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
21	Butanol	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
22	Butyl benzyl phthalate	Soxhlet Extraction, Gas Chromatographic Method <sup>[10,24]</sup>
23	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
24	Carbazole	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
27	Chlordane	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
28	p-Chloroaniline	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
31	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
32	2-Chlorophenol	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
34	Chromium (III)	Digestion, Inductively Coupled Plasma Method; Alkaline Digestion Colorimetric Calculation <sup>[7,8,15,18]</sup>

35 Chromium (VI)...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method <sup>[8,18]</sup>
36	Chrysene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
37	Cyanide	Extraction, Distillation, Colorimetric Method <sup>[29,30,31]</sup>
38	2,4-D	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[26]</sup>
39	DDD	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
40	DDE	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
41	DDT	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
42	Dibenz(a,h)anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
43	Di-n-butyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
44	1,2-Dichlorobenzene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
45	1,3-Dichlorobenzene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
46	1,4-Dichlorobenzene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
47	3,3'-Dichlorobenzidine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>

52 trans-1,2-Dichloroethylene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
53	2,4-Dichlorophenol	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
57	Dieldrin	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
58	Diethyl phthalate	Soxhlet Extraction, Gas Chromatographic Method <sup>[10,24]</sup>
59	2,4-Dimethylphenol	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
60	2,4-Dinitrophenol	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
61	2,4-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
62	2,6-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
63	Di-n-Octyl phthalate	Soxhlet Extraction, Gas Chromatographic Method <sup>[10,24]</sup>
64	Endosulfan	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
65	Endrin	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
67	Fluoranthene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
68	Fluorene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
69	Heptachlor	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
70	Heptachlor epoxide	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
71	Hexachlorobenzene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
72	Hexachloro-1,3-butadiene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
73	n-Hexane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
74	$\alpha$ -HCH	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
75	$\beta$ -HCH	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
76	$\gamma$ -HCH	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
77	Hexachlorocyclopentadiene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
78	Hexachloroethane	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
79	Indeno(1,2,3-cd)pyrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
80	Isophorone	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
81	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 2) Digestion, Inductively Coupled Plasma Atomic Emission Spectrometric Method <sup>[7,15]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
82	Manganese	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[20]</sup>
84	Methanol	Equilibrium Headspace, Gas chromatographic Method <sup>[12,22]</sup>
85	Methoxychlor	Soxhlet Extraction, Gas Chromatographic Method <sup>[10,23]</sup>
86	Methyl bromide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
87	Methylene chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
88	2-Methylphenol	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
89	2-Methylnaphthalene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
91	Naphthalene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
92	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
93	Nitrobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
94	N-Nitrosodiphenylamine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
95	N-Nitrosodi-n-propylamine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Meth

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
96	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
97	Pentachlorophenol	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
98	Phenanthrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
99	Phenol	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
100	Pyrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
101	Selenium	Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[7,21]</sup>
102	Silver	Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
103	Styrene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
106	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
107	Toxaphene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
108	TPH (C <sub>5</sub> -C <sub>8</sub> )	Purge and Trap, Gas Chromatographic Method <sup>[14,22]</sup>

H (C<sub>8</sub>-C<sub>16</sub>)...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
109	TPH (C <sub>8</sub> -C <sub>16</sub> )	Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup>
110	TPH (C <sub>16</sub> -C <sub>35</sub> )	Soxhlet Extraction, Gas Chromatographic Method <sup>[10,22]</sup>
111	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
112	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
113	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
114	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
115	2,4,5-Trichlorophenol	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
116	2,4,6-Trichlorophenol	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[10,28]</sup>
117	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
118	Vanadium	Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>
119	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
120	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
121	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
122	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
123	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>
124	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[14,27]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
125	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[7,16]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[7,15]</sup>

#### เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.ราชกิจจานุเบกษา. 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.
- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แก๊สเป็นเชื้อเพลิง.ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.
- สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. คู่มือวิเคราะห์น้ำเสีย. พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.
- APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 24<sup>th</sup> ed. Washington, DC: APHA, 2023.
- United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2023.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods**. SW-846, 2014.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils**. SW-846 Method 3050B, 1996.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium**. SW-846 Method 3060A, 1996.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction**. SW-846 Method 3510C, 1996.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soxhlet Extraction**. SW-846 Method 3540C, 1996.
- United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction**. SW-846 Method 3550C, 2007

12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A**, 2014.
13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Purge-and-Trap for Aqueous Samples. SW-846 Method 5030C**, 2003.
14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Closed-System Purge-and-Trap And Extraction For Volatile Organics in Soil and Waste Samples. SW-846 Method 5035A**, 2002.
15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-optical Emission Spectrometry. SW-846 Method 6010D**, 2018
16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B**, 2007.
17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Arsenic (Atomic Absorption, Gaseous Hydride). SW-846 Method 7061A**, 1992.
18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric), SW-846 Method 7196A**, 1992.
19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold-Vapor Technique, SW-846 Method 7470A**, 1994.
20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique, SW-846 Method 7471B**, 2007.
21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Gaseous Hydride), SW-846 Method 7741A**, 1994.
22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D**, 2003

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticide by Gas Chromatography. SW-846 Method 8081B**, 2007.
24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Phthalate Esters by Gas Chromatography with Electron Capture Detection (GC/ECD). SW-846 Method 8061A**, 1996.
25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organophosphorus Compounds by Gas Chromatography. SW-846 Method 8141B**, 2007.
26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chlorinated Herbicides By GC Using Methylation or Pentafluorobenzoylation Derivatization. SW-846 Method 8151A**, 1996.
27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8260D**, 2018.
28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **SemiVolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E**, 2018.
29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation. SW-846 Method 9010C**, 2004.
30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oils. SW-846 Method 9013A**, 2014.
31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric. SW-846 Method 9014**, 2014.
32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C**, 2004.
33. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Solid and Waste pH. SW-846 Method 9045D**, 2004.

ที่ อก ๐๓๑๐(๑)/๖๖๖



กรมโรงงานอุตสาหกรรม  
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท  
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๕ มกราคม ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากรและเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ

เรียน กรรมการผู้จัดการ บริษัท เอส.พี.เอส คอนสตรัคชั่น เซอร์วิส จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๒๖ ธันวาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ  
บริษัท เอส.พี.เอส คอนสตรัคชั่น เซอร์วิส จำกัด จำนวน ๘ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอส.พี.เอส คอนสตรัคชั่น เซอร์วิส จำกัด ห้องปฏิบัติการวิเคราะห์  
เอกชน เลขทะเบียน ว-๐๑๑ สถานที่ตั้งเลขที่ ๗ ซอยพหลโยธิน ๒๔ ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร  
กรุงเทพมหานคร แจ้งขอเปลี่ยนแปลงบุคลากรและเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษในสิ่งปฏิกูลหรือ  
วัสดุที่ไม่ใช้แล้วของห้องปฏิบัติการวิเคราะห์ นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว มีความเห็นให้เปลี่ยนแปลงดังนี้

๑. ให้ยกเลิกผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ ราย

๒. ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑ ราย

๓. ให้ยกเลิกผู้ช่วยห้องปฏิบัติการวิเคราะห์ จำนวน ๒ คน ได้แก่

๔. ให้ยกเลิกขอบข่ายรายการสารมลพิษในสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว ตามรายการ  
เอกสารแนบท้ายหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๑๑ ตุลาคม ๒๕๖๖

๕. ให้วิเคราะห์สารมลพิษตามขอบข่ายที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในสิ่งปฏิกูลหรือ  
วัสดุที่ไม่ใช้แล้ว จำนวน ๓๘ รายการ ตามเอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและเอกสารอ้างอิง  
วิธีวิเคราะห์สารมลพิษ ดังสิ่งที่ส่งมาด้วย

-๒-

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
คือในวันที่ ๑๐ กรกฎาคม ๒๕๖๙ ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงาน  
อุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

นักวิทยาศาสตร์เชี่ยวชาญ รักษาการแทน  
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน  
ปฏิบัติการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๔

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

อนึ่ง...



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”





เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและเอกสารอ้างอิงวิธีวิเคราะห์สารมลพิษ

บริษัท เอส.พี.เอส. คอนสตรัคชั่น เซอร์วิส จำกัด

เลขทะเบียน ว-๐๑๑

ที่ ออก ๐๓๑๐(๑)/ ๖๖๖

ลงวันที่ ๒๔ มกราคม ๒๕๖๗

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๘ รายการ

สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว 38 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acrylonitrile	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,23]</sup> 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[10,23]</sup>
2	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,5,19]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[6,19]</sup>
3	Antimony	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,2,12]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[3,12]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
4	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[1,2,13]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[3,13]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
5	Barium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
6	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
7	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,2,12]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[3,12]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>

8 Chlordane...

-๒-

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,5,24]</sup> 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[6,24]</sup>
9	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,2,12]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[3,12]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method <sup>[1,14]</sup> 2) Alkaline Digestion, Colorimetric Method <sup>[4,14]</sup>
11	Cobalt	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,2,12]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[3,12]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,2,12]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[3,12]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
13	2,4-D	1) Waste Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[22]</sup>
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,5,19]</sup> 2) Soxhlet Extraction, Gas Chromatographic Method <sup>[6,19]</sup>

15 DDE...



ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,5,19]</sup>
16	DDT	2) Soxhlet Extraction, Gas Chromatographic Method <sup>[6,19]</sup>
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,5,19]</sup>
18	Endrin	2) Soxhlet Extraction, Gas Chromatographic Method <sup>[6,19]</sup>
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,5,19]</sup>
20	Kepone	2) Soxhlet Extraction, Gas Chromatographic Method <sup>[6,19]</sup>
21	Lead	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,5,24]</sup>
22	Lindane	2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[7,24]</sup>
23	Mercury	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,2,12]</sup>
24	Methoxychlor	2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup>
		3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[3,12]</sup>
		4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
		1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,5,24]</sup>
		2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[6,24]</sup>
		1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[1,15]</sup>
		2) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method <sup>[16]</sup>
		1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method <sup>[1,5,19]</sup>
		2) Soxhlet Extraction, Gas Chromatographic Method <sup>[6,19]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
25	Mirex	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,5,24]</sup>
26	Molybdenum	2) Soxhlet Extraction, Gas Chromatographic Method <sup>[6,19]</sup>
27	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,2,12]</sup>
28	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup>
29	Pentachlorophenol	3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[3,12]</sup>
30	pH	4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
		1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,5,24]</sup>
		2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[6,24]</sup>
		Electrometric Method <sup>[28,29]</sup>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
31	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[1,2,17]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method <sup>[3,17]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
32	Silver	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,2,12]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[3,12]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
33	Silvex	1) Waste Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,22]</sup> 2) Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[22]</sup>
34	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 2) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>
35	Toxaphene	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[1,5,24]</sup> 2) Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method <sup>[6,24]</sup>
36	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[1,9,23]</sup> 2) Purge and Trap, Gas Chromatographic/Mass Spectrometric Method <sup>[10,23]</sup>
37	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 2) Digestion, Inductively Coupled Plasma Method

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
38	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method <sup>[1,2,12]</sup> 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method <sup>[1,2,11]</sup> 3) Digestion, Flame Atomic Absorption Spectrometric Method <sup>[3,12]</sup> 4) Digestion, Inductively Coupled Plasma Method <sup>[3,11]</sup>

#### เอกสารอ้างอิง

- กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2566. เรื่องการจัดการสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว. ราชกิจจานุเบกษา. 31 พฤษภาคม 2566. เล่ม 140 ตอนพิเศษ 126 ง.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846, 2014.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Soxhlet Extraction. SW-846 Method 3540C, 1996.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Ultrasonic Extraction. SW-846 Method 3550C, 2007.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds in Various Sample Matrices Using Equilibrium Headspace Analysis. SW-846 Method 5021A, 2014.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Purge-and-Trap for Aqueous Samples. SW-846 Method 5030C, 2003.
- United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed-System Purge-and-Trap And Extraction For Volatile Organics in Soil and Waste Samples. SW-846 Method 5035A, 2002.

11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-optical Emission Spectrometry. SW-846 Method 6010D**, 2018
12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B**, 2007.
13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Arsenic (Atomic Absorption, Gaseous Hydride). SW-846 Method 7061A**, 1992.
14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric), SW-846 Method 7196A**, 1992.
15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold-Vapor Technique, SW-846 Method 7470A**, 1994.
16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique, SW-846 Method 7471B**, 2007.
17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Gaseous Hydride), SW-846 Method 7741A**, 1994.
18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D**, 2003.
19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticide by Gas Chromatography. SW-846 Method 8081B**, 2007.
20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Phthalate Esters by Gas Chromatography with Electron Capture Detection (GC/ECD). SW-846 Method 8061A**, 1996.
21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organophosphorus Compounds by Gas Chromatography. SW-846 Method 8141B**, 2007.
22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chlorinated Herbicides By GC Using Methylation or Pentafluorobenzoylation Derivatization. SW-846 Method 8151A**, 1996.
23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/Mass Spectrometry (GC/MS). SW-846 Method 8210D**, 2018.

24. United...

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **SemiVolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E**, 2018.
25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation. SW-846 Method 9010C**, 2004.
26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oils. SW-846 Method 9013A**, 2014.
27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric. SW-846 Method 9014**, 2014.
28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C**, 2004.
29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Solid and Waste pH. SW-846 Method 9045C**, 2004.



ที่ อก ๐๓๑๐(๑)/ ๒๐๗๒



กรมโรงงานอุตสาหกรรม  
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท  
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๐๕ มีนาคม ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอส.พี.เอส. คอนสตรัคชั่น เซอร์วิส จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๘ กุมภาพันธ์ ๒๕๖๗

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์  
บริษัท เอส.พี.เอส. คอนสตรัคชั่น เซอร์วิส จำกัด จำนวน ๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอส.พี.เอส. คอนสตรัคชั่น เซอร์วิส จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน  
เลขทะเบียน ๖-๐๑๑ สถานที่ตั้งเลขที่ ๗ ซอยพหลโยธิน ๒๔ ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร  
กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์ ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้วมีความเห็นดังนี้

๑. ให้ยกเลิกผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย

๑  
๒

๒. ให้ยกเลิกผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ ราย

๓. ให้เพิ่มขอบข่ายสารมลพิษที่วิเคราะห์ในดิน ตามสิ่งที่ส่งมาด้วย

อนึ่ง หนังสือฉบับนี้จะหมดอายุพร้อมหนังสือต่ออายุรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน  
คือในวันที่ ๑๐ กรกฎาคม ๒๕๖๙ ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ทั้งหน้าเว็บไซต์  
กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



“อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว”



เอกสารแนบท้ายหนังสือเปลี่ยนแปลงบุคลากรและสารมลพิษที่วิเคราะห์

บริษัท เอส.พี.เอส. คอนสตรัคชั่น เซอร์วิส จำกัด


เลขทะเบียน ๖-๐๑๑

ที่ อก ๐๓๑๐(๑)/ ๒๐๗๒

ลงวันที่ ๐๕ มีนาคม ๒๕๖๗

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑ รายการ

ดิน จำนวน 1 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method 

เอกสารอ้างอิง

1. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Closed-System Purge-and-Trap And Extraction For Volatile Organics in Soil and Waste Samples. SW-846 Method 5035A, 2002.

2. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8260D, 2018.

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ กองวิจัยและเตือนภัยมลพิษโรงงาน กรมโรงงานอุตสาหกรรม โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕



ที่ อก ๐๓๑๐(๑)/ ๓๘๕๖



กรมโรงงานอุตสาหกรรม  
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท  
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๑๘ เมษายน ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท เอส.พี.เอส คอนสตรัคชั่น เซอร์วิส จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน  
ลงวันที่ ๑๙ มีนาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท เอส.พี.เอส คอนสตรัคชั่น เซอร์วิส จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน  
เลขทะเบียน ว-๐๑๑ สถานที่ตั้งเลขที่ ๗ ซอยพหลโยธิน ๒๔ ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร  
กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์  
จำนวน ๒ ราย ได้แก่

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

รองอธิบดี ปฏิบัติราชการแทน  
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๕๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๕๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

