

## ภาคผนวกที่ 4

เอกสารสอบเทียบความถูกต้องของเครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
<b>1. คุณภาพอากาศในบรรยากาศ</b>		
TSP	High Volume Air Sampler No. B02, B03, B14, B34	Digital Balance
PM-10	High Volume PM-10 Air Sampler No. B05, B14, B15, B20	Digital Balance
NO <sub>2</sub>	SO <sub>2</sub> Analyzer No. B05, B07, B11, B12	SO <sub>2</sub> Analyzer No. B05, B07, B11, B12
SO <sub>2</sub>	NO <sub>2</sub> Analyzer No. B10, B20, B21, B22	NO <sub>2</sub> Analyzer No. B10, B20, B21, B22
<b>2. คุณภาพอากาศจากปล่อง</b>		
Total Suspended Particulate (TSP)	Console No. B03, B04 Pitot Tube No. B04, B49	Digital Balance
Oxides of Nitrogen (NO <sub>x</sub> )	Vacuum Gauge	Spectrophotometer
Sulfur Dioxide (SO <sub>2</sub> )	Personal Pump SKC No. B16, B40 Rotameter No. H-B08	Digital Balance
<b>3. ระดับเสียงในบรรยากาศ</b>		
L <sub>eq</sub> 1 hr, L <sub>eq</sub> 8 hr, L <sub>eq</sub> 24 hr, L <sub>dn</sub> , L <sub>max</sub> และ L <sub>90</sub>	Acoustic Calibrator Sound Level Meter No. ACO-B34, B37, B38, B43	-
<b>4. คุณภาพน้ำ</b>		
Temperature	-	Thermometer
Conductivity	-	Conductivity Meter
Turbidity	-	Turbidity Meter
Color	-	Spectrophotometer
pH	-	pH Meter
BOD <sub>5</sub>	-	BOD Analyzer
COD	-	COD Reactor
Total Suspended Solids	-	Digital Balance
Total Dissolved Solids	-	Digital Balance
Grease & Oil	-	Digital Balance
Nitrate-Nitrogen	-	Spectrophotometer
Phosphate-Phosphorus	-	Spectrophotometer
Cadmium	-	ICP
Lead	-	ICP
Mercury	-	AAS
Manganese	-	ICP
Fluoride	-	Spectrophotometer
Sulfate	-	Spectrophotometer
Total Iron	-	ICP

ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม (ต่อ)

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
5. ระดับเสียงในสถานที่ทำงาน L <sub>eq</sub> 8 hr, L <sub>max</sub> และ Noise Dose	Acoustic Calibrator Sound Level Meter No. NMD-B12, B15	-
6. คุณภาพอากาศในสถานประกอบการ Total Dust	Personal Pump SKC No. B37, B52 Rotameter No. H-B06	Digital Balance
Respirable Dust	Personal Pump SKC No. B13, B53 Rotameter No. H-B06	Digital Balance

คุณภาพอากาศในบรรยากาศ





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE S025A

S/N : 3611

#### Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B01	B01	01/02/2024	y = 1.224x-3.492	0.998
B02	B02	01/02/2024	y = 1.143x+1.630	0.999
B03	B03	01/02/2024	y = 1.160x-2.783	1.000
B04	B04	02/02/2024	y = 1.257x-5.884	0.997
B05	B05	03/02/2024	y = 1.261x-7.123	0.999
B06	B06	02/02/2024	y = 1.245x-6.024	0.999
B07	B07	03/02/2024	y = 1.209x-6.025	0.997
B08	B08	02/02/2024	y = 1.239x-5.848	0.997
B09	B09	02/02/2024	y = 1.244x-5.247	0.997
B10	B10	02/02/2024	y = 1.153x+0.064	0.998
B11	B11	01/02/2024	y = 1.110x-1.064	1.000
B12	B12	03/02/2024	y = 1.227x-6.093	0.999
B13	B13	01/02/2024	y = 1.286x-7.460	1.000
B14	B14	02/02/2024	y = 1.220x-5.066	0.999
B15	B15	02/02/2024	y = 1.150x-1.264	0.999
B16	B16	03/02/2024	y = 1.177x-3.231	0.996
B17	B17	02/02/2024	y = 1.235x-5.039	0.999
B18	B18	03/02/2024	y = 1.210x-5.028	0.998
B19	B19	03/02/2024	y = 1.215x-7.087	0.998
B20	B20	02/02/2024	y = 1.204x-4.119	0.996
B21	B21	02/02/2024	y = 1.190x-4.960	0.999
B22	B22	02/02/2024	y = 1.208x-7.133	0.996
B23	B23	01/02/2024	y = 1.217x-4.085	0.998
B24	B24	01/02/2024	y = 1.145x-2.502	1.000
B25	B25	02/02/2024	y = 1.090x+1.068	0.999
B26	B26	03/02/2024	y = 1.234x-5.493	0.998
B27	B27	01/02/2024	y = 1.168x-4.382	0.999
B28	B28	02/02/2024	y = 1.237x-7.962	0.999
B29	B29	03/02/2024	y = 1.186x-2.530	0.996
B30	B30	02/02/2024	y = 1.212x-4.090	0.997
B31	B31	02/02/2024	y = 1.195x-4.732	0.999
B32	B32	03/02/2024	y = 1.169x-0.802	0.996
B33	B33	03/02/2024	y = 1.203x-2.954	0.996
B34	B34	02/02/2024	y = 1.221x-5.796	1.000

Calibrated by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

### High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

#### Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B01	B01	02/02/2024	$y = 1.147x - 0.194$	0.996
B02	B02	01/02/2024	$y = 1.060x + 2.506$	1.000
B03	B03	01/02/2024	$y = 1.216x - 3.895$	0.996
B04	B04	01/02/2024	$y = 1.224x - 5.960$	0.999
B05	B05	02/02/2024	$y = 1.220x - 5.384$	0.999
B06	B06	02/02/2024	$y = 1.197x - 4.228$	0.998
B07	B07	03/02/2024	$y = 1.208x - 4.865$	0.996
B08	B08	01/02/2024	$y = 1.171x - 1.266$	0.998
B09	B09	01/02/2024	$y = 1.198x - 5.197$	0.997
B10	B10	01/02/2024	$y = 1.219x - 5.339$	0.997
B11	B11	03/02/2024	$y = 1.211x - 3.765$	0.999
B12	B12	05/02/2024	$y = 1.203x - 3.968$	0.997
B13	B13	05/02/2024	$y = 1.158x - 1.909$	0.996
B14	B14	03/02/2024	$y = 1.190x - 3.316$	0.999
B15	B15	01/02/2024	$y = 1.163x - 1.150$	0.999
B16	B16	01/02/2024	$y = 1.170x + 0.508$	0.999
B17	B17	01/02/2024	$y = 1.186x - 2.843$	0.997
B18	B18	01/02/2024	$y = 1.207x - 1.821$	1.000
B19	B19	03/02/2024	$y = 1.178x - 2.990$	0.999
B20	B20	02/02/2024	$y = 1.206x - 5.507$	0.997
B21	B21	03/02/2024	$y = 1.172x - 0.702$	0.999
B22	B22	02/02/2024	$y = 1.175x - 1.992$	0.996
B23	B23	02/02/2024	$y = 1.196x - 3.382$	0.998
B24	B24	01/02/2024	$y = 1.181x - 2.463$	0.999
B25	B25	01/02/2024	$y = 1.204x - 3.960$	0.997
B26	B26	01/02/2024	$y = 1.218x - 5.354$	0.998
B27	B27	03/02/2024	$y = 1.178x - 4.891$	0.997
B28	B28	02/02/2024	$y = 1.226x - 6.323$	0.999
B29	B29	05/02/2024	$y = 1.174x - 3.753$	0.997
B30	B30	03/02/2024	$y = 1.179x - 3.207$	0.998
B31	B31	03/02/2024	$y = 1.189x - 1.040$	0.997
B32	B32	01/02/2024	$y = 1.222x - 3.815$	0.999
B33	B33	01/02/2024	$y = 1.159x - 1.689$	0.996
B34	B34	01/02/2024	$y = 1.191x - 1.278$	0.995

Calibrated by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE S025A

S/N : 3611

#### Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B01	B01	01/02/2024	y = 1.224x-3.492	0.998
B02	B02	01/02/2024	y = 1.143x+1.630	0.999
B03	B03	01/02/2024	y = 1.160x-2.783	1.000
B04	B04	02/02/2024	y = 1.257x-5.884	0.997
B05	B05	03/02/2024	y = 1.261x-7.123	0.999
B06	B06	02/02/2024	y = 1.245x-6.024	0.999
B07	B07	03/02/2024	y = 1.209x-6.025	0.997
B08	B08	02/02/2024	y = 1.239x-5.848	0.997
B09	B09	02/02/2024	y = 1.244x-5.247	0.997
B10	B10	02/02/2024	y = 1.153x+0.064	0.998
B11	B11	01/02/2024	y = 1.110x-1.064	1.000
B12	B12	03/02/2024	y = 1.227x-6.093	0.999
B13	B13	01/02/2024	y = 1.286x-7.460	1.000
B14	B14	02/02/2024	y = 1.220x-5.066	0.999
B15	B15	02/02/2024	y = 1.150x-1.264	0.999
B16	B16	03/02/2024	y = 1.177x-3.231	0.996
B17	B17	02/02/2024	y = 1.235x-5.039	0.999
B18	B18	03/02/2024	y = 1.210x-5.028	0.998
B19	B19	03/02/2024	y = 1.215x-7.087	0.998
B20	B20	02/02/2024	y = 1.204x-4.119	0.996
B21	B21	02/02/2024	y = 1.190x-4.960	0.999
B22	B22	02/02/2024	y = 1.208x-7.133	0.996
B23	B23	01/02/2024	y = 1.217x-4.085	0.998
B24	B24	01/02/2024	y = 1.145x-2.502	1.000
B25	B25	02/02/2024	y = 1.090x+1.068	0.999
B26	B26	03/02/2024	y = 1.234x-5.493	0.998
B27	B27	01/02/2024	y = 1.168x-4.382	0.999
B28	B28	02/02/2024	y = 1.237x-7.962	0.999
B29	B29	03/02/2024	y = 1.186x-2.530	0.996
B30	B30	02/02/2024	y = 1.212x-4.090	0.997
B31	B31	02/02/2024	y = 1.195x-4.732	0.999
B32	B32	03/02/2024	y = 1.169x-0.802	0.996
B33	B33	03/02/2024	y = 1.203x-2.954	0.996
B34	B34	02/02/2024	y = 1.221x-5.796	1.000

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard


Model : TE 5025A

S/N : 3611

#### Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B01	B01	02/02/2024	$y = 1.147x - 0.194$	0.996
B02	B02	01/02/2024	$y = 1.060x + 2.506$	1.000
B03	B03	01/02/2024	$y = 1.216x - 3.895$	0.996
B04	B04	01/02/2024	$y = 1.224x - 5.960$	0.999
B05	B05	02/02/2024	$y = 1.220x - 5.384$	0.999
B06	B06	02/02/2024	$y = 1.197x - 4.228$	0.998
B07	B07	03/02/2024	$y = 1.208x - 4.865$	0.996
B08	B08	01/02/2024	$y = 1.171x - 1.266$	0.998
B09	B09	01/02/2024	$y = 1.198x - 5.197$	0.997
B10	B10	01/02/2024	$y = 1.219x - 5.339$	0.997
B11	B11	03/02/2024	$y = 1.211x - 3.765$	0.999
B12	B12	05/02/2024	$y = 1.203x - 3.968$	0.997
B13	B13	05/02/2024	$y = 1.158x - 1.909$	0.996
B14	B14	03/02/2024	$y = 1.190x - 3.316$	0.999
B15	B15	01/02/2024	$y = 1.163x - 1.150$	0.999
B16	B16	01/02/2024	$y = 1.170x + 0.508$	0.999
B17	B17	01/02/2024	$y = 1.186x - 2.843$	0.997
B18	B18	01/02/2024	$y = 1.207x - 1.821$	1.000
B19	B19	03/02/2024	$y = 1.178x - 2.990$	0.999
B20	B20	02/02/2024	$y = 1.206x - 5.507$	0.997
B21	B21	03/02/2024	$y = 1.172x - 0.702$	0.999
B22	B22	02/02/2024	$y = 1.175x - 1.992$	0.996
B23	B23	02/02/2024	$y = 1.196x - 3.382$	0.998
B24	B24	01/02/2024	$y = 1.181x - 2.463$	0.999
B25	B25	01/02/2024	$y = 1.204x - 3.960$	0.997
B26	B26	01/02/2024	$y = 1.218x - 5.354$	0.998
B27	B27	03/02/2024	$y = 1.178x - 4.891$	0.997
B28	B28	02/02/2024	$y = 1.226x - 6.323$	0.999
B29	B29	05/02/2024	$y = 1.174x - 3.753$	0.997
B30	B30	03/02/2024	$y = 1.179x - 3.207$	0.998
B31	B31	03/02/2024	$y = 1.189x - 1.040$	0.997
B32	B32	01/02/2024	$y = 1.222x - 3.815$	0.999
B33	B33	01/02/2024	$y = 1.159x - 1.689$	0.996
B34	B34	01/02/2024	$y = 1.191x - 1.278$	0.995

Calibrated by :

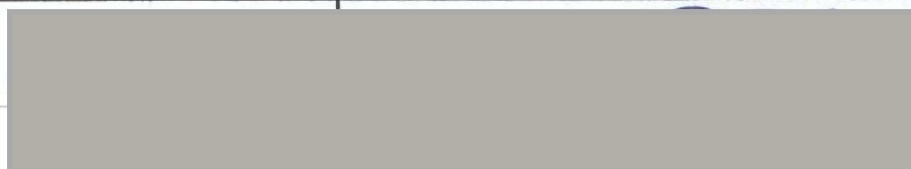





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 13 February 2024

BRAND : API

MODEL : 200E

NO. NOX-B10

SERIAL NO. 4465

#### Calibrator (Dilution System)

Brand : Teledyne

Model : 700E

Last Cal. Date : 30 October 2023

Serial No. : 201-S

#### Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : D686192

Certified Date : 20 April 2022

Expired Date : 20 April 2024

Cylinder Conc. : 49.1 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.6 °C

% RH 49

#### CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.9	-0.025	400.0	1.007
NO <sub>x</sub> Span	400	400.1	0.025	400.0	1.011

#### API Model 200E NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	505	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.1	mV	-20 - 150
AZERO	93.8	mV	-20 - 150
HVPS	674	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.1	°C	8 - 48
PMT TEMP	7.2	°C	7 ± 2
MOLY TEMP	315.3	°C	315 ± 5
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.007	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.011	-	1.0 ± 0.3
NO Offset	1.5	mV	-20 to +150
NO <sub>x</sub> Offset	0.9	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chulachak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 13 February 2024

BRAND : API

MODEL : TML-41M

NO. NOX-B20

SERIAL NO. N02782

#### Calibrator (Dilution System)

Brand : Teledyne

Model : 700E

Last Cal. Date : 30 October 2023

Serial No. : 201-S

#### Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : D636192

Certified Date : 20 April 2022

Expired Date : 20 April 2024

Cylinder Conc. : 49.1 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.6 °C

% RH 49

#### CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.6	-0.100	400.0	1.004
NO <sub>x</sub> Span	400	399.8	-0.050	400.0	1.007

#### API Model TML-41M NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	510	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	102.9	mV	-20 - 150
AZERO	93.7	mV	-20 - 150
HVPS	670	V	420 - 900 constant
RCELL TEMP	50.5	°C	50 ± 1
BOX TEMP	29.2	°C	8 - 48
PMT TEMP	7.4	°C	7 ± 2
MOLY TEMP	314.9	°C	315 ± 5
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.004	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.007	-	1.0 ± 0.3
NO Offset	1.2	mV	-20 to +150
NO <sub>x</sub> Offset	0.8	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 13 February 2024

BRAND : API

MODEL : TML-41M

NO. NOX-B21

SERIAL NO. N02374

#### Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700E
Last Cal. Date	: 30 Octobert 2023	Serial No.	: 201-S

#### Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)	Cylinder No.	: D636192
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024
		Cylinder Conc.	: 49.1 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 49

#### CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	400.1	0.025	400.0	1.009
NO <sub>x</sub> Span	400	400.2	0.050	400.0	1.013

#### API Model TML-41M NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	511	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.3	mV	-20 - 150
AZERO	94.1	mV	-20 - 150
HVPS	675	V	420 - 900 constant
RCELL TEMP	50.1	°C	50 ± 1
BOX TEMP	29.4	°C	8 - 48
PMT TEMP	7.3	°C	7 ± 2
MOLY TEMP	315.2	°C	315 ± 5
RCELL PRESS	8.5	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.7	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.009	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.013	-	1.0 ± 0.3
NO Offset	1.6	mV	-20 to +150
NO <sub>x</sub> Offset	1.0	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscn.com, www.spscn.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 13 February 2024

BRAND : API

MODEL : TML-41M

NO. NOX-B22

SERIAL NO. NO1618

#### Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700E
Last Cal. Date	: 30 Octobert 2023	Serial No.	: 201-S

#### Reference Standard Gas

Standard Gas	: Nitric Oxide (NO)	Cylinder No.	: D636192
Certified Date	: 20 April 2022	Expired Date	: 20 April 2024
		Cylinder Conc.	: 49.1 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 49

#### CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	400.2	0.050	400.0	1.010
NO <sub>x</sub> Span	400	400.3	0.075	400.0	1.015

#### API Model TML-41M NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	508	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.4	mV	-20 - 150
AZERO	94.2	mV	-20 - 150
HVPS	671	V	420 - 900 constant
RCELL TEMP	50.2	°C	50 ± 1
BOX TEMP	29.3	°C	8 - 48
PMT TEMP	7.1	°C	7 ± 2
MOLY TEMP	314.7	°C	315 ± 5
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.010	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.015	-	1.0 ± 0.3
NO Offset	1.7	mV	-20 to +150
NO <sub>x</sub> Offset	1.0	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	13 February 2024	BRAND :	API	MODEL :	100E
NO.	SO <sub>2</sub> -B05			SERIAL NO.	3270
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700E
Last Cal. Date	: 30 October 2023			Serial No.	: 201-S
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	49	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
SO <sub>2</sub> Span	400.0	400.2	0.050	400.0	1.014
API Model 100E SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.7	in-Hg	25-35		
SAMPLE FLOW	655	cc/min	650 ± 10%		
PMT	108.2	mV	-20-150 with Zero Air		
UV LAMP	3028.7	mV	1000-4900		
STR. LGT	61.9	PPB	<100		
DRK PMT	63.4	mV	-50 - 200		
DRK LMP	58.2	mV	-50 - 200		
HVPS	673	V	550-900 constant		
DCPS	2527	mV	2500 ± 200		
RCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.3	°C	5-40		
PMT TEMP	7.1	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.014	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	22.0	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sales@spscon.com www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	13 February 2024	BRAND :	API	MODEL :	100E
NO.	SO <sub>2</sub> -B07			SERIAL NO.	1706
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700E
Last Cal. Date	: 30 October 2023			Serial No.	: 201-S
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
			% RH	49	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.6	-0.100	400.0	1.008
API Model 100E SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.4	in-Hg	25-35		
SAMPLE FLOW	657	cc/min	650 ± 10%		
PMT	103.4	mV	-20-150 with Zero Air		
UV LAMP	3045.1	mV	1000-4900		
STR. LGT	61.6	PPB	<100		
DRK PMT	63.2	mV	-50 - 200		
DRK LMP	57.8	mV	-50 - 200		
HVPS	669	V	550-900 constant		
DCPS	2518	mV	2500 ± 200		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.0	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.008	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	21.9	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaituchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

## CALIBRATION REPORT

### SO<sub>2</sub> FLUORESCENT ANALYZER

DATE : 13 February 2024

BRAND : TELEDYNE

MODEL : TML-50

NO. SO<sub>2</sub>-B11

SERIAL NO. SO2187

#### Calibrator (Dilution System)

Brand	: Teledyne	Model	: 700E
Last Cal. Date	: 30 October 2023	Serial No.	: 201-S

#### Reference Standard Gas

Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )	Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029
		Cylinder Conc.	: 49.8 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 49

#### CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.8	-0.050	400.0	1.009

#### API Model TML-50 SO<sub>2</sub> Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.6	in-Hg	25-35
SAMPLE FLOW	659	cc/min	650 ± 10%
PMT	103.1	mV	-20-150 with Zero Air
UV LAMP	3018.4	mV	1000-4900
STR. LGT	61.5	PPB	<100
DRK PMT	62.9	mV	-50 - 200
DRK LMP	57.6	mV	-50 - 200
HVPS	674	V	550-900 constant
DCPS	2523	mV	2500 ± 200
RCELL TEMP	50.1	°C	50 ± 1
BOX TEMP	29.4	°C	5-40
PMT TEMP	7.5	°C	7 ± 2.0
SO <sub>2</sub> Span Conc	400	PPB	20-20,000
SO <sub>2</sub> Slope	1.009	-	1.0 ± 0.3
SO <sub>2</sub> Offset	22.2	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)

Calibrated by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chulachak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	13 February 2024	BRAND :	TELEDYNE	MODEL :	TML-50
NO.	SO <sub>2</sub> -B12	SERIAL NO.	1886		
Calibrator (Dilution System)					
Brand	: Teledyne			Model	: 700E
Last Cal. Date	: 30 October 2023			Serial No.	: 201-S
Reference Standard Gas					
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )			Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.	: 49.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C % RH 49
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
SO <sub>2</sub> Span	400.0	400.1	0.025	400.0	1.012
API Model TML-50 SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.5	in-Hg	25-35		
SAMPLE FLOW	653	cc/min	650 ± 10%		
PMT	103.3	mV	-20-150 with Zero Air		
UV LAMP	3036.2	mV	1000-4900		
STR. LGT	61.7	PPB	<100		
DRK PMT	63.1	mV	-50 - 200		
DRK LMP	58.0	mV	-50 - 200		
HVPS	671	V	550-900 constant		
DCPS	2515	mV	2500 ± 200		
RCELL TEMP	50.2	°C	50 ± 1		
BOX TEMP	29.5	°C	5-40		
PMT TEMP	7.4	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.012	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	21.8	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

Calibrated by :



CERTIFICATE No : 23M2441  
REFERENCE No : 68471-1

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905

**ID No** : BA 05/50


**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** :

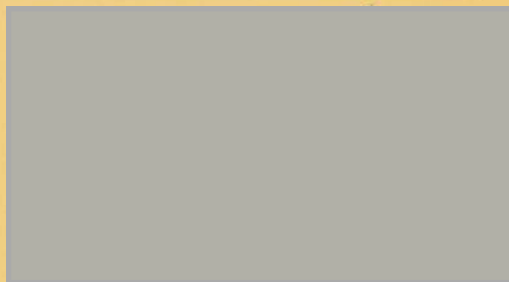

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23° C  $\pm$  1° C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA. THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

คุณภาพอากาศจากปล่องระบาย



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## Console Calibration Report

Calibration Method

Critical Orifices


### Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH <sub>g</sub> (mmH <sub>2</sub> O)
B01	1563	01/12/2023	0.998	50.05
B02	8002514	02/12/2023	1.006	49.58
B03	1503016	01/12/2023	1.003	50.16
B04	00006659	04/12/2023	0.998	49.71
B05	00007428	04/12/2023	0.999	49.24
R01	1561	02/12/2023	1.005	49.98
R02	8002513	03/12/2023	1.003	49.90
R03	1570	04/12/2023	0.996	49.68
R04	8002519	01/12/2023	1.002	49.43
R05	1503015	01/12/2023	0.997	50.24

Remark : Accept Value of y (test) is  $0.97 < y < 1.03$

Accept Value of DH<sub>g</sub> (test) is  $46.7 \pm 6.4$  (mmH<sub>2</sub>O)

Calibrated by :

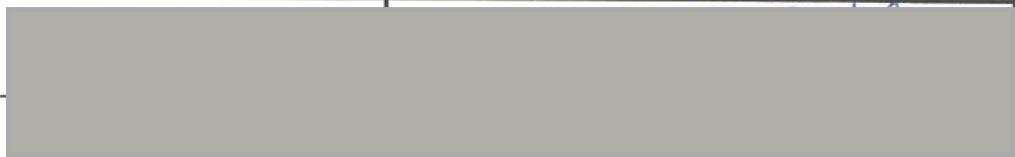





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

### Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	01/02/2024	0.84	0.83
B04	S	0.99	02/02/2024	0.85	0.84
B05	S	0.99	02/02/2024	0.84	0.84
B07	S	0.99	01/02/2024	0.84	0.85
B08	S	0.99	01/02/2024	0.83	0.84
B09	S	0.99	03/02/2024	0.84	0.85
B11	S	0.99	03/02/2024	0.84	0.84
B16	S	0.99	01/02/2024	0.83	0.84
B18	S	0.99	02/02/2024	0.84	0.84
B19	S	0.99	02/02/2024	0.84	0.83
B21	S	0.99	01/02/2024	0.84	0.85
B24	S	0.99	02/02/2024	0.85	0.84
B27	S	0.99	01/02/2024	0.84	0.84
B30	S	0.99	02/02/2024	0.84	0.83
B31	S	0.99	02/02/2024	0.84	0.85
B33	S	0.99	01/02/2024	0.84	0.84
B35	S	0.99	01/02/2024	0.85	0.84

Remark : Accept value of Cp (test) is  $0.84 \pm 0.01$

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

### Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B36	S	0.99	02/02/2024	0.84	0.83
B37	S	0.99	02/02/2024	0.84	0.84
B38	S	0.99	01/02/2024	0.84	0.84
B39	S	0.99	02/02/2024	0.85	0.84
B40	S	0.99	02/02/2024	0.84	0.83
B41	S	0.99	01/02/2024	0.84	0.85
B44	S	0.99	01/02/2024	0.85	0.84
B45	S	0.99	02/02/2024	0.83	0.84
B46	S	0.99	01/02/2024	0.84	0.85
B47	S	0.99	03/02/2024	0.84	0.84
B48	S	0.99	03/02/2024	0.84	0.85
B49	S	0.99	01/02/2024	0.83	0.84
B54	S	0.99	01/02/2024	0.84	0.85
B56	S	0.99	02/02/2024	0.84	0.84
B57	S	0.99	01/02/2024	0.83	0.84
B58	S	0.99	02/02/2024	0.84	0.85

Remark : Accept value of Cp (test) is  $0.84 \pm 0.01$

Calibrated by :



Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220088-1]  
CLID. NO. : 212301419  
JOB CONTROL NO. : 230725081570

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 25 July 2023

DATE OF ISSUED : 31 July 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
31 July 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23081570

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE	:	VACUUM GAUGE
MANUFACTURER	:	HI-LIGHT
MODEL / TYPE	:	N/A
SERIAL NO.	:	N/A[64-220088-1]
DATE OF CALIBRATION	:	26 July 2023
DUE DATE OF CALIBRATION	:	26 July 2024

---

#### ENVIRONMENT CONDITIONS :

Temperature : (  $23 \pm 2$  ) °C

Relative Humidity : (  $55 \pm 10$  ) %RH

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).

Certificate No. MP-0035-23, Due Date 02 February 2024.

#### UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2$ . It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q23081570

F3-011-04/01-12

page 2 of 3



@clccalibration



**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

## CALIBRATION DATA

### **CORRECTION OF PRESSURE**

DUC Test point ( inHg )	STD Reading ( kPa )		Conversion to inHg		Correction ( inHg )	
	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-15.07	-15.10	-4.5	-4.5	+0.5	+0.5
-10	-32.10	-32.13	-9.5	-9.5	+0.5	+0.5
-15	-49.20	-49.23	-14.5	-14.5	+0.5	+0.5
-20	-66.26	-66.26	-19.6	-19.6	+0.4	+0.4
-25	-83.30	-83.33	-24.6	-24.6	+0.4	+0.4
-30	-100.39	-100.39	-29.6	-29.6	+0.4	+0.4

Uncertainty of measurement  $\pm 0.2$  inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

**This report is valid for the above stated instrument/s only.**

**### End of Certificate ###**

Certificate No. Q23081570

F3-011-04/01-12

page 3 of 3



@clccalibration



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B01	SKC	224-PCXR4	262101	03/01/2024	1,000	1,500	2,000	993	1,497	1,998	1.002x - 4.467	1.000
B02	SKC	224-PCXR4	626166	03/01/2024	1,000	1,500	2,000	1,003	1,505	2,001	1.009x - 19.803	0.999
B03	SKC	224-PCXR4	612968	03/01/2024	1,000	1,500	2,000	996	1,494	2,001	1.006x - 12.799	1.000
B04	SKC	224-PCXR4	602804	04/01/2024	1,000	1,500	2,000	1,000	1,502	1,994	0.999x + 0.239	1.000
B05	SKC	224-PCXR4	612693	04/01/2024	1,000	1,500	2,000	1,003	1,500	2,002	1.011x - 21.266	0.999
B06	SKC	224-PCXR4	262188	05/01/2024	1,000	1,500	2,000	1,002	1,508	2,006	1.007x - 12.077	0.999
B07	SKC	224-PCXR4	626262	05/01/2024	1,000	1,500	2,000	998	1,492	1,997	0.994x + 4.810	1.000
B08	SKC	224-PCXR4	626100	04/01/2024	1,000	1,500	2,000	1,002	1,500	2,003	1.013x - 24.585	0.999
B09	SKC	224-PCXR4	626479	05/01/2024	1,000	1,500	2,000	998	1,490	1,994	0.993x + 3.837	1.000
B10	SKC	224-PCXR4	091950	04/01/2024	1,000	1,500	2,000	993	1,502	2,001	1.017x - 34.867	0.999
B11	SKC	224-PCXR8	564315	05/01/2024	1,000	1,500	2,000	996	1,492	1,999	1.004x - 7.965	1.000
B12	SKC	224-PCXR4	034656	05/01/2024	1,000	1,500	2,000	1,003	1,502	2,003	1.010x - 19.683	0.999
B13	SKC	224-PCXR4	602073	04/01/2024	1,000	1,500	2,000	997	1,500	1,998	1.000x - 0.862	1.000
B14	SKC	224-PCXR4	626313	03/01/2024	1,000	1,500	2,000	999	1,492	1,989	0.991x + 8.479	1.000
B15	SKC	224-PCXR4	626474	03/01/2024	1,000	1,500	2,000	1,002	1,502	2,005	1.012x - 21.697	0.999
B16	SKC	224-PCXR4	626477	04/01/2024	1,000	1,500	2,000	995	1,504	2,001	1.007x - 16.807	1.000
B17	SKC	224-PCXR4	626860	04/01/2024	1,000	1,500	2,000	997	1,494	1,991	0.997x + 0.331	1.000
B18	SKC	224-PCXR4	691484	05/01/2024	1,000	1,500	2,000	1,003	1,500	2,002	1.009x - 17.214	0.999
B19	SKC	224-PCXR4	691599	05/01/2024	1,000	1,500	2,000	993	1,503	1,999	1.005x - 8.906	1.000
B20	SKC	224-PCXR4	691587	05/01/2024	1,000	1,500	2,000	991	1,504	2,000	1.016x - 33.407	0.999
B21	SKC	224-PCXR4	691531	04/01/2024	1,000	1,500	2,000	993	1,499	1,995	1.001x - 5.540	1.000
B22	SKC	224-PCXR4	691654	03/01/2024	1,000	1,500	2,000	1,003	1,501	2,004	1.011x - 19.966	0.999
B23	SKC	224-PCXR4	798393	03/01/2024	1,000	1,500	2,000	993	1,507	2,002	1.017x - 33.276	0.999
B24	SKC	224-PCXR4	626363	03/01/2024	1,000	1,500	2,000	1,000	1,502	2,001	1.012x - 23.859	0.999
B25	SKC	224-PCXR4	798489	03/01/2024	1,000	1,500	2,000	1,001	1,492	2,001	0.998x + 0.694	1.000
B26	SKC	224-PCXR4	798479	04/01/2024	1,000	1,500	2,000	1,000	1,500	1,993	0.996x + 4.204	1.000
B27	SKC	224-PCXR4	691673	04/01/2024	1,000	1,500	2,000	994	1,503	2,002	1.016x - 30.902	0.999
B28	SKC	224-PCXR4	691570	05/01/2024	1,000	1,500	2,000	1,003	1,500	2,001	1.009x - 18.263	0.999
B29	SKC	224-PCXR4	626472	04/01/2024	1,000	1,500	2,000	1,002	1,498	2,000	1.002x - 3.909	1.000
B30	SKC	224-PCXR4	691489	04/01/2024	1,000	1,500	2,000	1,003	1,509	2,006	1.008x - 11.399	1.000
B31	SKC	224-PCXR4	691509	03/01/2024	1,000	1,500	2,000	993	1,496	1,997	1.005x - 11.275	1.000
B32	SKC	224-PCXR4	091567	03/01/2024	1,000	1,500	2,000	991	1,503	2,000	1.015x - 30.886	0.999
B33	SKC	224-PCXR4	091756	05/01/2024	1,000	1,500	2,000	993	1,498	1,992	0.999x - 2.317	1.000
B34	SKC	224-PCXR4	612962	05/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.007x - 13.995	1.000
B35	SKC	224-PCXR4	602682	05/01/2024	1,000	1,500	2,000	996	1,498	1,996	1.000x - 5.285	1.000
B36	SKC	224-PCXR4	626164	04/01/2024	1,000	1,500	2,000	999	1,510	1,999	1.004x - 10.131	0.999
B37	SKC	224-PCXR4	626256	05/01/2024	1,000	1,500	2,000	994	1,506	1,999	1.013x - 28.454	0.999
B38	SKC	224-PCXR4	626167	03/01/2024	1,000	1,500	2,000	997	1,498	1,998	1.003x - 5.983	1.000
B39	SKC	224-PCXR4	034637	03/01/2024	1,000	1,500	2,000	1,005	1,501	2,001	1.006x - 15.188	0.999
B40	SKC	224-PCXR4	798349	05/01/2024	1,000	1,500	2,000	994	1,505	2,000	1.014x - 29.004	0.999

Calibrated by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-B01	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	506.5	991.1	1974.3	0.989x + 9.286	1.000
H-B02	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	496.7	997.6	1996.1	0.994x + 4.509	1.000
H-B03	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	497.6	988.8	2009.6	1.004x - 14.177	0.999
H-B04	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	501.6	998.7	2006.5	0.997x - 0.777	1.000
H-B05	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	500.4	997.3	1974.3	0.980x + 21.602	0.999
H-B06	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	504.9	994.8	1984.0	1.003x - 5.213	1.000
H-B07	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	502.6	990.6	2016.7	1.001x - 0.998	1.000
H-B08	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	499.7	998.7	1979.8	0.996x + 3.580	0.999
H-B09	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	504.1	1004.3	2010.7	0.993x + 13.998	1.000
H-B10	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	496.2	999.3	2009.2	0.996x + 3.860	1.000

Calibrated by :





CERTIFICATE No : 23M2441  
REFERENCE No : 68471-1

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE  
**MANUFACTURER** : METTLER TOLEDO  
**MODEL** : XS105DU  
**SERIAL No** : 1126422905  
**ID No** : BA 05/50  
**CONDITION AS RECEIVED** : USED ITEM  
**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23° C  $\pm$  1° C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com <http://www.sithiphorn.com>

NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : SP23016

Pages : 1 of 3

## Calibration Certificate

**Equipment :** UV-VIS SPECTROPHOTOMETER  
**Manufacturer :** PERKINELMER  
**Model :** LAMBDA 25  
**Serial No.:** 501S14123010  
**ID No.:** SP03/58  
**Calibration Mode :** WAVELENGTH ACCURACY  
PHOTOMETRIC ACCURACY  
**Condition As Found :** GOOD  
**Customer :** S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,  
CHOMPHON, CHATUCHAK,  
BANGKOK 10900, THAILAND.  
**Location :** ORGANIC LABORATORY IV  
**Ambient Temperature :** ( 25.0 ± 5 ) °C  
**Relative Humidity :** ( 48.4 ± 25 ) %  
**Received Date :** 30 AUGUST 2023  
**Calibration Date :** 30 AUGUST 2023  
**Date of Issue :** 31 AUGUST 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**



This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : SP23016

Job No. : VC66SP0014

Pages : 2 of 3

**Calibration Method :**

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

**Condition of this result of calibration :**

## 1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	106864	01/11/2024
Didymium liquid	RM-DL	28912	106905	02/11/2024
Neutral density filter	RM-1N2N3N	13877	106918	03/11/2024
Potassium dichromate solutions	RM-0204060810	14204	106902	02/11/2024
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology, NIST.

**Result of calibration : Wavelength Accuracy**

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.3	0.05	0.16	2.00
	467.82	468.0	0.18	0.16	2.00
	536.56	536.6	0.04	0.16	2.00
	640.50	640.4	-0.10	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.0	0.06	0.16	2.00

UUC\* = Unit Under Calibration



Continuation of Calibration Certificate

Cert. No. : SP23016  
Job No. : VC66SP0014  
Pages : 3 of 3

**Result of calibration : Photometric Accuracy**

(Without adjustment)

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0517	1.0564	0.0047	0.0031	2.00
		29914	0.7	0.7445	0.7460	0.0015	0.0032	2.00
		29381	0.5	0.5416	0.5429	0.0013	0.0032	2.00
	546.1	29360	1.0	0.9821	0.9849	0.0028	0.0030	2.00
		29914	0.7	0.6961	0.6961	0.0000	0.0030	2.00
		29381	0.5	0.5073	0.5073	0.0000	0.0030	2.00
	590.0	29360	1.0	1.0222	1.0244	0.0022	0.0030	2.00
		29914	0.7	0.7237	0.7234	-0.0003	0.0030	2.00
		29381	0.5	0.5361	0.5360	-0.0001	0.0031	2.00
	635.0	29360	1.0	0.9753	0.9775	0.0022	0.0030	2.00
		29914	0.7	0.6910	0.6910	0.0000	0.0030	2.00
		29381	0.5	0.5211	0.5210	-0.0001	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2422	0.2462	0.0040	0.0101	2.00	
		40	0.4866	0.4900	0.0034	0.0115	2.00	
		60	0.7414	0.7390	-0.0024	0.0068	2.00	
		80	0.9858	0.9871	0.0013	0.0093	2.00	
		100	1.2442	1.2480	0.0038	0.0087	2.00	

UUC\* = Unit Under Calibration

**Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230**

Resolution of Wavelength Mode 0.1 nm  
Resolution of Photometric Mode 0.0001 A  
Parameter Setting  
Measurement Mode Wavelength, Absorbance  
Wavelength Scan 1100 nm-190 nm  
Scanning Speed 7.5 nm/min  
Data Pitch 0.1 nm  
Band width(Wavelength) 1.0 nm  
Band width(Vis) 1.0 nm  
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transimission T(%)	Absorbance(A)
0.0111	3.9564

\*\*Specific Acceptance :

Transmission  $\leq$  1.0 T(%), Absorbance  $\geq$  2.0 A

\*\*Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95%

**End of Calibration Certificate**

Certificate Of Analysis  
Special Gases Mixture

## Customer Details

Name: S.P.S Consulting Service Address: House No. 7, Soi Phahon Yothin 24, Phahon Yotin Rd., Chatujak, Bangkok 10900 Customer Tag No.:

## Certificate Details

Number:	3991/22	Date of Issue:	6-Jan-2023	Expiry date:	6-Jan-2026
Material Details					
Production Order:	90175195	Material Code:	553600-SV-44	Cylinder No.:	D869074
Gas content:	1.25 M <sup>3</sup>	Filling pressure:	130.0 bar	Valve:	CGA 660 SS
Cylinder Owner:	LINDE	Cylinder Material:	Spectra seal	Cylinder Size:	10 L

## Laboratory Report

## Analytical Result

Component	Normal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>	Assay Date
Nitric Oxide	100 ppm	101 ppm	± 1% relative	(6) I-PB-352	23-Dec-22 & 6-Jan-23
Other NOx impurity In Nitrogen		Less than 5.0 ppm			

## Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Nitric Oxide In Nitrogen	QA2565	99.4 ± 0.7 ppm	4-Feb-2023

## Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-NO	28-Nov & 28-Dec-22

## Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.  
Storage condition: Keep in well ventilation and secure area.

## Comments

When reordering, please quote the material number

## Note:

- All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/S31 for the Assay and Certification of Gaseous Calibration Standards using procedure G1
- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
- (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasoontorn

Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Page 1 of 1

This report shall not be reproduced except in full  
บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

เลขที่ใบรับเอกสารนี้ 0107537000785

ชั้น 15 อาคารทาวเวอร์ เอ 2/3 หมู่ 14 ถนนพหลโยธิน-ตราด กม. 6.5 แขวงคลอง

อ.บางพลี จ.สมุทรปราการ 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333

โรงงานเวลโกรว์: 105 หมู่ 5 ต.บางพลี อ.บางพลี จ.สมุทรปราการ 24180

โทรศัพท์ (66) 38.570-479-93

โทรสาร (66) 38.570-323

Linde (Thailand) Public Company Limited

PLC Registration no. 0107537000785

15<sup>th</sup> Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trid KM. 6.5 Road, Bangkaew

Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93

Fax (66) 38.570-323

PB-002/F006

Iss:K/2, 15 Oct 2021



Certificate Of Analysis  
Special Gases Mixture

## Customer Details

Name:

S.P.S Consulting Service

Address:

7 Soi Phahon Yothin 24,  
Khet Chatuchak, Bangkok 10900

Customer Tag No.:

## Certificate Details

Number:	1138/22	Date of Issue:	19-Apr-2022	Expiry date:	19-Apr-2024
Material Details					
Production Order:	90170869	Material Code:	411800-AL-44	Cylinder No.:	D824400
Gas content:	6.90 M <sup>3</sup>	Filling pressure:	145.0 bar	Valve:	CGA 660 SS
Cylinder Owner:	LINDE	Cylinder Material:	Aluminum	Cylinder Size:	50 L

## Laboratory Report

## Analytical Result

Component	Normal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>	Assay Date
Nitric Oxide	200 ppm	201 ppm	± 1% relative	(6) I-PB-352	7-Apr & 19-Apr-22
Other NOx impurity In Nitrogen		Less than 10.0 ppm			

## Reference Standard

Nitric Oxide  
In Nitrogen

## Reference Standard used in Assay

Cylinder number

QA2565

Concentration

99.4 ± 0.7 ppm

Expiry date:

4-Feb-2023

Instrument/Make/Model  
FTIR Spectrometers Nicolet i550

## Analytical Instruments used in Assay

Analytical Principle  
FTIR-NOLast Multipoint Calibration  
9-Mar & 8-Apr-22

## Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.

Storage condition: Keep in well ventilation and secure area.

## Comments

When reordering, please quote the material number

## Note:

1. All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1
2. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
3. (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasoontorn

Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Page 1 of 1

This report shall not be reproduced except in full

บริษัท ลินเด (ประเทศไทย) จำกัด (มหาชน)

เลขที่ใบรับรองมาตรฐาน 0107537000755

ชั้น 15 ถนนพหลโยธิน กม. 2/3 หมู่ 14 ถนนพหลโยธิน-ตราด กม. 6.5 ต.บางพลี

อ.บางพลี จ.สมุทรปราการ 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333

โรงงานเวลโกรว์: 105 หมู่ 5 ต.บางพลี อ.บางพลี จ.สมุทรปราการ 24180

โทรศัพท์ (66) 38.570-479-93

โทรสาร (66) 38.570-323

Linde (Thailand) Public Company Limited

P.L.C. Registration No. 0137537000755

15<sup>th</sup> Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trd Km. 6.5 Road, Bangkaew

Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant : 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93

Fax (66) 38.570-323

PB-002/F006

Iss:K/2, 15 Oct 2021

Certificate Of Analysis  
Special Gases Mixture

## Customer Details

Name:

S.P.S Consulting Service

Address:

7 Soi Phahon Yothin 24, Phahon Yotin Rd.,  
Chatujak, A. Chatuchak Bangkok 10900

Customer Tag No.:

## Certificate Details

Number:	2574/21	Date of Issue:	21-Jun-2021	Expiry date:	21-Jun-2029
Material Details					
Production Order:	90166199	Material Code:	627400-SK-44	Cylinder No.:	A007105K
Gas content:	5.52 M <sup>3</sup>	Filling pressure:	145.0 bar	Valve:	CGA 660 SS
Cylinder Owner:	LINDE	Cylinder Material:	Spectra seal	Cylinder Size:	40 L

## Laboratory Report

## Analytical Result

Component	Nominal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>	Assay Date
Sulphur Dioxide In Nitrogen	50.0 ppm	50.2 ppm	± 1% relative	(6) I-PB-352	12-Jun & 19-Jun-21

## Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Sulphur Dioxide In Nitrogen	133188SG	50.50 ± 0.40 ppm	16-Oct-2021

## Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-SO2	7-Jun-2021

## Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.

Storage condition: Keep in well ventilation and secure area.

## Comments

When reordering, please quote the material number

## Note:

- All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1
- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
- (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasoonorn

Signatory for and on behalf of Linde (Thailand) CO., Ltd.

PB-001/F006

Page 1 of 1

This report shall not be reproduced except in full

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

Linde (Thailand) Public Company Limited

15 อาคารทาวเวอร์เอ 2/3 หมู่ 14 ถนนพหลโยธิน-ลาดพร้าว แขวง 6-5 แขวงลาดพร้าว

เขตคลองสามวา กรุงเทพมหานคร 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333

โรงงานเวลโกรว์ 105 หมู่ 5 ตำบลลำโพง อำเภอลำโพง จังหวัดตราด 24130

โทรศัพท์ (66) 33-570-479-93

โทรสาร (66) 33-571-323

Linde (Thailand) Public Company Limited (SSJ) 21-Apr-2021

Reg. No. 019733710705

15<sup>th</sup> Floor, Bangna Tower A, 2/3 Moo 14, Bangna Freeway KM 3.5 Road, Bangnae

Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant 105 Moo 5, Tambon Lampong, Amphoe Lampong, Trat 24130

Thailand, Tel (66) 33-570-479-93

Fax (66) 33-570-323



Certificate Of Analysis  
Special Gases Mixture

## Customer Details

Name: S.P.S Consulting Service Address: 7, Soi Phahon Yothin 24, Phahon Yothin Rd., Chatujak, Bangkok, 10900 Customer Tag No.:

## Certificate Details

Number: 2420/19 Date of Issue: 25-Jul-2019 Expiry date: 24-Jul-2027  
Material Details  
Production Order: 90154858 Material Code: 636400-SK-44 Cylinder No.: A00797SK  
Gas content: 5.520 M<sup>3</sup> Filling pressure: 145.0 bar Valve: CGA 660 SS  
Cylinder Owner: LINDE Cylinder Material: Spectra seal Cylinder Size: 40 L

## Laboratory Report

## Analytical Result

Component	Nominal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>	Assay Date
Sulphur Dioxide In Nitrogen	100 ppm	102 ppm	± 1% relative	(6) I-PB-352	17-Jul & 24-Jul-19

## Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date
Sulphur Dioxide In Nitrogen	258005SG	103.1 ± 0.8 ppm	9-Aug-2020

## Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-SO2	24-Jun-2019

## Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.  
Storage condition: Keep in well ventilation and secure area.

## Comments

When reordering, please quote the material number

## Note:

- All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/331 for the Assay and Certification of Gaseous Calibration Standards using procedure G1.
- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
- (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasoonorn  
Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Page 1 of 1

This report shall not be reproduced except in full

PB-002 F006

Issue 2 of March 2019

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

เลขที่หนังสือแจ้ง: 017982000788

วันที่ 15 มิถุนายน 2563 (หรือ 2, 3 หรือ 14 มิถุนายน 2563) ณ กรุงเทพมหานคร

สำนักงานใหญ่/กรุงเทพฯ 10540 โทรศัพท์ (66) 2333-6100 โทรสาร (66) 2333-5333

โรงงานปทุมธานี 105 หมู่ 5 ต.บึงสามพัน อ.บึงสามพัน จ.ปทุมธานี 24180

โทรศัพท์ (66) 38.570-479-93

โทรสาร (66) 38.570-323

Linde (Thailand) Public Company Limited

15<sup>th</sup> Floor, Bangna Tower A, 2/3 Moo 14, Bangna-Traffic Jct. 45 Road, Bangnae

Bangplee, Samutprakarn 10540, Tel. (66) 2333-6100 Fax (66) 2333-5333

Wellgrow Plants 105 Moo 5, T. Bangsamak, A. Bangsakong, Chachoengsao 24180

Thailand, Tel. (66) 38.570-479-93

Fax (66) 38.570-323



Certificate Of Analysis  
Special Gases Mixture

## Customer Details

Name:

S.P.S Consulting Service

Address:

7 Soi Phahon Yothin 24, Phahon Yotin Rd.,  
Khet Chatuchak Bangkok 10900

Customer Tag No.:

## Certificate Details

Number:	2256/20	Date of Issue:	22-May-2020	Expiry date:	21-May-2028
Material Details					
Production Order:	90160385	Material Code:	590800-J-44	Cylinder No.:	5858
Gas content:	6.56 M <sup>3</sup>	Filling pressure:	145.0 bar	Valve:	CGA 590 BRASS
Cylinder Owner:	LINDE	Cylinder Material:	STEEL	Cylinder Size:	47 L

## Laboratory Report

## Analytical Result

Component	Nominal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>	Assay Date
Oxygen In Nitrogen	15.0%	14.9%	± 1% relative	(6) I-PB-352	22-May-2020

## Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Oxygen In Nitrogen	53281	9.98 ± 0.05%	13-Sep-2021

## Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Servomex 4100 O2 analyser	Paramagnetic	21-May-2020

## Recommend usage condition

Minimum utilization: 5% of actual content or before expiry date whichever comes first.  
Storage condition: Keep in well ventilation and secure area.

## Comments

When reordering, please quote the material number

## Note:

1. All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1  
2. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.  
3. (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasoonorn

Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Page 1 of 1

This report shall not be reproduced except in full

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

เลขที่ใบเสร็จรับเงิน 0107537000785

ชั้น 15 อาคารทาวเวอร์ เอ 2/3 หมู่ 14 ถนนบางนา-ตราด กม. 6.5 แขวงบางนา

อ.บางพลี อ.สมุทรปราการ 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333

โรงงานเวลโกรว์: 105 หมู่ 5 ต.บางพลี อ.บางพลี จ.สมุทรปราการ 24180

โทรศัพท์ (66) 38.570-479-93

โทรสาร (66) 38.570-323

Linde (Thailand) Public Company Limited

P.L.C. Registration no. 0107537000785

15<sup>th</sup> Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangkaew

Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333

Wellgrow Plant: 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93

Fax (66) 38.570-323

PB-002/F006

Iss: 1/1, 01 October 2019



บริษัท ยูไนเต็ดอินดัสเทรียลแก๊ส จำกัด (สำนักงานใหญ่)  
聯育股份有限公司  
UNITED INDUSTRIAL GASES CO., LTD. (Head Office)

29/3 หมู่ที่ 5 ถนนบางนา-ตราด ตำบลบางเสาธง อำเภอบางเสาธง จังหวัดสมุทรปราการ 10570

29/3 MOO 5 BANGNA-TRAD ROAD, TAMBOL BANGSAOTONG, AMPHUR BANGSAOTONG, SAMUTPRAKARN 10570

TEL.: 0-2338-1460-1, 0-2708-4148-9 FAX.: 0-2338-1548, 0-2708-3873 E-mail: uiggases@truemail.co.th, uiggases@gmail.com Web: http://www.uiggases.com

เลขประจำตัวผู้เสียภาษี : 0115528000610

## Certificate of Analysis

Page : 1/1

Certificate No.: QA24030256

**Client Name :** บริษัท เอส.พี.เอส. คอนสตรัคชั่น เซอร์วิส จำกัด  
**Address :** 7 ซอยพลโยธิน 24 ถนนพลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
**Telephone :** 0-2939-4370 **Fax :** 0-2513-4221  
**Contact Name :** - **Contact Email :** -

### Sample Description

**Sample Name :** Nitrogen 99.999% Ultra High Purity Grade **Shelf Life :** 3 Years  
**Sampling Condition :** Cylinder 7 M3 Pressure 2000 psig **Valve Type :** CGA 580  
**Lot No. :** - **Test Date :** 26/02/2023

รายการทดสอบ (Test Item)	วิธีทดสอบ (Test Method)	หน่วย (Unit)	เกณฑ์กำหนด (Specification)	ผลการทดสอบ (Results)
1. Moisture (H <sub>2</sub> O)	LT-UIG-01 (Shaw Moisture Meter)	ppm	≤ 3.0	< 3.0
2. Oxygen (O <sub>2</sub> )	LT-UIG-03 (Oxygen Analyzer)	ppm	≤ 3.0	< 3.0
3. Carbon Monoxide (CO)	In-house method : LT-UIG-05 ( Gas Chromatography )	ppm	≤ 1.0	< 1.0
4. Carbon Dioxide (CO <sub>2</sub> )	In-house method : LT-UIG-05 ( Gas Chromatography )	ppm	≤ 1.0	< 1.0
5. THC as CH <sub>4</sub>	In-house method : LT-UIG-06 ( Gas Chromatography )	ppm	≤ 1.0	< 1.0

Note : CYLINDER No. : NI0307-0060



Approved By :

( Miss.Nithinan Srirakham )  
Quality Control

Date : 26 / 02 / 2023



ระดับเสียงในบรรยากาศ

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

## CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.  
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.  
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.  
4. Digital Multimeter Agilent 34401A S/N MY44005560.  
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.  
6. Audio Analyzer Keithley 2015-P S/N 4106495.  
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 27 Mar. 2023

Date of Calibration : 29 Mar. 2023

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.94	-0.06	$\pm 0.10$	$\pm 0.40$ dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	$\pm 1.5$	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	$\pm 0.50$	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

(Mr. Weerachai Deechaiyae)

Approved by :

(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 29 Mar. 2023

Date of Issue : 30 Mar. 2023

Ref : 2011266032701228001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Noise B\_033/24

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	29 March 2023
		Due Date	29 March 2024

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B34	ACO	6236	00192025	13 February 2024	94.1	94.0
ACO-B37	ACO	6236	00192028	13 February 2024	94.0	94.0
ACO-B38	ACO	6236	00192029	13 February 2024	94.0	94.0
ACO-B43	ACO	6236	00192034	13 February 2024	93.9	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.94 ± 0.10 dB	

Calibrated by :

(Mr. Anut Dangkom)

(Mr. Peera Detudom)



คุณภาพน้ำ



# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



NSC-TISI-TIS17025  
CALIBRATION 0049

CERTIFICATE No : 23E8494

REFERENCE No : 70413-1

PAGE : 1 OF 3

## Certificate of Calibration

**EQUIPMENT** : pH METER

**MANUFACTURER** : HANNA

**MODEL** : HI 3512

**SERIAL No** : TH118035

**ID No** : pH04/56

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 06-Sep-23

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 06-Sep-23

**RECEIVED DATE** : 31-Aug-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 2 OF 3

## Calibration Report

EQUIPMENT : pH METER  
MANUFACTURER : HANNA  
ID No : pH04/56  
RECEIVED DATE : 31-Aug-23  
AMBIENT TEMPERATURE : 23 ° C ± 3 ° C  
MODEL : HI 3512  
SERIAL NUMBER : TH118035  
CALIBRATION DATE : 06-Sep-23  
RELATIVE HUMIDITY : 50 % RH ± 10% RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/ LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	23E1312	19-Apr-24
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION : ADJUSTMENT

#### 1. DISPLAY UNIT ONLY

SLOPE FACTOR  $k = 2.303 RT/F = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.6	-0.49	-0.290	0.15	2.00
354.95	355.4	-0.45	0.741	0.15	2.00
295.80	296.3	-0.50	1.773	0.15	2.00
236.64	237.1	-0.46	2.804	0.15	2.00
177.48	177.9	-0.42	3.835	0.15	2.00
118.32	118.7	-0.38	4.867	0.15	2.00
59.16	59.6	-0.44	5.898	0.15	2.00
0.00	0.4	-0.40	6.930	0.15	2.00
-59.16	-58.8	-0.36	7.961	0.15	2.00
-118.32	-117.9	-0.42	8.992	0.15	2.00
-177.48	-177.1	-0.38	10.024	0.15	2.00
-236.64	-236.3	-0.34	11.055	0.15	2.00
-295.80	-295.5	-0.30	12.087	0.15	2.00
-354.95	-354.6	-0.35	13.118	0.15	2.00
-414.11	-413.8	-0.31	14.149	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 3 OF 3

## Calibration Report

### RESULT OF CALIBRATION (CONTINUE) :

#### 2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ pH)	COVERAGE FACTOR k
4.006	4.006	0.000	4.015	0.012	2.00
7.000	7.000	0.000	6.914	0.012	2.00
10.008	10.010	-0.002	9.996	0.014	2.00

#### 3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ( $^{\circ}$ C)	UUC READING ( $^{\circ}$ C)	CORRECTION ( $^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ $^{\circ}$ C)	COVERAGE FACTOR k
25.005	25.0	0.005	---	0.0085	2.00

#### 4. PERCENT SLOPE 100%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : CONDUCTIVITY METER  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : SEVEN COMPACT S230  
SERIAL NO. : C141708983/5821320179  
CLID. NO. : 272300452  
JOB CONTROL NO. : 230211016445

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 11 February 2023

DATE OF ISSUED : 15 February 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
15 February 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23016445

F3-011-04/01-12

page 1 of 4



@clccalibration



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : CONDUCTIVITY METER  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : SEVEN COMPACT S230  
SERIAL NO. : C141708983/5821320179  
DATE OF CALIBRATION : 13 February 2023

#### ENVIRONMENT CONDITIONS :

Temperature :  $(25 \pm 2.5) ^\circ\text{C}$  Relative Humidity :  $(50 \pm 15) \% \text{ RH}$

#### PROCEDURE USED :

This instrument [ Conductivity Meter ] was calibrated under procedure No. **WI-305-130**. The calibration was performed by direct measurement with Certified Reference Material (CRM) and Reference Material (RM) .

This instrument [ Temperature ] was calibrated under procedure No. **WI-305-244**. The calibration was performed by Comparison with Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

1. Potassium Chloride Solution ( nominal 1.41 mS/cm , nominal 12.8 mS/cm )
2. Conductivity Solution , Hanna Product Code HI 7033L Lot Number 6436.
3. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
4. Precision Thermometer, ASL Model F250 S/N. 1334023800.
5. IPRT, ASL Model T100-250-1D S/N. L0193A-1-1.



## TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Merck Co., Ltd.

Certificate No. HC02139203 , HC04515254. Due Date 30 June 2023 , 30 November 2023.

2. The measurements are traceable to International System of Units (SI) , through Hanna instruments.

Certificate No. 12E12 , Due Date May 2024 .

3. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.

Certificate No. Q22130792, Due Date 05 January 2024.

4. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0823/65, Due Date 22 August 2023.

5. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).

Certificate No. TT-0166-22, Due Date 01 December 2023.

## UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"



## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Conductivity Meter.

### CALIBRATION DATA

#### 1. Conductivity Solution Test @ 25°C

Standard Conductivity Solution	DUC Reading	Uncertainty of Measurement	k Factor
*84.00 µS/cm	84.04 µS/cm [Cell Constant 0.548589]	± 1.00 µS/cm	2,00
1412.0 µS/cm	1413 µS/cm [Cell Constant 0.548589]	± 21.0 µS/cm	2,00
12.85 mS/cm	12.88 mS/cm [Cell Constant 0.573538]	± 0.19 mS/cm	2,00

Note. \* means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 01 Page 138 of 138

#### \*2. Temperature Result [ Probe Conductivity ]

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.00	25.0	0.00	0.07

Note. The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2,00$ .

\* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###





## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : CONDUCTIVITY METER  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : SEVEN COMPACT S230  
SERIAL NO. : C141708983/5821320179  
CLID. NO. : 272300452  
JOB CONTROL NO. : 240213016389  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 13 February 2024

DATE OF ISSUED : 16 February 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By :

Sukgasem Seehanart  
Calibration Engineer

Approved By :

Mongkol Yotsoontorn  
Authorized Signatory  
16 February 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units ( SI )

Certificate No. Q24016389

F3-011-05/12-23

page 1 of 4



@clccalibration

## REPORT OF CALIBRATION FOR

NOMENCLATURE : CONDUCTIVITY METER  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : SEVEN COMPACT S230  
SERIAL NO. : C141708983/5821320179  
DATE OF CALIBRATION : 13 February 2024

### ENVIRONMENT CONDITIONS :

Temperature :  $(25 \pm 2.5) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \% \text{ RH}$

### PROCEDURE USED :

This instrument [ Conductivity Meter ] was calibrated under procedure No. **WI-305-130**. The calibration was performed by direct measurement with Certified Reference Material (CRM) and Reference Material (RM) .

This instrument [ Temperature ] was calibrated under procedure No. **WI-305-244**. The calibration was performed by Comparison with Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

### REFERENCE STANDARD USED :

1. Conductivity Solution , Hanna Product Code HI 7033L Lot Number 7830.
2. Potassium Chloride Solution ( nominal 1.41 mS/cm )
3. Potassium Chloride Solution ( nominal 12.8 mS/cm )
4. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
5. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03.
6. IPRT, ASL Model T100-250-1D S/N. L0193A-1-1.



## TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Hanna instruments.  
Certificate No. 20F21 , Due Date June 2025 .
2. The measurements are traceable to International System of Units (SI) , through Sigma-Aldrich Canada Co.  
Certificate No. HC30595403 , Due Date 31 January 2026 .
3. The measurements are traceable to International System of Units (SI) , through Sigma-Aldrich Canada Co.  
Certificate No. HC20111554 , Due Date 30 September 2025.
4. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.  
Certificate No. Q23136342, Due Date 20 December 2024.
5. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0203/67, Due Date 07 December 2024.
6. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).  
Certificate No. TT-0136-23, Due Date 12 December 2024.

## UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"





**CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The table in the following gives the calibration results and associated measurement uncertainties of Conductivity Meter.

## CALIBRATION DATA

### 1. Conductivity Solution Test @ 25°C

Standard Conductivity Solution	DUC Reading	Uncertainty of Measurement
*84.00 µS/cm	84.05 µS/cm [Cell Constant 0.548589]	± 1.00 µS/cm
1414.0 µS/cm	1415 µS/cm [Cell Constant 0.548589]	± 21.0 µS/cm
12.83 mS/cm	12.75 mS/cm [Cell Constant 0.548589]	± 0.19 mS/cm

Note. \* means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 91 of 138

### \*2. Temperature Result [ Probe Conductivity ]

Immersion depth (mm)	Actual Temperature ( °C )	DUC Reading ( °C )	Correction ( °C )	Uncertainty ± ( °C )
100	25.00	24.9	+0.10	0.07

Note. \* means Calibrations marked " Not TISI Accredited " in this Certificate have been included for completeness.

**This report is valid for the above stated instrument/s only.**

**### End of Certificate ###**

Certificate No. Q24016389

F3-011-05/12-23

page 4 of 4



@clccalibration



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484

Cert.No.: 23CH432

Page.: 1 of 2

## Certificate of Calibration

**Equipment :** Turbidity Meter  
**Manufacturer :** Eutech  
**Model :** Cyberscan WL TB1000  
**Serial No. :** 201802206  
**ID. No. :** TB 03/61  
**Condition As-Received:** Used Item  
**Received Date :** 29 March 2023  
**Calibration Date :** 30 March 2023  
**Reference :** 2303-1034WN-1  
**Submitted by :** S.P.S. Consulting Service Co.,Ltd.  
7 Phaholyothin 24, Phaholyothin Road.,  
Jompol, Chatuchak, Bangkok 10900  
**Ambient Temperature :** (25 ± 2.5) °C  
**Relative Humidity :** (50 ± 20) %  
**Calibration Procedure :** In - house method : CP-CH11  
based on direct measurement by  
using Formazin standard solution

**Calibrated by :** Walalak Sirithean

**Approved by :**

( / ) Malee Butkruea  
( ) Saithip Meangmai  
( ) Warakorn Lerngagtrakul

**Issue Date :** 31 March 2023

**The Uncertainties are for a confidence probability of approximately 95%.**

This certificate may not be reproduced other than in full, except with the prior written  
approval of the head of Calibration and Testing Equipment Services.

A 0010867



Cert.No. : 23CH432

Page. : 2 of 2

**Condition of this calibration result**

## 1. Reference Standard Instruments :

This certification is traceable to the International System of unit (SI unit) through Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermo-Hygrograph	1103328	130EC010	22H1313	12 June 2023
2) Electronic Balance	N03679	140RC001	22MM49	20 Sep 2023

## 2. Standard Material : The Formazin suspension has been prepared gravimetric from

<u>Material</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Assay</u>
1) Hexamethylenetetramine	HIMEDIA	0000493947	99.65%
2) Hydrazinium Sulfate	HIMEDIA	0000522014	99.40%

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration result**

Performing three - Formazin suspension standard curve by using 0,10,1000 NTU  
Turbidity Meter Serial Number : 201802206

Standard Formazine suspension ( NTU )	UUC* Reading ( NTU )	Uncertainty of Measurement ( $\pm$ NTU )	Coverage Factor <i>k</i>
20	19.3	0.38	2.00
40	39.0	0.40	2.00
100	99.2	0.70	2.00
400	391	1.5	2.00

**Remark**

- UUC\* = Unit Under Calibration
- NTU = Nephelometric Turbidity Units

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484

## Certificate of Calibration

Cert.No.: 24CH285

Page.: 1 of 2

**Equipment :** Turbidity Meter  
**Manufacturer :** Eutech  
**Model :** CyberScan WLTB1000  
**Serial No. :** 201802206  
**ID. No. :** TB 03/61  
**Condition As-Received:** Used Item  
**Received Date :** 05 March 2024  
**Calibration Date :** 06 March 2024  
**Reference :** 2403-0144WN-1  
**Submitted by :** S.P.S. Consulting Service Co.,Ltd.  
7 Phaholyothin 24, Phaholyothin Road.,  
Jompol, Chatuchak, Bangkok 10900  
  
**Ambient Temperature :** (25 ± 2.5) °C  
**Relative Humidity :** (50 ± 20) %  
**Calibration Procedure :** In - house method : CP-CH11  
based on direct measurement by  
using Formazin standard solution

**Calibrated by :** Walalak Sirithean

**Approved by :**

Approved Signatory

( ) Pornthippa Tameyakul

( ) Unnopphol Harachai

(✓) Saithip Meangmai

**Issue Date :** 06 March 2024

**The Uncertainties are for a confidence probability of approximately 95%.**

This certificate may not be reproduced other than in full, except with the prior written  
approval of the head of Calibration and Testing Equipment Services.

A 0013024



Cert.No. : 24CH285

Page. : 2 of 2

### Condition of this calibration result

#### 1. Reference Standard Instruments :

This certification is traceable to the International System of unit (SI unit) through:-  
- Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermo-Hygograph	1103328	130EC010	23H1361	13 June 2024
2) Electronic Balance	14233821	110RC001	23MM405	16 July 2024

#### 2. Standard Material : The Formazin suspension has been prepared gravimetric from

<u>Material</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Assay</u>
1) Hexamethylenetetramine	HIMEDIA	0000493947	99.65%
2) Hydrazinium Sulfate	HIMEDIA	0000522014	99.40%

#### 3. This certificate is valid only to the item calibrated on date and place of calibration.

### Calibration result

Performing three - Formazin suspension standard curve by using 0,10,1000 NTU

Turbidity Meter Serial Number : 201802206

Standard Formazine suspension ( NTU )	UUC* Reading ( NTU )	Uncertainty of Measurement ( $\pm$ NTU )	Coverage Factor <i>k</i>
20	19.2	0.38	2.00
40	39.4	0.40	2.00
100	99.0	0.70	2.00
400	389	1.5	2.00

**Remark** - UUC\* = Unit Under Calibration  
- NTU = Nephelometric Turbidity Units

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : SP23016

Pages : 1 of 3

## Calibration Certificate

**Equipment :** UV-VIS SPECTROPHOTOMETER  
**Manufacturer :** PERKINELMER  
**Model :** LAMBDA 25  
**Serial No.:** 501S14123010  
**ID No.:** SP03/58  
**Calibration Mode :** WAVELENGTH ACCURACY  
PHOTOMETRIC ACCURACY  
**Condition As Found :** GOOD  
**Customer :** S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,  
CHOMPHON, CHATUCHAK,  
BANGKOK 10900, THAILAND.  
**Location :** ORGANIC LABORATORY IV  
**Ambient Temperature :** ( 25.0 ± 5 ) °C  
**Relative Humidity :** ( 48.4 ± 25 ) %  
**Received Date :** 30 AUGUST 2023  
**Calibration Date :** 30 AUGUST 2023  
**Date of Issue :** 31 AUGUST 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : SP23016

Job No. : VC66SP0014

Pages : 2 of 3

**Calibration Method :**

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01, ASTM E925-02

**Condition of this result of calibration :**

## 1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	106864	01/11/2024
Didymium liquid	RM-DL	28912	106905	02/11/2024
Neutral density filter	RM-1N2N3N	13877	106918	03/11/2024
Potassium dichromate solutions	RM-0204060810	14204	106902	02/11/2024
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology, NIST.

**Result of calibration : Wavelength Accuracy**

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.3	0.05	0.16	2.00
	467.82	468.0	0.18	0.16	2.00
	536.56	536.6	0.04	0.16	2.00
	640.50	640.4	-0.10	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.0	0.06	0.16	2.00

UUC\* = Unit Under Calibration

Continuation of Calibration Certificate

Cert. No. : SP23016  
Job No. : VC66SP0014  
Pages : 3 of 3

**Result of calibration : Photometric Accuracy**

(Without adjustment)

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0517	1.0564	0.0047	0.0031	2.00
		29914	0.7	0.7445	0.7460	0.0015	0.0032	2.00
		29381	0.5	0.5416	0.5429	0.0013	0.0032	2.00
	546.1	29360	1.0	0.9821	0.9849	0.0028	0.0030	2.00
		29914	0.7	0.6961	0.6961	0.0000	0.0030	2.00
		29381	0.5	0.5073	0.5073	0.0000	0.0030	2.00
	590.0	29360	1.0	1.0222	1.0244	0.0022	0.0030	2.00
		29914	0.7	0.7237	0.7234	-0.0003	0.0030	2.00
		29381	0.5	0.5361	0.5360	-0.0001	0.0031	2.00
	635.0	29360	1.0	0.9753	0.9775	0.0022	0.0030	2.00
		29914	0.7	0.6910	0.6910	0.0000	0.0030	2.00
		29381	0.5	0.5211	0.5210	-0.0001	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2422	0.2462	0.0040	0.0101	2.00	
		40	0.4866	0.4900	0.0034	0.0115	2.00	
		60	0.7414	0.7390	-0.0024	0.0068	2.00	
		80	0.9858	0.9871	0.0013	0.0093	2.00	
		100	1.2442	1.2480	0.0038	0.0087	2.00	

UUC\* = Unit Under Calibration

**Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230**

Resolution of Wavelength Mode 0.1 nm  
Resolution of Photometric Mode 0.0001 A  
Parameter Setting  
Measurement Mode Wavelength, Absorbance  
Wavelength Scan 1100 nm-190 nm  
Scanning Speed 7.5 nm/min  
Data Pitch 0.1 nm  
Band width(Wavelength) 1.0 nm  
Band width(Vis) 1.0 nm  
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transimission T(%)	Absorbance(A)
0.0111	3.9564

\*\*Specific Acceptance :

Transmission  $\leq$  1.0 T(%), Absorbance  $\geq$  2.0 A

\*\*Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95%

**End of Calibration Certificate**





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



NSC-TISI-TIS17025  
CALIBRATION 0049

CERTIFICATE No : 23E8494

REFERENCE No : 70413-1

PAGE : 1 OF 3

## Certificate of Calibration

**EQUIPMENT** : pH METER

**MANUFACTURER** : HANNA

**MODEL** : HI 3512

**SERIAL No** : TH118035

**ID No** : pH04/56

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 06-Sep-23

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 06-Sep-23

**RECEIVED DATE** : 31-Aug-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 2 OF 3

## Calibration Report

EQUIPMENT : pH METER  
MANUFACTURER : HANNA  
ID No : pH04/56  
RECEIVED DATE : 31-Aug-23  
AMBIENT TEMPERATURE : 23 ° C ± 3 ° C  
MODEL : HI 3512  
SERIAL NUMBER : TH118035  
CALIBRATION DATE : 06-Sep-23  
RELATIVE HUMIDITY : 50 % RH ± 10% RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/</u> <u>LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	23E1312	19-Apr-24
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

### RESULT OF CALIBRATION : ADJUSTMENT

#### 1. DISPLAY UNIT ONLY

SLOPE FACTOR  $k = 2.303 RT/F = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.6	-0.49	-0.290	0.15	2.00
354.95	355.4	-0.45	0.741	0.15	2.00
295.80	296.3	-0.50	1.773	0.15	2.00
236.64	237.1	-0.46	2.804	0.15	2.00
177.48	177.9	-0.42	3.835	0.15	2.00
118.32	118.7	-0.38	4.867	0.15	2.00
59.16	59.6	-0.44	5.898	0.15	2.00
0.00	0.4	-0.40	6.930	0.15	2.00
-59.16	-58.8	-0.36	7.961	0.15	2.00
-118.32	-117.9	-0.42	8.992	0.15	2.00
-177.48	-177.1	-0.38	10.024	0.15	2.00
-236.64	-236.3	-0.34	11.055	0.15	2.00
-295.80	-295.5	-0.30	12.087	0.15	2.00
-354.95	-354.6	-0.35	13.118	0.15	2.00
-414.11	-413.8	-0.31	14.149	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 3 OF 3

**Calibration Report****RESULT OF CALIBRATION (CONTINUE) :****2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ pH)	COVERAGE FACTOR k
4.006	4.006	0.000	4.015	0.012	2.00
7.000	7.000	0.000	6.914	0.012	2.00
10.008	10.010	-0.002	9.996	0.014	2.00

**3. DISPLAY UNIT WITH TEMPERATURE**

STANDARD READING ( $^{\circ}$ C)	UUC READING ( $^{\circ}$ C)	CORRECTION ( $^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT ( $\pm$ $^{\circ}$ C)	COVERAGE FACTOR k
25.005	25.0	0.005	---	0.0085	2.00

**4. PERCENT SLOPE 100%**

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

CERT.No.: HS-U017D

**Harikul Science Co.,Ltd.**  
 694 Soi Ratchadanivet 24, Pracharatbamphen,  
 Samsaennok, Huaikhwang, Bangkok 10310  
 Tel: 0-2274-2456 Fax: 0-2274-2443  
 Email: info@harikul.com www.harikul.com  
**Certificate of Calibration**

Calibration Date : 3 Apr 23  
 Submitted by : S.P.S CONSULTING SERVICE CO.,LTD  
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,  
 Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C  
 Avg Water Temp : 20 °C  
 Air Pressure : 760.00 mmHg  
 Salinity : 0 ppt

Model : YSI 5000  
 S/N : 15B100751  
 Probe : YSI 5010  
 S/N : 22D100097  
 ID NO. : -  
 Air Temp ref : S/N. E00522  
 Barometric ref : S/N. E00522  
 Water Temp ref : S/N. 11431  
 Technician : Kittipong M.

#### Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-
<hr/>			
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-
<hr/>			
Overall Status	(PASS)		

#### Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature

(Kittipong Maekwong)

Laboratory Manager

(Natenapha Pisatkunchon)



CERT.No.: HS-V015C

Calibration Date : 20 Mar 24  
 Submitted by : ASIA LAB @ CONSULTANT CO.,LTD  
 184 Soi Phutthamonthon Sai 2 Soi 12,  
 Bangphai, Bangkae, Bangkok 10160

Avg Room Temp : 20 °C  
 Avg Water Temp : 20 °C  
 Air Pressure : 760.00 mmHg  
 Salinity : 0 ppt

Model : YSI 5000  
 S/N : 15B100751  
 Probe : YSI 5010  
 S/N : 22D100097  
 ID NO. : -  
 Air Temp ref : S/N. F8065C26  
 Barometric ref : S/N. F8065C26  
 Water Temp ref : S/N. 11430  
 Technician : Kittipong M.

#### Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-

Overall Status (PASS)

#### Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature

(Kittipong Maekwong)

Laboratory Manager

(Supreecha Sumaritam)



# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 23T0959

REFERENCE No : 68047-2

PAGE : 1 OF 3

## Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB200


SERIAL No : 15110C0235

ID No : CRB 05/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 07-Feb-23

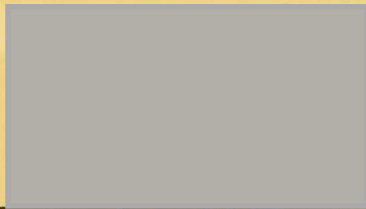APPROVED BY :   
PONGSAK J.

ISSUED DATE : 07-Feb-23

RECEIVED DATE : 31-Jan-23





CERTIFICATE No : 23T0959

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : COD REACTOR  
MANUFACTURER : HACH  
ID NUMBER : CRB 05/59  
RECEIVED DATE : 31-Jan-23  
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB200  
SERIAL NUMBER : 15110C0235  
CALIBRATION DATE : 07-Feb-23  
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	22T7511	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

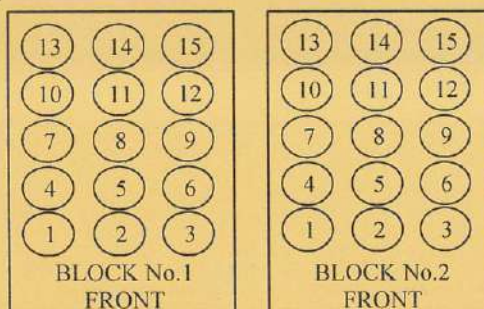

### TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	149.4
	2	149.5
	3	149.4
	4	149.4
	5	149.7
	6	149.4
	7	149.6
	8	149.3
	9	149.6
	10	149.6
	11	149.7
	12	149.3
	13	149.5
	14	149.8
	15	149.6
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY  
COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 24T0774

REFERENCE No : 71986-2

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : COD REACTOR

**MANUFACTURER** : HACH

**MODEL** : DRB 200

**SERIAL No** : 15110C0235

**ID No** : CRB 05/59

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : CHAICHARN CH.

**CALIBRATION DATE** : 5-Feb-24

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 5-Feb-24

**RECEIVED DATE** : 5-Feb-24





CERTIFICATE No : 24T0774

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : COD REACTOR  
MANUFACTURER : HACH  
ID NUMBER : CRB 05/59  
RECEIVED DATE : 5-Feb-24  
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200  
SERIAL NUMBER : 15110C0235  
CALIBRATION DATE : 5-Feb-24  
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	23T6640	14-Jul-24

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.  
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.  
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

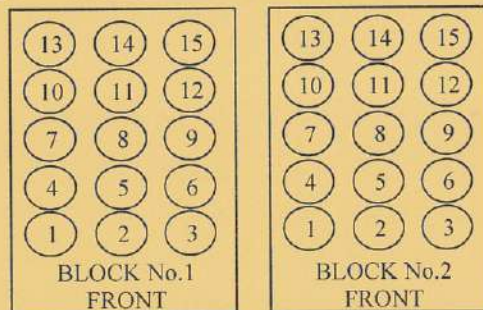

### TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	150.2
	2	150.2
	3	150.2
	4	149.9
	5	150.1
	6	150.7
	7	149.9
	8	149.9
	9	150.8
	10	149.5
	11	150.2
	12	150.0
	13	149.5
	14	149.5
	15	149.6
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY A  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERT  
COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 23M2442

REFERENCE No : 68471-2

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : SARTORIUS

**MODEL** : BSA224S-CW

**SERIAL No** : 36591843

**ID No** : BA 09/61

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23





CERTIFICATE No : 23M2442

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW  
MANUFACTURER : SARTORIUS S/N : 36591843  
ID No : BA 09/61 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23°C  $\pm$  1°C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000058
0.1	0.1000	0.0000	0.000059
0.2	0.2000	0.0000	0.000059
0.5	0.5000	0.0000	0.000060
1.0	1.0000	0.0000	0.000060
2.0	2.0000	0.0000	0.000061
5.0	5.0000	0.0000	0.000063
10.0	10.0000	0.0000	0.000067
20.0	20.0001	-0.0001	0.000073
50.0	50.0000	0.0000	0.00011
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	99.9999
3	99.9998
4	100.0001
5	100.0000
OFF-CENTER LOADING	0.0002

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 24M2229  
REFERENCE No : 72448-3

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : SARTORIUS

**MODEL** : BSA224S-CW

**SERIAL No** : 36591843

**ID No** : BA 09/61

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 08-Mar-24

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 14-Mar-24

**RECEIVED DATE** : 08-Mar-24





CERTIFICATE No : 24M2229

PAGE : 2 OF 2

## Calibration Report

**EQUIPMENT** : DIGITAL BALANCE **MODEL** : BSA224S-CW  
**MANUFACTURER** : SARTORIUS **S/N** : 36591843  
**ID No** : BA 09/61 **RECEIVED DATE** : 08-Mar-24  
**AIR PRESSURE** : 1010mbar  $\pm$  1mbar **CALIBRATION DATE** : 08-Mar-24  
**AMBIENT TEMPERATURE** : 25° C  $\pm$  1° C **RELATIVE HUMIDITY** : 55 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	50.0000	0.0000	0.00012
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>Customer :</b> <u>S.P.S.Consulting Service Co.,Ltd</u>	<b>Date Tested:</b> <u>January 4, 2024</u>	
	<b>Recommendation Recertification</b>	
<b>Address :</b> <u>7 Soi Phaholyothin 24</u>	<b>Period</b> <u>6</u> <b>Months</b>	
<u>Paholyothin Road</u>	<b>Recertification Due:</b> <u>July 4, 2024</u>	
<u>Jompol Chatuchak, Bangkok 1090</u>	<b>Date Last Certified:</b> <u>July 6, 2023</u>	
<b>User Name:</b> <u>K.Phenpha Vipasthawatt</u>	<b>Visit Number:</b> <u>2 of 2</u>	
<b>Phone:</b> <u>083-9269252</u>	<b>PerkinElmer Phone:</b> <u>02-719-6420 ext 206</u>	
<b>Fax:</b> <u>02-513-4221</u>	<b>PerkinElmer Fax:</b> <u>02-318-5597</u>	

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
<b>MODEL</b>	<b>SERIAL NUMBER</b>	
<u>OPTIMA 5300DV</u>	<u>077C7042401</u>	
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>December 30, 2024</u>
<u>Wavecal Solution</u>	<u>N058-2152</u>	<u>March 30, 2024</u>
<u>VIS Wavecal solution</u>	<u>N930-2946</u>	<u>February 28, 2024</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>November 30, 2024</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 4, 2024**1. MECHANICAL CHECKS**

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK**2. OPTICAL CHECKS**

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgefilters.

☐ OK

C. Recheck optical alignment.

☐ OK**3. COOLING SYSTEM CHECKS**

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ N/A**4. PERFORMANCE CHECKS**

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER :** 077C7042401
**DATE TESTED :** January 4, 2024

PARAMETER		SPECIFICATION		FINAL VALUE	
<b>Spectral Resolution : UV</b>	As 193.696 nm	≤ 0.007		0.00529	
	Ni 231.604 nm	≤ 0.008		0.00672	
	Ni 341.476 nm	≤ 0.012		0.00793	
<b>Spectral Resolution : VIS</b>	La 408.672 nm	≤ 0.020		0.01588	
	Ba 455.403 nm	≤ 0.025		0.02280	
<b>Precision</b>					
	As 193.656 nm	% RSD	< 1.0	0.92	%
	Zn 213.856 nm	% RSD	< 1.0	0.95	%
	Mn 257.610 nm	% RSD	< 1.0	0.75	%
	La 379.478 nm	% RSD	< 1.0	0.44	%
	Ba 455.403 nm	% RSD	< 1.0	0.46	%
	Ba 493.408 nm	% RSD	< 1.0	0.37	%
<b>Detection Limits : Axial</b>	Tl 190.080 nm	3(sd)		19.99	ppb
	As 193.696 nm	3(sd)		26.66	ppb
	Pb 220.353 nm	3(sd)		1.81	ppb
<b>Detection Limits : Radial</b>	As 193.696 nm	3(sd)		38.21	ppb
	Zn 213.856 nm	3(sd)		2.48	ppb
	Mn 257.610 nm	3(sd)		0.59	ppb
	La 379.478 nm	3(sd)		5.52	ppb
	Ba 455.403 nm	3(sd)		0.13	ppb
	Ba 493.408 nm	3(sd)		1.08	ppb
<b>BEC : Axial (IB X 500)/(IS-IB)</b>	Cd 226.502 nm	≤ 150 ppb		141.47	
<b>BEC : Radial (IB X 1000)/(IS-IB)</b>	Mn 257.610 nm	≤ 45 ppb		29.04	





## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

**SERIAL NUMBER** 077C7042401**DATE TESTED** January 4, 2024**Remarks :**

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

**Seal****Authorized Representative:**


(


Mr. Wiphan Promlumda

)

Service Engineer

## ***PinAAcle 900T Preventive Maintenance (PM)***

<b>Company Name:</b>	S.P.S. Consulting Service Co.,Ltd.		
<b>Address (Instrument Location):</b>	7, Soi Phaholyothin 24, Phaholyothin Road , Ladyao, Khet Jatujak,Bangkok, 		
<b>Serial Number:</b>	PTCS14111103	<b>PM Number:</b>	1OF2
<b>Customer Name (if applicable):</b>	K PHENPA	<b>Telephone Number:</b>	
<b>Customer Support Engineer Name:</b>	WIPHAN	<b>Service Order Number:</b>	WO-02602325
<b>Date PM Performed: (DD-MMM-YYYY)</b>	04-Jan-2024	<b>Next PM Due Date: (DD-MMM-YYYY)</b>	04-Jul-2024
<b>Standard Labor Hours to Complete PM :</b>		<b>5 hours</b>	

Part Number	Release	Publication Date	
09370143 Rev.8	A	January 2018	

### **Scope**

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900T by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

### **General Instructions:**

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

### **Copyright Information**

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

### **Trademarks**

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

**Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.**

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.



## Component List

Component / Specific Model	Serial #	Configuration Notes

## Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	1
B3002013	THGA Contact Cylinders	1
B3141064	Glycerol for THGA Cooling	N/A
N3160156	O-Ring Kits for Sampling Introduction ( Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction ( Plastic Nebulizer)	1
N9301714	Replacement Acetylene Filter Cartridge	1
TH001022	Replacement Air Filter Cartridge	1

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	26-87CYUY1	30-Jan-2024
N9300244	GFAAS Mixed Standard	AR	58-142CRY1	30-Oct-2024

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO <sub>3</sub>	250 ml.	AR	AR

Additional Tools Required for PM			
Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	MG0-252
N1013002	1.0A Neutral density filter	1	MG2-358
B3100652 Or N9307029	Electronic Flow Meter	1	N/A
B0505495	Test Jig	1	N/A
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	092216-010130
N3050109	Ba Lumina HCL	1	1-2416--040160
N3050139	K Lumina HCL	1	110716-010060
N3050152	Ni Lumina HCL	1	100516-030190
N3050119	Cr Lumina HCL	1	091911-020150



# Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

## 1. General:

- ✓ Review the instrument performance with the customer and document any recent problems.
- ✓ Inspect the customer log book and make any appropriate PM entries.
- ✓ Perform general inspection of system for cleanliness.

## 2. PC Instrument Software:

- ✓ Instrument Software user files/databases archived, packed, and/or deleted as needed.

## 3. Mechanical:

- ✓ Inspect and clean all fans and filters. Replace filters if necessary
- ☐ Inspect all gas and water lines for leaks and/or wear. Replace if needed. Thoroughly inspect all quick connects. Replace the Y connector, P/N 09921079, if needed.
- ✓ Clean exterior of the instrument.

### 3.1 Flame Technique

- ✓ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ✓ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ✓ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ✓ Check the drain system for signs of wear. Replace worn or damaged parts.
- ✓ Visually check for proper flame conditions when igniting the Air-C<sub>2</sub>H<sub>2</sub> and N<sub>2</sub>O-C<sub>2</sub>H<sub>2</sub> flames (if applicable).

### 3.2 THGA Technique

- ✓ Inspect the pole pieces and clean where the pole pieces contact the furnace. Replace the pole piece p-rings as needed, P/N's B0501018 & B0501250. Grease the O-rings as needed with Apiezon L grease, P/N 09905148
- ✓ Inspect the four insulation pads on the front contact housing of the THGA in furnace. If the pads are missing replace the THGA furnace or replace the insulator pads on the furnace.
- ✓ Inspect the graphite tube and clean the contact cylinders. Replace if necessary.
- ✓ Check internal and external gas flows with the Electronic Gas Flow Meter and the Gas Flow Test Probe as described in the Service Manual. Correct if necessary.
- ✓ Check furnace open/close function.
- ✓ Verify the operation of the GFTV Camera for proper operation and viewing alignment in the furnace camera Tube View window. Align if needed.
- ✓ Check the operation of the Halogen Light ASSY for the GFTV Camera. Replace if needed.
- ✓ Check the water level/quality in the recirculation (if applicable). Add distilled water if necessary.
- ✓ Check the cooling system fluid flow rate with the FCS In-Line Flow Meter for proper levels if needed. Refer to SDB# COSY008.STN

- ✓ Perform Cooling System maintenance if needed per SDB# COSY005.STN.
- ✓ Check auto sampler operation.
- ✓ Perform an auto sampler check valve test as described in the Service Manual.
- ✓ Lubricate the spindles of the auto sampler pumps and all moving parts of the tray mechanics as described in the Service Manual.
- ✓ Inspect the auto sampler sampling capillary as described in the Service Manual. Replace if necessary.

#### 4. Electrical:

- ✓ Inspect PC boards. Clean if necessary.
- ✓ Carefully check all internal and external cable connections.
- ✓ Check instrument firmware revisions upgrade to current levels (if necessary)
- ✓ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

#### 5. Optics:

- ✓ Inspect and clean the sample compartment windows, if needed.
- ✓ Inspect and clean the furnace windows, if needed.
- ✓ Inspect and clean the GFTV camera lens, if needed.
- ✓ Inspect optics. Clean or replace if necessary,

#### 6. Gasses:

- ☐ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ☐ Verify that the air filter element is dry. Replace if necessary.

#### 7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active	Passed
C <sub>2</sub> H <sub>2</sub> Pressure Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C <sub>2</sub> H <sub>2</sub> Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed



## 8. After PM Performance tests [Flame]:

### 8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.		0.1789	Passed
0.2 A ND Filter	± 5% from Cert.		1.0186	Passed

### 8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0017	Passed

### 8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0001	Passed

### 8.4 D<sub>2</sub> Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0084	Passed

### 8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0004	Passed

### 8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	$\leq 0.005$	0.0013	Passed

### 8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	$> 0.250$ Abs.	N/A	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	$> 0.250$ Abs.	0.4241	Passed

## 9. After PM Performance tests [THGA]:

### 9.1 Furnace Gas Flows

Description: Ensures the flow rates are within specification.

Parameter	Specification	Test Results	Pass/Fail
Internal Flow Rate	250 mL/min $\pm$ 25 mL/min	251	Passed
External Flow Rate	100 mL/min $\pm$ 10 mL/min	102	Passed

### 9.2 Chromium Baseline Noise

Description: Signal to noise check.

Parameter	Specification	Results	Pass/Fail
Baseline Noise	$\leq 0.005$ Abs.	0.0008	Passed
Standard Deviation	$\leq 0.005$	0.0003	Passed

### 9.3 Chromium Characteristic Mass and Precision

Description: Calculate the characteristic mass using the characteristic mass tool and precision from the integrated absorbance values.

Parameter	Specification	Results	Pass/Fail
Cr $m_0$ Results	$\leq 7.0$ pg/0.0044 A-s	6.2	Passed
Precision	$\leq 2.0$ %	0.61	Passed



#### 9.4 Copper Characteristic Mass and Zeeman Ratio

Description: Calculate the characteristic mass using the characteristic mass tool and check the Zeeman Ratio.

Parameter	Specification	Results	Pass/Fail
Cu m <sub>0</sub> Result	≤ 16.5 pg/0.0044 A-s	13.6	Passed
Zeeman Ratio	0.52 ± 0.04	0.544	Passed

#### 10. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

## Additional Comments

Additional Comments Regarding the PM	
Zeeman Ratio	$= \frac{\text{Atomic Signal (Peak area)}}{\text{Atomic Signal (Peak area)} + \text{Background Signal (Peak area)}}$ $= \frac{0.1602}{0.2940}$ $= 0.544$

## Review

<i>The preventive maintenance checks and if applicable performance tests for PinAAcle 900T have been completed.</i>	
<i>This PinAAcle 900T Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.</i>	
<b>Review of Preventive Maintenance:</b>	
Authorized PerkinElmer Representative:	Date: 04-Jan-2024 <small>(DD-MMM-YYYY)</small>
Authorized Customer Representative:	Date: 04-Jan-2024 <small>(DD-MMM-YYYY)</small>

ระดับเสียงในสถานที่ทำงาน





THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0639

MTC No. EEL. BP. 40/0866

## CALIBRATION CERTIFICATE

Submitted by : S.P.S Consulting Services Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : SVANTEK

Model : SV34

Serial No. : 83820

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.  
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.  
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.  
4. Digital Multimeter Agilent 34401A S/N MY44005560.  
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.  
6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.  
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2633526.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 11 Aug. 2023

Date of Calibration : 22 Aug. 2023

1/2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

Request No. 21-66/0639

MTC No. EEL. BP. 40/0866

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 114 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

### 1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	114.01	0.01	$\pm 0.10$	$\pm 0.75$ dB

### 2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1000.0	0.0	$\pm 1.5$	$\pm 2.0\%$

### 3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	0.19	$\pm 0.50$	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :



Approved by



Director  
TISTR

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 22 Aug. 2023

Date of Issue : 24 Aug. 2023

Ref : 2011266081103146003

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-1379-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Noise B\_036/24

## Noise Dose Meter Calibration Report

Acoustic Calibrator Data						
Brand	SVANTEK		Number	SV 03/60		
Model	SV34		Serial No.	83820		
Calibration Range	114 dB, 1000 Hz		Last Calibration	22 August 2023		
			Due Date	22 August 2024		
Calibration Data						
Sound Level Meter Data					Calibration Data	
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B12	SVANTEK	SV-104IS	80832	13 February 2024	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.01± 0.10 dB	

Calibrated by :







บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jomjol, Chatechak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscn.com, www.spscn.com

Noise Dose B\_041/24

## Noise Dose Meter Calibration Report

Acoustic Calibrator Data						
Brand	SVANTEK			Number	SV 03/60	
Model	SV34			Serial No.	83820	
Calibration Range	114 dB, 1000 Hz			Last Calibration	22 August 2023	
				Due Date	22 August 2024	
Calibration Data						
Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
NMD-B15	SVANTEK	SV-104IS	80880	13 February 2024	114.0	114.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					114.01± 0.10 dB	

Calibrated by :



คุณภาพอากาศในสถานประกอบการ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C  
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B01	SKC	224-PCXR4	262101	03/01/2024	1,000	1,500	2,000	993	1,497	1,998	1.002x - 4.467	1.000
B02	SKC	224-PCXR4	626166	03/01/2024	1,000	1,500	2,000	1,003	1,505	2,001	1.009x - 19.803	0.999
B03	SKC	224-PCXR4	612968	03/01/2024	1,000	1,500	2,000	996	1,494	2,001	1.006x - 12.799	1.000
B04	SKC	224-PCXR4	602804	04/01/2024	1,000	1,500	2,000	1,000	1,502	1,994	0.999x + 0.239	1.000
B05	SKC	224-PCXR4	612693	04/01/2024	1,000	1,500	2,000	1,003	1,500	2,002	1.011x - 21.266	0.999
B06	SKC	224-PCXR4	262188	05/01/2024	1,000	1,500	2,000	1,002	1,508	2,006	1.007x - 12.077	0.999
B07	SKC	224-PCXR4	626262	05/01/2024	1,000	1,500	2,000	998	1,492	1,997	0.994x + 4.810	1.000
B08	SKC	224-PCXR4	626100	04/01/2024	1,000	1,500	2,000	1,002	1,500	2,003	1.013x - 24.585	0.999
B09	SKC	224-PCXR4	626479	05/01/2024	1,000	1,500	2,000	998	1,490	1,994	0.993x + 3.837	1.000
B10	SKC	224-PCXR4	091950	04/01/2024	1,000	1,500	2,000	993	1,502	2,001	1.017x - 34.867	0.999
B11	SKC	224-PCXR8	564315	05/01/2024	1,000	1,500	2,000	996	1,492	1,999	1.004x - 7.965	1.000
B12	SKC	224-PCXR4	034656	05/01/2024	1,000	1,500	2,000	1,003	1,502	2,003	1.010x - 19.683	0.999
B13	SKC	224-PCXR4	602073	04/01/2024	1,000	1,500	2,000	997	1,500	1,998	1.000x - 0.862	1.000
B14	SKC	224-PCXR4	626313	03/01/2024	1,000	1,500	2,000	999	1,492	1,989	0.991x + 8.479	1.000
B15	SKC	224-PCXR4	626474	03/01/2024	1,000	1,500	2,000	1,002	1,502	2,005	1.012x - 21.697	0.999
B16	SKC	224-PCXR4	626477	04/01/2024	1,000	1,500	2,000	995	1,504	2,001	1.007x - 16.807	1.000
B17	SKC	224-PCXR4	626860	04/01/2024	1,000	1,500	2,000	997	1,494	1,991	0.997x + 0.331	1.000
B18	SKC	224-PCXR4	691484	05/01/2024	1,000	1,500	2,000	1,003	1,500	2,002	1.009x - 17.214	0.999
B19	SKC	224-PCXR4	691599	05/01/2024	1,000	1,500	2,000	993	1,503	1,999	1.005x - 8.906	1.000
B20	SKC	224-PCXR4	691587	05/01/2024	1,000	1,500	2,000	991	1,504	2,000	1.016x - 33.407	0.999
B21	SKC	224-PCXR4	691531	04/01/2024	1,000	1,500	2,000	993	1,499	1,995	1.001x - 5.540	1.000
B22	SKC	224-PCXR4	691654	03/01/2024	1,000	1,500	2,000	1,003	1,501	2,004	1.011x - 19.966	0.999
B23	SKC	224-PCXR4	798393	03/01/2024	1,000	1,500	2,000	993	1,507	2,002	1.017x - 33.276	0.999
B24	SKC	224-PCXR4	626363	03/01/2024	1,000	1,500	2,000	1,000	1,502	2,001	1.012x - 23.859	0.999
B25	SKC	224-PCXR4	798489	03/01/2024	1,000	1,500	2,000	1,001	1,492	2,001	0.998x + 0.694	1.000
B26	SKC	224-PCXR4	798479	04/01/2024	1,000	1,500	2,000	1,000	1,500	1,993	0.996x + 4.204	1.000
B27	SKC	224-PCXR4	691673	04/01/2024	1,000	1,500	2,000	994	1,503	2,002	1.016x - 30.902	0.999
B28	SKC	224-PCXR4	691570	05/01/2024	1,000	1,500	2,000	1,003	1,500	2,001	1.009x - 18.263	0.999
B29	SKC	224-PCXR4	626472	04/01/2024	1,000	1,500	2,000	1,002	1,498	2,000	1.002x - 3.909	1.000
B30	SKC	224-PCXR4	691489	04/01/2024	1,000	1,500	2,000	1,003	1,509	2,006	1.008x - 11.399	1.000
B31	SKC	224-PCXR4	691509	03/01/2024	1,000	1,500	2,000	993	1,496	1,997	1.005x - 11.275	1.000
B32	SKC	224-PCXR4	091567	03/01/2024	1,000	1,500	2,000	991	1,503	2,000	1.015x - 30.886	0.999
B33	SKC	224-PCXR4	091756	05/01/2024	1,000	1,500	2,000	993	1,498	1,992	0.999x - 2.317	1.000
B34	SKC	224-PCXR4	612962	05/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.007x - 13.995	1.000
B35	SKC	224-PCXR4	602682	05/01/2024	1,000	1,500	2,000	996	1,498	1,996	1.000x - 5.285	1.000
B36	SKC	224-PCXR4	626164	04/01/2024	1,000	1,500	2,000	999	1,510	1,999	1.004x - 10.131	0.999
B37	SKC	224-PCXR4	626256	05/01/2024	1,000	1,500	2,000	994	1,506	1,999	1.013x - 28.454	0.999
B38	SKC	224-PCXR4	626167	03/01/2024	1,000	1,500	2,000	997	1,498	1,998	1.003x - 5.983	1.000
B39	SKC	224-PCXR4	034637	03/01/2024	1,000	1,500	2,000	1,005	1,501	2,001	1.006x - 15.188	0.999
B40	SKC	224-PCXR4	798349	05/01/2024	1,000	1,500	2,000	994	1,505	2,000	1.014x - 29.004	0.999

Calibrated by :





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25 ± 3 °C  
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B41	SKC	224-PCXR4	612669	05/01/2024	1,000	1,500	2,000	999	1,496	1,991	0.996x + 1.914	1.000
B42	SKC	224-PCXR4	626041	03/01/2024	1,000	1,500	2,000	1,004	1,498	1,991	0.986x + 19.248	1.000
B43	SKC	224-PCXR4	034636	03/01/2024	1,000	1,500	2,000	1,000	1,501	1,992	0.991x + 11.682	1.000
B44	SKC	224-PCXR8	529341	03/01/2024	1,000	1,500	2,000	1,002	1,502	2,002	1.004x - 6.860	1.000
B45	SKC	224-PCXR8	529594	03/01/2024	1,000	1,500	2,000	1,001	1,501	1,987	0.987x + 16.026	1.000
B46	SKC	224-PCXR8	566743	04/01/2024	1,000	1,500	2,000	995	1,506	2,002	1.013x - 27.915	0.999
B47	SKC	224-PCXR8	566747	04/01/2024	1,000	1,500	2,000	1,002	1,502	2,004	1.010x - 21.769	0.999
B48	SKC	224-PCXR8	566753	04/01/2024	1,000	1,500	2,000	1,000	1,493	1,998	0.997x + 0.239	1.000
B49	SKC	224-PCXR8	566780	04/01/2024	1,000	1,500	2,000	1,003	1,502	2,006	1.011x - 21.550	0.999
B50	SKC	224-PCXR8	500400	03/01/2024	1,000	1,500	2,000	1,001	1,496	2,002	1.001x - 2.900	1.000
B51	SKC	224-PCXR8	500363	03/01/2024	1,000	1,500	2,000	996	1,502	2,000	1.011x - 25.709	0.999
B52	SKC	224-PCXR8	093186	03/01/2024	1,000	1,500	2,000	994	1,496	1,992	0.995x + 1.751	1.000
B53	SKC	224-PCXR8	707670	05/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.008x - 16.042	0.999
B54	SKC	224-PCXR3	509821	05/01/2024	1,000	1,500	2,000	995	1,501	2,002	1.016x - 32.282	0.999
B55	SKC	224-PCXR3	510710	05/01/2024	1,000	1,500	2,000	1,004	1,495	1,992	0.991x + 7.666	1.000
B56	SKC	224-PCXR3	511450	05/01/2024	1,000	1,500	2,000	1,002	1,500	2,001	1.005x - 8.559	1.000
B57	SKC	224-PCXR3	510798	03/01/2024	1,000	1,500	2,000	997	1,492	1,999	0.999x - 2.122	1.000
B58	SKC	224-PCXR3	509852	03/01/2024	1,000	1,500	2,000	1,000	1,500	1,999	1.007x - 19.073	0.999
B59	SKC	224-PCXR3	509862	04/01/2024	1,000	1,500	2,000	995	1,503	1,995	0.998x + 2.118	1.000
B60	SKC	224-PCXR3	512655	04/01/2024	1,000	1,500	2,000	1,004	1,510	2,004	1.005x - 6.421	0.999
B61	SKC	224-PCXR3	503915	04/01/2024	1,000	1,500	2,000	993	1,492	1,999	1.003x - 11.706	1.000
B62	SKC	224-PCXR3	505975	03/01/2024	1,000	1,500	2,000	999	1,494	1,996	0.996x + 0.822	1.000
B63	SKC	224-PCXR3	511432	03/01/2024	1,000	1,500	2,000	990	1,501	2,000	1.017x - 36.259	0.999
B64	SKC	224-PCXR3	508302	03/01/2024	1,000	1,500	2,000	998	1,492	1,989	0.990x + 10.175	1.000
B65	SKC	224-PCXR3	508310	03/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.007x - 13.537	1.000
B66	SKC	224-PCXR3	509861	04/01/2024	1,000	1,500	2,000	1,002	1,491	1,992	0.988x + 13.744	1.000
B67	SKC	224-PCXR3	506295	04/01/2024	1,000	1,500	2,000	995	1,508	2,004	1.007x - 12.843	1.000
B68	SKC	224-PCXR3	505872	04/01/2024	1,000	1,500	2,000	1,002	1,491	1,998	0.995x + 4.040	1.000
B69	SKC	224-PCXR3	508375	04/01/2024	1,000	1,500	2,000	1,003	1,499	2,000	1.009x - 18.977	0.999
B70	SKC	224-PCXR3	510623	05/01/2024	1,000	1,500	2,000	992	1,493	1,996	1.002x - 7.730	1.000
B71	SKC	224-PCXR3	508367	05/01/2024	1,000	1,500	2,000	994	1,506	2,002	1.015x - 31.561	0.999
B72	SKC	224-PCXR3	505977	03/01/2024	1,000	1,500	2,000	1,003	1,499	1,994	0.991x + 9.042	1.000
B73	SKC	224-PCXR3	512606	04/01/2024	1,000	1,500	2,000	1,001	1,501	2,004	1.008x - 14.346	1.000
B74	SKC	224-PCXR3	505993	04/01/2024	1,000	1,500	2,000	996	1,497	1,995	1.001x - 7.036	1.000
B75	SKC	224-PCXR3	509820	05/01/2024	1,000	1,500	2,000	996	1,496	1,991	0.996x + 1.432	1.000
B76	SKC	224-PCXR3	509811	05/01/2024	1,000	1,500	2,000	993	1,499	1,999	1.006x - 14.283	1.000
B77	SKC	224-PCXR3	508301	05/01/2024	1,000	1,500	2,000	1,001	1,501	2,003	1.013x - 25.406	0.999
B78	SKC	224-PCXR3	510677	05/01/2024	1,000	1,500	2,000	995	1,503	1,999	1.012x - 27.520	0.999
B79	SKC	224-PCXR3	510920	05/01/2024	1,000	1,500	2,000	994	1,494	1,994	1.001x - 6.178	1.000

Calibrated by :



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-B01	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	506.5	991.1	1974.3	0.989x + 9.286	1.000
H-B02	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	496.7	997.6	1996.1	0.994x + 4.509	1.000
H-B03	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	497.6	988.8	2009.6	1.004x - 14.177	0.999
H-B04	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	501.6	998.7	2006.5	0.997x - 0.777	1.000
H-B05	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	500.4	997.3	1974.3	0.980x + 21.602	0.999
H-B06	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	504.9	994.8	1984.0	1.003x - 5.213	1.000
H-B07	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	502.6	990.6	2016.7	1.001x - 0.998	1.000
H-B08	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	499.7	998.7	1979.8	0.996x + 3.580	0.999
H-B09	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	504.1	1004.3	2010.7	0.993x + 13.998	1.000
H-B10	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	496.2	999.3	2009.2	0.996x + 3.860	1.000

Calibrated by :



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)CERTIFICATE No : 23M2441  
REFERENCE No : 68471-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905

**ID No** : BA 05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** : [REDACTED]  
PONGSAK J.

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23° C  $\pm$  1° C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT