

# ภาคผนวกที่ 4

---

## เอกสารการสอบเทียบความถูกต้องของ เครื่องมือตรวจวัดคุณภาพสิ่งแวดล้อม

- 1) คุณภาพอากาศในบรรยากาศ
- 2) ผลการตรวจวัดคุณภาพอากาศจากปล่อง
- 3) ผลการตรวจวัดคุณภาพอากาศในสถานประกอบการ
- 4) ผลการตรวจวัดระดับเสียงในสถานประกอบการ
- 5) ผลการตรวจวัดระดับความร้อนในสถานประกอบการ
- 6) ผลการตรวจวิเคราะห์คุณภาพน้ำ

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
<b>1. คุณภาพอากาศในบรรยากาศ</b>		
Total Suspended Particulate	High Volume Air Sampler No. B21, B35, B44	Digital Balance
Sulfur Dioxide	SO <sub>2</sub> Analyzer No. B02, B06, B08	SO <sub>2</sub> Analyzer No. B01, B05, B06
Nitrogen Dioxide	NO/NO <sub>x</sub> /NO <sub>2</sub> Analyzer No. B07, B12, B14	NO/NO <sub>x</sub> /NO <sub>2</sub> Analyzer No. B07, B16, B18
<b>2. คุณภาพอากาศจากปล่อง</b>		
Total Suspended Particulate	Console No. B04 Pitot Tube No. B04	Digital Balance
Sulfur Dioxide	Personal Pump SKC No. B06 Rotameter No. H-B04	-
Oxides of Nitrogen	Vacuum Gauge	Spectrophotometer
Sulfuric Acid	Console No. B04 Pitot Tube No. B04	-
<b>3. คุณภาพอากาศในสถานประกอบการ</b>		
Total Dust	Personal Pump SKC No. B58, B75, B84, B86, B93 Rotameter No. H-B07, B10	Digital Balance
Sulfuric Acid	Personal Pump SKC No. B70, B78 Rotameter No. L-B07, B10	Ion Chromatography
<b>4. ระดับเสียงในสถานประกอบการ</b>		
L <sub>eq</sub> 8 hr	Acoustic Calibrator Sound Level Meter No. ACO-B18, B29, B33, B36, B41, B43	- -
<b>5. ความร้อนในสถานประกอบการ</b>		
WBGT	Digital Thermometer Heat Stress WBGT Meter No. B07, B11, B12, B17, B30	-
<b>6. คุณภาพน้ำ</b>		
pH	-	pH Meter
BOD <sub>5</sub>	-	BOD Analyzer
COD	-	COD Reactor
Grease & Oil	-	Digital Balance
Total Suspended Solids	-	Digital Balance
Total Dissolved Solids	-	Digital Balance
Zinc	-	ICP AAS
Nickel	-	ICP AAS
Cadmium	-	ICP AAS
Total Iron	-	ICP
Total Aluminum	-	ICP
TCB	-	Incubator Water Bath
Fluoride	-	Spectrophotometer

คุณภาพอากาศในบรรยากาศ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

### High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

#### Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B01	B01	01/02/2024	y = 1.224x-3.492	0.998
B02	B02	01/02/2024	y = 1.143x+1.630	0.999
B03	B03	01/02/2024	y = 1.160x-2.783	1.000
B04	B04	02/02/2024	y = 1.257x-5.884	0.997
B05	B05	03/02/2024	y = 1.261x-7.123	0.999
B06	B06	02/02/2024	y = 1.245x-6.024	0.999
B07	B07	03/02/2024	y = 1.209x-6.025	0.997
B08	B08	02/02/2024	y = 1.239x-5.848	0.997
B09	B09	02/02/2024	y = 1.244x-5.247	0.997
B10	B10	02/02/2024	y = 1.153x+0.064	0.998
B11	B11	01/02/2024	y = 1.110x-1.064	1.000
B12	B12	03/02/2024	y = 1.227x-6.093	0.999
B13	B13	01/02/2024	y = 1.286x-7.460	1.000
B14	B14	02/02/2024	y = 1.220x-5.066	0.999
B15	B15	02/02/2024	y = 1.150x-1.264	0.999
B16	B16	03/02/2024	y = 1.177x-3.231	0.996
B17	B17	02/02/2024	y = 1.235x-5.039	0.999
B18	B18	03/02/2024	y = 1.210x-5.028	0.998
B19	B19	03/02/2024	y = 1.215x-7.087	0.998
B20	B20	02/02/2024	y = 1.204x-4.119	0.996
B21	B21	02/02/2024	y = 1.190x-4.960	0.999
B22	B22	02/02/2024	y = 1.208x-7.133	0.996
B23	B23	01/02/2024	y = 1.217x-4.085	0.998
B24	B24	01/02/2024	y = 1.145x-2.502	1.000
B25	B25	02/02/2024	y = 1.090x+1.068	0.999
B26	B26	03/02/2024	y = 1.234x-5.493	0.998
B27	B27	01/02/2024	y = 1.168x-4.382	0.999
B28	B28	02/02/2024	y = 1.237x-7.982	0.999
B29	B29	03/02/2024	y = 1.186x-2.530	0.996
B30	B30	02/02/2024	y = 1.212x-4.090	0.997
B31	B31	02/02/2024	y = 1.195x-4.732	0.999
B32	B32	03/02/2024	y = 1.169x-0.802	0.996
B33	B33	03/02/2024	y = 1.203x-2.954	0.996
B34	B34	02/02/2024	y = 1.221x-5.796	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

### High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

#### Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (ft <sup>3</sup> /min)	R <sup>2</sup>
B35	B35	02/02/2024	y = 1.188x-3.435	0.996
B36	B36	01/02/2024	y = 1.201x-4.036	0.999
B37	B37	01/02/2024	y = 1.196x-2.671	0.998
B38	B38	02/02/2024	y = 1.232x-6.552	0.997
B39	B39	03/02/2024	y = 1.164x-0.902	0.997
B40	B40	01/02/2024	y = 1.225x-6.117	0.999
B41	B41	02/02/2024	y = 1.265x-6.140	0.999
B42	B42	02/02/2024	y = 1.187x-3.625	0.999
B43	B43	01/02/2024	y = 1.233x-2.707	0.997
B44	B44	01/02/2024	y = 1.202x-3.263	0.996
R01	R01	01/02/2024	y = 1.214x-4.512	0.999
R02	R02	02/02/2024	y = 1.222x-5.522	0.999
R03	R03	03/02/2024	y = 1.204x-5.785	0.999
R04	R04	01/02/2024	y = 1.220x-5.355	0.999
R05	R05	01/02/2024	y = 1.190x-5.262	0.997
R06	R06	02/02/2024	y = 1.223x-6.383	0.998
R07	R07	02/02/2024	y = 1.084x+0.577	0.999
R08	R08	01/02/2024	y = 1.157x-2.531	0.999
R09	R09	01/02/2024	y = 1.194x-3.227	0.998
R10	R10	02/02/2024	y = 1.198x-4.625	0.998
R11	R11	02/02/2024	y = 1.143x-2.176	1.000
R12	R12	02/02/2024	y = 1.165x-4.124	0.998
R13	R13	03/02/2024	y = 1.133x-1.833	0.997
R14	R14	01/02/2024	y = 1.216x-3.559	0.995
R15	R15	01/02/2024	y = 1.183x-5.143	0.999
R16	R16	01/02/2024	y = 1.227x-7.151	0.999
R17	R17	02/02/2024	y = 1.181x-3.964	0.996
R18	R18	02/02/2024	y = 1.195x-3.915	0.997
R19	R19	03/02/2024	y = 1.215x-6.609	1.000
R20	R20	03/02/2024	y = 1.208x-5.309	0.998

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

## CALIBRATION REPORT

### SO<sub>2</sub> FLUORESCENT ANALYZER

DATE : 17 February 2024

BRAND : API

MODEL : 100A

NO. SO<sub>2</sub>-B02

SERIAL NO. 1847

#### Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 08 August 2023

Serial No. : 911

#### Reference Standard Gas

Standard Gas : Sulphur Dioxide (SO<sub>2</sub>)

Cylinder No. : A00814SK

Certified Date : 21 June 2021

Expired Date : 21 June 2029

Cylinder Conc. : 49.8 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.4 °C

% RH 48

#### CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.8	-0.050	400.0	1.006

#### API Model 100A SO<sub>2</sub> Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.6	in-Hg	25-35
SAMPLE FLOW	655	cc/min	650 ± 10%
PMT	103.2	mV	-20-150 with Zero Air
UV LAMP	3038.4	mV	1000-4900
STR. LGT	61.7	PPB	<100
DRK PMT	63.2	mV	-50 - 200
DRK LMP	57.9	mV	-50 - 200
HVPS	669	V	550-900 constant
DCPS	2515	mV	2500 ± 200
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.0	°C	5-40
PMT TEMP	7.2	°C	7 ± 2.0
SO <sub>2</sub> Span Conc	400	PPB	20-20,000
SO <sub>2</sub> Slope	1.006	-	1.0 ± 0.3
SO <sub>2</sub> Offset	21.8	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com.. www.spscon.com

## CALIBRATION REPORT

### SO<sub>2</sub> FLUORESCENT ANALYZER

DATE : 17 February 2024

BRAND : API

MODEL : 100E

NO. SO<sub>2</sub>-B06

SERIAL NO. 3430

#### Calibrator (Dilution System)

Brand	: API	Model	: 700
Last Cal. Date	: 08 August 2023	Serial No.	: 911

#### Reference Standard Gas

Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )	Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029
		Cylinder Conc.	: 49.8 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.4 °C % RH 48

#### CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
SO <sub>2</sub> Span	400.0	400.1	0.025	400.0	1.010

#### API Model 100E SO<sub>2</sub> Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.4	in-Hg	25-35
SAMPLE FLOW	656	cc/min	650 ± 10%
PMT	103.3	mV	-20-150 with Zero Air
UV LAMP	3041.5	mV	1000-4900
STR. LGT	61.5	PPB	<100
DRK PMT	62.9	mV	-50 - 200
DRK LMP	57.8	mV	-50 - 200
HVPS	674	V	550-900 constant
DCPS	2528	mV	2500 ± 200
RCELL TEMP	50.1	°C	50 ± 1
BOX TEMP	29.3	°C	5-40
PMT TEMP	7.4	°C	7 ± 2.0
SO <sub>2</sub> Span Conc	400	PPB	20-20,000
SO <sub>2</sub> Slope	1.010	-	1.0 ± 0.3
SO <sub>2</sub> Offset	22.1	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

## CALIBRATION REPORT

### SO<sub>2</sub> FLUORESCENT ANALYZER

DATE : 17 February 2024

BRAND : API

MODEL : 100A

NO. SO<sub>2</sub>-B08

SERIAL NO. 1003

#### Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 08 August 2023

Serial No. : 911

#### Reference Standard Gas

Standard Gas : Sulphur Dioxide (SO<sub>2</sub>)

Cylinder No. : A008145K

Certified Date : 21 June 2021

Expired Date : 21 June 2029

Cylinder Conc. : 49.8 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.4 °C

% RH 48

#### CALIBRATION SETTING

Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.7	-0.075	400.0	1.004

#### API Model 100A SO<sub>2</sub> Analyzer Check list

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	0-500
SAMPLE PRESS	28.7	in-Hg	25-35
SAMPLE FLOW	658	cc/min	650 ± 10%
PMT	103.1	mV	-20-150 with Zero Air
UV LAMP	3018.7	mV	1000-4900
STR, LGT	61.9	PPB	<100
DRK PMT	63.3	mV	-50 - 200
DRK LMP	58.1	mV	-50 - 200
HVPS	675	V	550-900 constant
DCPS	2527	mV	2500 ± 200
RCELL TEMP	50.2	°C	50 ± 1
BOX TEMP	29.5	°C	5-40
PMT TEMP	7.1	°C	7 ± 2.0
SO <sub>2</sub> Span Conc	400	PPB	20-20,000
SO <sub>2</sub> Slope	1.004	-	1.0 ± 0.3
SO <sub>2</sub> Offset	22.2	mV	<250
Stability at Zero	0.1	PPB	<0.2
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 17 February 2024

BRAND : API

MODEL : 200E

NO. NOX-B07

SERIAL NO. 4338

#### Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 08 August 2023

Serial No. : 911

#### Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : A00726SV

Certified Date : 05 January 2023

Expired Date : 05 January 2026

Cylinder Conc. : 48.8 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.4 °C

% RH 48

#### CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.11	-	0	-
NO Span	400	399.9	-0.025	400.0	1.005
NO <sub>x</sub> Span	400	400.1	0.025	400.0	1.009

#### API Model 200E NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	507	cc/min	500 ± 50
OZONE FLOW	78	cc/min	80 ± 15
PMT	103.1	mV	-20 - 150
AZERO	93.8	mV	-20 - 150
HVPS	670	V	420 - 900 constant
RCELL TEMP	50.3	°C	50 ± 1
BOX TEMP	29.1	°C	8 - 48
PMT TEMP	7.2	°C	7 ± 2
MOLY TEMP	314.9	°C	315 ± 5
RCELL PRESS	8.4	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.6	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.005	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.009	-	1.0 ± 0.3
NO Offset	1.3	mV	-20 to +150
NO <sub>x</sub> Offset	0.9	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## CALIBRATION REPORT

### CHEMILUMINESCENT NO / NO<sub>2</sub> / NO<sub>x</sub> ANALYZER

DATE : 17 February 2024

BRAND : API

MODEL : 200A

NO. NOX-B12

SERIAL NO. 2675

#### Calibrator (Dilution System)

Brand : API

Model : 700

Last Cal. Date : 08 August 2023

Serial No. : 911

#### Reference Standard Gas

Standard Gas : Nitric Oxide (NO)

Cylinder No. : A00726SV

Certified Date : 05 January 2023

Expired Date : 05 January 2026

Cylinder Conc. : 48.8 ppm

#### CALIBRATING CONDITION

Pressure 1011 mmbar

Temp. 24.4 °C

% RH 48

#### CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.008
NO <sub>x</sub> Span	400	400.2	0.050	400.0	1.012

#### API Model 200A NO<sub>x</sub> Analyzer Check List

Test Values	Observed Value	Units	Nominal Range
RANGE	500	PPB	500 standard
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air
SAMPLE FLOW	512	cc/min	500 ± 50
OZONE FLOW	79	cc/min	80 ± 15
PMT	103.3	mV	-20 - 150
AZERO	94.1	mV	-20 - 150
HVPS	675	V	420 - 900 constant
RCELL TEMP	50.2	°C	50 ± 1
BOX TEMP	29.4	°C	8 - 48
PMT TEMP	7.3	°C	7 ± 2
MOLY TEMP	314.8	°C	315 ± 5
RCELL PRESS	8.3	IN-Hg-A	2 - 10 constant
SAMPLE PRESS	28.5	IN-Hg-A	25 - 30 constant
NO Span Conc	400	PPB	20 - 20,000
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000
NO Slope	1.008	-	1.0 ± 0.3
NO <sub>x</sub> Slope	1.012	-	1.0 ± 0.3
NO Offset	1.6	mV	-20 to +150
NO <sub>x</sub> Offset	1.0	mV	-20 to 150
Stability at Zero	0.1	PPB	< 0.2
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	17 February 2024	BRAND :	API	MODEL :	200A
NO.	NOX-B14	SERIAL NO.	212		
Calibrator (Dilution System)					
Brand	: API			Model	: 700
Last Cal. Date	: 08 August 2023			Serial No.	: 911
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)			Cylinder No.	: A00726SV
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.4	°C
			% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.11	-	0	-
NO Span	400	399.6	-0.100	400.0	1.004
NO <sub>x</sub> Span	400	399.8	-0.050	400.0	1.007
API Model 200A NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	504	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.2	mV	-20 - 150		
AZERO	93.9	mV	-20 - 150		
HVPS	669	V	420 - 900 constant		
RCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	28.8	°C	8 - 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	315.2	°C	315 ± 5		
RCELL PRESS	8.2	IN-Hg-A	2 - 10 constant		
SAMPLE PRESS	28.4	IN-Hg-A	25 - 30 constant		
NO Span Conc	400	PPB	20 - 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 - 20,000		
NO Slope	1.004	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.007	-	1.0 ± 0.3		
NO Offset	1.1	mV	-20 to +150		
NO <sub>x</sub> Offset	0.7	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905


**ID No** : BA 05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

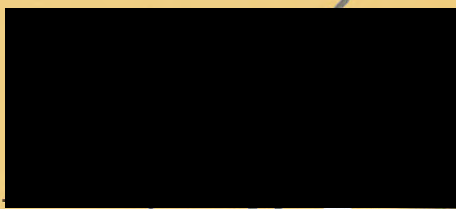**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23°C  $\pm$  1°C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





CERTIFICATE No : 24M2227

REFERENCE No : 72448-1

PAGE : 1 OF 2

## Certificate of Calibration

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905

**ID No** : BA05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 08-Mar-24

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 14-Mar-24

**RECEIVED DATE** : 08-Mar-24





CERTIFICATE No : 24M2227

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA05/50 RECEIVED DATE : 08-Mar-24  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 08-Mar-24  
AMBIENT TEMPERATURE : 25° C  $\pm$  1° C RELATIVE HUMIDITY : 53 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02001	-0.00001	0.000065
0.10	0.10002	-0.00002	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	9.99994	0.00006	0.000070
20.00	20.00008	-0.00008	0.000078
50.00	50.0000	0.0000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0001	-0.0001	0.00022

### 5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

คุณภาพอากาศจากปล่อง





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

## Console Calibration Report

Calibration Method

Critical Orifices

### Calibration Data

Console Data		Calibration Data		
No.	Serial No.	Date	y	DH <sub>g</sub> (mmH <sub>2</sub> O)
B01	1563	01/12/2023	0.998	50.05
B02	8002514	02/12/2023	1.006	49.58
B03	1503016	01/12/2023	1.003	50.16
B04	00006659	04/12/2023	0.998	49.71
B05	00007428	04/12/2023	0.999	49.24
R01	1561	02/12/2023	1.005	49.98
R02	8002513	03/12/2023	1.003	49.90
R03	1570	04/12/2023	0.996	49.68
R04	8002519	01/12/2023	1.002	49.43
R05	1503015	01/12/2023	0.997	50.24

Remark : Accept Value of y (test) is  $0.97 < y < 1.03$

Accept Value of DH<sub>g</sub> (test) is  $46.7 \pm 6.4$  (mmH<sub>2</sub>O)

Calibrated by :

[Redacted Signature]

(Mr. Adul Dangklom)

Approved by :

[Redacted Signature]

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

## Pitot Tube Calibration Report

Calibration Method

Standard Pitot Tube

### Calibration Data

Pitot Tube Data			Calibration Data		
No.	Type of Pitot	Coefficient of Standard Pitot	Date	Avg. of Cp (test)	
				Side A	Side B
B03	S	0.99	01/02/2024	0.84	0.83
B04	S	0.99	02/02/2024	0.85	0.84
B05	S	0.99	02/02/2024	0.84	0.84
B07	S	0.99	01/02/2024	0.84	0.85
B08	S	0.99	01/02/2024	0.83	0.84
B09	S	0.99	03/02/2024	0.84	0.85
B11	S	0.99	03/02/2024	0.84	0.84
B16	S	0.99	01/02/2024	0.83	0.84
B18	S	0.99	02/02/2024	0.84	0.84
B19	S	0.99	02/02/2024	0.84	0.83
B21	S	0.99	01/02/2024	0.84	0.85
B24	S	0.99	02/02/2024	0.85	0.84
B27	S	0.99	01/02/2024	0.84	0.84
B30	S	0.99	02/02/2024	0.84	0.83
B31	S	0.99	02/02/2024	0.84	0.85
B33	S	0.99	01/02/2024	0.84	0.84
B35	S	0.99	01/02/2024	0.85	0.84

Remark : Accept value of Cp (test) is  $0.84 \pm 0.01$

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C  
Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B01	SKC	224-PCXR4	262101	03/01/2024	1,000	1,500	2,000	993	1,497	1,998	1.002x - 4.467	1.000
B02	SKC	224-PCXR4	626166	03/01/2024	1,000	1,500	2,000	1,003	1,505	2,001	1.009x - 19.803	0.999
B03	SKC	224-PCXR4	612968	03/01/2024	1,000	1,500	2,000	996	1,494	2,001	1.006x - 12.799	1.000
B04	SKC	224-PCXR4	602804	04/01/2024	1,000	1,500	2,000	1,000	1,502	1,994	0.999x + 0.239	1.000
B05	SKC	224-PCXR4	612693	04/01/2024	1,000	1,500	2,000	1,003	1,500	2,002	1.011x - 21.266	0.999
B06	SKC	224-PCXR4	262188	05/01/2024	1,000	1,500	2,000	1,002	1,508	2,006	1.007x - 12.077	0.999
B07	SKC	224-PCXR4	626262	05/01/2024	1,000	1,500	2,000	998	1,492	1,997	0.994x + 4.810	1.000
B08	SKC	224-PCXR4	626100	04/01/2024	1,000	1,500	2,000	1,002	1,500	2,003	1.013x - 24.585	0.999
B09	SKC	224-PCXR4	626479	05/01/2024	1,000	1,500	2,000	998	1,490	1,994	0.993x + 3.837	1.000
B10	SKC	224-PCXR4	091950	04/01/2024	1,000	1,500	2,000	993	1,502	2,001	1.017x - 34.867	0.999
B11	SKC	224-PCXR8	564315	05/01/2024	1,000	1,500	2,000	996	1,492	1,999	1.004x - 7.965	1.000
B12	SKC	224-PCXR4	034656	05/01/2024	1,000	1,500	2,000	1,003	1,502	2,003	1.010x - 19.683	0.999
B13	SKC	224-PCXR4	602073	04/01/2024	1,000	1,500	2,000	997	1,500	1,998	1.000x - 0.862	1.000
B14	SKC	224-PCXR4	626313	03/01/2024	1,000	1,500	2,000	999	1,492	1,989	0.991x + 8.479	1.000
B15	SKC	224-PCXR4	626474	03/01/2024	1,000	1,500	2,000	1,002	1,502	2,005	1.012x - 21.697	0.999
B16	SKC	224-PCXR4	626477	04/01/2024	1,000	1,500	2,000	995	1,504	2,001	1.007x - 16.807	1.000
B17	SKC	224-PCXR4	626860	04/01/2024	1,000	1,500	2,000	997	1,494	1,991	0.997x + 0.331	1.000
B18	SKC	224-PCXR4	691484	05/01/2024	1,000	1,500	2,000	1,003	1,500	2,002	1.009x - 17.214	0.999
B19	SKC	224-PCXR4	691599	05/01/2024	1,000	1,500	2,000	993	1,503	1,999	1.005x - 8.906	1.000
B20	SKC	224-PCXR4	691587	05/01/2024	1,000	1,500	2,000	991	1,504	2,000	1.016x - 33.407	0.999
B21	SKC	224-PCXR4	691531	04/01/2024	1,000	1,500	2,000	993	1,499	1,995	1.001x - 5.540	1.000
B22	SKC	224-PCXR4	691654	03/01/2024	1,000	1,500	2,000	1,003	1,501	2,004	1.011x - 19.966	0.999
B23	SKC	224-PCXR4	798393	03/01/2024	1,000	1,500	2,000	993	1,507	2,002	1.017x - 33.276	0.999
B24	SKC	224-PCXR4	626363	03/01/2024	1,000	1,500	2,000	1,000	1,502	2,001	1.012x - 23.859	0.999
B25	SKC	224-PCXR4	798489	03/01/2024	1,000	1,500	2,000	1,001	1,492	2,001	0.998x + 0.694	1.000
B26	SKC	224-PCXR4	798479	04/01/2024	1,000	1,500	2,000	1,000	1,500	1,993	0.996x + 4.204	1.000
B27	SKC	224-PCXR4	691673	04/01/2024	1,000	1,500	2,000	994	1,503	2,002	1.016x - 30.902	0.999
B28	SKC	224-PCXR4	691570	05/01/2024	1,000	1,500	2,000	1,003	1,500	2,001	1.009x - 18.263	0.999
B29	SKC	224-PCXR4	626472	04/01/2024	1,000	1,500	2,000	1,002	1,498	2,000	1.002x - 3.909	1.000
B30	SKC	224-PCXR4	691489	04/01/2024	1,000	1,500	2,000	1,003	1,509	2,006	1.008x - 11.399	1.000
B31	SKC	224-PCXR4	691509	03/01/2024	1,000	1,500	2,000	993	1,496	1,997	1.005x - 11.275	1.000
B32	SKC	224-PCXR4	091567	03/01/2024	1,000	1,500	2,000	991	1,503	2,000	1.015x - 30.886	0.999
B33	SKC	224-PCXR4	091756	05/01/2024	1,000	1,500	2,000	993	1,498	1,992	0.999x - 2.317	1.000
B34	SKC	224-PCXR4	612962	05/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.007x - 13.995	1.000
B35	SKC	224-PCXR4	602682	05/01/2024	1,000	1,500	2,000	996	1,498	1,996	1.000x - 5.285	1.000
B36	SKC	224-PCXR4	626164	04/01/2024	1,000	1,500	2,000	999	1,510	1,999	1.004x - 10.131	0.999
B37	SKC	224-PCXR4	626256	05/01/2024	1,000	1,500	2,000	994	1,506	1,999	1.013x - 28.454	0.999
B38	SKC	224-PCXR4	626167	03/01/2024	1,000	1,500	2,000	997	1,498	1,998	1.003x - 5.983	1.000
B39	SKC	224-PCXR4	034637	03/01/2024	1,000	1,500	2,000	1,005	1,501	2,001	1.006x - 15.188	0.999
B40	SKC	224-PCXR4	798349	05/01/2024	1,000	1,500	2,000	994	1,505	2,000	1.014x - 29.004	0.999

Calibrated by :

(Mr. Abdul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-B01	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	506.5	991.1	1974.3	0.989x + 9.286	1.000
H-B02	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	496.7	997.6	1996.1	0.994x + 4.509	1.000
H-B03	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	497.6	988.8	2009.6	1.004x - 14.177	0.999
H-B04	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	501.6	998.7	2006.5	0.997x - 0.777	1.000
H-B05	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	500.4	997.3	1974.3	0.980x + 21.602	0.999
H-B06	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	504.9	994.8	1984.0	1.003x - 5.213	1.000
H-B07	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	502.6	990.6	2016.7	1.001x - 0.998	1.000
H-B08	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	499.7	998.7	1979.8	0.996x + 3.580	0.999
H-B09	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	504.1	1004.3	2010.7	0.993x + 13.998	1.000
H-B10	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	496.2	999.3	2009.2	0.996x + 3.860	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



CLC  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## CERTIFICATE OF CALIBRATION FOR

NOMENCLATURE : VACUUM GAUGE  
MANUFACTURER : HI-LIGHT  
MODEL / TYPE : N/A  
SERIAL NO. : N/A[64-220088-1]  
CLID. NO. : 212301419  
JOB CONTROL NO. : 230725081570


CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 25 July 2023

DATE OF ISSUED : 31 July 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sittipong Pimdee  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory

31 July 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23081570

F3-011-04/01-12

page 1 of 3



@clccalibration



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE	:	VACUUM GAUGE
MANUFACTURER	:	HI-LIGHT
MODEL / TYPE	:	N/A
SERIAL NO.	:	N/A[64-220088-1]
DATE OF CALIBRATION	:	26 July 2023
DUE DATE OF CALIBRATION	:	26 July 2024

---

#### ENVIRONMENT CONDITIONS :

Temperature :  $(23 \pm 2) ^\circ\text{C}$

Relative Humidity :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPPP-05** according to **DKD-R 6-1** as calibration guidelines.

The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).

Certificate No. MP-0035-23, Due Date 02 February 2024.

#### UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of  $k = 2$ . It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q23081570

F3-011-04/01-12

page 2 of 3



@clccalibration






**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14, 55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

## CALIBRATION DATA

### **CORRECTION OF PRESSURE**

DUC Test point ( inHg )	STD Reading ( kPa )		Conversion to inHg		Correction ( inHg )	
	Up	Down	Up	Down	Up	Down
0	0.00	0.00	0.0	0.0	0.0	0.0
-5	-15.07	-15.10	-4.5	-4.5	+0.5	+0.5
-10	-32.10	-32.13	-9.5	-9.5	+0.5	+0.5
-15	-49.20	-49.23	-14.5	-14.5	+0.5	+0.5
-20	-66.26	-66.26	-19.6	-19.6	+0.4	+0.4
-25	-83.30	-83.33	-24.6	-24.6	+0.4	+0.4
-30	-100.39	-100.39	-29.6	-29.6	+0.4	+0.4

Uncertainty of measurement  $\pm 0.2$  inHg

Transmitting fluid : Air.

Technical Note. Conversion factor 1 kPa ; 0.2953003 inHg

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

**This report is valid for the above stated instrument/s only.**

### End of Certificate ###

Certificate No. Q23081570

F3-011-04/01-12

page 3 of 3



@clccalibration

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905


**ID No** : BA 05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

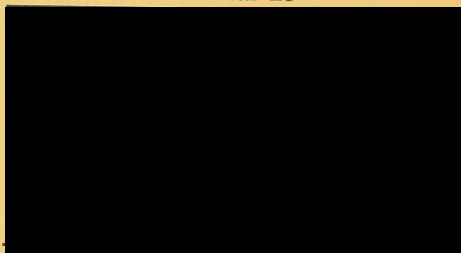**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23°C  $\pm$  1°C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd.,Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

NSC-TISI-TIS 17025  
CALIBRATION 0394

Cert. No. : SP23016

Pages : 1 of 3

## Calibration Certificate

**Equipment :** UV-VIS SPECTROPHOTOMETER  
**Manufacturer :** PERKINELMER  
**Model :** LAMBDA 25  
**Serial No.:** 501S14123010  
**ID No.:** SP03/58  
**Calibration Mode :** WAVELENGTH ACCURACY  
PHOTOMETRIC ACCURACY  
**Condition As Found :** GOOD  
**Customer :** S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN ROAD,  
CHOMPHON, CHATUCHAK,  
BANGKOK 10900, THAILAND.  
**Location :** ORGANIC LABORATORY IV  
**Ambient Temperature :** ( 25.0 ± 5 ) °C  
**Relative Humidity :** ( 48.4 ± 25 ) %  
**Received Date :** 30 AUGUST 2023  
**Calibration Date :** 30 AUGUST 2023  
**Date of Issue :** 31 AUGUST 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : SP23016

Job No. : VC66SP0014

Pages : 2 of 3

**Calibration Method :**

This instrument was calibrated by using on-site calibration procedure In-house method : CP-SP-01

The calibration procedure to direct measurement wavelength accuracy by using wavelength standard solution, Photometric accuracy by using absorbance standard filter and absorbance standard solution

The calibration procedure used was based on ASTM E275-01,ASTM E925-02

**Condition of this result of calibration :**

## 1. Certified reference materials

Material	Ref. type	Cell serial No.	Cert. No.	Due Date
Holmium liquid	RM-HL	29706	106864	01/11/2024
Didymium liquid	RM-DL	28912	106905	02/11/2024
Neutral density filter	RM-1N2N3N	13877	106918	03/11/2024
Potassium dichromate solutions	RM-0204060810	14204	106902	02/11/2024
Potassium Iodide solution	-	KI-0701-001	CI-0090-22	08/04/2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 The UK National Physical Laboratory (NPL)

3.2 The National Institute of Standards and Technology,NIST.

**Result of calibration : Wavelength Accuracy**

(Without adjustment)

Material	Certified Values of Reference Material (nm)	UUC* Reading (nm)	Error (nm)	Uncertainty ± (nm)	k Factor
RM-HL	278.13	278.3	0.17	0.16	2.00
	361.25	361.3	0.05	0.16	2.00
	467.82	468.0	0.18	0.16	2.00
	536.56	536.6	0.04	0.16	2.00
	640.50	640.4	-0.10	0.16	2.00
RM-DL	740.09	740.0	-0.09	0.16	2.00
	864.94	865.0	0.06	0.16	2.00

UUC\* = Unit Under Calibration



Continuation of Calibration Certificate

**Cert. No. : SP23016**  
**Job No. : VC66SP0014**  
**Pages : 3 of 3**

**Result of calibration : Photometric Accuracy**

(Without adjustment)

Material	Wavelength (nm)	Filter S/N	Nominal Absorbance (A)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor
Neutral Density glass filter	440.0	29360	1.0	1.0517	1.0564	0.0047	0.0031	2.00
		29914	0.7	0.7445	0.7460	0.0015	0.0032	2.00
		29381	0.5	0.5416	0.5429	0.0013	0.0032	2.00
	546.1	29360	1.0	0.9821	0.9849	0.0028	0.0030	2.00
		29914	0.7	0.6961	0.6961	0.0000	0.0030	2.00
		29381	0.5	0.5073	0.5073	0.0000	0.0030	2.00
	590.0	29360	1.0	1.0222	1.0244	0.0022	0.0030	2.00
		29914	0.7	0.7237	0.7234	-0.0003	0.0030	2.00
		29381	0.5	0.5361	0.5360	-0.0001	0.0031	2.00
	635.0	29360	1.0	0.9753	0.9775	0.0022	0.0030	2.00
		29914	0.7	0.6910	0.6910	0.0000	0.0030	2.00
		29381	0.5	0.5211	0.5210	-0.0001	0.0032	2.00
Material	Wavelength (nm)	Solution (mg/l)	Certified Absorbance (A)	UUC* Reading Absorbance (A)	Error (A)	Uncertainty ± (A)	k Factor	
RM-0204060810	235.0	20	0.2422	0.2462	0.0040	0.0101	2.00	
		40	0.4866	0.4900	0.0034	0.0115	2.00	
		60	0.7414	0.7390	-0.0024	0.0068	2.00	
		80	0.9858	0.9871	0.0013	0.0093	2.00	
		100	1.2442	1.2480	0.0038	0.0087	2.00	

UUC\* = Unit Under Calibration

**Condition of this result of calibration : Spectrophotometer PERKINELMER Model Lambda 25 S/N 501S141230**

Resolution of Wavelength Mode 0.1 nm  
Resolution of Photometric Mode 0.0001 A  
Parameter Setting  
Measurement Mode Wavelength, Absorbance  
Wavelength Scan 1100 nm-190 nm  
Scanning Speed 7.5 nm/min  
Data Pitch 0.1 nm  
Band width(Wavelength) 1.0 nm  
Band width(Vis) 1.0 nm  
Band width(Uv) 1.0 nm

Stray Light** UUC* Reading at 220 nm	
Transmission T(%)	Absorbance(A)
0.0111	3.9564

\*\*Specific Acceptance :

Transmission  $\leq$  1.0 T(%), Absorbance  $\geq$  2.0 A

\*\*Stray light not TISI Accredited

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95%

**End of Calibration Certificate**



คุณภาพอากาศในสถานประกอบการ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B41	SKC	224-PCXR4	612669	05/01/2024	1,000	1,500	2,000	999	1,496	1,991	0.996x + 1.914	1.000
B42	SKC	224-PCXR4	626041	03/01/2024	1,000	1,500	2,000	1,004	1,498	1,991	0.986x + 19.248	1.000
B43	SKC	224-PCXR4	034636	03/01/2024	1,000	1,500	2,000	1,000	1,501	1,992	0.991x + 11.682	1.000
B44	SKC	224-PCXR8	529341	03/01/2024	1,000	1,500	2,000	1,002	1,502	2,002	1.004x – 6.860	1.000
B45	SKC	224-PCXR8	529594	03/01/2024	1,000	1,500	2,000	1,001	1,501	1,987	0.987x + 16.026	1.000
B46	SKC	224-PCXR8	566743	04/01/2024	1,000	1,500	2,000	995	1,506	2,002	1.013x – 27.915	0.999
B47	SKC	224-PCXR8	566747	04/01/2024	1,000	1,500	2,000	1,002	1,502	2,004	1.010x – 21.769	0.999
B48	SKC	224-PCXR8	566753	04/01/2024	1,000	1,500	2,000	1,000	1,493	1,998	0.997x + 0.239	1.000
B49	SKC	224-PCXR8	566780	04/01/2024	1,000	1,500	2,000	1,003	1,502	2,006	1.011x – 21.550	0.999
B50	SKC	224-PCXR8	500400	03/01/2024	1,000	1,500	2,000	1,001	1,496	2,002	1.001x – 2.900	1.000
B51	SKC	224-PCXR8	500363	03/01/2024	1,000	1,500	2,000	996	1,502	2,000	1.011x – 25.709	0.999
B52	SKC	224-PCXR8	093186	03/01/2024	1,000	1,500	2,000	994	1,496	1,992	0.995x + 1.751	1.000
B53	SKC	224-PCXR8	707670	05/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.008x – 16.042	0.999
B54	SKC	224-PCXR3	509821	05/01/2024	1,000	1,500	2,000	995	1,501	2,002	1.016x – 32.282	0.999
B55	SKC	224-PCXR3	510710	05/01/2024	1,000	1,500	2,000	1,004	1,495	1,992	0.991x + 7.666	1.000
B56	SKC	224-PCXR3	511450	05/01/2024	1,000	1,500	2,000	1,002	1,500	2,001	1.005x – 8.559	1.000
B57	SKC	224-PCXR3	510798	03/01/2024	1,000	1,500	2,000	997	1,492	1,999	0.999x – 2.122	1.000
B58	SKC	224-PCXR3	509852	03/01/2024	1,000	1,500	2,000	1,000	1,500	1,999	1.007x – 19.073	0.999
B59	SKC	224-PCXR3	509862	04/01/2024	1,000	1,500	2,000	995	1,503	1,995	0.998x + 2.118	1.000
B60	SKC	224-PCXR3	512655	04/01/2024	1,000	1,500	2,000	1,004	1,510	2,004	1.005x – 6.421	0.999
B61	SKC	224-PCXR3	503915	04/01/2024	1,000	1,500	2,000	993	1,492	1,999	1.003x – 11.706	1.000
B62	SKC	224-PCXR3	505975	03/01/2024	1,000	1,500	2,000	999	1,494	1,996	0.996x + 0.822	1.000
B63	SKC	224-PCXR3	511432	03/01/2024	1,000	1,500	2,000	990	1,501	2,000	1.017x – 36.259	0.999
B64	SKC	224-PCXR3	508302	03/01/2024	1,000	1,500	2,000	998	1,492	1,989	0.990x + 10.175	1.000
B65	SKC	224-PCXR3	508310	03/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.007x – 13.537	1.000
B66	SKC	224-PCXR3	509861	04/01/2024	1,000	1,500	2,000	1,002	1,491	1,992	0.988x + 13.744	1.000
B67	SKC	224-PCXR3	506295	04/01/2024	1,000	1,500	2,000	995	1,508	2,004	1.007x – 12.843	1.000
B68	SKC	224-PCXR3	505872	04/01/2024	1,000	1,500	2,000	1,002	1,491	1,998	0.995x + 4.040	1.000
B69	SKC	224-PCXR3	508375	04/01/2024	1,000	1,500	2,000	1,003	1,499	2,000	1.009x – 18.977	0.999
B70	SKC	224-PCXR3	510623	05/01/2024	1,000	1,500	2,000	992	1,493	1,996	1.002x – 7.730	1.000
B71	SKC	224-PCXR3	508367	05/01/2024	1,000	1,500	2,000	994	1,506	2,002	1.015x – 31.561	0.999
B72	SKC	224-PCXR3	505977	03/01/2024	1,000	1,500	2,000	1,003	1,499	1,994	0.991x + 9.042	1.000
B73	SKC	224-PCXR3	512606	04/01/2024	1,000	1,500	2,000	1,001	1,501	2,004	1.008x – 14.346	1.000
B74	SKC	224-PCXR3	505993	04/01/2024	1,000	1,500	2,000	996	1,497	1,995	1.001x – 7.036	1.000
B75	SKC	224-PCXR3	509820	05/01/2024	1,000	1,500	2,000	996	1,496	1,991	0.996x + 1.432	1.000
B76	SKC	224-PCXR3	509811	05/01/2024	1,000	1,500	2,000	993	1,499	1,999	1.006x – 14.283	1.000
B77	SKC	224-PCXR3	508301	05/01/2024	1,000	1,500	2,000	1,001	1,501	2,003	1.013x – 25.406	0.999
B78	SKC	224-PCXR3	510677	05/01/2024	1,000	1,500	2,000	995	1,503	1,999	1.012x – 27.520	0.999
B79	SKC	224-PCXR3	510920	05/01/2024	1,000	1,500	2,000	994	1,494	1,994	1.001x – 6.178	1.000

Calibrated by :

(Mr. Abdul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (ml/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)			y	R <sup>2</sup>
					1	2	3	1	2	3		
B80	SKC	224-PCXR3	504569	05/01/2024	1,000	1,500	2,000	1,002	1,498	2,002	1.012x - 24.186	0.999
B81	SKC	224-PCXR3	503480	05/01/2024	1,000	1,500	2,000	996	1,499	2,000	1.014x - 30.165	0.999
B82	SKC	224-PCXR3	505673	04/01/2024	1,000	1,500	2,000	994	1,498	1,996	1.000x - 4.746	1.000
B83	SKC	224-PCXR3	510785	04/01/2024	1,000	1,500	2,000	1,010	1,500	1,999	1.003x - 7.793	0.999
B84	SKC	224-PCXR3	508333	04/01/2024	1,000	1,500	2,000	997	1,498	1,991	0.993x + 4.810	1.000
B85	SKC	224-PCXR3	505757	05/01/2024	1,000	1,500	2,000	994	1,502	1,998	1.006x - 14.562	1.000
B86	SKC	224-PCXR3	512625	03/01/2024	1,000	1,500	2,000	1,015	1,503	2,004	0.999x + 3.063	0.999
B87	SKC	224-PCXR3	504324	03/01/2024	1,000	1,500	2,000	1,000	1,496	2,000	1.000x - 0.710	1.000
B88	SKC	224-PCXR3	508307	03/01/2024	1,000	1,500	2,000	995	1,498	1,993	0.997x + 0.574	1.000
B89	SKC	224-PCXR3	509860	03/01/2024	1,000	1,500	2,000	1,000	1,499	2,004	1.010x - 17.509	1.000
B90	SKC	224-PCXR3	508366	04/01/2024	1,000	1,500	2,000	995	1,508	2,000	1.005x - 10.091	1.000
B91	SKC	224-PCXR3	510919	04/01/2024	1,000	1,500	2,000	1,000	1,500	1,997	0.992x + 7.522	1.000
B92	SKC	224-PCXR3	510987	04/01/2024	1,000	1,500	2,000	1,002	1,501	1,999	0.999x + 1.097	1.000
B93	SKC	224-PCXR3	509845	04/01/2024	1,000	1,500	2,000	996	1,496	2,004	1.009x - 15.822	1.000
B94	SKC	224-PCXR8	A127871	05/01/2024	1,000	1,500	2,000	1,000	1,499	2,002	1.007x - 19.184	0.999
B95	SKC	224-PCXR8	A127921	05/01/2024	1,000	1,500	2,000	994	1,502	2,002	1.015x - 30.559	0.999
B96	SKC	224-PCXR8	A127942	04/01/2024	1,000	1,500	2,000	998	1,499	1,996	1.001x - 3.486	1.000
B97	SKC	224-PCXR8	A127955	05/01/2024	1,000	1,500	2,000	1,003	1,501	2,003	1.010x - 20.082	0.999
B98	SKC	224-PCXR8	A127956	05/01/2024	1,000	1,500	2,000	996	1,497	1,998	1.003x - 6.330	1.000

Calibrated by :

(Mr. Abdul Dangkrom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

### Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Environmental Conditions

Temperature : 25  $\pm$  3  $^{\circ}$ C  
Pressure : 1010  $\pm$  15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B41	SKC	224-PCXR4	612669	05/04/2024	1,000	1,500	2,000	1,001	1,498	1,990	0.994x + 6.342	1.000
B42	SKC	224-PCXR4	626041	04/04/2024	1,000	1,500	2,000	1,006	1,496	1,990	0.984x + 20.844	1.000
B43	SKC	224-PCXR4	034636	04/04/2024	1,000	1,500	2,000	998	1,498	1,989	0.989x + 12.360	1.000
B44	SKC	224-PCXR8	529341	09/04/2024	1,000	1,500	2,000	1,000	1,501	2,002	1.005x – 9.213	1.000
B45	SKC	224-PCXR8	529594	04/04/2024	1,000	1,500	2,000	1,002	1,502	1,989	0.988x + 16.584	1.000
B46	SKC	224-PCXR8	566743	04/04/2024	1,000	1,500	2,000	996	1,507	2,001	1.012x – 24.724	0.999
B47	SKC	224-PCXR8	566747	08/04/2024	1,000	1,500	2,000	1,005	1,500	2,002	1.007x – 16.424	0.999
B48	SKC	224-PCXR8	566753	09/04/2024	1,000	1,500	2,000	998	1,492	1,997	0.998x - 1.157	1.000
B49	SKC	224-PCXR8	566780	08/04/2024	1,000	1,500	2,000	1,004	1,503	2,005	1.009x – 18.040	0.999
B50	SKC	224-PCXR8	500400	04/04/2024	1,000	1,500	2,000	1,003	1,495	2,003	1.000x – 1.783	1.000
B51	SKC	224-PCXR8	500363	04/04/2024	1,000	1,500	2,000	995	1,500	2,002	1.013x – 28.701	0.999
B52	SKC	224-PCXR8	093186	04/04/2024	1,000	1,500	2,000	992	1,494	1,991	0.996x + 0.116	1.000
B53	SKC	224-PCXR8	707670	08/04/2024	1,000	1,500	2,000	1,000	1,502	2,001	1.009x – 16.999	0.999
B54	SKC	224-PCXR3	509821	08/04/2024	1,000	1,500	2,000	996	1,503	2,002	1.015x – 30.009	0.999
B55	SKC	224-PCXR3	510710	05/04/2024	1,000	1,500	2,000	1,000	1,494	1,993	0.995x + 0.965	1.000
B56	SKC	224-PCXR3	511450	09/04/2024	1,000	1,500	2,000	1,004	1,499	2,000	1.002x – 4.651	1.000
B57	SKC	224-PCXR3	510798	08/04/2024	1,000	1,500	2,000	996	1,494	1,998	1.000x – 2.680	1.000
B58	SKC	224-PCXR3	509852	08/04/2024	1,000	1,500	2,000	1,002	1,501	2,000	1.006x – 16.480	0.999
B59	SKC	224-PCXR3	509862	08/04/2024	1,000	1,500	2,000	997	1,501	1,998	0.999x + 1.041	1.000
B60	SKC	224-PCXR3	512655	05/04/2024	1,000	1,500	2,000	1,005	1,507	2,003	1.003x – 4.627	1.000
B61	SKC	224-PCXR3	503915	05/04/2024	1,000	1,500	2,000	993	1,490	2,000	1.004x – 12.823	1.000
B62	SKC	224-PCXR3	505975	05/04/2024	1,000	1,500	2,000	1,001	1,495	1,997	0.995x + 2.616	1.000
B63	SKC	224-PCXR3	511432	05/04/2024	1,000	1,500	2,000	993	1,503	1,999	1.014x – 30.715	0.999
B64	SKC	224-PCXR3	508302	08/04/2024	1,000	1,500	2,000	1,000	1,493	1,987	0.988x + 13.991	1.000
B65	SKC	224-PCXR3	508310	09/04/2024	1,000	1,500	2,000	1,003	1,500	2,003	1.006x – 12.021	1.000
B66	SKC	224-PCXR3	509861	08/04/2024	1,000	1,500	2,000	1,004	1,489	1,990	0.986x + 16.775	1.000
B67	SKC	224-PCXR3	506295	04/04/2024	1,000	1,500	2,000	997	1,506	2,003	1.004x – 9.094	1.000
B68	SKC	224-PCXR3	505872	04/04/2024	1,000	1,500	2,000	1,004	1,490	1,997	0.992x + 7.829	1.000
B69	SKC	224-PCXR3	508375	04/04/2024	1,000	1,500	2,000	1,005	1,500	1,998	1.006x – 13.832	0.999
B70	SKC	224-PCXR3	510623	08/04/2024	1,000	1,500	2,000	995	1,491	1,996	1.000x – 4.938	1.000
B71	SKC	224-PCXR3	508367	09/04/2024	1,000	1,500	2,000	996	1,504	2,000	1.012x – 27.572	0.999
B72	SKC	224-PCXR3	505977	09/04/2024	1,000	1,500	2,000	1,001	1,500	1,995	0.994x + 5.791	1.000
B73	SKC	224-PCXR3	512606	04/04/2024	1,000	1,500	2,000	1,002	1,499	2,002	1.007x – 12.671	1.000
B74	SKC	224-PCXR3	505993	04/04/2024	1,000	1,500	2,000	995	1,495	1,996	1.003x – 9.987	1.000
B75	SKC	224-PCXR3	509820	05/04/2024	1,000	1,500	2,000	998	1,497	1,993	0.997x + 1.432	1.000
B76	SKC	224-PCXR3	509811	05/04/2024	1,000	1,500	2,000	992	1,497	2,000	1.008x – 17.753	1.000
B77	SKC	224-PCXR3	508301	05/04/2024	1,000	1,500	2,000	1,004	1,499	2,001	1.010x – 19.743	0.999
B78	SKC	224-PCXR3	510677	08/04/2024	1,000	1,500	2,000	997	1,505	2,001	1.013x – 27.321	0.999
B79	SKC	224-PCXR3	510920	09/04/2024	1,000	1,500	2,000	995	1,495	1,993	1.000x – 4.702	1.000

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
**S.P.S. CONSULTING SERVICE CO., LTD.**  
 7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
 Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 ± 3 °C  
 Pressure : 1010 ± 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R <sup>2</sup>
B80	SKC	224-PCXR3	504569	09/04/2024	1,000	1,500	2,000	1,003	1,501	2,004	1.013x – 23.428	0.999
B81	SKC	224-PCXR3	503480	04/04/2024	1,000	1,500	2,000	998	1,499	2,003	1.015x – 30.384	0.999
B82	SKC	224-PCXR3	505673	04/04/2024	1,000	1,500	2,000	995	1,496	1,998	1.001x – 5.105	1.000
B83	SKC	224-PCXR3	510785	08/04/2024	1,000	1,500	2,000	1,012	1,499	2,000	1.002x – 7.135	0.999
B84	SKC	224-PCXR3	508333	08/04/2024	1,000	1,500	2,000	998	1,500	1,990	0.991x + 8.599	1.000
B85	SKC	224-PCXR3	505757	09/04/2024	1,000	1,500	2,000	993	1,503	2,000	1.008x – 16.396	1.000
B86	SKC	224-PCXR3	512625	04/04/2024	1,000	1,500	2,000	1,011	1,501	2,002	1.000x + 0.072	0.999
B87	SKC	224-PCXR3	504324	04/04/2024	1,000	1,500	2,000	998	1,495	2,001	1.003x – 4.738	1.000
B88	SKC	224-PCXR3	508307	08/04/2024	1,000	1,500	2,000	997	1,500	1,994	0.996x + 3.047	1.000
B89	SKC	224-PCXR3	509860	04/04/2024	1,000	1,500	2,000	1,001	1,501	2,006	1.011x – 17.174	1.000
B90	SKC	224-PCXR3	508366	08/04/2024	1,000	1,500	2,000	997	1,510	2,001	1.004x – 8.814	1.000
B91	SKC	224-PCXR3	510919	04/04/2024	1,000	1,500	2,000	1,001	1,502	1,998	0.993x + 7.522	1.000
B92	SKC	224-PCXR3	510987	04/04/2024	1,000	1,500	2,000	1,000	1,504	2,000	1.001x - 0.858	1.000
B93	SKC	224-PCXR3	509845	08/04/2024	1,000	1,500	2,000	998	1,495	2,003	1.007x – 13.389	1.000
B94	SKC	224-PCXR8	A127871	08/04/2024	1,000	1,500	2,000	1,001	1,501	2,004	1.008x – 19.942	0.999
B95	SKC	224-PCXR8	A127921	08/04/2024	1,000	1,500	2,000	996	1,504	2,005	1.016x – 31.417	0.999
B96	SKC	224-PCXR8	A127942	08/04/2024	1,000	1,500	2,000	999	1,500	2,000	1.003x – 5.715	1.000
B97	SKC	224-PCXR8	A127955	08/04/2024	1,000	1,500	2,000	1,004	1,502	2,005	1.011x – 20.122	0.999
B98	SKC	224-PCXR8	A127956	08/04/2024	1,000	1,500	2,000	995	1,496	2,000	1.004x – 9.122	1.000

Calibrated by :

(Mr. Abdul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
H-B01	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	506.5	991.1	1974.3	0.989x + 9.286	1.000
H-B02	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	496.7	997.6	1996.1	0.994x + 4.509	1.000
H-B03	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	497.6	988.8	2009.6	1.004x - 14.177	0.999
H-B04	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	501.6	998.7	2006.5	0.997x - 0.777	1.000
H-B05	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	500.4	997.3	1974.3	0.980x + 21.602	0.999
H-B06	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	504.9	994.8	1984.0	1.003x - 5.213	1.000
H-B07	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	502.6	990.6	2016.7	1.001x - 0.998	1.000
H-B08	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	499.7	998.7	1979.8	0.996x + 3.580	0.999
H-B09	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	504.1	1004.3	2010.7	0.993x + 13.998	1.000
H-B10	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	496.2	999.3	2009.2	0.996x + 3.860	1.000

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

### Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

#### Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)			y	R <sup>2</sup>
				1	2	3	1	2	3		
H-B01	Dwyer	VFB-65	08/04/2024	500	1,000	2,000	504.3	992.1	1976.8	0.991x + 6.353	1.000
H-B02	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	496.5	998.8	1996.7	0.995x + 4.247	1.000
H-B03	Dwyer	VFB-65	05/04/2024	500	1,000	2,000	498.6	991.4	2011.0	1.003x - 12.161	0.999
H-B04	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	501.4	1000.9	2008.3	0.998x - 1.566	1.000
H-B05	Dwyer	VFB-65	08/04/2024	500	1,000	2,000	502.9	999.5	1974.5	0.979x + 24.520	0.999
H-B06	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	504.7	996.0	1984.4	1.005x - 6.145	1.000
H-B07	Dwyer	VFB-65	05/04/2024	500	1,000	2,000	502.2	992.8	2017.1	1.000x - 0.160	1.000
H-B08	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	500.3	1000.7	1980.2	0.995x + 5.203	0.999
H-B09	Dwyer	VFB-65	09/04/2024	500	1,000	2,000	503.3	1005.0	2011.1	0.994x + 13.348	1.000
H-B10	Dwyer	VFB-65	08/04/2024	500	1,000	2,000	498.2	1001.7	2008.8	0.995x + 5.854	1.000

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Comprehensive Calibration Data Report - Q1 2024											
Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
L-B01	Dwyer	VFA-21	04/01/2024	50	100	200	50.7	98.5	198.9	0.986x + 0.884	1.000
L-B02	Dwyer	VFA-21	04/01/2024	50	100	200	50.6	99.2	198.7	0.997x + 0.603	0.999
L-B03	Dwyer	VFA-21	04/01/2024	50	100	200	50.1	99.2	198.3	1.010x - 1.750	1.000
L-B04	Dwyer	VFA-21	03/01/2024	50	100	200	49.2	102.0	200.5	1.011x - 0.502	1.000
L-B05	Dwyer	VFA-21	05/01/2024	50	100	200	50.5	99.4	200.8	0.999x + 0.948	0.999
L-B06	Dwyer	VFA-21	05/01/2024	50	100	200	50.5	99.0	202.3	1.010x - 0.360	1.000
L-B07	Dwyer	VFA-21	03/01/2024	50	100	200	49.5	100.3	200.1	1.013x - 1.486	1.000
L-B08	Dwyer	VFA-21	04/01/2024	50	100	200	50.7	101.2	199.3	1.000x + 0.298	1.000
L-B09	Dwyer	VFA-21	04/01/2024	50	100	200	50.5	99.0	200.2	0.992x + 1.365	1.000
L-B10	Dwyer	VFA-21	03/01/2024	50	100	200	50.7	98.5	203.2	0.998x + 1.334	0.999

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72. Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Comprehensive Calibration Data Report - Q1 2024											
Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R <sup>2</sup>
L-B01	Dwyer	VFA-21	08/04/2024	50	100	200	50.7	98.8	199.3	0.987x + 1.039	1.000
L-B02	Dwyer	VFA-21	04/04/2024	50	100	200	50.2	98.8	198.3	0.998x + 0.180	0.999
L-B03	Dwyer	VFA-21	05/04/2024	50	100	200	50.5	98.8	197.9	1.012x - 1.915	1.000
L-B04	Dwyer	VFA-21	04/04/2024	50	100	200	49.8	101.6	201.9	1.010x - 0.036	1.000
L-B05	Dwyer	VFA-21	08/04/2024	50	100	200	50.9	99.0	201.2	0.998x + 0.999	1.000
L-B06	Dwyer	VFA-21	04/04/2024	50	100	200	50.1	99.4	202.7	1.011x - 0.423	1.000
L-B07	Dwyer	VFA-21	05/04/2024	50	100	200	50.3	99.9	200.5	1.009x - 0.861	1.000
L-B08	Dwyer	VFA-21	04/04/2024	50	100	200	50.6	100.8	198.9	1.002x - 0.189	1.000
L-B09	Dwyer	VFA-21	09/04/2024	50	100	200	50.1	99.4	200.6	0.997x + 0.731	1.000
L-B10	Dwyer	VFA-21	08/04/2024	50	100	200	51.0	98.9	202.8	0.996x + 1.709	0.999

Calibrated by :

  
(Mr. Adut Dangtom)

Approved by :

  
(Mr. Peera Detudom)

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 23M2441

REFERENCE No : 68471-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905


**ID No** : BA 05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 10-Mar-23

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 16-Mar-23

**RECEIVED DATE** : 10-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 23M2441

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA 05/50 RECEIVED DATE : 10-Mar-23  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 10-Mar-23  
AMBIENT TEMPERATURE : 23°C  $\pm$  1°C RELATIVE HUMIDITY : 49 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000039
0.02	0.02000	0.00000	0.000039
0.10	0.10000	0.00000	0.000039
0.20	0.20001	-0.00001	0.000040
0.50	0.50001	-0.00001	0.000040
1.00	1.00000	0.00000	0.000041
2.00	2.00003	-0.00003	0.000042
5.00	5.00001	-0.00001	0.000046
10.00	10.00003	-0.00003	0.000053
20.00	20.00005	-0.00005	0.000067
50.00	50.00001	-0.00001	0.00011
100.00	100.00001	-0.00001	0.00019
200.00	200.00001	-0.00001	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0001
3	50.0000
4	50.0000
5	49.9999
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY  
COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 24M2227

REFERENCE No : 72448-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905

**ID No** : BA05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 08-Mar-24

**APPROVED BY** :   
PONGSAK J.

**ISSUED DATE** : 14-Mar-24

**RECEIVED DATE** : 08-Mar-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.





CERTIFICATE No : 24M2227

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA05/50 RECEIVED DATE : 08-Mar-24  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 08-Mar-24  
AMBIENT TEMPERATURE : 25° C  $\pm$  1° C RELATIVE HUMIDITY : 53 %RH  $\pm$  10 % RH

### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02001	-0.00001	0.000065
0.10	0.10002	-0.00002	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	9.99994	0.00006	0.000070
20.00	20.00008	-0.00008	0.000078
50.00	50.0000	0.0000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0001	-0.0001	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





## Certificate of Calibration

**Aquion : Anion (ID#894)**

This certificate is to verify that instrument below are calibrated  
by Archemica Lab Co.,Ltd.

AQUION S/N : 190840059

AS-DV S/N : 190915235

for

**S.P.S. Consulting Service Co., Ltd.**



Operator Signature : \_\_\_\_\_

Date : Jul 3, 2023

(Mr.Nutdanai Laekhwan)

Applications Chemist



ระดับเสียงในสถานประกอบการ

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

## CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.  
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.  
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.  
4. Digital Multimeter Agilent 34401A S/N MY44005560.  
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.  
6. Audio Analyzer Keithley 2015-P S/N 4106495.  
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 27 Mar. 2023

Date of Calibration : 29 Mar. 2023

1 /

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.94	-0.06	$\pm 0.10$	$\pm 0.40$ dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	$\pm 1.5$	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	$\pm 0.50$	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

[Redacted Signature]

(Mr. Weerachai Deechaiyae)

Approved by :

[Redacted Signature]

(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 29 Mar. 2023

Date of Issue : 30 Mar. 2023

Ref : 2011266032701228001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com., www.spscon.com

Noise B\_043\_1/24

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	29 March 2023
		Due Date	29 March 2024

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B18	ACO	6236	00172048	24 February 2024	93.9	94.0
ACO-B29	ACO	6236	00182011	24 February 2024	94.0	94.0
ACO-B33	ACO	6236	00182015	24 February 2024	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.94 ± 0.10 dB	

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)





THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

**Request No.** 21-67/0304

**MTC No.** EEL. BP. 109/0267

## CALIBRATION CERTIFICATE

**Submitted by** : S.P.S.Consulting Service Co.,Ltd.

**Address** : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

**Calibrated at** : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

**Instrument Calibrated :**

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

**Ambient Environment**

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

**Standards used :**

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N4106495.
7. Condenser Microphone B&K 4180 S/N 2889871.

**Calibration Procedure:** CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

**Date of Receipt** : 22 Feb. 2024

**Date of Calibration** : 4 Mar. 2024

1 / 1

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th



Request No. 21-67/0304

MTC No. EEL. BP. 109/0267

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	93.85	-0.15	$\pm 0.10$	$\pm 0.75$ dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	$\pm 1.5$	$\pm 2.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1.65	$\pm 0.50$	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.


3. The microphone volume correction was not included.

Calibrated by :



(Mr. Weerachai Deechaiyae)

Approved by :



(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 4 Mar. 2024

Date of Issue : 5 Mar. 2024

Ref : 2011267022200795001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise B\_158/24

## Sound Level Meter Calibration Report

### Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	04 March 2024
		Due Date	04 March 2025

### Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B36	ACO	6236	00192027	12 May 2024	94.1	93.9
ACO-B41	ACO	6236	00192032	12 May 2024	93.9	93.9
ACO-B43	ACO	6236	00192034	12 May 2024	93.9	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.85 ± 0.10 dB	

Calibrated by :

(Mr. Adul Dangklorn)

Approved by :

(Mr. Peera Detudom)