


ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือที่ใช้ในการตรวจวิเคราะห์  
(Calibration)

THE UNIVERSITY OF CHICAGO

PH.D. THESIS

THE UNIVERSITY OF CHICAGO




Thai Environmental Technic Limited  
บริษัท เทคนิกสิ่งแวดล้อมไทย จำกัด

ตารางการสอบเทียบเครื่องมือที่ใช้ในการตรวจวัดและวิเคราะห์

Item	Description	Parameter	List of Equipment	Equipment No.	Calibration Date	Next Calibration
1.	Stack Air	Particulate	Dry Gas Method/SK25EX	S/N 1317	07/02/2024	February 2025
			Digital Barometer/PHB-318	S/N B11409	08/05/2023	May 2024
			Digital Thermometer/DP-52	S/N L210094	27/10-06/11/2023	October 2024
		NO <sub>x</sub> as NO <sub>2</sub> , SO <sub>2</sub>	Electronic Balance/METTLER TOLEDO	S/N 1116392227	11/04/2023	April 2024
			Gas Analyzer (E-instrument)/4400-S	S/N 6159	03/01/2024	January 2025
	Ambient Air	Cu	Dry Gas Method/SK25EX	S/N 1317	07/02/2024	February 2025
			Digital Barometer/PHB-318	S/N B11409	08/05/2023	May 2024
			Digital Thermometer/DP-52	S/N L210094	27/10-06/11/2023	October 2024
			Atomic Absorption Spectrophotometer	S/N 04050110503	28/03/2024	September 2024
			PerkinElmer/AAAnalyst 100			
2.	Ambient Air	CO, O <sub>2</sub> Orifice TSP	Gas Analyzer (E-instrument)/4400-S	S/N 6159	03/01/2024	January 2025
			ORIFICE TRANSFER STANDARD/Tisch	S/N 0068	21/09/2022	September 2023
			High Volume Air Sampler/TET	S/N TSP-03	04/07/2023	July 2024
			High Volume Air Sampler/TET	S/N TSP-35	11/07/2023	July 2024
			High Volume Air Sampler/TET	S/N TSP-32	05/07/2023	July 2024
	Ambient Air	Orifice PM-10	High Volume Air Sampler/TET	S/N TSP-37	13/07/2023	July 2024
			Electronic Balance/METTLER TOLEDO	S/N 1116392227	11/04/2023	April 2024
			ORIFICE TRANSFER STANDARD/Tisch	S/N 0068	21/09/2022	September 2023
			High Volume Air Sampler/TET	S/N PM10-09	05/07/2023	July 2024
			High Volume Air Sampler/TET	S/N PM10-20	13/07/2023	July 2024
	Ambient Air	Orifice PM-10	High Volume Air Sampler/TET	S/N PM10-19	13/07/2023	July 2024
			High Volume Air Sampler/TET	S/N PM10-23	05/07/2023	July 2024
			Electronic Balance/METTLER TOLEDO	S/N 1116392227	11/04/2023	April 2024






Thai Environmental Technic Limited  
บริษัท เทคนิสิ่งแวดล้อมไทย จำกัด

ตารางการสอบเทียบเครื่องมือที่ใช้ในการตรวจวัดและวิเคราะห์

Item	Description	Parameter	List of Equipment	Equipment No.	Calibration Date	Next Calibration
2.	Ambient Air (Cont.)	Orifice  Cu	ORIFICE TRANSFER STANDARD/Tisch	S/N 0068	21/09/2022	September 2023
			High Volume Air Sampler/TET	S/N TSP-03	04/07/2023	July 2024
			High Volume Air Sampler/TET	S/N TSP-35	11/07/2023	July 2024
			High Volume Air Sampler/TET	S/N TSP-32	05/07/2023	July 2024
			High Volume Air Sampler/TET	S/N TSP-37	13/07/2023	July 2024
	NO <sub>2</sub>		Atomic Absorption Spectrophotometer	S/N 040S0110503	28/03/2024	September 2024
			PerkinElmer/AAAnalyst 100			
			Certificate of Analysis Linde	S/N A00917SK	05/07/2023	July 2026
			NO <sub>x</sub> Analyzer/API 200E	S/N 481	09/11/2023	May 2024
			NO <sub>x</sub> Analyzer/Teledyne T200	S/N 5158	10/11/2023	May 2024
			NO <sub>x</sub> Analyzer/Teledyne 200A	S/N 1982	09/11/2023	May 2024
			NO <sub>x</sub> Analyzer/Teledyne 200E	S/N 2789	10/11/2023	May 2024
			Certificate of Analysis Linde	S/N D636157	18/09/2023	September 2027
			SO <sub>2</sub> Analyzer/Thermo 43C	S/N 43C73374373	06/11/2023	May 2024
			SO <sub>2</sub> Analyzer/API 100E	S/N 1341	09/11/2023	May 2024
	SO <sub>2</sub>		SO <sub>2</sub> Analyzer/API 100E	S/N 383	07/11/2023	May 2024
			SO <sub>2</sub> Analyzer/Thermo 43C	S/N 43C55175302	06/11/2023	May 2024
			Wind speed and wind direction/Weather Wizard III	S/N WC21014A92	17/01/2024	January 2025
			Wind speed and wind direction/Weather Wizard II	S/N WC80609A09	24/10/2023	October 2024
			Wind speed and wind direction/Weather Wizard III	S/N WE61121A25A	13/09/2023	September 2024
	WS & WD		Wind speed and wind direction/Weather Wizard II	S/N WC40105A43	21/06/2023	June 2024






Thai Environmental Technic Limited  
บริษัท เทคโนโลยีสิ่งแวดล้อมไทย จำกัด

ตารางการสอบเทียบเครื่องมือที่ใช้ในการตรวจวัดและวิเคราะห์

Item	Description	Parameter	List of Equipment	Equipment No.	Calibration Date	Next Calibration
3.	Working Air	Total Dust	Personal Air Sampler/Gilian	S/N 20120103081	14/03/2024	April 2024
			Personal Air Sampler/Gilian	S/N 20110505116	14/03/2024	April 2024
		Respirable Dust	Electronic Balance/XP 205	S/N 1129273885	11/04/2023	April 2024
			Personal Air Sampler/Gilian	S/N 20140505103	14/03/2024	April 2024
4.	Sound Level	Cu Fume	Electronic Balance/XP 205	S/N 1129273885	11/04/2023	April 2024
			Personal Air Sampler/Gilian	S/N 20120202031	14/03/2024	April 2024
		Cu Dust	Atomic Absorption Spectrophotometer Model/AAAnalyst 100	S/N 040S0110503	28/03/2024	September 2024
			Personal Air Sampler/Gilian	S/N 20120202045	14/03/2024	April 2024
		IPA	Atomic Absorption Spectrophotometer Model/AAAnalyst 100	S/N 040S0110503	28/03/2024	September 2024
			Personal Air Sampler/Gilian	S/N 20111001074	14/03/2024	April 2024
		CO	Gas Chromatograph/GC7890B	S/N CN16343040	25/09/2023	September 2024
			Gas Detector/BW Technologies	S/N J617-M027776	29/01/2024	January 2025
		Calibrator	Sound Level Calibrator/ST-120	S/N ST120C0263E	21/12/2023	December 2024
			Integrated Sound Level/ST-11D	S/N 820393	14/12/2023	December 2024
		& เสียงรบกวน	Integrated Sound Level/ST-11D	S/N 821293	04/01/2024	January 2025
			Integrated Sound Level/ST-11D	S/N 821294	04/01/2024	January 2025
			Integrated Sound Level/ST-11D	S/N 821298	04/01/2024	January 2025
			Integrated Sound Level/ST-11D	S/N 821299	04/01/2024	January 2025
			Integrated Sound Level/ST-11D	S/N 820877	30/01/2024	January 2025
			Integrated Sound Level/ST-11D	S/N 820878	30/01/2024	January 2025
			Integrated Sound Level/ST-11D	S/N 821294	04/01/2024	January 2025
			Integrated Sound Level/ST-11D	S/N 821295	04/01/2024	January 2025
Integrated Sound Level/ST-11D	S/N 820394		14/12/2023	December 2024		







Thai Environmental Technic Limited  
บริษัท เทคโนโลยีสิ่งแวดล้อมไทย จำกัด

ตารางการสอบเทียบเครื่องมือที่ใช้ในการตรวจวัดและวิเคราะห์

Item	Description	Parameter	List of Equipment	Equipment No.	Calibration Date	Next Calibration
5.	Occupational Safety and Health	Noise Contour	Sound Level Calibrator/TENMAR TM-100	S/N 180501628	16/08/2023	August 2024
			Integrated Sound Level/ACO TYPE 6236	S/N 222036	01/03/2024	31/03/2024
			Integrated Sound Level/ACO TYPE 6236	S/N 222037	01/03/2024	31/03/2024
			Integrated Sound Level/ACO TYPE 6226	S/N 100099	01/04/2024	30/04/2024
			Integrated Sound Level/ACO TYPE 6236	S/N 152074	01/04/2024	30/04/2024
			Integrated Sound Level/ACO TYPE 6236	S/N 222038	01/04/2024	30/04/2024
			Integrated Sound Level/ACO TYPE 6236	S/N 222040	01/04/2024	30/04/2024
			Noise Dose Meter/SOUNDTEK ST-130	S/N 200300134	23/02/2024	February 2025
6.	Water	Noise Dose	Noise Dose Meter/SOUNDTEK ST-130	S/N 220100050	15/02/2024	February 2025
			Noise Dose Meter/SOUNDTEK ST-130	S/N 220100051	15/02/2024	February 2025
			Liquid in Glass Thermometer	S/N 2197259	15/02/2024	February 2025
		Heat	Liquid in Glass Thermometer	S/N 2197260	15/02/2024	February 2025
			Liquid in Glass Thermometer	S/N 2197261	15/02/2024	February 2025
			Liquid in Glass Thermometer	S/N 2197262	15/02/2024	February 2025
			Liquid in Glass Thermometer	S/N 2197263	15/02/2024	February 2025
			Liquid in Glass Thermometer	S/N 2197264	15/02/2024	February 2025
			pH Meter/Horiba F-71G	S/N V381F8H3	31/10/2023	October 2024
		pH	pH Meter (Temperature)/Horiba F-71G	S/N V381F8H3	31/10/2023	October 2024
			Electronic Balance/METTLER TOLEDO	S/N 1116392227	10/04/2024	April 2025
			Electronic Balance/METTLER TOLEDO	S/N 1116392227	10/04/2024	April 2025
		H <sub>2</sub> S	Spectrophotometer/PerkinElmer	S/N 365K9042909	18/08/2023	August 2024
			Electronic Balance/METTLER TOLEDO	S/N 1116392227	10/04/2024	April 2025
			BOD Incubator/Model i250-DS	S/N 2059-1017-0029	29/06/2023	June 2024
		Oil & Grease	DO Meter/HORIBA	S/N D75J0012	09/02/2024	February 2025
			ICP394/PerkinElmer/OPTIMA8000	S/N 078N1310024C	28/03/2024	September 2024
			ICP394/PerkinElmer/OPTIMA8000	S/N 078N1310024C	28/03/2024	September 2024





THAI ENVIRONMENTAL TECHNIC LIMITED  
บริษัท เทคโนโลยีสิ่งแวดล้อมไทย จำกัด

## CONTROL UNIT CALIBRATION

( Metric units , mm )

Date **7-Feb-24**

	Initial	Final	Average	
Barometric press, Pb	759.2	759.5	759.4	mmHg

### Dry Gas Meter Data

Console No. **M50-07**

Metering System ID

DGM Number **1317**

DGM Model **SK25EX**

### Reference Dry Gas Meter Data

Serial No. **913428**

Model. **S-110**

Correction factor(Yr) **1.0209**

Last Calibration Data **26-May-23**

Orifice manometer setting $\Delta H$ mm H2O	Ref .	DGM	Temperature ( $^{\circ}$ C )				Time min	DGM Correction factor (Y)	$\Delta H@$ mm H <sub>2</sub> O
	DMG	Volume	Ref DGM	Dry Gas Meter					
	Volume $V_r$ Liters	$V_m$ Liters		Inlet $T_i$	Outlet $T_o$	Avg $T_m$			
			$T_r$						
15.00	100.00	99.80	29.00	29.10	29.30	29.20	8.36	1.0221	46.2103
25.00	100.00	99.20	29.00	29.10	29.30	29.20	6.49	1.0273	46.4605
50.00	100.00	99.50	29.00	29.10	29.30	29.20	4.58	1.0218	46.3877
80.00	100.00	99.10	29.00	29.10	29.30	29.20	3.59	1.0229	45.7335
100.00	100.00	99.30	29.00	29.10	29.30	29.20	3.23	1.0189	46.3655

Average **1.0226** **46.2315**

Dued Date of Calibrate **6-Feb-25**

Calibrated by

Approved :

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is  $\pm 0.02$ .

Note: For  $\Delta H@$ , Orifice pressure differential that equates to  $0.75 \text{ cfm}$  ( $0.0212 \text{ m}^3/\text{min}$ ) at standard temperature and pressure, acceptable tolerance of individual values from the average is  $\pm 0.2 \text{ inches}$  ( $5.1 \text{ mm}$ )  $H_{20}$ .





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23P1365

Page : 1 of 2

Equipment : Barometer

Manufacturer: Lutron

Model : PHB-318

Serial No.: B011409

ID No.: 3

Condition As-Received: Used Item

Received Date: 25 April 2023

Calibration Date: 08 May 2023

Reference: 2304-0600DSC

Submitted by: Thai Environmental Technic Limited

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1011 mbar

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung,  
Bangkok 10240

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Digital Manometer	767367	91R724799	23P1270	25 Apr 2024

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 7.50062 mmHg

4.This result of calibration instrument was in absolute pressure.

5.This instrument was used clean air as pressure media.

6.This instrument was installed in vertical orientation and center of the device was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Suwit Aussarree

Issue Date : 09 May 2023

Approved Signatory :

[ ] Sura Suwannasri

[x] Attapol Panurach

B 0314103



Cert.No.: 23P1365

Page: 2 of 2

**Result of calibration:- Without adjustment**

**Range :** 730 mmHg to 770 mmHg

**Function:- Absolute Pressure Measurement**

**Resolution :** 0.1 mmHg

**Increasing Pressure**

Applied Pressure (mmHg)	730.85	740.85	750.85	760.85	770.85
UUC* Indication (mmHg)	730.2	740.2	750.2	760.2	770.2
Error (mmHg)	-0.65	-0.65	-0.65	-0.65	-0.65

**Decreasing Pressure**

Applied Pressure (mmHg)	770.85	760.85	750.85	740.85	730.85
UUC* Indication (mmHg)	770.2	760.2	750.2	740.2	730.2
Error (mmHg)	-0.65	-0.65	-0.65	-0.65	-0.65

The uncertainty of measurement was  $\pm 0.27$  mmHg

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

a 1160425



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23T1980

Page : 1 of 2

Equipment : Digital Thermometer With Sensor

Manufacturer: Digicon

Model : DP-52

Serial No.: I.210094

ID No.: NO.5

Condition As-Received: Used Item

Received Date: 17 October 2023

Calibration Date: 27 October 2023  
to 06 November 2023

Reference: 2310-0561DSC

Submitted by: Thai Environmental Technic Limited

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung,  
Bangkok 10240

**Procedure used:** Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller and comparison with Standard Thermocouple (Type R/S) into high temperature furnace.  
The temperature scale used was based on ITS-90.

### Condition of this result of calibration

#### 1. Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Black Stack Thermometer	1560	8C454	23I600	30 May 2024
2) PRT Scanner Module	2562	A01303	23I600	30 May 2024
3) Industrial Platinum Resistance Thermometer	5627	739433	23I600	30 May 2024
4) Digital Thermometer	1529	A4B760	23I1123	21 Sep 2024
5) Industrial Platinum Resistance Thermometer	5627	824302	23I1123	21 Sep 2024
6) Digital Multimeter	DMM6500	4576227	E1U230074	11 Jan 2024
7) Standard Thermocouple Probe (Type S)	TCS	TCS-001	TT-0165-22	15 Dec 2023

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008
- NA Caltechnologies Co., Ltd., ANAB Accredited No. Calibration AC-2658
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Theerapong Ameen  
Issue Date : 08 November 2023

Approved Signatory :

[ ] P  
[x] Chatchawan Khunpiuek  
[ ] Wanlop Larpkern

B 0327784



Cert. No.: 23T1980

Page.: 2 of 2

**Result of Calibration:-**

Without Adjustment

**Function:**

Temperature measurement for Channel T1

This equipment was connected with Thermocouple Type K ID No. No.5

Dimension of probe : Diameter 8 mm, Length 1030 mm. Sheath material : Stainless Steel

Immersion Depth ( mm.)	Standard Temperature ( °C )	UUC* Reading ( °C )	Error ( °C )	Uncertainty of Measurement ( ± °C )
180	200.0009	200.0	-0.0009	0.74
180	400.0032	400.1	0.0968	1.4
180	599.92	601.3	1.38	3.1

**UUC\* : Unit Under Calibration**

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

-o0o-

a 1188568





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23P1365

Page : 1 of 2

Equipment : Barometer

Manufacturer: Lutron

Model : PHB-318

Serial No.: B011409

ID No.: 3

Condition As-Received: Used Item

Received Date: 25 April 2023

Calibration Date: 08 May 2023

Reference: 2304-0600DSC

Submitted by: Thai Environmental Technic Limited

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1011 mbar

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphan Sung,  
Bangkok 10240

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Digital Manometer	767367	91R724799	23P1270	25 Apr 2024

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 7.50062 mmHg

4.This result of calibration instrument was in absolute pressure.

5.This instrument was used clean air as pressure media.

6.This instrument was installed in vertical orientation and center of the device was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Suwit Aussarree

Issue Date : 09 May 2023

Approved Signatory :

[ ] Sura Suwannasri

[x] Attapol Panurach

B 0314103



Cert.No.: 23P1365

Page: 2 of 2

**Result of calibration:- Without adjustment**

**Range :** 730 mmHg to 770 mmHg

**Function:- Absolute Pressure Measurement**

**Resolution :** 0.1 mmHg

**Increasing Pressure**

Applied Pressure (mmHg)	730.85	740.85	750.85	760.85	770.85
UUC* Indication (mmHg)	730.2	740.2	750.2	760.2	770.2
Error (mmHg)	-0.65	-0.65	-0.65	-0.65	-0.65

**Decreasing Pressure**

Applied Pressure (mmHg)	770.85	760.85	750.85	740.85	730.85
UUC* Indication (mmHg)	770.2	760.2	750.2	740.2	730.2
Error (mmHg)	-0.65	-0.65	-0.65	-0.65	-0.65

The uncertainty of measurement was  $\pm 0.27$  mmHg

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o-o-

Attapol P.

a 1160425



Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## Portable Gas Calibration Report

Manufacturer: E-instruments  
Instrument Model: 4400S  
Instrument serial no.: 6159  
Instrument ID: 7

Date of Calibration: 3-Jan-24  
Ambient Condition  
Temperature (23±5 °C): 25.0 °C  
Humidity (55±15 % RH): 50.0 % RH  
Barometer (mmHg): 758.7 mmHg

## Standard gas References

Standard gas	Cylinder No.	Traceability	Due date
Oxygen (O <sub>2</sub> )	36232	Linde	June 26, 2031
Nitric Oxide(NO)	D824463	Linde	June 5, 2026
	D824524	Linde	August 22, 2025
Sulfer Dioxide (SO <sub>2</sub> )	D824500	Linde	October 11, 2024
	D271305	Linde	October 11, 2024
Carbon Monoxide(CO)	D824500	Linde	October 11, 2024
	D271305	Linde	October 11, 2024

## Calibration Results

Parameter	Standard gas	Reading	Actual Error	Test Limit	Results
O <sub>2</sub> (%vol)	0.0	0.0	0.0	±0.2 % vol	PASS
	14.0	14.0	0.0		
NO (ppm)	0.0	0.0	0.0	±5.0 ppm 0...100 ppm ±5% measured Value 101....5000 ppm	PASS
	198.0	199.0	1.0		
	392.0	393.0	1.0		
SO <sub>2</sub> (ppm)	0.0	0.0	0.0		PASS
	406.0	404.0	-2.0		
	804.0	803.0	-1.0		
CO (ppm)	0.0	0.0	0.0		PASS
	404.0	405.0	1.0		
	793.0	795.0	2.0		

Calibrate by:



Approved by :







## MAINTENANCE REPORT

### ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

AAAnalyst 100

<b>Customer :</b>	บริษัท เทคนิควัดแล้งไทย จำกัด	<b>Date Tested:</b>	28-มี.ค.-67
<b>Address :</b>	1/6 ซอยรามคำแหง 145, แขวงสะพานสูง, เขตสะพานสูง, กรุงเทพฯ 10240 TH	<b>Recommendation Recertification Period</b>	6 Months
<b>User Name:</b>	คุณ กิตติศักดิ์ เมืองงาม	<b>Recertification Due:</b>	27-ก.ย.-67
<b>Phone:</b>	02-3737799	<b>Date Last Certified:</b>	29-ก.ย.-66
<b>E-mail:</b>	phorntip.p@tet1995.com	<b>Visit Number:</b>	1 of 2
	Ketsarin.Chuayphin@eurofinsasia.com	<b>TH ONE SOURCE Phone:</b>	081-7316733, 082-1086572
		<b>E-mail:</b>	thonesource@gmail.com

CONFIGURATION TESTED		
MODEL	SERIAL NUMBER	SOFTWARE
AAAnalyst 100	040S0110503	AA WinLab 3.2
TEST STANDARD USED	PART NUMBER	
Copper	N9300183	
Filter 0.2 %	MG0-057	



# MAINTENANCE REPORT

## ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

### AAAnalyst 100

**SERIAL NUMBER**     040S0110503
**DATE TESTED**     28-มี.ค.-67
**1. OPTIC CHECKS**

A. Optical alignment condition (if necessary)

☐ OK

B. Condition of Mirrors,Lenses etc.(if necessary)

☐ OK

C. D2,HCL beam adjust (if necessary)

☐
**2. GAS SYSTEM CHECKS**

A. Leak test all internal and extenal gas box joints

☐ OK

B. All gas box safety features

☐ OK

C. Burner system including nebulizer and all o-ring and gasket

☐ OK

D. Drain system ( safety )

☐ F

**3. ELECTRONICS CHECKS**

A. Power Supplies

 + 5.00 Vdc  $\pm$  0.2 Vdc

+ 5.02 Vdc

 + 11.50 Vdc  $\pm$  0.2 Vdc

+ 11.46 Vdc

 + 15.00 Vdc  $\pm$  1.0 Vdc

+14.99 Vdc

 - 15.00 Vdc  $\pm$  1.0 Vdc

-15.06 Vdc

 + 35.00 Vdc  $\pm$  3.0 Vdc

+35.13 Vdc

**4. WAVELENGTH ACCURACY TEST**

 A. Zn Lamp wavelength 213.9 nm  $\pm$  0.3 nm.

214.08 nm.

 B. Fe Lamp wavelength 248.3 nm  $\pm$  0.3 nm.

248.24 nm.

 C. Cu Lamp wavelength 324.8 nm  $\pm$  0.3 nm.

324.82 nm.



# MAINTENANCE REPORT

## ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

### AAAnalyst 100

<b>SERIAL NUMBER</b> <u>040S0110503</u>	<b>DATE TESTED</b> <u>28-มี.ค.-67</u>
<b>5. PERFORMANCE TESTS</b>	<b>SPEC.                      RESULTS</b>
*A. Neutral density filter checks with Copper (324.8 nm)	
Neutral Density Filter 0.2 ± 10%	0.180 <u>0.175</u> Abs.
B. AA Baseline noise test with Copper (324.8 nm)	
Integration time                      = 0.5 seconds	
Replicates                                = 99 times	
Standard Deviation                      ≤ 0.001	<u>0.000</u>
C. Flame sensitivity with Copper (324.8nm)	
(5 mg/L Cu Standard a read time of 10 seconds	
10 replicates, standard burner)	
Stainless steel nebulizer                      ≥ 0.25	<u>0.332</u> Abs.
%RSD                      ≤ 0.3	<u>0.23</u> %
Measured Characteristic Concentration :	<u>0.066</u> mg/L

## ATOMIC ABSORPTION SPECTROPHOTOMETER MODEL

**SERIAL NUMBER**      **040S0110503**

DATE TESTED 28-มี.ค.-67

Remarks : \_\_\_\_\_

---

---

---

---

---

---

☒ meets


☐ does not meet

**Service Department TH ONE SOURCE CO., LTD.**


( [REDACTED] )  
Customer Support Engineer



Current Wavelength: 249.30    Peak Wavelength: 248.24

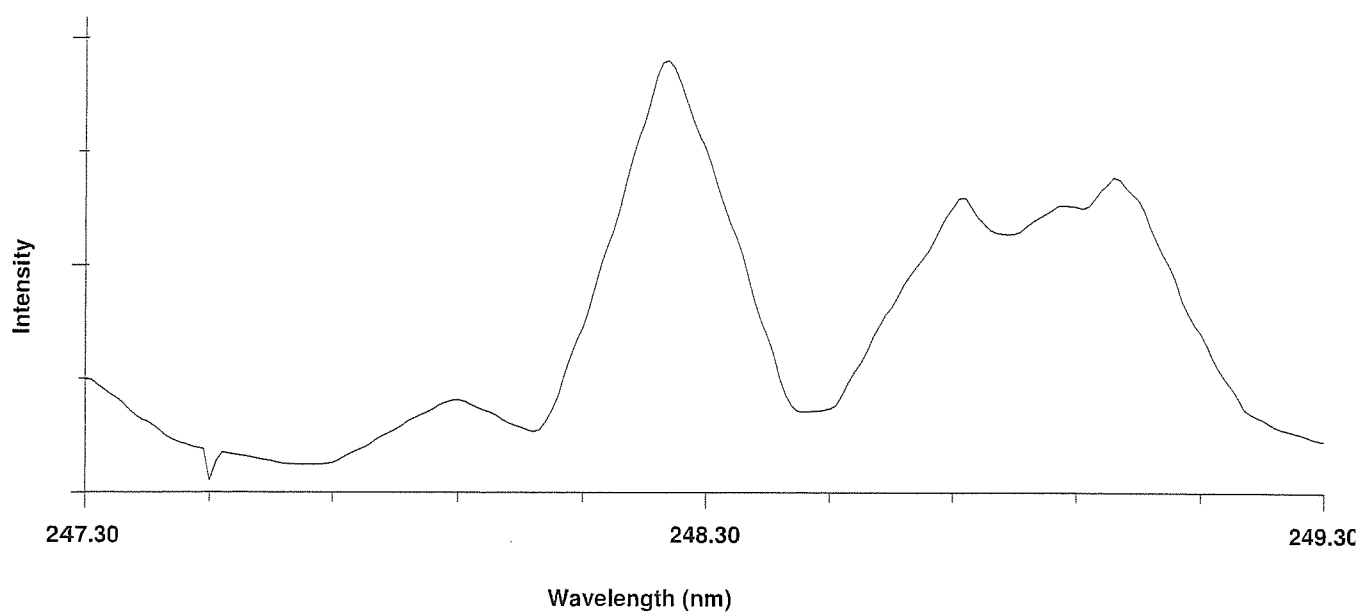

Current Wavelength: 214.90    Peak Wavelength: 214.08

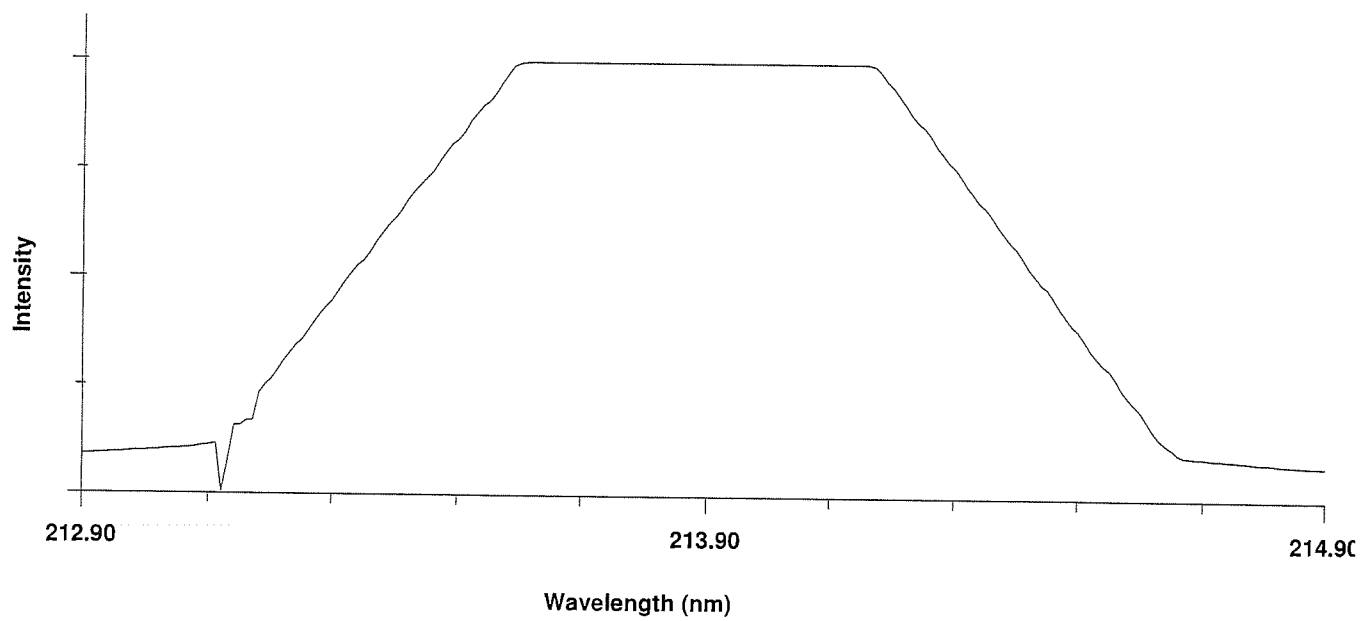

RECALIBRATION

DUE DATE:

September 21, 2023

## Certificate of Calibration

### Calibration Certification Information

Cal. Date: September 21, 2022      Rootsmeter S/N: 438320      Ta: 296 °K  
 Operator: Jim Tisch      Pa: 748.3 mm Hg  
 Calibration Model #: TE-5025A      Calibrator S/N: 0068

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.3760	3.2	2.00
2	3	4	1	0.9710	6.4	4.00
3	5	6	1	0.8730	8.0	5.00
4	7	8	1	0.8300	8.8	5.50
5	9	10	1	0.6870	12.7	8.00

### Data Tabulation

Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left( \frac{Ta}{Pa} \right)}$ (y-axis)
0.9870	0.7173	1.4080	0.9957	0.7236	0.8895
0.9828	1.0121	1.9912	0.9914	1.0211	1.2579
0.9806	1.1233	2.2262	0.9893	1.1332	1.4064
0.9796	1.1802	2.3349	0.9882	1.1907	1.4750
0.9744	1.4184	2.8160	0.9830	1.4309	1.7789
QSTD	m=	2.01042	QA	m=	1.25889
	b=	-0.03659		b=	-0.02312
	r=	0.99996		r=	0.99996

### Calculations

Vstd=	$\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$	Va=	$\Delta Vol((Pa-\Delta P)/Pa)$
Qstd=	$Vstd/\Delta Time$	Qa=	$Va/\Delta Time$
For subsequent flow rate calculations:			
Qstd=	$1/m \left( \left( \sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa=	$1/m \left( \left( \sqrt{\Delta H \left( \frac{Ta}{Pa} \right)} \right) - b \right)$


### Standard Conditions

Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH:	calibrator manometer reading (in H2O)
ΔP:	rootsmeter manometer reading (mm Hg)
Ta:	actual absolute temperature (°K)
Pa:	actual barometric pressure (mm Hg)
b:	intercept
m:	slope

### RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## High Volume TSP&PM-10 Calibration Report

Location : Thai Environmental Tech

Site ID : Bangkok

Date : 4-Jul-23

ITEM : TSP

Serial No : (No.3 )

Calibrate By : Pipat

### Site Conditions

Barometric Pressure (mm Hg) : 760.00

Temperature (°C) : 25.0

Average Press. (mm Hg) : 750.6

Average Temp (°C) : 28.2

Corrected Pressure (mm Hg) : 760.0

Temperature (deg K) : 298.0

Corrected Average (mm Hg) : -

Average Temp: (Deg K) : -

### Calibration Orifice

Make : Tisch

Model : TE-5025A

Serial# : 0068

Qstd Slope : 2.01042

Qstd Intercept : -0.36590

Calibration Due Date : 21-Sep-23

### Calibration Information

Plate or Test #	ORIFICE (in H <sub>2</sub> O)	Qstd (m <sup>3</sup> /min)	Indicate (CFM)	IC (corrected)	Linear Regression Slope : 29.8558 Intercept : 0.1836 Corr. Coeff : 0.9932 # of Observations: 5
1	12.30	1.926	60.0	57.00	
2	10.00	1.755	54.0	52.00	
3	7.60	1.553	50.0	48.00	
4	5.00	1.294	40.0	40.00	
5	3.00	1.044	30.0	30.00	

### Calculations

$$Qstd = 1/m[\text{Sqrt}(H_2O(P_a/P_{std}))(T_{std}/T_a)] - b]$$

$$IC = I[\text{Sqrt}(P_a/P_{std})(T_{std}/T_a)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

Tstd = 298 deg K

Pstd = 760 mm Hg

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/T_{av})(P_{av}/760)] - b)$$

m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily a

Calibrate By : \_\_\_\_\_

Approve By : \_\_\_\_\_

**NOTE: Ensure calibration orifice has been certified within 12 months of use**





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## High Volume TSP&PM-10 Calibration Report

Location : Thai Environmental Tech

Site ID : Bangkok

Date : 11-Jul-23

ITEM : TSP

Serial No : (No.35 )

Calibrate By : Pipat

### Site Conditions

Barometric Pressure (mm Hg) : 760.00

Temperature (°C) : 25.0

Average Press. (mm Hg) : 750.8

Average Temp (°C) : 28.4

Corrected Pressure (mm Hg) : 760.0

Temperature (deg K) : 298.0

Corrected Average (mm Hg) : -

Average Temp: (Deg K) : -

### Calibration Orifice

Make : Tisch

Model : TE-5025A

Serial# : 0068

Qstd Slope : 2.01042

Qstd Intercept : -0.36590

Calibration Due Date : 21-Sep-23

### Calibration Information

Plate or Test #	ORIFICE (in H <sub>2</sub> O)	Qstd (m <sup>3</sup> /min)	Indicate (CFM)	IC (corrected)	Linear Regression Slope : 30.1571 Intercept : 0.3626 Corr. Coeff : 0.9846 # of Observations: 5
1	12.50	1.941	60.0	57.00	
2	9.20	1.691	54.0	52.00	
3	7.00	1.498	50.0	48.00	
4	5.00	1.294	40.0	40.00	
5	3.00	1.044	30.0	30.00	

### Calculations

$$Qstd = 1/m[\text{Sqrt}(H_2O(Pa/Pstd)(Tstd/Ta)) - b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

Tstd = 298 deg K

Pstd = 760 mm Hg

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/Tav)(Pav/760)] - b)$$

**NOTE: Ensure calibration orifice has been certified within 12 months of use**


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily

Calibrate By : 

Approve By : 







Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## High Volume TSP&PM-10 Calibration Report

Location : Thai Environmental Tech

Site ID : Bangkok

Date : 5-Jul-23

ITEM : TSP

Serial No : (No.32 )

Calibrate By : Pipat

### Site Conditions

Barometric Pressure (mm Hg) : 760.00  
Temperature (°C) : 25.0  
Average Press. (mm Hg) : 750.6  
Average Temp (°C) : 28.4

Corrected Pressure (mm Hg) : 760.0  
Temperature (deg K) : 298.0  
Corrected Average (mm Hg) : -  
Average Temp: (Deg K) : -

### Calibration Orifice

Make : Tisch  
Model : TE-5025A  
Serial# : 0068

Qstd Slope : 2.01042  
Qstd Intercept : -0.36590  
Calibration Due Date : 21-Sep-23

### Calibration Information

Plate or Test #	ORIFICE (in H <sub>2</sub> O)	Qstd (m <sup>3</sup> /min)	Indicate (CFM)	IC (corrected)	Linear Regression Slope : 29.9470 Intercept : 0.4184 Corr. Coeff : 0.9883 # of Observations: 5
1	12.50	1.941	60.0	57.00	
2	9.50	1.715	54.0	52.00	
3	7.20	1.517	50.0	48.00	
4	5.00	1.294	40.0	40.00	
5	3.00	1.044	30.0	30.00	

### Calculations

$$Qstd = 1/m[\text{Sqrt}(H_2O(P_a/P_{std})(T_{std}/T_a))-b]$$

$$IC = I[\text{Sqrt}(P_a/P_{std})(T_{std}/T_a)]$$

Qstd = standard flow rate  
IC = corrected chart response  
I = actual chart response

m = calibrator Qstd slope  
b = calibrator Qstd intercept  
Ta = actual temperature during calibration (deg K)  
Pa = actual pressure during calibration (mm Hg)  
Tstd = 298 deg K  
Pstd = 760 mm Hg

For subsequent calculation of sampler flow:  
 $1/m((I[\text{Sqrt}(298/T_{av})(P_{av}/760)]-b)$

m = sampler slope  
b = sampler intercept  
I = chart response  
Tav = daily average temperature  
Pav = daily average pressure

Calibrate By : 

Approve By : 

**NOTE: Ensure calibration orifice has been certified within 12 months of use**





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## High Volume TSP&PM-10 Calibration Report

Location : Thai Environmental Tech

Site ID : Bangkok

Date : 13-Jul-23

ITEM : TSP

Serial No : (No.37 )

Calibrate By : Pipat

### Site Conditions

Barometric Pressure (mm Hg) : 760.00

Temperature (°C) : 25.0

Average Press. (mm Hg) : 750.8

Average Temp (°C) : 28.6

Corrected Pressure (mm Hg) : 760.0

Temperature (deg K) : 298.0

Corrected Average (mm Hg) : -

Average Temp: (Deg K) : -

### Calibration Orifice

Make : Tisch

Model : TE-5025A

Serial# : 0068

Qstd Slope : 2.01042

Qstd Intercept : -0.36590

Calibration Due Date : 21-Sep-23

### Calibration Information

Plate or Test #	ORIFICE (in H <sub>2</sub> O)	Qstd (m <sup>3</sup> /min)	Indicate (CFM)	IC (corrected)	Linear Regression Slope : 30.2297 Intercept : 0.1413 Corr. Coeff : 0.9875 # of Observations: 5
1	12.50	1.941	60.0	57.00	
2	9.20	1.691	54.0	52.00	
3	7.20	1.517	50.0	48.00	
4	5.00	1.294	40.0	40.00	
5	3.00	1.044	30.0	30.00	

### Calculations

$$Qstd = 1/m[\text{Sqrt}(H_2O(Pa/Pstd)(Tstd/Ta)) - b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

Tstd = 298 deg K

Pstd = 760 mm Hg

For subsequent calculation of sampler flow:

$$1/m((I[\text{Sqrt}(298/Tav)(Pav/760)] - b)$$

m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

Calibrate By : \_\_\_\_\_

Approve By : \_\_\_\_\_

**NOTE: Ensure calibration orifice has been certified within 12 months of use**





Thai Environmental Technic Limited  
บริษัท เทคโนโลยีสิ่งแวดล้อมไทย จำกัด

## High Volume TSP&PM-10 Calibration Report

Location : Thai Environmental Tech

Site ID : Bangkok

Date : 5-Jul-23

ITEM : PM10

Serial No : (No. 9 )

Calibrate By : Pipat

### Site Conditions

Barometric Pressure (mm Hg) : 760.00

Temperature (°C) : 25.0

Average Press. (mm Hg) : 750.6

Average Temp (°C) : 27.8

Corrected Pressure (mm Hg) : 760.0

Temperature (deg K) : 298.0

Corrected Average (mm Hg) : -

Average Temp (Deg K) : -

### Calibration Orifice

Make : Tisch

Model : TE-5025A

Serial# : 0068

Qstd Slope : 2.01042

Qstd Intercept : -0.03659

Calibration Due Date : 21-Sep-23

### Calibration Information

Plate or Test #	ORIFICE (in H <sub>2</sub> O)	Qstd (m <sup>3</sup> /min)	Indicate (CFM)	IC (corrected)	Linear Regression Slope : 35.3684 Intercept : 0.0092 Corr. Coeff : 0.9923 # of Observations: 5
1	12.00	1.741	60.0	60.00	
2	9.00	1.510	54.0	54.00	
3	7.20	1.353	50.0	50.00	
4	5.00	1.130	40.0	40.00	
5	3.00	0.880	30.0	30.00	

### Calculations

$$Qstd = 1/m[\text{Sqrt}(H_2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

Tstd = 298 deg K

Pstd = 760 mm Hg

For subsequent calculation of sampler flow:

$$1/m((I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$

m = sampler slope


b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

Calibrate By : 

Approve By : 

**NOTE: Ensure calibration orifice has been certified within 12 months of use**





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## High Volume TSP&PM-10 Calibration Report

Location : Thai Environmental Tech

Site ID : Bangkok

Date : 13-Jul-23

ITEM : PM10

Serial No : (No. 20 )

Calibrate By : Pipat

### Site Conditions

Barometric Pressure (mm Hg) : 760.00  
Temperature (°C) : 25.0  
Average Press. (mm Hg) : 750.6  
Average Temp (°C) : 29.3

Corrected Pressure (mm Hg) : 760.0  
Temperature (deg K) : 298.0  
Corrected Average (mm Hg) : -  
Average Temp (Deg K) : -

### Calibration Orifice

Make : Tisch  
Model : TE-5025A  
Serial# : 0068

Qstd Slope : 2.01042  
Qstd Intercept : -0.03659  
Calibration Due Date : 21-Sep-23

### Calibration Information

Plate or Test #	ORIFICE (in H <sub>2</sub> O)	Qstd (m <sup>3</sup> /min)	Indicate (CFM)	IC (corrected)	Linear Regression Slope : 34.6244 Intercept : 0.7804 Corr. Coeff : 0.9913 # of Observations: 5
1	12.20	1.756	60.0	60.00	
2	9.20	1.527	54.0	54.00	
3	7.20	1.353	50.0	50.00	
4	5.00	1.130	40.0	40.00	
5	3.00	0.880	30.0	30.00	

### Calculations

$$Qstd = 1/m[\text{Sqrt}(H_2O(P_a/P_{std})(T_{std}/T_a))-b]$$

$$IC = I[\text{Sqrt}(P_a/P_{std})(T_{std}/T_a)]$$

Qstd = standard flow rate  
IC = corrected chart response  
I = actual chart response

m = calibrator Qstd slope  
b = calibrator Qstd intercept  
T<sub>a</sub> = actual temperature during calibration (deg K)  
P<sub>a</sub> = actual pressure during calibration (mm Hg)  
T<sub>std</sub> = 298 deg K  
P<sub>std</sub> = 760 mm Hg

For subsequent calculation of sampler flow:  
 $1/m((I[\text{Sqrt}(298/T_{av})(P_{av}/760)]-b)$

m = sampler slope  
b = sampler intercept  
I = chart response  
T<sub>av</sub> = daily average temperature  
P<sub>av</sub> = daily average pressure

Calibrate By : 

Approve By : 

**NOTE: Ensure calibration orifice has been certified within 12 months of use**







Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## High Volume TSP&PM-10 Calibration Report

Location : Thai Environmental Tech

Site ID : Bangkok

Date : 13-Jul-23

ITEM : PM10

Serial No : (No. 19 )

Calibrate By : Pipat

### Site Conditions

Barometric Pressure (mm Hg) : 760.00  
Temperature (°C) : 25.0  
Average Press. (mm Hg) : 750.8  
Average Temp (°C) : 29.5

Corrected Pressure (mm Hg) : 760.0  
Temperature (deg K) : 298.0  
Corrected Average (mm Hg) : -  
Average Temp: (Deg K) : -

### Calibration Orifice

Make : Tisch  
Model : TE-5025A  
Serial# : 0068

Qstd Slope : 2.01042  
Qstd Intercept : -0.03659  
Calibration Due Date : 21-Sep-23

### Calibration Information

Plate or Test #	ORIFICE (in H <sub>2</sub> O)	Qstd (m <sup>3</sup> /min)	Indicate (CFM)	IC (corrected)	Linear Regression Slope : 35.8414 Intercept : -0.3794 Corr. Coeff : 0.9909 # of Observations: 5
1	11.80	1.727	60.0	60.00	
2	9.00	1.510	54.0	54.00	
3	7.00	1.334	50.0	50.00	
4	5.00	1.130	40.0	40.00	
5	3.00	0.880	30.0	30.00	

### Calculations

$$Qstd = 1/m[\text{Sqrt}(H_2O(P_a/P_{std})(T_{std}/T_a))-b]$$

$$IC = I[\text{Sqrt}(P_a/P_{std})(T_{std}/T_a)]$$


Qstd = standard flow rate  
IC = corrected chart response  
I = actual chart response


m = calibrator Qstd slope  
b = calibrator Qstd intercept  
T<sub>a</sub> = actual temperature during calibration (deg K)  
P<sub>a</sub> = actual pressure during calibration (mm Hg)  
T<sub>std</sub> = 298 deg K  
P<sub>std</sub> = 760 mm Hg

For subsequent calculation of sampler flow:  
 $1/m((I[\text{Sqrt}(298/T_a)(P_a/760)]-b)$

**NOTE: Ensure calibration orifice has been certified within 12 months of use**

m = sampler slope  
b = sampler intercept  
I = chart response  
T<sub>av</sub> = daily average temperature  
P<sub>av</sub> = daily average pressure

Calibrate By : 

Approve By : 





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## High Volume TSP&PM-10 Calibration Report

Location : Thai Environmental Tech

Site ID : Bangkok

Date : 5-Jul-23

ITEM : PM10

Serial No : (No. 23 )

Calibrate By : Pipat

### Site Conditions

Barometric Pressure (mm Hg) : 760.00

Temperature (°C) : 25.0

Average Press. (mm Hg) : 750.8

Average Temp (°C) : 29.4

Corrected Pressure (mm Hg) : 760.0

Temperature (deg K) : 298.0

Corrected Average (mm Hg) : -

Average Temp (Deg K) : -

### Calibration Orifice

Make : Tisch

Model : TE-5025A

Serial# : 0068

Qstd Slope : 2.01042

Qstd Intercept : -0.03659

Calibration Due Date : 21-Sep-23

### Calibration Information

Plate or Test #	ORIFICE (in H <sub>2</sub> O)	Qstd (m <sup>3</sup> /min)	Indicate (CFM)	IC (corrected)	Linear Regression Slope : 35.1530 Intercept : 0.0074 Corr. Coeff : 0.9904 # of Observations: 5
1	12.80	1.798	62.0	62.00	
2	10.20	1.607	56.0	56.00	
3	7.60	1.389	52.0	52.00	
4	5.20	1.152	40.0	40.00	
5	3.00	0.880	30.0	30.00	

### Calculations

$$Qstd = 1/m[\text{Sqrt}(H_2O(P_a/P_{std})(T_{std}/T_a)) - b]$$

$$IC = I[\text{Sqrt}(P_a/P_{std})(T_{std}/T_a)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

Tstd = 298 deg K

Pstd = 760 mm Hg

For subsequent calculation of sampler flow:

$$1/m((I[\text{Sqrt}(298/T_{av})(P_{av}/760)] - b)$$

**NOTE: Ensure calibration orifice has been certified within 12 months of use**

m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

Calibrate By : \_\_\_\_\_

Approve By : \_\_\_\_\_



## Certificate Of Analysis

## Special Gases Mixture

## Customer Details

Name:  
Thai Environmental Technic Limited

Address:  
1/6 Soi Ramkhamhaeng 45, Sapansoong,  
Khet Saphan Sung, Bangkok 10240

Customer Tag No.:

## Certificate Details

Number:	1734/23	Date of Issue:	5-Jul-2023	Expiry date:	5-Jul-2026
Material Details					
Production Order:	90178560	Material Code:	640300-SK-44	Cylinder No.:	A00917SK
Gas content:	5.520 M <sup>3</sup>	Filling pressure:	145.0 bar	Valve:	CGA 660 SS
Cylinder Owner:	LINDE	Cylinder Material:	Spectra seal	Cylinder Size:	40 L

## Laboratory Report

## Analytical Result

Component	Normal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>	Assay Date
Nitric Oxide	40.0 ppm	40.5 ppm	± 1% relative	(6) I-PB-352	28-Jun & 5-Jul-2023
Other NOx impurity In Nitrogen		Less than 2.0 ppm			

## Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date
Nitric Oxide In Nitrogen	258013SG	25.32 ± 0.25 ppm	13-Dec-2024

## Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-NO	28-Jun-2023

## Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.

Storage condition: Keep in well ventilation and secure area.

## Comments

When reordering, please quote the material number

## Note:

1. All results expressed in this report are on mole/mole basis, unless otherwise specified. 2. Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Calibration of Gaseous Calibration Standards using procedure G1. 3. The reported expanded uncertainty is based on a standard uncertainty multiplied by coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard, which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.
3. (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasontorn

Signatory for and on behalf of Linde (Thailand) Co., Ltd.

Linde (Thailand) Public Company Limited

P.O. Box 15, 15/01, 15/02, 15/03, 15/04, 15/05, 15/06, 15/07, 15/08, 15/09, 15/10, 15/11, 15/12, 15/13, 15/14, 15/15, 15/16, 15/17, 15/18, 15/19, 15/20, 15/21, 15/22, 15/23, 15/24, 15/25, 15/26, 15/27, 15/28, 15/29, 15/30, 15/31, 15/32, 15/33, 15/34, 15/35, 15/36, 15/37, 15/38, 15/39, 15/40, 15/41, 15/42, 15/43, 15/44, 15/45, 15/46, 15/47, 15/48, 15/49, 15/50, 15/51, 15/52, 15/53, 15/54, 15/55, 15/56, 15/57, 15/58, 15/59, 15/60, 15/61, 15/62, 15/63, 15/64, 15/65, 15/66, 15/67, 15/68, 15/69, 15/70, 15/71, 15/72, 15/73, 15/74, 15/75, 15/76, 15/77, 15/78, 15/79, 15/80, 15/81, 15/82, 15/83, 15/84, 15/85, 15/86, 15/87, 15/88, 15/89, 15/90, 15/91, 15/92, 15/93, 15/94, 15/95, 15/96, 15/97, 15/98, 15/99, 15/100

15<sup>th</sup> Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad Km. 6.5 Road, Bangnaeew  
Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333  
Wellgrow Plant 105 Moo 5, I.Bangsamak, A.Bangpakong, Chachoengsao 24180  
Thailand, Tel (66) 38 570-479-93 Fax (66) 38 570-323





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## NOx Analyzer Calibration Report

Calibrate Date : 9-Nov-23  
Analyzer Type : NOx  
Brand : Teledyne  
Model : 200 E  
Serial Number : 481 (No.37)  
Range : 500 ppb


Temperature (°C) : 25°C  
Barometer (mmHg) : 760.0  
Humidity (50±15 %) : 50.0%RH  
Dilutor : API M700 S/N 625  
Zero Air : API M701 S/N 1926  
Standard gas : A00917 SK

### Calibration of Span

Supply Gas	Ref Value(ppb)	Before of Span.(ppb)			After of Span.(ppb)			% diff of Span
		NOx	NO	NO <sub>2</sub>	NOx	NO	NO <sub>2</sub>	
Zero	0.0	0.9	0.4	0.5	0.0	0.0	0.0	0.0
Span	400.0	408.0	401.0	7.0	400.0	400.0	0.0	0.0

### Multi Point Calibration

Ref Value(ppb)	Analyzer Disp.(ppb)			Output Difference		
	NOx	NO	NO <sub>2</sub>	Diff(ppb)	% Diff	Abs (%) Diff
0.0	0.8	0.4	0.4	0.40	0.001	0.10
100.0	99.6	99.1	0.5	-0.90	-0.009	0.90
200.0	200.5	199.7	0.8	-0.30	-0.002	0.15
400.0	399.5	398.7	0.8	-1.30	-0.003	0.33
Average Diff (%)						0.37

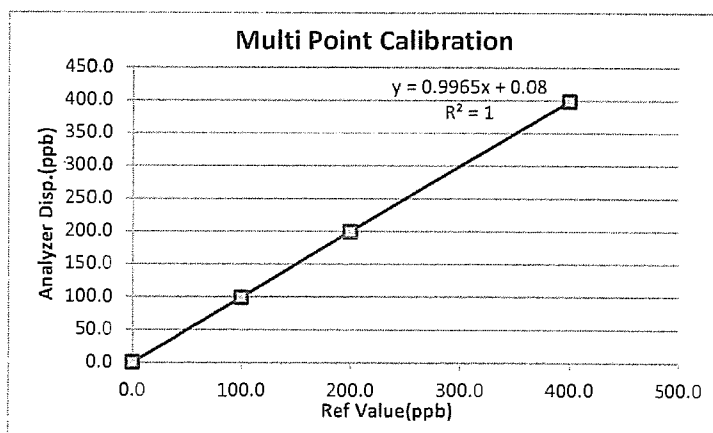

Calibrate by:



Approved by:









Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## NOx Analyzer Calibration Report


Calibrate Date	: 10-Nov-23	Temperature (°C)	: 25°C
Analyzer Type	: NOx	Barometer (mmHg)	: 760.0
Brand	: Teledyne	Humidity (50±15 %)	: 50.0%RH
Model	: T200	Dilutor	: API M700 S/N 625
Serial Number	: 5158 (No. 31)	Zero Air	: API M701 S/N 1926
Range	: 500 ppb	Standard gas	: A00917 SK

### Calibration of Span

Supply Gas	Ref Value(ppb)	Before of Span.(ppb)			After of Span.(ppb)			% diff of Span
		NOx	NO	NO <sub>2</sub>	NOx	NO	NO <sub>2</sub>	
Zero	0.0	2.5	2.2	0.3	0.0	0.0	0.0	0.0
Span	400.0	413.0	408.0	5.0	400.0	400.0	0.0	0.0

### Multi Point Calibration

Ref Value(ppb)	Analyzer Disp.(ppb)			Output Difference		
	NOx	NO	NO <sub>2</sub>	Diff(ppb)	% Diff	Abs (%) Diff
0.0	0.7	0.4	0.3	0.40	0.001	0.10
100.0	100.2	99.4	0.8	-0.60	-0.006	0.60
200.0	200.4	200.1	0.3	0.10	0.000	0.05
400.0	402.0	401.0	1.0	1.00	0.003	0.25
Average Diff (%)						0.30

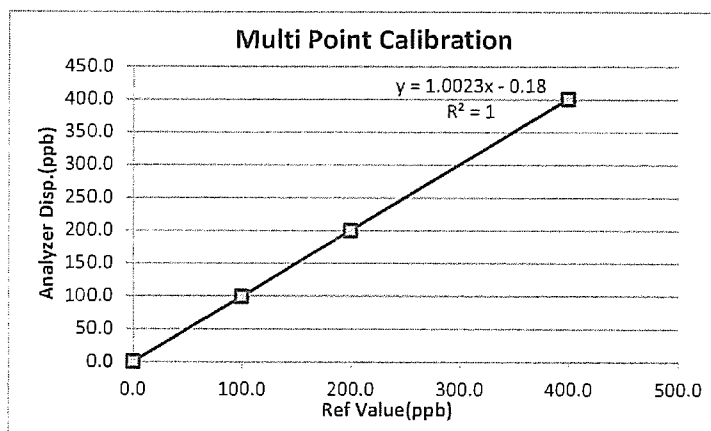

Calibrate by:



Approved by:







Thai Environmental Technic Limited  
บริษัท เทคโนโลยีสิ่งแวดล้อมไทย จำกัด

## NOx Analyzer Calibration Report

Calibrate Date : 9-Nov-23  
Analyzer Type : NOx  
Brand : API  
Model : 200A  
Serial Number : 1982 (No.16)  
Range : 500 ppb


Temperature (°C) : 25°C  
Barometer (mmHg) : 759.9  
Humidity (50±15 %) : 50.0%RH  
Dilutor : API M700 S/N 625  
Zero Air : API M701 S/N 1926  
Standard gas : A00917 SK

### Calibration of Span

Supply Gas	Ref Value(ppb)	Before of Span.(ppb)			After of Span.(ppb)			% diff of Span
		NOx	NO	NO <sub>2</sub>	NOx	NO	NO <sub>2</sub>	
Zero	0.0	0.5	0.8	-0.3	0.0	0.0	0.0	0.0
Span	400.0	420.0	413.0	7.0	400.0	400.0	0.0	0.0

### Multi Point Calibration

Ref Value(ppb)	Analyzer Disp.(ppb)			Output Difference		
	NOx	NO	NO <sub>2</sub>	Diff(ppb)	% Diff	Abs (%) Diff
0.0	0.3	0.1	0.2	0.10	0.000	0.03
100.0	100.3	100.2	0.1	0.20	0.002	0.20
200.0	199.8	199.5	0.3	-0.50	-0.003	0.25
400.0	399.2	399.1	0.1	-0.90	-0.002	0.22
Average Diff (%)						0.17

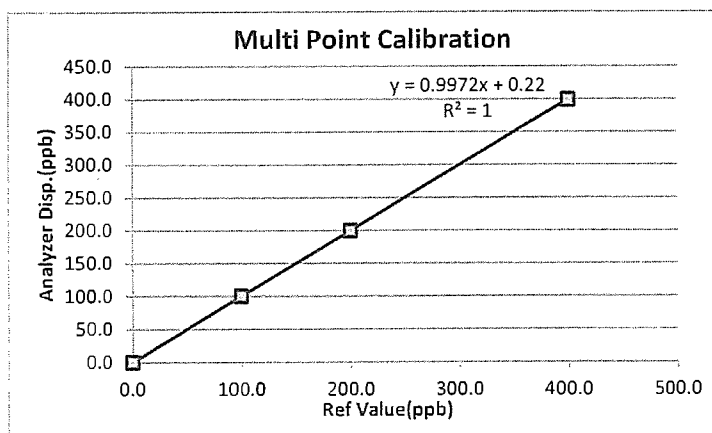

Calibrate by:

Approved by:

แก้ไขครั้งที่ : 00

วันที่อนุมัติ 02/09/15

เลขที่แบบฟอร์ม : QF-QP16-06





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## NOx Analyzer Calibration Report

Calibrate Date : 10-Nov-23  
Analyzer Type : NOx  
Brand : Teledyne  
Model : 200 E  
Serial Number : 2789 (No.36)  
Range : 500 ppb


Temperature (°C) : 25°C  
Barometer (mmHg) : 760.0  
Humidity (50±15 %) : 50.0%RH  
Dilutor : API M700 S/N 625  
Zero Air : API M701 S/N 1926  
Standard gas : A00917 SK

### Calibration of Span

Supply Gas	Ref Value(ppb)	Before of Span.(ppb)			After of Span.(ppb)			% diff of Span
		NOx	NO	NO <sub>2</sub>	NOx	NO	NO <sub>2</sub>	
Zero	0.0	2.5	1.1	1.4	0.0	0.0	0.0	0.0
Span	400.0	391.0	385.0	6.0	400.0	400.0	0.0	0.0

### Multi Point Calibration

Ref Value(ppb)	Analyzer Disp.(ppb)			Output Difference		
	NOx	NO	NO <sub>2</sub>	Diff(ppb)	% Diff	Abs (%) Diff
0.0	0.5	0.2	0.3	0.20	0.001	0.05
100.0	100.2	99.8	0.4	-0.20	-0.002	0.20
200.0	199.5	199.3	0.2	-0.70	-0.003	0.35
400.0	400.3	399.8	0.5	-0.20	0.000	0.05
Average Diff (%)						0.16

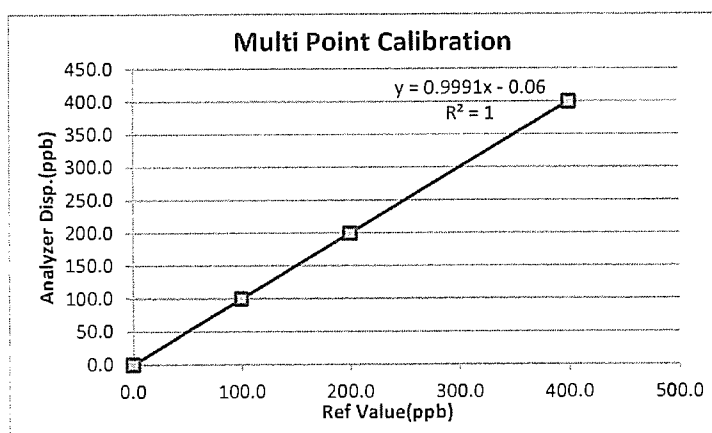

Calibrate by:



Approved by:





Certificate Of Analysis  
Special Gases Mixture

## Customer Details

Name: Thai Environmental Technic Limited. Address: 1/6 Soi Ramkhamhaeng 45, Sapansoong, Khet Saphan Sung, Bangkok 10240 Customer Tag No.: -

## Certificate Details

Number: 2500/23 Date of Issue: 18-Sep-2023 Expiry date: 18-Sep-2027  
Material Details  
Production Order: 90179846 Material Code: 608400-SK-44 Cylinder No.: D636157  
Gas content: 5.520 M<sup>3</sup> Filling pressure: 145 bar Valve: CGA 660 SS  
Cylinder Owner: LINDE Cylinder Material: Spectra seal Cylinder Size: 40 L

## Laboratory Report

## Analytical Result

Component	Nominal Concentration	Analysis Result <sup>1</sup>	Uncertainty <sup>2</sup>	Method of Analysis <sup>3</sup>	Assay Date
Sulphur Dioxide In Nitrogen	40.0 ppm	41.1 ppm	± 1% relative	(6) I-PB-352	8-Sep & 18-Sep-23

## Reference Standard used in Assay

Reference Standard	Cylinder number	Concentration	Expiry date:
Sulphur Dioxide In Nitrogen	BOC150629SG	25.35 ± 0.25 ppm	9-Jun-2024

## Analytical Instruments used in Assay

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
FTIR Spectrometers Nicolet iS50	FTIR-SO2	6-Sep-2023

## Recommend usage condition

Minimum utilization: 5% of actual content or before expire date whichever comes first.  
Storage condition: Keep in well ventilation and secure area.

## Comments

When reordering, please quote the material number

## Note:

1. All results expressed in this report are on mole/mole basis, unless otherwise specified. The Assay of this Standard has been performed in accordance with the EPA Traceability Protocol EPA-600/R-12/531 for the Assay and Certification of Gaseous Calibration Standards using procedure G1  
2. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%. The measurement of this material is traceable to the SI through the reference gas standard which is traceable to Swiss National Standard of Mass or other recognised national metrology institutes.  
3. (1) Gas Chromatography, (2) Paramagnetic Oxygen Analyzer, (3) Electrochemical Oxygen Analyzer, (4) Electrochemical Moisture Analyzer, (5) Total Hydrocarbon Analyzer, (6) Other - Specified

Sukanya Parinyasoonorn  
Signatory for and on behalf of Linde (Thailand) Public Company Limited

Page 1 of 1

This report shall not be reproduced except in full

PB-002/F006

Iss:L/2, 01 August 2023

บริษัท ลินด์ (ประเทศไทย) จำกัด (มหาชน)

เบอร์โทรศัพท์สำนักงาน 0107537000765

ชั้น 15 อาคารทาวเวอร์ เอ 2/3 หมู่ 14 ถนนบางนา-ตราด กม. 6.5 แขวงทวี

อ.บางพลี จ.สมุทรปราการ 10540 โทรศัพท์ (66) 2338-6100 โทรสาร (66) 2338-6333

โรงงานเวลโกรว์ : 105 หมู่ 5 ต.บางสนธิ์ อ.บางปะกง จ.ฉะเชิงเทรา 24180

โทรศัพท์ (66) 38.570-479-93

โทรสาร (66) 38.570-323

Linde (Thailand) Public Company Limited

PLC Registration no. 0107537000765

15<sup>th</sup> Floor, Bangna Tower A, 2/3 Moo 14, Bangna Trad KM. 6.5 Road, Bangkaew

Bangplee, Samutprakarn 10540, Tel (66) 2338-6100 Fax (66) 2338-6333


Wellgrow Plant : 105 Moo 5, T.Bangsamak, A.Bangpakong, Chachoengsao 24180

Thailand, Tel (66) 38.570-479-93

Fax (66) 38.570-323







Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## Analyzer Calibration Report


Calibrate Date	6-Nov-23	Temperature (°C)	: 25°C
Analyzer Type	SO <sub>2</sub>	Barometer (mmHg)	: 760.0
Brand	Thermo	Humidity (50±15 %)	: 50.0 %RH
Model	43C	Dilutor	: API M700 S/N 625
Serial Number	43C73374373 (No. 10)	Zero Air	: API M701 S/N 1926
Range	500 ppb	Standard gas	: D636157

### Calibration of Span

Supply Gas	Ref Value(ppb)	Before of Span.(ppb)	After of Span.(ppb)	Abs% diff of Span
Zero	0.0	0.8	0.0	0.0
Span	400.0	395.0	400.0	0.0

### Multi Point Calibration

Ref Value(ppb)	Analyzer Disp.(ppb)	Output Difference		
		Diff (ppb)	Percent Diff	Abs Percent Diff
0.0	0.3	0.3	0.00	0.08
100.0	99.8	-0.2	0.00	0.20
200.0	199.5	-0.5	0.00	0.25
400.0	399.6	-0.4	0.00	0.10
Average Diff (%)				0.16

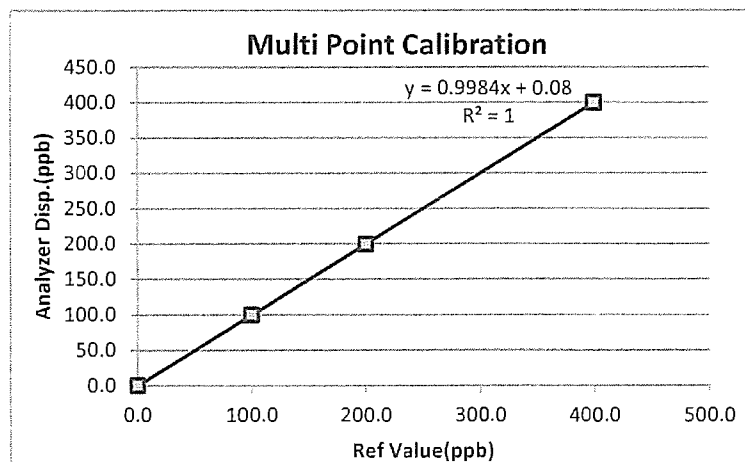

Calibrate by: \_\_\_\_\_


Approved by: \_\_\_\_\_

แก้ไขครั้งที่ : 00

วันที่อนุมัติ 02/09/15

เลขที่แบบฟอร์ม : QF-QP16-06





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## Analyzer Calibration Report


Calibrate Date	9-Nov-23	Temperature (°C)	: 25°C
Analyzer Type	SO <sub>2</sub>	Barometer (mmHg)	: 760.0
Brand	Teledyne	Humidity (50±15 %)	: 50.0 %RH
Model	100 E	Dilutor	: API M700 S/N 625
Serial Number	1341 (No. 20)	Zero Air	: API M701 S/N 1926
Range	500 ppm	Standard gas	: D636157

### Calibration of Span

Supply Gas	Ref Value(ppb)	Before of Span.(ppb)	After of Span.(ppb)	Abs% diff of Span
Zero	0.0	1.1	0.0	0.0
Span	400.0	408.0	400.0	0.0

### Multi Point Calibration

Ref Value(ppb)	Analyzer Disp.(ppb)	Output Difference		
		Diff (ppb)	Percent Diff	Abs Percent Diff
0.0	0.1	0.1	0.00	0.03
100.0	100.5	0.5	0.01	0.50
200.0	199.3	-0.7	0.00	0.35
400.0	400.7	0.7	0.00	0.17
Average Diff (%)				0.26

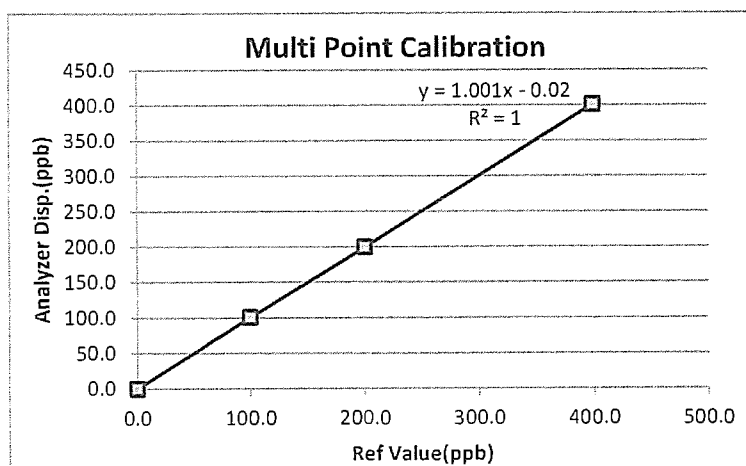

Calibrate by: \_\_\_\_\_


Approved by: \_\_\_\_\_

แก้ไขครั้งที่ : 00

วันที่อนุมัติ 02/09/15

เลขที่แบบฟอร์ม : QF-QP16-06





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## Analyzer Calibration Report


Calibrate Date	7-Nov-23	Temperature (°C)	: 25°C
Analyzer Type	SO <sub>2</sub>	Barometer (mmHg)	: 760.0
Brand	API	Humidity (50±15 %)	: 50.0 %RH
Model	100E	Dilutor	: API M700 S/N 625
Serial Number	383 (No. 12)	Zero Air	: API M701 S/N 1926
Range	500 ppb	Standard gas	: D636157

### Calibration of Span

Supply Gas	Ref Value(ppb)	Before of Span.(ppb)	After of Span.(ppb)	Abs% diff of Span
Zero	0.0	2.1	0.0	0.0
Span	400.0	399.0	400.0	0.0

### Multi Point Calibration

Ref Value(ppb)	Analyzer Disp.(ppb)	Output Difference		
		Diff (ppb)	Percent Diff	Abs Percent Diff
0.0	0.2	0.2	0.00	0.05
100.0	99.8	-0.2	0.00	0.20
200.0	199.5	-0.5	0.00	0.25
400.0	399.8	-0.2	0.00	0.05
Average Diff (%)				0.14

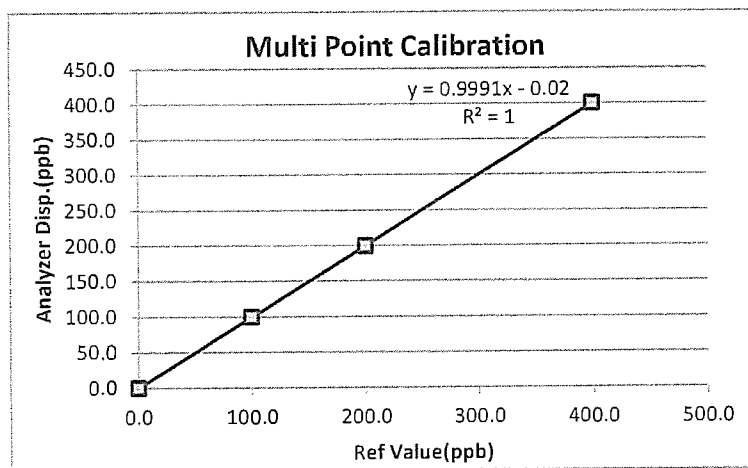

Calibrate by:


Approved by:

แก้ไขครั้งที่ : 00

วันที่อนุมัติ 02/09/15

เลขที่แบบฟอร์ม : QF-QP16-06





Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด

## Analyzer Calibration Report


Calibrate Date	6-Nov-23	Temperature (°C)	: 25 °C
Analyzer Type	SO <sub>2</sub>	Barometer (mmHg)	: 760.0
Brand	Thermo	Humidity (50±15 %)	: 50.0 %RH
Model	43C	Dilutor	: API M700 S/N 625
Serial Number	43C55175302 (No. 8)	Zero Air	: API M701 S/N 1926
Range	500 ppb	Standard gas	: D636157

### Calibration of Span

Supply Gas	Ref Value(ppb)	Before of Span.(ppb)	After of Span.(ppb)	Abs% diff of Span
Zero	0.0	2.3	0.0	0.0
Span	400.0	395.0	400.0	0.0

### Multi Point Calibration

Ref Value(ppb)	Analyzer Disp.(ppb)	Output Difference		
		Diff (ppb)	Percent Diff	Abs Percent Diff
0.0	0.4	0.4	0.00	0.10
100.0	98.9	-1.1	-0.01	1.10
200.0	198.5	-1.5	-0.01	0.75
400.0	399.2	-0.8	0.00	0.20
Average Diff (%)				0.54

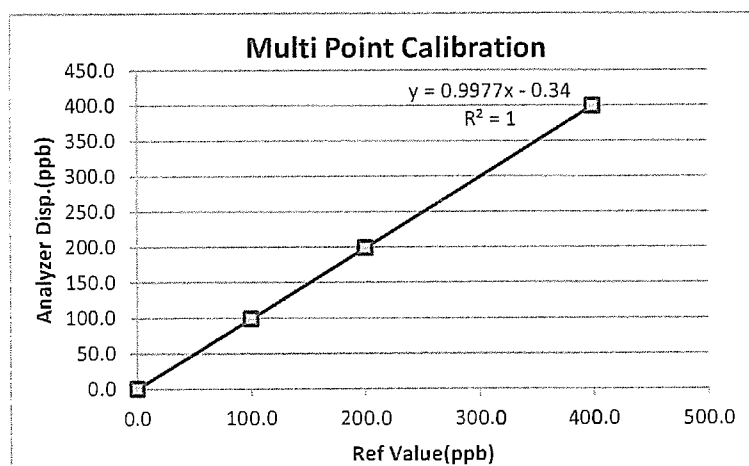

Calibrate by:

Approved by:

แก้ไขครั้งที่ : 00

วันที่อนุมัติ 02/09/15

เลขที่แบบฟอร์ม : QF-QP16-06







# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

## Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 17 January, 2024

Certification No. 046/24

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Weather Wizard III

Serial No. : WC21014A92 ID No. : No.17

Customer : Thai Environmental Technic Limited.  
1/6 Soi Ramkhamhaeng 145,  
Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1015.1 hPa

### NATIONAL STANDARD WIND TUNNEL :

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

### JAPAN QUALITY ASSURANCE ORGANIZATION

: Standard Velocity at 0 - 20 m/sec

Calibrated by


Mr. Watchara

Mechanical Engineer

(Authorised Signatory)

for the Chief

Sub-Standard Instrument

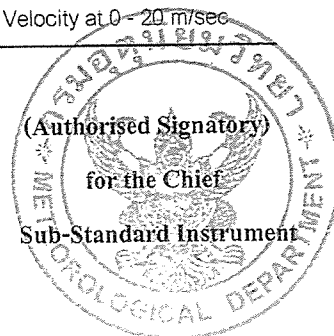



## THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

### The Result of Calibration

Certification No. 046/24

17 January, 2024

Page : 2 of 2


Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
Ultrasonic Anemometer	Pressure	Vacummi	Velocity	Velocity	Correction
m/sec	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	0.4	0.60
3.02	-	-	-	2.2	0.82
5.00	-	-	-	4.5	0.50
7.00	-	-	-	6.3	0.70
9.02	-	-	-	8.5	0.52
11.01	-	-	-	10.3	0.71
13.01	-	-	-	12.5	0.51
15.01	-	-	-	14.5	0.51
17.02	-	-	-	16.5	0.52
20.02	-	-	-	19.5	0.52

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :



Mr. Watcharapol Subwat  
Mechanical Engineer

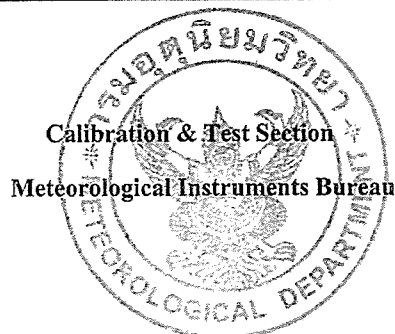



*THAI METEOROLOGICAL DEPARTMENT*

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

**Calibration Certificate**

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 24 October, 2023

Certification No. 375/23

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Weather Wizard II

Serial No. : WC80609A09 ID No. : No.27

Customer : Thai Environmental Technic Limited.  
1/6 Soi Ramkhamhaeng 145,  
Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1012.1 hPa

**NATIONAL STANDARD WIND TUNNEL :**

: Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by

Mr. Watcha

Mechanical Engineer





# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## The Result of Calibration

Certification No. 375/23

24 October, 2023

Page : 2 of 2


Standard Ultrasonic Anemometer	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacumm inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.04	-	-	-	6.7	0.34
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.7	0.31
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.8	0.21
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Mr. [REDACTED]

Mechanical Engineer

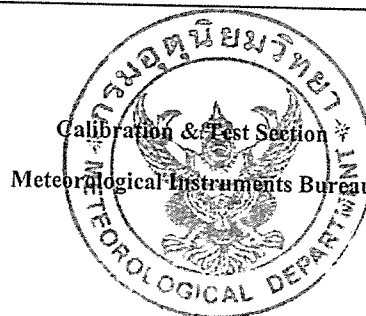



*THAI METEOROLOGICAL DEPARTMENT*

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

**Calibration Certificate**

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 13 September, 2023

Certification No. 315/23

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Weather Wizard III

Serial No. : WE61121A25A ID No. : No.23

Customer : Thai Environmental Technic Limited.  
1/6 Soi Ramkhamhaeng 145,  
Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1008.6 hPa

NATIONAL STANDARD WIND TUNNEL :

: Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023


N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

Calibrated by  
Mr. Watcha  
Mechanical Engineer





## THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

### The Result of Calibration

Certification No. 315/23

13 September, 2023


Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacumm inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.4	0.60
3.02	-	-	-	2.2	0.82
5.00	-	-	-	4.5	0.50
7.00	-	-	-	6.3	0.70
9.02	-	-	-	8.5	0.52
11.01	-	-	-	10.3	0.71
13.01	-	-	-	12.5	0.51
15.01	-	-	-	14.3	0.71
17.02	-	-	-	16.5	0.52
20.02	-	-	-	19.3	0.72

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by

Mr. Watcharapoi Subwat  
Mechanical Engineer

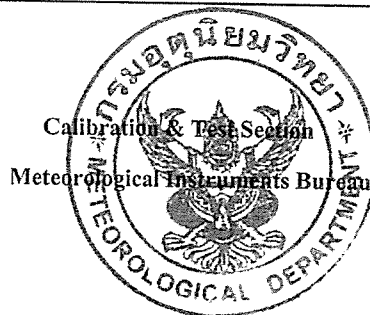



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 21 June, 2023

Certification No. 218/23

Page : 1 of 2

Object : Wind speed and wind direction

Manufacturer : Davis Instruments Inc.

Type : Weather Wizard III

Serial No. : WC40105A43 ID No. : No.8

Customer : Thai Environmental Technic Limited.  
1/6 Soi Ramkhamhaeng 145,  
Khwaeng/Khet Saphan Sung, Bangkok 10240.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1008.5 hPa

NATIONAL STANDARD WIND TUNNEL :

: Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 Pitot Tube Theodor Friedrichs Type 0800.0000 serial 9023

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)


JAPAN QUALITY ASSURANCE ORGANIZATION

: Standard Velocity at 0 - 20 m/sec

Calibrated by

Mr. Watchapol Subwat

Mechanical Engineer

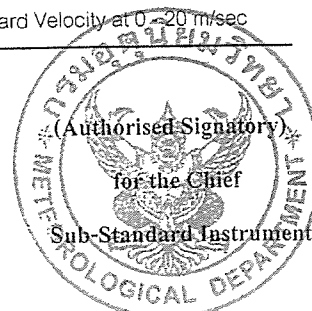



## THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

### The Result of Calibration

Certification No. 218/23


21 June, 2023

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H <sub>2</sub> O	Vacumm inches H <sub>2</sub> O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	0.9	0.10
3.02	-	-	-	2.7	0.32
5.00	-	-	-	4.9	0.10
7.00	-	-	-	6.7	0.30
9.02	-	-	-	8.9	0.12
11.01	-	-	-	10.7	0.31
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.7	0.31
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.7	0.32

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270


Calibrated by :



Mr. Watcharapol Subwat  
Mechanical Engineer







### Personal Pump Calibration Report

Equipment Type : Personal Pump/Parameter  
Equipment Range : 0.1-7.0 l/min  
Calibration Range : 0.1-4.0 l/min  
Calibration Type : Drycal  
Calibration S/N : 4491

Item	Personal Pump S/N	Hi Flow/Low Flow	ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	Average	Uncertainty
1.	20140505103	2.5	2.4970	2.4980	2.4990	2.4980	±0.0010
2.	20120103081	2.0	1.9960	1.9970	1.9980	1.9970	±0.0010
3.	20110505116	2.0	1.9970	1.9980	1.9990	1.9980	±0.0010
4.	20120202031	2.0	1.9950	1.9960	1.9970	1.9960	±0.0010
5.	20120202045	2.0	1.9970	1.9980	1.9990	1.9980	±0.0010
6.	20111001074	0.2	0.1986	0.1989	0.1991	0.1989	±0.0003

Calibration Date 14 / 03 / 67

Calibration By ปิยวิมล หัก

Remark : Uncertainty Type A =  $\frac{\sigma}{\sqrt{n}}$  = SD

: SD = Standard deviation

:  $\bar{X}$  = Mean





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23MM161

Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Electronic Balance

**Manufacturer :** Mettler Toledo

**Model :** XP205DR

**Serial No. :** 1129273885

**ID No. :** -

**Submitted by :** Thai Environmental Technic Limited  
1/6 Soi Ramkhamhaeng 145,  
Khwaeng/Khet Saphan Sung,  
Bangkok 10240

**Location :** Balance Room

**Received order :** 10 April 2023  
**Calibration Date :** 11 April 2023  
**Ambient Temperature :** 15 °C to 40 °C  
**Relative Humidity :** 30 % to 90 %

**Calibrated by :** Khit Ruttanaprapachai

**Approved by :** Malee Butkruea  
Approved Signatory

( ) Pornthippa Tameyakul  
(✓) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 25 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0053465



Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2304-0146OC-13

Cert.No.: 23MM161  
Page: 2 of 3

**Procedure used :-**

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

**Condition of this result of calibration**

1. Reference standard instruments:-

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Test report No.</u>	<u>Due date</u>
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

**Result of calibration** ( ) Without Adjustment ( \* ) After Adjustment by Internal Calibration

<b>Range capacity :</b>	0 g to 81 g	<b>Resolution</b>	0.00001 g
	81 g to 220 g	<b>Resolution</b>	0.0001 g

**Before Adjustment :**

<u>Applied Weight</u> ( g )	<u>Balance Reading</u> ( g )	<u>Correction</u> ( g )	<u>Measurement Uncertainty</u> ( $\pm$ mg )	<u>Coverage Factor</u> ( k )
80	79.99946	+0.00054	0.15	2.00
200	199.9984	+0.0016	0.30	2.00

**After Adjustment :**

1. Determination of the standard deviation of weighing machine

( n = 10 )

<u>Applied Weight</u> ( g )	<u>Standard Deviation of Reading ( g )</u>
80	0.000023
200	0.00008

*Mlu.*



Equipment : Electronic Balance  
Condition As-Received : Used Item  
Reference : 2304-0146OC-13  
Result of calibration

## 2. Effect of off center loading

A mass of 100 g was placed at various positions on the pan.  
The weighing machine reading error obtained is given in the table

Position 1	Position 2	Position 3	Position 4	Position 5
(g)	(g)	(g)	(g)	(g)
-0.0001	-0.0001	-0.0002	-0.0001	0.0000

## 3. Departure from nominal value


Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	( $\pm$ mg)	(k)
Unload	0.00000	0.00000	0.038	2.28
0.01	0.01000	0.00000	0.039	2.28
0.05	0.05000	0.00000	0.039	2.28
1	1.00001	-0.00001	0.040	2.23
2	2.00001	-0.00001	0.040	2.23
5	5.00001	-0.00001	0.042	2.17
10	10.00001	-0.00001	0.045	2.13
20	20.00001	-0.00001	0.051	2.06
50	49.99998	+0.00002	0.085	2.00
80	80.00002	-0.00002	0.15	2.00
200	199.9999	+0.0001	0.30	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

Cert.No.: 23MM161

Page: 3 of 3

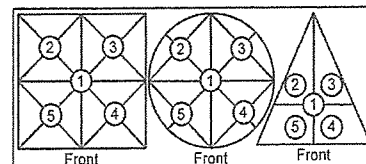

Maximum difference between  
off-center and central loading  
(g)  
0.0001

Malu

a 1158496



# Agilent CrossLab Start Up Services Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

## Introduction

### Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

### Important Customer Web Links

- For more information about **Agilent Technologies services**, please visit our website using the following URL: <http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair>
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>.
- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: <https://www.agilent.com/en-us/agilentresources>.
- Need technical support, FAQs, supplies? – visit our **Support Home page** <http://www.agilent.com/search/support>.
- **Videos** about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>.
- **7890B Manuals** are also available on Agilent.com:
  - **Safety**  
[https://www.agilent.com/cs/library/usermanuals/public/7890B\\_Safety.pdf](https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf)
  - **Installation and First Startup**  
[https://www.agilent.com/cs/library/usermanuals/Public/7890B\\_Installation.pdf](https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf)
  - **Operation Manual**  
[https://www.agilent.com/cs/library/usermanuals/Public/7890B\\_Operation.pdf](https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf)
  - **Maintaining Your GC**  
<https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B-Maintaining%20Guide.pdf>



## Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "**Section not applicable**" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- ***Ask the customer to sign the Service Completion section including the customer's and your signature.***

## Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

## System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table below.

<b>Instrument System Name and ID</b>	Ins-LAB-010 / CN16343040
<b>Instrument System Site and Location</b>	Thai Enviromental Technic Ltd / Lab

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3440B	CN16343040
2. G4513A	CN16350082
3. G4514A	CN16400014
4.	
5.	
6.	
7.	
8.	
9.	
10.	

## Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components, settings as defined by current Service Notes.
- ☒ Check for required firmware updates and verify with customers if they would like them installed.
- ☒ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

## Preventive Maintenance Procedure

### Clean and inspect GC

- ☐ Unplug power cord from the power source.
- ☐ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☐ Inspect internal connectors for proper contact and placement.
- ☐ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☐ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☐ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☐ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

### Inlet and detector consumable replacement

- ☐ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – “Maintaining Your GC” - for the inlet(s) installed.
- ☐ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☐ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☐ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

### Zero Sensors and Leak test

- ☐ Zero all pressure sensors per the procedure in the 7890 “Advanced User Guide”.
- ☐ Perform inlet pressure decay test(s) as defined in the 7890 “Troubleshooting Manual”.  
If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☐ Record if test passed or failed in the results table.

## ALS Maintenance

☐ **Section NOT applicable**

- ☒ Check all cabling and configuration settings between GC, tray, and injectors.
- ☒ Vacuum or remove any dust, especially around fans.
- ☒ Check operation of all fans.
- ☒ Check syringe for smooth plunger operation.
- ☒ Check for smooth operation of the needle support – clean if necessary

## Restore Instrument

- ☒ Restore the normal operating conditions or customer method using the Data System.
- ☒ Purge the system with carrier flow for 15 minutes
- ☒ Bake out the system, then restore the normal operating conditions
- ☒ After equilibration, check and record the post PM detector signal output values.  
Results should be similar or lower than the detector outputs recorded prior to PM.
- ☒ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

## Signature Page

### Service Review

- ☐ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review with the customer this service, parts replaced, and test results obtained.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

### 7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output	N/A	17.0/FID
Back detector output	N/A	1101/ $\mu$ ECD (unused)
AUX detector output	N/A	99.3/TCD (unused)
Pressure decay test	Expected test result	Actual test result
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	Pass

## 7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	1
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	N/A
PP Inlet PM kit	5188-6498	7890A/B	N/A
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	N/A
MMI Cleaning Kit	G3510-60820	7890A/B	N/A
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	N/A
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	N/A
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	1
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	N/A
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	1
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	N/A
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	N/A
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	N/A
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	N/A
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	N/A
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	N/A
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	N/A

Revision: 2.01, Issued: September 15, 2021

Agile Document Number: D0013618

DE number: 44166.759722222

© Agilent Technologies, Inc. 2021

## Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

## Service Completion

Service request number [REDACTED] Date service completed 25 Sep 2023  
Agilent signature [REDACTED] Customer signature [REDACTED]  
Total number of pages in this document 9 pages





## Gas Detector Certificate

Issued By	Sithiporn Associates Company Limited		
Owner Name	Thai Environmental Technic Limited		
Reference Number	SVO27504	Calibration Date	29-Jan-24
Product Brand	BW Technologies	Calibration Due	28-Jan-25
Type Systematic	Portable	Calibration Temp.	25°C
Battery Type	3 V Lithium Energizer (CR2) 1 pcs.	Calibration Humidity	65%RH

Product Model	Gas Alert Extreme CO	Serial Number	J617-M027776
Sensor Model	SR-M04-SC	Visual Gas Alarm	Red Light
Detection Gasses	Measuring Range	Detection Principles	
Carbon monoxide (CO)	0-1000 ppm in 1 ppm increments	Electrochemical cell	

Calibration Standard equipment : Std Gas Mixtures Cylinder Number 955-643239 Expired Date 04-Oct-25

Components	Concentration
Methane (CH <sub>4</sub> )	50.0 %LEL (2.5 %vol.)
Hydrogen Sulfide(H <sub>2</sub> S)	25.0 ppm
Carbon Monoxide(CO)	100.0 ppm
Oxygen (O <sub>2</sub> )	18.0 %Vol.

## Calibration Result

Item Calibration	Fresh Air			Standard Gas			Standrad Drift	Unit	*90%T (second)
	Before	Calibration	After	Before	Calibration	After			
Carbon monoxide (CO)	0	0	0	94	100	100	0	ppm	19

\*90 %T is respond time reading to 90% of standard gas

Gas Alarm Preset	Low Alarm	High Alarm	TWA	STEL	Unit
Carbon monoxide (CO)	35	200	35	200	ppm

## Operation Test

Function	Battery Indicate	Sampling Module	Self-Test	Gas Display	Alarm Report	PC/Data Collection	Alarm Functional		
							Audible	Visual	Vibration
Judgement	Pass	N/A	Pass	Pass	Pass	N/A	Pass	Pass	Pass

บริษัท ลิททิพรแอสโซซิเอต จำกัด

Remarks : SITHIPORN ASSOCIATES COMPANY LIMITED

Signature

Approved



Calgaz Ltd  
Unit 21/22, Rosevale Road  
Parkhouse Industrial Estate West  
Newcastle-under-Lyme  
Staffordshire  
ST5 7EF  
United Kingdom

info@calgaz.com  
Phone: +44 1782 566 897

## Certificate Of Composition WO420382 - 5

Part Code: C006852  
10ALQUAD-003-LUX

Customer: Calgaz International LLC  
Customer Order Number: PO23799/SO33513 SEI001

Cylinder No: 955-643239  
Cylinder Valve: C10  
Gross Weight: 1.5  
Nett Weight: 0.12

Component	Requested Values	Certified Values	Accuracy
Carbon Monoxide	100 ppm	100 ppm	+/- 2%
Oxygen	18 %	18 %	+/- 2%
Methane	2.5 %	2.5 %	+/- 2%
Hydrogen Sulphide	25 ppm	25 ppm	+/- 5%
Nitrogen	Balance	Balance	

Pressure: 1000 psi      Volume: 1.6 ltr      Size: 10AL

Please note all units are in mol % and methods used in analysis per WIN6 include, Chemiluminescence, Paramagnetic, NDIR, UV-VIS, GC (FID/TCD), Electrochemical cells, Zirconia, PID and Gravimetric. Product composition is verified by direct comparison to calibration standards traceable to NPL, NIST or equivalent National Standard weights or gas mixture reference materials. Traceable reference: 35903595 / 27605229 / 27605263.

Manufactured Date: 04/10/2023

Valid Until: 04/10/2025

UN 1956 Compressed gas, n.o.s.

(Oxygen, Nitrogen Mixture)

Certified By: Craig.Nichols

All Gas Mixtures that are quoted with a balance of Air contain 20.9% (+/-2%) Oxygen relative to the overall Gas Mixture

**The gases contained in this cylinder are not breathing gases.  
DO NOT INHALE**

บริษัท สิทธิพรแอสโซซิเอต จำกัด  
SITHIPORN ASSOCIATES COMPANY LIMITED


BANGKOK INDUSTRIAL GAS CO., LTD.

11<sup>th</sup> Floor Rajanekarn Building

3 South Sathorn Rd, Yanawa, Sathorn

Bangkok 10120, Thailand

Tel. : (662) 685-6789 Fax : (662) 685-6790-1



## CERTIFICATE OF CONFORMITY (For Package Gases)

Customer Name : Sithiporn Associates Co., Ltd.

Product Name : Nitrogen

Certificate No. : QC15B6-4298

Date of Issue : 12 DEC '21

Gas Content : 7 M<sup>3</sup>

Lot. No. : 171215N201/DO3300016058

Shelf Life : 36 months

Page no. : 1/1

Cylinder Valve Type : CGA 580

Components	Specification
Oxygen	< 2 ppm
Moisture	< 3 ppm
Carbon Dioxide	< 1 ppm
Carbon Monoxide	< 1 ppm
Total Hydrocarbon as CH <sub>4</sub>	< 1 ppm
Nitrogen	> 99.999 %

Cylinders' Number

M5281014

13D007140

บริษัท สิทธิพรแอสโซซิเอต จำกัด  
SITHIPORN ASSOCIATES COMPANY LIMITED

Signed: [Redacted Signature]





# Certificate of Calibrator

## for ST-120 Sound Calibrator

No. 20231221J143

Name of Product Sound Calibrator


Type ST-120

Serial Number ST120C0263E

Specification Class 1

Date 2023/12/21

Tested by

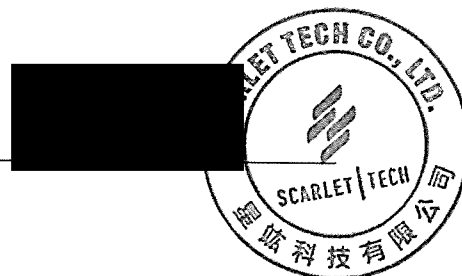

1. Outside : OK  
2. Sound Pressure Level : 93.97 dB ; 114.03 dB  
3. Frequency : 998.30 Hz  
4. Distortion : 1.15 % ; 1.35 %

### Environment conditions :

Air temperature : 18 °C  
Relative humidity : 62 %  
Static pressure : 101.9 kPa

**Scarlet Tech Co., Ltd.**

4F-3, No. 347, HePing E Rd, 2nd Sec, DaAn District, Taipei City 106, Taiwan  
E-mail: info@scarlet.com.tw    www.scarlet-tech.com






# CERTIFICATE OF CALIBRATION

NO. 20231214061

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820393
Specification:	Class1
Conclusion:	Pass
Date of calibration:	2023-12-14
Due Date:	2024-12-13

Calibrated by



- This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-52174

3. Adjustments to indicated sound levels:

Type of Calibrator B&K 4231 Sound

Pressure Level 94.0 dB

4. Measuring up limit: 140 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.1	-14.6	0.2	1000	0.0	0.0	-0.1
20	-50.3	-6.4	-0.3	2000	0.1	0.0	0.0
31.5	-39.4	-2.1	0.1	4000	1.2	-0.1	0.0
63	-26.1	-0.4	-0.1	8000	1.2	-0.8	0.0
125	-16.4	-0.1	-0.1	12500	-5.2	-7.2	0.1
250	-8.6	0.1	0.0	16000	-11.5	-13.3	0.2
500	-3.1	0.1	0.1	20000	-23.4	-25.8	-0.3

## 6. Self-generated noise

Microphone replaced by electrical input signal device

7.7 dB(A)	8.4 dB(C)	13.9 dB(Z)
-----------	-----------	------------

## 7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.2
Rate of the S weighting decrease (dB/s)	4.2
Deviation of F&S	-0.1

## 8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

## 9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-18.1	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

## 10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.4	2.4	2.3	2.4

## 11. Overload indication: Pass

## 12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.



Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
<b>LAeq,T</b>	103.2	103.2	0.0
<b>L5</b>	110.8	110.8	0.0
<b>L10</b>	108.8	108.8	0.0
<b>L50</b>	92.9	92.8	0.1
<b>L90</b>	76.9	76.8	0.1
<b>L95</b>	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

**Environment conditions:**

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

**Reference equipment used in the calibration:**

Description:	Model	Serial No.	Expiry Date	Traceable To
<b>Microphone</b>	B&K 4191	2929405	2024-12-15	NML
<b>Multi function sound calibrator</b>	B&K 4226	2288444	2024-10-15	CIGISMEC
<b>Signal generator</b>	DS 360	33873	2024-10-15	CEPREI

**Test specifications:**

1. All Scalet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of ±20%.
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

**References:**

IEC 61672-3 Sound Level Meters Part 3: Periodic tests






# CERTIFICATE OF CALIBRATION

NO. 20231130186

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	821293
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-04
Due Date:	2025-01-03

Calibrated by:



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-57087

4. Measuring up limit: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests. )

Type of Calibrator B&K 4231

Sound Pressure Level 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.1	-14.7	-0.9	1000	0.1	0.0	0.0
20	-50.2	-6.1	-0.2	2000	1.3	-0.1	-0.1
31.5	-39.5	-3.0	-0.2	4000	1.2	-0.7	0.0
63	-26.2	-0.8	-0.1	8000	-1.1	-3.1	0.0
125	-16.2	-0.2	0.1	12500	-6.0	-7.9	-0.1
250	-8.6	0.0	-0.1	16000	-11.8	-13.8	0.0
500	-3.3	0.0	0.0	20000	-23.9	-25.9	-0.2

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L <sub>Aeq,T</sub>	103.2	103.2	0.0
L <sub>5</sub>	110.8	110.8	0.0
L <sub>10</sub>	108.8	108.8	0.0
L <sub>50</sub>	92.9	92.8	0.1
L <sub>90</sub>	76.9	76.8	0.1
L <sub>95</sub>	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

**Environment conditions:**

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

**Reference equipment used in the calibration:**

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2025-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2025-10-15	CIGISMEC
Signal generator	DS 360	33873	2025-10-15	CEPREI

**Test specifications:**

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of  $\pm 20\%$ .
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

**References:**

IEC 61672-3 Sound Level Meters Part 3: Periodic tests




## CERTIFICATE OF CALIBRATION

NO. 20231130187

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	821294
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-04
Due Date:	2025-01-03

Calibrated by:



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-57484

4. Measuring up limit: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests. )

Type of Calibrator B&K 4231

Sound Pressure Level 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-70.8	-14.5	-0.8	1000	0.1	0.0	0.0
20	-50.2	-6.2	-0.1	2000	1.3	-0.1	-0.1
31.5	-39.4	-3.0	-0.2	4000	1.2	-0.7	0.0
63	-26.2	-0.8	-0.1	8000	-1.1	-3.1	0.0
125	-16.2	-0.2	0.1	12500	-6.0	-7.9	-0.1
250	-8.7	0.0	-0.1	16000	-11.8	-13.8	0.0
500	-3.2	0.0	0.0	20000	-23.8	-25.8	-0.2

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L <sub>Aeq,T</sub>	103.2	103.2	0.0
L <sub>5</sub>	110.8	110.8	0.0
L <sub>10</sub>	108.8	108.8	0.0
L <sub>50</sub>	92.9	92.8	0.1
L <sub>90</sub>	76.9	76.8	0.1
L <sub>95</sub>	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

**Environment conditions:**

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

**Reference equipment used in the calibration:**

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2025-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2025-10-15	CIGISMEC
Signal generator	DS 360	33873	2025-10-15	CEPREI

**Test specifications:**

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of  $\pm 20\%$ .
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

**References:**

IEC 61672-3 Sound Level Meters Part 3: Periodic tests




## CERTIFICATE OF CALIBRATION

NO. 20231130191

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	821298
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-04
Due Date:	2025-01-03

Calibrated by:



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-57090

4. Measuring up limit: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests. )

Type of Calibrator B&K 4231

Sound Pressure Level 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.1	-14.4	-1.0	1000	0.0	0.0	0.0
20	-50.2	-6.1	-0.2	2000	1.3	-0.1	0.0
31.5	-39.4	-2.9	0.0	4000	1.2	-0.7	0.0
63	-26.1	-0.8	-0.1	8000	-1.0	-3.0	0.0
125	-16.1	-0.2	0.0	12500	-6.0	-7.9	-0.1
250	-8.6	0.0	0.0	16000	-11.8	-13.8	0.0
500	-3.2	0.0	0.0	20000	-23.8	-25.8	-0.2

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L <sub>Aeq,T</sub>	103.2	103.2	0.0
L <sub>5</sub>	110.8	110.8	0.0
L <sub>10</sub>	108.8	108.8	0.0
L <sub>50</sub>	92.9	92.8	0.1
L <sub>90</sub>	76.9	76.8	0.1
L <sub>95</sub>	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

**Environment conditions:**

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

**Reference equipment used in the calibration:**

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2025-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2025-10-15	CIGISMEC
Signal generator	DS 360	33873	2025-10-15	CEPREI

**Test specifications:**

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of  $\pm 20\%$ .
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

**References:**

IEC 61672-3 Sound Level Meters Part 3: Periodic tests






## CERTIFICATE OF CALIBRATION

NO. 20231130192

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	821299
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-04
Due Date:	2025-01-03

Calibrated



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-60004

4. Measuring up limit: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests. )

Type of Calibrator B&K 4231

Sound Pressure Level 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-70.6	-14.5	-0.8	1000	0.1	0.0	0.0
20	-50.1	-6.1	-0.3	2000	1.3	-0.1	0.0
31.5	-39.3	-3.0	0.0	4000	1.2	-0.7	0.0
63	-26.1	-0.8	-0.1	8000	-1.0	-3.0	0.0
125	-16.1	-0.1	0.0	12500	-6.0	-7.9	-0.1
250	-8.6	0.0	0.0	16000	-11.7	-13.7	0.0
500	-3.1	0.1	0.0	20000	-23.8	-25.8	-0.2

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L <sub>Aeq,T</sub>	103.2	103.2	0.0
L <sub>5</sub>	110.8	110.8	0.0
L <sub>10</sub>	108.8	108.8	0.0
L <sub>50</sub>	92.9	92.8	0.1
L <sub>90</sub>	76.9	76.8	0.1
L <sub>95</sub>	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

**Environment conditions:**

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

**Reference equipment used in the calibration:**

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2025-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2025-10-15	CIGISMEC
Signal generator	DS 360	33873	2025-10-15	CEPREI

**Test specifications:**

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of  $\pm 20\%$ .
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

**References:**


IEC 61672-3 Sound Level Meters Part 3: Periodic tests



## CERTIFICATE OF CALIBRATION

NO. 20240130117

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820877
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-30
Due Date:	2025-01-29

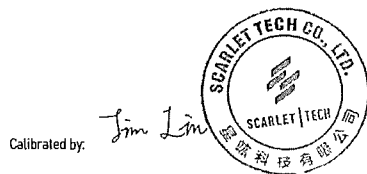

- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass them, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-50891

3. Adjustments to indicated sound levels:

Type of Calibrator B&K 4231 Sound

Pressure Level 94.0 dB

4. Measuring up limit: 140 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.1	-14.6	-0.1	1000	0.0	0.0	-0.1
20	-50.3	-6.1	-0.2	2000	1.1	-0.1	-0.1
31.5	-39.3	-2.9	0.0	4000	1.4	-0.8	-0.1
63	-26.1	-0.8	0.0	8000	1.2	-3.1	0.0
125	-16.1	-0.1	0.0	12500	5.8	-7.8	0.0
250	-8.6	0.1	0.0	16000	-11.3	-13.6	0.1
500	-3.1	0.1	0.0	20000	-23.5	-25.9	-0.1

### 6. Self-generated noise

Microphone replaced by electrical input signal device

7.3 dB(A)	7.8 dB(C)	14.8 dB(Z)
-----------	-----------	------------

### 7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.2
Rate of the S weighting decrease (dB/s)	4.4
Deviation of F&S	-0.1

### 8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

### 9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LA Fmax-LA	LA Smax-LA	LA E-LA	LA eqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-18.1	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

### 10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.4	2.4	2.3	2.4

### 11. Overload indication: Pass

### 12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
LAeq,T	103.2	103.2	0.0
L5	110.8	110.8	0.0
L10	108.8	108.8	0.0
L50	92.9	92.8	0.1
L90	76.9	76.8	0.1
L95	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2024-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2024-10-15	CIGISMEC
Signal generator	DS 360	33873	2024-10-15	CEPREI

Test specifications:

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of ±20%.
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests



## CERTIFICATE OF CALIBRATION

NO. 20240130118

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820878
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-30
Due Date:	2025-01-29

Calibrated by



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass them, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-52493

3. Adjustments to indicated sound levels:

Type of Calibrator: B&K 4231 Sound

Pressure Level: 94.0 dB

4. Measuring up limit: 140 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.1	-14.5	-0.1	1000	0.0	0.0	-0.1
20	-50.3	-6.2	-0.3	2000	0.0	-0.1	-0.1
31.5	-39.4	-3.0	-0.3	4000	1.3	-0.2	-0.1
63	-26.2	-0.8	-0.1	8000	1.1	-0.7	0.0
125	-16.2	-0.2	-0.1	12500	5.9	-7.8	0.0
250	-8.6	0.1	-0.1	16000	-11.6	-13.7	0.1
500	-3.2	0.1	-0.1	20000	-23.8	-25.8	-0.1

### 6. Self-generated noise

Microphone replaced by electrical input signal device

9.1 dB(A)	10.7 dB(C)	15.0 dB(Z)
-----------	------------	------------

### 7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.2
Rate of the S weighting decrease (dB/s)	4.4
Deviation of F&S	0.0

### 8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

### 9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-18.1	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

### 10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.4	2.4	2.3	2.4

11. Overload indication: Pass

### 12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
LAeq,T	103.2	103.2	0.0
L5	110.8	110.8	0.0
L10	108.8	108.8	0.0
L50	92.9	92.8	0.1
L90	76.9	76.8	0.1
L95	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2024-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2024-10-15	CIGISMEC
Signal generator	DS 360	33873	2024-10-15	CEPREI

Test specifications:

- All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
- The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of ±20%.
- The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests



## CERTIFICATE OF CALIBRATION

NO. 20231130187

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	821294
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-04
Due Date:	2025-01-03

Calibrated by:



- This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-57484

4. Measuring up limit: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Type of Calibrator B&K 4231

Sound Pressure Level 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-70.8	-14.5	-0.8	1000	0.1	0.0	0.0
20	-50.2	-6.2	-0.1	2000	1.3	-0.1	-0.1
31.5	-39.4	-3.0	-0.2	4000	1.2	-0.7	0.0
63	-26.2	-0.8	-0.1	8000	-1.1	-3.1	0.0
125	-16.2	-0.2	0.1	12500	-6.0	-7.9	-0.1
250	-8.7	0.0	-0.1	16000	-11.8	-13.0	0.0
500	-3.2	0.0	0.0	20000	-23.8	-25.8	-0.2

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
LAeq,T	103.2	103.2	0.0
L5	110.8	110.8	0.0
L10	108.8	108.8	0.0
L50	92.9	92.8	0.1
L90	76.9	76.8	0.1
L95	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C  
Relative humidity: 50 %  
Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2025-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2025-10-15	CIGISMEC
Signal generator	DS 360	33873	2025-10-15	CEPREI

Test specifications:

- All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
- The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of  $\pm 20\%$ .
- The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests







## CERTIFICATE OF CALIBRATION

NO. 20231130188

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	821295
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-04
Due Date:	2025-01-03

Calibrated by:



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass them, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-57346

4. Measuring up limits: 140 dBA

3. Adjustments to indicated sound levels:

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Type of Calibrator B&K 4231

Sound Pressure Level 94.0 dB

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-70.6	-14.6	-0.9	1000	0.1	0.0	0.0
20	-50.3	-6.0	-0.2	2000	1.4	-0.1	0.0
31.5	-39.3	-2.9	-0.2	4000	1.2	-0.7	0.0
63	-26.1	-0.8	-0.1	8000	-1.0	-3.0	0.0
125	-16.1	-0.2	0.0	12500	-6.0	-7.9	-0.1
250	-8.6	0.0	0.0	16000	-11.7	-13.7	0.0
500	-3.1	0.1	0.0	20000	-23.8	-25.8	-0.2

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
LAeq,T	103.2	103.2	0.0
L5	110.8	110.8	0.0
L10	108.8	108.8	0.0
L50	92.9	92.8	0.1
L90	76.9	76.8	0.1
L95	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2025-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2025-10-15	CIGISMEC
Signal generator	DS 360	33873	2025-10-15	CEPREI

Test specifications:

- All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
- The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of  $\pm 20\%$ .
- The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests






CERTIFICATE OF CALIBRATION

NO. 20231214062

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820394
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2023-12-14
Due Date:	2024-12-13

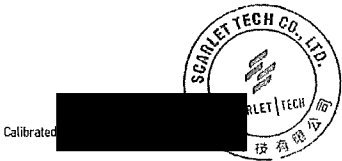

- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpasses then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AYA14425-52756

3. Adjustments to indicated sound levels:

Type of Calibrator\_B&K 4231 Sound

Pressure Level\_94.0 dB

4. Measuring up limit: 140.dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.1	-14.4	0.2	1000	0.0	0.0	-0.1
20	-50.3	-6.4	-0.3	2000	0.1	0.0	0.0
31.5	-39.4	-2.2	0.1	4000	1.2	-0.1	0.0
63	-26.1	-0.3	-0.1	8000	1.2	-0.8	0.0
125	-16.1	-0.1	-0.1	12500	-5.2	-7.2	0.1
250	-8.5	0.1	0.0	16000	-11.5	-13.4	0.2
500	-3.2	0.1	0.1	20000	-23.4	-25.8	-0.3

6. Self-generated noise

Microphone replaced by electrical input signal device

10.8 dB(A)	10.3 dB(C)	15.8 dB(Z)
------------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.1
Rate of the S weighting decrease (dB/s)	4.1
Deviation of F&S	-0.1

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-18.1	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.4	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L <sub>Aeq,T</sub>	103.2	103.2	0.0
L <sub>5</sub>	110.8	110.8	0.0
L <sub>10</sub>	108.8	108.8	0.0
L <sub>50</sub>	92.9	92.8	0.1
L <sub>90</sub>	76.9	76.8	0.1
L <sub>95</sub>	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C  
Relative humidity: 50 %  
Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2024-12-15	NIML
Multi function sound calibrator	B&K 4226	2288444	2024-10-15	CIGISMEC
Signal generator	DS 360	33873	2024-10-15	CEPREI

Test specifications:

- All Scarlett's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
- The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of ±20%.
- The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests



ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24020337-5

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan  
Sung, Bangkok 10240, Thailand.

Equipment Name : Noise Dose Meter

Manufacturer : SOUNDTEK

Model : ST-130

Serial Number : 200300134

ID. Number : No.29

### Environmental Conditions

Ambient Temperature :  $23\text{ }^{\circ}\text{C} \pm 3\text{ }^{\circ}\text{C}$

Received Date : 21 Feb 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 23 Feb 2024

Location of Calibration : In-Lab

Recommend Due Date : 23 Feb 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 24 Feb 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Karoon Pengsalung

Approved by :

Calibration Officer

( Mr.Nirut Loha )

Authorized Signatory



# Calibration Report

Certificate Number : SPR24020337-5

Page : 2 of 3

## Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

## Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research

69/29 Moo 1 Klongsi Klonguang Pathumtham 12120 ( Thailand ) Tel: (662) 193-2220 5 ไร่ 13 งาน 10 ตารางวา [www.southernbuddhism.com](http://www.southernbuddhism.com)



ID LINE : IEC17025



## Result of Calibration

Certificate No. : SPR24020337-5

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	113.9	113.9	-0.1	-0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.


### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.


- End of Certificate -







ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24020220-34

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan  
Sung, Bangkok 10240, Thailand.

Equipment Name : Noise Dose Meter

Manufacturer : SOUNDTEK

Model : ST-130

Serial Number : 220100050

ID. Number : No.30

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 14 Feb 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 15 Feb 2024

Location of Calibration : In-Lab

Recommend Due Date : 15 Feb 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 16 Feb 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul


Approved by :

Calibration Officer

Authorized Signatory



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24020220-34

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

### Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



## Result of Calibration

Certificate No. : SPR24020220-34

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -





ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24020220-35

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan  
Sung, Bangkok 10240, Thailand.

Equipment Name : Noise Dose Meter

Manufacturer : SOUNDTEK

Model : ST-130

Serial Number : 220100051

ID. Number : No.31

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 14 Feb 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 15 Feb 2024

Location of Calibration : In-Lab

Recommend Due Date : 15 Feb 2025

Calibration Procedure : SP-CPE-04-01

Date of Issue : 16 Feb 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Approved by :

Calibration Officer

Authorized Signatory



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24020220-35

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 140/0167	26 Jan 2025

### Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



## Result of Calibration

Certificate No. : SPR24020220-35

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty ( ± )
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -







ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24020220-29

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan  
Sung, Bangkok 10240, Thailand.

Equipment Name : Liquid in Glass Thermometer

Manufacturer : AMA

Model : N/A

Serial Number : 2197259

ID. Number : N/A

### Environmental Conditions

Ambient Temperature :  $23\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$

Received Date : 14 Feb 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 15 Feb 2024

Location of Calibration : In-Lab

Recommend Due Date : 15 Feb 2025

Calibration Procedure : SP-CPT-04-08

Date of Issue : 16 Feb 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Jirasak Pumbut

Approved by :

Calibration Officer

Authorized Signatory



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24020220-29

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Super Thermometer with PRT	1575/3850-40-392	58087/100288	PSL-T 0400/66	15 Feb 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



## Result of Calibration

Certificate No. : SPR24020220-29

Page : 3 of 3

Range : -5 to 110 °C

Resolution : 0.5 °C

Unit : °C

Setting Value	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
25.0	25.008	25.0	-0.008	0.29
30.0	30.008	30.0	-0.008	0.29
35.0	35.009	35.0	-0.009	0.29
40.0	40.010	40.0	-0.010	0.29
45.0	45.012	45.0	-0.012	0.29
50.0	50.014	50.0	-0.014	0.29

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -





ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24020220-28

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan  
Sung, Bangkok 10240, Thailand.

Equipment Name : Liquid in Glass Thermometer

Manufacturer : AMA

Model : N/A

Serial Number : 2197260

ID. Number : N/A

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Received Date : 14 Feb 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 15 Feb 2024

Location of Calibration : In-Lab

Recommend Due Date : 15 Feb 2025

Calibration Procedure : SP-CPT-04-08

Date of Issue : 16 Feb 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Jirasak Pumbut

Approved by

Calibration Officer

Authorized Signatory



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24020220-28

Page : 2 of 3


### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Super Thermometer with PRT	1575/3850-40-392	58087/100288	PSL-T 0400/66	15 Feb 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



## Result of Calibration

Certificate No. : SPR24020220-28

Page : 3 of 3

Range :        -5        to        110    °C

Resolution : 0.5 °C

Unit : °C

Setting Value	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
25.0	25.006	25.0	-0.006	0.29
30.0	30.007	30.0	-0.007	0.29
35.0	35.008	35.0	-0.008	0.29
40.0	40.009	40.0	-0.009	0.29
45.0	45.011	45.0	-0.011	0.29
50.0	50.012	50.0	-0.012	0.29

Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -







ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24020220-27

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan  
Sung, Bangkok 10240, Thailand.

Equipment Name : Liquid in Glass Thermometer

Manufacturer : AMA

Model : N/A

Serial Number : 2197261

ID. Number : N/A

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Received Date : 14 Feb 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 15 Feb 2024

Location of Calibration : In-Lab

Recommend Due Date : 15 Feb 2025

Calibration Procedure : SP-CPT-04-08

Date of Issue : 16 Feb 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Jirasak Pumbut

Approved by :

Calibration Officer

Authorized Signatory



ID LINE : IEC17025



# Calibration Report

Certificate Number : SPR24020220-27

Page : 2 of 3

## Reference Standards


Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Super Thermometer with PRT	1575/3850-40-392	58087/100288	PSL-T 0400/66	15 Feb 2024

## Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research

69/29 Moo 1 Klongsi Klongluang Pathumthani 12120 ( Thailand ) Tel: (662) 193-2220 5 คู่สาย [www.สออบไทยบดรีดผงอัจฉริยะ.com](http://www.สออบไทยบดรีดผงอัจฉริยะ.com)



ID LINE : IEC17025



## Result of Calibration

Certificate No. : SPR24020220-27

Page : 3 of 3

Range : -5 to 110 °C

Resolution : 0.5 °C

Unit : °C

Setting Value	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
25.0	25.007	25.0	-0.007	0.29
30.0	30.008	30.0	-0.008	0.29
35.0	35.008	35.0	-0.008	0.29
40.0	40.009	40.0	-0.009	0.29
45.0	45.011	45.0	-0.011	0.29
50.0	50.012	50.0	-0.012	0.29

### Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -





ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24020220-23

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan  
Sung, Bangkok 10240, Thailand.

Equipment Name : Liquid in Glass Thermometer

Manufacturer : AMA

Model : N/A

Serial Number : 2197262

ID. Number : N/A

### Environmental Conditions

Ambient Temperature :  $23\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$

Received Date : 14 Feb 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 15 Feb 2024

Location of Calibration : In-Lab

Recommend Due Date : 15 Feb 2025

Calibration Procedure : SP-CPT-04-08

Date of Issue : 16 Feb 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Surasak Ritthikaew

Approved by :

Calibration Officer



Authorized Signatory



ID LINE: IEC17025



## Calibration Report

Certificate Number : SPR24020220-23

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Super Thermometer with PRT	1575/3850-40-392	58087/100288	PSL-T 0400/66	15 Feb 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



## Result of Calibration

Certificate No. : SPR24020220-23

Page : 3 of 3

Range : -5 to 110 °C

Resolution : 0.5 °C

Unit : °C

Setting Value	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
25.0	25.008	25.0	-0.008	0.29
30.0	30.008	30.0	-0.008	0.29
35.0	35.009	35.0	-0.009	0.29
40.0	40.008	40.0	-0.008	0.29
45.0	45.010	45.0	-0.010	0.29
50.0	50.011	50.0	-0.011	0.29

### Note :

The result of calibration was found accurate as show on date and place of calibration only.

This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -







ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24020220-21

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan  
Sung, Bangkok 10240, Thailand.

Equipment Name : Liquid in Glass Thermometer

Manufacturer : AMA

Model : N/A

Serial Number : 2197263

ID. Number : N/A

### Environmental Conditions

Ambient Temperature :  $23\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$

Received Date : 14 Feb 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 15 Feb 2024

Location of Calibration : In-Lab

Recommend Due Date : 15 Feb 2025

Calibration Procedure : SP-CPT-04-08

Date of Issue : 16 Feb 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.


The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Surasak Ritthikaew

Approved by :

Calibration Officer

Authorized Signatory



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24020220-21

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Super Thermometer with PRT	1575/3850-40-392	58087/100288	PSL-T 0400/66	15 Feb 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



ID LINE : IEC17025



## Result of Calibration

Certificate No. : SPR24020220-21

Page : 3 of 3

Range : -5 to 110 °C

Resolution : 0.5 °C

Unit : °C

Setting Value	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
25.0	25.005	25.0	-0.005	0.29
30.0	30.004	30.0	-0.004	0.29
35.0	35.006	35.0	-0.006	0.29
40.0	40.006	40.0	-0.006	0.29
45.0	45.007	45.0	-0.007	0.29
50.0	50.009	50.0	-0.009	0.29

### Note :


The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -





ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR24020220-22

Page : 1 of 3

Customer : Thai Environmental Technic Limited.

1/6 Soi Ramkhamhaeng 145, Khwaeng Saphan Sung, Khet Saphan  
Sung, Bangkok 10240, Thailand.

Equipment Name : Liquid in Glass Thermometer

Manufacturer : AMA

Model : N/A

Serial Number : 2197264

ID. Number : N/A

### Environmental Conditions

Ambient Temperature :  $23\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$

Received Date : 14 Feb 2024

Relative Humidity :  $50\% \pm 15\%$

Calibration Date : 15 Feb 2024

Location of Calibration : In-Lab

Recommend Due Date : 15 Feb 2025

Calibration Procedure : SP-CPT-04-08

Date of Issue : 16 Feb 2024

### Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Surasak Ritthikaew

Approved by :

Calibration Officer

Authorized Signatory



ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR24020220-22

Page : 2 of 3


### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Super Thermometer with PRT	1575/3850-40-392	58087/100288	PSL-T 0400/66	15 Feb 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :

TISTR - Thailand Institute of Scientific and Technological Research



## Result of Calibration

Certificate No. : SPR24020220-22

Page : 3 of 3

Range :        -5        to        110        °C

Resolution : 0.5 °C

Unit : °C

Setting Value	Standard Reading	UUC Reading	Error	Uncertainty ( ± )
25.0	25.007	25.0	-0.007	0.29
30.0	30.008	30.0	-0.008	0.29
35.0	35.007	35.0	-0.007	0.29
40.0	40.008	40.0	-0.008	0.29
45.0	45.009	45.0	-0.009	0.29
50.0	50.012	50.0	-0.012	0.29

Note :

The result of calibration was found accurate as show on date and place of calibration only.  
This Certificate is not certified for any commercial transaction.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2.00$ , providing a level of confidence approximately 95%.

- End of Certificate -







THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0632

MTC No. EEL. BP. 28/0866

## CALIBRATION CERTIFICATE

Submitted by : THAI ENVIRONMENTAL TECHNIC LIMITED.

Address : 1/6 Soi Ramkhamhaeng 145, Khwaeng/Khet Saphansung, Bangkok, 10240, Thailand.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : Digicon

Model : Tenmars

Serial No. : 180501628

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Panasonic VP-7722A S/N 041477D122.

7. Condenser Microphone B&K 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 10 Aug. 2023

Date of Calibration : 16 Aug. 2023

1 / 3

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0632

MTC No. EEL. BP. 28/0866

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu\text{Pa}$  at 1000 Hz

Acoustic Output in dB re 20 $\mu\text{Pa}$ , Corrected to Reference Conditions : 101.325 kPa, 23.0 $^\circ\text{C}$  and 50 %RH

### 1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	94.45	0.45	$\pm 0.10$	$\pm 0.75 \text{ dB}$

### 2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	991.4	-8.6	$\pm 1.5$	$\pm 1.0\%$

### 3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1.40	$\pm 0.50$	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Date of Calibration : 16 Aug. 2023

2 / 3

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0632

MTC No. EEL. BP. 28/0866

Nominal Output of Unit Under Test = 114 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0 °C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	114.28	0.28	$\pm 0.10$	$\pm 0.75$ dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	986.9	-13.1	$\pm 1.5$	$\pm 2.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	3.14	$\pm 0.70$	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

.....  
(Mr. Weerachai Deechaiyae)

Approved by :

.....  
(Mr. Prawate Klutaypa)  
Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 16 Aug. 2023

Date of Issue : 21 Aug. 2023

Ref : 2011266081003103001

End of Certificate

3 / 3

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpal@tistr.or.th Website: www.tistr.or.th

Office/Laboratory  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



## Sound Level Meter Calibration Report

Equipment Type	: Sound Level Meter	Calibration Date	: 1-Mar-2024
Calibrator	: TENMARS Sound Calibrator TM-100	Barometric pressure (mmHg)	: 759.0 mmHg
Standard	: IEC 60942	Temperature (23±3)°C	: 25.00 °C
Accuracy	: 94.0 ±0.3 dB and 114.0±0.5 dB	Relative Humidity(50±15 %)	: 50.0 % RH
Frequency	: at 1,000 Hz ±1%	Dued Date of Calibrate	: 31-Mar-2024
Calibrator Serial NO.	: 180501628		

Item	Instrument Calibrated			Reference Acoustic dB	Before Adjust				After Adjust ± dB	Deviation ± dB	Result Calibrate
	Brand	Model	Serial NO.		ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	เฉลี่ย			
61	ACO	6226	160205	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
62	ACO	6226	160211	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	113.9	113.9	113.9	113.9			
63	ACO	6226	160212	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	113.9	113.9	113.9	113.9			
64	ACO	6226	160213	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.1	114.1	114.1	114.1			
66	ACO	6226	160215	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
67	ACO	6226	160216	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	113.9	113.9	113.9	113.9			
68	ACO	6236	222036	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.2	114.2	114.2	114.2			
69	ACO	6236	222037	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
70	ACO	6236	222038	94.0	94.0	94.0	94.0	94.0	94.0	0.0	PASS
				114.0	114.0	114.0	114.0	114.0			

Calibration By :

Approve by :







Thai Environmental Technic Limited  
บริษัท เทคนิกล้างแวล้อมไทย จำกัด

## Sound Level Meter Calibration Report

Equipment Type	: Sound Level Meter	Calibration Date	: 1-Apr-2024
Calibrator	: TENMARS Sound Calibrator TM-100	Barometric pressure (mmHg)	: 759.0 mmHg
Standard	: IEC 60942	Temperature (23±3)°C	: 25.00 °C
Accuracy	: 94.0 ±0.3 dB and 114.0±0.5 dB	Relative Humidity(50±15 %)	: 50.0 % RH
Frequency	: at 1,000 Hz ±1%	Dued Date of Calibrate	: 30-Apr-2024
Calibrator Serial NO.	: 180501628		

Item	Instrument Calibrated			Reference Acoustic dB	Before Adjust				After Adjust ± dB	Deviation ± dB	Result Calibrate
	Brand	Model	Serial NO.		ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	เฉลี่ย			
46	ACO	6236	112029	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	113.9	113.9	113.9	113.9			
48	ACO	6236	152074	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.2	114.2	114.2	114.2			
49	ACO	6236	152075	94.0	93.8	93.8	93.8	93.8	94.0	0.2	PASS
				114.0	113.8	113.8	113.8	113.8			
50	ACO	6236	152076	94.0	94.0	94.0	94.0	94.0	94.0	0.0	PASS
				114.0	114.0	114.0	114.0	114.0			
51	ACO	6236	152077	94.0	94.0	94.0	94.0	94.0	94.0	0.0	PASS
				114.0	114.0	114.0	114.0	114.0			
52	ACO	6226	150142	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
53	ACO	6226	160095	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
54	ACO	6226	160096	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	113.9	113.9	113.9	113.9			
55	ACO	6226	160097	94.0	93.8	93.8	93.8	93.8	94.0	0.2	PASS
				114.0	113.7	113.7	113.7	113.7			
56	ACO	6226	160098	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			

Calibration By : 

Approve by : 



Thai Environmental Technic Limited  
บริษัท เทคโนโลยีสิ่งแวดล้อมไทย จำกัด

## Sound Level Meter Calibration Report

Equipment Type : Sound Level Meter  
Calibrator : TENMARS Sound Calibrator TM-100  
Standard : IEC 60942  
Accuracy :  $94.0 \pm 0.3$  dB and  $114.0 \pm 0.5$  dB  
Frequency : at 1,000 Hz  $\pm 1\%$   
Calibrator Serial NO. : 180501628

Calibration Date : 1-Apr-2024  
Barometric pressure (mmHg) : 759.0 mmHg  
Temperature ( $23 \pm 3$ )°C : 25.00 °C  
Relative Humidity ( $50 \pm 15$  %) : 50.0 % RH  
Dued Date of Calibrate : 30-Apr-2024

Item	Instrument Calibrated			Reference Acoustic dB	Before Adjust				After Adjust ± dB	Deviation ± dB	Result Calibrate
	Brand	Model	Serial NO.		ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	เฉลี่ย			
21	ACO	6226	070049	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.2	114.2	114.2	114.2			
23	RION	NL-21	00487676	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	113.9	113.9	113.9	113.9			
25	ACO	6226	100098	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.1	114.1	114.1	114.1			
26	ACO	6226	100099	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
28	ACO	6226	100101	94.0	93.8	93.8	93.8	93.8	94.0	0.2	PASS
				114.0	113.8	113.8	113.8	113.8			
29	ACO	6226	100102	94.0	93.9	93.9	93.9	93.9	94.0	0.1	PASS
				114.0	113.9	113.9	113.9	113.9			
30	ACO	6226	100106	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.0	114.0	114.0	114.0			
31	ACO	6226	110098	94.0	94.2	94.2	94.2	94.2	94.0	0.2	PASS
				114.0	114.2	114.2	114.2	114.2			
32	ACO	6226	110105	94.0	93.8	93.8	93.8	93.8	94.0	0.2	PASS
				114.0	113.8	113.8	113.8	113.8			
34	ACO	6226	110099	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			

Calibration By : .....

Approve by : .....




Thai Environmental Technic Limited  
บริษัท เทคนิคสิ่งแวดล้อมไทย จำกัด


## Sound Level Meter Calibration Report

Equipment Type : Sound Level Meter  
Calibrator : TENMARS Sound Calibrator TM-100  
Standard : IEC 60942  
Accuracy : 94.0 ±0.3 dB and 114.0±0.5 dB  
Frequency : at 1,000 Hz ±1%  
Calibrator Serial NO. : 180501628

Calibration Date : 1-Apr-2024  
Barometric pressure (mmHg) : 759.0 mmHg  
Temperature (23±3)°C : 25.00 °C  
Relative Humidity(50±15 %) : 50.0 % RH  
Dued Date of Calibrate : 30-Apr-2024

Item	Instrument Calibrated			Reference Acoustic dB	Before Adjust				After Adjust ± dB	Deviation ± dB	Result Calibrate
	Brand	Model	Serial NO.		ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	เฉลี่ย			
68	ACO	6236	222036	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
69	ACO	6236	222037	94.0	94.0	94.0	94.0	94.0	94.0	0.0	PASS
				114.0	114.0	114.0	114.0	114.0			
70	ACO	6236	222038	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
71	ACO	6236	222039	94.0	94.1	94.1	94.1	94.1	94.0	0.1	PASS
				114.0	114.1	114.1	114.1	114.1			
72	ACO	6236	222040	94.0	94.0	94.0	94.0	94.0	94.0	0.0	PASS
				114.0	114.0	114.0	114.0	114.0			
74	ACO	6236	222245	94.0	94.0	94.0	94.0	94.0	94.0	0.0	PASS
				114.0	114.0	114.0	114.0	114.0			

Calibration By : 

Approve by : 







TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CHO641

Page.: 1 of 2

## Certificate of Calibration

**Equipment :** pH Meter  
**Manufacturer :** Horiba  
**Model :** F-71G  
**Serial No. :** V3B1F8H3  
**ID No. :** Ins-LAB-025  
**Condition As-Received:** Used Item  
**Received Date :** 31 October 2023  
**Calibration Date :** 31 October 2023  
**Reference :** 2310-0843OC-1  
**Submitted by :** Thai Environmental Technic Limited  
1/6 Soi Ramkhamhaeng 145,  
Khwaeng/Khet Saphan Sung,  
Bangkok 10240  
**Calibration Place :** Laboratory (Thai Environment Technic Limited)  
**Ambient Temperature :** (25.8 - 24.6) °C  
**Relative Humidity :** (69.3 - 65.6) %  
**Calibration Procedure :** In - house method :  
- CP-OCH2 by direct measurement with standard  
voltage calibrator and direct measurement  
with certified reference material (CRM)

**Calibrated by :** Khit Ruttanaprapachai

**Approved by :**

- (✓) Saithip Meangmai  
( ) Warakom Lernagtrakul  
( ) Ponpan Paipim

**Issue Date :** 10 November 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0060437



Cert. No.: 23CHO641

Page.: 2 of 2

**Condition of this calibration result**

## 1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	43160066	130RC092	23E1284	10 Apr 2024
2) Digital Thermometer	-	130RC018	23T1595	13 Sep 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	931958	01 Oct 2025
pH 6.865	CPA chem	788996	01 Jan 2024
pH 9.181	CPA chem	931960	01 Oct 2024

## 3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results****Function : mV Measurement****Performing standard curve by Fluke at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( $\pm$ mV)	Coverage factor $k$
	pH	mV	mV	pH		
pH Meter S/N.: V3B1F8H3	4.000	177.48	177.5	4.000	0.058	2.00
	6.860	8.28	8.3	6.860	0.058	2.00
	7.000	0.00	0.0	7.000	0.058	2.00
	9.180	-128.97	-128.9	9.180	0.058	2.00
	10.000	-177.48	-177.4	10.000	0.058	2.00

**Function : pH Measurement****Performing three buffers standard curve by using buffer nominal pH (4,7,9)**

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 9X2E0223	4.008	4.031	160.0	0.0052	2.00
	6.865	6.870	-7.4	0.0087	2.00
	9.181	9.186	-142.0	0.014	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

a 1188742



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert.No.: 24MM272

Page.: 1 of 3

**Equipment :** Electronic Balance

**Manufacturer :** Mettler Toledo

**Model :** AB204

**Serial No. :** 1116392227

**ID No. :** Ins-LAB-033

**Submitted by :** Thai Environmental Technic Limited  
1/6 Soi Ramkhamhaeng 145,  
Khwaeng/Khet Saphan Sung,  
Bangkok 10240

**Location :** Balance Room

**Received order :** 09 April 2024  
**Calibration Date :** 10 April 2024  
**Ambient Temperature :** 15 °C to 40 °C  
**Relative Humidity :** 30 % to 90 %

**Calibrated by :** Khit Ruttanaprapachai

**Approved by :**

( ) Ponpan Paipim  
( ) Suwit Imjai  
(✓) Kunchit Promprat

A

**Issue Date :**

12 April 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



**Equipment :** Electronic Balance  
**Condition As-Received :** Used Item  
**Reference :** 2404-0113OC-14

**Cert.No.:** 24MM272  
**Page:** 2 of 3

**Procedure used :-**

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14 according to direct measurement method against standard weight.

**Condition of this result of calibration**

1. Reference standard instruments:-

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Test report No.</u>	<u>Due date</u>
1) Standard Weight Set (E2)	15884	-	70RC138	MM-0020-23	30 Jan 2025

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

**Result of calibration** ( ) Without Adjustment ( \* ) After Adjustment by External Calibration

**Range capacity :** 0 g to 210 g **Resolution** 0.0001 g

**Before Adjustment :**

<u>Applied Weight</u> ( g )	<u>Balance Reading</u> ( g )	<u>Correction</u> ( g )	<u>Measurement Uncertainty</u> ( ± mg )	<u>Coverage Factor</u> ( k )
100	100.0000	0.0000	0.19	2
200	200.0001	-0.0001	0.30	2

**After Adjustment :**

1. **Determination of the standard deviation of weighing machine** ( n = 10 )

<u>Applied Weight</u> ( g )	<u>Standard Deviation of Reading ( g )</u>
100	0.00007
200	0.00008



**Equipment :** Electronic Balance  
**Condition As-Received :** Used Item  
**Reference :** 2404-0113OC-14


**Cert.No.:** 24MM272

**Page:** 3 of 3

## Result of calibration

### 2. Effect of off center loading

A mass of 100 g was placed at various positions on the pan. The weighing machine reading error obtained is given in the table

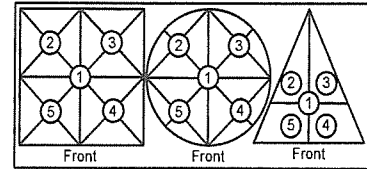

**Maximum difference between  
off-center and central loading**  
 ( g )  
 0.0003

Position 1	Position 2	Position 3	Position 4	Position 5
( g )	( g )	( g )	( g )	( g )
0.0000	+0.0001	0.0000	+0.0001	+0.0003

### 3. Departure from nominal value

<u>Applied Weight</u>	<u>Balance Reading</u>	<u>Correction</u>	<u>Measurement Uncertainty</u>	<u>Coverage Factor</u>
( g )	( g )	( g )	( $\pm$ mg )	( $k$ )
Unload	0.0000	0.0000	0.14	2.11
0.01	0.0101	-0.0001	0.14	2.11
0.1	0.1001	-0.0001	0.14	2.11
0.5	0.5002	-0.0002	0.14	2.11
1	1.0002	-0.0002	0.14	2.11
5	5.0000	0.0000	0.14	2.11
10	10.0001	-0.0001	0.14	2.11
25	25.0000	0.0000	0.15	2.07
50	49.9999	+0.0001	0.15	2.06
100	100.0002	-0.0002	0.19	2
200	200.0002	-0.0002	0.30	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CHO493

Page.: 1 of 3

## Certificate of Calibration

Equipment : Spectrophotometer  
Manufacturer : Perkin Elmer  
Model : Lambda 365  
Serial No. : 365K9042909  
ID No. : -  
Condition As-Received: Used Item  
Received Date : 18 August 2023  
Calibration Date : 18 August 2023  
Reference : 2308-0469OC-1  
Submitted by : Thai Environmental Technic Limited  
1/6 Soi Ramkhamhaeng 145,  
Khwaeng/Khet Saphan Sung,  
Bangkok 10240  
Calibration Place : Laboratory (Thai Environment Technic Limited)  
Ambient Temperature : ( 25.5 - 25.3 ) °C (On-Site)  
Relative Humidity : ( 57.8 - 60.6 ) % (On-Site)  
Calibration Procedure : In - house method :  
CP-OCH4 based on ASTM E 275-01

Calibrated by : Kunchit Promprat

Approved by :

(✓) Saithip Meangmai  
( ) Warakorn Lerngagtrakul  
( ) Ponpan Paipim

Issue Date : 22 August 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0057186



Cert. No. : 23CHO493

Page : 2 of 3

**Condition of calibration result**

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	8331	105939	28 Sep 2024
2. Wavelength Standard set	8417	100498	25 Mar 2024
3. Wavelength Standard set	8418	100499	25 Mar 2024
4. Stray Light Standard set	8419	108963	01 Feb 2025


2. This certificate is valid only to the item calibrated on date and place of calibration.  
3. This certificate is traceable to the International System of Unit maintained through :  
- Sarna Scientific Ltd.

4. Spectral BandWidth : 1 nm  
Scan Speed : 30 nm/min

**Calibration Results : without adjustment**

**Wavelength Accuracy**

<b>Certified Values of Reference Material ( nm )</b>	<b>UUC Reading ( nm )</b>	<b>Uncertainty of Measurement ( <math>\pm</math> nm )</b>	<b>Coverage Factor <i>k</i></b>
418.53	418.54	0.12	2.00
536.52	536.13	0.12	2.00
638.00	637.64	0.14	2.05
684.50	684.49	0.13	2.00
879.41	879.42	0.12	2.00



a 1176586





Cert. No. : 23CHO493

Page : 3 of 3

**Calibration Results : without adjustment**

**Photometric Accuracy**

Wavelength (nm)	Certified Values of Reference Material ( Abs )	UUC Reading ( Abs )	Uncertainty of Measurement ( $\pm$ Abs )	Coverage Factor <i>k</i>
420.0	Zero	0.0000	0.0028	2.00
	0.5712	0.5699	0.0031	2.00
	0.7510	0.7494	0.0031	2.00
	1.0893	1.0877	0.0033	2.00
546.1	Zero	-0.0001	0.0028	2.00
	0.5224	0.5209	0.0028	2.00
	0.6856	0.6839	0.0028	2.00
	0.9937	0.9921	0.0028	2.00
635.0	Zero	-0.0001	0.0028	2.00
	0.5397	0.5375	0.0028	2.00
	0.6832	0.6810	0.0028	2.00
	0.9886	0.9861	0.0028	2.00

**Stray Light**

* Straylight at 260.74 nm $\pm$ 0.11 nm	Reading at 260.74 nm $\pm$ 0.11 nm
Abs	2.0488
%T	0.8951

**Remark**

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- The Potassium Dichromate filled cells are measured against a Perchloric acid blank.
- Cut-off wavelength of stray light reference material (Potassium Iodide) at wavelength 260.74 nm  $\pm$  0.11 nm
- Result = Pass, If Absorbance > 2.00 Abs and Transmission < 1.0 %T at Wavelength 260.74 nm  $\pm$  0.11 nm
- \* : Not NSC-ONSC Accredited

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.


-o0o-

a 1176585





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM704

Page: 1 of 3

## Certificate of Calibration

Equipment : BOD Incubator  
Manufacturer : Accuplus  
Model : i250-DS  
Serial No. : 2059-1017-0029  
ID No. : LAB BOD 06  
Submitted by : Thai Environmental Technic Limited  
1/6 Soi Ramkhamhaeng 145,  
Khwaeng/Khet Saphan Sung,  
Bangkok 10240  
Location : Laboratory (Thai Environmental Technic Limited)  
Received Order : 29 June 2023  
Calibration Date : 29 June 2023  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
Calibrated by : Suwit Imjai

Approved by :

( ) Pornthippa Tameyakul  
(✓) Malee Butkruea

[Redacted Signature]

Issue Date :

5 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0053593



Equipment : BOD Incubator  
 Condition As-Received : Used Item  
 Reference : 2306-07120C-8  
 Procedure Used :-

Cert. No.: 23TM704  
 Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1 ) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Fresh air setting : Not Available

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	24	24
REL.Humid. ( % )	67	64
AC Supply ( Volt )	229	227

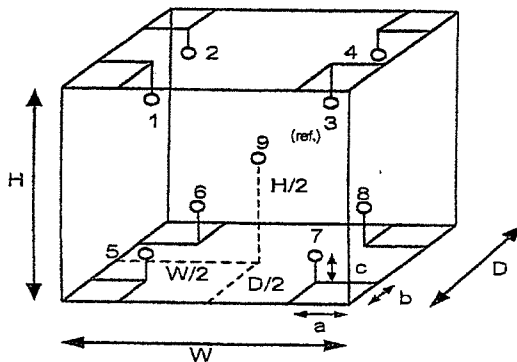

Position :	Ref. Std. ID No.:
1	21-17RTD-01
2	21-17RTD-02
3	17RTD-03
4	17RTD-04
5	17RTD-05
6	17RTD-06
7	17RTD-07
8	23-17RTD-08
9 (ref.)	23-17RTD-09

**Probe Installation Details :**

a = 10 cm  
 b = 10 cm  
 c = 10 cm

**Dimension of Chamber :**

D = 0.48 m  
 W = 0.50 m  
 H = 1.1 m  
 Capacity = 0.26 m<sup>3</sup>



**Equipment :** BOD Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2306-0712OC-8  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Not Available

**Cert. No.:** 23TM704  
**Page :** 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
20.0	20.0	19.7	0.38	0.38	1.1	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	20.244	20.180	20.158	20.066	20.002	19.974	19.712	19.822	19.965	0.58

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-oOo-



a 1168974





## MAINTENANCE REPORT

## OPTIMA 8000

Customer :	บริษัท เทคนิกสิ่งแวดล้อมไทย	Date Tested:	March 28, 2024
	จำกัด	Recommendation Recertification	
Address :	1/6 ซอยรามคำแหง 145,	Period	6 Months
	แขวงสะพานสูง, เขตสะพานสูง,	Recertification Due:	September 27, 2567
	กรุงเทพฯ 10240 TH	Date Last Certified:	September 29, 2023
User Name:	คุณ ญัฐพงศ์	Visit Number:	1 OF 2
Phone:	02-3737799, 081-1303495	TH ONE SOURCE Phone:	081-7316733, 081-1086572
E-mail:	Ketsarin.Chuayphan@eurofinsasia.co	E-mail :	thonesource@gmail.com

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
OPTIMA 8000	078S1310024C	WinLab32 Version 5.5.0
N0772045	1F1380368	PN:6150T21E4Q1E
TESTED EQUIPMENT		
IPV Methods		
TEST STANDARD USED	PE NUMBER	
Mixed standard 1/10	N0691579	
Mixed standard 1/100	N9300221	
CUSTOMER SUPPLIED	COMMENTS	
2 % HNO3		
10 % HNO3		



## MAINTENANCE REPORT

### OPTIMA 8000

**SERIAL NUMBER**    078S1310024C
**DATE TESTED**
March 28, 2024
**1. MECHANICAL CHECKS**

- A. Inspect and clean all fans and filters.
- B. Inspect and replace as necessary, all torch components including the RF Flat coil
- C. Inspect all tubing for sign of clacking or leaking.
- D. Adjust water and gas pressure regulator settings.
- E. Inspect and leak check pneumatics drawers.
- F. Clean the exterior of the instrument.

OK

OK

OK

OK

OK

OK

**2. OPTICAL CHECKS**

- A. Inspect and clean all optical components.
- B. As required, check and replace all purge filters.
- C. Recheck optical alignment.

OK

OK

OK

**3. COOLING SYSTEM CHECKS**

- A. Perform preventive maintenance on chiller.
- B. Flush out water the chiller and replace with coolant mix30plus every twelve months

OK

OK

**4. PERFORMANCE CHECKS**

- A. Torch View Alignment.
- B. Wavelength Calibration.

OK

OK





## MAINTENANCE REPORT

### OPTIMA 8000

<b>SERIAL NUMBER</b>	<b>078S1310024C</b>	<b>DATE TESTED</b>	<b>March 28, 2024</b>
<b>PARAMETER</b>	<b>SPECIFICATION</b>	<b>FINAL VAULE</b>	
<b>Precision</b>			
Zn 213.856	% RSD $\leq 1.0$	0.33	
Mg 280.260	% RSD $\leq 1.0$	0.63	
Mg 285.207	% RSD $\leq 1.0$	0.59	
Ba 455.403	% RSD $\leq 1.0$	0.28	
<b>Detection Limits: Axial</b>			
	As 193 nm, 3(sd) $\leq 10.0$ ppb	1.39	
	Se 196 nm, 3(sd) $\leq 5.0$ ppb	5	
	Tl 190 nm, 3(sd) $\leq 10.0$ ppb	1.08	
	Pb 220 nm, 3(sd) $\leq 3.0$ ppb	0.28	
<b>BEC: Axial</b>	Mn 257 nm, $\leq 30$ ppb	3.80	
<b>Detection Limits: Radial</b>			
	As 193 nm, 3(sd) $\leq 60.0$ ppb	2.53	
	Zn 213 nm, 3(sd) $\leq 2.0$ ppb	0.22	
	Mn 257 nm, 3(sd) $\leq 1.0$ ppb	0.05	
	La 379 nm, 3(sd) $\leq 3.0$ ppb	0.07	
	Ba 455 nm, 3(sd) $\leq 0.3$ ppb	0.04	
	Ba 493 nm, 3(sd) $\leq 0.6$ ppb	0.02	
<b>BEC: Radial</b>	Mn 257 nm, $\leq 30$ ppb	10.83	
<b>Spectral Resolution: UV</b>			
	As 193 nm, $\leq 0.009$	0.00687	
	Ni 231 nm, $\leq 0.011$	0.00792	
	Ni 341 nm, $\leq 0.015$	0.01195	
<b>Spectral Resolution: VIS</b>			
	Ba 455 nm, $\leq 0.020$	0.01482	



## MAINTENANCE REPORT

### OPTIMA 8000

**SERIAL NUMBER** 078S1310024C
**DATE TESTED**
March 28, 2024
**Remarks :**

Commissioning follow as commissioning performance sheets.

Calculate MnBEC =  $IB * STD \text{ Conc} / IS - IB$  , where standard conc = 1000 ug/L

IB = Intensity of blank

IS = Intensity of Standard

**Used Mira Mist Nebulizer**

ตรวจพบว่าLED(green)ในPlasma Control ติดเป็นบางครั้ง แสดงว่าวงจรควบคุมในส่วนของ Neb Flow

บน Pneumatics Controller Board เริ่มมีปัญหา.

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

**Service Department TH One Source Co., Ltd.**

(  )  
Customer Support Engineer

=====  
Method Loaded  
Method Name: Precision  
IEC File:  
Method Description: N=10- 1.0% RSD  
Method Last Saved: 22/4/2554 10:20:08  
MSF File: .

=====  
Sequence No.: 3  
Sample ID: Precision  
Analyst:  
Initial Sample Wt:  
Dilution:  
Wash Time:  
Autosampler Location:  
Date Collected: 28/3/2567 13:45:32  
Data Type: Original  
Initial Sample Vol:  
Sample Prep Vol:

-----  
Nebulizer Parameters: Precision  
Analyte Back Pressure Flow  
All 222.0 kPa 0.55 L/min

-----  
Mean Data: Precision  

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Zn 206.200	146145.0				482.54	0.33%
Mg 280.271	1334588.3				8458.45	0.63%
Mg 285.213	74404.6				440.15	0.59%
Ba 455.403	3373485.1				9503.39	0.28%

=====

=====

Analysis Begun

Start Time: 28/3/2567 13:57:16  
 Logged In Analyst: TET  
 Spectrometer: Optima 8000

Plasma On Time: 28/3/2567 13:19:06  
 Technique: ICP Continuous  
 Autosampler: S10

Sample Information File: C:\Users\Public\PerkinElmer\ICP\Data\Sample Information\24-03-28.sif  
 Batch ID:  
 Results Data Set: DLRL\_280324  
 Results Library: C:\Users\Public\PerkinElmer\ICP\Data\Results\Results.mdb

=====

Method Loaded

Method Name: DLRL-Cal

Method Last Saved: 5/10/2552 13:52:49

IEC File:

MSF File:

Method Description: Calibration for later test

=====

Sequence No.: 1

Autosampler Location:

Sample ID: Calib Blank 1

Date Collected: 28/3/2567 13:57:20

Analyst:

Data Type: Original

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Wash Time:

-----

Nebulizer Parameters: Calib Blank 1

Analyte	Back Pressure	Flow
All	222.0 kPa	0.55 L/min

-----

Mean Data: Calib Blank 1

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc. Units
As 193.696	20.4	0.64	3.16%	[0.00] mg/L
Zn 213.857	389.8	2.50	0.64%	[0.00] mg/L
Mn 257.610	373.7	31.47	8.42%	[0.00] mg/L
La 379.478	-39.2	19.10	48.73%	[0.00] mg/L
Ba 455.403	565.0	298.22	52.78%	[0.00] mg/L
Ba 493.408	595.9	5.51	0.92%	[0.00] mg/L

=====

Sequence No.: 2

Autosampler Location:

Sample ID: Calib Std 1

Date Collected: 28/3/2567 14:00:31

Analyst:

Data Type: Original

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Wash Time:

-----

Nebulizer Parameters: Calib Std 1

Analyte	Back Pressure	Flow
All	222.0 kPa	0.55 L/min

-----

Mean Data: Calib Std 1

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc. Units
As 193.696	5829.0	7.43	0.13%	[5.0] mg/L
Zn 213.857	68281.4	370.49	0.54%	[1.0] mg/L
Mn 257.610	682084.8	550.96	0.08%	[1.0] mg/L
La 379.478	151940.7	798.65	0.53%	[1.0] mg/L
Ba 455.403	389420.9	422.28	0.11%	[0.1] mg/L
Ba 493.408	293177.5	436.31	0.15%	[0.1] mg/L

-----

Calibration Summary

Analyte	1	Lin, Calc Int	0.0	1166	0.00000	1.000000
Zn 213.857	1	Lin, Calc Int	0.0	68280	0.00000	1.000000

Mn 257.610	1	Lin, Calc Int	0.0	682100	0.00000	1.000000
La 379.478	1	Lin, Calc Int	0.0	151900	0.00000	1.000000
Ba 455.403	1	Lin, Calc Int	0.0	3894000	0.00000	1.000000
Ba 493.408	1	Lin, Calc Int	0.0	2932000	0.00000	1.000000

```

=====
Sequence No.: 3                      Autosampler Location:
Sample ID: 2%                      Date Collected: 28/3/2567 14:03:02
Analyst:                          Data Type: Original
Initial Sample Wt:                 Initial Sample Vol:
Dilution:                         Sample Prep Vol:
Wash Time:
=====

```

```

-----
Nebulizer Parameters: 2%
Analyte      Back Pressure  Flow
All          222.0 kPa      0.55 L/min
-----

```

```

-----
Mean Data: 2%

```

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
As 193.696	43.7	0.0 mg/L	0.01	37.5 g/L	9.68	25.84%
Zn 213.857	-20.4	-0.0 mg/L	0.00	-0.3 g/L	0.41	136.74%
Mn 257.610	394.8	0.0 mg/L	0.00	0.6 g/L	0.10	16.69%
La 379.478	67.0	0.0 mg/L	0.00	0.4 g/L	0.24	55.45%
Ba 455.403	-236.1	-0.0 mg/L	0.00	-0.1 g/L	0.00	4.98%
Ba 493.408	-38.6	-0.0 mg/L	0.00	-0.0 g/L	0.02	177.50%

```

=====
Method Loaded
Method Name: DLRL-Check             Method Last Saved: 25/2/2543 11:12:48
IEC File:                          MSF File:
Method Description: As-60,Zn-2, Mn1.0,La-3,Ba455-0.3,Ba493-0.6
=====

```

```

=====
Sequence No.: 4                      Autosampler Location:
Sample ID: 2 % HNO3                 Date Collected: 28/3/2567 14:06:15
Analyst:                          Data Type: Original
Initial Sample Wt:                 Initial Sample Vol:
Dilution:                         Sample Prep Vol:
Wash Time:
=====

```

```

-----
Nebulizer Parameters: 2 % HNO3
Analyte      Back Pressure  Flow
All          222.0 kPa      0.55 L/min
-----

```

```

-----
Mean Data: 2 % HNO3

```

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
As 193.696	-7.1	-0.0 mg/L	0.01	-6.1 g/L	6.36	104.68%
Zn 213.857	192.0	0.0 mg/L	0.00	2.8 g/L	0.14	4.99%
Mn 257.610	91.2	0.0 mg/L	0.00	0.1 g/L	0.02	15.88%
La 379.478	223.8	0.0 mg/L	0.00	1.5 g/L	0.31	21.20%
Ba 455.403	-86.9	-0.0 mg/L	0.00	-0.0 g/L	0.03	139.07%
Ba 493.408	-179.8	-0.0 mg/L	0.00	-0.1 g/L	0.05	86.77%

```

=====

```

=====

Analysis Begun

Start Time: 28/3/2567 14:15:49  
 Logged In Analyst: TET  
 Spectrometer: Optima 8000

Plasma On Time: 28/3/2567 13:19:06  
 Technique: ICP Continuous  
 Autosampler: S10

Sample Information File: C:\Users\Public\PerkinElmer\ICP\Data\Sample Information\24-03-28.sif  
 Batch ID:  
 Results Data Set: DLXL\_280324  
 Results Library: C:\Users\Public\PerkinElmer\ICP\Data\Results\Results.mdb

=====

Method Loaded

Method Name: DLXL-Cal

Method Last Saved: 5/10/2552 13:39:33

IEC File:

MSF File:

Method Description: Calibration for later test

=====

Sequence No.: 1

Autosampler Location:

Sample ID: Calib Blank 1

Date Collected: 28/3/2567 14:15:53

Analyst:

Data Type: Original

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Wash Time:

-----

Nebulizer Parameters: Calib Blank 1

Analyte	Back Pressure	Flow
All	223.0 kPa	0.55 L/min

-----

Mean Data: Calib Blank 1

Analyte	Mean Corrected		Std.Dev.	RSD	Calib	
	Intensity				Conc.	Units
As 193.696	32.0		8.30	25.92%	[0.00]	g/L
Se 196.026	26.5		5.11	19.26%	[0.00]	g/L
Tl 190.801	-38.3		10.38	27.07%	[0.00]	g/L
Pb 220.353	353.9		3.91	1.11%	[0.00]	g/L

=====

Sequence No.: 2

Autosampler Location:

Sample ID: DL-Standard

Date Collected: 28/3/2567 14:18:16

Analyst:

Data Type: Original

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Wash Time:

-----

Nebulizer Parameters: DL-Standard

Analyte	Back Pressure	Flow
All	223.0 kPa	0.55 L/min

-----

Mean Data: DL-Standard

Analyte	Mean Corrected		Std.Dev.	RSD	Calib	
	Intensity				Conc.	Units
As 193.696	5168.6		94.41	1.83%	[1000]	g/L
Se 196.026	237.1		23.20	9.78%	[500]	g/L
Tl 190.801	6707.8		43.25	0.64%	[1000]	g/L
Pb 220.353	13300.0		22.38	0.17%	[500]	g/L

-----

Calibration Summary

Analyte		Lin, Calc Int				
As 193.696	1	Lin, Calc Int	0.0	5.169	0.00000	1.000000
Se 196.026	1	Lin, Calc Int	0.0	0.4743	0.00000	1.000000
Tl 190.801	1	Lin, Calc Int	0.0	6.708	0.00000	1.000000
Pb 220.353	1	Lin, Calc Int	0.0	26.60	0.00000	1.000000

=====

Sequence No.: 3

Autosampler Location:

Sample ID: QC01 MQCS

Date Collected: 28/3/2567 14:21:26

Analyst: Data Type: Original  
Initial Sample Wt: Initial Sample Vol:  
Dilution: Sample Prep Vol:  
Wash Time:

-----  
Nebulizer Parameters: QC01 MQCS

Analyte Back Pressure Flow  
All 222.0 kPa 0.55 L/min

-----  
Mean Data: QC01 MQCS

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
As 193.696	135.4	30 g/L	4.50	30 g/L	4.50	17.16%
Se 196.026	8.8	20 g/L	37.93	20 g/L	37.93	204.11%
Tl 190.801	2.4	0 g/L	0.03	0 g/L	0.03	9.11%
Pb 220.353	60.4	2 g/L	1.14	2 g/L	1.14	50.16%

=====  
Method Loaded

Method Name: DLXL-Check Method Last Saved: 25/2/2543 10:51:16  
IEC File: MSF File:  
Method Description: Sample Std.Dev As/Tl <=10 g/l ,Se<=-5 g/l ,Pb<=3 g/l

=====  
Sequence No.: 4

Sample ID: 2 % HNO3	Autosampler Location:
Analyst:	Date Collected: 28/3/2567 14:24:11
Initial Sample Wt:	Data Type: Original
Dilution:	Initial Sample Vol:
Wash Time:	Sample Prep Vol:

-----  
Nebulizer Parameters: 2 % HNO3

Analyte Back Pressure Flow  
All 222.0 kPa 0.55 L/min

-----  
Mean Data: 2 % HNO3

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
As 193.696	-1.6	-0.3 g/L	1.39	-0.3 g/L	1.39	459.43%
Se 196.026	10.9	20 g/L	11.69	20 g/L	5.00	50.84%
Tl 190.801	1.1	0.2 g/L	1.08	0.2 g/L	1.08	649.16%
Pb 220.353	-21.4	-0.8 g/L	0.28	-0.8 g/L	0.28	34.35%



**Global Service Training Department  
Service Engineer Certification**

---

**Krungchai Treevichien**

---

**This is to certify that the above mentioned  
PerkinElmer representative has trained to  
service the instrument indicated below:**

**ICP-Optima 7X00/8X00 Series**

---

**Instructor:-**

**Geoff Cook**

**Date:-13 FEB 2011 to 24 FEB 2011**

**Certified by :**

**(Manager, Global Training Operations)**