



Certificate No. : 23-148799  
Sample Code : 23-56200-001

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Calibrated by Mr. Somwang Sangdee  
Scientist

Approved by (Mr. Somchai Neampunt)  
Signed for Director

Issue date 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-148799  
Sample Code : 23-56200-001

## REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE  
Manufacturer : METTLER TOLEDO  
Model : XS205DU  
Capacity : Max 81 g / 220 g  
Resolution : 0.01 mg / 0.1 mg  
Serial No. : 1126323724  
ID No. : LABE 05/1

### Result of Calibration

#### 1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	40	80
<input checked="" type="checkbox"/> Adjustment	Standard weight	40.000054	80.000048
	Average reading of indicator	40.000026	80.000037
	Standard deviation	0.000015	0.000016
		0.000008	0.000009
Unit : g	Range : 200	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	100	200
<input checked="" type="checkbox"/> Adjustment	Standard weight	100.000042	200.000041
	Average reading of indicator	100.00003	200.00004
	Standard deviation	0.00005	0.00005
		0.00003	0.00005

Certificate No. : 23-148799  
Sample Code : 23-56200-001

Page 3 of 4

## REPORT OF CALIBRATION

## Result of Calibration

## 2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 80

Range : 200

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	1.00748	0	1.0274
40	0.98753	100	0.9975
80	0.99751	200	0.9975

## 3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.000012	2.05
0.01	0.0100025	0.01000	0.00000	0.000012	2.05
0.1	0.1000019	0.10001	-0.00001	0.000013	2.03
1	1.0000125	1.00001	0.00000	0.000015	2.02
5	5.0000208	5.00004	-0.00002	0.000021	2.00
10	10.000004	10.00008	-0.00008	0.000026	2.00
20	20.000030	20.00011	-0.00008	0.000036	2.00
50	50.000014	50.00014	-0.00013	0.000068	2.00
100	100.000042	100.0001	-0.0001	0.00016	2.00
150	150.000056	150.0001	0.0000	0.00022	2.00
200	200.000041	200.0002	-0.0002	0.00027	2.00

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 23-148799  
Sample Code : 23-56200-001

Page 4 of 4


## REPORT OF CALIBRATION

## Result of Calibration :

## 4. Eccentric or off-centre loading

Deviation of the measurement value through off-center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan	<input type="radio"/> Circle	Test weight : 50 and 100
	<input type="radio"/> Triangular	
	<input checked="" type="radio"/> Rectangular	
Range	80	200
Position	Reading of indicator	Reading of indicator
1	50.00015	100.0001
2	50.00022	100.0001
3	50.00008	100.0001
4	50.00002	100.0000
5	50.00016	100.0002
6	50.00014	100.0001
Maximum difference	0.00013	0.0001

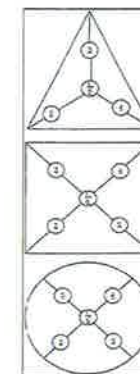

## Condition of Calibration

1. Calibration Method : WI-DL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration tem: Normal

4. This certification is traceable to the International System of Unit maintained at :

Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

## 5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-79	23-105642	10 September 2024

End of Report

6. Ambient conditions	Min	Max
Temperature (°C)	22.8	23.0
Relative Humidity (%Rh)	43.5	51.1
Air pressure (hPa)	1012.5	1014.5



Certificate No. : 23-148800  
Sample Code : 23-56200-002

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-1S

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Calibrated by Mr. Somwang Sangdee  
Scientist

Approved by (Mr. Somchai Neampunt)  
Signed for Director

Issue date : 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-148800  
Sample Code : 23-56200-002

## REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE  
Manufacturer : SARTORIUS  
Model : SECURA224-1S  
Capacity : Max 220 g  
Resolution : 0.0001 g  
Serial No. : 0036707137  
ID No. : LABE 05/2

## Result of Calibration

## 1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	100	200
<input checked="" type="checkbox"/> Adjustment	Standard weight	100.000042	200.000041
	Average reading of indicator	99.9998	199.9998
	Standard deviation	0.00006	0.00007

Unit :	Range :	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value		
<input type="checkbox"/> Adjustment	Standard weight		
	Average reading of indicator		
	Standard deviation		

COPY

Certificate No. : 23-148800  
Sample Code : 23-56200-002

## REPORT OF CALIBRATION

## Result of Calibration

## 2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 220

Range : -

Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.7980	-	-
100	0.8978	-	-
200	0.8978	-	-

## 3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.000086	2.00
0.01	0.0100025	0.0100	0.0000	0.000086	2.00
0.1	0.1000019	0.1000	0.0000	0.000087	2.00
1	1.0000125	1.0000	0.0000	0.000087	2.00
2	2.0000089	2.0000	0.0000	0.000087	2.00
5	5.0000208	5.0001	-0.0001	0.000088	2.00
10	10.000004	10.0000	0.0000	0.000090	2.00
20	20.000030	20.0000	0.0000	0.000093	2.00
50	50.000014	50.0000	0.0000	0.00011	2.00
100	100.000042	100.0000	0.0000	0.00016	2.00
200	200.000041	200.0000	0.0000	0.00028	2.00

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

Certificate No. : 23-148800  
Sample Code : 23-56203-002


## REPORT OF CALIBRATION

## Result of Calibration :

## 4. Eccentric or off-centre loading

Deviation of the measurement value through off-center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan	<input checked="" type="radio"/> Circle <input type="radio"/> Triangular <input type="radio"/> Rectangular	Test weight : 100 Unit : g
Range	220	
Position	Reading of indicator	Reading of indicator
1	100.0000	-
2	100.0000	-
3	100.0000	-
4	99.9999	-
5	100.0000	-
6	100.0000	-
Maximum difference	0.0001	-

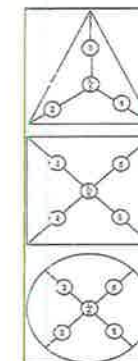

## Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019
2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : \*

\* Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1)

5. Reference standard instrument :

Instrument	Class	ID No.	Certificate No.	Due Date
1) STANDARD WEIGHT 1 mg to 1 kg	E2	LB-WE-79	23-105642	10 September 2024

End of Report

6. Ambient conditions	Min	Max
Temperature (°C)	24.4	24.8
Relative Humidity (%Rh)	39.9	41.1
Air pressure (hPa)	1012.2	1012.8

SK

S K SALES AND SERVICE CO.,LTD.  
194/56, 194/57 Thakham Rd. Samoe Dam  
Bang Khun Thien Bangkok 10150  
Tel. : 02-417-2144 Fax : 02-417-2155



## Certificate of Calibration

Reference No. : C03190/2309-025 Certificate No. : S2309-3014  
Customer : Eastern Thai Consulting 1992 Co.,Ltd. Page 1 of 2  
683 Moo 11, Sukhaphiban 8, Tambol Nongkham,  
Siracha District, Chonburi 20230, Thailand  
Equipment : Incubator  
Manufacturer : Lovibond  
Model : TC445S  
Serial No. : 0223/007275  
ID No. :  
Received Date : 15 September 2023  
Calibrated Date : 15 September 2023  
Issued Date : 18 September 2023  
Environment :

	Minimum Value	Maximum Value
Ambient Temperature ( °C )	27.5	28.1
Relative Humidity ( % RH )	57	58
AC Line Voltage ( VAC )	224	226
Place Of Calibration	Production Line	
Calibrated by	Mr. Teerasak Chalyaporn	

### Calibration Method

In-house method : SK-WI-23 base on Thai Laboratory Accreditation Scheme Publication Reference G-20

### Condition of this result of calibration

#### 1. Reference standard instrument

Instrument	Serial No.	Certificate No.	Due Date
1) Data acquisition/Switch unit	MY44047397	L2305-268	4 November 2023
2) Multiplexer Module	MY41105123	L2305-268	4 November 2023

2. This result of calibration was found accurate as shown on date and place of calibration only

3. This certificate can be traceable to International System of Unit :

- Through Thailand Institute of Scientific And Technological Research (TISTR)

Approved by

☒ Mr. Suphachai Saksri ☐ Mr. Phayak Toolit ☐ Miss Tantaraporn Pettong

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k = 2.0$  ,providing a level of confidence level of approximately 95 %

This certificate may not be reproduced other than in full except with the prior written approval of the S K Sales And Service Company Limited

Certificate No. : S2309-3014

Page 2 of 2

Table1 General Information

Working Area ( W*L*H )	60 *56 *145 cm
Fresh Air	OFF

Table2 Chamber Performance


Setting Temperature ( °C )	Average Indicating Temperature ( °C )	Measured Stability ( ± °C )	Measured Uniformity ( °C )	Overall Variation ( °C )
20.0	20.0	0.37	0.64	0.98

Table3 Temperature Distribution

Setting Temperature ( °C )	Average Standard Reading ( °C )									Uncertainty ( ± °C )
	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9	
20.0	19.52	19.40	19.70	19.43	19.33	19.39	19.45	19.58	19.67	0.55

Resolution : 0.1 ( °C )

\* Probe No. 9 is Reference Probe



Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The reported uncertainty of measurement were excluded Uniformity and Stability

\*\* End of Calibration Report \*\*

COPY

*[Signature]*



## REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 22-136844

Sample Code : 22-51164-006

## Results of Calibration

## Notes

1. Sensor installation locations
  - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
  - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :  
W = 60 cm ; D = 70 cm ; H = 124 cm
3. Air valve or fresh air level : Off
4. Fan level : open
5. The quoted uncertainty includes\* Stability of chamber and loading effect in chamber at 20% of uniformity \*.
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC\* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

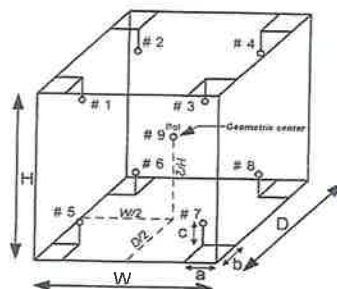


Figure: Example of sensor  
installation Positions

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

**COPY**



Page 1 of 3

## CERTIFICATE OF CALIBRATION

Certificate No. : 23-040768  
Sample Code : 23-16178-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapiban 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : Lovibond Model : Tc445S

Serial No. : 0520/005227 ID No. : LABE 19/5

Date of Receipt : 21 April 2023 Date of Calibration : 21 April 2023

## Condition of Calibration

1. Environment
- |                           |   |         |           |   |         |           |
|---------------------------|---|---------|-----------|---|---------|-----------|
| 1.1 Ambient temperature   | : | Maximum | 36.1 °C   | : | Minimum | 34.5 °C   |
| 1.2 Relative humidity     | : | Maximum | 51.8 %    | : | Minimum | 49.3 %    |
| 1.3 Line voltage supplied | : | Maximum | 224.7 VAC | : | Minimum | 221.9 VAC |

## 2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

## 3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-08 (RTD-239 to RTD-247)	22-077888	09 August 2023

## 4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Sarawoot Thammo  
Scientist

Approved by

(Mr. Somchai Neampunt)

Signed for Director

Issue date 24 April 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

NSC-TISI-TIS17025  
CALIBRATION 0152

Page 2 of 3

## REPORT OF CALIBRATION

Certificate No. : 23-040768  
Sample Code : 23-16178-002

## Results of Calibration

Resolution : 0.1 °C

## 1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor <i>k</i>
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 <sup>Ref</sup>		
20	20.0	20.0	20.06	19.92	19.96	19.89	19.93	20.08	19.97	19.79	19.86	0.42	2.00

## 2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.32	0.37	0.85

## Notes

- UUC\* = Unit Under Calibration

NSC-TISI-TIS17025  
CALIBRATION 0152

Page 3 of 3

## REPORT OF CALIBRATION


Certificate No. : 23-040768

Sample Code : 23-16178-002

## Results of Calibration

## Notes

1. Sensor installation locations
  - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
  - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :  
W = 60 cm ; D = 56 cm ; H = 146 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes" Stability of chamber and loading effect in chamber at 20% of uniformity ".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC\* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

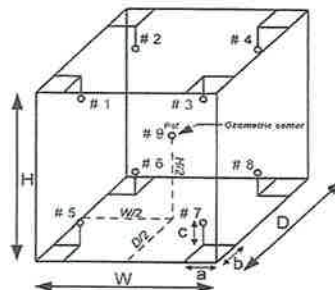Figure: Example of sensor  
installation Positions

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

End of Report

COPY

## CERTIFICATE OF CALIBRATION

Certificate No. : 24-046203

Sample Code : 24-18906-002

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Laboratory)

Equipment : Temperature controlled enclosures (Incubator)

Manufacturer : Lovibond Model : Tc445S

Serial No. : 0520/005227 ID No. : LABE 19/5

Date of Receipt : 18 April 2024 Date of Calibration : 18 April 2024

## Condition of Calibration

1. Environment
- |                           |   |         |           |   |         |           |
|---------------------------|---|---------|-----------|---|---------|-----------|
| 1.1 Ambient temperature   | : | Maximum | 35.0 °C   | : | Minimum | 33.7 °C   |
| 1.2 Relative humidity     | : | Maximum | 69.1 %    | : | Minimum | 50.0 %    |
| 1.3 Line voltage supplied | : | Maximum | 222.5 VAC | : | Minimum | 218.8 VAC |

## 2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

## 3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-08 (RTD-248 to RTD-256)	23-084070	06 August 2024

## 4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Sarawoot Thammo  
Scientist

Issue date 19 April 2024

Approved by

  
(Mr. Nuttaput Timula)

Signed for Director

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC)

## REPORT OF CALIBRATION

Certificate No. : 24-046203

Sample Code : 24-18906-002

## Results of Calibration

Resolution : 0.1 °C

## 1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9		
20	20.5	20.0	20.28	19.86	19.90	19.91	19.82	20.10	20.01	19.89	19.75	0.59	2.00

## 2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
20	0.45	0.85	1.31

## Notes

- UUC\* = Unit Under Calibration



**COPY**

## REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 24-046203

Sample Code : 24-18906-002

## Results of Calibration

## Notes

1. Sensor installation locations
  - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
  - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :  
W = 60 cm ; D = 56 cm ; H = 146 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC\* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

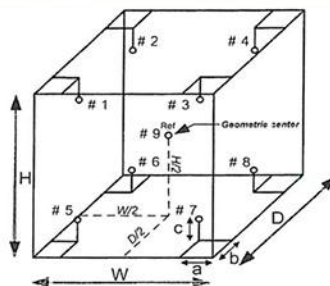


Figure: Example of sensor  
installation Positions

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -



COPY

## CERTIFICATE OF CALIBRATION

Certificate No. : 24-001944  
Sample Code : 24-00963-001Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert Model : UM 400

Serial No. : 900982 ID No. : LABE 17/1

Date of Receipt : 09 January 2024 Date of Calibration : 09 January 2024

## Condition of Calibration

1. Environment
- |                           |           |           |           |           |
|---------------------------|-----------|-----------|-----------|-----------|
| 1.1 Ambient temperature   | : Maximum | 30.6 °C   | : Minimum | 29.2 °C   |
| 1.2 Relative humidity     | : Maximum | 57.5 %    | : Minimum | 46.4 %    |
| 1.3 Line voltage supplied | : Maximum | 229.5 VAC | : Minimum | 222.5 VAC |

## 2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

## 3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-10 (RTD-257 to RTD-265)	23-066256	29 June 2024

## 4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Sarawoot Thammo  
Scientist

Approved by

(Mr. Somchai Nearnpunt)

Signed for Director

Issue date 09 January 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

## REPORT OF CALIBRATION

Certificate No. : 24-001944  
Sample Code : 24-00963-001

## Results of Calibration

Resolution : 0.1 °C

## 1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C)	UUC* reading (°C)	Measured temperature at each positions (°C)									Uncertainty ± (°C)	Coverage factor k
			# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9 <sup>Ref</sup>		
60	60.0	60.0	60.04	59.90	59.81	59.84	59.47	59.91	60.08	59.98	59.87	0.25	2.00
85	85.0	85.0	86.07	85.75	85.58	85.62	84.69	85.83	86.28	85.94	85.77	0.34	2.00

## 2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
60	0.11	0.49	0.80
85	0.09	1.13	1.72

## Notes

- UUC\* = Unit Under Calibration



## REPORT OF CALIBRATION

Page 3 of 3

Certificate No. : 24-001944

Sample Code : 24-00963-001

### Results of Calibration

#### Notes

1. Sensor installation locations
  - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
  - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :  
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC\* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

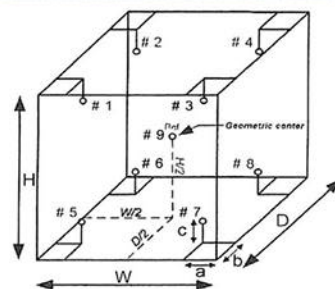


Figure: Example of sensor  
installation Positions

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

**COPY**



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com



CERTIFICATE No : 23T10864  
REFERENCE No : 71117-1

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : LIQUID IN GLASS THERMOMETER  
MANUFACTURER : PRECISION  
MODEL : 0 °C TO 100 °C  
SERIAL No : 43560  
ID No : LABE 16/1  
RESOLUTION : 0.1 °C  
TYPE : TOTAL IMMERSION  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 MOO 11, SUKHAPIBAN 8 ROAD, NONGKHAM,  
SRIRACHA, CHONBURI 20230

CALIBRATED BY : CHARUKIT L.  
CALIBRATION DATE : 09-Nov-23  
APPROVED BY : PONGSAK J.  
ISSUED DATE : 09-Nov-23  
RECEIVED DATE : 02-Nov-23

**COPY**

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.



QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com

CERTIFICATE No : 23T10864

PAGE : 2 OF 2

## Calibration Report

EQUIPMENT : LIQUID IN GLASS THERMOMETER  
MANUFACTURER : PRECISION  
MODEL : 0 °C TO 100 °C  
ID No : LABE 16/1  
RESOLUTION : 0.1 °C  
RECEIVED DATE : 02-Nov-23  
AMBIENT TEMPERATURE : 23 °C ± 3 °C  
SERIAL NUMBER : 43560  
TYPE : TOTAL IMMERSION  
CALIBRATION DATE : 09-Nov-23  
RELATIVE HUMIDITY : 50 %RH ± 20 %RH

### CONDITION OF THIS RESULTS OF CALIBRATION

- THIS INSTRUMENT WAS CALIBRATED BASED ON ASTM E77:1992 BY COMPARISON WITH STANDARD PLATINUM RESISTANCE THERMOMETER (SPRT) INTO LIQUID BATH TEMPERATURE CONTROLLER. THE TEMPERATURE SCALE USED WAS BASED ON ITS-90.
- REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD THERMOMETER	1502	77964	23T3927	08-Mar-24
2) SPRT PROBE	5614	636636	23T3927	08-Mar-24
3) PRECISION BATH	7320	A21105	22T13199	14-Dec-23
4) PRECISION BATH	CTR-40	A68155	22T13198	09-Dec-23
5) PRECISION BATH	6045	3C023	22T13200	19-Dec-23
- THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
- THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
- THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-  
- NATIONAL INSTITUTE OF METROLOGY (THAILAND).

### RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	EMERGENT STEM TEMPERATURE (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
0.009	0.0	60	0.0090	N/A	0.26
25.01	25.0	165	0.0050	N/A	0.26
50.00	50.0	275	0.0040	N/A	0.26
99.991	100.0	360	-0.009	29.3	0.26

### UUC\* : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.  
END OF CALIBRATION REPORT

**COPY**



## CERTIFICATE OF CALIBRATION

Page 1 of 3

Supersede to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapibarn 8 Rd., Nongkham,  
Sriracha, Chonburi 20230Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.  
(Laboratory)

Equipment : pH Meter

Manufacturer : METTLER TOLEDO

Model : SevenCompact S220

Serial No. : B448305208

ID No. : LABE 11/4

Date of Receipt : 09 January 2024

Date of Calibration : 09 January 2024

## Condition of Calibration

## 1. Environment

1.1 Ambient temperature : 22.4 ± 0.2 °C 1.2 Relative humidity : 56.4 % ± 2.1 %

## 2. Calibration method

In house method WI-CL-019: based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

## 3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	23E3244	03 October 2024
3.2 Digital Thermometer	LB-TH-33	23-098974	25 August 2024
Certified Reference Material		Lot. No.	Ref No.
3.3 Buffer Solution pH 4.008	919273	PH216.L5	24 September 2025
3.4 Buffer Solution pH 6.986	941727	PH107.L5	06 November 2024
3.5 Buffer Solution pH 9.997	919278	PH220.L5	24 September 2024

## 4. This certificate is traceable to the international system of unit (SI Unit).

4.1 Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).

4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

4.4 Buffer Solution No. 3.4 traceable to CPA chem (CPA RefN HARNED CELL LotN 61275737; CPA RefN HARNED CELL LotN 61273986 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

## 6. Condition of calibration item : Normal

Calibrated by Mr. Nuttaput Timula

Approved by

(Mr. Sornchai Neampunt)

Scientist

Issue date 31 January 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



## REPORT OF CALIBRATION

Page 2 of 3

Supersede to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Equipment : pH Meter Resolution : 0.01 pH ; 0.1 mV ; 0.1 °C  
Manufacturer : METTLER TOLEDO Model : SevenCompact S220  
Serial No. : B448305208 ID No. : LABE 11/4  
Range : -2.000 pH to 20.000 pH ; ± 2000.0 mV ; -5.0 °C to 130.0 °C

## Results of Calibration

## Part 1. DC Voltage measurement

pH Meter Serial No. : B448305208

Nominal Value	Applied DC Voltage	Average indicator reading		Uncertainty	Coverage factor
		mV	pH		
0	414.113	413.9	0.00	± 0.083	2.00
4	177.477	177.4	4.00	± 0.083	2.00
7	0.000	0.1	7.00	± 0.083	2.00
10	-177.477	-177.3	10.00	± 0.083	2.00
14	-414.113	-413.8	14.00	± 0.083	2.00

## Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Electrode Serial No. : 2453982

Three-Point Calibration at pH4, pH7 and pH10 Percent Slope : 98.3

Standard Buffer Solution	Average indicator reading		Error Value	Uncertainty	Coverage factor
	pH	mV			
pH (@ 25 °C)					
4.008	4.01	182.1	0.002	± 0.010	2.00
6.986	7.00	7.8	0.014	± 0.011	2.00
9.997	10.01	-167.2	0.013	± 0.011	2.00

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

NSC-TISI-TIS17025  
CALIBRATION 0152

Page 3 of 3

## REPORT OF CALIBRATION

Supersede to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Equipment : pH Meter (Digital Thermometer with sensor)

## Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220  
Serial No. : B448305208 ID No. : LABE 11/4  
Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

## Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM  
Serial No. : 2453982 ID No. : N/A

## Condition of Calibration

1. Environment 1.1 Ambient temperature : 22.6 °C ± 0.1 °C  
1.2 Relative humidity : 55.1 % ± 3.3 %

## 2. Calibration method

- 2.1 The calibration use in house method WI-CL-021 : by comparison with standard thermometer  
2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.  
2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

## 3. Reference standard instrument

Instrument	Model	ID. No.	Certificate No.	Due date
3.1 Resistance Thermometer	PT-100	RTD-90	23-098974	25 August 2024
3.2 Thermometer Readout	GT-11	LB-TH-33	23-098974	25 August 2024

## 4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

## 5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

## Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration			Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C	Correction value °C		
25	25.000	120	25.0	0.000	± 0.14	2.00

## Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of report -



Certificate No. : 22-052238  
Sample Code : 22-19150-003

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapiban 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee  
Scientist

Approved by : ( Mr. Somchai Neampunt )  
Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052238  
Sample Code : 22-19150-003

## REPORT OF CALIBRATION

Equipment : Standard Weight 50 g  
Manufacturer : METTLER TOLEDO  
Class : F1  
Serial No. : N/A  
ID No. : LABE 10/1

Result of Calibration : ☒ Without adjustment ☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature ( $t_{ref}$ ) of 20°C, the conventional mass is the mass of a reference weight of a density ( $\rho_{ref}$ ) of 8000 kg.m<sup>-3</sup> which it balances in air of a reference density ( $\rho_0$ ) of 1.2 kg.m<sup>-3</sup>

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
50 g	-0.324	49.999676 g	0.10	0.30	LABE 10/1

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.0$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

Certificate No. : 22-052238

Sample Code : 22-19150-003

Page 3 of 3

## REPORT OF CALIBRATION

## Condition of Calibration:

1. Ambient Conditions : Temperature 20 °C  $\pm$  1.5°C, Relative humidity 50%  $\pm$  10% and air density 1.20 kg/m<sup>3</sup>

2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

( Instrument number 1).

5. Condition of Calibration item: Normal

## 6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY



Certificate No. : 22-052239  
Sample Code : 22-19150-004

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapiban 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee  
Scientist

Approved by

( Mr. Somchai Neampunt )

Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052239  
Sample Code : 22-19150-004

## REPORT OF CALIBRATION

Equipment : Standard Weight 100 g  
Manufacturer : N/A  
Class : N/A  
Serial No. : N/A  
ID No. : LABE 10/2

### Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature ( $t_{ref}$ ) of 20°C, the conventional mass is the mass of a reference weight of a density ( $\rho_{ref}$ ) of 8000 kg.m<sup>-3</sup> which it balances in air of a reference density ( $\rho_0$ ) of 1.2 kg.m<sup>-3</sup>

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
100 g	-0.171	99.999829 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.0$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY



Certificate No. : 22-052239

Sample Code : 22-19150-004

## REPORT OF CALIBRATION

## Condition of Calibration

1. Ambient Conditions : Temperature  $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$ , Relative humidity  $50\% \pm 10\%$  and air density  $1.18 \text{ kg/m}^3$ 

2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)

3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

( Instrument number 1).

5. Condition of Calibration item: Normal

## 6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

COPY



Certificate No. : 22-052237  
Sample Code : 22-19150-002

## CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.  
683 Moo 11, Sukhapiban 8 Rd., Nongkham,  
Sriracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited  
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee  
Scientist

Approved by : ( Mr. Somchai Neampunt )  
Signed for Director

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052237  
Sample Code : 22-19150-002

## REPORT OF CALIBRATION

Equipment : Standard Weight 50 g  
Manufacturer : N/A  
Class : N/A  
Serial No. : N/A  
ID No. : LABE 10/4

### Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature ( $t_{ref}$ ) of 20°C, the conventional mass is the mass of a reference weight of a density ( $\rho_{ref}$ ) of 8000 kg.m<sup>-3</sup> which it balances in air of a reference density ( $\rho_a$ ) of 1.2 kg.m<sup>-3</sup>

Description	Deviation	Conventional Mass	Expanded Uncertainty	Maximum Permissible Error	ID No.
	(mg)		(mg)	± (mg)	
50 g	-0.111	49.999889 g	0.10	0.30	LABE 10/4

The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2.0$ , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

COPY

Certificate No. : 22-052237  
Sample Code : 22-19150-002

Page 3 of 3

## REPORT OF CALIBRATION

### Condition of Calibration

1. Ambient Conditions : Temperature  $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$ , Relative humidity  $50\% \pm 10\%$  and air density  $1.18 \text{ kg/m}^3$
2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)
3. Reference standard instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited

( Instrument number 1).

5. Condition of Calibration item: Normal

### 6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -



COPY



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor7 Rama4 Road  
Silom Bangrak Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



# Certificate of Calibration

Number of Page(s) 1 of 3

**Certificate No.** BSCC-UV-152/23  
**Equipment** UV/Vis Spectrophotometer  
**Model** UV-1800  
**Manufacturer** Shimadzu  
**Serial No.** A11635101643 CD  
**ID No.** N/A  
**Date of receipt** 25 April 2023  
**Date of calibration** 25 April 2023  
**Date of issue** 27 April 2023

**Customer name** Eastern Thai Consulting 1992 Co.,Ltd

**Address** 683 Moo 11, Sukkaphibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

**Temperature** (22.4-23.1) °C (On site)  
**Humidity** (44.5-45.2) %RH (On site)

**Equipment condition** Good Operation

**Calibration Location** Analysis Department

**Calibration Procedure** In-house method WI-UV-702-01 based on ASTM E275-01

**Traceability** Wavelength Accuracy is traceable to certificate No. 94780 and 94775  
Photometric Accuracy is traceable to certificate No. 94808 and 100147  
Stray Light is traceable to certificate No. 94791  
The above certificate are traceable to SI unit through Sarna Scientific Ltd.  
(UKAS accredited calibration laboratory NO. 0659)

**Calibrated by** Mr.Pannaphong Phanmekakul

Approved by

**Mr.Kanchit Choothep**  
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor7 Rama4 Road  
Silom Bangrak Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



# Certificate of Calibration

**Certificate No.** BSCC-UV-152/23

**Number of Page(s)** 2 of 3

## Calibration Results:

### 1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.65	-0.06	0.18
445.82	445.80	-0.02	0.18
536.52	536.35	-0.17	0.18
741.02	740.99	-0.03	0.18
879.41	879.27	-0.14	0.18

### 2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000 0.7311	0.0000 0.7313	0.0000 0.0002	0.0075 0.0075
257	CNR CNR	CNR CNR	CNR CNR	CNR CNR
313	CNR CNR	CNR CNR	CNR CNR	CNR CNR
350	0.0000 0.6306	0.0000 0.6314	0.0000 0.0008	0.0075 0.0075

\*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

# Certificate of Calibration

Certificate No. **BSCC-UV-152/23**

Number of Page(s) 3 of 3

## Calibration Results:

### 3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm A$ )
420.0	0.0000	0.0000	0.0000	0.0042
	0.5488	0.5508	0.0020	0.0042
	0.7527	0.7535	0.0008	0.0042
	1.0756	1.0758	0.0002	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5391	0.5406	0.0015	0.0042
	0.7355	0.7360	0.0005	0.0042
	1.0509	1.0501	-0.0008	0.0042
465.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
546.1	0.0000	0.0000	0.0000	0.0042
	0.5045	0.5044	-0.0001	0.0042
	0.6884	0.6885	0.0001	0.0042
	0.9816	0.9808	-0.0008	0.0042
590.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5183	0.5178	-0.0005	0.0042
	0.6864	0.6868	0.0004	0.0042
	0.9747	0.9739	-0.0008	0.0042

\*CNR = Customer not request

### 4. Stray Light\*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
200.75 $\pm$ 0.11nm	200.72	0.9630	2.0164

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A  
\*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is base on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\*\*\*End of Certificate\*\*\*

The above results are valid exclusively for the calibrated item(s) as mention in this report / Certificate. Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor7 Rama4 Road  
Silom Bangrak Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



## Certificate of Calibration

Number of Page(s) 1 of 3

**Certificate No.** BSCC-UV-146/24  
**Equipment** UV/Vis Spectrophotometer  
**Model** UV-1800  
**Manufacturer** Shimadzu  
**Serial No.** A11635101643 CD  
**ID No.** LABE 03/2  
**Date of receipt** 22 April 2024  
**Date of calibration** 22 April 2024  
**Date of issue** 29 April 2024

**Customer name** Eastern Thai Consulting 1992 Co., Ltd.

**Address** 683 Moo 11, Sukkhaphibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

**Temperature** (22.9-24.1) °C (On site)  
**Humidity** (41.7-46.9) %RH (On site)

**Equipment condition** Good Operation

**Calibration Location** Analysis Department

**Calibration Procedure** In-house method WI-UV-702-01 based on ASTM E275-01

**Traceability** Wavelength Accuracy is traceable to certificate No. 116614 and 116613  
Photometric Accuracy is traceable to certificate No. 116210 and 116224  
Stray Light is traceable to certificate No. 116616  
The above certificate are traceable to SI unit through Starna Scientific Ltd.  
(UKAS accredited calibration laboratory NO. 0659)

**Calibrated by** Mr.Poomjai Korsawatvorakul

Approved by

**Mr.Sonthi Temboonsakdi**  
Service Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

**COPY**



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor7 Rama4 Road  
Silom Bangrak Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



## Certificate of Calibration

**Certificate No.** BSCC-UV-146/24

Number of Page(s) 2 of 3

### Calibration Results:

#### 1.Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.75	0.04	0.18
445.82	445.89	0.07	0.18
536.52	536.50	-0.02	0.18
741.02	741.01	-0.01	0.18
879.41	879.33	-0.08	0.18

#### 2.Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000 0.7415	0.0000 0.7387	0.0000 -0.0028	0.0075 0.0075
257	CNR CNR	CNR CNR	CNR CNR	CNR CNR
313	CNR CNR	CNR CNR	CNR CNR	CNR CNR
350	0.0000 0.6406	0.0000 0.6395	0.0000 -0.0011	0.0075 0.0075

\*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

**COPY**



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor7 Rama4 Road  
Silom Bangrak Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barascientific.com



# Certificate of Calibration

Certificate No. **BSCC-UV-146/24** Number of Page(s) **3 of 3**

## Calibration Results:

### 3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty ( $\pm A$ )
420.0	0.0000	0.0000	0.0000	0.0042
	0.5715	0.5729	0.0014	0.0042
	0.7087	0.7087	0.0000	0.0042
	1.0987	1.1005	0.0018	0.0042
440.0	0.0000	0.0000	0.0000	0.0042
	0.5561	0.5578	0.0017	0.0042
	0.6968	0.6969	0.0001	0.0042
	1.0757	1.0774	0.0017	0.0042
465.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
546.1	0.0000	0.0000	0.0000	0.0042
	0.5193	0.5213	0.0020	0.0042
	0.6937	0.6940	0.0003	0.0042
	1.0411	1.0428	0.0017	0.0042
590.0	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	0.0000	0.0000	0.0000	0.0042
	0.5605	0.5624	0.0019	0.0042
	0.7579	0.7583	0.0004	0.0042
	1.1131	1.1138	0.0007	0.0042

\*CNR = Customer not request

### 4. Stray Light\*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)		
	Wavelength (nm)	Transmission (%T)	Absorbance (A)
201.33 $\pm$ 0.11nm	200.80	0.9750	2.0111

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

\*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

\*\*\*End of Certificate\*\*\*

The above results are valid exclusively for the calibrated item(s) as mentioned in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.

**COPY**

## Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

## Meter Console Information

Console Model: XC572V  
 Console serial: 1110070  
 DGM Model #: SK25EX  
 DGM Serial #: 0005413

## Calibration Condition

Calibration Date: 3-Jul-23  
 Due Date: 2-Jul-24  
 Cal Report No.: WDS-SV660107  
 Ambient Temp (°C): 25  
 Pressure (mm Hg): 758  
 Relative Humidity (%): 60

## Factors/Conversion

Std. Temp. (°K): 298  
 Std. Pressure (mm Hg): 760  
 K<sub>1</sub> (K/mm Hg): 0.3857

## Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Nov. 2022  
 WTM Serial: 600245 Gamma: 1.0000

## UUT Meter (DGM)

Run Time (minutes)	DGM Onifice (mm H <sub>2</sub> O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15.00	13.0	599.3828	599.5462	27	27	20.05690	20.22163	28	27
10.00	25.0	599.5689	599.7246	27	26	20.24425	20.39999	27	27
8.00	50.0	599.7405	599.9176	26	26	20.41592	20.59344	27	27
7.00	80.0	599.9333	600.1337	26	26	20.60920	20.81034	27	27
5.00	120.0	600.1559	600.3319	26	26	20.83271	21.00950	27	27

## Reference Meter (WTM)

## Standardized Data

Test Meter		Reference Meter		Correction Factor		Flow Rate		AH@ (mm H <sub>2</sub> O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation	
V <sub>measured</sub> (m <sup>3</sup> )	Q <sub>measured</sub> m <sup>3</sup> /min	V <sub>ref</sub> (m <sup>3</sup> )	Q <sub>ref</sub> m <sup>3</sup> /min	(Y)	(ΔY)	Q <sub>measured</sub> (m <sup>3</sup> /min)	ΔH <sub>0</sub>	ΔΔH <sub>0</sub>	
0.159	0.011	0.160	0.011	1.005	0.010	0.011	50.181	2.747	
0.152	0.015	0.152	0.015	0.996	0.000	0.015	48.096	0.662	
0.174	0.022	0.173	0.022	0.995	-0.001	0.022	47.605	0.171	
0.197	0.028	0.196	0.028	0.993	-0.003	0.028	45.688	-1.747	
0.174	0.035	0.172	0.034	0.990	-0.006	0.034	45.602	-1.832	
				0.996	= Y Avg		47.434	= ΔH@ Avg	

Pass/Fail Result: 

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is  $\pm 0.02$   
 Note: For  $\Delta H_{0,0}$ , onifice pressure differential that equates to 0 /scfm (0.0212m<sup>3</sup>/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is  $\pm 0.2$  inches (5.1mm) H<sub>2</sub>O

Approved By: \_\_\_\_\_

(Patpasu Chaisana)  
 Service Manager

Date: 3-Jul-23

COPY

## TEMPERATURE DISPLAY CALIBRATION

## Calibration Conditions

Cal Date: 3-Jul-23  
 Due Date: 2-Jul-24  
 Cal Report No.: WDS-SV660107  
 Ambient Temp (°C): 25  
 Pressure (mm Hg): 758  
 Humidity (%): 60

## Meter Console Information

Console Model: XC572V  
 Console serial: 1110070  
 Temp Indicator Model: 765-KF  
 Temp Indicator Serial: JC17852

## Reference Equipment

Temp Simulator Model: FLUKE 714B  
 Serial No: 60590035

## Temperature Sensor Calibration

Reference Point	Ref. Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
1	-18.0	-17.0	1.0
2	36.0	37.0	1.0
3	93.0	93.0	0.0
4	149.0	149.0	0.0
5	260.0	259.0	1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	594.0	-1.0
9	816.0	816.0	0.0
10	1038.0	1039.0	-1.0
		Maximum	1.0

PASS

## Note

For valid test results, the maximum difference between temperature readings should  $\leq 1.0^{\circ}\text{C}$  (EPA Method 5, Section 6.1.1.8)  
 Perform all TC Channel calibrations. Except meter (DGM) channel

## DGM Out Temperature Sensor Calibration

Temperature point	Ref. Thermometer Temperature	Thermocouple Display Temperature	Temperature Difference
#	°C	°C	°C
Ambient	26.5	27.0	-0.5
Heat	100.5	102.5	-2.0

## Difference Rang

DGM Out Temp. Diff.  $\pm 3^{\circ}\text{C}$ 

PASS

Approved By: \_\_\_\_\_

Patpasu Chaisana  
 Service Manager

บริษัท วิสโดม ไซนซ์ แอนด์ เซอร์วิส กรุ๊ป จำกัด  
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Address: 9/115 Lumpini Town Ville Rajchaphruek-Pinkao Village No. 4, Bang Khamun, Bang Kruai, Nonthaburi 11130 Thailand  
 Tel: 090-660 1332, 094-598 1944, 094-704-1020



## ELAPSED TIMER CALIBRATION

### Meter Console Information

Model #: XC572V  
Serial #: 1110070  
Elapsed Timer Model #: C342-1484  
Elapsed Timer Serial #:

### Calibration Conditions

Cal. Date : 03-Jul-23  
Due Date : 02-Jul-24  
Cal. Report No. : WDS-SV660107  
Ambient Temp. (°C) : 25  
Pressure (mm Hg) : 758  
Humidity (%) : 60

### Reference Equipment

Calibration Standard: JS-307  
Method Reference: Compare

Run Time Elapsed STD.	Calibration Results					
	Elapsed Timer		Average Time		Deviation	
Minute	1	2	3	4	Minute	Minute
2.00	Minute 2.00	Minute 2.00	Minute 2.00	Minute 2.00	2.000	0.000
3.00	3.00	3.00	3.00	3.00	3.000	0.000
5.00	5.00	5.00	5.00	5.00	5.000	0.000
7.00	7.00	7.00	7.00	7.00	7.000	0.000
9.00	9.00	9.00	9.00	9.00	9.000	0.000

Approved By

( Patpasu Chalsana )  
Service Engineer

**WISDOM  
SCIENCE**

บริษัท วิสโดม ไซนซ์ จำกัด  
WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

## Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

## Meter Console Information

Console Model : MC572V  
Console serial : 0504003  
DGM Model #: SK25EX  
DGM Serial #: 00009854

## Calibration Condition

Cal. Date: 22-Apr-24  
Due Date: 23-Apr-25  
Cal. Report No.: WDS-SV6704001  
Ambient Temp (°C): 25  
Pressure (mm Hg): 758  
Relative Humidity (%): 60

## Factors/Conversion

Std. Temp (°K): 298  
Std. Pressure (mm Hg): 760  
K: (K/mm Hg): 0.3857

## Reference Equipment

WTM Model: W-NKoDa-5B WTM Cal. Due Date: Dec 2023  
WTM Serial: 600245 Gamma: 1.0000

Run Time (minutes)	DGM Orifice (mm H <sub>2</sub> O)	UUT Meter (DGM)				Reference Meter (WTM)			
		Volume		Outlet Temp		Volume		Outlet Temp	
a	P <sub>mid</sub>	Initial V <sub>mid</sub>	Final V <sub>mid</sub>	Initial t <sub>in</sub>	Final t <sub>out</sub>	Initial V <sub>in</sub>	Final V <sub>out</sub>	Initial t <sub>in</sub>	Final t <sub>out</sub>
15.00	13.0	144.5926	144.7699	26	27	60.06607	60.24392	29	28
10.00	25.0	144.8168	144.9795	27	27	60.29098	60.45472	27	27
8.00	50.0	145.0164	145.2002	28	28	60.49135	60.67317	29	27
7.00	80.0	145.2238	145.4291	28	28	60.69691	60.90186	29	28
5.00	120.0	145.4909	145.6692	28	29	60.96349	61.14145	27	26


## Standardized Data

Test Meter		Reference Meter		Correction Factor		Flow Rate		VH@ (mm H <sub>2</sub> O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation	
V <sub>std</sub> (m <sup>3</sup> )	Q <sub>std</sub> m <sup>3</sup> /min	V <sub>ref</sub> (m <sup>3</sup> )	Q <sub>ref</sub> m <sup>3</sup> /min	(Y)	(ΔY)	Q <sub>ref</sub> (m <sup>3</sup> /min)	ΔH <sub>B</sub>	ΔΔH <sub>B</sub>	
0.173	0.012	0.173	0.012	0.997	0.003	0.012	43.309	-0.858	
0.159	0.016	0.160	0.016	1.004	0.011	0.016	43.381	-0.787	
0.179	0.022	0.176	0.022	0.984	-0.009	0.022	45.447	1.280	
0.201	0.029	0.199	0.028	0.989	-0.005	0.028	44.202	0.035	
0.175	0.035	0.174	0.035	0.994	0.000	0.035	44.497	0.330	
				0.993	= Y Avg				
								44.167	= ΔH <sub>B</sub> Avg

Pass/Fail Result: Pass

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ±0.02

Note: For ΔH<sub>B</sub>, onifice pressure differential that equates to 0.75cfm (0.0212m<sup>3</sup>/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H<sub>2</sub>O

Approved By:   
(Patpasu Chaisana)  
Service Manager

Date: 22-Apr-24

COPY

## TEMPERATURE DISPLAY CALIBRATION

Meter Console Information		Calibration Conditions		Reference Equipment	
Console Model : MC572V	Cal. Date: 22-Apr-24	Cal. Date: 23-Apr-25	Temp. Meter Model: Fluke 714B	Serial No: 60590035	Cal. Date: 07-Apr-24
Console serial: 0504003	Due Date: 23-Apr-25	Cal. Report No: WDS-SV6704001	Temp. Meter Model: Fluke 179	Serial No: 58820112	Cal. Date: 06-Feb-24
Temp Indicator Model: 785-KF	Ambient Temp (°C): 25	Pressure (mm Hg): 758			
Temp Indicator Serial: JC056330	Humidity (%): 60				

## Temperature Sensor Calibration

Reference Point	Ref. Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
1	-18.0	-17.0	1.0
2	38.0	37.0	1.0
3	93.0	93.0	0.0
4	149.0	150.0	-1.0
5	260.0	259.0	1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	593.0	0.0
9	816.0	816.0	0.0
10	1038.0	1038.0	0.0
Maximum			1.0

## Note

\* For valid test results, the maximum difference between temperature readings should be ±1.0°C (EPA Method 5, Section 6.1.1.8)  
Perform all TC Channel calibrations. Except meter (DGM) channel

PASS

## DGM Out Temperature Sensor Calibration

Temperature point	Ref. Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
Ice	0.0	1.0	-1.0
Ambient	26.5	26.0	0.5
Heat	109.3	110.0	-0.7

PASS

## Note

The temperatures of the thermocouple and reference thermometers shall agree to within ±2 °F (EPA Method 5, section 10.5)

Approved By:

(Patpasu Chaisana)  
Service Manager

WISDOM SCIENCE

COPY

# Certificate of Calibration - Supplemental

METHOD 5 PRE-TEST CONSOLE CALIBRATION

## Nomenclature

$P_b$  - Barometric Pressure  
 DGM - Dry Gas Meter  
 $K_1$  - Constant based on standard temp and press  
 $\Phi$  - Run time, in minutes  
 $P_m$  -  $\Delta H$  (Meter Pressure, gauge)  
 $V_m$  - Volume collected by test meter, corrected for STP  
 $Q_{m(std)}$  - Calculated flow rate of test meter  
 $K'$  - Critical orifice coefficient  
 $P_w$  - Measured pressure of reference meter  
 $T_w$  - Temperature measured in reference meter  
 $T_m$  - Temperature measured in test meter  
 $Y$  - Ratio of volume collected from test meter and orifice  
 $sc$  - Scaling Factor  
 $Counts_{sc}$  - Number of pulse counts, standardized  
 $Counts_{raw}$  - Number of raw pulse counts of a calibration run

## Equations

$$V_{m(std)} = Y * K_1 \frac{V_w * (P_{bar} + \frac{P_{m(std)}}{13.6})}{T_w}$$

$$V_{m(std)} = Counts_{std} * Y_{sc(avg)}$$

$$Counts_{std} = K_1 \frac{Counts_{raw} * (P_{bar} + \frac{P_{m(std)}}{13.6})}{T_w}$$

$$Q_{u(std)} = \frac{V_{u(std)}}{\Phi}$$


$$Y_w = \frac{V_{u(std)}}{Counts_{std}}$$

$$K_1 = \frac{T_{std}}{P_{std}}$$

$$Y = \frac{V_{u(std)}}{V_{u(std)}}$$


$$Meter \Delta H_{sc} = \frac{P_{m(std)} - 0.001696 * P_{bar} * \frac{T_w}{T_{std}}}{T_w} * \left( \frac{T_{std}}{P_{std}} \right)$$

## Calibration Train

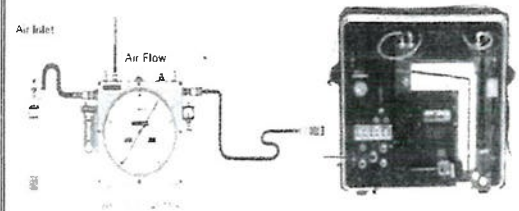

## Calibration Graphs


Meter Pressure vs Flowrate

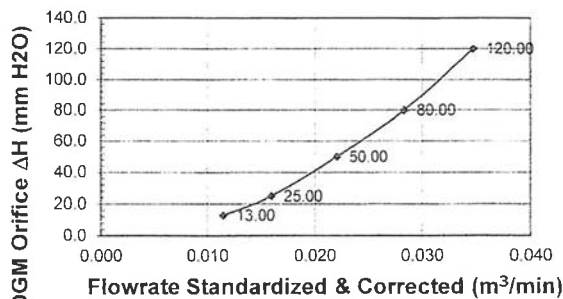

Console Serial: 0504003

Console Model: MC572V

Meter Gamma vs Flowrate

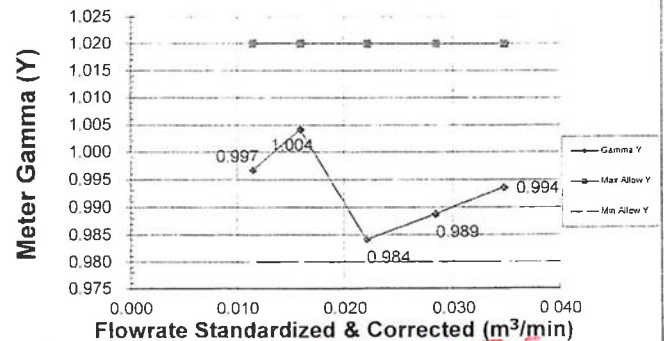

Console Serial: 0504003

Console Model: MC572V

**COPY**

Instrument description : Flue Gas Analyzer  
Instrument model : Testo 350 NEW  
Instrument serial no. : 60378478  
ID no. or control no. : -  
Manufacturer : Testo SE & Co. KGaA  
Probe description : -  
Probe model : -  
Probe serial : -  
Customer name : Eastern Thal Consulting 1992 Company Limited  
Customer address : 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Racha, Chon Buri 20280

Total pages of certificate : 2 Pages  
Receiving no. : L-231787  
Receiving date. : 16-Jun-23  
Parameter of calibration : Gas Calibration(Oxygen 2.498;10.04;21.02 %vol, Carbon Monoxide 80.14,309.9,1003 ppm  
Nitrogen Dioxide 80.96 ppm, Nitric Oxide 151.5 ppm, Sulphur Dioxide 100.8 ppm)

Condition of UUC. : Used  
Ambient condition : All of the Measurement were carried out the stabilized laboratory

Temperature : 23 ±5 °C  
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210

Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration work instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.  
This certificate is applied only to item under test Environmental condition.  
This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory.  
Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.  
This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 20-Jun-23

*Kwanchoi K.*  
Mr. Kwanchai Khamdourng  
Calibration Technician

*D. Witte*  
Mrs. Nongluck Wongsettee  
Technical Manager

COPY

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen ( O2 ) 2.498 % Vol	4219/21	Linde	30-Sep-25
Oxygen ( O2 ) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen ( O2 ) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide ( CO ) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide ( CO ) 309.9 ppm	2803/21	Linde	22-Jun-23
Carbon monoxide ( CO ) 1003 ppm	2583/22	Linde	09-Aug-24
Nitrogen Dioxide ( NO2 ) 80.96 ppm	3240/21	Linde	26-Jun-24
Nitric Oxide ( NO ) 151.5 ppm	0161/23	Linde	22-Jan-25
Sulphur Dioxide ( SO2 ) 100.8 ppm	3507/22	Linde	09-Nov-24

Measured room conditions

Temperature : 22.9 °C Humidity : 65.2 %RH Pressure : 1008.2 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,200 ml/min Gas pressure : 1019.4 mbar

Calibration Results (before adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.498	2.53	0.032	0.15
O2 (%Vol)	10.04	10.08	0.04	0.20
O2 (%Vol)	21.02	21.09	0.07	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	309.9	311	1.1	6.0
CO (ppm)	1003	1005	2	12
*NO2 (ppm)	80.96	72.1	-8.86	8.0
*NO (ppm)	151.5	142	-9.5	8.0
*SO2 (ppm)	100.8	102	1.2	6.0

Calibration Results (after adjustment) (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.498	2.53	0.032	0.15
O2 (%Vol)	10.04	10.08	0.04	0.20
O2 (%Vol)	21.02	21.09	0.07	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	309.9	311	1.1	6.0
CO (ppm)	1003	1005	2	12
*NO2 (ppm)	80.96	81.2	0.24	8.0
*NO (ppm)	151.5	152	0.5	8.0
*SO2 (ppm)	100.8	102	1.2	6.0

Remark : 1 cmol/mol = 1 %vol. , 1 µmol/mol = 1 ppm.

\* Calibrations marked Not TISI Accredited "in this Certificate have been included for completeness."

End of Report

COPY



**Certificate No:** G 660489  
**Date of issue :** 17-Aug-23

**Instrument description :** Flue Gas Analyzer  
**Instrument model :** Testo 350 New  
**Instrument serial no. :** 63455616/0722  
**Control unit serial no. :** 03600177/0722  
**ID no. or control no. :** -  
**Manufacturer :** Testo SE & Co. KGaA  
**Probe description :** -  
**Probe model :** -  
**Probe serial :** -  
**Customer name :** Eastern Thal Consulting 1992 Company Limited  
**Customer address :** 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Racha, Chon Buri 20280

**Total pages of certificate :** 2 Pages  
**Receiving no. :** L-232625  
**Receiving date. :** 10-Aug-23  
**Parameter of calibration :** Gas Calibration(Oxygen 2.498,10.04,21.02,100.8 ppm, Carbon Monoxide 80.14,302,1003 ppm, Nitrogen Dioxide 80.96 ppm, Nitric Oxide 151.5 ppm, Sulphur Dioxide 100.8 ppm)

**Condition of UUC. :** Used  
**Ambient condition :** All of the Measurement were carried out the stabilized laboratory  
**Temperature :** 23 ± 5 °C  
**Humidity :** 55 ± 15 %RH

**Calibration place :** 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210  
**Calibration procedure no.:** This instrument was calibrated by comparison with Standard gas mixture according to calibration work Instration no. WI-CL-28-C

*The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. This certificate is applied only to item under test Environmental condition.*  
*This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.*  
*This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).*

**Date of calibration :** 17-Aug-23

*Kwancheew P.*  
Mr. Kwanchai Khamdung  
Calibration Technician

*Wongsettee*  
Mrs. Nongluck Wongsettee  
Technical Manager

**COPY**



**Certificate No.:** G 660489

**Standard References (Table 1)**

Standard	Certificate No.	Vendor	Due date
Oxygen ( O2 ) 2.498 % Vol	4219/21	Linde	30-Sep-25
Oxygen ( O2 ) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen ( O2 ) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide ( CO ) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide ( CO ) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide ( CO ) 1003 ppm	2583/22	Linde	09-Aug-24
Nitrogen Dioxide ( NO2 ) 80.96 ppm	3240/21	Linde	26-Jun-24
Nitric Oxide ( NO ) 151.5 ppm	0161/23	Linde	22-Jan-25
Sulphur Dioxide ( SO2 ) 100.8 ppm	3507/22	Linde	09-Nov-24

**Measured room conditions**

**Calibration conditions**  
Temperature : 23.8 °C Humidity : 62.1 %RH Pressure : 1008.9 mbar  
Gas Temperature : 24 °C Flow rate : 1,300 ml/min Gas pressure : 1016.8 mbar

**Calibration Results (Without adjustment) (Table 2)**

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.498	2.55	0.052	0.15
O2 (%Vol)	10.04	10.11	0.07	0.20
O2 (%Vol)	21.02	21.14	0.12	0.30
CO (ppm)	80.14	80	-0.14	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1003	999	-4	12
*NO2 (ppm)	80.96	81.5	0.54	8.0
*NO (ppm)	151.5	150	-1.5	8.0
*SO2 (ppm)	100.8	100	-0.8	6.0

**Remark :** 1 cmol/mol = 1 %vol, 1 µmol/mol = 1 ppm.

\* Calibrations marked Not TISI Accredited "in this Certificate have been included for completeness."

**End of Report**

**COPY**

Certificate of Calibration

Customer : Eastern Thai Consulting 1992 Co., Ltd.  
Name : 683 Moo 11, Sukhapibam 8 Rd., Nongkham, Srirachai, Chonburi  
Address : 20230

Certificate No : 24-AFM-023

Request No : Req-2024-0095

Unit Under Calibration Details

Measurement Item : Primary Flow Calibrator  
Manufacturer : Bios  
Model : Defender 510-L  
Serial Number : 110619  
ID : -  
Sensor Model : -  
Sensor Serial Number : -

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 0.3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 11 January 2024  
Calibration Date : 30 January 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU651882	TPA	9 November 2024


Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By :   
Mr. Noppidon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Paet Mathavorn  
Calibration Engineer Supervisor

Issue Date : 30 January 2024



The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.01 Issue date 25/01/24

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)
24.80	101.23	0	0.00	0.0000	0.0058
24.40	101.18	50	49.629	-0.4	3.3
24.40	101.16	100	100.73	0.7	2.8
24.30	101.13	200	198.30	-1.7	5.6
24.30	101.10	300	298.14	-1.9	8.4
24.40	101.06	400	397.45	-3	11
24.20	101.00	500	496.93	-3.1	7.1

Note : STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P} \times \frac{T_{meas}}{T_{ref}}$$

where Q : Flow Rate

P : Absolute Pressure

T : Absolute Temperature

Meas = Measurement Condition

ref = Standard Condition

\* Indicates non accredited

End of Certificate



The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.01 Issue date 25/01/24

Page 2/2

Page 1/2

Certificate of Calibration

Customer

Name

Address

Certificate No : 24-AFM-022

Request No : Req-2024-0094

683 Mon 11, Sukhapibam 8 Rd., Nongkham, Srinacha, Chonburi

Unit Under Calibration Details

Measurement Item

Manufacturer

Model

Serial Number

ID

Primary Flow Calibrator

MesaLabs

Defender 510-M

207510

-

Sensor Model : -

Sensor Serial Number : -

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature

Humidity

Barometric Pressure

Received Date

Calibration Date

23 °C ± 3 °C

55 %RH ± 20 %RH

1013 hPa ± 10 hPa

11 January 2024

30 January 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000037	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A21/A Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.

Calibration By : Mr. Noppadom Luangart

Service Calibration Engineer

Approved By : Mr. Pait Mathavom

Calibration Engineer Supervisor

Issue Date : 30 January 2024

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)
24.80	101.23	0	0.00	0.0000	0.0058
24.70	101.58	101	101.48	0.5	2.8
24.80	101.50	200	201.14	1.1	5.6
24.70	101.50	500	503.87	3.9	7.1
24.80	101.50	1003	1010.1	7	14
24.70	101.60	2002	2014.6	13	29
24.60	101.33	2995	3007.6	13	43
24.60	101.65	4027	4007.5	-19	57
24.50	101.70	5035	5010.7	-24	72

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where

Q Flow Rate

P = Absolute Pressure

T = Absolute Temperature

Meas = Measurement Condition

ref Standard Condition

\* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev 01 Issue date 25/01/24

COPY



## Calibration Certificate

Equipment : SOUND CALIBRATOR

Manufacturer : RION

Model : NC-75

Serial No.: 34802645

ID No.:

Condition As Found :

GOOD

Customer :

EASTERN THAI CONSULTING 1992 CO., LTD.  
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,  
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :

Ambient Temperature : ( 23.0 ± 3 ) °C

Pressure : ( 101.3 ± 3 ) kPa

Relative Humidity : ( 50.0 ± 20 ) %

Received Date :

06 SEPTEMBER 2023

Calibration Date :

12 OCTOBER 2023

Date of Issue :

16 OCTOBER 2023

Calibrated by :

Nathakorn Pisutpaisan

Approved by :

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

**COPY**

Calibration Procedure : CP-AC-03

### Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

### Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

**COPY**

*T. Petchurai*

Continuation of Calibration Certificate

Cert. No. : ACC23037  
Job No. : VC66AC0097  
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	93.94	-0.06	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.24	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

7. Retain



## Calibration Certificate

### Equipment :

### Manufacturer :

### Model :

### Serial No.:

### ID No.:

SOUND LEVEL METER

RION

NL-21/ Microphone UC-52 / Preamplifier NH-21

00310455 / 157154 / 54250

### Condition As Found :

GOOD

### Customer :

EASTERN THAI CONSULTING 1992 CO., LTD.

SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,

NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

### Location :

### Ambient Temperature :

### Pressure :

### Relative Humidity :

( 23.0 ± 3 ) °C

( 101.3 ± 3 ) kPa

( 50.0 ± 20 ) %

### Received Date :

06 SEPTEMBER 2023

### Calibration Date :

10-12 OCTOBER 2023

### Date of Issue :

16 OCTOBER 2023

### Calibrated by :

Nathakorn Pisutpraisan

### Approved by :

( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

COPY

7. Petchurai

### Calibration Procedure :

CP-AC-02

### Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with A-weighting chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-4010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EELBP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EELBP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EELBP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL23303  
Job No. : VC66AC0097  
Pages : 3 of 9

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement

COPY

7. Reten.

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB )	Measured Value (dB )	Deviation (-dB <sub>r</sub> )	Acceptance Limit (dB )
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB )
22.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB )
A - weight	21.9
C - weight	22.8
Flat	26.1

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz )	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.1	0.2	0.2
1000	-0.2	-0.2	-0.2
8000	-2.0	-1.7	-1.8

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23303  
Job No. : VC66AC0097  
Pages : 5 of 9

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	-0.2	-0.1	±2.0
125	-0.1	-0.1	±1.5
250	-0.1	-0.1	±1.5
500	0.0	0.0	±1.5
1000	0.0	0.0	±1.0
2000	0.1	0.1	±2.0
4000	0.1	0.1	±3.0
8000	0.0	0.2	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A-weight	94.0	94.0	0.0	±0.2
C-weight	94.0	94.0	0.0	±0.2
Flat	94.0	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	±0.1
Slow	94.0	94.0	0.0	±0.1
Leq	94.0	94.0	0.0	±0.1

6. Long-term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A-weight	94.0	94.0	0.0	±0.3

Continuation of Calibration Certificate

Cert. No. : ACL23303  
Job No. : VC66AC0097  
Pages : 6 of 9

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
135.0	135.0	0.0	±1.1
134.0	134.0	0.0	±1.1
133.0	132.9	-0.1	±1.1
132.0	131.9	-0.1	±1.1
131.0	130.9	-0.1	±1.1
129.0	128.9	-0.1	±1.1
124.0	123.9	-0.1	±1.1
119.0	118.9	-0.1	±1.1
114.0	113.9	-0.1	±1.1
109.0	108.9	-0.1	±1.1
104.0	103.9	-0.1	±1.1
99.0	99.0	0.0	±1.1
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	39.0	0.0	±1.1

COPY

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23303  
Job No. : VC66AC0097  
Pages : 7 of 9

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	$\pm 0.5$
120	94.0	94.0	0.0	$\pm 0.5$
110	94.0	94.0	0.0	$\pm 0.5$
100	94.0	94.0	0.0	$\pm 0.5$
90	94.0	94.0	0.0	$\pm 0.5$

Level linearity on each level range

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	43.0	43.0	0.0	$\pm 0.5$
120	33.0	33.0	0.0	$\pm 0.5$

9. Tone burst response

Time Weighing	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	$\pm 1.0$
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	$\pm 1.0$
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	$\pm 1.0$

Continuation of Calibration Certificate

Cert. No. : ACL23303  
Job No. : VC66AC0097  
Pages : 8 of 9

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lepeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	$\pm 3.0$
One	136.4	135.9	-0.5	$\pm 3.0$

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	$\pm 2.0$
Positive half cycle	135.4	135.2	-0.2	$\pm 2.0$
Negative half cycle	135.4	135.2	-0.2	$\pm 2.0$

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	-0.2	$\pm 1.5$
89.4	89.2		

Continuation of Calibration Certificate

Cert No. : ACL23303  
Job No. : VC66AC0097  
Pages : 9 of 9

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

7. Retel

## Certificate of Calibration

Certificate No.: S2402-0651-01

**Customer:**

Eastern Thai Consulting 1992 Co., Ltd.  
683 Moo 11, Sukhapibam 8 Rd,  
Nongkham, Sriracha, Chonburi 20230

**Date of calibration:**

2024-03-04  
2024-03-26

**Date of issue:**

2024-03-26

**Instrument Calibrated:**

Sound Level Meter

**Manufacturer:**

Rion

**Model:**

NL-42A (Meter), UC-59 (Microphone), NH-25 (Preamplifier)

**Serial no:**

00322755 (Meter), 21960 (Microphone), 22336 (Preamplifier)

**Calibration and verification performed:**

Acoustical levels are stated relative to 20µPa. Other dB levels are relative values.  
The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which with the reported effective degree of freedom corresponds to coverage probability of approximately 95%.  
The sound level meter instrument submitted for periodic testing following the periodic tests of IEC 61672-3 : 2013.

**Preconditioning:**

The equipment was preconditioned for more than 16 hours at the specified calibration temperature and humidity.

**Instruments and Program:**

A complete list of instruments, hardware, and software, that has been used for this calibration is separately available from the calibration laboratory.

**Equipment standards used:**

- Sound measuring equipment calibration unit 483B S/N31083
- Digital multimeter Keysight S/N HP34401A
- Ultra-low distortion function generator Stanford SRS DS360 S/N123625
- Acoustic sound calibrator class 1 Nor1256 S/N125626542
- Combined Pressure, Humidity and Temperature Transmitter PTU300 S/NM2520568

**Traceability**

The measured values are traceable to following the ISO/IEC 17025 laboratories:

Sound Pressure Level: EEI, Thailand  
Reference Pressure, Humidity and Temperature: TPA, Thailand  
Voltage: TPA, Thailand  
Frequency: TPA, Thailand

This certificate of calibration is issued by Acoustic Laboratory Thailand (ALT). It also states that the laboratory has a satisfactory quality assurance system and traceability to accredited or national calibration laboratories. This certificate may not be reproduced other than in full

Certificate No.: S2402-0651-01

**Environmental conditions:**

Pressure:

101.325 kPa

Temperature:

23.0 °C

Relative humidity:

50 %RH

**Reference conditions:**

100.87 ± 0.10 kPa

23.5 ± 1.0 °C

57.0 ± 2.0 %RH

**Measurement conditions:**

**1. Indication at the calibration check frequency**

Reference Acoustic Signal (dB)	Measured value (dB)		Deviated value (dB)	Acceptance limit (dB)
	Before adjust	After adjust		
93.9	93.9	93.9	0.0	±1.0

Note: Indication at the checked calibration frequency was adjusted to 93.9 dB by the sound calibrator Type NC-75 S/N: 34234715

**2. Self-generated noise**

Frequency weightings		Measured value (dB)
A-Weighting		10.8
C-Weighting		15.3
Z-Weighting		20.7

**3. Electrical signal test of frequency weighting at 91 dB**

Frequency (Hz)	Deviation from various frequency weighting response curve			
	A-Weighting (dB)	C-Weighting (dB)	Z-Weighting (dB)	Acceptance limit (dB)
63	0.0	0.0	0.0	±2.0
125	0.1	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.1	0.1	0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	-0.1	-0.1	-0.2	±2.0
4000	-0.3	-0.3	-0.3	±3.0
8000	0.1	0.1	0.0	±5.0

Date of calibration : 2024-03-04

2024-03-26

Date of issue : 2024-03-26

4. Frequency and time weighting at 1 kHz

4.1 Frequency weighting at 1 kHz

Frequency weightings	Measured value (dB)	Deviated value (dB)	Acceptance limit (dB)
A	94.0	0.0	±0.3
C	94.0	0.0	±0.3
Z	94.0	0.0	±0.3

4.2 Time weighting at 1 kHz

Time weightings	Measured value (dB)	Deviated value (dB)	Acceptance limit (dB)
Fast	94.0	0.0	±0.3
Slow	94.0	0.0	±0.3
LAeq	94.0	0.0	±0.3

5. Long term stability

Time interval (mm:ss)	Start level (dB)	Stop level (dB)	Deviated value (dB)	Acceptance limit (dB)
28:58	94.0	94.0	0.0	±0.3

Date of calibration : 2024-03-04

2024-03-26

Date of issue : 2024-03-26

**COPY**

6. Level linearity on the reference level range

6.1 Measured at 31.5 Hz

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit (dB)
84.0	84.0	0.0	±1.1
89.0	89.0	0.0	±1.1
92.6	92.6	0.0	±1.1
93.6	93.6	0.0	±1.1
94.6	94.6	0.0	±1.1
95.6	95.6	0.0	±1.1
96.6	96.6	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.1	0.1	±1.1
40.0	39.9	-0.1	±1.1
39.0	38.9	-0.1	±1.1
38.0	38.0	0.0	±1.1
37.0	37.0	0.0	±1.1
36.0	36.0	0.0	±1.1

Date of calibration : 2024-03-04

2024-03-26

Date of issue : 2024-03-26

**COPY**

6.2 Measured at 1 kHz

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
132.0	132.0	0.0	±1.1
133.0	133.0	0.0	±1.1
134.0	134.0	0.0	±1.1
135.0	135.0	0.0	±1.1
136.0	136.0	0.0	±1.1
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
40.0	40.0	0.0	±1.1
39.0	38.9	-0.1	±1.1
38.0	38.0	0.0	±1.1
37.0	36.9	-0.1	±1.1
36.0	35.9	-0.1	±1.1

Date of calibration : 2024-03-04  
2024-03-26  
Date of issue : 2024-03-26

COPY

6.3 Measured at 8 kHz

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
130.9	130.9	0.0	±1.1
131.9	131.9	0.0	±1.1
132.9	132.8	-0.1	±1.1
133.9	133.9	0.0	±1.1
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	78.9	-0.1	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	63.9	-0.1	±1.1
59.0	59.0	0.0	±1.1
54.0	53.9	-0.1	±1.1
49.0	48.9	-0.1	±1.1
44.0	43.9	-0.1	±1.1
40.0	39.9	-0.1	±1.1
39.0	38.9	-0.1	±1.1
38.0	37.9	-0.1	±1.1
37.0	36.9	-0.1	±1.1
36.0	35.9	-0.1	±1.1

Date of calibration : 2024-03-04  
2024-03-26  
Date of issue : 2024-03-26

COPY

7. Tone burst response

Time weightings	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit (dB)
Fast	200	133.0	0.0	±1.0
	2	116.0	0.0	+1.0,-2.5
	0.25	107.0	0.0	+1.5,-5.0
Slow	200	126.6	0.0	±1.0
	2	107.0	0.0	+1.0,-5.0
	200	127.0	0.0	±1.0
SEL	2	107.0	0.0	+1.0,-2.5
	0.25	97.9	-0.1	+1.5,-5.0

8. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit (dB)
Complete cycle	128.4	127.4	-1.0	±3.0
Positive half cycle	130.4	130.1	-0.3	±2.0
Negative half cycle	130.4	130.1	-0.3	±2.0

9. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit (dB)
Positive one half cycle	Negative one half cycle		
139.1	138.9	0.2	±1.5

10. High level stability

Initial level (dB)	Final level (dB)	Deviated value (dB)	Acceptance limit (dB)
135.0	135.0	0.0	±0.3

Date of calibration : 2024-03-04  
2024-03-26  
Date of issue : 2024-03-26

COPY

Uncertainty of measurement

Parameters	Uncertainty
1. Indication at the calibration check frequency	0.12 dB
2. Self-generated noise	
- Frequency Weighting A	0.090 dB
- Frequency Weighting C	0.13 dB
- Frequency Weighting Z	0.090 dB
3. Electrical signal test of frequency weighting	0.13 dB
4. Frequency and time weightings at 1 kHz	0.13 dB
5. Long term stability test	0.10 dB
6. Level linearity on the reference level range	0.14 dB
7. Tone burst response	0.13 dB
8. Peak C sound level	0.13 dB
9. Overload indication	0.13 dB
10. High level stability test	0.10 dB

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

Remark : The acoustical signal test of frequency weighting at 125Hz, 1kHz, and 8kHz is not included, along with correction values for environmental conditions in a free-field or diffuse field, and the effect of reflection and diffraction on the measurement microphone and the sound level meter.

Replacement Calibration Certificate for calibration certificate number S2402-0651

Calibrated By: *Althakon* Approved By: *Mr. Pitupong Sarapho*  
(Mr. Athakorn Sumpphan) (Mr. Pitupong Sarapho)

Date of calibration : 2024-03-04  
2024-03-26  
Date of issue : 2024-03-26

----- End of Certificate of Calibration -----

COPY

# SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Siinthon Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel:0-2435-8800 Fax:0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

Cert. No. : ACL23241  
Pages : 1 of 9

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-21 / Microphone UC-52 / Preamplifier NH-21  
**Serial No.:** 00310456 / 153489 / 34625  
**ID No.:**

**Condition As Found :** GOOD

**Customer :** EASTERN THAI CONSULTING 1992 CO., LTD.  
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,  
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

**Location :**  
**Ambient Temperature :** ( 23.0 ± 3 ) °C  
**Pressure :** ( 101.3 ± 3 ) kPa  
**Relative Humidity :** ( 50.0 ± 20 ) %

**Received Date :** 28 JUNE 2023  
**Calibration Date :** 24-26 JULY 2023  
**Date of Issue :** 02 AUGUST 2023

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**  
  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

**COPY**

# SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

## Continuation of Calibration Certificate

Cert. No. : ACL23241  
Job No. : VC66AC0069  
Pages : 2 of 9

**Calibration Procedure :** CP-AC-02

### Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :


1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAJ	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.  
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

**COPY**



Continuation of Calibration Certificate

Cert. No. : ACL23241  
Job No. : VC66AC0069  
Pages : 3 of 9

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY

7. Peter

Continuation of Calibration Certificate

Cert. No. : ACL23241  
Job No. : VC66AC0069  
Pages : 4 of 9

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
22.5

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	21.7
C - weight	22.4
Flat	25.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
125	0.2	0.2	± 1.5
1000	0.0	0.0	± 1.0
8000	-0.8	-0.7	±5.0

COPY

7. Peter

## Continuation of Calibration Certificate

Cert. No. : ACL23241  
Job No. : VC66AC0069  
Pages : 5 of 9Cert. No. : ACL23241  
Job No. : VC66AC0069  
Pages : 6 of 9

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	-0.2	-0.1	-0.1
125	-0.1	-0.1	-0.1
250	-0.1	-0.1	-0.1
500	-0.1	0.0	-0.1
1000	0.0	0.0	0.0
2000	0.1	0.1	0.0
4000	0.1	0.1	0.0
8000	0.1	0.2	0.2

## 5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	$\pm 0.2$
C - weight	94.0	94.0	0.0	$\pm 0.2$
Flat	94.0	94.0	0.0	$\pm 0.2$

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	$\pm 0.1$
Slow	94.0	94.0	0.0	$\pm 0.1$
Leq	94.0	94.0	0.0	$\pm 0.1$

## 6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	$\pm 0.3$

## 7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
134.0	133.9	-0.1	$\pm 1.1$
133.0	132.9	-0.1	$\pm 1.1$
132.0	131.9	-0.1	$\pm 1.1$
131.0	130.9	-0.1	$\pm 1.1$
129.0	128.9	-0.1	$\pm 1.1$
124.0	123.9	-0.1	$\pm 1.1$
119.0	118.9	-0.1	$\pm 1.1$
114.0	113.9	-0.1	$\pm 1.1$
109.0	108.9	-0.1	$\pm 1.1$
104.0	103.9	-0.1	$\pm 1.1$
99.0	98.9	-0.1	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	43.9	-0.1	$\pm 1.1$
39.0	38.7	-0.3	$\pm 1.1$

Continuation of Calibration Certificate

Cert. No. : ACL23241  
Job No. : VC66AC0069  
Pages : 7 of 9

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.5
120	94.0	94.0	0.0	±0.5
110	94.0	94.0	0.0	±0.5
100	94.0	94.0	0.0	±0.5
90	94.0	94.1	0.1	±0.5

Level linearity on each level range

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	43.0	42.8	-0.2	±0.5
120	33.0	33.0	0.0	±0.5

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Continuation of Calibration Certificate

Cert. No. : ACL23241  
Job No. : VC66AC0069  
Pages : 8 of 9

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lopeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	-0.1	±1.5
89.3	89.2		

COPY

F. Retin

COPY

F. Retin

Continuation of Calibration Certificate

Cert. No. : ACL23241  
Job No. : VC66AC0069  
Pages : 9 of 9

12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

\_\_\_\_\_ End of Calibration Certificate \_\_\_\_\_

COPY

7. Belen



## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42A / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00322754 / 196477 / 15486  
**ID No.:** -

**Condition As Found :** GOOD  
**Customer :** EASTERN THAI CONSULTING 1992 CO., LTD.  
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,  
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0 ± 3 ) °C  
**Pressure :** ( 101.3 ± 3 ) kPa  
**Relative Humidity :** ( 50.0 ± 20 ) %

**Received Date :** 02 MAY 2023  
**Calibration Date :** 02 -04 MAY 2023  
**Date of Issue :** 05 MAY 2023

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**   
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

**COPY**

## Continuation of Calibration Certificate

**Calibration Procedure :** CP-AC-01

### Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.  
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL23143  
Job No. : VC66AC0047  
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

**COPY**

Continuation of Calibration Certificate

Cert. No. : ACL23143  
Job No. : VC66AC0047  
Pages : 4 of 8

Result of calibration :

**1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise**

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	16.3
Flat	22.2

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.0	0.0	0.0
8000	0.0	0.1	0.1
			Acceptance Limits
			±1.5
			±1.0
			±5.0

**COPY**

Continuation of Calibration Certificate

Cert. No. : ACL23143  
Job No. : VC66AC0047  
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	-0.1	-0.1	±2.0
125	0.0	0.0	±1.5
250	0.0	0.0	±1.5
500	0.0	-0.1	±1.5
1000	0.0	-0.1	±1.5
2000	0.0	0.0	±1.0
4000	0.0	0.0	±2.0
8000	0.0	0.0	±3.0
	0.0	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL23143  
Job No. : VC66AC0047  
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.1	0.1	± 1.1
69.0	69.1	0.1	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.1	0.1	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	24.9	-0.1	± 1.1

Continuation of Calibration Certificate

Cert No. : ACL23143  
Job No. : VC66AC0047  
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lcpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert No. : ACL23143  
Job No. : VC66AC0047  
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	-0.3	±1.5
89.8	89.5		

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

COPY



## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42A/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00322746 / 196469 / 15478  
**ID No.:**

**Condition As Found :** GOOD  
**Customer :** EASTERN THAI CONSULTING 1992 CO., LTD.  
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,  
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

**Location :**  
**Ambient Temperature :** ( 23.0 ± 3 ) °C  
**Pressure :** ( 101.3 ± 3 ) kPa  
**Relative Humidity :** ( 50.0 ± 20 ) %

**Received Date :** 11 JUNE 2023  
**Calibration Date :** 24 -25 JULY 2023  
**Date of Issue :** 02 AUGUST 2023

**Calibrated by :** Nathakorn Pisutpaian

**Approved by :**  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

**Calibration Procedure :** CP-AC-01

### Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.  
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

7. Petch.

Continuation of Calibration Certificate

Cert. No. : ACL23245  
Job No. : VC66AC0069  
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.3
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23245  
Job No. : VC66AC0069  
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.6
C - weight	18.9
Flat	24.3

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.4	0.4	0.4
1000	0.0	0.0	0.0
8000	0.4	0.5	0.5

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23245  
Job No. : VC66AC0069  
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	-0.1	-0.1	±2.0
125	0.0	0.0	±1.5
250	0.0	0.0	±1.5
500	0.0	0.0	±1.5
1000	0.0	0.0	±1.0
2000	0.0	0.0	±2.0
4000	0.0	0.0	±3.0
8000	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
------------------------	-------------------------------------	-----------------------------------	-----------------------------	--------------------------------

Continuation of Calibration Certificate

Cert. No. : ACL23245  
Job No. : VC66AC0069  
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.1	0.1	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.1	0.1	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

## Continuation of Calibration Certificate

Cert. No. : ACL23245  
Job No. : VC66AC0069  
Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L <sub>peak</sub> (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.5	-0.9	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

## Continuation of Calibration Certificate

Cert. No. : ACL23245  
Job No. : VC66AC0069  
Pages : 8 of 8

## 11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	0.1	±1.5
89.5	89.6		

## 12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate