

ภาคผนวก ณ

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.  
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Noise	Leq 24 hrs	Sound Calibrator	BKK_FS1221	19-Dec-23	18-Dec-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0101	29-May-23	29-May-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0994	19-Oct-23	19-Oct-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0995	16-Oct-23	16-Oct-24	12
Noise	Leq 24 hrs	Sound Calibrator	BKK_FS0618	19-Dec-23	18-Dec-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0875	10-Jan-24	9-Jan-25	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0876	11-Dec-23	10-Dec-24	12
Noise	Leq 24 hrs	Sound Level Meter	BKK_FS0877	1-Nov-23	1-Nov-24	12
Water Lab	pH at 25 °C	pH meter	BKK_EN0342	27-Oct-23	27-Oct-24	12
Water Lab	Total Alkalinity	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Total Hardness	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Color	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Turbidity	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Dissolved Oxygen	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Dissolved Oxygen	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Nitrate	Ion Chromatography	BKK_EN0069	12-Jan-24	12-Jan-25	12
Water Lab	Phosphate	Ion Chromatography	BKK_EN0069	12-Jan-24	12-Jan-25	12
Water Lab	Chloride	Ion Chromatography	BKK_EN0069	12-Jan-24	12-Jan-25	12
Water Lab	Sulfate	Ion Chromatography	BKK_EN0069	12-Jan-24	12-Jan-25	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0425	6-Nov-23	6-Nov-24	12
Water Lab	Total Solids	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Total Solids	Oven	BKK_EN0425	6-Nov-23	6-Nov-24	12
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0425	6-Nov-23	6-Nov-24	12
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0366	21-Apr-24	21-Apr-25	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	12-Jul-23	12-Jul-24	12
Water Lab	Conductivity	Conductivity meter	BKK_EN0373	25-Dec-23	25-Dec-24	12
Water Lab	Salinity	Conductivity meter	BKK_EN0373	25-Dec-23	25-Dec-24	12
Water Lab	BOD	DO Meter	BKK_EN0017	16-Nov-23	16-May-25	18
Water Lab	BOD	Incubator	BKK_EN0304	20-Mar-24	20-Mar-25	12
Water Lab	BOD	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	COD	Hot Block	BKK_EN0370	6-Dec-23	6-Dec-24	12
Water Lab	COD	Spectrophotometer	BKK_EN0018	15-Sep-23	15-Sep-24	12
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0148	4-Jul-23	4-Jan-25	18
Water Lab	Temperature	Digital Thermometer With Sensor	BKK_LG0055	24-Aug-23	24-Aug-24	12
Water Lab	Temperature	Digital Thermometer With Sensor	BKK_LG0064	12-Sep-23	12-Sep-24	12
Water Lab	Hexavalent Chromium	Spectrophotometer	BKK_EN0018	15-Sep-23	15-Sep-24	12
Water Lab	Iron	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Iron	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Iron	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Lead	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Lead	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Lead	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Manganese	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Manganese	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Manganese	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Calcium	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	18
Water Lab	Calcium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Calcium	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Magnesium	ICP-OES	BKK_EL0037	20-Mar-23	19-Sep-24	18
Water Lab	Magnesium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Magnesium	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Copper	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Copper	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Copper	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Cadmium	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Cadmium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Cadmium	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18

1

alsglobal.com



right solutions.  
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	Zinc	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Zinc	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Zinc	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Nickel	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Nickel	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Nickel	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Selenium	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Selenium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Selenium	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Barium	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Barium	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Barium	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Arsenic	ICP-MS	BKK_EL0043	6-Apr-23	6-Oct-24	18
Water Lab	Arsenic	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Water Lab	Arsenic	Chamber (Cold Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Mercury	Mercury Analyzer	BKK_EL0128	6-Dec-23	6-Dec-24	12
Water Lab	Total Coliform	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	23-Apr-24	23-Oct-25	18
Water Lab	Fecal Coliform	Autoclave	BKK_ML0037	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Fecal Coliform	Hot Air Oven	BKK_ML0013	23-Apr-24	23-Oct-25	18
Water Lab	Fecal Coliform	Water Bath	BKK_ML0056	1-Mar-24	1-Mar-25	12

2

alsglobal.com

## SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthon Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

Cert. No. : ACC23048  
Pages : 1 of 3

### Calibration Certificate

**Equipment :** SOUND CALIBRATOR  
**Manufacturer :** RION  
**Model :** NC-75  
**Serial No.:** 35024431  
**ID No.:** BKK\_FS1221

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :**  
**Ambient Temperature :** ( 23.0 ± 3 ) °C  
**Pressure :** ( 101.3 ± 3 ) kPa  
**Relative Humidity :** ( 50.0 ± 20 ) %

**Received Date :** 28 NOVEMBER 2023  
**Calibration Date :** 19 DECEMBER 2023  
**Date of Issue :** 22 DECEMBER 2023

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**   
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QP-TS12-04-04-020664

## SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

### Continuation of Calibration Certificate

**Cert. No. :** ACC23048  
**Job No. :** VC67AC0035  
**Pages :** 2 of 3

**Calibration Procedure :** CP-AC-03

#### Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

#### Condition of this result of calibration :

##### 1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KA1	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QP-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACC23048  
Job No. : VC67AC0035  
Pages : 3 of 3

**Result of calibration :**

**1. Sound pressure level**

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	93.96	-0.04	0.14	0.40

**2. Frequency**

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ( % )	Uncertainty ( % )	Acceptance limit ( % )
1000	1000.0	0.0	0.1	1.0

**3. Total distortion**

Measured value ( % )	Uncertainty ( % )	Acceptance limit ( % )
0.35	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

*T. Petchur*



451-451/1 Sirinthorn Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com

Cert. No. : ACL23173  
Pages : 1 of 8

**Calibration Certificate**

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00658244 / 158766 / 58768  
**ID No.:** BKK\_TS0101

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0 ± 3 ) °C  
**Pressure :** ( 101.3 ± 3 ) kPa  
**Relative Humidity :** ( 50.0 ± 20 ) %

**Received Date :** 29 MAY 2023  
**Calibration Date :** 29-30 MAY 2023  
**Date of Issue :** 31 MAY 2023

REVIEW BY *Nathakorn P*  
APPROVED BY *T. Petchur*  
NEXT CAL. DATE *29/5/24*

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*T. Petchur*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23173  
Job No. : VC66AC0060  
Pages : 2 of 8

**Calibration Procedure :** CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.  
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

**1. Reference Standard Instruments :**

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

*T. Petchur*

Continuation of Calibration Certificate

Cert. No. : ACL23173  
Job No. : VC66AC0060  
Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C' sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

QF-TS12-04-04-020664

*T. Petchur*



## Continuation of Calibration Certificate

Cert. No. : ACL23173  
Job No. : VC66AC0060  
Pages : 4 of 8

## Result of calibration :

## 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

## 2. Self-generated noise

## 2.1 Normal test

Measured Value ( dB )
16.8

## 2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.3
Flat	24.2

## 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.4	-0.3	-0.3	±5.0

QF-TS12-04-04-020664

7. Petch.

## Continuation of Calibration Certificate

Cert. No. : ACL23173  
Job No. : VC66AC0060  
Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

7. Petch.

## Continuation of Calibration Certificate

Cert. No. : ACL23173  
Job No. : VC66AC0060  
Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

QF-TS12-04-04-020664

7. Petch.

## Continuation of Calibration Certificate

Cert. No. : ACL23173  
Job No. : VC66AC0060  
Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.7	-0.7	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

7. Petch.



Continuation of Calibration Certificate

Cert. No. : ACL23173  
Job No. : VC66AC0060  
Pages : 8 of 8

11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchur

451-451/1 Sirinthorn Rd., Bangbunru, Banglud Bangkok 10700 THAILAND.  
Tel:0-2435-8800 Fax:0-2433-1679 e-mail:center@sithiporn.com http://www.sithiporn.com

Cert. No. : ACL23319  
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RION  
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24  
Serial No.: 00597156 / 170403 / 72904  
ID No.: BKK\_FS0994

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

Location : -  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 11 OCTOBER 2023  
Calibration Date : 19-20 OCTOBER 2023  
Date of Issue : 24 OCTOBER 2023



Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23319  
Job No. : VC67AC0011  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL_BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL_BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL_BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KA1	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL23319  
Job No. : VC67AC0011  
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

QF-TS12-04-04-020664

T. Petchur



## Continuation of Calibration Certificate

Cert. No. : ACL23319  
Job No. : VC67AC0011  
Pages : 4 of 8

## Result of calibration :

## 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

## 2. Self-generated noise

## 2.1 Normal test

Measured Value ( dB )
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	9.9
C - weight	16.0
Flat	21.9

## 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.5	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-1.6	-1.5	-1.5	±5.0

QF-TS12-04-04-020664

T. P. P.

## Continuation of Calibration Certificate

Cert. No. : ACL23319  
Job No. : VC67AC0011  
Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long-term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

T. P. P.

## Continuation of Calibration Certificate

Cert. No. : ACL23319  
Job No. : VC67AC0011  
Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

QF-TS12-04-04-020664

T. P. P.

## Continuation of Calibration Certificate

Cert. No. : ACL23319  
Job No. : VC67AC0011  
Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.5	-0.9	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

T. P. P.



## Continuation of Calibration Certificate

Cert. No. : ACL23319  
Job No. : VC67AC0011  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated	Acceptance
Positive	Negative	Value	Limits
one-half cycle	one-half cycle	( dB )	( dB )
89.7	89.7	0.0	±1.5

## 12. High level stability

Frequency	SLM Display	SLM Display	Deviated	Acceptance
Weighting	at initial	at final	Value	Limits
	( dB )	( dB )	( dB )	( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchurai

451-451/1 Srinthom Rd., Bangbunru, Banglud Bangkok 10700 THAILAND  
Tel:0-2435-8800 Fax:0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.comCert. No. : ACL23310  
Pages : 1 of 8

## Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RION  
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24  
Serial No. : 00597159 / 180402 / 88172  
ID No. : BKK\_FS0995

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

Location :  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 22 SEPTEMBER 2023  
Calibration Date : 16-18 OCTOBER 2023  
Date of Issue : 19 OCTOBER 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced  
other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

## Continuation of Calibration Certificate

Cert. No. : ACL23310  
Job No. : VC66AC0101  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference  
Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

T. Petchurai

## Continuation of Calibration Certificate

Cert. No. : ACL23310  
Job No. : VC66AC0101  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

QF-TS12-04-04-020664

T. Petchurai



Continuation of Calibration Certificate

Cert. No. : ACL23310  
Job No. : VC66AC0101  
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value ( dB )
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.6
C - weight	18.4
Flat	24.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.0	0.0	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	2.5	2.5	2.5	±5.0

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23310  
Job No. : VC66AC0101  
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.2	-0.1	±2.0
125	-0.1	0.0	-0.1	±1.5
250	-0.1	0.0	-0.1	±1.5
500	-0.1	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23310  
Job No. : VC66AC0101  
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	± 1.1
136.0	136.1	0.1	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.1	0.1	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.1	0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23310  
Job No. : VC66AC0101  
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

QF-TS12-04-04-020664

T. Petch



## Continuation of Calibration Certificate

Cert. No. : ACL23310  
Job No. : VC66AC0101  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchum

451-451/1 Sirinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.comCert. No. : ACC23046  
Pages : 1 of 3

## Calibration Certificate

Equipment : SOUND CALIBRATOR  
Manufacturer : RION  
Model : NC-74  
Serial No. : 34425567  
ID No. : BKK\_FS0618

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.Location :  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %Received Date : 28 NOVEMBER 2023  
Calibration Date : 19 DECEMBER 2023  
Date of Issue : 22 DECEMBER 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchum  
( Thanakul Petchum )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced  
other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

## Continuation of Calibration Certificate

Cert. No. : ACC23046  
Job No. : VC67AC0035  
Pages : 2 of 3

Calibration Procedure : CP-AC-03

## Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference  
microphone.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

T. Petchum

## Continuation of Calibration Certificate

Cert. No. : ACC23046  
Job No. : VC67AC0035  
Pages : 3 of 3

## Result of calibration :

## 1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.03	0.03	0.14	0.40

## 2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ( % )	Uncertainty ( % )	Acceptance limit ( % )
1000	1004.3	0.4	0.1	1.0

## 3. Total distortion

Measured value ( % )	Uncertainty ( % )	Acceptance limit ( % )
1.86	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchum

Cert. No. : ACL24017  
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RION  
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24  
Serial No. : 00572566 / 142140 / 22309  
ID No. : BKK\_FS0875

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

Location :  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 22 DECEMBER 2023  
Calibration Date : 10-11 JANUARY 2024  
Date of Issue : 12 JANUARY 2024

Calibrated by : Nathakorn Pisutpaisam

Approved by : *T. Petchur*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced  
other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL24017  
Job No. : VC67AC0045  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :  
This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference  
Standard Instruments.  
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL_BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL_BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL_BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.  
3. This certificate is traceable to the international system of unit maintained at :  
3.1 National Institute of Metrology (Thailand).  
3.2 Thailand Institute of Scientific and Technological Research (TISTR).

*T. Petchur*

Cert. No. : ACL24017  
Job No. : VC67AC0045  
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

*T. Petchur*

Cert. No. : ACL24017  
Job No. : VC67AC0045  
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value ( dB )
16.3

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	13.8
C - weight	19.9
Flat	25.8

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.2	-0.2	-0.2	± 5.0

*T. Petchur*



**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**

**5.1 Frequency weightings at 1 kHz**

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	±0.2
C - weight	94.0	94.0	0.0	±0.2
Flat	94.0	94.0	0.0	±0.2

**5.2 Time weighting at 1 kHz**

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	±0.1
Slow	94.0	94.0	0.0	±0.1
Leq	94.0	94.0	0.0	±0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	±0.3

*T. Petch*

**7. Level linearity on the reference level range**

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	±1.1
136.0	136.0	0.0	±1.1
135.0	135.0	0.0	±1.1
134.0	134.0	0.0	±1.1
133.0	133.0	0.0	±1.1
132.0	132.0	0.0	±1.1
131.0	131.0	0.0	±1.1
129.0	129.0	0.0	±1.1
124.0	124.0	0.0	±1.1
119.0	119.0	0.0	±1.1
114.0	114.0	0.0	±1.1
109.0	109.0	0.0	±1.1
104.0	104.0	0.0	±1.1
99.0	99.0	0.0	±1.1
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	39.0	0.0	±1.1
34.0	34.0	0.0	±1.1
30.0	30.0	0.0	±1.1
29.0	29.0	0.0	±1.1
28.0	28.0	0.0	±1.1
27.0	27.1	0.1	±1.1
26.0	26.1	0.1	±1.1
25.0	25.1	0.1	±1.1

*T. Petch*

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lepeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.7	-0.7	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

*T. Petch*

**11. Overload indication**

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

**12. High level stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

*T. Petch*



## Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RION  
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24  
Serial No. : 00572551 / 158776 / 58777  
ID No. : BKK\_FS0876

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

Location : -  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 17 NOVEMBER 2023  
Calibration Date : 11-13 DECEMBER 2023  
Date of Issue : 18 DECEMBER 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced  
other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference  
Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KA1	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

## Result of calibration :

## 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

## 2. Self-generated noise

## 2.1 Normal test

Measured Value ( dB )
16.3

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	13.8
C - weight	19.9
Flat	25.8

## 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.2	-0.2	-0.2	± 5.0



## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	±0.2
C - weight	94.0	94.0	0.0	±0.2
Flat	94.0	94.0	0.0	±0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	±0.1
Slow	94.0	94.0	0.0	±0.1
Leq	94.0	94.0	0.0	±0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	±0.3

T. Petch

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	±1.1
136.0	136.0	0.0	±1.1
135.0	135.0	0.0	±1.1
134.0	134.0	0.0	±1.1
133.0	133.0	0.0	±1.1
132.0	132.0	0.0	±1.1
131.0	131.0	0.0	±1.1
129.0	129.0	0.0	±1.1
124.0	124.0	0.0	±1.1
119.0	119.0	0.0	±1.1
114.0	114.0	0.0	±1.1
109.0	109.0	0.0	±1.1
104.0	104.0	0.0	±1.1
99.0	99.0	0.0	±1.1
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	39.0	0.0	±1.1
34.0	34.0	0.0	±1.1
30.0	30.0	0.0	±1.1
29.0	29.0	0.0	±1.1
28.0	28.0	0.0	±1.1
27.0	27.1	0.1	±1.1
26.0	26.1	0.1	±1.1
25.0	25.1	0.1	±1.1

T. Petch

## 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lepeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.7	-0.7	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

T. Petch

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

T. Petch



## Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RION  
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24  
Serial No.: 00572552 / 170384 / 72890  
ID No.: BKK\_FS0877

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

Location : -  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 20 OCTOBER 2023  
Calibration Date : 01-02 NOVEMBER 2023  
Date of Issue : 03 NOVEMBER 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced  
other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

## Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

QF-TS12-04-04-020664

## Result of calibration :

## 1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

## 2. Self-generated noise

## 2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.6
Flat	23.5

## 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.4	0.4	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-0.8	-0.8	-0.7	±5.0

QF-TS12-04-04-020664

T. Petchurai

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.1	±2.0
4000	0.0	0.1	0.1	±3.0
8000	0.1	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.3

QF-TS12-04-04-020664

T. Petchurai



## Continuation of Calibration Certificate

Cert. No. : ACL23335  
Job No. : VC67AC0014  
Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
SEL	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L <sub>peak</sub> (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.9	-0.5	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

QF-TS12-04-04-020664

T. Petsh

## Continuation of Calibration Certificate

Cert. No. : ACL23335  
Job No. : VC67AC0014  
Pages : 8 of 8

## 11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	0.0	±1.5
89.5	89.5		

## 12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A-weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petsh



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL: 0-2717-3000-29 FAX: 0-2719-9484

Cert.No.: 23CH1369  
Page.: 1 of 3

## Certificate of Calibration

Equipment : pH Meter  
Manufacturer : Hach  
Model : HQ411d  
Serial No. : 200100031163  
ID No. : BKK\_EN0342  
Condition As-Received: Used Item  
Received Date : 26 October 2023  
Calibration Date : 27 October 2023  
Reference : 2310-0865DSC-3  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khweng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
Ambient Temperature : (25 ± 2.5) °C  
Relative Humidity : (50 ± 15) %  
Calibration Procedure : In-house method :  
- CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)  
- CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lemgagrakul

Approved by :   
Approved Signatory(✓) Sathip Meangmai  
( ) Warakorn Lemgagrakul  
( ) Ponpan Paipim

Issue Date : 31 October 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Cert.No.: 23CH1369  
Page.: 2 of 3

## Condition of this calibration result

1. Reference Standard Instrument : -  
Instrument Serial No. ID No. Cert. No. Due Date  
1) Ref. Standard Thermometer 4982054 110RC044 231908 26 Jul 2024  
This certification is traceable to the International System of Unit maintained through:-  
- Technology Promotion Association (Thailand-Japan)  
2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	913598	14 July 2025
pH 6.985	CPA chem	913599	14 July 2024
pH 9.997	CPA chem	931961	30 Sep 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

## Calibration Results

## Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor k
pH Electrode S/N : 230473042902	4.008	4.002	166.5	0.0044	2.00
	6.985	6.967	-10.4	0.0084	2.00
	9.997	10.005	-189.3	0.0071	2.00

Remark : - Can not connect the BNC because the plug does not match with the socket.

a 1187344





Cert.No.: 23CH1369  
Page.: 3 of 3

#### Calibration Results

Function : Temperature Measurement

(\*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : PHC281  
- Serial No. : 230473042902  
Dimension of probe;  
- Length : 103 mm  
- Diameter : 12 mm  
- Immersion Depth : 90 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
25.0	25.002	25.1	0.098	0.13	2.00

Remark : - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-000-

Saithip

# 1187343



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert.No.: 24CG952  
Page.: 1 of 2

Equipment : Burette  
Capacity : 50 mL  
Serial No. : -  
ID. No. : BKK\_EN0171

Manufacturer : Witeg  
Made in : Germany

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Ambient Temperature : (20 ± 2.5) °C  
Relative Humidity : (50 ± 10) %  
Barometric Pressure : 760 mmHg  
Calibration Procedure : ASTM E 542 - 01

Calibrated by : Natcha Chayingcheiw

Approved by :   
Approved Signatory

( ) Unnopphol Harachai  
(✓) Srisuda Khamtha  
( ) Sa-ngeunkam Wongsu

Issue Date : 27 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Equipment : Burette  
Received Date : 23 February 2024  
Condition As-Received : New Item  
Calibration Date : 27 February 2024  
Reference : 2402-0757DSC-1

Cert.No.: 24CG952  
Page.: 2 of 2

#### Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	XP205DR	1126143764	140RC004	23MM538	TPA	15 Sep 2024
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	0834181	140EC005	231948	TPA	10 Aug 2024

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.  
3. True value is converted to true volume at the standard temperature of 20 °C

#### Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
50	50.0032	0.010	2.00

Remark : mL = cm<sup>3</sup>

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-000-



Metrology  
SCI ECO Services Company Limited  
33/2 Moo 3, T.Banpa, A.Kaengkhroi, Saraburi 18110, Thailand.  
Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100  
Bangkok Tel : +668 9205 6851, +669 8247 2360  
Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T232160

Page 1 of 4

## Certificate of Calibration

Equipment : Chamber (Cooling Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK\_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd., Khaeng Phatthanakan,  
Khet Suan Luang, Bangkok 10250

Customer Location : Laboratory

Date of Receipt : 29 November 2023

Calibrated By : Atiphong Rongrat (Technician)

Approved By :   
Boonchai Suriyawong (Site Calibration Manager)  
09 JAN 2024

Date of Issue : 09 JAN 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

FM-L14119/15-05-66



## Calibration Report

Equipment : Chamber (Cooling Room)  
Date of Calibration : 6 December 2023  
Environment : Temperature : 23.4-24.9 °C  
Line Voltage : 221.4-230.2 V  
Relative Humidity : 55 - 65 %RH

## Condition of this results of calibration :

1. This equipment was calibrated by insert 16 standard thermocouples type T into its chamber, the other one standard thermocouples type T use for ambient temperature measurement. The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986). All data show below were final values and the initial data from customer request. The temperature scale used was based on ITS - 90.

## 2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T230773	10 April 2024
TC	TYPE T	TN171-TN180	T230773	10 April 2024
DATA LOGGER	34970A	T149	T230773	10 April 2024

## 3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244).

## 4. Condition of calibrated item : good

## Equipment Description :

Time Constant : 1 Hour 30 Minute At 3 °C  
Fresh Air Damper : ☐ Open ☐ Min. ☐ Medium ☐ Max.  
☐ Close  
☒ Not Available


## 5. Adjustment :

( X ) without adjustment ( ) after adjustment

Approved By: 

FM-L15118/18-08-66

## Calibration Report

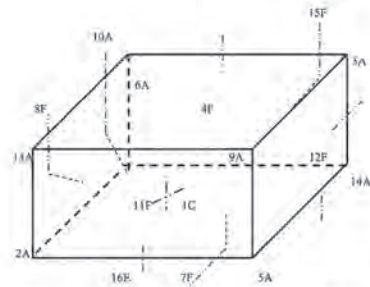

C = Centre, F = Centre of Face, A = Corner, B = Centre of Edge

1C = TN161	12F = TN172
2A = TN162	13A = TN173
3A = TN163	14A = TN174
4F = TN164	15F = TN175
5A = TN165	16E = TN176
6A = TN166	
7F = TN167	
8F = TN168	
9A = TN169	
10A = TN170	
11F = TN171	

Approved By: 

FM-L15118/18-08-66

## Calibration Report

## Measurement Results

Calibration Point	Average Standard Reading at each position (°C)											
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170	TN171	TN172
3.0	2.83	3.34	2.95	3.46	3.45	3.76	3.25	3.46	3.39	3.50	3.58	3.42
	TN173	TN174	TN175	TN176								
	3.33	3.39	3.13	3.43								

Chamber (Cooling Room)				Temperature Distribution				
Setting (°C)	Reading (°C)			Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min	Max	Average					
3.0	2.8	4.1	3.5	3.36	1.10	2.00	1.90	2.09

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By: 

FM-L15118/18-08-66







SARTORIUS

# Certificate of Calibration

REVIEW BY Sinluk B.  
APPROVED BY KLAL  
NEXT CAL DATE 09/02/24

Model Number : MSE224S-100-DU  
Description : Analytical Balance  
Serial Number : 27405555  
ID No. : BKK\_EN0003  
Manufacturer : Sartorius  
Certificate No. : 23BCI0310  
Issued Date : Friday, August 11, 2023  
Reference No. : 216011  
Page No. : 1 of 2

Customer Name : ALS Laboratory Group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250

Calibrated Place : Lab Room

Calibrated By : Mr. Chonchai Inthana  
Calibration Date : Wednesday, August 09, 2023

Metrological data :  
Capacity : 220 g Readability : 0.0001 g  
Ambients Conditions:  
Temperature : 22.8 °C ± 5.0 °C  
Humidity : 59.0 % RH ± 10.0 % RH  
Pressure : ±

Reasons for calibration  
☐ New Installation ☐ Service / Repair ☒ Re-calibration/ Maintenance  
Equipment Condition: ☒ Good Operate ☐ Fail

Measurement Method UKAS Publication Ref : Lab 14  
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2, YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp. Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.  
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division  
Sartorius (Thailand) Co., Ltd.

SOP FM 33 03 February 2022

Certificate No. T232009 Page 1 of 3

## Certificate of Calibration

Equipment : Chamber ( Oven )  
Manufacturer : Memmert  
Model : UF110  
Serial No. : B423.1549  
Customer Code : BKK\_EN0425  
ID No. : T4671A5  
Customer : ALS Laboratory Group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250  
Customer Location : Oven Room  
Date of Receipt : 1 November 2023  
Calibrated By : Atiphong Rongrat ( Technician )  
Approved By : Boonchai Suriyawong (Site Calibration Manager)  
Date of Issue : 09 NOV 2023

The uncertainties are for a confidence probability of approximately 95%.  
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

SARTORIUS

# Certificate of Calibration

Model Number : MSE224S-100-DU  
Description : Analytical Balance  
Serial Number : 27405555  
ID No. : BKK\_EN0003  
Manufacturer : Sartorius  
Certificate No. : 23BCI0310  
Issued Date : Friday, August 11, 2023  
Reference No. : 216011  
Page No. : 2 of 2

## Calibration Results : Without Adjustment

Repeatability	Eccentricity (Off-center loading error)
The repeatability is the ability of a weighing instrument to display nearly identical readout under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express repeatability quantitatively.	The off-center loading error is yielded by the difference between the readout of the load, i.e. 10 or 100 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to DIN, P75).
Nominal Value : (Low Load) 20 g Tolerance 0.0001 g Nominal Value : (High Load) 200 g Tolerance 0.0001 g Standard Deviation 0.00003 0.00005	Nominal value : 100 g Tolerance 0.0004 g Difference 1 2 0.0001 3 0.0000 4 0.0000 5 0.0001 6

Linearity  
The linearity, also called linearity error, describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g	Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
	0.01	0.0100	0.0100	0.0000	0.00014
	0.1	0.1000	0.1000	0.0000	0.00014
	1	1.0000	1.0000	0.0000	0.00014
	2	2.0000	2.0000	0.0000	0.00014
	5	5.0000	5.0000	0.0000	0.00014
	10	10.0000	10.0000	0.0000	0.00014
	20	20.0000	20.0000	0.0000	0.00014
	50	50.0000	50.0001	0.0001	0.00015
	100	100.0000	100.0000	0.0000	0.00019
	200	200.0000	200.0001	0.0001	0.00030

End of Report

SOP FM 33 03 February 2022

Certificate No. T232009 Page 2 of 3

## Calibration Report

Equipment : Chamber ( Oven )  
Date of Calibration : 6 November 2023  
Environment : Temperature : 27.6-28.1 °C  
Line Voltage : 222.7-227.4 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber, the other one resistance thermometer detector use for ambient temperature measurement. The calibration was done in according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001 ) and AS2853-1986 ).  
All data show below were final values and the initial data from customer request. The temperature scale used was based on ITS - 90.

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	31-(CH1-10)	T230504	24 March 2024
DATA LOGGER	34970A	T114	T230504	24 March 2024

3. This certificate is traceable to :  
National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244 )

4. Condition of calibrated item : good


Equipment Description :  
Time Constant 2 Hour 50 Minute At 104 °C  
Fresh Air Damper ☒ Open ☒ Min ☐ Medium ☐ Max  
☐ Close  
☐ Not Available

5. Adjustment :  
( X ) without adjustment ( ) after adjustment

Approved By : Boonchai Suriyawong



## Calibration Report

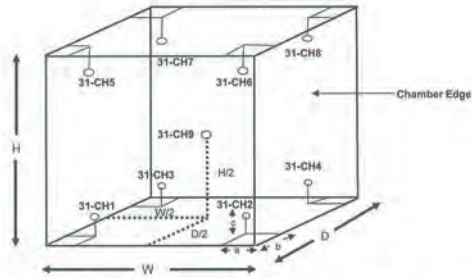

## Remark :

Internal Dimensions of Chamber : W (Width) = 56 cm, H (Height) = 41 cm, and D (Depth) = 48 cm.  
Size of Installed Standard sensor number 31-CH1 to number 31-CH9 : a = 5 cm, b = 5 cm, and c = 5 cm.  
Size of Installed Standard sensor number 31-CH9 : W/2 = 56 cm/2 H/2 = 41 cm/2 and D/2 = 48 cm/2

Measurement Results	Average Standard Reading at each position (°C)								
Calibration Point	31-CH1	31-CH2	31-CH3	31-CH4	31-CH5	31-CH6	31-CH7	31-CH8	31-CH9
104	103.82	104.10	103.74	104.26	103.95	104.31	103.87	104.00	103.81
180	180.04	180.21	179.44	180.31	179.02	180.13	180.17	180.35	179.69

Chamber ( Oven )		Temperature Distribution					
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (°C)	Uncertainty (±°C)	Coverage Factor k
	Min, Max	Average					
104.0	-	104.0	103.98	0.14	0.60	0.42	2.00
180.0	-	180.0	179.93	0.35	0.78	0.53	2.00

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By:

FM-L13 118/18-08-66

## Certificate of Calibration

Equipment : Digestion Unit

Manufacturer : SCP Science

Model : DigiPRER HT

Serial No. : HTC1120480658

Customer Code : BKK\_EN0366

ID No. : T2635A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 1

Date of Receipt : 11 April 2024

Calibrated By : Sujjar Naknakred ( Site Calibration Manager )

Approved By : / Boonchai Suriyawong ( Site Calibration Manager )

Date of Issue : 02 MAY 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L12 109/30-05-57

## Calibration Report

Equipment : Digestion Unit  
Date of Calibration : 21 April 2024  
Environment : Temperature : 23.9 - 26.3 °C  
Line Voltage : 221.8 - 225.9 V  
Relative Humidity : 55 - 65 %RH

## Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber, the other one thermocouple type T use for ambient temperature measurement. The calibration was done in according to W-T10.  
was based on ITS - 90.

## 2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A2-(CH11-CH14)	T230886	09 May 2024
DATA LOGGER	34970A	T47	T230886	09 May 2024

## 3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244 )

## 4. Condition of calibrated item : good

## Equipment Description :

Time Constant 1 Hour 6 Minute At 380 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

## 5. Adjustment :

( X ) without adjustment ( ) after adjustment

Approved By:

FM-L13 108/30-05-57

## Calibration Report



FRONT

## Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	MDA2-CH1 Block 1	MDA2-CH2 Block 2	MDA2-CH3 Block 3	MDA2-CH4 Block 4	MDA2-CH5 Block 5	MDA2-CH6 Block 6	MDA2-CH7 Block 7	MDA2-CH8 Block 8
380.0	380.0	379.2 - 380.5	Max °C	378.7	378.9	377.9	378.7	380.5	379.8	378.7	377.4
			Min °C	378.2	378.5	377.5	378.2	380.1	379.3	378.3	376.9
			Average °C	378.4	378.7	377.7	378.4	380.3	379.6	378.5	377.2
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.3	0.2	0.2

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	MDA2-CH9 Block 9	MDA2-CH10 Block 10	MDA2-CH11 Block 11	MDA2-CH12 Block 12	MDA2-CH13 Block 13	MDA2-CH14 Block 14	MDA2-CH15 Block 15	MDA2-CH16 Block 16
380.0	380.0	379.2 - 380.5	Max °C	378.4	378.6	379.2	379.6	381.9	380.6	379.1	378.1
			Min °C	377.8	378.2	378.7	379.2	381.4	379.9	378.3	377.2
			Average °C	378.1	378.4	379.0	379.4	381.6	380.3	378.7	377.7
			Stability ± °C	0.3	0.2	0.2	0.2	0.3	0.4	0.4	0.3

Approved By:

FM-L13 108/30-05-57





## Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoh, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T240742

Page 4 of 5

### Calibration Report



FRONT

#### Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	MDA3-CH1 Block 17	MDA3-CH2 Block 18	MDA3-CH3 Block 19	MDA3-CH4 Block 20	MDA3-CH1 Block 21	MDA3-CH2 Block 22	MDA3-CH3 Block 23	MDA3-CH4 Block 24
380.0	380.0	379.2 - 380.5	Max °C	378.9	379.2	379.5	380.1	382.1	381.0	378.9	377.8
			Min °C	378.2	378.6	379.1	379.6	381.7	380.2	378.3	377.2
			Average °C	378.5	378.9	379.3	379.8	381.9	380.6	378.6	377.5
			Stability ± °C	0.3	0.3	0.2	0.2	0.2	0.4	0.3	0.3

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	MDA3-CH1 Block 17	MDA3-CH2 Block 18	MDA3-CH3 Block 19	MDA3-CH4 Block 20	MDA3-CH1 Block 21	MDA3-CH2 Block 22	MDA3-CH3 Block 23	MDA3-CH4 Block 24
380.0	380.0	379.2 - 380.5	Max °C	378.5	378.1	378.0	378.6	380.7	379.7	377.7	380.9
			Min °C	378.2	377.8	377.7	378.1	380.3	379.0	377.2	380.4
			Average °C	378.4	378.0	377.9	378.4	380.5	379.4	377.5	380.6
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.3	0.2	0.3

Approved By:

FM-L13 10830-05-57



## Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoh, Saraburi 18110


Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T240742

Page 5 of 5

### Calibration Report

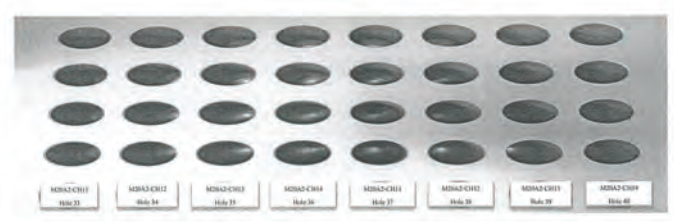

FRONT

#### Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block							
(°C)	(°C)	(°C)	Reading	MDA3-CH1 Block 17	MDA3-CH2 Block 18	MDA3-CH3 Block 19	MDA3-CH4 Block 20	MDA3-CH1 Block 21	MDA3-CH2 Block 22	MDA3-CH3 Block 23	MDA3-CH4 Block 24
380.0	380.0	379.2 - 380.5	Max °C	378.3	377.9	378.7	379.5	381.6	380.5	378.4	378.0
			Min °C	378.0	377.6	378.4	379.1	381.2	380.0	378.1	377.6
			Average °C	378.2	377.8	378.6	379.3	381.4	380.3	378.2	377.8
			Stability ± °C	0.2	0.2	0.2	0.2	0.2	0.2	0.2	0.2

The expanded uncertainty of temperature measurement was  $\pm 1.87^\circ\text{C}$

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95 %.

Approved By:

FM-L13 10830-05-57



บริษัท ดับเบิล เอส ไดแอกโนสติกส์ จำกัด  
DOUBLE S DIAGNOSTICS CO., LTD.

1. อาคาร 11 (11/11/11/11) ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110 โทรศัพท์ 02-247-7888  
2. 602 E-Mongkol 14, Bangkok, Thailand. Tel: +662 247-7888 Fax: +662 247-7888

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
Jan												

#### Periodical maintenance check list for Konelab

	6M	12M	Note
1. Diluent-wash tubing change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
2. ISE tubing change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	None
3. Syringe check/change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
4. Dispensing check/ change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
5. Waste tubing change when necessary	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
6. Lamp check/change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
7. Mixer paddle/paddle change(not Konelab20)	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
8. ISE needles check/change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	None
9. Pump tubing check/ change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
10. Broken/worn out part check /change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
11. Peristaltic pump check /cleaning/ lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
12. Heating check	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
13. Cooling check	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
14. Dispenser mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
15. Cuvette transfer mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
16. Dispenser movement check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
17. Sample/reagent register check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
18. Dispensing tubing tightness check	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
19. Photometer and optics cleaning/check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
20. Workstation PC cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
21. Mechanic cleaning/lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
22. Instrument cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
23. Complete analyzer testing with waterblank/QC or sample	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
24. Test parameters/Adjustment/config. Save to USB key	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
25. UPS Test	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

Place: DLS LAB Instrument: BSC Aquakem

Date/Time: 12/7/66 Serial no: 22981

Service done by: 57926 Install date:

Signature of customer: 07991 Date/Time: 12/12/66

#### Accuracy results

Aquakem 7.2.AQ2

Page: 1

Laboratory  
Analyzer User

7/12/2023 21:21

Performed

7/12/2023

Lot

W166

#### ACCEPTANCE CRITERIA

	Result	Limit	Warning
Temperature (°C)	37.7	37.0 $\pm$ 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	1.17	<1.7	
Photometric noise			
Max SD L340_2 (mV)	0.19	<2.0	
Max SD L340_4 (mV)	1.06	<3.0	
Linearity of photometer			
Slope	1.0188	0.94 - 1.06	
Curvature	0.0035	$\pm$ 0.02	
Max bias from linear fit (mV)	3.2	<15.0	
Max delta %	-2.0	$\pm$ 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (%)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (%)	4.13	3.85 - 4.40	
XDISP2 CV%	0.58	<2.0	
XDISP4 CV%	0.70	<2.0	
XDISP10 CV%	0.59	<2.0	
Needle 0.71 volume			
Average (A)	0.009	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (%)	0.06	<0.32	

#### OTHER INFORMATION

Dispensing ratio	Photom. noise: SD (mV)
Posit Result (A)	Posit L340_2 L340_4
1 0.1352	1 0.07 0.64
2 0.1624	2 0.09 3.06
3 0.1631	3 0.14 0.50
4 0.1631	4 0.13 0.53
5 0.1625	5 0.19 0.38
6 0.1650	6 0.02 0.64



Laboratory  
Analysar User


7/12/2023 21:21

## Linearity of sample dispensing

Test	Absorbance (A)
XD1SP2	0.311
XD1SP4	0.616
XD1SP10	1.478

## Linearity of photometer

U340	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.001	0.005	-0.004	-194.7
2	0.512	0.519	-0.007	-1.3
3	1.523	1.550	-0.027	-1.8
4	2.027	2.066	-0.039	-1.9
5	2.532	2.582	-0.050	-2.0

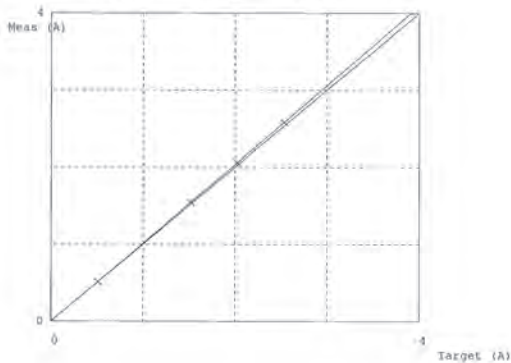

## Certificate of Calibration

Equipment:	CONDUCTIVITY METER	Certificate No.:	C24230292
Model:	ORION STAR A215	Issued Date:	25 December 2023
Serial No. (or ID.):	X58031	Job No.:	WD-00012882
Manufacturer:	Thermo Scientific	Page:	1 of 2
Electrode Serial No.	YV1-18416	Model:	ORION D13005MD
Condition:	In Condition	Brand:	Thermo Scientific

Customer: ALS Laboratory Group (Thailand) Co., Ltd.  
104 Soi Pattanakarn 40, Pattanakarn Rd.,  
Suan Luang, Bangkok 10250 Thailand

APPROVED BY Siwapan P.  
CAL DATE 15/12/24

Environment Condition: Temperature 21.7 °C ± 0.1 °C  
Humidity 53.7 %RH ± 0.1 %RH

Calibration Place: ALS Laboratory Group (Thailand) Co., Ltd. ( Wet Chemistry Lab 2 )  
104 Soi Pattanakarn 40, Pattanakarn Rd.,  
Suan Luang, Bangkok 10250 Thailand

Calibration By: Mr.Siwapan Srijan  
Calibration Date: 25 December 2023  
The Method used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14  
Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 850580, 890591 850592

Siwapan P.  
(Mr.Siwapan Srijan)  
Person in charge

Siwapan P.  
(Mr.Nitnun Srihawan)  
Authorized signatory

This certificate is issued in the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international standards or other recognized national standard laboratories.  
The measurement uncertainty stated in this report is a standard uncertainty which is obtained from this standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is expressed in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM).  
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced without the prior approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีเซีย จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110  
2533 Sukhumvit Road, Bangkok, Thailand, Bangkok 10110  
Phone: +66 2028 7000 Email: lab-calibration@dksh.com Website: www.dksh.com/calibration/thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C34-05: 12 Sep 2022



Certificate No.: C24230292 Page: 2 of 2

## Calibration Results:

## Before Adjustment

Standard	Unit Under Calibration	Correction	Coverage Factor	Uncertainty ( ± )
Conductivity Solution	Reading		( k )	
84.000 µS/cm	92.64 µS/cm	-8.640 µS/cm	2.00	0.88 µS/cm
1413.0 µS/cm	1423 µS/cm	-10.0 µS/cm	2.00	11 µS/cm
12.880 mS/cm	12.81 mS/cm	0.070 mS/cm	2.00	0.12 mS/cm

## After Adjustment: at 84.0 µS/cm, 1413 µS/cm, 12.88 mS/cm

Standard	Unit Under Calibration	Reading	Correction	Coverage Factor (k)	Uncertainty (±)
Conductivity Solution					
84.000 µS/cm	84.03 µS/cm	-0.030 µS/cm	2.00	0.68 µS/cm	
1413.0 µS/cm	1414 µS/cm	-1.0 µS/cm	2.00	11 µS/cm	
12.880 mS/cm	12.86 mS/cm	0.020 mS/cm	2.00	0.098 mS/cm	

The End of Certificate

บริษัท ดีเคเอส อีเซีย จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110  
2533 Sukhumvit Road, Bangkok, Thailand, Bangkok 10110  
Phone: +66 2028 7000 Email: lab-calibration@dksh.com Website: www.dksh.com/calibration/thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C34-05: 12 Sep 2022



## ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00012882

ชนิดเครื่องมือ: CONDUCTIVITY METER		รุ่น: ORION STAR A215		หมายเลขเครื่องมือ: X58031	
ตรวจสอบ (วัน)	รายการตรวจสอบ	ตรวจสอบ (ดี/ไม่)	ตรวจสอบ (ดี/ไม่)	ตรวจสอบ (ดี/ไม่)	หมายเหตุ
25 Dec 2023	รายการตรวจสอบ	25 Dec 2023	ไม่	ไม่	
ปกติ	ปกติ	ปกติ	ไม่ปกติ	ไม่	
General					
<input checked="" type="checkbox"/>	1. ความสมบูรณ์ของเครื่อง	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	3. สวิตช์ ปิด - เปิด เครื่อง (On-Off Switch)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
Spectrophotometer					
<input checked="" type="checkbox"/>	6. แบตเตอรี่สำรอง (Battery Backup) >= 2.5 VDC	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	7. ความแม่นยำของความยาวคลื่น (Wavelength Control)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	9. แสงยูวี/แสงอินฟราเรด (UV < 3,000 hour)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	10. แสงยูวี/แสงอินฟราเรด (Visible < 5,000 hour)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	11. ช่องใส่ตัวอย่าง (Caroussel Module)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
pH Meter and Conductivity Meter					
<input checked="" type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	13. ระดับการละลายใน Electrode (Level KCl)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	14. ฝาปิดกันละออง Electrode (Dust Protection Hood)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	15. ขาตั้งอิเล็กโทรด (Stand)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
Turbidimeter					
<input checked="" type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่น้อย 3.0)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
Automatic titrator					
<input checked="" type="checkbox"/>	18. สลัก Piston Burettes	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	19. Function Rinsing and Dosing	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
<input checked="" type="checkbox"/>	20. ระบบไหลเวียนของสารละลาย	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	

ผู้ตรวจสอบ:

Mr.Siwapan Srijan  
Service Engineer

บริษัท ดีเคเอส อีเซีย จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10110  
2533 Sukhumvit Road, Bangkok, Thailand, Bangkok 10110  
Phone: +66 2028 7000 Email: lab-calibration@dksh.com Website: www.dksh.com/calibration/thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-R143E: 20 Jul 2022



Cert.No.: 23TW243  
Page.: 1 of 2

## Certificate of Testing

Equipment : DO Meter  
Manufacturer : YSI  
Model : 5000-230V  
Serial No. : 09J101147  
ID No. : BKK\_EN0017  
Received Date : 15 November 2023  
Test Date : 16 November 2023  
Reference : 2311-0505OSC-4  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
Laboratory Condition : Temperature ( 25 ± 5 ) °C  
Humidity ( 50 ± 20 ) %  
Test Procedure : In - house method : CP-GHB  
by Comparison Technique with Azide Modification Method  
Tested by : Walailak Sinithean  
Approved by :   
Approved Signatory  
( ✓ ) Sathip Meangmai  
( ) Warakom Lemgatrakul  
( ) Ponpan Palpim  
Issue Date : 17 November 2023



0328569



Cert.No.: 23TW243  
Page.: 2 of 2

### Condition of this result of calibration

1. Reference Standard Instruments :  
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).
- | Instruments | Serial No. | ID No.   | Certificate No. | Due Date    |
|-------------|------------|----------|-----------------|-------------|
| 1) Burette  | -          | 130BU10  | 23CG1172        | 22 Mar 2025 |
| 2) Balance  | 1124013382 | 140RC006 | 23MM18          | 20 Feb 2024 |
2. Standard Material :-
- | Material                        | Manufacturer | Lot.No.   | Assay  |
|---------------------------------|--------------|-----------|--------|
| Sodium Thiosulfate pentahydrate | Merck        | AM1763316 | 100.2% |
- Result : Dissolved Oxygen Meter Adjustment With Air 100 %  
Dissolved Oxygen Probe No.: 16K100498

Titration Method (Azide Modification Method)	DO Meter Reading	Standard Deviation
(mg/L)	(mg/L)	(mg/L)
8.18	8.18	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency. The environmental impact control and present to organization it may concerned intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full without written approval of the laboratory.

-000-

1190297



Cert. No.: 23LM192  
Page.: 1 of 2

## Certificate of Calibration

Equipment : DO Meter with Sensor  
Manufacturer : YSI  
Model : 5000-230V  
Serial No. : 09J101147  
ID No. : BKK\_EN0017  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
Location : TPA Chemistry Calibration Laboratory  
Received Order : 15 November 2023  
Calibrated Date : 16 November 2023  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
AC Line Voltage : ( 220 ± 22 ) V  
Calibrated by : Kunchit Promprut  
Approved by :   
Approved Signatory  
( ) Pornthippa Tameyakul  
( ) Ponpan Palpim  
( ✓ ) Suwit Injai  
Issue Date : 17 November 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced without the written approval of the proper authority.  
Approved by the head of Corporate Services 3 : Equipment Calibration and Testing Services

0060730



Equipment : DO Meter with Sensor  
Condition As-Received : Used Item  
Reference : 2311-0505OSC-10  
Procedure Used :-

Cert. No.: 23LM192  
Page.: 2 of 2

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer ( IPRT ) into Temperature Bath.  
The temperature scale used was based on ITS-90.

### Condition of this result of calibration

1. Reference standard instrument:-
- | Instrument             | Serial No. | Cert. No. | Traceable | Due Date    |
|------------------------|------------|-----------|-----------|-------------|
| 1) Digital Thermometer | 3240076    | 23J305    | TPA       | 15 Mar 2024 |
2. This certificate is valid only to the item calibrated on date and place of calibration.  
3. This certification is traceable to the International System of Unit.  
Remark : TPA : Technology Promotion Association ( Thailand - Japan )  
Result of Calibration :- ( \* ) Without Adjustment  
Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N : 16K100498

Calibration Point ( °C )	Immersion Depth ( mm )	Standard Temperature ( °C )	UUC* Reading ( °C )	Error ( °C )	Uncertainty ( ± °C )	Coverage Factor k
20.0	60	19.997	19.93	-0.067	0.15	2.00

UUC\* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-

1190298





CERTIFICATE No : 24T2852  
REFERENCE No : 72619-8

PAGE : 1 OF 2

### Certificate of Calibration

EQUIPMENT : COOLED INCUBATOR

MANUFACTURER : MEMMERT

MODEL : ICP750

SERIAL No : F819.0021

ID No : BKK\_EN0304

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN  
RD., KHWAENG PHATTHANAKAN, KHET SUAN  
LUANG, BANGKOK 10250, THAILAND

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 20-Mar-24

APPROVED BY : PONGSAK J.

ISSUED DATE : 21-Mar-24

RECEIVED DATE : 20-Mar-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF QUALITY CALIBRATION CO., LTD.

F-G010 REV : 03



CERTIFICATE No : 24T2852

PAGE : 2 OF 2

### Calibration Report

EQUIPMENT : COOLED INCUBATOR

MANUFACTURER : MEMMERT

MODEL : ICP750

ID No : BKK\_EN0304

RECEIVED DATE : 20-Mar-24

AMBIENT TEMPERATURE : 26 °C ± 1 °C

S/N : F819.0021

CALIBRATION DATE : 20-Mar-24

RELATIVE HUMIDITY : 54 %RH ± 10 %RH

#### CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TIS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

#### 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7286308	23T6641	14-Jul-24
3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.				
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.				
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-				
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.				


#### RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

##### GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1

Overall Line Voltage (V) variation : 5

Instrument Condition : Normal



FRONT

##### CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
20.0	20.0	0.16	0.21	0.41

##### TEMPERATURE MEASUREMENT ACCURACY TEST

TEMPERATURE MEASUREMENT ACCURACY TEST											
Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
20.0	20.0	19.88	19.93	19.87	19.86	19.98	19.94	19.94	19.89	19.91	0.42

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA. THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.  
END OF CALIBRATION REPORT

F-G010 REV : 03



Certificate No. T232157

Page 1 of 4

### Certificate of Calibration

Equipment : Hot Block

Manufacturer : Environmental Express

Model : B3000-240

Serial No. : 2021CODW148

Customer Code : BKK\_EN0370

ID No. : T2940A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,  
Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab2

Date of Receipt : 29 November 2023

Calibrated By : Sujjar Naknakred ( Site Calibration Manager )

Approved By : Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 18 DEC 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L12 J0870-05-57



Certificate No. T232157

Page 2 of 4

### Calibration Report

Equipment : Hot Block

Date of Calibration : 6 December 2023

Environment : Temperature : 20.1°C-23.°C

Line Voltage : 222.1-227.3 V

Relative Humidity : 55 - 65 %RH

#### Condition of this results of calibration :

1. This equipment was calibrated by insert 29 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90

#### 2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN224-TN230	T230546	10 April 2024
TC	TYPE T	TN231-TN240	T230546	10 April 2024
TC	TYPE T	TN241-TN270	T230548	10 April 2024
DATA LOGGER	34970A	T149	T230546	10 April 2024

3. This certificate is traceable to : National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244 )

#### 4. Condition of calibrated item : good

##### Equipment Description :-

Time Constant	2	Hour	6	Minute	At 150 °C
Fresh Air Damper	<input type="checkbox"/> Open	<input type="checkbox"/> Min	<input type="checkbox"/> Medium	<input type="checkbox"/> Max	
	<input type="checkbox"/> Close				
	<input checked="" type="checkbox"/> Not Available				

5. Adjustment : ( ) without adjustment

( X ) after adjustment

Approved By : [Signature]

FM-L12 J0870-05-57






Certificate No. T232157

Page 3 of 4

## Calibration Report

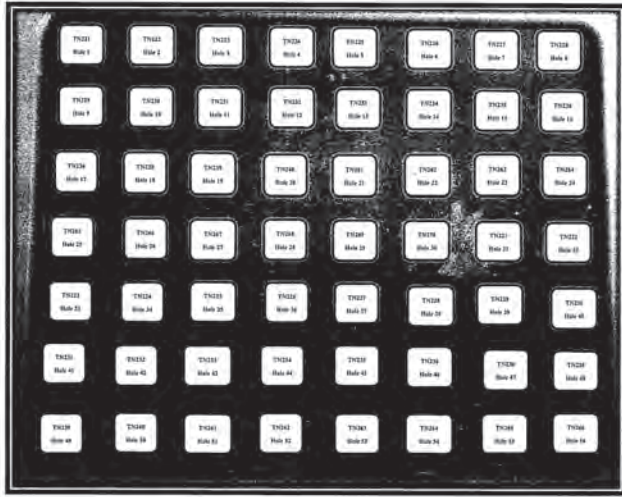

FRONT CONTROL

Approved By:

FM-L13 08/30-05-57



Certificate No. T232157

Page 4 of 4

## Calibration Report

### Measurement Results

		Average Standard Reading at each position (°C)															
		T2321 Max 1	T2322 Max 2	T2323 Max 3	T2324 Max 4	T2325 Max 5	T2326 Max 6	T2327 Max 7	T2328 Max 8	T2329 Max 9	T2330 Max 10	T2331 Max 11	T2332 Max 12	T2333 Max 13	T2334 Max 14	T2335 Max 15	T2336 Max 16
CAL POINT	Max	150.33	150.05	149.08	150.90	150.95	150.41	149.80	150.22	150.08	150.30	150.66	150.43	149.91	149.82	150.07	150.08
	Min	150.19	149.85	149.68	150.71	150.66	150.21	149.67	150.08	150.30	150.66	150.43	150.75	150.45	150.75	150.45	150.75
	Average	150.69	150.49	150.49	150.44	150.34	150.24	150.24	150.32	150.32	150.32	150.32	150.32	150.32	150.32	150.32	150.32
		T2337 Max 17	T2338 Max 18	T2339 Max 19	T2340 Max 20	T2341 Max 21	T2342 Max 22	T2343 Max 23	T2344 Max 24	T2345 Max 25	T2346 Max 26	T2347 Max 27	T2348 Max 28	T2349 Max 29	T2350 Max 30	T2351 Max 31	T2352 Max 32
		150.40	150.16	149.28	149.44	149.73	150.04	150.31	150.60	150.90	150.90	150.90	150.90	150.90	150.90	150.90	150.90
		150.43	149.91	149.01	149.23	149.55	149.90	150.06	150.43	150.75	150.75	150.75	150.75	150.75	150.75	150.75	150.75
		Average	150.56	150.64	149.14	149.33	149.64	149.87	150.18	150.53	150.87	150.87	150.87	150.87	150.87	150.87	150.87
		T2353 Max 33	T2354 Max 34	T2355 Max 35	T2356 Max 36	T2357 Max 37	T2358 Max 38	T2359 Max 39	T2360 Max 40	T2361 Max 41	T2362 Max 42	T2363 Max 43	T2364 Max 44	T2365 Max 45	T2366 Max 46	T2367 Max 47	T2368 Max 48
		150.28	150.20	149.67	149.99	150.07	149.93	150.90	150.48	150.21	150.54	150.54	150.54	150.54	150.54	150.54	150.54
		150.02	150.02	149.61	149.78	149.82	149.86	150.36	150.22	149.92	150.33	150.33	150.33	150.33	150.33	150.33	150.33
		Average	150.14	150.14	149.74	149.89	149.94	149.87	150.73	150.36	150.86	150.86	150.86	150.86	150.86	150.86	150.86
		T2369 Max 49	T2370 Max 50	T2371 Max 51	T2372 Max 52	T2373 Max 53	T2374 Max 54	T2375 Max 55	T2376 Max 56	T2377 Max 57	T2378 Max 58	T2379 Max 59	T2380 Max 60	T2381 Max 61	T2382 Max 62	T2383 Max 63	T2384 Max 64
		150.83	150.23	150.41	151.42	150.67	150.81	150.97	150.75	150.51	150.62	150.62	150.62	150.62	150.62	150.62	150.62
		150.61	150.28	151.18	150.41	150.41	150.69	150.73	150.33	150.24	149.91	149.91	149.91	149.91	149.91	149.91	149.91
		Average	150.73	150.41	150.88	150.93	150.54	150.76	150.88	150.64	150.38	150.38	150.38	150.38	150.38	150.38	150.38
		T2385 Max 65	T2386 Max 66	T2387 Max 67	T2388 Max 68	T2389 Max 69	T2390 Max 70	T2391 Max 71	T2392 Max 72	T2393 Max 73	T2394 Max 74	T2395 Max 75	T2396 Max 76	T2397 Max 77	T2398 Max 78	T2399 Max 79	T2400 Max 80
		150.37	150.85	150.35	149.72	149.43	149.30	151.26	150.64	151.11	150.75	150.75	150.75	150.75	150.75	150.75	150.75
		149.97	150.64	150.34	149.50	149.14	149.48	150.64	150.37	150.74	150.74	150.74	150.74	150.74	150.74	150.74	150.74
		Average	150.12	150.74	150.43	149.61	149.39	149.65	150.95	150.61	150.92	150.92	150.92	150.92	150.92	150.92	150.92
		T2401 Max 81	T2402 Max 82	T2403 Max 83	T2404 Max 84	T2405 Max 85	T2406 Max 86	T2407 Max 87	T2408 Max 88	T2409 Max 89	T2410 Max 90	T2411 Max 91	T2412 Max 92	T2413 Max 93	T2414 Max 94	T2415 Max 95	T2416 Max 96
		150.16	150.41	150.79	150.63	150.25	149.38	149.38	149.38	149.38	149.38	149.38	149.38	149.38	149.38	149.38	149.38
		149.95	150.24	150.59	150.85	150.08	149.40	149.40	149.40	149.40	149.40	149.40	149.40	149.40	149.40	149.40	149.40
		Average	150.66	150.53	150.68	150.54	150.17	149.49	149.49	149.49	149.49	149.49	149.49	149.49	149.49	149.49	149.49

		Hot Block		Temperature Distribution	
Setting (°C)	Reading (°C)	Reading (°C)		Stability (±°C)	Uncertainty (±°C)
		Min	Max		
150.0	149.9	150.1	150.0	0.31	1.02

The calibration results apply only to the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By:

FM-L13 08/30-05-57



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor 7 Ramak Road  
Silom Bangkok Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barscientific.com



## Certificate of Calibration

Number of Page(s) 1 of 3

Certificate No. BSCC-UV-367/23  
Equipment UV/Vis Spectrophotometer  
Model UV-1800  
Manufacturer Shimadzu  
Serial No. A11454908533CD  
ID No. BKK\_EN0018  
Date of receipt 15 September 2023  
Date of calibration 15 September 2023  
Date of issue 22 September 2023

Customer name ALS Laboratory Group (Thailand) Co., Ltd.

Address 104 Soi Phattananak 40, Phattananak Road, Phattananak, Suan Luang, Bangkok 10250

Temperature (23.4 - 24.7) °C (On site)  
Humidity (55.5 - 61.2) %RH (On site)

Equipment condition Good Operation

Calibration Location Organic Prep

Calibration Procedure In-house method WI-UV-702-01 based on ASTM E275-01

Traceability Wavelength Accuracy is traceable to certificate No. 95917 and 95918  
Photometric Accuracy is traceable to certificate No. 95937 and 95924  
Stray Light is traceable to certificate No. 95908  
The above certificate are traceable to SI unit through Bara Scientific Ltd.  
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by Mr. Wanchana Janloy

REVIEW BY

APPROVED BY

NEXT CAL DATE 15/9/2024

Approved by

Mr. Kanchit Choothep  
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.



**Bara Scientific Co., Ltd.**  
968 U Chu Liang Building Floor 7 Ramak Road  
Silom Bangkok Bangkok Thailand 10500  
Tel : 02-6324300 Fax : 02-6375496-7  
www.barscientific.com



## Certificate of Calibration

Certificate No. BSCC-UV-367/23

Number of Page(s) 2 of 3

### Calibration Results:

#### 1. Wavelength Accuracy

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
241.70	241.67	-0.03	0.18
334.02	334.03	0.01	0.18
418.53	418.59	0.06	0.18
572.99	573.14	0.15	0.18
879.41	879.21	-0.20	0.18

#### 2. Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.0075
	0.7467	0.7460	-0.0007	0.0075
257	0.0000	0.0000	0.0000	0.0075
	0.8662	0.8646	-0.0016	0.0075
313	0.0000	0.0000	0.0000	0.0075
	0.2904	0.2908	0.0004	0.0075
350	0.0000	0.0001	0.0001	0.0075
	0.6429	0.6415	-0.0014	0.0075

\*CNR = Customer not request

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate.  
Advertising the report / Certificate and publicity of the results are prohibited and also shall not be reproduced  
except in full, without written approval of the Bara Scientific Co., Ltd.