

ภาคผนวก ง

---

ใบรับรองการสอบเทียบเครื่องมือ



รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

right solutions.  
right partner.




Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Suspended Particulate	High Volume	RYG_FS0396	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0292	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	RYG_EN0001	1-Mar-23	1-Mar-24	12
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0189	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0192	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	RYG_EN0001	1-Mar-23	1-Mar-24	12
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0413	10-Feb-23	10-Aug-24	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0414	10-Feb-23	10-Aug-24	18
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0496	26-Jan-24	25-Jan-25	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0386	19-Oct-23	19-Oct-24	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0388	5-Jan-24	4-Jan-25	12
Sea Water	pH at 25 °C	pH Meter	RYG_EN0152	14-Dec-23	14-Dec-24	12
Sea Water	Dissolved Oxygen	Chamber (Cooling Room)	RYG_EN0184	25-Jan-23	25-Jul-24	18
Sea Water	BOD	DO meter with Sensor	RYG_EN0032	24-Jul-23	24-Jan-25	18
Sea Water	BOD	Incubator	RYG_EN0154	29-May-23	29-Nov-24	18
Sea Water	BOD	Burette	RYG_EN0216	25-Sep-23	25-Sep-24	12
Sea Water	Total Suspended Solids	Electronic Balance	RYG_EN0002	1-Mar-23	1-Mar-24	12
Sea Water	Total Suspended Solids	Hot Air Oven	RYG_EN0010	20-Oct-22	20-Apr-26	18
Sea Water	Total Solids	Electronic Balance	RYG_EN0002	1-Mar-23	1-Mar-24	12
Sea Water	Total Solids	Hot Air Oven	RYG_EN0010	20-Oct-22	20-Apr-26	18
Sea Water	Total Dissolved Solids 180°C	Electronic Balance	RYG_EN0002	1-Mar-23	1-Mar-24	12
Sea Water	Total Dissolved Solids 180°C	Hot Air Oven	RYG_EN0010	20-Oct-22	20-Apr-26	18
Sea Water	Salinity	Conductivity meter	RYG_EN0029	4-Sep-23	4-Mar-25	18
Sea Water	Oil & Grease	Electronic Balance	RYG_EN0002	1-Mar-23	1-Mar-24	12
Sea Water	Oil & Grease	Hot Air Oven	RYG_EN0006	20-Oct-22	20-Apr-24	18
Sea Water	Oil & Grease	Water Bath	RYG_EN0061	20-Oct-22	20-Apr-24	18
Sea Water	Temperature	DO Meter With Sensor	RYG_FS0529	6-Dec-23	6-Dec-24	12
Sea Water	Conductivity	Conductivity meter	RYG_EN0029	4-Sep-23	4-Mar-25	18
Sea Water	Lead	ICP-MS	BKK_EL0026	12-Dec-23	13-Jun-25	12
Sea Water	Lead	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sea Water	Lead	Chamber (Cooling Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Sea Water	Zinc	ICP-MS	BKK_EL0026	12-Dec-23	13-Jun-25	12
Sea Water	Zinc	Hot Block	BKK_EL0054	22-Sep-23	22-Mar-25	18
Sea Water	Zinc	Chamber (Cooling Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Sea Water	Mercury	Mercury Analyzer	BKK_EL0128	6-Dec-23	6-Dec-24	12
Sea Water	Total Coliform	Autoclave	BKK_ML0041	4-Oct-23	4-Apr-25	18
Sea Water	Total Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Sea Water	Total Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Sea Water	Fecal Coliform	Autoclave	BKK_ML0041	4-Oct-23	4-Apr-25	18
Sea Water	Fecal Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Sea Water	Fecal Coliform	Hot Air Oven	BKK_ML0013	21-Nov-22	21-May-24	18
Sea Water	Fecal Coliform	Water Bath	BKK_ML0056	20-Apr-23	20-Apr-24	12

## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow SPP 3 Co., Ltd.	Barometric Pressure (mm Hg) :	758
Calibrate Location :	Thai Tank Farm	Temperature ( °C ) :	29
Calibrate Date :	20-Feb-24	High Volume ID :	RYG_FS0396
CalibrationSheet No.:	C-200224-RYG_FS0396	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0206	High Volume S/N :	5688
Calibrator Model :	TE-5028A	Calibrator Slope :	1.47433
Calibrator S/N :	1543	Calibrator Intercept :	-0.01503

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.2	1.0131	40	Slope : 30.2766
2	3.0	1.1805	44	Intercept : 8.8129
3	4.0	1.3608	50	Correlation Coefficient : 0.9983
4	4.9	1.5045	54	
5	6.1	1.6769	60	

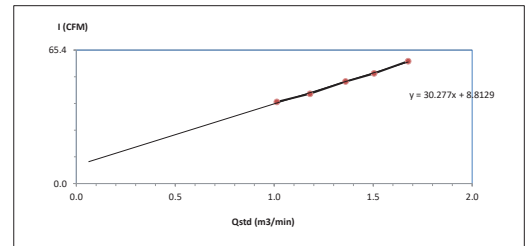

Calibrated by :   
(Mr. Anuwet Tema)  
Field Scientist(1)

Approved by :   
(Mr. Noppong Jantarupan)  
Enviro Field Coordinator Scientist (3)

FORM NO.: F-06-073 REVISION NO.: 2 ISSUE DATE: 20/11/23


RYG\_EN0001



## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow SPP 3 Co., Ltd.	Barometric Pressure (mm Hg) :	758
Calibrate Location :	Map Ta Phut Port (North of Project)	Temperature ( °C ) :	29
Calibrate Date :	20-Feb-24	High Volume ID :	RYG_FS0292
CalibrationSheet No.:	C-200224-RYG_FS0292	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0206	High Volume S/N :	5497
Calibrator Model :	TE-5028A	Calibrator Slope :	1.47433
Calibrator S/N :	1543	Calibrator Intercept :	-0.01503

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.2	1.0131	40	Slope : 30.2259
2	3.0	1.1805	44	Intercept : 8.7802
3	4.1	1.3775	50	Correlation Coefficient : 0.9978
4	4.9	1.5045	54	
5	6.1	1.6769	60	

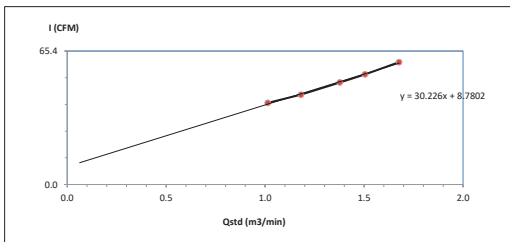

Calibrated by :   
(Mr. Anuwet Tema)  
Field Scientist(1)

Approved by :   
(Mr. Noppong Jantarupan)  
Enviro Field Coordinator Scientist (3)

FORM NO.: F-06-073 REVISION NO.: 2 ISSUE DATE: 20/11/23

Sartorius (Thailand) Co., Ltd.  
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310  
Tel: +66 2643 8351-6, e-mail: service.thailand@sartorius.com



SARTORIUS  
REVIEW BY :   
APPROVED BY :   
NEXT CAL DATE : 01/03/24

## Certificate of Calibration

Model Number :	LA130S-F	Certificate No. :	23BCI0110
Description :	Analytical Balance	Issued Date :	Friday, March 03, 2023
Serial Number :	25409684	Reference No. :	204833
ID No. :	RYG_EN0001	Page No. :	1 of 2
Manufacturer :	Sartorius		

Customer Name : ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)  
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd. (Balance Room)  
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated By : Mr.Chonchai Inthana  
Calibration Date : Wednesday, March 01, 2023  
Calibration Procedure No. : This calibration was conducted by  
Using in-house calibration procedure number (WI-003)  
Based on UKAS LAB 14 : 2019

Metrological data :  
Capacity : 150 g Readability : 0.0001 g  
Reasons for calibration : ☐ New Installation ☐ Service / Repair ☒ Re-calibration/ Maintenance  
Ambients Conditions :  
Temperature : 24.2 °C ± 5.0 °C  
Humidity : 60.0 % RH ± 10.0 % RH  
Pressure : ±  
Equipment Condition : ☒ Good Operate ☐ Fair

Measurement Method : UKAS Publication Ref :Lab 14  
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

## Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2.YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Luton MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division  
Sartorius (Thailand) Co., Ltd.

Mr.chonchai inthana(Technical Manager)



# Certificate of Calibration

Model Number: LA130S-F  
Description: Analytical Balance  
Serial Number: 25409664  
ID No.: RYG\_EN0001  
Manufacturer: Sartorius

Certificate No.: 23BCI0110  
Issued Date: Friday, March 03, 2023  
Reference No.: 204833  
Page No.: 2 of 2

## Calibration Results : Without Adjustment

**Repeatability**  
The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	10.0000	100.0001
10 g	10.0000	100.0002
Tolerance	10.0001	100.0001
0.0001 g	10.0000	100.0000
	9.9999	100.0002
Nominal Value : (High Load)	10.0000	100.0001
100 g	10.0001	100.0001
Tolerance	10.0000	100.0001
0.0001 g	9.9999	100.0002
	9.9998	100.0001
Standard Deviation	0.00009	0.00006

**Eccentricity (Off-center loading error)**  
The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value :	50 g
Tolerance	0.0004 g

**Linearity**  
The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance	0.0002 g			
Nominal Value	Conventional Mass Value	Displayed Value	Deviation	Uncertainty
(g)	(g)	(g)	(g)	(g)
0.01	0.0100	0.0100	0.0000	0.00022
0.05	0.0500	0.0500	0.0000	0.00023
0.1	0.1000	0.1000	0.0000	0.00023
0.5	0.5000	0.5000	0.0000	0.00023
1	1.0000	1.0000	0.0000	0.00023
2	2.0000	2.0000	0.0000	0.00023
5	5.0000	5.0000	0.0000	0.00023
10	10.0000	10.0001	0.0001	0.00024
20	20.0000	20.0001	0.0001	0.00023
100	100.0000	100.0002	0.0002	0.00026

End of Report


SOP FM 33 03 February 2022

## High Volume Air Sampler Calibration Worksheet

Project Site: Glow SPP 3 Co., Ltd.  
Calibrate Location: Thai Tank Farm  
Calibrate Date: 20-Feb-24  
Calibration Sheet No.: C-200224-RYG\_FS0189  
Calibrator ID: RYG\_FS0206  
Calibrator Model: TE-5028A  
Calibrator S/N: 1543

Barometric Pressure (mm Hg): 758  
Temperature (°C): 29  
High Volume ID: RYG\_FS0189  
High Volume Model: TE-5009X  
High Volume S/N: 4797  
Calibrator Slope: 0.92345  
Calibrator Intercept: -0.0095

Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I: Chart (CFM)	Linear Regression
1	2.2	1.023	32	Slope: 56.3870
2	2.5	1.090	36	Intercept: -25.4706
3	2.8	1.153	40	Correlation Coefficient: 0.9991
4	3.2	1.232	44	
5	3.6	1.306	48	

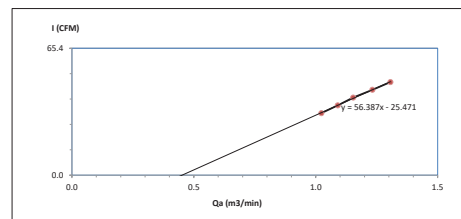

Calibrated by: (Mr. Anuwet Tema) Field Scientist(1)

Approved by: (Mr. Noppong Juntarapan) Enviro Field Coordinator Scientist (3)


FORM NO.: F 06-074 REVISION NO.:2 ISSUE DATE: 20/11/23

## High Volume Air Sampler Calibration Worksheet

Project Site: Glow SPP 3 Co., Ltd.  
Calibrate Location: Map Ta Phut Port (North of Project)  
Calibrate Date: 20-Feb-24  
Calibration Sheet No.: C-200224-RYG\_FS0192  
Calibrator ID: RYG\_FS0206  
Calibrator Model: TE-5028A  
Calibrator S/N: 1543

Barometric Pressure (mm Hg): 758  
Temperature (°C): 29  
High Volume ID: RYG\_FS0192  
High Volume Model: TE-5009X  
High Volume S/N: 5331  
Calibrator Slope: 0.92345  
Calibrator Intercept: -0.0095

Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I: Chart (CFM)	Linear Regression
1	2.1	1.006	32	Slope: 49.9639
2	2.4	1.068	36	Intercept: -17.7511
3	2.8	1.153	40	Correlation Coefficient: 0.9968
4	3.3	1.251	44	
5	3.6	1.306	48	

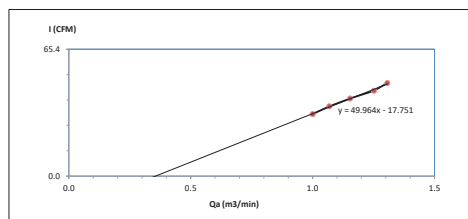

Calibrated by: (Mr. Anuwet Tema) Field Scientist(1)

Approved by: (Mr. Noppong Juntarapan) Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-074 REVISION NO.:2 ISSUE DATE: 20/11/23



JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.  
63/14-15, 67/35-36  
Petchkasem 2/17, Rd. Wattana, Bangkok 10110  
Bangkok 10500 (Thailand)  
Tel: +66(0)80812  
Mobile: +66(0)995453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
(ISO/IEC 17025:2017)  
NSC-TSI-TS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.



Certificate Number

CL-020-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

### MEASUREMENT ITEM

### MANUFACTURER

### MODEL/TYPE

### SERIAL NUMBER

### ID NUMBER

### CONDITION AS-RECEIVED

### CUSTOMER

### RECEIVED DATE

### MEASUREMENT DATE

### ISSUE DATE

### ENVIRONMENTAL CONDITIONS:

### PLACE OF CALIBRATION

### CALIBRATION CONDITIONS

### Preconditioning

### Measurement Condition

### TABULATION OF RESULTS:

### Remarks:

### Calibration procedure:

### Traceability:

### Uncertainty of Measurement:

### Approval signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:

### Signature:



Certificate Number

CL-020-66

Page 2 of 2 Pages

MEASUREMENT RESULTS<sup>1</sup>

The cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle. UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

$V_{std}$ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$V_{uuc}$ (m/s)	Error (m/s)	$U$ (k=2) (m/s)
0.984	24.10	24.00	0.7	-0.3	0.16
2.029	23.98	24.00	1.8	-0.3	0.16
3.044	23.96	24.00	2.9	-0.2	0.19
4.136	24.20	24.00	3.8	-0.3	0.20
5.00	23.80	24.00	4.8	-0.2	0.21
5.98	24.24	24.00	5.8	-0.2	0.17
7.05	23.90	24.00	6.9	-0.2	0.19
8.19	24.14	24.00	8.0	-0.2	0.19
9.09	23.88	24.00	8.9	-0.2	0.20
10.09	23.88	24.00	9.8	-0.2	0.19
11.16	23.74	24.00	11.0	-0.2	0.23
12.13	23.82	24.00	12.0	-0.2	0.24
13.19	23.70	24.00	13.0	-0.2	0.22
14.26	23.66	24.00	14.0	-0.3	0.28
15.24	23.66	24.00	14.8	-0.3	0.23
16.30	23.70	24.00	16.0	-0.3	0.23

## Remarks:

<sup>1</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>2</sup> Velocity of standard

<sup>3</sup> Velocity of Unit Under Calibration

## PHOTO OF CALIBRATION SET-UP



Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to editing geometry.



JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.  
63/14-15, 67/35-36  
Petchkasem 7, 7/1, Rd. Wattana, Bangkok, Thailand 10500 (Thailand)  
Tel: +6688888812  
Mobile: +6688399543  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TIS-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

Certificate Number

CL-018-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

## MEASUREMENT ITEM

## MANUFACTURER

## MODEL/TYPE

## SERIAL NUMBER

## ID NUMBER

## CONDITION AS-RECEIVED

## CUSTOMER

## RECEIVED DATE

## MEASUREMENT DATE

## ISSUE DATE

## ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure :  $1010 \pm 10$  hPa

## PLACE OF CALIBRATION

## CALIBRATION CONDITION

## Preconditioning

## Measurement Condition

## TABULATION OF RESULTS:

The table on next page give the measured values.

## Calibrated by:

☒ Mr. Sorawit Thachalad  
☐ Miss Jitragorn Lertsuamphol



## Approved signatory:

Mr. Parinya Booncharoen  
Calibration Department Manager

## Remarks:

<sup>1</sup> Nozzle cross-section area of the wind tunnel

<sup>2</sup> Projected cross-section area of the tested object include mounting pipe

<sup>3</sup> Diameter of mounting pipe

<sup>4</sup> Ratio  $^{1/3}$  to  $^{1/4}$

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number

CL-018-66

Page 2 of 2 Pages

MEASUREMENT RESULTS<sup>1</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D'_{std}$ Degree (°)	$D'_{uuc}$ Degree (°)	Error Degree (°)	$U$ (k=2) Degree (°)
	0.000	0	0	0.58
	45.000	41	-4	0.58
	90.001	87	-3	0.74
4.99	135.000	133	-2	0.74
	180.000	180	0	0.74
	225.000	227	2	0.68
	270.000	273	3	0.68
	315.000	318	3	0.74

## Remarks:

<sup>1</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>2</sup> Direction of standard

<sup>3</sup> Direction of Unit Under Calibration



\*\*\*End of Certificate of Calibration\*\*\*



JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.  
63/14-15, 67/35-36  
Petchkasem 7, 7/1, Rd. Wattana, Bangkok, Thailand 10500 (Thailand)  
Tel: +6688888812  
Mobile: +6688399543  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TIS-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

REVIEW BY: *Parinya Booncharoen*  
APPROVED BY: *Parinya Booncharoen*  
NEXT CAL DATE: 10/8/24

Certificate Number

CL-021-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

## MEASUREMENT ITEM

## MANUFACTURER

## MODEL/TYPE

## SERIAL NUMBER

## ID NUMBER

## CONDITION AS-RECEIVED

## CUSTOMER

## RECEIVED DATE

## MEASUREMENT DATE

## ISSUE DATE

## ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure :  $1010 \pm 10$  hPa

## PLACE OF CALIBRATION

## CALIBRATION CONDITIONS

## Preconditioning

## Measurement Condition

## TABULATION OF RESULTS:

The table on next page give the measured values.

## Calibrated by:

☒ Mr. Sorawit Thachalad  
☐ Miss Jitragorn Lertsuamphol



## Approved signatory:

Mr. Parinya Booncharoen  
Calibration Department Manager

## Remarks:

<sup>1</sup> Nozzle cross-section area of the wind tunnel

<sup>2</sup> Projected cross-section area of the tested object include mounting pipe

<sup>3</sup> Diameter of mounting pipe

<sup>4</sup> Ratio  $^{1/3}$  to  $^{1/4}$

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY



Certificate Number

CL-021-66

Page 2 of 2 Pages

MEASUREMENT RESULTS<sup>1</sup>

The cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

$V_{std}$ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$V_{uuc}$ (m/s)	Error (m/s)	$U$ (k=2) (m/s)
0.985	24.10	24.10	0.8	-0.2	0.36
2.033	24.10	24.10	1.9	-0.1	0.16
3.040	23.94	24.10	3.0	-0.1	0.23
4.134	24.10	24.10	4.0	-0.1	0.20
4.99	23.92	24.10	4.9	-0.1	0.44
5.98	24.10	24.10	6.0	0.0	0.18
7.05	23.90	24.10	7.0	-0.1	0.36
8.19	24.06	24.10	8.2	0.0	0.26
9.09	23.84	24.10	9.1	0.0	0.24
10.09	23.92	24.10	10.1	0.0	0.28
11.15	23.80	24.10	11.1	0.0	0.45
12.14	23.80	24.10	12.2	0.0	0.31
13.19	23.80	24.10	13.2	0.0	0.47
14.26	23.74	24.10	14.2	0.0	0.42
15.25	23.78	24.10	15.1	-0.1	0.66
16.28	23.70	24.10	16.3	0.0	0.56

## Remark:

<sup>1</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>2</sup> Velocity of standard

<sup>3</sup> Velocity of Unit Under Calibration

## PHOTO OF CALIBRATION SET-UP



Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging accuracy.



JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.  
62/54-15, 67/95-96  
Petchaburi 7, 7/1, Rd. Wutthaphong, Bangkok, 10250 (Thailand)  
Tel: +6628888812  
Mobile: +66833999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TIS-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

Certificate Number

CL-019-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM : Wind Direction Sensor  
MANUFACTURER : Novolynx  
MODEL/TYPE : Sensor: WS-02P  
Data logger: 200-WS-25L8  
SERIAL NUMBER : Sensor: -  
Data logger: AS376  
ID NUMBER : RYG\_FS0414  
CONDITION AS-RECEIVED : Used Item  
CUSTOMER : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE : 27 Jan 2023  
MEASUREMENT DATE : 10 Feb 2023  
ISSUE DATE : 10 Feb 2023

## ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure : 1010.1 hPa

## PLACE OF CALIBRATION

: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

## CALIBRATION CONDITION

: Wind tunnel cross-section area<sup>1</sup> : 900 cm<sup>2</sup>  
Win direction frontal area<sup>2</sup> : 129 cm<sup>2</sup>  
Diameter of mounting pipe<sup>3</sup> : - mm  
Blockage ratio of test object<sup>4</sup> : 0.143 [-]

## Preconditioning

: 24 hours at ambient conditions.

## Measurement Condition

: The average values during measurement are (24.0)°C, (49.0) %RH and (1014.1) hPa.

## TABULATION OF RESULTS:

The table on next page give the measured values.

## Calibrated by:

☒ Mr. Sorawit Thacholad  
☐ Miss Jitragorn Lertsomphol



## Approved signatory:

Mr. Parinya Booncharom  
Calibration Department Manager

## Remark:

<sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio "a" to "b"

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number

CL-019-66

Page 2 of 2 Pages

MEASUREMENT RESULTS<sup>1</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D'_{std}$ Degree (°)	$D'_{uuc}$ Degree (°)	Error Degree (°)	$U$ (k=2) Degree (°)
	0.000	0	0	0.59
	45.000	41	-4	0.58
	90.000	87	-3	0.58
	135.001	132	-3	0.68
4.99	180.000	179	-1	0.74
	225.000	227	2	0.91
	270.001	273	3	0.58
	315.000	318	3	0.74

## Remark:

<sup>1</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>2</sup> Direction of standard

<sup>3</sup> Direction of Unit Under Calibration



\*\*\*End of Certificate of Calibration\*\*\*

SITHIPORN ASSOCIATES CO., LTD.  
CALIBRATION LABORATORY

451-451/1 Sithiporn Road, Bangbunru, Bangkok, Bangkok, 10700 Thailand  
Tel: +66 2433 8331 Email: calibration@sithiporn.com

SITHIPORN ASSOCIATES



Cert. No.: ACC24008  
Pages : 1 of 3

## Calibration Certificate

Equipment : SOUND CALIBRATOR  
Manufacturer : RION  
Model : NC-75  
Serial No.: 35002736  
ID No.: RYG\_FS0496

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

Location :  
Ambient Temperature : (  $23.0 \pm 3$  ) °C  
Pressure : (  $101.3 \pm 3$  ) kPa  
Relative Humidity : (  $50.0 \pm 20$  ) %

Received Date : 19 JANUARY 2024  
Calibration Date : 26 JANUARY 2024  
Date of Issue : 29 JANUARY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :

( Thanakul Petchurni )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

**SITHIPORN ASSOCIATES CO., LTD.**  
**CALIBRATION LABORATORY**

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email: calibration@sithiporn.com



Cert. No. : ACC24008  
Job No. : VC67AC0058  
Pages : 2 of 3

Calibration Procedure : CP-AC-03

**Calibration Method :**

This equipment was calibrated by follow on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

**Condition of this result of calibration :**

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL_BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL_BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL_BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

*T. Petchur*

**SITHIPORN ASSOCIATES CO., LTD.**  
**CALIBRATION LABORATORY**

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email: calibration@sithiporn.com



Cert. No. : ACC24008  
Job No. : VC67AC0058  
Pages : 3 of 3

**Result of calibration :**

**1. Sound pressure level**

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	93.98	-0.02	0.14	0.40

**2. Frequency**

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ( % )	Uncertainty ( % )	Acceptance limit ( % )
1000	1000.0	0.0	0.1	1.0

**3. Total distortion**

Measured value ( % )	Uncertainty ( % )	Acceptance limit ( % )
0.83	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

*T. Petchur*

**SITHIPORN ASSOCIATES CO., LTD.**  
**CALIBRATION LABORATORY**

451-451/1 Sirinthorn Rd, Bangbunru, Bangplud Bangkok 10700 THAILAND  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



Cert. No. : ACL23325  
Pages : 1 of 8

**Calibration Certificate**

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 01073423 / 169513 / 73684  
**ID No.:** RYG\_FS0386

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0 ± 3 ) °C  
**Pressure :** ( 101.3 ± 3 ) kPa  
**Relative Humidity :** ( 50.0 ± 20 ) %

**Received Date :** 11 OCTOBER 2023  
**Calibration Date :** 19-20 OCTOBER 2023  
**Date of Issue :** 24 OCTOBER 2023

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*T. Petchur*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

**SITHIPORN ASSOCIATES CO., LTD.**  
**CALIBRATION LABORATORY**

**Continuation of Calibration Certificate**

Cert. No. : ACL23325  
Job No. : VC67AC0011  
Pages : 2 of 8

**Calibration Procedure :** CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL_BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL_BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL_BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

*T. Petchur*



## Continuation of Calibration Certificate

Cert. No. : ACL23325  
Job No. : VC67AC0011  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

QF-TS12-04-04-020664

P.T.M.

## Continuation of Calibration Certificate

Cert. No. : ACL23325  
Job No. : VC67AC0011  
Pages : 4 of 8

## Result of calibration :

## 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

## 2. Self-generated noise

## 2.1 Normal test

Measured Value ( dB )
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device:

Frequency Weighting	Measured value ( dB )
A - weight	13.1
C - weight	18.8
Flat	24.6

## 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.6	1.7	1.6	±5.0

QF-TS12-04-04-020664

P.T.M.

## Continuation of Calibration Certificate

Cert. No. : ACL23325  
Job No. : VC67AC0011  
Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

P.T.M.

## Continuation of Calibration Certificate

Cert. No. : ACL23325  
Job No. : VC67AC0011  
Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.8	-0.2	± 1.1

QF-TS12-04-04-020664

P.T.M.



## Continuation of Calibration Certificate

Cert. No. : ACL23325  
Job No. : VC67AC0011  
Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L <sub>peak</sub> (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.1	-0.3	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

T. Petchurai

## Continuation of Calibration Certificate

Cert. No. : ACL23325  
Job No. : VC67AC0011  
Pages : 8 of 8

## 11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	0.0	±1.5
89.6	89.6		

## 12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A-weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchurai

SITHIPORN ASSOCIATES CO., LTD.  
CALIBRATION LABORATORY451-451/1 Sirinthorn Road, Bangbuemue, Bangpuad, Bangkok, 10700 Thailand  
Tel: +66 2433 8331 Email: calibration@sithiporn.comSITHIPORN  
associatesCert. No. : ACL24007  
Pages : 1 of 8

## Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RION  
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24  
Serial No. : 01173609 / 172170 / 74021  
ID No. : RYG\_FS0388

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

Location : -  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 19 DECEMBER 2023  
Calibration Date : 05-08 JANUARY 2024  
Date of Issue : 09 JANUARY 2024



Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchurai  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN ASSOCIATES CO., LTD.  
CALIBRATION LABORATORY451-451/1 Sirinthorn Road, Bangbuemue, Bangpuad, Bangkok, 10700 Thailand  
Tel: +66 2433 8331 Email: calibration@sithiporn.comSITHIPORN  
associatesCert. No. : ACL24007  
Job No. : VC67AC0044  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.  
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).  
3.2 Thailand Institute of Scientific and Technological Research (TISTR).

T. Petchurai



Cert. No. : ACL24007  
Job No. : VC67AC0044  
Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Uncertainty	Maximum-permitted
	(dB)	uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

*T. Petch*

Cert. No. : ACL24007  
Job No. : VC67AC0044  
Pages : 4 of 8

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise**

**2.1 Normal test**

Measured Value ( dB )
15.1

**2.2 The microphone of the sound level meter was replaced by electrical signal input device.**

Frequency Weighting	Measured value ( dB )
A - weight	13.4
C - weight	19.9
Flat	25.3

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.8	0.9	0.9	± 5.0

*T. Petch*

Cert. No. : ACL24007  
Job No. : VC67AC0044  
Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**

**5.1 Frequency weightings at 1 kHz**

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

**5.2 Time weighting at 1 kHz**

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

*T. Petch*

Cert. No. : ACL24007  
Job No. : VC67AC0044  
Pages : 6 of 8

**7. Level linearity on the reference level range**

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

*T. Petch*



Cert. No. : ACL24007  
Job No. : VC67AC0044  
Pages : 7 of 8

## 8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

## 9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

## 10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L <sub>peak</sub> (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

T. Peteh

Cert. No. : ACL24007  
Job No. : VC67AC0044  
Pages : 8 of 8

## 11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

T. Peteh

TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
5344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484

## Certificate of Calibration

Certificate No. : 23E3924  
Page : 1 of 2Equipment : pH Meter  
Manufacturer: Mettler Toledo  
Model : SevenExcellence  
Serial No.: B834291445  
ID No.: RYG\_EN0152Condition As-Received: Used Item  
Received Date: 08 December 2023  
Calibration Date: 14 December 2023Reference: 2312-0151DSC  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 10 ) %  
Submitted by: ALS Laboratory Group (Thailand) Co., Ltd. Rayong Branch  
616/10 Moo 5, T.Maenam Khu, A.Puakdaeng,  
Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 according to EURAMET cg-15.

## Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Multi-Product Calibrator	5502A	2435802	EE-0041-23	26 Apr 2024

2. This result of calibration was made on requested at the point specified by customer.

3. The certificate is valid only to the item calibrated on date and place of calibration.

4. This Certification is traceable to the International System of Unit maintained through:-

- National Institute of Metrology Thailand (NIMT)

REVIEW BY Ni. Banwit  
APPROVED BY D. Sae  
NEXT CAL. DATE 14/12/24Calibrated by : Napachanok Prasomsosiri  
Issue Date : 15 December 2023Approved Signatory :  
[ ] Phalinee Pratsapaipal  
[x] Nuntawat Khanchai  
[ ] Pongsagorn Boonyaporn

B 0331106

Cert. No. : 23E3924  
Page: 2 of 2

Result of calibration :- (\*) Without adjustment ( ) After adjustment

Function: DC voltage measurement	Range: 2000 mV	Error	Uncertainty
Standard Value (mV)	UUC* Reading (mV)	(mV)	(± μV)
-200.0000	-199.9	0.1	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	50.0	0.0	61
100.0000	100.0	0.0	63
150.0000	150.0	0.0	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95 %

UUC\*= Unit Under Calibration.

-00-

a 1193422





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert.No.: 23CH1574  
Page.: 1 of 3

## Certificate of Calibration

Equipment : pH Meter  
Manufacturer : Mettler Toledo  
Model : SevenExcellence  
Serial No. : B834291445  
ID No. : RYG\_EN0152  
Condition As-Received: Used Item  
Received Date : 08 December 2023  
Calibration Date : 15 December 2023  
Reference : 2312-0151DSC-3  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch  
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,  
Rayong 21140, Thailand

Ambient Temperature : (25 ± 2.5) °C  
Relative Humidity : (50 ± 15) %  
Calibration Procedure : In-house method :  
- CP-CH5 by direct measurement with standard  
voltage calibrator and direct measurement with  
certified reference material (CRM)  
- CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lerngagrakul

Approved by :   
Approved Signatory

( ) Salthip Meangmai  
( ) Warakorn Lerngagrakul  
(x) Ponpan Palpim

Issue Date : 19 December 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services & Equipment Calibration and Testing Services.

A 0061696



Cert.No.: 23CH1574  
Page.: 2 of 3

### Condition of this calibration result

1. Reference Standard Instrument : -

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4962054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-  
- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	913598	14 July 2025
pH 6.986	CPA chem	931959	01 Oct 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

### Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor k
			mV	pH		
pH Meter S/N.: B834291445	4.000	177.48	177.3	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

a 1193852



Cert.No.: 23CH1574  
Page.: 3 of 3

### Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement ( ± )	Coverage factor k
pH Electrode S/N.: 3225368	4.008	4.013	184.1	0.0045	2.00
	6.986	6.998	8.7	0.0084	2.00
	9.997	10.002	-164.7	0.0088	2.11

### Function : Temperature Measurement

(\*) Without adjustment

This equipment was connected with Temperature Probe:

- Model : InLab®Expert Pro-ISM

- Serial No. : 3225368

Dimension of probe:

- Length : 120 mm

- Diameter : 12 mm

- Immersion Depth : 100 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement ( ± °C )	Coverage factor k
25.0	25.003	24.3	-0.703	0.13	2.00

Remark : - UUC\* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

a 1193851



## Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T. Banpa, A. Kaengkhoh, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 8851 +668 8247 2380

Website : www.scieco.co.th

E-Mail : calibrate@scg.com



Certificate No. T230116

Page 1 of 4

## Certificate of Calibration

Equipment : Chumbar ( Cooling Room )

Manufacturer : MODULAR

Model : IREVCOHCOO

Serial No. : C00351459

Customer Code : RYG\_EN0184

ID No. : T1939A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd. ( Rayong Branch)

616/10 Moo 5 T.Maenam Khu,

A.Pluakdaeng, Rayong 21140

Customer Location : Laboratory

Date of Receipt : 23 January 2023

Calibrated By : Atiphong Rongrat ( Technician )

Approved By : / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 07 FEB 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FSM-L101821908-4

Certificate No. T230116

Page 2 of 4

## Calibration Report

Equipment : Chamber ( Cooling Room )  
Date of Calibration : 25 January 2023  
Environment : Temperature : 23.4-24.9 °C  
Line Voltage : 221.4-230.2 V  
Relative Humidity : 55 - 65 %RH

### Condition of this results of calibration :

1. This equipment was calibrated by insert 16 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 ( based on ASTM E145-94 ( Reapproved 2001 ) and AS2853-1986 ) .

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

### 2. Reference Standard Instrument

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN141-TN150	T222123	5 October 2023
TC	TYPE T	TN151-TN160	T222123	5 October 2023
DATA LOGGER	34970A	T150	T222123	5 October 2023

### 3. This certificate is traceable to :

National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244 )

### 4. Condition of calibrated item : good

#### Equipment Description :

Time Constant : 1 Hour - Minute At 3 °C  
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available

### 5. Adjustment :

( X ) without adjustment ( ) after adjustment


Approved By: *[Signature]*

FORM 15 (17/15-01-01)

Certificate No. T230116

Page 3 of 4

## Calibration Report

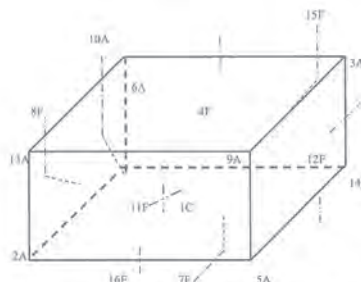

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C = TN141	12F = TN152
2A = TN142	13A = TN153
3A = TN143	14A = TN154
4F = TN144	15F = TN155
5A = TN145	16E = TN156
6A = TN146	
7F = TN147	
8F = TN148	
9A = TN149	
10A = TN150	
11F = TN151	

Approved By: *[Signature]*

FORM 15 (17/15-01-01)

Certificate No. T230116

Page 4 of 4

## Calibration Report

### Measurement Results

	Average Standard Reading at each position (°C)											
Calibration Point	TN141	TN142	TN143	TN144	TN145	TN146	TN147	TN148	TN149	TN150	TN151	TN152
3.0	3.03	3.16	3.15	3.19	3.45	3.47	3.21	3.35	3.54	3.45	3.24	3.34
	TN153	TN154	TN155	TN156								
	3.28	3.22	3.28	3.21								

Chamber ( Cooling Room )			Temperature Distribution			
Setting ( °C )	Reading ( °C )		Stability ( °C )	Uniformity ( °C )	Uncertainty ( ± °C )	Coverage Factor k
	Min, Max	Average				
3.0	2.8, 4.1	3.5	1.20	1.20	1.90	2.07

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By: *[Signature]*

FORM 15 (17/15-01-01)

Cert.No.: 23TW168  
Page: 1 of 2

## Certificate of Testing

Equipment : DO Meter  
Manufacturer : YSI  
Model : 5000-115V  
Serial No. : 15E102796  
ID No. : RYG\_EN0032  
Received Date : 21 July 2023  
Test Date : 24 July 2023  
Reference : 2307-0713DSC-1  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
Rayong Branch  
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,  
Rayong 21140, Thailand

Laboratory Condition : Temperature ( 25 ± 5 ) °C  
Humidity ( 50 ± 20 ) %  
Test Procedure : In - house method : CP-CH9  
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean  
Approved by : *[Signature]*  
Approved Signatory

( ) Malee Butkruea  
(✓) Saithip Meangmai  
( ) Warakorn Lemgratrakul

Issue Date : 26 July 2023

8 0320211





Cert.No.: 23TW168  
Page.: 2 of 2

#### Condition of this result of calibration

##### 1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

##### 2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 15E100464

Titration Method (Azide Modification Method)	DO Meter Reading	Standard Deviation
(mg/L)	(mg/L)	(mg/L)
8.18	8.17	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency. The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory.

-000-

Swit

a 1172155



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23LM125  
Page.: 1 of 2

## Certificate of Calibration

Equipment : DO Meter with Sensor  
Manufacturer : YSI  
Model : 5000-115V  
Serial No. : 15E102796  
ID No. : RYG\_EN0032  
Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.  
Rayong Branch  
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng,  
Rayong 21140 Thailand  
Location : TPA On Site Calibration Laboratory  
Received Order : 25 July 2023  
Calibrated Date : 27 July 2023  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
AC Line Voltage : ( 220 ± 22 ) V

Calibrated by : Preecha Hlahib

Approved by :   
Approved Signatory

( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
(✓) Suwit Imjai

Issue Date : 31 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

A 0053616



Equipment : DO Meter with Sensor  
Condition As-Received : Used Item  
Reference : 2307-0713DSC-2

Cert. No.: 23LM125  
Page.: 2 of 2

#### Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer ( IPRT ) into Temperature Bath.

The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

##### 1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	2211285	TPA	21 Oct 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association ( Thailand - Japan )

Result of Calibration :- ( \* ) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 1228475367

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
20.00	100	20.011	19.91	-0.101	0.15	2.00

UUC\* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

Swit

a 1159515



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM962  
Page : 1 of 3

## Certificate of Calibration

Equipment : Low Temp. Incubator  
Manufacturer : Memmert  
Model : IPP750  
Serial No. : V818.0084  
ID No. : RYG\_EN0154  
Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.  
(Rayong Branch)  
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand  
Location : BOD Room  
Received Order : 29 May 2023  
Calibration Date : 29 May 2023  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %

Calibrated by : Man Pattanapongpaiboon

Approved by :   
Approved Signatory

( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
(✓) Suwit Imjai

Issue Date : 7 June 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

A 0054967





Equipment : Low Temp. Incubator  
Condition As-Received : Used Item  
Reference : 2305-0898OC-2

Cert. No.: 23TM962  
Page : 2 of 3

#### Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

##### 1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013711	22LM93	02 Jul 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Fresh air setting : Close



#### Probe Installation Details :

Dimension of Chamber :	
a = 10 cm	D = 0.60 m
b = 10 cm	W = 1.0 m
c = 10 cm	H = 1.2 m
	Capacity = 0.75 m <sup>3</sup>

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	23	23
REL.Humid. ( % )	54	56
AC Supply ( Volt )	223	222

Position :	Ref. Std. ID No.:
1	18-18RTD-01
2	18-18RTD-02
3	18-18RTD-03
4	18-18RTD-04
5	18-18RTD-05
6	18-18RTD-10
7	18-18RTD-07
8	22-18RTD-08
9 (ref.)	18-18RTD-09

a 1165130



Equipment : Low Temp. Incubator  
Condition As-Received : Used Item  
Reference : 2305-0898OC-2  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 23TM962  
Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor k
20.0	20.0	20.0	0.019	0.72	1.0	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty ( ± °C )
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.547	19.780	19.487	19.529	19.408	20.139	20.112	20.406	20.116	0.30

Average\* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC\* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

a 1165129




TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CG3704  
Page.: 1 of 2

## Certificate of Calibration

Equipment : Burette  
Capacity : 50 mL  
Serial No. : -  
ID. No. : RYG\_EN0216  
Manufacturer : Witeg  
Made in : Germany  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
Rayong Branch  
616/10 Moo 5, T.Maenam Khu  
A.Pluakdaeng, Rayong 21140 Thailand  
Ambient Temperature : (20 ± 2.5) °C  
Relative Humidity : (50 ± 10) %  
Barometric Pressure : 756 mmHg  
Calibration Procedure : ASTM E 542 - 01  
Calibrated by : Srisuda Khamtha



Approved by :  
( ) Ponpan Paipim  
( ) Srisuda Khamtha  
( ) Sa-ngeunkam Wongsa

Issue Date : 28 September 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

A 0058881



Equipment : Burette  
Received Date : 19 September 2023  
Condition As-Received : Used Item  
Calibration Date : 25 September 2023  
Reference : 2309-0635DSC-31

Cert.No.: 23CG3704  
Page.: 2 of 2

#### Condition of this result of calibration

##### 1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	MS204TS	C226356983	140RC010	TH2068-012	METTLER	29 Sep 2023
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	1594592	140EC010	23I158	TPA	12 Feb 2024

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. True value is converted to true volume at the standard temperature of 20 °C

#### Calibration result :

Nominal capacity ( mL )	Reading ( mL )	Uncertainty ( ± mL )	k Factor
10	10.0224	0.0082	2.00
20	20.0064	0.0085	2.00
30	29.9931	0.0089	2.00
40	39.9910	0.0094	2.00
50	49.9806	0.010	2.00

Remark mL = cm<sup>3</sup>

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

a 1182477



Sartorius (Thailand) Co., Ltd.  
129 Rama 9 Road, Huaykwang, Bangkok 10310  
Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com



SARTORIUS



# Certificate of Calibration

Model Number : MSE224S-100-DU Certificate No. : 23BCI0112  
Description : Analytical Balance Issued Date : Friday, March 03, 2023  
Serial Number : 0026207038 Reference No. : 204833  
ID No. : RYG\_EN0002  
Manufacturer : Sartorius Page No. : 1 of 2

Customer Name : ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)  
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd. (Balance Room)  
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Calibrated By : Mr.Chonchai Inthana Calibration Procedure No. : This calibration was conducted by  
Calibration Date : Wednesday, March 01, 2023 Using in-house calibration procedure number (WI-003)  
Based on UKAS LAB 14 : 2019

Metrological data :  
Capacity : 220 g Readability : 0.0001 g  
Ambients Conditions:  
Temperature : 23.6 °C ± 5.0 °C  
Humidity : 60.0 % RH ± 10.0 % RH  
Pressure : ±  
Reasons for calibration:  
☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance ☐ Equipment Condition: ☒ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref : Lab 14  
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-362SD	Humidity/Barometer/Temp Lutron MHB-362SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.  
This certificate may not be reproduced other than in full, except with the prior written approval of the Verification Operation Division  
Sartorius (Thailand) Co., Ltd.  
SOP FM 33 03 February 2022  
Mr.chonchai inthana(Technical Manager)



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
5344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10251  
TEL: 0-2717-3000-21 FAX: 0-2719-9484



Cert. No.: 22TM1517  
Page : 1 of 3

## Certificate of Calibration

Equipment : Hot Air Oven  
Manufacturer : Memmert  
Model : UFE 500  
Serial No. : G511.1572  
ID No. : RYG\_EN0010  
Submitted by : ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)  
616/10 Moo 5 T. Maenam Khu,  
A. Pluakdaeng,  
Rayong 21140 Thailand  
Location : Oven Room  
Received Order : 20 October 2022  
Calibration Date : 20 October 2022  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
Calibrated by : Man Pattanapongpaiboon  
Approved by :  
( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
( ) Suwit Imjai  
Issue Date : 2 November 2022



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services : Equipment Calibration and Testing Services.

Sartorius (Thailand) Co., Ltd.  
129 Rama 9 Road, Huaykwang, Bangkok 10310  
Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

SARTORIUS

# Certificate of Calibration

Model Number : MSE224S-100-DU Certificate No. : 23BCI0112  
Description : Analytical Balance Issued Date : Friday, March 03, 2023  
Serial Number : 0026207038 Reference No. : 204833  
ID No. : RYG\_EN0002  
Manufacturer : Sartorius Page No. : 2 of 2

## Calibration Results : Without Adjustment

Repeatability		Eccentricity (Off-center loading error)	
The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.		The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).	
Nominal Value : (Low Load)	20,0000 199,9999	Nominal value :	100 g
20 g	20,0000 200,0000	Tolerance	0.0004 g
Tolerance	0.0001 g		
Nominal Value : (High Load)	20,0000 199,9999		
200 g	19,9999 200,0000		
Tolerance	0.0001 g		
Standard Deviation	0.00003 0.00005		

Linearity				
The linearity, also called linearity error, describes the deviation of the characteristic curve of a weighing instrument from the linear slope.				
Tolerance	0.0002 g			
Nominal Value	Conventional Mass Value	Displayed Value	Deviation	Uncertainty
(g)	(g)	(g)	(g)	(g)
0.01	0.0100	0.0100	0.0000	0.00014
0.05	0.0500	0.0500	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
0.5	0.5000	0.5000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0001	0.0001	0.00014
20	20.0000	20.0000	0.0000	0.00024
50	50.0000	50.0000	0.0000	0.00015
100	100.0000	99.9999	-0.0001	0.00019
200	200.0000	200.0000	0.0000	0.00032
End of Report				

SOP FM 33 03 February 2022



Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2210-0376OC-2  
Cert. No.: 22TM1517  
Page : 2 of 3

Procedure Used :-  
Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

### Condition of this result of calibration

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34972A	MY49023932	22LM97	29 Jul 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Fresh air setting : Close



Probe Installation Details : Dimension of Chamber :  
a = 5.0 cm D = 0.40 m  
b = 5.0 cm W = 0.56 m  
c = 5.0 cm H = 0.48 m  
Capacity = 0.11 m³

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	25	25
REL.Humid. ( % )	54	59
AC Supply ( Volt )	223	225

Ref. Std. ID No.: @ Calibration Point		
Position :	( 180 ) °C	( 104 ) °C
1	21-16TC-01	20-16RTD-01
2	21-16TC-02	20-16RTD-02
3	21-16TC-03	20-16RTD-03
4	21-16TC-04	20-16RTD-04
5	21-16TC-05	22-16RTD-05
6	21-16TC-06	20-16RTD-06
7	21-16TC-07	20-16RTD-07
8	21-16TC-08	22-16RTD-08
9 (ref.)	21-16TC-09	22-16RTD-09





Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2210-0376OC-2  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Close

Cert. No.: 22TM1517  
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
104.0	104.0	104.0	0.076	0.52	0.60	0.42	2
180.0	180.0	180.0	0.13	0.86	1.2	1.1	2

Calibration Point (°C)	Measured Temperature (°C)								
	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
104.0	103.768	103.734	103.723	103.800	104.215	104.131	104.132	103.740	103.747
180.0	179.723	179.359	179.439	179.489	180.361	180.114	180.131	180.243	179.605

Average\* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation

UUC\* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

Malu .

a 1132465



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH1088  
Page: 1 of 2

## Certificate of Calibration

Equipment : Conductivity Meter  
Manufacturer : Mettler Toledo  
Model : S230  
Serial No. : B241407147  
ID No. : RYG\_EN0029  
Condition As-Received : Used Item  
Received Date : 01 September 2023

Calibration Date : 04 September 2023  
Reference : 2309-0010DSC-7  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch  
616/10 Moo 5, T. Maenam Khu,  
A. Pluakdaeng, Rayong 21140, Thailand

Ambient Temperature : (25 ± 2.5) °C  
Relative Humidity : (50 ± 15) %  
Calibration Procedure : In -house method :  
- CP-CH6 : based on direct measurement by  
using certified reference material (CRM)

Calibrated by : Warakorn Lernagatrakul

Approved by :   
Approved Signatory

( ✓ ) Sathip Meangmai  
( ) Warakorn Lernagatrakul  
( ) Ponpan Paipim

Issue Date : 7 September 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment, Calibration and Testing Services.

A 0058059



Cert.No.: 23CH1088  
Page: 2 of 2

### Condition of this result of calibration

1. Reference Standard Instrument :-  
Instrument Serial No. ID No. Certificate No. Due date  
1) Thermometer 9549224 130RC003 231435 10 Apr 2024  
- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-  
- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI  
through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
84.000 µS/cm	CPA Chem	885120	28 Mar 2024
1413.0 µS/cm	CPA Chem	913596	14 July 2024
12.880 mS/cm	CPA Chem	885123	28 Mar 2024

- Control Conductivity calibration solution temperature by Water bath (25±0.1) °C  
3. This certificate is valid only to the item calibrated on date and place of calibration.

### Calibration results

Function : Conductivity Measurement

( \* ) After Adjustment at 1413.0 µS/cm

Conductivity Electrode Serial No.: 5823251000

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor k
84.000 µS/cm	83.8 µS/cm	85.3 µS/cm	0.62 µS/cm	2.00
1413.0 µS/cm	1388 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.880 mS/cm	12.41 mS/cm	12.63 mS/cm	0.086 mS/cm	2.00

Remark - UUC\* = Unit Under Calibration  
- Cell constant = 0.545371 cm<sup>-1</sup>

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

Sathip

a 1178950



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1492  
Page : 1 of 3

## Certificate of Calibration

Equipment : Hot Air Oven  
Manufacturer : Memmert  
Model : UM 400  
Serial No. : b495.0899  
ID No. : RYG\_EN0006

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)  
616/10 Moo 5, T. Maenam Khu,  
A. Pluakdaeng,  
Rayong 21140, Thailand  
Location : Oven Room

Received Order : 20 October 2022  
Calibration Date : 20 October 2022  
Ambient Temperature : (26 ± 10) °C  
Relative Humidity : (50 ± 30) %

Calibrated by : Preecha Hiahib

Approved by :   
Approved Signatory

( ✓ ) Porthippa Tameyakul  
( ✓ ) Malee Bulkruea  
( ) Suwit Imjai

Issue Date : 2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment, Calibration and Testing Services.

A 0046905





Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2210-0376OC-1

Cert. No.: 22TM1492  
Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

**1. Reference standard instrument:-**


Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022

2. This certificate is valid only to the item calibrated on date and place of calibration.  
3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close



**Probe Installation Details :**

a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm

**Dimension of Chamber :**

D = 0.33 m  
W = 0.40 m  
H = 0.40 m  
Capacity = 0.053 m<sup>3</sup>

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	28	29
REL.Humid. ( % )	43	47
AC Supply ( Volt )	220	221

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	18-10RTD-06
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09

a 1132473



Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2210-0376OC-1

Cert. No.: 22TM1492  
Page : 3 of 3

**Result of Calibration :-**

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Uncertainty ( ± °C )	Coverage Factor k
70.0	70.0	70.0	0.079	0.47	0.77	0.42	2

Measured Temperature ( °C )									
Calibration Point ( °C )	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
70.0	70.262	69.995	70.079	70.177	70.664	70.039	70.688	70.149	70.328

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.  
**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.  
**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

a 1132472

RYG\_EN0061



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL: 0-2717-3000-27 FAX: 0-2719-9484



Cert. No.: 22TM1491  
Page : 1 of 3

**Certificate of Calibration**

**Equipment :** Water Bath

**Manufacturer :** Memmert

**Model :** WNB22

**Serial No. :** L513.0648

**ID No. :** RYG\_EN0061

**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)  
616/10 Moo 5, T. Maenam Khu,  
A. Pluakdaeng,  
Rayong 21140, Thailand  
Wet Chemistry Lab

**Location :** Wet Chemistry Lab

**Received Order :** 20 October 2022

**Calibration Date :** 20 October 2022

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Preecha Hlahib

**Approved by :**   
Approved Signatory

( ) Pormthippa Tameyakul  
( / ) Mailee Butkrues  
( ) Suwit Imjai

**Issue Date :** 2 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0046906



Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2210-0376OC-4

Cert. No.: 22TM1491  
Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

**1. Reference standard instrument:-**

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44035217	21LM30	23 Dec 2022


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

	Environmental		AC Voltage Supply ( Volt )
	( °C )	( %R.H. )	
Beginning of Calibration	24	53	222
Finished of Calibration	24	50	221



Front

Position :	Ref. Std. S/N.:
1	N37P300726
2	N37P300727
3	N37P300728
4	N37P300729
5(ref.)	N37P300730

a 1132471





Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2210-0376OC-4  
Result of Calibration : ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 22TM1491  
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)				
			Position				
			1	2	3	4	5 (ref.)
85.0	85.0	85.0	84.527	84.563	84.628	84.516	84.580

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Uncertainty (± °C)	Coverage Factor k
85.0	0.12	0.081	0.18	2

Average\* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC\* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o-o-

Malu

a 1132470



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 23TW256  
Page: 1 of 2

## Certificate of Testing

Equipment : DO Meter  
Manufacturer : Mettler Toledo  
Model : Seven2Go S9  
Serial No. : B905192347  
ID No. : RYG\_FS0529  
Received Date : 04 December 2023  
Test Date : 06 December 2023  
Reference : 2312-0070DSC-3  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
Rayong Branch  
616/10 Moo 5, T.Maenam Khu, A.Piuaekdaeng,  
Rayong 21140, Thailand

Laboratory Condition : Temperature ( 25 ± 5 ) °C  
Humidity ( 50 ± 20 ) %  
Test Procedure : In - house method : CP-CH9  
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by :   
Approved Signatory

( ✓ ) Saithip Meangmai  
( ) Warakorn Lemgagtrakul  
( ) Ponpan Paipim

Issue Date : 8 December 2023

REVIEW BY   
APPROVED BY   
NEXT CAL DATE 06/12/24

B 0330512



Cert.No.: 23TW256  
Page: 2 of 2

### Condition of this result of calibration

#### 1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1124013382	140RC006	23MM18	20 Feb 2024

#### 2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %  
Dissolved Oxygen Probe No.: 796488

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.26	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency. The environmental impact control and present to organization it may concerned intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o-o-

Saithip

a 1192691



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23LM198  
Page: 1 of 2

## Certificate of Calibration

Equipment : DO Meter with Sensor  
Manufacturer : Mettler Toledo  
Model : Seven2Go S9  
Serial No. : B905192347  
ID No. : RYG\_FS0529  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
Rayong Branch  
616/10 Moo 5 T. Maenam Khu, A. Piuaekdaeng,  
Rayong 21140 Thailand

Location : TPA On Site Calibration Laboratory

Received Order : 04 December 2023  
Calibrated Date : 08 December 2023  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
AC Line Voltage : ( 220 ± 22 ) V

Calibrated by : Khil Ruttanaprapachai

Approved by :   
Approved Signatory

( ) Pomthippa Tameyakul  
( ) Panpan Paipim  
( ✓ ) Suwit Imjai

Issue Date : 15 December 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3 - Equipment Calibration and Testing Services.

A 0061580





Equipment : DO Meter with Sensor  
 Condition As-Received : Used Item  
 Reference : 2312-0070DSC-5  
 Cert. No.: 23LM198  
 Page.: 2 of 2

Procedure Used :-  
 Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer ( IPRT ) into Temperature Bath.  
 The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

1. Reference standard Instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	A7B843	23124	TPA	04 Jan 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association ( Thailand - Japan )

Result of Calibration :- ( \* ) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 796488

Calibration Point ( °C )	Immersion Depth ( mm )	Standard Temperature ( °C )	UUC* Reading ( °C )	Error ( °C )	Uncertainty ( ± °C )	Coverage Factor k
20.0	100	20.002	20.1	0.098	0.16	2.00

UUC\* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

a 1193730

Agilent Technologies

Agilent Technologies (Thailand) Limited  
 U CHU LIANG BLDG. 22/F UNIT A.D  
 888 RAMA 4 ROAD, SILOM, BANGRAK  
 Bangkok 10500 Thailand  
 Tel: +662 637 6363  
 Fax: +662 632 4334  
 Email: ccc-smt@agilent.com  
 Website: www.agilent.com/thai

#### Customer Contact:

ALS Laboratory Group (Thailand) Co  
 Ltd  
 Head Office  
 104 Phatthanakan 40 Phatthanakan Rd  
 Khwaeng Phatthanakan Khet Suan  
 TAX ID : 0105540004859  
 Chanattagarn.lmichom@alsglobal.com  
 27603068

#### Invoice To:

ALS Laboratory Group (Thailand) Co  
 Ltd  
 Head Office  
 104 Phatthanakan 40 Phatthanakan Rd  
 Khwaeng Phatthanakan Khet Suan

#### SERVICE REPORT

Customer Purchase Order Number:	Customer Number:
70371813	70371813
Service Request:	Service Request Date:
Service Order:	Service Confirmation:
6006041263	6905338201

REVIEW BY Supakwan M.  
 APPROVED BY Savitri N.  
 NEXT CAL. DATE 15/06/2025

#### Delivery Site:

ALS Laboratory Group (Thailand) Co  
 Ltd  
 Head Office  
 104 Phatthanakan 40 Phatthanakan Rd  
 Khwaeng Phatthanakan Khet Suan

#### Location:

Room  
 Bldg  
 Lab  
 Dept

#### Direct Inquiries to:

Contact Name: Customer Contact Center  
 Contact E-mail: ccc-smt@agilent.com  
 Contact Telephone: +662 637 6363  
 Contact Fax: +662 632 4334

Products / Applications / Software / Services

Learn more about Agilent's Special Offers, Products, Services and our full range of laboratory productivity solutions optimized for your applications and workflows. Visit us at [www.agilent.com/thai](http://www.agilent.com/thai)

Agilent Technologies (Thailand) Limited, Head Office  
 U Chu Liang Bldg. 22/F Unit A.D  
 888 Rama 4 Road, Silom, Bangkok,  
 Bangkok 10500 Thailand  
 Tax ID : 0105540004859

Citibank P.A. Bangkok Branch  
 388 Interchange 21 Building, Sukhumvit Road, Khongroy Nuea  
 Sub-district, Wattana District, Bangkok 10110 Thailand  
 Acc. No: 012-4452-007  
 THB-Kueng Thai Bank PCL  
 Siam Square Bldg. 415/1-2 Rama 1 Rd, Pathumwan, BKK 10330  
 Thailand

ORIGINAL

Page 1 of 3

Service Confirmation Number: 6905338201  
 Service Confirmation Date: 12.12.2023

#### Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM-7700-E	ICPMS 7700 System Enhanced		ICP MS 7700 (HPIC)	
G1316A	1260 Thermostatted Column Compartment	DEACN12300	ICP MS 7700 (HPIC)	SYS-IM-7700-E
G1329B	1260 Standard Autosampler	DEAAC11098	ICP MS 7700 (HPIC)	SYS-IM-7700-E
G1311B	1260 Quaternary Pump	DEAB704380	ICP MS 7700 (HPIC)	SYS-IM-7700-E
G3281A	Agilent 7700x ICP-MS	JP12091612	ICP MS 7700 (HPIC)	SYS-IM-7700-E

#### Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EQC	Enterprise Operational Qualification	1.00	Agreement Entitlement: 100 % covered	12.12.2023	12.12.2023
1010	5185-5959	ICP-MS Checkout Solutions	1.00	Agreement Entitlement: 100 % covered		

#### Additional Information:

#### Service Information:

<b>Problem Description:</b> WU-00-IM/HPIC-7700-5001143313		
<b>Service Provided:</b> Perform IQ Hardware control test CSD Ilogon, Autosample, IBS, Auto tune, BG and Stability. After done the instrument BKK_EL0026 calibrated pass all.		
<b>Service Overview Code:</b> Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
<b>Reported Hours:</b> 8.0	<b>Travel Hours:</b> 1.0	
<b>Customer Field Service Representative Name:</b> Pantthap Kuraathalein	<b>Customer Field Service Representative Signature:</b> 	<b>Date:</b> 12 Dec 2023
<b>Customer Name:</b> Supakwan Mak	<b>Customer Signature:</b> 	<b>Date:</b> 12 Dec 2023
<b>Additional Comments:</b>		





## Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 1 of 6

### Certificate of Calibration

Equipment : HEATING BLOCK  
Manufacturer : Environmental Express  
Model : SC 196  
Serial No. : 6974CECW3285  
Customer Code : BKK\_EL0054  
ID No. : T5306A3  
Customer : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,  
Khet Suan Luang, Bangkok 10250  
Customer Location : Acid Digestion Lab  
Date of Receipt : 13 September 2023  
Calibrated By : Saneek Musikanwan ( Site Calibration Manager )  
Approved By : / Sujjar Naknakred ( Site Calibration Manager )  
Date of Issue : 26 SEP 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L12 109/30-05-57



## Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 2 of 6

### Calibration Report

Equipment : HEATING BLOCK  
Date of Calibration : 22 September 2023  
Environment : Temperature : 21.8-23.1 °C  
Line Voltage : 221.6-226.3 V  
Relative Humidity : 55 - 65 %RH

#### Condition of this results of calibration :

- This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20.  
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .
- Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN21-TN30	T230014	17 January 2024
TC	TYPE T	TN31-TN40	T230014	17 January 2024
DATA LOGGER	34970A	T151	T230014	17 January 2024
- This certificate is traceable to :  
National Institute of Metrology ( Thailand ) through Metrological Center ( NSC-TISI-TIS 17025 CALIBRATION 0244 )
- Condition of calibrated item : good  
Equipment Description :  
Time Constant : 2 Hour 20 Minute At 95 °C  
Fresh Air Damper : ☐ Open ☐ Min ☐ Medium ☐ Max  
☐ Close  
☒ Not Available
- Adjustment :  
( ) without adjustment ( X ) after adjustment

Approved By.

FM-L13 108/30-05-57



## Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110


Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 3 of 6

### Calibration Report

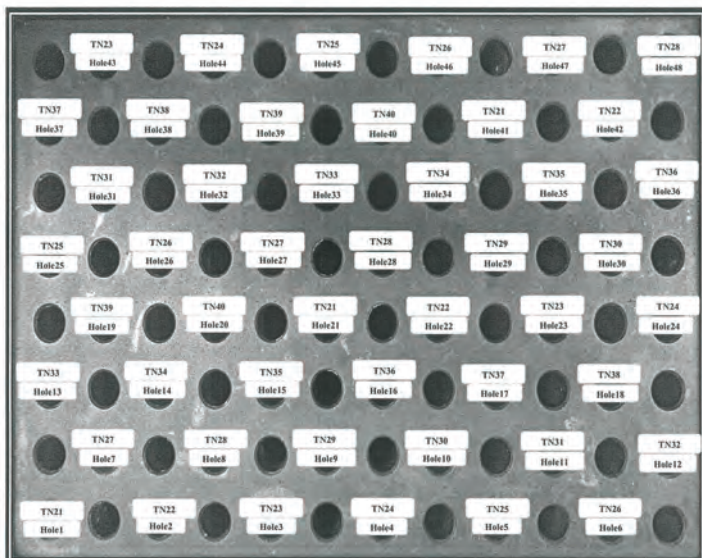

FRONT CONTROL

Approved By.

FM-L13 108/30-05-57



## Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No T231676

Page 4 of 6

### Calibration Report

#### Measurement Results

Calibration Point		Average Standard Reading at each position ( ° C )					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT 95	Max	95.01	94.41	95.20	95.41	94.51	95.17
	Min	94.57	93.95	94.75	94.92	94.00	94.72
	Average	94.79	94.18	94.98	95.17	94.26	94.95
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
	Max	95.36	95.43	95.19	95.16	95.35	94.97
	Min	94.94	94.95	94.72	94.71	94.90	94.57
	Average	95.15	95.19	94.96	94.94	95.13	94.77
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
	Max	95.37	95.50	95.22	95.21	95.33	95.31
	Min	94.99	95.09	94.78	94.82	94.88	94.96
	Average	95.18	95.30	95.00	95.02	95.11	95.13
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
	Max	95.59	94.42	94.52	94.24	94.63	94.67
	Min	95.21	94.06	94.13	93.88	94.28	94.27
	Average	95.40	94.24	94.33	94.06	94.45	94.47
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
	Max	95.19	95.38	92.93	95.30	95.14	95.03
	Min	94.83	95.03	92.56	94.95	94.79	94.70
	Average	95.01	95.20	92.75	95.12	94.96	94.87
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
	Max	94.63	94.90	94.77	94.31	94.24	93.87
	Min	94.24	94.35	94.44	93.98	93.92	93.56
	Average	94.43	94.72	94.60	94.14	94.08	93.71
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
	Max	94.30	94.44	94.04	93.81	94.89	95.35
	Min	93.95	94.05	93.67	93.48	94.39	94.90
	Average	94.13	94.24	93.86	93.65	94.64	95.12
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
	Max	95.99	95.63	95.28	95.29	95.45	94.87
	Min	95.57	95.15	94.82	94.84	94.99	94.48
	Average	95.78	95.39	95.05	95.07	95.22	94.68

Approved By.

FM-L13 108/30-05-57





## Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No T231676

Page 5 of 6

### Calibration Report

#### Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
CAL POINT	Max	TN21	TN22	TN23	TN24	TN25	TN26
	Min	105.23	104.32	105.43	105.25	104.44	105.27
	Average	105.09	104.13	105.29	105.15	104.28	105.12
R1 Hole1-Hole6		TN27	TN28	TN29	TN30	TN31	TN32
105	Max	105.30	105.12	105.18	105.22	105.12	105.16
	Min	105.11	104.92	104.96	105.00	104.92	104.97
	Average	105.20	105.02	105.07	105.11	105.02	105.06
R2 Hole7-Hole12		TN33	TN34	TN35	TN36	TN37	TN38
105	Max	105.37	105.63	105.02	104.80	104.69	105.19
	Min	105.17	105.37	104.75	104.59	104.50	105.00
	Average	105.27	105.50	104.88	104.69	104.60	105.09
R3 Hole13-Hole18		TN39	TN40	TN41	TN42	TN43	TN44
105	Max	105.31	104.43	106.41	104.71	105.63	105.82
	Min	105.08	104.22	106.15	104.41	105.37	105.56
	Average	105.19	104.33	106.28	104.56	105.50	105.69
R4 Hole19-Hole24		TN25	TN26	TN27	TN28	TN29	TN30
105	Max	104.95	105.26	103.34	105.78	105.59	105.87
	Min	104.67	105.96	103.08	105.56	105.36	105.68
	Average	104.81	106.11	103.21	105.67	105.48	105.77
R5 Hole25-Hole30		TN31	TN32	TN33	TN34	TN35	TN36
105	Max	104.75	104.86	104.80	105.20	104.50	104.39
	Min	104.54	104.63	104.59	105.00	104.32	104.18
	Average	104.65	104.75	104.69	105.10	104.41	104.28
R6 Hole31-Hole36		TN37	TN38	TN39	TN40	TN41	TN42
105	Max	104.30	104.90	104.85	104.65	104.88	104.85
	Min	104.09	104.72	104.66	104.49	104.63	104.52
	Average	104.19	104.81	104.75	104.57	104.76	104.68
R7 Hole37-Hole42		TN23	TN24	TN25	TN26	TN27	TN28
105	Max	105.71	105.85	105.39	105.61	105.42	105.19
	Min	105.45	105.61	105.14	105.27	105.18	104.94
	Average	105.58	105.73	105.27	105.44	105.30	105.07

Approved By.

FM-L13 108/30-05-57



## Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 6 of 6

### Calibration Report

#### Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (±°C)	Uncertainty (±°C)
	Min, Max	Average		
100.0	100.3, 100.5	100.4	0.26	0.81
107.0	107.0, 107.1	107.1	0.19	0.78

\* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$  which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By.

FM-L13 108/30-05-57



## Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851, +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T232160

Page 1 of 4

### Certificate of Calibration

Equipment : Chamber (Cooling Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK\_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,  
Khet Suan Luang, Bangkok 10250


Customer Location : Laboratory

Date of Receipt : 29 November 2023

Calibrated By : Atiphong Rongrat (Technician)

Approved By : Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 JAN 2024



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

FM-L14 119/15-06-66



## Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



Certificate No. T232160

Page 2 of 4

### Calibration Report

Equipment : Chamber (Cooling Room)

Date of Calibration : 6 December 2023

Environment : Temperature : 23.4-24.9 °C  
Line Voltage : 221.4-230.2 V  
Relative Humidity : 55-65 %RH

#### Condition of this results of calibration :


- This equipment was calibrated by insert 16 standard thermocouples type T into its chamber, the other one standard thermocouples type T use for ambient temperature measurement. The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986). All data show below were final values and the initial data from customer request. The temperature scale used was based on ITS-90.
- Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T230773	10 April 2024
TC	TYPE T	TN171-TN180	T230773	10 April 2024
DATA LOGGER	34970A	T149	T230773	10 April 2024
- This certificate is traceable to : National Institute of Metrology (Thailand) through Metrological Center (NSC-TIS-17025 CALIBRATION 0244).
- Condition of calibrated item : good  
Equipment Description :  
Time Constant : 1 Hour  
Fresh Air Damper : ☐ Open ☐ Min ☐ Medium ☐ Max  
☒ Not Available
- Adjustment : ( X ) without adjustment ( ) after adjustment

Approved By.

FM-L15 118/18-06-66

## Calibration Report

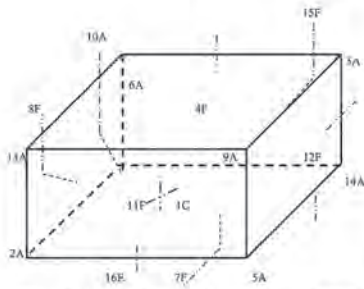

C = Centre, F = Centre of Face, A = Corner, B = Centre of Edge

1C = TN161	12F = TN172
2A = TN162	13A = TN173
3A = TN163	14A = TN174
4F = TN164	15F = TN175
5A = TN165	16E = TN176
6A = TN166	
7F = TN167	
8F = TN168	
9A = TN169	
10A = TN170	
11F = TN171	

Approved By:

FM-L15 (15/16-08-06)

## Calibration Report

## Measurement Results

Calibration Point	Average Standard Reading at each position (°C)										
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170	TN171
3.0	2.83	3.34	2.95	3.46	3.45	3.76	3.25	3.46	3.39	2.50	3.58
	TN172	TN173	TN174	TN175	TN176						
	3.33	3.39	3.13	3.43							

Chamber (Cooling Room)		Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)
	Min	Max				
3.0	2.8	4.1	3.5	3.36	1.10	2.00
						1.50
						2.00

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By:

FM-L15 (15/16-08-06)

BKK\_EL0128

Performance Verification Certificate  
for Mercury Analyzer

PRODUCT ID: Quicktrace M-8000, Teledyne Leeman Labs

Equipment ID: BKK\_EL0128 Mercury Analyzer  
S/N: US22133002

BKK\_EL0129 Autosampler  
S/N: 052222A560

Customer Name: ALS Laboratory Group (Thailand) Co., Ltd.  
Address: 104 Soi Pattana 40, Pattana Rd. Suan Luang, Suan Luang Bangkok 10250 Thailand

Date of Qualified: December 6, 2023  
Next Due date: December 6, 2024


This certifies for products which was performed in acceptable criteria specifications

Autosampler & Sample Introduction	PASSED
Analyzer	PASSED
Gas Liquid Separator & Dryer	PASSED
CVAFS Detector	PASSED
Electronics/Mechanical	PASSED
Data station/PC	PASSED
Analytical test	PASSED

Provided by

Scientist Instrument Co., Ltd.  
113 Soi Ekachai 44, Ekachai Road  
Khlong Bang Phran, Bangbon  
Bangkok 10150 Thailand

Certified by:   
Thunraphol Sakdayos  
Service Engineer



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert. No.: 23TM1408  
Page: 1 of 4

## Certificate of Calibration

Equipment: Autoclave

Manufacturer: TOMY

Model: SX-700

Serial No.: 48134190

ID No.: BKK\_ML0041

Submitted by: ALS Laboratory Group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Location: Media Preparation Room

Received Order: 03 October 2023  
Calibration Date: 04 October 2023  
Ambient Temperature: (26 ± 10) °C  
Relative Humidity: (50 ± 30) %

Calibrated by: Khit Rutanaprapachai

Approved by:   
Approved Signatory

( ) Pornthipha Tameyakul  
(x) Ponpan Paipim  
( ) Suwit Imjai

Issue Date: 11 October 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

A 0053272





Equipment : Autoclave  
Condition As-Received : Used Item  
Reference : 2310-0006OC-6  
Procedure Used :-

Cert. No.: 23TM1408  
Page : 2 of 4

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T  
The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

- Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024
- This certificate is valid only to the item calibrated on date and place of calibration.
- This certification is traceable to the International System of Unit.
- This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3\*\*  
(\* = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)  
It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.  
This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Remark : TPA : Technology Promotion Association ( Thailand - Japan )

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source



	Environmental		
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	26	64	221
Finished of Calibration	27	67	222

Position	Description	Ref. Std. ID No.:
1 =	Center of chamber	19-17TC-08
2 =	Temperature sensor	19-17TC-09
3 =	Exhaust port	19-17TC-10

PR

a 1184533



Equipment : Autoclave  
Condition As-Received : Used Item  
Reference : 2310-0006OC-6  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 23TM1408  
Page : 3 of 4

Operating parameter Set : Temperature = 108 °C  
Sterilization period = 10 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor k
108	108	1	108.352	0.12	0.04	0.90	2
		2	108.263				
		3	108.140				

Operating parameter Set : Temperature = 115 °C  
Sterilization period = 20 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor k
115	115	1	115.376	0.13	0.08	0.90	2
		2	115.297				
		3	115.157				

Operating parameter Set : Temperature = 118 °C  
Sterilization period = 10 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor k
118	118	1	118.083	0.11	0.09	0.90	2
		2	118.037				
		3	117.954				

Average\* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC\* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

PR

a 1184532



Equipment : Autoclave  
Condition As-Received : Used Item  
Reference : 2310-0006OC-6  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 23TM1408  
Page : 4 of 4

Operating parameter Set : Temperature = 121 °C  
Sterilization period = 30 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( MPa )	Uncertainty ( ± °C )	Coverage Factor k
121	121	1	121.186	0.17	0.11	0.91	2
		2	121.082				
		3	120.980				

Average\* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC\* : Unit Under Calibration

Note : The reported uncertainty of measurement was excluded stability.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

PR

a 1184531



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1146  
Page : 1 of 3

## Certificate of Calibration

Equipment : Incubator  
Manufacturer : SHEL-LAB  
Model : 1915A  
Serial No. : 0200599  
ID No. : BKK\_ML0010  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
Location : Incubation & Micrological Reading  
Received Order : 17 July 2023  
Calibration Date : 17 July 2023  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
Calibrated by : Man Pattanapongpaiboon


Approved by :  
( ) Pornthippa Tameyakul  
( ) Malee Butkruea  
( ) Suwit Injai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written

Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



A 0056489





Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2307-0285OC-1

Cert. No.: 23TM1146  
Page : 2 of 3

#### Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

##### 1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1 ) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association ( Thailand - Japan )

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Fresh air setting : Close



#### Probe Installation Details :

a = 10 cm  
b = 10 cm  
c = 10 cm

#### Dimension of Chamber :

D = 0.50 m  
W = 0.75 m  
H = 1.2 m  
Capacity = 0.45 m<sup>3</sup>

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	24	24
REL.Humid. ( % )	54	56
AC Supply ( Volt )	221	223

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Malee

a 1172189



Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2307-0285OC-1

Cert. No.: 23TM1146  
Page : 3 of 3

#### Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

##### 1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1 ) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

Measured Temperature ( °C )										Uncertainty ( ± °C )
Point ( °C )	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.888	34.933	34.815	34.813	35.064	35.019	35.156	35.141	35.087	0.30

Average\* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC\* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-000-

Malee

a 1172188



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES  
5344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert. No.: 22TM1571  
Page : 1 of 3

## Certificate of Calibration

Equipment : Hot Air Oven

Manufacturer : Binder

Model : ED 240/E2

Serial No. : 00-15533

ID No. : BKK\_ML0013

Submitted by : A.L.S Laboratory Group (Thailand) Co.,Ltd,  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 21 November 2022  
Calibration Date : 21 November 2022

Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %

Calibrated by : Krisda Malee

Approved by :   
Approved Signatory

( ) Pornthippa Tamayakul  
( ) Malee Butkrua  
( ) Suwit Injai

Issue Date : 29 November 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services & Equipment Calibration and Testing Services.

A 0048150



Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2211-0623OC-1

Cert. No.: 22TM1571  
Page : 2 of 3

#### Procedure Used :-

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

#### Condition of this result of calibration

##### 1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44067817	22LM121	22 Aug 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- ( \* ) After Adjustment

Function of UUC\* : Temperature Source

Fresh air setting : Not Available



#### Probe Installation Details :

a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm

#### Dimension of Chamber :

D = 0.50 m  
W = 0.80 m  
H = 0.80 m  
Capacity = 0.24 m<sup>3</sup>

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	26	26
REL.Humid. ( % )	53	55
AC Supply ( Volt )	219	220

Position :	Ref. Std. ID No.:
1	21-15TC-01
2	21-15TC-02
3	21-15TC-03
4	21-15TC-04
5	21-15TC-05
6	21-15TC-06
7	21-15TC-07
8	21-15TC-08
9 (ref.)	21-15TC-09

Malee

a 1138049





Equipment : Hot Air Oven  
Condition As-Received : Used Item  
Reference : 2211-0623OC-1  
Result of Calibration : ( \* ) After Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Not Available

Cert. No.: 22TM1571  
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Uncertainty (± °C)	Coverage Factor k
180	180	180	0.70	1.5	2.9	1.4	2

Calibration Point (°C)	Measured Temperature (°C)								
Position	Position								
	1	2	3	4	5	6	7	8	9 (ref.)
180	179.520	180.585	178.855	179.482	178.827	179.938	179.074	180.199	180.068

Average\* : The average of 30 values in each position.  
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.  
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.  
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.  
UUC\* : Unit Under Calibration  
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-000-

Malee

a 1138053



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
5344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM637  
Page : 1 of 3

## Certificate of Calibration

Equipment : Water Bath  
Manufacturer : Memmert  
Model : WNE 45  
Serial No. : L712.0429  
ID No. : BKK\_ML0056  
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Phatthanakan, Khet Suan Luang,  
Bangkok 10250 Thailand  
Location : Incubator & Microbiological Reading  
Received Order : 20 April 2023  
Calibration Date : 20 April 2023  
Ambient Temperature : ( 26 ± 10 ) °C  
Relative Humidity : ( 50 ± 30 ) %  
Calibrated by : Kunchit Promprat

Approved by : Malee  
Approved Signatory

( ) Ponthippa Tamayakul  
( ✓ ) Malee Butkruea  
( ) Suwit Imjai

Issue Date : 24 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

A 0053357



Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2304-0253OC-1

Cert. No.: 23TM637  
Page : 2 of 3

### Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

### Condition of this result of calibration

#### 1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1 ) Data Acquisition	34970A	MY44073381	22LM78/1	12 May 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

Result of Calibration :- ( \* ) Without Adjustment

Function of UUC\* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	25	45	223
Finished of Calibration	25	43	223



Front

Position :	Ref. Std. S/N :
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016

Malee

a 1158265



Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2304-0253OC-1  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 23TM637  
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty  (± °C)
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.492	44.463	44.475	44.510	44.491	0.15
45.0	45.0	45.0	45.005	44.962	44.979	45.016	44.986	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor k
44.5	0.051	0.022	2
45.0	0.080	0.026	2

Average\* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC\* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-000-

Malee

a 1158264