

คุณภาพน้ำผิวดิน



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 23E8494
REFERENCE No : 70413-1


PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : HANNA
MODEL : HI 3512
SERIAL No : TH118035
ID No : pH04/56
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 06-Sep-23

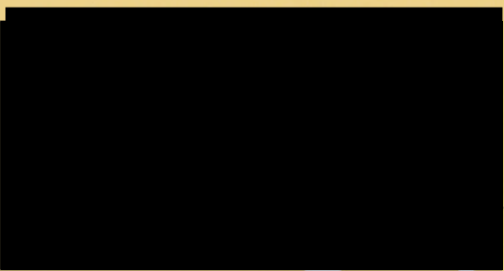APPROVED BY : 

ISSUED DATE : 06-Sep-23

RECEIVED DATE : 31-Aug-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 23E8494

PAGE : 2 OF 3

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : HANNA
ID No : pH04/56
RECEIVED DATE : 31-Aug-23
AMBIENT TEMPERATURE : 23 ° C ± 3 ° C

MODEL : HI 3512
SERIAL NUMBER : TH118035
CALIBRATION DATE : 06-Sep-23
RELATIVE HUMIDITY : 50 % RH ± 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/ LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	23E1312	19-Apr-24
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT

1. DISPLAY UNIT ONLY

SLOPE FACTOR $k = 2.303 RT/F = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.6	-0.49	-0.290	0.15	2.00
354.95	355.4	-0.45	0.741	0.15	2.00
295.80	296.3	-0.50	1.773	0.15	2.00
236.64	237.1	-0.46	2.804	0.15	2.00
177.48	177.9	-0.42	3.835	0.15	2.00
118.32	118.7	-0.38	4.867	0.15	2.00
59.16	59.6	-0.44	5.898	0.15	2.00
0.00	0.4	-0.40	6.930	0.15	2.00
-59.16	-58.8	-0.36	7.961	0.15	2.00
-118.32	-117.9	-0.42	8.992	0.15	2.00
-177.48	-177.1	-0.38	10.024	0.15	2.00
-236.64	-236.3	-0.34	11.055	0.15	2.00
-295.80	-295.5	-0.30	12.087	0.15	2.00
-354.95	-354.6	-0.35	13.118	0.15	2.00
-414.11	-413.8	-0.31	14.149	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3



CERTIFICATE No : 23E8494

PAGE : 3 OF 3

Calibration Report

RESULT OF CALIBRATION (CONTINUE) :**2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (\pm pH)	COVERAGE FACTOR k
4.006	4.006	0.000	4.015	0.012	2.00
7.000	7.000	0.000	6.914	0.012	2.00
10.008	10.010	-0.002	9.996	0.014	2.00

3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ($^{\circ}$ C)	UUC READING ($^{\circ}$ C)	CORRECTION ($^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (\pm $^{\circ}$ C)	COVERAGE FACTOR k
25.005	25.0	0.005	---	0.0085	2.00

4. PERCENT SLOPE 100%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

Certificate of Calibration

Certificate No. : 67-400037-2

Page : 1 of 2

Submitted by : S. P. S Consulting Service Co.,Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Equipment : Liquid in Glass Thermometer

Manufacturer : SK

Model : N/A

Range : 0 °C to 100 °C

Resolution : 1 °C

Serial No. : N/A

Immersion : Total

ID No. : TM21/59

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

Date of Received : 23 January 2024

Date of Calibration : 03 February 2024

Date of Issue : 03 February 2024

Calibrated by : Chortip Samchusri

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)
400004	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)

Approved by

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400037-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Ice point check : UUC* reading 0 °C Standard reading 0.4336 °C

Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
20.5609	20	0.6	0.31

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -





CERTIFICATE No : 23M2442

REFERENCE No : 68471-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY :

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23



CERTIFICATE No : 23M2442

PAGE : 2 OF 2

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	MODEL	:	BSA224S-CW
MANUFACTURER	:	SARTORIUS	S/N	:	36591843
ID No	:	BA 09/61	RECEIVED DATE	:	10-Mar-23
AIR PRESSURE	:	1010mbar \pm 1mbar	CALIBRATION DATE	:	10-Mar-23
AMBIENT TEMPERATURE	:	23° C \pm 1° C	RELATIVE HUMIDITY	:	49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000058
0.1	0.1000	0.0000	0.000059
0.2	0.2000	0.0000	0.000059
0.5	0.5000	0.0000	0.000060
1.0	1.0000	0.0000	0.000060
2.0	2.0000	0.0000	0.000061
5.0	5.0000	0.0000	0.000063
10.0	10.0000	0.0000	0.000067
20.0	20.0001	-0.0001	0.000073
50.0	50.0000	0.0000	0.00011
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	99.9999
3	99.9998
4	100.0001
5	100.0000
OFF-CENTER LOADING	0.0002

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 24M2229
REFERENCE No : 72448-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843


ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 08-Mar-24

APPROVED BY : 

ISSUED DATE : 14-Mar-24

RECEIVED DATE : 08-Mar-24



CERTIFICATE No : 24M2229

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE **MODEL** : BSA224S-CW
MANUFACTURER : SARTORIUS **S/N** : 36591843
ID No : BA 09/61 **RECEIVED DATE** : 08-Mar-24
AIR PRESSURE : 1010mbar \pm 1mbar **CALIBRATION DATE** : 08-Mar-24
AMBIENT TEMPERATURE : 25° C \pm 1° C **RELATIVE HUMIDITY** : 55 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	50.0000	0.0000	0.00012
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

CERT.No.: HS-U017D

Harikul Science Co.,Ltd.
 694 Soi Ratchadanivet 24, Pracharatbamphen,
 Samsaennok, Huaikhwang, Bangkok 10310
 Tel: 0-2274-2456 Fax: 0-2274-2443
 Email: info@harikul.com www.harikul.com
Certificate of Calibration

Calibration Date : 3 Apr 23
 Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
 7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
 Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C
 Avg Water Temp : 20 °C
 Air Pressure : 760.00 mmHg
 Salinity : 0 ppt

Model : YSI 5000
 S/N : 15B100751
 Probe : YSI 5010
 S/N : 22D100097
 ID NO. : -
 Air Temp ref : S/N. E00522
 Barometric ref : S/N. E00522
 Water Temp ref : S/N. 11431
 Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-
Overall Status	(PASS)		

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature
 (Kittipong Maekwong)

Laboratory Manager
 (Natenapha Pisatkunchon)

CERT.No.: HS-V015C

Calibration Date : 20 Mar 24
 Submitted by : ASIA LAB @ CONSULTANT CO.,LTD
 184 Soi Phutthamonthon Sai 2 Soi 12,
 Bangphai, Bangkae, Bangkok 10160

Avg Room Temp : 20 °C
 Avg Water Temp : 20 °C
 Air Pressure : 760.00 mmHg
 Salinity : 0 ppt

Model : YSI 5000
 S/N : 15B100751
 Probe : YSI 5010
 S/N : 22D100097
 ID NO. : -
 Air Temp ref : S/N. F8065C26
 Barometric ref : S/N. F8065C26
 Water Temp ref : S/N. 11430
 Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature
 (Kittipong Maekwong)

Laboratory Manager
 (Supreecha Sumaritam)



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 24T0774

REFERENCE No : 71986-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0235

ID No : CRB 05/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 5-Feb-24

APPROVED BY :

ISSUED DATE : 5-Feb-24

RECEIVED DATE : 5-Feb-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02



CERTIFICATE No : 24T0774

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : CRB 05/59
RECEIVED DATE : 5-Feb-24
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200
SERIAL NUMBER : 15110C0235
CALIBRATION DATE : 5-Feb-24
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	23T6640	14-Jul-24

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

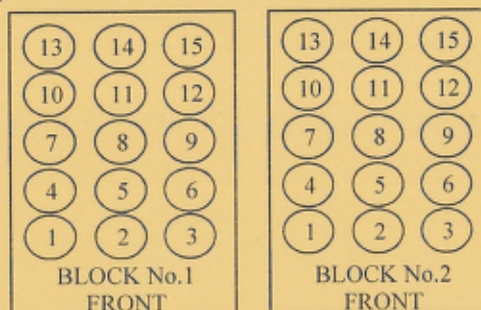

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	150.2
	2	150.2
	3	150.2
	4	149.9
	5	150.1
	6	150.7
	7	149.9
	8	149.9
	9	150.8
	10	149.5
	11	150.2
	12	150.0
	13	149.5
	14	149.5
	15	149.6
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

F-G0101

คุณภาพน้ำทิ้ง



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584



CERTIFICATE No : 23E8494
REFERENCE No : 70413-1

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : HANNA
MODEL : HI 3512
SERIAL No : TH118035
ID No : pH04/56
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 06-Sep-23

APPROVED BY : 

ISSUED DATE : 06-Sep-23

RECEIVED DATE : 31-Aug-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 23E8494

PAGE : 2 OF 3

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : HANNA
ID No : pH04/56
RECEIVED DATE : 31-Aug-23
AMBIENT TEMPERATURE : 23 ° C ± 3 ° C

MODEL : HI 3512
SERIAL NUMBER : TH118035
CALIBRATION DATE : 06-Sep-23
RELATIVE HUMIDITY : 50 % RH ± 10% RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No/ LOT No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	23E1312	19-Apr-24
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : ADJUSTMENT

1. DISPLAY UNIT ONLY

SLOPE FACTOR $k = 2.303 RT/F = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.6	-0.49	-0.290	0.15	2.00
354.95	355.4	-0.45	0.741	0.15	2.00
295.80	296.3	-0.50	1.773	0.15	2.00
236.64	237.1	-0.46	2.804	0.15	2.00
177.48	177.9	-0.42	3.835	0.15	2.00
118.32	118.7	-0.38	4.867	0.15	2.00
59.16	59.6	-0.44	5.898	0.15	2.00
0.00	0.4	-0.40	6.930	0.15	2.00
-59.16	-58.8	-0.36	7.961	0.15	2.00
-118.32	-117.9	-0.42	8.992	0.15	2.00
-177.48	-177.1	-0.38	10.024	0.15	2.00
-236.64	-236.3	-0.34	11.055	0.15	2.00
-295.80	-295.5	-0.30	12.087	0.15	2.00
-354.95	-354.6	-0.35	13.118	0.15	2.00
-414.11	-413.8	-0.31	14.149	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 3 OF 3

Calibration Report**RESULT OF CALIBRATION (CONTINUE) :****2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M**

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (\pm pH)	COVERAGE FACTOR k
4.006	4.006	0.000	4.015	0.012	2.00
7.000	7.000	0.000	6.914	0.012	2.00
10.008	10.010	-0.002	9.996	0.014	2.00

3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING ($^{\circ}$ C)	UUC READING ($^{\circ}$ C)	CORRECTION ($^{\circ}$ C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (\pm $^{\circ}$ C)	COVERAGE FACTOR k
25.005	25.0	0.005	---	0.0085	2.00

4. PERCENT SLOPE 100%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 23M2442

REFERENCE No : 68471-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 10-Mar-23

APPROVED BY :

ISSUED DATE : 16-Mar-23

RECEIVED DATE : 10-Mar-23



CERTIFICATE No : 23M2442

PAGE : 2 OF 2

Calibration Report

EQUIPMENT	:	DIGITAL BALANCE	MODEL	:	BSA224S-CW
MANUFACTURER	:	SARTORIUS	S/N	:	36591843
ID No	:	BA 09/61	RECEIVED DATE	:	10-Mar-23
AIR PRESSURE	:	1010mbar \pm 1mbar	CALIBRATION DATE	:	10-Mar-23
AMBIENT TEMPERATURE	:	23° C \pm 1° C	RELATIVE HUMIDITY	:	49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000058
0.1	0.1000	0.0000	0.000059
0.2	0.2000	0.0000	0.000059
0.5	0.5000	0.0000	0.000060
1.0	1.0000	0.0000	0.000060
2.0	2.0000	0.0000	0.000061
5.0	5.0000	0.0000	0.000063
10.0	10.0000	0.0000	0.000067
20.0	20.0001	-0.0001	0.000073
50.0	50.0000	0.0000	0.00011
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	99.9999
3	99.9998
4	100.0001
5	100.0000
OFF-CENTER LOADING	0.0002

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 24M2229
REFERENCE No : 72448-3

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE

MANUFACTURER : SARTORIUS

MODEL : BSA224S-CW

SERIAL No : 36591843

ID No : BA 09/61

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 08-Mar-24

APPROVED BY : 

ISSUED DATE : 14-Mar-24

RECEIVED DATE : 08-Mar-24



CERTIFICATE No : 24M2229

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW
MANUFACTURER : SARTORIUS S/N : 36591843
ID No : BA 09/61 RECEIVED DATE : 08-Mar-24
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 08-Mar-24
AMBIENT TEMPERATURE : 25° C \pm 1° C RELATIVE HUMIDITY : 55 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	50.0000	0.0000	0.00012
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

CERT.No.: HS-U017D

Harikul Science Co.,Ltd.
694 Soi Ratchadanivet 24, Pracharatbamphen,
Samsaennok, Huaikhwang, Bangkok 10310
Tel: 0-2274-2456 Fax: 0-2274-2443
Email: info@harikul.com www.harikul.com
Certificate of Calibration

Calibration Date : 3 Apr 23
Submitted by : S.P.S CONSULTING SERVICE CO.,LTD
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
Chatuchak, Bangkok, Thailand 10900

Avg Room Temp : 20 °C
Avg Water Temp : 20 °C
Air Pressure : 760.00 mmHg
Salinity : 0 ppt

Model : YSI 5000
S/N : 15B100751
Probe : YSI 5010
S/N : 22D100097
ID NO. : -
Air Temp ref : S/N. E00522
Barometric ref : S/N. E00522
Water Temp ref : S/N. 11431
Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-
Overall Status	(PASS)		

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature

(Kittipong Maekwong)

Laboratory Manager

(Natenapha Pisatkunchon)

CERT.No.: HS-V015C

Calibration Date : 20 Mar 24
 Submitted by : ASIA LAB @ CONSULTANT CO.,LTD
 184 Soi Phutthamonthon Sai 2 Soi 12,
 Bangphai, Bangkhae, Bangkok 10160

Avg Room Temp : 20 °C
 Avg Water Temp : 20 °C
 Air Pressure : 760.00 mmHg
 Salinity : 0 ppt

Model : YSI 5000
 S/N : 15B100751
 Probe : YSI 5010
 S/N : 22D100097
 ID NO. : -
 Air Temp ref : S/N. F8065C26
 Barometric ref : S/N. F8065C26
 Water Temp ref : S/N. 11430
 Technician : Kittipong M.

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.08	(PASS)	-
Measurement 10 (mg/l)	9.08	(PASS)	-
Mean Measurement	9.08	mg/l	-
Inaccuracy	0.01	mg/l	-

Overall Status (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature
 (Kittipong Maekwong)

Laboratory Manager
 (Supreecha Sumaritam)



QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 23T0959

REFERENCE No : 68047-2

PAGE : 1 OF 3

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB200

SERIAL No : 15110C0235

ID No : CRB 05/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 07-Feb-23

APPROVED BY :

ISSUED DATE : 07-Feb-23

RECEIVED DATE : 31-Jan-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 02



CERTIFICATE No : 23T0959

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : CRB 05/59
RECEIVED DATE : 31-Jan-23
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB200
SERIAL NUMBER : 15110C0235
CALIBRATION DATE : 07-Feb-23
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	22T7511	10-Jul-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

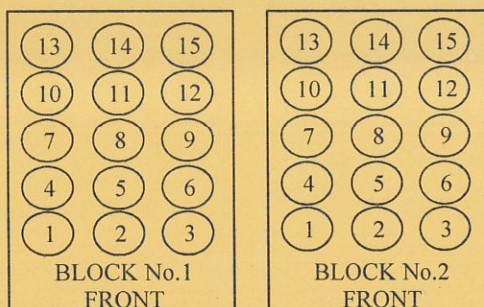

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	149.4
	2	149.5
	3	149.4
	4	149.4
	5	149.7
	6	149.6
	7	149.4
	8	149.3
	9	149.6
	10	149.6
	11	149.7
	12	149.5
	13	149.3
	14	149.5
	15	149.4
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLYING COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com

CERTIFICATE No : 24T0774

REFERENCE No : 71986-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COD REACTOR

MANUFACTURER : HACH

MODEL : DRB 200

SERIAL No : 15110C0235

ID No : CRB 05/59

SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 5-Feb-24

APPROVED BY :

ISSUED DATE : 5-Feb-24

RECEIVED DATE : 5-Feb-24



CERTIFICATE No : 24T0774

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COD REACTOR
MANUFACTURER : HACH
ID NUMBER : CRB 05/59
RECEIVED DATE : 5-Feb-24
AMBIENT TEMPERATURE : 23° C ± 1° C

MODEL : DRB 200
SERIAL NUMBER : 15110C0235
CALIBRATION DATE : 5-Feb-24
RELATIVE HUMIDITY : 52 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT TEMPERATURE RECORDER WITH THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON 15 POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE FOUR CORNERS OF THE REACTOR AND PLACED THE EIGHTH THERMOCOUPLE AT THE CENTER OF THE REACTOR.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	8009008	23T6640	14-Jul-24

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

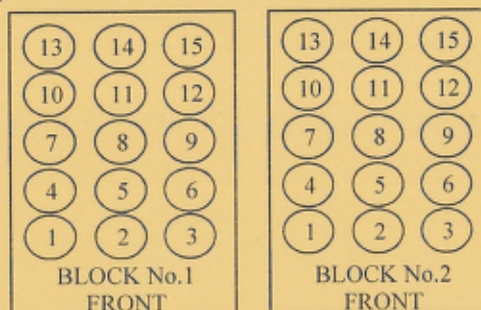

TEMPERATURE MEASUREMENT ACCURACY TEST

Block No.	1	2
Controller temperature (°C)	145	145
Indicating Temperature	145	145
Measured Temperature (°C) at Spread Locations	1	150.2
	2	150.2
	3	150.2
	4	149.9
	5	150.1
	6	150.7
	7	149.9
	8	149.9
	9	150.8
	10	149.5
	11	150.2
	12	150.0
	13	149.5
	14	149.5
	15	149.6
Uncertainty of Measurement(± °C)	0.86	0.86

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

F-G0101

คุณภาพอากาศในสถานประกอบการ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B01	SKC	224-PCXR4	262101	03/01/2024	1,000	1,500	2,000	993	1,497	1,998	1.002x - 4.467	1.000
B02	SKC	224-PCXR4	626166	03/01/2024	1,000	1,500	2,000	1,003	1,505	2,001	1.009x - 19.803	0.999
B03	SKC	224-PCXR4	612968	03/01/2024	1,000	1,500	2,000	996	1,494	2,001	1.006x - 12.799	1.000
B04	SKC	224-PCXR4	602804	04/01/2024	1,000	1,500	2,000	1,000	1,502	1,994	0.999x + 0.239	1.000
B05	SKC	224-PCXR4	612693	04/01/2024	1,000	1,500	2,000	1,003	1,500	2,002	1.011x - 21.266	0.999
B06	SKC	224-PCXR4	262188	05/01/2024	1,000	1,500	2,000	1,002	1,508	2,006	1.007x - 12.077	0.999
B07	SKC	224-PCXR4	626262	05/01/2024	1,000	1,500	2,000	998	1,492	1,997	0.994x + 4.810	1.000
B08	SKC	224-PCXR4	626100	04/01/2024	1,000	1,500	2,000	1,002	1,500	2,003	1.013x - 24.585	0.999
B09	SKC	224-PCXR4	626479	05/01/2024	1,000	1,500	2,000	998	1,490	1,994	0.993x + 3.837	1.000
B10	SKC	224-PCXR4	091950	04/01/2024	1,000	1,500	2,000	993	1,502	2,001	1.017x - 34.867	0.999
B11	SKC	224-PCXR8	564315	05/01/2024	1,000	1,500	2,000	996	1,492	1,999	1.004x - 7.965	1.000
B12	SKC	224-PCXR4	034656	05/01/2024	1,000	1,500	2,000	1,003	1,502	2,003	1.010x - 19.683	0.999
B13	SKC	224-PCXR4	602073	04/01/2024	1,000	1,500	2,000	997	1,500	1,998	1.000x - 0.862	1.000
B14	SKC	224-PCXR4	626313	03/01/2024	1,000	1,500	2,000	999	1,492	1,989	0.991x + 8.479	1.000
B15	SKC	224-PCXR4	626474	03/01/2024	1,000	1,500	2,000	1,002	1,502	2,005	1.012x - 21.697	0.999
B16	SKC	224-PCXR4	626477	04/01/2024	1,000	1,500	2,000	995	1,504	2,001	1.007x - 16.807	1.000
B17	SKC	224-PCXR4	626860	04/01/2024	1,000	1,500	2,000	997	1,494	1,991	0.997x + 0.331	1.000
B18	SKC	224-PCXR4	691484	05/01/2024	1,000	1,500	2,000	1,003	1,500	2,002	1.009x - 17.214	0.999
B19	SKC	224-PCXR4	691599	05/01/2024	1,000	1,500	2,000	993	1,503	1,999	1.005x - 8.906	1.000
B20	SKC	224-PCXR4	691587	05/01/2024	1,000	1,500	2,000	991	1,504	2,000	1.016x - 33.407	0.999
B21	SKC	224-PCXR4	691531	04/01/2024	1,000	1,500	2,000	993	1,499	1,995	1.001x - 5.540	1.000
B22	SKC	224-PCXR4	691654	03/01/2024	1,000	1,500	2,000	1,003	1,501	2,004	1.011x - 19.966	0.999
B23	SKC	224-PCXR4	798393	03/01/2024	1,000	1,500	2,000	993	1,507	2,002	1.017x - 33.276	0.999
B24	SKC	224-PCXR4	626363	03/01/2024	1,000	1,500	2,000	1,000	1,502	2,001	1.012x - 23.859	0.999
B25	SKC	224-PCXR4	798489	03/01/2024	1,000	1,500	2,000	1,001	1,492	2,001	0.998x + 0.694	1.000
B26	SKC	224-PCXR4	798479	04/01/2024	1,000	1,500	2,000	1,000	1,500	1,993	0.996x + 4.204	1.000
B27	SKC	224-PCXR4	691673	04/01/2024	1,000	1,500	2,000	994	1,503	2,002	1.016x - 30.902	0.999
B28	SKC	224-PCXR4	691570	05/01/2024	1,000	1,500	2,000	1,003	1,500	2,001	1.009x - 18.263	0.999
B29	SKC	224-PCXR4	626472	04/01/2024	1,000	1,500	2,000	1,002	1,498	2,000	1.002x - 3.909	1.000
B30	SKC	224-PCXR4	691489	04/01/2024	1,000	1,500	2,000	1,003	1,509	2,006	1.008x - 11.399	1.000
B31	SKC	224-PCXR4	691509	03/01/2024	1,000	1,500	2,000	993	1,496	1,997	1.005x - 11.275	1.000
B32	SKC	224-PCXR4	091567	03/01/2024	1,000	1,500	2,000	991	1,503	2,000	1.015x - 30.886	0.999
B33	SKC	224-PCXR4	091756	05/01/2024	1,000	1,500	2,000	993	1,498	1,992	0.999x - 2.317	1.000
B34	SKC	224-PCXR4	612962	05/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.007x - 13.995	1.000
B35	SKC	224-PCXR4	602682	05/01/2024	1,000	1,500	2,000	996	1,498	1,996	1.000x - 5.285	1.000
B36	SKC	224-PCXR4	626164	04/01/2024	1,000	1,500	2,000	999	1,510	1,999	1.004x - 10.131	0.999
B37	SKC	224-PCXR4	626256	05/01/2024	1,000	1,500	2,000	994	1,506	1,999	1.013x - 28.454	0.999
B38	SKC	224-PCXR4	626167	03/01/2024	1,000	1,500	2,000	997	1,498	1,998	1.003x - 5.983	1.000
B39	SKC	224-PCXR4	034637	03/01/2024	1,000	1,500	2,000	1,005	1,501	2,001	1.006x - 15.188	0.999
B40	SKC	224-PCXR4	798349	05/01/2024	1,000	1,500	2,000	994	1,505	2,000	1.014x - 29.004	0.999



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B41	SKC	224-PCXR4	612669	05/01/2024	1,000	1,500	2,000	999	1,496	1,991	0.996x + 1.914	1.000
B42	SKC	224-PCXR4	626041	03/01/2024	1,000	1,500	2,000	1,004	1,498	1,991	0.986x + 19.248	1.000
B43	SKC	224-PCXR4	034636	03/01/2024	1,000	1,500	2,000	1,000	1,501	1,992	0.991x + 11.682	1.000
B44	SKC	224-PCXR8	529341	03/01/2024	1,000	1,500	2,000	1,002	1,502	2,002	1.004x - 6.860	1.000
B45	SKC	224-PCXR8	529594	03/01/2024	1,000	1,500	2,000	1,001	1,501	1,987	0.987x + 16.026	1.000
B46	SKC	224-PCXR8	566743	04/01/2024	1,000	1,500	2,000	995	1,506	2,002	1.013x - 27.915	0.999
B47	SKC	224-PCXR8	566747	04/01/2024	1,000	1,500	2,000	1,002	1,502	2,004	1.010x - 21.769	0.999
B48	SKC	224-PCXR8	566753	04/01/2024	1,000	1,500	2,000	1,000	1,493	1,998	0.997x + 0.239	1.000
B49	SKC	224-PCXR8	566780	04/01/2024	1,000	1,500	2,000	1,003	1,502	2,006	1.011x - 21.550	0.999
B50	SKC	224-PCXR8	500400	03/01/2024	1,000	1,500	2,000	1,001	1,496	2,002	1.001x - 2.900	1.000
B51	SKC	224-PCXR8	500363	03/01/2024	1,000	1,500	2,000	996	1,502	2,000	1.011x - 25.709	0.999
B52	SKC	224-PCXR8	093186	03/01/2024	1,000	1,500	2,000	994	1,496	1,992	0.995x + 1.751	1.000
B53	SKC	224-PCXR8	707670	05/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.008x - 16.042	0.999
B54	SKC	224-PCXR3	509821	05/01/2024	1,000	1,500	2,000	995	1,501	2,002	1.016x - 32.282	0.999
B55	SKC	224-PCXR3	510710	05/01/2024	1,000	1,500	2,000	1,004	1,495	1,992	0.991x + 7.666	1.000
B56	SKC	224-PCXR3	511450	05/01/2024	1,000	1,500	2,000	1,002	1,500	2,001	1.005x - 8.559	1.000
B57	SKC	224-PCXR3	510798	03/01/2024	1,000	1,500	2,000	997	1,492	1,999	0.999x - 2.122	1.000
B58	SKC	224-PCXR3	509852	03/01/2024	1,000	1,500	2,000	1,000	1,500	1,999	1.007x - 19.073	0.999
B59	SKC	224-PCXR3	509862	04/01/2024	1,000	1,500	2,000	995	1,503	1,995	0.998x + 2.118	1.000
B60	SKC	224-PCXR3	512655	04/01/2024	1,000	1,500	2,000	1,004	1,510	2,004	1.005x - 6.421	0.999
B61	SKC	224-PCXR3	503915	04/01/2024	1,000	1,500	2,000	993	1,492	1,999	1.003x - 11.706	1.000
B62	SKC	224-PCXR3	505975	03/01/2024	1,000	1,500	2,000	999	1,494	1,996	0.996x + 0.822	1.000
B63	SKC	224-PCXR3	511432	03/01/2024	1,000	1,500	2,000	990	1,501	2,000	1.017x - 36.259	0.999
B64	SKC	224-PCXR3	508302	03/01/2024	1,000	1,500	2,000	998	1,492	1,989	0.990x + 10.175	1.000
B65	SKC	224-PCXR3	508310	03/01/2024	1,000	1,500	2,000	1,002	1,501	2,002	1.007x - 13.537	1.000
B66	SKC	224-PCXR3	509861	04/01/2024	1,000	1,500	2,000	1,002	1,491	1,992	0.988x + 13.744	1.000
B67	SKC	224-PCXR3	506295	04/01/2024	1,000	1,500	2,000	995	1,508	2,004	1.007x - 12.843	1.000
B68	SKC	224-PCXR3	505872	04/01/2024	1,000	1,500	2,000	1,002	1,491	1,998	0.995x + 4.040	1.000
B69	SKC	224-PCXR3	508375	04/01/2024	1,000	1,500	2,000	1,003	1,499	2,000	1.009x - 18.977	0.999
B70	SKC	224-PCXR3	510623	05/01/2024	1,000	1,500	2,000	992	1,493	1,996	1.002x - 7.730	1.000
B71	SKC	224-PCXR3	508367	05/01/2024	1,000	1,500	2,000	994	1,506	2,002	1.015x - 31.561	0.999
B72	SKC	224-PCXR3	505977	03/01/2024	1,000	1,500	2,000	1,003	1,499	1,994	0.991x + 9.042	1.000
B73	SKC	224-PCXR3	512606	04/01/2024	1,000	1,500	2,000	1,001	1,501	2,004	1.008x - 14.346	1.000
B74	SKC	224-PCXR3	505993	04/01/2024	1,000	1,500	2,000	996	1,497	1,995	1.001x - 7.036	1.000
B75	SKC	224-PCXR3	509820	05/01/2024	1,000	1,500	2,000	996	1,496	1,991	0.996x + 1.432	1.000
B76	SKC	224-PCXR3	509811	05/01/2024	1,000	1,500	2,000	993	1,499	1,999	1.006x - 14.283	1.000
B77	SKC	224-PCXR3	508301	05/01/2024	1,000	1,500	2,000	1,001	1,501	2,003	1.013x - 25.406	0.999
B78	SKC	224-PCXR3	510677	05/01/2024	1,000	1,500	2,000	995	1,503	1,999	1.012x - 27.520	0.999
B79	SKC	224-PCXR3	510920	05/01/2024	1,000	1,500	2,000	994	1,494	1,994	1.001x - 6.178	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B80	SKC	224-PCXR3	504569	05/01/2024	1,000	1,500	2,000	1,002	1,498	2,002	1.012x – 24.186	0.999
B81	SKC	224-PCXR3	503480	05/01/2024	1,000	1,500	2,000	996	1,499	2,000	1.014x – 30.165	0.999
B82	SKC	224-PCXR3	505673	04/01/2024	1,000	1,500	2,000	994	1,498	1,996	1.000x – 4.746	1.000
B83	SKC	224-PCXR3	510785	04/01/2024	1,000	1,500	2,000	1,010	1,500	1,999	1.003x – 7.793	0.999
B84	SKC	224-PCXR3	508333	04/01/2024	1,000	1,500	2,000	997	1,498	1,991	0.993x + 4.810	1.000
B85	SKC	224-PCXR3	505757	05/01/2024	1,000	1,500	2,000	994	1,502	1,998	1.006x – 14.562	1.000
B86	SKC	224-PCXR3	512625	03/01/2024	1,000	1,500	2,000	1,015	1,503	2,004	0.999x + 3.063	0.999
B87	SKC	224-PCXR3	504324	03/01/2024	1,000	1,500	2,000	1,000	1,496	2,000	1.000x – 0.710	1.000
B88	SKC	224-PCXR3	508307	03/01/2024	1,000	1,500	2,000	995	1,498	1,993	0.997x + 0.574	1.000
B89	SKC	224-PCXR3	509860	03/01/2024	1,000	1,500	2,000	1,000	1,499	2,004	1.010x – 17.509	1.000
B90	SKC	224-PCXR3	508366	04/01/2024	1,000	1,500	2,000	995	1,508	2,000	1.005x – 10.091	1.000
B91	SKC	224-PCXR3	510919	04/01/2024	1,000	1,500	2,000	1,000	1,500	1,997	0.992x + 7.522	1.000
B92	SKC	224-PCXR3	510987	04/01/2024	1,000	1,500	2,000	1,002	1,501	1,999	0.999x + 1.097	1.000
B93	SKC	224-PCXR3	509845	04/01/2024	1,000	1,500	2,000	996	1,496	2,004	1.009x – 15.822	1.000
B94	SKC	224-PCXR8	A127871	05/01/2024	1,000	1,500	2,000	1,000	1,499	2,002	1.007x – 19.184	0.999
B95	SKC	224-PCXR8	A127921	05/01/2024	1,000	1,500	2,000	994	1,502	2,002	1.015x – 30.559	0.999
B96	SKC	224-PCXR8	A127942	04/01/2024	1,000	1,500	2,000	998	1,499	1,996	1.001x – 3.486	1.000
B97	SKC	224-PCXR8	A127955	05/01/2024	1,000	1,500	2,000	1,003	1,501	2,003	1.010x – 20.082	0.999
B98	SKC	224-PCXR8	A127956	05/01/2024	1,000	1,500	2,000	996	1,497	1,998	1.003x – 6.330	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data					Calibration Data							
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)			y	R ²
					1	2	3	1	2	3		
B01	SKC	224-PCXR4	262101	05/04/2024	1,000	1,500	2,000	993	1,496	1,998	1.001x - 3.430	1.000
B02	SKC	224-PCXR4	626166	05/04/2024	1,000	1,500	2,000	1,004	1,506	2,000	1.007x - 16.572	0.999
B03	SKC	224-PCXR4	612968	09/04/2024	1,000	1,500	2,000	997	1,498	2,004	1.008x - 13.756	1.000
B04	SKC	224-PCXR4	602804	08/04/2024	1,000	1,500	2,000	1,001	1,511	1,993	0.997x + 4.427	1.000
B05	SKC	224-PCXR4	612693	08/04/2024	1,000	1,500	2,000	1,005	1,510	2,002	1.009x - 16.400	0.999
B06	SKC	224-PCXR4	262188	08/04/2024	1,000	1,500	2,000	1,003	1,510	2,004	1.005x - 8.687	0.999
B07	SKC	224-PCXR4	626262	05/04/2024	1,000	1,500	2,000	997	1,500	1,996	0.995x + 4.930	1.000
B08	SKC	224-PCXR4	626100	04/04/2024	1,000	1,500	2,000	1,003	1,508	2,002	1.011x - 19.679	0.999
B09	SKC	224-PCXR4	626479	08/04/2024	1,000	1,500	2,000	996	1,499	1,994	0.994x + 3.159	1.000
B10	SKC	224-PCXR4	091950	04/04/2024	1,000	1,500	2,000	995	1,512	2,000	1.015x - 30.041	0.998
B11	SKC	224-PCXR8	564315	08/04/2024	1,000	1,500	2,000	994	1,494	2,000	1.006x - 10.717	1.000
B12	SKC	224-PCXR4	034656	08/04/2024	1,000	1,500	2,000	1,005	1,511	2,002	1.008x - 14.857	0.999
B13	SKC	224-PCXR4	602073	05/04/2024	1,000	1,500	2,000	998	1,501	1,997	0.998x + 2.728	1.000
B14	SKC	224-PCXR4	626313	04/04/2024	1,000	1,500	2,000	998	1,491	1,991	0.994x + 4.411	1.000
B15	SKC	224-PCXR4	626474	04/04/2024	1,000	1,500	2,000	1,004	1,505	2,003	1.009x - 16.951	0.999
B16	SKC	224-PCXR4	626477	04/04/2024	1,000	1,500	2,000	997	1,502	2,000	1.005x - 13.936	1.000
B17	SKC	224-PCXR4	626860	05/04/2024	1,000	1,500	2,000	998	1,495	1,990	0.995x + 3.681	1.000
B18	SKC	224-PCXR4	691484	05/04/2024	1,000	1,500	2,000	1,004	1,506	2,001	1.007x - 12.627	0.999
B19	SKC	224-PCXR4	691599	08/04/2024	1,000	1,500	2,000	994	1,507	1,997	1.003x - 4.519	1.000
B20	SKC	224-PCXR4	691587	08/04/2024	1,000	1,500	2,000	993	1,514	1,999	1.013x - 27.943	0.998
B21	SKC	224-PCXR4	691531	08/04/2024	1,000	1,500	2,000	997	1,498	1,993	0.996x - 1.121	1.000
B22	SKC	224-PCXR4	691654	08/04/2024	1,000	1,500	2,000	1,002	1,500	2,005	1.013x - 23.316	0.999
B23	SKC	224-PCXR4	798393	09/04/2024	1,000	1,500	2,000	995	1,506	1,999	1.014x - 28.370	0.999
B24	SKC	224-PCXR4	626363	04/04/2024	1,000	1,500	2,000	997	1,505	2,003	1.016x - 28.805	0.999
B25	SKC	224-PCXR4	798489	04/04/2024	1,000	1,500	2,000	1,000	1,494	2,002	0.999x - 1.300	1.000
B26	SKC	224-PCXR4	798479	05/04/2024	1,000	1,500	2,000	1,001	1,501	1,997	0.998x + 2.010	1.000
B27	SKC	224-PCXR4	691673	08/04/2024	1,000	1,500	2,000	995	1,505	2,001	1.014x - 28.031	0.999
B28	SKC	224-PCXR4	691570	08/04/2024	1,000	1,500	2,000	1,004	1,498	2,000	1.007x - 15.352	0.999
B29	SKC	224-PCXR4	626472	08/04/2024	1,000	1,500	2,000	1,003	1,496	2,003	1.003x - 5.903	1.000
B30	SKC	224-PCXR4	691489	05/04/2024	1,000	1,500	2,000	1,005	1,511	2,005	1.007x - 8.527	0.999
B31	SKC	224-PCXR4	691509	09/04/2024	1,000	1,500	2,000	991	1,495	1,998	1.006x - 14.067	1.000
B32	SKC	224-PCXR4	091567	05/04/2024	1,000	1,500	2,000	993	1,504	1,999	1.013x - 26.659	0.999
B33	SKC	224-PCXR4	091756	05/04/2024	1,000	1,500	2,000	994	1,500	1,995	1.000x - 2.836	1.000
B34	SKC	224-PCXR4	612962	08/04/2024	1,000	1,500	2,000	1,004	1,503	2,001	1.006x - 11.243	0.999
B35	SKC	224-PCXR4	602682	08/04/2024	1,000	1,500	2,000	997	1,496	1,995	0.998x - 2.772	1.000
B36	SKC	224-PCXR4	626164	05/04/2024	1,000	1,500	2,000	997	1,506	2,000	1.006x - 14.159	0.999
B37	SKC	224-PCXR4	626256	04/04/2024	1,000	1,500	2,000	997	1,507	1,998	1.010x - 23.269	0.999
B38	SKC	224-PCXR4	626167	04/04/2024	1,000	1,500	2,000	996	1,496	1,997	1.004x - 7.259	1.000
B39	SKC	224-PCXR4	034637	04/04/2024	1,000	1,500	2,000	1,007	1,499	2,000	1.003x - 11.120	0.999
B40	SKC	224-PCXR4	798349	08/04/2024	1,000	1,500	2,000	995	1,506	2,001	1.013x - 26.810	0.999



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B41	SKC	224-PCXR4	612669	05/04/2024	1,000	1,500	2,000	1,001	1,498	1,990	0.994x + 6.342	1.000
B42	SKC	224-PCXR4	626041	04/04/2024	1,000	1,500	2,000	1,006	1,496	1,990	0.984x + 20.844	1.000
B43	SKC	224-PCXR4	034636	04/04/2024	1,000	1,500	2,000	998	1,498	1,989	0.989x + 12.360	1.000
B44	SKC	224-PCXR8	529341	09/04/2024	1,000	1,500	2,000	1,000	1,501	2,002	1.005x - 9.213	1.000
B45	SKC	224-PCXR8	529594	04/04/2024	1,000	1,500	2,000	1,002	1,502	1,989	0.988x + 16.584	1.000
B46	SKC	224-PCXR8	566743	04/04/2024	1,000	1,500	2,000	996	1,507	2,001	1.012x - 24.724	0.999
B47	SKC	224-PCXR8	566747	08/04/2024	1,000	1,500	2,000	1,005	1,500	2,002	1.007x - 16.424	0.999
B48	SKC	224-PCXR8	566753	09/04/2024	1,000	1,500	2,000	998	1,492	1,997	0.998x - 1.157	1.000
B49	SKC	224-PCXR8	566780	08/04/2024	1,000	1,500	2,000	1,004	1,503	2,005	1.009x - 18.040	0.999
B50	SKC	224-PCXR8	500400	04/04/2024	1,000	1,500	2,000	1,003	1,495	2,003	1.000x - 1.783	1.000
B51	SKC	224-PCXR8	500363	04/04/2024	1,000	1,500	2,000	995	1,500	2,002	1.013x - 28.701	0.999
B52	SKC	224-PCXR8	093186	04/04/2024	1,000	1,500	2,000	992	1,494	1,991	0.996x + 0.116	1.000
B53	SKC	224-PCXR8	707670	08/04/2024	1,000	1,500	2,000	1,000	1,502	2,001	1.009x - 16.999	0.999
B54	SKC	224-PCXR3	509821	08/04/2024	1,000	1,500	2,000	996	1,503	2,002	1.015x - 30.009	0.999
B55	SKC	224-PCXR3	510710	05/04/2024	1,000	1,500	2,000	1,000	1,494	1,993	0.995x + 0.965	1.000
B56	SKC	224-PCXR3	511450	09/04/2024	1,000	1,500	2,000	1,004	1,499	2,000	1.002x - 4.651	1.000
B57	SKC	224-PCXR3	510798	08/04/2024	1,000	1,500	2,000	996	1,494	1,998	1.000x - 2.680	1.000
B58	SKC	224-PCXR3	509852	08/04/2024	1,000	1,500	2,000	1,002	1,501	2,000	1.006x - 16.480	0.999
B59	SKC	224-PCXR3	509862	08/04/2024	1,000	1,500	2,000	997	1,501	1,998	0.999x + 1.041	1.000
B60	SKC	224-PCXR3	512655	05/04/2024	1,000	1,500	2,000	1,005	1,507	2,003	1.003x - 4.627	1.000
B61	SKC	224-PCXR3	503915	05/04/2024	1,000	1,500	2,000	993	1,490	2,000	1.004x - 12.823	1.000
B62	SKC	224-PCXR3	505975	05/04/2024	1,000	1,500	2,000	1,001	1,495	1,997	0.995x + 2.616	1.000
B63	SKC	224-PCXR3	511432	05/04/2024	1,000	1,500	2,000	993	1,503	1,999	1.014x - 30.715	0.999
B64	SKC	224-PCXR3	508302	08/04/2024	1,000	1,500	2,000	1,000	1,493	1,987	0.988x + 13.991	1.000
B65	SKC	224-PCXR3	508310	09/04/2024	1,000	1,500	2,000	1,003	1,500	2,003	1.006x - 12.021	1.000
B66	SKC	224-PCXR3	509861	08/04/2024	1,000	1,500	2,000	1,004	1,489	1,990	0.986x + 16.775	1.000
B67	SKC	224-PCXR3	506295	04/04/2024	1,000	1,500	2,000	997	1,506	2,003	1.004x - 9.094	1.000
B68	SKC	224-PCXR3	505872	04/04/2024	1,000	1,500	2,000	1,004	1,490	1,997	0.992x + 7.829	1.000
B69	SKC	224-PCXR3	508375	04/04/2024	1,000	1,500	2,000	1,005	1,500	1,998	1.006x - 13.832	0.999
B70	SKC	224-PCXR3	510623	08/04/2024	1,000	1,500	2,000	995	1,491	1,996	1.000x - 4.938	1.000
B71	SKC	224-PCXR3	508367	09/04/2024	1,000	1,500	2,000	996	1,504	2,000	1.012x - 27.572	0.999
B72	SKC	224-PCXR3	505977	09/04/2024	1,000	1,500	2,000	1,001	1,500	1,995	0.994x + 5.791	1.000
B73	SKC	224-PCXR3	512606	04/04/2024	1,000	1,500	2,000	1,002	1,499	2,002	1.007x - 12.671	1.000
B74	SKC	224-PCXR3	505993	04/04/2024	1,000	1,500	2,000	995	1,495	1,996	1.003x - 9.987	1.000
B75	SKC	224-PCXR3	509820	05/04/2024	1,000	1,500	2,000	998	1,497	1,993	0.997x + 1.432	1.000
B76	SKC	224-PCXR3	509811	05/04/2024	1,000	1,500	2,000	992	1,497	2,000	1.008x - 17.753	1.000
B77	SKC	224-PCXR3	508301	05/04/2024	1,000	1,500	2,000	1,004	1,499	2,001	1.010x - 19.743	0.999
B78	SKC	224-PCXR3	510677	08/04/2024	1,000	1,500	2,000	997	1,505	2,001	1.013x - 27.321	0.999
B79	SKC	224-PCXR3	510920	09/04/2024	1,000	1,500	2,000	995	1,495	1,993	1.000x - 4.702	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Personal Pump Calibration Report

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Environmental Conditions

Temperature : 25 \pm 3 $^{\circ}$ C
Pressure : 1010 \pm 15 mmbar

Personal Pump Data				Calibration Data								
No.	Brand	Model	Serial No.	Date	Flow Rate (mL/min)						Value From Calibration Curve	
					Setting			Actual (Q std.)				
					1	2	3	1	2	3	y	R ²
B80	SKC	224-PCXR3	504569	09/04/2024	1,000	1,500	2,000	1,003	1,501	2,004	1.013x - 23.428	0.999
B81	SKC	224-PCXR3	503480	04/04/2024	1,000	1,500	2,000	998	1,499	2,003	1.015x - 30.384	0.999
B82	SKC	224-PCXR3	505673	04/04/2024	1,000	1,500	2,000	995	1,496	1,998	1.001x - 5.105	1.000
B83	SKC	224-PCXR3	510785	08/04/2024	1,000	1,500	2,000	1,012	1,499	2,000	1.002x - 7.135	0.999
B84	SKC	224-PCXR3	508333	08/04/2024	1,000	1,500	2,000	998	1,500	1,990	0.991x + 8.599	1.000
B85	SKC	224-PCXR3	505757	09/04/2024	1,000	1,500	2,000	993	1,503	2,000	1.008x - 16.396	1.000
B86	SKC	224-PCXR3	512625	04/04/2024	1,000	1,500	2,000	1,011	1,501	2,002	1.000x + 0.072	0.999
B87	SKC	224-PCXR3	504324	04/04/2024	1,000	1,500	2,000	998	1,495	2,001	1.003x - 4.738	1.000
B88	SKC	224-PCXR3	508307	08/04/2024	1,000	1,500	2,000	997	1,500	1,994	0.996x + 3.047	1.000
B89	SKC	224-PCXR3	509860	04/04/2024	1,000	1,500	2,000	1,001	1,501	2,006	1.011x - 17.174	1.000
B90	SKC	224-PCXR3	508366	08/04/2024	1,000	1,500	2,000	997	1,510	2,001	1.004x - 8.814	1.000
B91	SKC	224-PCXR3	510919	04/04/2024	1,000	1,500	2,000	1,001	1,502	1,998	0.993x + 7.522	1.000
B92	SKC	224-PCXR3	510987	04/04/2024	1,000	1,500	2,000	1,000	1,504	2,000	1.001x - 0.858	1.000
B93	SKC	224-PCXR3	509845	08/04/2024	1,000	1,500	2,000	998	1,495	2,003	1.007x - 13.389	1.000
B94	SKC	224-PCXR8	A127871	08/04/2024	1,000	1,500	2,000	1,001	1,501	2,004	1.008x - 19.942	0.999
B95	SKC	224-PCXR8	A127921	08/04/2024	1,000	1,500	2,000	996	1,504	2,005	1.016x - 31.417	0.999
B96	SKC	224-PCXR8	A127942	08/04/2024	1,000	1,500	2,000	999	1,500	2,000	1.003x - 5.715	1.000
B97	SKC	224-PCXR8	A127955	08/04/2024	1,000	1,500	2,000	1,004	1,502	2,005	1.011x - 20.122	0.999
B98	SKC	224-PCXR8	A127956	08/04/2024	1,000	1,500	2,000	995	1,496	2,000	1.004x - 9.122	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72. Fax : (662) 513-4221. E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-B01	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	506.5	991.1	1974.3	0.989x + 9.286	1.000
H-B02	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	496.7	997.6	1996.1	0.994x + 4.509	1.000
H-B03	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	497.6	988.8	2009.6	1.004x - 14.177	0.999
H-B04	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	501.6	998.7	2006.5	0.997x - 0.777	1.000
H-B05	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	500.4	997.3	1974.3	0.980x + 21.602	0.999
H-B06	Dwyer	VFB-65	05/01/2024	500	1,000	2,000	504.9	994.8	1984.0	1.003x - 5.213	1.000
H-B07	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	502.6	990.6	2016.7	1.001x - 0.998	1.000
H-B08	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	499.7	998.7	1979.8	0.996x + 3.580	0.999
H-B09	Dwyer	VFB-65	04/01/2024	500	1,000	2,000	504.1	1004.3	2010.7	0.993x + 13.998	1.000
H-B10	Dwyer	VFB-65	03/01/2024	500	1,000	2,000	496.2	999.3	2009.2	0.996x + 3.860	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-801	Dwyer	VFA-21	04/01/2024	50	100	200	50.7	98.5	198.9	0.986x + 0.884	1.000
L-802	Dwyer	VFA-21	04/01/2024	50	100	200	50.6	99.2	198.7	0.997x + 0.603	0.999
L-803	Dwyer	VFA-21	04/01/2024	50	100	200	50.1	99.2	198.3	1.010x - 1.750	1.000
L-804	Dwyer	VFA-21	03/01/2024	50	100	200	49.2	102.0	200.5	1.011x - 0.502	1.000
L-805	Dwyer	VFA-21	05/01/2024	50	100	200	50.5	99.4	200.8	0.999x + 0.948	0.999
L-806	Dwyer	VFA-21	05/01/2024	50	100	200	50.5	99.0	202.3	1.010x - 0.360	1.000
L-807	Dwyer	VFA-21	03/01/2024	50	100	200	49.5	100.3	200.1	1.013x - 1.486	1.000
L-808	Dwyer	VFA-21	04/01/2024	50	100	200	50.7	101.2	199.3	1.000x + 0.298	1.000
L-809	Dwyer	VFA-21	04/01/2024	50	100	200	50.5	99.0	200.2	0.992x + 1.365	1.000
L-810	Dwyer	VFA-21	03/01/2024	50	100	200	50.7	98.5	203.2	0.998x + 1.334	0.999



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com., www.spscon.com

Rotameter Calibration Report (For Personal Pump High Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Calibration Data

Rotameter Data			Calibration Data								
No.	Brand	Model	Date	Flow Rate (ml/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
H-B01	Dwyer	VFB-65	08/04/2024	500	1,000	2,000	504.3	992.1	1976.8	0.991x + 6.353	1.000
H-B02	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	496.5	998.8	1996.7	0.995x + 4.247	1.000
H-B03	Dwyer	VFB-65	05/04/2024	500	1,000	2,000	498.6	991.4	2011.0	1.003x - 12.161	0.999
H-B04	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	501.4	1000.9	2008.3	0.998x - 1.566	1.000
H-B05	Dwyer	VFB-65	08/04/2024	500	1,000	2,000	502.9	999.5	1974.5	0.979x + 24.520	0.999
H-B06	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	504.7	996.0	1984.4	1.005x - 6.145	1.000
H-B07	Dwyer	VFB-65	05/04/2024	500	1,000	2,000	502.2	992.8	2017.1	1.000x - 0.160	1.000
H-B08	Dwyer	VFB-65	04/04/2024	500	1,000	2,000	500.3	1000.7	1980.2	0.995x + 5.203	0.999
H-B09	Dwyer	VFB-65	09/04/2024	500	1,000	2,000	503.3	1005.0	2011.1	0.994x + 13.348	1.000
H-B10	Dwyer	VFB-65	08/04/2024	500	1,000	2,000	498.2	1001.7	2008.8	0.995x + 5.854	1.000



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด

S.P.S. CONSULTING SERVICE CO., LTD.

7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Rotameter Calibration Report (For Personal Pump Low Flow Adjust)

Calibration Method : Dry Cal Primary Flowmeter

Model : Defender 510-H

S/N : 136164

Rotameter Data				Calibration Data							
No.	Brand	Model	Date	Flow Rate (mL/min)						Value From Calibration Curve	
				Flow Rate (Reading)			Actual (Q std.)				
				1	2	3	1	2	3	y	R ²
L-801	Dwyer	VFA-21	08/04/2024	50	100	200	50.7	98.8	199.3	0.987x + 1.039	1.000
L-802	Dwyer	VFA-21	04/04/2024	50	100	200	50.2	98.8	198.3	0.998x + 0.180	0.999
L-803	Dwyer	VFA-21	05/04/2024	50	100	200	50.5	98.8	197.9	1.012x - 1.915	1.000
L-804	Dwyer	VFA-21	04/04/2024	50	100	200	49.8	101.6	201.9	1.010x - 0.036	1.000
L-805	Dwyer	VFA-21	08/04/2024	50	100	200	50.9	99.0	201.2	0.998x + 0.999	1.000
L-806	Dwyer	VFA-21	04/04/2024	50	100	200	50.1	99.4	202.7	1.011x - 0.423	1.000
L-807	Dwyer	VFA-21	05/04/2024	50	100	200	50.3	99.9	200.5	1.009x - 0.861	1.000
L-808	Dwyer	VFA-21	04/04/2024	50	100	200	50.6	100.8	198.9	1.002x - 0.189	1.000
L-809	Dwyer	VFA-21	09/04/2024	50	100	200	50.1	99.4	200.6	0.997x + 0.731	1.000
L-810	Dwyer	VFA-21	08/04/2024	50	100	200	51.0	98.9	202.8	0.996x + 1.709	0.999



GAS CHROMATOGRAPH TEST CERTIFICATION

Certificate No. : SV0823/21044

Instrument Type : GC

Model : CP-3800

Serial Number : 00734

Organization : S.P.S. Consulting Service Co., Ltd.

Address : 7 Phahonyothin Soi 24 Phahonyothin Rd. Ladyao Chatuchak Bangkok 10900

Date : 09/08/2023

ELECTRONIC TEST

CPU	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
LCD TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
VENT TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
KEY ECHO TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL
DESTRUCTION RAM TEST	<input checked="" type="checkbox"/> PASS	<input type="checkbox"/> FAIL

RUN CHROMATOGRAM TEST

DETECTOR : Flame Ionization Detector (FID Channel Front)

INJECTOR : Capillary Injector Model 1079

GC CONDITION:

Column	80 °C hold 1 min., rate 20 °C/min. to 200 °C hold 1min.
Injector	220 °C
Detector	300 °C
Column flow	5 mL/min
Makeup flow	25 mL/min
Air flow	300 mL/min
Hydrogen flow	30 mL/min

Column:Capillary Column CP sil 5 CB 0.25 ID x 15 M

Sample: 1 µL Injection FID Test Sample 0.218 g/L C14,C15,C16 in hexane

SENSITIVITY TEST: C15. (Area count) = 362,972 Counts.



**Detector Sensitivity (FID)**


Detector Response	Result	Specification
Baseline Noise (µV)	1.47	≤ 50
Baseline Drift (%)	0.09	≤ 1
Sensitivity (S/N for C15)	19,600	≥ 1,024

Temperature Specification

Temperature	Set	Result	Specification
Column Oven (° C)	80	80	± 5
Injector (° C)	220	220	± 5
Detector (° C)	300	300	± 5
Incubator (° C)	60	N/A	± 5

Relative Standard Deviation % (% RSD)

Checkout Procedure	Result	Specification
Area C15 (%)	1.52	≤ 5
Retention Time C15(%)	0.01	≤ 0.5



Date : 09/08/2023





บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไตย แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 Area 1	357,863
C15 Area 2	357,824
C15 Area 3	367,724
C15 Area 4	361,724
C15 Area 5	369,724
C15 Area Average	362,972
* % RSD (< 5 %)	1.52

* The precision specification should be less than 2.0 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 5 % for Manual injections. To calculate the %RSD, select the C15 peak area for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by		
Date	09/08/2023	



Comments			
Reviewed by			Date 09/08/2023



VARIAN



บริษัท ไทยยูนิค จำกัด

THAI UNIQUE CO., LTD.

80-82 ถนนประชาธิปไทย์ แขวงบางขุนพรหม เขตพระนคร กรุงเทพฯ 10200

80-82 Prachathipatai Rd., Bangkhunphrom, Pranakorn, Bangkok 10200

Tel. 0-2629-0191-6, 0-2280-1787, Fax. 0-2280-1788, E-mail : thawatt@thaiunique.com, Website : www.thaiunique.com

Results Integrated System Testing

Checkout Procedure	FID
Detector Position	Front
Inlet Type	1079 Injector
C15 RT 1	4.125
C15 RT 2	4.125
C15 RT 3	4.125
C15 RT 4	4.124
C15 RT 5	4.124
C15 RT Average	4.122
* % RSD (< 0.5 %)	0.01

* The precision specification should be less than 0.5 % RSD ** (Relative Standard Deviation) for an Auto sampler injection and less than 0.5 % for Manual injections. To calculate the %RSD, select the RT C15 peak for each of the five (5) samples.

** (Relative Standard Deviation is determined by dividing the standard deviation by the average and multiplying by 100.)

$$\% \text{ RSD} = (\text{std.dev} / \text{avg}) * 100$$

Compliance	<input checked="" type="checkbox"/> Pass	<input type="checkbox"/> Fail
Performance by		
Date	09/08/2023	



Comments			
Reviewed by			Date 09/08/2023



VARIAN

ระดับเสียงในสถานประกอบการ

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

CALIBRATION CERTIFICATE

Submitted by : S.P.S. Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
: Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 27 Mar. 2023

Date of Calibration : 29 Mar. 2023

1 / 1

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0413

MTC No. EEL. BP. 109/0366

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions : 101.325 kPa, 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	93.94	-0.06	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 1.0\%$


3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

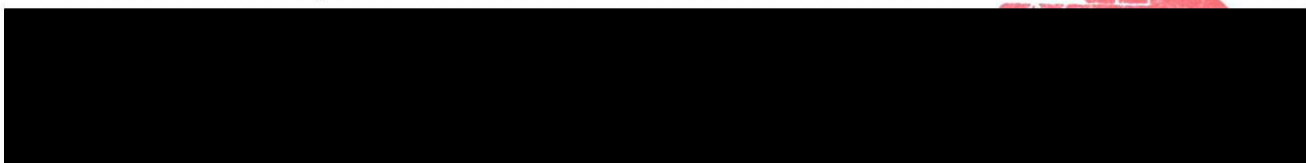

Director
Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 29 Mar. 2023

Date of Issue : 30 Mar. 2023

Ref : 2011266032701228001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise B_050/24

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	29 March 2023
		Due Date	29 March 2024

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B18	ACO	6236	00172048	03 March 2024	94.1	94.0
ACO-B29	ACO	6236	00182011	03 March 2024	94.1	94.0
ACO-B33	ACO	6236	00182015	03 March 2024	94.0	94.0
ACO-B36	ACO	6236	00192027	03 March 2024	94.0	94.0
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.94 ± 0.10 dB	

Request No. 21-67/0304

MTC No. EEL. BP. 109/0267

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used :

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N4106495.
7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 22 Feb. 2024

Date of Calibration : 4 Mar. 2024

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpa@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Request No. 21-67/0304

MTC No. EEL. BP. 109/0267

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	93.85	-0.15	± 0.10	± 0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	$\pm 2.0\%$

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1.65	± 0.50	$\pm 4.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Director

**Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre**

Date of Calibration : 4 Mar. 2024

Date of Issue : 5 Mar. 2024

Ref : 2011267022200795001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

Noise B_229/24

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	04 March 2024
		Due Date	04 March 2025

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B33	ACO	6236	00182015	13 June 2024	93.9	93.9
ACO-B36	ACO	6236	00192027	13 June 2024	93.9	93.9
ACO-B41	ACO	6236	00192032	13 June 2024	93.9	93.9
ACO-B43	ACO	6236	00192034	13 June 2024	94.1	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.85 ± 0.10 dB	