

ANALYTICAL BALANCE (DU)

Model : XS205DU

Serial No. : 1126323724

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : METTLER TOLEDO
Model : XS205DU
Capacity : Max 81 g / 220 g
Resolution : 0.01 mg / 0.1 mg
Serial No. : 1126323724
ID No. : LABE 05/1

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 80	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	40 80 40 80	
<input checked="" type="checkbox"/> Adjustment	Standard weight	40.000054 80.000048 40.000054 80.000048	
	Average reading of indicator	40.000026 80.000037 40.000017 80.000017	
	Standard deviation	0.000015 0.000016 0.000008 0.000009	
Unit : g	Range : 200	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	100 200 100 200	
<input checked="" type="checkbox"/> Adjustment	Standard weight	100.000042 200.000041 100.000042 200.000041	
	Average reading of indicator	100.00003 200.00004 100.00001 200.00001	
	Standard deviation	0.00005 0.00005 0.00003 0.00005	

COPY

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230
Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : METTLER TOLEDO

Model : XS205DU

Serial No. : 1126323724

ID No. : LABE 05/1

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Calibrated by : Mr. Somwang Sangdee
Scientist
Approved by : (Mr. Somchai Neampunt)
Signed for Director

Issue date : 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-148799

Sample Code : 23-56200-001

Page 3 of 4

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 80		Range : 200	
Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	1.00748	0	1.0274
40	0.98753	100	0.9975
80	0.99751	200	0.9975

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.00000	0.00000	0.000012	2.05
0.01	0.0100025	0.01000	0.00000	0.000012	2.05
0.1	0.1000019	0.10001	-0.00001	0.000013	2.03
1	1.0000125	1.00001	0.00000	0.000015	2.02
5	5.0000208	5.00004	-0.00002	0.000021	2.00
10	10.0000004	10.00008	-0.00008	0.000026	2.00
20	20.0000030	20.00011	-0.00008	0.000036	2.00
50	50.0000014	50.00014	-0.00013	0.000068	2.00
100	100.0000042	100.00001	-0.00001	0.00016	2.00
150	150.0000056	150.00001	0.00000	0.00022	2.00
200	200.0000041	200.00002	-0.00002	0.00027	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY



Certificate No. : 23-148799

Sample Code : 23-56200-001


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan ☐ Circle ☐ Triangular ☒ Rectangular
Test weight : 50 and 100
Unit : g

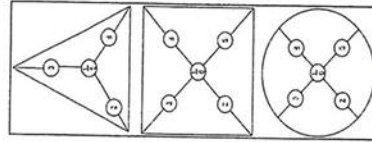

Range	Position	Reading of indicator	Reading of indicator
1	50.00015	100.0001	100.0001
2	50.00022	100.0001	100.0001
3	50.00008	100.0001	100.0001
4	50.00002	100.0000	100.0000
5	50.00016	100.0002	100.0001
6	50.00014	100.0001	100.0001
Maximum difference	0.00013	0.0001	0.0001

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -

Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument
1) STANDARD WEIGHT 1 mg to 1 kgClass ID No. Certificate No.
E2 LB-WE-79 23-105642Due Date
10 September 2024

- End of Report -

CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date : 15/10/21

ANALYTICAL BALANCE

Model : MS204TS/00

Serial No. : B904136539

Mettler-Toledo (Thailand) Ltd.
846/4 - 846/5 Lassaile Rd., Bangna Tai Sub-District
Bangna District, Bangkok 10260
+66 2723 0382
MT-TH ServiceSupport@mt.com



Accuracy Calibration Certificate

Customer

Company: EASTERN THAI CONSULTING 1992 CO., LTD.
Address: 683 Moo 11, Sukhaphiban 8 Rd., Nong Kham
City: Siracha
Zip / Postal: 20230
State / Province: Chonburi
Order Number: 0332980000

Contact: Sasiporn N.

Weighing Device

Manufacturer: Mettler Toledo
Model: MS204TS100
Serial No.: B904136539
Building: Laboratory
Floor: 1
Room: Balance

Instrument Type: Weighing Instrument
Asset Number: LABE 05/4
Terminal Model: N/A
Terminal Serial No.: N/A
Terminal Asset No.: N/A

Range	Max. Capacity	Readability (d)
1	220 g	0.0001 g

Procedure

Calibration Guideline: EURAMET cg-18 v. 4.0 (11/2015)
Mettler Toledo Work Instruction: CPW002/20

This calibration certificate contains measurements for As Found and As Left calibrations.
The sensitivity/span of the weighing instrument was adjusted before As Found and As Left calibrations with a built-in weight.
In accordance with EURAMET cg-18 (11/2015), the test loads were selected to reflect the specific use of the weighing device or to accommodate specific calibration conditions.

Temperature		Humidity	
As Found	Start: 23.4 °C End: 23.4 °C	Start: 50.6 % End: 50.6 %	
As Left	Start: 23.8 °C End: 23.4 °C	Start: 51.8 % End: 51.2 %	

As Found Calibration Date: 05-Feb-2024
As Left Calibration Date: 05-Feb-2024
Issue Date: 05-Feb-2024

Calibrator: Sathaporn T.
Sathaporn Tabson
Approved Signatory:

Technical Manager / Head of Calibration Center

Measurement Results


Repeatability

Test Load: 100 g		As Found	As Left	As Found	As Left
1	99.9996 g	100.0001 g	100.0001 g	25d	
2	99.9997 g	100.0001 g	100.0001 g	4d	
3	99.9997 g	100.0000 g	100.0001 g	3d	
4	99.9996 g	100.0001 g	100.0001 g	2d	
5	99.9997 g	100.0001 g	100.0001 g	1d	
6	99.9996 g	100.0000 g	100.0001 g		
7	99.9997 g	100.0001 g	100.0000 g		
8	99.9996 g	100.0000 g	100.0001 g		
9	99.9996 g	100.0001 g	100.0001 g		
10	99.9996 g	100.0001 g	100.0001 g		
Standard Deviation		0.00005 g	0.00005 g		

The "d" in the graph represents the readability of the range/interval in which the test was performed.
The results of this graph are based upon the absolute values of the differences from the mean value.

Eccentricity

Test Load: 100 g		Position	As Found	As Left
1	99.9996 g	1	100.0000 g	100.0000 g
2	99.9996 g	2	100.0000 g	100.0000 g
3	99.9997 g	3	100.0001 g	100.0001 g
4	99.9996 g	4	100.0001 g	100.0001 g
5	99.9996 g	5	100.0000 g	100.0000 g
Maximum Deviation			0.0001 g	0.0001 g

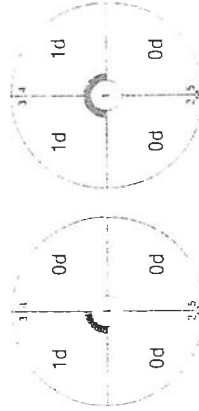

The "d" in the graph represents the readability of the range/interval in which the test was performed.

COPY


Error of Indication

The results of this calibration certificate relate only to the calibrated item.

As Found				
	Reference Value	Indication	Error of Indication	Expanded Uncertainty
1	0.0000 g	0.0000 g	0.0000 g	0.12 mg
2	0.0100 g	0.0100 g	0.0000 g	0.13 mg
3	0.0500 g	0.0499 g	-0.0001 g	0.13 mg
4	0.1000 g	0.0999 g	-0.0001 g	0.13 mg
5	1.0000 g	0.9999 g	-0.0001 g	0.13 mg
6	5.0000 g	4.9999 g	-0.0001 g	0.14 mg
7	10.0000 g	9.9999 g	-0.0001 g	0.14 mg
8	50.0000 g	49.9997 g	-0.0003 g	0.16 mg
9	100.0000 g	99.9995 g	-0.0005 g	0.20 mg
10 ¹	149.9999 g	149.9993 g	-0.0006 g	0.31 mg
11 ¹	199.9998 g	199.9990 g	-0.0008 g	0.35 mg

As Left				
	Reference Value	Indication	Error of Indication	Expanded Uncertainty
1	0.0000 g	0.0000 g	0.0000 g	0.11 mg
2	0.0100 g	0.0100 g	0.0000 g	0.13 mg
3	0.0500 g	0.0500 g	0.0000 g	0.13 mg
4	0.1000 g	0.1000 g	0.0000 g	0.13 mg
5	1.0000 g	1.0001 g	0.0001 g	0.13 mg
6	5.0000 g	5.0000 g	0.0000 g	0.13 mg
7	10.0000 g	10.0001 g	0.0001 g	0.14 mg
8	50.0000 g	50.0001 g	0.0001 g	0.15 mg
9 ¹	100.0000 g	100.0001 g	0.0001 g	0.20 mg
10 ¹	149.9999 g	150.0000 g	0.0001 g	0.31 mg
11 ¹	199.9998 g	199.9999 g	0.0001 g	0.35 mg

¹The calculated uncertainty was replaced by the CMC (Calibration and Measurement Capabilities) value because the calculated uncertainty was smaller than the CMC value.

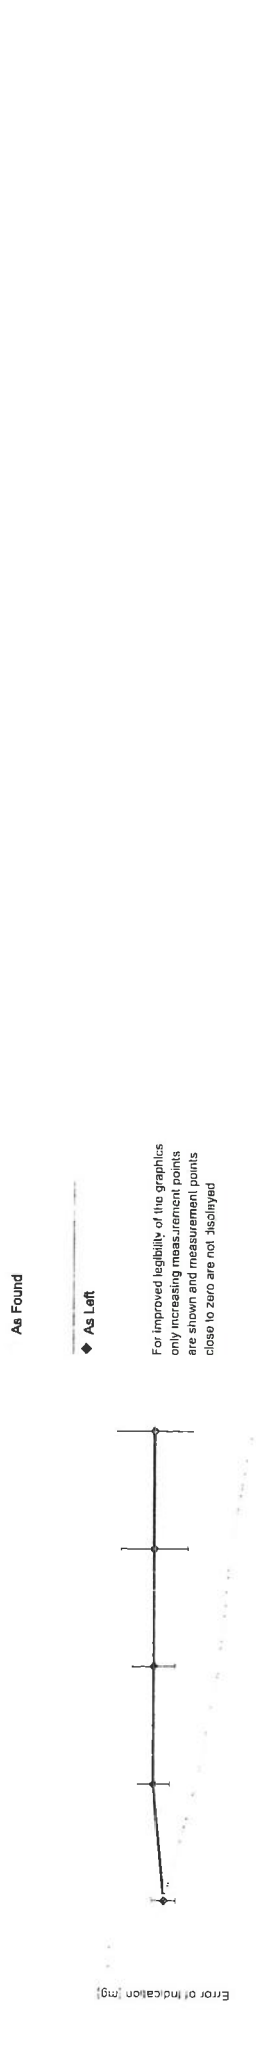

The uncertainty stated is the expanded uncertainty at calibration obtained by multiplying the standard combined uncertainty by the coverage factor k – which can be larger than 2 according to EURAMET cg-18. The value of the measurand lies within the assigned range of values with a probability of approximately 95%.

Measurement Uncertainty of the Weighing Instrument in Use

Stated is the expanded uncertainty with k=2 in use. The formula shall be used for the estimation of the uncertainty under consideration of the errors of indication. The value R represents the net load indication in the unit of measure of the device.

Temperature coefficient for the evaluation of the measurement uncertainty in use: 1.5 · 10⁻⁶ / K

Temperature range on site for the evaluation of the measurement uncertainty in use: 5 K


Uncertainty of Uncertainty Equation

1	Range		As Found	As Left
	d	Max		
1	0.0001 g	220 g	$U_1 = 0.13 \text{ mg} + 0.0101 \text{ mg/g} \cdot R$	$U_1 = 0.13 \text{ mg} + 0.00616 \text{ mg/g} \cdot R$

To optimize the stability of the linearization, besides of the zero load only increasing measurement points with a test load of 5% of the measurement range or larger are taken for the calculation of the linear equation.

Absolute and Relative Measurement Uncertainty in Use for Various Net Indications (Examples)

Net Indication	As Found		As Left	
	0.0220 g	0.13 mg	0.13 mg	0.59%
0.0220 g	0.2200 g	0.13 mg	0.13 mg	0.060%
2.2000 g	2.2000 g	0.15 mg	0.14 mg	0.0069%
22.0000 g	22.0000 g	0.35 mg	0.27 mg	0.0018%
220.0000 g	220.0000 g	2.4 mg	1.5 mg	0.0011%
				0.00068%

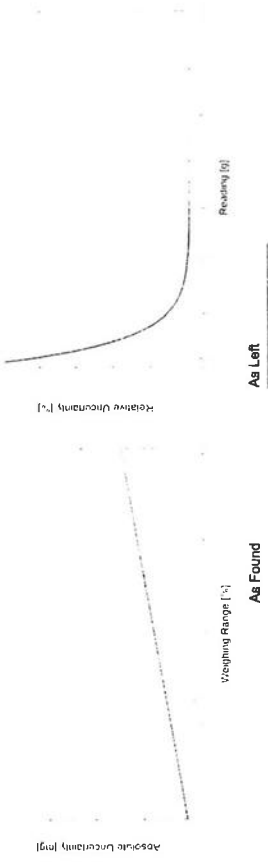

GWP®

Certificate



AS
Found

✓

AS
Left

✓


The weighing device meets the given process requirements.

The weighing device meets the given process requirements.

Tests Performed: As Found As Left

Process Requirements

Weighing Tolerance: 1% | Smallest Net Weight: 1.0000 g | Safety Factor: 2

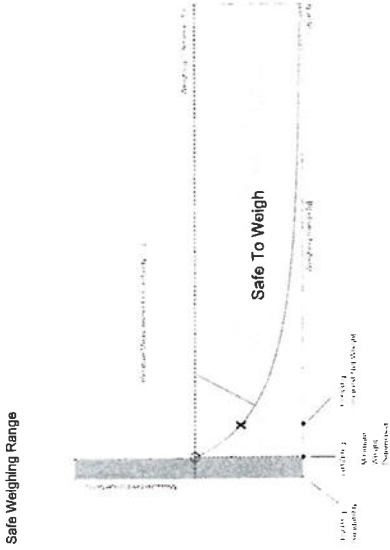

While the values in this graph reflect the actual calibration results, the measurement uncertainty curves are simply a visual representation. This graph reflects As Left testing, unless only As Found was performed.

COPY

Minimum Weight

As Found Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.13300 g	0.26873 g	0.40728 g	0.69320 g	1.46405 g
0.2%	0.06616 g	0.13300 g	0.20051 g	0.33764 g	0.69320 g
0.5%	0.02638 g	0.05288 g	0.07947 g	0.13300 g	0.26373 g
1%	0.01318 g	0.02638 g	0.03962 g	0.06616 g	0.13300 g
2%	0.00659 g	0.01318 g	0.01978 g	0.03300 g	0.06616 g
5%	0.00263 g	0.00527 g	0.00790 g	0.01318 g	0.02638 g

Pass: The determined minimum weight meets the requirement for the smallest net weight.

As Left Minimum Weight Table

Minimum weights for different weighing tolerances and safety factors					
Tolerance	Safety Factor				
	1	2	3	5	10
0.1%	0.12728 g	0.25614 g	0.38662 g	0.65256 g	1.34797 g
0.2%	0.06344 g	0.12728 g	0.19151 g	0.32118 g	0.65256 g
0.5%	0.02533 g	0.05072 g	0.07618 g	0.12728 g	0.25614 g
1%	0.01266 g	0.02533 g	0.03802 g	0.06344 g	0.12728 g
2%	0.00633 g	0.01266 g	0.01899 g	0.03167 g	0.06344 g
5%	0.00253 g	0.00506 g	0.00759 g	0.01266 g	0.02533 g

Pass: The determined minimum weight meets the requirement for the smallest net weight.

All these net minimum weight values, the measurement uncertainty of the weighing device is equal to or less than 1/1 (no safety factor), 1/2, 1/3, 1/5, or 1/10 of the required tolerance. The values are calculated with $k = 2$ and based on the linear formula of the measurement uncertainty of the weighing device in use.

The safety factor for As Found is always 1. This implies no safety factor. As Found testing looks at the behavior of the instrument from the past until test occurred. For the past, it is necessary to know that the tolerance was met, but not the safety factor. The safety factor is a proactive measure to apply for future measurements.

Notes on minimum weight values in above table:

- If "N/A" is shown above, no appropriate value could be calculated.
- METTLER TOLEDO is not responsible for the definition of the process requirements.

Measurement Results

Results Summary

Repeatability		Eccentricity		Error of Indication	
As Found	✓	As Found	✓	As Found	✓
As Left	✓	As Left	✓	As Left	✓

✓ = Passed

✗ = Failed

1. = Safety Factor not met

Repeatability

Test Load: 100 g

Tolerance		Control Limit		As Found		As Left	
				Std. Deviation	Result	Std. Deviation	Result
0.1%	0.00050 g	0.00050 g	✓		✓		✓
0.2%	0.00100 g	0.00100 g	✓		✓		✓
0.5%	0.00250 g	0.00250 g	✓		✓		✓
1%	0.00500 g	0.00500 g	✓	0.00005 g	✓	0.00005 g	✓
2%	0.01000 g	0.01000 g	✓		✓		✓
5%	0.02500 g	0.02500 g	✓		✓		✓

The weighing tolerance is met if the standard deviation is less than or equal to the corresponding control limit.

Eccentricity

Test Load: 100 g

Tolerance		Control Limit		As Found		As Left	
				Deviation	Result	Deviation	Result
0.1%	0.0500 g	0.0500 g	✓		✓		✓
0.2%	0.1000 g	0.1000 g	✓		✓		✓
0.5%	0.2500 g	0.2500 g	✓		✓		✓
1%	0.5000 g	0.5000 g	✓	0.0001 g	✓	0.0001 g	✓
2%	1.0000 g	1.0000 g	✓		✓		✓
5%	2.5000 g	2.5000 g	✓		✓		✓

The weighing tolerance is met if the deviation is less than or equal to the corresponding control limit.

Error of Indication

As Found

		Control limits for various weighing tolerances							
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%		
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A		
50.0000 g	-0.0003 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g		
100.0000 g	-0.0005 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g		
149.9999 g	-0.0006 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g		
199.9998 g	-0.0008 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g		
Result		✓	✓	✓	✓	✓	✓		

As Left

		Control limits for various weighing tolerances							
Reference Value	Error	0.1%	0.2%	0.5%	1%	2%	5%		
0.0000 g	0.0000 g	N/A	N/A	N/A	N/A	N/A	N/A		
50.0000 g	0.0001 g	0.0250 g	0.0500 g	0.1250 g	0.2500 g	0.5000 g	1.2500 g		
100.0000 g	0.0001 g	0.0500 g	0.1000 g	0.2500 g	0.5000 g	1.0000 g	2.5000 g		
149.9999 g	0.0001 g	0.0750 g	0.1500 g	0.3750 g	0.7500 g	1.5000 g	3.7500 g		
199.9998 g	0.0001 g	0.1000 g	0.2000 g	0.5000 g	1.0000 g	2.0000 g	5.0000 g		
Result		✓	✓	✓	✓	✓	✓		

The weighing tolerance is met if the error (of indication) for each test point is less than or equal to the corresponding control limit for that particular weighing tolerance. Results at or close to the zero point cannot be assessed.

COPY

ANALYTICAL BALANCE

Model : SECURA224-1S

Serial No. : 0036707137



Certificate No. : 23-148800

Sample Code : 23-56200-002

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
583 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Analytical Balance Room)

Equipment : ELECTRONIC BALANCE

Manufacturer : SARTORIUS

Model : SECURA224-1S

Serial No. : 0036707137

ID No. : LABE 05/2

Date of Receipt : 22 December 2023

Date of Calibration : 22 December 2023

Calibrated by Mr. Somwang Sangdee
Scientist

Issue date 25 December 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 23-148800

Sample Code : 23-56200-002

REPORT OF CALIBRATION

Equipment : ELECTRONIC BALANCE
Manufacturer : SARTORIUS
Model : SECURA224-1S
Capacity : Max 220 g
Resolution : 0.0001 g
Serial No. : 0036707137
ID No. : LABE 05/2

Result of Calibration

1. Test weight and repeatability of reading

Repeatability is a measure of the ability of a balance to supply the same result in repetitive weighings with one and the same load under the same measurement condition. The measurement of the repeatability must include both the balance specifications and the ambient (vibration, fluctuating air current/temperature/humidity, etc.) Operator handling of the balance is also included in the standard deviation.

Unit : g	Range : 220	<input checked="" type="checkbox"/> Before adjustment	<input checked="" type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	100 200 100 200	
<input checked="" type="checkbox"/> Adjustment	Standard weight	100.000042 200.000041 100.000042 200.000041	
	Average reading of indicator	99.9998 199.9998 100.0000 200.0000	
	Standard deviation	0.00006 0.00007 0.00003 0.00007	

Unit : -	Range : -	<input type="checkbox"/> Before adjustment	<input type="checkbox"/> After adjustment
<input type="checkbox"/> No adjustment	Nominal value	*	*
<input type="checkbox"/> Adjustment	Standard weight	*	*
	Average reading of indicator	*	*
	Standard deviation	*	*

COPY



Certificate No. : 23-148800

Sample Code : 23-56200-002

REPORT OF CALIBRATION

Result of Calibration

2. Sensitivity or value of a scale division

Change in the output variable of a measuring instrument divided by the associated change in the input variable.

Unit : g

Range : 220		Range :	
Test Point	Sensitivity, S	Test Point	Sensitivity, S
0	0.7980		
100	0.8978		
200	0.8978		

3. Departure of indication from nominal value, Linearity

Unit : g

Nominal Value	Standard Value	Average Reading of Indicator	Correction Value	Expanded Uncertainty	Coverage Factor (k)
Unload	0.0000000	0.0000	0.0000	0.000086	2.00
0.01	0.0100025	0.0100	0.0000	0.000086	2.00
0.1	0.1000019	0.1000	0.0000	0.000087	2.00
1	1.0000125	1.0000	0.0000	0.000087	2.00
2	2.0000089	2.0000	0.0000	0.000087	2.00
5	5.0000208	5.0001	-0.0001	0.000088	2.00
10	10.0000004	10.0000	0.0000	0.000090	2.00
20	20.0000030	20.0000	0.0000	0.000093	2.00
50	50.0000014	50.0000	0.0000	0.00011	2.00
100	100.0000042	100.0000	0.0000	0.00016	2.00
200	200.0000041	200.0000	0.0000	0.00028	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

COPY



Certificate No. : 23-148800

Sample Code : 23-56200-002


REPORT OF CALIBRATION

Result of Calibration :

4. Eccentric or off-centre loading

Deviation of the measurement value through off - center (eccentric) loading. The corner load increases with the weight of the load and its removal from the center of the pan support.

Weighing pan		Test weight : 100	
		Unit : g	
		Range	
		220	
Position	Reading of indicator	Reading of indicator	
1	100.0000	-	
2	100.0000	-	
3	100.0000	-	
4	99.9999	-	
5	100.0000	-	
6	100.0000	-	
Maximum difference		0.0001	

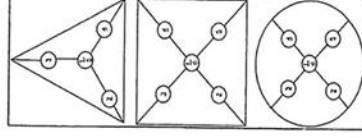

Condition of Calibration

1. Calibration Method : WI-CL-004 base on UKAS LAB 14: 2019

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. Condition of Calibration item: Normal

4. This certification is traceable to the International System of Unit maintained at : -
Through the reference standard laboratory of Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Instrument number 1).

5. Reference standard instrument :

Instrument

1) STANDARD WEIGHT 1 mg to 1 kg

Class ID.No.
E2 LB-WE-79Certificate No.
23-105642Due Date
10 September 2024

- End of Report -

COPY

Area Heat Stress Monitor

Model : QUESTemp 34

Serial No. : TEU080012



CALIBRATION CERTIFICATE

Certificate No. : L202306315-002
 Date Issued : 04-Jul-23

Customer : Eastern Thai Consulting 1992 Co., Ltd.
 683 Moo 11 Sukhapiarn 8 Rd., Nongkham, Siracha, Chonburi 20230

Equipment : Area Heat Stress Monitor

Manufacturer : TSI
Model : QUESTemp 34
Serial No. : TEU080012
ID No./Tag No. : NO.11
Date Received : 30-Jun-23
Date Calibrated : 02-Jul-23

Calibrated by : Mr. Apiwat Peanrungrat

Calibration Method or Calibration Procedure Used


In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter


This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: 
 (Mr. Sarayuth Tochua)



Page 1 of 2

Copy

Certificate No. : L202306315-002
 Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$
 Relative Humidity : $(50 \pm 15)\% \text{RH}$

STD Reading ($^\circ\text{C}$)	UUC Reading ($^\circ\text{C}$)		UUC Error ($^\circ\text{C}$)	Measurement Uncertainty ($\pm ^\circ\text{C}$)
	Before Adjusted	After Adjusted		
37.99	WET 37.9	-	-0.09	0.35
37.99	DRY 37.9	-	-0.09	0.35
37.99	GLOBE 37.9	-	-0.09	0.35
45.01	WET 45.3	-	0.29	0.35
45.01	DRY 45.2	-	0.19	0.35
45.01	GLOBE 45.1	-	0.09	0.35

STD = Standard

UUC = Unit Under Calibration

Description of UUC : Range 0 to 100 $^\circ\text{C}$
 Resolution 0.1 $^\circ\text{C}$

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202210258-006 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 10-Nov-23


End of Certificate

Copy

Area Heat Stress Monitor

Model : QUESTemp 34

Serial No. : TEU080011

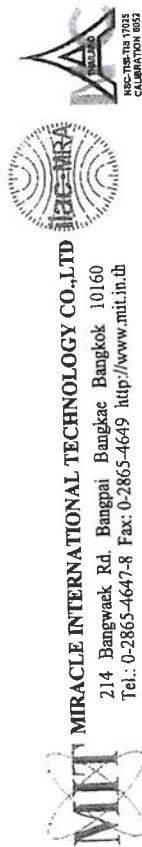

MIRACLE INTERNATIONAL TECHNOLOGY CO., LTD
214 Bangwaek Rd. Bangpai Bangkae Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : L202306315-001

Date Issued : 04-Jul-23

Customer : Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11 Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Area Heat Stress Monitor

Manufacturer : TSI
Model : QUESTemp 34
Serial No. : TEU080011
ID No./Tag No. : NO.10
Date Received : 30-Jun-23
Date Calibrated : 02-Jul-23

Calibrated by : Mr. Apiwat Peanrungrat

Calibration Method or Calibration Procedure Used

In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: *Saranyuth*
(Mr. Saranyuth Tochua)



Page 1 of 2

Certificate No. : L202306315-001

Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15)\%\text{RH}$

STD Reading ($^\circ\text{C}$)	UUC Reading ($^\circ\text{C}$)		UUC Error ($^\circ\text{C}$)	Measurement Uncertainty ($\pm^\circ\text{C}$)
	Before Adjusted	After Adjusted		
37.99	WET 37.9	-	-0.09	0.35
37.99	DRY 37.7	-	-0.29	0.35
37.99	GLOBE 37.9	-	-0.09	0.35
45.01	WET 44.9	-	-0.11	0.35
45.01	DRY 44.8	-	-0.21	0.35
45.01	GLOBE 45.0	-	-0.01	0.35

STD = Standard

UUC = Unit Under Calibration

Description of UUC :
Range 0 to 100 $^\circ\text{C}$
Resolution 0.1 $^\circ\text{C}$

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202210258-006 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 10-Nov-23

End of Certificate

COPY

Area Heat Stress Monitor

Model : HD32.2

Serial No. : 22004316



NSC-TISI-TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-040-67

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : Delta OHM
MODEL/TYPE : HD32.2
SERIAL NUMBER : 22004316
ID NUMBER :
CONDITION AS-RECEIVED :
CUSTOMER : Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriacha, Chonburi 20230

RECEIVED DATE : 08 Feb 2024
MEASUREMENT DATE : 12 Feb 2024
ISSUE DATE : 16 Feb 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Page 1 of 2 Pages

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CT-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0038-23, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 28 Mar 2024
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:


- ☐ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol
☒ Miss Ruangrumpai Phoommit

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



End of Certificate of Calibration



COL

Continuation of Certificate of Calibration Number CDT-040-67

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 22010213.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.052	20.1	0.0	0.099
80	25.057	25.1	0.0	0.099
80	30.042	30.1	0.1	0.099
80	35.032	35.1	0.1	0.099
80	40.018	40.1	0.1	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 22010923.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.052	20.1	0.0	0.099
110	25.057	25.1	0.0	0.099
110	30.042	30.1	0.1	0.099
110	35.032	35.1	0.1	0.099
110	40.018	40.1	0.1	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2 S/N: 22015193.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.052	20.0	-0.1	0.099
75	25.057	25.0	-0.1	0.099
75	30.043	29.9	-0.1	0.099
75	35.032	34.9	-0.1	0.099
75	40.017	39.8	-0.2	0.099

UUC*: Unit Under Calibration

Area Heat Stress Monitor

Model : QUESTemp 32

Serial No. : TPL060040



CALIBRATION CERTIFICATE

Certificate No. : L202305299-010
Date Issued : 07-Jun-23

Customer : Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11 Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Area Heat Stress Monitor

Manufacturer : Quest Technologies
Model : QUESTemp 32
Serial No. : TPL060040
ID No./Tag No. : NO.5
Date Received : 29-May-23
Date Calibrated : 05-Jun-23

Calibrated by : Mr. Apiwat Peanrungrat

Calibration Method or Calibration Procedure Used


In-house method : CP-19 by comparing against Standard Digital Humidity / Temperature Meter

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: 
(Mr. Sarayuth Tothua)



COPY

Certificate No. : L202305299-010
Environment : Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15)\% \text{RH}$

STD Reading ($^\circ\text{C}$)	UUC Reading ($^\circ\text{C}$)		UUC Error ($^\circ\text{C}$)	Measurement Uncertainty ($^\circ\text{C}$)
	Before Adjusted	After Adjusted		
38.00	WET 38.0	-	0.00	0.35
38.00	DRY 38.0	-	0.00	0.35
38.00	GLOBE 37.9	-	-0.10	0.35
44.99	WET 45.0	-	0.01	0.35
44.99	DRY 45.1	-	0.11	0.35
44.99	GLOBE 44.8	-	-0.19	0.35

STD = Standard
UUC = Unit Under Calibration

Description of UUC : Range 0 to 100 $^\circ\text{C}$
Resolution 0.1 $^\circ\text{C}$

Condition As-Received : Used Item
The measurement results and statements of conformity with specification only relate to the item calibrated.
Measurement Standards Used & Traceability :
The International System of Units (SI) through

MIT Certificate No. L202210258-006 for Digital Thermometer with Probe (Fluke) Serial No. 5856603, Due 10-Nov-23

End of Certificate

COPY

BAROMETER

Equipment : Analog Barometer

ID No. / Tag No. : BM001/41

CALIBRATION CERTIFICATE



Certificate No. : L202305085-002
 Date Issued : 16-May-23

Customer : Eastern Thai Consulting 1992 Co., Ltd.
 683 Moo 11 Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230

Equipment : Analog Barometer

Manufacturer : Barigo
Model : -
Serial No. : -
ID No./Tag No. : BM001/41
Date Received : 11-May-23
Date Calibrated : 15-May-23
Calibrated by : Mr. Jame Khaothong

Calibration Method or Calibration Procedure Used

In-house method : CP-21 base on DKD-R 6-1: Edition 3 2014.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by: *Sorayuth*
 (Mr. Sarayuth Tochua)



COPY

Certificate No : L202305085-002
 Environment : Ambient Temperature : (25 ± 2)°C
 Relative Humidity : (50 ± 15)%RH

STD Reading mbar	UUC Reading (mbar) Before Adjusted	UUC Reading (mbar) After Adjusted	UUC Error mbar	Uncertainty ± mbar
990.00	990.0	-	0.00	0.61
1000.00	1000.0	-	0.00	0.61
1010.00	1010.0	-	0.00	0.61
1020.00	1020.0	-	0.00	0.61
1030.00	1030.0	-	0.00	0.61

STD = Standard

UUC = Unit Under Calibration

Calibrated condition : Pressure Medium : Air : Density = 1.19 kg/m³ @ 20°C, 1 bar
 Mounting Position : Vertical
 Reference Level : at center of its dial
 Conversion Factor : Multiply by 1.0 E+02 - Pa unit

Description of UUC :

Range	990 - 1030	mbar Absolute
Calibration Range	990 - 1030	mbar Absolute
Scale Interval	1	mbar
Resolution	0.5	mbar Absolute

Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

IRPC Certificate No. CL1-P220104 for Reference Pressure Monitor Serial No. 1598, Due 11-Nov-23

End of Certificate

COPY

BOD INCUBATOR

Model : TC445S

Serial No. : 0223/007275

SK

S K SALES AND SERVICE CO.,LTD.
194/56, 194/57 Thakkom Rd. Sornae Dam
Bung Khun Thien Bangkok 10150
Tel : 02-417-2144 Fax : 02-417-2155



Certificate of Calibration

Reference No. : C03190/2309-025
Customer : Eastern Thai Consulting 1992 Co., Ltd.
Equipment : 883 Moo 11, Sukhaphiban 8, Tambol Nongkham,
Manufacturer : Siracha District, Chonburi 20230, Thailand
Model : Incubator
Serial No. : Lovibond
ID No. : TC445S
Received Date : 0223/007275
Calibrated Date : 15 September 2023
Issued Date : 15 September 2023
Environment : 18 September 2023

Ambient Temperature (°C)	27.5	Minimum Value	28.1	Maximum Value
Relative Humidity (% RH)	57		58	
AC Line Voltage (VAC)	224		226	
Place Of Calibration	Production Line			
Calibrated by	Mr. Teerasak Chalaporn			

Calibration Method

In-house method : SK-WI-23 base on Thai Laboratory Accreditation Scheme Publication Reference G-20

Condition of this result of calibration

- Reference standard instrument
- 1) Data acquisition/Switch unit
2) Multiplexer Module
- This result of calibration was found accurate as shown on date and place of calibration only
- This certificate can be traceable to International System of Unit :
- Through Thailand Institute of Scientific And Technological Research (TISTR)

Approved by

☒ Mr. Supachai Saksri ☐ Mr. Phayak Toolit ☐ Miss Tanjaraporn Pettong

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2.0$ providing a level of confidence level of approximately 95 %

This certificate may not be reproduced other than in full except with the prior written approval of the S K Sales And Service Company Limited

COPY

Certificate No. : S2309-3014

Page 2 of 2

Table1 General Information

Working Area (W*L*H) Fresh Air	60 *56 *1.45 cm OFF
-----------------------------------	------------------------

Table2 Chamber Performance


Setting Temperature (°C)	Average Indicating Temperature (°C)	Measured Stability (± °C)	Measured Uniformity (°C)	Overall Variation (°C)
20.0	20.0	0.37	0.64	0.98

Table3 Temperature Distribution

Setting Temperature (°C)	Average Standard Reading (°C)									Uncertainty (± °C)
	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9	
20.0	19.52	19.40	19.70	19.43	19.33	19.39	19.45	19.58	19.67	0.55

Resolution : 0.1 (°C)

* Probe No. 9 is Reference Probe



- Notes :
- The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.
 - The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time
 - Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.
 - The reported uncertainty of measurement were excluded Uniformity and Stability

** End of Calibration Report **

COPY

[Signature]

CERTIFICATE OF ANALYSIS

EPA PROTOCOL GAS

Cylinder No. : EB0145030

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E03NI99E15AC0U4
Cylinder Number: EB0145030
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12021
Gas Code: CH4,PPN,BALN

Reference Number: 160-40224242-1
Cylinder Volume: 144.4 CF
Cylinder Pressure: 2015 PSIG
Valve Outlet: 350
Certification Date: Oct 15, 2021

Expiration Date: Oct 15, 2029

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 000/R-12/021, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS				
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty
METHANE	180.0 PPM	177.0 PPM	G1	+/- 1.0% NIST Traceable
PROPANE	185.0 PPM	187.0 PPM	G1	+/- 1.0% NIST Traceable
NITROGEN	Balance			
ANALYTICAL DATES				
				10/15/2021
				10/15/2021
CALIBRATION STANDARDS				
Type	Lot ID	Cylinder No	Concentration	Uncertainty
NTRM	08011503	K002564	246.7 PPM METHANE/AIR	+/- 0.6%
NTRM	200602-06	6162660Y	243.3 PPM PROPANE/AIR	+/- 0.5%
ANALYTICAL EQUIPMENT				
Instrument/Make/Model			Last Multipoint Calibration	
Nicolet iS50 FTIR AUP2110295 CH4			Oct 13, 2021	
Nicolet iS50 FTIR AUP2110295 C3H8			Oct 14, 2021	

Triad Data Available Upon Request

NOTES:
Gross Weight: 28.0 Kg
Net Weight: 4.9 Kg
PO# 5221004851



COPY

Michael A. Huber
Approved for Release

CERTIFICATE OF ANALYSIS

EPA PROTOCOL GAS

Cylinder No. : EB0062815

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04N199E15ACX9C Reference Number: 82-401135335-1
Cylinder Number: EB0062815 Cylinder Volume: 144.4 CF
Laboratory: 124 - Riverton (SAP) - NJ Cylinder Pressure: 2015 PSIG
PGVP Number: B52018 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO2,BALN Certification Date: Mar 13, 2018
Expiration Date: Mar 13, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals

ANALYTICAL RESULTS				
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty
NOX	50.00 PPM	50.55 PPM	G1	+/- 1.4% NIST Traceable
NITRIC OXIDE	50.00 PPM	50.50 PPM	G1	+/- 1.4% NIST Traceable
SULFUR DIOXIDE	50.00 PPM	51.01 PPM	G1	+/- 1.0% NIST Traceable
CARBON MONOXIDE	2000 PPM	1977 PPM	G1	+/- 1.0% NIST Traceable
NITROGEN	Balance			
Assay Dates: 03/06/2018, 03/13/2018, 03/06/2018, 03/13/2018, 03/06/2018, 03/13/2018				
CALIBRATION STANDARDS				
Type	Lot ID	Cylinder No	Concentration	Uncertainty
NTRM	10080807	CC442554	50.42 PPM NITRIC OXIDE/NITROGEN	+/- 0.8%
PRM	12367	APEX1099237	9.82 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%
GMS	0315201604	CC503358	4.975 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.5%
NTRM	16011025	CC473218	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.5%
NTRM	12060735	CC356192	2486 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%
The SRM, PRM or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.				
Expiration Date: Jun 27, 2020, Jun 02, 2017, Mar 15, 2019, Jun 07, 2022, Dec 14, 2026				
ANALYTICAL EQUIPMENT				
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration		
Nicolet 6700 APW1100391 CO	FTIR	Feb 08, 2018		
Nicolet 6700 APW1100391 NO	FTIR	Feb 15, 2018		
Nicolet 6700 APW1100391 NO2	FTIR	Feb 16, 2018		
Nicolet 6700 APW1100391 SO2	FTIR	Mar 01, 2018		

Triad Data Available Upon Request

NOTES: NET WEIGHT: 10.43lbs
GROSS WEIGHT: 60.93lbs
PO# 5218000763

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol. Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2000 and relate only to items identified on this certificate. All concentrations are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



TESTING CERT No. 3082.05

Donna Morris
Approved for Release

DRY GAS METER XC-572-OV

Serial No. : A2204323



WISDOM SCIENCE

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m³)

Meter Console Information

Console Model : XC-572-OV
 Console serial : A2204323
 DGM Model #: SK25EX
 DGM Serial #: 00008294

Calibration Condition

Calibration Date: 2-May-2023
 Due Date: 1-May-2024
 Cal. Report No.: WDS-SV660066
 Ambient Temp (°C): 25
 Pressure (mm Hg): 758
 Relative Humidity (%): 55

Factors/Conversion

Std. Temp. (°K): 298
 Std. Pressure (mm Hg): 760
 K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B
 WTM Serial: 600245
 WTM Cal. Date: 22-Nov-2022
 Gamma: 1.0000

UUT Meter (DGM)

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15.00	13.0	18.0685	18.2252	25	26	17.55844	17.71573	25	25
10.00	25.0	18.2477	18.3984	25	26	17.73637	17.88948	25	25
8.00	50.0	18.4339	18.6056	25	26	17.92517	18.09730	25	25
7.00	80.0	18.6458	18.8344	25	27	18.13775	18.32707	25	25
5.00	120.0	18.8839	19.0510	25	27	18.37705	18.54528	25	25

Standardized Data

Test Meter		Reference Meter		Correction Factor		Calibration Results		
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Flow Rate	0.0212 SCMM	ΔH@
V _{mstd} (m ³)	Q _{mstd} m ³ /min	V _{wstd} (m ³)	Q _{wstd} m ³ /min	(Y)	(ΔY)	Q _{mstd} (cor)	ΔH _e	ΔΔH _e
0.154	0.010	0.154	0.010	1.004	0.003	0.010	54.437	3.293
0.148	0.015	0.148	0.015	1.002	0.001	0.015	50.528	-0.616
0.169	0.021	0.169	0.021	0.999	-0.001	0.021	50.086	-1.058
0.186	0.027	0.186	0.027	0.999	-0.001	0.027	50.928	-0.216
0.165	0.033	0.165	0.033	0.999	-0.002	0.033	49.741	-1.403
				1.001	= Y Avg.		51.144	= ΔH@ Avg.

Pass/Fail Result: PASS

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance for individual values from the average is ±0.02
 Note: For ΔH_e, orifice pressure differential that equates to 0.75cm (0.0212m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ±0.2inches (5.1mm) H₂O.

Approved By:


(Palpasu Chaisana)
 Service Manager

บริษัท วิสโดม สไซน์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

Date:

2-May-2023

Meter Gamma vs Flowrate

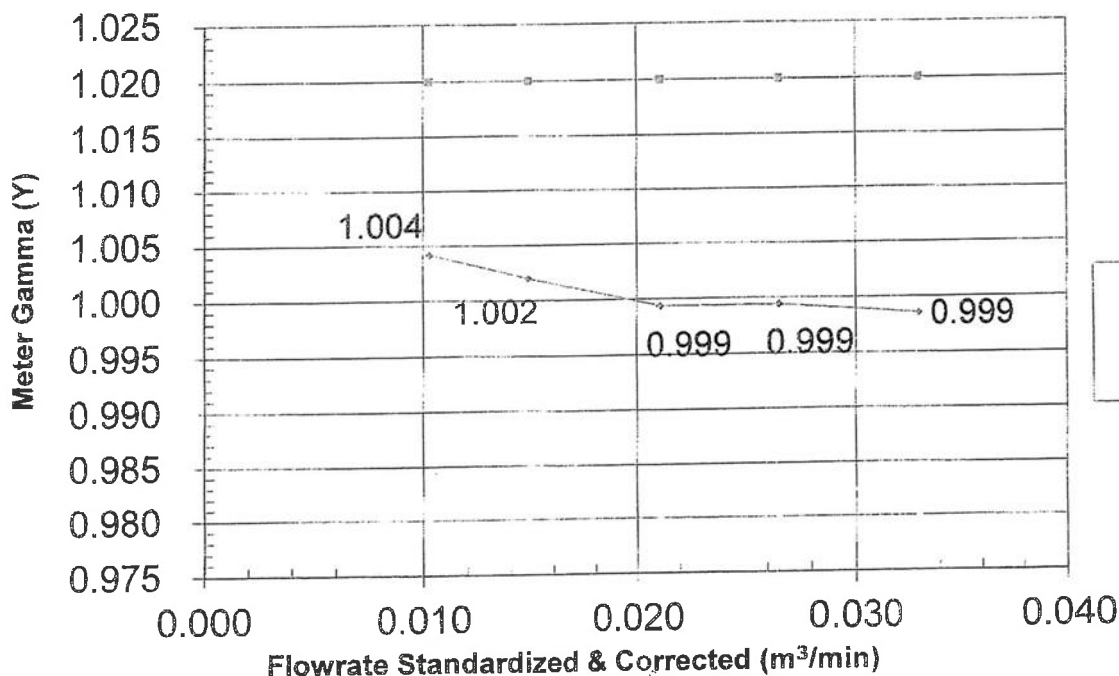

Console Serial:

A2204323

Console Model:

XC-572-OV

WISDOM SCIENCE
 บริษัท วิสโดม สไซน์ แอนด์ เซอร์วิส กรุ๊ป จำกัด
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY



WISDOM SCIENCE

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information

Console Model: XC-572-OV
Console Serial: A2204323
Temp Indicator Model: 765-KF
Temp Indicator Serial: JC19022

Calibration Conditions

Cal. Date: 2-May-2023
Due Date: 1-May-2024
Cal. Report No.: WDS-SV60066
Ambient Temp. (°C): 25
Pressure (mm Hg): 758
Humidity (%): 55

Reference Equipment

Temp. Simulator Model: FLUKE 714B
Serial No.: 60590035
Calibration Date: 14-Feb-2023

Temperature Sensor Calibration

Reference Point	Ref Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
1	-18.0	-17.0	1.0
2	25.0	25.0	0.0
3	90.0	90.0	0.0
4	120.0	120.0	0.0
5	250.0	249.0	1.0
6	380.0	380.0	0.0
7	500.0	500.0	0.0
8	620.0	620.0	0.0
9	740.0	739.0	1.0
10	860.0	860.0	0.0
Maximum ¹			1.0

Note

¹ For valid test results, the maximum difference between temperature readings should $\leq 1.0^{\circ}\text{C}$ (EPA Method 5, Section 6.1.1.8).
Perform AUX, STACK, PROBE, OVEN, FILTER, EXIT. Except meter (DGM) channel

DGM Out Temperature Sensor Calibration

Temperature point	Ref Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
Ambient	28.8	29.0	-0.2
Heat	100.0	101.3	-1.3

Difference Range


DGM Out Temp. Diff. $\pm 3^{\circ}\text{C}$

Approved By :

(Pattusu Chalsana)
Service Manager

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED
Address 9/115 Lumpini Town Ville Ratchaphruek-Pinklao Village No. 4, Bang Kharun, Bang Kruai, Nonthaburi 11130 Thailand

Meter Pressure vs Flowrate

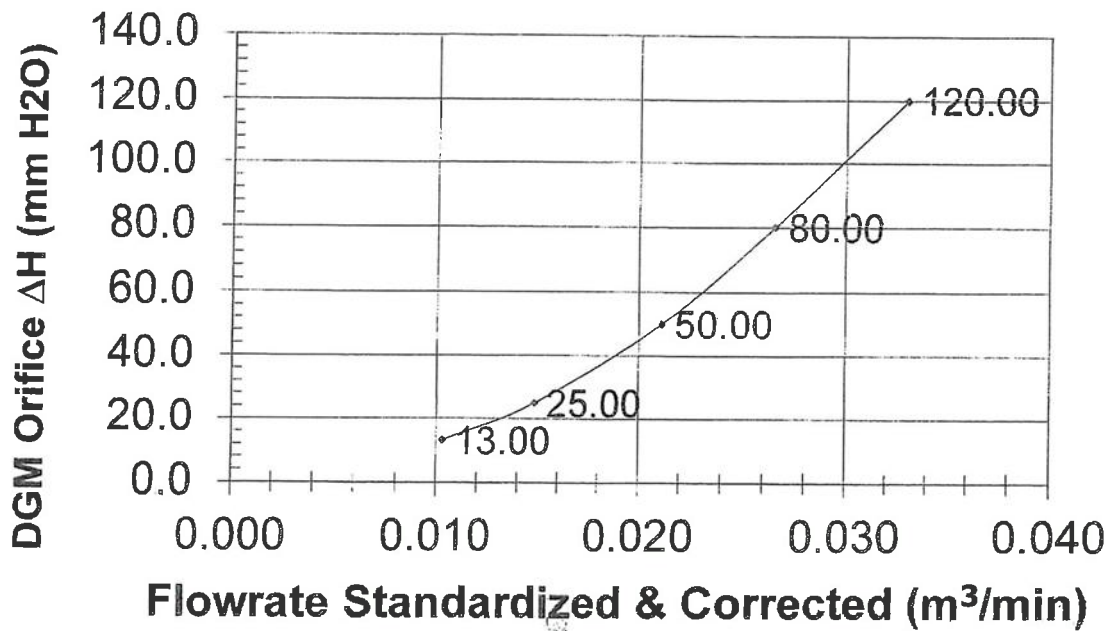

Console Serial:

A2204323

Console Model:

XC-572-OV

WISDOM SCIENCE

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY

COPY

DRY GAS METER XC572V

Serial No. : 1110070

Certificate Of Calibration

Method 5 Pre-Test Console Calibration - Cubic meter (m3)

Meter Console Information

Console Model: XC572V
 Console serial: 1110070
 DGM Model #: SK25EX
 DGM Serial #: 0005413

Calibration Condition

Calibration Date: 3-Jul-23
 Due Date: 2-Jul-24
 Cal Report No: WDS-SV660107
 Ambient Temp (°C): 25
 Pressure (mm Hg): 758
 Relative Humidity (%): 60

Factors/Conversion

Std Temp (°C): 298
 Std. Pressure (mm Hg): 760
 K₁ (K/mm Hg): 0.3857

Reference Equipment

WTM Model: W-NKoDa-5B
 WTM Serial: 600245
 WTM Cal Due Date: Nov. 2022
 Gamma: 1.0000

UUT Meter (DGM)

Run Time (minutes)	DGM Orifice (mm H ₂ O)	Volume		Outlet Temp		Volume		Outlet Temp	
		Initial	Final	Initial	Final	Initial	Final	Initial	Final
15:00	13.0	599.3828	599.5462	27	27	20.05690	20.22163	28	27
10:00	25.0	599.5689	599.7246	27	26	20.24425	20.39999	27	27
8:00	50.0	599.7405	599.9176	26	25	20.41592	20.59344	27	27
7:00	80.0	599.9333	600.1337	26	26	20.60920	20.81034	27	27
5:00	120.0	600.1559	600.3319	26	26	20.83271	21.00950	27	27

Reference Meter (WTM)

Standardized Data

Calibration Results

Test Meter		Reference Meter		Correction Factor		Flow Rate		VH@ (mm H ₂ O)	
Std. Volume	Std. Flow Rate	Std. Volume	Std. Flow Rate	"Gamma"	Variation	Std & Corr	0.0212 SCMM	Variation	
V _{test} (m ³)	Q _{test} m ³ /min	V _{ref} (m ³)	Q _{ref} m ³ /min	(Y)	(ΔY)	Q _{corrected}	ΔH ₀	ΔΔH ₀	
0.159	0.011	0.160	0.011	1.005	0.010	0.011	50.191	2.747	
0.152	0.015	0.152	0.015	0.996	0.000	0.015	48.096	0.662	
0.174	0.022	0.173	0.022	0.995	-0.001	0.022	47.805	0.171	
0.197	0.028	0.196	0.028	0.993	-0.003	0.028	45.688	-1.747	
0.174	0.035	0.172	0.034	0.990	-0.006	0.034	45.602	-1.832	
				0.996	Y Avg		47.434	ΔH@ Avg	

Pass/Fail Result: **Pass**

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance for individual values from the average is ±0.02.
 Note: For ΔH₀, orifice pressure differential that equates to 0.75cm H₂O (0.0272mm Hg) at standard temperature and pressure. Acceptable tolerance for individual values from the average is ±0.2inches (5.1mm) H₂O.

Approved By: _____

(Patpasu Chaisana)
 Service Manager

Date: 3-Jul-23

COPY

TEMPERATURE DISPLAY CALIBRATION

Meter Console Information		Calibration Conditions		Reference Equipment	
Console Model	XC572V	Cal Date	3-Jul-23	Temp Simulator Model	FLUKE 71HB
Console serial	1110070	Due Date	2-Jul-24	Serial No	60590035
Temp Indicator Model	765-KF	Cal Report No	WDS-SV660107		
Temp Indicator Serial	JC17852	Ambient Temp (°C)	25		
		Pressure (mm Hg)	758		
		Humidity (%)	60		

Temperature Sensor Calibration

Reference Point	Ref. Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
1	-18.0	-17.0	1.0
2	38.0	37.0	1.0
3	93.0	93.0	0.0
4	149.0	149.0	0.0
5	260.0	259.0	1.0
6	371.0	372.0	-1.0
7	482.0	482.0	0.0
8	593.0	594.0	-1.0
9	816.0	816.0	0.0
10	1038.0	1039.0	-1.0
		Maximum	1.0

PASS

Note

* For valid test results, the maximum difference between temperature readings should be ±1.0°C (EPA Method 5, Section 6.1.1.8).
 Perform all TC Channel calibrations. Except meter (DGM) channel.

DGM Out Temperature Sensor Calibration

Temperature point	Ref. Thermometer Temperature °C	Thermocouple Display Temperature °C	Temperature Difference °C
#			
Ambient	26.5	27.0	-0.5
Heat	100.5	102.5	-2.0

Difference Range
 DGM Out Temp. Diff. ±3 °C

PASS

Approved By: _____

(Patpasu Chaisana)
 Service Manager

WISDOM SCIENCE
 WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED

COPY



WISDOM SCIENCE

Calibration Conditions

Model #: XC572V

Serial #: 1110070

Elapsed Timer Model #: C342-1464

Elapsed Timer Serial #	Time
1	0.000000
2	0.000000
3	0.000000
4	0.000000
5	0.000000
6	0.000000
7	0.000000
8	0.000000
9	0.000000
10	0.000000
11	0.000000
12	0.000000
13	0.000000
14	0.000000
15	0.000000
16	0.000000
17	0.000000
18	0.000000
19	0.000000
20	0.000000
21	0.000000
22	0.000000
23	0.000000
24	0.000000
25	0.000000
26	0.000000
27	0.000000
28	0.000000
29	0.000000
30	0.000000
31	0.000000
32	0.000000
33	0.000000
34	0.000000
35	0.000000
36	0.000000
37	0.000000
38	0.000000
39	0.000000
40	0.000000
41	0.000000
42	0.000000
43	0.000000
44	0.000000
45	0.000000
46	0.000000
47	0.000000
48	0.000000
49	0.000000
50	0.000000
51	0.000000
52	0.000000
53	0.000000
54	0.000000
55	0.000000
56	0.000000
57	0.000000
58	0.000000
59	0.000000
60	0.000000
61	0.000000
62	0.000000
63	0.000000
64	0.000000
65	0.000000
66	0.000000
67	0.000000
68	0.000000
69	0.000000
70	0.000000
71	0.000000
72	0.000000
73	0.000000
74	0.000000
75	0.000000
76	0.000000
77	0.000000
78	0.000000
79	0.000000
80	0.000000
81	0.000000
82	0.000000
83	0.000000
84	0.000000
85	0.000000
86	0.000000
87	0.000000
88	0.000000
89	0.000000
90	0.000000
91	0.000000
92	0.000000
93	0.000000
94	0.000000
95	0.000000
96	0.000000
97	0.000000
98	0.000000
99	0.000000
100	0.000000

Cal. Date : _____

Due Date

Cal. Report No.

Ambient Temp. (°C):

Humidity (%) :

Humidity (%): —

Reference Equipment

Calibration Standard: JS-307

Method Reference ^a	Compare
-------------------------------	---------

[illegible]

Approved By

(Patpasu Chaisana)
Service Engineer



U.S. Patent 4,211,000

Y
L
C
C

WISDOM SCIENCE SALE AND SERVICE GROUP COMPANY LIMITED
Address 9/115 Luangprabang Town Villa Ratchapiruek-Pinklao Village, No. 4, Bang Khanun, Bang Kruat, Nonthaburi 11130 Thailand
Tel 090 660-1392, 084-598-1944, 084-704-1620

Flue gas Analyzer

Testo 350 NEW

Serial No. 63455616/0722



Calibration Certificate

Certificate No: G 660489
Date of issue : 17-Aug-23

Where

Instrument description : Flue Gas Analyzer
Instrument model : Testo 350 New
Instrument serial no. : 63455616/0722
Control unit serial no. : 0360017/0722
ID no. or control no. : -
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial : -
Customer name : Eastern Thai Consulting 1992 Company Limited
Customer address : 683 Moo 11, Sukhapibarn 8 Road, Nongkham, Si Racha, Chon Buri 20280

Total pages of certificate : 2 Pages
Receiving no. : L-232625
Receiving date. : 10-Aug-23

Parameter of calibration : Gas Calibration (Oxygen 2.498, 10.04, 21.02 %Vol, Carbon Monoxide 80.14, 302, 1003 ppm, Nitrogen Dioxide 80.96 ppm, Nitric Oxide 151.5 ppm, Sulphur Dioxide 100.8 ppm)

Condition of UUC. : Used
Ambient condition : All of the Measurement were carried out the stabilized laboratory
Temperature : 23 ± 5 °C
Humidity : 55 ± 15 %RH

Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210

Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration work instruction no. WI-CL-28-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. This certificate is applied only to item under test Environmental condition.
This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.
This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).

Date of calibration : 17-Aug-23

Kwancheep
Mr. Kwanchai Khamdoun
Calibration Technician

W. W. W.
Mrs. Nongluck Wongsettee
Technical Manager



Calibration Certificate

Certificate No.: G 660489

Where

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 2.498 % Vol	4219/21	Linde	30-Sep-25
Oxygen (O2) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen (O2) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.14 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 302 ppm	2583/22	Linde	09-Aug-24
Nitrogen Dioxide (NO2) 80.96 ppm	3240/21	Linde	26-Jun-24
Nitric Oxide (NO) 151.5 ppm	0161/23	Linde	22-Jan-25
Sulphur Dioxide (SO2) 100.8 ppm	3507/22	Linde	09-Nov-24

Measured room conditions

Calibration conditions
Temperature : 23.8 °C Humidity : 62.1 %RH Pressure : 1008.9 mbar
Gas Temperature : 24 °C Flow rate : 1,300 ml/min Gas pressure : 1016.8 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.498	2.55	0.052	0.15
O2 (%Vol)	10.04	10.11	0.07	0.20
O2 (%Vol)	21.02	21.14	0.12	0.30
CO (ppm)	80.14	80	-0.14	3.0
CO (ppm)	302	302	0	6.0
CO (ppm)	1003	999	-4	12
*NO2 (ppm)	80.96	81.5	0.54	8.0
*NO (ppm)	151.5	150	-1.5	8.0
*SO2 (ppm)	100.8	100	-0.8	6.0

Remark : 1 cmol/mol = 1 %vol, 1 μmol/mol = 1 ppm.

* Calibrations marked Not TSI Accredited "in this Certificate have been included for completeness."

End of Report

Hot Air Oven

Model : UM 400

Serial No. : 900982



CERTIFICATE OF CALIBRATION

Page 1 of 3

Certificate No. : 24-001944

Sample Code : 24-00963-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
683 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Siracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.
(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)
Manufacturer : Memmert : UM 400
Serial No. : 900982 : ID No. : LABE 17/1
Date of Receipt : 09 January 2024 : Date of Calibration : 09 January 2024

Condition of Calibration

1. Environment : 1.1 Ambient temperature : Maximum 30.6 °C : Minimum 29.2 °C
: 1.2 Relative humidity : Maximum 57.5 % : Minimum 48.4 %
: 1.3 Line voltage supplied : Maximum 229.5 VAC : Minimum 222.5 VAC

2. Calibration method

TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument

Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-P1100)	LB-DA-10 (RTD-257 to RTD-265)	23-066256	29 June 2024

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Mr. Sarawoot Thammo
Scientist

Approved by

(Mr. Somchai Neampunt)
Signed for Director

Issue date

09 January 2024

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



REPORT OF CALIBRATION

Page 2 of 3

Certificate No. : 24-001944

Sample Code : 24-00963-001

Results of Calibration

Resolution : 0.1 °C

1. Reporting of Temperature

Calibration point (°C)	UUC* setting (°C) reading (°C)	Measured temperature at each positions (°C)										Uncertainty ± (°C)	Coverage factor k
		# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	# 10		
60	60.0	60.04	59.90	59.81	59.84	59.47	59.91	60.08	59.98	59.87	59.87	0.25	2.00
85	85.0	86.07	85.75	85.58	85.62	84.69	85.83	86.28	85.94	85.77	85.77	0.34	2.00

2. Characterization results

Calibration point (°C)	Stability ± (°C)	Uniformity (°C)	Overall variation (°C)
60	0.11	0.49	0.80
85	0.09	1.13	1.72

Notes

UUC* = Unit Under Calibration

COPY



REPORT OF CALIBRATION


Certificate No. : 24-001944

Sample Code : 24-00963-001

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 40 cm ; D = 28 cm ; H = 39 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

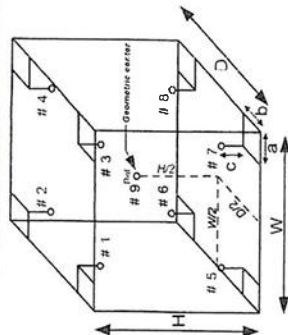Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003.

- End of Report -

COPY

Hot Air Oven

Model : UFE 500

Serial No. : G511.0182

REPORT OF CALIBRATION

Results of Calibration

Resolution : 0.5 °C

1. Reporting of Temperature

Calibration point (°C)	UUC: setting (°C)	UUC: reading (°C)	UUC*	Measured temperature at each positions (°C)								Uncertainty \pm (°C)	Coverage factor k	
				# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8			# 9 ^{low}
104	103.5	103.5	103.5	104.11	103.94	103.85	103.84	103.97	103.93	103.64	103.51	104.23	0.47	2.00

2. Characterization results

Calibration point (°C)	Stability \pm (°C)	Uniformity (°C)	Overall variation (°C)
104	0.04	0.78	0.81

Notes

UUC* = Unit Under Calibration

7

CERTIFICATE OF CALIBRATION

Page 1 of 3

Certificate No. : 23-148804

Sample Code : 23-56200-006

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapibarn 8 Rd., Nongkham,

Sriracha, Chonburi 20230

Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.

(Hot Lab)

Equipment : Temperature controlled enclosures (Hot air oven)

Manufacturer : Memmert Model : UFE 500

Serial No. : G511.0182
ID No. : LABE 17/4

Date of Receipt : 22 December 2023
Date of Calibration : 22 December 2023

Condition of Calibration

- | 1. Environment | | Ambient temperature | | 29.6 °C | |
|----------------|-----------------------|---------------------|-------|---------|---------|
| 1.1 | Relative humidity | Maximum | 30.9 | °C | Minimum |
| 1.2 | Relative humidity | Maximum | 54.5 | % | Minimum |
| 1.3 | Line voltage supplied | Maximum | 227.5 | VAC | Minimum |

2. Calibration method

Calibration method
TLAS-G-20: Guidelines for calibration and checks of temperature controlled enclosures.

3. Reference standard instrument


Instrument	ID No.	Certificate No.	Due Date
Data Acquisition With Sensor (RTD-Pt100)	LB-DA-08 (RTD-248 to RTD-256)	23-084070	06 August 2024

4. This certificate is traceable to the international system of unit (SI Unit).

The measurement is traceable to Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal



(Mr. Somchai Neampunt)
Signed for Director

Issue date	25 December 2023
------------	------------------

The uncertainties are for a confidence probability of approximately 95%

The uncertainties are for a confidence probability of approximately 95%. The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be

351 So1 Ladorado 022 L adorno Road,
Phahphah, Wang Thonglang, Bangkok 10310
TEL 02-516-2422
FAX 02-516-6949
Rev 01
CONTACT@AMARC.CO.TH
WWW.AMARC.CO.TH
Effective Date: 15/10/21
FW-CL-TH

361 Soi Ladprao 122, Ladprao Road,
 Phiatphla, Wang Thonglang, Bangkok 10310
 Rev 09
 TEL 02-516-2422
 FAX 02-515-5919
 CONTACT@AMARC.CO.TH
 WWW.AMARC.CO.TH
 Effective Date 15/07/21
 FM CL 018

2025



REPORT OF CALIBRATION


Certificate No. : 23-148804

Sample Code : 23 56200-006

Results of Calibration

Notes

1. Sensor installation locations
 - 1.1 All sensors at any corners or walls should be positioned 5 cm (a x b x c) from the wall.
 - 1.2 The reference sensor is preferably located of the geometric center of the chamber.
2. Interior dimensions approx of chamber :
W = 56 cm ; D = 40 cm ; H = 48 cm
3. Air valve or fresh air level : Off
4. Fan level : Open
5. The quoted uncertainty includes "Stability of chamber and loading effect in chamber at 20% of uniformity".
6. Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
7. Stability - one-half of the greatest maximum difference of measured temperatures at any one sensor.
8. Overall variation - the difference of the maximum and the minimum measured temperatures throughout observation time.
9. UUC* reading - the average reading of indicating device that forms the integral part of the enclosure.
10. Calibration results without adjustment.

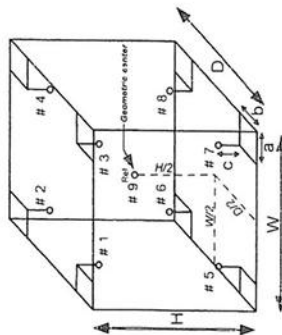Figure: Example of sensor
installation Positions

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M2003

- End of Report -

COPY

LIQUID IN GLASS THERMOMETER

Model : Total Immersion

Serial No. : 43560



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com



CERTIFICATE No : 23T10864
REFERENCE No : 71117-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : LIQUID IN GLASS THERMOMETER
MANUFACTURER : PRECISION
MODEL : 0 °C TO 100 °C

SERIAL No : 43560

ID No : LABE 16/1

RESOLUTION : 0.1 °C

TYPE : TOTAL IMMERSION

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : EASTERN THAI CONSULTING 1992 CO., LTD.
683 MOO 11, SUKHAPIBAN 8 ROAD, NONGKHAM,
SRIRACHA, CHONBURI 20230

CALIBRATED BY : CHARUKIT L.
CALIBRATION DATE : 09-Nov-23
APPROVED BY :
PONGSAK J.
ISSUED DATE : 09-Nov-23
RECEIVED DATE : 02-Nov-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

COPY

F-G010 REV 03



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com

CERTIFICATE No : 23T10864

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : LIQUID IN GLASS THERMOMETER
MANUFACTURER : PRECISION
MODEL : 0 °C TO 100 °C
ID No : LABE 16/1
RESOLUTION : 0.1 °C
RECEIVED DATE : 02-Nov-23
AMBIENT TEMPERATURE : 23 °C ± 3 °C
SERIAL NUMBER : 43560
TYPE : TOTAL IMMERSION
CALIBRATION DATE : 09-Nov-23
RELATIVE HUMIDITY : 50 %RH ± 20 %RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BASED ON ASTM E77:1992 BY COMPARISON WITH STANDARD PLATINUM RESISTANCE THERMOMETER (SPRT) INTO LIQUID BATH TEMPERATURE CONTROLLER. THE TEMPERATURE SCALE USED WAS BASED ON ITS-90.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD THERMOMETER	1502	77964	23T3927	08-Mar-24
2) SPRT PROBE	5614	636626	23T3927	08-Mar-24
3) PRECISION BATH	7320	A21105	22T13199	14-Dec-23
4) PRECISION BATH	CTR-40	A68155	22T13198	09-Dec-23
5) PRECISION BATH	6045	3C023	22T13200	19-Dec-23

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND).

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	EMERGENT STEM TEMPERATURE (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
0.009	0.0	60	0.0090	N/A	0.26
25.01	25.0	165	0.0050	N/A	0.26
50.00	50.0	275	0.0040	N/A	0.26
99.991	100.0	360	-0.009	29.3	0.26

UUC* : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

COPY

F-G010 REV 03

ORIFICE TRANSFER STANDARD CERTIFICATION

WORKSHEET TE-5025A

ROOTSMETER S/N 0438320

TISCH ENVIRONMENTAL, INC.
145 SOUTH MIAMI AVE
VILLAGE OF CLEVELAND, OH
45002
513.467.9000
877.283.7810 TOLL FREE
513.467.9009 FAX



ORIFICE TRANSFER STANDARD CERTIFICATION WORKSHEET TE-5025A

Date - Mar 24, 2016 Rootsmeter S/N 0438320 Ta (K) - 295
Operator Tisch Orifice I.D. - 0136 Pa (mm) - 742.95

PLATE OR Run #	VOLUME START (m3)	VOLUME STOP (m3)	DIFF VOLUME (m3)	DIFF TIME (min)	METER DIFF HG (mm)	ORIFICE DIFF H2O (in.)
1	NA	NA	1.00	1.3400	3.2	2.00
2	NA	NA	1.00	0.9510	6.3	4.00
3	NA	NA	1.00	0.8510	7.8	5.00
4	NA	NA	1.00	0.8130	8.6	5.50
5	NA	NA	1.00	0.6690	12.6	8.00

DATA TABULATION

Vstd	(x axis) Qstd	(y axis)	Va	(x axis) Qa	(y axis)
0.9832	0.7337	1.4054	0.9957	0.7430	0.8911
0.9791	1.0296	1.9875	0.9915	1.0426	1.2603
0.9770	1.1481	2.2221	0.9894	1.1626	1.4090
0.9760	1.2006	2.3305	0.9884	1.2157	1.4778
0.9707	1.4510	2.8107	0.9830	1.4694	1.7823
Qstd slope (m)	= 1.96262		Qa slope (m)	= 1.22896	
intercept (b)	= -0.03249		intercept (b)	= -0.02060	
coefficient (r)	= 0.99993		coefficient (r)	= 0.99993	
y axis = SQRT [H2O (Pa/760) (298/Ta)]			y axis = SQRT [H2O (Ta/Pa)]		

CALCULATIONS

$$Vstd = \text{Diff. Vol} [(Pa - \text{Diff. Hg}) / 760] (298 / Ta)$$

$$Qstd = Vstd / \text{Time}$$

$$Va = \text{Diff Vol} [(Pa - \text{Diff Hg}) / Pa]$$

$$Qa = Va / \text{Time}$$

For subsequent flow rate calculations:

$$Qstd = 1/m \{ [\text{SQRT} (H2O (Pa/760) (298/Ta))] - b \}$$

$$Qa = 1/m \{ [\text{SQRT} H2O (Ta/Pa)] - b \}$$

COPY

pH Meter

Model : SevenCompact S220

Serial No. : B448305208



CERTIFICATE OF CALIBRATION

Supersede to Calibration Certificate No. 24-001949

Page 1 of 3

Certificate No. : 24-001949/1
Sample Code : 24-00963-006Customer : EASTERN THAI CONSULTING 1992 CO., LTD.,
663 Moo 11, Sukhapibarn 8 Rd., Nongkham,
Siracha, Chonburi 20230
Location of Calibration : EASTERN THAI CONSULTING 1992 CO., LTD.,
(Laboratory)Equipment : pH Meter
Manufacturer : METTLER TOLEDO
Serial No. : B448305208
Date of Receipt : 09 January 2024
Condition of Calibration : SevenCompact S220
Model : LABE 11/4
ID No. :
Date of Calibration : 09 January 2024

1. Environment
1.1 Ambient temperature : 22.4 ± 0.2 °C 1.2 Relative humidity : 56.4 % ± 2.1 %
2. Calibration method
In house method W1-CL-019; based on direct measurement by using standard voltage calibrator and using certified reference material (CRM).

3. Reference standard / Certified reference material

Instrument	ID No.	Certificate No.	Due Date
3.1 Voltage Calibrator	LB-AMC-01	23E3244	03 October 2024
3.2 Digital Thermometer	LB-TH-33	23-096974	25 August 2024
Certified Reference Material			
3.3 Buffer Solution pH 4.008	919273	PH216.L5	24 September 2025
3.4 Buffer Solution pH 6.886	941727	PH107.L5	06 November 2024
3.5 Buffer Solution pH 9.597	919278	PH220.L5	24 September 2024

4. This certificate is traceable to the international system of unit (SI Unit).
- 4.1 Instrument No. 3.1 through Technology Promotion Association (Thailand-Japan).
- 4.2 Instrument No. 3.2 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.
- 4.3 Buffer Solution No. 3.3 and No. 3.5 traceable to CPA chem (through primary measurement method-Harned cell using calibrated thermometer, barometer, and nanovoltmeter Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).
- 4.4 Buffer Solution No. 3.4 traceable to CPA chem (CPA RefN HARNED CELL LotN 61275737; CPA RefN HARNED CELL LotN 61273966 Accredited laboratory ISO/IEC 17025 and ISO/IEC 17034).

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by Mr. Nuttaput Timula
Scientist
Approved by (Mr. Somchai Neamput)
Signed for Director

Issue date 31 January 2024

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

COPY



REPORT OF CALIBRATION

Supersede to Calibration Certificate No. 24-001949

Page 2 of 3

Certificate No. : 24-001949/1
Sample Code : 24-00963-006Equipment : pH Meter
Manufacturer : METTLER TOLEDO
Serial No. : B448305208
Range : -2,000 pH to 20,000 pH ; ± 2000.0 mV ; -5.0°C to 130.0°C
Resolution : 0.01 pH ; 0.1 mV ; 0.1 °C
Model : SevenCompact S220
ID No. : LABE 11/4

Results of Calibration

Part 1. DC Voltage measurement
pH Meter Serial No. : B448305208

Nominal Value	Applied DC Voltage mV	Average indicator reading		Uncertainty mV	Coverage factor k
		mV	pH		
0	414.113	413.9	0.00	± 0.083	2.00
4	177.477	177.4	4.00	± 0.083	2.00
7	0.000	0.1	7.00	± 0.083	2.00
10	-177.477	-177.3	10.00	± 0.083	2.00
14	-414.113	-413.8	14.00	± 0.083	2.00

Part 2. Performance of Electrode system

Electrode Manufacturer : METTLER TOLEDO
Electrode Serial No. : 2453982
Model : InLab Expert Pro-ISM
Three-Point Calibration at pH4, pH7 and pH10
Percent Slope : 98.3

Standard Buffer Solution pH (@ 25 °C)	Average indicator reading		Error Value	Uncertainty	Coverage factor k
	pH	mV			
4.008	4.01	182.1	0.002	± 0.010	2.00
6.986	7.00	7.8	0.014	± 0.011	2.00
9.997	10.01	-167.2	0.013	± 0.011	2.00

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

fmm.

COPY



REPORT OF CALIBRATION

Supersedes to Calibration Certificate No. 24-001949

Certificate No. : 24-001949/1

Sample Code : 24-00963-006

Equipment : pH Meter (Digital Thermometer with sensor)

Thermometer readout

Manufacturer : METTLER TOLEDO Model : SevenCompact S220

Serial No. : B448305208 ID No. : LABE 11/4

Resolution : 0.1 °C Range : -5.0 °C to 130.0 °C

Thermometer sensor

Manufacturer : METTLER TOLEDO Model : InLab Expert Pro-ISM

Serial No. : 2453982 ID No. : N/A

Condition of Calibration

1. Environment
 - 1.1 Ambient temperature : 22.6 °C ± 0.1 °C
 - 1.2 Relative humidity : 55.1 % ± 3.3 %

2. Calibration method

- 2.1 The calibration use in house method WI-CL-Q021 : by comparison with standard thermometer
- 2.2 The calibration by comparison unit under calibration (UUC) to the standard thermometer in a calibration bath at the controlled temperature.
- 2.3 The temperature scale in use of this laboratory is the international temperature scale of 1990 (ITS-90).

3. Reference standard instrument

Instrument	Model	ID. No.	Certificate No.	Due date
3.1 Resistance Thermometer	PT-100	RTD-90	23-098974	25 August 2024
3.2 Thermometer Readout	GT-11	LB-TH-33	23-098974	25 August 2024

4. This certificate is traceable to the international system of unit (SI Unit).

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (Accreditation Under TLAS Laboratory Calibration No.0152)

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibration item : Normal

Results of Calibration

Calibration point °C	Average of standard reading °C	Unit under calibration		Expanded uncertainty °C	Coverage factor k
		Immersion depth mm	Average reading °C		
25	25.000	120	25.0	± 0.14	2.00

Notes

- Calibration results without adjustment

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M0003

- End of report -

COPY

SPECTROPHOTOMETER

Model : PROVE 100

Serial No. : 1613110857

CERTIFICATE OF CALIBRATION

Function : Absorbance measurement.
All data shown below were final value of standard solution after adjustment.

Check Solution* (Abs.)	Desired Absorbance (Abs.)	Allowed tolerance (Abs.)	Actual Absorbance (Abs.)	Assessment Yes/No
445-1	0.198	± 0.020	0.196	Yes
445-2	0.496	± 0.030	0.493	Yes
445-3	0.994	± 0.040	0.985	Yes
445-4	1.492	± 0.050	1.475	Yes
525-1	0.197	± 0.020	0.195	Yes
525-2	0.494	± 0.030	0.491	Yes
525-3	0.986	± 0.040	0.984	Yes
525-4	1.482	± 0.050	1.480	Yes
690-1	0.197	± 0.020	0.197	Yes
690-2	0.498	± 0.030	0.497	Yes
690-3	0.985	± 0.040	0.978	Yes
690-4	1.485	± 0.050	1.482	Yes

* Spectroquant Photocheck (Check Solution) Lot : HC35941

- Check solution for this certification is traceable to : Reference Photometer Agilent Cary 4000 checked and calibrated using NIST-grey glass filter SRM 1930 and Holmiumoxide Solution NIST SRM 2034
- Desired absorbance round cell has been calculated from the absorbance of the 1 cm cell using the path length of the round cell and is entered as the desired



Merck Ltd. Thailand
19th Floor, Emporium Tower, 622 Sukhumvit Road
Klongtoey, Bangkok 10110
Tel : +66 (0) 2667 8000
Fax : +66 (0) 2667 8399
Customer Care Center : +66 (0) 2667 8333
www.merck.co.th



CERTIFICATE OF CALIBRATION

Instrument : SPECTROPHOTOMETER
Model : PROVE 100
Date of Calibration : February 13, 2023
Customer Name : Eastern Thai Consulting 1992 Co., Ltd.

Procedure used

The wavelength accuracy and the linearity of the absorbance measurement of photometers are checked using Check solutions according to Merck calibration laboratory work instruction.

Measurements results

Function : Absorbance measurement.
All data shown below as received values of blank solution before adjustment.

Check Solution (Abs.)	Wavelength (nm)	Desired Absorbance (Abs.)	Measured Absorbance (Abs.)	Error (Abs)
0.000	445	0.000 ± 0.005	0.000	0.000
0.000	525	0.000 ± 0.005	0.000	0.000
0.000	690	0.000 ± 0.005	0.000	0.000

CERTIFICATE No. **WO-02514383**



Merck Ltd. Thailand
19th Floor, Emporium Tower, 622 Sukhumvit Road
Klongtoey, Bangkok 10110
Tel : +66 (0) 2667 8000
Fax : +66 (0) 2667 8399
Customer Care Center : +66 (0) 2667 8333
www.merck.co.th



CERTIFICATE OF CALIBRATION

Software version: 1.5.1

Wavelength Accuracy*					
Equipment	Nominal value	Tolerance limit*	Actual value	Result	
Holmium Oxide Liquid Filter Hellma 667-UV5	361.25 nm	360.1 - 362.5 nm	360.8 nm	P	
	536.55 nm	535.4 - 539.3 nm	536.9 nm	P	
	640.55 nm	639.4 - 642.8 nm	640.9 nm	P	
Photometric Accuracy*					
Equipment	Wavelength	Nominal value	Tolerance limit*	Actual value	Result
Neutral Density 1.00 Abs. Hellma 666-F4	440 nm	1.079 A	1.067 - 1.091 A	1.083 A	P
	546 nm	1.012 A	1.004 - 1.020 A	1.015 A	P
	635 nm	1.050 A	1.042 - 1.058 A	1.051 A	P
Stray Light*					
Equipment	Wavelength	Nominal value	Actual value	Result	
UV-VIS Standard 2 Sodium Nitrite Solution	340 nm	≤0.10 %T	0.05 %T	P	
Self-test Hardware					
No visual flaws, no burrs, no loose parts and fastenings				P	

CERTIFICATE OF CALIBRATION

INSTRUMENT : SPECTROPHOTOMETER

MANUFACTURER : Merck KGaA, Darmstadt, Germany

MODEL : PROVE 100

SERIAL No. : 1613110857

CLIENT : Eastern Thai Consulting 1992 Co., Ltd.

DATE OF ISSUE : February 13, 2023

APPROVED SIGNATORY

NAME : Mr. Rawat Rattanachetthakul
(SERVICE ENGINEER)

SIGNATURE :

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

CERTIFICATE No. WO-02514383



Merck Ltd. Thailand
19th Floor, Emporium Tower, 622 Sukhumvit Road
Klongton, Klongtoey, Bangkok 10110
Tel. : +66 (0) 2667 8000
Fax : +66 (0) 2667 8399
Customer Care Center : +66 (0) 2667 8333

www.merck.co.th



Merck Ltd. Thailand
19th Floor, Emporium Tower, 622 Sukhumvit Road
Klongton, Klongtoey, Bangkok 10110
Tel. : +66 (0) 2667 8000
Fax : +66 (0) 2667 8399
Customer Care Center : +66 (0) 2667 8333

www.merck.co.th

COPY

SPECTROPHOTOMETER

Model : PROVE 100

Serial No. : 1613110857



CERTIFICATE OF CALIBRATION

Instrument : SPECTROPHOTOMETER
Model : PROVE 100
Date of Calibration : Feb 9, 2024
Customer Name : Eastern Thai Consulting 1992 Co., Ltd.
Procedure used

The wavelength accuracy and the linearity of the absorbance measurement of photometers are checked using Check solutions according to Merck calibration laboratory work instruction.

Measurements results

Function : Absorbance measurement.
All data shown below as received values of blank solution before adjustment.

Check Solution (Abs.)	Wavelength (nm)	Desired Absorbance (Abs.)	Measured Absorbance (Abs.)	Error (Abs)
0.000	445	0.000 ± 0.005	0.000	0.000
0.000	525	0.000 ± 0.005	0.000	0.000
0.000	690	0.000 ± 0.005	0.000	0.000

CERTIFICATE No. WO-02723295



Merck Ltd. Thailand
19th Floor, Emporium Tower, 622 Sukhumvit Road
Klongton, Klongtoey, Bangkok 10110
Tel. : +66 (0) 2667 8000
Fax : +66 (0) 2667 8399
Customer Care Center : +66 (0) 2667 8333

www.merck.co.th



Merck Ltd. Thailand
19th Floor, Emporium Tower, 622 Sukhumvit Road
Klongton, Klongtoey, Bangkok 10110
Tel. : +66 (0) 2667 8000
Fax : +66 (0) 2667 8399
Customer Care Center : +66 (0) 2667 8333

www.merck.co.th



CERTIFICATE OF CALIBRATION

Function : Absorbance measurement.
All data shown below were final value of standard solution after adjustment.

Check Solution* (Abs.)	Desired Absorbance (Abs.)	Allowed tolerance (Abs.)	Actual Absorbce (Abs.)	Assessment Yes/No
445-1	0.197	± 0.020	0.189	Yes
445-2	0.497	± 0.030	0.481	Yes
445-3	0.990	± 0.040	0.970	Yes
445-4	1.494	± 0.050	1.474	Yes
525-1	0.198	± 0.020	0.191	Yes
525-2	0.493	± 0.030	0.485	Yes
525-3	0.988	± 0.040	0.966	Yes
525-4	1.485	± 0.050	1.471	Yes
690-1	0.204	± 0.020	0.197	Yes
690-2	0.504	± 0.030	0.494	Yes
690-3	0.987	± 0.040	0.989	Yes
690-4	1.498	± 0.050	1.493	Yes

* Spectroquant Photocheck (Check Solution) Lot : HC299606

- Check solution for this certification is traceable to : Reference Photometer Agilent Cary 4000 checked and calibrated using NIST-grey glass filter SRM 1930 and Holmiumoxide Solution NIST SRM 2034
- Desired absorbance round cell has been calculated from the absorbance of the 1 cm cell using the path length of the round cell and is entered as the desired



CERTIFICATE OF CALIBRATION

Software version: 1.5.1

Wavelength Accuracy				
Equipment	Nominal value	Tolerance limit	Actual value	Result
Holmium Oxide Solution Standard 6	361.1 nm	359.1 – 363.1 nm	361.0 nm	P
	386.3 nm	382.3 – 390.3 nm	385.5 nm	P
	417.1 nm	413.1 – 421.1 nm	416.4 nm	P
	451.4 nm	447.4 – 455.4 nm	450.0 nm	P
	485.3 nm	481.3 – 489.3 nm	485.2 nm	P
	537.6 nm	533.6 – 541.6 nm	537.3 nm	P
Photometric Accuracy				
Equipment	Wavelength	Nominal value	Tolerance limit	Actual value
Neutral Density 1.00 Abs. Hellma 666-F4	440 nm	1.079 A	1.067 - 1.091 A	1.074 A
	546 nm	1.012 A	1.004 - 1.020 A	1.010 A
	635 nm	1.050 A	1.042 - 1.058 A	1.048 A
Stray Light				
Equipment	Wavelength	Nominal value	Actual value	Result
UV-VIS Standard 2 Sodium Nitrite Solution	340 nm	≤0.10 %T	0.05 %T	P
Self-test Hardware				
No visual flaws, no burrs, no loose parts and fastenings				P



Merck Ltd. Thailand
19th Floor, Emporium Tower, 622 Sukhumvit Road
Klongton, Klongtoey, Bangkok 10110
Tel. : +66 (0) 2667 8000
Fax : +66 (0) 2667 8399
Customer Care Center : +66 (0) 2667 8333

www.merck.co.th



Merck Ltd. Thailand
19th Floor, Emporium Tower, 622 Sukhumvit Road
Klongton, Klongtoey, Bangkok 10110
Tel. : +66 (0) 2667 8000
Fax : +66 (0) 2667 8399
Customer Care Center : +66 (0) 2667 8333

www.merck.co.th



CERTIFICATE OF CALIBRATION

INSTRUMENT : SPECTROPHOTOMETER

MANUFACTURER : Merck KGaA, Darmstadt, Germany

MODEL : PROVE 100

SERIAL No. : 1613110857

CLIENT : Eastern Thai Consulting 1992 Co., Ltd.

DATE OF ISSUE : Feb 9, 2024

APPROVED SIGNATORY

NAME : Mr.Rawat Rattanachethakul
(SERVICE ENGINEER)

SIGNATURE : _____

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

CERTIFICATE No. WO-02723295

STANDARD WEIGHT 50 g

Certificate No. : 22-052238

Sample Code : 22-19150-003

Page 1 of 3

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapiban 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

Certificate No. : 22-052238

Sample Code : 22-19150-003

Page 2 of 3

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : METTLER TOLEDO

Class : F1

Serial No. : N/A

ID No. : LABE 10/1

Result of Calibration :

☒ Without adjustment☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional Mass	Expanded Uncertainty	Maximum Permissible Error	ID No.
50 g	(mg) -0.324	49.999676 g	(mg) 0.10	\pm (mg) 0.30	LABE 10/1

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003



Certificate No. : 22-052238
Sample Code : 22-19150-003

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.20 kg/m³

2. Calibration Method : Direct comparison weighing according to OIML R111-1 : 2004(E)

3. Reference standard Instrument

Instrument	Class	ID No.	Certificate No.	Due Date
1) Standard Weight 1 mg to 1 kg	E2	LB-WE-79	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item : 50 g

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

Copy

STANDARD WEIGHT 100 g



Certificate No. : 22-052239

Sample Code : 22-19150-004

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapiban 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052239

Sample Code : 22-19150-004

REPORT OF CALIBRATION

Equipment : Standard Weight 100 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/2

Result of Calibration :

☒ Without adjustment☐ AdjustmentConventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_0) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
100 g	-0.171	99.999829 g	0.16	0.50	LABE 10/2

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k = 2.0, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003



Certificate No. : 22-052239

Sample Code : 22-19150-004

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature $20^{\circ}\text{C} \pm 1.5^{\circ}\text{C}$, Relative humidity $50\% \pm 10\%$ and air density 1.18 kg/m^3
 2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)
 3. Reference standard instrument
- | Instrument | Class | ID No. | Certificate No. | Due Date |
|---------------------------------|-------|----------|-----------------|-------------------|
| 1) Standard Weight 1 mg to 1 kg | E2 | LB-WE-79 | 21-079366 | 22 September 2022 |
4. This certification is traceable to the International System of Unit maintained at :-

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Instrument number 1).

5. Condition of Calibration item: Normal

6. Description of Calibrated Item	
Type and Nominal Value :	Standard Weight 100 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

- End of Report -

Handwritten signature

COPY

STANDARD WEIGHT 50 g



Certificate No. : 22-052237

Sample Code : 22-19150-002

Page 1 of 3

CERTIFICATE OF CALIBRATION

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapiban 8 Rd., Nongkham,

Siracha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration Laboratory)

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Date of Receipt : 18 May 2022

Date of Calibration : 30 May 2022

Calibrated by : Mr. Somwang Sangdee
Scientist

Issue date : 31 May 2022

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).



Certificate No. : 22-052237

Sample Code : 22-19150-002

Page 2 of 3

REPORT OF CALIBRATION

Equipment : Standard Weight 50 g

Manufacturer : N/A

Class : N/A

Serial No. : N/A

ID No. : LABE 10/4

Result of Calibration :

☒ Without adjustment

☐ Adjustment

Conventional value of the result of weighing in air. For a weight taken at a reference temperature (t_{ref}) of 20°C, the conventional mass is the mass of a reference weight of a density (ρ_{ref}) of 8000 kg.m⁻³ which it balances in air of a reference density (ρ_a) of 1.2 kg.m⁻³

Description	Deviation	Conventional	Expanded	Maximum	ID No.
		Mass	Uncertainty	Permissible Error	
	(mg)		(mg)	± (mg)	
50 g	-0.111	49.999889 g	0.10	0.30	LABE 10/4

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.0$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003



Certificate No. : 22-052237

Sample Code : 22-19150-002

REPORT OF CALIBRATION

Condition of Calibration

1. Ambient Conditions : Temperature 20 °C ± 1.5°C, Relative humidity 50% ± 10% and air density 1.19 kg/m³
2. Calibration Method : WI-CL-007 base on OIML R 111-1 : 2004(E)
3. Reference standard instrument

Instrument	ID.No.	Class	Certificate No.	Dua Date
1) Standard Weight 1 mg to 1 kg	LB-WE-79	E2	21-079366	22 September 2022

4. This certification is traceable to the International System of Unit maintained at : -

Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Instrument number 1).

5. Condition of Calibration Item: Normal

6. Description of Calibrated Item :

Type and Nominal Value :	Standard Weight 50 g
Shape :	Cylindrical weight with knob
Material :	Stainless steel
Case :	Wooden Box
Comments :	Recalibration

Handwritten signature

- End of Report -

COPY

THERMO-HYGROMETER

Model : 608-H1

Serial No. : 45106737



CERTIFICATE OF CALIBRATION

Page 1 of 2

Certificate No. : 23-055203
Sample Code : 23-21440-001

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.

683 Moo 11, Sukhapiarn 8 Rd., Nongkham,

Si-racha, Chonburi 20230

Location of Calibration : Asia Medical and Agricultural Laboratory and Research Center Public Company Limited
(Calibration laboratory)

Equipment : Digital thermo-hygrometer

Manufacturer : testo Model : 608-H1

Serial No. : 45106737 ID No. : LABE 09/7

Date of Receipt : 25 May 2023 Date of Calibration : 29 May 2023

Condition of Calibration

1. Environment 1.1 Ambient temperature : 23.0 °C ± 3.0 °C

1.2 Relative humidity : 55.0 % ± 15.0 %

2. Calibration method

2.1 In-house method: WI-CL-045 By comparison with thermometer standard / chilled mirror hygrometer in controlled chamber.

2.2 The calibration by comparison unit under calibration (UUC) to the thermometer standard / chilled mirror hygrometer in a chamber at the controlled temperature / relative humidity.

3. Reference standard instrument

Instrument	Model	ID No.	Certificate No.	Due Date
3.1 Chilled Mirror	Optidew Vision	LB-DP-02 & LB-DP-02 (DP)	TH-0157-22	05 December 2023
3.2 Digital Thermometer	Optidew Vision	LB-DP-02 & LB-DP-02 (Temp.)	23-014916	12 February 2024
3.3 Digital Thermometer	34972A	LB-DA-07 with RTD-89	22-095535	06 September 2023

4. This certificate is traceable to the international system of unit (SI Unit).

4.1 Instrument No. 3.1 through National Institute of Metrology (Thailand).

4.2 Instrument No. 3.2 and 3.3 through Asia Medical and Agricultural Laboratory and Research Center Public Company Limited.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of calibration item : Normal

Calibrated by

Miss Pornsuda Lohabal

Approved by

(Mr. Somchai Neampunt)

Scientist

Signed for Director

Issue date

31 May 2023

The uncertainties are for a confidence probability of approximately 95%.

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Asia Medical and Agricultural Laboratory and Research Center Public Company Limited (AMARC).

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

TEL 02-516-2422

FAX 02-516-6949

Rev. 01

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

File Issue Date: 15/07/21



REPORT OF CALIBRATION

Page 2 of 2
Certificate No. : 23-055203
Sample Code : 23-21440-001

Results of Calibration

Temperature measurement

Resolution : 0.1 °C
Range : 0 °C to 50 °C

Calibration point °C	Average of standard reading		Unit under calibration		Expanded uncertainty °C
	Controlled humidity %RH	Temperature °C	Average reading °C	Correction value °C	
20	50	20.00	20.0	0.00	± 0.39
25	50	25.02	25.1	- 0.08	± 0.39
30	50	30.00	30.0	0.00	± 0.39

Humidity measurement

Resolution : 0.1 %RH
Range : 10 %RH to 95 %RH

Calibration point %RH	Average of standard reading		Unit under calibration		Expanded uncertainty %RH
	Air temperature °C	Calculated humidity %RH	Average reading %RH	Correction value %RH	
45	25.00	45.18	53.5	- 8.32	± 1.3
60	25.00	60.03	68.3	- 8.27	± 1.5
75	25.00	75.20	83.2	- 8.00	± 1.7

Notes

Calibration results without adjustment.

The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k , which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty of measurement has been determined in accordance with UKAS M3003

- End of Report -



361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

TEL 02-516-2422

FAX 02-516-6949

Rev. 01

CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

File Issue Date: 15/07/21

361 Soi Ladprao 122, Ladprao Road,

Phlabphla, Wang Thonglang, Bangkok 10310

TEL 02 516-2422

FAX 02-516 6949

Rev. 01
















CONTACT@AMARC.CO.TH

WWW.AMARC.CO.TH

UV/VIS SPECTROPHOTOMETER

Model : UV - 1800

Serial No. : A11635101643 CD



2 of 3

Number of Page(s)

Certificate No.

BSCC-UV-152/23

Calibration Results:

1. Wavelength Accuracy

Calibration Results:

1. Wavelength Accuracy

Calibration Results:

1. Wavelength Accuracy

Calibration Results:

1. Wavelength Accuracy

Calibration Results:

1. Wavelength Accuracy

Calibration Results:

1. Wavelength Accuracy

Calibration Results:

Certified Wavelength (nm)	UUC (nm)	Error (nm)	Uncertainty (±nm)
287.71	287.65	-0.06	0.18
445.82	445.80	-0.02	0.18
536.52	536.35	-0.17	0.18
741.02	740.99	-0.03	0.18
879.41	879.27	-0.14	0.18







2. Photometric Accuracy (UV)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
235	0.0000	0.0000	0.0000	0.0075
	0.7311	0.7313	0.0002	0.0075
257	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
313	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
350	0.0000	0.0000	0.0000	0.0075
	0.6306	0.6314	0.0008	0.0075

*CNR = Customer not request



The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising this report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.



1 of 3

Number of Page(s)

Certificate No.

BSCC-UV-152/23

UV/Vis Spectrophotometer

Model

UVA-1800

Manufacturer

Shimadzu
A11635101643 CD
N/A
25 April 2023
25 April 2023
27 April 2023
Eastern Thai Consulting 1992 Co., Ltd
683 Moo 11, Sukkaphibam 8 Rd., Nongkham, Sriracha, Chonburi 20230

Temperature
(22.4-23.1) °C (On site)
Humidity
(44.5-45.2) %RH (On site)

Equipment condition
Good Operation

Calibration Location
Analysis Department

Calibration Procedure
In-house method WI-UV-702-01 based on ASTM E275-01

Traceability
Wavelength Accuracy is traceable to certificate No. 94780 and 94775
Photometric Accuracy is traceable to certificate No. 94808 and 100147
Stray Light is traceable to certificate No. 94791
The above certificate are traceable to SI unit through Starna Scientific Ltd.
(UKAS accredited calibration laboratory NO. 0659)

Calibrated by
Mr. Pannaphong Phannmekakul

Approved by

Mr. Kanchit Choothep
Technical Manager

The above results are valid exclusively for the calibrated item(s) as mention in this report / certificate. Advertising this report / Certificate and publicity of the results are prohibited and also shall not be reproduced except in full, without written approval of the Bara Scientific Co., Ltd.





Bara Scientific Co., Ltd.
988 U Chu Liang Building Floor 7 Rama 4 Road
Siam Bangkok Bangkok Thailand 10500
Tel : 02-6324300 Fax : 02-6375496-7
www.barascientific.com

Bara Scientific
Division of Success



Certificate of Calibration

Certificate No.

BSCC-UV-152/23

Calibration Results:

Number of Page(s)

3 of 3

3. Photometric Accuracy (Visible)

Wavelength (nm)	Certified Absorbance (A)	UUC (A)	Error (A)	Uncertainty (±A)
420.0	0.0000	0.0000	0.0000	0.0042
	0.5488	0.5508	0.0020	0.0042
	0.7527	0.7535	0.0008	0.0042
440.0	1.0756	1.0758	0.0002	0.0042
	0.0000	0.0000	0.0000	0.0042
	0.5391	0.5406	0.0015	0.0042
465.0	0.7355	0.7360	0.0005	0.0042
	1.0509	1.0501	-0.0008	0.0042
	CNR	CNR	CNR	CNR
546.1	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
590.0	0.0000	0.0000	0.0000	0.0042
	0.5045	0.5044	-0.0001	0.0042
	0.6884	0.6885	0.0001	0.0042
635.0	0.9816	0.9808	-0.0008	0.0042
	CNR	CNR	CNR	CNR
	CNR	CNR	CNR	CNR
635.0	CNR	CNR	CNR	CNR
	0.0000	0.0000	0.0000	0.0042
	0.5183	0.5178	-0.0005	0.0042
635.0	0.6864	0.6868	0.0004	0.0042
	0.9747	0.9739	-0.0008	0.0042

*CNR = Customer not request

4. Stray Light*

Standard cut-off wavelength (nm)	Unit Under Calibration(UUC)	
	Wavelength (nm)	Absorbance (A)
200.75±0.1nm	200.72	2.0164

The Stray light transmission reference is less than 1.0%T and Stray light absorbance reference is greater than 2.00A

*Stray Light not NSC-ONSC Accredited.

The measurement uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%
End of Certificate

The above results are valid exclusively for the calibrated item(s) as mentioned in this report / Certificate and shall not be reproduced or used for any other purpose without written approval of Bara Scientific Co., Ltd.
AC-Stray Light not NSC-ONSC Accredited.

COPY

SOUND LEVEL CALIBRATOR

MODEL : NC-75

SERIAL No. : 34802645



Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-75
Serial No.: 34802645
ID No.:

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 06 SEPTEMBER 2023
Calibration Date : 12 OCTOBER 2023
Date of Issue : 16 OCTOBER 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : T. Petchurai
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

Continuation of Calibration Certificate

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

T. Petchurai

Continuation of Calibration Certificate

Cert. No. : ACC23037
Job No. : VC66AC0097
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	93.94	-0.06	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1000.0	0.0	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
0.24	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

_____ End of Calibration Certificate _____

COPY

T. Retan

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 01120945

Cert. No. : ACL24040
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 01120945 / 22210 / 22422
ID No.: -

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : -
Ambient Temperature : (23.0 \pm 3) °C
Pressure : (101.3 \pm 3) kPa
Relative Humidity : (50.0 \pm 20) %

Received Date : 11 JANUARY 2024
Calibration Date : 16 - 17 JANUARY 2024
Date of Issue : 18 JANUARY 2024

Calibrated by : Nathakorn Pisumpaisan

Approved by : *T. Petchurai*
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

T. Petchurai
COPY

Cert. No. : ACL24040
Job No. : VC67AC0042
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For test results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EFL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

T. Petchurai
COPY

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

COPY
T. Petch...

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	8.7
C - weight	14.3
Flat	20.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.2	0.2	0.2	± 1.0
1000	0.2	0.2	0.2	± 0.7
8000	0.3	0.4	0.4	+ 1.5, - 2.5

COPY
T. Petch...

Cert. No. : ACL24040

Job No. : VC67AC0042

Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	-0.1	0.0	0.0
125	0.0	0.0	0.0
250	0.0	0.0	0.0
500	0.0	0.0	-0.1
1000	0.0	0.0	0.0
2000	0.0	0.0	0.0
4000	0.0	0.0	0.0
8000	0.0	0.0	0.0
16000	0.0	-1.3	-1.2

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.1	0.1	± 0.8
136.0	136.1	0.1	± 0.8
135.0	135.1	0.1	± 0.8
134.0	134.1	0.1	± 0.8
133.0	133.0	0.0	± 0.8
132.0	132.0	0.0	± 0.8
131.0	131.0	0.0	± 0.8
129.0	129.0	0.0	± 0.8
124.0	124.0	0.0	± 0.8
119.0	119.1	0.1	± 0.8
114.0	114.0	0.0	± 0.8
109.0	109.0	0.0	± 0.8
104.0	104.1	0.1	± 0.8
99.0	99.0	0.0	± 0.8
94.0	94.0	0.0	± 0.8
89.0	89.0	0.0	± 0.8
84.0	84.0	0.0	± 0.8
79.0	79.0	0.0	± 0.8
74.0	74.0	0.0	± 0.8
69.0	69.0	0.0	± 0.8
64.0	64.0	0.0	± 0.8
59.0	59.0	0.0	± 0.8
54.0	54.0	0.0	± 0.8
49.0	49.0	0.0	± 0.8
44.0	44.0	0.0	± 0.8
39.0	39.0	0.0	± 0.8
34.0	34.0	0.0	± 0.8
30.0	30.0	0.0	± 0.8
29.0	29.0	0.0	± 0.8
28.0	28.0	0.0	± 0.8
27.0	27.0	0.0	± 0.8
26.0	25.9	-0.1	± 0.8
25.0	24.9	-0.1	± 0.8

COPY

T. Petch.

COPY

T. Petch.

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
One	136.4	135.8	-0.6	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	89.5	-0.1	±1.5
Negative one-half cycle	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

T. Petch

COPY

T. Petch

SOUND LEVEL METER

MODEL : NL-52A

SERIAL No. : 00230994



Acoustic Laboratory (Thailand) Co., Ltd.
6/57 Soi Phoen Sin 42, Sai Mai, Sai Mai, Bangkok 10220
Tel: (+66) 02-1296780 Email: info@altbkk.com



Certificate of Calibration

Certificate No.: S2403-0659

Customer:

Eastern Thai Consulting 1992 Co., Ltd.
683 Moo 11, Sukhapibarn 8 Rd,
Nongkham, Sriacha, Chonburi 20230

Date of calibration:

2024-03-13

Date of issue:

2024-03-15

Instrument Calibrated:

Sound Level Meter

Manufacturer:

Rion

Model:

NL-52A (Meter), UC-59 (Microphone), NH-25 (Preamplifier)

Serial no:

00230994 (Meter), 22777 (Microphone), 22430 (Preamplifier)

Calibration and verification performed:

A coustical levels are stated relative to 20µPa. Other dB levels are relative values.
The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which with the reported effective degree of freedom corresponds to coverage probability of approximately 95%.

The sound level meter instrument submitted for periodic testing following the periodic tests of

IEC 61672-3 : 2013.

Preconditioning:

The equipment was preconditioned for more than 16 hours at the specified calibration temperature and humidity

Instruments and Program:

A complete list of instruments, hardware, and software, that has been used for this calibration is separately available from the calibration laboratory.

Equipment standards used:

- Sound measuring equipment calibration unit 483B S/N31083
- Digital multimeter Keysight S/N HP34401A
- Ultra-low distortion function generator Stanford SRS DS360 S/N123625
- Acoustic sound calibrator class 1 Nor1256 S/N125626542
- Combined Pressure, Humidity and Temperature Transmitter PTU300 S/NM2520568

Traceability

The measured values are traceable to following the ISO/IEC 17025 laboratories:

Sound Pressure Level: EEL, Thailand

Reference Pressure, Humidity and Temperature: TPA, Thailand

Voltage: TPA, Thailand

Frequency: TPA, Thailand

This certificate of calibration is issued by Acoustic Laboratory, Thailand (ALT). It also states that the laboratory has a satisfactory quality assurance system and is not to be reproduced other than in full.

Page 1 of 8



Certificate No.: S2403-0659

Environmental conditions:

Pressure:

101.325 kPa

Temperature:

23.0 °C

Relative humidity:

50 %RH

Measurement conditions:

101.08 ± 0.10 kPa

23.1 ± 1.0 °C

52.4 ± 2.0 %RH

1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)		Deviated value (dB)	Acceptant limit (dB)
	Before adjust	After adjusted		
93.9	94.0	93.9	0.0	±0.7

Note: Indication at the checked calibration frequency was adjusted to 93.9 dB by the sound calibrator Type NC-75 S/N 34234715

2. Self-generated noise

Frequency Weighting	Measured value (dB)
A-Weighting	10.3
C-Weighting	16.4
Z-Weighting	20.0

3. Electrical signal test of frequency weighting at 93 dB

Frequency (Hz)	Deviation from various frequency weighting response curve		
	A-Weighting (dB)	C-Weighting (dB)	Z-Weighting (dB)
63.0	-0.1	-0.1	-0.1
125.0	0.0	0.0	0.0
250.0	0.0	0.0	0.0
500.0	0.0	0.0	0.0
1000.0	0.0	0.0	0.0
2000.0	0.0	0.0	0.0
4000.0	0.0	0.0	0.0
8000.0	0.1	0.1	0.1
16000.0	+1.2	-1.2	0.0

Date of calibration : 2024-03-13

Date of issue : 2024-03-15

Registration number 01055408235
6/57 Phoen Sin 42, Sai Mai, 10220 Bangkok, Thailand
Tel (+66) 02-1296780 Email: info@altbkk.com
www.altbkk.com

Page 1 of 8

Page 2 of 8

4. Frequency and time weighting at 1 kHz

4.1 Frequency weighting at 1 kHz

Frequency weightings	Measured value (dB)	Deviated value (dB)	Acceptant limit (dB)
A	94.0	0.0	±0.2
C	94.0	0.0	±0.2
Z	94.0	0.0	±0.2

4.2 Time weighting at 1 kHz

Time weightings	Measured value (dB)	Deviated value (dB)	Acceptant limit (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAcq	94.0	0.0	±0.1

5. Long term stability

Time interval (mm:ss)	Start level (dB)	Stop level (dB)	Deviated value (dB)	Acceptant limit (dB)
27:11	94.0	94.0	0.0	±0.1

Date of calibration : 2024-03-13
Date of issue : 2024-03-15

6. Level linearity on the reference level range

6.1 Measured at 31.5 Hz

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptant limit (dB)
84.0	84.0	0.0	±0.8
89.0	89.0	0.0	±0.8
94.6	94.6	0.0	±0.8
95.6	95.6	0.0	±0.8
96.6	96.6	0.0	±0.8
97.6	97.6	0.0	±0.8
98.6	98.6	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.1	0.1	±0.8
44.0	44.3	0.3	±0.8
42.0	42.0	0.0	±0.8
41.0	41.0	0.0	±0.8
40.0	39.9	-0.1	±0.8
39.0	38.9	-0.1	±0.8
38.0	38.0	0.0	±0.8

Date of calibration : 2024-03-13
Date of issue : 2024-03-15



Certificate No.: S2403-0659

6.2 Measured at 1 kHz

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptant limit (dB)
109.0	109.0	0.0	± 0.8
114.0	114.0	0.0	± 0.8
119.0	119.0	0.0	± 0.8
124.0	124.0	0.0	± 0.8
129.0	129.0	0.0	± 0.8
134.0	134.0	0.0	± 0.8
135.0	135.0	0.0	± 0.8
136.0	136.0	0.0	± 0.8
137.0	137.0	0.0	± 0.8
138.0	138.0	0.0	± 0.8
94.0	94.0	0.0	± 0.8
89.0	89.0	0.0	± 0.8
84.0	84.0	0.0	± 0.8
79.0	79.0	0.0	± 0.8
74.0	74.0	0.0	± 0.8
69.0	69.0	0.0	± 0.8
64.0	64.0	0.0	± 0.8
59.0	59.0	0.0	± 0.8
54.0	54.0	0.0	± 0.8
49.0	49.0	0.0	± 0.8
44.0	44.0	0.0	± 0.8
42.0	42.0	0.0	± 0.8
41.0	41.0	0.0	± 0.8
40.0	40.0	0.0	± 0.8
39.0	39.0	0.0	± 0.8
38.0	38.0	0.0	± 0.8

Date of calibration : 2024-03-13

Date of issue : 2024-03-15

COPY
Page 5 of 8



Certificate No.: S2403-0659

6.3 Measured at 8 kHz

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptant limit (dB)
94.0	94.0	0.0	± 0.8
99.0	99.1	0.1	± 0.8
104.0	104.1	0.1	± 0.8
109.0	109.0	0.0	± 0.8
114.0	114.0	0.0	± 0.8
119.0	119.0	0.0	± 0.8
124.0	124.0	0.0	± 0.8
129.0	129.0	0.0	± 0.8
132.9	132.9	0.0	± 0.8
133.9	133.9	0.0	± 0.8
134.9	134.9	0.0	± 0.8
135.9	135.9	0.0	± 0.8
136.9	136.9	0.0	± 0.8
94.0	94.0	0.0	± 0.8
89.0	89.0	0.0	± 0.8
84.0	84.0	0.0	± 0.8
79.0	79.0	0.0	± 0.8
74.0	74.0	0.0	± 0.8
69.0	69.0	0.0	± 0.8
64.0	64.0	0.0	± 0.8
59.0	59.0	0.0	± 0.8
54.0	54.0	0.0	± 0.8
49.0	49.0	0.0	± 0.8
44.0	44.0	0.0	± 0.8
42.0	42.0	0.0	± 0.8
41.0	41.0	0.0	± 0.8
40.0	40.0	0.0	± 0.8
39.0	39.0	0.0	± 0.8
38.0	38.0	0.0	± 0.8

Date of calibration : 2024-03-13

Date of issue : 2024-03-15

COPY
Page 6 of 8

7. Tone burst response

Time weightings	Tone burst duration, T _b (ms)	Measured value (dB)	Deviated value (dB)	Tolerance limit (dB)
Fast	200	135.0	0.0	±0.5
	2	118.0	0.0	+1.0, -1.5
	0.25	108.9	-0.1	+1.0, -3.0
SEL	200	129.0	0.0	±0.5
	2	109.0	0.0	+1.0, -1.5
	0.25	99.9	-0.1	+1.0, -3.0

8. Overload indication

Measured value (dB)		Deviated value (dB)	Tolerance limit (dB)
Positive one half cycle	Negative one half cycle	139.3	±1.5
139.3			

9. High level stability

Initial level (dB)	Final level (dB)	Deviated value (dB)	Acceptant limit (dB)
137.0	137.0	0.0	±0.1

Date of calibration : 2024-03-13
Date of issue : 2024-03-15

Uncertainty of measurement

Parameters	Uncertainty
1. Indication at the calibration check frequency	0.12 dB
2. Self-generated noise	
- Frequency Weighting A	0.090 dB
- Frequency Weighting C	0.090 dB
- Frequency Weighting Z	0.090 dB
3. Electrical signal test of frequency weighting	
4. Frequency and time weightings at 1 kHz	0.13 dB
5. Long term stability test	0.13 dB
6. Level linearity on the reference level range	0.10 dB
7. Tone burst response	0.14 dB
8. Overload indication	0.13 dB
9. High level stability test	0.10 dB

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Remark : The acoustical signal test of frequency weighting at 125Hz, 1kHz, and 8kHz is not included, along with correction values for environmental conditions in a free-field or diffuse field, and the effect of reflection and diffraction on the measurement microphone and the sound level meter.

Signature

Calibrated By: (Mr. Chaiyaporn Sompichai)

Approved By: (Mr. Pitupong Sarapho)

Date of calibration : 2024-03-13
Date of issue : 2024-03-15

----- End of Certificate of Calibration -----

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322745



Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322745 / 196468 / 15477
ID No.: -

Condition As Found : GOOD
Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 10 MAY 2023
Calibration Date : 17-18 MAY 2023
Date of Issue : 24 MAY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23166
Job No. : VC66AC0058
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23166
Job No. : VC66AC0058
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	10.8
C - weight	17.2
Flat	23.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.3	0.3
1000	0.0	0.0	0.0
8000	0.5	0.6	0.6
			Acceptance Limits
			± 1.5
			± 1.0
			± 5.0

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23166
Job No. : VC66AC0058
Pages : 5 of 8

Cert. No. : ACL23166
Job No. : VC66AC0058
Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	0.0	-0.1	0.0
125	0.0	0.0	0.0
250	0.0	0.0	0.0
500	0.0	0.0	0.0
1000	0.0	0.0	0.0
2000	0.0	0.0	0.0
4000	0.0	0.0	0.0
8000	0.0	0.1	0.1

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.0	0.0	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL23166
Job No. : VC66AC0058
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23166
Job No. : VC66AC0058
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	-0.2	±1.5
89.8	89.6		

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322750



Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322750 / 196473 / 15482
ID No.:

Condition As Found : GOOD
Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 10 MAY 2023
Calibration Date : 17 -18 MAY 2023
Date of Issue : 24 MAY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

COPY

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23168
Job No. : VC66AC0058
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23168
Job No. : VC66AC0058
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	10.8
C - weight	17.3
Flat	23.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.0	0.0	0.0
8000	0.3	0.4	0.4
Acceptance Limits			± 1.5
			± 1.0
			± 5.0

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23168
Job No. : VC66AC0058
Pages : 5 of 8Cert. No. : ACL23168
Job No. : VC66AC0058
Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	0.0	-0.1	0.0 ±2.0
125	0.0	0.0	0.0 ±1.5
250	0.0	0.0	0.0 ±1.5
500	0.0	0.0	0.0 ±1.5
1000	0.0	0.0	0.0 ±1.0
2000	0.0	0.0	0.0 ±2.0
4000	0.0	0.0	0.0 ±3.0
8000	0.0	0.1	0.1 ±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	63.9	-0.1	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

Cert. No. : ACL23168
Job No. : VC66AC0058
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lepeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.7	-0.7	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

COPY

Cert No. : ACL23168
Job No. : VC66AC0058
Pages : 8 of 8

11. Overload indication

Measured value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	
89.6	89.7	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322754



Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00322754 / 196477 / 15486
ID No.: -

Condition As Found : GOOD
Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 02 MAY 2023
Calibration Date : 02 -04 MAY 2023
Date of Issue : 05 MAY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	BEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	BEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	BEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL23143
Job No. : VC66AC0047
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23143
Job No. : VC66AC0047
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	16.3
Flat	22.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.0	0.0	0.0
8000	0.0	0.1	0.1
			Acceptance Limits
			± 1.5
			± 1.0
			±5.0

COPY

Continuation of Calibration Certificate

Cert. No. : ACL23143
Job No. : VC66AC0047
Pages : 5 of 8

Cert. No. : ACL23143
Job No. : VC66AC0047
Pages : 6 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
63	-0.1	0.0	±2.0
125	0.0	0.0	±1.5
250	0.0	0.0	±1.5
500	0.0	-0.1	±1.5
1000	0.0	-0.1	±1.5
2000	0.0	0.0	±1.0
4000	0.0	0.0	±2.0
8000	0.0	0.0	±3.0
	0.0	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.1	0.1	± 1.1
69.0	69.1	0.1	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.1	0.1	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	24.9	-0.1	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL23143
Job No. : VC66AC0047
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

Continuation of Calibration Certificate

Cert. No. : ACL23143
Job No. : VC66AC0047
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	-0.3	±1.5
89.8	89.5		

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

COPY

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00222592



Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42A/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00222592 / 195904 / 15424
ID No.:

Condition As Found : GOOD

Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 10 MAY 2023
Calibration Date : 17 -18 MAY 2023
Date of Issue : 24 MAY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL23164
Job No. : VC66AC0058
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY

Cert. No. : ACL23164
Job No. : VC66AC0058
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.0
C - weight	18.7
Flat	24.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight Acceptance Limits
125	0.3	0.3	± 1.5
1000	0.0	0.0	± 1.0
8000	1.2	1.3	±5.0

COPY

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	0.0	0.0	-0.1
125	0.0	0.1	0.0
250	0.0	0.0	0.0
500	0.0	0.0	0.0
1000	0.0	0.0	0.0
2000	0.0	0.0	0.0
4000	0.0	0.0	0.0
8000	0.0	0.1	0.1

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.0	0.0	± 1.1

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle			
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

SOUND LEVEL METER

MODEL : NL-21

SERIAL No. : 00310456

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Banghumru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



NSC-TS1-TIS 17025
CALIBRATION 0394

Cert. No. : ACL23241
Pages : 1 of 9

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-21/ Microphone UC-52 / Preamplifier NH-21
Serial No.: 00310456 / 153489 / 34625
ID No.: .
Condition As Found : GOOD
Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHA, CHONBURI 20230 THAILAND.

Location : .
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 28 JUNE 2023
Calibration Date : 24-26 JULY 2023
Date of Issue : 02 AUGUST 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

SITHIPORN SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACL23241
Job No. : VC66AC0069
Pages : 2 of 9

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).





Continuation of Calibration Certificate

Cert. No. : ACL23241
Job No. : VC66AC0069
Pages : 3 of 9

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY

T. Petcha

Continuation of Calibration Certificate

Cert. No. : ACL23241
Job No. : VC66AC0069
Pages : 4 of 9

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
22.5

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	21.7
C - weight	22.4
Flat	25.2

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.2	0.2	0.2
1000	0.0	0.0	0.0
8000	-0.8	-0.7	-0.7
			Acceptance Limits
			± 1.5
			± 1.0
			± 5.0

COPY

T. Petcha

Continuation of Calibration Certificate

Cert. No. : ACL23241
Job No. : VC66AC0069
Pages : 5 of 9

Continuation of Calibration Certificate

Cert. No. : ACL23241
Job No. : VC66AC0069
Pages : 6 of 9

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.2	-0.1	-0.1	±2.0
125	-0.1	-0.1	-0.1	±1.5
250	-0.1	-0.1	-0.1	±1.5
500	-0.1	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.1	0.1	0.0	±2.0
4000	0.1	0.1	0.0	±3.0
8000	0.1	0.2	0.2	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
134.0	133.9	-0.1	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	128.9	-0.1	± 1.1
124.0	123.9	-0.1	± 1.1
119.0	118.9	-0.1	± 1.1
114.0	113.9	-0.1	± 1.1
109.0	108.9	-0.1	± 1.1
104.0	103.9	-0.1	± 1.1
99.0	98.9	-0.1	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.7	-0.3	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL23241
Job No. : VC66AC0069
Pages : 7 of 9

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.5
120	94.0	94.0	0.0	±0.5
110	94.0	94.0	0.0	±0.5
100	94.0	94.0	0.0	±0.5
90	94.0	94.1	0.1	±0.5

Level linearity on each level range

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	43.0	42.8	-0.2	±0.5
120	33.0	33.0	0.0	±0.5

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Continuation of Calibration Certificate

Cert. No. : ACL23241
Job No. : VC66AC0069
Pages : 8 of 9

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lpeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	-0.1	±1.5
89.3	89.2		

Continuation of Calibration Certificate

Cert No. : ACL23241
Job No. : VC66AC0069
Pages : 9 of 9

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

J. Petch

SOUND LEVEL METER

MODEL : NL-21

SERIAL No. : 00443357



Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-21/ Microphone UC-52 / Preamplifier NH-21
Serial No.: 00443357 / 153070 / 11330
ID No.:

Condition As Found : GOOD
Customer : EASTERN THAI CONSULTING 1992 CO., LTD.
SAHA GROUP INDUSTRIAL PARK, 683 MOO 11,
NONGKHAM, SIRACHIA, CHONBURI 20230 THAILAND.

Location :
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 16 OCTOBER 2023
Calibration Date : 06-07 NOVEMBER 2023
Date of Issue : 08 NOVEMBER 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :
T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.
3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

COPY

T. Petchur

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

COPY
F. Petcha

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
23.5

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	22.8
C - weight	23.9
Flat	26.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
125	0.6	0.6	± 1.5
1000	-0.1	-0.1	± 1.0
8000	-1.5	-1.4	±5.0

COPY
F. Petcha

Continuation of Calibration Certificate

Cert. No. : ACL23339
Job No. : VC67AC0012
Pages : 5 of 9

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)		
	Flat	C-weight	A-weight
63	-0.2	-0.1	0.0
125	-0.2	0.0	0.0
250	-0.1	0.0	0.0
500	0.0	0.0	0.0
1000	0.0	0.0	0.0
2000	0.1	0.1	0.1
4000	0.1	0.1	0.1
8000	0.0	0.2	0.3

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	93.9	-0.1	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Continuation of Calibration Certificate

Cert. No. : ACL23339
Job No. : VC67AC0012
Pages : 6 of 9

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.1	0.1	± 1.1
44.0	44.3	0.3	± 1.1
39.0	39.8	0.8	± 1.1

Continuation of Calibration Certificate

Cert. No. : ACL23339
Job No. : VC67AC0012
Pages : 7 of 9

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±0.5
120	94.0	94.0	0.0	±0.5
110	94.0	94.1	0.1	±0.5
100	94.0	94.1	0.1	±0.5
90	94.0	94.1	0.1	±0.5

Level linearity on each level range

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	43.0	42.7	-0.3	±0.5
120	33.0	32.6	-0.4	±0.5

9. Tone burst response

Time Weighting	Tone burst duration, T _b (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

Continuation of Calibration Certificate

Cert. No. : ACL23339
Job No. : VC67AC0012
Pages : 8 of 9

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle	-0.1	±1.5
89.4	89.3		

COPY
T. Petch

COPY
T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23339
Job No. : VC67AC0012
Pages : 9 of 9

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

COPY

7. Retu

SOUND LEVEL METER

MODEL : NL-42

SERIAL No. : 00322757



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL BP. 118/0366

Request No. 21-66/0321

CALIBRATION CERTIFICATE

Request No. 21-66/0321

MTC No. EEL BP. 118/0266

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)



Submitted by : Eastern Thai Consulting 1992 Co., Ltd.
Address : 683 Moo 11 Sukhapibarn 8 Rd., Nongkham, Sriracha, Chonburi 20230.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Ambient Environment

Instrument Calibrated :
Description : Sound Level Meter : $(23 \pm 3) ^\circ\text{C}$
Manufacturer : Rion : Relative Humidity : $(50 \pm 15) \%$
Model : NL-42 : Ambient Pressure : $(101.325 \pm 1.5) \text{ kPa}$
Serial No. : 00322757 (No.52)
Microphone : Type UC-52 No.196481
Preamplifier : Type NH-24 No.15489

Standards used :

1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 20 Feb. 2023

Date of Calibration : 13-17 Mar. 2023

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax (66) 0 2577 9000

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax (66) 0 2323 9165

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 13-17 Mar. 2023

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax (66) 0 2577 9000

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax (66) 0 2323 9165

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

COPY

COPY



TISTR

NSC-TIS-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0321

MTC No. EEL. BP. 118/0266

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.96	114.5	114.0	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 123.6 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20.2	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	11.1	0.10	N/A
C-Weight	16.6	0.10	N/A
Flat	22.5	0.10	N/A

Date of Calibration : 13-17 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 R4

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



TISTR

NSC-TIS-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0321

MTC No. EEL. BP. 118/0266

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)		Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight			
125	0.1	0.3	1.5	0.45	0.6
1 000	-0.2	-0.2	1.0	0.45	0.6
8 000	-2.2	-2.2	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)		Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight			
63	-0.1	-0.1	2.0	0.20	0.6
125	-0.1	0.0	1.5	0.20	0.6
250	-0.1	0.0	1.5	0.20	0.6
500	-0.1	0.0	1.5	0.20	0.6
1 000	0.0	0.0	1.0	0.20	0.6
2 000	0.0	-0.1	2.0	0.20	0.6
4 000	0.0	-0.1	3.0	0.20	0.6
8 000	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 13-17 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

COPY

COPY

4/9



Request No. 21-66/0321

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
136	136.0	0.0	1.1	0.30	0.3
135	135.0	0.0	1.1	0.30	0.3
134	134.0	0.0	1.1	0.30	0.3
133	133.0	0.0	1.1	0.30	0.3
132	132.0	0.0	1.1	0.30	0.3
131	131.0	0.0	1.1	0.30	0.3
130	130.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3

Date of Calibration : 13-17 Mar. 2023

...relates only to the items tested/calibrated or value assigned.

The results relate only to the items tested/calibrated or value assigned.

FM.BLMTC.002 Rev.4

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
710
711
712
713
714
715
716
717
718
719
720
721
722
723
724
725
726
727
728
729
730
731
732
733
734
735
736
737
738
739
740
741
742
743
744
745
746
747
748
749
750
751
752
753
754
755
756
757
758
759
760
761
762
763
764
765
766
767
768
769
770
771
772
773
774
775
776
777
778
779
780
781
782
783
784
785
786
787
788
789
790
791
792
793
794
795
796
797
798
799
800
801
802
803
804
805
806
807
808
809
810
811
812
813
814
815
816
817
818
819
820
821
822
823
824
825
826
827
828
829
830
831
832
833
834
835
836
837
838
839
840
84

Office
196 Phahonvithin Road, Chatuchak, Bangkok 10900,

Office/Laboratory
501 IC, Bangpoo Industrial Estate, Sukhumvit Road,
Bangpoo, Samut Prakan 10280, Thailand

Thailand
T-1 1660 2570 1121-30 ext. 5219. 5225. 5217

Tel. (66) 0 2579 1121-30 ext.
Fax (66) 0 2579 8592

Fax: (08) 0 231 7 0372
E-mail: sunmalee@tiscali.or.th

Head Office

Head Office
5 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,

55 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,

Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2677 9000

el. (66) 0 2577 9000
:ay (66) 0 2577 9009

TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL BP. 118/0266

5. Long-term stability

5. Long-term stability					
Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

6.1 Frequency weightings at 1 kHz					
Frequency	Measured Value	Deviated value	Acceptance limit	Uncertainty	Maximum-permitted uncertainty
Weighting	(dB)	(dB)	class 2 (±dB)	(±dB)	of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

6.2 Time weightings at 1 kHz					
Frequency	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Weighting					
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 13-17 Mar. 2023

[illegible]

The results relate only to the items tested/calibrated or value assigned.

FORM B1 MTC-002 Rev

Office/Laboratory _____

Office/Laboratory
196 Phaholajuthong Industrial Estate, Sukhumvit Road,

Soi 1C, Bangpoo Industrial Estate, Samutprakarn
Amphoe Muang Chonburi 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,

Changwat Pathumthani 12120, Thailand

5/5
COPY



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0321

MTC No. EEL. BP. 118/0266

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
54	53.9	-0.1	1.1	0.30	0.3
49	48.9	-0.1	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	34.0	0.0	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	27.0	0.0	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.9	-0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 13-17 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
15 Mu. 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sunalee@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 1090,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sunalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-66/0321

MTC No. EEL. BP. 118/0266

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
20-130	25	25.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	108.9	-0.1	±1.0; -2.5	0.20	0.3
	0.25	100.0	0.0	±1.5; -5.0	0.20	0.3
Slow	200	119.5	-0.1	±1.0	0.20	0.3
	2	100.0	0.0	±1.0; -5.0	0.20	0.3

Date of Calibration : 13-17 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
15 Mu. 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sunalee@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 1090,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sunalee@tistr.or.th



กท.ก.ก.ก.

NSC-TISI-TIS 17025
CALIBRATION 0037

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL. BP. 118/0266

Request No. 21-66/0321

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.5	0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle					
135.4		135.4	0.0	1.5	0.55
					0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	119.0				
End	119.0	0.0	0.3	0.10	0.1

Calibrated by :
(Mr. Pannasit Phasingri)

Approved by :
(Mr. Praveen Khueppa)
Director

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 13-17 Mar. 2023

Date of Issue : 17 Mar. 2023

End of Certificate

Ref : 2011266022000725006
COPY

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9000

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Re

SOUND LEVEL METER

MODEL : NL-42A

SERIAL No. : 00322749

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL. BP. 116/0266

MTC No. EEL. BP. 116/0266

Request No. 21-66/0321

Request No. 21-66/0321

CALIBRATION CERTIFICATE

Submitted by : Eastern Thai Consulting 1992 Co., Ltd.
Address : 683 Moo 11, Sukhapibam 8 Rd., Nongkham, Sriracha, Chonburi, 20230
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :
Description : Sound Level Meter
Manufacturer : Rion
Model : NL-42A
Serial No. : 00322749 (No.44)
Microphone : UC-52 No.196472
Preamplifier : NH-24 No.15481

Standards used :
1. Band Pass Filter Stanford Research Systems SR 650 S/N 28712.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 20 Feb. 2023

Date of Calibration : 16 Mar. 2023

1/5

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR

Head Office 15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changanwat Pathumthani 12120, Thailand Tel. (66) 0 2577 9000 Fax. (66) 0 2577 9009 E-mail : sumalee@tistr.or.th

Office/Laboratory Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changanwat Samutprakan 10280, Thailand Tel. (66) 0 2323 1672-80 ext. 115, 116 Fax. (66) 0 2323 9165 E-mail : mtr@tistr.or.th

FM.BL-MTC.002 R

FM.BL-MTC.002 R

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 16 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR

Head Office 15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changanwat Pathumthani 12120, Thailand Tel. (66) 0 2577 9000 Fax. (66) 0 2577 9009 E-mail : sumalee@tistr.or.th

Office/Laboratory Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changanwat Samutprakan 10280, Thailand Tel. (66) 0 2323 1672-80 ext. 115, 116 Fax. (66) 0 2323 9165 E-mail : mtr@tistr.or.th

FM.BL-MTC.002 R

FM.BL-MTC.002 R

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.97	114.2	114.0	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 113.7 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
14.0	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	11.3	0.10	N/A
C-Weight	17.6	0.10	N/A
Flat	22.3	0.10	N/A

Date of Calibration : 16 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.2	0.2	0.2	1.5	0.45	0.6
1 000	-0.3	-0.2	-0.2	1.0	0.45	0.6
8 000	0.8	0.7	0.6	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response curve (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	0.0	0.0	0.1	2.0	0.20	0.6
125	0.0	0.2	0.1	1.5	0.20	0.6
250	0.0	0.1	0.1	1.5	0.20	0.6
500	0.0	0.1	0.1	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	-0.1	-0.1	2.0	0.20	0.6
4 000	-0.3	-0.3	-0.3	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 16 Mar. 2023

The results relate only to the items tested/calibrated or value assigned. Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL. BP. 116/0266

Request No. 21-66/0321

5. Long-term stability

Time	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 16 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Lead Office : 15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Chongwat Phumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

Office/Laboratory : Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Chongwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtr@tistr.or.th

Office : 196 Phahonyothin Road, Chatuchak, Bangkok 10900
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BL.MTC.002 Re

Request No. 21-66/0321

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

MTC No. EEL. BP. 116/0266

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
128	128.1	0.1	1.1	0.30	0.3
127	127.1	0.1	1.1	0.30	0.3
126	126.1	0.1	1.1	0.30	0.3
125	125.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.1	0.1	1.1	0.30	0.3
74	74.1	0.1	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3

Date of Calibration : 16 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Lead Office : 15 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Chongwat Phumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : sumalee@tistr.or.th

Office/Laboratory : Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Chongwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtr@tistr.or.th

Office : 196 Phahonyothin Road, Chatuchak, Bangkok 10900
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BL.MTC.002 Re

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
44	44.0	0.0	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	34.0	0.0	1.1	0.30	0.3
29	29.0	0.0	1.1	0.30	0.3
28	28.0	0.0	1.1	0.30	0.3
27	27.0	0.0	1.1	0.30	0.3
26	26.0	0.0	1.1	0.30	0.3
25	24.9	-0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2(±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	94.0	94.0	0.0	1.1	0.30	0.3
30-120	94.0	94.0	0.0	1.1	0.30	0.3
20-110	94.0	94.0	0.0	1.1	0.30	0.3
20-100	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 16 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

FM.BLMTC.002 Re'

Head Office
155 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009

Office/Laboratory
Sui 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165

Office
196 Phahonyothin Road, Chatuchak, Bangkok 1090
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8552
E-mail: surnalee@jst.or.th

Date of Calibration : 16 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

FM.BLMTC.002 Re'

Head Office
155 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009

Office/Laboratory
Sui 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165

Office
196 Phahonyothin Road, Chatuchak, Bangkok 1090
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8552
E-mail: surnalee@jst.or.th

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2(±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
40-130	45	45.0	0.0	1.1	0.30	0.3
30-120	35	35.0	0.0	1.1	0.30	0.3
20-110	25	25.0	0.0	1.1	0.30	0.3
20-100	25	25.0	0.0	1.1	0.30	0.3
20-90	25	25.0	0.0	1.1	0.30	0.3
20-80	25	25.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time	Toneburst	Measured	Deviated	Acceptance	Uncertainty	Maximum-permitted uncertainty
Weighting	Duration, Tb(ms)	value (dB)	value (dB)	limit class 2(dB)	(±dB)	of measurement (±dB)
Fast	200	116.0	0.0	±1.0	0.20	0.3
	2	99.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	89.9	-0.1	+1.5; -5.0	0.20	0.3
Slow	200	109.5	-0.1	±1.0	0.20	0.3
	2	90.0	0.0	+1.0; -5.0	0.20	0.3
	200	110.0	0.0	±1.0	0.20	0.3
SEL	2	90.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	80.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 16 Mar. 2023

The results relate only to the items tested/calibrated or value assigned.

The results relate only to the items tested/calculated or value assigned.

FM, BL MTC.002 Re

Head Office	Office/Laboratory	Office
35 Mu. 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand Tel. (66) 0 2577 9000 Fax. (66) 0 2577 9009	Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Amphoe Muang, Changwat Samutprakan 10280, Thailand Tel. (66) 0 2323 1672-80 ext. 115, 116 Tel. (66) 0 2323 9165 Fax. (66) 0 2323 9165 E-mail: emr@elnet.or.th	196 Phahonyothin Road, Chatuchak, Bangkok 1090 Thailand Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217 Fax. (66) 0 2579 8592 E-mail: sunmalee@elnet.or.th

Request No. 21-66/0321

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.3	-0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
136.6	136.6	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Approved by :

Calibrated by : *Wattawat Supanich*

(Mr. Wittawat Supanich)

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Ref : 2011266022000725004

Date of Calibration : 16 Mar. 2023

Date of Issue : 17 Mar. 2023

End of Certificate

The results relate only to the items tested/calibrated or value assigned.

The results of the tests are prohibited unless written permission is obtained from the governor of TISTR.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Re

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road, Thailand

Lead Office
5 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Amphoe Muang, Changwat Samutprakan 10280, Thailand

Changwat Pathumthani 12120, Thailand

Fax. (66) 0 2579 8592

Tel. (66) 0 2323 1672-80 ext. 115, 116

el. (66) 0 2577 9000

E-mail : sumalee@tistr.or.th

Fax. (66) 0 2323 9165

ax. (66) 0 2577 9009

COPY