

ภาคผนวก ค

เอกสารสอบเทียบเครื่องมือ

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Office Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Tisch Environmental, Inc.	TE-5025A 3540	Jiranatee Associates Co., Ltd.	CL-011-65	31 Oct 22	30 Oct 24	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M	Technology Promotion Association (Thailand-Japan)	23P1400	9 May 23	8 May 24	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23P1856	2 Jun 23	1 Jun 24	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23H1201	5 Jun 23	5 Jun 24	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM08130002	UAE Consultant Co., Ltd.	01112023	1 Nov 23	31 Oct 24	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050148	UAE Consultant Co., Ltd.	13112023	13 Nov 23	12 Nov 24	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050149	UAE Consultant Co., Ltd.	01112023	1 Nov 23	31 Oct 24	-
8	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050150	UAE Consultant Co., Ltd.	01112023	1 Nov 23	31 Oct 24	-
9	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM22177051	UAE Consultant Co., Ltd.	21112023	21 Nov 23	20 Nov 24	-
10	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0162121 2016PSIG	Airgas an Air Liquide company	E05N091E15A0014	6 Jun 23	6 Jun 31	-
11	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1200906875	UAE Consultant Co., Ltd.	03112023	3 Nov 23	2 Nov 24	-
12	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1200906876	UAE Consultant Co., Ltd.	09112023	9 Nov 23	8 Nov 24	-
13	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1201778115	UAE Consultant Co., Ltd.	09112023	9 Nov 23	8 Nov 24	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
14	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1201778114	UAE Consultant Co.,Ltd.	03052023	3 May 23	2 May 24	-
15	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1182920012	UAE Consultant Co.,Ltd.	03112023	3 Nov 23	2 Nov 24	-
16	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0143262 2015P5IG	Airgas an Air Liquide company	E04N99E15A01D3	21 Jun 21	21 Jun 24	-
17	Wind Speed/Wind Direction	WSWD	Scarlet Tech Ltd.	WL-21 2205DT0113	Thai Meteorological Department	390/23	1 Nov 23	31 Oct 24	-
18	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6457	Innovative Instrument Co.,Ltd.	23-ACT-064	12 May 23	11 May 24	-
19	Sound Level Meter	L_{Aeq} 24 hours, L_{A90} , L_{A95} , L_{Amax}	Larson Davis	LxT2 0005289	Innovative Instrument Co.,Ltd.	23-SLM-224	28 Jun 23	27 Jun 25	-
20	Sound Level Meter	L_{Aeq} 24 hours, L_{A90} , L_{A95} , L_{Amax}	Larson Davis	LxT2 0005293	Innovative Instrument Co.,Ltd.	23-SLM-210	23 Jun 23	22 Jun 25	-
21	Sound Level Meter	L_{Aeq} 24 hours, L_{A90} , L_{A95} , L_{Amax}	Larson Davis	LxT2 0005294	Innovative Instrument Co.,Ltd.	23-SLM-222	28 Jun 23	27 Jun 25	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate	Apex Instruments, USA.	XC-572-V 0807048	Envi Equipment Service Co., Ltd.	E23-08069	9 Aug 23	8 Aug 24	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide Carbon Monoxide Oxygen	Testo	Testo 350 60899615	Entech Industrial Sulation Co., Ltd.	G 660354	20 Jun 23	19 Jun 24	-
3	Standard Gas	CO, CO ₂ , NO, NO _x , SO ₂ , BALN 400-800-900 ppm	Airgas	CC715540	Airgas	E05NI83E15A0004	27 Feb 19	27 Feb 27	-
4	Standard Gas	CO, CO ₂ , NO, NO _x , SO ₂ , BALN 200-400 ppm	Airgas	CC19340	Airgas	E05NI83E15001C	14 Oct 20	14 Oct 28	-
5	Standard Gas	CO, CO ₂ , NO, NO _x , SO ₂ , BALN 100-200 ppm	Airgas	CC429175	Airgas	E05NI91E15A003C	18 Sep 20	18 Sep 28	-
6	Standard Gas	O ₂ , BALN 15%	Airgas	CC719418	Airgas	E02NI85E15A3432	15 Oct 18	15 Oct 26	-
7	Standard Gas	O ₂ , BALN 7%	Airgas	CC232371	Airgas	E02NI93E15AC00C	12 Jan 21	12 Jan 29	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	SvanteK	SV35A 73246	Innovative Instrument Co.,Ltd.	23-ACT-110	27 Jun 23	26 Jun 24	-
2	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Lairson Davis	CAL150 6306	Innovative Instrument Co.,Ltd.	23-ACT-066	12 May 23	11 May 24	-
3	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	SvanteK	SV35A 73249	Innovative Instrument Co.,Ltd.	23-ACT-111	23 Jun 23	22 Jun 24	-
4	Sound Level Meter	L_{Aeq} 5 minutes, L_{Amax}	Rion, Japan	NL-42 00558036	Sithiporn Associates Co., Ltd.	ACL24057	18 Jan 24	17 Jan 25	-
5	Sound Level Meter	L_{Aeq} 5 minutes, L_{Amax}	Rion, Japan	NL-42 00409023	Sithiporn Associates Co., Ltd.	ACL23129	26 Apr 23	25 Apr 24	-
6	Sound Level Meter	L_{Aeq} 5 minutes, L_{Amax}	Rion, Japan	NL-42 01010782	Sithiporn Associates Co., Ltd.	ACL23148	9 May 23	8 May 24	-
7	Sound Level Meter	L_{Aeq} 5 minutes, L_{Amax}	Rion, Japan	NL-42 00409050	Sithiporn Associates Co., Ltd.	ACL24053	18 Jan 24	17 Jan 25	-
8	Sound Level Meter	L_{Aeq} 5 min, L_{Amax}	Rion, Japan	NL-43 00430305	Sithiporn Associates Co., Ltd.	ACL23289	27 Sep 23	26 Sep 24	-
9	Sound Level Meter	L_{Aeq} 5 min, L_{Amax}	Rion, Japan	NL-43 00430300	Sithiporn Associates Co., Ltd.	ACL23277	15 Sep 23	14 Sep 24	-
10	Sound Level Meter	L_{Aeq} 5 min, L_{Amax}	Rion, Japan	NL-43 00730426	Sithiporn Associates Co., Ltd.	ACL23290	27 Sep 23	26 Sep 24	-
11	Sound Level Meter	L_{Aeq} 8 hours, L_{Aeq} 12 hours, L_{Amax}	Rion, Japan	NL-42 00408982	Sithiporn Associates Co., Ltd.	ACL24051	18 Jan 24	17 Jan 25	-
12	Noise Dosimeter	Noise Dosimeter	SvanteK	SV 104 110833	Innovative Instrument Co.,Ltd.	23-NDM-268	27 Oct 23	26 Oct 24	-
13	Noise Dosimeter	Noise Dosimeter	SvanteK	SV 104 117688	Innovative Instrument Co.,Ltd.	23-NDM-108	12 May 23	11 May 24	-
14	Primary Flow Calibrator	Calibrate personal pump	TSI Inc	4146 41461214007	Innovative Instrument Co., Ltd.	23-AFM-082	23 Mar 23	22 Mar 24	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
15	Aneroid Barometer	Sodium Hydroxide Sulphuric Acid Total Dust Total Hydrocarbons	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23P1857	2 Jun 23	1 Jun 24	-
16	Digital Thermo - Hygrometer	Sodium Hydroxide Sulphuric Acid Total Dust Total Hydrocarbons	Digicon	TH-02 395034175	Technology Promotion Association (Thailand-Japan)	23H1101	24 May 23	23 May 24	-
17	Thermal Environment Monitor	Heat	3M	QuesTemp 32 TPS030008	Innovative Instrument Co.,Ltd.	24-TPM-044	23 Jan 24	22 Jan 25	-
18	Thermal Environment Monitor	Heat	TSI QUEST	QuesTemp 34 TEX040010	Innovative Instrument Co.,Ltd.	23-TPM-335	14 Jul 23	13 Jul 24	-
19	Thermal Environment Monitor	Heat	TSI QUEST	QuesTemp 34 TEX040012	Innovative Instrument Co.,Ltd.	23-TPM-337	14 Jul 23	13 Jul 24	-
20	Thermal Environment Monitor	Heat	TSI QUEST	QuesTemp 34 TEX040016	Innovative Instrument Co.,Ltd.	23-TPM-341	14 Jul 23	13 Jul 24	-
21	Thermal Environment Monitor	Heat	TSI QUEST	QuesTemp 32 TPT030008	Innovative Instrument Co.,Ltd.	23-TPM-502	2 Nov 23	1 Nov 24	-

CERTIFICATE OF CALIBRATION

Certificate No. : CL-011-65

Page 1 of 2 Pages

MEASUREMENT ITEM : Tip Load Orifice
MANUFACTURER : TSCH
MODEL/TYPE : TE-5025A
SERIAL NUMBER : 3540
ID NUMBER : UAE.EFM.176/2563
CONDITION AS-RECEIVED : Used item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 25 Oct 2022
MEASUREMENT DATE : 31 Oct 2022
ISSUE DATE : 02 Nov 2022

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 24.5 °C and 61.0%RH.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:
The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/MC/W2-20. The W2-2004 was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the measurement to realization of the national standards and to realization of the international system of units (SI) through the VSL (National Metrology Institute of Netherlands) via Certificate number: G2211903

Uncertainty of Measurement:
The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM Evaluation of measurement data - Guide to the expression of uncertainty in measurement

Calibrated by:
[] Mr. Sompote Thachulad
[] Miss Jiraporn Lertsomphol



Approved signatory:
Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION IS GRANTED IN WRITING FROM THE LABORATORY

เอกสารไม่ควบคุม

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Orifice inH ₂ O	Y'	Standard Flow [Qs] m ³ /min
1	0.702	758.204	24.560	23.900	57.190	1.568	1.252	0.650
2	0.999	758.182	24.620	24.010	60.852	3.088	1.756	0.919
3	1.119	758.204	24.550	23.960	40.965	4.167	2.041	1.060
4	1.169	758.228	24.540	24.060	30.007	4.728	2.374	1.124
5	1.419	758.202	24.720	24.250	28.776	7.044	2.852	1.366

Slope (w): 1.96180
Intercept (b): -0.03332
Correlation coefficient (r): 0.99914
Uncertainty (k=2): 0.017 m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Ap_meter mmHg	Ap_Orifice inH ₂ O	Y'	Standard Flow [Qs] m ³ /min
1	0.702	758.204	24.560	23.900	57.190	1.568	0.785	0.651
2	0.999	758.182	24.620	24.010	60.852	3.088	1.101	0.920
3	1.119	758.204	24.550	23.960	40.965	4.167	1.279	1.060
4	1.169	758.228	24.540	24.060	30.007	4.728	1.362	1.124
5	1.419	758.202	24.720	24.250	28.776	7.044	1.664	1.368

Slope (w): 1.22877
Intercept (b): -0.02091
Correlation coefficient (r): 0.99914
Uncertainty (k=2): 0.018 m³/min

End of Certificate of Calibration



เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL: 0-2717-3009-24 FAX: 0-2719-9484

Certificate of Calibration

Certificate No. : 23P1400
Page : 1 of 2

Equipment: U-Tube Manometer

Manufacturer: Dwyer

Model: 1221-36-W/M

Serial No.: -

ID No.: UAE.EFM.020/2500

Condition As-Received: Used item

Received Date: 26 April 2023

Calibration Date: 09 May 2023

Reference: 2304-0703WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1010 mbar

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using "DKD-R 6-1" Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PG106P	1189	MP-0137-22	24 Aug 2023

2. This result of calibration was made on requested at the point specified by customer.

3. Scale and conversion factor is 1 kPa = 4.0146293 inH₂O

4. This instrument was used clean air as pressure media.

5. This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6. This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7. The certificate is valid only to the item calibrated on date and place of calibration.

8. This Certification is traceable to the International System of Unit maintained through:

- National Institute of Metrology Thailand (NIMT)

Calibrated by: Suwit Aussarnee
Issue Date: 11 May 2023

Approved Signatory:
[] Phalinee Prabpaipal
[] Sura Suwannasri
[x] Attapol Panurach

เอกสารไม่ควบคุม

B 0314240



Cert.No.: 23P1400
Page: 2 of 2

Result of calibration: Without adjustment
Function: Pressure Measurement
Increasing Pressure

Range: 0 inH₂O to 36 inH₂O
Scale Interval: 0.1 inH₂O (The Fifth Estimate)

Applied Pressure (inH ₂ O)	UUC Indication			ΔP (inH ₂ O)	Error (inH ₂ O)
	High-port side (inH ₂ O)	Low-port side (inH ₂ O)	Low-port side (inH ₂ O)		
0.00	0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	-4.00	8.00	0.00
10.00	5.00	-5.00	-5.00	10.00	0.00
12.00	6.00	-6.00	-6.00	12.00	0.00
14.00	7.02	-7.02	-7.02	14.04	0.04
16.00	8.02	-8.02	-8.02	16.04	0.04
18.00	9.04	-9.04	-9.04	18.08	0.08
20.00	10.04	-10.04	-10.04	20.08	0.08
22.00	11.02	-11.02	-11.02	22.04	0.04
24.00	12.02	-12.02	-12.02	24.04	0.04
26.00	13.02	-13.02	-13.02	26.02	0.02
28.00	14.00	-14.00	-14.00	0.00	-28.00
30.00	15.00	-15.00	-15.00	30.00	0.00
32.00	16.00	-15.98	-15.98	31.98	-0.02
34.00	17.00	-16.96	-16.96	33.96	-0.04
35.80	18.00	-17.04	-17.04	35.94	0.14

The uncertainty of measurement was ± 0.11 inH₂O

* UUC = Unit Under Calibration

* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.

เอกสารไม่ควบคุม

a 1160341



Certificate of Calibration

Certificate No. : 23P1856
Page : 1 of 2

Equipment : Aneroid Barometer
Manufacturer : Barigo
Model : -
Serial No. : -
ID No. : UAE.EMA2.110/2555

Condition As-Received: Used Item
Received Date: 26 May 2023
Calibration Date: 02 June 2023

Reference: 2305-0919WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Atmospheric Pressure: 1006 mbar

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udonsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using "DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0004-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.This result of calibration instrument was in absolute pressure.

5.This instrument was used clean air as pressure media.

6.The certificate is valid only to the item calibrated on date and place of calibration.

7.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew
Issue Date : 08 June 2023

Approved Signatory : *Attapol P.*
[] Phalinnee Prabpalai
[] Sura Suwannasri
[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0316956



Result of calibration:- Without adjustment

Function:- Absolute Pressure Measurement

Range: 720 mmHg to 800 mmHg

Scale Interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	720.43	730.67	740.34	751.52	756.56	761.83	773.53	798.76
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	755.0	760.0	770.0	790.0
Error (mmHg)	-0.43	-0.67	-0.34	-1.52	-1.56	-1.83	-3.53	-8.76

Decreasing Pressure

Applied Pressure (mmHg)	798.76	773.60	761.89	756.65	751.59	740.72	730.68	720.59
UUC* Indication (mmHg)	790.0	770.0	760.0	755.0	750.0	740.0	730.0	720.0
Error (mmHg)	-8.76	-3.60	-1.89	-1.65	-1.59	-0.72	-0.68	-0.59

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-00-

Attapol P.

เอกสารไม่ควบคุม
a 1165202



Certificate of Calibration

Certificate No. : 23H1201
Page : 1 of 2

Equipment : Dial Thermo-Hygrometer
Manufacturer : Barigo
Model : -
Serial No. : -
ID No. : UAE.EMA2.014/2555

Condition As-Received: Used Item
Received Date: 26 May 2023
Calibration Date: 30 May 2023

Reference: 2305-0919WSC
Ambient Temperature: (25 ± 3) °C
Relative Humidity: (50 ± 20) %

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udonsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Hygro-M2 Dew Point Monitor	5112	2360195	20703	02 Aug 2023
2) Handheld Thermometer With Sensor	1523	3240076	231305	15 Mar 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Standards and Technology (NIST) , The United States of America

-Technology Promotion Association (Thailand-Japan), NSO-ONSC Accredited No. Calibration 0008

Calibrated by : Somchai Durmwor
Issue Date : 07 June 2023

Approved Signatory : *Chakrit Waeewanjua*
[x] Chakrit Waeewanjua
[] Ponthippa Tameyskul
[] Viporn Tantiyawutti

เอกสารไม่ควบคุม
B 0316275



Result of Calibration:-

Function: Humidity Measurement

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	55	14.9	1.6
25.0	60.0	66	6.0	1.7
25.0	80.0	78	-2.0	1.9

Result of Calibration:-

Function: Humidity Measurement

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	46	5.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	72	-8.0	1.9

Result of Calibration:-

Function: Temperature Measurement

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
19.987	20.0	0.013	0.72
30.016	30.0	-0.016	0.72
39.944	39.0	-0.944	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-00-

Chakrit Waeewanjua

เอกสารไม่ควบคุม
a 1165294

MULTI-POINT GAS TEST REPORT


Test Date : Nov 1, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM08130002

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0		0.90	0.90	0.90
Level 2	20.00%	100.0	101.3	1.30	1.28	1.28
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb		Average Difference (%)		0.59

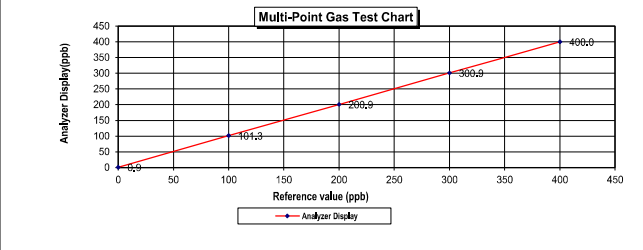

Calculate by

01 Nov / 2023

Approve by

01 Nov / 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 13, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050148

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]	
Level 1	Zero	0.0	0.8	0.80	0.80	0.80	
Level 2	20,00%	100.0	100.7	0.70	0.70	0.70	
Level 3	40,00%	200.0	200.9	0.90	0.45	0.45	
Level 4	60,00%	300.0	300.9	0.90	0.30	0.30	
Level 5	80,00%	400.0	400.0	0.00	0.00	0.00	
Remark : Measuring Range			500.0 ppb		Average Difference (%)		0.45

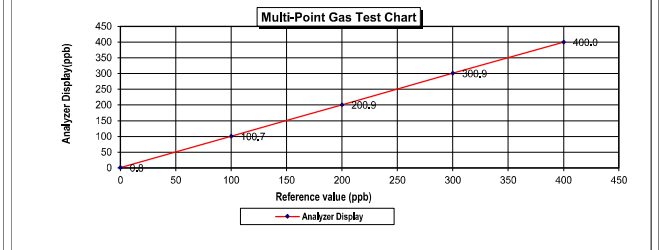

Calculate by

13 Nov / 2023

Approve by

13 Nov / 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 1, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050149

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.6	0.60	0.60	0.60
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.40

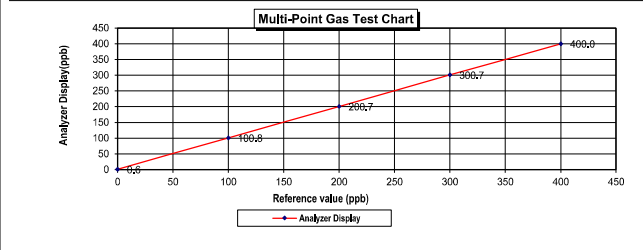

Calculate by

01 Nov / 2023

Approve by

01 Nov / 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 1, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050150

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.70	0.70	0.70
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.38

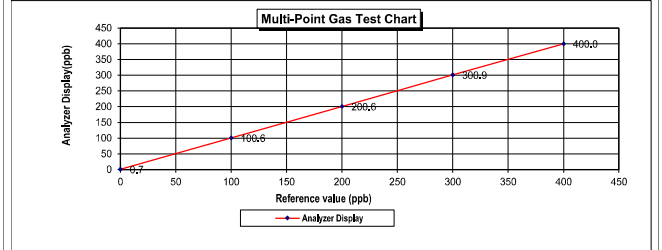

Calculate by

01 Nov / 2023

Approve by

01 Nov / 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 13, 2023

Equipment : Gas Analyzer (NO₂) **Model** : 42i
Manufacturer : Thermo Scientific **Serial Number** : CM19050151

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.8	0.80	0.80	0.80
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)			0.47

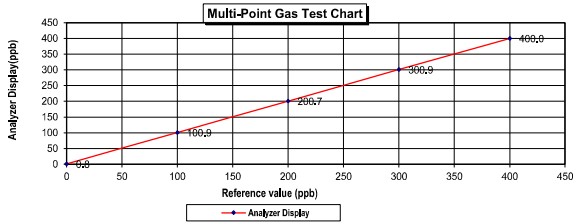

Calculate by

13 Nov 2023

Approve by

13 Nov 2023

CERTIFICATE OF ANALYSIS

Grade of Product: EPA PROTOCOL STANDARD

Customer: AIR LIQUIDE (THAILAND)
LTD.:
Part Number: E05N191E15A0014
Cylinder Number: EB0162121
Laboratory: 124 - Plumsteadville - PA
PGVP Number: A12023
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN

Reference Number: 160-402772205-1
Cylinder Volume: 144.0 CF
Cylinder Pressure: 2016 PSIG
Valve Outlet: 660
Certification Date: Jul 06, 2023

Expiration Date: Jul 06, 2031

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards" (May 2012) document EPA 800/R-12/031, using the assay procedure listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a molar/mole basis unless otherwise noted. The results relate only to the items tested. The report shall not be reproduced except in full without approval of the laboratory. Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.4 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/05/2023
NITRIC OXIDE	100.0 PPM	100.2 PPM	G1	+/- 0.9% NIST Traceable	06/27/2023, 07/05/2023
SULFUR DIOXIDE	100.0 PPM	100.0 PPM	G1	+/- 1.4% NIST Traceable	06/27/2023, 07/05/2023
CARBON MONOXIDE	200.0 PPM	199.2 PPM	G1	+/- 0.3% NIST Traceable	06/29/2023
CARBON DIOXIDE	8,000 %	7,982 %	G1	+/- 1.2% NIST Traceable	06/27/2023
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
GMIS	104202308	CC754364	98.36 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Jan 04, 2031
PRM	C2319101	APE1514048	100.19 PPM NITRIC OXIDE/NITROGEN	+/- 0.3%	Feb 28, 2025
GMIS	2023042525	CC754381	96.52 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Apr 25, 2031
PRM	12409	D913860	15.01 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Feb 17, 2023
GMIS	15340202002	E90130037	9.893 PPM NITROGEN DIOXIDE/NITROGEN	+/- 1.0%	Sep 29, 2025
NTRM	160102-22	KAL003620	97.69 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 01, 2027
CO	230901	CC745902	249.47 PPM CARBON MONOXIDE/NITROGEN	+/- 0.3%	Dec 09, 2028
NTRM	130606-02	CC411738	13.358 PPM CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet iS50 FTIR AUP2010245 CO ₂	FTIR	Jun 15, 2023
SIEMENS ULTRAMATE6 N1-D8-180	NDIR	Jun 14, 2023
Nicolet iS50 FTIR AUP2010245 NO	FTIR	Jun 29, 2023
Nicolet iS50 FTIR AUP2010245 NO ₂	FTIR	Jun 15, 2023
Nicolet iS50 FTIR AUP2010245 SO ₂	FTIR	Jun 08, 2023

Approved for Release

MULTI-POINT GAS TEST REPORT


Test Date : Nov 3, 2023

Equipment : Gas Analyzer (SO₂) **Model** : 43i
Manufacturer : Thermo SCIENTIFIC **Serial Number** : 1200906875

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 24, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	1.1	1.10	1.10	1.10
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	301.0	1.00	0.33	0.33
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.53

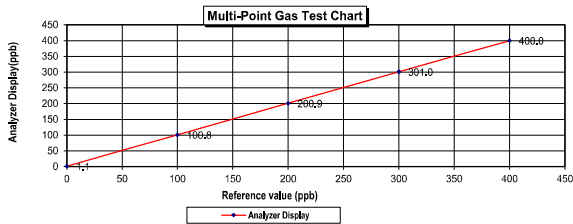

Calculate by

03 Nov 2023

Approve by

03 Nov 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 9, 2023

Equipment : Gas Analyzer (SO₂) **Model** : 43i
Manufacturer : Thermo SCIENTIFIC **Serial Number** : 1200906876

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo SCIENTIFIC
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 24, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.6	0.60	0.60	0.60
Level 2	20.00%	100.0	100.5	0.50	0.50	0.50
Level 3	40.00%	200.0	201.9	1.90	0.94	0.94
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)		0.46	

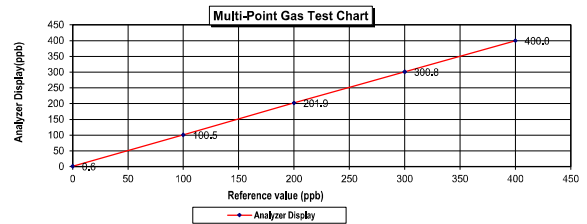

Calculate by

9 Nov 2023

Approve by

9 Nov 2023

MULTI-POINT GAS TEST REPORT

Test Date : Nov 9, 2023

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1201778115

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 24, 2024

Dilutor Detail

Manufacturer : Thermo SCIENTIFIC
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	% Error	
Level 1	Zero	0.0	0.7	0.70	0.70	0.70	
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60	
Level 3	40.00%	200.0	200.8	0.80	0.40	0.40	
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30	
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00	
Remark : Measuring Range			500.0 ppb		Average Difference (%)		0.40

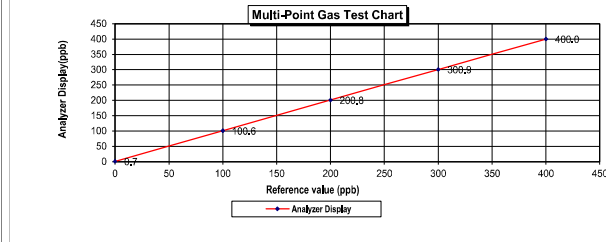

Calculate by

.....
03/...../.....11/...../.....66.....

Approve by

.....
03/...../.....Nov...../.....2023

MULTI-POINT GAS TEST REPORT

Test Date : May 3, 2023

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1201778114

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 24, 2024

Dilutor Detail

Manufacturer : Thermo SCIENTIFIC
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	% Error]
Level 1	Zero	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	0.80	0.79	0.79
Level 3	40.00%	200.0	0.70	0.35	0.35
Level 4	60.00%	300.0	1.60	0.53	0.53
Level 5	80.00%	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb			Average Difference (%)		0.33

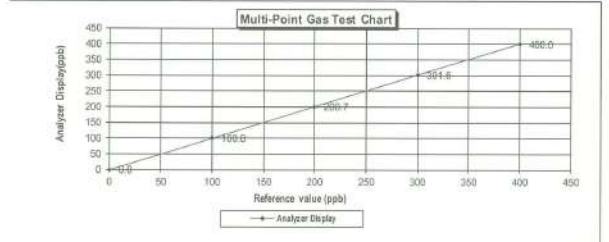

Calculate by

.....
03/...../.....11/...../.....66.....

Approve by

.....
03/...../.....May...../.....2023

MULTI-POINT GAS TEST REPORT

Test Date : Nov 3, 2023

Equipment : Gas Analyzer (SO₂) Model : 43i
Manufacturer : Thermo SCIENTIFIC Serial Number : 1182920012

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 24, 2024

Dilutor Detail

Manufacturer : Thermo SCIENTIFIC
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	% Error
Level 1	Zero	0.0	0.7	0.70	0.70	0.70
Level 2	20.00%	100.0	0.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.5	0.50	0.25	0.25
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.37

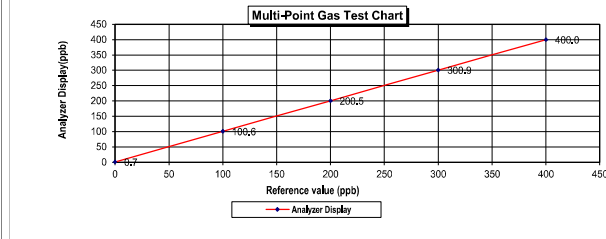

Calculate by

.....
03/...../.....Nov...../.....2023

Approve by

.....
03/...../.....Nov...../.....2023

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: EB0143262
Cylinder Number: 124 - Durham (SAF) - NC
Laboratory: B2202
Gas Code: CO, NO, NO₂, SO₂, BALN
Reference Number: 122-402135167-1
Cylinder Volume: 144.4 CF
Cylinder Pressure: 2015 PSI
Valve Outlet: 560
Certification Date: Jun 21, 2021
Expiration Date: Jun 21, 2024

Certificate performed in accordance with EPA Traceability Protocol for Analysis and Certification of Gaseous Calibration Standards (May 2012) (EPA 821-R-12-001). During the assay process, the Analytical Methodology does not require correction for analytical interference. The cylinder has a serial number 124 - Durham (SAF) - NC. There are no significant impurities which affect the use of this calibration gas. All concentrations are in % by volume unless otherwise noted.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NO _x	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	08/14/2021, 08/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	08/14/2021, 08/21/2021
SULFUR DIOXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	08/14/2021, 08/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 1.5% NIST Traceable	08/14/2021, 08/21/2021
NITROGEN	Balance	Balance	G1	+/- 0.75% NIST Traceable	08/14/2021

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NITROGEN	20201102	CC078028	45.92 PPM NITRIC OXIDE/NITROGEN	+/- 1.3%	Feb 02, 2025
PM	2186	CC080025	9.91 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.3%	Feb 20, 2020
PM	00142028183	CC080025	4.345 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 16, 2023
NITROGEN	16011043	CC0473277	45.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.2%	Jun 17, 2022
NITROGEN	14028118	CC0451277	395.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.2%	Nov 16, 2025

Instrument/Make/Model	Analytical Principle	Last Multi-point Calibration
N code: 9700 AHR800-333 CO	FTIR	Jun 03, 2021
N code: 9700 AHR800-333 NO	FTIR	Jun 03, 2021
N code: 9700 AHR800-333 NO ₂	FTIR	Jun 03, 2021
N code: 9700 AHR800-333 SO ₂	FTIR	Jun 03, 2021

Test Data Available Upon Request

NOTES: PO #522-007607

GROSS WT: 23.40kg

NET WT: 4.72kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This includes the test report.

Approved for Release



เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Calibration Certificate

Issued by: Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 1 November, 2023

Certification No. 390/23

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2205DR0113

Wind Sensor 2205DT0113

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Sol Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1013.5 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425

: Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer

Model DA-650-3TV

(sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

: Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER

: Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02618057

: Thermoschnelder No.918802

STANDARD BAROMETER

: Digital Barometer Vaisala Type PTB220 No. V1220015

: Digital Barometer Vaisala Type PTB350 No. 4320001

Calibrated by: Watcharapol

Signed:

Mr. Pisob Promsat

Authorized Signatory

for the Chief

Sub-Standard Instrument

Mr. Watcharapol Subwat

Mechanical Engineer



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

1 November, 2023

Certification No. 390/23

Page : 2 of 5

Standard Ultrasonic Anemometer	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacuum inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	1.0	0.0
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.0
7.04	-	-	-	7.0	0.04
9.02	-	-	-	8.9	0.12
11.02	-	-	-	9.0	2.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.9	0.11
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.9	0.12

Wind Aloft Plotting Board.	
U.S. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by: Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

Certification No. 390/23

1 November, 2023

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
1009.68	1009	0.68
1007.51	1007	0.51
1007.13	1007	0.13
1006.90	1007	-0.10
1006.72	1007	-0.28
1006.59	1006	0.59
1006.28	1006	0.28
1006.05	1006	0.05
1005.84	1006	-0.16
1005.48	1006	0.48
1009.61	1010	-0.39
1009.76	1010	-0.24
1009.69	1009	0.69
1009.45	1009	0.45
1009.24	1009	0.24
1008.89	1009	-0.11
1007.86	1006	-0.34
1006.99	1007	-0.01
1006.29	1006	0.29
1004.56	1006	-0.44

Average

0.12

Calibrated by: Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

1 November, 2023

Certification No. 390/23

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
757.32	757	0.32
755.69	756	-0.31
755.41	755	0.41
755.24	755	0.24
755.10	755	0.10
755.00	755	0.00
754.77	755	-0.23
754.60	754	0.60
754.44	754	0.44
754.17	754	0.17
757.27	757	0.27
757.38	757	0.38
757.33	757	0.33
757.15	757	0.15
756.99	757	-0.01
756.73	757	-0.27
755.81	756	-0.19
755.30	755	0.30
754.78	755	-0.22
753.48	753	0.48

Average

0.15

Calibrated by: Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

The Result of Calibration

1 November, 2023

Certification No. 390/23

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.12	45	0.12
30.21	30	0.21
15.42	15	0.42

Calibrated by :

Mr. Watcharapol Subwat

Mechanical Engineer



Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/19 MOO 13, SOI SUTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5800-1 FAX: 0660-2116-7140



Page 1 of 2

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-ACT-064
Request No : Req-2023-0975

Unit Under Calibration Details

Measurement item : Acoustic Calibrator
Manufacturer : LARSON DAVIS
Model : CAL150
Serial Number : 6457
ID : UAE.EFM.055/2564
Class : 2
Range : 94, 114 dB / 1000 Hz
Instrument Status : Used

Calibration Environment and Details

Temperature : (23 ± 2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ± 10.0 hPa)
Received Date : 9 May 2023
Calibration Date : 12 May 2023
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	31 May 2023
THD Multimeter	2015	1047765	NIMT	31 January 2024

Traceability

This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :

Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 12 May 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/19 MOO 13, SOI SUTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5800-1 FAX: 0660-2116-7140



Page 2 of 2

Certificate No : 23-ACT-064

Request No : Req-2023-0975

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 2 (± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	93.91	-0.09	-	-	0.13	0.40
114 dB / 1000 Hz	113.97	-0.03	-	-	0.13	0.40

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 2 (± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty (± %)	Acceptance limit Class 2 (± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.13	-	0.40	3.0
114 dB / 1000 Hz	0.29	-	0.40	3.0

Note :

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/19 MOO 13, SOI SUTINAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0660-2116-5800-1 FAX: 0660-2116-7140



Page 1/6

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-SLM-224
Request No : Req-2023-1412

Unit Under Calibration Details

Measurement item : Sound Level Meter
Manufacturer : LARSON DAVIS
Model : Lst2
Serial Number : 0005289
ID : UAE.EFM.105/2562
Resolution : 0.1 dB
Microphone Class : 2
Microphone Model : 375B02
Microphone S/N : 011752
Preamplifier Model : PRMLxT2B
Preamplifier S/N : 056076
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 26 June 2023
Calibrated Date : 28 June 2023
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	29 June 2023	TSI
Audio Generator	Svantek	Svan401	131	12 October 2023	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By :

Mr. Noppadon Luangart
Calibration Officer

Approved By :

Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 28 June 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

Certificate No : 23-SLM-224

Request No : Req-2023-1412

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
	Level (dB)	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)		
FAST / A / 37-139							
Calibrator Setting							
1000 Hz 114 dB	113.77	114.3	+0.53	113.8	+0.03	0.2	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN, 73246

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(\pm dB)
A	30.0	0.1

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(\pm dB)
A	29.7	0.1
C	29.1	0.1
Z	33.7	0.1

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
	A	C	Z		
FAST / 37-139					
STD Setting	(dB)	(dB)	(dB)		
125 Hz	0.0	0.2	0.0	0.6	2.0
1000 Hz	0.0	0.0	0.0	0.6	1.0
4000 Hz	1.1	1.1	1.1	0.6	3.0
8000 Hz	2.4	2.4	2.4	0.7	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-224

Request No : Req-2023-1412

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
	A (dB)	C (dB)	Z (dB)		
FAST / 37-139					
STD Setting					
63 Hz	-0.1	0.0	0.0	0.2	2.0
125 Hz	-0.1	0.1	0.0		1.5
250 Hz	0.0	0.0	0.0		1.5
500 Hz	0.0	0.1	0.0		1.5
1000 Hz	0.0	0.0	0.0		1.0
2000 Hz	0.1	0.1	0.0		2.0
4000 Hz	0.0	0.1	0.1		3.0
8000 Hz	0.0	0.0	0.1		5
16000 Hz	0.0	0.0	-0.1		+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
	REF	UUC (dB)	ERR (dB)		
FAST / 37-139					
UUC Weighting	(dB)	(dB)	(dB)		
A	114.00	114.0	0.0	0.2	0.2
C	114.00	114.0	0.0		0.2
Z	114.00	114.0	0.0		0.2

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
	REF	UUC (dB)	ERR (dB)		
37-139 / A					
UUC Time Response	(dB)	(dB)	(dB)		
Fast	114.00	114.0	0.0	0.2	0.1
Slow	114.00	114.0	0.0		0.1
Leq	114.00	114.0	0.0		0.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-224

Request No : Req-2023-1412

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / A / 37-139	UUC		
STD Setting	(dB)		
Initial	114.0		
Final	114.0		
Deviated	0.0		

8. Level linearity on the reference level range

UUC Setting	Anticipated		Deviation	UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
	REF	UUC			
FAST / A / 37-139					
STD dB	(dB)	(dB)	(dB)		
142.00	142	142.0	0.0	0.3	0.3
139.00	139	139.0	0.0		1.1
134.00	134	134.0	0.0		1.1
129.00	129	129.0	0.0		1.1
124.00	124	124.0	0.0		1.1
119.00	119	119.0	0.0		1.1
114.00	114	114.0	0.0		1.1
109.00	109	109.0	0.0		1.1
104.00	104	104.0	0.0		1.1
99.00	99	99.0	-0.1		1.1
94.00	94	93.9	-0.1		1.1
89.00	89	88.8	-0.1		1.1
84.00	84	83.9	-0.1		1.1
79.00	79	78.9	-0.1		1.1
74.00	74	73.8	-0.1		1.1
69.00	69	68.9	-0.1		1.1
64.00	64	63.9	-0.1		1.1
59.00	59	58.9	-0.1		1.1
54.00	54	53.9	-0.1		1.1
49.00	49	49.0	0.0		1.1
44.00	44	44.1	0.1		1.1
39.00	39	39.4	0.4		1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-224

Request No : Req-2023-1412

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
	REF	UUC (dB)	ERR (dB)		
FAST / A					
UUC Range	(dB)	(dB)	(dB)		
37-139	44.8	44.9	0.1	0.3	1.1
	114	114.0	0.0		1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
	Toneburst		Ref	UUC		
A / 37-139						
UUC Time Response	(ms)	(dB)	(dB)	(dB)		
Fast	200	135.0	134.9	-0.1	0.2	1
	2	118.0	117.8	-0.2		+1.0, -2.5
	0.25	109.0	108.6	-0.4		+1.5, -5.0
Slow	200	128.6	128.5	-0.1		1
	2	109.0	108.8	-0.2		+1.0, -5.0
	200	129.0	129.0	0.0		1
SEL	2	109.0	109.0	0.0		+1.0, -2.5
	0.25	100.0	99.8	-0.2		+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / C / 95-142	REF	UUC (dB)	ERR (dB)		
STD Setting	(dB)	(dB)	(dB)		
Complete cycle	137.4	136.7	-0.70	0.2	2.0
Positive half cycle	136.4	136.2	-0.20		2.0
Negative half cycle	136.4	136.2	-0.20		2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-224
Request No : Req-2023-1412

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)	(± dB)	(± dB)
Positive one-half cycle	143.9		
Negative one-half cycle	144.0		
Deviated	-0.1	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)	(± dB)	(± dB)
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangkok, Prakanong, Bangkok
10260
Certificate No : 23-SLM-210
Request No : Req-2023-1387

Unit Under Calibration Details

Measurement Item : Sound Level Meter
Microphone Class : 2
Manufacturer : LARSON DAVIS
Microphone Model : 375A04
Model : LA72
Microphone S/N : 346306
Serial Number : 0005293
Preamplifier Model : PRMLA72B
ID : UAE.EFM.108/2562
Preamplifier S/N : 056084
Resolution : 0.1 dB
Instrument Status : Used

Calibration Environment and Details


Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 21 June 2023
Calibrated Date : 23 June 2023
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3:2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic


Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EF A000234	29 June 2023	TSI
Audio Generator	Svante	Svan401	131	12 October 2023	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadol Luangart
Calibration Officer

Approved By : 
Mr. Pait Mahavorn
Calibration Engineer Supervisor
Issue Date : 23 June 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-210
Request No : Req-2023-1387

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust	After Adjust	UNCERTAINTY	Acceptance
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)
1000 Hz 114 dB	114.54	114.5	-0.04	114.5	-0.04
				(± dB)	(± dB)
				0.2	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand JM, Model AC-300, SN, AC-300001087

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	24.1	0.1

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	23.5	0.1
C	23.0	0.1
Z	27.5	0.1

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve	UNCERTAINTY	Acceptance
FAST / 37-139	A C Z	(± dB)	Limit
STD Setting	(dB) (dB) (dB)	(± dB)	(± dB)
125 Hz	0.0 0.1 0.1	0.6	2.0
1000 Hz	0.0 0.0 0.0	0.6	1.0
4000 Hz	0.0 0.0 0.1	0.6	3.0
8000 Hz	-0.6 -0.6 -0.5	0.7	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-210
Request No : Req-2023-1387

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve	UNCERTAINTY	Acceptance
FAST / 37-139	A (dB) C (dB) Z (dB)	(± dB)	Limit
STD Setting	(dB) (dB) (dB)	(± dB)	(± dB)
63 Hz	-0.2 -0.1 -0.1	0.2	2.0
125 Hz	-0.1 0.0 -0.1	0.2	1.5
250 Hz	-0.1 -0.1 -0.1	0.2	1.5
500 Hz	-0.1 0.0 -0.1	0.2	1.5
1000 Hz	0.0 0.0 0.0	0.2	1.0
2000 Hz	0.0 0.0 0.0	0.2	2.0
4000 Hz	0.0 0.0 0.0	0.2	3.0
8000 Hz	-0.1 -0.1 0.0	0.2	5
16000 Hz	-0.1 -0.1 -0.1	0.2	+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance
FAST / 37-139		REF	UUC		
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	Limit (± dB)
A	114.00	114.0	0.0	0.2	0.2
C	114.00	114.0	0.0		0.2
Z	114.00	114.0	0.0		0.2

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance	
27-139 / A	REF	UUC	ERR	(± dB)	Limit	
UUC Time Response	(dB)	(dB)	(dB)		(± dB)	
Fast	114.00	114.0	0.0		0.2	0.1
Slow	114.00	114.0	0.0			0.1
Leq	114.00	114.0	0.0	0.1		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-210

Request No : Req-2023-1387

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)	(\pm dB)	(\pm dB)
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation	UNCERTAINTY	Acceptance
FAST / A / 37-139	REF	UUC	ERR	Limit
STD dB	(dB)	(dB)	(dB)	(\pm dB)
139.00	139	139.0	0.0	1.1
134.00	134	134.0	0.0	1.1
129.00	129	129.0	0.0	1.1
124.00	124	124.0	0.0	1.1
119.00	119	119.0	0.0	1.1
114.00	114	114.0	0.0	1.1
109.00	109	109.0	0.0	1.1
104.00	104	104.0	0.0	1.1
99.00	99	99.0	0.0	1.1
94.00	94	93.9	-0.1	1.1
89.00	89	88.9	-0.1	1.1
84.00	84	83.9	-0.1	1.1
79.00	79	78.9	-0.1	1.1
74.00	74	73.9	-0.1	1.1
69.00	69	68.9	-0.1	1.1
64.00	64	63.9	-0.1	1.1
59.00	59	58.9	-0.1	1.1
54.00	54	53.9	-0.1	1.1
49.00	49	49.0	0.0	1.1
44.00	44	44.0	0.0	1.1
39.00	39	39.1	0.1	1.1
34.00	34	34.1	0.1	1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-210

Request No : Req-2023-1387

9. Level linearity including the level range control

UUC Setting	STD	Measured	UNCERTAINTY	Acceptance
FAST / A	REF	UUC	ERR	Limit
UUC Range	(dB)	(dB)	(dB)	(\pm dB)
37-139	39.3	39.5	0.2	1.1
	114	114.0	0.0	1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured	UNCERTAINTY	Acceptance
A / 37-139	Toneburst	Ref	UUC	ERR	Limit
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(\pm dB)
Fast	200	135.0	135.0	0.0	1
	2	118.0	117.9	-0.1	+1.0, -2.5
	0.25	109.0	108.8	-0.4	+1.5, -5.0
Slow	200	128.6	128.5	-0.1	1
	2	109.0	108.9	-0.1	+1.0, -5.0
SEL	200	129.0	129.0	0.0	1
	2	109.0	109.1	+0.1	+1.0, -2.5
	0.25	100.0	99.8	-0.2	+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured	UNCERTAINTY	Acceptance
FAST / C / 95-142	REF	UUC	ERR	Limit
STD Setting	(dB)	(dB)	(dB)	(\pm dB)
Complete cycle	137.4	136.6	-0.80	3.0
Positive half cycle	136.4	136.2	-0.20	2.0
Negative half cycle	136.4	136.2	-0.20	2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-210

Request No : Req-2023-1387

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)	(\pm dB)	(\pm dB)
Positive one-half cycle	142.5		
Negative one-half cycle	142.7		
Deviated	-0.2	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)	(\pm dB)	(\pm dB)
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name

UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Address

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-SLM-222

Request No : Req-2023-1410

Unit Under Calibration Details

Measurement item :

Sound Level Meter

Microphone Class : 2

Manufacturer :

LARSON DAVIS

Microphone Model : 375B02

Model :

LA52

Microphone S/N : 011736

Serial Number :

0005294

Preamplifier Model : PRMLAT2B

ID :

UAE-EFM-109-2562

Preamplifier S/N : 056093

Resolution :

0.1 dB

Instrument Status : Used

Calibration Environment and Details

Temperature :

23 °C ± 2 °C

Humidity :

50 %RH ± 20 %RH

Barometric Pressure :

1013 hPa ± 10 hPa

Received Date :

26 June 2023

Calibrated Date :

28 June 2023

Calibration Procedure :

In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests

Location of Calibration :


Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	29 June 2023	TSI
Audio Generator	Svante	Svan401	131	12 October 2023	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangrat
Calibration Officer

Approved By : 
Mr. Paitit Mathavorn
Calibration Engineer Supervisor
Issue Date : 28 June 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY	Acceptance
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR	(± dB)	Limit
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)		
1000 Hz 114 dB	113.77	114.0	+0.23	113.8	+0.03	0.2	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN: 73246

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(± dB)
A	30.5	0.1

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(± dB)
A	30.0	0.1
C	29.6	0.1
Z	33.8	0.1

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY	Acceptance
FAST / 37-139	A	C	Z	(± dB)	(± dB)
STD Setting	(dB)	(dB)	(dB)	0.6	2.0
125 Hz	0.1	0.1	0.1		
1000 Hz	0.0	0.0	0.0		
4000 Hz	1.1	1.1	1.1		
8000 Hz	2.7	2.7	2.7		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY	Acceptance
FAST / 37-139	A	C	Z	(± dB)	(± dB)
STD Setting	(dB)	(dB)	(dB)	0.2	2.0
63 Hz	-0.1	0.0	0.0		
125 Hz	-0.1	0.1	0.0		
250 Hz	0.0	0.0	0.0		
500 Hz	0.0	0.1	0.0		
1000 Hz	0.0	0.0	0.0		
2000 Hz	0.1	0.1	0.0		
4000 Hz	0.0	0.0	0.0		
8000 Hz	0.0	0.0	0.1		
16000 Hz	0.0	-0.1	-0.1		

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance
FAST / 37-139	REF	UUC	ERR	(± dB)	Limit
UUC Weighting	(dB)	(dB)	(dB)	0.2	0.2
A	114.00	114.0	0.0		
C	114.00	114.0	0.0		
Z	114.00	114.0	0.0		

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance
37-139 / A	REF	UUC	ERR	(± dB)	Limit
UUC Time Response	(dB)	(dB)	(dB)	0.2	0.1
Fast	114.00	114.0	0.0		
Slow	114.00	114.0	0.0		
Leq	114.00	114.0	0.0		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC	(± dB)	Limit
STD Setting	(dB)	0.1	0.3
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY	Acceptance
FAST / A / 37-139	REF	UUC	ERR	(± dB)	Limit
STD dB	(dB)	(dB)	(dB)	0.3	1.1
143.00	143	142.9	-0.1		
138.00	139	139.0	0.0		
134.00	134	134.0	0.0		
128.00	129	129.0	0.0		
124.00	124	124.0	0.0		
118.00	119	119.0	0.0		
114.00	114	114.0	0.0		
108.00	109	109.0	0.0		
104.00	104	104.0	0.0		
99.00	99	99.0	0.0		
94.00	94	94.0	0.0		
89.00	89	89.0	0.0		
84.00	84	84.0	0.0		
79.00	79	79.0	0.0		
74.00	74	74.0	0.0		
69.00	69	69.0	0.0		
64.00	64	64.0	0.0		
59.00	59	59.0	0.0		
54.00	54	54.0	0.0		
49.00	49	49.1	0.1		
44.00	44	44.2	0.2		
43.00	43	43.2	0.2		
42.00	42	42.4	0.4		
41.00	41	41.5	0.3		
40.00	40	40.5	0.5		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance
FAST / A	REF	UUC	ERR	(± dB)	Limit
UUC Range	(dB)	(dB)	(dB)	0.3	1.1
37-139	45.4	45.6	0.2		
	114	114.0	0.0		

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance
A / 37-139	Toneburst	Ref	UUC	ERR	(± dB)	Limit
UUC Time Response	(ms)	(dB)	(dB)	(dB)	0.2	1.1
Fast	200	135.0	135.0	0.0		
	2	118.0	117.6	-0.4		
	0.25	109.0	108.5	-0.5		
Slow	200	128.6	128.5	-0.1		
	2	109.0	108.9	-0.1		
	200	129.0	129.0	0.0		
SEL	2	109.0	108.9	-0.1		
	0.25	100.0	99.7	-0.3		

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance
FAST / C / 95-142	REF	UUC	ERR	(± dB)	Limit
STD Setting	(dB)	(dB)	(dB)	0.2	2.0
Complete cycle	137.4	136.7	-0.70		
Positive half cycle	136.4	136.2	-0.20		
Negative half cycle	136.4	136.2	-0.20		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)	(\pm dB)	(\pm dB)
Positive one-half cycle	144.5		
Negative one-half cycle	144.5		
Deviated	0.0	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)	(\pm dB)	(\pm dB)
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

Envi Equipment Service Co., Ltd.
110/254 Moo 3, Tambon Bang Rak Phatthana, Amphur Bang Rua Thong, Nonthaburi 11110
Tel. 098 362 9152, 089 478 7885
E-mail: sales@envi-ees.com

Certificate No. : E23-08069
Page : 1 of 6

CERTIFICATE OF CALIBRATION

Customer : United Analyst and Engineering Consultant Co., Ltd.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, BANGKOK, Phrakhanong, Bangkok 10260
Description of Equipment : Console meter
Manufacturer : Apex Instrument
Model Number : XC-572-V
Serial Number : 0807048
ID./Control No. : -
Environment Conditions : Temperature (25 \pm 2) °C
Humidity (50 \pm 15) % RH
Cal. Date : 09/08/2023
Issue Date : 09/08/2023

Calibration Method or Calibration Procedure Used

US EPA Method (United State Environmental Protection Agency)

This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : Mr. Sanya Sangnil

Approved by :
(Mr. Mana Fueknoi)
Technical Manager



เอกสารไม่ควบคุม

Certificate No. : E23-08069
Page : 2 of 6

METHOD 5 CONSOLE CALIBRATION USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425 5-POINT METRIC UNIT

Meter Console Information		Calibration Conditions				Factors/Conversions			
Console Model Number	XC-572-V	Date	Time	09/08/2023	09:45 AM	Std Temp	293	K	
Console Serial Number	0807048	Calibration Reference No.	SER23-08028			Std Press	760	mm Hg	
DGM Model Number	SK25EX	Barometric Pressure	758.24	mmHg		K _i	0.386		
DGM Serial Number	00003811	Calibration Meter Gamma	0.999			Console Leak Check	PASS		

Calibration Data									
Run Time		Metering Console				Calibration Meter			
Elapsed	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
(Q)	(P _o)	(V _{in})	(V _{out})	(t _{in})	(t _{out})	(V _{in})	(V _{out})	(t _{in})	(t _{out})
min	mm H ₂ O	m ³	m ³	°C	°C	m ³	m ³	°C	°C
12.83	13.0	1149.315	1149.455	29	29	160.47814	160.62142	27	27
12.87	13.0	1149.455	1149.595	29	29	160.62142	160.76496	27	27
9.27	26.0	1149.606	1149.746	29	29	160.78130	160.92678	27	27
9.23	26.0	1149.746	1149.886	29	29	160.92678	161.07252	26	26
14.58	40.0	1149.894	1150.174	29	29	161.08058	161.37034	26	26
14.60	40.0	1150.174	1150.454	29	29	161.37034	161.65974	26	26
11.07	70.0	1150.467	1150.747	29	29	161.67304	161.95980	26	26
11.07	70.0	1150.747	1151.027	29	29	161.95980	162.24604	25	25
9.52	90.0	1151.038	1151.318	29	29	162.25684	162.54152	25	25
9.50	90.0	1151.318	1151.598	30	30	162.54152	162.82528	25	25



เอกสารไม่ควบคุม

Certificate No. : E23-08069
Page : 3 of 6

METHOD 5 CONSOLE CALIBRATION USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425 5-POINT METRIC UNIT

Meter Console Information		Calibration Conditions				Factors/Conversions	
Console Model Number	XC-572-V	Date	Time	09/08/2023	09:45 AM	Std Temp	293 K
Console Serial Number	0807048	Calibration Reference No.	SER23-08028			Std Press	760 mm Hg
DGM Model Number	SK25EX	Barometric Pressure	758.24	mmHg		K _i	0.386
DGM Serial Number	00003811	Calibration Meter Gamma	0.999			Console Leak Check	PASS


Calibration Data									
Results									
Standardized Data				Dry Gas Meter					
Dry Gas Meter		Calibration Meter		Calibration Factor		Flowrate		Std & Corr	
(V _{in} (std))	(Q _{in} (std))	(V _{out} (std))	(Q _{out} (std))	Value	Variation	(Q _{in} (std)(corr))	(ΔH _g)	(ΔH _g)	Variation
m ³	m ³ /min	m ³	m ³ /min	(Y)	(ΔY)	m ³ /min	mm H ₂ O	(ΔH _g)	(ΔH _g)
0.137	0.011	0.139	0.011	1.021	-0.001	0.011	48.480	0.343	
0.137	0.011	0.140	0.011	1.023	0.001	0.011	48.556	0.419	
0.137	0.015	0.142	0.015	1.035	0.014	0.015	49.161	1.024	
0.137	0.015	0.142	0.015	1.037	0.016	0.015	48.472	0.335	
0.275	0.019	0.283	0.019	1.030	0.008	0.019	47.188	-0.949	
0.275	0.019	0.283	0.019	1.029	0.007	0.019	47.414	-0.724	
0.276	0.025	0.280	0.025	1.016	-0.005	0.025	48.836	0.699	
0.277	0.025	0.281	0.025	1.014	-0.007	0.025	48.850	0.713	
0.277	0.029	0.279	0.029	1.007	-0.015	0.029	47.137	-1.000	
0.277	0.029	0.278	0.029	1.004	-0.018	0.029	47.277	-0.860	
				1.022	Y Average			48.137	ΔH@ Average

Note: For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is ± 0.02 .
For ΔH_g , orifice pressure differential that equates to 0.75 cfm (0.0212 m³/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is ± 0.2 inches (5.1 mm).




เอกสารไม่ควบคุม

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	09/08/2023	09:45 AM	Std Temp	293	K
Console Serial Number	0807048	Calibration Reference No.	SER23-08028			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	758.24			K1	0.386	
DGM Serial Number	00003811	Calibration Meter Gamma	0.999			Console Leak Check	PASS	

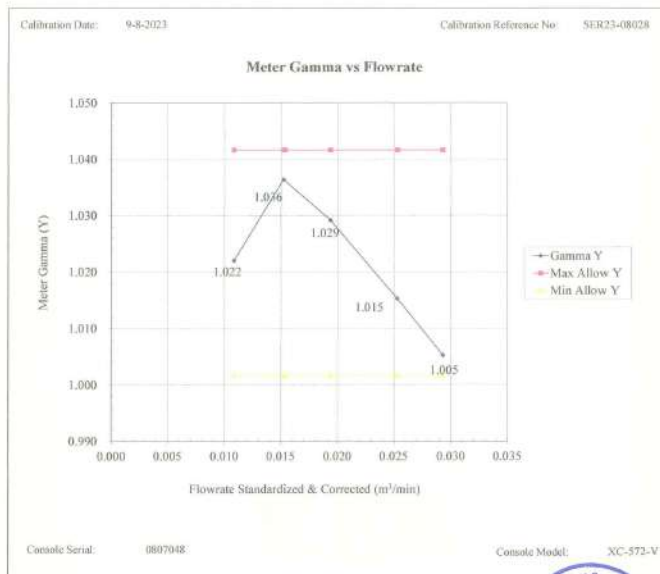

เอกสารไม่ควบคุม

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	09/08/2023	09:45 AM	Std Temp	293	K
Console Serial Number	0807048	Calibration Reference No.	SER23-08028			Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure	758.24			K1	0.386	
DGM Serial Number	00003811	Calibration Meter Gamma	0.999			Console Leak Check	PASS	

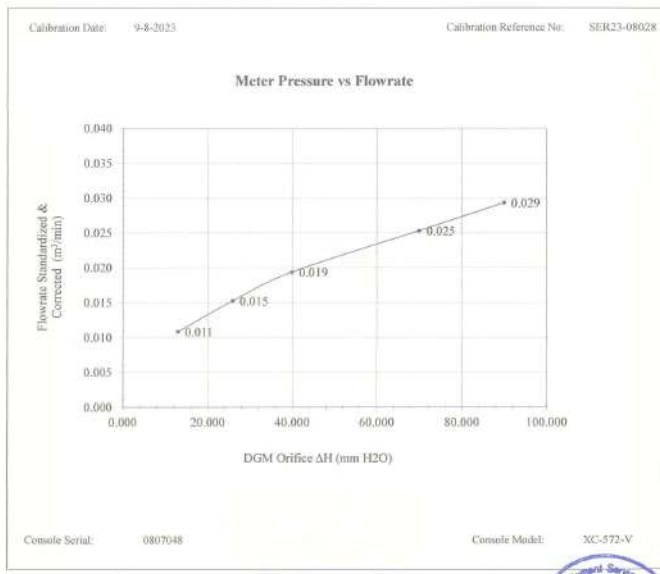

เอกสารไม่ควบคุม

THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information		Calibration Conditions			
Console Model Number	XC-572-V	Date	Time	09/08/2023	11:45 AM
Console Serial Number	0807048	Calibration Reference No.	SER23-08028		
DGM Model Number	SK25EX	Reference Thermometer	DIGICON		
DGM Serial Number	00003811	Serial Number	183169105		
Meter Box Model Number	JENCO 765 KF				
Meter Box Serial Number	JC 08944				

Results										
Console Thermocouple Simulator										
Channel and test point	Meter Box Channel Temperature Reading (°C)									
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0
Stack	-19.0	24.0	37.0	92.0	148.0	257.0	370.0	481.0	593.0	815.0
Aux	-19.0	23.0	37.0	92.0	147.0					
Probe	-19.0	23.0	37.0	92.0	148.0					
Filter	-19.0	23.0	37.0	92.0	147.0					
Exit	-18.0	23.0	37.0							

Tolerance Range			
Stack	± 1.50%	Absolute	Meter ± 3.0 °C
Probe	± 3.0 °C		Exit ± 2.0 °C
Filter	± 3.0 °C		



เอกสารไม่ควบคุม

Instrument description	Flue gas Analyzer
Instrument model	Testo 350 New
Instrument serial no.	60899615
ID no. or control no.	UAE.EPM. 006/2560
Manufacturer	Testo SE & Co. KGaA
Probe description	-
Probe model	-
Probe serial	-
Customer name	United Analyst and Engineering Consultant Co., Ltd.
Customer address	81 Soi Udomsuk 41, Sukhumvit Rd., Bangkok, Phrakhanong, Bangkok 10260

Total pages of certificate	3 Pages
Receiving no.	L-231754
Receiving date	20-Jun-23
Parameter of calibration	Gas Calibration(Oxygen 2.498,10.04,21.02 %vol, Carbon Monoxide 80.14,309.9,1003 ppm, Nitrogen Dioxide 30.34,80.96,202.2 ppm, Nitric Oxide 30.01,151.5,320.6 ppm, Sulphur Dioxide 50.04,100.8,601.1 ppm)
Condition of UUC	Used
Ambient condition	All of the Measurement were carried out the stabilized laboratory Temperature : 23 ±5 °C Humidity : 55 ± 15 %RH
Calibration place	17/121 Soi Ngomwongwan 47 Yeak 46, Toongsonghong, Laks, Bangkok 10210
Calibration procedure no.:	This instrument was calibrated by comparison with Standard gas mixture according to calibration work instruction no. WI-CL-26-C

The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.
This certificate is applied only to item under test Environmental condition.
This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory.
Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.
This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).
Date of calibration : 20-Jun-23.

Kwanchoi
Mr. Kwanchoi Khamdang
Calibration Technician

Wittan
Mrs. Nongluck Wongpettes
Technical Manager

เอกสารไม่ควบคุม

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O ₂) 2.498 % Vol	4219/21	Linde	30-Sep-25
Oxygen (O ₂) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen (O ₂) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide (CO) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide (CO) 309.9 ppm	2803/21	Linde	22-Jun-23
Carbon monoxide (CO) 1003 ppm	45513	Linde	09-Aug-24
Nitrogen Dioxide (NO ₂) 30.34 ppm	2703/22	Nimt	22-Aug-24
Nitrogen Dioxide (NO ₂) 80.96 ppm	3240/21	Linde	26-Jun-24
Nitrogen Dioxide (NO ₂) 202.2 ppm	3239/21	Linde	20-Jul-23
Nitric Oxide (NO) 30.01 ppm	CG-0014-23	Nimt	19-Feb-25
Nitric Oxide (NO) 151.5 ppm	0161/23	Linde	22-Jan-25
Nitric Oxide (NO) 320.6 ppm	2944/21	Linde	02-Jul-23
Sulphur Dioxide (SO ₂) 50.04 ppm	3205/21	Linde	25-Jul-23
Sulphur Dioxide (SO ₂) 100.8 ppm	3507/22	Linde	09-Nov-24
Sulphur Dioxide (SO ₂) 601.1 ppm	3204/21	Linde	20-Jul-23

Measured room conditions

Temperature : 22.7 °C Humidity : 67.8 %RH Pressure : 1005.1 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,200 ml/min Gas pressure : 1020.2 mbar

Calibration Results (before adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.498	2.56	0.062	0.15
O ₂ (%Vol)	10.04	10.11	0.07	0.20
O ₂ (%Vol)	21.02	21.10	0.08	0.30
CO (ppm)	80.14	78	-2.14	3.0
CO (ppm)	309.9	297	-12.9	6.0
CO (ppm)	1003	965	-38	12
NO ₂ (ppm)	30.34	27.9	-2.44	8.0
NO ₂ (ppm)	80.96	81.3	0.34	8.0
NO ₂ (ppm)	202.2	205.3	3.1	12
NO (ppm)	30.01	27	-3.01	8.0
NO (ppm)	151.5	143	-8.5	8.0
NO (ppm)	320.6	294	-26.6	12
SO ₂ (ppm)	50.04	53	2.96	6.0
SO ₂ (ppm)	100.8	111	10.2	6.0
SO ₂ (ppm)	601.1	665	63.9	13

FM-CL-09-C Rev.8

Page 2 of 3

Issued Date 26/02/16

Entech Industrial Solution Co., Ltd.

17/121 Soi Ngamwongwan 47, Yaek 48, Toongsonghong, Lakso, Bangkok 10210 THAILAND Tel: 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105530035591 www.entech.co.th

เอกสารไม่ควบคุม

Calibration Results (after adjustment) (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O ₂ (%Vol)	2.498	2.56	0.062	0.15
O ₂ (%Vol)	10.04	10.11	0.07	0.20
O ₂ (%Vol)	21.02	21.10	0.08	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	309.9	309	-0.9	6.0
CO (ppm)	1003	1001	-2	12
NO ₂ (ppm)	30.34	27.9	-2.44	8.0
NO ₂ (ppm)	80.96	81.3	0.34	8.0
NO ₂ (ppm)	202.2	205.3	3.1	12
NO (ppm)	30.01	32	1.99	8.0
NO (ppm)	151.5	155	3.5	8.0
NO (ppm)	320.6	318	-2.6	12
SO ₂ (ppm)	50.04	50	-0.04	6.0
SO ₂ (ppm)	100.8	100	-0.8	6.0
SO ₂ (ppm)	601.1	598	-3.1	13

Remark : 1 cmol/mol = 1 %vol, 1 μmol/mol = 1 ppm.

End of Report

FM-CL-09-C Rev.8

Page 3 of 3

Issued Date 26/02/16

Entech Industrial Solution Co., Ltd.

17/121 Soi Ngamwongwan 47, Yaek 48, Toongsonghong, Lakso, Bangkok 10210 THAILAND Tel: 0-2779-8888 Calibration@entech.co.th
Tax ID : 0105530035591 www.entech.co.th

เอกสารไม่ควบคุม



an Air Liquide company

Airgas Specialty Gases
Airgas USA, LLC
600 Union Landing Road
Cranston, NJ 08907-0000
Airgas.com

CERTIFICATE OF ANALYSIS
Grade of Product: EPA Protocol

Part Number: E05N183E15A0004 Reference Number: 82-401427550-1
Cylinder Number: CC715540 Cylinder Volume: 154.0 CF
Laboratory: 124 - Rverson (SAP) - NJ Cylinder Pressure: 2015 PSIG
PGVP Number: B52019 Valve Outlet: 660
Gas Code: CO₂, CO, NO, NO₂, SO₂, BALN Certification Date: Feb 27, 2019
Expiration Date: Feb 27, 2027

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.
Do Not Use This Cylinder below 100 psig, i.e. 6.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	400.0 PPM	405.0 PPM	G1	+/- 0.7% NIST Traceable	02/19/2019, 02/27/2019
NITRIC OXIDE	400.0 PPM	405.0 PPM	G1	+/- 0.7% NIST Traceable	02/19/2019, 02/27/2019
CARBON MONOXIDE	800.0 PPM	794.4 PPM	G1	+/- 0.7% NIST Traceable	02/19/2019
SULFUR DIOXIDE	900.0 PPM	913.4 PPM	G1	+/- 0.7% NIST Traceable	02/19/2019, 02/27/2019
CARBON DIOXIDE	16.00 %	16.09 %	G1	+/- 0.8% NIST Traceable	02/19/2019
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	15010127	KAL00437	494.6 PPM NITRIC OXIDE/NITROGEN	+/- 0.6%	Sep 01, 2021
PRM	12367	APX0109237	6.82 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Jun 02, 2017
GMS	1114201601	CC506710	4.971 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Nov 14, 2019
NTRM	14060148	CC436850	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	May 18, 2019
NTRM	111010354	KAL004822	968.8 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.6%	May 30, 2023
NTRM	12061504	CC354684	19.87 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	Jan 11, 2024

The SRM, PRM or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801933 CO ₂	FTIR	Feb 07, 2019
Siemens Ultramat 6 J3-599 COLOW	NDIR	Feb 19, 2019
Nicolet 6700 AHR0801933 NO	FTIR	Feb 01, 2019
Nicolet 6700 AHR0801933 NO ₂	FTIR	Feb 01, 2019
Nicolet 6700 AHR0801933 SO ₂	FTIR	Feb 14, 2019

Triad Data Available Upon Request

NOTES:
Gross Weight: 28291.4 grams
Net Weight: 5516.6 grams
PO# 5219000697

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2008 and relate only to items identified on this certificate. All values are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



TESTING CERT No. 3082.05

Approved for Release

เอกสารไม่ควบคุม



an Air Liquide company

Airgas Specialty Gases
Airgas USA, LLC
6041 Station Road
Bldg 1
Plumsteadville, PA 18949
Airgas.com

CERTIFICATE OF ANALYSIS
Grade of Product: EPA Protocol

Part Number: E05N183E15A001C Reference Number: 160-401892912-1A
Cylinder Number: CC19340 Cylinder Volume: 153.9 CF
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2015 PSIG
PGVP Number: A12020 Valve Outlet: 660
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN Certification Date: Oct 14, 2020
Expiration Date: Oct 14, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.
Do Not Use This Cylinder below 100 psig, i.e. 6.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	200.0 PPM	200.8 PPM	G1	+/- 0.8% NIST Traceable	10/06/2020, 10/13/2020
NITRIC OXIDE	200.0 PPM	200.8 PPM	G1	+/- 0.8% NIST Traceable	10/06/2020, 10/13/2020
SULFUR DIOXIDE	200.0 PPM	206.3 PPM	G1	+/- 0.9% NIST Traceable	10/06/2020, 10/13/2020
CARBON MONOXIDE	400.0 PPM	389.0 PPM	G1	+/- 0.8% NIST Traceable	10/14/2020
CARBON DIOXIDE	16.00 %	16.29 %	G1	+/- 1.0% NIST Traceable	10/06/2020
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	03161237	KAL004403	243.4 PPM NITRIC OXIDE/NITROGEN	+/- 0.5%	May 28, 2026
PRM	12396	D685025	9.91 PPM AIR/NITROGEN DIOXIDE	2.0%	Feb 20, 2020
GMS	124206889	CC323707	4.028 PPM NITROGEN DIOXIDE/NITROGEN	2.1%	Aug 15, 2021
NTRM	15006080	CC450677	248.1 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.6%	Dec 17, 2020
NTRM	042012	ND48548	495.4 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Jul 03, 2024
NTRM	060118	K008735	23.04 % CARBON DIOXIDE/NITROGEN	+/- 0.1%	Jun 27, 2022

The SRM, PRM or RGM noted above is only in reference to the GMS used in the assay and not part of the analysis.

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
HORIBA VAS011 TS6V/UP NDIR CO ₂	NDIR	Oct 02, 2020
SIEMENS ULTRAMAT6 N1-C8-180	NDIR	Oct 06, 2020
Nicolet iS60 FTIR AUP2010245 NO	FTIR	Sep 14, 2020
Nicolet iS60 FTIR AUP2010245 NO ₂	FTIR	Sep 22, 2020
Nicolet iS60 FTIR AUP2010245 SO ₂	FTIR	Sep 16, 2020

Triad Data Available Upon Request

NOTES: Gross Weight: 28.1 Kg, Net Weight: 5.1 Kg, PO#5220003826.



Approved for Release

เอกสารไม่ควบคุม
Page 1 of 160-401892912-1A

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E05N191E15A003C Reference Number: 160-401892911-1
Cylinder Number: CC429175 Cylinder Volume: 148.7 CF
Laboratory: 124 - Plumsteadville - PA Cylinder Pressure: 2015 PSIG
PGVP Number: A12020 Valve Outlet: 660
Gas Code: CO₂, CO, NO, NO₂, SO₂, BALN Certification Date: Sep 18, 2020

Expiration Date: Sep 18, 2028

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 800R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	100.0 PPM	100.5 PPM	G1	+/- 0.5% NIST Traceable	09/09/2020, 09/18/2020
NITRIC OXIDE	100.0 PPM	100.5 PPM	G1	+/- 0.5% NIST Traceable	09/09/2020, 09/18/2020
SULFUR DIOXIDE	100.0 PPM	100.1 PPM	G1	+/- 0.7% NIST Traceable	09/09/2020, 09/18/2020
CARBON MONOXIDE	200.0 PPM	200.3 PPM	G1	+/- 0.3% NIST Traceable	09/10/2020
CARBON DIOXIDE	8.000 %	8.023 %	G1	+/- 0.7% NIST Traceable	09/09/2020
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	12600111	KAL004089	249.9 PPM NITRIC OXIDE/NITROGEN	+/- 0.4%	Nov 08, 2023
NTRM	15060111	KAL004089	250.1 PPM NO ₂ /NITROGEN	+/- 0.4%	Nov 08, 2023
NTRM	15060970	CC449760	248.1 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.6%	Dec 17, 2020
NTRM	15060620	CC450449	248.1 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.6%	Dec 17, 2020
NTRM	041812	KAL003160	246.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.2%	Oct 16, 2024
NTRM	13060703	CC411728	16.939 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	May 14, 2025

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
MKS FTIR - CO ₂ - 000928781	FTIR	Aug 13, 2020
SIEMENS ULTRAMAT6E N1-C8-180	NDIR	Sep 09, 2020
MKS FTIR - NO - 000928781	FTIR	Sep 17, 2020
MKS FTIR - NO _x - 000928781	FTIR	Sep 17, 2020
MKS FTIR - SO ₂ - 000928781	FTIR	Sep 03, 2020

Triad Data Available Upon Request

NOTES: Gross Weight: 27.1 Kg, Net Weight: 4.6 Kg, PO# 5220003826.



เอกสารไม่ควบคุม
Page 1 of 160-401892911-1

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E02N185E15A3432 Reference Number: 82-401312965-1
Cylinder Number: CC719418 Cylinder Volume: 145.7 CF
Laboratory: 124 - Riverton (SAP) - NJ Cylinder Pressure: 2015 PSIG
PGVP Number: B52018 Valve Outlet: 590
Gas Code: O₂, BALN Certification Date: Oct 15, 2018

Expiration Date: Oct 15, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 800R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a volume/volume basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
OXYGEN	15.00 %	15.07 %	G1	+/- 0.6% NIST Traceable	10/15/2018
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	09051420	CC273871	22.53 % OXYGEN/NITROGEN	+/- 0.4%	Mar 05, 2019

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Horiba MPA 510-C2-71VMJ041	Paramagnetic	Oct 05, 2018

Triad Data Available Upon Request

NOTES:
Gross Weight: 60.8 lbs.
Net Weight: 11.3 lbs.
PO#5218004553
This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol, Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2008 and relate only to items identified on this certificate. All values are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.



Page 1 of 82-401312965-1
เอกสารไม่ควบคุม

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E05N183E15A000C Reference Number: 82-401241460-1
Cylinder Number: CC457499 Cylinder Volume: 153.9 CF
Laboratory: 124 - Riverton (SAP) - NJ Cylinder Pressure: 2015 PSIG
PGVP Number: B52018 Valve Outlet: 660
Gas Code: CO, CO₂, NO, NO₂, SO₂, BALN Certification Date: Jul 13, 2026

Expiration Date: Jul 13, 2026

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 800R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	400.0 PPM	400.6 PPM	G1	+/- 0.7% NIST Traceable	07/06/2018, 07/13/2018
NITRIC OXIDE	400.0 PPM	400.6 PPM	G1	+/- 0.6% NIST Traceable	07/06/2018, 07/13/2018
SULFUR DIOXIDE	400.0 PPM	411.4 PPM	G1	+/- 0.9% NIST Traceable	07/06/2018, 07/13/2018
CARBON MONOXIDE	800.0 PPM	783.1 PPM	G1	+/- 0.9% NIST Traceable	07/06/2018
CARBON DIOXIDE	16.00 %	16.09 %	G1	+/- 0.7% NIST Traceable	07/06/2018
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	15060436	CC450908	499.8 PPM NITRIC OXIDE/NITROGEN	+/- 0.8%	May 04, 2021
PRM	12368	5004119	29.86 PPM NITROGEN DIOXIDE/AIR	+/- 1.5%	Jun 02, 2017
GMS	7042010104	CC503641	5.101 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.0%	Jun 01, 2020
NTRM	16060125	CC437415	515.2 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Nov 16, 2021
NTRM	14060142	CC436630	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.8%	Nov 16, 2018
NTRM	12061519	CC354776	19.87 % CARBON DIOXIDE/NITROGEN	+/- 0.6%	Jan 11, 2024

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801933 CO ₂	FTIR	Jun 21, 2018
Siemens Ultramat 6 J3-599 COLDW	NDIR	Jun 28, 2018
Nicolet 6700 AHR0801933 NO	FTIR	Jul 12, 2018
Nicolet 6700 AHR0801933 NO ₂	FTIR	Jul 12, 2018
Nicolet 6700 AHR0801933 SO ₂	FTIR	Jul 05, 2018

Triad Data Available Upon Request

NOTES: PO# 5218002858

Net weight: 12.1 lbs
Gross weight: 62.1 lbs

This calibration std. has been certified in accordance with the May 2012 EPA Traceability Protocol, Document EPA-600/R-12/531. All testing processes and measurements conform to the requirements of ISO/IEC 17025 and to Airgas ISO 9001:2008 and relate only to items identified on this certificate. All values are certified to be NIST Traceable with total uncertainty as detailed under Analytical Uncertainty. This document shall not be reproduced in full without written approval of the issuer.

TESTING CERT No. 3082.05

Page 1 of 82-401241460-1

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI BUNTHAKORN 11 TAMBON BANG KHAO,
AMPHOE BANG PHU SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 1060-2116-5500-1 FAX: 1060-2116-7140



Certificate of Calibration

Customer Name: UNITED ANALYST AND ENGINEERING
Certificate No: 23-ACT-110
Request No: Req-2023-1407
CONSULTANT CO., LTD.
Address: 81 Soi Udomsak 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Unit Under Calibration Details
Measurement item: Acoustic Calibrator Class: I
Manufacturer: SVANTEK Range: 94, 114 dB / 1000 Hz
Model: SV 35A Instrument Status: Used
Serial Number: 73246
ID: UAE.EFM.104/2561

Calibration Environment and Details
Temperature: (23 ± 2 °C)
Humidity: (50 ± 20 %RH)
Barometric Pressure: (1013 ± 0.9 hPa)
Received Date: 26 June 2023
Calibration Date: 27 June 2023
Location of Calibration: LAB 1 Acoustic
Calibration Procedure: In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	S8079	EEL	31 May 2024
THD Multimeter	2015	1047765	NIMT	31 January 2024

Traceability: This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By: Mr. Noppadon Luangart
Service Calibration Engineer
Approved By: Mr. Paet Mathavorn
Calibration Engineer Supervisor
Issue Date: 27 June 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Calibration Lab.
เอกสารไม่ควบคุม

Certificate No : 23-ACT-110

Request No : Req-2023-1407

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class I (± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	93.82	-0.18	-	-	0.13	0.25
114 dB / 1000 Hz	113.77	-0.23	-	-	0.13	0.25

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class I (± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class I (± %)
	Measured (%)	Error (%)	Measured (%)	Error (%)		
94 dB / 1000 Hz	0.09	-	-	-	0.40	2.5
114 dB / 1000 Hz	0.28	-	-	-	0.40	2.5

Note :

- Acceptance limit was IEC60942:2017 Class I

- The calibration results exclude the calibration pressure correction

- The calibration results exclude the microphone volume correction

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-705

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Srinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24053

Job No. : VC67AC0034

Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand),

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

T. Petchur

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Srinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN
associates



Cert. No. : ACL24053

Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No. : 00409050 / 189687 / 90495
ID No. : UAE.EFM.012/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 21 DECEMBER 2023
Calibration Date : 18-19 JANUARY 2024
Date of Issue : 22 JANUARY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Srinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24053

Job No. : VC67AC0034

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม

T. Petchur

Cert. No. : ACL24053
Job No. : VC67AC0034
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	16.6
Flat	22.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.5	0.5	0.5	± 1.5
1000	0.3	0.3	0.3	± 1.0
8000	0.1	0.2	0.2	±5.0

Cert. No. : ACL24053
Job No. : VC67AC0034
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

Cert. No. : ACL24053
Job No. : VC67AC0034
Pages : 6 of 8Cert. No. : ACL24053
Job No. : VC67AC0034
Pages : 7 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.1	0.1	± 1.1
134.0	134.1	0.1	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.1	0.1	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.1	0.1	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.0	0.0	± 1.1
26.0	26.1	0.1	± 1.1
25.0	25.1	0.1	± 1.1

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

Cert. No. : ACL24053
Job No. : VC67AC0034
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม
T. Petchur

Cert. No. : ACL23129
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 00409023 / 185669 / 90468
ID No.: UAE.EFM.011/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 18 APRIL 2023
Calibration Date : 24 -26 APRIL 2023
Date of Issue : 27 APRIL 2023

Calibrated by : Nuthakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

เอกสารไม่ควบคุม
T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL23129
Job No. : VC66AC0048
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม
T. Petchur

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23129
Job No. : VC66AC0048
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

เอกสารไม่ควบคุม
T. Petchur

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23129
Job No. : VC66AC0048
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	11.6
C - weight	17.6
Flat	23.4

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.9	1.0	1.0	±5.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

T. Petch.

Continuation of Calibration Certificate

Cert. No. : ACL23129
Job No. : VC66AC0048
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.0	0.0	± 1.1
28.0	28.0	0.0	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.0	0.0	± 1.1
25.0	25.1	0.1	± 1.1

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

T. Petch.

Continuation of Calibration Certificate

Cert. No. : ACL23129
Job No. : VC66AC0048
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

T. Petch.

Continuation of Calibration Certificate

Cert. No. : ACL23129
Job No. : VC66AC0048
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

T. Petch.

Continuation of Calibration Certificate

Cert. No. : ACL23129
Job No. : VC66AC0048
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL23148
Job No. : VC66AC0053
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anchoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL-BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL-BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL-BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

T. Petchur

451-451/1 Sirinthorn Rd, Bangumru, Bangplud Bangkok 10700 THAILAND.
Tel:0-2435-8800 Fax:0-2433-1679 e-mail:cal-center@sithiporn.com http://www.sithiporn.com



Cert. No. : ACL23148
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RJON
Model : NL-42/ Microphone UC-52 / Preamplifier NH-24
Serial No.: 01010782 / 194537 / 14660
ID No.: UAE.EFM.085/2565

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 05 MAY 2023
Calibration Date : 08 -09 MAY 2023
Date of Issue : 10 MAY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

Continuation of Calibration Certificate

Cert. No. : ACL23148
Job No. : VC66AC0053
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For ≥ 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL23148
Job No. : VC66AC0053
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
14.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	16.6
Flat	22.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.3	0.4	0.4	±5.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

S. R. L.

Continuation of Calibration Certificate

Cert. No. : ACL23148
Job No. : VC66AC0053
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	33.9	-0.1	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

S. R. L.

Continuation of Calibration Certificate

Cert. No. : ACL23148
Job No. : VC66AC0053
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

S. R. L.

Continuation of Calibration Certificate

Cert. No. : ACL23148
Job No. : VC66AC0053
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.6	-0.8	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

QF-TS12-04-04-020664

เอกสารไม่ควบคุม

S. R. L.

Continuation of Calibration Certificate

Cert. No. : ACL23148
Job No. : VC66AC0053
Pages : 8 of 8

451-451/1 Srinthorn Road, Bangbunru, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com

Cert. No. : ACL24057
Pages : 1 of 8

11. Overload Indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00558036 / 176346 / 47891
ID No.: UAE.EFM.035/2558

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 21 DECEMBER 2023
Calibration Date : 18-19 JANUARY 2024
Date of Issue : 22 JANUARY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

เอกสารไม่ควบคุม



SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Srinthorn Road, Bangbunru, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24057
Job No. : VC67AC0034
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KA1	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม



SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-451/1 Srinthorn Road, Bangbunru, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24057
Job No. : VC67AC0034
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม



Cert. No. : ACL24057
Job No. : VC67AC0034
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	13.4
C - weight	20.0
Flat	25.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.6	0.7	0.7	±5.0

เอกสารไม่ควบคุม
F. KelwCert. No. : ACL24057
Job No. : VC67AC0034
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.2	0.0	±2.0
125	-0.1	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

เอกสารไม่ควบคุม
F. KelwCert. No. : ACL24057
Job No. : VC67AC0034
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	132.9	-0.1	± 1.1
132.0	131.9	-0.1	± 1.1
131.0	130.9	-0.1	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	27.0	0.0	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

เอกสารไม่ควบคุม
F. KelwCert. No. : ACL24057
Job No. : VC67AC0034
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.6	-0.8	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

เอกสารไม่ควบคุม
F. Kelw

Cert. No. : ACL24057
Job No. : VC67AC0034
Pages : 8 of 8

Cert. No. : ACL24051
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24
Serial No.: 00408982 / 186172 / 00727
ID No.: UAE.EFM.009/2564

Condition As Found : GOOD

Customer : UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,
BANGCHAK SUB-DISTRICT,
PHRAKHANONG DISTRICT, BANGKOK 10260
THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 21 DECEMBER 2023
Calibration Date : 18-19 JANUARY 2024
Date of Issue : 22 JANUARY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by : 
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced
other than in full, except with the prior written approval of the head of Calibration Laboratory.

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

Cert. No. : ACL24051
Job No. : VC67AC0034
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference
Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KA1	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

เอกสารไม่ควบคุม

Cert. No. : ACL24051
Job No. : VC67AC0034
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

เอกสารไม่ควบคุม

Cert. No. : ACL24051
Job No. : VC67AC0034
Pages : 4 of 8**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise**2.1 Normal test**

Measured Value (dB)
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	12.6
C - weight	19.2
Flat	24.7

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.1	0.1	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	2.3	2.4	2.4	±5.0

เอกสารไม่ควบคุม
T. KelnCert. No. : ACL24051
Job No. : VC67AC0034
Pages : 5 of 8**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz**5.1 Frequency weightings at 1 kHz**

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2

เอกสารไม่ควบคุม
T. KelnCert. No. : ACL24051
Job No. : VC67AC0034
Pages : 6 of 8**7. Level linearity on the reference level range**

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1

เอกสารไม่ควบคุม
T. KelnCert. No. : ACL24051
Job No. : VC67AC0034
Pages : 7 of 8**8. Level linearity including the level range control**

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, Lepeak (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

เอกสารไม่ควบคุม
T. Keln

SITHIPORN ASSOCIATES CO., LTD.
CALIBRATION LABORATORY

451-45/1 Sirinthorn Road, Bangbunru, Bangkok, 10700 Thailand
Tel: +66 2433 8331 Email: calibration@sithiporn.com



Cert. No. : ACL24051
Job No. : VC67AC0034
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
719/100 13, SOI SUTINAKORN 11 TAMBON BANG KAE0,
AMPHOE BANG PHU, SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0669-2116-5560-1 FAX: 0669-2116-7140



Certificate of Calibration

Customer: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 81 Soi Udomsak 41, Sukhumvit Road, Bangkok, Prakong, Bangkok 10260
Certificate No : 23-NDM-268
Request No : Req-2023-1465

Unit Under Calibration Details

Measurement Item : Noise Dosimeter
Manufacturer : SVANTEK
Model : SV 104
Serial Number : 110833
ID : -
Resolution : 0.1 dB
Microphone Class : 2
Microphone Model : SV27
Microphone S/N : 103079
Preamplifier Model : -
Preamplifier S/N : -
Instrument Status : Used

Calibration Environment and Details

Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 5 July 2023
Calibrated Date : 27 October 2023
Calibration Procedure : In-house method CP-NDM-01 based on IEC 61252:2017
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Multifrequency Calibrator	Quest	Quest-cal	188272	25 July 2024	TSI
Standard Microphone	GRAS	40AN	188273	21 August 2024	GRAS
Sine Generator	Svantek	Svan401	131	9 October 2024	WK Electric
Timer	EXTECH	-	05-ACT	20 March 2024	TPA

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : Mr. Noppon Luangart
Calibration Officer

Approved By : Mr. Paet Mathavorn
Calibration Engineer Supervisor
Issue Date : 27 October 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
719/100 13, SOI SUTINAKORN 11 TAMBON BANG KAE0,
AMPHOE BANG PHU, SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0669-2116-5560-1 FAX: 0669-2116-7140



Certificate No : 23-NDM-268
Request No : Req-2023-1465

1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY (%)	Tolerances Limit (%)
	Ref (s)	UUC (s)	Ref (Pa ² h)	UUC (Pa ² h)	Error (%)		
FAST / A / 55-140							
Calibrator Setting							
1000 Hz 114 dB	120	120	3.18	3.13	-1.57	3.1	-21, +26

Note : Absolute sensitivity was established by the use of Sound Calibrator brand SVANTEK, Model SV 35A, SN. 58079

2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY (± dB)	Tolerances Limit (± dB)
	A (dB)	C (dB)		
FAST / 55-140				
STD Setting	(dB)	(dB)		
*63 Hz	0.2	0.0	0.40	2.0
125 Hz	-0.1	0.0	0.40	1.5
250 Hz	-0.2	-0.1	0.40	1.5
500 Hz	0.0	0.1	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.2	0.3	0.40	2.0
4000 Hz	2.5	2.5	0.40	3.0
8000 Hz	-3.0	-3.1	0.40	5.0

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
719/100 13, SOI SUTINAKORN 11 TAMBON BANG KAE0,
AMPHOE BANG PHU, SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 0669-2116-5560-1 FAX: 0669-2116-7140



Certificate No : 23-NDM-268
Request No : Req-2023-1465

3. Linearity of response to steady signals

a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting	FAST / A / High										
	Ref (dB)	55.0	80.0	90.0	100.0	110.0	114.0	120.0	130.0	140.0	
1000 Hz	Level A (dB)	54.7	80.5	90.2	100.1	110.0	114.0	120.0	130.0	140.0	
	Error (dB)	-0.3	0.5	0.2	0.1	0.0	0.0	0.0	0.0	0.0	
	Ref (dB)			88.9	98.9	108.9	112.9	118.9	128.9	138.9	
8000 Hz	Level A (dB)			88.9	98.9	108.9	112.9	118.9	128.9	138.9	
	Error (dB)			0.0	0.0	0.0	0.0	-0.1	-0.1	-0.2	
	Ref (dB)						87.8	93.8	103.8	113.8	
63 Hz	Level A (dB)						87.8	93.8	103.8	113.8	
	Error (dB)						0.0	0.0	0.0	0.0	
	Ref (dB)										
Tolerances Limit (±dB)		1.0									
UNCERTAINTY (±dB)		0.3									

b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa ² h)	(Pa ² h)	(%)	(%)	(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00	5.6	-21, +26
1000 Hz 110 dB	45	45	0.50	0.51	+2.00		
1000 Hz 110 dB	90	90	1.00	1.01	+1.00		
1000 Hz 110 dB	180	180	2.00	2.02	+1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63	5.6	
1000 Hz 120 dB	90	90	10.00	10.13	+1.30		
1000 Hz 120 dB	180	180	20.00	20.22	+1.10		
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-NDM-268
Request No : Req-2023-1465

4. Response to short duration

a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa ² h)	(Pa ² h)	(Pa ² h)	(Pa ² h)	(Pa ² h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 ~ +0.41

b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa ² h)	(Pa ² h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00		-21 ~ +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00	5.6	-29 ~ +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 ~ +41

5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement		UNCERTAINTY	Tolerances
FAST / A / 55-140	UUC	UUC	Different		Limit
Calibrator Setting	(s)	(Pa ² h)	(%)	(%)	(%)
Continuous Rectangle +	29	10.37	0.00	3.7	-21 ~ +26
Continuous Rectangle -		10.37			

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-NDM-108
Request No : Req-2023-0954

1. Absolute acoustical sensitivity

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa ² h)	(Pa ² h)	(%)	(%)	(%)
1000 Hz 114 dB	120	120	3.19	3.20	+0.31	3.1	-21 ~ +26

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 55A, SN: 58079

2. Frequency weightings

UUC Setting	Deviation from various Frequency Weighting		UNCERTAINTY	Tolerances
FAST / 55-140	A	C		Limit
STD Setting	(dB)	(dB)	(± dB)	(± dB)
*63 Hz	0.0	0.1	0.40	2.0
125 Hz	-0.4	0.1	0.40	1.5
250 Hz	-0.4	0.1	0.40	1.5
500 Hz	-0.2	0.2	0.40	1.5
1000 Hz	0.0	0.0	0.40	-
2000 Hz	0.2	0.6	0.40	2.0
4000 Hz	1.8	1.9	0.40	3.0
8000 Hz	-3.3	-3.4	0.40	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-NDM-108
Request No : Req-2023-0954

3. Linearity of response to steady signals

a. Sound exposure meter, linearity of response for changes of input sinusoidal signal level

UUC Setting	FAST / A / High									
1000 Hz	Ref	(dB)	55.0	80.0	90.0	100.0	110.0	114.0	120.0	140.0
Level A	(dB)	54.5	80.1	90.1	100.0	110.0	114.0	119.9	129.9	138.9
Error	(dB)	-0.5	0.1	0.1	0.0	0.0	0.0	-0.1	-0.1	-0.1
8000 Hz	Ref	(dB)		88.9	98.9	108.9	112.9	118.9	128.9	138.9
Level A	(dB)			88.9	98.9	108.9	112.9	118.9	128.8	138.6
Error	(dB)			0.0	0.0	0.0	0.0	0.0	-0.1	-0.1
63 Hz	Ref	(dB)						87.8	93.8	103.8
Level A	(dB)							87.8	93.8	103.8
Error	(dB)							0.0	0.0	0.0
Tolerances Limit	(±dB)							1.0		
UNCERTAINTY	(±dB)							0.3		

b. Sound exposure meter linearity of error

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error		Limit
Calibrator Setting	(s)	(s)	(Pa ² h)	(Pa ² h)	(%)	(%)	(%)
1000 Hz 110 dB	27	27	0.30	0.30	0.00		
1000 Hz 110 dB	45	45	0.50	0.50	0.00		
1000 Hz 110 dB	90	90	1.00	0.99	-1.00	5.6	
1000 Hz 110 dB	180	180	2.00	1.98	-1.00		
1000 Hz 120 dB	36	36	4.00	4.03	+0.75		
1000 Hz 120 dB	72	72	8.00	8.05	+0.63		
1000 Hz 120 dB	90	90	10.00	10.13	+1.30		
1000 Hz 120 dB	180	180	20.00	20.22	+1.10	5.6	
1000 Hz 120 dB	360	360	40.00	40.34	+0.85		
1000 Hz 120 dB	720	720	80.00	80.49	+0.61		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-NDM-108
Request No : Req-2023-0954

4. Response to short duration

a. Response for sinusoidal signals - reference level

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error	(Pa ² h)	Limit
Calibrator Setting	(s)	(s)	(Pa ² h)	(Pa ² h)	(Pa ² h)	(Pa ² h)	(Pa ² h)
4000 Hz 95 dB	2846	2846	1.00	1.00	0.00	0.052	-0.29 ~ +0.41

b. Sound exposure meter response for series of toneburst impulses

UUC Setting	Time		Exposure Measurement			UNCERTAINTY	Tolerances
FAST / A / 55-140	Ref	UUC	Ref	UUC	Error	(%)	Limit
Calibrator Setting	(s)	(s)	(Pa ² h)	(Pa ² h)	(%)	(%)	(%)
Burst 1 ms, 95 dB	2846	2846	1.00	1.00	0.00	5.6	-21 ~ +26
Burst 1 ms, 100 dB	900	900	1.00	1.00	0.00		-29 ~ +41
Burst 1 ms, 108 dB	143	143	1.00	1.01	+1.00		-29 ~ +41

5. Response to unipolar pulse

UUC Setting	Time	Exposure Measurement	UNCERTAINTY	Tolerances
FAST / A / 55-140	UUC	UUC		Limit
Calibrator Setting	(s)	(Pa ² h)	Different (%)	(%)
Continuous Rectangle +	29	10.37	0.00	3.7
Continuous Rectangle -		10.37		

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Certificate No : 23-AFM-082

Request No : Req-2022-0619

Unit Under Calibration Details

Measurement Item : Primary Flow Calibrator
Manufacturer : TSI
Model : 4146

Serial Number : 41461214007

ID : UAE.EMAZ.093/2555

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 14 March 2023

Calibration Date : 23 March 2023

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	16 June 2023
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	15 June 2023

Traceability :

This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI)

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibration By :

Mr. Noppadon Luangrat
Service Calibration Engineer

Approved By :

Mr. Pacht Mathavorn
Calibration Engineer Supervisor

Issue Date : 23 March 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

Certificate No : 23-AFM-082
Request No : Req-2022-0619

Result of Calibration :

Flow Setting	STD Flow Reading	UUC Flow Reading	Correction Flow	Uncertainty
(LPM)	(LPM)	(LPM)	(LPM)	(LPM)
0.02	0.021	0.019	0.002	0.004
0.05	0.051	0.046	0.005	0.005
0.1	0.100	0.092	0.008	0.007
0.2	0.201	0.189	0.012	0.003
0.5	0.502	0.491	0.011	0.007
1.0	1.009	0.987	0.022	0.015
1.7	1.702	1.678	0.025	0.024
2.0	2.004	1.960	0.044	0.028
3.0	3.001	2.915	0.087	0.043
4.0	4.003	3.901	0.102	0.057
5.0	5.010	4.918	0.092	0.071

Note

STD : Standard

UUC : Unit Under Calibration

Calibration media : Air

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
334/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL: 0-2717-3000-24 FAX: 0-2719-9184



Certificate of Calibration

Certificate No. : 23P1857
Page : 1 of 2

Equipment : Aneroid Barometer

Manufacturer : Barigo

Model : -

Serial No. : -

ID No. : UAE/ANV/151/2550

Condition As-Received : Used Item

Received Date : 26 May 2023

Calibration Date : 02 June 2023

Reference : 2305-0919WSC

Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Atmospheric Pressure : 1007 mbar

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used : The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 8-1 : Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DP142	1422505046	MP-0094-23	03 May 2024

2. This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3. This result of calibration was made on requested at the point specified by customer.

4. This result of calibration instrument was in absolute pressure.

5. This instrument was used clean air as pressure media.

6. The certificate is valid only to the item calibrated on date and place of calibration.

7. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khanawee
Issue Date : 08 June 2023

Approved Signatory :

Attapol P.
[] Phalinee Prabpaipal
[] Sura Suwanasari
[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0316357



Cert.No.: 23P1857
Page: 2 of 2

Result of calibration: Without adjustment
Function: Absolute Pressure Measurement

Range: 960 hPa to 1030 hPa
Scale Interval: 1 hPa (The Fifth Estimate)

Increasing Pressure

Applied Pressure (hPa)	960.27	971.66	982.37	994.32	1001.76	1010.97	1020.99	1030.52
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	-0.27	-1.66	-2.37	-4.32	-1.76	-0.97	-0.99	-0.52

Decreasing Pressure

Applied Pressure (hPa)	1030.52	1021.07	1011.30	1001.83	992.38	982.43	971.77	960.50
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-0.52	-1.07	-1.30	-1.83	-2.38	-2.43	-1.77	-0.50

The uncertainty of measurement was ± 0.30 hPa

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-000-

Attest P.

เอกสารไม่ควบคุม
a 1165501



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
5344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 23H1101
Page: 1 of 2

Equipment: Digital Thermo-Hygrometer

Manufacturer: Digicon

Model: TH-02

Serial No.: 395034175

ID No.: UAE.EFM.184/2565

Condition As-Received: Used Item

Received Date: 18 May 2023

Calibration Date: 22 May 2023
to 24 May 2023

Reference: 2305-0641WSC

Ambient Temperature: $(25 \pm 3) ^\circ\text{C}$

Relative Humidity: $(50 \pm 20) \%$

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrahanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Chilled Mirror Hygrometer	Dew Master	44730	20563A	14 Jun 2023
2) Handheld Thermometer With Sensor	1521	ASA339	221251	12 Oct 2023

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

- National Institute of Standards and Technology (NIST), The United States of America
- National Institute of Metrology Thailand (NIMT)

Calibrated by: Knapop Onrat
Issue Date: 25 May 2023

Approved Signatory:

[✓] Chakrit Waowwanjua
[] Pornthippa Tameyakul
[] Viporn Tantiyawutti

เอกสารไม่ควบคุม
B 0314979



Cert. No.: 23H1101
Page: 2 of 2

Result of Calibration: Without Adjustment
Function: Humidity Measurement

Reference Temperature ($^\circ\text{C}$)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement ($\pm\%$ R.H.)
25.0	40.1	41	0.9	1.3
25.0	50.1	51	0.9	1.6
25.0	60.0	60	0.0	1.6
25.0	70.2	67	-3.2	1.6

Result of Calibration: Without Adjustment
Function: Temperature Measurement

Standard Temperature ($^\circ\text{C}$)	UUC* Reading ($^\circ\text{C}$)	Error ($^\circ\text{C}$)	Uncertainty of Measurement ($\pm\%$)
20.014	20.4	0.386	0.42
25.022	25.6	0.578	0.42
30.033	30.3	0.267	0.42
40.000	40.1	0.100	0.42

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-000-

Attest P.

เอกสารไม่ควบคุม
a 1162980

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7139 MOO 13, SOI SUTINAKORN II TAMBON BANG KAEU,
AMPHOE BANG PHAI SAMUT PRAKAN PROVINCE, 10540 THAILAND
TEL: 0660-2116-5869-1 FAX: 0660-2116-7140



Certificate of Calibration

Customer: UNITED ANALYST AND ENGINEERING
Name: CONSULTANT CO., LTD.
Address: 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrahanong, Bangkok 10260

Certificate No.: 24-TPM-044
Request No.: Req-2023-2685

Page: 1/2

Unit Under Calibration Details

Calibration Parameter: Temperature
Instrument Name: Thermal Environment Monitor
Manufacturer: 3M
Model: QT-32
Serial Number: TPS030008
Resolution: $0.1 ^\circ\text{C}$
ID Number: UAE.EFM.083/2561
Range Calibration: $30 ^\circ\text{C}$ to $60 ^\circ\text{C}$
Type of Sensor: RTD
Sensor Diameter (mm): 4.5
Calibration Position (mm): 67.5
Instrument Status: Used

Calibration Environment and Details

Temperature: $23 ^\circ\text{C} \pm 3 ^\circ\text{C}$
Humidity: $55 \% \text{RH} \pm 15 \% \text{RH}$
Received Date: 21 December 2023
Calibrated Date: 23 January 2024
Calibration Procedure: In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard: Digital Thermometer with Sensor, Manufacturer: GINGO-GINGO, Model: GT11/RTD160, SN: 08000057, ID: 92-TPM Which was calibrated on 27 February 2023, Calibration Certificate No.: QR23-0494

Traceability: This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSAC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By:

Mr. Noppidon Lumgan
Technical Manager

Issue Date:

23 January 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม
B 0314979

Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 23-TPM-044

Request No : Req-2023-2685

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty in °C
WET	20.032	20.1	-0.1	0.13
	25.033	25.1	-0.1	0.13
	30.034	30.1	-0.1	0.13
	35.036	35.1	-0.1	0.13
	40.038	40.1	-0.1	0.13
	45.042	45.1	-0.1	0.13
	50.050	50.1	-0.1	0.14
	60.046	60.1	-0.1	0.13
DRY	20.032	20.2	-0.2	0.13
	25.034	25.2	-0.2	0.13
	30.043	30.2	-0.2	0.14
	35.038	35.2	-0.2	0.13
	40.040	40.2	-0.2	0.13
	45.039	45.3	-0.3	0.13
	50.043	50.3	-0.3	0.13
	60.046	60.3	-0.3	0.13
GLOBE	20.032	20.2	-0.2	0.15
	25.033	25.2	-0.2	0.13
	30.034	30.2	-0.2	0.13
	35.036	35.2	-0.2	0.13
	40.039	40.2	-0.2	0.13
	45.040	45.1	-0.1	0.13
	50.043	50.2	-0.2	0.13
	60.045	60.2	-0.2	0.13

End of Certificate

Calibrated By :

Mr. Sittichok Jirapaksuksakul

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.

Certificate No : 23-TPM-335

Request No : Req-2023-1488

Page : 1/2

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Unit Under Calibration Details

Calibration Parameter : Temperature
Instrument Name : Thermal Environment Monitor
Manufacturer : TSI QUEST
Model : QT-34
Serial Number : TEX040010
Resolution : 0.1 °C
ID Number : -
Range Calibration : 20 °C to 60 °C
Type of Sensor : RTD
Sensor Diameter (mm) : 4.5
Calibration Position (mm) : 67.5
Instrument Status : New

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 12 July 2023
Calibrated Date : 14 July 2023
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/RTD100, SN: 08000057, ID: 02-TPM Which was calibrated on 27 February 2023, Calibration Certificate No. : QR23-0494

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By :

Mr. Noppadon Luangart

Technical Manager

Issue Date :

14 July 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Calibration Note

UUC Adjustment : Not Adjust

Certificate No : 23-TPM-335

Request No : Req-2023-1488

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty in °C
WET	20.024	20.1	-0.1	0.13
	25.028	25.0	0.0	0.13
	30.026	30.0	0.0	0.13
	35.026	35.0	0.0	0.13
	40.029	40.0	0.0	0.13
	45.027	45.0	0.0	0.13
	50.039	50.0	0.0	0.13
	60.042	60.0	0.0	0.13
DRY	20.024	20.0	0.0	0.13
	25.028	25.0	0.0	0.13
	30.027	30.0	0.0	0.13
	35.027	35.0	0.0	0.13
	40.033	40.0	0.0	0.13
	45.027	45.0	0.0	0.13
	50.038	50.0	0.0	0.13
	60.042	60.0	0.0	0.13
GLOBE	20.024	19.9	+0.1	0.13
	25.027	24.9	+0.1	0.13
	30.025	29.9	+0.1	0.13
	35.027	34.9	+0.1	0.13
	40.033	39.9	+0.1	0.13
	45.027	44.9	+0.1	0.13
	50.038	49.9	+0.1	0.13
	60.042	59.9	+0.1	0.13

End of Certificate

Calibrated By :

Mr. Sittichok Jirapaksuksakul

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.

Certificate No : 23-TPM-337

Request No : Req-2023-1488

Page : 1/2

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,
Bangkok 10260

Unit Under Calibration Details

Calibration Parameter : Temperature
Instrument Name : Thermal Environment Monitor
Manufacturer : TSI QUEST
Model : QT-34
Serial Number : TEX040012
Resolution : 0.1 °C
ID Number : -
Range Calibration : 20 °C to 60 °C
Type of Sensor : RTD
Sensor Diameter (mm) : 4.5
Calibration Position (mm) : 67.5
Instrument Status : New

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 15 %RH
Received Date : 12 July 2023
Calibrated Date : 14 July 2023
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/RTD100, SN: 08000057, ID: 02-TPM Which was calibrated on 27 February 2023, Calibration Certificate No. : QR23-0494

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By :

Mr. Noppadon Luangart

Technical Manager

Issue Date :

14 July 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Calibration Note

UUC Adjustment ☐ No Adjust

Certificate No : 23-TPM-502

Request No : Req-2023-2230

Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty in °C
WET	20.031	20.0	0.0	0.13
	25.033	25.0	0.0	0.13
	30.035	30.0	0.0	0.13
	35.036	35.0	0.0	0.13
	40.040	40.0	0.0	0.13
	45.040	45.0	0.0	0.13
	50.043	50.0	0.0	0.13
	60.047	60.0	0.0	0.13
DRY	20.033	20.1	- 0.1	0.13
	25.036	25.1	- 0.1	0.13
	30.037	30.1	- 0.1	0.13
	35.039	35.1	- 0.1	0.13
	40.039	40.1	- 0.1	0.13
	45.041	45.1	- 0.1	0.13
	50.043	50.1	- 0.1	0.13
	60.045	60.1	- 0.1	0.13
GLOBE	20.032	20.0	0.0	0.13
	25.033	25.0	0.0	0.13
	30.034	30.0	0.0	0.13
	35.035	35.0	0.0	0.13
	40.038	40.0	0.0	0.13
	45.040	45.0	0.0	0.13
	50.043	50.0	0.0	0.13
	60.046	60.0	0.0	0.13

End of Certificate

Calibrated By :


 Mr. Sittichok Jimpakdeesakul

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

รายงานผลการปฏิบัติตามมาตรการป้องกันและแก้ไขผลกระทบสิ่งแวดล้อม และมาตรการติดตามตรวจสอบผลกระทบสิ่งแวดล้อม

โครงการโรงไฟฟ้าเอกชน (ครั้งที่ 2) บริษัท โกลบอล เพาเวอร์ ซินเนอร์ยี จำกัด (มหาชน)

ครั้งที่ 1 ประจำปี พ.ศ. 2566 (มกราคม-มิถุนายน พ.ศ. 2567)

บัญชีรายการเครื่องมือหลักของห้องปฏิบัติการ สำหรับวิเคราะห์คุณภาพสิ่งแวดล้อม									
No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือหลักวิเคราะห์คุณภาพอากาศ									
1	Analytical Balance (Repeatability 0.1 mg)	ฝุ่นละอองรวม ฝุ่นละอองขนาดไม่เกิน 10 ไมครอน	Mettler-Toledo	AB204-S / 1128312528	Mettler-Toledo (Thailand) Ltd.	23MM331	7 Apr 23	5 Apr 24	-
2	Analytical Balance (Repeatability 0.1 mg)		Mettler-Toledo	AB204-S/FACT / B108115858	Mettler-Toledo (Thailand) Ltd.	23MM332	7 Apr 23	5 Apr 24	-
3	Ion Chromatography (IC)	กรดกำมะถัน โซเดียมไฮโปคลอไรท์	Dionex	AquionRFC / 220380031/220360045	Archemica Lab Co.Ltd.	Qualification Report Anion (ID#1047)	23 Apr 24	22 Apr 25	-
Laboratory Instrument/Equipments.(คุณภาพน้ำ)									
1	pH Meter	ความเป็นกรดและด่าง อุณหภูมิ	Mettler-Toledo	Seven Easy S20 / 1231155210	National Food Institute, Ministry of Industry, Thailand	2401718-001-01	11 Mar 24	10 Mar 25	น้ำดี น้ำดื่ม, น้ำได้ดื่ม
2	BOD Incubator	บีโอดี	Arco	UC4-1320 / (UAE.WAO.006/2553)	Technology Promotion Association (Thailand-Japan)	24๑7588	1 Apr 24	30 Mar 25	-
3	BOD Incubator		Arco	UC4-1320 / (UAE.WAO.015/2561)	Technology Promotion Association (Thailand-Japan)	24TM303	10 Feb 24	9 Feb 25	-
4	Analytical Balance (Repeatability 0.1 mg)	น้ำหนักและไขมัน	Mettler-Toledo	MS603S / B007010311	National Food Institute, Ministry of Industry, Thailand	2402284-001-01	2 Apr 24	1 Apr 25	-
5	UV-VIS Spectrophotometer	แอมโมเนีย	Agilent Technologies	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP24-018	7 May 24	6 May 25	-
6	UV-VIS Spectrophotometer		Hitachi	U-1900 / 2021-064	DQE Services Co.,Ltd.	SP24-008	16 Jan 24	15 Jan 25	-
7	UV-VIS Spectrophotometer		Hitachi	U-2900 / 21E22-009	DQE Services Co.,Ltd.	SP24-001	4 Jan 24	3 Jan 25	-
8	Analytical Balance (Readability 0.01 mg)	สารที่ละลายได้ทั้งหมด สารแขวนลอย	Mettler-Toledo	XSR205DU / C210685394	National Food Institute, Ministry of Industry, Thailand	2402283-002-01	2 Apr 24	1 Apr 25	-
9	Hot Air Oven		Memmert	UF55 / B216.1666	National Food Institute, Ministry of Industry, Thailand	2400141-001-01	11 Oct 24	10 Oct 25	-
10	Conductivity Meter	ค่าการนำไฟฟ้า	SI Analytics	Lab955 / 16300356	DKSH Technology Limited	C24240057	14 Mar 24	13 Mar 25	-

Due Date of Calibration* : กำหนดตามแผนการสอบเทียบประจำปี อย่างน้อยปีละ 1 ครั้ง



Cert.No.: 23MM331
Page.: 1 of 3

Certificate of Calibration

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : AB204-S
Serial No. : 1128312528
ID No. : UAE.AIR.019/2550
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Balance Room 2
Received order : 07 April 2023
Calibration Date : 07 April 2023
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Suwit Imjai
Approved by :
() Pornthippa Tameyakul
() Malee Butkruea
Issue Date : 10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-1
Procedure used :-

Cert.No.: 23MM331
Page: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

- | Instruments | Model | Serial No. | ID No. | Test report No. | Due date |
|-----------------------------|-------|------------|---------|-----------------|-------------|
| 1) Standard Weight Set (E2) | 15884 | 24053 | 70RC007 | MM-0010-22 | 20 Jan 2024 |
- This certificate is valid only to the item calibrated on date and place of calibration.
 - This result of calibration was made on requested at the point specified by customer.
 - This certificate is not certified for any commercial transaction.
 - This certification is traceable to the International System of Unit.
 - Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g **Resolution** 0.0001 g

Before Adjustment :	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
Applied Weight (g)	(g)	(g)	(± mg)	(k)
100	99.9999	+0.0001	0.19	2.03
200	200.0001	-0.0001	0.29	2.00

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

Applied Weight	Standard Deviation of Reading (g)
(g)	
100	0.00007
200	0.00007

เอกสารไม่ควบคุม




Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-1

Cert.No.: 23MM331
Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table



Maximum difference between off-center and central loading (g)

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)	
-0.0001	-0.0002	+0.0004	-0.0001	-0.0006	0.0005

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
Unload	0.0000	0.0000	0.15	2.13
0.1	0.0999	+0.0001	0.15	2.13
1	0.9999	+0.0001	0.15	2.13
5	4.9999	+0.0001	0.15	2.13
10	9.9999	+0.0001	0.15	2.11
20	20.0000	0.0000	0.15	2.11
50	50.0000	0.0000	0.16	2.06
70	69.9999	+0.0001	0.18	2.04
100	99.9999	+0.0001	0.19	2.03
150	150.0003	-0.0003	0.29	2.00
200	200.0005	-0.0005	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



Cert.No.: 23MM332
Page.: 1 of 3

Certificate of Calibration

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : AB204-S /FACT
Serial No. : B108115858
ID No. : UAE.AIR.016/2555
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Balance Room 2
Received order : 07 April 2023
Calibration Date : 07 April 2023
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Suwit Imjai
Approved by :
() Pornthippa Tameyakul
() Malee Butkruea
Issue Date : 10 April 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services

เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-2
Cert.No.: 23MM332
Page: 2 of 3

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0010-22	20 Jan 2024

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g **Resolution** 0.0001 g

Before Adjustment :

Applied Weight	Balance Reading	Correction	Measurement Uncertainty	Coverage Factor
(g)	(g)	(g)	(± mg)	(k)
100	100.0002	-0.0002	0.21	2.06
200	200.0003	-0.0003	0.29	2.00

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

Applied Weight	Standard Deviation of Reading (g)
(g)	
100	0.00009
200	0.00007

เอกสารไม่ควบคุม




Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2304-0015OC-2
Cert.No.: 23MM332
Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.

The weighing machine reading error obtained is given in the table



Maximum difference between off-center and central loading (g)

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)
+0.0001	-0.0003	+0.0003	+0.0006	+0.0002

0.0005

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
Unload	0.0000	0.0000	0.18	2.17
0.1	0.0999	+0.0001	0.18	2.17
1	0.9998	+0.0002	0.18	2.17
5	5.0000	0.0000	0.18	2.17
10	10.0000	0.0000	0.18	2.17
20	20.0000	0.0000	0.18	2.15
50	50.0001	-0.0001	0.19	2.11
70	70.0001	-0.0001	0.20	2.07
100	100.0002	-0.0002	0.21	2.06
150	150.0004	-0.0004	0.29	2.00
200	200.0005	-0.0005	0.29	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



Certificate of Calibration

AquionRFIC : Anion (ID#1047)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co.,Ltd.

AquionRFIC S/N : 220380031

AS-DV S/N : 220360045



United Analyst and Engineering Consultant Co.,Ltd.

Operator Signature : K. Channarong Khiao-Un Date : Apr 23, 2024

(Mr.Channarong Khiao-Un)

Test Engineer

เอกสารไม่ควบคุม

Qualification Report

PM Check list,CM_OQ and PQ

AquionRFIC : Anion (ID#1047)

Aquion : Cation (ID#1048)

For

United Analyst Engineering Consultand Co.,Ltd.

(Validate System 2024)

เอกสารไม่ควบคุม

PM Anion ID#1047

Preventive Maintenance Check List



Checklist ICS Preventive Maintenance

Dionex Ion Chromatography Preventive Maintenance Report

Customer Organization	Name/ Department
United Analyst and Engineering Consultant Co., Ltd.	Khun Suwan Kongthong / Lab
Engineer	Date
Mr.Channarong Khiao-Un	23-24/Apr/2024

Instrument Detail

Instrument Model	Application
AquionRFIC	Anion
Instrument components	Serial Number
AquionRFIC	220380031
AS-DV	220360045

Consumable Detail

Columns	Guard Columns	Suppressors	Concentrators	Etc.
AS18	AG18	ADRS-600	-	EGC III KOH
				CR-ATC

Remark: ตรวจพบการเปลี่ยน Column, Guard Column และ Suppressor เนื่องจาก peak shift และ tail

Perform By Archemica

K. Channarong Khiao-Un
Archemica
Date 23/Apr/2024

Khun Suwan Kongthong
Customer
Date 23/Apr/2024

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Checklist ICS Preventive Maintenance

General ICS Maintenance Checklist

No.	Description	Result			
Power on & Connection		Checked	Cleaned	Replaced	N.A.
1	Instrument power on	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
2	Instrument connection	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Injection Valve Rebuild		Checked	Cleaned	Replaced	N.A.
3	Rebuilt injection valve 6 port	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	- Rotor seal	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	- Stator face	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
(Optional) Auxiliary Valve Rebuild		Checked	Cleaned	Replaced	N.A.
6	Rebuilt auxiliary valve - port	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
7	- Rotor seal	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
8	- Stator face	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Check Valve Cartridge		Checked	Cleaned	Replaced	N.A.
9	Inlet check valve assembly	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Outlet check valve assembly	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Verified correct flow orientation	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Pump/Piston Rinse Seal, Piston Seal and Piston		Checked	Cleaned	Replaced	N.A.
12	Piston rinse seal in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Piston seal in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Piston in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Piston rinse seal in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Piston seal in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Piston in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Waste Valve and Priming Valve		Checked	Cleaned	Replaced	N.A.
18	Waste valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Priming valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cell Detector		Checked	Cleaned	Replaced	N.A.
20	Check conductivity cell	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Check electrochemical cell	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22	- Working electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23	- Reference electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24	- Gasket	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25	- Cell body	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Other		Checked	Cleaned	Replaced	N.A.
26	Sample Loop Size 25 uL	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	End-line filter	<input checked="" type="checkbox"/>	-	<input type="checkbox"/>	<input type="checkbox"/>
28	Leak sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29	Lubricate pump mechanic	<input type="checkbox"/>	Lubricated	-	<input type="checkbox"/>
30	Reconnected liquid lines to the valve	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
31	Reconnected liquid lines to pump heads	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
32	Primed pump	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
33	Checked pump for leaks	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
34	Checked gas for leaks	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>

เอกสารไม่ควบคุม



Checklist Sampler Preventive Maintenance

AS-DV Autosampler Preventive Maintenance Checklist

Model	Serial number	Firmware Version
<input checked="" type="checkbox"/> AS-DV	220360045	1.6.0

No.	Description	Result			
Power on & Connection		Checked	Cleaned	Replaced	N.A.
1.	AS-DV power on	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
2.	AS-DV connection	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Sampling Tip		Checked	Cleaned	Replaced	N.A.
3.	Sampling needle	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4.	Sampling tubing (Transfer line)	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5.	Reconnect sampling needle & tubing	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Other		Checked	Cleaned	Replaced	N.A.
6.	Check carousel movement	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
7.	Check needle movement	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
8.	Lubricate needle drive	<input type="checkbox"/>	Lubricated	-	<input type="checkbox"/>
9.	AS-DV cover	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
(Optional) High Pressure Valve		Checked	Cleaned	Replaced	N.A.
10.	High pressure valve - Port	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
11.	- Rotor seal	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
12.	- Stator face	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
13.	- Reconnected liquid line to the valve	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>

Others / comments

เอกสารไม่ควบคุม

PM Cation ID#1048

Preventive Maintenance Check List



Checklist ICS Preventive Maintenance

Dionex Ion Chromatography Preventive Maintenance Report

Customer Organization	Name/ Department
United Analyst and Engineering Consultant Co.,Ltd.	Khun.Suwan Kongthong / Lab
Engineer	Date
Mr.Channarong Khiao-Un	23-24/Apr/2024

Instrument Detail

Instrument Model	Application
Aquion	Cation
Instrument components	Serial Number
Aquion	220340349

Consumable Detail

Columns	Guard Columns	Suppressors	Concentrators	Etc.
CS12A	CG12A	CDER-600	-	-

Remark: ระบบไฟฟ้าและเครื่องใช้ภายในห้อง, System ยังไม่ผิดปกติ

Perform By Archemica

Archemica  23/Apr/2024
Date

 บริษัท อารเคมีกา แล็บ จำกัด
ARCHEMICA LAB CO.,LTD.
Customer  23/Apr/2024
Date

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Checklist ICS Preventive Maintenance

General ICS Maintenance Checklist

No.	Description	Result			
Power on & Connection		Checked	Cleaned	Replaced	N.A.
1	Instrument power on	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
2	Instrument connection	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Injection Valve Rebuild		Checked	Cleaned	Replaced	N.A.
3	Rebuilt injection valve s port	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	- Rotor seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	- Stator face	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
(Optional) Auxiliary Valve Rebuild		Checked	Cleaned	Replaced	N.A.
6	Rebuilt auxiliary valve - port	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
7	- Rotor seal	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
8	- Stator face	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Check Valve Cartridge		Checked	Cleaned	Replaced	N.A.
9	Inlet check valve assembly	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Outlet check valve assembly	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Verified correct flow orientation	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
Pump Piston Rinse Seal, Piston Seal and Plaston		Checked	Cleaned	Replaced	N.A.
12	Piston rinse seal in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Piston seal in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Piston in primary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Piston rinse seal in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Piston seal in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Piston in secondary pump head	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Waste Valve and Priming Valve		Checked	Cleaned	Replaced	N.A.
18	Waste valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Priming valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cell Detector		Checked	Cleaned	Replaced	N.A.
20	Check conductivity cell	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Check electrochemical cell	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22	- Working electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23	- Reference electrode	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24	- Gasket	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25	- Cell body	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Other		Checked	Cleaned	Replaced	N.A.
26	Sample Loop Size 25 uL	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	End-line filter	<input type="checkbox"/>	-	<input type="checkbox"/>	<input type="checkbox"/>
28	Leak sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29	Lubricate pump mechanic	<input type="checkbox"/>	Lubricated	-	<input type="checkbox"/>
30	Reconnected liquid lines to the valve	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
31	Reconnected liquid lines to pump heads	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
32	Primed pump	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
33	Checked pump for leaks	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>
34	Checked gas for leaks	<input checked="" type="checkbox"/>	-	-	<input type="checkbox"/>

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

CM OQ

Chromeleon Operation Qualification

ThermoFisher
SCIENTIFIC
Chromeleon Operational Qualification

General Information

Computer Name Version Number:
Instrument Controller: DESKTOP-C4FS3L7 7.3.1 Build 6535
Client: DESKTOP-C4FS3L7 7.3.1.6535
Operator: Mr.Channarong Khiao-Un

Overall Test Result: **Passed**

Comparison Format:

All Parameters:	Significant Digits:	10
-----------------	---------------------	----



K. Channarong 23/Apr/2024

Reviewer's Signature // Date

Operator's Signature // Date

เอกสารไม่ควบคุม

ThermoFisher
SCIENTIFIC
Chromeleon Operational Qualification, Part 1
Verification of Selected Results

Detection Algorithm: Cobra
Calibration Type: Lin, With Offset
Evaluation Type: Area
Standard Method: External
Calibration Mode: Total

Report Variable	Peak Name	Status
Offset (c0)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Slope (c1)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Correlation Coeffi.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Variance	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Std. Deviation	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Rel. Std. Dev.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Variance Coeff.	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

เอกสารไม่ควบคุม

ThermoFisher
SCIENTIFIC
Chromeleon Operational Qualification, Part 1
Verification of Selected Results

Report Variable	Peak Name	Status
Calibration Point X	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Calibration Point Y	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Amount [ng]	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Resolution (EP)	Acetanilide	ok
	Acetophenone	ok
Resolution (USP)	Acetanilide	ok
	Acetophenone	ok
Peak Asymmetry (EP/USP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Peak Asymmetry (AIA)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

เอกสารไม่ควบคุม

ThermoFisher
SCIENTIFIC
Chromeleon Operational Qualification, Part 1
Verification of Selected Results

Report Variable	Peak Name	Status
Theoretical Plates (EP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Theoretical Plates (USP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok
Theoretical Plates (JP)	Acetanilide	ok
	Acetophenone	ok
	Propiophenone	ok

Test Result: **Passed**

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Detection Algorithm: Cobra
Calibration Type: Lin, WithOffset
Evaluation Type: Area
Standard Method: External
Calibration Mode: Total

Variable Category	Report Variable	Peak Name	Status
Injection	No.		ok
	Name		ok
	Type		ok
	Position		ok
	Status		ok
	Volume		ok
	Dilution Factor		ok
	Weight		ok
	IntStd		ok
	InstrumentMethod		ok
	ProcessingMethod		ok
Chromatogram	Channel		ok
	No. of Peaks		ok
	Chromatogram Start Time		ok
	Signal Min.		ok
	Signal Max.		ok
	Unit		ok
	Noise		ok
Peak Results	No.	Acetanilide	ok
	No.	Acetophenone	ok
	No.	Propiophenone	ok
	Peak Name	Acetanilide	ok
	Peak Name	Acetophenone	ok
	Peak Name	Propiophenone	ok
	Ret.Time	Acetanilide	ok
	Ret.Time	Acetophenone	ok
	Ret.Time	Propiophenone	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Peak Width (50%)	Acetanilide	ok
	Peak Width (50%)	Acetophenone	ok
	Peak Width (50%)	Propiophenone	ok
	Left Width (0%)	Acetanilide	ok
	Left Width (0%)	Acetophenone	ok
	Left Width (0%)	Propiophenone	ok
	Right Width (0%)	Acetanilide	ok
	Right Width (0%)	Acetophenone	ok
	Right Width (0%)	Propiophenone	ok
	Peak Start	Acetanilide	ok
	Peak Start	Acetophenone	ok
	Peak Start	Propiophenone	ok
	Peak Stop	Acetanilide	ok
	Peak Stop	Acetophenone	ok
	Peak Stop	Propiophenone	ok
	Peak Start Value	Acetanilide	ok
	Peak Start Value	Acetophenone	ok
	Peak Start Value	Propiophenone	ok
	Peak Stop Value	Acetanilide	ok
	Peak Stop Value	Acetophenone	ok
	Peak Stop Value	Propiophenone	ok
	BL-Value Peak Start	Acetanilide	ok
	BL-Value Peak Start	Acetophenone	ok
	BL-Value Peak Start	Propiophenone	ok
	BL-Value Peak Stop	Acetanilide	ok
	BL-Value Peak Stop	Acetophenone	ok
	BL-Value Peak Stop	Propiophenone	ok
	Type	Acetanilide	ok
	Type	Acetophenone	ok
	Type	Propiophenone	ok
	Resolution (EP)	Acetanilide	ok
	Resolution(EP)	Acetophenone	ok
	Resolution(USP)	Acetanilide	ok
	Resolution(USP)	Acetophenone	ok
	Asymmetry(EP)	Acetanilide	ok
	Asymmetry(EP)	Acetophenone	ok
	Asymmetry(EP)	Propiophenone	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Abs.Ret.Dev.	Acetanilide	ok
	Ret.Dev.(abs)	Acetophenone	ok
	Ret.Dev.(abs)	Propiophenone	ok
	Rel.Ret.Dev.	Acetanilide	ok
	Ret.Dev.(rel)	Acetophenone	ok
	Ret.Dev.(rel)	Propiophenone	ok
	Area	Acetanilide	ok
	Area	Acetophenone	ok
	Area	Propiophenone	ok
	Ref.Area	Acetanilide	ok
	Ref.Area (Total)	Acetophenone	ok
	Ref.Area (Total)	Propiophenone	ok
	Height	Acetanilide	ok
	Height	Acetophenone	ok
	Height	Propiophenone	ok
	Rel.Height (Total)	Acetanilide	ok
	Rel.Height (Total)	Acetophenone	ok
	Rel.Height (Total)	Propiophenone	ok
	Amount	Acetanilide	ok
	Amount	Acetophenone	ok
	Amount	Propiophenone	ok
	Concentration	Acetanilide	ok
	Concentration	Acetophenone	ok
	Concentration	Propiophenone	ok
	Rel.Amount	Acetanilide	ok
	Rel.Amount	Acetophenone	ok
	Rel.Amount	Propiophenone	ok
	Peak Width (0%)	Acetanilide	ok
	Peak Width (0%)	Acetophenone	ok
	Peak Width (0%)	Propiophenone	ok
	Peak Width (5%)	Acetanilide	ok
	Peak Width (5%)	Acetophenone	ok
	Peak Width (5%)	Propiophenone	ok
	Peak Width (10%)	Acetanilide	ok
	Peak Width (10%)	Acetophenone	ok
	Peak Width (10%)	Propiophenone	ok

เอกสารไม่ควบคุม



Chromeleon Operational Qualification, Part 2

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Results	Asymmetry(AIA)	Acetanilide	ok
	Asymmetry(AIA)	Acetophenone	ok
	Asymmetry(AIA)	Propiophenone	ok
	Theor. Plates(EP)	Acetanilide	ok
	Theor. Plates(EP)	Acetophenone	ok
	Theor. Plates(EP)	Propiophenone	ok
	Theor. Plates(USP)	Acetanilide	ok
	Theor. Plates(USP)	Acetophenone	ok
	Theor. Plates(USP)	Propiophenone	ok
	Theor.Plates (JP)	Acetanilide	ok
	Theor. Plates(JP)	Acetophenone	ok
	Theor. Plates(JP)	Propiophenone	ok
Peak Calibration	Cal.Mode	Acetanilide	ok
	Cal.Mode	Acetophenone	ok
	Cal.Mode	Propiophenone	ok
	Cal.Type	Acetanilide	ok
	Cal.Type	Acetophenone	ok
	Cal.Type	Propiophenone	ok
	Weights	Acetanilide	ok
	Weights	Acetophenone	ok
	Weights	Propiophenone	ok
	Calibr. Coefficient C0	Acetanilide	ok
	Calibr. Coefficient C0	Acetophenone	ok
	Calibr. Coefficient C0	Propiophenone	ok
	Calibr. Coefficient C1	Acetanilide	ok
	Calibr. Coefficient C1	Acetophenone	ok
	Calibr. Coefficient C1	Propiophenone	ok
	RF-Value	Acetanilide	ok
	RF-Value	Acetophenone	ok
	RF-Value	Propiophenone	ok
	No. of Points	Acetanilide	ok
	No. of Points	Acetophenone	ok

เอกสารไม่ควบคุม

ThermoFisher
SCIENTIFIC**Chromeleon Operational Qualification, Part 2**

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Calibration	No. of Points	Propiophenone	ok
	No. of Points(disabled)	Acetanilide	ok
	No. of Points(disabled)	Acetophenone	ok
	No. of Points(disabled)	Propiophenone	ok
	Variance	Acetanilide	ok
	Variance	Acetophenone	ok
	Variance	Propiophenone	ok
	Var.Coeff	Acetanilide	ok
	Var.Coeff	Acetophenone	ok
	Var.Coeff	Propiophenone	ok
	Std.Dev.	Acetanilide	ok
	Std.Dev.	Acetophenone	ok
	Std.Dev.	Propiophenone	ok
	Rel.Std.Dev.	Acetanilide	ok
	Rel.Std.Dev.	Acetophenone	ok
	Rel.Std.Dev.	Propiophenone	ok
	Corr.Coeff.	Acetanilide	ok
	Corr.Coeff.	Acetophenone	ok
	Corr.Coeff.	Propiophenone	ok
	R-Square	Acetanilide	ok
	R-Square	Acetophenone	ok
	R-Square	Propiophenone	ok
	Adj. R-Square	Acetanilide	ok
	Adj. R-Square	Acetophenone	ok
	Adj. R-Square	Propiophenone	ok
	X	Acetanilide	ok
	X	Acetophenone	ok
	X	Propiophenone	ok
	Y	Acetanilide	ok
	Y	Acetophenone	ok
	Y	Propiophenone	ok
	W	Acetanilide	ok
	W	Acetophenone	ok
	W	Propiophenone	ok
	F(X)	Acetanilide	ok
	F(X)	Acetophenone	ok
	F(X)	Propiophenone	ok

เอกสารไม่ควบคุม

ThermoFisher
SCIENTIFIC**Chromeleon Operational Qualification, Part 2**

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Calibration	Residual for Cal.Point X	Acetanilide	ok
	Residual for Cal.Point X	Acetophenone	ok
	Residual for Cal.Point X	Propiophenone	ok
	Calibration Point Status	Acetanilide	ok
	Calibration Point Status	Acetophenone	ok
	Calibration Point Status	Propiophenone	ok
	Amount	Acetanilide	ok
	Amount	Acetophenone	ok
	Amount	Propiophenone	ok
Component	Cal.Type	Acetanilide	ok
	Peak Type	Acetanilide	ok
	Left Limit	Acetophenone	ok
	Right Limit	Acetanilide	ok
	Group	Acetanilide	ok
	Factor	Acetophenone	ok
	Amount	Acetanilide	ok
	Conc.Unit	Acetophenone	ok

เอกสารไม่ควบคุม

ThermoFisher
SCIENTIFIC**Chromeleon Operational Qualification, Part 2**

Most Frequently Used Parameters: Comparison with Expected Results

Variable Category	Report Variable	Peak Name	Status
Peak Purity	PPI	Acetanilide	ok
	PPI	Acetophenone	ok
	PPI	Propiophenone	ok
	RSD PPI	Acetanilide	ok
	RSD PPI	Acetophenone	ok
	RSD PPI	Propiophenone	ok
	Match	Acetanilide	ok
	Match	Acetophenone	ok
	Match	Propiophenone	ok
	RSD Match	Acetanilide	ok
	RSD Match	Acetophenone	ok
	RSD Match	Propiophenone	ok
	Rel.Max at	Acetanilide	ok
	Rel.Max at	Acetophenone	ok
	Rel.Max at	Propiophenone	ok

Test Result: Passed

เอกสารไม่ควบคุม

ThermoFisher
SCIENTIFIC**Chromeleon Operational Qualification, Part 3**

System Suitability Test: Comparison with Expected Results

Variable Category	Report Variable	Status
System Suitability Test Case	Number	ok
	Name	ok
	Inj.Condition	ok
	Eval. Formula	ok
	Operator	ok
	Statistics	ok
	Rounding	ok
	MinimumNumberOfInjections	ok
	MaximumNumberOfInjections	ok
	Channel	ok
	Peak	ok
	Ref. Value Formula 1	ok
	Ref. Value Formula 2	ok
	N.A.	ok
	Inj. Eval. Result	ok
	Eval. Result	ok
	Peak Result	ok
	Injection Condition Result	ok
	Ref. Value 1	ok
	Ref. Value 2	ok
	Result	ok
System Suitability Test Case Result	Message	ok
	Average	ok
	Count	ok
	Maximum	ok
	Minimum	ok
	Range	ok
	Rel. Range	ok
	Rel. Std. Dev.	ok
	Std. Dev.	ok
	Sum	ok

Test Result: Passed

เอกสารไม่ควบคุม

Chromeleon

Part 1 - Verification of Selected Results	PASS
Part 2 - Most Frequently Used Parameters: Comparison with Expected Results	PASS
Part 3 - System Suitability Test: comparison with Expected Results	PASS



OVERALL TEST RESULT: PASS

Field Service Representative Signature:	Customer Signature:
<i>K. Gammakorn</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

TEST EQUIPMENT AND STANDARDS

Test Equipment

Equipment	Manufacturer	Model	Serial Number	Cal/Ver Date	Good Until
Multimeter	Fluke	289	27970244	N/A	N/A
Thermocouple	Fluke	K-Type	27970244	N/A	N/A
Balance	Mettler Toledo	AB204-S	1129361010	N/A	N/A
IC Qualification	Thermo Scientific	Test Box	21379153	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A

Standards/Chemicals

Description	Manufacturer	Concentration	Part Number	Lot Number	Expiration Date
Nitrate	Thermo Scientific	5 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	10 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	25 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	50 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	100 ppm	060254	231226	Dec-2024
Nitrate	Thermo Scientific	1000 ppm	060254	231226	Dec-2024
N/A	N/A	N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A	N/A	N/A



Field Service Representative Signature:	Customer Signature:
<i>K. Gammakorn</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024


เอกสารไม่ควบคุม

PQ Anion ID#1047

Performance Qualification

เอกสารไม่ควบคุม

NOISE AND DRIFT (CD)

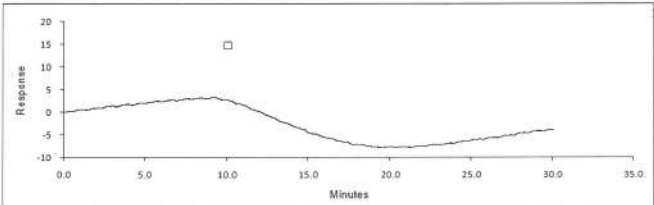

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	chrom://desktop-c4fs3i7/ChromeleonLocal/Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ.seq/278.smp/ICD_1.channel

Noise and Drift

Test	Measured (nS)	OQ Limit (nS)	Result	Conversion Factor
Noise	1.1 nS	≤ 2.0 nS	PASS	1000
Drift	16.1 nS/hr	≤ 20.0 nS/hr	PASS	1000



Field Service Representative Signature:	Customer Signature:
<i>K. Gammakorn</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	ChromeleonLocal://Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ

Peak Results

Sample Name	Injection Volume (µL)	Retention Time (min)	Area
Repeatability 01	25	0.265	2.825
Repeatability 02	25	0.265	2.822
Repeatability 03	25	0.265	2.831
Repeatability 04	25	0.265	2.835
Repeatability 05	25	0.265	2.834
Repeatability 06	25	0.265	2.836

Repeatability

Test	Measured (% RSD)	OQ Limit (% RSD)	Result
Retention Time	0.0	≤ 5.0	PASS
Area	0.2	≤ 1.0	PASS

OVERALL TEST RESULT: PASS

Field Service Representative Signature:	Customer Signature:
<i>K. Rattanaporn</i>	<i>Surin</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	ChromeleonLocal://Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ

Peak Results

Sample Name	Injection Volume (µL)	Retention Time (min)	Area
Reference Blank	25	0.265	0.053
High Standard	25	0.265	49.734
Carryover	25	0.265	0.051

Results


Test	Observed (%)	OQ Limit (%)	Result
AREA	0.00	≤ 0.10	PASS

OVERALL TEST RESULT: PASS

Field Service Representative Signature:	Customer Signature:
<i>K. Rattanaporn</i>	<i>Surin</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

DETECTOR LINEARITY (CD)

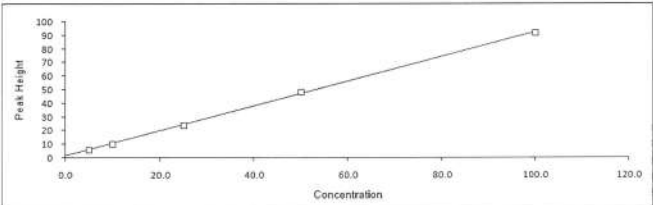

Information

System Name	Aquion RFIC
Detector SN	220360045
Data Path	ChromeleonLocal://Archemica/Service Contract/Validate 2024/1PM1PQ 23-04-24/Anion/IC OQ

Peak Results

Sample Name	Concentration	Peak Height	Calculated
Detector Linearity 01	5	5.872	4.82
Detector Linearity 02	10	10.299	9.68
Detector Linearity 03	25	23.794	24.52
Detector Linearity 04	50	48.473	51.65
Detector Linearity 05	100	91.855	99.34

Linearity

Test	Observed	OQ Limit	Result
r ²	0.999	≥ 0.999	PASS

OVERALL TEST RESULT: PASS

Field Service Representative Signature:	Customer Signature:
<i>K. Rattanaporn</i>	<i>Surin</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

ELUENT GENERATOR TEST

EG Current Test

Set Point (mM)	Expected (mA)	Reading (mA)	Deviation (mA)	OQ Limit (mA)	Result
1.00	1.6082	1.604	0.00	± 0.01	PASS
5.00	8.041	8.019	0.02	± 0.05	PASS
10.00	16.082	16.037	0.05	± 0.10	PASS
50.00	80.41	80.17	0.24	± 0.50	PASS
100.00	160.82	160.32	0.50	± 1.00	PASS

OVERALL TEST RESULT: PASS

Field Service Representative Signature:	Customer Signature:
<i>K. Rattanaporn</i>	<i>Surin</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

IC Pump Flow Rate

Set Point (mL) (mL/min)	Reading (mL/min)	Deviation (%)	OQ Limit (%)	Result
0.5	0.4995	0.100	± 2.0	PASS
1.0	0.999	0.10	± 2.0	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Khammarong</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

OQ EXCEPTIONS AND COMMENTS

N/A

Remainder of Page Intentionally Blank



Field Service Representative Signature:	Customer Signature:
<i>K. Khammarong</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

Column Compartment

Set Point (°C)	Reading (°C)	Deviation (°C)	OQ Limit (°C)	Result
30.0	30.5	0.5	± 2.0	PASS

OVERALL TEST RESULT: PASS



Field Service Representative Signature:	Customer Signature:
<i>K. Khammarong</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

OQ REVIEW AND COMPLETION

These Operational Qualification Results should be reviewed by the Customer. If the qualification is accepted, both the Customer and the Service Representative should sign the Operational Qualification Results, below.

OPERATIONAL QUALIFICATION RESULTS

Based upon the actual results obtained, this Operational Qualification **PASSED** the acceptance criteria described in the Operational Qualification in the Installation Checklist procedure.

Service Representative

A Field Service Representative signature below confirms the completion of all aspects of the Operational Qualification and have concluded that the system has been successfully verified to be operating as required.

Customer

A Customer signature below confirms the completion of all aspects of the Operational Qualification have been completed and that the system has been successfully verified to be operating as required.



Field Service Representative Signature:	Customer Signature:
<i>K. Khammarong</i>	<i>Simon</i>
Date: 23/Apr/2024	Date: 23/Apr/2024

เอกสารไม่ควบคุม

Calibration Certificate

Certificate No.: 2401718-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 5

Equipment: pH Meter
Manufacturer: METTLER TOLEDO
Model: SevenEasy pH
Serial No.: 1231155210
ID No.: UAE.WAT.010/2553
Order No.: 2401718
Operation No.: 2401718-001
Date of Receipt: 27 February 2024
Date of Calibration: 11 March 2024

Calibrated by Mr.Manas Somsak Specialist
Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 12 March 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full, except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2401718-001-01
Equipment: pH Meter
Resolution: 0.01 pH ; 1 mV
Manufacturer: METTLER TOLEDO
Model: SevenEasy pH
Serial No.: 1231155210
Type: Bench top
ID No.: UAE.WAT.010/2553
Date of Calibration: 11 March 2024
Location: Chemical Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature: (23.4 ± 1.5) °C Relative Humidity: (51 ± 3) %
Condition of Equipment: Good Condition
Condition of this Results of Calibration
1. Calibration Method: W-CC-002 : In house method based on direct measurement by using standard voltage calibrator and certified reference material (CRM)
2. Reference Standards / Certified Reference Material:
Instruments Serial / ID No. Manufacturer Certificate No. Due Date
2.1 DC Voltage Calibrator 2709007 Fluke 23E2003 14 June 2024
2.2 Digital Thermometer 2709007 Fluke CC 660570-01 30 October 2024
2.3 Thermo-Hygro Meter NPLBTH 014023 testo CC 660353-01 3 April 2024
Certified Reference Material Lot No. Manufacturer Ref N Expire Date
2.4 pH buffer 4.008 (Primary pH buffer Solution) 888842 CPAchem PH216.L5 13 April 2025
2.5 pH buffer 6.865 (Primary pH buffer Solution) 888843 CPAchem PH217.L5 13 April 2025
2.6 pH buffer 10.01 (Primary pH buffer Solution) 888844 CPAchem PH220.L5 13 April 2024
2.7 pH buffer 7.00 (Standard pH buffer Solution) C03109 HACH LANGE GmbH S11M064 18 October 2025
3. This certification is traceable to The International System of Units (SI Unit)
3.1 Instruments Ng.2.1 through NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments Ng.2.2 and 2.3 through NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Certified Reference Material Ng.2.4 to 2.6 traceable to Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.4 Certified Reference Material Ng.2.7 traceable to PTB Certificate Nr. PTB-PhDA-563/00504/23 and Certificate Nr. PTB-PhOB-565/06620/22 (PTB: Physikalisch-Technische Bundesanstalt, Braunschweig, Germany)
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2401718-001-01
Equipment: pH Meter
Resolution: 0.01 pH ; 1 mV
Manufacturer: METTLER TOLEDO
Model: SevenEasy pH
Serial No.: 1231155210
Type: Bench top
ID No.: UAE.WAT.010/2553
Date of Calibration: 11 March 2024
Page 3 of 5

1. Calibration of pH Meter (Manual Temperature Compensation at 25 °C)

Nominal pH	DC Voltage Standard (mV)	Average Indicator Reading		Uncertainty (±mV)	Coverage Factor (k)
		mV	pH		
0	414.121	414	0.00	0.58	2.00
2	295.814	296	2.00	0.58	2.00
4	177.464	178	4.00	0.58	2.00
6	59.160	59	6.00	0.58	2.00
7	0.001	0	7.00	0.58	2.00
8	-59.159	-59	8.00	0.58	2.00
10	-177.461	-177	10.00	0.58	2.00
12	-295.811	-296	12.00	0.58	2.00
14	-414.118	-414	14.00	0.58	2.00

2. Calibration of pH Meter with Electrode (Manual Temperature Compensation at 25 °C)

Equipment: pH Electrode Type: Combined Electrode
Manufacturer: METTLER TOLEDO Model: InLab Solids
Serial No.: 3065701 ID No.: N/A
Performance of Electrode system (Three-Point Calibration at pH 4, 7 and 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty (± pH)	Coverage Factor (k)
	pH	mV			
4.008	4.01	188	-	0.0071	2.00
7.001	7.00	13	98.9	0.0086	2.00
10.010	10.01	-160	97.2	0.0085	2.00
6.865	6.87	21	-	0.0074	2.00

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2401718-001-01
Equipment: Digital Thermometer with RTD (pH Meter)
Resolution: 0.1 °C Model: SevenEasy pH
Serial No.: 1231155210 ID No.: UAE.WAT.010/2553
Manufacturer: METTLER TOLEDO
Date of Calibration: 11 March 2024
Page 4 of 5

Location: Chemical Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature 23 °C ± 1 °C
Relative Humidity 51 % ± 2 %

Condition of this results of Calibration:

- Calibration Method :
 - In house method: W-TE-025 by comparison with standard thermometer.
 - The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
 - The temperature scale in use at this laboratory is the International Temperature scale of 1990 (ITS-90).
- Reference Standard Instrument

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1523	2118154	PSL-T 087/56	06-Jun-24	TISTR
Platinum Resistance Thermometer (PRT)	5627A	877332			

Support Equipment : Low Temperature Bath (ISOCAL-6), Model: Europa-6 Plus Basic, S/N: 341592/2

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good
Result of Calibration : ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65



กำหนดจุดห้ามใช้งาน

References Certificate Number. : 234TM588

Equipment : BOD Incubator

Model : UR-1320


Serial No. : -

ID No. : UAE.WAO.006/2553

Manufacturer : ARCO

Calibration Point : 20.0 °C

Unit Under Calibration Setting : 20.0 °C

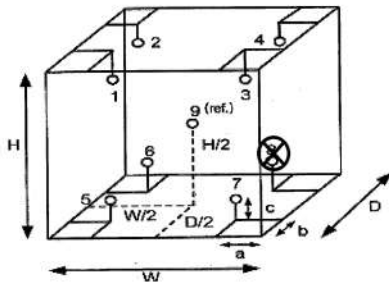

รูปภาพเครื่องมือ แสดงจุดที่ได้รับการสอบเทียบ และสัญลักษณ์ ⊗ แสดงจุดห้ามใช้งาน

กำหนดจุดห้ามใช้งานตำแหน่งที่.....8.....

หมายเหตุ เก็บใบแนบ.....

\\uae.net\appl\Lab-BOD\INSTRUMENT\B1-2563\Certificate\ป้ายห้ามใช้งานเครื่องมือ\ป้ายห้ามใช้งานเครื่องมือ 2567\กำหนดจุดห้ามใช้งาน.doc

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert. No.: 24TM303
Page : 1 of 3

Certificate of Calibration

Equipment : BOD Incubator
Manufacturer : Arco
Model : UC4-1320
Serial No. : 13URC4S013201
ID No. : UAE.WAO.015/2561
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 10 February 2024
Calibration Date : 10 February 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Tawatchai Pama

Approved by :
Approved Signatory

() Pornthippa Tameyakul
(x) Unnophol Harachai
() Suwit Imjai

Issue Date : 19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2402-0234OC-1
Result of Calibration : (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 24TM303
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.1	19.9	0.37	0.72	1.4	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.873	19.803	20.322	19.690	19.615	19.585	19.612	19.558	19.645	0.58

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2402-0234OC-1
Procedure Used :-

Cert. No.: 24TM303
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration


- Reference standard instrument-
Instrument Serial No. Cert. No. Traceable Due Date
1) Data Acquisition MY59003411 23LM208 TPA 27 Dec 2024
- This certificate is valid only to the item calibrated on date and place of calibration.
- This certificate is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	31
REL.Humid. (%)	70	65
AC Supply (Volt)	233	234

Position :	Ref. Std. ID No.:
1	20RTD-2/1
2	20RTD-2/2
3	20RTD-2/3
4	20RTD-2/4
5	20RTD-2/5
6	20RTD-2/6
7	20RTD-2/7
8	20RTD-2/8
9 (ref.)	20RTD-2/9

เอกสารไม่ควบคุม

Calibration Certificate

Certificate No.: 2402284-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS6035/01
Serial No.: B007010311
ID No.: UAE.TOX.008/2553
Order No.: 2402284
Operation No.: 2402284-001
Date of Receipt: 2 April 2024
Date of Calibration: 2 April 2024

Calibrated by Mr.Jerawut Prapawuttipong
Scientist
Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 9 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ๒๕๔๘ ถนนสุขุมวิท ๔๑ แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10700
2008 Soi 36, Aun Amai Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel :+66(0) 2-422 8668 Fax :+66(0) 2-422 8545



Calibration Report

Certificate No.: 2402284-001-01
Equipment: Electronic Balance
Model: MS6035/01
Serial No.: B007010311
Capacity: 620
Manufacturer: METTLER TOLEDO
Resolution: 0.001
ID No.: UAE.TOX.008/2553

Page 2 of 3

Date of Calibration: 2 April 2024
Environment Condition: Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 48 ± 2.5 %

Place of Calibration: Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NIT Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M23040535	8 April 2024
Standard Weight Class E2	500g	B505567696	TCS	M23040545	8 April 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NF1.BTH 017/23	Quality Reborn	QR24-0344	9 February 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
300	0.00000
600	0.00048

2. Off-Center Error:

A mass of 200 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	6 (g)	(Maximum Difference) (g)
200.000	199.997	199.999	199.999	199.998	200.000	0.003

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๔๘ ถนนสุขุมวิท ๔๑ แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10700
2008 Soi 36, Aun Amai Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel :+66(0) 2-422 8668 Fax :+66(0) 2-422 8545



Calibration Report

Certificate No.: 2402284-001-01
Equipment: Electronic Balance
Model: MS6035/01
Serial No.: B007010311
Capacity: 620
Manufacturer: METTLER TOLEDO
Resolution: 0.001
ID No.: UAE.TOX.008/2553

Date of Calibration: 2 April 2024

Page 3 of 3

Calibration Results: (Continued)

Calibration Range: 0 - 600 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:


Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor
Unload	0.0000	0.000	0.000	0.00082	2.00
0.1	0.1000	0.100	0.000	0.00082	2.00
0.5	0.5000	0.500	0.000	0.00082	2.00
1	1.0000	1.000	0.000	0.00082	2.00
2	2.0000	2.000	0.000	0.00082	2.00
5	5.0000	5.000	0.000	0.00082	2.00
10	10.0000	10.000	0.000	0.00082	2.00
20	20.0000	20.000	0.000	0.00082	2.00
50	50.0000	50.000	0.000	0.00082	2.00
100	100.0001	100.000	0.000	0.00083	2.00
150	150.0001	150.000	0.000	0.00084	2.00
200	200.0002	200.000	0.000	0.00086	2.00
300	300.0002	299.999	0.001	0.00090	2.00
400	400.0003	399.998	0.002	0.00100	2.00
500	500.0003	499.997	0.003	0.00111	2.00
600	600.0004	599.996	0.004	0.0012	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

***** End *****

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๔๘ ถนนสุขุมวิท ๔๑ แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10700
2008 Soi 36, Aun Amai Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10700, Thailand
Tel :+66(0) 2-422 8668 Fax :+66(0) 2-422 8545



Unit Value		Standard Value		Average Reading		Correction		Uncertainty (U)		Total Error		Judgement		Total Error < Judgement	
g		g		g		g		g		g		g		g	
30	0.0000	0.000	0.000	0.000	0.000	0.000	0.000	0.00082	0.001	0.001	0.001	Pass	Pass	Pass	Pass
60	0.1000	0.100	0.100	0.100	0.100	0.000	0.000	0.00082	0.001	0.001	0.001	Pass	Pass	Pass	Pass
90	0.5000	0.500	0.500	0.500	0.500	0.000	0.000	0.00082	0.001	0.001	0.001	Pass	Pass	Pass	Pass
120	1.0000	1.000	1.000	1.000	1.000	0.000	0.000	0.00082	0.001	0.001	0.001	Pass	Pass	Pass	Pass
150	2.0000	2.000	2.000	2.000	2.000	0.000	0.000	0.00082	0.001	0.001	0.001	Pass	Pass	Pass	Pass
180	5.0000	5.000	5.000	5.000	5.000	0.000	0.000	0.00082	0.001	0.001	0.001	Pass	Pass	Pass	Pass
210	10.0000	10.000	10.000	10.000	10.000	0.000	0.000	0.00082	0.001	0.001	0.001	Pass	Pass	Pass	Pass
240	20.0000	20.000	20.000	20.000	20.000	0.000	0.000	0.00082	0.001	0.001	0.001	Pass	Pass	Pass	Pass
270	50.0000	50.000	50.000	50.000	50.000	0.000	0.000	0.00082	0.001	0.001	0.001	Pass	Pass	Pass	Pass
300	100.0001	100.000	100.000	100.000	100.000	0.000	0.000	0.00083	0.001	0.001	0.001	Pass	Pass	Pass	Pass
330	150.0001	150.000	150.000	150.000	150.000	0.000	0.000	0.00084	0.001	0.001	0.001	Pass	Pass	Pass	Pass
360	200.0002	200.000	200.000	200.000	200.000	0.000	0.000	0.00086	0.001	0.001	0.001	Pass	Pass	Pass	Pass
390	300.0002	300.000	299.999	299.999	299.999	0.001	0.001	0.00090	0.001	0.001	0.001	Pass	Pass	Pass	Pass
420	400.0003	400.000	399.998	399.998	399.998	0.002	0.002	0.00100	0.001	0.001	0.001	Pass	Pass	Pass	Pass
450	500.0003	500.000	499.997	499.997	499.997	0.003	0.003	0.00111	0.001	0.001	0.001	Pass	Pass	Pass	Pass
480	600.0004	600.000	599.996	599.996	599.996	0.004	0.004	0.0012	0.001	0.001	0.001	Pass	Pass	Pass	Pass

Unit Under Calibration

เอกสารไม่ควบคุม



CERTIFICATE OF CALIBRATION

Certificate No. : SP24-018

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Agilent Technologies

Model : Cary 60

Serial No. : MY15410009


ID No. : UAE.WAT.020/2558

Received Date : 7 May 2024

Calibration Date : 7 May 2024

Issue Date : 9 May 2024

Condition Instrument : Good

Calibrated by : 
(Mr. Tanawut Rittidach)Approved by : 
(Ms. Chonthicha Sangnern)

Technical Manager

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม



REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °CRelative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 60 nm/min

Scan Interval of UUC : 0.15 nm.

Resolution of UUC : Photometric 0.0001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม



REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5747	0.0033	0.0031	2.00
	1.0484	1.0438	0.0046	0.0029	2.00
	2.1876	2.1832	0.0044	0.0080	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0231	0.0008	0.0035	2.00
	2.1230	2.1219	0.0011	0.0080	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5184	0.0046	0.0030	2.00
	0.9633	0.9614	0.0019	0.0029	2.00
	1.9753	1.9731	0.0022	0.0070	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5150	0.0031	0.0031	2.00
	1.0002	0.9964	0.0038	0.0033	2.00
	1.9973	1.9914	0.0059	0.0088	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5485	0.0032	0.0030	2.00
	1.0803	1.0772	0.0031	0.0030	2.00
	2.0373	2.0293	0.0080	0.0080	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5565	0.0026	0.0031	2.00
	1.0518	1.0482	0.0036	0.0030	2.00
	1.9274	1.9202	0.0072	0.0079	2.00

เอกสารไม่ควบคุม



REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7435	0.0034	0.0057	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8639	0.0035	0.0060	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2907	0.0012	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6402	0.0028	0.0055	2.00

เอกสารไม่ควบคุม

REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.9	-0.09	0.18	2.00
334.06	333.9	0.16	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.1	0.49	0.18	2.00
445.94	445.6	0.34	0.18	2.00
453.66	453.3	0.36	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.0	0.59	0.18	2.00
637.98	638.7	-0.72	0.18	2.00
431.38	430.8	0.58	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.7	-0.23	0.18	2.00
528.88	529.1	-0.22	0.18	2.00
573.17	573.5	-0.33	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.4	-0.68	0.20	2.00
748.55	749.1	-0.55	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.3	-0.02	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/1/2021

CERTIFICATE OF CALIBRATION

Certificate No. : SP24-008

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 315

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-1900

Serial No. : 2021-064

ID No. : UAE.WAS.006/2552

Received Date : 16 January 2024

Calibration Date : 16 January 2024

Issue Date : 19 January 2024

Condition Instrument : Good

Calibrated by :


(Mr.Tanawut Ritditch)

Technical Manager

Approved by :


(Ms. Chonthicha Sangern)

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards used to the units of measurement realized as the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/1/2021

REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °CRelative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 4.0 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/1/2021

REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
420	0.0000	0.000	0.0000	0.0028	2.00
	0.5780	0.575	0.0030	0.0031	2.00
	1.0484	1.046	0.0024	0.0029	2.00
	2.1876	2.186	0.0016	0.0080	2.00
440	0.0000	0.000	0.0000	0.0028	2.00
	0.5595	0.558	0.0015	0.0034	2.00
	1.0239	1.024	-0.0001	0.0035	2.00
	2.1230	2.121	0.0020	0.0079	2.00
465	0.0000	0.000	0.0000	0.0028	2.00
	0.5230	0.520	0.0030	0.0030	2.00
	0.9633	0.961	0.0023	0.0029	2.00
	1.9753	1.975	0.0003	0.0070	2.00
546.1	0.0000	0.000	0.0000	0.0028	2.00
	0.5181	0.516	0.0021	0.0031	2.00
	1.0002	0.999	0.0012	0.0033	2.00
	1.9973	1.994	0.0033	0.0084	2.00
590	0.0000	0.000	0.0000	0.0028	2.00
	0.5517	0.550	0.0017	0.0030	2.00
	1.0803	1.080	0.0003	0.0030	2.00
	2.0373	2.032	0.0053	0.0080	2.00
635	0.0000	0.000	0.0000	0.0028	2.00
	0.5591	0.558	0.0011	0.0031	2.00
	1.0518	1.051	0.0008	0.0030	2.00
	1.9274	1.923	0.0044	0.0079	2.00

เอกสารไม่ควบคุม

FM-708-02 R01 1/1/2021

REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 4 of 5

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor k
235	0.0000	0.000	0.0000	0.0050	2.00
	0.7469	0.748	-0.0011	0.0057	2.00
257	0.0000	0.000	0.0000	0.0050	2.00
	0.8674	0.865	0.0024	0.0059	2.00
313	0.0000	0.000	0.0000	0.0050	2.00
	0.2919	0.293	-0.0011	0.0051	2.00
350	0.0000	0.000	0.0000	0.0050	2.00
	0.6430	0.641	0.0020	0.0055	2.00

REPORT OF CALIBRATION

Certificate No. : SP24-008

Page 5 of 5

Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor k
241.54	241.1	0.44	0.18	2.00
279.40	278.9	0.50	0.18	2.00
288.70	288.0	0.70	0.18	2.00
334.22	333.8	0.42	0.18	2.00
361.26	360.8	0.46	0.18	2.00
418.48	418.2	0.28	0.18	2.00
446.70	446.0	0.70	0.18	2.00
453.20	453.1	0.10	0.18	2.00
460.06	459.6	0.46	0.18	2.00
536.90	536.4	0.50	0.18	2.00
637.94	637.6	0.34	0.18	2.00
440.74	440.1	0.64	0.18	2.00
472.22	472.0	0.22	0.18	2.00
513.70	513.5	0.20	0.18	2.00
528.72	528.2	0.52	0.18	2.00
574.60	574.3	0.30	0.18	2.00
585.48	585.0	0.48	0.20	2.00
684.63	684.2	0.43	0.18	2.00
740.27	740.0	0.27	0.20	2.00
748.28	747.8	0.48	0.18	2.00
807.16	806.8	0.36	0.18	2.00
879.70	879.2	0.50	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement U is stated as the standard uncertainty of measurement multiplied by the coverage factor k, which for a normal distribution corresponds to a coverage probability of approximately 95%

- * Indicates non TISI accredited

- End of Certificate -

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

CERTIFICATE OF CALIBRATION

Certificate No. : SP24-001

Page 1 of 5

Customer : United Analyst and Engineering Consultant Co.,Ltd. (Head Office)

Address : 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Location of calibration : Laboratory 213

Equipment : UV-Vis Spectrophotometer

Manufacturer : Hitachi

Model : U-2900

Serial No. : 21E22-009

ID No. : UAE.WAT.051/2564

Received Date : 4 January 2024

Calibration Date : 4 January 2024

Issue Date : 5 January 2024

Condition Instrument : Good

Calibrated by :


(Mr.Tanawut Rittidach)

Technical Manager

Approved by :


(Ms.Chonthicha Sangern)

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

REPORT OF CALIBRATION

Certificate No. : SP24-001

Page 2 of 5

Environment Condition : Ambient Temperature 25 ± 5 °CRelative humidity 55 ± 20 %RH

Calibration method : In-house method CP-01 Based on ASTM E275-08

Certified Reference Materials :

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

Traceability : This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Starna Scientific Limited

Spectral Band Width of UUC : 1.5 nm.

Scan Speed of UUC : 200 nm/min

Scan Interval of UUC : 0.1 nm.

Resolution of UUC : Photometric 0.001 Abs.

Wavelength 0.1 nm.

เอกสารไม่ควบคุม

FM-708-02 R01 1/11/2021

Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR2050U
Serial No.: C210683394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024 Page 2 of 4

Environment Condition: Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 47.5 ± 2.5 %

Place of Calibration: Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	8505567572	TCS	M23040535	8 April 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFLBTH 015/23	Quality Reborn	QB24-0343	9 February 2025

3. This certification is traceable to SI UNIT

4. This certification was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.000042
80	0.000052
100	0.000048
200	0.000048

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	6 (g)	(Maximum Difference) (g)
100.0000	100.0001	99.9999	99.9999	100.0001	100.0000	0.0001

F-CS-012 Revision: 01 Date: 20-04-65

2008 เอสอีเอ็มเอส 35 ถนนสุขุมวิท แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10110
2008 Soi 35, Aun Amarn Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10710, Thailand
Tel : +66(0) 2422 8668 Fax : +66(0) 2422 8545



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR2050U
Serial No.: C210683394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024 Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0 - 80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 80 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor
Unload	0.000000	0.00000	0.00000	0.0000086	2.00
0.001	0.001003	0.00101	-0.00001	0.0000089	2.00
0.005	0.005003	0.00500	0.00000	0.0000092	2.00
0.01	0.010003	0.01000	0.00000	0.0000089	2.00
0.05	0.049996	0.05000	0.00000	0.0000096	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50001	0.00001	0.000014	2.00
1	1.000003	1.00002	-0.00002	0.000016	2.00
2	2.000023	2.00001	0.00001	0.000017	2.00
5	5.000017	5.00002	0.00000	0.000020	2.00
10	10.000009	10.00000	0.00001	0.000026	2.00
20	20.000031	20.00000	0.00003	0.000037	2.00
30	30.000040	30.00001	0.00003	0.000050	2.00
50	50.000028	50.00002	0.00001	0.000068	2.00
80	80.000068	80.00002	0.00005	0.00011	2.00

F-CS-012 Revision: 01 Date: 20-04-65

2008 เอสอีเอ็มเอส 35 ถนนสุขุมวิท แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10110
2008 Soi 35, Aun Amarn Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10710, Thailand
Tel : +66(0) 2422 8668 Fax : +66(0) 2422 8545



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR2050U
Serial No.: C210683394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024 Page 4 of 4

Calibration Results: (Continued)

Calibration Range: 81 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 81 - 200 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor
90	90.00010	90.0001	0.0000	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00015	2.00
110	110.00007	110.0001	0.0000	0.00016	2.00
120	120.00009	120.0000	0.0001	0.00017	2.00
130	130.00010	130.0000	0.0001	0.00019	2.00
140	140.00014	140.0000	0.0001	0.00020	2.00
150	150.00009	150.0001	0.0000	0.00020	2.00
160	160.00010	160.0001	0.0000	0.00022	2.00
170	170.00012	170.0001	0.0000	0.00023	2.00
200	200.00016	200.0002	0.0000	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

F-CS-012 Revision: 01 Date: 20-04-65

2008 เอสอีเอ็มเอส 35 ถนนสุขุมวิท แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10110
2008 Soi 35, Aun Amarn Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10710, Thailand
Tel : +66(0) 2422 8668 Fax : +66(0) 2422 8545

Calibration Certificate

Certificate No.: 2400141-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road, Bangchack, Prakhonong, Bangkok 10260

Equipment: CHAMBER (Hot Air Oven)

Manufacturer: MEMMERT

Model: UF 55

Serial No.: B216.1666

ID No.: UAE.WAO.027/2559

Order No.: 2400141

Operation No.: 2400141-001

Date of Receipt: 11 October 2023

Date of Calibration: 11 October 2023

Calibrated by Mr.Worapob Sooktong
Scientist

Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 16 October 2023

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 เอสอีเอ็มเอส 35 ถนนสุขุมวิท แขวงคลองเตย เขตวัฒนา กรุงเทพมหานคร 10110
2008 Soi 35, Aun Amarn Road, Bang Yi Khan Subdistrict, Bang Phai District, Bangkok 10710, Thailand
Tel : +66(0) 2422 8668 Fax : +66(0) 2422 8545

Calibration Report

Certificate No.: 2400141-001-01
Equipment: CHAMBER (Hot Air Oven)
Model: UF 55 Serial No.: B216.1666
Resolution: 0.1 °C ID No.: UAE.WAO.027/2559
Manufacturer: MEMMERT
Date of Calibration: 11 October 2023 Page 2 of 3

Location: Laboratory, Floor 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Environment Condition: Ambient Temperature (28 ± 1) °C
Relative Humidity (63 ± 2) %
Line Voltage (228 ± 1) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E); Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016894	TE 660380-01	22 April 2024	NATIONAL FOOD INSTITUTE
	RTD	CHF201-209/ RTD#201-209			

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- Condition of Calibrated item : Good

UUC Description :

Time of Record 1 Hour 9 Minute At 104.0, 140.0 and 180.0 °C
Fresh air Damper ☒ Open Position ☐
☒ Close
☐ Not Available

- Result of Calibration : ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65



Certificate of Calibration

Equipment: CONDUCTIVITY METER Certificate No.: C24240057
Model: Lab 955 Issued Date: 11 March 2024
Serial No. (or ID.): 16300356 Job No.: WO-0020309
Manufacturer: SI Analytic Page: 1 of 2
Electrode Serial No. 16070067 Model : LF413T Brand : SI Analytic
Condition: In Condition

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udomsuk 41 Sukhumvit Road,
Bangkok, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature 23 °C ± 2 °C
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited.
2533 Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Mr. Pongpisut Suebchantha
Calibration Date: 11 March 2024
The Method used: In house method, CAL-WI-49, base on ASTM D 1125-14 and D 5391-14
Traceability: This certificate is traceable to the SI Units maintained by CRM of NIST(SRM) through CPA chem Co., Ltd. (ISO/IEC 17034) Certificate No. 960753, 890591, 890593

Mr. Pongpisut Suebchantha

Person in charge

Mr. Nitinun Srihawan

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

White Elephant เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ซอยสุขุมวิท 41 ถนนสุขุมวิท กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangkok, Prakanong, Bangkok 10260
Phone: +66 2638 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม

CAL-PM-C24-08: 12 Sep 2022

Calibration Report

Certificate No.: 2400141-001-01
Equipment: CHAMBER (Hot Air Oven)
Model: UF 55 Serial No.: B216.1666
Resolution: 0.1 °C ID No.: UAE.WAO.027/2559
Manufacturer: MEMMERT
Date of Calibration: 11 October 2023 Page 3 of 3

Calibration point: 104.0, 140.0 and 180.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	28.2	61.4	227.4
MAX	28.3	65.1	229.3




Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
104.0	104.05	103.98	104.02	104.08	104.00	104.05	103.99	104.17	104.00	0.53
140.0	140.09	139.99	139.91	140.05	139.99	139.91	139.97	140.26	139.97	0.73
180.0	180.46	180.33	180.25	180.28	180.33	179.96	180.31	180.64	180.16	0.90

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
104.0	104.0	104.0	104.0	0.090	0.18	0.38
140.0	140.0	140.1	140.0	0.075	0.28	0.47
180.0	180.0	180.1	180.0	0.13	0.48	0.88

Note: The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.


Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



Certificate No.: C24240057 Page: 2 of 2

Calibration Results:

Before Adjustment

Standard	Unit Under Calibration	Correction	Coverage Factor	Uncertainty (±)
Conductivity Solution	Reading		(k)	
25.000 μS/cm	26.7 μS/cm	-1.700 μS/cm	2.00	0.21 μS/cm
1413.0 μS/cm	1428 μS/cm	-15.0 μS/cm	2.00	9.0 μS/cm
111.3 mS/cm	108.4 mS/cm	2.9 mS/cm	2.00	0.67 mS/cm

After Adjustment ; at 1413 μS/cm

Standard	Unit Under Calibration	Correction	Coverage Factor	Uncertainty (±)
Conductivity Solution	Reading		(k)	
25.000 μS/cm	25.9 μS/cm	-0.900 μS/cm	2.00	0.21 μS/cm
1413.0 μS/cm	1413 μS/cm	0.0 μS/cm	2.00	9.0 μS/cm
111.3 mS/cm	107.5 mS/cm	3.8 mS/cm	2.00	0.67 mS/cm

The End of Certificate

White Elephant เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ซอยสุขุมวิท 41 ถนนสุขุมวิท กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangkok, Prakanong, Bangkok 10260
Phone: +66 2638 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม

CAL-PM-C24-08: 12 Sep 2022