

ภาคผนวก จ

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Water Lab	pH at 25 °C	pH meter	BKK_EN0342	27-Oct-23	27-Oct-24	12
Water Lab	Settleable Solids	Chamber (Cooling Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Sulfide	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Sulfide	Chamber (Cooling Room)	BKK_EN0167	6-Dec-23	6-Jun-25	18
Water Lab	Oil & Grease	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Oil & Grease	Water Bath	BKK_EN0148	4-Jul-23	4-Jan-25	18
Water Lab	Total Kjeldahl Nitrogen	Digestion Unit	BKK_EN0223	24-May-24	24-May-25	12
Water Lab	Total Kjeldahl Nitrogen	Discrete analyzer	BKK_EN0037	12-Jul-23	12-Jul-24	12
Water Lab	Total Suspended Solids	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Total Suspended Solids	Oven	BKK_EN0425	6-Nov-23	6-Nov-24	12
Water Lab	Total Dissolved Solids 103-105°C	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Total Dissolved Solids 103-105°C	Oven	BKK_EN0425	6-Nov-23	6-Nov-24	12
Water Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	BKK_EN0003	9-Aug-23	9-Aug-24	12
Water Lab	Total Dissolved Solids 180°C	Oven	BKK_EN0425	6-Nov-23	6-Nov-24	12
Water Lab	BOD	DO Meter	BKK_EN0017	16-Nov-23	16-May-25	18
Water Lab	BOD	Incubator	BKK_EN0304	20-Mar-24	20-Mar-25	12
Water Lab	BOD	Burette	BKK_EN0171	27-Feb-24	27-Aug-25	18
Water Lab	Total Coliform	Autoclave	BKK_ML0041	4-Oct-23	4-Apr-25	18
Water Lab	Total Coliform	Incubator	BKK_ML0010	17-Jul-23	17-Jan-25	18
Water Lab	Total Coliform	Hot Air Oven	BKK_ML0013	23-Apr-24	23-Oct-25	18



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH1369

Page.: 1 of 3

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Hach
Model :	HQ411d
Serial No. :	200100031163
ID No. :	BKK_EN0342
Condition As-Received:	Used Item
Received Date :	26 October 2023
Calibration Date :	27 October 2023
Reference :	2310-0865DSC-3
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

REVIEW BY	Siriluk B.
APPROVED BY	KL AL
NEXT CAL. DATE	27/10/24

Calibrated by : Warakorn Lernagtrakul

Approved by :

Saithip

Approved Signatory

- (✓) Saithip Meangmai
() Warakorn Lernagtrakul
() Ponpan Paipim

Issue Date : 31 October 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Cert.No.: 23CH1369

Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Ref. Standard Thermometer	4982054	110RC044	23I908	26 Jul 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	913598	14 July 2025
pH 6.985	CPA chem	913599	14 July 2024
pH 9.997	CPA chem	931961	30 Sep 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

<u>Unit Under Calibration</u>	<u>Standard pH Buffer Solution</u>	<u>Actual pH Reading</u>	<u>Actual mV Reading (mV)</u>	<u>Uncertainty of pH measurement (±)</u>	<u>Coverage factor k</u>
pH Electrode S/N.:230473042902	4.008	4.002	166.5	0.0044	2.00
	6.985	6.987	-10.4	0.0084	2.00
	9.997	10.005	-189.3	0.0071	2.00

Remark - Can not connect the BNC because the plug does not match with the socket.

Saithip



Cert.No.: 23CH1369

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : PHC281
- Serial No. : 230473042902

Dimension of probe;

- Length : 103 mm
- Diameter : 12 mm
- Immersion Depth : 90 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor <i>k</i>
25.0	25.002	25.1	0.098	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Saitip



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360
Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T232160

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cooling Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.


104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250



Customer Location : Laboratory

Date of Receipt : 29 November 2023

Calibrated By : Atiphong Rongrat (Technician)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 JAN 2024

REVIEW BY	<u></u>
APPROVED BY	<u></u>
NEXT CAL. DATE	<u>06/06/25</u>

The uncertainties are for a confidence probability of approximately 95%.


This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.



Certificate No. T232160

Page 3 of 4

Calibration Report

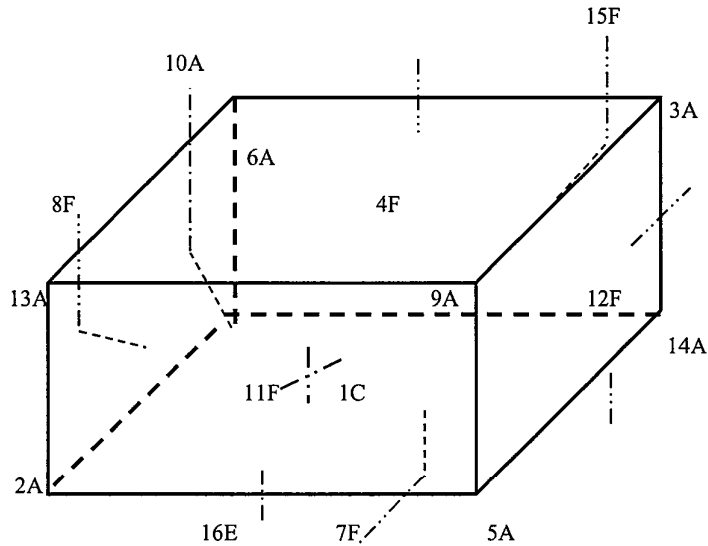

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C = TN161	12F = TN172
2A = TN162	13A = TN173
3A = TN163	14A = TN174
4F = TN164	15F = TN175
5A = TN165	16E = TN176
6A = TN166	
7F = TN167	
8F = TN168	
9A = TN169	
10A = TN170	
11F = TN171	

Approved By. 

Certificate No. T232160

Page 4 of 4

Calibration Report

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)											
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170	TN171	TN172
3.0	2.83	3.34	2.95	3.46	3.45	3.76	3.25	3.46	3.39	3.50	3.58	3.42
	TN173	TN174	TN175	TN176								
	3.33	3.39	3.15	3.43								

Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average					
3.0	2.8 , 4.1	3.5	3.36	1.10	2.00	1.90	2.09

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-27 FAX. 0-2719-9484



Cert.No.: 22CG3154

Page.: 1 of 2

Certificate of Calibration

Equipment :	Burette
Capacity :	50 mL
Serial No. :	-
ID. No. :	BKK_EN0171
Manufacturer :	Witeg
Made in :	Germany
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd. Khwaeng Phatthanakan, Khet Suan Luang Bangkok 10250 Thailand
Ambient Temperature :	(20 ± 2.5) °C
Relative Humidity :	(50 ± 10) %
Barometric Pressure :	759 mmHg
Calibration Procedure :	ASTM E 542 - 01
Calibrated by :	Panward Pramklam

REVIEW BY Sin'luk P.
APPROVED BY K L A L CWI
NEXT CAL. DATE	29/03/2024

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
() Malee Butkruea
(✓) Ponpan Paipim
() Srisuda Khamtha

Issue Date :

31 August 2022

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0044607



Equipment : Burette
Received Date : 26 August 2022
Condition As-Received : Used Item
Calibration Date : 30 August 2022
Reference : 2208-0918DSC-2

Cert.No.: 22CG3154

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	AE200S	N03679	140RC001	21MM429	NIMT	22 Sep 2022
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	22H1243	NIST,NIMT	09 June 2023
3) Thermometer	-	1594592	140EC010	22I181	NIMT	10 Feb 2023

This certification is traceable to SI Unit

- The certificate is valid only to the item calibrated on date and place of calibration.
- True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (\pm mL)	k Factor
50	49.9959	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

a 1123908



Certificate of Calibration

Cert.No.: 24CG952

Page.: 1 of 2

Equipment : Burette
Capacity : 50 mL
Serial No. : -
ID. No. : BKK_EN0171
Manufacturer : Witeg
Made in : Germany
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand
Ambient Temperature : (20 ± 2.5) °C
Relative Humidity : (50 ± 10) %
Barometric Pressure : 760 mmHg
Calibration Procedure : ASTM E 542 - 01
Calibrated by : Natcha Chayingcheiw

Approved by :

Approved Signatory

- () Unnophol Harachai
(✓) Srisuda Khamtha
() Sa-ngeunkam Wongsai

Issue Date :

27 February 2024

REVIEW BY *Siriluk P.*
APPROVED BY *Kank Anh.*
NEXT CAL DATE..... **27/08/25**

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Burette
Received Date : 23 February 2024
Condition As-Received : New Item
Calibration Date : 27 February 2024
Reference : 2402-0757DSC-1

Cert.No.: 24CG952

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

<u>Instruments</u>	<u>Model</u>	<u>Serial No.</u>	<u>ID. No.</u>	<u>Certificate No.</u>	<u>Traceability</u>	<u>Due date</u>
1) Balance	XP205DR	1126143764	140RC004	23MM538	TPA	15 Sep 2024
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	0834181	140EC005	23I948	TPA	10 Aug 2024

This certification is traceable to SI Unit

- The certificate is valid only to the item calibrated on date and place of calibration.
- True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (\pm mL)	k Factor
50	50.0032	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6 , e-mail: service.thailand@sartorius.com



NSC-TISI-TIS 17025

CALIBRATION 0426

SARTORIUS

Certificate

of Calibration

REVIEW BY	Simluk P.
APPROVED BY	KL AL
NEXT CAL. DATE	09/08/24

Model Number : MSE224S-100-DU

Description : Analytical Balance

Serial Number : 27405555

ID No.: BKK_EN0003

Manufacturer : Sartorius

Certificate No. : 23BC10310

Issued Date : Friday, August 11, 2023

Reference No. : 216011

Page No. : 1 Of 2

Customer Name : ALS Laboratory Group (Thailand)Co., Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok 10250.

Calibrated Place : Lab Room

Calibrated By : Mr.Chonchai Inthana

Calibration Date : Wednesday, August 09, 2023

Calibration

Procedure No. : This calibration was conducted by

Using in-house calibration procedure number (WI-003)

Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 220 g Readability : 0.0001 g

Ambients Conditions:

Temperature : 22.8 °C ± 5.0 °C

Humidity : 59.0 % RH ± 10.0 % RH

Pressure : ±

Reasons for calibration☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance**Equipment Condition:** ☒ Good Operate ☐ Fair**Measurement Method****UKAS Publication Ref :Lab 14**

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2, YCS011-522-00	SPC-RT	C02212565	14-Sep-2023
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19220444	5-Sep-2023

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

Mr.chonchai Inthana(Technical Manager)

S
T
A
M
P

Sartorius (Thailand) Co., Ltd.

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

SARTORIUS**Certificate****of Calibration**Model Number : MSE224S-100-DUCertificate No. : 23BCI0310Description : Analytical BalanceIssued Date : Friday, August 11, 2023Serial Number : 27405555Reference No. : 216011ID No. : BKK_EN0003Manufacturer : SartoriusPage No. : 2 of 2**Calibration Results : Without Adjustment****Repeatability**


The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.


Nominal Value : (Low Load)	20.0000	200.0000
20 g	20.0000	200.0000
Tolerance	20.0000	200.0000
0.0001 g	20.0000	200.0001
	20.0000	200.0001
Nominal Value : (High Load)	19.9999	200.0001
200 g	20.0000	200.0000
Tolerance	20.0000	200.0001
0.0001 g	20.0000	200.0001
	20.0000	200.0000
Standard Deviation	0.00003	0.00005

Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value :	100	g
Tolerance	0.0004	g





	Difference
1	—
2	0.0001
3	0.0000
4	0.0000
5	0.0001
6	-

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00014
0.1	0.1000	0.1000	0.0000	0.00014
1	1.0000	1.0000	0.0000	0.00014
2	2.0000	2.0000	0.0000	0.00014
5	5.0000	5.0000	0.0000	0.00014
10	10.0000	10.0000	0.0000	0.00014
20	20.0000	20.0000	0.0000	0.00014
50	50.0000	50.0001	0.0001	0.00015
100	100.0000	100.0000	0.0000	0.00019
200	200.0000	200.0001	0.0001	0.00030

End of Report.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T231303

Page 1 of 3

Certificate of Calibration

Equipment : Liquid Bath (Water)

Manufacturer : MEMMERT

Model : WNB29

Serial No. : L611.0135

Customer Code : BKK_EN0148

ID No. : T6455A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : ORGANIC PREPARATION LAB

Date of Receipt : 27 June 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By : Boonchai Suriyawong / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 11 JUL 2023

REVIEW BY	<u>Siriluk P.</u>
APPROVED BY	<u>KL AL</u>
NEXT CAL. DATE	<u>04/01/25</u>

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T231303

Page 2 of 3

Calibration Report

Equipment : Liquid Bath (Water)
Date of Calibration : 4 July 2023
Environment : Temperature : 22.2-22.5 °C
Line Voltage : 221.6-224.8 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert five resistance thermometer detectors into its water bath , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T36 (based on ASTM E715-80 (Reapproved 2001)).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 OHM	M18 (CH1,CH6-CH7,CH9-CH10)	T230545	10 April 2024
DATA LOGGER	34970A	T149	T230545	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 3 Hour 45 Minute At 60 °C

5. Adjustment :

(X) without adjustment

() after adjustment


Approved By. _____



Certificate No. T231303

Page 3 of 3

Calibration Report

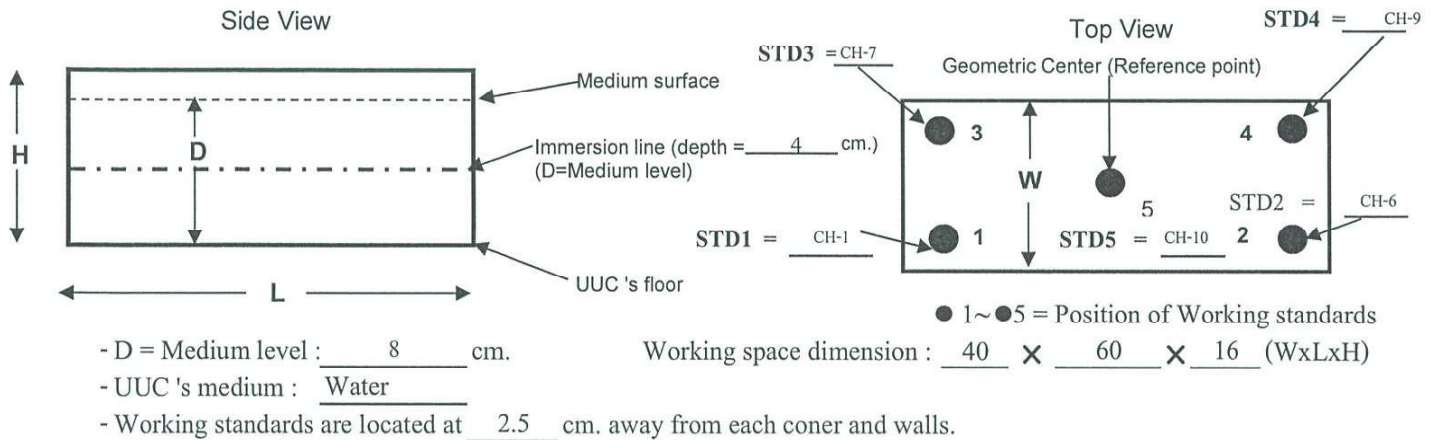

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)				
	CH-1	CH-6	CH-7	CH-9	CH-10
60	60.03	60.06	60.24	60.11	60.18
85	84.79	84.83	85.42	85.05	85.20
95	93.71	93.83	94.62	94.15	94.42


Liquid Bath (Water)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (±°C)	Uniformity (±°C)	Uncertainty (±°C)	Coverage Factor <i>k</i>
	Min , Max	Average					
61.0	60.9 , 61.1	61.0	60.12	0.13	0.19	0.29	2.04
86.0	85.8 , 86.2	86.0	85.06	0.19	0.47	0.44	2.17
95.0	94.6 , 95	94.9	94.15	0.32	0.65	0.55	2.13

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T232006

Page 1 of 5

Certificate of Calibration

Equipment : DIGESTION UNIT

Manufacturer : Environmental Express

Model : TKN100

Serial No. : 2017TKNBC142

Customer Code : BKK_EN0223

ID No. : T6773A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab1

Date of Receipt : 1 November 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 NOV 2023



The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T232006

Page 2 of 5

Calibration Report

Equipment : DIGESTION UNIT
Date of Calibration : 6 November 2023
Environment : Temperature : 28.7 - 30.0 °C
Line Voltage : 222.8 - 225.9 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A2-(CH11-CH14)	T230886	09 May 2024
DATA LOGGER	34970A	T47	T230886	09 May 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 47 Minute At 380 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment


() after adjustment

Approved By. Jun Kari

Certificate No. T232006

Page 3 of 5

Calibration Report

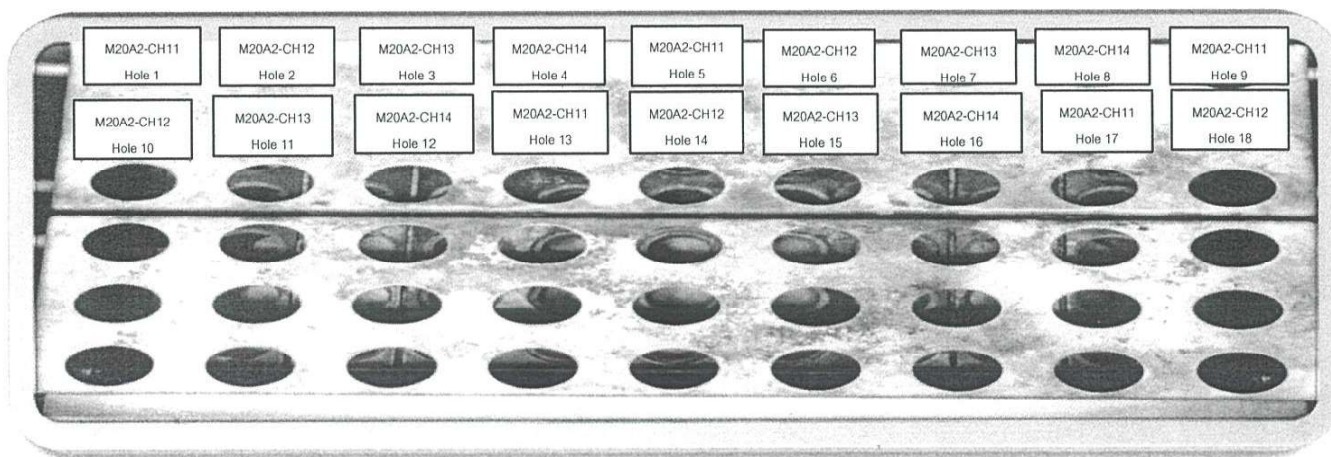

DISPLAY CONTROL (FRONT)

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block									
(°C)	(°C)	(°C)	Reading	M20A2-CH11 Hole 1	M20A2-CH12 Hole 2	M20A2-CH13 Hole 3	M20A2-CH14 Hole 4	M20A2-CH11 Hole 5	M20A2-CH12 Hole 6	M20A2-CH13 Hole 7	M20A2-CH14 Hole 8	M20A2-CH11 Hole 9	
380.0	380.0	379.8 - 380.2	Max °C	378.60	380.58	378.97	379.34	380.80	379.49	382.58	379.22	379.18	
			Min °C	378.12	380.09	378.57	379.02	380.56	379.18	382.30	378.97	378.88	
			Average °C	378.36	380.34	378.77	379.18	380.68	379.34	382.44	379.09	379.03	
			Stability ±°C	0.24	0.25	0.20	0.16	0.12	0.16	0.14	0.13	0.15	


Cal. Point	Setting	Reading	STD.	Position of Standards at Block									
(°C)	(°C)	(°C)	Reading	M20A2-CH12 Hole 10	M20A2-CH13 Hole 11	M20A2-CH14 Hole 12	M20A2-CH11 Hole 13	M20A2-CH12 Hole 14	M20A2-CH13 Hole 15	M20A2-CH14 Hole 16	M20A2-CH11 Hole 17	M20A2-CH13 Hole 18	
380.0	380.0	379.8 - 380.2	Max °C	378.04	382.06	382.55	379.39	377.99	380.37	380.15	379.85	377.74	
			Min °C	377.74	381.80	382.29	379.10	377.78	380.09	379.83	379.55	377.49	
			Average °C	377.89	381.93	382.42	379.25	377.88	380.23	379.99	379.70	377.62	
			Stability ±°C	0.15	0.13	0.13	0.14	0.10	0.14	0.16	0.15	0.13	

Approved By. 

Certificate No. T232006

Page 4 of 5

Calibration Report

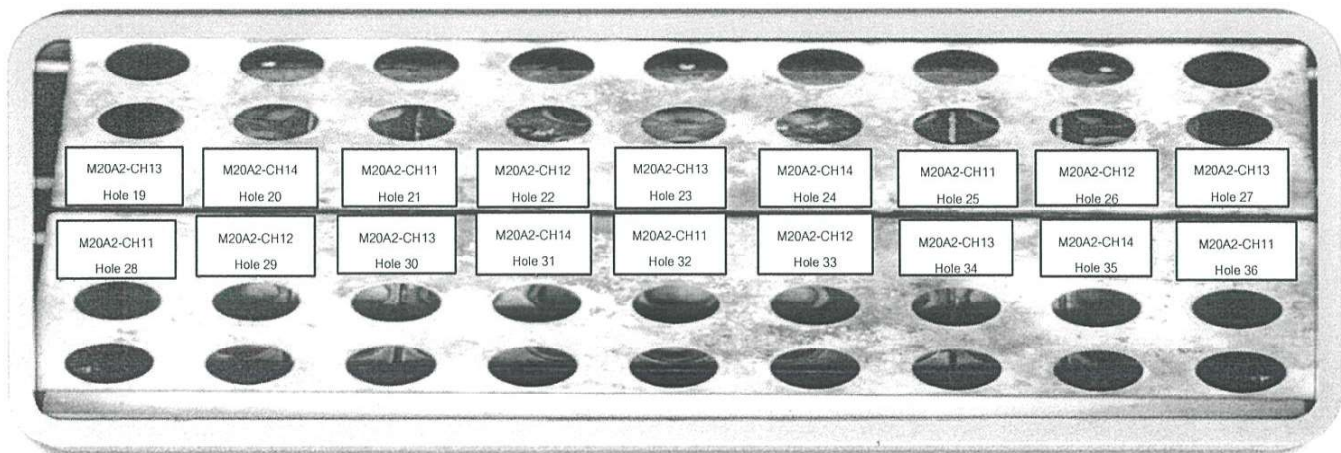

DISPLAY CONTROL (FRONT)

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	M20A2-CH13 Hole 19	M20A2-CH14 Hole 20	M20A2-CH11 Hole 21	M20A2-CH12 Hole 22	M20A2-CH13 Hole 23	M20A2-CH14 Hole 24	M20A2-CH11 Hole 25	M20A2-CH12 Hole 26	M20A2-CH13 Hole 27
380.0	380.0	379.8 - 380.2	Max °C	378.89	377.57	382.24	382.32	381.21	379.78	382.73	380.00	377.13
			Min °C	378.57	377.19	381.93	381.99	380.98	379.43	382.41	379.69	376.79
			Average °C	378.73	377.38	382.08	382.16	381.10	379.61	382.57	379.84	376.96
			Stability ±°C	0.16	0.19	0.15	0.16	0.12	0.18	0.16	0.16	0.17


Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	M20A2-CH11 Hole 28	M20A2-CH12 Hole 29	M20A2-CH13 Hole 30	M20A2-CH14 Hole 31	M20A2-CH11 Hole 32	M20A2-CH12 Hole 33	M20A2-CH13 Hole 34	M20A2-CH14 Hole 35	M20A2-CH11 Hole 36
380.0	380.0	379.8 - 380.2	Max °C	379.10	381.19	379.13	383.04	381.79	379.89	378.86	380.55	378.13
			Min °C	378.71	380.75	378.79	382.70	381.53	379.61	378.60	380.18	377.83
			Average °C	378.91	380.97	378.96	382.87	381.66	379.75	378.73	380.36	377.98
			Stability ± °C	0.19	0.22	0.17	0.17	0.13	0.14	0.13	0.19	0.15

Approved By. 

Certificate No. T232006

Page 5 of 5

Calibration Report

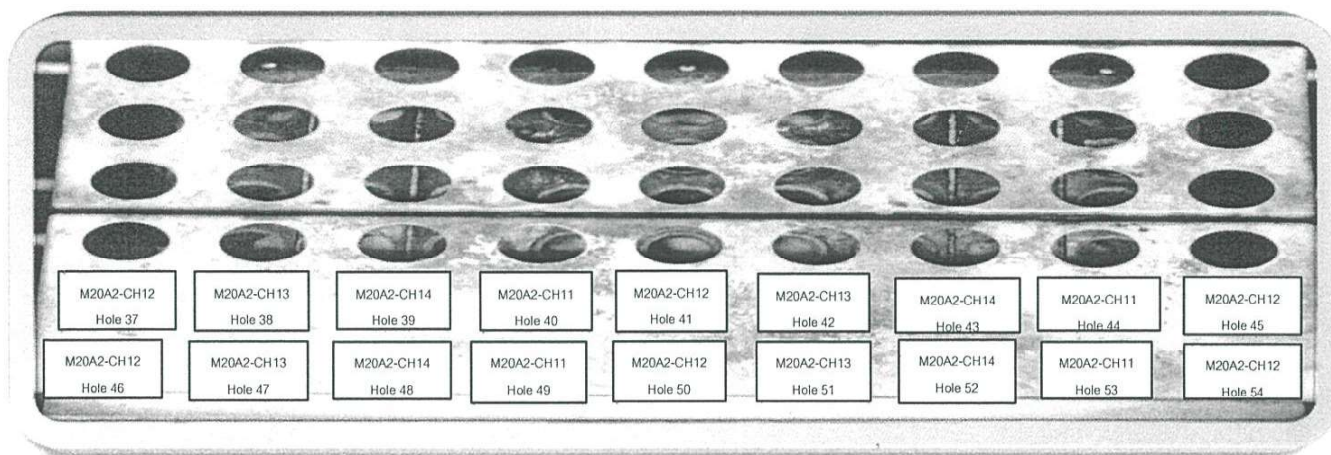

DISPLAY CONTROL (FRONT)

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block									
(°C)	(°C)	(°C)	Reading	M20A2-CH12 Hole 37	M20A2-CH13 Hole 38	M20A2-CH14 Hole 39	M20A2-CH11 Hole 40	M20A2-CH12 Hole 41	M20A2-CH13 Hole 42	M20A2-CH14 Hole 43	M20A2-CH11 Hole 44	M20A2-CH12 Hole 45	
380.0	380.0	379.8 - 380.2	Max °C	381.44	380.68	379.33	382.84	381.06	380.15	379.97	378.75	380.95	
			Min °C	381.04	380.35	379.01	382.49	380.79	379.76	379.63	378.38	380.42	
			Average °C	381.24	380.51	379.17	382.66	380.93	379.96	379.80	378.57	380.69	
			Stability ±°C	0.20	0.17	0.16	0.17	0.14	0.20	0.17	0.19	0.26	

Cal. Point	Setting	Reading	STD.	Position of Standards at Block									
(°C)	(°C)	(°C)	Reading	M20A2-CH12 Hole 46	M20A2-CH13 Hole 47	M20A2-CH14 Hole 48	M20A2-CH11 Hole 49	M20A2-CH12 Hole 50	M20A2-CH13 Hole 51	M20A2-CH14 Hole 52	M20A2-CH11 Hole 53	M20A2-CH12 Hole 54	
380.0	380.0	379.8 - 380.2	Max °C	379.55	379.74	381.56	381.74	381.03	381.18	379.98	380.75	380.86	
			Min °C	379.20	379.35	381.12	381.41	380.76	380.83	379.59	380.31	380.43	
			Average °C	379.37	379.55	381.34	381.57	380.89	381.00	379.79	380.53	380.65	
			Stability ± °C	0.18	0.20	0.22	0.17	0.14	0.18	0.20	0.22	0.22	

The expanded uncertainty of temperature measurement was ± 1.64 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2 , providing a level of confidence of approximately 95 % .

Approved By. 



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No.T240977

Page 1 of 5

Certificate of Calibration

Equipment : DIGESTION UNIT

Manufacturer : Environmental Express

Model : TKN100

Serial No. : 2017TKNBC142

Customer Code : BKK_EN0223

ID No. : T6773A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250



Customer Location : Wet Chemistry Lab1

Date of Receipt : 15 May 2024

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  Preecha Phisassutthikul (Temperature Calibration Manager)

Date of Issue : 28 MAY 2024

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	24/05/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T240977

Page 2 of 5

Calibration Report

Equipment : DIGESTION UNIT
Date of Calibration : 24 May 2024
Environment : Temperature : 28.7 - 30.0 °C
Line Voltage : 222.8 - 225.9 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert four standard thermocouples type S into its chamber , the other one thermocouple type T use for ambient temperature measurement . The calibration was done in according to WI-T10.

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	Type S	M20A1-(CH17-CH20)	T240714	23 April 2025
DATA LOGGER	34970A	T149	T240714	23 April 2025

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good


Equipment Description :

Time Constant 2 Hour 2 Minute At 380 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available


5. Adjustment :

() without adjustment

(X) after adjustment

Approved By. 

Calibration Report

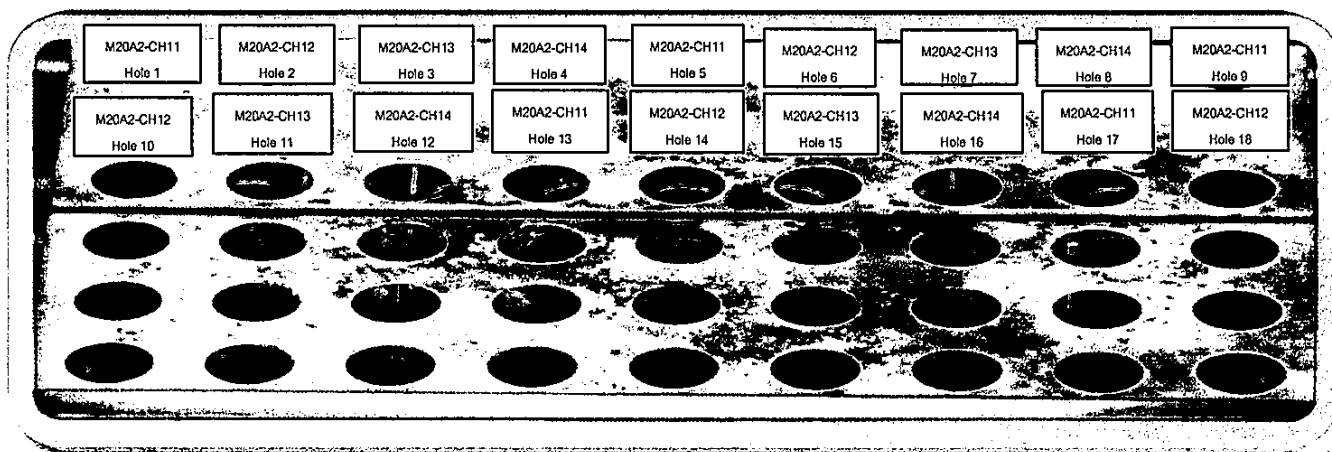


DISPLAY CONTROL (FRONT)

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	M20A2-CH11 Hole 1	M20A2-CH12 Hole 2	M20A2-CH13 Hole 3	M20A2-CH14 Hole 4	M20A2-CH11 Hole 5	M20A2-CH12 Hole 6	M20A2-CH13 Hole 7	M20A2-CH14 Hole 8	M20A2-CH11 Hole 9
380.0	380.0	379.8 - 380.2	Average °C	377.34	380.04	380.62	383.20	380.97	379.00	381.21	378.62	379.36
			Stability ±°C	0.31	0.27	0.31	0.25	0.24	0.37	0.15	0.26	0.23


Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	M20A2-CH12 Hole 10	M20A2-CH13 Hole 11	M20A2-CH14 Hole 12	M20A2-CH11 Hole 13	M20A2-CH12 Hole 14	M20A2-CH13 Hole 15	M20A2-CH14 Hole 16	M20A2-CH11 Hole 17	M20A2-CH12 Hole 18
380.0	380.0	379.8 - 380.2	Average °C	376.66	381.17	380.28	383.11	383.26	382.04	380.37	381.00	381.61
			Stability ± °C	0.35	0.34	0.35	0.24	0.21	0.23	0.23	0.20	0.22

 Approved By. 

Certificate No. T240977

Page 4 of 5

Calibration Report

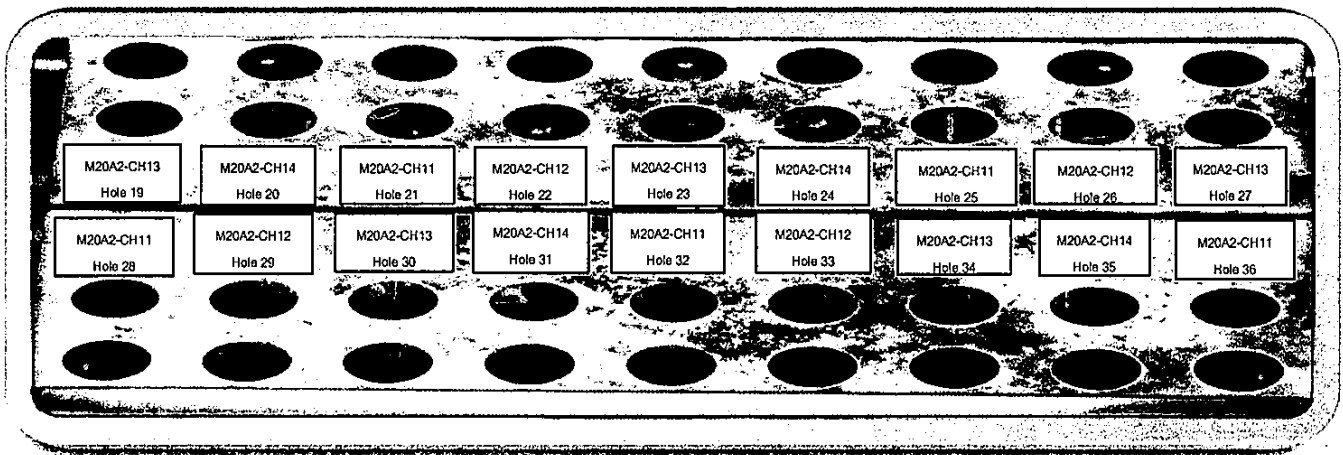


DISPLAY CONTROL (FRONT)

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	M20A2-CH13 Hole 19	M20A2-CH14 Hole 20	M20A2-CH11 Hole 21	M20A2-CH12 Hole 22	M20A2-CH13 Hole 23	M20A2-CH14 Hole 24	M20A2-CH11 Hole 25	M20A2-CH12 Hole 26	M20A2-CH13 Hole 27
380.0	380.0	379.8 - 380.2	Average °C	376.97	383.29	383.26	381.86	380.47	381.36	382.07	379.37	381.87
			Stability ±°C	0.22	0.26	0.22	0.22	0.23	0.22	0.25	0.21	0.22


Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	M20A2-CH11 Hole 28	M20A2-CH12 Hole 29	M20A2-CH13 Hole 30	M20A2-CH14 Hole 31	M20A2-CH11 Hole 32	M20A2-CH12 Hole 33	M20A2-CH13 Hole 34	M20A2-CH14 Hole 35	M20A2-CH11 Hole 36
380.0	380.0	379.8 - 380.2	Average °C	377.29	381.19	381.69	380.72	381.02	380.42	378.65	380.63	376.92
			Stability ±°C	0.25	0.27	0.27	0.26	0.22	0.28	0.19	0.23	0.22

 Approved By. 

Certificate No. T240977

Page 5 of 5

Calibration Report

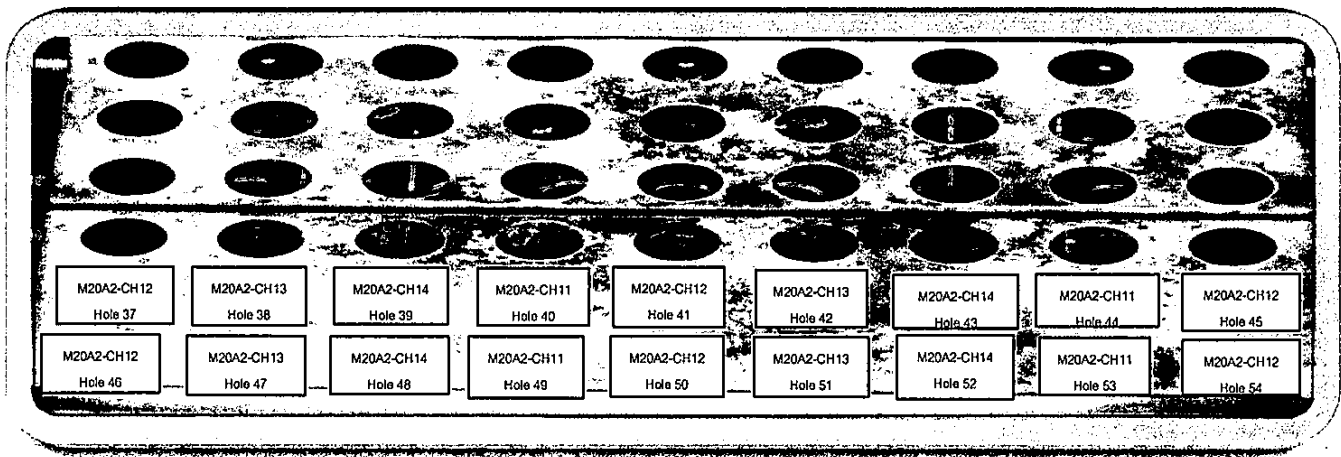

DISPLAY CONTROL (FRONT)

Measurement Results

Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	M20A2-CH12 Hole 37	M20A2-CH13 Hole 38	M20A2-CH14 Hole 39	M20A2-CH11 Hole 40	M20A2-CH12 Hole 41	M20A2-CH13 Hole 42	M20A2-CH14 Hole 43	M20A2-CH11 Hole 44	M20A2-CH12 Hole 45
380.0	380.0	379.8 - 380.2	Average °C	380.39	378.84	380.87	381.85	379.87	382.97	383.29	379.42	378.50
			Stability ± °C	0.21	0.16	0.19	0.25	0.18	0.19	0.19	0.23	0.42


Cal. Point	Setting	Reading	STD.	Position of Standards at Block								
(°C)	(°C)	(°C)	Reading	M20A2-CH12 Hole 46	M20A2-CH13 Hole 47	M20A2-CH14 Hole 48	M20A2-CH11 Hole 49	M20A2-CH12 Hole 50	M20A2-CH13 Hole 51	M20A2-CH14 Hole 52	M20A2-CH11 Hole 53	M20A2-CH12 Hole 54
380.0	380.0	379.8 - 380.2	Average °C	377.89	381.24	380.93	379.91	380.08	380.61	381.63	383.34	383.04
			Stability ± °C	0.63	0.41	0.24	0.14	0.15	0.15	0.14	0.16	0.38

 The expanded uncertainty of temperature measurement was ± 1.65 °C

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

 The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %.

 Approved By. 



บริษัท ดับเบิล เอส ไดแอกนอสติกส์ จำกัด
DOUBLE S DIAGNOSTICS CO., LTD.

4 ซอยอุดมสุข 14 แขวงบางนา เขตบางนา กรุงเทพมหานคร 10260 โทรศัพท์: (02) 747-7009 โทรสาร: (02) 747-7008
4 Soi Udomsuk 14, Bangna, Bangkok 10260 Tel. (02) 747-7009 Fax: (02) 747-7008

Maintenance Plan YEAR : 2023

เดือน	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec
รวม							12/7 OK					

Periodical maintenance check list for Konelab

	6M	12M	Note!
1.Diluent-wash tubing change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
2.ISE tubing change	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	none
3.Syringe check/change		<input checked="" type="checkbox"/>	
4.Dispensing check/ change		<input checked="" type="checkbox"/>	
5.Waste tubing change when necessary		<input checked="" type="checkbox"/>	
6.Lamp check/change	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
7.Mixer paddle/paddle change(not Konelab20)		<input checked="" type="checkbox"/>	
8.ISE needles check/change		<input checked="" type="checkbox"/>	none
9.Pump tubing check/ chance	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
10.Broken/worn out part check /change		<input checked="" type="checkbox"/>	
11.Peristaltic pump check /cleaning/ lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
12.Heating check		<input checked="" type="checkbox"/>	
13.Cooling check		<input checked="" type="checkbox"/>	
14.Dispenser mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
15.Cuvette transfer mechanic check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
16.Dispenser movement check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
17.Sample/reagent register check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
18.Dispensing tubing tightness check	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
19.Photometer and optics cleaning/check/adjustment	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
20.Workstation PC cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
21.Mechanic cleaning/lubrication	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
22.Instrument cleaning if necessary	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
23.Complete analyzer testing with waterblank/QC or sample	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
24.Test parameters/Adjustment/config. Save to USB key	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
25.UPS Test	<input type="checkbox"/>	<input checked="" type="checkbox"/>	

Place: ALS LAB Instrument: k90 Aquakem
Date/Time: 12/7/66 Serial no: 22781
Service done by: 12/7/66 Install date:
Signature of customer: 01/7/66 Date/Time: 12/7/66

Laboratory
Analyzer User

7/12/2023 21:21

Performed 7/12/2023
Lot W166

ACCEPTANCE CRITERIA

	Result	Limit	Warning
Temperature (?C)	37.7	37.0 +/- 1.0	
Dispensing ratio	16.4	14.8 - 17.2	
CV%	1.17	<1.7	
Photometric noise			
Max SD L340_2 (mA)	0.19	<2.0	
Max SD L340_4 (mA)	1.06	<3.0	
Linearity of photometer			
Slope	1.0188	0.94 - 1.06	
Curvature	0.0035	+/- 0.02	
Max bias from linear fit (mA)	3.2	<15.0	
Max delta %	-2.0	+/- 6.0	
Linearity of sample dispensing			
Proport. volume XDISP2 (?l)	2.06	1.96 - 2.16	
Proport. volume XDISP4 (?l)	4.13	3.85 - 4.40	
XDISP2 CV%	0.58	<2.0	
XDISP4 CV%	0.70	<2.0	
XDISP10 CV%	0.59	<2.0	
Needle 0 ?l volume			
Average (A)	0.009	<0.050	
Standard deviation (A)	0.002	<0.005	
Volume (?l)	0.06	<0.32	

OTHER INFORMATION

Dispensing ratio		Photom. noise: SD (mA)	
Posit	Result (A)	Posit	L340_2 L340_4
1	0.1592	1	0.07 0.64
2	0.1624	2	0.09 1.06
3	0.1631	3	0.14 0.50
4	0.1631	4	0.13 0.53
5	0.1625	5	0.19 0.38
6	0.1650	6	0.02 0.64

Laboratory
Analyzer User


7/12/2023 21:21

Linearity of sample dispensing

Test	Absorbance (A)
XDISP2	0.311
XDISP4	0.616
XDISP10	1.478

Linearity of photometer

L340_	Target (A)	Meas (A)	Delta (A)	Delta %
1	0.001	0.005	-0.004	-394.7
2	0.512	0.519	-0.007	-1.5
3	1.523	1.550	-0.027	-1.8
4	2.027	2.066	-0.039	-1.9
5	2.532	2.582	-0.050	-2.0

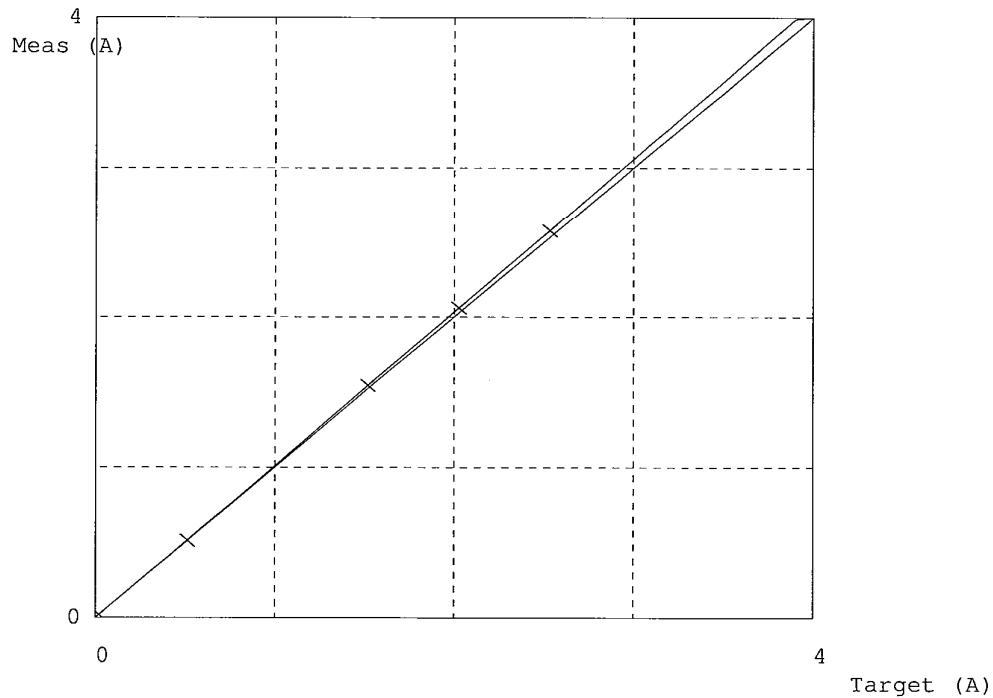



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th

E-Mail : calibrate@scg.com



Certificate No. T232009

Page 1 of 3

Certificate of Calibration

Equipment : Chamber (Oven)

Manufacturer : Memmert

Model : UF110

Serial No. : B423.1549

Customer Code : BKK_EN0425

ID No. : T4671A5

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,

Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250


Customer Location : Oven Room

Date of Receipt : 1 November 2023

Calibrated By : Atiphong Rongrat (Technician)

Approved By :  / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 NOV 2023

REVIEW BY	Siriruk B.
APPROVED BY	
NEXT CAL. DATE	06/11/24.

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T232009

Page 2 of 3

Calibration Report

Equipment : Chamber (Oven)
Date of Calibration : 6 November 2023
Environment : Temperature : 27.6-28.1 °C
Line Voltage : 222.7-227.4 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine resistance thermometer detectors into its chamber, the other one resistance thermometer detector use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	31-(CH1-10)	T230504	24 March 2024
DATA LOGGER	34970A	T114	T230504	24 March 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 2 Hour 50 Minute At 104 °C
Fresh Air Damper ☒ Open ☒ Min ☐ Medium ☐ Max
☐ Close
☐ Not Available

5. Adjustment :


(X) without adjustment

() after adjustment

Approved By. _____



Calibration Report

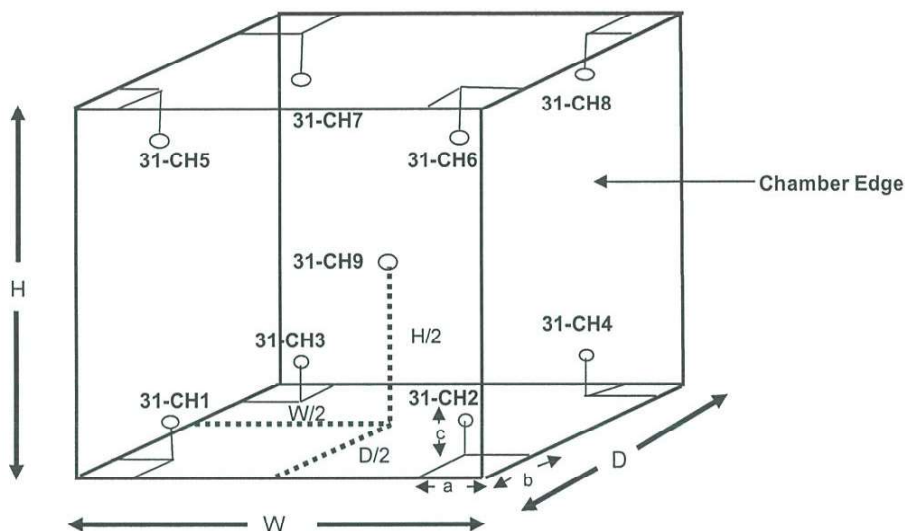

Remark :

Internal Dimensions of Chamber : W (Width) = 56 cm. H(Height)=41 cm. and D(Depth)=48 cm.
 Size of Installed Standard sensor number 31-CH1to number 31-CH8 : a = 5 cm. ,b = 5 cm. and c = 5 cm.
 Size of Installed Standard sensor number 31-CH9 : W/2=56 cm./2 H/2=41 cm./2 and D/2=48 cm./2

Measurement Results	Average Standard Reading at each position (° C)								
Calibration Point	31-CH1	31-CH2	31-CH3	31-CH4	31-CH5	31-CH6	31-CH7	31-CH8	31-CH9
104	103.82	104.10	103.74	104.26	103.95	104.31	103.87	104.00	103.81
180	180.04	180.21	179.44	180.31	179.02	180.13	180.17	180.35	179.69

Chamber (Oven)			Temperature Distribution				
Setting (° C)	Reading (° C)		Average (° C)	Stability (± ° C)	Uniformity (° C)	Uncertainty (± ° C)	Coverage Factor k
	Min , Max	Average					
104.0	-	104.0	103.98	0.14	0.60	0.42	2.00
180.0	-	180.0	179.93	0.35	0.78	0.53	2.00

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 23TW243

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000-230V
Serial No. :	09J101147
ID No. :	BKK_EN0017
Received Date :	15 November 2023
Test Date :	16 November 2023
Reference :	2311-0505DSC-4
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 Approved Signatory
<input checked="" type="checkbox"/> Saithip Meangmai <input type="checkbox"/> Warakorn Lergagtrakul <input type="checkbox"/> Ponpan Paipim	
Issue Date :	17 November 2023

REVIEW BY	<i>Kate Auk</i>
APPROVED BY	<i>Siriluk P.</i>
NEXT CAL. DATE	<i>16/05/25</i>



Cert.No.: 23TW243

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1124013382	140RC006	23MM18	20 Feb 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 16K100498

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.18	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency, The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Saitthip

a 1190297



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23LM192

Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-230V

Serial No. : 09J101147

ID No. : BKK_EN0017

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : TPA Chemistry Calibration Laboratory

Received Order : 15 November 2023


Calibrated Date : 16 November 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Kunchit Promprat

Approved by : 
Approved Signatory

() Pornthippa Tameyakul
() Ponpan Paipim
(✓) Suwit Imjai

Issue Date : 17 November 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0060730



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2311-0505DSC-10

Cert. No.: 23LM192

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	3240076	23I305	TPA	15 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 16K100498

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.0	60	19.997	19.93	-0.067	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Yunt

a 1190298



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T230682

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Incubator)

Manufacturer : MEMMERT

Model : ICP 750

Serial No. : F819.0021

Customer Code : BKK_EN0304

ID No. : T9572A4

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.

104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,

Khet Suan Luang, Bangkok 10250

Customer Location : Wet Chemistry Lab 2

Date of Receipt : 30 March 2023

Calibrated By : Sujjar Naknakred (Site Calibration Manager)

Approved By :  / Boonchai Suriyawong (Assistant Calibration Manager)

Date of Issue : 10 APR 2023

REVIEW BY	Sinluk P.
APPROVED BY	KL AL
NEXT CAL. DATE	05/04/24

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

Certificate No. T230682

Calibration Report

Page 2 of 4

Equipment : Chamber (Incubator)
Date of Calibration : 5 April 2023 (Finished Time 4:30 PM)
Environment : Temperature 22.9-28.6 °C
 Line Voltage 221.7-225.5 V

Condition of this results of test. :

- This instrument was calibrated by insert 12 standard resistance thermometer into its chamber and test according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986.)

All data show below were final values and the initial data may be obtained upon request.

The temperature scale used was based on ITS - 90.

- Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
RTD	100 ohm	37-(CH1-10)	T222493	28 November 2023
RTD	100 ohm	36-(CH1-10)	T222493	28 November 2023
DATA LOGGER	34970A	T193	T222493	28 November 2023

- This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

- Condition of calibrated item : good


UUC Description :

Time Constant 1 Hour 37 Minute At 20 °C
 Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
 ☐ Close
 ☒ Not Available

- Result of test :

() without adjustment


(X) after adjustment

Approved By. 

Certificate No T230682

Calibration Report

Page 3 of 4

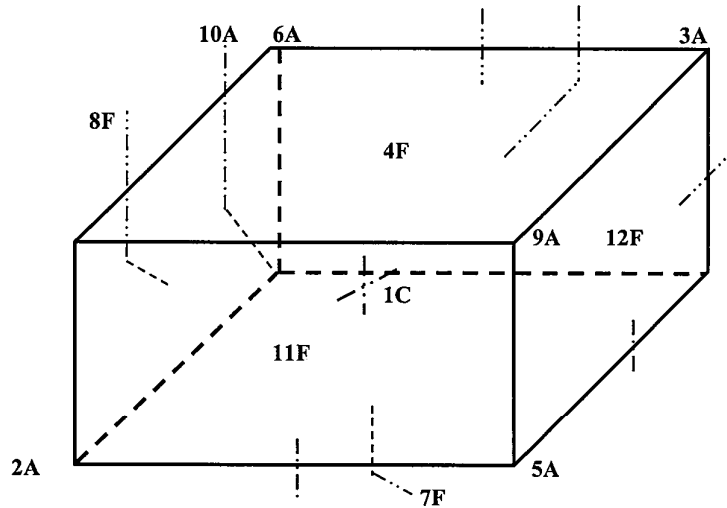

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	37CH1
2A	=	37CH2
3A	=	37CH3
4F	=	37CH4
5A	=	37CH5
6A	=	37CH6
7F	=	37CH7
8F	=	37CH8
9A	=	37CH9
10A	=	37CH10

11F	=	36CH1
12F	=	36CH2

Approved By. 

Certificate No. T230682

Calibration Report

Page 4 of 4

Measurement Results

Average Standard Reading at each position (°C)										
Calibration Point	37CH1	37CH2	37CH3	37CH4	37CH5	37CH6	37CH7	37CH8	37CH9	37CH10
20.0	20.26	20.17	20.10	20.15	20.12	19.96	20.14	19.69	20.20	19.82
	36CH1	36CH2								
	20.03	20.04								

Chamber (Incubator)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min , Max	Average					
20.0	19.9 , 20.1	20.0	19.98	0.19	0.53	0.38	2.00

* The quoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 24T2852

REFERENCE No : 72619-8

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : COOLED INCUBATOR

MANUFACTURER : MEMMERT

MODEL : ICP750

SERIAL No : F819.0021

ID No : BKK_EN0304

CONDITION AS RECEIVED : USED ITEM

SUBMITTED BY : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN
RD.,KHWAEANG PHATTHANAKAN,KHET SUAN
LUANG, BANGKOK 10250, THAILAND

REVIEW BY

Jinda K

APPROVED BY

Siriluk P.

NEXT CAL. DATE

20/03/25

CALIBRATED BY : CHAICHARN CH.

CALIBRATION DATE : 20-Mar-24

APPROVED BY

PONGSAK J.

ISSUED DATE : 21-Mar-24

RECEIVED DATE : 20-Mar-24



CERTIFICATE No : 24T2852

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : COOLED INCUBATOR
MANUFACTURER : MEMMERT
MODEL : ICP750
ID No : BKK_EN0304
RECEIVED DATE : 20-Mar-24
AMBIENT TEMPERATURE : 26 °C ± 1 °C

S/N : F819.0021
CALIBRATION DATE : 20-Mar-24
RELATIVE HUMIDITY : 54 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED THERMOCOUPLE TYPE K UNDER NO LOAD CONDITION. THE THERMOCOUPLES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOCOUPLE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOCOUPLE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH TC TYPE K	HYDRA 2635A	7286308	23T6641	14-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

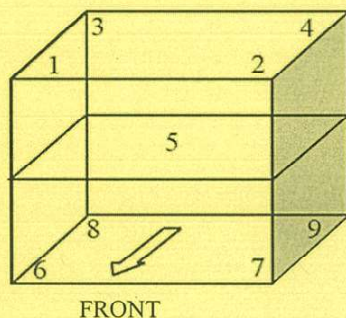

GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 5
Instrument Condition : Normal

CHAMBER PERFORMANCE

Controller Temperature (°C)	Indicating Temperature (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
20.0	20.0	0.16	0.21	0.41

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (±°C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
20.0	20.0	19.88	19.93	19.87	19.86	19.98	19.94	19.94	19.89	19.91	0.42

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.

NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.
END OF CALIBRATION REPORT



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1408

Page : 1 of 4

Certificate of Calibration

Equipment : Autoclave

Manufacturer : TOMY

Model : SX-700

Serial No. : 48134190

ID No. : BKK_ML0041

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 03 October 2023

Calibration Date : 04 October 2023

Ambient Temperature : (26 \pm 10) °C

Relative Humidity : (50 \pm 30) %

Calibrated by : Khit Ruttanaprapachai

Approved by :

Approved Signatory

() Pornthippa Tameyakul

(☒) Ponpan Paipim

() Suwit Imjai

Issue Date : 11 October 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

REVIEW BY	Sithichok
APPROVED BY	
NEXT CAL. DATE	04/04/25 03/10/24 punadon esp 16/10/23



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2310-0006OC-6

Cert. No.: 23TM1408

Page : 2 of 4

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY57013823	23LM66	TPA	25 Mar 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3**

(** = Categorization of pathogens according to hazard and categories of containment, second edition, 1990)


It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source



	Environmental		
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	26	64	221
Finished of Calibration	27	67	222

<u>Position</u>	<u>Description</u>	<u>Ref. Std. ID No.:</u>
1 =	Center of chamber	19-17TC-08
2 =	Temperature sensor	19-17TC-09
3 =	Exhaust port	19-17TC-10



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2310-0006OC-6
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM1408

Page : 3 of 4

Operating parameter Set : Temperature = 108 °C
Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
108	108	1	108.352	0.12	0.04	0.90	2
		2	108.263				
		3	108.140				

Operating parameter Set : Temperature = 115 °C
Sterilization period = 20 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
115	115	1	115.376	0.13	0.08	0.90	2
		2	115.297				
		3	115.157				

Operating parameter Set : Temperature = 118 °C
Sterilization period = 10 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
118	118	1	118.083	0.11	0.09	0.90	2
		2	118.037				
		3	117.954				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .



Equipment : Autoclave
Condition As-Received : Used Item
Reference : 2310-0006OC-6
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 23TM1408

Page : 4 of 4

Operating parameter Set : Temperature = 121 °C
Sterilization period = 30 minute

UUC* Setting (°C)	UUC* Reading (°C)	Position	Average* Standard Reading (°C)	Stability (± °C)	Pressure Reading (MPa)	Uncertainty (± °C)	Coverage Factor <i>k</i>
121	121	1	121.186	0.17	0.11	0.91	2
		2	121.082				
		3	120.980				

Average* : The average of 30 values in each position.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was excluded stability.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1146

Page : 1 of 3

Certificate of Calibration

Equipment : Incubator

Manufacturer : SHEL-LAB

Model : 1915A

Serial No. : 0200599

ID No. : BKK_ML0010

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthakan Rd.,
Khawng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Incubation & Micrological Reading

Received Order : 17 July 2023

Calibration Date : 17 July 2023

Ambient Temperature : (26 \pm 10) °C

Relative Humidity : (50 \pm 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

Malu.

Approved Signatory

() Pornthippa Tameyakul

(☒) Malee Butkruea

() Suwit Imjai

Issue Date : 24 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056489



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1
Procedure Used :-

Cert. No.: 23TM1146

Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	24
REL.Humid. (%)	54	56
AC Supply (Volt)	221	223

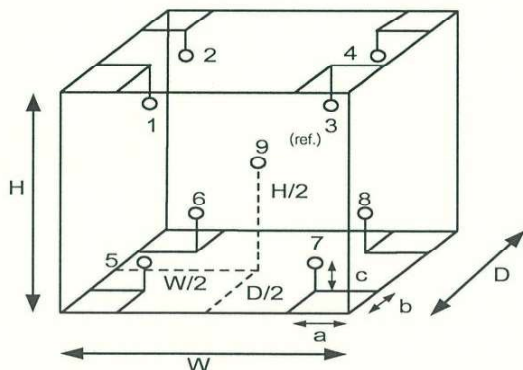

Position :	Ref. Std. ID No.:
1	19RTD-2/1
2	19RTD-2/2
3	19RTD-2/3
4	19RTD-2/4
5	19RTD-2/5
6	19RTD-2/6
7	19RTD-2/7
8	19RTD-2/8
9 (ref.)	19RTD-2/9

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.50 m
W = 0.75 m
H = 1.2 m
Capacity = 0.45 m³

Malu .



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2307-0285OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 23TM1146

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.055	0.30	0.44	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.888	34.933	34.815	34.813	35.064	35.019	35.156	35.141	35.087	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM667

Page : 1 of 3

Equipment : Hot Air Oven
Manufacturer : Binder
Model : ED 240/E2
Serial No. : 00-15533
ID No. : BKK_ML0013

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Location : Media Preparation Room

Received Order : 23 April 2024
Calibration Date : 23 April 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Tawatchai Pama

Approved by :

Approved Signatory

() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat

Issue Date : 26 April 2024

REVIEW BY Sithichok T.
APPROVED BY [Signature]
NEXT CAL DATE 23/10/25

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2404-0439OC-8
Procedure Used :-

Cert. No.: 24TM667
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY49001451	24LM44	TPA	17 Mar 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	24	23
REL.Humid. (%)	65	65
AC Supply (Volt)	223	222

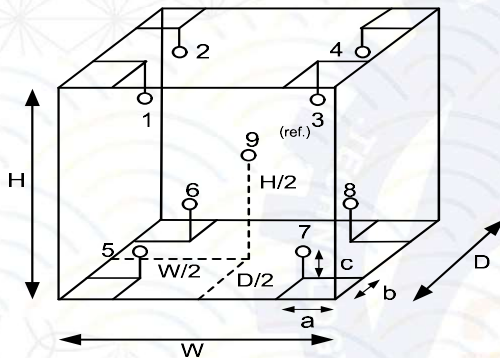

Position :	Ref. Std. ID No.:
1	24-19TC-01
2	24-19TC-02
3	24-19TC-03
4	24-19TC-04
5	24-19TC-05
6	24-19TC-06
7	24-19TC-07
8	24-19TC-08
9 (ref.)	24-19TC-09

Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.50 m
W = 0.80 m
H = 0.60 m
Capacity = 0.24 m³



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2404-0439OC-8
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM667

Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor <i>k</i>
180	180	180	0.64	2.7	3.7	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
180	181.009	181.511	180.922	181.359	181.217	183.659	181.664	181.986	181.474	1.5

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-