

# ภาคผนวกที่ 5

## เอกสารการสอบเทียบเครื่องมือ

- |        |     |   |
|--------|-----|---|
| เอกสาร | 5-1 | เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศในบรรยากาศ |
| เอกสาร | 5-2 | เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพน้ำ             |

**ตารางสรุปรายการเอกสารการสอบเทียบความถูกต้องของเครื่องมือเก็บตัวอย่าง  
และเครื่องมือตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม**

รายการตรวจวัด	เครื่องมือเก็บตัวอย่าง	เครื่องมือตรวจวิเคราะห์
	ชื่อเครื่องมือ	ชื่อเครื่องมือ
<b>คุณภาพอากาศ</b>		
- TSP	- High Volume Air Sampler No. B08, B10, B11 B20, B39	- Digital Balance
- PM <sub>10</sub>	- High Volume Air PM-10 Sampler No. B02, B03, B12, B29, R15	- Digital Balance
- PM <sub>2.5</sub>	- High Volume Air PM-2.5 Sampler No. PM2.5-05, PM2.5-09	- Digital Balance
- NO <sub>2</sub>	- NO <sub>2</sub> Analyzer No. B01, B08, B10, B13, B14	- NO <sub>2</sub> Analyzer No. B01, B08, B10, B13, B14
- SO <sub>2</sub>	- SO <sub>2</sub> Analyzer No. B01, B08, B10, R05, R08	- SO <sub>2</sub> Analyzer No. B01, B08, B10, R05, R08
- CO	- CO Analyzer No. B07, B08, B10, B11, B14	- CO Analyzer No. B07, B08, B10, B11, B14
<b>คุณภาพน้ำ</b>		
- Temperature	-	- Thermometer
- pH	-	- pH Meter
- Conductivity	-	- Conductivity Meter
- SS	-	- Digital Balance
- TDS	-	- Digital Balance
- DO	-	- ICP
- BOD <sub>5</sub>	-	- Digital Balance
- Grease & Oil	-	- Digital Balance

## เอกสารที่ 5-1

เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพอากาศในบรรยากาศ

High Volume Air Sampler Calibration Report				
Calibration Method : Multipoint Orifice Flow Transfer Standard			Model : TE 5025A	S/N : 3611
Calibration Data				
High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R <sup>2</sup>
B01	B01	10/05/2024	y = 1.153x-1.686	1.000
B02	B02	06/05/2024	y = 1.118x+2.367	0.999
B03	B03	06/05/2024	y = 1.188x-5.422	1.000
B04	B04	07/05/2024	y = 1.263x-5.863	0.999
B05	B05	07/05/2024	y = 1.265x-7.057	0.999
B06	B06	09/05/2024	y = 1.213x-4.898	0.997
B07	B07	07/05/2024	y = 1.193x-4.616	0.999
B08	B08	07/05/2024	y = 1.207x-4.482	0.998
B09	B09	06/05/2024	y = 1.216x-4.533	1.000
B10	B10	07/05/2024	y = 1.170x-0.607	1.000
B11	B11	07/05/2024	y = 1.135x-1.256	0.999
B12	B12	07/05/2024	y = 1.211x-4.879	0.997
B13	B13	07/05/2024	y = 1.237x-4.608	1.000
B14	B14	06/05/2024	y = 1.252x-5.906	0.998
B15	B15	09/05/2024	y = 1.192x-2.587	0.999
B16	B16	06/05/2024	y = 1.133x-0.425	0.996
B17	B17	06/05/2024	y = 1.250x-4.910	0.997
B18	B18	06/05/2024	y = 1.181x-4.244	0.998
B19	B19	09/05/2024	y = 1.246x-8.218	0.999
B20	B20	08/05/2024	y = 1.218x-4.223	0.999
B21	B21	08/05/2024	y = 1.189x-4.448	0.998
B22	B22	09/05/2024	y = 1.195x-6.295	0.999
B23	B23	06/05/2024	y = 1.247x-5.137	0.999
B24	B24	09/05/2024	y = 1.157x-1.861	0.998
B25	B25	07/05/2024	y = 1.079x+1.324	1.000
B26	B26	07/05/2024	y = 1.204x-3.730	0.997
B27	B27	07/05/2024	y = 1.140x-2.924	0.999
B28	B28	07/05/2024	y = 1.220x-7.484	0.999
B29	B29	07/05/2024	y = 1.215x-3.763	1.000
B30	B30	10/05/2024	y = 1.198x-3.745	0.998
B31	B31	10/05/2024	y = 1.209x-4.851	1.000
B32	B32	10/05/2024	y = 1.186x-0.772	0.996
B33	B33	10/05/2024	y = 1.237x-4.394	0.997
B34	B34	10/05/2024	y = 1.191x-4.725	0.999

High Volume Air Sampler Calibration Report				
Calibration Method : Multipoint Orifice Flow Transfer Standard		Model : TE 5025A		S/N : 3611
Calibration Data				
High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R <sup>2</sup>
B35	B35	06/05/2024	y = 1.193x-4.091	0.999
B36	B36	10/05/2024	y = 1.172x-3.010	0.998
B37	B37	06/05/2024	y = 1.212x-2.566	1.000
B38	B38	06/05/2024	y = 1.187x-3.844	0.997
B39	B39	06/05/2024	y = 1.178x-0.811	0.999
B40	B40	06/05/2024	y = 1.221x-5.480	0.998
B41	B41	06/05/2024	y = 1.219x-4.443	0.997
B42	B42	07/05/2024	y = 1.167x-2.748	0.997
B43	B43	07/05/2024	y = 1.161x-0.034	0.999
B44	B44	07/05/2024	y = 1.249x-4.278	0.999
R01	R01	07/05/2024	y = 1.183x-4.631	0.997
R02	R02	07/05/2024	y = 1.237x-5.919	0.998
R03	R03	07/05/2024	y = 1.234x-7.377	1.000
R04	R04	10/05/2024	y = 1.250x-6.680	0.996
R05	R05	10/05/2024	y = 1.176x-4.403	0.999
R06	R06	06/05/2024	y = 1.195x-4.419	0.999
R07	R07	06/05/2024	y = 1.061x+1.385	0.999
R08	R08	06/05/2024	y = 1.169x-1.426	0.999
R09	R09	06/05/2024	y = 1.150x-0.930	0.998
R10	R10	06/05/2024	y = 1.246x-6.734	0.999
R11	R11	06/05/2024	y = 1.171x-2.938	0.999
R12	R12	10/05/2024	y = 1.149x-3.415	0.998
R13	R13	10/05/2024	y = 1.158x-3.158	0.999
R14	R14	10/05/2024	y = 1.236x-4.390	1.000
R15	R15	06/05/2024	y = 1.229x-7.704	0.998
R16	R16	06/05/2024	y = 1.242x-7.570	0.998
R17	R17	07/05/2024	y = 1.211x-5.039	0.998
R18	R18	07/05/2024	y = 1.226x-5.530	0.999
R19	R19	07/05/2024	y = 1.185x-4.311	0.999
R20	R20	09/05/2024	y = 1.193x-4.417	1.000

Calibra

### High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard      Model : TE 5025A      S/N : 3611

#### Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R <sup>2</sup>
B01	B01	10/05/2024	y = 1.208x-2.196	0.999
B02	B02	06/05/2024	y = 1.126x+0.624	0.999
B03	B03	06/05/2024	y = 1.229x-3.954	0.999
B04	B04	06/05/2024	y = 1.179x-3.520	0.999
B05	B05	09/05/2024	y = 1.194x-4.966	0.998
B06	B06	09/05/2024	y = 1.211x-4.805	0.999
B07	B07	05/05/2024	y = 1.194x-4.491	0.998
B08	B08	06/05/2024	y = 1.199x-2.209	0.999
B09	B09	06/05/2024	y = 1.229x-6.309	0.999
B10	B10	07/05/2024	y = 1.205x-3.745	0.999
B11	B11	10/05/2024	y = 1.243x-4.611	0.998
B12	B12	07/05/2024	y = 1.235x-5.109	0.999
B13	B13	07/05/2024	y = 1.216x-4.616	0.999
B14	B14	08/05/2024	y = 1.206x-2.574	0.999
B15	B15	09/05/2024	y = 1.192x-1.864	0.999
B16	B16	07/05/2024	y = 1.198x-0.408	1.000
B17	B17	06/05/2024	y = 1.215x-4.321	0.996
B18	B18	10/05/2024	y = 1.221x-4.368	0.998
B19	B19	09/05/2024	y = 1.225x-4.263	0.999
B20	B20	07/05/2024	y = 1.236x-5.830	0.997
B21	B21	07/05/2024	y = 1.146x+0.363	0.998
B22	B22	09/05/2024	y = 1.204x-1.993	0.998
B23	B23	07/05/2024	y = 1.201x-3.338	0.999
B24	B24	09/05/2024	y = 1.155x-1.602	0.999
B25	B25	07/05/2024	y = 1.224x-5.057	0.998
B26	B26	06/05/2024	y = 1.188x-3.804	0.998
B27	B27	07/05/2024	y = 1.153x-4.016	0.998
B28	B28	07/05/2024	y = 1.197x-5.298	0.999
B29	B29	07/05/2024	y = 1.206x-4.662	0.999
B30	B30	07/05/2024	y = 1.181x-2.375	0.998
B31	B31	08/05/2024	y = 1.160x+0.847	0.999
B32	B32	08/05/2024	y = 1.223x-4.126	0.998
B33	B33	06/05/2024	y = 1.184x-1.773	0.999
B34	B34	07/05/2024	y = 1.229x-3.128	0.998

### High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard      Model : TE 5025A      S/N : 3611

#### Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R <sup>2</sup>
R01	R01	06/05/2024	y = 1.174x-4.049	0.999
R02	R02	06/05/2024	y = 1.205x-3.581	0.998
R03	R03	07/05/2024	y = 1.235x-6.580	0.999
R04	R04	10/05/2024	y = 1.165x-5.072	0.998
R05	R05	10/05/2024	y = 1.211x-6.166	0.997
R06	R06	06/05/2024	y = 1.203x-3.045	0.998
R07	R07	06/05/2024	y = 1.195x-3.082	0.997
R08	R08	06/05/2024	y = 1.229x-5.593	0.999
R09	R09	06/05/2024	y = 1.223x-4.946	0.997
R10	R10	09/05/2024	y = 1.169x-3.241	0.999
R11	R11	07/05/2024	y = 1.228x-2.749	0.997
R12	R12	10/05/2024	y = 1.226x-6.807	0.996
R13	R13	09/05/2024	y = 1.154x-1.960	0.998
R14	R14	06/05/2024	y = 1.205x-4.415	0.998
R15	R15	06/05/2024	y = 1.199x-3.887	0.998
R16	R16	06/05/2024	y = 1.188x-3.045	0.998
R17	R17	06/05/2024	y = 1.140x-0.557	0.997
R18	R18	06/05/2024	y = 1.165x-3.692	0.998
R19	R19	06/05/2024	y = 1.157x-0.982	0.999
R20	R20	06/05/2024	y = 1.177x-5.526	1.000

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	22 May 2024	BRAND :	API	MODEL :	200A
NO.	NOX-B01	SERIAL NO.	2368		
Calibrator (Dilution System)					
Brand :	Teledyne	Model :	700		
Last Cal. Date :	30 October 2023	Serial No. :	421		
Reference Standard Gas					
Standard Gas :	Nitric Oxide (NO)	Cylinder No. :	A00726SV		
Certified Date :	05 January 2023	Expired Date :	05 January 2026	Cylinder Conc. :	48.8 ppm
CALIBRATING CONDITION					
Pressure	1011 mmbar	Temp.	24.5 °C	% RH	48
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.11	-	0	-
NO Span	400	399.9	-0.025	400.0	1.007
NO <sub>x</sub> Span	400	400.2	0.050	400.0	1.011
API Model 200A NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	507	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.1	mV	-20 ~ 150		
AZERO	93.9	mV	-20 ~ 150		
HVPS	670	V	420 ~ 900 constant		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.4	°C	8 ~ 48		
PMT TEMP	7.2	°C	7 ± 2		
MOLY TEMP	314.9	°C	315 ± 5		
RCELL PRESS	8.2	IN-Hg-A	2 ~ 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 ~ 30 constant		
NO Span Conc	400	PPB	20 ~ 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 ~ 20,000		
NO Slope	1.007	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.011	-	1.0 ± 0.3		
NO Offset	1.5	mV	-20 to +150		
NO <sub>x</sub> Offset	0.9	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	22 May 2024	BRAND :	API	MODEL :	200E
NO.	NOX-B08	SERIAL NO.	4336		
Calibrator (Dilution System)					
Brand :	Teledyne	Model :	700		
Last Cal. Date :	30 October 2023	Serial No. :	421		
Reference Standard Gas					
Standard Gas :	Nitric Oxide (NO)	Cylinder No. :	A00726SV		
Certified Date :	05 January 2023	Expired Date :	05 January 2026	Cylinder Conc. :	48.8 ppm
CALIBRATING CONDITION					
Pressure	1011 mmbar	Temp.	24.5 °C	% RH	48
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	399.8	-0.050	400.0	1.006
NO <sub>x</sub> Span	400	400.1	0.025	400.0	1.009
API Model 200E NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	504	cc/min	500 ± 50		
OZONE FLOW	78	cc/min	80 ± 15		
PMT	103.4	mV	-20 ~ 150		
AZERO	94.2	mV	-20 ~ 150		
HVPS	675	V	420 ~ 900 constant		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.0	°C	8 ~ 48		
PMT TEMP	7.4	°C	7 ± 2		
MOLY TEMP	315.1	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 ~ 10 constant		
SAMPLE PRESS	28.4	IN-Hg-A	25 ~ 30 constant		
NO Span Conc	400	PPB	20 ~ 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 ~ 20,000		
NO Slope	1.006	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.009	-	1.0 ± 0.3		
NO Offset	1.4	mV	-20 to +150		
NO <sub>x</sub> Offset	0.9	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sales@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	22 May 2024	BRAND :	API	MODEL :	200E
NO.	NOX-B10	SERIAL NO.	4465		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 30 October 2023		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A00726SV	
Certified Date	: 05 January 2023		Expired Date	: 05 January 2026	
Cylinder Conc.				: 48.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
NO Span	400	399.7	-0.075	400.0	1.004
NO <sub>x</sub> Span	400	399.9	-0.025	400.0	1.007
API Model 200E NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	509	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.2	mV	-20 ~ 150		
AZERO	94.0	mV	-20 ~ 150		
HVPS	669	V	420 ~ 900 constant		
RCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	28.8	°C	8 ~ 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	315.3	°C	315 ± 5		
RCELL PRESS	8.5	IN-Hg-A	2 ~ 10 constant		
SAMPLE PRESS	28.7	IN-Hg-A	25 ~ 30 constant		
NO Span Conc	400	PPB	20 ~ 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 ~ 20,000		
NO Slope	1.004	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.007	-	1.0 ± 0.3		
NO Offset	1.2	mV	-20 to +150		
NO <sub>x</sub> Offset	0.8	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chaluchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sales@spscon.com, www.spscon.com

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	22 May 2024	BRAND :	API	MODEL :	200A
NO.	NOX-B13	SERIAL NO.	1983		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 30 October 2023		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A00726SV	
Certified Date	: 05 January 2023		Expired Date	: 05 January 2026	
Cylinder Conc.				: 48.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.11	-	0	-
NO Span	400	400.1	0.025	400.0	1.010
NO <sub>x</sub> Span	400	400.3	0.075	400.0	1.014
API Model 200E NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	510	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.3	mV	-20 ~ 150		
AZERO	94.1	mV	-20 ~ 150		
HVPS	672	V	420 ~ 900 constant		
RCELL TEMP	50.5	°C	50 ± 1		
BOX TEMP	29.3	°C	8 ~ 48		
PMT TEMP	7.1	°C	7 ± 2		
MOLY TEMP	315.2	°C	315 ± 5		
RCELL PRESS	8.3	IN-Hg-A	2 ~ 10 constant		
SAMPLE PRESS	28.5	IN-Hg-A	25 ~ 30 constant		
NO Span Conc	400	PPB	20 ~ 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 ~ 20,000		
NO Slope	1.010	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.014	-	1.0 ± 0.3		
NO Offset	1.7	mV	-20 to +150		
NO <sub>x</sub> Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

CALIBRATION REPORT					
CHEMILUMINESCENT NO / NO <sub>2</sub> / NO <sub>x</sub> ANALYZER					
DATE :	22 May 2024	BRAND :	API	MODEL :	200A
NO.	NOX-B14	SERIAL NO.	212		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 30 October 2023		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Nitric Oxide (NO)		Cylinder No.	: A00726SV	
Certified Date	: 05 January 2023	Expired Date	: 05 January 2026	Cylinder Conc.	: 48.8 ppm
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
NO Span	400	400.1	0.025	400.0	1.009
NO <sub>x</sub> Span	400	400.2	0.050	400.0	1.012
API Model 200A NO <sub>x</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	500 standard		
STABILITY (Zero Gas)	0.1	PPB	< 2 with zero air		
SAMPLE FLOW	511	cc/min	500 ± 50		
OZONE FLOW	79	cc/min	80 ± 15		
PMT	103.5	mV	-20 ~ 150		
AZERO	94.2	mV	-20 ~ 150		
HVPS	673	V	420 ~ 900 constant		
RCELL TEMP	50.4	°C	50 ± 1		
BOX TEMP	29.2	°C	8 ~ 48		
PMT TEMP	7.3	°C	7 ± 2		
MOLY TEMP	314.7	°C	315 ± 5		
RCELL PRESS	8.4	IN-Hg-A	2 ~ 10 constant		
SAMPLE PRESS	28.6	IN-Hg-A	25 ~ 30 constant		
NO Span Conc	400	PPB	20 ~ 20,000		
NO <sub>x</sub> Span Conc	400	PPB	20 ~ 20,000		
NO Slope	1.009	-	1.0 ± 0.3		
NO <sub>x</sub> Slope	1.012	-	1.0 ± 0.3		
NO Offset	1.6	mV	-20 to +150		
NO <sub>x</sub> Offset	1.0	mV	-20 to 150		
Stability at Zero	0.1	PPB	< 0.2		
Stability at Span	0.2	PPB	< 2 ppb @ 400 ppb span gas		

CALIBRATION REPORT				
SO <sub>2</sub> FLUORESCENT ANALYZER				
DATE :	22 May 2024	BRAND :	API	MODEL :
NO.	SO <sub>2</sub> -B01	SERIAL NO.	1749	
Calibrator (Dilution System)				
Brand	: Teledyne		Model	: 700
Last Cal. Date	: 30 October 2023		Serial No.	: 421
Reference Standard Gas				
Standard Gas	: Sulphur Dioxide (SO <sub>2</sub> )		Cylinder No.	: A00814SK
Certified Date	: 21 June 2021	Expired Date	: 21 June 2029	Cylinder Conc.
CALIBRATING CONDITION				
Pressure	1011	mmbar	Temp.	24.5
% RH	48			
CALIBRATION SETTING				
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	0.11	-	0
SO <sub>2</sub> Span	400.0	400.2	0.050	400.0
API Model 100A SO <sub>2</sub> Analyzer Check list				
Test Values	Observed Value	Units	Nominal Range	
RANGE	500	PPB	0-500	
SAMPLE PRESS	28.7	in-Hg	25-35	
SAMPLE FLOW	658	cc/min	650 ± 10%	
PMT	103.1	mV	-20-150 with Zero Air	
UV LAMP	3016.5	mV	1000-4900	
STR. LGT	61.9	PPB	<100	
DRK PMT	63.4	mV	-50 ~ 200	
DRK LMP	58.2	mV	-50 ~ 200	
HVPS	675	V	550-900 constant	
DCPS	2527	mV	2500 ± 200	
RCELL TEMP	50.2	°C	50 ± 1	
BOX TEMP	29.5	°C	5-40	
PMT TEMP	7.4	°C	7 ± 2.0	
SO <sub>2</sub> Span Conc	400	PPB	20-20,000	
SO <sub>2</sub> Slope	1.013	-	1.0 ± 0.3	
SO <sub>2</sub> Offset	22.2	mV	<250	
Stability at Zero	0.1	PPB	<0.2	
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)	





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพมหานคร 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	22 May 2024	BRAND :	API	MODEL :	100A
NO.	SO <sub>2</sub> -B08	SERIAL NO.	1003		
Calibrator (Dilution System)					
Brand : Teledyne		Model : 700			
Last Cal. Date : 30 October 2023		Serial No. : 421			
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO <sub>2</sub> )		Cylinder No. : A00814SK			
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011 mmbar	Temp.	24.5 °C	% RH	48
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.8	-0.050	400.0	1.007
API Model 100A SO <sub>2</sub> Analyzer Check List					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.6	in-Hg	25-35		
SAMPLE FLOW	654	cc/min	650 ± 10%		
PMT	103.0	mV	-20-150 with Zero Air		
UV LAMP	3011.7	mV	1000-4900		
STR. LGT	61.5	PPB	<100		
DRK PMT	63.0	mV	-50 - 200		
DRK LMP	57.7	mV	-50 - 200		
HVPS	672	V	550-900 constant		
DCPS	2516	mV	2500 ± 200		
RCELL TEMP	50.0	°C	50 ± 1		
BOX TEMP	28.9	°C	5-40		
PMT TEMP	7.1	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.007	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	21.8	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร เขตจตุจักร กรุงเทพมหานคร 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	22 May 2024	BRAND :	Thermo	MODEL :	43C
NO.	SO <sub>2</sub> -B10	SERIAL NO.	43C-69604-364		
Calibrator (Dilution System)					
Brand : Teledyne		Model : 700			
Last Cal. Date : 30 October 2023		Serial No. : 421			
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO <sub>2</sub> )		Cylinder No. : A00814SK			
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011 mmbar	24.5 °C	% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	-0.10	-	0	
SO <sub>2</sub> Span	400.0	400.1	0.025	400.0	
INSTRUMENT STATUS					
CHAMBER TEMP	44.5 °C	FLOW	1.0 LPM		
PRESSURE	728.7 mm Hg				

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	22 May 2024	BRAND :	API	MODEL :	100E
NO.	SO <sub>2</sub> -R05	SERIAL NO.	3490		
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 30 October 2023			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO <sub>2</sub> )			Cylinder No. : A00814SK		
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
			% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.6	-0.100	400.0	1.005
API Model 100E SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.4	in-Hg	25-35		
SAMPLE FLOW	657	cc/min	650 ± 10%		
PMT	103.3	mV	-20-150 with Zero Air		
UV LAMP	3037.4	mV	1000-4900		
STR. LGT	61.8	PPB	<100		
DRK PMT	63.3	mV	-50 - 200		
DRK LMP	58.0	mV	-50 - 200		
HVPS	669	V	550-900 constant		
DCPS	2521	mV	2500 ± 200		
RCELL TEMP	50.3	°C	50 ± 1		
BOX TEMP	29.0	°C	5-40		
PMT TEMP	7.2	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.005	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	21.9	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		

CALIBRATION REPORT					
SO <sub>2</sub> FLUORESCENT ANALYZER					
DATE :	22 May 2024	BRAND :	TELEDYNE	MODEL :	TML-60
NO.	SO <sub>2</sub> -R08	SERIAL NO.	TR51064		
Calibrator (Dilution System)					
Brand : Teledyne			Model : 700		
Last Cal. Date : 30 October 2023			Serial No. : 421		
Reference Standard Gas					
Standard Gas : Sulphur Dioxide (SO <sub>2</sub> )			Cylinder No. : A00814SK		
Certified Date : 21 June 2021		Expired Date : 21 June 2029		Cylinder Conc. : 49.8 ppm	
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.5	°C
			% RH	48	
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPB			Final Reading (After Adj.),PPB	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	Slope
Zero	0	-0.10	-	0	-
SO <sub>2</sub> Span	400.0	399.9	-0.025	400.0	1.010
API Model TML-60 SO <sub>2</sub> Analyzer Check list					
Test Values	Observed Value	Units	Nominal Range		
RANGE	500	PPB	0-500		
SAMPLE PRESS	28.5	in-Hg	25-35		
SAMPLE FLOW	659	cc/min	650 ± 10%		
PMT	103.2	mV	-20-150 with Zero Air		
UV LAMP	3031.8	mV	1000-4900		
STR. LGT	61.6	PPB	<100		
DRK PMT	63.1	mV	-50 - 200		
DRK LMP	57.9	mV	-50 - 200		
HVPS	671	V	550-900 constant		
DCPS	2519	mV	2500 ± 200		
RCELL TEMP	50.1	°C	50 ± 1		
BOX TEMP	29.3	°C	5-40		
PMT TEMP	7.5	°C	7 ± 2.0		
SO <sub>2</sub> Span Conc	400	PPB	20-20,000		
SO <sub>2</sub> Slope	1.010	-	1.0 ± 0.3		
SO <sub>2</sub> Offset	22.1	mV	<250		
Stability at Zero	0.1	PPB	<0.2		
Stability at Span	0.2	PPB	0.5% of reading (above 50 ppb)		



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spicon.com, www.spicon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	22 May 2024	Brand :	Thermo	Model :	48C
No.	CO-807	Serial No.	0335203746		
Calibrator (Dilution System)					
Brand : Teledyne		Model : 700			
Last Cal. Date : 30 October 2023		Serial No. : 421			
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)		Cylinder No. : D711839			
Certified Date : 14 March 2024	Expired Date : 14 March 2032	Cylinder Conc. : 4,580 ppm			
Calibrating Condition					
Pressure	1011 mmbar	Temp.	24.5 °C	% RH	48
Calibration Setting					
Span	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM	
Set Point	Expected Concentration	Analyzer Response	%Diff	Analyzer Response	
Zero	0	0.11	-	0	
CO Span	40.00	39.93	-0.175	40.00	
Instrument Status					
Chamber Temp	47.5 °C	Flow	1.5 LPM		
Pressure	730.7 mm Hg	Motor Speed	100.00%		



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chatuchak, Bangkok 10900  
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spicon.com, www.spicon.com

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	22 May 2024	Brand :	Thermo	Model :	48C
No.	CO-808	Serial No.	0508011067		
Calibrator (Dilution System)					
Brand : Teledyne		Model : 700			
Last Cal. Date : 30 October 2023		Serial No. : 421			
Reference Standard Gas					
Standard Gas : Carbon Monoxide (CO)		Cylinder No. : D711839			
Certified Date : 14 March 2024	Expired Date : 14 March 2032	Cylinder Conc. : 4,580 ppm			
Calibrating Condition					
Pressure	1011 mmbar	Temp.	24.5 °C	% RH	48
Calibration Setting					
Span	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM	
Set Point	Expected Concentration	Analyzer Response	%Diff	Analyzer Response	
Zero	0	0.10	-	0	
CO Span	40.00	39.95	-0.125	40.00	
Instrument Status					
Chamber Temp	47.2 °C	Flow	1.5 LPM		
Pressure	730.5 mm Hg	Motor Speed	100.00%		

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	22 May 2024	Brand :	API	Model :	300E
No.	CO-810	Serial No.	199-5		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 30 October 2023		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Carbon Monoxide (CO)		Cylinder No.	: D711839	
Certified Date	: 14 March 2024	Expired Date	: 14 March 2032	Cylinder Conc.	: 4,580 ppm
Calibrating Condition					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
Calibration Setting					
Span	Initial Reading (Before Adj.), PPM		Final Reading (After Adj.), PPM		
Set Point	Expected Concentration	Analyzer Response	%Diff	Analyzer Response	
Zero	0	0.11	-	0	
CO Span	40.00	40.04	0.100	40.00	
API Model 300E CO Analyzer Check List					
Parameter	Observed Value	Units	Nominal Range		
Range	50	PPM	0-1000 ppm		
Stability	0.10	PPM	± 1 ppm With Zero Air		
CO Measure	4015.3	mV	2500-4800 mV		
CO Reference	3947.8	mV	2500-4800 mV		
Measure/Reference Ratio	1.180	-	1.1-1.3 W/Zero Air		
Sample Pressure	28.7	In-Hg-A	±2"± Ambient Absolute Pressure		
Sample Flow	806	CC/Min	800 ± 10%		
Sample Temperature	48.4	°C	48 ± 4		
Bench Temperature	48.1	°C	48 ± 2		
Wheel Temperature	68.3	°C	68 ± 2		
Box Temperature	30.8	°C	Ambient Temp + 7 ± 10		
Photo-Drive	3027.3	mV	250 mV to 4750 mV		
Slope	1.017	-	1.0 ± 0.3		
Offset	0.2	-	0 ± 0.3		

Calibration Report					
Non-Dispersive Infrared CO Analyzer					
Date :	22 May 2024	Brand :	Thermo	Model :	68C
No.	CO-811	Serial No.	401304262		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700	
Last Cal. Date	: 30 October 2023		Serial No.	: 421	
Reference Standard Gas					
Standard Gas	: Carbon Monoxide (CO)		Cylinder No.	: D711839	
Certified Date	: 14 March 2024	Expired Date	: 14 March 2032	Cylinder Conc.	: 4,580 ppm
Calibrating Condition					
Pressure	1011	mmbar	Temp.	24.5	°C
% RH	48				
Calibration Setting					
Span	Initial Reading (Before Adj.),PPM		Final Reading (After Adj.),PPM		
Set Point	Expected Concentration	Analyzer Response	%Diff	Analyzer Response	
Zero	0	0.10	-	0	
CO Span	40.00	39.91	-0.225	40.00	
Instrument Status					
Chamber Temp	47.4	°C	Flow	1.5 LPM	
Pressure	730.6	mm Hg	Motor Speed	100.00%	



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอย พหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscs.com, www.spscs.com

Calibration Report							
Non-Dispersive Infrared CO Analyzer							
Date :	22 May 2024	Brand :	API				
No.	CO-B14	Model :	300EU				
		Serial No.	131				
Calibrator (Dilution System)							
Brand	: Teledyne		Model	: 700			
Last Cal. Date	: 30 October 2023		Serial No.	: 421			
Reference Standard Gas							
Standard Gas	: Carbon Monoxide (CO)		Cylinder No.	: D711839			
Certified Date	: 14 March 2024	Expired Date	: 14 March 2032	Cylinder Conc.	: 4,580 ppm		
Calibrating Condition							
Pressure	1011	mmbar	Temp.	24.5	°C	% RH	48
Calibration Setting							
Span	Initial Reading (Before Adj.), PPM			Final Reading (After Adj.), PPM			
Set Point	Expected Concentration	Analyzer Response	%Of	Analyzer Response			
Zero	0	0.11	-	0			
CO Span	40.00	40.03	0.075	40.00			
API Model 300EU CO Analyzer Check List							
Parameter	Observed Value	Units	Nominal Range				
Range	50	PPM	0-1000 ppm				
Stability	0.10	PPM	± 1 ppm With Zero Air				
CO Measure	4014.6	mV	2500-4800 mV				
CO Reference	3948.5	mV	2500-4800 mV				
Measure/Reference Ratio	1.179	-	1.1-1.3 W/Zero Air				
Sample Pressure	28.4	in-Hg-A	~2" ± Ambient Absolute Pressure				
Sample Flow	810	CC/Min	800 ± 10%				
Sample Temperature	48.5	°C	48 ± 4				
Bench Temperature	48.2	°C	48 ± 2				
Wheel Temperature	68.5	°C	68 ± 2				
Box Temperature	30.9	°C	Ambient Temp + 7 ± 10				
Photo-Drive	3049.8	mV	250 mV to 4750 mV				
Slope	1.017	-	1.0 ± 0.3				
Offset	0.2	-	0 ± 0.3				





บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
Tel: (662) 939-4370 (Automatic 5 Lines) Fax: (662) 513-4221 E-mail: sale@spscon.com

CALIBRATION REPORT			
PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)			
DATE :	22 May 2024	BRAND :	BGI
		MODEL :	PQ200
NO.	PM2.5-05	SERIAL NO.	160810-14(VSCC)
CALIBRATING CONDITION			
Pressure	1011	mmbar	Temp. 24.5 °C
		% RH	49
Calibration Method : Dry Cal Primary		Model : Defender 510 H	S/N : 136164
CALIBRATION SETTING			
detaCal	PM2.5 AIR SAMPLER		
Flowrate Reading,L/min	Initial Flowrate Reading (Before Adj.),L/min	%Dif.	Final Flowrate Reading (After Adj.),L/min
16.70	16.66	0.240	16.70



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด  
S.P.S. CONSULTING SERVICE CO., LTD.  
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900  
Tel: (662) 939-4370 (Automatic 5 Lines) Fax: (662) 513-4221 E-mail: sale@spscon.com

CALIBRATION REPORT			
PM2.5 AIR SAMPLER (VERY SHARP CUT CYCLONE-VSCC)			
DATE :	22 May 2024	BRAND :	BGI
		MODEL :	PQ200
NO.	PM2.5-09	SERIAL NO.	152125 (VSCC)
CALIBRATING CONDITION			
Pressure	1011	mmbar	Temp. 24.5 °C
		% RH	49
Calibration Method : Dry Cal Primary		Model : Defender 510 H	S/N : 136164
CALIBRATION SETTING			
detaCal	PM2.5 AIR SAMPLER		
Flowrate Reading,L/min	Initial Flowrate Reading (Before Adj.),L/min	%Dif.	Final Flowrate Reading (After Adj.),L/min
16.70	16.64	0.359	16.70

**ENVIR SERVICE CO., LTD.**

42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230  
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

**CALIBRATION TEST REPORT FOR Partisol® Model 2000-H Air Sampler**

Calibrated Date: 02 May 2024  
Calibrated Due on: 01 May 2025

Report No: PM-202405002

**Instruments Information**

Description : Thermo Scientific Partisol FRM  
2000 Air Sampler for PM-2.5

Model : 2000

Sample flow control and reporting : 5 - 18 L/min

Serial No. : 200FB211771101

**Instrument used for calibration [STD]**

Description : Flow Meter  
BIOS DryCal DC-Lite

Model : DCL-M REV. 1.08

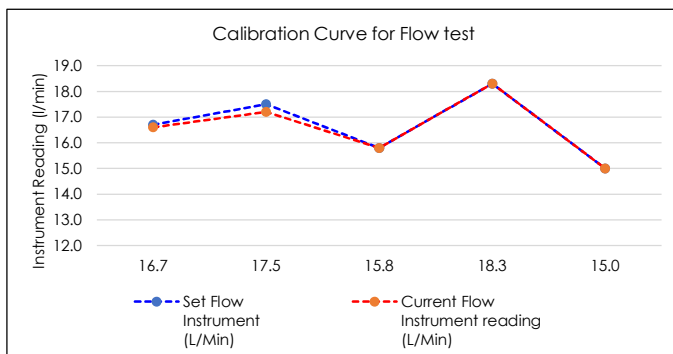
Range : 200 ml/min - 20 L/min

Serial No. : 1519

Environment : Temperature 25.5 °C Humidity: 51 %RH

**Calibration Report**

Filter	Set Flow Instrument (L/Min)	Current Flow Instrument reading (L/Min)	Actual Flow Reference standard (L/Min)	Flow Offset	Flow Span
47 mm.	16.7	16.6	16.7	0.0098	0.9987
	17.5	17.2	17.4	0.0098	0.9718
	15.8	15.8	15.7	0.0098	0.9634
	18.3	18.3	18.3	0.0098	0.9556
	15.0	15.0	15.1	0.0098	0.9635

**ENVIR SERVICE CO., LTD.**

42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230  
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

**CALIBRATION TEST REPORT FOR Partisol 2000i-D Air Sampler**

Calibrated Date: 11 October 2023  
Calibrated Due on: 10 October 2024

Report No: PM-202310012

**Instruments Information**

Description : Thermo Scientific Partisol 2000i-D  
Air Sampler

Model : 2000i-D

Sample flow control and reporting : 5 - 18 LPM

Serial No. : 200ID2 01061102

**Instrument used for calibration [STD]**

Description : Flow Meter  
BIOS DryCal DC-Lite

Model : DCL-M REV. 1.08

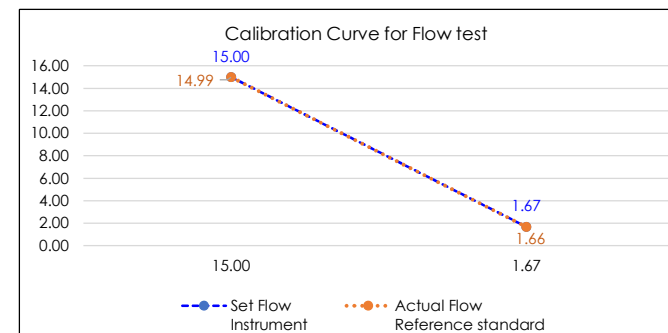
Range : 200 ml/min - 20 L/min

Serial No. : 5016

Environment : Temperature 25.5 °C Humidity: 51 %RH

**Calibration Report**

Filter	Set Flow Instrument (L/Min)	Current Flow Instrument reading (L/Min)	Actual Flow Reference standard (L/Min)	Error	Drift%
47 mm	15.00	15.00	14.99	-0.01	0.09
	1.67	1.67	1.66	-0.01	0.72





# ENVIR SERVICE CO., LTD.

42 Ramintra 14 Yeak 9, Tha Raeng, Bang Khen, Bangkok 10230  
Tel. 02-9435814-5 Fax. 02-9438201 www.envirservice.co.th

## CALIBRATION TEST REPORT FOR Partisol® Model 2000 Air Sampler

Calibrated Date: 05 June 2024  
Calibrated Due on: 04 June 2025

Report No: PM-202406002

### Instruments Information

Description : Thermo Scientific Partisol FRM  
2000 Air Sampler for PM-2.5

Model : 2000

Sample flow control and reporting : 5 - 18 L/min

Serial No. : 200FB208860804

### Instrument used for calibration [STD]

Description : Flow Meter  
BIOS DryCal DC-Lite

Model : DCL-M REV. 1.08

Range : 200 ml/min - 20 L/min

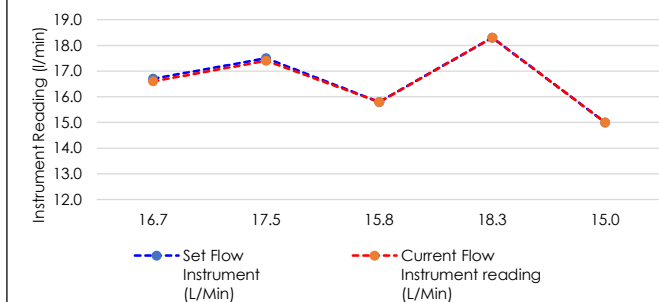
Serial No. : 1519

Environment : Temperature 25.5 °C Humidity: 51 %RH

### Calibration Report

Filter	Set Flow Instrument (L/Min)	Current Flow Instrument reading (L/Min)	Actual Flow Reference standard (L/Min)	Flow Offset	Flow Span
47 mm.	16.7	16.6	16.7	0.0078	1.0000
	17.5	17.4	17.4	0.0078	0.9180
	15.8	15.8	15.7	0.0078	0.9534
	18.3	18.3	18.3	0.0078	0.9540
	15.0	15.0	15.1	0.0078	0.9633

Calibration Curve for Flow test



**QUALITY CALIBRATION CO.,LTD.**235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584[www.qcalibration.com](http://www.qcalibration.com)CERTIFICATE No : 24M2227  
REFERENCE No : 72448-1

PAGE : 1 OF 2

**Certificate of Calibration**

**EQUIPMENT** : DIGITAL BALANCE

**MANUFACTURER** : METTLER TOLEDO

**MODEL** : XS105DU

**SERIAL No** : 1126422905


**ID No** : BA05/50

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 08-Mar-24

**APPROVED BY** : 

**ISSUED DATE** : 14-Mar-24

**RECEIVED DATE** : 08-Mar-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV 03

**QUALITY CALIBRATION CO.,LTD.**235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 24M2227

PAGE : 2 OF 2

**Calibration Report**

**EQUIPMENT** : DIGITAL BALANCE **MODEL** : XS105DU

**MANUFACTURER** : METTLER TOLEDO **S/N** : 1126422905

**ID No** : BA05/50 **RECEIVED DATE** : 08-Mar-24

**AIR PRESSURE** : 1010mbar  $\pm$  1mbar **CALIBRATION DATE** : 08-Mar-24

**AMBIENT TEMPERATURE** : 25° C  $\pm$  1° C **RELATIVE HUMIDITY** : 53 %RH  $\pm$  10 % RH

**CONDITION OF THIS RESULTS OF CALIBRATION**

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

**2. REFERENCE STANDARD INSTRUMENTS :-**

<u>INSTRUMENT</u>	<u>MODEL</u>	<u>SERIAL No</u>	<u>CERTIFICATE No</u>	<u>DUE DATE</u>
1) STANDARD WEIGHT SET	E2	QK-1-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

**RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT**


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000055
0.02	0.02001	-0.00001	0.000065
0.10	0.10002	-0.00002	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	9.99994	0.00006	0.000070
20.00	20.00008	-0.00008	0.000078
50.00	50.00000	0.00000	0.00013
100.00	100.00001	-0.00001	0.00019
120.00	120.00001	-0.00001	0.00022

**5. OFF CENTER LOADING ERROR**

POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A  
COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

## เอกสารที่ 5-2

เอกสารสอบเทียบเครื่องมือการตรวจวัดคุณภาพน้ำ



# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpoo, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



## Certificate of Calibration

**Certificate No. :** 67-400037-2

**Page : 1 of 2**

**Submitted by :** S. P. S Consulting Service Co.,Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900

**Equipment :** Liquid in Glass Thermometer

**Manufacturer :** SK

**Model :** N/A

**Range :** 0 °C to 100 °C

**Resolution :** 1 °C

**Serial No. :** N/A

**Immersion :** Total

**ID No. :** TM21/59

**Environment :** Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Line Voltage : (220 ± 22) VAC

**Date of Received :** 23 January 2024

**Date of Calibration :** 03 February 2024

**Date of Issue :** 03 February 2024

**Calibrated by :** Chortip Samchusri

**Calibration Method :** This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400003	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)
400004	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)

Approve

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL-F0031-03

# CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpoo, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

## Certificate of Calibration

**Certificate No. :** 67-400037-2

**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

Ice point check : UUC\* reading 0 °C Standard reading 0.4336 °C

Standard Reading ( °C )	UUC Reading ( °C )	Correction ( °C )	Uncertainty ( ± °C )
20.5609	20	0.6	0.31

**Remark**

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- 000 -



CAL-F0031-03

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

NCE-TIS-TS1725  
CALIBRATION ID#9

CERTIFICATE No : 23E8494

REFERENCE No : 70413-1

PAGE : 1 OF 3

**Certificate of Calibration**

**EQUIPMENT** : pH METER

**MANUFACTURER** : HANNA

**MODEL** : HI 3512

**SERIAL No** : TH118035

**ID No** : pH04/56

**CONDITION AS RECEIVED** : USED ITEM

**SUBMITTED BY** : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

**CALIBRATED BY** : ATSAWIN Y.

**CALIBRATION DATE** : 06-Sep-23

**APPROVED BY** : [Signature]

**ISSUED DATE** : 06-Sep-23

**RECEIVED DATE** : 31-Aug-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV 03

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 2 OF 3

**Calibration Report**

**EQUIPMENT** : pH METER

**MANUFACTURER** : HANNA

**ID No** : pH04/56

**RECEIVED DATE** : 31-Aug-23

**AMBIENT TEMPERATURE** : 23 ° C ± 3 ° C

**MODEL** : HI 3512

**SERIAL NUMBER** : TH118035

**CALIBRATION DATE** : 06-Sep-23

**RELATIVE HUMIDITY** : 50 % RH ± 10% RH

**CONDITION OF THIS RESULTS OF CALIBRATION**

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER
2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	23E1312	19-Apr-24
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
  - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
  - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

**RESULT OF CALIBRATION : ADJUSTMENT****1. DISPLAY UNIT ONLY**

SLOPE FACTOR k = 2.303 RT/F = 59 mV/pH

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UUC READING (pH)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
414.11	414.6	-0.49	-0.290	0.15	2.00
354.95	355.4	-0.45	0.741	0.15	2.00
295.80	296.3	-0.50	1.773	0.15	2.00
236.64	237.1	-0.46	2.804	0.15	2.00
177.48	177.9	-0.42	3.835	0.15	2.00
118.32	118.7	-0.38	4.867	0.15	2.00
59.16	59.6	-0.44	5.898	0.15	2.00
0.00	0.4	-0.40	6.930	0.15	2.00
-59.16	-58.8	-0.36	7.961	0.15	2.00
-118.32	-117.9	-0.42	8.992	0.15	2.00
-177.48	-177.1	-0.38	10.024	0.15	2.00
-236.64	-236.3	-0.34	11.055	0.15	2.00
-295.80	-295.5	-0.30	12.087	0.15	2.00
-354.95	-354.6	-0.35	13.118	0.15	2.00
-414.11	-413.8	-0.31	14.149	0.15	2.00

END OF CALIBRATION REPORT PAGE 2 OF 3





# QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23E8494

PAGE : 3 OF 3

## Calibration Report

### RESULT OF CALIBRATION (CONTINUE) :

#### 2. DISPLAY UNIT WITH pH ELECTRODE S/N: 09081C6M

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.006	4.006	0.000	4.015	0.012	2.00
7.000	7.000	0.000	6.914	0.012	2.00
10.008	10.010	-0.002	9.996	0.014	2.00

#### 3. DISPLAY UNIT WITH TEMPERATURE

STANDARD READING (°C)	UUC READING (°C)	CORRECTION (°C)	VALUE BEFORE ADJUSTMENT	UNCERTAINTY OF MEASUREMENT (± °C)	COVERAGE FACTOR k
25.005	25.0	0.005	---	0.0085	2.00

#### 4. PERCENT SLOPE 100%

UUC : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230

Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TIS-TIS 17025  
CALIBRATION 0089  
CLC

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : CONDUCTIVITY METER  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : SEVEN COMPACT S230  
SERIAL NO. : C141708983/5821320179  
CLID. NO. : 272300452  
JOB CONTROL NO. : 240213016389  
CALIBRATION SERVICE : ☒ IN-LABORATORY ☐ ON-SITE

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24 ROAD, JOMPOL,  
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 13 February 2024

DATE OF ISSUED : 16 February 2024

The report of calibration shall not be reproduced except in full without approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Sechanart  
Calibration Engineer



Approved By :

16 February 2024

This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q24016389

F3-011-05/12-23

page 1 of 4



@dcalibration



## CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



## REPORT OF CALIBRATION

### FOR

NOMENCLATURE : CONDUCTIVITY METER  
MANUFACTURER : METTLER TOLEDO  
MODEL / TYPE : SEVEN COMPACT S230  
SERIAL NO. : C141708983/5821320179  
DATE OF CALIBRATION : 13 February 2024

#### ENVIRONMENT CONDITIONS :

Temperature :  $(25 \pm 2.5) ^\circ\text{C}$  Relative Humidity :  $(50 \pm 15) \% \text{ RH}$

#### PROCEDURE USED :

This instrument [ Conductivity Meter ] was calibrated under procedure No. **WI-305-130**. The calibration was performed by direct measurement with Certified Reference Material (CRM) and Reference Material (RM) .

This instrument [ Temperature ] was calibrated under procedure No. **WI-305-244**. The calibration was performed by Comparison with Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

1. Conductivity Solution , Hanna Product Code HI 7033L Lot Number 7830.
2. Potassium Chloride Solution ( nominal 1.41 mS/cm )
3. Potassium Chloride Solution ( nominal 12.8 mS/cm )
4. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
5. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03.
6. IPRT, ASL Model T100-250-1D S/N. L0193A-1-1.

Certificate No. Q24016389

F3-011-05/12-23

page 2 of 4



@clccalibration



## CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



#### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through Hanna instruments.  
Certificate No. 20F21 , Due Date June 2025 .
2. The measurements are traceable to International System of Units (SI) , through Sigma-Aldrich Canada Co.  
Certificate No. HC30595403 , Due Date 31 January 2026 .
3. The measurements are traceable to International System of Units (SI) , through Sigma-Aldrich Canada Co.  
Certificate No. HC20111554 , Due Date 30 September 2025.
4. The measurements are traceable to International System of Units (SI) , through Calibration Laboratory Co., Ltd.  
Certificate No. Q23136342, Due Date 20 December 2024.
5. The measurements are traceable to International System of Units (SI) , through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0203/67, Due Date 07 December 2024.
6. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).  
Certificate No. TT-0136-23, Due Date 12 December 2024.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 % .  
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q24016389

F3-011-05/12-23

page 3 of 4



@clccalibration





# CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : RECEIVED IN GOOD OPERATIONAL CONDITION

MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of Conductivity Meter.

## CALIBRATION DATA

### 1. Conductivity Solution Test @ 25°C

Standard Conductivity Solution	DUC Reading	Uncertainty of Measurement
*84.00 µS/cm	84.05 µS/cm [Cell Constant 0.548589]	± 1.00 µS/cm
1414.0 µS/cm	1415 µS/cm [Cell Constant 0.548589]	± 21.0 µS/cm
12.83 mS/cm	12.75 mS/cm [Cell Constant 0.548589]	± 0.19 mS/cm

Note. \* means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 91 of 138

### \*2. Temperature Result [ Probe Conductivity ]

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty ± (°C)
100	25.00	24.9	+0.10	0.07

Note. \* means Calibrations marked "Not TISI Accredited" in this Certificate have been included for completeness.

This report is valid for the above stated instrument/s only.

### End of Certificate ###

Certificate No. Q24016389

F3-011-05/12-23

page 4 of 4



## QUALITY CALIBRATION CO.,LTD.

235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

www.qcalibration.com



CERTIFICATE No : 24M2229  
REFERENCE No : 72448-3

PAGE : 1 OF 2

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE  
MANUFACTURER : SARTORIUS  
MODEL : BSA224S-CW  
SERIAL No : 36591843  
ID No : BA 09/61  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.  
CALIBRATION DATE : 08-Mar-24

APPROVED BY :  
ISSUED DATE : 14-Mar-24  
RECEIVED DATE : 08-Mar-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV 03



**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 24M2229

PAGE : 2 OF 2

**Calibration Report**

EQUIPMENT : DIGITAL BALANCE MODEL : BSA224S-CW  
MANUFACTURER : SARTORIUS S/N : 36591843  
ID No : BA 09/61 RECEIVED DATE : 08-Mar-24  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 08-Mar-24  
AMBIENT TEMPERATURE : 25°C  $\pm$  1°C RELATIVE HUMIDITY : 55 %RH  $\pm$  10 % RH

**CONDITION OF THIS RESULTS OF CALIBRATION**

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

**2. REFERENCE STANDARD INSTRUMENTS :-**

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-1-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

**RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT**

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	50.0000	0.0000	0.00012
100.0	100.0001	-0.0001	0.00019
200.0	200.0000	0.0000	0.00032

**5. OFF CENTER LOADING ERROR**

POINT	READING (g)
1	100.0000
2	100.0000
3	100.0000
4	100.0000
5	100.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

**QUALITY CALIBRATION CO.,LTD.**

235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160

Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

[www.qcalibration.com](http://www.qcalibration.com)

CERTIFICATE No : 24M2227

PAGE : 2 OF 2

**Calibration Report**

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU  
MANUFACTURER : METTLER TOLEDO S/N : 1126422905  
ID No : BA05/50 RECEIVED DATE : 08-Mar-24  
AIR PRESSURE : 1010mbar  $\pm$  1mbar CALIBRATION DATE : 08-Mar-24  
AMBIENT TEMPERATURE : 25°C  $\pm$  1°C RELATIVE HUMIDITY : 53 %RH  $\pm$  10 % RH

**CONDITION OF THIS RESULTS OF CALIBRATION**

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

**2. REFERENCE STANDARD INSTRUMENTS :-**

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-1-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

**RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT**


1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY ( $\pm$ g)
0.00	0.00000	0.00000	0.000065
0.02	0.02001	-0.00001	0.000065
0.10	0.10002	-0.00002	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	9.99994	0.00006	0.000070
20.00	20.00008	-0.00008	0.000078
50.00	50.0000	0.0000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0001	-0.0001	0.00022

**5. OFF CENTER LOADING ERROR**

POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA  
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR  $k=2$ , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT





QUALITY CALIBRATION CO.,LTD.  
235 Petchkasem 63/2 Road, Laksong, Bangkae, Bangkok 10160  
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584  
www.qcalibration.com



PAGE : 1 OF 2

CERTIFICATE No : 24M2227  
REFERENCE No : 72448-1

## Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE  
MANUFACTURER : METTLER TOLEDO  
MODEL : XS105DU  
SERIAL No : 1126422905  
ID No : BA05/50  
CONDITION AS RECEIVED : USED ITEM  
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.  
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,  
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.  
CALIBRATION DATE : 08-Mar-24

APPROVED BY :  
ISSUED DATE : 14-Mar-24  
RECEIVED DATE : 08-Mar-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF  
QUALITY CALIBRATION CO., LTD.

F-G010 REV 03



WO-02612424/2024

## MAINTENANCE AND TEST CERTIFICATE MODEL OPTIMA 5300DV

Customer : S.P.S.Consulting Service Co.,Ltd Date Tested: July 4, 2024  
Recommendation Recertification  
Address : 7 Soi Phaholyothin 24 Period 6 Months  
Paholyothin Road Recertification Due: January 4, 2025  
Jompol Chatuchak, Bangkok 1090 Date Last Certified: January 4, 2024  
User Name: K.Phenpha Vipasthawatt Visit Number: 1 of 2  
Phone: 083-9269252 PerkinElmer Phone: 02-719-6420 ext 206  
Fax: 02-513-4221 PerkinElmer Fax: 02-318-5597

CONFIGURATION TESTED		ACCESSORIES/COMPONENT NOT INCLUDED
MODEL	SERIAL NUMBER	
OPTIMA 5300DV	077C7042401	
TESTED EQUIPMENT	CALIBRATION NUMBER	EXPIRATION
IPV Methods		
TEST STANDARD USED	PART NUMBER	EXPIRATION DATE
Multielement Standard	N069-1579	December 30, 2024
Wavecal Solution	N058-2152	September 30, 2024
VIS Wavecal solution	N930-2946	January 30, 2025
Instrument Cal. STD4	N930-0221	November 30, 2024
CUSTOMER SUPPLIED	COMMENTS	CUSTOMER INITIALS
2 % HNO3		
10 % HNO3		

Page 1 of 4

PerkinElmer Scientific (Thailand) Co., Ltd.  
290 Soi Soonvijai 4, Bangkok, Huay Kwang, Bangkok 10310 Head Office



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>SERIAL NUMBER</b>	077C7042401	<b>DATE TESTED</b>	July 4, 2024
<b>1. MECHANICAL CHECKS</b>			
A. Inspect and clean all fans and filters.	<input type="text" value="OK"/>		
B. Inspect and replace as necessary, all torch components including the RF coil.	<input type="text" value="OK"/>		
C. Inspect all tubing for sign of clacking or leaking.	<input type="text" value="OK"/>		
D. Adjust water and gas pressure regulator settings.	<input type="text" value="OK"/>		
E. Inspect and leak check pneumatics drawers.	<input type="text" value="OK"/>		
F. Clean the exterior of the instrument.	<input type="text" value="OK"/>		
<b>2. OPTICAL CHECKS</b>			
A. Inspect and clean all optical components.	<input type="text" value="OK"/>		
B. As required, check and replace all purgefilters.	<input type="text" value="OK"/>		
C. Recheck optical alignment.	<input type="text" value="OK"/>		
<b>3. COOLING SYSTEM CHECKS</b>			
A. Perform preventive maintenance on chiller.	<input type="text" value="OK"/>		
B. Flush out the chiller every year.	<input type="text" value="N/A"/>		
<b>4. PERFORMANCE CHECKS</b>			
A. Torch View Alignment.	<input type="text" value="OK"/>		
B. Wavelength Calibration.	<input type="text" value="OK"/>		



## MAINTENANCE AND TEST CERTIFICATE MODEL

### OPTIMA 5300DV

<b>SERIAL NUMBER :</b> 077C7042401		<b>DATE TESTED :</b> July 4, 2024	
<b>PARAMETER</b>	<b>SPECIFICATION</b>		<b>FINAL VALUE</b>
<b>Spectral Resolution : UV</b>	As 193.696 nm	≤ 0.007	0.00550
	Ni 231.604 nm	≤ 0.008	0.00714
	Ni 341.476 nm	≤ 0.012	0.00790
<b>Spectral Resolution : VIS</b>	La 408.672 nm	≤ 0.020	0.01655
	Ba 455.403 nm	≤ 0.025	0.02391
<b>Precision</b>	As 193.656 nm	% RSD < 1.0	0.72 %
	Zn 213.856 nm	% RSD < 1.0	0.66 %
	Mn 257.610 nm	% RSD < 1.0	0.30 %
	La 379.478 nm	% RSD < 1.0	0.98 %
	Ba 455.403 nm	% RSD < 1.0	0.95 %
	Ba 493.408 nm	% RSD < 1.0	0.78 %
<b>Detection Limits : Axial</b>	Tl 190.080 nm	3(sd)	6.22 ppb
	As 193.696 nm	3(sd)	6.44 ppb
	Pb 220.353 nm	3(sd)	2.06 ppb
<b>Detection Limits : Radial</b>	As 193.696 nm	3(sd)	78.26 ppb
	Zn 213.856 nm	3(sd)	2.07 ppb
	Mn 257.610 nm	3(sd)	0.52 ppb
	La 379.478 nm	3(sd)	2.63 ppb
	Ba 455.403 nm	3(sd)	0.08 ppb
	Ba 493.408 nm	3(sd)	0.75 ppb
<b>BEC : Axial (1B X 500)/(1S-1B)</b>	Cd 226.502 nm	≤ 150 ppb	64.72
<b>BEC : Radial (1B X 1000)/(1S-1B)</b>	Mn 257.610 nm	≤ 45 ppb	15.04



**MAINTENANCE AND TEST CERTIFICATE MODEL**  
**OPTIMA 5300DV**

**SERIAL NUMBER** 077C7042401 **DATE TESTED** July 4, 2024

**Remarks :**

Commissioning follow as commissioning performance sheets.

---

---

---

---

---

---

---

---

This is to certify that the above tests have been performed and the configuration tested

☒

meets

☐

does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale,  
including warranty terms.

**Authorized Representative**

