

ภาคผนวก ง

เอกสารการสอบเทียบเครื่องมือตรวจวิเคราะห์



DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	8 Jan 24	Ambient Temperature (°C)	27.3		
Calibration sheet No. : C-080124-BKK_FS0469		Relative Humidity (%) :	35		
Digital Temperature ID : BKK_FS0469		Reference Temperature ID	RYG_FS0681		
Serial No. : 1302005		Serial No. :	201090014918		
Model : XC-572-V		Model :	Digicon-CC-VT-MS		
		Next Calibrate :	13 Nov 24		
Location	Reference Temperature °C	Digital Temperature °C	Error °C	MPE	Pass / Fail
Stack	0	0	0	±3	Pass
	25	24	-1	±3	Pass
	50	49	-1	±3	Pass
	100	101	1	±3	Pass
	150	150	0	±3	Pass
	200	200	0	±3	Pass
	250	250	0	±3	Pass
Probe	300	300	0	±3	Pass
	500	501	1	±3	Pass
	100	101	1	±3	Pass
	120	120	0	±3	Pass
	140	140	0	±3	Pass
	100	100	0	±3	Pass
	120	121	1	±3	Pass
Oven	140	141	1	±3	Pass
	100	102	2	±3	Pass
	120	121	1	±3	Pass
Filter	140	141	1	±3	Pass
	0	0	0	±3	Pass
	10	9	-1	±3	Pass
Exit	20	19	-1	±3	Pass
	0	-1	-1	±3	Pass
	25	24	-1	±3	Pass
Meter	50	48	-2	±3	Pass
	0	0	0	±3	Pass
	25	24	-1	±3	Pass
AUX	50	49	-1	±3	Pass

MPE : (Maximum permissible error of measurement) ค่าความผิดพลาดสูงสุดของการวัดที่อนุญาต

Calibrated by :

Saksit Phaisanphiset

(Mr. Saksit Phaisanphiset)

RYG Field Service Scientist (4)

Approved by :

Natthapol Jengwareewong

(Mr.Natthapol Jengwareewong)

RYG Field Service Specialist (1)

FORM NO.: F 06-027 REVISION NO.: 2 ISSUE DATE: 16/2/23



PROBE NOZZLE DIAMETER CALIBRATION DATA SHEET


Calibration Date : 8 Jan 24		Nozzle Set ID. : BKK_FS0474			
Calibration Sheet No. : C-080124-BKK_FS0474		Vernier Caliper ID. : BKK_FS1123			
Nozzle ID #	Nozzle Diameter (cm.)			Hi - Lo	(D ₁ + D ₂ + D ₃) / 3
	D ₁	D ₂	D ₃	ΔD	D _{avg}
1	0.305	0.300	0.305	0.005	0.303
2	0.455	0.455	0.455	0.000	0.455
3	0.604	0.602	0.601	0.003	0.602
4	0.760	0.765	0.770	0.010	0.765
5	0.935	0.945	0.935	0.010	0.938
6	1.095	1.098	1.092	0.006	1.095
7	1.260	1.260	1.260	0.000	1.260
8	1.605	1.600	1.610	0.010	1.605

Where :

D₁, D₂, D₃ = There different nozzle diameters at 60 degrees to each other, each measured the nearest 0.025 mm.

ΔD = Maximum distance between any two diameters, must be ≤ 0.100 mm.

D_{avg} = (D₁ + D₂ + D₃) / 3



Calibrated by :

Saksit Phaisanphiset

(Mr. Saksit Phaisanphiset)

Field Scientist (4)

Approved by :

Natthapol Jengwareewong

(Mr.Natthapol Jengwareewong)

Field Specialist (1)

FORM NO.: F 06-028 REVISION NO.: 1 ISSUE DATE: 16/1/23



DRY GAS METER CALIBRATION TEST REPORT

Calibration of Date 8-Jan-24 Barometric Pressure (mm.Hg) : 755.3
Next Calibration Date 8-Jul-24 Relative Humidity (%) : 35.0
Temperature (°C) : 27.3

Dry Gas Meter Data

Calibration sheet No. : C-080124-BKK_FS0465
Dry Gas Meter ID BKK_FS0465
Serial No. 1302005
Model No. XC-60C-V

Reference Dry Gas Meter Data

Reference Dry Gas Meter ID : BKK_FS1122
Serial No. : A2003240
Correction Factor (Y) : 0.9824
Next Calibration Date : 7 Nov 24

Reference Dry Gas Meter Calibration				Dry Gas Meter							Dry Gas Meter
Vr (Liters)			Tr	Vm (Liters)			Ti	To	Avg. Tm	Correction	
Final	Initial	Total	(°C)	Final	Initial	Total	(°C)	(°C)	(°C)	Factor (Y)	
30.00	0.00	30.00	28.0	29.03	0.00	29.03	25.0	25.0	25.0	1.0052	
30.00	0.00	30.00	28.0	29.04	0.00	29.04	25.0	25.0	25.0	1.0048	
60.00	0.00	60.00	28.0	60.42	0.00	60.42	25.0	25.0	25.0	0.9659	
60.00	0.00	60.00	28.0	60.42	0.00	60.42	25.0	25.0	25.0	0.9658	
90.00	0.00	90.00	27.0	91.48	0.00	91.48	25.0	25.0	25.0	0.9601	
90.00	0.00	90.00	27.0	91.49	0.00	91.49	25.0	25.0	25.0	0.9600	
Avg.										0.9770	

Y = Ratio of reading of reference dry gas meter to dry gas meter ; tolerance for individual ± 0.05 from average.

Calibrate by :

Jittakorn

Mr. (Jittakorn.sriwasa)
RYG Field Service Scientist (2)

Approved by :

Natthapol Jengwareewong

Mr.(Natthapol Jengwareewong)
RYG Field Service Specialist (1)

FORM NO.: F 06-023 REVISION NO.: 1 ISSUE DATE: 30/6/22



Stopwatch Calibration Test Report

Calibration Date : 8 Jan 24 Next Cal. Date : 8 Jul 24
Barometric Pressure (mmHg) : 755.3 Temperature (°C) : 27.3
Relative Humidity (%) : 35.0

Reference Stopwatch Data

Stopwatch ID No. : E18061
Model : F808
Serial No. : -
Calibration Date : 8 Sep 20
Certificate No. : E-2009018

Console Control Meter Data

Dry Gas Meter No. : BKK_FS0465
Model : XC-60C-V
Serial No. : 1302005

Run No.	Time Actual (m:ss.ms)	Time Reading (m:ss)	Diff. (ms)	Diff. (min)
1	5:00:03	5:00	3	0.00005
2	5:00:09	5:00	8	0.00013
3	5:00:09	5:00	9	0.00015
4	5:00:11	5:00	11	0.00018
5	5:00:05	5:00	5	0.00008
6	5:00:06	5:00	6	0.00010
7	5:00:06	5:00	6	0.00010
8	5:00:08	5:00	8	0.00013
9	5:00:09	5:00	9	0.00015
10	5:00:07	5:00	7	0.00012
Average				0.00012
SD				0.00004

Calibrate by :

Saksit Phaisanphiset

Mr. Saksit Phaisanphiset

RYG Field Service Scientist (4)

Approved by :

Natthapol Jengwareewong

Mr.Natthapol Jengwareewong

RYG Field Service Specialist (1)



DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date :	8 Jan 24	Ambient Temperature (°C)	27.3
Calibration sheet No. : C-080124-BKK_FS0467		Relative Humidity (%) :	35
Digital Temperature ID : BKK_FS0467		Reference Temperature ID	RYG_FS0681
Serial No. : 1302005		Serial No. :	201090014918
Model : XC-572-V		Model :	Digicon-CC-VT-MS
		Next Calibrate :	13 Nov 24

Location	Reference Temperature °C	Digital Temperature °C	Error °C	MPE	Pass / Fail
Stack	0	0	0	±3	Pass
	25	24	-1	±3	Pass
	50	49	-1	±3	Pass
	100	99	-1	±3	Pass
	150	151	1	±3	Pass
	200	201	1	±3	Pass
	250	251	1	±3	Pass
	300	301	1	±3	Pass
	500	501	1	±3	Pass
	100	99	-1	±3	Pass
Probe	120	121	1	±3	Pass
	140	141	1	±3	Pass
Oven	100	101	1	±3	Pass
	120	121	1	±3	Pass
Filter	140	141	1	±3	Pass
	100	99	-1	±3	Pass
	120	121	1	±3	Pass
	140	141	1	±3	Pass
Exit	0	0	0	±3	Pass
	10	9	-1	±3	Pass
	20	19	-1	±3	Pass
Meter	0	0	0	±3	Pass
	25	24	-1	±3	Pass
AUX	50	49	-1	±3	Pass
	0	0	0	±3	Pass
	25	24	-1	±3	Pass
	50	49	-1	±3	Pass

MPE : (Maximum permissible error of measurement) ค่าความผิดพลาดสูงสุดของการวัดที่อนุญาต

Calibrated by :

Jittakorn

(Mr.Jittakorn.Srivasa)
Enviro Field Service Scientist (2)

Approved by :

Nattapon Jengwareewong

(Mr.Nattapon Jengwareewong)
Enviro Field Service Specialist (1)


FORM NO.: F 06-027 REVISION NO.: 2 ISSUE DATE: 16/2/23



Type S Pitot Tube Calibration

Date Calibration 8-Jan-24
Pitot ID BKK_FS0473
Pitot SN -

Due Date 8-Jul-24
Inclinometer ID BKK_FS1131
Vernier ID RYG_FS0539



Parameter	Value	Allowable Range	Check
α1	2.5	-10° < α1 < +10°	OK
α2	1.4	-10° < α2 < +10°	OK
β1	-0.8	-5° < β1 < +5°	OK
β2	-0.4	-5° < β2 < +5°	OK
γ	0.3	-	-
θ	0.2	-	-
Z = A tan γ	0.005	Z ≤ 0.125"	OK
W = A tan θ	0.003	W ≤ 0.031"	OK
Dt	0.310	0.188" to 0.375"	OK
A/2Dt	1.484	1.05 ≤ PA/Dt ≤ 1.5	OK
A	0.92	2.1Dt ≤ A ≤ 3Dt	OK

Certify that pitot tube/porbe meets or exceeds all specifications, criteria and/or applicable design features and is hereby assigned a pitot tube certification fact of 0.84 . See 40 CFR Pt. 60, App. A, EPA Method 2.

Calibrated by :

Saksit Phaisanphit
(Mr. Saksit Phaisanphit)
RYG Field Services Scientist (4)

Approved by :

Nattapon Jengwareewong
(Mr.Nattapon Jengwareewong)
RYG Field Services Specialist (1)

FORM NO.: F 06-124 REVISION NO.: 0 ISSUE DATE: 25/12/23



Calibration Certificate



Certificate No: G 670124
Date of issue : 22-Feb-24

Instrument description : Flue Gas Analyzer
Instrument model : Testo 340
Control unit serial no. : -
Instrument serial no. : 62150585
ID no. or control no. : RYG_FS0465
Manufacturer : Testo SE & Co. KGaA
Probe description : -
Probe model : -
Probe serial no. : -
Customer name : ALS LABORATORY GROUP (THAILAND) CO.,LTD.
Customer address : 104 Phatthanakan 40, Phatthanakan Road, Khwaeng Phatthanakan, Khet Suan Luang, Bangkok, 10250 Thailand
Total pages of certificate : 2 Pages
Receiving no. : L-240604
Receiving date. : 19-Feb-24
Parameter of calibration : Gas Calibration(Oxygen 2.50,10.04,21.02 %vol, Carbon Monoxide 80.14,302,1003 ppm)
Nitric Oxide 30.01,151.5,322.5 ppm, Sulphur Dioxide 50.36,100.8,600.8 ppm)
Condition of UUC. : Used
Ambient condition : All of the Measurement were carried out the stabilized laboratory
Temperature : 23 ±5 °C
Humidity : 55 ± 15 %RH
Calibration place : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210
Calibration procedure no. : This instrument was calibrated by comparison with Standard gas mixture according to calibration Work Instruction no. WI-CL-28-C



The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.
This certificate is applied only to item under test Environmental condition.
This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory.
Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.
This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).
Date of calibration : 22-Feb-24

Kwanthai
Mr. Kwanthai Khamsoung
Calibration Technician

Nattapon
Mrs. Nongluck Wongsettee
Technical Manager



Calibration Certificate



Certificate No.: G 670124

Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen (O2) 2.50 % Vol	2412/23	Linde	27-Aug-27
Oxygen (O2) 10.04 % Vol	CG-0153-21	Nimrt	18-Nov-26
Oxygen (O2) 21.02 % Vol	CG-0041-22	Nimrt	10-Feb-27
Carbon monoxide (CO) 80.14 ppm	CG-0040-22	Nimrt	14-Feb-27
Carbon monoxide (CO) 302 ppm	1915/23	Linde	16-Jun-25
Carbon monoxide (CO) 1003 ppm	2584/23	Linde	10-Sep-25
Nitric Oxide (NO) 30.01 ppm	CG-0014-23	Nimrt	19-Feb-25
Nitric Oxide (NO) 151.5 ppm	0161/23	Linde	22-Jan-25
Nitric Oxide (NO) 322.5 ppm	1974/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 50.36 ppm	2004/23	Linde	17-Jul-25
Sulphur Dioxide (SO2) 100.8 ppm	3501/22	Linde	09-Nov-24
Sulphur Dioxide (SO2) 600.8 ppm	2003/23	Linde	17-Jul-25

Measured room conditions

Temperature : 22.7 °C Humidity : 60.2 %RH Pressure : 1011.8 mbar

Calibration conditions

Gas Temperature : 23 °C Flow rate : 600 ml/min Gas pressure : 1014.1 mbar

Calibration Results (Without adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (+)
O2 (%Vol)	2.50	2.44	-0.06	0.15
O2 (%Vol)	10.04	9.92	-0.12	0.30
O2 (%Vol)	21.02	21.11	0.09	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	302	303	1	6.0
CO (ppm)	1003	1003	0	12
NO (ppm)	30.01	29	-1.01	8.0
NO (ppm)	151.5	151	-0.5	8.0
NO (ppm)	322.5	321	-1.5	12
SO2 (ppm)	50.36	52	1.64	6.0
SO2 (ppm)	100.8	102	1.2	6.0
SO2 (ppm)	600.8	604	3.2	13

Remark : 1 cmol/mol = 1 %vol, 1 μmol/mol = 1 ppm.

End of Report



SARTORIUS

Certificate of Calibration

REVIEW BY: Thawit
APPROVED BY: [Signature]
NEXT CAL. DATE: 02/02/2025

Model Number: MSU224S-100-DU Certificate No.: 24BCI0073
Description: Analytical Balance Issued Date: Friday, February 23, 2024
Serial Number: 0031709552 Reference No.: 229196
ID No.: RYG_EN0003
Manufacturer: Sartorius Page No.: 1 of 2

Customer Name: ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place: ALS Laboratory Group (Thailand) Co., Ltd. (Balance Room)
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated By: Mr.Chonchai Inthana
Calibration Date: Thursday, February 22, 2024

Metrological data:
Capacity: 220 g Readability: 0.0001 g
Reasons for calibration:
☐ New Installation ☐ Service / Repair ☒ Re-calibration/ Maintenance
Calibration Procedure No.: This calibration was conducted by Using in-house calibration procedure number (WI-003) Based on UKAS LAB 14 : 2019
Ambients Conditions:
Temperature: 23.7 °C ± 5.0 °C
Humidity: 62.0 % RH ± 10.0 % RH
Pressure: ±
Equipment Condition: ☒ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref : Lab 14
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	TCS	M2308197S	23-Aug-2025
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C1923184S	23-Aug-2024

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

[Signature]

Mr.chonchai inthana(Technical Manager)



SOP FM 33 03 February 2022

SARTORIUS

Certificate of Calibration

Model Number: MSU224S-100-DU Certificate No.: 24BCI0073
Description: Analytical Balance Issued Date: Friday, February 23, 2024
Serial Number: 0031709552 Reference No.: 229196
ID No.: RYG_EN0003
Manufacturer: Sartorius Page No.: 2 of 2

Calibration Results : Without Adjustment

Repeatability			Eccentricity (Off-center loading error)		
The reproducibility is the ability of a weighing instrument to display nearly identical readings under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.			The off-center loading error is yielded by the difference between the readout of the load, i.e. 10 or 1% of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).		
Nominal Value : (Low Load)	20.0000	200.0001	Nominal value :	100	g
20 g	20.0000	200.0000	Tolerance	0.0004	g
Tolerance	20.0001	200.0001	Difference		
0.0001 g	20.0000	200.0001	1		
	20.0000	200.0001	2		
	20.0000	200.0001	3		
	20.0000	200.0001	4		
Nominal Value : (High Load)	20.0000	200.0001	5		
200 g	19.9999	200.0001	6		
Tolerance	20.0000	200.0000			
0.0001 g	20.0000	200.0000			
	20.0000	200.0001			
Standard Deviation	0.00005	0.00005			

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance	0.0002	g		
Nominal Value	Conventional Mass Value	Displayed Value	Deviation	Uncertainty
(g)	(g)	(g)	(g)	(g)
0.01	0.0100	0.0100	0.0000	0.00013
0.1	0.1000	0.1000	0.0000	0.00013
0.5	0.5000	0.5000	0.0000	0.00013
1	1.0000	1.0000	0.0000	0.00013
5	5.0000	5.0000	0.0000	0.00013
10	10.0000	10.0000	0.0000	0.00013
20	20.0000	20.0000	0.0000	0.00013
50	50.0000	50.0000	0.0000	0.00024
100	100.0000	99.9999	-0.0001	0.00018
200	200.0000	199.9999	-0.0001	0.00029

End of Report.

SOP FM 33 03 February 2022



CALIBRATION LABORATORY CO., LTD.

2110-11,14,35 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : QUALITYWELL
MODEL / TYPE : N/A
SERIAL NO. : VG01[RYG_FS0332]
CLID. NO. : 212300695
JOB CONTROL NO. : 230329034806

REVIEW BY: Mongkol P
APPROVED BY: [Signature]
NEXT CAL. DATE: 30/9/24

CUSTOMER : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTANAKAN 40, PHATTANAKAN RD.,
KHWAENG PHATTANAKAN, KHET SUAN LUANG, BANGKOK 10250, THAILAND

DATE OF RECEIVED : 29 March 2023 DATE OF ISSUED : 31 March 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By: Sittipong Pimdee
Calibration Engineer

[Signature]

Approved By: Mongkol Yotsoontorn
Authorized Signatory
31 March 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23034806

F3-011-04/01-12

page 1 of 3



CALIBRATION LABORATORY CO., LTD.

2110-11,14,35 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



REPORT OF CALIBRATION

FOR

NOMENCLATURE : VACUUM GAUGE
MANUFACTURER : QUALITYWELL
MODEL / TYPE : N/A
SERIAL NO. : VG01[RYG_FS0332]
DATE OF CALIBRATION : 30 March 2023

ENVIRONMENT CONDITIONS :

Temperature : (23 ± 2) °C Relative Humidity : (55 ± 10) %RH

PROCEDURE USED :

This instrument was calibrated under procedure No. CLC-CPPP-05 according to DKD-R 6-1 as calibration guidelines.
The calibration was performed by direct measurement with Document Process Calibrator and Pressure Module which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Document Process Calibrator, Fluke Model 741B S/N. 8295020 with Pressure Module Model 700PD5 S/N. 89404505.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. MP-0035-23, Due Date 02 February 2024.

UNCERTAINTY :

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor of $k = 2$. It has been evaluated according to the "Calibration of Pressure Gauges (DKD-R 6-1)" which provides a level of confidence approximately 95%.

Certificate No. Q23034806

F3-011-04/01-12

page 2 of 3





CALIBRATION LABORATORY CO., LTD.

2/10-11/14, 55 Soi Prasert Mansuk 29 Yaek 4, Prasert Mansuk Rd., Ladphrao, Bangkok 10230
Tel: 02-578-0353-4 Fax: 02-578-2672 www.cai-laboratory.com E-mail: sale@cai-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC was exercised by applying a known pressure from its zero to full scale 1 times. Then 2 series of known gauge pressure were applied. The STD reading were recorded and the means value were reported in the table below.

CALIBRATION DATA

CORRECTION OF PRESSURE

DUC Test point (inHg)	STD Reading (inHg)		Correction (inHg)	
	Up	Down	Up	Down
-10.0	-9.75	-9.76	+0.25	+0.24
-20.0	-19.90	-19.91	+0.10	+0.09
-26.0	-26.02	-26.03	-0.02	-0.03
-27.0	-27.04	-27.05	-0.04	-0.05
-28.0	-28.05	-28.05	-0.05	-0.05

Uncertainty of measurement ± 0.06 inHg

Transmitting fluid : Air.

Note: The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 36 of 54

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23034806

F3-011-0401-12

page 3 of 3



Certificate of Calibration

Equipment: SPECTROPHOTOMETER
Model: DR6000
Serial No. (or ID.): 1627845 (RYG_EN0037)
Manufacturer: HACH
Condition: In Condition

Certificate No.: C06230441
Issued Date: 19 September 2023
Job No.: WO-00005382
Page: 1 of 3

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu,
A.Pluaekdaeng, Rayong 21140, Thailand.

Environment Condition: Temperature 23.9 °C ± 0.2
Humidity 65.3 %RH ± 1.4

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) (Wet Chemistry)
616/10 Moo 5 T.Maenam Khu,
A.Pluaekdaeng, Rayong 21140, Thailand.

Calibration By: Mr.Nattapat Rungreueang

Calibration Date: 18 September 2023

The Method used: In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

Traceability: This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 111583 and 111584
The standard for Photometric Certificate No. 9114984 and 111588
The standard for Stray light Certificate No. 111586 and 111585
The standard for Spectral resolution Certificate No. 111587

(Mr. Nattapat Rungreueang)

Person in charge

(Mr. Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items listed, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Thailand 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C06-15: 12 Sep 2022



Certificate No.: C06230441

Page 2 of 3

Calibration Results: Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.3	0.31	0.13
536.66	536.6	0.06	0.13
637.98	638.3	-0.32	0.13
748.48	748.7	-0.22	0.13
807.03	807.4	-0.37	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2930	0.289	0.0040	0.0045
	0.5168	0.519	-0.0022	0.0045
	1.0298	1.029	0.0008	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2867	0.283	0.0037	0.0045
	0.5073	0.509	-0.0017	0.0045
	1.0083	1.007	0.0013	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2516	0.250	0.0016	0.0045
	0.4595	0.462	-0.0025	0.0045
	0.9334	0.933	0.0004	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2461	0.245	0.0011	0.0045
	0.4652	0.466	-0.0008	0.0045
	0.9468	0.946	0.0008	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2594	0.259	0.0004	0.0045
	0.5040	0.505	-0.0010	0.0045
	1.0032	1.002	0.0012	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2579	0.257	0.0009	0.0045
	0.4971	0.497	0.0001	0.0045
	0.9720	0.971	0.0010	0.0045

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Thailand 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C06-15: 12 Sep 2022



Certificate No.: C06230441

Page 3 of 3

Calibration Results: Without Adjustment

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7355	0.737	-0.0015	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8574	0.857	0.0004	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2864	0.290	-0.0036	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6374	0.637	0.0004	0.0080

Stray light *

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.62 +/- 0.11 nm	260.6	1.3	1.886
391.44 +/- 0.11 nm	391.4	1.3	1.886

Spectral Resolution *

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength (nm)	268.66	266.69	1.38	2.00
UUC: Wavelength (nm)	268.2	266.1		
Std Absorbance (A)	0.4566	0.2780		
Absorbance (A)	0.413	0.300		

* Calibration Marked * Not TISI Accredited * in this Certificate have been included for completeness.

The End of Certificate

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Thailand 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C06-15: 12 Sep 2022



ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-0005382

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: DR6000

หมายเลขเครื่อง: 1627845

ตรวจสอบ (วัน)		รายการตรวจเช็ค	ตรวจสอบ (ตั้ง)		หมายเหตุ
18 Sep 2023			18 Sep 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด – เปิด เครื่อง (On-Off Switch)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	*
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	9.2 Hours
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	741.5 Hours
<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. ช่องจัดหลายตัวอย่าง (Carousel Module)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด (Electrode and Connection Cable)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาตั้งอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความทึบที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่นเกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Pison Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

เส้นผ่านศูนย์กลาง: *656.1mm=656.1mm

*486.0mm=485.5mm

Mr.Nattapat Rungueang
Service Engineer

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangkok, Thailand 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-R31-03: 20 Jul 2022



DRY GAS METER CALIBRATION TEST REPORT

Calibration of Date : 4 Apr 24
Next Calibration Date 3 Oct 24

Barometric Pressure (mm.Hg) : 757
Relative Humidity (%) : 35.0
Temperature (°C) : 32.0

Dry Gas Meter Data

Calibration sheet No.: C-040424-BKK_FS0525
Dry Gas Meter No.: BKK_FS0424
Console Serial No.: 20151402
Model No.: XC-60B-V

Reference Dry Gas Meter Data

Reference Dry Gas Meter ID.: BKK_FS0629
Serial No.: 1607009
Correction Factor (Yr): 1.0000
Next Calibration Date : 9 Jun 24

Reference Dry Gas Meter Calibration				Dry Gas Meter							Dry Gas Meter Correction Factor (Y)
Vr (Liters)			Tr (°C)	Vm (Liters)			Ti (°C)	To (°C)	Avg. Tm (°C)		
Final	Initial	Total		Final	Initial	Total					
30.00	0.00	30.00	31.0	30.91	0.00	30.91	31.0	31.0	31.0	0.9707	
30.01	0.00	30.01	31.0	30.91	0.00	30.91	31.0	31.0	31.0	0.9708	
60.02	0.00	60.02	32.0	61.76	0.00	61.76	31.0	31.0	31.0	0.9687	
60.02	0.00	60.02	32.0	61.76	0.00	61.76	32.0	32.0	32.0	0.9718	
90.02	0.00	90.02	32.0	92.67	0.00	92.67	33.0	33.0	33.0	0.9746	
90.01	0.00	90.01	33.0	92.63	0.00	92.63	34.0	34.0	34.0	0.9749	
									Avg.	0.9719	

Y = Ratio of reading of reference dry gas meter to dry gas meter ; tolerance for individual \pm 0.02 from average.

Calibrate by :

Mr. Apisit Sing-ha

Approved by :

Mr. Samart Roo-ngan

Mr.Apisit Sing-ha
Field Scientist (4)

Mr.Samart Roo-ngan
Specialist (1)

FORM NO.: F-06-027 REVISION NO.: 1 ISSUE DATE: 2022/01



DIGITAL TEMPERATURE CALIBRATION DATA SHEET

Calibration Date : 4 Apr 24		Ambient Temperature (°C) 32			
Calibration sheet No. : C-040424-BKK_FS0424		Relative Humidity (%) : 35			
Digital Temperature ID : BKK_FS0424		Reference Temperature ID BKK_FS1144			
Serial No. : 6011003		Serial No. : 201090006013			
Model : XC-60B-V		Model : Digicon-CC-VT-MS			
Next Calibrate :		14 Oct 24			
Location	Reference Temperature °C	Digital Temperature °C	Error °C	MPE	Pass / Fail
Stack	0	0	0	±3	Pass
	25	24	-1	±3	Pass
	50	50	0	±3	Pass
	100	101	1	±3	Pass
	150	152	2	±3	Pass
	200	202	2	±3	Pass
	250	252	2	±3	Pass
Probe	300	303	3	±3	Pass
	500	503	3	±3	Pass
	100	101	1	±3	Pass
	120	122	2	±3	Pass
	140	142	2	±3	Pass
	100	-	-	±3	-
	120	-	-	±3	-
Filter	140	-	-	±3	-
	100	102	2	±3	Pass
	120	122	2	±3	Pass
Exit	140	142	2	±3	Pass
	0	0	0	±3	Pass
	10	10	0	±3	Pass
Meter	20	21	1	±3	Pass
	0	0	0	±3	Pass
	25	26	1	±3	Pass
AUX	50	50	0	±3	Pass
	0	0	0	±3	Pass
	25	24	-1	±3	Pass
	50	50	0	±3	Pass

MPE : (Maximum permissible error of measurement) ค่าความผิดพลาดสูงสุดของการวัดที่อนุญาต

Calibrated by :

Mr. Apisit Sing-ha

(Mr.Apisit Sing-ha)
Field Scientist (4)

Approved by :

Mr. Samart Roo-ngan

(Mr.Samart Roo-ngan)
Specialist (1)

FORM NO.: F-06-027 REVISION NO.: 2 ISSUE DATE: 9 Feb 23



Certificate of Calibration

ICS-2100: Anion (ID#659)

This certificate is to verify that instrument below are calibrated

by Archemica Lab Co., Ltd.

ICS-2100 S/N: 15010977

AS-HV S/N: 5450A36659

For

ALS Laboratory Group (Thailand) Co., Ltd.



Operator Signature: *Nutdanai*

Date: Jan 12, 2024

(Mr.Nutdanai Laekhwan)

Application Chemist



Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A.D
968 RAMA 4 ROAD, SILOM, BANGRAK
Bangkok 10500 Thailand

Tel: +662 637 6363
Fax: +662 632 4334
Email: ccc-smt@agilent.com
Website: www.agilent.com/thai

Service Confirmation Number: 6904800024
Service Confirmation Date: 20.03.2023

Customer Contact:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan
TAX ID : 0105540004859
Chanattagarn.lmchom@alsglobal.com
27603068

Invoice To:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Delivery Site:


ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Location:

Room
Bldg
Lab
Dept

SERVICE REPORT

Customer Purchase Order Number:	Customer Number: 70371013
Service Request:	Service Request Date:
Service Order: 6006033911	Service Confirmation: 6904800024



Direct Inquiries to:

Contact Name: Customer Contact Center
Contact E-mail: ccc-smt@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

products | applications | software | services

Learn more about Agilent's Special Offers, Products, Services and our
full range of laboratory productivity solutions optimized for your
applications and workflows. Visit us at www.agilent.com/thai

Agilent Technologies (Thailand) Limited, Head Office
U Chu Liang Bldg. 22/F Unit A.D
968 Rama 4 Road, Silom, Bangkok,
Bangkok 10500 Thailand
Tax ID : 0105540004859

Citibank N.A. Bangkok Branch
399 Interchange 21 Building, Sukhumvit Road, Klongtoey New
Sub-district, Wattana District, Bangkok 10110 Thailand
Acc. No: 912-4452-007
TIBK/King Thai Bank PCL
Siam Square Bldg., 416/1-2 Rama 1 Rd., Pathumwan, BKK 10339
Thailand

ORIGINAL

Service Instrument:

Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-ID-5100	ICP-OES 5100/S110 System			
G8010A	Agilent 5100 SVDV ICP-OES Spectrometer	MY16010005	ICP OES 5100	SYS-ID-5100
G8410A	SPS 4 Autosampler	AU15440764	ICP OES 5100	SYS-ID-5100

Service Rems:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EQO	Enterprise Operational Qualification	1.00	Agreement Entitlement - 100 % covered	20.03.2023	20.03.2023

Additional Information:

Service Confirmation Number: 6904800024
Service Confirmation Date: 20.03.2023

Service Information:


Problem Description: WU-S-QQ-ID-5100-6001143313		
Service Provided: Complete OQHW 5100ICPOES Equipment ID: BKK_EL0037, all tests passed		
Service Overview Code: Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
Reported Hours: 4.0	Travel Hours: 2.0	
Customer Field Service Representative Name: Kanyakorn Sukphatjarern	Customer Field Service Representative Signature: 	Date: 20 Mar 2023
Customer Name: Thirima Boonpeng	Customer Signature: 	Date: 20 Mar 2023
Additional Comments:		



High Volume Air Sampler Calibration Worksheet

Project Site:	Sumiden Steel Wire (Thailand) Co., Ltd.	Barometric Pressure (mm Hg):	754
Calibrate Location:	บึง 5 ไร่ (A1)	Temperature (°C):	29
Calibrate Date:	23-May-24	High Volume ID:	RYG-FS0397
Calibration Sheet No.:	C-230524-RYG-FS0397	High Volume Model:	TE-5009X
Calibrator ID:	RYG-FS0205	High Volume S/N:	5687
Calibrator Model:	TE-5028A	Calibrator Slope:	0.95561
Calibrator S/N:	1166	Calibrator Intercept:	-0.02266

Test No.	Delta H ₂ O (inch)	Qa (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.8	0.911	30	Slope: 46.4729
2	2.2	1.005	34	Intercept: -12.4645
3	2.8	1.131	40	Correlation Coefficient: 0.9996
4	3.2	1.207	44	
5	4.0	1.347	50	

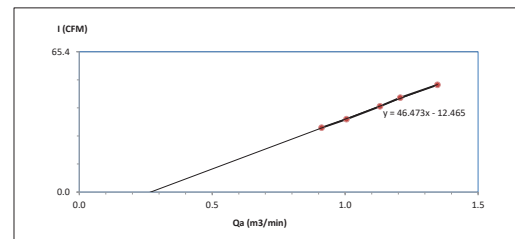

Calibrated by
(Mr. Nontachai Uppathamp)
Field Scientist(1)


Approved by
(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)



High Volume Air Sampler Calibration Worksheet

Project Site : Sumiden Steel Wire (Thailand) Co., Ltd.
Calibrate Location : หมู่ที่ 3 บ้านนาทรายทอง (A2)
Calibrate Date : 23-May-24
CalibrationSheet No.: C-230524-RYG_FS0188
Calibrator ID: RYG_FS0205
Calibrator Model: TE-5028A
Calibrator S/N: 1166
Barometric Pressure (mm Hg) : 754
Temperature (°C) : 29
High Volume ID : RYG_FS0188
High Volume Model : TE-5009X
High Volume S/N : 4796
Calibrator Slope : 0.95561
Calibrator Intercept : -0.02266

Test No.	Delta H ₂ O (inch)	Qa (m ³ /min)	I : Chart (CFM)	Linear Regression
1	1.6	0.860	30	Slope : 35.9888 Intercept : -0.7519 Correlation Coefficient : 0.9998
2	2.0	0.959	34	
3	2.8	1.131	40	
4	3.4	1.244	44	
5	4.4	1.412	50	

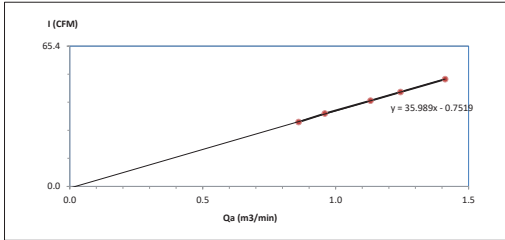

Calibrated by : *N. Uppathamp*
(Mr. Nontachai Uppathamp)
Field Scientist(1)

Approved by : *N. Jantarupan*
(Mr. Noppong Jantarupan)
Enviro Field Coordinator Scientist (3)

FORM NO.: F 06-074 REVISION NO.: 2 ISSUE DATE: 20/11/23

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6, e-mail: service.thailand@sartorius.com



SARTORIUS

Certificate of Calibration

Model Number : LA130S-F
Description : Analytical Balance
Serial Number : 25409664
ID No. : RYG_EN0001
Manufacturer : Sartorius
Certificate No. : 24BCI0068
Issued Date : Friday, February 23, 2024
Reference No. : 229196
Page No. : 1 of 2

Customer Name : ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)
616/10 Moo 5 T. Maenam Khu, A. Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd. (Balance Room)
616/10 Moo 5 T. Maenam Khu, A. Pluak Daeng, Rayong 21140, Thailand.

Calibrated By : Mr. Chonchai Inthana
Calibration Date : Thursday, February 22, 2024
Calibration Procedure No. : This calibration was conducted by Using in-house calibration procedure number (WI-003) Based on UKAS LAB 14 : 2019

Metrological data : Capacity : 150 g Readability : 0.0001 g
Reasons for calibration : ☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance
Ambients Conditions : Temperature : 23.6 °C ± 5.0 °C Humidity : 54.0 % RH ± 10.0 % RH Pressure : ±
Equipment Condition : ☒ Good Operate ☐ Fair

Measurement Method : UKAS Publication Ref : Lab 14
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2, YCS011-522-00	TCS	M2308197S	23-Aug-2025
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19231845	23-Aug-2024

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division Sartorius (Thailand) Co., Ltd.

Mr. Chonchai Inthana (Technical Manager)



SOP FM 33 03 February 2022

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Bangkok 10310
Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

SARTORIUS

Certificate of Calibration

Model Number : LA130S-F
Description : Analytical Balance
Serial Number : 25409664
ID No. : RYG_EN0001
Manufacturer : Sartorius
Certificate No. : 24BCI0068
Issued Date : Friday, February 23, 2024
Reference No. : 229196
Page No. : 2 of 2

Calibration Results : Without Adjustment

Repeatability		Eccentricity (Off-center loading error)	
The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.		The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (1 positions defined according to OIML R76).	
Nominal Value : (Low Load) 10 g Tolerance 0.0001 g	10.0000 10.0000 10.0000 10.0000 9.9999 10.0000 10.0000 10.0000 9.9999 10.0000 9.9999 Standard Deviation 0.00005	Nominal value : 50 g Tolerance 0.0004 g	100.0000 100.0001 100.0001 100.0000 100.0000 100.0001 100.0001 100.0000 100.0002 100.0001 100.0001 0.00005

Linearity				
The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.				
Tolerance	0.0002 g			
Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00020
0.05	0.0500	0.0500	0.0000	0.00021
0.1	0.1000	0.1000	0.0000	0.00021
0.5	0.5000	0.5000	0.0000	0.00021
1	1.0000	1.0000	0.0000	0.00021
2	2.0000	2.0000	0.0000	0.00021
5	5.0000	5.0000	0.0000	0.00021
10	10.0000	10.0001	0.0001	0.00024
20	20.0000	20.0001	0.0001	0.00021
100	100.0000	99.9999	-0.0001	0.00024

End of Report.


SOP FM 33 03 February 2022



High Volume Air Sampler Calibration Worksheet

Project Site : Sumiden Steel Wire (Thailand) Co., Ltd.
Calibrate Location : หมู่ที่ 5 บ้านนาทรายทอง (A1)
Calibrate Date : 23-May-24
CalibrationSheet No.: C-230524-RYG_FS0182
Calibrator ID: RYG_FS0205
Calibrator Model: TE-5028A
Calibrator S/N: 1166
Barometric Pressure (mm Hg) : 754
Temperature (°C) : 29
High Volume ID : RYG_FS0182
High Volume Model : TE-5170D
High Volume S/N : 5335
Calibrator Slope : 1.52567
Calibrator Intercept : -0.03613

Test No.	Delta H ₂ O (inch)	Qad (m ³ /min)	I : Chart (CFM)	Linear Regression
1	2.6	1.0818	40	Slope : 33.3706 Intercept : 3.7042 Correlation Coefficient : 0.9993
2	3.6	1.2666	46	
3	4.4	1.3965	50	
4	5.2	1.5150	54	
5	6.4	1.6768	60	

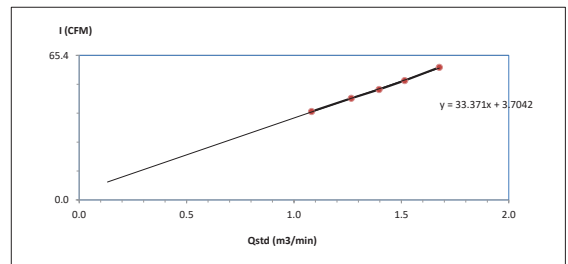

Calibrated by : *N. Uppathamp*
(Mr. Nontachai Uppathamp)
Field Scientist(1)

Approved by : *N. Jantarupan*
(Mr. Noppong Jantarupan)
Enviro Field Coordinator Scientist (3)


FORM NO.: F 06-073 REVISION NO.: 2 ISSUE DATE: 20/11/23



High Volume Air Sampler Calibration Worksheet

Project Site : Sumiden Steel Wire (Thailand) Co., Ltd. Barometric Pressure (mm Hg) : 754
Calibrate Location : หมู่ที่ 3 บ้านนาทรายทอง (A2) Temperature (°C) : 29
Calibrate Date : 23-May-24 High Volume ID : RYG_FS0180
Calibration Sheet No.: C-230524-RYG_FS0180 High Volume Model : TE-5170D
Calibrator ID : RYG_FS0205 High Volume S/N : 1328
Calibrator Model : TE-5028A Calibrator Slope : 1.52567
Calibrator S/N : 1166 Calibrator Intercept : -0.03613

Test No.	Delta H ₂ O (inch)	Q _{ad} (m ³ /min)	I: Chart (CFM)	Linear Regression
1	2.8	1.1213	40	Slope : 34.1772 Intercept : 1.5094 Correlation Coefficient : 0.9994
2	3.8	1.3003	46	
3	4.6	1.4270	50	
4	5.4	1.5431	54	
5	6.6	1.7022	60	

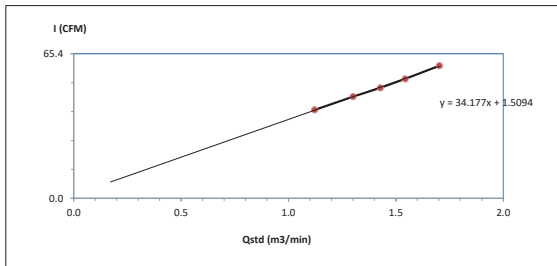

Calibrated by N. Nontachai Uppathamp
(Mr. Nontachai Uppathamp)
Field Scientist(1)

Approved by N. Noppong Juntarupan
(Mr. Noppong Juntarupan)
Enviro Field Coordinator Scientist (3)


FORM NO.: F 06-073 REVISION NO.:2 ISSUE DATE: 20/11/23



MULTIPOINT CALIBRATION REPORT

Calibration Date 4-Jan-24 Equipment Name NOx Analyzer
Manufacturer HORIBA Model APNA-370
Serial No. R08K0177 Equipment ID RYG_FS0463
Calibrator Manufacturer Teledyne API Model 700
Serial No. 947
Std. Gas Concentration (PPM) 55.88 Cylinder No. GN0027222
Cylinder Pressure (psi) 1800 Certified By Airgas Inc.
Certified Date 9-Feb-22 Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	98.80	-1.20	-1.20	101.10	1.10	1.10
2	200.00	201.30	1.30	0.65	201.20	1.20	0.60
3	300.00	299.40	-0.60	-0.20	302.60	2.60	0.87
4	400.00	398.70	-1.30	-0.33	401.50	1.50	0.38
AVERAGE (%)				-0.20			0.61

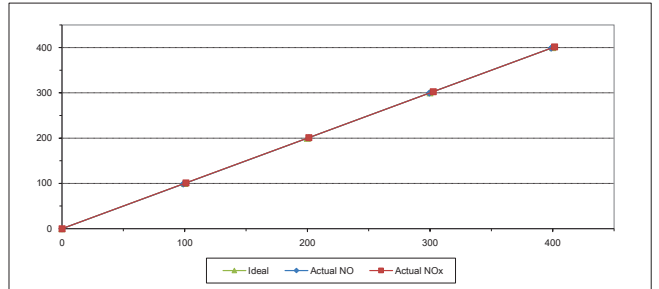

Calibrated By (Mr. Jirawut Sakam)
Field Environmental Scientist (3)

Approved By (Mr. Sarayuth Jittrantont)
Assistant General Manager


ALS Laboratory Group
FORM NO.: F 06-056 REVISION NO.: - ISSUE DATE: 02/04/12



MULTIPOINT CALIBRATION REPORT

Calibration Date 4-Jan-24 Equipment Name NOx Analyzer
Manufacturer HORIBA Model APNA-370
Serial No. SEEAW53E Equipment ID RYG_FS0261
Calibrator Manufacturer Teledyne API Model 700
Serial No. 947
Std. Gas Concentration (PPM) 55.88 Cylinder No. GN0027222
Cylinder Pressure (psi) 1800 Certified By Airgas Inc.
Certified Date 9-Feb-22 Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	98.70	-1.30	-1.30	100.20	0.20	0.20
2	200.00	197.70	-2.30	-1.15	201.50	1.50	0.75
3	300.00	298.10	-1.90	-0.63	302.00	2.00	0.67
4	400.00	398.50	-1.50	-0.38	401.40	1.40	0.35
AVERAGE (%)				-0.67			0.41

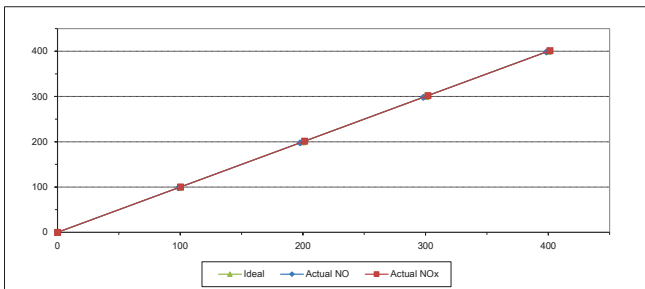

Calibrated By (Mr. Jirawut Sakam)
Field Environmental Scientist (3)

Approved By (Mr. Sarayuth Jittrantont)
Assistant General Manager


ALS Laboratory Group
FORM NO.: F 06-056 REVISION NO.: - ISSUE DATE: 02/04/12



MULTIPOINT CALIBRATION REPORT

Calibration Date 4-Jan-24 Equipment Name SO2 Analyzer
Manufacturer HORIBA Model APSA-370
Serial No. XL29Y85B Equipment ID RYG_FS0462
Calibrator Manufacturer Teledyne API Model 700
Serial No. 947
Std. Gas Concentration (PPM) 58.3 Cylinder No. GN0027222
Cylinder Pressure (psi) 1800 Certified By Airgas Inc.
Certified Date 9-Feb-22 Expired Date 9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Actual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	99.10	-0.90	-0.90
2	200.00	198.10	-1.90	-0.95
3	300.00	299.90	-0.10	-0.03
4	400.00	403.20	3.20	0.80
AVERAGE (%)				-0.20

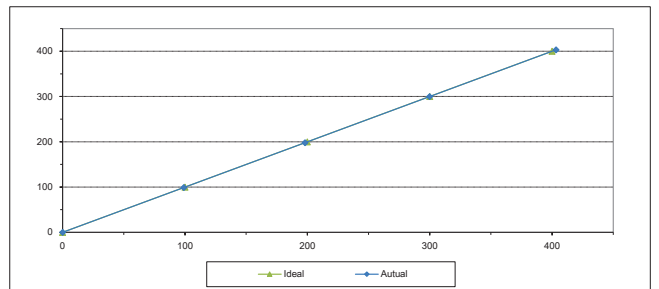

Calibrated By (Mr. Jirawut Sakam)
Field Environmental Scientist (3)

Approved By (Mr. Sarayuth Jittrantont)
Assistant General Manager


ALS Laboratory Group
FORM NO.: F 06-056 REVISION NO.: - ISSUE DATE: 02/04/12



MULTIPOINT CALIBRATION REPORT

Calibration Date	4-Jan-24	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	8HC0DGJF	Equipment ID	RYG_FS0280
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Actual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	99.10	-0.90	-0.90
2	200.00	198.50	-1.50	-0.75
3	300.00	299.00	-1.00	-0.33
4	400.00	398.50	-1.50	-0.38
	AVERAGE (%)			-0.45

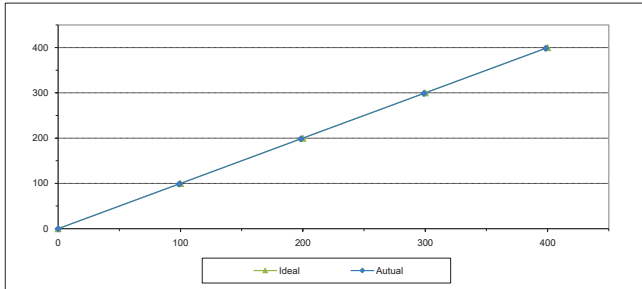

Calibrated By

(Mr. Jirawat Sakarn)
Field Environmental Scientist (3)

Approved By

(Mr. Sarayuth Jitranont)
Assistant General Manager

ALS Laboratory Group
FORM NO.: F-06-056 REVISION NO.: ISSUE DATE: 02/04/12




JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.
63/14-15, 6/73-36
Ponhkaem 7, 7/1, Rd. Wattana, Bangkok,
Bangkok 10600 (Thailand)
Tel: +6688808812
Mobile: +6688899543
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TIS-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.



Certificate Number

CL-009-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE
SERIAL NUMBER
ID NUMBER
CONDITION AS-RECEIVED
CUSTOMER

Cup anemometer
: Novalyxa
: Sensor: WS-02E
: Data logger: 110-WS-16N
: Sensor: -
: Data logger: 1159
: RYG_FS0081
: Used item
: ALS laboratory group (Thailand) Co., Ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
: Khet Suan Luang, Bangkok 10250 Thailand.

Calibration procedure:
The cup anemometer was calibrated against
Standard air velocity transducer model 845502
and pilot tube with precision differential pressure
meter model 0744500 in a large calibration
facility of Eiffel-type wind tunnel with 900 cm² cross test
section area. The WI-CL-008 based on IEC 61400-12-1,
Wind energy generation systems - Part 12-1:
Power performance measurements of
electricity producing wind turbines, March 2017
was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the
measurement to recognized the national
standards, and to realization of the international
system of units (SI) through the NIMT (National
Metrology Institute of Thailand) via Certificate
Number: MW-0052-21 and MW-0066-22.

Uncertainty of Measurement:
The reported uncertainty of measurement is
based on the standard uncertainty multiplied by a
coverage factor k=2, Which for a normal
distribution corresponds to a coverage probability
of approximately 95%. The standard uncertainty
has been determined in accordance with the GUM
"Evaluation of measurement
data - Guide to the expression of uncertainty in
measurement".

RECEIVED DATE
MEASUREMENT DATE
ISSUE DATE

: 16 Jan 2023
: 18 Jan 2023
: 20 Jan 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION

: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area¹ 900 cm²
Win direction frontal area² 100 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.111 [-]

Preconditioning

: 24 hours at ambient conditions.

Measurement Condition

: The average values during measurement are (23.5) °C, (52.2) %RH and (1014.5) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☒ Mr. Sorawit Thachakul
☐ Miss Jittratanee Jittratanont

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Remarks:

¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio $\frac{A_o}{A_t}$

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY



JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.
63/14-15, 6/73-36
Ponhkaem 7, 7/1, Rd. Wattana, Bangkok,
Bangkok 10600 (Thailand)
Tel: +6688808812
Mobile: +6688899543
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TIS-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

Certificate Number

CL-009-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM
MANUFACTURER
MODEL/TYPE
SERIAL NUMBER
ID NUMBER
CONDITION AS-RECEIVED
CUSTOMER

Wind Direction Sensor
: Novalyxa
: Sensor: WS-02E
: Data logger: 110-WS-16N
: Sensor: -
: Data logger: 1159
: RYG_FS0081
: Used item
: ALS laboratory group (Thailand) Co., Ltd.
: 104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
: Khet Suan Luang, Bangkok 10250 Thailand.

Calibration procedure:
The wind direction sensor was calibrated against
Standard Rotary Encoder, model AXR0075P
DA004-P3-5-UD in an close calibration
facility of Eiffel-type wind tunnel with 900 cm² cross test
section area. The WI-CL-008 based on IEC 61400-12-1,
Wind energy generation systems - Part 12-1:
Power performance measurements of
electricity producing wind turbines, March 2017
was used as a calibration guideline.

Traceability:
This certificate provides a traceability of the
measurement to recognized the national
standards, and to realization of the international
system of units (SI) through the NIMT (National
Metrology Institute of Thailand) via Certificate
Number: DA-0043-22.

Uncertainty of Measurement:
The reported uncertainty of measurement is
based on the standard uncertainty multiplied by a
coverage factor k=2, Which for a normal
distribution corresponds to a coverage probability
of approximately 95%. The standard uncertainty
has been determined in accordance with the GUM
"Evaluation of measurement
data - Guide to the expression of uncertainty in
measurement".

RECEIVED DATE
MEASUREMENT DATE
ISSUE DATE

: 16 Jan 2023
: 19 Jan 2023
: 19 Jan 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

PLACE OF CALIBRATION

: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

: Wind tunnel cross-section area¹ 900 cm²
Win direction frontal area² 129 cm²
Diameter of mounting pipe³ - mm
Blockage ratio of test object⁴ 0.143 [-]

Preconditioning

: 24 hours at ambient conditions.

Measurement Condition

: The average values during measurement are (23.8) °C, (47.3) %RH and (1014.8) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☒ Mr. Sorawit Thachakul
☐ Miss Jittratanee Jittratanont

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Remarks:

¹ Nozzle cross-section area of the wind tunnel
² Projected cross-section area of the tested object include mounting pipe
³ Diameter of mounting pipe
⁴ Ratio $\frac{A_o}{A_t}$

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Page 2 of 2 Pages

MEASUREMENT RESULTS¹

The cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration before performing. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pilot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle. UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{std} (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{meas} (m/s)	Error (m/s)	U (k=2) (m/s)
0.981	23.56	23.45	0.8	-0.2	0.15
2.030	23.40	23.45	1.9	-0.2	0.16
3.049	23.50	23.45	2.9	-0.2	0.17
4.129	23.50	23.45	3.9	-0.3	0.20
5.01	23.50	23.45	4.8	-0.2	0.17
5.97	23.54	23.45	5.7	-0.3	0.17
7.05	23.42	23.45	6.8	-0.3	0.18
8.18	23.50	23.45	7.9	-0.3	0.19
9.10	23.34	23.45	8.8	-0.3	0.19
10.10	23.40	23.45	9.7	-0.4	0.19
11.14	23.40	23.45	10.8	-0.4	0.20
12.13	23.32	23.45	11.8	-0.4	0.20
13.20	23.10	23.45	12.9	-0.3	0.20
14.25	23.36	23.45	13.9	-0.4	0.22
15.24	23.22	23.45	14.9	-0.4	0.21
16.30	23.40	23.45	15.8	-0.5	0.22


Remark:

¹ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

² Velocity of standard

³ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.

End of Certificate of Calibration

Certificate Number

CL-009-66

Page 2 of 2 Pages

MEASUREMENT RESULTS¹

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D ₁₀₀ Degree (°)	D ₁₀₀ Degree (°)	Error Degree (°)	U (k=2) Degree (°)
5.01	0.000	0	0	0.59
	45.000	43	-3	0.76
	90.000	89	-2	0.74
	135.000	134	-1	0.74
	180.000	177	-3	0.74
	225.000	229	4	0.58
	270.000	273	3	0.68
	315.000	317	2	0.74

Remark:

¹ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place.

² Direction of standard

³ Direction of Unit Under Calibration

End of Certificate of Calibration

J NAC

JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.
63/14-15, 63/20-36
Petchkasem 7, 7/1, Rd. Wattana, Bangkok, Thailand
Bangkok 10500 (Thailand)
Tel: +6686808012
Mobile: +6686399453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TIS-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

REVIEW BY: *Naratorn P.*
APPROVED BY: *47*
NEXT CALIBRATION: 10/1/24

Certificate Number

CL-010-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM

: Wind Direction Sensor

MANUFACTURER

: Novalyxa

MODEL/TYPE

: Sensor: WS-02F

: Data logger: 200-WS-250L

SERIAL NUMBER

: Sensor: -

: Data logger: A4986

ID NUMBER

: RYG JS0087

CONDITION AS-RECEIVED

: Used item

CUSTOMER

: ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE

: 16 Jan 2023

MEASUREMENT DATE

: 19 Jan 2023

ISSUE DATE

: 20 Jan 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature: 23.0 ± 3.0 °C

Relative Humidity: 55.0 ± 15.0 %RH

Atmospheric Pressure: 1010 ± 10 hPa

PLACE OF CALIBRATION

: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITION

: Wind tunnel cross-section area: 900 cm²: Win direction frontal area: 129 cm²

: Diameter of mounting pipe: - mm

: Blockage ratio of test object: 0.143 [-]

Preconditioning

: 24 hours at ambient conditions.

Measurement Condition

The average values during measurement are (23.5)°C, (47.4) %RH and (1015.6) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☒ Mr. Sorawit Jachachul

☐ Miss Jittrapa Lerttongphol

Remark:

¹ Nozzle cross-section area of the wind tunnel

² Projected cross-section area of the tested object include mounting pipe

³ Diameter of mounting pipe

⁴ Ratio "to" 1

Calibration procedure:

The wind direction sensor was calibrated against Standard Rotary Encoder model AX002750 DMD4-P3-S-UD in an class B section of Eiffel-type wind tunnel with 900 cm² cross section area. The WS-CL-008 based on IEC 61400-12-1: Wind energy generation systems - Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate Number: DA-0043-22

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number

CL-010-66

Page 2 of 2 Pages

MEASUREMENT RESULTS¹

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	D ₁₀₀ Degree (°)	D ₁₀₀ Degree (°)	Error Degree (°)	U (k=2) Degree (°)
5.02	0.000	0	0	0.58
	45.000	43	-2	0.74
	90.000	88	-2	0.74
	135.000	133	-2	0.74
	180.000	179	-1	0.74
	225.000	225	0	0.68
	270.000	273	3	0.58
	315.000	319	4	0.74

Remark:

¹ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place.

² Direction of standard

³ Direction of Unit Under Calibration

End of Certificate of Calibration

J NAC

JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.
63/14-15, 63/20-36
Petchkasem 7, 7/1, Rd. Wattana, Bangkok, Thailand
Bangkok 10500 (Thailand)
Tel: +6686808012
Mobile: +6686399453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TIS-TIS 17025
CALIBRATION 0367

Air speed measurement laboratory
Calibration services department.

Certificate Number

CL-010-66

CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

MEASUREMENT ITEM

: Cup anemometer

MANUFACTURER

: Novalyxa

MODEL/TYPE

: Sensor: WS-02F

: Data logger: 200-WS-250L

SERIAL NUMBER

: Sensor: -

: Data logger: A4986

ID NUMBER

: RYG JS0087

CONDITION AS-RECEIVED

: Used item

CUSTOMER

: ALS laboratory group (Thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,
Khet Suan Luang, Bangkok 10250 Thailand.

RECEIVED DATE

: 16 Jan 2023

MEASUREMENT DATE

: 18 Jan 2023

ISSUE DATE

: 20 Jan 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature: 23.0 ± 3.0 °C

Relative Humidity: 55.0 ± 15.0 %RH

Atmospheric Pressure: 1010 ± 10 hPa

PLACE OF CALIBRATION

: Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

CALIBRATION CONDITIONS

: Wind tunnel cross-section area: 900 cm²: Win direction frontal area: 100 cm²

: Diameter of mounting pipe: - mm

: Blockage ratio of test object: 0.111 [-]

Preconditioning

: 24 hours at ambient conditions.

Measurement Condition

The average values during measurement are (23.6) °C, (55.3) %RH and (1013.5) hPa.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibrated by:

☒ Mr. Sorawit Jachachul

☐ Miss Jittrapa Lerttongphol

Remark:

¹ Nozzle cross-section area of the wind tunnel

² Projected cross-section area of the tested object include mounting pipe

³ Diameter of mounting pipe

⁴ Ratio "to" 1

Calibration procedure:

The cup anemometer was calibrated against Standard air velocity transducer model B45502 and pitot tube with precision differential pressure meter model: DPM2500 in an class B section of Eiffel-type wind tunnel with 900 cm² cross section area. The WS-CL-007 based on IEC 61400-12-1: Wind energy generation systems - Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of the measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate Number: MW-0052-21 and MW-0066-22

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Certificate Number

CL-010-66

Page 2 of 2 Pages

MEASUREMENT RESULTS¹

The cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

V_{std} (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	V_{UUC} (m/s)	Error (m/s)	U (k=2) (m/s)
0.985	23.68	23.60	0.8	-0.2	0.15
2.033	23.54	23.60	1.8	-0.2	0.16
3.045	23.69	23.60	2.9	-0.1	0.19
4.136	23.66	23.60	3.9	-0.2	0.20
5.03	23.50	23.60	4.9	-0.1	0.20
5.98	23.50	23.60	5.9	-0.1	0.18
7.05	23.36	23.60	7.0	-0.1	0.18
8.18	23.54	23.60	8.0	-0.2	0.20
9.10	23.30	23.60	8.9	-0.2	0.20
10.10	23.50	23.60	10.0	-0.1	0.19
11.14	23.28	23.60	11.1	-0.1	0.22
12.12	23.40	23.60	11.9	-0.2	0.21
13.19	23.10	23.60	13.0	-0.2	0.26
14.25	23.46	23.60	14.0	-0.2	0.32
15.26	23.10	23.60	15.0	-0.2	0.23
16.31	23.26	23.60	16.2	-0.1	0.29


Remark:

¹ Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

² Velocity of standard

³ Velocity of Unit Under Calibration

PHOTO OF CALIBRATION SET-UP



Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.

End of Certificate of Calibration



ROTA METER CALIBRATION RESULT APRIL 2024

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
BKK_FS0585	23 Apr 24	Y = 1.0322x + 2.25	0.9997
BKK_FS0587	23 Apr 24	Y = 1.0111x + 16.357	0.9994
BKK_FS0592	23 Apr 24	Y = 1.001x + 14.551	1.0000
BKK_FS0594	23 Apr 24	Y = 1.0048x + 4.9762	1.0000
BKK_FS1004	01 Apr 24	Y = 0.9826x + 12.32	0.9998
BKK_FS1005	01 Apr 24	Y = 1.0183x - 0.0633	0.9998
BKK_FS1006	01 Apr 24	Y = 1.1534x - 3.3241	0.9989
BKK_FS1007	23 Apr 24	Y = 1.1084x + 2.9017	0.9994
BKK_FS1008	06 May 24	Y = 1.1347x + 2.1915	0.9996
BKK_FS1011	07 May 24	Y = 1.3995x - 7.1671	0.9994
BKK_FS1012	07 May 24	Y = 1.0488x - 26.533	0.9998
BKK_FS1013	07 May 24	Y = 1.0255x - 57.741	1.0000
BKK_FS1017	04 Apr 24	Y = 1.0213x + 0.1156	1.0000
BKK_FS1018	04 Apr 24	Y = 1.0007x + 1.3933	0.9999
BKK_FS1019	04 Apr 24	Y = 1.0038x - 1.3381	1.0000
BKK_FS1020	04 Apr 24	Y = 1.003x + 5.7656	1.0000
BKK_FS1021	04 Apr 24	Y = 1.0096x - 25.605	0.9926
BKK_FS1022	04 Apr 24	Y = 1.0937x - 103.66	0.9980
BKK_FS1023	07 May 24	Y = 1.1613x - 2.675	1.0000
BKK_FS1024	07 May 24	Y = 1.0157x - 4.3362	1.0000
BKK_FS1025	07 May 24	Y = 1.0018x - 4.6236	0.9999
BKK_FS1026	19 Jan 24	Y = 0.9618x + 1.9626	0.9999
BKK_FS1027	19 Jan 24	Y = 1.0065x - 4.3786	1.0000
BKK_FS1028	19 Jan 24	Y = 1.0184x - 37.308	0.9997
BKK_FS1029	19 Jan 24	Y = 0.9809x + 2.7925	0.9977
BKK_FS1030	19 Jan 24	Y = 0.996x - 1.3286	1.0000
BKK_FS1031	19 Jan 24	Y = 1.015x - 27.236	0.9997
BKK_FS1039	01 Apr 24	Y = 0.9909x + 11.357	0.9991
BKK_FS1040	01 Apr 24	Y = 1.0121x - 19.203	0.9996
BKK_FS1041	01 Apr 24	Y = 1.0176x + 1.4813	0.9996
BKK_FS1042	01 Apr 24	Y = 0.9927x + 10.76	0.9995
BKK_FS1043	01 Apr 24	Y = 0.9965x + 13.696	1.0000
BKK_FS1044	01 Apr 24	Y = 1.1159x - 0.9354	0.9978
PHK_FS0027	06 May 24	Y = 1.1281x + 0.4949	0.9997
PHK_FS0028	06 May 24	Y = 1.0332x - 1.8233	0.9999
PHK_FS0029	06 May 24	Y = 1.001x + 10.848	1.0000
RYG_FS0197	01 Apr 24	Y = 1.0045x + 10.275	1.0000
RYG_FS0198	01 Apr 24	Y = 1.0061x + 0.715	0.9999
RYG_FS0199	01 Apr 24	Y = 0.976x + 3.1497	0.9998

Page 1 of 2

ALS Laboratory Group



ROTA METER CALIBRATION RESULT APRIL 2024

Rotameter ID.	Calibration Date	Regression Result	Coefficient (R ²)
RYG_FS0654	01 Apr 24	Y = 1.0354x + 0.3361	0.9998
RYG_FS0655	01 Apr 24	Y = 0.978x + 13.603	0.9991
RYG_FS0656	01 Apr 24	Y = 1.0035x + 6.879	0.9999
RYG_FS0657	01 Apr 24	Y = 1.0233x + 0.8908	0.9982
RYG_FS0658	01 Apr 24	Y = 0.9905x + 9.8867	0.9996
RYG_FS0659	01 Apr 24	Y = 0.9994x + 13.924	1.0000
SGK_FS0135	23 Apr 24	Y = 1.0117x + 4.8833	1.0000
SGK_FS0136	23 Apr 24	Y = 1.0134x + 3.6467	1.0000
SGK_FS0138	04 Apr 24	Y = 1.0449x - 0.3684	0.9988
SGK_FS0139	04 Apr 24	Y = 1.0086x + 3.1267	0.9988
SGK_FS0140	04 Apr 24	Y = 1.0029x + 7.5181	1.0000
SGK_FS0141	23 Apr 24	Y = 1.1129x - 0.0619	0.9997
SGK_FS0142	23 Apr 24	Y = 1.0136x + 2.4267	0.9999
SGK_FS0143	23 Apr 24	Y = 1.0036x + 8.3162	1.0000

Review By :

(Mr. Wichan Choonharat)

Enviro Field Services Manager

Approved By :

(Mr. Sarayuth Jitranont)

Assistant General Manager



Calibration Certificate

Certificate No. 551422

Product 200-510M Defender 510 Medium Flow

Serial No. 208345

Cal. Date 18-Aug-2023

Sold To:


All calibrations are performed in accordance with ISO 17025 at Mesa Laboratories, Inc., 12100 W. 6th Ave, Lakewood, CO 80228, an ISO 17025:2017 accredited laboratory through NVLAP. This report shall not be reproduced except in full without the written approval of the laboratory. Results only relate to the items calibrated. This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.

As Received Calibration Data

Technician	Aaron Schwartz		Lab. Pressure	620.1 mmHg
			Lab. Temperature	23.5 °C
Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Received
4523.09 ccm	4519.02 ccm	0.09%	1.00%	In Tolerance
999.43 ccm	999.31 ccm	0.01%	1.00%	In Tolerance
245.22 ccm	245.88 ccm	-0.27%	1.00%	In tolerance

Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML_800_24	205307	25-May-2023	25-May-2024



As Shipped Calibration Data

Certificate No	Technician	Lab. Pressure	Lab. Temperature	618.8 mmHg	24.2 °C
551422	Xiem Ly				
Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Shipped	
4516.61 ccm	4515.56 ccm	0.02%	1.00%	In Tolerance	
1000.87 ccm	1000.87 ccm	0.02%	1.00%	In Tolerance	
249.84 ccm	249.93 ccm	-0.04%	1.00%	In Tolerance	


Mesa Laboratories Standards Used


Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML_800_24	100439	14-Sep-2022	14-Sep-2023

Calibration Notes

The expanded uncertainty of flow has a coverage factor of $k = 2$ for a confidence interval of approximately 95%.
Flow testing is in accordance with our test number MP-00672 with an expanded uncertainty of 0.27% using high-purity nitrogen or filtered laboratory air.
Traceability to the International System of Units (SI) is verified by accreditation to ISO/IEC 17025 by NVLAP under NVLAP Code 200661-0.

Technician Notes:

By: 
Xiem Ly
Production Technician II

Approved By: 
Norma Aragon
QC Inspector

Mesa Laboratories, Inc. certifies that the above instrument meets or exceeds published specifications, and that the calibration results in this certificate were obtained using equipment capable of producing results that are traceable through NIST to the International System of Units (SI). Calibration results are in compliance with ISO/IEC 17025:2017. Calibrations process has a Test Uncertainty Ratio (TUR) of 4:1 or greater. Any Pass/Fail determination is made without taking measurement uncertainty into account and is based on UUT performance against required tolerance only.

Calibration Certificate

Certificate No. 561587
Product 200-510L Defender 510 Low Flow
Serial No. 130026
Cal. Date 25-Sep-2023

Sold To:

All calibrations are performed in accordance with ISO 17025 at Mesa Laboratories, Inc., 12100 W. 6th Ave, Lakewood, CO 80228, an ISO 17025:2017 accredited laboratory through NVLAP. This report shall not be reproduced except in full without the written approval of the laboratory. Results only relate to the items calibrated. This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.

As Received Calibration Data

Technician	Aaron Schwartz	Lab. Pressure	Lab. Temperature	616.1 mmHg	24 °C
Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Received	
0 ccm	456.41 ccm	-100.0%	1.00%	Out of Tolerance	
0 ccm	101.19 ccm	-100.0%	1.00%	Out of Tolerance	
0 ccm	30.36 ccm	-100.0%	1.00%	Out of Tolerance	

Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML_800_10	103743	25-Jan-2023	25-Jan-2024

REVIEW BY: 
APPROVED BY: 
NEXT CAL DATE: 25/01/24

As Shipped Calibration Data

Certificate No	Technician	Lab. Pressure	Lab. Temperature	622.2 mmHg	23.6 °C
561587	Aaron Schwartz				
Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Shipped	
449.75 ccm	450.46 ccm	-0.16%	1.00%	In Tolerance	
100.96 ccm	100.82 ccm	0.14%	1.00%	In Tolerance	
30.63 ccm	30.38 ccm	0.82%	1.00%	In Tolerance	


Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML_800_10	103743	25-Jan-2023	25-Jan-2024

Calibration Notes

The expanded uncertainty of flow has a coverage factor of $k = 2$ for a confidence interval of approximately 95%.
Flow testing is in accordance with our test number MP-00672 with an expanded uncertainty of 0.27% using high-purity nitrogen or filtered laboratory air.
Traceability to the International System of Units (SI) is verified by accreditation to ISO/IEC 17025 by NVLAP under NVLAP Code 200661-0.

Technician Notes:

By: 
Aaron Schwartz
Assembler I

Approved By: 
David Thomas
Quality Engineer

Mesa Laboratories, Inc. certifies that the above instrument meets or exceeds published specifications, and that the calibration results in this certificate were obtained using equipment capable of producing results that are traceable through NIST to the International System of Units (SI). Calibration results are in compliance with ISO/IEC 17025:2017. Calibrations process has a Test Uncertainty Ratio (TUR) of 4:1 or greater. Any Pass/Fail determination is made without taking measurement uncertainty into account and is based on UUT performance against required tolerance only.

Calibration Certificate

Certificate No. 561588
Product 200-510M Defender 510 Medium Flow
Serial No. 151114
Cal. Date 30-Sep-2023

Sold To:

All calibrations are performed in accordance with ISO 17025 at Mesa Laboratories, Inc., 12100 W. 6th Ave, Lakewood, CO 80228, an ISO 17025:2017 accredited laboratory through NVLAP. This report shall not be reproduced except in full without the written approval of the laboratory. Results only relate to the items calibrated. This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government.

As Received Calibration Data

Technician	Xiem Ly	Lab. Pressure	Lab. Temperature	616.8 mmHg	25.8 °C
Instrument Reading	Lab Standard Reading	Deviation	Allowable Deviation	As Received	
0 ccm	4499.86 ccm	-100.0%	1.00%	Out of Tolerance	
0 ccm	997.38 ccm	-100.0%	1.00%	Out of Tolerance	
0 ccm	250.32 ccm	-100.0%	1.00%	Out of Tolerance	

Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML_800_24	117991	16-Aug-2023	16-Aug-2024

REVIEW BY: 
APPROVED BY: 
NEXT CAL DATE: 30/09/24



As Shipped Calibration Data

Technician	561588 Xiem Ly	Lab. Pressure	616.2 mmHg 26.1 °C
Instrument Reading	4496.74 cm	Lab. Standard Reading	4494.43 cm
	997.03 cm		997.16 cm
	249.84 cm		250.5 cm
Deviation	0.05%	Allowable Deviation	1.00%
	-0.01%		1.00%
	-0.26%		1.00%
As Shipped	In Tolerance		In Tolerance
	In Tolerance		In Tolerance

Mesa Laboratories Standards Used

Description	Standard Serial Number	Calibration Date	Calibration Due Date
ML_800_24	117991	05-Dec-2022	05-Dec-2023

Calibration Notes

The expanded uncertainty of flow has a coverage factor of $k = 2$ for a confidence interval of approximately 95%.
Flow testing is in accordance with our test number MP-00672 with an expanded uncertainty of 0.27% using high-purity nitrogen or filtered laboratory air.
Traceability to the International System of Units (SI) is verified by accreditation to ISO/IEC 17025 by NVLAP under NVLAP Code 200661-0.

Technician Notes:
By:

Xiem Ly
Xiem Ly
Production Technician II

Approved By:

Norma Aragon
Norma Aragon
QC Inspector

Mesa Laboratories, Inc. certifies that the above instrument meets or exceeds published specifications, and that the calibration results in this certificate were obtained using equipment capable of producing results that are traceable through NIST to the International System of Units (SI). Calibration results are in compliance with ISO/IEC 17025:2017. Calibrations process has a Test Uncertainty Ratio (TUR) of 4:1 or greater. Any Pass/Fail determination is made without taking measurement uncertainty into account and is based on UUT performance against required tolerance only.

Mesa Laboratories Inc. 12100 W. 6th Ave, Lakewood, CO 80228 USA
(303) 987-8000 www.mesalabs.com Symbol "MLAB" on the NASDAQ

FM-00228 Rev. B

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/19 MOO 13, SOI SUNTANAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 1660-2116-5860-1 FAX: 1660-2116-7140



Certificate of Calibration

Certificate No : 24-AFM-018 Rev.1

Request No : Roq-2024-0043

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok
10250

Unit Under Calibration Details

Measurement Item : Air Flow Meter
Manufacturer : Bios
Model : Defender 510-L
Serial Number : 206895
ID : BKK_FS1346

Sensor Model : -

Sensor Serial Number : -

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 3 January 2024
Calibration Date : 29 January 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

This Certificate was issued to replace to Calibration Certificate No. 24-AFM-018

Calibration By :

MC
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :

MC
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 1 February 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.01 Issue date 25/01/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/19 MOO 13, SOI SUNTANAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 1660-2116-5860-1 FAX: 1660-2116-7140



Certificate No : 24-AFM-018 Rev.1

Request No : Roq-2024-0043

Result of Calibration : Without Adjustment

Temperature	Pressure	STD	UUC	Error	Uncertainty
(°C)	(kPa)	(ml/min)	(ml/min)	(ml/min)	(ml/min)
25.00	101.66	20	20.148	0.1	1.3
25.00	101.67	100	99.409	-0.6	2.8
24.90	101.63	199	197.46	-1.5	5.6
25.00	101.61	300	298.15	-1.8	8.4
24.90	101.60	399	400.13	1	11
24.90	101.59	480	478.02	-2.0	6.8

Note

STD : Standard UUC : Unit Under Calibration

- UUC Reference Condition : At atmospheric pressure and room temperature condition

- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.01 Issue date 25/01/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/19 MOO 13, SOI SUNTANAKORN 11 TAMBON BANG KAEO,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL: 1660-2116-5860-1 FAX: 1660-2116-7140



Certificate of Calibration

Certificate No : 24-AFM-033

Request No : Roq-2024-0241

Customer

Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok
10250

Unit Under Calibration Details

Measurement Item : Primary Flow Calibrator
Manufacturer : Bios
Model : Defender 510-L
Serial Number : 130027
ID : RYG_FS0208

Sensor Model : -

Sensor Serial Number : -

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 31 January 2024
Calibration Date : 13 February 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By :

MC
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :

MC
Mr. Pacit Mathavorn
Calibration Engineer Supervisor

Issue Date : 13 February 2024

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.01 Issue date 25/01/24

Certificate No : 24-AFM-033
Request No : Req-2024-0241

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)
24.50	101.26	20	19.965	0.0	1.3
24.20	101.25	101	100.50	-0.5	2.8
24.00	101.31	200	199.13	-0.9	5.6
23.90	101.42	301	303.56	2.6	8.4
24.10	101.41	401	404.57	4	11
24.10	101.49	480	483.81	3.8	7.0

Note
STD : Standard
UUC : Unit Under Calibration
- UUC Reference Condition : At atmospheric pressure and room temperature condition
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

Certificate of Calibration

Certificate No : 24-AFM-032
Request No : Req-2024-0240

Customer
Name : ALS Laboratory Group Thailand Co., Ltd.
Address : 104 Soi Phatthanakan 40, Phatthanakan Road, Suan Luang, Bangkok
10250

Unit Under Calibration Details

Measurement Item : Primary Flow Calibrator
Manufacturer : Bios
Model : Defender 510-M
Serial Number : 129958
ID : RVG_FS0209
Sensor Model : -
Sensor Serial Number : -

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C
Humidity : 55 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 31 January 2024
Calibration Date : 13 February 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Air Flow Meter	Gilibrator 3 Low flow	18501010006	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qebom	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne AZLA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibration By :
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By :
Mr. Pachi Mathavorn
Calibration Engineer Supervisor
Issue Date : 13 February 2024

Certificate No : 24-AFM-032
Request No : Req-2024-0240

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (cc/min)	UUC (cc/min)	Error (cc/min)	Uncertainty (cc/min)
23.80	101.89	95	100.13	5.1	2.8
23.90	101.71	501	513.93	12.9	7.2
24.18	101.62	1006	1019.3	13	14
24.00	101.81	1997	2023.0	26	29
24.10	101.87	2999	3035.5	37	45
24.60	102.00	3944	3991.8	48	59
24.60	102.08	4739	4790.5	52	72

Note
STD : Standard
UUC : Unit Under Calibration
- UUC Reference Condition : At atmospheric pressure and room temperature condition
- Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$$

where Q = Flow Rate P = Absolute Pressure T = Absolute Temperature
Meas = Measurement Condition ref = Standard Condition

* Indicates non accredited

End of Certificate

Sartorius (Thailand) Co., Ltd.
129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310
Tel: +66 2643 8561-6, e-mail: service.thailand@sartorius.com



NSC-TIS-TIS 17025
CALIBRATION 0426

SARTORIUS

Certificate of Calibration

REVIEW BY : Thawit
APPROVED BY :
NEXT CAL. DATE : 02/02/2025

Model Number : MSE125P-100-DU
Description : Semi-micro Balance
Serial Number : 0033108993
ID No. : RYG_EN0004
Manufacturer : Sartorius
Certificate No. : 24BC0071
Issued Date : Friday, February 23, 2024
Reference No. : 229196
Page No. : 1 of 3

Customer Name : ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd.(Balance Room)
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated By : Mr.Chonchal Inthana
Calibration Date : Thursday, February 22, 2024
Calibration Procedure No. : This calibration was conducted by Using in-house calibration procedure number (WI-003)
Based on UKAS LAB 14 : 2019

Metrological data :

Capacity : 60. /120. g Readability : 0.00001/0.0001 g

Ambients Conditions:

Temperature : 24.0 °C ± 5.0 °C
Humidity : 60.0 % RH ± 10.0 % RH
Pressure : ±

Reasons for calibration

☐ New Installation ☐ Service / Repair ☒ Re-calibration/ Maintenance

Equipment Condition: ☒ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref :Lab 14


The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	TCS	M2308197S	23-Aug-2025
MHB-382SD	Humidity/Barometer/Temp. Lutron MHB-382SD	DKSH	C19231845	23-Aug-2024

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.




Mr.chonchal Inthana(Technical Manager)



Certificate of Calibration

Model Number: MSE125P-100-DU Certificate No.: 24BCI0071
Description: Semi-micro Balance Issued Date: Friday, February 23, 2024
Serial Number: 0033108993 Reference No.: 229196
ID No.: RYG_EN0004
Manufacturer: Sartorius Page No.: 2 of 3

Calibration Results : Without Adjustment

Repeatability			Eccentricity (Off-center loading error)		
The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.			The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/2 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).		
Nominal Value : (Low Load)	5.00003	50.00003	Nominal value :	50	g
5 g	5.00001	50.00003	Tolerance	0.00015	g
Tolerance	5.00003	50.00002			
0.000015 g	5.00002	50.00003			
Nominal Value : (High Load)	5.00001	50.00003			
50 g	5.00001	50.00003			
Tolerance	5.00001	50.00002			
0.000015 g	5.00002	50.00003			
Standard Deviation	0.000008	0.000005			




Linearity				
The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.				
Tolerance	0.00004	g		
Nominal Value	Conventional Mass Value	Displayed Value	Deviation	Uncertainty
(g)	(g)	(g)	(g)	(g)
0.01	0.01000	0.01000	0.00000	0.000024
0.1	0.10000	0.10000	0.00000	0.000025
1	1.00000	1.00000	0.00000	0.000027
2	2.00002	2.00002	0.00000	0.000028
5	5.00002	5.00003	0.00001	0.000031
10	10.00002	10.00004	0.00002	0.000036
20	20.00002	20.00002	0.00000	0.000049
30	30.00004	30.00003	-0.00001	0.000089
40	40.00005	40.00003	-0.00002	0.000089
50	50.00002	50.00001	-0.00001	0.000089

SOP FM 33 03 February 2022

Certificate of Calibration

Model Number: MSE125P-100-DU Certificate No.: 24BCI0071
Description: Semi-micro Balance Issued Date: Friday, February 23, 2024
Serial Number: 0033108993 Reference No.: 229196
ID No.: RYG_EN0004
Manufacturer: Sartorius Page No.: 3 of 3

Calibration Results : Without Adjustment

Repeatability			Eccentricity (Off-center loading error)		
The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.			The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/2 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).		
Nominal Value : (Low Load)	100.0000	100.0000	Nominal value :	50	g
100 g	100.0000	100.0000	Tolerance	0.00015	g
Tolerance	100.0000	100.0000			
0.000015 g	100.0000	100.0000			
Nominal Value : (High Load)	100.0000	100.0000			
100 g	100.0001	100.0000			
Tolerance	100.0000	100.0000			
0.000015 g	100.0000	100.0000			
Standard Deviation	0.00003				

Linearity				
The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.				
Tolerance	0.0001	g		
Nominal Value	Conventional Mass Value	Displayed Value	Deviation	Uncertainty
(g)	(g)	(g)	(g)	(g)
65	65.0000	65.0000	0.0000	0.00015
70	70.0000	70.0000	0.0000	0.00015
75	75.0001	75.0000	-0.0001	0.00015
80	80.0001	80.0000	-0.0001	0.00016
85	85.0001	85.0001	0.0000	0.00018
90	90.0001	90.0001	0.0000	0.00017
95	95.0001	95.0001	0.0000	0.00019
100	100.0000	100.0000	0.0000	0.00024
110	110.0000	110.0000	0.0000	0.00026
120	120.0000	120.0000	0.0000	0.00026

End of Report.

SOP FM 33 03 February 2022



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0292 MTC No. EEL. BP. 83/0267

CALIBRATION CERTIFICATE

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
Address : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok, 10250.
Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre, Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated : Ambient Environment
Description : Sound Calibrator Temperature : (23 ± 3) °C
Manufacturer : Rion Relative Humidity : (50 ± 15) %
Model : NC-74 Ambient Pressure : (101.325 ± 1.500) kPa
Serial No. : 34178121 (ID: RYG_FS0213)

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N4106495.
7. Condenser Microphone B&K 4180 S/N 2889871.

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 19 Feb. 2024
Date of Calibration : 28 Feb. 2024

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.5

Head Office 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9036 Fax. (66) 0 2577 9009
Office/Laboratory 668 Mu 2 Tambon Bangsoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116 (66) 08 3219 9440 E-mail : mtctr@tistr.or.th Website : www.tistr.or.th
Office 196 Phahonyothin Road, Ladysa, Chantachak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217 (66) 08 1889 8827 E-mail : mtctr@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0292 MTC No. EEL. BP. 83/0267

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20µPa at 1000 Hz

Acoustic Output in dB re 20µPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone	Measured Sound Pressure	Deviated value	Uncertainty	Tolerance limit
Type	Level (dB)	(dB)	(dB)	IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	94.01	0.01	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone	Measured Frequency	Deviated value	Uncertainty	Tolerance limit
Type	(Hz)	(Hz)	(Hz)	IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1003.1	3.1	± 1.5	± 1.0%

3. Total Distortion

Standard Microphone	Measured Total Distortion	Uncertainty	Tolerance limit
Type	(%)	(%)	IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	± 0.50	± 3.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was included at level of 0.16 dB from manual.

Calibrated by : (Mr. Weerachai Deechaiyae)

Approved by : (Mr. Pawate Khaiyap)

Director
Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 28 Feb. 2024
Date of Issue : 29 Feb. 2024

End of Certificate

Ref : 2011267021900719001

2 / 2

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office 35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang, Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000 Fax. (66) 0 2577 9009 E-mail : rampa@tistr.or.th Website: www.tistr.or.th
Office/Laboratory 668 Mu 2 Tambon Bangsoomai, Amphoe Muang Samutprakan, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116 Fax. (66) 0 2323 9165 E-mail : mtctr@tistr.or.th
Office 196 Phahonyothin Road, Chantachak, Bangkok 10900, Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217 Fax. (66) 0 2579 8992 E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 176/0167

CALIBRATION CERTIFICATE

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.

Address : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter

Manufacturer : Rion

Model : NL-42

Serial No. : 00900071 (ID-RYG_FS0492)

Microphone : UC-52 No.188464

Preamplifier : NH-24 No.01733

Standards used :

1. Band Pass Filter Wavetek 752A S/N 90010494.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 24 Jan. 2024

Date of Calibration : 23 Feb.2024-1 Mar.2024

1 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 176/0167

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.

10. Speaker Tannoy Limited, Great Britain Patent No. 215300.

11. Digital Multimeter Agilent 34401A S/N MY44005560.

12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 23 Feb.2024-1 Mar.2024

2 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 176/0167

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.94	113.7	113.9	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 124.2 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
17.3	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	12.4	0.10	N/A
C-Weight	18.1	0.10	N/A
Flat	23.9	0.10	N/A

Date of Calibration : 23 Feb.2024-1 Mar.2024

3 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 176/0167

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.1	0.2	0.2	1.5	0.45	0.6
1 000	-0.1	-0.1	-0.1	1.0	0.45	0.6
8 000	0.3	0.3	0.2	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	-0.1	0.0	0.0	2.0	0.20	0.6
125	0.0	0.0	0.0	1.5	0.20	0.6
250	0.0	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	0.0	0.0	0.0	2.0	0.20	0.6
4 000	0.0	0.0	0.0	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 23 Feb.2024-1 Mar.2024

4 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 176/0167

5. Long-term stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 23 Feb.2024-1 Mar.2024

5 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Tel. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtic@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 176/0167

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
136	136.0	0.0	1.1	0.30	0.3
135	135.0	0.0	1.1	0.30	0.3
134	134.0	0.0	1.1	0.30	0.3
133	133.0	0.0	1.1	0.30	0.3
132	132.0	0.0	1.1	0.30	0.3
131	131.0	0.0	1.1	0.30	0.3
130	130.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.1	0.1	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

6 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Tel. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtic@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 176/0167

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.8	-0.2	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

7 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Tel. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtic@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 176/0167

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35.0	35.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	108.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	99.9	-0.1	+1.5; -5.0	0.20	0.3
Slow	200	119.6	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -5.0	0.20	0.3
SEL	200	120.0	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	90.8	-0.2	+1.5; -5.0	0.20	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

8 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Tel. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtic@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 176/0167

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.2	-0.2	3.0	0.20	0.35
Positive half cycle	124.4	124.2	-0.2	2.0	0.20	0.35
Negative half cycle	124.4	124.2	-0.2	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive	Negative	value (dB)	(±dB)	(±dB)	(±dB)
one-half cycle	one-half cycle				
135.0	135.0	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

Approved by :

(Mr. Tawikiat Iamsamran)

(Mr. Prawate Klauya)

Director

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 23 Feb.2024-1 Mar.2024

Date of Issue : 1 Mar. 2024

Ref : 2011267012400347006

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpalit@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

CALIBRATION CERTIFICATE

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.

Address : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter

Manufacturer : Rion

Model : NL-42

Serial No. : 00900072 (ID:RYG_FS0493)

Microphone : UC-52 No.188465

Preamplifier : NH-24 No.01734

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325±1.5) kPa

Standards used :

1. Band Pass Filter Wavetek 752A S/N 90010494.
2. Condenser Microphone Brüel&Kjaer 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjaer 2636 S/N 1537484.

Date of Receipt : 24 Jan. 2024

Date of Calibration : 23 Feb.2024-1 Mar.2024

1 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpalit@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

9. Power Amplifier Brüel&Kjaer 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 23 Feb.2024-1 Mar.2024

2 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpalit@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust	(dB)	(±dB)	(±dB)	(±dB)
113.91	114.0	113.9	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 123.8 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
17.8	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighing	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	11.3	0.10	N/A
C-Weight	17.0	0.10	N/A
Flat	23.4	0.10	N/A

Date of Calibration : 23 Feb.2024-1 Mar.2024

3 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpalit@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.3	0.4	0.4	1.5	0.45	0.6
1 000	-0.2	-0.2	-0.2	1.0	0.45	0.6
8 000	-0.4	-0.5	-0.5	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	-0.1	0.0	0.0	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	-0.1	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	0.0	2.0	0.20	0.6
4 000	-0.1	0.0	0.0	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 23 Feb.2024-1 Mar.2024

4 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtci@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 23 Feb.2024-1 Mar.2024

5 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtci@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
136	136.0	0.0	1.1	0.30	0.3
135	135.0	0.0	1.1	0.30	0.3
134	134.1	0.1	1.1	0.30	0.3
133	133.0	0.0	1.1	0.30	0.3
132	132.0	0.0	1.1	0.30	0.3
131	131.0	0.0	1.1	0.30	0.3
130	130.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.1	0.1	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

6 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtci@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.9	-0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

7 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtci@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35.0	35.0	0.0	±1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	109.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	99.9	-0.1	+1.5; -5.0	0.20	0.3
Slow	200	119.6	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -5.0	0.20	0.3
	200	120.0	0.0	±1.0	0.20	0.3
SEL	2	100.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	90.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

8 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.2	-0.2	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
135.5	135.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

Approved by :

(Mr. Tawikiat Iamsamran)

(Mr. Prawate Klunayra)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 23 Feb.2024-1 Mar.2024

Date of Issue : 1 Mar. 2024

Ref : 2011267012400347007

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

CALIBRATION CERTIFICATE

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.

Address : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter

Manufacturer : Rion

Model : NL-402

Serial No. : 09090073 (ID-RYG_FS0494)

Microphone : UC-52 No.188466

Preamplifier : NH-24 No.01735

Standards used :

1. Band Pass Filter Wavetek 752A S/N 90010494.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Date of Receipt : 24 Jan. 2024

Date of Calibration : 23 Feb.2024-1 Mar.2024

1 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.

10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.

11. Digital Multimeter Agilent 34401A S/N MY44005560.

12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor k=2, providing a level of confidence of approximately 95%.

Date of Calibration : 23 Feb.2024-1 Mar.2024

2 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpal@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	Before adjust	After adjust				
113.91	114.1	113.9	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 124.6 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
17.8	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
A-Weight	12.9	0.10	N/A
C-Weight	18.5	0.10	N/A
Flat	24.2	0.10	N/A

Date of Calibration : 23 Feb.2024-1 Mar.2024

3 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : numpat@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	A-weight	C-weight	Flat			
125	0.1	0.2	0.2	1.5	0.45	0.6
1 000	-0.1	-0.1	-0.1	1.0	0.45	0.6
8 000	-0.7	-0.7	-0.7	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	A-weight	C-weight	Flat			
63	-0.1	0.0	0.0	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	-0.1	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	0.0	2.0	0.20	0.6
4 000	-0.1	0.0	0.0	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 23 Feb.2024-1 Mar.2024

4 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : numpat@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	Begin	End			
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 23 Feb.2024-1 Mar.2024

5 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : numpat@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
136	136.0	0.0	1.1	0.30	0.3
135	135.0	0.0	1.1	0.30	0.3
134	134.0	0.0	1.1	0.30	0.3
133	133.0	0.0	1.1	0.30	0.3
132	132.0	0.0	1.1	0.30	0.3
131	131.0	0.0	1.1	0.30	0.3
130	130.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	68.9	-0.1	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

6 / 9

The results relate only to the items tested/calibrated or value assigned.
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FMBL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : numpat@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
64	63.9	-0.1	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.9	-0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpat@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.4



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35.0	35.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	109.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	99.9	-0.1	+1.5; -5.0	0.20	0.3
Slow	200	119.6	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -5.0	0.20	0.3
SEL	200	120.0	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	90.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpat@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.4



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.3	-0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
135.5	135.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

Approved by :

(Mr. Tawikiat Iamsamran)

(Mr. Prayale Klauya)

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 23 Feb.2024-1 Mar.2024

Date of Issue : 1 Mar. 2024

Ref : 2011267012400347008

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpat@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.4



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

CALIBRATION CERTIFICATE

Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.

Address : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Level Meter

Manufacturer : Rion

Model : NL-42

Serial No. : 00900074 (ID:RYG_FS0495)

Microphone : UC-52 No.188467

Preamplifier : NH-24 No.01736

Standards used :


- Band Pass Filter Wavetek 752A S/N 90010494.
- Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
- Decade Attenuator Ando AL-205 S/N 00464602.
- Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
- Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
- Digital Multimeter Fluke 8520A S/N 4985007.
- Pistonphone Rion NC-72 S/N 00402446.
- Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

Ambient Environment

Temperature : (23 ± 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.5) kPa



Date of Receipt : 24 Jan. 2024

Date of Calibration : 23 Feb.2024-1 Mar.2024

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpat@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtg@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

FM.BLMTC.002 Rev.4



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

Calibration Procedure :

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

Date of Calibration : 23 Feb.2024-1 Mar.2024

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35/14-3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpag@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Mahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	Before adjust	After adjust				
113.94	114.1	113.9	0.0	1.0	0.30	N/A

Note: The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 124.2 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
16.5	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
A-Weight	11.7	0.10	N/A
C-Weight	17.2	0.10	N/A
Flat	22.5	0.10	N/A

Date of Calibration : 23 Feb.2024-1 Mar.2024

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35/14-3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpag@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Mahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	A-weight	C-weight	Flat			
125	-0.2	-0.3	0.3	1.5	0.45	0.6
1 000	-0.2	-0.2	-0.2	1.0	0.45	0.6
8 000	-0.7	-0.8	-0.8	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
	A-weight	C-weight	Flat			
63	-0.1	-0.1	0.0	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	-0.1	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	-0.1	0.0	2.0	0.20	0.6
4 000	-0.1	-0.1	0.0	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 23 Feb.2024-1 Mar.2024

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35/14-3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpag@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Mahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (\pm dB)	Uncertainty (\pm dB)	Maximum-permitted uncertainty of measurement (\pm dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 23 Feb.2024-1 Mar.2024

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35/14-3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpag@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Mahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
136	136.0	0.0	1.1	0.30	0.3
135	135.0	0.0	1.1	0.30	0.3
134	134.0	0.0	1.1	0.30	0.3
133	133.0	0.0	1.1	0.30	0.3
132	132.0	0.0	1.1	0.30	0.3
131	131.0	0.0	1.1	0.30	0.3
130	130.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	68.9	-0.1	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

6/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpagtdtr@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtr@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
64	63.9	-0.1	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	48.9	-0.1	1.1	0.30	0.3
44	43.9	-0.1	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.8	-0.2	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

7/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpagtdtr@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtr@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35.0	35.0	0.0	1.1	0.30	0.3

9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	108.9	-0.1	+1.0/-2.5	0.20	0.3
	0.25	99.9	-0.1	+1.5/-5.0	0.20	0.3
Slow	200	119.6	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0/-5.0	0.20	0.3
	0.25	90.8	-0.2	+1.5/-5.0	0.20	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

8/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpagtdtr@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtr@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.4	0.0	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
135.0	135.0	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

(Mr. Tawikiat Iamsamran)

Approved by :

(Mr. Pravee Khayapa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 23 Feb.2024-1 Mar.2024

Date of Issue : 1 Mar. 2024

Ref : 2011267012400347009

End of Certificate

9/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BLMTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpagtdtr@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtr@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphom.com http://www.sithiphom.com



Cert. No. : ACC23028
Pages : 1 of 3

Calibration Certificate

Equipment : SOUND CALIBRATOR
Manufacturer : RION
Model : NC-74
Serial No.: 34478385
ID No.: NKH_FS0019



Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 07 SEPTEMBER 2023
Calibration Date : 20 SEPTEMBER 2023
Date of Issue : 20 SEPTEMBER 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACC23028
Job No. : VC66AC0100
Pages : 2 of 3

Calibration Procedure : CP-AC-03

Calibration Method :

This equipment was calibrated by based on IEC-60942-2003 Standard.
The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL_BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL_BP 30/0267	13-FEB-24
Digital Multimeter	33461A	MY60024273	EEL_BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24
Audio Analyzer	AVR-3360A	V744B6069	EF-0012-23	10-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

T. Petchur

SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

Continuation of Calibration Certificate

Cert. No. : ACC23028
Job No. : VC66AC0100
Pages : 3 of 3

Result of calibration :

1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.13	0.13	0.14	0.40

2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value (%)	Uncertainty (%)	Acceptance limit (%)
1000	1002.3	0.2	0.1	1.0

3. Total distortion

Measured value (%)	Uncertainty (%)	Acceptance limit (%)
1.41	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchur

SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand
Tel. +66 2433 8331 Email : calibration@sithiphom.com



Cert. No. : ACL24096
Pages : 1 of 9

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-21/ Microphone UC-52 / Preamplifier NH-21
Serial No.: 00465461 / 108081 / 19513
ID No.: RYG_FS0007

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 19 JANUARY 2024
Calibration Date : 25-26 JANUARY 2024
Date of Issue : 29 JANUARY 2024



Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL24095
Job No. : VC67AC0058
Pages : 2 of 9

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

S. Petch.

Cert. No. : ACL24095
Job No. : VC67AC0058
Pages : 3 of 9

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.1	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

S. Petch.

Cert. No. : ACL24095
Job No. : VC67AC0058
Pages : 4 of 9

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
24.0

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	22.9
C - weight	24.9
Flat	27.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.1	0.2	0.2	± 5.0

S. Petch.

Cert. No. : ACL24095
Job No. : VC67AC0058
Pages : 5 of 9

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.2	-0.1	-0.1	±2.0
125	-0.1	-0.1	-0.2	±1.5
250	-0.1	-0.1	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.1	0.1	0.1	±2.0
4000	0.1	0.1	0.0	±3.0
8000	0.1	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

S. Petch.

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1

g. Petch.

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1
120	94.0	94.0	0.0	±1.1
110	94.0	94.0	0.0	±1.1
100	94.0	94.0	0.0	±1.1
90	94.0	94.0	0.0	±1.1

Level linearity on each level range

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	41.6	41.8	0.2	±1.1
120	32.3	32.0	-0.3	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

g. Petch.

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	132.6	-0.8	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
Positive half cycle	132.4	133.6	1.2	±2.0
Negative half cycle	132.4	133.6	1.2	±2.0

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.4	89.3	-0.1	±1.5

g. Petch.

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

g. Petch.

Cert. No. : ACL24095
Pages : 1 of 9

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-21/ Microphone UC-52 / Preamplifier NH-21
Serial No.: 00376364 / 71486 / 23142
ID No.: RYG_FS0012

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 19 JANUARY 2024
Calibration Date : 25-26 JANUARY 2024
Date of Issue : 29 JANUARY 2024

Calibrated by : Nathakorn Pisutpaisan

Approved by : *T. Petchurai*
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced
other than in full, except with the prior written approval of the head of Calibration Laboratory.

Cert. No. : ACL24096
Job No. : VC67AC0058
Pages : 2 of 9

Calibration Procedure : CP-AC-02

Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference
Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EELBP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EELBP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EELBP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KA1	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand),
3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Cert. No. : ACL24096
Job No. : VC67AC0058
Pages : 3 of 9

Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.1	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

Cert. No. : ACL24096
Job No. : VC67AC0058
Pages : 4 of 9

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	93.9	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
26.2

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	22.9
C - weight	24.2
Flat	27.6

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.3	0.3	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.5	0.6	0.6	± 5.0

Cert. No. : ACL24096
Job No. : VC67AC0058
Pages : 5 of 9

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.1	0.1	0.0	±2.0
4000	0.1	0.1	0.0	±3.0
8000	0.1	0.1	0.1	±5.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.3

T. Petch

Cert. No. : ACL24096
Job No. : VC67AC0058
Pages : 6 of 9

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1

T. Petch

Cert. No. : ACL24096
Job No. : VC67AC0058
Pages : 7 of 9

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	94.0	94.0	0.0	±1.1
120	94.0	94.0	0.0	±1.1
110	94.0	94.0	0.0	±1.1
100	94.0	94.0	0.0	±1.1
90	94.0	94.0	0.0	±1.1

Level linearity on each level range

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
130	41.6	41.9	0.3	±1.1
120	32.0	31.9	-0.1	±1.1

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

T. Petch

Cert. No. : ACL24096
Job No. : VC67AC0058
Pages : 8 of 9

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±3.0
One	133.4	132.8	-0.6	±3.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	130.0	130.0	0.0	±2.0
Positive half cycle	132.4	132.1	-0.3	±2.0
Negative half cycle	132.4	132.1	-0.3	±2.0

11. Overload indication

Measured value (dB)		Deviated Value	Acceptance Limits
Positive one-half cycle	Negative one-half cycle	(dB)	(dB)
89.3	89.3	0.0	±1.5

T. Petch

Cert. No. : ACL24096
Job No. : VC67AC0058
Pages : 9 of 9

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

T. Petchur

Cert. No. : ACL23218
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No.: 00531296 / 23161 / 32972
ID No.: - www.60532

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 21 JUNE 2023
Calibration Date : 04-05 JULY 2023
Date of Issue : 06 JULY 2023

REVIEW BY: *Nathakorn P.*
APPROVED BY: *T. Petchur*
NEXT CAL DATE: 4/4/24

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced
other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23218
Job No. : VC66AC0071
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference
Standard Instruments.
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL_BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL_BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL_BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL23218
Job No. : VC66AC0071
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

QF-TS12-04-04-020664

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL23218
Job No. : VC66AC0071
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	9.9
C - weight	14.7
Flat	20.5

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.1	± 1.0
1000	0.2	0.2	0.2	± 0.7
8000	-0.2	-0.1	-0.2	+ 1.5, - 2.5

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23218
Job No. : VC66AC0071
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
63	0.1	0.0	0.1	±1.0
125	0.1	0.1	0.1	±1.0
250	0.0	0.1	0.0	±1.0
500	0.1	0.1	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.1	0.1	± 0.1

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23218
Job No. : VC66AC0071
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.1	0.1	±0.8
29.0	29.0	0.0	±0.8
28.0	28.1	0.1	±0.8
27.0	27.1	0.1	±0.8
26.0	26.2	0.2	±0.8
25.0	25.2	0.2	±0.8

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23218
Job No. : VC66AC0071
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	108.0	0.0	1.0 ; -3.0
	2	8	117.0	117.0	0.0	±0.5 ; -1.5
	200	800	134.0	134.1	0.1	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
SEL	2	8	108.0	108.1	0.1	1.0 ; -1.5
	200	800	128.0	128.1	0.1	±0.5

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
One	136.4	136.4	0.0	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23218
Job No. : VC66AC0071
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchur

451-451/1 Sirinthern Rd.,Bangbunru, Banglud Bangkok 10700 THAILAND.
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL23203
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No. : 00531297 / 23200 / 32973
ID No. : - 10.11.1.0115

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.

Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %

Received Date : 21 JUNE 2023
Calibration Date : 28-30 JUNE 2023
Date of Issue : 06 JULY 2023

Calibrated by : Nathakorn Pisutpaisan

Approved by : T. Petchur
(Thanakul Petchur)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23203
Job No. : VC66AC0071
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL_BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL_BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL_BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

- 3.1 National Institute of Metrology (Thailand).
- 3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL23203
Job No. : VC66AC0071
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

QF-TS12-04-04-020664

T. Petchur

Cert. No. : ACL23203
Job No. : VC66AC0071
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	7.8
C - weight	13.2
Flat	18.9

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.2	± 1.0
1000	0.1	0.1	0.1	± 0.7
8000	-0.4	-0.4	-0.3	+ 1.5, - 2.5

QF-TS12-04-04-020664

T. Petch.

Cert. No. : ACL23203
Job No. : VC66AC0071
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.1	0.0	±1.0
125	0.1	0.1	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.1	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

QF-TS12-04-04-020664

T. Petch.

Cert. No. : ACL23203
Job No. : VC66AC0071
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.0	0.0	±0.8
136.0	136.0	0.0	±0.8
135.0	135.0	0.0	±0.8
134.0	134.0	0.0	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	53.9	-0.1	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	29.9	-0.1	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

QF-TS12-04-04-020664

T. Petch.

Cert. No. : ACL23203
Job No. : VC66AC0071
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.1	0.1	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.1	0.1	±0.5

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
One	136.4	136.4	0.0	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	132.9	-0.1	±1.0
Positive half cycle	135.4	135.1	-0.3	±1.0
Negative half cycle	135.4	135.1	-0.3	±1.0

QF-TS12-04-04-020664

T. Petch.

Continuation of Calibration Certificate

Cert. No. : ACL23203
Job No. : VC66AC0071
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value	Acceptance Limits
Positive one-half cycle	Negative one-half cycle	(dB)	(dB)
89.5	89.5	0.0	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

T. Petchur

451-451/1 Sirinthon Rd, Bangbunmu, Bangplud Bangkok 10700 THAILAND.
Tel:0-2435-8800 Fax:0-2433-1679 e-mail:cal-center@sithiphom.com http://www.sithiphom.comCert. No. : ACL23204
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER
Manufacturer : RION
Model : NL-52A / Microphone UC-59 / Preamplifier NH-25
Serial No. : 00531298 / 23203 / 32974
ID No. : -

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,
BANGKOK, 10250 THAILAND.Location : -
Ambient Temperature : (23.0 ± 3) °C
Pressure : (101.3 ± 3) kPa
Relative Humidity : (50.0 ± 20) %Received Date : 21 JUNE 2023
Calibration Date : 28-30 JUNE 2023
Date of Issue : 06 JULY 2023REVIEW BY : *Nathakorn P.*
APPROVED BY : *T. Petchur*
NEXT CAL DATE : 28/6/24

Calibrated by : Nathakorn Pisutpaisan

Approved by :

T. Petchur
(Thanakul Petchurai)

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

QF-TS12-04-04-020664

Continuation of Calibration Certificate

Cert. No. : ACL23204
Job No. : VC66AC0071
Pages : 2 of 8

Calibration Procedure : CP-AC-01

Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For test results of each items were made by observation of each Instruments display and also with SLM's display.

Condition of this result of calibration :

1. Reference Standard Instruments :

Instrument	Model	Serial No.	Cert. No.	Due Date
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL_BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL_BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL_BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAJ	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

QF-TS12-04-04-020664

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL23204
Job No. : VC66AC0071
Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter, will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

QF-TS12-04-04-020664

T. Petchur

Continuation of Calibration Certificate

Cert. No. : ACL23204
Job No. : VC66AC0071
Pages : 4 of 8

Result of calibration :

1. Absolute sensitivity

Reference Acoustic Signal (dB)	Measured Value (dB)	Deviation (dB)	Acceptance Limit (dB)
93.9 (93.98)	94.0	0.0	±0.3

2. Self-generated noise

2.1 Normal test

Measured Value (dB)
13.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value (dB)
A - weight	8.7
C - weight	14.3
Flat	20.0

3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.0	0.1	0.1	± 1.0
1000	0.0	0.0	0.0	± 0.7
8000	-0.5	-0.5	-0.5	+ 1.5, - 2.5

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23204
Job No. : VC66AC0071
Pages : 5 of 8

4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.0	0.0	+ 1.5, - 2.5
16000	0.0	-1.3	-1.2	+ 2.5, -16.0

5. Frequency and time weightings at 1 kHz

5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

6. Long - term stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	94.0	94.0	0.0	± 0.1

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23204
Job No. : VC66AC0071
Pages : 6 of 8

7. Level linearity on the reference level range

Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
137.0	137.1	0.1	±0.8
136.0	136.1	0.1	±0.8
135.0	135.1	0.1	±0.8
134.0	134.1	0.1	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.1	0.1	±0.8
124.0	124.0	0.0	±0.8
119.0	119.1	0.1	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.1	0.1	±0.8
99.0	99.1	0.1	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	26.0	0.0	±0.8
25.0	24.9	-0.1	±0.8

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23204
Job No. : VC66AC0071
Pages : 7 of 8

8. Level linearity including the level range control

Range	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Auto	94.0	94.0	0.0	±0.8

9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Cycle	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
	0.25	1	99.0	98.9	-0.1	1.0 ; -3.0
SEL	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

10. Peak C sound level

Number of cycle in test signal	Anticipated Value (dB)	Measured Value, L _{peak} (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±2.0
One	136.4	136.3	-0.1	±2.0

Number of cycle in test signal	Anticipated Value (dB)	Measured Value (dB)	Deviated Value (dB)	Acceptance Limits (dB)
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.2	-0.2	±1.0

QF-TS12-04-04-020664

T. Petch

Continuation of Calibration Certificate

Cert. No. : ACL23204
Job No. : VC66AC0071
Pages : 8 of 8

11. Overload indication

Measured value (dB)		Deviated Value (dB)	Acceptance Limits (dB)
Positive one-half cycle	Negative one-half cycle		
89.8	89.7	-0.1	±1.5

12. High level stability

Frequency Weighting	SLM Display at initial (dB)	SLM Display at final (dB)	Deviated Value (dB)	Acceptance Limits (dB)
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor $k = 2$ or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

QF-TS12-04-04-020664

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research plc

DATE OF ISSUE 10 November 2023

CERTIFICATE NUMBER 202607

REVIEW BY *Michael P.*
APPROVED BY *HE*
NEXT CAL. DATE 9/11/24

Cirrus Research plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
N.Smith
Electronically signed:

doseBadge Reader : IEC 60942:2003

Instrument information

Manufacturer: Cirrus Research plc

Notes:

Model: RC:110A

Serial number: 79625

Class: 2

Test summary

Date of calibration: 10 November 2023

The doseBadge reader detailed above has been calibrated to the published data as described in the operating manual and in the half-inch configuration. The procedures and techniques used are as described in IEC60942_2003 Annex B – Periodic Tests and three determinations of the sound pressure level, frequency and total distortion were made.

The sound pressure level was measured using a WS2F condenser microphone type MK224 manufactured by Cirrus Research plc.

The results have been corrected to the reference pressure of 101.33 kPa using the manufacturer's data.

The doseBadge Reader has been shown to conform to the Class 2 requirements for periodic testing, described in Annex B of IEC 60942:2003 for the sound pressure level(s) and frequency(ies) stated, for the environmental conditions under which the tests were performed.

However, as public evidence was not available, from a testing organisation responsible for pattern approval, to demonstrate that the model of doseBadge Reader conformed to the requirements for pattern evaluation described in Annex A of IEC 60942:2003, no general statement or conclusion can be made about conformance of the doseBadge Reader to the requirements of IEC 60942:2003.

Notes:

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:
202607

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 98.74 kPa Temperature: 21.8 °C Humidity: 40.4 %
After Pressure: 98.75 kPa Temperature: 22.7 °C Humidity: 37.5 %

Test equipment

Equipment	Manufacturer	Model	Serial number
Distortion Meter	Keithley	2015	0994818
Acoustic Calibrator	Bruel and Kjaer	4231	2610257
Environmental Monitor	Comet	T7510	21962628

Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	114.00	114.00	114.00	114.00	0.00	±0.75	0.11 dB
Distortion (%)	< 4.00	0.23	0.23	0.23	0.23	0.23	+4.00	0.13 %
Frequency (Hz)	1000.0	1005.0	1005.0	1005.0	1005.0	5.0	±20.0	0.1 Hz

The measured quantities or deviations (as applicable), extended by the expanded combined uncertainty of measurement, must not exceed the corresponding tolerance.

Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

End of results

CERTIFICATE OF CALIBRATION

ISSUED BY Cirrus Research

DATE OF ISSUE 18 August 2023

CERTIFICATE NUMBER 197597

REVIEW BY *Michael P.*
APPROVED BY *HE*
NEXT CAL. DATE 18/8/24

Cirrus Research
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory
R.Thomas
Electronically signed:

doseBadge Reader : IEC 60942:2003

Instrument information

Manufacturer: Cirrus Research plc

Notes:

Model: RC:110A

Serial number: 76062

Class: 2

Test summary

Date of calibration: 18 August 2023

The doseBadge reader detailed above has been calibrated to the published data as described in the operating manual and in the half-inch configuration. The procedures and techniques used are as described in IEC60942_2003 Annex B – Periodic Tests and three determinations of the sound pressure level, frequency and total distortion were made.

The sound pressure level was measured using a WS2F condenser microphone type MK224 manufactured by Cirrus Research plc.

The results have been corrected to the reference pressure of 101.33 kPa using the manufacturer's data.

The doseBadge Reader has been shown to conform to the Class 2 requirements for periodic testing, described in Annex B of IEC 60942:2003 for the sound pressure level(s) and frequency(ies) stated, for the environmental conditions under which the tests were performed.

However, as public evidence was not available, from a testing organisation responsible for pattern approval, to demonstrate that the model of doseBadge Reader conformed to the requirements for pattern evaluation described in Annex A of IEC 60942:2003, no general statement or conclusion can be made about conformance of the doseBadge Reader to the requirements of IEC 60942:2003.

Notes:

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate No. : CDT-018-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : Delta OHM
MODEL/TYPE : HD32.2
SERIAL NUMBER : 18018311
ID NUMBER : RYG_F50356
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 11 Jan 2024
MEASUREMENT DATE : 12 Jan 2024
ISSUE DATE : 17 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0038-23, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 28 Mar 2024
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM Evaluation of measurement data - Guide to the expression of uncertainty in measurement

APPROVED BY: *Nasom P*
11/1/25
NEXT CAL. DATE



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Calibrated by:
☐ Mr. Sorawit Thalalad
☒ Miss Jittaporn Lertsomphol
☐ Miss Ruangrumpai Phoommitt

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Continuation of Certificate of Calibration Number CDT-018-67

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 18021466.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.053	20.0	-0.1	0.099
80	25.045	25.0	0.0	0.099
80	30.040	30.0	0.0	0.099
80	35.039	35.0	0.0	0.099
80	40.030	40.0	0.0	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 18020493.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.052	20.0	0.0	0.14
110	25.045	25.1	0.1	0.099
110	30.040	30.1	0.1	0.099
110	35.039	35.1	0.1	0.099
110	40.030	40.1	0.1	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2 S/N: 18021258.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.053	20.2	0.1	0.099
75	25.045	25.0	0.0	0.099
75	30.040	30.0	0.0	0.099
75	35.039	34.9	-0.1	0.099
75	40.030	39.9	-0.1	0.099

UUC*: Unit Under Calibration

Remark: The reported uncertainty of measurement is 0.14, based on standard uncertainty multiplied by a coverage factor $k=2.14$ providing a level of confidence of approximately 95%

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-019-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : Delta OHM
MODEL/TYPE : HD32.2
SERIAL NUMBER : 18018312
ID NUMBER : RYG_F50357
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 11 Jan 2024
MEASUREMENT DATE : 12 Jan 2024
ISSUE DATE : 17 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0038-23, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 28 Mar 2024
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-
00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM Evaluation of measurement data - Guide to the expression of uncertainty in measurement

APPROVED BY: *Nasom P*
11/1/25
NEXT CAL. DATE



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Calibrated by:
☐ Mr. Sorawit Thalalad
☒ Miss Jittaporn Lertsomphol
☐ Miss Ruangrumpai Phoommitt

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Continuation of Certificate of Calibration Number CDT-019-67

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 – 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 18021464.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.039	20.0	0.0	0.099
80	25.051	25.0	-0.1	0.099
80	30.045	30.0	0.0	0.099
80	35.036	35.0	0.0	0.099
80	40.030	40.0	0.0	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 18020495.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.038	20.0	0.0	0.099
110	25.051	25.1	0.0	0.099
110	30.045	30.1	0.1	0.099
110	35.036	35.1	0.1	0.099
110	40.030	40.1	0.1	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2 S/N: 18021263.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.039	20.1	0.1	0.099
75	25.051	25.0	-0.1	0.099
75	30.045	30.0	0.0	0.099
75	35.036	34.9	-0.1	0.099
75	40.030	39.9	-0.1	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-020-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : Delta OHM
MODEL/TYPE : HD32.2
SERIAL NUMBER : 18018313
ID NUMBER : RVG_F50358
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 11 Jan 2024
MEASUREMENT DATE : 15 Jan 2024
ISSUE DATE : 17 Jan 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0038-23, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 28 Mar 2024
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$. Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM Evaluation of measurement data - Guide to the expression of uncertainty in measurement.

REVIEW BY: *Handorn P.*
APPROVED BY: *[Signature]*
NEXT CAL. DATE: 4/1/25



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jittaporn Lertsomphol
☐ Miss Ruangrumpal Poommitt

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Continuation of Certificate of Calibration Number CDT-020-67

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 ~ 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 18021467.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.039	20.1	0.1	0.099
80	25.051	25.1	0.0	0.099
80	30.045	30.0	0.0	0.099
80	35.036	35.1	0.1	0.099
80	40.030	40.0	0.0	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 18020497.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.039	20.1	0.1	0.099
110	25.051	25.1	0.0	0.099
110	30.045	30.1	0.1	0.099
110	35.036	35.1	0.1	0.099
110	40.030	40.1	0.1	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2 S/N: 18021270.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.039	20.2	0.2	0.099
75	25.051	25.1	0.0	0.099
75	30.045	30.1	0.1	0.099
75	35.036	35.0	0.0	0.099
75	40.030	39.9	-0.1	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration



CERTIFICATE OF CALIBRATION

Certificate No. : CDT-036-67

Page 1 of 2 Pages

MEASUREMENT ITEM : Heat Stress Monitor
MANUFACTURER : Delta OHM
MODEL/TYPE : HD32.2
SERIAL NUMBER : 20032237
ID NUMBER : NIKH_F50060
CONDITION AS-RECEIVED : Used item
CUSTOMER : ALS laboratory group (thailand) Co., Ltd.
104 Phatthanakan 40, Phatthanakan Rd.,
Khaeng Suan Luang, Khet Suan Luang,
Bangkok 10250 Thailand.

RECEIVED DATE : 05 Feb 2024
MEASUREMENT DATE : 05 Feb 2024
ISSUE DATE : 07 Feb 2024

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:
The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

Traceability:
The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0038-23, Certificate number: ER-0101-23

Reference Used During Calibration:

1. Standard Temperature Probe
Model: STS-100 A500, Serial No.: 667682-09,
Due date: 28 Mar 2024
2. Digital Temperature Indicator
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$. Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM Evaluation of measurement data - Guide to the expression of uncertainty in measurement.

REVIEW BY: *Handorn P.*
APPROVED BY: *[Signature]*
NEXT CAL. DATE: 4/1/25



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jittaporn Lertsomphol
☐ Miss Ruangrumpal Poommitt

THIS CERTIFICATE MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

Continuation of Certificate of Calibration Number CDT-036-67

Page 2 of 2 Pages

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 ~ 40 °C

Function:

Table 1: This equipment was connected with wet bulb probe Model: HP3201.2 S/N: 21001210.
Dimension: Diameter 3.3 mm. Length 170 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
80	20.048	20.0	0.0	0.099
80	25.054	25.0	-0.1	0.099
80	30.047	30.0	0.0	0.099
80	35.038	35.0	0.0	0.099
80	40.035	40.0	0.0	0.099

Table 2: This equipment was connected with Globe thermometer probe Model: TP3276.2 S/N: 21001236.
Dimension: Diameter 3.3 mm. Length 205 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
110	20.048	20.0	0.0	0.099
110	25.054	25.0	-0.1	0.099
110	30.047	30.0	0.0	0.099
110	35.038	35.0	0.0	0.099
110	40.035	40.0	0.0	0.099

Table 3: This equipment was connected with temperature probe Model: TP3207.2 S/N: 21001789.
Dimension: Diameter 14 mm. Length 150 mm.

Immersion Depth (mm)	Standard Reading (°C)	UUC Reading (°C)	Error (°C)	Uncertainty (°C)
75	20.048	20.2	0.2	0.099
75	25.054	25.1	0.0	0.099
75	30.047	30.0	0.0	0.099
75	35.038	34.8	-0.2	0.099
75	40.035	39.8	-0.2	0.099

UUC*: Unit Under Calibration

End of Certificate of Calibration





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
5344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 24PH145
Page: 1 of 2

Equipment: Lux Meter
Manufacturer: Tenmars
Model: TM-201L
Serial No.: 190702490
ID No.: RYG_FS0471
Condition As-Received: Used Item
Received Date: 12 March 2024
Calibration Date: 14 March 2024
Reference: 2403-0392WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.



Submitted by: ALS Laboratory Group (Thailand) Co., Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-PH01 based on inverse square law technique.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Photometry & Encoder	LMguide 9,6 m	120RC003	DL-0064-22	20 Jul 2025
2) Luminous intensity standard lamp	OL FEL-U	F-1543	TP-1030-23	08 Jun 2024

2. This result of calibration was made on requested at the point specified by customer.

3. Test Equipment: Programmable Voltage/Current Source (Model: OL83A, SN: 16221394).

4. Test Equipment: Illuminance Meter (Model: 51002, SN: 080129).

5. The certificate is valid only to the item calibrated on date and place of calibration.

6. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by: Nivat Nitas
Issue Date: 18 March 2024

Approved Signatory:

[] Phalinee Prabpaipal
[] Wanlop Larpkern
[x] Nuntawat Khanchai

B 0337449



Cert. No.: 24PH145
Page.: 2 of 2

Result of calibration:- () Without adjustment (*) After adjustment

Function : Illuminance Measurement	Range :	200	lx
<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>
(lx)	(lx)	(lx)	(± lx)
0	0.0	0.0	-
20	20.1	0.1	0.26
50	50.0	0.0	0.65
100	100.0	0.0	1.3
150	150.0	0.0	2.0
190	190.0	0.0	2.5

Function : Illuminance Measurement	Range :	2000 lx	
<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>
(lx)	(lx)	(lx)	(± lx)
200	199	-1	2.6
500	499	-1	6.5
1000	1000	0	13
1500	1501	1	20
1900	1901	1	25

Function : Illuminance Measurement		Range :	20000	lx
<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>	
(lx)	(lx)	(lx)	(± lx)	
2000	1990	-10	26	
3000	3000	0	39	
4000	4000	0	52	
5000	5000	0	65	

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %

UUC* = Unit Under Calibration.

-000-

a 1206570



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
5344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 23PH628
Page: 1 of 2

Equipment: Lux Meter
Manufacturer: PEAK METER
Model: PM8612L
Serial No.: H12A-D16324
ID No.: RYG_FS0536
Condition As-Received: Used Item
Received Date: 27 November 2023
Calibration Date: 28 November 2023
Reference: 2311-0889WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co., Ltd.

104 Phatthanakan 40, Phatthanakan Rd.,
Khwaeng Phatthanakan, Khet Suan Luang,
Bangkok 10250 Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-PH01 based on inverse square law technique.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Photometry & Encoder	LMguide 9,6 m	120RC003	DL-0064-22	20 Jul 2025
2) High-accuracy Irradiance Standard	OL-FEL-U	F-1473	TP-1028-23	14 Feb 2024

2. This result of calibration was made on requested at the point specified by customer.

3. Test Equipment: Programmable Voltage/Current Source (Model: OL83A, SN: 16221394).

4. Test Equipment: Illuminance Meter (Model: 51002, SN: 080129).

5. The certificate is valid only to the item calibrated on date and place of calibration.

6. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by: Nivat Nitas
Issue Date: 30 November 2023

Approved Signatory:

[] Phalinee Prabpaipal
[] Chatchawan Khunpilaek
[x] Nuntawat Khanchai

B 0330105



Cert. No.: 23PH628
Page.: 2 of 2

Result of calibration:- () Without adjustment (*) After adjustment

Function : Illuminance Measurement		Range : Autorange		
Standard Value	Before Adjust UUC* Reading	After Adjust UUC* Reading	Error	Uncertainty
(lx)	(lx)	(lx)	(lx)	(± lx)
0	0.00	0.00	0.00	-
15	-	14.79	-0.21	0.20
100	-	99.2	-0.8	1.3
500	-	500	0	6.5
1000	775	1005	5	13
2000	-	2013	13	26
3000	-	3030	30	39
4000	-	4040	40	52
5000	3900	5050	50	65

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %

Before adjustment light source factor setting mode: $L1 = 0.990$

After adjustment light source factor setting mode: $L1 = 1.284$

UUC* = Unit Under Calibration.

-000-

a 1192374



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
5344 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLIANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 23T2261
Page: 1 of 2

Cert. No.: 23T2261
Page: 2 of 2

Equipment: Digital Thermometer With Sensor
Manufacturer: Testo
Model: 106
Serial No.: 31281488/504
ID No.: RYG_FSO489
Condition As-Received: Used Item
Received Date: 08 December 2023
Calibration Date: 14 December 2023
Reference: 2312-0151DSC
Ambient Temperature: (25 ± 3) °C
Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1.Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Black Stack Thermometer	1560	8C454	238600	30 May 2024
2) PRT Scanner Module	2562	A01303	238600	30 May 2024
3) Industrial PRT Probe	5627A	979442	238600	30 May 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONS Accredited No. Calibration 0008

REVIEW BY *Prithiya Th*
APPROVED BY *Supt S*
NEXT CAL. DATE *30/12/24*

Calibrated by: Theerapong Ameen
Issue Date: 21 December 2023

Approved Signatory:

- ☐ Phalinee Prabpaipal
☐ Chatchawan Khunpluek
☒ Wanlop Larphem

B 0330901



Result of Calibration:-

Without Adjustment

Function: Temperature measurement

Dimension of probe: Diameter 3 mm., Length 55 mm. Sheath material: Stainless Steel

Immersion Depth (mm.)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)
45	25.0020	24.9	-0.1020	0.12
45	30.0028	29.9	-0.1028	0.24
45	40.0021	40.0	-0.0021	0.63

UUC*: Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

-000-

a 1194808



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
5344 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLIANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 23E3924
Page: 1 of 2

Cert. No.: 23E3924
Page: 2 of 2

Equipment: pH Meter
Manufacturer: Mettler Toledo
Model: SevenExcellence
Serial No.: B834291445
ID No.: RYG_EN0152
Condition As-Received: Used Item
Received Date: 08 December 2023
Calibration Date: 14 December 2023
Reference: 2312-0151DSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 10) %

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 according to EURAMET cg-15.

Condition of this result of calibration

1.Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Multi-Product Calibrator	5502A	2435802	EE-0041-23	26 Apr 2024

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

REVIEW BY *Ni.Bannit*
APPROVED BY *D.Bo*
NEXT CAL. DATE *30/12/24*

Calibrated by: Napachanok Prasomsosiri
Issue Date: 15 December 2023

Approved Signatory:

- ☐ Phalinee Prabpaipal
☒ Nuntawat Khamchai
☐ Pongsagorn Boonyaporn

B 0331106



Result of calibration:- (*) Without adjustment () After adjustment

Function: DC voltage measurement

Range: 2000 mV

Standard Value (mV)	UUC* Reading (mV)	Error (mV)	Uncertainty (± μV)
-200.0000	-199.9	0.1	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	50.0	0.0	61
100.0000	100.0	0.0	63
150.0000	150.0	0.0	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95 %

UUC*= Unit Under Calibration.

-000-

a 1193422



Cert.No.: 23CH1574
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Mettler Toledo
Model : SevenExcellence
Serial No. : B834291445
ID No. : RYG_EN0152
Condition As-Received: Used Item
Received Date : 08 December 2023
Calibration Date : 15 December 2023
Reference : 2312-0151DSC-3
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lemgagtrakul

Approved by :
Approved Signatory

() Salthip Meangmai
() Warakorn Lemgagtrakul
(✓) Ponpan Palpim

Issue Date : 19 December 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

A 0061696



Cert.No.: 23CH1574
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-
- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	913598	14 July 2025
pH 6.986	CPA chem	931959	01 Oct 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (mV)	Coverage factor k
			mV	pH		
pH Meter S/N.: B834291445	4.000	177.48	177.3	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

a 1193852



Cert.No.: 23CH1574
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor k
pH Electrode S/N.: 3225368	4.008	4.013	184.1	0.0045	2.00
	6.986	6.998	8.7	0.0084	2.00
	9.997	10.002	-164.7	0.0088	2.11

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : InLab®Expert Pro-ISM

- Serial No. : 3225368

Dimension of probe:

- Length : 120 mm

- Diameter : 12 mm

- Immersion Depth : 100 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
25.0	25.003	24.3	-0.703	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

a 1193851



Cert.No.: 23TW168
Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter

Manufacturer : YSI

Model : 5000-115V

Serial No. : 15E102796

ID No. : RYG_EN0032

Received Date : 21 July 2023

Test Date : 24 July 2023

Reference : 2307-0713DSC-1

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Rayong Branch
616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,
Rayong 21140, Thailand

Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %

Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method

Tested by : Walalak Sirithean

Approved by :
Approved Signatory

() Malee Butkruea
(✓) Salthip Meangmai
() Warakorn Lemgagtrakul

Issue Date : 26 July 2023

B 0320211



Cert.No.: 23TW168
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1126143764	140RC004	22MM50	20 Sep 2023

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 15E100464

Titration Method (Azide Modification Method)	DO Meter Reading	Standard Deviation
(mg/L)	(mg/L)	(mg/L)
8.18	8.17	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency. The environmental impact control and present to organization it may concerned intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory

-o0o-

Switjip

a 1172155



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert. No.: 23LM125
Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor
Manufacturer : YSI
Model : 5000-115V
Serial No. : 15E102796
ID No. : RYG_EN0032
Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
Rayong Branch
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng,
Rayong 21140 Thailand
Location : TPA On Site Calibration Laboratory
Received Order : 25 July 2023
Calibrated Date : 27 July 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V

Calibrated by : Preecha Hlahib

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Malee Butkruea
(✓) Suwit Imjai

Issue Date : 31 July 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0053616



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2307-0713DSC-2

Cert. No.: 23LM125
Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Digital Thermometer	2188080	2211285	TPA	21 Oct 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (°) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 1228475367

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
20.00	100	20.011	19.91	-0.101	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

Switjip

a 1159515



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert. No.: 23TM962
Page.: 1 of 3

Certificate of Calibration

Equipment : Low Temp. Incubator
Manufacturer : Memmert
Model : IPP750
Serial No. : V818.0084
ID No. : RYG_EN0154
Submitted by : ALS Laboratory Group (Thailand) Co., Ltd.
(Rayong Branch)
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand
BOD Room
Location :
Received Order : 29 May 2023
Calibration Date : 29 May 2023
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Malee Butkruea
(✓) Suwit Imjai

Issue Date : 7 June 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0054967



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2305-0898OC-2
Procedure Used :-

Cert. No.: 23TM962
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Data Acquisition	34972A	MY57013711	22LM93	02 Jul 2023


2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.60 m
W = 1.0 m
H = 1.2 m
Capacity = 0.75 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	23	23
REL Humid. (%)	54	56
AC Supply (Volt)	223	222

Position :	Ref. Std. ID No.:
1	18-18RTD-01
2	18-18RTD-02
3	18-18RTD-03
4	18-18RTD-04
5	18-18RTD-05
6	18-18RTD-10
7	18-18RTD-07
8	22-18RTD-08
9 (ref.)	18-18RTD-09

a 1165130



Equipment : Low Temp. Incubator
Condition As-Received : Used Item
Reference : 2305-0898OC-2
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 23TM962
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.0	20.0	0.019	0.72	1.0	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.547	19.780	19.487	19.529	19.408	20.139	20.112	20.406	20.116	0.30

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

a 1165129



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
5344 PATTANAKARN ROAD SOI 18, SUANLIANG, SUANLIANG BANGKOK 10250
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Cert.No.: 23CG3704
Page.: 1 of 2

Certificate of Calibration

Equipment : Burette

Capacity : 50 mL

Serial No. :

ID. No. : RYG_EN0216

Manufacturer :

Witeg

Made in :

Germany

Submitted by :

ALS Laboratory Group (Thailand) Co.,Ltd.
Rayong Branch
616/10 Moo 5, T.Maenam Khu
A.Pluakdaeng, Rayong 21140 Thailand

Ambient Temperature : (20 ± 2.5) °C

Relative Humidity : (50 ± 10) %

Barometric Pressure : 756 mmHg

Calibration Procedure : ASTM E 542 - 01

Calibrated by : Srisuda Khamtha

Approved by :

Suh.
Approved Signatory

() Ponpan Palpim
() Srisuda Khamtha
() Sa-ngeunkam Wongsa

Issue Date : 28 September 2023

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than as full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

A 0058881



Equipment : Burette
Received Date : 19 September 2023
Condition As-Received : Used Item
Calibration Date : 25 September 2023
Reference : 2309-0635DSC-31

Cert.No.: 23CG3704
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	MS204TS	C226356983	140RC010	TH2068-012	METTLER	29 Sep 2023
2) Thermo-Hygrograph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	1594592	140EC010	23I158	TPA	12 Feb 2024

This certification is traceable to SI Unit

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
10	10.0224	0.0082	2.00
20	20.0064	0.0085	2.00
30	29.9931	0.0089	2.00
40	39.9910	0.0094	2.00
50	49.9806	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

a 1182477



SARTORIUS

Certificate of Calibration

REVIEW BY: *Thirakul*
APPROVED BY: *D. J. J.*
NEXT CAL DATE: 02/02/2025

Model Number: MSE224S-100-DU
Description: Analytical Balance
Serial Number: 0026207038
ID No.: RYG_EN0002
Manufacturer: Sartorius

Certificate No.: 24BC10069
Issued Date: Friday, February 23, 2024
Reference No.: 229196
Page No.: 1 of 2

Customer Name: ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140, Thailand.

Calibrated Place: ALS Laboratory Group (Thailand) Co., Ltd. (Balance Room)
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140, Thailand.

Calibrated By: Mr. Chonchai Inthana
Calibration Date: Thursday, February 22, 2024
Calibration Procedure No.: This calibration was conducted by
Using in-house calibration procedure number (WI-003)
Based on UKAS LAB 14: 2019

Metrological data:
Capacity: 220 g Readability: 0.0001 g
Reasons for calibration
☐ New Installation ☐ Service / Repair ☒ Re-calibration / Maintenance

Ambients Conditions:
Temperature: 24.2 °C ± 5.0 °C
Humidity: 57.0 % RH ± 10.0 % RH
Pressure: ±
Equipment Condition: ☒ Good Operate ☐ Fair

Measurement Method UKAS Publication Ref: Lab 14
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came from list of Sartorius Metrological Specifications.

Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2, YCS011-522-00	TCS	M2308197S	23-Aug-2025
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19231845	23-Aug-2024

This certificate relate and apply this equipment only.
This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division
Sartorius (Thailand) Co., Ltd.

Mr. Chonchai Inthana

Mr. Chonchai Inthana (Technical Manager)



SOP FM 33 03 February 2022

SARTORIUS

Certificate of Calibration

Model Number: MSE224S-100-DU
Description: Analytical Balance
Serial Number: 0026207038
ID No.: RYG_EN0002
Manufacturer: Sartorius

Certificate No.: 24BC10069
Issued Date: Friday, February 23, 2024
Reference No.: 229196
Page No.: 2 of 2

Calibration Results : Without Adjustment

Repeatability			Eccentricity (Off-center loading error)		
The reproducibility is the ability of a weighing instrument to display nearly identical readings under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.			The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).		
Nominal Value : (Low Load)	20.0000	199.9999	Nominal value :	100	g
20 g	20.0000	200.0000	Tolerance	0.0004	g
Tolerance	0.0001 g	200.0000			
20.0001	200.0000	200.0000			
Nominal Value : (High Load)	19.9999	200.0000			
200 g	20.0000	200.0000			
Tolerance	0.0001 g	199.9999			
19.9999	200.0001	200.0000			
19.9999	200.0000	200.0000			
Standard Deviation	0.00007	0.00006			

Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance		0.0002 g		
Nominal Value	Conventional Mass Value	Displayed Value	Deviation	Uncertainty
(g)	(g)	(g)	(g)	(g)
0.01	0.0100	0.0100	0.0000	0.00018
0.05	0.0500	0.0500	0.0000	0.00018
0.1	0.1000	0.1000	0.0000	0.00018
0.5	0.5000	0.5000	0.0000	0.00018
1	1.0000	1.0000	0.0000	0.00018
5	5.0000	5.0000	0.0000	0.00018
10	10.0000	10.0000	0.0000	0.00018
20	20.0000	20.0000	0.0000	0.00024
50	50.0000	49.9999	-0.0001	0.00019
100	100.0000	100.0000	0.0000	0.00023
200	200.0000	199.9999	-0.0001	0.00032

End of Report.

SOP FM 33 03 February 2022



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL: 0-2717-3000-29 FAX: 0-2719-9484



Certificate of Calibration

Cert. No.: 24TM632
Page: 1 of 3

Equipment: Hot Air Oven
Manufacturer: Memmert
Model: UFE 500
Serial No.: G511.1572
ID No.: RYG_EN0010

Submitted by: ALS Laboratory Group (Thailand) Co., Ltd. (Rayong Branch)
616/10 Moo 5 T. Maenam Khu, A. Pluakdaeng, Rayong 21140 Thailand
Location: Oven Room

Received Order: 21 March 2024
Calibration Date: 21 March 2024
Ambient Temperature: (26 ± 10) °C
Relative Humidity: (50 ± 30) %

Calibrated by: Man Pattanapongpaiboon

Approved by: *Man Pattanapongpaiboon*
Approved Signatory

Issue Date: 22 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.



Equipment: Hot Air Oven
Condition As-Received: Used Item
Reference: 2403-05630C-1
Procedure Used:-

Cert. No.: 24TM632
Page: 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark: TPA: Technology Promotion Association (Thailand - Japan)

Result of Calibration:- (*) Without Adjustment

Function of UUC:- Temperature Source

Fresh air setting: Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	27	27
REL. Humid. (%)	57	59
AC Supply (Volt)	222	224



Probe Installation Details: Dimension of Chamber:
a = 5.0 cm D = 0.40 m
b = 5.0 cm W = 0.56 m
c = 5.0 cm H = 0.48 m
Capacity = 0.11 m³

Ref. Std. ID No.: @ Calibration Point		
Position:	(180) °C	(104) °C
1	18-18TC-01	18-18RTD-01
2	18-18TC-02	18-18RTD-02
3	18-18TC-03	18-18RTD-03
4	18-18TC-04	18-18RTD-04
5	18-18TC-05	18-18RTD-05
6	18-18TC-06	23-18RTD-06
7	18-18TC-07	18-18RTD-07
8	18-18TC-08	22-18RTD-08
9 (ref.)	18-18TC-09	18-18RTD-09



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2403-0563OC-1
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM632
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
104.0	104.0	104.0	0.051	0.59	0.62	2
180.0	180.0	180.0	0.15	1.3	1.7	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	103.921	103.786	103.757	103.759	103.950	103.817	104.213	103.672	103.673	0.42
180.0	179.614	179.270	179.145	179.599	180.001	180.423	180.293	180.629	179.429	1.1

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24TM634
Page : 1 of 3

Equipment : Hot Air Oven
Manufacturer : Memmert
Model : UF 110
Serial No. : B423.0853
ID No. : RYG_EN0213

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T. Maenam Khu,
A. Pluakdaeng,
Rayong 21140 Thailand

Location : Oven Room

Received Order : 21 March 2024
Calibration Date : 21 - 22 March 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Suwit Imjai

Issue Date : 23 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2403-0563OC-3

Cert. No.: 24TM634
Page : 2 of 3

Procedure Used :- Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-


Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close



Probe Installation Details : Dimension of Chamber :
a = 5.0 cm D = 0.40 m
b = 5.0 cm W = 0.56 m
c = 5.0 cm H = 0.48 m
Capacity = 0.11 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	27	27
REL.Humid. (%)	59	59
AC Supply (Volt)	224	223

Ref. Std. ID No.: @ Calibration Point		
Position :	(180) °C	(104) °C
1	18-18TC-01	18-18RTD-01
2	18-18TC-02	18-18RTD-02
3	18-18TC-03	18-18RTD-03
4	18-18TC-04	18-18RTD-04
5	18-18TC-05	18-18RTD-05
6	18-18TC-06	23-18RTD-06
7	18-18TC-07	18-18RTD-07
8	18-18TC-08	22-18RTD-08
9 (ref.)	18-18TC-09	18-18RTD-09



Equipment : Hot Air Oven
Condition As-Received : Used Item
Reference : 2403-0563OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Close

Cert. No.: 24TM634
Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
104.0	104.0	104.0	0.065	0.52	0.90	2
180.0	180.0	180.0	0.20	1.2	2.0	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	104.169	103.506	103.898	103.712	103.772	103.730	104.289	103.805	103.798	0.42
180.0	180.701	179.239	179.935	179.999	180.127	180.138	180.895	179.313	180.211	1.1

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-



Certificate of Calibration

Cert. No.: 24TM635
Page : 1 of 3

Equipment : Water Bath
Manufacturer : Memmert
Model : WNB22
Serial No. : L513.0648
ID No. : RYG_EN0061

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5, T. Maenam Khu,
A. Pluakdaeng,
Rayong 21140, Thailand

Location : Wet Chemistry Lab

Received Order : 21 March 2024

Calibration Date : 21 March 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

Calibrated by : Man Pattanapongpaiboon

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Suwit Imjai

Issue Date : 23 March 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2403-0563OC-4
Procedure Used :-

Cert. No.: 24TM635
Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply
	(°C)	(%R.H.)	(Volt)
Beginning of Calibration	25	55	222
Finished of Calibration	25	57	223



Front

Position :	Ref. Std. ID No.:
1	4803988-001
2	4803988-002
3	4803988-003
4	4803988-004
5(ref.)	4803988-005



Equipment : Water Bath
Condition As-Received : Used Item
Reference : 2403-0563OC-4
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source

Cert. No.: 24TM635
Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
85.0	85.0	85.0	84.428	84.424	84.489	84.507	84.477	0.18

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor k
85.0	0.19	0.11	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-



Cert.No.: 23CG3704
Page.: 1 of 2

Certificate of Calibration

Equipment : Burette
Capacity : 50 mL
Serial No. : -
ID. No. : RYG_EN0216
Manufacturer : Witeg
Made in : Germany
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Rayong Branch
616/10 Moo 5, T.Maenam Khu
A.Pluaekdaeng, Rayong 21140 Thailand

Ambient Temperature : (20 ± 2.5) °C
Relative Humidity : (50 ± 10) %
Barometric Pressure : 756 mmHg
Calibration Procedure : ASTM E 542 - 01

Calibrated by : Srisuda Khamtha

Approved by :
Approved Signatory

() Ponpan Paipim
(✓) Srisuda Khamtha
() Sa-ngeunkam Wongsa

Issue Date : 28 September 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

Certificate of Calibration

Represent to Certificate of Calibration No. C29240007

Equipment: Block Digestion Unit Certificate No.: C29240011
Model: KT-20s Issued Date: 22 March 2024
Serial No. (or ID.): 5720210009/5770200073 Job No.: WO-00020429
Manufacturer: Gerhardt Page: 1 of 4
Condition: In Condition Digestion Block: 20 holes.

Customer: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Environment Condition: Temperature: 25 °C ± 0.7 °C
Humidity: 54 %RH ± 4.1 %RH
Voltage: 225 VAC ± 1.7 VAC

REVIEW BY: N. Benet
APPROVED BY: [Signature]
NEXT CAL DATE: 11/09/25

Calibration Place: ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)
(Wet Chemistry Lab)
616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand.

Calibration By: Mr. Thanathorn Phunook
Calibration Date: 11 March 2024
The Method used: In house method, base on by comparison with standard
Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through N.M. Technical Center Laboratory (NTL) Certificate No.: TC22/0080

[Signature]
(Mr. Thanathorn Phunook)

[Signature]
(Mr. Udon Srichana)

Person in charge
This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C29-07: 20 Jul 2022



Equipment: Burette
Received Date: 19 September 2023
Condition As-Received: Used Item
Calibration Date: 25 September 2023
Reference: 2309-0635DSC-31

Cert.No.: 23CG3704
Page: 2 of 2

Condition of this result of calibration

- Reference Standard Instruments :

Instruments	Model	Serial No.	ID. No.	Certificate No.	Traceability	Due date
1) Balance	MS204TS	C226356983	140RC010	TH2068-012	METTLER	29 Sep 2023
2) Thermo-Hygraph	THDX-CE	00016540	140EC001	23H1275	TPA	09 June 2024
3) Thermometer	-	1594592	140EC010	231158	TPA	12 Feb 2024

This certification is traceable to SI Unit

- The certificate is valid only to the item calibrated on date and place of calibration.
- True value is converted to true volume at the standard temperature of 20 °C

Calibration result :

Nominal capacity (mL)	Reading (mL)	Uncertainty (± mL)	k Factor
10	10.0224	0.0082	2.00
20	20.0064	0.0085	2.00
30	29.9931	0.0089	2.00
40	39.9910	0.0094	2.00
50	49.9806	0.010	2.00

Remark mL = cm³

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-

a 1182477

Certificate No.: C29240011

Page: 2 of 4





Fig. 1.: Front view



Location of standard

Fig. 2.: Digestion block

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the Digestion block.

Measured Temperature: The average reading of working standard at any positions or location.

Certificate No.: C29240011

Page: 3 of 4

Calibration Results:

Pre Calibration

Locations	Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
A1				401.5	21.5	1.5
A2				401.2	21.2	1.5
A3				399.1	19.1	1.5
A4				397.8	17.8	1.5
A5				395.1	15.1	1.5
B1				396.6	16.6	1.5
B2				396.1	16.1	1.5
B3				392.9	12.9	1.5
B4				391.6	11.6	1.5
B5				390.7	10.7	1.5
C1	380	380	380	395.3	15.3	1.5
C2				395.6	15.6	1.5
C3				392.8	12.8	1.5
C4				391.7	11.7	1.5
C5				390.3	10.3	1.5
D1				397.6	17.6	1.5
D2				396.6	16.6	1.5
D3				395.0	15.0	1.5
D4				394.2	14.2	1.5
D5				393.6	13.6	1.5

Calibration Results:
Without adjustment

Locations	Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature (°C)	Correction of UUC. (°C)	Uncertainty (± °C)
A1	380	365	365	382.5	17.5	1.5
A2				382.4	17.4	1.5
A3				382.1	17.1	1.5
A4				379.7	14.7	1.5
A5				378.3	13.3	1.5
B1				380.1	15.1	1.5
B2				380.1	15.1	1.5
B3				378.5	13.5	1.5
B4				378.3	13.3	1.5
B5				379.1	14.1	1.5
C1				380.1	15.1	1.5
C2				380.1	15.1	1.5
C3				378.9	13.9	1.5
C4				378.2	13.2	1.5
C5				377.3	12.3	1.5
D1				380.5	15.5	1.5
D2				380.6	15.6	1.5
D3				378.1	13.1	1.5
D4				378.7	13.7	1.5
D5				377.7	12.7	1.5

The End of Certificate

ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: WO-00020429

ชนิดเครื่องมือ: Block Digestion Unit รุ่น: KT-20s
หมายเลขเครื่อง: 5720210009/5770200073

ตรวจสอบ (รับ)	ตรวจสอบ (ส่ง)	หมายเหตุ
11 Mar 2024	11 Mar 2024	
ปกติ	ปกติ	
ไม่ปกติ	ไม่ปกติ	
General		
<input type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ
<input type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch
<input type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key
<input type="checkbox"/>	<input type="checkbox"/>	4. การแสดงผล Display
<input type="checkbox"/>	<input type="checkbox"/>	5. สภาพ Hole
<input type="checkbox"/>	<input type="checkbox"/>	6. สภาพฝาปิด
<input type="checkbox"/>	<input type="checkbox"/>	7. สภาพตัวเครื่อง
<input type="checkbox"/>	<input type="checkbox"/>	8. สภาพแวดล้อม ณ สถานที่ตั้งเครื่อง

ชื่อแนะนำ :

Mr. Thanathorn Phunook
Service Engineer

BKK_EL0026



Agilent Technologies (Thailand) Limited
U CHU LIANG BLDG. 22/F UNIT A.D
968 RAMA 4 ROAD, SILOM, BANGKOK
Bangkok 10500 Thailand
Tel: +662 637 6363
Fax: +662 632 4334
Email: ccc-sm@agilent.com
Website: www.agilent.com/csm

Customer Contact:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan
TAX ID: 0105540004859
Chanattagarn.lmchom@alsglobal.com
27893068

Invoice To:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Delivery Site:

ALS Laboratory Group (Thailand) Co
Ltd
Head Office
104 Phatthanakan 40 Phatthanakan Rd
Khwaeng Phatthanakan Khet Suan

Location:
Room
Bldg
Lab
Dept

SERVICE REPORT

Customer Purchase Order Number:	Customer Number: 70371013
Service Request:	Service Request Date:
Service Order: 6006041263	Service Confirmation: 6905338201



Direct Inquiries to:

Contact Name: Customer Contact Center
Contact E-mail: ccc-sm@agilent.com
Contact Telephone: +662 637 6363
Contact Fax: +662 632 4334

Learn more about Agilent's Special Offers, Products, Services and our
full range of laboratory productivity solutions optimized for your
applications and workflows. Visit us at www.agilent.com/csm

Original
Cibank N.A. Bangkok Branch
380 Interchange 21 Building, Sukhumvit Road, Khlongtoei New
Sub-district, Wattana District, Bangkok 10110 Thailand
Attn: Mr. 612-4452-007
THB Krung Thai Bank PCL
Siam Square Bldg. A16/1-2 Rama 1 Rd, Pathumwan, BKK 10330
Thailand

Service Confirmation Number: 6905338201
Service Confirmation Date: 12.12.2023

Service Instrument:



Model Number	Model Description	Serial Number	System Handle	Parent Asset
SYS-IM- 7700-E	ICPMS 7700 System Enhanced		ICP MS 7700 (HPLC)	
G1316A	1260 Thermostatted Column Compartment	DEACN12300	ICP MS 7700 (HPLC)	SYS-IM-7700-E
G1329B	1260 Standard Autosampler	DEAAC11098	ICP MS 7700 (HPLC)	SYS-IM-7700-E
G1311B	1260 Quaternary Pump	DEAB704380	ICP MS 7700 (HPLC)	SYS-IM-7700-E
G3281A	Agilent 7700x ICP-MS	JP12091612	ICP MS 7700 (HPLC)	SYS-IM-7700-E

Service Items:

Item	Service/Part #	Description	Qty	Entitlement	Service Start	Service End
1000	EQQ	Enterprise Operational Qualification	1.00	Agreement Entitlement 100 % covered	12.12.2023	12.12.2023
1010	5185-5850	ICP-MS Checkout Solutions	1.00	Agreement Entitlement 100 % covered		

Additional Information:

Service Information:

Problem Description: WU-OQ-IM/HPLC-7700-6001143313		
Service Provided: Perform OQ Hardware control test CSO Ilogon, Autosample, ISIS, Auto tune, BG and Stability. After done the instrument BKK_EL0026 calibrated pass all.		
Service Overview Code: Reason Code: Scheduled Service Diagnosis Code: Scheduled Service Resolution Code: Scheduled Service		
Reported Hours: 6.0	Travel Hours: 1.0	
Customer Field Service Representative Name: Pantep Kurasathain	Customer Field Service Representative Signature: 	Date: 12 Dec 2023
Customer Name: Supakwan Mak	Customer Signature: 	Date: 12 Dec 2023
Additional Comments:		



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 1 of 6

Certificate of Calibration

Equipment : HEATING BLOCK
Manufacturer : Environmental Express
Model : SC 196
Serial No. : 6974CECW3285
Customer Code : BKK_EL0054
ID No. : T5306A3
Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250
Customer Location : Acid Digestion Lab
Date of Receipt : 13 September 2023
Calibrated By : Sancee Musikawan (Site Calibration Manager)
Approved By :  / Sujjar Naknakred (Site Calibration Manager)
Date of Issue : 26 SEP 2023

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrological Center.

FM-L12 109/30-05-57



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109

Website : www.scieco.co.th E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 2 of 6

Calibration Report

Equipment : HEATING BLOCK
Date of Calibration : 22 September 2023
Environment : Temperature : 21.8-23.1 °C
Line Voltage : 221.6-226.3 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 20 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement , The calibration was done in according to WI-T20.

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN21-TN30	T230014	17 January 2024
TC	TYPE T	TN31-TN40	T230014	17 January 2024
DATA LOGGER	34970A	T151	T230014	17 January 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant : 2 Hour 20 Minute At 95 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

() without adjustment (X) after adjustment

Approved By. 



Metrological Center

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110

Telephone : +66 2 586 5792-4 Fax : +66 2 586 5109


Website : www.scieco.co.th

E-Mail : calibrate@scg.co.th

Certificate No. T231676

Page 3 of 6

Calibration Report

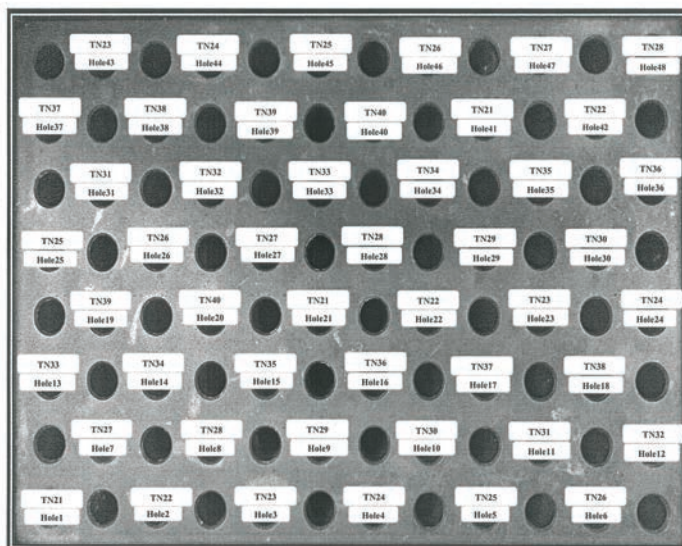

FRONT CONTROL

Approved By. 



Certificate No T231676

Page 4 of 6

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT	Max	95.01	94.41	95.20	95.41	94.51	95.17
	Min	94.57	93.95	94.75	94.92	94.00	94.72
	Average	94.79	94.18	94.98	95.17	94.26	94.95
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
Max	95.36	95.43	95.19	95.16	95.35	94.97	
	Min	94.94	94.95	94.72	94.71	94.90	94.57
	Average	95.15	95.19	94.96	94.94	95.13	94.77
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
Max	95.37	95.50	95.22	95.21	95.33	95.31	
	Min	94.99	95.09	94.78	94.82	94.88	94.96
	Average	95.18	95.30	95.00	95.02	95.11	95.13
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
Max	95.59	94.42	94.52	94.24	94.63	94.67	
	Min	95.21	94.06	94.13	93.88	94.28	94.27
	Average	95.40	94.24	94.33	94.06	94.45	94.47
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
Max	95.19	95.38	92.93	95.30	95.14	95.03	
	Min	94.83	95.03	92.56	94.95	94.79	94.70
	Average	95.01	95.20	92.75	95.12	94.96	94.87
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
Max	94.63	94.90	94.77	94.31	94.24	93.87	
	Min	94.24	94.55	94.44	93.98	93.92	93.56
	Average	94.43	94.72	94.60	94.14	94.08	93.71
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
Max	94.30	94.44	94.04	93.81	94.89	95.35	
	Min	93.95	94.05	93.67	93.48	94.39	94.90
	Average	94.13	94.24	93.86	93.65	94.64	95.12
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
Max	95.99	95.63	95.28	95.29	95.45	94.87	
	Min	95.57	95.15	94.82	94.84	94.99	94.48
	Average	95.78	95.39	95.05	95.07	95.22	94.68

Approved By.

FM-L13 108/30-05-57



Certificate No T231676

Page 5 of 6

Calibration Report

Measurement Results

Calibration Point		Average Standard Reading at each position (°C)					
R1 Hole1-Hole6		TN21	TN22	TN23	TN24	TN25	TN26
CAL POINT	Max	105.23	104.32	105.43	105.25	104.44	105.27
	Min	104.94	103.95	105.15	105.04	104.11	104.96
	Average	105.09	104.13	105.29	105.15	104.28	105.12
R2 Hole7-Hole12		TN27	TN28	TN29	TN30	TN31	TN32
Max	105.30	105.12	105.18	105.22	105.12	105.16	
	Min	105.11	104.92	104.96	105.00	104.92	104.97
	Average	105.20	105.02	105.07	105.11	105.02	105.06
R3 Hole13-Hole18		TN33	TN34	TN35	TN36	TN37	TN38
Max	105.37	105.63	105.02	104.80	104.69	105.19	
	Min	105.17	105.37	104.75	104.59	104.50	105.00
	Average	105.27	105.50	104.88	104.69	104.60	105.09
R4 Hole19-Hole24		TN39	TN40	TN21	TN22	TN23	TN24
Max	105.31	104.43	106.41	104.71	105.63	105.82	
	Min	105.08	104.22	106.15	104.41	105.37	105.56
	Average	105.19	104.33	106.28	104.56	105.50	105.69
R5 Hole25-Hole30		TN25	TN26	TN27	TN28	TN29	TN30
Max	104.95	106.26	103.34	105.78	105.59	105.87	
	Min	104.67	105.96	103.08	105.56	105.36	105.68
	Average	104.81	106.11	103.21	105.67	105.48	105.77
R6 Hole31-Hole36		TN31	TN32	TN33	TN34	TN35	TN36
Max	104.75	104.86	104.80	105.20	104.50	104.39	
	Min	104.54	104.63	104.59	105.00	104.32	104.18
	Average	104.65	104.75	104.69	105.10	104.41	104.28
R7 Hole37-Hole42		TN37	TN38	TN39	TN40	TN21	TN22
Max	104.30	104.90	104.85	104.65	104.88	104.85	
	Min	104.09	104.72	104.66	104.49	104.63	104.52
	Average	104.19	104.81	104.75	104.57	104.76	104.68
R8 Hole43-Hole48		TN23	TN24	TN25	TN26	TN27	TN28
Max	105.71	105.85	105.39	105.61	105.42	105.19	
	Min	105.45	105.61	105.14	105.27	105.18	104.94
	Average	105.58	105.73	105.27	105.44	105.30	105.07

Approved By.

FM-L13 108/30-05-57



Certificate No. T231676

Page 6 of 6

Calibration Report

Measurement Results:

HEATING BLOCK			Temperature Distribution	
Setting (°C)	Reading (°C)		Stability (± °C)	Uncertainty (± °C)
	Min , Max	Average		
100.0	100.3 , 100.5	100.4	0.26	0.81
107.0	107.0 , 107.1	107.1	0.19	0.78

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

FM-L13 108/30-05-57



Certificate No. T232160

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cooling Room)

Manufacturer : KOLDTECH

Model : KM 320

Serial No. : TBN-1012061/05

Customer Code : BKK_EN0167

ID No. : T2463A3

Customer : ALS Laboratory Group (Thailand) Co.,Ltd.
104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan,
Khet Suan Luang, Bangkok 10250

Customer Location : Laboratory

Date of Receipt : 29 November 2023

Calibrated By : Atiphong Rongrat (Technician)

Approved By : / Boonchai Suriyawong (Site Calibration Manager)

Date of Issue : 09 JAN 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.

FM-L14 119/18-08-66

Certificate No. T232160

Page 2 of 4

Calibration Report

Equipment : Chamber (Cooling Room)
Date of Calibration : 6 December 2023
Environment : Temperature : 23.4-24.9 °C
Line Voltage : 221.4-230.2 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

- This equipment was calibrated by insert 16 standard thermocouples type T into its chamber, the other one standard thermocouples type T use for ambient temperature measurement. The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986). All data show below were final values and the initial data from customer request. The temperature scale used was based on ITS - 90.
- Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T230773	10 April 2024
TC	TYPE T	TN171-TN180	T230773	10 April 2024
DATA LOGGER	34970A	T149	T230773	10 April 2024
- This certificate is traceable to :
National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244).
- Condition of calibrated item : good
Equipment Description :
Time Constant 1 Hour 30 Minute At 3 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available
- Adjustment :
(X) without adjustment () after adjustment


Approved By. 

FM-L15 118/18-08-66

Certificate No. T232160

Page 3 of 4

Calibration Report

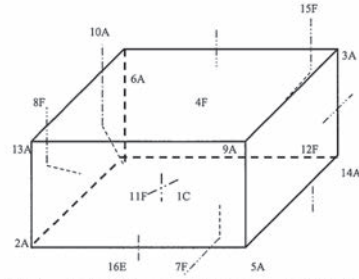

C = Centre, F = Centre of Face, A = Corner, E = Centre of Edge

1C = TN161	12F = TN172
2A = TN162	13A = TN173
3A = TN163	14A = TN174
4F = TN164	15F = TN175
5A = TN165	16E = TN176
6A = TN166	
7F = TN167	
8F = TN168	
9A = TN169	
10A = TN170	
11F = TN171	

Approved By. 

FM-L15 118/18-08-66

Certificate No. T232160

Page 4 of 4

Calibration Report

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)											
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170	TN171	TN172
3.0	2.83	3.34	2.95	3.46	3.45	3.76	3.25	3.46	3.39	3.50	3.58	3.42
	TN173	TN174	TN175	TN176								
	3.33	3.39	3.15	3.43								

Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor k
	Min, Max	Average					
3.0	2.8, 4.1	3.5	3.36	1.10	2.00	1.90	2.09

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k which for a t-distribution, providing a level of confidence of approximately 95 %.

Approved By. 

FM-L15 118/18-08-66