ภาคผนวก ง

ข้อมูลการตรวจเทียบเครื่องมือ

(Calibration Data Sheets)

Sheet No. : CAL-M5006/01/24

CONTROL UNIT CALIBRATION
(Metric units, mm)

Date 6 Jan 24

	Initial	Final	Average	
Barometric press, Pb	759	759	759	mmHg

Dry Gas Meter Data

Console No. M50-06

Metering System ID

DGM Number 917415

DGM Model MST-C2-1

Calibrated by : Montri P.

Reference Dry Gas Meter Data

Serial No. 358794

Model S110

Correction factor (Yr) 1.0068

Last Calibration Date 26 Oct 23

Orifice manometer setting, ΔH mm H2O	Ref. DGM Volume V_r Liters	DGM Volume V_m Liters	Temperature (^{O}C) Ref DGM T_r	Dry Gas Meter Inlet T_i	Dry Gas Meter Outlet T_o	Dry Gas Meter Avg T_m	Time Θ min	DGM Correction factor (Y)	ΔH@ mm
12.5	100.2	101.7	25	25	24	24.5	8.87	0.9901	44.4570
25.0	100.1	102.0	25	25	24	24.5	6.52	0.9854	48.0383
50.0	100.3	101.1	25	25	24	24.5	4.72	0.9935	50.1707
76.0	99.3	99.3	25	25	24	24.5	3.70	0.9987	47.9159
100.0	100.1	101.6	25	25	24	24.5	3.70	0.9816	49.8135
150.0	100.2	100.2	25	25	24	24.5	2.67	0.9919	48.1679
						Average		0.9902	48.0939

Approved by :

SECOT CO., LTD.
239 Rimklongprapa Rd. Bangsue, Bangkok, 10800, THAILAND
Tel: (662) 9593600 Fax: (662) 9593535
E-Mail: envserv@secot.co.th

Sheet No. : CAL-M5007/01/24

CONTROL UNIT CALIBRATION
(Metric units, mm)

Date 12 Jan 24

	Initial	Final	Average	
Barometric press, Pb	758	758	758	mmHg

Dry Gas Meter Data

Console No. M50-07

Metering System ID

DGM Number 90331

DGM Model MST-C2-1

Calibrated by Montri P.

Reference Dry Gas Meter Data

Serial No. 358794

Model S110

Correction factor (Yr) 1.0068

Last Calibration Date 26 Oct 23

Orifice manometer setting, ΔH mm H2O	Ref. DGM Volume V_r Liters	DGM Volume V_m Liters	Temperature (^{O}C) Ref DGM T_r	Dry Gas Meter Inlet T_i	Dry Gas Meter Outlet T_o	Dry Gas Meter Avg T_m	Time Θ min	DGM Correction factor (Y)	ΔH@ mm
12.5	100.0	100.6	25	25	24	24.5	9.72	0.9981	53.7523
25.0	100.2	100.2	25	25	24	24.5	6.48	1.0029	47.6709
50.0	100.0	100.8	25	25	24	24.5	4.77	0.9919	51.7327
76.0	100.2	100.9	25	25	24	24.5	3.90	0.9908	52.4606
100.0	100.1	99.6	25	25	24	24.5	3.90	1.0005	53.0627
150.0	100.2	98.9	25	25	24	24.5	2.82	1.0032	54.0289
						Average		0.9979	52.1180

Approved by :

SECOT CO., LTD.
239 Rimklongprapa Rd. Bangsue, Bangkok, 10800, THAILAND
Tel: (662) 9593600 Fax: (662) 9593535
E-Mail: envserv@secot.co.th

Sheet No. : CAL-PI-PS20-01/2024

PITOT TUBE CALIBRATION

Calibration Location: SECOT
Calibration Date : 09-01-2024
Calibration Duct No.: CD-0123

Calibration Standard Pitot tube data
Pitot No. : Std-02
Coefficient (Cp) : 0.99
Type S Pitot No. : PS20-01

Calibrated by : Mr. Montri P.

A Side Calibration

Run No.	ΔPstd ($mm H_2O$)	ΔPs ($mm H_2O$)	Cp(s)	Deviation,δ Cp(s) -Cp(A)
1	15.00	21.50	0.8269	-0.0065
2	15.00	21.00	0.8367	0.0033
3	15.00	21.00	0.8367	0.0033

$C_{P(A)}$,avg = 0.8334

B Side Calibration

Run No.	ΔPstd ($mm H_2O$)	ΔPs ($mm H_2O$)	Cp(s)	Deviation,δ Cp(s) -Cp(B)
1	15.00	21.00	0.8367	0.0065
2	15.00	21.50	0.8269	-0.0033
3	15.00	21.50	0.8269	-0.0033

$C_{P(B)}$,avg = 0.8302

| CP(A)-CP(B) | = 0.0033
$C_{P(Avg)}$ = 0.8318

Approved by : _____

*** δ must be ≤ 0.01 for the test to be acceptable ***
*** | Cp(A)-Cp(B) | must also be < 0.01 if average of Cp(A) and Cp(B) is ot be used ***

SECOT CO., LTD.
239 Rimklongprapa Rd. Bangsue, Bangkok, 10800, THAILAND
Tel: (662) 9593600 Fax: (662) 9593535
E-Mail: envser@secot.th.com

Sheet No. : CAL-PI-LL10-01/2024

PITOT TUBE CALIBRATION

Calibration Location: SECOT
Calibration Date : 09-01-2024
Calibration Duct No.: CD-0123

Calibration Standard Pitot tube data
Pitot No. : Std-02
Coefficient (Cp) : 0.99
Type S Pitot No. : LL10-01

Calibrated by : Mr. Montri P.

A Side Calibration

Run No.	ΔPstd ($mm H_2O$)	ΔPs ($mm H_2O$)	Cp(s)	Deviation,δ Cp(s) -Cp(A)
1	15.00	20.50	0.8468	0.0000
2	15.00	20.50	0.8468	0.0000
3	15.00	20.50	0.8468	0.0000

$C_{P(A)}$,avg = 0.8468

B Side Calibration

Run No.	ΔPstd ($mm H_2O$)	ΔPs ($mm H_2O$)	Cp(s)	Deviation,δ Cp(s) -Cp(B)
1	15.00	20.50	0.8468	0.0000
2	15.00	20.50	0.8468	0.0000
3	15.00	20.50	0.8468	0.0000

$C_{P(B)}$,avg = 0.8468

| CP(A)-CP(B) | = 0.0000
$C_{P(Avg)}$ = 0.8468

Approved by : _____

*** δ must be ≤ 0.01 for the test to be acceptable ***
*** | Cp(A)-Cp(B) | must also be < 0.01 if average of Cp(A) and Cp(B) is ot be used ***

SECOT CO., LTD.
239 Rimklongprapa Rd. Bangsue, Bangkok, 10800, THAILAND
Tel: (662) 9593600 Fax: (662) 9593535
E-Mail: envser@secot.th.com

ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT
975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917

NSC-TISI-TIS 17025
CALIBRATION 0119

Certificate No.: CP20230345EA
Operation No.: CP2023080023

Certificate of Calibration

Equipment:	Sound Calibrator
Manufacturer:	Cirrus Research Plc
Model/Type:	CR:515
Serial No.:	97097
ID No.:	-
Customer:	SECOT Co.,Ltd.
Address:	239 Rimklongprapa Rd., Bangsue, Bangkok 10800 Thailand
Received Date:	28 August 2023
Calibrated Date:	4 September 2023
Issued Date:	8 September 2023
Calibrated by:	Ms. Juntaporn Kunhakom

Approved by: _____
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20230345EA

Calibration Report

Equipment: Sound Calibrator
Manufacturer: Cirrus Research Plc
Model/Type: CR:515
Serial No.: 97097
ID No.: -
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa
Method of Calibration :-
IEC 60942:2017

Condition of this result of calibration

1. Reference standards instrument :-

	Instrument	Model	Serial No.	Cert. No.	Due Date
1)	Standard microphone	4180	2787490	AA-1024-22	6 November 2023
2)	Waveform Generator	33511B	MY52302264	CK20230039EA	27 June 2024
3)	Audio Analyzing DMM	2015-P	000136E	E1U225466	2 December 2023
4)	Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P230024 CD20230196EA	20 March 2024 23 July 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.
3. This certification is traceable to the international system of unit maintained at :-
   Reference standards instrument for Acoustic function
   - National Institute of Metrology (Thailand)
   Reference standards instrument for Electrical function
   - Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

1. Function : Sound pressure level

Norminal Frequency (Hz)	Specified Sound Pressure level (dB)	Measured value (dB)	Deviated value[1] (dB)	Acceptance limit[3] (dB)
1000	94	94.13	0.13	±0.25

2. Function : Frequency

Norminal Sound Pressure level (dB)	Specified Frequency (Hz)	Measured value (Hz)	Deviated value[2] (%)	Acceptance limit[3] (%)
94	1000	1000.3	0.0	±.0.7

สถาบันไฟฟ้าและอิเล็กทรอนิกส์
ELECTRICAL AND ELECTRONICS INSTITUTE

ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20230345EA

Calibration Report

3. Function : Total distortion + noise

Norminal Sound Pressure level (dB)	Norminal Frequency (Hz)	Measured value[4] (%)	Acceptance limit[5] (%)
94	1000	1.0	2.5

Uncertainty of measurement

Function	Uncertainty	Maximum-permitted uncertainty of measurement
Sound pressure level	0.10 dB	0.15 dB
Frequency	0.10 %	0.20 %
Total distortion + noise	0.40 %	0.50 %

Note: [1] The deviated value is the absolube valule of the difference between the measured value and the corresponding specified sound pressure level.
[2] The deviated value is the absolube valule of the difference in percent between the measured value and the corresponding specified frequency.
[3] The acceptance limit is for the deviated value.
[4] The measured value is the total distortion + noise, measured over the frequency range from 20 Hz to 20 kHz.
[5] The acceptance limit is for the Measured value.

Remarks: 1. Acceptance limit was IEC 60942:2017 Class 1.
2. Maximum-permitted uncertainty of measurement was IEC 60942:2017 Class 1.
3. The coverage factor k = 2.00

- - End of Report - -

Sheet No. : CR-515-2024-078

SOUND LEVEL METER CALIBRATION

Calibration Location: SECOT Calibration Date: Mar 7, 24

ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Frequency (Hz)	Ref.Calibrated (dB)	Eff.Calibrated (dB)
Cirrus	CR:515	97097	1000.00	94.0	93.7

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
20	Cirrus	CR162B	G301014	93.7	0.0
32	Cirrus	CR161B	G302356	93.7	0.0
45	Cirrus	CR161B	G303385	93.7	0.0
48	Cirrus	CR162B	G302237	93.7	0.0
49	Cirrus	CR162B	G302330	93.7	0.0

Calibrated by : _____ Approved by : Preeda S.

SECOT CO., LTD.
239 Rimklongprapa Rd. Bangsue, Bangkok, 10800, THAILAND
Tel: (662)959-3600 Fax: (662) 959-3535
E-Mail: envserv@secot.co.th

Sheet No. : CR-515-2024-147

SOUND LEVEL METER CALIBRATION

Calibration Location: SECOT **Calibration Date:** May 29, 24

ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Frequency (Hz)	Ref.Calibrated (dB)	Eff.Calibrated (dB)
Cirrus	CR:515	97097	1000.00	94.0	93.7

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
39	Cirrus	CR162B	G302743	93.7	0.0
44	Cirrus	CR162B	G302742	93.7	0.0

Calibrated by : _____ **Approved by :** _____

SECOT CO., LTD.
239 Rimklongprapa Rd. Bangsue, Bangkok, 10800, THAILAND
Tel: (662)959-3600 Fax: (662) 959-3535
E-Mail: envserv@secot.co.th

CERTIFICATE OF CALIBRATION

ISSUED BY **Noisemeters**

DATE OF ISSUE **26 March 2024** CERTIFICATE NUMBER **211259**

Approved signatory
N.Smith
Electronically signed:



NoiseMeters
Acoustic House
Bridlington Road
Hunmanby
YO14 0PH
United Kingdom
www.noisemeters.com

doseBadge Reader : IEC 60942:2003

Instrument information

Manufacturer: Cirrus Research plc

Model: RC:110A

Serial number: 95167

Class: 2

Notes:

Test summary

Date of calibration: 25 March 2024

The doseBadge reader detailed above has been calibrated to the published data as described in the operating manual and in the half-inch configuration. The procedures and techniques used are as described in IEC60942_2003 Annex B – Periodic Tests and three determinations of the sound pressure level, frequency and total distortion were made.

The sound pressure level was measured using a WS2F condenser microphone type MK:224 manufactured by Cirrus Research plc.

The results have been corrected to the reference pressure of 101.33 kPa using the manufacturer's data.

The doseBadge Reader has been shown to conform to the Class 2 requirements for periodic testing, described in Annex B of IEC 60942:2003 for the sound pressure level(s) and frequency(ies) stated, for the environmental conditions under which the tests were performed.

However, as public evidence was not available, from a testing organisation responsible for pattern approval, to demonstrate that the model of doseBadge Reader conformed to the requirements for pattern evaluation described in Annex A of IEC 60942:2003, no general statement or conclusion can be made about conformance of the doseBadge Reader to the requirements of IEC 60942:2003.

Notes:

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number: **211259**

Environmental conditions

The following conditions were recorded at the time of the test:

Before Pressure: 99.26 kPa Temperature: 22.1 °C Humidity: 33.4 %

After Pressure: 99.26 kPa Temperature: 22.1 °C Humidity: 34.6 %

Test equipment

Equipment	Manufacturer	Model	Serial number
Distortion Meter	Keithley	2015	0839263
Acoustic Calibrator	Bruel and Kjaer	4231	2610257
Environmental Monitor	Comet	T7510	21962628

Initial Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	113.41	113.54	113.55	**113.50**	-0.50	±0.75	0.11 dB
Distortion (%)	< 4.00	0.49	0.50	0.55	**0.51**	0.51	+4.00	0.13 %
Frequency (Hz)	1000.0	990.5	990.5	990.4	**990.5**	-9.5	±20.0	0.1 Hz

The measured quantities or deviations (as applicable), extended by the expanded combined uncertainty of measurement, must not exceed the corresponding tolerance.

Adjusted Acoustic Results

	Expected	Sample 1	Sample 2	Sample 3	Average	Deviation	Tolerance	Uncertainty
Level (dB)	114.00	113.99	113.99	113.98	**113.99**	-0.01	±0.75	0.11 dB
Distortion (%)	< 4.00	0.42	0.41	0.41	**0.42**	0.42	+4.00	0.13 %
Frequency (Hz)	1000.0	990.3	990.4	990.3	**990.4**	-9.6	±20.0	0.1 Hz

Functionality Results

Function	Result
Keypad	Pass
Battery Power	Pass
Display	Pass
Communication	Pass
2 way IR link	Pass
Clock	Pass

End of results

Sheet No. : NC-CIRRUS-2024-070

NOISE DOSE METER CALIBRATION

Calibration Location: SECOT **Calibration Date:** May 7, 24

ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
CIRRUS	RC 110A	95167	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Cirrus	CR110A	CB1023	114.0	0.0
2	Cirrus	CR110A	CB1025	113.8	0.2
3	Cirrus	CR110A	CB1042	114.1	-0.1
4	Cirrus	CR110A	CB1053	114.2	-0.2
5	Cirrus	CR110A	CB1055	113.1	0.9
6	Cirrus	CR110A	CB1056	113.8	0.2
7	Cirrus	CR110A	CB1101	113.6	0.4
8	Cirrus	CR110A	CB1102	114.1	-0.1

Calibrated by : **Approved by :**

SECOT CO., LTD.
239 Rimklongprapa Rd. Bangsue, Bangkok, 10800, THAILAND
Tel: (662)959-3600 Fax: (662) 959-3535
E-Mail: envserv@secot.co.th

Sheet No. : NC-CIRRUS-2024-106

NOISE DOSE METER CALIBRATION

Calibration Location: SECOT Calibration Date: Jun 11, 24

ACOUSTIC CALIBRATOR

Brand	Model	Serial No.	Calibrated (dB)	Frequency (Hz)
CIRRUS	RC 110A	95167	114.00	1000

No.	Brand	Model	Serial No.	Reading (dB)	dB Adjust
1	Cirrus	CR110A	CB1104	114.0	0.0

Calibrated by : _____ Approved by : _____

SECOT CO., LTD.
239 Rimklongprapa Rd. Bangsue, Bangkok, 10800, THAILAND
Tel: (662)959-3600 Fax: (662) 959-3535
E-Mail: envserv@secot.co.th

Calibration Certificate

BEIJING J.T TECHNOLOGY CO., LTD.
www.bjittec.com
www.jianttech.com

JANTYTECH 建通科技

Instrument information

Name	WET BULB GLOBE TEMPERATURE (WBGT)METER
Series No	3522210172
Type	JT2011-E2A
Customer	SECOT CO., LTD.
Address	239 Rim Klong Prapa Road, Bang Sue, Bang Sue, Bangkok 10800

Integrity check of instrument

Appearance	√
Parts integrity	√
Screen display or touch	√
Instrument button	√
Power supply	√
battery	√
Data storage and export	√
Deviation degree of comparison test with	√
standard instrument	√

Calibration Results

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (±°C)
WET	25.0	25.1	-0.1	0.2
	30.0	30.1	0.1	0.2
	35.0	35.2	-0.2	0.2
	40.0	39.9	0.1	0.2
	45.0	45.1	-0.1	0.2
DRY	25.0	24.9	0.1	0.2
	30.0	29.9	0.1	0.2
	35.0	35.1	-0.1	0.2
	40.0	39.8	0.2	0.2
	45.0	44.9	0.1	0.2
GLOBE	25.0	24.9	0.1	0.2
	30.0	29.8	0.2	0.2
	35.0	35.1	-0.1	0.2
	40.0	39.9	0.1	0.2
	45.0	44.9	0.1	0.2

Environmental conditions: temperature: 26 °C±2°C, relative humidity: 30% RH± 10RH%

Reference Standard : Standard Mercury Thermometers, Manufacturer: BGRI, Model: STA, SN : 2-56, Calibrated Date : 20 February 2023, Calibration Certificate No. : RA21H-AB1000009

This Certificate is traceable to NCMT North China, Certificate No.: RA20J-AK000073

Calibration Engineer : _____

Date : January 16, 2024

北京世纪建通科技股份有限公司 质检专用章

GC-MS (Amb)

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Agilent

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about ***Agilent Technologies services***, please visit our website using the following URL: http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome.
- To access **Agilent University,** visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: https://www.agilent.com/en-us/agilentresources.
- Need technical support, FAQs, supplies? – visit our **Support Home page** http://www.agilent.com/search/support.
- **Videos** about specific preparation requirements for your instrument can be found by searching the *Agilent YouTube* channel at https://www.youtube.com/user/agilent.
- **7890B Manuals** are also available on Agilent.com:
  - **Safety** https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf
  - **Installation and First Startup** https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf
  - **Operation Manual** https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf
  - **Maintaining Your GC** https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf

Revision: 2.01, Issued: September 15, 2021
Agile Document Number: D0013618
DE number: 44166.7597222222
© Agilent Technologies, Inc. 2021

Agilent

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Section not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- ***Ask the customer to sign the Service Completion section including the customer's and your signature.***

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

© Agilent Technologies, Inc. 2021

System Information

☐ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	7890A GC System / GCMS
Instrument System Site and Location	SECOT Co., Ltd.

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3440A	CN10750035
2. N/A	N/A
3. N/A	N/A
4. N/A	N/A
5. N/A	N/A
6. N/A	N/A
7. N/A	N/A
8. N/A	N/A
9. N/A	N/A
10. N/A	N/A

Preparation

☑ Discuss any specific issues with the customer before starting.
☑ Review the instrument logbook for recorded problems and comments.
☑ Save instrument control settings before starting the procedure.
☑ Perform a general inspection of the system for cleanliness.
☑ Check for proper installation of parts, assemblies, sensors etc.
☑ Check system for required installation of components, settings as defined by current Service Notes.
☑ Check for required firmware updates and verify with customers if they would like them installed.
☐ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

© Agilent Technologies, Inc. 2021

Preventive Maintenance Procedure

Clean and inspect GC

- ☑ Unplug power cord from the power source.
- ☑ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☑ Inspect internal connectors for proper contact and placement.
- ☑ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☑ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☑ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☑ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☑ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – "Maintaining Your GC" - for the inlet(s) installed.
- ☑ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☑ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☐ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

Zero Sensors and Leak test

- ☑ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ☑ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual".
  If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☑ Record if test passed or failed in the results table.

© Agilent Technologies, Inc. 2021

ALS Maintenance

- ☑ **Section NOT applicable**
- ☐ Check all cabling and configuration settings between GC, tray, and injectors.
- ☐ Vacuum or remove any dust, especially around fans.
- ☐ Check operation of all fans.
- ☐ Check syringe for smooth plunger operation.
- ☐ Check for smooth operation of the needle support – clean if necessary

Restore Instrument

- ☑ Restore the normal operating conditions or customer method using the Data System.
- ☑ Purge the system with carrier flow for 15 minutes
- ☑ Bake out the system, then restore the normal operating conditions
- ☑ After equilibration, check and record the post PM detector signal output values.
  Results should be similar or lower than the detector outputs recorded prior to PM.
- ☐ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

© Agilent Technologies, Inc. 2021

Signature Page

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review with the customer this service, parts replaced, and test results obtained.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output	N/A	N/A
Back detector output	N/A	N/A
AUX detector output	N/A	N/A
Pressure decay test	**Expected test result**	**Actual test result**
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	Pass

© Agilent Technologies, Inc. 2021

7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	1
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	N/A
PP Inlet PM kit	5188-6498	7890A/B	N/A
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	N/A
MMI Cleaning Kit	G3510-60820	7890A/B	N/A
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	N/A
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	N/A
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	N/A
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	N/A
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	N/A
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	N/A
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	N/A
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	N/A
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	N/A
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	N/A
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	N/A
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	N/A

© Agilent Technologies, Inc. 2021

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

N/A

Service Completion

Service request number 6026807758 Date service completed 12 Jun 2024

Agilent signature Customer signature Srinivas C.

Total number of pages in this document 10

Do not include this section/page in the published, customer-facing PDF version.

This page is only relevant for Agilent source documents for document control purposes and is NOT intended for customer viewing. Refer to the SPIFPM checklist Authoring Guide for more information.

Document Control Logs

Revision Log

Revision	Date	Author	Reason for update
Revision of document	Date of issuance	Author of document	Author to describe main features/changes made for this specific revision
1.0 Draft	4-Mar-2011	Dave Park	Migrated the content of revision A.01.05 to the new Agilent template. Reviewed by subject matter expert, Dave Park.
1.1 Draft	20-Jan-2015	Dave Park	Added Split Vent trap to MMI, PTV and VE - also PTV and FID PM Parts
1.2 Draft	31-March-2015	Dave Park	Added Ultra Inert Gold Seal and Liner to SS Consumables
A.01.11	10-Dec-2015	Dave Park	Added step to perform maintenance on the Split Vent Tube and .018" FID Jet part numbers - Fixed broken web links
2.00	30-Dec-2020	Gary Boardman	Updated New Template and terminology change: Familiarization to Introduction. Create New Agile Document Number: D0007063

Approval Log

Revision	Approver	Title of approver
Add revision number	Add approver name here	Add approver's function or title here
A.01.06	Don Gage	Product support manager
A.01.09	Kai Meng	Product support manager
A.01.10	Suneetha Tippireddy	Product support manager
A.01.11	Suneetha Tippireddy	Product support manager
2.00	Josh Roark	GC Product Support Manager

Designated Evaluation Log

Revision	Designated Evaluator (DE)	Title of DE	DE Number
Add revision number	Add name	Add function or title	Add DE number here
2.00	Michael Zumwalt	CrossLab Start Up Services Application Consulting Lead	44166.7597222222

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent GCMS Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Introduction

Select the appropriate PM to be done and then perform the checklist under that section

- ☐ Interim Preventive Maintenance — 6 months
- ☑ Major Preventive Maintenance — Yearly

This checklist covers the following model(s):

Type	Model
SQ	5973 Series MSD
SQ	5975 Series MSD
SQ	5977 Series MSD
TQ	7000 Series MS/MS
TQ	7010 Series MS/MS
QTOF	7200 Series QTOF
QTOF	7250 Series QTOF

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Revision A.20 Issued November 2021
DE Number 44145.7539351852
© Agilent Technologies, Inc. 2021

Agilent

Important Customer Web Links

- For more information about *Agilent Technologies services*, please visit our website using the following URL: *http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair*
- To access *Agilent University*, visit *http://www.agilent.com/crosslab/university/* to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful *Agilent Resource Center* web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: *https://www.agilent.com/en-us/agilentresources*
- Need technical support, FAQs, supplies? – visit our *Support Home page* at *http://www.agilent.com/search/support*
- Get answers. Share insights. Build connections:
  Join the *Agilent Community* at *https://community.agilent.com/welcome*

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Section not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- **Ask the customer to sign the Service Completion section including the customer's and your signature.**

Additional Instruction Notes

- Preventive maintenance is a factory recommended procedure designed to reduce the likelihood of electromechanical failures. Failure to perform preventive maintenance may reduce the long-term reliability of certain instruments and systems. **Two preventative maintenances (PMs) per year are recommended, the Major PM Service will be performed annually with an Interim PM performed 6 months after the Major PM.**

© Agilent Technologies, Inc. 2021

System Information

☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	5975C MSD
Instrument System Site and Location	SECOT Co., Ltd.

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3172A	US74838080
2. N/A	N/A
3. N/A	N/A
4. N/A	N/A
5. N/A	N/A
6. N/A	N/A
7. N/A	N/A
8. N/A	N/A

Preparation

☑ Discuss any specific issues with the customer before starting.
☑ Review the instrument logbook for recorded problems and comments.
☑ Save instrument control settings before starting the procedure.
☑ Perform a general inspection of the system for cleanliness.
☑ Check for proper installation of parts, assemblies, sensors etc.
☑ Check system for required installation of components and settings as defined by current Service Notes
☑ Check for firmware updates and verify with customers if they would like them installed. Firmware update(s) are strongly recommended.

Customer Responsibilities

Customers should ensure that all necessary operating supplies, consumables, and usage-dependent items such as gases, vials, syringes, calibrant solution and solvents required for successful preventive maintenance are available. A customer representative should be available while the preventive maintenance is being performed.

© Agilent Technologies, Inc. 2021

Important notice for customers

The customer should complete the following before the Support Provider arrives on site:

☑ Perform an autotune and retain the printed tune report just prior to the start of the PM to verify performance of the equipment.

Note: it is recommended to have the customer run the autotune and tune evaluation prior to the PM and then start the vent cycle so that the instrument will be ready for the service representative.

Definition of the Task/Recommended items within the document

Task		Recommended			
Yes	No	Interim	Major	As needed	
☑	☐	☐	☐	☐	**Yes** selected means that the task was done or the part was required.
☐	☑	☐	☐	☐	**No** selected means that the task was not done or the part was not required.
☐	☐	☑	☐	☐	**Interim** selected means that this task is recommended to be done at 6-month intervals.
☐	☐	☐	☑	☐	**Major** selected means that this task is recommended to be done yearly; if the customer would like a service to be done at the 6-month interval then the service could be purchased.
☐	☐	☐	☐	☑	**As needed** selected means that the task was done or the part was used as needed. For example, there could be two types of filters that could be used and this was the one selected.

Preventive Maintenance Procedures

Yes/No		Interim/Major		Description
☑	☐	☑	☑	Perform general inspection of system for cleanliness
☑	☐	☑	☑	Discuss any problems the customer is having with the instrument
☑	☐	☑	☑	Review customer maintenance records and exclude maintenance on recently serviced items
☑	☐	☑	☑	Review the most recent autotune report. This will give a starting point for evaluating spectral peaks, baseline noise, peak shape, mass assignments and resolution.

				GCMS	
Yes/No		Interim/Major		Description	
☑	☐	☑	☑	Record Instrument model no.	
☑	☐	☑	☑	Record Instrument serial no.	
☑	☐	☑	☑	Record Rough Vacuum	
☑	☐	☑	☑	Record Manifold Vacuum	
☑	☐	☑	☑	Type of Column installed	

© Agilent Technologies, Inc. 2021

Agilent

				System Checks	
Yes/No		Interim/Major		Description	
☑	☐	☑	☑	Verify that calibration peaks were seen prior to starting the PM	
☑	☐	☑	☑	Vent the instrument	
☑	☐	☑	☑	Inspect vacuum hoses, pump, exhaust tubing, and power cords for excessive wear.	
☑	☐	☑	☑	Visually inspect calibrant levels – PFTBA PFDTD (if appl.), IRM (if appl.). Refill if available.	
☑	☐	☑	☑	Look for any obvious external damage or problems.	
☑	☐	☑	☑	Clean air intake(s). Cosmetic cover(s) may need to be removed.	
☑	☐	☑	☑	Verify system line voltage meets instrument specifications: Yes ☑ No ☐	

Yes/No ☑ ☐				Wet Mechanical vacuum pumps	
Yes/No		Interim/Major		Description	
☑	☐	☑	☑	Check for evidence of oil leakage. Check pump gasket for leakage.	
☑	☐	☑	☑	Drain and replace mechanical pump oil.	
☐	☑	☑	☑	Replace Oil Mist Filter if applicable.	
☑	☐	☑	☑		Discuss with customer the need for more frequent oil changes if the oil is dirty
☐	☑	☑	☑		Don't use mist filters with Chemical Ionization.
☑	☐	☑	☑	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed. Visually confirm that no oil returns up vacuum hose.	
Yes/No	☐	☑		Dry Mechanical vacuum pumps - Diaphragm	
Yes/No		Interim/Major		Description	
☐	☐	☑	☑	Check for evidence of poor vacuum – Turbo power demand, poor manifold vacuum, etc.	
☐	☐	☑	☑	Clear air flow paths of dust.	
☐	☐	☑	☑	If vacuum is poor, then replace the diaphragm pump.	
☐	☐	☑	☑	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.	

Yes/No ☐ ☑				Dry Mechanical vacuum pumps - Scroll	
Yes/No		Interim/Major		Description	
☐	☐	☑	☑	Replace the tips seal on the IDP pump.	
☐	☐	☑	☑	Check for evidence of poor vacuum – Turbo power demand, poor manifold vacuum, etc.	
☐	☐	☑	☑	Replace the Exhaust Filter if required.	
☐	☐	☑	☑		Discuss with customer the need for more frequent changes, if needed.
☐	☐	☑	☑		Inform customer that pump gas ballast should be installed all the time.
☐	☐	☑	☑	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.	

				Cleaning System and Filters	
Yes/No		Interim/Major		Description	
				Fans	
☑	☐	☑	☑		Remove dust from fans and vent covers.
☑	☐	☑	☑		Verify fans are functional and that there is enough space around the instrument for proper cooling.
				Source cleaning	
☑	☐	☑	☑		Open analyzer and remove the source.
☑	☐	☑	☑		Disassemble, Clean, Re-assemble source.
☑	☐	☑	☑		Re-install source and close analyzer.
				Filters	
☑	☐	☑	☑		Replace RMSH-2 Helium gas filter – if applicable.
☐	☑	☑	☑		Replace RMSN-2 Nitrogen gas filter – if applicable.
☐	☑	☑	☑		Replace RMSHY-2 Hydrogen gas filter – if applicable.
☐	☑	☑	☑		CP17988 – Gas Clean Carrier Gas Kit for 7890 for Nitrogen or Helium; Bracket, Mount, and Filter – if applicable.
☐	☑	☑	☑		CP17974 – Gas Clean Filter Kit GC/MS 1/8", Mount and Filter – if applicable.
☐	☑	☑	☑		CP17973 – Gas Clean Filter; Replacement Filter – if applicable.
☐	☑	☑	☑		5190-9071 – Methane Gas Filter – if applicable

Guidance: If gas filter is replaced, write the change date on the filter using a permanent marker.

© Agilent Technologies, Inc. 2021

Agilent

				System post-check	
Yes/No		Interim/Major		Description	
☑	☐	☑	☑	Pump system back down. Wait until system stability has been achieved.	
☑	☐	☑	☑	Verify system vacuum reading(s) via the gauge controller.	
☑	☐	☑	☑	Leak Check	
☑	☐	☑	☑		Verify system in manual tune
☑	☐	☑	☑		Compare against previous tune file report(s)
☑	☐	☑	☑	Change to Tune and verify that all temperatures, pressures, and gas flows reach method set points	
☑	☐	☑	☑	Check manually that you have calibration peaks.	
☑	☐	☑	☑	EI Autotune Performed	

Guidance: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument setup and checkout.

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook. Record the PM event in the Smart Alerts logbook, if applicable.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review this service, parts replaced, and test results obtained with the customer.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comment box. Systems in a compliant environment may need additional documentation.

Agilent Test Results Table

Test Description	Expected Test Result	Actual Test Result
Atune and Evaluation	Pass	Pass
N/A	N/A	N/A

© Agilent Technologies, Inc. 2021

Agilent Consumed Parts List Table

☐ Section not applicable

Part Description	Part Number	Product or Model# where used	Quantity consumed
Agilent Vacuum Fluid	5191-5851	Rough Pump	1
N/A	N/A	N/A	N/A

© Agilent Technologies, Inc. 2021

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box

N/A

Service Completion

Service request number 6006807758 Date service completed 12 Jun 2024

Agilent signature Sinan Th. Customer signature Sirinan C.

Total number of pages in this document 12

© Agilent Technologies, Inc. 2021

Parts – As needed as part of the PM

Common MS Filters and Seals – 5973/5975/5977/7000/7010/7200/7250 Series

					Supplies	
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☑	☑	Helium gas filter – if required	RMSH-2
☐	☐	☐	☑	☑	Nitrogen gas filter – if required	RMSN-2
☐	☐	☐	☑	☑	Big Universal Trap, 1/8" fittings, Hydrogen, if required	RMSHY-2
☐	☐	☐	☑	☑	Gas Clean Carrier Gas Kit for 7890 for Nitrogen or Helium; Bracket, Mount and Filter – if required	CP17988
☐	☐	☐	☑	☑	Gas Clean Filter Kit GC/MS 1/8 in (complete replacement kit) – if required	CP17974
☐	☐	☐	☑	☑	Gas Clean GS/MS Filter – if required	CP17973
☐	☐	☐	☑	☑	Chemical Ionization Gas Purifier (CI systems) – if required	5190-9071
☑	☐	☑	☑	☐	Agilent AVF Platinum, 1 quart	5191-5851

Gas filters need to be changed only if required

MS Maintenance Supplies for 5973/5975/5977 Series

Yes/No ☑ ☐					Supplies	
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☑	☑	Diffusion pump fluid (Diffusion Pump Models)	6040-0809 Qty 2
☐	☐	☐	☑	☑	IDP-3 Tip Seal Replacement Kit (IDP-3 Dry Pump Models)	G7077-67018
☐	☐	☐	☑	☑	IDP-3 Tip Seal Replacement Kit (no tools – CSD P/N)	5190-9561
☐	☐	☐	☑	☑	IDP-3 Tip Seal Replacement Kit (no tools – VPD P/N)	IDP3TS
☐	☐	☐	☑	☑	Filter element for IDP-3	REPLSLRFILTER2
☐	☐	☐	☑	☑	DS42 Oil Mist Eliminator 3/4G & 3/8	SR03706556
☐	☐	☐	☑	☑	Exhaust oil mist trap (thread) Edwards/Pfeiffer	G1099-80039

MS Maintenance Supplies for 7000/7010 Series

Yes/No ☐ ☑					Supplies	
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☑	☑	Nitrogen gas filter	RMSN-2
☐	☐	☐	☑	☑	IDP-10 Tip Seal Replacement Kit (IDP-10 Dry Scroll Pump Models)	G7004-67023
☐	☐	☐	☑	☑	IDP-10 Tip Seal Replacement Kit (no tools – VPD P/N)	X3807-67000
☐	☐	☐	☑	☑	Oil Mist Filter RV5	G6600-80043
☐	☐	☐	☑	☑	Filter element for the IDP-10	REPLSLRFILTER1

MS Maintenance Supplies for 7200/7250 Series

Yes/No ☐ ☑					Supplies	
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☑	☑	Nitrogen gas filter – if required	RMSN-2
☐	☐	☐	☑	☑	RIS Probe Maintenance Kit (7200 Series only)	G7005-60170
☐	☐	☐	☑	☑	DS202 Oil Mist Eliminator	SR03706800
☐	☐	☐	☑	☑	IDP-15 Tip Seal Replacement Kit (IDP-15 Dry Pump Models)	5190-9613
☐	☐	☐	☑	☑	IDP-15 Tip Seal Replacement Kit (no tools – VPD P/N)	X3815-67000
☐	☐	☐	☑	☑	Filter element, for SH-110/SH-112/IDP-15 exhaust silencer	REPLSLRFILTER
☐	☐	☐	☑	☑	DS 3/8 MAG. PLUG AND GASKET	SR03701824

MS Maintenance Supplies for JetClean

Yes/No ☐ ☑					Supplies	
Yes/No		Interim/Major/As needed			Description	Part number

© Agilent Technologies, Inc. 2021

☐	☐	☐	☑	☑	Big Universal Trap, 1/8" fittings, Hydrogen, if required	RMSHY-2

Consumable Parts Reference – Purchasable by customer, not included as part of PM

Common MSD Maintenance Supplies 5973/5975/5977/7000/7010/7200/7250 Series

					Common Recommended Consumables Parts	
Yes/No		Interim/Major/As needed			Description	Part number
☑	☐	☐	☐	☑	EI High Temperature Filaments	G7005-60061 Qty 2
☐	☐	☐	☐	☑	HES EI Filaments	G7002-60001
☐	☐	☐	☐	☑	LE-EI Filaments	G3850-60021
☐	☐	☐	☐	☑	CI High Temperature Filament – all MSDs	G7005-60072
☐	☐	☐	☐	☑	PFTBA GCMS Tuning Standard calibrant	05971-60571
☐	☐	☐	☐	☑	PFDTD calibrant, 1 mL	8500-8510
☐	☐	☐	☐	☑	PFET, IRM calibrant for GC QTOF 0.5 mL	5190-0531

MSD Maintenance Supplies 5973/5975/5977 Series

Yes/No	☐	☑			Supplies	
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☐	☑	CI Interface tip seal (tip and spring combo)	G1999-60412
☐	☐	☐	☐	☑	CI Interface tip seal (tip only)	G3870-20542
☐	☐	☐	☐	☑	CI Interface tip seal spring (spring only)	G1999-20023
☐	☐	☐	☐	☑	Repeller insulator	G1099-20133 Qty 2
☐	☐	☐	☐	☑	Lens insulator/holder (HES)	G7002-20074
☐	☐	☐	☐	☑	Ring heater/sensor assembly (HES)	G7002-60043
☐	☐	☐	☐	☑	Ceramic insulator for Extractor (HES)	G7002-20064
☐	☐	☐	☐	☑	Transfer-Line Tip Cap, Threaded	G3870-20547
☐	☐	☐	☐	☑	Transfer-Line Tip Base, Threaded	G3870-20548

MS Maintenance Supplies for 7000/7010 Series

Yes/No	☐	☑			Supplies	
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☐	☑	CI Interface tip seal - 7000	G1999-60412
☐	☐	☐	☐	☑	CI Interface tip seal - 7010	G7002-60412
☐	☐	☐	☐	☑	CI Interface tip seal (tip only)	G3870-20542
☐	☐	☐	☐	☑	CI Interface tip seal spring (spring only)	G1999-20023
☐	☐	☐	☐	☑	Repeller insulator - 7000	G1099-20133 Qty 2
☐	☐	☐	☐	☑	Lens insulator/holder (HES)	G7002-20074
☐	☐	☐	☐	☑	Ring heater/sensor assembly (HES)	G7002-60043
☐	☐	☐	☐	☑	Ceramic insulator for Extractor (HES)	G7002-20064
☐	☐	☐	☐	☑	Transfer-Line Tip Cap, Threaded	G3870-20547
☐	☐	☐	☐	☑	Transfer-Line Tip Base, Threaded	G3870-20548

MS Maintenance Supplies for 7200 Series

Yes/No	☐	☑			Supplies	
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☐	☑	Extractor Lens Insulator	G7005-20133
☐	☐	☐	☐	☑	Ion Focus Insulator	G7005-20442
☐	☐	☐	☐	☑	Ring Heater/Sensor Assembly	G7005-60110
☐	☐	☐	☐	☑	RIS Xfer Tip	G7005-20542
☐	☐	☐	☐	☑	RIS Xfer Tip Spring	G7005-20024

© Agilent Technologies, Inc. 2021

MS Maintenance Supplies for 7250 Series

Yes/No	☐	☑			Supplies	
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☐	☑	Lens insulator/holder (HES)	G7002-20074
☐	☐	☐	☐	☑	Ring heater/sensor assembly (HES)	G7002-60043
☐	☐	☐	☐	☑	Ceramic insulator for Extractor (HES)	G7002-20064
☐	☐	☐	☐	☑	Transfer-Line Tip Cap, Threaded	G3870-20547
☐	☐	☐	☐	☑	Transfer-Line Tip Base, Threaded	G3870-20548
☐	☐	☐	☐	☑	EI Extractor Transfer Tip	G3870-20542
☐	☐	☐	☐	☑	CI Tip Compression Spring	G1999-20023

MS Maintenance Supplies for Intuvo 9000 MS Systems

Yes/No	☐	☑			Supplies	
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☐	☑	Swaged MS Tail - Packaged	G4590-60009
☐	☐	☐	☐	☑	Swaged MS Tail (HES) - Packaged	G4590-60109

Common MS Maintenance Supplies

Parts required						
Yes/No		Interim/Major/As needed			Description	Part number
☐	☐	☐	☐	☑	Abrasive paper, 30 um	5061-5896
☐	☐	☐	☐	☑	Alumina powder	393706201
☐	☐	☐	☐	☑	Cloths, clean (pkg of 15)	05980-60051
☐	☐	☐	☐	☑	Cloths, cleaning (pkg of 300)	9310-4828
☐	☐	☐	☐	☑	Cotton swabs (pkg of 100)	5080-5400
☐	☐	☐	☐	☑	Gloves, clean, large	8650-0030
☐	☐	☐	☐	☑	Gloves, clean, small	8650-0029

© Agilent Technologies, Inc. 2021

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Agilent

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about ***Agilent Technologies services***, please visit our website using the following URL: http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome.
- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: https://www.agilent.com/en-us/agilentresources.
- Need technical support, FAQs, supplies? – visit our **Support Home page** http://www.agilent.com/search/support.
- **Videos** about specific preparation requirements for your instrument can be found by searching the ***Agilent YouTube*** channel at https://www.youtube.com/user/agilent.
- **7890B Manuals** are also available on Agilent.com:
  - **Safety**
    https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf
  - **Installation and First Startup**
    https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf
  - **Operation Manual**
    https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf
  - **Maintaining Your GC**
    https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf

Revision: 2.01, Issued: September 15, 2021
Agile Document Number: D0013618
DE number: 44166.7597222222
© Agilent Technologies, Inc. 2021

Agilent

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Section not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- ***Ask the customer to sign the Service Completion section including the customer's and your signature.***

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

© Agilent Technologies, Inc. 2021

System Information

☐ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	7890A GC System
Instrument System Site and Location	SECOT CO., LTD.

List System Component Product Numbers	**List the Serial Numbers of each Component**
1. G3440A	US10943001
2. G4513A	CN10110080
3. G4514A	CN93901235
4. N/A	N/A
5. N/A	N/A
6. N/A	N/A
7. N/A	N/A
8. N/A	N/A
9. N/A	N/A
10. N/A	N/A

Preparation

☑ Discuss any specific issues with the customer before starting.
☑ Review the instrument logbook for recorded problems and comments.
☑ Save instrument control settings before starting the procedure.
☑ Perform a general inspection of the system for cleanliness.
☑ Check for proper installation of parts, assemblies, sensors etc.
☑ Check system for required installation of components, settings as defined by current Service Notes.
☑ Check for required firmware updates and verify with customers if they would like them installed.
☐ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

© Agilent Technologies, Inc. 2021

Preventive Maintenance Procedure

Clean and inspect GC

- ☑ Unplug power cord from the power source.
- ☑ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☑ Inspect internal connectors for proper contact and placement.
- ☑ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☑ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☑ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☑ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☑ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – "Maintaining Your GC" - for the inlet(s) installed.
- ☑ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☑ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☑ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

Zero Sensors and Leak test

- ☑ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ☑ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual".
  If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☑ Record if test passed or failed in the results table.

© Agilent Technologies, Inc. 2021

ALS Maintenance

- ☐ **Section NOT applicable**
- ☑ Check all cabling and configuration settings between GC, tray, and injectors.
- ☑ Vacuum or remove any dust, especially around fans.
- ☑ Check operation of all fans.
- ☑ Check syringe for smooth plunger operation.
- ☑ Check for smooth operation of the needle support – clean if necessary

Restore Instrument

- ☑ Restore the normal operating conditions or customer method using the Data System.
- ☑ Purge the system with carrier flow for 15 minutes
- ☑ Bake out the system, then restore the normal operating conditions
- ☑ After equilibration, check and record the post PM detector signal output values.
  Results should be similar or lower than the detector outputs recorded prior to PM.
- ☑ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

© Agilent Technologies, Inc. 2021

Signature Page

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review with the customer this service, parts replaced, and test results obtained.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

7890 GC Test Results Table

Detector Signal Outputs		Before PM Service	After PM Service
Front detector output	FID	-	15
Back detector output	FPD	-	60
AUX detector output		N/A	N/A
Pressure decay test		**Expected test result**	**Actual test result**
Front inlet pressure decay test		Pass	Pass
Back inlet pressure decay test		Pass	Pass

© Agilent Technologies, Inc. 2021

7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	1
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	N/A
PP Inlet PM kit	5188-6498	7890A/B	N/A
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	N/A
MMI Cleaning Kit	G3510-60820	7890A/B	N/A
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	N/A
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	N/A
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	1
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	N/A
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	N/A
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	N/A
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	N/A
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	N/A
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	N/A
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	N/A
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	N/A
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	N/A

© Agilent Technologies, Inc. 2021

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

N/A

Service Completion

Service request number 6006785689 Date service completed 23 May 2024

Agilent signature [signature] Customer signature [signature]

Total number of pages in this document 10

© Agilent Technologies, Inc. 2021

Do not include this section/page in the published, customer-facing PDF version.

This page is only relevant for Agilent source documents for document control purposes and is NOT intended for customer viewing. Refer to the SPIFPM checklist Authoring Guide for more information.

Document Control Logs

Revision Log

Revision	Date	Author	Reason for update
Revision of document	Date of issuance	Author of document	Author to describe main features/changes made for this specific revision
1.0 Draft	4-Mar-2011	Dave Park	Migrated the content of revision A.01.05 to the new Agilent template. Reviewed by subject matter expert, Dave Park.
1.1 Draft	20-Jan-2015	Dave Park	Added Split Vent trap to MMI, PTV and VE - also PTV and FID PM Parts
1.2 Draft	31-March-2015	Dave Park	Added Ultra Inert Gold Seal and Liner to SS Consumables
A.01.11	10-Dec-2015	Dave Park	Added step to perform maintenance on the Split Vent Tube and .018" FID Jet part numbers - Fixed broken web links
2.00	30-Dec-2020	Gary Boardman	Updated New Template and terminology change: Familiarization to Introduction. Create New Agile Document Number: D0007063

Approval Log

Revision	Approver	Title of approver
Add revision number	Add approver name here	Add approver's function or title here
A.01.06	Don Gage	Product support manager
A.01.09	Kai Meng	Product support manager
A.01.10	Suneetha Tippireddy	Product support manager
A.01.11	Suneetha Tippireddy	Product support manager
2.00	Josh Roark	GC Product Support Manager

Designated Evaluation Log

Revision	Designated Evaluator (DE)	Title of DE	DE Number
Add revision number	Add name	Add function or title	Add DE number here
2.00	Michael Zumwalt	CrossLab Start Up Services Application Consulting Lead	44166.7597222222

© Agilent Technologies, Inc. 2021

GC-MS (ATOM)

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Agilent

1 of 9

Agilent CrossLab
From Insight to Outcome

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about ***Agilent Technologies services***, please visit our website using the following URL: http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome.
- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: https://www.agilent.com/en-us/agilentresources.
- Need technical support, FAQs, supplies? – visit our **Support Home page** http://www.agilent.com/search/support.
- **Videos** about specific preparation requirements for your instrument can be found by searching the ***Agilent YouTube*** channel at https://www.youtube.com/user/agilent.
- **7890B Manuals** are also available on Agilent.com:
  - **Safety**
    https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf
  - **Installation and First Startup**
    https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf
  - **Operation Manual**
    https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf
  - **Maintaining Your GC**
    https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf

Revision: 2.00, Issued: December 30, 2020
Agile Document Number: D0007063
DE number: 44166.7597222222
© Agilent Technologies, Inc. 2020

Agilent

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Section not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- ***Ask the customer to sign the Service Completion section including the customer's and your signature.***

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

© Agilent Technologies, Inc. 2020

System Information

☐ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	CN13201053
Instrument System Site and Location	SECOT, Bangkok

List System Component Product Numbers		**List the Serial Numbers of each Component**
1.	G3440A	CN13201053
2.	G4513A	CN13360196
3.	G4514A	CN13230031
4.		
5.		
6.		
7.		
8.		
9.		
10.		

Preparation

☑ Discuss any specific issues with the customer before starting.
☑ Review the instrument logbook for recorded problems and comments.
☑ Save instrument control settings before starting the procedure.
☑ Perform a general inspection of the system for cleanliness.
☑ Check for proper installation of parts, assemblies, sensors etc.
☑ Check system for required installation of components, settings as defined by current Service Notes.
☑ Check for required firmware updates and verify with customers if they would like them installed.
☑ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

© Agilent Technologies, Inc. 2020

Preventive Maintenance Procedure

Clean and inspect GC

- ☑ Unplug power cord from the power source.
- ☑ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☑ Inspect internal connectors for proper contact and placement.
- ☑ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☑ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☑ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☑ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☑ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – "Maintaining Your GC" - for the inlet(s) installed.
- ☑ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☑ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☐ N/A If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

Zero Sensors and Leak test

- ☑ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ☑ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual". If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☑ Record if test passed or failed in the results table.

© Agilent Technologies, Inc. 2020

ALS Maintenance

- ☐ **Section NOT applicable**
- ☑ Check all cabling and configuration settings between GC, tray, and injectors.
- ☑ Vacuum or remove any dust, especially around fans.
- ☑ Check operation of all fans.
- ☑ Check syringe for smooth plunger operation.
- ☑ Check for smooth operation of the needle support – clean if necessary

Restore Instrument

- ☑ Restore the normal operating conditions or customer method using the Browser interface or Data System.
- ☑ Purge the system with carrier flow for 15 minutes
- ☑ Bake out the system, then restore the normal operating conditions
- ☑ After equilibration, check and record the post PM detector signal output values. Results should be similar or lower than the detector outputs recorded prior to PM.
- ☐ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

© Agilent Technologies, Inc. 2020

Signature Page

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review with the customer this service, parts replaced, and test results obtained.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

7890 GC Test Results Table

Detector Signal Outputs	Before PM Service	After PM Service
Front detector output	N/A	N/A
Back detector output		
AUX detector output		
Pressure decay test	**Expected test result**	**Actual test result**
Front inlet pressure decay test	Pass	Pass
Back inlet pressure decay test	Pass	N/A

© Agilent Technologies, Inc. 2020

7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	N/A
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	1
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	
PP Inlet PM kit	5188-6498	7890A/B	
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	
MMI Cleaning Kit	G3510-60820	7890A/B	
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	

© Agilent Technologies, Inc. 2020

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

Service Completion

Service request number 6006590978 Date service completed 13 Feb 2024

Agilent signature [signature] Customer signature [signature]

Total number of pages in this document _____

Revision: 2.00, Issued: December 30, 2020
Agile Document Number: D0007063
DE number: 44166.7597222222
© Agilent Technologies, Inc. 2020

Agilent Preventive Maintenance Services

Agilent GCMS Preventive Maintenance

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.

Agilent CrossLab
From Insight to Outcome

Introduction

This checklist covers the following model(s):

Type	Model
SQ	5973 Series MSD
SQ	5975 Series MSD
SQ	5977 Series MSD
TQ	7000 Series MS/MS
TQ	7010 Series MS/MS
QTOF	7200 Series QTOF
QTOF	7250 Series QTOF

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Customer Responsibilities

Customers should ensure that all necessary operating supplies, consumables, and usage-dependent items such as gases, vials, syringes, calibrant solution and solvents required for successful preventive maintenance are available. A customer representative should be available while the preventive maintenance is being performed.

© Agilent Technologies, Inc. 2023

Agilent

Agilent CrossLab
From Insight to Outcome

Important notice for customers

The customer should complete the following before the Support Provider arrives on site:

☑ Perform an autotune and retain the printed tune report just prior to the start of the PM to verify performance of the equipment.

Note: it is recommended to have the customer run the autotune and tune evaluation prior to the PM and then start the vent cycle so that the instrument will be ready for the service representative.

Important Customer Web Links

- To access Agilent training and education, visit http://www.agilent.com/chem/training to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit https://www.agilent.com/en-us/agilentresources. The following information topics are available:
  - Sample Prep and Containment
  - Chemical Standards
  - Analysis
  - Service and Support
  - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at https://www.youtube.com/user/agilent
- **Need to place a service call?** Flexible Repair Options | Agilent

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.

© Agilent Technologies, Inc. 2023

Agilent

- Complete the relevant checkboxes in the checklist using either a "**X**" or tick mark "✓".
- Check "**Service not applicable**" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in order by sections: Review, System Checks, Pump maintenance, Cleaning System and Filters, then System Post Check.
    - The tasks in each section may be completed in the most logical order relevant to the system. Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Verification section
- Complete Signature Page and attach Signature Page to Service Order.

Additional Instruction Notes

- Preventive maintenance is a factory recommended procedure designed to reduce the likelihood of electromechanical failures. Failure to perform preventive maintenance may reduce the long-term reliability of certain instruments and systems. **Two preventative maintenances (PMs) per year are recommended, the Major PM Service will be performed annually with an Interim PM performed 6 months after the Major PM.**

Definition of the Task/Recommended items within the document

Task		Recommended			
Yes	No	Interim	Major	As Needed	
✓					**Yes** selected means that the task was done or the part was required
	✓				**No** selected means that the task was not done or the part was not required.
		✓			**Interim** selected means that this task is recommended to be done at 6-month intervals
			✓		**Major** selected means that this task is recommended to be done yearly; if the customer would like a service to be done at the 6-month interval then the service could be purchased
				✓	**As needed** selected means that the task was done, or the part was used as needed. For example, there could be two types of filters that could be used, and this was the one selected.

© Agilent Technologies, Inc. 2023

Instrument Maintenance

Select the appropriate service to be performed.

- ☐ Interim Preventive Maintenance (when available, is typically 6 months or at the request of the customer)
- ☑ Major Preventive Maintenance (Yearly)
- ☐ Enhanced Preventive Maintenance (when available, is provided "As needed")

System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID	
Instrument System Site and Location	SECOT, Bangkok

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3172A	US13343601
2.	
3.	
4.	
5.	
6.	

Preparation

- ☑ Discuss any specific issues with the customer before starting.
- ☑ Review the instrument logbook for recorded problems and comments.
- ☑ Save instrument control settings before starting the procedure.
- ☑ Perform a general inspection of the system for cleanliness.
- ☑ Check for proper installation of parts, assemblies, sensors etc.
- ☑ Check system for required installation of components and implementation of Service Notes
- ☑ Check firmware version(s). Updating to the most current versions is strongly recommended. Verify with the customer before updating.

© Agilent Technologies, Inc. 2023

Agilent CrossLab
From Insight to Outcome

Preventive Maintenance Procedures

☐ Service Not Applicable

Interim / Major Preventive Maintenance – GCMS

Yes/No		Interim/Major		Description
☑	☐	☑	☑	Perform general inspection of system for cleanliness
☑	☐	☑	☑	Discuss any problems the customer is having with the instrument
☑	☐	☑	☑	Review customer maintenance records and exclude maintenance on recently serviced items
☑	☐	☑	☑	Review the most recent autotune report. This will give a starting point for evaluating spectral peaks, baseline noise, peak shape, mass assignments and resolution.

Interim / Major Preventive Maintenance – System Checks

☐ Service Not Applicable

				System Checks
Yes/No		Interim/Major		Description
☑	☐	☑	☑	Verify that calibration peaks were seen prior to starting the PM
☑	☐	☑	☑	Vent the instrument
☑	☐	☑	☑	Inspect vacuum hoses, pump, exhaust tubing, and power cords for excessive wear.
☑	☐	☑	☑	Visually inspect calibrant levels – PFTBA PFDTD (if appl.), IRM (if appl.). Refill if available.
☑	☐	☑	☑	Look for any obvious external damage or problems.
☑	☐	☑	☑	Clean air intake(s). Cosmetic cover(s) may need to be removed.
☑	☐	☑	☑	Verify system line voltage meets instrument specifications: Yes ☐ No ☐
☐	☐	☑	☑	For HydroInert systems, verify customer is running hydrogen: Yes ☐ No ☑

Interim / Major Preventive Maintenance – Wet Mechanical vacuum pumps

☐ Service Not Applicable

Yes/No	☐	☐		Wet Mechanical vacuum pumps
Yes/No		Interim/Major		Description
☑	☐	☑	☑	Check for evidence of oil leakage. Check pump gasket for leakage.
☑	☐	☐	☑	GC/MS SQ with diffusion pump; drain and replace diffusion pump oil.
☑	☐	☑	☑	Drain and replace mechanical pump oil.
☐	☑	☑	☑	Replace Oil Mist Filter if applicable.

© Agilent Technologies, Inc. 2023

Agilent

Agilent CrossLab
From Insight to Outcome

Yes/No	☐	☐		Wet Mechanical vacuum pumps
☐	☑	☑	☑	Discuss with customer the need for more frequent oil changes if the oil is dirty
☐	☑	☑	☑	Don't use mist filters with Chemical Ionization.
☑	☐	☑	☑	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed. Visually confirm that no oil returns up vacuum hose.

Interim / Major Preventive Maintenance – Dry Mechanical vacuum pumps - Diaphragm

☑ Service Not Applicable

Yes/No	☐	☐		Dry Mechanical vacuum pumps - Diaphragm
Yes/No		Interim/Major		Description
☐	☐	☑	☑	Check for evidence of poor vacuum – Turbo power demand, poor manifold vacuum, etc.
☐	☐	☑	☑	Clear air flow paths of dust.
☐	☐	☑	☑	If vacuum is poor, then replace the diaphragm pump.
☐	☐	☑	☑	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.

Interim / Major Preventive Maintenance – Dry Mechanical vacuum pumps - Scroll

☑ Service Not Applicable

Yes/No	☐	☐		Dry Mechanical vacuum pumps - Scroll
Yes/No		Interim/Major		Description
☐	☐	☑	☑	Replace the tips seal on the IDP pump.
☐	☐	☑	☑	Check for evidence of poor vacuum – Rough vac pressure, turbo power demand, poor manifold vacuum, etc.
☐	☐	☑	☑	Replace the Exhaust Filter if required.
☐	☐	☑	☑	Discuss with customer the need for more frequent changes, if needed.
☐	☐	☑	☑	Inform customer that pump gas ballast should be installed all the time.
☐	☐	☑	☑	Perform anti-suckback valve test. Power on until side plate is held closed, power off and check that side plate holds closed.

© Agilent Technologies, Inc. 2023

Agilent

Interim / Major Preventive Maintenance – Cleaning System and Filters

☐ **Service Not Applicable**

Cleaning System and Filters				
Yes/No	Interim/Major		Description	
		Fans		
☑ ☐	☑	☑		Remove dust from fans and vent covers.
☑ ☐	☑	☑		Verify fans are functional and that there is enough space around the instrument for proper cooling.
		Source cleaning (all sources **except** HydroInert)		
☑ ☐	☐	☑		Open analyzer and remove the source.
☑ ☐	☐	☑		Disassemble, Clean, Re-assemble source. (7200, also, remove and clean entrance lens)
☑ ☐	☐	☑		Re-install source and close analyzer.
		HydroInert Source		
☐ ☑	☐	☐		Source **NOT** to be abrasively cleaned. No cleaning required at PM. If a decrease in performance is observed, recommend to the customer that filaments, insulators (repeller and extractor), extractor lens, and repeller lens may need to be replaced to restore performance. HydroInert source should not be run with helium carrier.
		Filters		
☑ ☐	☐	☑		Replace RMSH-2 Helium gas filter (collision cell gas) – if applicable.
☐ ☑	☐	☑		Replace RMSN-2 Nitrogen gas filter (collision cell gas) – if applicable.
☐ ☑	☐	☑		Replace RMSHY-2 Hydrogen gas filter (HydroInert and JetClean) – if applicable.
☐ ☑	☐	☑		CP17973 – Gas Clean GS/MS Filter (for He, N2 or H2 carrier) – if required
☐ ☑	☐	☑		5190-9071 – Methane Gas Filter (CI systems) – if applicable

Guidance: Gas filters need to be changed only if required (ie indicating traps show color change, or if Big Universal Trap are approaching saturation based on time installed or number of gas cylinders changed for that trap)

© Agilent Technologies, Inc. 2023

Interim / Major Preventive Maintenance – System Post Check

☐ **Service Not Applicable**

System post-check				
Yes/No	Interim/Major		Description	
☑ ☐	☑	☑		Pump system back down. Wait until system stability has been achieved.
☑ ☐	☑	☑		Verify system vacuum reading(s) via the gauge controller.
☑ ☐	☑	☑		Leak Check
☑ ☐	☑	☑		Verify system in manual tune
☑ ☐	☑	☑		Compare against previous tune file report(s)
☑ ☐	☑	☑		Change to Tune and verify that all temperatures, pressures, and gas flows reach method set points
☑ ☐	☑	☑		Check manually that you have calibration peaks.
☑ ☐	☑	☑		EI Autotune Performed

Guidance: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument setup and checkout.

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Record the PM event in the Smart Alerts logbook, if applicable.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments..
- ☑ Review this service, parts replaced, and test results obtained with the customer.
- ☑ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☑ Complete Signature Page and attach Signature Page to Service Order.

Test Results

Test Description	Expected Test Result	Actual Test Result

© Agilent Technologies, Inc. 2023

Agilent CrossLab
From Insight to Outcome

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the service review or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number: 6006590978

Date of Service Completion: 13 Feb 2024

Service Engineer Name: Suparsh N.

Customer Name:

Service Engineer Signature:

Total number of pages in this document:

© Agilent Technologies, Inc. 2023

Agilent

Agilent CrossLab
From Insight to Outcome

Interim / Major Preventive Maintenance – System Post Check

☐ Service Not Applicable

System post-check				
Yes/No	Interim	Major	Description	
☑	☐	☑	☑	Pump system back down. Wait until system stability has been achieved.
☑	☐	☑	☑	Verify system vacuum reading(s) via the gauge controller.
☑	☐	☑	☑	Leak Check
☑	☐	☑	☑	Verify system in manual tune
☑	☐	☑	☑	Compare against previous tune file report(s)
☑	☐	☑	☑	Change to Tune and verify that all temperatures, pressures, and gas flows reach method set points
☑	☐	☑	☑	Check manually that you have calibration peaks.
☑	☐	☑	☑	EI Autotune Performed

Guidance: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument setup and checkout.

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Record the PM event in the Smart Alerts logbook, if applicable.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review this service, parts replaced, and test results obtained with the customer.
- ☑ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☑ Complete Signature Page and attach Signature Page to Service Order.

Test Results

Test Description	Expected Test Result	Actual Test Result

© Agilent Technologies, Inc. 2023

Agilent

Parts for consumption during PM

Common Oil and MS Gas Filters – 5973/5975/5977/7000/7010/7200/7250 Series

Part Description	Part Number	Interim	Major	As Needed
Agilent AVF Platinum, 1 quart	5191-5851	✓	✓	✓
Helium gas filter* (collision cell gas) – if required	RMSH-2		✓	✓
Nitrogen gas filter*(collision cell gas) – if required	RMSN-2		✓	✓
Hydrogen gas filter* ^ (HydroInert and JetClean) – if required	RMSHY-2		✓	✓
Chemical Ionization Gas Purifier (CI systems) (Methane) – if required	5190-9071		✓	✓
Gas Clean GS/MS Filter (for He, N2 or H2) – if required	CP17973		✓	✓
# Gas Clean Filter Kit GC/MS 1/8 in (complete replacement kit - bench mounted) – if required	CP17974			✓
# Gas Clean Carrier Gas Kit for 7890 for He, N2 or H2; Bracket, Mount and Filter – if required	CP17988			✓
# Gas Clean Carrier Gas Kit for 8890 & 8860 for He, N2 or H2; Bracket, Mount and Filter – if required	CP179880			✓

Gas filters need to be changed only if required (ie indicating traps show color change, or if Big Universal Trap are approaching saturation based on time installed or number of gas cylinders changed for that trap)

* Big Universal Trap (BUT), 1/8" fittings
^ HydroInert and JetClean Systems
Alternate Gas Clean kit part numbers. A Gas Clean filter is included in the kits. They are only necessary if replacing carrier gas Big Universal Traps with indicating traps

MS Maintenance Supplies for 5973/5975/5977 Series

Part Description	Part Number	Interim	Major	As Needed
Diffusion pump fluid (Diffusion Pump Models)	6040-0809 Qty 2		✓	✓
Exhaust oil mist trap (threaded) Edwards/Pfeiffer	G1099-80039	✓	✓	✓
DS42 Oil Mist Eliminator 3/4G & 3/8	SR03706556	✓	✓	✓
IDP-3 Tip Seal Replacement Kit (IDP-3 Dry Scroll Pump Models – Includes tip seal, 60mm filter element, tools, mask and cleaning supplies)	G7077-67018	✓	✓	✓
IDP-3 Tip Seal Replacement Kit (no tools – CSD P/N)	5190-9561	✓	✓	✓
IDP-3 Tip Seal Replacement Kit (no tools – VPD P/N)	IDP3TS	✓	✓	✓
Filter element for IDP-3 (diameter: 60mm)	REPLSLRFILTER2	✓	✓	✓

© Agilent Technologies, Inc. 2023

Agilent

MS Maintenance Supplies for 7000/7010 Series

Part Description	Part Number	Interim	Major	As Needed
Oil Mist Filter RV5	G6600-80043	✓	✓	✓
IDP-10 Tip Seal Replacement Kit (IDP-10 Dry Scroll Pump Models – Includes tip seal, 102mm filter element, tools, mask and cleaning supplies)	G7004-67023	✓	✓	✓
IDP-10 Tip Seal Replacement Kit (no tools etc. – VPD P/N)	X3807-67000	✓	✓	✓
Filter element for IDP-10/IDP15 (diameter: 102mm)	REPLSLRFILTER	✓	✓	✓
Filter element for IDP-10/IDP15 (diameter: 79mm)	REPLSLRFILTER1	✓	✓	✓

MS Maintenance Supplies for 7200/7250 Series

Part Description	Part Number	Interim	Major	As Needed
RIS Probe Maintenance Kit (7200 Series only)	G7005-60170		✓	✓
DS202 Oil Mist Eliminator	SR03706800	✓	✓	✓
DS202 3/8' Magnetic Plug and Gasket	SR03701824	✓	✓	✓
IDP-15 Tip Seal Replacement Kit (IDP-15 Dry Scroll Pump Models – Includes tip seal, 102mm filter element, tools, mask and cleaning supplies)	5190-9613	✓	✓	✓
IDP-15 Tip Seal Replacement Kit (no tools etc.– VPD P/N)	X3815-67000	✓	✓	✓
Filter element for IDP-10/IDP15 (diameter: 102mm)	REPLSLRFILTER	✓	✓	✓
Filter element for IDP-10/IDP15 (diameter: 79mm)	REPLSLRFILTER1	✓	✓	✓

HydroInert Source Supplies

To determine if replacement of HydroInert parts is required, please review tune history and sample signal intensity performance. If performance is decreasing, the below parts maybe use to restore performance as part of the PM.

One way to determine if the source performance on SQ is being affected is to review the gain factor history in autotune reports or tune history csv file. If the gain factor is increasing the source performance maybe degrading.

Since TQ tunes to a fixed gain factor, review PFTBA abundance. If PFTBA abundance is decreasing over time, the source performance maybe degrading.

Real sample/standard area counts are another way to determine the performance, there could also be other factors that affect compounds abundance such as inlet and column status.

Part Description	Part Number	Interim	Major	As Needed
Repeller Insulator (qty 2)	G1099-20133			✓
Lens insulator for Extractor (ring insulator)	G3870-20445			✓
HydroInert Extractor lens (9mm)	G7078-20909			✓
HydroInert Repeller	G7078-20902			✓

© Agilent Technologies, Inc. 2023

Agilent

Common Parts Reference
(Purchased by customer, not included as part of PM)

Filaments and Calibrant Supplies 5973/5975/5977/7000/7010/7200/7250 Series

Part Description	Part Number	SQ	TQ	QTOF
EI High Temperature Filaments	G7005-60061 Qty 2	597X	7000x	N/A
HES EI Filaments	G7002-60001	5977B/C	7010x	N/A
LE-EI Filaments (7250 QTOF)	G3850-60021	N/A	N/A	7250
CI High Temperature Filament – SQ, TQ, 7200 QTOF	G7005-60072	N/A	N/A	7200A/B
Axial CI Filament, W/Re Straight (7250 QTOF)	G7250-60095	N/A	N/A	7250
PFTBA GCMS Tuning Standard calibrant	05971-60571	597X	70X0	72X0
PFDTD calibrant, 1 mL	8500-8510	597X	70X0	72X0
PFET, IRM calibrant for GC QTOF 0.5 mL (7200)	5190-0531	N/A	N/A	7200A/B

Transfer line seals and springs 5973/5975/5977/7000/7010/7200/7250 Series

Part Description	Part Number	SQ	TQ	QTOF
CI Interface tip seal (ceramic tip and spring combo) (non-captured CI tip seal interface) (5973, 5975, 7000B)	G1999-60412	5973, 5975	7000B	N/A
CI Interface tip seal (ceramic tip and spring low/non-magnetic spring combo) (non-captured CI tip seal interface) (7010A)	G7002-60412	N/A	7010A	N/A
CI Interface tip seal spring (spring only)	G1999-20023	597X	70X0	72X0
CI Interface tip seal (tip only) (captured style)	G3870-20542	5977x	70X0	72X0
Transfer-Line Tip Base, Threaded (captured style)	G3870-20548	5977x	70X0	72X0
Transfer-Line Tip Cap, Threaded (captured style)	G3870-20547	5977x	70X0	72X0
RIS Xfer Tip (7200)	G7005-20542	N/A	N/A	7200A/B
RIS Xfer Tip Spring (7200)	G7005-20024	N/A	N/A	7200A/B

MS Maintenance Supplies for Intuvo 9000 MS Series

Part Description	Part Number	SQ	TQ	QTOF
Swaged MS Tail - Packaged	G4590-60009	5977x	7000	N/A
Swaged MS Tail (HES) - Packaged	G4590-60109	5977x	7010x	N/A

© Agilent Technologies, Inc. 2023

Ion source insulators for 5973/5975/5977/7000/7010/7200/7250 Series

Part Description	Part Number	SQ	TQ	QTOF
Repeller insulator (SQ, TQ)	G1099-20133 Qty 2	597X	7000x	N/A
Lens insulator for extractor lens (ceramic ring insulator) (Extractor source)	G3870-20445	5977x	7000C/D/E	N/A
Lens insulator for Extractor lens (Vespel ring insulator) (7000B extractor ion source)	G7000-20445	N/A	7000B only	N/A
Lens stack insulator for SS, Inert, Extractor sources (captures ion focus and entrance lens) (Vespel)	G3170-20530	597X	7000x	N/A
Lens insulator for Extractor lens for HES/LEEI (ceramic ring insulator)	G7002-20064	5977B/C	7010x	7250
Lens stack insulator/holder for HES/LLEI (Vespel)	G7002-20074	5977B/C	7010x	7250
CI Repeller Lens Insulator (SQ, TQ)	G1999-20433	597X	70X0x	N/A
CI Lens stack insulator (SQ, TQ) (Vespel)	G3170-20540	597X	70X0x	N/A
Repeller insulator (7200 RIS) (Ceramic)	G7005-20447	N/A	N/A	7200A/B
Extractor Lens Insulator (7200 RIS) (Vespel)	G7005-20133	N/A	N/A	7200A/B
Ion Focus Insulator (7200 RIS) (Vespel)	G7005-20442	N/A	N/A	7200A/B
CI Repeller Insulator/bushing (7200 RIS) (Ceramic)	G7005-20030	N/A	N/A	7200A/B

HydroInert coated lenses for 5977/7000 Series

Part Description	Part Number	SQ	TQ	QTOF
HydroInert Repeller	G7078-20902	5977x	7000C/D/E	N/A
Ext Source Body – HydroInert	G7078-20903	5977x	7000C/D/E	N/A
HydroInert Extractor lens (9mm)	G7078-20909	5977x	7000C/D/E	N/A
Ion Focus Lens – HydroInert	G7078-20905	5977x	7000C/D/E	N/A
Entrance Lens – HydroInert	G7078-20904	5977x	7000C/D/E	N/A

© Agilent Technologies, Inc. 2023

Heater/Sensor assemblies for 5973/5975/5977/7000/7010/7200/7250 Series

Part Description	Part Number	SQ	TQ	QTOF
Stainless Steel Heater/Sensor assembly (SST EI 350)	G3870-67180	597X	N/A	N/A
Inert Heater/Sensor assembly (inert EI 350)	G3870-67179	597X	7000A/B	N/A
Extractor Heater/Sensor assembly (Xtr EI 350)	G3870-67177	5977x	7000C/D/E	N/A
H2 EI Heater/Sensor Assembly – HydroInert (H2 EI 350)	G7078-67910	5977x	7000C/D/E	N/A
CI 350 Heater/Sensor Assembly (CI 350)	G3870-67415	597X	70X0x	N/A
Ring heater/sensor assembly (HES, RIS and LEEI) (ceramic ring)	G7002-60058	5977B/C	7010x	72X0

Rough pump hoses 5973/5975/5977/7000/7010/7200/7250 Series

Part Description	Part Number	SQ	TQ	QTOF
Foreline Hose - imbedded spring	G7077-60119	597X	70X0x	72X0

Common MS Maintenance Supplies

Part Description	Part Number	SQ	TQ	QTOF
Abrasive paper, 30 µm	5061-5896	597X	70X0	72X0
Alumina powder	393706201	597X	70X0	72X0
Cloths, clean (pkg of 15)	05980-60051	597X	70X0	72X0
Cloths, cleaning (pkg of 300)	9310-4828	597X	70X0	72X0
Cotton swabs (pkg of 100)	5080-5400	597X	70X0	72X0
Gloves, clean, large	8650-0030	597X	70X0	72X0
Gloves, clean, small	8650-0029	597X	70X0	72X0

© Agilent Technologies, Inc. 2023

Agilent

Teledyne Tekmar ATOMX Purge and Trap Preventive Maintenance Checklist - Standard

Agilent Technologies

Agilent Preventive Maintenance provides factory recommended service for your analytical systems to assure reliable operation and the accuracy of your results. Delivered by highly-trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak.

For more information about Agilent Technologies services please visit our web site using the following URL http://www.chem.agilent.com/en-us/products/services/pages/default.aspx

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of additional or special procedures and/or parts for the instrument service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Service Engineer's Responsibilities

- Only complete/printout pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using a "X" or tick mark "✓" in the checkbox.
- Complete Not Applicable check boxes to indicate services not delivered, as needed.
- Complete the PM service in the order of the tasks listed.
- Complete the Service Review section together with the customer.

Copyright © 2013 Agilent Technologies

System Information

Guidance

☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument system name and ID	
Instrument system site and location	SECOT, Bangkok
List system component product numbers	**List the serial numbers of each component**
1. TMK-ATOMX	1. US 17296002
2.	2.
3.	3.
4.	4.
5.	5.
6.	6.
7.	7.
8.	8.
9.	9.
10.	10.

Preparation

☑ Discuss any specific issues with the customer prior to starting.
☑ Review the instrument logbook.
☑ Save instrument control settings before starting the procedure.
☑ Perform general inspection of system for cleanliness
☑ Check for proper installation of safety-related parts, assemblies , sensors etc
☑ Check for required firmware updates and verify with customers if they would like it installed.

Check External Supplies

☐ **Section NOT Applicable**
☑ Verify the gas source is supplying an input pressure of 50 - 100 psi to the ATOMX. If the customer is using a gas cylinder, verify the cylinder is at 500+ psi.
☑ Verify that the waste container has sufficient volume to contain the waste generated. Empty if necessary.
☑ Replace the DI water supply with fresh DI water.
  - Make sure the DI water supply is sufficient for sample analysis (1 Liter minimum)
☑ Make sure the methanol supply is sufficient for sample analysis.

Atomx Leak and Pressure Check

☐ **Section NOT Applicable**
☑ Scan through the sample log to verify that the purge pressures are staying consistent throughout the daily runs.
☑ Use the Teklink software to check the standard pressure.
☑ Run a leak check to ensure that the unit is leak tight.

Inspect ATOMX Hardware

☐ **Section NOT Applicable**
☑ Check the tray vial holes for foreign particles. Clean if necessary.
☑ Inspect the needle for particles or sample build up. Clean if necessary.
☑ Inspect the sparger glassware for damage and/or discoloration that could restrict flow or cause contamination. Replace if necessary.
☑ Inspect the drain tubing for clogging. Replace the drain line if necessary.
☑ Lubricate the ATOMX Carousel Drive. Refer to the diagram on page 6-25 of the ATOMX User Manual for lubrication points. Teledyne Tekmar recommends using DuPont Krytox lubrication.
☑ Lubricate the ATOMX Elevator. Refer to the diagram on page 6-32 of the ATOMX User Manual for lubrication points. Teledyne Tekmar recommends using DuPont Krytox lubrication.

Restore Instrument

Guidance

If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the PM service activity in the customer's instrument records/logbook
- ☑ Update/reset instrument maintenance counters as appropriate
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section below if there are additional comments
- ☑ Review the service and any test results with the customer.
- ☑ If the Instrument firmware was updated, record the details of the change in the Service Engineer's Comments box below or if necessary, in the customer's IQ records.

Product or Product Type Test Results Table

Test Description	Expected Test Result	Actual Test Result
Leak Test	Pass	Pass

Product or Product Type Parts List Table

Part Description	Part Number	Product or Model# where used	Quantity Consumed
Sparger Glassware	Ask the customer what size sparger glassware they are using; refer to the ATOMX parts list for part numbers.	TMR-ATOMX	1
Lubricant, Dupont Krytok	15-0293-000	TMR-ATOMX	1
Tubing, Drain, Self Retracting	15-0087-002	TMR-ATOMX	1

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write in this box.

Other Important Customer Web Links

- ☐ How to get information on your product: Literature Library - http://www.agilent.com/chem/library
- ☐ Need to know more? - www.agilent.com/chem/education
- ☐ Need technical support, FAQs? - www.agilent.com/chem/techsupp
- ☐ Need supplies? - www.agilent.com/chem/supplies

Service Completion

Service request number 6006590978 Date service completed 13 Feb 2024

Agilent signature [signature] Customer signature [signature]

Number of pages in this document _____

Agilent CrossLab
From Insight to Outcome

Agilent CrossLab Start Up Services

Agilent 7890 Gas Chromatograph Preventive Maintenance Checklist

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results.

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides everything you need to reduce unplanned downtime and keep your systems operating at their peak. This checklist will be completed at the end of the service and provided to you as a record of the preventive maintenance activities.

Agilent

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures.
- Any parts, not included in the Parts Lists section of this document, are not part of the recommended Preventive Maintenance service, nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.

Important Customer Web Links

- For more information about ***Agilent Technologies services***, please visit our website using the following URL: http://www.agilent.com/en-us/products/crosslab-instrument-services/service-repair
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit https://community.agilent.com/welcome.
- To access **Agilent University**, visit http://www.agilent.com/crosslab/university/ to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- A useful **Agilent Resource Center** web page is available, which includes short videos on maintenance, quick lists of consumables for new instruments, and other valuable information. Check out the Resource Page here: https://www.agilent.com/en-us/agilentresources.
- Need technical support, FAQs, supplies? – visit our **Support Home page** http://www.agilent.com/search/support.
- **Videos** about specific preparation requirements for your instrument can be found by searching the ***Agilent YouTube*** channel at https://www.youtube.com/user/agilent.
- **7890B Manuals** are also available on Agilent.com:
  - **Safety** https://www.agilent.com/cs/library/usermanuals/public/7890B_Safety.pdf
  - **Installation and First Startup** https://www.agilent.com/cs/library/usermanuals/Public/7890B_Installation.pdf
  - **Operation Manual** https://www.agilent.com/cs/library/usermanuals/Public/7890B_Operation.pdf
  - **Maintaining Your GC** https://www.agilent.com/cs/library/usermanuals/public/G3430-90052%207890B_Maintaining%20Guide.pdf

Revision: 2.01, Issued: September 15, 2021
Agile Document Number: D0013618
DE number: 44166.7597222222
© Agilent Technologies, Inc. 2021

Agilent

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check **"Section not applicable"** check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance service in the order of the tasks listed.
- Complete the Service Review section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Complete the total number of pages field in the Service Completion section
- ***Ask the customer to sign the Service Completion section including the customer's and your signature.***

Additional Instruction Notes

- Check for any active service notes for this unit. If there are any applicable "Safety" or "Modification Recommended" Service notes, plan to implement the changes on this unit before doing any qualification service.
- Do not implement firmware updates, unless you get approval from the customer and are sure that they are compatible with the instrument control software.

© Agilent Technologies, Inc. 2021

System Information

❑ Check this box if an instrument configuration report is attached instead of completing the table below.

Instrument System Name and ID	7890A GC System
Instrument System Site and Location	SECOT CO., LTD.

List System Component Product Numbers	List the Serial Numbers of each Component
1. G3440B	CN15343147
2. G4513A	CN11350133
3. G4514A	CN13080006
4. N/A	N/A
5. N/A	N/A
6. N/A	N/A
7. N/A	N/A
8. N/A	N/A
9. N/A	N/A
10. N/A	N/A

Preparation

☑ Discuss any specific issues with the customer before starting.
☑ Review the instrument logbook for recorded problems and comments.
☑ Save instrument control settings before starting the procedure.
☑ Perform a general inspection of the system for cleanliness.
☑ Check for proper installation of parts, assemblies, sensors etc.
☑ Check system for required installation of components, settings as defined by current Service Notes.
☑ Check for required firmware updates and verify with customers if they would like them installed.
❑ Before starting the following procedures, record the Detector Signal Output(s) in the results table. If the GC is turned OFF or in a service mode, comparing the detector outputs before and after the service is not possible.

© Agilent Technologies, Inc. 2021

Preventive Maintenance Procedure

Clean and inspect GC

- ☑ Unplug power cord from the power source.
- ☑ Open GC covers and vacuum/remove any dust/debris. Pay particular attention to cooling fans.
- ☑ Inspect internal connectors for proper contact and placement.
- ☑ Reconnect Power to the GC. Power the GC on and verify the power on self-test passed.
- ☑ Verify oven motor spins freely and turns on with the oven door closed; off when the door is opened.
- ☑ Verify operation of all other fans - the inlet and EPC cooling fans.
- ☑ Verify oven intake/outlet flap assembly is operating smoothly while heating and cooling the oven

Inlet and detector consumable replacement

- ☑ For the inlets installed, perform inlet maintenance as defined in the 7890 manual – "Maintaining Your GC" - for the inlet(s) installed.
- ☑ Replace the split vent trap cartridge filter on units with these inlets: Split/Splitless Capillary (SSL), Multi-Mode Inlet (MMI), Programmed Temperature Vaporizer (PTV), Volatiles Interface (VI).
- ☑ If the inlet system is used in Split Mode with viscous samples, inspect and clean the split vent tube on the inlet and flush or replace the tubing between the inlet and the split vent trap.
- ☑ If the GC includes a Flame Ionization Detector (FID), replace the jet. If the ignitor shows any buildup of sample or corrosion, replace the ignitor. Examine the FID collector and castle assemblies for contamination – clean as necessary.

Zero Sensors and Leak test

- ☑ Zero all pressure sensors per the procedure in the 7890 "Advanced User Guide".
- ☑ Perform inlet pressure decay test(s) as defined in the 7890 "Troubleshooting Manual".
  If the PM is done in preparation for an Operational Qualification, then the pressure decay test defined within that protocol can be used for the PM.
- ☑ Record if test passed or failed in the results table.

© Agilent Technologies, Inc. 2021

ALS Maintenance

- ❑ **Section NOT applicable**
- ☑ Check all cabling and configuration settings between GC, tray, and injectors.
- ☑ Vacuum or remove any dust, especially around fans.
- ☑ Check operation of all fans.
- ☑ Check syringe for smooth plunger operation.
- ☑ Check for smooth operation of the needle support – clean if necessary

Restore Instrument

- ☑ Restore the normal operating conditions or customer method using the Data System.
- ☑ Purge the system with carrier flow for 15 minutes
- ☑ Bake out the system, then restore the normal operating conditions
- ☑ After equilibration, check and record the post PM detector signal output values.
  Results should be similar or lower than the detector outputs recorded prior to PM.
- ☑ Perform a chemical checkout. If this is a routine PM, inject the customer's sample using the ALS if applicable. This will act as a final checkout of both the ALS and the GC.

Note: If the PM Service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

© Agilent Technologies, Inc. 2021

Signature Page

Service Review

- ☑ Attach available reports/printouts of all tests to this documentation.
- ☑ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☑ Update/reset instrument maintenance counters as appropriate.
- ☑ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☑ Complete the Service Engineer Comments section if there are additional comments.
- ☑ Review with the customer this service, parts replaced, and test results obtained.
- ☐ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box or if necessary, in the customer's IQ records.
- ☐ Supply the customer with a copy of the Smart Alerts flyer.
- ☐ Describe Smart Alerts to the customer.
- ☐ Install Smart Alerts if requested.

7890 GC Test Results Table

Detector Signal Outputs		Before PM Service	After PM Service
Front detector output	uECD	-	180
Back detector output	FID	-	15
AUX detector output		N/A	N/A
Pressure decay test		**Expected test result**	**Actual test result**
Front inlet pressure decay test		Pass	Pass
Back inlet pressure decay test		Pass	Pass

© Agilent Technologies, Inc. 2021

7890 Parts List Table

The following kits are recommended for capillary and purged packed inlets. If this is a general PM and the customer has a preferred set of consumables, you may use the customer's consumables.

Part description	Part number	Product or model# where used	Quantity consumed
SSL Capillary Inlet PM kit, Splitless	5188-6497	7890A/B	2
SSL Capillary Inlet PM kit, split	5188-6496	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Low Pressure Drop Split Liner - with Glass Wool	5190-2295	7890A/B	N/A
PP Inlet PM kit	5188-6498	7890A/B	N/A
Split vent trap PM kit, single cartridge (for MMI, PTV & VI)	5188-6495	7890A/B	N/A
MMI Cleaning Kit	G3510-60820	7890A/B	N/A
PTV Septumless Head Rebuild Kit	5182-9747	7890A/B	N/A
PTV Septumless Head Teflon Guide	5182-9748	7890A/B	N/A
Ignitor (glow plug) assembly with O-ring	19231-60680	7890A/B	1
FID Collector Rebuild/Cleaning Kit	G1531-67000	7890A/B	N/A
Standard .011-inch FID Jet for capillary FID base	G1531-80560	7890A/B	N/A
High Temperature .018-inch FID Jet for capillary FID base	G1531-80620	7890A/B	N/A
Standard .018-inch FID Jet for packed column with packed FID base	18710-20119	7890A/B	N/A
Standard .011-inch FID Jet for capillary column with packed/adaptable FID base	19244-80560	7890A/B	N/A
High Temperature .018-inch FID Jet for capillary column with packed/adaptable FID base	19244-80620	7890A/B	N/A
NPD Jet, universal fit, .011-inch ID	G1534-80580	7890A/B	N/A
NPD Jet, universal fit, .011-inch ID Extended tip	G1534-80590	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Gold Seal with Washer	5190-6144	7890A/B	N/A
SSL Capillary Ultra Inert Inlet Splitless Liner - Single taper with Glass Wool	5190-2293	7890A/B	N/A
**FID Collector Replacement Kit, if needed	G1531-67001	7890A/B	N/A

© Agilent Technologies, Inc. 2021

Service Engineer Comments

If there are any specific points you wish to note as part of performing the service or other items of interest for the customer, please write include them in this box.

N/A

Service Completion

Service request number 6006786001 Date service completed 23 May 2024

Agilent signature [signature] Customer signature [signature]

Total number of pages in this document 10

© Agilent Technologies, Inc. 2021

Do not include this section/page in the published, customer-facing PDF version.

This page is only relevant for Agilent source documents for document control purposes and is NOT intended for customer viewing. Refer to the SPIFPM checklist Authoring Guide for more information.

Document Control Logs

Revision Log

Revision	Date	Author	Reason for update
Revision of document	Date of issuance	Author of document	Author to describe main features/changes made for this specific revision
1.0 Draft	4-Mar-2011	Dave Park	Migrated the content of revision A.01.05 to the new Agilent template. Reviewed by subject matter expert, Dave Park.
1.1 Draft	20-Jan-2015	Dave Park	Added Split Vent trap to MMI, PTV and VE - also PTV and FID PM Parts
1.2 Draft	31-March-2015	Dave Park	Added Ultra Inert Gold Seal and Liner to SS Consumables
A.01.11	10-Dec-2015	Dave Park	Added step to perform maintenance on the Split Vent Tube and .018" FID Jet part numbers - Fixed broken web links
2.00	30-Dec-2020	Gary Boardman	Updated New Template and terminology change: Familiarization to Introduction. Create New Agile Document Number: D0007063

Approval Log

Revision	Approver	Title of approver
Add revision number	Add approver name here	Add approver's function or title here
A.01.06	Don Gage	Product support manager
A.01.09	Kai Meng	Product support manager
A.01.10	Suneetha Tippireddy	Product support manager
A.01.11	Suneetha Tippireddy	Product support manager
2.00	Josh Roark	GC Product Support Manager

Designated Evaluation Log

Revision	Designated Evaluator (DE)	Title of DE	DE Number
Add revision number	Add name	Add function or title	Add DE number here
2.00	Michael Zumwalt	CrossLab Start Up Services Application Consulting Lead	44166.7597222222

© Agilent Technologies, Inc. 2021

Request Service No. 099/67

Calibration Certificate

Nomenclature : Brand : Mettler Toledo Type : Top-Loading Electronic Balance

Model : AG245 Serial No. : 1117293916 (198129-0)

Submitted by : Laboratory of SECOT CO., LTD.

Location of Calibration : BAL Room , 6th Floor, Secot Co., Ltd.

Calibration range : 0 – 200 g Scale division : 0.00001 g (41g)/ 0.0001 g (210g)

Calibration date : May 24,2024

Reference Standard No. M2310081S,M2402083S,M2302167S,M2403062N,M2303005N

Traceable to : Metrological Center SCI ECO Services Company Limited.

Thai Caribration Services CO., LTD.

Ambient Condition : Temperature 24.20 – 24.70 °C

Humidity 50.70 – 52.00 % RH

Calibrated By : ..... Approved By : .....

(Miss Pornnapa Budthum) (Miss Narisa Poowasanpetch)

Testing Officer Chief of Technical Management

Date : 25/05/2024 Date : 25/05/2024

Issued Date : May 25,2024

Measurement Report

Request Service No. 099/67

Description : Brand : Mettler Toledo Type : Top-Loading Electronic Balance

Model : AG245 Serial No. : 1117293916 (198129-0)

Calibration range : 0 – 200 g Scale division : 0.00001 g (41g)/ 0.0001 g (210g)

Calibration date : May 24,2024

Ambient Condition : Temperature 24.20-24.70 °C Relative humidity 50.70-52.00 .% RH

Measurement data :

1. Repeatability of Reading :

Load (g)	Standard Deviation of Reading (g)	Maximum Difference between Successive Reading (g)
50	0.000125	0.0004
100	0.000105	0.0003
150	0.000125	0.0003
200	0.000173	0.0005

2. Off-Center Loading :

A Mass of 50.0000 g was placed and moved to various position on the pan.

Unit : g

Center	Front	Left	Back	Right	Center	Maximum Difference
50.00010	50.00032	50.00048	50.00002	50.00008	50.00020	0.00038

Issued Date : May 25,2024

3. Departure from Nominal Valve :

Reading (g)	Correction (g)	Uncertainty (+/- g)
0	0.000000	± 0.000034
0.5	0.000022	± 0.000033
1	0.000037	± 0.000018
10	-0.000067	± 0.000036
20	-0.000060	± 0.000044
40	-0.000193	± 0.000072
60	-0.00032	± 0.00011
80	-0.00033	± 0.00013
100	-0.00048	± 0.00015
120	-0.00049	± 0.00017
140	-0.00040	± 0.00022
160	-0.00054	± 0.00023
180	-0.00053	± 0.00024
200	-0.00084	± 0.00027

Calibrated by : Pornnapa Budthum Approved By : Narisa Poowasanpetch

(Miss Pornnapa Budthum) (Miss Narisa Poowasanpetch)

Testing Officer Chief of Technical Management

Date : 25/05/2024 Date : 25/05/2024

Issued Date : May 25,2024

Calibration Certificate

Nomenclature : Brand : Sartorius Type : Top-Loading Electronic Balance

Model : BSA224S-CW Serial No. : 32191636

Submitted by : Laboratory of SECOT CO., LTD.

Location of Calibration : BAL Room , 6th Floor, Secot Co., Ltd.

Calibration range : 0 – 200 g Scale division : 0.0001 g (220 g)

Calibration date : May 22,2023

Reference Standard No. M2402083S, M2302167S,M2403062N,M2303005N

Traceable to : Thai Carlibration services Co.,Ltd

Ambient Condition : Temperature 23.41-24.71 °C

Humidity 48.2-53.1 % RH

Calibrated By : Khemchuda Insorn Approved By : Narisa Poowasanpetch

(Miss Khemchuda Insorn) (Miss Narisa Poowasanpetch)

Testing Officer Chief of Technical Management

Date : 23/05/2024 Date : 23/05/2024

Issued Date : May 23,2024

Measurement Report

Request Service No.100/67

Description : Brand : Sartorius Type : Top-Loading Electronic Balance

Model : BSA224S-CW Serial No. : 32191636

Calibration range : 0 – 200 g Scale division : 0.0001 g (220 g)

Calibration date : May 22,2023

Ambient Condition : Temperature 23.41-24.71 °C Relative humidity 48.2-53.1 % RH

Measurement data :

1. Repeatability of Reading :

Load (g)	Standard Deviation of Reading (g)	Maximum Difference between Successive Reading (g)
50	0.00007	0.0002
100	0.00005	0.0001
150	0.00005	0.0001
200	0.00005	0.0001

2. Off-Center Loading :

A Mass of 50.0000 g was placed and moved to various position on the pan.

Unit : g

Center	Front	Left	Back	Right	Center	Maximum Difference
49.99990	49.99992	49.99988	49.99992	49.99990	49.99992	0.00004

Issued Date : May 24,2024

3. Departure from Nominal Valve :

Reading (g)	Correction (g)	Uncertainty (+/- g)
0	0.00000	± 0.00007
1	+ 0.00003	± 0.00007
5	+ 0.00004	± 0.00008
10	+ 0.00008	± 0.00008
20	+ 0.00003	± 0.00009
40	+ 0.00012	± 0.00010
60	+ 0.00004	± 0.00012
80	+ 0.00005	± 0.00013
100	+ 0.00006	± 0.00016
120	+ 0.00007	± 0.00018
140	+ 0.00008	± 0.00020
160	+ 0.00006	± 0.00022
180	+ 0.00007	± 0.00024
200	+ 0.00010	± 0.00027

Calibrated by : Khemchuda Insorn Approved By : Narisa Poowasanpetch

(Miss Khemchuda Insorn) (Miss Narisa Poowasanpetch)

Testing Officer Chief of Technical Management

Date : 23/05/2024 Date : 23/05/2024

Issued Date : May 23,2024

Bangkok High Lab Co.,Ltd.
4/176 Soi Ladplakao 66, Ladplakao Rd., Anusawari, Bangkhen, Bangkok 10220
Tel: (662) 971-5800 Fax: (662) 971-5300
Website: www.bangkokhighlab.com E-mail: info@bangkokhighlab.com

NSC-TISI-TIS 17025
CALIBRATION 0366

CERTIFICATE OF CALIBRATION

Certificate No : S2024/033
Page : 1/5
Order No : 010/2024

Customer	:	SECOT COMPANY LIMITED
Address	:	239 Rimklongprapa Road, Bangsue, Bangkok 10800, Thailand
Instrument	:	UV/VIS spectrophotometer
Manufacture	:	Thermo Scientific
Model	:	Genesys 150 UV-VIS
Serial Number	:	9A5Y332022
Environment	:	Temperature (25.1 - 24.8) °C
	:	Humidity (52 - 55) %RH
Received Date	:	February 20, 2024
Calibration Date	:	February 20, 2024
Issued Date	:	February 22, 2024
Calibrate Status	:	No Adjustment
Calibration Area	:	Customer area
Roomname	:	Laboratory Room of SECOT COMPANY LIMITED

Calibrated By : Pacharapol
(Mr. Pacharapol Kwanbang)
Calibration Engineer

Approved By : Teerasak Auiphat
(Mr.Teerasak Auiphat)
Authorized signatory

This calibration certificate shall not be reproduced other than in full except with the prior written approval of the Bangkok High Lab Co.,Ltd.

Bangkok High Lab Co.,Ltd.
4/176 Soi Ladplakao 66, Ladplakao Rd., Anusawari, Bangkhen, Bangkok 10220
Tel: (662) 971-5800 Fax: (662) 971-5300
Website: www.bangkokhighlab.com E-mail: info@bangkokhighlab.com

NSC-TISI-TIS 17025
CALIBRATION 0366

1. Photometric Accuracy

CRMs: Neutral Density Glass Filters **CRMs Serial Number: 10563**

Traceability: Traceable to NIST, U.S.A. through Neutral density filters NIST SRM 930e & 1930, Double Aperture method through Starna certificate report no.113594

Spectral slit width : 2.00 nm

1.1 Reading scale at 420.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5604	0.559	0.0014	0.0044
1.0723	1.073	-0.0007	0.0038
2.1753	2.179	-0.0037	0.0064

1.2 Reading scale at 440.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5503	0.548	0.0023	0.0040
1.0467	1.047	-0.0003	0.0040
2.1117	2.114	-0.0023	0.0064

1.3 Reading scale at 465.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.4996	0.498	0.0016	0.0034
0.9649	0.963	0.0019	0.0040
1.9646	1.966	-0.0014	0.0060

1.4 Reading scale at 546.1 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5136	0.511	0.0026	0.0028
0.9765	0.976	0.0005	0.0028
1.9848	1.984	0.0008	0.0064

Bangkok High Lab Co.,Ltd.
4/176 Soi Ladplakao 66, Ladplakao Rd., Anusawari, Bangkhen, Bangkok 10220
Tel: (662) 971-5800 Fax: (662) 971-5300
Website: www.bangkokhighlab.com E-mail: info@bangkokhighlab.com

NSC-TISI-TIS 17025
CALIBRATION 0366

1.5 Reading scale at 590.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5424	0.540	0.0024	0.0029
1.0130	1.011	0.0020	0.0029
2.0238	2.021	0.0028	0.0061

1.6 Reading scale at 635.0 nm

Filter STDs (Abs) Certificate	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
0.0000	0.000	0.0000	0.0028
0.5265	0.524	0.0025	0.0030
0.9667	0.963	0.0037	0.0031
1.9145	1.910	0.0045	0.0062

2. Photometric Accuracy

CRMs: Potassium Dichromate in Perchloric acid

CRMs Serial Number: 109966 **Blank Serial Number: 110516**

Traceability: Traceable to NIST, U.S.A. through crystalline potassium dichromate NIST SRM 935a through Starna certificate report no.113596

Spectral slit width : 2.00 nm

Wavelength (nm)	Certificate (Abs)	Average Measured Value (A)	Correction (A)	Uncertainty ± (A)
235	0.0000	0.000	0.0000	0.0050
	0.7428	0.738	0.0048	0.0056
257	0.0000	0.000	0.0000	0.0050
	0.8605	0.856	0.0045	0.0055
313	0.0000	0.000	0.0000	0.0050
	0.2885	0.288	0.0005	0.0054
350	0.0000	0.000	0.0000	0.0050
	0.6376	0.635	0.0026	0.0056

Bangkok High Lab Co.,Ltd.
4/176 Soi Ladplakao 66, Ladplakao Rd., Anusawari, Bangkhen, Bangkok 10220
Tel: (662) 971-5800 Fax: (662) 971-5300
Website: www.bangkokhighlab.com E-mail: info@bangkokhighlab.com
NSC-TISI-TIS 17025
CALIBRATION 0366

3. Wavelength Accuracy

Spectral slit width : 2.00 nm

3.1 CRMs: Holmium Glass Filter

CRMs Serial Number: 10763

Traceability: Traceable to NIST Holmium oxide filter NIST SRM 2034, through Starna certificate report no. 113607

Filter STDs (nm) Certificate	Average Measured Value (nm)	Correction (nm)	Uncertainty ± (nm)
241.74	241.301	0.439	0.12
279.44	279.243	0.197	0.12
287.98	287.555	0.425	0.12
334.10	333.778	0.322	0.12
361.00	360.913	0.087	0.12
418.61	418.457	0.153	0.12
453.63	453.543	0.087	0.12
460.05	459.911	0.139	0.12
536.66	536.327	0.333	0.12
637.98	637.449	0.531	0.12

3.2 CRMs: Didymium Glass Filter

CRMs Serial Number: 10764

Traceability: Traceable to NIST Didymium filter NIST SRM 2034, through Starna certificate report no. 113608

Filter STDs (nm) Certificate	Average Measured Value (nm)	Correction (nm)	Uncertainty ± (nm)
585.29	584.949	0.341	0.12
684.49	683.901	0.589	0.12
740.18	739.646	0.534	0.12
748.48	747.844	0.636	0.12
807.03	806.832	0.198	0.12
879.27	878.923	0.347	0.12

Bangkok High Lab Co.,Ltd.
4/176 Soi Ladplakao 66, Ladplakao Rd., Anusawari, Bangkhen, Bangkok 10220
Tel: (662) 971-5800 Fax: (662) 971-5300
Website: www.bangkokhighlab.com E-mail: info@bangkokhighlab.com

NSC-TISI-TIS 17025
CALIBRATION 0366

Certificate No : S2024/033
Page : 5/5

4. *Stray Light

CRMs: Potassium Chloride aqueous solution

CRMs Serial Number: 14912 **Blank Serial Number: 14958**

Traceability: Traceable to NIST, U.S.A. potassium chloride NIST SRM2032, through Starna certificate report no.113597

Spectral slit width : 2.00 nm

Wavelength (nm)	Certificate	Average Measured
201.13	>2A	2.0170
201.13	<1%T	0.9818

5. *Spectral Resolution

CRMs: Toluene in Hexane

CRMs Serial Number: 14812 **Blank Serial Number: 14803**

Traceability: Traceable to toluene in hexane NIST SRM2034,through Starna certificate report no. 113598

Spectral slit width (nm)	Abs Ratio
0.5	#N/A
1.0	#N/A
1.5	#N/A
2.0	1.401
3.0	#N/A

Note : * "Not TISI Accredited" in this certificate have been included for completeness

Remark:

1. Calibrate Method
   - 1.1 Photometric and Wavelength accuracy: In-house method W-SER-001 based on ASTM E925-02 and ASTM E275-01
   - 1.2 Stray light: Measuring the CRMs in both absorbance and transmittance unit at wavelength 201.23 nm. Base on European Pharmacopoeia V.6.19.3 1984
   - 1.3 Spectral resolution: Measuring the CRMs.The maximum absorbance values were read at closest to 268.7nm and the minimum absorbance values were read at closest 267.0 nm. Refer to European Pharmacopoeia V.6.19.3 1984
2. N/A = not available.
3. Uncertainty of Measurement: The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.
4. This result of calibration was found accurate as shown on date and place of calibration only.
5. This report will certify of calibrated equipment only.

- End of Report -

nfi national food institute ministry of industry
สุขสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการสุขสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2402881-001-01
Client name: SECOT CO., LTD.
Address: 239 Rimklongprapa Road, Bangsue, Bangsue, Bangkok 10800

Equipment: CHAMBER (Hot Air Oven)
Manufacturer: MEMMERT
Model: UF55
Serial No.: B213.0295
ID No.: N/A
Order No.: 2402881
Operation No.: 2402881-001
Date of Receipt: 24 May 2024
Date of Calibration: 24 May 2024

Calibrated by Mr.Pheraphat Tuanjit
Scientist

Approved by
(Miss Preeyaporn Jaengkarnkit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team

Date of Issue: 30 May 2024

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยเฉลิมพระเกียรติ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8688 Fax +66(0) 2422 8545
nfi.or.th

สถาบันอุตสาหกรรมพัฒนาแห่งชาติเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
national food institute ministry of industry
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2402881-001-01

Equipment: CHAMBER (Hot Air Oven)

Model: UF55 Serial No.: B213.0295

Resolution: 0.1 °C ID No.: N/A

Manufacturer: MEMMERT

Date of Calibration: 24 May 2024

Location: Laboratory, SECOT CO., LTD.

Environment Condition: Ambient Temperature (31.0 ± 1) °C

Relative Humidity (68 ± 5) %

Line Voltage (220 ± 3) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY59003377	TE 670223-01	13 January 2025	NATIONAL FOOD INSTITUTE
	RTD	CH#101-109/ RTD#101-109			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good

   UUC Description :

   Time of Record 1 Hour 9 Minute At 80.0, 104.0 and 180.0 °C

   Fresh air Damper [-] Open Position [-]

   [X] Close Fan [60%]

   [-] Not Available
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

P. Jeenghanbit
30 May 2024

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8538 Fax +66(0) 2422 8545

สถาบันอุตสาหกรรมพัฒนาแห่งชาติเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
national food institute ministry of industry
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2402881-001-01

Equipment: CHAMBER (Hot Air Oven)

Model: UF55 Serial No.: B213.0295

Resolution: 0.1 °C ID No.: N/A

Manufacturer: MEMMERT

Date of Calibration: 24 May 2024

Calibration point: 80.0, 104.0 and 180.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	30.7	63.6	217.0
MAX	31.4	73.1	223.0

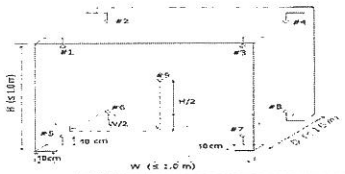


Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF) # 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	Uncertainty ± (°C)
80.0	79.99	79.94	80.08	80.08	80.13	79.95	79.90	80.17	80.13	0.46
104.0	103.86	103.80	104.00	103.99	104.10	103.83	103.81	104.18	104.10	0.53
180.0	179.73	179.73	180.01	180.00	180.44	179.81	180.20	180.56	180.25	0.90

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* reading (°C) MIN	MAX	Average	Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
80.0	80.0	80.0	80.0	0.06	0.23	0.37
104.0	104.0	104.0	104.0	0.10	0.30	0.53
180.0	180.0	180.0	180.0	0.10	0.52	0.98

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

P. Jeenghanbit
30 May 2024

F-CS-012 Revision: 01 Date: 20-04-65

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8538 Fax +66(0) 2422 8545

CAL
Calibratech Co.,Ltd.
7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120
Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-420019-1 **Page : 1 of 2**

Submitted by : Secot Co.,Ltd.
239 RimKlongprapa Road, Bangsue, Bangkok 10800 Thailand

Equipment : pH Meter with electrode
pH meter
Manufacturer : Mettler Toledo Model : Seven2Go S2
Range : N/A pH Resolution : 0.01 pH
Serial No. : B924795409 ID No. : PH No.12
Electrode
Model : InLab Expert Go Serial No. : 3051249

Environment : Ambient Temperature : (25 ± 2) °C
Relative Humidity : (50 ± 15) %

Date of Received : 13 February 2024
Date of Calibration : 20 February 2024
Date of Issue : 20 February 2024
Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
440001	23E1240	24 Mar 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	944535	27 Nov 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	944537	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	944536	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :
(Surachai Promthong)
Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This cerificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL
Calibratech Co.,Ltd.
7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120
Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-420019-1 **Page : 2 of 2**

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement
pH meter
Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading (pH)	UUC Reading (mV)	Correction (mV)	Uncertainty (± mV)
4, 7, 10	177.4800	4	4.00	177	0	0.58
	0.0000	7	7.00	0	0	0.58
	-177.4800	10	10.00	-177	0	0.58

Function : pH meter with electrode
Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	9.997	10.01	-0.01	0.014

Remark
UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.
This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -

CAL-F0031-03

nfi
national food institute
ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2304081-001-01
Client name: SECOT CO., LTD.
Address: 239 Rimklongprapa Road,
Bangsue, Bangsue, Bangkok 10800

Equipment: CHAMBER (Incubator)
Manufacturer: MEMMERT
Model: ICP 400
Serial No.: K406.0004
ID No.: N/A
Order No.: 2304081
Operation No.: 2304081-001
Date of Receipt: 27 July 2023
Date of Calibration: 27 July 2023

Calibrated by Mr.Worapob Sooktong
Scientist

Approved by
(Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 7 August 2023

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8888 Fax +66(0) 2422 8545
nfi.or.th

nfi
national food institute
ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2304081-001-01
Equipment: CHAMBER (Incubator)
Model: ICP 400 Serial No.: K406.0004
Resolution: 0.1 °C ID No.: N/A
Manufacturer: MEMMERT
Date of Calibration: 27 July 2023

Location: Laboratory, SECOT CO., LTD.
Environment Condition:
Ambient Temperature (30 ± 1) °C
Relative Humidity (54 ± 1) %
Line Voltage (228 ± 0) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
   - The temperature scale used was based on ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016894	TE 660380-01	22 April 2024	NATIONAL FOOD INSTITUTE
	RTD	CH#301-309/ RTD#301-309			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
   UUC Description :
   Time of Record 1 Hour 9 Minute At 20.0 °C
   Fresh air Damper [-] Open Position [-]
   [X] Close
   [-] Not Available
7. Result of Calibration : [X] Without adjustment [ ] After adjustment

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่ขัน เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8888 Fax +66(0) 2422 8545
nfi.or.th

nfi
national food institute
ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2304081-001-01

Equipment: CHAMBER (Incubator)

Model: ICP 400 Serial No.: K406.0004

Resolution: 0.1 °C ID No.: N/A

Manufacturer: MEMMERT

Date of Calibration: 27 July 2023

Calibration point: 20.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	28.6	53.0	227.3
MAX	31.4	54.1	228.1




Table1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
20.0	20.42	20.39	20.40	20.43	20.47	20.49	20.42	20.41	20.43	0.27

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
20.0	20.0	20.1	20.0	0.065	0.053	0.220

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8698 Fax: +66(0) 2422 8545
nfi.or.th

nfi
national food institute
ministry of industry
อุตสาหกรรมพัฒนามูลนิธิเพื่อสถาบันอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Certificate

Certificate No.: 2304081-002-01

Client name: SECOT CO., LTD.

Address: 239 Rimklongprapa Road,
Bangsue, Bangsue, Bangkok 10800

Equipment: Water Bath

Manufacturer: MEMMERT

Model: WB 29

Serial No.: I698.0051

ID No.: N/A

Order No.: 2304081

Operation No.: 2304081-002

Date of Receipt: 27 July 2023

Date of Calibration: 27 July 2023

Calibrated by Mr.Worapob Sooktong
Scientist

Approved by
(Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 7 August 2023

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8698 Fax: +66(0) 2422 8545
nfi.or.th

สถาบันอาหาร
national food institute
ministry of industry
สถาบันพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

MAC THAILAND
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2304081-002-01

Equipment: Water Bath

Model: WB 29 Serial No.: I698.0051

Resolution: 0.1 °C ID No.: N/A

Manufacturer: MEMMERT

Date of Calibration: 27 July 2023

Location: Laboratory, SECOT CO., LTD.

Environment Condition:
Ambient Temperature (24 ± 1) °C
Relative Humidity (58 ± 2) %
Line Voltage (229 ± 1) Volt

Condition of this results of Calibration:

1. This instrument was calibrated by insert 5 standard thermometer into its liquid bath and calibration according to W-TE-011 based on ASTM E715-80 (2016): Standard Specification for Gravity-Convection and Forced-Circulation Water Baths.
   - The temperature scale used is ITS - 90.
   - All data show below were final values and the initial data may be obtained upon request.
2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016894	TE 660380-01	22 April 2024	NATIONAL FOOD INSTITUTE
	RTD	RTD#201-205 / CH#201-205			

3. This certificate is traceable to International System of Units (SI Units).
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.
6. Condition of Calibrated item : Good
   UUC Description:
   Time of Record 1 Hour 9 Minute At 95.0 °C
7. Result of Calibration :
   [X] Without adjustment
   [ ] After adjustment

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8588 Fax +66(0) 2422 8545
nfi.or.th

สถาบันอาหาร
national food institute
ministry of industry
สถาบันพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center

ilac-MRA

MAC THAILAND
NSC-TISI-TIS 17025
CALIBRATION 0061

Calibration Report

Certificate No.: 2304081-002-01

Equipment: Water Bath

Model: WB 29 Serial No.: I698.0051

Resolution: 0.1 °C ID No.: N/A


Manufacturer: MEMMERT

Date of Calibration: 27 July 2023

Calibration point: 95.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	23.0	56.3	227.5
Max	25.0	60.2	229.6

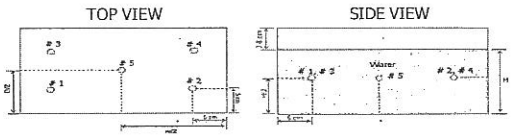

Sensor Installation Location

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.5 is REF)					Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	
95.0	95.03	94.96	95.10	94.97	95.02	0.28

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
95.0	94.9	95.1	95.0	0.18	0.080	0.47

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity)"
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The difference of the maximum and minimum measured temperatures througout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

--------- End ---------

2008 ซอยอรุณอมรินทร์ 36 ถนนอรุณอมรินทร์ แขวงบางยี่เรือ เขตบางพลัด กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel. +66(0) 2422 8588 Fax +66(0) 2422 8545
nfi.or.th

ภาคผนวก จ

หนังสืออนุญาตขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน จากกรมโรงงานอุตสาหกรรม

ที่ อก ๐๓๑๐(๑)/ ๑๑๐๑๖

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๐ กรกฎาคม ๒๕๖๖

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท ซีคอท จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๗ เมษายน ๒๕๖๖

สิ่งที่ส่งมาด้วย ๑. รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๒. รายชื่อเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๑ แผ่น
๓. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๙ แผ่น

ตามหนังสือที่อ้างถึง บริษัท ซีคอท จำกัด ขอต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๓๙ สถานที่ตั้งเลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท ซีคอท จำกัด ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐ ราย ตามสิ่งที่ส่งมาด้วย ๑
ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๘ ราย ตามสิ่งที่ส่งมาด้วย ๒
ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย น้ำใต้ดิน อากาศเสีย สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว และดิน ตามสิ่งที่ส่งมาด้วย ๓

หนังสือฉบับนี้จะหมดอายุในวันที่ ๒ พฤษภาคม ๒๕๖๙ หากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม ทั้งนี้ สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายประสม ดำรงพงษ์)
ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

Green Industry
"อุตสาหกรรมก้าวไกล ประเทศไทยก้าวหน้า ร่วมกันพัฒนา อุตสาหกรรมสีเขียว"

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท ซีคอท จำกัด **เลขทะเบียน ว-๒๓๙**

ที่ อก ๐๓๑๐(๑)/ ๑๑๐๑๖ **ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๖**

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ จำนวน ๑๐ ราย

๑) นายขรรชัย เกรียงไกรอุดม	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๒
๒) นางสมฤดี เกรียงไกรอุดม	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๓
๓) นางอารยา ทิพรักษ์	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๔
๔) นางสาวเขมชุดา อินทร์ศร	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๕
๕) นางสาวปรีดา สมใจ	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๖
๖) นางสาวอรัญญา มาตา	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๗
๗) นางสาวลดาวัลย์ วงศ์เจริญ	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๘
๘) นางสาวมณีวรรณ เกตะวันดี	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๐๙
๙) นางสาวนริสา ภูวสรรเพ็ชญ์	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๑๐
๑๐) นางสาวศิริวรรณ ฉิมสง่า	ทะเบียนเลขที่ ว-๒๓๙-ค-๐๐๑๑

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ซีคอท จำกัด เลขทะเบียน ว-๒๓๙
ที่ อก ๐๓๑๐(๑)/ ๑๑๐๑๖ ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๖

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๓๘ ราย

๑) นางสาวสุดาพร สุนทร ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๐๑
๒) นางสาวสุธาทิพย์ เทียนเตี้ย ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๐๓
๓) นางสาวสุนันทา ศิรวุฒินานนท์ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๐๔
๔) นายบวร ดีชัยยะ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๐๕
๕) นางสาวเกศรินทร์ วรเดชวิทยา ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๐๖
๖) นายอนิวัฒน์ พิมวันนา ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๐๗
๗) นายชิตพล สมประสงค์ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๐๘
๘) นางสาวศศิธร พรหมประเสริฐ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๐๙
๙) นายศิวะนนท์ กุลวงษ์ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๐
๑๐) นางสาวอลิษา คนิวรานนท์ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๑
๑๑) นางสาวสิริวรรณ แก้วชิงดวง ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๒
๑๒) นางสาวปัทมวรรณ สุวรรณวิโรจน์ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๓
๑๓) นางสาวกนิษฐา เจริญเชื้อ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๔
๑๔) นายวัชรกานต์ ประมาคะเต ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๕
๑๕) นายซอง เฮงชวัลกุล ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๖
๑๖) นางสาวกฤษณา จันทุม ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๗
๑๗) นางสาวพรนภา บุตรธรรม ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๘
๑๘) นางสาวธาริณี อาจปลิว ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๙
๑๙) นายธนโชติ ช่างล้อ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๐
๒๐) นางสาวพัชรา สมานฉันท์ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๑
๒๑) นางสาวจุฑารัตน์ แจ่มเรือน ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๒
๒๒) นางสาวจณิสตา กุ้ยอ่อน ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๓
๒๓) นายกิตติพงศ์ ถะเกิงสุข ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๔
๒๔) นายจีรวัฒน์ โคตรคำหาญ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๕
๒๕) นายชนะพล อัครผล ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๖
๒๖) นางสาวทิพย์สุดา วรรณการ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๗
๒๗) นายสิทธิชัย สว่างวงศ์ไชย ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๘
๒๘) นายพิษณุ สีนามเพ็ง ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๒๙
๒๙) นายรัตนชัย ชอบทำกิจ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๐
๓๐) นายธนาวุฒิ ด่วนแสง ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๑
๓๑) นายณัฐชัย ไชยโคตร ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๒
๓๒) นายณัฐดนัย กฤษณะโลม ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๓
๓๓) นายศุภชัย สุขใหม่ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๔
๓๔) นายรอมฎอน เหล็มหมาด ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๕
๓๕) นางสาวสุภาวดี บัวแก้ว ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๖
๓๖) นางสาวมารียาณี ฮาแว ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๗
๓๗) นางสาววิระยา ปัจฉิมบูรณ์ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๘
๓๘) นางสาวศลิษา อินรีย์ ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๙

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท ซีคอท จำกัด เลขทะเบียน ว-๒๓๙
ที่ อก ๐๓๑๐(๑)/ ๑๑๐๑๖ ลงวันที่ ๒๐ กรกฎาคม ๒๕๖๖

ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๕๕ รายการ

น้ำเสีย จำนวน 45 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
2	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
3	Barium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
4	α-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
5	β-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
6	δ-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
7	γ-BHC	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method[4] 2) 5-Day BOD Test, Membrane Electrode Method[4]
9	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
10	Chemical Oxygen Demand	1) Open Reflux, Titrimetric method[4] 2) Closed Reflux, Colorimetric method[4] 3) Closed Reflux, Titrimetric Method[4]
11	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
12	Chromium	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
13	Color	ADMI Weighted-Ordinate Spectrophotometric Method[4]
14	Copper	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Method[4]
15	Cyanide	Distillation, Colorimetric method[4]
16	4,4′-DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

17 4,4′-DDE...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	4,4′-DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
18	4,4′-DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
19	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
20	Endosulfan I	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
21	Endosulfan II	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
22	Endosulfan Sulfate	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
23	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
24	Endrin Aldehyde	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

25 Formaldehyde...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
25	Formaldehyde	Distillation, Colorimetric Method[3]
26	Free Chlorine	1) Iodometric Method[4]
		2) DPD Colorimetric Method[4]
27	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
28	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
29	Hexavalent Chromium	1) Colorimetric Method[4]
		2) Extraction, Air-Acetylene Flame Method[4]
30	Lead	1) Digestion, Direct Air-Acetylene Flame Method[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4]
		3) Digestion, Inductively Coupled Plasma Method[4]
31	Manganese	1) Digestion, Direct Air-Acetylene Flame Method[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4]
		3) Digestion, Inductively Coupled Plasma Method[4]
32	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4]
33	Methoxychlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
34	Nickel	1) Digestion, Direct Air-Acetylene Flame Method[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4]

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		3) Digestion, Inductively Coupled Plasma Method[4]
35	Oil & Grease	1) Liquid-Liquid, Partition-Gravimetric Method[4]
		2) Soxhlet Extraction Method[4]
36	pH	Electrometric Method[4]
37	Phenols	1) Distillation, Chloroform Extraction Method[4]
		2) Distillation, Direct Photometric Method[4]
38	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4]
		2) Digestion, Inductively Coupled Plasma Method[4]
39	Sulfide	1) Iodometric method[4]
		2) Methylene blue method[4]
40	Temperature	Laboratory and Field Methods[4]
41	Total Dissolved Solids	Dried at 180 °C[4]
42	Total Kjeldahl Nitrogen	1) Macro Kjeldahl Method[4]
		2) Semi-Micro Kjeldahl Method[4]
43	Total Suspended Solids	Dried at 103-105 °C[4]
44	Trivalent Chromium	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method; Colorimetric Method; Calculation[4]
		3) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[4]
45	Zinc	1) Digestion, Direct Air-Acetylene Flame Method[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4]
		3) Digestion, Inductively Coupled Plasma Method[4]

น้ำใต้ดิน...

น้ำใต้ดิน จำนวน 125 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
2	Acetone	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
3	Aldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4] 2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
4	Anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
5	Antimony	Digestion, Inductively Coupled Plasma Spectrometric Method[4]
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
7	Atrazine	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
8	Barium	1) Digestion, Direct Nitrous Oxide-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Spectrometric Method[4]
9	Benz(a)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
10	Benzene	Purge and Trap Gas Chromatographic/Mass spectrometric Method[4]
11	Benzo(b)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
12	Benzo(k)fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

13 Benzoic acid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	Benzoic acid	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
14	Benzo(a)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
15	Benzo(g,h,i)perylene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
16	Beryllium	Digestion, Inductively Coupled Plasma Spectrometric Method[4]
17	Bis(2-chloroethyl)ether	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
18	Bis(2-ethylhexyl)phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
19	Bromodichloromethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
20	Bromoform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
21	Butanol	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
22	Butyl benzyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
23	Cadmium	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Spectrometric Method[4]
24	Carbazole	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
25	Carbon disulfide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
26	Carbon tetrachloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]

27 Chlordane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
27	Chlordane	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
28	p-Chloroaniline	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
29	Chlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
30	Chlorodibromomethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
31	Chloroform	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
32	2-Chlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
33	Chromium	1) Digestion, Direct Air-Acetylene Flame Method[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4]
		3) Digestion, Inductively Coupled Plasma Spectrometric Method[4]
34	Chromium (III)	1) Digestion, Direct Air-Acetylene Flame Method; Colorimetric Method; Calculation[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method; Colorimetric Method; Calculation[4]
		3) Digestion, Inductively Coupled Plasma Spectrometric Method; Colorimetric Method; Calculation[4]
35	Chromium (VI)	1) Colorimetric Method[4]
		2) Extraction, Air-Acetylene Flame Method[4]
36	Chrysene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]

37 Cyanide...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
37	Cyanide	1) Distillation, Titrimetric Method[4]
		2) Distillation, Colorimetric Method[4]
38	2,4-D	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
39	DDD	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
40	DDE	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
41	DDT	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
42	Dibenz(a,h)anthracene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
43	Di-n-butyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
44	1,2-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
45	1,3-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
46	1,4-Dichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
47	3,3′-Dichlorobenzidine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
48	1,1-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
49	1,2-Dichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]

50 1,1-Dichloroethylene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
50	1,1-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
51	cis-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
52	trans-1,2-Dichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
53	2,4-Dichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
54	1,2-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
55	1,3-Dichloropropane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
56	1,3-Dichloropropene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
57	Dieldrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
58	Diethyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
59	2,4-Dimethylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
60	2,4-Dinitrophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
61	2,4-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
62	2,6-Dinitrotoluene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
63	Di-n-Octyl phthalate	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
64	Endosulfan	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]

2) Liquid-Liquid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
65	Endrin	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
66	Ethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
67	Fluoranthene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
68	Fluorene	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
69	Heptachlor	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
70	Heptachlor epoxide	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
71	Hexachlorobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
72	Hexachloro-1,3-butadiene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
73	n-Hexane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
74	α-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
75	β-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]

2) Liquid-Liquid...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
76	γ-HCH	1) Liquid-Liquid Extraction, Gas Chromatographic Method[4]
		2) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
77	Hexachlorocyclopentadiene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
78	Hexachloroethane	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
79	Indeno(1,2,3-cd)pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
80	Isophorone	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
81	Lead	1) Digestion, Direct Air-Acetylene Flame Method[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4]
		3) Digestion, Inductively Coupled Plasma Spectrometric Method[4]
82	Manganease	1) Digestion, Direct Air-Acetylene Flame Method[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4]
		3) Digestion, Inductively Coupled Plasma Spectrometric Method [4]
83	Mercury	Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[4]
84	Methanol	Purge and Trap Gas Chromatographic/ Mass spectrometric Method[4]
85	Methoxychlor	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
86	Methyl bromide	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]

87 Methylene chloride...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
87	Methylene chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
88	2-Methylphenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
89	2-Methylnaphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
90	Methyl tert-butyl ether	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
91	Naphthalene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
92	Nickel	1) Digestion, Direct Air-Acetylene Flame Method[4]
		2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4]
		3) Digestion, Inductively Coupled Plasma Spectrometric Method[4]
93	Nitrobenzene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
94	N-Nitrosodiphenylamine	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
95	N-Nitrosodi-n-propylamine	Liquid-Liquid Extraction, Gas Chromatographic/Mass Spectrometric Method[4]
96	Polychlorinated Biphenyls	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
	- PCB-1016	
	- PCB-1221	
	- PCB-1232	
	- PCB-1242	
	- PCB-1248	
	- PCB-1254	
	- PCB-1260	
97	Pentachlorophenol	Liquid-Liquid Extraction, Gas Chromatographic Method[4]
98	pH	Electrometric method[4]

99 Phenanthrene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
99	Phenanthrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
100	Phenol	1) Distillation, Chloroform Extraction Method[4] 2) Distillation, Direct Photometric Method[4] 3) Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
101	Pyrene	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
102	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
103	Silver	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Inductively Coupled Plasma Method[4]
104	Styrene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
105	1,1,2,2-Tetrachloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
106	Tetrachloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
107	Toluene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
108	TPH (C_5-C_8)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[12,25]
109	TPH ($C_{>8}$-C_{16})	1) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,21] 2) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass spectrometric Method[9,25]
110	TPH ($C_{>16}$-C_{35})	1) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[9,21]

2) Separatory...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/Mass spectrometric Method[9,25]
111	1,2,4-Trichlorobenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
112	1,1,1-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
113	1,1,2-Trichloroethane	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
114	Trichloroethylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
115	2,4,5-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
116	2,4,6-Trichlorophenol	Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[4]
117	1,3,5-Trimethylbenzene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
118	Vanadium	Digestion, Inductively Coupled Plasma Spectrometric Method[4]
119	Vinyl acetate	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
120	Vinyl chloride	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
121	m-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
122	o-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
123	p-Xylene	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]
124	Xylene (Total)	Purge and Trap Gas Chromatographic/Mass Spectrometric Method[4]

125 Zinc ...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
125	Zinc	1) Digestion, Direct Air-Acetylene Flame Method[4] 2) Digestion, Electrothermal Atomic Absorption Spectrometric Method[4] 3) Digestion, Inductively Coupled Plasma Spectrometric Method[4]

<u>อากาศเสีย (ปล่องระบาย) จำนวน 27 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Antimony	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
2	Arsenic	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
3	Beryllium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
4	Cadmium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
5	Carbon monoxide	Instrumental Analyzer Method[5]
6	Chlorine	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method[5]
7	Chromium	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
8	Cobalt	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
9	Copper	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
10	Cresol	Adsorption Sampling, Gas Chromatographic Method[5]
11	Dioxin/Furans	Isokinetic Sampling[5]
12	Hydrogen chloride	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method[5]
13	Hydrogen Fluoride	1) Absorption Sampling, Ion Chromatographic Method[5] 2) Isokinetic Sampling, Ion Chromatographic Method[5]
14	Hydrogen Sulfide	Absorption Sampling, Iodometric Method[5]
15	Lead	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
16	Manganese	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
17	Mercury	Isokinetic Sampling, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[5]
18	Nickel	1) Isokinetic Sampling, Digestion, Direct Air-Acetylene Flame Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
19	Opacity	Ringelmann's Method[2]
20	Oxides of Nitrogen	1) Absorption Sampling, Phenoldisulfonic acid Method[5] 2) Absorption Sampling, Ion Chromatographic Method[5] 3) Instrumental Analyzer Method[5]
21	Selenium	1) Isokinetic Sampling, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[5] 2) Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
22	Sulfur dioxide	1) Isokinetic Sampling, Barium-Thorin Titrimetric Method[5] 2) Absorption Sampling, Barium-Thorin Titrimetric Method[5] 3) Instrumental Analyzer Method[5]
23	Sulfuric acid	Isokinetic Sampling, Barium-Thorin Titrimetric Method[5]
24	Tin	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
25	Total Suspended Particulate	1) Isokinetic Sampling, Gravimetric Method[5] 2) Paired Train, Isokinetic Sampling, Gravimetric Method[5]
26	Vanadium	Isokinetic Sampling, Digestion, Inductively Coupled Plasma Method[5]
27	Xylene	1) Adsorption Sampling, Gas Chromatographic Method[5] 2) Adsorption Sampling, Gas Chromatographic/ Mass Spectrometric Method[5]

สิ่งปฏิกูล...

<u>สิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว จำนวน 34 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,6,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,6,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
2	Antimony	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,16] 4) Digestion, Inductively Coupled Plasma Method[7,14]
3	Arsenic	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[1,6,16] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14] 3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,16] 4) Digestion, Inductively Coupled Plasma Method[7,14]
4	Barium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,15]

2) Waste Extraction...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]
		3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15]
		4) Digestion, Inductively Coupled Plasma Method[7,14]
5	Beryllium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]
		2) Digestion, Inductively Coupled Plasma Method[7,14]
6	Cadmium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,15]
		2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]
		3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15]
		4) Digestion, Inductively Coupled Plasma Method[7,14]
7	Chlordane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22]
		2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,9,27]
		3) Soxhlet Extraction, Gas Chromatographic Method[10,22]
		4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
8	Chromium	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,15]
		2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15]
		4) Digestion, Inductively Coupled Plasma Method[7,14]
9	Chromium (III)	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method; Waste Extraction, Colorimetric Method; Calculation[1,6,15,17]
		2) Waste Extraction, Digestion, Inductively Coupled Plasma Method; Waste Extraction, Colorimetric Method; Calculation[1,6,14,17]
		3) Digestion, Flame Atomic Absorption Spectrometric Method; Alkaline Digestion, Colorimetric Method; Calculation[7,8,15,17]
		4) Digestion, Inductively Coupled Plasma Method; Alkaline Digestion, Colorimetric Method; Calculation[7,8,14,17]
10	Chromium (VI)	1) Waste Extraction, Colorimetric Method[1,17]
		2) Alkaline Digestion, Colorimetric Method[8,17]
11	Cobalt	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]
		2) Digestion, Inductively Coupled Plasma Method[7,14]
12	Copper	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,15]
		2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]
		3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15]
		4) Digestion, Inductively Coupled Plasma Method[7,14]

13 2,4-D...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
13	2,4-D	1) Waste Extraction, Gas Chromatographic/Mass Spectrometric Method[1,25] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[25]
14	DDD	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
15	DDE	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
16	DDT	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]

17 Dieldrin...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
17	Dieldrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
18	Endrin	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
19	Heptachlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22] 2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,9,27] 3) Soxhlet Extraction, Gas Chromatographic Method[10,22] 4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
20	Lead	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]

3) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15]
		4) Digestion, Inductively Coupled Plasma Method[7,14]
21	Lindane	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22]
		2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,9,27]
		3) Soxhlet Extraction, Gas Chromatographic Method[10,22]
		4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
22	Mercury	1) Waste Extraction, Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[1,18]
		2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]
		3) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[19]
		4) Digestion, Inductively Coupled Plasma Method[7,14]
23	Methoxychlor	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,22]
		2) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,9,27]
		3) Soxhlet Extraction, Gas Chromatographic Method[10,22]
		4) Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]

24 Molybdenum...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
24	Molybdenum	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]
		2) Digestion, Inductively Coupled Plasma Method[7,14]
25	Nickel	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,15]
		2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]
		3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15]
		4) Digestion, Inductively Coupled Plasma Method[7,14]
26	Polychlorinated Biphenyls	1) Waste Extraction, Separatory Funnel Liquid-Liquid Extraction, Gas Chromatographic Method[1,9,23]
	- Aroclor 1016	
	- Aroclor 1221	
	- Aroclor 1232	2) Soxhlet Extraction, Gas Chromatographic Method[10,23]
	- Aroclor 1242	
	- Aroclor 1248	
	- Aroclor 1254	
	- Aroclor 1260	
27	Pentachlorophenol	1) Waste Extraction, Gas Chromatographic/ Mass Spectrometric Method[1,25]
		2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[25]
28	pH	Electrometric Method[31,32]
29	Selenium	1) Waste Extraction, Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[1,6,20]
		2) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14]
		3) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,20]

4) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		4) Digestion, Inductively Coupled Plasma Method[7,14]
30	Silver	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
31	Thallium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
32	Trichloroethylene	1) Waste Extraction, Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[1,12,26] 2) Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[12,26]
33	Vanadium	1) Waste Extraction, Digestion, Inductively Coupled Plasma Method[1,6,14] 2) Digestion, Inductively Coupled Plasma Method[7,14]
34	Zinc	1) Waste Extraction, Digestion, Flame Atomic Absorption Spectrometric Method[1,6,15] 2) Waste Extraction, Digestion, Inductively Coupled Plasma Method [1,6,14] 3) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 4) Digestion, Inductively Coupled Plasma Method [7,14]

<u>ดิน จำนวน 124 รายการ</u>

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Acenaphthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]

2 Acetone...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
2	Acetone	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
3	Aldrin	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
4	Anthracene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
5	Antimony	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,16] 2) Digestion, Inductively Coupled Plasma Method[7,14]
6	Arsenic	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,16] 2) Digestion, Inductively Coupled Plasma Method[7,14]
7	Atrazine	Ultrasonic Extraction, Gas Chromatographic Method[11,24]
8	Barium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
9	Benz(a)anthracene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
10	Benzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
11	Benzo(b)fluoranthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
12	Benzo(k)fluoranthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
13	Benzoic acid	Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]

14 Benzo(a)pyrene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
14	Benzo(a)pyrene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
15	Benzo(g,h,i)perylene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
16	Beryllium	Digestion, Inductively Coupled Plasma Method[7,14]
17	Bis(2-chloroethyl)ether	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
18	Bis(2-ethylhexyl)phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
19	Bromodichloromethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
20	Bromoform	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
21	Butanol	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
22	Butyl benzyl phthalate	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
23	Cadmium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
24	Carbazole	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
25	Carbon disulfide	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
26	Carbon tetrachloride	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
27	Chlordane	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
28	p-Chloroaniline	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
29	Chlorobenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
30	Chlorodibromomethane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
31	Chloroform	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
32	2-Chlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[11,27]
33	Chromium	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
34	Chromium (III)	1) Digestion, Flame Atomic Absorption Spectrometric Method; Colorimetric Method; Calculation[7,8,15,17] 2) Digestion, Inductively Coupled Plasma Method; Colorimetric Method; Calculation[7,8,14,17]
35	Chromium (VI)	Alkaline Digestion, Colorimetric Method[8,17]
36	Chrysene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
37	Cyanide	1) Extraction, Distillation, Titrimetric Method[28,29,30] 2) Extraction, Distillation, Colorimetric Method[28,29,30]
38	2,4-D	Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[24]
39	DDD	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
40	DDE	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
41	DDT	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
42	Dibenz(a,h)anthracene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
43	Di-n-butyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
44	1,2-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
45	1,3-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
46	1,4-Dichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
47	3,3′-Dichlorobenzidine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
48	1,1-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
49	1,2-Dichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
50	1,1-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
51	cis-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
52	trans-1,2-Dichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
53	2,4-Dichlorophenol	Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]

54 1,2-Dichloropropane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
54	1,2-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
55	1,3-Dichloropropane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
56	1,3-Dichloropropene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
57	Dieldrin	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
58	Diethyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
59	2,4-Dimethylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[11,27]
60	2,4-Dinitrophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[11,27]
61	2,4-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
62	2,6-Dinitrotoluene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
63	Di-n-Octyl phthalate	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
64	Endosulfan	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
65	Endrin	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
66	Ethylbenzene	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]

67 Fluoranthene...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
67	Fluoranthene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
68	Fluorene	Soxhlet Extraction, Gas Chromatographic/ Mass Spectrometric Method[10,27]
69	Heptachlor	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
70	Heptachlor epoxide	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
71	Hexachlorobenzene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[11,27]
72	Hexachloro-1,3-butadiene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
73	n-Hexane	Purge and Trap, Gas Chromatographic/ Mass Spectrometric Method[13,26]
74	α-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
75	β-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
76	γ-HCH	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
77	Hexachlorocyclopentadiene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]

78 Hexachloroethane...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
78	Hexachloroethane	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
79	Indeno(1,2,3-cd)pyrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
80	Isophorone	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
81	Lead	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
82	Manganease	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
83	Mercury	1) Digestion, Cold-Vapor Atomic Absorption Spectrometric Method[19] 2) Digestion, Inductively Coupled Plasma Method[7,14]
84	Methanol	Ultrasonic Extraction, Direct Aqueous Injection, Gas Chromatographic Method[11,21]
85	Methoxychlor	1) Ultrasonic Extraction, Gas Chromatographic Method[11,22] 2) Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
86	Methyl bromide	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
87	Methylene chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
88	2-Methylphenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[11,27]
89	2-Methylnaphthalene	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[11,27]

90 Methyl tert-butyl ether...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
90	Methyl tert-butyl ether	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
91	Naphthalene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
92	Nickel	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
93	Nitrobenzene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
94	N-Nitrosodiphenylamine	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
95	N-Nitrosodi-n-propylamine	Soxhlet Extration, Gas Chromatographic/Mass Spectrometric Method[10,27]
96	Polychlorinated Biphenyls - Aroclor 1016 - Aroclor 1221 - Aroclor 1232 - Aroclor 1242 - Aroclor 1248 - Aroclor 1254 - Aroclor 1260	Soxhlet Extraction, Gas Chromatographic Method[10,23]
97	Pentachlorophenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[24]
98	Phenanthrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
99	Phenol	Ultrasonic Extraction, Gas Chromatographic/Mass Spectrometric Method[11,27]
100	Pyrene	Soxhlet Extraction, Gas Chromatographic/Mass Spectrometric Method[10,27]
101	Selenium	1) Digestion, Hydride Generation/Atomic Absorption Spectrometric Method[7,20]

2) Digestion...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
		2) Digestion, Inductively Coupled Plasma Method[7,14]
102	Silver	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]
103	Styrene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
104	1,1,2,2-Tetrachloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
105	Tetrachloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
106	Toluene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
107	TPH (C_5-C_8)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
108	TPH ($C_{>8}$-C_{16})	1) Soxhlet Extraction, Gas Chromatographic Method[10,21] 2) Soxhlet Extraction, Gas Chromatographic/ Mass spectrometric Method[10,26]
109	TPH ($C_{>16}$-C_{35})	1) Soxhlet Extraction, Gas Chromatographic Method[10,21] 2) Soxhlet Extraction, Gas Chromatographic/ Mass spectrometric Method[10,26]
110	1,2,4-Trichlorobenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
111	1,1,1-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
112	1,1,2-Trichloroethane	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
113	Trichloroethylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]

114 2,4,5-Trichlorophenol...

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
114	2,4,5-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
115	2,4,6-Trichlorophenol	Ultrasonic Extraction, Gas Chromatographic/ Mass Spectrometric Method[11,27]
116	1,3,5-Trimethylbenzene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
117	Vanadium	Digestion, Inductively Coupled Plasma Method[7,14]
118	Vinyl acetate	Purge and Trap, Gas Chromatographic/Mass spectrometric Method[13,26]
119	Vinyl chloride	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
120	m-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
121	o-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
122	p-Xylene	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
123	Xylene (Total)	Purge and Trap, Gas Chromatographic/Mass Spectrometric Method[13,26]
124	Zinc	1) Digestion, Flame Atomic Absorption Spectrometric Method[7,15] 2) Digestion, Inductively Coupled Plasma Method[7,14]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2548. เรื่อง การกำจัดสิ่งปฏิกูลหรือวัสดุที่ไม่ใช้แล้ว.**ราชกิจจานุเบกษา.** 25 มกราคม 2549. เล่มที่ 123 ตอนพิเศษ 11ง.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้แกลบเป็นเชื้อเพลิง. **ราชกิจจานุเบกษา.** 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.

3. สมาคมวิศวกรรมสิ่งแวดล้อมแห่งประเทศไทย. **คู่มือวิเคราะห์น้ำเสีย.** พิมพ์ครั้งที่ 4. กรุงเทพฯ: เรือนแก้วการพิมพ์, 2547.

4. APHA...

4. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater.** 23rd ed. Washington, DC: APHA, 2017.

5. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources.** 40 CFR 60. Appendix A, 2023.

6. United States Environmental Protection Agency. **Test Methods for Evaluation Solid Waste Physical/Chemical Methods. SW-846,** 2020.

7. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Acid Digestion of Sediments, Sludges, and Soils. SW-846 Method 3050B,** 1996.

8. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Alkaline Digestion for Hexavalent Chromium. SW-846 Method 3060A,** 1996.

9. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Separatory Funnel Liquid-Liquid Extraction. SW-846 Method 3510C,** 1996.

10. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Soxhlet Extraction. SW-846 Method 3540C,** 1996.

11. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Ultrasonic Extraction. SW-846 Method 3550C,** 2007.

12. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Purge-and-Trap for Aqueous Samples. SW-846 Method 5030C,** 2003.

13. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Closed-System Purge-and-Trap and Extraction for Volatile Organics in Soil and Waste Samples. SW-846 Method 5035,** 1996.

14. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Inductively Coupled Plasma-optical Emission Spectrometry. SW-846 Method 6010D,** 2018.

15. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Flame Atomic Absorption Spectrophotometry. SW-846 Method 7000B,** 2007.

16. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Antimony and Arsenic (Atomic Absorption, Borohydride Reduction). SW-846 Method 7062,** 1994.

17. United States...

17. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chromium, Hexavalent (Colorimetric), SW-846 Method 7196A**, 1992.

18. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Liquid Waste (Manual Cold-Vapor Technique, SW-846 Method 7470A**, 1994.

19. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Mercury in Solid or Semisolid Waste (Manual Cold-Vapor Technique, SW-846 Method 7471B**, 2007.

20. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Selenium (Atomic Absorption, Borohydride Reduction), SW-846 Method 7742**, 1994.

21. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Nonhalogenated Organics Using GC/FID. SW-846 Method 8015D**, 2003.

22. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organochlorine Pesticide by Gas Chromatography. SW-846 Method 8081B**, 2007.

23. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Polychlorinated Biphenyls (PCBs) By Gas Chromatography. SW-846 Method 8082A**, 2007.

24. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Organophosphorus Compounds by Gas Chromotography. SW-846 Method 8141B**, 2007.

25. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Chlorinated Herbicides By GC Using Methylation or Pentafluorobenzylation Derivatization. SW-846 Method 8151A**, 1996.

26. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Volatile Organic Compounds by Gas Chromatography/ Mass Spectrometry (GC/MS). SW-846 Method 8260D**, 2018.

27. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **SemiVolatile Organic Compounds by Gas Chromatography/Mass Spectrometry. SW-846 Method 8270E**, 2018.

28. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Total and Amenable Cyanide: Distillation. SW-846 Method 9010C**, 2004.

29. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide Extraction Procedure for Solids and Oils. SW-846 Method 9013A**, 2014.

30. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Cyanide in Waters and Extracts Using Titrimetric and Manual Spectrophotometric. SW-846 Method 9014**, 2014.

31. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **pH Electrometric Measurement. SW-846 Method 9040C**, 2004.

32. United States Environmental Protection Agency. Test Methods for Evaluation Solid Waste Physical/Chemical Methods. **Solid and Waste pH. SW-846 Method 9045D**, 2004.



ที่ อก ๐๓๑๐(๑)/ ๕๐๕๔

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๔๐๐

๒๗ พฤษภาคม ๒๕๖๗

เรื่อง เปลี่ยนแปลงบุคลากรของห้องปฏิบัติการวิเคราะห์

เรียน กรรมการผู้จัดการ บริษัท ซีคอท จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน ลงวันที่ ๒๑ พฤษภาคม ๒๕๖๗

ตามคำขอที่อ้างถึง บริษัท ซีคอท จำกัด ห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๓๙ สถานที่ตั้งเลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร ขอเปลี่ยนแปลงบุคลากร ความละเอียดแจ้งแล้ว นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้ยกเลิกเจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์ จำนวน ๒ ราย ได้แก่

๑) นายวัชรกานต์ ประมาคะเต	ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๑๕
๒) นายรัตนชัย ชอบทำกิจ	ทะเบียนเลขที่ ว-๒๓๙-จ-๐๐๓๐

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ

(นายพรยศ กลั่นกรอง)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน
กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ
โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕
โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙
ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th

ภาคผนวก ฉ

ใบรับรองความสามารถห้องปฏิบัติการและขอบข่ายการรับรองห้องปฏิบัติการทดสอบ ตามมาตรฐาน ISO/IEC 17025 จากสำนักงานมาตรฐานอุตสาหกรรม (สมอ.)

แบบ กมช./สมอ.๒
Form NSC/TISI 2

ใบรับรองเลขที่ 24-LB0026
(Certificate No.)

ใบรับรองระบบงาน
(Certificate of Accreditation)

อาศัยอำนาจตามความในพระราชบัญญัติการมาตรฐานแห่งชาติ พ.ศ. ๒๕๕๑
(By Virtue of National Standardization Act B.E. 2551 (2008))

เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม
(Secretary-General, Thai Industrial Standards Institute)

ออกใบรับรองฉบับนี้ให้
(Issues this certificate to)

บริษัท ซีคอท จำกัด ฝ่ายห้องปฏิบัติการทดสอบด้านสิ่งแวดล้อม
(Secot Company Limited, Environmental Laboratory Division)

ตั้งอยู่เลขที่
(Address)

๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร
(239 Rimklongprapa Road, Bangsue, Bangsue, Bangkok)

ได้รับการรับรองความสามารถ
(Certificate of competence)

ตามมาตรฐานเลขที่ มอก. ๑๗๐๒๕ - ๒๕๖๑
(Standard No. TIS 17025-2561 (2018) (IS0/IEC 17025: 2017))

ข้อกำหนดทั่วไปว่าด้วยความสามารถของ ห้องปฏิบัติการทดสอบและห้องปฏิบัติการสอบเทียบ
(General requirements for the competence of testing and calibration laboratories)

หมายเลขการรับรองที่ ทดสอบ ๐๓๙๔
(Accreditation No. Testing 0394)

โดยมีรายละเอียดสาขาและขอบข่ายที่ได้ใบรับรอง แสดงไว้ใน QR CODE และ www.tisi.go.th
(Details of the scheme and scope of the certificate are shown in QR CODE and www.tisi.go.th)

ออกให้ ณ วันที่ ๖ ธันวาคม พ.ศ. ๒๕๖๖
(Issue date : 6 December B.E. 2566 (2023))

(นายวีระศักดิ์ เพ็งหล้ง)
ผู้อำนวยการสำนักงานคณะกรรมการการมาตรฐานแห่งชาติ
ปฏิบัติราชการแทน
เลขาธิการสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

Signed by สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม (สมอ.)
Thai Industrial Standards Institute (TISI)
Date: 2023-12-06T08:49:04.476+07:00
d68cbe6b

กระทรวงอุตสาหกรรม สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม
(Ministry of Industry Thailand, Thai Industrial Standards Institute)

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)

ชื่อห้องปฏิบัติการ (Laboratory Name): บริษัท ซีคอท จำกัด ฝ่ายห้องปฏิบัติการทดสอบด้านสิ่งแวดล้อม (Secot Company Limited, Environmental Laboratory Division)

หมายเลขการรับรองที่ (Accreditation No.): ทดสอบ 0394 (Testing 0394)

ฉบับที่ 02 (Issue No.02)

ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023))

ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ (Laboratory status): ☑ ถาวร (Permanent) ☐นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสิ่งแวดล้อม (environmental field) 1. น้ำและน้ำเสีย (water and wastewater)	- โลหะหนัก (heavy metals) • สารหนู (Arsenic, As) 0.000 5 mg/L ถึง 0.090 0 mg/L	- Standard Methods for the Examination of Water and Wastewater, APHA , AWWA, WEF, 23rd edition , 2017, Part 3030 F and Part 3114 C
	• สารหนู (Arsenic, As) 0.05 mg/L ถึง 4.50 mg/L • แบเรียม (Barium, Ba) 0.02 mg/L ถึง 4.50 mg/L • แคดเมียม (Cadmium, Cd) 0.01 mg/L ถึง 4.50 mg/L • โครเมียม (Chromium, Cr) 0.01 mg/L ถึง 4.50 mg/L	- Standard Methods for the Examination of Water and Wastewater, APHA , AWWA, WEF, 23rd edition , 2017, Part 3030 E and Part 3120 B

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)

ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ (Laboratory status) ☑ ถาวร (Permanent) ☐นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสิ่งแวดล้อม (environmental field) 1. น้ำและน้ำเสีย (ต่อ) (water and wastewater) (cont.)	- โลหะหนัก (heavy metals) • ทองแดง (Copper, Cu) 0.02 mg/L ถึง 4.50 mg/L • เหล็ก (Iron, Fe) 0.05 mg/L ถึง 9.00 mg/L • ตะกั่ว (Lead, Pb) 0.03 mg/L ถึง 4.50 mg/L • แมงกานีส (Manganese, Mn) 0.01 mg/L ถึง 9.00 mg/L • นิกเกิล (Nickel, Ni) 0.01 mg/L ถึง 4.50 mg/L • สังกะสี (Zinc, Zn) 0.02 mg/L ถึง 9.00 mg/L	- Standard Methods for the Examination of Water and Wastewater, APHA , AWWA, WEF, 23rd edition , 2017, Part 3030 E and Part 3120 B

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)

ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ (Laboratory status) ☑ ถาวร (Permanent) ☐นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสิ่งแวดล้อม (environmental field) 1. น้ำและน้ำเสีย (ต่อ) (water and wastewater) (cont.)	- ซีโอดี (Chemical oxygen demand, COD) 100 mg/L ถึง 4 000 mg/L	- Standard Methods for the Examination of Water and Wastewater, APHA, AWWA, WEF,23rd edition , 2017, Part 5220 D
2. บริเวณทำงาน (workplace)	- ฝุ่นละอองรวม (Total dust) 0.10 mg/filter ถึง 2.00 mg/filter	- NIOSH Manual of Analytical Methods (NMAM) , method 0500, 4th edition , 15th August 1994 (Exclude Sampling)
	- ฝุ่นละอองขนาดเล็ก (Respirable dust) 0.10 mg/filter ถึง 2.00 mg/filter	- NIOSH Manual of Analytical Methods (NMAM) , method 0600, 4th edition , 15th January 1998 (Exclude Sampling)

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)

ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ (Laboratory status) ☑ ถาวร (Permanent) ☐นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสิ่งแวดล้อม (environmental field)		
2. บริเวณทำงาน (ต่อ) (workplace) (cont.)	- เบนซีน (Benzene) 1.10 µg/tube ถึง 420 µg/tube - โทลูอีน (Toluene) 1.10 µg/tube ถึง 420 µg/tube - โทโทรไซลีน (Total xylenes) 2.20 µg/tube ถึง 840 µg/tube - เมตา, พารา-ไซลีน (m, p- Xylene) 1.10 µg/tube ถึง 420 µg/tube - ออร์โธ-ไซลีน (o- Xylene) 1.10 µg/tube ถึง 420 µg/tube	- NIOSH Manual of Analytical Methods (NMAM) , method 1501, 4th edition , 15th March 2003 (Exclude Sampling)
3. ปล่องระบายอากาศ (stack)	- ซัลเฟอร์ไดออกไซด์ (Sulfur dioxide) 1.00 mg/L ถึง 16 000 mg/L (solution)	- US.EPA , Code of Federal Regulations , 40 CFR 60 appendix A , method 6 , July 2019 (Exclude Sampling)

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)

ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ (Laboratory status) ☑ ถาวร (Permanent) ☐นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสิ่งแวดล้อม (environmental field)		
3. ปล่องระบายอากาศ (ต่อ) (stack) (cont.)	- ไฮโดรเจนฟลูออไรด์ (Hydrogen fluoride) 5 µg/sample ถึง 400 µg/sample - ไฮโดรเจนคลอไรด์ (Hydrogen chloride) 5 µg/sample ถึง 400 µg/sample	- WI-7.2-1-22 based on US.EPA , Code of Federal Regulations , 40 CFR 60 appendix A, method 26 , 2019 (Exclude Sampling)

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)

ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ (Laboratory status) ☑ ถาวร (Permanent) ☑นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสิ่งแวดล้อม (environmental field) 4. บรรยากาศทั่วไป (ambient air)	- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs) • คลอโรอีทีน (Chloroethene) 0.05 $\mu g/m^3$ ถึง 51.00 $\mu g/m^3$ (0.02 ppbv ถึง 20.00 ppbv) • 1,3-บิวทาไดอีน (1,3-butadiene) 0.04 $\mu g/m^3$ ถึง 44.00 $\mu g/m^3$ (0.02 ppbv ถึง 20.00 ppbv) • โบรโมมีเทน (Bromomethane) 0.08 $\mu g/m^3$ ถึง 77.00 $\mu g/m^3$ (0.02 ppbv ถึง 20.00 ppbv) • อะคลอลีน (Acrolein) 0.05 $\mu g/m^3$ ถึง 45.00 $\mu g/m^3$ (0.02 ppbv ถึง 20.00 ppbv)	- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)

ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ (Laboratory status) ☑ ถาวร (Permanent) ☑นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสิ่งแวดล้อม (environmental field) 4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)	- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs) • อะคริโลไนไตรล์ (Acrylonitrile) 0.04 $\mu g/m^3$ ถึง 43.00 $\mu g/m^3$ (0.02 ppbv ถึง 20.00 ppbv) • ไดคลอโรมีเทน (Dichloromethane) 0.14 $\mu g/m^3$ to 69.00 $\mu g/m^3$ (0.04 ppbv ถึง 20.00 ppbv) • คาร์บอนไดซัลไฟด์ (Carbon disulfide) 0.06 $\mu g/m^3$ ถึง 62.00 $\mu g/m^3$ (0.02 ppbv ถึง 20.00 ppbv) • ไตรคลอโรมีเทน (Trichloromethane) 0.20 $\mu g/m^3$ ถึง 97.00 $\mu g/m^3$ (0.04 ppbv ถึง 20.00 ppbv) • 1,2–ไดคลอโรอีเทน (1,2–dichloroethane) 0.08 $\mu g/m^3$ ถึง 80.00 $\mu g/m^3$ (0.02 ppbv ถึง 20.00 ppbv)	- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)

ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ (Laboratory status) ☑ ถาวร (Permanent) ☑นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสิ่งแวดล้อม (environmental field) 4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)	- สารอินทรีย์ระเหยง่าย (Volatile organic compounds, VOCs) • เบนซีน (Benzene) 0.06 $\mu g/m^3$ ถึง 63.00 $\mu g/m^3$ (0.02 ppbv ถึง 20.00 ppbv) • คาร์บอนเตตระคลอไรด์ (Carbon tetrachloride) 0.25 $\mu g/m^3$ ถึง 125 $\mu g/m^3$ (0.04 ppbv ถึง 20.00 ppbv) • ไตรคลอโรเอทิลีน (Trichloroethylene) 0.21 $\mu g/m^3$ ถึง 107 $\mu g/m^3$ (0.04 ppbv ถึง 20.00 ppbv) • 1,2-ไดคลอโรโพเพน (1,2–dichloropropane) 0.18 $\mu g/m^3$ ถึง 92.00 $\mu g/m^3$ (0.04 ppbv ถึง 20.00 ppbv) • เตตระคลอโรเอทิลีน (Tetrachloroethylene) 0.27 $\mu g/m^3$ ถึง 135 $\mu g/m^3$ (0.04 ppbv ถึง 20.00 ppbv)	- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999

รายละเอียดสาขาและขอบข่ายใบรับรองห้องปฏิบัติการ
(Scope of Accreditation for Testing)
ใบรับรองเลขที่ 24-LB0026
(Certification No. 24-LB0026)

ฉบับที่ 02 (Issue No.02) ออกให้ตั้งแต่วันที่ 30 ตุลาคม พ.ศ. 2566 (Valid from) (30 October B.E.2566 (2023)) ถึงวันที่ 8 กันยายน พ.ศ. 2571 (Until) (8 September B.E.2571 (2028))

สถานภาพห้องปฏิบัติการ (Laboratory status) ☑ ถาวร (Permanent) ☑นอกสถานที่ (Site) ☐ชั่วคราว (Temporary) ☐เคลื่อนที่ (Mobile) ☐หลายสถานที่ (Multisite)

สาขาการทดสอบ (Field of Testing)	รายการทดสอบ (Parameter)	วิธีทดสอบ (Test Method)
สาขาสิ่งแวดล้อม (environmental field) 4. บรรยากาศทั่วไป (ต่อ) (ambient air) (cont.)	- สารอินทรีย์ระเหยง่าย (Volatile organic compounds ,VOCs) • 1,2–ไดโบรโมอีเทน (1,2–dibromoethane) 0.31 $\mu g/m^3$ ถึง 153 $\mu g/m^3$ (0.04 ppbv ถึง 20.00 ppbv) • 1,1,2,2-เตตระคลอโรอีเทน (1,1,2,2–tetrachloroethane) 0.69 $\mu g/m^3$ ถึง 137 $\mu g/m^3$ (0.10 ppbv ถึง 20.00 ppbv) • เบนซิลคลอไรด์ (Benzyl chloride) 0.52 $\mu g/m^3$ ถึง 103 $\mu g/m^3$ (0.10 ppbv ถึง 20.00 ppbv) • 1,4–ไดคลอโรเบนซีน (1,4–dichlorobenzene) 0.24 $\mu g/m^3$ ถึง 120 $\mu g/m^3$ (0.04 ppbv ถึง 20.00 ppbv)	- WI-7.2-1-24 based on US EPA , Compendium Method TO-15 , EPA/625/R-96/010b, Second edition, January 1999

ภาคผนวก ช

ใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์การทำงาน จากกรมสวัสดิการและคุ้มครองแรงงาน

แบบ กภ.บญ
นิติบุคคล



กรมสวัสดิการและคุ้มครองแรงงาน

ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตราย

ในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย

ใบอนุญาตเลขที่ ๐๒๐๑-๐๓-๒๕๖๕-๐๐๔๙

อนุญาตให้ บริษัท ซีคอท จำกัด

เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๖๐๐๐๙๗๖

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวงกำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงานเกี่ยวกับสารเคมีอันตราย พ.ศ. ๒๕๕๖ ในการเป็นผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย ประกอบกับกฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริมความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๑๔ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม
ข-๑๑-๐๒๐๑-๐๔๙-๐๑-๖๕

(ลงนาม)..... (นายทะเบียน)
(นายศักดิ์ศิลป์ ตุลาธร)
ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการตรวจวัดระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงาน
และสถานที่เก็บรักษาสารเคมีอันตราย
ของบริษัท ซีคอท จำกัด
ใบอนุญาตเลขที่ ๐๒๐๑-๐๓-๒๕๖๕-๐๐๔๙

๑. นายชิตพล	สมประสงค์
๒. นายอนิวัฒน์	พิมวันนา
๓. นายศิวะนนท์	กุลวงษ์
๔. นายวัชรกานต์	ประมาคะเต
๕. นายธนโชติ	ช่างล้อ
๖. นายกิตติพงศ์	ถะเกิงสุข
๗. นายจีรวัฒน์	โคตรคำหาญ
๘. นายศุภกิจ	ต๊ะมูกา
๙. นางสาวธัญลักษณ์	โยธา
๑๐.นางสาวทิพย์สุดา	วรรณการ
๑๑.นางสาวสายธาร	ภูเขียว
๑๒.นายภาคภูมิ	แทนไทย
๑๓.นายธนาวุฒิ	ด่วนแสง
๑๔.นายรัตนชัย	ชอบทำกิจ

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

แบบ กภ.บญ
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน
ใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตราย
ในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย

ใบอนุญาตเลขที่ ๐๒๐๒-๐๓-๒๕๖๕-๐๐๓๔

อนุญาตให้ บริษัท ซีคอท จำกัด
เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๖๐๑๐๙๖
ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร
เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวงกำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงานเกี่ยวกับสารเคมีอันตราย พ.ศ. ๒๕๕๖ ในการเป็นผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงานและสถานที่เก็บรักษาสารเคมีอันตราย ประกอบกับกฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริมความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๑๔ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๔ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม
ข-๑๑-๐๒๐๒-๐๓๔-๐๑-๖๕
(ลงนาม).....(นายทะเบียน)
(นายศักดิ์ศิลป์ ตุลาธร)
ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการวิเคราะห์ระดับความเข้มข้นของสารเคมีอันตรายในบรรยากาศของสถานที่ทำงาน
และสถานที่เก็บรักษาสารเคมีอันตราย
ของบริษัท ซีคอท จำกัด
ใบอนุญาตเลขที่ ๐๒๐๒-๐๓-๒๕๖๕-๐๐๓๔

๑.	นางสาวนริสา	ภูวสรรเพ็ชญ์
๒.	นางอารยา	ทิพรักษ์
๓.	นางสาวศิริวรรณ	ฉิมสง่า
๔.	นางสาวสุธาทิพย์	เทียนเตี้ย
๕.	นางสาวพรนภา	บุตรธรรม
๖.	นางสาวธาริณี	อาจปลิว
๗.	นางสาวกฤษณา	จันทุม
๘.	นางสาวพัชรา	สมานฉันท์
๙.	นางสาวจณิสตา	กุ้ยอ่อน
๑๐.	นางสาวศศิภา	ใจดี
๑๑.	นางสาวจุฑารัตน์	แจ่มเรือน
๑๒.	นางสาวณัฐศิริ	เลิศธีรพิพัฒน์
๑๓.	นางสาวสัญญลักษณ์	อินทรประสิทธิ์
๑๔.	นางสาวสุดาพร	สุนทร

ทั้งนี้ ตั้งแต่วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๓ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๕ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน



แบบ กภ.บญ
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน

ใบอนุญาต

เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับความร้อน

ใบอนุญาตเลขที่ ๐๔๐๑-๐๓-๒๕๖๕-๐๐๔๘

อนุญาตให้ บริษัท ซีคอท จำกัด

เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๖๐๐๐๙๗๖

ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร

เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวงกำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงานเกี่ยวกับความร้อน แสงสว่าง และเสียง พ.ศ. ๒๕๕๙ ในการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับความร้อน ประกอบกับกฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริมความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๕ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม
ข-๑๑-๐๔๐๑-๐๔๘-๐๑-๖๕

(ลงนาม)..... (นายทะเบียน)
(นายศักดิ์ศิลป์ ตุลาธร)
ตำแหน่ง ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับความร้อน
ของบริษัท ซีคอท จำกัด
ใบอนุญาตเลขที่ ๐๔๐๑-๐๓-๒๕๖๕-๐๐๔๘

๑. นางสาวสุนันทา	ศิรวุฒินานนท์
๒. นางสาวกนิษฐา	เจริญเชื้อ
๓. นางสาวปัทมวรรณ	สุวรรณวิโรจน์
๔. นางสาวอลิษา	คนิวรานนท์
๕. นางสาวชนิตา	หล่ำสาย

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากร (เพิ่มเติม)
แนบท้ายใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับความร้อน
ของบริษัท ซีคอท จำกัด
ใบอนุญาตเลขที่ ๐๔๐๑-๐๓-๒๕๖๕-๐๐๔๘

๑. นางสาวศลิษา	อินรีย์
๒. นางสาวมารียาณี	ฮาแว
๓. นางสาววิระยา	ปัจฉิมบูรณ์

ทั้งนี้ ตั้งแต่วันที่ ๑๙ มกราคม พ.ศ. ๒๕๖๖ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๙ มกราคม พ.ศ. ๒๕๖๖

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน



แบบ กภ.บญ
นิติบุคคล

กรมสวัสดิการและคุ้มครองแรงงาน
ใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับเสียง

ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

อนุญาตให้ บริษัท ซีคอท จำกัด
เลขทะเบียนนิติบุคคล ๐๑๐๕๕๓๖๐๐๐๙๗๖
ตั้งอยู่ เลขที่ ๒๓๙ ถนนริมคลองประปา แขวงบางซื่อ เขตบางซื่อ กรุงเทพมหานคร
เป็นนิติบุคคลผู้ให้บริการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน ตามกฎกระทรวงกำหนดมาตรฐานในการบริหาร จัดการ และดำเนินการด้านความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงานเกี่ยวกับความร้อน แสงสว่าง และเสียง พ.ศ. ๒๕๕๙ ในการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับเสียง ประกอบกับกฎกระทรวงการขึ้นทะเบียนและการอนุญาตให้บริการเพื่อส่งเสริม ความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๖๔ แห่งพระราชบัญญัติความปลอดภัย อาชีวอนามัย และสภาพแวดล้อมในการทำงาน พ.ศ. ๒๕๕๔ โดยมีบุคลากร จำนวน ๕ ราย ดังรายชื่อแนบท้ายใบอนุญาตนี้

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

เลขทะเบียนควบคุม
ข-๑๑-๐๔๐๓-๐๔๘-๐๑-๖๕

(ลงนาม) .....(นายทะเบียน)
(นายศักดิ์ศิลป์ ตุลาธร)
ตำแหน่ง ผู้อำนวยการกองความปลอดภัยแรงงาน

รายชื่อบุคลากรแนบท้ายใบอนุญาต
เป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับเสียง
ของบริษัท ซีคอท จำกัด
ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

๑. นางสาวสุนันทา	ศิรวุฒินานนท์
๒. นางสาวกนิษฐา	เจริญเชื้อ
๓. นางสาวปัทมวรรณ	สุวรรณวิโรจน์
๔. นางสาวอลิษา	คนิวรานนท์
๕. นางสาวชนิตา	หล่ำสาย

ทั้งนี้ ตั้งแต่วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๗ มิถุนายน พ.ศ. ๒๕๖๕

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน

รายชื่อบุคลากร (เพิ่มเติม)
แนบท้ายใบอนุญาตเป็นนิติบุคคลผู้ให้บริการตรวจวัดและวิเคราะห์สภาวะการทำงานเกี่ยวกับระดับเสียง
ของบริษัท ซีคอท จำกัด
ใบอนุญาตเลขที่ ๐๔๐๓-๐๓-๒๕๖๕-๐๐๔๘

๑. นางสาวศลิษา	อินรีย์
๒. นางสาวมารียาณี	ฮาแว
๓. นางสาววิระยา	ปัจฉิมบูรณ์

ทั้งนี้ ตั้งแต่วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖ ถึงวันที่ ๑๖ มิถุนายน พ.ศ. ๒๕๖๘

ให้ไว้ ณ วันที่ ๑๓ มกราคม พ.ศ. ๒๕๖๖

(นายสมพจน์ กวางแก้ว)
รองอธิบดี ปฏิบัติราชการแทน
อธิบดีกรมสวัสดิการและคุ้มครองแรงงาน