

ภาคผนวก จ

เอกสารสอบเทียบเครื่องมือ



List of Instruments Certification for Water Quality Analysis

1.โครงการรถไฟฟ้าสีเขียวอ่อนช่วงแบร์ริง-สมุทรปราการ

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Water									
1	pH Meter	pH	YSI	pH100A JC03354	Technology Promotion Association (Thailand-Japan)	23CH1487	22 Nov 23	21 Nov 24	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Particulate Matter < 10 µm (PM ₁₀)	Andersen Instruments, Inc.	G25A 11MX	Jiranatee Associates Co., Ltd.	CO-005-66	12 Jun 23	11 Jun 24	-
2	U-Tube Manometer	Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	23P1402	9 May 23	8 May 24	-
3	Aneroid Barometer	Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23P1855	2 Jun 23	1 Jun 24	-
4	Dial Thermo-Hygrometer	Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23H1200	6 Jun 23	5 Jun 24	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1182920005	UAE Consultant Co.,Ltd.	13112023	13 Nov 23	12 Nov 24	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1182920006	UAE Consultant Co.,Ltd.	01112023	1 Nov 23	31 Oct 24	-
7	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1182920009	UAE Consultant Co.,Ltd.	13112023	13 Nov 23	12 Nov 24	-
8	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1191503036	UAE Consultant Co.,Ltd.	13112023	13 Nov 23	12 Nov 24	-
9	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1191503037	UAE Consultant Co.,Ltd.	13112023	13 Nov 23	12 Nov 24	-
10	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
11	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48C 48C-62460-355/5	UAE Consultant Co.,Ltd.	08122023	8 Dec 23	7 Dec 24	-
12	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48C 48C-62494-335-5	UAE Consultant Co.,Ltd.	08112023	8 Nov 23	7 Nov 24	-
13	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48C 48C-69160-362	UAE Consultant Co.,Ltd.	08112023	8 Nov 23	7 Nov 24	-

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
14	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48C 48C-73881-375	UAE Consultant Co.,Ltd.	08112023	8 Nov 23	7 Nov 24	-
15	Carbon Monoxide Analyzer	Carbon Monoxide	Thermo	48C 48C-71185-368	UAE Consultant Co.,Ltd.	18122023	18 Dec 23	17 Dec 24	-
16	Standard Gases (Mixture)	Carbon Monoxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
17	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2111DR0052	Thai Meteorological Department	098/24	22 Feb 24	21 Feb 25	-
18	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2111DT0058	Thai Meteorological Department	121/24	13 Mar 24	12 Mar 25	-
19	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2112DR0065	Thai Meteorological Department	097/24	22 Feb 24	21 Feb 25	-
20	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2311DR0037	Thai Meteorological Department	123/24	13 Mar 24	12 Mar 25	-
21	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2205DT0008	Thai Meteorological Department	122/24	13 Mar 24	12 Mar 25	-
22	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	Larson Davis	CAL150 6171	Innovative Instrument Co.,Ltd.	23-ACT-118	4 Aug 23	3 Aug 24	-
23	Sound Level Meter	$L_{Aeq} 1 \text{ hour}$, $L_{Aeq} 24 \text{ hours}$, L_{Amax} L_{A90} , L_{Adn}	Larson Davis	LxT2 0005293	Innovative Instrument Co.,Ltd.	23-SLM-210	23 Jun 23	22 Jun 24	-
24	Sound Level Meter	$L_{Aeq} 1 \text{ hour}$, $L_{Aeq} 24 \text{ hours}$, L_{Amax} L_{A90} , L_{Adn}	Larson Davis	LxT2 0005294	Innovative Instrument Co.,Ltd.	23-SLM-222	28 Jun 23	27 Jun 24	-
25	Sound Level Meter	$L_{Aeq} 1 \text{ hour}$, $L_{Aeq} 24 \text{ hours}$, L_{Amax} L_{A90} , L_{Adn}	Larson Davis	LxT2 0005296	Innovative Instrument Co.,Ltd.	23-SLM-209	23 Jun 23	22 Jun 24	-
26	Sound Level Meter	$L_{Aeq} 1 \text{ hour}$, $L_{Aeq} 24 \text{ hours}$, L_{Amax} L_{A90} , L_{Adn}	Larson Davis	LxT2 0005305	Innovative Instrument Co.,Ltd.	23-SLM-225	28 Jun 23	27 Jun 24	-
27	Sound Level Meter	$L_{Aeq} 1 \text{ hour}$, $L_{Aeq} 24 \text{ hours}$, L_{Amax} L_{A90} , L_{Adn}	Larson Davis	LxT2 0005339	Innovative Instrument Co.,Ltd.	23-SLM-223	28 Jun 23	27 Jun 24	-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES & EQUIPMENT CALIBRATION AND TESTING SERVICES
5344 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-9000-29 FAX. 0-2719-9484



Cert.No.: 23CH1487
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : EcoSense
Model : pH10DA
Serial No. : JC03354
ID No. : UAE.EFM.063/2562(ENV.pH 03/62)
Condition As-Received: Used Item
Received Date : 21 November 2023
Calibration Date : 22 November 2023
Reference : 2311-0720WSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with standard
voltage calibrator and direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lemgagatrakul

Approved by :
Approved Signatory

(✓) Sathip Meangmal
() Warakorn Lemgagatrakul
() Ponpan Palpim

Issue Date : 27 November 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the Head of Corporate Services & Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม
A 0061266



Cert.No.: 23CH1487
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument : -
Instrument Serial No. ID No. Cert. No. Due Date
1) Document Process Calibrator 54030049 130RC116 23E2802 27 Aug 2024
2) Ref. Standard Thermometer 4982054 110RC044 23I908 26 July 2024
This certification is traceable to the International System of Unit maintained through:-
- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	913598	14 July 2025
pH 6.985	CPA chem	913599	14 July 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of measurement (\pm mV)	Coverage factor k
	pH	mV	mV	pH		
pH Meter S/N.: JC03354	4.00	177.48	177	4.01	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	7.00	0.00	0	7.00	0.58	2.00
	10.00	-177.48	-178	10.01	0.58	2.00

Sathip

เอกสารไม่ควบคุม
a 1191352



Cert.No.: 23CH1487
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (\pm)	Coverage factor k
pH Electrode S/N.: 230906SIA605377	4.008	4.01	174	0.0085	2.05
	6.985	7.00	-2	0.0099	2.00
	6.985	7.00	-2	0.0093	2.00
	9.997	10.00	-177	0.0092	2.00

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model :
- Serial No. : 230906SIA605377
Dimension of probe;
- Length : 110 mm
- Diameter : 12 mm
- Immersion Depth : 100 mm

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (\pm °C)	Coverage factor k
25.0	25.002	25.1	0.098	0.13	2.00
30.0	30.001	30.1	0.099	0.13	2.00
35.0	35.003	35.0	-0.003	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-000-

Sathip

เอกสารไม่ควบคุม
a 1191351



Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7/71, Rd. Wattthana, Bangkok, Thailand
Tel: +6628680813
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367
Flow measurement laboratory
Calibration services department.



NSC - TISI - TIS 17025
CALIBRATION 0367

CERTIFICATE OF CALIBRATION

Certificate No. : CO-005-66

Page 1 of 2 Pages

MEASUREMENT ITEM

MANUFACTURER : Top Load Orifice
MODEL/TYPE : Andersen Instruments
SERIAL NUMBER : G25A
ID NUMBER : 11MX
CONDITION AS-RECEIVED : UAE.ANV.008/2543
CUSTOMER : Used item

RECEIVED DATE : 02 Jun 2023
MEASUREMENT DATE : 12 Jun 2023
ISSUE DATE : 12 Jun 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 24.0 °C and 56.4%RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:
The Orifice gas flow device was calibrated against
Standard Rotary Displacement Meter (Roots,
Meter) Model G65/IMC/W2-dp. The Wt-GI-004
was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The
measurement to recognized the national
standards and to realization of the international
system of units (SI) through the VSL (National
Metrology Institute of Netherlands) via Certificate
number: G2211901

Uncertainty of Measurement:
The reported uncertainty of measurement is based
on the standard uncertainty multiplied by a
coverage factor $k=2$. Which for a normal
distribution corresponds to a coverage probability
of approximately 95%. The standard uncertainty
has been determined in accordance with the GUM
Evaluation of measurement
data - Guide to the expression of uncertainty in
measurement



Calibrated by:

Mr. Sorawit Thachalad
Ms. Jitraporn Lertsomphol

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q standard calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH ₂ O	γ	Standard Flow [Q _s] m ³ /min
1	0.705	754.535	24.09	23.49	51.470	1.745	1.318	0.656
2	0.998	754.592	24.01	23.68	55.777	3.453	1.855	0.922
3	1.124	754.473	23.93	23.53	37.502	4.619	2.145	1.066
4	1.172	754.436	23.39	23.00	27.960	5.187	2.275	1.128
5	1.418	754.502	23.52	23.02	28.014	7.616	2.756	1.365

Slope (m): 2.02897
Intercept (b): -0.01391
Correlation coefficient (r): 0.99986
Uncertainty (k=2): 0.015 m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH ₂ O	γ	Standard Flow [Q _s] m ³ /min
1	0.705	754.535	24.09	23.49	51.470	1.745	0.829	0.658
2	0.998	754.592	24.01	23.68	55.777	3.453	1.166	0.925
3	1.124	754.473	23.93	23.53	37.502	4.619	1.349	1.070
4	1.172	754.436	23.39	23.00	27.960	5.187	1.428	1.130
5	1.418	754.502	23.52	23.02	28.014	7.616	1.730	1.368

Slope (m): 1.27084
Intercept (b): -0.00875
Correlation coefficient (r): 0.99986
Uncertainty (k=2): 0.015 m³/min

End of Certificate of Calibration



เอกสารไม่ควบคุม



Certificate of Calibration

Certificate No.: 23P1402
Page: 1 of 2

Equipment: U Tube Manometer

Manufacturer: Dwyer

Model: 1221-36-W/M

Serial No.: -

ID No.: UAE.EFM.180/2561

Condition As-Received: Used Item

Received Date: 26 April 2023

Calibration Date: 09 May 2023

Reference: 2304-0703WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1010 mbar

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using "DKD-R 6-1"; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0137-22	24 Aug 2023
2.This result of calibration was made on requested at the point specified by customer.				
3.Scale and conversion factor is 1 kPa = 4.0146293 inH ₂ O				
4.This instrument was used clean air as pressure media.				
5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.				
6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.				
7.The certificate is valid only to the item calibrated on date and place of calibration.				
8.This Certification is traceable to the International System of Unit maintained through:-				
-National Institute of Metrology Thailand (NIMT)				

Calibrated by: Suwit Aussarree
Issue Date: 11 May 2023

Approved Signatory: Attapol P.
[] Phalinee Prabpaipal
[] Sura Suwannasri
[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0314242



Cert.No.: 23P1402
Page: 2 of 2

Result of calibration:- Without adjustment
Function:- Pressure Measurement
Increasing Pressure

Range: 0 inH₂O to 36 inH₂O
Scale Interval: 0.1 inH₂O (The Fifth Estimate)

UUC Indication			ΔP (inH ₂ O)	Error (inH ₂ O)
Applied Pressure (inH ₂ O)	High-port side (inH ₂ O)	Low-port side (inH ₂ O)		
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	8.00	0.00
10.00	5.00	-5.00	10.00	0.00
12.00	6.00	-6.00	12.00	0.00
14.00	7.00	-7.02	14.02	0.02
16.00	8.00	-8.02	16.02	0.02
18.00	9.02	-9.04	18.06	0.06
20.00	10.02	-10.04	20.06	0.06
22.00	11.00	-11.04	22.04	0.04
24.00	12.02	-12.06	24.08	0.08
26.00	13.02	-13.06	26.08	0.08
28.00	14.02	-14.04	28.06	0.06
30.00	15.02	-15.02	30.04	0.04
32.00	16.00	-16.02	32.02	0.02
34.00	17.00	-17.00	34.00	0.00
35.80	17.96	-17.98	35.94	0.14

The uncertainty of measurement was ± 0.11 inH₂O

* UUC = Unit Under Calibration

* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-o-o-

Attapol P.

เอกสารไม่ควบคุม
a 1160343



Certificate of Calibration

Certificate No.: 23P1855
Page: 1 of 2

Equipment: Aneroid Barometer

Manufacturer: Barigo

Model: -

Serial No.: -

ID No.: UAE.ANV.122/2550

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 02 June 2023

Reference: 2305-0919WSC

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1007 mbar

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using "DKD-R 6-1"; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024
2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.				
3.This result of calibration was made on requested at the point specified by customer.				
4.This result of calibration instrument was in absolute pressure.				
5.This instrument was used clean air as pressure media.				
6.The certificate is valid only to the item calibrated on date and place of calibration.				
7.This Certification is traceable to the International System of Unit maintained through:-				
-National Institute of Metrology Thailand (NIMT)				

Calibrated by: Suksan Khankaew
Issue Date: 08 June 2023

Approved Signatory: Attapol P.
[] Phalinee Prabpaipal
[] Sura Suwannasri
[x] Attapol Panurach

เอกสารไม่ควบคุม
B 0316955



Cert.No.: 23P1855
Page: 2 of 2

Result of calibration:- Without adjustment
Function:- Absolute Pressure Measurement

Range: 960 hPa to 1030 hPa
Scale interval: 1 hPa (The Fifth Estimate)

Increasing Pressure

Applied Pressure (hPa)	958.50	969.59	980.35	990.39	1001.01	1011.15	1020.94	1031.45
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	1.50	0.41	-0.35	-0.39	-1.01	-1.15	-0.94	-1.45

Decreasing Pressure

Applied Pressure (hPa)	1031.45	1021.61	1012.16	1002.38	992.17	982.20	970.69	959.32
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-1.45	-1.61	-2.16	-2.38	-2.17	-2.20	-0.69	0.68

The uncertainty of measurement was ± 0.30 hPa

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-000-

Aitapoi R

เอกสารไม่ควบคุม
a 1165504



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 23H1200
Page: 1 of 2

Equipment: Dial Thermo-Hygrometer

Manufacturer: Barigo

Model: -

Serial No.: -

ID No.: UAE.ANV.130/2550

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 30 May 2023
to 06 June 2023

Reference: 2305-0919WSC

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments:

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Hygro-M2 Dew Point Monitor	5112	2360195	20703	02 Aug 2023
2) Handheld Thermometer With Sensor	1523	3240076	23105	15 Mar 2024

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

- National Institute of Standards and Technology (NIST), The United States of America
- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by: Somchai Durmwor
Issue Date: 07 June 2023

Approved Signatory:

[] Chakrit Waewwanjua
[] Pornthippa Tameyakul
[] Viporn Tantiyawutti

เอกสารไม่ควบคุม
B 0316274



Cert. No.: 23H1200
Page: 2 of 2

Result of Calibration:-
Function: Humidity Measurement

Before Adjustment

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	48	7.9	1.6
25.0	60.0	63	3.0	1.7
25.0	80.0	76	-4.0	1.9

Result of Calibration:-
Function: Humidity Measurement

After Adjustment

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	44	3.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	75	-5.0	1.9

Result of Calibration:-
Function: Temperature Measurement

Without Adjustment

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
19.987	20.0	0.013	0.72
30.016	30.0	-0.016	0.72
39.944	39.5	-0.444	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-000-

Aitapoi R

เอกสารไม่ควบคุม
a 1165295



United Analyst and Engineering Consultant Co., Ltd.

3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Tel. 0 2763 2828 Fax 0 2763 2800 www.uaiconsultant.com E-mail: uae@uaiconsultant.com

MULTI-POINT GAS TEST REPORT

Test Date: Nov 13, 2023


Equipment: Gas Analyzer (NO₂)
Manufacturer: Thermo Scientific
Model: 42i
Serial Number: 1182920005

Standard Gas Concentration

Standard Gas Concentration	Value	Unit	Dilutor Detail
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer: Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model: 146i
Methane (CH ₄)	-	PPM	Serial Number: 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No.:	EB0143262		
Expiration Date:	Jun 21, 2024		

Multi-point gas test data

Reference Value (ppb)	Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1 Zero	0.0	0.70	0.70	0.70
Level 2 20.00%	100.0	0.90	0.89	0.89
Level 3 40.00%	200.0	0.50	0.25	0.25
Level 4 60.00%	300.0	0.70	0.23	0.23
Level 5 80.00%	400.0	0.00	0.00	0.00
Remark: Measuring Range	500.0 ppb	Average Difference (%)	0.41	
:Acceptable Limit $\pm 5\%$				

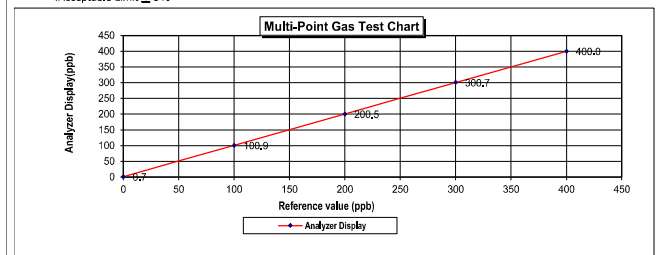

Calculate by

13 / Nov / 2023

Approve by

13 / Nov / 2023

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Nov 1, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1182920006

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.80	0.80	0.80
Level 2	20.00%	100.0	1.10	1.09	1.09
Level 3	40.00%	200.0	0.70	0.35	0.35
Level 4	60.00%	300.0	0.70	0.23	0.23
Level 5	80.00%	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)		0.49

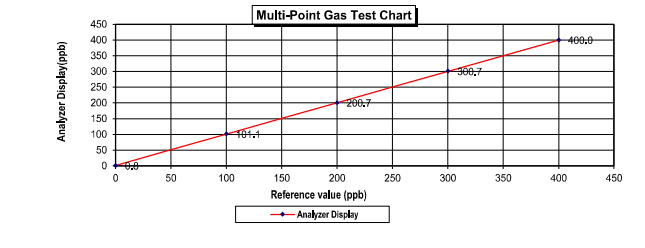

Calculate by

01 Nov 2023

Approve by

01 Nov 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 13, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1182920009

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.70	0.70	0.70
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.8	0.80	0.40	0.40
Level 4	60.00%	300.0	300.6	0.60	0.20	0.20
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.44

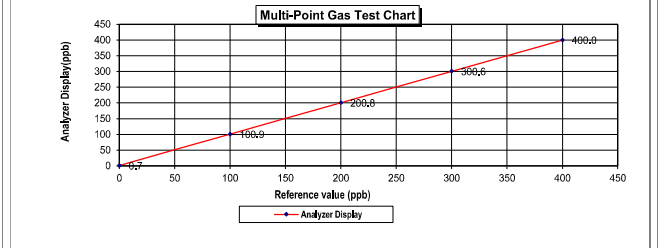

Calculate by

13 Nov 2023

Approve by

13 Nov 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 13, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1191503036

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.70	0.70	0.70
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	301.1	1.10	0.37	0.37
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.46

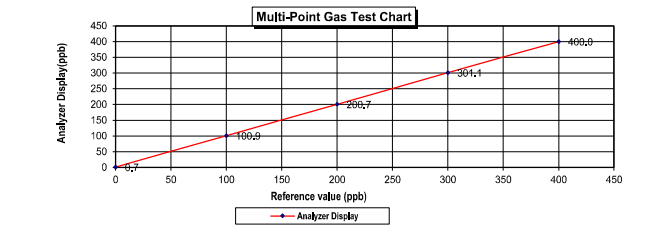

Calculate by

13 Nov 2023

Approve by

13 Nov 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 13, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : 1191503037

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8			
Cylinder No. :	EB0143262			
Expiration Date :	Jun 21, 2024			

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.70	0.70	0.70
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.8	0.80	0.40	0.40
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)		0.41	

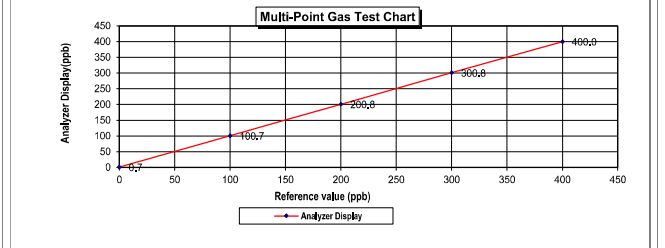

Calculate by

13 Nov 2023

Approve by

13 Nov 2023

CERTIFICATE OF ANALYSIS
Grade of Product: EPA Protocol

Part Number: E04NI99E15A01D3 Reference Number: 122-402135187-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 690
Gas Code: CO,NO,NOX,SO2,BALN Certification Date: Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA-800R-12/21, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a label analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.98 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.90 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	05/14/2021
NITROGEN	Balance				

Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
INTRM	20051120	CC738029	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D585025	9.81 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	40142383102	CC595981	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 16, 2023
INTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
INTRM	14050119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.6%	Nov 16, 2025

The GMS, PRM or RDM noted above is only in reference to the GMS used in the assay and not part of the analysis.

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0601333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0601333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0601333 NO2	FTIR	Jun 03, 2021
Nicolet 6700 AHR0601333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Dec 8, 2023

Equipment : Gas Analyzer (CO) Model : 48C
Manufacturer : Thermo Environmental Instruments Serial Number : 48C-62460-335/5

Standard Gas Concentration


Sulphur Dioxide (SO ₂)	41.68	PPM
Nitric Oxide (NO)	45.94	PPM
Methane (CH ₄)	-	PPM
Carbon Monoxide (CO)	984.8	PPM
Cylinder No. :	EB0143262	
Expiration Date :	Jun 20, 2024	

Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	1461
Serial Number :	1180540071

Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.7	0.7
Level 2	20.00%	10.0	10.8	0.8	7.4
Level 3	40.00%	20.0	20.8	0.8	3.8
Level 4	60.00%	30.0	30.9	0.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0
Remark : Measuring Range	50.0 ppm		Average Difference (%)	2.97	
:Acceptable Limit \pm 5%					

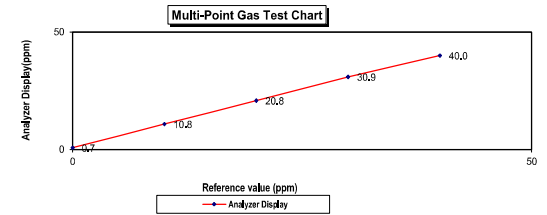

Calculate by

Spirita: C
.....8...../.....12...../.....2023.

Approve by

Pattana: P
.....8...../.....Dec...../.....2023

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Nov 8, 2023


Equipment : Gas Analyzer (CO) Model : 48C
Manufacturer : Thermo Environmental Instruments Serial Number : 48C-62494-335/5

Standard Gas Concentration

Sulphur Dioxide (SO ₂)	41.68	PPM
Nitric Oxide (NO)	45.94	PPM
Methane (CH ₄)	-	PPM
Carbon Monoxide (CO)	984.8	PPM
Cylinder No. :	EB0143262	
Expiration Date :	Jun 20, 2024	

Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.8	0.8	0.8
Level 2	20.00%	10.0	10.5	0.5	4.8
Level 3	40.00%	20.0	20.6	0.6	2.9
Level 4	60.00%	30.0	30.9	0.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0
Remark : Measuring Range	50.0 ppm		Average Difference (%)	2.28	
:Acceptable Limit \pm 5%					

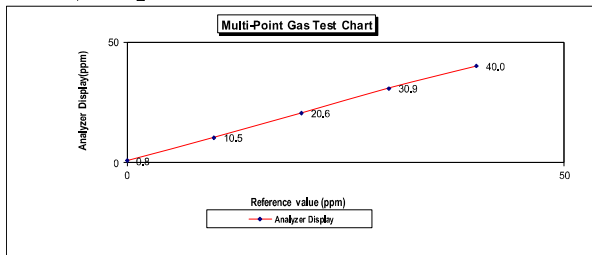

Calculate by

Spirita: C
.....8...../.....11...../.....2023.

Approve by

Pattana: P
.....8...../.....Nov...../.....2023

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Nov 8, 2023

Equipment : Gas Analyzer (CO) Model : 48C
Manufacturer : Thermo Environmental Instruments Serial Number : 48C-69160-362

Standard Gas Concentration


Sulphur Dioxide (SO ₂)	41.68	PPM
Nitric Oxide (NO)	45.94	PPM
Methane (CH ₄)	-	PPM
Carbon Monoxide (CO)	984.8	PPM
Cylinder No. :	EB0143262	
Expiration Date :	Jun 20, 2024	

Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	1461
Serial Number :	1180540071

Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.9	0.9	0.9
Level 2	20.00%	10.0	10.7	0.7	6.5
Level 3	40.00%	20.0	20.6	0.6	2.9
Level 4	60.00%	30.0	30.9	0.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0
Remark : Measuring Range	50.0 ppm		Average Difference (%)	2.65	
:Acceptable Limit \pm 5%					

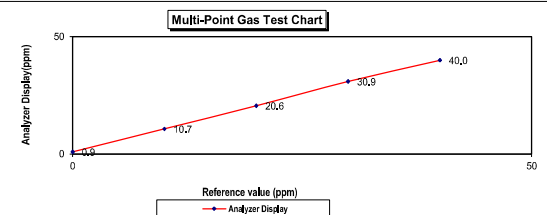

Calculate by

Spirita: C
.....8...../.....11...../.....2023.

Approve by

Pattana: P
.....8...../.....Nov...../.....2023

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Nov 8, 2023

Equipment : Gas Analyzer (CO) Model : 48C
Manufacturer : Thermo Environmental Instruments Serial Number : 48C-73881-375

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 1461
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No. :	EB0143262		
Expiration Date :	Jun 20, 2024		

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.7	0.7	0.7
Level 2	20.00%	10.0	10.6	0.6	5.7	5.7
Level 3	40.00%	20.0	20.8	0.8	3.8	3.8
Level 4	60.00%	30.0	30.4	0.4	1.3	1.3
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)			2.30

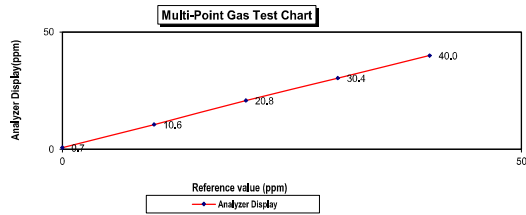

Calculate by

8 / 11 / 2023

Approve by

8 / Nov / 2023

Page 1 of 1

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT


Test Date : Dec 18, 2023

Equipment : Gas Analyzer (CO) Model : 48C
Manufacturer : Thermo Environmental Instruments Serial Number : 48C-71185-368

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 1461
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No. :	EB0143262		
Expiration Date :	Jun 20, 2024		

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.8	0.8	0.8	0.8
Level 2	20.00%	10.0	10.6	0.6	5.7	5.7
Level 3	40.00%	20.0	20.9	0.9	4.3	4.3
Level 4	60.00%	30.0	30.8	0.8	2.6	2.6
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)			2.67

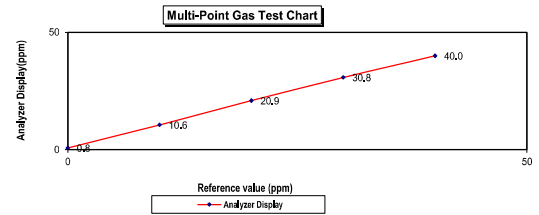

Calculate by

18 / 12 / 2023

Approve by

18 / Dec / 2023

Page 1 of 1

เอกสารไม่ควบคุม



Airgas Specialty Gases
Airgas USA, LLC
650 United Drive
Durham, NC 27713
Airgas.com

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04N198E15A01D3 Reference Number: 122-402135187-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO2,BALN Certification Date: Jun 21, 2021
Expiration Date: Jun 21, 2024

Certification performed in accordance with EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012) (current EPA 600R-12/2011), using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder had a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a nitrogen basis unless otherwise noted.
Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.98 PPM	G1	\pm 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	\pm 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.98 PPM	G1	\pm 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	\pm 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

Type	Lot ID	Cylinder No.	Concentration	Uncertainty	Expiration Date
NTRM	20061120	CC708088	49.82 PPM NITRIC OXIDE/NITROGEN	\pm 1.0%	Feb 02, 2025
PRM	12386	D585025	9.91 PPM NITROGEN DIOXIDE/AIR	\pm 2.0%	Feb 20, 2020
GMIS	401423838102	CC059581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	\pm 2.1	Feb 16, 2023
NTRM	16011043	CC432277	49.02 PPM SULFUR DIOXIDE/NITROGEN	\pm 0.8%	Jun 17, 2022
NTRM	14050119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	\pm 0.6%	Nov 16, 2025

Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO2	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002607
GROSS WT: 28.40kg
NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

Calibration Certificate

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue : 22 February, 2024

Certification No. 098/24

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2111DR0052

Wind Sensor 2111DT0052

Customer : United Analyst and Engineering Consultant Co., Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1009.5 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

: Digital Barometer Vaisala Type PTB333 No. 34320001

Calibrated by : Mr. Watcharapol Subwat

Signed : Mr. Pisod Promsut

Mechanical Engineer

(Authorized Signatory)

for the Chief

Sub-Standard Instrument

เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 098/24

Page : 3 of 5

22 February, 2024

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1010.84	1011	-0.16
1010.60	1010	0.60
1011.71	1012	-0.29
1012.17	1012	0.17
1012.31	1012	0.31
1012.25	1012	0.25
1012.79	1013	-0.21
1012.95	1012	0.95
1013.52	1014	-0.48
1014.16	1014	0.16
1015.79	1016	-0.21
1016.02	1016	0.02
1015.86	1016	-0.14
1015.69	1015	0.69
1011.51	1012	-0.49
1011.80	1012	-0.20
1012.06	1012	0.06
1012.81	1013	-0.19
1013.22	1013	0.22
1013.49	1013	0.49
Average		0.08

Calibrated by :

Mr. Watcharapol Subwat
Mechanical EngineerCalibration & Test Section
Meteorological Instruments Bureau

Calibrated by :

Mr. Watcharapol Subwat
Mechanical EngineerCalibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 098/24

22 February, 2024

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
758.19	758	0.19
758.01	758	0.01
758.84	759	-0.16
759.19	759	0.19
759.29	759	0.29
759.25	759	0.25
759.65	760	-0.35
759.77	760	-0.23
760.20	760	0.20
760.68	760	0.68
761.90	762	-0.10
762.08	762	0.08
761.96	762	-0.04
761.83	762	-0.17
758.69	759	-0.31
758.91	759	-0.09
759.11	759	0.11
759.67	760	-0.33
759.98	760	-0.02
760.18	760	0.18
Average		0.02

Calibrated by :

Mr. Watcharapol Subwat
Mechanical EngineerCalibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 098/24

22 February, 2024

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.2	45	0.2
30.3	30	0.3
15.8	15	0.8

Calibrated by :

Mr. Watcharapol Subwat
Mechanical EngineerCalibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 13 March, 2024

Certification No. 121/24

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2111DR0058

Wind Sensor 2111DT0058

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1011.9 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-850-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

: Digital Barometer Vaisala Type PTB330 No. J43900001

Calibrated by :

Signed :

(Authorised Signatory

for the Chief

Sub-Standard Instrument

Mr. Watcharapol Subwat

Mr. Pisood Promsut

Mechanical Engineer

Sub-Standard Instrument

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

13 March, 2024

Certification No. 121/24

Page : 2 of 5

Standard	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Velocity	Velocity	Correction
Ultrasonic Anemometer	m/sec	inches H2O	inches H2O	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	8.9	0.12
11.02	-	-	-	11.0	0.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.9	0.12

Wind Aloft Plotting Board.	
U.S.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

Mechanical Engineer

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 121/24

13 March, 2024

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1009.59	1009	0.59
1009.45	1010	-0.55
1010.10	1010	0.10
1010.94	1011	-0.06
1011.46	1011	0.46
1011.84	1012	-0.16
1012.06	1012	0.06
1013.04	1013	0.04
1013.18	1013	0.18
1012.89	1013	-0.11
1013.20	1013	0.20
1013.44	1013	0.44
1013.81	1014	-0.19
1014.19	1014	0.19
1015.96	1016	-0.04
1016.23	1016	0.23
1015.64	1015	0.64
1015.23	1015	0.23
1012.87	1013	-0.13
1013.63	1014	-0.37

Average

0.09

Calibrated by :

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

13 March, 2024

Certification No. 121/24

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
757.25	757	0.25
757.15	757	0.15
757.64	758	-0.36
758.27	758	0.27
758.66	758	0.66
758.94	759	-0.06
759.11	759	0.11
759.84	760	-0.16
759.95	760	-0.05
759.73	760	-0.27
759.96	760	-0.04
760.14	760	0.14
760.42	761	-0.58
760.70	761	-0.30
762.03	762	0.03
762.24	762	0.24
761.79	762	-0.21
761.48	762	-0.52
759.71	760	-0.29
760.28	760	0.28

Average

-0.03

Calibrated by :

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau

เอกสารไม่ควบคุม



The Result of Calibration

13 March, 2024

Certification No. 121/24

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.1	45	0.1
30.2	30	0.2
15.4	16	-0.6

Calibrated by :

Watharapol

Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



เอกสารไม่ควบคุม



Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 22 February, 2024

Certification No. 097/24

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2112DR0065

Wind Sensor 2112DT0065

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1009.8 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo 645 Serial No. 02848057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

: Digital Barometer Vaisala Type PTB320 No. K4360001

Calibrated by : Watharapol

Signed :

(Authorized Signatory)

Mr. Watcharapol Subwat

Mr. Pisod Promsut

for the Chief

Mechanical Engineer

Sub-Standard Instrument

เอกสารไม่ควบคุม



The Result of Calibration

22 February, 2024

Certification No. 097/24

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1010.84	1011	-0.16
1010.60	1011	-0.40
1011.71	1011	0.71
1012.17	1012	0.17
1012.31	1012	0.31
1012.25	1012	0.25
1012.79	1013	-0.21
1012.95	1012	0.95
1013.52	1014	-0.48
1014.16	1014	0.16
1015.79	1016	-0.21
1016.02	1016	0.02
1015.86	1016	-0.14
1015.69	1015	0.69
1011.51	1012	-0.49
1011.80	1012	-0.20
1012.06	1012	0.06
1012.81	1013	-0.19
1013.22	1013	0.22
1013.49	1014	-0.51
Average		0.03

Calibrated by :

Watharapol

Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



เอกสารไม่ควบคุม



The Result of Calibration

22 February, 2024

Certification No. 097/24

Page : 2 of 5

Standard Ultrasonic Anemometer	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacuum inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	2.9	0.12
5.00	-	-	-	4.9	0.10
7.04	-	-	-	7.0	0.04
9.02	-	-	-	9.0	0.02
11.02	-	-	-	11.0	0.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Wind Aloft Plotting Board.	
U.S. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Watharapol

Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau



เอกสารไม่ควบคุม

Calibration & Test Section
Meteorological Instruments Bureau



เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 097/24

22 February, 2024

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
758.19	758	0.19
758.01	758	0.01
758.84	758	0.84
759.19	759	0.19
759.29	759	0.29
759.25	759	0.25
759.65	759	0.65
759.77	760	-0.23
760.20	760	0.20
760.68	760	0.68
761.90	762	-0.10
762.08	762	0.08
761.96	762	-0.04
761.83	762	-0.17
758.69	759	-0.31
758.91	759	-0.09
759.11	759	0.11
759.67	760	-0.33
759.98	760	-0.02
760.18	760	0.18

Average 0.12

Calibrated by :

Hatchaporn

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 097/24

22 February, 2024

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.2	45	0.2
30.3	30	0.3
15.8	16	-0.2

Calibrated by :

Hatchaporn

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 13 March, 2024

Certification No. 123/24

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2311DR0037
Wind Sensor 2112DT0102Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1013.1 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. V1220015

: Digital Barometer Vaisala Type PTB330 No. K4320001

Calibrated by : Hatchaporn

Signed :

(Authorised Signatory)

Mr. Watcharapol Subwat

Mr. Pisoot Promsut

for the Chief

Mechanical Engineer

Sub-Standard Instruments

เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 123/24

13 March, 2024

Page : 2 of 5

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure inches H2O	Vacuum inches H2O	Velocity m/sec	Velocity m/sec	Correction m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	6.9	0.14
9.02	-	-	-	9.0	0.02
11.02	-	-	-	10.9	0.12
13.01	-	-	-	13.0	0.01
15.01	-	-	-	15.0	0.01
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Wind Aloft Plotting Board.	
U.S. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Hatchaporn

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 123/24

13 March, 2024

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1009.59	1009	0.59
1009.45	1009	0.45
1010.10	1010	0.10
1010.94	1011	-0.06
1011.46	1011	0.46
1011.84	1012	-0.16
1012.06	1012	0.06
1013.04	1013	0.04
1013.18	1013	0.18
1012.89	1013	-0.11
1013.20	1013	0.20
1013.44	1014	-0.56
1013.81	1014	-0.19
1014.19	1014	0.19
1015.96	1016	-0.04
1016.23	1016	0.23
1015.64	1016	-0.36
1015.23	1015	0.23
1012.87	1013	-0.13
1013.63	1013	0.63

Average

0.09


Calibrated by :

Watcharapol

Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau



เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 123/24

13 March, 2024

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
757.25	757	0.25
757.15	757	0.15
757.64	758	-0.36
758.27	758	0.27
758.66	759	-0.34
758.94	759	-0.06
759.11	759	0.11
759.84	760	-0.16
759.95	760	-0.05
759.73	760	-0.27
759.96	760	-0.04
760.14	760	0.14
760.42	760	0.42
760.70	761	-0.30
762.03	762	0.03
762.24	762	0.24
761.79	762	-0.21
761.48	761	0.48
759.71	760	-0.29
760.28	760	0.28

Average

0.02


Calibrated by :

Watcharapol

Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau



เอกสารไม่ควบคุม



The Result of Calibration

Certification No. 123/24

13 March, 2024

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.1	45	0.1
30.2	30	0.2
15.4	15	0.4

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section

Meteorological Instruments Bureau



เอกสารไม่ควบคุม



Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 13 March, 2024

Certification No. 122/24

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2205DR0008

Wind Sensor 2205DT0008

Customer : United Analyst and Engineering Consultant Co.,Ltd.
81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1012.5 hPa

NATIONAL STANDARD WIND TUNNEL : Wind Aloft Plotting Board

: Micromanometer Theodor Friedrichs FC014 Serial No. 9310119 : HOOK GAGE NO 1425

N.I.S.T. Test Reference Number 731/241460 : Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)
Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION : Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER : Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057 : Thermoschneider No.918802

STANDARD BAROMETER : Digital Barometer Vaisala Type PTB220 No. Y4220015

: Digital Barometer Vaisala Type PTB330 No. K4320001

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat
Mechanical Engineer

Signed :

Mr. Pisod Promsut

(Authorised Signatory)

for the Chief

Sub-Standard Instrument

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 122/24

13 March, 2024

Page : 2 of 5

Standard Ultrasonic Anemometer	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacuum	Velocity	Velocity	Correction
	m/sec	inches H2O	inches H2O	m/sec	m/sec
1.00	-	-	-	1.0	0.00
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.00
7.04	-	-	-	7.0	0.04
9.02	-	-	-	8.9	0.12
11.02	-	-	-	11.0	0.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.9	0.11
17.02	-	-	-	17.0	0.02
20.02	-	-	-	20.0	0.02

Wind Aloft Plotting Board.	
U.S. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by:
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 122/24

13 March, 2024

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mbar
1009.59	1009	0.59
1009.45	1009	0.45
1010.10	1010	0.10
1010.94	1011	-0.06
1011.46	1012	-0.54
1011.84	1012	-0.16
1012.06	1012	0.06
1013.04	1013	0.04
1013.18	1013	0.18
1012.89	1013	-0.11
1013.20	1013	0.20
1013.44	1013	0.44
1013.81	1014	-0.19
1014.19	1014	0.19
1015.96	1016	-0.04
1016.23	1016	0.23
1015.64	1015	0.64
1015.23	1015	0.23
1012.87	1013	-0.13
1013.63	1013	0.63

Average 0.14

Calibrated by:
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 122/24

13 March, 2024

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	mmHg
757.25	757	0.25
757.15	757	0.15
757.64	758	-0.36
758.27	758	0.27
758.66	759	-0.34
758.94	759	-0.06
759.11	759	0.11
759.84	760	-0.16
759.95	760	-0.05
759.73	760	-0.27
759.96	760	-0.04
760.14	760	0.14
760.42	760	0.42
760.70	761	-0.30
762.03	762	0.03
762.24	762	0.24
761.79	762	-0.21
761.48	762	-0.52
759.71	760	-0.29
760.28	760	0.28

Average 0.03

Calibrated by:
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม



THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

The Result of Calibration

Certification No. 122/24

13 March, 2024

Page : 5 of 5

Standard Temp.	Temperature Sensor Reading	
	Reading	Correction
°C	°C	°C
45.1	45	0.1
30.2	30	0.2
15.4	15	0.4

Calibrated by:
Mr. Watcharapol Subwat
Mechanical Engineer

Calibration & Test Section
Meteorological Instruments Bureau

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING
CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Prakanong, Bangkok 10260

Certificate No : 23-ACT-118
Request No : Req-2023-1547

Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 2
Manufacturer : LARSON DAVIS Range : 94 , 114 dB / 1000 Hz
Model : CAL150 Instrument Status : Used
Serial Number : 6171
ID : UAE.EFM.117/2562

Calibration Environment and Details


Temperature : (23 ±2 °C)
Humidity : (50 ± 20 %RH)
Barometric Pressure : (1013 ±10.0 hPa)
Received Date : 21 July 2023
Calibration Date : 4 August 2023
Location of Calibration : LAB 1 Acoustic
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEL	31 May 2024
THD Multimeter	2015	1047765	NIMT	31 January 2024

Traceability : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k=2, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Service Calibration Engineer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor
Issue Date : 4 August 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-1-1-12-Rev.01 Issue Date: 01/07/21

เอกสารไม่ควบคุม

Certificate No : 23-ACT-118
Request No : Req-2023-1547

Sound pressure level

Calibration Results : Without Adjustment

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty (± dB)	Acceptance limit Class 2 (± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	94.14	0.14	-	-	0.13	0.40
114 dB / 1000 Hz	114.15	0.15	-	-	0.13	0.40

Frequency of Sound pressure level

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 2 (± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7
114 dB / 1000 Hz	1000.00	0.00	-	-	0.01	1.7

Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty (± %)	Acceptance limit Class 2 (± %)
	Measured (%)		Measured (%)			
94 dB / 1000 Hz	0.04		-		0.40	3.0
114 dB / 1000 Hz	0.20		-		0.40	3.0

Note :

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

End of Calibration

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-1-1-12-Rev.01 Issue Date: 01/07/21

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok
10260

Certificate No : 23-SLM-210
Request No : Req-2023-1387

Unit Under Calibration Details

Measurement item : Sound Level Meter Microphone Class : 2
Manufacturer : LARSON DAVIS Microphone Model : 375A04
Model : LXT2 Microphone S/N : 346386
Serial Number : 0005293 Preamplifier Model : PRMLxT2B
ID : UAE.EFM.108/2562 Preamplifier S/N : 056084
Resolution : 0.1 dB Instrument Status : Used


Calibration Environment and Details


Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 21 June 2023
Calibrated Date : 23 June 2023
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	29 June 2023	TSI
Audio Generator	Svante	Svan401	131	12 October 2023	WK Electric

Note
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor k = 2, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Calibration Officer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor
Issue Date : 23 June 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

Certificate No : 23-SLM-210
Request No : Req-2023-1387

1. Indication at the calibration check frequency

UUC Setting FAST / A / 37-139	Nominal Level (dB)	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)		
1000 Hz 114 dB	114.54	114.5	-0.04	114.5	-0.04	0.2	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand 3M, Model AC-300, SN: AC-300001087

2. Self-generated noise, Microphone installed

UUC Setting FAST / 37-139	Measured (dB)	UNCERTAINTY (± dB)
UUC Weighting A	24.1	0.1

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting FAST / 37-139	Measured (dB)	UNCERTAINTY (± dB)
UUC Weighting A	23.5	0.1
C	23.0	0.1
Z	27.5	0.1

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting FAST / 37-139	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)		
STD Setting 125 Hz	0.0	0.1	0.1	0.6	2.0
1000 Hz	0.0	0.0	0.0	0.6	1.0
4000 Hz	0.0	0.0	0.1	0.6	3.0
8000 Hz	-0.6	-0.6	-0.5	0.7	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
เอกสารไม่ควบคุม

Certificate No : 23-SLM-210
Request No : Req-2023-1387

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

Electrical signal test frequency weightings, weighting network response with relative to 1 kHz				UNCERTAINTY (± dB)	Acceptance Limit (± dB)
UUC Setting	Deviation from various Frequency				
FAST / 37-139	Weighting Response curve				
STD Setting	A (dB)	C (dB)	Z (dB)	0.2	2.0
63 Hz	-0.2	-0.1	-0.1		1.5
125 Hz	-0.1	0.0	-0.1		1.5
250 Hz	-0.1	-0.1	-0.1		1.5
500 Hz	-0.1	0.0	-0.1		1.0
1000 Hz	0.0	0.0	-0.1		2.0
2000 Hz	0.0	0.0	0.0		3.0
4000 Hz	0.0	0.0	0.0		5
8000 Hz	-0.1	-0.1	0.0		+5, -INF
16000 Hz	-0.1	-0.1	-0.1		

6. Frequency and time weightings at 1kHz

UUC Setting	STD FAST / 37-139	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)		
UUC Weighting	REF (dB)	UUC (dB)	ERR (dB)	0.2	0.2
A	114.00	114.0	0.0		
C	114.00	114.0	0.0		
Z	114.00	114.0	0.0		

UUC Setting	STD 37-139 / A	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)		
UUC Time Response	REF (dB)	UUC (dB)	ERR (dB)	0.2	0.1
Fast	114.00	114.0	0.0		
Slow	114.00	114.0	0.0		
Leq	114.00	114.0	0.0		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-210
Request No : Req-2023-1387

9. Level linearity including the level range control

UUC Setting	STD FAST / A	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)		
UUC Range	REF (dB)	UUC (dB)	ERR (dB)	0.3	1.1
37-139	39.3	39.5	0.2		
	114	114.0	0.0		

10. Tone burst response

UUC Setting	STD A / 37-139	Toneburst (ms)	Anticipated Ref (dB)	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
				UUC (dB)	ERR (dB)		
UUC Time Response						0.2	1
Fast	200	135.0	135.0	0.0			
	2	118.0	117.9	-0.1			
	0.25	109.0	108.6	-0.4			
Slow	200	128.6	128.5	-0.1			
	2	109.0	108.9	-0.1			
	200	129.0	129.0	0.0			
SEL	2	109.0	109.1	+0.1			
	0.25	100.0	99.8	-0.2			

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance
FAST / C / 95-142	REF	UUC	ERR		Limit
STD Setting (dB)	(dB)				(± dB)
Complete cycle	137.4	136.6	-0.80	0.2	3.0
Positive half cycle	136.4	136.2	-0.20		2.0
Negative half cycle	136.4	136.2	-0.20		2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-210
Request No : Req-2023-1387

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC (dB)		
STD Setting	(dB)	0.1	0.3
Initial	114.0		
Final	114.0		
Deviated	0.0		

8. Level linearity on the reference level range

UUC Setting	Anticipated FAST / A / 37-139	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		REF (dB)	UUC (dB)	ERR (dB)	
STD dB	(dB)	UUC (dB)	ERR (dB)	0.3	1.1
139.00	139	139.0	0.0		
134.00	134	134.0	0.0		
129.00	129	129.0	0.0		
124.00	124	124.0	0.0		
119.00	119	119.0	0.0		
114.00	114	114.0	0.0		
109.00	109	109.0	0.0		
104.00	104	104.0	0.0		
99.00	99	99.0	0.0		
94.00	94	93.9	-0.1		
89.00	89	88.9	-0.1		
84.00	84	83.9	-0.1		
79.00	79	78.9	-0.1		
74.00	74	73.9	-0.1		
69.00	69	68.9	-0.1		
64.00	64	63.9	-0.1		
59.00	59	58.9	-0.1		
54.00	54	53.9	-0.1		
49.00	49	49.0	0.0		
44.00	44	44.0	0.0		
39.00	39	39.1	0.1		
34.00	34	34.4	0.4		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-210
Request No : Req-2023-1387

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC (dB)		
STD Setting	(dB)	0.2	1.5
Positive one-half cycle	142.5		
Negative one-half cycle	142.7		
Deviated	-0.2	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC (dB)		
STD Setting	(dB)	0.1	0.3
Initial	138.0		
Final	138.0		
Deviated	0.0		

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate of Calibration

Customer
Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 23-SLM-222
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok Request No : Req-2023-1410
10260

Unit Under Calibration Details

Measurement item : Sound Level Meter Microphone Class : 2
Manufacturer : LARSON DAVIS Microphone Model : 375B02
Model : LxT2 Microphone S/N : 011736
Serial Number : 0005294 Preamplifier Model : PRMLxT2B
ID : UAE.EFM.109/2562 Preamplifier S/N : 056083
Resolution : 0.1 dB Instrument Status : Used


Calibration Environment and Details


Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 26 June 2023
Calibrated Date : 28 June 2023
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	29 June 2023	TSI
Audio Generator	Svante	Svan401	131	12 October 2023	WK Electric

Note
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangari
Calibration Officer

Approved By : 
Mr. Paet Mathavorn
Calibration Engineer Supervisor
Issue Date : 28 June 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

1. Indication at the calibration check frequency

UUC Setting	Nominal Level	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)		
FAST / A / 37-139							
Calibrator Setting							
1000 Hz 114 dB	113.77	114.0	+0.23	113.8	+0.03	0.2	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 73246

2. Self-generated noise, Microphone installed

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	30.5	0.1

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured (dB)	UNCERTAINTY (± dB)
FAST / 37-139		
UUC Weighting		
A	30.0	0.1
C	29.6	0.1
Z	33.8	0.1

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)		
FAST / 37-139					
STD Setting					
125 Hz	0.1	0.1	0.1	0.6	2.0
1000 Hz	0.0	0.0	0.0	0.6	1.0
4000 Hz	1.1	1.1	1.1	0.6	3.0
8000 Hz	2.7	2.7	2.7	0.7	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)		
FAST / 37-139					
STD Setting					
63 Hz	-0.1	0.0	0.0	0.2	2.0
125 Hz	-0.1	0.1	0.0		1.5
250 Hz	0.0	0.0	0.0		1.5
500 Hz	0.0	0.1	0.0		1.5
1000 Hz	0.0	0.0	0.0		1.0
2000 Hz	0.1	0.1	0.0		2.0
4000 Hz	0.0	0.0	0.0		3.0
8000 Hz	0.0	0.0	0.1		5
16000 Hz	0.0	-0.1	-0.1		+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD REF (dB)	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)		
FAST / 37-139					
UUC Weighting					
A	114.00	114.0	0.0	0.2	0.2
C	114.00	114.0	0.0		0.2
Z	114.00	114.0	0.0		0.2

UUC Setting	STD REF (dB)	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)		
37-139 / A					
UUC Time Response					
Fast	114.00	114.0	0.0	0.2	0.1
Slow	114.00	114.0	0.0		0.1
Leq	114.00	114.0	0.0		0.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC (dB)		
STD Setting			
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting	Anticipated REF (dB)	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC (dB)	UUC (dB)	ERR (dB)		
STD dB					
143.00	143	142.9	-0.1	0.3	0.8
139.00	139	139.0	0.0		1.1
134.00	134	134.0	0.0		1.1
129.00	129	129.0	0.0		1.1
124.00	124	124.0	0.0		1.1
119.00	119	119.0	0.0		1.1
114.00	114	114.0	0.0		1.1
109.00	109	109.0	0.0		1.1
104.00	104	104.0	0.0		1.1
99.00	99	99.0	0.0		1.1
94.00	94	94.0	0.0		1.1
89.00	89	89.0	0.0		1.1
84.00	84	84.0	0.0		1.1
79.00	79	79.0	0.0		1.1
74.00	74	74.0	0.0		1.1
69.00	69	69.0	0.0		1.1
64.00	64	64.0	0.0		1.1
59.00	59	59.0	0.0		1.1
54.00	54	54.0	0.0		1.1
49.00	49	49.1	0.1		1.1
44.00	44	44.2	0.2		1.1
43.00	43	43.2	0.2		1.1
42.00	42	42.4	0.4		1.1
41.00	41	41.3	0.3		1.1
40.00	40	40.5	0.5		1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / A	REF	UUC	ERR		
UUC Range	(dB)	(dB)	(dB)		
37-139	45.4	45.6	0.2	0.3	1.1
	114	114.0	0.0		1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
A / 37-139	Toneburst (ms)	Ref (dB)	UUC (dB)	ERR (dB)		
UUC Time Response						
Fast	200	135.0	135.0	0.0	0.2	1
	2	118.0	117.6	-0.4		+1.0, -2.5
	0.25	109.0	108.5	-0.5		+1.5, -5.0
Slow	200	128.6	128.5	-0.1		1
	2	109.0	108.9	-0.1		+1.0, -5.0
	200	129.0	129.0	0.0		1
SEL	2	109.0	108.9	-0.1	0.2	+1.0, -2.5
	0.25	100.0	99.7	-0.3		+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / C / 95-142	REF (dB)	UUC (dB)	ERR (dB)		
STD Setting	(dB)	(dB)	(dB)		
Complete cycle	137.4	136.7	-0.70	0.2	3.0
Positive half cycle	136.4	136.2	-0.20		2.0
Negative half cycle	136.4	136.2	-0.20		2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-222
Request No : Req-2023-1410

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / A / 37-139	UUC (dB)		
STD Setting	(dB)		
Positive one-half cycle	144.5		
Negative one-half cycle	144.5		
Deviated	0.0	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / A / 37-139	UUC (dB)		
STD Setting	(dB)		
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 23-SLM-209
Address : 81 Soi Udonsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok Request No : Req-2023-1386
10260

Unit Under Calibration Details

Measurement item : Sound Level Meter Microphone Class : 2
Manufacturer : LARSON DAVIS Microphone Model : 375B02
Model : LxT2 Microphone S/N : 011739
Serial Number : 0005296 Preamplifier Model : PRMLxT2B
ID : UAE.EFM.111/2562 Preamplifier S/N : 056086
Resolution : 0.1 dB Instrument Status : Used


Calibration Environment and Details


Temperature : $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$
Humidity : $50\% \text{RH} \pm 20\% \text{RH}$
Barometric Pressure : $1013 \text{ hPa} \pm 10 \text{ hPa}$
Received Date : 21 June 2023
Calibrated Date : 23 June 2023
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3: 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	29 June 2023	TSI
Audio Generator	Svante	Svan401	131	12 October 2023	WK Electric

Note
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Calibration Officer

Approved By : 
Mr. Pait Mathavorn
Calibration Engineer Supervisor
Issue Date : 23 June 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-209
Request No : Req-2023-1386

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / A / 37-139	Level (dB)	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)		
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)		
1000 Hz 114 dB	114.54	114.6	+0.06	114.5	-0.04	0.2	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand 3M, Model AC-300, SN. AC-300001087

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(\pm dB)
UUC Weighting	(dB)	(\pm dB)
A	29.9	0.1

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139	(dB)	(\pm dB)
UUC Weighting	(dB)	(\pm dB)
A	29.7	0.1
C	29.0	0.1
Z	33.4	0.1

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Responce curve			UNCERTAINTY (\pm dB)	Acceptance Limit (\pm dB)
FAST / 37-139	A (dB)	C (dB)	Z (dB)		
STD Setting	(dB)	(dB)	(dB)		
125 Hz	0.1	0.1	0.1	0.6	2.0
1000 Hz	0.0	0.0	0.0	0.6	1.0
4000 Hz	1.0	1.0	1.0	0.6	3.0
8000 Hz	2.0	1.9	2.0	0.7	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-209
Request No : Req-2023-1386

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	FAST / 37-139				
STD Setting	A (dB)	C (dB)	Z (dB)		
63 Hz	-0.2	-0.1	-0.1	0.2	2.0
125 Hz	-0.1	0.0	-0.1		1.5
250 Hz	-0.1	-0.1	-0.1		1.5
500 Hz	-0.1	0.0	-0.1		1.5
1000 Hz	0.0	0.0	-0.1		1.0
2000 Hz	0.0	0.0	0.0		2.0
4000 Hz	0.0	0.0	0.0		3.0
8000 Hz	-0.1	-0.1	0.0		5
16000 Hz	-0.1	-0.1	-0.1		+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	REF	UUC	ERR		
FAST / 37-139	REF	UUC	ERR	0.2	0.2
UUC Weighting	(dB)	(dB)	(dB)		
A	114.00	114.0	0.0		
C	114.00	114.0	0.0		
Z	114.00	114.0	0.0	0.2	0.2

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	REF	UUC	ERR		
37-139 / A	REF	UUC	ERR	0.2	0.1
UUC Time Response	(dB)	(dB)	(dB)		
Fast	114.00	114.0	0.0		
Slow	114.00	114.0	0.0		
Leq	114.00	114.0	0.0	0.2	0.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-209
Request No : Req-2023-1386

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)
STD Setting	(dB)		
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	REF	UUC	ERR		
STD dB	(dB)	(dB)	(dB)	0.3	1.1
139.00	139	139.0	0.0		
134.00	134	134.0	0.0		
129.00	129	129.0	0.0		
124.00	124	124.0	0.0		
119.00	119	119.0	0.0		
114.00	114	114.0	0.0		
109.00	109	109.0	0.0		
104.00	104	104.0	0.0		
99.00	99	99.0	0.0		
94.00	94	94.0	0.0		
89.00	89	89.0	0.0		
84.00	84	84.0	0.0		
79.00	79	79.0	0.0		
74.00	74	74.0	0.0		
69.00	69	69.0	0.0		
64.00	64	64.0	0.0		
59.00	59	59.0	0.0		
54.00	54	54.1	0.1		
49.00	49	49.1	0.1		
44.00	44	44.2	0.2		
39.00	39	39.5	0.5		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-209
Request No : Req-2023-1386

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A	REF	UUC	ERR		
UUC Range	(dB)	(dB)	(dB)	0.3	1.1
37-139	44.7	44.8	0.1		
	114	114.0	0.0		

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
A / 37-139	Toneburst	Ref	UUC	ERR		
UUC Time Response	(ms)	(dB)	(dB)	(dB)	0.2	+1.0, -2.5
Fast	200	135.0	134.9	-0.1		
	2	118.0	117.6	-0.4		
	0.25	109.0	108.6	-0.4		
Slow	200	128.6	128.4	-0.2		
	2	109.0	108.8	-0.2		
	200	129.0	129.0	0.0		
SEL	2	109.0	108.8	-0.2		
	0.25	100.0	99.8	-0.2		

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / C / 95-142	REF	UUC	ERR		
STD Setting	(dB)	(dB)	(dB)	0.2	2.0
Complete cycle	137.4	136.8	-0.60		
Positive half cycle	136.4	136.2	-0.20		
Negative half cycle	136.4	136.2	-0.20		

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-209
Request No : Req-2023-1386

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)
STD Setting	(dB)		
Positive one-half cycle	143.8		
Negative one-half cycle	143.9		
Deviated	-0.1	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC	(± dB)	Limit (± dB)
STD Setting	(dB)		
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate of Calibration

Customer
Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 23-SLM-225
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok Request No : Req-2023-1413
10260

Unit Under Calibration Details

Measurement item : Sound Level Meter Microphone Class : 2
Manufacturer : LARSON DAVIS Microphone Model : 375B02
Model : LxT2 Microphone S/N : 011769
Serial Number : 0005305 Preamplifier Model : PRMLXT2B
ID : UAEEFM.116/2562 Preamplifier S/N : 056100
Resolution : 0.1 dB Instrument Status : Used


Calibration Environment and Details


Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 26 June 2023
Calibrated Date : 28 June 2023
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic

Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	29 June 2023	TSI
Audio Generator	Svanck	Svan401	131	12 October 2023	WK Electric

Note
The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangrat
Calibration Officer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor
Issue Date : 28 June 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-225
Request No : Req-2023-1413

1. Indication at the calibration check frequency

UUC Setting FAST / A / 37-139	Nominal Level	Before Adjust		After Adjust		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	(dB)	UUC (dB)	ERR (dB)	UUC (dB)	ERR (dB)		
1000 Hz 114 dB	113.77	114.0	+0.23	113.8	+0.03	0.2	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 73246

2. Self-generated noise, Microphone installed

UUC Setting FAST / 37-139	Measured	UNCERTAINTY
UUC Weighting	(dB)	(± dB)
A	30.9	0.1

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting FAST / 37-139	Measured	UNCERTAINTY
UUC Weighting	(dB)	(± dB)
A	30.6	0.1
C	30.1	0.1
Z	34.5	0.1

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting FAST / 37-139	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)		
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)
125 Hz	0.0	0.1	0.0	0.6	2.0
1000 Hz	0.0	0.0	0.0	0.6	1.0
4000 Hz	1.0	1.1	1.0	0.6	3.0
8000 Hz	2.1	2.1	2.1	0.7	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-225
Request No : Req-2023-1413

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting FAST / 37-139	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)		
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)
63 Hz	-0.2	0.0	0.0	0.2	2.0
125 Hz	-0.1	0.0	0.0		1.5
250 Hz	-0.1	0.0	0.0		1.5
500 Hz	-0.1	0.0	0.0		1.5
1000 Hz	0.0	0.0	0.0		1.0
2000 Hz	0.0	0.0	0.0		2.0
4000 Hz	0.0	0.0	0.0		3.0
8000 Hz	0.0	0.0	0.0		5
16000 Hz	-0.1	-0.1	-0.1		+5, -INF.

6. Frequency and time weightings at 1kHz

UUC Setting FAST / 37-139	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	REF	UUC	ERR		
UUC Weighting	(dB)	(dB)	(dB)	(± dB)	(± dB)
A	114.00	114.0	0.0	0.2	0.2
C	114.00	114.0	0.0		0.2
Z	114.00	114.0	0.0		0.2

UUC Setting 37-139 / A	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	REF	UUC	ERR		
UUC Time Response	(dB)	(dB)	(dB)	(± dB)	(± dB)
Fast	114.00	114.0	0.0	0.2	0.1
Slow	114.00	114.0	0.0		0.1
Leq	114.00	114.0	0.0		0.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-225
Request No : Req-2023-1413

7. Long Term Stability

UUC Setting FAST / A / 37-139	Measured UUC	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
STD Setting	(dB)		
Initial	114.0		
Final	114.0		
Deviated	0.0	0.1	0.3

8. Level linearity on the reference level range

UUC Setting FAST / A / 37-139	Anticipated REF	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
STD dB	(dB)	UUC (dB)	ERR (dB)		
143.00	143	143.0	0.0	0.3	0.8
139.00	139	139.0	0.0		1.1
134.00	134	134.0	0.0		1.1
129.00	129	129.0	0.0		1.1
124.00	124	124.0	0.0		1.1
119.00	119	119.0	0.0		1.1
114.00	114	114.0	0.0		1.1
109.00	109	109.0	0.0		1.1
104.00	104	104.0	0.0		1.1
99.00	99	98.9	-0.1		1.1
94.00	94	94.0	0.0		1.1
89.00	89	89.0	0.0		1.1
84.00	84	84.0	0.0		1.1
79.00	79	79.0	0.0		1.1
74.00	74	74.0	0.0		1.1
69.00	69	69.0	0.0		1.1
64.00	64	64.0	0.0		1.1
59.00	59	59.0	0.0		1.1
54.00	54	54.0	0.0		1.1
49.00	49	49.1	0.1	0.3	1.1
44.00	44	44.2	0.2		1.1
43.00	43	43.2	0.2		1.1
42.00	42	42.3	0.3		1.1
41.00	41	41.4	0.4		1.1
40.00	40	40.5	0.5		1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-225
Request No : Req-2023-1413

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY	Acceptance
FAST / A	REF	UUC	ERR		Limit
UUC Range	(dB)	(dB)	(dB)	(± dB)	(± dB)
37-139	45.9	46.0	0.1	0.3	1.1
	114	114.0	0.0		1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY	Acceptance
A / 37-139	Toneburst	Ref	UUC	ERR		Limit
UUC Time Response	(ms)	(dB)	(dB)	(dB)	(± dB)	(± dB)
Fast	200	135.0	134.9	-0.1	0.2	1
	2	118.0	117.8	-0.2		+1.0, -2.5
	0.25	109.0	108.8	-0.2		+1.5, -5.0
Slow	200	128.6	128.4	-0.2		1
	2	109.0	108.8	-0.2		+1.0, -5.0
	0.25	100.0	100.0	0.0		+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY	Acceptance
FAST / C / 95-142	REF	UUC	ERR		Limit
STD Setting	(dB)	(dB)	(dB)	(± dB)	(± dB)
Complete cycle	137.4	136.8	-0.60	0.2	3.0
Positive half cycle	136.4	136.2	-0.20		2.0
Negative half cycle	136.4	136.2	-0.20		2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-225
Request No : Req-2023-1413

12. Overload indication

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)	(± dB)	(± dB)
Positive one-half cycle	144.9		
Negative one-half cycle	144.8		
Deviated	0.1	0.2	1.5

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY	Acceptance
FAST / A / 37-139	UUC		Limit
STD Setting	(dB)	(± dB)	(± dB)
Initial	138.0		
Final	138.0		
Deviated	0.0	0.1	0.3

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Name UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD. Certificate No : 23-SLM-223
Address 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok Request No : Req-2023-1411
10260

Unit Under Calibration Details

Measurement item : Sound Level Meter Microphone Class : 2
Manufacturer : LARSON DAVIS Microphone Model : 375B02
Model : LxT2 Microphone S/N : 11791
Serial Number : 0005339 Preamplifier Model : PRMLX72B
ID : UAEEFM036/2563 Preamplifier S/N : 056131
Resolution : 0.1 dB Instrument Status : Used

Calibration Environment and Details


Temperature : 23 °C ± 2 °C
Humidity : 50 %RH ± 20 %RH
Barometric Pressure : 1013 hPa ± 10 hPa
Received Date : 26 June 2023
Calibrated Date : 28 June 2023
Calibration Procedure : In-house method CP-SLM-01 based on IEC 61672-3 : 2013 Electroacoustics - Sound level meters - Part 3: Periodic tests
Location of Calibration : Lab Acoustic


Reference Standard

Instrument	Brand	Model	SN.	Due calibration	Traceability
Standard Microphone	GRAS	40AN	188273	6 October 2023	GRAS
Multifrequency Calibrator	Quest	Quest-cal	EFA000234	29 June 2023	TSI
Audio Generator	Svante	Svan401	131	12 October 2023	WK Electric

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibrated By : 
Mr. Noppadon Luangart
Calibration Officer

Approved By : 
Mr. Pacit Mathavorn
Calibration Engineer Supervisor
Issue Date : 28 June 2023

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-223
Request No : Req-2023-1411

1. Indication at the calibration check frequency

UUC Setting	Nominal	Before Adjust		After Adjust		UNCERTAINTY	Acceptance
FAST / A / 37-139	Level	UUC	ERR	UUC	ERR		Limit
Calibrator Setting	(dB)	(dB)	(dB)	(dB)	(dB)	(± dB)	(± dB)
1000 Hz 114 dB	113.77	114.3	+0.53	113.8	+0.03	0.2	0.3

Note : Absolute sensitivity was established by the use of Sound Calibrator Brand SVANTEK, Model SV 35A, SN. 73246

2. Self-generated noise, Microphone installed

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	28.0	0.1

3. Self-generated noise, Microphone replaced by the electrical input signal device

UUC Setting	Measured	UNCERTAINTY
FAST / 37-139		
UUC Weighting	(dB)	(± dB)
A	27.3	0.1
C	27.2	0.1
Z	31.5	0.1

4. Acoustic signal test of frequency weightings (Without Windscreen)

UUC Setting	Deviation from various Frequency Weighting Response curve			UNCERTAINTY	Acceptance
FAST / 37-139	A	C	Z	(± dB)	(± dB)
STD Setting	(dB)	(dB)	(dB)		
125 Hz	1.2	1.3	1.3	0.6	2.0
1000 Hz	0.0	0.0	0.0	0.6	1.0
4000 Hz	0.2	0.2	0.2	0.6	3.0
8000 Hz	0.3	0.3	0.4	0.7	5.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-223
Request No : Req-2023-1411

5. Electrical signal test of frequency weightings, Weighting network response with relative to 1 kHz

UUC Setting FAST / 37-139	Deviation from various Frequency Weighting Response curve			UNCERTAINTY (± dB)	Acceptance Limit (± dB)
	A (dB)	C (dB)	Z (dB)		
STD Setting					
63 Hz	-0.1	0.0	0.0	0.2	2.0
125 Hz	-0.1	0.0	0.0		1.5
250 Hz	-0.1	0.0	0.0		1.5
500 Hz	0.0	0.0	0.0		1.5
1000 Hz	0.0	0.0	0.0		1.0
2000 Hz	0.0	0.1	0.0		2.0
4000 Hz	0.0	0.0	0.0		3.0
8000 Hz	0.0	0.0	0.0		5
16000 Hz	0.0	-0.1	-0.1		+5,-INF.

6. Frequency and time weightings at 1kHz

UUC Setting FAST / 37-139	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)		
UUC Weighting	(dB)	(dB)	(dB)		
A	114.00	114.0	0.0	0.2	0.2
C	114.00	114.0	0.0		0.2
Z	114.00	114.0	0.0		0.2

UUC Setting 37-139 / A	STD REF	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
		UUC (dB)	ERR (dB)		
UUC Time Response	(dB)	(dB)	(dB)		
Fast	114.00	114.0	0.0	0.2	0.1
Slow	114.00	114.0	0.0		0.1
Leq	114.00	114.0	0.0		0.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-223
Request No : Req-2023-1411

7. Long Term Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC		
STD Setting	(dB)		
Initial	114.0	0.1	0.3
Final	114.0		
Deviated	0.0		

8. Level linearity on the reference level range

UUC Setting	Anticipated	Deviation		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	REF	UUC	ERR		
STD dB	(dB)	(dB)	(dB)		
140.00	140	139.9	-0.1	0.3	0.8
139.00	139	139.0	0.0		1.1
134.00	134	134.0	0.0		1.1
129.00	129	129.0	0.0		1.1
124.00	124	124.0	0.0		1.1
119.00	119	119.0	0.0		1.1
114.00	114	114.0	0.0		1.1
109.00	109	109.0	0.0		1.1
104.00	104	104.0	0.0		1.1
99.00	99	99.0	0.0		1.1
94.00	94	94.0	0.0		1.1
89.00	89	89.0	0.0		1.1
84.00	84	84.0	0.0		1.1
79.00	79	79.0	0.0		1.1
74.00	74	74.0	0.0		1.1
69.00	69	69.0	0.0		1.1
64.00	64	64.0	0.0		1.1
59.00	59	59.0	0.0		1.1
54.00	54	54.0	0.0		1.1
49.00	49	49.0	0.0		1.1
44.00	44	44.1	0.1		1.1
39.00	39	39.3	0.3		1.1
38.00	38	38.4	0.4		1.1
37.00	37	37.5	0.5		1.1

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-223
Request No : Req-2023-1411

9. Level linearity including the level range control

UUC Setting	STD	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A	REF	UUC	ERR		
UUC Range	(dB)	(dB)	(dB)		
37-139	42.5	42.6	0.1	0.3	1.1
	114	114.0	0.0		1.1

10. Tone burst response

UUC Setting	STD	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
A / 37-139	Toneburst	Ref	UUC	ERR		
UUC Time Response	(ms)	(dB)	(dB)	(dB)		
Fast	200	135.0	134.9	-0.1	0.2	1
	2	118.0	117.6	-0.4		+1.0, -2.5
	0.25	109.0	108.6	-0.4		+1.5, -5.0
Slow	200	128.6	128.5	-0.1		1
	2	109.0	108.8	-0.2		+1.0, -5.0
	200	129.0	129.0	0.0		1
SEL	2	109.0	109.0	0.0		+1.0, -2.5
	0.25	100.0	99.8	-0.2		+1.5, -5.0

11. Peak C Sound level

UUC Setting	Anticipated	Measured		UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / C / 95-142	REF	UUC	ERR		
STD Setting	(dB)	(dB)	(dB)		
Complete cycle	137.4	136.8	-0.60	0.2	3.0
Positive half cycle	136.4	136.2	-0.20		2.0
Negative half cycle	136.4	136.2	-0.20		2.0

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

Certificate No : 23-SLM-223
Request No : Req-2023-1411

12. Overload indication

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC		
STD Setting	(dB)		
Positive one-half cycle	141.4	0.2	1.5
Negative one-half cycle	141.5		
Deviated	-0.1		

13. High Level Stability

UUC Setting	Measured	UNCERTAINTY (± dB)	Acceptance Limit (± dB)
FAST / A / 37-139	UUC		
STD Setting	(dB)		
Initial	138.0	0.1	0.3
Final	138.0		
Deviated	0.0		

End of Certificate

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

เอกสารไม่ควบคุม

List of Instruments Certification for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Equipment for Air Quality Analysis									
1	Analytical Balance (Readability 0.1 mg)	ฝุ่นละอองขนาดไม่เกิน 10 ไมครอน (PM10)	Mettler-Toledo	MS204TS/00 C252436235	National Food Institute, Ministry of Industry, Thailand	2402420-003-01	19 Apr 24	18 Apr 25	-
Equipment for Water Quality Analysis									
2	pH Meter	pH	Mettler-Toledo	Seven Easy S20 / 1230525212	DKSH (Thailand) Ltd.	C07240167	9 Apr 24	8 Apr 25	-
3	Analytical Balance (Readability 0.01 mg)	SS TDS	Mettler-Toledo	XSR205DU / C210685394	National Food Institute, Ministry of Industry, Thailand	2402283-002-01	2 Apr 24	1 Apr 25	-
4	Hot Air Oven		Memmert	UF55 / B216.1666	National Food Institute, Ministry of Industry, Thailand	2400141-001-01	11 Oct 23	10 Oct 24	-
5	Analytical Balance (Readability 0.1 mg)	Oil&Grease	Mettler-Toledo	AB-204S/FACT / 1129361010	Technology Promotion Association (Thailand-Japan)	24MM292	11 May 24	10 May 25	-
6	Digestor Unit	TKN	FOSS TECATOR	DT2520 / 91794469	FOSS South East Asia	9809	8 Feb 24	7 Feb 25	-
7	Distillation Unit (Kjeldahl Method)		FOSS TECATOR	KT200 / 91790524	FOSS South East Asia	9810	9 Feb 24	7 Feb 25	-
8	BOD Incubator	BOD	Arco	UC4-1320 / (UAE.WAO.015/2561)	Technology Promotion Association (Thailand-Japan)	24TM303	10 Feb 24	9 Feb 25	-
9	DO Meter		YSI	5100 / 11B101863	Technology Promotion Association (Thailand-Japan)	24TW39	21 Feb 24	20 Feb 25	-

List of Instruments Certification for Environmental Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Equipment for Water Quality Analysis									
10	Incubator	TCB	Memmert	IPP 260 / V616.0066	Technology Promotion Association (Thailand-Japan)	24TM650	2 Apr 24	1 Apr 25	-
11	Water Bath		Memmert	WNE 14 / L416.0606	Technology Promotion Association (Thailand-Japan)	24TM29	10 Feb 24	8 Feb 25	-
12	Auto Clave		ALP	CL-40L / 808763	National Food Institute, Ministry of Industry, Thailand	2402281-001-01	2 Apr 24	1 Apr 25	-
13	Analytical Balance		OHAUS	PX623 / C236754745	DKSH (Thailand) Ltd.	C01234158	7 Dec 23	6 Dec 24	-

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

Calibration Certificate

Certificate No.: 2402420-003-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakanong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Serial No.: C252436235
ID No.: UAE.AIR.023/2566
Order No.: 2402420
Operation No.: 2402420-003
Date of Receipt: 19 April 2024
Date of Calibration: 19 April 2024

Calibrated by Mr.Pheraphat Tuanjit
Scientist
Approved by P. Jungsakulit
(Miss Preeyaporn Jaengkarnkit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team
Date of Issue: 23 April 2024

The uncertainties are for a confidence probability of approximately 95%
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-003-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Serial No.: C252436235
Capacity: 220 g
Resolution: 0.0001 g
ID No.: UAE.AIR.023/2566

Page 2 of 3

Date of Calibration: 19 April 2024

Environment Condition: Ambient Temperature: 21.7 ± 1.5 °C Relative Humidity: 65 ± 6.7 %
Place of Calibration: Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M23111815	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M23111825	28 November 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
100	0.000074
200	0.000074

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.0005	100.0006	100.0003	100.0006	100.0003	100.0005	0.0002

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-003-01
Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: MS204TS/00
Serial No.: C252436235
Capacity: 220 g
Resolution: 0.0001 g
ID No.: UAE.AIR.023/2566

Date of Calibration: 19 April 2024 Page 3 of 3

Calibration Results: (Continued)

Calibration Range: 0-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000094	2.00
0.1	0.10000	0.1000	0.0000	0.000094	2.00
1	0.99998	1.0000	0.0000	0.000097	2.00
5	4.99997	5.0000	0.0000	0.000096	2.00
10	10.00002	10.0000	0.0000	0.00012	2.00
20	20.00003	20.0001	-0.0001	0.00014	2.00
50	49.99998	50.0003	-0.0003	0.00012	2.00
70	70.00000	70.0005	-0.0005	0.00017	2.00
100	99.99997	100.0006	-0.0006	0.00017	2.00
150	149.99994	150.0012	-0.0013	0.00022	2.00
200	200.00001	200.0015	-0.0015	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

Certificate of Calibration

Equipment: pH METER
Model: SevenEasy
Serial No. (or ID.): 1230525212 (UAE.WAS.003/2553)
Manufacturer: METTLER TOLEDO
Electrode Serial No.: 1156883
Condition: In Condition
Certificate No.: C07240167
Issued Date: 9 April 2024
Job No.: WO-0002408
Page: 1 of 3
Model: InLab Solids Brand: METTLER TOLEDO

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udomsuk 41 Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature 23 °C ± 2 °C
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited.
2533 Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Miss.Orawan Khlaiphloi
Calibration Date: 9 April 2024
The Method used: In house method, CAL-WI-58, base on ASTM E 70-07
Traceability: This certificate is traceable to SI Units, Sample Test is assured through primary measurement method Harned cell, through CPAchem Ltd. (ISO/IEC 17034) Certificate No. 938377, 931985, 931984 And pH Scale traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Industrial Foundation Electrical and Electronics Institute Certificate No. CA20230350EA

Orawan Khlaiphloi
(Miss Orawan Khlaiphloi)
Person in charge

Nitinun Srihawan
(Mr. Nitinun Srihawan)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

Calibration Results:

pH Scale

Input (mV)	pH Meter Reading			Uncertainty of Measurement (mV)	Coverage Factor (k)
	(mV)	Error (mV)	(pH)		
414.12	414	-0.12	0.00	0.58	2.00
354.96	355	0.04	1.00	0.58	2.00
295.8	296	0.20	2.00	0.58	2.00
236.64	237	0.36	3.00	0.58	2.00
177.48	178	0.52	4.00	0.58	2.00
118.32	118	-0.32	5.00	0.58	2.00
59.16	59	-0.16	6.00	0.58	2.00
0	0	0.00	7.00	0.58	2.00
-59.16	-59	0.16	8.00	0.58	2.00
-118.32	-118	0.32	9.00	0.58	2.00
-177.48	-177	0.48	10.00	0.58	2.00
-236.64	-236	0.64	11.00	0.58	2.00
-295.8	-296	-0.20	12.00	0.58	2.00
-354.96	-355	-0.04	13.00	0.58	2.00
-414.12	-414	0.12	14.00	0.58	2.00

Practical slope and zero point*

The three-point calibration using three standard buffer solutions; pH 4.008 , pH 6.985 and pH 9.997

-During calibration, display of pH meter reading; pH 4.00 , pH 7.00 and pH 10.01

The practical slope of the pH electrode; 57.01 (mV/pH), 96.37%

The zero point of the pH electrode; 6.88 (pH)

Sample Test Results

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Uncertainty of Measurement (pH)	Coverage Factor (k)
4.008	3.99	-0.018	0.0070	2.00
6.985	7.00	0.015	0.0091	2.00
9.997	10.02	0.023	0.0074	2.00

* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

The End of Certificate



Certificate of Calibration

Equipment:	Digital Thermometer with Probe	Certificate No.: C15240373
Model:	SevenEasy pH	Issued Date: 09 April 2024
Serial No.:	1230525212	Job No.: WO-00024208
Manufacturer:	METTLER TOLEDO	Page: 1 of 2
ID No.:	UAE.WAS.003/2553	Condition: In Condition

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udumsuk 41 Sukhumvit Road,
Bangkok, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature: 22 °C ± 3 °C
Humidity: 50 %RH ± 20 %RH
Voltage: 220 VAC ± 10 %

Calibration Place: Thermo-Hygro Laboratory, DKSH Technology Limited,
2533 Sukhumvit Road, Bangkok,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Mr. Nateekarn Mitjit
Calibration Date: 09 April 2024
The Method used: In house method, CAL-WI-19, by comparison with standard thermometer
Traceability: This certificate is traceable to the International System of Unit maintained by Quality Reborn Co.,Ltd. (QR) Certificate No. QR23-1073

(Mr. Nateekarn Mitjit)

Person in charge

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled.
The report shall not be reproduced except in full without approval of DKSH Technology Limited.

(Mr. Pramote Ramrong)

Authorized signatory

Reference standard equipment:

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR23-1073	2 May 23	2 May 24

Calibration Results:

Without Adjustment

Sensor Type: RTD

Channel: -


Diameter (mm) 4

Length (mm): 135

Immersion (mm): 110

Calibrate Point (°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty (± °C)
15.0	15.010	15.1	-0.090	0.076
25.0	25.006	25.1	-0.094	0.076
35.0	35.004	35.0	0.004	0.076

The End of Certificate

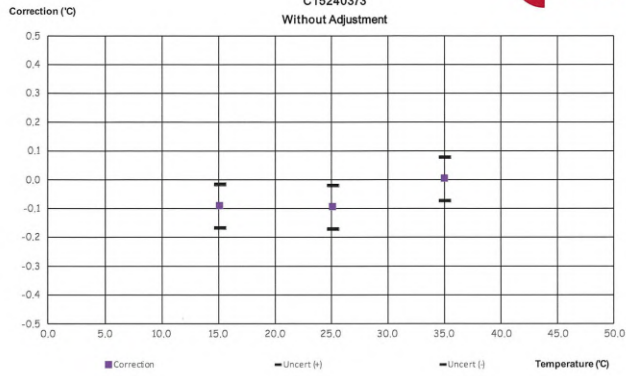

Delivering Growth – in Asia and Beyond.

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2402283-002-01

Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C210685394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024 Page 2 of 4

Environment Condition: Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 47.5 ± 2.5 %

Place of Calibration: Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M23040535	8 April 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 016/23	Quality Reborn	QR24-0343	9 February 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.000042
80	0.000052
100	0.000048
200	0.000048

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100.000	100.0001	99.9999	99.9999	100.0001	100.0000	0.0001

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

Calibration Certificate

Certificate No.: 2402283-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 SOI UDOMSUK 41, SUKHUMVIT ROAD,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C210685394
ID No.: UAE.WAO.010/2565
Order No.: 2402283
Operation No.: 2402283-002
Date of Receipt: 2 April 2024
Date of Calibration: 2 April 2024

Calibrated by Mr.Jerawut Prapawuttipong Scientist
Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 9 April 2024

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402283-002-01

Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C210685394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024 Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0 - 80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 80 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.000000	0.00000	0.00000	0.0000086	2.00
0.001	0.001003	0.00101	-0.00001	0.0000089	2.00
0.005	0.005003	0.00500	0.00000	0.0000092	2.00
0.01	0.010003	0.01000	0.00000	0.0000089	2.00
0.05	0.049996	0.05000	0.00000	0.0000096	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50001	0.00001	0.000014	2.00
1	1.000003	1.00002	-0.00002	0.000016	2.00
2	2.000023	2.00001	0.00001	0.000017	2.00
5	5.000017	5.00002	0.00000	0.000020	2.00
10	10.000009	10.00000	0.00001	0.000026	2.00
20	20.000031	20.00000	0.00003	0.000037	2.00
30	30.000040	30.00001	0.00003	0.000050	2.00
50	50.000028	50.00002	0.00001	0.000068	2.00
80	80.000068	80.00002	0.00005	0.00011	2.00

F-CS-012 Revision: 01 Date: 20-04-65

เอกสารไม่ควบคุม

Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR2050U
Serial No.: C210685394
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.0001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024 Page 4 of 4

Calibration Results: (Continued)

Calibration Range: 81 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 81 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
90	90.00010	90.0001	0.0000	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00015	2.00
110	110.00007	110.0001	0.0000	0.00016	2.00
120	120.00009	120.0000	0.0001	0.00017	2.00
130	130.00010	130.0000	0.0001	0.00019	2.00
140	140.00014	140.0000	0.0001	0.00020	2.00
150	150.00009	150.0001	0.0000	0.00020	2.00
160	160.00010	160.0001	0.0000	0.00022	2.00
170	170.00012	170.0001	0.0000	0.00023	2.00
200	200.00016	200.0002	0.0000	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

***** End *****

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๕๑ ถนนสุขุมวิท 35 แขวงคลองตันใต้ เขตวัฒนา กรุงเทพมหานคร 10700
2008 Soi 35, Aun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel : +66(0) 2422 8688 Fax : +66(0) 2422 8545 nfi.co.th

Calibration Report

Certificate No.: 2400141-001-01
Equipment: CHAMBER (Hot Air Oven)
Model: UF 55
Serial No.: B216.1666
Resolution: 0.1 °C
ID No.: UAE.WAO.027/2559
Manufacturer: MEMMERT

Date of Calibration: 11 October 2023 Page 2 of 3

Location: Laboratory, Floor 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.

Environment Condition:
Ambient Temperature (28 ± 1) °C
Relative Humidity (63 ± 2) %
Line Voltage (228 ± 1) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 9 standard thermometer into its chamber and calibration according to W-TE-014 Based on TLAS G-20-1/02-08 (E): Guidelines for Calibration and Checks of Temperature Controlled Enclosures.
- The temperature scale used was based on ITS - 90.
- All data show below were final values and the initial data may be obtained upon request.

2. Reference Standard Instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date	Through
Digital Thermometer with sensor	34972A	MY49016894	TE 660380-01	22 April 2024	NATIONAL FOOD INSTITUTE
	RTD	CH201-209/ RTD#201-209			

3. This certificate is traceable to International System of Units (SI Units).

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibrated item : Good

UUC Description :

Time of Record 1 Hour 9 Minute At 104.0, 140.0 and 180.0 °C
Fresh air Damper
- Open Position
- X Close
- Not Available

7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๕๑ ถนนสุขุมวิท 35 แขวงคลองตันใต้ เขตวัฒนา กรุงเทพมหานคร 10700
2008 Soi 35, Aun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel : +66(0) 2422 8688 Fax : +66(0) 2422 8545 nfi.co.th

Calibration Certificate

Certificate No.: 2400141-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsak 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: CHAMBER (Hot Air Oven)

Manufacturer: MEMMERT

Model: UF 55

Serial No.: B216.1666

ID No.: UAE.WAO.027/2559

Order No.: 2400141

Operation No.: 2400141-001

Date of Receipt: 11 October 2023

Date of Calibration: 11 October 2023

Calibrated by Mr.Worapob Sooktong
Scientist

Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

Date of Issue: 16 October 2023

The uncertainties are for a confidence probability of approximately 95 %.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 ๒๕๕๑ ถนนสุขุมวิท 35 แขวงคลองตันใต้ เขตวัฒนา กรุงเทพมหานคร 10700
2008 Soi 35, Aun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel : +66(0) 2422 8688 Fax : +66(0) 2422 8545 nfi.co.th

Calibration Report

Certificate No.: 2400141-001-01
Equipment: CHAMBER (Hot Air Oven)
Model: UF 55
Serial No.: B216.1666
Resolution: 0.1 °C
ID No.: UAE.WAO.027/2559
Manufacturer: MEMMERT

Date of Calibration: 11 October 2023 Page 3 of 3

Calibration point: 104.0, 140.0 and 180.0 °C

Calibration result:

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
MIN	28.2	61.4	227.4
MAX	28.3	65.1	229.3

Table 1 : Reporting of Temperature

Calibration point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty ± (°C)
	# 1	# 2	# 3	# 4	# 5	# 6	# 7	# 8	# 9	
104.0	104.05	103.98	104.02	104.08	104.00	104.05	103.99	104.17	104.00	0.53
140.0	140.09	139.99	139.91	140.05	139.99	139.91	139.97	140.26	139.97	0.73
180.0	180.46	180.33	180.25	180.28	180.33	179.96	180.31	180.64	180.16	0.90

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* reading (°C)			Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	MIN	MAX	Average			
104.0	104.0	104.0	104.0	0.090	0.18	0.38
140.0	140.0	140.1	140.0	0.075	0.28	0.47
180.0	180.0	180.1	180.0	0.13	0.48	0.88

Note The quoted uncertainty include " Stability " and " Loading effect (20% of Temp Uniformity) "

UUC* = Unit Under Calibration

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.

Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which is observed at the same time.

Overall Variation = The difference of the maximum and minimum measured temperatures throughout observation time.

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

***** End *****

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๕๑ ถนนสุขุมวิท 35 แขวงคลองตันใต้ เขตวัฒนา กรุงเทพมหานคร 10700
2008 Soi 35, Aun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel : +66(0) 2422 8688 Fax : +66(0) 2422 8545 nfi.co.th



Certificate of Calibration

Cert.No.: 24MM292
Page: 1 of 3

Equipment : Electronic Balance
Manufacturer : Mettler Toledo
Model : AB204-S/FACT
Serial No. : 1129361010
ID No. : UAE.WAS.002/2552
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Balance Room (108)
Received order : 11 May 2024
Calibration Date : 11 May 2024
Ambient Temperature : 15 °C to 40 °C
Relative Humidity : 30 % to 90 %
Calibrated by : Khit Ruttanaprapachai
Approved by :
() Ponpan Palpim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 15 May 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2405-0166OC-1
Procedure used :-

Cert.No.: 24MM292
Page: 2 of 3

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14
according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0013-24	25 Jan 2026

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g Resolution 0.0001 g

Before Adjustment :

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
100	100.0000	0.0000	0.19	2.03
200	200.0006	-0.0006	0.30	2

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)


Applied Weight (g)	Standard Deviation of Reading (g)
100	0.00007
200	0.00005

เอกสารไม่ควบคุม



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2405-0166OC-1
Result of calibration

Cert.No.: 24MM292
Page: 3 of 3



Maximum difference between
off-center and central loading

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)	Maximum difference between off-center and central loading (g)
-0.0004	-0.0004	-0.0003	-0.0003	-0.0004	0.0001

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
Unload	0.0000	0.0000	0.15	2.13
0.01	0.0100	0.0000	0.15	2.13
0.05	0.0500	0.0000	0.15	2.13
0.1	0.1000	0.0000	0.15	2.13
0.5	0.5000	0.0000	0.15	2.13
1	1.0000	0.0000	0.15	2.13
10	10.0000	0.0000	0.15	2.11
50	49.9999	+0.0001	0.17	2.06
100	99.9999	+0.0001	0.19	2.03
150	149.9998	+0.0002	0.29	2
200	199.9990	+0.0010	0.30	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage
factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

FOSS

Customer Service Report

Date: 8 Feb 2024
Customer: UAE
Instrument: DT2520

FOSS South East Asia
3388 Sirinrat Building, 25th - 26th Floor, Unit No. 3388/90,
Rama IV Road, Klongtoey, Bangkok, Thailand 10110

Report No: 9809

Address: BANSONG

Serial: 91794469

Hours
Start
Finish

Travel To Customer
14:00
09:10

Labour
14:00
16:00 2hrs

Travel From Customer
16:00
18:00 2hrs

Application		Special		Standard	
Normal	x	Courtesy Visit	x	Installation	x
Distributor	x	PMA Onboarding	x	Quote	x
Internal	x	Warranty	x	Repair	x
Digital Service	x	Sales Support	x	Remote	x

PO/Quote Number: if applicable

PMA Type: FOSScare if applicable Contract No. if applicable

Details of Work / Test	Condition / Status
H PM DT2520	
- ตรวจสอบสายเคเบิล	
- ตรวจสอบ connection	
- ตรวจสอบ cable kit, temp out out	
- ตรวจสอบ cable kit	
- 30°C - 100°C = 10 min	
- 30°C - 420°C = 37 min	
- Instrument 419.0 tcher = 419.0	

Instrument Ready for Use ☒ OK ☐ Not OK If not OK - Comment

Part No.	Batch	Description	Qty
60079652	23.09.2023	cable kit digitor	1
10013654	03.01.2024	temperature control	1

I confirm this report is accurate and complete
Signed FOSS
Name
Signed Customer
Name
Email

Would you be willing to participate in a brief survey in order to tell us how we performed?

เอกสารไม่ควบคุม

Date: 9 Feb 2024

Customer: UAE

Address: Bangkok

Instrument: KT200

Serial: 91790524

Hours	Travel To Customer	Labour	Travel From Customer
Start	08:00	09:30	14:50
Finish	09:30	12:00	16:30

Application	Special	Job Type	Standard
Normal	Courtesy Visit	Installation	Training
Distributor	PMA Onboarding	Quote	In House
Internal	Warranty	Repair	PM
Digital Service	Sales Support	Remote	Other

PO/Quote Number: - if applicable

PMA Type: FOSSCATE if applicable Contract No. - if applicable

Details of Work / Test	Condition / Status
# PM KT200	
- ตรวจสอบเครื่องวัดอุณหภูมิ	
- ตรวจสอบเครื่องวัดความชื้น	
- ตรวจสอบเครื่องวัดความดัน	
- ตรวจสอบเครื่องวัดความเร็วลม	
- ตรวจสอบเครื่องวัดความถี่	
- ตรวจสอบเครื่องวัดความถี่	
# ตรวจสอบ SOPH Model ตรวจสอบเครื่องวัดอุณหภูมิ	
10000725 SOPH Model Complete 1 PC	

Instrument Ready for Use: ☒ OK ☐ Not OK If not OK - Comment

Part No:	Batch	Description	Qty
10009965	14.12.2020	Foss PM kit let 300 let 300 Analysis E200	1

I confirm this report is accurate and complete	
Signed FOSS	Signed Customer
Name	Name

Would you be willing to participate in a brief survey in order to tell us how we performed? Email

เอกสารไม่ควบคุม



Certificate of Calibration

Equipment : BOD Incubator
Manufacturer : Arco
Model : UC4-1320
Serial No. : 13URC4S013201
ID No. : UAE.WAO.015/2561
Submitted by : United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Lab Floor 2
Received Order : 10 February 2024
Calibration Date : 10 February 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Tawatchai Pama
Approved by :
() Pornthippa Tameyakul
() Unnophol Harachai
() Suwit Imjai

Issue Date : 19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2402-0234OC-1
Result of Calibration : () Without Adjustment
Function of UUC* : Temperature Source
Fresh air setting : Not Available

Cert. No.: 24TM303
Page: 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
20.0	20.1	19.9	0.37	0.72	1.4	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (± °C)
	1	2	3	4	5	6	7	8	9 (ref.)	
20.0	19.873	19.803	20.322	19.690	19.615	19.585	19.612	19.558	19.645	0.58

Average* : The average of 30 values in each position.
Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.
Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.
Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.
UUC* : Unit Under Calibration
Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



Equipment : BOD Incubator
Condition As-Received : Used Item
Reference : 2402-0234OC-1
Procedure Used :-

Cert. No.: 24TM303
Page: 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration


- Reference standard instrument:-
- Instrument Serial No. Cert. No. Traceable Due Date
- 1) Data Acquisition MY59003411 23LM208 TPA 27 Dec 2024
2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certificate is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration : () Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Not Available



Probe Installation Details :

a = 10 cm
b = 10 cm
c = 10 cm

Dimension of Chamber :

D = 0.62 m
W = 1.2 m
H = 1.2 m
Capacity = 0.89 m³

Environment during calibration		
	Beginning	Finished
Temp. (°C)	28	31
REL.Humid. (%)	70	65
AC Supply (Volt)	233	234

Position :	Ref. Std. ID No.:
1	20RTD-2/1
2	20RTD-2/2
3	20RTD-2/3
4	20RTD-2/4
5	20RTD-2/5
6	20RTD-2/6
7	20RTD-2/7
8	20RTD-2/8
9 (ref.)	20RTD-2/9

เอกสารไม่ควบคุม



Cert.No.: 24TW39
Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : YSI
Model : 5100
Serial No. : 11B 101863
ID No. : UAE.WAO.004/2554
Received Date : 20 February 2024
Test Date : 21 February 2024
Reference : 2402-0629DSC-1
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Sirithean
Approved by :
Approved Signatory
() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Saithip Meangmai
Issue Date : 22 February 2024

เอกสารไม่ควบคุม



Cert.No.: 24TW39
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 22B100125

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.19	0.0055

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-

เอกสารไม่ควบคุม



Certificate of Calibration

Cert. No.: 24TM850
Page : 1 of 3

Equipment : Incubator
Manufacturer : Memmert
Model : IPP 260
Serial No. : V616.0066
ID No. : UAE.MIC.032/2559
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : Microbiology Laboratory (302)
Received Order : 01 April 2024
Calibration Date : 02 - 03 April 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
Calibrated by : Man Pattanapongpaiboon
Approved by :
Approved Signatory
() Ponpan Paipim
(✓) Suwit Imjai
() Kunchit Promprat
Issue Date : 7 April 2024

The Uncertainties are for a confidence probability of approximately 95%
This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Incubator
Condition As-Received : Used Item
Reference : 2404-0003OC-2
Procedure Used :-

Cert. No.: 24TM850
Page : 2 of 3

Calibration were conducted using calibration procedure CP-OT02 based on TLAS G-20 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector (RTD).
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49023932	23LM122	TPA	26 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration : (*) Without Adjustment

Function of UUC* : Temperature Source

Fresh air setting : Close

Environment during calibration		
	Beginning	Finished
Temp. (°C)	25	25
REL.Humid. (%)	57	54
AC Supply (Volt)	221	222



Probe Installation Details :

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of Chamber :

D = 0.50 m
W = 0.64 m
H = 0.80 m
Capacity = 0.26 m³

Position :	Ref. Std. ID No.:
1	19-16RTD-01
2	19-16RTD-02
3	19-16RTD-03
4	19-16RTD-04
5	19-16RTD-05
6	19-16RTD-06
7	21-16RTD-07
8	19-16RTD-08
9 (ref.)	19-16RTD-09

เอกสารไม่ควบคุม



Equipment : Incubator
 Condition As-Received : Used Item
 Reference : 2404-0003OC-2
 Result of Calibration :- (*) Without Adjustment
 Function of UUC* : Temperature Source
 Fresh air setting : Close

Cert. No.: 24TM650
 Page : 3 of 3

Calibration Point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Temperature stability (± °C)	Temperature uniformity (°C)	Overall Variation (°C)	Coverage Factor k
25.0	25.0	25.0	0.053	0.78	1.3	2
36.0	36.0	36.0	0.14	0.57	0.93	2

Calibration Point (°C)	Measured Temperature (°C)									Uncertainty (±°C)
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
25.0	25.596	25.310	25.439	25.412	24.347	24.332	24.313	24.414	24.875	0.30
36.0	35.843	35.965	35.618	35.701	36.239	36.260	36.343	36.357	36.063	0.31

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

Temperature uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Overall Variation : The Difference of the maximum and minimum measured temperatures throughout observation.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
 CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
 534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
 TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 24TM29
 Page : 1 of 3

Certificate of Calibration

Equipment : Water Bath
 Manufacturer : Memmert
 Model : WNE 14
 Serial No. : L416.0606
 ID No. : UAE.MIC.002/2560
 Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
 3 Soi Udomsuk 41, Sukhumvit Road,
 Bangchak, Phrakhanong,
 Bangkok 10260
 Location : Microbiology Laboratory
 Received Order : 10 February 2024
 Calibration Date : 10 February 2024
 Ambient Temperature : (26 ± 10) °C
 Relative Humidity : (50 ± 30) %

Calibrated by : Krisda Malee

Approved by :
 Approved Signatory

() Pornthippa Tameyakul
 (✓) Unnopphol Harachai
 () Suwit Imjai

Issue Date : 19 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
 Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2402-0232OC-2
 Procedure Used :-

Cert. No.: 24TM29
 Page : 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer (IPRT).

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

Instrument	Serial No.	Cert. No.	Traceable	Due Date
1) Data Acquisition	MY49001451	23LM27	TPA	25 Feb 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Water

	Environmental		AC Voltage Supply (Volt)
	(°C)	(%R.H.)	
Beginning of Calibration	26	51	220
Finished of Calibration	25	50	221



Front

Position :	Ref. Std. ID No.:
1	N37P301419
2	N37P300732
3	N37P301420
4	N37P301421
5(ref.)	N37P301425

เอกสารไม่ควบคุม



Equipment : Water Bath
 Condition As-Received : Used Item
 Reference : 2402-0232OC-2
 Result of Calibration :- (*) Without Adjustment
 Function of UUC* : Temperature Source

Cert. No.: 24TM29
 Page : 3 of 3

Calibration point (°C)	UUC* Setting (°C)	UUC* Reading (°C)	Average* Standard Reading (°C)					Uncertainty (± °C)
			1	2	3	4	5 (ref.)	
44.5	44.4	44.4	44.508	44.469	44.502	44.521	44.527	0.15

Calibration point (°C)	Uniformity (°C)	Stability (± °C)	Coverage Factor k
44.5	0.15	0.074	2

Average* : The average of 30 values in each position.

Uniformity : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

Stability : One-half of the greatest maximum difference of measured temperature at any one probe.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

Calibration Certificate

Certificate No.: 2402281-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Autoclave
Manufacturer: ALP
Model: CL-40L
Serial No.: 808763
ID No.: UAE.MIC.026/2563
Order No.: 2402281
Operation No.: 2402281-001
Date of Receipt: 2 April 2024
Date of Calibration: 2 April 2024

Calibrated by Mr.Jerawut Prapawuttipong
Scientist
Approved by (Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 9 April 2024

The uncertainties are for a confidence probability of approximately 95 %.
This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402281-001-01
Equipment: Autoclave
Model: CL-40L Serial No.: 808763
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563
Manufacturer: ALP
Date of Calibration: 2 April 2024

Page 2 of 3

Location: LABORATORY, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Environment Condition: Ambient Temperature (25 ± 1) °C
Relative Humidity (55 ± 7) %
Line Voltage (225 ± 5) Volt

Condition of this results of Calibration:

- This instrument was calibrated by insert 3 standard temperature recorder with RTD into its autoclave and calibration according to W-TE-018 based on BS 2646-1(2021) : Autoclaves for sterilization in laboratories Design, construction, safety and performance Specification.
- The temperature scale used was based on ITS - 90 .
- All data show below were final values and the initial data may be obtained upon request.

Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
Digital Thermometer with RTD (Data Logger)	HiTemp140-2	R54918	TE 660383-01	8 April 2024	NATIONAL FOOD INSTITUTE
	HiTemp140-2	S25601	TE 670033-01	9 November 2024	MADGETECH INC.
	HiTemp140-2	S25602	TE 670034-01	9 November 2024	MADGETECH INC.

- This certificate is traceable to International System of Units (SI Units).
- This certificate was certified only for the instrument we calibrated.
- This result of calibration was found accurate as shown on date and place of calibration only.
- This standard does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical.
- Condition of Calibrated item : Good
UUC Description : Setting program function sterilization : STERILIZE/NORMAL
Time of sterilization 15 Minute At 115.0 and 121.0 °C
- Result of Calibration : ☒ Without adjustment
☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65


Calibration Report

Certificate No.: 2402281-001-01
Equipment: Autoclave
Model: CL-40L Serial No.: 808763
Resolution: 0.1 °C ID No.: UAE.MIC.026/2563
Manufacturer: ALP
Date of Calibration: 2 April 2024

Page 3 of 3

Calibration point: 115.0 and 121.0 °C

Calibration Condition	Temperature (°C)	Relative Humidity (%)	Line Voltage (Volt)
Min	24.4	48.6	220
Max	25.5	62.1	230



Standard at Position
S1(S1) = Attached to the top temperature probe, within 20 mm.
S2(S2) = In the upper half of the chamber
S3(S3) = In the chamber drain, within 150 mm.

Table1 : Reporting of Temperature

Calibration Point (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.2 is REF)			Uncertainty ± (°C)
	Std.# 1	Std.# 2 (Ref)	Std.# 3	
115.0	115.28	115.35	115.38	0.64
121.0	121.28	121.36	121.37	0.64

Table 2 : Reporting of Characterization Result

UUC* Setting (°C)	UUC* Reading				Stability ± (°C)	Uniformity (°C)	Overall Variation (°C)
	Min (°C)	Max (°C)	Average (°C)	MPA			
115.0	115.0	115.1	115.0	0.08	0.19	0.13	0.48
121.0	121.0	121.1	121.0	0.12	0.17	0.10	0.38

Note

The quoted uncertainty include " Stability " and " Loading effect (20% of Uniformity) "
UUC* = Unit Under Calibration
Stability = One-half of the greatest maximum difference of measured temperatures at any one sensors, for at least half an hour after reaching steady state.
Uniformity = The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time.
Overall Variation = The Difference of the maximum and minimum measured temperatures throughout observation time.
The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k = 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

Certificate of Calibration

Equipment: Balance
Model: PX623
Serial No. (or ID.): C236754745 (UAE.MIC.055/2565)
Manufacturer: Ohaus
Condition: In condition
Certificate No.: C01234158
Issued Date: 08 December 2023
Job No.: WO-00011251
Page: 1 of 3

Customer: United Analyst and Engineering Consultant Co., Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,
Phrakhanong District, Bangkok, THAILAND 10260

Environment Condition: Temperature 25 °C ± 0.5 °C
Humidity 54 %RH ± 1.7 %RH

Calibration Place: United Analyst and Engineering Consultant Co., Ltd. (301 Microbiology Room)
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak Sub-District,
Phrakhanong District, Bangkok, THAILAND 10260

Calibration By: Mr. Adisai Maknoi
Calibration Date: 07 December 2023
The Method used: In-house method, CAL-WI-47, based on UKAS Lab 14
Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02222534

(Mr. Adisai Maknoi)
Person in charge

(Mr. Rungrod Jenkitrakulchai)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 สุขุมวิท 41 แขวงคลองตันใต้ เขตวัฒนา กรุงเทพมหานคร 10260
Phone : +66 2639 7000 Email : info.calibration@dksh.com Website : www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.




เอกสารไม่ควบคุม

CAL-FM-C01-14: 12 Sep 2022

Calibration Results:

Before Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

			Nominal Test Value	200	(g)
Reference Points (g)					
A	B	C	D	E	
-	0.000	-0.003	0.000	0.001	

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.001 (g)




Nominal test value (g)	Standard Deviation
50	0.0006
500	0.0008

Error of indication from nominal or conventional mass value., Readability 0.001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of indication (g)	Uncertainty (g)	k
1	1.0000	1.000	0.000	0.0013	2.10
5	5.0001	5.000	0.000	0.0013	2.10
10	10.0001	10.001	0.001	0.0013	2.10
20	20.0000	20.000	0.000	0.0013	2.09
50	50.0001	50.000	0.000	0.0013	2.09
100	100.0001	100.001	0.001	0.0013	2.09
200	200.0004	200.002	0.002	0.0014	2.07
300	300.0005	300.002	0.002	0.0015	2.05
400	400.0006	400.004	0.003	0.0016	2.03
500	500.0006	500.008	0.007	0.0019	2.02
600	600.0007	600.009	0.008	0.0021	2.01

After Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

			<div>Nominal Test Value200(g)</div> <table><tr><th colspan="5">Reference Points (g)</th></tr><tr><th>A</th><th>B</th><th>C</th><th>D</th><th>E</th></tr><tr><td>-</td><td>0.001</td><td>-0.002</td><td>-0.002</td><td>0.001</td></tr></table>	Reference Points (g)					A	B	C	D	E	-	0.001	-0.002	-0.002	0.001
Reference Points (g)																		
A	B	C	D	E														
-	0.001	-0.002	-0.002	0.001														

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.001 (g)

Nominal test value (g)	Standard Deviation
50	0.0006
500	0.0008

Error of indication from nominal or conventional mass value., Readability 0.001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of indication (g)	Uncertainty (g)	k
1	1.0000	1.000	0.000	0.0013	2.10
5	5.0001	5.000	0.000	0.0013	2.10
10	10.0001	10.000	0.000	0.0013	2.10
20	20.0000	20.000	0.000	0.0013	2.10
50	50.0001	50.000	0.000	0.0013	2.10
100	100.0001	100.000	0.000	0.0014	2.09
200	200.0004	200.000	0.000	0.0014	2.07
300	300.0005	300.001	0.001	0.0015	2.05
400	400.0006	400.002	0.001	0.0017	2.04
500	500.0006	500.001	0.000	0.0019	2.02
600	600.0007	600.002	0.001	0.0021	2.01

The End of Certificate

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The error of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, UKAS Lab14. Therefore, those parameters have not been assessed separately.

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk < 50% PFA.
- ☒ Choice B Non-binary statement with guard band ($w = 1 U$), Pass or Fail Specific Risk < 2.5% PFA and Condition Pass or Condition Fail Specific Risk < 50% PFA.
- ☐ Choice C Customer defined, Customers may define arbitrary multiple of r to have applied as guard band ($w = r U$).
- ; PFA – Probability of False Accept

Rungrod

(Mr. Rungrod Jenkitrakulchai)

Authorized signatory

Statements of conformity:

Before Adjustment

Readability: 0.001 g

Nominal Value (g)	Error of indication (g)	Guard band (w) (g)	Tolerance (\pm) (g)	Conformity
1	0.000	0.0013	0.002	Pass
5	0.000	0.0013	0.010	Pass
10	0.001	0.0013	0.020	Pass
20	0.000	0.0013	0.040	Pass
50	0.000	0.0013	0.100	Pass
100	0.001	0.0013	0.200	Pass
200	0.002	0.0014	0.400	Pass
300	0.002	0.0015	0.600	Pass
400	0.003	0.0016	0.800	Pass
500	0.007	0.0019	1.000	Pass
600	0.008	0.0021	1.200	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

Statements of conformity:



After Adjustment

Readability: 0.001 g

Nominal Value g	Error of indication g	Guard band (w) g	Tolerance (±) g	Conformity
1	0.000	0.0013	0.002	Pass
5	0.000	0.0013	0.010	Pass
10	0.000	0.0013	0.020	Pass
20	0.000	0.0013	0.040	Pass
50	0.000	0.0013	0.100	Pass
100	0.000	0.0014	0.200	Pass
200	0.000	0.0014	0.400	Pass
300	0.001	0.0015	0.600	Pass
400	0.001	0.0017	0.800	Pass
500	0.000	0.0019	1.000	Pass
600	0.001	0.0021	1.200	Pass

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

The End of Statements of conformity

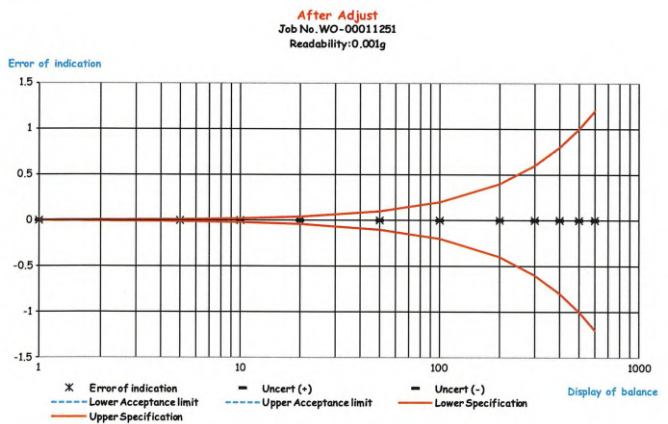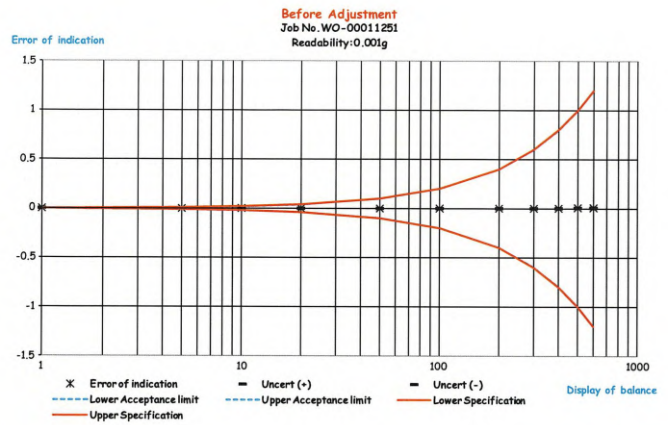

บริษัท ดีเคเอสเอ เอเชีย (ไทย) จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangkok, Prachinbong, Bangkok 10260
Phone: +66 2638 7000 Email: info.asia@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม

CAL-FM-C01-14: 12 Sep 2022

เอกสารไม่ควบคุม

ใบตรวจสอบสภาพเครื่องชั่ง

เลขที่ใบงาน: WO-00011251

ชนิดเครื่องมือ: Balance

รุ่น: PX623

หมายเลขเครื่อง: C236754745

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
07 Dec 2023			07 Dec 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ/Adapter, power supply 220/110V	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสมบูรณ์ชุดกระงะกักันลม (Cover)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. ความสมบูรณ์ชุดของระดับน้ำ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การปรับระดับของขาตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. การตอบสนองของไม่กด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. ความสมบูรณ์ของ Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. การแสดงผลของ Display หลังวางน้ำหนัก	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ชุดรองจานชั่ง (Stopper) / pan support	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานของ Function Internal / External	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. ความสะอาดของตัวเครื่องภายนอกและถาด load cell	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. สภาวะแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

หมายเหตุเพิ่มเติม/ข้อแนะนำ :

Mr. Adisai Maknoi

Service Engineer