

ภาคผนวกที่ 5

เอกสารสอบเทียบความถูกต้องของเครื่องมือ

เอกสารแนบ	5-1	เอกสารการสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศบริเวณพื้นที่อ่อนไหว
เอกสารแนบ	5-2	เอกสารการสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศบริเวณอาคารจอดรถ
เอกสารแนบ	5-3	เอกสารสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศภายในขบวนและสถานีรถไฟ
เอกสารแนบ	5-4	เอกสารการสอบเทียบเครื่องมือตรวจวัดระดับเสียง
เอกสารแนบ	5-5	เอกสารสอบเทียบเครื่องมือตรวจวิเคราะห์คุณภาพน้ำ

เอกสาร 5-1

เอกสารการสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศบริเวณพื้นที่อ่อนไหว



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spsc.com, www.spsc.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R ²
B01	B01	01/02/2024	y = 1.224x-3.492	0.998
B02	B02	01/02/2024	y = 1.143x+1.630	0.999
B03	B03	01/02/2024	y = 1.180x-2.783	1.000
B04	B04	02/02/2024	y = 1.257x-5.884	0.997
B05	B05	03/02/2024	y = 1.261x-7.123	0.999
B06	B06	02/02/2024	y = 1.245x-6.024	0.999
B07	B07	03/02/2024	y = 1.209x-6.025	0.997
B08	B08	02/02/2024	y = 1.239x-5.848	0.997
B09	B09	02/02/2024	y = 1.244x-5.247	0.997
B10	B10	02/02/2024	y = 1.153x+0.064	0.998
B11	B11	01/02/2024	y = 1.110x-1.064	1.000
B12	B12	03/02/2024	y = 1.227x-6.093	0.999
B13	B13	01/02/2024	y = 1.286x-7.480	1.000
B14	B14	02/02/2024	y = 1.220x-5.066	0.999
B15	B15	02/02/2024	y = 1.150x-1.264	0.999
B16	B16	03/02/2024	y = 1.177x-3.231	0.996
B17	B17	02/02/2024	y = 1.235x-5.039	0.999
B18	B18	03/02/2024	y = 1.210x-5.028	0.998
B19	B19	03/02/2024	y = 1.215x-7.087	0.998
B20	B20	02/02/2024	y = 1.204x-4.119	0.996
B21	B21	02/02/2024	y = 1.190x-4.960	0.999
B22	B22	02/02/2024	y = 1.208x-7.133	0.996
B23	B23	01/02/2024	y = 1.217x-4.085	0.998
B24	B24	01/02/2024	y = 1.145x-2.502	1.000
B25	B25	02/02/2024	y = 1.090x+1.068	0.999
B26	B26	03/02/2024	y = 1.234x-5.493	0.998
B27	B27	01/02/2024	y = 1.168x-4.382	0.999
B28	B28	02/02/2024	y = 1.237x-7.982	0.999
B29	B29	03/02/2024	y = 1.186x-2.530	0.996
B30	B30	02/02/2024	y = 1.212x-4.090	0.997
B31	B31	02/02/2024	y = 1.195x-4.732	0.999
B32	B32	03/02/2024	y = 1.169x-0.802	0.996
B33	B33	03/02/2024	y = 1.203x-2.954	0.996
B34	B34	02/02/2024	y = 1.221x-5.796	1.000

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompet, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spsc.com, www.spsc.com

High Volume Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard Model : TE 5025A S/N : 3611

Calibration Data

High Volume Air Sampler Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R ²
B35	B35	02/02/2024	y = 1.188x-3.435	0.996
B36	B36	01/02/2024	y = 1.201x-4.036	0.999
B37	B37	01/02/2024	y = 1.196x-2.671	0.998
B38	B38	02/02/2024	y = 1.232x-6.552	0.997
B39	B39	03/02/2024	y = 1.164x-0.902	0.997
B40	B40	01/02/2024	y = 1.225x-6.117	0.999
B41	B41	02/02/2024	y = 1.265x-6.140	0.999
B42	B42	02/02/2024	y = 1.187x-3.625	0.999
B43	B43	01/02/2024	y = 1.233x-2.707	0.997
B44	B44	01/02/2024	y = 1.202x-3.263	0.996
R01	R01	01/02/2024	y = 1.214x-4.512	0.999
R02	R02	02/02/2024	y = 1.222x-5.522	0.999
R03	R03	03/02/2024	y = 1.204x-5.785	0.999
R04	R04	01/02/2024	y = 1.220x-5.355	0.999
R05	R05	01/02/2024	y = 1.190x-5.262	0.997
R06	R06	02/02/2024	y = 1.223x-6.383	0.998
R07	R07	02/02/2024	y = 1.084x+0.577	0.999
R08	R08	01/02/2024	y = 1.157x-2.531	0.999
R09	R09	01/02/2024	y = 1.194x-3.227	0.998
R10	R10	02/02/2024	y = 1.198x-4.625	0.998
R11	R11	02/02/2024	y = 1.143x-2.176	1.000
R12	R12	02/02/2024	y = 1.165x-4.124	0.998
R13	R13	03/02/2024	y = 1.133x-1.833	0.997
R14	R14	01/02/2024	y = 1.216x-3.559	0.995
R15	R15	01/02/2024	y = 1.183x-5.143	0.999
R16	R16	01/02/2024	y = 1.227x-7.151	0.999
R17	R17	02/02/2024	y = 1.181x-3.964	0.996
R18	R18	02/02/2024	y = 1.195x-3.915	0.997
R19	R19	03/02/2024	y = 1.215x-6.609	1.000
R20	R20	03/02/2024	y = 1.208x-5.309	0.998

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพมหานคร 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jomjol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscs.com, www.spscs.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R ²
B01	B01	02/02/2024	y = 1.147x-0.194	0.996
B02	B02	01/02/2024	y = 1.060x+2.506	1.000
B03	B03	01/02/2024	y = 1.216x-3.895	0.996
B04	B04	01/02/2024	y = 1.224x-5.960	0.999
B05	B05	02/02/2024	y = 1.220x-5.384	0.999
B06	B06	02/02/2024	y = 1.197x-4.228	0.998
B07	B07	03/02/2024	y = 1.208x-4.865	0.996
B08	B08	01/02/2024	y = 1.171x-1.266	0.998
B09	B09	01/02/2024	y = 1.198x-5.197	0.997
B10	B10	01/02/2024	y = 1.219x-5.339	0.997
B11	B11	03/02/2024	y = 1.211x-3.765	0.999
B12	B12	05/02/2024	y = 1.203x-3.968	0.997
B13	B13	05/02/2024	y = 1.158x-1.909	0.996
B14	B14	03/02/2024	y = 1.190x-3.316	0.999
B15	B15	01/02/2024	y = 1.163x-1.150	0.999
B16	B16	01/02/2024	y = 1.170x+0.508	0.999
B17	B17	01/02/2024	y = 1.186x-2.843	0.997
B18	B18	01/02/2024	y = 1.207x-1.821	1.000
B19	B19	03/02/2024	y = 1.178x-2.990	0.999
B20	B20	02/02/2024	y = 1.206x-5.507	0.997
B21	B21	03/02/2024	y = 1.172x-0.702	0.999
B22	B22	02/02/2024	y = 1.175x-1.992	0.996
B23	B23	02/02/2024	y = 1.196x-3.382	0.998
B24	B24	01/02/2024	y = 1.181x-2.463	0.999
B25	B25	01/02/2024	y = 1.204x-3.960	0.997
B26	B26	01/02/2024	y = 1.218x-5.354	0.998
B27	B27	03/02/2024	y = 1.178x-4.891	0.997
B28	B28	02/02/2024	y = 1.226x-6.323	0.999
B29	B29	05/02/2024	y = 1.174x-3.753	0.997
B30	B30	03/02/2024	y = 1.179x-3.207	0.998
B31	B31	03/02/2024	y = 1.189x-1.040	0.997
B32	B32	01/02/2024	y = 1.222x-3.816	0.999
B33	B33	01/02/2024	y = 1.159x-1.689	0.996
B34	B34	01/02/2024	y = 1.191x-1.278	0.995

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจตุจักร กรุงเทพมหานคร 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jomjol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscs.com, www.spscs.com

High Volume PM-10 Air Sampler Calibration Report

Calibration Method : Multipoint Orifice Flow Transfer Standard

Model : TE 5025A

S/N : 3611

Calibration Data

High Volume PM-10 Data		Calibration Data		
Recorder No.	Blower No.	Date	Actual Flowrate (l/min)	R ²
R01	R01	02/02/2024	y = 1.206x-5.952	0.998
R02	R02	02/02/2024	y = 1.219x-3.961	0.997
R03	R03	01/02/2024	y = 1.203x-5.426	0.998
R04	R04	01/02/2024	y = 1.191x-6.027	0.997
R05	R05	01/02/2024	y = 1.199x-5.883	1.000
R06	R06	01/02/2024	y = 1.192x-3.038	0.998
R07	R07	02/02/2024	y = 1.169x-2.670	0.996
R08	R08	02/02/2024	y = 1.186x-4.195	0.997
R09	R09	03/02/2024	y = 1.184x-3.512	1.000
R10	R10	03/02/2024	y = 1.179x-3.695	0.999
R11	R11	03/02/2024	y = 1.202x-2.389	0.997
R12	R12	01/02/2024	y = 1.194x-5.194	0.998
R13	R13	01/02/2024	y = 1.173x-2.754	0.999
R14	R14	01/02/2024	y = 1.176x-2.291	0.997
R15	R15	02/02/2024	y = 1.188x-3.910	0.998
R16	R16	02/02/2024	y = 1.180x-3.568	0.998
R17	R17	02/02/2024	y = 1.195x-3.126	0.998
R18	R18	03/02/2024	y = 1.143x-2.749	1.000
R19	R19	01/02/2024	y = 1.154x-2.002	0.996
R20	R20	01/02/2024	y = 1.161x-4.362	0.998

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)



CERTIFICATE No : 24M2227
REFERENCE No : 72448-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : METTLER TOLEDO
MODEL : XS105DU
SERIAL No : 1126422905
ID No : BA05/50
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24, PHAHOLYOTHIN RD.,
JOMPOL, CHATUCHAK, BANGKOK 10900

CALIBRATED BY : ATSAWIN Y.

CALIBRATION DATE : 08-Mar-24

APPROVED BY : PONGSAK J.

ISSUED DATE : 14-Mar-24

RECEIVED DATE : 08-Mar-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 24M2227

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : XS105DU
MANUFACTURER : METTLER TOLEDO S/N : 1126422905
ID No : BA05/50 RECEIVED DATE : 08-Mar-24
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 08-Mar-24
AMBIENT TEMPERATURE : 25° C \pm 1° C RELATIVE HUMIDITY : 53 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL

2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0.000055 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.00	0.00000	0.00000	0.000065
0.02	0.02001	-0.00001	0.000065
0.10	0.10002	-0.00002	0.000066
0.20	0.20001	-0.00001	0.000066
0.50	0.50001	-0.00001	0.000065
1.00	1.00003	-0.00003	0.000066
2.00	2.00001	-0.00001	0.000067
5.00	5.00001	-0.00001	0.000068
10.00	9.99994	0.00006	0.000070
20.00	20.00008	-0.00008	0.000078
50.00	50.0000	0.0000	0.00013
100.00	100.0001	-0.0001	0.00019
120.00	120.0001	-0.0001	0.00022

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	50.0000
2	50.0000
3	50.0000
4	50.0000
5	50.0000
OFF-CENTER LOADING	0.0000

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

NON-DISPERSIVE INFRARED CO ANALYZER

DATE : 25 April 2024 BRAND : API MODEL : 300E
NO. CO-B01 SERIAL NO. 782

Calibrator (Dilution System)

Brand : Teledyne Model : 700E
Last Cal. Date : 30 October 2023 Serial No. : 201-S

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO) Cylinder No. : D711839
Certified Date : 14 March 2024 Expired Date : 14 March 2032 Cylinder Conc. : 4,580 PPM

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	-0.10	-	0
CO Span	40.00	39.90	-0.250	40.00

API Model 300E CO Analyzer Check list

Parameter	Observed Value	Units	Nominal Range
RANGE	50	PPM	0-1000 ppm
STABILITY	0.10	PPM	< 1 ppm with zero air
CO MEASURE	4016.4	mV	2500-4800 mV
CO REFERENCE	3949.8	mV	2500-4800 mV
MEASURE/REFERENCE RATIO	1.180	-	1.1-1.3 w/zero air
SAMPLE PRESSURE	28.6	In-Hg-A	~2" < ambient absolute pressure
SAMPLE FLOW	808	cc/min	800 ± 10%
SAMPLE TEMPERATURE	48.2	°C	48 ± 4
BENCH TEMPERATURE	48.0	°C	48 ± 2
WHEEL TEMPERATURE	68.2	°C	68 ± 2
BOX TEMPERATURE	30.7	°C	Ambient temp + 7 ± 10
PHOTO-DRIVE	3035.4	mV	250 mV to 4750 mV
SLOPE	1.017	-	1.0 ± 0.3
OFFSET	0.2	-	0 ± 0.3

Calibrated by : (Mr.Adul Dangklom)

Approved by : (Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

NON-DISPERSIVE INFRARED CO ANALYZER

DATE : 25 April 2024 BRAND : API MODEL : 300E
NO. CO-B02 SERIAL NO. 965

Calibrator (Dilution System)

Brand : Teledyne Model : 700E
Last Cal. Date : 30 October 2023 Serial No. : 201-S

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO) Cylinder No. : D711839
Certified Date : 14 March 2024 Expired Date : 14 March 2032 Cylinder Conc. : 4,580 PPM

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	-0.10	-	0
CO Span	40.00	40.05	0.125	40.00

API Model 300E CO Analyzer Check list

Parameter	Observed Value	Units	Nominal Range
RANGE	50	PPM	0-1000 ppm
STABILITY	0.10	PPM	< 1 ppm with zero air
CO MEASURE	4017.3	mV	2500-4800 mV
CO REFERENCE	3948.5	mV	2500-4800 mV
MEASURE/REFERENCE RATIO	1.180	-	1.1-1.3 w/zero air
SAMPLE PRESSURE	28.4	In-Hg-A	~2" < ambient absolute pressure
SAMPLE FLOW	805	cc/min	800 ± 10%
SAMPLE TEMPERATURE	48.5	°C	48 ± 4
BENCH TEMPERATURE	48.2	°C	48 ± 2
WHEEL TEMPERATURE	68.5	°C	68 ± 2
BOX TEMPERATURE	30.9	°C	Ambient temp + 7 ± 10
PHOTO-DRIVE	3043.5	mV	250 mV to 4750 mV
SLOPE	1.017	-	1.0 ± 0.3
OFFSET	0.2	-	0 ± 0.3


Calibrated by : (Mr.Adul Dangklom)

Approved by : (Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
NON-DISPERSIVE INFRARED CO ANALYZER					
DATE :	25 April 2024	BRAND :	API	MODEL :	300E
NO.	CO-B05	SERIAL NO.	3116		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700E	
Last Cal. Date	: 30 October 2023		Serial No.	: 201-S	
Reference Standard Gas					
Standard Gas	: Carbon Monoxide (CO)		Cylinder No.	: D711839	
Certified Date	: 14 March 2024		Expired Date	: 14 March 2032	
Cylinder Conc.	: 4,580 PPM				
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	0.10	-	0	
CO Span	40.00	40.06	0.150	40.00	
API Model 300E CO Analyzer Check list					
Parameter	Observed Value	Units	Nominal Range		
RANGE	50	PPM	0-1000 ppm		
STABILITY	0.10	PPM	< 1 ppm with zero air		
CO MEASURE	4014.9	mV	2500-4800 mV		
CO REFERENCE	3948.1	mV	2500-4800 mV		
MEASURE/REFERENCE RATIO	1.180	-	1.1-1.3 w/zero air		
SAMPLE PRESSURE	28.5	In-Hg-A	~2"± ambient absolute pressure		
SAMPLE FLOW	811	cc/min	800 ± 10%		
SAMPLE TEMPERATURE	48.3	°C	48 ± 4		
BENCH TEMPERATURE	48.1	°C	48 ± 2		
WHEEL TEMPERATURE	68.4	°C	68 ± 2		
BOX TEMPERATURE	30.6	°C	Ambient temp + 7 ± 10		
PHOTO-DRIVE	3045.9	mV	250 mV to 4750 mV		
SLOPE	1.017	-	1.0 ± 0.3		
OFFSET	0.2	-	0 ± 0.3		

Calibrated by : 
(Mr.Abul Dangklom)

Approved by : 
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT					
NON-DISPERSIVE INFRARED CO ANALYZER					
DATE :	25 April 2024	BRAND :	API	MODEL :	300E
NO.	CO-B06	SERIAL NO.	3117		
Calibrator (Dilution System)					
Brand	: Teledyne		Model	: 700E	
Last Cal. Date	: 30 October 2023		Serial No.	: 201-S	
Reference Standard Gas					
Standard Gas	: Carbon Monoxide (CO)		Cylinder No.	: D711839	
Certified Date	: 14 March 2024		Expired Date	: 14 March 2032	
Cylinder Conc.	: 4,580 PPM				
CALIBRATING CONDITION					
Pressure	1011	mmbar	Temp.	24.6	°C
% RH	49				
CALIBRATION SETTING					
Span	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM	
Set Point	Expected Concentration	Analyzer Response	%Dif	Analyzer Response	
Zero	0	0.10	-	0	
CO Span	40.00	40.04	0.100	40.00	
API Model 300E CO Analyzer Check list					
Parameter	Observed Value	Units	Nominal Range		
RANGE	50	PPM	0-1000 ppm		
STABILITY	0.10	PPM	< 1 ppm with zero air		
CO MEASURE	4015.8	mV	2500-4800 mV		
CO REFERENCE	3949.5	mV	2500-4800 mV		
MEASURE/REFERENCE RATIO	1.179	-	1.1-1.3 w/zero air		
SAMPLE PRESSURE	28.5	In-Hg-A	~2"± ambient absolute pressure		
SAMPLE FLOW	807	cc/min	800 ± 10%		
SAMPLE TEMPERATURE	48.5	°C	48 ± 4		
BENCH TEMPERATURE	48.2	°C	48 ± 2		
WHEEL TEMPERATURE	68.4	°C	68 ± 2		
BOX TEMPERATURE	30.6	°C	Ambient temp + 7 ± 10		
PHOTO-DRIVE	3028.7	mV	250 mV to 4750 mV		
SLOPE	1.017	-	1.0 ± 0.3		
OFFSET	0.2	-	0 ± 0.3		

Calibrated by : 
(Mr.Abul Dangklom)

Approved by : 
(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

NON-DISPERSIVE INFRARED CO ANALYZER

DATE : 25 April 2024 BRAND : API MODEL : 300E
NO. CO-B13 SERIAL NO. 176

Calibrator (Dilution System)

Brand : Teledyne Model : 700E
Last Cal. Date : 30 October 2023 Serial No. : 201-S

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO) Cylinder No. : D711839
Certified Date : 14 March 2024 Expired Date : 14 March 2032 Cylinder Conc. : 4,580 PPM

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	-0.10	-	0
CO Span	40.00	39.96	-0.100	40.00

API Model 300E CO Analyzer Check list

Parameter	Observed Value	Units	Nominal Range
RANGE	50	PPM	0-1000 ppm
STABILITY	0.10	PPM	< 1 ppm with zero air
CO MEASURE	4015.7	mV	2500-4800 mV
CO REFERENCE	3947.5	mV	2500-4800 mV
MEASURE/REFERENCE RATIO	1.180	-	1.1-1.3 w/zero air
SAMPLE PRESSURE	28.7	In-Hg-A	-2" < ambient absolute pressure
SAMPLE FLOW	809	cc/min	800 ± 10%
SAMPLE TEMPERATURE	48.2	°C	48 ± 4
BENCH TEMPERATURE	48.0	°C	48 ± 2
WHEEL TEMPERATURE	68.3	°C	68 ± 2
BOX TEMPERATURE	30.9	°C	Ambient temp + 7 ± 10
PHOTO-DRIVE	3023.2	mV	250 mV to 4750 mV
SLOPE	1.017	-	1.0 ± 0.3
OFFSET	0.2	-	0 ± 0.3

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol, Chatuchak, Bangkok 10900
Tel : (662) 939-4370-72, Fax : (662) 513-4221, E-mail : sale@spscon.com, www.spscon.com

CALIBRATION REPORT

NON-DISPERSIVE INFRARED CO ANALYZER

DATE : 25 April 2024 BRAND : API MODEL : 300EU
NO. CO-B14 SERIAL NO. 131

Calibrator (Dilution System)

Brand : Teledyne Model : 700E
Last Cal. Date : 30 October 2023 Serial No. : 201-S

Reference Standard Gas

Standard Gas : Carbon Monoxide (CO) Cylinder No. : D711839
Certified Date : 14 March 2024 Expired Date : 14 March 2032 Cylinder Conc. : 4,580 PPM

CALIBRATING CONDITION

Pressure 1011 mmbar Temp. 24.6 °C % RH 49

CALIBRATION SETTING

Span Set Point	Initial Reading (Before Adj.),PPM			Final Reading (After Adj.),PPM
	Expected Concentration	Analyzer Response	%Dif	Analyzer Response
Zero	0	0.10	-	0
CO Span	40.00	39.98	-0.050	40.00

API Model 300EU CO Analyzer Check list

Parameter	Observed Value	Units	Nominal Range
RANGE	50	PPM	0-1000 ppm
STABILITY	0.10	PPM	< 1 ppm with zero air
CO MEASURE	4014.5	mV	2500-4800 mV
CO REFERENCE	3947.8	mV	2500-4800 mV
MEASURE/REFERENCE RATIO	1.180	-	1.1-1.3 w/zero air
SAMPLE PRESSURE	28.6	In-Hg-A	-2" < ambient absolute pressure
SAMPLE FLOW	810	cc/min	800 ± 10%
SAMPLE TEMPERATURE	48.4	°C	48 ± 4
BENCH TEMPERATURE	48.2	°C	48 ± 2
WHEEL TEMPERATURE	68.4	°C	68 ± 2
BOX TEMPERATURE	30.7	°C	Ambient temp + 7 ± 10
PHOTO-DRIVE	3051.3	mV	250 mV to 4750 mV
SLOPE	1.017	-	1.0 ± 0.3
OFFSET	0.2	-	0 ± 0.3

Calibrated by :

(Mr.Adul Dangklom)

Approved by :

(Mr.Peera Detudom)

เอกสาร 5-2

เอกสารการสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศบริเวณอาคารจอดรถ

CERTIFICATE OF CALIBRATION

Certificate No. : CO-004-66

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : Andersen Instruments
MODEL/TYPE : G25A
SERIAL NUMBER : 1270
ID NUMBER : UAE.ANV.009/2542
CONDITION AS-RECEIVED : Used item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udumsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 02 Jun 2023
MEASUREMENT DATE : 12 Jun 2023
ISSUE DATE : 12 Jun 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.3 °C and 55.0%RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the VSL (National Metrology Institute of Netherlands) via Certificate number: G2211901

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$. Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH ₂ O	y	Standard Flow [Q _s] m ³ /min
1	0.705	755.787	24.17	23.48	47.401	1.708	1.305	0.661
2	0.999	755.849	23.95	23.54	51.522	3.383	1.837	0.930
3	1.119	755.810	23.39	22.98	35.502	4.448	2.109	1.068
4	1.170	755.752	23.42	23.02	26.462	4.999	2.235	1.131
5	1.425	755.681	23.52	23.12	26.582	7.431	2.725	1.376

Slope (m): 1.98561
Intercept (b): -0.00879
Correlation coefficient (r): 0.99984
Uncertainty (k=2): 0.015 m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m ³ /min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH ₂ O	y	Standard Flow [Q _a] m ³ /min
1	0.705	755.787	24.17	23.48	47.401	1.708	0.820	0.663
2	0.999	755.849	23.95	23.54	51.522	3.383	1.153	0.932
3	1.119	755.810	23.39	22.98	35.502	4.448	1.321	1.068
4	1.170	755.752	23.42	23.02	26.462	4.999	1.401	1.131
5	1.425	755.681	23.52	23.12	26.582	7.431	1.708	1.377

Slope (m): 1.24382
Intercept (b): -0.00554
Correlation coefficient (r): 0.99984
Uncertainty (k=2): 0.015 m³/min

End of Certificate of Calibration

Calibrated by:

☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager





Certificate of Calibration

Certificate No. : 24P1250
Page : 1 of 2

Equipment : U Tube Manometer

Manufacturer: Dwyer

Model : 1221-36-W/M

Serial No.: -

ID No.: UAE.EFM.076/2566

Condition As-Received: Used Item

Received Date: 03 April 2024

Calibration Date: 10 April 2024

Reference: 2404-0118WSC

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1007 mbar

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3: Equipment Calibration and Testing Services.

81 Soi Udumsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments
Standard according to calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as
a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0176-23	12 Sep 2024

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH₂O

4.This instrument was used clean air as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by : Suksan Khankaew
Issue Date : 17 April 2024

Approved Signatory : _____

[] Phalinee Prabpaipal

[] Sura Suwannasri

[✓] Attapol Panurach

เอกสารไม่ควบคุม



Cert.No.: 24P1250

Page: 2 of 2

Result of calibration:- Without adjustment

Function:- Pressure Measurement

Increasing Pressure

Range : 0 inH₂O to 36 inH₂O

Scale Interval : 0.1 inH₂O (The Second Estimate)

Applied Pressure	High-port side	UUC Indication Low-port side	ΔP	Error
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	8.00	0.00
10.00	5.05	-4.95	10.00	0.00
12.00	6.05	-5.95	12.00	0.00
14.00	7.05	-6.95	14.00	0.00
16.00	8.10	-7.95	16.05	0.05
18.00	9.10	-8.95	18.05	0.05
20.00	10.10	-9.95	20.05	0.05
22.00	11.10	-10.95	22.05	0.05
24.00	12.10	-11.95	24.05	0.05
26.00	13.15	-12.95	26.10	0.10
28.00	14.15	-13.95	28.10	0.10
30.00	15.20	-14.95	30.15	0.15
32.00	16.20	-15.95	32.15	0.15
34.00	17.20	-16.95	34.15	0.15
35.50	18.00	-17.70	35.70	0.20

The uncertainty of measurement was ± 0.11 inH₂O

* ΔP = High-port side - Low-port side

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied
by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No.: 23P1856

Page: 1 of 2

Equipment: Aneroid Barometer
Manufacturer: Barigo
Model: -
Serial No.: -
ID No.: UAE.EMA2.110/2555

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 02 June 2023

Reference: 2305-0919WSC

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: (23 ± 2) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: 1006 mbar

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

Condition of this result of calibration

1. Reference standards instruments :

Instrument

Model

Serial No.

Certificate No.

Due Date

1) Standard Barometer

DPI142

1422505046

MP-0094-23

03 May 2024

2. This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3. This result of calibration was made on requested at the point specified by customer.

4. This result of calibration instrument was in absolute pressure.

5. This instrument was used clean air as pressure media.

6. The certificate is valid only to the item calibrated on date and place of calibration.

7. This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by: Suksan Khankaew
Issue Date: 08 June 2023

Approved Signatory:

[] Phalinee Prabpaipal

[] Sura Suwannasri

✓ [] Attapol Panurach

เอกสารไม่ควบคุม
B 0316956



Cert.No.: 23P1856

Page: 2 of 2

Result of calibration:- Without adjustment

Range: 720 mmHg to 800 mmHg

Function:- Absolute Pressure Measurement

Scale Interval: 1 mmHg (The Fifth Estimate)

Increasing Pressure

Applied Pressure (mmHg)	720.43	730.67	740.34	751.52	756.56	761.83	773.53	798.76
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	755.0	760.0	770.0	790.0
Error (mmHg)	-0.43	-0.67	-0.34	-1.52	-1.56	-1.83	-3.53	-8.76

Decreasing Pressure

Applied Pressure (mmHg)	798.76	773.60	761.89	756.65	751.59	740.72	730.68	720.59
UUC* Indication (mmHg)	790.0	770.0	760.0	755.0	750.0	740.0	730.0	720.0
Error (mmHg)	-8.76	-3.60	-1.89	-1.65	-1.59	-0.72	-0.68	-0.59

The uncertainty of measurement was ± 0.24 mmHg

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม
a 1165502



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23H1201
Page : 1 of 2

Equipment : Dial Thermo-Hygrometer
Manufacturer: Barigo
Model : -
Serial No.: -
ID No.: UAE.EMA2.014/2555

This certificate may not be reproduced other than in full,
except with the prior written approval of the head of
Corporate Services 3; Equipment Calibration and Testing Services.

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 30 May 2023
to 06 June 2023

Reference: 2305-0919WSC

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

81 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1. Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Hygro-M2 Dew Point Monitor	5112	2360195	20703	02 Aug 2023
2) Handheld Thermometer With Sensor	1523	3240076	231305	15 Mar 2024

2. The certificate is valid only to the item calibrated on date and place of calibration.

3. This Certification is traceable to the International System of Unit maintained through:-

- National Institute of Standards and Technology (NIST) , The United States of America
- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Somchai Dumwor
Issue Date : 07 June 2023

Approved Signatory :

[✓] Chakrit Waewwanjua
[] Pornthippa Tameyakul
[] Viporn Tantiyawutti

เอกสารไม่ควบคุม
B 0316275



Cert. No.: 23H1201
Page.: 2 of 2

Result of Calibration:- Before Adjustment
Function: Humidity Measurement

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(%R.H.)	(%R.H.)	(%R.H.)	(±%R.H.)
25.0	40.1	55	14.9	1.6
25.0	60.0	66	6.0	1.7
25.0	80.0	78	-2.0	1.9

Result of Calibration:- After Adjustment
Function: Humidity Measurement

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(%R.H.)	(%R.H.)	(%R.H.)	(±%R.H.)
25.0	40.1	46	5.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	72	-8.0	1.9

Result of Calibration:- Without Adjustment
Function: Temperature Measurement

Standard Temperature	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(°C)	(°C)	(±°C)
19.987	20.0	0.013	0.72
30.016	30.0	-0.016	0.72
39.944	39.0	-0.944	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม
a 1165294

MULTI-POINT GAS TEST REPORT


Test Date : Nov 1, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM08130002

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 146i
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8		
Cylinder No. :	EB0143262		
Expiration Date :	Jun 21, 2024		

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.9	0.90	0.90	0.90
Level 2	20.00%	100.0	101.3	1.30	1.28	1.28
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)			0.59

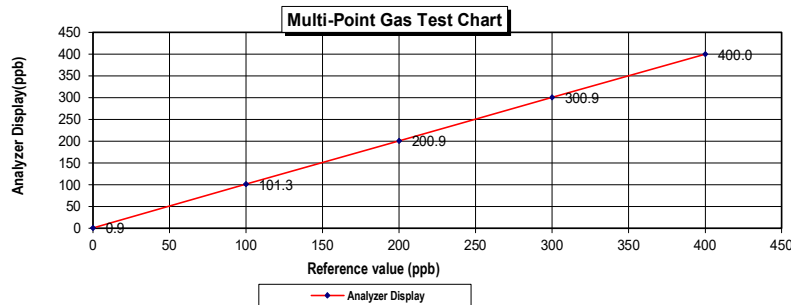

Calculate by

01 / Nov / 2023

Approve by

01 / Nov / 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 13, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050148

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 146i
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8		
Cylinder No. :	EB0143262		
Expiration Date :	Jun 21, 2024		

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.8	0.80	0.80	0.80
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.45

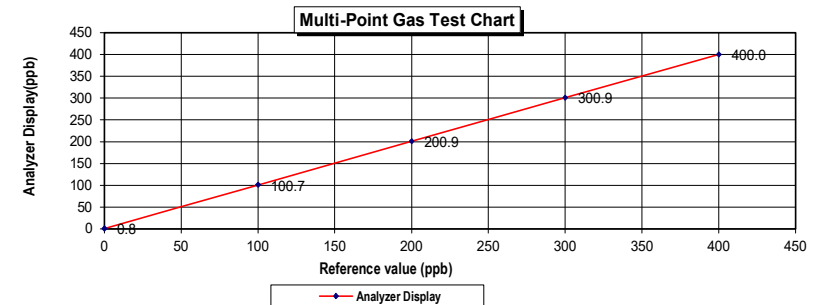

Calculate by

13 / Nov / 2023

Approve by

13 / Nov / 2023

MULTI-POINT GAS TEST REPORT

Test Date : Nov 1, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050149

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 21, 2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.6	0.60	0.60	0.60
Level 2	20.00%	100.0	100.8	0.80	0.79	0.79
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.40

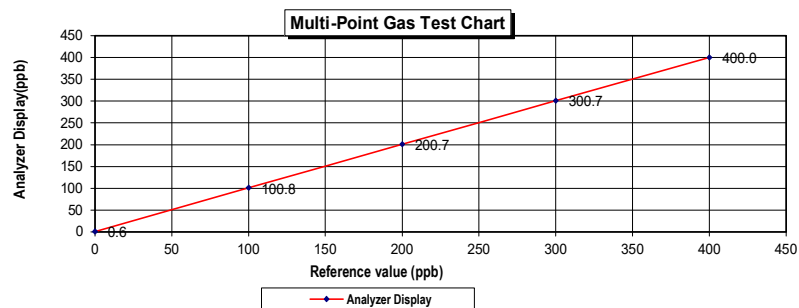

Calculate by

...../...../.....2023

Approve by

...../...../.....2023

MULTI-POINT GAS TEST REPORT

Test Date : Nov 1, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM19050150

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 21, 2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.70	0.70	0.70
Level 2	20.00%	100.0	100.6	0.60	0.60	0.60
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.38

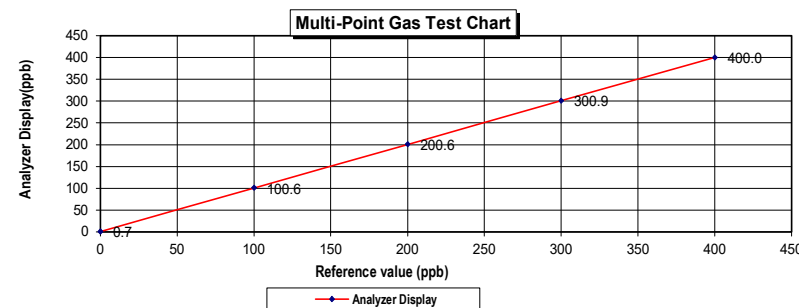

Calculate by

...../...../.....2023

Approve by

...../...../.....2023

MULTI-POINT GAS TEST REPORT

Test Date : Nov 21,2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM22177051

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 21,2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.9	0.90	0.90	0.90
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)			0.46

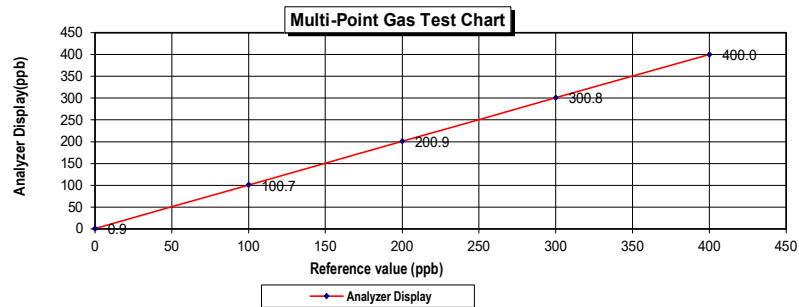

Calculate by

21 / Nov / 2023

Approve by

22 / Nov / 2023

MULTI-POINT GAS TEST REPORT

Test Date : Nov 7,2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM22387035

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 21,2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.5	0.50	0.50	0.50
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)			0.41

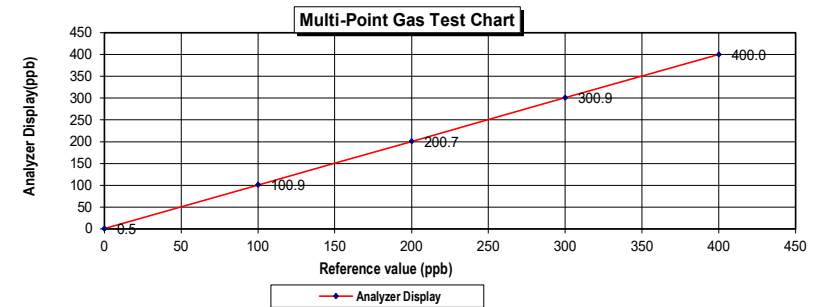

Calculate by

07 / Nov / 2023

Approve by

08 / Nov / 2023

MULTI-POINT GAS TEST REPORT

Test Date : Nov 7, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM22387039

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 21, 2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.9	0.90	0.90	0.90
Level 2	20.00%	100.0	100.9	0.90	0.89	0.89
Level 3	40.00%	200.0	200.7	0.70	0.35	0.35
Level 4	60.00%	300.0	300.8	0.80	0.27	0.27
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.48

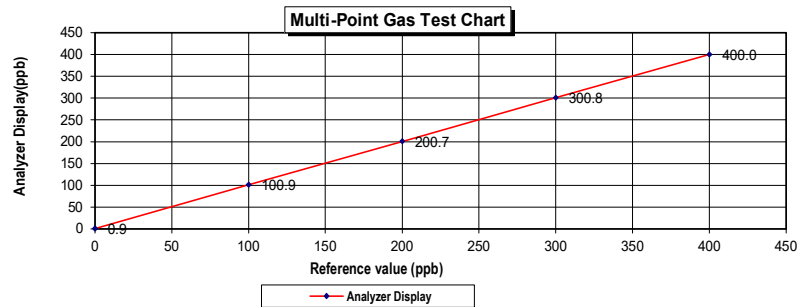

Calculate by

07 / Nov / 2023

Approve by

08 / Nov / 2023

MULTI-POINT GAS TEST REPORT

Test Date : Nov 7, 2023

Equipment : Gas Analyzer (NO₂) Model : 42i
Manufacturer : Thermo Scientific Serial Number : CM22387040

Standard Gas Concentration


Sulphur Dioxide (SO₂) 44.68 PPM
Nitric Oxide (NO) 45.94 PPM
Methane (CH₄) - PPM
Carbon Monoxide (CO) 984.8 PPM
Cylinder No. : EB0143262
Expiration Date : Jun 21, 2024

Dilutor Detail

Manufacturer : Thermo Scientific
Model : 146i
Serial Number : 1180540071

Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.8	0.80	0.80	0.80
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.9	0.90	0.30	0.30
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range		500.0 ppb	Average Difference (%)			0.42

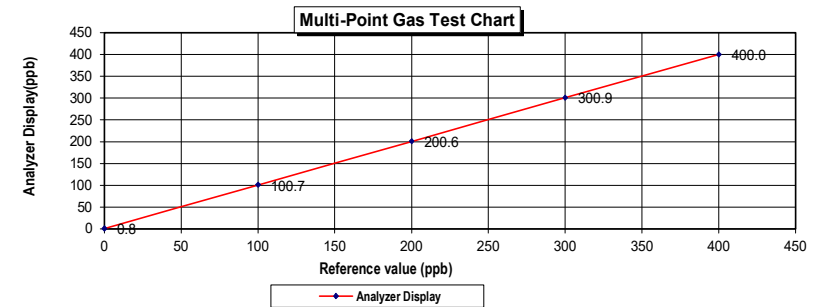

Calculate by

07 / Nov / 2023

Approve by

08 / Nov / 2023

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04N199E15A01D3 Reference Number: 122-402135187-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO2,BALN Certification Date: Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 6.7 megapascals

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.68 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20061120	CC708068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12388	D885025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505681	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	CC473277	46.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14080119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.5%	Nov 15, 2025

The SRM, PRM or GMIS noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 8700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 8700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 8700 AHR0801333 NO2	FTIR	Jun 03, 2021
Nicolet 8700 AHR0801333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



CERT 3082.01

เอกสารไม่ควบคุม

MULTI-POINT GAS TEST REPORT

Test Date : Nov 9, 2023

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : CM08140003

Standard Gas Concentration			Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer :	Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model :	146i
Methane (CH ₄)	-	PPM	Serial Number :	1180540071
Carbon Monoxide (CO)	984.8	PPM		
Cylinder No. :	EB0143262			
Expiration Date :	Jun 20, 2024			


Multi-point gas test data

Level	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.0	0.0
Level 2	20.00%	10.0	0.5	4.8	4.8
Level 3	40.00%	20.0	0.7	3.4	3.4
Level 4	60.00%	30.0	0.5	1.6	1.6
Level 5	80.00%	40.0	0.6	1.5	1.5

Remark : Measuring Range 50.0 ppm

Average Difference (%) 2.25

:Acceptable Limit \pm 5%

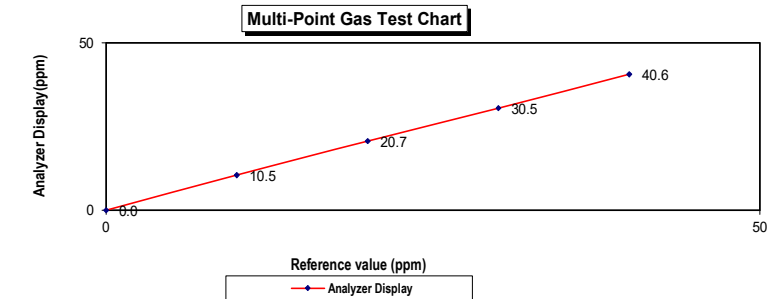

Calculate by

Approve by

8 / 11 / 2023

8 / Nov / 2023

MULTI-POINT GAS TEST REPORT


Test Date : Dec 8, 2023

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1180540068

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 146i
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No. :	EB0143262		
Expiration Date :	Jun 20, 2024		

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.7	0.7	0.7
Level 2	20.00%	10.0	10.8	0.8	7.4	7.4
Level 3	40.00%	20.0	20.7	0.7	3.4	3.4
Level 4	60.00%	30.0	30.6	0.6	2.0	2.0
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)			2.69

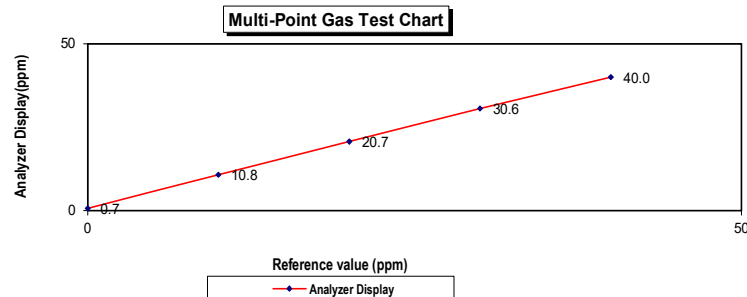

Calculate by

8 / 12 / 2023

Approve by

8 / Dec / 2023

MULTI-POINT GAS TEST REPORT


Test Date : Nov 13, 2023

Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1180540074

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 146i
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No. :	EB0143262		
Expiration Date :	Jun 20, 2024		

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.9	0.9	0.9	0.9
Level 2	20.00%	10.0	10.7	0.7	6.5	6.5
Level 3	40.00%	20.0	20.8	0.8	3.8	3.8
Level 4	60.00%	30.0	30.9	0.9	2.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)			2.84

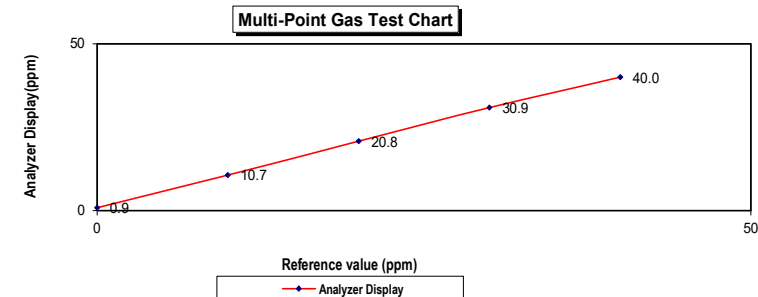

Calculate by

13 / 11 / 2023

Approve by

13 / Nov / 2023

MULTI-POINT GAS TEST REPORT


Test Date : Dec 8, 2023

Equipment : Gas Analyzer (CO) Model : APMA-370
Manufacturer : HORIBA Serial Number : YRLHTB7G

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 146i
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No. :	EB0143262		
Expiration Date :	Jun 20, 2024		

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.6	0.6	0.6	0.6
Level 2	20.00%	10.0	10.7	0.7	6.5	6.5
Level 3	40.00%	20.0	20.9	0.9	4.3	4.3
Level 4	60.00%	30.0	30.6	0.6	2.0	2.0
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)			2.68

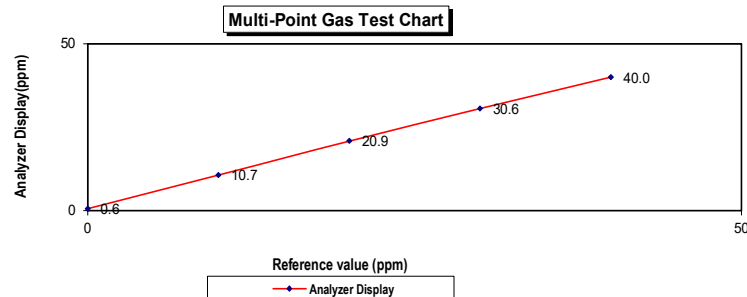

Calculate by

8 / 12 / 2023

Approve

8 / Dec / 2023

MULTI-POINT GAS TEST REPORT


Test Date : Dec 8, 2023

Equipment : Gas Analyzer (CO) Model : 48C
Manufacturer : Thermo Environmental Instruments Serial Number : 48C-65506-348

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 146i
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No. :	EB0143262		
Expiration Date :	Jun 20, 2024		

Multi-point gas test data

Reference Value (ppm)			Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.8	0.8	0.8	0.8
Level 2	20.00%	10.0	10.6	0.6	5.7	5.7
Level 3	40.00%	20.0	20.9	0.9	4.3	4.3
Level 4	60.00%	30.0	30.7	0.7	2.3	2.3
Level 5	80.00%	40.0	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)			2.61

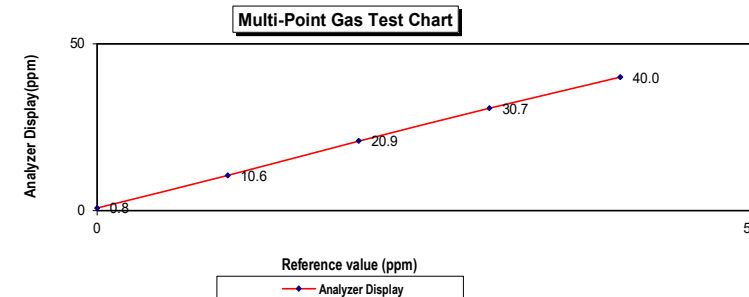

Calculate by

8 / 12 / 2023

Approve by

8 / Dec / 2023

MULTI-POINT GAS TEST REPORT

Test Date : Nov 13, 2023


Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : CM08140004

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 146i
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No. :	EB0143262		
Expiration Date :	Jun 20, 2024		

Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.8	0.8	0.8
Level 2	20.00%	10.0	10.7	6.5	6.5
Level 3	40.00%	20.0	20.9	4.3	4.3
Level 4	60.00%	30.0	30.7	2.3	2.3
Level 5	80.00%	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)		2.79

:Acceptable Limit $\pm 5\%$

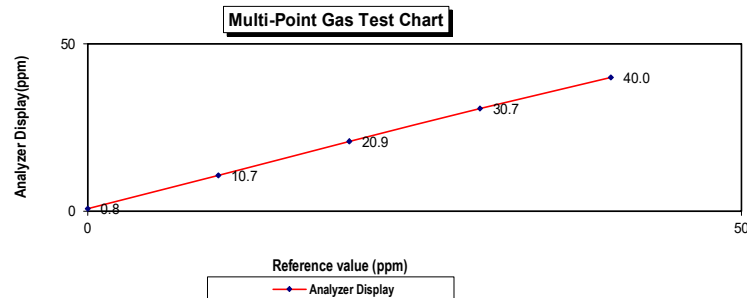

Calculate by

13 / 11 / 2023

Approve by

13 / Nov / 2023

MULTI-POINT GAS TEST REPORT

Test Date : Dec 18, 2023


Equipment : Gas Analyzer (CO) Model : 48i
Manufacturer : Thermo Scientific Serial Number : 1182920020

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 146i
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No. :	EB0143262		
Expiration Date :	Jun 20, 2024		

Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.7	0.7
Level 2	20.00%	10.0	10.9	8.3	8.3
Level 3	40.00%	20.0	20.7	3.4	3.4
Level 4	60.00%	30.0	30.7	2.3	2.3
Level 5	80.00%	40.0	0.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)		2.92

:Acceptable Limit $\pm 5\%$

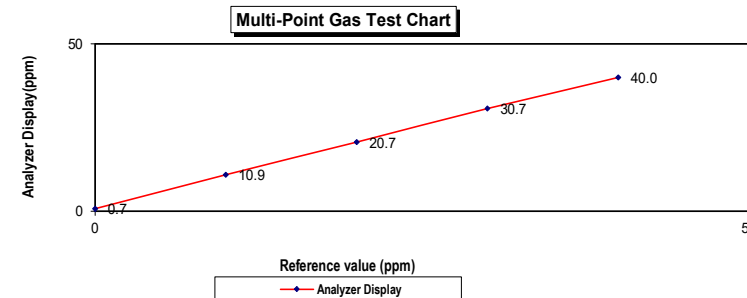

Calculate by

18 / 12 / 2023

Approve by

18 / Dec / 2023

MULTI-POINT GAS TEST REPORT

Test Date : Dec 8, 2023


Equipment : Gas Analyzer (CO) Model : 48C
Manufacturer : Thermo Environmental Instruments Serial Number : 48C-62460-335/5

Standard Gas Concentration		Dilutor Detail	
Sulphur Dioxide (SO ₂)	44.68	PPM	Manufacturer : Thermo Scientific
Nitric Oxide (NO)	45.94	PPM	Model : 146i
Methane (CH ₄)	-	PPM	Serial Number : 1180540071
Carbon Monoxide (CO)	984.8	PPM	
Cylinder No. :	EB0143262		
Expiration Date :	Jun 20, 2024		

Multi-point gas test data

	Reference Value (ppm)	Analyzer Display (ppm)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.7	0.7	0.7
Level 2	20.00%	10.0	10.8	0.8	7.4
Level 3	40.00%	20.0	20.8	0.8	3.8
Level 4	60.00%	30.0	30.9	0.9	2.9
Level 5	80.00%	40.0	40.0	0.0	0.0
Remark : Measuring Range		50.0 ppm	Average Difference (%)		2.97

:Acceptable Limit $\pm 5\%$

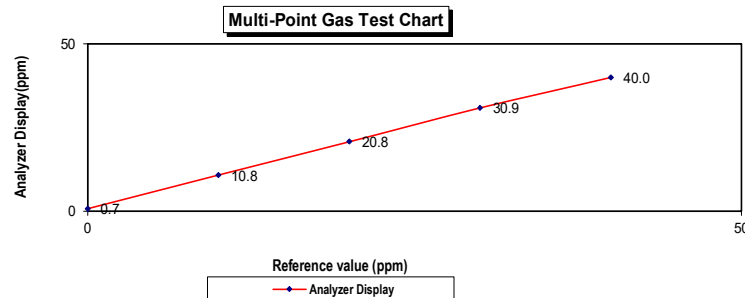

Calculate by

.....8...../.....12...../.....2023.

Approve by

.....8...../.....Dec...../.....2023

CERTIFICATE OF ANALYSIS

Grade of Product: EPA Protocol

Part Number: E04N199E15A01D3 Reference Number: 122-402135167-1
Cylinder Number: EB0143262 Cylinder Volume: 144.4 CF
Laboratory: 124 - Durham (SAP) - NC Cylinder Pressure: 2015 PSIG
PGVP Number: B22021 Valve Outlet: 660
Gas Code: CO,NO,NOX,SO₂,BALN Certification Date: Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a molefraction basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.68 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20061120	CC706068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D885025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	CC473277	48.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14080119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/- 0.5%	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 8700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 8700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 8700 AHR0801333 NO ₂	FTIR	Jun 03, 2021
Nicolet 8700 AHR0801333 SO ₂	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES: PO #5221002807

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

Approved for Release



CERT 3082.01

เอกสารไม่ควบคุม

เอกสาร 5-3

เอกสารการสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศในขบวน
และสถานีรถไฟ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

การเปรียบเทียบความถูกต้องของอุปกรณ์ Microbiological air sampler
(โดยเปรียบเทียบกับ Dry Cal Primary Flowmeter(Defender 510 High Flow) : S/N 136164)

ข้อมูลการเปรียบเทียบ			
เบอร์เครื่อง	: Microflow α 90C (No.B02)	วันที่ทำการเปรียบเทียบ	: 29/03/2024
Serial number	: G9CP M2861	อุณหภูมิ	: 24.7 °C
ยี่ห้อ	: AQUARIA	ความดันบรรยากาศ	: 1011 mmbar
รุ่น	: Microflow α 90C	ความชื้นสัมพัทธ์	: 50 %

แสดงการคำนวณ

$$Q(\text{std.}) = Q \times \frac{P}{(1.333224 \times 760) \times 10^3} \times \frac{298}{(T+273)}$$

Q = อัตราการไหลที่แท้จริงของอากาศขณะเปรียบเทียบ (mL/min)
Q (std.) = อัตราการไหลที่แท้จริงของอากาศที่สภาวะมาตรฐาน (lit/min)
P = ความดันบรรยากาศขณะเปรียบเทียบ (มิลลิบาร์)
T = อุณหภูมิอากาศขณะเปรียบเทียบ (องศาเซลเซียส)

ตารางแสดงค่าที่เปรียบเทียบ

DATA	Flow rate ที่อ่านได้ จากเครื่อง Microflow α 90C (lit/min)	Actual flow rate (ml/min)						Actual flow rate ที่อุณหภูมิและความดัน มาตรฐาน(Qstd.) (lit/min)
		ที่อุณหภูมิและความดันขณะเปรียบเทียบ (Q)						
		ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	ครั้งที่ 4	ครั้งที่ 5	เฉลี่ย	
1	30	29891	29895	29889	29896	29887	29891.60	29.86

ผู้ทำการเปรียบเทียบ

(นายอตุลย์ แดงกล่อม)

ผู้ตรวจสอบ

(นายยุทธนา ธารณาธรนิค)
หัวหน้าส่วนงานเก็บตัวอย่าง

ผู้รับรองผล

(นายพีระ เดชอุดม)
ผู้จัดการวิชาการ



บริษัท เอส.พี.เอส. คอนซัลติ้ง เซอร์วิส จำกัด
S.P.S. CONSULTING SERVICE CO., LTD.
7 ซอยพหลโยธิน 24 ถนนพหลโยธิน แขวงจอมพล เขตจตุจักร กรุงเทพฯ 10900
Tel : (662) 939-4370-72 Fax : (662) 513-4221 E-mail : sale@spscon.com, www.spscon.com

การเปรียบเทียบความถูกต้องของอุปกรณ์ Microbiological air sampler
(โดยเปรียบเทียบกับ Dry Cal Primary Flowmeter(Defender 510 High Flow) : S/N 136164)

ข้อมูลการเปรียบเทียบ			
เบอร์เครื่อง	: Microflow α 90C (No.B04)	วันที่ทำการเปรียบเทียบ	: 29/03/2024
Serial number	: G9ER M3095	อุณหภูมิ	: 24.7 °C
ยี่ห้อ	: AQUARIA	ความดันบรรยากาศ	: 1011 mmbar
รุ่น	: Microflow α 90C	ความชื้นสัมพัทธ์	: 50 %

แสดงการคำนวณ

$$Q(\text{std.}) = Q \times \frac{P}{(1.333224 \times 760) \times 10^3} \times \frac{298}{(T+273)}$$

Q = อัตราการไหลที่แท้จริงของอากาศขณะเปรียบเทียบ (mL/min)
Q (std.) = อัตราการไหลที่แท้จริงของอากาศที่สภาวะมาตรฐาน (lit/min)
P = ความดันบรรยากาศขณะเปรียบเทียบ (มิลลิบาร์)
T = อุณหภูมิอากาศขณะเปรียบเทียบ (องศาเซลเซียส)

ตารางแสดงค่าที่เปรียบเทียบ

DATA	Flow rate ที่อ่านได้ จากเครื่อง Microflow α 90C (lit/min)	Actual flow rate (mL/min)						Actual flow rate ที่อุณหภูมิและความดัน มาตรฐาน(Std.) (lit/min)
		ที่อุณหภูมิและความดันขณะเปรียบเทียบ (Q)						
		ครั้งที่ 1	ครั้งที่ 2	ครั้งที่ 3	ครั้งที่ 4	ครั้งที่ 5	เฉลี่ย	
1	30	29887	29894	29898	29890	29885	29890.80	29.85

ผู้ทำการเปรียบเทียบ

(นายอตุลย์ แดงกล่อม)

ผู้ตรวจสอบ

(นายยุทธนา ธารณาธรนิค)
หัวหน้าส่วนงานเก็บตัวอย่าง

ผู้รับรองผล

(นายพีระ เดชอุดม)
ผู้จัดการวิชาการ



ISOCAL TECHNOLOGY CO.,LTD.

Industrial Instrument Calibration Center

170/405 Moo 3 Serithai Rd., Kannayao Kannayao Bangkok 10230

Tel. 0-2906-3040-1 Fax. 0-2919-9948

Certificate of Calibration

Certificate Number : E23/0599B

Page : 1 of 3

Customer : S.P.S. Consulting Service Co.,Ltd.

7 Soi Phaholyothin 24, Phaholyothin Rd., Jompol,
Chatuchak, Bangkok 10900

Equipment Name : Hot Wire Anemometer

Model : 425

Serial No. : 02591869

ID No. : B02

Manufacture : Testo

Environment : Ambient Temperature (23 ± 2) °C

: Relative Humidity (50 ± 15) %

Location of Calibration : In-Lab

Date of Received : 19-Dec-2023

Date of Calibration : 20-Dec-2023

Date of Issued : 25-Dec-2023

Condition as Received : Normal

Calibration Method : Calibration Procedure Number WE-119

The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

This certificate is issued in accordance with ISO/IEC 17025:2017 and the conditions of accreditation granted by the Accreditation Body which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory, The result relate only to the item calibrated.

This certificate shall not be reproduced other than in full except without the prior written approval of the Head of Calibration Laboratory of Isocal Technology Co.,Ltd.

Calibrated by : Mr. Panya Darasom

Technical

Approved by :

(Mr. Narong Phetjaroon)



ISOCAL TECHNOLOGY CO.,LTD.

Calibration Report

Certificate Number : E23/0599B

Page : 2 of 3

Equipment Standards Used

Description	Serial No.	Traceability to	Certificate No.	Cal. Due Date
Anemometer	Q431637	SI Unit	L202304196-001	26-Apr-24

Definitions :-

* SI Unit - International System of Units



ISOCAL TECHNOLOGY CO.,LTD.

Calibration Report

Certificate Number : E23/0599B

Page : 3 of 3

Result of Calibration : Adjustment (No)

Function : Air Velocity Measurement

Standard Reading (m/S)	UUC Reading (m/S)	Error (m/S)	Uncertainty (m/S)
1.02	0.96	-0.06	0.15
2.02	1.96	-0.06	0.15
4.04	3.95	-0.09	0.20
6.05	5.95	-0.10	0.20
8.05	7.94	-0.11	0.20
10.07	9.94	-0.13	0.20
12.04	11.96	-0.08	0.20

... END ...



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CALIBRATION LABORATORY Co.,LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : HUMIDITY/TEMPERATURE DATA LOGGER
MANUFACTURER : HTI
MODEL / TYPE : HT-2000
SERIAL NO. : 2021020002298
CLID. NO. : 232100961
JOB CONTROL NO. : 230530057620

CUSTOMER : S.P.S. CONSULTING SERVICE CO., LTD.
7 SOI PHAHOLYOTHIN 24 ROAD., JOMPOL,
CHATUCHAK, BANGKOK 10900

DATE OF RECEIVED : 30 May 2023

DATE OF ISSUED : 02 June 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Tanawan Seenam-Ngoen
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
02 June 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the
International System of Units (SI)

Certificate No. Q23057620

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : HUMIDITY/TEMPERATURE DATA LOGGER
MANUFACTURER : HTI
MODEL / TYPE : HT-2000
SERIAL NO. : 2021020002298
DATE OF CALIBRATION : 01 June 2023

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$ Relative Humidity : $(55 \pm 10) \% \text{RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. WI-305-74. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 36151.
Temperature & Humidity Chamber, PGC Model 9141-5114 S/N.0802282.

TRACEABILITY :

The measurements are traceable to International System of Units (SI), through Thunder Scientific Corporation.
Certificate No. 21028, Due Date 09 December 2023.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2.00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23057620

F3-011-04/01-12

page 2 of 3



@clccalibration



CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring humidity/temperature data logger.

CALIBRATION DATA

1. CORRECTION OF TEMPERATURE

Test point (° C)	Actual Temperature (° C)	DUC Reading (° C)	Correction (° C)	Uncertainty ± (° C)
20.0	20.01	20.1	-0.09	0.40
25.0	25.01	25.0	+0.01	
30.0	30.00	29.9	+0.10	

2. CORRECTION OF HUMIDITY

STD Temperature (° C)	STD Reading (%RH)	DUC Reading (%RH)	Correction (%RH)	Uncertainty ± (%RH)
25	35.00	46.5	-11.50	1.20
25	50.00	58.4	-8.40	1.20
25	64.99	72.2	-7.21	1.40

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 48 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23057620

F3-011-04/01-12

page 3 of 3



@clccalibration

เอกสาร 5-4

เอกสารการสอบเทียบเครื่องมือตรวจวัดระดับเสียง



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0304

MTC No. EEL. BP. 109/0267

CALIBRATION CERTIFICATE

Submitted by : S.P.S.Consulting Service Co.,Ltd.

Address : 7 Soi Phaholyothin 24, Phaholyothin Road, Jompol, Chatuchak, Bangkok 10900.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : ACO

Model : 2127

Serial No. : 130006

Standards used : 1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.

2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.

3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.

4. Digital Multimeter Agilent 34401A S/N MY44005560.

5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.

6. Audio Analyzer Keithley 2015-P S/N4106495.

7. Condenser Microphone B&K 4180 S/N 2889871.

Ambient Environment

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

Calibration Procedure: CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 22 Feb. 2024

Date of Calibration : 4 Mar. 2024

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0304

MTC No. EEL. BP. 109/0267

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20μPa at 1000 Hz

Acoustic Output in dB re 20μPa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	93.85	-0.15	± 0.10	±0.75 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	999.9	-0.1	± 1.5	±2.0%

3. Total Distortion

Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 2
1/2 inch Bruel&Kjaer 4180	1.65	± 0.50	±4.0%

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

(Mr.Weerachai Deechaiyae)

Approved by :

(Mr.Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 4 Mar. 2024

Date of Issue : 5 Mar. 2024

Ref : 2011267022200795001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Head Office
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office
196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

Noise B_112/24

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	04 March 2024
		Due Date	04 March 2025

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B03	ACO	6236	00222297	18 April 2024	93.9	93.9
ACO-B18	ACO	6236	00172048	18 April 2024	94.0	93.9
ACO-B28	ACO	6236	00182009	18 April 2024	94.0	93.9
ACO-B29	ACO	6236	00182011	18 April 2024	93.9	93.9
ACO-B33	ACO	6236	00182015	18 April 2024	93.9	93.9
ACO-B41	ACO	6236	00192032	18 April 2024	94.0	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.85 ± 0.10 dB	

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)

Noise B_107/24

Sound Level Meter Calibration Report

Acoustic Calibrator Data

Brand	ACO	Number	AC 03/56
Model	2127	Serial No.	130006
Calibration Range	94 dB, 1000 Hz	Last Calibration	04 March 2024
		Due Date	04 March 2025

Calibration Data

Sound Level Meter Data				Calibration Data		
SLM No.	Brand	Model	Serial No.	Date	Actual Reading [dB]	
					Before Adjustment	After Adjustment
ACO-B46	ACO	6236	00222305	18 April 2024	94.0	93.9
Acoustic Certified Value : Thailand Institute of Scientific and Technological Research (TISTR)					93.85 ± 0.10 dB	

Calibrated by :

(Mr. Adul Dangklom)

Approved by :

(Mr. Peera Detudom)

เอกสาร 5-5

เอกสารสอบเทียบเครื่องมือตรวจวิเคราะห์น้ำ



CERTIFICATE No : 24E0681
REFERENCE No : 71961-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : DKK TOA
MODEL : HM-25R
SERIAL No : 760205
ID No : EQL-183
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT D.
CALIBRATION DATE : 23-Jan-24

APPROVED BY : PONGVAK J.

ISSUED DATE : 24-Jan-24

RECEIVED DATE : 23-Jan-24

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.



CERTIFICATE No : 24E0681

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : DKK TOA
ID No : EQL-183
RECEIVED DATE : 23-Jan-24
AMBIENT TEMPERATURE : 25° C ± 1° C
MODEL : HM-25R
SERIAL NUMBER : 760205
CALIBRATION DATE : 23-Jan-24
RELATIVE HUMIDITY : 50 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

- THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062 AND WI-TQ-063. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER SOLUTION.
- REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-06	CC767907	4880-13836406	29-Dec-24
2) pH STANDARD SOLUTION	00651-08	CC765602	4881-13757019	18-Nov-24
3) pH STANDARD SOLUTION	00651-10	CC767180	4882-13813369	14-Dec-24
4) PROCESS CALIBRATOR	CA150	91S6079	23E1312	19-Apr-24
5) BATH	260014	1247 48074	23T9014	13-Sep-24
6) THERMOMETER WITH PROBE	421504	55000379	23T9623	13-Sep-24

- THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
- THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
- THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
 - NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

- DISPLAY UNIT ONLY

SLOPE FACTOR $k = 2.303 \text{ RT/F} = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
177.48	178	-0.52	0.59	2.0
0.00	1	-1.00	0.59	2.0
-177.48	-177	-0.48	0.59	2.0

- DISPLAY UNIT WITH pH ELECTRODE S/N: 202F0138MK

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.0061	4.01	-0.004	0.013	2.0
6.9994	7.00	-0.001	0.013	2.0
10.0070	10.01	-0.003	0.014	2.0

- PERCENT SLOPE 97%

- DISPLAY UNIT MEASUREMENT TEMPERATURE WITH PROBE

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	UNCERTAINTY OF MEASUREMENT (± °C)
24.999	25.0	80	-0.001	0.21

UUC : UNIT UNDER CALIBRATION

THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY M
FACTOR k, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 23E3129
REFERENCE No : 68715-2

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : pH METER
MANUFACTURER : TOA-DKK
MODEL : HM-41X
SERIAL No : 784878
ID No : EQL-199
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT D.
CALIBRATION DATE : 29-Mar-23

APPROVED BY : PONGSAK J.

ISSUED DATE : 30-Mar-23

RECEIVED DATE : 29-Mar-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV 02



CERTIFICATE No : 23E3129

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : pH METER
MANUFACTURER : TOA-DKK
ID No : EQL-199
RECEIVED DATE : 29-Mar-23
AMBIENT TEMPERATURE : 25° C ± 1° C
MODEL : HM-41X
SERIAL NUMBER : 784878
CALIBRATION DATE : 29-Mar-23
RELATIVE HUMIDITY : 49 %RH ± 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY DIRECT MEASUREMENT METHOD BASED ON WI-TQ-062. THE DISPLAY UNIT WAS TESTED BY GENERATING STANDARD VOLTAGE TO THE UNIT AND READ THE VALUE COMPARED WITH CALCULATED VALUE. THE DISPLAY AND ELECTRODE WAS CALIBRATED BY USING STANDARD pH BUFFER SOLUTION.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No/ LOT No	CERTIFICATE No	DUE DATE
1) pH STANDARD SOLUTION	00651-06	CC719181	4880-12119147	05-Apr-23
2) pH STANDARD SOLUTION	00651-08	CC718727	4881-12110709	31-Mar-23
3) pH STANDARD SOLUTION	00651-10	CC747845	4882-13159657	02-Mar-24
4) PROCESS CALIBRATOR	CA150	91S6079	22E1145	31-Mar-23
5) BATH	260014	1247 48074	22T9870	13-Sep-23
6) THERMOMETER WITH PROBE	421504	55000379	22T9904	13-Sep-23

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO SI UNIT MAINTAINED AT :-
- NATIONAL INSTITUTE OF STANDARD AND TECHNOLOGY, USA.
- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

1. DISPLAY UNIT ONLY

SLOPE FACTOR $k = 2.303 \text{ RT/F} = 59 \text{ mV/pH}$

mV APPLIED	UUC READING (mV)	CORRECTION (mV)	UNCERTAINTY OF MEASUREMENT (± mV)	COVERAGE FACTOR k
177.48	177	0.48	0.59	2.0
0.00	0	0.00	0.59	2.0
-177.48	-178	0.52	0.59	2.0

2. DISPLAY UNIT WITH pH ELECTRODE S/N: N/A

STANDARD pH BUFFER SOLUTION (pH)	UUC READING (pH)	CORRECTION (pH)	UNCERTAINTY OF MEASUREMENT (± pH)	COVERAGE FACTOR k
4.007	4.01	-0.003	0.013	2.0
7.003	7.00	0.003	0.013	2.0
10.003	10.01	-0.007	0.014	2.0

3. PERCENT SLOPE 95%

4. DISPLAY UNIT MEASUREMENT TEMPERATURE WITH PROBE

STANDARD READING (°C)	UUC* READING (°C)	IMMERSION DEPTH (mm)	CORRECTION (°C)	UNCERTAINTY OF MEASUREMENT (±°C)
25.002	25.0	80	0.002	0.21


UUC : UNIT UNDER CALIBRATION

THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k , PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT

Certificate of Calibration

Date of Issue : 21 August 2023
Certificate No. : 231872/ME
Customer Company : Test Tech Co., Ltd.
30,32 Rama II Soi 63, Rama II Rd., Samaedam,
Bangkhunthian, Bangkok 10150
Instrument Manufacturer : Metrohm
Instrument Type : pH meter
Model : 781
Instrument Serial Number : 1781001011219 (ID : EQL-131)
Calibration Place : Laboratory, Test Tech Co., Ltd.
30,32 Rama II Soi 63, Rama II Rd., Samaedam,
Bangkhunthian, Bangkok 10150
Environment Status : Temperature : $22.65^{\circ}\text{C} \pm 0.15^{\circ}\text{C}$
Humidity : $63.25\% \pm 2.75\%$
Date of Receipt : 18 August 2023
Date of Calibration : 18 August 2023
Job Number : CAL230577/ME
Condition of Calibration Item : Used Item
Result of Calibration : ☒ Without Adjustment ☐ Adjustment
Calibrated By : Mr. Monton Tontun
Approved By : 
Authorized Signatory
☐ Mr. Kowit Photaeng
☒ Mr. Patipon Musigapala
☐ Mr. Teerayut Cheepdamrong

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the issuing Laboratory Metrohm Siam Ltd.

Calibration Report

Certificate No: 231872/ME

1. Reference Standards

Item	Description/Model	Serial No.	Manufacturing	Certificate No.	Due Date
1	Digital Multimeter 34401A	MY41054280	Agilent	E1U231457	25 Mar 2024
2	Multifunction Calibrator MC3	30328644	Beamex	CAL0252-22P0214	15 Nov 2023
3	Temperature and Humidity Logger	62225348	Ebro	L202209318-001	28 Sep 2023

2. The measurement standards are traceable to International system of units (SI) by mean of an unbroken chain of calibration via accredited calibration laboratory, National or International metrology institute.

3. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

4. The results of test were found accurate as shown on date and place of test only.

5. Procedure Used :

- On-site method WI-02 by substitute measurement with digital multimeter (DC Voltage)
- On-site method WI-02 based on BS 3145 : 1978 (pH)
- On-site method WI-02 based on CEI IEC 751 : 1983 (Temperature)

6. The calibration results apply only accuracy of display unit pH meter. User shall be electrode test and calibrate pH meter with traceability standard buffer.

Calibration Report

Certificate No: 231872/ME

1. Input I (DC Voltage)

Range (mV)	¹ STD Setting (mV)	² Tolerance (mV)	³ UUC Reading (mV)	Uncertainty (± mV)
2 V	0.00	-1.0 to 1.0	0.1	0.092
	300.00	299.0 to 301.0	300.0	0.12
	600.00	599.0 to 601.0	599.9	0.14
	900.00	899.0 to 901.0	899.9	0.15
	1900.00	1899.0 to 1901.0	1899.7	0.19
	-1900.00	-1901.0 to -1899.0	-1899.7	0.19

2. Input I (pH)*

¹ STD Setting (mV)	Nominal Value (pH)	² Tolerance (pH)	³ UUC Reading (pH)	Uncertainty (± pH)
414.12	0	-0.017 to 0.017	0.001	0.0019
354.96	1	0.983 to 1.017	1.001	0.0018
295.80	2	1.983 to 2.017	2.000	0.0015
236.64	3	2.983 to 3.017	3.000	0.0013
177.48	4	3.983 to 4.017	4.000	0.0011
118.32	5	4.983 to 5.017	5.000	0.0009
59.16	6	5.983 to 6.017	5.999	0.0008
0.00	7	6.983 to 7.017	7.000	0.0010
-59.16	8	7.983 to 8.017	7.999	0.0008
-118.32	9	8.983 to 9.017	8.999	0.0009
-177.48	10	9.983 to 10.017	9.999	0.0011
-236.64	11	10.983 to 11.017	10.998	0.0013
-295.80	12	11.983 to 12.017	11.998	0.0015
-354.96	13	12.983 to 13.017	12.998	0.0017
-414.12	14	13.983 to 14.017	13.997	0.0019

Reference Temperature : 25° C

Calibration Report

Certificate No: 231872/ME

3. Temperature PT-1000 (385)

¹ STD Setting (Ω)	Nominal Value (°C)	² Tolerance (°C)	³ UUC Reading (°C)	Uncertainty (± °C)
1000.0	0	-0.5 to 0.5	0.0	0.18
1077.9	20	19.5 to 20.5	20.0	0.18
1097.3	25	24.5 to 25.5	24.9	0.18
1116.7	30	29.5 to 30.5	30.0	0.18
1194.0	50	49.5 to 50.5	50.0	0.22
1385.1	100	99.5 to 100.5	99.9	0.22

Remark:

- ¹STD = Standard Equipment.
- ²Tolerance according to manufacturer specification and service manual.
- ³UUC = Unit Under Calibration.
- The result as per (*) marked are not TISI Accreditation Scope.

End of data



CERTIFICATE No : 23M6754
REFERENCE No : 69854-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : BP210S
SERIAL No : S0736477
ID No : EQL-008
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD.,
SAMAEDAM, BANGKHUNTHIAN, BANGKOK
10150

CALIBRATED BY : PRASERT D.
CALIBRATION DATE : 13-Jul-23

APPROVED BY : PONGSAK J.
ISSUED DATE : 17-Jul-23
RECEIVED DATE : 13-Jul-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV 03



CERTIFICATE No : 23M6754

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BP210S
MANUFACTURER : SARTORIUS S/N : S0736477
ID No : EQL-008 RECEIVED DATE : 13-Jul-23
AIR PRESSURE : 1011mbar \pm 1mbar CALIBRATION DATE : 13-Jul-23
AMBIENT TEMPERATURE : 23°C \pm 1°C RELATIVE HUMIDITY : 50 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING INTERNAL WEIGHT TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN. THE INTERNAL WEIGHT WAS CHECKED BY USING

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	49.9999	0.0001	0.00012
100.0	99.9999	0.0001	0.00019
200.0	199.9997	0.0003	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9998
2	99.9997
3	99.9998
4	99.9998
5	99.9998
OFF-CENTER LOADING	0.0001

6. INTERNAL WEIGHT ERROR : 0.000499999999988177 g

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY OF MEASUREMENT
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 23M8800
REFERENCE No : 70515-8

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : AND
MODEL : GR-200
SERIAL No : 14243876
ID No : EQL-130
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : PRASERT P.
CALIBRATION DATE : 11-Sep-23

APPROVED BY : PONGSAK J.
ISSUED DATE : 15-Sep-23
RECEIVED DATE : 11-Sep-23



CERTIFICATE No : 23M8800

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : GR-200
MANUFACTURER : AND S/N : 14243876
ID No : EQL-130 RECEIVED DATE : 11-Sep-23
AIR PRESSURE : 1011mbar \pm 1mbar CALIBRATION DATE : 11-Sep-23
AMBIENT TEMPERATURE : 24° C \pm 1° C RELATIVE HUMIDITY : 50 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	15843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-


- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

- ZERO SETTING FUNCTION : NORMAL
- TARE FUNCTION : NORMAL
- REPEATABILITY OF READING AT 200 g WAS 0 g
- DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0000	0.0000	0.000094
50.0	50.0000	0.0000	0.00012
100.0	100.0000	0.0000	0.00019
200.0	200.0000	0.0000	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	100.0000
2	100.0001
3	100.0001
4	99.9999
5	100.0001
OFF-CENTER LOADING	0.0001

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



CERTIFICATE No : 23M11118
REFERENCE No : 71188-2


PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : BCA3202I-1S
SERIAL No : 0039407364
ID No : EQL-257
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD.,
SAMAEDAM, BANGKHUNTHIAN, BANGKOK
10150

CALIBRATED BY : PRASERT D.

CALIBRATION DATE : 09-Nov-23

APPROVED BY :  PONGSAK J.

ISSUED DATE : 13-Nov-23

RECEIVED DATE : 09-Nov-23



CERTIFICATE No : 23M11118

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE MODEL : BCA3202I-1S
MANUFACTURER : SARTORIUS S/N : 0039407364
ID No : EQL-257 RECEIVED DATE : 09-Nov-23
AIR PRESSURE : 1010mbar \pm 1mbar CALIBRATION DATE : 09-Nov-23
AMBIENT TEMPERATURE : 23°C \pm 1°C RELATIVE HUMIDITY : 49 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS NOT ADJUSTED BEFORE CALIBRATION. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	---	0094-51	23M1296	07-Feb-24
2) STANDARD WEIGHT	---	QK-I-009	23M1297	07-Feb-24
3) STANDARD WEIGHT	---	QK-I-010	M2302003S	01-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND)

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 2500 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.00	0.00	0.012
10.0	10.00	0.00	0.012
20.0	20.00	0.00	0.012
50.0	50.00	0.00	0.012
100.0	100.00	0.00	0.012
200.0	200.00	0.00	0.012
500.0	500.00	0.00	0.012
700.0	700.00	0.00	0.012
1000.0	1000.00	0.00	0.012
2000.0	2000.00	0.00	0.012
3000.0	3000.00	0.00	0.012


5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	1000.00
2	1000.00
3	1000.00
4	1000.00
5	1000.00
OFF-CENTER LOADING	0.00

NOTE : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A
COVERAGE FACTOR $k=2$, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



Certificate of Calibration

Equipment: Balance
Model: BCA2241-1S
Serial No. (or ID.): 0043402017 (EQL - 268)
Manufacturer: Sartorius
Condition: New

Certificate No.: C01232449
Issued Date: 08 July 2023
Job No.: KSPR2310693
Page: 1 of 2

Customer: TEST TECH CO., LTD.
 30,32 Rama II Soi 63, Rama II Rd.,
 Samaedam, Bangkhuntien Bangkok 10150 Thailand.

Environment Condition: Temperature 23 °C ± 0.4 °C
 Humidity 59 %RH ± 4.2 %RH

Calibration Place: TEST TECH CO., LTD. (302 Room)
 30,32 Rama II Soi 63, Rama II Rd.,
 Samaedam, Bangkhuntien Bangkok 10150 Thailand.

Calibration By: Mr. Hattapong Pumnil

Calibration Date: 07 July 2023

The Method used: In-house method, CAL-WI-47, based on UKAS Lab 14

Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Co., Ltd. Certificate No. C02220533

(Mr. Hattapong Pumnil)

Person in charge

(Mr. Rungrod Jenkitrakulchai)

Authorized signatory

This certificate is issued the units of measurement according to the international System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
 DKSH Technology Limited
 2533 ถนนสุขุมวิท แขวงคลองตันเหนือ เขตวัฒนา กรุงเทพมหานคร 10260
 2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
 Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-C01-14: 12 Sep 20:




Certificate No.: C01232449

Page: 2 of 2

Calibration Results:

Without Adjustment

Eccentric Error: Weight to be 1/3 or 1/2 of Maximum capacity, taken from the center of the pan as a zero reference.

			Nominal Test Value 100 (g)				
Reference Points (g)							
A	B	C	D	E			
-	0.0000	0.0000	-0.0001	-0.0001			

Repeatability: Determination of the standard deviation of weighing balance., Readability 0.0001 (g)

Nominal test value (g)	Standard Deviation
20	0.00004
200	0.00005

Error of indication from nominal or conventional mass value., Readability 0.0001 (g)

Nominal Value (g)	Conventional Mass (g)	Displayed Value (g)	Error of Indication (g)	Uncertainty (g)	k
0.001	0.00100	0.0010	0.0000	0.00010	2.03
0.01	0.01000	0.0100	0.0000	0.00010	2.03
0.1	0.10001	0.1000	0.0000	0.00010	2.03
0.5	0.50000	0.5000	0.0000	0.00010	2.03
1	1.00001	1.0000	0.0000	0.00010	2.03
2	2.00002	2.0000	0.0000	0.00010	2.03
5	5.00002	5.0000	0.0000	0.00011	2.03
10	10.00002	10.0000	0.0000	0.00011	2.03
20	20.00000	20.0000	0.0000	0.00011	2.02
25	25.00003	25.0000	0.0000	0.00012	2.02
50	49.99996	50.0000	0.0000	0.00013	2.01
100	100.00002	100.0000	0.0000	0.00017	2.00
120	120.00002	120.0000	0.0000	0.00021	2.00
150	149.99998	150.0000	0.0000	0.00023	2.00
200	200.00004	200.0000	0.0000	0.00029	2.00

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
 DKSH Technology Limited
 2533 ถนนสุขุมวิท แขวงคลองตันเหนือ เขตวัฒนา กรุงเทพมหานคร 10260
 2533 Sukhumvit Road, Bangkok, Phrakhanong, Bangkok 10260
 Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-C01-14: 12 Sep 20

การดูแลบำรุงรักษาเชิงป้องกัน

Preventive Maintenance



ซ15

ใบรับรองการทวนสอบ "เครื่องกลั่นไนโตรเจน"

(Calibration Certificate of Distillation Unit VAPODEST

VAP20, VAP30s)



บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

ฝ่ายบริการหลังการขาย

โทร 0 2 639 7000 E-mail: service.rec.d@dksh.com

ฝ่ายขายและการตลาด

โทร 0 2 639 7000 E-Mail : marketing.tha.d@dksh.com

Website : www.dksh.co.th/technology/solutions/thailand

เงื่อนไขการให้บริการ Preventive Maintenance

บริษัทฯ จะส่งวิศวกรผู้ชำนาญ เพื่อให้บริการตามขอบข่ายของการบริการ เฉพาะ ในวันและเวลา ราชการ หากมีความประสงค์ที่จะรับบริการนอกเหนือจากวัน เวลา ราชการ (วันหยุดเสาร์ – อาทิตย์ หรือวันหยุด น้อดังกล่าว) บริษัทฯ จะคิดค่าบริการเพิ่มเติมตามอัตราที่กฎหมายแรงงานกำหนดไว้

ขอบข่ายการบริการ

- ตรวจสอบสภาพการทำงานต่าง ๆ ของเครื่องมือ
- ทดสอบประสิทธิภาพการทำงานของเครื่องมือ
- รายการผลการตรวจสอบเครื่องมือ

หมายเหตุ

- ราคาไม่รวมถึงค่าบริการซ่อม หรือ เปลี่ยนอะไหล่ที่ชำรุดเสียหาย หรือหมดสภาพการใช้งาน
- ในกรณีที่ผู้รับบริการนอกเขตพื้นที่ให้บริการ บริษัทฯ จำเป็นต้องคิดค่าใช้จ่ายเพิ่มเติม ได้แก่ ค่าเดินทาง เป็นต้น
- บริษัทฯ ขอสงวนสิทธิ์ในการเปลี่ยนแปลงราคา โดยไม่แจ้งให้ทราบล่วงหน้า

ช่องทางการติดต่อ



DKSH Technology Limited (บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด)
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260
เลขประจำตัวผู้เสียภาษี 010-555-001-4547 (สำนักงานใหญ่)



LINE @dkshscientific



Call center 0 2 639 7000



DKSH Scientific



www.dksh.com/scientific-thailand



marketing.thai@dksh.com



@dkshscientific

Preventive Maintenance Contract

จำนวนในการทำสัญญาบริการ ...ครั้ง ต่อปี
ครั้งที่ 1 วันที่ 27/03/2024

รายละเอียดผู้รับบริการ

หน่วยงาน	บริษัท เทสท์ เทคโนโลยี จำกัด		
ที่อยู่	30,32 ซอยพระรามที่ 2 ซอย 63 ถนนพระรามที่ 2 แขวงสามค่า เขตบางขุนเทียน กรุงเทพมหานคร 10150		
โทรศัพท์	0-2893-4211-7	แฟกซ์	0-2893-4218

ผู้ติดต่อ

ชื่อ - นามสกุล	คุณกรรณก ชุมพิทักษ์		
ตำแหน่ง	หัวหน้าส่วน		
โทรศัพท์	087 398 9274	เบอร์ติดต่อ	-
E-mail	lab_center@testtech.co.th		

รายละเอียดผู้ให้บริการ

บริษัท ดิเคอเอส เทคโนโลยี จำกัด (ฝ่ายบริการหลังการขาย) (สำนักงานใหญ่)	
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260	
โทรศัพท์ 0 2 693 7000 Email: sudat.sk@dksh.com	
เจ้าหน้าที่ประสานงาน : คุณสุภารัตน์ ศิริรัตน์ โทรศัพท์ 090 678 6925	
เจ้าหน้าที่ผู้ให้บริการ	นายจิรายุช ผลิตอด
ตำแหน่ง	Specialist, Technical Service.
โทรศัพท์	0938138736
E-mail	Jirayut.js@dksh.com


ลงนามผู้รับบริการ		ลงนามผู้ให้บริการ	
ตัวบรรจง		ตัวบรรจง	(นายจิรายุช ผลิตอด)
ตำแหน่ง	หัวหน้าส่วนภาคกลางฝั่ง 2	ตำแหน่ง	Specialist, Technical Service.
วันที่ / ประทับตราบริษัท	27/03/2024	วันที่ / ประทับตราบริษัท	27/03/2024

JOB No: LSPR2402246 MODEL: Ysp30 S/N: GER003718

Part 1: Operational Qualification (OQ)


ตรวจสอบสภาพเครื่อง

FRONT

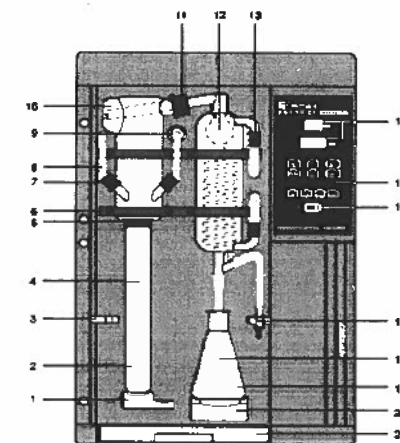

	Pass	Fail	N/A	Remark
1. Quick clamping device with wedge	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
2. Kjeldatherm digestion tube	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
3. Holder for steam inlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
4. PTFP-Inlet tubing, steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
5. Viton-cone	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
6. Clamping for glassware	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
7. Screw cap GL18 with silicone seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
8. PTFP-Inlet tubing, NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
9. PP-Distributor with PP-threaded joint	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
10. Distribution head, glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
11. Screw cap GL32 with silicone seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
12. Distillation condenser	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
13. Screw cap GL14 with plastic screw connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
14. Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
15. Keyboard, chemical-resistant	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
16. Main switch, green	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
17. Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
18. Distillate outlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
19. Erlenmeyer flask	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
20. Platform	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
21. Drip tray	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	

REAR

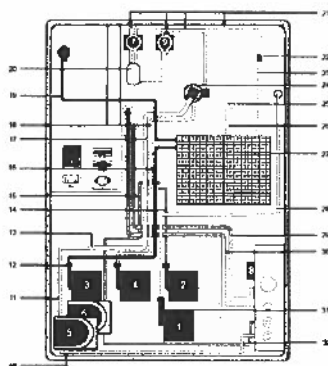

	Pass	Fail	N/A	Remark
1. Diaphragm pump NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2. Diaphragm pump H_3BO_3	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
3. Diaphragm pump H_2O for steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4. Diaphragm pump H_2O for sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
5. Peristaltic pump for suction sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
6. Peristaltic pump for suction receiver	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option
7. Pinch-solenoid valve, steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8. Magnetic valve with pressure control	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9. Pinch-solenoid valve, shut-off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10. Verprene-tubing 4x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11. Verprene-tubing 4x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
12. Non-return valve for diaphragm pumps	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13. Tubing reduction PP 51x10x5 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
14. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
15. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option
16. Silicone -tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17. Verprene-tubing 8x12 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
18. Verprene tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
19. Silicone tubing 4x7 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20. Ventilation glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21. Novoprene-tubing 4.8x8 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22. Tubing reduction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23. Silicone tubing 6x10 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
24. PP-distributor with PP-thread	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
25. SKT-valve (built in with brass fitting)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
26. Silicone tubing 8x16x80 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27. Steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
28. PTFE-inlet tubing NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29. Silicone tubing 8x16 for cooling water inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
30. Silicone tubing 8x16 for cooling water outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
31. Viton-tubing 6x12*50 mm.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
32. Silicone tubing 4x7 mm.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	option

2 รายละเอียดการตรวจสอบ

2.1 ขั้นตอนการบริการ

ตรวจสอบระบบไฟฟ้า (Electrical Test)

- ความต้านทานทางไฟฟ้าของเครื่องกับกราวด์
- กระแสไฟฟ้าใช้งาน

ตรวจสอบสภาพเครื่อง (Optical Test)

- Main cable
- Electric wiring
- Pumps
- Distribution Head
- Condensor
- Steam generator
- Tubing
- Viton code

ตรวจสอบ Function การทำงาน (The Function Test)

- ระบบสร้างและควบคุมความดันของ Steam
- ระบบการเติมน้ำเข้า Sample Tube
- ระบบการเติม Na OH
- ระบบการ Suction ค้าง Sample Tube และ Receiver

2.2 รายงานผลการให้บริการ

1. TECHNICAL DATA

	Pass	Fail	N/A	Remark
Main Supply 220 volt + 10% 50 Hz with ground	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Normal current	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>6A.....

1.1 COOLING WATER BATH

	Pass	Fail	N/A	Remark
Temperature 15-20 °C	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Control Temperature	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

1.2 OPTICAL TEST VAP30....

	Pass	Fail	N/A	Remark
Screw cap GL14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Screw cap GL18	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Screw cap GL32	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Distillation Head	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Condensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Viton Cone	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ventilation Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Micro Switch Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

2. SYSTEM COOLING WATER INLET

	Pass	Fail	N/A	Remark
Cooling Water Inlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Cooling Water Outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Magnetic valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

3.SYSTEM CONTROL

	Pass	Fail	N/A	Remark
Key Board	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Program	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Adding H ₂ O	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only
Adding NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Adding H ₃ BO ₃	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	vap 40 only
Suction Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	vap 30,40 only

4.SYSTEM DISTILLATION

	Pass	Fail	N/A	Remark
Boiler	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Level Sensor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Novprene-Tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Solenoid Valve Shut-Off	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Solenoid Valve Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Excess Pressure Detector	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ventilation Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Heater	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

5. PUMP

	Pass	Fail	N/A	Remark
Pump H ₂ O Steam	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Pump H ₂ O Sample	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Pump NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
- Non-Return Valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Pump H ₃ BO ₃	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
- Non-Return Valve	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Pump Suction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

6. The Following Program Run :

	Pass	Fail	N/A	Remark
Addition H ₂ O 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Addition NaOH 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Addition H ₃ BO ₃ 0-99 sec.	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Reaction Time 0-99 min.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Distillation Time 0-99 min	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Steam Capacity 30%-100%	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Suction Time 0-99 sec.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
The Instrument is in perfect technical shape	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Remark :

.....

.....

Part 3: ข้อมูลสนับสนุนด้านเทคนิค (General Technical Support)

3.1 การบำรุงรักษาทั่วไป (Basic maintenance)

Cleaning

Glass parts and suction pump should be cleaned before long periods of non-usage (i.e. holidays). This way blockages caused by crystalline deposits are avoided.

The following program should be run:

Addition H_2BO_3	0	s
Addition H_2O :	13	s
Addition NaOH:	0	s
Reaction time:	0	s
Distillation time:	7	min.
Steam capacity:	100	%
Suction time:	20	s

Place an empty digestion tube and an Erlenmeyer flask into position, and start the program.

In case of extreme deposits in the glassware you can clean the system by putting about 10 ml of sulphuric acid into the digestion tube.

3.1 Error Code

The micro-processor continually surveys all the functions of the distillation system. As soon as an error arises it is shown on the display and accompanied by an acoustic signal.

Error message	Measures
No tap water	Check cooling water inlet for blockages. Ensure the tap is turned on
No sample tube	Insert tube
Check chemicals	Check set of tanks
Low water Press Enter	Check the water inlet distilled H_2O
Filling Steam generator	This message disappears as soon as steam generator is filled

After the above mentioned errors are corrected, the following message is displayed.

Error message	Measures
Stop Prog. No. x Continue=Enter	Enter = continue of interrupted program Reset = Standby-mode

Other error messages

Error message	Measures
Wait for steam	Message disappears as soon as stand-by is reached
Add sol. > 1min Continue=Enter	Check programming Enter=continue of interrupted program Reset=Standby-mode
Program undefined	Check programming
Excess steam pressure	Switch the system off and call service
Sensor error	Switch the system off and call service