

เอกสารแนบ 4

เอกสารผลการตรวจวัดคุณภาพสิ่งแวดล้อม



ANALYSIS REPORT

CUSTOMER NAME : วาเลน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : หลังการบำบัดน้ำเสีย
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส มีตะกอน มีกลิ่น
SAMPLING DATE : JANUARY 31, 2024
SAMPLING TIME : 12:00
SAMPLING BY : นายปริญญา กล้าน้อย

REPORT NO. : RN240110205
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JANUARY 31, 2024
ANALYTICAL DATE : JANUARY 31 - FEBRUARY 12, 2024
REPORT DATE : FEBRUARY 12, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH	-	Electrometric (SM: 4500-H ⁺ B.)	7.7 at 25°C	-	5-9
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	47.3	-	≤40
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	420.0	-	≤500
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105 °C (SM: 2540 D.)	30.0	-	≤50
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	≤0.5
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	<1.0	-	≤3.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	33.0	-	≤40
Grease & Oil	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	N.D.	1.4	≤20

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. Notification of the Ministry of Natural Resources and Environment, dated November 7, B.E. 2548 (2005), which was published in the Royal Government Gazette, Vol. 122, Part 125D dated December 19, B.E. 2548 (2005) . (Category C)

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาลเด็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : น้ำประปา
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใสไม่มีตะกอน
SAMPLING DATE : JANUARY 31, 2024
SAMPLING TIME : 10:20
SAMPLING BY : นายปริญญา กล้าน้อย
REPORT NO. : RN240110206
SAMPLING SOURCE : WATER SUPPLY
RECEIVED DATE : JANUARY 31, 2024
ANALYTICAL DATE : JANUARY 31 - FEBRUARY 12, 2024
REPORT DATE : FEBRUARY 12, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	232.0	-	<1000

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

Remark : 1. - Not available .

2. *ค่ามาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๔

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ANALYSIS REPORT

CUSTOMER NAME	: วาเล็น อโศก	REPORT NO.	: RN240110208
ADDRESS	: ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110	SAMPLING SOURCE	: SWIMMING POOL
SAMPLING LOCATION	: สระว่ายน้ำ (ส่วนต้น)	RECEIVED DATE	: JANUARY 31, 2024
SAMPLING METHOD	: GRAB	ANALYTICAL DATE	: JANUARY 31 - FEBRUARY 12, 2024
SAMPLING CONDITION	: NORMAL	REPORT DATE	: FEBRUARY 12, 2024
CHARACTERISTICS OF WATER	: ใส่ไม่มีตะกอน		
SAMPLING DATE	: JANUARY 31, 2024		
SAMPLING TIME	: 10:20		
SAMPLING BY	: นายปริญญา กล้าน้อย		

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

Remark : 1. - Not available .

- Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
- N.D. (Not Detectable) หมายถึง ตรวจไม่พบ



(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ห้องปฏิบัติการวิเคราะห์เอกชน บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

โทร: (66)02-868-1246 โทรสาร: (66)02-868-0860 Website: www.okla-testing.com J-NAC Group

ANALYSIS REPORT

CUSTOMER NAME : วาเลน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนเล็ก)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : JANUARY 31, 2024
SAMPLING TIME : 12:00
SAMPLING BY : นายปริญญา กล้าน้อย

REPORT NO. : RN240110207
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : JANUARY 31, 2024
ANALYTICAL DATE : JANUARY 31 - FEBRUARY 12, 2024
REPORT DATE : FEBRUARY 12, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

- Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
- N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาลเดิน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : ถังเก็บน้ำใต้ดิน
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : JANUARY 31, 2024
SAMPLING TIME : 10:20
SAMPLING BY : นายปริญญา กล้าน้อย
REPORT NO. : RN240110210
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JANUARY 31, 2024
ANALYTICAL DATE : JANUARY 31 - FEBRUARY 12, 2024
REPORT DATE : FEBRUARY 12, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Color	CU	Visual	2.1	-	≤ 15.0
Turbidity	NTU	Nephelometric Method, (SM: 2130 B.)	0.8	-	≤ 1.0
Odor	-	-	Non-Objectionable	-	Non-Objectionable
Escherichia Coli	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

- ค่ามาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๕
- Non-Objectionable หมายถึง ไม่เป็นที่น่ารังเกียจ
- Not Detected หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาดัน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : ถังเก็บน้ำดาดฟ้า
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : JANUARY 31, 2024
SAMPLING TIME : 10:20
SAMPLING BY : นายปริญญา กล้าน้อย

REPORT NO. : RN240110209
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JANUARY 31, 2024
ANALYTICAL DATE : JANUARY 31 - FEBRUARY 12, 2024
REPORT DATE : FEBRUARY 12, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Color	CU	Visual	2.4	-	≤ 15.0
Turbidity	NTU	Nephelometric Method, (SM: 2130 B.)	0.9	-	≤ 1.0
Odor	-	-	Non-Objectionable	-	Non-Objectionable
Escherichia Coli	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	Not Detected	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. * คำมาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๕
3. Non-Objectionable หมายถึง ไม่เป็นที่น่ารังเกียจ
4. Not Detected หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ANALYSIS REPORT

CUSTOMER NAME	: วาลเด็น อโศก	REPORT NO.	: RN240210475
ADDRESS	: ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110	SAMPLING SOURCE	: WASTEWATER
SAMPLING LOCATION	: หลังการบำบัดน้ำเสีย	RECEIVED DATE	: FEBRUARY 29, 2024
SAMPLING METHOD	: GRAB	ANALYTICAL DATE	: FEBRUARY 29-MARCH 12, 2024
SAMPLING CONDITION	: NORMAL	REPORT DATE	: MARCH 12, 2024
CHARACTERISTICS OF WATER	: เหลืองใส มีตะกอน มีกลิ่น		
SAMPLING DATE	: FEBRUARY 29, 2024		
SAMPLING TIME	: 12:00		
SAMPLING BY	: นายโกวิท บุหา		

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD**
pH	-	Electrometric (SM: 4500-H ⁺ B.)	7.3 at 25°C	-	5-9
Biochemical Oxygen Demand	mg/l	Azide Modification	26.4	-	≤40
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	430.0	-	≤500
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105 °C (SM: 2540 D.)	15.0	-	≤50
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	≤0.5
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	<3.0	-	≤3.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	14.0	-	≤40
Grease & Oil	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	N.D.	1.4	≤20

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

- Remark : 1. - Not available .
2. * mean analysis were performed by HVE Co.,Ltd .
3. ** Notification of the Ministry of Natural Resources and Environment, dated November 7, B.E. 2548 (2005), which was published in the Royal Government Gazette, Vol. 122, Part 125D dated December 19, B.E. 2548 (2005) . (Category C)
4. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาเลน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : น้ำประปา
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : FEBRUARY 29, 2024
SAMPLING TIME : 12:00
SAMPLING BY : นายโกวิท นุหา

REPORT NO. : RN240210476
SAMPLING SOURCE : WATER SUPPLY
RECEIVED DATE : FEBRUARY 29, 2024
ANALYTICAL DATE : FEBRUARY 29-MARCH 12, 2024
REPORT DATE : MARCH 12, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Dissolved Solids	mg/L	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	280.0	-	<1000

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

Remark : 1. - Not available .

2. * คำมาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๕

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full,
without written approval of Laboratory.***



ห้องปฏิบัติการวิเคราะห์เอกชน บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

โทร: (66)02-868-1246 โทรสาร: (66)02-868-0860 Website: www.okla-testing.com J-NAC Group

ANALYSIS REPORT

CUSTOMER NAME	: วาเลน อโศก	REPORT NO.	: RN240210478
ADDRESS	: ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110	SAMPLING SOURCE	: SWIMMING POOL
SAMPLING LOCATION	: สระว่ายน้ำ (ส่วนต้น)	RECEIVED DATE	: FEBRUARY 29, 2024
SAMPLING METHOD	: GRAB	ANALYTICAL DATE	: FEBRUARY 29-MARCH 12, 2024
SAMPLING CONDITION	: NORMAL	REPORT DATE	: MARCH 12, 2024
CHARACTERISTICS OF WATER	: ใส่ไม่มีตะกอน		
SAMPLING DATE	: FEBRUARY 29, 2024		
SAMPLING TIME	: 12:00		
SAMPLING BY	: นายโกวิท บุฬา		

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.

3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ห้องปฏิบัติการวิเคราะห์เอกชน บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

โทร: (66)02-868-1246 โทรสาร: (66)02-868-0860 Website: www.okla-testing.com J-NAC Group

ANALYSIS REPORT

CUSTOMER NAME	: วาดัน อโค	REPORT NO.	: RN240210477
ADDRESS	: ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110	SAMPLING SOURCE	: SWIMMING POOL
SAMPLING LOCATION	: สระว่ายน้ำ (ส่วนลึก)	RECEIVED DATE	: FEBRUARY 29, 2024
SAMPLING METHOD	: GRAB	ANALYTICAL DATE	: FEBRUARY 29-MARCH 12, 2024
SAMPLING CONDITION	: NORMAL	REPORT DATE	: MARCH 12, 2024
CHARACTERISTICS OF WATER	: ใสไม่มีตะกอน		
SAMPLING DATE	: FEBRUARY 29, 2024		
SAMPLING TIME	: 12:00		
SAMPLING BY	: นายโกวิท บุหา		

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

Remark : 1. - Not available .

- Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
- N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาเลน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : หลังการบำบัดน้ำเสีย
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส มีตะกอน มีกลิ่น
SAMPLING DATE : MARCH 08, 2024
SAMPLING TIME : 13:15
SAMPLING BY : นายปริญญา กล้าน้อย
REPORT NO. : RN240310541
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MARCH 08, 2024
ANALYTICAL DATE : MARCH 08-18, 2024
REPORT DATE : MARCH 19, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD**
pH	-	Electrometric (SM: 4500-H ⁺ B.)	7.1 at 25°C	-	5-9
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	25.9	-	≤40
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	416.0	-	≤500
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105 °C (SM: 2540 D.)	22.0	-	≤50
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	≤0.5
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	<3.0	-	≤3.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	17.0	-	≤40
Grease & Oil	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	N.D.	1.4	≤20

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

- Remark : 1. - Not available .
2. * mean analysis were performed by HVE Co.,Ltd .
3. ** Notification of the Ministry of Natural Resources and Environment, dated November 7, B.E. 2548 (2005), which was published in the Royal Government Gazette, Vol. 122, Part 125D dated December 19, B.E. 2548 (2005) . (Category C)
4. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ห้องปฏิบัติการวิเคราะห์เอกชน บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด
63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

โทร: (66)02-868-1246 โทรสาร: (66)02-868-0860 Website: www.okla-testing.com J-NAC Group

ANALYSIS REPORT

CUSTOMER NAME : วาลเด็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : น้ำประปา
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ไม่มีส่วนตะกอน
SAMPLING DATE : MARCH 08, 2024
SAMPLING TIME : 13:15
SAMPLING BY : นายปริญญา กล้าน้อย

REPORT NO. : RN240310542
SAMPLING SOURCE : WATER SUPPLY
RECEIVED DATE : MARCH 08, 2024
ANALYTICAL DATE : MARCH 08-18, 2024
REPORT DATE : MARCH 19, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	196.0	-	<1000

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

Remark : 1. - Not available .

2. * คำมาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๔

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ANALYSIS REPORT

CUSTOMER NAME	: วาลเด็น อโศก	REPORT NO.	: RN240310544
ADDRESS	: ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110	SAMPLING SOURCE	: SWIMMING POOL
SAMPLING LOCATION	: สระว่ายน้ำ (ส่วนต้น)	RECEIVED DATE	: MARCH 08, 2024
SAMPLING METHOD	: GRAB	ANALYTICAL DATE	: MARCH 08-18, 2024
SAMPLING CONDITION	: NORMAL	REPORT DATE	: MARCH 19, 2024
CHARACTERISTICS OF WATER	: ไม่พบตะกอน		
SAMPLING DATE	: MARCH 08, 2024		
SAMPLING TIME	: 13:15		
SAMPLING BY	: นายปริญญา กล้าน้อย		

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

- Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
- N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ANALYSIS REPORT

CUSTOMER NAME : วาเลน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนเล็ก)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : MARCH 08, 2024
SAMPLING TIME : 13:15
SAMPLING BY : นายปริญญา กล้าน้อย

REPORT NO. : RN240310543
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : MARCH 08, 2024
ANALYTICAL DATE : MARCH 08-18, 2024
REPORT DATE : MARCH 19, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

- Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
- N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ANALYSIS REPORT

CUSTOMER NAME : วาลเด็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : หลังการบำบัดน้ำเสีย
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส มีตะกอน มีกลิ่น
SAMPLING DATE : APRIL 05, 2024
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุญหา

REPORT NO. : RN240410825
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : APRIL 05, 2024
ANALYTICAL DATE : APRIL 05-17, 2024
REPORT DATE : APRIL 17, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
pH	-	Electrometric (SM: 4500-H ⁺ B.)	6.9 at 25°C	-	5-9
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	33.0	-	≤40
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	424.0	-	≤500
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105 °C (SM: 2540 D.)	11.0	-	≤50
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	<0.1	-	≤0.5
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	<3.0	-	≤3.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	25.0	-	≤40
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	N.D.	1.4	≤20

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. Notification of the Ministry of Natural Resources and Environment, dated November 7, B.E. 2548 (2005), which was published in the Royal Government Gazette, Vol. 122, Part 125D dated December 19, B.E. 2548 (2005) . (Category C)

3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาดัน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : น้ำประปา
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : APRIL 05, 2024
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุนหา

REPORT NO. : RN240410826
SAMPLING SOURCE : WATER SUPPLY
RECEIVED DATE : APRIL 05, 2024
ANALYTICAL DATE : APRIL 05-17, 2024
REPORT DATE : APRIL 17, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	198.0	-	<1000
SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23 rd ED.,2017 (AWWA,APHA, WEF)					

Remark : 1. - Not available .

2. * คำมาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๕

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ANALYSIS REPORT

CUSTOMER NAME : วาเล็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนต้น)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ไม่พบตะกอน
SAMPLING DATE : APRIL 05, 2024
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุญหา

REPORT NO. : RN240410828
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : APRIL 05, 2024
ANALYTICAL DATE : APRIL 05-17, 2024
REPORT DATE : APRIL 17, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ANALYSIS REPORT

CUSTOMER NAME : วาลเด็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนลึก)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ไม่พบตะกอน
SAMPLING DATE : MARCH 08, 2024
SAMPLING TIME : 13:15
SAMPLING BY : นายปริญญา กล้าน้อย

REPORT NO. : RN240410827
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : MARCH 08, 2024
ANALYTICAL DATE : MARCH 08-18, 2024
REPORT DATE : MARCH 19, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***



ANALYSIS REPORT

CUSTOMER NAME : วาลเด็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : ถังเก็บน้ำใต้ดิน
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ไม่ไม่มีตะกอน
SAMPLING DATE : APRIL 05, 2024
SAMPLING TIME : 11:00
SAMPLING BY : นายไกรวิทย์ บุฬา

REPORT NO. : RN240410830
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : APRIL 05, 2024
ANALYTICAL DATE : APRIL 05-17, 2024
REPORT DATE : APRIL 17, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Color	CU	Visual	2.6	-	≤ 15.0
Turbidity	NTU	Nephelometric Method, (SM: 2130 B.)	0.3	-	≤ 1.0
Odor	-	-	Non-Objectionable	-	Non-Objectionable
Escherichia Coli	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	N.D.	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

Remark : 1. - Not available .

2. *ค่ามาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๕

3. Non-Objectionable หมายถึง ไม่เป็นที่น่ารังเกียจ

4. Not Detected หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาเลน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : ถังเก็บน้ำคัดฟ้า
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : APRIL 05, 2024
SAMPLING TIME : 11:00
SAMPLING BY : นายโกวิท บุฬา
REPORT NO. : RN240410829
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : APRIL 05, 2024
ANALYTICAL DATE : APRIL 05-17, 2024
REPORT DATE : APRIL 17, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Color	CU	Visual	2.1	-	≤ 15.0
Turbidity	NTU	Nephelometric Method, (SM: 2130 B.)	0.2	-	≤ 1.0
Odor	-	-	Non-Objectionable	-	Non-Objectionable
Escherichia Coli	per 100 ml	E.coli Procedure Using Fluorogenic Substrate (SM: 9221 F.)	N.D.	-	Not Detected

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

Remark : 1. - Not available .

- ค่ามาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๕
- Non-Objectionable หมายถึง ไม่เป็นที่น่ารังเกียจ
- Not Detected หมายถึง ตรวจไม่พบ

น.จิณารัตน์
(Nijinart Matiyapak)
Scientist

ท.ทวัชชัย
(Tawatchai Chongvutichai)
Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาดเต็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : หลังการบำบัดน้ำเสีย
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองขุ่น มีตะกอน มีกลิ่น
SAMPLING DATE : MAY 16, 2024
SAMPLING TIME : 12:10
SAMPLING BY : นายไกรวิทย์ บุษหา
REPORT NO. : RN240511193
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : MAY 16, 2024
ANALYTICAL DATE : MAY 16-27, 2024
REPORT DATE : MAY 27, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
pH	-	Electrometric (SM: 4500-H ⁺ B.)	7.3 at 25°C	-	5-9
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O G, 5210 B.)	64.0	-	≤40
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	514.0	-	≤500
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105 °C (SM: 2540 D.)	32.0	-	≤50
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	0.3	-	≤0.5
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	<3.0	-	≤3.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	40.0	-	≤40
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	N.D.	1.4	≤20

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

Remark : 1. - Not available .

2. Notification of the Ministry of Natural Resources and Environment, dated November 7, B.E. 2548 (2005), which was published in the Royal Government Gazette, Vol. 122, Part 125D dated December 19, B.E. 2548 (2005) . (Category C)

3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาดัน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : น้ำประปา
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : MAY 16, 2024
SAMPLING TIME : 12:10
SAMPLING BY : นายโกวิท นูหา

REPORT NO. : RN240511194
SAMPLING SOURCE : WATER SUPPLY
RECEIVED DATE : MAY 16, 2024
ANALYTICAL DATE : MAY 16-27, 2024
REPORT DATE : MAY 27, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	192.0	-	<1000

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. * ค่ามาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๕

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***



ANALYSIS REPORT

CUSTOMER NAME : วาดัน โอโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนต้น)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : MAY 16, 2024
SAMPLING TIME : 12:10
SAMPLING BY : นายโกวิท บุษหา

REPORT NO. : RN240511196
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : MAY 16, 2024
ANALYTICAL DATE : MAY 16-27, 2024
REPORT DATE : MAY 27, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. * Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ANALYSIS REPORT

CUSTOMER NAME : วาเล็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนลึก)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : MAY 16, 2024
SAMPLING TIME : 12:10
SAMPLING BY : นายโกวิท บุนหา
REPORT NO. : RN240511195
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : MAY 16, 2024
ANALYTICAL DATE : MAY 16-27, 2024
REPORT DATE : MAY 27, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.

3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาลเด็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : หลังการบำบัดน้ำเสีย
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : เหลืองใส มีตะกอน ไม่มีกลิ่น
SAMPLING DATE : JUNE 14, 2024
SAMPLING TIME : 15:10
SAMPLING BY : นายพีรพล ถวิลหวัง
REPORT NO. : RN240611479
SAMPLING SOURCE : WASTEWATER
RECEIVED DATE : JUNE 14, 2024
ANALYTICAL DATE : JUNE 14-24, 2024
REPORT DATE : JUNE 25, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
pH	-	Electrometric (SM: 4500-H ⁺ B.)	7.4 at 25°C	-	5-9
Biochemical Oxygen Demand	mg/l	Membrane Electrode (SM: 4500-O ₂ G, 5210 B.)	29.8	-	≤40
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	512.0	-	≤500
Total Suspended Solids	mg/l	Total Suspended Solids Dried at 103-105 °C (SM: 2540 D.)	32.0	-	≤50
Settleable Solids	ml/l	Settleable Solids (SM: 2540 F.)	0.3	-	≤0.5
Sulfide as H ₂ S	mg/l	Iodometric (SM: 4500-S ²⁻ F.)	<3.0	-	≤3.0
Total Kjeldahl Nitrogen	mg/l	Macro Kjeldahl (SM: 4500-N _{org} B)	15.0	-	≤40
Oil & Grease	mg/l	Liquid-Liquid Partition-Gravimetric (SM: 5520 B.)	N.D.	1.4	≤20

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

- Remark : 1. - Not available .
2. Notification of the Ministry of Natural Resources and Environment, dated November 7, B.E. 2548 (2005), which was published in the Royal Government Gazette, Vol. 122, Part 125D dated December 19, B.E. 2548 (2005) . (Category C)
3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)
Scientist

(Tawatchai Chongvutichai)
Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ห้องปฏิบัติการวิเคราะห์เอกชน บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติง เซอร์วิส จำกัด

63/13 เพชรเกษม ซอย 7 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600

โทร: (66)02-868-1246 โทรสาร: (66)02-868-0860 Website: www.okla-testing.com J-NAC Group

ANALYSIS REPORT

CUSTOMER NAME	: วาลเด็น อโศก	REPORT NO.	: RN240611480
ADDRESS	: ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110	SAMPLING SOURCE	: WATER SUPPLY
SAMPLING LOCATION	: น้ำประปา	RECEIVED DATE	: JUNE 14, 2024
SAMPLING METHOD	: GRAB	ANALYTICAL DATE	: JUNE 14-24, 2024
SAMPLING CONDITION	: NORMAL	REPORT DATE	: JUNE 25, 2024
CHARACTERISTICS OF WATER	: ไม่มีการตกตะกอน		
SAMPLING DATE	: JUNE 14, 2024		
SAMPLING TIME	: 15:10		
SAMPLING BY	: นายพีรพล ธีรวิหัง		

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD*
Total Dissolved Solids	mg/l	Total Dissolved Solids Dried at 180 °C (SM: 2540 C.)	260.0	-	<1000

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. * ค่ามาตรฐานเกณฑ์กำหนดคุณภาพน้ำประปาของการประปานครหลวง ประกาศ ณ วันที่ ๑๑ ตุลาคม พ.ศ. ๒๕๖๕

(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***

ANALYSIS REPORT

CUSTOMER NAME : วาเลน อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนต้น)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER :ใสไม่มีตะกอน
SAMPLING DATE : JUNE 14, 2024
SAMPLING TIME : 15:10
SAMPLING BY : นายพีรพล ถวิลหวัง
REPORT NO. : RN240611482
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : JUNE 14, 2024
ANALYTICAL DATE : JUNE 14-24, 2024
REPORT DATE : JUNE 25, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED.,2017 (AWWA,APHA, WEF)

Remark : 1. - Not available .

2. Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ

(Nijinart Matiyapak)
Scientist

(Tawatchai Chongvutichai)
Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory.***



ANALYSIS REPORT

CUSTOMER NAME : วาลเด็น อโศก
ADDRESS : ถนนสุขุมวิท แขวงคลองเตยเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
SAMPLING LOCATION : สระว่ายน้ำ (ส่วนลึก)
SAMPLING METHOD : GRAB
SAMPLING CONDITION : NORMAL
CHARACTERISTICS OF WATER : ใส่ไม่มีตะกอน
SAMPLING DATE : JUNE 14, 2024
SAMPLING TIME : 15:10
SAMPLING BY : นายพีรพล ถวิลหวัง

REPORT NO. : RN240611481
SAMPLING SOURCE : SWIMMING POOL
RECEIVED DATE : JUNE 14, 2024
ANALYTICAL DATE : JUNE 14-24, 2024
REPORT DATE : JUNE 25, 2024

PARAMETER	UNIT	METHODS OF ANALYSIS	RESULT	MDL	STANDARD
Total Coliform Bacteria	MPN/100 ml	MPN Test	<1.8	-	<10
Fecal Coliform Bacteria	MPN/100 ml	MPN Test	N.D.	-	N.D.

SM : STANDARD METHODS FOR EXAMINATION OF WATER AND WASTEWATER 23rd ED., 2017 (AWWA, APHA, WEF)

Remark : 1. - Not available .

2. Recommendations of the Public Health Committee No. 1/2007 regarding the control of swimming pool operations or other businesses Likewise.
3. N.D. (Not Detectable) หมายถึง ตรวจไม่พบ



(Nijinart Matiyapak)

Scientist

(Tawatchai Chongvutichai)

Environmental Laboratory Section Manager

*** Reported analysis refers to submitted sample only. Report analysis shall not be reproduced except in full, without written approval of Laboratory. ***

เอกสารแนบ 5

หนังสือรับรองห้องปฏิบัติการวิเคราะห์เอกชน



๐๔ พฤศจิกายน ๒๕๖๔

เรื่อง ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๒ กรกฎาคม ๒๕๖๔

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด จำนวน ๑ แผ่น

ตามหนังสือที่อ้างถึง บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด ขอต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน เลขทะเบียน ว-๒๑๙ สถานที่ตั้งเลขที่ ๖๓/๑๓ ซอยเพชรเกษม ๗
แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพมหานคร ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท โอกลา เทสต์ติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด
ต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- | | |
|-----------------------------|----------------------------|
| ๑) นายธวัชชัย จงวุฒิชัย | ทะเบียนเลขที่ ว-๒๑๙-ค-๕๑๒๔ |
| ๒) นางสาวปนัดดา พันธุ์กะจับ | ทะเบียนเลขที่ ว-๒๑๙-ค-๖๖๙๙ |
| ๓) นางสาวจามจุรี คำปุย | ทะเบียนเลขที่ ว-๒๑๙-ค-๙๖๖๓ |

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์

- | | |
|--|----------------------------|
| ๑) นางสาวธัญชนก ชำขุน | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๔๑๖ |
| ๒) ว่าที่ร้อยตรีหญิงสาวตรี เวียงจันทร์ | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๔๑๗ |
| ๓) นางสาวภาณุชนารถ เชี่ยวชาญ | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๔๑๘ |
| ๔) นางสาววันวิสา หวังแวกลาง | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๔๑๙ |
| ๕) นางสาวธิดารัตน์ กลัดตลาด | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๔๒๐ |
| ๖) นางสาวรัตตชา ศรีปราสาท | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๔๒๑ |
| ๗) นางสาวแพรวพรรณ กองกะแซง | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๔๒๒ |
| ๘) นางสาวจุลฑา สมบุญ | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๔๒๓ |
| ๙) นางสาวนิจินา มะติยาภักดิ์ | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๔๒๔ |
| ๑๐) นางสาวเบญจพร อินแก้ว | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๖๖๔ |
| ๑๑) นายธนทัต เวชกิจ | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๖๖๕ |
| ๑๒) นายปริญญา กล้าน้อย | ทะเบียนเลขที่ ว-๒๑๙-จ-๙๖๖๖ |

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสีย จำนวน ๙ รายการ และ
อากาศเสีย จำนวน ๕ รายการ รวมทั้งสิ้น ๑๔ รายการ ตามสิ่งที่ส่งมาด้วย

หนังสือฉบับนี้จะหมดอายุในวันที่ ๑๕ สิงหาคม ๒๕๖๗ หากประสงค์จะต่ออายุหนังสือ
รับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อ
กรมโรงงานอุตสาหกรรมภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
ซึ่งคำขอต่ออายุดังกล่าวขอรับได้ที่กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นางจินดา เตชะศรีนทร์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๔-๖

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๙๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.gmail.go.th

เอกสารแนบท้ายหนังสือรับต่ออายุขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท โอกลา เทสติ้ง แอนด์ คอนซัลติ้ง เซอร์วิส จำกัด เลขทะเบียน ว-๒๑๙
ที่ อก ๐๓๑๐(๑)/ ๑ ๐ ๔๓ ๑ ลงวันที่ ๐ ๔ พฤศจิกายน ๒๕๖๕

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๑๔ รายการ

น้ำเสีย จำนวน 9 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Biochemical Oxygen Demand	1) 5-Day BOD Test, Azide Modification Method ^[3] 2) 5-Day BOD Test, Membrane Electrode Method ^[3]
2	Free Chlorine	Iodometric Method ^[3]
3	Oil & Grease	Liquid-Liquid, Partition-Gravimetric Method ^[3]
4	pH	Electrometric Method ^[3]
5	Sulfide	Iodometric Method ^[3]
6	Temperature	Laboratory and Field Methods ^[3]
7	Total Dissolved Solids	Dried at 180 °C ^[3]
8	Total Kjeldahl Nitrogen	Macro-Kjeldahl Method ^[3]
9	Total Suspended Solids	Dried at 103-105 °C ^[3]

อากาศเสีย (ปล่องระบาย) จำนวน 5 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Carbon Monoxide	Instrumental Analyzer ^[4]
2	Opacity	Ringelmann's Method ^[1,2]
3	Oxides of Nitrogen	Instrumental Analyzer ^[4]
4	Sulfur Dioxide	Instrumental Analyzer ^[4]
5	Total Suspended Particulate	Isokinetic Sampling, Gravimetric Method ^[4]

เอกสารอ้างอิง

1. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณ
เขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงสีข้าวที่ใช้กลบเป็นเชื้อเพลิง.

ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125 ง.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม, พ.ศ. 2549. เรื่อง กำหนดค่าปริมาณ
เขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำโรงงาน. ราชกิจจานุเบกษา. 4 ธันวาคม 2549.
เล่มที่ 123 ตอนพิเศษ 125 ง.

3. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC: APHA, 2017.

4. United States Environmental Protection Agency. **Standards of Performance for New Stationary Sources**. 40 CFR 60. Appendix A, 2018.

(นางริกาญจน์ ฉัตรสกุลวิไล)

ผู้อำนวยการกลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษ
และทะเบียนห้องปฏิบัติการ



ที่ อก ๐๓๑๐(๑)/ ๑ ๒ ๓ ๗ ๒

กรมโรงงานอุตสาหกรรม
ถนนพระรามที่ ๖ แขวงทุ่งพญาไท
เขตราชเทวี กรุงเทพฯ ๑๐๕๐๐

๒ ๘ สิงหาคม ๒๕๖๖

เรื่อง ขันทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

เรียน กรรมการผู้จัดการ บริษัท เอชวีอี จำกัด

อ้างถึง คำขอขึ้นทะเบียน/ต่ออายุ/เปลี่ยนแปลงบุคลากร และชนิดสารมลพิษของห้องปฏิบัติการวิเคราะห์เอกชน
ลงวันที่ ๑๘ พฤษภาคม ๒๕๖๖

สิ่งที่ส่งมาด้วย เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน
บริษัท เอชวีอี จำกัด จำนวน ๒ แผ่น

ตามหนังสือที่อ้างถึง บริษัท เอชวีอี จำกัด ขอขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน พร้อม
รายชื่อผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์ เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์และรายการสารมลพิษ
ที่จะทำการวิเคราะห์ ต่อกรมโรงงานอุตสาหกรรม นั้น

กรมโรงงานอุตสาหกรรมพิจารณาแล้ว ให้บริษัท เอชวีอี จำกัด ขันทะเบียนห้องปฏิบัติการ
วิเคราะห์เอกชน มีเลขทะเบียน ว-๓๕๘ สถานที่ตั้งเลขที่ ๖๐๓ ซอยเจริญสนิทวงศ์ ๔๖ แขวงบางยี่ขัน
เขตบางพลัด กรุงเทพมหานคร โดยมีองค์ประกอบดังนี้

ก. ผู้ควบคุมดูแลห้องปฏิบัติการวิเคราะห์

- | | |
|-----------------------------|----------------------------|
| ๑) นายเอกลักษณ์ สีสลาบริหาร | ทะเบียนเลขที่ ว-๓๕๘-ค-๐๐๐๑ |
| ๒) นางสาวทิพวรรณ วงศ์บุญตัน | ทะเบียนเลขที่ ว-๓๕๘-ค-๐๐๐๒ |
| ๓) นายพล ม่วงใหญ่ | ทะเบียนเลขที่ ว-๓๕๘-ค-๐๐๐๓ |

ข. เจ้าหน้าที่ประจำห้องปฏิบัติการวิเคราะห์

- | | |
|-----------------------------|----------------------------|
| ๑) นางสาวสุปรียา หล้าอิน | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๑ |
| ๒) นางสาวจิราภรณ์ ผงผานอก | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๒ |
| ๓) นายธรรมรัตน์ จริยวัฒนสุข | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๓ |
| ๔) นางสาวธนภรณ์ กำทา | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๔ |
| ๕) นางสาวณัฐรดา คงบัน | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๕ |
| ๖) นายฐานันท์ นิภารัตน์ | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๖ |
| ๗) นายมนโรด สุดจันทร์ | ทะเบียนเลขที่ ว-๓๕๘-จ-๐๐๐๗ |

ค. ขอบข่ายสารมลพิษที่ได้รับขึ้นทะเบียนให้วิเคราะห์ในน้ำเสียและอากาศเสีย ตามสิ่งที่

ส่งมาด้วย

หนังสือฉบับ...

หนังสือฉบับนี้มีอายุครั้งละ ๓ ปี นับจากวันที่กรมโรงงานอุตสาหกรรมออกหนังสือหากประสงค์จะต่ออายุหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน ให้ยื่นคำขอต่ออายุพร้อมเอกสารประกอบคำขอต่อกรมโรงงานอุตสาหกรรม ภายใน ๓๐ วัน ก่อนวันสิ้นอายุของหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชนทั้งนี้สามารถยื่นคำขอผ่านระบบอิเล็กทรอนิกส์ได้ที่หน้าเว็บไซต์กรมโรงงานอุตสาหกรรม

จึงเรียนมาเพื่อทราบ

ขอแสดงความนับถือ



(นายประสม คำรพงษ์)

ผู้อำนวยการกองวิจัยและเตือนภัยมลพิษโรงงาน
ปฏิบัติราชการแทนอธิบดีกรมโรงงานอุตสาหกรรม

กองวิจัยและเตือนภัยมลพิษโรงงาน

กลุ่มมาตรฐานวิธีการวิเคราะห์ทดสอบมลพิษและทะเบียนห้องปฏิบัติการ

โทร. ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๐๓-๕

โทรสาร ๐ ๒๔๓๐ ๖๓๑๒ ต่อ ๒๑๔๙

ไปรษณีย์อิเล็กทรอนิกส์ saraban@diw.mail.go.th



เอกสารแนบท้ายหนังสือรับขึ้นทะเบียนห้องปฏิบัติการวิเคราะห์เอกชน

บริษัท เอชวีอี จำกัด

เลขทะเบียน ว-๓๕๘

ที่ ออก ๐๓๑๐(๑)/ ๑ ๒ ๓ ๗ ๒

ลงวันที่ ๒๘ สิงหาคม ๒๕๖๖

ขอขยายสารมลพิษที่ได้รับขึ้นทะเบียนจากกรมโรงงานอุตสาหกรรม จำนวน ๓๑ รายการ

น้ำเสีย จำนวน 30 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Aldicarb	High-Performance Liquid Chromatographic Method ^[1]
2	Aldicarb sulfone	High-Performance Liquid Chromatographic Method ^[1]
3	Aldicarb sulfoxide	High-Performance Liquid Chromatographic Method ^[1]
4	Aldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
5	α-BHC	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
6	Biochemical Oxygen Demand	5-Day BOD Test, Azide Modification Method ^[1]
7	Carbaryl	High-Performance Liquid Chromatographic Method ^[1]
8	Carbofuran	High-Performance Liquid Chromatographic Method ^[1]
9	Chemical Oxygen Demand	Closed Reflux, Titrimetric Method ^[1]
10	4,4'-DDD	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
11	4,4'-DDE	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
12	Dieldrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
13	Endosulfan I	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
14	Endosulfan II	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
15	Endrin	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
16	Heptachlor	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
17	Heptachlo Epoxide	Liquid-Liquid Extraction, Gas Chromatographic Method ^[1]
18	3-Hydroxycarbofuran	High-Performance Liquid Chromatographic Method ^[1]
19	Methiocarb	High-Performance Liquid Chromatographic Method ^[1]
20	Methomyl	High-Performance Liquid Chromatographic Method ^[1]
21	1-Naphthol	High-Performance Liquid Chromatographic Method ^[1]
22	Oil & Grease	Liquid-Liquid, Partition-Gravimetric Method ^[1]
23	Oxamyl	High-Performance Liquid Chromatographic Method ^[1]
24	pH	Electrometric Method ^[1]
25	Propoxur	High-Performance Liquid Chromatographic Method ^[1]
26	Sulfide	Iodometric Method ^[1]
27	Temperature	Laboratory and Field Methods ^[1]
28	Total Dissolved Solids	Dried at 180 °C ^[1]
29	Total Kjeldahl Nitrogen	Macro Kjeldahl Method ^[1]
30	Total Suspended Solids	Dried at 103-105 °C ^[1]

อากาศเสีย (ปล่อยระบาย) จำนวน 1 รายการ

ลำดับที่	สารมลพิษ	วิธีวิเคราะห์
1	Opacity	Ringelmann's Method ^[2]

เอกสารอ้างอิง

1. APHA, AWWA, WEF. **Standard Methods for the Examination of Water and Wastewater**. 23rd ed. Washington, DC: APHA, 2017.

2. กระทรวงอุตสาหกรรม. ประกาศกระทรวงอุตสาหกรรม เรื่อง กำหนดค่าปริมาณเขม่าควันที่เจือปนในอากาศที่ระบายออกจากปล่องของหม้อน้ำของโรงงาน พ.ศ. 2549. ราชกิจจานุเบกษา. 4 ธันวาคม 2549. เล่มที่ 123 ตอนพิเศษ 125ง.



Ref No. : 0303/16367

CERTIFICATE OF TESTING LABORATORY ACCREDITATION

This is to certify that

HVE Co., Ltd.

**603 Soi Jarunsanitwong 46, Jarunsanitwong Road,
Bangyee Khan, Bang Phlat, Bangkok 10700**

has successfully undergone assessment according to ISO/IEC 17025 : 2017
and under the Bureau of Laboratory Accreditation, Department of Science Service
for the requirements, regulations and criteria for the competence of testing laboratories

Accreditation Number TESTING - 0090

The scope of accreditation is as annexed hereto

Issue date : **22nd November 2021**

Expired date : **21st November 2025**

Signature : 

(Mrs. Pochaman Tagheen)

Director of Bureau of Laboratory Accreditation

Bureau of Laboratory Accreditation, Department of Science Service,
Ministry of Higher Education, Science, Research and Innovation

เอกสารแนบ 6

เอกสารสอบเทียบเครื่องมือที่ใช้ในการวิเคราะห์



Certificate of Calibration

Certificate No.: WK2402-300-865

Page 1 of 2

Customer : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Watthapra, Bangkok Yai, Bangkok 10600 Thailand.

Instrument	: Dissolved Oxygen	Ambient Temperature	: (25.0 ± 2) °C
Manufacturer	: HANNA	Humidity	: (50.0 ± 15) %RH
Model	: HI5421	Received Date	: 27-Feb-24
Serial No.	: 04240005101	Calibrated Date	: 27-Feb-24
Identity No.	: KC1A11T8H	Issued Date	: 27-Feb-24
Range	: See to data	Calibrated Location	: In Lab
Resolution	: See to data		
Calibration Method	: CP-WK-C03		

Reference standard instruments :

<u>Instrument</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>	<u>Traceability to</u>
Zero Oxygen Solution	HI7040L	S0115/20	30-Aug-25	NIST
DO Meter	874477	WK2305-300-241	25-May-24	WK Electric Co.,Ltd.
Digital Thermometer	WK-CT-025	WK2402-300-25	25-Feb-25	WK Electric Co.,Ltd.

NIST : National Institute of Standard and Technology.

This result calibrate was found accurate as shown on date place of calibrate only

This certificate is traceability to th International System of Unit (SI)

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95 %

Calibrated by : Mr. Usa Phuangphiphat

Approved by :

Mr. Ratchadawut Rungravee

Authorized Signatory

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.



Calibration Results

Certificate No. : WK2402-300-865

Page 2 of 2

Calibration Result of the Accuracy

Function : Dissolved Oxygen Measurement at 25 °C

Resolution : 0.01 mg/L

Unit : mg/L

STD Solution	UUC Reading		Error	Uncertainty (± mg/L)
	Before Adjustment	After Adjustment		
0.00	0.32	0.00	0.00	0.15
8.40	9.15	8.37	-0.03	0.33
8.70	9.01	8.65	-0.05	0.33
9.00	9.24	8.92	-0.08	0.33

() Without Adjustment (X) After Adjustment

This certificate may not be reproduced except in full unless permission for the reproduction has been obtained in writing from the laboratory.

**** End of Certificate****

Certificate No. : HIT-2410-0320

Page : 1 of 2

CERTIFICATE OF CALIBRATION

Equipment :	pH/mV and EC/TDS/Salinity/Resistivity Meter		
Meter Model :	HI5521-02	Serial No. :	04160019101
Probe Model :	HI1131B	Serial No. :	094430BN
Resolution (pH) :	0.01	Resolution (mV) :	0.1
Manufacturer :	Hanna Instruments	Made in :	Romania
Condition As-Received :	Used Product	Reference :	RE240370
Ambient Temperature :	(25 ± 2) °C	Relative Humidity :	(50 ± 15) % RH
Customer name :	Okla Testing & Consulting Service Co., Ltd. 67/35-36, 3RD Floor, Phetkasem 7/1 Road, Wat Tha Pra, Bangkok Yai, Bangkok 10600 Thailand		
Received date :	28 February 2024		
Calibrate date :	4 March 2024		
Issue date :	5 March 2024		
Calibrated Location :	Hanna Instruments (Thailand) Ltd.		
Calibration Procedure :	This calibrator was conducted by using in-house: calibration procedure CP-01, CP-02 by using certified reference material (CRM)		

Calibrated by :

☒ Mr. Pichit Petthong
☐ Mr. Channarong Soinak

Approved by :


Mr. Anan Suwanchaisakul

Authorized Signatory



This certificate was certified only for the instrument we calibrated.

This result of calibration was found accurate on date and place of calibration only.

** This certificate may not be reproduced other than in full, except with the prior written **

approval of the head of Hanna Instrument (Thailand)

Condition of this calibration result

1. Reference Standard Instruments : This certification is traceable to the international unit of unit maintained through:

Instruments	Model	Serial No.	Certificate No.	Traceable
Documenting Process Calibrator	Fluke 753	43160061	LF24-0014	Measuretronix Limited.
Thermometer with sensor	HI98509	39643D	23T1453	Technology Promotion Association (Thailand-Japan).
Digital Thermo-Hygrometer	HT-771SD	AI.07155	24H41	

2. Reference Standard Materials : pH calibration standard traceable thru CPA chem Ltd.

Buffer Solution	Manufacture	Certified Value	Lot Number	Exp. date
pH 4.0	CPA chem	$4.008 \pm 0.006 @ 25^{\circ}\text{C}$	898494	3 June 2024
pH 7.0	CPA chem	$6.985 \pm 0.007 @ 25^{\circ}\text{C}$	898500	28 May 2024
pH 10.0	CPA chem	$10.011 \pm 0.012 @ 25^{\circ}\text{C}$	898502	24 May 2024

Calibration Result :

1. Performing standard curve by Simulator at: -177.5, 0.0, 177.5 mV

(Measurement Electrical Potential) After Adjust Result.

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (\pm mV)
	pH	mV	pH	mV	
pH Meter S/N 04160019101	4.01	177.5	4.01	177.5	0.097
	7.01	0.0	7.01	0.0	0.058
	10.01	-177.5	10.01	-177.5	0.097

2. Performing three buffer standard curve by using buffer nominal : pH 4,7,10 After Adjustment.

Unit Under Calibration	Standard pH Buffer Solution	Actual Reading (pH)	Actual Reading (mV)	Uncertainty of Measurement (\pm pH)
pH Electrode S/N 094430BN	4.008	4.02	159.3	0.010
	6.985	6.99	-13.6	0.011
	10.011	10.04	-187.9	0.014

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

** End of certificate **

CERTIFICATE OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOMETER
MANUFACTURER : HANNA INSTRUMENTS
MODEL / TYPE : HI5521/HI7662-W
SERIAL NO. : 04160019101/0615024N
CLID. NO. : 232202088
JOB CONTROL NO. : 231017115955

CUSTOMER : OKLA TESTING & CONSULTING SERVICE CO., LTD.
67/35-36, 3RD FLOOR, PHETKASEM 7/1 RD., WATTHAPRA,
BANGKOKYAI, BANGKOK 10600 THAILAND

DATE OF RECEIVED : 17 October 2023

DATE OF ISSUED : 20 October 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Pimsiri Hemtanon
Calibration Engineer

Approved By : Mongkol Yotsoontorn
Authorized Signatory
20 October 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI)

Certificate No. Q23115955

F3-011-04/01-12

page 1 of 3



@clccalibration

REPORT OF CALIBRATION

FOR

NOMENCLATURE : DIGITAL THERMOMETER
MANUFACTURER : HANNA INSTRUMENTS
MODEL / TYPE : HI5521/HI7662-W
SERIAL NO. : 04160019101/0615024N
DATE OF CALIBRATION : 19 October 2023

ENVIRONMENT CONDITIONS :

Temperature : $(23 \pm 2) ^\circ\text{C}$ Relative Humidity : $(55 \pm 10) \% \text{ RH}$

PROCEDURE USED :

This instrument was calibrated under procedure No. **WI-305-187** based on **ASTM E 644-11:2019** as calibration guidelines.
The calibration was performed by using Calibration Bath, Precision Thermometer and IPRT which maintained by the Calibration Laboratory Co., Ltd.

REFERENCE STANDARD USED :

1. Calibration Bath, Kambic Model OB-22/2 ULT S/N. 17115653.
2. Precision Thermometer, ASL Model F200-A-8 S/N. 014433/03.
3. IPRT, ASL Model T100-250-1D S/N. PO106346-1-13.

TRACEABILITY :

1. The measurements are traceable to International System of Units (SI), through Calibration Laboratory Co., Ltd.
Certificate No. Q22130792, Due Date 05 January 2024.
2. The measurements are traceable to International System of Units (SI), through Thailand Institute of Scientific and Technological Research (TISTR). Certificate No. PSL-T 0010/66, Due Date 06 November 2023.
3. The measurements are traceable to International System of Units (SI), through National Institute of Metrology (Thailand).
Certificate No. TT-0020-23, Due Date 22 February 2024.

UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2,00$ which for a normal distribution corresponds to a coverage probability of approximately 95 %.
It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

Certificate No. Q23115955

F3-011-04/01-12

page 2 of 3





CLC
Accredited
ISO/IEC 17025

CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



NSC-TISI-TIS 17025
CALIBRATION 0059
CLC

CONDITION OF CALIBRATION ITEM : GOOD

MEASUREMENT RESULTS : (X) without adjustment () adjustment

The DUC Reading were recorded and the means value were reported of five times measurement in the table below.

CALIBRATION DATA

CORRECTION OF TEMPERATURE [THERMISTOR]

Immersion depth (mm)	Actual Temperature (°C)	DUC Reading (°C)	Correction (°C)	Uncertainty \pm (°C)
105	19.99	20.0	-0.01	0.07
	24.98	25.0	-0.02	
	30.01	30.1	-0.09	

Note. Probe \varnothing 3.5 mm

Materials : Metal Sheath.

Note. The Scope of Accredited TISI Certificate No. 23-LB0092 Issue 02 Page 35 of 138

This report is valid for the above stated instrument/s only.

End of Certificate

Certificate No. Q23115955

F3-011-04/01-12

page 3 of 3



@clccalibration

Certificate of Calibration

Certificate No. : 67-200069-1

Page : 1 of 2

Submitted by : Okla Testing&Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Electronic Balance
Manufacturer : Sartorius Model : BSA224S-CW
Serial No. : 35790699
Capacity : 200 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the Laboratory Environmental, Okla
Testing&Consulting Service Co.,Ltd.

Ambient Temperature : (28.4 to 28.5) °C

Relative Humidity : (49.4 to 51.1) %

Air Pressure : 1012.0 mbar

Date of Received : 26 February 2024

Date of Calibration : 26 February 2024

Date of Issue : 27 February 2024

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E264	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-200069-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.01	0.0000	0.00011
0.05	0.0000	0.00011
0.1	0.0000	0.00011
0.2	0.0000	0.00011
0.5	0.0000	0.00011
1	0.0000	0.00011
10	0.0000	0.00011
50	0.0000	0.00014
100	0.0000	0.00020
150	0.0001	0.00038
200	0.0002	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

-0.0001 0.0001 0.0001 0.0000 0.0000 g



Repeatability

Load test : 200 g

Stdev. : 0.00000 g

- o0o -



Certificate of Calibration

Certificate No. : 67-400117-2

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co., Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Watthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Temperature controlled enclosure (Oven)

Manufacturer : KWF

Model : S0V70B

Range : N/A °C

Resolution : 0.1 °C

Serial No. : KWF2021021902

ID No. : OKLA-LAB-013/170621

Environment : On site calibration was carried out at the Laboratory,
Okla Testing & Consulting Service Co., Ltd.

Ambient Temperature : (32.0 to 33.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (221.0 to 223.0) V

Date of Received : 26 February 2024

Date of Calibration : 26 February 2024

Date of Issue : 29 February 2024

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400032	66-400594-1	27 Apr 2024	National Institute of Metrology Thailand (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400117-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

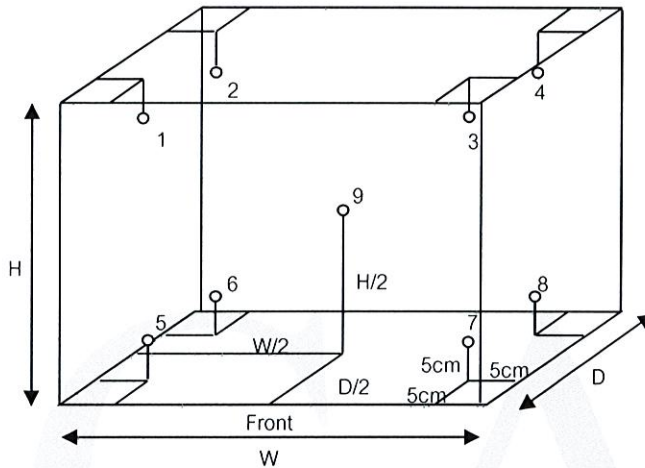

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
104.0	102.5	102.5	106.4	105.0	105.2	106.1	103.0	104.0	103.4	105.4	104.0	0.94
140.0	139.5	139.5	144.1	142.2	142.4	143.7	138.5	139.7	139.3	142.4	140.2	1.3
160.0	159.5	159.5	164.3	162.4	162.6	163.8	158.6	159.8	159.3	162.5	160.3	1.3
180.0	179.5	179.5	186.2	183.7	183.8	185.7	174.7	180.1	179.4	183.7	180.3	1.7

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
104.0	102.5	102.5	2.6	0.3	3.8
140.0	139.5	139.5	4.1	0.4	6.1
160.0	159.5	159.5	4.1	0.4	6.2
180.0	179.5	179.5	6.0	0.6	12.0

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-400117-1

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co., Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : S-Cool

Model : SM 61 M

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 18021147

ID No. : OKLA-LAB-011/190

Environment : On site calibration was carried out at the Laboratory,
Okla Testing & Consulting Service Co., Ltd.

Ambient Temperature : (32.0 to 33.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (221.0 to 223.0) V

Date of Received : 26 February 2024

Date of Calibration : 26 February 2024

Date of Issue : 29 February 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400047	67-400047-2	26 Jul 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400117-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

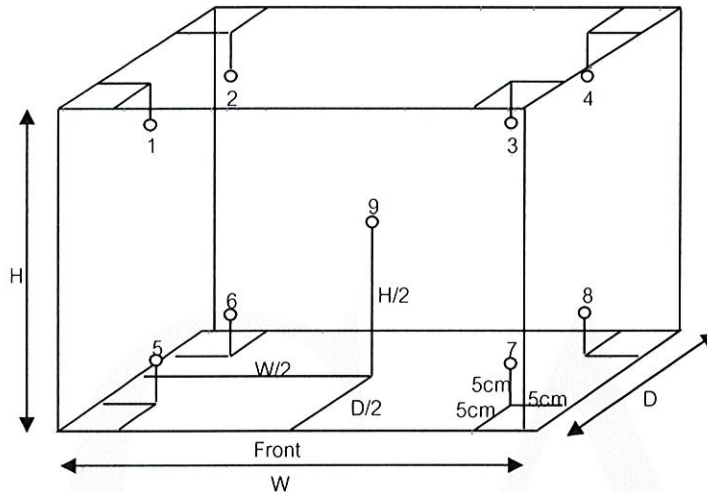

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	20.46	20.25	19.60	19.58	19.84	19.64	19.45	19.59	20.01	0.34

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.589	0.073	1.129

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate No. : J048-TC24021201

Page : 1 of 3

Certificate of Calibration

Customer : Okla Testing & Consulting Service Co., Ltd.

Address : 67/35-36, 3rd Floor, Phetkasem 7/1 Rd.,
Wathapra, Bangkokyai, BKK. 10600

Equipment : Refrigerator

Manufacturer : SANDEN

Model : SPB-0500

Serial No. : SPB0500-231007454

ID No. : -

Resolution : 0.1 °C

Location of Calibration : Central Laboratory FL.3


Reference Job No. : JB24048

Received Request Date : 12 February 2024

Calibrated by : Pawut Wongnarakornkul

Date of Calibration : 12 February 2024

Approved by :



☒ Mr. Pairat Chobna
☐ Mr. Sarawut Panpet

Date of Issue : 13 February 2024

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval the Megafil Co.,Ltd.

Calibration Report

Equipment	: Refrigerator	Manufacturer	: SANDEN
Model	: SPB-0500	Serial No	: SPB0500-231007454
Environment	: Ambient Temperature	(24.3 to 24.9) °C	
	Relative Humidity	(45.3 to 51.9) %	
	Line Voltage	(226 to 228) V _{ac}	

Detail of this calibration result. :

1. This instrument was calibrated by insert 9 standards Resistance Thermometer Detector, in to the chamber, under no load condition in according to TLAS G-20-1/02-08 (E).
2. The temperature scale used was based on ITS-90.
3. Reference standards instrument :

Instrument	Model	Serial No./ID No.	Certificate No.	Due Date
Data Acquisition Switch unit	34972A	MY49010832	QR23-2679	15 November 2024
Resistance Thermometer Detector	100 ohm	RTD505(01 to 10)	QR23-2679	15 November 2024

4. This certificate was certified only for the instrument we calibrated.
5. The measured values in this report refer to the time of examination.
6. This certificate is traceable to SI Unit through Quality Reborn Co.,Ltd.
NSC - ONSC accredited no. Calibration 0292
7. Condition of calibrated item : Good

UUC Description :

Operation time 5 Hour 00 Minute Calibration point 2.0, 4.0, 6.0 °C

The air ventilation of the instrument was set at position.

Fresh Air Damper

<input type="checkbox"/>	Open	Position	<input type="checkbox"/>	Min	<input type="checkbox"/>	Medium	<input type="checkbox"/>	Max
<input type="checkbox"/>	Close							
<input checked="" type="checkbox"/>	X	Not Available						

8 Result of calibration :


(X) Without adjustment () After adjustment

Result of Calibration

Page : 3 of 3

Sensor installation at nine locations as show in figure.

Chamber capacity (W x H x D) : (0.55 x 1.61 x 0.42) m : 0.37 m³

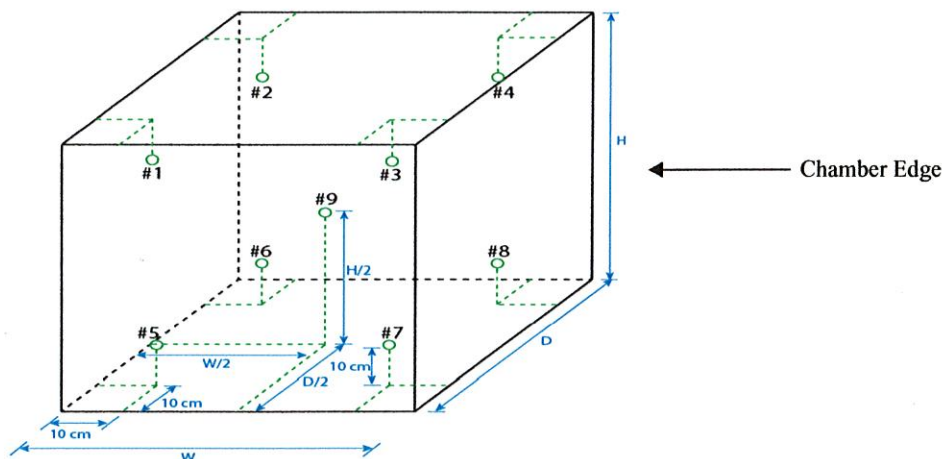

Position	1	2	3	4	5	6	7	8	9
Ref. Std/ID No.:	RTD50501	RTD50502	RTD50503	RTD50504	RTD50505	RTD50506	RTD50507	RTD50508	RTD50509

Temperature distribution

Cal. Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No. (Sensor No.9 is REF)									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
2.0	2.0	2.0	2.03	1.26	1.94	1.31	3.06	2.95	2.21	2.15	2.17	0.44
4.0	4.0	4.0	3.96	3.22	3.84	3.31	5.05	4.91	4.19	4.18	4.14	0.44
6.0	6.0	6.0	5.85	5.16	5.88	5.32	7.07	6.91	6.18	6.24	6.10	0.44

Chamber performance

Cal. Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)			Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
		Min	Max	Average			
2.0	2.0	2.0	2.0	2.0	1.07	0.19	2.06
4.0	4.0	4.0	4.0	4.0	1.09	0.22	2.04
6.0	6.0	6.0	6.0	6.0	0.98	0.24	2.18

Note: The quoted uncertainty include Stability and 20% of Uniformity.

Stability = One-half of the greatest maximum difference of measured temperatures at any one sensor.

Uniformity = The maximum difference of measured temperatures at any sensors and measured temperature at the reference location which are observed at the same time.

Overall Variation = The Difference of the maximum and minimum measured temperatures throughout observation.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%.

- End of Certificate -

Certificate of Calibration

Certificate No. : 67-400117-4

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co., Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Water Bath

Manufacturer : LabTech

Model : LWB-222A

Range : N/A °C

Resolution : 0.01 °C

Serial No. : BCCLJ23001C

ID No. : OKLA-LAB-008/122011

Environment : On site calibration was carried out at the Laboratory,
Okla Testing & Consulting Service Co., Ltd.

Ambient Temperature : (32.0 to 33.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (221.0 to 223.0) V

Date of Received : 26 February 2024

Date of Calibration : 26 February 2024

Date of Issue : 29 February 2024

Calibrated by : Permpoon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400043	66-400593-1	25 Apr 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration


Certificate No. : 67-400117-4

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

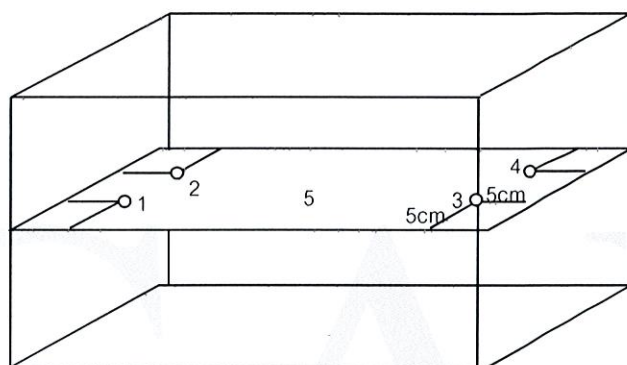

Front

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor					Uncertainty (± ° C)	Measured Uniformity (° C)	Measured Stability (° C)
			No.							
			1	2	3	4	5			
60	As Mark 60	-	60.02	59.97	60.02	59.95	60.05	0.53	0.69	0.40

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Air Temperature measurement laboratory
Calibration services department.

CERTIFICATE OF CALIBRATION

Certificate No. : CAT-006-66

Page 1 of 2 Pages

MEASUREMENT ITEM : Digital Thermo Hygrometer
MANUFACTURER : KEPLER
MODEL/TYPE : KTH-02
SERIAL NUMBER : 234011890
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : Okla Testing and consulting services Co., Ltd.
67/35-36, 3rd Fl, Phetkasem soi 7/1, Wat Thapra,
Bangkokyai, Bangkok, Thailand 10600.

RECEIVED DATE : 18 Oct 2023
MEASUREMENT DATE : 19 Oct 2023
ISSUE DATE : 19 Oct 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Air Temperature calibration was done by In-House calibration method as WI-CL-009 according to comparison method with Standard Chilled Mirror hygrometer and standard Humidity generator chamber.

Traceability:

This instrument was calibrated using standard equipment whose accuracy is traceability through National Institute of Standards and Technology to the international system of units (SI) via Process Sensing Technologies, Corp. Certificate number: 57483-A.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'



Calibrated by:

- ☐ Mr. Sorawit Thachalad
☐ Miss Jitraporn Lertsomphol
☒ Miss Ruangrumpai Phoommit

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number: CAT-006-66

Page 2 of 2 Pages

Measurement Results:

This equipment was connected with Air temperature Sensor on display. Model: -, Serial number: -.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 20 °C to 30 °C

The results of calibration of air temperature are reported in table below.

<u>Determined</u> (°C)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
20.0	20.00	20.1	0.1	0.30
25.0	25.00	25.3	0.3	0.30
30.0	30.00	30.3	0.3	0.30

UUC*: Unit Under Calibration

End of Certificate of Calibration





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd
63/14-15, 67/35-36
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,
Bangkok 10600 (Thailand)
Tel: +6608680812
Mobile: +66863999453
E-mail: jnac-calibration@jiranatee.com
Web site: www.jiranatee.com

Accredited calibration laboratory
ISO/IEC 17025:2017
NSC-TISI-TIS 17025
CALIBRATION 0367

Relative humidity measurement laboratory
Calibration services department.

CERTIFICATE OF CALIBRATION

Certificate No. : CRH-008-66

Page 1 of 2 Pages

MEASUREMENT ITEM : Digital Thermo Hygrometer
MANUFACTURER : KEPLER
MODEL/TYPE : KTH-02
SERIAL NUMBER : 234011890
ID NUMBER : -
CONDITION AS-RECEIVED : Used item
CUSTOMER : Okla Testing and consulting services Co., Ltd.
67/35-36, 3rd Fl, Phetkasem soi 7/1, Wat Thapra,
Bangkokyai, Bangkok, Thailand 10600.

RECEIVED DATE : 18 Oct 2023
MEASUREMENT DATE : 19 Oct 2023
ISSUE DATE : 19 Oct 2023

ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:

The table on next page give the measured values.

Calibration procedure:

The Relative humidity calibration was done by In-House calibration method as WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer and standard Humidity generator chamber.

Traceability:

This instrument was calibrated using standard equipment whose accuracy is traceability through National Institute of Standards and Technology to the international system of units (SI) via Process Sensing Technologies, Corp. Certificate number: 57483-A.

Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor $k=2$, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'



Calibrated by:

- ☐ Mr. Sorawit Thachalad
☐ Miss Jittraporn Lertsomphol
☒ Miss Ruangrumpai Phoommit

Approved signatory:

Mr. Parinya Booncharoen
Calibration Department Manager

Measurement Results:

This equipment was connected with Relative humidity Sensor on display. Model: -, Serial number: -.

Result of Calibration: ☒ Without Adjustment ☐ With Adjustment

Calibration Range: 40%RH to 80%RH

The results of calibration of relative humidity are reported in table below.

<u>Determined</u> (%RH)	<u>Standard Reading</u> (%RH)	<u>UUC Reading</u> (%RH)	<u>Error</u> (%RH)	<u>Uncertainty</u> (%RH)
40.0	40.12	40.0	-0.1	1.16
60.0	60.22	60.0	-0.2	1.17
80.0	80.39	79.0	-1.4	1.15

UUC*: Unit Under Calibration

End of Certificate of Calibration



Certificate of Calibration

Certificate No. : 67-300115-14

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Burette
Manufacturer : ISOLAB Class : A
Capacity : 25 ml Graduation : 0.05 ml
ID No. : BU25/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1011.8 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Wipa Tovadec

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241003	66-200388-2	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadec)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-14

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 38.85 sec.

Nominal Volume (ml)	Measuring Volume (ml)
5	5.0020
15	14.9767
25	24.9836

Uncertainty of measurement with in \pm 0.0066 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300115-12

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Cylinder
Manufacturer : DURAN Class : A
Capacity : 100 ml Graduation : 1 ml
ID No. : CY100/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1011.1 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Kovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-12

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
50	50.07
100	100.13

Uncertainty of measurement with in \pm 0.063 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300115-11

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.

67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Cylinder

Manufacturer : FAVORIT

Class : A

Capacity : 50 ml

Graduation : 1 ml

ID No. : CY50/01

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1005.8 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-11

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
30	30.24
50	50.27

Uncertainty of measurement with in \pm 0.054 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300115-13

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Cylinder
Manufacturer : BOROSIL Class : A
Capacity : 500 ml Graduation : 5 ml
ID No. : CY500/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1005.7 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-13

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
250	248.94
500	499.25

Uncertainty of measurement with in \pm 0.12 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300115-1

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Measuring Pipette

Manufacturer : GLASSCO

Class : A

Capacity : 1 ml

Graduation : 0.01 ml

ID No. : MP1/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1007.4 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	66-200388-4	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-1

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 5.89 sec.

Nominal Volume (ml)	Measuring Volume (ml)
0.1	0.1010
0.5	0.4988
1	1.0004

Uncertainty of measurement with in \pm 0.0026 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300115-2

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.

67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Measuring Pipette

Manufacturer : GLASSCO

Class : A

Capacity : 5 ml

Graduation : 0.05 ml

ID No. : MP5/01

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1007.4 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.

Cert. No.

Due Date

Traceability

241005

66-200388-4

02 Jun 2024

National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-2

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 9.75 sec.

Nominal Volume (ml)	Measuring Volume (ml)
0.5	0.5023
2.5	2.4847
5	4.9835

Uncertainty of measurement with in \pm 0.0027 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300115-3

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Measuring Pipette

Manufacturer : GLASSCO

Class : A

Capacity : 10 ml

Graduation : 0.1 ml

ID No. : MP10/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1007.2 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	66-200388-4	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-3

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 11.11 sec.

Nominal Volume (ml)	Measuring Volume (ml)
1	1.0010
5	4.9790
10	9.9759

Uncertainty of measurement with in \pm 0.0039 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300115-6

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Pipette
Manufacturer : GLASSCO Class : A
Capacity : 20 ml
ID No. : VP20/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1007.6 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	66-200388-4	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-6

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 15.28 sec.

Nominal Volume (ml)	Measuring Volume (ml)
20	20.0063

Uncertainty of measurement with in \pm 0.0064 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300115-8

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wattthapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Flask

Manufacturer : SCI

Class : A

Capacity : 100 ml

ID No. : VF100/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1005.8 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	66-200388-4	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-8

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
100	99.983

Uncertainty of measurement with in \pm 0.018 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300115-9

Page : 1 of 2

Submitted by : Okla Testing & Consulting Service Co.,Ltd.
67/35-36, 3rd Floor, Petchkasem 7/1, Petchkasem Rd.,
Wathapra, Bangkok Yai, Bangkok 10600 Thailand

Equipment : Volumetric Flask
Manufacturer : BOROSIL Class : A
Capacity : 500 ml
ID No. : VF500/01

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1006.0 mbar.

Date of Received : 26 February 2024

Date of Calibration : 02 March 2024

Date of Issue : 02 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300115-9

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
500	499.92

Uncertainty of measurement with in \pm 0.075 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- oOo -



Certificate of Calibration

Certificate No. : 67-200134-1

Page : 1 of 2

Submitted by : HVE Co.,Ltd.

603 Soi Jarunsanitwong 46, Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : Electronic Balance

Manufacturer : SHIMADZU **Model :** AX200

Serial No. : D432620040 **ID No. :** 114

Capacity : 200 g **Resolution :** 0.0001 g

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (30.8 to 31.6) °C

Relative Humidity : (50.4 to 53.4) %

Air Pressure : 1008.0 mbar

Date of Received : 17 April 2024

Date of Calibration : 17 April 2024

Date of Issue : 24 April 2024

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-200134-1

Page : 2 of 2

Result of Calibration : After Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)	Error before Adjustment (g)
0.01	0.0000	0.00012	0.0000
0.1	0.0000	0.00012	0.0000
0.5	0.0000	0.00013	0.0000
1	-0.0001	0.00013	0.0000
10	0.0000	0.00013	-0.0002
20	0.0000	0.00014	-0.0003
50	0.0001	0.00015	-0.0004
100	0.0001	0.00020	-0.0007
150	0.0002	0.00038	-0.0014
200	0.0005	0.00038	-0.0019

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error Load test : 50 g

A	B	C	D	E	
0.0003	-0.0006	-0.0003	0.0006	0.0000	g



Repeatability Load test : 200 g

Stdev. : 0.00005 g

- o0o -



Certificate No. C17240065

Calibration Certificate

Equipment:	Oven	Job No.:	KSMT2400663
Model:	UNB 500	Received Date:	01 April 2024
Serial No.(or ID):	C507.1007 (012)	Issued Date:	03 April 2024
Manufacturer:	Memmert	Page:	1 of 4
Condition:	In Condition		
Ventilation Valve:	Closed	Shelves(pc.):	2

Customer

HVE Co., Ltd.
603 Soi Charansanitwong 46, Charansanitwong Road Bang Yi Khan, Bang Phlat, Bangkok 10700

Calibration Place

HVE Co., Ltd. (Laboratory)
603 Soi Charansanitwong 46, Charansanitwong Road Bang Yi Khan, Bang Phlat, Bangkok 10700

Calibration Date

01 April 2024

Environment Condition

Temperature: 30.1 °C \pm 1.3 °C
Humidity: 60.9 %RH \pm 3.3 %RH

The Method used

In-house method, WI17, based on TLAS-G20

Traceability

This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Quality Reborn Co.,Ltd.Certificate No. QR23-1906

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of SCIMET Co., Ltd.




(Mr. Hattapong Pumnil)

Person in charge



(Mr. Thalerngkeat POUNGNGAM)

Authorized signatory

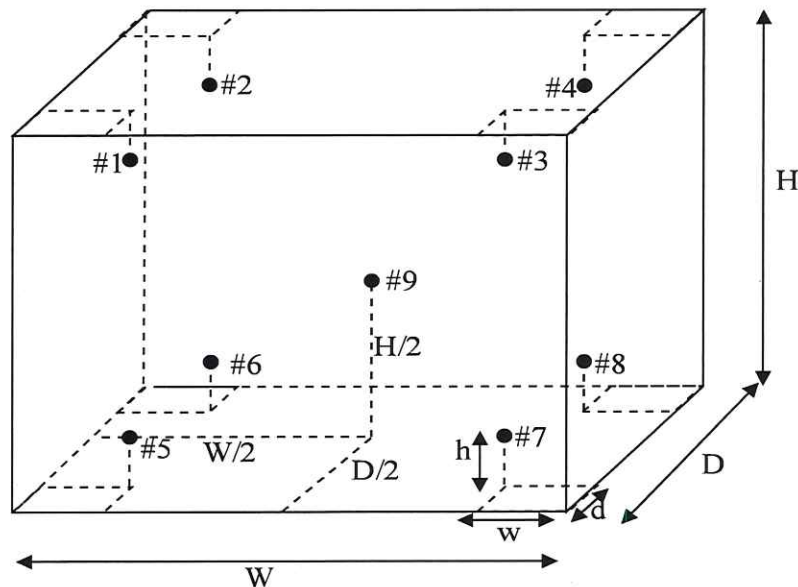

Standard Installation Locations

Volume (Calibration Zone)= 6 (Liters)

Inside chamber: $W = 56$ (cm) $D = 40$ (cm) $H = 48$ (cm)

Standard Locations (#1, #2, #3, #4): $w = 20$ (cm) $d = 10$ (cm) $h = 15$ (cm)

Standard Locations (#5, #6, #7, #8): $w = 20$ (cm) $d = 10$ (cm) $h = 15$ (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	101	102	103	104	105	106	107	108	109

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results:

Pre-Calibration

Desired	Setting	Indicating	#1	#2	#3	#4	#5	#6	#7	#8	#9
104.0	104.0	104.0	103.23	103.17	103.10	103.10	101.81	101.68	101.89	101.61	102.51

Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 105.5 °C

Locations	Measured Temperature (°C)	Correction (°C)	Uncertainty (± °C)
#1	104.48	0.48	0.39
#2	104.51	0.51	0.39
#3	104.43	0.43	0.39
#4	104.45	0.45	0.39
#5	103.20	-0.80	0.39
#6	103.11	-0.89	0.39
#7	103.27	-0.73	0.39
#8	103.07	-0.93	0.39
#9	103.87	-0.13	0.39

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
104.0	105.5	105.5	104.48	104.51	104.43	104.45	103.20	103.11	103.27	103.07	103.87	0.39

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
105.5	0.89	0.12	1.64

Note: * Maximum uncertainty of the each position

Without adjustment (Cont.)

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 182.0 °C

Locations	Measured Temperature (°C)	Correction (°C)	Uncertainty (± °C)
#1	181.05	1.05	0.49
#2	181.24	1.24	0.49
#3	180.99	0.99	0.49
#4	181.18	1.18	0.49
#5	179.64	-0.36	0.50
#6	179.63	-0.37	0.51
#7	179.84	-0.16	0.50
#8	180.00	0.00	0.50
#9	180.18	0.18	0.50

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
180.0	182.0	182.0	181.05	181.24	180.99	181.18	179.64	179.63	179.84	180.00	180.18	0.51

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
182.0	1.17	0.16	1.83

Note: * Maximum uncertainty of the each position

The End of Certificate

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The correction of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, TLAS-G20. Therefore, those parameters have not

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk $< 50\%$ PFA.
- ☒ Choice B Non-binary statement with guard band ($w = 1$ U), Pass or Fail Specific Risk $< 2.5\%$ PFA and Condition Pass or Condition Fail Specific Risk $< 50\%$ PFA.
- ☐ Choice C Customer defined, Customers may define arbitrary multiple of r to have applied as guard band ($w = r$ U) .
- ; PFA: Probability of False Accept



(Mr. Thalerngkeat Pongngam)

Authorized signatory

Without adjustment

Desired Temperature : 104.0°C

Tolerances : 1.0 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 105.5 °C

Locations	Measured (°C)	Correction of UUC. (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	104.48	0.48	0.39	1.0	Pass
#2	104.51	0.51	0.39	1.0	Pass
#3	104.43	0.43	0.39	1.0	Pass
#4	104.45	0.45	0.39	1.0	Pass
#5	103.20	-0.80	0.39	1.0	Condition Pass
#6	103.11	-0.89	0.39	1.0	Condition Pass
#7	103.27	-0.73	0.39	1.0	Condition Pass
#8	103.07	-0.93	0.39	1.0	Condition Pass
#9	103.87	-0.13	0.39	1.0	Pass

Correction of UUC.* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.

Statements of conformity:(Cont.)

Without adjustment (Cont.)

Desired Temperature : 180.0°C

Tolerances : 2 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 182.0 °C

Locations	Measured (°C)	Correction of UUC. (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	181.05	1.05	0.49	2	Pass
#2	181.24	1.24	0.49	2	Pass
#3	180.99	0.99	0.49	2	Pass
#4	181.18	1.18	0.49	2	Pass
#5	179.64	-0.36	0.50	2	Pass
#6	179.63	-0.37	0.51	2	Pass
#7	179.84	-0.16	0.50	2	Pass
#8	180.00	0.00	0.50	2	Pass
#9	180.18	0.18	0.50	2	Pass

Correction of UUC.* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use.


The End of Statements of Conformity

Corr_Distribution & Max_Measurement Uncertainty

Job_No. KSMT2400663

Without adjustment

Correction (°C)

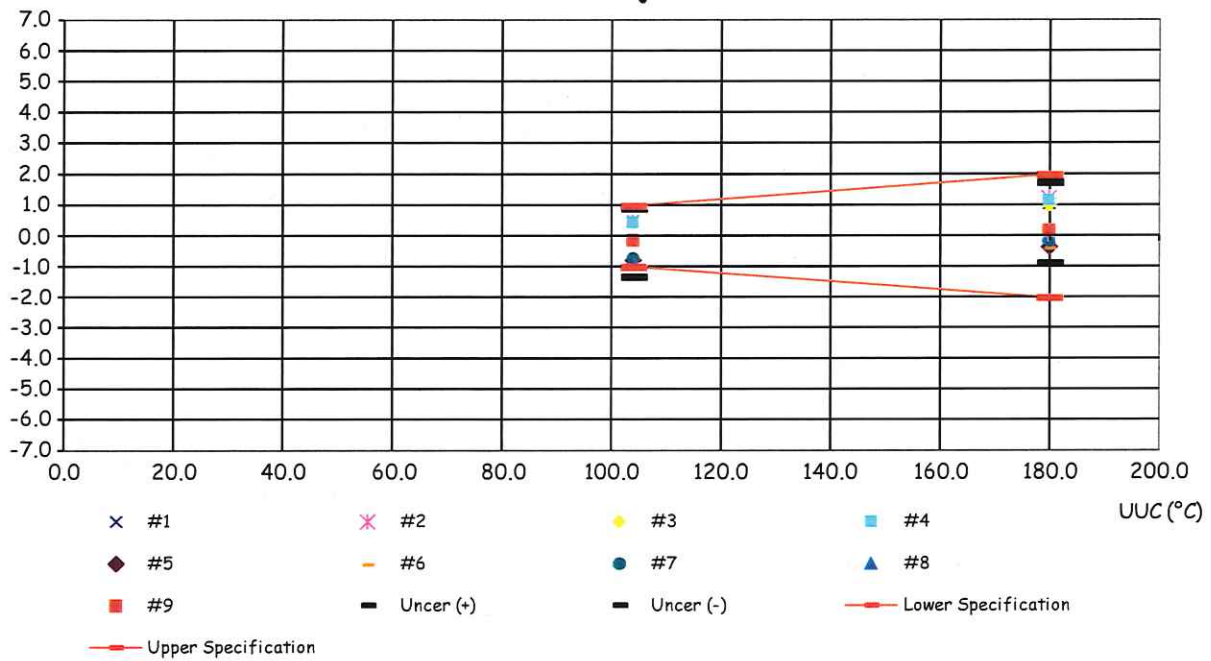


Temperature Distribution @ 104.0°C

Job_No. KSMT2400663

Without adjustment


Std(°C)

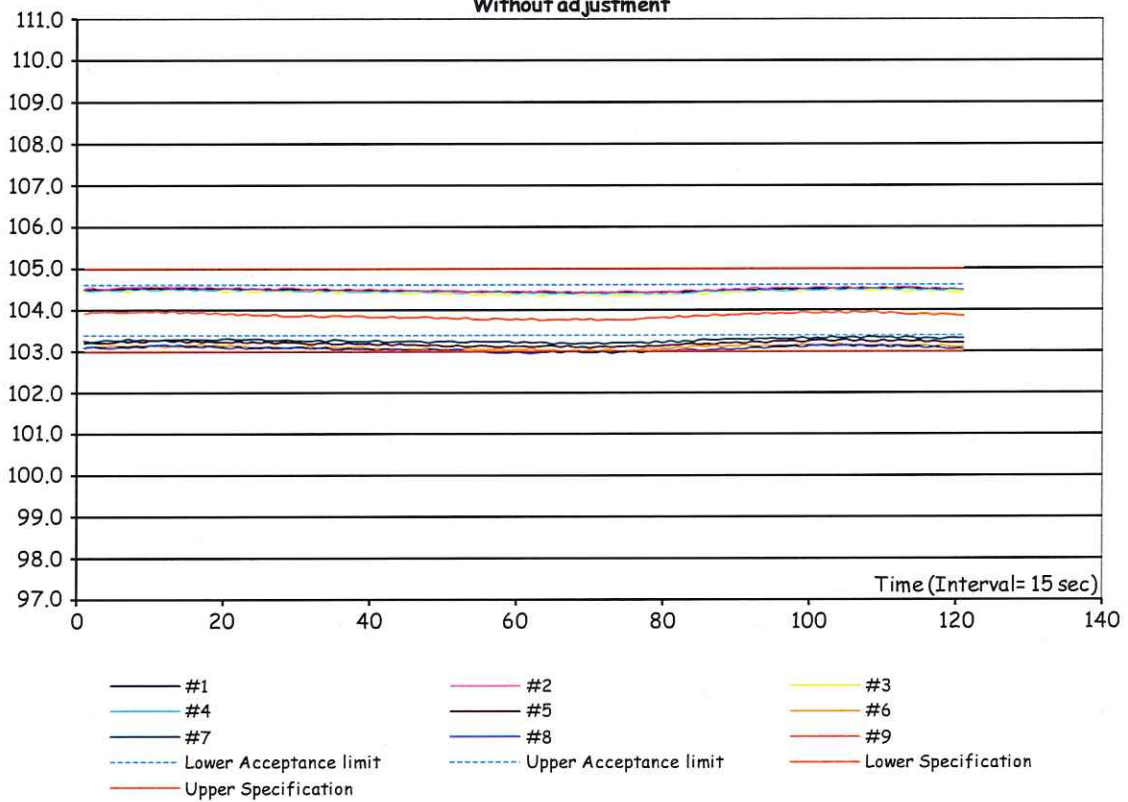

Temperature Distribution @ 180.0°C

Job_No. KSMT2400663

Without adjustment (Cont.)

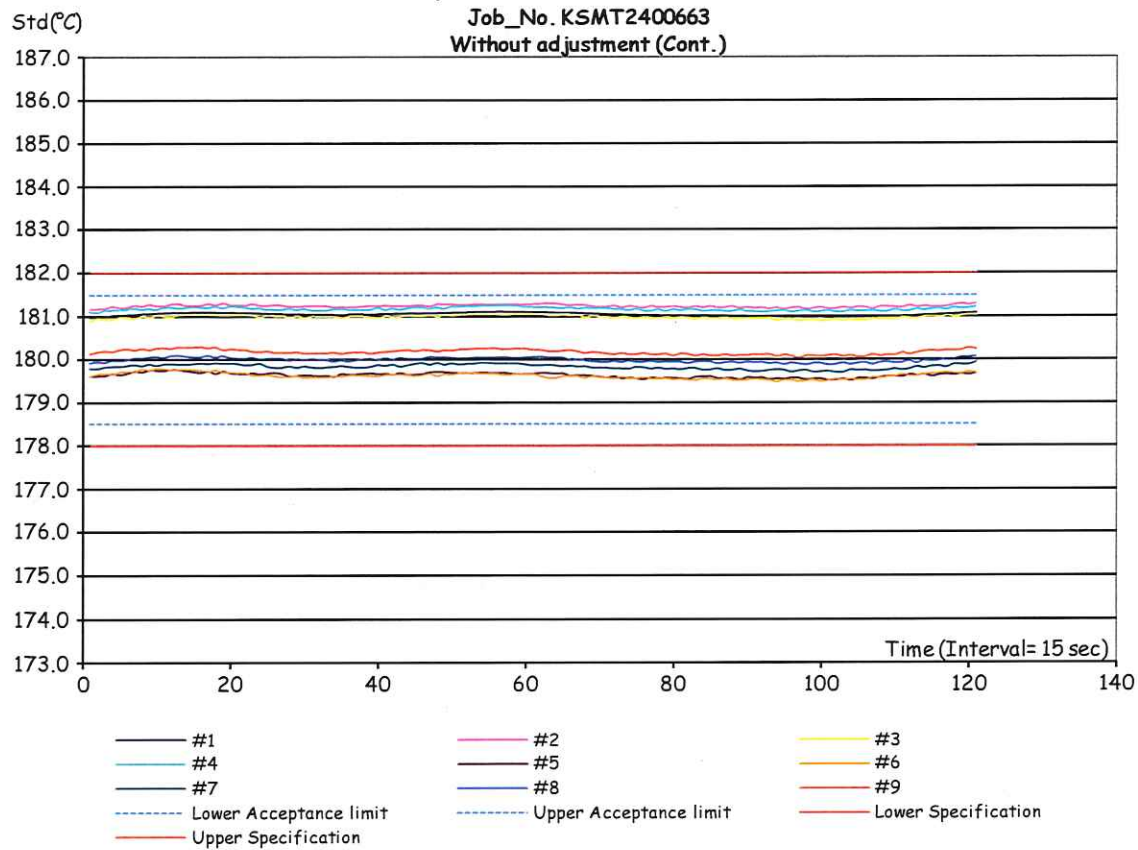



ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: KSMT2400663

ชนิดเครื่องมือ: Oven

รุ่น: UNB 500

หมายเลขเครื่อง: C507.1007 (012)

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
01 Apr 2024			01 Apr 2024		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. สายไฟ	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การแสดงผล Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	5. การทำงาน พัดลม	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. สภาพ Lever of Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สภาพ Lever door open / close	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. สภาพ Door seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานของระบบ Safety	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	10. การทำงานของระบบทำความเย็น	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input type="checkbox"/>	<input type="checkbox"/>	11. การทำงานของระบบทำความชื้น	<input type="checkbox"/>	<input type="checkbox"/>	ไม่มี
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. สภาพตัวเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	13. สภาพแวดล้อม ณ สถานที่ตั้งเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

ข้อแนะนำ :

Mr. Hattapong Pumnil

Service Engineer

บริษัท ชายนีเมท จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 02 460 9239

FI17-00: 08 MAR 2023

Certificate of Calibration

Certificate No. : 67-400216-6

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46, Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Lovibond

Model : ET636-6

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 9982523-03

ID No. : 011

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (27.0 to 28.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (229.0 to 230.0) V

Date of Received : 17 April 2024

Date of Calibration : 18 April 2024

Date of Issue : 19 April 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400047	67-400047-2	26 Jul 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400216-6


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

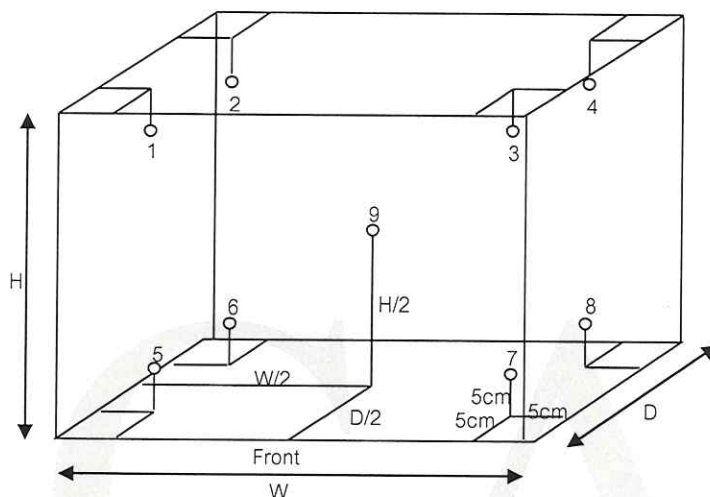

Inside of Chamber

W = 0.53 m

D = 0.43 m

H = 1.40 m

Capacity = 0.32 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	21.0	21.0	20.24	20.19	20.28	20.16	20.15	20.08	19.95	19.87	19.98	0.36

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	21.0	21.0	0.3	0.1	0.6

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-420044-2

Page : 1 of 2

Submitted by : HVE Co., Ltd.

603 Soi Jarunsanitwong 46 Jarunsanitwong Road, Bangyeekun, Bangplad, Bangkok 10700

Equipment : pH Meter with electrode

pH meter

Manufacturer : Hanna

Model : HI 2211

Range : N/A pH

Resolution : 0.01 pH

Serial No. : 08376721

ID No. : N/A

Electrode

Model : HI 1131

Serial No. : 084809EN

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (25.0 to 26.0)° C

Relative Humidity : (40 to 45) %

Date of Received : 18 April 2024

Date of Calibration : 18 April 2024

Date of Issue : 19 April 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Certified Reference Material (CRM)

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	944535	27 Nov 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	944537	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	944536	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-420044-2

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement
pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7) and (7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7	177.4800	4	4.00	177.3	0.2	0.12
	0.0000	7	7.00	0.0	0.0	0.086
7,10	0.0000	7	7.00	0.0	0.0	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7) and (7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7	4.008	4.01	0.00	0.010
	6.986	7.01	-0.02	0.011
7, 10	6.986	7.01	-0.02	0.011
	9.997	10.01	-0.01	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- ๐0๐ -



Certificate of Calibration

Certificate No. : 67-400222-2

Page : 1 of 2

Submitted by : HVE Co.,Ltd.

603 Soi Jarunsanitwong 46 Jarunsanitwong Road, Bangyeekun Bangplad Bangkok 10700

Equipment : Digital Thermometer with Thermistor Probe (Temp pH)
Temperature Indicator

Manufacturer : Hanna

Model : HI 2211

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 08376721

ID No. : N/A

Thermistor Probe

Model : N/A

Sheath Material : Stainless

Diameter : 3.5 mm.

Length : 100 mm.

Serial No. : N/A

ID No. : 08376721

Environment : On site calibration was carried out at the Laboratory, HVE Co., Ltd.

Ambient Temperature : (25.0 to 26.0) °C

Relative Humidity : (40 to 45) %

Line Voltage : (229.0 to 230.0) VAC

Date of Received : 18 April 2024

Date of Calibration : 18 April 2024

Date of Issue : 19 April 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No.	Cert. No.	Due Date	Traceability
400002	TT-0074-22	20 Jun 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No.	Cert. No.	Due Date	Traceability
400033	24E633	21 Feb 2026	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400222-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (±°C)
100	25.002	24.8	0.2	0.19

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES



Cert.No.: 24TW74

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %

Dissolved Oxygen Probe No.: 07-07

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.20	8.2	0.045

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-

a 1209346



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-23-754

Page : 1 of 4

CERTIFICATE OF CALIBRATION

Equipment	:	Spectrophotometer
Manufacturer	:	Thermo Scientific
Model	:	Genesys 10S UV-VIS
Serial No.	:	2L9Q310003
ID No.	:	071
Customer	:	HVE CO., Ltd.
	:	603 Soi Jarunsanitwong 46, Jarunsanitwong Road,
	:	Bangyeekun, Bangplad, Bangkok 10700
Location	:	แผนกน้ำรีโค
Date of Receipt	:	21 November 2023
Date of Calibration	:	21 November 2023
Date of Issue	:	21 November 2023
Ambient Temperature	:	(25±10) °C
Relative Humidity	:	(60±20) %
Condition As-Received	:	Used Item

Calibrated by

.....

(Mr.Somphop Duangnguan)

Calibration Engineer

Approved by

.....

(Ms. Jintana Sangthaijaroenlap)

Calibration Manager

The reported expanded uncertainty of measurement was based on a combined standard uncertainty multiplied by a coverage factor $k=2$, providing a level of confidence of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Indicated values are valid for the state of the Spectrophotometer at the time of calibration only.



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-23-754

Page : 2 of 4

CALIBRATION REPORT

Conditions of this result of calibration

1. Reference Standard Material :

<u>Material</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert.No.</u>	<u>Due date</u>
Holmium Glass Filter	RM-HG	24563	109211	13 Feb 25
Didymium Glass Filter	RM-DG	24562	109212	13 Feb 25
Neutral Density Filter	RM-1N2N3N	24568	109249	14 Feb 25
Potassium Dichromate Solution	RM-06	24567	109222	13 Feb 25

2. Traceability : This certification is traceable to the International System of Unit maintained at;

The Starna Scientific Ltd. Accredited Calibration Laboratory No. 0659.

3. Method of calibration :

The calibration procedure was carried out according to ASTM E275-08 (2022) and ASTM E925-09 (2014).

4. Result of calibration :

(✓) without adjustment

() after adjustment

5. Equipment Specifications:

Spectral Bandwidth :	1.8	nm
Data Interval :	0.1	nm
Scan Speed :	Slow	nm/min



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-23-754

Page : 3 of 4

CALIBRATION REPORT

Wavelength Calibration

Certified Values of Reference Material (nm)	Nominal Value (nm)	UUC*Reading (nm)	Error (nm)	Uncertainty of Measurement (\pm nm)
361.00	361.00	360.7	-0.30	0.13
536.66	536.66	536.7	0.04	0.13
879.27	879.27	879.8	0.53	0.13

Photometric Calibration for Visible

Wavelength (nm)	Certified Values of Reference Material (A)	UUC* Reading (A)	Error (A)	Uncertainty of Measurement (\pm A)
420.0	Zero	0.000	0.0000	0.0028
	0.5835	0.585	0.0015	0.0044
	0.725	0.725	0.0000	0.0040
	1.0367	1.037	0.0003	0.0039
440.0	Zero	0.000	0.0000	0.0028
	0.5662	0.567	0.0008	0.0042
	0.7106	0.710	-0.0006	0.0037
	1.0159	1.016	0.0001	0.0037
465.0	Zero	0.000	0.0000	0.0028
	0.5257	0.527	0.0013	0.0044
	0.6682	0.668	-0.0002	0.0039
	0.9547	0.954	-0.0007	0.0034
546.1	Zero	0.000	0.0000	0.0028
	0.5226	0.523	0.0004	0.0036
	0.6939	0.693	-0.0009	0.0039
	0.9919	0.991	-0.0009	0.0032
590.0	Zero	0.000	0.0000	0.0028
	0.5567	0.556	-0.0007	0.0035
	0.7502	0.748	-0.0022	0.0037
	1.0732	1.071	-0.0022	0.0033
635.0	Zero	0.000	0.0000	0.0028
	0.5643	0.563	-0.0013	0.0035
	0.7299	0.728	-0.0019	0.0038
	1.0437	1.042	-0.0017	0.0034

Remark : Each individual filter is measured against the empty filter holder (blank) used to zero the Spectrophotometer.

Note:

UUC* : Unit Under Calibration



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

300 Phaholyothin Road, Phayathai, Bangkok 10400, Thailand Tel: +66 2615-2929 Fax: +66 2615-2350-1
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-23-754

Page : 4 of 4

CALIBRATION REPORT

Photometric Calibration for UV

Wavelength (nm)	Certified Values of Reference Material (A)	UUC* Reading (A)	Error (A)	Uncertainty of Measurement (\pm A)
235.0	Zero	0.000	0.0000	0.0050
	0.7385	0.735	-0.0035	0.0076
257.0	Zero	0.000	0.0000	0.0050
	0.8556	0.851	-0.0046	0.0077
313.0	Zero	0.000	0.0000	0.0050
	0.2882	0.288	-0.0002	0.0059
350.0	Zero	0.000	0.0000	0.0050
	0.6346	0.631	-0.0036	0.0069

Remark : The Potassium Dichromate Filled cells are measured against a Perchloric acid blank.

Note:

UUC* : Unit Under Calibration

- End of Report -