

ภาคผนวก ง

ใบรับรองผลการตรวจวิเคราะห์คุณภาพอากาศ



บริษัท ซี.ที. เอ็นไวรอนเม้นท์ แอนด์ เคมีคัล จำกัด

C.T. ENVIRONMENT AND CHEMICAL CO., LTD. E-mail: cte_envi@yahoo.com. http://www.ctenvi.com

9/40-41 ม.2 ต.บางคูเวียง อ.บางกรวย จ.นนทบุรี 11130 โทรศัพท์ : 02-101-3409 โทรสาร: 02-101-3410

9/40-41 Moo. 2 T.Bangkooveang A.Bangkruai Nonthaburi 11130 TEL: 02-101-3409 FAX: 02-101-3410


ANALYSIS / TEST REPORT

Lab No. WP263/67

Project : Staybridge Suites Bangkok Thonglor, an IHG Hotel
Address : 101 ถนนทองหล่อ แขวงคลองตันเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
Type of Sample : Air Collected Date : June 07, 2024
Method Of Analyzer : Gas Chromatography Receive Date : June 08, 2024
Collected By : C.T. Environment and Chemical Co., Ltd. Analytical Date : June 17, 2024

Location	Parameter	Unite	Results	Standard ^{1/}
พื้นที่โครงการ	Total Hydrocarbon	ppm	<0.001	-
		mg/m ³	<0.001	-

Source : ^{1/} Notification of the Ministry of Interior, issued under the Announcement of the Revolutionary Party, No.103, dated May 30, B.E. 2520 (1977), published in the Royal Government Gazette Vol.94, Part 64, dated July 12, B.E. 2520 (1977)



Analyst Supervisor

Do not copy partial of this analysis report without authorize signature approval

Report analysis refer to submitted sample(s) only

Page 1 of 3



บริษัท ซี.ที. เอ็นไวรอนเม้นท์ แอนด์ เคมีคัล จำกัด

C.T. ENVIRONMENT AND CHEMICAL CO., LTD. E-mail: cte_envi@yahoo.com. http://www.ctenvi.com

9/40-41 ม.2 ต.บางคูเวียง อ.บางกรวย จ.นนทบุรี 11130 โทรศัพท์ : 02-101-3409 โทรสาร: 02-101-3410

9/40-41 Moo. 2 T.Bangkooveang A.Bangkruai Nonthaburi 11130 TEL: 02-101-3409 FAX: 02-101-3410

ANALYSIS / TEST REPORT

Lab No. WP263/67

Project : Staybridge Suites Bangkok Thonglor, an IHG Hotel
Address : 101 ถนนทองหล่อ แขวงคลองตันเหนือ เขตวัฒนา กรุงเทพมหานคร 10110
Type of Sample : High Volume Collected Date : June 07, 2024
Method Of Analyzer : Gravimetric Receive Date : June 08, 2024
Collected By : C.T. Environment and Chemical Co., Ltd. Analytical Date : June 17, 2024

Parameter	Unite	Results	Standard ^{1/}
		พื้นที่โครงการ	
Total Suspended Particulate Matter (TSP)	mg/m ³	0.036	0.33
Particulate Matter Less Than 10 Micron (PM-10)	mg/m ³	0.018	0.12

Source : ^{1/} Notification of the Ministry of Natural Resource and Environment, dated August 9, B.E.2547 (2004), published in the Royal Government Gazette, Vol. 121, Part 105 D, dated September 22, B.E. 2547 (2004).



Mr. Chainarong Toeakbandit

Analyst Supervisor

Do not copy partial of this analysis report without authorize signature approval

Report analysis refer to submitted sample(s) only

Page 2 of 3



บริษัท ซี.ที. เอ็นไวรอนเมนต์ แอนด์ เคมีคัล จำกัด

C.T. ENVIRONMENT AND CHEMICAL CO., LTD. E-mail: cte_envi@yahoo.com. http://www.ctenvi.com

9/40-41 ม.2 ต.บางคูเวียง อ.บางกรวย จ.นนทบุรี 11130 โทรศัพท์ : 02-101-3409 โทรสาร: 02-101-3410

9/40-41 Moo. 2 T.Bangkooveang A.Bangkruai Nonthaburi 11130 TEL: 02-101-3409 FAX: 02-101-3410

ANALYSIS / TEST REPORT

Lab No. WP263/67

Project : Staybridge Suites Bangkok Thonglor, an IHG Hotel

Address : 101 ถนนทองหล่อ แขวงคลองตันเหนือ เขตวัฒนา กรุงเทพมหานคร 10110

Location : พื้นที่โครงการ

Type of Sample : Analyzer

Collected Date : June 07, 2024

เวลา	NO ₂ (mg/m ³)	CO (mg/m ³)
14.00 – 15.00 น.	0.0047	0.011
15.00 – 16.00 น.	0.0030	0.010
16.00 – 17.00 น.	0.0011	0.012
17.00 – 18.00 น.	0.0016	0.010
18.00 – 19.00 น.	0.0045	0.010
19.00 – 20.00 น.	0.0008	0.010
20.00 – 21.00 น.	0.0011	0.014
21.00 – 22.00 น.	0.0002	0.013
22.00 – 23.00 น.	0.0002	0.009
23.00 – 00.00 น.	0.0022	0.008
00.00 – 01.00 น.	0.0004	0.006
01.00 – 02.00 น.	0.0009	0.007
02.00 – 03.00 น.	0.0019	0.008
03.00 – 04.00 น.	0.0035	0.008
04.00 – 05.00 น.	0.0037	0.010
05.00 – 06.00 น.	0.0004	0.007
06.00 – 07.00 น.	0.0003	0.015
07.00 – 08.00 น.	0.0012	0.012
08.00 – 09.00 น.	0.0017	0.011
09.00 – 10.00 น.	0.0040	0.009
10.00 – 11.00 น.	0.0050	0.009
11.00 – 12.00 น.	0.0087	0.010
12.00 – 13.00 น.	0.0017	0.013
13.00 – 14.00 น.	0.0020	0.016
ค่าเฉลี่ย 24 ชั่วโมง	0.0023	0.010
ค่าสูงสุด 1 ชั่วโมง	0.0087	0.016
ค่ามาตรฐาน 24 ชั่วโมง	-	-
ค่ามาตรฐาน 1 ชั่วโมง	0.32	34.2



Mr. Chainarong Toeakbandit

Analyst Supervisor

Do not copy partial of this analysis report without authorize signature approval

Report analysis refer to submitted sample(s) only

Page 3 of 3

ภาคผนวก จ

สำหรับเอกสารการสอบเทียบเครื่องมือตรวจวัดคุณภาพน้ำและอากาศ



บริษัท ซี.ที. เอ็นไวรอนเม้นท์ แอนด์ เคมีคัล จำกัด

C.T. ENVIRONMENT AND CHEMICAL CO., LTD. E-mail: cte_envi@yahoo.com.

9/40-41 ม.2 ต.บางคูเวียง อ.บางกรวย จ.นนทบุรี 11130 โทรศัพท์: 02-101-3409 โทรสาร: 02-101-3410

9/40-41 Moo. 2 T.Bangkooveang A.Bangkrui Nonthaburi 11130 TEL: 02-101-3409 FAX: 02-101-3410

Analyzer Performance Test

Calibrated Date: 30 April 2024

Instruments Information

Analyzer Type: NO/NO₂/NO_x Analyzer
Model: 42C

Manufacturer: Thermo Environmental
S/N: 42C-69067-362

Calibration System

Calibrator Unit	Standard Gas
Dilutor Model API Model 700 S/N: 556	NO Conc 45.4 PPM SO ₂ Conc 44.9 PPM CO Conc 4,480 PPM Expire Date: 30 April 2025
ZERO AIR Generator API Model 701 S/N: 233	

Environment: Temperature 25.5 °C


Humidity: 51 %RH

Calibration Check (Before adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.1	0.0	0.1	398.6	400.0	-0.3
NO _x	0.1	0.0	0.1	400.0	400.0	0.0

Calibration Check (After adjust)

GAS	Zero			Span		
	Reading Value (ppb)	Expected Value (ppb)	Drift (ppb)	Reading Value (ppb)	Expected Value (ppb)	Drift%
NO	0.0	0.0	0.0	400.0	400.0	0.0
NO _x	0.0	0.0	0.0	400.0	400.0	0.0

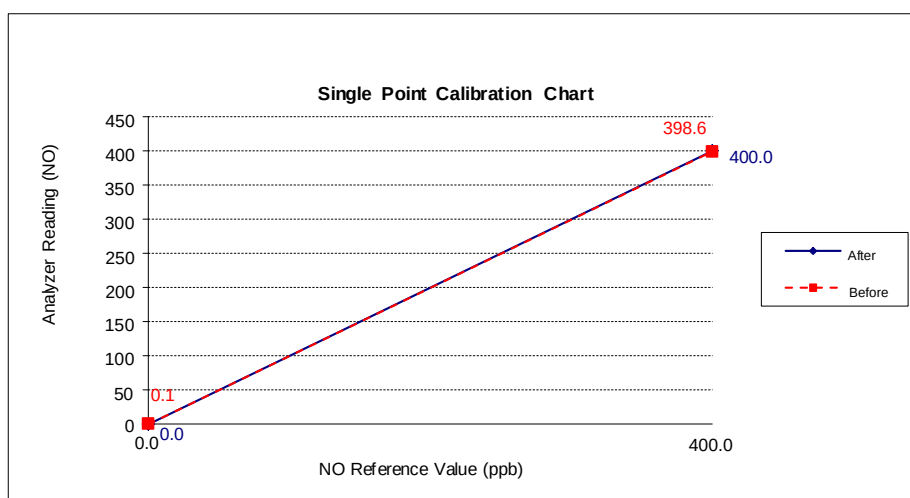

Calibrate By :

Supervisor :

Mr.Chatchai Hermkhunthod

Mr.thammarat Khamsiang



บริษัท ซี.ที. เอ็นไวรอนเม้นท์ แอนด์ เคมีคัล จำกัด

C.T. ENVIRONMENT AND CHEMICAL CO., LTD. E-mail: cte_envi@yahoo.com.

9/40-41 ม.2 ต.บางคูเวียง อ.บางกรวย จ.นนทบุรี 11130 โทรศัพท์: 02-101-3409 โทรสาร: 02-101-3410

9/40-41 Moo. 2 T.Bangkooveang A.Bangkrui Nonthaburi 11130 TEL: 02-101-3409 FAX: 02-101-3410

Analyzer Performance Test

Calibrated Date: 30 April 2024

Instruments Information

Analyzer Type: CO Analyzer Model: 48C	Manufacturer Thermo Environmental S/N: 48C-53842-297
--	---

Calibration System


Calibrator Unit	Standard Gas
Dilutor Model API Model 700 S/N: 556 ZERO AIR Generator API MODEL 701 S/N: 233	NO Conc 45.4 PPM SO2 Conc 44.9 PPM CO Conc 4,480 PPM Expire Date: 30 April 2025

Environment: Temperature 25.5 °C

Humidity: 51 %RH

Calibration Report

Status	Zero			Span		
	Reference (PPM)	Reading (PPM)	Drift (PPM)	Reference (PPM)	Reading (PPM)	Drift%
Before	0.0	0.1	0.1	45.0	44.9	-0.2
After	0.0	0.0	0.0	45.0	45.0	0.0

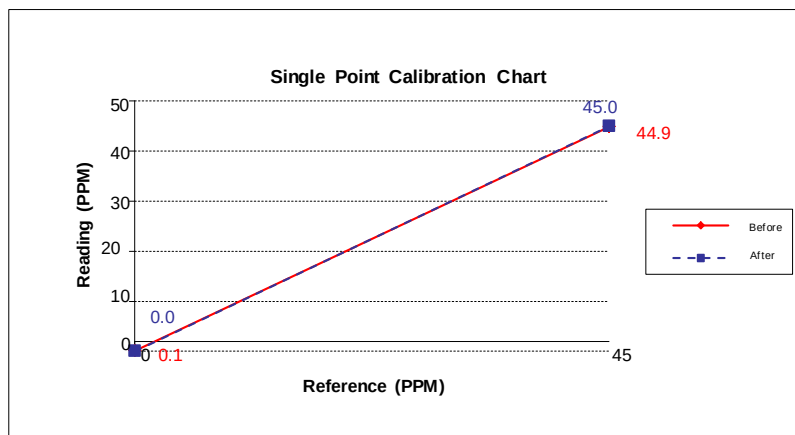

Calibrate By :

Mr.Chatchai Hermkhunthod

Supervisor :

Mr.thammarat Khamsiang


PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	March 13, 2024
Project Site				Start Time	2:30 PM
Sampler Number	PM-10 No.6	Transfer Standard Type	Orifice	Stop Time	2:40 PM
Motor Serial Number	PM-10 No.6	Calibrator Model	TE-5025A	Person	Mr.Thammarat Khamsiang
Recorder Serial Number	PM-10 No.6	Calibrator Serial Number	801		

Plate	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric	Start	Stop
No.	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	Qstd = (1/m)[(A-b)] (m ³ /min)	Sample Flow Rate Indication (ft ³ /min)	IC = I[(Pa/P _{std})(T _{std} /Ta)] ^{1/2}	(°K = °C+273)	Pressure (mmHg)	Meter	Meter
	Positive	Negative	ΔH ₂ O								
5	0.30	0.36	0.7	0.80329	0.40546	36.0	35.60	304.0	758.0		
7	0.47	0.54	1.0	0.99371	0.49552	38.0	37.57	304.0	758.0		
10	0.68	0.74	1.4	1.17827	0.58281	39.0	38.56	304.0	758.0		
13	0.83	0.89	1.7	1.29677	0.63886	40.0	39.55	304.0	758.0		
18	0.99	1.10	2.1	1.42946	0.70161	42.0	41.53	304.0	758.0		
Linear Regression Y ON X : Y= mX + b							Average	304.0	758.0		
1	Slope (m)			2.11434	Linear Equation			r ²	0.993341	Pstd(mmHg)	760.0
2	Intercept (b)			-0.05399	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.99666494	T _{NTP}	298.0
3	Correlation Coefficient (r)			0.99975	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)		0.977683518	
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5		0.988778801	

COMMENT

Andersen Instruments, Inc.											
----------------------------	--	--	--	--	--	--	--	--	--	--	--

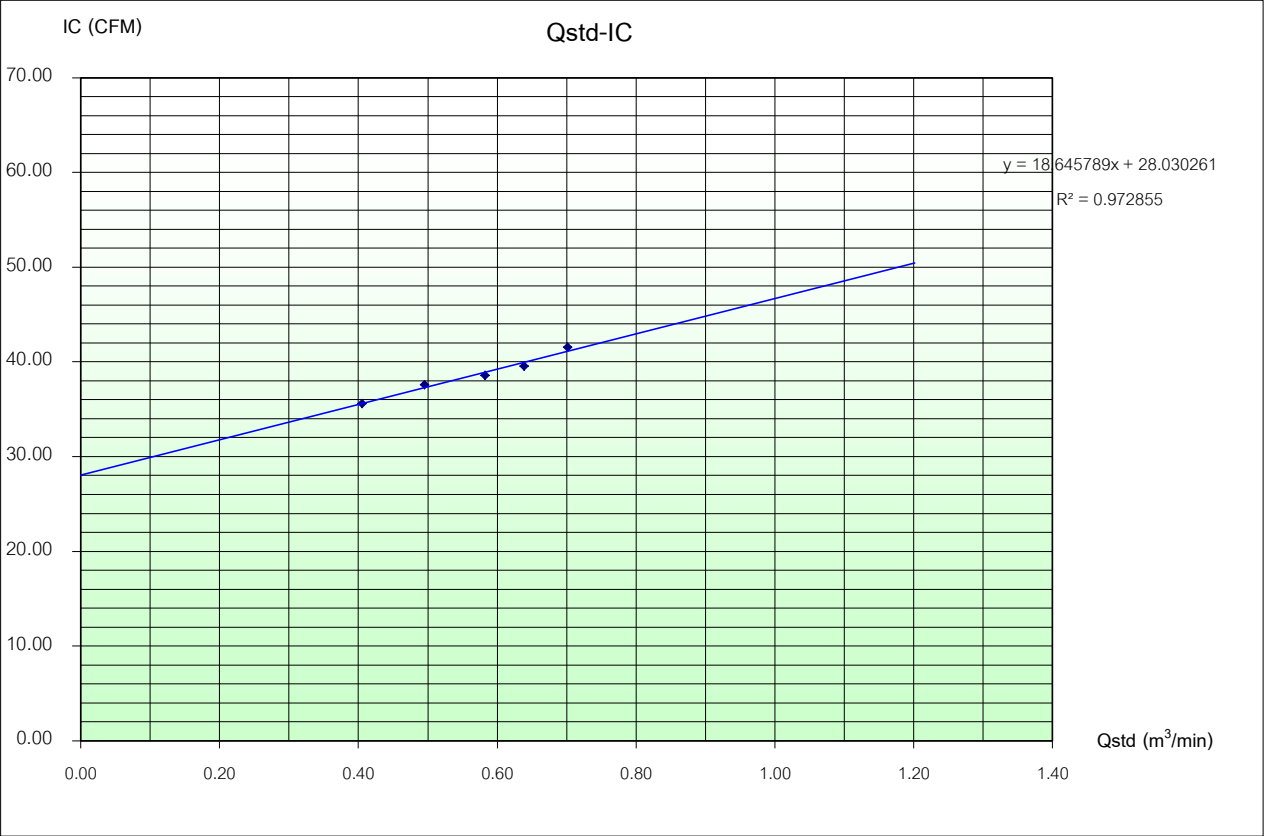

Calibrated By
Mr.C
Technician

Approved By
Mr.thammarat Khamsiang
Environmental Scientist


TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Sampler Location				Date	March 14, 2024
Project Site				Start Time	3:20 PM
Sampler Number	TSP No.6	Transfer Standard Type	Orifice	Stop Time	3:30 PM
Motor Serial Number	TSP No.6	Calibrator Model	TE-5025A	Person	Mr.Thammarat Khamsiang
Recorder Serial Number	TSP No.6	Calibrator Serial Number	801		


Plate	(Delta H)			(A)	(X)	(I)	(Y)	Temperature	Barometric	Start	Stop
No.	Pressure Drop Across Orifice (inH ₂ O)			$[\Delta H_2O(Pa/P_{std})(T_{std}/Ta)]^{1/2}$	Qstd = (1/m)[(A-b)] (m ³ /min)	Sample Flow Rate Indication (ft ³ /min)	IC = I[(Pa/P _{std})(T _{std} /Ta)] ^{1/2}	("K = °C+273)	Pressure (mmHg)	Meter	Meter
	Positive	Negative	ΔH ₂ O								
5	2.4	2.9	5.3	2.27260	1.12268	51.0	50.34	305.0	758.0		
7	4.0	4.5	8.5	2.87803	1.41656	54.0	53.31	305.0	758.0		
10	6.3	6.9	13.2	3.58652	1.76047	60.0	59.23	305.0	758.0		
13	8.4	8.7	17.1	4.08210	2.00103	62.0	61.20	305.0	758.0		
18	10.4	10.8	21.2	4.54521	2.22583	66.0	65.15	305.0	758.0		
Linear Regression Y ON X : Y= mX + b							Average	305.0	758.0		
1	Slope (m)			2.06011	Linear Equation			r ²		0.994144	Pstd(mmHg)
2	Intercept (b)			-0.04024	Set Point Flow Rate (X) (m ³ /min)		1.133	r	0.9970677	T _{NTP}	298.0
3	Correlation Coefficient (r)			0.99998	Final Set Flow Rate = (I)		0	(Pa/Pstd)*(Tstd/Ta)			0.974477998
Result								C=(Pa/Pstd)*(Tstd/Ta)^0.5			0.987156522

COMMENT

Andersen Instruments, Inc.											
----------------------------	--	--	--	--	--	--	--	--	--	--	--

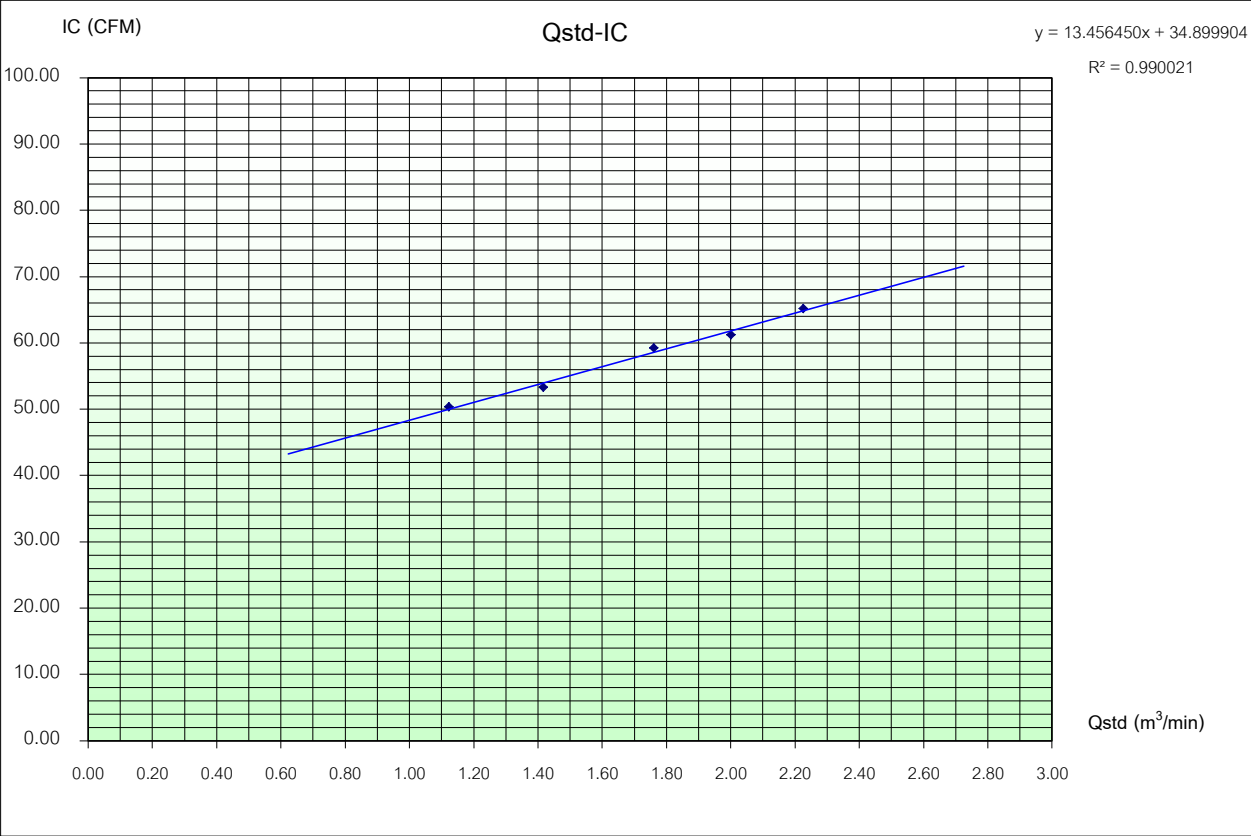

Calibrated By



Technician

Approved By



Mr.Thammarat Khamsiang
Environmental Scientist

Certificate of Calibration

Certificate No. : 66-300471-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.

47/91-93,96 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Piston Pipette

Manufacturer : sartorius

Model : N/A

Serial No. : 4541601431

ID No. : LB-Eg-045

Capacity : 100 μ l to 1000 μ l Resolution : 5 μ l

Environment : Ambient Temperature : (20 $\pm$ 3) $^{\circ}$ C

Relative Humidity : (55 $\pm$ 10) %

Air Pressure : (1007.6 to 1007.7) mbar.

Date of Received : 03 August 2023

Date of Calibration : 07 August 2023

Date of Issue : 07 August 2023

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3002 base on ISO 8655-6 : 2002-09

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	66-200196-4	02 Dec 2023	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-300471-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Test Volume (μl)	Measuring Volume at 20 ^o C (μl)	Systematic error (e_s %)	Coeff. of Variation (CV%)	Uncertainty ($\pm \mu\text{l}$)
100	97.92	0.21	0.15	0.69
500	496.58	0.34	0.04	0.69
1000	997.55	0.24	0.01	0.69

e_s : Systematic error (%)

CV : Coefficient of variation (%)

UUC Calibrated by : Blue Tip

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-300222-6

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.

47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Burette

Manufacturer : Witeg

Class : A

Capacity : 25 ml

Graduation : 0.05 ml

ID No. : LB-Gw-001

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1002.7 mbar.

Date of Received : 20 April 2024

Date of Calibration : 27 April 2024

Date of Issue : 27 April 2024

Calibrated by : Wipa Tovadee

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241003	66-200388-2	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-300222-6

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 40.01 sec.

Nominal Volume (ml)	Measuring Volume (ml)
10	10.0029
20	20.0018
25	25.0167

Uncertainty of measurement with in $\pm$ 0.0066 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Cert.No.: 24TW29

Page.: 1 of 2

Certificate of Testing

Equipment :	DO Meter
Manufacturer :	Hanna
Model :	HI98193
Serial No. :	03030056991
ID No. :	LB-Eq-014
Received Date :	05 February 2024
Test Date :	06 February 2024
Reference :	2402-0129WN-1
Submitted by :	Special Lab Envi And Consultant Co.,Ltd 47/91-93, 96 Moo 3 Tambon Tha-it, Pakkret, Nonthaburi 11120
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 Approved Signatory
(☒) Saithip Meangmai (☐) Warakorn Lerngagtrakul (☐) Ponpan Paipim	
Issue Date :	7 February 2024



Cert.No.: 24TW29

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	1124013382	140RC006	23MM18	20 Feb 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: KC1N20CDJ

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.18	0.0084

This report was certified only for the instrument we tested. It is allowable to use for study
Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced
other in full, without written approval of the laboratory

-o0o-

a 1201024

Certificate of Calibration

Certificate No. : 67-200136-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Electronic Balance
Manufacturer : AND Model : GR-200
Serial No. : 14245322 ID No. : LB-Eq-016
Capacity : 210 g Resolution : 0.0001 g

Environment : On site calibration was carried out at the Laboratory,
Special Lab Envi and Consultant Co., Ltd.
Ambient Temperature : (27.3 to 27.7) °C
Relative Humidity : (42.5 to 44.0) %
Air Pressure : 1006.0 mbar

Date of Received : 20 April 2024

Date of Calibration : 20 April 2024

Date of Issue : 24 April 2024

Calibrated by : Akaradath Thippichai

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-200136-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value

Nominal Value (g)	Correction (g)	Uncertainty $\pm$ (g)
0.001	0.0000	0.00012
0.01	0.0000	0.00012
0.1	0.0000	0.00012
0.5	0.0000	0.00013
2	0.0000	0.00013
5	-0.0001	0.00013
10	0.0000	0.00013
50	0.0000	0.00015
100	0.0000	0.00020
200	0.0001	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.


This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.06$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g

A B C D E

-0.0003 0.0000 0.0006 -0.0001 0.0000 g




Repeatability

Load test : 200 g

Stdev. : 0.00005 g

- o0o -



Certificate of Calibration

Certificate No. : 67-400217-2

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91 Moo 3 Thambol Tha-it, Pakkret, Nonthaburi 11120

Equipment : Temperature controlled enclosure(Incubator)
Manufacturer : Lovibond Model : FKU 1800
Range : N/A °C Resolution : 0.1 °C
Serial No. : 0914643-01 ID No. : LB-Eq-004

Environment : On site calibration was carried out at the Laboratory, Special Lab Envi and Consultant Co., Ltd.
Ambient Temperature : (26.0 to 27.0) °C
Relative Humidity : (45 to 50) %
Line Voltage : (226.0 to 226.5) V

Date of Received : 20 April 2024

Date of Calibration : 20 April 2024

Date of Issue : 26 April 2024

Calibrated by : Kittisak Kokaco


Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400042	67-400047-1	25 Jul 2024	National Institute of Metrology Thailand (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400217-2


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

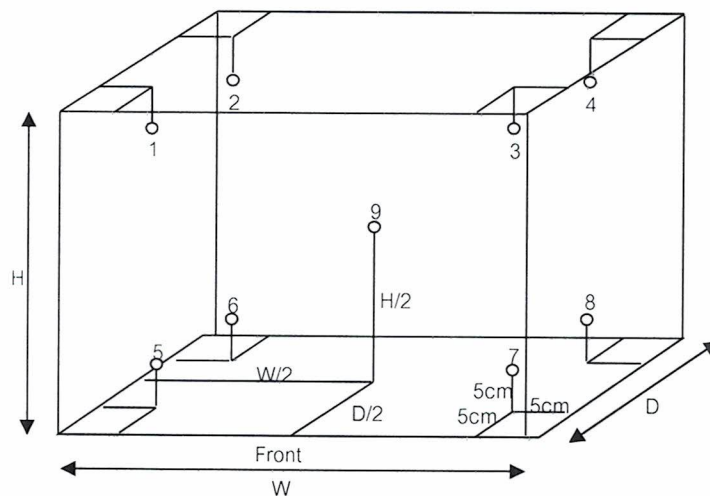

Inside of Chamber

W = 0.55 m

D = 0.73 m

H = 0.50 m

Capacity = 0.20 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
20.0	19.9	19.9	20.27	20.24	20.07	20.06	20.15	20.14	20.21	20.03	20.12	0.44

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
20.0	19.9	19.9	0.24	0.20	0.54

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-400217-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91 Moo 3 Thambol Tha-it, Pakkret, Nonthaburi 11120

Equipment : Temperature controlled enclosure(Incubator)
 Manufacturer : Lovibond Model : FKU 1800
 Range : N/A °C Resolution : 0.1 °C
 Serial No. : 0925481-19 ID No. : LB-Eq-005

Environment : On site calibration was carried out at the Laboratory, Special Lab Envi and Consultant Co., Ltd.
 Ambient Temperature : (24.0 to 25.0) °C
 Relative Humidity : (50 to 55) %
 Line Voltage : (226.0 to 226.5) V

Date of Received : 20 April 2024

Date of Calibration : 20 April 2024

Date of Issue : 26 April 2024

Calibrated by : Kittisak Kokaco

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
 Standard Digital Thermometer with RTD Probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400047	67-400047-2	26 Jul 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400217-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

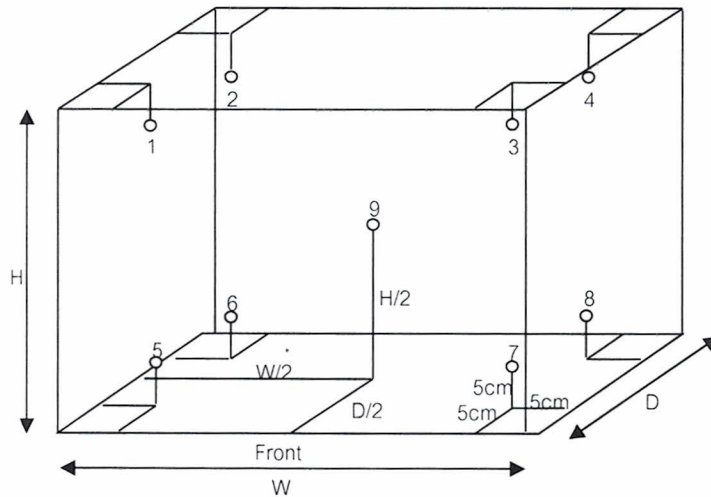

Inside of Chamber

W = 0.55 m

D = 0.73 m

H = 0.50 m

Capacity = 0.20 m³

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.									Uncertainty (± ° C)
			1	2	3	4	5	6	7	8	9	
30.0	30.0	30.0	30.09	30.21	30.18	30.17	30.52	30.49	30.13	30.32	30.13	0.31
35.0	35.0	35.0	34.95	35.17	35.13	35.14	35.62	35.67	35.04	35.40	35.19	0.32
37.0	37.0	37.0	36.94	37.16	37.13	37.11	37.60	37.64	37.02	37.37	37.16	0.33


Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Uniformity (° C)	Measured Stability (° C)	Overall Variation (° C)
30.0	30.0	30.0	0.42	0.03	0.46
35.0	35.0	35.0	0.50	0.04	0.77
37.0	37.0	37.0	0.51	0.06	0.79

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)

CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH951

Page.: 1 of 2

Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Eutech
Model :	pH 700
Serial No. :	2858459
ID No. :	LB-Eq-027
Condition As-Received:	Used Item
Received Date :	04 August 2023
Calibration Date :	07 August 2023
Reference :	2308-0115WN-1
Submitted by :	Special Lab Envi And Consultant Co.,Ltd 47/91-93, 96 Moo 3 Thambon Tha-it, Pakkret Nonthaburi 11120
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM)
Calibrated by :	Warakorn Lerngagtrakul
Approved by :	 Approved Signatory
☒ Saithip Meangmai ☐ Warakorn Lerngagtrakul ☐ Ponpan Paipim	
Issue Date :	16 August 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0057105



Cert. No.: 23CH951

Page.: 2 of 2

Condition of this calibration result

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	22E2769	24 Aug 2023

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	863832	28 Dec 2024
pH 6.986	CPA chem	863833	28 Dec 2023
pH 10.010	CPA chem	863835	28 Dec 2023

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Fluke at pH (4,7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: 2858459	4.00	177.48	177.5	4.01	0.058	2.00
	7.00	0.00	0.1	7.00	0.058	2.00
	10.00	-177.48	-177.4	10.01	0.058	2.00

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH measurement (±)	Coverage factor <i>k</i>
pH Electrode S/N.: 3101624	4.008	4.01	170.7	0.0085	2.05
	6.986	6.99	-2.0	0.011	2.00
	10.010	10.01	-178.2	0.0096	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

a 1174396



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23LM132

Page.: 1 of 2

Certificate of Calibration

Equipment : pH Meter with Sensor

Manufacturer : Eutech

Model : pH 700

Serial No. : 2858459

ID No. : LB-Eq-027

Submitted by : Special Lab Envi And Consultant Co.,Ltd.
47/91-93 Moo 3 Thambon Tha-it,
Pakkret,
Nonthaburi 11120

Location : TPA On Site Calibration Laboratory

Received Order : 04 August 2023

Calibrated Date : 09 August 2023

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Preecha Hlahib

Approved by :

Approved Signatory

() Pornthippa Tameyakul
() Ponpan Paipim
(✓) Suwit Imjai

Issue Date : 17 August 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0057254



Equipment : pH Meter with Sensor

Cert. No.: 23LM132

Condition As-Received : New Item

Page.: 2 of 2

Reference : 2308-0115WN-2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	2211285	TPA	21 Oct 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: PH5TEMB01P

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
25.0	100	25.002	25.0	-0.002	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Certificate of Calibration

Certificate No. : 67-400217-4

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93 Moo 3, Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Temperature controlled enclosure (Refrigerator)
Manufacturer : Frozen Model : CC-2288F
Range : N/A °C Resolution : 1 °C
Serial No. : CC-2288F-1163-003 ID No. : LB-Eq-046

Environment : On site calibration was carried out at the Laboratory, Special Lab Envi and Consultant Co., Ltd.
Ambient Temperature : (32.0 to 33.0) °C
Relative Humidity : (40 to 45) %
Line Voltage : (226.0 to 226.5) V

Date of Received : 20 April 2024

Date of Calibration : 20 April 2024

Date of Issue : 26 April 2024

Calibrated by : Permpon Chanpu


Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400030	66-400595-1	26 Apr 2024	National Institute of Metrology Thailand (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400217-4


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

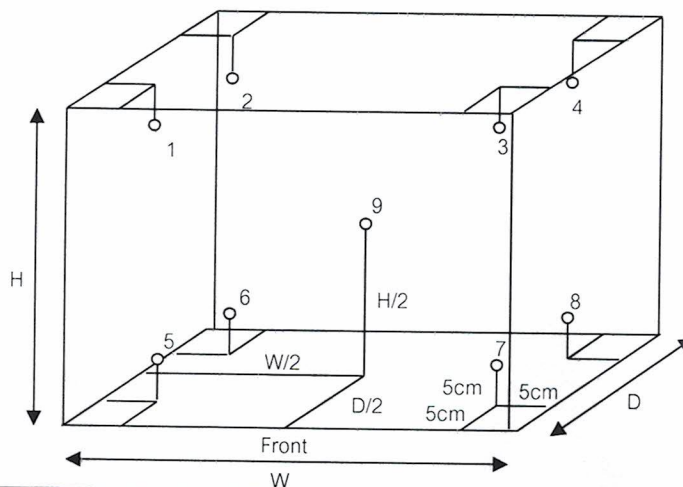

Inside of Chamber

W = 1.02 m

D = 0.47 m

H = 1.48 m

Capacity = 0.71 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
3	3	3	4.0	3.0	2.6	2.5	4.0	4.1	2.1	2.1	3.1	0.85

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
3	3	3	1.2	0.2	2.3

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -





BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

99/9 Moo 2, Maha Sawat, Phutthamonthon, Nakhon Pathom. 73170. Thailand. Tel: +66 3424 5299 Fax: +66 3424 5250
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-24-099

Page : 1 of 3

CERTIFICATE OF CALIBRATION

Equipment : Spectrophotometer
Manufacturer : Thermo Scientific
Model : Genesys 20
Serial No. : 3SGT041007
ID No. : LB-Eq-029
Customer : Special Lab Envi And Consultant Co.,Ltd.
: 47/91-93 Moo 3, Tambol Tait, Amphur Pakrad,
: Nonthaburi, 11120
Location : Becthai Laboratory
Date of Receipt : 30 April 2024
Date of Calibration : 2 May 2024
Date of Issue : 2 May 2024
Ambient Temperature : (25±10) °C
Relative Humidity : (60±20) %
Condition As-Received : Used Item

Calibrated by

Ms. Bussayamas Noppakhun

Calibration Engineer

Approved by

.....

(Ms. Jintana Sangthaijaroenlap)

Calibration Manager

The reported expended uncertainty of measurement was based on a combined standard uncertainty multiplied by a coverage factor k providing a level of confidence of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

Indicated values are valid for the state of the Spectrophotometer at the time of calibration only.



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

99/9 Moo 2, Maha Sawat, Phutthamonthon, Nakhon Pathom. 73170. Thailand. Tel: +66 3424 5299 Fax: +66 3424 5250
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-24-099

Page : 2 of 3

CALIBRATION REPORT

Conditions of this result of calibration

1. Reference Standard Material :

<u>Material</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert.No.</u>	<u>Due date</u>
Holmium Glass Filter	RM-HG	12705	117342	13 December 2025
Neutral Density Filter	RM-1N2N3N	8323	117341	13 December 2025

2. Traceability : This certification is traceable to the International System of Unit maintained at;
The Starna Scientific Ltd. Accredited Calibration Laboratory No. 0659.

3. Method of calibration :

The calibration procedure was carried out according to ASTM E275-08 (2022) and ASTM E925-09 (2014).

4. Result of calibration :

(☒) without adjustment (☐) after adjustment

5. Equipment Specifications:

Spectral Bandwidth :	8	nm
Data Interval :	1	nm
Scan Speed :	N/A	nm/min



BECTHAI BANGKOK EQUIPMENT & CHEMICAL CO., LTD.
CALIBRATION LABORATORY

99/9 Moo 2, Maha Sawat, Phutthamonthon, Nakhon Pathom. 73170. Thailand. Tel: +66 3424 5299 Fax: +66 3424 5250
E-mail: bkk@becthai.com Website: www.becthai.com



Certificate No. : CAL-24-099

Page : 3 of 3

CALIBRATION REPORT

Wavelength Calibration

Certified Values of Reference Material	Nominal Value (nm)	UUC*Reading (nm)	Error (nm)	Uncertainty of Measurement ($\pm$ nm)	k Factor
418.40	418	418	-0.40	0.59	2.00
537.00	537	537	0.00	0.59	2.00
638.00	638	639	1.00	0.59	2.00

Photometric Calibration for Visible

Wavelength (nm)	Certified Values of Reference Material (A)	UUC* Reading (A)	Error (A)	Uncertainty of Measurement ($\pm$ A)	k Factor
420.0	Zero	0.000	0.0000	0.0028	2.00
	0.5703	0.573	0.0027	0.0045	2.00
	0.7336	0.734	0.0004	0.0045	2.00
	1.0709	1.075	0.0041	0.0045	2.00
440.0	Zero	0.000	0.0000	0.0028	2.00
	0.5592	0.557	-0.0022	0.0045	2.00
	0.716	0.717	0.0010	0.0045	2.00
	1.0454	1.044	-0.0014	0.0045	2.00
465.0	Zero	0.000	0.0000	0.0028	2.00
	0.5094	0.511	0.0016	0.0045	2.00
	0.6601	0.664	0.0039	0.0045	2.00
	0.963	0.966	0.0030	0.0045	2.00
546.1 (546.0)	Zero	0.000	0.0000	0.0028	2.00
	0.5206	0.523	0.0024	0.0045	2.00
	0.6677	0.665	-0.0027	0.0045	2.00
	0.9763	0.979	0.0027	0.0045	2.00
590.0	Zero	0.000	0.0000	0.0028	2.00
	0.5522	0.555	0.0028	0.0045	2.00
	0.6966	0.699	0.0024	0.0045	2.00
	1.0201	1.022	0.0019	0.0045	2.00
635.0	Zero	0.000	0.0000	0.0028	2.00
	0.5377	0.538	0.0003	0.0045	2.00
	0.6649	0.667	0.0021	0.0045	2.00
	0.9736	0.977	0.0034	0.0045	2.00

Remark : Each individual filter is measured against the empty filter holder (blank) used to zero the Spectrophotometer.

Note:

UUC* : Unit Under Calibration

- End of Report -

Certificate of Calibration

Certificate No. : 66-410081-1

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91-93,96 Moo 3,Tambol Tha-It, Pakkret, Nonthaburi 11120

Equipment : Digital Thermo-Hygrometer

Manufacturer :	Testo	Model :	608-H1
Range Temperature :	0 °C to 50 °C	Resolution :	0.1 °C
Range Humidity :	10 %R.H. to 95 %R.H.	Resolution :	0.1 %R.H.
Serial No. :	2083236817	ID No. :	LB-Eg-042

Environment : Ambient Temperature : $(23 \pm 2) ^\circ\text{C}$
Relative Humidity : $(50 \pm 15) \%$

Date of Received : 03 August 2023

Date of Calibration : 09 August 2023

Date of Issue : 09 August 2023

Calibrated by : Chortip Samchusri


Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4013 by compared with standard probe sensor humidity/temperature into humidity/temperature chamber.

Reference Standard Instruments : This certification is traceable to the International System of Units

Digital Indicator with Standard Probe Temp&Hum

ID No.	Cert. No.	Due Date	Traceability
400034 & 400035	SG-H-00502/66	06 Jan 2024	Success Gateway Co., Ltd., Accredited by TISI Calibration No.0268

Approved by :



Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



www.calibratech.co.th

Certificate of Calibration

Certificate No. : 66-410081-1

Page : 2 of 2

UUC Condition As-Received : Good

Result of Calibration : Without Adjustment

Function : Temperature measurement

Reference Humidity @ 50 %R.H.

Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25.01	25.0	0.0	0.46

Result of Calibration : Without Adjustment

Function : Humidity measurement

Reference Temperature @ 25 °C

Standard Humidity (%R.H.)	UUC Reading (%R.H.)	Correction (%R.H.)	Uncertainty (± %R.H.)
49.97	57.0	-7.0	2.2


Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 67-400217-3

Page : 1 of 2

Submitted by : Special Lab Envi and Consultant Co., Ltd.
47/91 Moo 3 Thambol Tha-it, Pakkret, Nonthaburi 11120

Equipment : Water Bath
Manufacturer : Memmert Model : WNB22
Range : N/A °C Resolution : 0.1 °C
Serial No. : L520.0201 ID No. : LB-Eq-041

Environment : On site calibration was carried out at the Laboratory, Special Lab Envi and Consultant Co., Ltd.
Ambient Temperature : (34.0 to 35.0) °C
Relative Humidity : (35 to 40) %
Line Voltage : (226.0 to 226.5) V

Date of Received : 20 April 2024

Date of Calibration : 20 April 2024

Date of Issue : 26 April 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

ID No.	Cert. No.	Due Date	Traceability
400029 & 400031	66-400592-1	24 Apr 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration


Certificate No. : 67-400217-3

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

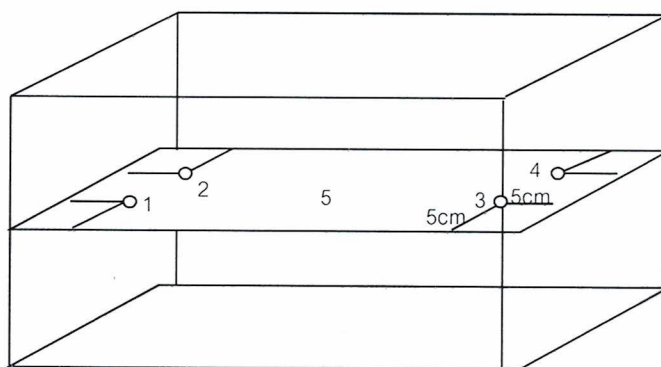

Front

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor					Uncertainty (± ° C)	Measured Uniformity (° C)	Measured Stability (° C)
			No.							
			1	2	3	4	5			
62.0	62.0	62.0	62.04	62.05	62.03	62.05	62.02	0.18	0.09	0.04
85.0	85.0	85.0	85.05	85.05	85.04	85.06	85.02	0.18	0.09	0.05
95.0	95.0	95.0	94.92	94.82	94.81	94.78	94.80	0.21	0.21	0.10
100.0	CCC	100.6	100.44	100.47	100.55	100.50	100.36	0.21	0.28	0.09

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Certificate of Calibration

Certificate No. : 66-210415-1

Page : 1 of 2

Submitted by : Special Lab Envi And Consultant Co, Ltd.
47/91-93,96 Moo 3, Tambol Tha - It, Pakkret, Nonthaburi 11120

Equipment : Weight
Manufacturer : LS Material : Stainless Steel
Weight size : 1 g
ID No. : LB-Eq-034
Assumed density of weight : 7950 kg / m³
Assumed Air density : 1.2 kg / m³

Environment : Ambient Temperature : (20 ± 2) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1005.9 mbar

Date of Received : 03 August 2023

Date of Calibration : 16 August 2023

Date of Issue : 16 August 2023

Calibrated by : Wuttichai Swatphong

Calibration Method : In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E221-E2210	MM-0042-22	21 Mar 2025	National Institute of Metrology (Thailand), (NIMT)

Approved by :

(Sarachan Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-210415-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good


No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	1 g	none	1 g	-0.017 mg	± 0.023 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -

CAL



Certificate of Calibration

Certificate No. : 66-210415-2

Page : 1 of 2

Submitted by : Special Lab Envi And Consultant Co, Ltd.
47/91-93,96 Moo 3, Tambol Tha - It, Pakkret, Nonthaburi 11120

Equipment : Weight
Manufacturer : LS Material : Stainless Steel
Weight size : 100 g
ID No. : LB-Eq-035
Assumed density of weight : 7950 kg / m³
Assumed Air density : 1.2 kg / m³

Environment : Ambient Temperature : (20 ± 2) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1005.9 mbar

Date of Received : 03 August 2023

Date of Calibration : 16 August 2023

Date of Issue : 16 August 2023

Calibrated by : Wuttichai Swatphong


Calibration Method : In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E221-E2210	MM-0042-22	21 Mar 2025	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Surachai Promthong)
Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-210415-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	100 g	none	100 g	-0.20 mg	$\pm$ 0.11 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

CAL



Certificate of Calibration

Certificate No. : 66-210415-3

Page : 1 of 2

Submitted by : Special Lab Envi And Consultant Co, Ltd.
47/91-93,96 Moo 3, Tambol Tha - It, Pakkret, Nonthaburi 11120

Equipment : Weight

Manufacturer : LS

Material : Stainless Steel

Weight size : 200 g

ID No. : LB-Eq-036

Assumed density of weight : 7950 kg / m³

Assumed Air density : 1.2 kg / m³

Environment : Ambient Temperature : (20 ± 2) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1005.9 mbar

Date of Received : 03 August 2023

Date of Calibration : 16 August 2023

Date of Issue : 16 August 2023

Calibrated by : Wuttichai Swatphong


Calibration Method : In-house method CAL-M2101 based on OIML R 111-1 : 2004(E)

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

ID No.	Cert. No.	Due Date	Traceability
E221-E2210	MM-0042-22	21 Mar 2025	National Institute of Metrology (Thailand), (NIMT)

Approved by :



(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-210415-3

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good


No.	Nominal Value	Id.Mark	Conventional mass Value		Measuring Uncertainty
1	200 g	none	200 g	+0.11 mg	$\pm$ 0.17 mg

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

CAL



www.calibratech.co.th