

CERTIFICATE OF CALIBRATION

Certificate No. : 66S1031-25 Job No. : 66S1031 Page : 1 of 2

Customer : C.E.M. Technology (Thailand) Co., Ltd.

Address : 31/8 Moo 13, Raikhing, Samphran,

Nakhornpathom 73210

Location : Laboratory

Equipment : Sound Level Meter

Ambient temperature : $(20 \pm 2) ^\circ\text{C}$

Manufacturer : ACO

Relative humidity : $(50 \pm 15) \%$

Model : 6236

Atmospheric pressure : -

Serial No. : 222128

Date of received : 26-Oct-2023

Identity No. : NS-03-013

Date of calibration : 30-Oct-2023

Range : See to Data

Date of issued : 01-Nov-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.40/0666	21-Jun-2025

Traceability : This certification is traceable to the International System of Unit maintained at :

- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn

Approved By :

Ms. Bhacharin Phanangkaew (MD)

Reviewed By : Mr. Sompong Srisert

Mr. Boonyarit Auejirakarn

Ms. Natthaprakarn Thammaphan

The reported expanded uncertainty is based on uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95%. This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Continuation of Calibration Report

Certificate No. : 66S1031-25 Job No. : 66S1031

Page : 2 of 2

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.0	0.0	0.20
	104	104.0	0.0	0.20
	114	114.0	0.0	0.20
C	94	94.0	0.0	0.20
	104	104.0	0.0	0.20
	114	114.0	0.0	0.20
Z	94	93.9	-0.1	0.20
	104	103.9	-0.1	0.20
	114	113.9	-0.1	0.20

UUC* = Unit Under Calibration

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S1031-24 Job No. : 66S1031 Page : 1 of 2

Customer : C.E.M. Technology (Thailand) Co., Ltd.

Address : 31/8 Moo 13, Raikhing, Samphran,

Nakhornpathom 73210

Location : Laboratory

Equipment : Sound Level Meter

Ambient temperature : $(20 \pm 2) ^\circ\text{C}$

Manufacturer : ACO

Relative humidity : $(50 \pm 15) \%$

Model : 6236

Atmospheric pressure : -

Serial No. : 222129

Date of received : 26-Oct-2023

Identity No. : NS-03-014

Date of calibration : 30-Oct-2023

Range : See to Data

Date of issued : 01-Nov-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.40/06666	21-Jun-2025

Traceability : This certification is traceable to the International System of Unit maintained at :

- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn

Approved By :

Ms. Bhacharin Phanangkaew (MD)

Reviewed By : Mr. Sompong Srisert

Mr. Boonyarit Auejirakarn

Ms. Natthaparakarn Thammaphan

The reported expanded uncertainty is based on uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95%. This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

06Jun-2019

FM-FCS-040

Continuation of Calibration Report

Certificate No. : 66S1031-24 Job No. : 66S1031

Page : 2 of 2

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.1	0.1	0.20
	104	104.2	0.2	0.20
	114	114.2	0.2	0.20
C	94	94.1	0.1	0.20
	104	104.1	0.1	0.20
	114	114.1	0.1	0.20
Z	94	94.1	0.1	0.20
	104	104.1	0.1	0.20
	114	114.1	0.1	0.20

UUC* = Unit Under Calibration

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S1229-11 Job No. : 66S1229 Page : 1 of 2

Customer : C.E.M. Technology (Thailand) Co.,Ltd.
Address : 31/8 Moo 13, Raikhing, Samphran,
Nakhornpathom 73210
Location : Laboratory

Equipment : Sound Level Meter **Ambient temperature** : $(20 \pm 2) ^\circ\text{C}$
Manufacturer : ACO **Relative humidity** : $(50 \pm 15) \%$
Model : 6236 **Atmospheric pressure** : -
Serial No. : 222185 **Date of received** : 12-Dec-2023
Identity No. : NS-03-015 **Date of calibration** : 15-Dec-2023
Range : See to Data **Date of issued** : 18-Dec-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.40/0666	21-Jun-2025

Traceability : This certification is traceable to the International System of Unit maintained at :
- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn

Approved By :

Ms. Bhacharin Phanangkaew (MD)

Reviewed By : Mr. Sompong Srisert

Ms. Natthaprakarn Thammaphan

The reported expanded uncertainty is based uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95%. This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Rev.06/Jun-2019

FM-FCS-040

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.5	0.5	0.20
	104	104.5	0.5	0.20
	114	114.5	0.5	0.20
C	94	94.5	0.5	0.20
	104	104.4	0.4	0.20
	114	114.4	0.4	0.20
Z	94	94.5	0.5	0.20
	104	104.4	0.4	0.20
	114	114.4	0.4	0.20

UUC = Unit Under Calibration*

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S0420-22 Job No. : 66S0420 Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.

Address : 31/8 Moo 13, Raikhang, Samphran,
Nakhornpathom 73210

Location : Laboratory

Equipment : Sound Level Meter

Manufacturer : ACO

Model : 6236

Serial No. : 222188

Identity No. : NS-03-018

Range : See to Data

Ambient temperature : $(20 \pm 2) ^\circ\text{C}$

Relative humidity : $(50 \pm 15) \%$

Atmospheric pressure : -

Date of received : 30-Mar-2023

Date of calibration : 03-Apr-2023

Date of issued : 05-Apr-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at :-

- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn

Approved By :

[] Ms. Bhacharin Phanangkaew (MD)

Reviewed By : [] Mr. Sompong Srisert

[] Mr. Boonyarit Auejirakarn

[] Ms. Natthaparkarn Thammaphan

The reported expanded uncertainty is based uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95%.
This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Continuation of Calibration Report

Certificate No. : 66S0420-22 Job No. : 66S0420 Page : 2 of 2

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.0	0.0	0.20
	104	104.0	0.0	0.20
	114	113.9	-0.1	0.20
B	94	94.0	0.0	0.20
	104	103.9	-0.1	0.20
	114	113.8	-0.2	0.20
Z	94	94.0	0.0	0.20
	104	103.9	-0.1	0.20
	114	113.9	-0.1	0.20

UUC* = Unit Under Calibration

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S0205-5 Job No. : 66S0205 Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.

Address : 31/9 Moo 13, Raikhing, Samphan,

Nakhornpathom 73210

Location : Laboratory

Equipment : Sound Level Meter

Ambient temperature : (20 ± 2) °C

Manufacturer : ACO

Relative humidity : (50 ± 15) %

Model : 6236

Atmospheric pressure : -

Serial No. : 222189

Date of received : 03-Feb-2023

Identity No. : NS-03-019

Date of calibration : 07-Feb-2023

Range : See to Data

Date of issued : 09-Feb-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at :
- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn

Approved By :

Reviewed By : [] Mr. Sompong Srisert

[x] Ms. Natthaparakarn Thammaphan

[] Ms. Bhacharin Phanangkaew (MD)

[x] Mr. Boonyarit Auejirakarn

The reported expanded uncertainty is based uncertainty multiplied by a coverage factor k = 2, providing a level of confidence approximately 95%.
This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Continuation of Calibration Report

Certificate No. : 66S0205-5 Job No. : 66S0205 Page : 2 of 2

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.4	0.4	0.20
	104	104.1	0.1	0.20
	114	114.0	0.0	0.20
B	94	94.4	0.4	0.20
	104	104.1	0.1	0.20
	114	113.9	-0.1	0.20
Z	94	94.4	0.4	0.20
	104	104.1	0.1	0.20
	114	113.9	-0.1	0.20

UUC* = Unit Under Calibration

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S0330-4 Job No. : 66S0330 Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.
 Address : 31/9 Moo 13, Raikhing, Samphran,
 Nakhornpathom 73210
 Location : Laboratory

Equipment : Sound Level Meter Ambient temperature : $(20 \pm 2) ^\circ\text{C}$
 Manufacturer : ACO Relative humidity : $(50 \pm 15) \%$
 Model : 6236 Atmospheric pressure : -
 Serial No. : 222190 Date of received : 08-Mar-2023
 Identity No. : NS-03-020 Date of calibration : 10-Mar-2023
 Range : See to Data Date of issued : 13-Mar-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EELBP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at : -

- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn Approved By : [] Ms. Bhacharin Phanangkaew (MD)
 Reviewed By : [] Mr. Sompong Srisert [] Mr. Boonyarit Auejirakarn
 [] Ms. Natthaprakarn Thammaphan

The reported expanded uncertainty is based uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95%.
 This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.0	0.0	0.20
	104	104.1	0.1	0.20
	114	114.1	0.1	0.20
C	94	94.2	0.2	0.20
	104	104.1	0.1	0.20
	114	113.8	-0.2	0.20
Z	94	94.0	0.0	0.20
	104	104.0	0.0	0.20
	114	114.0	0.0	0.20

UUC* = Unit Under Calibration

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S0420-21 Job No. : 66S0420 Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.
Address : 31/8 Moo 13, Raikhing, Samphan,
Nakhornpathom 73210
Location : Laboratory

Equipment : Sound Level Meter
Manufacturer : ACO
Model : 6236
Serial No. : 222191
Identity No. : NS-03-021
Range : See to Data

Ambient temperature : $(20 \pm 2) ^\circ\text{C}$
Relative humidity : $(50 \pm 15) \%$
Atmospheric pressure : -
Date of received : 30-Mar-2023
Date of calibration : 03-Apr-2023
Date of issued : 05-Apr-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at :
- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn
Reviewed By : [] Mr. Sompong Srisert
[] Ms. Natthaprakarn Thammaphan
Approved By : [] Ms. Bhacharin Phanangkaew (MD)
[] Mr. Boonyarit Auejirakarn

The reported expanded uncertainty is based uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95%.
This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Result of Calibration : Without Adjustment
Function : Sound Level Measurement
Calibration Range : @ 1 kHz
Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.2	0.2	0.20
	104	104.2	0.2	0.20
	114	114.2	0.2	0.20
B	94	94.2	0.2	0.20
	104	104.2	0.2	0.20
	114	114.2	0.2	0.20
Z	94	94.2	0.2	0.20
	104	104.2	0.2	0.20
	114	114.2	0.2	0.20

UUC = Unit Under Calibration*

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S0420-24 Job No. : 66S0420 Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.
Address : 31/8 Moo 13, Raikhang, Samphran,
Nakhornpathom 73210
Location : Laboratory

Equipment : Sound Level Meter
Manufacturer : ACO
Model : 6236
Serial No. : 222193
Identity No. : NS-03-023
Range : See to Data
Ambient temperature : (20 ± 2) °C
Relative humidity : (50 ± 15) %
Atmospheric pressure : -
Date of received : 30-Mar-2023
Date of calibration : 03-Apr-2023
Date of issued : 05-Apr-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at : -
National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn
Reviewed By : [] Mr. Sompong Srisert
[] Ms. Natthaprakarn Thammanphan
Approved By : [] Ms. Bhacharin Phanangkaew (MD)
[] Mr. Boonyarit Auejirakarn

The reported expanded uncertainty is based uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95%.
This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Result of Calibration : Without Adjustment
Function : Sound Level Measurement
Calibration Range : @ 1 kHz
Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	93.8	-0.2	0.20
	104	103.8	-0.2	0.20
	114	113.8	-0.2	0.20
B	94	93.8	-0.2	0.20
	104	103.8	-0.2	0.20
	114	113.8	-0.2	0.20
Z	94	93.8	-0.2	0.20
	104	103.8	-0.2	0.20
	114	113.8	-0.2	0.20

UUC = Unit Under Calibration*

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S0330-1 Job No. : 66S0330 Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.
Address : 31/9 Moo 13, Raikhing, Samphran,
Nakhornpathom 73210
Location : Laboratory
Equipment : Sound Level Meter Ambient temperature : $(20 \pm 2) ^\circ\text{C}$
Manufacturer : ACO Relative humidity : $(50 \pm 15) \%$
Model : 6236 Atmospheric pressure : -
Serial No. : 222196 Date of received : 08-Mar-2023
Identity No. : NS-03-026 Date of calibration : 10-Mar-2023
Range : See to Data Date of issued : 13-Mar-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EELBP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at :-

- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn Approved By : [] Ms. Bhacharin Phanangkaew (MD)
Reviewed By : [] Mr. Sompong Srisert [x] Mr. Boonyarit Auejirakarn
[x] Ms. Natthaparakarn Thammaphan

The reported expanded uncertainty is based uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence approximately 95%.
This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Continuation of Calibration Report

Certificate No. : 66S0330-1 Job No. : 66S0330 Page : 2 of 2

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.1	0.1	0.20
	104	103.8	-0.2	0.20
	114	113.6	-0.4	0.20
C	94	94.0	0.0	0.20
	104	103.8	-0.2	0.20
	114	113.7	-0.3	0.20
Z	94	94.0	0.0	0.20
	104	103.8	-0.2	0.20
	114	113.6	-0.4	0.20

UUC* = Unit Under Calibration

- The End -



SMART TECH CALIBRATION & SERVICES CO., LTD.
14/508 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,
THANYABURI, PATHUM THANI 12110, THAILAND
Tel. +662-114-3148 Email : stc.th@gmail.com Website : stc-th.com



Certificate of Calibration

Certificate No. STCR-2307040-1
Work Order No. STCR-2307040
Page 1 of 3

Customer Name : CEM Technology Thailand Co., Ltd.
31/8 Moo.13 Raikhing Sub-district, Samphran District, Nakhonpathom, 73210

Equipment Name : Sound Level Meter
Manufacturer : pulsar
Model : 44
Serial Number : PN2308
Control Number : NS-08-002
Received Date : Jul 20, 2023
Calibration Date : Jul 21, 2023
Recommended Due Date : Jul 21, 2024
Calibration Method : Calibration Procedure No. CPE-04-01

Environmental Conditions
Ambient Temperature : $(25 \pm 2) ^\circ\text{C}$
Ambient Relative Humidity : $(50 \pm 15) \% \text{RH}$
Calibration Place : Permanent Calibration Laboratory

Condition as received : Normal
Calibration Result : See data attached

- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.
- The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
- The working standard is indicated in page 2 of this certificate.
- This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
- This results of this report only to the items calibrated.

Date of Issue : Jul 21, 2023
Calibrated by : S. Sompoch
Approved by :



Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2307040-1

Page 2 of 3

Standards Equipment Used

Equipment Name	Serial No.	Certificate No.	Due Date	Traceability to
Sound Calibrator	N975186	551220085447862	Nov 2, 2023	ANAB : AC-1969

Traceability

This calibration is traceable to the International System of Unit via :
- ANAB : The ANSI National Accreditation Bord.



Calibration Report

Smart Tech Calibration & Services Co.,Ltd.

Certificate No.: STCR-2307040-1

Page 3 of 3

UUC Range : (20 to 140) dB Resolution : 0.1 dB

Results of Calibration: [] Without adjustment [☒] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz

Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.07 dB 114.05 dB	93.3 dB 113.1 dB	94.0 dB 113.9 dB	0.07 dB 0.15 dB	0.40 dB 0.40 dB
SLOW	94.07 dB 114.05 dB	93.3 dB 113.2 dB	94.0 dB 113.9 dB	0.07 dB 0.15 dB	0.40 dB 0.40 dB

Sound Level Calibration @ Frequency 1 kHz

Select : C

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.07 dB 114.05 dB	93.4 dB 113.2 dB	94.0 dB 114.0 dB	0.07 dB 0.05 dB	0.40 dB 0.40 dB
SLOW	94.07 dB 114.05 dB	93.3 dB 113.2 dB	94.0 dB 113.9 dB	0.07 dB 0.15 dB	0.40 dB 0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -



SMART TECH CALIBRATION & SERVICES CO., LTD.
14/56 MOO 3, RANGSI-NAKHON NAYOK ROAD, LAM PHAK KUT,
THANYABURI, PATHUM THANI 12110, THAILAND
Tel. +662-114-3148 Email : stcal.mt@gmail.com



Certificate of Calibration

Certificate No. STCR-2302027-13
Work Order No. STCR-2302027

Page 1 of 3

Customer Name : CEM Technology Thailand Co., Ltd.
31/8 Village No.13 Rakkhing Sub-district, Samphran District, Nakhonpathom, 73210

Equipment Name : Sound Level Meter
Manufacturer : pulsar
Model : 44
Serial Number : PN2362
Control Number : NS-08-004
Received Date : Feb 18, 2023
Calibration Date : Feb 20, 2023
Recommended Due Date : Feb 20, 2024
Calibration Method : Calibration Procedure No. CPE-04-01

Environmental Conditions
Ambient Temperature : (25 ± 2) °C
Ambient Relative Humidity : (50 ± 15) %RH
Calibration Place : Permanent Calibration Laboratory

Condition as received : Normal
Calibration Result : See data attached

- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.
- The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
- The working standard is indicated in page 2 of this certificate.
- This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co.,Ltd.
- This results of this report only to the items calibrated.

Date of Issue : Feb 24, 2023
Calibrated by : M. Thippatai

Approved by :



(Mr. Sanyut Worapong)
Laboratory Manager

Calibration Report

Smart Tech Calibration & Services Co.,Ltd.

Certificate No.: STCR-2302027-13

Page 2 of 3

Standards Equipment Used

Equipment Name: Sound Calibrator Serial No.: N975186 Certificate No.: 551220085447862 Due Date: Nov 2, 2023 Traceability to: ANAB : AC-1969.20

Traceability

This calibration is traceable to the International System of Unit via :
- ANAB : The ANSI National Accreditation Bord.

Calibration Report

Smart Tech Calibration & Services Co.,Ltd.

Certificate No.: STCR-2302027-13

Page 3 of 3

UUC Range : (20 to 140) dB Resolution : 0.1 dB
Results of Calibration: [] Without adjustment [✓] With adjustment
Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.07 dB 114.05 dB	95.1 dB 115.0 dB	94.0 dB 114.0 dB	0.07 dB 0.05 dB	0.40 dB 0.40 dB
SLOW	94.07 dB 114.05 dB	95.2 dB 115.0 dB	94.0 dB 113.9 dB	0.07 dB 0.15 dB	0.40 dB 0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -





SMART TECH CALIBRATION & SERVICES CO., LTD.
14506 MOO 3, RANGSIT-NAKHON NAYOK ROAD, LAM PHAK KUT,
THANYABURI, PATHUM THANI 12110, THAILAND
Tel. +662-114-3148 Email : stcal.md@gmail.com Website : stc-cal.com



Certificate of Calibration

Certificate No. STCR-2311033-7
Work Order No. STCR-2311033
Page 1 of 3

Customer Name : CEM Technology Thailand Co., Ltd.
31/8 Moo.13 Raikhing Sub-district, Samphan District, Nakhonpathom, 73210

Equipment Name : Sound Level Meter
Manufacturer : Pulsar
Model : 44
Serial Number : PN2385
Control Number : NS-08-005
Received Date : Nov 15, 2023
Calibration Date : Nov 16, 2023
Recommended Due Date : Nov 16, 2024
Calibration Method : Calibration Procedure No. CPE-04-01

Environmental Conditions
Ambient Temperature : (25 ± 2) °C
Ambient Relative Humidity : (50 ± 15) %RH
Calibration Place : Permanent Calibration Laboratory

Condition as received : Normal
Calibration Result : See data attached

- The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.
- The Unit Under Calibration (UUC) has been calibrated by using the working standard which is traceable to SI-Units. The calibration procedure documented is intended to implement the requirements of ISO/IEC 17025 : 2017
- The working standard is indicated in page 2 of this certificate.
- This report applies to the item calibrated and shall not be reproduced except in full, without written approval by Calibration Laboratory, Smart Tech Calibration & Services Co., Ltd.
- This results of this report only to the items calibrated.



Date of Issue : Nov 17, 2023
Calibrated by : A. Sornchai

Approved by :



(Mr. Sornchai Sornchai)
Laboratory Manager

Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2311033-7

Page 2 of 3

Standards Equipment Used

Equipment Name	Serial No.	Certificate No.	Due Date	Traceability to
Sound Calibrator	N975196	5523631030478623	Nov 9, 2024	ANAB : AC-1969

Traceability

This calibration is traceable to the International System of Unit via :
- ANAB : The ANSI National Accreditation Bord.



Calibration Report

Smart Tech Calibration & Services Co., Ltd.

Certificate No.: STCR-2311033-7

Page 3 of 3

UUC Range : (20 to 140) dB Resolution : 0.1 dB

Results of Calibration: [] Without adjustment [✓] With adjustment

Appearance and Function of Use Inspection : GOOD

Sound Level Calibration @ Frequency 1 kHz

Select : A

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB 114.07 dB	91.4 dB 111.5 dB	93.9 dB 113.9 dB	0.19 dB 0.17 dB	0.40 dB 0.40 dB
SLOW	94.09 dB 114.07 dB	91.4 dB 111.5 dB	93.9 dB 113.8 dB	0.19 dB 0.27 dB	0.40 dB 0.40 dB

Sound Level Calibration @ Frequency 1 kHz

Select : C

Response times	STD. Value	UUC. Reading		Correction	(±) Uncertainty
		Before Adjustment	After Adjustment		
FAST	94.09 dB 114.07 dB	91.4 dB 111.5 dB	93.9 dB 113.8 dB	0.19 dB 0.27 dB	0.40 dB 0.40 dB
SLOW	94.09 dB 114.07 dB	91.4 dB 111.5 dB	93.9 dB 113.8 dB	0.19 dB 0.27 dB	0.40 dB 0.40 dB

STD = Standard

UUC = Unit Under Calibration

- End of Certificate -



www.forthcal.com

FORTH CALIBRATION & SERVICE CO., LTD.

305/47 Sor Ramintra 123, Ramintra Rd., Minburi, Minburi, Bangkok 10510
Tel. 0-2948-6668, 0-2517-6650-1 Fax. 0-2517-6674
E-mail: forthcalibration@gmail.com



CERTIFICATE OF CALIBRATION

Certificate No. : 66S0330-5

Job No. : 66S0330

Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.

Address : 31/9 Moo 13, Raikhing, Samphran,

Nakhornpathom 73210

Location : Laboratory

Equipment : Sound Level Meter

Ambient temperature : (20 ± 2) °C

Manufacturer : Tenmars

Relative humidity : (50 ± 15) %

Model : ST-109R

Atmospheric pressure : -

Serial No. : 221201934

Date of received : 08-Mar-2023

Identity No. : NS-11-001

Date of calibration : 10-Mar-2023

Range : See to Data

Date of issued : 13-Mar-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at :

- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn

Approved By :

Reviewed By : [] Mr. Sompong Srisert

[] Ms. Bhacharin Phanangkaw (MD)

[✓] Mr. Boonyarit Auejirakarn

[✓] Ms. Natthaparakarn Thammaphan

The reported expanded uncertainty is based on uncertainty multiplied by a coverage factor k = 2, providing a level of confidence approximately 95%.
This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.5	0.5	0.20
	104	104.5	0.5	0.20
	114	114.4	0.4	0.20
C	94	94.4	0.4	0.20
	104	104.4	0.4	0.20
	114	114.5	0.5	0.20
Z	94	94.4	0.4	0.20
	104	104.4	0.4	0.20
	114	114.5	0.5	0.20

UUC* = Unit Under Calibration

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S0330-7

Job No. : 66S0330

Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.

Address : 31/9 Moo 13, Raikhing, Samphran,

Nakhornpathom 73210

Location : Laboratory

Equipment : Sound Level Meter Ambient temperature : (20 ± 2) °C

Manufacturer : Scarlet Tech Relative humidity : (50 ± 15) %

Model : ST-11D Atmospheric pressure : -

Serial No. : 820388 Date of received : 08-Mar-2023

Identity No. : NS-12-001 Date of calibration : 10-Mar-2023

Range : See to Data Date of issued : 13-Mar-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at :

- National Institute of Metrology Thailand. (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn

Approved By :

Reviewed By : | Mr. Sompong Srisert

| Ms. Natthaparakarn Thammaphan

| Ms. Bhacharin Phanangkaew (MD)

| Mr. Boonyarit Auejirakarn

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.3	0.3	0.20
	104	104.3	0.3	0.20
	114	114.2	0.2	0.20
B	94	94.0	0.0	0.20
	104	103.8	-0.2	0.20
	114	113.6	-0.4	0.20
Z	94	94.3	0.3	0.20
	104	103.8	-0.2	0.20
	114	113.6	-0.4	0.20

UUC* = Unit Under Calibration

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S0330-6

Job No. : 66S0330

Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.

Address : 31/9 Moo 13, Raikhing, Samphran,

Nakhornpathom 73210

Location : Laboratory

Equipment : Sound Level Meter Ambient temperature : (20 ± 2) °C

Manufacturer : Scarlet Tech Relative humidity : (50 ± 15) %

Model : ST-11D Atmospheric pressure : -

Serial No. : 820891 Date of received : 08-Mar-2023

Identity No. : NS-12-002 Date of calibration : 10-Mar-2023

Range : See to Data Date of issued : 13-Mar-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EELBP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at :

- National Institute of Metrology Thailand. (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn

Approved By :

1 Ms. Bhacharin Phannangkaew (MD)

Reviewed By : 1 Mr. Sompong Srisert

1 Mr. Boonyarit Auejirakarn

1 Ms. Natthaprakarn Thammaphan

The reported expanded uncertainty is based uncertainty multiplied by a coverage factor k = 2, providing a level of confidence approximately 95%. This result relates only to the item calibrated. The certificate shall not be reproduced except in full, without the written approval of the calibration director.

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.0	0.0	0.20
	104	104.0	0.0	0.20
	114	114.0	0.0	0.20
B	94	94.4	0.4	0.20
	104	104.0	0.0	0.20
	114	113.8	-0.2	0.20
Z	94	94.0	0.0	0.20
	104	104.0	0.0	0.20
	114	113.8	-0.2	0.20

UUC* = Unit Under Calibration

- The End -

CERTIFICATE OF CALIBRATION

Certificate No. : 66S0330-8

Job No. : 66S0330

Page : 1 of 2

Customer : C.E.M Technology (Thailand) Co.,Ltd.

Address : 31/9 Moo 13, Raikhing, Samphran,

Nakhornpathom 73210

Location : Laboratory

Equipment : Sound Level Meter

Ambient temperature : (20 ± 2) °C

Manufacturer : Scarlet Tech

Relative humidity : (50 ± 15) %

Model : ST-11D

Atmospheric pressure : -

Serial No. : 820892

Date of received : 08-Mar-2023

Identity No. : NS-12-003

Date of calibration : 10-Mar-2023

Range : See to Data

Date of issued : 13-Mar-2023

Calibration Method : This instrument was calibrated by comparison measurement with sound level calibrator, according to in house calibration method.

Reference Standard Instruments :

Equipment	Model	Serial No.	Certification No.	Due Date
Sound Level Calibrator	8930B	2000210	EEL.BP.31/0664	15-Jun-2023

Traceability : This certification is traceable to the International System of Unit maintained at :

- National Institute of Metrology Thailand, (NIMT).

Calibrated By : Mr. Boonyarit Auejirakarn

Approved By :

Reviewed By : [] Mr. Sompong Srisert

[] Ms. Bhacharin Phannangkuew (MD)

✓ [] Ms. Natthaprakarn Thammaphan

✓ [] Mr. Boonyarit Auejirakarn

Result of Calibration : Without Adjustment

Function : Sound Level Measurement

Calibration Range : @ 1 kHz

Resolution : 0.1 dB / 1 dB

Response	Standard Setting (dB)	UUC Reading (dB)	Error Value (dB)	Uncertainty (+/-dB)
A	94	94.1	0.1	0.20
	104	104.0	0.0	0.20
	114	114.0	0.0	0.20
B	94	93.8	-0.2	0.00
	104	103.7	-0.3	0.00
	114	113.7	-0.3	0.00
Z	94	93.9	-0.1	0.00
	104	103.9	-0.1	0.00
	114	113.9	-0.1	0.00

UUC* = Unit Under Calibration

- The End -

Certificate of Calibration

EQUIPMENT : SOUND LEVEL METER

MANUFACTURER : ACO

MODEL : TYPE 6226

SERIAL No. : 060209

ID No. : CEM-SI-01

SUBMITTED BY : C.E.M TECHNOLOGY (THAILAND) CO.,LTD.
219/43 MOO 12, PETCHKASEM RD., OMNOI,
KRATHUMBAN SAMUTSAKORN 74130

CALIBRATED BY : *Suvant K.*

CALIBRATION DATE : 9-May-23

APPROVED BY : *Dongorn (Dn)*
PHUDIT P.

ISSUED DATE : 9-May-23

Calibration Report

EQUIPMENT : SOUND LEVEL METER
MANUFACTURER : ACO
MODEL : TYPE 6226
ID No. : CEM-SI-01
RECEIVED DATE : 4-May-23
AMBIENT TEMPERATURE : 22 °C ± 3°C
RELATIVE HUMIDITY : 50%RH ± 20%RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO IEC 61672-2:2003-04 AGAINST MULTIFUNCTION SOUND CALIBRATOR.
 THIS INSTRUMENT WAS PERFORMED SELF-CALIBRATION BY CALIBRATOR FROM CUSTOMER AT 114 Hz BEFORE CALIBRATION.

2. REFERENCE STANDARD INSTRUMENTS :

INSTRUMENT : 1986
MODEL : 01827
SERIAL No. : EEL BP 55/0974
CERTIFICATE No. : 12-Jan-24
DUE DATE :

1) MULTIFUNCTION
 SOUND CALIBRATOR.

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO :-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR).

RESULT OF CALIBRATION :

WITHOUT ADJUSTMENT

1. A-WEIGHTING ACOUSTIC FREQUENCY RESPONSE

FREQUENCY (Hz)	STANDARD EXPECTED READING (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
125.00	-16.10	-16.80	-0.30	0.50
250.00	-8.60	-8.10	-0.50	0.50
500.00	-3.20	-3.0	-0.20	0.50
1000.00	0.00	0.00	0.0	0.50
2000.00	1.20	0.90	0.3	0.50

2. C-WEIGHTING ACOUSTIC FREQUENCY RESPONSE

FREQUENCY (Hz)	STANDARD EXPECTED READING (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
125.00	-0.20	0.1	-0.3	0.50
250.00	0.00	0.5	-0.5	0.50
500.00	0.00	0.3	-0.3	0.50
1000.00	0.00	0.0	0.0	0.50
2000.00	-0.20	-0.4	0.2	0.50

3. SOUND LEVEL LINEARITY TEST AT 1000 Hz

STANDARD APPLIED (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
74	74.0	0.0	0.50
84	84.0	0.0	0.50
94	94.0	0.0	0.50
104	104.1	-0.1	0.50
114	114.2	-0.2	0.50

UUC* : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%

END OF CALIBRATION REPORT

Certificate of Calibration

EQUIPMENT : SOUND LEVEL METER
MANUFACTURER : ACO
MODEL : TYPE 6226
SERIAL No. : 060209
ID No. : CEM-SI-01
SUBMITTED BY : C.E.M TECHNOLOGY (THAILAND) CO.,LTD.
 219/43 MOO 12, PETCHKASEM RD., OMNOI,
 KRATHUMBAN SAMUTSAKORN 74130

CALIBRATED BY :

CALIBRATION DATE : 25-April-24

APPROVED BY :

ISSUED DATE : 25-April-24

Calibration Report

EQUIPMENT : SOUND LEVEL METER
 MANUFACTURER : ACO
 MODEL : TYPE 6226
 ID No. : CEM-SI-01
 RECEIVED DATE : 23-April-24
 AMBIENT TEMPERATURE : 22 °C ± 3°C
 RELATIVE HUMIDITY : 50%RH ± 20%RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO IEC 61672-2:2003-04 AGAINST MULTIFUNCTION SOUND CALIBRATOR.
 THIS INSTRUMENT WAS PERFORMED SELF-CALIBRATION BY CALIBRATOR FROM CUSTOMER AT 114 Hz BEFORE CALIBRATION.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT MODEL SERIAL No. CERTIFICATE No. DUE DATE
 1) MULTIFUNCTION 1986 01827 EEL BP.67/0874 10-Jan-25

SOUND CALIBRATOR.

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO :-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR).

RESULT OF CALIBRATION :

WITHOUT ADJUSTMENT

1. A-WEIGHTING ACOUSTIC FREQUENCY RESPONSE

FREQUENCY (Hz)	STANDARD EXPECTED READING (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
125.00	-16.10	-16.80	-0.30	0.50
250.00	-8.60	-8.10	-0.50	0.50
500.00	-3.20	-3.0	-0.20	0.50
1000.00	0.00	0.00	0.0	0.50
2000.00	1.20	0.90	0.3	0.50

2. C-WEIGHTING ACOUSTIC FREQUENCY RESPONSE

FREQUENCY (Hz)	STANDARD EXPECTED READING (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
125.00	-0.20	0.1	-0.3	0.50
250.00	0.00	0.5	-0.5	0.50
500.00	0.00	0.3	-0.3	0.50
1000.00	0.00	0.0	0.0	0.50
2000.00	-0.20	-0.4	0.2	0.50

3. SOUND LEVEL LINEARITY TEST AT 1000 Hz

STANDARD APPLIED (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
74	74.0	0.0	0.50
84	84.0	0.0	0.50
94	94.0	0.0	0.50
104	104.1	-0.1	0.50
114	114.2	-0.2	0.50

UUC* : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%

END OF CALIBRATION REPORT

Certificate of Calibration

EQUIPMENT : SOUND LEVEL METER
 MANUFACTURER : ACO
 MODEL : TYPE 6226
 SERIAL No. : 060210
 ID No. : CEM-SI-03
 SUBMITTED BY : C.E.M TECHNOLOGY (THAILAND) CO.,LTD.
 219/43 MOO 12, PETCHKASEM RD., OMNOI,
 KRATHUMBAN SAMUTSAKORN 74130

CALIBRATED BY

CALIBRATION DATE

APPROVED BY

ISSUED DATE

Calibration Report

EQUIPMENT : SOUND LEVEL METER
MANUFACTURER : ACO
MODEL : TYPE 6226
ID No. : CEM-SI-03
RECEIVED DATE : 4-May-23
AMBIENT TEMPERATURE : 22 °C ± 3 °C
RELATIVE HUMIDITY : 50%RH ± 20%RH

SERIAL NUMBER : 060210

CALIBRATION DATE : 9-May-23

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO IEC 61672-2:2003-04 AGAINST MULTIFUNCTION SOUND CALIBRATOR.
 THIS INSTRUMENT WAS PERFORMED SELF-CALIBRATION BY CALIBRATOR FROM CUSTOMER AT 114 Hz BEFORE CALIBRATION.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT : 1986
MODEL : 01827
SERIAL No. : EEL.BP.55/0974
CERTIFICATE No. :
DUE DATE : 12-Jan-24

1) MULTIFUNCTION
 SOUND CALIBRATOR.

3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO :-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR).

RESULT OF CALIBRATION :

WITHOUT ADJUSTMENT

1. A-WEIGHTING ACOUSTIC FREQUENCY RESPONSE

FREQUENCY (Hz)	STANDARD EXPECTED READING (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
125.00	-16.10	-16.80	-0.30	0.50
250.00	-8.60	-8.10	-0.50	0.50
500.00	-3.20	-3.0	-0.20	0.50
1000.00	0.00	0.00	0.0	0.50
2000.00	1.20	0.90	0.3	0.50

2. C-WEIGHTING ACOUSTIC FREQUENCY RESPONSE

FREQUENCY (Hz)	STANDARD EXPECTED READING (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
125.00	-0.20	0.1	-0.3	0.50
250.00	0.00	0.5	-0.5	0.50
500.00	0.00	0.3	-0.3	0.50
1000.00	0.00	0.0	0.0	0.50
2000.00	-0.20	-0.4	0.2	0.50

3. SOUND LEVEL LINEARITY TEST AT 1000 Hz

STANDARD APPLIED (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
74	74.0	0.0	0.50
84	84.0	0.0	0.50
94	94.0	0.0	0.50
104	104.1	-0.1	0.50
114	114.2	-0.2	0.50

UUC* : UNIT UNDER CALIBRATION

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%

END OF CALIBRATION REPORT

Certificate of Calibration

EQUIPMENT : SOUND LEVEL METER
MANUFACTURER : ACO
MODEL : TYPE 6226
SERIAL No. : 150008
ID No. : CEM-SI-08
SUBMITTED BY : C.E.M TECHNOLOGY (THAILAND) CO.,LTD.
 219/43 MOO 12, PETCHKASEM RD., OMNOI,
 KRATHUMBAN SAMUTSAKORN 74130

CALIBRATED BY

SURAWIT K.

SURAWIT K.

9-May-23

CALIBRATION DATE

APPROVED BY

PHUDIT P.

ISSUED DATE

9-May-23

Calibration Report

EQUIPMENT : SOUND LEVEL METER
MANUFACTURER : ACO
MODEL : TYPE 6226 **SERIAL NUMBER** : 150008
ID No. : CEM-SI-08
RECEIVED DATE : 4-May-23 **CALIBRATION DATE** : 9-May-23
AMBIENT TEMPERATURE : 22 °C ± 3 °C **RELATIVE HUMIDITY** : 50%RH ± 20%RH

CONDITION OF THIS RESULTS OF CALIBRATION
 1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO IEC 61672-2:2003-04 AGAINST MULTIFUNCTION SOUND CALIBRATOR.
 THIS INSTRUMENT WAS PERFORMED SELF-CALIBRATION BY CALIBRATOR FROM CUSTOMER AT 114 Hz BEFORE CALIBRATION.
 2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT **MODEL** **SERIAL No.** **CERTIFICATE No.** **DUE DATE**
 1) MULTIFUNCTION 1986 01827 EEL.BP.55/0974 12-Jan-24
 SOUND CALIBRATOR.
 3. THIS RESULT WAS FOUND ACCURATE AS SHOWN ON DATE AND PLACE OF CALIBRATION ONLY.
 4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
 5. THIS CERTIFICATE IS TRACEABLE TO :-
 - NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR).

RESULT OF CALIBRATION : WITHOUT ADJUSTMENT

1. A-WEIGHTING ACOUSTIC FREQUENCY RESPONSE				
FREQUENCY (Hz)	STANDARD EXPECTED READING (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
125.00	-16.10	-15.80	-0.30	0.50
250.00	-8.60	-8.10	-0.50	0.50
500.00	-3.20	-3.0	-0.20	0.50
1000.00	0.00	0.00	0.0	0.50
2000.00	1.20	0.90	0.3	0.50
2. C-WEIGHTING ACOUSTIC FREQUENCY RESPONSE				
FREQUENCY (Hz)	STANDARD EXPECTED READING (dB)	UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
125.00	-0.20	0.1	-0.3	0.50
250.00	0.00	0.5	-0.5	0.50
500.00	0.00	0.3	-0.3	0.50
1000.00	0.00	0.0	0.0	0.50
2000.00	-0.20	-0.4	0.2	0.50
3. SOUND LEVEL LINEARITY TEST AT 1000 Hz				
STANDARD APPLIED (dB)		UUC READING (dB)	CORRECTION (dB)	UNCERTAINTY OF MEASUREMENT (±dB)
74		74.0	0.0	0.50
84		84.0	0.0	0.50
94		94.0	0.0	0.50
104		104.1	-0.1	0.50
114		114.2	-0.2	0.50

UUC* : UNIT UNDER CALIBRATION
 THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%

END OF CALIBRATION REPORT



**ELECTRICAL AND ELECTRONICS INSTITUTE
 FOUNDATION FOR INDUSTRIAL DEVELOPMENT**
 975 Moo 4, Bangsoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
 Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
 Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240128EA
Operation No.: CP2024030097

Certificate of Calibration

Equipment: Sound Level Meter
Manufacturer: ACO
Model/Type: 6236 (Meter), 7052NR (Microphone), - (Preamplifier)
Serial No.: 222189 (Meter), 84153 (Microphone), - (Preamplifier)
ID No.: NS-03-019

Customer: C.E.M. Technology (Thailand) Co.,Ltd.

Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,
 Nakorn Phatom 73210

Received Date: 7 March 2024

Calibrated Date: 18 - 19 March 2024

Issued Date: 21 March 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by:

(Mr. Sittichai Swaksuriyawong)
 Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
 The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



Certificate No.: CP20240128EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: ACO
Model/Type: 6236 (Meter), 7052NR (Microphone), - (Preamplifier)
Serial No.: 222189 (Meter), 84153 (Microphone), - (Preamplifier)
ID No.: NS-03-019
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa
Method of Calibration :-
IEC61672-3:2013

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20230040EA	26 June 2024
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9609027	CB20230108EB	8 June 2024
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P230024 CD20230196EA	20 March 2024 23 July 2024
6) Pressure humidity and Temperature Transmitter	PTU301	F0640003	CL1-P230032 CD20230197EA	4 April 2024 23 July 2024
7) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EA CK20230072EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

- Reference standards instrument for Acoustic function
 - National Institute of Metrology (Thailand)
- Reference standards instrument for Electrical function
 - National Institute of Metrology (Thailand)
 - Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Certificate No.: CP20240128EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed	Measured value (dB)
	20.7

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	17.2
C-weighting	24.8
Z-weighting	32.1

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve		
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)
125	0.2	0.1	0.1
1000	-0.2	-0.2	-0.2
8000	-0.5	-0.4	-0.3

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve		
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)
63	-0.1	-0.2	0.0
125	0.0	-0.2	0.1
250	0.0	0.0	0.0
500	0.1	0.0	0.1
1000	0.0	0.0	0.0
2000	-0.1	0.0	0.0
4000	-0.3	-0.3	0.0
8000	-0.5	-0.4	-0.2



Certificate No.: CP20240128EA

CP20240128EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
120.0	120.0	0.0	±1.1
121.0	121.0	0.0	±1.1

Certificate No.: CP20240128EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	43.9	-0.1	±1.1
39.0	38.9	-0.1	±1.1
34.0	34.0	0.0	±1.1
33.0	33.1	0.1	±1.1
32.0	32.2	0.2	±1.1
31.0	31.3	0.3	±1.1
30.0	30.4	0.4	±1.1
29.0	29.5	0.5	±1.1

Function : 8. Level Linearity including level range control

8.1 Level Linearity Including the Level Range (Reference Signal)

Range	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
20-100	94.0	94.0	0.0	±1.1
20-110	94.0	94.0	0.0	±1.1
30-120	94.0	94.0	0.0	±1.1
40-130	94.0	94.0	0.0	±1.1

8.2 Level Linearity including the Level range (5dB Above Under-range)

Range	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
20-80	25.0	25.3	0.3	±1.1
20-90	25.0	25.3	0.3	±1.1
20-100	25.0	25.2	0.2	±1.1
20-110	25.0	25.5	0.5	±1.1
30-120	35.0	35.0	0.0	±1.1
40-130	45.0	45.0	0.0	±1.1

Certificate No.: CP20240128EA

Calibration Report

Function : 9. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	116.0	0.0	±1.0
	2	98.9	-0.1	+1.0 ; -2.5
	0.25	89.9	-0.1	+1.5 ; -5.0
Slow	200	109.5	-0.1	±1.0
	2	89.8	-0.2	+1.0 ; -5.0
	0.25	80.9	-0.1	+1.5 ; -5.0
LAE	200	109.9	-0.1	±1.0
	2	90.0	0.0	+1.0 ; -2.5
	0.25	80.9	-0.1	+1.5 ; -5.0

Function : 10. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	125.4	125.4	0.0	±3.0
Positive half cycle	124.4	124.2	-0.2	±2.0
Negative half cycle	124.4	124.2	-0.2	±2.0

Function : 11. Overload indication

Positive one-half cycle	Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
	Negative one-half cycle			
-	-	-	-	-

Function : 12. High-Level Stability

High-Level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	129.0	129.0	0.0	±0.3

Certificate No.: CP20240128EA

Calibration Report

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Level Linearity including level range control	0.30	0.30
9) Tone burst response	0.20	0.30
10) Peak C sound level	0.20	0.35
11) Overload indication	0.20	0.25
12) High-Level Stability	0.10	0.10

Remarks: 1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. Overload indication can not measured because sound level meter can not set to Reference value of the standard calibration.
3. The acceptance limit is for the deviated value.
4. Acceptance limits was IEC61672-3:2013 Class 2.
5. The coverage factor $k = 2.00$

-- End of Report --



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT
975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240129EA
Operation No.: CP2024030098

Certificate of Calibration

Equipment: Sound Level Meter
Manufacturer: SCARLET TECH
Model/Type: ST11D (Meter), AWA14425 (Microphone), - (Preamplifier)
Serial No.: 820891 (Meter), 57258 (Microphone), - (Preamplifier)
ID No.: NS-12-002
Customer: C.E.M. Technology (Thailand) Co.,Ltd.
Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,
Nakorn Phatom 73210

Received Date: 7 March 2024
Calibrated Date: 20 - 21 March 2024
Issued Date: 21 March 2024
Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k)
providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except
with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

Certificate No.: CP20240129EA

Calibration Report

Equipment: Sound Level Meter
Manufacturer: SCARLET TECH
Model/Type: ST11D (Meter), AWA14425 (Microphone), - (Preamplifier)
Serial No.: 820891 (Meter), 57258 (Microphone), - (Preamplifier)
ID No.: NS-12-002
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Pressure: (101.3 ± 1.5) kPa
Method of Calibration :-
IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1012-23	12 November 2024
2) Arbitrary Function Generator	AFG2021	C010063	CK20230040EA	26 June 2024
3) Programmable Attenuator	PA5	2755	EF-0040-23	1 October 2024
4) 6.5 Digit precision multimeter	8846A	9609027	CB20230108EB	8 June 2024
5) Pressure humidity and Temperature Transmitter	PTU301	F0640003	CD20230197EA	4 April 2024 23 July 2024
6) Performance Audio Analyzer	U8903B	MY56510003	CB20240035EA	13 February 2025 13 September 2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

- Reference standards instrument for Acoustic function
 - National Institute of Metrology (Thailand)
- Reference standards instrument for Electrical function
 - National Institute of Metrology (Thailand)
 - Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-



Certificate No.: CP20240129EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
15.9

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	6.6
C-weighting	8.0
Z-weighting	15.3

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve		
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)
125	0.5	0.4	0.4
1000	-0.1	-0.1	-0.1
8000	-0.7	-0.6	-0.7
			Acceptance limits (dB)
			±1.0
			±0.7
			+1.5; -2.5

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve		
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)
63	0.0	0.0	0.0
125	0.0	-0.1	0.0
250	0.0	-0.1	0.0
500	0.0	0.0	0.0
1000	0.0	0.0	0.0
2000	0.1	0.0	0.0
4000	0.1	0.1	0.0
8000	-0.1	-0.1	0.1
16000	-5.3	-5.2	0.1
			Acceptance limits (dB)
			±1.0
			±1.0
			±1.0
			±0.7
			±1.0
			+1.5; -2.5
			+2.5; -16.0

Certificate No.: CP20240129EA

Calibration Report

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.1	0.1	±0.2
Z-weighting	94.0	0.0	±0.2

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	SPL Reference (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.1

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
99.0	99.0	0.0	±0.8
104.0	104.0	0.0	±0.8
109.0	109.0	0.0	±0.8
114.0	114.0	0.0	±0.8
119.0	119.0	0.0	±0.8
124.0	124.0	0.0	±0.8
129.0	129.0	0.0	±0.8
134.0	134.0	0.0	±0.8
139.0	139.0	0.0	±0.8

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8

Certificate No.: CP20240129EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	33.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	27.9	-0.1	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.8	-0.2	±0.8
24.0	23.9	-0.1	±0.8
23.0	22.8	-0.2	±0.8
22.0	21.6	-0.4	±0.8
21.0	20.5	-0.5	±0.8
20.0	19.5	-0.5	±0.8
19.0	18.5	-0.5	±0.8

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±0.5
	2	118.9	-0.1	+1.0 ; -1.5
	0.25	109.9	-0.1	+1.0 ; -3.0
Slow	200	129.6	0.0	±0.5
	2	110.0	0.0	+1.0 ; -3.0
	200	130.1	0.1	±0.5
SEL	2	110.0	0.0	+1.0 ; -1.5
	0.25	100.9	-0.1	+1.0 ; -3.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	135.7	0.3	±2.0
Positive half cycle	134.4	133.9	-0.5	±1.0
Negative half cycle	134.4	134.0	-0.4	±1.0

Certificate No.: CP20240129EA

Calibration Report

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
142.5	143.3	0.8	±1.5

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.1

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks: 1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.

2. The acceptance limit is for the deviated value.

3. Acceptance limits was IEC61672-3:2013 Class 1.

4. The coverage factor $k = 2.00$

-- End of Report --



Trade & Engineering
TSP High Volume Sampler
TE-5000 TSP Sampler Verification
Site Information

Location: -	Site ID: -	Date: 16 Oct 23
Sampler: TE-5000 TSP	Serial No: 3269	Tech: Tong.P

Site Conditions

Barometric Pressure (in Hg): 27.80	Corrected Pressure (mm Hg): 705.1
Temperature (deg F): 76.1	Temperature (deg K): 297.7
Average Press. (in Hg): 27.30	Corrected Average (mm Hg): 693.4
Average Temp (Deg F): 75.0	Average Temp: (Deg K): 297.0

Calibration Orifice

Make: Tisch	Qstd Slope: 1.56304
Model: TE-5028A	Qstd Intercept: -0.01520
Serial#: 1179	Calibration Due Date 12 December 2023

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	Linear Regression Slope
1	7.50	1.678	59.7	57.58	35.4041
2	6.30	1.539	55.4	53.43	Intercept: -2.1709
3	5.20	1.399	47.9	46.20	Corr. Coeff: 0.9834
4	4.50	1.302	43.7	42.15	
5	3.10	1.112	40.1	38.68	# of Observations: 5

Calculations

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$
$$IC = [(\text{Sqrt}(Pa/Pstd)(Tstd/Ta))]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

Tstd = 298 deg K

Pstd = 760 mm Hg

For subsequent calculation of sampler flow:


$$1/m[(I) \text{Sqrt}(298/Tav)(Pav/760))-b]$$

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure

Enter Average I (chart): 49.4
Average Flow Calculation m3/min
1.395189676
Average Flow Calculation in cfm
49.26517152
Sample Time (Hrs): 24.0
Total flow in 24 hours m3/min
2009.073133
Total flow in 24 hours cfm
70941.84699

NOTE: Ensure calibration orifice has been certified within 12 months of use

เอกสารการสอบเทียบเครื่องมือตรวจวัดคุณภาพอากาศในบรรยากาศ



Trade & Engineering

**TSP High Volume Sampler
TE-5000 TSP Sampler Verification
Site Information**

Location: -	Site ID: -	Date: 16 Oct. 23
Sampler: TE-5000 TSP	Serial No: 3270	Tech: Tong, P

Site Conditions

Barometric Pressure (in Hg): 27.60	Corrected Pressure (mm Hg): 701.0
Temperature (deg F): 76.0	Temperature (deg K): 297.6
Average Press. (in Hg): 27.50	Corrected Average (mm Hg): 698.5
Average Temp (Deg F): 74.8	Average Temp: (Deg K): 296.9

Calibration Orifice

Make: Tisch	Qstd Slope: 1.56304
Model: TE-5028A	Qstd Intercept: -0.01520
Serial#: 1179	Calibration Due Date: 12 December 2023

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	Linear Regression Slope
1	7.80	1.705	60.1	57.76	28.1557
2	6.00	1.497	57.2	54.97	11.0629
3	5.30	1.407	53.4	51.32	
4	4.50	1.297	49.7	47.77	0.9717
5	3.90	1.209	45.6	43.83	
					# of Observations: 5

Calculations

$$Qstd = 1/m[\sqrt{Pa(Pa/Pstd)(Tstd/Ta))}-b]$$
$$IC = [(\sqrt{Pa/Pstd)(Tstd/Ta))}]$$

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg

For subsequent calculation of sampler flow:

$$1/m[(I)[\sqrt{Pa(Pa/Pstd)(Tstd/Ta))}-b]$$

Enter Average 1 (chart): 53.2
Average Flow Calculation m3/min 1.421779972
Average Flow Calculation in cfm 50.2040944
Sample Time (Hrs): 24.0
Total flow in 24 hours m3/min 2047.36316
Total flow in 24 hours cfm 72293.89593

NOTE: Ensure calibration orifice has been certified within 12 months of use

Tisch Environmental 145 South Miami Ave, Cleves OH 45002 • 877.263.7610 • sales@tisch-env.com • www.tisch-env.com



Trade & Engineering

**TSP High Volume Sampler
TE-5000 TSP Sampler Verification
Site Information**

Location: -	Site ID: -	Date: 18 Oct. 23
Sampler: TE-5000 TSP	Serial No: 3280	Tech: Tong, P

Site Conditions

Barometric Pressure (in Hg): 28.40	Corrected Pressure (mm Hg): 721.4
Temperature (deg F): 77.0	Temperature (deg K): 298.2
Average Press. (in Hg): 26.50	Corrected Average (mm Hg): 673.1
Average Temp (Deg F): 75.8	Average Temp: (Deg K): 297.5

Calibration Orifice

Make: Tisch	Qstd Slope: 1.56304
Model: TE-5028A	Qstd Intercept: -0.01520
Serial#: 1179	Calibration Due Date: 12 December 2023

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart)	IC (corrected)	Linear Regression Slope
1	7.50	1.695	60.9	59.32	39.2312
2	6.00	1.517	56.0	54.54	-5.8658
3	4.80	1.358	50.7	49.38	
4	4.30	1.285	45.8	44.61	0.9824
5	3.60	1.177	39.7	38.67	
					# of Observations: 5

Calculations

$$Qstd = 1/m[\sqrt{Pa(Pa/Pstd)(Tstd/Ta))}-b]$$
$$IC = [(\sqrt{Pa/Pstd)(Tstd/Ta))}]$$

Qstd = standard flow rate
IC = corrected chart response
I = actual chart response
m = calibrator Qstd slope
b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)
Pa = actual pressure during calibration (mm Hg)
Tstd = 298 deg K
Pstd = 760 mm Hg

For subsequent calculation of sampler flow:

$$1/m[(I)[\sqrt{Pa(Pa/Pstd)(Tstd/Ta))}-b]$$

Enter Average 1 (chart): 50.6
Average Flow Calculation m3/min 1.364865144
Average Flow Calculation in cfm 48.19439004
Sample Time (Hrs): 24.0
Total flow in 24 hours m3/min 1965.405807
Total flow in 24 hours cfm 69399.92166

NOTE: Ensure calibration orifice has been certified within 12 months of use

Tisch Environmental 145 South Miami Ave, Cleves OH 45002 • 877.263.7610 • sales@tisch-env.com • www.tisch-env.com



PM10 High Volume Sampler Verification

Site Information

Location: - Site ID: - Date: 2 October 2023
Sampler: TE-6070 PM10 Serial No: 3183 Tech: Tong P.

Site Conditions

Barometric Pressure (in Hg): 27.02
Temperature (deg F): 75.3
Average Press. (in Hg): 26.70
Average Temp. (deg F): 76.1
Corrected Pressure (mm Hg): 686.3
Temperature (deg K): 297.1
Corrected Average (mm Hg): 678.2
Average Temp. (deg K): 297.5

Calibration Orifice

Make: Tisch Environmental, Inc.
Model: TE-5028A
Serial#: 1179
Qstd Slope: 1.58304
Qstd Intercept: -0.01520
Calibration Due Date: 12 Dec 23

Calibration Data

Plate or Test #	In H2O	Qa (m3/min)	I (chart) (corrected)	IC
1	9.45	1.287	60.5	39.80
2	7.75	1.167	55.3	36.38
3	6.50	1.069	50.7	33.36
4	5.75	1.006	45.3	29.80
5	4.60	0.901	39.6	26.05

Linear Regression
Slope 36.1461
Intercept -6.1754
Corr. Coeff 0.9935
SFR 1.115
SSP 51.87

of Observations: 5

Calculations

$$Qa = 1/m(\sqrt{(H2O)(Ta/Pa)} - b)$$
$$IC = I(\sqrt{(Ta/Pa)})$$

$$SFR = 1.13(Ps/Pa)(Ta/Ts)$$
$$SSP = (m^2SFR + b)(\sqrt{(Pa/Ta)})$$

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure


$$Qa = \text{actual flow rate}$$
$$IC = \text{corrected chart response}$$
$$m = \text{calibrator slope}$$
$$b = \text{calibrator intercept}$$
$$Ta = \text{actual temperature (deg K)}$$
$$Pa = \text{actual pressure (mm Hg)}$$

For subsequent calculation of sampler flow:

$$Qa = \text{sampler set point flow rate}$$
$$SSP = \text{sampler chart set point}$$
$$m = \text{sampler slope}$$
$$b = \text{sampler intercept}$$
$$Ta = \text{actual temperature (deg K)}$$
$$Pa = \text{actual pressure (mm Hg)}$$
$$Ts = \text{Average temperature (deg K)}$$
$$Ps = \text{Average pressure (mm Hg)}$$

Average I (chart): 50.3
Average Flow over Sample (m3/min) 1.092521097
Enter Total Time (Hrs): 24.0
Total flow over sample (m3/min) 1573.23038
Total flow over sample (CFM) 55550.76473

NOTE: Ensure calibration orifice has been certified within 12 months of use



TSP High Volume Sampler TE-5000 TSP Sampler Verification

Site Information

Location: - Site ID: - Date: 16 Oct 23
Sampler: TE-5000 TSP Serial No: 3273 Tech: Tong P.

Site Conditions

Barometric Pressure (in Hg): 27.50
Temperature (deg F): 76.0
Average Press. (in Hg): 27.00
Average Temp (Deg F): 75.5
Corrected Pressure (mm Hg): 698.5
Temperature (deg K): 297.6
Corrected Average (mm Hg): 685.8
Average Temp: (Deg K): 297.3

Calibration Orifice

Make: Tisch
Model: TE-5028A
Serial#: 1179
Qstd Slope: 1.58304
Qstd Intercept: -0.01520
Calibration Due Date 12 December 2023

Calibration Information

Plate or Test #	H2O (in)	Qstd (m3/min)	I (chart) (corrected)	IC
1	6.60	1.566	61.0	58.52
2	5.50	1.431	57.9	55.55
3	4.20	1.252	51.3	49.21
4	3.70	1.175	47.3	45.38
5	3.00	1.059	40.0	38.37

of Observations: 5

Calculations

$$Qstd = 1/m(\sqrt{(H2O)(Pa/Pstd)}(Tstd/Ta)) - b$$
$$IC = I(\sqrt{(Pa/Pstd)}(Tstd/Ta))$$

m = sampler slope
b = sampler intercept
I = chart response
Tav = daily average temperature
Pav = daily average pressure


$$Qstd = \text{standard flow rate}$$
$$IC = \text{corrected chart response}$$
$$I = \text{actual chart response}$$
$$m = \text{calibrator Qstd slope}$$
$$b = \text{calibrator Qstd intercept}$$
$$Ta = \text{actual temperature during calibration (deg K)}$$
$$Pa = \text{actual pressure during calibration (mm Hg)}$$
$$Tstd = 298 \text{ deg K}$$
$$Pstd = 760 \text{ mm Hg}$$

For subsequent calculation of sampler flow:

$$Qstd = \text{sampler slope}$$
$$b = \text{sampler intercept}$$
$$I = \text{chart response}$$
$$Tav = \text{daily average temperature}$$
$$Pav = \text{daily average pressure}$$

Enter Average I (chart): 51.5
Average Flow Calculation m3/min 1.28570333
Average Flow Calculation in cfm 45.39912828
Sample Time (Hrs): 24.0
Total flow in 24 hours m3/min 1851.412795
Total flow in 24 hours cfm 65374.74472

NOTE: Ensure calibration orifice has been certified within 12 months of use



PM10 High Volume Sampler Verification

Site Information

Location: - Site ID: - Date: 2 October 2023
Sampler: TE-6070 PM10 Serial No: 3183 Tech: Tong P.

Site Conditions

Barometric Pressure (in Hg): 27.02 Corrected Pressure (mm Hg): 686.3
Temperature (deg F): 75.3 Temperature (deg K): 297.1
Average Press. (in Hg): 26.70 Corrected Average (mm Hg): 678.2
Average Temp. (deg F): 76.1 Average Temp. (deg K): 297.5

Calibration Orifice

Make: Tisch Environmental, Inc. Qstd Slope: 1.58304
Model: TE-5028A Qstd Intercept: -0.01520
Serial#: 1179 Calibration Due Date: 12 Dec 23

Calibration Data

Plate or Test #	In H2O	Qa (m3/min)	I (chart) (corrected)	IC	Linear Regression Slope
1	9.45	1.287	60.5	39.80	36.1461
2	7.75	1.167	55.3	36.38	-6.1754
3	6.50	1.069	50.7	33.36	0.9935
4	5.75	1.006	45.3	29.80	1.115
5	4.60	0.901	39.6	26.05	51.87

of Observations: 5

Calculations

Qa = $1/m(\sqrt{(H_2O)(Ta/Pa)})-b$
IC = $I(\sqrt{(Ta/Pa)})$

m = sampler slope
b = sampler intercept
I = chart response

Tav = daily average temperature
Pav = daily average pressure

Qa = actual flow rate
IC = corrected chart response
m = calibrator slope

b = calibrator intercept


Ta = actual temperature (deg K)
Pa = actual pressure (mm Hg)

Ts = Average temperature (deg K)
Ps = Average pressure (mm Hg)

Average I (chart): 50.3
Average Flow over Sample (m3/min) 1.092521097
Enter Total Time (Hrs): 24.0
Total flow over sample (m3/min) 1573.23038

NOTE: Ensure calibration orifice has been certified within 12 months of use

Total flow over sample (CFM) 55550.76473



PM10 High Volume Sampler Verification

Site Information

Location: - Site ID: - Date: 2 October 2023
Sampler: TE-6070 PM10 Serial No: 3211 Tech: Tong P.

Site Conditions

Barometric Pressure (in Hg): 27.10 Corrected Pressure (mm Hg): 688.3
Temperature (deg F): 75.3 Temperature (deg K): 297.0
Average Press. (in Hg): 26.55 Corrected Average (mm Hg): 674.4
Average Temp. (deg F): 76.2 Average Temp. (deg K): 297.6

Calibration Orifice

Make: Tisch Environmental, Inc. Qstd Slope: 1.58304
Model: TE-5028A Qstd Intercept: -0.01520
Serial#: 1179 Calibration Due Date: 12 Dec 23

Calibration Data

Plate or Test #	In H2O	Qa (m3/min)	I (chart) (corrected)	IC	Linear Regression Slope
1	9.60	1.295	60.7	39.87	34.8028
2	7.50	1.146	55.5	36.46	-4.2838
3	6.45	1.063	50.8	33.37	0.9827
4	5.35	0.969	45.9	30.15	1.105
5	4.60	0.900	39.2	25.75	52.02

of Observations: 5

Calculations

Qa = $1/m(\sqrt{(H_2O)(Ta/Pa)})-b$
IC = $I(\sqrt{(Ta/Pa)})$

m = sampler slope
b = sampler intercept
I = chart response

Tav = daily average temperature
Pav = daily average pressure

Qa = actual flow rate
IC = corrected chart response
m = calibrator slope

b = calibrator intercept

Ta = actual temperature (deg K)
Pa = actual pressure (mm Hg)

Ts = Average temperature (deg K)
Ps = Average pressure (mm Hg)

Average I (chart): 50.4
Average Flow over Sample (m3/min) 1.085070646
Enter Total Time (Hrs): 24.0
Total flow over sample (m3/min) 1562.501731

NOTE: Ensure calibration orifice has been certified within 12 months of use

Total flow over sample (CFM) 55171.9361



PM10 High Volume Sampler Verification

Site Information

Location: - Site ID: - Date: 2 October 2023
Sampler: TE-6070 PM10 Serial No: 3245 Tech: Tong P.

Site Conditions

Barometric Pressure (in Hg): 27.50 Corrected Pressure (mm Hg): 698.5
Temperature (deg F): 75.2 Temperature (deg K): 297.0
Average Press. (in Hg): 26.48 Corrected Average (mm Hg): 672.6
Average Temp. (deg F): 76.0 Average Temp. (deg K): 297.4

Calibration Orifice

Make: Tisch Environmental, Inc. Qstd Slope: 1.58304
Model: TE-5028A Qstd Intercept: -0.01520
Serial#: 1179 Calibration Due Date: 12 Dec 23

Calibration Data

Plate or Test #	In H2O	Qa (m3/min)	I (chart) (corrected)	IC	Linear Regression Slope	Intercept	Corr. Coeff	SFR	SSP	# of Observations:
1	9.35	1.269	60.0	39.12	36.6800	-6.6541	0.9908	1.091533108	50.2	5
2	7.65	1.149	55.4	36.12						
3	6.55	1.064	50.9	33.19						
4	5.70	0.993	45.5	29.67						
5	4.65	0.898	39.4	25.69						

Calculations

$Qa = 1/m(\sqrt{(H2O)(Ta/Pa)})-b$
 $IC = I(\sqrt{(Ta/Pa)})$

m = sampler slope
b = sampler intercept
I = chart response

Tav = daily average temperature
Pav = daily average pressure

Qa = actual flow rate
IC = corrected chart response
m = calibrator slope

b = calibrator intercept


Ta = actual temperature (deg K)
Pa = actual pressure (mm Hg)

Ts = Average temperature (deg K)
Ps = Average pressure (mm Hg)

For subsequent calculation of sampler flow:

Average I (chart): 50.2
Average Flow over Sample (m3/min): 1.091533108
Enter Total Time (Hrs): 24.0
Total flow over sample (m3/min): 1571.807676
Total flow over sample (CFM): 55500.52903

NOTE: Ensure calibration orifice has been certified within 12 months of use



PM10 High Volume Sampler Verification

Site Information

Location: - Site ID: - Date: 2 October 2023
Sampler: TE-6070 PM10 Serial No: 3482 Tech: Tong P.

Site Conditions

Barometric Pressure (in Hg): 26.65 Corrected Pressure (mm Hg): 676.9
Temperature (deg F): 75.3 Temperature (deg K): 297.1
Average Press. (in Hg): 26.50 Corrected Average (mm Hg): 673.1
Average Temp. (deg F): 76.3 Average Temp. (deg K): 297.6

Calibration Orifice

Make: Tisch Environmental, Inc. Qstd Slope: 1.58304
Model: TE-5028A Qstd Intercept: -0.01520
Serial#: 1179 Calibration Due Date: 12 Dec 23

Calibration Data

Plate or Test #	In H2O	Qa (m3/min)	I (chart) (corrected)	IC	Linear Regression Slope	Intercept	Corr. Coeff	SFR	SSP	# of Observations:
1	9.65	1.310	60.5	40.08	34.0516	-3.5657	0.9827	1.1122	52.27	5
2	7.50	1.156	55.5	36.77						
3	6.45	1.072	50.6	33.52						
4	5.35	0.978	45.8	30.34						
5	4.60	0.907	39.4	26.10						

Calculations

$Qa = 1/m(\sqrt{(H2O)(Ta/Pa)})-b$
 $IC = I(\sqrt{(Ta/Pa)})$

m = sampler slope
b = sampler intercept
I = chart response

Tav = daily average temperature
Pav = daily average pressure

Qa = actual flow rate
IC = corrected chart response
m = calibrator slope

b = calibrator intercept

Ta = actual temperature (deg K)
Pa = actual pressure (mm Hg)

Ts = Average temperature (deg K)
Ps = Average pressure (mm Hg)

For subsequent calculation of sampler flow:

Average I (chart): 50.4
Average Flow over Sample (m3/min): 1.08858164
Enter Total Time (Hrs): 24.0
Total flow over sample (m3/min): 1567.955756
Total flow over sample (CFM): 55364.51773

NOTE: Ensure calibration orifice has been certified within 12 months of use

Certificate of Analyzer Performance Testing

Calibrated Date : 15-Jan-24 Certificate No. : 0124-001 Page : 1/1

Analyzer Instruments
 Analyzer Type : THC Analyzer
 Model : 51
 Manufacturer : Thermo Environmental
 Serial No. : 51HT-72244-373


Environmental
 Temperature : 25.1 °C
 Humidity : 40.4 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 Propane Conc. : 150 ppm
 Cylinder No. : 21W281046
 Expire Date : 26-Sep-25

Calibration Check

Gas	Zero				Span			
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)		Reading Value (ppm)	Expected Value (ppm)	Drift (%)	
Before								
THC	0.041	0.050	0.041		132	150	1.333	
After								
THC	0.050	0.050	0.000		150	150	0.000	

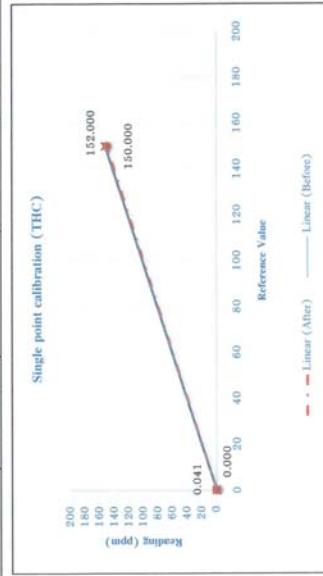

Calibrated by : *Topin*
 (Mr. Tong Pina)

Certificate of Analyzer Performance Testing

Calibrated Date : 15-Jan-24 Certificate No. : 0124-002 Page : 1/1

Analyzer Instruments
 Analyzer Type : THC Analyzer
 Model : Series 8800
 Manufacturer : Baseline
 Serial No. : 584


Environmental
 Temperature : 24.6 °C
 Humidity : 45.1 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 Propane Conc. : 150 ppm
 Cylinder No. : 21W281046
 Expire Date : 26-Sep-25

Calibration Check

Gas	Zero				Span			
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)		Reading Value (ppm)	Expected Value (ppm)	Drift (%)	
Before								
THC	0.046	0.000	0.046		151	150	0.667	
After								
THC	0.050	0.000	0.000		150	150	0.000	

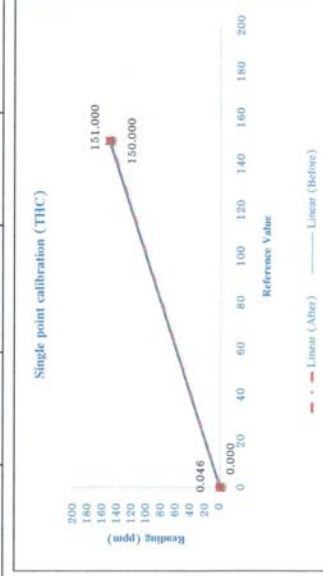

Calibrated by : *Topin*
 (Mr. Tong Pina)

Certificate of Analyzer Performance Testing

Calibrated Date : 22-Jul-23 Certificate No. : 0723-001 Page : 1/1

Analyzer Instruments

Analyzer Type : CO Analyzer Manufacturer : Thermo Environmental
Model : 48C Serial No. : 508011061

Environmental

Temperature : 24.2 °C
Humidity : 52.0 %RH

Calibration System

Calibrator Units


Gas Calibration : Thermo Environmental : API
Model : 146C Model : 701
Serial No. : 514811438 Serial No. : 179

Standard Gas

NO Conc. : 2 ppm
SO2 Conc. : 2 ppm
CO Conc. : 50 ppm

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
CO	0.089	0.000	0.09	Before		
				50.2	50.000	0.40
CO	0.000	0.000	0.00	After		
				50.0	50.000	0.00

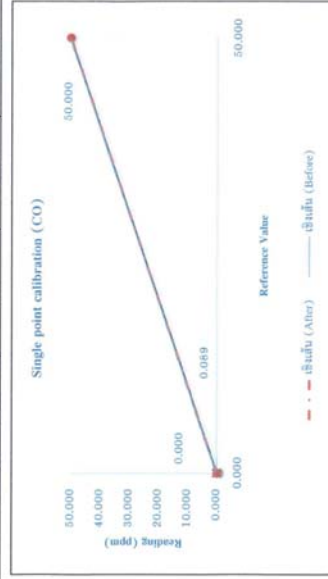

Calibrated by :
(Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 11-Mar-23 Certificate No. : 0323-001 Page : 1/1

Analyzer Instruments

Analyzer Type : CO Analyzer Manufacturer : Thermo Environmental
Model : 48C Serial No. : 65775350

Environmental

Temperature : 24.3 °C
Humidity : 51.4 %RH

Calibration System

Calibrator Units


Gas Calibration : Thermo Environmental : API
Model : 146C Model : 701
Serial No. : 514811458 Serial No. : 179

Standard Gas

NO Conc. : 2 ppm
SO2 Conc. : 2 ppm
CO Conc. : 50 ppm

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
CO	0.044	0.000	0.04	Before		
				49.670	50.000	-0.66
CO	0.000	0.000	0.00	After		
				50.000	50.000	0.00

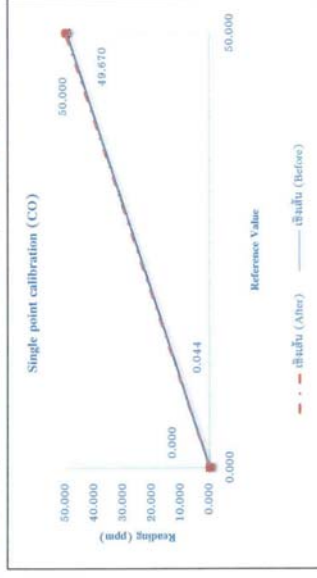

Calibrated by :
(Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 1-Apr-23 Certificate No. : 0423-001 Page : 1/1

Analyzer Instruments
 Analyzer Type : CO Analyzer
 Model : 48C
 Manufacturer : Thermo Environmental
 Serial No. : 401304261


Environmental
 Temperature : 25.2 °C
 Humidity : 52.3 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
CO	0.025	0.000	0.03	49.456	50.000	-1.09
	0.000	0.000	0.00	50.000	50.000	0.00

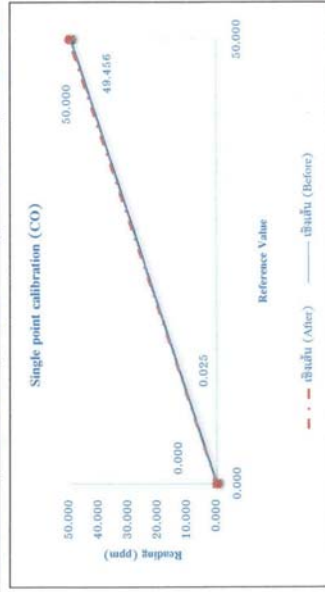

Calibrated by :

Thong
(Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 26-Aug-23 Certificate No. : 0823-003 Page : 1/1

Analyzer Instruments
 Analyzer Type : CO Analyzer
 Model : 48C
 Manufacturer : Thermo Environmental
 Serial No. : 508011069


Environmental
 Temperature : 25.6 °C
 Humidity : 53.7 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
CO	0.076	0.000	0.08	50.1	50.000	0.20
	0.000	0.000	0.00	50.0	50.000	0.00

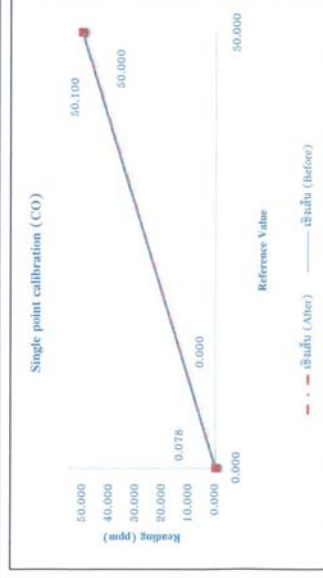

Calibrated by :

Thong
(Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 26-Aug-23 Certificate No. : 0823-006 Page : 1/1

Analyzer Instruments
 Analyzer Type : CO Analyzer
 Model : 48C
 Manufacturer : Thermo Environmental
 Serial No. : 508011064

Environmental
 Temperature : 24.9 °C
 Humidity : 41.3 %RH


Calibration System

Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811438
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
CO	Before			After		
	0.098	0.000	0.10	50.3	50.000	0.60
CO	0.000	0.000	0.00	50.0	50.000	0.00

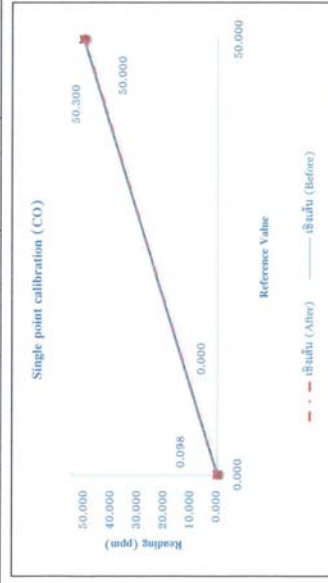

Calibrated by :  (Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 10-Jun-23 Certificate No. : 0023-001 Page : 1/1

Analyzer Instruments
 Analyzer Type : CO Analyzer
 Model : 48C
 Manufacturer : Thermo Environmental
 Serial No. : 508011068

Environmental
 Temperature : 25.2 °C
 Humidity : 51.3 %RH


Calibration System


Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811438
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
CO	Before			After		
	0.059	0.000	0.06	50.1	50.000	0.18
CO	0.000	0.000	0.00	50.0	50.000	0.00

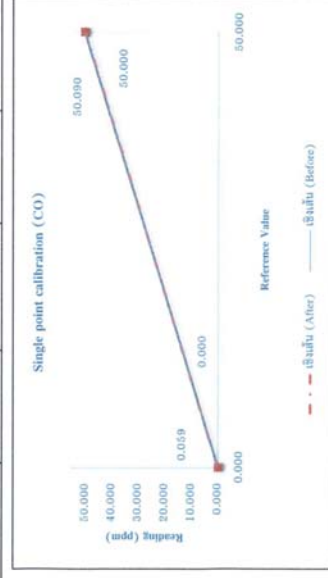

Calibrated by :  (Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 26-Aug-23 Certificate No. : 0823-001 Page : 1/1

Analyzer Instruments
 Analyzer Type : NO/NO_x/NO_x Analyzer
 Model : 42C
 Manufacturer : Thermo Environmental
 Serial No. : 66193-351


Environmental
 Temperature : 25.3 °C
 Humidity : 40.2 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO₂ : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
NO	0.061	0.000	0.06	2.01	2.00	0.50
NO _x	0.052	0.000	0.05	1.99	2.00	-0.50
After						
NO	0.000	0.000	0.00	2.00	2.00	0.00
NO _x	0.000	0.000	0.00	2.00	2.00	0.00

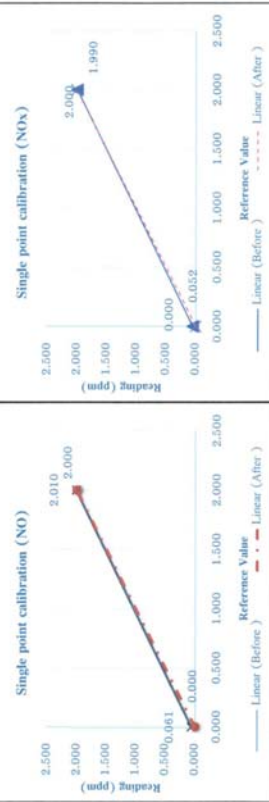

Calibrated by :
 (Mr. Yong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 11-Mar-23 Certificate No. : 0323-003 Page : 1/1

Analyzer Instruments
 Analyzer Type : NO/NO_x/NO_x Analyzer
 Model : 42C
 Manufacturer : Thermo Environmental
 Serial No. : 58926-320


Environmental
 Temperature : 24.3 °C
 Humidity : 51.4 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO₂ : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
NO	0.065	0.000	0.07	1.99	2.00	-0.50
NO _x	0.052	0.000	0.05	1.97	2.00	-1.50
After						
NO	0.000	0.000	0.00	2.00	2.00	0.00
NO _x	0.000	0.000	0.00	2.00	2.00	0.00

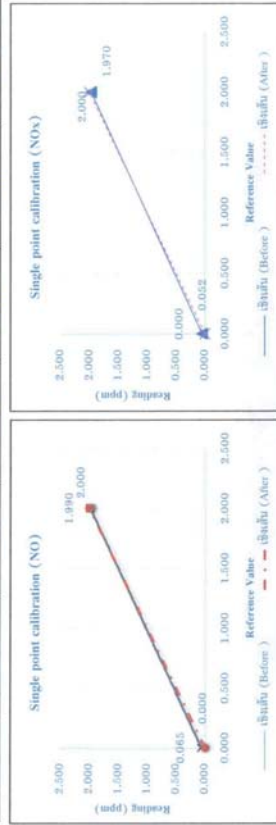

Calibrated by :
 (Mr. Yong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 1-Apr-23 Certificate No. : 0423-004 Page : 1/1

Analyzer Instruments
 Analyzer Type : NO/NO_x Analyzer
 Model : 42C
 Manufacturer : Thermo Environmental
 Serial No. : 72454-371


Environmental
 Temperature : 25.2 °C
 Humidity : 52.3 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO₂ : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
NO	0.046	0.000	0.07	1.98	2.00	-1.00
NO _x	0.037	0.000	0.06	1.99	2.00	-0.50
After						
NO	0.000	0.000	0.00	2.00	2.00	0.00
NO _x	0.000	0.000	0.00	2.00	2.00	0.00

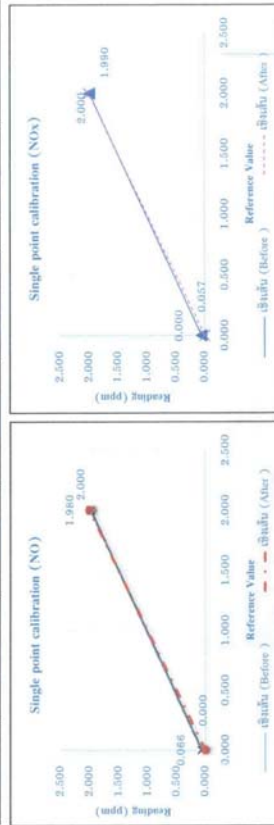

Calibrated by : *Tong*
 (Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 4-Jul-23 Certificate No. : 0723-001 Page : 1/1

Analyzer Instruments
 Analyzer Type : NO/NO_x Analyzer
 Model : 42C
 Manufacturer : Thermo Environmental
 Serial No. : 63470-339


Environmental
 Temperature : 25.1 °C
 Humidity : 40.4 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO₂ : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
NO	0.042	0.000	0.04	2.01	2.00	0.50
NO _x	0.049	0.000	0.05	2.03	2.00	1.50
After						
NO	0.000	0.000	0.00	2.00	2.00	0.00
NO _x	0.000	0.000	0.00	2.00	2.00	0.00

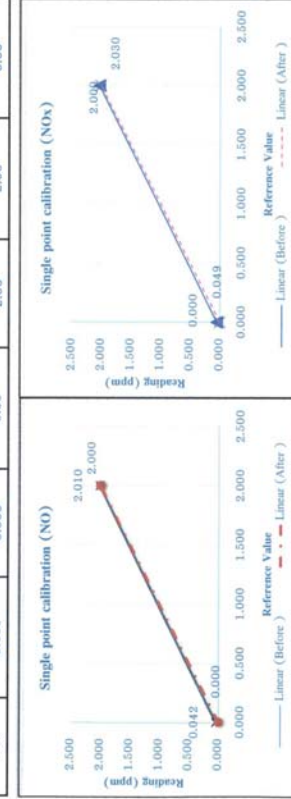

Calibrated by : *Tong*
 (Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 4-Aug-23 Certificate No. : 0823-002 Page : 1/1

Analyzer Instruments
 Analyzer Type : NO/NO/NOx Analyzer
 Model : 42C
 Manufacturer : Thermo Environmental
 Serial No. : 508011077

Environmental
 Temperature : 24.9 °C
 Humidity : 41.3 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458


Standard Gas
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 : 2 ppm
 CO Conc. : 50 ppm

Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
NO	0.081	0.000	0.06	1.99	2.00	-0.50
NOx	0.060	0.000	0.06	2.01	2.00	0.50
After						
NO	0.000	0.000	0.00	2.00	2.00	0.00
NOx	0.000	0.000	0.00	2.00	2.00	0.00

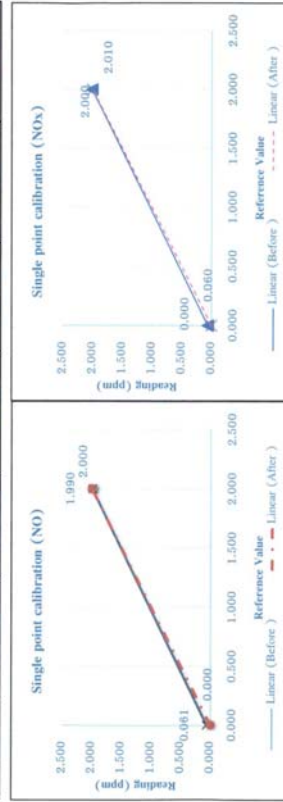

Calibrated by : *Top*
(Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 4-Aug-23 Certificate No. : 0823-003 Page : 1/1

Analyzer Instruments
 Analyzer Type : NO/NO/NOx Analyzer
 Model : 42C
 Manufacturer : Thermo Environmental
 Serial No. : 59406-323

Environmental
 Temperature : 26.3 °C
 Humidity : 42.5 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458


Standard Gas
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 : 2 ppm
 CO Conc. : 50 ppm

Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
NO	0.051	0.000	0.05	2.03	2.00	1.50
NOx	0.062	0.000	0.06	2.01	2.00	0.50
After						
NO	0.000	0.000	0.00	2.00	2.00	0.00
NOx	0.000	0.000	0.00	2.00	2.00	0.00

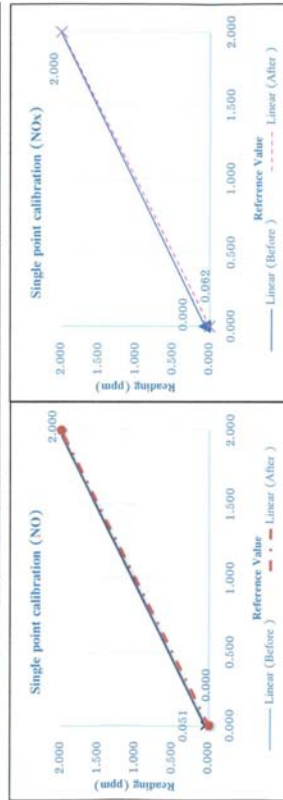

Calibrated by : *Top*
(Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 5-Aug-23 Certificate No. : 0823-001 Page : 1/1

Analyzer Instruments
 Analyzer Type : SO2 Analyzer
 Model : 43C
 Manufacturer : Thermo Environmental
 Serial No. : 43C-62201-334


Environmental
 Temperature : 25.0 °C
 Humidity : 51.9 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811438
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
SO2	0.039	0.000	0.04	1.97	2.000	-1.50
After						
SO2	0.000	0.000	0.00	2.00	2.000	0.00

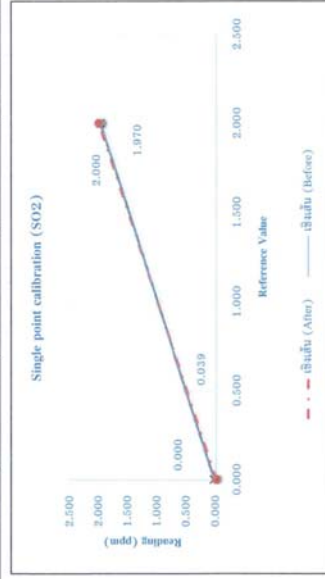

Calibrated by :  (Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 26-Aug-23 Certificate No. : 0823-002 Page : 1/1

Analyzer Instruments
 Analyzer Type : SO2 Analyzer
 Model : 43C
 Manufacturer : Thermo Environmental
 Serial No. : 43C-70853-367


Environmental
 Temperature : 25.1 °C
 Humidity : 47.9 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811438
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
Before						
SO2	0.039	0.000	0.06	1.99	2.000	-0.50
After						
SO2	0.000	0.000	0.0	2.00	2.000	0.00

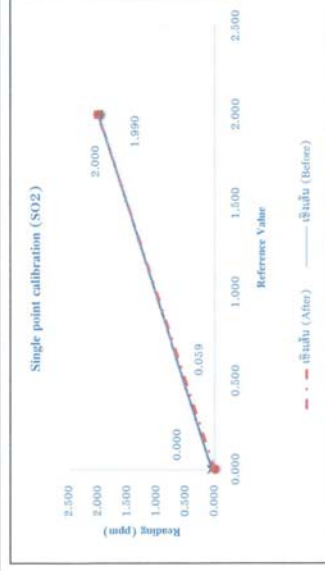

Calibrated by :  (Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 30-Sep-23 Certificate No. : 0923-006 Page : 1/1

Analyzer Instruments
 Analyzer Type : SO2 Analyzer
 Model : 43C
 Manufacturer : Thermo Environmental
 Serial No. : CTL63388-340


Environmental
 Temperature : 26.7 °C
 Humidity : 44.0 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811438
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
SO2	Before			After		
	0.065	0.060	0.07	2.01	2.000	0.50
SO2	0.000	0.000	0.00	2.00	2.000	0.00

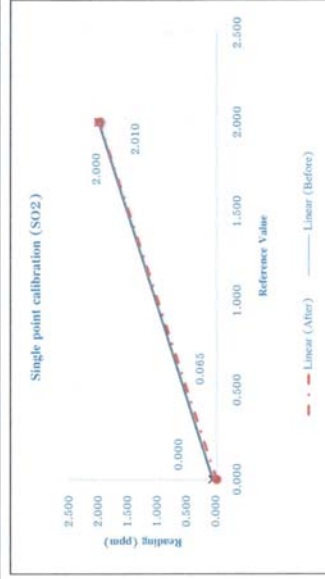

Calibrated by :

Tong

(Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 26-Aug-23 Certificate No. : 0823-003 Page : 1/1

Analyzer Instruments
 Analyzer Type : SO2 Analyzer
 Model : 43C
 Manufacturer : Thermo Environmental
 Serial No. : 43C-70852-367


Environmental
 Temperature : 24.9 °C
 Humidity : 46.9 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811438
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
SO2	Before			After		
	0.087	0.000	0.09	1.97	2.000	-1.50
SO2	0.000	0.000	0.00	2.00	2.000	0.00

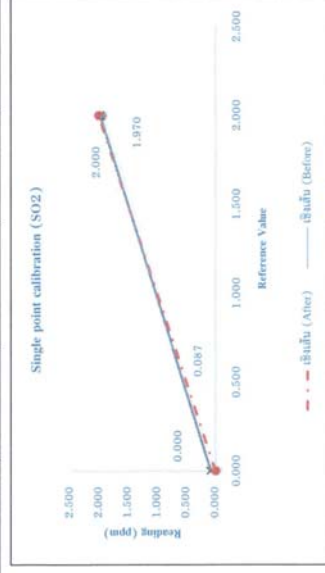

Calibrated by :

Tong

(Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 26-Aug-23 Certificate No. : 0823-004 Page : 1/1

Analyzer Instruments
 Analyzer Type : SO2 Analyzer
 Model : 43C
 Manufacturer : Thermo Environmental
 Serial No. : 43C-77419-385


Environmental
 Temperature : 25.1 °C
 Humidity : 46.2 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
SO2	Before					2.00
	0.074	0.000	0.07	2.04	2.000	
SO2	After					0.00
	0.000	0.000	0.00	2.00	2.000	

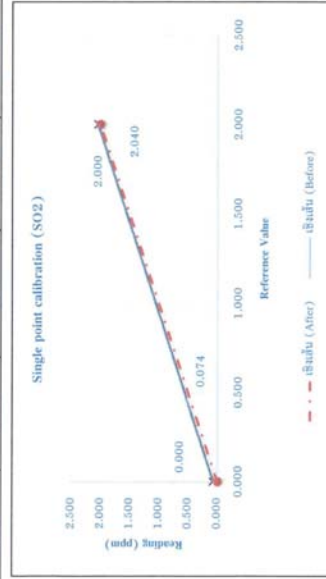

Calibrated by : *Tanvir*
(Mr. Tong Pima)

Certificate of Analyzer Performance Testing

Calibrated Date : 1-Apr-23 Certificate No. : 0423-003 Page : 1/1

Analyzer Instruments
 Analyzer Type : SO2 Analyzer
 Model : 43C
 Manufacturer : Thermo Environmental
 Serial No. : 69858-364


Environmental
 Temperature : 25.2 °C
 Humidity : 52.3 %RH

Calibration System
Calibrator Units
 Gas Calibration : Thermo Environmental
 Model : 146C
 Serial No. : 514811458
 Zero Air Generator : API
 Model : 701
 Serial No. : 179

Standard Gas
 NO Conc. : 2 ppm
 SO2 Conc. : 2 ppm
 CO Conc. : 50 ppm
 Cylinder No. : CC750227
 Expire Date : 21-Nov-23

Calibration Check

Gas	Zero			Span		
	Reading Value (ppm)	Expected Value (ppm)	Drift (%)	Reading Value (ppm)	Expected Value (ppm)	Drift (%)
SO2	Before					-1.00
	0.049	0.000	0.03	1.98	2.000	
SO2	After					0.00
	0.000	0.000	0.00	2.00	2.000	

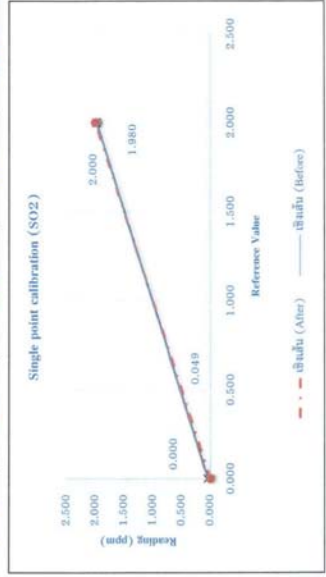

Calibrated by : *Tanvir*
(Mr. Tong Pima)



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT
975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917

Certificate No.: CP20240107EA
Operation No.: CP2024020076

Certificate of Calibration

Equipment: Vibration Meter
Manufacturer: Instantel
Model/Type: Micromate
Serial No.: UM15904
ID No.: VB-01-002
Customer: C.E.M. Technology (Thailand) Co.,Ltd.
Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,
Nakorn Phatom 73210
Received Date: 19 February 2024
Calibrated Date: 5 - 8 March 2024
Issued Date: 11 March 2024
Calibrated by: Ms. Juntaporn Kunhakom

Approved by: _____
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k)
providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except
with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

เอกสารการสอบเทียบเครื่องมือตรวจวัดความสั่นสะเทือน



Certificate No.: CP20240107EA

Calibration Report

Equipment: Vibration Meter
Manufacturer: Instantel
Model: Micromate
Serial No.: UM15904
ID No.: VB-01-002
Ambient Temperature: (23 ± 5) °C
Relative Humidity: (50 ± 15) %

Method of Calibration :-

In-house method : CC-SV004 by comparison with standard accelerometer.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument

Model	Serial No.	Cert. No.	Due Date
8305	2708237	AV-0001-23	20-Jul-2024
2525	2685967	AV-0044-23	20-Jul-2024
3050-A-060	3050-110127	CQ20230024EA	5-Nov-2024
3160-4-042	3060-106135	CQ20230025EA	5-Nov-2024
HMT331	K3810009	CD20230166EA	14-Jun-2024

Transmitter

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

- National Institute of Metrology (Thailand)

Certificate No.: CP20240107EA

Calibration Report

Result of Calibration:-

Function : Frequency response and Linearity test at 16 Hz

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	10.003	9.947	-0.056	1.50	Longitudinal (L)
5.0	10.000	10.006	9.931	-0.075	1.50	
6.3	10.000	9.996	10.175	0.179	1.50	
8.0	10.000	10.004	9.971	-0.033	1.50	
10.0	10.000	10.017	9.986	-0.031	1.50	
12.5	10.000	10.008	9.994	-0.014	1.50	
16.0	10.000	10.021	10.041	0.020	1.50	
	20.000	19.997	20.075	0.078	1.50	
	30.000	29.995	29.990	-0.005	1.50	
20.0	50.000	49.992	50.042	0.050	1.50	
	10.000	10.000	10.104	0.104	1.50	
	25.0	9.998	10.160	0.162	1.50	
31.5	10.000	10.007	10.175	0.168	1.50	
40.0	10.000	10.000	10.215	0.215	1.50	
50.0	10.000	10.003	10.396	0.393	1.50	
52.0	10.000	10.006	10.404	0.398	1.50	
63.0	10.000	10.011	10.640	0.629	1.50	
80.0	10.000	10.003	10.861	0.858	1.50	



Certificate No.: CP20240107EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	10.006	9.766	-0.240	1.50	Transverse (T)
5.0	10.000	10.006	9.805	-0.201	1.50	
6.3	10.000	10.008	10.002	-0.006	1.50	
8.0	10.000	10.015	9.844	-0.171	1.50	
10.0	10.000	10.017	9.923	-0.094	1.50	
12.5	10.000	10.014	9.860	-0.154	1.50	
16.0	10.000	10.015	9.907	-0.108	1.50	
	20.000	19.997	19.933	-0.064	1.50	
	30.000	30.010	29.880	-0.130	1.50	
	50.000	49.992	49.837	-0.155	1.50	
20.0	10.000	9.998	9.971	-0.027	1.50	
25.0	10.000	10.011	10.049	0.038	1.50	
31.5	10.000	10.017	10.104	0.087	1.50	
40.0	10.000	10.018	10.215	0.197	1.50	
50.0	10.000	9.991	10.231	0.240	1.50	
52.0	10.000	10.023	10.317	0.294	1.50	
63.0	10.000	10.006	10.538	0.532	1.50	
80.0	10.000	10.013	10.822	0.809	1.50	

Remark

1. UUC: Unit Under Calibration
2. The coverage factor $k = 2.00$

-- End of Report --

Certificate No.: CP20240107EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	9.997	9.482	-0.515	1.50	Vertical (V)
5.0	10.000	9.996	9.576	-0.420	1.50	
6.3	10.000	10.013	9.821	-0.192	1.50	
8.0	10.000	10.000	9.734	-0.266	1.50	
10.0	10.000	9.997	9.789	-0.208	1.50	
12.5	10.000	10.014	9.978	-0.036	1.50	
16.0	10.000	9.997	10.081	0.084	1.50	
	20.000	19.997	20.177	0.180	1.50	
	30.000	29.995	30.219	0.224	1.50	
	50.000	49.978	50.586	0.608	1.50	
20.0	10.000	10.001	10.207	0.206	1.50	
25.0	10.000	10.003	10.065	0.062	1.50	
31.5	10.000	10.001	10.302	0.301	1.50	
40.0	10.000	9.997	10.467	0.470	1.50	
50.0	10.000	10.001	10.664	0.663	1.50	
52.0	10.000	9.996	10.830	0.834	1.50	
63.0	10.000	10.004	10.869	0.865	1.50	
80.0	10.000	9.997	11.515	1.518	1.50	

Remark

1. UUC: Unit Under Calibration
2. The coverage factor $k = 2.00$

-- End of Report --



975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20240134EA
Operation No.: CP2024030105

Certificate of Calibration

Equipment: Vibration Meter

Manufacturer: Instantel

Model/Type: Micromate

Serial No.: UM16048

ID No.: VB-01-003

Customer: C.E.M. Technology (Thailand) Co.,Ltd.

Address: 31/8 Moo 13 T.Rai Khung, A.Sam Phran,
Nakorn Phatom 73210

Received Date: 15 March 2024

Calibrated Date: 19 - 20 March 2024

Issued Date: 21 March 2024

Calibrated by: Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.
The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20240134EA

Calibration Report

Equipment: Vibration Meter

Manufacturer: Instantel

Model: Micromate

Serial No.: UM16048

ID No.: VB-01-003

Ambient Temperature: (23 ± 5) °C

Relative Humidity: (50 ± 15) %

Method of Calibration :-

In-house method : CC-SV004 by comparison with standard accelerometer.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard Accelerometer	8305	2708237	AV-0001-23	20-Jul-2024
2) Measuring Amplifier	2525	2685967	AV-0044-23	20-Jul-2024
3) PULSE Multi-analyzer system	3050-A-060	3050-110127	CQ20230024EA	5-Nov-2024
4) PULSE Multi-analyzer system	3160-4-042	3060-106135	CQ20230025EA	5-Nov-2024
5) Humidity and Temperature Transmitter	HMT331	K3810009	CD20230166EA	14-Jun-2024

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

- National Institute of Metrology (Thailand)



Certificate No.: CP20240134EA

Calibration Report

Result of Calibration:-

Function : Frequency response and Linearity test at 16 Hz

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty \pm (%)	Direction
4.0	10.000	10.015	9.576	-0.439	1.50	Longitudinal (L)
5.0	10.000	10.000	9.679	-0.321	1.50	
6.3	10.000	9.998	9.939	-0.059	1.50	
8.0	10.000	10.008	9.805	-0.203	1.50	
10.0	10.000	10.015	9.852	-0.163	1.50	
12.5	10.000	10.001	9.884	-0.117	1.50	
16.0	10.000	10.004	9.915	-0.089	1.50	
	20.000	19.983	19.917	-0.066	1.50	
	30.000	29.995	29.927	-0.068	1.50	
	50.000	49.992	49.884	-0.108	1.50	
20.0	10.000	10.001	10.026	0.025	1.50	
25.0	10.000	10.006	10.073	0.067	1.50	
31.5	10.000	10.015	10.104	0.089	1.50	
40.0	10.000	10.000	10.168	0.168	1.50	
50.0	10.000	10.001	10.238	0.237	1.50	
52.0	10.000	10.000	10.278	0.278	1.50	
63.0	10.000	10.003	10.467	0.464	1.50	
80.0	10.000	9.998	10.617	0.619	1.50	

Certificate No.: CP20240134EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty \pm (%)	Direction
4.0	10.000	10.008	9.876	-0.132	1.50	Transverse (T)
5.0	10.000	10.006	9.971	-0.035	1.50	
6.3	10.000	10.001	10.183	0.182	1.50	
8.0	10.000	10.001	10.049	0.048	1.50	
10.0	10.000	10.001	10.041	0.040	1.50	
12.5	10.000	10.014	10.034	0.020	1.50	
16.0	10.000	10.011	10.065	0.054	1.50	
	20.000	19.997	20.138	0.141	1.50	
	30.000	30.010	30.124	0.114	1.50	
	50.000	49.992	50.234	0.242	1.50	
20.0	10.000	9.998	10.144	0.146	1.50	
25.0	10.000	10.006	10.207	0.201	1.50	
31.5	10.000	10.000	10.231	0.231	1.50	
40.0	10.000	9.999	10.302	0.303	1.50	
50.0	10.000	9.998	10.372	0.374	1.50	
52.0	10.000	9.998	10.396	0.398	1.50	
63.0	10.000	9.998	10.585	0.587	1.50	
80.0	10.000	10.007	10.908	0.901	1.50	



Certificate No.: CP20240134EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty \pm (%)	Direction
4.0	10.000	10.020	9.915	-0.105	1.50	Vertical (V)
5.0	10.000	10.021	10.057	0.036	1.50	
6.3	10.000	10.017	10.317	0.300	1.50	
8.0	10.000	10.000	10.144	0.144	1.50	
10.0	10.000	9.996	10.073	0.077	1.50	
12.5	10.000	9.998	10.160	0.162	1.50	
16.0	10.000	9.997	10.199	0.202	1.50	
	20.000	19.997	20.177	0.180	1.50	
	30.000	29.995	30.219	0.224	1.50	
20.0	50.000	49.978	50.554	0.576	1.50	
	10.000	9.998	10.137	0.139	1.50	
	10.000	10.001	10.026	0.025	1.50	
25.0	10.000	9.998	10.309	0.311	1.50	
31.5	10.000	10.000	10.428	0.428	1.50	
40.0	10.000	10.001	10.617	0.616	1.50	
50.0	10.000	9.998	10.672	0.674	1.50	
63.0	10.000	10.004	10.743	0.739	1.50	
80.0	10.000	10.013	11.098	1.085	1.50	

- Remark
1. UUC: Unit Under Calibration
 2. The coverage factor $k = 2.00$

-- End of Report --

Calibration Certificate

Part Number: 721A2601
Description: Micromate with DIN Geophone
Serial Number: UM20453
Calibration Date: April 21, 2023
Calibration Reference Equipment: SRV-AFR 714J7401
*Calibrated with Geo UM6231

Instantel certifies that the above product was calibrated in accordance with the applicable Instantel procedures. These procedures are part of a quality system that is designed to assure that the product listed above meets or exceeds Instantel specifications.

Instantel further certifies that the measurement instruments used during the calibration of this product are traceable to the National Institute of Standards and Technology; or National Research Council of Canada. Evidence of traceability is on file at Instantel and is available upon request.


The environment in which this product was calibrated is maintained within the operating specifications of the instrument.

Please note that the sensor check function is intended to check that the sensors are connected to the unit, installed in the proper orientation and sufficiently level to operate properly. This function should not be confused with a formal calibration, which requires the sensors be checked against a reference that is traceable to a known standard. Instantel recommends that products be returned to Instantel or an authorized service and calibration facility for annual calibration.

Calibrated By: 
Yaksh Patel

 309 Leggett Drive, Ottawa, Ontario K2K 3A3, (613) 592-4642

Frequency Response of UM20453 (As Found)

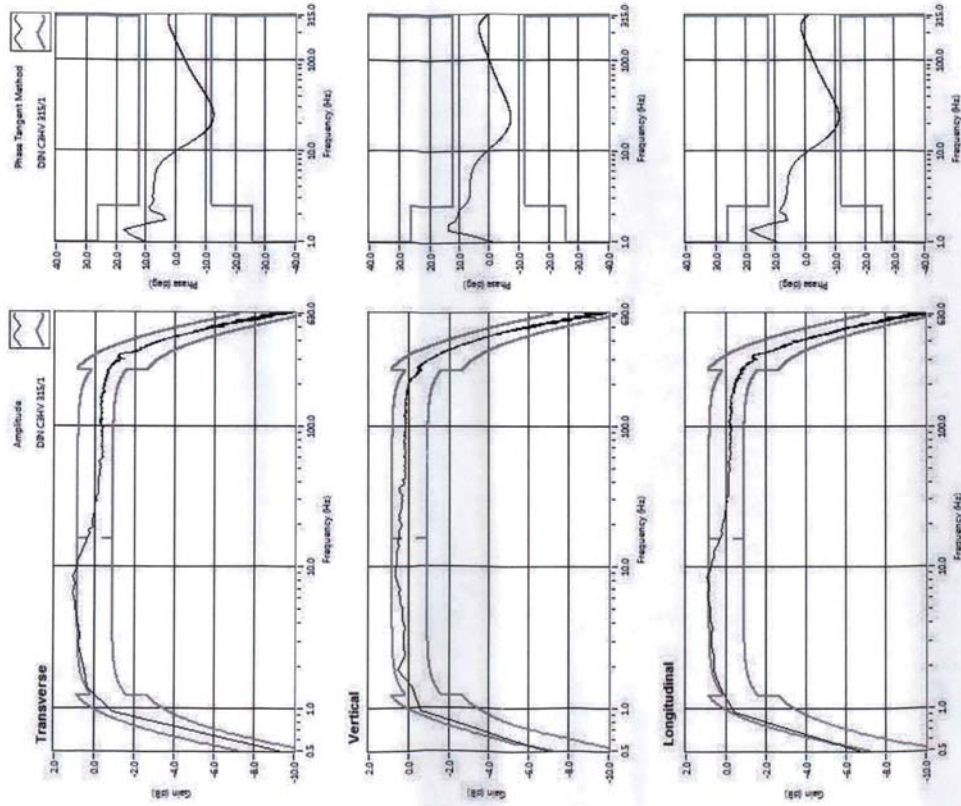

Calibration Certificate

Part Number: 721A2601
 Description: Micromate with DIN Geophone
 Serial Number: UM20454
 Calibration Date: April 21, 2023
 Calibration Reference Equipment: SRV-AFR 714J7401

Instantel certifies that the above product was calibrated in accordance with the applicable Instantel procedures. These procedures are part of a quality system that is designed to assure that the product listed above meets or exceeds Instantel specifications.

Instantel further certifies that the measurement instruments used during the calibration of this product are traceable to the National Institute of Standards and Technology, or National Research Council of Canada. Evidence of traceability is on file at Instantel and is available upon request.

The environment in which this product was calibrated is maintained within the operating specifications of the instrument.


Please note that the sensor check function is intended to check that the sensors are connected to the unit, installed in the proper orientation and sufficiently level to operate properly. This function should not be confused with a formal calibration, which requires the sensors be checked against a reference that is traceable to a known standard. Instantel recommends that products be returned to Instantel or an authorized service and calibration facility for annual calibration.

Calibrated By: Martin Hogue

Instantel
 309 Leggett Drive, Ottawa, Ontario, K2K 3A3, (613) 592-4642

Instantel

Frequency Response of UM20454 (As Found)

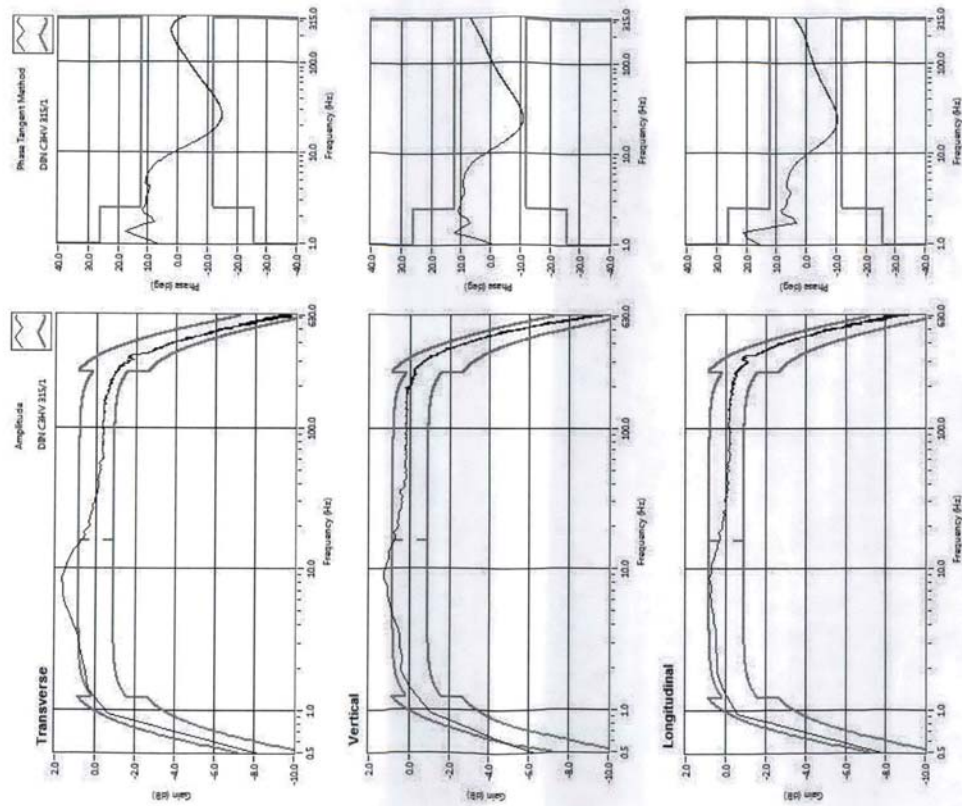

Thursday, April 20, 2023

Calibration Certificate

Part Number: 721A2601
Description: Micromate with DIN Geophone
Serial Number: UM21467
Calibration Date: MAY 29 2023
Calibration Reference Equipment: 71417403

Instantel certifies that the above product was calibrated in accordance with the applicable Instantel procedures. These procedures are part of a quality system that is designed to assure that the product listed above meets or exceeds Instantel specifications.

Instantel further certifies that the measurement instruments used during the calibration of this product are traceable to the National Institute of Standards and Technology, or National Research Council of Canada. Evidence of traceability is on file at Instantel and is available upon request.

The environment in which this product was calibrated is maintained within the operating specifications of the instrument.

Please note that the sensor check function is intended to check that the sensors are connected to the unit, installed in the proper orientation and sufficiently level to operate properly. This function should not be confused with a formal calibration, which requires the sensors be checked against a reference that is traceable to a known standard. Instantel recommends that products be returned to Instantel or an authorized service and calibration facility for annual calibration.

Calibrated By: 
Xiaoming Yang

Instantel 309 Legget Drive, Ottawa, Ontario, K2K 3A3, (613) 592-4642



Merci d'avoir choisi Instantel!

Votre engagement avec
« les moniteurs les plus fiables au monde »
vous servira pour les années à venir.

Grâce à votre achat, vous êtes à la pointe de la technologie en matière de moniteurs. Au nom de tous les collaborateurs d'Instantel, nous vous remercions d'avoir fait choisir nos produits pour la réalisation de vos projets. Les produits Instantel incluent les éléments les plus aboutis du domaine tels que:

- 1) Plus de 30 années au service des secteurs du bâtiment, d'activités minières et de géotechnologie
- 2) Des conceptions durables et résistantes
- 3) Des produits faciles à utiliser grâce à une interface intuitive
- 4) Des options étendues de conformité réglementaire
- 5) Un programme d'assistance, un service technique et une aide en ligne complets
- 6) Logiciel THOR® disponible en téléchargement gratuit sur le site Web d'Instantel: www.instantel.com
- 7) Garantie d'un an sur les pièces; si un moniteur ou un capteur est ramené à l'usine pour étalonnage jusqu'à un an après la date d'achat, la garantie sera automatiquement prolongée d'un an supplémentaire

Instantel est RESPECTUEUX DE L'ENVIRONNEMENT! Instantel n'envoie plus de manuels en version papier. Les manuels de l'opérateur pour chaque produit et pour THOR sont disponibles en téléchargement sur le site Web d'Instantel à l'adresse www.instantel.com/resources.

Nous nous engageons pour que votre satisfaction en tant que client soit la meilleure possible. En cas de questions ou de commentaires, n'hésitez pas à nous contacter. Veuillez appeler notre numéro gratuit **+1 800 267 9111** ou nous envoyer un e-mail à service@instantel.com ou sales@instantel.com.

Nous vous remercions de nouveau et avons hâte de collaborer avec vous!

© 2018 Xmark Corporation. Instantel et son logo sont des marques déposées de Stanley Black & Decker, Inc. ou de ses filiales. 720U001 R4v 05.



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT
9715 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37
Phraek Sai, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917

Certificate No.: CP20230379EA
Operation No.: CP2023100002

Certificate of Calibration

Equipment:	Vibration Meter
Manufacturer:	Instantel
Model/Type:	Micromate
Serial No.:	UM14163
ID No.:	VB-01-001
Customer:	C.E.M. Technology (Thailand) Co.,Ltd.
Address:	31/8 Moo 13 T.Rai Khung, A.Sam Phran, Nakorn Phatom 73210
Received Date:	6 October 2023
Calibrated Date:	18 - 20 October 2023
Issued Date:	31 October 2023
Calibrated by:	Ms. Juntaporn Kunhakom

Approved by: 
(Mr. Sittichai Swaksuriyavong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full, except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.



Certificate No.: CP20230379EA

Calibration Report

Equipment: Vibration Meter
Manufacturer: Instantel
Model: Micromate
Serial No.: UM14163
ID No.: VB-01-001
Ambient Temperature: (23 ± 5) °C
Relative Humidity: (50 ± 15) %

Method of Calibration :-

In-house method : CC-SV004 by comparison with standard accelerometer.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument

Model	Serial No.	Cert. No.	Due Date
8305	2708237	AV-0001-23	20-Jul-2024
2525	2685967	AV-0044-23	20-Jul-2024
3560-C	2705645	CQ20230003EA	25-Dec-2023
HMT331	K3810009	CD20230166EA	14-Jun-2024

Transmitter

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-
- National Institute of Metrology (Thailand)

Certificate No.: CP20230379EA

Calibration Report

Result of Calibration:-

Function : Frequency response and Linearity test at 16 Hz

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	10.006	10.412	0.406	1.50	Longitudinal (L)
5.0	10.000	9.984	10.254	0.270	1.50	
6.3	10.000	9.991	10.483	0.492	1.50	
8.0	10.000	10.013	10.215	0.202	1.50	
10.0	10.000	10.008	10.199	0.191	1.50	
12.5	10.000	10.000	10.104	0.104	1.50	
16.0	10.000	9.993	10.073	0.080	1.50	
	20.000	19.983	20.146	0.163	1.50	
	30.000	29.995	30.219	0.224	1.50	
20.0	50.000	49.992	50.396	0.404	1.50	
	10.000	10.006	10.112	0.106	1.50	
	25.0	10.000	10.003	0.097	1.50	
31.5	10.000	10.000	10.160	0.160	1.50	
40.0	10.000	10.008	10.302	0.294	1.50	
50.0	10.000	10.006	10.357	0.351	1.50	
52.0	10.000	9.994	10.412	0.418	1.50	
63.0	10.000	10.008	10.711	0.703	1.50	
80.0	10.000	9.984	11.097	1.113	1.50	



Certificate No.: CP20230379EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	9.997	10.372	0.375	1.50	Transverse (T)
5.0	10.000	9.991	10.325	0.334	1.50	
6.3	10.000	10.000	10.501	0.501	1.50	
8.0	10.000	10.008	10.357	0.349	1.50	
10.0	10.000	10.015	10.294	0.279	1.50	
12.5	10.000	9.997	10.231	0.234	1.50	
16.0	10.000	10.004	10.191	0.187	1.50	
	20.000	20.011	20.248	0.237	1.50	
	30.000	29.995	30.298	0.303	1.50	
20.0	50.000	49.978	50.562	0.584	1.50	
	10.000	10.001	10.144	0.143	1.50	
	10.000	9.997	10.120	0.123	1.50	
25.0	10.000	9.998	10.144	0.146	1.50	
31.5	10.000	10.013	10.246	0.233	1.50	
40.0	10.000	9.991	10.388	0.397	1.50	
50.0	10.000	10.006	10.404	0.398	1.50	
63.0	10.000	10.013	10.696	0.683	1.50	
80.0	10.000	9.991	11.098	1.107	1.50	



Certificate No.: CP20230379EA

Calibration Report

Function : Frequency response and Linearity test at 16 Hz (Cont.)

Frequency (Hz)	Nominal (mm/s)	Standard (mm/s)	UUC (mm/s)	Deviation (mm/s)	Uncertainty ± (%)	Direction
4.0	10.000	10.008	10.002	-0.006	1.50	Vertical (V)
5.0	10.000	9.991	10.136	0.145	1.50	
6.3	10.000	9.997	10.365	0.368	1.50	
8.0	10.000	10.008	10.270	0.262	1.50	
10.0	10.000	9.990	10.278	0.288	1.50	
12.5	10.000	9.997	10.238	0.241	1.50	
16.0	10.000	9.994	10.175	0.181	1.50	
	20.000	19.997	20.445	0.448	1.50	
	30.000	29.995	30.597	0.602	1.50	
20.0	50.000	49.992	51.043	1.051	1.50	
	10.000	10.003	10.231	0.228	1.50	
	10.000	9.997	9.726	-0.271	1.50	
25.0	10.000	10.000	10.057	0.057	1.50	
31.5	10.000	9.996	10.168	0.172	1.50	
40.0	10.000	9.996	10.199	0.203	1.50	
50.0	10.000	9.994	10.309	0.315	1.50	
63.0	10.000	9.984	10.396	0.412	1.50	
80.0	10.000	9.998	10.672	0.674	1.50	

Remark
1. UUC: Unit Under Calibration
2. The coverage factor $k = 2.00$

-- End of Report --

Certificate of Calibration

Certificate No. : 67-420018-1

Page : 1 of 2

Submitted by :

C.E.M Technology (Thailand) Co., Ltd.

219/43 Moo.12 Petchkasem Rd. Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

Equipment :

pH Meter with electrode

pH meter

Manufacturer :

Thermo Scientific

Model : VERSA STAR PRO

Range : N/A

pH

Resolution : 0.01

Serial No. : 12260

ID No. : WW-03-001

Electrode

Model : 9156BNWP

Serial No. : VV1-15843

ID No. : WW-03-001

Environment :

On site calibration was carried out at the Laboratory, C.E.M Technology (Thailand) Co., Ltd.

Ambient Temperature : (23.0 to 24.0)°C

Relative Humidity : (50 to 55) %

Date of Received : 10 February 2024

Date of Calibration : 10 February 2024

Date of Issue : 15 February 2024

Calibrated by :

Permpoon Chanpu

Calibration Method :

In-house method CAL-M4201 direct measurement by using standard voltage calibrator

and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	944535	27 Nov 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	944537	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	944536	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co., Ltd.



Certificate of Calibration

Certificate No. : 67-420018-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement
pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177.4	0.1	0.12
	0.0000	7	7.00	0.0	0.0	0.086
	-177.4800	10	10.00	-177.4	-0.1	0.12

Function :

pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.01	0.00	0.0097
	6.986	7.00	-0.01	0.011
	9.997	10.01	-0.01	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

- 0.00 -



Approved by :

(Surachai Promthong)
Laboratory Manager

Certificate of Calibration

Certificate No. : 67-400074-1

Page : 1 of 2

Submitted by :

C.E.M Technology (Thailand) Co.,Ltd.

219/43 Moo.12 Petchkasem Rd. Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

Equipment :

Digital Thermometer with Thermistor probe

Temperature Indicator

Manufacturer : Thermo Scientific Model : VERSA STAR PRO

Range : N/A °C Resolution : 0.1 °C

Serial No. : 12260 ID No. : WW-03-001

Thermistor probe

Model : N/A

Diameter : 6.5 mm.

Sheath Material : Stainless

Length : 120 mm.

ID No. : WW-03-001

On site calibration was carried out at the Laboratory, C.E.M Technology (Thailand) Co., Ltd.

Environment :

Ambient Temperature : (23.0 to 24.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (224.5 to 226.0) VAC

Date of Received :

10 February 2024

Date of Calibration :

10 February 2024

Date of Issue :

15 February 2024

Calibrated by :

Permpoon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003
by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No. Cert. No. Due Date Traceability

400002 TT-0074-22 20 Jun 2024

National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No. Cert. No. Due Date Traceability

400033 22E569 22 Feb 2024

National Institute of Metrology Thailand (NIMT)

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400074-1

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
120	25.002	25.0	0.0	0.19

Remarks

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

-000-




Certificate of Calibration

Certificate No. : 67-420018-3

Page : 1 of 2

Submitted by :

C.E.M Technology (Thailand) Co., Ltd.

219/43 Moo.12 Petchkasem Rd. Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

Equipment :

pH Meter with electrode

pH meter

Manufacturer : Apera

Model : PC 910

Range : N/A

pH

Resolution : 0.01

pH

Serial No. : PC910X1220811001

ID No. : WW-03-002

Electrode

Model : LabSen 211

Serial No. : 2110009213

ID No. : WW-03-002

Environment :

On site calibration was carried out at the Laboratory, C.E.M Technology (Thailand) Co., Ltd.

Ambient Temperature : (23.0 to 24.0) °C

Relative Humidity : (50 to 55) %

Date of Received : 10 February 2024

Date of Calibration : 10 February 2024

Date of Issue : 15 February 2024

Calibrated by : Permpon Chantpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator

and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	944535	27 Nov 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	944537	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	944536	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Surchai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-420018-3

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement
pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	4.00	177	0	0.59
	0.0000	7	7.00	0	0	0.58
	-177.4800	10	10.00	-178	1	0.59

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading		Correction (pH)	Uncertainty (± pH)
		(pH)	(pH)		
4, 7, 10	4.008	4.00	0.00	0.00	0.010
	6.986	7.00	-0.01	0.011	0.011
	9.997	10.01	-0.01	0.014	0.014

Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- 0(0)0 -

P.P.

Approved by :

(Surachai Promthong)

Laboratory Manager



Certificate of Calibration

Certificate No. : 67-400074-2

Page : 1 of 2

Submitted by :

C.E.M Technology (Thailand) Co.,Ltd.

21943 Moo.12 Petchkasem Rd. Omnoi, Krathumban, Samutsakorn 74130 (Head Office)

Equipment : Digital Thermometer with Thermistor probe

Temperature Indicator

Manufacturer : Apera Model : PC 910

Range : N/A °C Resolution : 0.1 °C

Serial No. : PC910X1220811001 ID No. : WW-03-002

Thermistor probe

Model : N/A

Diameter : 4.8 mm.

Serial No. : N/A ID No. : WW-03-002

Environment :

On site calibration was carried out at the Laboratory, C.E.M Technology (Thailand) Co., Ltd.

Ambient Temperature : (23.0 to 24.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (224.5 to 226.0) VAC

Date of Received : 10 February 2024

Date of Calibration : 10 February 2024

Date of Issue : 15 February 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method comparison technique CAL-M4003 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

ID No. Cert.No. Due Date Traceability

400002 TT-0074-22 20 Jun 2024 National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

ID No. Cert.No. Due Date Traceability

400033 22E569 22 Feb 2024 National Institute of Metrology Thailand (NIMT)

P.P.

Approved by :

(Surachai Promthong)

Laboratory Manager



The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

Certificate of Calibration

Certificate No. : 67-400074-2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

Immersion Depth (mm.)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
100	25.005	25.1	-0.1	0.19


Remarks

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o O o -

Certificate of Calibration

Equipment: Cooled Incubator
Model: KB 240
Serial No.(or ID): 20180000012164(VWV-16-001)
Manufacturer:
Condition: In Condition
Shelves(pc.): 3

Certificate No.: C31240373
Issued Date: 16 February 2024
Job No.: WO-00017098
Page: 1 of 3
Ventilation Valve: None

Customer: C.E.M Technology (Thailand) Co., Ltd.
 31/8 Moo 13, Tambom Raikhing,
 Amphur Sampran, Nakhonpathom 73210 Thailand.

Environment Condition: Temperature: 24 °C ± 1.1 °C
 Humidity: 63 %RH ± 5.9 %RH
 Voltage: 229 VAC ± 1.2 VAC

Calibration Place: C.E.M Technology (Thailand) Co., Ltd. (Laboratory Room)
 219/43 Moo 12 Petchkasam Road,
 Omnoi Krathum Baen, Samut Sakthon 74130 Thailand

Calibration By: Mr. Ampol Srisumphan

Calibration Date: 14 February 2024

The Method used: In house method, CAL-WI-16, base on TLAS-G20
Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
 Certificate No. C10240001



(Mr. Ampol Srisumphan)

Person in charge



(Mr. Udon Srichana)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national laboratories.
 The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
 These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อีเซีย จำกัด
 DKSH Technology Limited
 2533 คู่มือ/ที่แจ้งการตรวจวัด : 10220
 2533 คู่มือ/ที่แจ้งการตรวจวัด : 10220
 Phone : +66 2639 7000 Email : info.calibration@dksh.com Website : www.dksh.com/scientific-thailand

Delivering Growth - In Asia and Beyond.

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate:

The correction of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, TLAS-G20. Therefore, those parameters have not been assessed separately.

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk < 50% PFA.
☒ Choice B Non-binary statement with guard band ($w = 1$ U), Pass or Fail Specific Risk < 2.5% PFA and Condition Pass or Condition Fail Specific Risk < 50% PFA.
☐ Choice C Customer defined. Customers may define arbitrary multiple of r to have applied as guard band ($w = r$ U).
: PFA – Probability of False Accept


(Mr. Udon Srichana)
Authorized signatory

Without adjustment

Desired Temperature : 20.0 °C Tolerances : 1.0 °C


Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 20.0 °C

Locations	Measured (°C)	Correction* (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	20.17	0.17	0.49	1.0	Pass
#2	20.13	0.13	0.49	1.0	Pass
#3	19.99	-0.01	0.56	1.0	Pass
#4	19.98	-0.02	0.60	1.0	Pass
#5	20.21	0.21	0.51	1.0	Pass
#6	20.17	0.17	0.46	1.0	Pass
#7	19.97	-0.03	0.57	1.0	Pass
#8	20.07	0.07	0.47	1.0	Pass
#9	20.13	0.13	0.43	1.0	Pass

Correction* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use

The End of Statements of Conformity

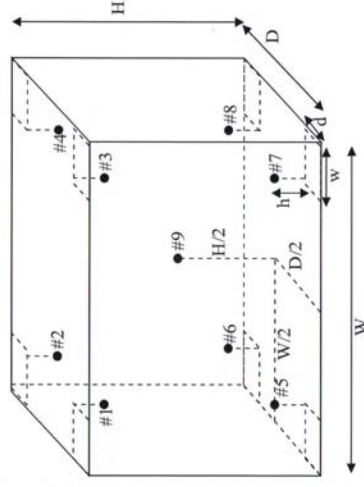

Standard Installation Locations

Volume (Calibration Zone) = 122 (Liters)

Inside chamber: W = 65 (cm) D = 50 (cm) H = 76 (cm)

Standard Locations (#1, #2, #3, #4): w = 7 (cm) h = 8 (cm)

Standard Locations (#5, #6, #7, #8): w = 7 (cm) h = 8 (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	101	102	103	104	105	106	107	108	109

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.



Calibration Results:
Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 20.0 °C

Locations	Measured Temperature (°C)	Correction of UUC, (°C)	Uncertainty (± °C)
#1	20.17	0.17	0.49
#2	20.13	0.13	0.49
#3	19.99	-0.01	0.56
#4	19.98	-0.02	0.60
#5	20.21	0.21	0.51
#6	20.17	0.17	0.46
#7	19.97	-0.03	0.57
#8	20.07	0.07	0.47
#9	20.13	0.13	0.43

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
20.0	20.0	20.0	20.17	20.13	19.99	19.98	20.21	20.17	19.97	20.07	20.13	0.60


Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
20.0	0.47	0.48	1.13


Note: * Maximum uncertainty of the each position

The End of Certificate

Corr_Distribution & Max_Measurement Uncertainty
Job_No. WO-00017098
Without adjustment

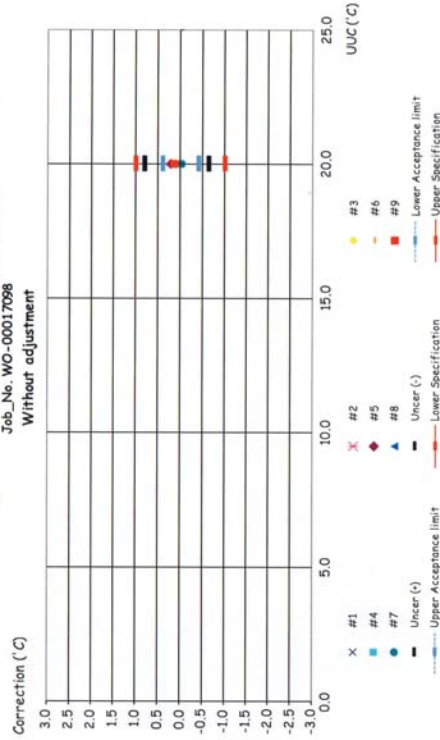

Temperature Distribution @ 20.0 °C
Job_No. WO-00017098
Without adjustment

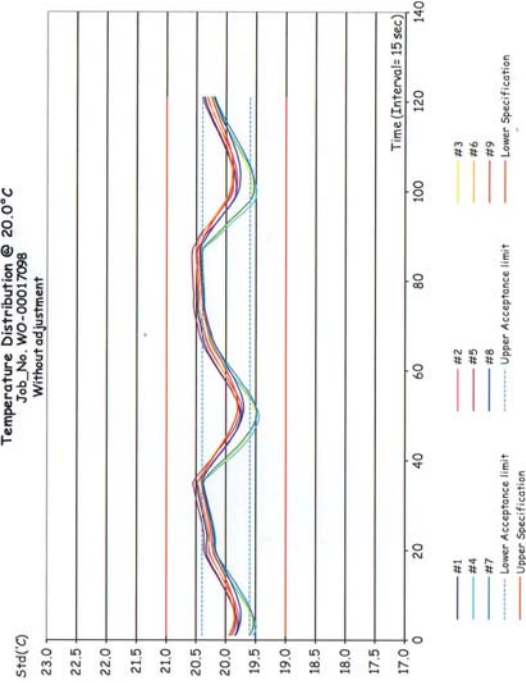



ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: WO-00017098

ชนิดเครื่อง: Cooled Incubator

ยี่ห้อ: KB 240

หมายเลขเครื่อง: 2018000012164(WW-16-001)

ตรวจสอบ (เป็น)		รายการ (เป็น)	ผลการตรวจสอบ (เป็น)	หมายเหตุ
14 Feb 2024	14 Feb 2024			
ปกติ	ไม่ปกติ	General	ปกติ	ไม่ปกติ
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ส่วน	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. การแสดง Display	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. การทำงาน พัดลม	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	6. การทำงาน Lever of Ventilation valve	<input type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. การทำงาน Lever door open / close	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. การทำงาน Door seal	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. การทำงานระบบความปลอดภัย Safety	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. การทำงานระบบแจ้งเตือนความเย็น	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	11. การทำงานระบบแจ้งเตือนความร้อน	<input type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. การทำงานระบบแจ้งเตือนเสียง	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	13. การทำงานระบบแจ้งเตือนเสียง	<input checked="" type="checkbox"/>	<input type="checkbox"/>

ผู้ตรวจ:

Mr. Ampol Srisumphan
Service Engineer

บริษัท ดีเคเอส อี.พี.
DKSH Technology Limited
2533 ถนนสุขุมวิท กรุงเทพมหานคร 10260
โทรศัพท์: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/certificate-thailand

Delivering Growth - in Asia and Beyond.



Certificate of Calibration

Equipment: Hot Air Oven
Model: UF 55
Serial No.(or ID): B219.0142 (WW-05-002)
Manufacturer: Memmert
Condition: In Condition
Shelves(pc.): 2
Certificate No.: C31240372
Issued Date: 15 February 2024
Job No.: WO-00017098
Page: 1 of 5
Ventilation Valve: Closed

Customer: C.E.M Technology (Thailand) Co., Ltd.
31/8 Moo 13, Tamborn Raikhing,
Amphur Sampran, Nakhonpathom 73210 Thailand.

Environment Condition: Temperature: 29 °C ± 0.6 °C
Humidity: 61 %RH ± 5.3 %RH
Voltage: 230 VAC ± 1.5 VAC

Calibration Place: C.E.M Technology (Thailand) Co., Ltd. (Laboratory Room)
219/43 Moo 12 Petchkasam Road,
Omnoi Krathum Baen, Samut Sakhon 74130 Thailand

Calibration By: Mr. Ampol Srisumphan
Calibration Date: 14 February 2024

The Method used: In house method, CAL-WI-16, base on TLAS-G20
Traceability: This certificate is traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through DKSH Technology Limited.
Certificate No. C10240001

Signature of the Engineer
(Mr. Ampol Srisumphan)

Signature of the Customer
(Mr. Udon Srichana)

Person in charge


Authorized signatory

This certificate is issued in the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national laboratories.
The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).
These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอส อี.พี.
DKSH Technology Limited
2533 ถนนสุขุมวิท กรุงเทพมหานคร 10260
โทรศัพท์: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/certificate-thailand

Delivering Growth - in Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022

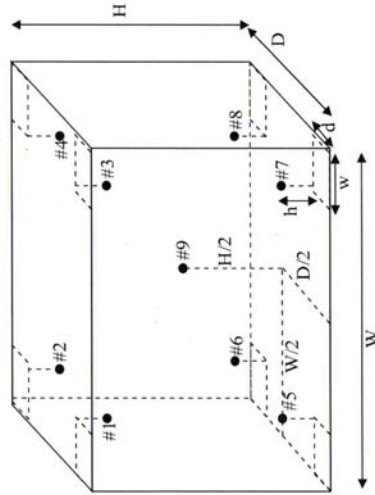

Standard Installation Locations

Volume (Calibration Zone) = 21 (Liters)

Inside chamber:

W = 40 (cm) D = 33 (cm) H = 40 (cm)

Standard Locations (#1, #2, #3, #4):

w = 5 (cm) d = 5 (cm) h = 5 (cm)

Standard Locations (#5, #6, #7, #8):

w = 5 (cm) d = 5 (cm) h = 5 (cm)

#9: Geometric center of the chamber

Position of Std	#1	#2	#3	#4	#5	#6	#7	#8	#9
Channel of Logger	201	202	203	204	205	206	207	208	209

Definitions

Indicating Temperature: The average reading of indicating device which forms the integral part of the enclosure.

Measured Temperature: The average reading of standards at any positions or location.

Measured Uniformity: The maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time or at close observation time as possible to determine the temperature pattern or homogeneity with the chamber at steady-state. The reference probe is preferably located in the geometric center of the chamber.

Measured Stability: The one-half of greatest maximum difference of measured temperatures at any one probe.

Overall Variation: The difference of maximum and minimum measured temperatures throughout observation time.

Calibration Results: Without adjustment

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 104.0 °C

Locations	Measured Temperature (°C)	Correction of UUC (°C)	Uncertainty (± °C)
#1	104.38	0.38	0.39
#2	104.15	0.15	0.39
#3	104.39	0.39	0.39
#4	104.26	0.26	0.39
#5	103.88	-0.12	0.39
#6	104.13	0.13	0.39
#7	104.47	0.47	0.39
#8	104.41	0.41	0.39
#9	104.65	0.65	0.39

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
			#1	#2	#3	#4	#5	#6	#7	#8	#9	
104.0	104.0	104.0	104.38	104.15	104.39	104.26	103.88	104.13	104.47	104.41	104.65	0.39

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
104.0	0.83	0.12	0.96

Note: * Maximum uncertainty of the each position



Without adjustment (Cont.)

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 180.0 °C

Locations	Measured Temperature (°C)	Correction of UUC (°C)	Uncertainty (± °C)
#1	180.34	0.34	0.56
#2	179.98	-0.02	0.56
#3	180.46	0.46	0.56
#4	180.34	0.34	0.56
#5	180.63	0.63	0.56
#6	180.33	0.33	0.56
#7	179.22	-0.78	0.56
#8	179.80	-0.20	0.56
#9	180.74	0.74	0.56

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
180.0	180.0	180.0	#1	#2	#3	#4	#5	#6	#7	#8	#9	0.56
			180.34	179.98	180.46	180.34	180.63	180.33	179.22	179.80	180.74	

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
180.0	1.59	0.08	1.66

Note: * Maximum uncertainty of the each position

The End of Certificate



Without adjustment (Cont.)

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 110.0 °C

Locations	Measured Temperature (°C)	Correction of UUC (°C)	Uncertainty (± °C)
#1	110.40	0.40	0.46
#2	110.15	0.15	0.46
#3	110.45	0.45	0.46
#4	110.37	0.37	0.46
#5	110.42	0.42	0.46
#6	110.29	0.29	0.46
#7	109.86	-0.14	0.46
#8	110.12	0.12	0.46
#9	110.51	0.51	0.46

Temperature Distribution

Desired (°C)	Setting (°C)	Indicating (°C)	Measured Temperature at Spread Locations (°C)									Uncertainty (± °C)*
110.0	110.0	110.0	#1	#2	#3	#4	#5	#6	#7	#8	#9	0.46
			110.40	110.15	110.45	110.37	110.42	110.29	109.86	110.12	110.51	

Chamber Characterization

Indicating (°C)	Measured Uniformity (°C)	Measured Stability (± °C)	Overall Variation (°C)
110.0	0.71	0.11	0.86

Note: * Maximum uncertainty of the each position



Refer to Certificate No.: C31240372 Page: 1 of 2

Statements of conformity:

This conformity certificate documents the validity of the following statements of conformity based on the measurement results of corresponding calibration certificate.

The correction of indication determined during calibration are under given measurement and environmental conditions and considering the expanded measurement uncertainty (coverage probability 95%) within the specification. The given measurement uncertainty already includes other all effects by according to the standard method, TLAS-G20. Therefore, those parameters have not been assessed separately.

Tolerance and Decision rules:

Assessment of the conformity of the measurement device are done based on direct comparison of the relevant measurement results with the tolerances and decision rule are prescribed by the customer.

- Decision rule :** ☐ Choice A Binary Statement for Simple Acceptance Rule ($w = 0$), Specific Risk < 50% PFA.
- ☒ Choice B Non-binary statement with guard band ($w = 1$ U), Pass or Fail Specific Risk < 2.5% PFA and Condition Pass or Condition Fail Specific Risk < 50% PFA.
- ☐ Choice C Customer defined. Customers may define arbitrary multiple of r to have applied as guard band ($w = r$ U).
- : PFA – Probability of False Accept


(Mr. Udon Srichana)
Authorized signatory

Without adjustment

Desired Temperature : 104.0 °C Tolerances : 1.0 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 104.0 °C

Locations	Measured (°C)	Correction* (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	104.38	0.38	0.39	1.0	Pass
#2	104.15	0.15	0.39	1.0	Pass
#3	104.39	0.39	0.39	1.0	Pass
#4	104.26	0.26	0.39	1.0	Pass
#5	103.88	-0.12	0.39	1.0	Pass
#6	104.13	0.13	0.39	1.0	Pass
#7	104.47	0.47	0.39	1.0	Pass
#8	104.41	0.41	0.39	1.0	Pass
#9	104.65	0.65	0.39	1.0	Condition Pass

Correction* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Prachinok, Bangkok 10260
Phone: +66 2539 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - In Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022



Refer to Certificate No.: C31240372 Page: 2 of 2

Statements of conformity:(Cont.)

Without adjustment (Cont.)

Desired Temperature : 110.0 °C Tolerances : 5.0 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 110.0 °C

Locations	Measured (°C)	Correction* (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	110.40	0.40	0.46	5.0	Pass
#2	110.15	0.15	0.46	5.0	Pass
#3	110.45	0.45	0.46	5.0	Pass
#4	110.37	0.37	0.46	5.0	Pass
#5	110.42	0.42	0.46	5.0	Pass
#6	110.29	0.29	0.46	5.0	Pass
#7	109.86	-0.14	0.46	5.0	Pass
#8	110.12	0.12	0.46	5.0	Pass
#9	110.51	0.51	0.46	5.0	Pass

Correction* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use

Without adjustment

Desired Temperature : 180.0 °C Tolerances : 2.0 °C

Measurement Temperature at Spread Locations, Indicating of Unit Under Calibration: 180.0 °C

Locations	Measured (°C)	Correction* (°C)	Guard band (W) (± °C)	Tolerance (± °C)	Conformity
#1	180.34	0.34	0.56	2.0	Pass
#2	179.98	-0.02	0.56	2.0	Pass
#3	180.46	0.46	0.56	2.0	Pass
#4	180.34	0.34	0.56	2.0	Pass
#5	180.63	0.63	0.56	2.0	Pass
#6	180.33	0.33	0.56	2.0	Pass
#7	179.22	-0.78	0.56	2.0	Pass
#8	179.80	-0.20	0.56	2.0	Pass
#9	180.74	0.74	0.56	2.0	Pass

Correction* = Measured Temperature - Desired Temperature

The validity of the statements of conformity cannot be guaranteed for different places of use, environmental conditions or improper use


The End of Statements of Conformity

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Prachinok, Bangkok 10260
Phone: +66 2539 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand


Delivering Growth - In Asia and Beyond.

CAL-FM-C31-10: 12 Sep 2022


Corr_Distribution & Max_Measurement Uncertainty
Job_No. WO-00017098
Without adjustment

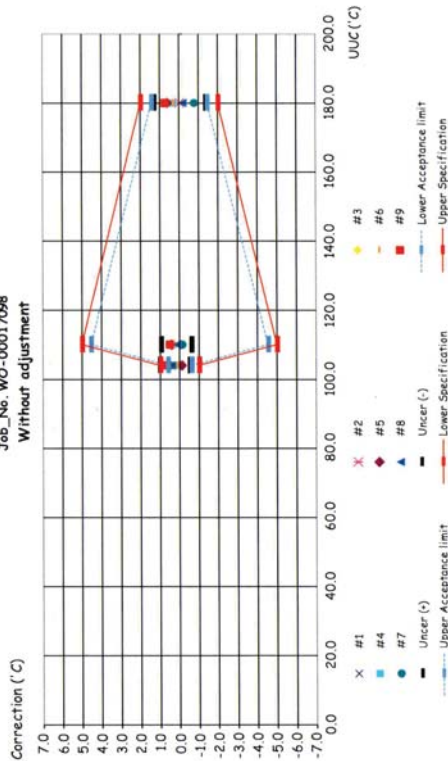


Temperature Distribution @ 110.0°C
Job_No. WO-00017098
Without adjustment (Cont.)

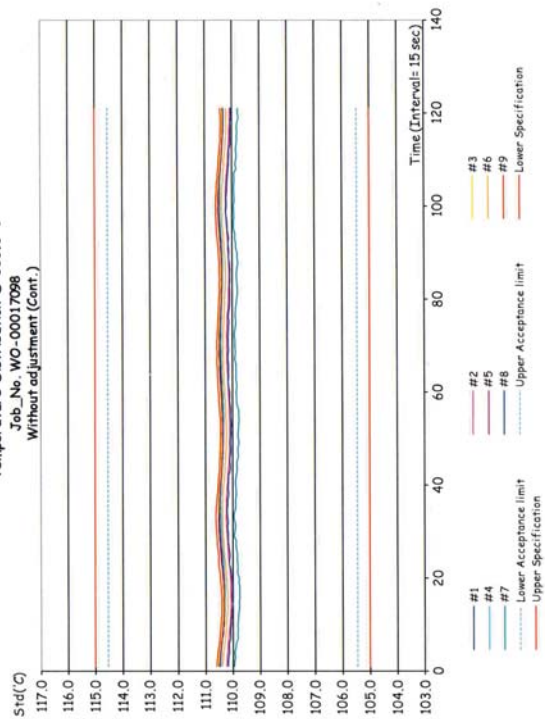

Temperature Distribution @ 104.0°C
Job_No. WO-00017098
Without adjustment

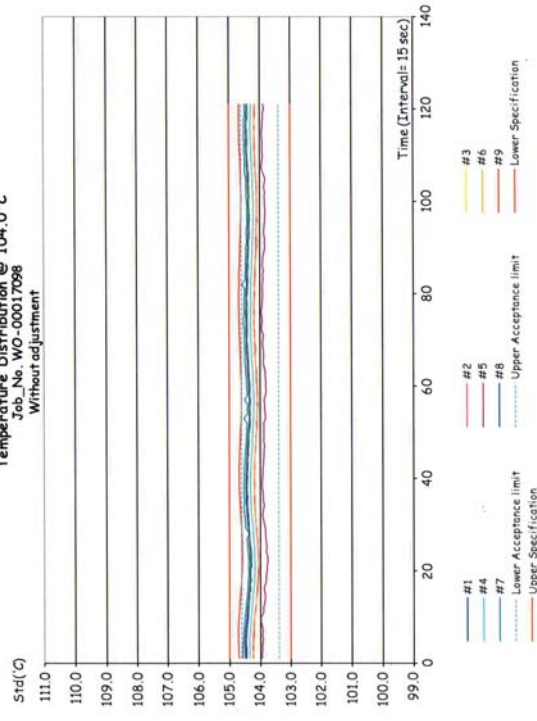

Temperature Distribution @ 180.0°C
Job_No. WO-00017098
Without adjustment (Cont.)

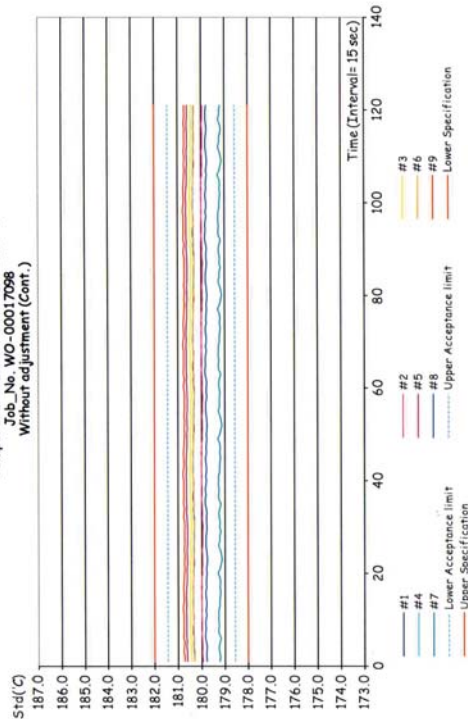



ใบตรวจสอบสภาพเครื่องควบคุมอุณหภูมิ

เลขที่ใบงาน: WO-00017098

ชนิดเครื่อง: Hot Air Oven

หมายเลขเครื่อง: B219.0142 (WW-05-002)

รุ่น: UF-55

รายการ (It.)	รายการตรวจสอบ		รายการ (It.)		หมายเหตุ
	14 Feb 2024	14 Feb 2024	14 Feb 2024	14 Feb 2024	
1. ส่วนใด	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	2. การทำงาน Main Switch	<input checked="" type="checkbox"/>	
2. การทำงาน Selector Key	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	3. การทำงาน Display	<input checked="" type="checkbox"/>	
3. การทำงาน Filter	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	4. การทำงาน Lever of Ventilation valve	<input checked="" type="checkbox"/>	
4. การทำงาน Door seal	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	5. การทำงาน Lever door open / close	<input checked="" type="checkbox"/>	
5. การทำงาน Safety	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	6. การทำงาน Door seal	<input checked="" type="checkbox"/>	
6. การทำงาน Safety	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	7. การทำงาน Safety	<input checked="" type="checkbox"/>	
7. การทำงาน Safety	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	8. การทำงาน Safety	<input checked="" type="checkbox"/>	
8. การทำงาน Safety	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	9. การทำงาน Safety	<input checked="" type="checkbox"/>	
9. การทำงาน Safety	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	10. การทำงาน Safety	<input checked="" type="checkbox"/>	
10. การทำงาน Safety	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	11. การทำงาน Safety	<input checked="" type="checkbox"/>	
11. การทำงาน Safety	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	12. การทำงาน Safety	<input checked="" type="checkbox"/>	
12. การทำงาน Safety	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	13. การทำงาน Safety	<input checked="" type="checkbox"/>	

ผู้ตรวจ:

Mr. Ampol Srisumphan
Service Engineer

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 หมู่ 10 ตำบลบางนาเหนือ เขตภาษีเจริญ กรุงเทพมหานคร 10260
Phone: +66 2639 7005 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.



Harikul Science Co., Ltd.
694 Soi Ratchaditwit 24, Pracharatbampien,
Samsenok, Hualkhwang, Bangkok 10310
Tel: 0-274-2456 Fax: 0-274-2443
Email: info@harikul.com www.harikul.com

CERT. No.: HS-U059H

Certificate of Calibration

Calibration Date : 28 Aug 23

Submitted by : C.E.M TECHNOLOGY (THAILAND) Co., LTD.
219/43 Moo 12, Peichkasem Road, Omnoi, Krathumban,
Samutsakom 74130

Model : YSI 5000

S/N : 18L109487

Probe : YSI 5010

S/N : 22G100123

ID NO. :

Air Temp ref : S/N. F8065C26

Barometric ref : S/N. F8065C26

Water Temp ref : S/N. 11430

Technician : Kittipong M.

Avg Room Temp : 20 °C

Avg Water Temp : 20 °C

Air Pressure : 760.00 mmHg

Salinity : 0 ppt

Calibration Details

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.08	(PASS)	-
Measurement 2 (mg/l)	9.08	(PASS)	-
Measurement 3 (mg/l)	9.08	(PASS)	-
Measurement 4 (mg/l)	9.08	(PASS)	-
Measurement 5 (mg/l)	9.08	(PASS)	-
Measurement 6 (mg/l)	9.08	(PASS)	-
Measurement 7 (mg/l)	9.08	(PASS)	-
Measurement 8 (mg/l)	9.08	(PASS)	-
Measurement 9 (mg/l)	9.09	(PASS)	-
Measurement 10 (mg/l)	9.09	(PASS)	-

Mean Measurement : 9.08 mg/l

Inaccuracy : 0.01 mg/l

Overall Status : (PASS)

Manufacturer Specification

Accuracy = +/- 0.02 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.

Technician Signature
(Kittipong Maekwong)

Supreecha Su
Laboratory Manager
(Supreecha Sumritam)



Avio200 Preventive Maintenance Report

Company Name: CEM TECHNOLOGY
Instrument Location: 219/43 Krathum Baen District
Samut Sakhon 74130
Instrument Serial No.: M79S2103051
Date: 02-Aug-2023

ICP-OES/Avio200 Preventive Maintenance (PM)					
Company Name:		CEM TECHNOLOGY.			
Address (Instrument Location):		219/43 Krathum Baen District Samut Sakhon 74130			
Serial Number:		M7952103051	PM Number:		4 of 4 Warranty
Customer Name (if applicable):		K. Wichuda	Telephone Number:		086 905 4664
Service Engineer Name:		K. Chayanan	Service Order Number:		WO-02409475
Date PM Performed: (DD-MM-YYYY)		02-Aug-2023	Next PM Due Date: (DD-MM-YYYY)		02-Feb-2024
Standard Labor Hours to Complete PM :					4 hours

Part Number	Release	Publication Date
09370140 Rev.5	B	January 2018



Scope

The purpose of this PM is to ensure the continued functionality of the PerkinElmer/Avio200 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM. Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files. The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer. Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes
Avio200	M7952103051	Syngistix V 5.1.0.0293
523 Autosampler	0121106523	

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
09995098	Air Filter-Spectrometer	Not Applicable
N077520	Air Filter-RF Generator	Not Applicable
09992731	Axial Window	Not Applicable
B0810377	Radial Window	Not Applicable
N0770438	O-ring kit, injector support adapter	Not Applicable
N0780437	O-ring kit, torch	Not Applicable

Additional Reagents and Standards Required for PM			
Part Number (if applicable)	Description	Quantity	Batch/Lot # Expiration Date: (MM/YY)
N0691579	Multi-Element Standard (N069-1579 diluted 10X)	1	57-024CRX1 Oct-2024
N9300221	Instrument Calibration-4 (N9300221 diluted 100X)	1	54-134CRY1 Jun-2024

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ✓ Ask customer about unit's performance since last visit.
- ✓ Check incoming AC line voltage under load for proper levels and grounding.
- ✓ Is the instrument operational?

2. Mechanical:

- ✓ Inspect and clean all fans and filters.
- ✓ Inspect and replace torch components and necessary.
Torch Components Replaced: ☐Yes ☒No
If yes, list components replaced:
- ✓ Inspect all tubing for signs of cracking or leaking and replace as necessary.
Tubing Replaced: ☒Yes ☐No
If yes, list tubing replaced:
- ✓ Inspect the peristaltic pump for proper operation.
- ✓ Check and adjust if necessary, the external nitrogen, argon shear gas and water supply pressures.
- ✓ Check and adjust if necessary, the internal nitrogen, main argon, torch argon and shear gas pressures

Regulator	Measured Pressure	Set Pressure
Nitrogen	N/A	NA (calibrated in Factory)
Main Argon	76	76psig
Torch Argon	67	67psig
Shear Gas	65	65psig
Water	35	35psi

- ✓ Check the shear gas nozzle for blockages and proper, uniform flow.
- ✓ Inspect nitrogen Hi/Low purge and shear gas solenoids for proper function.
- ✓ Inspect the function of all spectrometer motors. Drive the motors from the Spectrometer DCM. Check all motors, couplings, set screws, gears or drive assembly located on the spectrometer (prism/grating wavelength drives, slits, shutter, DV mirror, XY mirror) if problems are found.
- ✓ Perform preventative maintenance on the chiller as required. Make the customer aware of the importance of maintaining the chiller fluid level and filter replacement.
- ✓ Drain air compressor surge tank.
- ✓ Clean exterior of instrument.

3. Electrical:

- ☒ Visually inspect all PC boards for cleanliness and signs of corrosion.
- ☒ Check all RF generator and spectrometer power supply voltages.
- ☒ Run instrument diagnostic checks from the appropriate Device Control Module.

RF Generator:

- ☒ Check the RF generator status screens.
- ☒ Check the function of all interlocks.

Spectrometer:

- ☒ Check the spectrometer status screens.
- ☒ Check for proper function of all motors from the Motor Control window.

4. Optical:

- ☒ Check the neon lamp for proper operation.
- ☒ Ensure that neon initialization passes at power up.
- ☒ Ensure that there is a single, well defined peak of sufficient intensity (approximately 15,000 to 60,000 cts.) for the 703.241nm neon line viewed in the DCM Collect Spectra window. Re-generate the neon correction table if problems are encountered. If problems are still exhibited after the table is re-generated, replace the neon lamp assembly.

Neon Lamp Replaced: ☐ Yes ☒ No

- ☒ Perform the Initialize Optics routine from the Spectrometer Control window.
- ☒ Ensure that the routine passes with no error codes. If it fails, run a manual prism scan from the spectrometer DCM.
- ☒ Insure the Dark Current measurement (Detector Calibration) passes at initialization.
- ☒ Check the shutter home sensor position.
- ☒ Check prism/electronics temperature sensor readback values from the DCM. It is normal for these readings to be shown in red. A typical prism temperature is approximately 29.5 degree C. A typical electronics temperature is approximately 35 degree C.
- ☒ Check the detector temperature from the DCM for -7.0 to -8.5 degree C. If outside of this range the detector cooling fan may not be operational. Further inspection may be necessary.
- ☒ Inspect for proper function of the transfer optics. 1) shutter 2) DV mirror 3) X/Y mirror.
- ☒ Clean or replace the axial and radial view windows as necessary.

Axial Window Replaced: ☒ Yes ☐ No
Radial Window Replaced: ☒ Yes ☐ No

5. Post PM Performance Tests:

- ☒ Perform View Align.

5.1 Spectral Resolution:

- ☒ Measure the spectrometers ability to separate two adjacent wavelengths.

Parameter	Specification	Test Result	Pass/Fail
As 193.696 - Resolution	≤0.009	0.007	Passed
Ni 231.604 - Resolution	≤0.011	0.009	Passed
Ni 341.476 - Resolution	≤0.015	0.013	Passed
Ba 455.403 - Resolution	≤0.020	0.017	Passed

5.2 Precision:

- ☒ Test for reproducibility of a set of measurement.

Parameter	Specification	Test Result	Pass/Fail
Zn 213.856	%RSD ≤ 1 %	0.46	Passed
Mg 280.856	%RSD ≤ 1 %	0.25	Passed
Mg 285.207	%RSD ≤ 1 %	0.22	Passed
Ba 455.403	%RSD ≤ 1 %	0.15	Passed

5.3 Mn BEC:

- ☒ Run Axial and Radial BEC according to the A&T spec, or the commissioning test procedure.

Mn Background Equivalent Concentration:

Method "MnBEC" For Samples "IB (2% HNO_3)" and "IS (N069-1579/10)", record intensities.

Calculated BEC: $\text{BEC} = (\text{IB} * \text{Conc of Std}) / (\text{IS} - \text{IB})$. Where Conc of Std = 1,000 PPB

Element	Mode	Conc.	IB	IS
Mn 257.610	Radial	1,000 ppb	66993.5	1909809.2
Mn 257.610	Axial	1,000 ppb	152396.8	10817525.8
Mn 257.610	IB* Conc.	IS - IB	BEC	Spec
Radial	66993500	1842815.7	20.25	<30 PPB
Axial	152396800	10665129	13.12	<30 PPB

6. Review:

- ☒ Review with the customer PM work performed.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.



THAI HEART CALIBRATION CO., LTD.
112/1 Moo 5, Phraek Sa, Muang, Samut Prakan 10280
Tel. 0-2394-2162, 0-2351-6435; 0-2757-6496 Fax. 0-2757-8507



Additional Comments

Additional Comments Regarding the PM

Review

The preventive maintenance checks and if applicable performance tests for ICP-OES/Avio200 have been completed.

This ICP-OES/Avio200 Passes ☒ Fails ☐ the preventive maintenance.

Review of Preventive Maintenance:

Authorized PerkinElmer Representative:

Chaymark

Date:

02-Aug-2023
(DD-MM-YYYY)

Authorized Customer Representative:

Wong

Date:

02-Aug-2023
(DD-MM-YYYY)

CERTIFICATE OF CALIBRATION

Certificate No.: T0-2109034/23 Page 1 of total 4 pages

Customer

C.E.M TECHNOLOGY (THAILAND) CO., LTD.
219/43 Moo 12, Petchkasem Road, Onnmoi,
Krathumban, Samutsakorn 74130

Equipment

Thermo Reactor

Manufacturer

Spectroquant

Model

TR 420

Serial No.

23290802

ID No.

Description

Resolution of UUC : 1 °C

Environmental Conditions

Ambient Temperature: (23 ± 3) °C

Relative Humidity: (50 ± 15) %

Atmospheric Pressure: -

Calibration Location

Blue Devils Laboratory (TL)

Received Date

21 September 2023

Calibration Date

22 September 2023

Date of Issue

23 September 2023

Condition of Artifacts

Used conditions but can be calibrated

Checked by

Wong

Approved by

Wong

Act as Technical Manager

Representative of Managing Director

() (Krisyosl K.) () (Sakda Y.)
() (Patiphan K.) () (Onnapa P.)
() (Pongsak H.) () (Nitiiphong K.)
() (Kanung C.) () (Nonthachai K.)
() (Pramong P.) () (Noppol P.)

(Dr. Ekachai Puttitwong)

Certificate No.: T0-2109034/23

Page 2 of total 4 pages

Reference Method :

- The calibration method used was CP-142 based on an in-house method.
- The temperature scale used was an ITS-90.
- This certificate can be traceable to the national standards, which is realized the shown measurement units according to the International System of Units (SI Units).

Reference Standard Instruments:

Type	Model	Serial No.	Cert. No.	Due Date	Traceability
Data Logger with Sensors	34972A/ 34901A	MY59002120/ MY41211040	10-0302002/23	Feb. 3, 2024	THC

Remark: This certificate is traceable to the International System of Unit (SI Unit) through:

- THC, Thai Heart Calibration Co., Ltd.

Measurement Results:

L

Hole No.	UUC Setting (°C)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Stability of UUC (± °C)	Uncertainty (± °C)
# 1	150	149.9	150	-0.1	0.22	0.68
# 2	150	149.8	150	-0.2	0.14	
# 3	150	149.5	150	-0.5	0.21	
# 4	150	149.8	150	-0.2	0.20	
# 5	150	149.1	150	-0.9	0.16	
# 6	150	149.6	150	-0.4	0.32	
# 7	150	149.2	150	-0.8	0.14	
# 8	150	149.7	150	-0.3	1.80	
# 9	150	149.5	150	-0.5	0.18	
# 10	150	149.1	150	-0.9	0.16	
# 11	150	149.1	150	-0.9	0.16	
# 12	150	149.2	150	-0.8	0.17	

UUC : Unit Under Calibration

FE-169

Calibrated by Pongsak
REV.02/02/24/21

Certificate No.: T0-2109034/23

Page 3 of total 4 pages

Measurement Results (Cont.):

R

Hole No.	UUC Setting (°C)	Standard Reading (°C)	UUC Reading (°C)	Correction (°C)	Stability of UUC (± °C)	Uncertainty (± °C)
# 1	150	150.2	150	0.2	0.25	0.68
# 2	150	150.2	150	0.2	0.29	
# 3	150	150.0	150	0.0	0.29	
# 4	150	149.6	150	-0.4	0.18	
# 5	150	149.1	150	-0.9	0.13	
# 6	150	149.5	150	-0.5	0.25	
# 7	150	149.1	150	-0.9	0.16	
# 8	150	149.1	150	-0.9	0.13	
# 9	150	149.7	150	-0.3	0.20	
# 10	150	149.5	150	-0.5	0.20	
# 11	150	149.2	150	-0.8	0.13	
# 12	150	149.6	150	-0.4	0.23	

UUC : Unit Under Calibration



Calibrated by Pongsak
REV.02/02/24/21

FE-169

Certificate No.: T0-2109034/23

Page 4 of total 4 pages

Measurement Results (Cont.):



The above reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

Calibrated by: Pongsak
REV.02.02/24/21

Performance Verification Certificate

Job No. LSPR2306369

Equipment: AA SPECTROMETER

Serial No.: A7310

Manufacturer: GBC Scientific

Verification Date: 23-Jun-2023

Model Type: SavantAA

Customer: บริษัท ซี.ดี.เอ็ม เทคโนโลยีส์ (ไทยแลนด์) จำกัด

219/43 หมู่12 ถนนพหลโยธิน ตำบลคลองน้อย อำเภอคลองหลวง จังหวัดปทุมธานี 74130

Result of Verification

Test Description	Criteria	Reading	Result
1. EHT Photometric Noise (if >350 V)	< 350 V Std. Dev <0.0002	332 V	PASS
2. Wavelength Accuracy, Cu 324.75 nm	± 0.20 nm	324.65 nm	PASS
3. Wavelength Accuracy, Cs 852.10 nm	± 0.20 nm	852.30 nm	PASS
4. Slit Width 0.2 nm	± 0.02 nm	0.22 nm	PASS
5. Slit Width 0.5 nm	± 0.05 nm	0.51 nm	PASS
6. Slit Width 1.0 nm	± 0.10 nm	0.99 nm	PASS
7. Standard Gauze Screen 0.49 Abs* BC mode with gauze BC mode without gauze Difference between With gauze and without gauze	± 0.02 Abs. < 0.004 Abs.	0.4888 Abs. -0.0001 Abs. -0.0004 Abs. 0.0003 Abs.	PASS PASS
8. ABS Reading 5ppm Cu	> 0.7 Abs.	0.740 Abs.	PASS
9. %RSD	< 0.5 %	0.48 %	PASS

* Write in the criteria column the Abs reading on the gauze screen calibration label

We hereby certify that instrument complies with GBC factory specifications

Your satisfaction is our promise @ DKSH Technology Limited

Verification By: Mr. NIWAT SUPATANIT

Signatory: [Signature]

Issued Date: 3-Jul-2023

DKSH Technology Limited
2533 Sukhumvit Road, Bangkok, Phraekhanong, Bangkok 10260
Phone +662 639 7000, www.dksh.com

Delivering growth - in Asia and beyond

02 639 7000

This is to certify that

Niwat Supatanit

From

**DKSH Technology Limited
Thailand**

has successfully completed GBC Service
Training including hardware and software training,
installation and repair on the following instruments:

AAS Instruments and Accessories
UV-Vis Instruments and Accessories
ICP-OES Quantima and Accessories

Introduction to:

ICP-TOFMS OptiMass

High Performance Liquid Chromatography

X-ray Equipment Emma

Training conducted in Penang, Malaysia

From 22 July to 2 August 2019

Geoff

Geoff Condict
CEO



Supelco

www.sigmaaldrich.com

Certified Reference Material Reference material certificate

Copper Standard for AAS

Product no.: 38996

Lot no.: BCCH9264

Description of CRM: Copper metal (pure material) in 2% HNO₃ (prepared with HNO₃ suitable for trace analysis and high-purity water, 18.2 MΩ·cm, 0.22 µm filtered).

Expiry date: JUN 2025

Storage: Store at 5°C-25°C

Density (certified) at 20°C: 1011.3 kg m⁻³ ± 0.5 kg m⁻³

TraceCERT

Constituent Certified values at 20°C and expanded uncertainties, $U = k \cdot u$ ($k = 2$) [1][2]

Copper	989 mg kg ⁻¹ ± 4 mg kg ⁻¹	1000 mg L ⁻¹ ± 4 mg L ⁻¹
--------	---	--

Metrological traceability:

Certified values are traceable to the International System of units (SI) through a metrologically valid weighing process. Details see "Details on metrological traceability" [3]

Measurement method:

The certified value is determined by high-precision weighing of thoroughly characterized starting materials and verified by measurement against NIST SRMs or similar CRMs in accordance with ISO/IEC 17025 [4]

Intended use:

Calibration of AAS, ICP, spectrophotometry or any other analytical technique.

Instructions for handling and correct use:

The bottle's temperature must be 20°C. Shake well before every use. If storage of a partially used bottle is necessary (at the user's risk), the cap should be tightly sealed and the bottle should be stored at reduced temperature (e.g. refrigerator) to minimize transpiration rate.

Health and safety information:

Please refer to the Safety Data Sheet for detailed information about the nature of any hazard and appropriate precautions to be taken.

Packaging:

250 mL HDPE bottle

Accreditation:

Sigma-Aldrich Production GmbH is accredited by the Swiss Accreditation Service SAS as reference material producer under no. SRMS 0001 in accordance with international standard ISO 17034 [5]

Certificate issue date:

29 JUL 2022



ISO 17034
SRMS 0001

S. Matt

S. Matt - CRM Operations

Dr. P. Zell - Approving Officer

Sigma-Aldrich Production GmbH, Industriestrasse 25, 9471 Buchs, Switzerland;
Tel +41-81-755-2511; Fax +41-81-756-5445; www.sigmaaldrich.com
Sigma-Aldrich Production GmbH is a subsidiary of Merck KGaA, Darmstadt, Germany.

Certificate Page 1 of 3

Certificate version 01





CERTIFICATE OF CONFORMANCE

Equipment name : Gauze membrane
Serial Number : F104
Procedure Used : NIST neutral density filter: 8661/SRM 930D (1210)
Reference Standard : Spectrophotometer, LIBRA S70
Serial Number : 136821

Result :

Wavelength (nm)	Measured Value (A.U.)
440	0.489

Valid for 12 months from date of issue.

Issue Date : 5 March 2023
Operator by : Mr. Niwat Supatanit

PREVENTIVE MAINTENANCE AND PERFORMANCE VERIFICATION REPORT

ATOMIC ABSORPTION SPECTROPHOTOMETER (AAS)

Issued Date: 23/06/23

Customer : บริษัท ซี.อี.เอ็ม เทคโนโลยี (ไทยแลนด์) จำกัด

Manufacturer : GBC Scientific Equipment Pty Ltd.

Address : 219/43 หมู่12 ถนนเพชรเกษม ตำบลอ้อมน้อย

Model : SavantAA

Contract : อำเภอกระทุ่มแบน จังหวัดสมุทรสาคร 74130

Serial No. : A7310

Location :


Power on switch and initial status

Instrument Ready, มีค่าความเข้มข้น 2.489


Preventive Maintenance	Pass	Fail	Remarks
Electrical Voltage			
- Main voltage (power supply check 220V \pm 10V).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	220.1 V
- Power indicator light (Replace if faulty).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	N/A
- Power core (Clean or replace as appropriate).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	N/A
- Fan (Clean or replace filter element as appropriate).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	N/A
Environment			
- Temperature (10 to 35 deg.C)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	25.1 C
- Humidity (8 to 80%).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	44 %
- Air Quality (No Dust)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	N/A
- No corrosive vapours present from laboratory sample preparation or external sources.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	N/A
Optics			
- Windows lens (Clean or replace as appropriate).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
- Light Source (Check operation. Replace if required).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
- D2 Lamp (Check operation. Replace if required).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
Gas system			
- General (Tube and Fitting /Check for leaks).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
- Air Zero (Inlet pressure range 300-400 kPa).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	400kPa
- Acetylene (Inlet pressure range 55-96 kPa).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	0.1kPa
- Nitrous oxide (Inlet pressure range 300-400 kPa).	<input type="checkbox"/>	<input type="checkbox"/>	
Computer			
- Operating system	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Windows 7
- Software Version	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Savant 3.0
- Verify that all computer links and installed software operate correctly	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready

Spray Chamber Type

☐ ABR Spray Chamber

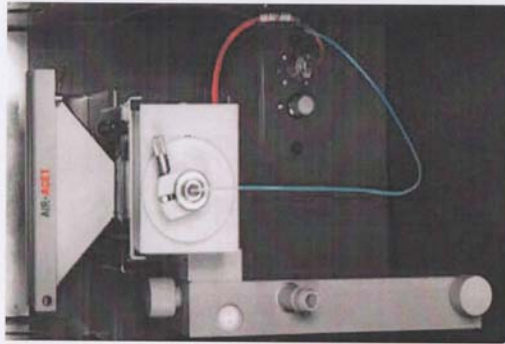

☒ Standard Spray Chamber

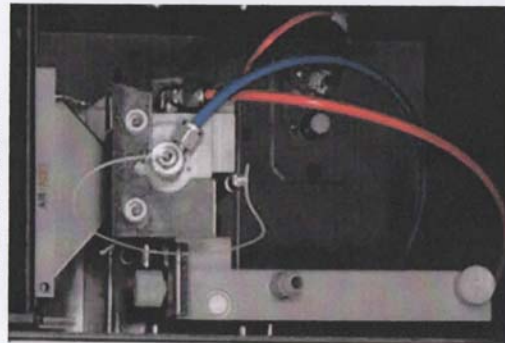

Preventive Maintenance		Pass	Fail	Remark
Flame system				
-	Burner head (Clean the jaws using GBC Burner Cleaning Card).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Burner mount (Check for wear. Replace the burner retaining plate if required).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Spray chamber (Visually inspect the bead for cracks, pitting or solid deposits. Check or replace O-ring kit).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Safety interlocks			
	➢ Burner (Check for Interlocks connector)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
	➢ Spray chamber (Check for Interlocks connector)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Pressure relief bung. (Check or replace O-ring)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Nebulizer (Clean and check operation / Replace the O-ring)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Gas connections (Check for leaks).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Capillary tube (Check bends and clog).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Liquid trap (Drain / clean and replace O-ring).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready

Gas Flow Optimisation		Pass	Fail	Remark
-	Bleed gas lines (Relieve pressure in the spray chamber).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Ignitor (Ignite the flame several times to check ignition reliability. Replace the glow plug if required).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Extinguish (Check operation).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Horizontal movement (Check operation for STD. Spray Chamber).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Vertical movement (Check operation for STD. Spray Chamber).	<input checked="" type="checkbox"/>	<input type="checkbox"/>	Ready
-	Burner Adjuster (Check operation for ABR Spray Chamber)			
	➢ Burner Angle (° C)	<input type="checkbox"/>	<input type="checkbox"/>	
	➢ Angle Zero (mm)	<input type="checkbox"/>	<input type="checkbox"/>	
	➢ Work head Height (mm)	<input type="checkbox"/>	<input type="checkbox"/>	
	➢ Work head Centre (mm)	<input type="checkbox"/>	<input type="checkbox"/>	

Note:

N/A

Signature	
Customer :	Date :
(.....)	
Service Engineer :	Maintenance Date :
(Mr. NIWAT SUPATANIT)	23 / Jun / 2023



บริษัท ดีเคเอส อีซี จำกัด

Job No. LSPR2306389
□ Service contract Basic Plan
□ Service contract Performance Plan

Performance Verification	Specification	Actual Value	Pass	Failed	Remarks
1. Wavelength accuracy (optic calibration check).	Cu 324.75 nm \pm 0.2 nm Cs 852.10 nm \pm 0.2 nm	324.65 nm 852.20 nm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
2. Slit width accuracy (0.2 nm, 0.5 nm, 1.0 nm)	0.2 nm \pm 0.02 nm 0.5 nm \pm 0.05 nm 1.0 nm \pm 0.10 nm	0.216 nm 0.51 nm 0.99 nm	<input checked="" type="checkbox"/> <input checked="" type="checkbox"/> <input checked="" type="checkbox"/>	<input type="checkbox"/> <input type="checkbox"/> <input type="checkbox"/>	
3. EHT	<350V	332V	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
4. Absorbance accuracy (absorbance calibration check). ➢ Gauze 0.49 A.U.	Reading \pm 10% of calibrated value.	0.4988 Abs.	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
5. Background correction (optics alignment check). difference between measurement with and without 0.49 A.U. gauze for 10 samples.	SavantAA <1% SensAA/XplorAA <2%	BC on with gauze: -0.0001 Abs BC on without gauze: -0.0004 Abs	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
6. Sensitivity / noise flame test (aqueous Cu solution test under air-acetylene flame).	Cu 5 ppm >0.7 A.U. <0.5% RSD	0.7396 Abs 0.48 %	<input checked="" type="checkbox"/> <input checked="" type="checkbox"/>	<input type="checkbox"/> <input type="checkbox"/>	

Note: N/A

Signature	Date :
Customer : (.....)	Maintenance Date : 23 / Jun / 2023
Service Engineer : Niwat S. (Mr. NIWAT SUPATANIT)	



Certificate of Calibration

Aquion RFIC: Anion (ID#1084)

This certificate is to verify that instrument below are calibrated
by Archemica International Co., Ltd.

Aquion S/N: 221280114
AS-DV S/N: 2205880126

For
C.E.M Technology (Thailand) Co., Ltd.



Operator Signature: Date: Jan 25, 2024
(Mr. Itsaraphap Bumrungrjeam)
Applications Chemist

การดูแลบำรุงรักษาเชิงป้องกัน Preventive Maintenance



บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

ฝ่ายบริการหลังการขาย

โทร 0 2 639 7000 E-mail: service.tec.th@dksh.com

ฝ่ายขายและการตลาด

โทร 0 2 639 7000 E-Mail : marketing.tec.th@dksh.com

Website : www.dksh.co.th/technology/scientific-thailand

เงื่อนไขการให้บริการ Preventive Maintenance

บริษัทฯ จะส่งวิศวกรผู้ชำนาญ เพื่อให้บริการตรวจซ่อมบำรุงของการบริการ เฉพาะ ในวันและเวลา ราชการ หากมีความประสงค์ที่จะรับบริการนอกเหนือจากวัน เวลา ราชการ (วันหยุดเสาร์ – อาทิตย์ หรือวันหยุด นักชดถุณ) บริษัทฯ จะคิดค่าบริการเพิ่มเติมตามอัตราที่กฎหมายแรงงานกำหนดไว้

ขอบข่ายการบริการ

- ตรวจสภาพการทำงานต่าง ๆ ของเครื่องมือ
- ทดสอบประสิทธิภาพการทำงานของเครื่องมือ
- รายการผลการตรวจสอบเครื่องมือ

หมายเหตุ

- ราคาไม่รวมถึงค่าบริการซ่อมหรือ เปลี่ยนอะไหล่ที่ชำรุดเสียหาย หรือหมดสภาพการใช้งาน
- ในกรณีที่ผู้รับบริการอยู่นอกเขตที่ให้บริการ บริษัทฯ จำเป็นต้องคิดค่าใช้จ่ายเพิ่มเติม ใต้ค่าเดินทาง เป็นต้น
- บริษัทฯ ขอสงวนสิทธิ์ในการเปลี่ยนแปลงราคา โดยไม่แจ้งให้ทราบล่วงหน้า



ช่องทางการติดต่อ

DKSH Technology Limited (บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด)
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260
เลขประจำตัวผู้เสียภาษี 010-555-001-4547 (สำนักงานใหญ่)



Call center 0 2 639 7000



DKSH Scientific



www.dksh.com/scientific-thailand



marketing.tec.th@dksh.com



@dkshscientific

Preventive Maintenance Contract

จำนวนใบการทำสัญญาบริการ ครั้งต่อปี
ครั้งที่ 1. วันที่ 15/05/2024.....

รายละเอียดผู้รับบริการ

หน่วยงาน	บริษัท จี.อี.เอ็ม เทคโนโลยี (ไทยแลนด์) จำกัด		
ที่อยู่	219/43 หมู่ 12 ถนนพหลโยธิน ตำบลอ้อมน้อย อำเภอกระทุ่มแบน จังหวัดสมุทรสาคร 74130		
โทรศัพท์	0869054664	แฟกซ์	-

ผู้ติดต่อ

ชื่อ - นามสกุล	คุณศิริพร พินพา		
ตำแหน่ง	เจ้าหน้าที่ห้องปฏิบัติการ		
โทรศัพท์	0869054664	เบอร์โทร	- แฟกซ์ -
E-mail	lab.cemtech1@gmail.com		


รายละเอียดผู้ให้บริการ

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด (ฝ่ายบริการหลังการขาย) (สำนักงานใหญ่) เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260 โทรศัพท์ 0 2 693 7000 Email: support.sk@dksh.com เจ้าหน้าที่ประสานงาน : คุณสุธาวัฒน์ ศรีรัตน์ โทรศัพท์ 090 678 6925			
เจ้าหน้าที่ผู้ให้บริการ	นายวิชาญ สดอาด		
ตำแหน่ง	Specialist, Technical Service.		
โทรศัพท์	0938138736	แฟกซ์	-
E-mail	Jirayut.js@dksh.com		

ลงนามผู้รับบริการ	ลงนามผู้ให้บริการ
ตัวจริง (.....)	ตัวจริง (นาย วิชาญ สดอาด)
ตำแหน่ง	ตำแหน่ง Specialist, Technical Service.
วันที่ / ประทับตราบริษัท	วันที่ / ประทับตราบริษัท 15/05/2024

JOB:LSR2403415.....MODEL:VAP.200.....S/N: GER5200180181.
Operational Qualification (OQ)
ทดสอบสมรรถภาพ


FRONT

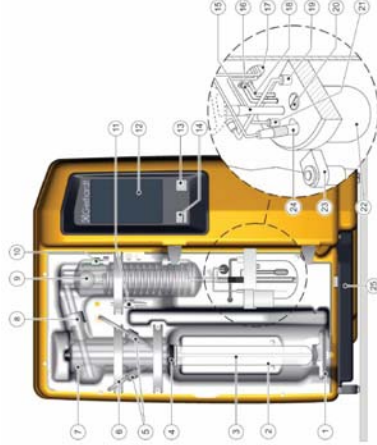

No		PASS	FAIL	N/A
1	Quick clamping device with clamping block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
2	Digestion tube 250/300 ml	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	PTFE steam inlet tubing	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Connection stopper , Viton	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Screw cap GL18	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	PTFE-inlet tubing NaOH	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Distribution head made of glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Screw cap GL32	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Distillation condenser made of glass	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Screw cap GL14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Ventilation valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	Control panel	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Operating Button	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	USB interface (with protective cap)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Silicone tubing 8/10 for distillate discharge **	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
16	Verprene tubing 4/8 , receiver suction **	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
17	Cable duct for electrode cable + titration tube**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
18	Silicone tubing 4/7 , boric acid inlet**	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
19	Sensor for level monitoring including connector**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
20	Agitator motor with propeller**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
21	Titration acid inlet tube **	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
22	Receiver glass**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
23	Holder for pH electrode , removable**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
24	pH electrode (combined electrode)**	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
25	Drip tray PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>


** only VAP 450

REAR

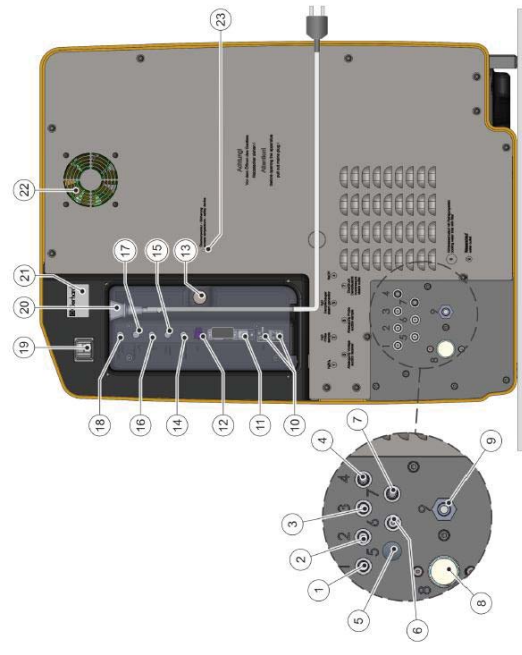


No		PASS	FAIL	N/A
1	Tube connection for sample H3BO3 supply	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
2	Tube connection for sample H2O supply	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
3	Tube connection for steam generator H2O supply	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Tube connection for NaOH supply	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Tube connection for receiver glass extraction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	Tube connection for sample waste extraction	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Tube connection , overpressure steam outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Connection for cooling water supply (with cleaning sieve)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Tube connection for cooling water outlet	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	4 X USB interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	1 X RS-232 Interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	LAN Interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Screw cap for Perspex cover	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Connection socket for sample waste tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
15	Connection (not used)	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Connection socket for H2O tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Connection socket for H3BO3 tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18	Connection socket for NaOH tank level monitoring	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Overcurrent circuit breaker	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20	Apparatus socket (mains cable connection)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Rating plate with serial number	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22	Exhaust air fan	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23	Excess temperature switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Inside Steam generator

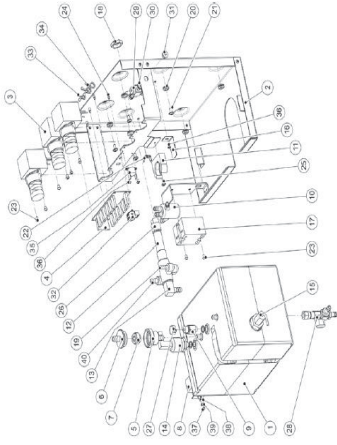

No		PASS	FAIL	N/A
1	Steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	N/A
2	Steam generator traverse	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	Pinch valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Circuit board distributor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Valve tubing connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	Housing safety valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Safety valve SKT	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Excess temperature protection , steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Safety valve G 1/8 0.5 bar	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Ventilation glass pinch valve VAPODEST	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Hose clamp for ventilation clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	Distributor PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Angle connection PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Pressure transmitter	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Level switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Fixing bracket steam generator	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Relay HT+	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18	VA Hexagon nut 1/2"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Angle connection 1/8"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20	Bushing nipple 6-10-14	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	VA Lens head screw M5 X 10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22	Grounding connection , 2-pole	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23	VA Lens head screw M4 X 6	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
24	Spacer bolt 5 mm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
25	VA Lens head screw M4 X 10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
26	Tubing connection	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	Hose clamp 14.5 mm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
28	Module ball valve with nozzles	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
29	Cross manifold with spout	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
30	Seal copper G 1/8	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
31	Locking screw 1/8"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
32	Pin strip	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
33	Bundle clamp 12 H 4500	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
34	Bundle clamp 12 H 4502	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
35	Temperature switch 80°C	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
36	VA Lens head screw M3 X 6	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
37	VA Hexagon nut M4	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
38	Lins head screw M4 X 8	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
39	VA Spring washer	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
40	Angle connection , reduced , 1/8" PP	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Module Pump holder VAP200 - 450 V3

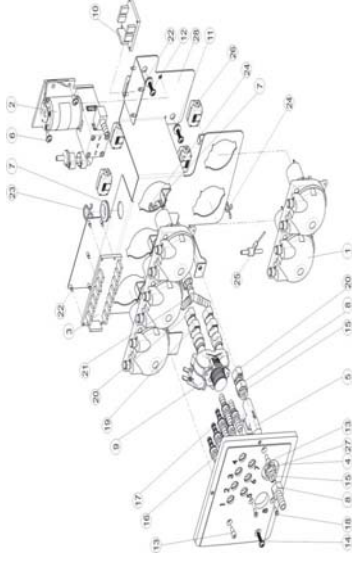

No		PASS	FAIL	N/A
1	Peristaltic pump	<input checked="" type="checkbox"/>	<input type="checkbox"/>	N/A
2	Diaphragm pump NaOH, with non-return valve	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
3	Circuit board	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4	Tubing connection module	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
5	Flow controller	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
6	Lens head screw M5 x 10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
7	Bushing nozzle	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
8	Screw in socket	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
9	Magnetic valve 2/2 way	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
10	Circuit board distributor	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
11	Bushing nozzle	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
12	Screw 5 x 25	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
13	Cylinder screw	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
14	Screw 5 x 20	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
15	Seal EPDM 15 x 4	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
16	Tubing connection piece 51x10x6,5	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
17	Tubing connection piece 51x10x10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
18	Screw M4x10	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
19	Clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
20	Clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
21	Y-tube connector	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
22	Spacer bolt 5 mm	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
23	Bundle clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
24	Bundle clamp	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
25	Retrofit earthing pumpv	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
26	Snap ferrite	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
27	Nut G 3/8"	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
28	Pump holder plate	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Control panel



No		PASS	FAIL
1	Title bar	<input checked="" type="checkbox"/>	<input type="checkbox"/>
2	Status bar	<input checked="" type="checkbox"/>	<input type="checkbox"/>
3	Navigation button	<input checked="" type="checkbox"/>	<input type="checkbox"/>
4	Smart switch with multiple functions	<input checked="" type="checkbox"/>	<input type="checkbox"/>
5	USB interface	<input checked="" type="checkbox"/>	<input type="checkbox"/>

รายละเอียดการตรวจสอบ

ขั้นตอนการบริการ

- ตรวจสอบระบบไฟฟ้า (Electrical Test)
- ความต้านทานทางไฟฟ้าของเครื่องกับกราวด์
 - กระแสไฟฟ้าที่ใช้งาน

ตรวจสอบสภาพเครื่อง (Optical Test)

- Main cable
- Electric wiring
- Pumps
- Distribution Head
- Condensor
- Steam generator
- Tubing
- Viton cone

ตรวจสอบ Function การทำงาน (The Function Test)

- ระบบสร้างและควบคุมความดันของ Steam
- ระบบการเติมน้ำเข้าสู่ Sample Tube
- ระบบการเติม Na OH
- ระบบการเติม H3BO3

รายงานผลการปฏิบัติงาน

1. TECHNICAL DATA

Main Supply 220 volt + 10% 50 Hz with ground
Nominal current

Pass ☒ ☒
Fail ☐ ☐
N/A ☐ ☐
Remark
.....
.....8a.....

1.1 COOLING WATER BATH

Temperature 15-20 °C
Cooling Water Outlet
Control Temperature

Pass ☒ ☒ ☒ ☒
Fail ☐ ☐ ☐ ☐
N/A ☐ ☐ ☐ ☐
Remark
.....
.....
.....

1.2 OPTICAL TEST VAP200

Screw cap GL14
Screw cap GL18
Screw cap GL32
Distillation Head
Condensor
Viton Cone
Ventilation Valve BV
Micro Switch Sample
Agitator motor for propeller

Pass ☒ ☒ ☒ ☒ ☒ ☐ ☒ ☒ ☐
Fail ☐ ☐ ☐ ☐ ☐ ☒ ☐ ☐ ☐
N/A ☐ ☐ ☐ ☐ ☐ ☐ ☒ ☐ ☐
Remark
.....
.....
.....
.....
.....
.....
.....
.....
.....

2.SYSTEM COOLING WATER INLET

Cooling Water Inlet
Cooling Water Outlet
Flow control valve

Pass ☒ ☒ ☒
Fail ☐ ☐ ☐
N/A ☐ ☐ ☐
Remark
.....
.....
.....

3.SYSTEM CONTROL

Display
Program
Adding NaOH
Adding H2O
Adding H3BO3
Suction Sample
Suction Receiver

Pass ☒ ☒ ☒ ☐ ☐ ☐ ☐
Fail ☐ ☐ ☐ ☐ ☐ ☐ ☐
N/A ☐ ☐ ☐ ☒ ☒ ☒ ☒
Remark
.....
.....
.....
.....
.....
.....
.....

4.SYSTEM DISTILLATION

Boiler
Level Sensor
Novopren
Solenoid Valve Shut-Off
Solenoid Valve Steam
Solenoid Valve soft steam
Ventilation Valve Premount
Excess Pressure Detector
Heating Element

Pass ☒ ☒ ☒ ☒ ☒ ☒ ☒ ☒ ☒
Fail ☐ ☐ ☐ ☐ ☐ ☐ ☐ ☐ ☐
N/A ☐ ☐ ☐ ☐ ☐ ☐ ☐ ☐ ☐
Remark
.....
.....
.....
.....
.....
.....
.....
.....
.....

5. PUMP

Pump H₂O Steam
- Non-Return Valve
Pump H₂O Sample
- Non-Return Valve
Pump NaOH
- Non-Return Valve
Pump H3BO3
- Non-Return Valve
Pump suction
Pump suction receiver

Pass ☒ ☐ ☐ ☒ ☒ ☐ ☐ ☐ ☐
Fail ☐ ☐ ☐ ☐ ☐ ☐ ☐ ☐ ☐
N/A ☐ ☒ ☐ ☐ ☒ ☒ ☒ ☒ ☒
Remark
.....
.....
.....
.....
.....
.....
.....
.....
.....

6. The Following Program Run :

Addition H2O 0-999 ml.
Addition NaOH 0-999 ml.
Addition H3BO3 0-999 ml.
Reaction Time 0-108 min
Distillation Time 0-108 min
Steam Capacity 10%-100%
Suction Sample
Suction Receiver

Pass ☐ ☒ ☐ ☒ ☒ ☒ ☐ ☐ ☐
Fail ☐ ☐ ☐ ☐ ☐ ☐ ☐ ☐ ☐
N/A ☒ ☐ ☒ ☐ ☐ ☐ ☒ ☒
Remark
.....
.....
.....
.....
.....
.....
.....
.....
.....

7. Measured pumps

Pump NaOH

Volume : ...13.33.....ml
Remark :

ข้อมูลสนับสนุนด้านเทคนิค (General Technical Support)

การบำรุงรักษาทั่วไป (Basic maintenance)

Cleaning program

Glass parts and tubes must be rinsed daily before starting analysis in order to prevent clogging by crystallizing chemicals. The following settings are recommended for this:

parameters	Value
H ₂ O addition	150 ml
NaOH addition	0 ml
Distillation time	7 min
Steam power	100 %
Reaction time	0 s
Suction sample	30 s

→ Insert a digestion tube (without sample) and start the program.
→ All liquid carrying parts are cleaned. In the case of strong soiling, approx. 10 ml of sulphuric acid can also be added to the digestion tube.

Analytical errors

Fault description	Cause	Remedy
Analyte results too high	The chemicals used are contaminated with nitrogen compounds.	■ Detailed checking of the chemicals. ■ Determination of a blank value. ■ Replace the chemicals if necessary.
	Valent reaction in the digestion tube: sodium hydride drops get into the receiver.	■ Increase of the water addition amount.
	Glass bridges of the condenser is broken or worn out, sodium hydride drops get into the receiver.	■ Replacement of the glass condenser.
	Glass cleaning agents in the digestion tube.	■ Clean digestion tube in advance with distilled water.
	Entrainment of ammonia from the previous sample.	■ Increase distillation time. ■ Check whether sample was previously sufficiently alkalized.
Analyte result too low or no result	Incomplete distillation; distillation time too short.	■ No quantitative explosion of the ammonia content. ■ The distillation amount should be 100 ml.
	Ammonia escapes at leaking places.	■ Solid or defective Viton plugs: clean or replace. ■ Check seals (G.L. screw connections) on the condenser and receiver. ■ Check valve at the condenser is gummed up; clean or replace. ■ Digestion tube is damaged at the neck or bottom.
	Adding amount of the sodium hydride too little; no ammonia development.	■ Distribution head glass leaks: replace. ■ Check the content flow rate of the NaOH pump (see technical data).
	Too low boric acid amount in the receiver; escaping ammonia is not completely bonded.	■ Increase of the boric acid amount.
	Tube not completely immersed in the acid receiver.	■ Increase of the acid amount.
	Formation of stable ammonia compounds with sodium hydroxide destroyed with sodium hydroxide.	■ This problem only occurs with catalysts and reagents. Sodium hydroxide solution destroys these compounds.

General error message

Fault description	Cause	Remedy
'Cooling water flow volume too low'	Cooling water pressure under 1 bar	■ Open water tap. ■ Check coolant pressure. ■ Check coolant tube. Program continues automatically once error has been fixed.
'Sample tube missing'	Sample tube missing.	■ Insert sample tube. Continue program or restart.
'Distillation room protective door open'	Protection door not closed	■ Close protection door. Program continues automatically once error has been fixed.
'Reagent storage/waste'	One or more storage tanks are empty	■ Fill storage tank. ■ Check correct sealing of the universal sensors. The running program can be continued after rectification of the error.
	The sample waste tank is full.	■ Empty sample waste tank. ■ Check correct sealing of the universal sensors. The running program can be continued after rectification of the error.

การดูแลบำรุงรักษาเชิงป้องกัน

Preventive Maintenance



บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด

ฝ่ายบริการหลังการขาย

โทร 0 2 639 7000 E-mail: service.tcc.th@dksh.com

ฝ่ายขายและการตลาด

โทร 0 2 639 7000 E-Mail : marketing.tcc.th@dksh.com

Website : www.dksh.co.th/technology/scientific-thailand

เงื่อนไขการให้บริการ Preventive Maintenance

บริษัทฯ จะส่งวิศวกรผู้ชำนาญ เพื่อให้บริการตามขอบข่ายของบริการ เฉพาะ ในวันและเวลา ราชการ หากมีความประสงค์ที่จะรับบริการนอกเหนือจากรัน เวลา ราชการ (วันหยุดเสาร์ – อาทิตย์ หรือวันหยุด นักชดถุณ) บริษัทฯ จะคิดค่าบริการเพิ่มเติมตามอัตราที่กฎหมายแรงงานกำหนดไว้

ขอบข่ายการบริการ

- ตรวจสอบสภาพการทำงานต่าง ๆ ของเครื่องมือ
- ทดสอบประสิทธิภาพการทำงานของเครื่องมือ
- รายการผลการตรวจสอบเครื่องมือ

หมายเหตุ

- ราคานี้ ไม่รวมถึงค่าบริการซ่อม หรือ เปลี่ยนอะไหล่ที่ชำรุดเสียหาย หรือหมดสภาพการใช้งาน
- ในกรณีที่ผู้รับบริการอยู่นอกเขตพื้นที่ให้บริการ บริษัทฯ จำเป็นต้องคิดค่าใช้จ่ายเพิ่มเติม ได้แก่ ค่าเดินทาง เป็นต้น
- บริษัทฯ ขอสงวนสิทธิ์ในการเปลี่ยนแปลงราคา โดยไม่แจ้งให้ทราบล่วงหน้า



ช่องทางการติดต่อ

DKSH Technology Limited (บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด)
เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260
เลขประจำตัวผู้เสียภาษี 010-555-001-4547 (สำนักงานใหญ่)



Call center 0 2 639 7000



DKSH Scientific



www.dksh.com/scientific-thailand



marketing.tec.th@dksh.com



@dkshscientific

Preventive Maintenance Contract

จำนวนใบการทำสัญญาบริการ ...๑...ครั้งต่อปี
ครั้งที่ ๑..วันที่ 15.05.2024.....

รายละเอียดผู้รับบริการ

หน่วยงาน	บริษัท ซี.อี.เอ็ม เทคโนโลยี (ไทยแลนด์) จำกัด		
ที่อยู่	219/43 หมู่2 ถนนเพชรเกษม ตำบลอ้อมน้อย อำเภอกะห้ล่นแบน จังหวัดสมุทรสาคร 74130		
โทรศัพท์	0869054664	แฟกซ์	-

ผู้ติดต่อ

ชื่อ - นามสกุล	คุณศิริพร พิมพ์		
ตำแหน่ง	เจ้าหน้าที่ห้องปฏิบัติการ		
โทรศัพท์	0869054664	เบอร์ดี	แฟกซ์ -
E-mail	lab.centechl@gmail.com		


รายละเอียดผู้ให้บริการ

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด (ฝ่ายบริการหลังการขาย) (สำนักงานใหญ่) เลขที่ 2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพฯ 10260 โทรศัพท์ 0 2 693 7000 Email: sudarat.sk@dksh.com เจ้าหน้าที่ประสานงาน : คุณสุดารัตน์ ศิริรัตน์ โทรศัพท์ 090 678 6925			
เจ้าหน้าที่ผู้ให้บริการ	นายจิรายุ สดอาด		
ตำแหน่ง	Specialist, Technical Service.		
โทรศัพท์	0938138736	แฟกซ์	-
E-mail	Jirayut.js@dksh.com		

ลงนามผู้รับบริการ		ลงนามผู้ให้บริการ	
ตัวจริง	(.....)	ตัวจริง	(นาย จิรายุ สดอาด)
ตำแหน่ง		ตำแหน่ง	Specialist, Technical Service.
วันที่ / ประทับตราบริษัท		วันที่ / ประทับตราบริษัท	15/05/2024

Part 3: ตรวจเช็คสภาพเครื่อง

Front and rear view of KT-L version

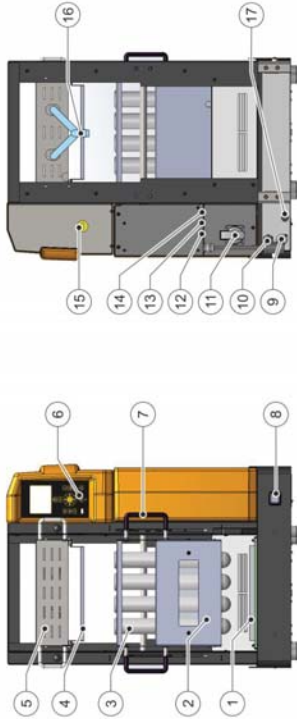


No.		PASS	Fail	N/A	Remark
1	KJELDATHERM digestion block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	เสื่อมสภาพ
2	Insert rack	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
3	Digestion tube	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
4	Stainless steel drip tray	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
5	Exhaust manifold	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
6	Controls module, removable	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
7	Handle for insert rack	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
8	Mains switch with overcurrent protection function	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
9	Connection for lift unit	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
10	Mains cable with plug	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
11	Power supply for TURBOSOG	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
12	Connects controller module to block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
13	Connection for fan for cooling samples (optional)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
14	Connection for external cooling water valve (optional)	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
15	Connects controller module to block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
16	Connection for Iso-Versinic hose (extraction)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
17	Excess temperature fuse	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	
18	Lift	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	

Part 4: ฉะเอียดและรายงานผลการให้บริการ Preventive Maintenance

4.1 ตรวจเช็คระบบไฟฟ้า

ใช้ไฟ 220 V 50 Hz	Pass	Fail	N/A	Remark
กระแสไฟฟ้าตามพิกัดเครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
4.2 ตรวจสอบสภาพอุปกรณ์ภายนอก	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
สายไฟของเครื่อง	Pass	Fail	N/A	Remark
ท่อแก้วรวมไอกรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
สายขมวดกับท่อแก้วรวมไอกรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
สภาพของ A aluminum block	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
การขึ้นลงของ Lift	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Light	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Current Switch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Thermostat	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

4.ตรวจเช็คระบบการทำงาน

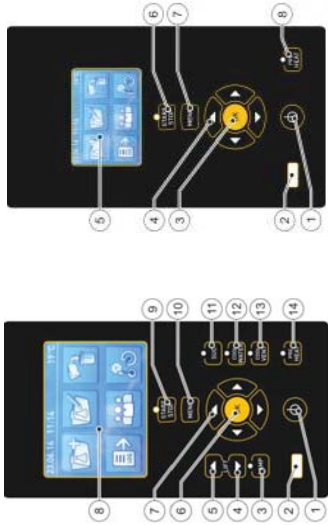

☐ KT-L

☒ KT

- Switch controller on or off:
- USB port
- LAMP button
- LIFT down button
- LIFT up button
- OK button
- Navigation buttons
- Display
- START/STOP button
- MENU button
- SUC button
- COOL/WATER button (optional)
- COOL /VENT" button (optional)
- PRE HEAT" button
- การขึ้นของอุณหภูมิมานกกว่า10องศาต่อนาทีที่25องศา
- การทำงานของตัวป้องกันอุณหภูมิสูงเกิน
- การทำงานของระบบควบคุมอุณหภูมิ

Pass	Fail	N/A	Remark
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

การบำรุงรักษาทั่วไป (Basic maintenance)

- การย่อยตัวอย่างเกิดการเค็ดที่รุนแรงอันเนื่องจากตัวอย่างนั้นสามารถป้องกันได้โดยแนะนำให้ย่อยด้วยการตั้งการเพิ่มอุณหภูมิเป็นระดับเช่น ย่อยที่ระดับอุณหภูมิ 250 C ครบเวลา 15 นาทีจึงเปลี่ยนเป็นอุณหภูมิ 380 C เพื่อป้องกันการสั่นออกมา
- เมื่อใช้เสร็จ ไม่ควรปล่อยให้ Tube เย็นกับตัวเครื่อง
- ต้องนำเอาคาลองไอการใส่ทุกครั้งหลังจากใช้งานเสร็จ เพื่อป้องกันการหยดของไอกรดที่จะหยดลงไปที่ตัวเครื่อง
- ทำความสะอาดตัวหลุมย่อยด้วยน้ำหรือผ้าชุบน้ำในกรณีที่มีคราบกรดลงมาติดอยู่ในหลุม

เพื่อป้องกันไม่ให้เกิดราดังกล่าวก็นำไปกับการเผอุณหภูมิ