

**Certificate No.:** T/O 660198

**Date of issue :** 11-Oct-2023

**Equipment Description** : Refrigerator  
**Equipment Model** : P1010  
**Equipment Serial No.** : P1010-1020-0005  
**I.D. No. or Control No.** : TNP.LAB.01  
**Manufacturer** : Entech Industrial Solution Co.,Ltd.  
**Customer Name** : TNP ENVIRONMENT CO.,LTD.  
**Customer Address** : 332/173 Moo. 3 Tambon Bang Rak Phatthana, Amphoe Bang Bua Thong,  
Nonthaburi 11110  
**Total pages of certificate** : 2 pages  
**Instrument Receiving Date** : 9-Oct-2023  
**Receiving No.** : O-230230  
**Environmental Conditions** : All of the measurement were carried out in the working area  
Temperature : ( 25 ± 15 ) °C  
Humidity : ( 55 ± 30 ) % RH  
Voltage : ( 220 ± 22 ) VAC  
**Calibration Place** : 332/173 Moo. 3 Tambon Bang Rak Phatthana, Amphoe Bang Bua Thong,  
Nonthaburi 11110  
**Calibration Procedure No.** : This instrument was calibrated by comparison of reference radiation source standard  
according to calibration work instration no WI-CL-18-C

*The calibration certificate expended uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ , which for a normal distribution corresponds to a coverage probability of approximately 95%*

*The standard uncertainty of measurement has been determined in accordance with M 3003  
The expression uncertainty and confidence in measurement.*

*This certificate is applied only to item under test environmental condition.*

*This calibration certificate may not be reproduced other than in full except with the permission of the issuing laboratory.  
Calibration certificates without signature and seal are not valid.*

*This calibration certificate documents are traceability to national standards, which realize the unit of measurement according to the International system of units (SI).*

**Date of Calibration** : 9-Oct-2023



Mr. Kittipong Kaewsai  
Calibration Engineer



Ms. Nongluck Wongsettee  
Technical Manager

**Certificate No. : T/O 660198**


**The Reference Standard Instrument :-**

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert No.</u>	
1) Data logger with RTD Probe	Agilent 34972A	MY41187730	PSL-T 0651-1/66	21-Apr-2024
		MY60008352	PSL-T 0651-3/66	21-Apr-2024

**Measured room conditions**

<b>Temperature :</b>	Minimum: 30.8 °C	Maximum: 31.9 °C
<b>Humidity :</b>	Minimum: 50.7 %RH	Maximum: 57.2 %RH
<b>Voltage :</b>	Minimum: 219.8 VAC	Maximum: 223.4 VAC
<b>Fresh Air Setting:</b>	off	

**Sensor Position :**

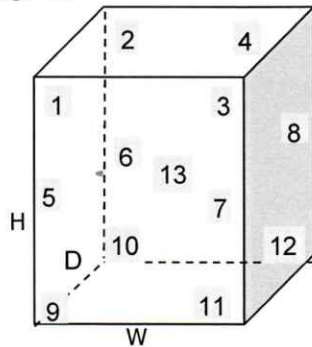

**Working Space of chamber :**

(Inside Dimensions) W x D x H : 1560 mm x 500 mm x 1380 mm

**Sensor Installation Details :**

- Sensor Number 1 to 12 installed approximately 50 mm From each wall.
- Sensor Number 13 installed approximately geometric of the chamber.

**Results :** The measurement results of the calibration were reported in the table below.

(\*) Without adjustment

( ) After adjustment

<b>UUC* Setting</b>	<b>UUC* Reading</b>	<b>Temperature Reading of Standard Sensor</b>								
( °C )	( °C )	<b>Sensor Position</b>								
		<b>1</b>	<b>2</b>	<b>3</b>	<b>4</b>	<b>5</b>	<b>6</b>	<b>7</b>	<b>8</b>	<b>9</b>
		4.02	4.35	4.01	4.20	4.37	4.22	4.17	4.39	4.05
		<b>Sensor Position</b>								
		<b>10</b>	<b>11</b>	<b>12</b>	<b>13</b>					
		4.29	4.30	4.28	4.19					

<b>UUC* Setting</b>	<b>UUC* Reading</b>	<b>Temperature Uniformity</b>	<b>Temperature Stability</b>	<b>Overall Variation</b>	<b>Uncertainty of Measurement</b>	<b>Coverage Factor K</b>
( °C )	( °C )	( °C )	( ± °C )	( °C )	( ± °C )	
4.0	4.1	1.19	1.08	2.47	1.5	2

**UUC\* = Unit Under Calibration**

**Remark :-**

- Temperature reading of Standard Sensors shown in the table were taken from the average of Standard reading at each position.
- Temperature Uniformity was calculated from the difference between the maximum and minimum of actual temperature reading from all reference sensors at the same time.
- Temperature Stability was calculated from the maximum stability of nine positions, and formula of Stability is  $[( \text{Maximum Temperature Value} - \text{Minimum Temperature Value} ) / 2 ]$
- Overall Variation was calculated from the difference between the maximum and minimum measured temperature throughout observation time.

**End of Report**

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : pH METER  
MANUFACTURER : HORIBA  
MODEL / TYPE : LAQUA-PH1100/9615S  
SERIAL NO. : B80A0042/9X0B0575  
CLID. NO. : 272001452  
JOB CONTROL NO. : 230911100397

CUSTOMER : TNP ENVIRONMENT CO., LTD.  
332/173 MOO 3 TAMBON BANG RAK PHATTANA,  
AMPHOE BANG BUA THONG, NONTABURI 11110

DATE OF RECEIVED : 11 September 2023

DATE OF ISSUED : 14 September 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Sukgasem Seehanart  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory  
14 September 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to  
the International System of Units ( SI )

Certificate No. Q23100397

F3-011-04/01-12

page 1 of 3



@clccalibration

## REPORT OF CALIBRATION

### FOR

**NOMENCLATURE** : pH METER  
**MANUFACTURER** : HORIBA  
**MODEL / TYPE** : LAQUA-PH1100/9615S  
**SERIAL NO.** : B80A0042/9X0B0575  
**DATE OF CALIBRATION** : 12 September 2023

---

#### ENVIRONMENT CONDITIONS :

**Temperature** :  $(25 \pm 2.5) ^\circ\text{C}$

**Relative Humidity** :  $(50 \pm 15) \% \text{ RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPCH-01**. The calibration was performed by direct measurement with Certified Reference Material (CRM).

#### REFERENCE STANDARD USED :

1. pH Standard Solution, NIMT TRM CODE TRM-S-2003, TRM CODE TRM-S-2007.
2. pH Standard Solution, Control Company Catalog Number 06664263,11784256, Lot Number CC752722.

#### TRACEABILITY :

1. The measurements are traceable to International System of Units (SI) , through National Institute of Metrology (Thailand).  
Lot Number. 040822 , 230822. Due Date 26 April 2024.
2. The measurements are traceable to International System of Units (SI) , through Control Company.  
Certificate No. 4288-13355261 , Due Date 06 May 2024.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor complies with the table which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

**Certificate No. Q23100397**

**F3-011-04/01-12**

page 2 of 3







**CLC**  
Accredited  
ISO/IEC 17025

# CALIBRATION LABORATORY Co., LTD.

2/10-11,14,55 Soi Prasert Manukit 29 Yaek 4, Prasert Manukit Rd., Ladphrao, Bangkok 10230  
Tel. 02-578-0353-4 Fax: 02-578-2672 www.cal-laboratory.com E-mail:sale@cal-laboratory.com



**CONDITION OF CALIBRATION ITEM : GOOD**

**MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment**

The table in the following gives the calibration results and associated measurement uncertainties of pH meter.

## CALIBRATION DATA

### **pH METER RESULT @ 25 °C**

Standard pH Buffer Solution (pH)	pH Meter Reading (pH)	pH Meter Reading (mV)	Correction (pH)	Uncertainty of pH Measurement ( $\pm$ pH)	k Factor
4.003	4.01	150.2	-0.007	0.010	2,00
7.000	7.00	-26.1	0.000	0.015	2,06
10.003	10.01	-187.1	-0.007	0.016	2,05

Technical Note. Setting function CAL 3 point ( 4,7,10 ).

The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 2,3 of 54

**This report is valid for the above stated instrument/s only.**

**CLC**

**### End of Certificate ###**

Certificate No. Q23100397

F3-011-04/01-12

page 3 of 3



@clccalibration

## CERTIFICATE OF CALIBRATION

### FOR

NOMENCLATURE : DIGITAL THERMO-HYGROMETER  
MANUFACTURER : EXTECH INSTRUMENTS  
MODEL / TYPE : 445814  
SERIAL NO. : PONPE5816745  
CLID. NO. : 232303263  
JOB CONTROL NO. : 230911100396

CUSTOMER : TNP ENVIRONMENT CO., LTD.  
332/173 MOO 3 TAMBON BANG RAK PHATTANA,  
AMPHOE BANG BUA THONG, NONTABURI 11110

DATE OF RECEIVED : 11 September 2023

DATE OF ISSUED : 15 September 2023

Report of calibration screening must not be taken in part. Except complete. Without the approval of the Calibration Laboratory Co., Ltd.

Calibrated By : Oranut Kamchatphai  
Calibration Engineer



Approved By : Mongkol Yotsoontorn  
Authorized Signatory

15 September 2023



This Calibration Certificate documents the traceability to national standards, which realize the units of measurement according to the  
International System of Units (SI)

Certificate No. Q23100396

F3-011-04/01-12

page 1 of 3



@clccalibration

## REPORT OF CALIBRATION

### FOR

**NOMENCLATURE** : **DIGITAL THERMO-HYGROMETER**  
**MANUFACTURER** : **EXTECH INSTRUMENTS**  
**MODEL / TYPE** : **445814**  
**SERIAL NO.** : **PONPE5816745**  
**DATE OF CALIBRATION** : **13 September 2023**

---

#### ENVIRONMENT CONDITIONS :

**Temperature** :  $(23 \pm 2) ^\circ\text{C}$

**Relative Humidity** :  $(55 \pm 10) \% \text{RH}$

#### PROCEDURE USED :

This instrument was calibrated under procedure No. **CLC-CPTH-11**. The calibration was performed by using Chilled Mirror Hygrometer and Temperature & Humidity Chamber which maintained by the Calibration Laboratory Co., Ltd.

#### REFERENCE STANDARD USED :

Chilled Mirror Hygrometer, Edgetech Model Dew Master S/N. 36151.

Temperature & Humidity Chamber, PGC Model 9141-5114 S/N.0802282.

#### TRACEABILITY :

The measurements are traceable to International System of Units (SI) , through Thunder Scientific Corporation.

Certificate No. 21028, Due Date 09 December 2023.

#### UNCERTAINTY :

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k = 2,00$  which for a normal distribution corresponds to a coverage probability of approximately 95 %.

It has been evaluated according to the "Evaluation of the Uncertainty of Measurement in Calibration (EA-4/02 M:2022)"

**Certificate No. Q23100396**

**F3-011-04/01-12**

page 2 of 3



@clccalibration

## CONDITION OF CALIBRATION ITEM : GOOD

## MEASUREMENT RESULTS : ( X ) without adjustment ( ) adjustment

The table in the following gives the calibration results and associated measurement uncertainties of the measuring digital thermo-hygrometer.

### CALIBRATION DATA

#### 1. CORRECTION OF TEMPERATURE

Test point ( ° C )	Actual Temperature ( ° C )	DUC Reading ( ° C )	Correction ( ° C )	Uncertainty ± ( ° C )
20.0	20.01	19.9	+0.11	0.27
25.0	25.01	25.2	-0.19	

#### 2. CORRECTION OF HUMIDITY

STD Temperature ( ° C )	STD Reading ( %RH )	DUC Reading ( %RH )	Correction ( %RH )	Uncertainty ± ( %RH )
25	50.0	47	+3.0	0.8

Note. The Scope of Accredited ANAB Certificate No. ACDM-2814 Version 008 Page 49 of 54

**This report is valid for the above stated instrument/s only.**

**### End of Certificate ###**

**Certificate No. Q23100396**

**F3-011-04/01-12**

page 3 of 3



@clccalibration



## Certificate of Calibration

**Certificate No. :** 67-400049-1

**Page : 1 of 2**

**Submitted by :** TNP Environment Co., Ltd.  
332/173 Moo 3 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

**Equipment :** Liquid in Glass Thermometer

Manufacturer :	SK	Model :	N/A
Range :	0 °C to 200 °C	Resolution :	1 °C
Serial No. :	N/A	Immersion :	Total
ID No. :	TNP.LAB.12		

**Environment :**

Ambient Temperature :	(23 ± 2) °C
Relative Humidity :	(50 ± 15) %
Line Voltage :	(220 ± 22) VAC

**Date of Received :** 26 January 2024

**Date of Calibration :** 01 February to 02 February 2024

**Date of Issue :** 02 February 2024

**Calibrated by :** Chortip Samchusri

**Calibration Method :** This instrument was calibrated by In-house method comparison technique CAL-M4001 based on ASTM E77-07 by compared with PRT in the liquid bath at the constant controlled temperature.

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units

1. Platinum Resistance Thermometer (PRT)

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400001	TT-0016-22	07 Feb 2024	National Institute of Metrology Thailand (NIMT)

2. Standard Digital Thermometer

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400003	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)
400004	23E1866	01 Jun 2025	National Institute of Metrology Thailand (NIMT)

Approved by :

( Surachai Promthong )

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



## Certificate of Calibration

**Certificate No. :** 67-400049-1

**Page :** 2 of 2

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

Ice point check : UUC\* reading 0 ° C Standard reading 0.8789 ° C

Standard Reading ( ° C )	UUC Reading ( ° C )	Correction ( ° C )	Uncertainty ( ± ° C )
21.2064	20	1.2	0.31
31.3084	30	1.3	0.31

### Remark

UUC : Unit Under Calibration

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- o0o -



**Certificate no:** H/T 670338

**Date of issue :** 21-Mar-24

**Instrument description** : Thermo-Hygrometer  
**Instrument model** : Extech 445815  
**Instrument serial no.** : PONPE5899554  
**ID no. or control no.** : TNP.LAB.21  
**Manufacturer** : Extech Instruments  
**Probe description** : -  
**Probe model** : -  
**Probe serial** : -  
**Customer name** : TNP ENVIRONMENT CO.,LTD.  
**Customer address** : 332/173 Moo 3 Tambon Bang Rak Phatthana, Amphoe Bang Bua Thong, Nonthaburi 11110

**Total pages of certificate** : 2 Pages  
**Receiving no.** : L-241004-1  
**Receiving date.** : 08-Mar-24  
**Parameter of calibration** : Temperature Calibration  
**Condition of UUC.** : Used  
**Ambient condition** : All of the Measurement were carried out the stabilized laboratory  
Temperature :  $23 \pm 5$  °C  
Humidity :  $55 \pm 15$  %RH  
**Calibration place** : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210  
**Calibration procedure no.** : This instrument was calibrated by comparison of indication with the Standard Thermo- hygrometer according to calibration Work Instruction no .WI-CL-11-C

*The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.*

*This certificate is applied only to item under test Environmental condition.*

*This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid.*

*This calibration certificate documents are tracebility to national standards, which realize measurement according to the International System of Units (SI).*

**Date of calibration** : 20-Mar-24



Mr. Peerawat Thongbai

**Calibration Technician**



Mrs. Nongluck Wongsettee

**Technical Manager**



**Certificate no:** H/T 670338

**Standard refereces**

Standard	Reference No.	Vendor	Due Date
ARALAB 300ECP,Fitoclima	S2023070040-001	MIT	07-Jul-24
Thermo HygroPalm HP 23-A	SG-H-00579/66	Success Gateway	16-Aug-24

**Measured room conditions**

**Temperature :** 22.1 °C

**Humidity :** 55.9 %RH

**Pressure :** 1019.3 mbar

**Calibration results (Without Adjustment)**

**Reference temperature :** - °C

Parameter of standard	Standard values	Mean of UUC.	Error	Uncertainty (±)
Temperature (°C)	19.97	20.1	0.13	0.50
Temperature (°C)	25.02	25.2	0.18	0.50
Temperature (°C)	29.99	30.2	0.21	0.50

**Remark :** -

**End of Report**



**Certificate no:** H 670285

**Date of issue :** 21-Mar-24

**Instrument description** : Thermo-Hygrometer  
**Instrument model** : Extech 445815  
**Instrument serial no.** : PONPE5899554  
**ID no. or control no.** : TNP.LAB.21  
**Manufacturer** : Extech Instruments  
**Probe description** : -  
**Probe model** : -  
**Probe serial** : -  
**Customer name** : TNP ENVIRONMENT CO.,LTD.  
**Customer address** : 332/173 Moo 3 Tambon Bang Rak Phatthana, Amphoe Bang Bua Thong, Nonthaburi 11110

**Total pages of certificate** : 2 Pages  
**Receiving no.** : L-241004  
**Receiving date.** : 08-Mar-24  
**Parameter of calibration** : Humidity Calibration  
**Condition of UUC.** : Used  
**Ambient condition** : All of the Measurement were carried out the stabilized laboratory  
Temperature :  $23 \pm 5$  °C  
Humidity :  $55 \pm 15$  %RH  
**Calibration place** : 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210

**Calibration procedure no.** : This instrument was calibrated by comparison of indication with the Standard Thermo- hygrometer according to calibration Work Instruction no .WI-CL-11-C

*The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurent Multiplied by coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.*

*This certificate is applied only to item under test Environmental condition.*

*This Calibration Certificate may not be reporduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid.*

*This calibration certificate documents are tracebility to national standards, which realize measurement according to the International System of Units (SI).*

**Date of calibration** : 19-Mar-24



Mr. Peerawat Thongbai

**Calibration Technician**



Mrs. Nongluck Wongsettee

**Technical Manager**

**Certificate no:** H 670285

**Standard references**

Standard	Reference No.	Vendor	Due Date
Thermo HygroPalm HP 23-A	SG-H-00579/66	Success Gateway	16-Aug-24
Hydrogen 2-XL	Performance	Entech	24-Mar-24

**Measured room conditions**

Temperature : 22.7 °C      Humidity : 56.7 %RH      Pressure : 1013.3 mbar.

**Calibration results (Without Adjustment)**

Reference temperature : 25.0 °C

Parameter of standard	Standard values	Mean of UUC.	Error	Uncertainty (±)
Humidity (%RH)	35.09	31	-4.09	1.3
Humidity (%RH)	50.03	48	-2.03	1.5
Humidity (%RH)	64.97	68	3.03	1.5

**Remark :** -

**End of Report**



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23M455

Page : 1 of 2

Equipment : Standard Weight Set

Manufacturer: -

Model : Class:F1

Serial No.: 15022021-01

ID No.: TNP.LAB.25

Condition As-Received: Used Item

Received Date: 02 March 2023

Calibration Date: 04 March 2023

Reference: 2303-0104WN

Submitted by: TNP ENVIRONMENT CO.,LTD.

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

Atmospheric Pressure: 1015.25 mbar

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

332/173 Moo 3, Bang Rak Phatthana, Bang Bua Thong,  
Nonthaburi 11110

**Procedure used:** Calibration were conducted using in-house calibration procedure CP-M01 according to comparison method against standard weights on the basis of weighings at an average air density of 1.2 kg/m<sup>3</sup> and a temperature of 23.4 °C material density of weight is 8000 kg/m<sup>3</sup>.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Weight Set (E2)	73336	20026	MM-0018-22	28 Feb 2024
2) Standard Weight Set (E2)	73338	20028	MM-0019-22	28 Feb 2024

2.This certificate is not certified for any commercial transaction.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained at:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Thapakorn Thammachai

Issue Date : 07 March 2023

Approved Signatory : \_\_\_\_\_

☐ Phalinee Prabpaipal

☒ Sura Suwannasri

☐ Chaowalit Rittirak

B 0309848





Cert No.: 23M455

Page: 2 of 2

**Result of calibration**

Nominal Value	Conventional mass		Uncertainty of Measurement ( $\pm$ )	Maximum Permissible error ( $\pm$ )
	Before Adjustment	After Adjustment		
200 g	199.99986 g	-	0.30 mg	1.0 mg
100 g	100.00015 g	-	0.16 mg	0.50 mg
50 g	50.00015 g	-	0.10 mg	0.30 mg
20 g	20.000116 g	-	0.080 mg	0.25 mg
10 g	10.000041 g	-	0.060 mg	0.20 mg
5 g	5.000010 g	-	0.050 mg	0.16 mg
2 g	1.999936 g	-	0.040 mg	0.12 mg
1 g	0.999973 g	-	0.030 mg	0.10 mg
200 mg	200.059 mg	200.007 mg	0.020 mg	0.060 mg
100 mg	100.037 mg	99.981 mg	0.016 mg	0.050 mg

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

a 1151188





# THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



## CALIBRATION CERTIFICATE

Certificate No.S2306518S

page 1 of 2

**Customer :** TNP ENVIRONMENT CO., LTD.  
332/173 Moo 3 Tambon Bang Rak Phatthana,  
Amphoe Bang Bua Thong, Nonthaburi 11110

**Equipment :** Non-automatic weighing instrument (Electronic instrument)

**Manufacturer :** Shimadzu **Order No. :** 66S2523-1

**Model :** AP225WD **Ambient temperature :**  $(26.9 \pm 5.0) ^\circ\text{C}$

**Accuracy class :** - **Relative humidity :**  $(52.0 \pm 10.0) \%$

**Capacity :** 10 g / 220 g **Received date :** 21-Jun-2023

**Resolution :** 0.00001 g / 0.0001 g **Date of calibration :** 21-Jun-2023

**Serial No. :** D316301848 **Date of issue :** 24-Jun-2023

**ID No. :** TNP.LAB.30 **Condition of the balance :** Good working conditions

**Place of calibration :** ห้อง LAB

### Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.


### Condition of reference standard weight

<u>Instrument</u>	<u>Nominal value</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due-date</u>	<u>Density (kg/m<sup>3</sup>)</u>
1 Standard weight set	1 mg to 2 kg	15885+15849	M2210001S	8-Oct-2023	7950

### Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By : Aekhasak Silarut  
Technician

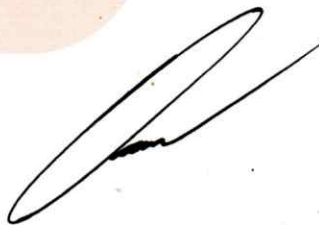Approved Signatory :   
Chonlatee Pongwatvisanon

This calibration certificate may not be reproduced other than in full,  
except with the prior written approval of the head of TCS calibration laboratory.



# THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



## CALIBRATION CERTIFICATE

Certificate No.S2306518S


page 2 of 2

### The repeatability of indication

Nominal Value ( g )	Standard Deviation of reading ( g )	Maximum difference between suscensive reading ( g )	n
100	0.000005	0.00001	5
200	0.00005	0.0001	5

### The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading ( g )
Point 1	100.0000
Point 2	100.0002
Point 3	100.0001
Point 4	100.0000
Point 5	100.0001
Eccentric Value	0.0002



### The error of indication

Nominal Value ( g )	Value of Reference Standard Weight ( g )	Balance Reading ( g )	Correction ( g )	Uncertainty (±) ( g )	k
Unload	0.00000	0.00000	0.00000	0.000016	2.32
0.1	0.10000	0.10003	-0.00003	0.000019	2.10
0.5	0.50000	0.50001	-0.00001	0.000023	2.04
1	1.00001	1.00000	+0.00001	0.000026	2.00
5	5.00000	5.00001	-0.00001	0.000038	2.00
10	9.99999	10.00001	-0.00002	0.000046	2.00
20	20.0000	20.0000	0.0000	0.000085	2.00
50	50.0000	50.0001	-0.0001	0.00011	2.00
100	100.0000	100.0000	0.0000	0.00018	2.00
200	200.0000	200.0004	-0.0004	0.00034	2.00

Remark : Adjustment, External weight nominal value 100 g, Standard weight of Lab

### Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor ( $k$ ), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

**This report will certify of the calibrated equipment only.**

--End--





# THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



## CALIBRATION CERTIFICATE

Certificate No.S2306519S

page 1 of 2

**Customer :** TNP ENVIRONMENT CO., LTD.

332/173 Moo 3 Tambon Bang Rak Phatthana,

Amphoe Bang Bua Thong, Nonthaburi 11110

**Equipment :** Non-automatic weighing instrument (Electronic instrument)

**Manufacturer :** Sartorius

**Order No. :** 66S2523-2

**Model :** SECURA224-1S

**Ambient temperature :**  $(26.8 \pm 5.0) ^\circ\text{C}$

**Accuracy class :** -

**Relative humidity :**  $(52.0 \pm 10.0) \%$

**Capacity :** 220 g

**Received date :** 21-Jun-2023

**Resolution :** 0.0001 g

**Date of calibration :** 21-Jun-2023

**Serial No. :** 0041305301

**Date of issue :** 24-Jun-2023

**ID No. :** TNP.LAB.31

**Condition of the balance :** Good working conditions

**Place of calibration :** ห้อง LAB

### Calibration method

This instrument was calibrated according to the EURAMET Calibration Guide No. 18.


### Condition of reference standard weight

<u>Instrument</u>	<u>Nominal value</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due-date</u>	<u>Density (kg/m<sup>3</sup>)</u>
1 Standard weight set	1 mg to 2 kg	15885+15849	M2210001S	8-Oct-2023	7950

### Traceability of the reference standard weight

This certificate is traceable to SI unit through Mass Calibration Laboratory Thai Calibration Services Co., Ltd., NSC-ONSC accredited no. Calibration 0189.

Calibrated By : Aekhasak Silarut  
Technician

Approved Signatory :   
Chonlatee Pongwatvisanon

This calibration certificate may not be reproduced other than in full,  
except with the prior written approval of the head of TCS calibration laboratory.



# THAI CALIBRATION SERVICES CO., LTD.

19/8 Moo 9 Soi Raiking 30 Puttamonthon 5 Rd., Sampran, Nakornpatom 73210

Tel. 0-3439-7682-5 Fax: 0-3439-7687

www.thaical.com E-mail : sale@thaicalibration.com, lab@thaicalibration.com



## CALIBRATION CERTIFICATE

Certificate No.S2306519S


page 2 of 2

### The repeatability of indication

Nominal Value ( g )	Standard Deviation of reading ( g )	Maximum difference between successive reading ( g )	n
200	0.00000	0.0000	5

### The effect of eccentric application of a load on the indication (test load : 100 g)

Position	Balance Reading ( g )
Point 1	100.0000
Point 2	100.0000
Point 3	100.0000
Point 4	99.9998
Point 5	99.9998
Eccentric Value	0.0002



### The error of indication

Nominal Value ( g )	Value of Reference Standard Weight ( g )	Balance Reading ( g )	Correction ( g )	Uncertainty (±) ( g )	k
Unload	0.0000	0.0000	0.0000	0.000082	2.00
0.1	0.1000	0.1000	0.0000	0.000083	2.00
0.5	0.5000	0.5000	0.0000	0.000084	2.00
1	1.0000	0.9999	+0.0001	0.000085	2.00
5	5.0000	5.0000	0.0000	0.000090	2.00
10	10.0000	10.0000	0.0000	0.000094	2.00
20	20.0000	20.0001	-0.0001	0.00011	2.00
50	50.0000	50.0001	-0.0001	0.00013	2.00
100	100.0000	100.0000	0.0000	0.00019	2.00
200	200.0000	199.9998	+0.0002	0.00033	2.00

Remark : Without adjustment

### Uncertainty of measurement

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor ( $k$ ), which for a normal distribution corresponds to a coverage probability of approximately 95% (confidence level).

**This report will certify of the calibrated equipment only.**

--End--



CERT.No.: HS-U039F

**Certificate of Calibration**

Calibration Date : 20 Jun 23  
 Submitted by : TNP ENVIRONMENT COMPANY LIMITED.  
 332/173 Moo. 3, Tambon Bang Rak Phatthana,  
 Amphoe Bang Bua Thong, Nonthaburi 11110

Avg Room Temp : 20 °C  
 Avg Water Temp : 20 °C  
 Air Pressure : 757.00 mmHg  
 Salinity : 0 ppt

Model : YSI 4010-2W  
 S/N : 22051520  
 Probe : YSI 4100  
 S/N : 22C102711  
 ID NO. : -  
 Air Temp ref : S/N. E00522  
 Barometric ref : S/N. E00522  
 Water Temp ref : S/N. 11431  
 Technician : Kittipong M.

**Calibration Details**

Calibration Point	100% air sat. (@20 °C, DO = 9.09 mg/l)	(status)	(status)
Measurement 1 (mg/l)	9.05	(PASS)	-
Measurement 2 (mg/l)	9.05	(PASS)	-
Measurement 3 (mg/l)	9.04	(PASS)	-
Measurement 4 (mg/l)	9.03	(PASS)	-
Measurement 5 (mg/l)	9.04	(PASS)	-
Measurement 6 (mg/l)	9.04	(PASS)	-
Measurement 7 (mg/l)	9.04	(PASS)	-
Measurement 8 (mg/l)	9.03	(PASS)	-
Measurement 9 (mg/l)	9.03	(PASS)	-
Measurement 10 (mg/l)	9.03	(PASS)	-
Mean Measurement	9.04	mg/l	-
Inaccuracy	0.05	mg/l	-

Overall Status (PASS)

**Manufacturer Specification**

Accuracy = +/- 0.2 mg/l

- 1) This certificate is issued based on the result that are found as shown on date and place of test only.
- 2) The calibration procedure followed in accordance with Harikul Science Co., Ltd.
- 3) This result shall not be used for advertising purpose.



Technician Signature

(Kittipong Maekwong)



Laboratory Manager

(Natenapha Pisatkunchon)

## Certificate of Calibration

**Certificate No. :** 66-400687-1

**Page : 1 of 2**

**Submitted by :** TNP Environment Co., Ltd.  
332/173 Moo 3 Bang Rak Phatthana, Bang Bua Thong, Nonthaburi 11110

**Equipment :** Air Chamber (Oven)  
Manufacturer : Memmert Model : UF75  
Range : N/A °C Resolution : 0.1 °C  
Serial No. : B320.0251 ID No. : N/A

**Environment :** On site calibration was carried out at the Laboratory, TNP Environment Co., Ltd.  
Ambient Temperature : (27.0 to 28.0) °C  
Relative Humidity : (45 to 50) %  
Line Voltage : (228.0 to 230.0) V

**Date of Received :** 11 December 2023

**Date of Calibration :** 11 December 2023

**Date of Issue :** 14 December 2023

**Calibrated by :** Permpon Chanpu

**Calibration Method :** CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

**Reference Standard Instruments :** This certification is traceable to the International System of Units  
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400023	66-400547-1	04 Apr 2024	National Institute of Metrology Thailand (NIMT)

Approved by :



( Surachai Promthong )

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



## Certificate of Calibration

**Certificate No. : 66-400687-1**


**Page : 2 of 2**

**Result of Calibration :** Without Adjustment

**UUC Condition As-Received :** Good

**Function :** Temperature measurement

This instrument was setting air ventilation at position 0 (close)

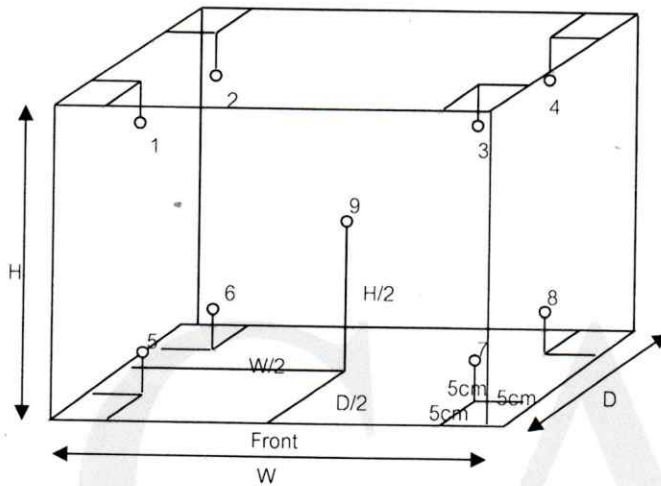

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.56 m

Capacity = 0.07 m<sup>3</sup>

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
85.0	85.0	85.0	85.3	85.1	85.2	85.1	85.0	84.8	84.7	84.7	85.0	0.64
104.0	104.0	104.0	104.3	104.2	104.3	104.1	104.0	103.8	103.7	103.7	104.0	0.69
180.0	180.0	180.0	179.5	179.9	180.0	179.8	179.9	179.4	178.9	179.4	180.0	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
85.0	85.0	85.0	0.4	0.1	0.8
104.0	104.0	104.0	0.4	0.1	0.8
180.0	180.0	180.0	1.4	0.3	1.6

**Remark** The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%

- o0o -

*Handwritten signature*







ID LINE : IEC17025



## Certificate of Calibration

Certificate Number : SPR23110535-2

Page : 1 of 3

Customer : TNP ENVIRONMENT CO.,LTD.

332/173 Moo.3, Bang Rak Phatthana, Bang Bua Thong, Nonthaburi  
11110

Equipment Name : Water Quality Meter

Manufacturer : Digicon

Model : WA-48SD

Serial Number : T.075714

ID. Number : TNP-LAB-46

### Environmental Conditions

Ambient Temperature :  $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$

Relative Humidity :  $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPC-04-01,  
SP-CPC-04-02,

Method of Calibration : SP-CPC-04-11

Received Date : 30 Nov 2023

Calibration Date : 19 Jan 2024

Recommend Due Date : 19 Jan 2025

Date of Issue : 20 Jan 2024

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Sarawut Khitmai

Calibration Officer

Approved by :

( Mr.Prayoon Topart )

Authorized Signatory





ID LINE : IEC17025



## Calibration Report

Certificate Number : SPR23110535-2

Page : 2 of 3

### Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Zero Oxygen Solution	HI7040L	Lot S0027-23 _	21C31	21 Mar 2028
Standard pH Solution	PH016.L5	Lot No.882984	61267077	20 Mar 2024
Standard pH Solution	PH107.L5	Lot No.882985	61275614	13 Apr 2024
Standard pH Solution	PH020.L5	Lot No.882986	61268050	20 Mar 2024
Conductivity Standard 84 uS/cm	CS84M0S.L5	Lot No.882987	61247444	20 Mar 2024
Conductivity Standard 1413 uS/cm	CS1413M0S.L5	Lot No.882988	61267992	20 Mar 2024
Conductivity Standard 12880 uS/cm	CS1288P1S.L5	Lot No.882989	61247253	20 Mar 2024
Sodium Chloride Standard Solution	RM003461L25	Lot No.841770	97756699	23 Sep 2024

### Traceability

This certification is traceable to the International System of Unit maintained at :  
HANNA - Hanna Instruments (Thailand) Ltd.

C.P.A. Chem - ANAB#AT-1836 (ISO/IEC 17025:2017) and ANAB#AR-1835 (ISO/IEC  
17034:2016)



ID LINE : IEC17025



## Result of Calibration

Certificate No. : SPR23110535-2

Page : 3 of 3

pH Measurement @ 25 °C

Unit : pH

Standard Solution	UUC Reading	Error	Uncertainty ( ± )
4.008	3.98	-0.028	0.014
6.984	7.01	0.026	0.012
10.011	10.02	0.009	0.018

Conductivity Measurement @ 25 °C

Standard Solution	UUC Reading	Error	Uncertainty ( ± )
84 µS/cm	84.6 µS/cm	0.6 µS/cm	0.60 µS/cm
1.413 mS/cm	1.415 mS/cm	0.002 mS/cm	0.0082 mS/cm
12.88 mS/cm	12.89 mS/cm	0.01 mS/cm	0.075 mS/cm

\* Dissolved Oxygen Permanance Test

Unit : mg/L

Actual Standard	UUC Reading	Error	Uncertainty ( ± )
0.0	0.0	0.0	0.13
5.0	4.9	-0.1	0.13
8.3	8.2	-0.1	0.13

Salinity Measurement

Unit : % Salinity

Actual Standard	UUC Reading	Error	Uncertainty ( ± )
5.0269	5.04	0.0131	0.015

### Note:


The result of calibration was found accurate as show on date and place of calibration only.  
 This Certificate is not certified for any commercial transaction.  
 Calibration Marked (\*) "Not ANAB Accredited " in this Certificate have been included for completeness.

### Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor  $k = 2$ , providing a level of confidence approximately 95%.

- End of Certificate -





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1099

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Autoclave

**Manufacturer :** Rexall

**Model :** LS-2D

**Serial No. :** 04131

**ID No. :** AUT-01

**Submitted by :** Environment & Laboratory Co.,Ltd.  
40 Soi Liangmueangnonthaburi 13,  
Talad Kwan, Mueang,  
Nonthaburi 11000

**Location :** Room No. 205

**Received Order :** 12 July 2023

**Calibration Date :** 12 July 2023

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Preecha Hlahib

**Approved by :**

*Malee*

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ✓ ) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 24 July 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056477





**Equipment :** Autoclave  
**Condition As-Received :** Used Item  
**Reference :** 2307-0094OC-7

**Cert. No.:** 23TM1099

**Page :** 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT03 according to direct measurement method with Data Acquisition which connected with Thermocouple Type T

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY41021843	22LM172	TPA	27 Dec 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.

4. This result of calibration covers laboratory autoclaves for the sterilization of goods and material which could be infected with organisms categorized as Hazard Group 1, 2 and 3\*\*

(\*\* = Categorization of pathogens according to hazard and categories of containment, second edition, 1990 )


It does not cover autoclaves for use with material infect with organisms in Hazard Group 4, for which complete containment and sterilization of infected condensate is considered to be essential.

This result of calibration does not apply to sterilizers or disinfectors used for medical, dental, pharmaceutical or veterinary purposes which are directly concerned with patient care, or those used for fabrics subjected to sterilization which are required to be dry at the end of cycle.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

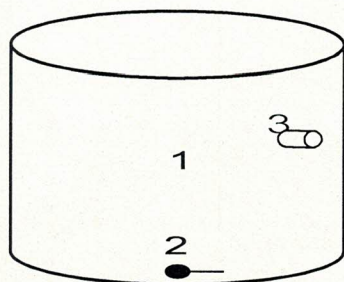

	<b>Environmental</b>		
	( °C )	( %R.H. )	( Volt )
<b>Beginning of Calibration</b>	30	55	220
<b>Finished of Calibration</b>	30	57	220

<u>Position</u>	<u>Description</u>	<u>Ref. Std. ID No.:</u>
1 =	Center of chamber	21-04TC-01
2 =	Temperature sensor	21-04TC-02
3 =	Exhaust port	21-04TC-03

*Malu .*





Equipment : Autoclave  
Condition As-Received : Used Item  
Reference : 2307-0094OC-7  
Result of Calibration :- ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 23TM1099

Page : 3 of 3

Operating parameter Set : Temperature = 121 °C  
Sterilization period = 15 minute

UUC* Setting ( °C )	UUC* Reading ( °C )	Position	Average* Standard Reading ( °C )	Stability ( ± °C )	Pressure Reading ( kg/cm <sup>2</sup> )	Uncertainty ( ± °C )	Coverage Factor <i>k</i>
121	-	1	121.837	0.89	1.2	1.3	2
		2	121.869				
		3	121.875				

**Average\*** : The average of 30 values in each position.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration


Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

*Malu.*





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1100

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Incubator

**Manufacturer :** Memmert

**Model :** BM 500

**Serial No. :** D593.0342

**ID No. :** CHI-002

**Submitted by :** Environment & Laboratory Co.,Ltd.  
40 Soi Liangmueangnonthaburi 13,  
Talad Kwan, Mueang,  
Nonthaburi 11000

**Location :** Room No. 204

**Received Order :** 12 July 2023

**Calibration Date :** 12 July 2023

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Preecha Hlahib

**Approved by :**

  
Approved Signatory

- ( ) Pornthippa Tameyakul  
(✓) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 24 July 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056478





Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2307-0094OC-4

Cert. No.: 23TM1100

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY41021843	22LM172	TPA	27 Dec 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	22	22
REL.Humid. ( % )	64	66
AC Supply ( Volt )	222	221

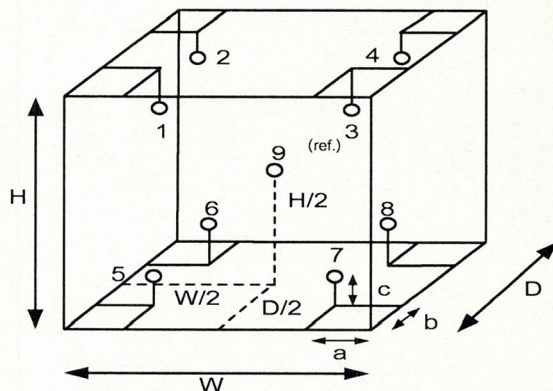

Position :	Ref. Std. ID No.:
1	18-04RTD-01
2	18-04RTD-02
3	18-04RTD-03
4	18-04RTD-04
5	18-04RTD-05
6	18-04RTD-06
7	18-04RTD-07
8	18-04RTD-08
9 (ref.)	18-04RTD-09

**Probe Installation Details :**

a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm

**Dimension of Chamber :**

D = 0.40 m  
W = 0.56 m  
H = 0.48 m  
Capacity = 0.11 m<sup>3</sup>

Malu.





**Equipment :** Incubator  
**Condition As-Received :** Used Item  
**Reference :** 2307-0094OC-4  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Not Available

**Cert. No.:** 23TM1100

**Page :** 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.040	0.27	0.48	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	35.021	34.900	35.010	35.284	34.853	34.919	34.945	34.964	35.089	0.30

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

Malu.





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1273

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Incubator

**Manufacturer :** Envilab-Intiligent

**Model :** -

**Serial No. :** -

**ID No. :** CHI-005

**Submitted by :** Environment & Laboratory Co.,Ltd.  
40 Soi Liangmueangnonthaburi 13,  
Talad Kwan, Mueang,  
Nonthaburi 11000

**Location :** Room No. 204

**Received Order :** 24 August 2023

**Calibration Date :** 24 August 2023

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Preecha Hlahib

**Approved by :**

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ) Ponpan Paipim  
( ☒ ) Suwit Imjai

**Issue Date :** 29 August 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0057741





Equipment : Incubator  
 Condition As-Received : Used Item  
 Reference : 2308-0600OC-1

Cert. No.: 23TM1273

Page : 2 of 3

**Procedure Used :-**

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY44035217	22LM170	TPA	16 Dec 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Not Available

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	23	23
REL.Humid. ( % )	50	54
AC Supply ( Volt )	220	220

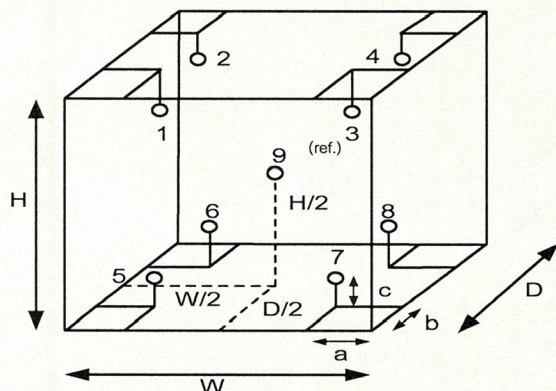

Position :	Ref. Std. ID No.:
1	18-10RTD-01
2	18-10RTD-02
3	18-10RTD-03
4	18-10RTD-04
5	18-10RTD-05
6	18-10RTD-06
7	18-10RTD-07
8	18-10RTD-08
9 (ref.)	18-10RTD-09

**Probe Installation Details :**

a = 5.0 cm  
 b = 5.0 cm  
 c = 5.0 cm

**Dimension of Chamber :**

D = 0.40 m  
 W = 0.70 m  
 H = 1.0 m  
 Capacity = 0.28 m<sup>3</sup>

*Yunt*

a 1176747





Equipment : Incubator  
Condition As-Received : Used Item  
Reference : 2308-0600OC-1  
**Result of Calibration :-** ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source  
Fresh air setting : Not Available

Cert. No.: 23TM1273

Page : 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
35.0	35.0	35.0	0.47	1.2	1.8	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
35.0	34.805	34.737	34.701	34.435	34.724	34.783	35.228	35.604	34.816	0.71

**Average\*** : The average of 30 values in each position.

**Temperature stability** : One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation** : The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\*** : Unit Under Calibration


Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

*Qunt*





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CHO420

Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Spectrophotometer  
**Manufacturer :** Hach  
**Model :** DR 3900  
**Serial No. :** 1988383  
**ID No. :** SPE-002  
**Condition As-Received:** Used Item  
**Received Date :** 12 July 2023  
**Calibration Date :** 12 July 2023  
**Reference :** 2307-0094OC-11  
**Submitted by :** Environment & Laboratory Co.,Ltd.  
40 Soi Liangmueangnonthaburi 13  
Talat Kwan, Mueang, Nonthaburi 11000  
**Calibration Place :** Room No. 304  
**Ambient Temperature :** ( 26.7 - 26.9 ) °C (On-Site)  
**Relative Humidity :** ( 57.2 - 51.2 ) % (On-Site)  
**Calibration Procedure :** In - house method :  
CP-OCH4 based on ASTM E 275-01  
**Calibrated by :** Kunchit Promprat

**Approved by :**

Approved Signatory

- (✓) Malee Butkruea  
( ) Saithip Meangmai  
( ) Warakorn Lernagtrakul

**Issue Date :** 24 July 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056486





Cert. No. : 23CHO420

Page : 2 of 3

**Condition of calibration result**

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	32587	100509	28 Mar 2024
2. Absorbance Standard set	32590	100508	28 Mar 2024
3. Absorbance Standard set	8331	105939	28 Sep 2024
4. Wavelength Standard set	29829	94776	02 Sep 2023
5. Wavelength Standard set	29829	94777	02 Sep 2023

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained at :

- National Physical Laboratory (NPL), The United Kingdom of Great Britain and Northern Ireland
- National Institute of Standards and Technology (NIST), The United States of America

4. Spectral BandWidth : 5 nm  
Scan Speed : - nm/min

**Calibration Results : without adjustment**

**Wavelength Accuracy**

<b>Certified Values of Reference Material ( nm )</b>	<b>UUC Reading ( nm )</b>	<b>Uncertainty of Measurement ( <math>\pm</math> nm )</b>	<b>Coverage Factor <i>k</i></b>
361.40	361	0.59	2.00
447.20	446	0.59	2.00
537.00	536	0.59	2.00
638.00	637	0.59	2.00
740.51	741	0.59	2.00
807.04	807	0.59	2.00

Maku





Cert. No. : 23CHO420

Page : 3 of 3

**Calibration Results : without adjustment**

**Photometric Accuracy**

Wavelength (nm)	Certified Values of Reference Material ( Abs )	UUC Reading ( Abs )	Uncertainty of Measurement ( $\pm$ Abs )	Coverage Factor <i>k</i>
350.0	Zero	0.000	0.0046	2.00
	0.4246	0.423	0.0061	2.00
	Zero	0.000	0.0050	2.00
	0.6385	0.633	0.0055	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5607	0.560	0.0030	2.00
	0.7336	0.733	0.0030	2.00
	1.0636	1.063	0.0030	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5224	0.522	0.0028	2.00
	0.6856	0.684	0.0029	2.00
	0.9937	0.992	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5397	0.538	0.0028	2.00
	0.6832	0.680	0.0028	2.00
	0.9886	0.985	0.0028	2.00

**Remark**

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer
- The Potassium Dichromate filled cells are measured against a Perchloric acid blank.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k* , providing a level of confidence of approximately 95 %.

-o0o-

*Malu.*





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert. No.: 23TM1173

Page : 1 of 3

## Certificate of Calibration

**Equipment :** Water Bath

**Manufacturer :** Memmert

**Model :** WB 22

**Serial No. :** I505.0053

**ID No. :** WAB-01

**Submitted by :** Environment & Laboratory Co.,Ltd.  
40 Soi Liangmueangnonthaburi 13,  
Talad Kwan, Mueang,  
Nonthaburi 11000

**Location :** Room No. 303

**Received Order :** 12 July 2023

**Calibration Date :** 12 - 13 July 2023

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Khit Ruttanaprapachai

**Approved by :**

*Malee*

Approved Signatory

- ( ) Pornthippa Tameyakul  
( ✓ ) Malee Butkruea  
( ) Suwit Imjai

**Issue Date :** 24 July 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0056487





**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2307-0094OC-3

**Cert. No.:** 23TM1173

**Page :** 2 of 3

**Procedure Used :-**

Calibration were conducted using in-house calibration procedure CP-OT04 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY44073381	23LM95	TPA	19 May 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	Environmental		AC Voltage Supply
	( °C )	( %R.H. )	( Volt )
Beginning of Calibration	30	47	220
Finished of Calibration	31	50	221

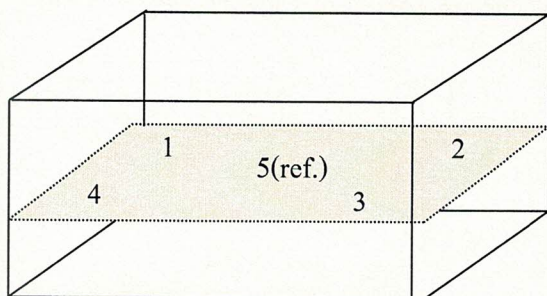

Front

Position :	Ref. Std. S/N.:
1	4803988-006
2	4803988-007
3	4804539-014
4	4804539-015
5(ref.)	4804539-016

Mahu.





Equipment : Water Bath  
Condition As-Received : Used Item  
Reference : 2307-0094OC-3  
**Result of Calibration :-** ( \* ) Without Adjustment  
Function of UUC\* : Temperature Source

Cert. No.: 23TM1173

Page : 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty  ( ± °C )
			Position					
			1	2	3	4	5 (ref.)	
44.5	44.5	44.5	44.507	44.503	44.498	44.509	44.502	0.15
60.0	60.0	60.0	59.914	59.928	59.912	59.899	59.894	0.15

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <i>k</i>
44.5	0.039	0.023	2
60.0	0.098	0.042	2

**Average\*** : The average of 30 values in each position.

**Uniformity** : The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability** : One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\*** : Unit Under Calibration

**Note** : The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-

*Malu.*





## CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2419

Site Calibration

Order No. 24060337

**Customer** Bureau Veritas AQ Lab (Thailand) Limited  
111 Thailand Science Park  
Moo 9 Paholyothin Rd., Klong 1, Klong Luang, Pathumthani 12120 Thailand

**Place of Calibration** Prepare Culture Media

**Description** Autoclave

**Model** VE-65

**Serial No.** 7202

**ID.No.** CHM000206

**Date of Receipt** Jun 26, 2024

**Date of Calibration** Jun 26, 2024

### Environment

Temperature	(Min)	22.1	°C	(Max)	25.5	°C
Relative Humidity	(Min)	42.7	%RH	(Max)	56.3	%RH

### Calibration Method

WI-22 : The reference thermometer was placing into the chamber and measurement based on BS-2646.  
The temperature scale in use at this laboratory is the International Temperature Scale of 1990.



## CALIBRATION CERTIFICATE


Date of Issue Jun 28, 2024

Cert No. 24/2419

Site Calibration

Order No. 24060337

Results (without adjustment)

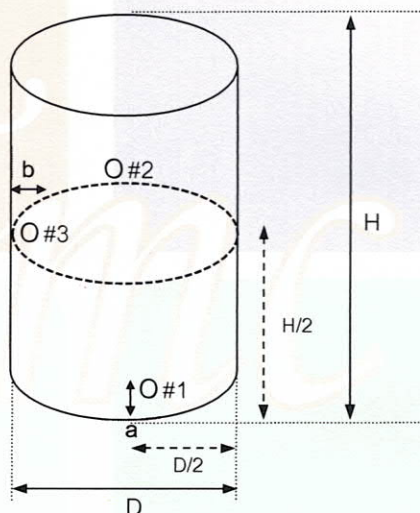

Position of reference thermometers were placed

### Note.

- 1). Duration of the holding time was 45 minutes.
- 2). Stability - greatest one half of difference between max peak and min peak of each reference probe measured temperature obtained during the calibration interval.
- 3). Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.





## CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2419

Site Calibration

Order No. 24060337

### Results (without adjustment)

UUC Setting (°C)	UUC Reading		Reference Thermometer (°C)		Stability ±(°C)	Uniformity (°C)	Uncertainty ±(°C)
	(°C)	(KPa)					
115.0	115.3	179.6	Position 1	115.58	0.25	0.15	0.70
			Position 2	115.58			
			Position 3	115.48			

UUC Setting (°C)	UUC Reading		Reference Thermometer (°C)		Stability ±(°C)	Uniformity (°C)	Uncertainty ±(°C)
	(°C)	(KPa)					
121.0	121.4	211.0	Position 1	121.59	0.20	0.13	0.70
			Position 2	121.60			
			Position 3	121.52			

### Standard

1) Standard Datalogger with RTD Model. HiTemp. 140-PT S/N. R32397, Certificate No. QR23-1962, Calibrated by Quality Reborn Co., Ltd., ONAC Calibration No. 0292. Due Date Aug 07, 2024.

2) Standard Datalogger with RTD Model. HiTemp. 140-PT S/N. R32398, Certificate No. QR23-1963, Calibrated by Quality Reborn Co., Ltd., ONAC Calibration No. 0292. Due Date Aug 07, 2024.

3) Standard Datalogger with RTD Model. HiTemp. 140-PT S/N. R32399, Certificate No. QR23-1964, Calibrated by Quality Reborn Co., Ltd., ONAC Calibration No. 0292. Due Date Aug 07, 2024.

This certificate is traceable to SI unit.



## CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2419

Site Calibration



Order No. 24060337

The stability and uniformity was taken into account in the measurement uncertainty stated.

The above results are valid exclusively for calibration samples as mentioned in the report.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with ONAC requirements.

APPROVED SIGNATORY :

-  
- ☐ MR. PRAJUCKPETCH THONGSOOKCHOTE  
☐ MR. DAMRONG MULSING  
☒ MR. JATURAPAT THONGSOOKCHOTE


Thermology



Autoclave

Model. VE-65 S/N. 7202 ID.No. CHM000206

Cert.No. 24/2419

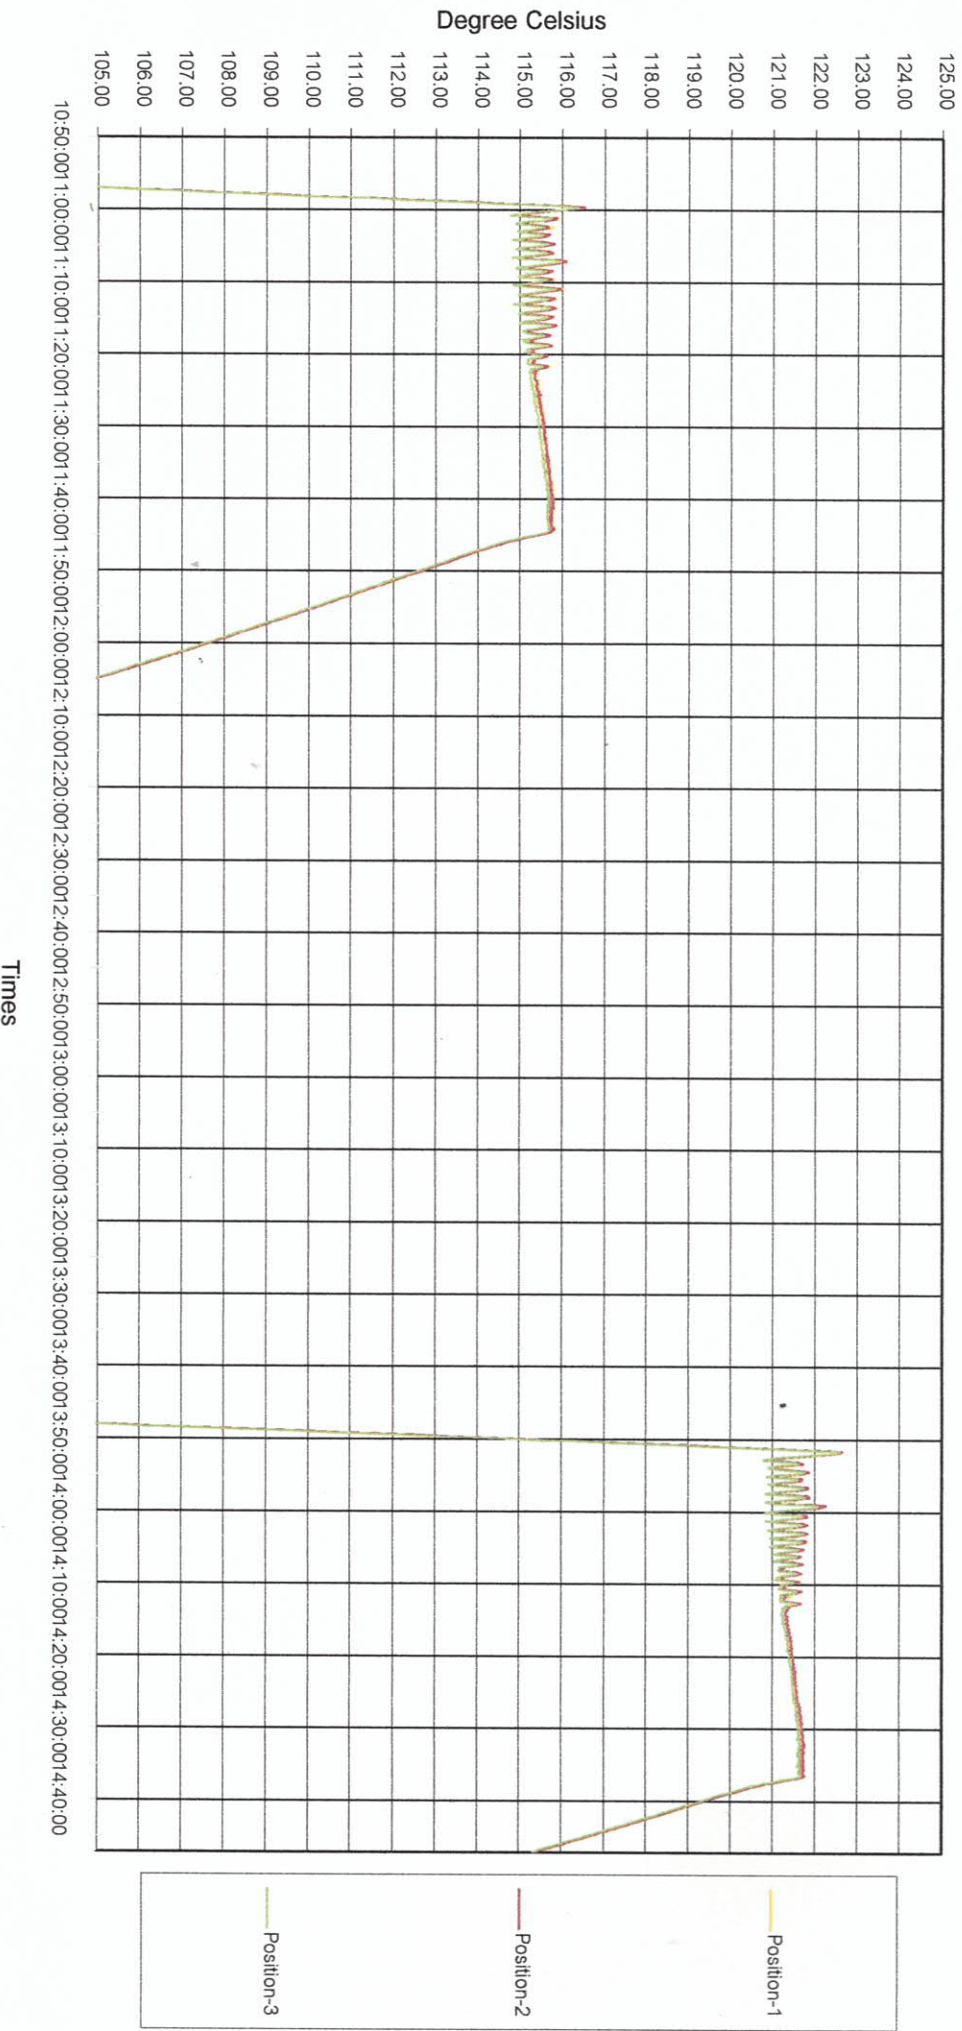

28.7



## CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2418

Site Calibration

Order No. 24060337

**Customer** Bureau Veritas AQ Lab (Thailand) Limited  
111 Thailand Science Park  
Moo 9 Paholyothin Rd., Klong 1, Klong Luang, Pathumthani 12120 Thailand

**Place of Calibration** Incubation Room

**Description** Water Bath

**Model** SC100

**Serial No.** 0152187501160414

**ID.No.** CHM000205

**Date of Receipt** Jun 24, 2024

**Date of Calibration** Jun 24, 2024

### Environment

<b>Temperature</b>	(Min)	22.8	°C	(Max)	25.2	°C
<b>Relative Humidity</b>	(Min)	44.1	%RH	(Max)	58.5	%RH
<b>Line Voltage</b>	(Min)	227.2	VAC	(Max)	229.6	VAC

### Calibration Method

WI-18 : The reference thermometer was placed into the chamber and measurement was performed based on AS-2853.

The temperature scale in use at this laboratory is the International Temperature Scale of 1990.

### Standard

1) Data Acquisition with Sensor Model 34972A S/N. MY49007789, Certificate No. QR24-0186, Calibrated by Quality Reborn Co., Ltd., ONAC Calibration No. 0292. Due Date Jan 23, 2025.

This certificate is traceable to SI unit.






## CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024  
Site Calibration

Cert No. 24/2418  
Order No. 24060337

Results (without adjustment)

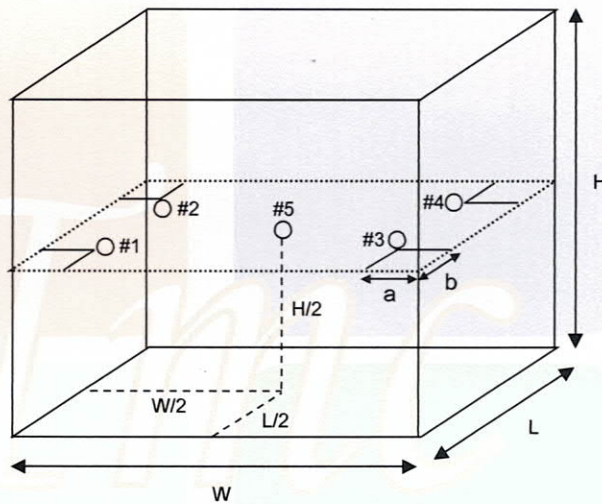

Position of reference thermometers were placed

### Note.

- 1). Dimension (W x L x H) is 30 x 34 x 20 cm.
- 2). Stability - greatest one half of difference between max peak and min peak of each reference probe measured temperature obtained during the calibration interval.
- 3). Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.



## CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2418

Site Calibration

Order No. 24060337

Results (without adjustment)


Cal Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)		Stability $\pm$ (°C)	Uniformity (°C)	Uncertainty $\pm$ (°C)
44.5	44.5	44.5	Position 1	44.490	0.020	0.043	0.13
			Position 2	44.494			
			Position 3	44.491			
			Position 4	44.499			
			Position 5	44.503			

The stability and uniformity was taken into account in the measurement uncertainty stated.

The above results are valid exclusively for calibration samples as mentioned in the report.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with ONAC requirements.

APPROVED SIGNATORY :


  
☐ MR. PRAJUCKPETCH THONGSOOKCHOTE  
☐ MR. DAMRONG MULSING  
☒ MR. JATURAPAT THONGSOOKCHOTE



Cert.No. 24/2418

Water Bath

Model. SC100 S/N. 0152187501160414 ID.No. CHM000205

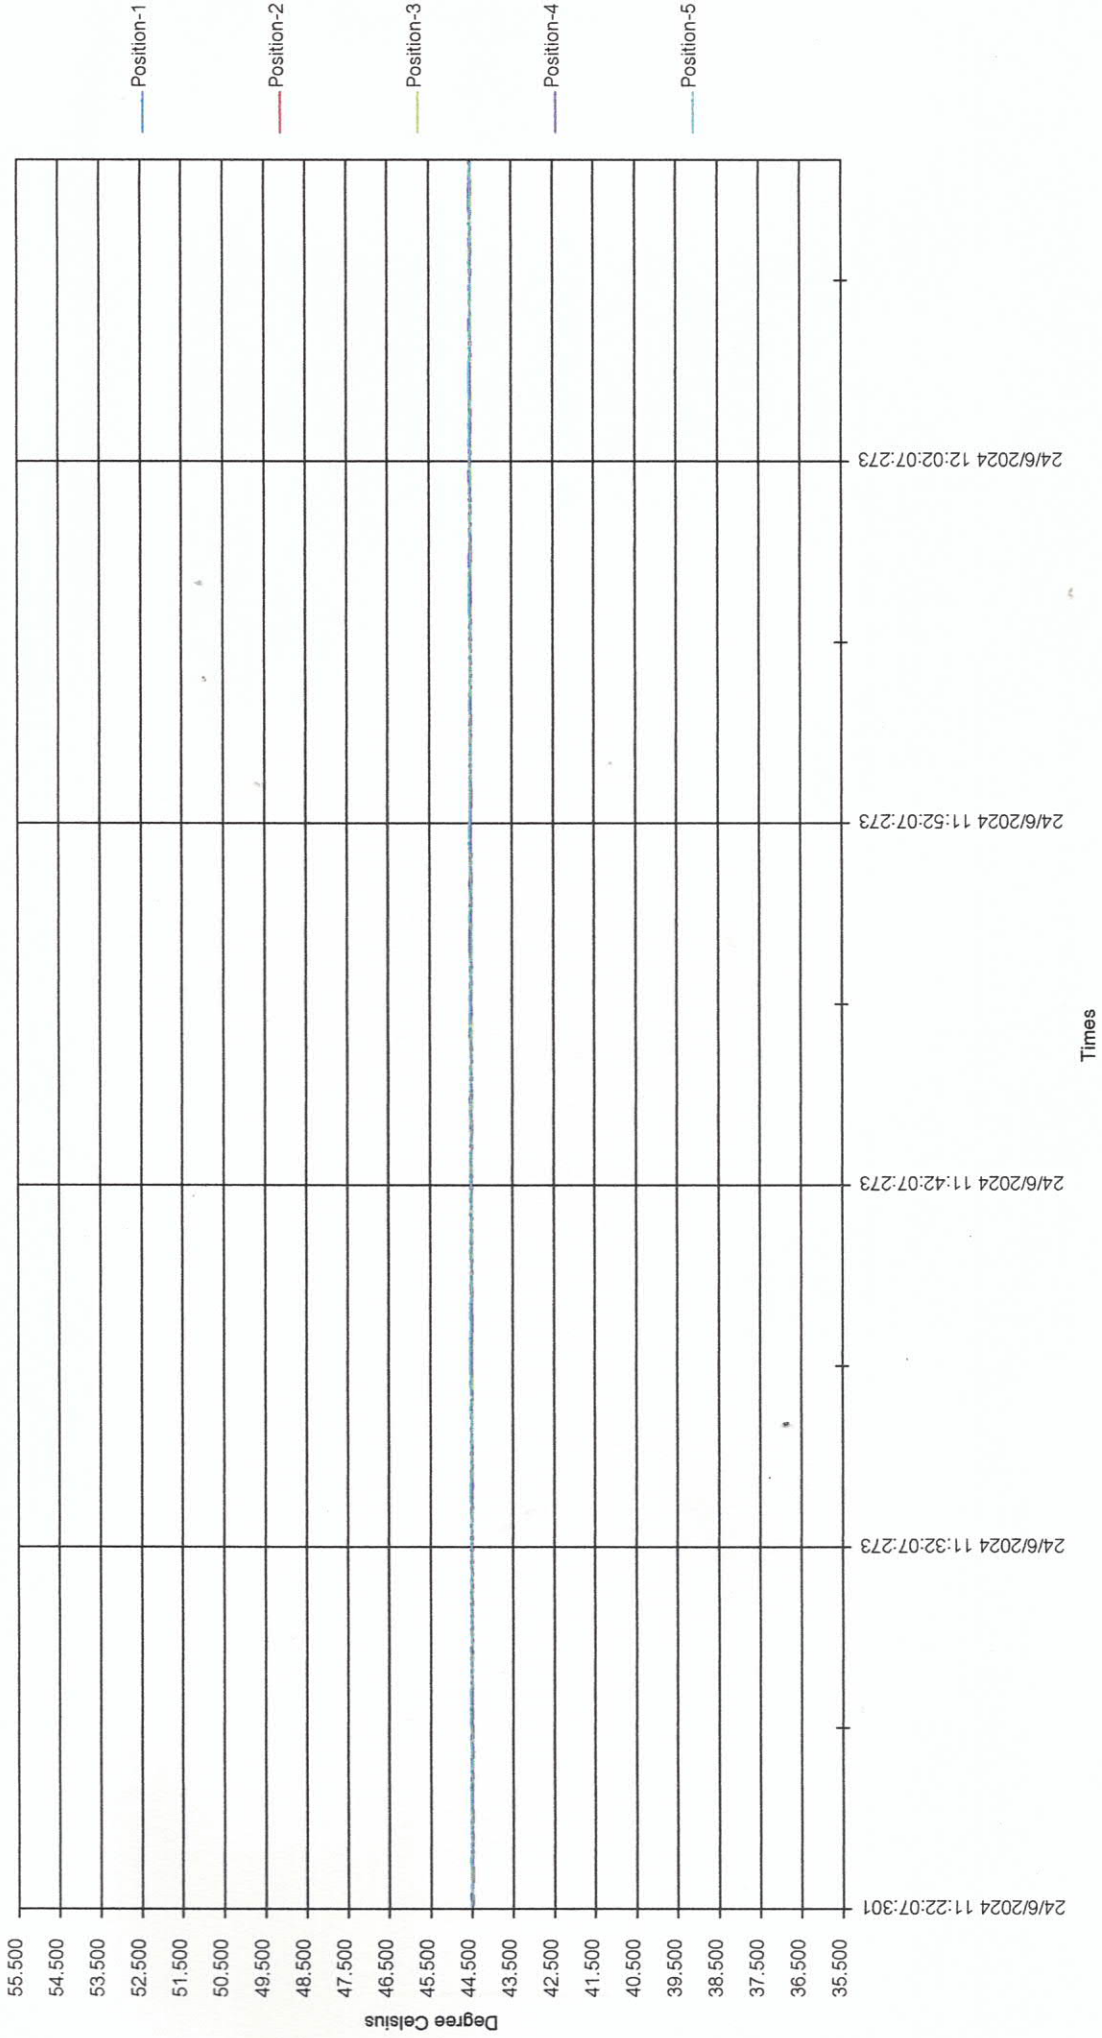

Handwritten signature and initials.



## CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2415

Site Calibration

Order No. 24060337

**Customer** Bureau Veritas AQ Lab (Thailand) Limited  
111 Thailand Science Park  
Moo 9 Paholyothin Rd., Klong 1, Klong Luang, Pathumthani 12120 Thailand

**Place of Calibration** Incubation Room

**Description** Incubator

**Model** IN110

**Serial No.** D415.0797

**ID.No.** CHM000181

**Date of Receipt** Jun 24, 2024

**Date of Calibration** Jun 24, 2024

**Environment**

**Temperature** (Min) 22.8 °C (Max) 25.2 °C

**Relative Humidity** (Min) 44.1 %RH (Max) 58.5 %RH

**Calibration Method**

WI-17 : The reference thermometer was placed into the chamber and measurement was performed based on AS-2853.

The temperature scale in use at this laboratory is the International Temperature Scale of 1990.

**Standard**

1) Data Acquisition with Sensor Model 34972A S/N. MY49010059, Certificate No. QR24-0874, Calibrated by Quality Reborn Co., Ltd., ONAC Calibration No. 0292. Due Date Apr 24, 2025.

This certificate is traceable to SI unit.






## CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024  
Site Calibration

Cert No. 24/2415  
Order No. 24060337

Results (without adjustment)

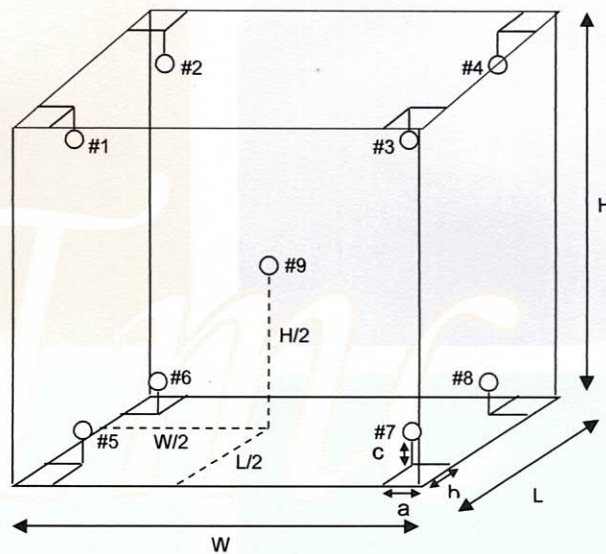

Position of reference thermometers were placed

### Note.

- 1). Dimension (W x L x H) is 56 x 40 x 48 cm.
- 2). Stability - greatest one half of difference between max peak and min peak of each reference probe measured temperature obtained during the calibration interval.
- 3). Uniformity - the maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady state conditions. The reference sensor should preferably be located at the geometric center of the chamber.



## CALIBRATION CERTIFICATE

Date of Issue Jun 28, 2024

Cert No. 24/2415

Site Calibration

Order No. 24060337

Results (without adjustment)

Cal Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Reference Thermometer (°C)		Stability $\pm$ (°C)	Uniformity (°C)	Uncertainty $\pm$ (°C)
35.0	35.0	35.0	Position 1	35.138	0.067	0.253	0.30
			Position 2	35.099			
			Position 3	35.075			
			Position 4	35.187			
			Position 5	35.173			
			Position 6	34.988			
			Position 7	34.878			
			Position 8	34.965			
			Position 9	34.970			

The stability and uniformity was taken into account in the measurement uncertainty stated.

The above results are valid exclusively for calibration samples as mentioned in the report.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with ONAC requirements.

APPROVED SIGNATORY :

☐ MR. PRAJUCKPETCH THONGSOOKCHOTE


☐ MR. DAMRONG MULSING

☒ MR. JATURAPAT THONGSOOKCHOTE



Incubator  
Model: IN110 S/N: D415.0797 ID.No: CHM000181

Cert.No. 24/2415

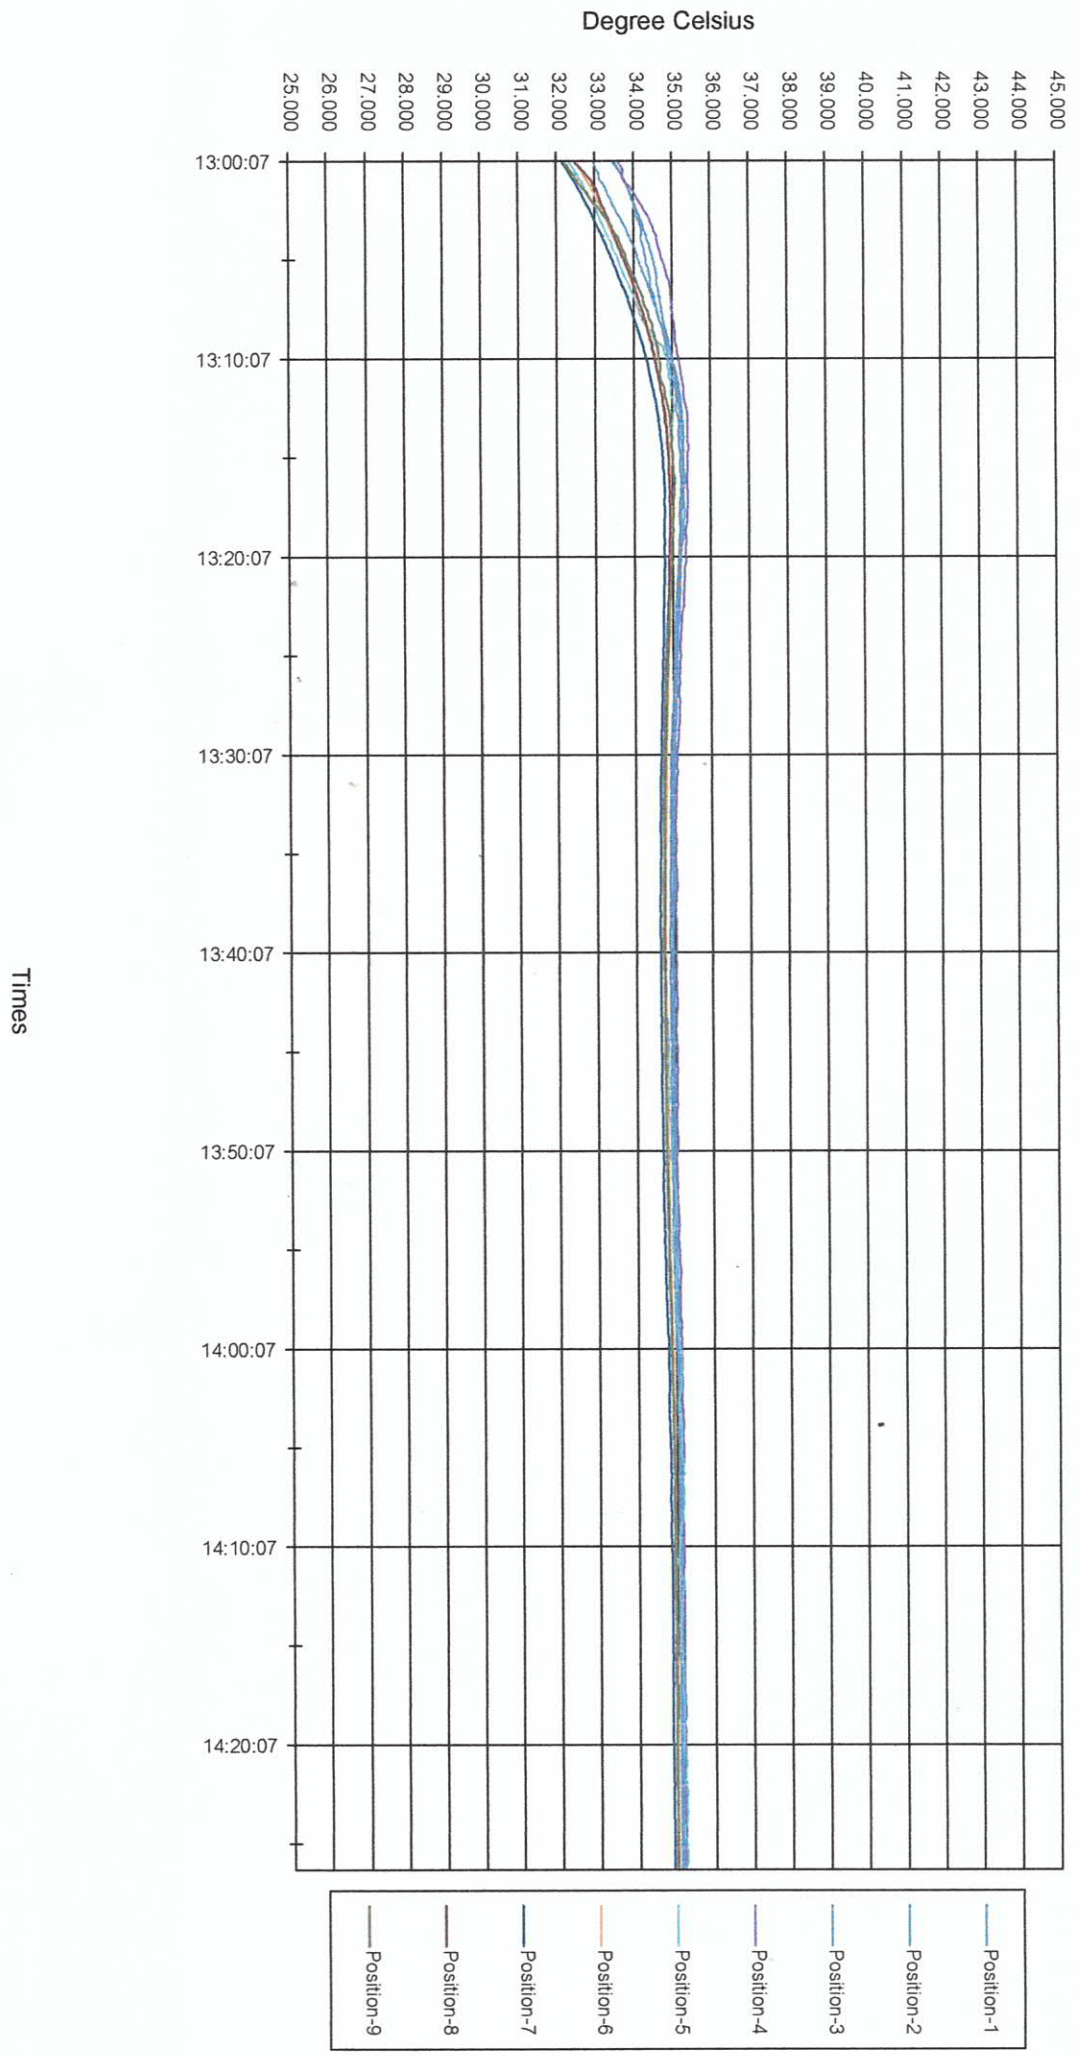

*Handwritten signature*



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CHO565

Page.: 1 of 3

## Certificate of Calibration

**Equipment :** Spectrophotometer  
**Manufacturer :** Merck  
**Model :** Prove 100  
**Serial No. :** 1904113676  
**ID No. :** S2019025  
**Condition As-Received:** Used Item  
**Received Date :** 21 September 2023  
**Calibration Date :** 21 September 2023  
**Reference :** 2309-0483OC-2  
**Submitted by :** SGS (Thailand) Limited  
1/209, 1/211 Moo 1, Ban Chang,  
Ban Chang, Rayong 21130  
**Calibration Place :** Spectrophotometry Lab  
**Ambient Temperature :** ( 23.8 - 20.9 ) °C (On-Site)  
**Relative Humidity :** ( 50.1 - 50.2 ) % (On-Site)  
**Calibration Procedure :** In - house method :  
CP-OCH4 based on ASTM E 275-01

**Calibrated by :** Kunchit Promprat

**Approved by :**

Approved Signatory

- ☒ Saithip Meangmai  
☐ Warakorn Lerngagtrakul  
☐ Ponpan Paipim

**Issue Date :** 26 September 2023

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.





Cert. No. : 23CHO565

Page : 2 of 3

**Condition of calibration result**

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	39130	106269	10 Oct 2024
2. Wavelength Standard set	36730	98330	19 Jan 2024
3. Wavelength Standard set	36730	98331	19 Jan 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained through :  
- Starna Scientific Ltd.

4. Spectral BandWidth : 4 nm  
Scan Speed : - nm/min

**Calibration Results : without adjustment**

**Wavelength Accuracy**

<b>Certified Values of Reference Material ( nm )</b>	<b>UUC Reading ( nm )</b>	<b>Uncertainty of Measurement ( <math>\pm</math> nm )</b>	<b>Coverage Factor <i>k</i></b>
418.48	418.5	0.15	2.00
513.70	513.1	0.14	2.00
536.90	536.3	0.14	2.00
637.94	637.6	0.14	2.00
879.70	878.8	0.15	2.00

*Saithip*



Cert. No. : 23CHO565

Page : 3 of 3

**Calibration Results : without adjustment**

**Photometric Accuracy**

Wavelength (nm)	Certified Values of Reference Material ( Abs )	UUC Reading ( Abs )	Uncertainty of Measurement ( $\pm$ Abs )	Coverage Factor $k$
440.0	Zero	0.000	0.0028	2.00
	0.5645	0.563	0.0028	2.00
	0.6988	0.698	0.0028	2.00
	1.0017	1.001	0.0028	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5281	0.527	0.0028	2.00
	0.6962	0.696	0.0028	2.00
	0.9984	0.998	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5699	0.569	0.0028	2.00
	0.7606	0.760	0.0028	2.00
	1.0927	1.092	0.0028	2.00

**Remark**

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

*Saithip*



## Verification COD Reactor

Equipment Name	Dri-Block Heater-Digital	Temperature Ver.	150±2 °C
Serial No.	000827-A	Model	DB 200/3
Reference Standard	Thermocouple Type K	Certificate No.	21/4272
Calibration Date	10/03/2023	Next Cal. Date	10/03/2024

<b>Left</b>											
Hole 1				Hole 2				Hole 3			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.1	-0.36	150.7	1	150.6	-0.36	150.2	1	151.4	-0.36	151.0
2	150.8	-0.36	150.4	2	151.7	-0.36	151.3	2	151.3	-0.36	150.9
3	151.2	-0.36	150.8	3	151.1	-0.36	150.7	3	151.7	-0.36	151.3
		Mean	150.67			Mean	150.77			Mean	151.11
		SD	0.208			SD	0.551			SD	0.208
		%RSD	0.138			%RSD	0.365			%RSD	0.138

Hole 4				Hole 5				Hole 6			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.7	-0.36	151.3	1	150.5	-0.36	150.1	1	151.5	-0.36	151.1
2	151.6	-0.36	151.2	2	151.3	-0.36	150.9	2	151.4	-0.36	151.0
3	151.5	-0.36	151.1	3	150.6	-0.36	150.2	3	150.5	-0.36	150.1
		Mean	151.24			Mean	150.44			Mean	150.77
		SD	0.100			SD	0.436			SD	0.551
		%RSD	0.066			%RSD	0.290			%RSD	0.365

Hole 7				Hole 8				Hole 9			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.3	-0.36	150.9	1	151.7	-0.36	151.3	1	150.5	-0.36	150.1
2	151.0	-0.36	150.6	2	150.5	-0.36	150.1	2	151.2	-0.36	150.8
3	151.3	-0.36	150.9	3	151.4	-0.36	151.0	3	150.8	-0.36	150.4
		Mean	150.84			Mean	150.84			Mean	150.47
		SD	0.173			SD	0.624			SD	0.351
		%RSD	0.115			%RSD	0.414			%RSD	0.233

Hole 10				Hole 11				Hole 12			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.6	-0.36	151.2	1	151.5	-0.36	151.1	1	150.7	-0.36	150.3
2	151.6	-0.36	151.2	2	151.2	-0.36	150.8	2	151.6	-0.36	151.2
3	150.8	-0.36	150.4	3	151.5	-0.36	151.1	3	151.2	-0.36	150.8
		Mean	150.97			Mean	151.04			Mean	150.81
		SD	0.462			SD	0.173			SD	0.451
		%RSD	0.306			%RSD	0.115			%RSD	0.299

Verified By Hatirat L. Approved By Jaipin R.

**Confidential** - Not to be photocopied except by permission of the Laboratory Quality Manager or nominee.

## Verification COD Reactor

Equipment Name      Dri-Block Heater Digital  
 Serial No.              000827-A  
 Reference Standard    Thermocouple Type K  
 Calibration Date       10/03/2023

Temperature Ver        150±2 °C  
 Model                    DB 200/3  
 Certificate No.         21/4272  
 Next Cal. Date         10/03/2024

**Middle**

Hole 1				Hole 2				Hole 3			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.2	-0.36	150.8	1	150.7	-0.36	150.3	1	151.1	-0.36	150.7
2	151.5	-0.36	151.1	2	151.7	-0.36	151.3	2	151.6	-0.36	151.2
3	151.6	-0.36	151.2	3	150.8	-0.36	150.4	3	150.9	-0.36	150.5
		Mean	151.07			Mean	150.71			Mean	150.84
		SD	0.208			SD	0.551			SD	0.361
		%RSD	0.138			%RSD	0.365			%RSD	0.239

Hole 4				Hole 5				Hole 6			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.5	-0.36	151.1	1	151.6	-0.36	151.2	1	150.5	-0.36	150.1
2	150.7	-0.36	150.3	2	151.2	-0.36	150.8	2	150.6	-0.36	150.2
3	151.6	-0.36	151.2	3	151.2	-0.36	150.8	3	151.2	-0.36	150.8
		Mean	150.91			Mean	150.97			Mean	150.41
		SD	0.493			SD	0.231			SD	0.379
		%RSD	0.327			%RSD	0.153			%RSD	0.252

Hole 7				Hole 8				Hole 9			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151.5	-0.36	151.1	1	151.5	-0.36	151.1	1	151.2	-0.36	150.8
2	150.5	-0.36	150.1	2	151.7	-0.36	151.3	2	150.9	-0.36	150.5
3	150.8	-0.36	150.4	3	151.1	-0.36	150.7	3	151.4	-0.36	151.0
		Mean	150.57			Mean	151.07			Mean	150.81
		SD	0.513			SD	0.306			SD	0.252
		%RSD	0.341			%RSD	0.202			%RSD	0.167

Hole 10				Hole 11				Hole 12			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	151	-0.36	150.6	1	151.5	-0.36	151.1	1	151.2	-0.36	150.8
2	150.6	-0.36	150.2	2	150.6	-0.36	150.2	2	150.5	-0.36	150.1
3	151.5	-0.36	151.1	3	151.0	-0.36	150.6	3	151.1	-0.36	150.7
		Mean	150.67			Mean	150.67			Mean	150.57
		SD	0.451			SD	0.451			SD	0.379
		%RSD	0.299			%RSD	0.299			%RSD	0.251

Verified By

Hafiqat L

Approved By

Jaifai R

**Confidential** - Not to be photocopied except by permission of the Laboratory Quality Manager or nominee.



## Verification COD Reactor

Equipment Name	Dri-Block Heater Digital	Temperature Ver	150±2 °C
Serial No.	000827/A	Model	DB 200/3
Reference Standard	Thermocouple Type K	Certificate No.	21/4272
Calibration Date	10/03/2023	Next Cal. Date	10/03/2024

Right

Hole 1				Hole 2				Hole 3			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	149.9	-0.36	149.5	1	150.3	-0.36	149.9	1	151.0	-0.36	150.6
2	151.1	-0.36	150.7	2	151.0	-0.36	150.6	2	151.0	-0.36	150.6
3	150.9	-0.36	150.5	3	149.9	-0.36	149.5	3	150.4	-0.36	150.0
		Mean	150.27			Mean	150.04			Mean	150.44
		SD	0.643			SD	0.557			SD	0.346
		%RSD	0.428			%RSD	0.371			%RSD	0.230

Hole 4				Hole 5				Hole 6			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	150.8	-0.36	150.4	1	150.0	-0.36	149.6	1	150.5	-0.36	150.1
2	151.0	-0.36	150.6	2	150.0	-0.36	149.6	2	150.8	-0.36	150.4
3	150.9	-0.36	150.5	3	150.7	-0.36	150.3	3	149.8	-0.36	149.4
		Mean	150.54			Mean	149.87			Mean	150.01
		SD	0.100			SD	0.404			SD	0.513
		%RSD	0.066			%RSD	0.270			%RSD	0.342

Hole 7				Hole 8				Hole 9			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	150.8	-0.36	150.4	1	151.1	-0.36	150.7	1	150.2	-0.36	149.8
2	150.9	-0.36	150.5	2	150.7	-0.36	150.3	2	150.2	-0.36	149.8
3	151.0	-0.36	150.6	3	151.1	-0.36	150.7	3	149.9	-0.36	149.5
		Mean	150.54			Mean	150.61			Mean	149.74
		SD	0.100			SD	0.231			SD	0.173
		%RSD	0.066			%RSD	0.153			%RSD	0.116

Hole 10				Hole 11				Hole 12			
NO.	Result			NO.	Result			NO.	Result		
	temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.		temp. °C	Corr.	temp+Corr.
1	150.6	-0.36	150.2	1	150.5	-0.36	150.1	1	150.9	-0.36	150.5
2	150.5	-0.36	150.1	2	150.9	-0.36	150.5	2	150.0	-0.36	149.6
3	149.9	-0.36	149.5	3	151.1	-0.36	150.7	3	150.5	-0.36	150.1
		Mean	149.97			Mean	150.47			Mean	150.11
		SD	0.379			SD	0.306			SD	0.451
		%RSD	0.252			%RSD	0.203			%RSD	0.300

Verified By

Habirul L

Approved By

Sanjay R

**Confidential** - Not to be photocopied except by permission of the Laboratory Quality Manager or nominee.

## สรุปผลการ Verify

ปรับอุณหภูมิ 154.0 °C แต่คนควบคุมอุณหภูมิ 150 ± 2 °C ทุกครั้ง

Verified By

Hatairat L.

Approved By

Sajjai R.

**Confidential** - Not to be photocopied except by permission of the Laboratory Quality Manager or nominee.





**ARCHEMICA**

## **Certificate of Calibration**

**Aquion RFIC : Anion System (ID#1054)**

**This certificate is to verify that instrument below are calibrated  
by**

**Archemica Lab Co.,Ltd.**

**Aquion**

**S/N 220380025**

**AS-DV**

**S/N 2203880170**

**For**

**SGS (Thailand) Limited (Rayong Branch).**



**ARCHEMICA LAB**  
**บริษัท อาร์เคมีกา แล็บ จำกัด**  
**ARCHEMICA LAB CO.,LTD.**

**Operator Signature:     วิสรรค์กมล**

**Date: 15 / Nov / 2023**

**(Mr. Itsaraphap Bumrunjeam)**

**Applications Chemist**



## MAINTENANCE AND TEST CERTIFICATE MODEL

### Avio220 Max

<b>Customer :</b> <u>SGS(Thailand)Limited</u> <u>Rayong Branch</u> <b>Address :</b> <u>1/209 , 1/211 Moo 1,</u> <u>T. Banchang, A. Banchang</u> <u>Rayong 21130</u> <b>User Name</b> <u>Khun Saijai Ruangsawat</u> <b>Phone:</b> <u>+66(0)38685260-64</u> <b>Email:</b> <u><a href="mailto:saijai.ruangsawat@sgs.com">saijai.ruangsawat@sgs.com</a></u>	<b>Date Tested:</b> <u>January 10, 2024</u> <b>Recommendation Recertification</b> <b>Period</b> <u>6</u> <b>Months</b> <b>Recertification Due:</b> <u>July 10, 2024</u> <b>Date Last Certified:</b> <u>N/A</u> <b>Visit Number:</b> <u>1OF2 W</u> <b>PerkinElmer Phone:</b> <u>02-719-6420 ext 206</u> <b>PerkinElmer Fax:</b> <u>02-318-5597</u>
--	--

#### CONFIGURATION TESTED

<b>MODEL</b>	<b>SERIAL NUMBER</b>	<b>SOFTWARE</b>
<u>AVIO200 MAX</u>	<u>M79S2304111</u>	<u>Syngristix V5</u>
<b>TESTED EQUIPMENT</b>	<b>CALIBRATION NUMBER</b>	<b>EXPIRATION</b>
<u>IPV Methods</u>		
<b>TEST STANDARD USED</b>	<b>PART NUMBER</b>	<b>EXPIRATION DATE</b>
<u>Multielement Standard</u>	<u>N069-1579</u>	<u>30-Dec-24</u>
<u>Instrument Cal. STD4</u>	<u>N930-0221</u>	<u>30-Nov-24</u>
<b>CUSTOMER SUPPLIED</b>	<b>COMMENTS</b>	<b>CUSTOMER INITIALS</b>
<u>2 % HNO3</u>		
<u>10 % HNO3</u>		





**MAINTENANCE AND TEST CERTIFICATE MODEL**  
**Avio220 Max**

**SERIAL NUMBER** M79S2304111**DATE TESTED** January 10, 2024**1. MECHANICAL CHECKS**

A. Inspect and clean all fans and filters.

☐ OK

B. Inspect and replace as necessary, all torch components including the RF coil.

☐ OK

C. Inspect all tubing for sign of clacking or leaking.

☐ OK

D. Adjust water and gas pressure regulator settings.

☐ OK

E. Inspect and leak check pneumatics drawers.

☐ OK

F. Clean the exterior of the instrument.

☐ OK**2. OPTICAL CHECKS**

A. Inspect and clean all optical components.

☐ OK

B. As required, check and replace all purgebfilters.

☐ OK

C. Recheck optical alignment.

☐ OK**3. COOLING SYSTEM CHECKS**

A. Perform preventive maintenance on chiller.

☐ OK

B. Flush out the chiller every year.

☐ OK**4. PERFORMANCE CHECKS**

A. Torch View Alignment.

☐ OK

B. Wavelength Calibration.

☐ OK



## MAINTENANCE AND TEST CERTIFICATE MODEL

### Avio220 Max

SERIAL NUMBER <u>M79S2304111</u>		DATE TESTED <u>January 10, 2024</u>	
PARAMETER	SPECIFICATION		FINAL VALUE
Spectral Resolution : UV			
As 193.696 nm	≤ 0.009 nm	<u>0.00864</u> nm	
Ni 231.604 nm	≤ 0.011 nm	<u>0.01009</u> nm	
Ni 341.476 nm	≤ 0.015 nm	<u>0.01169</u> nm	
Spectral Resolution : VIS			
Ba 455.403 nm	≤ 0.020 nm	<u>0.01776</u> nm	
Precision			
Zn 206.200 nm	% RSD ≤ 1.0 %	<u>0.28</u> %	
Mg 280.271 nm	% RSD ≤ 1.0 %	<u>0.73</u> %	
Mg 285.213 nm	% RSD ≤ 1.0 %	<u>0.61</u> %	
Ba 455.403 nm	% RSD ≤ 1.0 %	<u>0.54</u> %	
Detection Limits : Axial			
Tl 190.801 nm	3(sd)	<u>1.52</u> ppb	
As 193.696 nm	3(sd)	<u>1.4</u> ppb	
Se 196.026 nm	3(sd)	<u>1.53</u> ppb	
Pb 220.353 nm	3(sd)	<u>1.72</u> ppb	
Detection Limits : Radial			
As 193.696 nm	3(sd)	<u>1.69</u> ppb	
Zn 213.857 nm	3(sd)	<u>0.42</u> ppb	
Mn 257.610 nm	3(sd)	<u>0.1</u> ppb	
La 379.478 nm	3(sd)	<u>0.61</u> ppb	
Ba 455.403 nm	3(sd)	<u>0.13</u> ppb	
Ba 493.408 nm	3(sd)	<u>0.1</u> ppb	
BEC : Axial (IB X 1000)/(IS-IB)			
Mn 257.610 nm	≤ 30 ppb	<u>7.83</u> ppb	
BEC : Radial (IB X 1000)/(IS-IB)			
Mn 257.610 nm	≤ 30 ppb	<u>17.57</u> ppb	



**SERIAL NUMBER M79S2304111**      **DATE TESTED**    **January 10, 2024**

Commissioning follow as commissioning performance sheets.

☒

□

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Customer Service Engineer:

( Wiphan Promlumda )

Page 4 of 4