



ICP02329207

MAINTENANCE AND TEST CERTIFICATE MODEL
OPTIMA 8000

SERIAL NUMBER : 078S1411171C DATE TESTED : May 18, 2023

PARAMETER	SPECIFICATION			FINAL VALUE	
Spectral Resolution : UV	As	193.696 nm	≤ 0.009 nm	0.00720	nm
	Ni	231.604 nm	≤ 0.011 nm	0.00892	nm
	Ni	341.476 nm	≤ 0.015 nm	0.01343	nm
Spectral Resolution : VIS	Ba	455.403 nm	≤ 0.020 nm	0.01726	nm
Precision	Zn	206.200 nm	% RSD ≤ 1.0 %	0.35	%
	Mg	280.271 nm	% RSD ≤ 1.0 %	0.19	%
	Mg	285.213 nm	% RSD ≤ 1.0 %	0.19	%
	Ba	455.403 nm	% RSD ≤ 1.0 %	0.13	%
Detection Limits : Axial	Tl	190.801 nm	3(SD) ppb ≤ 10 ppb	1.54	ppb
	As	193.696 nm	3(SD) ppb ≤ 10 ppb	2.10	ppb
	Se	196.026 nm	3(SD) ppb ≤ 5.0 ppb	2.43	ppb
	Pb	220.353 nm	3(SD) ppb ≤ 3.0 ppb	1.40	ppb
Detection Limits : Radial	As	193.696 nm	3(SD) ppb ≤ 60 ppb	4.44	ppb
	Zn	213.857 nm	3(SD) ppb ≤ 2.0 ppb	0.12	ppb
	Mn	257.610 nm	3(SD) ppb ≤ 1.0 ppb	0.05	ppb
	La	379.478 nm	3(SD) ppb ≤ 3.0 ppb	0.21	ppb
	Ba	455.403 nm	3(SD) ppb ≤ 0.3 ppb	0.01	ppb
	Ba	493.408 nm	3(SD) ppb ≤ 0.6 ppb	0.01	ppb
BEC : Axial (IB X 1000)/(IS-IB)	Mn	257.610 nm	≤ 30 ppb	6.83	ppb
BEC : Radial (IB X 1000)/(IS-IB)	Mn	257.610 nm	≤ 30 ppb	9.29	ppb

Page 3 of 4



ICP02329207

MAINTENANCE REPORT AND IPV TEST CERTIFICATE
OPTIMA 8000

SERIAL NUMBER : 078S1411171C DATE TESTED : May 18, 2023

Remarks :

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested



meets



does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department PerkinElmer Ltd.

Authorized Representative :



Customer Support Engineer

Page 4 of 4



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 23H2216

Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: EQL-064

Condition As-Received: Used Item

Received Date: 12 October 2023

Calibration Date: 17 October 2023

to 20 October 2023

Reference: 2310-0447DN

Submitted by: TEST TECH CO.,LTD. (HEAD Office)

Ambient Temperature: (25 ± 3) °C

Relative Humidity: (50 ± 20) %

30, 32 Rama II Soi 63, Rama II Rd.,

Samaedam, Bangkhunthian, Bangkok 10150

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Handheld Thermometer With Sensor	1523	3240076	23I305	15 Mar 2024
2) Dew Point Hygrometer	Optidew 401	164756	TH-0158-22	13 Dec 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

-National Institute of Metrology Thailand (NIMT)

Calibrated by [Redacted]
Issue Date : 26 October 2023

Approved Signatory : [Redacted]

B 0327545



Cert. No.: 23H2216

Page.: 2 of 2

Result of Calibration:-

Without Adjustment

Function:

Humidity Measurement

Reference Temperature	Standard Humidity	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(%R.H.)	(%R.H.)	(%R.H.)	(±%R.H.)
25.0	30.1	30.0	-0.1	1.5
25.0	40.1	39.0	-1.1	1.5
25.0	50.1	49.0	-1.1	1.7
25.0	60.0	59.0	-1.0	1.7
25.0	75.2	75.5	0.3	1.8

Result of Calibration:-

Without Adjustment

Function:

Temperature Measurement

Standard Temperature	UUC* Reading	Error	Uncertainty of Measurement
(°C)	(°C)	(°C)	(±°C)
15.046	15.0	-0.046	0.72
19.975	20.0	0.025	0.72
25.022	25.0	-0.022	0.72
30.000	30.0	0.000	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor k = 2.00, providing confidence level approximately 95%.

-o-o-

a 1185882



CERTIFICATE No : 23M6754
REFERENCE No : 69854-1

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
MODEL : BP210S
SERIAL No : S0736477
ID No : EQL-008
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD.,
SAMAEDAM, BANGKHUNTHIAN, BANGKOK
10150

CALIBRATED BY : 
CALIBRATION DATE : 13-Jul-23

APPROVED BY : 
ISSUED DATE : 17-Jul-23
RECEIVED DATE : 13-Jul-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV 03



CERTIFICATE No : 23M6754

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : DIGITAL BALANCE
MANUFACTURER : SARTORIUS
ID No : EQL-008
AIR PRESSURE : 1011mbar \pm 1mbar
AMBIENT TEMPERATURE : 23° C \pm 1° C
MODEL : BP210S
S/N : S0736477
RECEIVED DATE : 13-Jul-23
CALIBRATION DATE : 13-Jul-23
RELATIVE HUMIDITY : 50 %RH \pm 10 % RH

CONDITION OF THIS RESULTS OF CALIBRATION

1. THIS INSTRUMENT WAS CALIBRATED BY ACCORDING TO UKAS LAB 14 EDITION 6:2019 BY USING KNOWN WEIGHT STANDARD WEIGHT. THE BALANCE WAS ADJUSTED USING INTERNAL WEIGHT TO ADJUST. THE BALANCE HAS NO ZERO TRACKING FUNCTION. REPEATABILITY WAS MEASURED BY USING 10 REPEATED MEASUREMENTS. LINEARITY WAS MEASURED COVERING 10 POINTS, EVENLY SPREAD OVER THE RANGE. THE INSTRUMENT WAS SET ZERO BEFORE PERFORMING THE LINEARITY TEST. OFF-CENTER LOADING WAS MEASURED BY USING STANDARD WEIGHTS PLACED ON THE PAN AND MOVED TO VARIOUS POSITIONS ON THE PAN. THE INTERNAL WEIGHT WAS CHECKED BY USING

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) STANDARD WEIGHT SET	E2	QK-I-151	M2302013S	02-Feb-25
2) STANDARD WEIGHT	E2	I5843	M2302014S	02-Feb-25

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.

4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.

5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-

- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH CENTRAL BUREAU OF WEIGHTS&MEASURES

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT

1. ZERO SETTING FUNCTION : NORMAL


2. TARE FUNCTION : NORMAL

3. REPEATABILITY OF READING AT 200 g WAS 0 g

4. DEPARTURE FROM NOMINAL VALUE/ LINEARITY

NOMINAL VALUE (g)	BALANCE READING (g)	CORRECTION (g)	UNCERTAINTY (\pm g)
0.0	0.0000	0.0000	0.000082
0.1	0.1000	0.0000	0.000083
0.2	0.2000	0.0000	0.000083
0.5	0.5000	0.0000	0.000083
1.0	1.0000	0.0000	0.000084
2.0	2.0000	0.0000	0.000084
5.0	5.0000	0.0000	0.000086
10.0	10.0000	0.0000	0.000089
20.0	20.0001	-0.0001	0.000094
50.0	49.9999	0.0001	0.00012
100.0	99.9999	0.0001	0.00019
200.0	199.9997	0.0003	0.00032

5. OFF CENTER LOADING ERROR



POINT	READING (g)
1	99.9998
2	99.9997
3	99.9998
4	99.9998
5	99.9998
OFF-CENTER LOADING	0.0001

6. INTERNAL WEIGHT ERROR : -0.000499999999988177 g

NOTE: THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA

THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.

END OF CALIBRATION REPORT



F-G010 REV 03



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584
www.qcalibration.com



CERTIFICATE No : 23T8798
REFERENCE No : 70515-6

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UFE 500
SERIAL No : G508.0791
ID No : EQL-128
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : 
CALIBRATION DATE : 11-Sep-23

APPROVED BY : 
ISSUED DATE : 15-Sep-23
RECEIVED DATE : 11-Sep-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 03



QUALITY CALIBRATION CO.,LTD.
235 Petchkasem 63/2 Road, Laksong, Bangkai, Bangkok 10160
Tel (662) 421-5402, (662) 444-0152-3, Fax (662) 809-4584

CERTIFICATE No : 23T8798

PAGE : 2 OF 2

Calibration Report


EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UFE 500
ID No : EQL-128
RECEIVED DATE : 11-Sep-23
AMBIENT TEMPERATURE : 24 °C ± 1 °C
S/N : G508.0791
CALIBRATION DATE : 11-Sep-23
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION

- THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.
- REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	23T6636	10-Jul-24
3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.				
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.				
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:- - NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.				

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT



GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 10
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

CHAMBER PERFORMANCE

Calibrate Piont (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	104.49	0.28	0.66	0.93
180.0	180.25	0.32	0.62	1.11

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.46	104.13	104.45	104.28	104.57	104.67	104.60	104.58	104.67	0.38
180.0	180.0	180.27	179.85	180.41	179.93	180.19	180.54	180.41	180.51	180.13	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.
NOTE 2: LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k =2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.
END OF CALIBRATION REPORT




CERTIFICATE No : 23T8799
REFERENCE No : 70515-7

PAGE : 1 OF 2

Certificate of Calibration

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UFE 500
SERIAL No : G512.2005
ID No : EQL-161
CONDITION AS RECEIVED : USED ITEM
SUBMITTED BY : TEST TECH CO., LTD.
30,32 RAMA II SOI 63, RAMA II RD., SAMAEDAM,
BANGKHUNTHIAN, BANGKOK 10150

CALIBRATED BY : 
CALIBRATION DATE : 11-Sep-23

APPROVED BY : 
ISSUED DATE : 15-Sep-23
RECEIVED DATE : 11-Sep-23

THIS CERTIFICATE MAY NOT BE REPRODUCED OTHER THAN IN FULL EXCEPT WITH THE PRIOR WRITTEN APPROVAL OF
QUALITY CALIBRATION CO., LTD.

F-G010 REV : 03



CERTIFICATE No : 23T8799

PAGE : 2 OF 2

Calibration Report

EQUIPMENT : HOT AIR OVEN
MANUFACTURER : MEMMERT
MODEL : UFE 500
ID No : EQL-161
RECEIVED DATE : 11-Sep-23
AMBIENT TEMPERATURE : 24 °C ± 1 °C
S/N : G512.2005
CALIBRATION DATE : 11-Sep-23
RELATIVE HUMIDITY : 51 %RH ± 10 %RH

CONDITION OF THIS RESULTS OF CALIBRATION


1. THIS INSTRUMENT WAS CALIBRATED ACCORDING TO TLAS G-20 BY COMPARISON WITH CALIBRATED RTD Pt100 UNDER NO LOAD CONDITION. THE TEMPERATURE PROBES WERE PLACED ON NINE POINTS AND LOCATED ONE THERMOMETER PROBE IN EACH OF THE EIGHT CORNERS OF THE CHAMBER AND WAS AWAY FROM THE EACH WALL OF 5 cm TO 10 cm. AND PLACED THE NINTH THERMOMETER PROBE WITHIN 2.5 cm. OF THE GEOMETRIC CENTER OF THE CHAMBER. THE UNIFORMITY WAS MEASURED BETWEEN REFERENCE PROBE AND OTHER PROBES AT THE SAME TIME.

2. REFERENCE STANDARD INSTRUMENTS :-

INSTRUMENT	MODEL	SERIAL No	CERTIFICATE No	DUE DATE
1) DATA LOGGER WITH RTD	HYDRA 2635A	7301307	23T6636	10-Jul-24

3. THE CERTIFICATE IS VALID FOR THE ITEM CALIBRATED AS SHOWN ON THE DATE AND PLACE OF CALIBRATION ONLY.
4. THIS RESULT EXCLUDE LONG TERM STABILITY OF THE UNIT UNDER CALIBRATION.
5. THIS CERTIFICATE IS TRACEABLE TO THE INTERNATIONAL SYSTEM OF UNIT MAINTAINED AT:-
- NATIONAL INSTITUTE OF METROLOGY (THAILAND) THROUGH QUALITY CALIBRATION CO.,LTD.

RESULT OF CALIBRATION :- WITHOUT ADJUSTMENT



GENERAL INFORMATION

Overall Ambient Temperature around the Chamber (°C) variation : 1
Overall Line Voltage (V) variation : 10
Instrument Condition : Normal
Chamber Size (W*L*H): 56*40*48 cm

CHAMBER PERFORMANCE

Calibrate Piont (°C)	Average All Position Temp. (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
104.0	103.96	0.14	0.58	0.73
180.0	179.55	0.22	0.93	1.47

TEMPERATURE MEASUREMENT ACCURACY TEST

Controller Temp (°C)	Indicating Temp (°C)	Measured Temperature (°C) at Spread Locations									Uncertainty (± °C)
		#1	#2	#3	#4	Ref. 5	#6	#7	#8	#9	
104.0	104.0	104.16	104.13	104.20	103.98	103.76	103.76	104.06	103.71	103.93	0.38
180.0	180.0	179.73	179.89	180.04	179.54	179.30	178.98	179.75	178.97	179.77	1.1

NOTE 1 : THE UNCERTAINTY OF MEASUREMENT EXCLUDED TEMPERATURE UNIFORMITY OF THE CHAMBER.
NOTE 2 : LOCATION 5 WAS REFERENCE LOCATION.

NOTE 3 : THIS CALIBRATION WAS CARRIED OUT AT THE CUSTOMER'S PLACE AT LABORATORY AREA.
THE REPORTED UNCERTAINTY OF MEASUREMENT WAS BASED ON A STANDARD UNCERTAINTY MULTIPLIED BY A COVERAGE FACTOR k=2, PROVIDING A LEVEL OF CONFIDENCE APPROXIMATELY 95%.
END OF CALIBRATION REPORT

Certificate of Calibration


Equipment: TURBIDIMETER
Model: 2100N
Serial No. (or ID.): 970400003415 (EQL-024)
Manufacturer: HACH
Condition: In Condition

Certificate No.: C08230153
Issued Date: 15 September 2023
Job No.: WO-00005226
Page: 1 of 2

Customer: TEST TECH CO., LTD.
30,32 Rama II Soi 63, Rama II Rd.,
Samaedam, Bangkhuntien Bangkok 10150 Thailand

Environment Condition: Temperature 23 °C ± 2 °C
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited.
2533 Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: 
Calibration Date: 14 September 2023
The Method used: In house method, CAL-WI-23, base on Hach Manufacturer Method 8195
Traceability: This certificate is traceable to Primary standard Fromazin and StablCal accepted by United States Environmental Protection Agency (EPA) through Hach Company
Certificate No. A1075 , A1074 , A1091 , A1074 , A1074

Person in charge

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ($k=2$) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองตันใต้ เขตวัฒนา กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-C08-08: 20 Jul 2022

Calibration Results:

Before Adjustment

Std Turbidity (NTU)	UUC Reading	Correction	Deviation	Uncertainty
0.050	0.088	-0.038	0.0	0.070
20.40	19.1	1.30	0.0	1.0
205.0	195	10.0	0.5	10
1028.0	952	76.0	0.9	50
4068.0	3942	126.0	0.9	200

After Adjustment

Std Turbidity (NTU)	UUC Reading	Correction	Deviation	Uncertainty
0.050	0.084	-0.034	0.0	0.070
20.40	20.4	0.00	0.0	1.0
205.0	205	0.0	0.5	10
1028.0	1026	2.0	0.5	50
4068.0	4063	5.0	0.5	200

The End of Certificate

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองตันใต้ เขตวัฒนา กรุงเทพมหานคร 10260
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth – in Asia and Beyond.

CAL-FM-C08-08: 20 Jul 2022

๕๒

ใบรับรองการสอบเทียบ “เครื่องวัดความนำไฟฟ้า”
(Calibration Certificate of Conductivity Meter)



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 24CH59

Page.: 1 of 3

Certificate of Calibration

Equipment :	Conductivity Meter
Manufacturer :	TOA
Model :	CM-41X
Serial No. :	842572
ID No. :	EQL-211
Condition As-Received:	Used Item
Received Date :	11 January 2024
Calibration Date :	15 January 2024
Reference :	2401-0300DN-1
Submitted by :	TEST TECH CO.,LTD. (HEAD Office) 30, 32 Rama II Soi 63, Rama II Rd., Samaedam, Bangkhunthian, Bangkok 10150
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure:	In -house method : - CP-CH6 by direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lerngagtrakul

Approved by :

(✓)
()
()

Approved Signatory

Issue Date : 17 January 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0062587



Cert.No.: 24CH59

Page.: 2 of 3

Condition of this result of calibration

1. Reference Standard Instrument :-

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1) Thermometer	1963878	130RC095	23I1051	05 Sep 2024
2) Ref. Std.Thermometer	4982054	110RC044	23I908	26 Jul 2024

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Conductivity Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
147.0 $\mu\text{S/cm}$	CPA Chem	913595	14 July 2024
1.413 mS/cm	CPA Chem	931955	30 Sep 2024
12.880 mS/cm	CPA Chem	913597	14 July 2024

- Control Conductivity calibration solution temperature by Water bath $(25 \pm 0.1) ^\circ\text{C}$

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

(*) After Adjustment at 147.0, 1413.0, 12880 $\mu\text{S/cm}$

Conductivity Electrode Serial No.: 806F0005

Standard Conductivity Solution	After Adjustment UUC* Reading	Uncertainty of Measurement (\pm)	Coverage factor k
147.0 $\mu\text{S/cm}$	147.1 $\mu\text{S/cm}$	0.99 $\mu\text{S/cm}$	2.00
1.413 mS/cm	1.413 mS/cm	0.0092 mS/cm	2.00
12.880 mS/cm	12.88 mS/cm	0.086 mS/cm	2.00

Remark - UUC* = Unit Under Calibration

- Adjustment Cell constant = $147.0 \mu\text{S/cm} \times 96.8 \text{ m}^{-1}$, $1.413 \text{ mS/cm} = 98.0 \text{ m}^{-1}$, $12.880 \text{ mS/cm} = 99.4 \text{ m}^{-1}$

a 1197672



Cert.No.: 24CH59

Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

(*) Without adjustment

This equipment was connected with Temperature Probe;

- Model : CT-58101B

- Serial No. : 806F0005

Dimension of probe;

- Length : 114 mm

- Diameter : 12 mm

- Immersion Depth : 100 mm

Calibration Point ($^\circ\text{C}$)	Standard Temperature ($^\circ\text{C}$)	UUC* Reading ($^\circ\text{C}$)	Error ($^\circ\text{C}$)	Uncertainty of Measurement ($\pm ^\circ\text{C}$)	Coverage factor k
25.0	25.003	25.0	-0.003	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

-o0o-

a 1197671

๗๙

ใบรับรองการสอบเทียบ “ห้องเย็น”
(Calibration Certificate of Cool Room)

**Metrology**

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360

Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T240070

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cooling Room)

Manufacturer : -

Model : -

Serial No. : -

Customer Code : EQL-167

ID No. : T1447A1

Customer : Test Tech Co.,Ltd
30, 32 Rama II Soi 63, Rama II Rd., Samaedam,
Bangkhunthian Bangkok 10150

Customer Location : LABORATORY FLOOR 3

Date of Receipt : 12 January 2024

Calibrated By : [REDACTED] (Site Calibration Manager)

Approved By : [REDACTED] (Site Calibration Manager)

Date of Issue : 24 JAN 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology



Certificate No. T240070

Page 2 of 4

Calibration Report

Equipment : Chamber (Cooling Room)
Date of Calibration : 16 January 2024
Environment : Temperature : 19.4-24.1 °C
Line Voltage : 221.3-226.1 V
Relative Humidity : 55 - 65 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert nine standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).
All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T230773	10 April 2024
TC	TYPE T	TN161-TN170	T230773	10 April 2024
DATA LOGGER	34970A	T149	T230773	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant - Hour 37 Minute At 3 °C

Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

() without adjustment

(X) after adjustment


Approved By



Certificate No. T240070

Page 3 of 4

Calibration Report

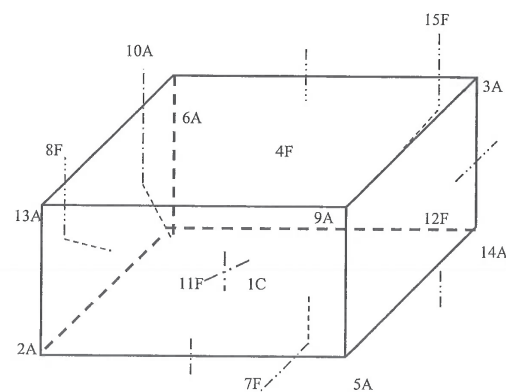

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN161
12F	=	TN162
13A	=	TN163
14A	=	TN164
15F	=	TN165

Approved By



Certificate No. T240070

Page 4 of 4

Calibration Report

Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)									
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	3.17	3.11	3.11	3.33	2.94	3.06	2.95	3.17	2.86	2.59
	TN161	TN162	TN163	TN164	TN165					
	2.74	2.95	2.75	2.95	2.85					

Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage
	Min , Max	Average					Factor <i>k</i>
3.0	2.9 , 3.1	3.0	2.97	0.29	0.64	0.80	2.00

* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 

FM-L15 I18/18-08-66



Certificate No. T240161

Page 1 of 4

Certificate of Calibration

Equipment : Chamber (Cooling Room)

Manufacturer : -

Model : -

Serial No. : -

Customer Code : EQL-181

ID No. : T0399A5


Customer : Test Tech Co.,Ltd


30, 32 Rama II Soi 63, Rama II Rd., Samaedam,

Bangkhunthian Bangkok 10150

Customer Location : LABORATORY FLOOR 4

Date of Receipt : 24 January 2024

Calibrated By :  (Temperature Calibration Manager)

Approved By :  (Site Calibration Manager)

Date of Issue : 31 JAN 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.



Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



Certificate No. T240161

Page 2 of 4

Calibration Report

Equipment : Chamber (Cooling Room)
Date of Calibration : 29 January 2024
Environment : Temperature : 25.4-27.9 °C
Line Voltage : 223.4-227.1 V
Relative Humidity : 45 - 49 %RH

Condition of this results of calibration :

1. This equipment was calibrated by insert 15 standard thermocouples type T into its chamber , the other one standard thermocouples type T use for ambient temperature measurement . The calibration was done in according to WI-T20 (based on ASTM E145-94 (Reapproved 2001) and AS2853-1986).

All data show below were final values and the initial data from customer request . The temperature scale used was based on ITS - 90 .

2. Reference Standard Instrument :

Instrument	Model	Instrument No.	Certificate No.	Due Date
TC	TYPE T	TN161-TN170	T230773	10 April 2024
TC	TYPE T	TN171-TN180	T230773	10 April 2024
DATA LOGGER	34970A	T149	T230773	10 April 2024

3. This certificate is traceable to :

National Institute of Metrology (Thailand) through Metrological Center (NSC-TISI-TIS 17025 CALIBRATION 0244.)

4. Condition of calibrated item : good

Equipment Description :

Time Constant 1 Hour 30 Minute At 3 °C
Fresh Air Damper ☐ Open ☐ Min ☐ Medium ☐ Max
☐ Close
☒ Not Available

5. Adjustment :

(X) without adjustment () after adjustment

Approved By. _____



Metrology

SCI ECO Services Company Limited


33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.



Certificate No. T240161

Page 3 of 4

Calibration Report

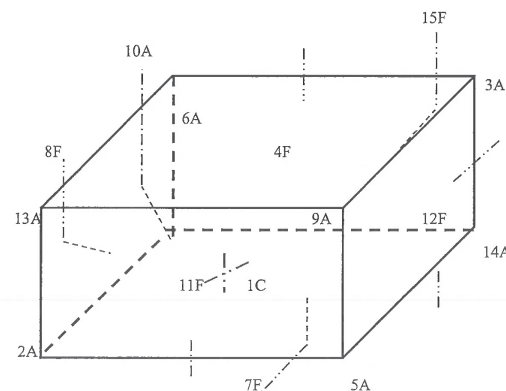

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170
11F	=	TN171

12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175

Approved By. _____



Certificate No. T240161

Page 4 of 4

Calibration Report

Measurement Results

Calibration Point	Average Standard Reading at each position (°C)									
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3.0	2.81	3.01	2.99	2.87	2.92	3.08	3.04	2.93	3.31	3.10
	TN171	TN172	TN173	TN174	TN175					
	3.08	3.10	3.40	3.00	3.24					

Chamber (Cooling Room)			Temperature Distribution				
Setting (°C)	Reading (°C)		Average (°C)	Stability (± °C)	Uniformity (°C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
	Min , Max	Average					
3.0	2.8 , 3.1	3.0	3.06	0.40	0.92	1.07	2.00

* The Acuoted uncertainty exclude "uniformity"

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor *k* which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. _____

MAINTENANCE AND IPV TEST CERTIFICATE MODEL OPTIMA 8000

Customer : บริษัท เทสท์ เทคโนโลยี จำกัด.
Address : 30,32 ซอยพระรามที่ 2 ซอย 63
ถนนพระรามที่ 2 แขวงสมเด็จเจ้าพระยา กรุงเทพมหานคร 10150
User Name: XXXXXXXXXX
Phone: XXXXXXXXXX
Fax: XXXXXXXXXX

Date Tested: May 14, 2024
Recommendation Recertification
Period 12 Months
Recertification Due: May 14, 2025
Date Last Certified: May 18, 2023
Visit Number: 1 of 1
PerkinElmer Phone: 02-719-6420 ext 206
PerkinElmer Fax: 02-318-5597

CONFIGURATION TESTED

MODEL	SERIAL NUMBER	SOFTWARE
OPTIMA 8000 (EQL-180)	078S1411171C	ICP WinLab32 version 5
TESTED EQUIPMENT IPV Methods	CALIBRATION NUMBER	EXPIRATION
TEST STANDARD USED Multielement Standard Instrument Cal. STD4	PART NUMBER N069-1579 N930-0221	EXPIRATION DATE Dec 30, 2024 Nov 30, 2024
CUSTOMER SUPPLIED 2 % HNO3 10 % HNO3	COMMENTS	CUSTOMER INITIALS

MAINTENANCE AND IPV TEST CERTIFICATE MODEL OPTIMA 8000

SERIAL NUMBER: 078S1411171C DATE TESTED: May 14, 2024

1. MECHANICAL CHECKS
A. Inspect and clean all fans and filters. ☐ OK
B. Inspect and replace as necessary, all torch components including the RF coil. ☐ OK
C. Inspect all tubing for sign of clacking or leaking. ☐ OK
D. Adjust water and gas pressure regulator settings. ☐ OK
E. Inspect and leak check pneumatics drawers. ☐ OK
F. Clean the exterior of the instrument. ☐ OK

2. OPTICAL CHECKS

A. Inspect and clean all optical components. ☐ OK
B. As required, check and replace all purge filters. ☐ OK
C. Recheck optical alignment. ☐ OK

3. COOLING SYSTEM CHECKS

A. Perform preventive maintenance on chiller. ☐ OK
B. Flush out the chiller every six months. ☐ OK

4. PERFORMANCE CHECKS

A. Torch View Alignment. ☐ OK
B. Wavelength Calibration. ☐ OK

MAINTENANCE AND IPV TEST CERTIFICATE MODEL
OPTIMA 8000

SERIAL NUMBER: 078S1411171C		DATE TESTED: May 14, 2024	
PARAMETER	SPECIFICATION		FINAL VALUE
Spectral Resolution : UV			
As	193.696 nm	≤ 0.009 nm	0.00735 nm
Ni	231.604 nm	≤ 0.011 nm	0.00913 nm
Ni	341.476 nm	≤ 0.015 nm	0.01386 nm
Spectral Resolution : VIS			
Ba	455.403 nm	≤ 0.020 nm	0.01721 nm
Precision			
Zn	206.200 nm	% RSD ≤ 1.0 %	0.35 %
Mg	280.271 nm	% RSD ≤ 1.0 %	0.27 %
Mg	285.213 nm	% RSD ≤ 1.0 %	0.46 %
Ba	455.403 nm	% RSD ≤ 1.0 %	0.48 %
Detection Limits : Axial			
Tl	190.801 nm	3(sd) ≤ 10.0 ppb	1.00 ppb
As	193.696 nm	3(sd) ≤ 10.0 ppb	3.32 ppb
Se	196.026 nm	3(sd) ≤ 5.0 ppb	3.88 ppb
Pb	220.353 nm	3(sd) ≤ 3.0 ppb	1.45 ppb
Detection Limits : Radial			
As	193.696 nm	3(sd) ≤ 60.0 ppb	3.41 ppb
Zn	213.857 nm	3(sd) ≤ 2.0 ppb	0.30 ppb
Mn	257.610 nm	3(sd) ≤ 1.0 ppb	0.03 ppb
La	379.478 nm	3(sd) ≤ 3.0 ppb	0.27 ppb
Ba	455.403 nm	3(sd) ≤ 0.3 ppb	0.05 ppb
Ba	493.408 nm	3(sd) ≤ 0.6 ppb	0.06 ppb
BEC : Axial (IB X 1000)/(IS-IB)			
Mn	257.610 nm	≤ 30 ppb	10.70 ppb
BEC : Radial (IB X 1000)/(IS-IB)			
Mn	257.610 nm	≤ 30 ppb	21.54 ppb

MAINTENANCE AND IPV TEST CERTIFICATE MODEL
OPTIMA 8000

SERIAL NUMBER: 078S1411171C DATE TESTED: May 14, 2024

Remarks :

Commissioning follow as commissioning performance sheets.

This is to certify that the above tests have been performed and the configuration tested

☒

☐

meets


does not meet

the PerkinElmer Specifications listed on this certificate.

This certificate does not modify PerkinElmer's standard terms and condition of sale, including warranty terms.

Service Department PerkinElmer Scientific (Thailand)Co.,Ltd.

Customer Service Engineer:



Service Engineer