



บริษัท เอ็นไวแล็บ จำกัด 540.540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540.540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab S. FineLine Supply Environment

Verification Test Report

Report No.:

SO2400021-E002 -SLM 07

☒ PM

☐ Onsite UTM :

47P 1514458 654247

Calibrated Date: 26 February 2024

Site : บริษัท เอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 44

Serial : 1821

Environment: Temperature 25 °C Humidity 60 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 16 March 2023

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.78	93.74	-0.04	93.78

Calibrated By:

(Nattawut Sardpum)

Date:

26 February 2024

Approve By:

(Wisan Ritthikamon)

Date:

26 February 2024

This report shall not be reproduced except in full without the written approval of Envilab Co., Ltd.



บริษัท เอ็นไวเล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhoe 7 Bangkhoe Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab & Envilab Supply Instrument

Verification Test Report

Report No.:

SO2400021-E002 -SLM 08

☒ PM

☐ Onsite UTM :

47P 1514458 654247

Calibrated Date: 26 February 2024

Site : บริษัท เอ็นไวเล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 44

Serial : 1877

Environment: Temperature 25 °C Humidity 60 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 16 March 2023

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.78	93.74	-0.04	93.78

Calibrated By:

(Nattawut Sardpum)

Date:

26 February 2024

Approve By:

(Wisan Ritthikamon)

Date:

26 February 2024

This report shall not be reproduced except in full without the written approval of Envilab Co., Ltd.



บริษัท เอ็นไวแล็บ จำกัด 540.540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540.540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax: 02-802-3773 E-mail : info@evltesting.com



Envilab & Nidec Supply Instrument

Verification Test Report

Report No.:

SO2400021-E002 -SLM 09

☒ PM

☐ Onsite UTM :

47P 1514458 654247

Calibrated Date: 26 February 2024

Site : บริษัท เอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 44

Serial : 1842

Environment: Temperature 25 °C Humidity 60 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 16 March 2023

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.78	93.72	-0.06	93.78

Calibrated By:

(Nattawut Sardpum)

Date:

26 February 2024

Approve By:

(Wisan Ritthikamon)

Date:

26 February 2024

This report shall not be reproduced except in full without the written approval of Envilab Co., Ltd.





บริษัท เอ็นไวเทสท์ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkhae Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab S. Limited Safety Instrument

Verification Test Report

Report No.:

SO2400021-E002 -SLM 10

☒ PM

☐ Onsite UTM :

47P 1514458 654247

Calibrated Date: 26 February 2024

Site : บริษัท เอ็นไวเทสท์ จำกัด

Equipment: Sound Level Meter

Manufacturer: PULSAR

Model: 44

Serial : 1810

Environment: Temperature 25 °C Humidity 60 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 16 March 2023

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.78	93.74	-0.04	93.78

Calibrated By:


(Nattawut Sardpum)

Date:

26 February 2024

Approve By:


(Wisan Ritthikamon)

Date:

26 February 2024

This report shall not be reproduced except in full without the written approval of Envilab Co., Ltd.



Certificate of Calibration

Certificate Number : SPR23040182-10

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae Bangkok 10160

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1796

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23\text{ }^{\circ}\text{C} \pm 3\text{ }^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Apr 2023

Calibration Date : 20 Apr 2023

Recommend Due Date : 20 Apr 2024

Date of Issue : 21 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Prayoon Topart

Calibration Officer

Approved by :

(Mr. Nirut Loha)



Calibration Report

Certificate Number : SPR23040182-10

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at ;
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23040182-10

Page : 3 of 3

Range : 20 to 140 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

– End of Certificate –



Certificate of Calibration

Certificate Number : SPR23040182-2

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae Bangkok 10160

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1805

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 19 Apr 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 20 Apr 2023

Location of Calibration : In-Lab

Recommend Due Date : 20 Apr 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 21 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Prayoon Topart

Approved by :

Calibration Officer

(Mr. Nirut Loha)

Authorized Signatory



Calibration Report

Page : 2 of 3

Certificate Number : SPR23040182-2

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at:
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23040182-2

Page : 3 of 3

Range : 20 to 140 dB

Function : @1kHz

Select A Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15


Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

– End of Certificate –



Certificate of Calibration

Certificate Number : SPR23070059-9

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae Bangkok 10160

Equipment Name : Sound Level Meter
Manufacturer : Pulsar
Model : 44
Serial Number : PN1807
ID. Number : NSMPUMD44N1807

Environmental Conditions

Ambient Temperature	: 23 °C ± 3 °C	Received Date	: 05 Jul 2023
Relative Humidity	: 50 % ± 15 %	Calibration Date	: 06 Jul 2023
Location of Calibration	: In-Lab	Recommend Due Date	: 06 Jul 2024
Calibration Procedure	: SP-CPE-04-01	Date of Issue	: 07 Jul 2023

Method of Calibration


This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by :

(Mr.Nirut Loha)



Calibration Report

Certificate Number : SPR23070059-9

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23070059-9

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select **A** Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Select **C** Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Select **Z** Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Page : 1 of 3

Certificate Number : SPR23070059-5

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae Bangkok 10160

Equipment Name : Sound Level Meter
Manufacturer : Pulsar
Model : 44
Serial Number : PN1879
ID. Number : NSMPUMD44N1879

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 05 Jul 2023

Calibration Date : 06 Jul 2023

Recommend Due Date : 06 Jul 2024

Date of Issue : 07 Jul 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).


Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by :

(Mr.Nirut Loha)

Authorized Signatory

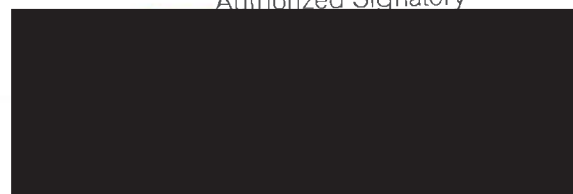



Calibration Report

Certificate Number : SPR23070059-5

Page : 2. of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at:
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23070059-5

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select C Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Select Z Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.2	94.2	0.2	0.2	0.15
114	113.8	113.8	-0.2	-0.2	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23070059-7

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae Bangkok 10160

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1881

ID. Number : NSMPUMD44N1881

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 05 Jul 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jul 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jul 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jul 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by :

(Mr.Nirut Loha)

Authorized Signatory



Calibration Report

Certificate Number : SPR23070059-7

Page : 2, of 3


Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at ;

TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23070059-7

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select A

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.2	94.2	0.2	0.2	0.15
114	114.1	114.1	0.1	0.1	0.15

Select C

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.2	94.2	0.2	0.2	0.15
114	114.1	114.1	0.1	0.1	0.15

Select Z

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.2	94.2	0.2	0.2	0.15
114	114.1	114.1	0.1	0.1	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate Number : SPR23040182-1

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae Bangkok 10160

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1810

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 19 Apr 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 20 Apr 2023

Location of Calibration : In-Lab

Recommend Due Date : 20 Apr 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 21 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Prayoon Topart

Calibration Officer

Approved by :

(Mr. Nirut Loha)

Authorized Signatory



Calibration Report

Certificate Number : SPR23040182-1

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Page : 3 of 3

Range : 20 to 140 dB

Function : @1kHz

Unit : dB

Select Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Unit : dB

Select Z Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

Note:
The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



(Mr.Nirut Loha)

Calibration Officer

69/29 Moo 1, Klangsi Klongluang Pathumthani 12120 (Thailand) Tel: (662) 193-2220 5 คู่มือ www.สอบเทียบอุปกรณ์เครื่องวัด.com



METROLOGY SYSTEM (THAILAND) CO.,LTD.



Calibration Report

Certificate Number : SPR23040182-8

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at:
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23040182-8

Page : 3 of 3

Range : 20 to 140 dB

Function : @1kHz

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -

CERTIFICATE OF CALIBRATION

ISSUED BY **Pulsar Instruments Plc**

DATE OF ISSUE **29 June 2023**

CERTIFICATE NUMBER **194449**



**Pulsar Instruments Plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom**

Page 1 of 2

Approved signatory

T. Goodrich

Electronically signed:

A handwritten signature in black ink, appearing to read 'T. A. Goodrich', written over a horizontal line.

Sound Level Meter : IEC 61672-3:2013

Instrument information

Manufacturer: Pulsar Instruments Plc
Model: Model 44
Serial number: PN1821
Class: 2
Firmware version: 2.6.0.328

Notes:

Test summary

Date of calibration: 29 June 2023

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.
Periodic tests were performed in accordance with procedures from IEC 61672-3:2013.

The sound level meter submitted for testing successfully completed the class 2 periodic tests of IEC 61672-3:2013, for the environmental conditions under which the tests were performed.

However, no general statement or conclusion can be made about conformance of the sound level meter to the full specifications of IEC 61672-1:2013 because (a) evidence was not publicly available, from an independent testing organisation responsible for pattern approvals, to determine that the model of sound level meter fully conformed to the class 2 specifications in IEC 61672-1:2013 or correction data for acoustical test of frequency weighting were not provided in the Instruction Manual and (b) because the periodic tests of IEC 61672-3:2013 cover only a limited subset of the specifications in IEC 61672-1:2013.

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

ISSUED BY **Pulsar Instruments Plc**
DATE OF ISSUE **28 June 2023** CERTIFICATE NUMBER **194448**



Pulsar Instruments Plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Test engineer:
D.Swalwell
Electronically signed:

A handwritten signature in black ink, appearing to be 'D. Swalwell', written over a horizontal line.

Microphone

Microphone capsule

Manufacturer: Pulsar Instruments

Model: PM2

Serial Number: 022540E

Calibration procedure

Date of calibration: 28 June 2023

Open circuit: 50.3 mV/Pa

Sensitivity at 1 kHz: -26.0 dB rel 1 V/Pa

The microphone capsule detailed above has been calibrated to the published data as described in the operating manual of the associated sound level meter (where applicable).

The frequency response was measured using an electrostatic actuator in accordance with BS EN 61094-6:2005 with the free-field response derived via standard correction data traceable to a National Measurement Institute.

The absolute sensitivity at 1 kHz was measured using an acoustic calibrator conforming to IEC 60942:2003 Class 1.

Environmental conditions

Pressure: 100.70 kPa

Temperature: 21.0 °C

Humidity: 69.0 %



Service Report

Instrument Manufacturer: Pulsar Instruments Plc
Job Reference Number: 84203
Instrument Type: Model 44
Serial Number: PN1821

Customer Name: Neediss Supply Instrument Co., Ltd.,
Customer Address: 536, Soi Bangkhuae 7
Bangkhuae
Thailand
10160

Issue	Action	Result	Engineer
Recal & repair LCD problem and microphone failure. Keypad top right key failure, incorrect pre amp s/n programmed 1768. Actually fitted s/n 1899.	Reprogrammed correct pre amp s/n. New PM2 microphone s/n 022540E fitted. Replaced "blotchy" display. Replaced the keypad.	Recal ok tag	Terry Goodrich


Engineer:

T. A. Goodrich

Date: 29 June 2023

We hope that you are satisfied with the service you have received from Pulsar Instruments plc.
If you have any concerns, would like further information or have any feedback do not hesitate to contact us.

Pulsar Instrument Plc, Acoustic House, Bridlington Road, Hunmanby, YO14 0PH
Telephone: +44 (0) 1723 518011 Fax: +44 (0) 1723 518043
Email: sales@pulsarinstruments.com



Certificate of Calibration

Certificate Number : SPR23070059-6

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae Bangkok 10160

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1877

ID. Number : NSMPUMD44N1877

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$ Received Date : 05 Jul 2023

Relative Humidity : $50\% \pm 15\%$ Calibration Date : 06 Jul 2023

Location of Calibration : In-Lab Recommend Due Date : 06 Jul 2024

Calibration Procedure : SP-CPE-04-01 Date of Issue : 07 Jul 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Calibration Officer

Approved by :

(Mr.Nirut Loha)

Authorized Signatory



Calibration Report

Certificate Number : SPR23070059-6

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23070059-6

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Unit : dB

Select A Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.3	114.3	0.3	0.3	0.15

Unit : dB

Select C Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.3	114.3	0.3	0.3	0.15

Unit : dB

Select Z Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.3	114.3	0.3	0.3	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



ELECTRICAL AND ELECTRONICS INSTITUTE
FOUNDATION FOR INDUSTRIAL DEVELOPMENT

975 Moo 4, Bangpoo Industrial Estate, Soi 8, Sukhumvit Road km 37,
Phraek Sa, Mueang Samut Prakan, Samut Prakan 10280
Tel: +66 2709 4860 Fax: +66 2324 0917



Certificate No.: CP20230179EA
Operation No.: CP2023030029

Certificate of Calibration

Equipment: Sound Level Meter
Manufacturer: Pulsar Instruments Plc
Model/Type: 44 (Meter), PM2 (Microphone), PA40 (Preamplifier)
Serial No.: PN1842 (Meter), 022722D (Microphone), 1769 (Preamplifier)
ID No.: NSMPUMD44N1842
Customer: Envilab Co., Ltd.
Address: 540,540/1 Soi Bangkhuae 7, Bangkhuae,
Bangkhuae, Bangkok 10160
Received Date: 16 March 2023
Calibrated Date: 29 March 2023 - 4 April 2023
Issued Date: 5 April 2023
Calibrated by: Ms. Juntaporn Kunhakom

Approved by: _____

(Mr. Sittichai Swaksuriyawong)
Group Manager

This report was prepared electronically using applicable electronic signature. Printing or copy of file are considered as a copy of the document.

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor (k) providing a level of confidence of approximately 95%. This certificate may not be reproduced other than in full except with the prior written approval of the Electrical and Electronics Institute, Foundation for Industrial Development.

Certificate No.: CP20230179EA

Calibration Report

Equipment: Sound Level Meter
 Manufacturer: Pulsar Instruments Plc
 Model/Type: 44 (Meter), PM2 (Microphone), PA40 (Preamplifier)
 Serial No.: PN1842 (Meter), 022722D (Microphone), 1769 (Preamplifier)
 ID No.: NSMPUMD44N1842
 Ambient Temperature: (23 ± 2) °C
 Relative Humidity: (50 ± 15) %
 Pressure: (101.3 ± 1.5) kPa
 Method of Calibration :-
 IEC 61672-3:2013.

Condition of this result of calibration

1. Reference standards instrument :-

Instrument	Model	Serial No.	Cert. No.	Due Date
1) Standard microphone	4180	2787490	AA-1024-22	6 November 2023
2) Arbitrary Function Generator	AFG2021	C010063	CK20220059EA	19 June 2023
3) Programmable Attenuator	PA5	2755	EF-0034-22	30 October 2023
4) 6.5 Digit precision multimeter	8846A	9610014	CB20220223EA	14 November 2023
5) Pressure humidity and Temperature Transmitter	PTU301	F0640002	CL1-P230024 CD20220164EA	20/3/20224 24 July 2023
6) Performance Audio Analyzer	U8903B	MY56510003	CB20230038EA CK20220080EA	14 February 2024 8 September 2023

2. This result of calibration was found accurate as shown on date and place of calibration only.

3. This certification is traceable to the international system of unit maintained at :-

Reference standards instrument for Acoustic function

- National Institute of Metrology (Thailand)

Reference standards instrument for Electrical function

- National Institute of Metrology (Thailand)

- Electrical and Electronics Institute; NSC Accredited Calibration No.0119

Result of Calibration:-

Function : 1. Indication at the calibration check frequency

Reference Acoustic Signal (dB)	Measured value (dB)	Deviation (dB)	Acceptance limits (dB)
-	-	-	-

Certificate No.: CP20230179EA

Calibration Report

Function : 2. Self-generated Noise

2.1 Microphone Installed

Measured value (dB)
17.0

2.2 Microphone replaced by the electrical input signal device

Frequency Weighting	Measured value (dB)
A-weighting	Under-range
C-weighting	18.1
Z-weighting	26.6

Function : 3. Acoustical signal tests of frequency weightings (Without Windscreen)

Meter free-field acoustic response at a level of 84 dB.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
125	0.5	0.3	0.3	±1.5
1000	0.3	0.3	0.4	±1.0
8000	1.0	1.0	0.9	±5.0

Function : 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency (Hz)	Deviation from various Frequency Weighting Response Curve			
	C-Weighting (dB)	A-Weighting (dB)	Z-Weighting (dB)	Acceptance limits (dB)
63	0.0	0.0	0.0	±2.0
125	0.0	-0.1	0.0	±1.5
250	0.0	-0.1	0.0	±1.5
500	0.0	-0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.1	0.1	0.1	±2.0
4000	0.1	0.1	0.1	±3.0
8000	0.4	0.4	0.3	±5.0

Function : 5. Frequency and time weighting at 1 kHz

5.1 Frequency weighting at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
C-weighting	94.0	0.0	±0.2
A-weighting	94.0	0.0	±0.2
Z-weighting	94.0	0.0	±0.2

Certificate No.: CP20230179EA

Calibration Report

5.2 Time weighting at 1 kHz

Time Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	94.0	0.0	±0.1
Slow	94.0	0.0	±0.1
LAeq	94.0	0.0	±0.1

Function : 6. Long-Term Stability

Long-term stability over 30 minutes, with steady 1 kHz signal at reference level.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
30	94.0	94.0	0.0	±0.3

Function : 7. Level Linearity on the reference level range

7.1 Level Linearity on the reference level range, Upper

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
99.0	99.0	0.0	±1.1
104.0	104.0	0.0	±1.1
109.0	109.0	0.0	±1.1
114.0	114.0	0.0	±1.1
119.0	119.0	0.0	±1.1
124.0	124.0	0.0	±1.1
129.0	129.0	0.0	±1.1
134.0	134.0	0.0	±1.1

7.2 Level Linearity on the reference level range, Lower

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
94.0	94.0	0.0	±1.1
89.0	89.0	0.0	±1.1
84.0	84.0	0.0	±1.1
79.0	79.0	0.0	±1.1
74.0	74.0	0.0	±1.1
69.0	69.0	0.0	±1.1
64.0	64.0	0.0	±1.1
59.0	59.0	0.0	±1.1

Certificate No.: CP20230179EA

Calibration Report

7.2 Level Linearity on the reference level range, Lower (Cont.)

Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
54.0	54.0	0.0	±1.1
49.0	49.0	0.0	±1.1
44.0	44.0	0.0	±1.1
39.0	38.8	-0.2	±1.1
34.0	33.8	-0.2	±1.1
29.0	28.9	-0.1	±1.1

Function : 8. Tone burst response

Time Weighting	Tone burst duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Fast	200	136.0	0.0	±1.0
	2	118.9	-0.1	+1.0 ; -2.5
	0.25	109.8	-0.2	+1.5 ; -5.0
Slow	200	129.6	0.0	±1.0
	2	110.0	0.0	+1.0 ; -5.0
LAE	200	130.0	0.0	±1.0
	2	110.0	0.0	+1.0 ; -2.5
	0.25	100.9	-0.1	+1.5 ; -5.0

Function : 9. Peak C sound level

Number of cycles in test signal	Anticipated Value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limits (dB)
Complete cycle	135.4	135.1	-0.3	±3.0
Positive half cycle	134.4	134.1	-0.3	±2.0
Negative half cycle	134.4	134.1	-0.3	±2.0

Function : 10. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limits (dB)
Positive one-half cycle	Negative one-half cycle		
142.8	142.8	0.0	±1.5

Certificate No.: CP20230179EA

Calibration Report

Function : 11. High-Level Stability

High-level stability over 5 minutes, with steady 1 kHz signal, 1 dB below upper boundary.

Time Period to Apply Signal (min)	Reference SPL (dB)	Record SPL at Conclusion of Time Period (dB)	Deviated value (dB)	Acceptance limits (dB)
5	139.0	139.0	0.0	±0.3

Uncertainty of measurement

Function	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1) Indication at the calibration check frequency	0.30	Not applicable
2) Self-generated Noise	0.10	Not applicable
3) Acoustical signal tests of frequency weightings - Free-field sound pressure response level	0.30	0.60 (10Hz to 4kHz) 0.70 (>4kHz to 10kHz)
4) Electrical signal tests of frequency weightings	0.20	0.20
5) Frequency and time weighting at 1 kHz	0.20	0.20
6) Long-Term Stability	0.10	0.10
7) Level Linearity on the reference level range	0.30	0.30
8) Tone burst response	0.20	0.30
9) Peak C sound level	0.20	0.35
10) Overload indication	0.20	0.25
11) High-Level Stability	0.10	0.10

Remarks:

1. Indication at the calibration check frequency can not measured because customer does not provide a sound calibrator.
2. The acceptance limit is for the deviated value.
3. Acceptance limits was IEC61672-3:2013 Class 2.
4. The coverage factor $k = 2.00$

- - End of Report - -



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab S. Noise Supply Instrument

Verification Test Report

Report No.:

SO2400021-E002 -SLM 01

☒ PM

☐ Onsite UTM :

47P 1514458 N 654247 E

Calibrated Date: 3 March 2024

Site : บริษัท เอ็นไวแล็บ จำกัด

Equipment: Noise Dosemeter

Manufacturer: Pulsar

Model: Model 22

Serial : PB722

Environment: Temperature 25 °C Humidity 60 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 16 March 2023

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.78	93.73	-0.05	93.78

Calibrated By:

(Lerdfa Srimuangkaew)

Date:

3 March 2024

Approve By:

(Wisan Ritthikamon)

Date:

3 March 2024

This report shall not be reproduced except in full without the written approval of Envilab Co., Ltd.



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab 3 Year Supply Instruction

Verification Test Report

Report No.:

SO2400021-E002 -SLM 02

☒ PM

☐ Onsite UTM :

47P 1514458 N 654247 E

Calibrated Date: 3 March 2024

Site : บริษัท เอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: Pulsar

Model: Model 22

Serial : PB723

Environment: Temperature 25 °C Humidity 60 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 16 March 2023

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.78	93.71	-0.07	93.78

Calibrated By:

(Lerdfa Srimuangkaew)

Date:

3 March 2024

Approve By:

(Wisan Ritthikamon)

Date:

3 March 2024

This report shall not be reproduced except in full without the written approval of Envilab Co., Ltd.



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab & Needles Supply Instrument

Verification Test Report

Report No.:

SO2400021-E002 -SLM 03

☒ PM ☐ Onsite UTM : 47P 1514458 N 654247 E

Calibrated Date: 3 March 2024

Site : บริษัท เอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: Pulsar

Model: Model 22

Serial : PB721

Environment: Temperature 25 °C Humidity 60 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 16 March 2023

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.78	93.72	-0.06	93.78

Calibrated By:

(Lerdfa Srimuangkaew)

Date:

3 March 2024

Approve By:

(Wisan Ritthikamon)

Date:

3 March 2024

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkok Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab & Nivich Supply Instrument

Verification Test Report

Report No.:

SO2400021-E002 -SLM 04

☒ PM ☐ Onsite UTM : 47P 1514458 N 654247 E

Calibrated Date: 3 March 2024

Site : บริษัท เอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: Pulsar

Model: Model 22

Serial : PB724

Environment: Temperature 25 °C Humidity 60 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 16 March 2023

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.78	93.72	-0.06	93.78

Calibrated By:

(Lerdfa Srimuangkaew)

Date:

3 March 2024

Approve By:

(Wisan Ritthikamon)

Date:

3 March 2024

This report shall not be reproduced except in full without the written approval of Envilab Co., Ltd.



บริษัท เอ็นไวแล็บ จำกัด 540,540/1 ซอยบางแค 7 แขวงบางแค เขตบางแค กรุงเทพฯ 10160
Envilab Co., Ltd. 540,540/1 Soi Bangkhae 7 Bangkhae Bangkhoe Bangkok 10160
Tel : 02-802-3577-8 Fax. 02-802-3773 E-mail : info@evltesting.com



Envilab is a member of Supply and Phone

Verification Test Report

Report No.:

SO2400021-E002 -SLM 05

☒ PM

☐ Onsite UTM:

47P 1514458 N 654247 E

Calibrated Date: 3 March 2024

Site : บริษัท เอ็นไวแล็บ จำกัด

Equipment: Sound Level Meter

Manufacturer: Pulsar

Model: Model 22

Serial : PB711

Environment: Temperature 25 °C Humidity 60 %RH

Reference Standard: Acoustic Calibrator Class 1 Model 4230, Bruel&Kjaer

Serial No.1351075

Date of Calibration : 16 March 2023

Result of Test

Reference Standard (dB)	Instrument reading (dB)	Error (dB)	Adjust (dB)
93.78	93.74	-0.04	93.78

Calibrated By:

(Lerdfa Srimuangkaew)

Date:

3 March 2024

Approve By:

(Wisan Ritthikamon)

Date:

3 March 2024

This report shall not be reproduced except in full, without the written approval of Envilab Co., Ltd.



CERTIFICATE OF CALIBRATION

ISSUED BY **Pulsar Instruments Plc**

DATE OF ISSUE **10 May 2023**

CERTIFICATE NUMBER **191906**



Pulsar Instruments Plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory

S.Doveton

Electronically signed:

A handwritten signature in black ink, appearing to be 'S.Doveton', written over a horizontal line.

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Pulsar Instruments Plc Notes:
Model: Model 22TH
Serial number: PB711
Firmware version: 5.1

Test summary

Date of calibration: 10 May 2023

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	TTi	TG4001	395851
Attenuator	Cirrus Research	ZE:952	52200
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	79620

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

191906

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before	Pressure: 100.37 kPa	Temperature: 20.7 °C	Humidity: 50.0 %
After	Pressure: 100.37 kPa	Temperature: 20.8 °C	Humidity: 49.2 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity	Complies
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies



Service Report

Instrument Manufacturer: Pulsar Instruments Plc

Job Reference Number: 82822

Instrument Type: Model 22

Serial Number: PB711

Customer Name: Neediss Supply Instrument Co., Ltd.

Customer Address: 536, Soi Bangkhao 7

Bangkhao

Thailand

10160

Issue	Action	Result	Engineer
Shortened run times due to a faulty battery. Failing linearity tests at 80dB.	Replaced faulty battery. Replaced faulty IC U1.	Recalibrated, soaked and tested.	Shane Doveton

Engineer:

A handwritten signature in black ink, appearing to read "S.Doveton", written over a horizontal line.

Date: 10 May 2023

We hope that you are satisfied with the service you have received from Pulsar Instruments plc.
If you have any concerns, would like further information or have any feedback do not hesitate to contact us.

Pulsar Instrument Plc, Acoustic House, Bridlington Road, Hunmanby, YO14 0PH

Telephone: +44 (0) 1723 518011 Fax: +44 (0) 1723 518043

Email: sales@pulsarinstruments.com

CERTIFICATE OF CALIBRATION

ISSUED BY **Pulsar Instruments Plc**

DATE OF ISSUE **10 May 2023**

CERTIFICATE NUMBER **191900**



Pulsar Instruments Plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory

S.Doveton

Electronically signed:

A handwritten signature in black ink, appearing to be 'S.Doveton', written over a horizontal line.

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Pulsar Instruments Plc Notes:
Model: Model 22TH
Serial number: PB721
Firmware version: 5.1

Test summary

Date of calibration: 09 May 2023

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	TTi	TG4001	395851
Attenuator	Cirrus Research	ZE:952	52200
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	79620

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

191900

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before	Pressure: 100.18 kPa	Temperature: 21.6 °C	Humidity: 51.6 %
After	Pressure: 100.17 kPa	Temperature: 20.8 °C	Humidity: 50.2 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity	Complies
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies



Service Report

Instrument Manufacturer: Pulsar Instruments Plc
Job Reference Number: 82822
Instrument Type: Model 22
Serial Number: PB721

Customer Name: Neediss Supply Instrument Co., Ltd.
Customer Address: 536, Soi Bangkhae 7
Bangkhae
Thailand
10160

Issue	Action	Result	Engineer
Shortened run times due to a faulty battery.	Battery replaced.	Dosebadge, recalibrated, soaked and tested.	Shane Doveton

Engineer:

A handwritten signature in black ink, appearing to be "S.D.", written over a horizontal line.

Date: 10 May 2023

We hope that you are satisfied with the service you have received from Pulsar Instruments plc.
If you have any concerns, would like further information or have any feedback do not hesitate to contact us.

Pulsar Instrument Plc, Acoustic House, Bridlington Road, Hunmanby, YO14 0PH
Telephone: +44 (0) 1723 518011 Fax: +44 (0) 1723 518043
Email: sales@pulsarinstruments.com

CERTIFICATE OF CALIBRATION

ISSUED BY **Pulsar Instruments Plc**

DATE OF ISSUE **10 May 2023**

CERTIFICATE NUMBER **191901**



Pulsar Instruments Plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory

S.Doveton

Electronically signed:

A stylized, handwritten signature in black ink, appearing to be 'S.Doveton', located below the 'Electronically signed:' text.

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Pulsar Instruments Plc Notes:
Model: Model 22TH
Serial number: PB722
Firmware version: 5.1

Test summary

Date of calibration: 09 May 2023

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	TTi	TG4001	395851
Attenuator	Cirrus Research	ZE:952	52200
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	79620

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

191901

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before	Pressure: 100.26 kPa	Temperature: 21.1 °C	Humidity: 53.0 %
After	Pressure: 100.25 kPa	Temperature: 21.2 °C	Humidity: 53.0 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity	Complies
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies



Service Report

Instrument Manufacturer: Pulsar Instruments Plc

Job Reference Number: 82822

Instrument Type: Model 22

Serial Number: PB722

Customer Name: Neediss Supply Instrument Co., Ltd.

Customer Address: 536, Soi Bangkhae 7

Bangkhae

Thailand

10160

Issue	Action	Result	Engineer
Shortened run times due to a faulty battery.	Battery replaced.	Dosebadge recalibrated, soaked and tested.	Shane Doveton

Engineer:

A handwritten signature in black ink, appearing to be "S.D.", written over a horizontal line.

Date: 10 May 2023

We hope that you are satisfied with the service you have received from Pulsar Instruments plc.
If you have any concerns, would like further information or have any feedback do not hesitate to contact us.

Pulsar Instrument Plc, Acoustic House, Bridlington Road, Hunmanby, YO14 0PH
Telephone: +44 (0) 1723 518011 Fax: +44 (0) 1723 518043
Email: sales@pulsarinstruments.com

CERTIFICATE OF CALIBRATION

ISSUED BY **Pulsar Instruments Plc**

DATE OF ISSUE **10 May 2023**

CERTIFICATE NUMBER **191904**



Pulsar Instruments Plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory

S.Doveton

Electronically signed:

A handwritten signature in black ink, appearing to be 'S.Doveton', written over a horizontal line.

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Pulsar Instruments Plc Notes:
Model: Model 22TH
Serial number: PB723
Firmware version: 5.1

Test summary

Date of calibration: 09 May 2023

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	TTi	TG4001	395851
Attenuator	Cirrus Research	ZE:952	52200
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	79620

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

191904

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before	Pressure: 100.26 kPa	Temperature: 20.8 °C	Humidity: 54.8 %
After	Pressure: 100.22 kPa	Temperature: 20.5 °C	Humidity: 53.3 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity	Complies
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies



Service Report

Instrument Manufacturer: Pulsar Instruments Plc

Job Reference Number: 82822

Instrument Type: Model 22

Serial Number: PB723

Customer Name: Neediss Supply Instrument Co., Ltd.

Customer Address: 536, Soi Bangkhae 7

Bangkhae

Thailand

10160

Issue	Action	Result	Engineer
Shortened run times due to a faulty battery.	Replaced faulty battery.	Dosebadge recalibrated, soaked and tested.	Shane Doveton

Engineer:

A handwritten signature in black ink, appearing to read "S.Doveton", written over a horizontal line.

Date: 10 May 2023

We hope that you are satisfied with the service you have received from Pulsar Instruments plc.
If you have any concerns, would like further information or have any feedback do not hesitate to contact us.

Pulsar Instrument Plc, Acoustic House, Bridlington Road, Hunmanby, YO14 0PH

Telephone: +44 (0) 1723 518011 Fax: +44 (0) 1723 518043

Email: sales@pulsarinstruments.com



CERTIFICATE OF CALIBRATION

ISSUED BY **Pulsar Instruments Plc**

DATE OF ISSUE **10 May 2023**

CERTIFICATE NUMBER **191905**



Pulsar Instruments Plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory

S.Doveton

Electronically signed:

A handwritten signature in black ink, appearing to be 'S.Doveton', written over a horizontal line.

Dosemeter : IEC 61252-1993+A1:2000

Instrument information

Manufacturer: Pulsar Instruments Plc

Notes:

Model: Model 22TH

Serial number: PB724

Firmware version: 5.1

Test summary

Date of calibration: 09 May 2023

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

The dosimeter submitted for testing successfully completed the periodic tests of IEC 61252-1993+A1:2000.

The dosimeter submitted for testing conforms to the specifications in IEC 61252-1993+A1:2000.

Test equipment

Equipment	Manufacturer	Model	Serial number
Signal Generator	TTi	TG4001	395851
Attenuator	Cirrus Research	ZE:952	52200
Environmental Monitor	Comet	T7510	16966334
doseBadge Reader	Cirrus Research plc	RC:110A	79620

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

Certificate Number:

191905

Page 2 of 2

Environmental conditions

The following conditions were recorded at the time of the test:

Before	Pressure: 100.25 kPa	Temperature: 21.1 °C	Humidity: 53.5 %
After	Pressure: 100.26 kPa	Temperature: 20.9 °C	Humidity: 54.5 %

Test results summary

Test	Result
Absolute Acoustic Sensitivity	Complies
Linearity	Complies
Short Duration	Complies
Overload Latching	Complies
Frequency weighting	Complies



Service Report

Instrument Manufacturer: Pulsar Instruments Plc

Job Reference Number: 82822

Instrument Type: Model 22

Serial Number: PB724

Customer Name: Neediss Supply Instrument Co., Ltd.

Customer Address: 536, Soi Bangkhae 7

Bangkhae

Thailand

10160

Issue	Action	Result	Engineer
Shortened run times due to a faulty battery.	Replaced faulty battery.	Dosebadge recalibrated, soaked and tested.	Shane Doveton

Engineer:

A handwritten signature in black ink, appearing to be "S.Doveton", written over a horizontal line.

Date: 10 May 2023

We hope that you are satisfied with the service you have received from Pulsar Instruments plc.
If you have any concerns, would like further information or have any feedback do not hesitate to contact us.

Pulsar Instrument Plc, Acoustic House, Bridlington Road, Hunmanby, YO14 0PH

Telephone: +44 (0) 1723 518011 Fax: +44 (0) 1723 518043

Email: sales@pulsarinstruments.com



INTERNATIONAL TESTING SERVICE CO., LTD

1213/388 Ladprao 94 Ladprao Rd. Wangtonglang Bangkok 10310
Tel 0-2559-2095 Fax 0-2559-2096

E-mail : sale@itest-lab.com web site : www.itest-lab.com



NSC-TISI-TIS 17025
CALIBRATION 129

CALIBRATION CERTIFICATE

Issued date: 24 April 2023

Client Name : **ENVILAB CO., LTD.**

Address : 540,540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160.

Request No : **C-2304 - 179**

Laboratory No.: **CAL- 179**

Date of Request: 20 April 2023.

Date of Calibration: 21 April 2023.

1. Unit Under Calibration (UUC) :

Nomenclature : Lux / Fc Light Meter

Serial No.: 180501322

Maker : TENMARS

Model : TM-201

2. Place of Calibration: Photometry Standard Laboratory, INTERNATIONAL TESTING SERVICE CO., LTD.

3. Range of Calibration: 1 Range

4. Condition of Laboratory: Ambient temperature: (25 ± 2) °C and relative humidity (60 ± 20) %.

5. Reference Standard: Standard Tungsten Halogen Lamp, Serial No.: 504011, which was calibrated on 5 October 2022, can be traceable to International System of Unit (SI) through National Institute of Metrology (Thailand), Certificate No.: TP-1024-22.

6. Support Equipment:

1. Photometric bench, 6.3 meter long.
2. DC. power supply, Serial No.: EJ 19A 009, Model: GPR-25H 300, Maker: GW INSTEK.
3. Digital Multimeter, Model: 34401A, S/N: MY44011212 and MY44011215.
4. Foot Candle / Lux Meter, Model: 407026, S/N: Q 558437, Maker: EXTECH.

7. Calibration Procedure:

The measurement was done in accordance with WI-CP-01. The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

The Results shown in this certification report refer only to the equipment(s) calibrated unless otherwise stated
This Calibration Certificate cannot be reproduced, except in full



**INTERNATIONAL TESTING SERVICE CO., LTD**

1213/388 Ladprao 94 Ladprao Rd. Wangtonglang Bangkok 10310
Tel 0-2559-2095 Fax 0-2559-2096

E-mail : sale@itest-lab.com web site : www.itest-lab.com



Request No: **C-2304 - 179**

Serial No.: 180501322


Laboratory No.: **CAL - 179**

Results :

UUC Range	Standard (lx)	Unit Under Calibration Reading (lx)	Correction (lx)	Uncertainty of Measurement (\pm lx)
2000	0	000	0	0.6
	100	103	- 3	2.0 % of Reading
	500	500	0	
	1000	987	+ 13	
	1500	1469	+ 31	
	2000	1948	+ 52	

Note: The results relate only to the items calibrated.

Calibration result approved by


(Mr. Yuttana Tholueng)



Approved on behalf of
International Testing Service Co., Ltd


(Mr. Pichit Vivat-Anant)
Managing Director



Certificate of Calibration

Certificate Number : SPR23040182-9

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae Bangkok 10160

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1575

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 19 Apr 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 20 Apr 2023

Location of Calibration : In-Lab

Recommend Due Date : 20 Apr 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 21 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system

requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Prayoon Topart

Approved by :

Calibration Officer

(Mr. Nirut Loha)

natory



Calibration Report

Certificate Number : SPR23040182-9

Page : 2, of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at ;
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23040182-9

Page : 3 of 3

Range : 20 to 140 dB

Function : @1kHz

Select A Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select C Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Select Z Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



CERTIFICATE OF CALIBRATION

ISSUED BY **Pulsar Instruments Plc**

DATE OF ISSUE **29 June 2023**

CERTIFICATE NUMBER **194449**



Pulsar Instruments Plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Approved signatory

T. Goodrich

Electronically signed:

A handwritten signature in black ink, appearing to read 'T. A. Goodrich', written over a horizontal line.

Sound Level Meter : IEC 61672-3:2013

Instrument information

Manufacturer: **Pulsar Instruments Plc**

Notes:

Model: **Model 44**

Serial number: **PN1821**

Class: **2**

Firmware version: **2.6.0.328**

Test summary

Date of calibration: **29 June 2023**

The calibration was performed respecting the requirements of ISO/IEC 17025:2017.

Periodic tests were performed in accordance with procedures from IEC 61672-3:2013.

The sound level meter submitted for testing successfully completed the class 2 periodic tests of IEC 61672-3:2013, for the environmental conditions under which the tests were performed.

However, no general statement or conclusion can be made about conformance of the sound level meter to the full specifications of IEC 61672-1:2013 because (a) evidence was not publicly available, from an independent testing organisation responsible for pattern approvals, to determine that the model of sound level meter fully conformed to the class 2 specifications in IEC 61672-1:2013 or correction data for acoustical test of frequency weighting were not provided in the Instruction Manual and (b) because the periodic tests of IEC 61672-3:2013 cover only a limited subset of the specifications in IEC 61672-1:2013.

Notes



This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$, providing a coverage probability of approximately 95%.

CERTIFICATE OF CALIBRATION

ISSUED BY **Pulsar Instruments Plc**
DATE OF ISSUE **28 June 2023** CERTIFICATE NUMBER **194448**



Pulsar Instruments Plc
Acoustic House
Bridlington Road
Hunmanby
North Yorkshire
YO14 0PH
United Kingdom

Page 1 of 2

Test engineer:
D.Swalwell
Electronically signed:

A handwritten signature in black ink, appearing to be 'D. Swalwell', written over a horizontal line.

Microphone

Microphone capsule

Manufacturer: Pulsar Instruments

Model: PM2

Serial Number: 022540E

Calibration procedure

Date of calibration: 28 June 2023

Open circuit: 50.3 mV/Pa

Sensitivity at 1 kHz: -26.0 dB rel 1 V/Pa

The microphone capsule detailed above has been calibrated to the published data as described in the operating manual of the associated sound level meter (where applicable).

The frequency response was measured using an electrostatic actuator in accordance with BS EN 61094-6:2005 with the free-field response derived via standard correction data traceable to a National Measurement Institute.

The absolute sensitivity at 1 kHz was measured using an acoustic calibrator conforming to IEC 60942:2003 Class 1.

Environmental conditions

Pressure: 100.70 kPa

Temperature: 21.0 °C

Humidity: 69.0 %





Service Report

Instrument Manufacturer: Pulsar Instruments Plc

Job Reference Number: 84203

Instrument Type: Model 44

Serial Number: PN1821

Customer Name: Neediss Supply Instrument Co., Ltd.

Customer Address: 536, Soi Bangkhao 7

Bangkhao

Thailand

10160

Issue	Action	Result	Engineer
Recal & repair LCD problem and microphone failure. Keypad top right key failure, incorrect pre amp s/n programmed 1768. Actually fitted s/n 1899.	Reprogrammed correct pre amp s/n. New PM2 microphone s/n 022540E fitted. Replaced "blotchy" display. Replaced the keypad.	Recal ok tag	Terry Goodrich

Engineer:

T. A. Goodrich

Date: 29 June 2023

We hope that you are satisfied with the service you have received from Pulsar Instruments plc.
If you have any concerns, would like further information or have any feedback do not hesitate to contact us.

Pulsar Instrument Plc, Acoustic House, Bridlington Road, Hunmanby, YO14 0PH

Telephone: +44 (0) 1723 518011 Fax: +44 (0) 1723 518043

Email: sales@pulsarinstruments.com





Certificate of Calibration

Certificate Number : SPR23040182-8

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae Bangkok 10160

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1812

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Apr 2023

Calibration Date : 20 Apr 2023

Recommend Due Date : 20 Apr 2024

Date of Issue : 21 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).


Calibrated by : Mr. Prayoon Topart

Approved by :

(Mr. Nirut Loha)

Calibration

Authorized Signatory



Calibration Report

Certificate Number : SPR23040182-8

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23040182-8

Page : 3 of 3

Range : 20 to 140 dB

Function : @1kHz

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -





Certificate of Calibration

Certificate Number : SPR23070059-9

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkhuae Bangkok 10160

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1807

ID. Number : NSMPUMD44N1807

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Received Date : 05 Jul 2023

Relative Humidity : $50\% \pm 15\%$

Calibration Date : 06 Jul 2023

Location of Calibration : In-Lab

Recommend Due Date : 06 Jul 2024

Calibration Procedure : SP-CPE-04-01

Date of Issue : 07 Jul 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr.Chumpon Dokpikul

Approved by :

Calibration C

Nirut Loha)

Authorized Signatory



Calibration Report

Certificate Number : SPR23070059-9

Page : 2, of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23070059-9

Page : 3 of 3

Range : 94 to 114 dB

Function : @1kHz

Select **A** Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Select **C** Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Select **Z** Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.1	94.1	0.1	0.1	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -





Certificate of Calibration

Certificate Number : SPR23040182-2

Page : 1 of 3

Customer : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae Bangkok 10160

Equipment Name : Sound Level Meter

Manufacturer : Pulsar

Model : 44

Serial Number : PN1805

ID. Number : N/A

Environmental Conditions

Ambient Temperature : $23^{\circ}\text{C} \pm 3^{\circ}\text{C}$

Relative Humidity : $50\% \pm 15\%$

Location of Calibration : In-Lab

Calibration Procedure : SP-CPE-04-01

Received Date : 19 Apr 2023

Calibration Date : 20 Apr 2023

Recommend Due Date : 20 Apr 2024

Date of Issue : 21 Apr 2023

Method of Calibration

This certifies that the above instrument was calibrated in compliance with the calibration system requirement of ISO/IEC 17025:2017 in accordance with reference procedure. Standards used to perform this calibration are certified by to NIST or equivalent, National metrology institute, Natural physical constants, consensus standards. The result reported herein apply only to the calibration of the item described above as received. Our decision rule is to contact the customer if the item pass and fail calibration when the results include the uncertainties and the customer must determine if the results meets their needs.

All calibrations are performed within manufacture's specifications. The calibration certificate shall not be reproduced except in full, without written approval of SP Metrology System (Thailand).

Calibrated by : Mr. Prayoon Topart

Approved by :

Calibration

Mr. Nirut Loha)

Authorized Signatory



Calibration Report

Certificate Number : SPR23040182-2

Page : 2 of 3

Reference Standards

Equipment Name	Model	Serial No.	Certificate No.	Due. Date
Sound Level Calibrator	ST-120	211203773	EEL.BP. 114/0166	17 Jan 2024

Traceability

This certification is traceable to the International System of Unit maintained at :
TISTR - Thailand Institute of Scientific and Technological Research



Result of Calibration

Certificate No. : SPR23040182-2

Page : 3 of 3

Range : 20 to 140 dB

Function : @1kHz

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Unit : dB

Standard Setting	UUC Reading		Error		Uncertainty (±)
	Fast	Slow	Fast	Slow	
94	94.0	94.0	0.0	0.0	0.15
114	114.0	114.0	0.0	0.0	0.15

Note:

The result of calibration was found accurate as show on date and place of calibration only.
This Certificate is not certified for any commercial transaction.

Measurement Uncertainty

The reported uncertainty of measurement is the expanded uncertainty obtained by multiplying the standard uncertainty with the coverage factor $k = 2.00$, providing a level of confidence approximately 95%.

- End of Certificate -



Certificate of Calibration

Certificate No. : 67-420034-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : pH Meter with electrode
pH meter
Manufacturer : Horiba Model : F-74BW-G
Range : N/A pH Resolution : 0.001 pH
Serial No. : B41J0001 ID No. : ELABPHHB74BW01
Electrode
Model : 9615S Serial No. : 9X1K0003

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.
Ambient Temperature : (22.0 to 23.0)° C
Relative Humidity : (50 to 55) %

Date of Received : 20 March 2024

Date of Calibration : 20 March 2024

Date of Issue : 23 March 2024

Calibrated by : Permpon Chanpu

Calibration Method : In-house method CAL-M4201 direct measurement by using standard voltage calibrator and using certified reference material (CRM)

Reference Standard Instruments : This certification is traceable to the International System of Units

1. Multiproduct Calibrator

ID No.	Cert. No.	Due Date	Traceability
400005	SG-E-00307/66	23 Aug 2025	National Institute of Metrology Thailand (NIMT)

2. Standard Buffer Solution

pH	Cert. No.	Lot No.	Exp. Date	Traceability
4.008	61293328	944535	27 Nov 2025	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
6.986	61281486	944537	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025
9.997	61281073	944536	17 Nov 2024	CPA Chem Ltd. Accredited to ISO 17034 and ISO/IEC 17025

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-420034-1

Page : 2 of 2

Result of Calibration :

UUC Condition As-Received : Good

Function : Electrical measurement

pH meter

Performing standard curve by Multiproduct Calibrator at pH (4,7,10)

Adjustment Curve at nominal pH	Applied Voltage (mV)	Nominal Value (pH)	UUC Reading		Correction (mV)	Uncertainty (± mV)
			(pH)	(mV)		
4, 7, 10	177.4800	4	3.998	177.5	0.0	0.12
	0.0000	7	7.000	0.0	0.0	0.086
	-177.4800	10	10.000	-177.4	-0.1	0.12

Function : pH meter with electrode

Performing a three - buffer standard curve using buffer nominal pH (4,7,10)

Adjustment Curve at nominal pH	Standard Buffer (pH)	UUC Reading (pH)	Correction (pH)	Uncertainty (± pH)
4, 7, 10	4.008	4.009	-0.001	0.0084
	6.986	7.000	-0.014	0.0092
	9.997	10.008	-0.011	0.014

Remark

UUC : Unit Under Calibration.

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurment was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o O o -

Handwritten signature



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 66-400546-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhuae 7, Bangkhuae, Bangkok 10160

Equipment : Air Chamber (Incubator)

Manufacturer : M-LAB

Model : BIC-140

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 100613-1

ID No. : ELABBODC140N01

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (25.0 to 26.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (224.0 to 225.0) V

Date of Received : 03 October 2023

Date of Calibration : 03 October 2023

Date of Issue : 06 October 2023

Calibrated by : Permpon Chanpu

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD Probe

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
400029 & 400048	66-400454-1	05 Feb 2024	National Institute of Metrology Thailand (NIMT)

Approved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 66-400546-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

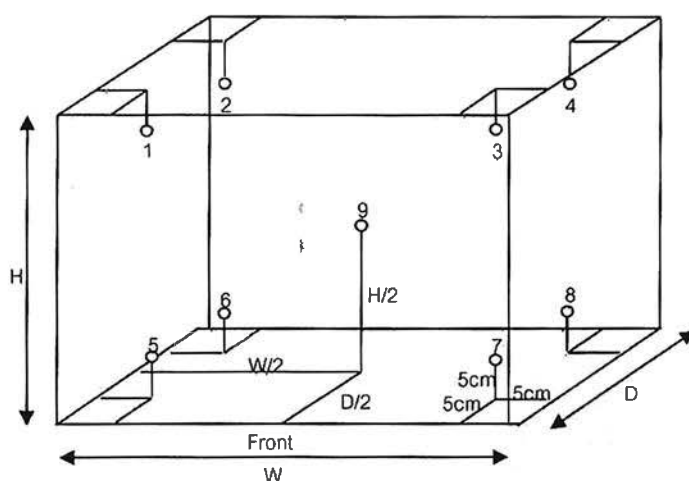

Inside of Chamber

W = 0.38 m

D = 0.35 m

H = 1.15 m

Capacity = 0.15 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
20.0	20.0	20.0	20.18	19.98	20.08	19.97	20.39	20.36	20.20	20.18	20.28	0.30

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
20.0	20.0	20.0	0.35	0.03	0.47

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o O o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 66-400320-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : COD Reactor

Manufacturer : Hanna

Model : HI839800

Range : N/A °C

Resolution : 0.1 °C

Serial No. : 06480040101

ID No. : ELABHI83980001

Environment : Ambient Temperature : (23 ± 2) °C

Relative Humidity : (50 ± 15) %

Date of Received : 02 June 2023

Date of Calibration : 05 June 2023

Date of Issue : 05 June 2023

Calibrated by : Bunjerd Masri

Calibration Method : This instrument was calibrated by In-house method direct measurement with

The temperature scale used was based on ITS-90

Reference Standard Instruments :

Standard Digital Thermometer with TC Type T probe

ID No.

Cert. No.

Due Date

Traceability

400029 & 400030

66-400227-1

24 Oct 2023

National Institute of Metrology Thailand (NIMT)

Approved by :

(Bunjerd Masri)

Supervisor

The Uncertainties are for a confidence probability

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com


Certificate of Calibration

Certificate No. : 66-400320-1

Page : 2 of 2

Result of Calibration : Without Adjustment

Function : Temperature measurement

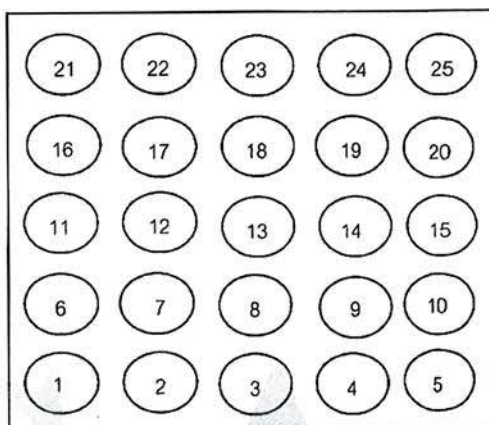

Controller

Test Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Standard Reading at Position (°C)									
			1	2	3	4	5	6	7	8	9	10
150.0	150.0	150.0	149.7	150.1	150.0	149.8	149.5	150.1	151.2	152.1	150.9	150.4
Test Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Standard Reading at Position (°C)									
			11	12	13	14	15	16	17	18	19	20
150.0	150.0	150.0	150.3	151.3	151.5	151.1	150.7	149.9	151.5	152.1	151.1	149.9

Test Point (°C)	UUC Setting (°C)	UUC Reading (°C)	Standard Reading at Position (°C)					Uncertainty (± °C)
			21	22	23	24	25	
150.0	150.0	150.0	149.6	150.5	150.8	150.3	149.8	0.78

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- oOo -





SCIMET Co., Ltd.
1194 Soi Wachirathamsathit 57, Bangchak,
Phrakhanong, Bangkok 10260 Thailand
Email:scimet2022@gmail.com, Tel:095-552-4939

Certificate No. C27240002

Calibration Certificate

Equipment: DO METER
Model: WQ-330-K
Serial No.(or ID): SF9M0013
Manufacturer: HORIBA
Condition: In Condition

Job No.: KSMT2400727
Received Date: 04 March 2024
Issued Date: 05 April 2024
Page: 1 of 2

Customer

Envilab Co., Ltd.
540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkhae, Bangkok 10160

Calibration Place

Environment Laboratory, SCIMET Co., Ltd.
1194 Soi Wachirathamsathit 57, Bangchak, Prakhnong, Bangkok 10260 Thailand

Calibration Date

05 April 2024

Environment Condition

Temperature: 23 °C \pm 2 °C
Humidity: 50 %RH \pm 15 %RH

The Method used

In-house method, W127 , By comparison with certified
dissolved oxygen solution standard

Traceability

This is certificate is traceable to SI Units , Sample test and
temperature test are assured through HANNA instruments
company certificare No. 29E31, through Quality Reborn
Co.,LTD certificare No.QR23-1169

This certificate is issued the units of
measurement according to the International
System of Units (SI). It provides traceability
of measurement to international or national
standard or other recognized national
standard laboratories.

The measurement uncertainty stated is
the expanded uncertainty which is obtained
from the standard uncertainty multiplied by
the coverage factor ($k=2$) to provide a level
of confidence of approximately 95%. It is
determined in accordance with the Guide to
Expression of Uncertainty in Measurement
(GUM).

These results may be affected by
deviations from specified conditions. The
results relate only to the items tested,
calibrated or sampled. The report shall not be
reproduced except in full without approval of

Mr.Dumrong Boonsopon
Person in charge



SCIMET CO.,LTD.
บริษัท ชัยวัฒน์ เทคโนโลยี จำกัด

Mr. Thalerngkeat Pongngarm
Authorized signatory

Calibration Results:

Electrode Serial No. KS9F5037
Model : 300-D-5
Brand : HORIBA

Electrode Test

Atmospheric pressure measured while calibrating. 755.46 mmHg
Temperature measured while calibrating. (± 0.2 °C) 25.0 °C
The Oxygen Solubility was calculated from the ambient conditions. 8.21 \pm 0.03 mg/L
The Oxygen Solubility reading from the DO METER 8.21 mg/L

Sample Test

Standard Oxygen Solution	Unit Under Calibration Reading	Correction	Coverage Factor (<i>k</i>)	Uncertainty of Measurement (\pm)
0.00 mg/L	0.09 mg/L	-0.09 mg/L	2.00	0.13 mg/L


Temperature Electrode

Dimension of Probe;

Length : 105 mn.
Diameter : 16 mn.
Immersion Depth 80 mn.

STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Coverage Factor (<i>k</i>)	Uncertainty of Measurement (\pm °C)
25.02	25.1	-0.08	2.00	0.15

The End of Certificate



ใบตรวจสอบสภาพเครื่อง Do Meter

เลขที่ใบงาน: KSMT2400727

ชนิดเครื่องมือ: DO METER

รุ่น: WQ-330-K

หมายเลขเครื่อง: SF9M0013

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
05 Apr 2024			05 Apr 2024		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด (ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด – เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. อิเล็กโทรด (Electrode and Connection Cable)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. สายอิเล็กโทรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. เชื้อนเซอร์อิเล็กโทรด	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	9. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	-

ข้อแนะนำ :

Mr.Dumrong Boonsopon

Service Engineer

บริษัท ชายนันเบก จำกัด (SCIMET CO., LTD.)

1194 Soi Wachirathamsathit 57, Bangchak, Phrakhanong, Bangkok 10260 Thailand
Email: scimet2022@gmail.com, Tel: 095 552 4939

Certificate of Calibration

Certificate No. : 67-400166-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhak 7, Bangkhak, Bangkok 10160

Equipment : Water Bath
 Manufacturer : Memmert
 Range : N/A °C
 Serial No. : L412.2222
 Model : WNB 14
 Resolution : 0.1 °C
 ID No. : ELABWBWNB29N01

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (29.0 to 30.0) °C

Relative Humidity : (60 to 650) %

Line Voltage : (224.2 to 225.2) V

Date of Received : 20 March 2024

Date of Calibration : 20 March 2024

Date of Issue : 22 March 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : This instrument was calibrated by In-house method CAL-M4006 based on ASTM E715-80
The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with RTD probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400024	66-400547-2	02 Apr 2024	National Institute of Metrology Thailand (NIMT)

ed by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration


Certificate No. : 67-400166-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

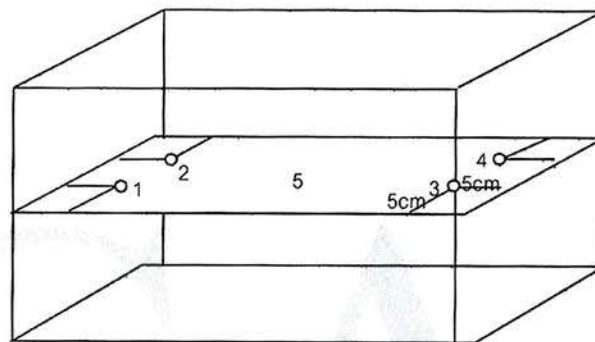

Front

Test Point (° C)	Setting Temperature (° C)	Indicating Temperature (° C)	Measured Temperature (° C) @ Sensor No.					Uncertainty (± ° C)	Measured Uniformity (° C)	Measured Stability (° C)
			1	2	3	4	5			
95.0	94.5	94.5	95.12	95.18	95.11	95.02	95.17	0.23	0.26	0.12

Remark The uncertainty is not combine uniformity of the water bath

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -



Handwritten signature



Certificate of Calibration

Certificate No. : 67-400166-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Temperature controlled enclosure (Oven)

Manufacturer : Memmert

Model : UF 75

Range : N/A °C

Resolution : 0.1 °C

Serial No. : B319.0600

ID No. : ELABHAOVEN0600

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (29.0 to 30.0) °C

Relative Humidity : (60 to 650) %

Line Voltage : (224.2 to 225.2) V

Date of Received : 20 March 2024

Date of Calibration : 20 March 2024

Date of Issue : 22 March 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units
Standard Digital Thermometer with Thermocouple probe

ID No.	Cert. No.	Due Date	Traceability
400046 & 400028	66-400547-3	05 Apr 2024	National Institute of Metrology Thailand (NIMT)

ved by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. :67-400166-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

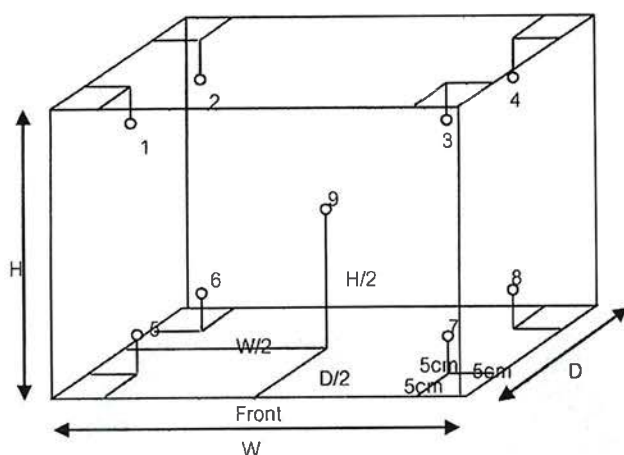

Inside of Chamber

W = 0.40 m

D = 0.33 m

H = 0.56 m

Capacity = 0.07 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
104.0	103.5	103.5	104.1	104.4	104.1	104.3	104.1	104.0	104.0	103.7	104.3	0.70
110.0	109.5	109.5	110.1	110.4	110.1	110.3	110.2	110.1	110.1	109.4	110.3	0.72
180.0	179.0	179.0	179.5	180.9	180.3	180.6	180.5	180.3	180.2	180.2	180.8	0.95

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
104.0	103.5	103.5	0.7	0.1	1.0
110.0	109.5	109.5	1.1	0.1	1.2
180.0	179.0	179.0	1.5	0.2	1.6

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- oOo -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-200060-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540, 540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Electronic Balance
Manufacturer : METTLER TOLEDO **Model :** XSR205DU
Serial No. : B911363567 **ID No. :** ELABBALANCEN06
Capacity : 220 g **Resolution :** 0.00001g/81g, 0.0001g/220g

Environment : On site calibration was carried out at the B304 Balance Room, Envilab Co., Ltd.
Ambient Temperature : (20.0 to 20.5) °C
Relative Humidity : (54.2 to 59.1) %
Air Pressure : 1013.0 mbar

Date of Received : 20 February 2024

Date of Calibration : 20 February 2024

Date of Issue : 21 February 2024

Calibrated by : Satja Sangkhum

Calibration Method : In-house method CAL-M2001 based on UKAS Publication ref : LAB 14
Edition 7 - November 2022

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Weights

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
E261-E2624	C02232088	08 Nov 2024	National Institute of Metrology (Thailand), (NIMT)

Surachai Promthong)
Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-200060-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Departure of indication from nominal value


Nominal Value (g)	Correction (g)	Uncertainty \pm (g)
0.1	0.00000	0.000015
0.5	0.00001	0.000022
1	0.00000	0.000026
2	0.00001	0.000034
5	-0.00001	0.000043
10	0.00000	0.000053
50	0.00003	0.00011
100	0.0001	0.00020
150	0.0001	0.00038
200	0.0002	0.00038

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$, providing a level of confidence of approximately 95%

Eccentric error

Load test : 50 g
A B C D E
0.00000 0.00000 0.00010 0.00000 0.00000 g



Repeatability

Load test : 200 g
Stdev. : 0.000032 g

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-7

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Measuring Pipette

Manufacturer : Witeg

Class : A

Capacity : 1 ml

Graduation : 0.01 ml

ID No. : B-WW-002/21

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1008.1 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241005	66-200388-4	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

The Uncertainties are for a confidence probability of approximately

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-7

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Delivery Time : 4.98 sec.

Nominal Volume (ml)	Measuring Volume (ml)
0.2	0.2006
0.5	0.4992
1	0.9929

Uncertainty of measurement with in \pm 0.0026 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -





MIRACLE INTERNATIONAL TECHNOLOGY CO., LTD

214 Bangwack Rd. Bangpai Bangkac Bangkok 10160
Tel.: 0-2865-4647-8 Fax: 0-2865-4649 <http://www.mit.in.th>



CALIBRATION CERTIFICATE

Certificate No. : S2024040558-0002

Date Issued : 03-May-24

Customer : Envilab Co., Ltd.
540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkhac, Bangkok, Thailand
10160

Equipment : Lab Refrigerator (TMF-PLR221)

Manufacturer : Thermo Scientific

Model : PLR221

Serial No. : 2210M319042801

ID No./Tag No. : ELABREFRIGEN02

Date Received : 02-May-24

Date Calibrated : 02-May-24

Calibrated by : Mr. Varuch Jearrajinda

Calibration Method or Calibration Procedure Used

Standard method : CP-05 TLAS G-20.

This certificate is traceable to national standards, which realize the units of measurement according to the International System of Units (SI).

Result of Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level confidence approximately 95 percent.

This certificate may not be reproduced other than in full except with the prior written approval of the Miracle International Technology Company Limited.

Approved by:

Sarayuth T.
(Mr. Sarayuth Tochua)



Page 1 of 2



Certificate No. : S2024040558-0002

Environment : Ambient Temperature : Start record 26.6 °C, Stop record 26.8 °C
Relative Humidity : Start record 54.1 %RH, Stop record 54.5 %RH

Calibration Temperature (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Stability ¹ (°C)	Measured Uniformity ² (°C)	Overall Variation ³ (°C)
4	4	4	0.88	0.69	1.94

Without adjustment

Calibration Temperature (°C)	STD No. 1 (°C)	STD No. 2 (°C)	STD No. 3 (°C)	STD No. 4 (°C)	STD No. 5 (°C)	STD No. 6 (°C)	STD No. 7 (°C)	STD No. 8 (°C)	STD No. 9 (°C)	Uncertainty ⁴ (°C)
4	4.23	4.35	4.44	4.46	4.35	4.24	4.34	3.96	4.13	1.2

Decision Rule with Guard Band


Calibration Temperature (°C)	No. 1	No. 2	No. 3	No. 4	No. 5	No. 6	No. 7	No. 8	No. 9	MPE (±°C)
4	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass	2

Pass = $|\text{error}| + |\text{uncertainty}| \leq |\text{MPE}|$ MPE = Maximum Permissible Error

Fail = $|\text{error}| + |\text{uncertainty}| > |\text{MPE}|$

Note : Probe No. 9 is Reference Probe

Setting Air Fresh No. 0



Condition As-Received : Used Item

The measurement results and statements of conformity with specification only relate to the item calibrated.

Measurement Standards Used & Traceability :

The International System of Units (SI) through

MIT Certificate No. L202403007-0012 for Digital Thermometer with Probe (Agilent) Module 1 (93) Serial No. MY41008700, Due 10-Sep-24

Notes : 1. The temperature stability is the one-half of greatest maximum difference of measured temperatures at any one probe.

2. The temperature uniformity is the maximum difference of measured temperatures between of any probes and the measured temperature at the reference location which are observed at same time.

3. Overall variation is the difference of maximum and minimum measured temperatures throughout observation time.

4. The uncertainty of measurement is included temperature stability.

5. The temperature uniformity, stability, overall variation and indicating temperature is applicable to all air or gas filled temperature controlled enclosures at atmospheric pressure.

End of Certificate

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-1

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Cylinder

Manufacturer : Witeg

Class : A

Capacity : 25 ml

Graduation : 0.5 ml

ID No. : C-WW-001/23

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.5 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.

Cert. No.

Due Date

Traceability

241002

66-200388-1

02 Jun 2024

National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadee)

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-1

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
10	10.04
25	25.06

Uncertainty of measurement with in \pm 0.049 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-2

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 50 ml

Graduation : 1 ml

ID No. : C-WW-011/23

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.4 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadce)

Supervisor

The Uncertainties are for a confidence probability of approxi

This certificate may not be reproduced other than in full excep



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-2

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
30	29.69
50	49.87

Uncertainty of measurement with in \pm 0.054 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-3

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 100 ml

Graduation : 1 ml

ID No. : C-WW-002/22

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.4 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.

Cert. No.

Due Date

Traceability

241002

66-200388-1

02 Jun 2024

National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wina Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-3

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
50	49.78
100	99.74

Uncertainty of measurement with in \pm 0.063 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-4

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 250 ml

Graduation : 2 ml

ID No. : C-WW-007/23

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.4 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.

Cert. No.

Due Date

Traceability

241002

66-200388-1

02 Jun 2024

National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Tovadcc)

Supervisor

The Uncertainties are for a confidence probability of 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-4

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good


Nominal Volume (ml)	Measuring Volume (ml)
150	150.31
250	250.38

Uncertainty of measurement with in \pm 0.087 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -

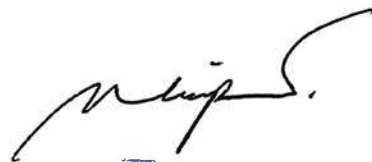

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech_cal@yahoo.com, calibratech_cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-5

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 500 ml

Graduation : 5 ml

ID No. : C-WW-005/21

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (50 ± 10) %

Air Pressure : 1009.3 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Areerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by :

(Wipa Toradec)

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-5

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
250	250.57
500	500.25

Uncertainty of measurement with in \pm 0.12 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS 17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300147-6

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Cylinder

Manufacturer : PYREX

Class : A

Capacity : 1000 ml

Graduation : 10 ml

ID No. : C-WW-001/24

Environment : Ambient Temperature : (20 ± 3) °C
Relative Humidity : (50 ± 10) %
Air Pressure : 1009.3 mbar.

Date of Received : 13 March 2024

Date of Calibration : 19 March 2024

Date of Issue : 19 March 2024

Calibrated by : Arcerat Sombun

Calibration Method : In-house method CAL-M3001 based on ASTM E 542-22

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

ID No.	Cert. No.	Due Date	Traceability
241002	66-200388-1	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by : 

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech-cal@yahoo.com, calibratech-cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300147-6

Page : 2 of 2

Result of Calibration : This result of true Volume is referred to standard temperature at 20 °C

UUC Condition As-Received : Good

Nominal Volume (ml)	Measuring Volume (ml)
500	500.75
1000	1000.66

Uncertainty of measurement with in \pm 0.17 ml

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2.00$,
providing a level of confidence of approximately 95%

- o0o -





AIRFLOW CALIBRATION CO.,LTD.

CERTIFICATION OF TEST REPORT

Equipment	: Biological Safety Cabinet (Class II)	Report Number	: B224051
Manufacturer	: Heal Force	Issued Date	: 1 March 2024
Model	: HFsafe-1200LC	Job Number	: B224051
Serial Number	: EX042012LC5497	Page	: 1 of 7 Pages
Identification Number	: ELABMICROBSC01		

Customer : ENVILAB CO.,LTD. (HEAD OFFICE)
540, 540/1 Soi Bangkhao 7, Bangkhao, Bangkhao, Bang 10160

Environment Condition : Temperature: 20.8 °C ± 0.5 °C
Humidity: 53.0 %RH ± 3.1 %RH
Voltage: 221.5 VAC ± 0.3 VAC

Test Place : ENVILAB CO.,LTD. (HEAD OFFICE) Laboratory Floor 3

Test By : Mr.Achira Kaewpaitoon

Test Date : 29 February 2024

Due Date : 28 February 2025

Test Procedure : EN 12469: 2000 Biotechnology performance criteria for microbiological safety cabinet
AS 1807.23: 2000 Determination of intensity of radiation from germicidal ultraviolet lamp

Traceability : Velocity test is traceable to TAT Certificate Number :TTH-0-86850
Leak test of HEPA filter is traceable to WK Certificate Number :WK2309-176-1
Illumination test is traceable to SP Certificate Number :SPR23030030-1
UltravioletRadiation test is traceable to EEI Certificate Number :CO20230085EA
Sound test is traceable to SP Certificate Number :SPR23030030-2

This calibration certificate documents the traceability to national standards, which realize the unit of measurement according to the International System of Units (SI).

This certificate may not be reproduced other than in full except with the prior written approval of the Air Flow Calibration Company Limited.

Watcharin Tavera
Authorized Signatory

R FM - SV - 08 : 01 Sep 2021

51/104 Moo 9, Ladsawai, Lamlukka Phatumthani 12150 Thailand

Tel : 0 2152 8350 , 0 2152 8348 , 0 2152 8070 ,08 4360 2558 , 09 2265 3175 Fax : 0 2152 8348

[http:// www.airflow-calibration.com](http://www.airflow-calibration.com) E-mail : bm.airflow@gmail.com , nop.airflow@gmail.com.



Primary Test Results

1. Downflow Velocity Test

Test equipment used

- Thermo anemometer
- Brand: Testo
- Model: 425
- Serial number: 3101751
- Calibration due: 6-Nov-2024

Instruction: Work opening in normal positions. With the anemometer inside the MSC, make air velocity measurements in horizontal plane 50 mm to 100 mm above the top edge of the front aperture. Make measurements over a period of at least 1 min in each position. Measure in 2 rows along a line 1/4 of the depth of the working space forward of the rear wall and along a line the same distance behind the front window. Start 150 mm from the left side window and with 300 mm between the measuring spots.

Back			
0.35	0.36	0.35	0.34
0.33	0.35	0.35	0.34
Front			

Characteristic of downflow velocities

Measurement	Mean	Maximum	Minimum	20% of Mean
• Mean downflow velocity to achieve product protection : 0.25 m/s - 0.50 m/s. All measurements should be within $\pm 20\%$ of mean values.	0.35	0.36	0.33	0.28 - 0.42

Result Summary : Pass

AIR FM - SV - 08 : 01 Sep 2021

51/104 Moo 9, Ladswai, Lamukha Phatumthani 12150 Thailand

Tel : 0 2152 8350 , 0 2152 8348 , 0 2152 8070 , 08 4360 2558 , 09 2265 3175 Fax : 0 2152 8348

http://www.airflow-calibration.com E-mail : bm.airflow@gmail.com , nop.airflow@gmail.com



AIRFLOW CALIBRATION CO.,LTD.

Continuation of the Certificate of Test Report Number : B224051

Page 3 of 7 Pages

2. Inflow Velocity Test

Test equipment used

- Thermo anemometer ● Brand: Testo ● Model: 425
- Serial number: 3101751 ● Calibration due: 6-Nov-2024

Exhaust Measurement

Instruction: The alternative procedure to determine inflow velocity uses a thermoanemometer in a constricted window access opening of 3 inches (76mm) with the armrest removed. Inflow air velocity is measured in the center of the constricted opening 1-1/2 inches (38mm) below the top of the work access opening on the following specified grid. Use the correction factor table to calculate the inflow velocity.

Inflow Velocity Table m/s										
1.29	1.28	1.29	1.31	1.32	1.32	1.31	1.32	1.31	1.32	1.32

Characteristic of air velocities in the work opening

Specification	Min. Inflow (m/s)
• Mean Inflow velocity to achieve product protection : ≥ 0.40 m/s.	0.50

Result Summary : Pass

Adjustments Required

Fan speed



No Change

Damper



No Change

AIR FM - SV - 08 : 01 Sep 2021

51/104 Moo 9, Ladsawai, Lamukha Phatumthani 12150 Thailand

Tel : 0 2152 8350 , 0 2152 8348 . 0 2152 8070 , 08 4360 2558 . 09 2265 3175 Fax : 0 2152 8348

http:// www.airflow-calibration.com E-mail : bm.airflow@gmail.com , nop.airflow@gmail.com



AIRFLOW CALIBRATION CO.,LTD.

Continuation of the Certificate of Test Report Number : B224051

Page 4 of 7 Pages

3. Leak Test of HEPA Filters

Test equipment used

- Aerosol Photometer ● Brand: ATI ● Model: 2H
- Serial number: 20627 ● Calibration due: 20-Sep-2024

Test equipment used:

- Aerosol Generator ● Brand: ATI ● Model: 6C
- Serial number: 20554 ● Calibration date: -

Instruction: The aerosol through the "Challenge" valve to the backside of HEPA filter and maximum local penetration: 0.01 % of upstream concentration. (PAO test substitute for DOP test)

Characteristic of PAO test

Concentration of the aerosol used for main HEPA filter	34	µg/l
Downstream concentration of aerosol concentration of main HEPA filter	0.001	%
Downstream concentration of aerosol concentration of main HEPA filter	0.001	%

Main HEPA Filter

Leak position



: 10 cm. x 10 cm. X : Media leak position G : Gasket leak position M : Maximum leak position

AIR FM - SV - 08 : 01 Sep 2021

51/104 Moo 9, Ladsawai, Lamukha Phatumthani 12150 Thailand

Tel : 0 2152 8350 , 0 2152 8348 , 0 2152 8070 , 08 4360 2558 , 09 2265 3175 Fax : 0 2152 8348

http://www.airflow-calibration.com E-mail : bm.airflow@gmail.com , nep.airflow@gmail.com



AIRFLOW CALIBRATION CO.,LTD.

Continuation of the Certificate of Test Report Number : B224051

Page 5 of 7 Pages

Exhaust HEPA Filter

Leak position

☐ : 10 cm x 10 cm X : Media leak position G : Gasket leak position M : Maximum leak position

Result Summary : Pass

4. Airflow Patterns

Test equipment used

Smoke Generator

Instruction : The purpose of the test is to verify that no smoke escapes from the working space to the room, and that smoke will be drawn into the working space from the room.

Pass the smoke in an easy movement along the front opening outside the cabinet. The smoke must be drawn into the cabinet without visible turbulence.

Test the laminarity of the downflow and along the side-and back wall. No smoke must come out in the room and only small Turbulence must be observed.

Result Summary :

Downflow Pattern Test

Pass

View Screen Retention Test

Pass

Work Opening Edge Retention Test

Pass

Sash/Window Seal Test

Pass

AIR FM - SV - 08 : 01 Sep 2021

51/104 Moo 9, Ladsawai, Lam Lukka Phatumthani 12150 Thailand

Tel : 0 2152 8350 , 0 2152 8348 , 0 2152 8070 , 08 4360 2558 , 09 2265 3175 Fax : 0 2152 8348

http:// www.airflow-calibration.com E-mail : bm.airflow@gmail.com , nsp.airflow@gmail.com



AIRFLOW CALIBRATION CO.,LTD.

Continuation of the Certificate of Test Report Number : B224051

Page 6 of 7 Pages

5. Site Installation

5.1 Sash Alarm	Pass
5.2 Interlocks	N/A
5.3 Exhaust System Alarm	N/A

6. Soap Solution

Instruction: Comprising 25g/l soft soap in tepid distilled water prepared in grease free vessel.

Result Summary : Absence of soap bubbles. N/A

Secondary Test Results

7. Illumination Test

Instruction: Take readings at approximately 300 mm centres across the full front width of the work floor surface, starting approximately 150 mm in from each side.

Test equipment used

- Lux meter
- Brand: Daiichi
- Model: LM507
- Serial number: 1300421511013
- Calibration due: 2-Mar-2024




Back

819	923	944	1059	1049
-----	-----	-----	------	------

Front

Lighting should be adequate for safe working within the cabinet. Illumination measured at the work surface should be at least 750 lux.

Result Summary : Pass

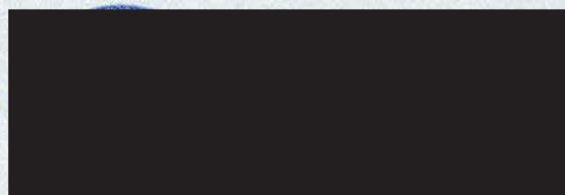

AIR FM - SV - 08 : 01 Sep 2021

51/104 Moo 9, Ladsawai, Lam Lukka Phatumthani 12150 Thailand

Tel : 0 2152 8350 , 0 2152 8348 , 0 2152 8070 , 08 4360 2558 , 09 2263 3175 Fax : 0 2152 8348

http://www.airflow-calibration.com E-mail : bm.airflow@gmail.com , nnp.airflow@gmail.com



AIRFLOW CALIBRATION CO., LTD.

Continuation of the Certificate of Test Report Number : B224051


Page 7 of 7 Pages

8. Ultraviolet Radiation Test

Instruction: Take readings at approximately 300 mm centres across the full front width of the work floor surface, starting approximately 150 mm in from each side.

Test equipment used

- UVC Light Meter
- Brand: Lutron
- Model: UVC-254SD
- Serial number: Q853539
- Calibration due: 26-Sep-2024



Back				
2300	2920	3350	2080	1960
Front				

Ultraviolet radiation where UV lamps are fitted, the intensity of radiation at a wave length of 254 nm shall be not less than 400 mW/m^2 when measured at the work floor surface.

Result Summary : Pass

9. Sound levels Test

Instruction: Sound levels in a cabinet should be low enough not to distract a worker. When tested in accordance with EN ISO 3744 using a sound level meter situated 1.0 m from the centre of the front aperture of the cabinet, or 1.0 m from any part of the installation within the laboratory, the A-weighted sound pressure level generated by the cabinet should not exceed 65 dB when the A-weighted sound pressure level of the background is less than 55 dB. If the background noise exceeds 55 dB then the corrected cabinet A-weighted sound pressure level should not exceed 65 dB.

Test equipment used

- Sound Meter
- Brand: Daiichi
- Model: SL332
- Serial number: 19090231
- Calibration due: 2-Mar-2024

* Sound pressure level of the background: 50.6 dBA

* Sound levels: 59.2 dBA

Result Summary : Pass

End of Certificate

AIR FM - SV - 08 : 01 Sep 2021

51/104 Moo 9, Ladsawai, Lamlukka Phatumthani 12150 Thailand

Tel : 0 2152 8350 , 0 2152 8348 , 0 2152 8070 , 08 4360 2558 , 09 2265 3175 Fax : 0 2152 8348

http:// www.airflow-calibration.com E-mail : bm.airflow@gmail.com , nsp.airflow@gmail.com

CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



Certificate of Calibration

Certificate No. : 67-400054-2

Page : 1 of 2

Submitted by : Envilab Co., Ltd.
540,540/1 Soi Bangkhae7, Bangkhae, Bangkok 10160

Equipment : Autoclave
Manufacturer : Tomy Model : SX-500
Range : N/A °C Resolution 1 °C
Serial No. : 55133094 ID No. : N/A

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.
Ambient Temperature : (30.0 to 31.0) °C
Relative Humidity : (50 to 55) %
Line Voltage : (224.0 to 225.0) V

Date of Received : 01 February 2024

Date of Calibration : 01 February 2024

Date of Issue : 03 February 2024

Calibrated by : Permpon Chanpu

Calibration Method : This instrument was calibrated by In-house method CAL-M4007 based on
BS 2646 Part 1 : 2021

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Temperature Data Logger with RTD pt 100

ID No.	Cert. No.	Due Date	Traceability
400039	66-400707-1	27 Jun 2024	National Institute of Metrology Thailand (NIMT)
400040	66-400707-2	27 Jun 2024	National Institute of Metrology Thailand (NIMT)
400041	66-400707-3	27 Jun 2024	National Institute of Metrology Thailand (NIMT)

by :

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration


Certificate No. 67-400054-2

Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

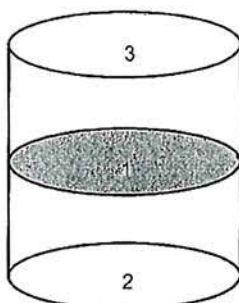

Front

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.			Uncertainty (± °C)	Measured Uniformity (°C)	Measured Stability (°C)	Sterilizing Time (minute)	Pressure Gauge Reading (MPa)
			1	2	3					
121	121	121	121.4	121.4	121.4	1.0	1.0	0.5	15	0.11

Remark

1. UUC : Unit Under Calibration
2. Pressure Gauge reading are out of accreditation's scope.

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

- o0o -

Handwritten signature



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaprachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-300021-2

Page : 1 of 2

Submitted by : Envilab Co.,Ltd.

540, 540/1 Soi Bangkhac 7, Bangkhac, Bangkok 10160

Equipment : Piston Pipette

Manufacturer : sartorius

Model : N/A

Serial No. : 4538803008

ID No. : ELABMICROPP005

Capacity : 100 µl to 1000 µl

Resolution : 5 µl

Environment : Ambient Temperature : (20 ± 3) °C

Relative Humidity : (55 ± 10) %

Air Pressure : (1007.9 to 1008.1) mbar.

Date of Received : 18 January 2024

Date of Calibration : 20 January 2024

Date of Issue : 20 January 2024

Calibrated by : Wipa Tovadee

Calibration Method : In-house method CAL-M3002 base on ISO 8655-6 : 2022-04

Reference Standard Instruments : This certification is traceable to the International System of Units

Electronic Balance

<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>	<u>Traceability</u>
241003	66-200388-2	02 Jun 2024	National Institute of Metrology (Thailand) (NIMT)

Approved by:

(Wipa Tovadee)

Supervisor

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.

CAL-F0031-03



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com

Certificate of Calibration

Certificate No. : 67-300021-2

Page : 2 of 2

Result of Calibration : Without Adjustment

based on the gravimetric determination of the quantity of water which is converted to true volume at the standard temperature of 20 °C

Setting Volume (µl)	Measuring Volume (µl)	e_s (µl)	η_s (%)	S_r (µl)	C_v (%)	Uncertainty (± µl)	Coverage Factor (k)
100	99.47	-0.53	0.53	0.10	0.10	3.1	2.00
500	498.36	-1.64	0.33	0.06	0.01	3.2	2.00
1000	997.93	-2.07	0.21	0.07	0.01	3.3	2.00

Note : e_s : Systematic error (µl), η_s : Relative systematic error (%)

S_r : Standard deviation (µl), C_v : Coefficient of variation (%)

The formula used to convert weighing values into volume is

$$V_{20} = M \times Z$$

V_{20} = is the water volume at standard temperature of 20 °C

M = is the balance reading of delivered water

Z = is the combined factor for buoyancy correction and conversion from mass to volume

UUC Condition As-Received : Good

UUC Calibrated to delivery (Ex) by using : White Tip

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor (k)

providing a level of confidence of approximately 95%

- o0o -



CAL

Calibratech Co.,Ltd.

7/106-7 Moo 2, Sukhaphrachasan 3 Rd., Bangpood, Pakkred, Nonthaburi 11120

Tel.(02) 964-6211 Fax.(02) 964-5155, e-mail : calibratech.cal@yahoo.com, calibratech.cal@hotmail.com



NSC-TISI-TIS17025
CALIBRATION 0030

Certificate of Calibration

Certificate No. : 67-400101-1

Page : 1 of 2

Submitted by : Envilab Co., Ltd.

540, 540/1 Soi Bangkhae 7, Bangkhae, Bangkok 10160

Equipment : Temperature controlled enclosure (Incubator)

Manufacturer : Memmert

Model : IF 110

Range : N/A °C

Resolution : 0.1 °C

Serial No. : D419.0525

ID No. : ELABINCUBATOR1

Environment : On site calibration was carried out at the Laboratory, Envilab Co., Ltd.

Ambient Temperature : (23.0 to 24.0) °C

Relative Humidity : (50 to 55) %

Line Voltage : (223.0 TO 225.0)V

Date of Received : 20 February 2024

Date of Calibration : 20 February 2024

Date of Issue : 22 February 2024

Calibrated by : Kittisak Kokaeo

Calibration Method : CAL-M4004, TLAS G-20

The temperature scale used was based on ITS-90

Reference Standard Instruments : This certification is traceable to the International System of Units

Standard Digital Thermometer with RTD Probe

ID No.

Cert. No.

Due Date

Traceability

400046 & 400042

67-400047-1

25 Jul 2024

National Institute of Metrology Thailand (NIMT)

(Surachai Promthong)

Laboratory Manager

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full except with the prior written approval of the Calibratech Co.,Ltd.



Certificate of Calibration

Certificate No. : 67-400101-1


Page : 2 of 2

Result of Calibration : Without Adjustment

UUC Condition As-Received : Good

Function : Temperature measurement

This instrument was setting air ventilation at position 0 (close)

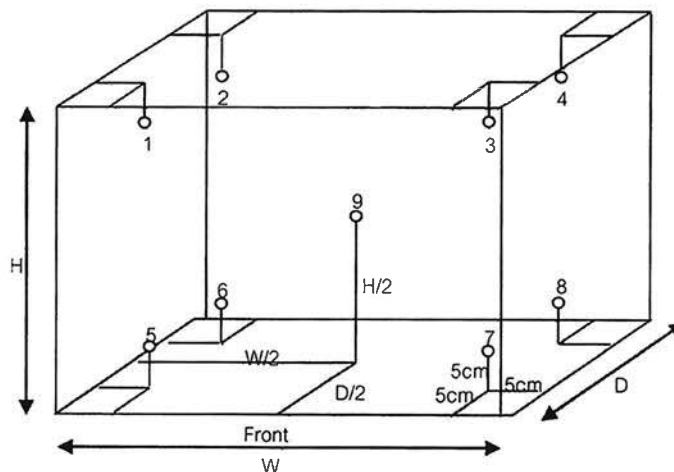

Inside of Chamber

W = 0.56 m

D = 0.48 m

H = 0.40 m

Capacity = 0.11 m³

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Temperature (°C) @ Sensor No.									Uncertainty (± °C)
			1	2	3	4	5	6	7	8	9	
35.0	35.0	35.0	35.00	35.10	35.16	35.14	35.15	35.14	35.03	35.00	35.12	0.30
37.0	37.0	37.0	37.01	37.11	37.17	37.15	37.16	37.15	37.04	37.01	37.13	0.30

Test Point (°C)	Setting Temperature (°C)	Indicating Temperature (°C)	Measured Uniformity (°C)	Measured Stability (°C)	Overall Variation (°C)
35.0	35.0	35.0	0.1	0.0	0.2
37.0	37.0	37.0	0.1	0.0	0.2

Remark The uncertainty is not combine uniformity of the air chamber

This result of calibration was found accurate as shown on date and place of calibration only.

This reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2 , providing a level of confidence of approximately 95%

- o0o -

Signature





PinAAcle 900F Preventive Maintenance Report

Company Name:

Envilab Co.,Ltd

Instrument Location: 540/1 ซอยบางแค 7, แขวงบางแค เขตบางแค

กรุงเทพมหานคร 10160


Instrument Serial No.:

PFBS20011403

Date: 05-Apr-2024

PinAAcle 900F Preventive Maintenance (PM)

Company Name:	Envilab Co.,Ltd		
Address (Instrument Location):	540/1 ซอยบางแค 7, แขวงบางแค เขตบางแค กรุงเทพมหานคร 10160		
Serial Number:	PFBS20011403	PM Number:	4/4
Customer Name (if applicable):	K.Janjira	Telephone Number:	095-550-0510
Customer Support Engineer Name:	Khwanchai	Service Order Number:	WO-02707812
Date PM Performed: (DD-MMM-YYYY)	05-Apr-2024	Next PM Due Date: (DD-MMM-YYYY)	05-Oct-2024
Standard Labor Hours to Complete PM :		5 hours	

Part Number	Release	Publication Date	
09370145 Rev.9	A	January 2018	

Scope

The purpose of this PM is to ensure the continued functionality of the PinAAcle 900F by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

The customer must provide the engineer operational data to demonstrate recent instrument performance prior to starting the PM.

Always check with the customer before making any changes that may affect the customer's analysis or calibration, including a current back-up of system software and/or data files.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc.

Copyright © 2013 PerkinElmer, Inc.

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no Warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Configuration Notes

Parts Lists

Parts Included with the PM		
Part Number (if applicable)	Description	Quantity
B0501696	Fan Filters	N/A
N3160156	O-Ring Kits for Sampling Introduction (Stainless Steels Nebulizer)	N/A
N3160157	O-Ring Kits for Sampling Introduction (Plastic Nebulizer)	N/A
N9301714	Replacement Acetylene Filter Cartridge	N/A
TH001022	Replacement Air Filter Cartridge	N/A

Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quality	Batch/Lot #	Expired Date (MM/YY)
N9300183	1000 mg/L Copper Standard	AR	27-39CUY1	04/25

Additional Reagents and Standards Required for PM (Customer Support Solution)				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
N/A	DI Water	250 ml.	AR	AR
N/A	0.5% HNO ₃	250 ml.	AR	AR

Additional Tools Required for PM			
Part Number (if applicable)	Description	Quantity	Serial #
N1013000	0.2A Neutral density filter	1	MG0-056
N1013002	1.0A Neutral density filter	1	MG2-054
03030997	System 2 EDL Driver	1	03030997
N3050605	As System 2 EDL	1	16148
N3050121	Cu Lumina HCL	1	092216-010130
N3050109	Ba Lumina HCL	1	102416-040160
N3050139	K Lumina HCL	1	110716-010060
N3050152	Ni Lumina HCL	1	100516-030190

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.
- ☒ Inspect the customer log book and make any appropriate PM entries.
- ☒ Perform general inspection of system for cleanliness.

2. PC Instrument Software:

- ☒ Instrument Software user files/databases archived, packed, and/or deleted as needed.

3. Mechanical:

- ☒ Inspect and clean all fans and filters. Replace filters if necessary
- ☒ Inspect all gas lines for leaks and/or wear. Replace if needed.
- ☒ Clean exterior of the instrument.
- ☒ Inspect the burner head, burner chamber, and nebulizer. Clean if needed as stated in the Hardware Guide.
- ☒ Check burner head dimensions with the feeler gauge as stated in the Hardware Guide in the Maintenance chapter section on cleaning the burner head and checking sloth width. Replace if out of specification
- ☒ Check the condition of the end cap, burner head, and nebulizer O-rings. Replace if necessary.
- ☒ Check the drain system for signs of wear. Replace worn or damaged parts.
- ☒ Visually check for proper flame conditions when igniting the Air-C₂H₂ and N₂O-C₂H₂ flames (if applicable).

4. Electrical:

- ☒ Inspect PC boards. Clean if necessary.
- ☒ Carefully check all internal and external cable connections.
- ☒ Check instrument firmware revisions upgrade to current levels (if necessary)
- ☒ Run Diagnostics Test within the Advanced function of the Spectrometer page. Check the results in the service log folder in the Spectrometer BM Log Viewer.

5. Optics:

- ☒ Inspect and clean the sample compartment windows, if needed.
- ☒ Inspect optics. Clean or replace if necessary,

6. Gasses:

- ☒ Verify that the Gasses supplied to the instrument are within the pressure and purity specifications found in the PinAAcle 900 Series Pre-installation Checklist SDB.
- ☒ Verify that the acetylene filter and air filter element is dry. Replace if necessary.

7. Flame Interlock Check:

Description: Check to ensure that all safety interlocks are closed.

Parameter	Specification	Test Results	Pass/Fail
Flame Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Drain Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Nebulizer Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
C ₂ H ₂ Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Air Pressure Sensor	Air/C ₂ H ₂ Flame correctly shuts down	Active	Passed
Burner Head Sensor	Choosing Nitrous Oxide as the oxidant should trigger an interlock shuts down	Active	Passed

8. After PM Performance tests:

8.1 Detector Linearity with Barium

Description: Ensures that the detector is linear in the Visible Range.

Parameter	Specification	Certificate Value at 553.6 nm (Abs.)	Test Results	Pass/Fail
1.0 A ND Filter	± 5% from Cert.	1.0531	1.0606	Passed
0.2 A ND Filter	± 5% from Cert.	0.1806	0.1840	Passed

8.2 Baseline Noise at 1.0 Absorbance with Barium

Description: Ensures that a high absorbance will not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0020	Passed

8.3 AA Baseline Noise with Copper

Description: Check baseline noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.001	0.0004	Passed

8.4 D₂ Background Compensation with Copper

Description: Verifies the instruments ability to compensate for Background absorption.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.010	0.0069	Passed

8.5 AA-BG Baseline Noise with Copper

Description: Ensures that background correction does not produce excessive noise.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0005	Passed

8.6 AA-BG Baseline Noise with Arsenic

Description: Ensures that background correction does not produce excessive noise at a low wavelength.

Parameter	Specification	Results	Pass/Fail
Standard Deviation	≤ 0.005	0.0003	Passed

8.7 Flame Sensitivity

Description: Instrument Sensitivity checked against Copper standard.

Standard Copper Sensitivity	Specification	Results (Abs.)	Pass/Fail
5 mg/L Sensitivity SS Neb (if applicable)	> 0.250 Abs.	-	Not Applicable
2 mg/L Sensitivity HS Neb (if applicable)	> 0.250 Abs.	0.3090	Passed

10. Review:


- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer supplied materials to have on hand.
- ☒ Attach PM sticker.

Additional Comments

Additional Comments Regarding the PM	

Review

<p><i>The preventive maintenance checks and if applicable performance tests for PinAAcle 900F have been completed.</i></p>	
<p><i>This PinAAcle 900F Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.</i></p>	
<p>Review of Preventive Maintenance:</p>	
<p>Authorized PerkinElmer Representative:</p> <p><i>KL.S</i></p>	<p>Date:</p> <p>05-Apr-2024 (DD-MMM-YYYY)</p>
<p>Authorized Customer Representative:</p> <p><i>6996957</i></p>	<p>Date:</p> <p>05-Apr-2024 (DD-MMM-YYYY)</p>

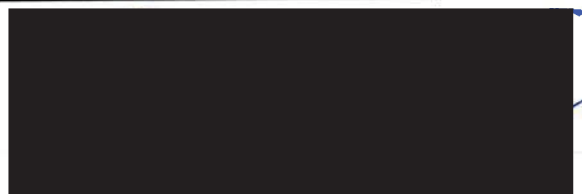

Atomic Absorption/FIAS 100/400 Preventive Maintenance (PM)			
Company Name:	Envilab Co.,Ltd		
Address (Instrument Location):	540/1 ซอยบางแค 7, แขวงบางแค เขตบางแค กรุงเทพมหานคร 10160		
Room Number:	-		
Asset Number (if applicable):	100S20010501	Customer System ID:	
Service Engineer Name:	Pattrayut W.	Service Order Number:	WO-02707811
Date PM Performed: (DD-MMM-YYYY)	05-Apr-2024	Next PM Due Date: (DD-MMM-YYYY)	05-Oct-2024

Part Number	Release	Publication Date	
09370005	C	January 2013	

Scope

The purpose of this PM is to ensure the continued functionality of the Atomic Absorption/FIAS 100/400 by inspecting and replacing any worn or damaged parts. This service should only be performed by a trained representative of PerkinElmer.

The customer should save their method before the PM begins.

General Instructions:

Always check with the customer before making any changes that may affect the customer's analysis or calibration.

The completed document should be signed by an authorized PerkinElmer and customer representative and left with the customer.

Update the PM sticker and instrument logbook as required.

Copyright Information

This document contains proprietary information that is protected by copyright. All rights are reserved.

No part of this publication may be reproduced in any form whatsoever or translated into any language without the prior, written permission of PerkinElmer, Inc. **Copyright © 2013 PerkinElmer, Inc.**

Trademarks

Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are protected by law. PerkinElmer is a registered trademark of PerkinElmer, Inc. All other trademarks and registered trademarks not owned by PerkinElmer, Inc. or its subsidiaries that are depicted herein are the property of their respective owners.

Except as specifically set forth in its terms and conditions of sale, PerkinElmer makes no warranty of any kind with regard to this document, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

PerkinElmer shall not be liable for incidental or consequential damages in connection with the furnishing or use of this document.

Component List

Component / Specific Model	Serial #	Firmware Version	Configuration Notes

Parts Lists

Parts Included with the PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)
B050 2706	Fan Filter	1	N/A	

Additional Tools Required for PM				
Part Number (if applicable)	Description	Quantity	Serial #	Calibration Due Date (MM/YY)
	Digital Volt Meter	1	N/A	
Additional Reagents and Standards Required for PM				
Part Number (if applicable)	Description	Quantity	Batch/Lot #	Expiration Date (MM/YY)

Procedure Checklist

Use (✓) to check off those steps in the checklist that have been completed.

1. General:

- ☒ Review the instrument performance with the customer and document any recent problems.

-
- ☒ Is the Working Environment Acceptable? If not, document.

-
- ☐ Visual Damage (if yes, describe)

-
- ☒ Check incoming AC line voltage for proper levels and grounding.
 - ☒ Verify Voltage switch on back of instrument is correct
 - ☒ Perform general inspection of system for cleanliness. Clean if needed.
 - ☒ Gas supply cylinders secured, lines leak checked and argon or nitrogen supply pressure verified (45 – 58 psi).
 - ☒ Inspect the customer log book and make any appropriate PM entries.
 - ☒ Fan checked and filter cleaned
 - ☒ Heating mantle or Universal Cell Holder checked

2. Instrument components

- ☒ Non-return valve checked/repaired/replaced if needed (B019 8111). Clean the valve if there is any liquid in it. Replace the rubber sleeve (B013 5123) if it is worn. Check the flow meter for any signs of fluid in it. Clean the flow meter if needed.
- ☒ Verify condition of pump pressure adjustment levers (B050 7794 - look for cracks or problems with the springs), pump rollers (B300 0251 check for wear), and thumb screws (B050 7796).
- ☒ Check the Multiport valve for proper switching, flow, and insure there are no leaks. Clean valve parts and replace o-rings if needed (large o-ring: B050 1250, small o-ring: B004 5095). Use a squirt bottle & fishing line to try to dislodge clogs.
- ☒ Firmware Version checked. Latest is 2.20.

3. Mixing/Separation Assembly & Pump Tubing:

- ☒ Mixing separator assembly checked
- ☒ Filter/membrane checked (B050 8306)
- ☒ Condition of the pump tubing (replace if necessary), correct pump tubing for the solutions being run. Make sure the correct magazines are being used. B050 7791 for 0.13 – 1.80 mm tubing; B050 7792 for 1.60 – 3.18 mm tubing.

4. Cell, Cell Windows, Transfer Line:

- ☒ Cell checked
- ☒ Cell windows checked
- ☒ Transfer line checked for moisture (if moisture is a problem, the Nafion dryer might be needed)

5. Operational Tests:

- ☒ Run DI water through the carrier/reductant/sample system. Verify smooth flow of liquid throughout without leaks. Replace tubing & fittings if needed.



6. Review:

- ☒ Review with the customer PM work performed.
- ☒ Review with the customer routine maintenance procedures.
- ☒ Discuss recommended customer-supplied materials to have on hand.
- ☒ Attach PM sticker.
- ☒ Update Logbook.

Additional Comments

Additional Comments Regarding the PM

Review

<i>The preventive maintenance checks and if applicable performance tests for FIAS 100/400 have been completed.</i>	
<i>This FIAS 100/400 Passes <input checked="" type="checkbox"/> Fails <input type="checkbox"/> the preventive maintenance.</i>	
Review of Preventive Maintenance:	
Authorized PerkinElmer Representative: 	Date: 05-Apr-2024 (DD-MMM-YYYY)
Authorized Customer Representative: 	Date: 05-Apr-2024 (DD-MMM-YYYY)



Document History

Revision	Description of Change	Page(s)	Date
A	First release		May 2008
B	Addition of Batch/Lot Number, Expiration Date, and Report Fields.	2,7	February 2009
C	Update to new format	All	January 2013



PerkinElmer TruQ

PerkinElmer Number: N9300183
Element and Matrix: 1000 µg/mL Copper in 2% HNO₃
Starting Material: Copper Metal
Starting Material Lot No: 06201C
Density: 1.011 g/mL @ 20°C

Lot No: 27-39CUY1
Certification Date: OCT -- 2023
Expiration Date: APR 30 2025

Trace Metallic Impurities in the Actual Solution via ICP / ICP-MS Analysis:

Element	µg/mL	Element	µg/mL	Element	µg/mL	Element	µg/mL	Element	µg/mL
Ag	0.001	Dy	<0.001	Li	<0.001	Pt	<0.001	Tb	<0.001
Al	0.003	Er	<0.001	Lu	<0.001	Rb	<0.005	Te	<0.001
As	<0.001	Eu	<0.001	Mg	0.002	Re	<0.001	Th	<0.001
Au	<0.001	Fe	0.02	Mn	<0.001	Rh	0.002	Ti	<0.001
B	<0.001	Ga	<0.001	Mo	<0.001	Ru	<0.001	Tl	<0.001
Ba	<0.001	Gd	<0.001	Na	<0.001	Sb	0.004	Tm	<0.001
Be	<0.001	Ge	<0.001	Nb	<0.001	Sc	<0.001	U	<0.001
Bi	<0.001	Hf	<0.001	Nd	<0.001	Se	<0.006	V	<0.001
Ca	<0.01	Hg	<0.001	Ni	<0.002	Si	<0.1	W	<0.001
Cd	<0.001	Ho	<0.001	P	<0.5	Sm	<0.001	Y	<0.001
Ce	<0.001	In	<0.001	Pb	0.004	Sn	0.002	Yb	<0.001
Co	<0.001	Ir	<0.001	Pd	<0.001	Sr	<0.001	Zn	<0.02
Cr	<0.001	K	0.5	Pr	<0.001	Ta	<0.001	Zr	<0.001
Cs	<0.001	La	<0.001						

Traceability Documentation for Solution Standard:

Certified Value: 999 µg/mL ±5 µg/mL (refer to side 2)

Certified Value is Traceable to: NIST SRM #3114

* Classical Wet Assay: 998 µg/mL

Method: EDTA titration using PAN as indicator. EDTA standardized against Pb(NO₃)₂ NIST SRM #928.

*Instrument Analysis using ICP Spectrometer: 1000 µg/mL
via NIST SRM #3114

We guarantee that our PerkinElmer TruQ Atomic Spectroscopy Standards are stable and accurate to ±0.5% of certified concentration until the expiration date, provided the standards are kept tightly capped and stored under normal laboratory conditions. This value is the sum of cumulative errors associated with the analytical determinations, pipetting, and diluting to final volume. For these solutions we use high purity acids, ASTM Type 1 water (18 megohm double deionized), and leached, triple-rinsed bottles. All glassware used is class A.

Certifying Officer:

Y. Parikh
Yogesh Parikh, Senior Spectroscopist

PerkinElmer Secondary Spectrometric Calibration Standards

Certificate of Calibration

for

Report Number: MG2-054-20110324

Ordinate Calibration

Calibration Data for Gray Glass Secondary Calibration Standards:

Wavelength / Absorbance	Number	Ordinate Reading (Absorbance) at the following wavelengths:							
Wavelength		193.70	324.80	553.60	766.50				
Standard 1	MG2-054	1.0904	1.0082	1.0531	1.0170				

The uncertainty of the given absorbance values is ± 0.003 A at the given wavelengths.

The uncertainty is the expanded uncertainty expressed at an approximate level of confidence of 95% and a coverage factor of $k=2$ based on JCGM 100:2008 Evaluation of measurement data - Guide to the expression of uncertainty in measurement.

Conditions of Calibration

The following settings were used on the Lambda 900 UV/Vis/NIR Spectrometer employed to obtain the calibration data quoted on this certificate:

Measurement of Calibration

Ordinate mode	Absorbance		
Slit mode UV/Vis	Fix	Slit UV/Vis	1 nm
Integration time UV/Vis	5 s		
Slit mode NIR	Servo	Slit NIR	Servo
Integration time NIR	5 s	Gain	2

The instrument's wavelength program facility was used to measure the absorbance of the standards at the wavelength given above.

This set of Spectrometric Solution was calibrated on a PerkinElmer high performance Lambda 900 UV/Vis/NIR Spectrometer.

Serial Number: 89015

This instrument is used solely for calibration purposes. The most recent quality control check of this instrument was performed on:

Date / Time: 3/17/2011

using the standard PerkinElmer quality control procedure. A set of NIST or NBS/PTB Standard Reference Standard Materials:

NIST model SRM 1930 filter set S/N 155 Calibration Date 11/05/2009 NRC Calibration Report No. PAR 2009 2759

was used during this procedure. Measurements were performed at an ambient temperature of: 24.1 C° and the humidity of: 18 %

Date / Time: 3/24/2011 / 11:15:32 AM

Operator: Cam Le Horvath

Signature:



PerkinElmer LAS, Inc., 710 Bridgeport Avenue, Shelton, CT 06484-4794, USA

End of Report



CERTIFICATE OF CALIBRATION
Test Standard for Instrument Performance Validation
(ISO 9000, GMP, GLP)

This is to certify that this PerkinElmer Reference Standard was tested and verified to be in conformance with all applicable quality requirements, including specifications, drawings, calibration, preservation, packing, marking requirements and part identification.

Declaration of Validation


The Reference Standard was found to meet its functional and performance specification prior to shipment. To support this declaration, the following Engineering, Production and Test Documents are held by PerkinElmer and are available for reference upon request in justified cases and to an appropriate extent:

The Test Specification
The Final Test Protocol
The Records of the Primary Standard
The Calibration Records

Note: PerkinElmer will maintain possession of all documents; their reproduction may require a nondisclosure agreement to be provided by those requiring access to them.

The existence of these documents and the procedures used in their production are formal requirements of the PerkinElmer Quality System. The integrity of this PerkinElmer Quality System is routinely audited and is certified by the British Standards Institution as meeting all the requirements of ISO 9001, the internationally recognized standard for Quality Assurance.

This document shall not be reproduced except in full without the express written approval of the PerkinElmer UV Standards Certification Laboratory.



Quality Manager PKI RMCL
PerkinElmer Instruments
Shelton, CT. USA

PerkinElmer Inc., Shelton, CT 06484 USA An ISO 9001 Company



Secondary Spectrometric Calibration Standards

Certificate of Calibration

Ordinate Calibration

Calibration Data for Secondary Calibration Standards:

Wavelength / Absorbance	Number	Ordinate Reading (Absorbance) at the following wavelengths:							
Wavelength		193.70	324.80	553.60	766.50				
Standard 1	MG0-056	0.2483	0.1857	0.1806	0.1674				

The tolerance of the given absorbance values is ± 0.006 A in the ultra violet and visible range, and ± 0.010 A in the near infrared range. The uncertainty is the sum of the tolerance of the primary NIST/PTB reference material, the measurement reproducibility, and an estimated bias due to the possible systematic errors.

We recommend that you recalibrate this set of spectrometric standards once a year.

Conditions of Calibration

The following settings were used on the Lambda 900 UV/Vis/NIR Spectrometer employed to obtain the calibration data quoted on this certificate:

Measurement of Calibration

Ordinate mode	Absorbance		
Slit mode UV/Vis	Fix	Slit UV/Vis	1 nm
Integration time UV/Vis	5 s		
Slit mode NIR	Servo	Slit NIR	Servo
Integration time NIR	5 s	Gain	2

The instrument's wavelength program facility was used to measure the absorbance of the standards at the wavelength given above.

This set of Spectrometric Solution was calibrated on a PerkinElmer high performance Lambda 900 UV/Vis/NIR Spectrometer.

Serial Number: 89015

This instrument is used solely for calibration purposes. The most recent quality control check of this instrument was performed on:

Date / Time: 9/18/2010

using the standard PerkinElmer quality control procedure. A set of NIST or NBS/PTB Standard Reference Standard Materials certified on:

Date: NIST 1930 S/N 155 11/05/2009

was used during this procedure. Measurements were performed at an ambient temperature of: 25.6 C° and the humidity of: 14 %

Date / Time: 12/20/2010 / 1:48:28 PM

Operator: Cam Le Horvath

Signature:



PerkinElmer Instruments, 710 Bridgeport Avenue, Shelton, CT 06484-4794



CERTIFICATE OF CALIBRATION
Test Standard for Instrument Performance Validation
(ISO 9000, GMP, GLP)

This is to certify that this PerkinElmer Reference Standard was tested and verified to be in conformance with all applicable quality requirements, including specifications, drawings, calibration, preservation, packing, marking requirements and part identification.

Declaration of Validation


The Reference Standard was found to meet its functional and performance specification prior to shipment. To support this declaration, the following Engineering, Production and Test Documents are held by PerkinElmer and are available for reference upon request in justified cases and to an appropriate extent:

The Test Specification
The Final Test Protocol
The Records of the Primary Standard
The Calibration Records

Note: PerkinElmer will maintain possession of all documents; their reproduction may require a nondisclosure agreement to be provided by those requiring access to them.

The existence of these documents and the procedures used in their production are formal requirements of the PerkinElmer Quality System. The integrity of this PerkinElmer Quality System is routinely audited and is certified by the British Standards Institution as meeting all the requirements of ISO 9001, the internationally recognized standard for Quality Assurance.

This document shall not be reproduced except in full without the express written approval of the PerkinElmer UV Standards Certification Laboratory.



Quality Manager PKI RMCL
PerkinElmer Instruments
Shelton, CT. USA

PerkinElmer Inc., Shelton, CT 06484 USA An ISO 9001 Company





Certificate of Completion

This certifies that

Khwanchai Siangwong

Has successfully completed

AA PinAAcle 900 T, H, Z, F and 500

Completed on 4/7/2017 05:00 AM Eastern/New York

Certified By: Fred Rubino

Global Training Leader

Print Date May 19, 2017, 2:42 AM

This Certificate has been generated electronically from PerkinElmer Learning Management System, LMS ES-009-000, 0-05-55-11.



Certificate of Completion

This certifies that

Khwanchai Siangwong

Has successfully completed

FIAS 100 & 400 System

Completed on 8/17/2016 06:00 AM Eastern/New York

Certified By: Fred Rubino

Global Training Leader

Print Date Nov 17, 2016, 8:31 AM

This Certificate has been generated electronically from PerkinElmer Learning Management System, LMS ES-009-000, 0-05-55-11.

Agilent CrossLab Start Up Services

Agilent 5100 5110 ICP-OES Preventive Maintenance

Agilent Preventive Maintenance provides factory recommended service for your analytical instruments to assure reliable operation and the accuracy of your results

Delivered by highly trained and certified service engineers using genuine Agilent parts and supplies, Agilent Preventive Maintenance provides what you need to reduce unplanned downtime and keep your systems operating at their peak performance.

This checklist is used as a guide for completing the preventive maintenance tasks. A signed copy of this checklist is provided for your records.

Introduction

Customer Information

- Customers should provide all necessary operating supplies upon request of the engineer.
- A customer representative should be available to the engineer while performing the preventive maintenance procedures. Customers are responsible for regular maintenance and are encouraged to observe the service representative.
- Any parts not included in the Parts Lists section of this document are not part of the recommended Preventive Maintenance service nor are they included in the price of this service.
- If a system requires the use of extra or special procedures and/or parts for the maintenance service, then these must be ordered separately and charged as a repair, which may incur additional costs.
- For customers using HF applications, the instrument should be returned to its standard sample introduction system.

Important Customer Web Links

- To access **Agilent University**, visit <http://www.agilent.com/crosslab/university/> to learn about training options, which include online, classroom and onsite delivery. A training specialist can work directly with you to help determine your best options.
- To access the **Agilent Resource Center** web page, visit <https://www.agilent.com/en-us/agilentresources>. The following information topics are available:
 - Sample Prep and Containment
 - Chemical Standards
 - Analysis
 - Service and Support
 - Application Workflows
- The **Agilent Community** is an excellent place to get answers, collaborate with others about applications and Agilent products, and find in-depth documents and videos relevant to Agilent technologies. Visit <https://community.agilent.com/welcome>
- Videos about specific preparation requirements for your instrument can be found by searching the **Agilent YouTube** channel at <https://www.youtube.com/user/agilent>
- **Need to place a service call?** Flexible Repair Options | Agilent

Service Engineer's Responsibilities

- Contact the customer and ensure that all necessary supplies are available before the preventive maintenance visit.
- Only select those pages that relate to the system or module being serviced.
- Complete empty fields with the relevant information.
- Complete the relevant checkboxes in the checklist using either a "X" or tick mark "✓".
- Check "**Service not applicable**" check boxes to indicate services/tasks not delivered, as appropriate.
- Complete the Preventive Maintenance services in the most logical order relevant to the individual system service in the order of the tasks listed.
- Complete the **Service Review** section together with the customer.
- Complete the fields for page numbers at the foot of each selected page
- Add relevant page numbers to selected pages and complete the total number of pages field in the Service Completion section
- **Ask the customer to sign the Service Verification section including the customer's and your signature.**

Instrument Maintenance

System Information

- ☐ Check this box if an instrument configuration report is attached instead of completing the table.

Instrument System Name and ID
Instrument System Site and Location

5110 VDV ICP-OES

Envilab Company limited

List System Component Product Numbers	List the Serial Numbers of each Component
1. G 8015 A	MY 17490002
2. G 8410 A	AU17393768
3. G 8481-80002	1709-05327
4.	
5.	
6.	
7.	
8.	
9.	

ICP-OES Configuration Table	Circle the type or write in the type if other
Nebulizer Type	SeaSpray OneNeb Conikal Other
Spray Chamber	Cyclonic Single Pass Cyclonic Double Pass Other
Torch	Radial Dual View Other
Torch Type	One Piece Semi Demountable Fully Demountable Other
Injector Diameter	2.4mm 1.8mm 1.4mm 0.8mm Other
Injector Material	Quartz Ceramic Other

Preparation

- ☒ Discuss any specific issues with the customer before starting.
- ☒ Review the instrument logbook for recorded problems and comments.
- ☒ Save instrument control settings before starting the procedure.
- ☒ Perform a general inspection of the system for cleanliness.
- ☒ Check for proper installation of parts, assemblies, sensors etc.
- ☒ Check system for required installation of components and implementation of Service Notes
- ☒ Check for required firmware/software updates and verify with customers if they would like them installed.
- ☐ For HF application systems, if standard sample introduction system was not installed, ask the customer to install it. *N/A*
- ☒ Ask the customer to remove any samples from the ICP-OES sample introduction area, auto sampler or around the ICP-OES.

Preventive Maintenance Procedures

Record Pre-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table – Pre-PM.

Clean and inspect ICP-OES system

- ☒ Look for any obvious external damage or problems.
- ☒ Inspect water cooling hoses, gas lines and power cord for excessive wear or damage.
- ☒ Perform a general internal inspection of the system for excessive dust accumulation, clean if necessary.
- ☒ Inspect sample introduction components and record any required maintenance in the Service Engineer Comments and notify the customer as the required actions required.
- ☒ Record the instrument operating conditions in the ICP-OES Status Results Table.
- ☒ Replace the polychromator purge filter.
- ☒ Replace the radial pre-optics window
- ☒ Replace the axial pre-optics window for SVDV and VDV instruments.
- ☒ Check exhaust flow for the correct positive extraction at the exhaust duct to insure they meet minimum specifications.
- ☒ Replace air inlet dust filter.
- ☐ Replace high capacity air inlet dust filter element if installed. N/A
- ☒ Remove and clean instrument water inlet filter.

Agilent Water Recirculator

- ☐ **Service not applicable**
- ☒ Drain cooling fluid and remove any particles from the chiller reservoir
- ☒ Remove, clean and reinstall water inlet metal mesh filter if present.
- ☒ Re fill with Agilent Cool Clear cooling fluid.
- ☒ Clean the cooling system Air filter and the condenser.

SPS 3 Auto Sampler


- ☒ **Service not applicable**
- ☐ Power cycle the autosampler and verify successful initialization.
- ☐ Inspect X and Z axis belts for wear. Replace is necessary.
- ☐ Clean X and Z axis slide shafts.
- ☐ Using customer's racks and the Agilent software move the sample probe to the 4 outermost corners and rinse port, ensure that the probe is approximately centered in the vial.

SPS 4 Auto sampler

- ☐ **Service not applicable**
- ☒ Clean the spill tray, rack location mat, end frames and chassis with a damp soft cloth and diluted mild detergent.
- ☒ Clean the auto sampler cover panels, if cover kit is installed, with domestic window cleaner.
- ☒ Check the X-axis and Z-axis drive belts for cracks, splits, damaged teeth, excessive fraying, color changes or degradation from fumes.
- ☒ Check the X-axis, Theta-axis and Z-axis FFC cables for cracks, incorrect positioning, damaged edges or damaged connectors.
- ☒ Pump Tubing Replacement. Replace peristaltic pump tubing. Replace all tubing that goes from the rinse station to the pump and from the pump to the waste/rinse bottles *only checked; passed*
- ☒ Test using customer's tray and move the sample probe to the sample vial 1, wash vial and rinse port and ensure that the probe is centered in the vial. If not use calibration wizard and calibrate the position.

AVS 4, 6, 7 Advanced Valve System

- ☒ **Service not applicable**
- ☐ Replace valve rotor seal
- ☐ Check fittings for signs of leaks
- ☐ Check tubing including autosampler tubing for kinks or excessive wear
- ☐ Check high flow pump for signs of leaks



ICP-OES adjustment

- ☒ Check position of Zn peak, adjust if required.
- ☒ Check Argon Ratio, adjust to specified value if required.
- ☒ Perform Detector Calibration.
- ☒ Perform Instrument Calibration.

Record Post-PM instrument performance

- ☒ Run Instrument Performance test.
- ☒ Record results in Instrument Performance Test Results Table - Post PM.
- ☒ For systems using ICP Expert version 7.3 and above, run the following Instrument tests
 - ☒ Subsystem Communications Test
 - ☒ Air Flow
 - ☒ Water Flow
 - ☒ Gas Flows
 - ☒ RF Generator
 - ☒ Camera Test
 - ☒ Optics Test
 - ☒ Nebulizer Test
- ☒ Record the result in the Instrument Test Results Table

Restore Instrument

- ☐ For HF applications, ask the customer to reinstall their sample introduction system. N10
- ☒ Leave system in an idle state: on and purging.
- ☒ Guidance: If the PM service is performed prior to a qualification service, then use the qualification procedure as a guide for final instrument set up and checkout.

Service Review

- ☒ Attach available reports/printouts of all tests to this documentation.
- ☒ Record the Preventive Maintenance service activity in the customer's records/logbook.
- ☒ Record the PM event in the Smart Alerts logbook, if applicable.
- ☒ Update/reset instrument maintenance counters as appropriate.
- ☒ Affix the PM sticker to the system or instrument logbook based on the customer's request.
- ☒ Complete the Service Engineer Comments section if there are additional comments.
- ☒ Review this service, parts replaced, and test results obtained with the customer.
- ☒ If the instrument firmware was updated, record the details of the change in the Service Engineer's Comments box. Systems in a compliant environment may need additional documentation.
- ☒ **Complete the Signature Page with both Service Engineer and Customer signatures.**

Test Results

Instrument Performance Test Results Table

Note: These measurements do not form part of any specification and are for reference only.

	Pre PM Sensitivity Check		Post PM Sensitivity Check	
	Radial	Axial *	Radial	Axial*
Zn 213.857 nm SRBR	1597.1	3382.6	2348.2	6129.9
Mn 257.610 nm SRBR	5945.3	16145.3	10768.1	39073.2
Al 396.152 nm SBR	7.0	16.3	8.5	25.7
K 766.491 nm SBR	6.2	67.3	4.7	83.6

* Axial result is not applicable for G8016AA, G8012AA Radial View instruments.

Instrument Test Results Table

Note: The Instrument Test results are for systems using ICP Expert version 7.3 and above only.

Instrument Test	Result
Subsystem Communications Test	Pass
Air Flow	Pass
Water Flow	Pass
Gas Flows	Pass
RF Generator	Pass
Camera Test	Pass
Optics Test	Pass
Nebulizer test	Pass

ICP-OES Status Results Table

Note: These measurements do not form part of any specification and are for reference only.

Measurement	Standby Mode		Plasma On	
Mains Voltage	219.371	VAC	217.484	VAC
Mains Current	0.082	A	0.098	A
Instrument Temperature	23.5	°C	23.1	°C
RF Air Flow (sensor speed)	13.0	Hz	19.0	Hz
Plasma Exhaust Temperature	No measurement		56.4	°C
Water Flow Oscillator	No measurement		1.51	L/min
Water Flow Detector	1.09	L/min	1.06	L/min
Water Inlet Temperature	16.9	°C	16.7	°C
Polychromator Temperature	35.0	°C	35.0	°C
CCD Temperature	-39.6	°C	-39.4	°C
Thermal Stabilizer	35.0	°C	35.0	°C
Argon Supply Pressure	619.13	kPa	560.32	kPa
Purge Gas Supply Pressure*1	616.63	kPa	597.43	kPa
Option Gas Supply Pressure*1	-	kPa	-	kPa
Nebulizer Flow	No measurement		0.70	L/min
Nebulizer Back Pressure	No measurement		283.17	kPa
Plasma Gas Flow	No measurement		11.98	L/min
Auxiliary Gas Flow	No measurement		1.00	L/min
RF Power	No measurement		1195.1	W
RF Supply Current	No measurement		8.190	A
RF Supply Voltage	No measurement		194.557	V

*1 If option installed

Consumed PM Parts

Part Description	Part Number	Product or Model# where used	Quantity consumed
Axial Pre-Optic Window	G8010-68014	G8010A, G8011A, G8014A/G8015A	1
Radial Pre-Optic Window	G8010-68015	All	1
Agilent Cool Clear Coolant Fluid	5799-0037	Agilent Water Recirculator	—
Purge Gas Filter	G8010-60136	All	1
Air inlet filter	G8000-68002	All	1
High Capacity Air Filter	G8010-60189	Optional	—
Rotor seal for 6-7 port valve for AVS6/7	G8494-60002	G8494A/G8495	—
Rotor seal for 4 port valve for AVS4	G8493-60002	G8493A	—
Rinse solution to rinse station 2.5mm id x 1m	G8410-80123	SPS 4	—
Barb connector 2.5mm-1.5mm ID	G8410-80124	SPS 4	—
PVC waste tubing, 8mm od x 5mm id, 2m	G8410-80122	SPS 4	—
Additional Parts may be required from engineer's stock:			
X axis drive belt	5410047500	SPS 3	—
Z axis drive belt	5410047400	SPS 3	—
Peristaltic pump tubing, PVC SolvaFlex, 3 bridged,	3710049000	SPS 4	—

Consumed Parts Reference
(Purchased by customer, not included as part of PM)☐ Section Not Applicable.

Part Description	Part Number	Product or Model# where used	Quantity consumed
------------------	-------------	------------------------------	-------------------

Signature Page

Service Engineer Comments (optional)

If there are any specific points you wish to note as part of performing the installation or other items of interest for the customer, please write in this box.

Service Verification

Service Request Number:

6006121636

Service Engineer Name:

Kanyakorn S.

Service Engineer Signature:

Kanyakorn S.

Total number of pages in this document:

14

Date Service Completed:

31 May 2023

Customer Name:

บริษัท

Customer Signature:

บริษัท

Report Summary

Instrument Model Agilent 5100/5110 VDV ICP-OES
Instrument ID G8011A/G8015A
Instrument Serial Number MY17490002
Software Version 7.4.0.10280
Firmware Version 3562
Tested By Kanyakorn S.
Test Started On 5/31/2023 12:22:01 PM
Test Completed On 5/31/2023 12:26:21 PM

Result Summary

Subsystem Communications Test Pass
Air Flow Test Skipped
Water Flow Test Skipped
Gas Flows Test Skipped
RF Generator Test Skipped
Camera Test Skipped
Optics Test Pass
Advanced Valve System Test Skipped
Resolution Test Pass
Sensitivity Test Pass
Precision Test Pass

Subsystem Communications Test Pass

Optics Test Pass

	Radial	Axial
Intensity	3397602	2923418
Wavelength	737.212	737.212

Resolution Test**Pass**

Element Wavelength	Specification	Width
N (174.213 nm)	≤ 9.40	6.72
As (188.980 nm)	≤ 8.20	6.49
C (193.027 nm)	≤ 11.50	8.01
Mo (202.032 nm)	≤ 8.20	6.43
Cr (206.158 nm)	≤ 13.40	8.50
Zn (213.857 nm)	≤ 8.70	7.16
Pb (220.353 nm)	≤ 9.50	7.51
Co (228.615 nm)	≤ 17.20	11.32
Ba (230.424 nm)	≤ 9.40	7.80
Mn (257.610 nm)	≤ 13.30	9.78
Mn (260.568 nm)	≤ 20.30	13.88
Cr (267.716 nm)	≤ 11.00	9.09
Cu (324.754 nm)	≤ 25.00	18.88
Cu (327.395 nm)	≤ 14.20	12.41
Sr (338.071 nm)	≤ 33.50	24.27
Ba (455.403 nm)	≤ 44.00	34.07
Sr (460.733 nm)	≤ 36.00	22.56
Ba (493.408 nm)	≤ 36.00	27.79
Ba (614.171 nm)	≤ 42.00	27.97
Ar (675.283 nm)	≤ 74.00	62.41
K (766.491 nm)	≤ 80.00	65.95

Sensitivity Test**Pass****Radial**

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 46.0	SRBR	108.0	934.0	64.8
Se (196.026 nm)	≥ 41.0	SRBR	110.2	1159.4	93.6
Zn (213.857 nm)	≥ 1421.0	SRBR	2348.2	23561.0	99.8
Pb (220.353 nm)	≥ 46.0	SRBR	98.7	1075.1	98.0
Mn (257.610 nm)	≥ 3518.0	SRBR	10768.1	218704.5	411.0
Al (396.152 nm)	≥ 3.4	SBR	8.5	40909.0	4325.8
Ba (493.408 nm)	≥ 34.0	SBR	111.9	1396218.4	12367.4
K (766.491 nm)	≥ 1.8	SBR	4.7	108989.7	19076.8

Axial

Element Wavelength	Specification	Method	Ratio	Standard	Blank
As (188.980 nm)	≥ 208.0	SRBR	267.6	3134.3	126.3
Se (196.026 nm)	≥ 159.0	SRBR	284.6	4158.5	194.0
Zn (206.200 nm)	≥ 234.0	SRBR	495.4	1165.9	5.5
Zn (213.857 nm)	≥ 1743.0	SRBR	6129.9	92298.3	225.6
Cd (214.439 nm)	≥ 4227.0	SRBR	16998.9	48382.7	8.1
Pb (220.353 nm)	≥ 320.0	SRBR	416.4	6520.1	228.4
Mn (257.610 nm)	≥ 10625.0	SRBR	39073.2	1331904.8	1159.9
Cr (267.716 nm)	≥ 1048.0	SRBR	5986.5	203686.5	1144.7
Cu (324.754 nm)	≥ 19.0	SBR	77.1	389900.7	4991.6
Al (396.152 nm)	≥ 6.0	SBR	25.7	268775.7	10073.7
Ba (493.408 nm)	≥ 60.0	SBR	293.9	8244793.3	27957.8
K (766.491 nm)	≥ 24.0	SBR	83.6	3030541.1	35817.8

Radial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 2.60	0.75
Se (196.026 nm)	≤ 2.60	0.69
Zn (213.857 nm)	≤ 1.50	0.27
Pb (220.353 nm)	≤ 2.60	1.06
Mn (257.610 nm)	≤ 1.50	0.30
Al (396.152 nm)	≤ 1.50	0.27
Ba (493.408 nm)	≤ 1.50	0.99
K (766.491 nm)	≤ 1.50	0.25

Axial

Element Wavelength	Specification	Measured Value % RSD
As (188.980 nm)	≤ 1.50	0.54
Se (196.026 nm)	≤ 1.50	0.48
Zn (206.200 nm)	≤ 1.50	1.06
Zn (213.857 nm)	≤ 1.50	0.48
Cd (214.439 nm)	≤ 1.50	0.33
Pb (220.353 nm)	≤ 1.50	0.37
Mn (257.610 nm)	≤ 1.50	0.77
Cr (267.716 nm)	≤ 1.50	0.62
Cu (324.754 nm)	≤ 1.50	0.45
Al (396.152 nm)	≤ 1.50	0.45
Ba (493.408 nm)	≤ 1.50	0.80
K (766.491 nm)	≤ 1.50	0.91

Report Summary

Instrument Model Agilent 5100/5110 VDV ICP-OES
Instrument ID G8011A/G8015A
Instrument Serial Number MY17490002
Software Version 7.4.0.10280
Firmware Version 3562
Tested By Kanyakorn S.
Test Started On 5/31/2023 12:34:17 PM
Test Completed On 5/31/2023 12:46:55 PM

Result Summary

Subsystem Communications Test Pass
Air Flow Test Pass
Water Flow Test Pass
Gas Flows Test Pass
RF Generator Test Pass
Camera Test Pass
Optics Test Skipped
Advanced Valve System Test Skipped
Resolution Test Skipped
Sensitivity Test Skipped
Precision Test Skipped

Subsystem Communications Test Pass

Air Flow Test Pass

30% Air Flow (relative speed)	75% Air Flow (relative speed)
12.00	18.00

Water Flow Test Pass

RF Water Flow(L/min)	Camera Water Flow (L/min)	Water Inlet Temperature (°C)
1.45	1.06	16.78

Gas Flows Test**Pass**

Nebulizer Target Flow	Actual Flow	Back Pressure
0.70	0.71	280.77

Auxiliary Target Flow	Actual Flow	Back Pressure
2.00	2.00	93.84

Makeup Target Flow	Actual Flow	Back Pressure
2.00	1.99	95.26

Plasma Target Flow	Actual Flow	Back Pressure
18.00	17.94	23.27

RF Generator Test**Pass**

RF Power Supply Test	Passed
RF Power Supply (V)	147.418

RF Oscillator Test	Passed
RF Oscillator Frequency (MHz)	25.961
Work Coil Current (A)	45.326
RF Power Supply Current (A)	2.000

Camera Test**Pass**

	Integration Time (ms)	Standard Deviation	Status
Electronic Offset Test	1000	5.120	Passed
Array Test	5	0.015	Passed
Linearity Test		0.122	Passed