

ภาคผนวก จ

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Songkhla Lab	BOD	Incubator	SGK_CL0028	13-Jul-23	13-Jan-25	18
Songkhla Lab	BOD	DO/BOD Analyser	SGK_CL0073	21-May-24	21-Nov-25	18
Songkhla Lab	COD	COD Reactor	SGK_CL0085	24-Jan-24	24-Jan-25	12
Songkhla Lab	COD	Spectrophotometer	SGK_CL0038	24-Jan-24	24-Jan-25	12
Songkhla Lab	pH at 25 °C	pH meter	SGK_CL0030	19-Oct-24	19-Apr-26	18
Songkhla Lab	Oil & Grease	Electronic Top-Loading Balance	SGK_CL0045	15-Jan-24	15-Jan-25	12
Songkhla Lab	Oil & Grease	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Songkhla Lab	Oil & Grease	Water Bath	SGK_CL0035	13-Jul-23	13-Jan-25	18
Songkhla Lab	Total Dissolved Solids 180°C	Electronic Top-Loading Balance	SGK_CL0045	15-Jan-24	15-Jan-25	12
Songkhla Lab	Total Dissolved Solids 180°C	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Songkhla Lab	Total Suspended Solids	Electronic Top-Loading Balance	SGK_CL0045	15-Jan-24	15-Jan-25	12
Songkhla Lab	Total Suspended Solids	Oven	SGK_CL0024	19-Oct-24	19-Apr-26	18
Ambient	Benzene	GC-MSD	RYG_EN0136	5-Jan-24	4-Jul-25	18
Ambient	Total Hydrocarbon	Total Hydrocarbon Analyzer	BKK_FS1068	11-Dec-23	11-Jun-25	18



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 16-Jul-2023

Certificate No. : 23TH3096

CSR No. : A095/04743

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory
Instrument Name : Incubator
Manufacturer : Memmert
Model : ICP750
Serial No. : F816.0063
ID No. : SGK_CL0028
Resolution : 0.1 °C
Received Date : 13-Jul-2023
Calibrated Date : 13-Jul-2023
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BY

APPROVED BY

NEXT CAL. DATE 13/01/25

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- ScaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanayam Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	23SDAT004	23-May-2024


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (☒) Without Adjustment (☐) After Adjustment

1. Sensor Installation Diagram

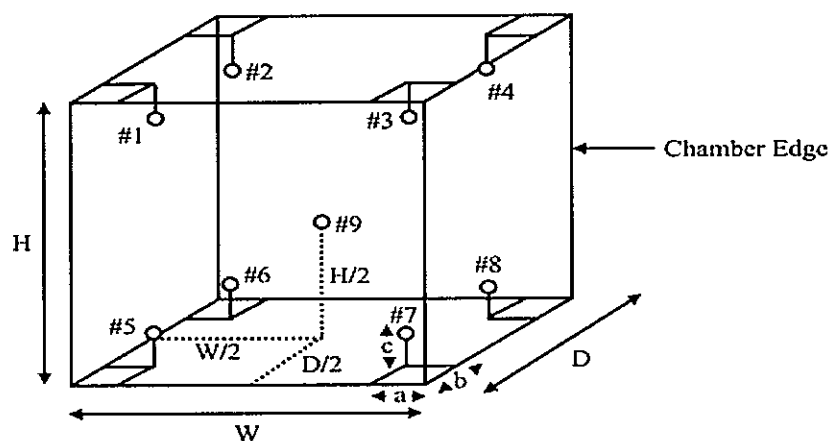

Sensor Installation Details

a = 5.0 cm
b = 5.0 cm
c = 5.0 cm

Dimension of the chamber

W = 40.0 cm
H = 40.0 cm
D = 33.0 cm



Certificate No. : 23TH3096

CSR No. : A095/04743

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Incubator and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (± °C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
20	20.10	20.04	20.03	19.97	20.08	20.23	20.10	19.94	20.07	0.38

3. Performance Result

The performance of the Incubator are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
20	20.0	20.0	0.14	0.17	0.32

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES


534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000 FAX. 0-2719-9484

Certificate of Testing

Cert.No.: 24TW96

Page.: 1 of 2

Equipment :	DO Meter
Manufacturer :	YSI
Model :	5000
Serial No. :	17B101473
ID No. :	SGK_CL0073
Received Date :	17 May 2024
Test Date :	21 May 2024
Reference :	2405-0608DSC-1
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch. 114/1 Moo 8 Karnchanawanich Rd., T.Ban Phru, A.Hat Yai, Songkhla 90250 Thailand
Laboratory Condition :	Temperature (25 ± 5) °C Humidity (50 ± 20) %
Test Procedure :	In - house method : CP-CH9 by Comparison Technique with Azide Modification Method
Tested by :	Walalak Sirithean
Approved by :	 Approved Signatory
() Unnopphol Harachai () Ponpan Paipim (✓) Saithip Meangmai	

Issue Date : 21 May 2024

REVIEW BY

APPROVED BY..

NEXT CAL DATE..... 21/11/25



Cert.No.: 24TW96

Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :

This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

<u>Instruments</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1. Burette	-	130BU10	23CG1172	22 Mar 2025
2. Balance	14233821	110RC001	23MM405	16 July 2024

2. Standard Material :-

<u>Material</u>	<u>Manufacturer</u>	<u>Lot.No.</u>	<u>Assay</u>
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : **Dissolved Oxygen Meter Adjustment With Air 100 %**

Dissolved Oxygen Probe No.: 17B100103

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.18	0.0071

This report was certified only for the instrument we tested. It is allowable to use for study. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL.0-2717-3000-29 FAX.0-2719-9484



Certificate of Calibration

Cert. No.: 24LM77

Page.: 1 of 2

Equipment : DO Meter with Sensor

Manufacturer : YSI

Model : 5000-115

Serial No. : 17B101473

ID No. : SGK_CL0073

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
Songkhla Branch.
114/1 Moo 8 Karnchanawanich Rd.,
T.Ban Phru, A.Hat Yai,
Songkhla 90250 Thailand

Location : TPA On Site Calibration Laboratory


Received Order : 17 May 2024


Calibrated Date : 27 May 2024

Ambient Temperature : (26 ± 10) °C

Relative Humidity : (50 ± 30) %

AC Line Voltage : (220 ± 22) V

Calibrated by : Khit Ruttanaprapachai


Approved by : 
Approved Signatory

() Ponpan Paipim
() Suwit Imjai
(✓) Kunchit Promprat

Issue Date : 28 May 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2405-0608DSC-2

Cert. No.: 24LM77

Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Digital Thermometer	2188080	231216	TPA	11 Oct 2024
2. This certificate is valid only to the item calibrated on date and place of calibration.				
3. This certification is traceable to the International System of Unit.				

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 17B100103

<u>Calibration Point</u> (°C)	<u>Immersion Depth</u> (mm)	<u>Standard Temperature</u> (°C)	<u>UUC* Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (± °C)	<u>Coverage Factor</u> <i>k</i>
20.00	60	20.005	19.79	-0.215	0.15	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3 : EQUIPMENT CALIBRATION AND TESTING SERVICES

534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250

TEL. 0-2717-3000-29 FAX. 0-2719-9484

Cert. No.: 24TM152

Page.: 1 of 3

Certificate of Calibration

Equipment : COD Reactor
Manufacturer : Hach
Model : DRB200
Serial No. : 21120C1313
ID No. : SGK_CL0085
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd.
(Songkhla Branch)
114/1 Moo 8 Kanjanavanij Rd., Banphru,
Hatyai, Songkhla 90250 Thailand

Location : Chemistry Room
Received Order : 24 January 2024
Calibration Date : 24 - 25 January 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BY ..	[REDACTED]
APPROVED BY ..	[REDACTED]
NEXT CAL. DATE	24/01/25

Calibrated by : Kunchit Promprat

Approved by :

Approved Signatory

- () Pornthippa Tameyakul
() Ponpan Paipim
(✓) Suwit Imjai

Issue Date : 29 January 2024

The Uncertainties are for a confidence probability of approximately 95%.

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Calibration and Testing Equipment Services.

A 0012840



Equipment : COD Reactor
 Condition As-Received : Used Item
 Reference : 2401-0645OC-3
 Procedure Used :-

Cert. No.: 24TM152
 Page.: 2 of 3

As agreed with customer the calibration was perform using in-house calibration method according to directed measurement method with Data Acquisition which connected with Thermocouple Type T.

The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1) Data Acquisition	MY44073381	23LM95	TPA	19 Jun 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.



Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function of UUC* : Temperature Source

Heat transfer medium used : Alumina Calcined

Environment during calibration		
	Beginning	Finished
Temp.(°C)	26	27
REL.Humi.(%)	54	61
AC Supply (Volt)	226	227

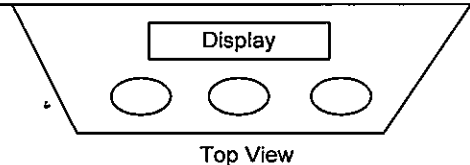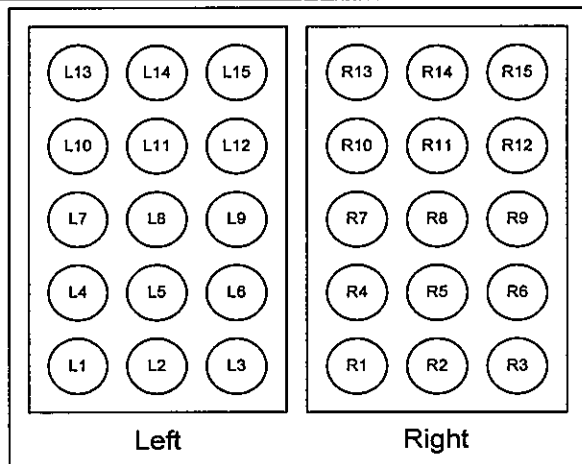

Left		Right	
Position	ID No. of Sensor	Position	ID No. of Sensor
L1	23-01TC-01	R1	23-01TC-01
L2	23-01TC-02	R2	23-01TC-02
L3	23-01TC-03	R3	23-01TC-03
L4	23-01TC-04	R4	23-01TC-04
L5	23-01TC-05	R5	23-01TC-05
L6	23-01TC-06	R6	23-01TC-06
L7	23-01TC-07	R7	23-01TC-07
L8	23-01TC-08	R8	23-01TC-08
L9	23-01TC-09	R9	23-01TC-09
L10	23-01TC-10	R10	23-01TC-10
L11	23-01TC-01	R11	23-01TC-01
L12	23-01TC-02	R12	23-01TC-02
L13	23-01TC-03	R13	23-01TC-03
L14	23-01TC-04	R14	23-01TC-04
L15	23-01TC-05	R15	23-01TC-05



Equipment : COD Reactor
Condition As-Received : Used Item
Reference : 2401-0645OC-3
Result of Calibration :- (*) Without Adjustment
Function of UUC* : Temperature Source
Calibration Point : 150 °C

Cert. No.: 24TM152

Page.: 3 of 3

UUC* Setting (°C)	UUC* Reading (°C)	Measured Temperature (°C)						Temperature stability (± °C)	Uncertainty (± °C)	Coverage Factor <i>k</i>
		Position								
		Left			Right					
150	150	L13	L14	L15	R13	R14	R15	0.12	1.1	2
		148.341	148.341	148.230	148.998	149.015	149.078			
		L10	L11	L12	R10	R11	R12			
		149.185	148.528	148.840	149.456	148.501	148.504			
		L7	L8	L9	R7	R8	R9			
151	151	149.460	149.692	150.210	149.845	150.020	150.266	0.10		
		L4	L5	L6	R4	R5	R6			
		149.759	149.784	149.899	150.332	149.962	150.233			
		L1	L2	L3	R1	R2	R3			
		149.241	149.588	149.525	149.776	149.847	149.313			

Average* : The average of 30 values in each position.

Temperature stability : One-half of the greatest maximum difference of measured temperature at any one sensor.

UUC* : Unit Under Calibration

Note : The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



a 1199639



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 24CHO44

Page.: 1 of 3

Certificate of Calibration

Equipment : Spectrophotometer
Manufacturer : Hach
Model : DR 3900
Serial No. : 1687645
ID No. : SGK_CL0038
Condition As-Received: Used Item
Received Date : 24 January 2024
Calibration Date : 24 January 2024
Reference : 2401-0645OC-2
Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. Songkhla Branch.
114/1 Moo 8 , Kanjanavanij Rd.,
Banphru , Hatyai ,
Songkhla 90250 , Thailand

REVIEW BY	[Redacted]
APPROVED BY	[Redacted]
NEXT CAL. DATE	24/01/25

Calibration Place : Chemistry Room
Ambient Temperature : (26.4 - 25.6) °C (On-Site)
Relative Humidity : (61.5 - 64.1) % (On-Site)
Calibration Procedure : In - house method :
CP-OCH4 based on ASTM E 275-01

Calibrated by : Kunchit Promprat



Approved by :

Approved Signatory

- () Saithip Meangmai
() Warakorn Lerngagtrakul
(☒) Ponpan Paipim

Issue Date : 29 January 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

A 0062930



Cert. No. : 24CHO44

Page : 2 of 3

Condition of calibration result

1. Reference Standard Material :

<u>Material</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due date</u>
1. Absorbance Standard set	8331	105939	28 Sep 2024
2. Wavelength Standard set	29829	114509	11 Sep 2025
3. Wavelength Standard set	29829	114510	11 Sep 2025

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certificate is traceable to the International System of Unit maintained through :


- Starna Scientific Ltd.

4. Spectral BandWidth : 5 nm
Scan Speed : - nm/min

Calibration Results : without adjustment

Wavelength Accuracy

Certified Values of Reference Material (nm)	UUC Reading (nm)	Uncertainty of Measurement (\pm nm)	Coverage Factor <i>k</i>
418.40	418	0.59	2.00
479.88	480	0.59	2.00
513.75	514	0.59	2.00
537.00	537	0.59	2.00
638.00	638	0.59	2.00
684.70	685	0.59	2.00
747.61	748	0.59	2.00
807.04	807	0.59	2.00



a 1199642



Cert. No. : 24CHO44

Page : 3 of 3

Calibration Results : without adjustment

Photometric Accuracy

Wavelength (nm)	Certified Values of Reference Material (Abs)	UUC Reading (Abs)	Uncertainty of Measurement (\pm Abs)	Coverage Factor <i>k</i>
420.0	Zero	0.000	0.0028	2.00
	0.5712	0.572	0.0031	2.00
	0.7510	0.752	0.0032	2.00
	1.0893	1.092	0.0033	2.00
440.0	Zero	0.000	0.0028	2.00
	0.5607	0.560	0.0030	2.00
	0.7336	0.733	0.0030	2.00
	1.0636	1.063	0.0031	2.00
465.0	Zero	0.000	0.0028	2.00
	0.5111	0.514	0.0030	2.00
	0.6768	0.679	0.0029	2.00
	0.9802	0.985	0.0029	2.00
546.1	Zero	0.000	0.0028	2.00
	0.5224	0.522	0.0028	2.00
	0.6856	0.684	0.0029	2.00
	0.9937	0.993	0.0028	2.00
590.0	Zero	0.000	0.0028	2.00
	0.5542	0.551	0.0028	2.00
	0.7155	0.712	0.0028	2.00
	1.0366	1.033	0.0028	2.00
635.0	Zero	0.000	0.0028	2.00
	0.5397	0.538	0.0028	2.00
	0.6832	0.680	0.0029	2.00
	0.9886	0.986	0.0028	2.00

Remark *

- Each individual filter is measured against the empty filter holder (blank) used to zero the spectrophotometer

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-



a 1199641



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 22-Oct-2024

Certificate No. : 24CH0526

CSR No. : A163/08133

Page. : 1 of 2

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : pH meter

Manufacturer : Mettler Toledo

Model : S220

Serial No. : B625631849

ID No. : SGK_CL0030

Electrode No. : 2281592

Received Date : 19-Oct-2024

Calibrated Date : 19-Oct-2024

Ambient Temperature : $(25 \pm 3) ^\circ\text{C}$

Relative Humidity : $(55 \pm 15) \%$

REVIEW BY Ananta B.
APPROVED BY Kanitta H.
NEXT CAL. DATE 19/4/26

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.008 based on direct measurement by using certified reference Material (CRM)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- CPAchem : CPAchem Ltd
- WK : WK Electric Co., Ltd.
- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Alisara Ma

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Solution	4.000	61310674	1042701	26-Oct-2025
Standard Solution	7.000	61314184	1042700	26-Oct-2025
Standard Solution	10.01	61313804	1042702	26-Oct-2025
Temperature/Electrical Calibrator	MC2-TE	14987	WK2106-299-223	31-May-2025
Digital Thermometer With Sensor	DP-77	1.360896	24SDTH005	7-Aug-2025

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration :

1. Electrical Measurement

Applied Voltage (mV)	pH meter Reading		Correction (mV)	Uncertainty (± mV)
	(mV)	(pH)		
177.48	177.5	4.00	-0.02	0.17
0.00	0.0	7.00	0.00	0.13
-177.48	-177.5	10.00	0.02	0.17

2. Before Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.007	3.99	178.1	0.017	0.0092
6.976	7.02	1.7	-0.044	0.019
10.009	9.96	-169.6	0.049	0.038

3. After Sample Test Measurement

Standard Buffer Solutions (pH)	pH meter Reading		Correction (pH)	Uncertainty (± pH)
	(pH)	(mV)		
4.007	3.99	177.7	0.017	0.0092
6.976	7.01	3.7	-0.034	0.019
10.009	10.00	-169.0	0.009	0.038

4. Temperature Measurement

Cal Point (°C)	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
25	25.021	25.0	0.02	0.060

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...

Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 18-Jan-2024

Certificate No. : 24MA0199

CSR No. : A123/06123

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory
Instrument Name : Electronic Balance
Manufacturer : Sartorius
Model : MSE224S-100-DU
Serial No. : 34705158
ID No. : SGK_CL0045
Resolution : 0.0001 g
Received Date : 15-Jan-2024
Calibrated Date : 15-Jan-2024
Ambient Temperature : $(30 \pm 10) ^\circ\text{C}$
Relative Humidity : $(50 \pm 20) \%$

REVIEW BY ...
APPROVED BY ...
NEXT CAL. DATE 15/1/25

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.001 based on UKAS LAB 14 : 2015

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Hadbordee Dettawee

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.



Certificate No. : 24MA0199

CSR No. : A123/06123

Page. : 2 of 3

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Standard Weight Set	2 mg - 1 kg	11119514/01	23SWS001	4-Jul-2024

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration : (✓) Without Adjustment () After Adjustment

1. Repeatability

Nominal Value (g)	Standard Deviation (g)
20	0.00000
200	0.00000

2. Effect of tare

Nominal Value (g)	Standard Value (g)	Balance Reading (g)	Correction (g)
20	20.0000	20.0000	0.0000
40	40.0001	40.0000	0.0001
60	60.0000	60.0001	-0.0001
80	80.0001	80.0001	-0.0001
100	100.0000	100.0000	0.0000




Result of Calibration :

3. Off-centre loading

A mass approximately 100g was placed on a pan and moved to various position .

The balance reading obtained are given in the table.

Position					Maximum Difference (g)
1	2	3	4	5	
100.0000	100.0001	100.0000	100.0000	100.0000	0.0001



4. Departure from nominal value

Nominal Value (g)	Standard Value (g)	UUC Reading (g)	Correction (g)	Uncertainty (\pm g)	Coverage Factor (k)
0	0.0000	0.0000	0.0000	0.00008	2.0
0.01	0.0100	0.0100	0.0000	0.00008	2.0
0.1	0.1000	0.1000	0.0000	0.00008	2.0
0.5	0.5000	0.5000	0.0000	0.00008	2.0
1	1.0000	1.0000	0.0000	0.00008	2.0
2	2.0000	2.0000	0.0000	0.00008	2.0
5	5.0000	5.0000	0.0000	0.00009	2.0
10	10.0000	10.0000	0.0000	0.00009	2.0
20	20.0000	20.0000	0.0000	0.00009	2.0
50	50.0000	50.0000	0.0000	0.00011	2.0
100	100.0000	100.0000	0.0000	0.00016	2.0
120	120.0000	120.0000	0.0000	0.00024	2.0
140	140.0001	140.0000	0.0001	0.00024	2.0
160	160.0000	160.0000	0.0000	0.00026	2.0
180	180.0000	180.0000	0.0000	0.00029	2.0
200	200.0000	200.0000	0.0000	0.00030	2.0

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95%

...End...



CALIBRATION CERTIFICATE

Issued Date : 22-Oct-2024

Certificate No. : 24TH4295

CSR No. : A163/08133

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory
Instrument Name : Hot Air Oven
Manufacturer : Memmert
Model : UF110
Serial No. : B416.3387
ID No. : SGK_CL0024
Resolution : 0.1 °C
Received Date : 19-Oct-2024
Calibrated Date : 19-Oct-2024
Ambient Temperature : (30 ± 10) °C
Relative Humidity : (50 ± 30) %

REVIEW BY	
APPROVED BY	
NEXT CAL. DATE	19/04/2026

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.012 based on GLA - 20

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement according to the International System of Unit (SI) through :

- TISTR : Thailand Institute of Scientific and Technological Research

Calibrated by : Ibrrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager



The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	PSL-T0707-1/67	22-May-2025


2. The results reported in this certificate refer to the condition of the instrument on the date of calibration and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction

4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration .: (✓) Without Adjustment () After Adjustment

1. Sensor Installation Diagram

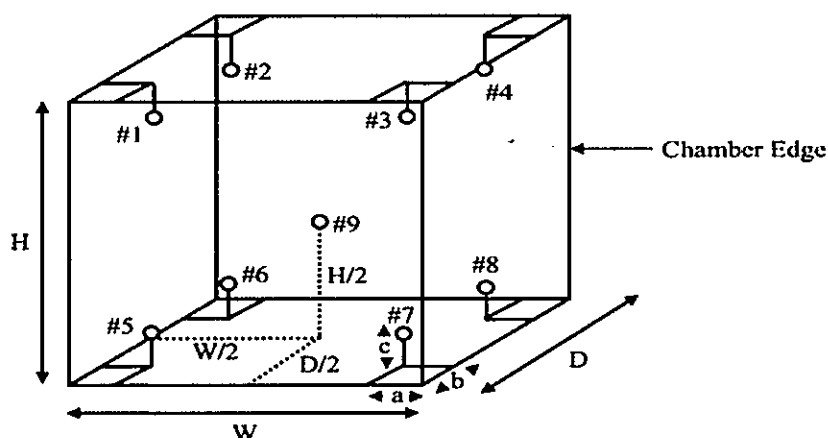

Sensor Installation Details

a = 5.0 cm
 b = 5.0 cm
 c = 5.0 cm

Dimension of the chamber

W = 55.0 cm
 H = 48.0 cm
 D = 40.0 cm

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Hot Air Oven and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)									Uncertainty (±°C)
	#1	#2	#3	#4	#5	#6	#7	#8	Ref. 9	
40	40.36	40.40	40.51	40.43	40.05	40.24	40.09	40.14	39.75	0.38
70	70.27	70.30	70.45	70.24	70.24	70.43	70.29	70.30	69.95	0.36
103	102.94	102.90	103.55	102.96	103.22	103.14	103.10	103.01	102.88	0.36
104	104.15	103.99	104.27	104.06	104.09	104.23	104.26	104.15	103.90	0.36
105	105.04	104.90	105.05	104.87	104.91	104.80	104.82	104.98	104.70	0.36
180	179.19	178.93	179.82	179.10	179.27	179.68	179.12	179.73	179.12	0.41

3. Performance Result

The performance of the Hot Air Oven are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (±°C)	Temperature Uniformity (°C)	Overall Variation (°C)
40	40.0	40.0	0.20	0.84	0.84
70	70.0	70.0	0.10	0.59	0.59
103	103.0	103.0	0.20	0.73	0.74
104	104.0	104.0	0.20	0.47	0.56
105	105.0	105.0	0.20	0.44	0.46
180	180.0	180.0	0.50	0.86	1.11

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%

... End ...



Southern Calibration Service Co., Ltd.

669/35 Karnjanavanit Rd., Banpru, Hatyai, Songkla 90250 Thailand
Tel : 08 1599 0417 Fax : 0 7480 5133 Email : s.calibration@gmail.com www.scal-lab.com



CALIBRATION CERTIFICATE

Issued Date : 16-Jul-2023

Certificate No. : 23TH3097

CSR No. : A095/04743

Page. : 1 of 3

Customer : ALS Laboratory Group (Thailand) Co., Ltd
114/1 Moo 8, Karnchanawanich Rd. Tambon, Ban Phru,
Amphoe Hat Yai, Songkhla, 90250

Calibration Place : Chemical Laboratory

Instrument Name : Water Bath

Manufacturer : Memmert

Model : WNE29

Serial No. : L616.0538

ID No. : SGK_CL0035

Resolution : 0.1 °C

Received Date : 13-Jul-2023

Calibrated Date : 13-Jul-2023

Ambient Temperature : (30 ± 10) °C

Relative Humidity : (50 ± 30) %

REVIEW BY ...

APPROVED BY

NEXT CAL. DATE 13/01/25

Calibration Method Used :

This instrument was calibrated using the Calibration In - house method : SCAL.WI.014 based on ASTM E 715 : 1980
(reapproved 2001)

The Southern Calibration Service Co.,Ltd.calibration control system complies with requirement of ISO/IEC 17025:2017

Traceability of measurement :

This Certificate is traceable to the International and /or national standards which realize the units of measurement
according to the International System of Unit (SI) through :

- SCaL : Sounthern Calibration Service Co., Ltd.,

Calibrated by : Ibrorhim Saleemin

Approved by :

Imron Rattanaylum / Technical Manager

The uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written approval of Southern Calibration Service Co., Ltd.

Details of Calibration

1. Reference Standard Equipment Used:

Equipment	Model	Serial No.	Cert. no.	Due Date
Data Acquisition/Switch Unit	34970A	MY58009813	23SDAT004	23-May-2024

2. The results reported in this certificate refer to the condition of the instrument on the date of calibration

and carry no implication regarding the longterm stability of instrument.

3. This certificate is not certified any commercial transaction


4. Condition of Item : normal condition , no indication for any damage or malfunction

Result of Calibration .:

(✓) Without Adjustment

() After Adjustment

1. Sensor Installation Diagram

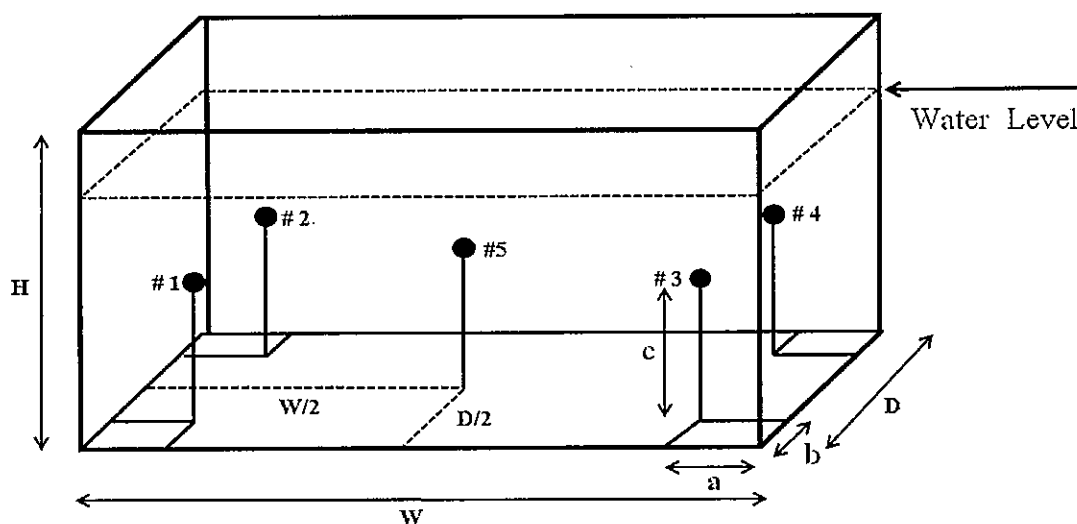

Sensor Installation Details

a = 5 cm
b = 5 cm
c = 5 cm

Dimension of the chamber

W = 45 cm
H = 30 cm
D = 35 cm



Certificate No. : 23TH3097

CSR No. : A095/04743

Page. : 3 of 3

Result of Calibration :

2. Temperature Measurement Accuracy Test

The measurement results of the Water Bath and associates are reported in the manner as shown below

Cal point (°C)	Measured Standard Temperature At Spread Locations (°C)					Uncertainty (± °C)
	#1	#2	#3	#4	Ref.5	
80	79.17	79.47	79.43	79.25	79.38	0.14

3. Performance Result

The performance of the Water Bath are reported as shown below

Cal point (°C)	UUC Setting (°C)	UUC Reading (°C)	Temperature Stability (± °C)	Temperature Uniformity (°C)	Overall Variation (°C)
80	80.0	80.0	0.24	0.38	0.38

- UUC = Unit Under Calibration

The report uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$,
providing a level of confidence of approximately 95%

... End ...

Certificate of System Qualification

GC-OQ + GCMS-OQ

System ID: RYG_EN0136
Organization Name: ALS Laboratory Group (Thailand) Co.Ltd.
Organization Location: 616/10, Moo 5, Tambol Mae Nam Khu, Pluak Daeng, Rayong,21140, Thailand

Date: January 5, 2024 10:53:24 AM
EQP Name: AgilentRecommended , AgilentRecommended
EQP Revision: GC.02.54, GCMS.02.54
Overall Qualification Status: Pass

REVIEW BY

APPROVED BY

NEXT CAL. DATE

1/07/2025

CDS Logon Verification - GC

Logon: chonticha.khunkaew

Overall CDS Logon Verification - GC Test Status

Pass

System Inspection and Basic Safety and Operation

Name: 7890

Setpoint Status: Pass

Overall System Inspection and Basic Safety and Operation Test Status

Pass

Inlet Pressure Accuracy

Name: 7890

Front SSL

Setpoint Status: Pass

	Setpoint		Actual	
Inlet Pressure:	25.0	psi	25	psi
Accuracy:			0.0	psi
Agilent Recommended:			<= 1.2	

Date: January 5, 2024 10:53:24 AM
System ID: RYG_EN0136

Overall Inlet Pressure Accuracy Test Status

Pass

GC Oven Temperature Accuracy

Name:	7890				
Setpoint Status:	Pass				
Zone:	Oven				
	Setpoint/Actual				
Temperature:	230.0	229	°C		
Accuracy:		-1.0	°C		
Agilent Recommended:	>=	-1.0	% setpoint in K	(-5.0	°C)
	<=	1.0	% setpoint in K	(5.0	°C)
Setpoint Status:	Pass				
Zone:	Oven				
	Setpoint/Actual				
Temperature:	100.0	100.8	°C		
Accuracy:		0.8	°C		
Agilent Recommended:	>=	-1.0	% setpoint in K	(-3.7	°C)
	<=	1.0	% setpoint in K	(3.7	°C)

Overall GC Oven Temperature Accuracy Test Status

Pass

GC Oven Temperature Stability

Name:	7890				
Setpoint Status:	Pass				
	Setpoint/Average				
Temperature:	100.0	100.8167	°C		
Stability:		0.1	°C		
Agilent Recommended:	<=	0.5			

Overall GC Oven Temperature Stability Test Status

Pass

Log Amp

Tested Combination1 Front SSL / External SQ

Name: 5977B

Setpoint Status: Pass

Overall Log Amp Test Status

Pass

RFPA

Tested Combination1 Front SSL / External SQ

Name: 5977B

Setpoint Status: Pass

Amu: 1050 m/z

Drift After Five Minutes:

6 mV

RFPA Voltage:

509 mV

Agilent Recommended:

>= -100

and

<= 100

<= 1100

Overall RFPA Test Status

Pass

Tune EI

Tested Combination1 Front SSL / External SQ

Name: 5977B

Setpoint Status: Pass

Filament: 1

Setpoint Status: Pass

Filament: 2

Overall Tune EI Test Status

Pass

Scouting Run

Date: January 5, 2024 10:53:24 AM
System ID: RYG_EN0136

Tested Combination1	Front	SSL	/ External	SQ
	Manual Injection			
Name:	Not applicable			
Source:	EI - Extractor			
Setpoint Status:	Completed			
Injection Volume on Column:	1.0 uL			
Overall Scouting Run Status				
Completed				

Signal to Noise EI

Tested Combination1	Front	SSL	/ External	SQ
Name:	5977B			
Source:	EI - Extractor	Filament:	1	
Setpoint Status:	Pass			
Signal to Noise:	5113			
Agilent Recommended:	>= 1200			
Source:	EI - Extractor	Filament:	2	
Setpoint Status:	Pass			
Signal to Noise:	4456			
Agilent Recommended:	>= 1200			

Overall Signal to Noise EI Test Status

Pass

NOTE: This test's 2 comment(s) and 3 deviation(s) are available in the Attachments section.

Instrument Details

Purpose

This section describes the as found system configuration.

Details

System

System ID	RYG_EN0136
Manufacturer	Agilent Technologies
Name	7890
Flow Data Input	Manual Data
Temperature Data Input	Manual Data or Other Data Logging

Tested Combination1

Injection Technique	Manual Injection
Inlet	Front
Detector	External
LTM Included?	No

Sampler 1

Manufacturer	Agilent Technologies
Type	Manual Injection
Usage	Sample Injection
Syringe Volume (µL)	10

Mainframe 1

Manufacturer	Agilent Technologies
Name	7890
Model Number	G3442B
Serial Number	CN16463238
Firmware Revision	B.02.04.3
Component ID/Asset No.	081117000236
Oven Type	Standard

Inlet 1

Manufacturer	Agilent Technologies
Name	7890
Type	SSL
Location	Front
Carrier Gas	Helium
Control Type	Electronic Pressure Control (EPC)
Purged Inlet	Yes

Detector 1

Manufacturer	Agilent Technologies
Name	Mass Spectrometer
Type	Mass Spectrometer
Location	External

Mass Spectrometer 1

Manufacturer	Agilent Technologies
Type	SQ
Name	5977B
Model Number	G7077B
Serial Number	US1701M008
Firmware Revision	5977 6.00.34
High Vacuum System	Turbo Pump
Scouting Run Standard	OFN Std
Component ID/Asset No.	081117000236

MS EI Source 1

Manufacturer	Agilent Technologies
Source Type	EI - Extractor
Number of filaments	2

Electronic Signature

Purpose

This signature page was created and published because the ACE sign-off action was executed, which is valid for the entire document, including attachments. The ACE sign-off is an electronic signature that requires two distinct identification components: unique username and personal password. The Agilent representative who has delivered this service understands the meaning and legal status of an electronic signature. As a trained official operator, the Agilent representative has a unique password and logon to access ACE and electronically sign this document. (Other e-signatures can be applied to this document using a Document Content Management or other suitable method defined in your data access and control procedures.)

Details

Full Name of Signer:	Eaknarin Puangsopa
Logged On User Name:	eaknarin_puangsopa@agilent.com
Signature Creation Date:	January 5, 2024
Reason for Signature:	Executed protocol and published this original version of document

Regulatory Disclaimer

This document provides a protocol to verify and record instrument configuration and evidence of proper operation. It has been prepared from our interpretation of applicable regulations as well as industry best practices. The document is designed to provide an important component of a complete compliance package. Validation depends upon many factors and use of this protocol alone does not assure compliance. Agilent Technologies makes no promises or representations as to its sufficiency for any specific regulatory program.

Warranty

Agilent Technologies makes no warranty of any kind to this material, including but not limited to, the implied warranties or merchantability and fitness for a particular purpose. Agilent Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

User Name: eaknarin_puangsoa
Report Generated by Hostname: ASRYGWX074

System Id: RYG_EN0136
Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 4, 2024 10:37:31 AM	Audit	SessionCreated	Session	None
January 4, 2024 10:37:31 AM	Start	Configuration	Session	None
January 4, 2024 10:37:31 AM	Audit	Entitlement	Licensing	User is FieldEngineer and does not require an unlock code
January 4, 2024 10:39:29 AM	Audit	EqpLoaded	Session	EQP details for primary technique [Gc] - File path: [ProtocolPacks/Gc/Configurations/02.54/Gc.02.54.eqp], EQP File Name: [Gc.02.54.eqp], EQP Name: [AgilentRecommended], Protocol Revision :[Gc.02.54] EQP details for hyphenated technique [GcMs] - File path: [ProtocolPacks/GcMs/Configurations/02.54/GcMs.02.54.eqp], EQP File Name: [GcMs.02.54.eqp], EQP Name: [AgilentRecommended]
January 4, 2024 10:39:40 AM	End	Configuration	Session	None
January 4, 2024 10:39:44 AM	Start	Qualification	Session	OQ
January 4, 2024 10:39:44 AM	Start	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	None
January 4, 2024 10:46:00 AM	End	Execution	CDS Logon Verification - GC - 7890: - Qualitative test	Run Count : 1

User Name: eaknarin_puangsoa
Report Generated by Hostname: ASRYGWX074

System Id: RYG_EN0136
Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 4, 2024 10:46:05 AM	Start	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	None
January 4, 2024 10:46:18 AM	End	Execution	System Inspection and Basic Safety and Operation - 7890: - Qualitative Test - No setpoints associated	Run Count : 1
January 4, 2024 10:46:22 AM	Start	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	None
January 4, 2024 10:48:52 AM	End	Execution	Inlet Pressure Accuracy - Front SSL: - Pressure Controlled Inlet - S: 25.0 psi - L: <= 1.2 psi	Run Count : 1
January 4, 2024 10:48:54 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
January 4, 2024 10:51:05 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry
January 4, 2024 10:51:08 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 230.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
January 4, 2024 10:51:43 AM	Start	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	None
January 4, 2024 10:58:45 AM	Audit	Data	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Manual Data Entry

Page 2 / 7

User Name: eaknarin_puangsoa
Report Generated by Hostname: ASRYGWX074

System Id: RYG_EN0136
Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 4, 2024 10:58:46 AM	End	Execution	GC Oven Temperature Accuracy - 7890: - Temperature : Oven - S: 100.0°C - L: >= -1.0 AND <= 1.0 % setpoint in K	Run Count : 1
January 4, 2024 10:58:59 AM	Start	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	None
January 4, 2024 11:23:26 AM	Audit	Data	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Manual Data Entry
January 4, 2024 11:23:29 AM	End	Execution	GC Oven Temperature Stability - 7890: - Temperature : Oven - S: 100.0°C - L: <= 0.5°C	Run Count : 1
January 4, 2024 11:23:35 AM	Start	Execution	Log Amp - 5977B SQ: - Source: EI - Extractor	None
January 4, 2024 11:43:23 AM	End	Execution	Log Amp - 5977B SQ: - Source: EI - Extractor	Run Count : 1
January 4, 2024 11:43:26 AM	Start	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	None
January 4, 2024 11:53:23 AM	End	Execution	RFPA - 5977B SQ: - Source: EI - Extractor	Run Count : 1
January 4, 2024 11:53:28 AM	Start	Execution	Tune EI - 5977B SQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	None
January 4, 2024 1:37:26 PM	End	Execution	Tune EI - 5977B SQ: - Source: - EI - Extractor Filament 1 (Qualitative - No setpoints associated)	Run Count : 1
January 4, 2024 1:37:29 PM	Start	Execution	Tune EI - 5977B SQ: - Source: - EI - Extractor Filament 2 (Qualitative - No setpoints associated)	None

Page 3 / 7

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Report Generated by Hostname: ASRYGWX074

Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 4, 2024 1:48:59 PM	End	Execution	Tune EI - 5977B SQ: - Source: - Run Count : 1 EI - Extractor Filament 2 (Qualitative - No setpoints associated)	
January 4, 2024 1:49:02 PM	Start	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
January 4, 2024 2:20:35 PM	Audit	AceClosed	Session	None
January 5, 2024 8:28:16 AM	Audit	AceRestarted	Session	None
January 5, 2024 8:28:18 AM	Audit	SessionReloaded	Session	None
January 5, 2024 8:28:29 AM	Start	Qualification	Session	OQ
January 5, 2024 8:28:29 AM	Start	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	None
January 5, 2024 9:21:29 AM	Audit	Data	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Data files Path : D:\OQ2024\scout1.D
January 5, 2024 9:21:53 AM	End	Execution	Scouting Run - Manual Injection, Front SSL, SQ: - Source: - EI - Extractor- Part of GCMS System Preparation	Run Count : 1
January 5, 2024 9:21:58 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None

Page 4 / 7

User Name: eaknarin_puangsoapa

System Id: RYG_EN0136

Report Generated by Hostname: ASRYGWX074

Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 5, 2024 9:25:39 AM	End	Qualification	Session	OQ
January 5, 2024 9:25:39 AM	Start	Reporting	Session	None
January 5, 2024 9:27:46 AM	End	Reporting	Session	None
January 5, 2024 9:27:46 AM	Start	Qualification	Session	OQ
January 5, 2024 9:27:46 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	None
January 5, 2024 9:33:18 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Data files Path : D:\OQ2024\SN_F1.D
January 5, 2024 9:45:22 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 1 - L: >= 1200	Run Count : 1
January 5, 2024 9:45:32 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
January 5, 2024 9:56:15 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2024\SN_F2.D
January 5, 2024 10:00:19 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 1

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Report Generated by Hostname: ASRYGWX074

Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 5, 2024 10:03:53 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 1
January 5, 2024 10:03:53 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
January 5, 2024 10:13:48 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2024\SN_F02.D
January 5, 2024 10:17:58 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 2
January 5, 2024 10:22:04 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 2
January 5, 2024 10:22:04 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
January 5, 2024 10:22:15 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2024\SN_F02.D
January 5, 2024 10:25:37 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 3

Page 6 / 7

User Name: eaknarin_puangsoa

System Id: RYG_EN0136

Report Generated by Hostname: ASRYGWX074

Print Date: January 5, 2024 10:53:25 AM

ALS_OQ_RYG_EN0136 Transaction log :

Time	Transaction State	Activity Performed	Type of Transaction	Optional Information
January 5, 2024 10:29:11 AM	Audit	TestUnlocked	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Deviation filed for Run Count : 3
January 5, 2024 10:29:11 AM	Start	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	None
January 5, 2024 10:42:05 AM	Audit	Data	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Data files Path : D:\OQ2024\SN_F002.D
January 5, 2024 10:46:34 AM	End	Execution	Signal to Noise EI - Liquid Injection, Front SSL, SQ: - Source: EI - Extractor using Filament 2 - L: >= 1200	Run Count : 4
January 5, 2024 10:46:41 AM	End	Qualification	Session	OQ
January 5, 2024 10:46:41 AM	Start	Reporting	Session	None
January 5, 2024 10:50:27 AM	Audit	Reporting	Session	Report Generated : Certificate
January 5, 2024 10:51:07 AM	Audit	Reporting	Session	Report Generated : Report
January 5, 2024 10:51:29 AM	Audit	Reporting	Session	Report Generated : Certificate
January 5, 2024 10:52:00 AM	Audit	Reporting	Session	Report Generated : Report

Page 7 / 7

TEST REPORT

REVIEW BY ...


APPROVED BY ...

NEXT CAL. DATE 11/6/25

CUSTOMER NAME : ALS Laboratory Group (Thailand) Co., Ltd. [บริษัท เอแอลเอส แล็บอราทอรี กรุ๊ป (ประเทศไทย) จำกัด]			
EQRIPMENT NAME : THC Analyzer			
MANUFACTURER : HORIBA		MODEL : APHA-370	SERIAL NO : WKJ0NS9M
STANDARD GAS CONCENTRATION (PPM) : 506.1 PPM			CYLINDER NO : CC734373
CYLINDER PRESSURE (pslg) : 1,000 PSI			CERTIFIED DATE : 12/05/2020
CERTIFIED BY : AIRGAS			EXPIRED DATE : 12/05/2028


TEST RESULTS

POINT NO	TEST RESULTS						
	IDEAL	ACTUAL CH4	ERROR CH4	%ERROR CH4	ACTUAL THC	ERROR THC	%ERROR THC
ZERO	0.000	0.00	0.000	-	0.00	0.000	-
1	10.000	10.30	0.300	3.00	10.29	0.290	2.90
2	20.000	20.20	0.200	1.00	20.09	0.090	0.45
3	30.000	30.01	0.010	0.03	30.10	0.100	0.33
4	40.000	39.90	-0.100	-0.25	39.99	-0.010	-0.02
AVERAGE (%)				0.95			0.91

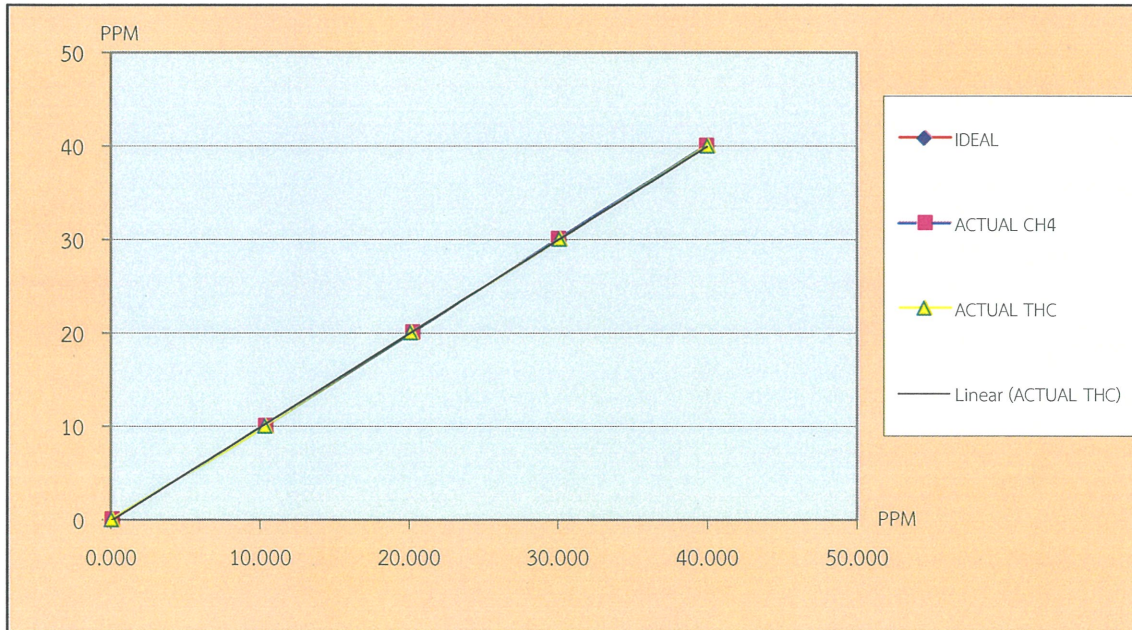

CALIBRATED BY :

CHECKED BY :

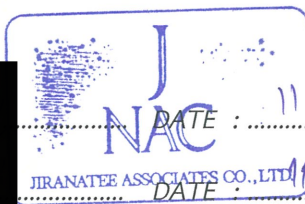

DATE :

DATE :

ต้องการข้อมูลทางด้านเทคนิคเพิ่มเติม : เจ้าหน้าที่ฝ่ายบริการหลังการขาย , โทร 02-868-0812 # 15,16 , E-Mail : Engineer@jiranatee.com
เลขที่ 63/14-15,67/35-36 ถนนเพชรเกษม 7,7/1 แขวงวัดท่าพระ เขตบางกอกใหญ่ กรุงเทพฯ 10600 โทร 02-8680812-13 โทรสาร 02-868-1889