

ภาคผนวก ณ

สำเนาเอกสารสอบเทียบเครื่องมือตรวจวัดและวิเคราะห์

List of Instruments Certification for Air & Noise Quality Analysis

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration	Remark
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Andersen Instruments, Inc.	G25A 1901	Jiranatee Associates Co., Ltd.	COF-002-66	14 Jul 23	13 Jul 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	24P1251	11 Apr 24	10 Apr 25	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24P1369	22 Apr 24	21 Apr 25	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM ₁₀)	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	24H753	10 Apr 24	9 Apr 25	-
Water									
1	pH Meter	pH	Horiba	LAQUA-PH210 HA0D0078	Technology Promotion Association (Thailand-Japan)	24CH239	20 Feb 24	19 Feb 25	-
2	DO Meter	DO	Horiba	LAQUA-DO210 HE9M0013	Technology Promotion Association (Thailand-Japan)	24TW5	10 Jan 24	9 Jan 25	-
3	Conductivity Meter	Conductivity	Horiba	LAQUA-EC210 HC1L0016	Technology Promotion Association (Thailand-Japan)	24CH236	20 Feb 24	19 Feb 25	-

CERTIFICATE OF CALIBRATION

Certificate No. : COF-002-66

Page 1 of 2 Pages

MEASUREMENT ITEM : Top Load Orifice
MANUFACTURER : Andersen Instruments
MODEL/TYPE : G25A
SERIAL NUMBER : 1901
ID NUMBER : UAE.ANV.051/2547
CONDITION AS-RECEIVED : Used item
CUSTOMER : United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,
Bangkok 10260

RECEIVED DATE : 07 Jul 2023
MEASUREMENT DATE : 14 Jul 2023
ISSUE DATE : 18 Jul 2023

ENVIRONMENTAL CONDITIONS:
Ambient condition in the laboratory are as follow:
Temperature : 23.0 ± 3.0 °C
Relative Humidity : 55.0 ± 15.0 %RH
Atmospheric Pressure : 1010 ± 10 hPa

CALIBRATION CONDITION:
Preconditioning : 24 hours at ambient conditions.
Measurement Condition : The average values during measurement are 23.9 °C and 54.5%RH.

NOTED: The certificate is valid only to the item calibrated on date and place of calibration.

TABULATION OF RESULTS:
The table on next page give the measured values.

Calibration procedure:
The Orifice gas flow device was calibrated against
Standard Rotary Displacement Meter (Roots
Meter) Model G65/IMC/V2-dp. The Wt-GL-004
was used as a calibration guideline.

Traceability:
This certificate provides a traceability of The
measurement to recognized the national
standards, and to realization of the international
system of units (SI) through the VSL (National
Metrology Institute of Netherlands) via Certificate
number: G2211901

Uncertainty of Measurement:
The reported uncertainty of measurement is based
on the standard uncertainty multiplied by a
coverage factor k=2, Which for a normal
distribution corresponds to a coverage probability
of approximately 95%. The standard uncertainty
has been determined in accordance with the GUM
Evaluation of measurement
data - Guide to the expression of uncertainty in
measurement

MEASUREMENT RESULTS:

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

Table 1: The results of Q Standard calibration data

Plate	Flow rate m³/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH₂O	γ	Standard Flow [Qs] m³/min
1	0.701	754.115	23.87	23.10	55.600	1.626	1.273	0.648
2	0.997	754.083	23.80	23.23	61.350	3.236	1.795	0.914
3	1.121	754.005	23.81	23.20	41.923	4.338	2.079	1.057
4	1.172	754.004	23.72	23.16	30.933	4.891	2.208	1.122
5	1.410	753.994	23.76	23.18	29.415	7.159	2.671	1.352

Slope (m): 1.98463
Intercept (b): -0.01636
Correlation coefficient (r): 0.99972
Uncertainty (k=2): 0.015 m³/min

Table 2: The results of Q actual calibration data

Plate	Flow rate m³/min	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	Δp_meter mmHg	Δp_Orifice inH₂O	γ	Standard Flow [Qs] m³/min
1	0.701	754.115	23.87	23.10	55.600	1.626	0.800	0.651
2	0.997	754.083	23.80	23.23	61.350	3.236	1.129	0.917
3	1.121	754.005	23.81	23.20	41.923	4.338	1.307	1.061
4	1.172	754.004	23.72	23.16	30.933	4.891	1.388	1.126
5	1.410	753.994	23.76	23.18	29.415	7.159	1.679	1.357

Slope (m): 1.24306
Intercept (b): -0.01029
Correlation coefficient (r): 0.99972
Uncertainty (k=2): 0.015 m³/min

End of Certificate of Calibration

Calibrated by:
☐ Mr. Sorawit Thachalad
☒ Miss Jitraporn Lertsomphol



Approved signatory: Mr. Parinya Booncharoen
Calibration Department Manager



เอกสารไม่ควบคุม

เอกสารไม่ควบคุม

THIS CERTIFICATE REPORT MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484

Certificate of Calibration

Certificate No. : 24P1251
Page : 1 of 2

Equipment : U Tube Manometer
Manufacturer: Dwyer
Model : 1221-36-W/M
Serial No.: -
ID No.: UAE.EFM.077/2566

Condition As-Received: Used Item
Received Date: 03 April 2024
Calibration Date: 11 April 2024

Reference: 2404-0118WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Atmospheric Pressure: 1012 mbar

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Pressure Calibrator	PC106P	1189	MP-0176-23	12 Sep 2024

- This result of calibration was made on requested at the point specified by customer.
- Scale and conversion factor is 1 kPa = 4.0146293 inH₂O
- This instrument was used clean air as pressure media.
- This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.
- This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.
- The certificate is valid only to the item calibrated on date and place of calibration.
- This Certification is traceable to the International System of Unit maintained through:-
-National Institute of Metrology (Thailand), NSC-ONSC Accredited No. Calibration 0144

Calibrated by : Suksan Khankaew
Issue Date : 17 April 2024

Approved Signatory :
[] Phalinee Pratsapaipal
[] Sura Suwannasri
[✓] Attapol Panurach

เอกสารไม่ควบคุม



Cert.No.: 24P1251
Page : 2 of 2

Result of calibration:- Without adjustment
Function:- Pressure Measurement
Increasing Pressure

Range: 0 inH₂O to 36 inH₂O
Scale Interval: 0.1 inH₂O (The Second Estimate)

Applied Pressure	High-port side	UUC Indication Low-port side	ΔP	Error
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-1.00	2.00	0.00
4.00	2.00	-2.00	4.00	0.00
6.00	3.00	-3.00	6.00	0.00
8.00	4.00	-4.00	8.00	0.00
10.00	5.00	-5.00	10.00	0.00
12.00	6.00	-6.00	12.00	0.00
14.00	7.05	-7.05	14.10	0.10
16.00	8.05	-8.05	16.10	0.10
18.00	9.05	-9.05	18.10	0.10
20.00	10.05	-10.05	20.10	0.10
22.00	11.05	-11.05	22.10	0.10
24.00	12.05	-12.05	24.10	0.10
26.00	13.05	-13.05	26.10	0.10
28.00	14.05	-14.05	28.10	0.10
30.00	15.05	-15.05	30.10	0.10
32.00	16.05	-16.10	32.15	0.15
34.00	17.05	-17.10	34.15	0.15
35.80	18.00	-18.00	36.00	0.20

The uncertainty of measurement was ± 0.11 inH₂O

* ΔP = High-port side - Low-port side

* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม

Certificate of Calibration

Customer

Certificate No : 24-AFM-173

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Request No : Req-2024-1833

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Unit Under Calibration Details

Measurement Item : Air Flow Meter

Manufacturer : BGI Accuracy : 0.75% of Reading

Model : Delta Cal DC1 Sensor Model : -

Serial Number : 158850 Sensor Serial Number : -

ID : UAE.EFM.038/2561 Instrument Status : Used

Location of Calibration : LAB 4 AIR VELOCITY METER

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 20 %RH

Barometric Pressure : 1013 hPa ± 10 hPa

Received Date : 15 August 2024

Calibration Date : 28 August 2024

Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator

Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 High flow	18501012012	Sensidyne	1 August 2025
Temperature meter	GT 11	08000057	Qreborn	1 March 2025
Pressure meter	CPG2400	41000KDU/651882	TPA	9 November 2024

Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k = 2$, providing a level of confidence approximately 95 %.

Calibration By : 

Approved By : 

Mr. Noppadon Luangart

Mr. Pacit Mathavorn

Service Calibration Engineer

Calibration Engineer Supervisor

Issue Date : 28 August 2024

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.04 Issue date 17/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAE0,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 660-2116-5860-1 FAX: 660-2116-7140



ASST National Accreditation Board
A C C R E D I T E D
CALIBRATION LABORATORY
AC 2901

Page 2/3

Certificate No : 24-AFM-173

Request No : Req-2024-1833

Result of Calibration : Without Adjustment

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Uncertainty (l/min)	MPE (l/min)	Result
25.60	99.80	14.50	14.46	-0.04	0.20	0.109	N/A
25.60	99.80	15.00	14.95	-0.05	0.21	0.113	N/A
25.50	99.70	15.80	15.73	-0.07	0.22	0.119	N/A
25.40	99.60	16.67	16.59	-0.08	0.23	0.125	N/A
25.50	99.50	18.30	18.20	-0.10	0.26	0.137	N/A

Note

STD : Standard

UUC : Unit Under Calibration

- UUC Reference Condition : 25 °C, 101.3 kPa, Air

- Flow Rate was corrected for non-standard operating condition by using equation :

$Q_{meas} = Q_{ref} \times \frac{P_{ref}}{P_{meas}} \times \frac{T_{meas}}{T_{ref}}$

where

Q = Flow Rate

P = Absolute Pressure

T = Absolute Temperature

Meas = Measurement Condition

ref = Standard Condition

* Indicates non accredited

MPE = Maximum Permissible Error (Specified in Manufacturer's Specifications)

N/A = Not Available, Customer does not require a statement of conformity.

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.04 Issue date 17/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAE0,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 660-2116-5860-1 FAX: 660-2116-7140



ASST National Accreditation Board
ACCREDITED
CALIBRATION LABORATORY
AC 2901

Page 3/3

Certificate No : 24-AFM-173

Request No : Req-2024-1833

Decision Rule for Statements of Conformity


The standard decision rule employed for the statements of conformity to each calibration result will be applied using ILAC-G8:09:2019; Guidelines on the Reporting of Compliance with Specification as following Fig. and statements

Pass = The measurement result plus the expanded uncertainty with a 95% coverage probability were within the limit.

Pass¹ = The measurement result was within the limit. However, a portion of the expanded uncertainty of measurement at 95% exceeds the limit.

Fail¹ = The measurement result was out of the limit. However, a portion of the expanded uncertainty of measurement at 95% is within the limit.

Fail = The measurement result plus the expanded uncertainty with a 95% coverage probability were outside the limit.

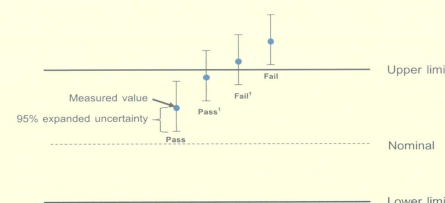

End of Certificate

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-AFM-01 Rev.04 Issue date 17/6/24

INNOVATIVE INSTRUMENT CALIBRATION LAB
INNOVATIVE INSTRUMENT CO., LTD. HEAD OFFICE
7/139 MOO 13, SOI SUNTINAKORN 11 TAMBON BANG KAE0,
AMPHOE BANG PHLI SAMUT PRAKAN PROVINCE 10540 THAILAND
TEL.: 660-2116-5860-1 FAX: 660-2116-7140



NSC-TISI-TIS17225
CALIBRATION 0298

Certificate of Calibration

Customer

Certificate No : 24-TPM-390

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Request No : Req-2024-1833

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong, Bangkok 10260

Page : 1/2

Unit Under Calibration Details

Calibration Parameter : Temperature

Instrument Name : Air Flow meter Range Calibration : 20 °C to 50 °C

Manufacturer : BGI Type of Sensor : RTD

Model : Delta Cal DC1 Sensor Diameter (mm) : 3

Serial Number : 158850 Calibration Position (mm) : 45

Resolution : 0.1 °C Instrument Status : Used

ID Number : UAE.EFM.038/2561

Calibration Environment and Details

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 15 %RH

Received Date : 15 August 2024

Calibrated Date : 29 August 2024

Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard

Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN: 08000057, ID: 02-TPM Which was calibrated on 1 March 2024, Calibration Certificate No. : QR24-0478

Traceability

This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.: Calibration 0292

Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor $k=2$, providing a level of confidence approximately 95 %.

Approved By : 

Mr. Noppadon Luangart

Technical Manager

29 August 2024

Issue Date :

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.

FM-708-TPM-01 Rev.01 Issue date 13/02/20



Calibration Note
UUC Adjustment : Not Adjust
Certificate No : 24-TPM-391
Request No : Req-2024-1832
Page : 2/2

Result of Calibration :

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
Ta	20.031	20.0	0.0	0.13
	25.034	25.1	-0.1	0.13
	30.035	30.1	-0.1	0.13
	35.029	35.1	-0.1	0.13
	40.011	39.9	+0.1	0.13
	45.008	44.8	+0.2	0.13
	50.007	49.8	+0.2	0.13
Tf	20.031	19.9	+0.1	0.13
	25.034	24.9	+0.1	0.13
	30.035	30.0	0.0	0.13
	35.029	35.1	-0.1	0.13
	40.011	40.1	-0.1	0.13
	45.008	45.2	-0.2	0.13
	50.007	50.2	-0.2	0.13

End of Certificate

Calibrated By :
Mr. Sitsichok Jarapakdeesakul

เอกสารไม่ควบคุม

The results related only to the item calibrated. The certificate shall not be reproduced except in full, without written approval of the Innovative Instrument Co., Ltd.
FM-708-TPM-01 Rev.01 Issue date 13/02/20



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 24P1369
Page : 1 of 2

Equipment : Aneroid Barometer
Manufacturer: Barigo
Model : -
Serial No.: -
ID No.: UAE.ANV.013/2547

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item
Received Date: 05 April 2024
Calibration Date: 22 April 2024

Reference: 2404-0243WSC
Ambient Temperature: (23 ± 2) °C
Relative Humidity: (50 ± 15) %
Atmospheric Pressure: 1007 mbar
Submitted by: United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges " as a guidelines.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024
2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.				
3.This result of calibration was made on requested at the point specified by customer.				
4.Scale and conversion factor is 1 kPa = 7.50062 mmHg				
5.This result of calibration instrument was in absolute pressure.				
6.This instrument was used clean air as pressure media.				
7.The certificate is valid only to the item calibrated on date and place of calibration.				
8.This Certification is traceable to the International System of Unit maintained through-				
-National Institute of Metrology Thailand (NIMT)				

Calibrated by : Suksan Khankaew
Issue Date : 23 April 2024

Approved Signatory :
[] Phalinee Prabpaipal
[] Sura Suwannasri
[✓] Attapol Panurach

เอกสารไม่ควบคุม



Cert.No.: 24P1369
Page: 2 of 2

Result of calibration:- Without adjustment
Function:- Absolute Pressure Measurement

Range : 720 mmHg to 780 mmHg
Scale Interval : 1 mmHg (The Fifth Estimate)

Increasing Pressure	718.40	729.71	740.61	751.07	761.97	773.05	786.91
Applied Pressure (mmHg)	718.40	729.71	740.61	751.07	761.97	773.05	786.91
UUC* Indication (mmHg)	720.0	730.0	740.0	750.0	760.0	770.0	780.0
Error (mmHg)	1.60	0.29	-0.61	-1.07	-1.97	-3.05	-6.91

Decreasing Pressure	786.91	772.99	761.71	750.69	740.13	729.35	718.44
Applied Pressure (mmHg)	786.91	772.99	761.71	750.69	740.13	729.35	718.44
UUC* Indication (mmHg)	780.0	770.0	760.0	750.0	740.0	730.0	720.0
Error (mmHg)	-6.91	-2.99	-1.71	-0.69	-0.13	0.65	1.56

The uncertainty of measurement was ± 0.24 mmHg
* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %.

-000-



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250
TEL. 0-2717-3000-24 FAX. 0-2719-9484



Certificate of Calibration

Certificate No. : 24H753
Page : 1 of 2

Equipment : Dial Thermo-Hygrometer
Manufacturer: Barigo
Model : -
Serial No.: -
ID No.: UAE.ANV.127/2550

This certificate may not be reproduced other than in full, except with the prior written approval of the head of Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item
Received Date: 05 April 2024
Calibration Date: 10 April 2024
to 18 April 2024

Reference: 2404-0247WSC
Ambient Temperature: (25 ± 3) °C
Relative Humidity: (50 ± 20) %
Submitted by: United Analyst and Engineering Consultant Co., Ltd.
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

Condition of this result of calibration

1.Reference standards instruments :

Instrument	Model	Serial No.	Certificate No.	Due Date
1) Chilled Mirror Hygrometer	Dew Master	44730	21656	02 Aug 2024
2) Handheld Thermometer With Sensor	1521	A5A339	231238	16 Oct 2024
2.The certificate is valid only to the item calibrated on date and place of calibration.				
3.This Certification is traceable to the International System of Unit maintained through-				
-Thunder Scientific Corporation, NVLAB Accreditation No, Calibration 200582-0				
-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No, Calibration 0008				

Calibrated by : Chakrit Waewwanjua
Issue Date : 18 April 2024

Approved Signatory :
[] Chakrit Waewwanjua
[✓] Vipom Tantiyawutti
[] Unnophol Harachai

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม



Cert. No.: 24H753
Page.: 2 of 2

Result of Calibration:- Without Adjustment
Function: Humidity Measurement.

Reference Temperature (°C)	Standard Humidity (%R.H.)	UUC* Reading (%R.H.)	Error (%R.H.)	Uncertainty of Measurement (±%R.H.)
25.0	40.1	43	2.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	78	-2.0	1.8

Result of Calibration:- Without Adjustment
Function: Temperature Measurement.

Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (±°C)
20.014	20.0	-0.014	0.72
25.033	25.0	-0.033	0.72
30.010	30.0	-0.010	0.72
35.027	34.5	-0.527	0.72
40.013	39.5	-0.513	0.72

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2.00$, providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 24CH239
Page.: 1 of 3

Certificate of Calibration

Equipment : pH Meter
Manufacturer : Horiba
Model : LAQUA-PH210
Serial No. : HA0D0078
ID No. : UAE.EFM.073/2564(EFM.pH.06/64)
Condition As-Received: Used Item
Received Date : 19 February 2024
Calibration Date : 20 February 2024
Reference : 2402-0594WSC-3
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure : In - house method :
- CP-CH5 by direct measurement with
DC Voltage Standard and direct measurement
with certified reference material (CRM)
- CP-CH8 by comparison with temperature standard

Calibrated by : Walalak Sirithean

Approved by :
Approved Signatory

() Pornthippa Tameyakul
() Unnophol Harachai
(✓) Salthip Meangmai

Issue Date : 22 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0063841



Cert.No.: 24CH239
Page.: 2 of 3

Condition of this calibration result

1. Reference Standard Instrument

Instrument	Serial No.	ID No.	Cert. No.	Due Date
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-
- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Buffer Solution	Manufacturer	Lot No.	Exp. date
pH 4.008	CPA chem	940102	27 Nov 2025
pH 6.986	CPA chem	940104	02 Nov 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration Results

Function : mV Measurement

Performing standard curve by Document Process Calibrator at pH (4,7)(7,10)

Unit Under Calibration	Nominal Value	Standard Voltage Input		Actual Reading		Uncertainty of Measurement (±mV)	Coverage factor k
	pH	mV	mV	pH	pH		
pH Meter S/N.: HA0D0078	4.00	177.48	177.4	4.01	0.058	2.00	
	7.00	0.00	0.0	7.00	0.058	2.00	
	7.00	0.00	0.0	7.00	0.058	2.00	
	10.00	-177.48	-177.5	10.01	0.058	2.00	



Cert.No.: 24CH239
Page.: 3 of 3

Calibration Results

Function : pH Measurement

Performing three buffers standard curve by using buffer nominal pH (4,7)(7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading (mV)	Uncertainty of pH Measurement (±)	Coverage factor k
pH Electrode S/N.: 992H0385	4.008	4.02	168.3	0.0086	2.05
	6.986	6.99	-7.7	0.0093	2.00
	6.986	6.99	-7.6	0.011	2.00
	9.997	10.01	-180.7	0.0085	2.00

Function : Temperature Measurement

(°) Without adjustment

This equipment was connected with Temperature Probe;

- Model : 9652
- Serial No. : 992H0385
Dimension of probe
- Length : 110 mm.
- Diameter : 16 mm.
- Immersion Depth : 100 mm.

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of measurement (± °C)	Coverage factor k
25.0	25.000	25.0	0.000	0.13	2.00
30.0	30.000	30.0	0.000	0.13	2.00
35.0	34.999	35.0	0.001	0.13	2.00

Remark - UUC* = Unit Under Calibrator

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

a 1203291



Cert.No.: 24TW5
Page.: 1 of 2

Certificate of Testing

Equipment : DO Meter
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE9M0013
ID No. : UAE.EFM.016/2563 (EFM.DO.05/63)
Received Date : 09 January 2024
Test Date : 10 January 2024
Reference : 2401-0221WSC-5
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260
Laboratory Condition : Temperature (25 ± 5) °C
Humidity (50 ± 20) %
Test Procedure : In - house method : CP-CH9
by Comparison Technique with Azide Modification Method
Tested by : Walalak Sirinthean
Approved by : 
Approved Signatory
(✓) Saithip Meangmai
() Warakorn Lerngagtrakul
() Ponpan Paipim
Issue Date : 12 January 2024

เอกสารไม่ควบคุม
B 0331592



Cert.No.: 24TW5
Page.: 2 of 2

Condition of this result of calibration

1. Reference Standard Instruments :
This certification is traceable to the International System of Unit through the reference standards laboratory of Industrial Calibration Center, Technology Promotion Association (Thailand-Japan).

Instruments	Serial No.	ID No.	Certificate No.	Due Date
1) Burette	-	130BU10	23CG1172	22 Mar 2025
2) Balance	1124013382	140RC006	23MM18	20 Feb 2024

2. Standard Material :-

Material	Manufacturer	Lot.No.	Assay
Sodium Thiosulfate pentahydrate	Merck	AM1763316	100.2%

Result : Dissolved Oxygen Meter Adjustment With Air 100 %
Dissolved Oxygen Probe No.: 9K9G0097

Titration Method (Azide Modification Method) (mg/L)	DO Meter Reading (mg/L)	Standard Deviation (mg/L)
8.18	8.18	0.0045

This report was certified only for the instrument we tested. It is allowable to use for study the system efficiency. The environmental impact control and present to organization it may concerned. Intend to use for advertising and referral purpose is prohibited. This report may not be reproduced other in full, without written approval of the laboratory.

-000-

เอกสารไม่ควบคุม
a 1197577



Cert. No.: 24LM4
Page.: 1 of 2

Certificate of Calibration

Equipment : DO Meter with Sensor
Manufacturer : Horiba
Model : LAQUA-DO210
Serial No. : HE9M0013
ID No. : UAE.EFM.016/2563 (EFM.DO.05/63)
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udomsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong,
Bangkok 10260
Location : TPA Chemistry Calibration Laboratory
Received Order : 09 January 2024
Calibrated Date : 11 January 2024
Ambient Temperature : (26 ± 10) °C
Relative Humidity : (50 ± 30) %
AC Line Voltage : (220 ± 22) V
Calibrated by : Kunchit Promprat
Approved by : 
Approved Signatory
() Ponthippa Tameyakul
(✓) Ponpan Paipim
() Suwit Imjai
Issue Date : 16 January 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม
A 0062563



Equipment : DO Meter with Sensor
Condition As-Received : Used Item
Reference : 2401-0221WSC-6
Cert. No.: 24LM4
Page.: 2 of 2

Procedure Used :-

Calibration were conducted using in-house calibration procedure CP-OT01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into Temperature Bath.
The temperature scale used was based on ITS-90.

Condition of this result of calibration

1. Reference standard instrument:-
Instrument Serial No. Cert. No. Traceable Due Date
1) Digital Thermometer A52847 2311222 TPA 10 Oct 2024
2. This certificate is valid only to the item calibrated on date and place of calibration.
3. This certification is traceable to the International System of Unit.

Remark : TPA : Technology Promotion Association (Thailand - Japan)

Result of Calibration :- (*) Without Adjustment

Function : Temperature measurement.

This instrument was connected with temperature sensor, S/N.: 9K0E0260

Calibration Point (°C)	Immersion Depth (mm)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty (± °C)	Coverage Factor k
25.0	60	25.000	25.0	0.000	0.16	2.00
30.0	60	30.003	30.0	-0.003	0.16	2.00
35.0	60	35.002	34.9	-0.102	0.16	2.00

UUC* : Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-000-

เอกสารไม่ควบคุม
a 1197712



Cert.No.: 24CH236
Page.: 1 of 3

Certificate of Calibration

Equipment : Conductivity Meter
Manufacturer : Horiba
Model : LAQUA-EC210
Serial No. : HC1L0016
ID No. : UAE.EFM.014/2565(EFM.SCT.01/65)
Condition As-Received: Used Item
Received Date : 19 February 2024
Calibration Date : 20 February 2024
Reference : 2402-0591WSC-5
Submitted by : United Analyst and Engineering Consultant Co.,Ltd.
3 Soi Udornsuk 41, Sukhumvit Road,
Bangchak, Phrakhanong, Bangkok 10260
Ambient Temperature : (25 ± 2.5) °C
Relative Humidity : (50 ± 15) %
Calibration Procedure: In -house method :
- CP-CH6 : based on direct measurement with
certified reference material (CRM)
- CP-CH8 by comparison with Temperature standard

Calibrated by : Warakorn Lemgagtrakul

Approved by :

() Pornthippa Tameyakul
() Unnopphol Harachai
(✓) Saithip Meangmai

Issue Date : 21 February 2024

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.

เอกสารไม่ควบคุม

A 0063816



Cert.No.: 24CH236
Page.: 2 of 3

Condition of this result of calibration

1. Reference Standard Instrument :-

Instrument	Serial No.	ID No.	Certificate No.	Due date
1) Thermometer	1963878	130RC095	2311051	05 Sep 2024
2) Ref. Std. Thermometer	4982054	110RC044	231908	26 July 2024

- This Certification is traceable to SI Through Technology Promotion Association (Thailand - Japan)

2. Certified Reference Materials :-

- Conductivity calibration solution, CPA chem Ltd., The measurement results are traceable to SI
through CPA chem Ltd., ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

Conductivity Solution	Manufacturer	Lot No.	Exp. date
1413.0 µS/cm	CPA Chem	936624	19 Oct 2024
12.880 mS/cm	CPA Chem	931956	30 Sep 2024

- Control Conductivity calibration solution temperature by Water bath (25 ± 0.1) °C

3. This certificate is valid only to the item calibrated on date and place of calibration.

Calibration results

Function : Conductivity Measurement

After Adjustment at 1413.0 µS/cm

Conductivity Electrode Serial No.: 9B1J0042

Standard Conductivity Solution	Before Adjustment UUC* Reading	After Adjustment UUC* Reading	Uncertainty of Measurement (±)	Coverage factor k
1413.0 µS/cm	1422 µS/cm	1413 µS/cm	9.2 µS/cm	2.00
12.880 mS/cm	12.83 mS/cm	12.72 mS/cm	0.086 mS/cm	2.00

Remark : - UUC* = Unit Under Calibration

เอกสารไม่ควบคุม

a 1203079



Cert.No.: 24CH236
Page.: 3 of 3

Calibration Results

Function : Temperature Measurement

This equipment was connected with Temperature Probe;

- Model : 9383
- Serial No. : 9B1J0042

Dimension of probe;

- Length : 110 mm
- Diameter : 16 mm
- Immersion Depth : 100 mm

Calibration Result : Without adjustment

Calibration Point (°C)	Standard Temperature (°C)	UUC* Reading (°C)	Error (°C)	Uncertainty of Measurement (± °C)	Coverage factor k
25.0	25.003	25.0	-0.003	0.13	2.00
30.0	30.004	30.0	-0.004	0.13	2.00
35.0	35.004	35.0	-0.004	0.13	2.00

Remark : - UUC* = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

a 1203078

รายการใบรับรองสอบเทียบ/ทวนสอบ เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์สำหรับวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์คุณภาพอากาศ									
1	Analytical Balance (Readability 0.1 mg)	ฝุ่นละอองรวม (TSP) ฝุ่นละอองขนาดไม่เกิน 10 ไมครอน (PM 10)	Mettler-Toledo	AB204-S/FACT / B108115858	National Food Institute, Ministry of Industry, Thailand	2402420-001-01	19 Apr 24	18 Apr 25	-
2	Analytical Balance (Readability 0.001 mg)		Mettler-Toledo	XP6 / B322373893	National Food Institute, Ministry of Industry, Thailand	2402420-002-01	19 Apr 24	18 Apr 25	-
เครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์คุณภาพน้ำ									
3	pH Meter	ค่าความเป็นกรด-ด่าง (pH)	Mettler-Toledo	Seven Easy S20 / 1230525212	DKSH (Thailand) Ltd.	C07240167	9 Apr 24	8 Apr 25	-
4	pH Meter		Hanna Instrument	HI2020-02 / C0051107	National Food Institute, Ministry of Industry, Thailand	2404042 001 01	14 Aug 24	13 Aug 25	-
5	Analytical Balance (Readability 0.01 mg)	ปริมาณของแข็งแขวนลอย (Suspended Solids)	Mettler-Toledo	XSR205DU / C210685394	National Food Institute, Ministry of Industry, Thailand	2402283-002-01	2 Apr 24	1 Apr 25	-
6	Hot Air Oven		Memmert	UF55 / B212.0411	Technology Promotion Association (Thailand-Japan)	24TM859	1 Apr 24	31 Mar 25	-
7	Analytical Balance (Readability 0.1 mg)	น้ำมันและไขมันบนผิวน้ำ (Floatable Oil & Grease)	Mettler-Toledo	XSR204 / C117635043	Technology Promotion Association (Thailand-Japan)	24MM293	11 May 24	10 May 25	-

Due Date of Calibration* : Based on the annual calibration plan. At least 1 time per year.

Calibration Certificate

Certificate No.: 2402420-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: AB204-S/FACT
Serial No.: B108115858
ID No.: UAE.AIR.016/2555
Order No.: 2402420
Operation No.: 2402420-001
Date of Receipt: 19 April 2024
Date of Calibration: 19 April 2024

Calibrated by Mr.Pheraphat Tuanjit
Scientist
Approved by *P. Jaenghanit*
(Miss Preeyaporn Jaengkanrit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-001-01
Equipment: Electronic Balance
Model: AB204-S/FACT
Serial No.: B108115858
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.0001 g
ID No.: UAE.AIR.016/2555

Page 2 of 3

Date of Calibration: 19 April 2024
Environment Condition: Ambient Temperature: 22.1 ± 0.6 °C Relative Humidity: 49 ± 1.9 %
Place of Calibration: Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Condition of Equipment: Good Condition

Condition of This Results of Calibration:
1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019
2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M23111815	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M23111825	28 November 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFL.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT
4. This certificate was certified only for the instrument we calibrated.
5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:

1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
100	0.000057
200	0.000079

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.
The balance reading obtained is given in the table.

☐	☒	☐
1 (g) 99.9999	2 (g) 99.9997	3 (g) 99.9996
4 (g) 99.9998	5 (g) 100.0000	6 (g) 99.9998
(Maximum Difference) (g) 0.0003		

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-001-01
Equipment: Electronic Balance
Model: AB204-S/FACT
Serial No.: B108115858
Capacity: 220 g
Manufacturer: METTLER TOLEDO
Resolution: 0.0001 g
ID No.: UAE.AIR.016/2555

Date of Calibration: 19 April 2024 **Page 3 of 3**

Calibration Results: (Continued)

Calibration Range: 0-200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000089	2.00
0.1	0.10000	0.1000	0.0000	0.000089	2.00
1	0.99998	1.0000	0.0000	0.000092	2.00
5	4.99997	5.0000	0.0000	0.000091	2.00
10	10.00002	10.0001	-0.0001	0.00012	2.00
20	20.00003	20.0001	-0.0001	0.00014	2.00
50	49.99998	50.0000	0.0000	0.00012	2.00
70	70.00000	69.9999	0.0001	0.00016	2.00
100	99.99997	100.0000	0.0000	0.00017	2.00
150	149.99994	149.9997	0.0002	0.00022	2.00
200	200.00001	199.9995	0.0005	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Certificate

Certificate No.: 2402420-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XP6
Serial No.: B322373893
ID No.: UAE.AIR.019/2556
Order No.: 2402420
Operation No.: 2402420-002
Date of Receipt: 19 April 2024
Date of Calibration: 19 April 2024

Calibrated by Mr.Pheraphat Tuanjit
Scientist
Approved by *P. Jaenghanit*
(Miss Preeyaporn Jaengkanrit)
Vice President, Department of Laboratory Services
Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2402420-002-01
Equipment: Electronic Balance
Model: XP6
Serial No.: B322373893
Capacity: 6.1 g
Manufacturer: METTLER TOLEDO
Resolution: 0.000001 g
ID No.: UAE.AIR.019/2556

Date of Calibration: 19 April 2024 Page 2 of 3

Environment Condition: Ambient Temperature: 22.6 ± 1.8 °C Relative Humidity: 48 ± 6.0 %
Place of Calibration: Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M23111815	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M23111825	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH.019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
3	0.0000057
6	0.0000019

2. Off-Center Error:

A mass of 2 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
(g)	(g)	(g)	(g)	(g)	(g)	(g)
1.999981	1.999983	1.999980	1.999984	1.999983	1.999981	0.000003

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๔๘ ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร 10700
2008 Soi 35, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8588 Fax: +66(0) 2422 8545



nfi.or.th

Calibration Report

Certificate No.: 2402420-002-01
Equipment: Electronic Balance
Model: XP6
Serial No.: B322373893
Capacity: 6.1 g
Manufacturer: METTLER TOLEDO
Resolution: 0.000001 g
ID No.: UAE.AIR.019/2556

Date of Calibration: 19 April 2024 Page 3 of 3

Calibration Results: (Continued)

Calibration Range: 0-6 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value:

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.0000000	0.000000	0.000000	0.0000032	2.00
0.01	0.0099970	0.009999	-0.000002	0.0000047	2.00
0.05	0.0500010	0.050003	-0.000002	0.0000048	2.00
0.10	0.1000010	0.100001	0.000000	0.0000069	2.00
0.15	0.1500020	0.150002	0.000000	0.0000083	2.00
0.17	0.1700050	0.170006	-0.000001	0.000012	2.00
0.20	0.1999990	0.200002	-0.000003	0.0000083	2.00
1.50	1.4999750	1.499971	0.000004	0.000027	2.00
3.00	2.9999680	2.999959	0.000009	0.000028	2.00
4.50	4.4999810	4.499967	0.000014	0.000022	2.00
6.00	5.9999490	5.999931	0.000018	0.000032	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.


----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

2008 ๒๕๔๘ ถนนสุขุมวิท แขวงคลองตัน เขตคลองเตย กรุงเทพมหานคร 10700
2008 Soi 35, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand
Tel: +66(0) 2422 8588 Fax: +66(0) 2422 8545



nfi.or.th



Certificate of Calibration

Equipment: pH METER
Model: SevenEasy
Serial No. (or ID.): 1230525212 (UAE.WAS.003/2553) Job No.: WO-00024208
Manufacturer: METTLER TOLEDO Page: 1 of 3
Electrode Serial No.: 1156883 Model: InLab Solids Brand: METTLER TOLEDO
Condition: In Condition

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udomsuk 41 Sukhumvit Road,
Bangcack, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature 23 °C ± 2 °C
Humidity 50 %RH ± 15 %RH

Calibration Place: Environment Laboratory, DKSH Technology Limited.
2533 Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Miss.Orawan Khlaiphloi

Calibration Date: 9 April 2024

The Method used: In house method, CAL-WI-58, base on ASTM E 70-07

Traceability: This certificate is traceable to SI Units, Sample Test is assured through primary measurement method Harned cell, through CPChem Ltd. (ISO/IEC 17034) Certificate No. 938377, 931985, 931984 And pH Scale traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Industrial Foundation Electrical and Electronics Institute Certificate No. CA20230350EA

Orawan Khlaiphloi
(Miss Orawan Khlaiphloi)
Person in charge

Mr. Nitinun Srihawan
(Mr. Nitinun Srihawan)
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.



Certificate No.: C07240167 Page 2 of 3

Calibration Results:

pH Scale

Input (mV)	pH Meter Reading			Uncertainty of Measurement (mV)	Coverage Factor (k)
	(mV)	Error (mV)	(pH)		
414.12	414	-0.12	0.00	0.58	2.00
354.96	355	0.04	1.00	0.58	2.00
295.8	296	0.20	2.00	0.58	2.00
236.64	237	0.36	3.00	0.58	2.00
177.48	178	0.52	4.00	0.58	2.00
118.32	118	-0.32	5.00	0.58	2.00
59.16	59	-0.16	6.00	0.58	2.00
0	0	0.00	7.00	0.58	2.00
-59.16	-59	0.16	8.00	0.58	2.00
-118.32	-118	0.32	9.00	0.58	2.00
-177.48	-177	0.48	10.00	0.58	2.00
-236.64	-236	0.64	11.00	0.58	2.00
-295.8	-296	-0.20	12.00	0.58	2.00
-354.96	-355	-0.04	13.00	0.58	2.00
-414.12	-414	0.12	14.00	0.58	2.00



Practical slope and zero point*

The three-point calibration using three standard buffer solutions; pH 4.008, pH 6.985 and pH 9.997
-During calibration, display of pH meter reading; pH 4.00, pH 7.00 and pH 10.01
The practical slope of the pH electrode; 57.01 (mV/pH), 96.37%
The zero point of the pH electrode; 6.88 (pH)

Sample Test Results

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Uncertainty of Measurement (pH)	Coverage Factor (k)
4.008	3.99	-0.018	0.0070	2.00
6.985	7.00	0.015	0.0091	2.00
9.997	10.02	0.023	0.0074	2.00

* Calibration Marked "Not TISI Accredited" in this Certificate have been included for completeness.

The End of Certificate

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม

CAL-FM-C07-14: 9 Apr 2024

Certificate No.: C15240373

Page: 2 of 2

Reference standard equipment:

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR23-1073	2 May 23	2 May 24

Calibration Results:

Without Adjustment

Sensor Type: RTD

Channel: -

Diameter (mm) 4

Length (mm): 135

Immersion (mm): 110

Calibrate Point (°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty (± °C)
15.0	15.010	15.1	-0.090	0.076
25.0	25.006	25.1	-0.094	0.076
35.0	35.004	35.0	0.004	0.076


The End of Certificate

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม

CAL-FM-C15-14: 06 Dec 2022



Certificate of Calibration

Equipment: Digital Thermometer with Probe
Model: SevenEasy pH
Serial No.: 1230525212
Manufacturer: METTLER TOLEDO
ID No.: UAE.WAS.003/2553
Certificate No.: C15240373
Issued Date: 09 April 2024
Job No.: WO-00024208
Page: 1 of 2
Condition: In Condition

Customer: United Analyst and Engineering Consultant Company Limited
3 Soi Udomsuk 41 Sukhumvit Road,
Bangchak, Prakanong, Bangkok 10260 Thailand

Environment Condition: Temperature: 22 °C ± 3 °C
Humidity: 50 %RH ± 20 %RH
Voltage: 220 VAC ± 10 %

Calibration Place: Thermo-Hygro Laboratory, DKSH Technology Limited.
2533 Sukhumvit Road, Bangchak,
Phrakhanong, Bangkok 10260 Thailand

Calibration By: Mr. Nateekarn Mitjit
Calibration Date: 09 April 2024
The Method used: In house method, CAL-WI-19, by comparison with standard thermometer
Traceability: This certificate is traceable to the International System of Unit maintained by Quality Reborn Co.,Ltd. (QR) Certificate No. QR23-1073

(Mr. Nateekarn Mitjit)

Person in charge

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

(Mr. Pramote Ramrong)

Authorized signatory

บริษัท ดีเคเอส อีเซีย จำกัด
DKSH Technology Limited
2533 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10260
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand

Delivering Growth - in Asia and Beyond.

เอกสารไม่ควบคุม

CAL-FM-C15-14: 06 Dec 2022



มูลนิธิสถาบันพัฒนาอุตสาหกรรมอาหาร
ศูนย์บริการห้องปฏิบัติการอุตสาหกรรมอาหาร
Foundation for Industrial Development National Food Institute
Food Industrial Laboratory Service Center



Calibration Certificate

Certificate No.: 2404042-001-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO.,LTD.
Address: 3 Soi Udomsuk 41, Sukhumvit Road,
Bangchack, Prakanong, Bangkok 10260

Page 1 of 5

Equipment: pH Meter
Manufacturer: HANNA Instruments
Model: HI2020-02
Serial No.: C0051107
ID No.: UAE.WAO.005/2557
Order No.: 2404042
Operation No.: 2404042-001
Date of Receipt: 14 August 2024
Date of Calibration: 21 August 2024

Calibrated by Mr. Manas Somsak Specialist
Approved by (Mr. Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team
Date of Issue: 21 August 2024

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65

2008 16669 ถนนสุขุมวิท แขวงคลองเตย เขตคลองเตย กรุงเทพมหานคร 10700
2008 Soi 36, Arun Amarin Road, Bang Yi Khan Subdistrict, Bang Phlat District, Bangkok 10700, Thailand.
Tel: +66(0) 2422 6568 Fax: +66(0) 2422 8545

เอกสารไม่ควบคุม

PH-0011

Calibration Report

Certificate No.: 2404042-001-01
Equipment: pH Meter
Resolution: 0.001 pH ; 0.1 mV
Manufacturer: HANNA Instruments Model: HI2020-02
Serial No.: C0051107 Type: Bench top
ID No.: UAE.WAO.005/2557

Date of Calibration: 21 August 2024 Page 2 of 5

Location: Chemical Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature: (23.1 ± 1.5) °C Relative Humidity: (55 ± 3) %
Condition of Equipment: Good Condition

Condition of this Results of Calibration

1. Calibration Method W-CC-002 : In house method based on direct measurement by using standard voltage calibrator and certified reference material (CRM)

2. Reference Standards / Certified Reference Material

Instruments	Serial / ID No.	Manufacturer	Certificate No.	Due Date
2.1 DC Voltage Calibrator	2709007	Fluke	24E1752	30 May 2025
2.2 Digital Thermometer	2709007	Fluke	CC 660570-01	30 October 2024
2.3 Thermo-Hygro Meter	NFI.BTH.019/23	testo	QR24-0492	4 March 2025
Certified Reference Material	Lot. No.	Manufacturer	Ref N	Expire Date
2.4 pH buffer 4.008 (Primary pH buffer Solution)	873608	CPAchem	PH216.L5	16 February 2025
2.5 pH buffer 6.865 (Primary pH buffer Solution)	873609	CPAchem	PH217.L5	16 February 2025
2.6 pH buffer 10.01 (Primary pH buffer Solution)	949189	CPAchem	PH220.L5	30 November 2024
2.7 pH buffer 7.00 (Standard pH buffer Solution)	C03109	HACH LANGE GmbH	S11M004	16 October 2025

3. This certification is traceable to The International System of Unit (SI Unit)

- 3.1 Instruments Ng.2.1 through NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0008
3.2 Instruments Ng.2.2 through NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0061
3.3 Instruments Ng.2.3 through NSC-TISI-TIS 17025 Laboratory Accreditation of Calibration No.0292
3.4 Certified Reference Material Ng.2.4 to 2.6 traceable to Primary measurement method- Harned cell using calibrated thermometer, barometer, and nanovoltmeter. The Standard Solution preparation and certified by CPAchem Ltd is accredited to ISO 17034 and ISO/IEC 17025
3.5 Certified Reference Material Ng.2.7 traceable to PTB Certificate Nr. PTB-PHOA-563/30504/23 and Certificate Nr. PTB-PHOB-555/30620/22 (PTB: Physikalisch-Technische Bundesanstalt, Braunschweig, Germany)

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2404042-001-01
Equipment: pH Meter
Resolution: 0.001 pH ; 0.1 mV
Manufacturer: HANNA Instruments Model: HI2020-02
Serial No.: C0051107 Type: Bench top
ID No.: UAE.WAO.005/2557

Date of Calibration: 21 August 2024 Page 3 of 5

Calibration Results:
1. Calibration of pH Meter (Manual Temperature Compensation at 25 °C)

Nominal pH	DC Voltage Standard (mV)	Average Indicator Reading		Uncertainty (±mV)	Coverage Factor (k)
		mV	pH		
0	414.122	421.0	-0.001	0.063	2.00
2	295.815	302.7	1.999	0.063	2.00
4	177.463	184.3	4.000	0.063	2.00
6	59.160	66.0	6.000	0.063	2.00
7	0.001	6.8	7.001	0.063	2.00
8	-59.159	-52.3	8.000	0.063	2.00
10	-177.462	-170.6	10.000	0.063	2.00
12	-295.813	-289.0	12.002	0.063	2.00
14	-414.121	-407.3	14.002	0.063	2.00

2. Calibration of pH Meter with Electrode (Manual Temperature Compensation at 25 °C)

Equipment: pH Electrode Type: Combined Electrode
Manufacturer: HANNA Instruments Model: HI11310
Serial No.: 539960 ID No.: N/A

Performance of Electrode system (Three-Point Calibration at pH 4, 7 and 10)

Certified Value @25 °C (pH)	Average Indicator Reading		Relative Slope (%)	Uncertainty (± pH)	Coverage Factor (k)
	pH	mV			
4.008	4.011	173.4	-	0.0043	2.00
7.001	7.004	-1.6	98.8	0.0073	2.00
9.997	10.011	-175.9	98.0	0.0073	2.00
6.865	6.870	6.4	-	0.0049	2.00

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2404042-001-01
Equipment: Digital Thermometer with RTD (pH Meter)
Resolution: 0.1 °C Model: HI2020-02
Serial No.: C0051107 ID No.: UAE.WAO.005/2557
Manufacturer: HANNA Instruments

Date of Calibration: 21 August 2024 Page 4 of 5

Location: Chemical Calibration Laboratory, National Food Institute
Environment Condition: Ambient Temperature 23 °C ± 1 °C
Relative Humidity 55 % ± 3 %

Condition of this results of Calibration:

1. Calibration Method :
- In house method: W-TE-025 by comparison with standard thermometer.
- The Calibration is determined by comparing with a known temperature from a standard resistance thermometer.
- The temperature scale in use at this laboratory is the International Temperature scale of 1990 (ITS-90).

2. Reference Standard Instrument :

Instrument	Model	Serial No.	Certificate No.	Due Date	Through
HANDHELD THERMOMETER	1521	A85997	TE 670101-01	16-Dec-24	NATIONAL FOOD INSTITUTE
Platinum Resistance Thermometer (PRT)	385	509201			

Support Equipment : - Low Temperature Bath (AMETEK RTC-187), Model: RTC-187C, S/N: 670930-00018

3. This certificate is traceable to International System of Units (SI Units).

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

6. Condition of Calibrated item : Good
7. Result of Calibration : ☒ Without adjustment ☐ After adjustment

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Report

Certificate No.: 2404042-001-01
Equipment: Digital Thermometer with RTD (pH Meter)
Resolution: 0.1 °C Model: HI2020-02
Serial No.: C0051107 ID No.: UAE.WAO.005/2557
Manufacturer: HANNA Instruments

Date of Calibration: 21 August 2024 Page 5 of 5

Calibration point: 15.0, 20.0 and 25.0 °C
Calibration result:

- The probe was immersed in liquid bath or dry bath to a minimum depth of 120 mm.
- Description of probe, model : HI11310 S/N : 539960
Dimension of probe : Diameter 12 mm., Length 120 mm.,
Sheath material : Glass

UUC* Reading	Standard Temperature (°C)	Correction Value (°C)	Uncertainty ± (°C)
15.0	14.998	0.0	0.099
20.0	19.999	0.0	0.099
25.0	24.999	0.0	0.099

Note

- UUC* : Unit Under Calibration

The report uncertainty of measurement was based on standard uncertainty multiplied by coverage factor k= 2, providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65

Calibration Certificate

Certificate No.: 2402283-002-01
Client name: UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.
Address: 3 SOI UDOMSUK 41, SUKHUMVIT ROAD,
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 4

Equipment: Electronic Balance
Manufacturer: METTLER TOLEDO
Model: XSR205DU
Serial No.: C210685394
ID No.: UAE.WAO.010/2565
Order No.: 2402283
Operation No.: 2402283-002
Date of Receipt: 2 April 2024
Date of Calibration: 2 April 2024

Calibrated by Mr.Jerawut Prapawuttipong
Scientist
Date of Issue: 9 April 2024

Approved by
(Mr.Pheraphat Tuanjit)
Manager, Division of Calibration Laboratory
Responsible for the Technical Management Team

The uncertainties are for a confidence probability of approximately 95%

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C210685394
Capacity: 220 g

Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Page 2 of 4

Date of Calibration: 2 April 2024
Environment Condition: Ambient Temperature: 24.5 ± 0.5 °C Relative Humidity: 47.5 ± 2.5 %

Place of Calibration: Laboratory, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

Condition of Equipment: Good Condition

Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1mg to 200g	B505567572	TCS	M23040535	8 April 2024
Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 016/23	Quality Reborn	QR24-0343	9 February 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

Calibration Results:


1. Repeatability of Reading:

Nominal Value (g)	Standard Deviation of Reading (g)
40	0.0000042
80	0.0000052
100	0.000048
200	0.000048

2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1 (g)	2 (g)	3 (g)	4 (g)	5 (g)	6 (g)	(Maximum Difference) (g)
100.0000	100.0001	99.9999	99.9999	100.0001	100.0000	0.0001

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C210685394
Capacity: 220 g

Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024

Page 3 of 4

Calibration Results: (Continued)

Calibration Range: 0 - 80 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 0 - 80 g ; Resolution: 0.00001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
Unload	0.000000	0.000000	0.000000	0.0000086	2.00
0.001	0.001003	0.00101	-0.00001	0.0000089	2.00
0.005	0.005003	0.00500	0.00000	0.0000092	2.00
0.01	0.010003	0.01000	0.00000	0.0000089	2.00
0.05	0.049996	0.05000	0.00000	0.0000096	2.00
0.1	0.100011	0.10000	0.00001	0.000011	2.00
0.5	0.500016	0.50001	0.00001	0.000014	2.00
1	1.000003	1.00002	-0.00002	0.000016	2.00
2	2.000023	2.00001	0.00001	0.000017	2.00
5	5.000017	5.00002	0.00000	0.000020	2.00
10	10.000009	10.00000	0.00001	0.000026	2.00
20	20.000031	20.00000	0.00003	0.000037	2.00
30	30.000040	30.00001	0.00003	0.000050	2.00
50	50.000028	50.00002	0.00001	0.000068	2.00
80	80.000068	80.00002	0.00005	0.00011	2.00

F-CS-012 Revision: 01 Date: 20-04-65



Calibration Report

Certificate No.: 2402283-002-01
Equipment: Electronic Balance
Model: XSR205DU
Serial No.: C210685394
Capacity: 220 g

Manufacturer: METTLER TOLEDO
Resolution: 0.00001 g / 0.0001 g
ID No.: UAE.WAO.010/2565

Date of Calibration: 2 April 2024

Page 4 of 4

Calibration Results: (Continued)

Calibration Range: 81 - 200 g

Calibration Adjustment: Internal Calibration

3. Departure from Nominal Value: (Range: 81 - 200 g ; Resolution: 0.0001 g)

Nominal Value (g)	Standard Value (g)	Average Reading (g)	Correction (g)	Uncertainty (± g)	Coverage Factor k
90	90.00010	90.0001	0.0000	0.00015	2.00
100	100.00006	100.0001	0.0000	0.00015	2.00
110	110.00007	110.0001	0.0000	0.00016	2.00
120	120.00009	120.0000	0.0001	0.00017	2.00
130	130.00010	130.0000	0.0001	0.00019	2.00
140	140.00014	140.0000	0.0001	0.00020	2.00
150	150.00009	150.0001	0.0000	0.00020	2.00
160	160.00010	160.0001	0.0000	0.00022	2.00
170	170.00012	170.0001	0.0000	0.00023	2.00
200	200.00016	200.0002	0.0000	0.00028	2.00

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k, providing a level of confidence of approximately 95 %.

F-CS-012 Revision: 01 Date: 20-04-65





Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2405-0166OC-2

Cert.No.: 24MM293
Page: 2 of 3

Procedure used :-

Calibration were conducted using in-house calibration procedure CP-OB01 based on UKAS LAB 14 according to direct measurement method against standard weight.

Condition of this result of calibration

1. Reference standard instruments:-

Instruments	Model	Serial No.	ID No.	Test report No.	Due date
1) Standard Weight Set (E2)	15884	24053	70RC007	MM-0013-24	25 Jan 2026

- This certificate is valid only to the item calibrated on date and place of calibration.
- This result of calibration was made on requested at the point specified by customer.
- This certificate is not certified for any commercial transaction.
- This certification is traceable to the International System of Unit.

Result of calibration () Without Adjustment (*) After Adjustment by Internal Calibration

Range capacity : 0 g to 220 g Resolution 0.0001 g

Before Adjustment :

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
100	100.0000	0.0000	0.27	2.03
200	200.0001	-0.0001	0.31	2

After Adjustment :

1. Determination of the standard deviation of weighing machine (n = 10)

Applied Weight (g)	Standard Deviation of Reading (g)
100	0.00007
200	0.00007



Equipment : Electronic Balance
Condition As-Received : Used Item
Reference : 2405-0166OC-2


Cert.No.: 24MM293
Page: 3 of 3

Result of calibration

2. Effect of off center loading

A mass of 100 g was placed to various position on the pan.
The weighing machine reading error obtained is given in the table

Position 1 (g)	Position 2 (g)	Position 3 (g)	Position 4 (g)	Position 5 (g)
+0.0002	-0.0001	0.0000	+0.0002	0.0000



Maximum difference between off-center and central loading (g)

0.0003

3. Departure from nominal value

Applied Weight (g)	Balance Reading (g)	Correction (g)	Measurement Uncertainty (± mg)	Coverage Factor (k)
Unload	0.0000	0.0000	0.15	2.13
1	1.0000	0.0000	0.15	2.13
5	5.0000	0.0000	0.15	2.13
10	10.0000	0.0000	0.15	2.11
20	20.0000	-0.0000	0.19	2.03
50	50.0001	-0.0001	0.19	2.06
60	60.0001	-0.0001	0.19	2.04
80	80.0001	-0.0001	0.27	2
100	100.0002	-0.0002	0.27	2.03
120	120.0001	-0.0001	0.29	2
200	200.0001	-0.0001	0.31	2

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor k , providing a level of confidence of approximately 95 %.

-o0o-

เอกสารไม่ควบคุม

เอกสารไม่ควบคุม