

Request No. 21-67/0517

MTC No. EEL. BP. 14/0767

CALIBRATION CERTIFICATE

Submitted by : Smile Laboratory Co.,Ltd.

Address : 563/1, Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160, Thailand.

Calibrated at : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

Instrument Calibrated :

Description : Acoustic Calibrator

Manufacturer : Quest Technologies

Model : QC-20

Serial No. : QF4090085

Ambient Environment

Temperature : $(23 \pm 3) ^\circ\text{C}$

Relative Humidity : $(50 \pm 15) \%$

Ambient Pressure : $(101.325 \pm 1.500) \text{ kPa}$

Standards used :

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N 4106495.
7. Condenser Microphone Bruel&Kjaer 4180 S/N 2633526.

Calibration Procedure: CP-102-04 based on IEC 60942-2003. The sound pressure level of instrument was measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

Date of Receipt : 8 Jul. 2024

Date of Calibration : 12 Jul. 2024

1 / 3
✓

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

Request No. 21-67/0517

MTC No. EEL. BP. 14/0767

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa , Corrected to Reference Conditions : 101.325 kPa , 23.0°C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	93.80	-0.20	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	1000.6	0.6	± 1.5	$\pm 1.0\%$

3. Total distortion

Standard Microphone Type	Measured Total distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	2.50	± 0.60	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Date of Calibration : 12 Jul. 2024

2 / 3

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0517

MTC No. EEL. BP. 14/0767

Nominal Output of Unit Under Test = 114 dB re 20 μ Pa at 1000 Hz

Acoustic Output in dB re 20 μ Pa , Corrected to Reference Conditions : 101.325 kPa , 23.0 °C and 50 %RH

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	113.74	-0.26	± 0.10	± 0.40 dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	1000.6	0.6	± 1.5	$\pm 1.0\%$

3. Total Distortion


Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Brüel&Kjaer 4180	0.50	± 0.50	$\pm 3.0\%$

Note : 1. No adjustment.

2. The calibrator pressure correction was not included.

3. The microphone volume correction was not included.

Calibrated by :

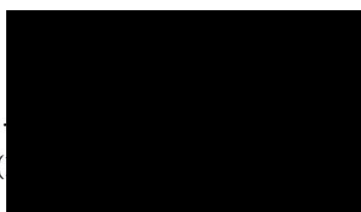

Approved by :



Electrical and Electronic Standards Laboratory
Industrial Metrology and Testing Service Centre

Date of Calibration : 12 Jul. 2024

Date of Issue : 15 Jul. 2024

Ref : 2011267070802505001

End of Certificate

3 / 3

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,
Changwat Pathumthani 12120, Thailand
Tel. (66) 0 2577 9000
Fax. (66) 0 2577 9009
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,
Amphoe Muang, Changwat Samutprakan 10280, Thailand
Tel. (66) 0 2323 1672-80 ext. 115, 116
Fax. (66) 0 2323 9165
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,
Thailand
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217
Fax. (66) 0 2579 8592
E-mail : sumalee@tistr.or.th

CERTIFICATE OF CALIBRATION

NO. 20231214051

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820384
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2023-12-14
Due Date:	2024-12-13



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-54570

3. Adjustments to indicated sound levels:

Type of Calibrator B&K 4231 SoundPressure Level 94.0 dB4. Measuring up limit: 140 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.0	-14.6	0.2	1000	0.0	0.0	-0.1
20	-50.3	-6.4	-0.4	2000	0.1	0.0	0.0
31.5	-39.4	-2.2	0.1	4000	1.3	-0.1	0.0
63	-26.1	-0.8	-0.1	8000	1.2	-0.8	0.0
125	-16.3	-0.2	-0.2	12500	-5.7	-7.2	0.1
250	-8.6	0.1	0.0	16000	-11.7	-13.4	0.2
500	-3.2	0.1	0.0	20000	-23.9	-25.8	-0.3

6. Self-generated noise

Microphone replaced by electrical input signal device

8.8 dB(A)	8.4 dB(C)	15.9 dB(Z)
-----------	-----------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.1
Rate of the S weighting decrease (dB/s)	4.4
Deviation of F&S	-0.1

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-18.1	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.4	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L _{Aeq,T}	103.2	103.2	0.0
L ₅	110.8	110.8	0.0
L ₁₀	108.8	108.8	0.0
L ₅₀	92.9	92.8	0.1
L ₉₀	76.9	76.8	0.1
L ₉₅	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2024-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2024-10-15	CIGISMEC
Signal generator	DS 360	33873	2024-10-15	CEPREI

Test specifications:

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of $\pm 20\%$.
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests

CERTIFICATE OF CALIBRATION

NO. 20231214052

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820385
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2023-12-14
Due Date:	2024-12-13

Calibrat

- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-54573

3. Adjustments to indicated sound levels:

Type of Calibrator B&K 4231 SoundPressure Level 94.0 dB4. Measuring up limit: 140 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.1	-14.6	0.2	1000	0.0	0.0	-0.1
20	-50.4	-6.4	-0.4	2000	0.1	0.0	0.0
31.5	-39.4	-2.2	0.1	4000	1.3	-0.1	0.0
63	-26.2	-0.8	-0.1	8000	1.2	-0.8	0.0
125	-16.3	-0.1	-0.2	12500	-5.7	-7.2	0.1
250	-8.5	0.2	0.0	16000	-11.7	-13.4	0.2
500	-3.2	0.1	0.0	20000	-23.9	-25.8	-0.3

6. Self-generated noise

Microphone replaced by electrical input signal device

7.3 dB(A)	11.2 dB(C)	13.3 dB(Z)
-----------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.1
Rate of the S weighting decrease (dB/s)	4.3
Deviation of F&S	-0.1

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-18.1	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.4	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S: Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L _{Aeq,T}	103.2	103.2	0.0
L ₅	110.8	110.8	0.0
L ₁₀	108.8	108.8	0.0
L ₅₀	92.9	92.8	0.1
L ₉₀	76.9	76.8	0.1
L ₉₅	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2024-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2024-10-15	CIGISMEC
Signal generator	DS 360	33873	2024-10-15	CEPREI

Test specifications:

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of $\pm 20\%$.
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests

CERTIFICATE OF CALIBRATION

NO. 20231214072

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820265
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2023-12-14
Due Date:	2024-12-13

Ca



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-54838

3. Adjustments to indicated sound levels:

Type of Calibrator B&K 4231 Sound

Pressure Level 94.0 dB

4. Measuring up limit: 140 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.1	-14.6	0.2	1000	0.0	0.0	-0.1
20	-50.3	-6.1	-0.4	2000	1.2	-0.2	0.0
31.5	-39.6	-3.1	0.1	4000	1.0	-0.8	0.0
63	-26.3	-0.9	-0.1	8000	-1.2	-3.2	0.0
125	-16.2	-0.2	-0.2	12500	-5.8	-7.8	0.1
250	-8.7	0.0	0.0	16000	-11.7	-13.7	0.0
500	-3.2	0.0	0.0	20000	-23.8	-25.8	-0.2

6. Self-generated noise

Microphone replaced by electrical input signal device

7.6 dB(A)	11.0 dB(C)	18.9 dB(Z)
-----------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.2
Rate of the S weighting decrease (dB/s)	4.4
Deviation of F&S	-0.1

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-18.1	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.4	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
L _{Aeq,T}	103.2	103.2	0.0
L ₅	110.8	110.8	0.0
L ₁₀	108.8	108.8	0.0
L ₅₀	92.9	92.8	0.1
L ₉₀	76.9	76.8	0.1
L ₉₅	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2024-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2024-10-15	CIGISMEC
Signal generator	DS 360	33873	2024-10-15	CEPREI

Test specifications:

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of $\pm 20\%$.
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests

CERTIFICATE OF CALIBRATION

NO. 20240113133

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820893
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-31
Due Date:	2025-01-29

Calibrated by:



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-58633

3. Adjustments to indicated sound levels:

Type of Calibrator B&K 4231 Sound

Pressure Level 94.0 dB

4. Measuring up limit: 140 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.2	-14.3	-0.2	1000	0.0	0.0	-0.1
20	-50.1	-6.2	-0.2	2000	1.3	-0.1	-0.1
31.5	-39.2	-2.5	-0.1	4000	1.1	-0.8	-0.1
63	-26.1	-0.2	-0.1	8000	-1.0	-3.2	0.0
125	-16.2	-0.1	0.1	12500	-11.5	-13.5	0.1
250	-8.7	0.1	-0.1	16000	-11.5	-13.3	0.1
500	-3.2	0.2	-0.1	20000	-23.9	-25.9	-0.1

6. Self-generated noise

Microphone replaced by electrical input signal device

7.0 dB(A)	8.6 dB(C)	13.8 dB(Z)
-----------	-----------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.1
Rate of the S weighting decrease (dB/s)	4.3
Deviation of F&S	-0.1

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-18.1	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.4	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
LAeq,T	103.2	103.2	0.0
L5	110.8	110.8	0.0
L10	108.8	108.8	0.0
L50	92.9	92.8	0.1
L90	76.9	76.8	0.1
L95	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2024-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2024-10-15	CIGISMEC
Signal generator	DS 360	33873	2024-10-15	CEPREI

Test specifications:

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of $\pm 20\%$.
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests

CERTIFICATE OF CALIBRATION

NO. 20240113130

Name of Product:	Sound Level Meter
Model:	ST-11D
Serial Number:	820890
Specification:	Class 1
Conclusion:	Pass
Date of calibration:	2024-01-31
Due Date:	2025-01-29

Calibrated



- I. This report certifies that all calibration equipment used in the test is traceable with the internal ISO9001 procedures and meets all specification given in the Manual(s) or respectively surpass then, and applies only to the unit identified above.
- II. This certificate is produced with advanced equipment & procedures which permit comprehensive quality assurance verification of all data supplied herein.
- III. This certificate of calibration shall not be reproduced except in full, without written permission of the Scarlet Tech Co Ltd Taiwan.

1. Preliminary inspection: OK

2. Type & serial No. of Microphone: AWA14425-57144

3. Adjustments to indicated sound levels:

Type of Calibrator B&K 4231 SoundPressure Level 94.0 dB4. Measuring up limit: 140 dBA

5. Frequency weightings (Acoustic signal tests for Z weighting, other electric signal tests.)

Equivalent Free-field Sound Level (reference environment conditions) 93.8 dB

Nominal frequency /Hz	Frequency weighting / dB			Nominal frequency /Hz	Frequency weighting / dB		
	A	C	Z		A	C	Z
10	-71.1	-14.2	-0.4	1000	0.0	0.0	-0.1
20	-50.1	-6.3	-0.1	2000	1.3	-0.1	-0.1
31.5	-39.1	-2.6	-0.1	4000	1.1	-0.9	-0.1
63	-26.1	-0.4	-0.1	8000	-1.0	-3.1	0.0
125	-16.2	-0.1	0.1	12500	-11.5	-13.5	0.1
250	-8.7	0.1	-0.1	16000	-11.5	-13.4	0.1
500	-3.1	0.1	-0.2	20000	-23.8	-25.8	-0.1

6. Self-generated noise

Microphone replaced by electrical input signal device

7.5 dB(A)	10.9 dB(C)	10.9 dB(Z)
-----------	------------	------------

7. F&S Weighting

Rate of the F weighting decrease (dB/s)	35.1
Rate of the S weighting decrease (dB/s)	4.4
Deviation of F&S	-0.1

8. Level Linearity (A-weighting at frequency 1 kHz)

Reference sound level 90.0 dB

Max error at 10dB steps upper reference sound level 0.1 dB

Max error at 1dB steps within 5dB of the upper limit linear operating range 0.0 dB

Max error at 10dB steps below reference sound level 0.1 dB

Max error at 1dB steps within 5dB upper the lower limit linear operating range 0.1 dB

9. Tone burst response (A Weighting) :

Single Toneburst duration /ms	Toneburst response /dB			
	LAFmax-LA	LASmax-LA	LAE-LA	LAeqT-LA
500	0.0	-4.0	-2.9	-7.0
200	-1.0	-7.4	-6.9	-7.0
2	-18.1	-26.9	-26.9	-7.0
0.25	-27.2	/	-36.0	-7.0

10. Peak C sound level (500Hz) :

Cycle	One cycle	nominal value	Positive half	nominal value	Negative half	nominal value
LCpeak-LC(dB)	3.5	3.5	2.4	2.4	2.3	2.4

11. Overload indication: Pass

12. Statistical analysis function

Sweep signal maximum indicated sound level: 112.8 dB

Sweep amplitude: 40 dB

Scan cycle time: 60 S; Measurement period: 180 S.

Items	Measured value/dB	Theoretical calculated value/dB	Error/dB
LAeq,T	103.2	103.2	0.0
L5	110.8	110.8	0.0
L10	108.8	108.8	0.0
L50	92.9	92.8	0.1
L90	76.9	76.8	0.1
L95	75.0	74.9	0.1

Uncertainty of measurement results: 0.4 dB (k=2)

Environment conditions:

Air temperature: 20 °C

Relative humidity: 50 %

Static pressure: 101.8 kPa

Reference equipment used in the calibration:

Description:	Model	Serial No.	Expiry Date	Traceable To
Microphone	B&K 4191	2929405	2024-12-15	NML
Multi function sound calibrator	B&K 4226	2288444	2024-10-15	CIGISMEC
Signal generator	DS 360	33873	2024-10-15	CEPREI

Test specifications:

1. All Scarlet's Sound level Meter has been calibrated in accordance with the requirements as specified in ISO 17025 and the lab calibration procedure SMTP004-CA-152.
2. The electrical tests were performed using an electrical signal substituted for the microphone which was removed and replaced by an equivalent capacitance within a tolerance of $\pm 20\%$.
3. The acoustic calibration was performed using an B&K 4226 sound calibrator and corrections was applied for the difference between the free-field and pressure responses of the Sound Level Meter.

References:

IEC 61672-3 Sound Level Meters Part 3: Periodic tests



SMILE
Laboratory Co., Ltd.

บริษัท สไมล์ แล็บอราทอรี จำกัด

Smile Laboratory Co., Ltd.

563/1 ถนนทองเอก แขวงบางกอกว่า เขตภาษีเจริญ กรุงเทพฯ 10160 โทรศัพท์ 02-227-0265 โทรสาร 02-454-0317
563/1 Thuet Thai Rd., Bangwa, Phasicharoen, Bangkok 10160 Tel. 02-227-0265 Fax. 02-454-0317

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวลอปเม้นท์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	พื้นที่โครงการ	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q _{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q _{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	TSP No.01	Motor Serial Number	1203-415	Recorder Serial Number	596
----------------	-----------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH_2O) (inH ₂ O)			(A)	(X)	(I)	(Y)	Temperature (°K = °C+273)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH_2O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication	IC = $l[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	2.2	2.1	4.30	2.05646	0.99603	36.0	35.70	303.0	760.0
2	3.2	2.9	6.10	2.44936	1.18279	43.0	42.64	303.0	760.0
3	4.1	3.8	7.90	2.78741	1.34348	50.0	49.59	303.0	760.0
4	5.4	5.3	10.70	3.24398	1.56051	55.0	54.54	303.0	760.0
5	6.3	6.2	12.50	3.50624	1.68518	60.0	59.50	303.0	760.0
Average								303.0	760.0

Linear Regression : $y = mX + b$

Slope (m)	33.768326
Intercept (b)	2.686962
R-Square (R^2)	0.990356
Correlation Coefficient (r)	0.995166

Andersen Instruments, Inc.

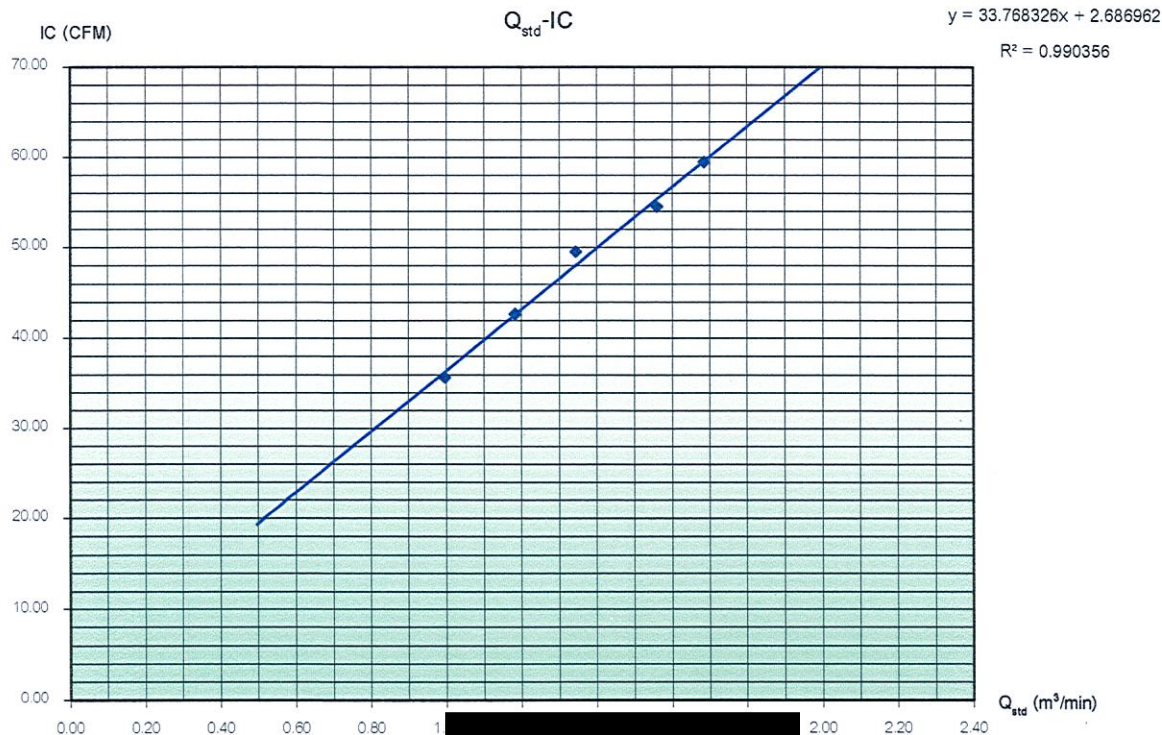

Calibrated By

SMILE
Laboratory Co., Ltd.



SMILE
Laboratory Co., Ltd.

บริษัท สไมล์ แล็บอราทอรี จำกัด

Smile Laboratory Co., Ltd.

563/1 ถนนทองเอก แขวงบางกอกใหญ่ เขตภาษีเจริญ กรุงเทพฯ 10160 โทร/โทรสาร 02-227-0265 โทรสาร 02-454-0317
563/1 Thoe Thai Rd., Bangwa, Phasicharoen, Bangkok 10160 Tel. 02-227-0265 Fax. 02-454-0317

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวลอปเม้นท์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	พื้นที่โครงการ	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q_{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q_{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	PM10 No.01	Motor Serial Number	1203-440	Recorder Serial Number	604
----------------	------------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH_2O) (inH ₂ O)			(A)	(X)	(I)	(Y)	Temperature (°K = °C+273)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH_2O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication	IC = $I[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	1.6	1.5	3.10	1.74036	0.84577	32.0	31.63	305.0	760.0
2	3.0	2.9	5.90	2.40096	1.15978	42.0	41.52	305.0	760.0
3	4.2	4.1	8.30	2.84772	1.37215	52.0	51.40	305.0	760.0
4	5.7	5.5	11.20	3.30801	1.59095	58.0	57.33	305.0	760.0
5	6.6	6.4	13.00	3.56394	1.71260	62.0	61.28	305.0	760.0
Average								305.0	760.0

Linear Regression : $y = mX + b$

Slope (m)	34.767147
Intercept (b)	2.174514
R-Square (R^2)	0.994020
Correlation Coefficient (r)	0.997006

Andersen Instruments, Inc.

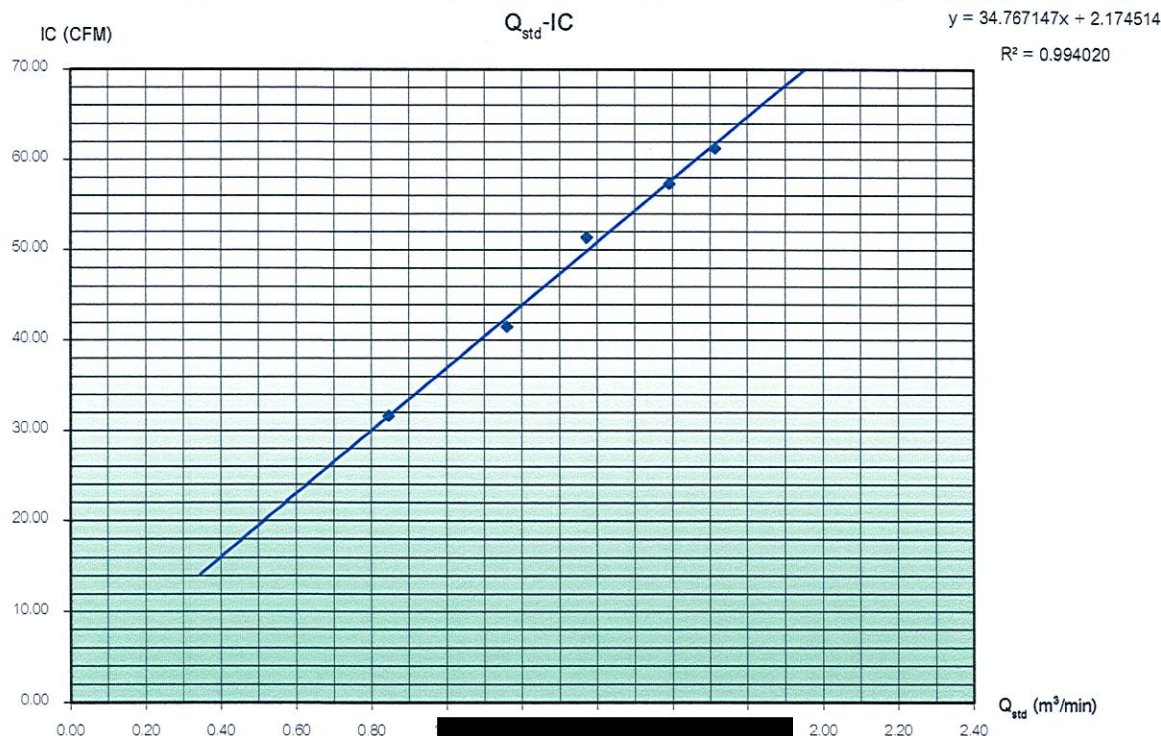

Calibrated By

SMILE
Laboratory Co., Ltd.

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวลอปเม้นท์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	สุสานไทยสมุทร (ชุมชนบ้านมาบใหญ่)	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q _{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q _{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	TSP No.03	Motor Serial Number	1203-426	Recorder Serial Number	600
----------------	-----------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH ₂ O) (inH ₂ O)			(A)	(X)	(I)	(Y)	Temperature (°K = °C+273)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH ₂ O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication	IC = $I[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	2.0	1.9	3.90	1.95848	0.94945	36.0	35.70	303.0	760.0
2	3.3	3.1	6.40	2.50886	1.21107	43.0	42.64	303.0	760.0
3	4.4	4.3	8.70	2.92514	1.40895	50.0	49.59	303.0	760.0
4	5.5	5.4	10.90	3.27416	1.57486	55.0	54.54	303.0	760.0
5	6.3	6.1	12.40	3.49219	1.67850	60.0	59.50	303.0	760.0
Average								303.0	760.0

Linear Regression : y = mX + b

Slope (m)	32.249636
Intercept (b)	4.388908
R-Square (R ²)	0.992855
Correlation Coefficient (r)	0.996421

Andersen Instruments, Inc.

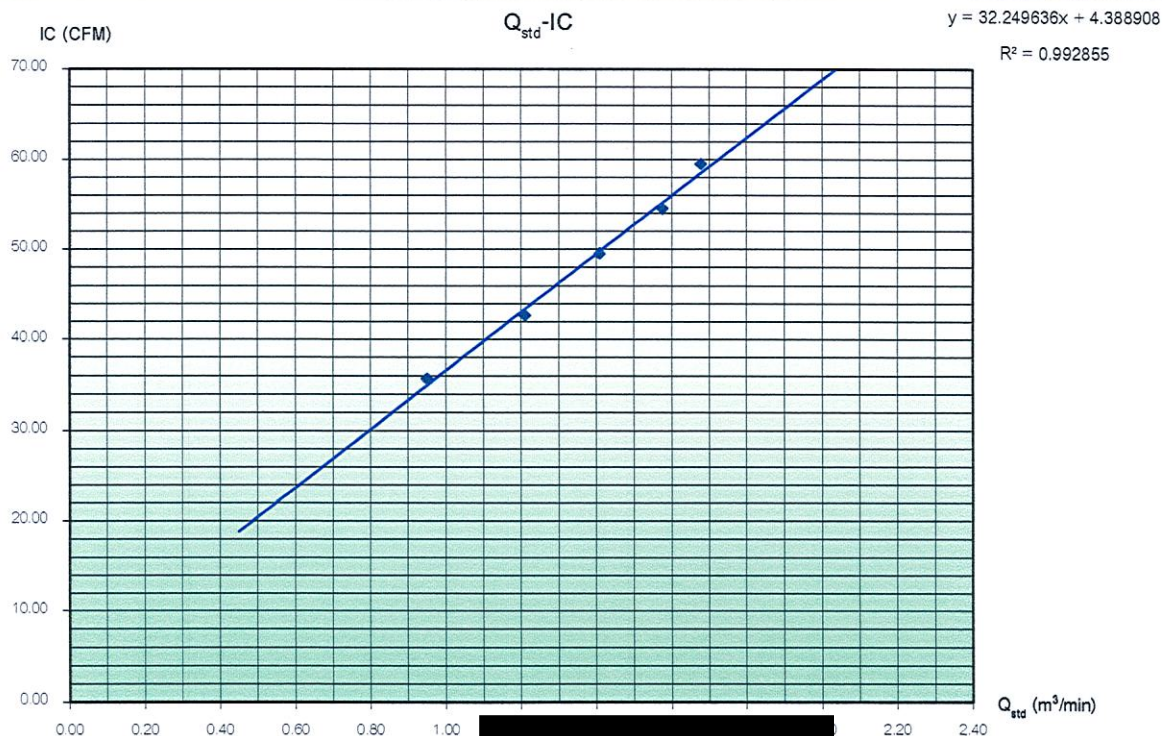

Calibrated By

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวล๊อปเมนต์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	สุสานไทยสมุทร (ชุมชนบ้านนาใหญ่)	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q _{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q _{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	PM10 No.03	Motor Serial Number	1203-449	Recorder Serial Number	608
----------------	------------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH ₂ O) (inH ₂ O)			(A)	(X)	(I)	(Y)	Temperature (°K = °C+273)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH ₂ O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication	IC = $I[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	1.8	1.7	3.50	1.84924	0.89752	32.0	31.63	305.0	760.0
2	2.9	2.7	5.60	2.33912	1.13039	42.0	41.52	305.0	760.0
3	4.2	4.1	8.30	2.84772	1.37215	52.0	51.40	305.0	760.0
4	5.8	5.6	11.40	3.33742	1.60493	58.0	57.33	305.0	760.0
5	6.5	6.4	12.90	3.55020	1.70607	62.0	61.28	305.0	760.0
Average								305.0	760.0

Linear Regression : y = mX + b

Slope (m)	36.049868
Intercept (b)	0.245557
R-Square (R ²)	0.991639
Correlation Coefficient (r)	0.995811

Andersen Instruments, Inc.

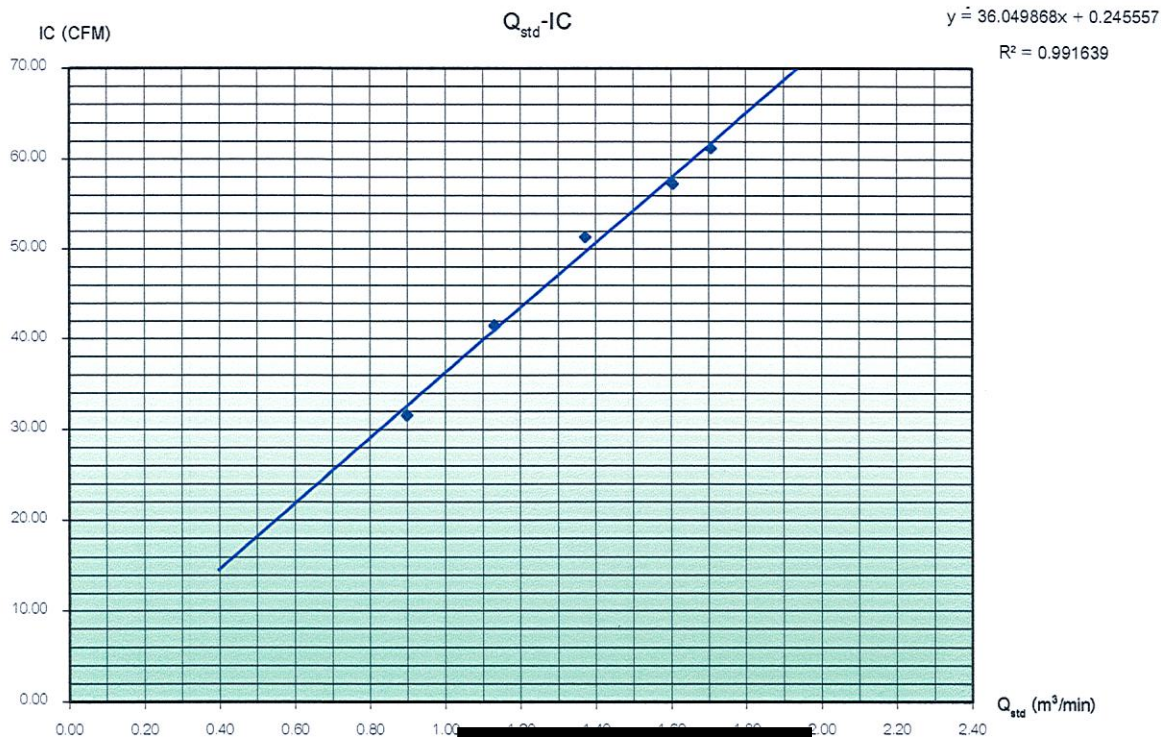

Calibrated By



SMILE
Laboratory Co., Ltd.

บริษัท สไมล์ แล็บอราทอรี จำกัด

Smile Laboratory Co., Ltd.

563/1 ถนนทองหล่อ แขวงบางหว้า เขตภาษีเจริญ กรุงเทพฯ 10160 โทรศัพท์ 02-227-0265 โทรสาร 02-454-0317
563/1 Thoe Thai Rd., Bangwa, Phasicharoen, Bangkok 10160 Tel. 02-227-0265 Fax. 02-454-0317

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวลอปเม้นท์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	ศาลเจ้าข้าไทจื้อ	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q_{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q_{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	TSP No.02	Motor Serial Number	1203-421	Recorder Serial Number	598
----------------	-----------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH_2O) (in H_2O)			(A)	(X)	(I)	(Y)	Temperature ($^{\circ}K = ^{\circ}C + 273$)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH_2O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m^3/min)	Sample Flow Rate Indication	$IC = I[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	2.2	2.1	4.30	2.05646	0.99603	36.0	35.70	303.0	760.0
2	3.1	3.0	6.10	2.44936	1.18279	43.0	42.64	303.0	760.0
3	4.3	4.2	8.50	2.89132	1.39288	50.0	49.59	303.0	760.0
4	5.2	5.1	10.30	3.18277	1.53142	55.0	54.54	303.0	760.0
5	6.1	6.0	12.10	3.44969	1.65829	60.0	59.50	303.0	760.0
Average								303.0	760.0

Linear Regression : $y = mX + b$

Slope (m)	35.494588
Intercept (b)	0.397050
R-Square (R^2)	0.999329
Correlation Coefficient (r)	0.999664

Andersen Instruments, Inc.

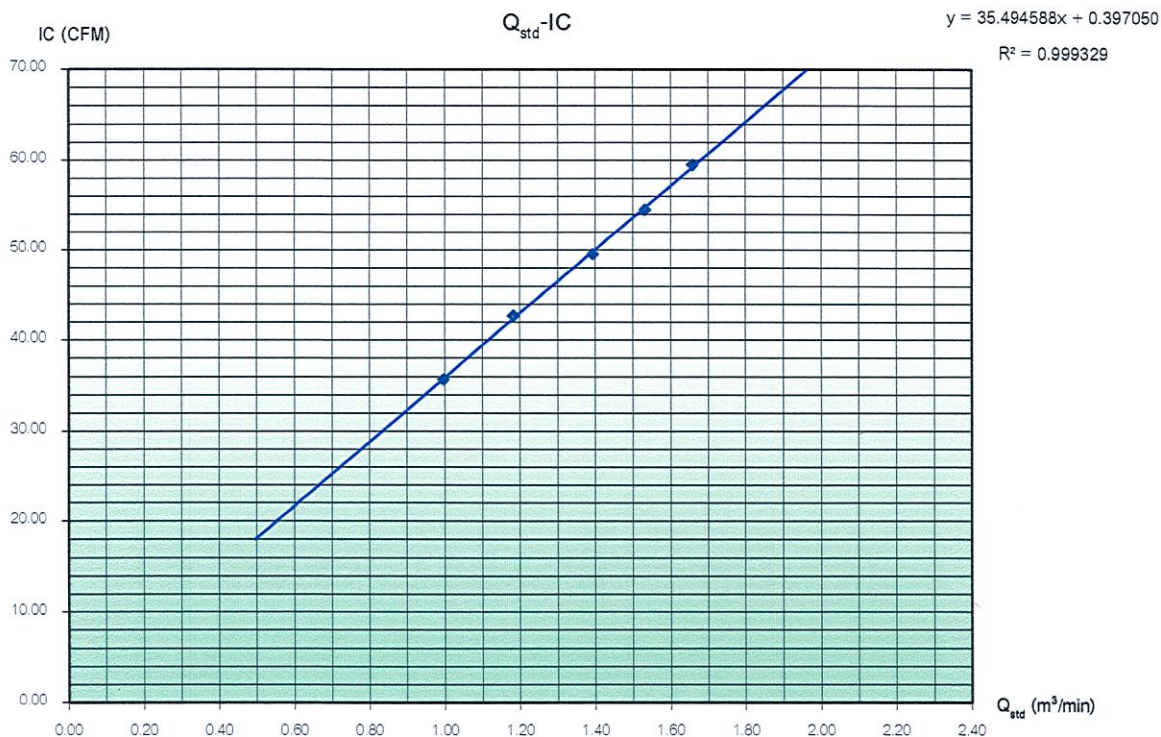

Calibrated By

SMILE
Laboratory Co., Ltd.



SMILE
Laboratory Co., Ltd.

บริษัท สไมล์ แล็บอราทอรี จำกัด

Smile Laboratory Co., Ltd.

563/1 ถนนเทวโลก แขวงบางหว้า เขตภาษีเจริญ กรุงเทพฯ 10160 โทรศัพท์ 02-227-0265 โทรสาร 02-454-0317
563/1 Thoe Thai Rd., Bangwa, Phasicharoen, Bangkok 10160 Tel. 02-227-0265 Fax. 02-454-0317

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวลอปเม้นท์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	ศาลเจ้าข่าไทรงิ้ว	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q_{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q_{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	PM10 No.02	Motor Serial Number	1203-444	Recorder Serial Number	606
----------------	------------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH_2O) (in H_2O)			(A)	(X)	(I)	(Y)	Temperature ($^{\circ}K = ^{\circ}C + 273$)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH_2O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m^3/min)	Sample Flow Rate Indication	IC = $I[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	1.7	1.6	3.30	1.79562	0.87204	32.0	31.63	305.0	760.0
2	3.0	2.9	5.90	2.40096	1.15978	42.0	41.52	305.0	760.0
3	4.4	4.3	8.70	2.91553	1.40438	52.0	51.40	305.0	760.0
4	5.7	5.5	11.20	3.30801	1.59095	58.0	57.33	305.0	760.0
5	6.6	6.4	13.00	3.56394	1.71260	62.0	61.28	305.0	760.0
Average								305.0	760.0

Linear Regression : $y = mX + b$

Slope (m)	35.689774
Intercept (b)	0.524055
R-Square (R^2)	0.998524
Correlation Coefficient (r)	0.999262

Andersen Instruments, Inc.

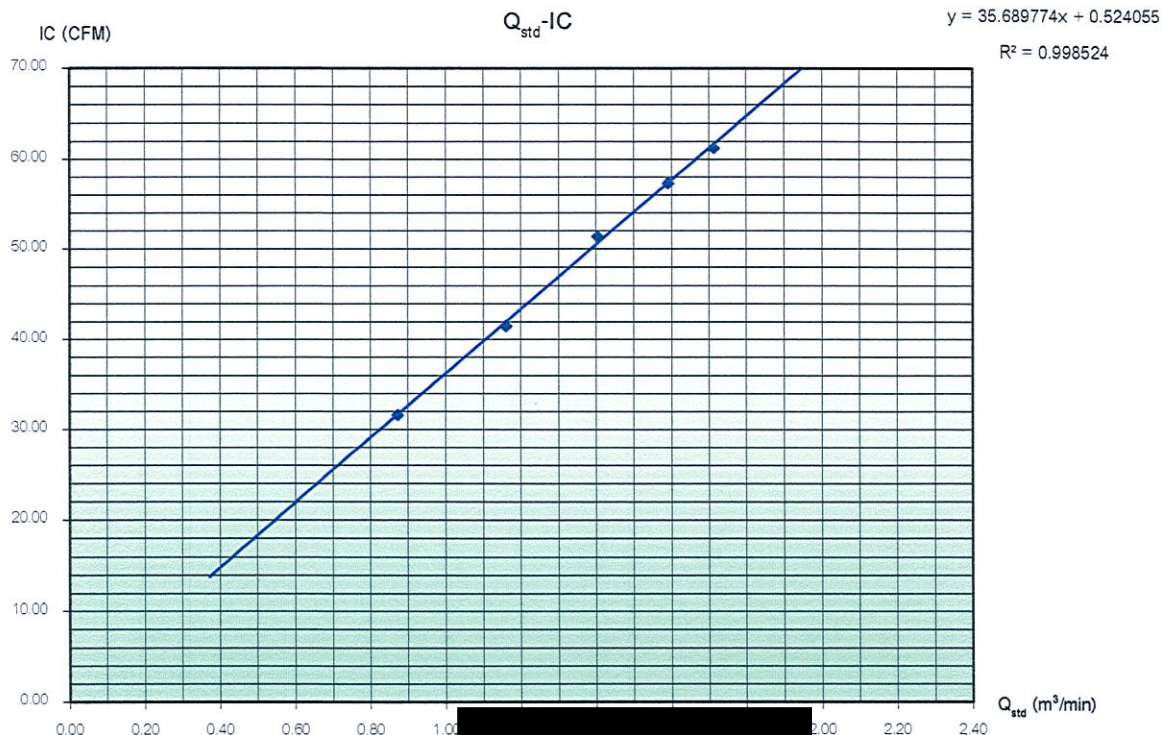

Calibrated By

SMILE
Laboratory Co., Ltd.



SMILE
Laboratory Co., Ltd.

บริษัท สไมล์ แล็บอราทอรี จำกัด

Smile Laboratory Co., Ltd.

563/1 ถนนพหลโยธิน แขวงบางหว้า เขตภาษีเจริญ กรุงเทพฯ 10160 โทรศัพท์ 02-227-0265 โทรสาร 02-454-0317
563/1 Thoe Thai Rd., Bangwa, Phasicharoen, Bangkok 10160 Tel. 02-227-0265 Fax. 02-454-0317

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวลอปเม้นท์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	สุสานสุขสันต์สุขาวดี	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q _{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q _{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	TSP No.05	Motor Serial Number	1203-422	Recorder Serial Number	599
----------------	-----------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH ₂ O) (inH ₂ O)			(A)	(X)	(I)	(Y)	Temperature (°K = °C+273)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH ₂ O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$	Sample Flow Rate Indication	IC = $I[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	2.2	2.1	4.30	2.05646	0.99603	36.0	35.70	303.0	760.0
2	3.1	3.0	6.10	2.44936	1.18279	43.0	42.64	303.0	760.0
3	4.3	4.2	8.50	2.89132	1.39288	50.0	49.59	303.0	760.0
4	5.2	5.1	10.30	3.18277	1.53142	55.0	54.54	303.0	760.0
5	6.1	6.0	12.10	3.44969	1.65829	60.0	59.50	303.0	760.0
Average								303.0	760.0

Linear Regression : y = mX + b

Slope (m)	35.494588
Intercept (b)	0.397050
R-Square (R ²)	0.999329
Correlation Coefficient (r)	0.999664

Andersen Instruments, Inc.

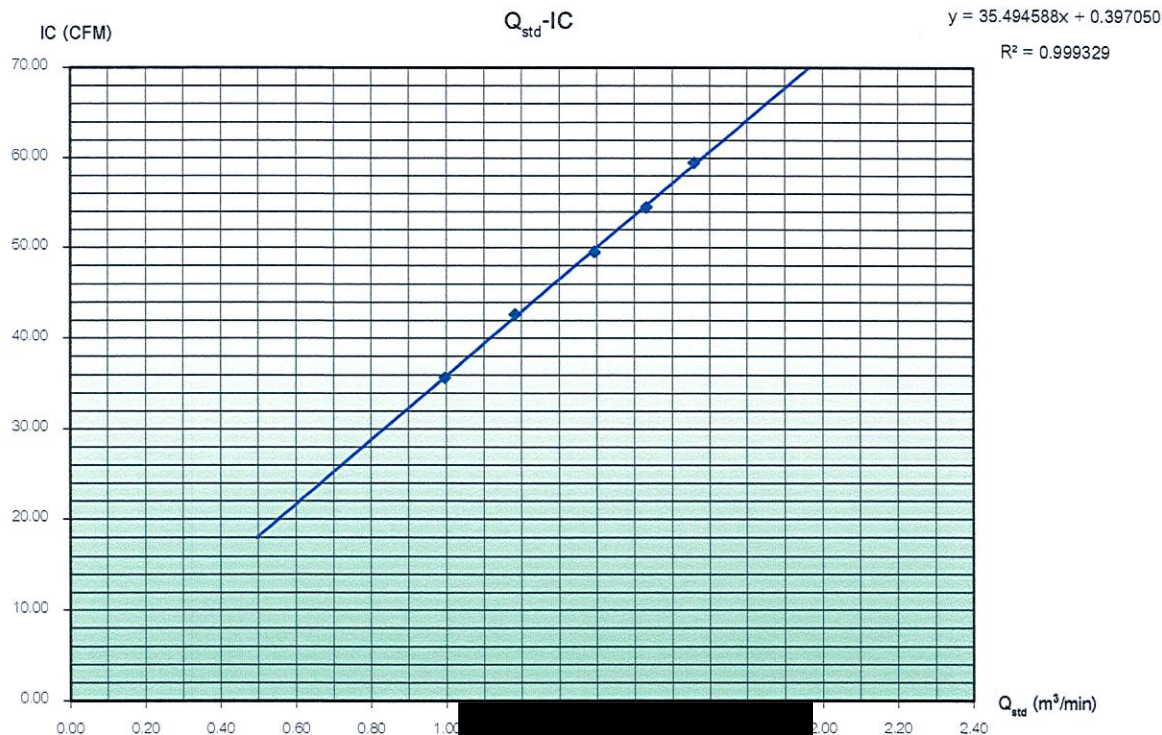

Calibrated By

SMILE
Laboratory Co., Ltd.



บริษัท สไมล์ แล็บอราทอรี จำกัด
Smile Laboratory Co., Ltd.

563/1 ถนนทองหล่อ แขวงบางนา เขตภาษีเจริญ กรุงเทพฯ 10160 โทรศัพท์ 02-227-0265 โทรสาร 02-454-0317
563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok 10160 Tel. 02-227-0265 Fax. 02-454-0317

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวลอปเม้นท์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	สุสานสุขสันต์สุขาวดี	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q _{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q _{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	PM10 No.05	Motor Serial Number	1203-447	Recorder Serial Number	605
----------------	------------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH ₂ O) (inH ₂ O)			(A)	(X)	(I)	(Y)	Temperature (°K = °C+273)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH ₂ O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication	IC = $I[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	1.6	1.5	3.10	1.74036	0.84577	32.0	31.63	305.0	760.0
2	3.0	2.9	5.90	2.40096	1.15978	42.0	41.52	305.0	760.0
3	4.2	4.1	8.30	2.84772	1.37215	52.0	51.40	305.0	760.0
4	5.7	5.5	11.20	3.30801	1.59095	58.0	57.33	305.0	760.0
5	6.6	6.4	13.00	3.56394	1.71260	62.0	61.28	305.0	760.0
Average								305.0	760.0

Linear Regression : y = mX + b

Slope (m)	34.767147
Intercept (b)	2.174514
R-Square (R ²)	0.994020
Correlation Coefficient (r)	0.997006

Andersen Instruments, Inc.

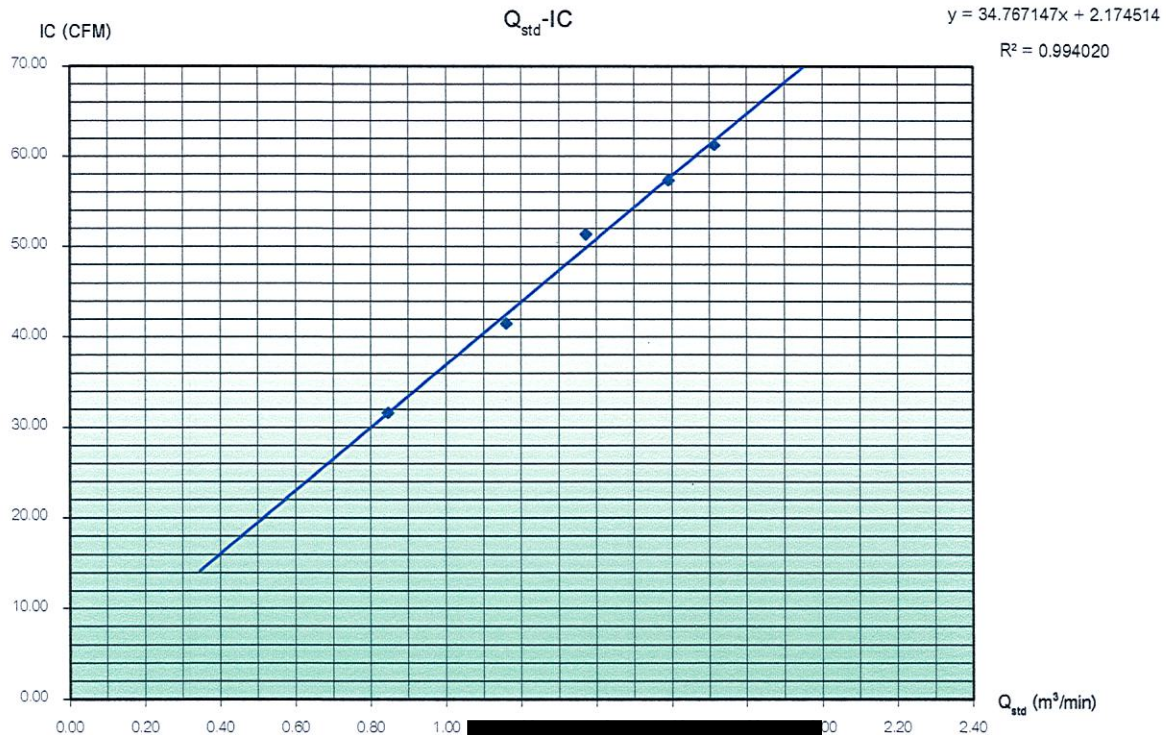

Calibrated By

SMILE
Laboratory Co., Ltd.

TSP HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวลอปเม้นท์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	บ้านราษฎรที่ใกล้เคียง พื้นที่ทิศตะวันตก	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q _{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q _{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	TSP No.04	Motor Serial Number	1203-432	Recorder Serial Number	602
----------------	-----------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH ₂ O) (inH ₂ O)			(A)	(X)	(I)	(Y)	Temperature (°K = °C+273)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH ₂ O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication	IC = $I[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	1.9	1.9	3.80	1.93321	0.93744	36.0	35.70	303.0	760.0
2	3.3	3.2	6.50	2.52839	1.22036	43.0	42.64	303.0	760.0
3	4.4	4.2	8.60	2.90828	1.40094	50.0	49.59	303.0	760.0
4	5.2	5.1	10.30	3.18277	1.53142	55.0	54.54	303.0	760.0
5	6.4	6.2	12.60	3.52024	1.69183	60.0	59.50	303.0	760.0
Average								303.0	760.0

Linear Regression : y = mX + b

Slope (m)	32.301714
Intercept (b)	4.581780
R-Square (R ²)	0.991793
Correlation Coefficient (r)	0.995888

Andersen Instruments, Inc.

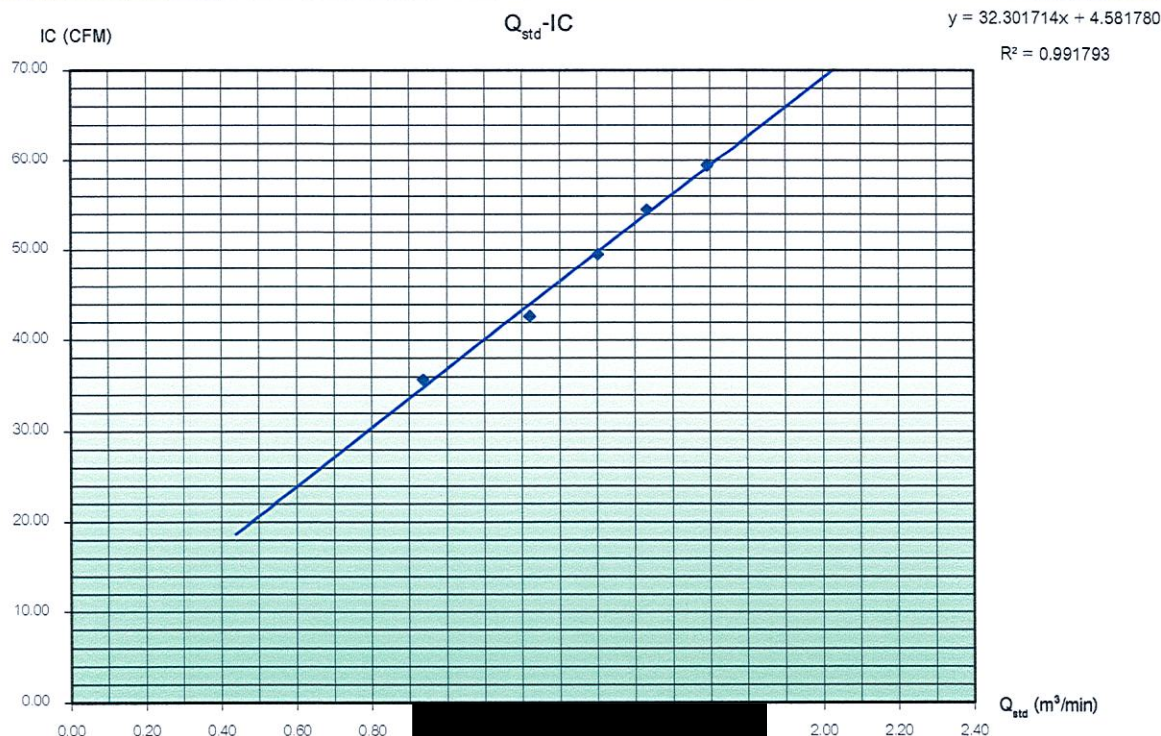

Calibrated By



SMILE
Laboratory Co., Ltd.

บริษัท สไมล์ แล็บอราทอรี จำกัด

Smile Laboratory Co., Ltd.

563/1 ถนนเทวโลก แขวงบางหว้า เขตภาษีเจริญ กรุงเทพฯ 10160 โทรศัพท์ 02-227-0265 โทรสาร 02-454-0317
563/1 Thoet Thal Rd., Bangwa, Phasicharoen, Bangkok 10160 Tel. 02-227-0265 Fax. 02-454-0317

PM10 HIGH VOLUME AIR SAMPLER CALIBRATION REPORT

Site Information

Sampler Location	บริษัท อิตาเลียนไทย ดีเวลอปเม้นท์ จำกัด (มหาชน)	Date	08 September 2024
Project Site	บ้านราษฎรทีใกล้เคียง พื้นที่ทิศตะวันตก	Person	Mr. Jakkreewat Chaichana

Calibration Orifice

Transfer Standard Type	Orifice	Q _{std} Slope (m)	2.10372
Calibrator Model	TE-5025A	Q _{std} Intercept (b)	-0.03890
Calibrator Serial Number	3092		

Calibration Information


Sampler Number	PM10 No.04	Motor Serial Number	1203-453	Recorder Serial Number	610
----------------	------------	---------------------	----------	------------------------	-----

Test No.	Pressure Drop Across Orifice (ΔH ₂ O) (inH ₂ O)			(A)	(X)	(I)	(Y)	Temperature (°K = °C+273)	Barometric Pressure (mmHg)
	Positive	Negative	ΔH ₂ O	$[\Delta H_2O(P_a/P_{std})(T_{std}/T_a)]^{1/2}$	$Q_{std} = (1/m)[(A-b)]$ (m ³ /min)	Sample Flow Rate Indication	IC = $I[(P_a/P_{std})(T_{std}/T_a)]^{1/2}$		
1	1.9	1.8	3.70	1.90134	0.92229	32.0	31.63	305.0	760.0
2	3.1	3.0	6.10	2.44131	1.17896	42.0	41.52	305.0	760.0
3	4.2	4.0	8.20	2.83051	1.36397	52.0	51.40	305.0	760.0
4	5.7	5.5	11.20	3.30801	1.59095	58.0	57.33	305.0	760.0
5	6.1	6.0	12.10	3.43836	1.65291	62.0	61.28	305.0	760.0
Average								305.0	760.0

Linear Regression : y = mX + b

Slope (m)	39.949045
Intercept (b)	4.972153
R-Square (R ²)	0.990397
Correlation Coefficient (r)	0.995187

Andersen Instruments, Inc.

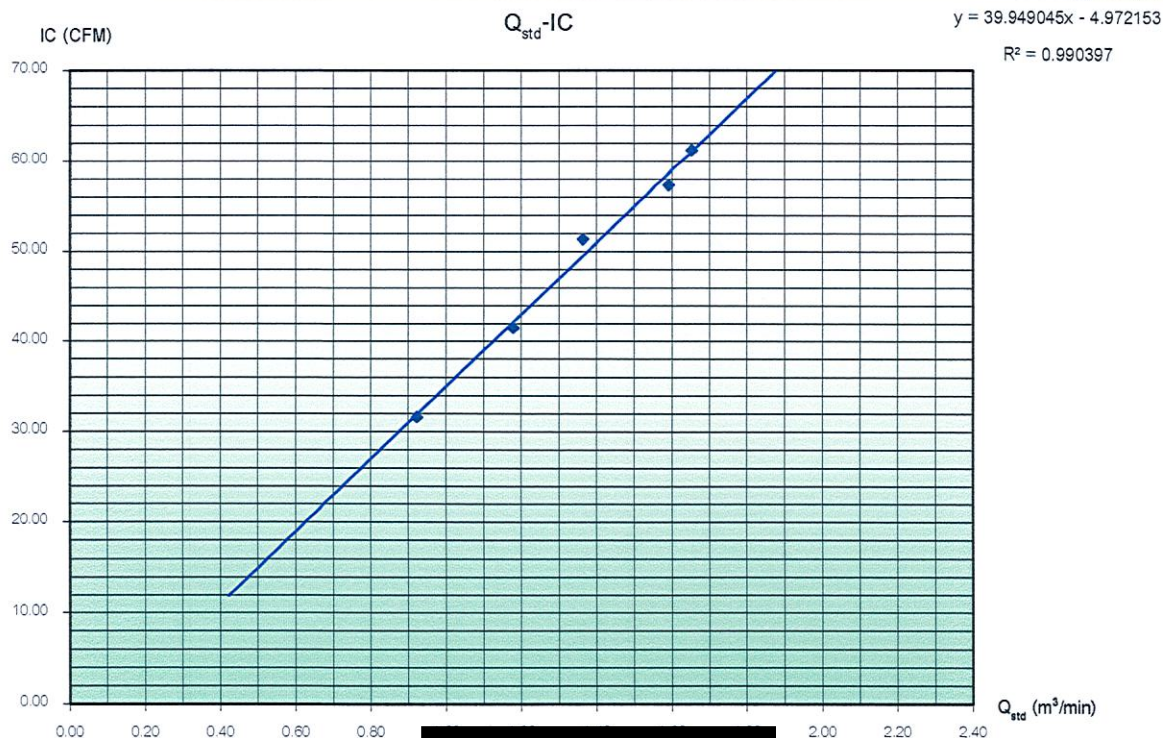

Calibrated By

SMILE
Laboratory Co., Ltd.

Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 21 January 2024

Certificate No. 123/21

Page : 1 of 2

Manufacture Yong Instruments

Type four blade helicoid propeller

Model No. 05103

Mfg Code Logger 30908233

Transmitter -

Customer ENVIR SERVICE CO., LTD.

42 Raminthra 14 yeak 9, Tha Raeng,

Bangkhen, Bangkok 10230

Calibration Condition : Temperature 25.2 °C

Barometric Pressure 1012.8 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)


JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER : Theodor Friedrich : Dry No. 8390/94 Wet No. 8389/94

: Thermoschneider No. 918802

STANDARD BAROMETER : Digital Barometer Vaisala Type RTB220 No. V1220015

Calibrated by



The Result of Calibration

Date of Issue 21 January 2024


Certificate No. 123/21

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO 1425			TESTED ANEMOMETER			
	Pressure inches	Vacuum inches	Pressure hPa	Pressure hPa	Correction hPa	Velocity m/sec	Correction m/sec
1.00	-	-	-	-	-	0.7	0.30
3.02	-	-	-	-	-	2.7	0.32
5.04	-	-	-	-	-	4.7	0.34
7.03	-	-	-	-	-	6.7	0.33
9.01	-	-	-	-	-	8.5	0.51
11.03	-	-	-	-	-	10.7	0.33
13.01	-	-	-	-	-	12.4	0.61
15.03	-	-	-	-	-	14.1	0.93
17.05	-	-	-	-	-	16.4	0.65
20.02	-	-	-	-	-	19.1	0.92

Wind Aloft Plotting Board. US. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated



Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 21 January 2024

Certificate No. 124/21

Page : 1 of 2

Manufacture Yong Instruments

Type four blade helicoid propeller

Model No. 05103

Mfg Code Logger 30908695

Transmitter -

Customer ENVIR SERVICE CO., LTD.

42 Raminthra 14 yeak 9, Tha Raeng,

Bangkhen, Bangkok 10230

Calibration Condition : Temperature 25.2 °C

Barometric Pressure 1012.8 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)


JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER : Theodor Friedrich : Dry No. 8390/94 Wet No. 8389/94

: Thermoschneider No. 918802

STANDARD BAROMETER : Digital Barometer Vaisala Type RTB220 No. V1220015

Calibrated by



The Result of Calibration

Date of Issue 21 January 2024


Certificate No. 124/21

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO 1425			TESTED ANEMOMETER			
	Pressure inches	Vacuum inches	Pressure hPa	Pressure hPa	Correction hPa	Velocity m/sec	Correction m/sec
1.00	-	-	-	-	-	0.7	0.30
3.02	-	-	-	-	-	2.7	0.32
5.04	-	-	-	-	-	4.7	0.34
7.03	-	-	-	-	-	6.7	0.33
9.01	-	-	-	-	-	8.5	0.51
11.03	-	-	-	-	-	10.7	0.33
13.01	-	-	-	-	-	12.4	0.61
15.03	-	-	-	-	-	14.1	0.93
17.05	-	-	-	-	-	16.4	0.65
20.02	-	-	-	-	-	19.1	0.92

Wind Aloft Plotting Board. US. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by



Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 21 January 2024

Certificate No. 122/21

Page : 1 of 2

Manufacture Yong Instruments

Type four blade helicoid propeller

Model No. 05103

Mfg Code Logger 30908794

Transmitter -

Customer ENVIR SERVICE CO., LTD.

42 Raminthra 14 yeak 9, Tha Raeng,

Bangkhen, Bangkok 10230

Calibration Condition : Temperature 25.2 °C

Barometric Pressure 1012.8 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)


JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER : Theodor Friedrich : Dry No. 8390/94 Wet No. 8389/94

: Thermoschneider No. 918802

STANDARD BAROMETER : Digital Barometer Vaisala Type RTB220 No. V1220015

Calibrated by :



The Result of Calibration

Date of Issue 21 January 2024


Certificate No. 122/21

Page : 2 of 2

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO 1425			TESTED ANEMOMETER			
	Pressure inches	Vacuum inches	Pressure hPa	Pressure hPa	Correction hPa	Velocity m/sec	Correction m/sec
1.00	-	-	-	-	-	0.7	0.30
3.02	-	-	-	-	-	2.7	0.32
5.04	-	-	-	-	-	4.5	0.54
7.03	-	-	-	-	-	6.7	0.33
9.01	-	-	-	-	-	8.5	0.51
11.03	-	-	-	-	-	10.7	0.33
13.01	-	-	-	-	-	12.4	0.61
15.03	-	-	-	-	-	14.1	0.93
17.05	-	-	-	-	-	16.4	0.65
20.02	-	-	-	-	-	19.1	0.92

Wind Aloft Plotting Board. US. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :



Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 11 May 2024

Certificate No. 114/21

Page : 1 of 2

Manufacture Yong Instruments

Type four blade helicoid propeller

Model No. 05103

Mfg Code Logger 309020206

Transmitter -

Customer ENVIR SERVICE CO., LTD.

42 Raminthra 14 yeak 9, Tha Raeng,

Bangkhen, Bangkok 10230

Calibration Condition : Temperature

25.2 °C

Barometric Pressure

1012.8 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425

: Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV

(sensor TR-90AH)

Serial Number 110730029

(sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER


: Theodor Friedrich : Dry No. 8390/94 Wet No. 8389/94

: Thermoschneider No. 918802

STANDARD BAROMETER

: Digital Barometer Vaisala Type RTB220 No. V1220015

Calibrated by



The Result of Calibration

Date of Issue 11 May 2024


Certificate No. 114/21

Page : 2 of 2

Standard	HOOK GAGE NO 1425			TESTED ANEMOMETER			
	Pressure	Vacuum	Pressure	Pressure	Correction	Velocity	Correction
Ultrasonic							
Anemometer m/sec	inches			hPa	hPa	m/sec	m/sec
1.00	-	-	-	-	-	0.7	0.30
3.02	-	-	-	-	-	2.7	0.32
5.04	-	-	-	-	-	4.8	0.24
7.03	-	-	-	-	-	6.7	0.33
9.01	-	-	-	-	-	8.7	0.31
11.03	-	-	-	-	-	10.7	0.33
13.01	-	-	-	-	-	12.4	0.61
15.03	-	-	-	-	-	14.1	0.93
17.05	-	-	-	-	-	16.4	0.65
20.02	-	-	-	-	-	19.1	0.92

Wind Aloft Plotting Board.	
US. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by



Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 11 May 2024

Certificate No. 241/21

Page : 1 of 2

Manufacture NRG Instruments

Type 3 Cup Anemometer

Model No. 40C

Mfg Code Logger 309012581

Transmitter -

Customer ENVIR SERVICE CO., LTD.

42 Raminthra 14 yeak 9, Tha Raeng,

Bangkhen, Bangkok 10230

Calibration Condition : Temperature 25.2 °C Barometric Pressure 1012.8 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425 : Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Ultrasonic Anemometer Model DA-650-3TV (sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)


JAPAN QUALITY ASSURANCE ORGANIZATION

STANDARD THERMOMETER : Theodor Friedrich : Dry No. 8390/94 Wet No. 8389/94

: Thermoschneider No. 918802

STANDARD BAROMETER : Digital Barometer Vaisala Type RTB220 No. V1220015

Calibrated



The Result of Calibration

Date of Issue 11 May 2024


Certificate No. 241/21

Page : 2 of 2

Standard	HOOK GAGE NO 1425			TESTED ANEMOMETER			
	Pressure	Vacuum	Pressure	Pressure	Correction	Velocity	Correction
Ultrasonic							
Anemometer m/sec	inches	inches	hPa	hPa	hPa	m/sec	m/sec
1.00	-	-	-	-	-	0.9	0.10
3.02	-	-	-	-	-	2.9	0.12
5.04	-	-	-	-	-	4.8	0.24
7.03	-	-	-	-	-	6.9	0.13
9.01	-	-	-	-	-	8.7	0.31
11.03	-	-	-	-	-	10.7	0.33
13.01	-	-	-	-	-	12.5	0.51
15.03	-	-	-	-	-	14.1	0.93
17.05	-	-	-	-	-	16.4	0.65
20.02	-	-	-	-	-	19.1	0.92

Wind Aloft Plotting Board.	
US. DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRECTION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :



Calibration Certificate

Part Number: 721A2601

Description: Micromate with DIN Geophone

Serial Number: UM22200

Calibration Date: **NOV 17 2023**

Calibration Reference Equipment: 714J7402

Instantel certifies that the above product was calibrated in accordance with the applicable Instantel procedures. These procedures are part of a quality system that is designed to assure that the product listed above meets or exceeds Instantel specifications.

Instantel further certifies that the measurement instruments used during the calibration of this product are traceable to the National Institute of Standards and Technology; or National Research Council of Canada. Evidence of traceability is on file at Instantel and is available upon request.

The environment in which this product was calibrated is maintained within the operating specifications of the instrument.

Please note that the sensor check function is intended to check that the sensors are connected to the unit, installed in the proper orientation and sufficiently level to operate properly. This function should not be confused with a formal calibration, which requires the sensors be checked against a reference that is traceable to a known standard. Instantel recommends that products be returned to Instantel or an authorized service and calibration facility for annual calibration.







Calibrated By: _____



Instantel®

309 Legget Drive, Ottawa, Ontario, K2K 3A3, (613) 592-4642

Frequency Response of UM22200

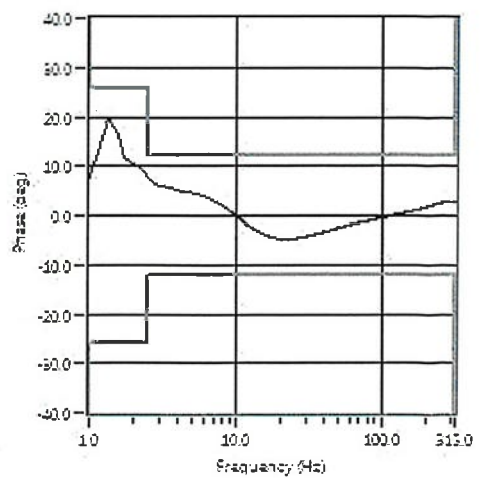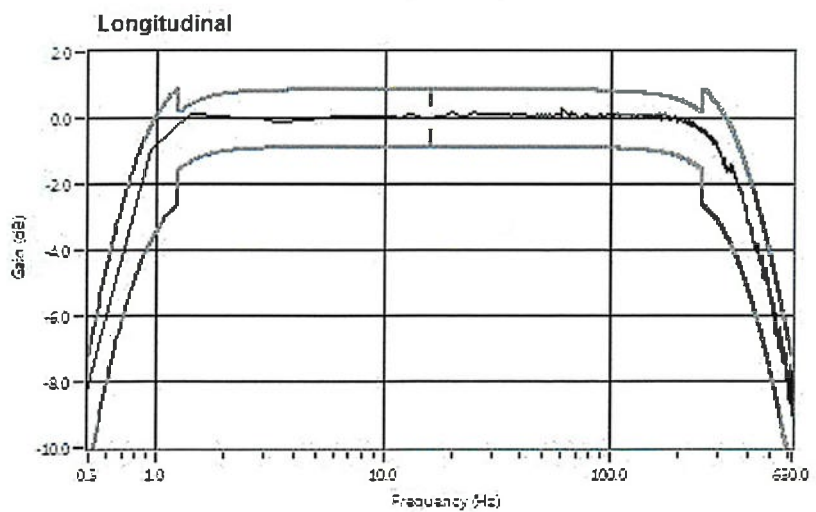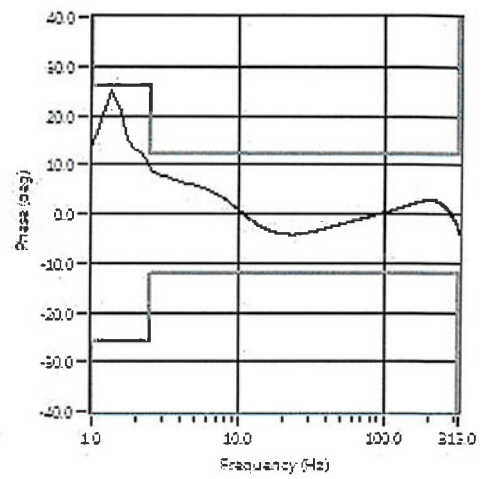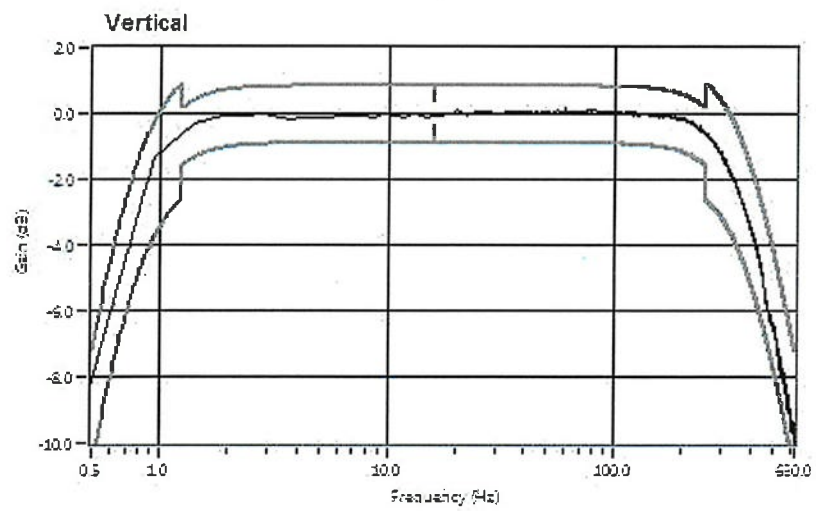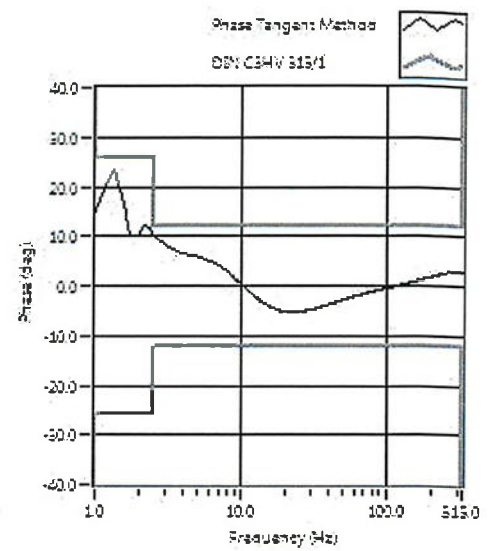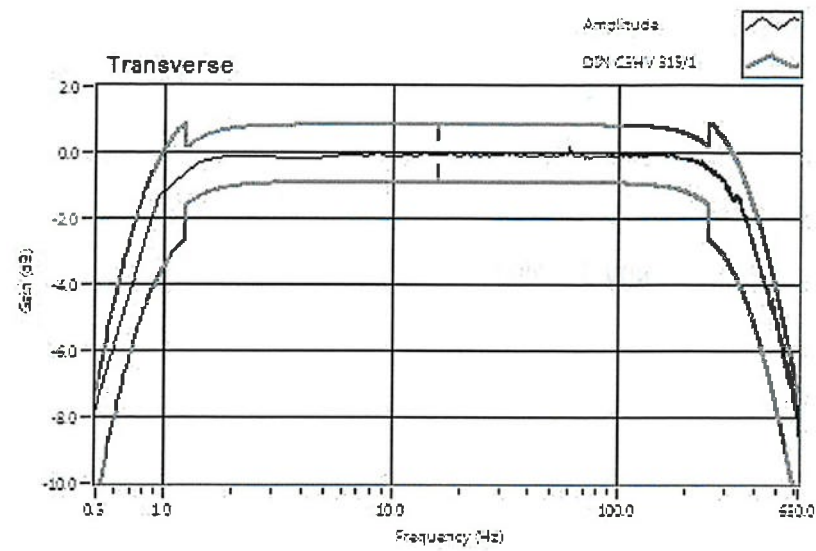

**Inctech Metrological Center Co.Ltd.**39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,
Saimai, Bangkok 10220, ThailandTel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.comCalibration Cert. # 3884.01
ISO/IEC 17025

Certificate of Calibration

Certificate No. : MT23-6059

Page : 1 of 2

Customer : Smile Laboratory Co.,Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160

Description : Digital Thermometer

Manufacturer : Fluke

Model : 51II

Serial No. : 36650190WS

Identification No. : SML.DT001/61

Calibration Place : Temperature Laboratory

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 06, 2023

Environment Condition :

Temperature : (23+/-3) °C

Humidity : (50+/-15) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-001* According to comparison with Standard Digital Thermometer with 2 PRT.
The calibration methods based on ITS-90.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Standard Digital Thermometer with 2 PRT	1586A/5609/5609	41130006/00543/03713	TE23-0007	Jan 13, 2024

This result of calibration was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through
National Institute of Metrology Thailand (NIMT)

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$,
providing a level of confidence of not less than 95%



Calibrated by : _____

Issue date : _____

Approved by : _____

This calibration certificate shall not be reproduced other than in full except with the prior written
approval of Inctech Metrological Center Co.,Ltd

**Inctech Metrological Center Co.Ltd.**39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,
Saimai, Bangkok 10220, ThailandTel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.comCalibration Cert. # 3884.01
ISO/IEC 17025**Certificate No. : MT23-6059****Page : 2 of 2**

Result : Without Adjustment
Function : Temperature measurement
Sensor Type : Thermocouple type K (wire)
Diameter : - mm
Calibration point : 4, 20, 104, 150, 180 °C

Resolution : 0.1 °C

Immersion depth (mm)	Calibration point (°C)	Standard reading (°C)	UUC* reading (°C)	UUC* correction (°C)	Uncertainty of measurement (+/- °C)
140	4	4.053	4.2	-0.147	0.24
140	20	20.025	20.2	-0.175	0.24
140	104	104.075	103.7	0.375	0.47
140	150	150.061	149.6	0.461	0.47
140	180	180.036	179.6	0.436	0.47
140	4	4.044	4.2	-0.156	0.24

UUC* = Unit under calibration



Inctech Metrological Center Co.Ltd.

39/1 Soi 82, Sukhapiaban 5 Rd., O ngoen,
Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com



Calibration Cert. # 3884.01
ISO/IEC 17025

Certificate of Calibration

Certificate No. : MT23-6082

Page : 1 of 2

Customer : Smile Laboratory Co.,Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160

Description : Digital Thermo & Hygrometer

Manufacturer : Genec

Model : ETTH2000-TH

Serial No. : H2000BC271

Identification No. : SML.TH001/61

Calibration Place : Temperature & Humidity Laboratory

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 06, 2023

Environment Condition :

Temperature : (23+/-3) °C

Humidity : (50+/-15) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-007* According to comparison with Standard Temperature & Humidity into Environmental Stability Chamber.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Standard Digital Hygrometer	One-TH	0x0000158D000E121E	SG-H-00987/65	Nov 10, 2023
Standard Digital Thermometer with Probe	UM RTD	2002Z A21 0181A	MT23-4665	Jul 14, 2024

This result of calibration was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through
National Institute of Metrology Thailand (NIMT)

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$,
providing a level of confidence of not less than 95%



Calibrated by
Issue date

Approved by :

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd



Result : Without adjustment
Function : Temperature measurement
Calibration point : 25 °C
Resolution : 0.1 °C
Standard Humidity reading : 49.91 %RH

Test point (°C)	Standard reading (°C)	UUC* reading (°C)	UUC* correction (°C)	Uncertainty of measurement (+/- °C)
25	25.06	25.6	-0.54	0.36

Result : Without adjustment
Function : Humidity measurement
Calibration point : 50 %RH
Resolution : 1 %RH
Standard Temperature reading : 25.08 °C

Test point (%RH)	Standard reading (%RH)	UUC* reading (%RH)	UUC* correction (%RH)	Uncertainty of measurement (+/- %RH)
50	50.16	47	3.16	2.3

UUC* = Unit under calibration



Inctech Metrological Center Co.Ltd.

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com



Calibration Cert. # 3884.01
ISO/IEC 17025

Certificate of Calibration

Certificate No. : MM23-3120

Page : 1 of 2

Customer : Smile Laboratory Co.,Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160

Description : Standard Weight Set

Manufacturer : N/A

Model : 500 mg-200 g

Serial No. : N/A

Identification No. : STD.W.001-007-55

Calibration Place : Mass & Torque Laboratory

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 05, 2023

Environment Condition :

Temperature : (23+/-3) °C

Humidity : (50+/-15) %RH

Atm. Pressure : (1010+/-10) hPa

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MM-007* According to comparison with the reference Standard Weight Set and mass comparator.
The calibration methods based on OIML : R111-1 : 2004


Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Standard Weight Set E1	NC-001-0.2K-E1-ASS	0022	NC-527	Oct 17, 2024

This result of calibration was found accurate as shown on date place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology (Thailand)

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%

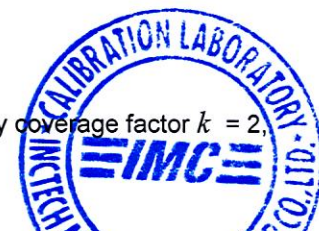

Calibrated by :
Issue date :

Approved by :

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd

**Inctech Metrological Center Co.Ltd.**

39/1 Soi 82, Sukhapiaban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.comCalibration Cert. # 3884.01
ISO/IEC 17025

Certificate No. : MM23-3120

Page : 2 of 2

Calibration Result : Without Adjustment

Identification No.	Nominal Values			Conventional Mass						Uncertainty of Measurement	
	Weight			Before Adjustment			After Adjusment			(+/-)	
-	500	mg		500	mg	-0.01	mg	-	-	0.012	mg
-	1	g		1	g	0.00	mg	-	-	0.014	mg
-	5	g		5	g	0.01	mg	-	-	0.020	mg
-	10	g		10	g	0.02	mg	-	-	0.025	mg
-	50	g		50	g	-0.01	mg	-	-	0.037	mg
-	100	g		100	g	-0.02	mg	-	-	0.060	mg
-	200	g		200	g	0.02	mg	-	-	0.61	mg



Certificate of Calibration

Certificate No. : MT23-6058

Page : 1 of 2

Customer : Smile Laboratory Co.,Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160

Description : Refrigerator

Manufacturer : Accuplus

Model : SMART i250

Serial No. : 2059-1117-0035

Identification No. : SML.IN002/61

Calibration Place : Laboratory Room

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 03, 2023

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-006* According to comparison with LXI Data Acquisition Switch Unit with sensor. The calibration methods based on Euramet Calibration Guide No.20 - guidelines on the Calibration of Temperature and/or Humidity Controlled Enclosures.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
LXI Data Acquisition Switch Unit with Sensor	34972A	MY49028922	MT22-6393	Nov 24, 2023

This result of calibration was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through
National Institute of Metrology Thailand (NIMT)

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$,
providing a level of confidence of not less than 95%



Calibrated by :

Issue date :

Approved by :

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd

Certificate No. : MT23-6058

Page : 2 of 2

Function : Temperature measurement


Result : Without adjustment

Calibration point : 4 °C

Resolution : 0.1 °C

Calibration point (°C)	Temperature of UUC* at each position (°C)									Uncertainty of measurement (+/- °C)
	Ch.1	Ch.2	Ch.3	Ch.4	Ch.5	Ch.6	Ch.7	Ch.8	Ch.9	
4	5.321	4.710	4.983	4.837	4.990	4.665	5.131	4.696	4.933	0.31

Setting temperature (°C)	Indicating Temperature (°C)	Measured stability (+/- °C)	Measured uniformity (°C)	Overall variation (°C)
4.0	4.1 to 4.3	0.15	0.53	1.0

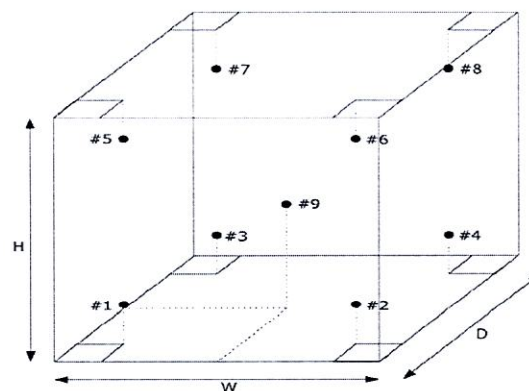

- #1 Lower Left Front
- #2 Lower Right Front
- #3 Lower Left Rear
- #4 Lower Right Rear
- #5 Upper Left Front
- #6 Upper Right Front
- #7 Upper Left Rear
- #8 Upper Right Rear
- #9 Geometric Center

Front view

UUC* = Unit under calibration

Uniformity = Maximum and Minimum difference of measured temperature at any probes and the measured temperature at the reference and same time.

Overall Variation = Difference of temperature value between the maximum and minimum any time.

Stability = One half of the maximum difference of measured temperatures at any one probe.



Inctech Metrological Center Co.Ltd.

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,
Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com



Calibration Cert. # 3884.01
ISO/IEC 17025

Certificate of Calibration

Certificate No. : MM23-3116

Page : 1 of 3

Customer : Smile Laboratory Co.,Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160

Description : Electronic Balance

Manufacturer : Mettler Toledo

Model : MS205DU

Serial No. : 850938841

Identification No. : SML.AB002/61

Calibration Place : Balance Room

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 03, 2023

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Atm. Pressure : (1010+/-10) hPa

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MM-001*
According to comparison with Standard Weight Set.
The calibration methods based on UKAS - LAB 14 : 2022

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Standard Weight Set	NC-001-0.2K-E1-ASS	0022	NC-527	Oct 17, 2024

This result of calibration was found accurate as shown on date place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through
National Institute of Metrology (Thailand)

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor $k = 2$,
providing a level of confidence of not less than 95%



Calibrated by : M

Issue date :

Approved by :

This calibration certificate shall not be reproduced other than in full except with the prior written
approval of Inctech Metrological Center Co.,Ltd

**Inctech Metrological Center Co.Ltd.**39/1 Soi 82, Sukhapiaban 5 Rd., O ngoen,
Saimai, Bangkok 10220, ThailandTel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.comCalibration Cert. # 3884.01
ISO/IEC 17025



Certificate No. : MM23-3116

Page : 2 of 3

Calibration Result : Without Adjustment
 Function : Repeatability
 Maximum Capacity : 200 g
 Resolution : 0 to 82 g = 0.00001 g
 > 82 g = 0.0001 g

Nominal Weight Value	Instrument Deviation of Reading
(g)	(g)
200	0.0000

Calibration Result : Without Adjustment
 Function : Effect of Off Center Loading



A Mass of 100 Was Placed to various Position on the pan.

The Weight Machine Reading Obtained is Given in The Tabel

Load	Measuring Positions					Maximum Different
	A	B	C	D	E	
(g)	(g)	(g)	(g)	(g)	(g)	(g)
100	100.0001	100.0001	100.0001	100.0003	100.0001	100.0001
						0.0002

Calibration Result : Without Adjustment
 Function : Effect of Tare

Nominal Tare Weight	Standard Weight	UUC* Reading	UUC* Deviation
(g)	(g)	(g)	(g)
100	Tare	0.00000	0.00000
	At 20 %	20	20.00002
	At 40 %	40	40.00006
	At 60 %	60	60.00001
	At 80 %	80	80.00001
	At 100 %	100	100.0002

UUC* = Unit Under Calibration

**Inctech Metrological Center Co.Ltd.**

39/1 Soi 82, Sukhapiaban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.comCalibration Cert. # 3884.01
ISO/IEC 17025

Certificate No. : MM23-3116

Page : 3 of 3

Calibration Result : Without Adjustment

Function : Departure of indication from nominal value

Standard Weight Value (g)	UUC* Reading (g)	UUC* Correction (g)	Uncertainty of Measurement (+/- g)
0.00000	0.00000	0.00000	0.000010
20.00003	20.00002	0.00001	0.000056
40.00008	40.00006	0.00002	0.000084
60.00006	60.00004	0.00002	0.00015
80.00004	80.00001	0.00003	0.00015
100.0000	100.0000	0.0000	0.00016
120.0002	120.0002	0.0000	0.00031
140.0001	140.0001	0.0000	0.00031
160.0002	160.0002	0.0000	0.00031
180.0002	180.0002	0.0000	0.00031
200.0001	200.0001	0.0000	0.00031

UUC* = Unit Under Calibration



Certificate of Calibration

Certificate No. : MC23-2400

Page : 1 of 3

Customer : Smile Laboratory Co., Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160

Description : Spectrophotometer

Manufacturer : Hach

Model : DR 6000

Serial No. : 1735844

Identification No. : SML.UV001/61

Calibration Place : Chemical Laboratory 1

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 05, 2023

Environment Condition :

Temperature : (23+/-3) °C

Humidity : (50+/-15) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MC-008*. According to direct measurement with wavelength standard filter and absorbance standard filter.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Neutral Density Filter	RM-1N2N3N	18944	CI-0137-23	Apr 25, 2025
Holmium Filter	RM-HG	19136	CI-0138-23	Apr 24, 2025

This result of calibration was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology Thailand (NIMT)

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%



Calibrated by : 

Issue date : 

Approved by : 

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd

**Inctech Metrological Center Co.Ltd.**

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.comCalibration Cert. # 3884.01
ISO/IEC 17025

Certificate No. : MC23-2400

Page : 2 of 3

Result : Without adjustment
Function : Photometric accuracy

Wavelength setting (nm)	Standard value (Abs)	UUC* reading (Abs)	UUC* correction (Abs)	Uncertainty of measurement (+/- Abs)
440	0.0000	0.000	0.0000	0.003
	0.5537	0.557	-0.0033	0.003
	0.7450	0.749	-0.0040	0.003
	0.9898	0.990	-0.0002	0.003
465	0.0000	0.000	0.0000	0.003
	0.5142	0.517	-0.0028	0.003
	0.6873	0.691	-0.0037	0.003
	0.9400	0.939	0.0010	0.003
546.1	0.0000	0.000	0.0000	0.003
	0.5104	0.511	-0.0006	0.003
	0.6953	0.697	-0.0017	0.003
	0.9831	0.981	0.0021	0.003
590	0.0000	0.000	0.0000	0.003
	0.5439	0.543	0.0009	0.003
	0.7230	0.724	-0.0010	0.003
	1.0785	1.076	0.0025	0.003
635	0.0000	0.000	0.0000	0.003
	0.5511	0.550	0.0011	0.003
	0.6900	0.691	-0.0010	0.003
	1.0715	1.069	0.0025	0.003

UUC* = Unit under calibration

**Inctech Metrological Center Co.Ltd.**

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.comCalibration Cert. # 3884.01
ISO/IEC 17025

Certificate No. : MC23-2400

Page : 3 of 3

Result : Without adjustment
Function : Wavelength accuracy

Spectral Band Width : 2 nm
Scan Speed : -

Standard value (nm)	UUC* reading (nm)	UUC* correction (nm)	Uncertainty of measurement (+/- nm)
288.04	288.0	0.04	0.14
418.34	418.0	0.34	0.14
446.01	446.0	0.01	0.14
536.39	536.0	0.39	0.14
637.84	638.0	-0.16	0.14

UUC* = Unit under calibration



Certificate of Calibration

Certificate No. : MC23-2370

Page : 1 of 2

Customer : Smile Laboratory Co., Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160

Description : pH Meter

Manufacturer : Mettler Toledo

Model : Seven Direct SD20

Serial No. : C238817351

Identification No. : SML.PH001/61

Calibration Place : Laboratory Room

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 03, 2023

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MC-001* According to direct with Standard Thermometer and Standard Buffer Solution at 25 °C. The calibration methods based on ISO 10523 Water quality - Determination of pH, NIST : 1994.

Calibration were conducted using In-house calibration procedure *CP-MT-001* According to comparison with Standard Digital Thermometer.

The calibration methods based on ITS-90.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Digital Thermometer	EFT-4	EFT42020033	MT23-3227	May 01, 2024
Standard Digital Thermometer	UM RTD	2002Z Z38 0073A	MT22-6383	Nov 21, 2023
<u>Instrument</u>	<u>Model</u>	<u>Lot No.</u>	<u>Expired Date.</u>	
Standard Buffer Solution (4 pH)	1040525C	4C22E1	May 28, 2025	
Standard Buffer Solution (7 pH)	1070525C	725C22B1	Feb 28, 2024	
Standard Buffer Solution (10 pH)	1100525C	1125C22B1	Feb 28, 2024	

This result of calibration was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through
National Institute of Metrology Thailand (NIMT)

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$,
providing a level of confidence of not less than 95%



Calibrated by
Issue date

Approved by :

This calibration certificate shall not be reproduced other than in full except with
approval of Inctech Metrological Center Co.,Ltd

**Inctech Metrological Center Co.Ltd.**

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com

Calibration Cert. # 3884.01
ISO/IEC 17025

Certificate No. : MC23-2370

Page : 2 of 2

Function : pH measurement (Electrode)

Calibration point : 4, 7, 10 pH

Probe S/N : 2228537

Result : Without adjustment

Resolution : 0.01 pH

Standard Buffer (pH)	UUC* reading (pH)	UUC* correction (pH)	Uncertainty of measurement (+/- pH)
4.01	4.00	0.01	0.017
7.00	6.99	0.01	0.017
9.99	10.00	-0.01	0.017

Function : Temperature measurement

Sensor Type : Thermistor

Diameter : 12 mm

Calibration point : 23, 25, 27 °C

Result : Without adjustment

Resolution : 0.1 °C

Immersion depth (mm)	Calibration point (°C)	Standard reading (°C)	UUC* reading (°C)	UUC* correction (°C)	Uncertainty of measurement (+/- °C)
100	23	23.04	23.3	-0.26	0.20
100	25	25.04	25.2	-0.16	0.20
100	27	27.04	27.1	-0.06	0.20
100	23	23.04	23.3	-0.26	0.20

UUC* = Unit under calibration



Certificate of Calibration

Certificate No. : MT23-6054

Page : 1 of 2

Customer : Smile Laboratory Co.,Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160

Description : Incubator

Manufacturer : Bio Base

Model : BJPX-B7011

Serial No. : 201705233231

Identification No. : SML.IN001/61

Calibration Place : Laboratory Room

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 03, 2023

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-006* According to comparison with LXI Data Acquisition Switch Unit with sensor. The calibration methods based on Euramet Calibration Guide No.20 - guidelines on the Calibration of Temperature and/or Humidity Controlled Enclosures.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
LXI Data Acquisition Switch Unit with Sensor	34972A	MY49028922	MT22-6393	Nov 24, 2023

This result of calibration was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through
National Institute of Metrology Thailand (NIMT)

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$,
providing a level of confidence of not less than 95%



Calibrated by
Issue date

Approved by

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd

**Inctech Metrological Center Co.Ltd.**

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,


Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com

Calibration Cert. # 3884.01
ISO/IEC 17025**Certificate No.** : MT23-6054**Page** : 2 of 2**Function** : Temperature measurement**Result** : Without adjustment**Calibration point** : 20 °C**Resolution** : 0.1 °C

Calibration point (°C)	Temperature of UUC* at each position (°C)									Uncertainty of measurement (+/- °C)
	Ch.1	Ch.2	Ch.3	Ch.4	Ch.5	Ch.6	Ch.7	Ch.8	Ch.9	
20	20.110	19.987	20.380	20.217	20.126	20.149	20.103	20.045	20.259	0.31

Setting temperature (°C)	Indicating Temperature (°C)	Measured stability (+/- °C)	Measured uniformity (°C)	Overall variation (°C)
20.0	20.0	0.07	0.32	0.53

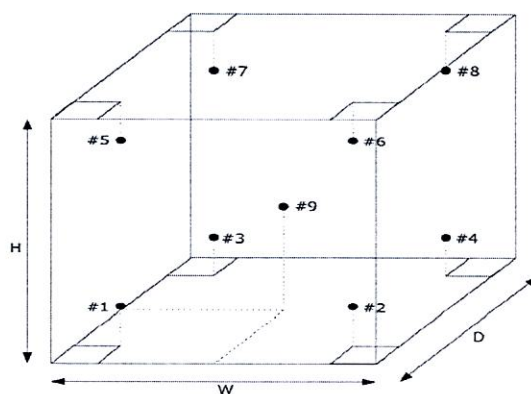

- #1 Lower Left Front
- #2 Lower Right Front
- #3 Lower Left Rear
- #4 Lower Right Rear
- #5 Upper Left Front
- #6 Upper Right Front
- #7 Upper Left Rear
- #8 Upper Right Rear
- #9 Geometric Center

Front view**UUC*** = Unit under calibration**Uniformity** = Maximum and Minimum difference of measured temperature at any probes and the measured temperature at the reference and same time.**Overall Variation** = Difference of temperature value between the maximum and minimum any time.**Stability** = One half of the maximum difference of measured temperatures at any one probe.

**Inctech Metrological Center Co.Ltd.**39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,
Saimai, Bangkok 10220, ThailandTel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.comCalibration Cert. # 3884.01
ISO/IEC 17025

Certificate of Calibration

Certificate No. : MT23-6057

Page : 1 of 2

Customer : Smile Laboratory Co.,Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok, 10160

Description : Hot Air Oven

Manufacturer : Bio Base

Model : BOV-V30F

Serial No. : 175226

Identification No. : SML.OV001/61

Calibration Place : Laboratory Room

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 03, 2023

Environment Condition :

Temperature : (25+/-10) °C

Humidity : (50+/-30) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-MT-006* According to comparison with LXI Data Acquisition Switch Unit with sensor. The calibration methods based on Euramet Calibration Guide No.20 - guidelines on the Calibration of Temperature and/or Humidity Controlled Enclosures.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
LXI Data Acquisition Switch Unit with Sensor	34972A	MY49028922	MT22-6393	Nov 24, 2023

This result of calibration was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through National Institute of Metrology Thailand (NIMT)

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$, providing a level of confidence of not less than 95%



Calibrated by : _____

Issue date : _____

Approved by : _____

This calibration certificate shall not be reproduced other than in full except with the prior written approval of Inctech Metrological Center Co.,Ltd

Certificate No. : MT23-6057

Page : 2 of 2

Function : Temperature measurement


Result : Without adjustment

Calibration point : 104, 150, 180 °C

Resolution : 0.1 °C

Calibration point (°C)	Temperature of UUC* at each position (°C)									Uncertainty of measurement (+/- °C)
	Ch.1	Ch.2	Ch.3	Ch.4	Ch.5	Ch.6	Ch.7	Ch.8	Ch.9	
104	104.459	104.103	104.369	104.477	104.772	104.047	104.293	104.497	104.837	0.44
150	150.112	150.203	150.620	150.164	150.465	150.112	150.498	150.129	150.623	0.44
180	178.765	179.298	179.719	179.639	179.695	179.465	179.079	179.155	179.774	0.58

Setting temperature (°C)	Indicating Temperature (°C)	Measured stability (+/- °C)	Measured uniformity (°C)	Overall variation (°C)
104.0	104.0	0.15	0.95	1.1
150.0	150.1 to 150.2	0.24	0.90	1.2
180.0	180 to 180.2	0.34	1.6	1.9

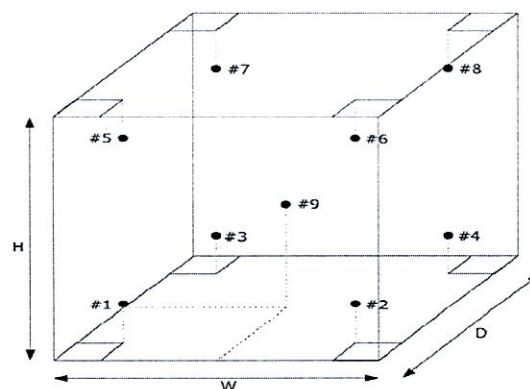

- #1 Lower Left Front
- #2 Lower Right Front
- #3 Lower Left Rear
- #4 Lower Right Rear
- #5 Upper Left Front
- #6 Upper Right Front
- #7 Upper Left Rear
- #8 Upper Right Rear
- #9 Geometric Center

Front view
UUC* = Unit under calibration

Uniformity = Maximum and Minimum difference of measured temperature at any probes and the measured temperature at the reference and same time.

Overall Variation = Difference of temperature value between the maximum and minimum any time.

Stability = One half of the maximum difference of measured temperatures at any one probe.



Inctech Metrological Center Co.Ltd.

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,
Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.com



Calibration Cert. # 3884.01
ISO/IEC 17025

Certificate of Calibration

Certificate No. : ME23-2507

Page : 1 of 2

Customer : Smile Laboratory Co.,Ltd.

Address : 563/1 Thoet Thai Rd., Bangwa, Phasicharoen, Bangkok 10160

Description : Stop Watch

Manufacturer : Seiko

Model : S23601P

Serial No. : A12BI0147

Identification No. : ACF.WA002/59

Calibration Place : Time and Frequency Laboratory

Order No. : 3156/23

Received date : Oct 03, 2023

Calibration date : Oct 05, 2023

Environment Condition :

Temperature : (23 +/- 3) °C

Humidity : (50 +/- 15) %RH

Calibration Method : Calibration were conducted using In-house calibration procedure *CP-ME-001*.
According to comparison with Universal Counter.
The calibration methods based on NIST : SP960-12 : 2009.

Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
Universal Counter	53131A	3416A06010	E3U230553	Apr 09, 2024

This result of calibration was found accurate as shown on date and place of calibration only.

Traceability : This measurement are traceable to the International System of Unit (SI), through
National Institute of Metrology Thailand (NIMT)

The reported uncertainty of measurement was based on standard uncertainty multiplied by coverage factor $k = 2$,
providing a level of confidence of not less than 95%



Calibrated by : _____

Issue date : _____

Approved _____

(pa)

This calibration certificate shall not be reproduced other than in full except with the prior written
approval of Inctech Metrological Center Co.,Ltd

**Inctech Metrological Center Co.Ltd.**

39/1 Soi 82, Sukhapiban 5 Rd., O ngoen,

Saimai, Bangkok 10220, Thailand

Tel. (662) 909-8820 (Auto 10 lines) www.imcinstrument.comCalibration Cert. # 3884.01
ISO/IEC 17025**Certificate No. : ME23-2507****Page : 2 of 2**

Calibration Result : Without Adjustment
Function : Quartz Crystal Measurement
Frequency Range : 32 kHz

Nominal Value (kHz)	Measurement Value (kHz)	Measurement Error (kHz)	Uncertainty of Measurement (+/- mHz)
32.768	32.7671	-0.0009	0.76

$$\begin{aligned}\text{Timebase in 1 second} &= \frac{\text{Nominal frequency (Hz)}}{\text{Actual frequency (Hz)}} \\ &= 1.0000275 \text{ sec}\end{aligned}$$

The uncertainty of time measurement was ± 0.76 mHz or ± 0.76 ms/s