

# ภาคผนวก ง

---

ใบรับรองการสอบเทียบเครื่องมือ



right solutions.  
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ

Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Ambient	Total Suspended Particulate	High Volume	RYG_FS0181	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0180	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0395	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0173	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0182	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0291	-	-	On site Calibration
Ambient	Total Suspended Particulate	High Volume	RYG_FS0175	-	-	On site Calibration
Ambient	Total Suspended Particulate	Digital Balance	RYG_EN0001	22-Feb-24	22-Feb-25	12
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0666	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0399	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0183	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0667	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0189	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0665	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	High Volume	RYG_FS0398	-	-	On site Calibration
Ambient	Particulate Matter (PM-10)	Digital Balance	RYG_EN0001	22-Feb-24	22-Feb-25	12
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	RYG_FS0255	2-Jul-24	2-Jan-25	6
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	RYG_FS0272	2-Jul-24	2-Jan-25	6
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	RYG_FS0457	3-Jul-24	3-Jan-25	6
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	RYG_FS0533	3-Jul-24	3-Jan-25	6
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	BKK_FS0797	2-Jul-24	2-Jan-25	6
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	RYG_FS0453	3-Jul-24	3-Jan-25	6
Ambient	Nitrogen Dioxide	NO <sub>2</sub> Analyzer	RYG_FS0463	3-Jul-24	3-Jan-25	6
Ambient	Sulfur Dioxide	SO <sub>2</sub> Analyzer	RYG_FS0254	4-Jul-24	4-Jan-25	6
Ambient	Sulfur Dioxide	SO <sub>2</sub> Analyzer	RYG_FS0460	5-Jul-24	5-Jan-25	6
Ambient	Sulfur Dioxide	SO <sub>2</sub> Analyzer	RYG_FS0456	5-Jul-24	5-Jan-25	6
Ambient	Sulfur Dioxide	SO <sub>2</sub> Analyzer	BKK_FS0796	4-Jul-24	4-Jan-25	6
Ambient	Sulfur Dioxide	SO <sub>2</sub> Analyzer	RYG_FS0534	5-Jul-24	5-Jan-25	6
Ambient	Sulfur Dioxide	SO <sub>2</sub> Analyzer	RYG_FS0452	5-Jul-24	5-Jan-25	6
Ambient	Sulfur Dioxide	SO <sub>2</sub> Analyzer	RYG_FS0462	5-Jul-24	5-Jan-25	6
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	BKK_FS0143	20-Aug-24	20-Feb-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0608	18-Jul-24	18-Jan-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0329	18-Aug-23	18-Feb-25	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0328	18-Aug-23	18-Feb-25	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0609	18-Jul-24	18-Jan-26	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0085	19-Jun-23	19-Dec-24	18
Ambient	Wind Speed / Wind Direction	Wind Speed / Wind Direction	RYG_FS0544	21-Jul-23	21-Jan-25	18
Noise	Leq 24 hrs	Sound Calibrator	RYG_FS0215	23-Aug-24	23-Aug-25	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0431	22-Feb-24	21-Feb-25	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0437	19-Oct-23	19-Oct-24	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0615	5-Jan-24	4-Jan-25	12
Noise	Leq 24 hrs	Sound Level Meter	RYG_FS0616	5-Jan-24	4-Jan-25	12
Noise	Leq 8 hrs	Sound Calibrator	RYG_FS0213	28-Feb-24	27-Feb-25	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0494	23-Feb-24	22-Feb-25	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0495	23-Feb-24	22-Feb-25	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0612	5-Jan-24	4-Jan-25	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0615	5-Jan-24	4-Jan-25	12
Noise	Leq 8 hrs	Sound Level Meter	NKH_FS0115	1-Nov-23	1-Nov-24	12
Noise	Leq 8 hrs	Sound Calibrator	RYG_FS0213	28-Feb-24	27-Feb-25	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0301	12-Jan-24	11-Jan-25	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0302	19-Sep-24	19-Sep-25	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0438	30-Oct-24	30-Oct-25	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0439	9-Oct-24	9-Oct-25	12
Noise	Leq 8 hrs	Sound Level Meter	RYG_FS0493	23-Feb-24	22-Feb-25	12



right solutions.  
right partner.

รายการเครื่องมือที่ใช้ในการวิเคราะห์ / ทดสอบ


Sample Name	Parameter	Equipment Name	ID No.	Calibrated Date	Next Cal	Freq. Calibrate (Months)
Rayong Lab	pH at 25 °C	pH Meter	RYG_EN0152	14-Dec-23	14-Jun-25	18
Rayong Lab	Total Suspended Solids	Electronic Balance	RYG_EN0002	22-Feb-24	22-Feb-25	12
Rayong Lab	Total Suspended Solids	Hot Air Oven	RYG_EN0010	21-Mar-24	21-Sep-25	18
Rayong Lab	Total Dissolved Solids 180°C	Electronic Balance	RYG_EN0002	22-Feb-24	22-Feb-25	12
Rayong Lab	Total Dissolved Solids 180°C	Hot Air Oven	RYG_EN0010	21-Mar-24	21-Sep-25	18
Rayong Lab	Oil & Grease	Electronic Balance	RYG_EN0002	22-Feb-24	22-Feb-25	12
Rayong Lab	Oil & Grease	Hot Air Oven	RYG_EN0213	21-Mar-24	21-Mar-25	12
Rayong Lab	Oil & Grease	Water Bath	RYG_EN0061	21-Mar-24	21-Sep-25	18
Rayong Lab	Temperature	Digital Thermometer	RYG_FS0568	23-Apr-24	23-Apr-25	12
Rayong Lab	Chlorine	pH ISE Meter	RYG_EN0152	14-Dec-23	14-Jun-25	18
Rayong Lab	Sulfate	Spectrophotometer	RYG_EN0037	18-Sep-23	18-Mar-25	18
Rayong Lab	Sulfide	Chamber (Cold Room)	RYG_EN0184	11-Jun-24	11-Dec-25	18





## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	ริมรั้วโครงการด้านทิศตะวันออก (A1)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0181
CalibrationSheet No.:	C-270924-RYG_FS0181	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	5334
Calibrator Model :	TE-5028A	Calibrator Slope :	1.52567
Calibrator S/N :	1166	Calibrator Intercept :	-0.03613

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.4	1.0428	40	Slope : 36.4574 Intercept : 1.7956 Correlation Coefficient : 0.9992
2	3.0	1.1616	44	
3	3.9	1.3194	50	
4	4.7	1.4449	54	
5	5.7	1.5875	60	

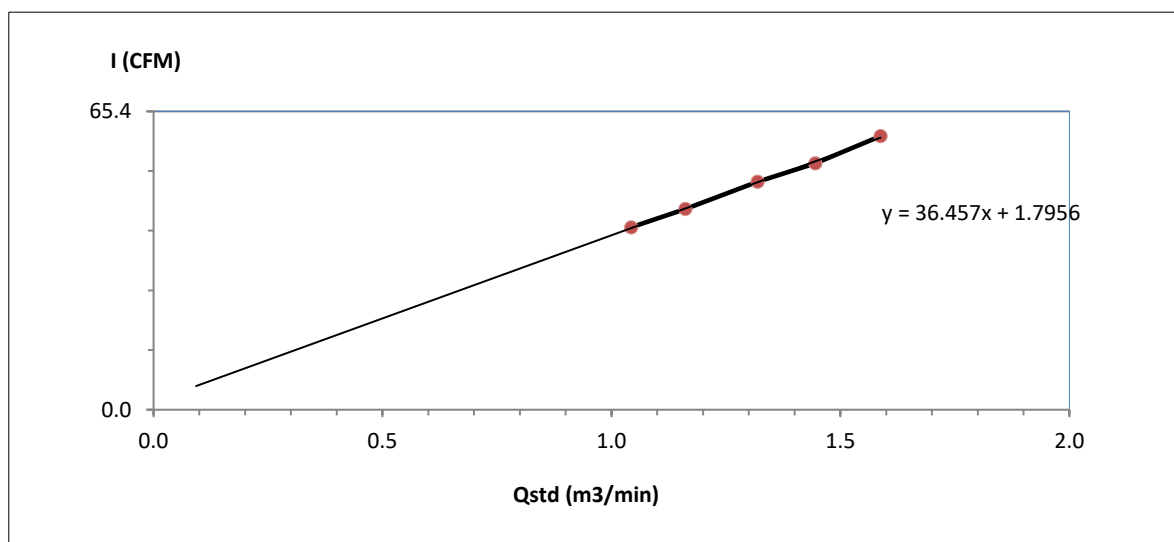

Calibrated by   
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)

Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)






## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	บริเวณสถานีไฟฟ้าอ้อย (A2)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0180
CalibrationSheet No.:	C-270924-RYG_FS0180	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	1328
Calibrator Model :	TE-5028A	Calibrator Slope :	1.52567
Calibrator S/N :	1166	Calibrator Intercept :	-0.03613

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.6	1.0839	40	Slope : 39.1399 Intercept : -2.9507 Correlation Coefficient : 0.9983
2	3.3	1.2166	44	
3	4.1	1.3519	50	
4	4.8	1.4598	54	
5	5.8	1.6011	60	

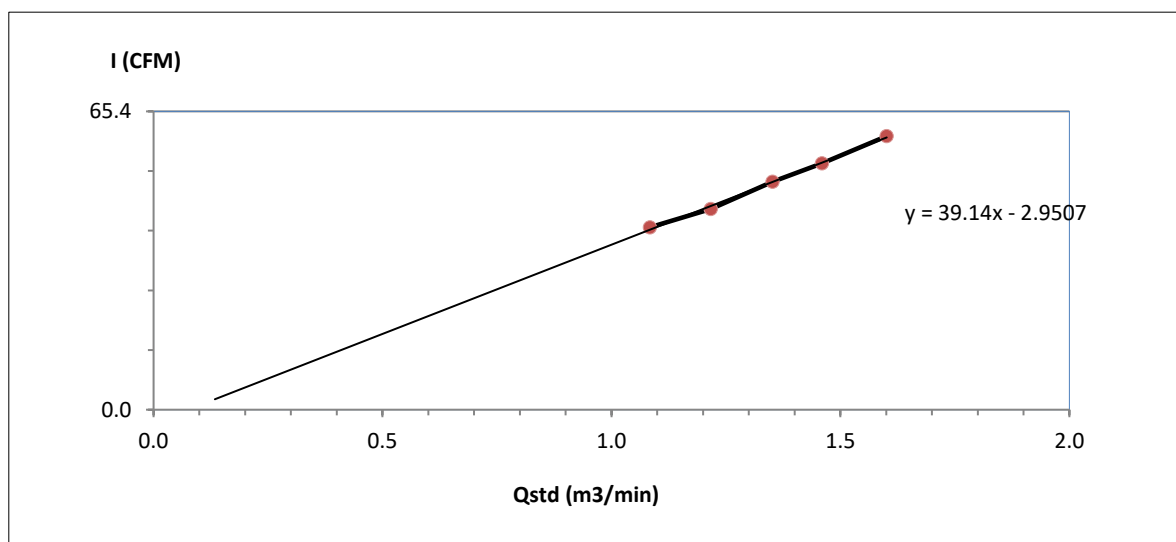

Calibrated by

( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)

Approved by :


(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)





## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	วัดหนองนาราม (A3)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0395
Calibration Sheet No.:	C-270924-RYG_FS0395	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	5692
Calibrator Model :	TE-5028A	Calibrator Slope :	1.52567
Calibrator S/N :	1166	Calibrator Intercept :	-0.03613

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.5	1.0636	40	Slope : 38.7979 Intercept : -1.2114 Correlation Coefficient : 0.9998
2	3.0	1.1616	44	
3	3.9	1.3194	50	
4	4.6	1.4298	54	
5	5.6	1.5738	60	

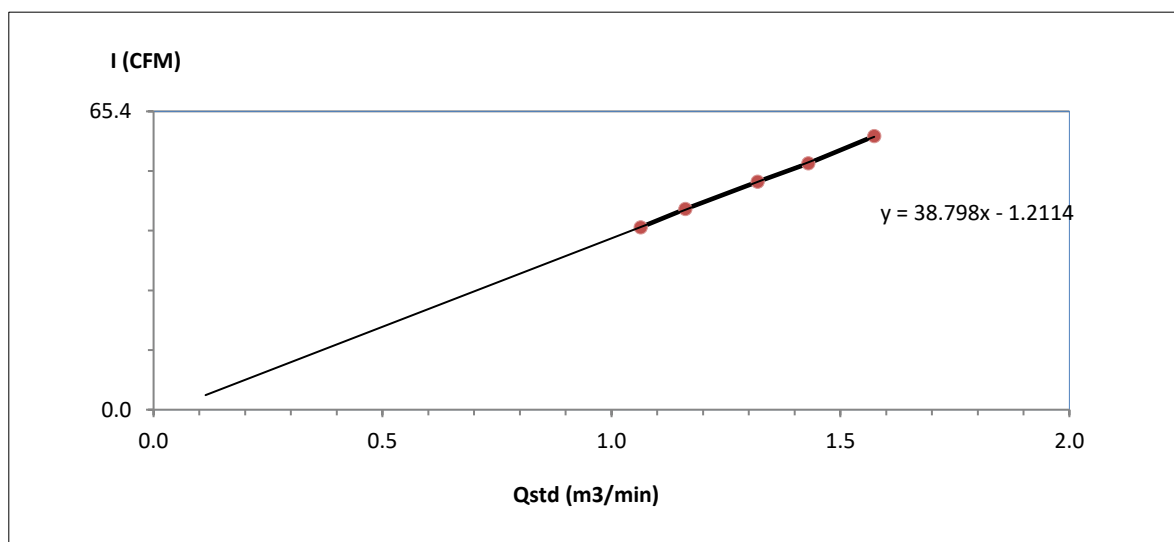

Calibrated by   
( Mr. Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)





## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	วัดบ่อวิน (A4)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0173
CalibrationSheet No.:	C-270924-RYG_FS0173	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	4799
Calibrator Model :	TE-5028A	Calibrator Slope :	1.52567
Calibrator S/N :	1166	Calibrator Intercept :	-0.03613

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.5	1.0636	40	Slope : 38.9302 Intercept : -1.6469 Correlation Coefficient : 0.9985
2	3.1	1.1802	44	
3	3.9	1.3194	50	
4	4.7	1.4449	54	
5	5.6	1.5738	60	

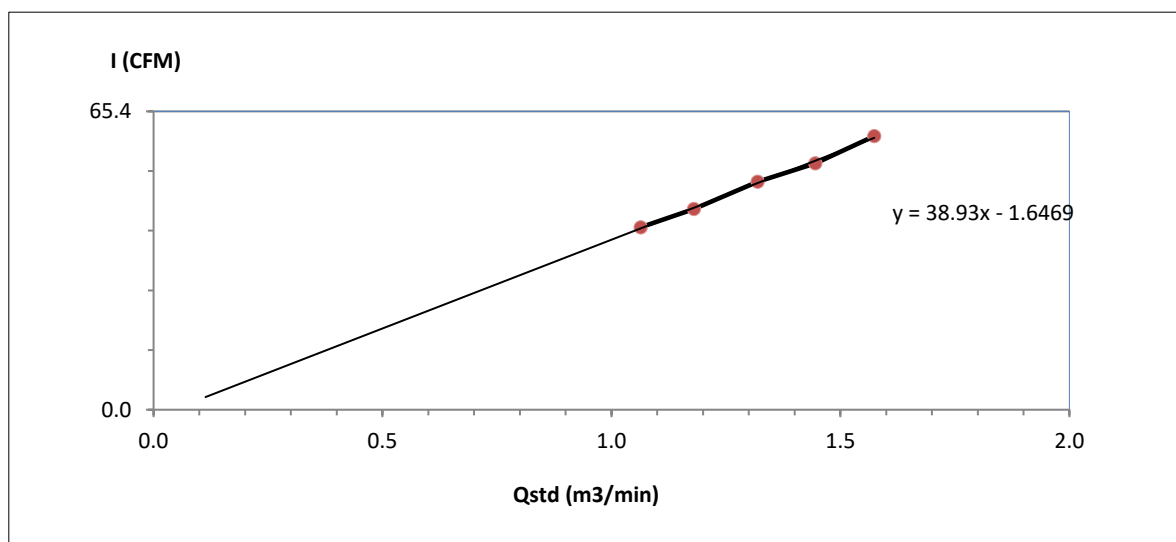

Calibrated by   
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)





## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	วัดพันเสด็จนอก (A5)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0182
CalibrationSheet No.:	C-270924-RYG_FS0182	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	5335
Calibrator Model :	TE-5028A	Calibrator Slope :	1.52567
Calibrator S/N :	1166	Calibrator Intercept :	-0.03613

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.4	1.0428	40	Slope : 37.1620 Intercept : 0.9733 Correlation Coefficient : 0.9983
2	3.0	1.1616	44	
3	3.9	1.3194	50	
4	4.7	1.4449	54	
5	5.6	1.5738	60	

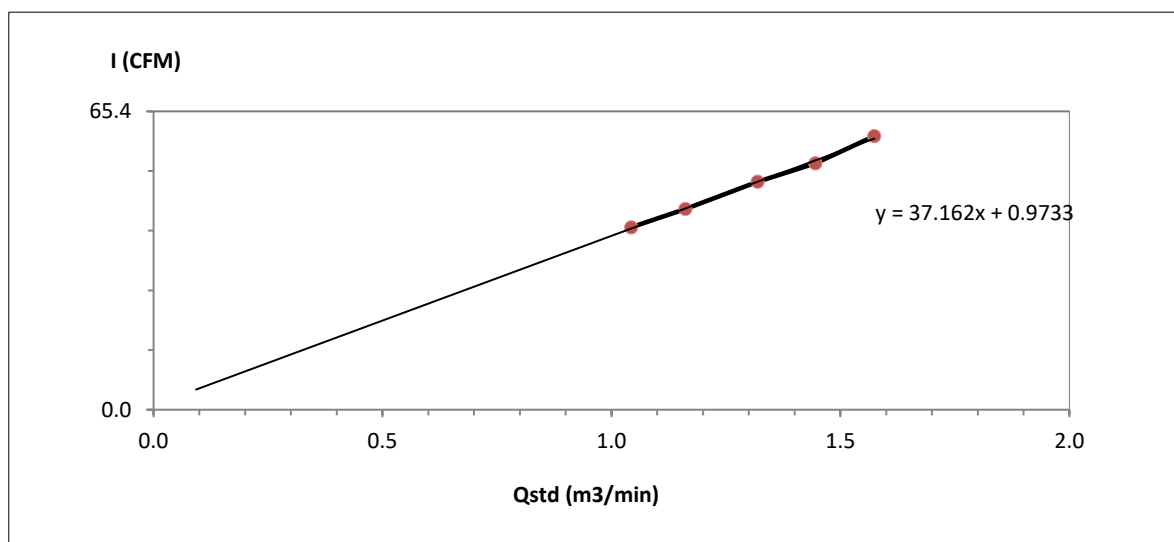

Calibrated by   
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)



## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	ชุมชนห้วยเหียน (A6)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0291
CalibrationSheet No.:	C-270924-RYG_FS0291	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	5333
Calibrator Model :	TE-5028A	Calibrator Slope :	1.52567
Calibrator S/N :	1166	Calibrator Intercept :	-0.03613

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.5	1.0636	40	Slope : 42.6952 Intercept : -5.8464 Correlation Coefficient : 0.9980
2	3.1	1.1802	44	
3	3.8	1.3028	50	
4	4.5	1.4146	54	
5	5.3	1.5321	60	

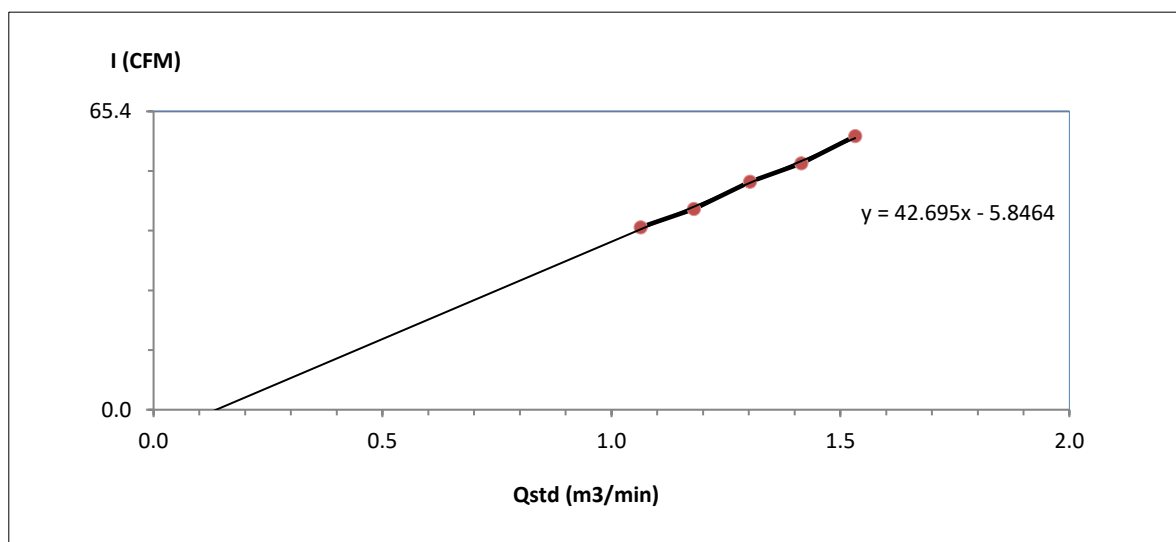

Calibrated by   
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)





## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	บ้านนาบอน (A7)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0175
Calibration Sheet No.:	C-270924-RYG_FS0175	High Volume Model :	TE-5170D
Calibrator ID:	RYG_FS0205	High Volume S/N :	4801
Calibrator Model :	TE-5028A	Calibrator Slope :	1.52567
Calibrator S/N :	1166	Calibrator Intercept :	-0.03613

Test No.	Delta H <sub>2</sub> O (inch)	Q <sub>std</sub> (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	2.6	1.0839	40	Slope : 42.2522 Intercept : -6.2408 Correlation Coefficient : 0.9989
2	3.2	1.1985	44	
3	4.0	1.3357	50	
4	4.6	1.4298	54	
5	5.5	1.5601	60	

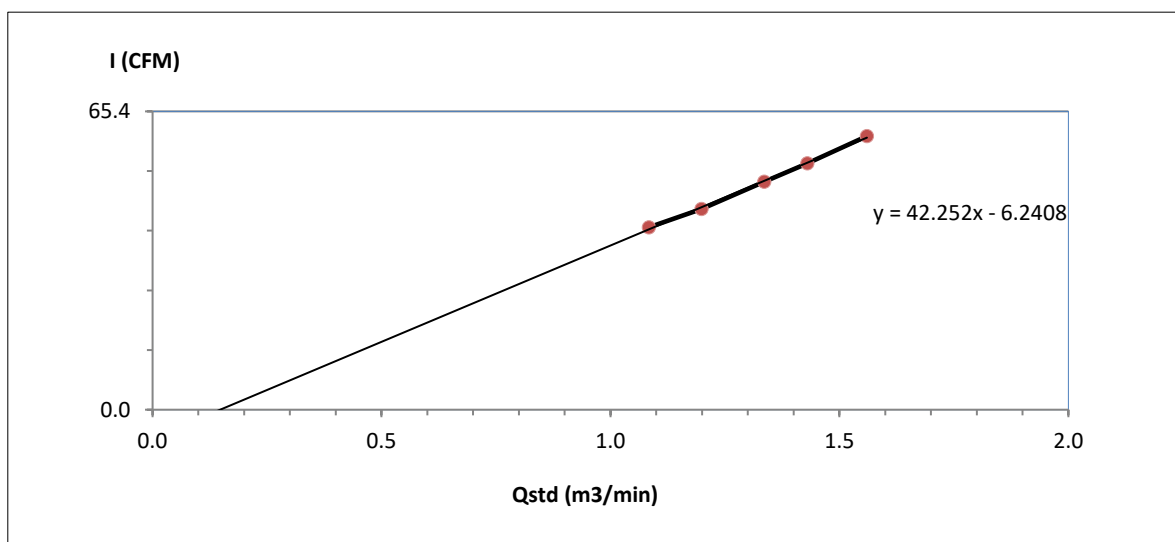

Calibrated by   
( Mr. Anurak Tongkhajonsakda )  
Field Scientist(2)

Approved by   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)



**SARTORIUS**

NSC-TISI-TIS 17025  
CALIBRATION 0426

# Certificate

## of Calibration

Model Number : LA130S-F  
Description : Analytical Balance  
Serial Number : 25409664  
ID No. : RYG\_EN0001  
Manufacturer : Sartorius

Certificate No. : 24BCI0068  
Issued Date : Friday, February 23, 2024  
Reference No. : 229196

Customer Name : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)  
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd.(Balance Room)  
616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated By : Mr.Chonchai Inthana  
Calibration Date : Thursday, February 22, 2024

Page No. : 1 of 2  
REVIEW BY Thamitak  
APPROVED BY [Signature]  
NEXT CAL. DATE 22/02/2025

### Metrological data :

Capacity : 150 g Readability : 0.0001 g

### Reasons for calibration

☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance

### Calibration

Procedure No. : This calibration was conducted by  
Using in-house calibration procedure number (WI-003)  
Based on UKAS LAB 14 : 2019

### Ambients Conditions:

Temperature : 23.6 °C ± 5.0 °C  
Humidity : 54.0 % RH ± 10.0 % RH  
Pressure :                      ±                     

Equipment Condition: ☒ Good Operate ☐ Fair

## Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

## Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	TCS	M2308197S	23-Aug-2025
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19231845	23-Aug-2024

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division  
Sartorius (Thailand) Co., Ltd.

[Signature]

Mr.chonchai Intrhana(Technical Manager)

S  
T  
A  
M  
P



**Sartorius (Thailand) Co., Ltd.**

129 Rama 9 Road, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

**SARTORIUS**

# Certificate of Calibration

Model Number : LA130S-F

Description : Analytical Balance

Serial Number : 25409664

ID No. : RYG\_EN0001

Manufacturer : Sartorius

Certificate No. : 24BCI0068

Issued Date : Friday, February 23, 2024

Reference No. : 229196

Page No. : 2 of 2

## Calibration Results : Without Adjustment

### Repeatability



The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	10.0000	99.9999
10 g	10.0000	100.0000
Tolerance	10.0000	100.0001
0.0001 g	10.0000	100.0001
	9.9999	100.0000
Nominal Value : (High Load)	10.0000	100.0001
100 g	10.0000	100.0000
Tolerance	10.0000	100.0001
0.0001 g	9.9999	100.0002
	9.9999	100.0001
Standard Deviation	0.00005	0.00008

### Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 50 g  
Tolerance 0.0004 g



	Difference
1	—
2	-0.0001
3	0.0001
4	0.0002
5	0.0000
6	-

### Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00020
0.05	0.0500	0.0500	0.0000	0.00021
0.1	0.1000	0.1000	0.0000	0.00021
0.5	0.5000	0.5000	0.0000	0.00021
1	1.0000	1.0000	0.0000	0.00021
2	2.0000	2.0000	0.0000	0.00021
5	5.0000	5.0000	0.0000	0.00021
10	10.0000	10.0001	0.0001	0.00024
20	20.0000	20.0001	0.0001	0.00021
100	100.0000	99.9999	-0.0001	0.00024

End of Report.








## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	ริมรั้วโครงการด้านทิศตะวันออก (A1)	Temperature ( °C) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0666
CalibrationSheet No.:	C-270924-RYG_FS0666	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	6265
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95561
Calibrator S/N :	1166	Calibrator Intercept :	-0.02266

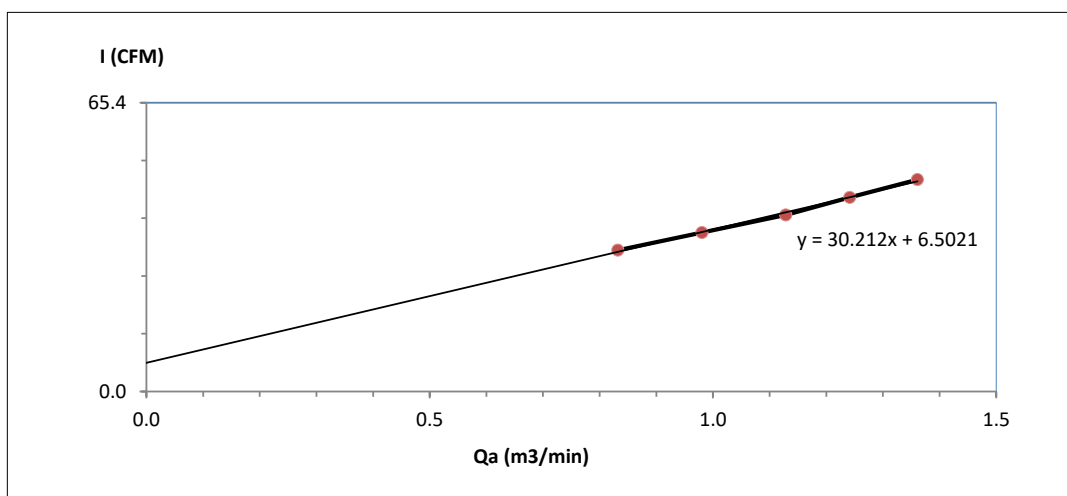Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	1.5	0.832	32	Slope : 30.2125 Intercept : 6.5021 Correlation Coefficient : 0.9980
2	2.1	0.980	36	
3	2.8	1.129	40	
4	3.4	1.241	44	
5	4.1	1.361	48	



Calibrated by   
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)



### High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	บริเวณสถานีไฟฟ้าอ้อย (A2)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0399
CalibrationSheet No.:	C-270924-RYG_FS0399	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	5683
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95561
Calibrator S/N :	1166	Calibrator Intercept :	-0.02266

Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	1.7	0.884	32	Slope : 31.9671 Intercept : 4.2461 Correlation Coefficient : 0.9981
2	2.1	0.980	36	
3	2.7	1.109	40	
4	3.4	1.241	44	
5	4.2	1.377	48	

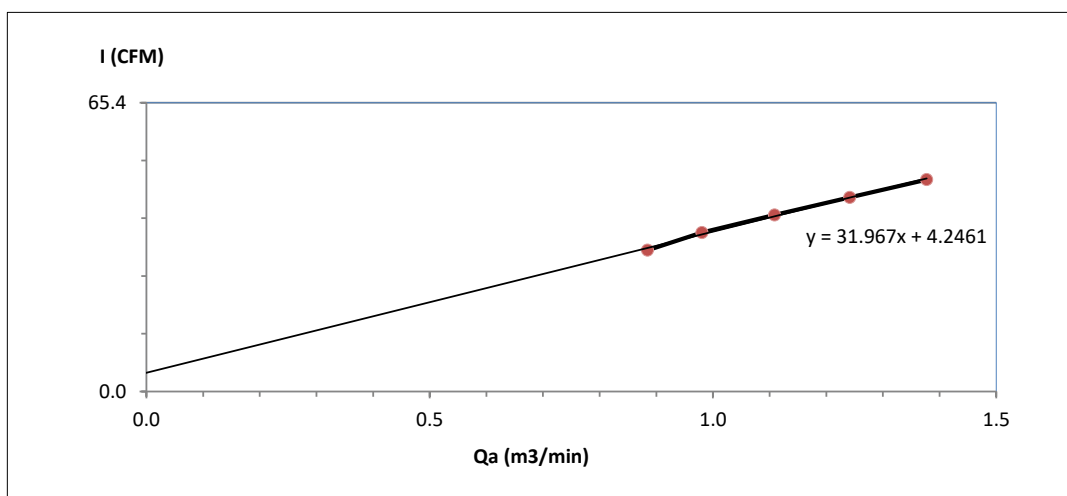

Calibrated by Anurak T.  
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by : Noppong J.  
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)





### High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	วัดหุบบอนวนาราม (A3)	Temperature ( °C) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0183
CalibrationSheet No.:	C-270924-RYG_FS0183	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	4791
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95561
Calibrator S/N :	1166	Calibrator Intercept :	-0.02266

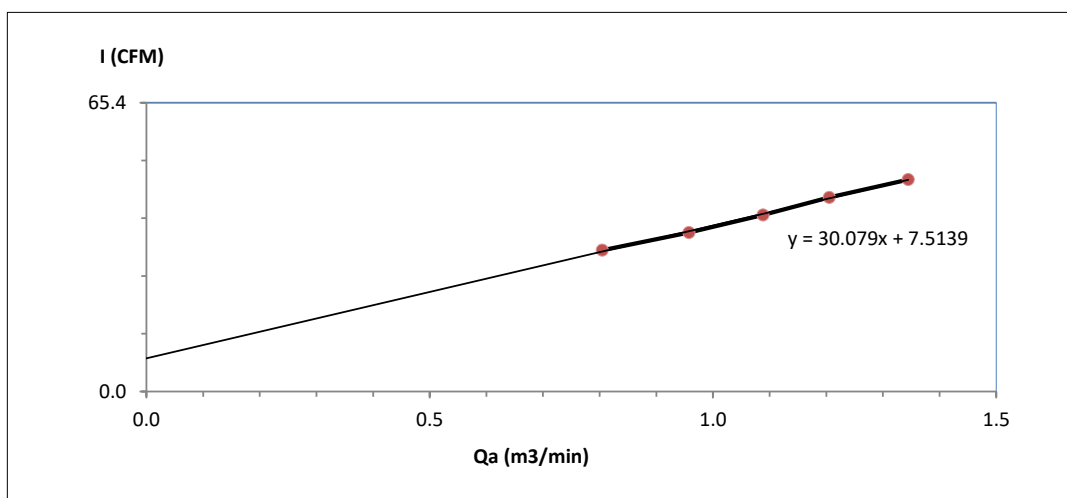Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	1.4	0.805	32	Slope : 30.0790 Intercept : 7.5139 Correlation Coefficient : 0.9991
2	2.0	0.957	36	
3	2.6	1.088	40	
4	3.2	1.205	44	
5	4.0	1.345	48	



Calibrated by   
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)





## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	วัดบ่อวิน (A4)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0667
CalibrationSheet No.:	C-270924-RYG_FS0667	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	6266
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95561
Calibrator S/N :	1166	Calibrator Intercept :	-0.02266

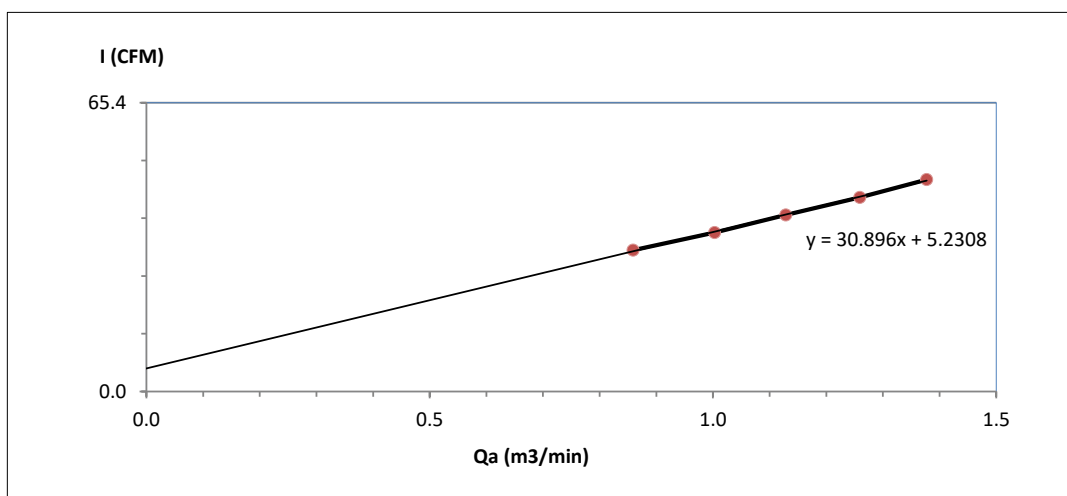Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	1.6	0.859	32	Slope : 30.8960 Intercept : 5.2308 Correlation Coefficient : 0.9994
2	2.2	1.003	36	
3	2.8	1.129	40	
4	3.5	1.259	44	
5	4.2	1.377	48	



Calibrated by   
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)





### High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	วัดพันเสด็จนอก (A5)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0189
CalibrationSheet No.:	C-270924-RYG_FS0189	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	4797
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95561
Calibrator S/N :	1166	Calibrator Intercept :	-0.02266

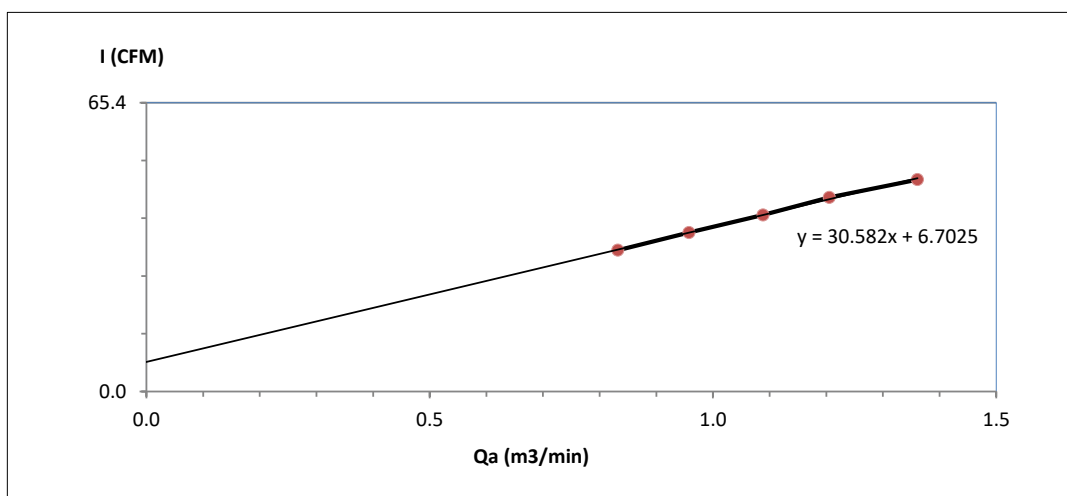Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	1.5	0.832	32	Slope : 30.5818 Intercept : 6.7025 Correlation Coefficient : 0.9990
2	2.0	0.957	36	
3	2.6	1.088	40	
4	3.2	1.205	44	
5	4.1	1.361	48	



Calibrated by   
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)





### High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	ชุมชนห้วยเหียน (A6)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0665
CalibrationSheet No.:	C-270924-RYG_FS0665	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	6264
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95561
Calibrator S/N :	1166	Calibrator Intercept :	-0.02266

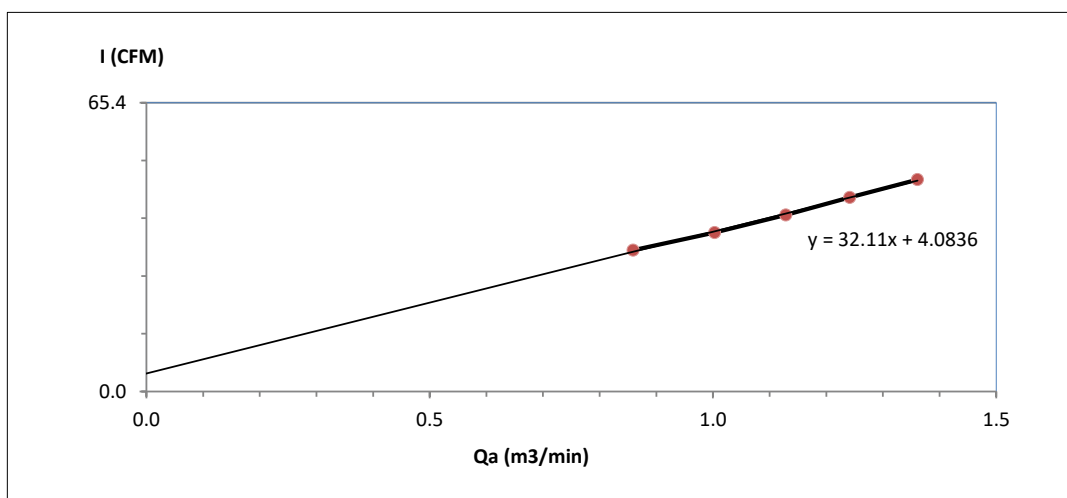Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	1.6	0.859	32	Slope : 32.1095 Intercept : 4.0836 Correlation Coefficient : 0.9989
2	2.2	1.003	36	
3	2.8	1.129	40	
4	3.4	1.241	44	
5	4.1	1.361	48	



Calibrated by   
( Mr.Anurak Tongkhajonsakda )  
Field Scientist(2)


Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)





## High Volume Air Sampler Calibration Worksheet

Project Site :	Glow IPP Co., Ltd.	Barometric Pressure (mm Hg) :	757
Calibrate Location :	บ้านนาบว (A7)	Temperature ( °C ) :	29
Calibrate Date :	27-Sep-24	High Volume ID :	RYG_FS0398
Calibration Sheet No.:	C-270924-RYG_FS0398	High Volume Model :	TE-5009X
Calibrator ID:	RYG_FS0205	High Volume S/N :	5684
Calibrator Model :	TE-5028A	Calibrator Slope :	0.95561
Calibrator S/N :	1166	Calibrator Intercept :	-0.02266

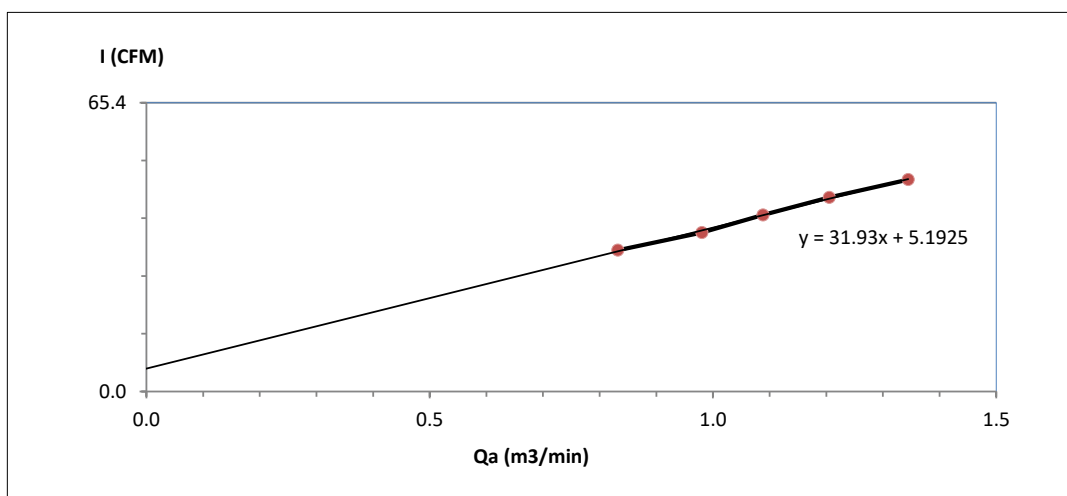Test No.	Delta H <sub>2</sub> O (inch)	Qa (m <sup>3</sup> /min)	I : Chart (CFM)	Linear Regression
1	1.5	0.832	32	Slope : 31.9296 Intercept : 5.1925 Correlation Coefficient : 0.9986
2	2.1	0.980	36	
3	2.6	1.088	40	
4	3.2	1.205	44	
5	4.0	1.345	48	



Calibrated by   
( Mr. Anurak Tongkhajonsakda )  
Field Scientist(2)

Approved by :   
(Mr. Noppong Juntarupan)  
Enviro Field Coordinator Scientist (3)




## MULTIPOINT CALIBRATION REPORT

Calibration Date 2-Jul-24  
Manufacturer Teledyne API  
Serial No. 2197  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 55.88  
Cylinder Pressure (psi) 1800  
Certified Date 9-Feb-22

Equipment Name NOx Analyzer  
Model T200  
Equipment ID RYG\_FS0255  
Model 700  
Cylinder No. GN0027222  
Certified By Airgas Inc.  
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.60	-0.40	-0.40	100.10	0.10	0.10
2	200.00	198.00	-2.00	-1.00	198.70	-1.30	-0.65
3	300.00	297.30	-2.70	-0.90	298.70	-1.30	-0.43
4	400.00	396.40	-3.60	-0.90	398.80	-1.20	-0.30
AVERAGE (%)				-0.62			-0.24

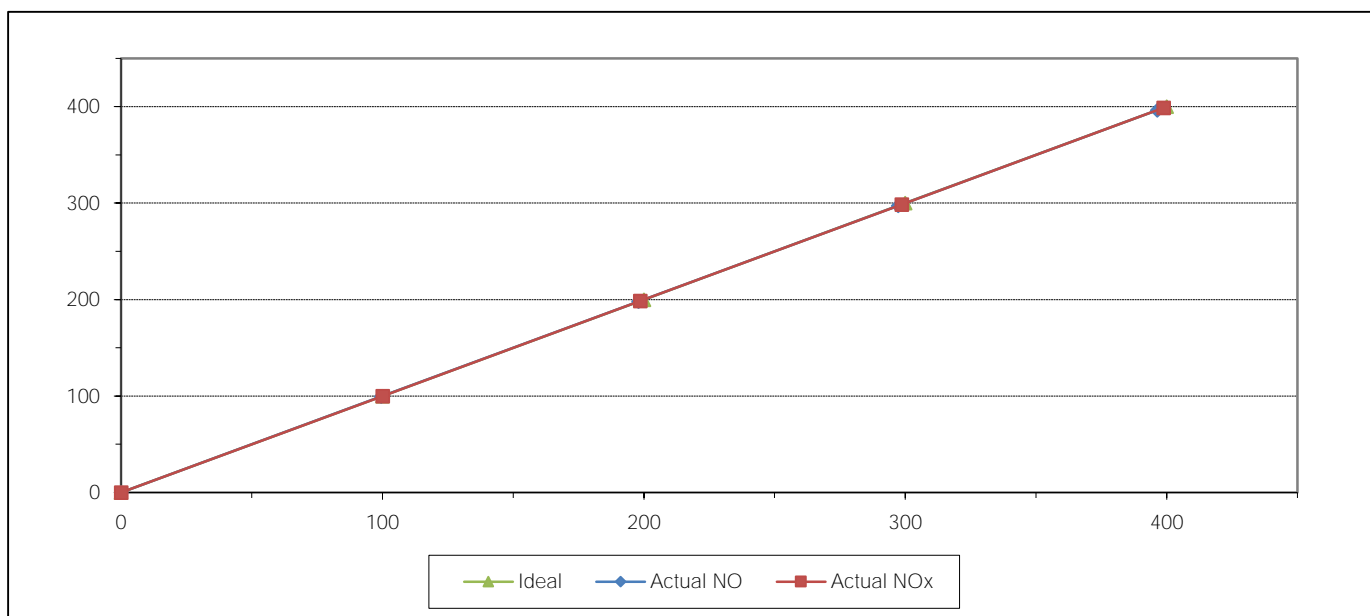

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jittranont )  
Assistant General Manager






## MULTIPOINT CALIBRATION REPORT

Calibration Date 2-Jul-24  
Manufacturer HORIBA  
Serial No. 7AV89544  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 55.88  
Cylinder Pressure (psi) 1800  
Certified Date 9-Feb-22

Equipment Name NOx Analyzer  
Model APNA-370  
Equipment ID RYG\_FS0272  
Model 700  
Cylinder No. GN0027222  
Certified By Airgas Inc.  
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.05	0.05	0.05	0.10	0.10	0.10
1	100.00	99.10	-0.90	-0.90	100.10	0.10	0.10
2	200.00	198.50	-1.50	-0.75	199.20	-0.80	-0.40
3	300.00	298.60	-1.40	-0.47	300.50	0.50	0.17
4	400.00	398.10	-1.90	-0.47	398.70	-1.30	-0.33
AVERAGE (%)				-0.51			-0.07

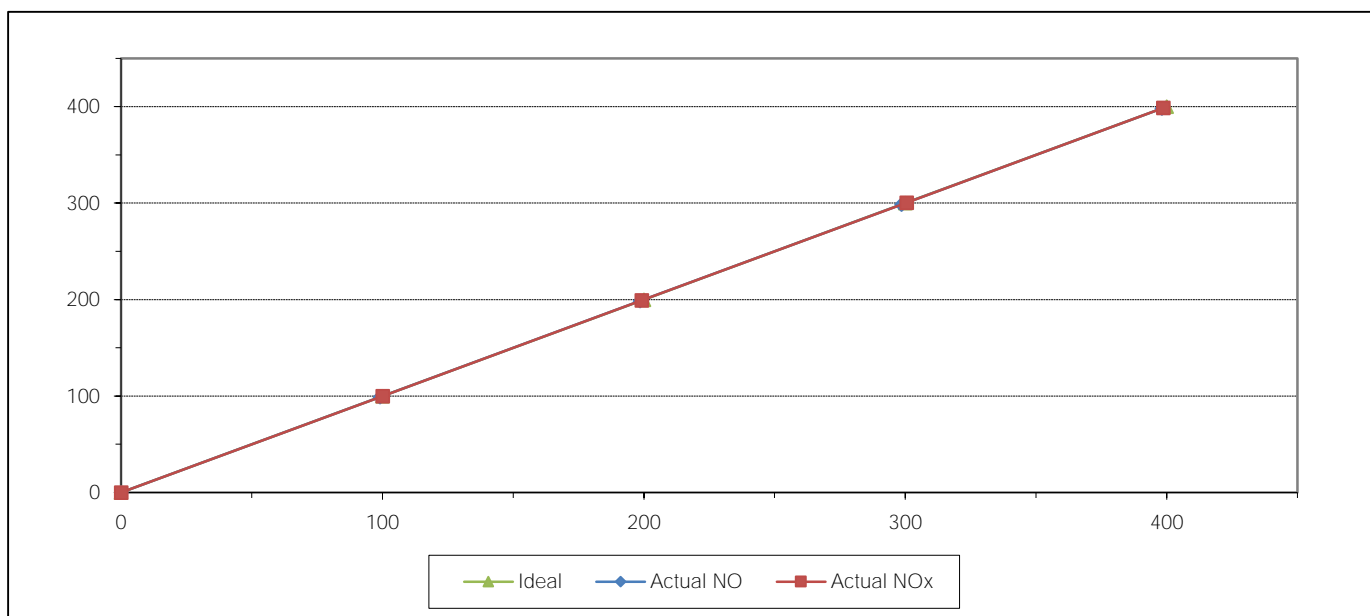

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jittranont )  
Assistant General Manager




## MULTIPOINT CALIBRATION REPORT

Calibration Date 3-Jul-24  
Manufacturer HORIBA  
Serial No. T2T8YRLL  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 55.88  
Cylinder Pressure (psi) 1800  
Certified Date 9-Feb-22

Equipment Name NOx Analyzer  
Model APNA-370  
Equipment ID RYG\_FS0457  
Model 700  
Cylinder No. GN0027222  
Certified By Airgas Inc.  
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	98.30	-1.70	-1.70	100.30	0.30	0.30
2	200.00	198.40	-1.60	-0.80	199.80	-0.20	-0.10
3	300.00	297.90	-2.10	-0.70	298.50	-1.50	-0.50
4	400.00	398.60	-1.40	-0.35	400.80	0.80	0.20
AVERAGE (%)				-0.69			0.00

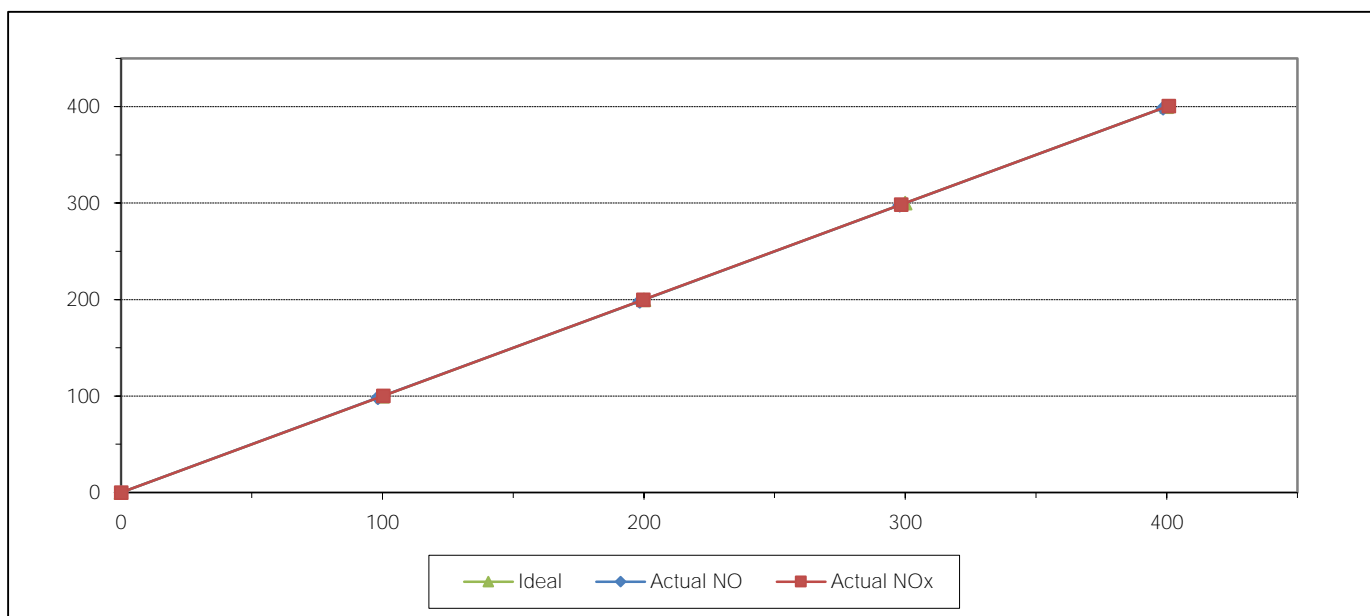

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jittranont )  
Assistant General Manager




## MULTIPOINT CALIBRATION REPORT

Calibration Date 3-Jul-24  
Manufacturer Teledyne API  
Serial No. 7238  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 55.88  
Cylinder Pressure (psi) 1800  
Certified Date 9-Feb-22

Equipment Name NOx Analyzer  
Model T200  
Equipment ID RYG\_FS0533  
Model 700  
Cylinder No. GN0027222  
Certified By Airgas Inc.  
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.50	-0.50	-0.50	101.10	1.10	1.10
2	200.00	198.90	-1.10	-0.55	201.20	1.20	0.60
3	300.00	298.80	-1.20	-0.40	301.10	1.10	0.37
4	400.00	398.30	-1.70	-0.42	401.80	1.80	0.45
AVERAGE (%)				-0.35			0.52

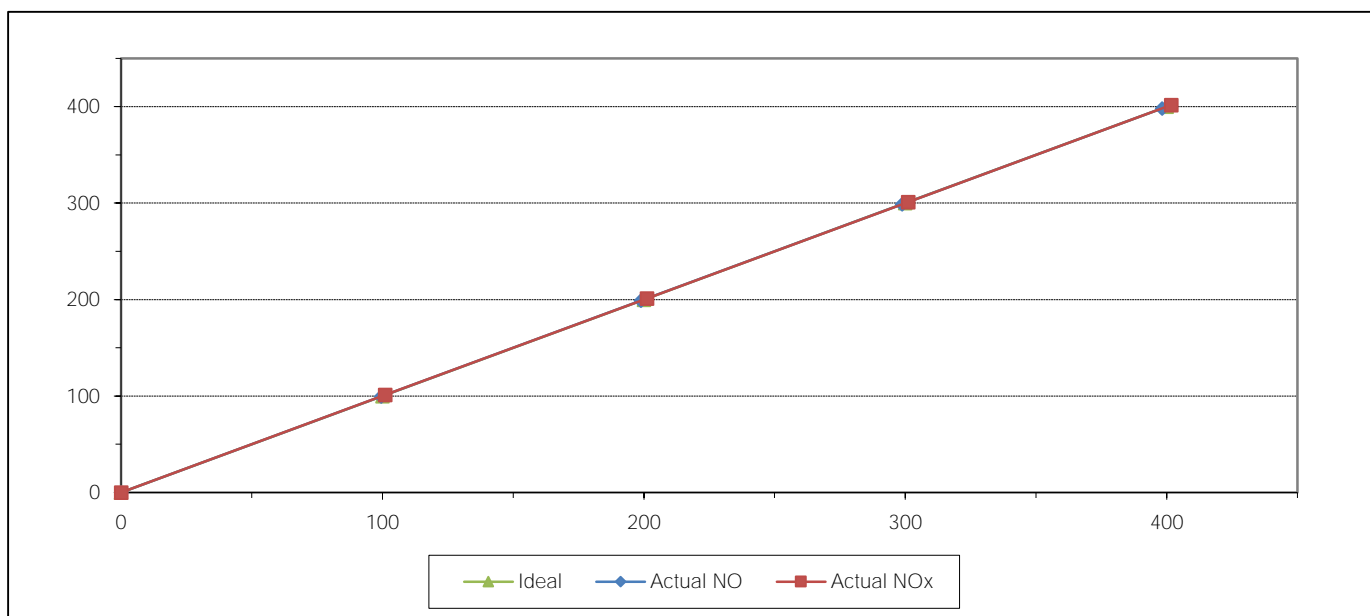

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jittranont )  
Assistant General Manager




## MULTIPOINT CALIBRATION REPORT

Calibration Date 2-Jul-24  
Manufacturer HORIBA  
Serial No. H73KYD1M  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 55.88  
Cylinder Pressure (psi) 1800  
Certified Date 9-Feb-22

Equipment Name NOx Analyzer  
Model APNA-370  
Equipment ID BKK\_FS0797  
Model 700  
Cylinder No. GN0027222  
Certified By Airgas Inc.  
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.70	-0.30	-0.30	101.00	1.00	1.00
2	200.00	198.60	-1.40	-0.70	201.30	1.30	0.65
3	300.00	299.10	-0.90	-0.30	299.70	-0.30	-0.10
4	400.00	402.10	2.10	0.53	399.50	-0.50	-0.13
AVERAGE (%)				-0.13			0.31

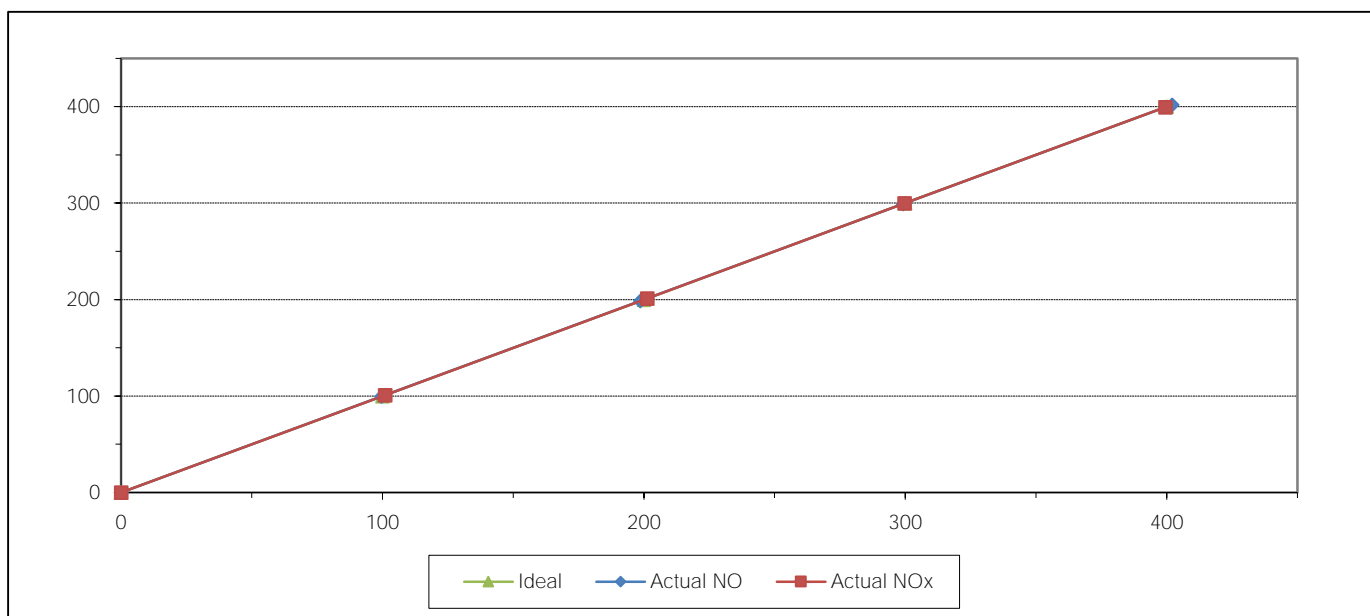

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jittranont )  
Assistant General Manager




## MULTIPOINT CALIBRATION REPORT

Calibration Date 3-Jul-24  
Manufacturer HORIBA  
Serial No. AWXG87CR  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 55.88  
Cylinder Pressure (psi) 1800  
Certified Date 9-Feb-22

Equipment Name NOx Analyzer  
Model APNA-370  
Equipment ID RYG\_FS0453  
Model 700  
Cylinder No. GN0027222  
Certified By Airgas Inc.  
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	99.60	-0.40	-0.40	101.10	1.10	1.10
2	200.00	198.60	-1.40	-0.70	199.80	-0.20	-0.10
3	300.00	299.00	-1.00	-0.33	298.60	-1.40	-0.47
4	400.00	401.10	1.10	0.28	401.10	1.10	0.28
AVERAGE (%)				-0.21			0.18

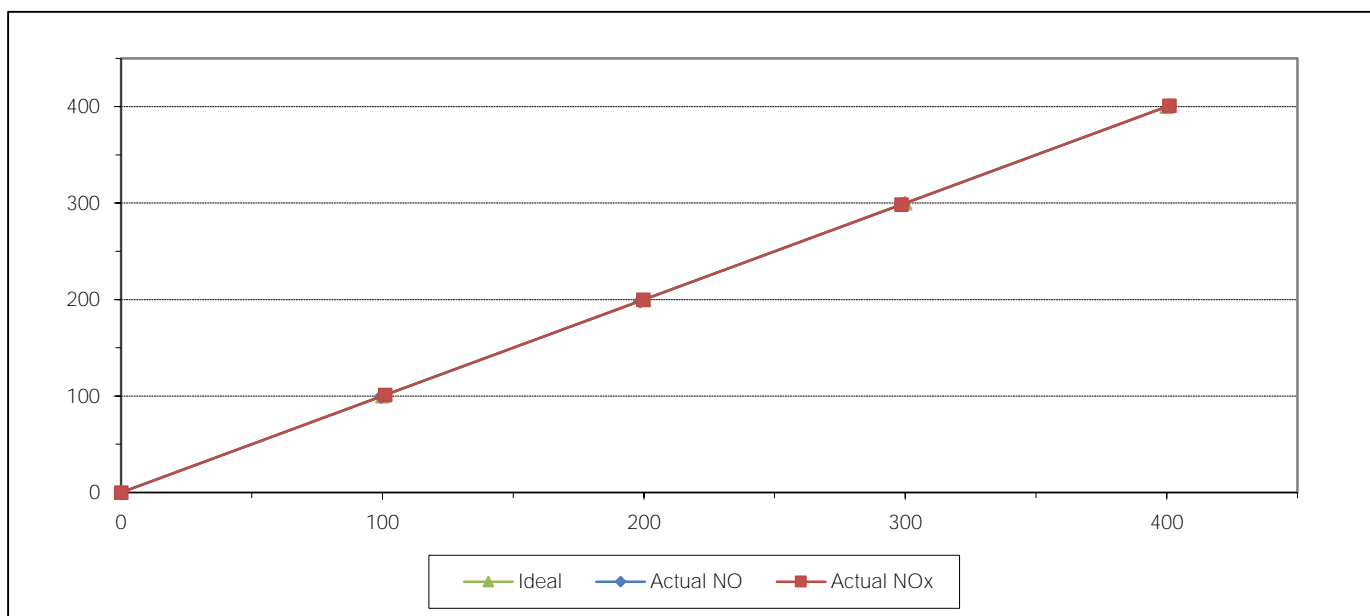

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jittranont )  
Assistant General Manager




## MULTIPOINT CALIBRATION REPORT

Calibration Date 3-Jul-24  
Manufacturer HORIBA  
Serial No. R06K0177  
Calibrator Manufacturer Teledyne API  
Serial No. 947  
Std. Gas Concentration (PPM) 55.88  
Cylinder Pressure (psi) 1800  
Certified Date 9-Feb-22

Equipment Name NOx Analyzer  
Model APNA-370  
Equipment ID RYG\_FS0463  
Model 700  
Cylinder No. GN0027222  
Certified By Airgas Inc.  
Expired Date 9-Feb-30

Point	CALIBRATION RESULTS						
	Ideal	Actual NO	Error NO	%Error NO	Actual NOx	Error NOx	%Error NOx
ZERO	0.00	0.10	0.10	0.10	0.10	0.10	0.10
1	100.00	98.80	-1.20	-1.20	101.30	1.30	1.30
2	200.00	201.30	1.30	0.65	201.20	1.20	0.60
3	300.00	299.40	-0.60	-0.20	302.60	2.60	0.87
4	400.00	398.70	-1.30	-0.33	401.50	1.50	0.38
AVERAGE (%)				-0.20			0.65

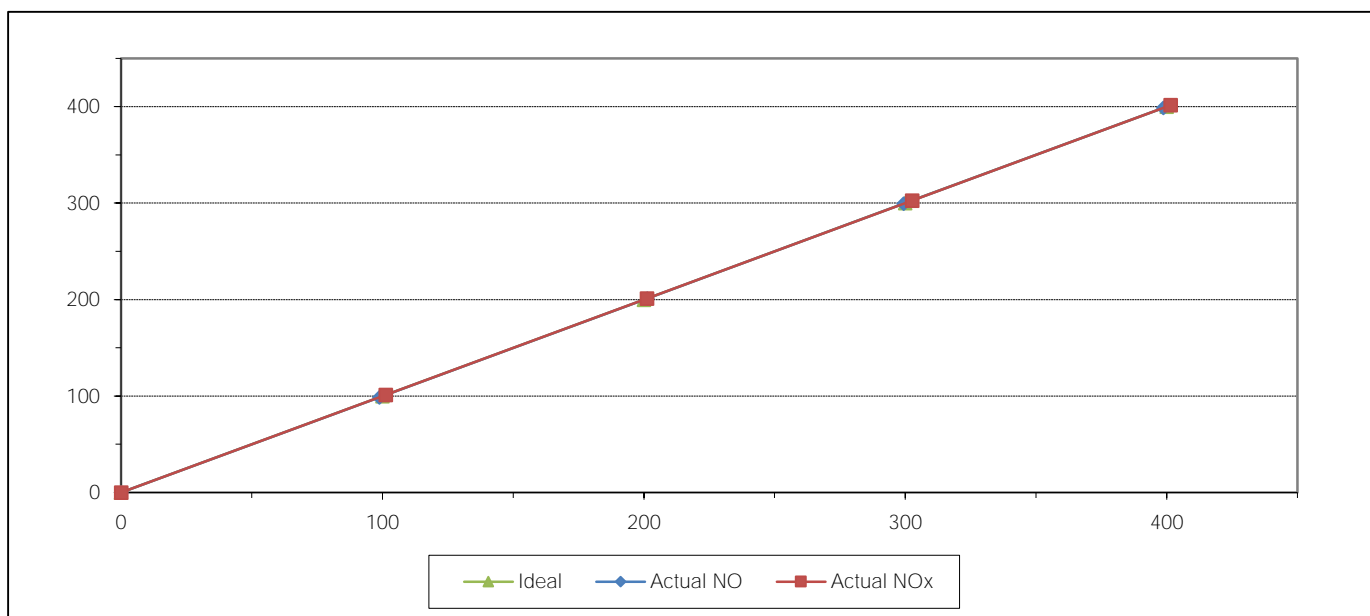

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By


( Mr.Sarayuth Jittranont )  
Assistant General Manager



## MULTIPOINT CALIBRATION REPORT

Calibration Date	4-Jul-24	Equipment Name	SO2 Analyzer
Manufacturer	Teledyne API	Model	T100
Serial No.	1772	Equipment ID	RYG_FS0254
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.05	0.05	0.05
1	100.00	99.00	-1.00	-1.00
2	200.00	199.60	-0.40	-0.20
3	300.00	297.50	-2.50	-0.83
4	400.00	398.90	-1.10	-0.28
AVERAGE (%)				-0.45

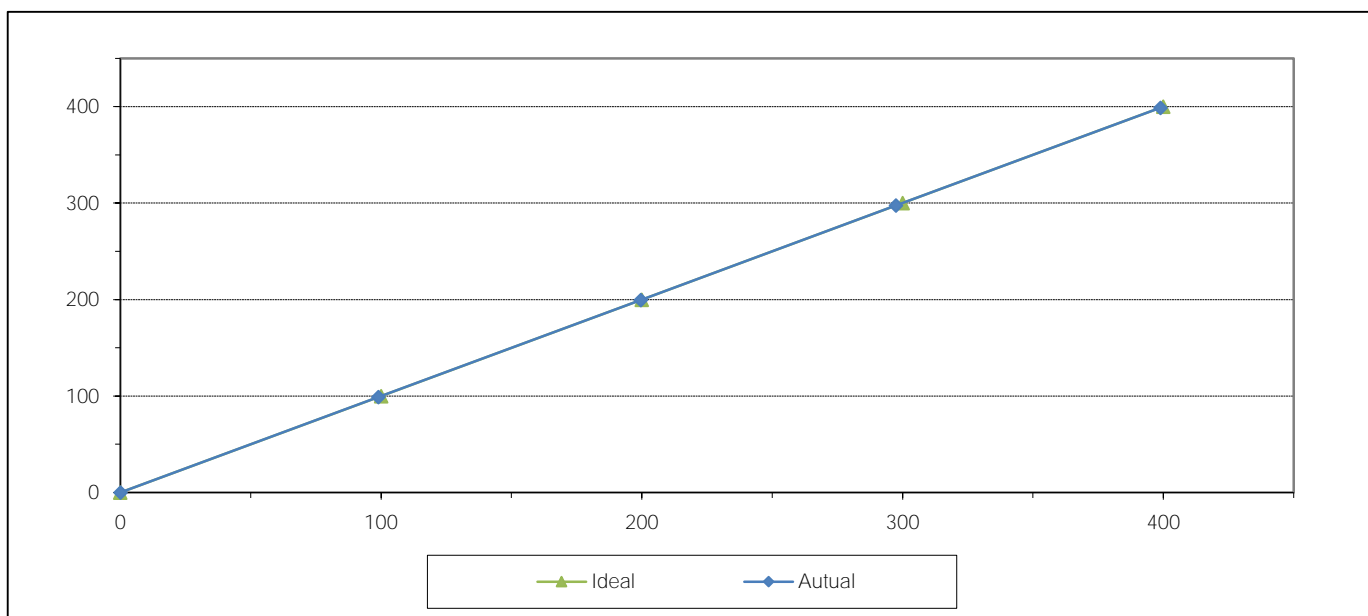

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By


( Mr.Sarayuth Jittranont )  
Assistant General Manager



## MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jul-24	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	VABF9LSH	Equipment ID	RYG_FS0460
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.70	-1.30	-1.30
2	200.00	198.80	-1.20	-0.60
3	300.00	296.90	-3.10	-1.03
4	400.00	398.20	-1.80	-0.45
AVERAGE (%)				-0.66

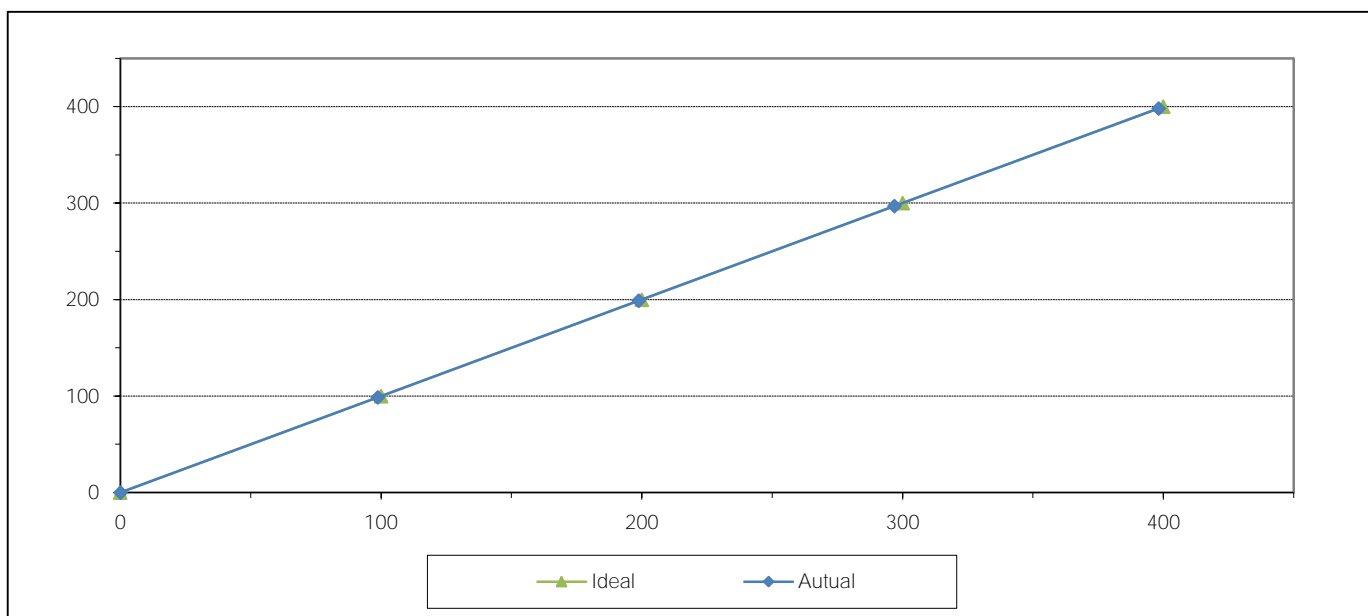

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jittranont )  
Assistant General Manager






## MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jul-24	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	R0HWYDVW	Equipment ID	RYG_FS0456
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	99.70	-0.30	-0.30
2	200.00	199.50	-0.50	-0.25
3	300.00	298.00	-2.00	-0.67
4	400.00	398.80	-1.20	-0.30
AVERAGE (%)				-0.28

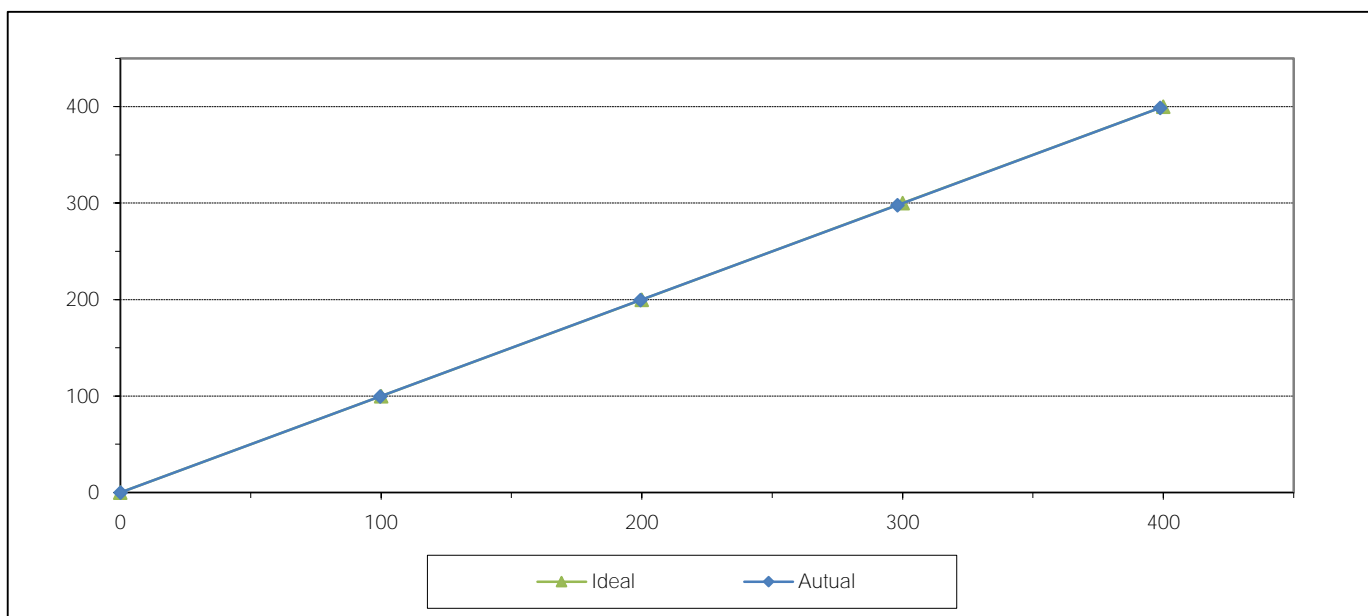

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By


( Mr.Sarayuth Jittranont )  
Assistant General Manager



## MULTIPOINT CALIBRATION REPORT

Calibration Date	4-Jul-24	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	G2CH436B	Equipment ID	BKK_FS0796
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.05	0.05	0.05
1	100.00	98.91	-1.09	-1.09
2	200.00	198.10	-1.90	-0.95
3	300.00	298.00	-2.00	-0.67
4	400.00	398.50	-1.50	-0.38
AVERAGE (%)				-0.61

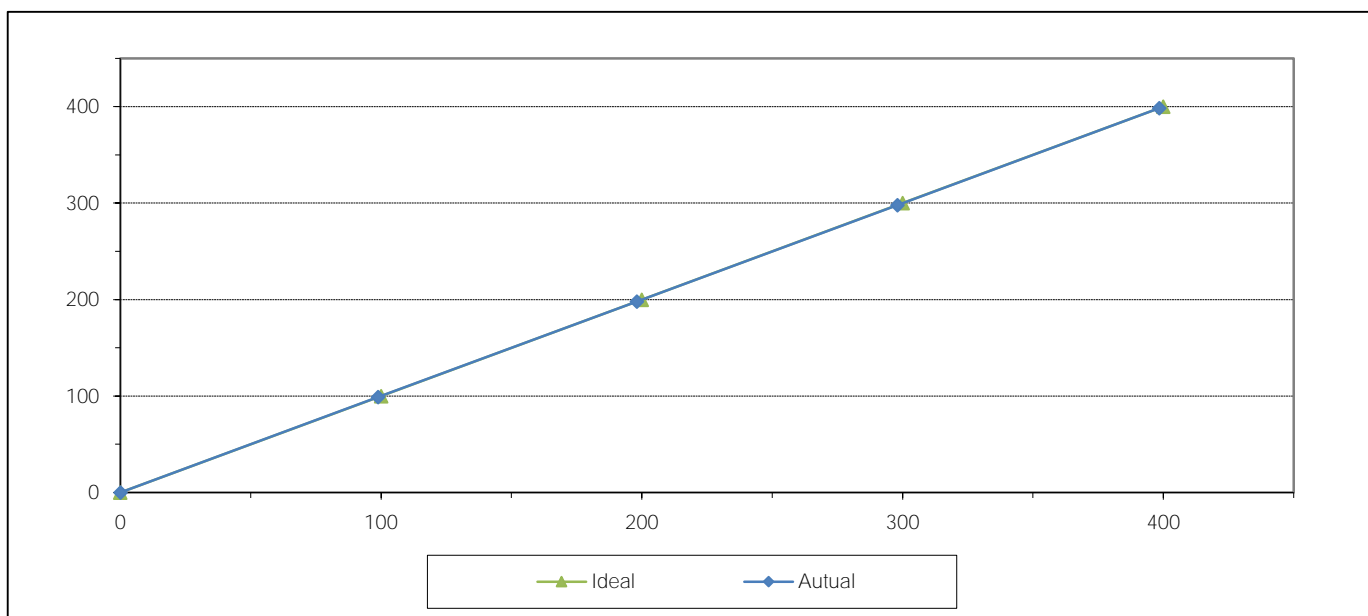

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By


( Mr.Sarayuth Jittranont )  
Assistant General Manager



## MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jul-24	Equipment Name	SO2 Analyzer
Manufacturer	Teledyne API	Model	T100
Serial No.	6061	Equipment ID	RYG_FS0534
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.90	-1.10	-1.10
2	200.00	198.70	-1.30	-0.65
3	300.00	298.30	-1.70	-0.57
4	400.00	398.70	-1.30	-0.33
AVERAGE (%)				-0.51

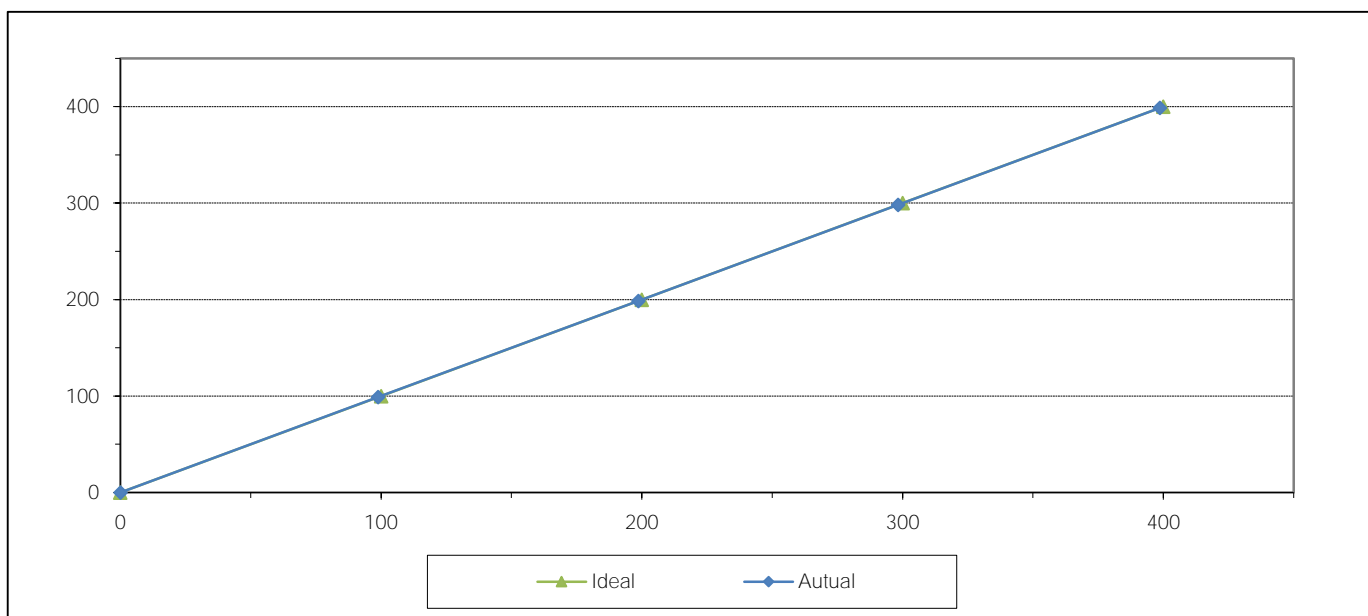

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By


( Mr.Sarayuth Jittranont )  
Assistant General Manager



## MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jul-24	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	90U0XJ31	Equipment ID	RYG_FS0452
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	98.60	-1.40	-1.40
2	200.00	198.00	-2.00	-1.00
3	300.00	298.00	-2.00	-0.67
4	400.00	398.50	-1.50	-0.38
AVERAGE (%)				-0.67

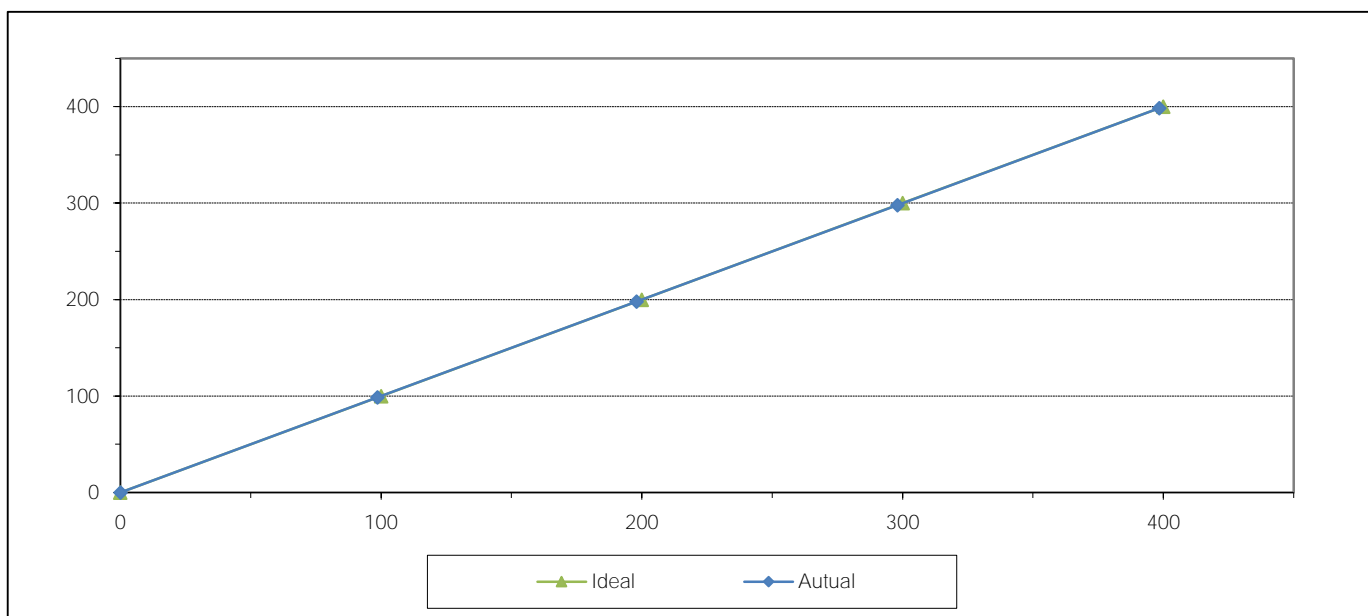

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By


( Mr.Sarayuth Jittranont )  
Assistant General Manager



## MULTIPOINT CALIBRATION REPORT

Calibration Date	5-Jul-24	Equipment Name	SO2 Analyzer
Manufacturer	HORIBA	Model	APSA-370
Serial No.	XL29Y85B	Equipment ID	RYG_FS0462
Calibrator Manufacturer	Teledyne API	Model	700
Serial No.	947		
Std. Gas Concentration (PPM)	56.3	Cylinder No.	GN0027222
Cylinder Pressure (psi)	1800	Certified By	Airgas Inc.
Certified Date	9-Feb-22	Expired Date	9-Feb-30

Point	CALIBRATION RESULTS			
	Ideal	Autual	Error	%Error
ZERO	0.00	0.10	0.10	0.10
1	100.00	99.10	-0.90	-0.90
2	200.00	198.00	-2.00	-1.00
3	300.00	299.90	-0.10	-0.03
4	400.00	403.20	3.20	0.80
AVERAGE (%)				-0.21

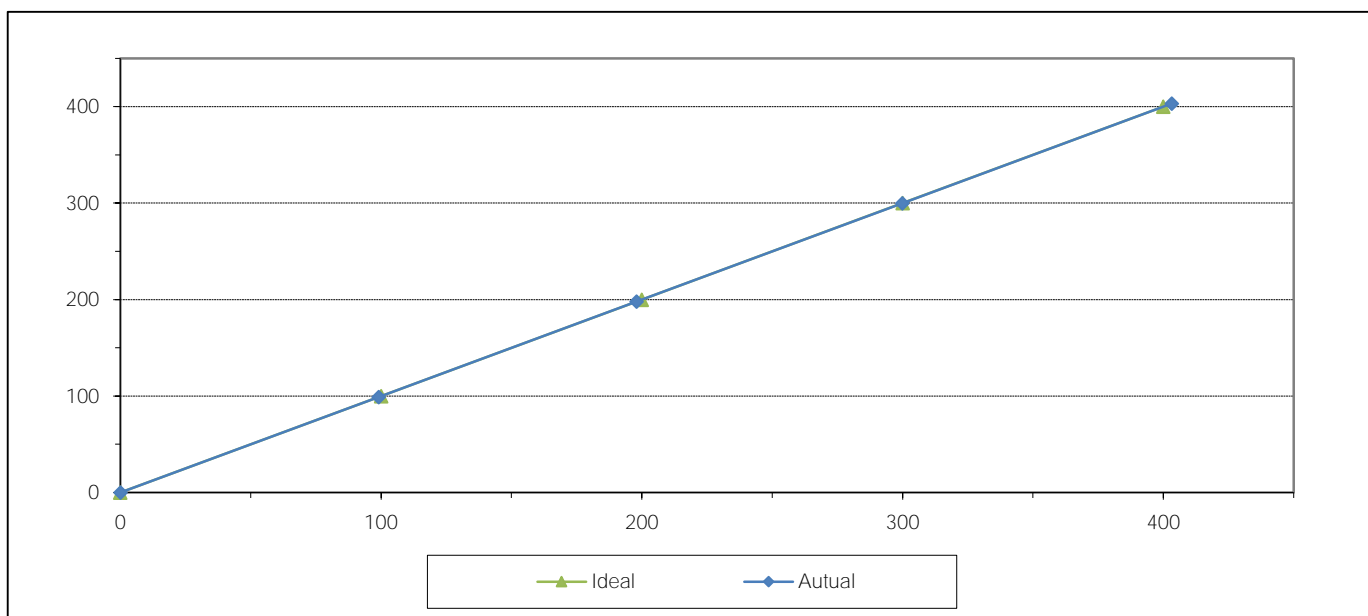

Calibrated By

( Mr.Jirawut Sakarn )  
Field Environmental Scientist (3)

Approved By

( Mr.Sarayuth Jittranont )  
Assistant General Manager

Certificate Number

CWS-030-67

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Cup anemometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: WS-25DL  
**SERIAL NUMBER** : Sensor: WSD-A4562  
Data logger: A4562  
**ID NUMBER** : BKK\_FS0143  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 08 Aug 2024  
**MEASUREMENT DATE** : 20 Aug 2024  
**ISSUE DATE** : 20 Aug 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITIONS</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Wind direction frontal area <sup>2</sup>	100	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.111	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (24.2) °C, (41.9) %RH and (1007.9) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

REVIEW BY .....  
APPROVED BY .....  
NEXT CAL. DATE 20/2/26

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>



MEASUREMENT RESULTS <sup>5</sup>

The Cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

$V_{std}$ <sup>6</sup> (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$V_{uuc}$ <sup>7</sup> (m/s)	Error (m/s)	$U (k=2)$ (m/s)
0.999	23.98	24.20	0.9	-0.1	0.31
2.043	24.42	24.20	1.8	-0.2	0.31
2.982	23.80	24.20	2.9	-0.1	0.31
4.108	23.82	24.20	3.8	-0.3	0.31
4.97	23.62	24.20	4.9	-0.1	0.31
5.95	23.94	24.20	6.0	0.0	0.31
7.01	23.46	24.20	7.0	0.0	0.31
7.96	23.80	24.20	8.0	0.0	0.31
8.98	23.90	24.20	9.1	0.1	0.31
9.96	23.74	24.20	10.1	0.1	0.31
10.94	24.00	24.20	11.1	0.2	0.31
12.01	23.82	24.20	12.2	0.2	0.31
12.92	24.00	24.20	13.1	0.2	0.31
14.06	23.86	24.20	14.2	0.2	0.31
15.00	24.00	24.20	15.2	0.2	0.31
15.93	23.96	24.20	16.2	0.2	0.31


## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Velocity of standard

<sup>7</sup> Velocity of Unit Under Calibration

## PHOTO OF CALIBRATION SET-UP

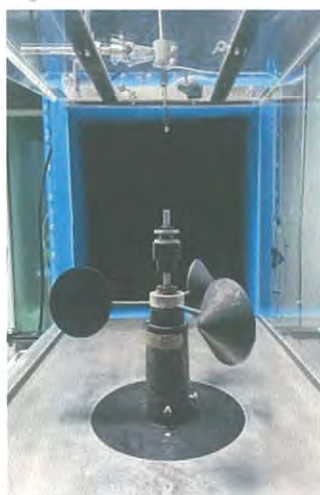

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

\*\*\*End of Certificate of Calibration\*\*\*

NAC

JIRANATEE ASSOCIATES CO., LTD.

Certificate Number

CWD-030-67

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Wind Direction Sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: WS-25DL  
**SERIAL NUMBER** : Sensor: WSD-A4562  
Data logger: A4562  
**ID NUMBER** : BKK\_FS0143  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 08 Aug 2024  
**MEASUREMENT DATE** : 20 Aug 2024  
**ISSUE DATE** : 20 Aug 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITION</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Wind direction frontal area <sup>2</sup>	129	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.143	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (23.7)°C, (42.6) %RH and (1007.9) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>



MEASUREMENT RESULTS <sup>5</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D^{\circ}_{std}$ Degree (°)	$D^{\circ}_{uuc}$ Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.01	45.000	41	-4	0.80
	90.000	87	-3	0.80
	135.000	132	-3	0.80
	180.000	181	1	0.80
	225.000	229	4	0.80
	270.000	275	5	0.80
	315.000	320	5	0.80
	360.000	359	-1	0.80

## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Direction of standard

<sup>7</sup> Direction of Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.



NSC – TISI – TIS 17025  
CALIBRATION 0367

Certificate Number

CWS-025-67

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Cup anemometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-A5909  
Data logger: A5909  
**ID NUMBER** : RYG\_FS0608  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 08 Jul 2024  
**MEASUREMENT DATE** : 18 Jul 2024  
**ISSUE DATE** : 18 Jul 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure :  $1010 \pm 10$  hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

**CALIBRATION CONDITIONS** : Wind tunnel cross-section area<sup>1</sup> 900 cm<sup>2</sup>  
Wind direction frontal area<sup>2</sup> 100 cm<sup>2</sup>  
Diameter of mounting pipe<sup>3</sup> - mm  
Blockage ratio of test object<sup>4</sup> 0.111 [-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (24.5) °C, (43.4) %RH and (1006.7) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

### Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm<sup>2</sup> cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

### Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0055-23

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY

Narakorn P.

APPROVED BY

Nichol

NEXT CAL. DATE

48/1/26

Approved signatory:

Mr. Parinya Booncharoen

Calibration Department Manager



MEASUREMENT RESULTS<sup>5</sup>

The Cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

$v_{std}$ <sup>6</sup> (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$v_{uuc}$ <sup>7</sup> (m/s)	Error (m/s)	$U (k=2)$ (m/s)
0.997	24.78	24.45	0.8	-0.2	0.31
2.014	24.20	24.45	1.8	-0.2	0.31
2.990	24.80	24.45	2.9	-0.1	0.31
4.102	24.80	24.45	3.8	-0.3	0.31
4.97	24.80	24.45	5.0	0.0	0.31
5.98	24.50	24.45	6.0	0.0	0.31
7.03	24.70	24.45	7.1	0.1	0.31
7.95	24.38	24.45	8.1	0.1	0.31
9.04	24.70	24.45	9.1	0.1	0.31
9.98	24.36	24.45	10.2	0.2	0.31
10.99	24.80	24.45	11.2	0.2	0.31
12.03	24.40	24.45	12.2	0.2	0.31
12.97	24.70	24.45	13.2	0.2	0.31
14.10	24.50	24.45	14.3	0.2	0.31
15.03	24.70	24.45	15.2	0.2	0.31
15.99	24.58	24.45	16.2	0.2	0.31

## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Velocity of standard

<sup>7</sup> Velocity of Unit Under Calibration

## PHOTO OF CALIBRATION SET-UP



Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.



Certificate Number

CWD-025-67

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Wind Direction Sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-A5909  
Data logger: A5909  
**ID NUMBER** : RYG\_FS0608  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 08 Jul 2024  
**MEASUREMENT DATE** : 18 Jul 2024  
**ISSUE DATE** : 18 Jul 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITION</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Wind direction frontal area <sup>2</sup>	129	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.143	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (22.4)°C, (43.3) %RH and (1004.5) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

### Calibration procedure:

The wind direction sensor was calibrated against Standard Rotary Encoder model: AX4009TS-DM04-P3-S-U0 in an close test-section of Eiffel-type wind tunnel with 900 cm<sup>2</sup> cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

### Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0036-23.

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'



MEASUREMENT RESULTS<sup>5</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D^{\text{std}}$ Degree (°)	$D^{\text{uuc}}$ Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.04	0.000	0	0	0.80
	45.000	41	-4	0.80
	90.000	87	-3	0.80
	135.000	132	-3	0.80
	180.000	178	-2	0.80
	225.000	225	0	0.80
	270.000	272	2	0.80
	315.000	319	4	0.80

## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Direction of standard

<sup>7</sup> Direction of Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Temperature measurement laboratory  
Calibration services department.



NSC – TISI – TIS 17025  
CALIBRATION 0367

## CERTIFICATE OF CALIBRATION

Certificate No. : CDT-120-67

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Data Logger with Temperature sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : 110-WS-25DL-D  
**SERIAL NUMBER** : A5909  
**ID NUMBER** : RYG\_FS0608  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Suan Luang, Khet Suan Luang,  
Bangkok 10250 Thailand.

**RECEIVED DATE** : 08 Jul 2024  
**MEASUREMENT DATE** : 18 Jul 2024  
**ISSUE DATE** : 18 Jul 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH

**NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

### Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: ER-0101-23

### Reference Used During Calibration:


1. Standard Temperature Probe  
Model: STS-100 A500, Serial No.: 667682-09,  
Due date: 26 Mar 2025
2. Digital Temperature Indicator  
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor  $k=2$ , Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

### Calibrated by:

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jittraporn Lertsomphol  
☐ Miss Ruangrumpai Phoommit

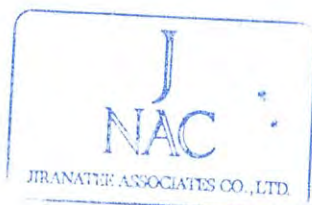

Approved signatory: \_\_\_\_\_

Mr. Parinya Booncharoen  
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number CDT-120-67

Page 2 of 2 Pages

**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20 °C to 40 °C

**Function:**

Table 3: This equipment was connected with temperature sensor Model: HMP60 S/N: U3641220.  
Dimension: Diameter 12 mm. Length 80 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
80	20.047	19.8	-0.2	0.099
80	25.043	24.8	-0.2	0.099
80	30.034	29.8	-0.2	0.099
80	35.028	34.8	-0.2	0.099
80	40.018	39.7	-0.3	0.16

**UUC\*:** Unit Under Calibration

**Remark:** The reported uncertainty of measurement is 0.16, based on standard uncertainty multiplied by a coverage factor k=2.21 providing a level of confidence of approximately 95%.

\*\*\*End of Certificate of Calibration\*\*\*







JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Relative humidity and Air Temperature measurement laboratory  
Calibration services department.

## CERTIFICATE OF CALIBRATION

Certificate No. : CRT-022-67

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Relative humidity with data logger  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Data Logger: 110-WS-25DL-D  
Sensor: HMP60  
**SERIAL NUMBER** : Data Logger: A5909  
Sensor: U3641220  
**ID NUMBER** : RYG\_FS0608  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 08 Jul 2024  
**MEASUREMENT DATE** : 18 Jul 2024  
**ISSUE DATE** : 18 Jul 2024

**Calibration procedure:**

The Relative humidity and Air Temperature calibration was done by In-House calibration method as WI-CL-009 and WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

**Traceability:**

The measurements are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT). Certificate number: TH-0079-23 and through Jiranatee Associates Co., Ltd. Certificate number: CDT-001-67.

**Uncertainty of Measurement:**

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor  $k=2$ , Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

**ENVIRONMENTAL CONDITIONS:**

Ambient condition in the laboratory are as follow:

Temperature	: $23.0 \pm 3.0$	°C
Relative Humidity	: $55.0 \pm 15.0$	%RH

**NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.

**TABULATION OF RESULTS:**

The table on next page give the measured values.

**Calibrated by:**

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jittraporn Lertsomphol  
☐ Miss Ruangrumpai Phoommit



**Approved signatory:**

Mr. Parinya Booncharoen  
Calibration Department Manager





JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number: CRT-022-67

Page 2 of 2 Pages

**Measurement Results:**

The results of calibration and associated measurement uncertainties are reported in the table below.

**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Table 1:** The results of calibration of relative humidity at 30 °C are reported in table below.

**Calibration Range:** 20%RH to 80%RH

<u>Air Temperature</u> (°C)	<u>Standard Reading</u> (%RH)	<u>UUC Reading</u> (%RH)	<u>Error</u> (%RH)	<u>Uncertainty</u> ± (%RH)
29.79	19.49	17.5	-1.9	0.83
29.82	50.54	47.3	-3.3	1.3
29.81	81.68	77.1	-4.6	2.3

UUC\*: Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

REVIEW BY	Narakorn P
APPROVED BY	[Signature]
NEXT CAL. DATE	18/2/25

Certificate Number

CWS-003-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Cup anemometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 200-WS-25LB  
**SERIAL NUMBER** : Sensor: WSD-A5190  
Data logger: A5190  
**ID NUMBER** : RYG\_FS0329  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 11 Aug 2023  
**MEASUREMENT DATE** : 18 Aug 2023  
**ISSUE DATE** : 21 Aug 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITIONS</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Win direction frontal area <sup>2</sup>	100	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.111	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (24.3) °C, (43.1) %RH and (1005.59) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory: \_\_\_\_\_

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>



**MEASUREMENT RESULTS <sup>5</sup>**

The cup anemometer, Unit Under Calibration (UUC) was exercise at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


$v_{std}^6$ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$v_{uuc}^7$ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.032	24.10	24.30	0.9	-0.1	0.31
2.095	24.54	24.30	1.9	-0.2	0.31
3.006	24.08	24.30	2.9	-0.1	0.31
4.220	24.04	24.30	4.0	-0.2	0.31
5.00	23.78	24.30	4.9	-0.1	0.31
5.97	23.82	24.30	5.9	-0.1	0.31
7.01	23.78	24.30	6.9	-0.1	0.31
8.13	24.00	24.30	8.0	-0.1	0.31
9.07	23.82	24.30	9.0	-0.1	0.31
10.07	23.90	24.30	9.9	-0.1	0.31
11.13	23.84	24.30	11.1	0.0	0.31
12.13	23.80	24.30	12.0	-0.1	0.31
13.19	23.82	24.30	13.2	0.0	0.31
14.24	23.74	24.30	14.1	-0.1	0.31
15.20	23.80	24.30	15.2	0.0	0.33
16.26	23.74	24.30	16.1	-0.2	0.31

**Remark:**

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Velocity of standard

<sup>7</sup> Velocity of Unit Under Calibration

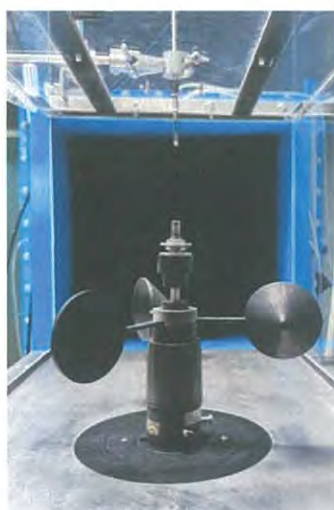**PHOTO OF CALIBRATION SET-UP**

Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

Certificate Number

CWD-003-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Wind Direction Sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 200-WS-25LB  
**SERIAL NUMBER** : Sensor: WSD-A5190  
Data logger: A5190  
**ID NUMBER** : RYG\_FS0329  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 11 Aug 2023  
**MEASUREMENT DATE** : 18 Aug 2023  
**ISSUE DATE** : 21 Aug 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure :  $1010 \pm 10$  hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

**CALIBRATION CONDITION** : Wind tunnel cross-section area<sup>1</sup> 900 cm<sup>2</sup>  
Win direction frontal area<sup>2</sup> 129 cm<sup>2</sup>  
Diameter of mounting pipe<sup>3</sup> - mm  
Blockage ratio of test object<sup>4</sup> 0.143 [-]

**Preconditioning** : 24 hours at ambient conditions.

**Measurement Condition** : The average values during measurement are (23.9)°C, (44.8) %RH and (1009.2) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

<sup>1</sup> Nozzle cross-section area of the wind tunnel

<sup>2</sup> Projected cross-section area of the tested object include mounting pipe

<sup>3</sup> Diameter of mounting pipe

<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>



MEASUREMENT RESULTS<sup>5</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D^{\circ}_{std}$ Degree (°)	$D^{\circ}_{uuc}$ Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.00	45.000	41	-4	1.0
	90.000	87	-3	1.0
	135.001	132	-3	1.0
	180.000	178	-2	1.0
	225.000	226	1	1.0
	270.000	272	2	1.0
	315.000	319	4	1.0
	360.000	359	-1	1.0

## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Direction of standard

<sup>7</sup> Direction of Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*



Certificate Number

CWS-004-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Cup anemometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 200-WS-25LB  
**SERIAL NUMBER** : Sensor: WSD-A5191  
Data logger: A5191  
**ID NUMBER** : RYG\_FS0328  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 11 Aug 2023  
**MEASUREMENT DATE** : 18 Aug 2023  
**ISSUE DATE** : 21 Aug 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure :  $1010 \pm 10$  hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

**CALIBRATION CONDITIONS** : Wind tunnel cross-section area<sup>1</sup> 900 cm<sup>2</sup>  
Win direction frontal area<sup>2</sup> 100 cm<sup>2</sup>  
Diameter of mounting pipe<sup>3</sup> - mm  
Blockage ratio of test object<sup>4</sup> 0.111 [-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (24.1) °C, (44.3) %RH and (1005.44) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>



Certificate Number

CWD-004-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Wind Direction Sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 200-WS-25LB  
**SERIAL NUMBER** : Sensor: WSD-A5191  
Data logger: A5191  
**ID NUMBER** : RYG\_FS0328  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 11 Aug 2023  
**MEASUREMENT DATE** : 18 Aug 2023  
**ISSUE DATE** : 21 Aug 2023

**ENVIRONMENTAL CONDITIONS:**

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITION</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Win direction frontal area <sup>2</sup>	129	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.143	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (23.9)°C, (41.2) %RH and (1009.3) hPa.

**TABULATION OF RESULTS:**

The table on next page give the measured values.

**Calibrated by:**

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

**Remark:**

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

MEASUREMENT RESULTS <sup>5</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D^{6}_{std}$ Degree (°)	$D^{7}_{uuc}$ Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.01	45.000	42	-3	1.0
	90.000	87	-3	1.0
	135.000	133	-2	1.0
	180.000	182	2	1.0
	225.000	229	4	1.0
	270.000	275	5	1.0
	315.000	320	5	1.0
	360.000	359	-1	1.0

## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Direction of standard

<sup>7</sup> Direction of Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*







JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.



NSC – TISI – TIS 17025  
CALIBRATION 0367

Certificate Number

CWS-026-67

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Cup anemometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-A5910  
Data logger: A5910  
**ID NUMBER** : RYG\_FS0609  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 08 Jul 2024  
**MEASUREMENT DATE** : 18 Jul 2024  
**ISSUE DATE** : 18 Jul 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure :  $1010 \pm 10$  hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

**CALIBRATION CONDITIONS** : Wind tunnel cross-section area<sup>1</sup> 900 cm<sup>2</sup>  
Wind direction frontal area<sup>2</sup> 100 cm<sup>2</sup>  
Diameter of mounting pipe<sup>3</sup> - mm  
Blockage ratio of test object<sup>4</sup> 0.111 [-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (23.8) °C, (44.9) %RH and (1003.3) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



### Calibration procedure:

The Cup anemometer was calibrated against Standard air velocity transducer model: 8455-12 and pitot tube with precision differential pressure meter model: DPM2500 in an close test-section of Eiffel-type wind tunnel with 900 cm<sup>2</sup> cross test section area. The WI-CL-007 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

### Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: MW-0007-24 and MW-0055-23

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor  $k=2$ , Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

REVIEW BY *Margalonn P*

APPROVED BY *Wichit Ch*

NEXT CAL. DATE 18/1/26

Approved signatory: *Mr. Parinya Booncharoen*

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

THIS CERTIFICATE OF CALIBRATION MAY NOT BE REPRODUCED EXCEPT IN FULL UNLESS PERMISSION FOR REPRODUCTION HAS BEEN OBTAINED IN WRITING FROM THE LABORATORY

**MEASUREMENT RESULTS <sup>5</sup>**

The Cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section and the standard air velocity 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 50 mm away from wind tunnel nozzle and installed 40 mm away from top of the test section, UUC was mounted on a round vertical tube of the lower plate at center of test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


$v_{std}^6$ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$v_{uuc}^7$ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
0.997	23.70	23.80	0.9	-0.1	0.31
2.021	23.90	23.80	1.8	-0.2	0.31
2.990	23.70	23.80	2.9	-0.1	0.31
4.094	23.70	23.80	3.8	-0.3	0.31
4.97	23.72	23.80	5.0	0.0	0.31
5.97	23.60	23.80	6.0	0.0	0.31
7.04	23.80	23.80	7.0	0.0	0.31
7.98	23.62	23.80	8.0	0.0	0.31
9.00	23.72	23.80	9.1	0.1	0.31
9.98	23.50	23.80	10.1	0.1	0.31
10.97	23.70	23.80	11.1	0.1	0.31
12.04	23.50	23.80	12.1	0.1	0.31
12.96	23.80	23.80	13.1	0.1	0.33
14.10	23.50	23.80	14.2	0.1	0.31
15.04	23.70	23.80	15.2	0.2	0.31
15.97	23.60	23.80	16.2	0.2	0.31

**Remark:**

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Velocity of standard

<sup>7</sup> Velocity of Unit Under Calibration

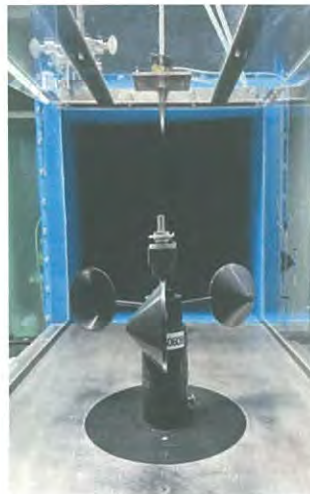**PHOTO OF CALIBRATION SET-UP**

Calibration set-up of the Cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The Cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set- up is not true to scale due to imaging geometry.

\*\*\*End of Certificate of Calibration\*\*\*

NAC

JIRANATEE ASSOCIATES CO., LTD.



Certificate Number

CWD-026-67

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Wind Direction Sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-A5910  
Data logger: A5910  
**ID NUMBER** : RYG\_FS0609  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 08 Jul 2024  
**MEASUREMENT DATE** : 18 Jul 2024  
**ISSUE DATE** : 18 Jul 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITION</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Wind direction frontal area <sup>2</sup>	129	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.143	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (22.2)°C, (47.5) %RH and (1001.7) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

### Calibration procedure:

The wind direction sensor was calibrated against Standard Rotary Encoder model: AX4009TS-DM04-P3-S-U0 in an close test-section of Eiffel-type wind tunnel with 900 cm<sup>2</sup> cross test section area. The WI-CL-008 based on IEC 61400-12-1, Wind energy generation systems – Part 12-1: Power performance measurements of electricity producing wind turbines, March 2017 was used as a calibration guideline.

### Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the NIMT (National Metrology Institute of Thailand) via Certificate number: DA-0036-23.

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor k=2, Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

MEASUREMENT RESULTS<sup>5</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D^s_{std}$ Degree (°)	$D^7_{unc}$ Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.04	0.000	0	0	0.80
	45.000	44	-1	0.80
	90.000	87	-3	0.80
	135.000	131	-4	0.80
	180.000	176	-4	0.80
	225.000	222	-3	0.80
	270.000	272	2	0.80
	315.000	320	5	0.80

## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Direction of standard

<sup>7</sup> Direction of Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*







JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Temperature measurement laboratory  
Calibration services department.



## CERTIFICATE OF CALIBRATION

Certificate No. : CDT-121-67

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Data Logger with Temperature sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : 110-WS-25DL-D  
**SERIAL NUMBER** : A5910  
**ID NUMBER** : RYG\_FS0609  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Suan Luang, Khet Suan Luang,  
Bangkok 10250 Thailand.

**RECEIVED DATE** : 08 Jul 2024  
**MEASUREMENT DATE** : 18 Jul 2024  
**ISSUE DATE** : 18 Jul 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH

**NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibration procedure:

The temperature calibration was done by In-House calibration method as WI-CL-001 according to comparison method with standard digital temperature indicator and standard temperature probe. The temperature scale use was based on ITS-90.

### Traceability:

The measurement results are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT) Certificate number: TT-0047-24, Certificate number: ER-0101-23

### Reference Used During Calibration:

1. Standard Temperature Probe  
Model: STS-100 A500, Serial No.: 667682-09,  
Due date: 26 Mar 2025
2. Digital Temperature Indicator  
Model: DTI-1000-A MK II, Serial No.: 671407-00591 Due date: 14 Sep 2024

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor  $k=2$ , Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

### Calibrated by:

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jittraporn Lertsomphol  
☐ Miss Ruangrumpai Phoommit



### Approved signatory:

Mr. Parinya Booncharoen  
Calibration Department Manager

**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20 °C to 40 °C

**Function:**

Table 3: This equipment was connected with temperature sensor Model: HMP60 S/N: U3641223.  
Dimension: Diameter 12 mm. Length 80 mm.

<u>Immersion Depth</u> (mm)	<u>Standard Reading</u> (°C)	<u>UUC Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
80	20.047	19.6	-0.4	0.099
80	25.043	24.6	-0.4	0.099
80	30.034	29.7	-0.3	0.099
80	35.028	34.7	-0.3	0.099
80	40.018	39.5	-0.5	0.099

**UUC\*:** Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*







JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,  
Bangkok 10600(Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Relative humidity and Air Temperature measurement laboratory  
Calibration services department.

## CERTIFICATE OF CALIBRATION

Certificate No. : CRT-023-67

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Relative humidity with data logger  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Data Logger: 110-WS-25DL-D  
Sensor: HMP60  
**SERIAL NUMBER** : Data Logger: A5910  
Sensor: U3641223  
**ID NUMBER** : RYG\_FS0609  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.  
**RECEIVED DATE** : 08 Jul 2024  
**MEASUREMENT DATE** : 18 Jul 2024  
**ISSUE DATE** : 18 Jul 2024

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH

**NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibration procedure:

The Relative humidity and Air Temperature calibration was done by In-House calibration method as WI-CL-009 and WI-CL-010 according to comparison method with Standard Chilled Mirror hygrometer with Temperature sensor and standard Humidity generator chamber.

### Traceability:

The measurements are traceable to the international system of units (SI) through National Institute of Metrology Thailand (NIMT). Certificate number: TH-0079-23 and through Jiranatee Associates Co., Ltd. Certificate number: CDT-001-67.

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor  $k=2$ , Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jittraporn Lertsomphol  
☐ Miss Ruangrumpai Phoommit



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager



JIRANATEE ASSOCIATES CO.,LTD.

Continuation of Certificate of Calibration Number: CRT-023-67

Page 2 of 2 Pages

**Measurement Results:**

The results of calibration and associated measurement uncertainties are reported in the table below.

**Result of Calibration:** ☒ Without Adjustment ☐ With Adjustment

**Table 1:** The results of calibration of relative humidity at 30 °C are reported in table below.

**Calibration Range:** 20%RH to 80%RH

<u>Air Temperature</u> (°C)	<u>Standard Reading</u> (%RH)	<u>UUC Reading</u> (%RH)	<u>Error</u> (%RH)	<u>Uncertainty</u> ± (%RH)
29.79	19.50	17.7	-1.8	0.83
29.83	50.52	47.9	-2.7	1.3
29.80	81.80	78.0	-3.8	2.3

UUC\*: Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*







JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

REVIEW BY	Nara korn P.
APPROVED BY	[Signature]
NEXT CAL. DATE	19/12/24

Certificate Number

CC-008-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Cup anemometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 200-WS-25DL  
**SERIAL NUMBER** : Sensor: WSD-A4985  
Data logger: A4985  
**ID NUMBER** : RYG\_FS0085  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 16 Jun 2023  
**MEASUREMENT DATE** : 19 Jun 2023  
**ISSUE DATE** : 19 Jun 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITIONS</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Win direction frontal area <sup>2</sup>	100	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.111	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (25.0) °C, (42.7) %RH and (1011.7) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



Approved signatory:

[Signature]

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

**MEASUREMENT RESULTS<sup>5</sup>**

The cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.

$v_{std}^6$ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$v_{uuc}^7$ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.025	24.90	24.95	0.9	-0.1	0.31
2.028	24.96	24.95	1.9	-0.1	0.31
2.997	25.00	24.95	2.9	-0.1	0.31
4.126	25.00	24.95	4.0	-0.1	0.31
5.02	24.90	24.95	4.9	-0.1	0.31
6.00	24.88	24.95	5.9	-0.1	0.31
7.05	24.90	24.95	7.0	-0.1	0.31
8.18	24.74	24.95	8.0	-0.1	0.31
9.09	24.84	24.95	9.0	0.0	0.31
10.07	24.70	24.95	10.0	-0.1	0.31
11.14	24.78	24.95	11.1	-0.1	0.31
12.12	24.70	24.95	12.0	-0.1	0.31
13.17	24.70	24.95	13.1	0.0	0.35
14.24	24.70	24.95	14.1	-0.2	0.31
15.20	24.70	24.95	15.2	0.0	0.44
16.28	24.70	24.95	16.2	-0.1	0.31

**Remark:**

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Velocity of standard

<sup>7</sup> Velocity of Unit Under Calibration

**PHOTO OF CALIBRATION SET-UP**

Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.





JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

Certificate Number

CD-008-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Wind Direction Sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 200-WS-25DL  
**SERIAL NUMBER** : Sensor: WSD-A4985  
Data logger: A4985  
**ID NUMBER** : RYG\_FS0085  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 16 Jun 2023  
**MEASUREMENT DATE** : 19 Jun 2023  
**ISSUE DATE** : 19 Jun 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure :  $1010 \pm 10$  hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

**CALIBRATION CONDITION** : Wind tunnel cross-section area<sup>1</sup> 900 cm<sup>2</sup>  
Win direction frontal area<sup>2</sup> 129 cm<sup>2</sup>  
Diameter of mounting pipe<sup>3</sup> - mm  
Blockage ratio of test object<sup>4</sup> 0.143 [-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (24.1)°C, (55.4) %RH and (1008.5) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jitraporn Lertsomphol



Approved signatory: \_\_\_\_\_

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

MEASUREMENT RESULTS <sup>5</sup>

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D^6_{std}$ Degree (°)	$D^7_{uuc}$ Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.01	45.000	44	-1	1.0
	90.001	87	-3	1.0
	135.000	132	-3	1.0
	180.000	179	-1	1.0
	225.000	228	3	1.0
	270.000	273	3	1.0
	315.000	319	4	1.0
	360.000	359	-1	1.0

## Remark:

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Direction of standard

<sup>7</sup> Direction of Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*







JIRANATEE ASSOCIATES CO., LTD.

Jiranatee Associates Co., Ltd.  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

REVIEW BY ..... *Manakorn P.*

APPROVED BY ..... *[Signature]*

NEXT CAL. DATE ..... 21/1/25

Certificate Number

CWS-001-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Cup anemometer  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-A5662  
Data logger: A5662  
**ID NUMBER** : RYG\_FS0544  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 11 Jul 2023  
**MEASUREMENT DATE** : 21 Jul 2023  
**ISSUE DATE** : 21 Jul 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

<b>CALIBRATION CONDITIONS</b>	: Wind tunnel cross-section area <sup>1</sup>	900	cm <sup>2</sup>
	Win direction frontal area <sup>2</sup>	100	cm <sup>2</sup>
	Diameter of mounting pipe <sup>3</sup>	-	mm
	Blockage ratio of test object <sup>4</sup>	0.111	[-]

**Preconditioning** : 24 hours at ambient conditions.  
**Measurement Condition** : The average values during measurement are (24.0) °C, (41.7) %RH and (1009.1) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittrapor Lertsomphol



Approved signatory: ..... *[Signature]*

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

**MEASUREMENT RESULTS <sup>5</sup>**

The cup anemometer, Unit Under Calibration (UUC) was exercised at 10 m/s for 5 minutes prior to calibration being performed. The standard air velocity 0.5 m/s to 5 m/s was calculated by a standard air velocity transducer and above 5 m/s to 30 m/s was calculated by a pitot tube with precision differential pressure meter which was installed 40 mm and 300 mm respectively away from wind tunnel nozzle, UUC was installed at center of the test section. The calibration was carried out under both rising and falling air velocity in the range of 1 m/s to 16 m/s at calibration interval of 1 m/s. The results of calibration and associated measurement uncertainties are reported in the table below.


$V_{std}^6$ (m/s)	Temp. wind tunnel (°C)	Temp. room (°C)	$V_{uuc}^7$ (m/s)	Error (m/s)	$U (k=2)$ (m/s)
1.024	23.84	23.95	0.8	-0.2	0.31
2.079	24.08	23.95	1.8	-0.3	0.31
3.019	24.04	23.95	2.8	-0.2	0.31
4.150	24.12	23.95	3.9	-0.3	0.31
5.00	23.72	23.95	4.8	-0.2	0.31
5.99	23.88	23.95	5.8	-0.2	0.31
7.04	23.68	23.95	6.9	-0.2	0.31
8.15	23.64	23.95	7.9	-0.2	0.31
9.09	23.30	23.95	9.0	-0.1	0.31
10.05	23.40	23.95	9.9	-0.1	0.31
11.13	23.48	23.95	11.0	-0.2	0.31
12.11	23.40	23.95	12.0	-0.1	0.31
13.16	23.50	23.95	13.0	-0.1	0.31
14.22	23.40	23.95	14.0	-0.2	0.31
15.22	23.50	23.95	15.0	-0.2	0.31
16.27	23.44	23.95	16.1	-0.2	0.31

**Remark:**

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Velocity of standard

<sup>7</sup> Velocity of Unit Under Calibration

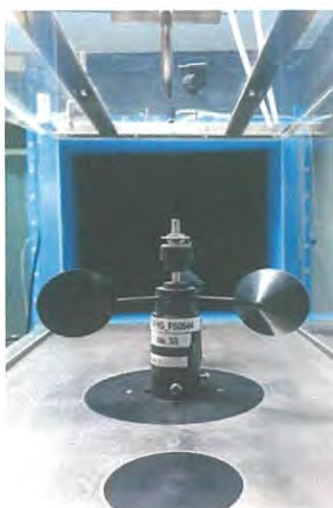**PHOTO OF CALIBRATION SET-UP**

Calibration set-up of the cup anemometer calibration in the wind tunnel of Jiranatee Associates Co., Ltd. The cup anemometer shown may differ from the calibrated one. Remark: The proportion of the set-up is not true to scale due to imaging geometry.







JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd. Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Air speed measurement laboratory  
Calibration services department.

Certificate Number

CWD-001-66

## CERTIFICATE OF CALIBRATION

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Wind Direction Sensor  
**MANUFACTURER** : Novalynx  
**MODEL/TYPE** : Sensor: WS-02F  
Data logger: 110-WS-25DL-D  
**SERIAL NUMBER** : Sensor: WSD-A5662  
Data logger: A5662  
**ID NUMBER** : RYG\_FS0544  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : ALS laboratory group (Thailand) Co., Ltd.  
104 Phatthanakan 40, Phatthanakan Rd, Khwaeng Suan Luang,  
Khet Suan Luang, Bangkok 10250 Thailand.

**RECEIVED DATE** : 11 Jul 2023  
**MEASUREMENT DATE** : 21 Jul 2023  
**ISSUE DATE** : 21 Jul 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature :  $23.0 \pm 3.0$  °C  
Relative Humidity :  $55.0 \pm 15.0$  %RH  
Atmospheric Pressure :  $1010 \pm 10$  hPa

**PLACE OF CALIBRATION** : Eiffel-type wind tunnel of Jiranatee Associates Co., Ltd.

**CALIBRATION CONDITION** : Wind tunnel cross-section area<sup>1</sup> 900 cm<sup>2</sup>  
Win direction frontal area<sup>2</sup> 129 cm<sup>2</sup>  
Diameter of mounting pipe<sup>3</sup> - mm  
Blockage ratio of test object<sup>4</sup> 0.143 [-]

**Preconditioning** : 24 hours at ambient conditions.

**Measurement Condition** : The average values during measurement are (23.8)°C, (43.0) %RH and (1011.6) hPa.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibrated by:

- ☒ Mr. Sorawit Thachalad  
☐ Miss Jittraporn Lertsomphol



Approved signatory: .....

Mr. Parinya Booncharoen  
Calibration Department Manager

### Remark:

- <sup>1</sup> Nozzle cross-section area of the wind tunnel  
<sup>2</sup> Projected cross-section area of the tested object include mounting pipe  
<sup>3</sup> Diameter of mounting pipe  
<sup>4</sup> Ratio <sup>2</sup> to <sup>1</sup>

**MEASUREMENT RESULTS <sup>5</sup>**

The wind direction sensor was calibrated against standard rotary encoder by comparison method. During calibration, the measurement was carried out at 45° intervals in clockwise and counterclockwise directions after offset adjustment has been made. The flow speed of wind tunnel (usually 5 m/s) is kept constant while the sensor is rotated around its vertical axis. The results of calibration and associated measurement uncertainties are reported in the table below.

Air speed m/s	$D^6_{std}$ Degree (°)	$D^7_{uuc}$ Degree (°)	Error Degree (°)	$U (k=2)$ Degree (°)
5.00	45.000	41	-4	1.0
	90.000	87	-3	1.0
	135.000	132	-3	1.0
	180.000	180	0	1.0
	225.000	228	3	1.0
	270.000	273	3	1.0
	315.000	318	3	1.0
	360.000	359	-1	1.0

**Remark:**

<sup>5</sup> Calibration results only count for the tested circumstances and environmental conditions during which calibration took place

<sup>6</sup> Direction of standard

<sup>7</sup> Direction of Unit Under Calibration

\*\*\*End of Certificate of Calibration\*\*\*





## CERTIFICATE OF CALIBRATION

Certificate No. : CDT-037-66  
Page 1 of 2

**Equipment Name:** Data Logger with Temperature sensor  
**Manufacturer:** Novalynx  
**Model:** 110-WS-25DL-D  
**Serial No.:** A5662  
**ID No.:** RYG\_FS0544

### Customer

**Name:** ALS laboratory group (Thailand) Co., Ltd.  
**Address:** 104 Phatthanakan 40, Phatthanakan Rd.,  
Khwaeng Suan Luang, Khet Suan Luang, Bangkok  
10250 Thailand.

**Received date:** 11 Jul 2023  
**Calibration date:** 21 Jul 2023  
**Issue date:** 21 Jul 2023

### Reference Used During Calibration

1. Standard Temperature Probe Model: STS-100 A500,  
Serial No.: 667682-09, Due date: 28 Mar 2024  
2. Digital Temperature Indicator Model: DTI-1000-A MK  
II, Serial No.: 671407-00591 Due date: 22 July 2023

### Calibration Condition

Temperature:  $(23 \pm 3)^{\circ}\text{C}$   
Relative Humidity:  $(55 \pm 15)\%$

### Calibration Procedure

The temperature calibration was done by In-House  
calibration method as WI-CL-001 according to  
comparison method with standard digital temperature  
indicator and standard temperature probe. The  
temperature scale use was based on ITS-90.

### Traceability

The measurement results are traceable to the  
international system of units (SI) through National  
Institute of Metrology Thailand (NIMT) Certificate  
number: TT-0038-23, Certificate number: ER-0092-  
22

**Noted:** The certificate is valid only to the item calibrated on date and place of calibration.

### Calibrated by

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jitraporn Lertsomphol  
☐ Miss Ruangrumpai Phoommit



### Approved Signatory:

Mr. Parinya Booncharoen  
Calibration Department Manager

**Result of Calibration:-** ☒ Without Adjustment ☐ With Adjustment

**Calibration Range:** 20-40 °C

**Function:**

This equipment was connected with temperature sensor Model: HMP60 S/N: T2320591.

Dimension : Diameter 12 mm. Length 80 mm.

<u>Immersion</u> <u>Depth</u> (mm)	<u>Standard</u> <u>Reading</u> (°C)	<u>UUC</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> (°C)
70	20.060	19.6	-0.5	0.099
70	25.054	24.6	-0.5	0.099
70	30.050	29.7	-0.3	0.14
70	35.043	34.5	-0.5	0.099
70	40.036	39.5	-0.5	0.14

UUC\* : Unit Under Calibration

The reported expanded uncertainty is based on standard uncertainty multiplied by a coverage factor k=2 providing a level of confidence of approximately 95%.

**\* End of Certificate \***





## CERTIFICATE OF CALIBRATION

Calibration No. : RH-01072023

Page 1 of 1 Pages

Measurement Item : Relative humidity with data logger  
Manufacturer : Novalynx  
Model/Type : 110-WS-25DL-D  
Serial Number : A5662  
ID No. : RYG\_FS0544  
Customer : ALS laboratory group (Thailand) Co., Ltd.  
: 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Suan Luang, Khet Suan Luang, Bangkok  
10250 Thailand.

### Environmental Condition:

The measurement was carried out in an ambient temperature of  $(25\pm3)^{\circ}\text{C}$ , and relative humidity of  $(50\pm15)\%$ .

### Measurement Method:

Unit Under Calibration (UUC) was calibrated by comparison method with standard chilled mirror hygrometer model: 1860-3 in the humidity generator chamber to determine the errors.

### Traceability:

This instrument was calibrated using standard equipment whose accuracy is traceability through National Institute of Standards and Technology to the international system of units (SI) via MCS Calibration, Inc. Certificate number: 20926-601. Due date: Sep 26, 2024.

Measurement Date : Jul 21, 2023

Issued Date : Jul 21, 2023

### Measurement Results:

This equipment was connected with Indoor air quality probe and Displayed (UR) on display. Model: HMP60, Serial number: T2320591.

Calibration was performed in the range of 20%RH to 80%RH

The results of calibration are reported in table below.

Determined (%RH)	Standard (Reading) (%RH)	UUC (Reading) (%RH)	Error (%RH)	Uncertainty $\pm$ (%RH)
20	20.07	16.3	-3.8	0.51
50	50.23	45.0	-5.2	0.51
80	80.23	73.5	-6.7	0.51

### Performed by

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jitraporn Lertsomphol  
☐ Miss Ruangrumpai Phoommit



### Approved Signatory:

Mr. Parinya Booncharoen.  
Calibration Department Manager

Cert. No. : ACC24037

Pages : 1 of 3

## Calibration Certificate

**Equipment :** SOUND CALIBRATOR  
**Manufacturer :** RION  
**Model :** NC-74  
**Serial No.:** 34178123  
**ID No.:** RYG\_FS0215

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 09 AUGUST 2024  
**Calibration Date :** 23 AUGUST 2024  
**Date of Issue :** 26 AUGUST 2024

REVIEW BY	<i>Nathakorn P</i>
APPROVED BY	<i>Thanakul Petchurai</i>
NEXT CAL. DATE	23/8/25

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

*Thanakul Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACC24037

Job No. : VC67AC0140

Pages : 2 of 3

Calibration Procedure : CP-AC-03

### Calibration Method :

This equipment was calibrated by follow on IEC-60942-2003 Standard.

The sound pressure level, frequency and total distortion of the sound calibrator was measured using the reference microphone.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	33461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25
Audio Analyzer	AVR-3360A	V744B6069	EF-0009-24	09-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

*S. Ketch.*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACC24037  
Job No. : VC67AC0140  
Pages : 3 of 3

### Result of calibration :

#### 1. Sound pressure level

Specified sound pressure level (dB)	Measured value (dB)	Deviated value (dB)	Uncertainty (dB)	Acceptance limit (dB)
94	94.06	0.06	0.45	0.40

#### 2. Frequency

Specified Frequency (Hz)	Measured value (Hz)	Deviated value ( % )	Uncertainty ( % )	Acceptance limit ( % )
1000	1001.4	0.1	0.1	1.0

#### 3. Total distortion

Measured value ( % )	Uncertainty ( % )	Acceptance limit ( % )
2.02	0.10	3.0

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————

*T. Petch.*



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 171/0167

## CALIBRATION CERTIFICATE

**Submitted by** : ALS Laboratory Group (Thailand) Co., Ltd.

**Address** : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phattankan, Khet Suan Luang, Bangkok 10250.

**Calibrated at** : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

**Instrument Calibrated :**

Description : Sound Level Meter

Manufacturer : Rion

Model : NL-42

Serial No. : 00296518 (ID: RYG\_FS0431)

Microphone : Type UC-52 No.66239

Preamplifier : Type NH-24 No.34375

**Ambient Environment**

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Relative Humidity :  $(50 \pm 15) \%$

Ambient Pressure :  $(101.325 \pm 1.5) \text{ kPa}$

**Standards used :**

1. Band Pass Filter Wavetek 752A S/N 90010494.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.



**Date of Receipt** : 24 Jan. 2024

**Date of Calibration** : 22-28 Feb. 2024

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 171/0167

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

**Calibration Procedure :**

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%.

**Date of Calibration** : 22-28 Feb. 2024

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 171/0167

**1. Absolute Sensitivity**

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
	Before adjust	After adjust				
113.96	114.3	113.9	-0.1	1.0	0.30	N/A

**Note:** The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 125.1 dB.

**2. Self-generated noise**

**2.1 Normal test**

Measured value (dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
20.2	0.10	N/A

**2.2 The microphone of the sound level meter was replaced by electrical signal input device**

Frequency Weighting	Measured value (dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
A-Weight	14.4	0.10	N/A
C-Weight	19.9	0.10	N/A
Flat	25.3	0.10	N/A

Date of Calibration : 22-28 Feb. 2024

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 171/0167

### 3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
	A-weight	C-weight	Flat			
125	-0.1	0.2	0.1	1.5	0.45	0.6
1 000	0.0	0.0	0.0	1.0	0.45	0.6
8 000	-1.7	-1.7	-1.7	5.0	0.45	0.7

### 4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
	A-weight	C-weight	Flat			
63	-0.1	-0.1	-0.1	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	-0.1	0.0	0.0	1.5	0.20	0.6
500	-0.1	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	-0.1	2.0	0.20	0.6
4 000	-0.1	0.0	0.0	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 22-28 Feb. 2024

4 / 9

*Pha*

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 171/0167

### 5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

### 6. Frequency and time weightings at 1 kHz

#### 6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.1	0.1	0.2	0.20	0.2

#### 6.2 Time weightings at 1 kHz

Frequency Weighting	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 22-28 Feb. 2024

5 / 9

Ph

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

7. Level linearity on the reference level range

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
137	137.0	0.0	1.1	0.30	0.3
136	136.0	0.0	1.1	0.30	0.3
135	135.0	0.0	1.1	0.30	0.3
133	133.0	0.0	1.1	0.30	0.3
132	132.0	0.0	1.1	0.30	0.3
131	131.0	0.0	1.1	0.30	0.3
130	130.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3
64	63.9	-0.1	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3

Date of Calibration : 22-28 Feb. 2024

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 171/0167

**7. Level linearity on the reference level range (cont.)**

Anticipated value (dB)	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
54	53.9	-0.1	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	43.9	-0.1	1.1	0.30	0.3
39	39.0	0.0	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.8	-0.2	1.1	0.30	0.3

**8. Level linearity including the level range control**

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 22-28 Feb. 2024

7 / 9  
Pha

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 171/0167

### 8. Level linearity including the level range control

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
30-130	25	25.0	0.0	1.1	0.30	0.3

### 9. Tone burst response

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
Fast	200	126.0	0.0	$\pm 1.0$	0.20	0.3
	2	108.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	100.0	0.0	+1.5; -5.0	0.20	0.3
Slow	200	119.5	-0.1	$\pm 1.0$	0.20	0.3
	2	100.0	0.0	+1.0; -5.0	0.20	0.3

Date of Calibration : 22-28 Feb. 2024

8 / 9

*Pha*

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 171/0167

### 10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
Complete cycle	125.4	125.5	0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35


### 11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
Positive one-half cycle	Negative one-half cycle				
135.4	135.4	0.0	1.5	0.55	0.25

### 12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :



(Mr. Pannasit Phasingsri)

Approved by :



(Mr. Prawate Kluaypa)  
Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 22-28 Feb. 2024

Date of Issue : 29 Feb. 2024

Ref : 2011267012400347001

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th



# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd., Bangbumru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

Cert. No. : ACL23320

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00597167 / 179118 / 87525  
**ID No.:** RYG\_FS0437

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

REVIEW BY	<i>Nathakorn P</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	19/10/24

**Received Date :** 11 OCTOBER 2023  
**Calibration Date :** 19-20 OCTOBER 2023  
**Date of Issue :** 24 OCTOBER 2023

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : ACL23320  
Job No. : VC67AC0011  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



## Continuation of Calibration Certificate

Cert. No. : ACL23320

Job No. : VC67AC0011

Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.



## Continuation of Calibration Certificate

Cert. No. : ACL23320

Job No. : VC67AC0011

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	11.2
C - weight	17.5
Flat	23.1

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.3	1.4	1.4	±5.0

## Continuation of Calibration Certificate

Cert. No. : ACL23320

Job No. : VC67AC0011

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	-0.1	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL23320  
Job No. : VC67AC0011  
Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	63.9	-0.1	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	48.9	-0.1	± 1.1
44.0	43.9	-0.1	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	34.0	0.0	± 1.1
30.0	29.9	-0.1	± 1.1
29.0	28.9	-0.1	± 1.1
28.0	27.9	-0.1	± 1.1
27.0	26.9	-0.1	± 1.1
26.0	25.9	-0.1	± 1.1
25.0	24.9	-0.1	± 1.1



Continuation of Calibration Certificate

**Cert. No. : ACL23320**  
**Job No. : VC67AC0011**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.1	0.1	±3.0
One	136.4	136.1	-0.3	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.1	0.1	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

## Continuation of Calibration Certificate

Cert. No. : ACL23320

Job No. : VC67AC0011

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— End of Calibration Certificate —————



**SITHIPORN ASSOCIATES CO., LTD.**  
**CALIBRATION LABORATORY**

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24012

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42A / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00623390 / 198637 / 26418  
**ID No.:** RYG\_FS0615

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 19 DECEMBER 2023  
**Calibration Date :** 05-08 JANUARY 2024  
**Date of Issue :** 09 JANUARY 2024



**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

*T. Petchurai*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24012  
Job No. : VC67AC0044  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.  
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

*G. Retheh*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24012  
Job No. : VC67AC0044  
Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty	Maximum-permitted
	(dB)	uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

*T. Petcha*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN  
associates



Cert. No. : ACL24012

Job No. : VC67AC0044

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.6
C - weight	19.2
Flat	24.8

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.3	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.0	1.1	1.1	±5.0

T. Peter.



# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24012

Job No. : VC67AC0044

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

## 5. Frequency and time weightings at 1 kHz

### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

*T. Retan.*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24012

Job No. : VC67AC0044

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	38.9	-0.1	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	27.9	-0.1	$\pm 1.1$
27.0	26.8	-0.2	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	24.9	-0.1	$\pm 1.1$

T. Petch.



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24012  
Job No. : VC67AC0044  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

*T. Petun*



# SITHIPHORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPHORN  
associates



Cert. No. : ACL24012  
Job No. : VC67AC0044  
Pages : 8 of 8

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.5	-0.2	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

\_\_\_\_\_  
End of Calibration Certificate

*G. Petch*

**Cert. No. : ACL24013**

**Pages : 1 of 8**

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42A / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00623391 / 198638 / 26419  
**ID No.:** RYG\_FS0616

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 19 DECEMBER 2023  
**Calibration Date :** 05-08 JANUARY 2024  
**Date of Issue :** 09 JANUARY 2024



**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**   
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24013  
Job No. : VC67AC0044  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

*T. Peter*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24013  
Job No. : VC67AC0044  
Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty	Maximum-permitted
	(dB)	uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

*T. Retan.*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24013

Job No. : VC67AC0044

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
15.1

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	13.8
C - weight	20.3
Flat	25.8

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.5	1.6	1.6	±5.0

*S. Petchum*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24013  
Job No. : VC67AC0044  
Pages : 5 of 8

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

*Signature*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24013

Job No. : VC67AC0044

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.1	0.1	$\pm 1.1$
84.0	84.1	0.1	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.1	0.1	$\pm 1.1$
69.0	69.1	0.1	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.1	0.1	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.1	0.1	$\pm 1.1$
30.0	30.1	0.1	$\pm 1.1$
29.0	29.1	0.1	$\pm 1.1$
28.0	28.1	0.1	$\pm 1.1$
27.0	27.2	0.2	$\pm 1.1$
26.0	26.2	0.2	$\pm 1.1$
25.0	25.3	0.3	$\pm 1.1$

*G. Ketun.*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24013  
Job No. : VC67AC0044  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.8	-0.6	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.1	0.1	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.3	-0.1	±2.0

*G. Retana*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24013  
Job No. : VC67AC0044  
Pages : 8 of 8

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.8	0.3	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

————— **End of Calibration Certificate** —————

*G. Peter*





THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0292

MTC No. EEL. BP. 83/0267

## CALIBRATION CERTIFICATE

**Submitted by** : ALS Laboratory Group (Thailand) Co.,Ltd.  
**Address** : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok, 10250.  
**Calibrated at** : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Calibrator

Manufacturer : Rion

Model : NC-74

Serial No. : 34178121 (ID:RYG\_FS0213)

### Ambient Environment

Temperature : (23 + 3) °C

Relative Humidity : (50 ± 15) %

Ambient Pressure : (101.325 ± 1.500) kPa

**Standards used :**

1. Digital Function Synthesizer NF Electronic DF-193A S/N 122037.
2. Measuring Amplifier Bruel&Kjaer 2636 S/N 1537484.
3. Programmable Attenuator Tamagawa TPA-303A S/N OF 2214.
4. Digital Multimeter Agilent 34401A S/N MY44005560.
5. Pressure Transmitter Vaisala PTB202AD S/N T0650001.
6. Audio Analyzer Keithley 2015-P S/N4106495.
7. Condenser Microphone B&K 4180 S/N 2889871.



**Calibration Procedure:** CP-102-04 based on IEC 60942-2003; The sound pressure level generated by sound calibrator under test shall be measured by standard microphone using an insert voltage technique.

This instrument has been calibrated against standards maintained at Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

**Date of Receipt** : 19 Feb. 2024

**Date of Calibration** : 28 Feb. 2024

1 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.5

**Head Office**  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9036  
Fax. (66) 0 2577 9009

**Office/Laboratory**  
668 Mu 2 Tambon Bangpoomai, Amphoe Muang Samutprakan,  
Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
(66) 08 3219 9440  
E-mail : mtc@tistr.or.th Website : www.tistr.or.th

**Office**  
196 Phahonyothin Road, Ladyao, Chatuchak,  
Bangkok 10900, Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
(66) 08 1889 6827



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0292

MTC No. EEL. BP. 83/0267

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

Nominal Output of Unit Under Test = 94 dB re 20 $\mu$ Pa at 1000 Hz

Acoustic Output in dB re 20 $\mu$ Pa, Corrected to Reference Conditions: 101.325 kPa, 23.0 °C and 50 %RH.

1. Sound Pressure Level

Standard Microphone Type	Measured Sound Pressure Level (dB)	Deviated value (dB)	Uncertainty (dB)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	94.01	0.01	$\pm 0.10$	$\pm 0.40$ dB

2. Frequency

Standard Microphone Type	Measured Frequency (Hz)	Deviated value (Hz)	Uncertainty (Hz)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1003.1	3.1	$\pm 1.5$	$\pm 1.0\%$

3. Total Distortion


Standard Microphone Type	Measured Total Distortion (%)	Uncertainty (%)	Tolerance limit IEC60942:2003 Class 1
1/2 inch Bruel&Kjaer 4180	1.80	$\pm 0.50$	$\pm 3.0\%$

Note : 1. No adjustment.


2. The calibrator pressure correction was not included.

3. The microphone volume correction was included at level of 0.16 dB from manual.

Calibrated by :

  
.....  
(Mr. Weerachai Deechaiyae)

Approved by :

  
.....  
(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 28 Feb. 2024

Date of Issue : 29 Feb. 2024

Ref : 2011267021900719001

End of Certificate

2 / 2

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

## CALIBRATION CERTIFICATE

**Submitted by** : ALS Laboratory Group (Thailand) Co., Ltd.  
**Address** : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.  
**Calibrated at** : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

### Instrument Calibrated :

Description : Sound Level Meter  
Manufacturer : Rion  
Model : NL-42  
Serial No. : 00900073 (ID:RYG\_FS0494)  
Microphone : UC-52 No.188466  
Preamplifier : NH-24 No.01735

### Ambient Environment

Temperature :  $(23 \pm 3) ^\circ\text{C}$   
Relative Humidity :  $(50 \pm 15) \%$   
Ambient Pressure :  $(101.325 \pm 1.5) \text{ kPa}$

### Standards used :

1. Band Pass Filter Wavetek 752A S/N 90010494.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.



**Date of Receipt** : 24 Jan. 2024

**Date of Calibration** : 23 Feb.2024-1 Mar.2024

1 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

**Calibration Procedure :**

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%.

**Date of Calibration** : 23 Feb.2024-1 Mar.2024

2 / 9 

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.91	114.1	113.9	0.0	1.0	0.30	N/A

**Note:** The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 124.6 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
17.8	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	12.9	0.10	N/A
C-Weight	18.5	0.10	N/A
Flat	24.2	0.10	N/A

Date of Calibration : 23 Feb.2024-1 Mar.2024

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.1	0.2	0.2	1.5	0.45	0.6
1 000	-0.1	-0.1	-0.1	1.0	0.45	0.6
8 000	-0.7	-0.7	-0.7	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	-0.1	0.0	0.0	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	-0.1	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	0.0	2.0	0.20	0.6
4 000	-0.1	0.0	0.0	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 23 Feb.2024-1 Mar.2024

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

5. Long-term stability

Time	Measured Value	Deviated value	Acceptance limit	Uncertainty	Maximum-permitted uncertainty of measurement
	(dB)	(dB)	class 2 (±dB)	(±dB)	(±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value	Deviated value	Acceptance limit	Uncertainty	Maximum-permitted uncertainty of measurement
	(dB)	(dB)	class 2 (±dB)	(±dB)	(±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value	Deviated value	Acceptance limit	Uncertainty	Maximum-permitted uncertainty of measurement
	(dB)	(dB)	class 2 (±dB)	(±dB)	(±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 23 Feb.2024-1 Mar.2024

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
136	136.0	0.0	1.1	0.30	0.3
135	135.0	0.0	1.1	0.30	0.3
134	134.0	0.0	1.1	0.30	0.3
133	133.0	0.0	1.1	0.30	0.3
132	132.0	0.0	1.1	0.30	0.3
131	131.0	0.0	1.1	0.30	0.3
130	130.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	68.9	-0.1	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
64	63.9	-0.1	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.9	-0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

**8. Level linearity including the level range control**

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35.0	35.0	0.0	1.1	0.30	0.3

**9. Tone burst response**

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	109.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	99.9	-0.1	+1.5; -5.0	0.20	0.3
Slow	200	119.6	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -5.0	0.20	0.3
SEL	200	120.0	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	90.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 178/0167

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.3	-0.1	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
135.5	135.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

*Tawikiat Iamsamran*

(Mr. Tawikiat Iamsamran)

Approved by :

*Prawate Kluaypa*

(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 23 Feb.2024-1 Mar.2024

Date of Issue : 1 Mar. 2024

Ref : 2011267012400347008

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

## CALIBRATION CERTIFICATE

**Submitted by** : ALS Laboratory Group (Thailand) Co., Ltd.  
**Address** : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.  
**Calibrated at** : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

### Instrument Calibrated :


**Description** : Sound Level Meter  
**Manufacturer** : Rion  
**Model** : NL-42  
**Serial No.** : 00900074 (ID:RYG\_FS0495)  
**Microphone** : UC-52 No.188467  
**Preamplifier** : NH-24 No.01736

### Ambient Environment

**Temperature** :  $(23 \pm 3) ^\circ\text{C}$   
**Relative Humidity** :  $(50 \pm 15) \%$   
**Ambient Pressure** :  $(101.325 \pm 1.5) \text{ kPa}$

### Standards used :

1. Band Pass Filter Wavetek 752A S/N 90010494.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

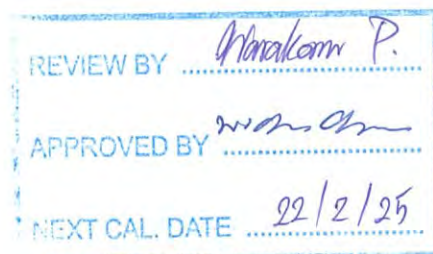

**Date of Receipt** : 24 Jan. 2024

**Date of Calibration** : 23 Feb.2024-1 Mar.2024

1 / 9

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

#### Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

#### Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

#### Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

**Calibration Procedure :**

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%.

**Date of Calibration** : 23 Feb.2024-1 Mar.2024

2 / 9

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
	Before adjust	After adjust				
113.94	114.1	113.9	0.0	1.0	0.30	N/A

**Note:** The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 124.2 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
16.5	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
A-Weight	11.7	0.10	N/A
C-Weight	17.2	0.10	N/A
Flat	22.5	0.10	N/A

Date of Calibration : 23 Feb.2024-1 Mar.2024

3 / 9

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.2	0.3	0.3	1.5	0.45	0.6
1 000	-0.2	-0.2	-0.2	1.0	0.45	0.6
8 000	-0.7	-0.8	-0.8	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	-0.1	-0.1	0.0	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	-0.1	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	-0.1	0.0	2.0	0.20	0.6
4 000	-0.1	-0.1	0.0	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 23 Feb.2024-1 Mar.2024

4/9

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 23 Feb.2024-1 Mar.2024

5 / 9

The results relate only to the items tested/calibrated or value assigned.  
Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
136	136.0	0.0	1.1	0.30	0.3
135	135.0	0.0	1.1	0.30	0.3
134	134.0	0.0	1.1	0.30	0.3
133	133.0	0.0	1.1	0.30	0.3
132	132.0	0.0	1.1	0.30	0.3
131	131.0	0.0	1.1	0.30	0.3
130	130.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.0	0.0	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	68.9	-0.1	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

6/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
64	63.9	-0.1	1.1	0.30	0.3
59	58.9	-0.1	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	48.9	-0.1	1.1	0.30	0.3
44	43.9	-0.1	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.8	-0.2	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

7/9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

**8. Level linearity including the level range control**

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35.0	35.0	0.0	1.1	0.30	0.3

**9. Tone burst response**

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	108.9	-0.1	+1.0; -2.5	0.20	0.3
	0.25	99.9	-0.1	+1.5; -5.0	0.20	0.3
Slow	200	119.6	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -5.0	0.20	0.3
SEL	200	120.0	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	90.8	-0.2	+1.5; -5.0	0.20	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 179/0167

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.4	0.0	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
135.0	135.0	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

*Tawikiat Iamsamran*

(Mr. Tawikiat Iamsamran)

Approved by :

*Prawate Khuaypa*

(Mr. Prawate Khuaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 23 Feb.2024-1 Mar.2024

Date of Issue : 1 Mar. 2024

Ref : 2011267012400347009

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



**Cert. No. : ACL24009**

**Pages : 1 of 8**

## Calibration Certificate


**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42A / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00623387 / 198634 / 26415  
**ID No.:** RYG\_FS0612

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 19 DECEMBER 2023  
**Calibration Date :** 05-08 JANUARY 2024  
**Date of Issue :** 09 JANUARY 2024

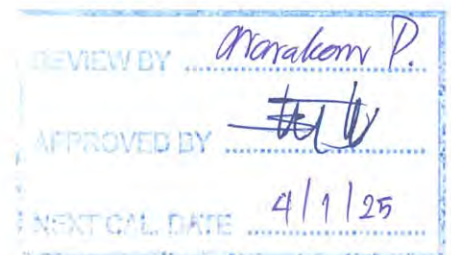

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24009

Job No. : VC67AC0044

Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

*T. Petcha -*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24009

Job No. : VC67AC0044

Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty	Maximum-permitted
	(dB)	uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

*T. Petcha*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24009

Job No. : VC67AC0044

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	11.6
C - weight	17.8
Flat	23.6

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.6	0.7	0.7	±5.0

*T. Petur.*



**Cert. No. : ACL24009**

**Job No. : VC67AC0044**

**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	0.0	±2.0
125	0.0	0.1	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

*G. Petu...*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24009

Job No. : VC67AC0044

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	27.9	-0.1	$\pm 1.1$
27.0	26.9	-0.1	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	24.8	-0.2	$\pm 1.1$

*G. Peter*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24009  
Job No. : VC67AC0044  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.1	0.1	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.1	0.1	±1.0

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.1	0.1	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

*G. Retina*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24009

Job No. : VC67AC0044

Pages : 8 of 8

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.5	-0.2	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

*G. Retam*

# SITHIPHORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY



451-451/1 Sirinthorn Rd., Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com

Cert. No. : ACL23330

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42A/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00222542 / 195375 / 15374  
**ID No.:** NKH\_FS0115

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAENG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 20 OCTOBER 2023  
**Calibration Date :** 01-02 NOVEMBER 2023  
**Date of Issue :** 03 NOVEMBER 2023

REVIEW BY	Nathakorn P.
APPROVED BY	[Signature]
NEXT CAL. DATE	11/11/24

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**

[Signature]  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL23330

Job No. : VC67AC0013

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



## Continuation of Calibration Certificate

Cert. No. : ACL23330

Job No. : VC67AC0013

Pages : 3 of 8

Summary of Measurement Result :

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

## Continuation of Calibration Certificate

Cert. No. : ACL23330

Job No. : VC67AC0013

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
14.6

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	10.8
C - weight	16.9
Flat	22.6

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.2	0.2	0.2	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	1.2	1.2	1.2	±5.0



## Continuation of Calibration Certificate

Cert. No. : ACL23330

Job No. : VC67AC0013

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	-0.1	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.0	0.0	±5.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3



## Continuation of Calibration Certificate

Cert. No. : ACL23330  
Job No. : VC67AC0013  
Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	$\pm 1.1$
136.0	136.1	0.1	$\pm 1.1$
135.0	135.1	0.1	$\pm 1.1$
134.0	134.1	0.1	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.1	0.1	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.1	0.1	$\pm 1.1$
114.0	114.1	0.1	$\pm 1.1$
109.0	109.1	0.1	$\pm 1.1$
104.0	104.1	0.1	$\pm 1.1$
99.0	99.1	0.1	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.0	0.0	$\pm 1.1$
28.0	28.0	0.0	$\pm 1.1$
27.0	27.0	0.0	$\pm 1.1$
26.0	26.1	0.1	$\pm 1.1$
25.0	25.1	0.1	$\pm 1.1$

## Continuation of Calibration Certificate

Cert. No. : ACL23330

Job No. : VC67AC0013

Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.2	-0.2	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0



## Continuation of Calibration Certificate

Cert. No. : ACL23330

Job No. : VC67AC0013

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate



Cert. No. : ACL24027

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00472126 / 158778 / 88180  
**ID No.:** RYG\_FS0301

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 19 DECEMBER 2023  
**Calibration Date :** 12 JANUARY 2024  
**Date of Issue :** 16 JANUARY 2024



**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :**   
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24027

Job No. : VC67AC0044

Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.  
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

*G. Petcha*



# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24027  
Job No. : VC67AC0044  
Pages : 3 of 8

## Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	-	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

*T. Retun*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24027

Job No. : VC67AC0044

Pages : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
18.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	12.0
C - weight	18.4
Flat	24.2

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.7	0.8	0.9	± 1.5
1000	-0.2	-0.2	-0.2	± 1.0
8000	-2.5	-2.5	-2.5	±5.0

*G. Petch.*

**Cert. No. : ACL24027**

**Job No. : VC67AC0044**

**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	-0.1	0.0	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

*G. Peter*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24027

Job No. : VC67AC0044

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.1	0.1	$\pm 1.1$
84.0	84.1	0.1	$\pm 1.1$
79.0	79.1	0.1	$\pm 1.1$
74.0	74.1	0.1	$\pm 1.1$
69.0	69.1	0.1	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.1	0.1	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.1	0.1	$\pm 1.1$
28.0	28.1	0.1	$\pm 1.1$
27.0	27.1	0.1	$\pm 1.1$
26.0	26.1	0.1	$\pm 1.1$
25.0	25.1	0.1	$\pm 1.1$

*G. Retan*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24027  
Job No. : VC67AC0044  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.3	-1.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

*T. Retan.*

# SITHIPHORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPHORN  
associates



Cert. No. : ACL24027  
Job No. : VC67AC0044  
Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.6	-0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

*Signature*



Cert. No. : ACL24283  
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RION  
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24  
Serial No.: 00472127 / 169440 / 72461  
ID No.: RYG\_FS0302

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

Location : -  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 04 SEPTEMBER 2024  
Calibration Date : 19 SEPTEMBER 2024  
Date of Issue : 20 SEPTEMBER 2024

REVIEW BY	<i>Nathakorn P.</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	19/9/25

Calibrated by : Nathakorn Pisutpaisan

Approved by : *[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com



Cert. No. : ACL24283  
Job No. : VC67AC0148  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

A handwritten signature in blue ink, appearing to read 'P. Ketchu'.

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24283

Job No. : VC67AC0148

Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

*Z. Letch.*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24283  
Job No. : VC67AC0148  
Page : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.94)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
17.5

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting ( dB )
A - weight	12.0
C - weight	18.2
Flat	24.1

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.2	0.2	± 1.5
1000	-0.2	-0.2	-0.2	± 1.0
8000	-1.2	-1.1	-1.1	±5.0

*T. Petch.*



**Cert. No. : ACL24283**  
**Job No. : VC67AC0148**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.1	0.1	0.0	±1.5
250	0.1	0.0	0.0	±1.5
500	0.0	0.1	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.1	0.1	±2.0
4000	0.0	0.1	0.1	±3.0
8000	0.1	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.1	0.1	± 0.3

*T. Petcha-*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24283

Job No. : VC67AC0148

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.1	0.1	$\pm 1.1$
134.0	134.1	0.1	$\pm 1.1$
133.0	133.0	0.0	$\pm 1.1$
132.0	132.0	0.0	$\pm 1.1$
131.0	131.0	0.0	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.1	0.1	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.1	0.1	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	33.9	-0.1	$\pm 1.1$
30.0	29.9	-0.1	$\pm 1.1$
29.0	28.9	-0.1	$\pm 1.1$
28.0	27.9	-0.1	$\pm 1.1$
27.0	26.9	-0.1	$\pm 1.1$
26.0	25.9	-0.1	$\pm 1.1$
25.0	24.9	-0.1	$\pm 1.1$

*T. Petch.*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiphorn.com

SITHIPORN  
associates



Cert. No. : ACL24283  
Job No. : VC67AC0148  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
130	30.0	30.0	0.0	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

*G. Retchin.*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24283

Job No. : VC67AC0148

Pages : 8 of 8

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.8	-0.6	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.1	-0.3	±2.0

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.7	0.0	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

*T. Ketch.*

Cert. No. : ACL24339  
Pages : 1 of 8

Calibration Certificate

Equipment : SOUND LEVEL METER  
Manufacturer : RION  
Model : NL-42 / Microphone UC-52 / Preamplifier NH-24  
Serial No.: 00597168 / 180411 / 88181  
ID No.: RYG\_FS0438

Condition As Found : GOOD

Customer : ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

Location : -  
Ambient Temperature : ( 23.0 ± 3 ) °C  
Pressure : ( 101.3 ± 3 ) kPa  
Relative Humidity : ( 50.0 ± 20 ) %

Received Date : 18 OCTOBER 2024  
Calibration Date : 30 OCTOBER 2024  
Date of Issue : 31 OCTOBER 2024

REVIEW BY ..... *Supt. S.* .....  
APPROVED BY ..... *[Signature]* .....  
NEXT CAL DATE..... 30 Oct 2025 .....

Calibrated by : Nathakorn Pisutpaisan

Approved by : *[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24339

Job No. : VC67AC0168

Pages : 2 of 8

**Calibration Procedure :** CP-AC-01

### Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

### Condition of this result of calibration :

#### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24339  
Job No. : VC67AC0168  
Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

*T. Petch.*



**Cert. No. : ACL24339**

**Job No. : VC67AC0168**

**Page : 4 of 8**

**Result of calibration :**

**1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.94)	93.9	0.0	±0.3

**2. Self-generated noise**

**2.1 Normal test**

Measured Value ( dB )
14.6

**2.2 The microphone of the sound level meter was replaced by electrical signal input device.**

Frequency Weighting	Weighting ( dB )
A - weight	11.6
C - weight	17.8
Flat	23.4

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.2	0.3	0.4	± 1.5
1000	0.1	0.1	0.1	± 1.0
8000	0.6	0.7	0.7	±5.0

*T. Peter.*

**Cert. No. : ACL24339**  
**Job No. : VC67AC0168**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.2	-0.1	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	-0.1	±1.5
500	0.0	0.0	-0.1	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

*T. Petcha*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24339

Job No. : VC67AC0168

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	$\pm 1.1$
136.0	136.0	0.0	$\pm 1.1$
135.0	135.0	0.0	$\pm 1.1$
134.0	134.0	0.0	$\pm 1.1$
133.0	132.9	-0.1	$\pm 1.1$
132.0	131.9	-0.1	$\pm 1.1$
131.0	130.9	-0.1	$\pm 1.1$
129.0	129.0	0.0	$\pm 1.1$
124.0	124.0	0.0	$\pm 1.1$
119.0	119.0	0.0	$\pm 1.1$
114.0	114.0	0.0	$\pm 1.1$
109.0	109.0	0.0	$\pm 1.1$
104.0	104.0	0.0	$\pm 1.1$
99.0	99.0	0.0	$\pm 1.1$
94.0	94.0	0.0	$\pm 1.1$
89.0	89.0	0.0	$\pm 1.1$
84.0	84.0	0.0	$\pm 1.1$
79.0	79.0	0.0	$\pm 1.1$
74.0	74.0	0.0	$\pm 1.1$
69.0	69.0	0.0	$\pm 1.1$
64.0	64.0	0.0	$\pm 1.1$
59.0	59.0	0.0	$\pm 1.1$
54.0	54.0	0.0	$\pm 1.1$
49.0	49.0	0.0	$\pm 1.1$
44.0	44.0	0.0	$\pm 1.1$
39.0	39.0	0.0	$\pm 1.1$
34.0	34.0	0.0	$\pm 1.1$
30.0	30.0	0.0	$\pm 1.1$
29.0	29.1	0.1	$\pm 1.1$
28.0	28.0	0.0	$\pm 1.1$
27.0	27.1	0.1	$\pm 1.1$
26.0	26.0	0.0	$\pm 1.1$
25.0	25.1	0.1	$\pm 1.1$

*T. Peter*



**Cert. No. : ACL24339**  
**Job No. : VC67AC0168**  
**Pages : 7 of 8**

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
130	29.0	29.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

*T. Keteh -*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24339  
Job No. : VC67AC0168  
Pages : 8 of 8

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	130.0	130.0	0.0	±3.0
One	133.4	133.4	0.0	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.1	-0.3	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.5	-0.1	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

*T. Petcha*

**SITHIPORN ASSOCIATES CO., LTD.**  
**CALIBRATION LABORATORY**

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24306  
Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42 / Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 00597169 / 158770 / 34370  
**ID No.:** RYG\_FS0439

**Condition As Found :** GOOD

**Customer :** ALS LABORATORY GROUP (THAILAND) CO., LTD.  
104 PHATTHANAKAN 40, PHATTHANAKAN ROAD,  
KHWAEANG PHATTHANAKAN, KHET SUAN LUANG,  
BANGKOK, 10250 THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 23 SEPTEMBER 2024  
**Calibration Date :** 09 OCTOBER 2024  
**Date of Issue :** 09 OCTOBER 2024

REVIEW BY	<i>Nathakorn P</i>
APPROVED BY	<i>[Signature]</i>
NEXT CAL. DATE	9/10/25

**Calibrated by :** Nathakorn Pisutpaisan

**Approved by :** *[Signature]*  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



# SITHIPORN ASSOCIATES CO., LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24306  
Job No. : VC67AC0164  
Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by follow on IEC-61672-3 (2013) Standard for sound level meter (SLM).  
The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.  
For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

### 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-24	05-FEB-25
Waveform Generator	33511B	MY52302742	EF-0007-24	05-FEB-25
Digital Multimeter	33461A	MY53220104	EEL.BP 21/0267	13-FEB-25
Digital Multimeter	33461A	MY53220076	EEL.BP 20/0267	15-FEB-25
Digital Multimeter	34461A	MY60024273	EEL.BP 22/0267	15-FEB-25
Programmable Attenuator	MAT-1070	62100114	EF-0008-24	05-FEB-25
Condenser Microphone	4180	2977900	AA-1001-24	12-FEB-25
Measuring Amplifier	NA-42KAI	34560495	AA-3001-24	05-FEB-25

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

*T. Petch.*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24306  
Job No. : VC67AC0164  
Pages : 3 of 8

### Summary of Measurement Result :

Parameter	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	0.2	N/A
2. Self-generated noise	0.2	N/A
3. Acoustical signal tests of frequency weightings		
125 Hz	0.3	0.6
1000 Hz	0.3	0.6
8000 Hz	0.3	0.7
4. Electrical signal tests of frequency weightings		
For 10 Hz to 4 kHz	0.3	0.6
For > 4 kHz to 10 kHz	0.3	0.7
For > 10 kHz to 20 kHz	0.3	1.0
5. Frequency and time weightings at 1 kHz	0.2	0.2
6. Long - term stability	0.1	0.1
7. Level linearity on the reference level range	0.2	0.3
8. Level linearity including the level range control	0.2	0.3
9. Tone burst response	0.2	0.3
10. Peak C sound level	0.2	0.35
11. Overload indication	0.2	0.25
12. High level stability	0.1	0.1

*G. Petch.*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24306

Job No. : VC67AC0164

Page : 4 of 8

### Result of calibration :

#### 1. Absolute sensitivity

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.94)	93.9	0.0	±0.3

#### 2. Self-generated noise

##### 2.1 Normal test

Measured Value ( dB )
13.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Weighting ( dB )
A - weight	10.8
C - weight	16.8
Flat	22.4

#### 3. Acoustical signal tests of frequency weightings

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.3	0.4	0.4	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	-1.9	-1.8	-1.8	±5.0

*S. Retch.*



**Cert. No. : ACL24306**  
**Job No. : VC67AC0164**  
**Pages : 5 of 8**

#### 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	0.0	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

#### 5. Frequency and time weightings at 1 kHz

##### 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

##### 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

#### 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

*G. Petch*

# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24306

Job No. : VC67AC0164

Pages : 6 of 8

### 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	54.0	0.0	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	38.9	-0.1	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.0	0.0	± 1.1
29.0	29.1	0.1	± 1.1
28.0	28.1	0.1	± 1.1
27.0	27.1	0.1	± 1.1
26.0	26.2	0.2	± 1.1
25.0	25.3	0.3	± 1.1

*Signature*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbumru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24306  
Job No. : VC67AC0164  
Pages : 7 of 8

### 8. Level linearity including the level range control

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
130	94.0	94.0	0.0	±1.1

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
130	30.0	30.1	0.1	±1.1

### 9. Tone burst response

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

*T. Petch*



# SITHIPORN ASSOCIATES CO., LTD.

## CALIBRATION LABORATORY

451-451/1 Sirinthorn Road, Bangbunru, Bangplud, Bangkok, 10700 Thailand  
Tel. +66 2433 8331 Email : calibration@sithiporn.com

SITHIPORN  
associates



Cert. No. : ACL24306

Job No. : VC67AC0164

Pages : 8 of 8

### 10. Peak C sound level

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	136.3	-0.1	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0

### 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.6	89.6	0.0	±1.5

### 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$   
or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

## CALIBRATION CERTIFICATE

**Submitted by** : ALS Laboratory Group (Thailand) Co., Ltd.

**Address** : 104 Phatthanakan 40, Phatthanakan Rd., Khwaeng Phatthanakan, Khet Suan Luang, Bangkok 10250.

**Calibrated at** : Electrical and Electronic Standards Laboratory, Industrial Metrology and Testing Service Centre.  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Rd., A.Muang, Samutprakan 10280.

**Instrument Calibrated :**

**Ambient Environment**

Description : Sound Level Meter

Temperature :  $(23 \pm 3) ^\circ\text{C}$

Manufacturer : Rion

Relative Humidity :  $(50 \pm 15) \%$

Model : NL-42

Ambient Pressure :  $(101.325 \pm 1.5) \text{ kPa}$


Serial No. : 00900072 (ID:RYG\_FS0493)

Microphone : UC-52 No.188465

Preamplifier : NH-24 No.01734

**Standards used :**

1. Band Pass Filter Wavetek 752A S/N 90010494.
2. Condenser Microphone Brüel&Kjær 4180 S/N 2889871.
3. Decade Attenuator Ando AL-205 S/N 00464602.
4. Function/Arbitrary Waveform Generator Agilent 33220A S/N MY44042668.
5. Digital Function Synthesizer NF Electronic Instruments DF-193A S/N 122037.
6. Digital Multimeter Fluke 8520A S/N 4985007.
7. Pistonphone Rion NC-72 S/N 00402446.
8. Measuring Amplifier Brüel&Kjær 2636 S/N 1537484.

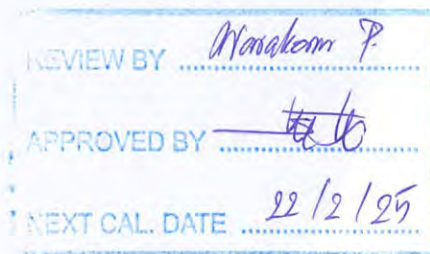

**Date of Receipt** : 24 Jan. 2024

**Date of Calibration** : 23 Feb.2024-1 Mar.2024

1 / 9

9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

9. Power Amplifier Brüel&Kjær 2706 S/N 1517650.
10. Speaker Tannoy Limited, Great Britain British Patent No. 215300.
11. Digital Multimeter Agilent 34401A S/N MY44005560.
12. Programmable Attenuator Tamagawa TPA-303A S/N 2212.

**Calibration Procedure :**

This instrument was calibrated by using calibration procedures no CP-102-02 and CP-102-03, which were based on IEC 61672-3 Electroacoustics - Sound Level Meters - Part 3 : Periodic tests (2013). These calibration procedures were related to the electrical and acoustic signal tests. The electrical signal test was carried out with the direct measurement method. The acoustic signal test was performed in an anechoic room with the comparison measurement method.

This instrument has been calibrated against standards maintained at the Electrical and Electronic Standards Laboratory (EEL), which are traceable to the International System of Units through the National Institute of Metrology (Thailand).

The information on actual reading is attached herewith and the uncertainty limits quoted refer to the measured values only.

The reported expanded uncertainty is based upon a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95%.

**Date of Calibration** : 23 Feb.2024-1 Mar.2024

2 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

1. Absolute Sensitivity

Reference Acoustic Signal (dB)	Measured value (dB)		Deviation value (dB)	Acceptance limit Class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	Before adjust	After adjust				
113.91	114.0	113.9	0.0	1.0	0.30	N/A

**Note:** The external calibration adjustment was firstly performed. The internal calibration adjustment was then completed at the display of 123.8 dB.

2. Self-generated noise

2.1 Normal test

Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
17.8	0.10	N/A

2.2 The microphone of the sound level meter was replaced by electrical signal input device

Frequency Weighting	Measured value (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-Weight	11.3	0.10	N/A
C-Weight	17.0	0.10	N/A
Flat	23.4	0.10	N/A

Date of Calibration : 23 Feb.2024-1 Mar.2024

3 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

3. Acoustical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
125	0.3	0.4	0.4	1.5	0.45	0.6
1 000	-0.2	-0.2	-0.2	1.0	0.45	0.6
8 000	-0.4	-0.5	-0.5	5.0	0.45	0.7

4. Electrical signal test of frequency weightings

Frequency (Hz)	Deviation from frequency response (dB)			Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
	A-weight	C-weight	Flat			
63	-0.1	0.0	0.0	2.0	0.20	0.6
125	-0.1	0.0	0.0	1.5	0.20	0.6
250	-0.1	0.0	0.0	1.5	0.20	0.6
500	0.0	0.0	0.0	1.5	0.20	0.6
1 000	0.0	0.0	0.0	1.0	0.20	0.6
2 000	-0.1	0.0	0.0	2.0	0.20	0.6
4 000	-0.1	0.0	0.0	3.0	0.20	0.6
8 000	0.0	0.0	0.0	5.0	0.20	0.7

Date of Calibration : 23 Feb.2024-1 Mar.2024

4 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

5. Long-term stability

Time	Measured Value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	94.0	0.0	0.3	0.10	0.1
End	94.0				

6. Frequency and time weightings at 1 kHz

6.1 Frequency weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
A-weight	94.0	0.0	0.2	0.20	0.2
C-weight	94.0	0.0	0.2	0.20	0.2
Flat	94.0	0.0	0.2	0.20	0.2

6.2 Time weightings at 1 kHz

Frequency Weighting	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	94.0	0.0	0.1	0.20	0.2
Slow	94.0	0.0	0.1	0.20	0.2
Leq	94.0	0.0	0.1	0.20	0.2

Date of Calibration : 23 Feb.2024-1 Mar.2024

5 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

7. Level linearity on the reference level range

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
136	136.0	0.0	1.1	0.30	0.3
135	135.0	0.0	1.1	0.30	0.3
134	134.1	0.1	1.1	0.30	0.3
133	133.0	0.0	1.1	0.30	0.3
132	132.0	0.0	1.1	0.30	0.3
131	131.0	0.0	1.1	0.30	0.3
130	130.0	0.0	1.1	0.30	0.3
129	129.0	0.0	1.1	0.30	0.3
124	124.0	0.0	1.1	0.30	0.3
119	119.0	0.0	1.1	0.30	0.3
114	114.0	0.0	1.1	0.30	0.3
109	109.0	0.0	1.1	0.30	0.3
104	104.0	0.0	1.1	0.30	0.3
99	99.0	0.0	1.1	0.30	0.3
94	94.0	0.0	1.1	0.30	0.3
89	89.0	0.0	1.1	0.30	0.3
84	84.1	0.1	1.1	0.30	0.3
79	79.0	0.0	1.1	0.30	0.3
74	74.0	0.0	1.1	0.30	0.3
69	69.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

6 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**  
35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**  
Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**  
196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th

THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

7. Level linearity on the reference level range (cont.)

Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
64	64.0	0.0	1.1	0.30	0.3
59	59.0	0.0	1.1	0.30	0.3
54	53.9	-0.1	1.1	0.30	0.3
49	49.0	0.0	1.1	0.30	0.3
44	44.0	0.0	1.1	0.30	0.3
39	38.9	-0.1	1.1	0.30	0.3
34	33.9	-0.1	1.1	0.30	0.3
29	28.9	-0.1	1.1	0.30	0.3
28	27.9	-0.1	1.1	0.30	0.3
27	26.9	-0.1	1.1	0.30	0.3
26	25.9	-0.1	1.1	0.30	0.3
25	24.9	-0.1	1.1	0.30	0.3

8. Level linearity including the level range control

At reference sound level on the reference level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 ( $\pm$ dB)	Uncertainty ( $\pm$ dB)	Maximum-permitted uncertainty of measurement ( $\pm$ dB)
30-130	94.0	94.0	0.0	1.1	0.30	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

7 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

**8. Level linearity including the level range control**

At reference level at 5 dB greater than the under-range on a level range

Range	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
30-130	35.0	35.0	0.0	1.1	0.30	0.3

**9. Tone burst response**

Time Weighting	Toneburst Duration, Tb (ms)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Fast	200	126.0	0.0	±1.0	0.20	0.3
	2	109.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	99.9	-0.1	+1.5; -5.0	0.20	0.3
Slow	200	119.6	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -5.0	0.20	0.3
SEL	200	120.0	0.0	±1.0	0.20	0.3
	2	100.0	0.0	+1.0; -2.5	0.20	0.3
	0.25	90.9	-0.1	+1.5; -5.0	0.20	0.3

Date of Calibration : 23 Feb.2024-1 Mar.2024

8 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

**Head Office**

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand  
Tel. (66) 0 2577 9000  
Fax. (66) 0 2577 9009  
E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

**Office/Laboratory**

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand  
Tel. (66) 0 2323 1672-80 ext. 115, 116  
Fax. (66) 0 2323 9165  
E-mail : mtc@tistr.or.th

**Office**

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand  
Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217  
Fax. (66) 0 2579 8592  
E-mail : sumalee@tistr.or.th



THAILAND INSTITUTE OF SCIENTIFIC AND TECHNOLOGICAL RESEARCH (TISTR)

Request No. 21-67/0232

MTC No. EEL. BP. 177/0167

10. Peak C sound level

Number of cycles in test signal	Anticipated value (dB)	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Complete cycle	125.4	125.2	-0.2	3.0	0.20	0.35
Positive half cycle	124.4	124.1	-0.3	2.0	0.20	0.35
Negative half cycle	124.4	124.1	-0.3	2.0	0.20	0.35

11. Overload indication

Measured value (dB)		Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Positive one-half cycle	Negative one-half cycle				
135.5	135.5	0.0	1.5	0.20	0.25

12. High-level stability

Time	Measured value (dB)	Deviated value (dB)	Acceptance limit class 2 (±dB)	Uncertainty (±dB)	Maximum-permitted uncertainty of measurement (±dB)
Begin	129.0	0.0	0.3	0.10	0.1
End	129.0				

Calibrated by :

*Tawikiat Iamsamran*

(Mr. Tawikiat Iamsamran)

Approved by :

*Prawate Kluaypa*

(Mr. Prawate Kluaypa)

Director

Electrical and Electronic Standards Laboratory

Industrial Metrology and Testing Service Centre

Date of Calibration : 23 Feb.2024-1 Mar.2024

Date of Issue : 1 Mar. 2024

Ref : 2011267012400347007

End of Certificate

9 / 9

The results relate only to the items tested/calibrated or value assigned.

Advertising the Report/Certificate and publicity of the results except in full are prohibited unless written permission is obtained from the governor of TISTR.

FM.BL.MTC.002 Rev.4

Head Office

35 Mu 3 Tambon Khlong Ha, Amphoe Khlong Luang,  
Changwat Pathumthani 12120, Thailand

Tel. (66) 0 2577 9000

Fax. (66) 0 2577 9009

E-mail : rumpai@tistr.or.th Website:www.tistr.or.th

Office/Laboratory

Soi 1C, Bangpoo Industrial Estate, Sukhumvit Road,  
Amphoe Muang, Changwat Samutprakan 10280, Thailand

Tel. (66) 0 2323 1672-80 ext. 115, 116

Fax. (66) 0 2323 9165

E-mail : mtc@tistr.or.th

Office

196 Phahonyothin Road, Chatuchak, Bangkok 10900,  
Thailand

Tel. (66) 0 2579 1121-30 ext. 5219, 5225, 5217

Fax. (66) 0 2579 8592

E-mail : sumalee@tistr.or.th



TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23E3924

Page : 1 of 2

Equipment : pH Meter  
Manufacturer: Mettler Toledo  
Model : SevenExcellence  
Serial No.: B834291445  
ID No.: RYG\_EN0152  
Condition As-Received: Used Item  
Received Date: 08 December 2023  
Calibration Date: 14 December 2023

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Reference: 2312-0151DSC  
Ambient Temperature: ( 23 ± 2 ) °C  
Relative Humidity: ( 50 ± 10 ) %

Submitted by: ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch

616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,  
Rayong 21140, Thailand

Procedure used: Calibration were conducted using calibration procedure No. CP-E17 according to EURAMET cg-15.

### Condition of this result of calibration

1.Reference standards instruments :


Instrument	Model	Serial No.	Certificate No.	Due Date
1) Multi-Product Calibrator	5502A	2435802	EE-0041-23	26 Apr 2024

2.This result of calibration was made on requested at the point specified by customer.

3.The certificate is valid only to the item calibrated on date and place of calibration.

4.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

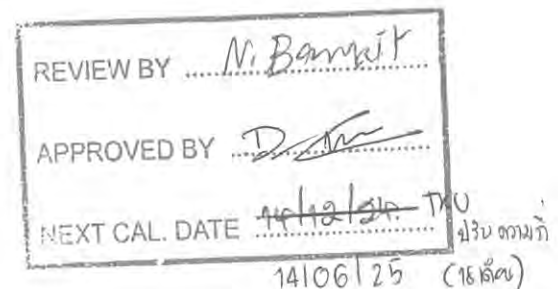

Calibrated by : Napachanok Prasomsoosiri  
Issue Date : 15 December 2023

Approved Signatory :

- [ ] Phalinee Prabpaipal  
[✓] Nuntawat Khamchai  
[ ] Pongsagorn Boonyaporn

B 0331106



Cert. No.: 23E3924

Page.: 2 of 2

**Result of calibration :-** (\*) Without adjustment ( ) After adjustment

**Function:** DC voltage measurement

**Range:**

2000

mV

<u>Standard Value</u>	<u>UUC* Reading</u>	<u>Error</u>	<u>Uncertainty</u>
( mV )	( mV )	( mV )	( $\pm$ $\mu$ V )
-200.0000	-199.9	0.1	68
-150.0000	-150.0	0.0	65
-100.0000	-100.0	0.0	63
-50.0000	-50.0	0.0	61
0.0000	0.0	0.0	58
50.0000	50.0	0.0	61
100.0000	100.0	0.0	63
150.0000	150.0	0.0	65
200.0000	199.9	-0.1	68

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k=2$ , providing a level of confidence of approximately 95 %

**UUC\*= Unit Under Calibration.**

-o0o-

a 1193422





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3; EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL. 0-2717-3000-29 FAX. 0-2719-9484



Cert.No.: 23CH1574

Page.: 1 of 3

## Certificate of Calibration

Equipment :	pH Meter
Manufacturer :	Mettler Toledo
Model :	SevenExcellence
Serial No. :	B834291445
ID No. :	RYG_EN0152
Condition As-Received:	Used Item
Received Date :	08 December 2023
Calibration Date :	15 December 2023
Reference :	2312-0151DSC-3
Submitted by :	ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch 616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng, Rayong 21140, Thailand
Ambient Temperature :	(25 ± 2.5) °C
Relative Humidity :	(50 ± 15) %
Calibration Procedure :	In - house method : - CP-CH5 by direct measurement with standard voltage calibrator and direct measurement with certified reference material (CRM) - CP-CH8 by comparison with standard thermometer

Calibrated by : Warakorn Lerngagtrakul

Approved by :

Approved Signatory

- ( ) Saithip Meangmai  
( ) Warakorn Lerngagtrakul  
( ☒ ) Ponpan Paipim

Issue Date : 19 December 2023

The Uncertainties are for a confidence probability of approximately 95%

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 ; Equipment Calibration and Testing Services.

A 0061696



Cert.No.: 23CH1574

Page.: 2 of 3

**Condition of this calibration result**

1. Reference Standard Instrument : -

<u>Instrument</u>	<u>Serial No.</u>	<u>ID No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
1) Document Process Calibrator	54030049	130RC116	23E2802	27 Aug 2024
2) Ref. Standard Thermometer	4982054	110RC044	23I908	26 July 2024

This certification is traceable to the International System of Unit maintained through:-

- Technology Promotion Association (Thailand-Japan)

2. Certified Reference Materials : The measurement results are traceable to SI through CPA chem Ltd.,  
ANSI-ASQ National Accreditation Board, Accredited No. AR-1835

<u>Buffer Solution</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. date</u>
pH 4.008	CPA chem	913598	14 July 2025
pH 6.986	CPA chem	931959	01 Oct 2024
pH 9.997	CPA chem	940106	02 Nov 2024

3. This certificate is valid only to the item calibrated on date and place of calibration.

**Calibration Results**

**Function : mV Measurement**

**Performing standard curve by Fluke at pH (4,7,10)**

Unit Under Calibration	Nominal Value	Standard Voltage Input	Actual Reading		Uncertainty of Measurement ( ±mV )	Coverage factor <i>k</i>
	pH	mV	mV	pH		
pH Meter S/N.: B834291445	4.000	177.48	177.3	4.000	0.058	2.00
	7.000	0.00	-0.1	7.000	0.058	2.00
	10.000	-177.48	-177.5	10.000	0.058	2.00

a 1193852



Cert.No.: 23CH1574

Page.: 3 of 3

**Calibration Results****Function : pH Measurement**

Performing three buffers standard curve by using buffer nominal pH (4,7,10)

Unit Under Calibration	Standard pH Buffer Solution	Actual pH Reading	Actual mV Reading ( mV )	Uncertainty of pH measurement ( $\pm$ )	Coverage factor $k$
pH Electrode S/N.: 3225368	4.008	4.013	184.1	0.0045	2.00
	6.986	6.998	8.7	0.0084	2.00
	9.997	10.002	-164.7	0.0088	2.11

**Function : Temperature Measurement****( \* ) Without adjustment**

This equipment was connected with Temperature Probe;

- Model : InLab®Expert Pro-ISM  
- Serial No. : 3225368

Dimension of probe;

- Length : 120 mm  
- Diameter : 12 mm  
- Immersion Depth : 100 mm

Calibration Point ( °C )	Standard Temperature ( °C )	UUC* Reading ( °C )	Error ( °C )	Uncertainty of measurement ( $\pm$ °C )	Coverage factor $k$
25.0	25.003	24.3	-0.703	0.13	2.00

**Remark : - UUC\* = Unit Under Calibration**

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

-o0o-

a 1193851





**SARTORIUS**

NSC-TISI-TIS 17025  
CALIBRATION 0426

# Certificate

## of Calibration

REVIEW BY Tranitall.

APPROVED BY D. [Signature]

NEXT CAL. DATE 22/02/2025

Model Number : MSE224S-100-DU

Certificate No. : 24BC10069

Description : Analytical Balance

Issued Date : Friday, February 23, 2024

Serial Number : 0026207038

Reference No. : 229196

ID No. : RYG\_EN0002

Manufacturer : Sartorius

Page No. : 1 of 2

Customer Name : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)

616/10 Moo 5 T.Maenam Khu, A.Pluak Daeng, Rayong 21140, Thailand.

Calibrated Place : ALS Laboratory Group (Thailand) Co., Ltd.(Balance Room)

616/10 Moo 5 T.Maenam Khu, A.Pluakdaeng, Rayong.21140, Thailand.

Calibrated By : Mr.Chonchai Inthana

Calibration Date : Thursday, February 22, 2024

Calibration

Procedure No. : This calibration was conducted by

Using in-house calibration procedure number (WI-003)

Based on UKAS LAB 14 : 2019

*Metrological data :*

Capacity : 220 g Readability : 0.0001 g

*Ambients Conditions:*

Temperature : 24.2 °C ± 5.0 °C

Humidity : 57.0 % RH ± 10.0 % RH

Pressure :                      ±                     

*Reasons for calibration*

☐ New Installation ☐ Service / Repaired ☒ Re-calibration/ Maintenance

*Equipment Condition:* ☒ Good Operate ☐ Fair

## Measurement Method UKAS Publication Ref :Lab 14

The measurement uncertainty stated is the expended uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM). The calibration certificate documents the traceability to National Standards, which realise the unit of measurement according to the International Standard System of Units (SI). Report of Tolerance came form list of Sartorius Metrological Specifications.

## Traceability:

Model Number	Description	Traceability	Certificate No.	Due Date
YCS011-522-00	Sartorius weight set 1mg - 5000g E2,YCS011-522-00	TCS	M2308197S	23-Aug-2025
MHB-382SD	Humidity/Barometer/Temp Lutron MHB-382SD	DKSH	C19231845	23-Aug-2024

This certificate relate and apply this equipment only.

This certificate may not be reproduced other than in full except with the prior written approval of the Verification Operation Division  
Sartorius (Thailand) Co., Ltd.

[Signature]

Mr.chonchai Inthana(Technical Manager)

S  
T  
A  
M  
P



**Sartorius (Thailand) Co., Ltd.**

129 Rama 9 Road, Huaykwang, Huaykwang, Bangkok 10310

Tel: +66 2643 8361-6 Fax: +66 2643-8367, e-mail: service.thailand@sartorius.com

**SARTORIUS**

# Certificate of Calibration

Model Number : MSE224S-100-DUDescription : Analytical BalanceSerial Number : 0026207038ID No. : RYG\_EN0002Manufacturer : SartoriusCertificate No. : 24BCI0069Issued Date : Friday, February 23, 2024Reference No. : 229196Page No. : 2 of 2

## Calibration Results : Without Adjustment

### Repeatability


The reproducibility is the ability of a weighing instrument to display nearly identical readouts under constant test conditions when the same load within a measurement series is placed repeatedly on the weighing pan in the same manner. The standard deviation is used to express reproducibility quantitatively.

Nominal Value : (Low Load)	20.0000	199.9999
20 g	20.0000	200.0000
Tolerance	20.0001	200.0000
0.0001 g	20.0000	199.9999
	20.0001	200.0000
Nominal Value : (High Load)	19.9999	200.0000
200 g	20.0000	200.0000
Tolerance	20.0000	199.9999
0.0001 g	19.9999	200.0001
	19.9999	200.0000
Standard Deviation	0.00007	0.00006

### Eccentricity (Off-center loading error)

The off-center loading error is yielded by the difference between the readout of the load, i.e. 1/3 or 1/4 of maximum capacity, placed in the middle of the weighing pan and between each of four additional measurement points (positions defined according to OIML R76).

Nominal value : 100 g  
Tolerance 0.0004 g



Difference	
1	-
2	-0.0001
3	-0.0001
4	0.0000
5	-0.0001
6	-

### Linearity

The linearity, also called linearity error. Describes the deviation of the characteristic curve of a weighing instrument from the linear slope.

Tolerance 0.0002 g

Nominal Value (g)	Conventional Mass Value (g)	Displayed Value (g)	Deviation (g)	Uncertainty (g)
0.01	0.0100	0.0100	0.0000	0.00018
0.05	0.0500	0.0500	0.0000	0.00018
0.1	0.1000	0.1000	0.0000	0.00018
0.5	0.5000	0.5000	0.0000	0.00018
1	1.0000	1.0000	0.0000	0.00018
5	5.0000	5.0000	0.0000	0.00018
10	10.0000	10.0000	0.0000	0.00018
20	20.0000	20.0000	0.0000	0.00024
50	50.0000	49.9999	-0.0001	0.00019
100	100.0000	100.0000	0.0000	0.00023
200	200.0000	199.9999	-0.0001	0.00032

End of Report.



## Certificate of Calibration

Cert. No.: 24TM632

Page : 1 of 3

**Equipment :** Hot Air Oven  
**Manufacturer :** Memmert  
**Model :** UFE 500  
**Serial No. :** G511.1572  
**ID No. :** RYG\_EN0010

REVIEW BY *Thanitak.*

APPROVED BY *D. J. J. J.*

NEXT CAL DATE *21/09/25*

**Submitted by :** ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)  
616/10 Moo 5 T. Maenam Khu,  
A. Pluakdaeng,  
Rayong 21140 Thailand

**Location :** Oven Room

**Received Order :** 21 March 2024

**Calibration Date :** 21 March 2024

**Ambient Temperature :** ( 26 ± 10 ) °C

**Relative Humidity :** ( 50 ± 30 ) %

**Calibrated by :** Man Pattanapongpaiboon

**Approved by :**

Approved Signatory

( ) Pornthippa Tameyakul

( ) Unnopphol Harachai

(✓) Suwit Imjai

**Issue Date :** 22 March 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.





**Equipment :** Hot Air Oven  
**Condition As-Received :** Used Item  
**Reference :** 2403-0563OC-1  
**Procedure Used :-**

**Cert. No.:** 24TM632

**Page :** 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

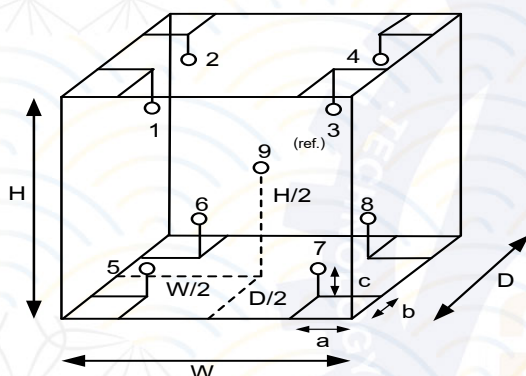

Environment during calibration		
	Beginning	Finished
Temp. ( °C )	27	27
REL.Humid. ( % )	57	59
AC Supply ( Volt )	222	224

**Ref. Std. ID No.: @  
Calibration Point**

Position :	( 180 ) °C	( 104 ) °C
1	18-18TC-01	18-18RTD-01
2	18-18TC-02	18-18RTD-02
3	18-18TC-03	18-18RTD-03
4	18-18TC-04	18-18RTD-04
5	18-18TC-05	18-18RTD-05
6	18-18TC-06	23-18RTD-06
7	18-18TC-07	18-18RTD-07
8	18-18TC-08	22-18RTD-08
9 (ref.)	18-18TC-09	18-18RTD-09

**Probe Installation Details :**

a = 5.0 cm  
b = 5.0 cm  
c = 5.0 cm

**Dimension of Chamber :**

D = 0.40 m  
W = 0.56 m  
H = 0.48 m  
Capacity = 0.11 m<sup>3</sup>



**Equipment :** Hot Air Oven  
**Condition As-Received :** Used Item  
**Reference :** 2403-0563OC-1  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Close

**Cert. No.:** 24TM632

**Page :** 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.051	0.59	0.62	2
180.0	180.0	180.0	0.15	1.3	1.7	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ± °C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	103.921	103.786	103.757	103.759	103.950	103.817	104.213	103.672	103.673	0.42
180.0	179.614	179.270	179.145	179.599	180.001	180.423	180.293	180.629	179.429	1.1

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert. No.: 24TM634

Page : 1 of 3

Equipment : Hot Air Oven  
Manufacturer : Memmert  
Model : UF 110  
Serial No. : B423.0853  
ID No. : RYG\_EN0213

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)  
616/10 Moo 5 T. Maenam Khu,  
A. Pluakdaeng,  
Rayong 21140 Thailand

Location : Oven Room

Received Order : 21 March 2024  
Calibration Date : 21 - 22 March 2024  
Ambient Temperature : (  $26 \pm 10$  ) °C  
Relative Humidity : (  $50 \pm 30$  ) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul  
( ) Unnopphol Harachai  
(✓) Suwit Imjai

Issue Date : 23 March 2024

REVIEW BY *Thanita K.*  
APPROVED BY *D. Khunon.*  
NEXT CAL DATE *21/03/25*

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.





**Equipment :** Hot Air Oven  
**Condition As-Received :** Used Item  
**Reference :** 2403-0563OC-3  
**Procedure Used :-**

**Cert. No.:** 24TM634

**Page :** 2 of 3

Calibration were conducted using calibration procedure CP-OT02 according to direct measurement method with Data Acquisition which connected with Resistance Temperature Detector ( RTD ) and Thermocouple Type T.

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.


3. This certification is traceable to the International System of Unit.

**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Fresh air setting :** Close

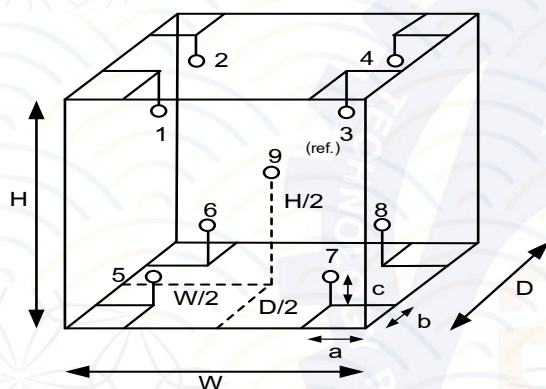

<b>Environment during calibration</b>		
	<b>Beginning</b>	<b>Finished</b>
Temp. ( °C )	27	27
REL.Humid. ( % )	59	59
AC Supply ( Volt )	224	223

**Ref. Std. ID No.: @  
Calibration Point**

<b>Position :</b>	<b>( 180 ) °C</b>	<b>( 104 ) °C</b>
1	18-18TC-01	18-18RTD-01
2	18-18TC-02	18-18RTD-02
3	18-18TC-03	18-18RTD-03
4	18-18TC-04	18-18RTD-04
5	18-18TC-05	18-18RTD-05
6	18-18TC-06	23-18RTD-06
7	18-18TC-07	18-18RTD-07
8	18-18TC-08	22-18RTD-08
9 (ref.)	18-18TC-09	18-18RTD-09

**Probe Installation Details :**

**Dimension of Chamber :**

a =	5.0	cm	D =	0.40	m
b =	5.0	cm	W =	0.56	m
c =	5.0	cm	H =	0.48	m
			Capacity =	0.11	m <sup>3</sup>



**Equipment :** Hot Air Oven  
**Condition As-Received :** Used Item  
**Reference :** 2403-0563OC-3  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source  
**Fresh air setting :** Close

**Cert. No.:** 24TM634

**Page :** 3 of 3

Calibration Point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Temperature stability ( ± °C )	Temperature uniformity ( °C )	Overall Variation ( °C )	Coverage Factor <i>k</i>
104.0	104.0	104.0	0.065	0.52	0.90	2
180.0	180.0	180.0	0.20	1.2	2.0	2

Calibration Point ( °C )	Measured Temperature ( °C )									Uncertainty  ( ±°C )
	Position									
	1	2	3	4	5	6	7	8	9 (ref.)	
104.0	104.169	103.506	103.898	103.712	103.772	103.730	104.289	103.805	103.798	0.42
180.0	180.701	179.239	179.935	179.999	180.127	180.138	180.895	179.313	180.211	1.1

**Average\* :** The average of 30 values in each position.

**Temperature stability :** One-half of the greatest maximum difference of measured temperature at any one sensor.

**Temperature uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Overall Variation :** The Difference of the maximum and minimum measured temperatures throughout observation.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity .

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor *k*, providing a level of confidence of approximately 95 %.

-o0o-





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG BANGKOK 10250  
TEL.0-2717-3000-29 FAX.0-2719-9484



## Certificate of Calibration

Cert. No.: 24TM635

Page : 1 of 3

Equipment : Water Bath  
Manufacturer : Memmert  
Model : WNB22  
Serial No. : L513.0648  
ID No. : RYG\_EN0061

Submitted by : ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)  
616/10 Moo 5, T. Maenam Khu,  
A. Pluakdaeng,  
Rayong 21140, Thailand

Location : Wet Chemistry Lab

Received Order : 21 March 2024

Calibration Date : 21 March 2024

Ambient Temperature : (  $26 \pm 10$  ) °C

Relative Humidity : (  $50 \pm 30$  ) %

Calibrated by : Man Pattanapongpaiboon

Approved by :

Approved Signatory

( ) Pornthippa Tameyakul

( ) Unnoppol Harachai

(☒) Suwit Imjai

Issue Date : 23 March 2024

**The Uncertainties are for a confidence probability of approximately 95%**

This certificate may not be reproduced other than in full, except with the prior written  
Approval of the head of Corporate Services 3 : Equipment Calibration and Testing Services.





**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2403-0563OC-4  
**Procedure Used :-**

**Cert. No.:** 24TM635

**Page :** 2 of 3

Calibration were conducted using in-house calibration procedure CP-OT04 Based on ASTM E715 according to direct measurement method with Data Acquisition which connected with Industrial Platinum Resistance Thermometer ( IPRT ).

The temperature scale used was based on ITS-90.

**Condition of this result of calibration**

1. Reference standard instrument:-

<u>Instrument</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Traceable</u>	<u>Due Date</u>
1 ) Data Acquisition	MY57013711	23LM115	TPA	11 Jul 2024

2. This certificate is valid only to the item calibrated on date and place of calibration.

3. This certification is traceable to the International System of Unit.


**Remark :** TPA : Technology Promotion Association ( Thailand - Japan )

**Result of Calibration :-** ( \* ) Without Adjustment

**Function of UUC\* :** Temperature Source

**Heat transfer medium used :** Water

	<u>Environmental</u>		<u>AC Voltage Supply</u>
	( °C )	( %R.H. )	( Volt )
<b>Beginning of Calibration</b>	25	55	222
<b>Finished of Calibration</b>	25	57	223

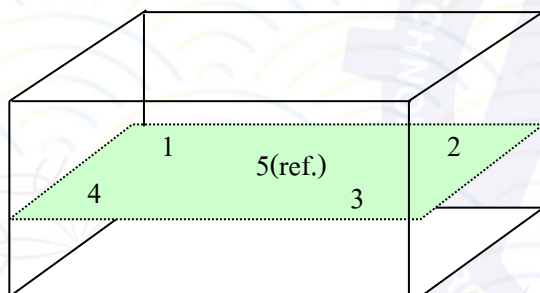

Front

<u>Position :</u>	<u>Ref. Std. ID No.:</u>
1	4803988-001
2	4803988-002
3	4803988-003
4	4803988-004
5(ref.)	4803988-005



**Equipment :** Water Bath  
**Condition As-Received :** Used Item  
**Reference :** 2403-0563OC-4  
**Result of Calibration :-** ( \* ) Without Adjustment  
**Function of UUC\* :** Temperature Source

**Cert. No.:** 24TM635

**Page :** 3 of 3

Calibration point ( °C )	UUC* Setting ( °C )	UUC* Reading ( °C )	Average* Standard Reading ( °C )					Uncertainty
			Position					
			1	2	3	4	5 (ref.)	( ± °C )
85.0	85.0	85.0	84.428	84.424	84.489	84.507	84.477	0.18

Calibration point ( °C )	Uniformity ( °C )	Stability ( ± °C )	Coverage Factor <b>k</b>
85.0	0.19	0.11	2

**Average\* :** The average of 30 values in each position.

**Uniformity :** The maximum difference of measured temperatures at any sensors and the measured temperature at the reference location which are observed at the same time or at as close an observation time as possible to determine the temperature pattern or homogeneity within the chamber under steady-state conditions.

**Stability :** One-half of the greatest maximum difference of measured temperature at any one probe.

**UUC\* :** Unit Under Calibration

**Note :** The reported uncertainty of measurement was included stability and excluded uniformity.

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor **k**, providing a level of confidence of approximately 95 %.

-o0o-





## Certificate of Calibration

Certificate No. : 24T726

Page : 1 of 2

**Equipment :** Digital Thermometer

**Manufacturer:** Testo

**Model :** 106

**Serial No.:** 83461616/0721

**ID No.:** RYG\_FS0568

**Condition As-Received:** Used Item

**Received Date:** 29 March 2024

**Calibration Date:** 23 April 2024  
to 25 April 2024

**Reference:** 2403-1017DSC

**Ambient Temperature:** ( 25 ± 3 ) °C

**Relative Humidity:** ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

**Submitted by:** ALS Laboratory Group (Thailand) Co.,Ltd. Rayong Branch

616/10 Moo 5, T.Maenam Khu, A.Pluakdaeng,  
Rayong 21140, Thailand

**Procedure used:** Calibration were conducted using in-house calibration procedure CP-T01 according to comparison with Industrial Platinum Resistance Thermometer (IPRT) into liquid bath temperature controller.  
The temperature scale used was based on ITS-90.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Black Stack Thermometer	1560	8C454	23I600	30 May 2024
2) PRT Scanner Module	2562	A01303	23I600	30 May 2024
3) Industrial PRT Probe	5627A	979442	23I600	30 May 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through-

-Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

REVIEW BY Pitthaya T.  
APPROVED BY Supt S.  
NEXT CAL DATE 23/04/25

**Calibrated by :** Anuchit Pangchata  
**Issue Date :** 30 April 2024

**Approved Signatory :**

- [ ] Phalinee Prabpaipal  
[ ] Chatchawan Khunpiluek  
☒ Wanlop Larpkern





Cert. No.: 24T726

Page.: 2 of 2

**Result of Calibration:-**

Without Adjustment

**Function:**

Temperature measurement


Dimension of probe : Diameter 3 mm., Length 55 mm. Sheath material : Stainless Steel

<b>Immersion</b>	<b>Standard</b>	<b>UUC*</b>		<b>Uncertainty</b>
<b>Depth</b>	<b>Temperature</b>	<b>Reading</b>	<b>Error</b>	<b>of Measurement</b>
( mm.)	( °C )	( °C )	( °C )	( ±°C )
50	25.0016	24.9	-0.1016	0.12
50	30.0023	29.9	-0.1023	0.12
50	40.0018	40.0	-0.0018	0.12

**UUC\*** : Unit Under Calibration

The reported uncertainty of measurement was based on standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95%.

-o0o-

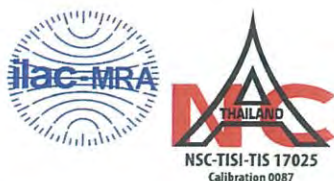

# Certificate of Calibration

<b>Equipment:</b>	SPECTROPHOTOMETER	<b>Certificate No.:</b>	C06230441
<b>Model:</b>	DR6000	<b>Issued Date:</b>	19 September 2023
<b>Serial No. (or ID.):</b>	1627845 (RYG_EN0037)	<b>Job No.:</b>	WO-00005382
<b>Manufacturer:</b>	HACH	<b>Page:</b>	1 of 3
<b>Condition:</b>	In Condition		

**Customer:** ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch)  
616/10 Moo 5 T.Maenam Khu,  
A.Pluakdaeng, Rayong 21140, Thailand.

**Environment Condition:**

Temperature	23.9	°C	±	0.2
Humidity	65.3	%RH	±	1.4

REVIEW BY	<i>N. Banerjee</i>
APPROVED BY	<i>D. [Signature]</i>
NEXT CAL. DATE	18/3/25

**Calibration Place:** ALS Laboratory Group (Thailand) Co.,Ltd. (Rayong Branch) (Wet Chemistry)  
616/10 Moo 5 T.Maenam Khu,  
A.Pluakdaeng, Rayong 21140, Thailand.

**Calibration By:** Mr.Nattapat Rungrueng

**Calibration Date:** 18 September 2023

**The Method used:** In house method, CAL-WI-24, base on ASTM E 275-08 and ASTM E 387-04

**Traceability:** This certificate is traceable to the CRM maintained by National Institute of Standards and Technology (NIST) through Starna Scientific Limited.

The standard for Wavelength Certificate No. 111583 and 111584  
The standard for Photometric Certificate No. 9114984 and 111588  
The standard for Stray light Certificate No. 111586 and 111585  
The standard for Spectral resolution Certificate No. 111587

*[Signature]*  
(Mr. Nattapat Rungrueng)  
Person in charge

*[Signature]*  
(Mr. Nitinun Srihawan)  
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

บริษัท ดีเคเอสเอช เทคโนโลยี จำกัด  
DKSH Technology Limited  
2533 ถนนสุขุมวิท แขวงบางจาก เขตพระโขนง กรุงเทพมหานคร 10260  
2533 Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260  
Phone: +66 2639 7000 Email: info.calibration@dksh.com Website: www.dksh.com/scientific-thailand



## Calibration Results:

### Without Adjustment

Wavelength Accuracy (nm), The spectral bandwidth of Std at 2 nm and UUC at 2 nm

Standard Wavelength	Unit Under Calibration	Correction	Uncertainty
418.61	418.3	0.31	0.13
536.66	536.6	0.06	0.13
637.98	638.3	-0.32	0.13
748.48	748.7	-0.22	0.13
807.03	807.4	-0.37	0.13

Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
420 nm	0.0000	0.000	0.0000	0.0045
	0.2930	0.289	0.0040	0.0045
	0.5168	0.519	-0.0022	0.0045
	1.0298	1.029	0.0008	0.0045
440 nm	0.0000	0.000	0.0000	0.0045
	0.2867	0.283	0.0037	0.0045
	0.5073	0.509	-0.0017	0.0045
	1.0083	1.007	0.0013	0.0045
465 nm	0.0000	0.000	0.0000	0.0045
	0.2516	0.250	0.0016	0.0045
	0.4595	0.462	-0.0025	0.0045
	0.9334	0.933	0.0004	0.0045
546.1 nm	0.0000	0.000	0.0000	0.0045
	0.2461	0.245	0.0011	0.0045
	0.4652	0.466	-0.0008	0.0045
	0.9468	0.946	0.0008	0.0045
590 nm	0.0000	0.000	0.0000	0.0045
	0.2594	0.259	0.0004	0.0045
	0.5040	0.505	-0.0010	0.0045
	1.0032	1.002	0.0012	0.0045
635 nm	0.0000	0.000	0.0000	0.0045
	0.2579	0.257	0.0009	0.0045
	0.4971	0.497	0.0001	0.0045
	0.9720	0.971	0.0010	0.0045



## Calibration Results:

### Without Adjustment

#### Photometric Accuracy (Absorbance)

Wavelength	Standard absorbance	Unit Under Calibration	Correction	Uncertainty
235 nm	0.0000	0.000	0.0000	0.0080
	0.7355	0.737	-0.0015	0.0080
257 nm	0.0000	0.000	0.0000	0.0080
	0.8574	0.857	0.0004	0.0080
313 nm	0.0000	0.000	0.0000	0.0080
	0.2864	0.290	-0.0036	0.0080
350 nm	0.0000	0.000	0.0000	0.0080
	0.6374	0.637	0.0004	0.0080

#### Stray light \*

Standard: cut-off	UUC: Wavelength (nm)	UUC: Transmission (%T)	Absorbance (A)
260.62 +/- 0.11 nm	260.6	1.3	1.886
391.44 +/- 0.11 nm	391.4	1.3	1.886

#### Spectral Resolution \*

Nominal Concentration 0.02 % v/v	Peak	Trough	Ratio	SBW
Standard Wavelength ( nm )	268.66	266.69	1.38	2.00
UUC: Wavelength (nm)	268.2	266.1		
Std Absorbance ( A )	0.4566	0.2780		
Absorbance ( A )	0.413	0.300		

\* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

**The End of Certificate**

## ใบตรวจสอบสภาพเครื่องวัดสิ่งแวดล้อม

เลขที่ใบงาน: WO-00005382

ชนิดเครื่องมือ: SPECTROPHOTOMETER

รุ่น: DR6000

หมายเลขเครื่อง: 1627845

ตรวจสอบ (รับ)		รายการตรวจเช็ค	ตรวจสอบ (ส่ง)		หมายเหตุ
18 Sep 2023			18 Sep 2023		
ปกติ	ไม่ปกติ		ปกติ	ไม่ปกติ	
		General			
<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. ความสมบูรณ์เครื่อง	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. ความสะอาด ( ช่องใส่ตัวอย่าง, ภายใน-นอกเครื่อง)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	3. สวิตช์ ปิด – เปิด เครื่อง (On-Off Swicth)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. ปุ่มกด (Keypad)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. หน้าจอ (Display, Screen Contrast)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		Spectrophotometer			
<input type="checkbox"/>	<input type="checkbox"/>	6. แรงดันไฟฟ้า (Battery Backup) >= 2.5 VDC	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	7. ตัวหมุนเลือกความยาวคลื่น (Wavelength Control)	<input type="checkbox"/>	<input type="checkbox"/>	
<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. ความยาวคลื่น (Wavelength Check)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	*
<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. แหล่งกำเนิดแสง (UV < 3,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	9.2 Hours
<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. แหล่งกำเนิดแสง (Visible < 5,000 hour)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	741.5 Hours
<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. ช่องวัดหลายตัวอย่าง (Carousel Module)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
		pH Meter and Conductivity Meter			
<input type="checkbox"/>	<input type="checkbox"/>	12. อิเล็กโทรด ( Electrode and Connection Cable )	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	13. ระดับสารละลายใน Electrode (Level KCl )	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	14. ฝาปิดกันปลาย Electrode (Dust Protection Hood)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	15. ขาจับอิเล็กโทรด (Stand)	<input type="checkbox"/>	<input type="checkbox"/>	
		Turbidimeter			
<input type="checkbox"/>	<input type="checkbox"/>	16. ค่าความขุ่นที่ต่ำสุด (No Sample)	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	17. ระดับการส่องสว่างของแสง (>= 2.5 ไม่เกิน 3.0)	<input type="checkbox"/>	<input type="checkbox"/>	
		Automatic titrator			
<input type="checkbox"/>	<input type="checkbox"/>	18. สภาพ Piston Burettes	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	19. Function Rinsing and Dosing	<input type="checkbox"/>	<input type="checkbox"/>	
<input type="checkbox"/>	<input type="checkbox"/>	20. ระบบท่อสายยางและอุปกรณ์ประกอบ	<input type="checkbox"/>	<input type="checkbox"/>	

เพิ่มเติม/ข้อแนะนำ : \*656.1nm=656.1nm

\*486.0nm=485.5nm

Mr.Nattapat Rungrueang

Service Engineer





# Metrology

SCI ECO Services Company Limited

33/2 Moo 3, T.Banpa, A.Kaengkhoi, Saraburi 18110, Thailand.

Saraburi Tel : +66 3627 3096 Fax : +66 3627 3100

Bangkok Tel : +668 9205 6851 , +669 8247 2360  
Website : www.scieco.co.th E-Mail : calibrate@scg.com



Certificate No. T241120

Page 1 of 4

## Certificate of Calibration

**Equipment** : Chamber ( Cold Room )

**Manufacturer** : MODULAR

**Model** : IREVCOHCOO

**Serial No.** : C00351459

**Customer Code** : RYG\_EN0184


**ID No.** : T1939A5

**Customer** : ALS Laboratory Group (Thailand) Co.,Ltd. ( Rayong Branch)  
616/10 Moo 5 T.Maenam Khu,  
A.Plukdaeng, Rayong 21140


**Customer Location** : Laboratory

**Date of Receipt** : 5 June 2024

**Calibrated By** : Sujjar Naknakred ( Site Calibration Manager )

**Approved By** :  Preecha Phisassutthikul (Temperature Calibration Manager)

**Date of Issue** : 12 JUN 2024

REVIEW BY	Thanitall.
APPROVED BY	
NEXT CAL. DATE	11/12/25

The uncertainties are for a confidence probability of approximately 95%.

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standard laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the Metrology.






Certificate No. T241120

Page 3 of 4

## Calibration Report

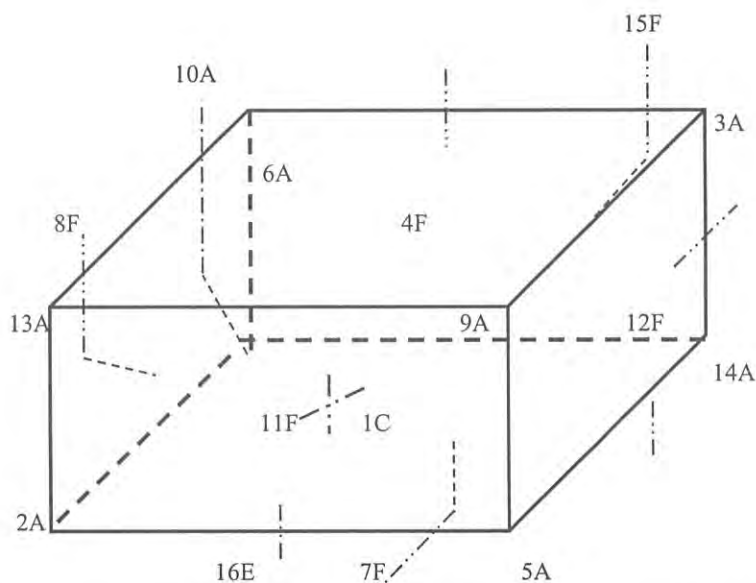

C = Centre , F = Centre of Face , A = Corner , E = Centre of Edge

1C	=	TN161
2A	=	TN162
3A	=	TN163
4F	=	TN164
5A	=	TN165
6A	=	TN166
7F	=	TN167
8F	=	TN168
9A	=	TN169
10A	=	TN170

11F	=	TN171
12F	=	TN172
13A	=	TN173
14A	=	TN174
15F	=	TN175
16E	=	TN176

Approved By. 

Certificate No. T241120

Page 4 of 4

## Calibration Report

### Measurement Results:

Calibration Point	Average Standard Reading at each position (°C)									
	TN161	TN162	TN163	TN164	TN165	TN166	TN167	TN168	TN169	TN170
3	2.73	2.70	2.77	2.78	2.99	2.35	3.09	3.21	3.08	2.90
	TN171	TN172	TN173	TN174	TN175	TN176				
	3.39	3.01	2.92	2.81	3.42	3.42				

Chamber ( Cold Room )			Temperature Distribution				
Setting (°C )	Reading (°C )		Average (°C )	Stability ( $\pm$ °C )	Uniformity (°C )	Uncertainty ( $\pm$ °C )	Coverage Factor $k$
	Min , Max	Average					
3.0	2.9 , 4.4	3.7	2.97	1.32	1.13	2.02	2.00

\* The quoted uncertainty exclude " uniformity "

The calibration result apply only the above calibrated item.

The result of test was found accurate as shown on date and place of test only.

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor  $k$  which for a t-distribution, providing a level of confidence of approximately 95 % .

Approved By. 