

ภาคผนวก จ

เอกสารเทียบเครื่องมือที่ใช้ในการตรวจวิเคราะห์

---

รายงานผลการปฏิบัติตามมาตรฐานการป้องกัน และแก้ไขผลกระทบสิ่งแวดล้อม และมาตรการติดตามตรวจสอบผลกระทบสิ่งแวดล้อม

สำหรับโครงการโรงไฟฟ้าชีวมวล (ส่วนขยาย) ระยะดำเนินการ ระหว่างเดือนมกราคม-มิถุนายน พ.ศ. 2567

บริษัท ไทยรุ่งเรือง โฮลดิ้ง จำกัด

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Laboratory Instrument/Equipments.(คุณภาพอากาศ)									
Equipment for Air Quality Analysis									
1	Analytical Balance (Readability 0.1 mg)	ฝุ่นละอองรวม (TSP) ฝุ่นละอองขนาดเล็กไม่เกิน 10 ไมครอน (PM-10)	Mettler-Toledo	AB204-S/FACT / B108115858	National Food Institute, Ministry of Industry, Thailand	2402420-001-01	19 Apr 24	18 Apr 25	-
2	Analytical Balance (Readability 0.001 mg)	ฝุ่นทุกขนาด (Total Dust) ฝุ่นขนาดเล็กที่เข้าถึงและสะสมในถุงลมของปอด (Respirable Dust)	Mettler-Toledo	XP6 / B322373893	National Food Institute, Ministry of Industry, Thailand	2402420-002-01	19 Apr 24	18 Apr 25	-
3	UV-VIS Spectrophotometer	ก๊าซออกไซด์ของไนโตรเจน (NO <sub>x</sub> as NO2)	Agilent	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP24-018	9 May 24	8 May 25	-
Equipment for Water Quality Analysis									
4	pH Meter	pH	Mettler-Toledo	Seven Easy S20 / 1230525212	DKSH (Thailand) Ltd.	C07240167	9 Apr 24	8 Apr 25	-
5	UV-VIS Spectrophotometer	Sulphate ไนเตรด (Nitrate, NO <sub>3</sub> <sup>-</sup> )	Agilent Technologies	Cary60 G6860A / MY15410009	DQE Services Co.,Ltd.	SP24-018	7 May 24	6 May 25	-

รายงานผลการปฏิบัติตามมาตรการป้องกัน และแก้ไขผลกระทบสิ่งแวดล้อม และมาตรการติดตามตรวจสอบผลกระทบสิ่งแวดล้อม

สำหรับโครงการโรงไฟฟ้าชีวมวล (ส่วนขยาย) ระยะดำเนินการ ระหว่างเดือนมกราคม-มิถุนายน พ.ศ. 2567

บริษัท ไทยรุ่งเรือง โฮลดิ้ง จำกัด

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Stack									
1	Pre-Test Console	Total Suspended Particulate	Apex Instruments, USA.	XC-572-V 1904011	Envi Equipment Service Co., Ltd.	E23-08066	5 Aug 23	4 Aug 24	-
2	Flue gas Analyzer	Sulphur Dioxide Oxide of Nitrogen as Nitrogen Dioxide	Testo	Testo 350 60899615	Entech Industrial Sulation Co., Ltd.	G 660354	20 Jun 23	19 Jun 24	-
Ambient									
1	Orifice Transfer Standard Calibrator	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Andersen Instruments, Inc.	G25A 1901	Jirantee Associates Co., Ltd.	COF-002-66	14 Jul 23	13 Jul 25	-
2	U-Tube Manometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Dwyer	1221-36-W/M -	Technology Promotion Association (Thailand-Japan)	23P1401	9 May 23	8 May 24	-
3	Aneroid Barometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23P1859	2 Jun 23	1 Jun 24	-
4	Dial Thermo-Hygrometer	Total Suspended Particulate (TSP) Particulate Matter < 10 µm (PM <sub>10</sub> )	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23H1200	6 Jun 23	5 Jun 24	-
5	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i CM19050150	UAE Consultant Co.,Ltd.	01112023	1 Nov 23	31 Oct 24	-
6	Nitrogen Dioxide Analyzer	Nitrogen Dioxide	Thermo Scientific	42i 1201778109	UAE Consultant Co.,Ltd.	21112023	21 Nov 23	20 Nov 24	-

รายงานผลการปฏิบัติตามมาตรฐานการป้องกัน และแก้ไขผลกระทบสิ่งแวดล้อม และมาตรการติดตามตรวจสอบผลกระทบสิ่งแวดล้อม

สำหรับโครงการโรงไฟฟ้าชีวมวล (ส่วนขยาย) ระยะดำเนินการ ระหว่างเดือนมกราคม-มิถุนายน พ.ศ. 2567

บริษัท ไทยรุ่งเรือง ไปโอ-เอ็นเนอร์จี้ จำกัด

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Ambient									
7	Standard Gases (Mixture)	Nitrogen Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
8	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i 1201778115	UAE Consultant Co.,Ltd.	09112023	9 Nov 23	8 Nov 24	-
9	Sulphur Dioxide Analyzer	Sulphur Dioxide	Thermo Scientific	43i CM22387061	UAE Consultant Co.,Ltd.	03112023	3 Nov 23	2 Nov 24	-
10	Standard Gases (Mixture)	Sulphur Dioxide	Airgas	EB0143262 2015PSIG	Airgas an Air Liquide company	E04NI99E15A01D3	21 Jun 21	21 Jun 24	-
11	Wind Speed/Wind Direction	WS/WD	Scarlet Tech Ltd.	WL-21 2205DT0113	Thai Meteorological Department	390/23	1 Nov 23	31 Oct 24	-
12	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	01dB	CAL31 84065	Innovative Instrument Co.,Ltd.	23-ACT-115	4 Aug 23	3 Aug 24	-
13	Sound Level Meter	L <sub>Aeq</sub> 24 hrs, L <sub>A90</sub> , L <sub>Amax</sub> , L <sub>Adn</sub> ระดับเสียงรบกวน	Rion, Japan	NL-62 00130355	Sithiporn Associates Co., Ltd.	ACT23199	27 Jun 23	26 Jun 24	-
14	Sound Level Meter	L <sub>Aeq</sub> 24 hrs, L <sub>A90</sub> , L <sub>Amax</sub> , L <sub>Adn</sub> ระดับเสียงรบกวน	Rion, Japan	NL-62 00130359	Innovative Instrument Co.,Ltd.	CP20230290EA	8 Jun 23	6 Jun 24	-



รายงานผลการปฏิบัติตามมาตรฐานการป้องกัน และแก้ไขผลกระทบสิ่งแวดล้อม และมาตรการติดตามตรวจสอบผลกระทบสิ่งแวดล้อม

สำหรับโครงการโรงไฟฟ้าชีวมวล (ส่วนขยาย) ระยะดำเนินการ ระหว่างเดือนมกราคม-มิถุนายน พ.ศ. 2567

บริษัท ไทยรุ่งเรือง ไปโอ-เอ็นเนอร์จี้ จำกัด

รายการเครื่องมือหลักประจำห้องปฏิบัติการวิเคราะห์ สำหรับตรวจวิเคราะห์คุณภาพสิ่งแวดล้อม

No.	Instrument/Equipment	Parameter	Manufacturer	Model/Serial No.	Calibrator	Certification No.	Date of Calibration	Due date of Calibration*	Remark
Workplace									
1	Sound Level Calibrator (Acoustic Calibrator)	Calibrate Sound Level Meter	01dB	CAL31 82795	Innovative Instrument Co.,Ltd.	23-ACT-109	27 Jun 23	26 Jun 24	-
2	Sound Level Meter	L <sub>Aeq</sub> 8 hrs, L <sub>Amax</sub>	Rion, Japan	NL-42 01010780	Sithiporn Associates Co., Ltd.	ACL23119	11 Apr 23	10 Apr 24	-
3	Air Flow Meter	Calibrate personal pump	TSL,Inc	4146 41461813030	Innovative Instrument Co., Ltd.	23-AFM-219 Rev.1	25 Oct 23	24 Oct 24	-
4	Aneroid Barometer	Total Dust Respirable Dust	Barigo, Germany	-	Technology Promotion Association (Thailand-Japan)	23P1858	2 Jun 23	1 Jun 24	-
5	Digital Thermo - Hygrometer	Total Dust Respirable Dust	Digicon	TH-02 395034175	Technology Promotion Association (Thailand-Japan)	23H1101	24 May 23	23 May 24	-
6	Thermal Environment Monitor	Heat Meter	3M	QuesTemp 32 TPQ020025	Innovative Instrument Co.,Ltd.	23-TPM-253	12 May 23	11 May 24	-
7	Thermal Environment Monitor	Heat Meter	3M	QuesTemp 32 TPT060015	Innovative Instrument Co.,Ltd.	24-TPM-046	23 Jan 24	22 Jan 25	-

## Calibration Certificate

**Certificate No.:** 2402420-001-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhnong, Bangkok 10260

Page 1 of 3

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** AB204-S/FACT  
**Serial No.:** B108115858  
**ID No.:** UAE.AIR.016/2555  
**Order No.:** 2402420  
**Operation No.:** 2402420-001  
**Date of Receipt:** 19 April 2024  
**Date of Calibration:** 19 April 2024

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by**   
( Miss Preeyaporn Jaengkarnkit )  
Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

**Date of Issue:** 23 April 2024

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65



## Calibration Report

**Certificate No.:** 2402420-001-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** AB204-S/FACT

**Resolution:** 0.0001 g

**Serial No.:** B108115858

**ID No.:** UAE.AIR.016/2555

**Capacity:** 220 g

**Date of Calibration:** 19 April 2024

Page 2 of 3

**Environment Condition:** Ambient Temperature: 22.1 ± 0.6 °C Relative Humidity: 49 ± 1.9 %

**Place of Calibration:** Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

### Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M2311181S	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M2311182S	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

### Calibration Results:




#### 1. Repeatability of Reading:

Nominal Value ( g )	Standard Deviation of Reading ( g )
100	0.000057
200	0.000079

#### 2. Off-Center Error:

A mass of 100 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
99.9999	99.9997	99.9996	99.9998	100.0000	99.9998	0.0003

*P. Jongsamrit*  
23 April 2024

F-CS-012 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2402420-001-01

**Equipment:**

Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** AB204-S/FACT

**Resolution:** 0.0001 g

**Serial No.:** B108115858

**ID No.:** UAE.AIR.016/2555

**Capacity:** 220 g

**Date of Calibration:** 19 April 2024

Page 3 of 3

**Calibration Results:** (Continued)

**Calibration Range:** 0-200 g

**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.00000	0.0000	0.0000	0.000089	2.00
0.1	0.10000	0.1000	0.0000	0.000089	2.00
1	0.99998	1.0000	0.0000	0.000092	2.00
5	4.99997	5.0000	0.0000	0.000091	2.00
10	10.00002	10.0001	-0.0001	0.00012	2.00
20	20.00003	20.0001	-0.0001	0.00014	2.00
50	49.99998	50.0000	0.0000	0.00012	2.00
70	70.00000	69.9999	0.0001	0.00016	2.00
100	99.99997	100.0000	0.0000	0.00017	2.00
150	149.99994	149.9997	0.0002	0.00022	2.00
200	200.00001	199.9995	0.0005	0.00028	2.00

*P. Jenghauhit*  
23 April 2024

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.

----- End -----

F-CS-012 Revision: 01 Date: 20-04-65



## Calibration Certificate

**Certificate No.:** 2402420-002-01  
**Client name:** UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
**Address:** 3 Soi Udomsuk 41, Sukhumvit Road,  
Bangchack, Prakhonong, Bangkok 10260

Page 1 of 3

**Equipment:** Electronic Balance  
**Manufacturer:** METTLER TOLEDO  
**Model:** XP6  
**Serial No.:** B322373893  
**ID No.:** UAE.AIR.019/2556  
**Order No.:** 2402420  
**Operation No.:** 2402420-002  
**Date of Receipt:** 19 April 2024  
**Date of Calibration:** 19 April 2024

**Calibrated by** Mr.Pheraphat Tuanjit  
Scientist

**Approved by**   
( Miss Preeyaporn Jaengkarnkit )

Vice President, Department of Laboratory Services  
Responsible for the Technical Management Team

**Date of Issue:** 23 April 2024

**The uncertainties are for a confidence probability of approximately 95%**

This Certificate is issued in accordance with the conditions of accreditation granted by the Thai Laboratory Accreditation Scheme which has assessed the measurement capability of the laboratory and its traceability to recognized national standards and to the units of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the National Food Institute.

F-CS-009 Revision: 01 Date: 20-04-65





## Calibration Report

**Certificate No.:** 2402420-002-01

**Equipment:** Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XP6

**Resolution:** 0.000001 g

**Serial No.:** B322373893

**ID No.:** UAE.AIR.019/2556

**Capacity:** 6.1 g

**Date of Calibration:** 19 April 2024

Page 2 of 3

**Environment Condition:** Ambient Temperature: 22.6 ± 1.8 °C Relative Humidity: 48 ± 6.0 %

**Place of Calibration:** Room 206 Balance Room 2, UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.

**Condition of Equipment:** Good Condition

### Condition of This Results of Calibration:

1. Calibration Method: NFI Method W-MA-001 In-House Method based on UKAS Lab 14 : 2019

2. Reference Standards:

Reference Standard	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Standard Weight Class E2	1-500mg	15880	TCS	M2311181S	28 November 2024
Standard Weight Class E2	1-500g	15882	TCS	M2311182S	28 November 2024

Instrument	Model	Serial No.	Calibrated By	Certificate No.	Due Date
Thermo-Hygro Meter	608-H1	NFI.BTH 019/23	Quality Reborn	QR24-0492	4 March 2025

3. This certification is traceable to SI UNIT

4. This certificate was certified only for the instrument we calibrated.

5. This result of calibration was found accurate as shown on date and place of calibration only.

### Calibration Results:




#### 1. Repeatability of Reading:

Nominal Value ( g )	Standard Deviation of Reading ( g )
3	0.00000057
6	0.00000019

#### 2. Off-Center Error:

A mass of 2 g was placed and moved to various position on pan.

The balance reading obtained is given in the table.



1	2	3	4	5	6	(Maximum Difference)
( g )	( g )	( g )	( g )	( g )	( g )	( g )
1.999981	1.999983	1.999980	1.999984	1.999983	1.999981	0.000003

P. Jongsakulit  
23 April 2024

## Calibration Report

**Certificate No.:** 2402420-002-01

**Equipment:** Electronic Balance

**Manufacturer:** METTLER TOLEDO

**Model:** XP6

**Resolution:** 0.000001 g

**Serial No.:** B322373893

**ID No.:** UAE.AIR.019/2556

**Capacity:** 6.1 g

**Date of Calibration:** 19 April 2024

Page 3 of 3

**Calibration Results:** (Continued)

**Calibration Range:** 0-6 g

**Calibration Adjustment:** Internal Calibration

### 3. Departure from Nominal Value:

Nominal Value ( g )	Standard Value ( g )	Average Reading ( g )	Correction ( g )	Uncertainty ( ± g )	Coverage Factor k
Unload	0.0000000	0.000000	0.000000	0.0000032	2.00
0.01	0.0099970	0.009999	-0.000002	0.0000047	2.00
0.05	0.0500010	0.050003	-0.000002	0.0000048	2.00
0.10	0.1000010	0.100001	0.000000	0.0000069	2.00
0.15	0.1500020	0.150002	0.000000	0.0000083	2.00
0.17	0.1700050	0.170006	-0.000001	0.000012	2.00
0.20	0.1999990	0.200002	-0.000003	0.0000083	2.00
1.50	1.4999750	1.499971	0.000004	0.000027	2.00
3.00	2.9999680	2.999959	0.000009	0.000028	2.00
4.50	4.4999810	4.499967	0.000014	0.000022	2.00
6.00	5.9999490	5.999931	0.000018	0.000032	2.00

*S. Jongsakulkit*  
23 April 2024

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k$ , providing a level of confidence of approximately 95 %.


----- End -----

F-CS-012 Revision: 01 Date: 20-04-65




**CERTIFICATE OF CALIBRATION****Certificate No. :** SP24-018

Page 1 of 5

**Customer :** United Analyst and Engineering Consultant Co.,Ltd. (Head Office)**Address :** 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260**Location of calibration :** Laboratory 315**Equipment :** UV-Vis Spectrophotometer**Manufacturer :** Agilent Technologies**Model :** Cary 60**Serial No. :** MY15410009**ID No. :** UAE.WAT.020/2558**Received Date :** 7 May 2024**Calibration Date :** 7 May 2024**Issue Date :** 9 May 2024**Condition Instrument :** Good**Calibrated by :**

( Mr.Tanawut Rittidach )

Technical Manager

**Approved by :**

( Ms. Chonthicha Sangngern )

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.



## REPORT OF CALIBRATION

**Certificate No. :** SP24-018

Page 2 of 5

**Environment Condition :** Ambient Temperature  $25 \pm 5$  °CRelative humidity  $55 \pm 20$  %RH**Calibration method :** In-house method CP-01 Based on ASTM E275-08**Certified Reference Materials :**

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

**Traceability :** This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Sarna Scientific Limited

**Spectral Band Width of UUC :** 1.5 nm.**Scan Speed of UUC :** 60 nm/min**Scan Interval of UUC :** 0.15 nm.**Resolution of UUC :** Photometric 0.0001 Abs.

Wavelength 0.1 nm.

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5747	0.0033	0.0031	2.00
	1.0484	1.0438	0.0046	0.0029	2.00
	2.1876	2.1832	0.0044	0.0080	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0231	0.0008	0.0035	2.00
	2.1230	2.1219	0.0011	0.0080	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5184	0.0046	0.0030	2.00
	0.9633	0.9614	0.0019	0.0029	2.00
	1.9753	1.9731	0.0022	0.0070	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5150	0.0031	0.0031	2.00
	1.0002	0.9964	0.0038	0.0033	2.00
	1.9973	1.9914	0.0059	0.0088	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5485	0.0032	0.0030	2.00
	1.0803	1.0772	0.0031	0.0030	2.00
	2.0373	2.0293	0.0080	0.0080	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5565	0.0026	0.0031	2.00
	1.0518	1.0482	0.0036	0.0030	2.00
	1.9274	1.9202	0.0072	0.0079	2.00

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 4 of 5

### Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7435	0.0034	0.0057	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8639	0.0035	0.0060	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2907	0.0012	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6402	0.0028	0.0055	2.00

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 5 of 5

### Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.9	-0.09	0.18	2.00
334.06	333.9	0.16	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.1	0.49	0.18	2.00
445.94	445.6	0.34	0.18	2.00
453.66	453.3	0.36	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.0	0.59	0.18	2.00
637.98	638.7	-0.72	0.18	2.00
431.38	430.8	0.58	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.7	-0.23	0.18	2.00
528.88	529.1	-0.22	0.18	2.00
573.17	573.5	-0.33	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.4	-0.68	0.20	2.00
748.55	749.1	-0.55	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.3	-0.02	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement *U* is stated as the standard uncertainty of measurement multiplied by the coverage factor *k*,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- \* Indicates non TISI accredited

- End of Certificate -





# Certificate of Calibration

**Equipment:** pH METER Certificate No.: C07240167  
**Model:** SevenEasy Issued Date: 9 April 2024  
**Serial No. (or ID.):** 1230525212 (UAE.WAS.003/2553) Job No.: WO-00024208  
**Manufacturer:** METTLER TOLEDO Page: 1 of 3  
**Electrode Serial No.:** 1156883 Model: InLab Solids Brand: METTLER TOLEDO  
**Condition:** In Condition

**Customer:** United Analyst and Engineering Consultant Company Limited  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangkok, Prakanong, Bangkok 10260 Thailand

**Environment Condition:** Temperature 23 °C ± 2 °C  
Humidity 50 %RH ± 15 %RH

**Calibration Place:** Environment Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangkok,  
Phrakhanong, Bangkok 10260 Thailand

**Calibration By:** Miss.Orawan Khlaiphloi

**Calibration Date:** 9 April 2024

**The Method used:** In house method, CAL-WI-58, base on ASTM E 70-07

**Traceability:** This certificate is traceable to SI Units, Sample Test is assured through primary measurement method Harned cell, through CPAchem Ltd. (ISO/IEC 17034) Certificate No. 938377, 931985, 931984 And pH Scale traceable to the SI Units maintained by National Institute of Metrology (NIMT), Thailand through Industrial Foundation Electrical and Electronics Institute Certificate No. CA20230350EA

(Miss Orawan Khlaiphloi)

Person in charge

(Mr. Nitinun Srihawan)

Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor ( $k=2$ ) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.

## Calibration Results:

### pH Scale

Input	pH Meter Reading			Uncertainty of Measurement (mV)	Coverage Factor (k)
	(mV)	Error (mV)	(pH)		
414.12	414	-0.12	0.00	0.58	2.00
354.96	355	0.04	1.00	0.58	2.00
295.8	296	0.20	2.00	0.58	2.00
236.64	237	0.36	3.00	0.58	2.00
177.48	178	0.52	4.00	0.58	2.00
118.32	118	-0.32	5.00	0.58	2.00
59.16	59	-0.16	6.00	0.58	2.00
0	0	0.00	7.00	0.58	2.00
-59.16	-59	0.16	8.00	0.58	2.00
-118.32	-118	0.32	9.00	0.58	2.00
-177.48	-177	0.48	10.00	0.58	2.00
-236.64	-236	0.64	11.00	0.58	2.00
-295.8	-296	-0.20	12.00	0.58	2.00
-354.96	-355	-0.04	13.00	0.58	2.00
-414.12	-414	0.12	14.00	0.58	2.00

**Practical slope and zero point\***

The three-point calibration using three standard buffer solutions; pH 4.008 , pH 6.985 and pH 9.997

-During calibration, display of pH meter reading; pH 4.00 , pH 7.00 and pH 10.01

The practical slope of the pH electrode; 57.01 (mV/pH), 96.37%


The zero point of the pH electrode; 6.88 (pH)

**Sample Test Results**

Standard Buffer Solution (pH)	Unit Under Calibration (pH)	Difference (pH)	Uncertainty of Measurement (pH)	Coverage Factor (k)
4.008	3.99	-0.018	0.0070	2.00
6.985	7.00	0.015	0.0091	2.00
9.997	10.02	0.023	0.0074	2.00

\* Calibration Marked " Not TISI Accredited " in this Certificate have been included for completeness.

**The End of Certificate**

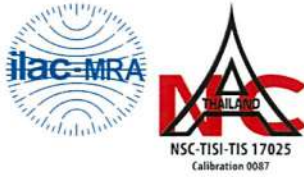

# Certificate of Calibration

<b>Equipment:</b>	Digital Thermometer with Probe	<b>Certificate No.:</b>	C15240373
<b>Model:</b>	SevenEasy pH	<b>Issued Date:</b>	09 April 2024
<b>Serial No.:</b>	1230525212	<b>Job No.:</b>	WO-00024208
<b>Manufacturer:</b>	METTLER TOLEDO	<b>Page:</b>	1 of 2
<b>ID No.:</b>	UAE.WAS.003/2553	<b>Condition:</b>	In Condition

**Customer:** United Analyst and Engineering Consultant Company Limited  
3 Soi Udomsuk 41 Sukhumvit Road,  
Bangchak, Prakanong, Bangkok 10260 Thailand

**Environment Condition:** Temperature: 22 °C ± 3 °C  
Humidity: 50 %RH ± 20 %RH  
Voltage: 220 VAC ± 10 %

**Calibration Place:** Thermo-Hygro Laboratory, DKSH Technology Limited.  
2533 Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260 Thailand

**Calibration By:** Mr. Nateekarn Mitjit  
**Calibration Date:** 09 April 2024  
**The Method used:** In house method, CAL-WI-19, by comparison with standard thermometer  
**Traceability:** This certificate is traceable to the International System of Unit maintained by Quality Reborn Co.,Ltd. (QR) Certificate No. QR23-1073



(Mr. Nateekarn Mitjit)  
Person in charge



(Mr. Pramote Ramrong)  
Authorized signatory

This certificate is issued the units of measurement according to the International System of Units (SI). It provides traceability of measurement to international or national standard or other recognized national standard laboratories.

The measurement uncertainty stated is the expanded uncertainty which is obtained from the standard uncertainty multiplied by the coverage factor (k=2) to provide a level of confidence of approximately 95%. It is determined in accordance with the Guide to Expression of Uncertainty in Measurement (GUM).

These results may be affected by deviations from specified conditions. The results relate only to the items tested, calibrated or sampled. The report shall not be reproduced except in full without approval of DKSH Technology Limited.



**Reference standard equipment:**

Equipment	Certificate no	Cal. date	Next Cal. date
Digital Thermometer with Probe	QR23-1073	2 May 23	2 May 24

**Calibration Results:****Without Adjustment**

Sensor Type: RTD

Channel: -


Diameter (mm) 4

Length (mm): 135

Immersion (mm): 110


Calibrate Point.(°C)	STD. Reading (°C)	UUC. Reading (°C)	Correction of UUC (°C)	Uncertainty ( $\pm$ °C)
15.0	15.010	15.1	-0.090	0.076
25.0	25.006	25.1	-0.094	0.076
35.0	35.004	35.0	0.004	0.076

**The End of Certificate**

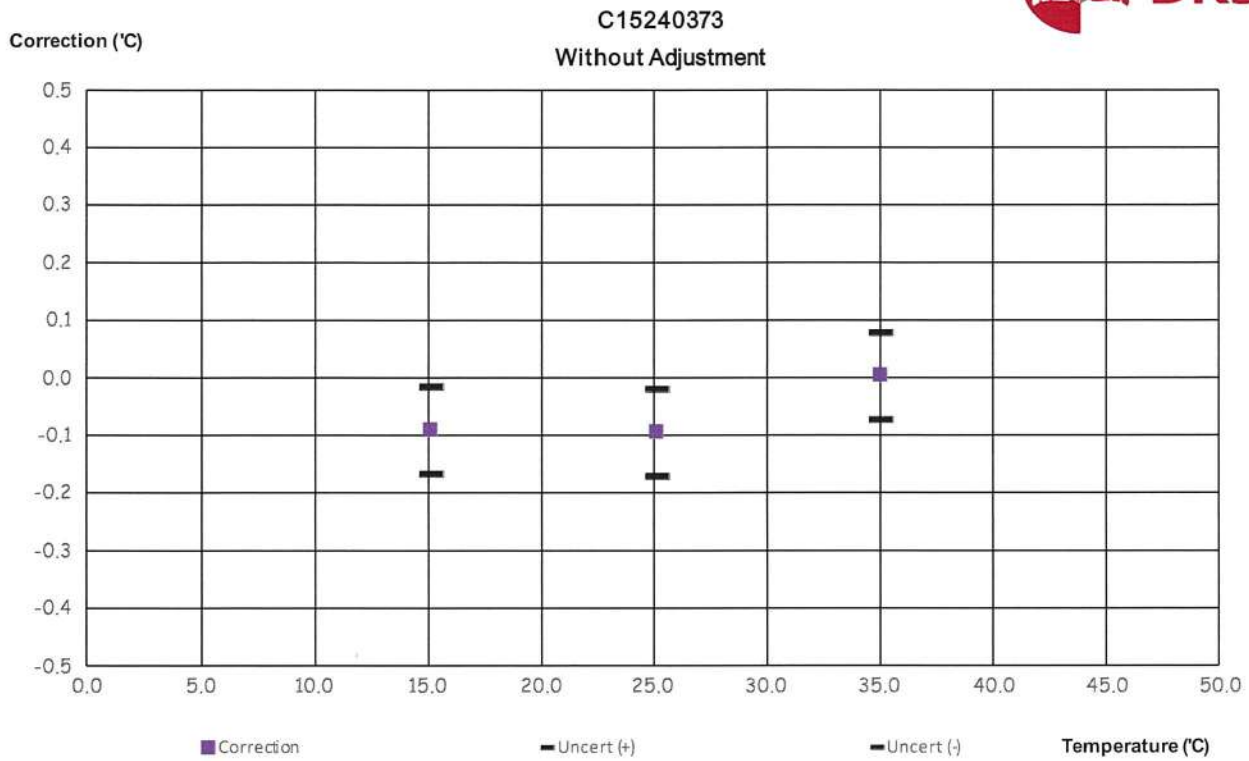


**CERTIFICATE OF CALIBRATION****Certificate No. :** SP24-018

Page 1 of 5

**Customer :** United Analyst and Engineering Consultant Co.,Ltd. (Head Office)**Address :** 3 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260**Location of calibration :** Laboratory 315**Equipment :** UV-Vis Spectrophotometer**Manufacturer :** Agilent Technologies**Model :** Cary 60**Serial No. :** MY15410009**ID No. :** UAE.WAT.020/2558**Received Date :** 7 May 2024**Calibration Date :** 7 May 2024**Issue Date :** 9 May 2024**Condition Instrument :** Good**Calibrated by :**

( Mr.Tanawut Rittidach )

Technical Manager

**Approved by :**

( Ms. Chonthicha Sangngern )

Quality Manager

The calibration result is applied only to the above calibrated item and was found accurate as shown on date and place of calibration only.

The measurement capability of the laboratory and its traceability to recognized national standards and to the unit of measurement realized at the corresponding national standards laboratory. This certificate may not be reproduced other than in full except with the prior written approval of the DQE Services Co., Ltd.

## REPORT OF CALIBRATION

**Certificate No. :** SP24-018

Page 2 of 5

**Environment Condition :** Ambient Temperature  $25 \pm 5$  °CRelative humidity  $55 \pm 20$  %RH**Calibration method :** In-house method CP-01 Based on ASTM E275-08**Certified Reference Materials :**

Material	Serial No.	Certificate No.	Due date
Absorbance Standard set	25760	115663	25 October 2025
Absorbance Standard set	25757	115638	25 October 2025
Wavelength Standard set	25806	115657	25 October 2025
Wavelength Standard set	25758	115665	25 October 2025

**Traceability :** This certification is traceable to the International System of Unit maintained at National -

Institute of Standards and Technology (NIST) through Sarna Scientific Limited

**Spectral Band Width of UUC :** 1.5 nm.**Scan Speed of UUC :** 60 nm/min**Scan Interval of UUC :** 0.15 nm.**Resolution of UUC :** Photometric 0.0001 Abs.

Wavelength 0.1 nm.

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 3 of 5

Calibration Results : Without adjustment

Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
420	0.0000	0.0000	0.0000	0.0028	2.00
	0.5780	0.5747	0.0033	0.0031	2.00
	1.0484	1.0438	0.0046	0.0029	2.00
	2.1876	2.1832	0.0044	0.0080	2.00
440	0.0000	0.0000	0.0000	0.0028	2.00
	0.5595	0.5581	0.0014	0.0034	2.00
	1.0239	1.0231	0.0008	0.0035	2.00
	2.1230	2.1219	0.0011	0.0080	2.00
465	0.0000	0.0000	0.0000	0.0028	2.00
	0.5230	0.5184	0.0046	0.0030	2.00
	0.9633	0.9614	0.0019	0.0029	2.00
	1.9753	1.9731	0.0022	0.0070	2.00
546.1	0.0000	0.0000	0.0000	0.0028	2.00
	0.5181	0.5150	0.0031	0.0031	2.00
	1.0002	0.9964	0.0038	0.0033	2.00
	1.9973	1.9914	0.0059	0.0088	2.00
590	0.0000	0.0000	0.0000	0.0028	2.00
	0.5517	0.5485	0.0032	0.0030	2.00
	1.0803	1.0772	0.0031	0.0030	2.00
	2.0373	2.0293	0.0080	0.0080	2.00
635	0.0000	0.0000	0.0000	0.0028	2.00
	0.5591	0.5565	0.0026	0.0031	2.00
	1.0518	1.0482	0.0036	0.0030	2.00
	1.9274	1.9202	0.0072	0.0079	2.00



## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 4 of 5

### Photometric Accuracy :

Wavelength (nm.)	CRMs Values (Abs)	UUC Reading (Abs)	Correction (Abs)	Uncertainty (Abs)	Coverage factor <i>k</i>
235	0.0000	0.0000	0.0000	0.0050	2.00
	0.7469	0.7435	0.0034	0.0057	2.00
257	0.0000	0.0000	0.0000	0.0050	2.00
	0.8674	0.8639	0.0035	0.0060	2.00
313	0.0000	0.0000	0.0000	0.0050	2.00
	0.2919	0.2907	0.0012	0.0051	2.00
350	0.0000	0.0000	0.0000	0.0050	2.00
	0.6430	0.6402	0.0028	0.0055	2.00

## REPORT OF CALIBRATION

Certificate No. : SP24-018

Page 5 of 5

### Wavelength Accuracy :

CRMs Values (nm.)	UUC Reading (nm.)	Correction (nm.)	Uncertainty (nm.)	Coverage factor <i>k</i>
241.72	242.0	-0.28	0.18	2.00
279.45	279.5	-0.05	0.18	2.00
287.81	287.9	-0.09	0.18	2.00
334.06	333.9	0.16	0.18	2.00
360.93	360.5	0.43	0.18	2.00
418.59	418.1	0.49	0.18	2.00
445.94	445.6	0.34	0.18	2.00
453.66	453.3	0.36	0.18	2.00
460.02	459.8	0.22	0.18	2.00
536.59	536.0	0.59	0.18	2.00
637.98	638.7	-0.72	0.18	2.00
431.38	430.8	0.58	0.18	2.00
472.50	472.4	0.10	0.18	2.00
513.47	513.7	-0.23	0.18	2.00
528.88	529.1	-0.22	0.18	2.00
573.17	573.5	-0.33	0.18	2.00
585.35	585.2	0.15	0.20	2.00
684.40	685.1	-0.70	0.18	2.00
740.72	741.4	-0.68	0.20	2.00
748.55	749.1	-0.55	0.18	2.00
807.03	807.3	-0.27	0.18	2.00
879.28	879.3	-0.02	0.18	2.00

Remark : - UUC = Unit Under Calibration

- N/A = Not Available

- The result expanded uncertainty of measurement  $U$  is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k$ ,

which for a normal distribution corresponds to a coverage probability of approximately 95%

- \* Indicates non TISI accredited

- End of Certificate -

**Envi Equipment Service Co., Ltd.**

110/254 Moo 3, Tumbon Bang Rak Phatthana, Amphur Bang Bua Thong, Nonthaburi 11110

Tel. 098 362 9152, 089 478 7885

E-mail: sales@envi-ees.com

Certificate No. : E23-08066

Page : 1 of 6

**CERTIFICATE OF CALIBRATION**

**Customer** : United Analyst and Engineering Consultant Co., Ltd.

**Address** : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong, Bangkok 10260

**Description of Equipment** : Console meter

**Manufacturer** : Apex Instrument

**Model Number** : XC-572-V

**Serial Number** : 1904011

**ID./Control No.** : -

**Environment Conditions** : Temperature (25 ± 2) °C  
Humidity (50 ± 15) % RH

**Cal. Date** : 05/08/2023

**Issue Date** : 05/08/2023

**Calibration Method or Calibration Procedure Used**

US EPA Method (United State Environmental Protection Agency)


This certificate is traceable to national standard, which realize the units of measurement according to the International System of Units (IS).

**Result of Calibration**

This certificate may not be reproduced other than in full except with prior Written approval of the Technical Manager, Envi Equipment Service Company Limited.

These reported uncertainties of measurement are expanded by a coverage factor of k=2, providing a 95% confidence level

Calibrated by : Mr. Sanya Sangnil

Approved by :   
(Mr. Mana Fuekhud)  
Technical Manger



**เอกสารไม่ควบคุม**



**METHOD 5 CONSOLE CALIBRATION  
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425  
5-POINT METRIC UNIT**

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	05/08/2023	09:50 AM	Std Temp	293	K
Console Serial Number	1904011	Calibration Reference No.		SER23-08027		Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure		758.99	mmHg	K <sub>1</sub>	0.386	
DGM Serial Number	00004114	Calibration Meter Gamma		0.999		Console Leak Check		PASS

Calibration Data									
Run Time	Metering Console					Calibration Meter			
Elapsed	DGM Orifice DH	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final	Volume Initial	Volume Final	Outlet Temp Initial	Outlet Temp Final
(Q)	(P <sub>m</sub> )	(V <sub>mi</sub> )	(V <sub>mf</sub> )	(t <sub>mi</sub> )	(t <sub>mf</sub> )	(V <sub>wi</sub> )	(V <sub>wf</sub> )	(t <sub>wi</sub> )	(t <sub>wf</sub> )
min	mm H <sub>2</sub> O	m <sup>3</sup>	m <sup>3</sup>	°C	°C	m <sup>3</sup>	m <sup>3</sup>	°C	°C
12.35	13.0	1342.996	1343.136	29	29	155.32046	155.46168	27	27
12.42	13.0	1343.136	1343.276	29	29	155.46168	155.60264	27	27
8.80	26.0	1343.282	1343.422	29	29	155.60872	155.75014	27	27
8.80	26.0	1343.422	1343.562	30	30	155.75014	155.89098	26	26
13.95	40.0	1343.569	1343.849	30	30	155.89796	156.17902	26	26
13.95	40.0	1343.849	1344.129	31	31	156.17902	156.45838	26	26
10.50	70.0	1344.138	1344.418	31	31	156.46734	156.74556	26	26
10.47	70.0	1344.418	1344.698	32	32	156.74556	157.02264	26	26
9.12	90.0	1344.711	1344.991	32	32	157.03528	157.31088	26	26
9.12	90.0	1344.991	1345.271	32	32	157.31088	157.58638	25	25



**METHOD 5 CONSOLE CALIBRATION  
USING REFERENCE WET GAS METER W-NK-2.5-B-Z No.547425  
5-POINT METRIC UNIT**

Meter Console Information		Calibration Conditions				Factors/Conversions		
Console Model Number	XC-572-V	Date	Time	05/08/2023	09:50 AM	Std Temp	293	K
Console Serial Number	1904011	Calibration Reference No.		SER23-08027		Std Press	760	mm Hg
DGM Model Number	SK25EX	Barometric Pressure		758.99	mmHg	K <sub>1</sub>	0.386	
DGM Serial Number	00004114	Calibration Meter Gamma		0.999		Console Leak Check		PASS

Calibration Data								
Results								
Standardized Data				Dry Gas Meter				
Dry Gas Meter		Calibration Meter		Calibration Factor		Flowrate		
(V <sub>m(std)</sub> )	(Q <sub>m(std)</sub> )	(V <sub>w(std)</sub> )	(Q <sub>w(std)</sub> )	Value	Variation	Std & Corr	.0212 m <sup>3</sup> <sub>std</sub> /min	Variation
m <sup>3</sup>	m <sup>3</sup> /min	m <sup>3</sup>	m <sup>3</sup> /min	(Y)	(ΔY)	(Q <sub>m(std)(corr)</sub> )	(ΔH <sub>@</sub> )	(ΔH <sub>@</sub> )
						m <sup>3</sup> /min	mm H <sub>2</sub> O	
0.137	0.011	0.138	0.011	1.006	0.014	0.011	46.171	-0.333
0.137	0.011	0.137	0.011	1.005	0.012	0.011	46.843	0.339
0.137	0.016	0.138	0.016	1.007	0.014	0.016	46.870	0.366
0.137	0.016	0.138	0.016	1.002	0.010	0.016	47.099	0.595
0.275	0.020	0.275	0.020	0.999	0.006	0.020	45.847	-0.657
0.275	0.020	0.273	0.020	0.993	0.000	0.020	46.407	-0.097
0.276	0.026	0.272	0.026	0.986	-0.007	0.026	46.656	0.152
0.276	0.026	0.271	0.026	0.982	-0.011	0.026	46.743	0.239
0.276	0.030	0.269	0.030	0.975	-0.018	0.030	46.263	-0.241
0.277	0.030	0.270	0.030	0.974	-0.018	0.030	46.142	-0.362
				0.993	Y Average		46.504	ΔH <sub>@</sub> Average

**Note:** For Calibration Factor Y, the ratio of the reading of the calibration meter to the dry gas meter, acceptable tolerance of individual values from the average is  $\pm 0.02$ .  
For  $\Delta H_{@}$ , orifice pressure differential that equates to 0.75 cfm (0.0212 m<sup>3</sup>/min) at standard temperature and pressure, acceptable tolerance of individual values from the average is  $\pm 0.2$  inches (5.1mm) H<sub>2</sub>O.



**เอกสารไม่ควบคุม**



Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	1904011
DGM Model Number	SK25EX
DGM Serial Number	00004114


Calibration Conditions			
Date	Time	05/08/2023	09:50 AM
Calibration Reference No.	SER23-08027		
Barometric Pressure	758.99	mm Hg	
Calibration Meter Gamma	0.999		

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K <sub>1</sub>	0.386	
Console Leak Check	PASS	

Calibration Date: 5-8-2023

Calibration Reference No: SER23-08027

Meter Gamma vs Flowrate

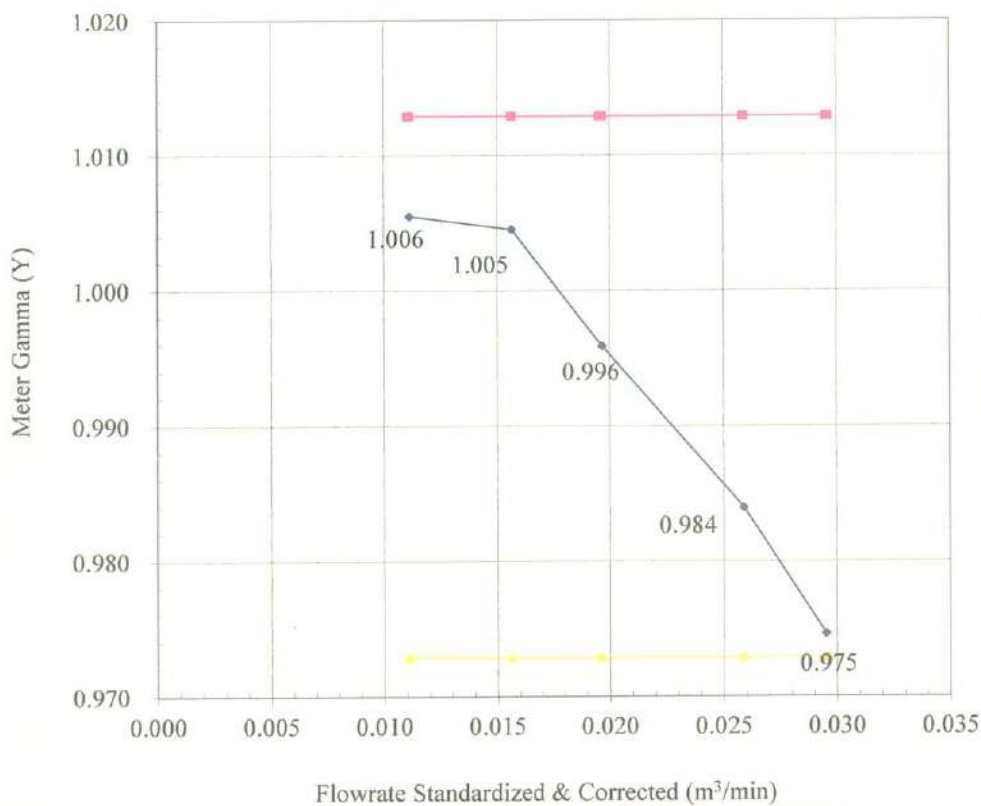

Console Serial: 1904011

Console Model: XC-572-V



เอกสารไม่ควบคุม

Meter Console Information	
Console Model Number	XC-572-V
Console Serial Number	1904011
DGM Model Number	SK25EX
DGM Serial Number	00004114


Calibration Conditions			
Date	Time	05/08/2023	09:50 AM
Calibration Reference No.		SER23-08027	
Barometric Pressure		758.99	mmHg
Calibration Meter Gamma		0.999	

Factors/Conversions		
Std Temp	293	K
Std Press	760	mm Hg
K <sub>1</sub>	0.386	
Console Leak Check		PASS

Calibration Date: 5-8-2023

Calibration Reference No: SER23-08027

Meter Pressure vs Flowrate

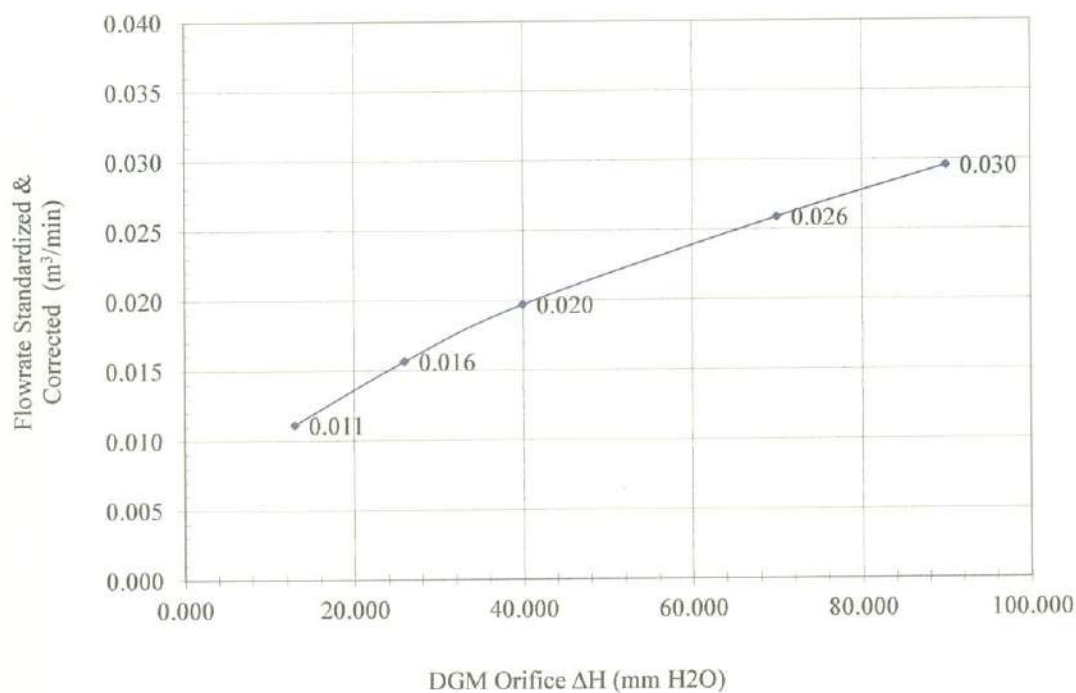

Console Serial: 1904011

Console Model: XC-572-V



เอกสารไม่ควบคุม

## THERMOCOUPLES SYSTEM CALIBRATION

Sampling System Equipment Information	
Console Model Number	XC-572-V
Console Serial Number	1904011
DGM Model Number	SK25EX
DGM Serial Number	00004114
Meter Box Model Number	JENCO 765 KF
Meter Box Serial Number	JC 17215

Calibration Conditions			
Date	Time	05/08/2023	12:10 PM
Calibration Reference No.	SER23-08027		
Reference Thermometer	DIGICON		
Serial Number	183169105		

Results											
Console Thermocouple Simulator											
Channel and test point	Meter Box Channel Temperature Reading ( °C )										
	-18.0	25.0	38.0	93.0	149.0	260.0	371.0	482.0	593.0	816.0	1038.0
Stack	-17.0	25.0	37.0	93.0	149.0	258.0	370.0	481.0	592.0	814.0	1037.0
Aux	-16.0	25.0	37.0	93.0	149.0						
Probe	-17.0	24.0	37.0	93.0	149.0						
Filter	-16.0	24.0	37.0	93.0	149.0						
Oven	-16.0	24.0	37.0	93.0	149.0						
Exit	-16.0	24.0	37.0								

### Tolerance Range

Stack      ± 1.50%      Absolute  
 Probe      ± 3.0 °C  
 Filter      ± 3.0 °C

Meter      ± 3.0 °C  
 Exit      ± 2.0 °C

# EES

Envl Equipment Service Co., Ltd.



เอกสารไม่ควบคุม



**Certificate No:** G 660354

**Date of issue :** 20-Jun-23

**Instrument description :** Flue gas Analyzer  
**Instrument model :** Testo 350 New  
**Instrument serial no. :** 60899615  
**ID no. or control no. :** UAE.EFM. 006/2560  
**Manufacturer :** Testo SE & Co. KGaA  
**Probe description :** -  
**Probe model :** -  
**Probe serial :** -  
**Customer name :** United Analyst and Engineering Consultant Co., Ltd.  
**Customer address :** 81 Soi Udomsuk 41, Sukhumvit Rd., Bangchak, Phrakhanong, Bangkok 10260

**Total pages of certificate :** 3 Pages  
**Receiving no. :** L-231754  
**Receiving date. :** 20-Jun-23  
**Parameter of calibration :** Gas Calibration(Oxygen 2.498,10.04,21.02 %vol, Carbon Monoxide 80.14,309.9,1003 ppm, Nitrogen Dioxide 30.34,80.96,202.2 ppm, Nitric Oxide 30.01,151.5,320.6 ppm, Sulphur Dioxide 50.04,100.8,601.1 ppm)  
**Condition of UUC. :** Used  
**Ambient condition :** All of the Measurement were carried out the stabilized laboratory  
Temperature : 23 ± 5 °C  
Humidity : 55 ± 15 %RH  
**Calibration place :** 17/121 Soi Ngamwongwan 47 Yaek 48, Toongsonghong, Laksi, Bangkok 10210  
**Calibration procedure no. :** This instrument was calibrated by comparison with Standard gas mixture according to calibration work instruction no. WI-CL-28-C

*The calibration certificate expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.*

*This certificate is applied only to item under test Environmental condition.*

*This Calibration Certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without signature and seal not valid and The results relate only to the items tested/calibrated.*

*This calibration certificate documents are traceability to national standards, which realize measurement according to the International System of Units (SI).*

**Date of calibration :** 20-Jun-23



Mr. Kwanchai Khamdoun  
Calibration Technician



Mrs. Nongluck Wongsettee  
Technical Manager

### Standard References (Table 1)

Standard	Certificate No.	Vendor	Due date
Oxygen ( O <sub>2</sub> ) 2.498 % Vol	4219/21	Linde	30-Sep-25
Oxygen ( O <sub>2</sub> ) 10.04 % Vol	CG-0153-21	Nimt	18-Nov-26
Oxygen ( O <sub>2</sub> ) 21.02 % Vol	CG-0041-22	Nimt	10-Feb-27
Carbon monoxide ( CO ) 80.14 ppm	CG-0040-22	Nimt	14-Feb-27
Carbon monoxide ( CO ) 309.9 ppm	2803/21	Linde	22-Jun-23
Carbon monoxide ( CO ) 1003 ppm	45513	Linde	09-Aug-24
Nitrogen Dioxide ( NO <sub>2</sub> ) 30.34 ppm	2703/22	Nimt	22-Aug-24
Nitrogen Dioxide ( NO <sub>2</sub> ) 80.96 ppm	3240/21	Linde	26-Jun-24
Nitrogen Dioxide ( NO <sub>2</sub> ) 202.2 ppm	3239/21	Linde	20-Jul-23
Nitric Oxide ( NO ) 30.01 ppm	CG-0014-23	Nimt	19-Feb-25
Nitric Oxide ( NO ) 151.5 ppm	0161/23	Linde	22-Jan-25
Nitric Oxide ( NO ) 320.6 ppm	2944/21	Linde	02-Jul-23
Sulphur Dioxide ( SO <sub>2</sub> ) 50.04 ppm	3205/21	Linde	25-Jul-23
Sulphur Dioxide ( SO <sub>2</sub> ) 100.8 ppm	3507/22	Linde	09-Nov-24
Sulphur Dioxide ( SO <sub>2</sub> ) 601.1 ppm	3204/21	Linde	20-Jul-23

### Measured room conditions

Temperature : 22.7 °C Humidity : 67.8 %RH Pressure : 1005.1 mbar

### Calibration conditions

Gas Temperature : 23 °C Flow rate : 1,200 ml/min Gas pressure : 1020.2 mbar

### Calibration Results (before adjustment) (Table 2)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O <sub>2</sub> (%Vol)	2.498	2.56	0.062	0.15
O <sub>2</sub> (%Vol)	10.04	10.11	0.07	0.20
O <sub>2</sub> (%Vol)	21.02	21.10	0.08	0.30
CO (ppm)	80.14	78	-2.14	3.0
CO (ppm)	309.9	297	-12.9	6.0
CO (ppm)	1003	965	-38	12
NO <sub>2</sub> (ppm)	30.34	27.9	-2.44	8.0
NO <sub>2</sub> (ppm)	80.96	81.3	0.34	8.0
NO <sub>2</sub> (ppm)	202.2	205.3	3.1	12
NO (ppm)	30.01	27	-3.01	8.0
NO (ppm)	151.5	143	-8.5	8.0
NO (ppm)	320.6	294	-26.6	12
SO <sub>2</sub> (ppm)	50.04	53	2.96	6.0
SO <sub>2</sub> (ppm)	100.8	111	10.2	6.0
SO <sub>2</sub> (ppm)	601.1	665	63.9	13

Calibration Results (after adjustment) (Table 3)

Parameter of Standard	Standard Values	Mean of UUC	Error	Uncertainty (±)
O2 (%Vol)	2.498	2.56	0.062	0.15
O2 (%Vol)	10.04	10.11	0.07	0.20
O2 (%Vol)	21.02	21.10	0.08	0.30
CO (ppm)	80.14	81	0.86	3.0
CO (ppm)	309.9	309	-0.9	6.0
CO (ppm)	1003	1001	-2	12
NO2 (ppm)	30.34	27.9	-2.44	8.0
NO2 (ppm)	80.96	81.3	0.34	8.0
NO2 (ppm)	202.2	205.3	3.1	12
NO (ppm)	30.01	32	1.99	8.0
NO (ppm)	151.5	155	3.5	8.0
NO (ppm)	320.6	318	-2.6	12
SO2 (ppm)	50.04	50	-0.04	6.0
SO2 (ppm)	100.8	100	-0.8	6.0
SO2 (ppm)	601.1	598	-3.1	13

Remark : 1 cmol/mol = 1 %vol. , 1 µmol/mol = 1 ppm.

## End of Report





JIRANATEE ASSOCIATES CO.,LTD.

Jiranatee Associates Co.,Ltd.  
63/14-15, 67/35-36  
Petchkasem 7,7/1, Rd.Watthapra, Bangkokyai,  
Bangkok 10600 (Thailand)  
Tel: +6608680812  
Mobile: +66863999453  
E-mail: jnac-calibration@jiranatee.com  
Web site: www.jiranatee.com

Accredited calibration laboratory  
ISO/IEC 17025:2017  
NSC-TISI-TIS 17025  
CALIBRATION 0367

Flow measurement laboratory  
Calibration services department.



## CERTIFICATE OF CALIBRATION

Certificate No. : COF-002-66

Page 1 of 2 Pages

**MEASUREMENT ITEM** : Top Load Orifice  
**MANUFACTURER** : Andersen Instruments  
**MODEL/TYPE** : G25A  
**SERIAL NUMBER** : 1901  
**ID NUMBER** : UAE.ANV.051/2547  
**CONDITION AS-RECEIVED** : Used item  
**CUSTOMER** : United Analyst and Engineering Consultant Co., Ltd.  
81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Phrakhanong,  
Bangkok 10260

**RECEIVED DATE** : 07 Jul 2023  
**MEASUREMENT DATE** : 14 Jul 2023  
**ISSUE DATE** : 18 Jul 2023

### ENVIRONMENTAL CONDITIONS:

Ambient condition in the laboratory are as follow:

Temperature	: 23.0 ± 3.0	°C
Relative Humidity	: 55.0 ± 15.0	%RH
Atmospheric Pressure	: 1010 ± 10	hPa

### CALIBRATION CONDITION:

Preconditioning : 24 hours at ambient conditions.  
Measurement Condition : The average values during measurement are 23.9 °C and 54.5%RH.

**NOTED:** The certificate is valid only to the item calibrated on date and place of calibration.

### TABULATION OF RESULTS:

The table on next page give the measured values.

### Calibration procedure:

The Orifice gas flow device was calibrated against Standard Rotary Displacement Meter (Roots Meter) Model G65/IMC/W2-dp. The WI-CL-004 was used as a calibration guideline.

### Traceability:

This certificate provides a traceability of The measurement to recognized the national standards, and to realization of the international system of units (SI) through the VSL (National Metrology Institute of Netherlands) via Certificate number: G2211901

### Uncertainty of Measurement:

The reported uncertainty of measurement is based on the standard uncertainty multiplied by a coverage factor  $k=2$ , Which for a normal distribution corresponds to a coverage probability of approximately 95%. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the expression of uncertainty in measurement'

Calibrated by:

- ☐ Mr. Sorawit Thachalad  
☒ Miss Jittraporn Lertsomphol



Approved signatory:

Mr. Parinya Booncharoen  
Calibration Department Manager

เอกสารไม่ควบคุม

**MEASUREMENT RESULTS:**

The Orifice gas flow device was calibrated by direct comparison method with the Standard Rotary Displacement Meter (Roots Meter). The Humid air was used as a medium in the system. The standard conditions are 25°C (298.15 K) and 760 mmHg for standard temperature and standard pressure respectively.

**Table 1:** The results of  $Q$  Standard calibration data

Plate	Flow rate $m^3/min$	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p_{meter}$ mmHg	$\Delta p_{Orifice}$ inH <sub>2</sub> O	$Y$	Standard Flow [ $Q_s$ ] $m^3/min$
1	0.701	754.115	23.87	23.10	55.600	1.626	1.273	0.648
2	0.997	754.083	23.80	23.23	61.350	3.236	1.795	0.914
3	1.121	754.005	23.81	23.20	41.923	4.338	2.079	1.057
4	1.172	754.004	23.72	23.16	30.933	4.891	2.208	1.122
5	1.410	753.994	23.76	23.18	29.415	7.159	2.671	1.352

Slope ( $m$ ): 1.98463  
 Intercept ( $b$ ): -0.01636  
 Correlation coefficient ( $r$ ): 0.99972  
 Uncertainty ( $k=2$ ): 0.015  $m^3/min$

**Table 2:** The results of  $Q$  actual calibration data

Plate	Flow rate $m^3/min$	Pressure [Pa] mmHg	Temperature [Ta] °C	Temperature [Tm] °C	$\Delta p_{meter}$ mmHg	$\Delta p_{Orifice}$ inH <sub>2</sub> O	$Y$	Standard Flow [ $Q_a$ ] $m^3/min$
1	0.701	754.115	23.87	23.10	55.600	1.626	0.800	0.651
2	0.997	754.083	23.80	23.23	61.350	3.236	1.129	0.917
3	1.121	754.005	23.81	23.20	41.923	4.338	1.307	1.061
4	1.172	754.004	23.72	23.16	30.933	4.891	1.388	1.126
5	1.410	753.994	23.76	23.18	29.415	7.159	1.679	1.357

Slope ( $m$ ): 1.24306  
 Intercept ( $b$ ): -0.01029  
 Correlation coefficient ( $r$ ): 0.99972  
 Uncertainty ( $k=2$ ): 0.015  $m^3/min$

\*\*\*End of Certificate of Calibration\*\*\*



เอกสารไม่ควบคุม





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484

## Certificate of Calibration

Certificate No. : 23P1401  
Page : 1 of 2

Equipment : U-Tube Manometer  
Manufacturer: Dwyer  
Model : 1221-36-W/M  
Serial No.: -  
ID No.: UAE.EFM.022/2560

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item

Received Date: 26 April 2023

Calibration Date: 09 May 2023

Reference: 2304-0703WSC

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

Ambient Temperature: ( 23 ± 2 ) °C

Relative Humidity: ( 50 ± 15 ) %

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

Atmospheric Pressure: 1010 mbar

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P04, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Pressure Calibrator	PC106P	1189	MP-0137-22	24 Aug 2023

2.This result of calibration was made on requested at the point specified by customer.

3.Scale and conversion factor is 1 kPa = 4.0146293 inH<sub>2</sub>O

4.This instrument was used clean air and oil as pressure media.

5.This instrument was calibrated by applied pressure to high-port (+) side and low-port (-) side open to atmospheric pressure.

6.This instrument was installed in vertical orientation and top of the pressure port was used as the reference level.

7.The certificate is valid only to the item calibrated on date and place of calibration.

8.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suwit Aussarree  
Issue Date : 11 May 2023

Approved Signatory : Attapol P.  
[ ] Phalinee Prabpaipal  
[ ] Sura Suwannasri  
[x] Attapol Panurach

เอกสารไม่ควบคุม  
B 0314241



Cert.No.: 23P1401

Page: 2 of 2

Result of calibration:- Without adjustment

Function:- Pressure Measurement

Increasing Pressure

Range : 0 inH<sub>2</sub>O to 36 inH<sub>2</sub>O

Scale Interval : 0.1 inH<sub>2</sub>O ( The Fifth Estimate )

<u>UUC Indication</u>				
<u>Applied Pressure</u>	<u>High-port side</u>	<u>Low-port side</u>	<u>ΔP</u>	<u>Error</u>
(inH <sub>2</sub> O)	(inH <sub>2</sub> O)	(inH <sub>2</sub> O)	(inH <sub>2</sub> O)	(inH <sub>2</sub> O)
0.00	0.00	0.00	0.00	0.00
2.00	1.00	-0.98	1.98	-0.02
4.00	2.00	-1.98	3.98	-0.02
6.00	3.00	-2.98	5.98	-0.02
8.00	4.00	-3.98	7.98	-0.02
10.00	5.00	-4.98	9.98	-0.02
12.00	6.00	-6.00	12.00	0.00
14.00	7.00	-7.00	14.00	0.00
16.00	8.00	-8.00	16.00	0.00
18.00	9.00	-9.00	18.00	0.00
20.00	10.00	-10.00	20.00	0.00
22.00	11.00	-11.00	22.00	0.00
24.00	12.02	-12.00	24.02	0.02
26.00	13.02	-13.00	26.02	0.02
28.00	14.02	-14.00	28.02	0.02
30.00	15.04	-15.00	30.04	0.04
32.00	16.04	-16.00	32.04	0.04
34.00	17.02	-17.00	34.02	0.02
35.80	18.00	-17.96	35.96	0.16

The uncertainty of measurement was  $\pm 0.11$  inH<sub>2</sub>O

\* UUC = Unit Under Calibration

\* ΔP = High-port side - Low-port side

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.

เอกสารไม่ควบคุม  
a 1160340





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23P1859

Page : 1 of 2

Equipment : Aneroid Barometer  
Manufacturer: Barigo  
Model : -  
Serial No.: -  
ID No.: UAE.ANV.123/2550

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 02 June 2023

Reference: 2305-0919WSC

Submitted by: United Analyst and Engineering Consultant Co., Ltd.

Ambient Temperature: ( 23  $\pm$  2 ) °C

Relative Humidity: ( 50  $\pm$  15 ) %

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

Atmospheric Pressure: 1007 mbar

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.This result of calibration instrument was in absolute pressure.

5.This instrument was used clean air as pressure media.

6.The certificate is valid only to the item calibrated on date and place of calibration.

7.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew  
Issue Date : 08 June 2023

Approved Signatory :

Attapol P.  
[ ] Phalinee Prabpaipal  
[ ] Sura Suwannasri  
[x] Attapol Panurach

เอกสารไม่ควบคุม  
B 0316959



Cert.No.: 23P1859

Page: 2 of 2

Result of calibration:- Without adjustment

Range : 960 hPa to 1030 hPa

Function:- Absolute Pressure Measurement

Scale Interval : 1 hPa ( The Fifth Estimate )

Increasing Pressure

Applied Pressure (hPa)	958.80	969.94	981.10	991.92	1003.33	1013.39	1024.48	1035.27
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	1.20	0.06	-1.10	-1.92	-3.33	-3.39	-4.48	-5.27

Decreasing Pressure

Applied Pressure (hPa)	1035.27	1023.97	1013.46	1003.54	992.07	981.34	970.00	959.03
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-5.27	-3.97	-3.46	-3.54	-2.07	-1.34	0.00	0.97

The uncertainty of measurement was  $\pm 0.30$  hPa

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.

เอกสารไม่ควบคุม  
a 1165505





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23H1200

Page : 1 of 2

Equipment : Dial Thermo-Hygrometer

Manufacturer: Barigo

Model : -

Serial No.: -

ID No.: UAE.ANV.130/2550

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 30 May 2023  
to 06 June 2023

Reference: 2305-0919WSC

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H02 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Hygro-M2 Dew Point Monitor	5112	2360195	20703	02 Aug 2023
2) Handheld Thermometer With Sensor	1523	3240076	231305	15 Mar 2024

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

- National Institute of Standards and Technology (NIST) , The United States of America
- Technology Promotion Association (Thailand-Japan), NSC-ONSC Accredited No. Calibration 0008

Calibrated by : Somchai Dumwor  
Issue Date : 07 June 2023

Approved Signatory :

-   
☒ Chakrit Waewwanjua  
☐ Pornthippa Tameyakul  
☐ Viporn Tantiyawutti

เอกสารไม่ควบคุม  
B 0316274



Cert. No.: 23H1200

Page.: 2 of 2

**Result of Calibration:-**

Before Adjustment

Function:

Humidity Measurement

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	40.1	48	7.9	1.6
25.0	60.0	63	3.0	1.7
25.0	80.0	76	-4.0	1.9

**Result of Calibration:-**

After Adjustment

Function:

Humidity Measurement

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	40.1	44	3.9	1.6
25.0	60.0	60	0.0	1.7
25.0	80.0	75	-5.0	1.9

**Result of Calibration:-**

Without Adjustment

Function:

Temperature Measurement

<u>Standard</u> <u>Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (±°C)
19.987	20.0	0.013	0.72
30.016	30.0	-0.016	0.72
39.944	39.5	-0.444	0.72

**UUC\*** : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor  $k = 2.00$ , providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม  
a 1165295



### MULTI-POINT GAS TEST REPORT

**Test Date** : Jan 16, 2023

<b>Equipment :</b>	Gas Analyzer (NO <sub>2</sub> )	<b>Model :</b>	42i
<b>Manufacturer :</b>	Thermo Scientific	<b>Serial Number :</b>	CM19050150

#### Standard Gas Concentration


Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 21, 2024

#### Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.5	0.50	0.50	0.50
Level 3	40.00%	200.0	200.6	0.60	0.30	0.30
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.21
:Acceptable Limit $\pm 5\%$						

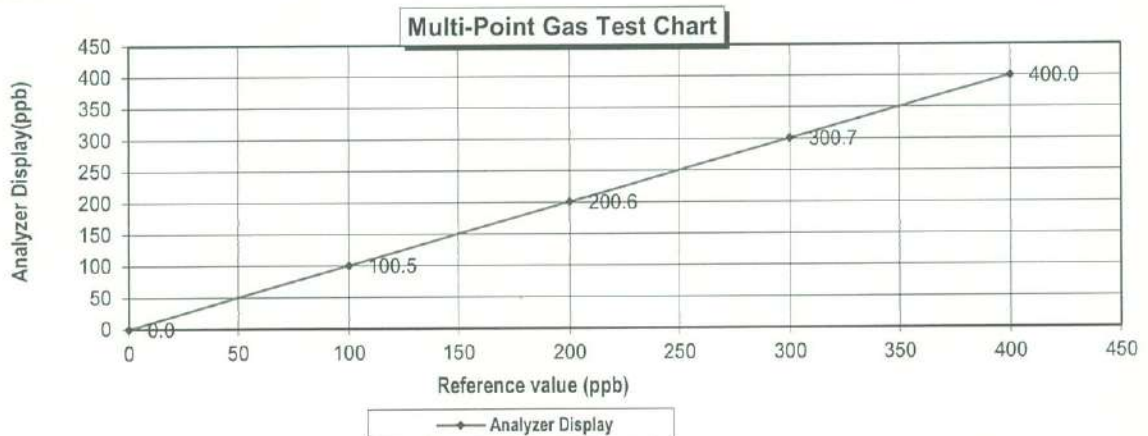

Calculate by

Aphiwat h.

16 / 01 / 66

Approve by

W. Thern h.

16 / Jan / 2023

### MULTI-POINT GAS TEST REPORT

**Test Date** : Feb 28, 2023

**Equipment** : Gas Analyzer (NO<sub>2</sub>)

**Model** : 42i

**Manufacturer** : Thermo Scientific

**Serial Number** : 1201778109

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 21, 2024


#### Dilutor Detail

Manufacturer :	Thermo Scientific
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

	Reference Value (ppb)		Analyzer Display (ppb)	Difference Error	Percent Error	[% Error]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	101.4	1.40	1.38	1.38
Level 3	40.00%	200.0	200.9	0.90	0.45	0.45
Level 4	60.00%	300.0	300.7	0.70	0.23	0.23
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.41
:Acceptable Limit $\pm 5\%$						

Multi-Point Gas Test Chart

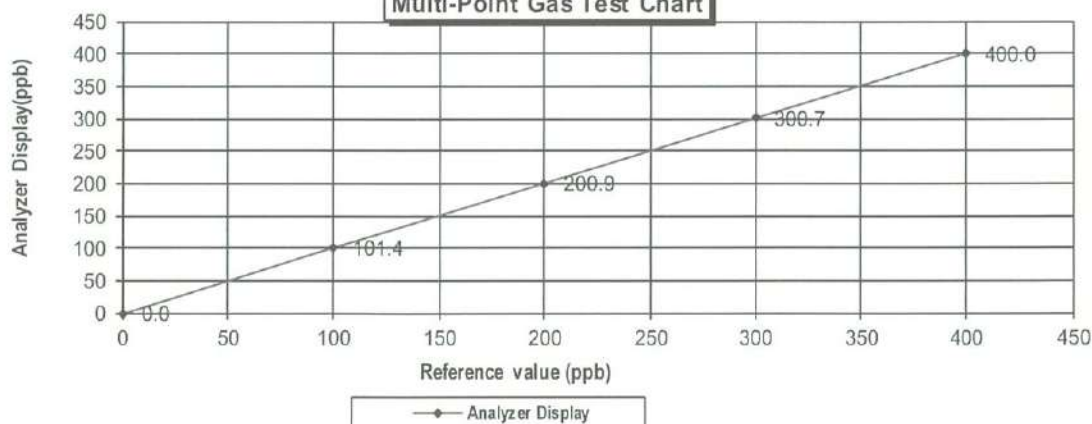

Calculate by

*Sirichai Gornchai*  
28 / 2 / 66

Approve by

*Adithorn H.*  
28 / Feb / 2023

# CERTIFICATE OF ANALYSIS

## Grade of Product: EPA Protocol

Part Number:	E04NI99E15A01D3	Reference Number:	122-402135167-1
Cylinder Number:	EB0143262	Cylinder Volume:	144.4 CF
Laboratory:	124 - Durham (SAP) - NC	Cylinder Pressure:	2015 PSIG
PGVP Number:	B22021	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.68 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20081120	CC708068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D885025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14060119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/-0.6%	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO2	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES:PO #5221002607

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

*[Signature]*

Approved for Release



CERT 3082.01

เอกสารไม่ควบคุม



### MULTI-POINT GAS TEST REPORT

**Test Date** : Feb 9, 2023

**Equipment :** Gas Analyzer (SO<sub>2</sub>)

**Model :** 43i

**Manufacturer :** Thermo SCIENTIFIC

**Serial Number :** 1201778115

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 24, 2024


#### Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[ % Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.5	0.50	0.50	0.50
Level 3	40.00%	200.0	201.1	1.10	0.55	0.55
Level 4	60.00%	300.0	300.6	0.60	0.20	0.20
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range 500.0 ppb				Average Difference (%)		0.25

Multi-Point Gas Test Chart

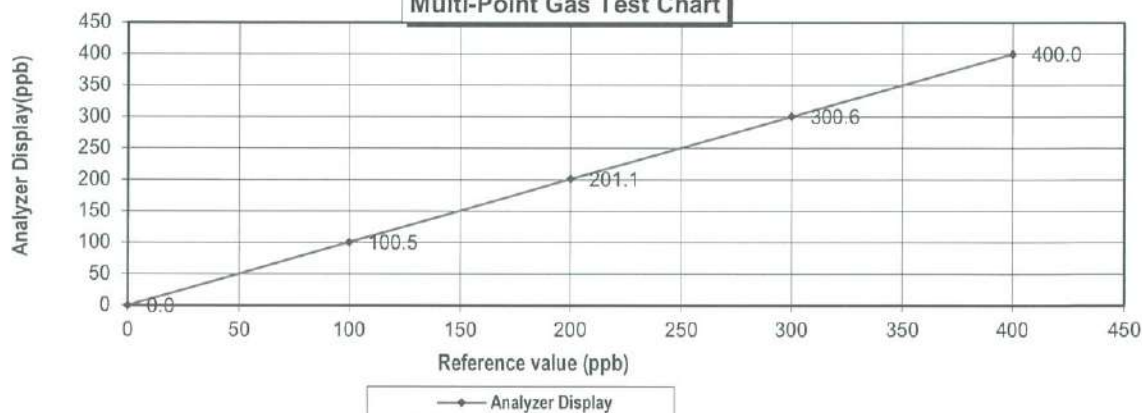

Calculate by

*Sirichon Gamman*  
9 / 2 / 66

Approve by

*Ratana*  
9 / Feb / 2023



### MULTI-POINT GAS TEST REPORT

**Test Date** : Jan 17, 2023

**Equipment** : Gas Analyzer (SO<sub>2</sub>)

**Model** : 43i

**Manufacturer** : Thermo SCIENTIFIC

**Serial Number** : CM22387061

#### Standard Gas Concentration

Sulphur Dioxide (SO <sub>2</sub> )	44.68
Nitric Oxide (NO)	45.94
Methane (CH <sub>4</sub> )	-
Carbon Monoxide (CO)	984.8
Cylinder No. :	EB0143262
Expiration Date :	Jun 24, 2024


#### Dilutor Detail

Manufacturer :	Thermo SCIENTIFIC
Model :	146i
Serial Number :	1180540071

#### Multi-point gas test data

Reference Value (ppb)			Analyzer Display (ppb)	Difference Error	Percent Error	[% Error ]
Level 1	Zero	0.0	0.0	0.00	0.00	0.00
Level 2	20.00%	100.0	100.7	0.70	0.70	0.70
Level 3	40.00%	200.0	201.1	1.10	0.55	0.55
Level 4	60.00%	300.0	301.5	1.50	0.50	0.50
Level 5	80.00%	400.0	400.0	0.00	0.00	0.00
Remark : Measuring Range			500.0 ppb	Average Difference (%)		0.35

Multi-Point Gas Test Chart

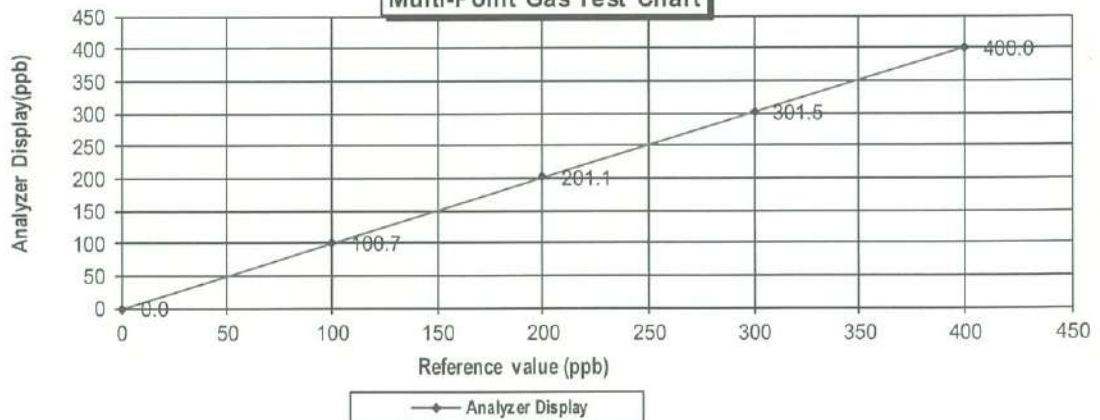

Calculate by

*Sirichon Yomgarn*  
17 / 1 / 66

Approve by

*Patthana U*  
17 / Jan / 2023

# CERTIFICATE OF ANALYSIS

## Grade of Product: EPA Protocol

Part Number:	E04NI99E15A01D3	Reference Number:	122-402135167-1
Cylinder Number:	EB0143262	Cylinder Volume:	144.4 CF
Laboratory:	124 - Durham (SAP) - NC	Cylinder Pressure:	2015 PSIG
PGVP Number:	B22021	Valve Outlet:	660
Gas Code:	CO,NO,NOX,SO2,BALN	Certification Date:	Jun 21, 2021

Expiration Date: Jun 21, 2024

Certification performed in accordance with "EPA Traceability Protocol for Assay and Certification of Gaseous Calibration Standards (May 2012)" document EPA 600/R-12/531, using the assay procedures listed. Analytical Methodology does not require correction for analytical interference. This cylinder has a total analytical uncertainty as stated below with a confidence level of 95%. There are no significant impurities which affect the use of this calibration mixture. All concentrations are on a mole/mole basis unless otherwise noted.

Do Not Use This Cylinder below 100 psig, i.e. 0.7 megapascals.

ANALYTICAL RESULTS					
Component	Requested Concentration	Actual Concentration	Protocol Method	Total Relative Uncertainty	Assay Dates
NOX	45.00 PPM	45.96 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
NITRIC OXIDE	45.00 PPM	45.94 PPM	G1	+/- 1.4% NIST Traceable	06/14/2021, 06/21/2021
SULFUR DIOXIDE	45.00 PPM	44.68 PPM	G1	+/- 1.0% NIST Traceable	06/14/2021, 06/21/2021
CARBON MONOXIDE	1000 PPM	984.8 PPM	G1	+/- 0.7% NIST Traceable	06/14/2021
NITROGEN	Balance				

CALIBRATION STANDARDS					
Type	Lot ID	Cylinder No	Concentration	Uncertainty	Expiration Date
NTRM	20081120	CC708068	49.82 PPM NITRIC OXIDE/NITROGEN	+/- 1.0%	Feb 02, 2025
PRM	12386	D885025	9.91 PPM NITROGEN DIOXIDE/AIR	+/- 2.0%	Feb 20, 2020
GMIS	401423838102	CC505581	4.348 PPM NITROGEN DIOXIDE/NITROGEN	+/- 2.1	Feb 18, 2023
NTRM	16011043	CC473277	49.02 PPM SULFUR DIOXIDE/NITROGEN	+/- 0.8%	Jun 17, 2022
NTRM	14060119	CC434277	990.9 PPM CARBON MONOXIDE/NITROGEN	+/-0.6%	Nov 15, 2025

The SRM, PRM or RGM noted above is only in reference to the GMIS used in the assay and not part of the analysis.

ANALYTICAL EQUIPMENT		
Instrument/Make/Model	Analytical Principle	Last Multipoint Calibration
Nicolet 6700 AHR0801333 CO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 NO2	FTIR	Jun 03, 2021
Nicolet 6700 AHR0801333 SO2	FTIR	Jun 03, 2021

Triad Data Available Upon Request

NOTES:PO #5221002607

GROSS WT: 28.40kg

NET WT: 4.73kg



The analytical test results reported on this certificate relate only to the cylinder number specified above. This concludes the test report.

*[Signature]*

Approved for Release



CERT 3082.01

เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## Calibration Certificate

Issued by : Calibration & Test Section : Meteorological Instruments Bureau

Date of Issue 1 November, 2023

Certification No. 390/23

Page : 1 of 5

Object : Wind Speed & Wind Direction Data Logger

Manufacturer : SCARLET/TECH

Type : WL-21

Mfg Code : Wireless Receiver 2205DR0113

Wind Sensor 2205DT0113

Customer : United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road,

Bangchak, Prakanong, Bangkok 10260.

Calibration Condition : Temperature 25.1 °C Barometric Pressure 1013.5 hPa

NATIONAL STANDARD WIND TUNNEL : Thermal Anemometer 642 S/N 91563

: HOOK GAGE NO 1425

: Wind Aloft Plotting Board

N.I.S.T. Test Reference Number 731/241460

: Standard Velocity at 20 - 30 m/sec

: Ultrasonic Anemometer

Model DA-650-3TV

(sensor TR-90AH)

Serial Number 110730029 (sensor 120629586)

JAPAN QUALITY ASSURANCE ORGANIZATION

: Standard Velocity at 0 - 20 m/sec

STANDARD THERMOMETER

: Theodor Friedrich : Dry No.8390/94 Wet No. 8389/94

: testo, testo 645 Serial No. 02848057

: Thermoschneider No.918802

STANDARD BAROMETER

: Digital Barometer Vaisala Type PTB220 No. V1220015

: Digital Barometer Vaisala Type PTB330 No. K4320001

Calibrated by :

*Watchapol*

Signed :

*Pisood Promsut*

Mr. Watchapol Subwat

Mr. Pisood Promsut

Mechanical Engineer

(Authorised Signatory)

for the Chief

Sub-Standard Instrument



เอกสารไม่ควบคุม





## THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804, 0-2399-0469

### The Result of Calibration

Certification No. 390/23

1 November, 2023

Page : 2 of 5

Standard Ultrasonic Anemometer m/sec	HOOK GAGE NO. 1425			TESTED ANEMOMETER	
	Pressure	Vacumm	Velocity	Velocity	Correction
	inches H2O	inches H2O	m/sec	m/sec	m/sec
1.00	-	-	-	1.0	0.0
3.02	-	-	-	3.0	0.02
5.00	-	-	-	5.0	0.0
7.04	-	-	-	7.0	0.04
9.02	-	-	-	8.9	0.12
11.02	-	-	-	9.0	2.02
13.01	-	-	-	13.0	0.01
15.01	-	-	-	14.9	0.11
17.02	-	-	-	17.0	0.02
20.02	-	-	-	19.9	0.12

Wind Aloft Plotting Board.	
US.DEPARTMENT OF COMMERCE WEATHER BUREAU	
WIND DIRETION	TESTED WIND DIRECTION
0	0
90	90
180	180
270	270

Calibrated by :

Mr. Watcharapol Subwat  
Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau



เอกสารไม่ควบคุม





# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## The Result of Calibration

Certification No. 390/23

1 November, 2023

Page : 3 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
1009.68	1009	0.68
1007.51	1007	0.51
1007.13	1007	0.13
1006.90	1007	-0.10
1006.72	1007	-0.28
1006.59	1006	0.59
1006.28	1006	0.28
1006.05	1006	0.05
1005.84	1006	-0.16
1005.48	1005	0.48
1009.61	1010	-0.39
1009.76	1010	-0.24
1009.69	1009	0.69
1009.45	1009	0.45
1009.24	1009	0.24
1008.89	1009	-0.11
1007.66	1008	-0.34
1006.99	1007	-0.01
1006.29	1006	0.29
1004.56	1005	-0.44

Average

0.12

Calibrated by :

Watcharapol

Mr. Watcharapol Subwat

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau



เอกสารไม่ควบคุม



# THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

## The Result of Calibration

Certification No. 390/23

1 November, 2023

Page : 4 of 5

Standard Barometer	Tested Barometer	Correction
Pressure	Pressure	
757.32	757	0.32
755.69	756	-0.31
755.41	755	0.41
755.24	755	0.24
755.10	755	0.10
755.00	755	0.00
754.77	755	-0.23
754.60	754	0.60
754.44	754	0.44
754.17	754	0.17
757.27	757	0.27
757.38	757	0.38
757.33	757	0.33
757.15	757	0.15
756.99	757	-0.01
756.73	757	-0.27
755.81	756	-0.19
755.30	755	0.30
754.78	755	-0.22
753.48	753	0.48

Average

0.15

Calibrated by :

Mr. Watcharapol Subwat

Mechanical Engineer



เอกสารไม่ควบคุม



## THAI METEOROLOGICAL DEPARTMENT

4353 Sukhumvit, Bangna, Bangkok 10260 Tel. 081-454-2804,0-2399-0469

### The Result of Calibration

Certification No. 390/23

1 November, 2023

Page : 5 of 5

Standard Temp. °C	Temperature Sensor Reading	
	Reading °C	Correction °C
45.12	45	0.12
30.21	30	0.21
15.42	15	0.42

Calibrated by :

*Watchapol*

Mr. Watchapol Subwat

Mechanical Engineer

Calibration & Test Section  
Meteorological Instruments Bureau



เอกสารไม่ควบคุม



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Prakanong, Bangkok 10260

Certificate No : 23-ACT-115  
Request No : Req-2023-1544

### Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1  
Manufacturer : 01dB Range : 94 dB / 1000 Hz  
Model : CAL31 Intrument Status : Used  
Serial Number : 84065  
ID : UAE.EFM.167/2561

### Calibration Environment and Details

Temperature : ( 23 ±2 °C )  
Humidity : ( 50 ± 20 %RH )  
Barometric Pressure : ( 1013 ±10.0 hPa )  
Received Date : 21 July 2023  
Calibration Date : 4 August 2023  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators

Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	31 May 2024
THD Multimeter	2015	1047765	NIMT	31 January 2024

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Calibrated By : me  
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By : ม.ร.น.  
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 4 August 2023

Certificate No : 23-ACT-115

Request No : Req-2023-1544

**Sound pressure level**

**Calibration Results : Without Adjustment**

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB)	Acceptance limit Class 1 ( ± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	93.90	-0.10	-	-	0.14	0.25

**Frequency of Sound pressure level**

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70

**Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)**

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.12	-	0.40	2.5

**Note :**

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

**End of Calibration**

# SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL23199

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-62 / Microphone UC-59L / Preamplifier NH-26  
**Serial No.:** 00130355 / 02734 / 00389  
**ID No.:** UAE.EMA2.102/2556

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 21 JUNE 2023  
**Calibration Date :** 26-27 JUNE 2023  
**Date of Issue :** 28 JUNE 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL23199

Job No. : VC66AC0067

Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL23199  
Job No. : VC66AC0067  
Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.4	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

## Continuation of Calibration Certificate

Cert. No. : ACL23199

Job No. : VC66AC0067

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	94.0	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
15.4

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	11.0
C - weight	15.7
Flat	24.8

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
125	0.1	0.1	0.1	± 1.0
1000	-0.1	-0.1	-0.1	± 0.7
8000	-0.7	-0.6	-0.6	+ 1.5, - 2.5



## Continuation of Calibration Certificate

Cert. No. : ACL23199

Job No. : VC66AC0067

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.1	0.0	0.0	±1.0
125	0.0	0.1	0.1	±1.0
250	0.0	0.0	0.0	±1.0
500	0.0	0.1	0.0	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.1	0.1	+ 1.5, - 2.5
16000	0.0	-1.2	-1.2	+ 2.5, -16.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.1	0.1	± 0.1

## Continuation of Calibration Certificate

Cert. No. : ACL23199

Job No. : VC66AC0067

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	±0.8
136.0	136.1	0.1	±0.8
135.0	135.1	0.1	±0.8
134.0	134.1	0.1	±0.8
133.0	133.1	0.1	±0.8
132.0	132.1	0.1	±0.8
131.0	131.1	0.1	±0.8
129.0	129.1	0.1	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	53.9	-0.1	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	38.9	-0.1	±0.8
34.0	33.9	-0.1	±0.8
30.0	29.9	-0.1	±0.8
29.0	28.9	-0.1	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	25.0	0.0	±0.8



Continuation of Calibration Certificate

Cert. No. : ACL23199

Job No. : VC66AC0067

Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±0.8

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.0 ; -3.0
	2	8	117.0	117.0	0.0	1.0 ; -1.5
	200	800	134.0	134.0	0.0	±0.5
Slow	2	8	108.0	108.0	0.0	1.0 ; -3.0
	200	800	127.6	127.6	0.0	±0.5
SEL	0.25	1	99.0	98.8	-0.2	1.0 ; -3.0
	2	8	108.0	108.0	0.0	1.0 ; -1.5
	200	800	128.0	128.0	0.0	±0.5

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
One	136.4	135.7	-0.7	±2.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±1.0
Positive half cycle	135.4	135.2	-0.2	±1.0
Negative half cycle	135.4	135.1	-0.3	±1.0



## Continuation of Calibration Certificate

Cert. No. : ACL23199

Job No. : VC66AC0067

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.6	0.1	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

# SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL23182

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-62 / Microphone UC-59L / Preamplifier NH-26  
**Serial No.:** 00130359 / 02371 / 00390  
**ID No.:** UAE.EFM.105/2556

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -

**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 29 MAY 2023  
**Calibration Date :** 07-08 JUNE 2023  
**Date of Issue :** 09 JUNE 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.

## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 2 of 8

Calibration Procedure : CP-AC-01

## Calibration Method :

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

## Condition of this result of calibration :

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).



## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.3	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	✓	-	0.3	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.98)	94.0	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
14.8

2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	9.5
C - weight	13.9
Flat	23.3

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.3	0.3	0.3	± 1.0
1000	0.1	0.1	0.1	± 0.7
8000	0.1	0.1	0.1	+ 1.5, - 2.5

## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 5 of 8

## 4. Electrical signal tests of frequency weightings

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	-0.1	±1.0
125	0.0	0.0	0.0	±1.0
250	0.0	0.0	-0.1	±1.0
500	0.0	0.0	-0.1	±1.0
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±1.0
4000	0.0	0.0	0.0	±1.0
8000	0.0	0.0	0.1	+ 1.5, - 2.5
16000	0.0	-1.3	-1.2	+ 2.5, -16.0

## 5. Frequency and time weightings at 1 kHz

## 5.1 Frequency weightings at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

## 5.2 Time weighting at 1 kHz

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

## 6. Long - term stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.1



## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.1	0.1	±0.8
136.0	136.1	0.1	±0.8
135.0	135.1	0.1	±0.8
134.0	134.1	0.1	±0.8
133.0	133.0	0.0	±0.8
132.0	132.0	0.0	±0.8
131.0	131.0	0.0	±0.8
129.0	129.0	0.0	±0.8
124.0	124.0	0.0	±0.8
119.0	119.0	0.0	±0.8
114.0	114.0	0.0	±0.8
109.0	109.0	0.0	±0.8
104.0	104.0	0.0	±0.8
99.0	99.0	0.0	±0.8
94.0	94.0	0.0	±0.8
89.0	89.0	0.0	±0.8
84.0	84.0	0.0	±0.8
79.0	79.0	0.0	±0.8
74.0	74.0	0.0	±0.8
69.0	69.0	0.0	±0.8
64.0	64.0	0.0	±0.8
59.0	59.0	0.0	±0.8
54.0	54.0	0.0	±0.8
49.0	49.0	0.0	±0.8
44.0	44.0	0.0	±0.8
39.0	39.0	0.0	±0.8
34.0	34.0	0.0	±0.8
30.0	30.0	0.0	±0.8
29.0	29.0	0.0	±0.8
28.0	28.0	0.0	±0.8
27.0	26.9	-0.1	±0.8
26.0	25.9	-0.1	±0.8
25.0	24.9	-0.1	±0.8

Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±0.8

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	116.9	-0.1	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	107.9	-0.1	1.5 ; -5.0
	200	800	127.6	127.5	-0.1	±1.0
SEL	0.25	1	99.0	98.8	-0.2	1.5 ; -5.0
	2	8	108.0	107.9	-0.1	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, Lcpeak ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
One	136.4	136.0	-0.4	±2.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	132.9	-0.1	±1.0
Positive half cycle	135.4	135.1	-0.3	±1.0
Negative half cycle	135.4	135.0	-0.4	±1.0

## Continuation of Calibration Certificate

Cert. No. : ACL23182

Job No. : VC66AC0062

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.5	89.5	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.1

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Prakanong, Bangkok 10260

Certificate No : 23-ACT-109  
Request No : Req-2023-1406

### Unit Under Calibration Details

Measurement item : Acoustic Calibrator Class : 1  
Manufacturer : 01dB Range : 94 dB / 1000 Hz  
Model : CAL31 Intrument Status : Used  
Serial Number : 82795  
ID : UAE.EFM.113/2560

### Calibration Environment and Details


Temperature : ( 23  $\pm$ 2  $^{\circ}$ C )  
Humidity : ( 50  $\pm$  20 %RH )  
Barometric Pressure : ( 1013  $\pm$ 10.0 hPa )  
Received Date : 26 June 2023  
Calibration Date : 27 June 2023  
Location of Calibration : LAB 1 Acoustic  
Calibration Procedure : In-house method CP-ACT-02 based on IEC 60942:2017 Electroacoustics - Sound calibrators


Reference Standard	Model	Serial Number	Traceable	Due Calibration
Sound Calibrator	SV 35A	58079	EEI	31 May 2024
THD Multimeter	2015	1047765	NIMT	31 January 2024

**Traceability** : This certificate provides traceability of measurement to recognized national standard, and to the realization of the international System of Units (SI).

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Calibrated By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 27 June 2023

Certificate No : 23-ACT-109

Request No : Req-2023-1406

**Sound pressure level**

**Calibration Results : Without Adjustment**

Calibration Range (dB)	Without Adjustment (dB)		Adjustment (dB)		Uncertainty ( ± dB)	Acceptance limit Class 1 ( ± dB)
	Measured	Error	Measured	Error		
94 dB / 1000 Hz	94.11	0.11	-	-	0.13	0.25

**Frequency of Sound pressure level**

Calibration Range (Hz)	Without Adjustment		Adjustment		Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (Hz)	Error (%)	Measured (Hz)	Error (%)		
94 dB / 1000 Hz	1000.00	0.00	-	-	0.01	0.70

**Total Harmonic Distortion plus Noise of Sound pressure level (THD+N %)**

Calibration Range (Hz)	Without Adjustment	Adjustment	Uncertainty ( ± %)	Acceptance limit Class 1 ( ± %)
	Measured (%)	Measured (%)		
94 dB / 1000 Hz	0.08	-	0.40	2.5

**Note :**

- Acceptance limit was IEC60942:2017 Class 1
- The calibration results exclude the calibrator pressure correction
- The calibration results exclude the microphone volume correction

**End of Calibration**

# SITHIPORN ASSOCIATES CO.,LTD. CALIBRATION LABORATORY

451-451/1 Sirinthorn Rd.,Bangbunru, Bangplud Bangkok 10700 THAILAND.  
Tel.0-2435-8800 Fax.0-2433-1679 e-mail:cal-center@sithiphorn.com http://www.sithiphorn.com



Cert. No. : ACL23119

Pages : 1 of 8

## Calibration Certificate

**Equipment :** SOUND LEVEL METER  
**Manufacturer :** RION  
**Model :** NL-42/ Microphone UC-52 / Preamplifier NH-24  
**Serial No.:** 01010780 / 194535 / 14658  
**ID No.:** UAE.EFM.083/2565

**Condition As Found :** GOOD

**Customer :** UNITED ANALYST AND ENGINEERING CONSULTANT (UAE)  
81 SOI UDOMSUK 41, SUKHUMVIT ROAD,  
BANGCHAK SUB-DISTRICT,  
PHRAKHANONG DISTRICT, BANGKOK 10260  
THAILAND.

**Location :** -  
**Ambient Temperature :** ( 23.0  $\pm$  3 ) °C  
**Pressure :** ( 101.3  $\pm$  3 ) kPa  
**Relative Humidity :** ( 50.0  $\pm$  20 ) %

**Received Date :** 05 APRIL 2023  
**Calibration Date :** 10 -11 APRIL 2023  
**Date of Issue :** 18 APRIL 2023

**Calibrated by :**

Nathakorn Pisutpaisan

**Approved by :**

  
( Thanakul Petchurai )

This certificate is issued in accordance with the requirements of ISO/IEC 17025 standard, may not be reproduced other than in full, except with the prior written approval of the head of Calibration Laboratory.



## Continuation of Calibration Certificate

Cert. No. : ACL23119

Job No. : VC66AC0044

Pages : 2 of 8

Calibration Procedure : CP-AC-01

**Calibration Method :**

This equipment was calibrated by based on IEC-61672-3 (2013) Standard for sound level meter (SLM).

The SLM had tests to Acoustical and Electrical signal tests of frequency weighting with Anechoic chamber and Reference Standard Instruments.

For tests results of each items were made by observation of each Instruments display and also with SLM's display.

**Condition of this result of calibration :**

## 1. Reference Standard Instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Cert. No.</u>	<u>Due Date</u>
Waveform Generator	33210A	MY48017076	EF-0009-23	07-FEB-24
Waveform Generator	33511B	MY52302742	EF-0010-23	07-FEB-24
Digital Multimeter	33461A	MY53220104	EEL.BP 30/0266	13-FEB-24
Digital Multimeter	33461A	MY53220076	EEL.BP 29/0266	13-FEB-24
Digital Multimeter	34461A	MY60024273	EEL.BP 31/0266	14-FEB-24
Programmable Attenuator	MAT-1070	62100114	EF-0011-23	08-FEB-24
Condenser Microphone	4180	2977900	AA-1001-23	14-FEB-24
Measuring Amplifier	NA-42KAI	34560495	AA-3002-23	14-FEB-24

2. This result of calibration was found accurate as shown on date and place of calibration for this calibrated item only.

3. This certificate is traceable to the international system of unit maintained at :

3.1 National Institute of Metrology (Thailand).

3.2 Thailand Institute of Scientific and Technological Research (TISTR).

Continuation of Calibration Certificate

Cert. No. : ACL23119  
Job No. : VC66AC0044  
Pages : 3 of 8

**Summary of Measurement Result :**

Parameter	Pass	Fail	Uncertainty (dB)	Maximum-permitted uncertainty of measurement (dB)
1. Absolute sensitivity	✓	-	0.2	N/A
2. Self-generated noise	✓	-	0.2	N/A
3. Acoustical signal tests of frequency weightings				
125 Hz	✓	-	0.3	0.6
1000 Hz	✓	-	0.3	0.6
8000 Hz	✓	-	0.3	0.7
4. Electrical signal tests of frequency weightings				
For 10 Hz to 4 kHz	✓	-	0.3	0.6
For > 4 kHz to 10 kHz	✓	-	0.3	0.7
For > 10 kHz to 20 kHz	-	-	-	1.0
5. Frequency and time weightings at 1 kHz	✓	-	0.2	0.2
6. Long - term stability	✓	-	0.1	0.1
7. Level linearity on the reference level range	✓	-	0.2	0.3
8. Level linearity including the level range control	✓	-	0.2	0.3
9. Tone burst response	✓	-	0.2	0.3
10. Peak C sound level	✓	-	0.2	0.35
11. Overload indication	✓	-	0.2	0.25
12. High level stability	✓	-	0.1	0.1

Note : Pass/Fail evaluation for each parameter,  
will be considered together from the acceptance limit and the Maximum-permitted uncertainty of measurement.

## Continuation of Calibration Certificate

Cert. No. : ACL23119

Job No. : VC66AC0044

Pages : 4 of 8

**Result of calibration :****1. Absolute sensitivity**

Reference Acoustic Signal ( dB )	Measured Value ( dB )	Deviation ( dB )	Acceptance Limit ( dB )
93.9 (93.95)	93.9	0.0	±0.3

**2. Self-generated noise**

## 2.1 Normal test

Measured Value ( dB )
14.6

## 2.2 The microphone of the sound level meter was replaced by electrical signal input device.

Frequency Weighting	Measured value ( dB )
A - weight	10.8
C - weight	16.8
Flat	22.6

**3. Acoustical signal tests of frequency weightings**

Meter free-field acoustic response at a level of 84 dB

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			Acceptance Limits
	Flat	C-weight	A-weight	
125	0.3	0.3	0.3	± 1.5
1000	0.0	0.0	0.0	± 1.0
8000	0.5	0.6	0.6	±5.0



Continuation of Calibration Certificate

Cert. No. : ACL23119  
Job No. : VC66AC0044  
Pages : 5 of 8

**4. Electrical signal tests of frequency weightings**

Weighting network response with relative to 1 kHz.

Frequency ( Hz )	Deviation from various frequency weighting response curve (dB)			
	Flat	C-weight	A-weight	Acceptance Limits
63	0.0	-0.1	0.0	±2.0
125	0.0	0.0	0.0	±1.5
250	0.0	0.0	0.0	±1.5
500	0.0	0.0	0.0	±1.5
1000	0.0	0.0	0.0	±1.0
2000	0.0	0.0	0.0	±2.0
4000	0.0	0.0	0.0	±3.0
8000	0.0	0.1	0.1	±5.0

**5. Frequency and time weightings at 1 kHz**

**5.1 Frequency weightings at 1 kHz**

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.2
C - weight	94.0	94.0	0.0	± 0.2
Flat	94.0	94.0	0.0	± 0.2

**5.2 Time weighting at 1 kHz**

Frequency Weighting	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	94.0	94.0	0.0	± 0.1
Slow	94.0	94.0	0.0	± 0.1
Leq	94.0	94.0	0.0	± 0.1

**6. Long - term stability**

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	94.0	94.0	0.0	± 0.3

## Continuation of Calibration Certificate

Cert. No. : ACL23119

Job No. : VC66AC0044

Pages : 6 of 8

## 7. Level linearity on the reference level range

Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
137.0	137.0	0.0	± 1.1
136.0	136.0	0.0	± 1.1
135.0	135.0	0.0	± 1.1
134.0	134.0	0.0	± 1.1
133.0	133.0	0.0	± 1.1
132.0	132.0	0.0	± 1.1
131.0	131.0	0.0	± 1.1
129.0	129.0	0.0	± 1.1
124.0	124.0	0.0	± 1.1
119.0	119.0	0.0	± 1.1
114.0	114.0	0.0	± 1.1
109.0	109.0	0.0	± 1.1
104.0	104.0	0.0	± 1.1
99.0	99.0	0.0	± 1.1
94.0	94.0	0.0	± 1.1
89.0	89.0	0.0	± 1.1
84.0	84.0	0.0	± 1.1
79.0	79.0	0.0	± 1.1
74.0	74.0	0.0	± 1.1
69.0	69.0	0.0	± 1.1
64.0	64.0	0.0	± 1.1
59.0	59.0	0.0	± 1.1
54.0	53.9	-0.1	± 1.1
49.0	49.0	0.0	± 1.1
44.0	44.0	0.0	± 1.1
39.0	39.0	0.0	± 1.1
34.0	34.0	0.0	± 1.1
30.0	30.3	0.3	± 1.1
29.0	29.3	0.3	± 1.1
28.0	28.4	0.4	± 1.1
27.0	27.2	0.2	± 1.1
26.0	26.6	0.6	± 1.1
25.0	25.8	0.8	± 1.1



Continuation of Calibration Certificate

Cert. No. : ACL23119  
Job No. : VC66AC0044  
Pages : 7 of 8

**8. Level linearity including the level range control**

Range	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Auto	94.0	94.0	0.0	±1.1

**9. Tone burst response**

Time Weighting	Tone burst duration, Tb ( ms )	Cycle	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Fast	0.25	1	108.0	107.9	-0.1	1.5 ; -5.0
	2	8	117.0	117.0	0.0	1.0 ; -2.5
	200	800	134.0	134.0	0.0	±1.0
Slow	2	8	108.0	108.0	0.0	1.5 ; -5.0
	200	800	127.6	127.6	0.0	±1.0
SEL	0.25	1	99.0	98.9	-0.1	1.5 ; -5.0
	2	8	108.0	108.0	0.0	1.0 ; -2.5
	200	800	128.0	128.0	0.0	±1.0

**10. Peak C sound level**

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value, L <sub>peak</sub> ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±3.0
One	136.4	135.6	-0.8	±3.0

Number of cycle in test signal	Anticipated Value ( dB )	Measured Value ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
Continuous	133.0	133.0	0.0	±2.0
Positive half cycle	135.4	135.2	-0.2	±2.0
Negative half cycle	135.4	135.2	-0.2	±2.0



## Continuation of Calibration Certificate

Cert. No. : ACL23119

Job No. : VC66AC0044

Pages : 8 of 8

## 11. Overload indication

Measured value ( dB )		Deviated Value ( dB )	Acceptance Limits ( dB )
Positive one-half cycle	Negative one-half cycle		
89.7	89.7	0.0	±1.5

## 12. High level stability

Frequency Weighting	SLM Display at initial ( dB )	SLM Display at final ( dB )	Deviated Value ( dB )	Acceptance Limits ( dB )
A - weight	137.0	137.0	0.0	±0.3

The reported uncertainty is based on a standard uncertainty multiplied by coverage factor  $k = 2$  or any value following calculation, providing a level of confidence of approximately 95 %

End of Calibration Certificate

## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING CONSULTANT CO., LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

Certificate No : 23-AFM-219 Rev.1

Request No : Req-2023-2171

### Unit Under Calibration Details

Measurement Item : Air Flow Meter  
Manufacturer : TSI  
Model : 4146 Sensor Model : -  
Serial Number : 41461813030 Sensor Serial Number : -  
ID : UAE.EFM.102/2561  
Location of Calibration : LAB 4 AIR VELOCITY METER

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 20 %RH  
Barometric Pressure : 1013 hPa ± 10 hPa  
Received Date : 11 October 2023  
Calibration Date : 25 October 2023  
Calibration Procedure : In-house method CP-AFM-01 by Comparison technique with Standard Primary Flow Calibrator


Reference Standard	Model	Serial Number	Traceble	Due Calibration
Air Flow Meter	Gilibrator 3 Standard flow	19031011003	Sensidyne	12 July 2024
Air Flow Meter	Gilibrator 3 High flow	18501012012	Sensidyne	12 July 2024
Temperature meter	GT 11	08000057	Qreborn	27 February 2024
Pressure meter	CPG2400	41000KDU/651882	TPA	7 November 2023


### Traceability :

This Certificate is traceable to SI Unit through Sensidyne A2LA Accreditation No. 3943.01

### Note :

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k = 2$ , providing a level of confidence approximately 95 %.  
This Certificate was issued to replace to Calibration Certificate No. 23-AFM-219

Calibration By :   
Mr. Noppadon Luangart  
Service Calibration Engineer

Approved By :   
Mr. Pacit Mathavorn  
Calibration Engineer Supervisor

Issue Date : 7 November 2023

Certificate No : 23-AFM-219

Request No : Req-2023-2171

**Result of Calibration :**

Temperature (°C)	Pressure (kPa)	STD (l/min)	UUC (l/min)	Error (l/min)	Uncertainty (l/min)
25.00	101.20	0.018	0.020	0.002	0.0013
25.10	101.30	0.047	0.050	0.003	0.0033
25.30	101.27	0.096	0.100	0.004	0.0028
25.30	101.27	0.195	0.200	0.005	0.0056
25.30	101.27	0.493	0.500	0.007	0.0071
25.30	101.21	0.997	1.000	0.003	0.083
25.20	101.20	1.688	1.698	0.010	0.085
25.40	101.18	2.002	2.007	0.005	0.086
25.30	101.10	2.991	3.014	0.023	0.042
25.30	101.10	3.994	4.002	0.008	0.056
25.30	101.10	5.032	5.009	-0.023	0.070

**Note**                      STD : Standard                      UUC : Unit Under Calibration  
 - UUC Reference Condition : At 21.1 °C, 101.3 kPa, Air  
 - Flow Rate was corrected for non-standard operating condition by using equation :

$$Q_{\text{meas}} = Q_{\text{ref}} \times \frac{P_{\text{ref}}}{P_{\text{meas}}} \times \frac{T_{\text{meas}}}{T_{\text{ref}}}$$

where    Q = Flow Rate                      P = Absolute Pressure                      T = Absolute Temperature  
           Meas = Measurement Condition                      ref = Standard Condition

\* Indicates non accredited

**End of Certificate**





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23P1858

Page : 1 of 2

Equipment : Aneroid Barometer  
Manufacturer: Barigo  
Model : -  
Serial No.: -  
ID No.: UAE.ANV.124/2550

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Condition As-Received: Used Item

Received Date: 26 May 2023

Calibration Date: 02 June 2023

Reference: 2305-0919WSC

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

Ambient Temperature: ( 23  $\pm$  2 ) °C

Relative Humidity: ( 50  $\pm$  15 ) %

81 Soi Udomsuk 41, Sukhumvit Road,  
Bangchak, Phrakhanong, Bangkok 10260

Atmospheric Pressure: 1007 mbar

Procedure used: The calibration was conducted by direct comparison method against Pressure Measuring Instruments Standard according to in-house calibration procedure CP-P10, using " DKD-R 6-1 ; Calibration of Pressure Gauges, Edition 03/2014 " as a guidelines.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Standard Barometer	DPI142	1422505046	MP-0094-23	03 May 2024

2.This instrument was installed in vertical orientation and center of the dial was used as the reference level.

3.This result of calibration was made on requested at the point specified by customer.

4.This result of calibration instrument was in absolute pressure.

5.This instrument was used clean air as pressure media.

6.The certificate is valid only to the item calibrated on date and place of calibration.

7.This Certification is traceable to the International System of Unit maintained through:-

-National Institute of Metrology Thailand (NIMT)

Calibrated by : Suksan Khankaew  
Issue Date : 08 June 2023

Approved Signatory :

Attapol P.  
[ ] Phalinee Prabpaipal  
[ ] Sura Suwannasri  
[x] Attapol Panurach

เอกสารไม่ควบคุม  
B 0316958



Cert.No.: 23P1858

Page: 2 of 2

Result of calibration:- Without adjustment

Range : 960 hPa to 1030 hPa

Function:- Absolute Pressure Measurement

Scale Interval : 1 hPa ( The Fifth Estimate )

Increasing Pressure

Applied Pressure (hPa)	959.93	970.47	981.93	991.32	1002.29	1011.64	1021.14	1032.30
UUC* Indication (hPa)	960.0	970.0	980.0	990.0	1000.0	1010.0	1020.0	1030.0
Error (hPa)	0.07	-0.47	-1.93	-1.32	-2.29	-1.64	-1.14	-2.30

Decreasing Pressure

Applied Pressure (hPa)	1032.30	1021.44	1011.67	1002.36	992.35	981.94	970.49	959.94
UUC* Indication (hPa)	1030.0	1020.0	1010.0	1000.0	990.0	980.0	970.0	960.0
Error (hPa)	-2.30	-1.44	-1.67	-2.36	-2.35	-1.94	-0.49	0.06

The uncertainty of measurement was  $\pm 0.30$  hPa

\* UUC = Unit Under Calibration

The reported uncertainty of measurement was based on a standard uncertainty multiplied by a coverage factor  $k = 2$ , providing a level of confidence of approximately 95 %.

-o0o-

Attapol P.

เอกสารไม่ควบคุม  
a 1165506





TECHNOLOGY PROMOTION ASSOCIATION (THAILAND-JAPAN)  
CORPORATE SERVICES 3: EQUIPMENT CALIBRATION AND TESTING SERVICES  
534/4 PATTANAKARN ROAD SOI 18, SUANLUANG, SUANLUANG, BANGKOK 10250  
TEL. 0-2717-3000-24 FAX. 0-2719-9484



## Certificate of Calibration

Certificate No. : 23H1101

Page : 1 of 2

Equipment : Digital Thermo-Hygrometer

Manufacturer: Digicon

Model : TH-02

Serial No.: 395034175

ID No.: UAE.EFM.184/2565

Condition As-Received: Used Item

Received Date: 18 May 2023

Calibration Date: 22 May 2023  
to 24 May 2023

Reference: 2305-0641WSC

Ambient Temperature: ( 25 ± 3 ) °C

Relative Humidity: ( 50 ± 20 ) %

This certificate may not be reproduced other than in full,  
except with the prior written approval of the head of  
Corporate Services 3: Equipment Calibration and Testing Services.

Submitted by: United Analyst and Engineering Consultant Co.,Ltd.

81 Soi Udomsuk 41, Sukhumvit Road, Bangchak,  
Phrakhanong, Bangkok 10260

Procedure used: Calibration were conducted using in-house calibration procedure CP-H03 according to comparison with standard chilled mirror sensor for humidity measurement function and comparison with standard temperature probe for temperature measurement function into humidity / temperature chamber.

### Condition of this result of calibration

1.Reference standards instruments :

<u>Instrument</u>	<u>Model</u>	<u>Serial No.</u>	<u>Certificate No.</u>	<u>Due Date</u>
1) Chilled Mirror Hygrometer	Dew Master	44730	20563A	14 Jun 2023
2) Handheld Thermometer With Sensor	1521	A5A339	2211251	12 Oct 2023

2.The certificate is valid only to the item calibrated on date and place of calibration.

3.This Certification is traceable to the International System of Unit maintained through:-

- National Institute of Standards and Technology (NIST) , The United States of America
- National Institute of Metrology Thailand (NIMT)

Calibrated by : Kraipop Onrat

Issue Date : 25 May 2023

Approved Signatory :

[✓] Chakrit Waewwanjua

[ ] Pornthippa Tameyakul

[ ] Viporn Tantiyawutti

เอกสารไม่ควบคุม

B 0314979





Cert. No.: 23H1101

Page.: 2 of 2

**Result of Calibration:-**

Without Adjustment

Function:

Humidity Measurement

<u>Reference</u> <u>Temperature</u> (°C)	<u>Standard</u> <u>Humidity</u> (%R.H.)	<u>UUC*</u> <u>Reading</u> (%R.H.)	<u>Error</u> (%R.H.)	<u>Uncertainty</u> <u>of Measurement</u> (±%R.H.)
25.0	40.1	41	0.9	1.3
25.0	50.1	51	0.9	1.6
25.0	60.0	60	0.0	1.6
25.0	70.2	67	-3.2	1.6

**Result of Calibration:-**

Without Adjustment

Function:

Temperature Measurement

<u>Standard</u> <u>Temperature</u> (°C)	<u>UUC*</u> <u>Reading</u> (°C)	<u>Error</u> (°C)	<u>Uncertainty</u> <u>of Measurement</u> (±°C)
20.014	20.4	0.386	0.42
25.022	25.6	0.578	0.42
30.033	30.3	0.267	0.42
40.000	40.1	0.100	0.42

**UUC\*** : Unit Under Calibration

The reported uncertainty of measurement was base on standard uncertainty multiplied by coverage factor  $k = 2.00$ , providing confidence level approximately 95%.

-o0o-

เอกสารไม่ควบคุม  
a 1162980



## Certificate of Calibration

**Customer**

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.

**Certificate No : 23-TPM-253****Request No : Req-2023-0955**

Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangchak, Prakanong,  
Bangkok 10260

**Page : 1/2****Unit Under Calibration Details**

Calibration Parameter : Temperature

Instrument Name : Thermal Environment Monitor

Range Calibration : 20 °C to 60 °C

Manufacturer : 3M

Type of Sensor : RTD

Model : QT-32

Sensor Diameter (mm) : 4.5

Serial Number : TPQ020025

Calibration Position (mm) : 67.5

Resolution : 0.1 °C

Instrument Status : Used

ID Number : UAE.EFM.008/2559

**Calibration Environment and Details**

Temperature : 23 °C ± 3 °C

Humidity : 55 %RH ± 15 %RH

Received Date : 4 May 2023

Calibrated Date : 12 May 2023

Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

**Reference Standard** : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN:  
08000057, ID: 02-TPM Which was calibrated on 27 February 2023, Calibration Certificate No. : QR23-  
0494

**Traceability** : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.:  
Calibration 0292

**Note**

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

**Approved By :**

Mr. Noppadon Luangart

Technical Manager

**Issue Date :**

12 May 2023

**Calibration Note**

UUC Adjustment : Not Adjust

Certificate No : 23-TPM-253

Request No : Req-2023-0955

Page : 2/2

**Result of Calibration :**

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	20.031	20.1	- 0.1	0.13
	25.033	25.1	- 0.1	0.13
	30.036	30.1	- 0.1	0.13
	35.039	35.1	- 0.1	0.13
	40.040	40.1	- 0.1	0.13
	45.042	45.1	- 0.1	0.13
	50.045	50.1	- 0.1	0.13
	60.050	60.1	- 0.1	0.13
DRY	20.033	20.0	0.0	0.13
	25.034	25.0	0.0	0.13
	30.034	30.0	0.0	0.13
	35.036	35.0	0.0	0.13
	40.040	40.0	0.0	0.13
	45.044	45.0	0.0	0.13
	50.042	50.0	0.0	0.13
	60.048	60.0	0.0	0.13
GLOBE	20.032	20.1	- 0.1	0.13
	25.034	25.1	- 0.1	0.13
	30.034	30.1	- 0.1	0.13
	35.037	35.1	- 0.1	0.13
	40.038	40.0	0.0	0.13
	45.039	45.0	0.0	0.13
	50.044	50.0	0.0	0.13
	60.047	60.0	0.0	0.13

End of Certificate

Calibrated By :



Mr. Sittichok Jirapukdeesakun



## Certificate of Calibration

### Customer

Name : UNITED ANALYST AND ENGINEERING  
CONSULTANT CO.,LTD.  
Address : 81 Soi Udomsuk 41, Sukhumvit Road, Bangehak, Prakanong,  
Bangkok 10260

Certificate No : 23-TPM-046

Request No : Req-2023-0045

Page : 1/2

### Unit Under Calibration Details

Calibration Parameter : Temperature  
Instrument Name : Thermal Environment Monitor Range Calibration : 20 °C to 60 °C  
Manufacturer : 3M Type of Sensor : RTD  
Model : QT-32 Sensor Diameter (mm) : 4.5  
Serial Number : TPS030008 Calibration Position (mm) : 67.5  
Resolution : 0.1 °C Intrument Status : Used  
ID Number : UAE.EFM083/2561

### Calibration Environment and Details

Temperature : 23 °C ± 3 °C  
Humidity : 55 %RH ± 15 %RH  
Received Date : 10 January 2023  
Calibrated Date : 25 January 2023  
Calibration Procedure : In-house method CP-TPM-01 by Comparison with Standard Thermometer.

Reference Standard : Digital Thermometer with Sensor, Manufacturer: GINGO/GINGO, Model: GT11/ RTD100, SN:  
08000057, ID: 02-TPM Which was calibrated on 10 March 2022, Calibration Certificate No. : QR22-0578

Traceability : This Certificate is traceable to SI Unit through Quality Reborn Co., Ltd., NSC-ONSC Accreditation No.:  
Calibration 0292

### Note

The reported uncertainty is based on standard uncertainty multiplied by the Coverage Factor  $k=2$ , providing a level of confidence approximately 95 %.

Approved By :



Mr. Pacit Mathavorn

Calibration Engineer Supervisor

Issue Date :

25 January 2023

**Calibration Note**

UUC Adjustment : Not Adjust

**Certificate No :** 23-TPM-046

**Request No :** Req-2023-0045

**Page :** 2/2

**Result of Calibration :**

UUC Sensor	Standard Temperature (°C)	UUC Reading (°C)	Correction (°C)	Uncertainty (± °C)
WET	20.003	20.0	0.0	0.14
	25.006	25.0	0.0	0.14
	30.005	30.0	0.0	0.14
	35.003	35.0	0.0	0.14
	40.005	40.0	0.0	0.14
	45.005	45.0	0.0	0.14
	50.006	50.0	0.0	0.14
	60.004	60.0	0.0	0.14
DRY	20.003	20.2	- 0.2	0.14
	25.002	25.2	- 0.2	0.14
	30.004	30.2	- 0.2	0.14
	35.004	35.2	- 0.2	0.14
	40.004	40.2	- 0.2	0.14
	45.003	45.2	- 0.2	0.14
	50.004	50.2	- 0.2	0.14
	60.007	60.2	- 0.2	0.14
GLOBE	20.004	20.0	0.0	0.14
	25.005	25.0	0.0	0.14
	30.004	30.0	0.0	0.14
	35.005	35.0	0.0	0.14
	40.006	40.1	- 0.1	0.14
	45.006	45.1	- 0.1	0.14
	50.004	50.1	- 0.1	0.14
	60.005	60.1	- 0.1	0.14

End of Certificate

Calibrated By :



Mr. Sittichok Jirapukdeesakun